



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
23.12.2009 Bulletin 2009/52

(51) Int Cl.:
A61B 5/1455 (2006.01)

(21) Application number: **09162886.7**

(22) Date of filing: **17.06.2009**

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK TR

- **Kanemoto, Michio**
Shinjuku-ku Tokyo (JP)
- **Fuse, Masayoshi**
Shinjuku-ku Tokyo (JP)
- **Ukawa, Teiji**
Shinjuku-ku Tokyo (JP)

(30) Priority: **19.06.2008 JP 2008160013**

(71) Applicant: **Nihon Kohden Corporation**
Shinjuku-ku
Tokyo (JP)

(74) Representative: **Grünecker, Kinkeldey, Stockmair & Schwanhäusser**
Anwaltssozietät
Leopoldstrasse 4
80802 München (DE)


(72) Inventors:
• **Aoyagi, Takuo**
Shinjuku-ku Tokyo (JP)

(54) **Pulse oximetry and pulse oximeter**

(57) A pulse oximetry includes: irradiating living tissue with a plurality of light beams of different wavelengths; receiving the light beams transmitted through or reflected from the living tissue and converting the received light beams to electric signals which correspond to the different wavelengths; time-segmenting time series data of the electric signals; calculating, with respect

to each of the segmented time series data of the electric signals, a slope value of a regression line between each two of the electric signals; calculating SaO₂ based on the slope value of each of the segmented time series data of the electric signals; constructing a histogram of SaO₂ for each predetermined number of time segments; and obtaining a mode value from the histogram as SpO₂ to be output of the pulse oximetry.

FIG. 1

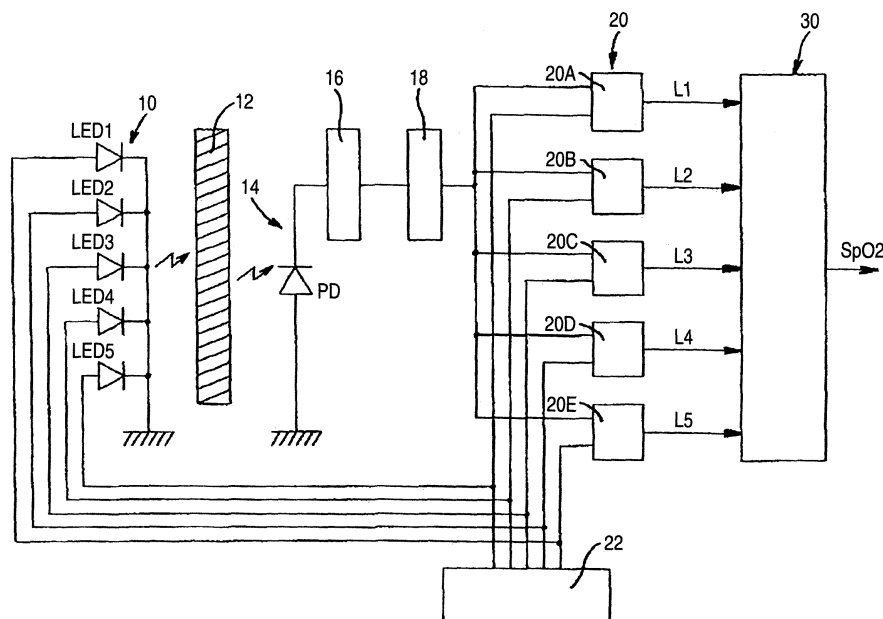

Description

BACKGROUND OF THE INVENTION

[0001] The present invention relates to a pulse oximetry which measures continuously arterial oxygen saturation (SaO₂) in a non-invasive manner by using a blood volume variation of the tissue arterial blood caused by pulsation, and also to a pulse oximeter which performs such a pulse oximetry.

[0002] Today, in a related-art technique called a pulse oximetry, in the case where SaO₂ is to be obtained, the following procedure is usually adopted.

- (1) Tissue transmitted or reflected light is continuously measured at a plurality of wavelengths.
- (2) The peak and bottom of pulsation of the measured tissue transmitted or reflected light are determined, and the transmitted or reflected light beams at the peak and bottom are indicated by $L + \Delta L$ and L , respectively.
- (3) $\Delta A \equiv \log [(L + \Delta L)/L] \approx \Delta L/L$ is obtained.
- (4) $\Phi_{ij} \equiv \Delta A_i / \Delta A_j$ is obtained.
- (5) Since Φ_{ij} corresponds on a substantially one-to-one base to SaO₂, Φ_{ij} is converted to SaO₂.

[0003] Many apparatuses which are currently commercially available, and which measure SaO₂ employ two wavelengths, and, when above-described Φ_{ij} is to be converted to SaO₂, use a conversion table. In the case of a two-wavelength apparatus, the use of a conversion table is not particularly problematic. In the case where a larger number of wavelengths are used in order to improve the measurement accuracy, however, the conversion must be performed by using a calculation expression which is obtained theoretically and experimentally.

[0004] For example, as a related-art apparatus which measures continuously SaO₂ in a non-invasive manner by using a volume variation of arterial blood caused by pulsation, there is a five-wavelength pulse oximeter which irradiates living tissue with five light beams of different wavelengths (see JP-A-2005-95606).

[0005] The pulse oximeter disclosed in JP-A-2005-95606 includes: a light emitting portion which irradiates living tissue with five light beams of different wavelengths; a light receiving portion which receives the light beams that are emitted from the light emitting portion, and that are transmitted through or reflected from the living tissue, and which converts the light beams to electric signals; an optical-density-variation calculating portion which obtains optical density variations for the living tissue on the basis of variations of the transmitted or reflected light beams of different wavelengths and output from the light receiving portion; an optical-density-variation-ratio calculating portion which obtains at least four of mutual ratios of five optical density variations obtained in the optical-density-variation calculating portion; and an oxygen saturation calculating portion which, based on the optical-density-variation ratios obtained in the optical-density-variation-ratio calculating portion, calculates oxygen saturation in blood while using four unknowns of the SaO₂, the venous oxygen saturation, a ratio of variations of arterial blood and venous blood, and a tissue term, and obtains oxygen saturation of arterial blood while eliminating artifacts of variations of venous blood and the tissue.

[0006] According to the thus configured pulse oximeter disclosed in JP-A-2005-95606, in the case where venous blood is pulsated by any reason, an artifact of the pulsation can be surely eliminated, and SaO₂ can be accurately measured without producing a time delay and smoothing. In the case where the pulse wave is so small that a pulse oximetry is impossible, body motion is intentionally applied, thereby enabling SaO₂ contained in this case to be obtained. The pulse oximeter has another advantage that also venous oxygen saturation can be simultaneously measured.

[0007] A longstanding problem of a pulse oximetry is that transmitted or reflected light is disturbed by mechanical disturbances such as body motion. Namely, disturbances of transmitted or reflected light cause adequate detection of peaks and bottoms of a measured pulsative waveform to be hardly performed.

[0008] A related-art technique which has been proposed or adopted as a countermeasure against these problems is a statistical technique in which the correct value of SaO₂ is estimated from preceding and subsequent data. However, the technique has the following problems.

- (1) Since a long time delay is produced, detection of, for example, a start of reduction of SaO₂ is delayed.
- (2) Changes of SaO₂ are smoothed. When SaO₂ is largely reduced, for example, the degree of the reduction cannot be known.

[0009] In the related-art pulse oximetry technique, it will be further expected that a change in SaO₂ of a patient is quickly detected, so that the change is early coped with. In order to utilize the original feature of the pulse oximetry technique, the above-discussed problems must be solved.

Furthermore, it has been found that, in the related-art pulse oximetry technique which is based on determination of peaks and bottoms of the pulsative waveform of measured transmitted or reflected light cannot obtain a satisfactory measurement result when the body a patient is vigorously moved.

[0010] From this viewpoint, the following related-art technique has been proposed, a time-segmented pulse oximetry and pulse oximeter in which, with respect to the pulsative waveform of measured transmitted or reflected light, the whole of a signal of the measured transmitted or reflected light is used, whereby SaO₂ can be adequately measured (see JP-A-2007-90047).

[0011] In the related-art technique disclosed in JP-A-2007-90047, the whole of time series data of the transmitted or reflected light is used, so that determination of peaks and bottoms of the measured waveform is not necessary. Namely, the related-art technique disclosed in JP-A-2007-90047 is **characterized in that** light emitting elements irradiate living tissue with a plurality of light beams of different wavelengths, light receiving elements receive the light beams transmitted through or reflected from the living tissue, and converts the respective light beams to electric signals, time series data of the electric signals obtained by the light receiving elements are time-segmented, with respect to the segmented time series data, slope values of regression lines between two different wavelengths are calculated, the calculated slope values are converted to SaO₂, respectively, and then smoothing is performed, thereby obtaining SaO₂ from which an artifact of body motion is eliminated.

[0012] According to the related-art technique disclosed in JP-A-2007-90047, with respect to the pulsative waveform of measured transmitted or reflected light, therefore, determination of peaks and bottoms of the measured waveform is not performed, and the whole of time series data of the transmitted or reflected light is used, whereby an artifact of body motion is eliminated, contribution to improvement of the measurement accuracy of SaO₂ is obtained, and measurement flexibility of a measurement portion can be enhanced. Even with these two related-art techniques, an artifact of the body motion can not be eliminated sufficiently.

SUMMARY

[0013] It is therefore an object of the invention to provide a pulse oximetry and pulse oximeter in which, with respect to the pulsative waveform of measured transmitted or reflected light, the whole of time series data of the transmitted or reflected light is used, whereby an artifact of body motion is eliminated, and contribution to further improvement of the measurement accuracy of SaO₂ is obtained.

[0014] In order to achieve the object, according to the invention, there is provided a pulse oximetry comprising:

irradiating living tissue with a plurality of light beams of different wavelengths;
 receiving the light beams transmitted through or reflected from the living tissue and converting the received light beams to electric signals which correspond to the different wavelengths;
 time-segmenting time series data of the electric signals;
 calculating, with respect to each of the segmented time series data of the electric signals, a slope value of a regression line between each two of the electric signals;
 calculating SaO₂ based on the slope values of each of the segmented time series data of the electric signals;
 constructing a histogram of SaO₂ for each predetermined number of time segments; and
 obtaining a mode value from the histogram as SpO₂ to be output of the pulse oximetry.

[0015] The time series data of the electric signals may be passed through a filter to block a low-frequency component, before time-segmenting the time series data of the electric signals.

[0016] The pulse oximetry may further include: calculating, with respect to each of the segmented time series data of the electric signals, correlation between each two of the electric signals. When the correlation is less than a predetermined value, the slope value which corresponds to the correlation may be deleted.

[0017] A smoothing process may be applied to the histogram of the SaO₂, before obtaining the mode value.

[0018] In order to achieve the object, according to the invention, there is also provided a pulse oximeter comprising:

a light emitter, which irradiates living tissue with a plurality of light beams of different wavelengths;
 a light receiver, which receives the light beams transmitted through or reflected from the living tissue and which converts the received light beams to electric signals which correspond to the different wavelengths;
 a processor, which segments time series data of the electric signals;
 a slope value calculator, which calculates, with respect to each of the segmented time series data of the electric signals, a slope value of a regression line between each two of the electric signals;
 an SaO₂ calculator, which calculates SaO₂ based on the slope value of each of the segmented time series data of the electric signals;
 a histogram constructor, which constructs a histogram of SaO₂ for each predetermined number of time segments; and
 an obtainer, which obtains a mode value from the histogram as SpO₂ to be output of the pulse oximeter.

BRIEF DESCRIPTION OF THE DRAWINGS**[0019]**

- 5 Fig. 1 is a diagram schematically showing the configuration of a pulse oximeter which performs a pulse oximetry of the present invention.
 Fig. 2 is a diagram showing the configuration of a system in a calculating portion of the pulse oximeter shown in Fig. 1.
 Fig. 3 is a waveform chart showing a change of SpO₂ which is obtained in a rest side by a five-wavelength calculation while peaks and bottoms are determined for each beat.
 10 Fig. 4 is a waveform chart showing a change of SpO₂ which is obtained in a body-motion side by the five-wavelength calculation while peaks and bottoms are determined for each beat.
 Fig. 5 is a waveform chart showing a change of 5wSall which is obtained in the body-motion side for each time segment.
 Fig. 6 is a waveform chart showing a display example of a histogram in the pulse oximetry of the invention.
 15 Fig. 7 is a waveform chart showing a change of SpO₂ which is obtained in the body-motion side by the pulse oximetry of the invention.

DETAILED DESCRIPTION OF EMBODIMENTS

- 20 **[0020]** Next, an embodiment of a pulse oximetry of the present invention will be described in relation with the configuration of a pulse oximeter which performs the pulse oximetry, in detail with reference to the accompanying drawings.

I. Summary of configuration of pulse oximeter

- 25 **[0021]** Fig. 1 is a diagram schematically showing the configuration of a pulse oximeter which performs a pulse oximetry of the present invention. In Fig. 1, the reference numeral 10 denotes a light emitting portion in which five light emitting elements LED1 to LED5 that irradiate living tissue with five light beams of different wavelengths, respectively, 12 denotes the living tissue which is irradiated with the light beams emitted from the light emitting portion 10, and 14 denotes a light receiving portion configured by: a light receiving element PD which receives light beams transmitted through or reflected
 30 from the living tissue 12; a current-voltage converter 16; and an AD converter 18.
[0022] The reference numeral 20 denotes a storage portion configured by transmitted-light-signal temporary storage devices 20A to 20E which temporarily store transmitted or reflected light signals obtained by the light receiving element PD of the light receiving portion 14, in time series for the respective wavelengths. For example, 60 transmitted or reflected light signals are stored per second in each of the storage devices.
 35 **[0023]** The reference numeral 30 denotes a calculating portion which, on the basis of the transmitted or reflected light signals L1 to L5 that are temporarily stored in time series in the respective transmitted-light-signal temporary storage devices 20A to 20E, performs the following procedures: (1) the transmitted or reflected light signals L1 to L5 are segmented for each predetermined time; (2) with respect to each of the transmitted or reflected light signals L1 to L5 which are segmented for each predetermined time, then, a slope value of a regression line between each two different wavelengths
 40 is calculated; (3) SaO₂ is calculated based on the calculated slope values; (4) a correlation coefficient is further calculated, a slope value in the case where the correlation coefficient is less than a predetermined value is deleted, and a histogram of SaO₂ is constructed for every predetermined number of time segments; and (5) a mode value of the histogram is set as an SpO₂ value.
[0024] The reference numeral 22 denotes a timing device which is configured so as to control light emitting timings of the light emitting elements LED1 to LED5 of the light emitting portion 10, and timings of storing the transmitted or reflected light signals in the transmitted-light-signal temporary storage devices 20A to 20E of the storage portion 20.
[0025] Fig. 2 is a diagram showing the configuration of a system for performing the above-described calculating procedures in an oxygen saturation calculator that functions as the calculating portion 30. In Fig. 2, the reference numeral 32 denotes a segment storage portion for the transmitted or reflected light signals. The segment storage portion is
 50 configured by segment storing circuits 32A to 32E which segment the transmitted or reflected light signals L1 to L5 supplied from the transmitted-light-signal temporary storage devices 20A to 20E, for each predetermined time (for example, 0.2 second), and which sequentially store the transmitted or reflected light signals in time series for each of the segmented times.
[0026] The reference numeral 34 denotes a slope-value calculating portion. The calculating portion is configured by slope-value calculating circuits 34a, 34b, 34c, 34d calculate, using output of 32, slope values Φ_{12} , Φ_{32} , Φ_{42} , Φ_{52} of the regression lines, respectively.
 55 **[0027]** The reference numeral 36 denotes a first calculating circuit which obtains the SaO₂ value as a solution of simultaneous equations with the slope values Φ_{12} , Φ_{32} , Φ_{42} , Φ_{52} of the regression lines that are obtained by the slope-

value calculating circuits 34a, 34b, 34c, 34d. The value which is the solution of simultaneous equations obtained by the first calculating circuit is called 5wSall.

[0028] The reference numeral 38 denotes a second calculating circuit which, with respect to SaO2 that is obtained as the solution of the simultaneous equations, obtains a histogram for every predetermined number of time segments (for example, every 5 seconds), and which determines the mode value of the histogram. Therefore, the second calculating circuit 38 calculates blood oxygen saturation [SpO2]. This is output of this pulse oximetry.

[0029] In order to obtain a higher accuracy, it is preferred to additionally perform at least one of the following methods.

<1> a low-frequency component of log Li is eliminated.

<2> Φi2 is selected based on correlation between two data.

<3> Smoothing is performed on the histogram.

II. Calculating processing of pulse oximeter

[0030] Next, the operation of calculating SaO2 by the configuration of the above-described pulse oximeter, i.e., the pulse oximetry of the invention will be described together with the function of the pulse oximeter.

(1) Processing of time-segmenting transmitted or reflected light signal

[0031] First, the five light emitting elements LED1 to LED5 of the light emitting portion 10 sequentially emit light beams of different wavelengths λ1, λ2, λ3, λ4, and λ5, respectively, on the basis of a signal from the timing device 22. Therefore, the light receiving portion 14 receives light beams transmitted through or reflected from the living tissue 12, and, in accordance with the wavelengths of the light emitting elements LED1 to LED5, the transmitted or reflected light signals L1, L2, L3, L4, L5 are stored at respective predetermined timings into the transmitted-light-signal temporary storage devices 20A to 20E of the storage portion 20 (see Fig. 1).

[0032] The transmitted or reflected light signals L1 to L5 which are stored respectively in the transmitted-light-signal temporary storage devices 20A to 20E in this way are supplied to the segment storing circuits 32A to 32E of the segment storage portion 32 in the calculating portion 30, segmented for each predetermined time (for example, 0.2 second), and then sequentially stored in time series for each of the segmented times (see Fig. 2).

(2) Calculating processing of obtaining slope value of regression line relating to time-segmented transmitted or reflected light beams

[0033] The calculation of blood oxygen saturation (SpO2) is performed based on optical density variations (ΔAi) which are obtained for the transmitted or reflected light beams of, for example, five wavelengths. The oxygen saturation is obtained by the following expression using a ratio (Φij, i and j are wavelength number) of the optical density variations.

[0034] The elements constituting the pulsation of a transmitted or reflected light beam are arterial blood (a), venous blood (v), and tissue other than blood, i.e., pure tissue (t).

$$\Phi_{ij} \equiv \Delta A_i / \Delta A_j$$

$$= [\sqrt{E_{ai}(E_{ai} + F)} + \sqrt{E_{vi}(E_{vi} + F)} * V + E_{xi}] / [\sqrt{E_{aj}(E_{aj} + F)} + \sqrt{E_{vj}(E_{vj} + F)} * V + E_{xj}]$$

where

$$\Delta A_i \equiv \log[(L_i + \Delta L_i) / L_i] \cong \Delta L_i / L_i$$

$$E_{ai} \equiv S_a E_{oi} + (1 - S_a) E_{ri}$$

$$E_{vi} \equiv S_v E_{oi} + (1 - S_v) E_{ri}$$

5

$$V \equiv \Delta D_v / \Delta D_a$$

10

$$E_{xi} \equiv Z_{ti} \Delta D_t / (H_b \Delta D_a) \equiv A_i E_{x2} + B_i$$

[0035] In the above expression, L_i is a tissue transmitted or reflected light beam, ΔA_i is an optical density variation, E_{oi} is an extinction coefficient of oxygenated hemoglobin, E_{ri} is an extinction coefficient of deoxygenated hemoglobin, S_a is S_aO_2 , S_v is oxygen saturation of peripheral venous blood (S_vO_2), ΔD_a is a variation of the effective thickness of arterial blood, ΔD_v is a variation of the effective thickness of venous blood, ΔD_t is a variation of the effective thickness of pure tissue, Z_{ti} is a constant of attenuation of pure tissue, E_{x2} is the value of E_{xi} at a second wavelength, and A_i and B_i are tissue constants (determined by actual measurement).

Therefore, the above expression has four unknowns of S_a , S_v , V , and E_{x2} .

[0036] In this case, tissue transmitted or reflected light beams are measured at five adequate wavelengths, simultaneous equations with 4 unknowns are set with respect to the above expression, and then S_a can be obtained as the solution of the simultaneous equations. Preferred examples of the five wavelengths are $\lambda_1 = 805$ nm, $\lambda_2 = 875$ nm, $\lambda_3 = 660$ nm, $\lambda_4 = 700$ nm, and $\lambda_5 = 730$ nm.

[0037] In the time-segmented oximetry of the invention, based on the transmitted or reflected light signals L_1 to L_5 of the five wavelengths (λ_1 to λ_5) which are time-segmented and stored, therefore, the segment storage portion 32 obtains the slope values (Φ_{ij} , i and j are wavelength number) of the regression lines by using the following expression. Namely, the slope value (Φ_{ij}) in the above corresponds to $\Phi_{ij} = \Delta A_i / \Delta A_j$ above. In the following expression, n is the number of data in a time segment, t is a segmented time (for example, 0.2 second), and Σ is a sum of data in a segmented time.

30

$$\Phi_{ij} \equiv \{ n \Sigma [L_i(t) * L_j(t)] - \Sigma [L_i(t)] * \Sigma [L_j(t)] \} / \{ n \Sigma L_j(t)^2 - [\Sigma L_j(t)]^2 \}$$

35

(3) Calculating processing of obtaining solution of simultaneous equations with slope values

[0038] On the basis of the above expression, simultaneous equations with 4 unknowns are set with respect to the slope values (Φ_{12} , Φ_{32} , Φ_{42} , Φ_{52}) of the regression lines for the tissue transmitted or reflected light beams of the five wavelengths (λ_1 to λ_5), and S_a is calculated as a solution of the simultaneous equations (see Fig. 2). These S_a are named S_{wSall} .

III. Example of calculating processing

[0039] An example where, based on the above-described pulse oximetry of the invention, S_aO_2 is calculated with respect to actual measurement data of a subject will be described together with graphs in which the example is compared with the case of a related-art pulse oximetry, and which show their measurement results.

[0040] The light emitting portion 10 and the light receiving portion 14 are attached to a finger tip of a subject, and breathing is performed in the following manner.

50

- <1> Air breathing is performed.
- <2> S_aO_2 is reduced by holding breath.
- <3> Air breathing is again performed.
- <4> S_aO_2 is increased by oxygen breathing.

55

[0041] In the middle of <1>, a motion of squeezing a sponge by hand is performed. The body motion is continued to the middle of <4>.

Similarly, a light emitting portion and a light receiving portion are attached to the other hand opposite to the one which

performs the body motion. The other hand is kept at rest, and data of the other hand are set as control data.

[0042] Fig. 3 shows a result of SpO₂ which is obtained in the rest side by a five-wavelength calculation while peaks and bottoms are determined for each beat. In Fig. 3, a change of SaO₂ due to a change of breathing is clearly shown. In the graph, timings when breathing is changed and the body motion is started and ended are indicated by vertical bars.

[0043] Fig. 4 shows a result of SpO₂ which is obtained in the body-motion side by a five-wavelength calculation while peaks and bottoms are determined for each beat. In Fig. 4, SpO₂ is largely disturbed. This disturbance is caused by the artifact of the body motion.

[0044] Fig. 5 shows the distribution characteristic of 5wSall which is obtained in the body-motion side for each 0.2 second by the method of the invention. Namely, Fig. 5 is a view showing results of the following processing.

<1> The transmitted or reflected light signal Li is logarithmically converted to log Li.

<2> A low-frequency component of log Li is eliminated. Specifically, the average value of log Li for each 0.1 second is subtracted from log Li.

<3> For each 0.2 second, a slope $\Phi i2$ of a regression line of log Li ($i = 1, 3, 4, \text{ and } 5$) and log L2 is obtained.

<4> For each 0.2 second, a correlation coefficient Ri2 of log Li ($i = 1, 3, 4, \text{ and } 5$) and log L2 is obtained, and $R12 \cdot R32 \cdot R42 \cdot R52 = PR$ is obtained.

<5> $\Phi i2$ in the case of $PR < 0.9$ is deleted.

<6> The remaining $\Phi i2$ is converted to SaO₂ on the basis of simultaneous equations. This is 5wSall.

<7> 5wSall is time-segmented for each 5 seconds, and a histogram of time segments of 5 seconds is obtained.

<8> The histogram is smoothed. Fig. 6 shows a display example of such a histogram.

<9> The mode value is determined on the basis of the histogram of 5wSall.

<10> The result is output as SpO₂. Fig. 7 shows a change of SpO₂ which is obtained in the body-motion side.

[0045] As described above, according to the pulse oximetry of the invention, an artifact of body motion is sufficiently eliminated, and a rapid change of SaO₂ is definitely measured. Particularly, it is confirmed that the timing when the reduction of SaO₂ is started can be detected without delay.

[0046] In the above, the preferred embodiment of the invention has been described. However, the invention is not restricted to the embodiment. Although the case where five wavelengths are used has been described, the invention can be applied also to the case where the number of wavelengths is larger or smaller than five. Furthermore, the invention can be applied also to all of measurement objects which pulsate, for instance, together with arterial blood, such as CO hemoglobin in blood, the diluted state of a dye injected from the outside of the body, etc. The interval of the time segment may be adequately changed in accordance with the respective objects. Various modifications may be performed without departing from the spirit of the invention.

[0047] According to an aspect of the invention, with respect to the pulsative waveform of measured transmitted or reflected light, determination of peaks and bottoms of the measured waveform is not performed, and the whole of time series data of the transmitted or reflected light is used, whereby an artifact of body motion is eliminated, and contribution to improvement of the measurement accuracy of SaO₂ is obtained.

Claims

1. A pulse oximetry comprising:

irradiating living tissue with a plurality of light beams of different wavelengths;
receiving the light beams transmitted through or reflected from the living tissue and converting the received light beams to electric signals which correspond to the different wavelengths;
time-segmenting time series data of the electric signals;
calculating, with respect to each of the segmented time series data of the electric signals, a slope value of a regression line between each two of the electric signals;
calculating SaO₂ based on the slope values of each of the segmented time series data of the electric signals;
constructing a histogram of SaO₂ for each predetermined number of time segments; and
obtaining a mode value from the histogram as SpO₂ to be output of the pulse oximetry.

2. The pulse oximetry according to claim 1, wherein

the time series data of the electric signals are passed through a filter to block a low-frequency component, before time-segmenting the time series data of the electric signals.

3. The pulse oximetry according to claim 1, further comprising:

calculating, with respect to each of the segmented time series data of the electric signals, correlation between each two of the electric signals,

wherein, when the correlation is less than a predetermined value, the slope value which corresponds to the correlation is deleted.

4. The pulse oximetry according to claim 1, wherein a smoothing process is applied to the histogram of the SaO₂, before obtaining the mode value.

5. A pulse oximeter comprising:

a light emitter, which irradiates living tissue with a plurality of light beams of different wavelengths;
a light receiver, which receives the light beams transmitted through or reflected from the living tissue and which converts the received light beams to electric signals which correspond to the different wavelengths;
a processor, which segments time series data of the electric signals;
a slope value calculator, which calculates, with respect to each of the segmented time series data of the electric signals, a slope value of a regression line between each two of the electric signals;
an SaO₂ calculator, which calculates SaO₂ based on the slope values of each of the segmented time series data of the electric signals;
a histogram constructor, which constructs a histogram of SaO₂ for each predetermined number of time segments;
and
an obtainer, which obtains a mode value from the histogram as SpO₂ to be output of the pulse oximeter.

FIG. 1

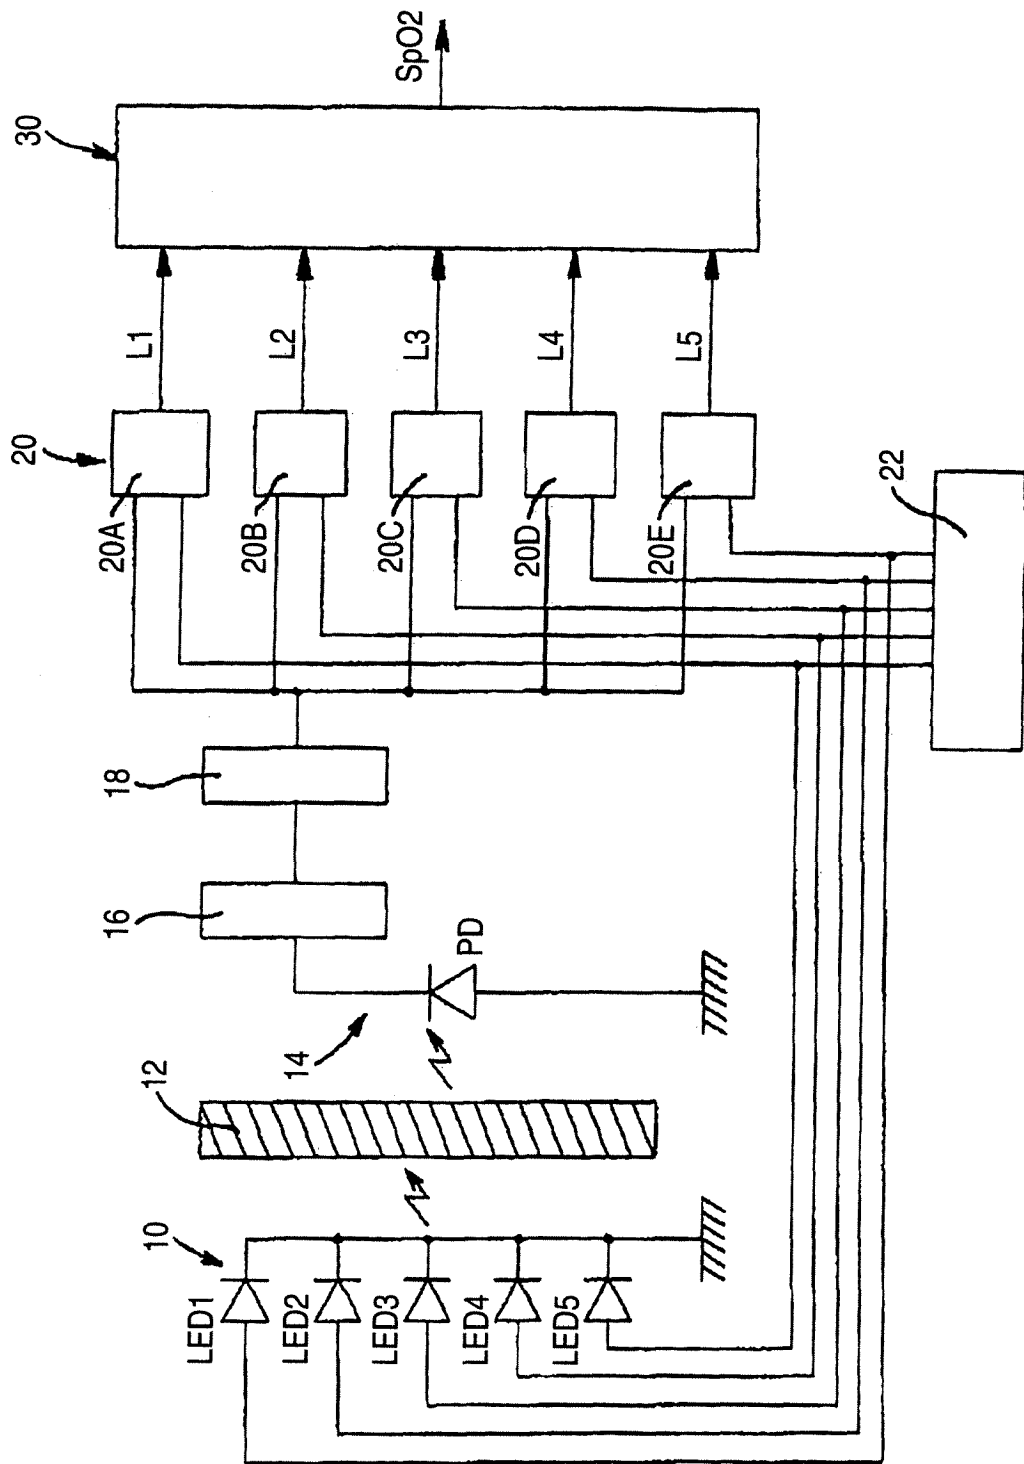


FIG. 2

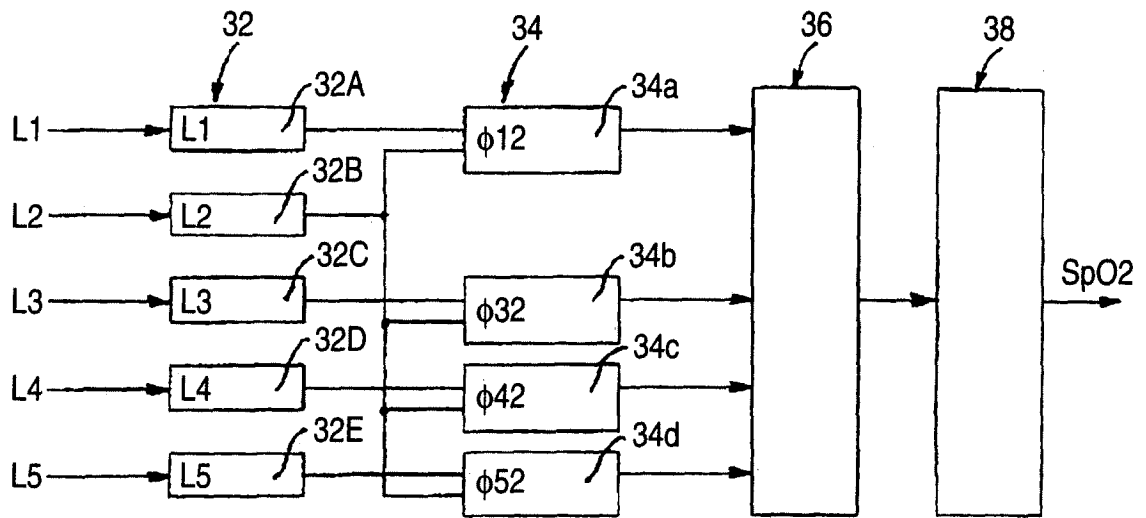


FIG. 3

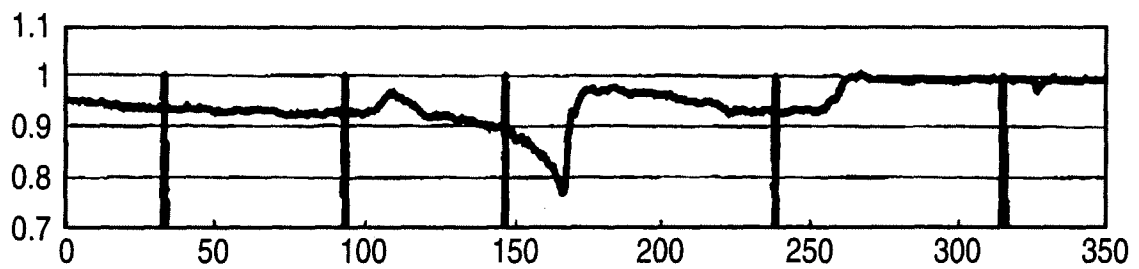


FIG. 4

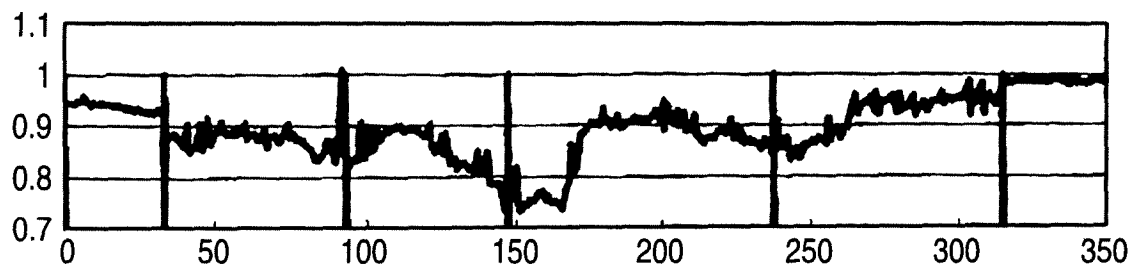


FIG. 5

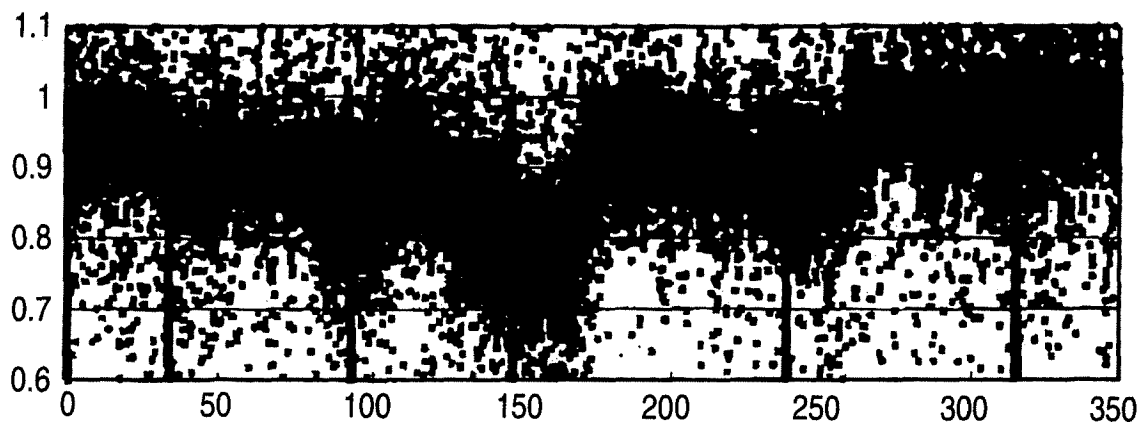


FIG. 6


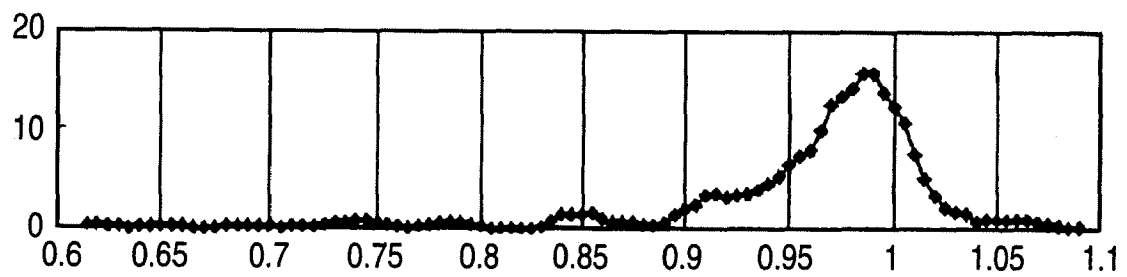


FIG. 7



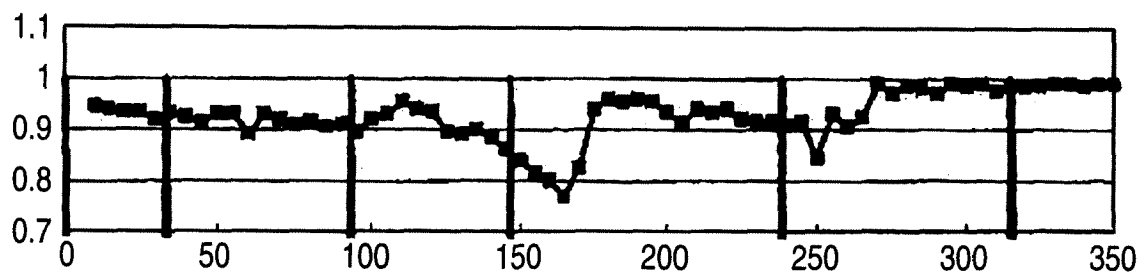

EUROPEAN SEARCH REPORT

Application Number
EP 09 16 2886

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
Y	US 2007/049812 A1 (AOYAGI TAKUO [JP] ET AL) 1 March 2007 (2007-03-01) * paragraph [0043] - paragraph [0062] * * figures 1,2 *	1-3,5	INV. A61B5/1455
Y	US 2008/033266 A1 (DIAB MOHAMED K [US] ET AL) 7 February 2008 (2008-02-07) * paragraph [0248] * * paragraph [0273] - paragraph [0274] * * paragraph [0342] - paragraph [0344] * * figures 12,22-24 *	1-3,5	
A	JP 07 327964 A (NIPPON KODEN KOGYO KK) 19 December 1995 (1995-12-19) * the whole document *	1-5	
A	US 2004/267140 A1 (ITO KAZUMASA [JP] ET AL) 30 December 2004 (2004-12-30) * the whole document * * figures 2B,7,8 *	1-5	
D,A	JP 2007 090047 A (NIPPON KODEN KOGYO KK) 12 April 2007 (2007-04-12) * the whole document *	1-5	
D,A	JP 2005 095606 A (NIPPON KODEN KOGYO KK) 14 April 2005 (2005-04-14) * the whole document *	1-5	TECHNICAL FIELDS SEARCHED (IPC) A61B
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 12 August 2009	Examiner Gärtner, Andreas
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

3

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 09 16 2886

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

12-08-2009

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2007049812 A1	01-03-2007	NONE	
US 2008033266 A1	07-02-2008	US 2009182211 A1	16-07-2009
JP 7327964 A	19-12-1995	JP 3270917 B2	02-04-2002
US 2004267140 A1	30-12-2004	JP 2008188442 A	21-08-2008
JP 2007090047 A	12-04-2007	NONE	
JP 2005095606 A	14-04-2005	NONE	

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2005095606 A [0004] [0005] [0006]
- JP 2007090047 A [0010] [0011] [0012]

专利名称(译)	脉搏血氧仪和脉搏血氧仪		
公开(公告)号	EP2135550A1	公开(公告)日	2009-12-23
申请号	EP2009162886	申请日	2009-06-17
[标]申请(专利权)人(译)	日本光电工业株式会社		
申请(专利权)人(译)	日本光电公司		
当前申请(专利权)人(译)	日本光电公司		
[标]发明人	AOYAGI TAKUO KANEMOTO MICHIO FUSE MASAYOSHI UKAWA TEIJI		
发明人	AOYAGI, TAKUO KANEMOTO, MICHIO FUSE, MASAYOSHI UKAWA, TEIJI		
IPC分类号	A61B5/1455 A61B5/00		
CPC分类号	A61B5/1455 A61B5/7207		
优先权	2008160013 2008-06-19 JP		
其他公开文献	EP2135550B1		
外部链接	Espacenet		

摘要(译)

脉搏血氧测定法包括：用多个不同波长的光束照射活组织；接收通过活组织透射或从活组织反射的光束，并将接收到的光束转换成对应于不同波长的电信号；时间分段电信号的时间序列数据；计算关于每个电信号的分段时间序列数据的每两个电信号之间的回归线的斜率值；根据电信号的每个分段时间序列数据的斜率值计算SaO2；为每个预定数量的时间段构建SaO2直方图；从直方图中获得模式值作为SpO2，输出脉搏血氧饱和度。

