



(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
30.10.2013 Bulletin 2013/44

(51) Int Cl.:
A61B 5/00 (2006.01)

(21) Application number: **11851174.0**

(86) International application number:
PCT/ES2011/070877

(22) Date of filing: **19.12.2011**

(87) International publication number:
WO 2012/085315 (28.06.2012 Gazette 2012/26)

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **MARTINEZ NICOLAS, Antonio**
E-30100 Murcia (ES)
- **MADRID PEREZ, Juan Antonio**
E-30100 Murcia (ES)
- **ROL DE LAMA, María Angeles**
E-30100 Murcia (ES)
- **ORTIZ TUDELA, Elisabet**
E-30100 Murcia (ES)

(30) Priority: **21.12.2010 ES 201031894**

(71) Applicant: **Universidad de Murcia**
30100 Espinardo, Murcia (ES)

(72) Inventors:
• **SARABIA CARRAZO, Juan Antonio**
E-30100 Murcia (ES)

(74) Representative: **Carvajal y Urquijo, Isabel**
Clarke, Modet & Co.
c/ Goya, 11
28001 Madrid (ES)

(54) **DEVICE WHICH COMPRISES A PHYSICAL ACTIVITY AND POSITION SENSOR, A PERIPHERAL TEMPERATURE SENSOR AND A LIGHT SENSOR FOR PROVIDING INFORMATION RELATING TO THE STATE OF THE CIRCADIAN SYSTEM**

(57) The invention is a device consisting of at least one body position and activity sensor, at least one peripheral temperature sensor and at least one light sensor, configured to provide information on the circadian system status and the sleep-wake status of an individual based

on the data obtained from said sensors. It can be placed on the wrist of the subject, or on the subject's arm. The device may also include a blood pressure sensor. This device may be used in general studies of the human circadian system and, more specifically, for the study of sleep-wake and blood pressure rhythms.

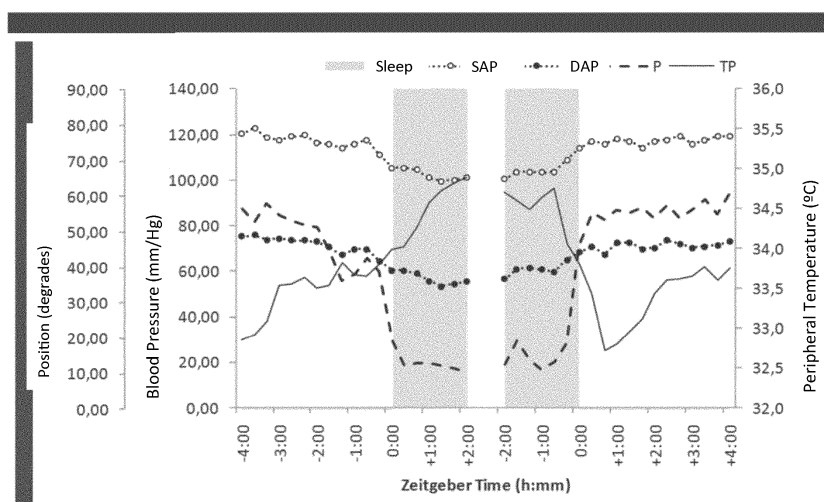


Fig 3

Description

FIELD OF THE INVENTION

[0001] The invention concerns a device that constitutes a body position and activity sensor, a peripheral temperature sensor and a light sensor. This device may be used in general studies of the human circadian system and, more specifically, for the study of sleep-wake and blood pressure rhythms.

BACKGROUND OF THE INVENTION

[0002] Biological rhythms are biological variables that oscillate on a regular basis and have a specific period. Circadian rhythms have a period of approximately 24 hours.

[0003] The circadian system consists of all structures responsible for generating the different biological rhythms and synchronizing them to environmental cycles. Its main component is a pacemaker made up by a group of neurons located in the hypothalamus (the suprachiasmatic nucleus). This pacemaker uses nervous and hormonal signals to control the circadian rhythms of the rest of the body.

[0004] In order to evaluate the functioning of the circadian system correctly, one or more biological rhythms controlled by the circadian pacemaker must be monitored for the longest period of time possible, the ideal being one or more weeks. Traditional methods of measurement involve invasive procedures, such as the determination of blood melatonin and cortisol levels; uncomfortable methods, such as recording the body's core temperature with a rectal probe; and procedures in which the determination of one variable alters one of the most important rhythms, the sleep-wake rhythm, as it requires the active cooperation of the patient or experimental subject, as in the case of determining melatonin and cortisol levels in saliva or measuring tympanic temperature.

[0005] Its ease of use for recording and non-invasive nature have gradually led to the increased use of actimetry for evaluating the human circadian system. Actimetry allows for determining whether the subject is asleep or engaged in various intensities of activity based on the movements within a certain area of the body, usually the wrist. However, the use of actimetry to evaluate the circadian system presents certain disadvantages, among them the fact that it is difficult to differentiate between the initial rest period associated with sleep and when the subject has removed the sensor, for example, to take a bath or shower, or an increase in movement associated with car trips or even the movement of a partner in bed.

[0006] Recently, the peripheral temperature rhythm has been suggested as a marker rhythm, given that it has obvious advantages in terms of measurement and is also a circadian system indicator (Sarabia, J.A. et al., Circadian rhythm of wrist temperature in normal-living subjects. A candidate of new index of the circadian sys-

tem. *PhysiolBehav.* 2008; 95(4) :570-80).

[0007] The body's peripheral temperature follows a circadian profile in such a way that the temperature increases as a prelude to sleep and remains high for the rest of the night. Upon awakening, it drops sharply, and its levels remain low throughout the day. In fact, it is this rhythm that instigates the changes in the core body temperature, which has been used for decades as a reliable marker rhythm in chronobiological studies. This is due to the fact that vasodilation of the extremities and the subsequent increase in peripheral temperature is what triggers the drop in core temperature. Recent studies have identified a direct relationship with melatonin production, making it an indirect method of determining melatonin levels in the body.

[0008] The problem this technique poses is obtaining information on the status of the human circadian system in a non-invasive manner and with more than one variable. The solution proposed by this invention is a device that jointly integrates and processes the information generated by a body position and activity sensor, a peripheral temperature sensor worn on the wrist and a light sensor.

DESCRIPTION OF THE INVENTION

[0009] The invention is a device consisting of at least one body position and activity sensor, at least one peripheral temperature sensor and at least one light sensor, configured to provide information on the circadian system status and the sleep-wake status of an individual based on the data obtained from said sensors.

[0010] In terms of the present invention, "circadian system" is understood to mean the set of biological variables in an individual, which undergo regular oscillations over a 24-hour period. The invented device stores and processes information about peripheral temperature of the wrist, body position and activity and environmental light parameters. All sensors can be programmed to record information over a wide range of time intervals. The device's sampling interval can be programmed, which makes it more useful in clinical settings.

[0011] The body position and activity sensor is a 3-axis accelerometer with a measurement range of $\pm 3g$ that provides information on the position of the X, Y and Z axes. These data are used to define 2 variables: body position and motor activity. The values for body position are defined with regard to the X axis (perpendicular to the earth's surface) and with a range between 0 and 90°, with 0° representing a horizontal position and 90° representing the maximum vertical position. Motor activity is defined as the number of degrees of change in the position of the activity sensor as compared to the recording taken immediately before, and the average acceleration to which the sensor has been subjected during each recording interval.

[0012] The light sensor records exposure to different light intensities the subject receives (measured in luxes), evaluated at very short time intervals. Light intensity is

the most important external synchronization signal, and is responsible for setting the time of the circadian clock and preventing it from falling behind.

[0013] A preferred implementation is a device based on this invention, which is placed on the subject's wrist.

[0014] Another implementation of this invention is a device which also consists of at least one blood pressure sensor and that is programmed to provide information about the status of a subject's blood pressure.

[0015] This device improves the diagnostic accuracy of changes in circadian blood pressure rhythms, enabling the subject's rest period to be objectively determined based on position changes. Existing devices for blood pressure measurement arbitrarily establish rest periods, and therefore do not provide a reliable measurement of the changes in blood pressure values when the subject lies down or stands up. These changes are very important for the diagnosis of hypertension.

[0016] A preferred implementation is the use of the invention in a way in which the aforementioned peripheral temperature and light sensors are positioned on the wrist of the subject, while the body position and activity and blood pressure sensors are placed on the subject's arm.

[0017] Yet another implementation of the invention is a procedure to determine the circadian system status and the sleep-wake status of the subject that consists of:

- a) Obtaining peripheral temperature, motor activity per minute and body position values for the subject.
- b) Drawing conclusions as to the circadian system status and the sleep-wake status of a subject based on the changes in the values from step a).

[0018] A preferred implementation involves a procedure using the invention to obtain information on blood pressure and hypertension, characterized by the fact that in step a) blood pressure measurements are also taken for the subject, and in step b) the blood pressure values are compared, along with the rest of the values, to determine any changes in blood pressure upon lying down or standing up.

[0019] Figure 3 shows the inverse proportional relationship that exists between the peripheral temperature pattern and blood pressure, and the direct relationship between the position measured on the arm and blood pressure.

BRIEF DESCRIPTION OF THE FIGURES

[0020]

Figure 1. Seven-day recording and average daily wave of the main recorded variables; light intensity (Figure 1A), peripheral temperature (Figure 1B), motor activity (Figure 1C), body position (Figure 1D) and the integrated TAP variable (Figure 1E) for a representative subject. The grey shaded area shows the subject's sleep periods, and the values of

the recorded variables are shown by the solid line.

Figure 2. Comparison of the TAP variable and sleep probability. The vertical axis shows the probability of sleep, expressed in decimal form. Accordingly, a value of 1 indicates that 100% of the subjects were asleep, and a value of 0 indicates that they were all awake.

Figure 3. Representation of wrist peripheral temperature (solid line), body position (dotted line), systolic blood pressure (empty circles) and diastolic blood pressure (solid circles). The four hours prior to going to bed and the two hours afterwards are shown, as are the two hours prior to getting up and the four hours afterwards. The shaded area represents the rest phase. The data are adapted to a synchronizer (*zeitgeber*), which in this case is sleep onset (left) and sleep end (right). Therefore, the horizontal axis represent time in relation to the start and end of sleep (*zeitgeber time*).

EXAMPLES OF THE INVENTION

Example 1. Recording wrist peripheral temperature, motor activity and body position variables, as well as blood pressure, in various subjects.

[0021] Data was recorded for 37 subjects, who wore sensors consecutively for one week. All subjects were young people between 20 and 30 years of age. The subjects lived a normal life, as the technique is precisely intended to study the status of the circadian rhythm in persons without the need to modify their daily habits. The sensors were only removed to allow the subjects to shower.

Example 2. Processing of physiological data

[0022] TAP is a modular variable and consists of 3 separate variables: peripheral temperature (T), motor activity per minute (A) and body position (P). The TAP variable was obtained in the following manner: the first step consisted of standardizing these variables as values between 0 and 1. To do this, the 95th and 5th percentiles were calculated for each variable and participating subject. All values above the 95th percentile were considered to be 1, and all values below the 5th percentile were considered to be 0. For intermediate values between the 5th and 95th percentile, the proportional value between 0 and 1 was calculated.

[0023] So that the highest values were indicative of greater levels of activity in all three variables, the standardized values were inverted for the peripheral temperature ($T' \text{ norm} = 1 - T \text{ norm}$). Once the data had been standardized, the sum of the 3 variables was then calculated. Thus, the TAP variable had a maximum value of 3 (maximum level of activity) and a minimum value of 0 (complete state of rest).

[0024] After standardizing the variables and calculat-

ing the TAP variable, the match rates were calculated for each of the variables studied (including TAP) and the daily sleep diary (with values of 0 whenever the individual claimed to be awake, and values of 1 when he/she reported being asleep), in order to ascertain whether our TAP variable improved the ability to predict each of the variables separately. These results are shown in Figure 1.

5

10

Claims

1. Device that consists of at least one body position and activity sensor, at least one peripheral temperature sensor and at least one light sensor, configured to provide information about the circadian system status and the sleep-wake status of an individual based on the data obtained from said sensors. 15
2. Device as described in claim 1, **characterized by** the fact that this device is placed on the person's wrist. 20
3. Device as described in claim 1, **characterized by** the fact that it also includes at least one blood pressure sensor and is configured to provide information on the status of a person's blood pressure. 25
4. Device as described in claim 3, **characterized by** the fact that these peripheral temperature and light sensors are placed on the person's wrist and said body position and activity sensors and blood pressure sensor are placed on the person's arm. 30
5. Procedure to determine the circadian system status and the sleep-wake status of a person, consisting of: 35
 - a) Obtaining the peripheral temperature, motor activity per minute and body position values for an individual. 40
 - b) Drawing conclusions about the circadian system status and the sleep-wake status of an individual based on the changes in the values resulting from step a). 45
6. Procedure as described in claim 5 to obtain information about blood pressure and hypertension, **characterized by** the fact that in step a) blood pressure values are also recorded for said individual, and that in step b) the blood pressure values are compared to the rest of the values to determine any changes in blood pressure upon lying down or standing up. 50

55

Fig 1A

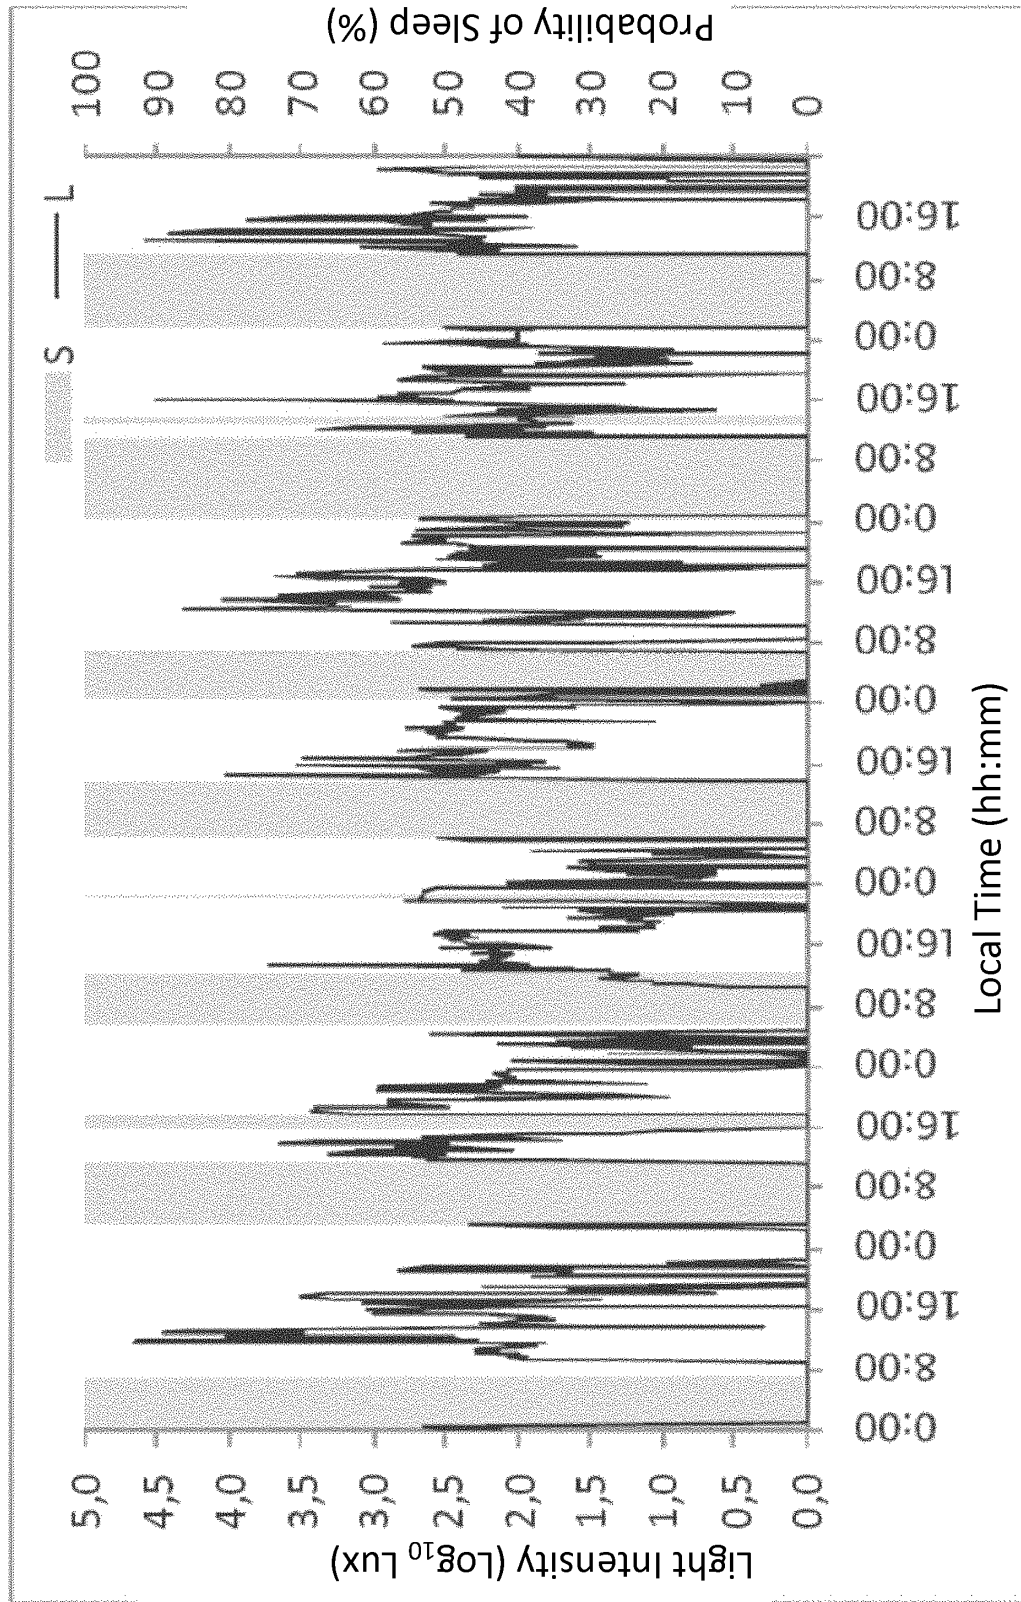


Fig 1A

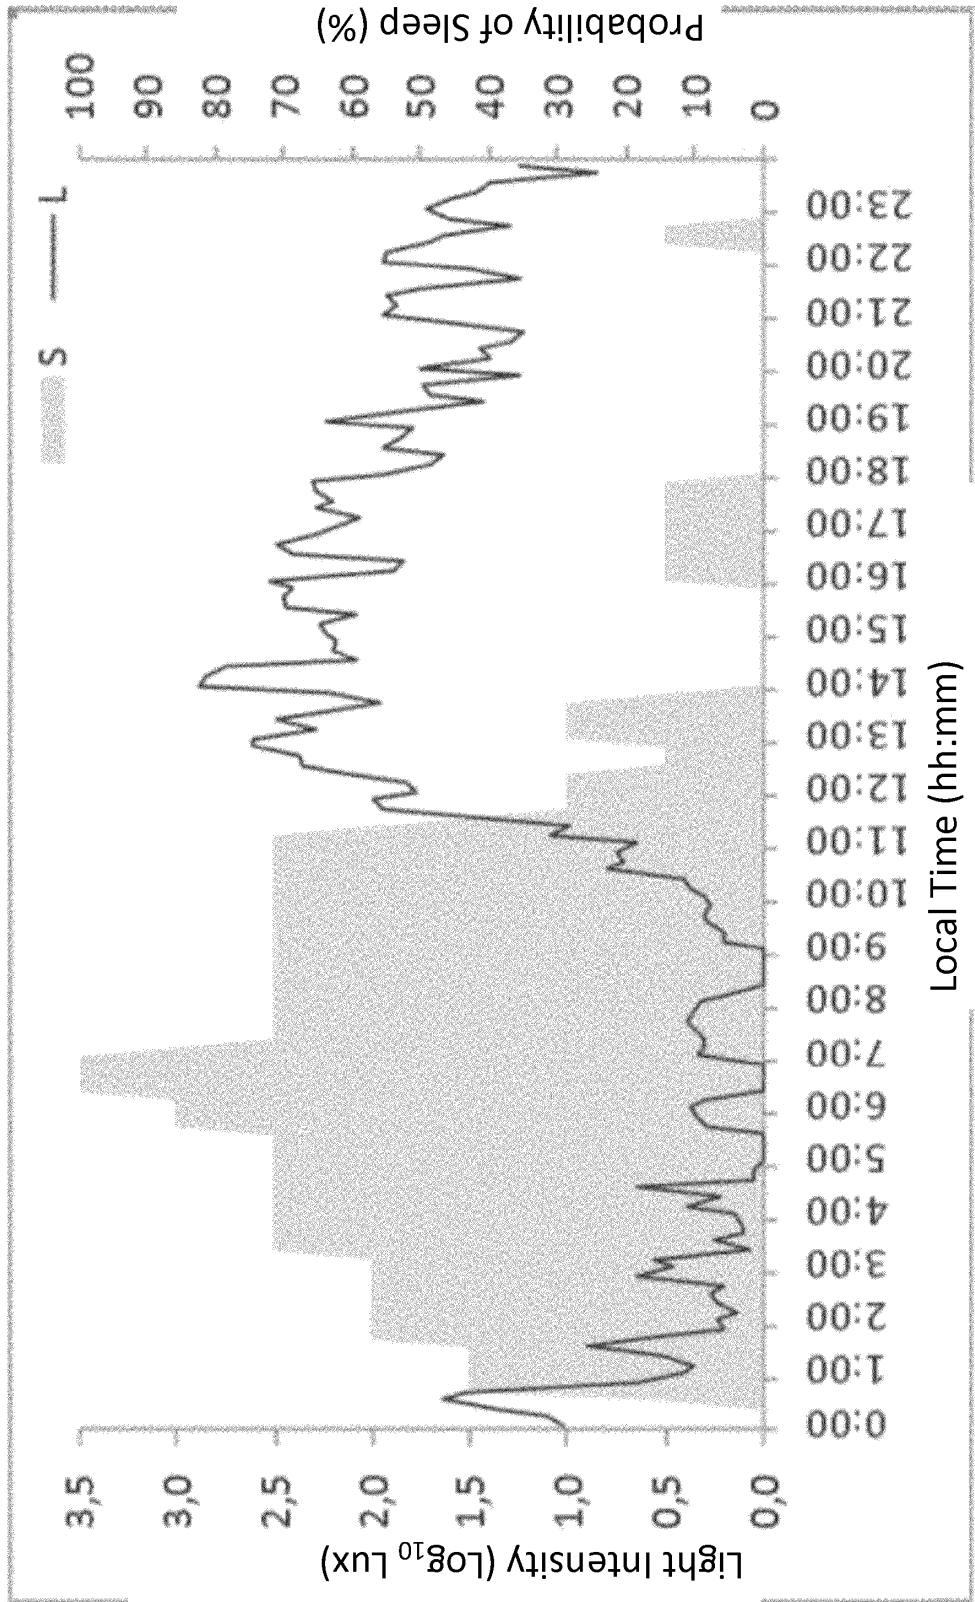


Fig 1B

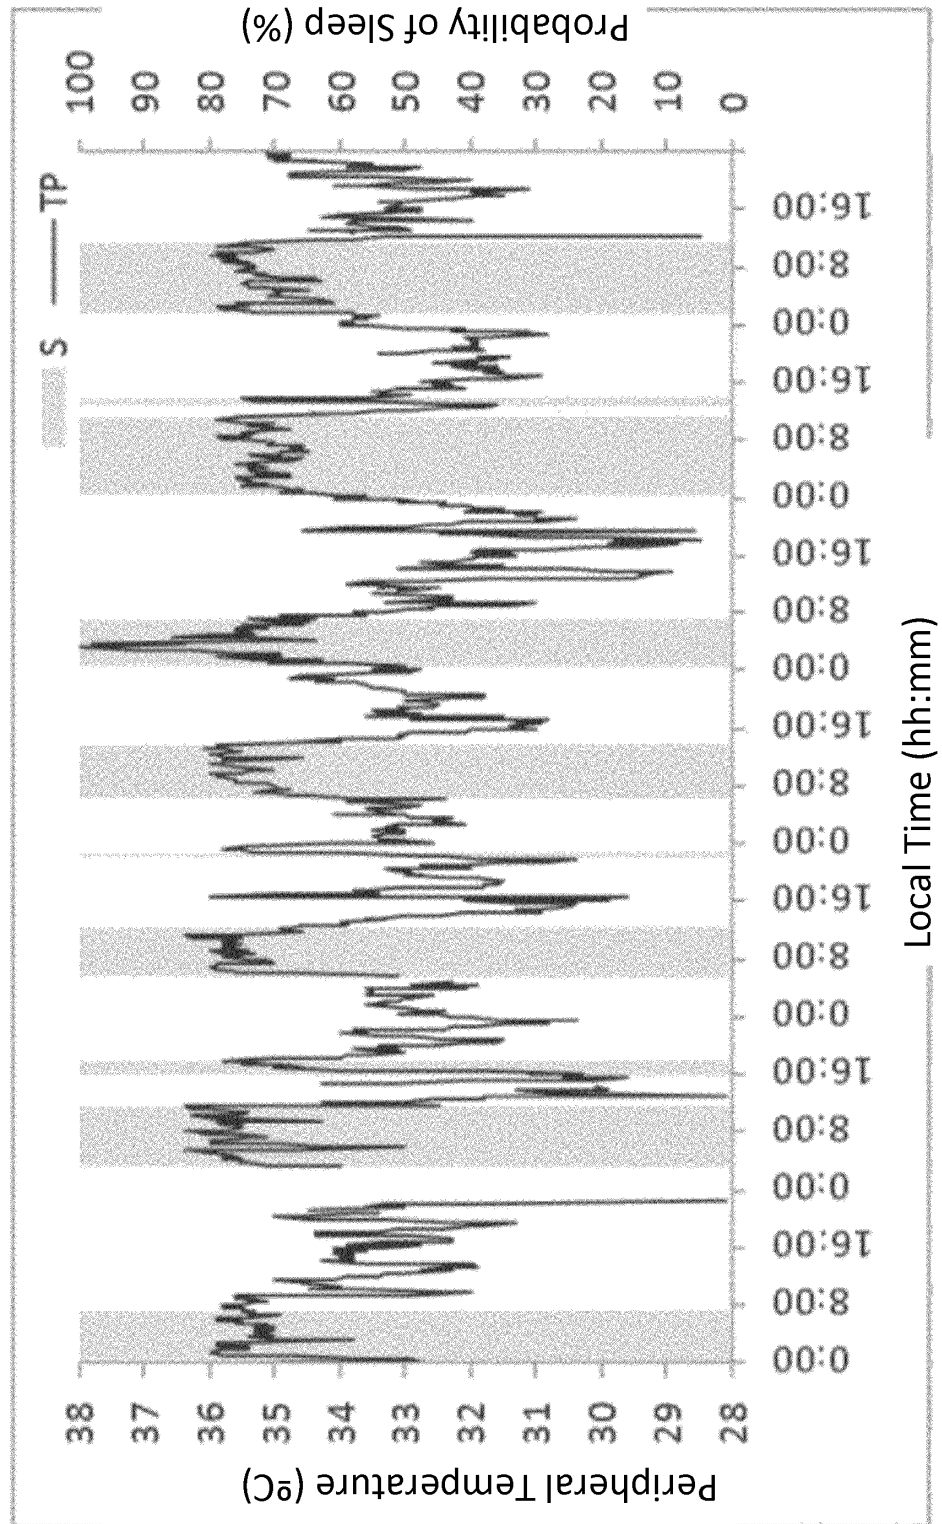


Fig 1B

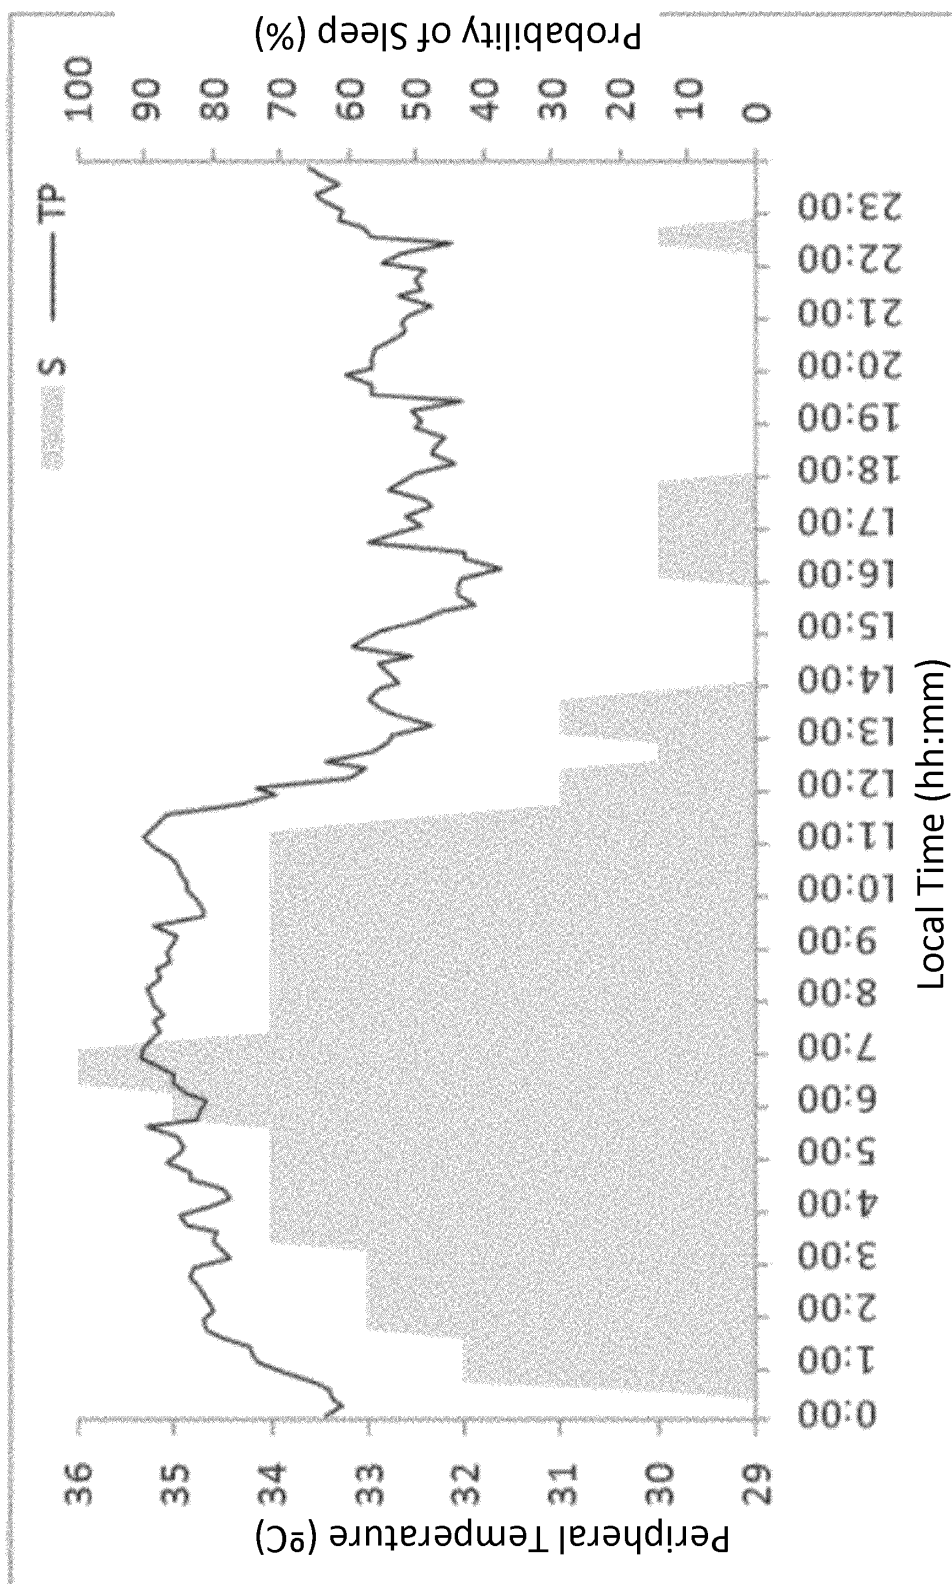


Fig 1C

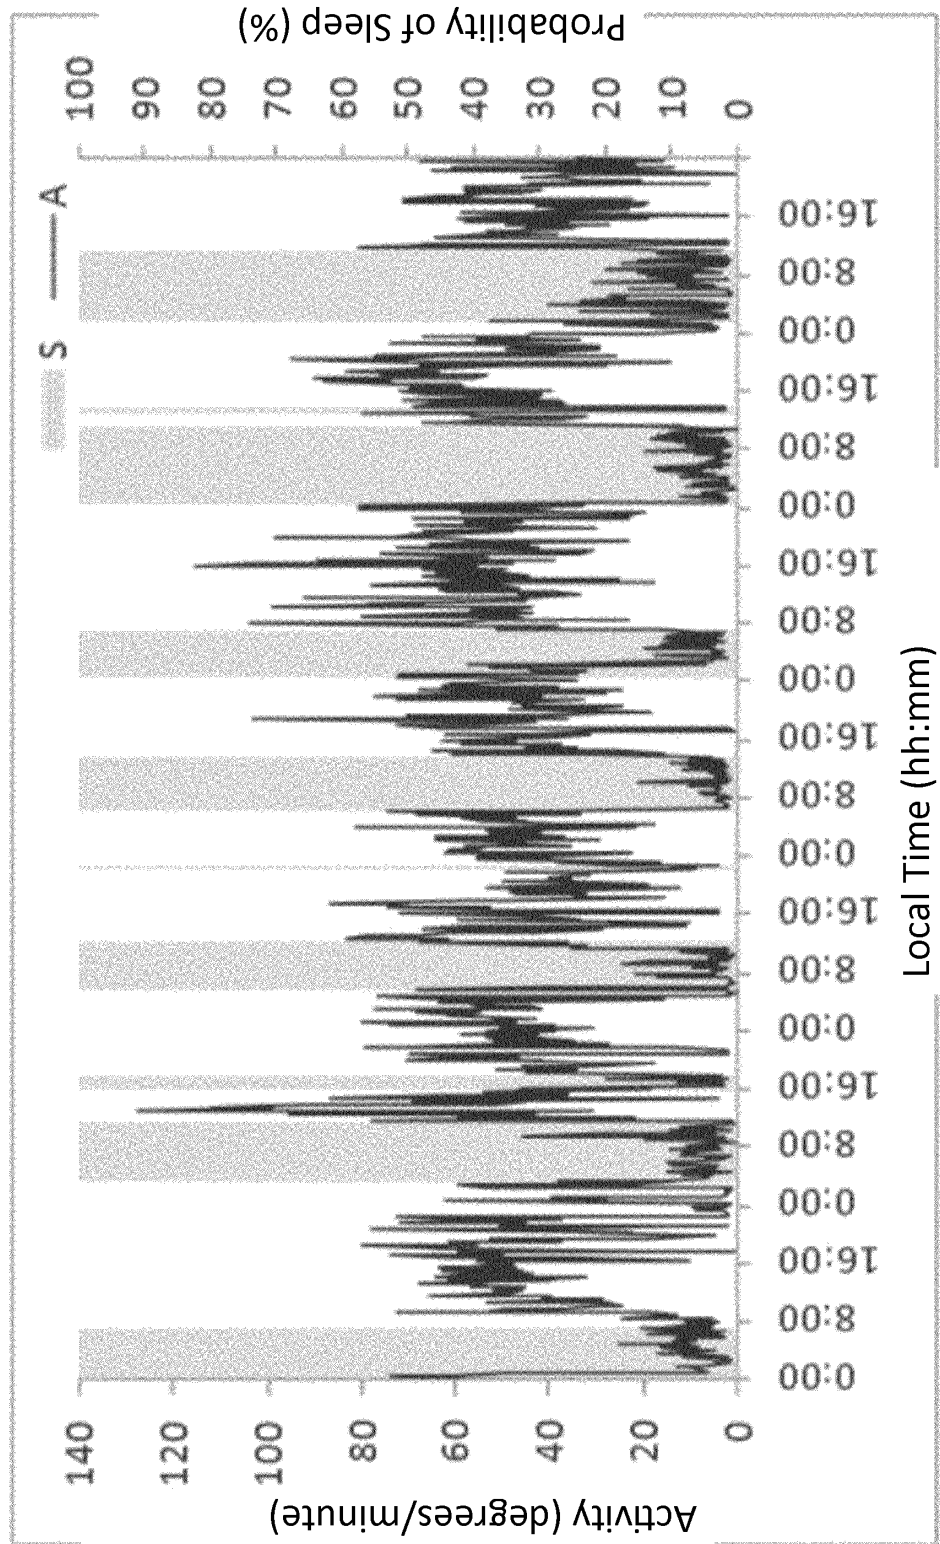


Fig 1C

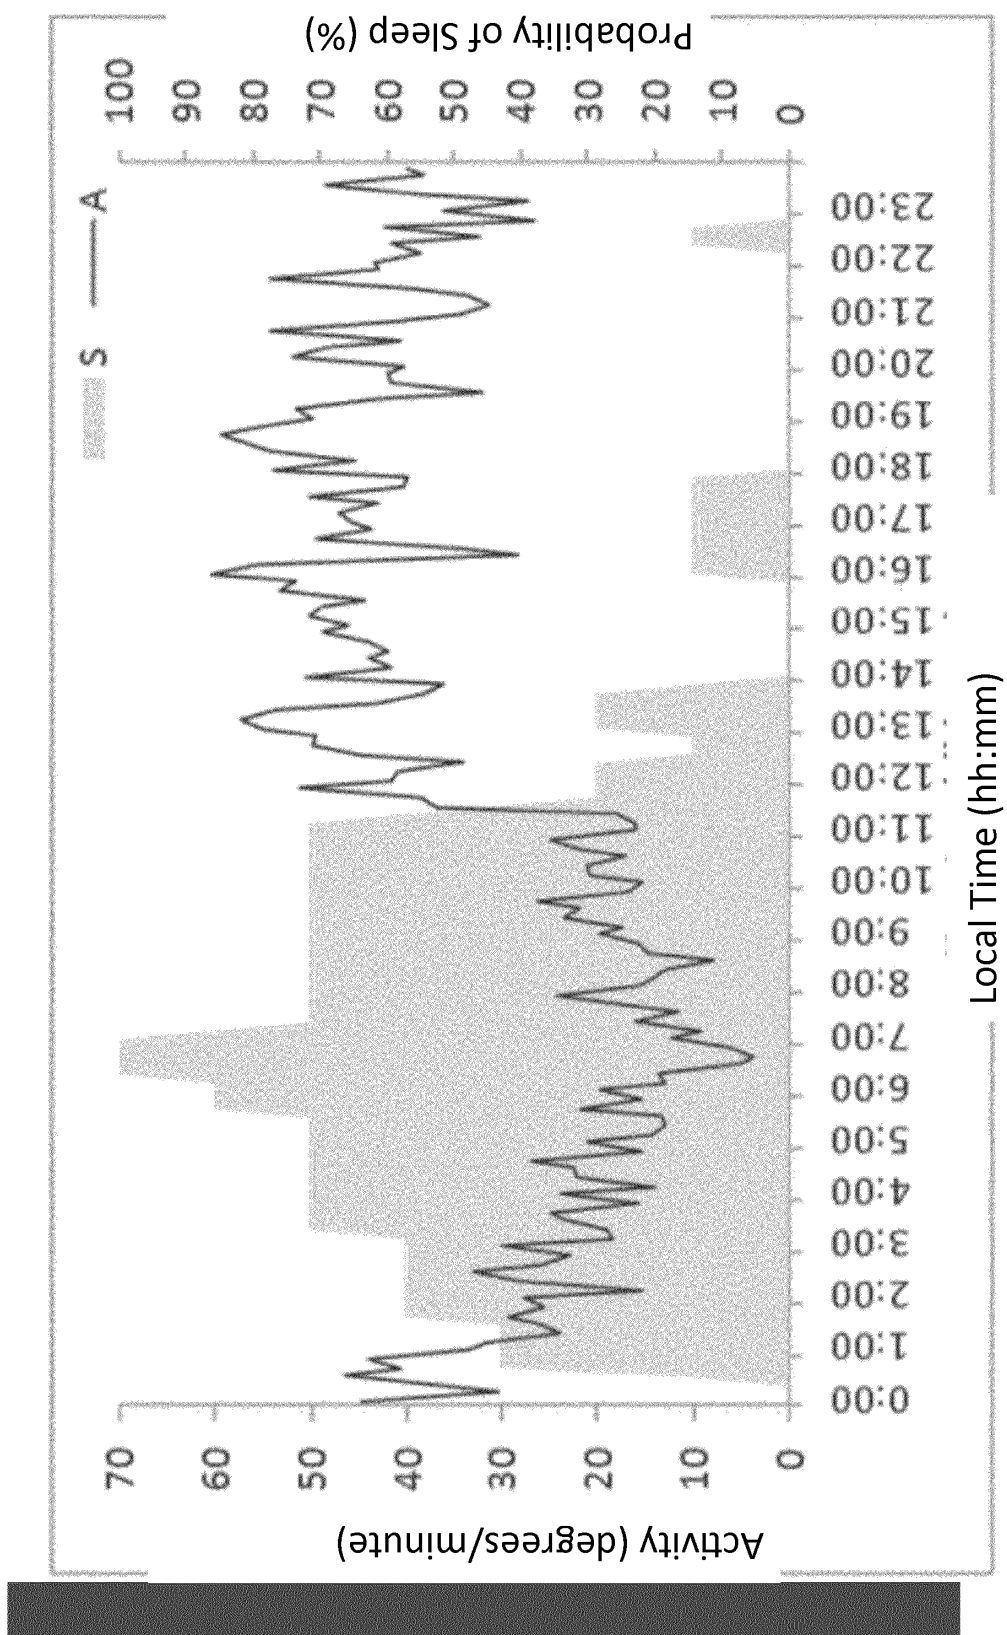


Fig 1D

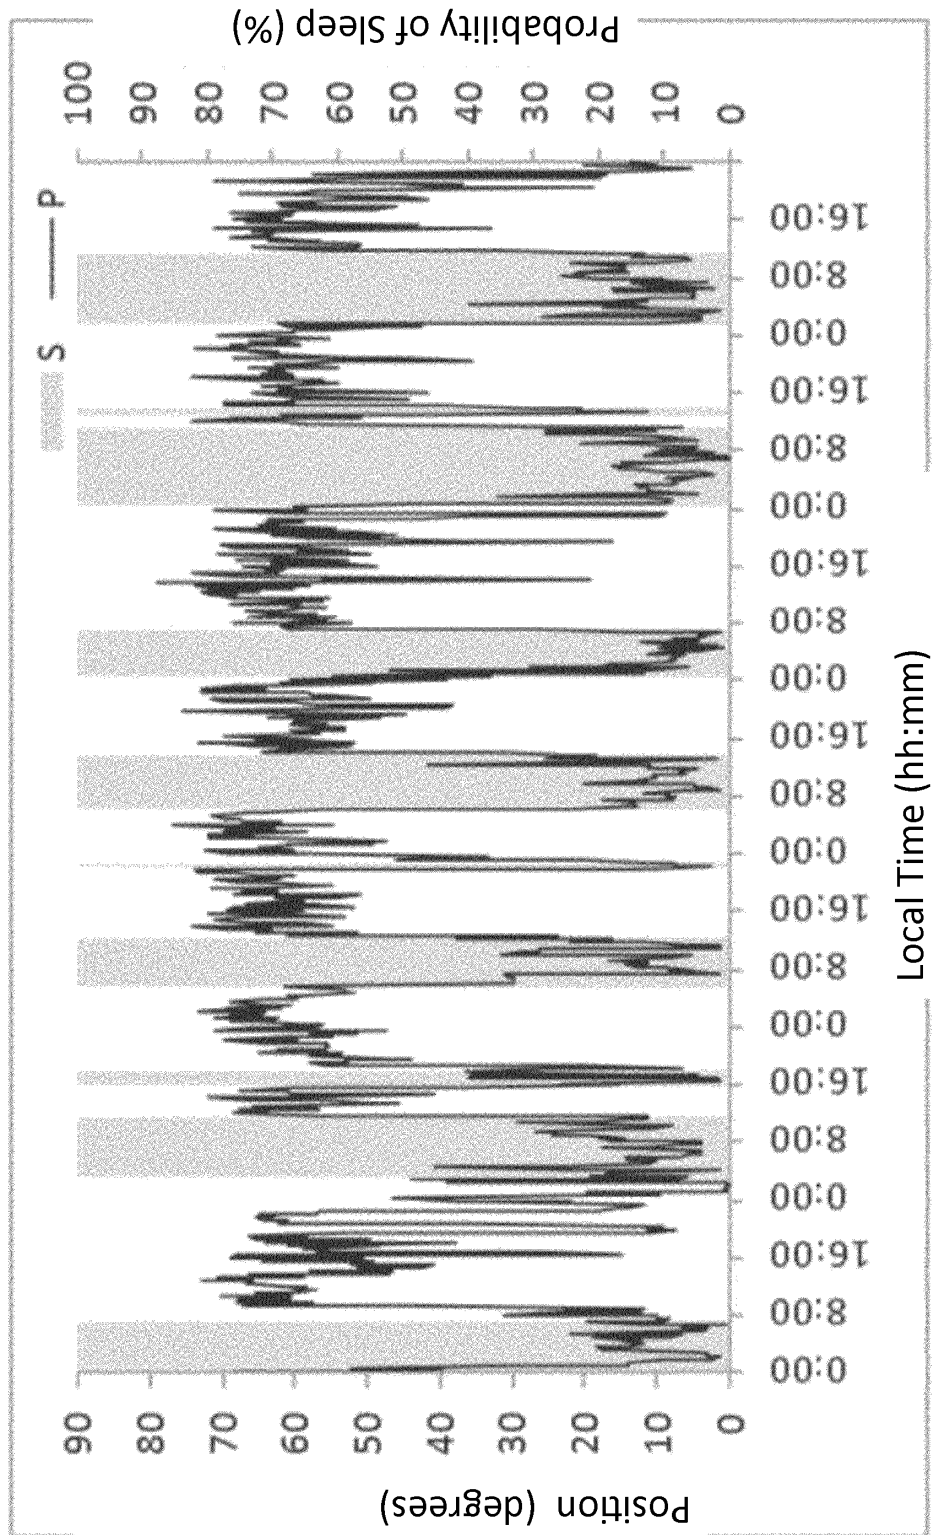


Fig 1D

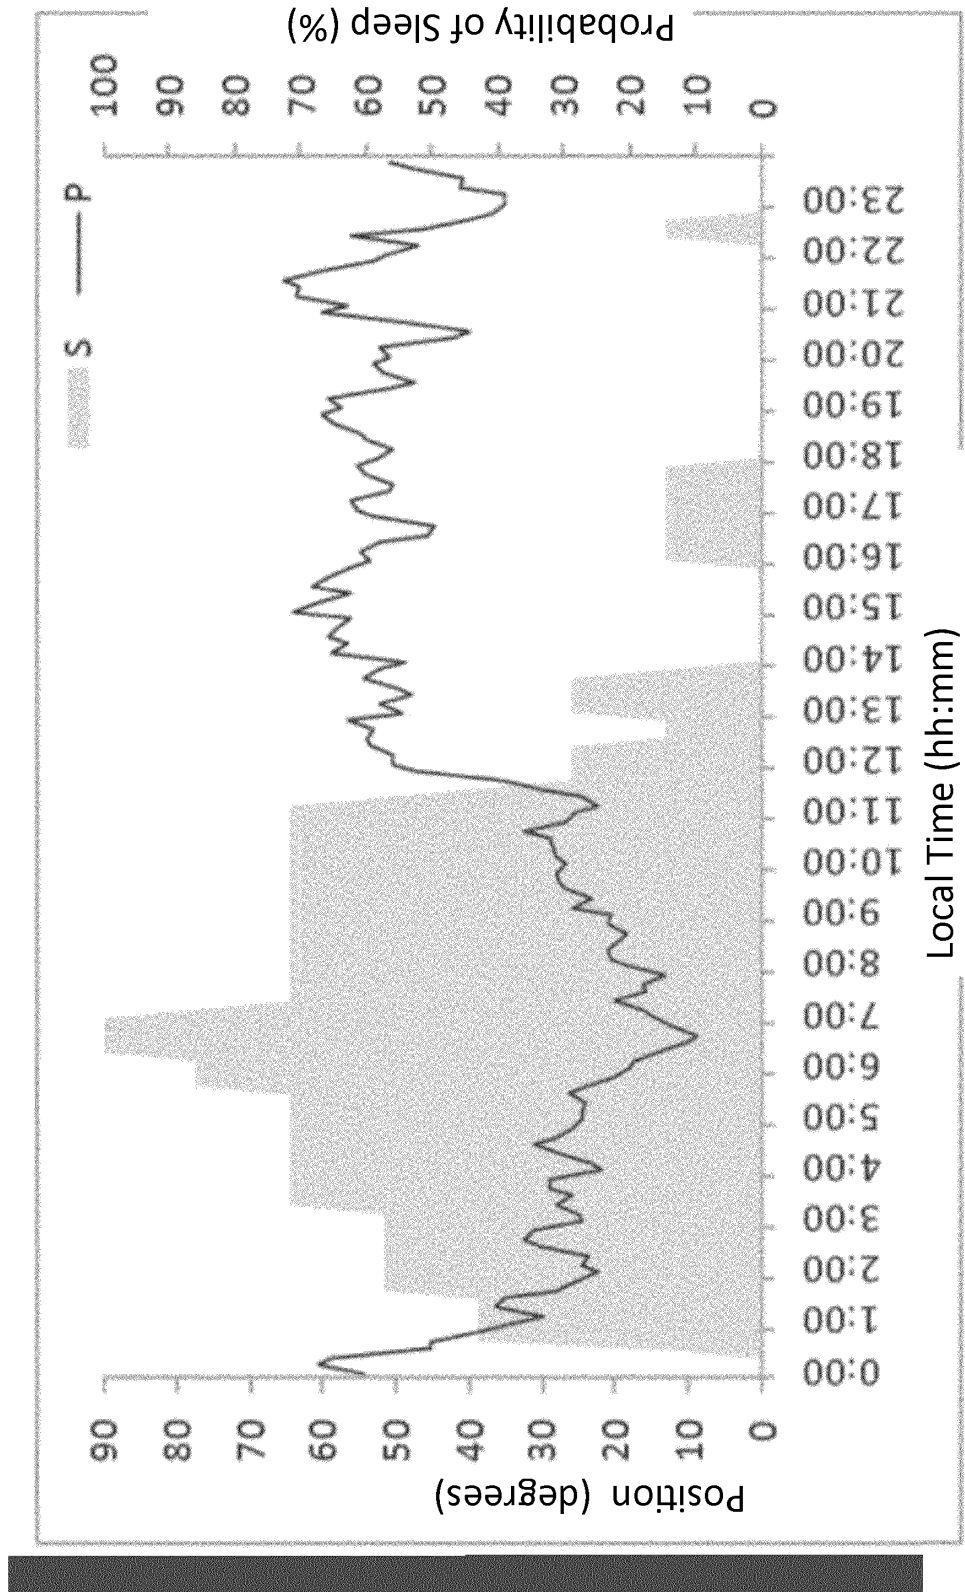


Fig 1E

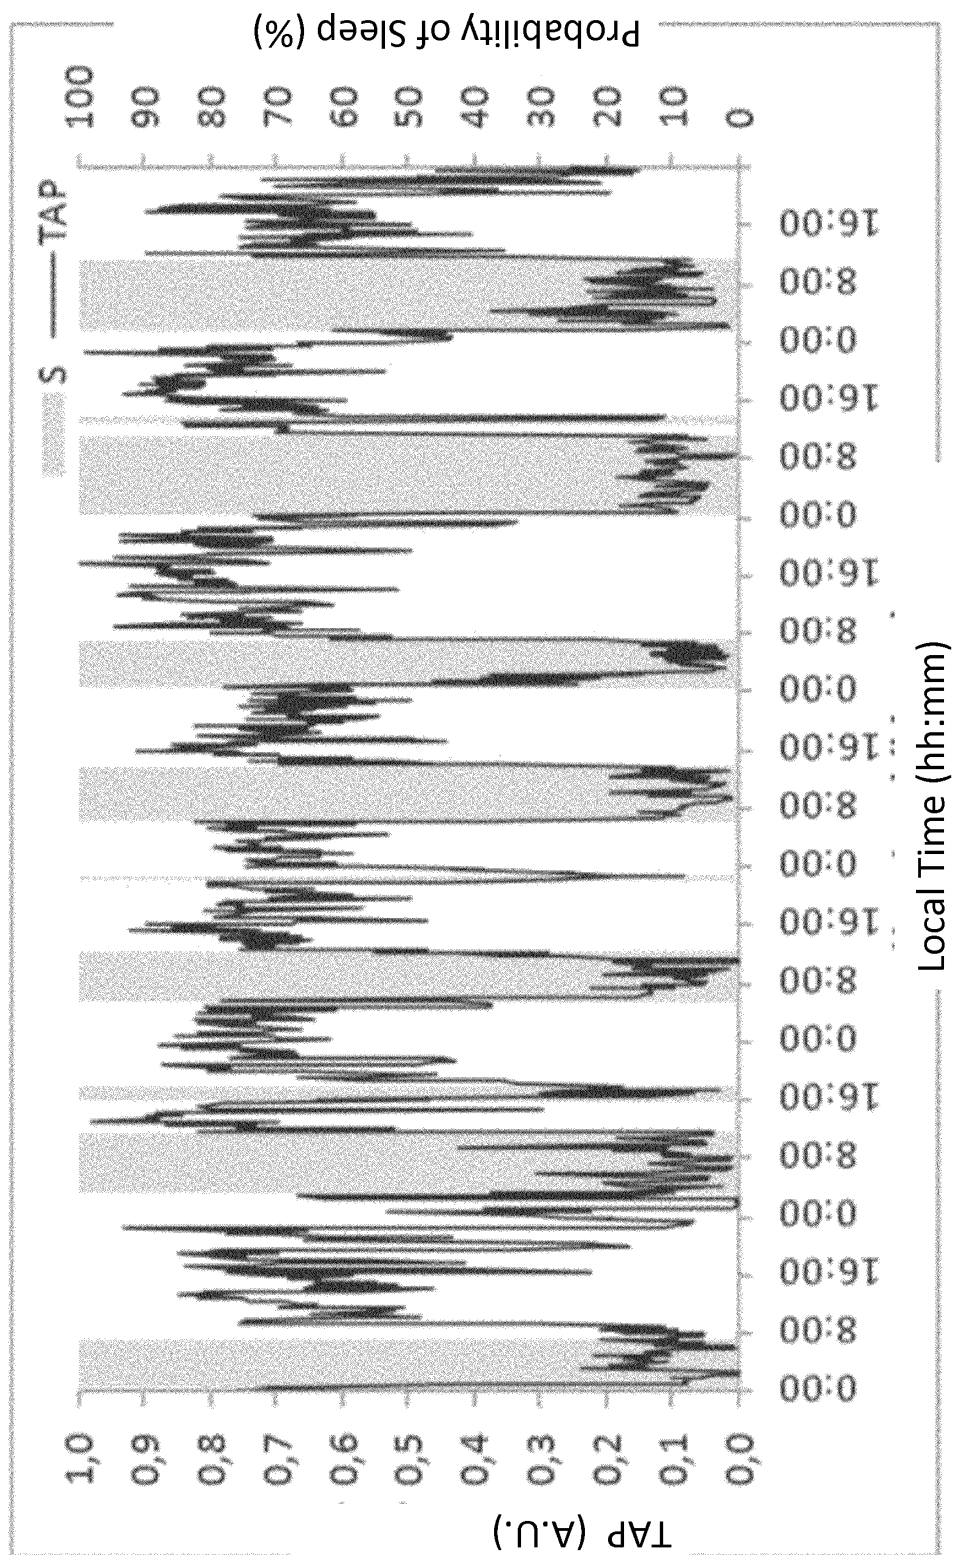
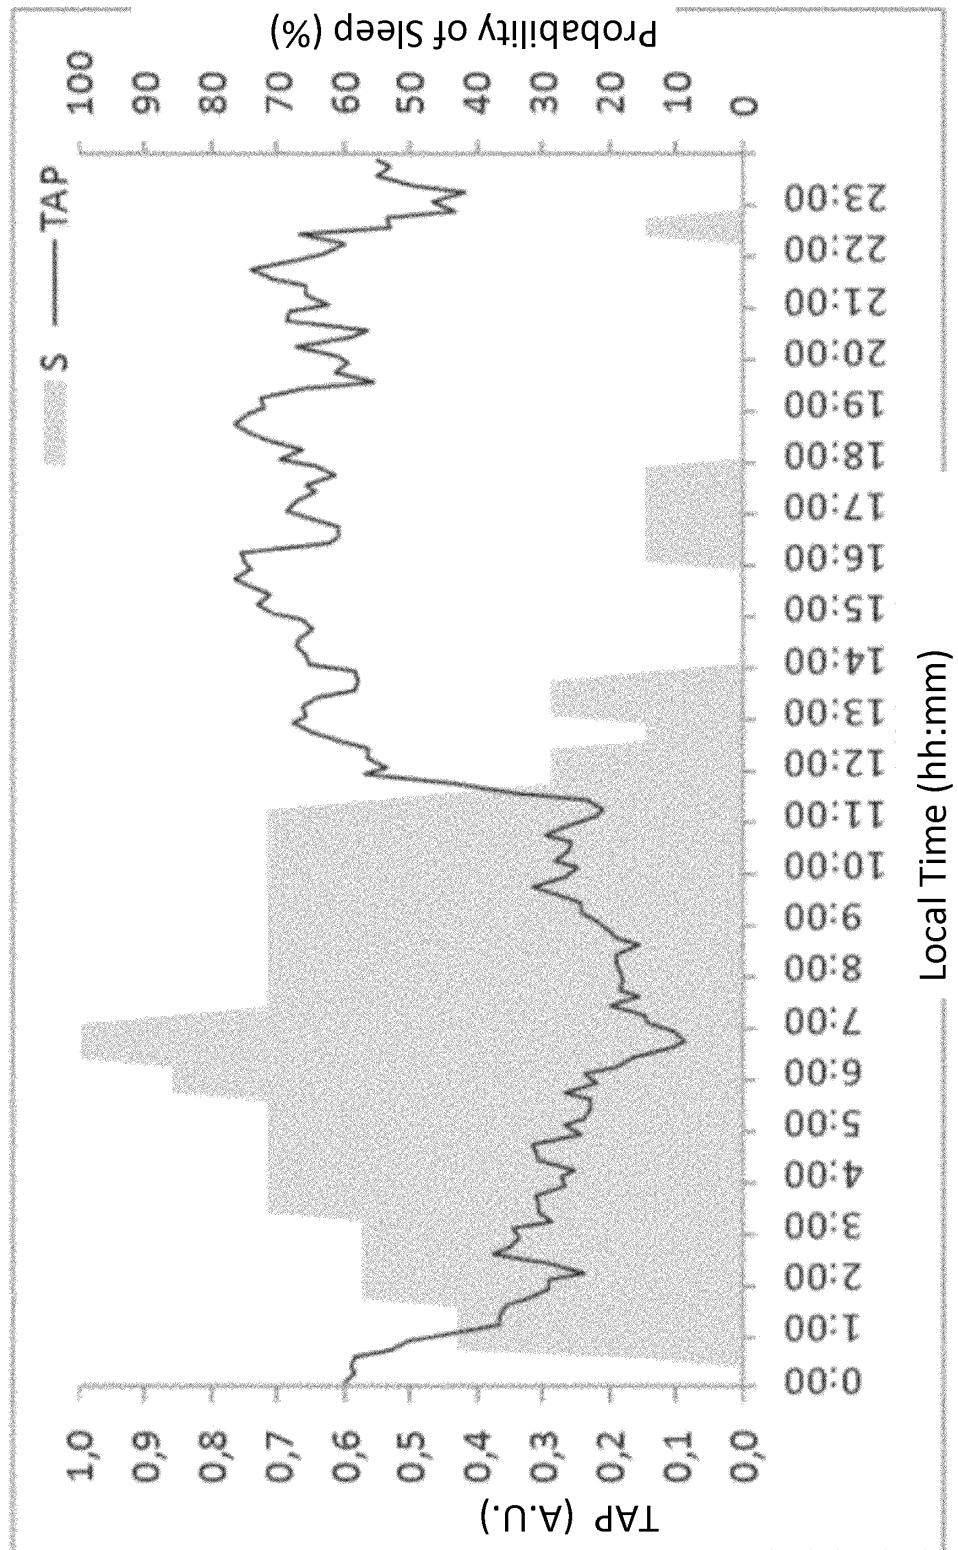


Fig 1E



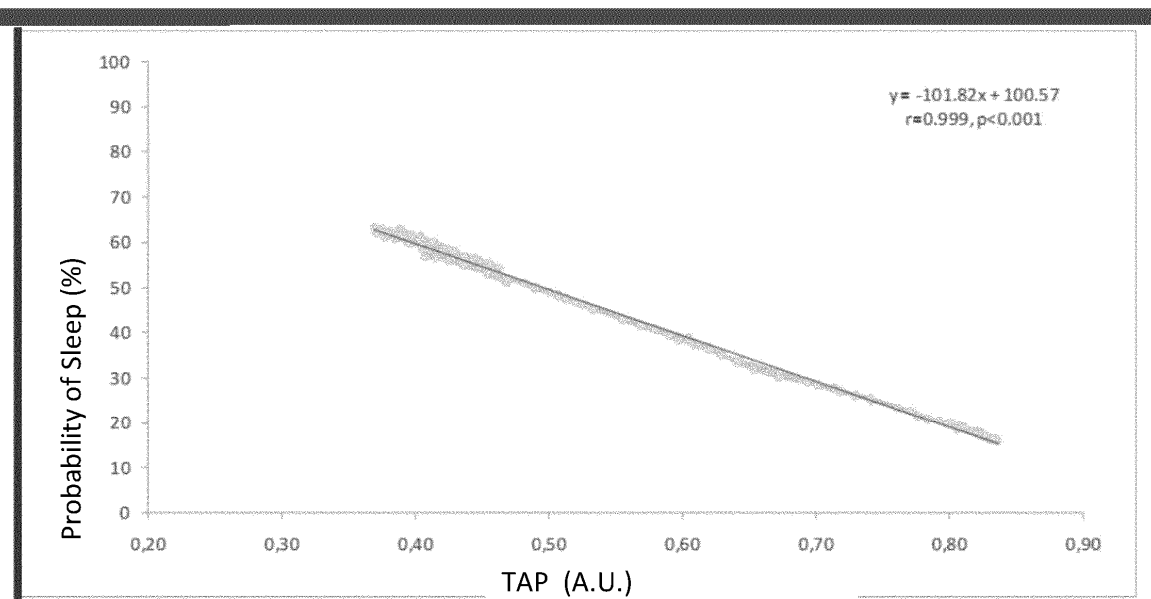


Fig 2

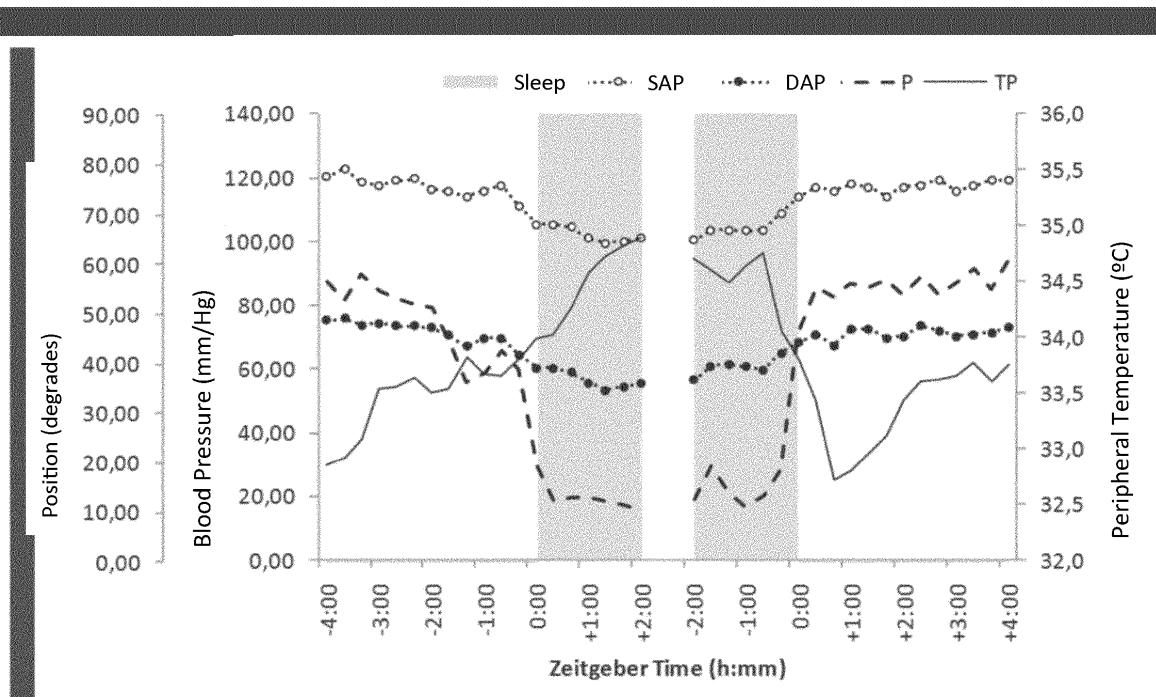


Fig 3

INTERNATIONAL SEARCH REPORT

International application No.

PCT/ES2011/070877

A. CLASSIFICATION OF SUBJECT MATTER

A61B5/00 (2006.01)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPODOC, INVENES, WPI, NPL, INSPEC, BIOSIS, MEDLINE

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2005143617 A1 (Auphan) 30.06.2005Párrafos 31 – 36, 48, 49	1 - 6
X	US 2008171918 A1 (Teller et al.) 17.07.2008Párrafos 30 – 34, 71	1 - 6
X	US 2007150026 A1 (Bourget et al.) 28.06.2007Párrafos 7, 46, 59	1 - 6
X	US 2006224047 A1 (Suzuki et al.) 05.10.2006Párrafos 28 – 31, 40, 41, 61, 64	1 - 6
X	US 2005042589 A1 (Hatleestad et al.) 24.02.2005Párrafos 56 – 60, 74	1 - 6

☐ Further documents are listed in the continuation of Box C.☒ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance.

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure use, exhibition, or other means.

"P" document published prior to the international filing date but later than the priority date claimed

"T"

later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X"

document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y"

document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other documents, such combination being obvious to a person skilled in the art

"&"

document member of the same patent family

Date of the actual completion of the international search

07/05/2012

Date of mailing of the international search report

(08/05/2012)

Name and mailing address of the ISA/

OFICINA ESPAÑOLA DE PATENTES Y MARCAS
Paseo de la Castellana, 75 - 28071 Madrid (España)
Facsimile No.: 91 349 53 04

Authorized officer

A. Cárdenas Villar

Telephone No. 91 3495393

Form PCT/ISA/210 (second sheet) (July 2009)

EP 2 656 782 A1

INTERNATIONAL SEARCH REPORT

Information on patent family members		International application No. PCT/ES2011/070877	
Patent document cited in the search report	Publication date	Patent family member(s)	Publication date
US2005143617 A	30.06.2005	US7524279 B WO2005066868 A EP1704503 A EP20040806467 US2009264715 A US7967739 B	28.04.2009 21.07.2005 27.09.2006 30.12.2004 22.10.2009 28.06.2011
----- US2008171918 A	----- 17.07.2008	WO0196986 A CA2413220 AC AU6708301 A CA2413148 AC WO0200111 A AU7009201 A US2002019586 A US7261690 B CA2454655 A WO03015005 A AU2002330965 A EP1292218 AB EP20010948636 EP1292217 AB EP20010944698 BR0111918 AB US6605038 B JP2004500949 A US2004034289 A JP2004512061 A EP1414340 A EP20020768402 MXPA04001055 A US2004152957 A US7285090 B MXPA02012482 A MXPA02012643 A BR0211760 A JP2004538066 A JP4283672B2 B WO2005016124 A CA2538758 A WO2005029242 A US2005113650 A BR0111995 AB AT310444 T US2006031102 A US8073707 B EP1639939 A EP20050077625 AT324066 T ES2253393 T EP1662989 A	20.12.2001 20.12.2001 24.12.2001 03.01.2002 03.01.2002 08.01.2002 14.02.2002 28.08.2007 20.02.2003 20.02.2003 24.02.2003 19.03.2003 22.06.2001 19.03.2003 13.06.2001 13.05.2003 12.08.2003 15.01.2004 19.02.2004 22.04.2004 06.05.2004 01.08.2002 20.05.2004 05.08.2004 23.10.2007 10.09.2004 10.09.2004 13.10.2004 24.12.2004 24.06.2009 24.02.2005 31.03.2005 31.03.2005 26.05.2005 28.06.2005 15.12.2005 09.02.2006 06.12.2011 29.03.2006 13.06.2001 15.05.2006 01.06.2006 07.06.2006

Form PCT/ISA/210 (patent family annex) (July 2009)

INTERNATIONAL SEARCH REPORT

International application No.

PCT/ES2011/070877

Information on patent family members

Patent document cited in the search report	Publication date	Patent family member(s)	Publication date
		EP20040784031	13.09.2004
		US2006122474 A	08.06.2006
		MXPA06002836 A	14.06.2006
		DE60115234 T	10.08.2006
		DE60119100 T	31.08.2006
		EP1702560 A	20.09.2006
		EP20060075949	22.06.2001
		PT1292218 E	29.09.2006
		US2006224051 A	05.10.2006
		ES2260245 T	01.11.2006
		BRPI0414359 A	14.11.2006
		IL153516 A	24.07.2007
		US2007173705 A	26.07.2007
		US2008171919 A	17.07.2008
		US2008177158 A	24.07.2008
		US2008183052 A	31.07.2008
		US2008183051 A	31.07.2008
		US2008275309 A	06.11.2008
		US7959567 B	14.06.2011
		US2009118590 A	07.05.2009
		IL153478 A	03.08.2009
		US7689437 B	30.03.2010
		EP2363061 A	07.09.2011
		EP20110159897	13.09.2004
		US2012059230 A	08.03.2012
-----	-----	-----	-----
US2007150026 A	28.06.2007	WO2007064936 A	07.06.2007
		WO2007064924 A	07.06.2007
		US2007129774 A	07.06.2007
		US7853322 B	14.12.2010
		US7957797 B	07.06.2011
		US2007150029 A	28.06.2007
		US7957809 B	07.06.2011
		EP1960046 A	27.08.2008
		EP20060844725	01.12.2006
		EP1960047 A	27.08.2008
		EP20060844740	01.12.2006
		US2011082522 A	07.04.2011
		US2011238130 A	29.09.2011
		US2011238136 A	29.09.2011
-----	-----	-----	-----
US2006224047 A	05.10.2006	JP2006271897 A	12.10.2006
		JP4421507B2 B	24.02.2010
-----	-----	-----	-----
US2005042589 A	24.02.2005	US8002553 B	23.08.2011
		WO2005018737 A	03.03.2005
		WO2005028029 A	31.03.2005
		US2005115561 A	02.06.2005
		US7787946 B	31.08.2010

Form PCT/ISA/210 (patent family annex) (July 2009)

INTERNATIONAL SEARCH REPORT

International application No.

PCT/ES2011/070877

Information on patent family members

Patent document cited in the search report	Publication date	Patent family member(s)	Publication date
		EP1656181 AB	17.05.2006
		EP20040781543	18.08.2004
		EP1670547 AB	21.06.2006
		EP20040784602	17.09.2004
		JP2007502670 A	15.02.2007
		JP4750032B2 B	17.08.2011
		AT397475 T	15.06.2008
		EP1938862 AB	02.07.2008
		EP20080006191	18.08.2004
		AT413902 T	15.11.2008
		EP2008581 AB	31.12.2008
		EP20080075738	17.09.2004
		US2011061647 A	17.03.2011
		AT529156 T	15.11.2011
		US2011306850 A	15.12.2011
-----	-----	-----	-----

Form PCT/ISA/210 (patent family annex) (July 2009)

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Non-patent literature cited in the description

- **SARABIA, J.A. et al.** Circadian rhythm of wrist temperature in normal-living subjects. A candidate of new index of the circadian system. *PhysiolBehav.*, 2008, vol. 95 (4), 570-80 [0006]

专利名称(译)	包括物理活动和位置传感器，外围温度传感器和光传感器的装置，用于提供与昼夜节律系统状态有关的信息		
公开(公告)号	EP2656782A1	公开(公告)日	2013-10-30
申请号	EP2011851174	申请日	2011-12-19
申请(专利权)人(译)	大学德MURCIA		
当前申请(专利权)人(译)	大学德MURCIA		
[标]发明人	SARABIA CARRAZO JUAN ANTONIO MARTINEZ NICOLAS ANTONIO MADRID PEREZ JUAN ANTONIO ROL DE LAMA MARIA ANGELES ORTIZ TUDELA ELISABET		
发明人	SARABIA CARRAZO, JUAN ANTONIO MARTINEZ NICOLAS, ANTONIO MADRID PEREZ, JUAN ANTONIO ROL DE LAMA, MARÍA ANGELES ORTIZ TUDELA, ELISABET		
IPC分类号	A61B5/00 A61B5/01 A61B5/0205 A61B5/021 A61B5/11 G06F19/00		
CPC分类号	A61B5/002 A61B5/01 A61B5/021 A61B5/4809 A61B5/7264 A61B5/7275 A61B2560/0242 G06F19/00 G06F19/3481 G16H40/63 G16H50/30 A61B5/00 A61B5/02055 A61B5/1116 A61B5/1118 A61B5/4812 A61B5/681		
代理机构(译)	卡瓦哈尔·乌尔基霍, ISABEL		
优先权	2010031894 2010-12-21 ES		
其他公开文献	EP2656782A4		
外部链接	Espacenet		

摘要(译)

本发明是一种装置，包括至少一个身体位置和活动传感器，至少一个外围温度传感器和至少一个光传感器，被配置为基于所述个体的昼夜系统状态和睡眠 - 唤醒状态提供信息。从所述传感器获得的数据。它可以放在受试者的手腕上，也可以放在受试者的手臂上。该装置还可包括血压传感器。该装置可用于人类昼夜节律系统的一般研究，更具体地，用于睡眠 - 觉醒和血压节律的研究。

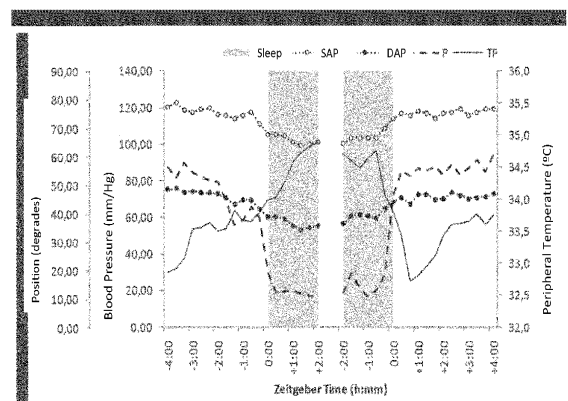


Fig 3