



(11) **EP 1 722 680 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
10.04.2013 Bulletin 2013/15

(51) Int Cl.:
A61B 5/04 (2006.01)

(21) Application number: **05713679.8**

(86) International application number:
PCT/US2005/004960

(22) Date of filing: **16.02.2005**

(87) International publication number:
WO 2005/079429 (01.09.2005 Gazette 2005/35)

(54) **DISTRIBUTED CARDIAC ACTIVITY MONITORING WITH SELECTIVE FILTERING**

VERTEILTE HERZAKTIVITÄTS-ÜBERWACHUNG MIT SELEKTIVER FILTERUNG

SURVEILLANCE REPARTIE DE L'ACTIVITE CARDIAQUE AVEC FILTRAGE SELECTIF

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU MC NL PL PT RO SE SI SK TR**

(56) References cited:
**AU-B2- 506 062 US-A- 3 474 778
US-A- 3 593 705 US-A- 3 672 353
US-A- 4 240 442 US-A- 4 667 682
US-A- 4 887 609 US-A- 6 167 258
US-A1- 2003 187 479 US-A1- 2003 204 215**

(30) Priority: **17.02.2004 US 781045**

(43) Date of publication of application:
22.11.2006 Bulletin 2006/47

(60) Divisional application:
11181851.4

(73) Proprietor: **CardioNet, Inc.
San Diego, CA 92101 (US)**

(72) Inventors:
• **KORZINOV, Lev
San Diego, CA 92122 (US)**
• **CHURCHVILLE, Dave
San Diego, CA 92129 (US)**
• **CYBULSKI, Zach
San Diego, CA 92107 (US)**

(74) Representative: **Curran, Clair et al
Ropes & Gray International LLP
5 New Street Square
London EC4A 3BF (GB)**

- **PAUL J ZSOMBOR-MURRAY ET AL: "A Miniature Recording Cardiotachometer", IEEE TRANSACTIONS ON INDUSTRIAL ELECTRONICS AND CONTROLINSTRUMENTATION, IEEE, NEW YORK, N. Y., N/A, vol. IECI-11, no. 2, 1 May 1981 (1981-05-01), pages 90-97, XP011178852, ISSN: 0018-9421**
- **SZILDGYI S M ET AL: "Comparison Between Neural-Network-Based Adaptive Filtering and Wavelet Transform for Ecg Characteristic Points Detection", ENGINEERING IN MEDICINE AND BIOLOGY SOCIETY, 1997. PROCEEDINGS OF THE 19TH ANNUAL INTERNATIONAL CONFERENCE OF THE IEEE CHICAGO, IL, USA 30 OCT.-2 NOV. 1997, PISCATAWAY, NJ, USA, IEEE, US, 30 October 1997 (1997-10-30), pages 272-274, XP031461909, ISBN: 978-0-7803-4262-0**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 722 680 B1

Description

BACKGROUND

[0001] The present application describes systems and techniques relating to monitoring cardiac activity, for example, processing cardiac electrical activity to determine heart rate.

[0002] The electrical activity of the heart can be monitored to track various aspects of the functioning of the heart. Given the volume conductivity of the body, electrodes on the body surface or beneath the skin can display potential differences related to this activity. Anomalous electrical activity can be indicative of disease states or other physiological conditions ranging from benign to fatal.

[0003] Cardiac monitoring devices can sense the cardiac electrical activity of a living being and identify heart beats. Frequently, identification of heart beats is performed by identifying the R waves in the QRS complex, as can be seen in an electrocardiogram (ECG). The R wave is the first positive deflection in the QRS complex, representing ventricular depolarization. The typically large amplitude of this positive deflection in the QRS complex is useful in identifying a heart beat.

[0004] US 3,593,705 describes a monitoring apparatus and method for determining the presence of cardiac arrhythmias by means of pattern recognition techniques. In one embodiment, the arrangement rejects a QRS complex based on a measure of the T-wave. US 4,240,442 describes an R wave detector for use in monitoring and/or analyzing electrical heart waveforms. A variable threshold is provided which enables increased sensitivity to small amplitude R waves without requiring the threshold to remain so low as to additionally detect the subsequent T waves. US 2003/204215 describes a method and apparatus for automatically identifying various types of cardiac and non-cardiac over sensing. In one arrangement, if T wave over sensing is detected, the ventricular sensitivity can be reprogrammed. US 4,887,609 describes an electro cardiograph filtering apparatus and method in which an ECG signal is filtered to remove unwanted signals, such as contamination signals produced by the use of a nuclear magnetic resonance imaging system or muscle artefact signals. US 6,167,258 describes a programmable wireless data acquisition system and describes various kinds of filters, including a prefilter to reject inputs that are outside of a frequency band of interest, an AC coupling high pass filter to reject the DC offset or steady state value of an external input, an anti-alias low pass filter to guard against false signals caused by aliasing between the external input content and the sampling rate of downstream sampling functions, and a digital filter to reject certain portions of the digital data stream to provide an effective decrease in resolution.

SUMMARY

[0005] According to the invention, there is provided a machine-implemented method according to claim 1. Further, according to the invention, there is provided a method according to claim 11. Further, according to the invention there is provided an apparatus according to claim 15.

[0006] The details of one or more embodiments are set forth in the accompanying drawings and the description below. Other features and advantages will become apparent from the description, the drawings, and the claims.

DRAWING DESCRIPTIONS

[0007] FIG. 1 illustrates a distributed cardiac activity monitoring system in which a cardiac signal is monitored for medical purposes.

[0008] FIG. 2 illustrates an example cardiac monitoring apparatus used with a living being.

[0009] FIG. 3 illustrates an example ECG of a normal patient.

[0010] FIG. 4 illustrates an example ECG of a patient with abnormal T waves.

[0011] FIG. 5 illustrates a process of selectively activating a T wave filter.

[0012] FIG. 6 illustrates a frequency response of an example T wave filter.

[0013] FIG. 7 illustrates an impulse response of an example T wave filter.

[0014] FIG. 8 illustrates an example distributed process for selectively activating a T wave filter.

DETAILED DESCRIPTION

[0015] FIG. 1 illustrates a distributed cardiac activity monitoring system 100 in which a cardiac signal is monitored for medical purposes. A living being 110 (e.g., a human patient, including potentially a healthy patient for whom cardiac monitoring is nonetheless deemed appropriate) has a cardiac monitoring apparatus 120 configured to obtain cardiac signals from the patient's heart. The cardiac monitoring apparatus 120 can be composed of one or more devices, such as a sensing device 122 and a processing device 124. The cardiac monitoring apparatus 120 can communicate with a monitoring station 140 (e.g., a computer in a monitoring center) via a communications channel 130. The cardiac monitoring apparatus 120 can include one or more sensing, calibration, signal processing, control, data storage, and transmission elements suitable for generating and processing the cardiac signal, as well as for relaying all or a portion of the cardiac signal over the communications channel 130. The communications channel 130 can be part of a communications network and can include any suitable medium for data transmission, including wired and wireless media suitable for carrying optical and/or electrical sig-

nals.

[0016] The cardiac monitoring apparatus 120 can communicate sensed cardiac signals (e.g., ECG data), cardiac event information (e.g., real-time heart rate data), and additional physiological and/or other information to the monitoring station 140. The cardiac monitoring apparatus 120 can include an implantable medical device, such as an implantable cardiac defibrillator and an associated transceiver or pacemaker and an associated transceiver, or an external monitoring device that the patient wears. Moreover, the cardiac monitoring apparatus 120 can be implemented using, for example, the CardioNet Mobile Cardiac Outpatient Telemetry (MCOT) device, which is commercially available and provided by CardioNet, Inc of San Diego, CA.

[0017] The monitoring station 140 can include a receiver element for receiving transmitted signals, as well as various data processing and storage elements for extracting and storing information carried by transmissions regarding the state of the individual 110. The monitoring station 140 can be located in the same general location (e.g., in the same room, building or health care facility) as the monitoring apparatus 120, or at a remote location. The monitoring station 140 can include a display and a processing system, and a system operator 150 (e.g., a doctor or a cardiovascular technician) can use the monitoring station 140 to evaluate physiological data received from the cardiac monitoring apparatus 120. The system operator 150 can use the monitoring station 140 to change operational settings of the cardiac monitoring apparatus 120 remotely during active cardiac monitoring of the living being 110. Moreover, the cardiac monitoring apparatus 120 can selectively activate a T wave filter in response to discovery of a predetermined characteristic in the sensed cardiac signal, such as described further below. For example, the system operator can determine that the patient has consistently abnormal T waves and cause the monitoring station 140 to send a message to the monitoring apparatus 120 to activate the T wave filter.

[0018] FIG. 2 illustrates an example cardiac monitoring apparatus 200 used with a living being. The apparatus 200 can include a sensor 210, a signal amplifier 220, a T wave filter 230, a selector 240, a beat detector 250, additional logic 260, and a communications interface 270. The sensor 210 can include two or more electrodes subject to one or more potential differences that yield a voltage signal, such as the signals illustrated in FIGS. 3 and 4. The electrodes can be body surface electrodes such as silver/silver chloride electrodes and can be positioned at defined locations to aid in monitoring the electrical activity of the heart. The sensor 210 can also include leads or other conductors that form a signal path to the signal amplifier 220. The signal amplifier 220 can receive and amplify the voltage signals.

[0019] Furthermore, the signal amplifier 220 can include additional processing logic. For example, the additional processing logic can perform filtering and analog-to-digital conversion; the T wave filter 230 can be

integrated into the signal amplifier 220. Additional processing logic can also be implemented elsewhere in the apparatus 200, and the amplification and other additional processing can occur before or after digitization.

5 The signal amplifier 220 can provide an amplified and processed signal to the T wave filter 230 and to the selector 240. Moreover, some of the additional processing logic discussed in connection with FIG. 2 can also be implemented in the monitoring station 140.

10 **[0020]** The various components of the apparatus 200 can be implemented as analog or digital components. For example, the selector 240 can be analog, selective activation circuitry that selects one of its two inputs (from the signal amplifier 220 and from the T wave filter 230) to be provided to the beat detector 250. Alternatively, the selector 240 can enable and disable the T wave filter 230 (e.g., the T wave filter 230 can be integrated into the beat detector 250 and turned on and off as needed). In general, the selector 240 activates the T wave filter 230 with respect to the heart beat detector 250, to preprocess the signal, in response to a message (e.g., a message received from the monitoring station 140 or a message generated within the apparatus 200).

15 **[0021]** The beat detector 250 is a component (e.g., analog circuitry or digital logic) that identifies the time period between ventricular contractions. For example, the beat detector 250 can be a real-time QRS detector that identifies successive QRS complexes, or R waves, and determines the beat-to-beat timing in real time (i.e., output data is generated directly from live input data). The beat-to-beat timing can be determined by measuring times between successive R-waves. The beat detector 250 can provide information regarding the time period between ventricular contractions to additional logic 260. The additional logic 260 can include logic to determine if an abnormal T wave potentially is occurring based on signal morphology analysis, an atrial fibrillation/atrial flutter (AF) detector, AF decision logic, and an event generator. The heart rate information can be transmitted using the communications interface 270, which can be a wired or wireless interface. Moreover, the sensed cardiac signal, or portions thereof, can be sent to a monitoring station, periodically, upon being interrogated and/or in response to identified events/conditions.

25 **[0022]** The morphology of a cardiac signal can vary significantly from patient to patient. Sometimes, the patient's ECG has a very tall T wave, which might result in false classification of this T wave as an R wave. When this happens, the heart rate reported by the apparatus may be twice the real heart rate, and the morphology of beats may not be detected correctly. The T wave filter 230 can reduce the amplitude of T waves, while preserving or slightly increasing the amplitude of R waves.

30 **[0023]** FIG. 3 illustrates an example ECG 300 of a normal patient. The heart cycle has four generally recognized waveforms: the P wave, the QRS complex, the T wave, and the U wave. The relative sizes of a QRS complex 310 and a T wave 320 represent the signal from a

typical heart. FIG. 4 illustrates an example ECG 400 of a patient with abnormal T waves. As shown, a T wave 420 is tall in comparison with a normal T wave 320, and the rest of the cardiac cycle looks the same. In general, abnormal T waves can result in misclassification of T waves as R waves. In these cases, the T wave filter can be selectively applied to improve cardiac monitoring performance. The reduction in amplitude of the T wave may be up to 80% (five times) and can thus create a significant increase in the accuracy of QRS detection in patients with abnormal T waves.

[0024] FIG. 5 illustrates a process of selectively activating a T wave filter. Heart beats are identified in sensed cardiac signals at 500. A T wave filter is selectively activated in response to discovery of a predetermined characteristic in the sensed cardiac signal at 510. The discovery of the predetermined characteristic can involve an operator's identification of a tall T wave in at least a portion of the sensed cardiac signal, and activating the T wave filter can improve the cardiac monitoring. After filter activation, heart beats are identified in sensed cardiac signals using the activated T wave filter at 520. The T wave filter can be a custom highpass-like filter. The filter can be such that it reduces signal amplitude at low frequencies of the sensed cardiac signal and increases signal amplitude at high frequencies of the sensed cardiac signal.

[0025] FIG. 6 illustrates a frequency response 600 of an example T wave filter. As shown, the filter's frequency response can be less than or equal to -10 dB in the low frequency range of 0-5 Hertz (Hz). This frequency range is where T wave power spectrum is predominantly located. At higher frequencies, the filter can preserve and/or increase the amplitude of the signal (e.g., modify the signal by 0 dB or more for frequencies above 10 Hz), which can increase the amplitude of the R wave and make the beat detection more reliable. As shown, the filter's frequency response can be +2 dB or more in a high frequency range of 20-25 Hz. FIG. 7 illustrates an impulse response 700 of the example T wave filter illustrated in FIG. 6.

[0026] FIG. 8 illustrates an example distributed process for selectively activating a T wave filter. Heart beats are identified in a sensed cardiac signal at 800. The cardiac signal can be from a monitoring apparatus in contact with a living being under active cardiac monitoring, as described above. A possibly abnormal T wave can be determined in a post-processing operation that analyzes signal morphology, and a system operator can be notified of the possible abnormal T wave at 805; this operation can alternatively be done at the monitoring station, as mentioned below. This can assist the operator in identifying patients that may benefit from having the T wave filter activated in their monitors. Additionally, the operator can proactively check the sensed cardiac signal from the monitor to assess the T waves.

[0027] At least a portion of the sensed cardiac signal can be sent to a monitoring station at 810. This can in-

volve continuously or periodically sending the cardiac signal, or sending the cardiac signal in response to identified events/conditions, such as the identification of the possible abnormal T wave at 805. The sensed cardiac signals are received from the monitoring apparatus at 815. A possibly abnormal T wave can be determined using a signal morphology analyzer, and a system operator can be notified of the possible abnormal T wave at 820.

[0028] An abnormal T wave can be identified, such as by a system operator, in the received cardiac signal at 825, and a message can be sent to the monitoring apparatus over a communications channel at 830. The message causes the monitoring apparatus to activate a T wave filter used in identifying heart beats of the living being under active cardiac monitoring. The T wave filter is activated in response to the message at 835. Information corresponding to the heart beats identified using the T wave filter (e.g., heart rate data) can be output to the communications channel at 840. This information can be received at the monitoring station at 845.

[0029] Moreover, if the system operator subsequently determines that the T wave filter is not needed for the patient, a message to deactivate the T wave filter can be sent at 850, and the T wave filter can be deactivated in response to this second message at 855. The T wave filter may not distinguish morphology of the beat. Therefore, slow ventricular beats, such as premature ventricular contractions (PVCs), or some ectopic beats may also be reduced in amplitude when the filter is applied. In cases where multiple PVCs are monitored, the T wave filter may reduce the amplitude of these beats, and thus a pause or asystole event may be generated, which generally should alert the system operator to deactivate the T wave filter. However, this may not be relevant in the particular application as many cardiac monitoring applications do not require monitoring of PVCs or ectopic beats.

[0030] Fast ventricular beats (with a rate over 100 beats per minute) may be left unchanged by the T wave filter because their power spectrum is usually above 10Hz. The T wave filter described can be installed into a monitoring apparatus that includes a preexisting beat detector. The T wave filter can preprocess the input provided to the preexisting beat detector, improving the functioning of the beat detector for individuals with abnormal T waves, even though the preexisting beat detector was designed without a T wave filter in mind. The T wave filter can be in a disabled state by default and may be turned on only for the monitors used with those individuals with abnormal T waves (e.g., patients whose cardiac signal features constant tall T waves).

[0031] The systems and techniques described and illustrated in this specification can be implemented in analog electronic circuitry, digital electronic circuitry, integrated circuitry, computer hardware, firmware, software, or in combinations of the foregoing, such as the structural means disclosed in this specification and structural equivalents thereof. Apparatus can be implemented in a

software product (e.g., a computer program product) tangibly embodied in a machine-readable storage device for execution by a programmable processor, and processing operations can be performed by a programmable processor executing a program of instructions to perform functions by operating on input data and generating output. Further, the system can be implemented advantageously in one or more software programs that are executable on a programmable system. This programmable system can include the following: 1) at least one programmable processor coupled to receive data and instructions from, and to transmit data and instructions to, a data storage system; 2) at least one input device; and 3) at least one output device. Moreover, each software program can be implemented in a high-level procedural or object-oriented programming language, or in assembly or machine language if desired; and in any case, the language can be a compiled or an interpreted language.

[0032] Also, suitable processors include, by way of example, both general and special purpose microprocessors. Generally, a processor will receive instructions and data from a read-only memory, a random access memory, and/or a machine-readable signal (e.g., a digital signal received through a network connection). Generally, a computer will include one or more mass storage devices for storing data files. Such devices can include magnetic disks, such as internal hard disks and removable disks, magneto-optical disks, and optical disks. Storage devices suitable for tangibly embodying software program instructions and data include all forms of non-volatile memory, including, by way of example, the following: 1) semiconductor memory devices, such as EPROM (electrically programmable read-only memory); EEPROM (electrically erasable programmable read-only memory) and flash memory devices; 2) magnetic disks such as internal hard disks and removable disks; 3) magneto-optical disks; and 4) optical disks, such as CD-ROM disks. Any of the foregoing can be supplemented by, or incorporated in, ASICs (application-specific integrated circuits).

[0033] To provide for interaction with a user (such as the system operator), the system can be implemented on a computer system having a display device such as a monitor or LCD (liquid crystal display) screen for displaying information to the user and a keyboard and a pointing device such as a mouse or a trackball by which the user can provide input to the computer system. The computer system can be programmed to provide a graphical user interface through which computer programs interact with users and operational settings can be changed in the monitoring system.

[0034] Finally, while the foregoing system has been described in terms of particular implementations, other embodiments are within the scope of the following claims.

Claims

1. A machine-implemented method comprising:

5 identifying (800) heart beats in a sensed cardiac signal; **characterised by** :

10 selectively activating (835) a T wave filter (230) used in said identifying heart beats in response to a message from a monitoring station (140), the message generated at least in part based upon discovery of a predetermined characteristic in the sensed cardiac signal; and
15 outputting (840) information corresponding to the identified heart beats to a communications channel of a distributed cardiac activity monitoring system (100).

20 2. The method of claim 1, wherein said identifying (800) heart beats comprises identifying R waves in the sensed cardiac signal.

25 3. The method of claim 1, further comprising sending (810) at least a portion of the sensed cardiac signal to the monitoring station (140), and wherein the discovery of the predetermined characteristic comprises identification of a tall T wave in the at least a portion of the sensed cardiac signal by an operator at the monitoring station (140).
30

35 4. The method of claim 1, wherein said selectively activating (835) the T wave filter comprises selectively activating a filter that reduces signal amplitude at low frequencies of the sensed cardiac signal.

40 5. The method of claim 4, wherein the filter has a frequency response of about 0 dB or more at frequencies above ten Hertz.

45 6. The method of claim 5, wherein the filter has a frequency response of about -10 dB or less in a low frequency range of zero to five Hertz.

50 7. The method of claim 6, wherein the filter has a frequency response of about +2 dB or more in a high frequency range of twenty to twenty five Hertz.

8. The method of claim 1, wherein said outputting (840) information comprises outputting heart rate data to a wireless communications channel.

9. The method of claim 1, further comprising:

55 determining that an abnormal T wave is possible based on signal morphology analysis; and notifying a system operator of the possible abnormal T wave.

10. The method of claim 1, further comprising deactivating the T wave filter in response to a second message.
11. A method comprising:
- receiving at least a portion of a sensed cardiac signal from a monitoring apparatus in contact with a living being under active cardiac monitoring;
 identifying (825) an abnormal T wave in the received cardiac signal; and
characterised by further comprising :
- sending (830) a message to the monitoring apparatus over a communications channel, the message causing the monitoring apparatus to selectively activate a T wave filter used in identifying heart beats of the living being under active cardiac monitoring.
12. The method of claim 11, further comprising:
- determining that the abnormal T wave is possible based on signal morphology analysis; and
 notifying a system operator of the possible abnormal T wave, wherein the system operator performs said identifying the abnormal T wave.
13. The method of claim 11, wherein said sending (830) the message comprises sending the message over a wireless communications channel.
14. The method of claim 11, further comprising installing the T wave filter (230) into the monitoring apparatus (120), which comprises a preexisting beat detector.
15. A cardiac monitoring apparatus (120) comprising:
- a communications interface (270);
 a real-time heart beat detector (250);
 a T wave filter (230); and **characterised by** :
- a selector (240) that is configured to selectively activate the T wave filter (230) with respect to the real-time heart beat detector (250) in response to a message, wherein the selectively activated T wave filter (230) is configured to preprocess a cardiac signal provided to the real-time heart beat detector (250).
16. The apparatus of claim 15, wherein the real-time heart beat detector (250) comprises an analog heart beat detector, the T wave filter (230) comprises an analog T wave filter, and the selector (240) comprises analog, selective activation circuitry.
17. The apparatus of claim 15, further comprising additional logic that is configured to determine if an abnormal T wave is possible based on signal morphology analysis, and notifies a system operator of the possible abnormal T wave.
18. A distributed cardiac activity monitoring system (100) comprising: an apparatus according to claim 15 and a monitoring station (140) that is configured to communicatively couple with the monitoring apparatus (120) via the communications interface and to transmit the message to the monitoring apparatus to selectively activate the T wave filter (230) based at least in part upon a predetermined criteria.
19. The system of claim 18, wherein the selector (240) comprises analog, selective activation circuitry.
20. The system of claim 18, wherein the monitoring apparatus (120) or the monitoring station (140) further comprises additional logic that is configured to determine if an abnormal T wave is possible based on signal morphology analysis, and to notify a system operator of the possible abnormal T wave.
21. The apparatus of claim 15 or the system of claim 18, wherein the communications interface (270) comprises a wireless communications interface.
22. The apparatus of claim 15 or the system of claim 18, wherein the T wave filter comprises a filter that is configured to reduce signal amplitude at low frequencies.
23. The apparatus of claim 15 or the system of claim 22, wherein the filter has a frequency response of about -10 dB or less in a low frequency range of zero to five Hertz.
24. The apparatus of claim 15 or the system of claim 22, wherein the filter has a frequency response of about 0 dB or more at frequencies above ten Hertz.
25. The apparatus of claim 15 or the system of claim 24, wherein the filter has a frequency response of about +2 dB or more in a high frequency range of twenty to twenty five Hertz.
- Patentansprüche**
1. Maschinell durchgeführtes Verfahren, das Folgendes umfasst:
- Identifizierung (800) von Herzschlägen in einem gemessenen Herzsignal;
gekennzeichnet durch:

- selektive Aktivierung (835) eines T-Wellen-Filters (230) zu der Identifizierung von Herzschlägen als Reaktion auf eine Nachricht von einer Überwachungsstation (140), wobei die Nachricht zumindest teilweise auf Grundlage der Entdeckung einer vorbestimmten Eigenschaft im gemessenen Herzsignal erzeugt wird; und
Ausgabe (840) von Information, die den identifizierten Herzschlägen entspricht, an einen Kommunikationskanal eines verteilten Herzaktivitäts-Überwachungssystems (100).
2. Verfahren nach Anspruch 1, worin die Identifizierung (800) der Herzschläge die Identifizierung von R-Wellen im gemessenen Herzsignal umfasst.
 3. Verfahren nach Anspruch 1, das ferner die Sendung (810) zumindest eines Teils des gemessenen Herzsignals an die Überwachungsstation (140) umfasst und worin die Entdeckung der vorbestimmten Eigenschaft die Identifizierung einer großen T-Welle in dem zumindest einen Teil des gemessenen Herzsignals durch einen Bediener an der Überwachungsstation (140) umfasst.
 4. Verfahren nach Anspruch 1, worin die selektive Aktivierung (835) des T-Wellen-Filters die selektive Aktivierung eines Filters umfasst, der die Signalamplitude bei niedrigen Frequenzen des gemessenen Herzsignals reduziert.
 5. Verfahren nach Anspruch 4, worin der Filter eine Frequenzantwort von ca.
0 dB oder mehr bei Frequenzen über zehn Hertz aufweist.
 6. Verfahren nach Anspruch 5, worin der Filter eine Frequenzantwort von ca.
- 10 dB oder weniger in einem niedrigen Frequenzbereich von null bis fünf Hertz aufweist.
 7. Verfahren nach Anspruch 6, worin der Filter eine Frequenzantwort von ca.
+2 dB oder mehr in einem hohen Frequenzbereich von zwanzig oder fünfundzwanzig Hertz aufweist.
 8. Verfahren nach Anspruch 1, worin die Ausgabe (840) von Information die Ausgabe von Herzfrequenzdaten an einen drahtlosen Kommunikationskanal umfasst.
 9. Verfahren nach Anspruch 1, das ferner Folgendes umfasst:
- Bestimmung, dass eine anomale T-Welle möglich ist, auf Grundlage von Signalmorphologieanalyse; und
Benachrichtigung eines Systembedieners über die mögliche anomale T-Welle.
10. Verfahren nach Anspruch 1, das ferner die Deaktivierung des T-Wellen-Filters als Reaktion auf eine zweite Nachricht umfasst.
 11. Verfahren, das Folgendes umfasst:
Empfang zumindest eines Teils eines gemessenen Herzsignals von einem Überwachungsgerät, das mit einem unter aktiver Herzüberwachung stehenden Lebewesen in Kontakt ist; Identifizierung (825) einer anomalen T-Welle in dem empfangenen Herzsignal; und
dadurch gekennzeichnet, dass es ferner Folgendes umfasst:
Senden (830) einer Nachricht an das Überwachungsgerät über einen Kommunikationskanal, wobei die Nachricht das Überwachungsgerät veranlasst, einen zur Identifizierung von Herzschlägen des unter aktiver Herzüberwachung stehenden Lebewesens verwendeten T-Wellen-Filter selektiv zu aktivieren.
 12. Verfahren nach Anspruch 11, das ferner Folgendes umfasst:
Bestimmung, dass die anomale T-Welle möglich ist, auf Grundlage von Signalmorphologieanalyse; und
Benachrichtigung eines Systembedieners über die mögliche anomale T-Welle, worin der Systembediener die Identifizierung der anomalen T-Welle durchführt.
 13. Verfahren nach Anspruch 11, worin das Senden (830) der Nachricht das Senden der Nachricht über einen drahtlosen Kommunikationskanal umfasst.
 14. Verfahren nach Anspruch 11, das ferner die Installation des T-Wellen-Filters (230) in dem Überwachungsgerät (120) umfasst, das einen bereits existierenden Herzschlagdetektor umfasst.
 15. Herzüberwachungsgerät (120), das Folgendes umfasst:
eine Kommunikationsschnittstelle (270);
einen Echtzeit-Herzschlagdetektor (250);
einen T-Wellen-Filter (230); und **gekennzeichnet**

net durch:

- einen Selektor (240), der zur selektiven Aktivierung des T-Wellen-Filters (230) relativ zum Echtzeit-Herzschlagdetektor (250) als Reaktion auf eine Nachricht konfiguriert ist, worin der selektiv aktivierte T-Wellen-Filter (230) zur Voraufbereitung eines Herzsignals, das dem Echtzeit-Herzschlagdetektor (250) zugeführt wird, konfiguriert ist.
16. Gerät nach Anspruch 15, worin der Echtzeit-Herzschlagdetektor (250) einen analogen Herzschlagdetektor umfasst, der T-Wellen-Filter (230) einen analogen T-Wellen-Filter umfasst und der Selektor (240) einen analogen selektiven Aktivierungskreislauf umfasst.
17. Gerät nach Anspruch 15, das ferner eine zusätzliche Logik umfasst, die dazu konfiguriert ist auf Grundlage von Signalmorphologieanalyse zu bestimmen, ob eine anomale T-Welle möglich ist, und einen Systembediener über die mögliche anomale T-Welle benachrichtigt.
18. Verteiltes Herzaktivitätsüberwachungssystem (100), das Folgendes umfasst:
- ein Gerät nach Anspruch 15 und eine Überwachungsstation (140), die zur kommunikativen Verbindung mit dem Überwachungsgerät (120) über die Kommunikationsschnittstelle und zur Übertragung der Nachricht an das Überwachungsgerät zur selektiven Aktivierung des T-Wellen-Filters (230) zumindest teilweise auf Grundlage eines vorbestimmten Kriteriums konfiguriert ist.
19. System nach Anspruch 18, worin der Selektor (240) einen analogen selektiven Aktivierungskreislauf umfasst.
20. System nach Anspruch 18, worin das Überwachungsgerät (120) oder die Überwachungsstation (140) ferner eine zusätzliche Logik umfasst, die dazu konfiguriert ist auf Grundlage von Signalmorphologieanalyse zu bestimmen, ob eine anomale T-Welle möglich ist, und einen Systembediener über die mögliche anomale T-Welle benachrichtigt.
21. Gerät nach Anspruch 15 oder System nach Anspruch 18, worin die Kommunikationsschnittstelle (270) eine drahtlose Kommunikationsschnittstelle umfasst.
22. Gerät nach Anspruch 15 oder System nach Anspruch 18, worin der T-Wellen-Filter einen Filter um-

fasst, der zur Reduzierung der Signalamplitude bei niedrigen Frequenzen konfiguriert ist.

23. Gerät nach Anspruch 15 oder System nach Anspruch 22, worin der Filter eine Frequenzantwort von ca. -10 dB oder weniger in einem niedrigen Frequenzbereich von null bis fünf Hertz aufweist.
24. Gerät nach Anspruch 15 oder System nach Anspruch 22, worin der Filter eine Frequenzantwort von ca. 0 dB oder mehr bei Frequenzen über zehn Hertz aufweist.
25. Gerät nach Anspruch 15 oder System nach Anspruch 24, worin der Filter eine Frequenzantwort von ca. +2 dB oder mehr in einem hohen Frequenzbereich von zwanzig bis fünfundzwanzig Hertz aufweist.

Revendications

1. Procédé mis en oeuvre par machine, comprenant l'étape consistant à :

identifier (800) des battements de coeur dans un signal cardiaque détecté ;
le procédé étant **caractérisé en ce qu'il** comprend les étapes consistant à :

activer de façon sélective (835) un filtre d'ondes T (230) utilisé à ladite étape consistant à identifier des battements de coeur en réponse à un message provenant d'un poste de surveillance (140), le message étant généré en fonction en partie au moins de la découverte d'une caractéristique prédéfinie dans le signal cardiaque détecté ; et fournir (840) des informations correspondant aux battements de coeur identifiés sur un canal de communication d'un système de surveillance répartie de l'activité cardiaque (100).

2. Procédé selon la revendication 1, dans lequel ladite étape consistant à identifier (800) des battements de coeur comprend l'étape consistant à identifier des ondes R dans le signal cardiaque détecté.
3. Procédé selon la revendication 1, comprenant en outre l'étape consistant à transmettre (810) au moins une partie du signal cardiaque détecté au poste de surveillance (140), et dans lequel la découverte de la caractéristique prédéfinie comprend l'identification, par un opérateur au niveau du poste de surveillance (140), d'une onde T haute dans ladite au moins une partie du signal cardiaque détecté.

4. Procédé selon la revendication 1, dans lequel ladite étape consistant à activer de façon sélective (835) le filtre d'ondes T comprend l'étape consistant à activer de façon sélective un filtre qui réduit l'amplitude du signal aux basses fréquences du signal cardiaque détecté. 5
5. Procédé selon la revendication 4, dans lequel le filtre possède une réponse en fréquence d'environ 0 dB ou plus aux fréquences supérieures à 10 Hz. 10
6. Procédé selon la revendication 5, dans lequel le filtre possède une réponse en fréquence d'environ 10 dB ou moins dans une plage de basses fréquences allant de 0 à 5 Hz. 15
7. Procédé selon la revendication 6, dans lequel le filtre possède une réponse en fréquence d'environ +2 dB ou plus dans une plage de hautes fréquences allant de 20 à 25 Hz. 20
8. Procédé selon la revendication 1, dans lequel ladite étape consistant à fournir (840) des informations comprend l'étape consistant à fournir des données de fréquence cardiaque sur un canal de communication sans fil. 25
9. Procédé selon la revendication 1, comprenant en outre les étapes consistant à : 30
- établir qu'une onde T anormale est possible à partir d'une analyse morphologique de signal ; et
- informer un opérateur du système de l'onde T anormale possible. 35
10. Procédé selon la revendication 1, comprenant en outre l'étape consistant à désactiver le filtre d'ondes T en réponse à un deuxième message. 40
11. Procédé, comprenant les étapes consistant à : 45
- recevoir au moins une partie d'un signal cardiaque détecté provenant d'un appareil de surveillance au contact d'un être vivant sous surveillance cardiaque active ;
- identifier (825) une onde T anormale dans le signal cardiaque reçu ; et
- le procédé étant **caractérisé en ce qu'il** comprend en outre l'étape consistant à : 50
- transmettre (830) un message à l'appareil de surveillance sur un canal de communication, le message amenant l'appareil de surveillance à activer de façon sélective un filtre d'ondes T utilisé pour identifier des battements de coeur de l'être vivant sous surveillance cardiaque active. 55
12. Procédé selon la revendication 11, comprenant en outre les étapes consistant à : 60
- établir que l'onde T anormale est possible à partir d'une analyse morphologique de signal ; et
- informer un opérateur du système de l'onde T anormale possible, lequel opérateur du système exécute ladite étape consistant à identifier l'onde T anormale. 65
13. Procédé selon la revendication 11, dans lequel ladite étape consistant à transmettre (830) le message comprend l'étape consistant à transmettre le message sur un canal de communication sans fil. 70
14. Procédé selon la revendication 11, comprenant en outre l'étape consistant à installer le filtre d'ondes T (230) dans l'appareil de surveillance (120), lequel comprend un détecteur de battements préexistant. 75
15. Appareil de surveillance cardiaque (120), comprenant : 80
- une interface de communication (270) ;
- un détecteur de battements de coeur en temps réel (250) ;
- un filtre d'ondes T (230) ; et
- l'appareil étant **caractérisé par** : 85
- un sélecteur (240) conçu pour activer de façon sélective le filtre d'ondes T (230) par rapport au détecteur de battements de coeur en temps réel (250) en réponse à un message, le filtre d'ondes T (230) activé de façon sélective étant conçu pour soumettre à un prétraitement un signal cardiaque fourni au détecteur de battements de coeur en temps réel (250). 90
16. Appareil selon la revendication 15, dans lequel le détecteur de battements de coeur en temps réel (250) comprend un détecteur de battements de coeur analogique, le filtre d'ondes T (230) comprend un filtre d'ondes T analogique et le sélecteur (240) comprend un montage de circuits d'activation sélective analogique. 95
17. Appareil selon la revendication 15, comprenant en outre une logique supplémentaire conçue pour établir si une onde T anormale est possible à partir d'une analyse morphologique de signal, et pour informer un opérateur du système de l'onde T anormale possible. 100
18. Système de surveillance répartie de l'activité cardiaque (100), comprenant 105
- un appareil selon la revendication 15 ; et
- un poste de surveillance (140) conçu pour être relié

à l'appareil de surveillance (120) pour communiquer avec lui par l'interface de communication, et pour transmettre le message à l'appareil de surveillance afin d'activer de façon sélective le filtre d'ondes T (230) en fonction en partie au moins d'un critère prédéfini. 5

19. Système selon la revendication 18, dans lequel le sélecteur (240) comprend un montage de circuits d'activation sélective analogique. 10
20. Système selon la revendication 18, dans lequel l'appareil de surveillance (120) le poste de surveillance (140) comprend en outre une logique supplémentaire conçue pour établir si une onde T anormale est possible à partir d'une analyse morphologique de signal, et pour informer un opérateur du système de l'onde T anormale possible. 15
21. Appareil selon la revendication 15 ou système selon la revendication 18, dans lequel l'interface de communication (270) comprend une interface de communication sans fil. 20
22. Appareil selon la revendication 15 ou système selon la revendication 18, dans lequel le filtre d'ondes T comprend un filtre conçu pour réduire l'amplitude du signal aux basses fréquences. 25
23. Appareil selon la revendication 15 ou système selon la revendication 22, dans lequel le filtre possède une réponse en fréquence d'environ -10 dB ou moins dans une plage de basses fréquences allant de 0 à 5 Hz. 30
24. Appareil selon la revendication 15 ou système selon la revendication 22, dans lequel le filtre possède une réponse en fréquence d'environ 0 dB ou plus aux fréquences supérieures à 10 Hz. 35
25. Appareil selon la revendication 15 ou système selon la revendication 24, dans lequel le filtre possède une réponse en fréquence d'environ +2 dB ou plus dans une plage de hautes fréquences allant de 20 à 25 Hz. 40

45

50

55

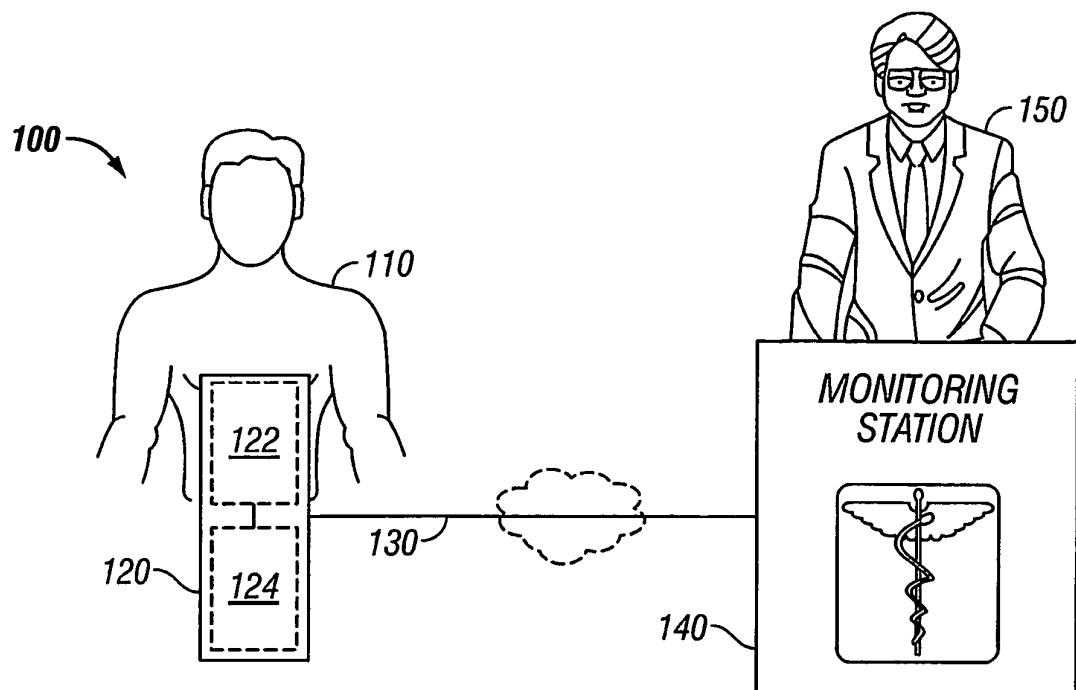


FIG. 1

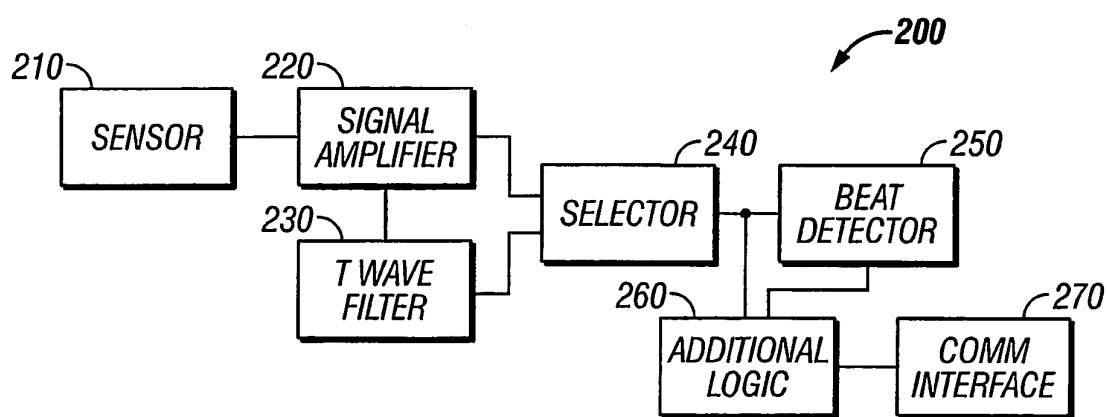


FIG. 2

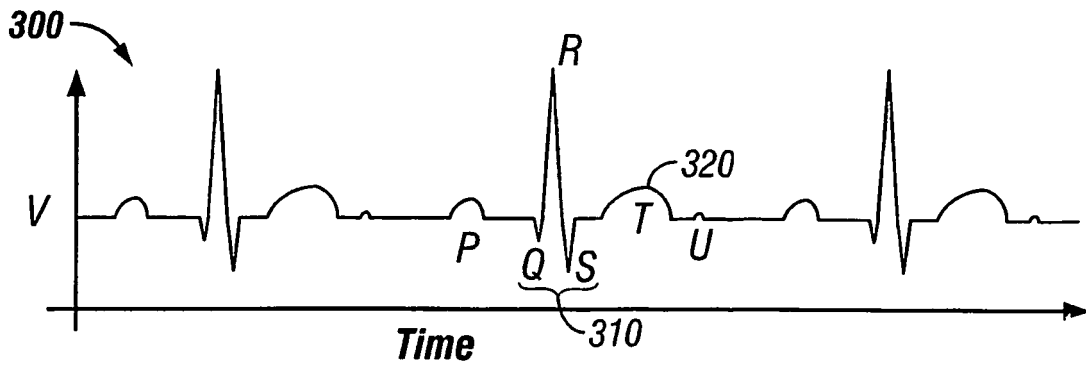


FIG. 3

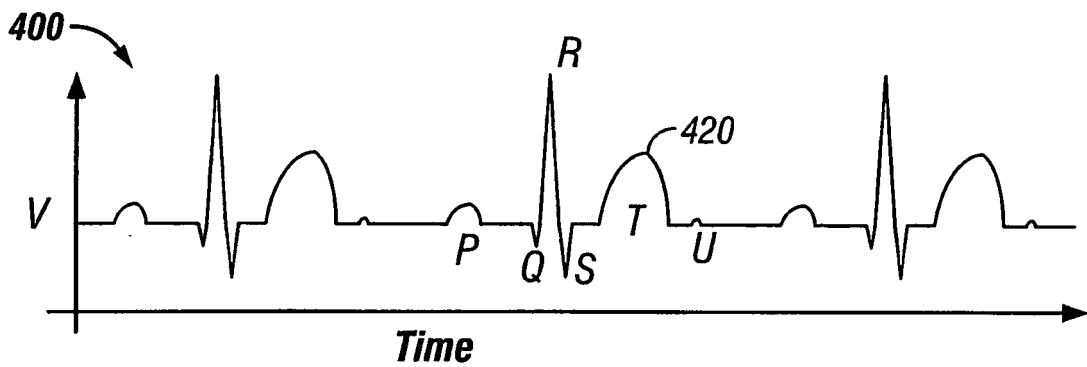


FIG. 4

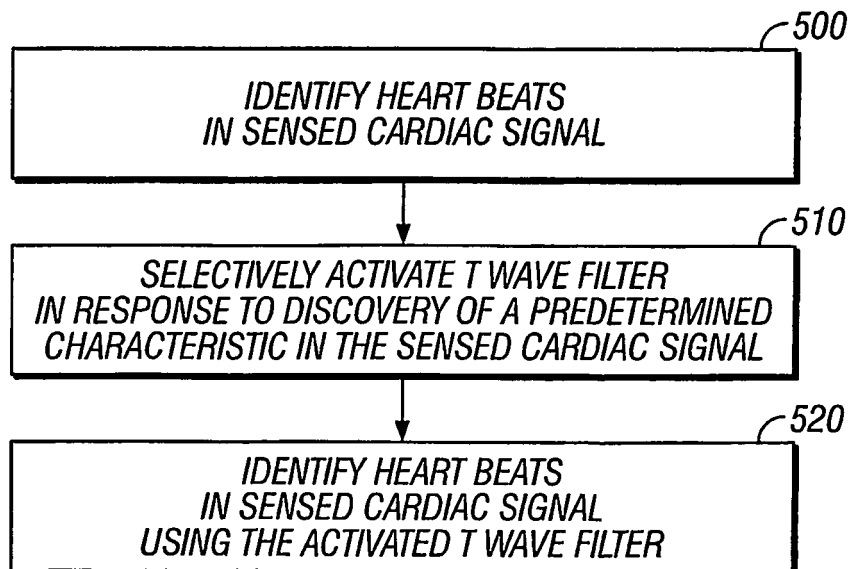


FIG. 5

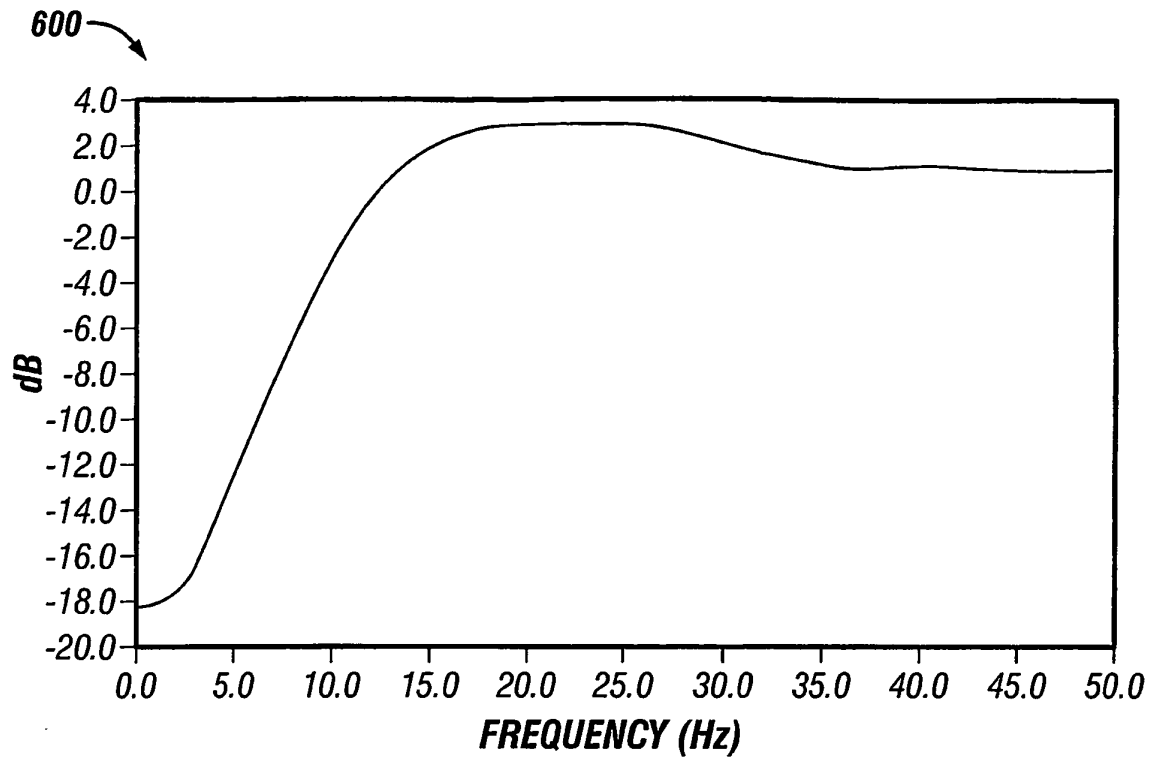


FIG. 6

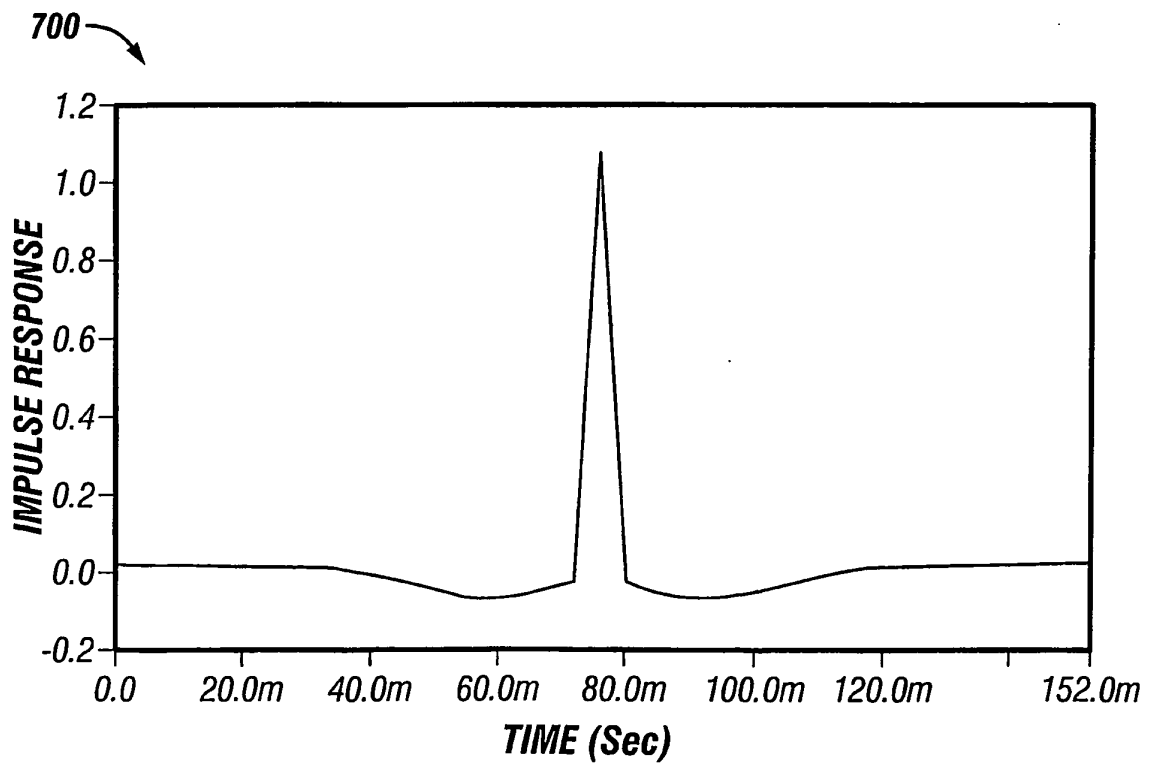


FIG. 7

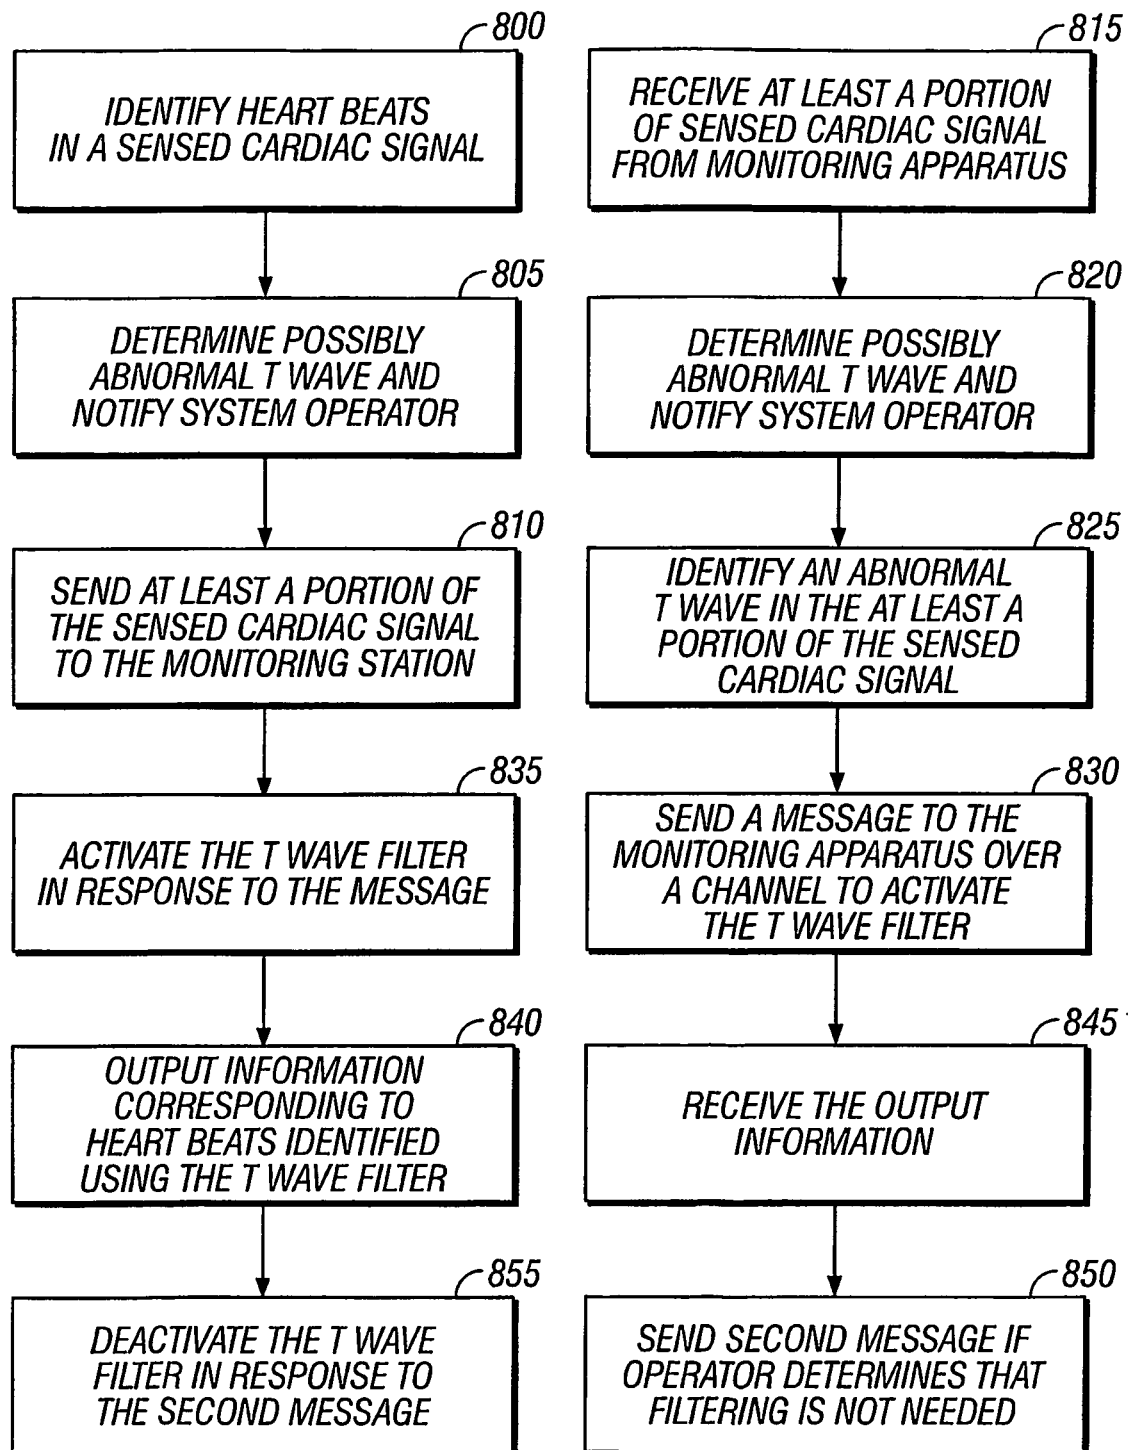


FIG. 8

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 3593705 A [0004]
- US 4240442 A [0004]
- US 2003204215 A [0004]
- US 4887609 A [0004]
- US 6167258 A [0004]

专利名称(译)	分布式心脏活动监测与选择性过滤		
公开(公告)号	EP1722680A4	公开(公告)日	2009-07-01
申请号	EP2005713679	申请日	2005-02-16
申请(专利权)人(译)	CARDIONET INC.		
当前申请(专利权)人(译)	CARDIONET INC.		
[标]发明人	KORZINOV LEV CHURCHVILLE DAVE CYBULSKI ZACH		
发明人	KORZINOV, LEV CHURCHVILLE, DAVE CYBULSKI, ZACH		
IPC分类号	A61B5/04 A61B5/00 A61B5/0452		
CPC分类号	A61B5/0006 A61B5/0452 Y10S128/901		
优先权	10/781045 2004-02-17 US		
其他公开文献	EP1722680A2 EP1722680B1		
外部链接	Espacenet		

摘要(译)

用于心脏活动的分布式监测的系统和技术包括选择性T波滤波。通常，在一个实施方式中，分布式心脏活动监测系统包括监测装置，其具有选择性激活的T波滤波器和监测站。监视设备可以包括通信接口，实时QRS检测器，T波滤波器和选择器，其激活T波滤波器以响应于消息预处理提供给实时QRS检测器的心脏信号。监控站可以通过通信接口通过通信接口与监控设备通信耦合，并且可以至少部分地基于预定标准（例如，异常T波）将消息发送到监控设备以激活T波滤波器。对于个人而言，由系统操作员确定）。

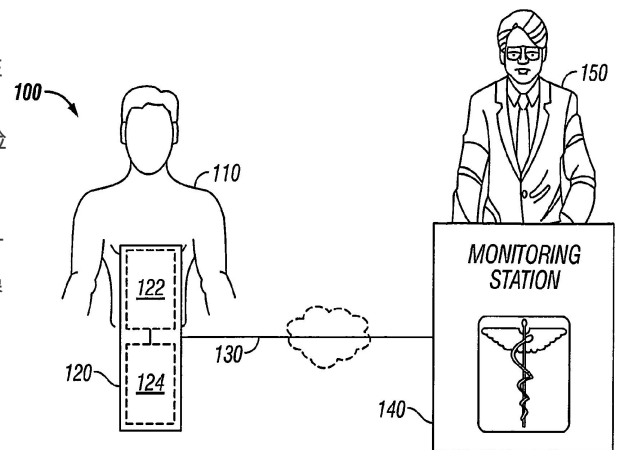


FIG. 1