

(19)



(11)

EP 1 586 051 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:

13.04.2016 Bulletin 2016/15

(51) Int Cl.:

G06F 17/00 (2006.01) **A61B 5/00** (2006.01)
A61B 5/1455 (2006.01) **A61B 5/01** (2006.01)
A61B 5/021 (2006.01) **A61B 5/024** (2006.01)
G06K 9/00 (2006.01)

(21) Application number: **03800274.7**

(22) Date of filing: **29.12.2003**

(86) International application number:
PCT/US2003/041467

(87) International publication number:
WO 2004/066161 (05.08.2004 Gazette 2004/32)

(54) SELECTION OF PRESET FILTER PARAMETERS BASED ON SIGNAL QUALITY

AUSWAHL VOREINGESTELLTER FILTERPARAMETER AUF GRUNDLAGE DER SIGNALQUALITÄT

SELECTION DE PARAMETRES DE FILTRE PREREGLES FONDEE SUR LA QUALITE DU SIGNAL

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PT RO SE SI SK TR

(30) Priority: **13.01.2003 US 341722**

(43) Date of publication of application:
19.10.2005 Bulletin 2005/42

(73) Proprietor: **Covidien LP**
Mansfield, MA 02048 (US)

(72) Inventor: **STETSON, Paul, F.**
Oakland, CA 94611 (US)

(74) Representative: **Kinsler, Maureen Catherine et al**
Marks & Clerk LLP
Atholl Exchange
6 Canning Street
Edinburgh EH3 8EG (GB)

(56) References cited:
US-A- 5 769 785 **US-A- 6 135 952**
US-A1- 2002 003 832 **US-A1- 2002 045 806**
US-A1- 2002 099 282

EP 1 586 051 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

[0001] The present invention relates to the processing of signals obtained from a medical diagnostic apparatus, such as a pulse oximeter, using a digital filter to reduce noise effects.

[0002] A typical pulse oximeter measures two physiological parameters, percent oxygen saturation of arterial blood hemoglobin (SpO₂ or sat) and pulse rate. Oxygen saturation can be estimated using various techniques. In one common technique, the photocurrent generated by the photo-detector is conditioned and processed to determine the ratio of modulation ratios (ratio of ratios) of the red to infrared signals. This modulation ratio has been observed to correlate well to arterial oxygen saturation. The pulse oximeters and sensors are empirically calibrated by measuring the modulation ratio over a range of in vivo measured arterial oxygen saturations (SaO₂) on a set of patients, healthy volunteers, or animals. The observed correlation is used in an inverse manner to estimate blood oxygen saturation (SpO₂) based on the measured value of modulation ratios of a patient. The estimation of oxygen saturation using modulation ratios is described in U.S. Patent No. 5,853,364, entitled "METHOD AND APPARATUS FOR ESTIMATING PHYSIOLOGICAL PARAMETERS USING MODEL-BASED ADAPTIVE FILTERING," issued December 29, 1998, and U.S. Patent No. 4,911,167, entitled "METHOD AND APPARATUS FOR DETECTING OPTICAL PULSES," issued March 27, 1990. The relationship between oxygen saturation and modulation ratio is further described in U.S. Patent No. 5,645,059, entitled "MEDICAL SENSOR WITH MODULATED ENCODING SCHEME," issued July 8, 1997. Most pulse oximeters extract the plethysmographic signal having first determined saturation or pulse rate, both of which are susceptible to interference.

[0003] A challenge in pulse oximetry is in analyzing the data to obtain a reliable measure of a physiologic parameter in the presence of large interference sources. Various solutions to this challenge have included methods that assess the quality of the measured parameter and decide on displaying the measured value when it is deemed reliable based upon a signal quality. Another approach involves a heuristic-based signal extraction technology, where the obtained signals are processed based on a series of guesses of the ratio, and which require the algorithm to start with a guess of the ratio, which is an unknown. Both the signal-quality determining and the heuristic signal extraction technologies are attempts at separating out a reliable signal from an unreliable one, one method being a phenomenological one and the other being a heuristic one.

[0004] A known approach for the reduction of noise in medical diagnostic devices including pulse oximeters involves the use of an adaptive filter, such as an adaptive

digital filter, for example as described in US 6,135,952 and US 6,721,584. The adaptive filter is actually a data processing algorithm, and in most typical applications, the filter is a computer program that is executed by a central processor. As such, the filter inherently incorporates discrete-time measurement samples rather than continuous time inputs. A type of digital filter that is used in pulse oximeter systems is a Kalman filter. While conventional adaptive digital filters in general and Kalman filters in particular have been assimilated in medical diagnostics system to help reduce noise in a signal, there are still many challenges that need to be addressed to improve the techniques that are used to reduce noise effects in signals; noise effects such as those present in a medical diagnostic device. One of the shortcomings of using a Kalman filter is that a Kalman filter is an adaptive filter whose functioning is mathematically-based and where its aim is to compare the output of the filter with a desired output, and reduce the error in the comparison by continuously varying the filter's coefficients. So, a Kalman filter generates filter coefficients in an adaptive manner to minimize an error. While this method has been adopted by many, it is still a method that is somewhat blind regarding the signal that it is being filtered. Such an approach does not take into account the unique attributes that an input signal may possess and which are physiologically based. Another shortcoming of the Kalman filtering is that the Kalman filter is linear in its input-output relationship. One can appreciate that in certain conditions, the requirement that the filter be linear in its input-output relationship is too constraining. Yet another shortcoming of a Kalman filter is that filter parameters are continuously tuned, which can be computationally expensive.

[0005] There is therefore a need to develop a filter for reducing noise effects in signals that does not suffer from the above-mentioned constraints of conventional adaptive filters.

BRIEF SUMMARY OF THE INVENTION

[0006] The present invention is directed towards methods and devices as defined in claims 1 and 10.

[0007] The digital filter can have either a linear or preferably a non-linear input-output relationship.

[0008] In pulse oximetry applications, the quality of the input signal may be assessed by obtaining or measuring signal parameters that include the skew of the time derivative of the signal; the correlation between signals from different wavelengths; the variation in signal amplitude, as well as others. Other assessments, such as maximum values or spectral peak frequencies, may also be used in determining filter parameters.

[0009] In some embodiments, the selection of filter parameters or coefficients is performed in real time, with the coefficients of the digital filter being determined using a current input sample. In certain other embodiments, the selection of filter parameters is performed using a

previously stored input signal sample.

[0010] In pulse oximetry applications, the input signals can be a function of an oxygen saturation, or a pulse rate. Furthermore, these signals correspond with sensed optical energies from a plurality of wavelengths.

[0011] For a further understanding of the nature and advantages of the invention, reference should be made to the following description taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012]

Fig. 1 is a block diagram of an exemplary oximeter. Fig. 2 is a block diagram depicting the operation of the signal-quality based filter operation in accordance with embodiments of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0013] The methods and systems in accordance with embodiments of the present invention are directed towards selecting and adjusting the parameters of a digital filter based an assessment of the quality of the input signals to the filter. The invention is particularly applicable to and will be explained by reference to measurements of oxygen saturation of hemoglobin in arterial blood and patient heart rate, as in pulse oximeter monitors and pulse oximetry sensors. However, it should be realized the invention is equally applicable to any generalized patient monitor and associated patient sensor, such as ECG, blood pressure, temperature, etc., and is not to be limited for use only with oximetry or pulse oximetry.

[0014] Fig. 1 is a block diagram of a pulse oximeter that may be configured to implement the embodiments of present invention. The filter embodiments of the present invention can be a data processing algorithm that is executed, by the microprocessor 122, described below. Light from light source 110 passes into patient tissue 112, and is scattered and detected by photodetector 114. A sensor 100 containing the light source and photodetector may also contain an encoder 116 which provides signals indicative of the wavelength of light source 110 to allow the oximeter to select appropriate calibration coefficients for calculating oxygen saturation. Encoder 116 may, for instance, be a resistor.

[0015] Sensor 100 is connected to a pulse oximeter 120. The oximeter includes a microprocessor 122 connected to an internal bus 124. Also connected to the bus is a RAM memory 126 and a display 128. A time processing unit (TPU) 130 provides timing control signals to light drive circuitry 132 which controls when light source 110 is illuminated, and if multiple light sources are used, the multiplexed timing for the different light sources. TPU 130 also controls the gating-in of signals from photodetector 114 through an amplifier 133 and a switching circuit 134. These signals are sampled at the proper time, depending

upon which of multiple light sources is illuminated, if multiple light sources are used. The received signal is passed through an amplifier 136, a low pass filter 138, and an analog-to-digital converter 140. The digital data is then stored in a queued serial module (QSM) 142, for later downloading to RAM 126 as QSM 142 fills up. In one embodiment, there may be multiple parallel paths of separate amplifier filter and A/D converters for multiple light wavelengths or spectrums received.

[0016] Based on the value of the received signals corresponding to the light received by photodetector 114, microprocessor 122 will calculate the oxygen saturation using various algorithms. These algorithms require coefficients, which may be empirically determined, corresponding to, for example, the wavelengths of light used. These are stored in a ROM 146. In a two-wavelength system, the particular set of coefficients chosen for any pair of wavelength spectrums is determined by the value indicated by encoder 116 corresponding to a particular light source in a particular sensor 100. In one embodiment, multiple resistor values may be assigned to select different sets of coefficients. In another embodiment, the same resistors are used to select from among the coefficients appropriate for an infrared source paired with either a near red source or far red source. The selection between whether the near red or far red set will be chosen can be selected with a control input from control inputs 154. Control inputs 154 may be, for instance, a switch on the pulse oximeter, a keyboard, or a port providing instructions from a remote host computer. Furthermore, any number of methods or algorithms may be used to determine a patient's pulse rate, oxygen saturation or any other desired physiological parameter.

[0017] The brief description of an exemplary pulse oximeter set forth above, serves as a contextual fabric for describing the methods for reducing noise effects in the received signals according to embodiments of the present invention, which are described below. The embodiments of the present invention, which are used to reduce the noise effects in the signal using an assessment of the quality of the input signal, are described below in conjunction with the block diagram of Fig. 2.

[0018] A signal quality indicator is a measured parameter that is capable of estimating the reliability and accuracy of a signal. For example, when measuring blood oxygen saturation using a pulse oximeter, a signal quality indicator is able to indirectly assess whether an estimate of a value of blood oxygen saturation is an accurate one. This determination of accuracy is made possible by a thorough and detailed study of volumes of measured values and various indicators to determine which indicators are indicative of signal quality and what, if any, is the correlation between the indicator and the accuracy of the estimated value.

[0019] In pulse oximetry, examples of signal quality indicators include the skew of the time derivative of the signal; the correlation between signals from different wavelengths; the variation in signal amplitude, as well as

others. Other assessments, such as maximum values or spectral peak frequencies, may also be used in determining filter parameters. In addition to these signal quality indicators, other signal quality indicators may also be used for the selection of filter coefficients. In pulse oximetry, these additional signal quality indicators include: a signal measure indicative of the degree of similarity of an infrared and red waveforms; a signal measure indicative of a low light level; a signal measure indicative of an arterial pulse shape; a signal measure indicative of the high frequency signal component in the measure value; a signal measure indicative of a consistency of a pulse shape; a signal measure indicative of an arterial pulse amplitude; a signal measure indicative of modulation ratios of red to infrared modulations and a signal measure indicative of a period of an arterial pulse. These various indicators provide for an indirect assessments of the presence of known error sources in pulse oximetry measurements, which include optical interference between the sensor and the tissue location; light modulation by other than the patient's pulsatile tissue bed; physical movement of the patient and improper tissue-to-sensor positioning. These additional signal quality indicators are described in further detail in a copending US patent application entitled: "SIGNAL QUALITY METRICS DESIGN FOR QUALIFYING DATA FOR A PHYSIOLOGICAL MONITOR," attorney docket 009103-017600US.

[0020] Fig. 2 is a block diagram 200 depicting the operation of the signal-quality-based selection of filter parameters in accordance with embodiments of the present invention. In one embodiment, the digital filter is a linear filter. For linear filter is chosen, the filter can have either a finite or an infinite impulse response. Alternately, the filter may be a non-linear filter. Inputs 202 are applied to the digital filter 204 and to a signal quality assessment subsystem 206 that assesses how noisy the inputs look. Subsystem 206 calculates various signal quality metrics and provides the information to the selection subsystem 208, which selects filter parameters according to the criteria calculated by the signal quality subsystem 206. Storage subsystem 210 interfaces with the subsystems 206 and 208 to store and provide signal quality metrics as well as filter parameters. In one embodiment, the selection of filter parameters is performed in real time, with the filter parameters being determined using current input samples.

[0021] In an alternate embodiment, the filter parameters are calculated using a buffer 212 of recent input samples. In addition, signal assessment criteria and filter parameters can also be held in storage 210 for reference or for use in the calculation of new values.

[0022] As set forth above, various signal quality indicators may be used to select filter parameters. Additionally, the selection of the filter parameters may be based on more than one signal quality indicator. Furthermore, the selection of the filter parameters may be based on the output of an algorithm that combines several signal quality indicators. In one embodiment in an oximeter sys-

tem, the variance in the raw saturation value is used to determine the filter's smoothing coefficients. In this embodiment, the selection is achieved by comparing the variance in the raw sat signal to several thresholds, and the filter's smoothing coefficients are selected depending on which range the variance falls in.

[0023] In an alternate embodiment in an oximeter system used for average pulse estimation, the filter parameter selection algorithm uses a combination of various signal quality metrics, Z to select values for filter coefficients for the digital filter, where

$$Z = w_1 * SQ1 + w_2 * SQ2 + w_3 * SQ3,$$

where

w_1 , w_2 , and w_3 are weighting factors

SQ1 is a measure of the variance in the raw saturation signal

SQ2 is a measure of the correlation between signals from different wavelengths

SQ3 is a measure of the skew of the derivative waveform

[0024] Yet alternately, instead of using Z to select the filter coefficients, a non-linear function of Z can be used to select a coefficient or coefficients for the filter. In operation, the selection algorithm may first be tuned before it is fully implemented in a particular diagnostics system. The tuning of the selection algorithm(s) may be done manually using heuristic approaches. Alternately, the selection algorithm may be tuned statistically, in a manner similar to training a neural network.

[0025] Embodiments of the present invention offer several advantages over conventional adaptive filtering. It is known that conventional adaptive filtering seeks to optimize some output criterion by continuously tuning the coefficients in a linear filter. The approach as embodied by the present invention is advantageous over conventional adaptive filtering for the following reasons. First, filter parameters in accordance with embodiments of the present invention are selected by switching among several preset or fixed values, rather than being varied or tuned continuously. By switching the parameters of the digital filter among fixed, preset values, the embodiments of the present invention provide for computational savings and simplicity of implementation. Second, the parameters of the digital filter are selected based upon an assessment of the input signal received by the filter rather than by comparing the filter's output with its input. This too, provides for computational savings and simplicity of implementation. Third, the filter need not be a linear filter, that is the filter is not required to be linear in its input-output relationship. Since the filter in accordance with embodiments of the present invention is not constrained to be linear, the filter's design can correspond more to

physiological than to mathematical requirements, as is the case with most conventional adaptive filtering schemes. This physiological-based filter parameter selection may be used to, for example, attenuate pulse amplitudes above a threshold, or respond more quickly to decreases than to increases in blood oxygen saturation. [0026] Accordingly, as will be understood by those of skill in the art, the present invention which is related to reducing noise effects in a system for measuring a physiological parameter, may be embodied in other specific forms without departing from the scope of the claims. For example, signals indicative of any physiological parameter other than oxygen saturation, such as pulse rate, blood pressure, temperature, or any other physiological variable could be filtered using the techniques of the present invention. Moreover, many other indicators of the quality of the input signal can be used as a basis for the selection of the filter's coefficients. Further, while the present embodiments have been described in the time-domain, frequency-based methods are equally relevant to the embodiments of the present invention. Accordingly, the foregoing disclosure is intended to be illustrative, but not limiting, of the scope of the invention, which is set forth in the following claims.

Claims

1. A method of reducing noise effects in a system for measuring a physiological parameter, comprising: receiving an input signal (202); obtaining an assessment of the signal quality of said input signal (206); selecting coefficients by switching among a plurality of stored discrete preset values (208) for a digital filter (204) using said assessment of signal quality, wherein the stored discrete preset values are fixed or non-changing values; and filtering said input signal using said digital filter (204), without comparing said filter's output signal with said input signal.
2. The method of claim 1, wherein said filtering comprises operating a digital filter (204) having a linear input-output relationship.
3. The method of claim 1, wherein said filtering comprises operating a digital filter (204) having a non-linear input-output relationship.
4. The method of claim 1 wherein said obtaining an assessment of said signal quality (206) comprises obtaining a measure of the skew of the time-derivative of the input signal.
5. The method according to any one of the preceding claims, wherein said receiving (202) comprises receiving input signals from more than one wavelength, and said obtaining an assessment of said signal quality (206) comprises obtaining a measure of the correlation between the signals from different wavelengths.
6. The method according to any one of the preceding claims, wherein said obtaining an assessment of said signal quality (206) comprises obtaining a measure of the variation in the amplitude of the input signal, a measure of the maximum value of the input signal, or a measure of the spectral peak frequency or frequencies of the input signal.
7. The method according to any one of the preceding claims, wherein said selecting (208) is performed in real time, with said coefficients of said digital filter being determined using a current input sample.
8. The method of any of claims 1 to 6, wherein said selecting (208) is performed using a previously stored input signal sample.
9. The method of claim 1 wherein said receiving (202) comprises receiving a signal from an oximeter, wherein said signal is a function of oxygen saturation or of a pulse rate.
10. An apparatus for reducing noise effects in a system for measuring a physiological parameter, comprising: means for receiving an input signal (114); means for obtaining an assessment of the signal quality of the input signal (122); means for selecting coefficients by switching among a plurality of stored discrete preset values (122) for a digital filter (138) using said assessment of signal quality, wherein the stored discrete preset values are fixed or non-changing values; and means for filtering said input signal using said digital filter (138), without comparing said filter's output signal with said input signal.
11. The apparatus of claim 10, wherein said means for filtering comprise a digital filter (138) having a linear input-output relationship.
12. The apparatus of claim 10, wherein said means for filtering comprise a digital filter (138) having a non-linear input-output relationship.
13. The apparatus according to any of claims 10 to 12, wherein said means for obtaining an assessment of said signal quality are configured to obtain a measure of the skew of the time-derivative of said input signal.
14. The apparatus according to any of claims 10 to 13, wherein said means for receiving are configured to receive input signals from more than one wavelength, and said means for obtaining an assessment of said signal quality obtain a measure of the correlation between said signals from different wave-

lengths.

15. The apparatus according to any of claims 10 to 14, wherein said means for obtaining an assessment of said signal quality (122) are configured to obtain a measure of the variation in the amplitude of said input signal, a measure of the maximum value of said input signal, or a measure of the spectral peak frequency or frequencies of said input signal.
16. The apparatus according to any of claims 10 to 15, wherein said means for selecting (122) are configured to select said coefficients in real time, with said coefficients for said digital filter (138) being determined using a current input sample.
17. The apparatus according to any of claims 10 to 16, wherein said means for selecting (122) are configured to select said coefficients using a previously stored input signal sample.
18. The apparatus according to any of claims 10 to 17 wherein said means for receiving (114) are configured to receive a signal from an oximeter, wherein said signal is a function of an oxygen saturation or a function of a pulse rate.
19. The apparatus of claim 18 wherein said means for receiving (114) are configured to receive signals corresponding to sensed optical energies from a plurality of wavelengths.

Patentansprüche

1. Verfahren zum Reduzieren von Rauscheffekten in einem System zur Messung eines physiologischen Parameters, umfassend: Empfangen eines Eingabesignals (202); Erhalten einer Bewertung der Signalqualität des eingegebenen Signals (206); Auswählen von Koeffizienten durch Umschalten zwischen einer Mehrzahl von gespeicherten diskreten voreingestellten Werten (208) für einen digitalen Filter (204) durch Verwenden der Bewertung der Signalqualität, wobei die gespeicherten diskreten voreingestellten Werte feste oder sich nicht ändernde Werte sind; und Filtern des Eingabesignals mittels des digitalen Filters (204), ohne das Filterausgabesignal mit dem Eingabesignal zu vergleichen.
2. Verfahren nach Anspruch 1, wobei das Filtern das Betreiben eines digitalen Filters (204) umfasst, welcher eine lineare Eingabe-Ausgabebeziehung aufweist.
3. Verfahren nach Anspruch 1, wobei das Filtern das Betreiben eines digitalen Filters (204) umfasst, welcher eine nicht-lineare Eingabe-Ausgabebeziehung

aufweist.

4. Verfahren nach Anspruch 1, wobei das Erhalten einer Bewertung der Signalqualität (206) das Erhalten einer Messung des Versatzes der zeitlichen Ableitung des Eingabesignals umfasst.
5. Verfahren nach einem der vorhergehenden Ansprüche, wobei das Empfangen (202) das Empfangen von Eingabesignalen von mehr als einer Wellenlänge umfasst, und das Erhalten einer Bewertung der Signalqualität (206) das Erhalten einer Messung der Korrelation zwischen den Signalen von unterschiedlichen Wellenlängen umfasst.
6. Verfahren nach einem der vorhergehenden Ansprüche, wobei das Erhalten einer Bewertung der Signalqualität (206) das Erhalten einer Messung der Änderung der Amplitude des Eingabesignals, einer Messung des maximalen Wertes des Eingabesignals, oder einer Messung der spektralen Spitzenfrequenz oder -frequenzen des Eingabesignals umfasst.
7. Verfahren nach einem der vorhergehenden Ansprüche, wobei das Auswählen (208) in Echtzeit ausgeführt wird, wobei die Koeffizienten des digitalen Filters mittels eines aktuellen Eingabemusters festgestellt werden.
8. Verfahren nach einem der Ansprüche 1 bis 6, wobei das Auswählen (208) mittels eines vorher gespeicherten Eingabesignalmusters ausgeführt wird.
9. Verfahren nach Anspruch 1, wobei das Empfangen (202) das Empfangen eines Signals von einem Oximeter umfasst, wobei das Signal eine Funktion der Sauerstoffsättigung oder einer Impulsrate ist.
10. Vorrichtung zum Reduzieren von Rauscheffekten in einem System zur Messung eines physiologischen Parameters, umfassend: Mittel zum Empfangen eines Eingabesignals (114); Mittel zum Erhalten einer Bewertung der Signalqualität des Eingabesignals (122); Mittel zum Auswählen von Koeffizienten mittels Umschalten zwischen einer Mehrzahl von gespeicherten diskreten voreingestellten Werten (122) für einen digitalen Filter (138), durch Verwendung der Bewertung der Signalqualität, wobei die gespeicherten diskreten voreingestellten Werte feste oder sich nicht ändernde Werte sind; und Mittel zum Filtern des Eingabesignals mittels des digitalen Filters (138), ohne das Filterausgabesignal mit dem Eingabesignal zu vergleichen.
11. Vorrichtung nach Anspruch 10, wobei die Mittel zum Filtern einen digitalen Filter (138) umfassen, welcher eine lineare Eingabe-Ausgabebeziehung aufweist.

12. Vorrichtung nach Anspruch 10, wobei die Mittel zum Filtern einen digitalen Filter (138) umfassen, welcher eine nicht lineare Eingabe-Ausgabebeziehung aufweist.
13. Vorrichtung nach einem der Ansprüche 10 bis 12, wobei die Mittel zum Erhalten einer Bewertung der Signalqualität ausgebildet sind, um eine Messung des Versatzes der zeitlichen Ableitung des Eingabesignals zu erhalten.
14. Vorrichtung nach einem der Ansprüche 10 bis 13, wobei die Mittel zum Empfangen ausgebildet sind, um Eingabesignale von mehr als einer Wellenlänge zu empfangen, und die Mittel zum Erhalten einer Bewertung der Signalqualität eine Messung der Korrelation zwischen den Signalen von unterschiedlichen Wellenlängen erhalten.
15. Vorrichtung nach einem der Ansprüche 10 bis 14, wobei die Mittel zum Erhalten einer Bewertung der Signalqualität (122) ausgebildet sind, um eine Messung einer Änderung der Amplitude des Eingabesignals, eine Messung des maximalen Wertes des Eingabesignals, oder eine Messung der spektralen Spitzenfrequenz oder -frequenzen des Eingabesignals zu erhalten.
16. Vorrichtung nach einem der Ansprüche 10 bis 15, wobei die Mittel zum Auswählen (122) ausgebildet sind, um die Koeffizienten in Echtzeit auszuwählen, wobei die Koeffizienten für den digitalen Filter (138) mittels eines aktuellen Eingabemusters festgestellt werden.
17. Vorrichtung nach einem der Ansprüche 10 bis 16, wobei die Mittel zum Auswählen (122) ausgebildet sind, um die Koeffizienten mittels eines vorher gespeicherten Eingabesignalmusters auszuwählen.
18. Vorrichtung nach einem der Ansprüche 10 bis 17, wobei die Mittel zum Empfangen (114) eingestellt sind, um ein Signal von einem Oximeter zu empfangen, wobei das Signal eine Funktion einer Sauerstoffsättigung oder einer Impulsrate ist.
19. Vorrichtung nach Anspruch 18, wobei die Mittel zum Empfangen (114) ausgebildet sind, um Signale zu empfangen, welche erfassten optischen Energien aus einer Mehrzahl von Wellenlängen entsprechen.
- Revendications**
1. Procédé de réduction d'effets de bruit dans un système permettant de mesurer un paramètre physiologique, comprenant les étapes consistant à : recevoir un signal d'entrée (202) ; obtenir une évaluation de la qualité de signal dudit signal d'entrée (206) ; sélectionner des coefficients par commutation entre une pluralité de valeurs prédéfinies discrètes stockées (208) pour un filtre numérique (204) en utilisant ladite évaluation de qualité de signal, les valeurs prédéfinies discrètes stockées représentant des valeurs fixes ou à caractère permanent ; et filtrer ledit signal d'entrée en utilisant ledit filtre numérique (204), sans comparer le signal de sortie dudit filtre avec ledit signal d'entrée.
2. Procédé selon la revendication 1, dans lequel ledit filtrage comprend une étape consistant à utiliser un filtre numérique (204) présentant une relation entrée-sortie linéaire.
3. Procédé selon la revendication 1, dans lequel ledit filtrage comprend une étape consistant à utiliser un filtre numérique (204) présentant une relation entrée-sortie non linéaire.
4. Procédé selon la revendication 1, dans lequel ladite obtention d'une évaluation de ladite qualité de signal (206) comprend une étape consistant à obtenir une mesure de l'étalement de la dérivée temporelle du signal d'entrée.
5. Procédé selon l'une quelconque des revendications précédentes, dans lequel ladite réception (202) comprend une étape consistant à recevoir des signaux d'entrée à partir de plus d'une longueur d'onde, et ladite obtention d'une évaluation de ladite qualité de signal (206) comprend une étape consistant à obtenir une mesure de la corrélation entre les signaux à partir de différentes longueurs d'onde.
6. Procédé selon l'une quelconque des revendications précédentes, dans lequel ladite obtention d'une évaluation de ladite qualité de signal (206) comprend une étape consistant à obtenir une mesure de la variation de l'amplitude du signal d'entrée, une mesure de la valeur maximale du signal d'entrée, ou une mesure de la ou des fréquence(s) de crête spectrale du signal d'entrée.
7. Procédé selon l'une quelconque des revendications précédentes, dans lequel ladite sélection (208) est mise en oeuvre en temps réel, lesdits coefficients dudit filtre numérique étant déterminés en utilisant un échantillon d'entrée actuelle.
8. Procédé selon l'une quelconque des revendications 1 à 6, dans lequel ladite sélection (208) est mise en oeuvre en utilisant un échantillon de signal d'entrée préalablement stocké.
9. Procédé selon la revendication 1, dans lequel ladite réception (202) comprend une étape consistant à

recevoir un signal en provenance d'un oxymètre, ledit signal étant fonction d'une saturation en oxygène ou d'un pouls.

10. Appareil permettant de réduire des effets de bruit dans un système permettant de mesurer un paramètre physiologique, comprenant : des moyens permettant de recevoir un signal d'entrée (114) ; des moyens permettant d'obtenir une évaluation de la qualité de signal du signal d'entrée (122) ; des moyens permettant de sélectionner des coefficients par commutation entre une pluralité de valeurs prédéfinies discrètes stockées (122) pour un filtre numérique (138) en utilisant ladite évaluation de qualité de signal, les valeurs prédéfinies discrètes stockées représentant des valeurs fixes ou à caractère permanent ; et des moyens permettant de filtrer ledit signal d'entrée en utilisant ledit filtre numérique (138), sans comparer le signal de sortie dudit filtre avec ledit signal d'entrée.
11. Appareil selon la revendication 10, dans lequel lesdits moyens de filtrage comprennent un filtre numérique (138) présentant une relation entrée-sortie linéaire.
12. Appareil selon la revendication 10, dans lequel lesdits moyens de filtrage comprennent un filtre numérique (138) présentant une relation entrée-sortie non linéaire.
13. Appareil selon l'une quelconque des revendications 10 à 12, dans lequel lesdits moyens d'obtention d'une évaluation de ladite qualité de signal sont configurés pour obtenir une mesure de l'étalement de la dérivée temporelle dudit signal d'entrée.
14. Appareil selon l'une quelconque des revendications 10 à 13, dans lequel lesdits moyens de réception sont configurés pour recevoir des signaux d'entrée à partir de plus d'une longueur d'onde, et lesdits moyens d'obtention d'une évaluation de ladite qualité de signal obtiennent une mesure de la corrélation entre lesdits signaux à partir de différentes longueurs d'onde.
15. Appareil selon l'une quelconque des revendications 10 à 14, dans lequel lesdits moyens d'obtention d'une évaluation de ladite qualité de signal (122) sont configurés pour obtenir une mesure de la variation de l'amplitude dudit signal d'entrée, une mesure de la valeur maximale dudit signal d'entrée, ou une mesure de la ou des fréquence(s) de crête spectrale dudit signal d'entrée.
16. Appareil selon l'une quelconque des revendications 10 à 15, dans lequel lesdits moyens de sélection (122) sont configurés pour sélectionner lesdits coef-
17. Appareil selon l'une quelconque des revendications 10 à 16, dans lequel lesdits moyens de sélection (122) sont configurés pour sélectionner lesdits coefficients en utilisant un échantillon de signal d'entrée préalablement stocké.
18. Appareil selon l'une quelconque des revendications 10 à 17, dans lequel lesdits moyens de réception (114) sont configurés pour recevoir un signal en provenance d'un oxymètre, ledit signal étant fonction d'une saturation en oxygène ou fonction d'un pouls.
19. Appareil selon la revendication 18, dans lequel lesdits moyens de réception (114) sont configurés pour recevoir des signaux correspondant à des énergies optiques détectées à partir d'une pluralité de longueurs d'onde.

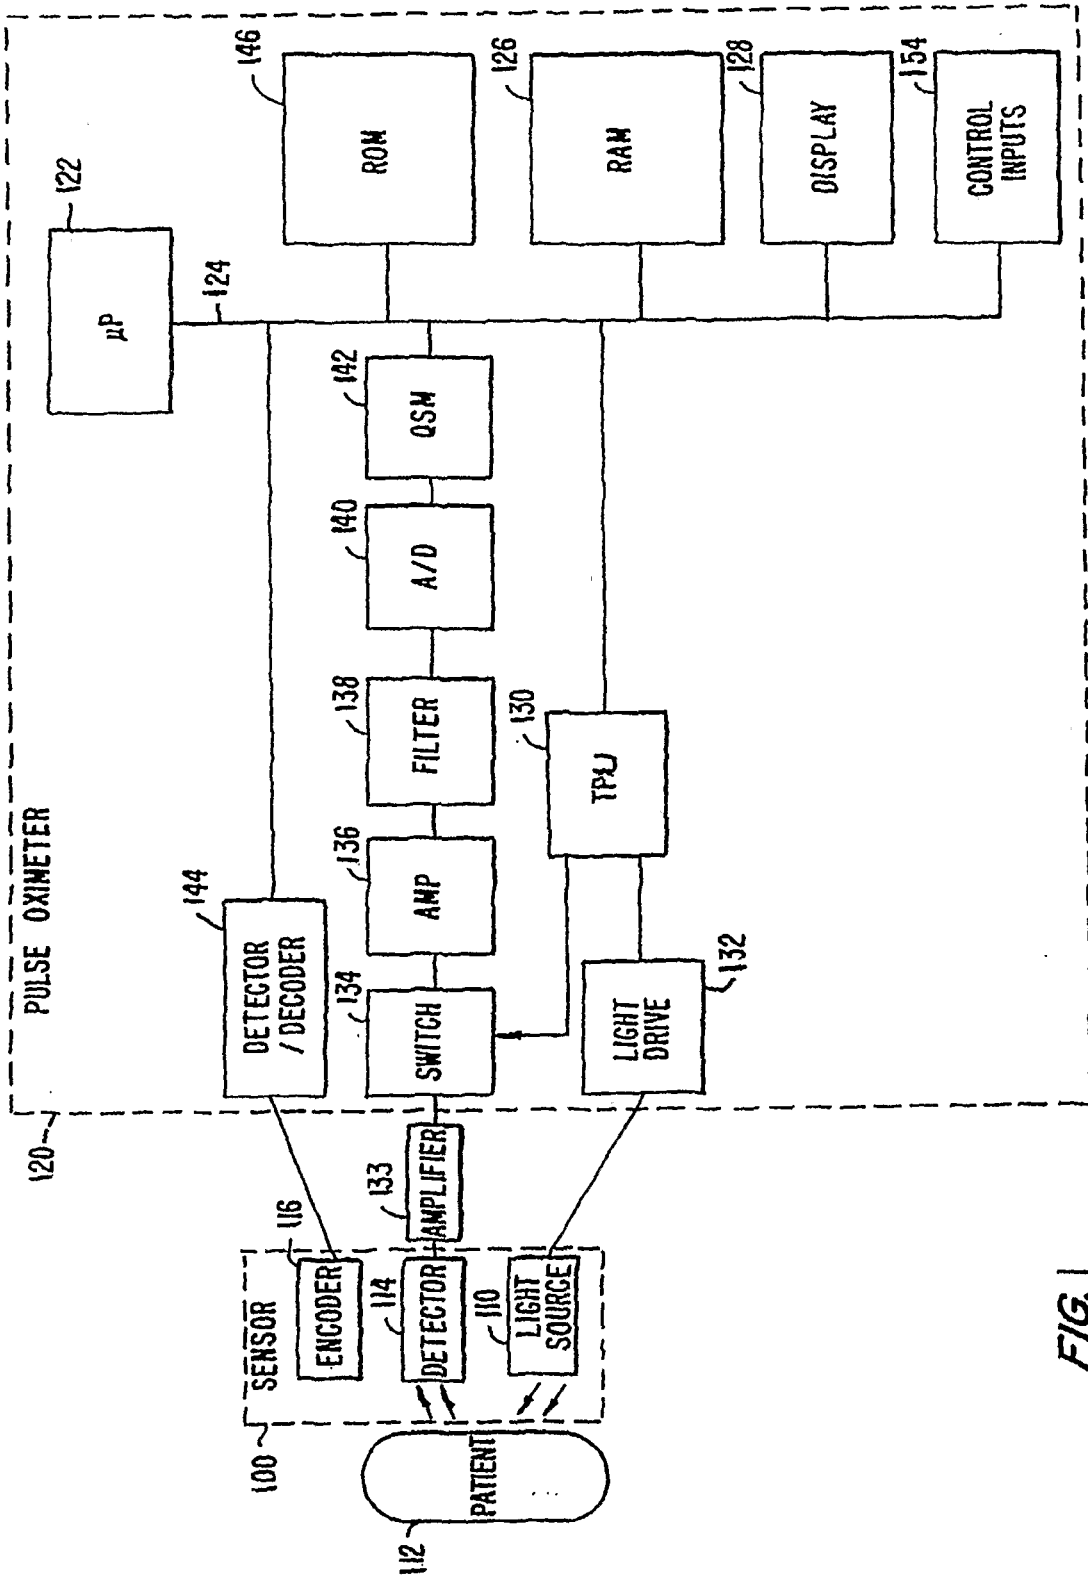


FIG. 1

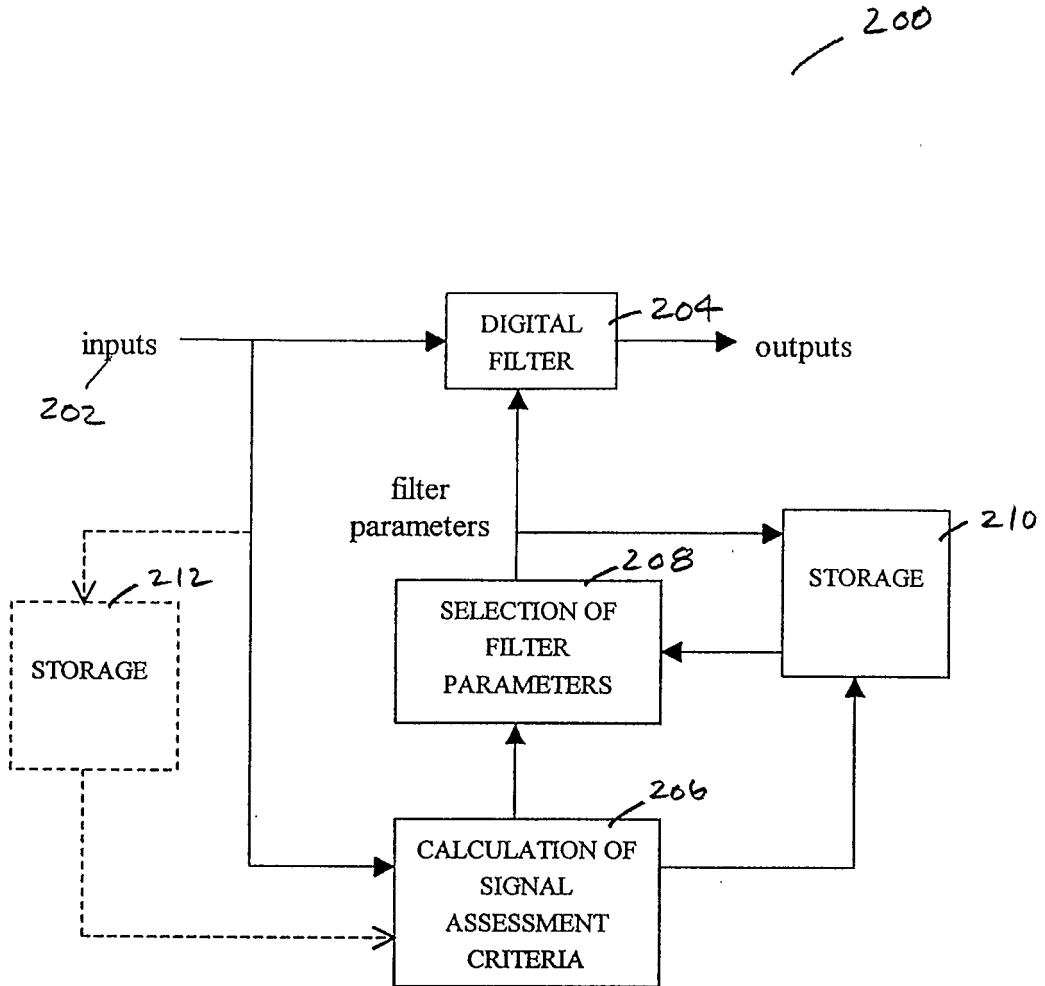


Fig. 2

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5853364 A [0002]
- US 4911167 A [0002]
- US 5645059 A [0002]
- US 6135952 A [0004]
- US 6721584 B [0004]

专利名称(译)	根据信号质量选择预设滤波器参数		
公开(公告)号	EP1586051B1	公开(公告)日	2016-04-13
申请号	EP2003800274	申请日	2003-12-29
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT INCORPORATED		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	STETSON PAUL F		
发明人	STETSON, PAUL, F.		
IPC分类号	G06F17/00 A61B5/00 A61B5/1455 A61B5/01 A61B5/021 A61B5/024 G06K9/00		
CPC分类号	A61B5/14551 A61B5/01 A61B5/021 A61B5/02416 A61B5/14552 A61B5/7203 A61B5/7221 A61B5/7239 A61B5/725 G06K9/00503		
优先权	10/341722 2003-01-13 US		
其他公开文献	EP1586051A1		
外部链接	Espacenet		

摘要(译)

用于降低用于测量生理参数的系统中的噪声影响的方法和设备，包括接收输入信号；获得输入信号的信号质量评估；使用信号质量评估选择数字滤波器的系数；并使用数字滤波器对输入信号进行滤波，而不将滤波器的输出信号与输入信号进行比较。

$$Z = w_1 * SQ1 + w_2 * SQ2 + w_3 * SQ3$$