

(19)



(11)

EP 3 171 777 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

18.12.2019 Bulletin 2019/51

(21) Application number: **15823957.4**

(22) Date of filing: **23.07.2015**

(51) Int Cl.:

A61B 5/11 (2006.01)	A61H 1/00 (2006.01)
A61H 1/02 (2006.01)	A61B 5/00 (2006.01)
A61B 5/0476 (2006.01)	A61B 5/0482 (2006.01)
A61B 5/22 (2006.01)	G06F 3/01 (2006.01)
G09B 9/06 (2006.01)	G09B 5/06 (2006.01)

(86) International application number:

PCT/SG2015/050227

(87) International publication number:

WO 2016/013980 (28.01.2016 Gazette 2016/04)

(54) **A METHOD AND SYSTEM FOR USING HAPTIC DEVICE AND BRAIN-COMPUTER INTERFACE FOR REHABILITATION**

VERFAHREN UND SYSTEM ZUR VERWENDUNG EINER HAPTISCHEN VORRICHTUNG UND GEHIRN-COMPUTER-SCHNITTSTELLE ZUR REHABILITATION

PROCÉDÉ ET SYSTÈME D'UTILISATION DE DISPOSITIF HAPTIQUE ET INTERFACE CERVEAU-ORDINATEUR POUR LA RÉÉDUCATION

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **23.07.2014 SG 10201404337Y**

(43) Date of publication of application:
31.05.2017 Bulletin 2017/22

(73) Proprietor: **Agency for Science, Technology and
Research
Singapore 138632 (SG)**

(72) Inventors:

- **ANG, Kai Keng
Singapore 138632 (SG)**
- **GUAN, Cuntai
Singapore 138632 (SG)**
- **PHUA, Kok Soon
Singapore 138632 (SG)**
- **ZHOU, Longjiang
Singapore 138632 (SG)**

- **WANG, Chuan Chu
Singapore 138632 (SG)**

(74) Representative: **Stöckeler, Ferdinand et al
Schoppe, Zimmermann, Stöckeler
Zinkler, Schenk & Partner mbB
Patentanwälte
Radtkoferstrasse 2
81373 München (DE)**

(56) References cited:

WO-A2-2005/074371	WO-A2-2005/074373
US-A1- 2008 300 521	US-A1- 2012 029 391
US-A1- 2013 138 011	US-A1- 2014 018 694

- **LAMBERCY, O. ET AL.: 'A Haptic Knob for
Rehabilitation of Hand Function' IEEE
TRANSACTIONS ON NEURAL SYSTEMS AND
REHABILITATION ENGINEERING vol. 15, no. 3,
01 September 2007, pages 356 - 366,
XP011192080 DOI: 10.1109/TNSRE.2007.903913**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description**PRIORITY CLAIM**

5 **[0001]** The present application claims priority to Singapore patent application 10201404337Y.

TECHNICAL FIELD

10 **[0002]** The following discloses a method and system for using a haptic device and a brain computer interface (BCI) for rehabilitation purposes. In particular, to rehabilitate stroke patients.

BACKGROUND ART

15 **[0003]** Haptic knobs with brain-computer interface (BCI) systems aid stroke patients with arm or hand paralysis in the rehabilitation process. BCI systems use electroencephalogram (EEG) based motor imagery to detect the patient's thinking abilities which control motor movement, while the haptic knob functions as a haptic-assisted device which specifically trains the opening/closing of the paralyzed hand with intensive repetitions.

20 **[0004]** Prior to the commencement of the rehabilitation, the mechanics of the haptic knob is usually calibrated by a therapist. This is an important step as this determines the movement or range of movement of the haptic knob when rehabilitating the stroke-affected or paralyzed hand. The therapist typically begins by manually moving the patient's stroke-affected hand to assess the range of movement the patient is capable of performing. Based on the results of this exercise, and applying his/her experience, the therapist then enter values into a computer to configure the haptic knob.

25 **[0005]** The drawback with this is that the calibration process is essentially a manual one, with the accuracy of the calibration largely determined on how experienced the therapist is. Further, it is prone to human error as the therapist would have to essentially translate the results of the exercise into calibration values. Any miscalibration of the haptic knob would have very undesirable results. An under-calibrated haptic knob will result in the rehabilitation exercises being largely ineffective as the range of motion of the patient's stroke-affected hand during the rehabilitation exercises will be under-stressed or under-taxed and as such, there would be little improvement on the patient's disability. On the other hand, an over-calibrated haptic knob will result in excruciating pain on the patient's part as his stroke-affected hand

30 **[0006]** Thus, there is a want for a method and system which is able to more effectively and more accurately calibrate the range of movement of the haptic knob.

35 **[0007]** Another drawback with current haptic knobs-BCI systems is that the assistive forces that the haptic knob applies, to aid the patient in moving the stroke-affected hand during the rehabilitation exercises, do not factor in the actual hand strength of a patient nor the patient's motor imagery score. In other words, the assistive force applied by the haptic knob is not cognizant of either the hand strength or motor imagery ability of the patient, which means that the assistive force is not tailored to the actual capability of the patient. Furthermore, when the hand strength used by a patient is excessive, current haptic knobs in the art do not provide a resistive force to restrict the movement of the stroke-affected hand to incite greater effort from the patient.

40 **[0008]** WO 2005/074373 A2 discloses a method of rehabilitation using an actuator type that includes a movement mechanism capable of applying a force that interacts with a motion of a patient's limb in a volume of at least 30 cm in diameter, in at least three degrees of freedom of motion of the actuator and capable of preventing substantial motion in any point in any direction in the volume. The method comprises exercising a patient at a first place of rehabilitation selected from a bed, a wheel-chair, a clinic and a home, using an actuator of the actuator type which interacts with a motion of the patient. The method further comprises exercising the patient at a second place of rehabilitation selected from a bed, a wheel-chair, a clinic and a home using a second actuator of the actuator type which interacts with a motion of the patient. The first exercising and the second exercising utilize a same movement mechanism design for moving the actuators.

50 **[0009]** Thus, there is a want for a haptic knob that is capable of applying an assistive force that takes into account the hand strength and motor imagery ability of the patient, and is also able to provide a resistive force as well during the rehabilitation exercises.

55 **[0010]** Furthermore, other desirable features and characteristics will become apparent from the subsequent detailed description and the appended claims, taken in conjunction with the accompanying drawings and this background of the disclosure.

SUMMARY OF INVENTION

[0011] The invention provides a system for calibrating a haptic device according to claim 1.

[0012] According to the invention, a system for calibrating and executing a rehabilitation exercise for a stroke-affected limb of a stroke patient is disclosed, the stroke patient having an able limb. The system comprises a haptic device, an interface, at least one sensor and a processor. Wherein the haptic device is capable of being manipulated by the able limb, in response to automated visual/audio instructions provided by the interface to guide the stroke patient in using the able limb to manipulate the haptic device to perform at least one calibration action, wherein the at least one sensor is configured to determine a first position of the haptic device, the first position resultant from the manipulation of the haptic device by the able limb in completing the at least one calibration action. Wherein the haptic device is also capable of being manipulated by the stroke-affected limb, in response to automated visual/audio instructions provided by the interface to guide the stroke patient in using the stroke-affected limb to manipulate the haptic device to perform the at least one calibration action; wherein the at least one sensor is configured to determine a second position of the haptic device, the second position resultant from the manipulation of the haptic device by the stroke-affected limb in completing the at least one calibration action. Wherein the haptic device is also capable of moving, coupled with the stroke-affected limb, from the second position towards the first position until a predetermined counterforce emanating from the stroke-affected limb is detected by the least one sensor, indicating an extreme position for the stroke-affected limb using the haptic device. Wherein the processor is configured to calibrate the haptic device with the extreme position such that during the rehabilitation exercise for the stroke-affected limb, the haptic device is prevented from moving beyond the extreme position. The haptic device is further capable of applying a force which is a function of a motor imagery score of the stroke patient, a limb strength of the stroke-affected limb and a maximum limb strength of the able limb. The force applied by the haptic device is represented by an equation

$$\alpha = -\tanh\left(\frac{5}{h_{max}}\left(h - \frac{h_{max}}{2}\right)\right)\tanh\left(\frac{5m}{m_{max}}\right),$$

wherein α is the force applied by the haptic device, h is the limb strength of the stroke-affected limb, h_{max} is the maximum limb strength of the able limb, m is the motor imagery score of the stroke patient, and m_{max} is a maximum motor imagery score.

[0013] Preferably, the haptic device is a robotic device and is shaped in the form of a glove or a knob.

[0014] Preferably, the at least one sensor comprises position encoders for providing position and orientation data of the haptic device.

[0015] Preferably, the system further comprises a brain computer interface (BCI) system, the BCI system configured to obtain electroencephalogram (EEG) data from the brain of the stroke patient, and determine from the EEG data a motor imagery score of the stroke patient.

[0016] Preferably, the haptic device is configured to execute the rehabilitation exercise by applying the force during the rehabilitation exercise for the stroke-affected limb.

[0017] Preferably, the force applied by the haptic device is an assistive force or a resistive force depending on the limb strength of the stroke-affected limb.

[0018] Preferably, the EEG data is used to compute a Temporal Spectral-dependent Brain Index (TSBI), and the TSBI is then plotted against Fugl-Meyer Score Improvement in a graph so as to predict the progress of stroke rehabilitation.

BRIEF DESCRIPTION OF THE DRAWINGS

[0019] The accompanying figures, where like reference numerals refer to identical or functionally similar elements throughout the separate views and which together with the detailed description below are incorporated in and form part of the specification, serve to illustrate various embodiments, by way of example only, and to explain various principles and advantages in accordance with a present embodiment.

[Figure 1] shows an illustration of a haptic device module in accordance with an embodiment of the invention.

[Figure 2(a)] shows an illustration of a finger flexion action and a finger extension action. [Figure 2(b)] shows an illustration of a forearm supination action and a forearm pronation action.

[Figure 3] is a flow chart depicting a method for calibrating a haptic device.

[Figure 4] is a flow chart depicting a method for calibrating a haptic device.

[Figure 5] is a flow chart depicting a method for calibrating a haptic device.

[Figure 6] shows an illustration of the range of movement for rehabilitating a finger on the patient's stroke-affected hand.

[Figure 7] shows an illustration of the range of movement for rehabilitating the patient's stroke-affected hand.

[Figure 8] illustrates a patient undergoing the rehabilitation exercises.

[Figure 9(a)] shows a graph of assistive force/resistive force applied by haptic device plotted against hand strength of stroke-affected hand. [Figure 9(b)] shows a graph of assistive force/resistive force applied by haptic device plotted against motor imagery score of the patient. [Figure 9(c)] shows a graph that plots the change in assistive force/resistive force applied by haptic device against motor imagery score of the patient and hand strength of stroke-affected hand.

[Figure 10] shows the locations of the channel electrodes on the brain.

[Figure 11] shows a graph of Temporal Spectral-dependent Brain Indexes (TSBI) plotted against Fugl-Meyer Score Improvement.

[0020] Skilled artisans will appreciate that elements in the figures are illustrated for simplicity and clarity and have not necessarily been depicted to scale. For example, the dimensions of some of the elements in the block diagrams or steps in the flowcharts may be exaggerated in respect to other elements to help improve understanding of the present embodiment.

DETAILED DESCRIPTION

[0021] The following detailed description is merely exemplary in nature and is not intended to limit the invention or the application and uses of the invention. Furthermore, there is no intention to be bound by any theory presented in the preceding background of the invention or the following detailed description. It is the intent of the preferred embodiments to disclose a method and system which is able to effectively and accurately calibrate the haptic device. Furthermore, the extreme positions for the stroke-affected hand when using the haptic device can be automatically and accurately determined, enhancing the effectiveness of the rehabilitation exercises and avoiding excruciating pain for the patient. The disclosed method and system is fully automated and does not rely on the manual calibration of a therapist which is subject to human error.

[0022] Further, in accordance with the present embodiments, during the execution of the rehabilitation exercises, the haptic device takes into account the maximum hand strength of the able hand, the hand strength of the stroke-affected hand and motor imagery ability of the patient when applying an assistive force as well as a resistive force during the rehabilitation exercises. Further still, in accordance with the present embodiments, the electroencephalogram (EEG) data can be used to predict the progress of the stroke rehabilitation. While exemplary embodiments have been presented in the foregoing detailed description of the invention, it should be appreciated that a vast number of variations exist.

[0023] Figure 1 illustrates a haptic device module 100 in accordance with an embodiment of the invention. The haptic device module 100 comprises processor 101, haptic device 102, sensors 103, memory 104 and visual/audio means 105. Processor 101 can provide instructions for controlling and moving haptic device 102. Haptic device 102 can be a robotic glove or robotic knob. Haptic device 102 can have actuators to supply a force. Haptic device 102 can be powered by a motor. Sensors 103 can be connected to haptic device 102. Sensors 103 can include position encoders which provide position/orientation data of haptic device 102. Sensors 103 can also include force sensors. Sensors 103 feed sensor data and position data into processor 101. Processor 101 can store position data into memory 104. Processor 101 can provide visual or audible instructions to the patient via visual/audio means 105. Visual/audio means 105 can be any display screen or any speaker or the like.

[0024] The method for calibrating haptic device 102 as disclosed involves a patient performing calibration actions. These calibration actions can include a finger flexion action, a finger extension action, a forearm supination action and a forearm pronation action. An illustration of a finger flexion action and a finger extension action is shown in figure 2(a) and an illustration of a forearm supination action and a forearm pronation action is shown in figure 2(b).

[0025] Figures 3, 4 and 5 are flow charts depicting a method for calibrating haptic device 102.

[0026] In step 301 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to place his/her able hand (un-paralyzed hand) on or within haptic device 102 such that the patient can manipulate haptic device 102 with his/her able hand.

[0027] In step 302 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to close, open his/her hand and assume a resting/static position, and rotate left, rotate right his/her forearm and then assume a resting/static position. The position data of these six positions is saved into memory 104 and this position data will be

the initial coordinates of the stroke-affected hand.

[0028] In step 303 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to perform a finger flexion action and a finger extension action with his/her able hand.

[0029] In step 304 of figure 3, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the position data resulting from the finger flexion action as f_a and the finger extension action as e_a into memory 104.

[0030] In step 305 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to perform a forearm pronation action and a forearm supination action with his/her able hand.

[0031] In step 306 of figure 3, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the forearm pronation action as p_a and the forearm supination action as s_a into memory 104.

[0032] In step 307 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to use his/her maximum strength to perform a finger flexion action and a finger extension action at a midpoint between position f_a and e_a with his/her able hand. The midpoint is a position where the patient's hand is at rest and not exerting any muscle force. It is not necessarily the half point between the maximum finger flexion and maximum finger extension. It is just the position whereby the patient's hand is comfortably relaxed and at rest. In essence, the patient is asked to exert maximum force with his able hand from a stationary position.

[0033] In step 308 of figure 3, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the maximum strength of the able hand in performing a finger flexion action and a finger extension action as $h_{max,1}$ into memory 104.

[0034] In step 309 of figure 3, processor 101 provides instructions to the patient via visual/audio means 105 to use his/her maximum strength to perform a forearm pronation action and a forearm supination action at a midpoint between position p_a and s_a with his/her able hand. The midpoint is a position where the patient's hand is at rest and not exerting any muscle force. It is not necessarily the half point between the maximum pronation and maximum supination. It is just the position whereby the patient's hand is comfortably relaxed and at rest.

[0035] In step 310 of figure 3, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the maximum strength of the able hand in performing a pronation and supination action as $h_{max,2}$ into memory 104.

[0036] It is to be noted that the manipulation of haptic device 102 by the patient through steps 301 to 310 is unassisted (no force is applied by haptic device 102) and is done entirely by the patient's able hand.

[0037] In step 401 of figure 4, processor 101 provides instructions to the patient via visual/audio means 105 to remove able hand and place his/her stroke-affected hand (paralyzed hand) on or within haptic device 102 such that the patient can manipulate haptic device 102 with his/her stroke-affected hand.

[0038] In step 402 of figure 4, processor 101 provides instructions to the patient via visual/audio means 105 to perform a finger flexion action and a finger extension action with his/her stroke-affected hand.

[0039] In step 403 of figure 4, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the finger flexion action as f_s and the finger extension action as e_s into memory 104.

[0040] In step 404 of figure 4, processor 101 provides instructions to the patient via visual/audio means 105 to perform a forearm pronation action and a forearm supination action with his/her stroke-affected hand.

[0041] In step 405 of figure 4, after the actions have been performed, processor 101 obtains the sensory data from sensors 103 and records the finger flexion action as p_s and the finger extension action as s_s into memory 104.

[0042] It is to be noted that the manipulation of haptic device 102 by the patient through steps 401 to 405 is unassisted (no force is applied by haptic device 102) and is done entirely by the patient's stroke-affected hand.

[0043] In step 501 of figure 5, processor 101 provides instructions to haptic device 102 to perform a finger flexion action from position f_s to position f_a (the patient's stroke-affected hand will move along with haptic device 102 as they are still coupled together at this juncture) until sensors 103 detect a counter-force as a result of the patient's stroke-affected hand resistance to movement. Preferably, the counterforce is larger than one quarter of the maximum strength of the able hand in performing a finger flexion action and a finger extension action $h_{max,1}$, i.e. counter force $> 0.25 h_{max,1}$.

[0044] In step 502 of figure 5, processor 101 obtains the sensory data from sensors 103 and records the position data resulting from the finger flexion action as f_p into memory 104. f_p therefore represents the extreme position in which the patient can flex his/her fingers with his/her stroke-affected hand without causing the patient excruciating pain and yet providing the necessary leeway for improvement in his/her stroke-affected hand.

[0045] In step 503 of figure 5, processor 101 provides instructions to haptic device 102 to perform a finger extension action from position e_s to position e_a (the patient's stroke-affected hand will move along with haptic device 102 as they are still coupled together at this juncture) until sensors 103 detect a counter-force as a result of the patient's stroke-affected hand resistance to movement. Preferably, the counterforce is larger than one quarter of the maximum strength of the able hand in performing a finger flexion action and a finger extension action $h_{max,1}$, i.e. counter force $> 0.25 h_{max,1}$.

[0046] In step 504 of figure 5, processor 101 obtains the sensory data from sensors 103 and records the position data resulting from the finger extension action as e_p into memory 104. e_p therefore represents the extreme position in which

the patient can extend his/her fingers with his/her stroke-affected hand without causing the patient excruciating pain and yet providing the necessary leeway for improvement in his/her stroke-affected hand.

[0047] In step 505 of figure 5, processor 101 provides instructions to haptic device 102 to perform a forearm pronation action from position p_s to position p_a (the patient's stroke-affected hand will move along with haptic device 102 as they are still coupled together at this juncture) until sensors 103 detect a counter-force as a result of the patient's stroke-affected hand resistance to movement. Preferably, the counterforce is larger than one quarter of the maximum strength of the able hand in performing a pronation and supination action $h_{max,2}$, i.e. counter force $> 0.25 h_{max,2}$.

[0048] In step 506 of figure 5, processor 101 obtains the sensory data from sensors 103 and records the position data resulting from the forearm pronation action as p_p into memory 104. p_p therefore represents the extreme position in which the patient can pronate his/her forearm with his/her stroke-affected hand without causing the patient excruciating pain and yet providing the necessary leeway for improvement in his/her stroke-affected hand.

[0049] In step 507 of figure 5, processor 101 provides instructions to haptic device 102 to perform a forearm supination action from position s_s to position s_a (the patient's stroke-affected hand will move along with haptic device 102 as they are still coupled together at this juncture) until sensors 103 detect a counter-force as a result of the patient's stroke-affected hand resistance to movement. Preferably, the counterforce is larger than one quarter of the maximum strength of the able hand in performing a pronation and supination action $h_{max,2}$, i.e. counter force $> 0.25 h_{max,2}$.

[0050] In step 508 of figure 5, processor 101 obtains the sensory data from sensors 103 and records the position data resulting from the forearm pronation supination as s_p into memory 104. s_p therefore represents the maximum position or extent in which the patient can supinate his/her forearm with his/her stroke-affected hand without causing the patient excruciating pain and yet providing the necessary leeway for improvement in his/her stroke-affected hand.

[0051] The range of movement to rehabilitate the fingers of the patient's stroke-affected hand is therefore determined i.e. f_p for the finger flexion action and e_p for the finger extension action. The range of movement to rehabilitate the fingers of the patient's stroke-affected hand is illustrated in figure 6. The range of movement to rehabilitate the patient's stroke-affected hand is therefore determined i.e. p_p for the pronation action and s_p for the supination action. The range of movement to rehabilitate the patient's stroke-affected hand is illustrated in figure 7.

[0052] Once memory 104 has stored f_p for the finger flexion action, e_p for the finger extension action, p_p for the pronation action and s_p for the supination action, haptic device 102 is successfully calibrated and configured for the patient. f_p , e_p , p_p and s_p represent the extreme positions for the stroke-affected hand when using haptic device 102 for the rehabilitation exercises. In other words, during the rehabilitation exercises, the haptic device 102 would not move beyond these extreme positions. These extreme positions represent the ideal upper limit for the rehabilitation exercises. Any position before or below these extreme positions mean that the stroke-affected hand still has room for improvement, while any position beyond these extreme positions will cause the patient excruciating pain. The calibration process is advantageous because it can automatically determine the extreme positions which haptic device 102 can assume when the patient undergoes the rehabilitation exercises.

[0053] The calibration process is also advantageous because it is automatic and does not require a therapist, thereby reducing manpower costs. Further, as the calibration process is computerized with sensors 103 providing the necessary feedback, this calibration process is not subject to human error. Furthermore, the calibration process is robust enough to accommodate patients with varying hand sizes as well as right handed and left handed individuals. Obviously, for varying hand sizes, the range of movement and extreme positions will be different.

[0054] After the calibration of haptic device 102, the patient can begin the rehabilitation exercises. Figure 8 illustrates a patient undergoing the rehabilitation exercises. Figure 8 shows an electroencephalogram (EEG) headset 801 on patient's 802 head. Patient's 802 stroke-affected hand is placed on or within haptic device 102. EEG headset 801 measures patient's 802 brain signals. The image of a moving hand is shown on screen 803. This image provides the visual cue for patient 802 to perform motor imagery i.e. imagining moving his stroke-affected hand. During this time, patient 802 is unable to move or manipulate haptic device 102 due to a resistive force being applied by a motor of haptic device 102.

[0055] Once motor imaginary is successfully detected, patient 802 can then perform the rehabilitation exercises which can include finger flexion, finger extension, forearm pronation and forearm supination exercises. To supplement these rehabilitation exercises, screen 803 can display a virtual simulation which mirrors the rehabilitation exercises being performed by patient 802.

[0056] Haptic device 102 executes or helps to execute the rehabilitation exercises by applying an assistive force or resistive force when necessary. This assistive force or resistive force is denoted as α . When α is a positive value (+ve), haptic device 102 provides an assistive force to aid patient 802 in performing the exercises. When α is a negative value (-ve), haptic device 102 provides a resistive force to prevent patient 802 from overexerting himself/herself during the exercises. Assistive force/resistive force α can be a function of the hand strength of stroke-affected hand h , maximum hand strength of the able hand h_{max} ($h_{max,1}$ if it is a finger flexion and extension exercise, and $h_{max,2}$ if it is a forearm pronation and supination exercise), motor imagery score m , and maximum motor imagery score m_{max} . m_{max} is typically 100. The reason why assistive/resistive force α is dependent on the maximum hand strength h_{max} is because different

patients have different hand strength. So instead of setting assistive force/resistive force α to a fixed value, it is advantageous to account for the varying hand strength of patients by making assistive force/resistive force α dependent on the hand strength of the patient 802. The maximum strength of patient's 802 stroke-affected hand is more or less the same as the maximum strength of his able hand. Therefore, the maximum strength of patient's 802 able hand is used as an approximation of the maximum strength of his stroke-affected hand.

[0057] Assistive force/resistive force α can therefore be presented as :

$$\alpha = -\tanh\left(\frac{5}{h_{max}}\left(h - \frac{h_{max}}{2}\right)\right)\tanh\left(\frac{5m}{m_{max}}\right)$$

[0058] Figure 9(a) shows a graph of assistive force/resistive force α applied by haptic device 102 plotted against hand strength of the stroke-affected hand h . The relationship between hand strength of the stroke-affected hand h and assistive force/resistive force α applied by haptic device 102 is that if patient 802 uses very little hand strength with his/her stroke-affected hand when performing the rehabilitation exercise, α becomes a positive value and haptic device 102 applies an assistive force α to aid patient 802 in the rehabilitation exercise.

[0059] However, if patient 802 applies a significant amount of hand strength with his/her stroke-affected hand when performing the rehabilitation exercise, α becomes a negative value and haptic device 102 applies a resistive force α to slow down the movement of patient 802 stroke-affected hand, thereby increasing the effort patient 802 has to exert on his/her stroke-affected hand during the rehabilitation exercise. This is advantageous as existing haptic systems provides only an assistive force, and not a resistive force. The haptic device 102 as described herein therefore contemplates a scenario where patient 802 may be able to move his/her stroke-affected hand, which in this case the haptic device 102 applies a resistive force α and moving against this resistive force helps patient 802 to gain further strength on the stroke-affected hand. In other words, if patient 802 is capable of moving his/her stroke-affected hand, one of the objectives of the rehabilitation exercises would be to make patient 802 exert even more force. Therefore, a resistive force is applied so that patient 802 can be trained to exert even more effort. This is similar in concept to weight training. Once a person can move a certain amount of weights, the training will progress on to heavier weights.

[0060] Figure 9(b) shows a graph of assistive force/resistive force α applied by haptic device 102 plotted against motor imagery score m . A low motor imagery score means that patient 802 is unable to properly imagine or visualize moving his/her stroke-affected hand while a high motor imagery score means that patient 802 is able to properly imagine or visualize moving his/her stroke-affected hand. Motor imagery score m and assistive force α have a directly proportional relationship in that the higher the motor imagery score m obtained by patient 802, the greater the assistive force α applied by haptic device 102 to aid patient 802 in the exercise. This is advantageous because the better patient 802 can visualize moving his/her stroke-affected hand (i.e. higher motor imagery score), the further patient 802 can push or extend himself/herself during the rehabilitation exercises. Therefore, haptic device 102 applies a larger assistive force α to increase the speed of movement during the rehabilitation exercises. The disability of patient 802 is usually tied to his/her volition, willpower and effort. The more involved a patient is, or the more effort the patient imagines the motor imagery, the more assistive movement is provided to make the intensity of the rehabilitation exercises coincide with the effort put forth. The invention therefore capitalizes on the correlation between effort and the intensity of the rehabilitation exercises to enhance the effectiveness of the rehabilitation process.

[0061] Figure 9(c) shows a graph that plots the change in assistive force/resistive force α against motor imagery score m and hand strength h .

[0062] The hand strength of the stroke-affected hand h exerted by patient 802 when performing the rehabilitation exercises can be evaluated by measuring the force applied to sensors 103. However, sometimes sensors 103 can be cumbersome due to the additional wiring. Therefore preferably, hand strength of the stroke-affected hand h is measured by measuring the driving motor current necessary to maintain the same servo motor position. The linear relationship between the applied force F and the driving motor current I is given by :

$$I = kcF + I_0,$$

and therefore

$$F = \frac{I - I_0}{kc},$$

where k is the transferring factor of the applied to the analogous current output of the motor for hand grasping movement, c is the conversion factor of the analog-to-digital (AD) convertor of the driving motor, and I_0 is a constant caused by inertia and friction of the mechanism.

[0063] Therefore, the hand strength of the stroke-affected hand applied during the rehabilitation exercises is therefore :

$$F_i = \frac{1}{n} \sum_{j=1}^n F_{i,j}$$

where F_i is the average hand strength of the stroke-affected hand for the i^{th} rehabilitation exercise, $F_{i,j}$ is the actively evaluated hand strength of the stroke-affected hand for the j^{th} rehabilitation exercise.

[0064] In another embodiment of the invention, the EEG data collected during the rehabilitation exercises can be used to compute the Temporal Spectral-dependent Brain Index (TSBI). TSBI can be computed using the following equation:

$$TSBI(t) = \frac{1}{n_k} \sum_{n=k_1}^{k_2} \left| \frac{R_n^*(t) - L_n^*(t)}{R_n^*(t) + L_n^*(t)} \right|,$$

where

$$R_n^*(t) = \frac{1}{n_c} \sum_{c=1}^{n_c} a_n^2(c, t)$$

evaluates the averaged Fourier coefficient of eleven channel electrodes 1001 taken from the right hemisphere of the brain as shown in figure 10 (i.e. $n_c = 11$);

and where

$$L_n^*(t) = \frac{1}{n_c} \sum_{c=1}^{n_c} a_n^2(c, t)$$

evaluates the averaged Fourier coefficient of eleven channel electrodes 1002 taken from the left hemisphere of the brain as shown in figure 10 (i.e. $n_c = 11$);

and where

$$a_n(c, t)$$

is the Fourier coefficient of index n of channel electrode c evaluated at time t that corresponds to a particular time segment $[t-T, t]$, with T being the duration in which the motor imagery is being performed;

and where the Fourier coefficients $[k_1$ and $k_2]$ corresponds to the frequency band $[4-40 \text{ Hz}]$ evaluated by the brain-computer interface (BCI) for performing motor imagery, and n_k is the number of Fourier coefficients evaluated that correspond to the frequency band $[4-40 \text{ Hz}]$.

[0065] Preferably, TSBI can be used as a prognostic measure to predict the possible outcome of the rehabilitation. When TSBI are plotted against Fugl-Meyer Score Improvement, the results show that a lower TSBI resulted in a higher Fugl-Meyer Score Improvement. See figure 11 which plots a graph of TSBI calculated using motor imagery (MI) against Fugl-Meyer Score Improvement. Therefore, this shows that TSBI can be used to predict the progress of stroke rehabilitation.

[0066] Although all the embodiments of the invention have been described with the rehabilitation of a stroke-affected hand, forearm or wrist, one skilled in the art will appreciate that the invention can be applied to rehabilitate other stroke-affected limbs, for example, a stroke-affected leg.

[0067] It should further be appreciated that the exemplary embodiments are only examples, and are not intended to

limit the scope, applicability, operation, or configuration of the invention in any way. Rather, the foregoing detailed description will provide those skilled in the art with a convenient road map for implementing an exemplary embodiment of the invention, it being understood that various changes may be made in the function and arrangement of elements and method of operation described in an exemplary embodiment without departing from the scope of the invention as set forth in the appended claims.

Claims

1. A system for calibrating a haptic device (102) for a stroke-affected limb of a stroke patient (802), the stroke patient having an able limb, the system comprising the haptic device, an interface (105), at least one sensor (103) and a processor (101); wherein the haptic device is capable of:

being manipulated by the able limb, in response to automated visual/audio instructions provided by the interface to guide the stroke patient in using the able limb to manipulate the haptic device to perform at least one calibration action, wherein the at least one sensor is configured to determine a first position of the haptic device, the first position resultant from the manipulation of the haptic device by the able limb in completing the at least one calibration action;

being manipulated by the stroke-affected limb, in response to automated visual/audio instructions provided by the interface to guide the stroke patient in using the stroke-affected limb to manipulate the haptic device to perform the at least one calibration action; wherein the at least one sensor is configured to determine a second position of the haptic device, the second position resultant from the manipulation of the haptic device by the stroke-affected limb in completing the at least one calibration action; and

moving, coupled with the stroke-affected limb, from the second position towards the first position until a predetermined counterforce emanating from the stroke-affected limb is detected by the least one sensor, indicating an extreme position for the stroke-affected limb using the haptic device; and

wherein the processor is configured to calibrate the haptic device with the extreme position such that during a rehabilitation exercise for the stroke-affected limb, the haptic device is prevented from moving beyond the extreme position,

wherein the haptic device is **characterized by**:

being further capable of applying a force which is a function of a motor imagery score of the stroke patient, a limb strength of the stroke-affected limb and a maximum limb strength of the able limb, wherein the force applied by the haptic device is represented by an equation

$$\alpha = -\tanh\left(\frac{5}{h_{max}}\left(h - \frac{h_{max}}{2}\right)\right)\tanh\left(\frac{5m}{m_{max}}\right),$$

wherein α is the force applied by the haptic device, h is the limb strength of the stroke-affected limb, h_{max} is the maximum limb strength of the able limb, m is the motor imagery score of the stroke patient, and m_{max} is a maximum motor imagery score.

2. The system of claim 1 wherein the haptic device is a robotic device and is shaped in the form of a glove or a knob.
3. The system of claim 1 wherein the at least one sensor comprises position encoders for providing position and orientation data of the haptic device.
4. The system of claim 1 further comprising a brain computer interface (BCI) system, the BCI system configured to obtain electroencephalogram (EEG) data from a brain of the stroke patient, and determine from the EEG data the motor imagery score of the stroke patient; wherein optionally the haptic device is configured to execute the rehabilitation exercise by applying the force during the rehabilitation exercise for the stroke-affected limb, wherein the force is a function of the motor imagery score of the stroke patient, the limb strength of the stroke-affected limb and the maximum limb strength of the able limb; wherein optionally the force applied by the haptic device is an assistive force or a resistive force depending on the limb strength of the stroke-affected limb;

wherein optionally the EEG data is used to compute a Temporal Spectral-dependent Brain Index (TSBI), and the TSBI is then plotted against Fugl-Meyer Score Improvement in a graph so as to predict progress of stroke rehabilitation.

Patentansprüche

1. Ein System zum Kalibrieren einer haptischen Vorrichtung (102) für ein vom Schlaganfall betroffenes Glied eines Schlaganfallpatienten (802), wobei der Schlaganfallpatient ein unversehrtes Glied aufweist, wobei das System die haptische Vorrichtung, eine Schnittstelle (105), zumindest einen Sensor (103) und einen Prozessor (101) aufweist; wobei die haptische Vorrichtung in der Lage ist:

durch das unversehrte Glied manipuliert zu werden, ansprechend auf automatisierte visuelle Anweisungen/Audioanweisungen, die durch die Schnittstelle bereitgestellt werden, um den Schlaganfallpatienten beim Verwenden des unversehrten Glieds zu führen, um die haptische Vorrichtung dahin gehend zu manipulieren, zumindest eine Kalibrierungsmaßnahme durchzuführen, wobei der zumindest eine Sensor dazu konfiguriert ist, eine erste Position der haptischen Vorrichtung zu bestimmen, wobei die erste Position aus der Manipulation der haptischen Vorrichtung durch das unversehrte Glied beim Abschließen der zumindest einen Kalibrierungsmaßnahme resultiert;

durch das vom Schlaganfall betroffene Glied manipuliert zu werden, ansprechend auf automatisierte visuelle Anweisungen/Audioanweisungen, die durch die Schnittstelle bereitgestellt werden, um den Schlaganfallpatienten beim Verwenden des vom Schlaganfall betroffenen Glieds zu führen, um die haptische Vorrichtung dahin gehend zu manipulieren, die zumindest eine Kalibrierungsmaßnahme durchzuführen; wobei der zumindest eine Sensor dazu konfiguriert ist, eine zweite Position der haptischen Vorrichtung zu bestimmen, wobei die zweite Position aus der Manipulation der haptischen Vorrichtung durch das vom Schlaganfall betroffene Glied beim Abschließen der zumindest einen Kalibrierungsmaßnahme resultiert; und

sich, gekoppelt mit dem vom Schlaganfall betroffenen Glied, von der zweiten Position zu der ersten Position zu bewegen, bis eine vorbestimmte Gegenkraft, die von dem vom Schlaganfall betroffenen Glied ausgeht, durch den zumindest einen Sensor erfasst wird, wodurch eine extreme Position für das vom Schlaganfall betroffene Glied, das die haptische Vorrichtung verwendet, angezeigt wird; und

wobei der Prozessor dazu konfiguriert ist, die haptische Vorrichtung mit der extremen Position derart zu kalibrieren, dass während einer Rehabilitationsübung für das vom Schlaganfall betroffene Glied die haptische Vorrichtung daran gehindert wird, sich über die extreme Position hinaus zu bewegen,

wobei die haptische Vorrichtung **dadurch gekennzeichnet ist, dass:**

dieselbe eine Kraft ausüben kann, die von einer Bewertung der motorischen Vorstellungen des Schlaganfallpatienten, einer Gliedstärke des vom Schlaganfall betroffenen Glieds und einer maximalen Gliedstärke des unversehrten Glieds abhängig ist,

wobei die Kraft, die durch die haptische Vorrichtung ausgeübt wird, durch eine Gleichung dargestellt wird:

$$\alpha = -\tanh\left(\frac{5}{h_{\max}}\left(h - \frac{h_{\max}}{2}\right)\right)\tanh\left(\frac{5m}{m_{\max}}\right),$$

wobei α die Kraft ist, die durch die haptische Vorrichtung ausgeübt wird, h die Gliedstärke des vom Schlaganfall betroffenen Glieds ist, $h_{\max}$ die maximale Gliedstärke des unversehrten Glieds ist, m die Bewertung der motorischen Vorstellungen des Schlaganfallpatienten ist und $m_{\max}$ eine maximale Bewertung der motorischen Vorstellungen ist.

2. Das System gemäß Anspruch 1, bei dem die haptische Vorrichtung eine Robotervorrichtung ist und in Gestalt eines Handschuhs oder eines Bedienungsknopfs gebildet ist.
3. Das System gemäß Anspruch 1, bei dem der zumindest eine Sensor Stellungsgeber zum Bereitstellen von Positions- und Ausrichtungsdaten der haptischen Vorrichtung aufweist.
4. Das System gemäß Anspruch 1, das ferner ein Gehirn-Computer-Schnittstelle(BCI)-System aufweist, wobei das BCI-System dazu konfiguriert ist, Elektroenzephalogramm(EEG)-Daten von dem Gehirn eines Schlaganfallpatienten zu erhalten und aus den EEG-Daten die Bewertung der motorischen Vorstellungen des Schlaganfallpatienten zu

bestimmen;

wobei optional die haptische Vorrichtung dazu konfiguriert ist, die Rehabilitationsübung auszuführen, indem während der Rehabilitationsübung für das vom Schlaganfall betroffene Glied die Kraft ausgeübt wird, wobei die Kraft von der Bewertung der motorischen Vorstellungen des Schlaganfallpatienten, der Gliedstärke des vom Schlaganfall betroffenen Glieds und der maximalen Gliedstärke des unversehrten Glieds abhängig ist;

wobei optional die Kraft, die durch die haptische Vorrichtung ausgeübt wird, eine Unterstützungskraft oder eine Widerstandskraft ist, die von der Gliedstärke des vom Schlaganfall betroffenen Glieds abhängt;

wobei optional die EEG-Daten dazu verwendet werden, einen Temporal-Spektralabhängiger-Gehirn-Index (TSBI) zu berechnen, und der TSBI anschließend grafisch hinsichtlich einer Fugl-Meyer-Score-Verbesserung in einer Grafik dargestellt wird, um den Fortschritt einer Schlaganfallrehabilitation zu veranschaulichen.

Revendications

1. Système pour étalonner un dispositif haptique (102) pour un membre affecté par un accident vasculaire cérébral d'un patient ayant subi un accident vasculaire cérébral (802), le patient ayant subi un accident vasculaire cérébral présentant un membre non affecté, le système comprenant le dispositif haptique, une interface (105), au moins un capteur (103) et un processeur (101); dans lequel le dispositif haptique est à même de:

être manipulé par le membre non affecté, en réponse aux instructions visuelles/audio automatisées fournies par l'interface pour guider le patient ayant subi un accident vasculaire cérébral dans l'utilisation du membre non affecté pour manipuler le dispositif haptique pour réaliser au moins une action d'étalonnage, où l'au moins un capteur est configuré pour déterminer une première position du dispositif haptique, la première position résultant de la manipulation du dispositif haptique par le membre non affecté pour réaliser l'au moins une action d'étalonnage;

être manipulé par le membre affecté par l'accident vasculaire cérébral, en réponse aux instructions visuelles/sonores automatisées fournies par l'interface pour guider le patient ayant subi un accident vasculaire cérébral dans l'utilisation du membre affecté par l'accident vasculaire cérébral pour manipuler le dispositif haptique pour réaliser l'au moins une action d'étalonnage; où l'au moins un capteur est configuré pour déterminer une deuxième position du dispositif haptique, la deuxième position résultant de la manipulation du dispositif haptique par le membre affecté par l'accident vasculaire cérébral pour réaliser l'au moins une action d'étalonnage; et

se déplacer, couplé au membre affecté par l'accident vasculaire cérébral, de la deuxième position vers la première position jusqu'à ce qu'une contre-force prédéterminée émanant du membre affecté par l'accident vasculaire cérébral soit détectée par l'au moins un capteur, indiquant une position extrême pour le membre affecté par l'accident vasculaire cérébral à l'aide du dispositif haptique; et

dans lequel le processeur est configuré pour étalonner le dispositif haptique avec la position extrême de sorte que, pendant un exercice de rééducation du membre affecté par un accident vasculaire cérébral, le dispositif haptique soit empêché de se déplacer au-delà de la position extrême, dans lequel le dispositif haptique est **caractérisé par** le fait de:

être par ailleurs à même d'appliquer une force qui est fonction du score d'imagerie motrice du patient ayant subi un accident vasculaire cérébral, une force du membre affecté par un accident vasculaire cérébral et une force maximale du membre non affecté,

dans lequel la force appliquée par le dispositif haptique est représentée par une équation

$$\alpha = -\tanh\left(\frac{5}{h_{max}}\left(h - \frac{h_{max}}{2}\right)\right)\tanh\left(\frac{5m}{m_{max}}\right),$$

où α est la force appliquée par le dispositif haptique, h est la force du membre affecté par un accident vasculaire cérébral, h_{max} est la force maximale du membre non affecté, m est le score d'imagerie motrice du patient ayant subi un accident vasculaire cérébral, et m_{max} est un score d'imagerie motrice maximum.

2. Système selon la revendication 1, dans lequel le dispositif haptique est un dispositif robotique et présente la forme d'un gant ou d'un bouton.

3. Système selon la revendication 1, dans lequel l'au moins un capteur comprend des codeurs de position destinés à fournir les données de position et d'orientation du dispositif haptique.
4. Système selon la revendication 1, comprenant par ailleurs un système d'interface cerveau-ordinateur (BCI), le système BCI étant configuré pour obtenir les données d'électroencéphalogramme (EEG) d'un cerveau du patient ayant subi un accident vasculaire cérébral et pour déterminer, à partir des données d'EEG, le score d'imagerie motrice du patient ayant subi un accident vasculaire cérébral;
 dans lequel, optionnellement, le dispositif haptique est configuré pour exécuter l'exercice de rééducation en appliquant la force pendant l'exercice de rééducation pour le membre affecté par l'accident vasculaire cérébral, où la force est fonction du score d'imagerie motrice du patient ayant subi un accident vasculaire cérébral, de la force du membre affecté par l'accident vasculaire cérébral et de la force maximale du membre non affecté;
 dans lequel, optionnellement, la force appliquée par le dispositif haptique est une force d'assistance ou une force de résistance en fonction de la force du membre affecté par l'accident vasculaire cérébral;
 dans lequel, optionnellement, les données d'EEG sont utilisées pour calculer un Indice Cérébral dépendant du Spectre Temporel (TSBI), et le TSBI est alors tracé en fonction de l'Amélioration du Score de Fugl-Meyer dans un graphique de manière à prédire le progrès de la rééducation après un accident vasculaire cérébral.

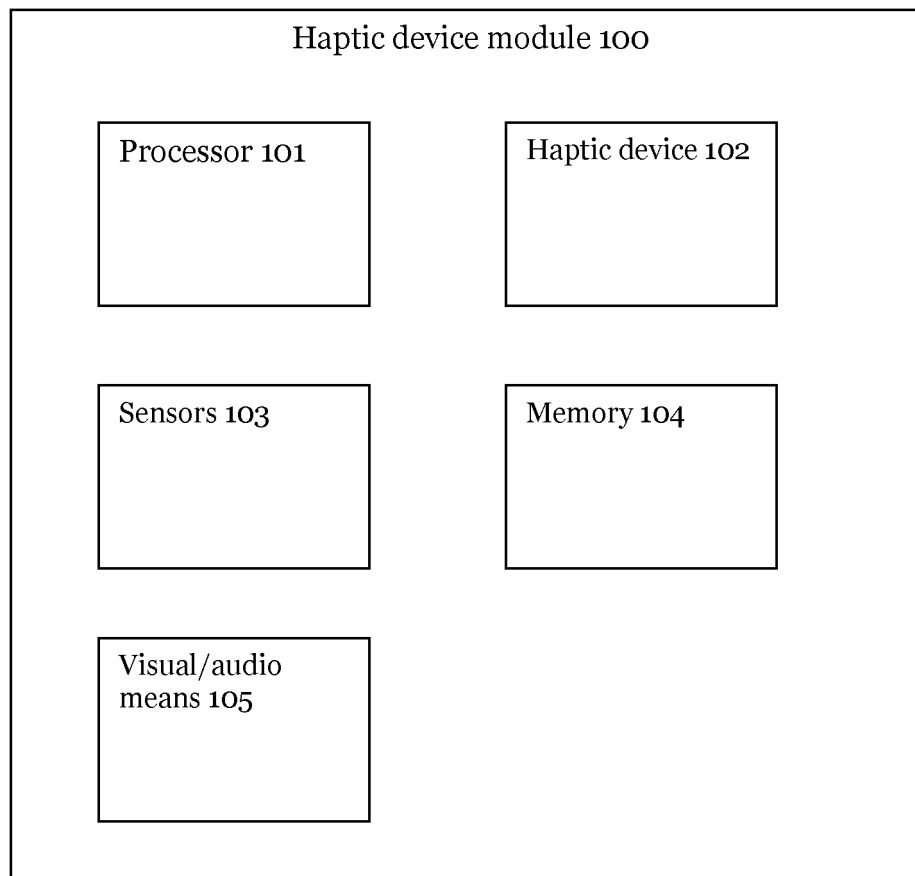


Figure 1

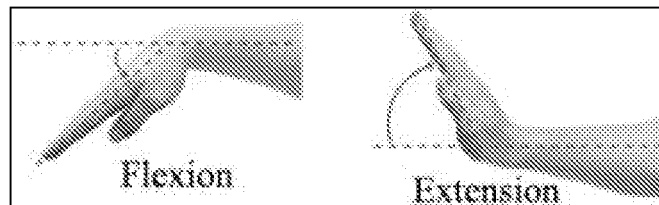


Figure 2(a)

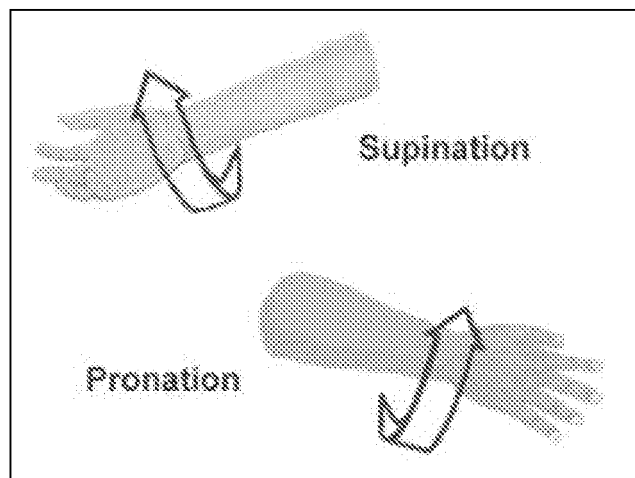


Figure 2(b)

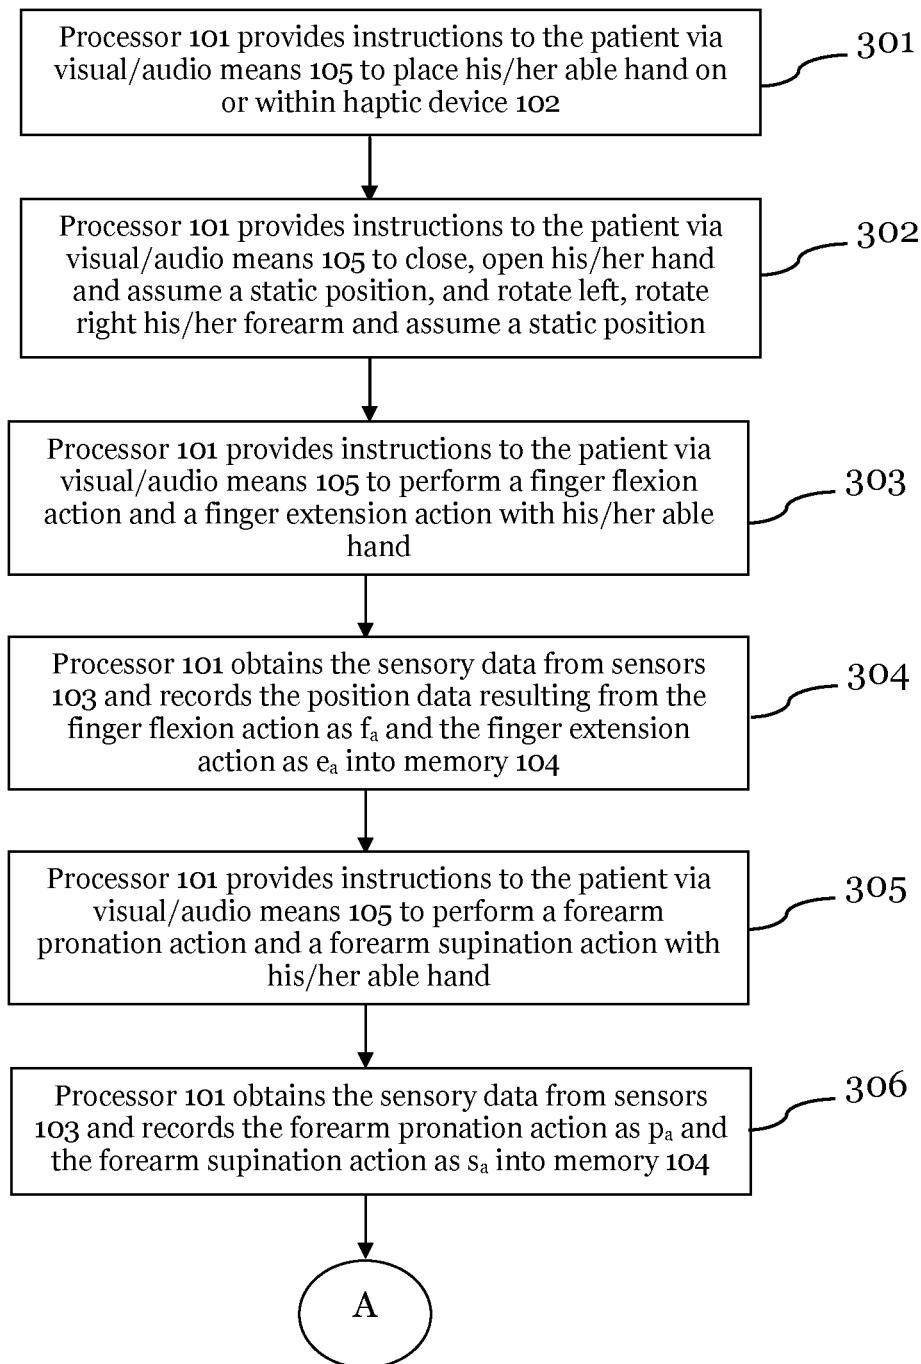


Figure 3

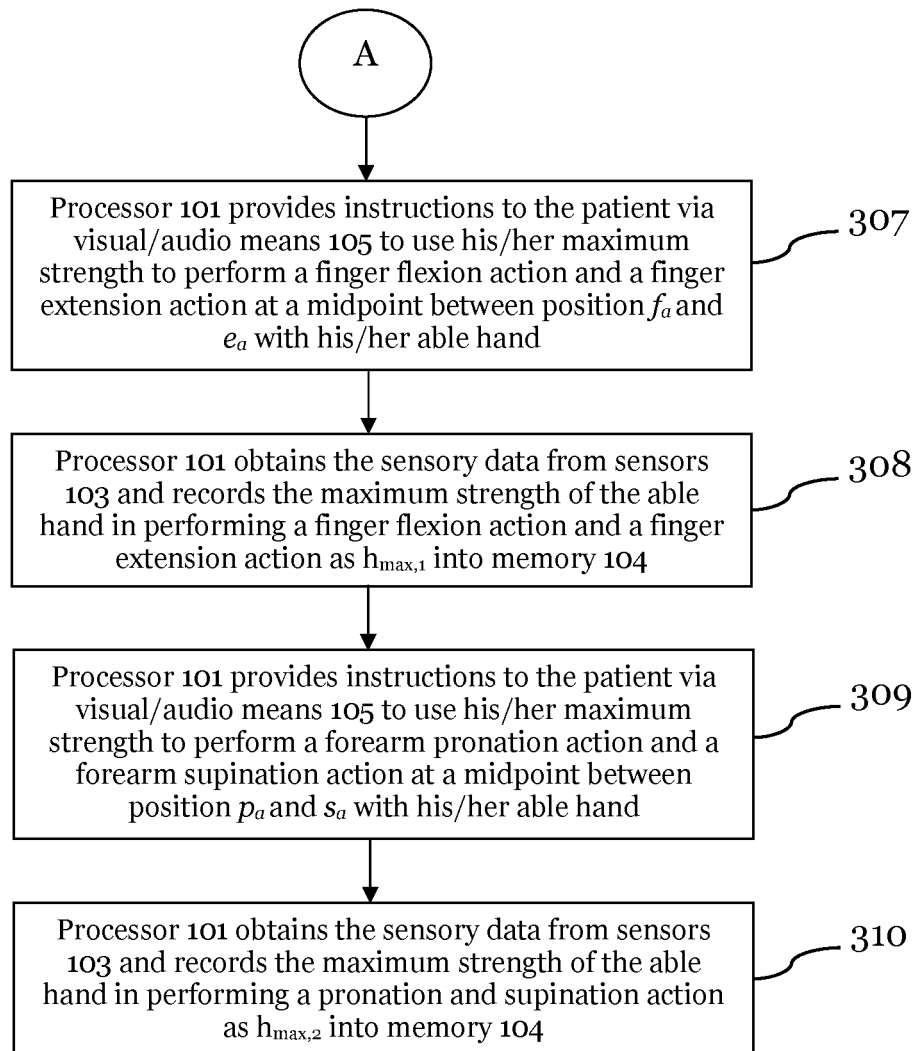


Figure 3
(continued)

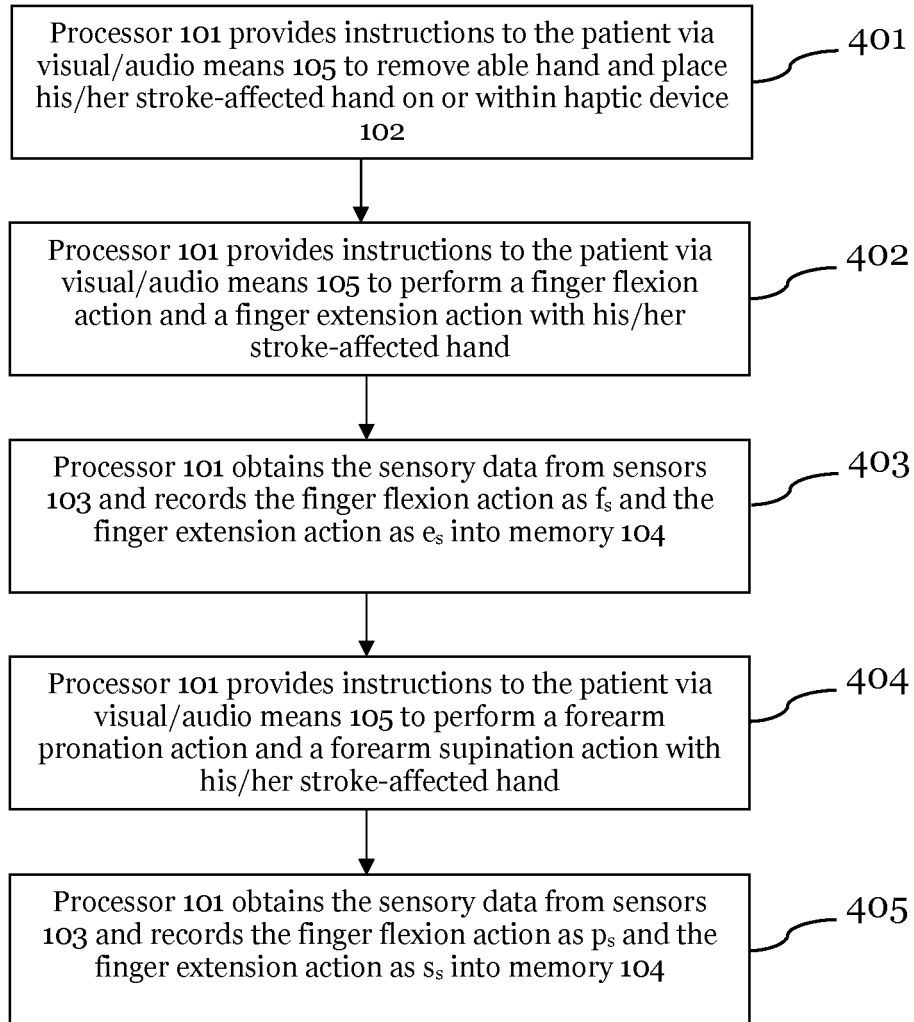


Figure 4

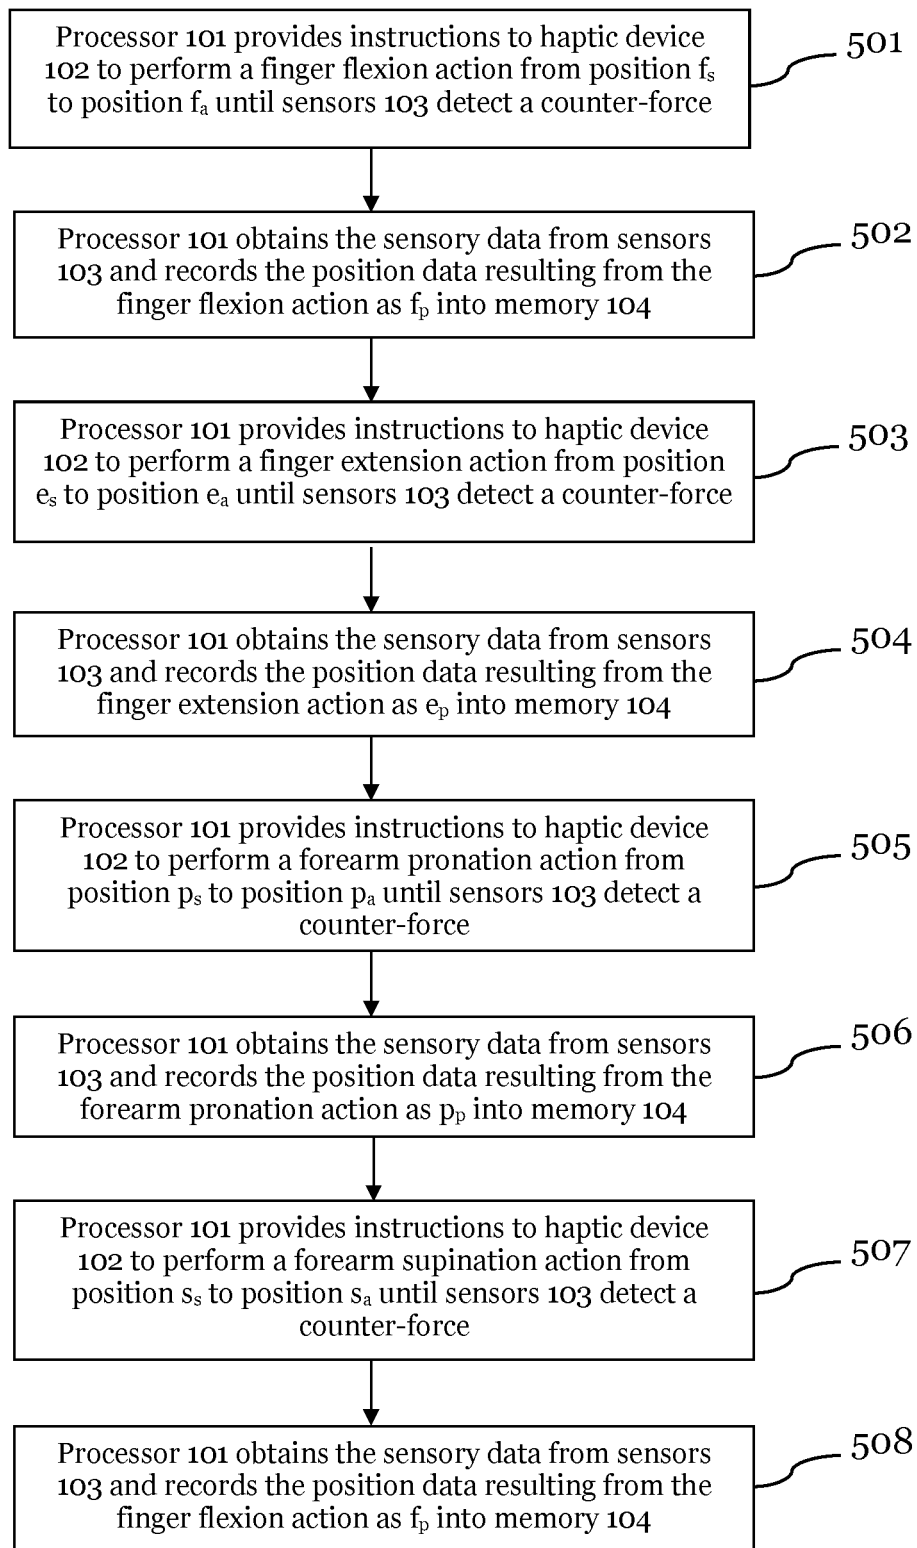


Figure 5

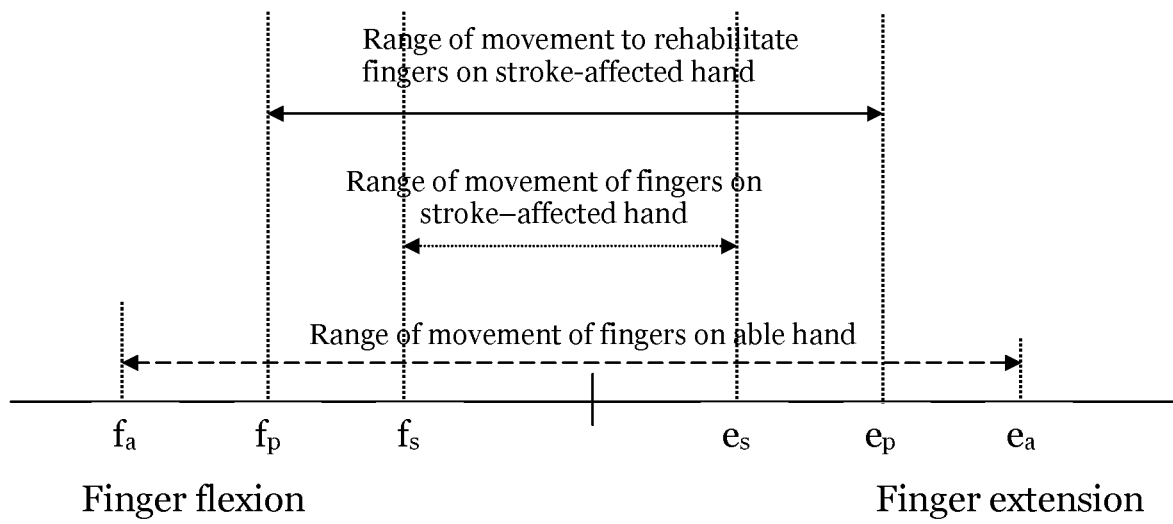


Figure 6

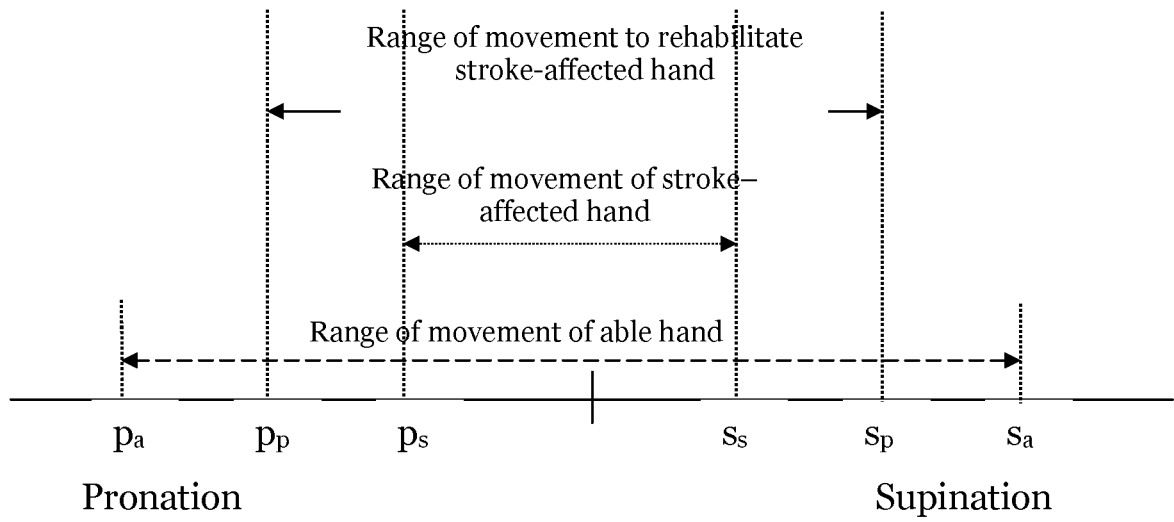


Figure 7

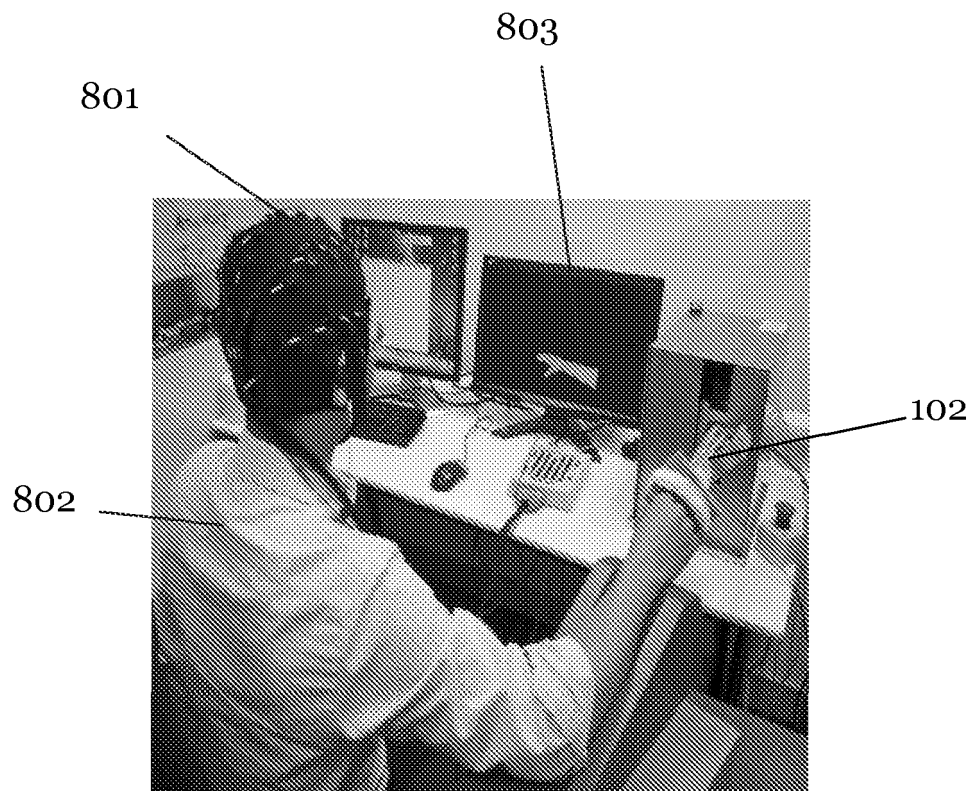


Figure 8

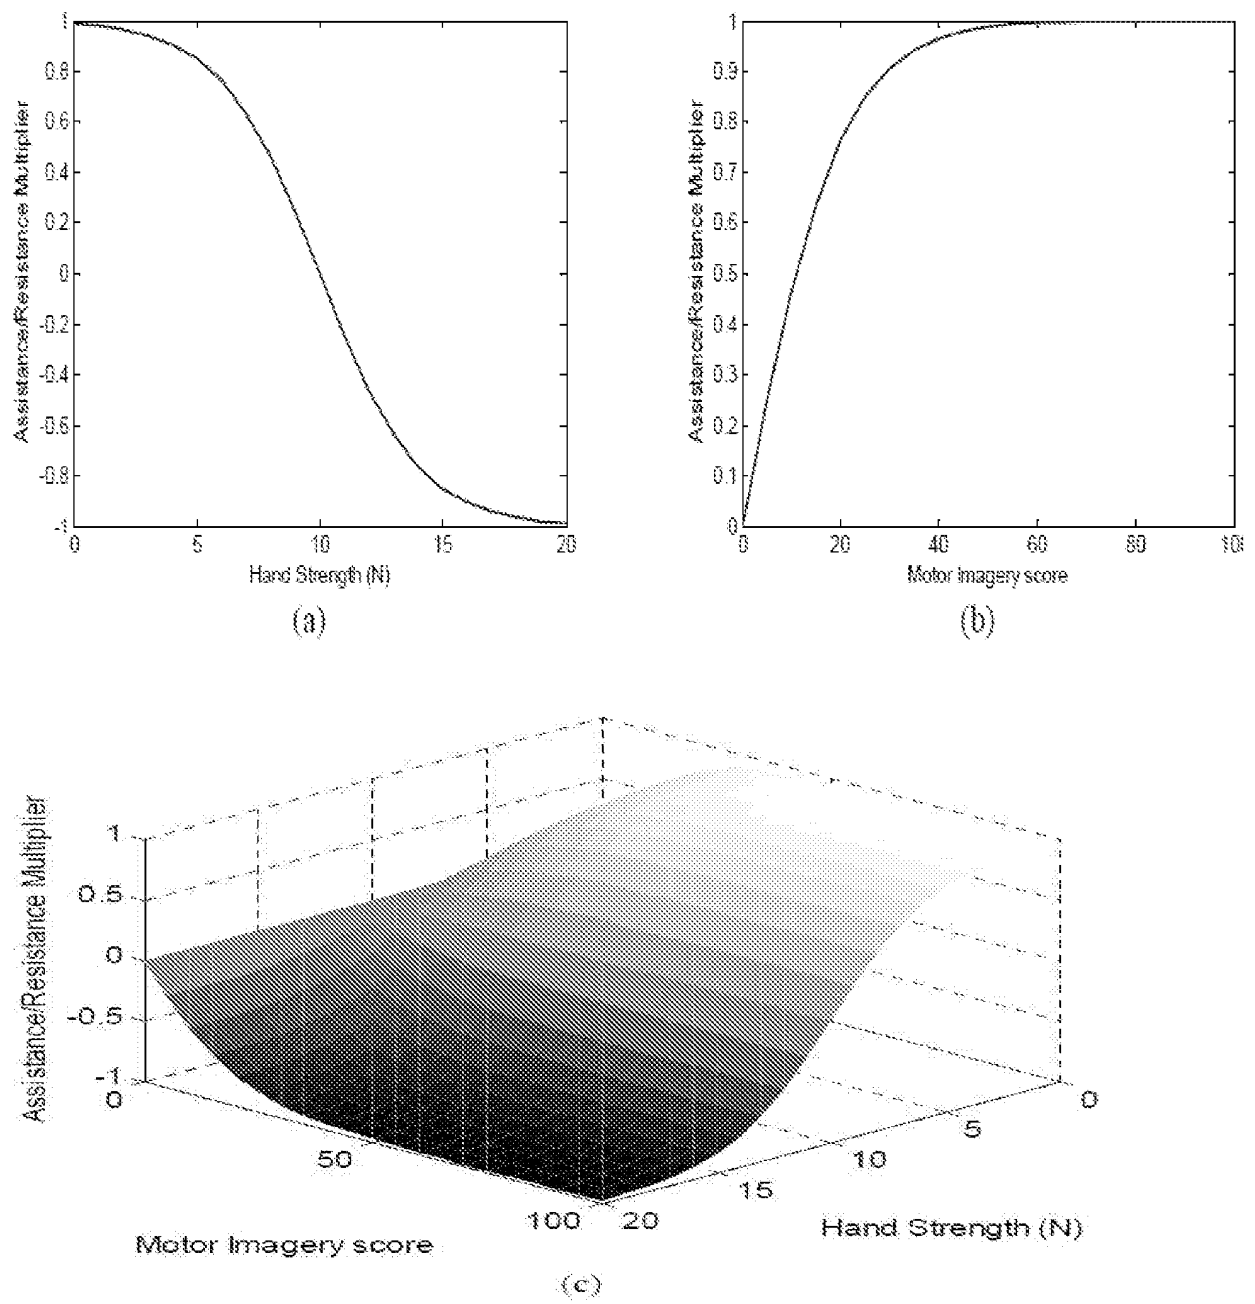


Figure 9

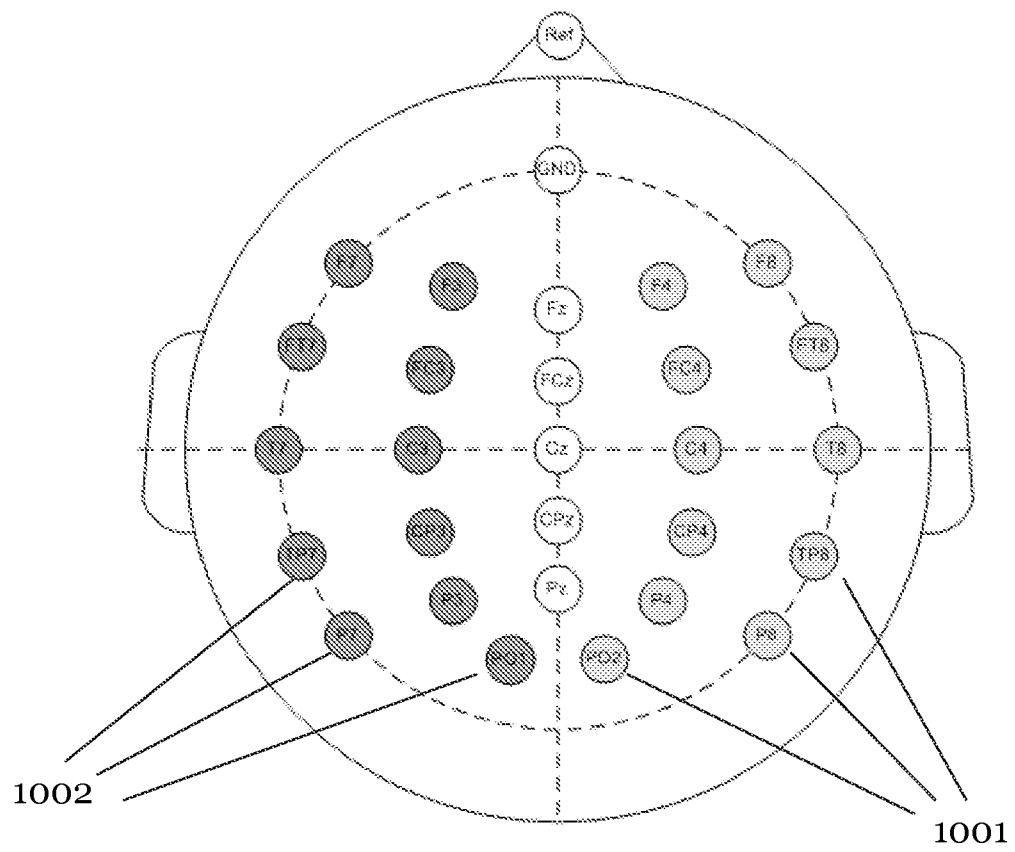


Figure 10

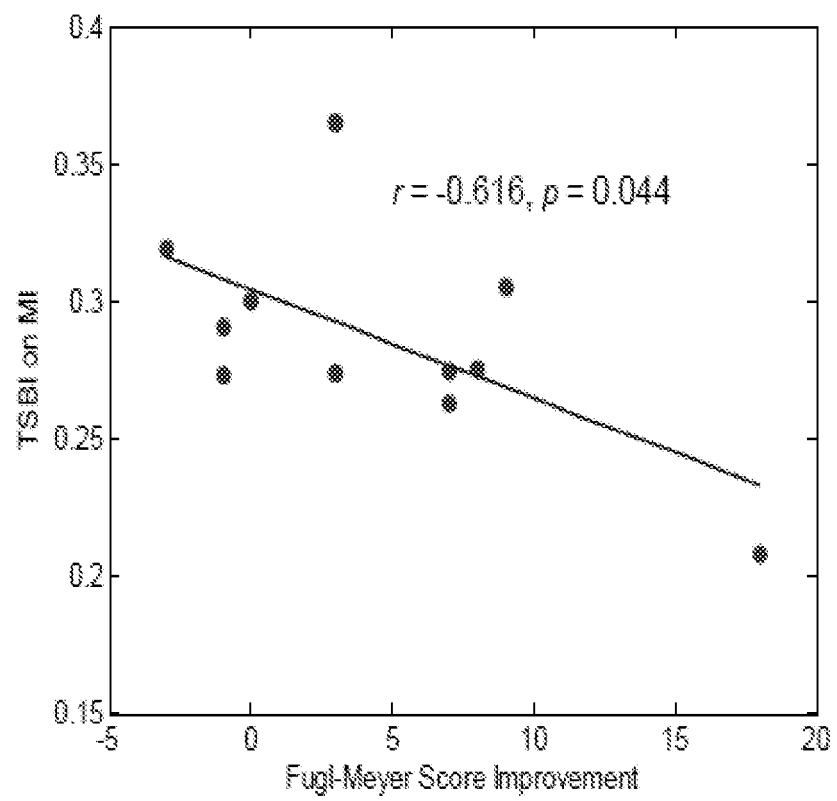


Figure 11

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- SG 10201404337 Y [0001]
- WO 2005074373 A2 [0008]

专利名称(译)	使用机器人设备和脑计算机接口进行修复的方法和系统		
公开(公告)号	EP3171777B1	公开(公告)日	2019-12-18
申请号	EP2015823957	申请日	2015-07-23
[标]申请(专利权)人(译)	新加坡科技研究局		
申请(专利权)人(译)	机构科学，技术和研究		
当前申请(专利权)人(译)	机构科学，技术和研究		
[标]发明人	ANG KAI KENG GUAN CUNTAI PHUA KOK SOON ZHOU LONGJIANG WANG CHUAN CHU		
发明人	ANG, KAI KENG GUAN, CUNTAI PHUA, KOK SOON ZHOU, LONGJIANG WANG, CHUAN CHU		
IPC分类号	A61B5/11 A61H1/00 A61H1/02 A61B5/00 A61B5/0476 A61B5/0482 A61B5/22 G06F3/01 G09B9/06 G09B5/06		
CPC分类号	A61B5/0482 A61B5/1121 A61B5/1126 A61B5/225 A61B5/7475 A61B2560/0223 A61H1/02 A61H1/0274 A61H1/0285 A61H1/0288 A61H2001/0203 A61H2201/1635 A61H2201/1671 A61H2201/5043 A61H2201/5048 A61H2201/5061 A61H2201/5064 A61H2230/105 G06F3/014 G06F3/015 G06F3/016 A61B5/0476 G09B5/06		
优先权	10201404337Y 2014-07-23 SG		
其他公开文献	EP3171777A1 EP3171777A4		
外部链接	Espacenet		

摘要(译)

公开了一种用于校准和执行针对中风患者的中风患者的肢体的康复运动的方法，该方法包括以下步骤：提供触觉设备，以使中风患者的有能力的肢体进行操纵以执行校准动作以导致 触觉设备的第一位置，并为受中风影响的肢体提供触觉设备以进行操纵以执行校准动作，以产生触觉设备的第二位置。该方法还包括以下步骤：将与受冲程影响的肢体耦接的触觉设备从第二位置移向第一位置，直到检测到预定的反作用力，使用该触觉设备指示受卒中的肢体的极限位置，并进行校准 该触觉设备具有极限位置，使得在康复锻炼期间，防止该触觉设备移动超出极限位置。

$$\alpha = -\tanh\left(\frac{5}{h_{\max}}\left(h - \frac{h_{\max}}{2}\right)\right) \tanh\left(\frac{5m}{m_{\max}}\right),$$