



(11) **EP 2 249 694 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:

02.09.2015 Bulletin 2015/36

(21) Application number: **09711443.3**

(22) Date of filing: **26.01.2009**

(51) Int Cl.:

A61B 5/00 (2006.01)

(86) International application number:

PCT/US2009/032057

(87) International publication number:

WO 2009/102549 (20.08.2009 Gazette 2009/34)

(54) **APPARATUS AND METHOD FOR NON-INVASIVE MEASUREMENT OF THE CONCENTRATION OF A SUBSTANCE IN A SUBJECT'S BLOOD**

VORRICHTUNG UND VERFAHREN ZUR NICHT-INVASIVEN MESSUNG DER KONZENTRATION
EINES STOFFES IM BLUT EINER PERSON

APPAREIL ET PROCÉDÉ POUR UNE MESURE NON INVASIVE DE LA CONCENTRATION D'UNE
SUBSTANCE DANS LE SANG D'UN PATIENT

(84) Designated Contracting States:

**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL
PT RO SE SI SK TR**

(30) Priority: **11.02.2008 US 29339**

(43) Date of publication of application:

17.11.2010 Bulletin 2010/46

(73) Proprietor: **Gluco Vista LLC**

Fairfield, NJ 07004 (US)

(72) Inventor: **GERLITZ, Jonathan**

46473 Herzliya (IL)

(74) Representative: **Casbon, Paul Richard**

Lucas & Co

135 Westhall Road

Warlingham, Surrey CR6 9HJ (GB)

(56) References cited:

US-A1- 2006 015 022

US-B1- 6 226 089

US-B1- 6 931 268

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionBackground of the Invention5 Field of the Invention

[0001] This application relates generally to devices and methods for non-invasively measuring the concentration of a substance in a subject's blood, and more particularly, to devices and methods for non-invasively measuring the concentration of glucose in the subject's blood.

10 Description of Related Art

[0002] Numerous systems were suggested in the last decades, to solve the problem of non-invasively measuring the level of substances (e.g., glucose) in a subject's blood. The main drawback of all those systems was a very poor signal to noise ratio, which required a very heavy computing system, and resulted in inconsistent and unrepeatable results.

15 [0003] In addition, conventional systems for non-invasive measurement of substances (e.g., glucose) in the blood do not take into consideration the various parameters that affect such measurements in human tissue. For example, conventional systems that utilize measurements taken from the eye do not take into consideration the changing parameters of the eye, such as pupil size, other materials of the eye, the absorption or scattering of light inside the eyeball. In particular, U.S. Patent Nos. 6,494,576 and 5,820,557 suggest subtracting the reflected light intensity from the intensity of the originally irradiated light and to correlate this subtracted value to glucose concentration. A method for optically measuring glucose taking into account temperature effects is known from U.S. patent No. 6,226,089.

25 Summary of the Invention

[0004] In certain embodiments, a method determines the concentration of a substance in a subject's blood. The method comprises noninvasively irradiating an eye of the subject with a measurement light beam having a first wavelength and a first power. At least a portion of the measurement light beam is retro-reflected from the retina of the eye, thereby producing a measurement retro-reflected light beam having the first wavelength. The method further comprises noninvasively irradiating the eye of the subject with a reference light beam having a second wavelength and a second power. The second wavelength is different from the first wavelength. At least a portion of the reference light beam is retro-reflected from the retina of the eye, thereby producing a reference retro-reflected light beam having the second wavelength. The method further comprises measuring at least one of a body temperature of the subject and an ambient temperature of the subject. The method further comprises detecting a power of the measurement retro-reflected light beam. The method further comprises detecting a power of the reference retro-reflected light beam. The method further comprises calculating a measurement ratio of the detected power of the measurement retro-reflected light beam and the first power. The method further comprises calculating a reference ratio of the detected power of the reference retro-reflected light beam and the second power. The method further comprises calculating a parameter dependent on the measurement ratio and the reference ratio. The method further comprises determining a concentration of the substance in the subject's blood in response to the calculated parameter and to the at least one of the body temperature and the ambient temperature.

35 [0005] In certain embodiments, an apparatus measures a concentration of a substance in a subject's blood. The apparatus comprises at least one light source generating light having a first wavelength and generating light having a second wavelength. The second wavelength is different from the first wavelength. The apparatus further comprises an optical system which directs at least a portion of the light having the first wavelength towards the subject's eye as a measurement light beam having a first power. At least a portion of the measurement light beam is retro-reflected from the subject's retina. The optical system directs at least a portion of the light having the second wavelength towards the subject's eye as a reference light beam having a second power. At least a portion of the reference light beam is retro-reflected from the subject's retina. The apparatus further comprises a detector system receiving the retro-reflected portion of the measurement light beam and the retro-reflected portion of the reference light beam. The detector system is responsive to the received retro-reflected portion of the measurement light beam by generating a first signal indicative of the power of the received retro-reflected portion of the measurement light beam. The detector system is responsive to the received retro-reflected portion of the reference light beam by generating a second signal indicative of the power of the received retro-reflected portion of the reference light beam. The apparatus further comprises at least one temperature detector which measures at least one of a body temperature of the subject and an ambient temperature of the subject and which generates at least one signal indicative of the at least one of the body temperature and the ambient temperature. The apparatus further comprises a computing system which receives the first signal, the second signal, and the at least one signal. The computing system calculates a first ratio of the first power and the power of the received

retro-reflected portion of the measurement light beam. The computing system calculates a second ratio of the second power and the power of the received retro-reflected portion of the reference light beam. The computing system calculates a parameter dependent on the first ratio and the second ratio, and determines a concentration of the substance in the subject's blood in response to the calculated parameter and to the at least one signal.

[0006] In certain embodiments, a computing system measures a concentration of a substance in a subject's blood. The computing system comprises one or more inputs configured to receive a first signal indicative of a first power of a measurement light beam incident on a subject's eye, a second signal indicative of a second power of a reference light beam incident on a subject's eye, a third signal indicative of a third power of a portion of the measurement light beam retro-reflected from the subject's retina, a fourth signal indicative of a fourth power of a portion of the reference light beam retro-reflected from the subject's retina, and at least one signal indicative of at least one of a body temperature of the subject and an ambient temperature of the subject. The measurement light beam has a first wavelength and the reference light beam has a second wavelength different from the first wavelength. The computing system further comprises an electric circuit configured to calculate a first ratio of the first power and the third power. The electric circuit is further configured to calculate a second ratio of the second power and the fourth power. The electric circuit is further configured to calculate a parameter dependent on the first ratio and the second ratio. The electric circuit is further configured to determine a concentration of the substance in the subject's blood in response to the calculated parameter and to the at least one of a body temperature of the subject and an ambient temperature of the subject.

[0007] In certain embodiments, a method determines the concentration of a substance in a subject's blood. The method comprises measuring an interaction of at least one light beam with a portion of the subject's body. The method further comprises calculating a value of an optically-measured parameter indicative of the interaction of the at least one light beam with the substance in the portion of the subject's body. The method further comprises measuring values of one or more temperature-indicative parameters corresponding to a temperature of the portion of the subject's body. The method further comprises accessing an empirical correlation of the optically-measured parameter and the one or more temperature-indicative parameters to concentrations of the substance in blood. The method further comprises obtaining a concentration of the substance in the subject's blood using the empirical correlation. The concentration corresponds to the value of the optically-measured parameter and the values of the one or more temperature-indicative parameters.

[0008] In certain embodiments, a method determines a correlation of a concentration of a substance in a person's blood with a plurality of parameters. The method comprises invasively measuring values of the concentration of the substance in the blood of a plurality of people at a plurality of conditions. The plurality of people is statistically representative of a larger population of people. The method further comprises non-invasively optically measuring values of a parameter from the plurality of people at the plurality of conditions. The value of the optically-measured parameter measured from a portion of a person's body is indicative of the concentration of the substance in the person's blood. The method further comprises measuring values of one or more temperature-indicative parameters for the plurality of people at the plurality of conditions. The one or more temperature-indicative parameters corresponds to a temperature of the portion of the person's body. The method further comprises generating a correlation by correlating the measured values of the optically-measured parameter and the measured values of the one or more temperature-indicative parameters to the measured values of the concentration of the substance in the blood of the plurality of people. A method according to the invention is disclosed in claim 1. A device according to the invention is disclosed in claim 13.

Brief Description of the Drawings

[0009]

Figure 1 schematically illustrates an example configuration of an apparatus in accordance with certain embodiments described herein.

Figure 2 schematically illustrates an example configuration of an apparatus having a first light source and a second light source coupled to a movable element in accordance with certain embodiments described herein.

Figure 3 schematically illustrates an example configuration of an apparatus having a first light source and a second light source spaced from one another in accordance with certain embodiments described herein.

Figure 4 schematically illustrates an example configuration of an apparatus having a single wide band light source in accordance with certain embodiments described herein.

Figure 5 schematically illustrates an example configuration of an apparatus having two light detectors in accordance with certain embodiments described herein.

Figure 6 schematically illustrates an example electronic circuit in accordance with certain embodiments described herein.

Figure 7 is an example plot of the temperature dependence of transmission measurements for water and for a water/glucose mixture.

Figure 8 schematically illustrates another example configuration of an apparatus in accordance with certain embod-

iments described herein.

Figure 9 schematically illustrates an example multi-parameter look-up table in accordance with certain embodiments described herein.

Detailed Description

[0010] As described more fully below, the simple subtraction scheme utilized in the conventional systems of the prior art fails to account for other parameters which affect the concentration measurements of substances in the subject's body. Thus, these simple subtraction schemes cannot reliably be used as measures of the substance concentration of the subject's blood.

[0011] Certain embodiments described herein provide an apparatus and a measurement and calculation method to isolate a measurable parameter that can be correlated to the concentration of substances (e.g., glucose) in the subject's blood. As described more fully below, in certain embodiments, the method includes constraints on (i) the wavelengths and relationships between the wavelengths of the light being used; and (ii) the method of calculations based on measurements with these wavelengths in order to eliminate or otherwise account for various parameters that may affect the measurements but are not relevant to the actual concentrations of the substances (e.g., glucose) being measured.

[0012] While certain embodiments are described herein in the context of measuring glucose concentrations, concentrations of other substances which can be measured in accordance with certain embodiments described herein include, but are not limited to, cholesterol. While certain embodiments are described herein in the context of infrared or near-infrared optical absorption measurements, other near-infrared optical measurements which can be improved in accordance with certain embodiments described herein include, but are not limited to, transmission measurements, reflection measurements, scattering measurements, polarization measurements, and Roman measurements. While certain embodiments are described herein in the context of non-invasive optical measurements taken from the subject's eye, other non-invasive optical measurements which can be improved in accordance with certain embodiments described herein are taken from other portions of the subject's body including, but not limited to, skin, earlobe, finger (web or cuticle), lip, or cheek.

[0013] Certain embodiments described herein advantageously provide a non-invasive glucose meter which has a good signal to noise ratio, thus making the measurement consistent, repeatable and reliable. Certain embodiments described herein advantageously provide such an apparatus for non-invasive glucose measurement, which is easy and simple to handle by the user, small sized and inexpensive. Certain embodiments described herein advantageously provide a non-invasive glucose meter which can be used in various environments, indoors and outdoors.

[0014] Certain embodiments described herein utilize the properties of the eye as an optical apparatus. Every optical apparatus, which is equipped with focusing means and a focal plane, shows the phenomenon of retro-reflection, meaning that the apparatus reflects back at least a portion of the entering light beam in the same direction it comes from. Certain embodiments described herein provide an electro-optical apparatus which uses the retro-reflection characteristic of the eye in order to determine the concentration of glucose or of another substance in the eye liquid (the vitreous body) and/or in the blood.

[0015] Figure 1 schematically illustrates an example apparatus 10 in accordance with certain embodiments described herein. The apparatus 10 comprises at least one light source 20 which generates light having a first wavelength. The at least one light source 20 further generates light having a second wavelength. The apparatus 10 further comprises an optical system 30 which directs at least a portion of the light having the first wavelength towards the subject's eye 40 as a measurement light beam 32 having a first power, at least a portion of the measurement light beam 32 retro-reflecting from the subject's retina 42. The optical system 30 also directs at least a portion of the light having the second wavelength towards the subject's eye 40 as a reference light beam 34 having a second power, at least a portion of the reference light beam 34 retro-reflecting from the subject's retina 42. The apparatus 10 further comprises a detector system 50 which receives the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34. The detector system 50 is responsive to the received retro-reflected portion of the measurement light beam 32 by generating a first signal indicative of the power of the received retro-reflected portion of the measurement light beam 32. The detector system 50 is responsive to the received retro-reflected portion of the reference light beam 34 by generating a second signal indicative of the power of the received retro-reflected portion of the reference light beam 34. The apparatus 10 further comprises a computing system 60 which receives the first signal and the second signal from the detector system 50. The computing system 60 calculates a first ratio of the first power and the power of the received retro-reflected portion of the measurement light beam 32. The computing system 60 further calculates a second ratio of the second power and the power of the received retro-reflected portion of the reference light beam 34. The computing system 60 further calculates a parameter dependent on the first ratio and the second ratio (e.g., a difference of the first ratio and the second ratio or a difference between a logarithm of the first ratio and a logarithm of the second ratio) and determines a concentration of the substance in the subject's blood in response to the calculated parameter.

[0016] In certain embodiments, the apparatus 10 is sized to be portable and easily held by a user (e.g., a medical practitioner or the subject themselves). As described more fully below, the apparatus 10 can comprise an internal power supply (e.g., battery or fuel cell) and can comprise a display (e.g., liquid-crystal display) to receive signals indicative of the concentration values from the computing system 60 and to present information regarding the concentration values (e.g., the concentration values themselves or indications that the concentration values are above or below a predetermined value) to the user. The apparatus 10 can also comprise a memory system (e.g., flash memory, dynamic random-access memory) configured to receive signals indicative of information regarding the concentration values from the computing system 60 and to store information for later use or for display to the user. In certain embodiments, the computer system 60 can comprises the display and/or the memory system.

[0017] In certain embodiments, the apparatus 10 is configured to be positioned at a distance of at least 100 millimeters from the subject's eye during operation (e.g., while the measurement light beam 32 and the reference light beam 34 are directed towards the subject's retina 42). In certain other embodiments, the apparatus 10 is configured to be positioned such that the optical pathlength of the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34 from the subject's eye 40 to the detector system 50 is at least 100 millimeters. The optical pathlength from the subject's eye 40 to the detector system 50 for certain embodiments is sufficiently long such that the detector system 50 receives mainly the retro-reflected portions of the measurement light beam 32 and the reference light beam 34, and advantageously avoids receiving other reflections (e.g., from the subject's cornea) which the apparatus 10 could interpret to be noise.

[0018] The at least one light source 20 is configured to output light having the first wavelength to the optical system 30 and to output light having the second wavelength to the optical system 30. In certain embodiments, the at least one light source 20 comprises at least two infrared (IR) emitters which emit light within two different wavelength bands. For example, Figure 2 schematically illustrates an example apparatus 10 having a first light source 21 and a second light source 22 in accordance with certain embodiments described herein. Examples of light sources compatible with certain embodiments described herein include, but are not limited to, a light bulb with a bandpass filter, a laser diode, and a high power infrared light emitting diode.

[0019] In the apparatus 10 schematically illustrated by Figure 2, the first light source 21 and the second light source 22 are coupled to a movable element 23 (e.g., a motor) which can be actuated to position either the first light source 21 or the second light source 22 so as to transmit light to the optical system 30. Thus, in certain such embodiments, the measurement light beam 32 and the reference light beam 34 are directed towards the subject's eye 40 sequentially, one after the other. In certain embodiments, the light having the first wavelength and the light having the second wavelength propagate towards the optical system 30 along the same path as one another, as schematically illustrated by Figure 2. In certain embodiments, the at least one light source 20 comprises at least one optical element 24 (e.g., lens) which directs light from the at least one light source 20 towards the optical system 30.

[0020] In the apparatus 10 schematically illustrated by Figure 3, the first light source 21 and the second light source 22 are spaced from one another but are each positioned to transmit light to the optical system 30. Thus, in certain such embodiments, the measurement light beam 32 and the reference light beam 34 are directed towards the subject's eye 40 concurrently with one another. In certain embodiments, the light having the first wavelength and the light having the second wavelength propagate towards the optical system 30 along different paths which can be parallel or non-parallel to one another. For example, the first light source 21 and a corresponding optical element 24 (e.g., lens) are positioned on one side of the optical system 30, and the second light source 22 and a corresponding optical element 25 are positioned on another side of the optical system 30. Other configurations of the first light source 21, the second light source 22, and optical elements of the at least one light source 20 are also compatible with certain embodiments described herein.

[0021] In certain embodiments, as schematically illustrated by Figure 4, the at least one light source 20 comprises a single wideband light source 26 (e.g., a miniature lamp) which emits light in a wide wavelength band, an optical element 27 (e.g., lens), and a filter wheel 28 comprising two or more narrow band filters which filter the light from the wide band light source 26 into two different wavelength bands. Certain such embodiments are advantageously used for providing more than two wavelengths to analyze the concentrations of glucose or other substances. In certain embodiments, the filter wheel 28 comprises a motor which can be actuated to position a selected filter of the filter wheel 28 in the path of the light from the wideband light source 26, thereby filtering out selected wavelengths from the light emitted by the at least one light source 20. While Figure 4 schematically illustrates an embodiment in which the optical element 27 is between the wideband light source 26 and the filter wheel 28, in certain other embodiments, the filter wheel 28 is between the wideband light source 26 and the optical element 27.

[0022] In certain embodiments, the light emitted by the at least one light source 20 having the first wavelength comprises a light beam (e.g., a nearly parallel, substantially parallel, or collimated light beam) which the optical system 30 directs towards the subject's eye 40 as the measurement light beam 32, and the light emitted by the at least one light source 20 having the second wavelength comprises a light beam (e.g., a nearly parallel, substantially parallel, or collimated light beam) which the optical system 30 directs towards the subject's eye 40 as the reference light beam 34. In certain

other embodiments, the light emitted by the at least one light source 20 comprises a non-parallel or non-collimated light beam, but the optical system 30 is configured to receive the light having the first wavelength and to generate a nearly parallel, substantially parallel, or collimated measurement light beam 32 and to receive the light having the second wavelength and to generate a nearly parallel, substantially parallel, or collimated reference light beam 34. In certain various embodiments, the measurement light beam 32 has a beam divergence less than or equal to 5 degrees, less than or equal to 3 degrees, or less than or equal to 1 degree. In certain various embodiments, the reference light beam 34 has a beam divergence less than or equal to 5 degrees, less than or equal to 3 degrees, or less than or equal to 1 degree. In certain embodiments, the measurement light beam 32 and the reference light beam 34 are substantially parallel to one another. In certain embodiments, the measurement light beam 32 and the reference light beam 34 are parallel to one another such that an angle between the two beams is less than or equal to 0.1 degree. In certain embodiments, the measurement light beam 32 and the reference light beam 34 are substantially co-linear with one another. For example, the measurement light beam 32 and the reference light beam 34 of certain embodiments are parallel to one another and spaced from one another by less than 0.2 millimeter.

[0023] In certain embodiments, the first wavelength is in a range of wavelengths in which the substance to be measured (e.g., glucose) has a high absorption coefficient, and the second wavelength is in a range of wavelengths in which the substance to be measured has a low absorption coefficient. In certain embodiments, the first wavelength is in the infrared (IR) or near-infrared (near-IR) range of wavelengths, and the second wavelength is in the infrared (IR) or near-infrared (near-IR) range of wavelengths. In certain various embodiments in which glucose is measured, the first wavelength can be selected to be in a range between about 920 nanometers and about 980 nanometers (e.g., 950 nanometers), in a range between about 1130 nanometers and about 1190 nanometers (e.g., 1160 nanometers), or in a range between about 1.3 microns and about 1.5 microns (e.g., 1460 nanometers). In certain various embodiments in which glucose is measured, the second wavelength is selected to be close to the first wavelength, but having substantially no absorption due to glucose. For example, in certain embodiments in which the first wavelength is in a range between about 920 nanometers and about 980 nanometers, the second wavelength can be in a range between about 800 nanometers and about 905 nanometers (e.g., 870 nanometers or 880 nanometers). In another example, in certain embodiments, the first wavelength is about 1160 nanometers and the second wavelength is about 1120 nanometers. To measure concentrations of other substances in the subject's eye liquid and/or blood, other wavelengths are advantageously used. In certain embodiments, the reference light beam 34 is used as a reference beam which can be used to compensate for changes of the pupil and/or iris, and thus enables the use of the apparatus 10 in various light conditions.

[0024] In certain embodiments, the optical system 30 receives light from the at least one light source 20 and directs the measurement light beam 32 and the reference light beam 34 towards the subject's eye 40. In certain embodiments, the optical system 30 is located in the center of the apparatus 10. Figures 2 and 3 schematically illustrate an example optical system 30 in accordance with certain embodiments described herein. The optical system 30 of Figures 2 and 3 comprises a dichroic coating layer 36, an optical glass layer 37, a holographic beam splitter layer 38, and a cover glass layer 39. This combination of four layers operates in certain embodiments as an optical combiner. The dichroic coating layer 36 of certain embodiments is applied on at least one surface of the optical glass layer 37. In certain embodiments, the dichroic coating layer 36 has a center wavelength corresponding to the wavelength of the first light source 21 or corresponding to the wavelength of the second light source 22. The dichroic coating layer 36 of certain embodiments enables 50-60% of the IR light from the at least one light source 20 to pass through, and 40-50% of the IR light from the at least one light source 20 to be reflected at a 90° angle towards the subject's eye 40.

[0025] In certain embodiments, the holographic beam splitter layer 38 is on the other surface of the optical glass layer 37 and is covered by the cover glass layer 39. The holographic beam splitter layer 38 of certain embodiments has a center wavelength corresponding to the wavelength of the first light source 21 or the second light source 22. In certain embodiments, the holographic beam splitter layer 38 allows 50-60% of the light from the at least one light source 20 having the center wavelength to pass through, and 40-50% of the light from the at least one light source 20 having the center wavelength to be reflected at a 270° angle towards the subject's eye 40.

[0026] In certain embodiments, the optical system 30 comprises only a single dichroic coating layer 36. For example, in certain such embodiments, the first light source 21 and the second light source 22 change position to emit light towards the optical system 30 intermittently (e.g., by actuating a movable element or motor 23 to move the first light source 21 and the second light source 22 as in Figure 2). The dichroic coating layer 36 of certain such embodiments is a wide band coating for the wavelengths of both the first light source 21 and the second light source 22.

[0027] In certain embodiments, the at least one light source 20 comprises optical elements (e.g., lenses 24, 25) such that the measurement light beam 32 is a nearly parallel, substantially parallel, or collimated beam and the reference light beam 34 is a nearly parallel, substantially parallel, or collimated beam. In certain other embodiments, the optical system 30 comprises optical elements (e.g., lenses) such that the measurement light beam 32 is a nearly parallel, substantially parallel, or collimated beam and the reference light beam 34 is a nearly parallel, substantially parallel, or collimated beam. In certain embodiments, the measurement light beam 32 and the reference light beam 34 are on the same optical path as one another. In certain embodiments, the measurement light beam 32 and the reference light beam

34 each have a diameter (e.g., the full-width-at-half-maximum diameter) of about 2 millimeters. In certain embodiments, the measurement light beam 32 and the reference light beam 34 each have a generally Gaussian beam intensity profile and have a substantially circular or substantially elliptical beam spot shape. In certain embodiments, the measurement light beam 32 and the reference light beam 34 are continuous-wave beams, while in certain other embodiments, the measurement light beam 32 and the reference light beam 34 are pulsed light beams.

[0028] The measurement light beam 32 and the reference light beam 34 are directed towards and enter the subject's eye 40 by passing through the cornea, the pupil and/or the iris, the eye lens, and the eye liquid. The two light beams 32, 34 are focused approximately on the retina 42 at a focal point 44. A portion of the measurement light beam 32 is reflected from the retina 42, and a retro-reflected portion of this reflected light comes out of the subject's eye 40 from the same focal point 44 on the exact optical path of the incoming measurement light beam 32, but in the opposite direction. This retro-reflected portion of the measurement light beam 32 propagates towards, and is received by, the apparatus 10. Similarly, a portion of the reference light beam 34 is reflected from the retina 42, and a retro-reflected portion of this reflected light comes out of the subject's eye 40 from the same focal point 44 on the exact optical path of the incoming reference light beam 34, but in the opposite direction. This retro-reflected portion of the reference light beam 34 propagates towards, and is received by, the apparatus 10.

[0029] Each of the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34 in certain embodiments passes twice through the eye 40, first through the cornea, the eye lens, and liquid (vitreous body), then focuses on the retina 42, and subsequently is reflected back through the eye liquid, lens, and cornea towards the optical system 30.

[0030] In certain embodiments, the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34 are received by the detector system 50 directly from the eye 40. In certain other embodiments, the optical system 30 receives the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34 directly from the eye 40 and transmits these retro-reflected portions to the detector system 50. As schematically illustrated by Figures 2, 3, and 4, the detector system 50 is located on the same optical path as the measurement and reference light beams 32, 34 such that the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34 pass through the components of the optical system 30 (e.g., through the beam splitter layer 38) to the detector system 50. For example, in certain embodiments, 50-60% of the retro-reflected portions of the measurement and reference light beams 32, 34 can pass through the beam splitter layer 38 to the detector system 50.

[0031] In certain embodiments, the detector system 50 comprises at least one optical element 52 (e.g., lens) and at least one light detector 54. As schematically illustrated by Figures 2, 3, and 4, the at least one optical element 52 of certain embodiments receives the retro-reflected light and focuses the retro-reflected light onto the at least one light detector 54. The at least one light detector 54 of certain embodiments is configured to generate a first signal indicative of the power of the received retro-reflected portion of the measurement light beam 32 and to generate a second signal indicative of the power of the received retro-reflected portion of the reference light beam 34. Examples of light detectors compatible with certain embodiments described herein include, but are not limited to, silicon detectors, PbS detectors, or any other kind of IR detector known in the art.

[0032] Figure 5 schematically illustrates an example configuration of an apparatus having two optical elements 52, 56 and two light detectors 54, 58 in accordance with certain embodiments described herein. The optical element 52 and the light detector 54 receive the two retro-reflected light beams and the light detector 54 is configured to generate signals corresponding to the powers of the retro-reflected light beams. The optical element 56 and the light detector 58 receive a portion of the light generated by the at least one light source 20 and the light detector 58 is configured to generate signals corresponding to the powers of the measurement and reference light beams 32, 34 incident on the subject's eye 40. Certain such embodiments provide measurements of the power of the incident light beams to compare to the power of the retro-reflected light beams. Other configurations of the at least one light source 20, the optical system 30, and the detection system 50 are also compatible with certain embodiments described herein.

[0033] Figure 6 schematically illustrates an electronic diagram of an example apparatus 10 in accordance with certain embodiments described herein. In certain embodiments, the computing system 60 comprises a central processing unit (CPU) 61 (e.g., an Epson 6200, produced by Epson, Japan). The CPU 61 of certain embodiments is electrically coupled to one or more of the at least one light source 20, the optical system 30, and the detector system 50 to control the operation of the apparatus 10.

[0034] In certain embodiments, the at least one light source 20 comprises the first light source 21, the second light source 22, a first amplifier 62 electrically coupled to the first light source 21, and a second amplifier 63 electrically coupled to the second light source 22, as schematically illustrated by Figure 6. The first amplifier 62 and the second amplifier 63 receive signals from the computing system 60 and, in response, activate the first and second light sources 21, 22 (e.g., sequentially or concurrently). In certain embodiments, the at least one light source 20 further comprises a movable element 23 (e.g., motor) and a third amplifier 64 electrically coupled to the movable element 23, as schematically illustrated by Figure 6. The third amplifier 64 receives signals from the computing system 60 and, in response, activates

the movable element 23 so as to position the first and second light sources 21, 22 for transmitting light to the optical system 30.

[0035] In certain embodiments, the detector system 50 comprises at least one light detector 54, an amplifier 65, a filter 66, and an analog-to-digital (A/D) converter 67, as schematically illustrated by Figure 6. For example, in certain embodiments, the A/D converter 67 comprises a fast 12-bit converter. Analog signals from the at least one light detector 54 corresponding to the detected powers of the retro-reflected portions of the measurement light beam 32 and the reference light beam 34 are amplified, filtered, converted to digital signals, and transmitted to the computing system 60. In certain embodiments in which the detector system 50 comprises a second light detector 58 (e.g., as schematically illustrated by Figure 5), signals from the second light detector 58 corresponding to the power of the incident light beams are amplified, filtered, and converted into digital signals in a similar way. These digital signals can then be used by the computing system 60 as described further herein.

[0036] In certain embodiments, the apparatus 10 is turned on by switch 68, which connects the power source 69 (e.g., a lithium battery) to the circuitry. After a self-check, the CPU 61 of certain embodiments displays "Ready" on a display unit 70 (e.g., a liquid crystal display (LCD)). In certain embodiments, to perform a measurement, switch 71 is activated, and, in response, the CPU 61 starts a measurement procedure. In certain embodiments, the CPU 71 activates in sequence the first light source 21 through the first amplifier 62 and the second light source 22 through the second amplifier 63, and activates the movable element 23 through the third amplifier 64 in certain embodiments in which such a movable element 23 is used. The retro-reflected portions of the measurement light beam 32 and the reference light beam 34 detected from the eye 40 are translated by the at least one light detector 54 (e.g., an IR detector) to an analog voltage signal, which is amplified by amplifier 65 and filtered by filter 66. This analog signal is converted to a digital form by the A/D converter 67 and is received and stored by the CPU 71 (e.g., in memory 72). After receiving measurement data corresponding to the two wavelengths, the CPU 71 calculates the concentration of the substance (e.g., glucose) according to the absorption level calculated using calibration parameters stored in the memory 72 (e.g., electrically-erasable programmable read-only memory or E²PROM). The CPU 71 of certain embodiments also transmits signals to the display 70 to make the results of the calculation available to the user.

[0037] The absorption of the light beams 32, 34 due to substances within the eye 40 having non-negligible absorption coefficients α_λ at the wavelengths of the measurement or reference light beams 32, 34, correlates to the exponential of $(\alpha_\lambda x)$, where x is the optical pathlength within the eye 40. Thus, the magnitude of the absorption is proportional to

$\int_{\lambda_1}^{\lambda_2} e^{\alpha_\lambda x} d\lambda$ where x is the length of the optical path through the absorbing medium and α_λ is the absorption coefficient of the substance (e.g., glucose) to be measured at wavelength λ .

[0038] In certain embodiments, due to the long optical pathlength within the eye 40, the absorption can be significant even in a low concentration of the substance being measured (e.g., glucose). Because the light beams pass through the eye 40 twice, the optical path in the absorbing medium is long, and the absorption signal correlating to the exponential of $(\alpha_\lambda x)$ will be much stronger than in conventional systems which do not primarily use the retro-reflected portions of the light beams. By using the retro-reflected light from the eye, which travels through a long optical path in the absorbing medium, certain embodiments described herein advantageously overcome the main drawback of all previous suggested systems, and inherently have a good signal to noise ratio. The apparatus 10 of certain embodiments is quite simple, as described herein, and due to the good signal to noise ratio, the processing of the signal is also simple and inexpensive.

[0039] Certain embodiments described herein advantageously provide improved determinations of the concentration of a substance in a subject's blood using non-invasive optical measurements in conjunction with measurements of other parameters (e.g., temperature) that may affect the measurements of the concentration of the substances (e.g., glucose). In certain embodiments, a method of determining the concentration of a substance in a subject's blood comprises measuring an interaction of at least one light beam with a portion of the subject's body, and calculating a value of an optically-measured parameter indicative of the interaction of the at least one light beam with the portion of the subject's body. The method of certain embodiments further comprises noninvasively measuring values of one or more temperature-indicative parameters corresponding to a temperature of the portion of the subject's body. The method of certain embodiments further comprises accessing an empirical correlation of the optically-measured parameter and the one or more temperature-indicative parameters to concentrations of the substance in blood. The method of certain embodiments further comprises obtaining a concentration of the substance in blood from the empirical correlation. The concentration corresponds to the value of the optically-measured parameter and the values of the one or more temperature-indicative parameters.

[0040] Figure 7 is a plot of the temperature dependence of transmission measurements for water and for a water/glucose mixture. The measurements of Figure 7 were taken by transmitting light having a wavelength of 1160 nanometers through a cuvette having a pathlength of about 25 millimeters containing either distilled water (shown as square datapoints) or distilled water having a known concentration (250 milligrams in 1 deciliter of distilled water) of glucose (shown as circular

datapoints) at various temperatures.

[0041] As shown by Figure 7, the measured near-infrared transmission varies significantly with varying temperature of the liquid. The measured datapoints for the distilled water and for the water/glucose mixture can both be generally fit with linear functions, which are shown in Figure 7 as solid lines. These linear functions are generally offset from one another by a temperature of about 2 degrees Celsius. For example, the measured transmission through the distilled water at a temperature of 30 degrees Celsius is approximately equal to the measured transmission through the water/glucose mixture at a temperature of 32 degrees Celsius. Thus, the measured near-infrared transmission alone is insufficient information for determining the glucose concentration of the material being probed. In particular, to measure glucose concentration in blood to a tolerance of 10 milligrams/deciliter or better, the temperature is advantageously measured to an accuracy of 0.05 degrees Celsius or better. Such results highlight the importance of accurately accounting for the temperature of the material being probed by the light in using near-infrared optical measurements (e.g., absorption, transmission) to accurately determine the concentration of a substance (e.g., glucose) in the material.

[0042] In certain embodiments in which a portion of the subject's body is probed, the temperature of the portion being probed is directly measured (e.g., either non-invasively or invasively) using a temperature detector (e.g., a thermocouple, a thermistor, an infrared detector (e.g., a thermopile), or any other type of thermometer known to persons of skill in the art). In certain other embodiments, the temperature of the portion being probed is not measured, but measurements of other parameters (e.g., other temperatures) which are expected to be indicative of the temperature of the portion being probed are used instead. For example, for optical measurements made from the subject's eye, the temperature of the subject's eye can be useful for determining the glucose concentration to a desired precision. However, in certain embodiments in which measurements of the temperature of the subject's eye may be impractical to obtain, the subject's body temperature and the ambient temperature can be measured instead and used to account for the temperature dependence of the optical measurements.

[0043] Figure 8 schematically illustrates another example apparatus 10 in accordance with certain embodiments described herein. While this example apparatus 10 is described in conjunction with optical absorption measurements made from the subject's eye, persons skilled in the art recognize that certain embodiments described herein can be used as well with other types of near-infrared optical measurements taken from other portions of the subject's body. For example, other near-infrared optical measurements which can be improved in accordance with certain embodiments described herein include, but are not limited to, transmission measurements, reflection measurements, scattering measurements, polarization measurements, and Raman measurements. In certain embodiments, these measurements are taken from other portions of the subject's body besides the eye, including, but not limited to, skin, earlobe, finger (web or cuticle), lip, or cheek.

[0044] In certain embodiments, the apparatus 10 comprises at least one light source 20, an optical system 30, a detector system 50, at least one temperature detector 80, and a computing system 60. The at least one light source 20 (e.g., a first light source 21 and a second light source 22) of certain embodiments is configured to generate light having a first wavelength and light having a second wavelength different from the first wavelength. Various configurations of the at least one light source 20 described herein are compatible with the example apparatus 10 of Figure 8.

[0045] In certain embodiments, the optical system 30 is configured to direct at least one light beam towards a portion of the subject's body. For example, the optical system 30 of certain embodiments is configured to direct at least a portion of the light having the first wavelength towards the subject's eye 40 as a measurement light beam 32 having a first power, wherein at least a portion of the measurement light beam 32 retro-reflects from the subject's retina 42. The optical system 30 of certain embodiments is further configured to direct at least a portion of the light having the second wavelength towards the subject's eye 40 as a reference light beam 34 having a second power, wherein at least a portion of the reference light beam 34 retro-reflects from the subject's retina 42. In certain embodiments, the measurement light beam 32 is a nearly parallel beam and the reference light beam 34 is a nearly parallel beam. Various configurations of the optical system 30 described herein are compatible with the example apparatus 10 of Figure 8.

[0046] In certain embodiments, the apparatus 10 further comprises a detector system 50 configured to receive at least a portion of the at least one light beam after the at least one light beam has interacted with the portion of the subject's body and to generate at least one corresponding signal. For example, in certain embodiments, the detector system 50 is configured to receive the retro-reflected portion of the measurement light beam 32 and the retro-reflected portion of the reference light beam 34. The detector system 50 of certain embodiments is configured to respond to the received retro-reflected portion of the measurement light beam 32 by generating a first signal indicative of the power of the received retro-reflected portion of the measurement light beam 32. The detector system 50 of certain embodiments, is configured to respond to the received retro-reflected portion of the reference light beam 34 by generating a second signal indicative of the power of the received retro-reflected portion of the reference light beam 34. Various configurations of the detector system 50 described herein are compatible with the example apparatus 10 of Figure 8.

[0047] In certain embodiments, the apparatus 10 further comprises at least one detector of one or more temperature-indicative parameters corresponding to a temperature of the portion of the subject's body, and is configured to generate at least one signal corresponding to measured values of the one or more temperature-indicative parameters. For example,

in certain embodiments, the apparatus 10 comprises at least one temperature detector 80 configured to measure at least one of a body temperature of the subject and an ambient temperature of the subject. The at least one temperature detector 80 is further configured to generate at least one signal indicative of the at least one of the body temperature of the subject and the ambient temperature of the subject. In certain embodiments, the at least one temperature detector 80 can comprise a thermocouple, a thermistor, an infrared detector (e.g., a thermopile), or another type of thermometer known to persons of skill in the art. In certain embodiments, the at least one temperature detector 80 measures temperature to an accuracy of 0.05 degree Celsius or better.

[0048] In certain embodiments, the at least one temperature detector 80 is configured to measure both a body temperature of the subject and an ambient temperature of the subject. In certain embodiments, the measurement of the at least one of the body temperature and the ambient temperature is performed concurrently with detecting the power of the retro-reflected portion of the measurement light beam 32 or with detecting the retro-reflected portion of the reference light beam 34. In certain embodiments, the measurement of the at least one of the body temperature and the ambient temperature is performed concurrently with both detecting the power of the retro-reflected portion of the measurement light beam 32 and with detecting the retro-reflected portion of the reference light beam 34.

[0049] As used herein, the term "body temperature" has its broadest reasonable meaning, including but not limited to, a temperature of at least a portion of the subject's body. For example, in certain embodiments, the body temperature can be the subject's oral temperature, temporal artery or forehead temperature, eardrum temperature, earlobe temperature, finger temperature, skin temperature, or axillary temperature. In certain embodiments, the body temperature is measured from the same portion of the subject's body from which the optical measurements are made. In certain other embodiments, the body temperature is measured from a portion of the subject's body spaced from the portion of the subject's body from which the optical measurements are made. As used herein, the term "ambient temperature" has its broadest reasonable meaning, including but not limited to, a temperature of a region in proximity to the subject or generally surrounding the subject. For example, in certain embodiments, the ambient temperature can be the room temperature of the room in which the subject is located, the temperature in a region containing the apparatus 10 and the subject, or the temperature within two meters of the subject. The body temperature and the ambient temperature of certain embodiments are parameters which are indicative of the temperature of the portion of the subject's body from which the optical measurements are being made. Thus, in certain embodiments, the body and ambient temperatures are used as proxies for the temperature of the portion of the subject's body (e.g., subject's eye) from which the optical measurements are being made.

[0050] In certain embodiments, the apparatus 10 further comprises a computing system 60 configured to receive the first signal, the second signal, and the at least one signal. For example, the computing system 60 can comprise one or more inputs configured to receive the first signal, the second signal, and the at least one signal. In certain embodiments, the one or more inputs of the computing system 60 are also configured to receive a signal indicative of the power of the measurement light beam 32 incident on the subject's eye 40 and to receive a signal indicative of the power of the reference light beam 34 incident on the subject's eye 40.

[0051] The computing system 60 of certain embodiments is configured to calculate a value of an optically-measured parameter indicative of the interaction of the at least one light beam with the portion of the subject's body. For example, in certain embodiments, the computing system 60 comprises an electric circuit which is configured to calculate a first ratio of the first power and the power of the retro-reflected portion of the measurement light beam 32, to calculate a second ratio of the second power and the power of the retro-reflected portion of the reference light beam 34, to calculate a parameter dependent on the first ratio and the second ratio (e.g., a difference between the first ratio and the second ratio or a difference between a logarithm of the first ratio and a logarithm of the second ratio), and to determine a concentration of the substance in the subject's blood in response to the calculated parameter and to the at least one signal. Various configurations of the computing system 60 described herein are compatible with the example apparatus 10 of Figure 6.

[0052] When using the near-infrared wavelengths to measure the concentration of substances in the eye, the absorption due to water and possibly other substances can affect the measurements. In order to determine the desired concentration, certain embodiments described herein advantageously separate the absorption due to the substance of interest from the absorption due to other materials, mainly water. Certain embodiments described herein utilize light having one or more wavelengths that are absorbed primarily by water and the substance of interest (e.g., glucose). Certain embodiments described herein take into account that a second substance will have an absorption in a region of wavelengths close to or the same as the region of wavelengths absorbed by the substance of interest.

[0053] In certain embodiments, $I_0(\lambda)$ is defined as the power of the light beam having wavelength λ incident on the subject's eye 40 (e.g., as measured by the detector system 50), and $I_R(\lambda)$ is defined as the power of the retro-reflected light beam having wavelength λ received from the subject's eye (e.g., as measured by the detector system 50). The retro-reflected power $I_R(\lambda)$ can be expressed as:

$$I_R(\lambda) = R \cdot I_0(\lambda) \cdot e^{-\alpha(\lambda, c)x} \quad (1)$$

where R is an optical coefficient that includes the parameters that influence the retro-reflected power at the time of the measurement (e.g., reflectivity of the retina at wavelength λ , the size of the pupil, etc.), $\alpha(\lambda, c)$ is the absorption coefficient of the substance (e.g., glucose) as a function of wavelength λ and concentration c , and x is the optical pathlength through the material that contains the substance. This relation can be used to express the transmittance T_λ as:

$$T_\lambda = \ln\left(\frac{I_R(\lambda)}{I_0(\lambda)}\right) - \ln(R) = -\alpha(\lambda, c) \cdot x \quad (2)$$

[0054] To find the parameter that is to be correlated to the concentration of the substance (e.g., glucose), the absorption due to water is separated from the total absorption. The wavelength λ_1 is defined as the wavelength of light which is absorbed by both the substance and water, and the wavelength λ_2 is defined as the wavelength of light which is absorbed by water but not by the substance. The transmittance at these two wavelengths can be expressed as:

$$T_{\lambda_1} = \ln\left(\frac{I_R(\lambda_1)}{I_0(\lambda_1)}\right) - \ln(R) = (-\alpha(\lambda_1, c) \cdot x + \beta(\lambda_1) \cdot x) \quad (3)$$

$$T_{\lambda_2} = \ln\left(\frac{I_R(\lambda_2)}{I_0(\lambda_2)}\right) - \ln(R) = \beta(\lambda_2) \cdot x \quad (4)$$

where β is the absorption coefficient of water. Persons skilled in the art would recognize that logarithms in other bases (e.g., base 10) are also compatible with certain embodiments described herein.

[0055] The parameter T_f is defined as the difference between the transmittance at the two wavelengths of Equations (3) and (4), and can be expressed as:

$$T_f = T_{\lambda_1} - T_{\lambda_2} = \ln\left(\frac{I_R(\lambda_1)}{I_0(\lambda_1)}\right) - \ln\left(\frac{I_R(\lambda_2)}{I_0(\lambda_2)}\right) = -x \cdot (\Delta\beta(\lambda_1, \lambda_2) + \alpha(\lambda_1, c)) \quad (5)$$

where $\Delta\beta(\lambda_1, \lambda_2) = \beta(\lambda_1) - \beta(\lambda_2)$, which is a constant.

[0056] In deriving Equation (5), the parameter $\ln(R)$ was eliminated by subtracting the transmittance at the wavelength λ_2 from the transmittance at the wavelength λ_1 . This subtraction is advantageously made when the parameter $\ln(R)$ is stable in the wavelength region of λ_1 to λ_2 , such as when λ_1 and λ_2 are close to one another (e.g., differing by less than 0.2 microns). In certain embodiments, the value of $\Delta\beta(\lambda_1, \lambda_2)$ is selected to be small (e.g., by selecting the two wavelengths to have similar water absorption coefficients), in order to have a small amount of noise in the measurements.

[0057] In certain embodiments, the parameter T_f is calculated by the computing system 60 from the measured powers of the incident light beams and the retro-reflected light beams, and is correlated to the concentration of the substance (e.g., glucose) by accessing and referring to a previously-obtained correlation of the difference T_f and other non-invasively measured parameters (e.g., body temperature, ambient temperature) to clinically accepted invasive measurements. In certain embodiments, the resulting determination of the concentration of the substance in the subject's blood is stored in the memory, is displayed on the display, or both.

[0058] In certain embodiments, the computing system 60 is further configured to access an empirical correlation of the optically-measured parameter and the one or more temperature-indicative parameters to concentrations of the substance in blood. For example, in certain embodiments, the computing system 60 accesses one or more previously-determined correlations (e.g., stored in memory) of similar absorption measurements taken from a person's body (e.g., the eye) with empirical or clinical invasive measurements of the concentration of the substance (e.g., glucose) in the person's blood.

[0059] In certain embodiments, the computing system 60 is further configured to obtain a concentration of the substance

in the subject's blood using the empirical correlation. The obtained concentration corresponds to the value of the optically-measured parameter and the values of the one or more temperature-indicative parameters. For example, in certain embodiments, the computing system 60 uses the previously-determined correlation to equate or correlate the absorption measurements taken from the subject's body (e.g., the eye) to concentrations of the substance of interest in the subject's blood. In certain such embodiments, these calculations also include previously-determined correlations of other non-invasively measured parameters (e.g., body temperature, ambient temperature) with the empirical or clinical invasive measurements, and these other measured parameters, along with the absorption measurements taken from the subject's body, are used to determine the concentration of the substance of interest in the subject's blood. Other examples of non-invasively measured temperature-indicative parameters which can be used in certain embodiments described herein include, but are not limited to, ambient humidity and air flow in a region near the portion of the subject's body (e.g., the eye) from which the optical measurements are being made.

[0060] In certain embodiments, at least a portion of the correlation is stored in the memory of the apparatus 10 in the form of a look-up table which relates the concentration of the substance in a person's blood to values of the optically measured parameter (e.g., the difference T_f) and the other non-invasively measured parameters (e.g., body temperature, ambient temperature). Figure 9 schematically illustrates an example multi-parameter look-up table in accordance with certain embodiments described herein. The measured body temperature, the measured ambient temperature, and the optically measured parameter provide three coordinates to a location in the three-dimensional parameter space represented by the look-up table. This location contains a previously empirically-derived value of the concentration of the substance (e.g., glucose) corresponding to the values of these three coordinates. While Figure 9 schematically illustrates a three-dimensional parameter space, certain other embodiments utilize a parameter space with more than three dimensions. For example, air flow can be used in certain embodiments as a fourth coordinate which is used to specify a location in the parameter space containing a value of the concentration of the substance corresponding to the values of the measured body temperature, measured ambient temperature, measured air flow, and optically measured parameter.

[0061] In certain embodiments, at least a portion of the correlation is stored in the memory of the apparatus 10 in the form of one or more formulae which relates the concentration of the substance in a person's blood to values of the difference T_f and the other non-invasively measured parameters (e.g., body temperature, ambient temperature). For example, in certain embodiments, the correlation can be stored as a plurality of linear formulae which interpolate between empirical values of the non-invasively measured parameters to provide estimates of the concentration of the substance.

[0062] In certain embodiments, the correlation is an empirical correlation which is the result of a previously-performed study of invasive measurements of the concentrations of the substance in the blood of members of a study group with the non-invasive measurements of the difference T_f and the other non-invasively measured parameters (e.g., body temperature, ambient temperature). For example, the invasive measurements can comprise glucose concentration measurements of blood samples extracted from the members of the study group and these invasive measurements can be correlated with substantially concurrent non-invasive measurements of the difference T_f and the other non-invasively measured parameters (e.g., body temperature, ambient temperature) taken from the members of the study group. In certain embodiments, the empirical study includes measurements from a statistically representative group of people selected to represent a larger population of people for whom concentration measurements are to be made. The group of people in certain embodiments can include both male and female individuals of various ages, weights, and having various physical conditions (e.g., diabetic and non-diabetic individuals). In certain embodiments, the empirical study includes measurements made from these people under a wide variety of conditions. For example, the optically measured parameter, the temperature-indicative parameters (e.g., the body temperature and the ambient temperature), and the invasively-measured concentration are measured over a range of ambient temperatures for which the system is anticipated to be used (e.g., 16 degrees Celsius to 36 degrees Celsius). In certain embodiments, the optically measured parameter, the temperature-indicative parameters, and the invasively-measured concentration are measured over ranges of other variables (e.g., times of day, intervals before and after meals) in order to provide a large database from which correlations of the invasively-measured concentration with the optically measured parameter and the temperature-indicative parameters can reliably be obtained. Thus, the study can be used to provide the correlation of the substance in a person's blood to values of the optically-measured parameter indicative of the concentration of the substance (e.g., the difference T_f) and the other non-invasively measured parameters (e.g., body temperature, ambient temperature). In certain embodiments, a look-up table comprising at least a portion of the resultant correlation can be stored in a computer-readable medium (e.g., read-only memory, dynamic random-access memory, flash memory, hard disk drive, compact disk, digital video disk). In certain embodiments, one or more formulae comprising at least a portion of the resultant correlation can be stored in a computer-readable medium.

[0063] The results of these measurements in certain embodiments are averaged to provide a correlation representative of an average individual. In certain embodiments, the probability distribution of the values from the group can have a sufficiently large standard deviation, indicating that there are significant variations among individuals. In certain such embodiments, the apparatus can be individually calibrated to a particular subject from whom the optical measurements

of the concentration of the substance are to be made. For example, in certain embodiments, an invasive measurement (e.g., a blood droplet glucose measurement) from a subject is used to calibrate subsequent non-invasive optical determinations of the concentration of the substance. Such an invasive measurement from the particular subject can be used to normalize the results obtained from that subject to the average correlation (e.g., by providing a normalization factor in the formula). For example, a measurement of a glucose concentration of 120 mg/dl made from a subject under conditions for which the expected measurement made from an average individual would be 100 mg/dl, a factor of 1.2 can be used to normalize the subsequent determinations of the glucose concentration of the subject. In this way, certain embodiments advantageously provide periodic non-invasive measurements of the concentration while reducing the number of invasive measurements that would otherwise be needed.

[0064] In certain embodiments, additional substances with absorptions at the wavelengths used can be accounted for by utilizing additional measurements at additional wavelengths. These measurements are then used with additional equations similar to those described above to determine the unknown values.

[0065] Although the invention has been described in terms of certain embodiments, other embodiments that are apparent to those of ordinary skill in the art, including embodiments which do not provide all of the features and advantages set forth herein, are also within the scope of this invention. Accordingly, the scope of the invention is defined by the claims that follow.

Claims

1. A method of determining the concentration of a substance in a subject's blood, the method comprising:

measuring an interaction of at least one light beam with a portion of the subject's body, the measuring of the interaction of the at least one light beam including measuring reflections of a reference light beam (34) and of a measurement light beam (32) from the portion of the subject's body;

calculating a value of an optically-measured parameter indicative of the interaction of the at least one light beam with the substance in the portion of the subject's body, the optically measured parameter including a reference ratio of a reflected power of the reference light beam (34) to an incident power of the reference light beam (34) and a measurement ratio of a reflected power of the measurement light beam (32) to an incident power of the measurement light beam (32);

measuring values of temperature-indicative parameters corresponding to a temperature of the portion of the subject's body, the temperature-indicative parameters including both a body temperature of the subject and an ambient temperature of the subject;

accessing an empirical correlation of the optically-measured parameter and the temperature-indicative parameters to concentrations of the substance in blood; and

obtaining a concentration of the substance in the subject's blood using the empirical correlation, wherein the concentration corresponds to the value of the optically-measured parameter and the values of the temperature-indicative parameters.

2. The method of claim 1, wherein the substance is glucose.

3. The method of claim 1 or 2, wherein measuring the interaction of the at least one light beam includes measuring an absorption of the at least one light beam by the portion of the subject's body, a transmittance of the at least one light beam through the portion of the subject's body, or performing Raman spectroscopy on the portion of the subject's body.

4. The method of claim 1 or 2, wherein the measurement and reference light beams (32, 34) are retro-reflected from a retina (42) of an eye (40).

5. The method of claim 4, wherein the measurement and reference light beams are transmitted from and detected by apparatus (10) located at least 100 mm from the eye (40) of the user, such that the received light beam is mainly light from the retina (42) and reception of other reflections is avoided.

6. The method of claim 2, wherein the measurement light beam (32) exhibits a wavelength in a range between about 920 nanometers and about 980 nanometers, which is absorbed by the substance, and the reference light beam (34) exhibits a wavelength in a range between about 800 nanometers and about 905 nanometers, which is not substantially absorbed by the substance.

7. The method of any preceding claim, wherein the measuring values of the one or more temperature-indicative parameters is performed non-invasively.

8. The method of any preceding claim, wherein the empirical correlation comprises one or more formulae relating concentrations of the substance in a person's blood to values of the optically-measured parameter and of both a body temperature of the subject and an ambient temperature of the subject.

9. The method of any preceding claim, wherein the empirical correlation comprises a look-up table relating concentrations of the substance in a subject's blood to values of the optically-measured parameter and of both a body temperature of the subject and an ambient temperature of the subject.

10. The method of claim 1, further comprising a method of determining the empirical correlation of the concentration of the substance in a person's blood with a plurality of parameters, the further method including:

using invasively measured values of the concentration of the substance in the blood of a plurality of people at a plurality of conditions, the plurality of people statistically representative of a larger population of people; non-invasively optically-measuring values of a parameter from the plurality of people at the plurality of conditions, wherein the value of the optically-measured parameter measured for a portion of a person's body is indicative of the concentration of the substance in the person's blood; measuring values of one or more temperature-indicative parameters for the plurality of people at the plurality of conditions, the one or more temperature-indicative parameters corresponding to a temperature of the portion of the person's body; and generating the empirical correlation by correlating the measured values of the optically-measured parameter and the measured values of the one or more temperature-indicative to the measured values of the concentration of the substance in the blood of the plurality of people.

11. The method of claim 10, wherein using invasively measured values of the concentration of the substance in blood comprises measuring glucose concentration of blood samples previously extracted from the plurality of people.

12. The method of any preceding claim, further comprising the step of storing at least a portion of the correlation in a computer-readable medium (72).

13. A computing system for determining the concentration of a substance in a subject's blood, the computing system comprising:

a detector system (50) for measuring an interaction of at least one light beam with a portion of the subject's body, the measuring of the interaction of the at least one light beam including measuring reflections of a reference light beam (34) and of a measurement light beam (32) from the portion of the subject's body; means for calculating a value of an optically-measured parameter indicative of the interaction of the at least one light beam with the substance in the portion of the subject's body; a temperature detector (80) for measuring values of temperature-indicative parameters corresponding to a temperature of the portion of the subject's body, the temperature-indicative parameters including both a body temperature of the subject and an ambient temperature of the subject; means for accessing an empirical correlation of the optically-measured parameter and the temperature-indicative parameters to concentrations of the substance in blood and obtaining a concentration of the substance in the subject's blood using the empirical correlation, wherein the concentration corresponds to the value of the optically-measured parameter and the values of the temperature-indicative parameters and wherein said empirical correlation is comprised in the computing system.

14. The system of Claim 13, wherein the calculating means comprises a central processing unit (61), and the accessing means comprises a computer-readable medium (72) in which the empirical correlation is stored.

15. The system of claim 13, wherein the empirical correlation is stored in the computer-readable medium (72) as a look-up table or as one or more formulae.

Patentansprüche

1. Verfahren zum Bestimmen der Konzentration von einer Substanz in einem Blut von einem Subjekt, wobei das Verfahren umfasst:

Messen von einer Interaktion von mindestens einem Lichtstrahl mit einem Körperteil von dem Subjekt, wobei das Messen von der Interaktion von dem mindestens einen Lichtstrahl das Messen der Reflexionen von einem Referenzlichtstrahl (34) und einem Messungslichtstrahl (32) von dem Körperteil von dem Subjekt umfasst;
Berechnen von einem Wert von einem optisch gemessenen Parameter, der die Interaktion von dem mindestens einen Lichtstrahl mit der Substanz in dem Körperteil von dem Subjekt anzeigt, wobei der optisch gemessene Parameter ein Referenzverhältnis von einer reflektierten Energie von dem Referenzlichtstrahl (34) zu einer einfallenden Energie von dem Referenzlichtstrahl (34) und ein Messungsverhältnis von einer reflektierten Energie von dem Messungslichtstrahl (32) zu einer einfallenden Energie von dem Messungslichtstrahl (32) umfasst;
Messen der Werte von temperaturanzeigenden Parametern, die einer Temperatur von dem Körperteil von dem Subjekt entsprechen, wobei die temperaturanzeigenden Parameter sowohl eine Körpertemperatur von dem Subjekt als auch eine Umgebungstemperatur von dem Subjekt umfassen;
Zugreifen auf eine empirische Korrelation von dem optisch gemessenen Parameter und den temperaturanzeigenden Parametern mit den Konzentrationen von der Substanz im Blut; und
Erhalten von einer Konzentration für die Substanz in dem Blut des Subjekts unter Verwendung der empirischen Korrelation, wobei die Konzentration dem Wert von dem optisch gemessenen Parameter und den Werten von den temperaturanzeigenden Parametern entspricht.

2. Verfahren nach Anspruch 1, wobei die Substanz Glukose ist.

3. Verfahren nach Anspruch 1 oder 2, wobei die Messung von der Interaktion von dem mindestens einen Lichtstrahl die Messung einer Absorption von dem mindestens einen Lichtstrahl durch den Körperteil von dem Subjekt, die Messung einer Transmission von dem mindestens einen Lichtstrahl durch den Körperteil von dem Subjekts oder das Durchführen von einer Raman-Spektroskopie an dem Körperteil des Subjekts umfasst.

4. Verfahren nach Anspruch 1 oder 2, wobei die Messungs- und die Referenzlichtstrahlen (32, 34) von einer Retina (42) eines Auges (40) retroreflektiert werden.

5. Verfahren nach Anspruch 4, wobei die Messungs- und die Referenzlichtstrahlen von einem Apparat (10) ausgesendet und detektiert werden, der mindestens 100 mm von dem Auge (40) eines Benutzers entfernt angeordnet ist, sodass der empfangene Lichtstrahl hauptsächlich Licht von der Retina (42) ist und der Empfang von anderen Reflexionen vermieden wird.

6. Verfahren nach Anspruch 2, wobei der Messungslichtstrahl (32) eine Wellenlänge in einem Bereich zwischen etwa 920 Nanometern und etwa 980 Nanometern aufweist, welche von der Substanz absorbiert wird, und der Referenzlichtstrahl (34) eine Wellenlänge in einem Bereich zwischen etwa 800 Nanometern und etwa 905 Nanometern aufweist, welche nicht wesentlich von der Substanz absorbiert wird.

7. Verfahren nach einem der vorhergehenden Ansprüche, wobei die Messung der Werte von den ein oder mehreren temperaturanzeigenden Parametern nicht-invasiv durchgeführt wird.

8. Verfahren nach einem der vorhergehenden Ansprüche, wobei die empirische Korrelation ein oder mehrere Formeln umfasst, die Konzentrationen von der Substanz in einem Blut von einer Person mit Werten von dem optisch gemessenen Parameter und von sowohl einer Körpertemperatur von dem Subjekt als auch von einer Umgebungstemperatur von dem Subjekt in Beziehung setzt.

9. Verfahren nach einem der vorhergehenden Ansprüche, wobei die empirische Korrelation eine Nachschlagetabelle umfasst, die Konzentrationen von der Substanz in einem Blut von einer Person mit Werten von dem optisch gemessenen Parameter und von sowohl einer Körpertemperatur von dem Subjekt als auch von einer Umgebungstemperatur von dem Subjekt in Beziehung setzt.

10. Verfahren nach Anspruch 1, ferner umfassend ein Verfahren zur Bestimmung der empirischen Korrelation von der Konzentration der Substanz in einem Blut von einer Person mit einer Vielzahl von Parametern, wobei das Verfahren ferner umfasst:

Verwendung von invasiv gemessenen Werten für die Konzentration von der Substanz in dem Blut von einer Vielzahl von Personen bei einer Vielzahl von Konditionen, wobei die Vielzahl von Personen für eine größere Population von Personen statistisch signifikant ist;

nicht-invasiv optisch gemessene Werte von einem Parameter für die Vielzahl von Personen bei einer Vielzahl von Konditionen, wobei der Wert von dem optisch gemessenen Parameter, der für einen Körperteil von einer Person gemessen wird, die Konzentration von der Substanz in dem Blut von der Person anzeigt;

Messen der Werte von ein oder mehreren temperaturanzeigenden Parametern von der Vielzahl von Personen bei der Vielzahl von Konditionen, wobei die ein oder mehreren temperaturanzeigenden Parameter einer Temperatur von dem Körperteil der Person entsprechen; und

Erzeugen der empirischen Korrelation, indem die gemessenen Werte von dem optisch gemessenen Parameter und die gemessenen Werte von den ein oder mehreren temperaturanzeigenden Parametern mit den gemessenen Werten für die Konzentration von der Substanz in dem Blut von der Vielzahl von Personen korreliert werden.

11. Verfahren nach Anspruch 10, wobei die Verwendung von invasiv gemessenen Werten für die Konzentration von der Substanz im Blut die Messung der Glukosekonzentration von Blutproben umfasst, die vorher aus einer Vielzahl von Personen entnommen wurden.

12. Verfahren nach einem der vorhergehenden Ansprüche, ferner umfassend den Schritt des Speicherns von mindestens einem Teil der Korrelation in einem computerlesbaren Medium (72).

13. Computersystem zum Bestimmen der Konzentration von einer Substanz in einem Blut von einem Subjekt, wobei das Computersystem umfasst:

ein Detektorsystem zum Messen von einer Interaktion von mindestens einem Lichtstrahl mit einem Körperteil von dem Subjekt, wobei das Messen von der Interaktion von dem mindestens einen Lichtstrahl das Messen der Reflexionen von einem Referenzlichtstrahl (34) und von einem Messungslichtstrahl (32) von dem Körperteil von dem Subjekt umfasst;

ein Mittel zum Berechnen von einem Wert von einem optisch gemessenen Parameter, der die Interaktion von dem mindestens einen Lichtstrahl mit der Substanz in dem Körperteil des Subjekts anzeigt;

einen Temperaturdetektor (80) zum Messen der Werte von temperaturanzeigenden Parametern, die einer Temperatur von dem Körperteil von dem Subjekts entsprechen, wobei die temperaturanzeigenden Parameter sowohl eine Körpertemperatur von dem Subjekt als auch eine Umgebungstemperatur von dem Subjekt umfassen;

ein Mittel zum Zugreifen auf eine empirische Korrelation von dem optisch gemessenen Parametern und den temperaturanzeigenden Parametern mit den Konzentrationen von der Substanz im Blut und zum Erhalten von einer Konzentration für die Substanz in dem Blut von dem Subjekt unter Verwendung der empirischen Korrelation, wobei die Konzentration dem Wert von dem optisch gemessenen Parameter und den Werten von den temperaturanzeigenden Parametern entspricht und wobei die empirische Korrelation in dem Computersystem umfasst ist.

14. System nach Anspruch 13, wobei das Berechnungsmittel eine zentrale Prozessierungseinheit (61) umfasst und das Zugreifmittel ein computerlesbares Medium (72) umfasst, in dem die empirische Korrelation gespeichert ist.

15. System nach Anspruch 13, wobei die empirische Korrelation in dem computerlesbaren Medium (72) als eine Nachschlagetabelle oder als ein oder mehrere Formeln gespeichert ist.

Revendications

1. Procédé de détermination de la concentration d'une substance dans le sang d'un sujet, le procédé comprenant :

la mesure d'une interaction d'au moins un faisceau de lumière avec une partie du corps du sujet, la mesure de l'interaction du au moins un faisceau de lumière incluant la mesure de réflexions d'un faisceau de lumière de référence (34) et d'un faisceau de lumière de mesure (32) à partir de la partie du corps du sujet ;

le calcul d'une valeur d'un paramètre mesuré optiquement indicatif de l'interaction du au moins un faisceau de lumière avec la substance dans la partie du corps du sujet, le paramètre mesuré optiquement incluant un rapport de référence entre une puissance réfléchie du faisceau de lumière de référence (34) et une puissance incidente

du faisceau de lumière de référence (34) et un rapport de mesure entre une puissance réfléchie du faisceau de lumière de mesure (32) et une puissance incidente du faisceau de lumière de mesure (32) ;
la mesure de valeurs de paramètres indicateurs de température correspondant à une température de la partie du corps du sujet, les paramètres indicateurs de température incluant à la fois une température corporelle du sujet et une température ambiante du sujet ;
l'accès à une corrélation empirique du paramètre mesuré optiquement et des paramètres indicateurs de température avec des concentrations de la substance dans le sang ; et
l'obtention d'une concentration de la substance dans le sang du sujet en utilisant la corrélation empirique, la concentration correspondant à la valeur du paramètre mesuré optiquement et aux valeurs des paramètres indicateurs de température.

2. Procédé selon la revendication 1, dans lequel la substance est le glucose.

3. Procédé selon la revendication 1 ou 2, dans lequel la mesure de l'interaction du au moins un faisceau de lumière inclut la mesure d'une absorption du au moins un faisceau de lumière par la partie du corps du sujet, une transmission du au moins un faisceau de lumière à travers la partie du corps du sujet, où la réalisation d'une spectroscopie Raman sur la partie du corps du sujet.

4. Procédé selon la revendication 1 ou 2, dans lequel les faisceaux de lumière de mesure et de référence (32, 34) sont rétro réfléchis par une rétine (42) d'un oeil (40).

5. Procédé selon la revendication 4, dans lequel les faisceaux de lumière de mesure et de référence sont transmis à partir de et détectés par un appareil (10) situé à au moins 100 mm de l'oeil (40) de l'utilisateur, de sorte que le faisceau de lumière reçu soit principalement la lumière provenant de la rétine (42) et que la réception d'autres réflexions soit évitée.

6. Procédé selon la revendication 2, dans lequel le faisceau de lumière de mesure (32) présente une longueur d'onde dans une plage entre environ 920 nanomètres et environ 980 nanomètres, qui est absorbée par la substance, et le faisceau de lumière de référence (34) présente une longueur d'onde dans une plage entre environ 800 nanomètres et environ 905 nanomètres, qui n'est pas absorbée de façon substantielle par la substance.

7. Procédé selon l'une quelconque des revendications précédentes, dans lequel la mesure des valeurs des un ou plusieurs paramètres indicateurs de température est réalisée de façon non invasive.

8. Procédé selon l'une quelconque des revendications précédentes, dans lequel la corrélation empirique comprend une ou plusieurs formules associant des concentrations de la substance dans le sang d'une personne à des valeurs du paramètre mesuré optiquement et à la fois d'une température corporelle du sujet et d'une température ambiante du sujet.

9. Procédé selon l'une quelconque des revendications précédentes, dans lequel la corrélation empirique comprend une table de consultation associant des concentrations de la substance dans le sang d'un sujet à des valeurs du paramètre mesuré optiquement et à la fois d'une température corporelle du sujet et d'une température ambiante du sujet.

10. Procédé selon la revendication 1, comprenant en outre un procédé de détermination de la corrélation empirique de la concentration de la substance dans le sang d'une personne avec une pluralité de paramètres, le procédé supplémentaire comprenant:

l'utilisation de valeurs, mesurées de façon invasive, de la concentration de la substance dans le sang d'une pluralité de personnes dans une pluralité de conditions, la pluralité de personnes étant statistiquement représentative d'une plus grande population de personnes ;
la mesure optique non invasive de valeurs d'un paramètre à partir de la pluralité de personnes dans la pluralité de conditions, la valeur du paramètre mesuré optiquement pour une partie du corps d'une personne étant indicative de la concentration de la substance dans le sang de la personne ;
la mesure de valeurs d'un ou plusieurs paramètres indicateurs de température pour la pluralité de personnes dans la pluralité de conditions, les un ou plusieurs paramètres indicateurs de température correspondant à une température de la partie du corps de la personne ; et
la génération de la corrélation empirique en corrélant les valeurs mesurées du paramètre mesuré optiquement

et les valeurs mesurées des un ou plusieurs paramètres indicateurs de température avec les valeurs mesurées de la concentration de la substance dans le sang de la pluralité de personnes.

5 11. Procédé selon la revendication 10, dans lequel l'utilisation de valeurs, mesurées de façon invasive, de la concentration de la substance dans le sang comprend la mesure de la concentration en glucose d'échantillons de sang prélevés précédemment chez la pluralité de personnes.

10 12. Procédé selon l'une quelconque des revendications précédentes, comprenant en outre l'étape de stockage d'au moins une partie de la corrélation dans un support lisible par ordinateur (72).

13. Système informatique pour déterminer la concentration d'une substance dans le sang d'un sujet, le système informatique comprenant :

15 un système de détection (50) destiné à mesurer une interaction d'au moins un faisceau de lumière avec une partie du corps du sujet, la mesure de l'interaction du au moins un faisceau de lumière incluant la mesure de réflexions d'un faisceau de lumière de référence (34) et d'un faisceau de lumière de mesure (32) à partir de la partie du corps du sujet ;

un moyen permettant de calculer une valeur d'un paramètre mesuré optiquement indicatif de l'interaction du au moins un faisceau de lumière avec la substance dans la partie du corps du sujet ;

20 un détecteur de température (80) destiné à mesurer des valeurs de paramètres indicateurs de température correspondant à une température de la partie du corps du sujet, les paramètres indicateurs de température incluant à la fois une température corporelle du sujet et une température ambiante du sujet ;

25 un moyen permettant d'accéder à une corrélation empirique du paramètre mesuré optiquement et des paramètres indicateurs de température avec des concentrations de la substance dans le sang et l'obtention d'une concentration de la substance dans le sang d'un sujet en utilisant la corrélation empirique, la concentration correspondant à la valeur du paramètre mesuré optiquement et aux valeurs des paramètres indicateurs de température et ladite corrélation empirique étant comprise dans le système informatique.

30 14. Système selon la revendication 13, dans lequel le moyen de calcul comprend une unité de traitement centrale (61), et le moyen d'accès comprend un support lisible par ordinateur (72) dans lequel la corrélation empirique est stockée.

15 15. Système selon la revendication 13, dans lequel la corrélation empirique est stockée dans le support lisible par ordinateur (72) sous la forme d'une table de consultation ou d'une ou plusieurs formules.

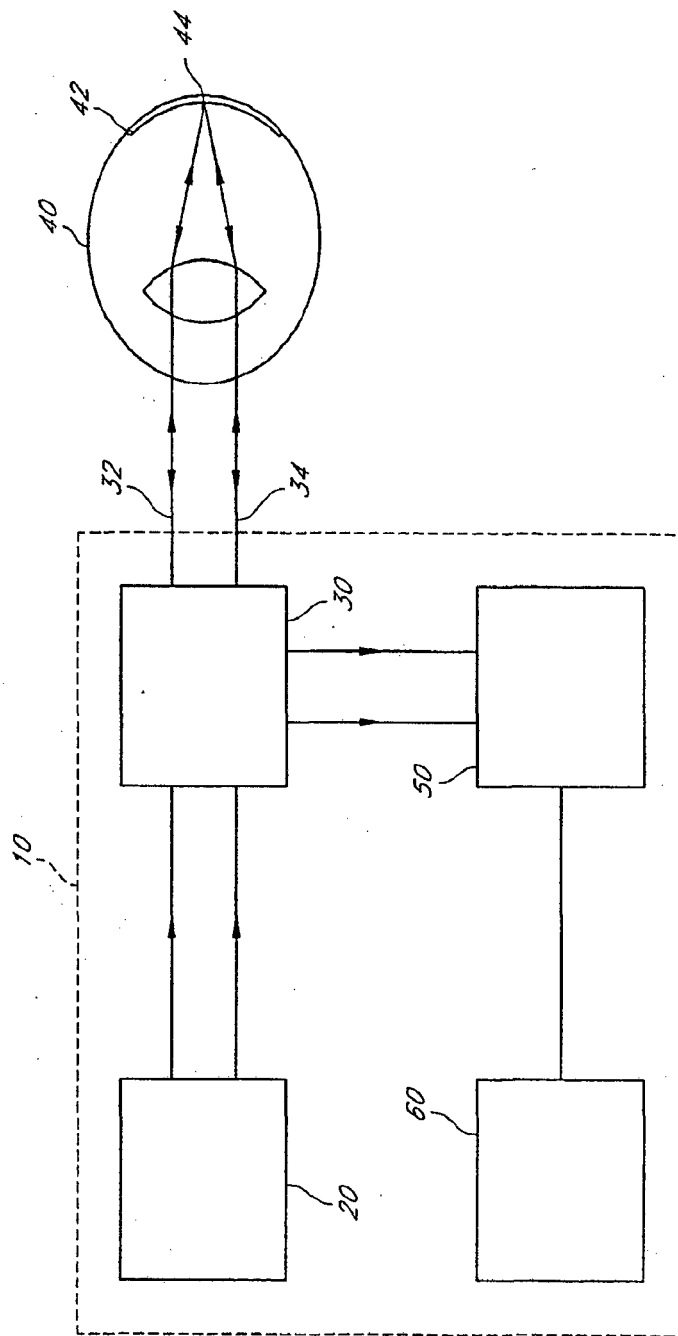


FIG. 1

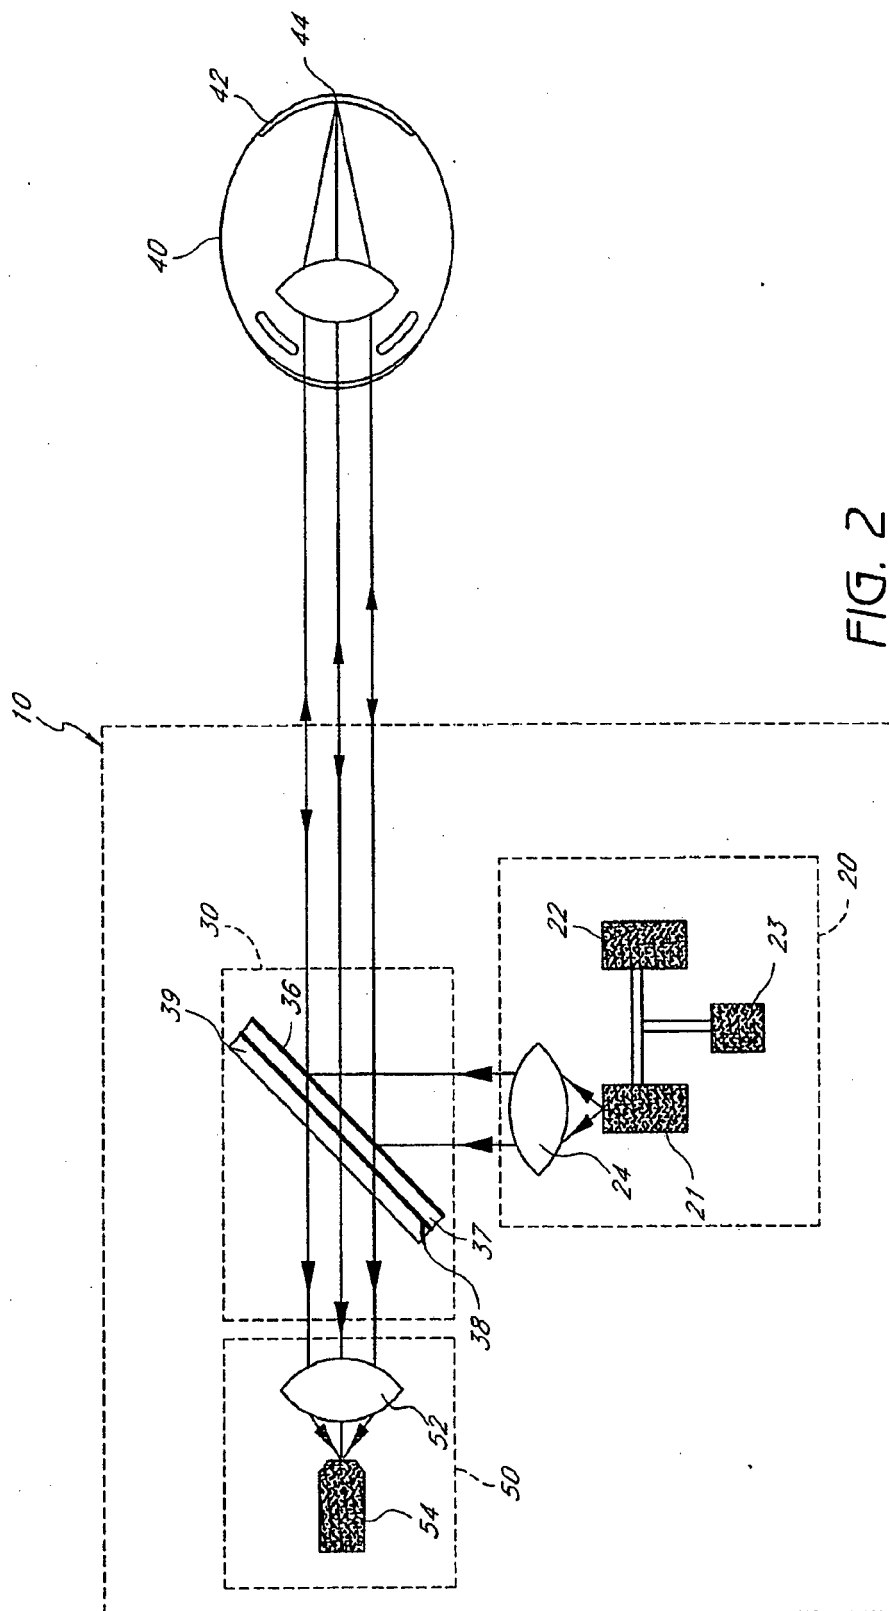


FIG. 2

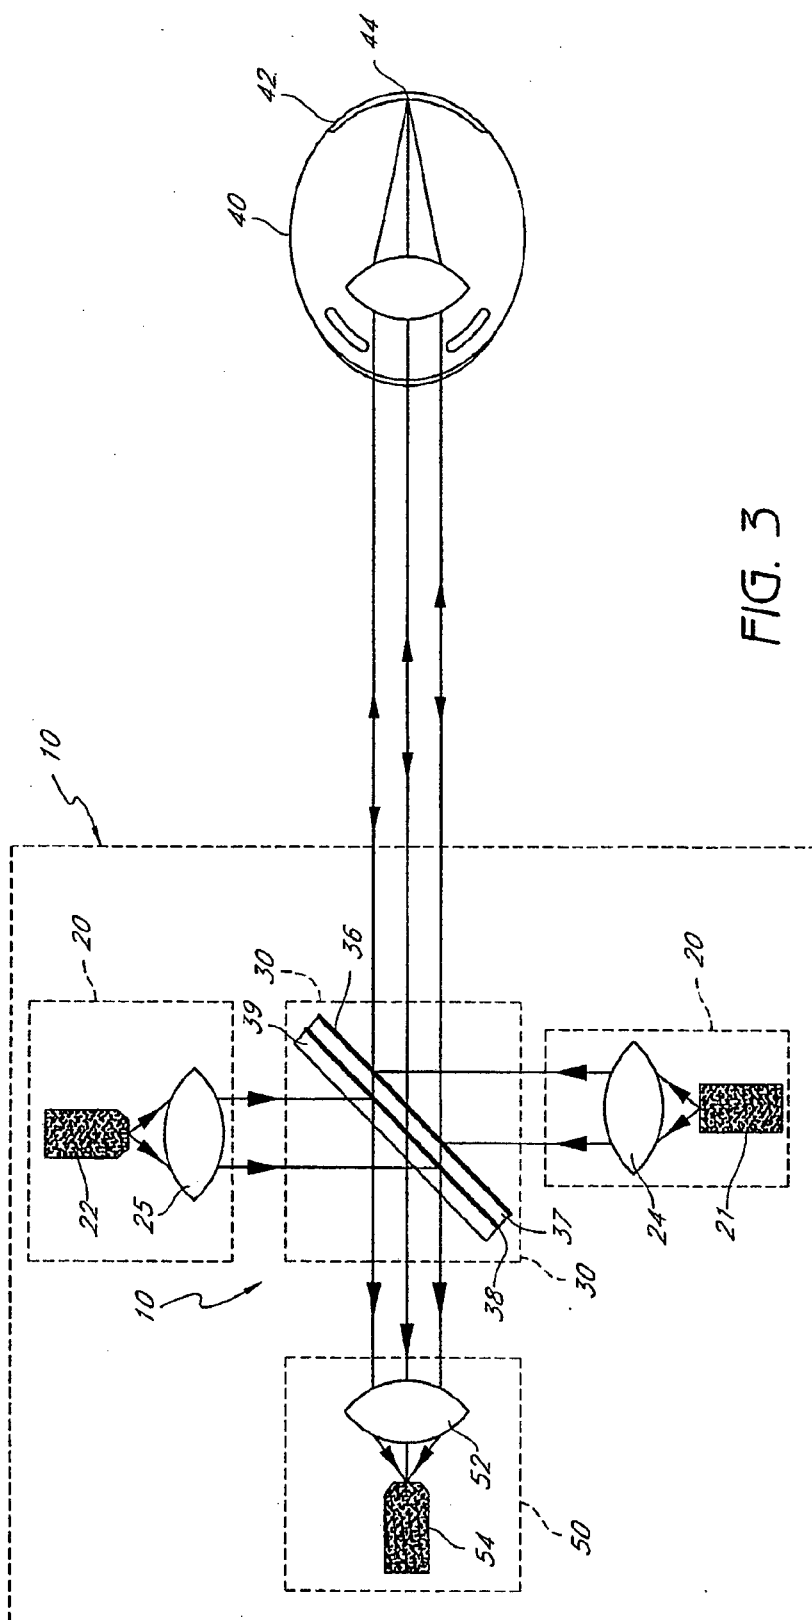


FIG. 3

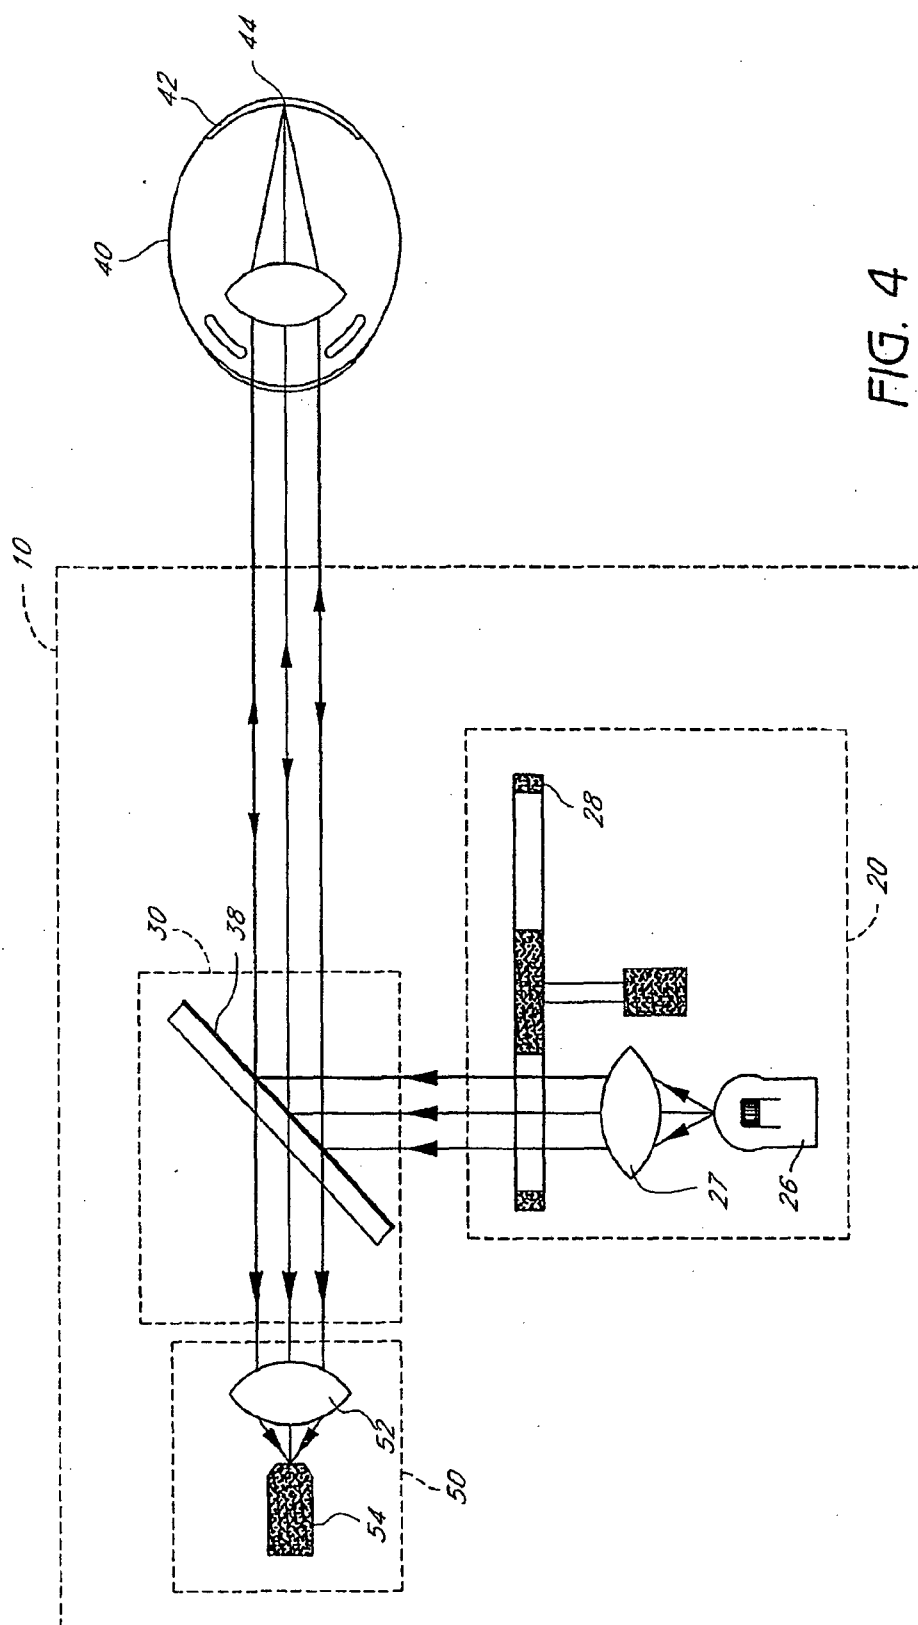


FIG. 4

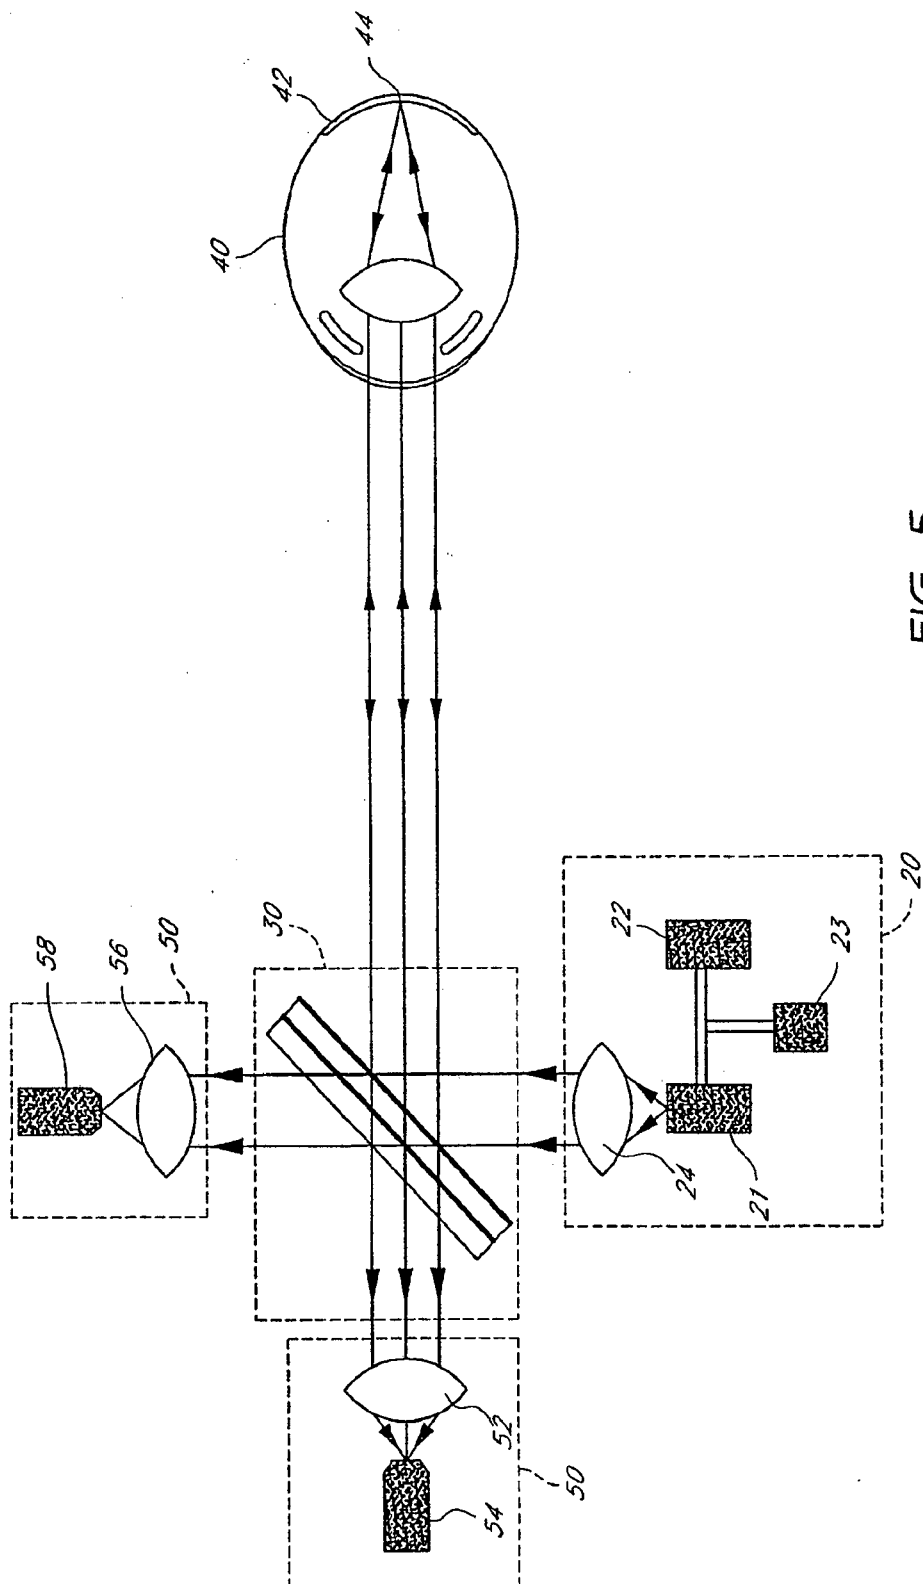


FIG. 5

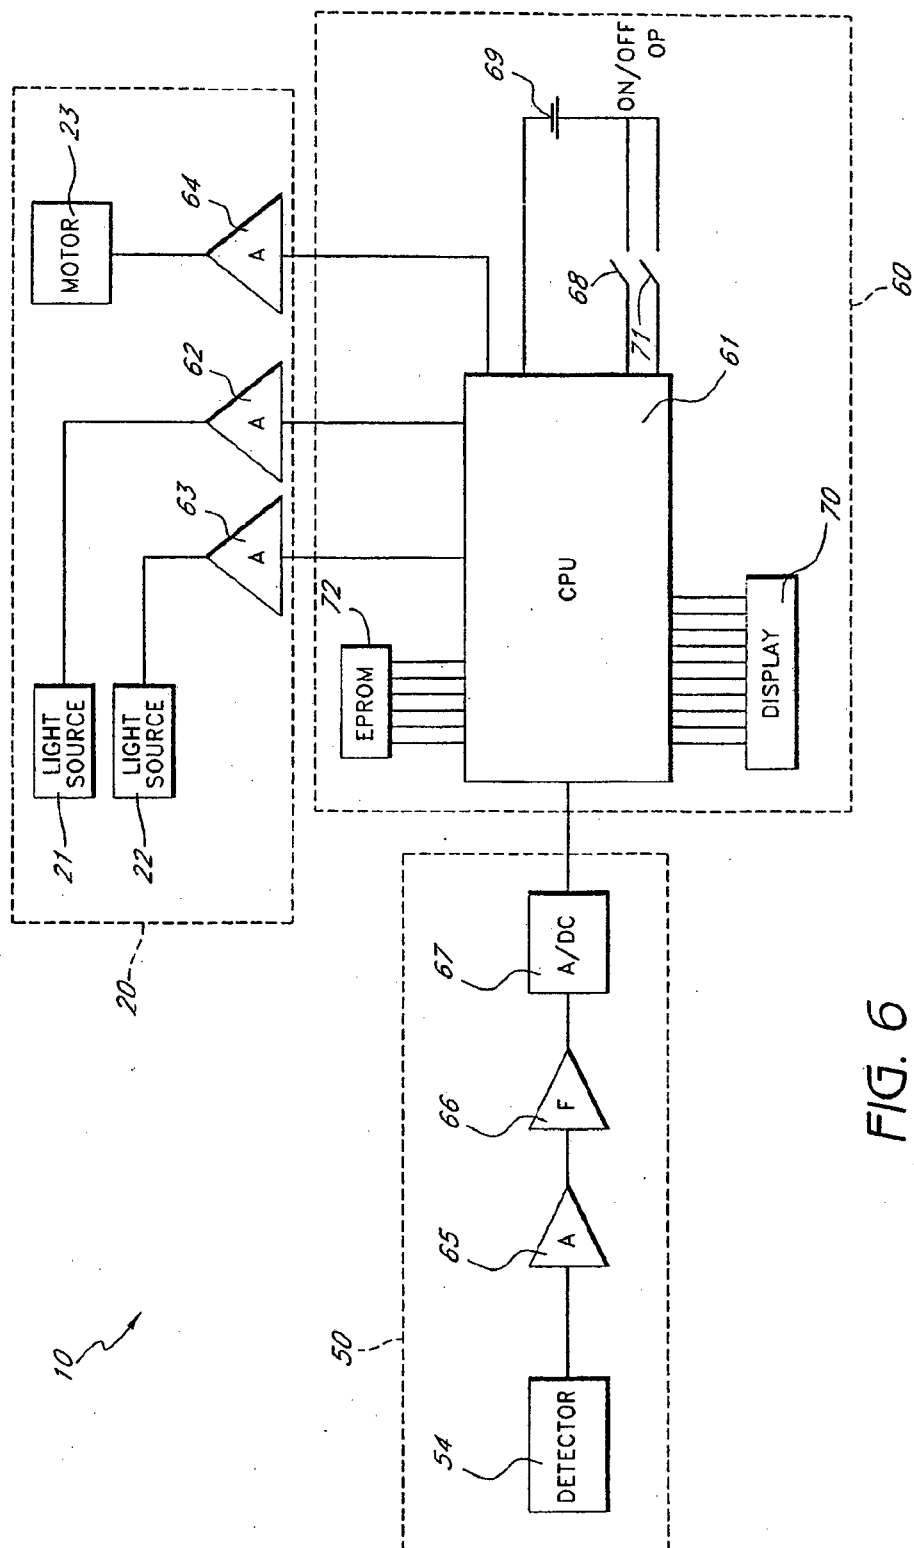
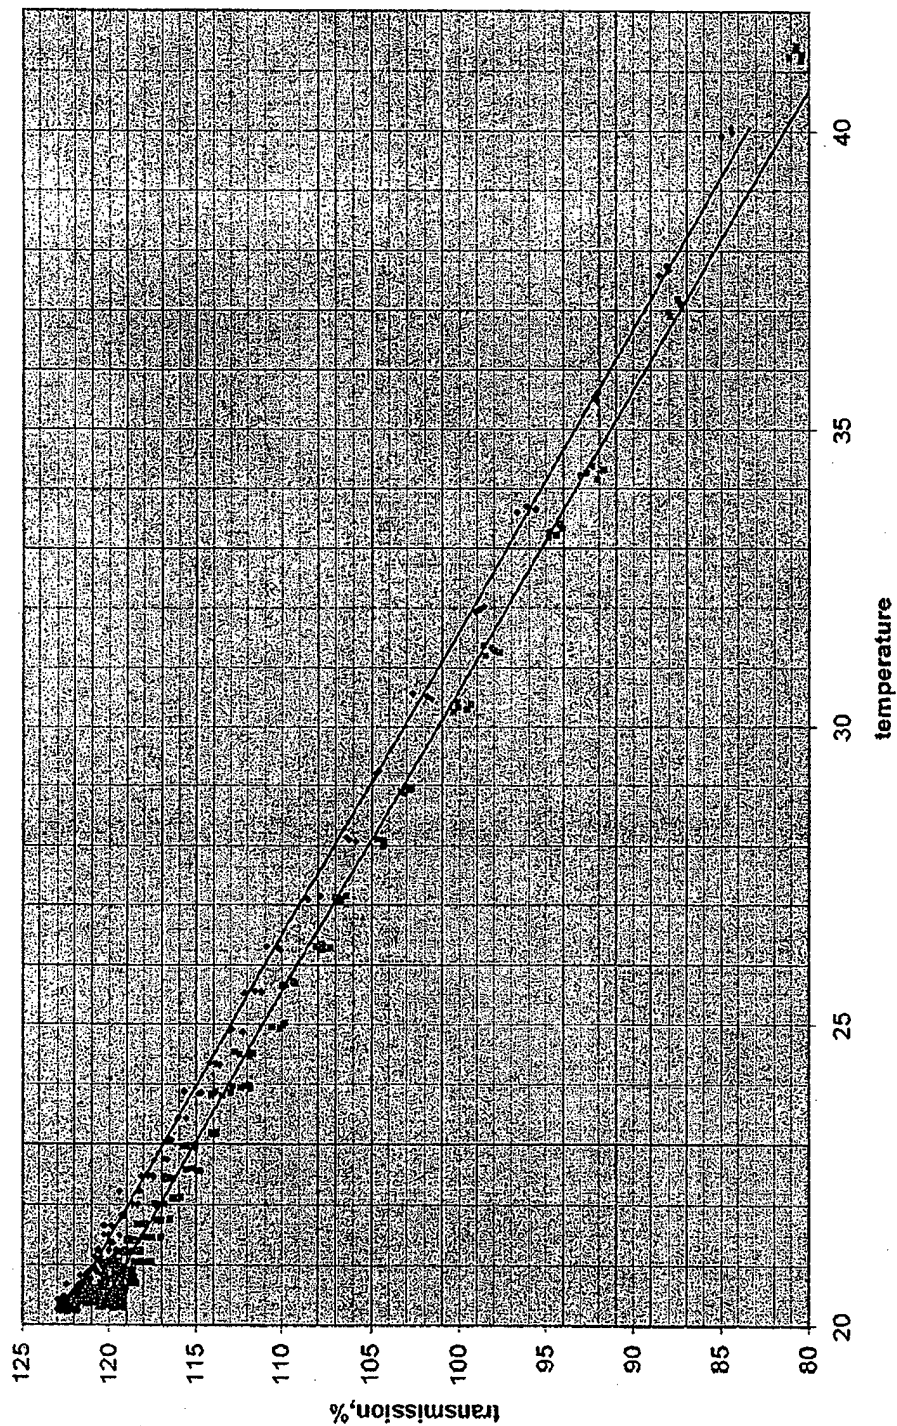
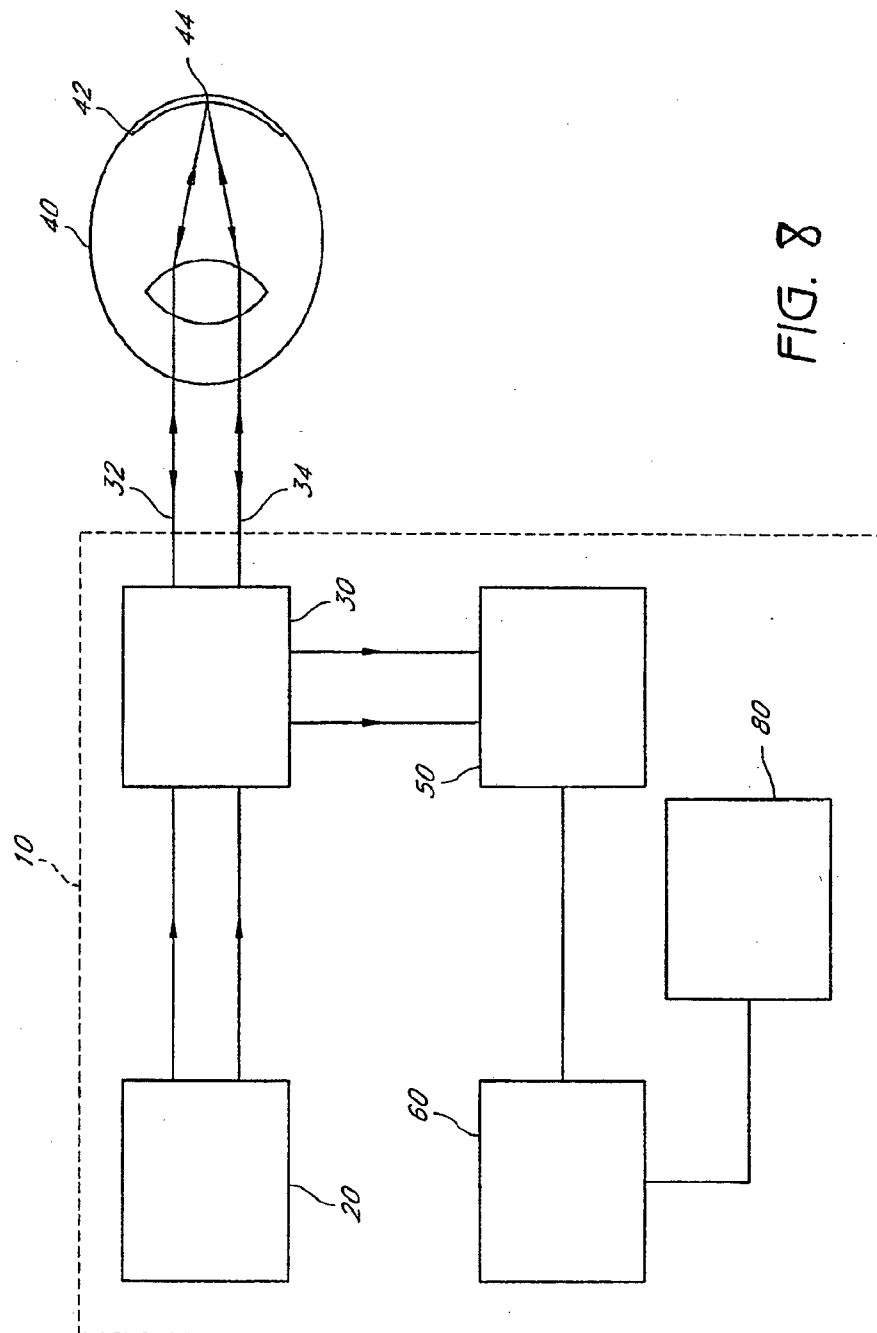


FIG. 6

Figure 7:

Transmission versus cuvette temperature





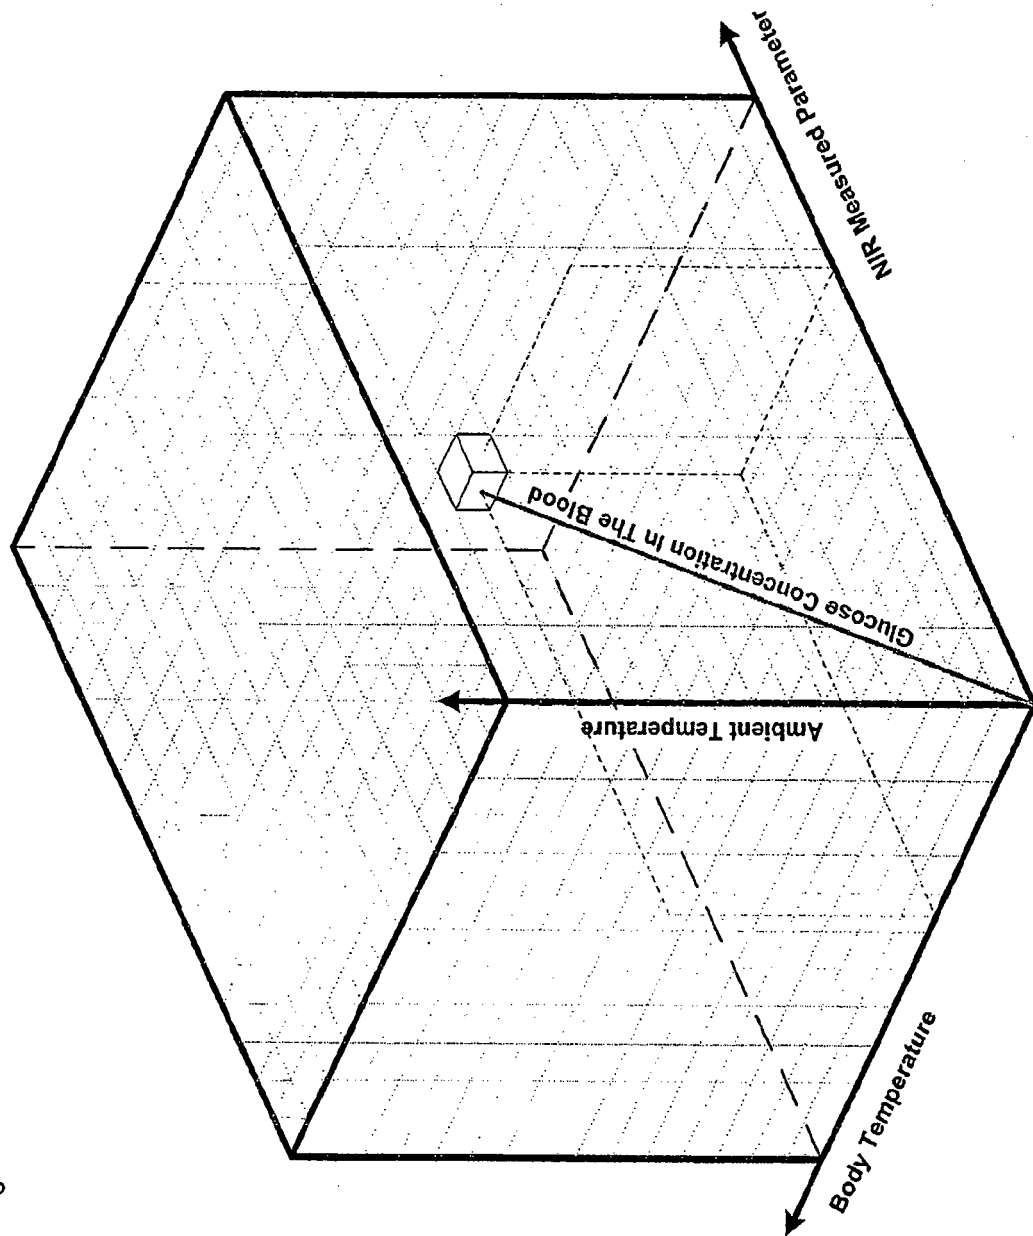


Figure 9:

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6494576 B [0003]
- US 5820557 B [0003]
- US 6226089 B [0003]

专利名称(译)	用于非侵入性地测量受试者血液中物质浓度的装置和方法		
公开(公告)号	EP2249694B1	公开(公告)日	2015-09-02
申请号	EP2009711443	申请日	2009-01-26
[标]申请(专利权)人(译)	格鲁科威斯塔有限公司		
申请(专利权)人(译)	GLUCO VISTA LLC		
当前申请(专利权)人(译)	GLUCO VISTA LLC		
[标]发明人	GERLITZ JONATHAN		
发明人	GERLITZ, JONATHAN		
IPC分类号	A61B5/00		
CPC分类号	A61B5/1455 A61B5/14532		
优先权	12/029339 2008-02-11 US		
其他公开文献	EP2249694A1		
外部链接	Espacenet		

摘要(译)

方法确定受试者血液中物质的浓度。该方法包括测量至少一个光束与受试者身体的一部分的相互作用。该方法还包括计算光学测量参数的值，该参数指示至少一个光束与受试者身体部分中的物质的相互作用。该方法还包括测量对应于受试者身体部分的温度的一个或多个温度指示参数的值。该方法还包括获得光学测量参数和一个或多个温度指示参数的经验相关性与血液中物质的浓度。该方法还包括使用经验相关性获得受试者血液中的物质浓度。浓度对应于光学测量参数的值和一个或多个温度指示参数的值。

$$\int_{\lambda_1}^{\lambda_2} e^{\alpha_{\lambda} x} d\lambda$$