

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
22 January 2004 (22.01.2004)

PCT

(10) International Publication Number
WO 2004/006768 A1

(51) International Patent Classification⁷: **A61B 5/11**

[CA/CA]; 4471 Shoreway Drive, Victoria, British Columbia V8N 3V1 (CA).

(21) International Application Number:
PCT/CA2003/001081

(74) Agents: **MANNING, Gavin** et al.; OYEN WIGGS GREEN & MUTALA, 480 - The Station, 601 West Cordova Street, Vancouver, British Columbia V6B 1G1 (CA).

(22) International Filing Date: 17 July 2003 (17.07.2003)

(25) Filing Language: English

(81) Designated States (*national*): AE, AG, AL, AM, AT (utility model), AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ (utility model), CZ, DE (utility model), DE, DK (utility model), DK, DM, DZ, EC, EE (utility model), EE, ES, FI (utility model), FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK (utility model), SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(26) Publication Language: English

(30) Priority Data:
2,393,880 17 July 2002 (17.07.2002) CA

(71) Applicant (*for all designated States except US*): **TACTEX CONTROLS INC.** [CA/CA]; TACTEX CONTROLS INC., 240 Bay Street, Victoria, British Columbia V9A 3K5 (CA).


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,

(72) Inventors; and

(75) Inventors/Applicants (*for US only*): **LOKHORST, David, M.** [CA/CA]; 16 Parkcrest Drive, Victoria, British Columbia V9B 5E7 (CA). **INKSTER, D., Robert**

[Continued on next page]

(54) Title: **BED OCCUPANT MONITORING SYSTEM**

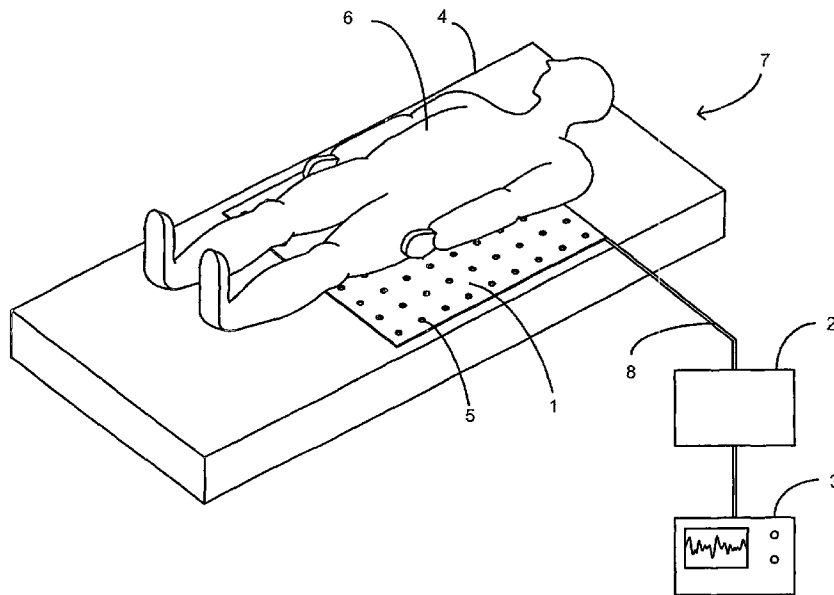

(57) Abstract: The invention provides a bed occupant monitoring system comprising a pressure sensitive member attached to a support member for supporting a bed occupant, the pressure sensitive member comprising a plurality of pressure sensors. Each of the pressure sensors is configured to provide a reflected wave energy pressure signal by reflecting incident wave energy with an intensity which varies with a pressure applied to the sensor. A pair of fibres are coupled to each pressure sensor, each pair of fibres comprising an input fibre and an output fibre. The fibres are coupled to interface electronics comprising a wave energy source coupled to the input fibre of each of the pairs of fibres for providing the applied light energy, and, a wave energy detector coupled to the output fibre of each of the pairs of fibres for converting the scattered light energy into an electrical signal.

WO 2004/006768 A1



SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*

BED OCCUPANT MONITORING SYSTEM**Technical Field**

[0001] This invention relates to monitoring the health and/or activity of a person occupying a bed. This invention provides a novel system comprising a pressure sensitive member coupled to interface electronics.

Background

[0002] It is known to use sensors coupled to a mattress for monitoring a bed occupant. For example, Triplett et al. (U.S. Patent No. 4,175,263) disclose a pressure sensing mechanism for placement on a hospital bed. The pressure sensing mechanism comprises a first pressure sensing pad for sensing a patient's weight when the patient is near the centre of the bed, and a second pressure sensing pad for sensing the patient's weight when the patient is near the edges of the bed. An alarm may be triggered when the patient moves to a location near the edge of the bed.

[0003] Tucknott et al. (U.S. Patent No. 4,633,237) disclose a patient bed alarm system comprising a matrix of sensors woven into a mat for placement on a bed. The matrix of sensors is coupled to a micro computer for calculating the position of a patient in the bed. An alarm may be triggered when the patient is about to leave the bed.

[0004] Alihanka et al. (U.S. Patent No. 4,320,766) disclose a capacitive motion sensor placed under a mattress or the like for monitoring the movements of a person.

[0005] McMahon et al. (U.S. Patent No. 5,435,317) disclose a device for detecting a respiratory dysfunction of a person located in a bed. The device comprises a detection unit which is provided under the mattress of the bed, and a stimulation unit, which acts, in response to a signal from the detection unit, to impart a rocking motion to the bed. The detection unit is embodied as a pad-like device provided under the mattress.

[0006] Bellin et al. (U.S. Patent No. 5,558,996) disclose a patient monitoring device wherein sensors are located in a bed sheet with which a subject comes in contact. One sensor produces a signal corresponding to respiratory induced, pulmonary motion, and myocardial pumping sounds. A second sensor produces a signal corresponding to changes in body position. A processor amplifies and filters the induced signals resulting in resolved output highly correlated to respiration rate, heart beat rate, and changes in body position.

[0007] Reimer et al. (U.S. Patent No. 5,917,180) disclose a pressure sensor which relies on detecting multiply scattered light within an optical cavity. Changes in the volume of the cavity are sensed by the change in sampled light intensity. Pressure

- 2 -

sensitive mats with a high density of sensors are assembled using optical fiber technology.

5 [0008] Musick (U.S. Patent No. 5,844,488) discloses a narrow, pressure-sensitive sensor pad for installation on top of and across the width of a mattress proximate the midsection of a reclining patient. The pad has both central and edge switching areas. The central pressure sensitive switch indicates the presence of a patient in the center of the bed. When a patient moves toward either edge of the bed, an edge switch is activated which generates an early warning signal indicating to attending personnel that a patient has moved from the center of the bed to an edge and may be attempting to exit the bed unattended.

10 [0009] Hammett (U.S. Patent No. 5,144,284) discloses a bed covering device adapted to cover a mattress. The device has compliant flat pressure sensitive means disposed its lower surface for detecting compressive force exerted by a person, and electrical connector means emergent from the pressure sensitive means and configured to connect in modular fashion with a monitoring device and alarm.

15 [0010] Rudeke (PCT publication No. WO9010281A1) discloses a bed alarm intended for use with patients in hospitals and like establishments for indicating when a patient leaves his or her bed. The alarm includes a pressure sensor which functions to detect whether a patient is lying in bed or not and which is intended to be positioned in the bed and preferably between the bed-bottom and the mattress.

20 [0011] Rincoe et al. (U.S. Patent No. 5,993,400) and Scott (U.S. Patent No. 6,067,019) disclose devices that utilize arrangements of sensors to detect the impending egress of a bed occupant. Joseph et al. (U.S. Patent No. 5,410,297) disclose a weight-sensitive capacitive sensor for tracking the position of an occupant. Dixon et al. (U.S. Patent No. 6,208,250) disclose a system comprising two sensors and a processor used to determine the location of a patient on a bed.

25 [0012] Rosenthal (U.S. Patent No. 3,961,201) discloses a switch located between a mattress and a bedframe that is used to detect when a patient moves close to the edge of a bed. Feldl (U.S. Patent No. 4,020,482) discloses an air bladder below a mattress that signals egress of a patient when air pressure in the bladder falls below a threshold. Nicholas (U.S. Patent No. 4,381,434) discloses a device including a spring-loaded plate with a limit switch, all mounted below a mattress.

30 [0013] Despite the volume of existing patent literature, there are significant shortcomings in the known devices. For many devices, reliable operation requires installation on top of the mattress. This has two major shortcomings: firstly, the devices are often stiff (i.e. resistant to flexing) and hard, thereby causing discomfort to the bed occupant. In some applications (for example, monitoring of demented

occupants) this can cause physical and psychological irritation to the bed occupant. Secondly, because the devices are on top of the mattress, they rapidly suffer material fatigue and fail under normal use.

5 Summary of Invention

[0014] One embodiment of the invention provides a bed occupant monitoring system comprising a pressure sensitive member coupled to a support member for supporting a bed occupant, the pressure sensitive member comprising a plurality of pressure sensors. Each of the pressure sensors is configured to provide an optical
10 pressure signal having an intensity which varies with a pressure applied thereto.

The monitoring system also includes at least one wave energy source coupled to the plurality of pressure sensors for providing wave energy to the sensors, and, at least one wave energy detector coupled to the plurality of pressure sensors for converting the optical pressure signals into electrical pressure signals.

15 [0015] The wave energy source may be coupled to the plurality of pressure sensors by means of optical fibres, and the wave energy detector may also be coupled to the plurality of pressure sensors by means of optical fibres. An indicator device may be coupled to the interface electronics.

[0016] The wave energy detector may comprise a photodetector. The photodetector
20 may comprise an array of photo-diodes, and each of the photo-diodes may be coupled to one of the plurality of pressure sensors by means of an optical fibre.

[0017] The interface electronics may further comprise threshold circuitry for comparing the electrical pressure signals to a predetermined threshold. The threshold circuitry may comprise a threshold comparer for determining if the
25 electrical pressure signals are below the predetermined threshold. The threshold circuitry may further comprise a threshold crossing detector configured to reset a timer when the electrical pressure signals cross the predetermined threshold. The system may further comprise an alarm signal generator coupled to the timer and the threshold comparer by means of an AND gate, the alarm signal generator
30 configured to generate an alarm signal if the timer is not reset for a predetermined time period and the electrical pressure signals are below the predetermined threshold.

[0018] The pressure sensitive member may comprise a top foam layer and a bottom foam layer, and each pressure sensor may be formed by securing a pair of optical
35 fibres between the top foam layer and the bottom foam layer, the pair of optical fibres comprising an input fibre coupled to the wave energy source and an output fibre coupled to the wave energy detector.

[0019] The pressure sensitive member may comprise an area of a mattress constructed from a compressible material, and each pressure sensor may be formed by securing a pair of optical fibres between the top foam layer and the bottom foam layer, the pair of optical fibres comprising an input fibre coupled to the wave energy source and an output fibre coupled to the wave energy detector.

5 [0020] Each of the pressure sensors may be responsive to pressure in a range of 1 to 15 mmHg.

[0021] The support member may comprise a mattress, and the pressure sensitive member may be positioned atop the mattress, below the mattress, within a cavity in the mattress, in a recess near a top of the mattress, such that a top surface of the pressure sensitive member is flush with a top surface of the mattress, or in a recess near a bottom of the mattress, such that a bottom surface of the pressure sensitive member is flush with a bottom surface of the mattress.

10 [0022] The plurality of pressure sensors may be arranged in an array across a width of the support member, and the interface electronics may comprise signal processing means for determining a position of the occupant on the support member. The plurality of pressure sensors may be arranged into a central group and two side groups, with the side groups positioned adjacent to edges of the support member and the central group positioned therebetween, and the signal processing means are configured to calculate a total applied pressure for each group.

15 [0023] The monitoring system may further comprise an opaque covering material for shielding the pressure sensors from ambient light.

[0024] The monitoring system may further comprise a protective sheath covering the optical fibres between the pressure sensitive member and the interface electronics.

25 [0025] Another embodiment of the invention provides a method of monitoring a bed occupant occupying a bed with a pressure sensitive member coupled thereto, the pressure sensitive member comprising a plurality of pressure sensors, each of the pressure sensors configured to provide a reflected wave energy pressure signal by reflecting incident wave energy with an intensity which varies with a pressure applied thereto. The method comprises applying wave energy to the pressure sensors, and, measuring pressure signals received from the pressure sensitive member.

30 [0026] The method may comprise processing the measured pressure signals by taking a sum of a time derivative of the absolute values of the pressure signals, taking a sum of a time derivative of the pressure signals, or taking a sum of a time derivative of the squared pressure signals.

35

[0027] The method may comprise comparing the measured pressure signals to a predetermined threshold. The method may comprise generating an alarm signal if the measured pressure signals remain below the predetermined threshold for a predetermined time period. The predetermined threshold and predetermined time period may be set in relation to an expected heart beat pressure signal, an expected pulmonary pressure signal, or an expected bodily movement pressure signal.

5 [0028] The method may comprise computing a heart rate of the bed occupant from the measured pressure signals, and/or computing a respiration rate of the bed occupant from the measured pressure signals.

10 [0029] Another embodiment of the invention provides a bed occupant monitoring system comprising a pressure sensitive member coupled to a support member for supporting a bed occupant, the pressure sensitive member comprising a plurality of pressure sensors, interface electronics coupled to the pressure sensors for producing at least one pressure signal; and, threshold circuitry for comparing the pressure
15 signals to a predetermined threshold.

Brief Description of Drawings

[0030] In drawings which illustrate non-limiting embodiments of the invention:

20 [0031] Figure 1 illustrates schematically an occupant lying in a bed equipped with a monitoring system according to one embodiment of the invention;

[0032] Figure 2 illustrates schematically interface electronics according to an embodiment of the invention;

[0033] Figure 3 is a block diagram of some circuit elements of interface electronics according to another embodiment of the invention;

25 [0034] Figure 4 graphically depicts externally applied pressure over time for an example situation of a patient occupying a bed equipped with a monitoring system according to the invention;

[0035] Figure 5 is a flowchart illustrating a method of monitoring a bed occupant according to one embodiment of the invention;

30 [0036] Figure 6 shows a pressure sensitive member and interface electronics according to one embodiment of the invention;

[0037] Figure 7(a) shows a top view of a portion of the pressure sensitive member of Figure 2, with the top layer removed;

35 [0038] Figure 7(b) is a cross-sectional view of the portion of the pressure sensitive member of Figure 3(a), with the top layer present;

[0039] Figure 8 is a sectional view of a portion of a mattress with a pair of fibres inserted therein according to another embodiment of the invention;

[0040] Figure 9(a) illustrates an embodiment of the invention wherein the pressure sensitive member is coupled to the top of a support member;

[0041] Figure 9(b) illustrates an alternative embodiment of the invention wherein the pressure sensitive member is coupled within a recess in a top surface of the support member;

[0042] Figure 9(c) illustrates an alternative embodiment of the invention wherein the pressure sensitive member is coupled within a cavity within the support member;

[0043] Figure 9(d) illustrates an alternative embodiment of the invention wherein the pressure sensitive member is coupled within a recess in a bottom surface of the support member;

[0044] Figure 9(e) illustrates an alternative embodiment of the invention wherein the pressure sensitive member is coupled to the bottom of the support member; and,

[0045] Figure 10 illustrates an alternative embodiment of the invention wherein pressure sensors are arranged into three groups within the pressure sensitive member.

Description

[0046] Throughout the following description specific details are set forth in order to provide a more thorough understanding of the invention. However, the invention may be practiced without these particulars. In other instances, well known elements have not been shown or described in detail to avoid unnecessarily obscuring the present invention. Accordingly, the specification and drawings are to be regarded in an illustrative, rather than a restrictive, sense.

[0047] The invention provides apparatus and methods for monitoring a bed occupant, such as a patient, lying in a bed. Apparatus according to the invention can facilitate monitoring of the bed occupant's presence, heart rate, respiration, and/or movement. The apparatus comprises a pressure sensitive member in the bed coupled to interface electronics. The pressure sensitive member preferably comprises an array of pressure sensors which produce signals representative of the pressures applied to the sensors.

[0048] Figure 1 is a schematic view of a bed occupant monitoring system 7 according to one embodiment of the invention. A bed occupant 6 lies upon a bed which includes a mattress or other support member 4. Monitoring system 7 includes a pressure sensitive member 1 on support member 4. Pressure sensitive member 1 is coupled to interface electronics 2 by signal carriers 8. Signal carriers 8 may comprise optical fibres, wires or other signal carriers capable of carrying

- 7 -

signals from pressure sensors 5 in pressure sensitive members 1 to interface electronics 2.

5 [0049] Interface electronics 2 may be housed in a single enclosure as illustrated in Figure 1, or they may be housed in more than one enclosure connected by signal means (not shown). The signal means may comprise any suitable signal carriers, for example, one or more wires, optical signal carriers, wireless connections, or the like. Optionally, interface electronics 2 comprises an indicator device 3. Indicator device 3 may comprise an visible or audible alarm, a data display system, an attendant call system, a data logging system, or the like.

10 [0050] Pressure sensitive member 1 comprises a plurality of pressure sensors 5. Each pressure sensor 5 measures the bearing pressure applied by occupant 6 in proximity thereto. A change in the bearing pressure results in a change in the output of pressure sensor 5. Pressure sensors 5 are preferably responsive to pressures in the range of 1 to 15 mmHg. Pressure sensors 5 preferably comprise
15 pressure sensors which produce optical output signals. Most preferably the pressure sensors are optical sensors which do not require any electrical or electronic devices to be at the location of the sensor. The term "optical", as used herein, is to be understood to refer to electromagnetic wave energy of any wavelength, and not only to those wavelengths which correspond to the visible spectrum. Optical pressure
20 sensors are advantageous because they allow monitoring of occupant 6 without the need for electrical devices in the bed, which may be hazardous.

[0051] Pressure sensors 5 may be constructed in accordance with US Patent 5,917,180 to Reimer et al., which is hereby incorporated by reference. Such sensors are available under the brand name Kinotex™ from Tactex Contols Inc. of
25 Victoria, British Columbia, Canada. Such sensors are particularly advantageous for bed occupant monitoring as they exhibit a high level of sensitivity to minor pressure variations over a wide range of pressure levels. Conventional pressure sensors with comparable sensitivity typically will be unable to sense minor pressure variations at elevated pressure levels, such as when a person is lying or sitting upon them.

30 [0052] In certain specific embodiments of the invention, each pressure sensor 5 is configured to reflect incident wave energy received from interface electronics 2 with an intensity which varies with a pressure applied to pressure sensor 5. In such embodiments, signal carriers 8 comprise a plurality of pairs of fibres, with one pair coupled to each pressure sensor 5. Each pressure sensor is coupled to interface
35 electronics 2 by an input fibre 15 (see Figure 2), which provides incident wave energy, and an output fibre 14 (see Figure 2), which transmits reflected wave energy to interface electronics 2.

[0053] As described in Reimer et al., Kinotex™ pressure sensors utilize an optical-to-electronic interface. The optical-to-electronic interface comprises one or more wave energy sources, typically light transmitters (such as one or more light-emitting-diodes) and one or more wave energy detectors, typically photodetectors (such as one or more photo-diodes or photo-transistors). Interface electronics 2 includes the optical-to electronic interface.

[0054] In one embodiment of this invention, the optical-to-electronic interface comprises one light emitter and one photodetector, and the interface electronics comprise analog and/or digital circuit elements configured to provide an output signal representative of the total pressure applied to pressure sensitive member 1. In another embodiment, the optical-to-electronic interface comprises at least one light emitter and more than one photodetector, and the signal conditioning electronics comprise analog and/or digital circuit elements configured to provide multiple output signals representative of the pressures applied to different regions of the pressure sensitive member, as discussed below with reference to Figure 10.

[0055] In another embodiment of the invention, the interface electronics are configured to measure signals from each of the pressure sensors individually. Alternatively (or additionally) further circuit elements may be included to extract other information from the signals, such as the time-derivative (i.e. time rate of change) of the signal or a high-pass filter or a low-pass filter or a notch filter or any combination of the foregoing. Each of these provides valuable information regarding the condition of the bed occupant.

[0056] Although it is possible in principle to implement the invention using entirely analog electronics, it is preferable to use a combination of analog, optical and digital electronics. The signal processing function of interface electronics 2 may be provided in hardware, in software, or in a combination of hardware and software. Standard signal processing techniques may be used to increase the signal to noise ratio of such signals and to extract desired information from the signals.

[0057] As an example of a preferred embodiment, a simplified schematic illustration of interface electronics 2 is shown in Figure 2. A microprocessor 32 is coupled to two LED drive circuits 31 that provide current to two LEDs 30. LEDs 30 provide illumination for pressure sensors 5. Although two LEDs 30 and LED drive circuits 31 are shown in Figure 2 for ease of illustration, it is to be understood that any number of LEDs 30 and drive circuits 31 are possible. An input fibre 15 provides light energy from LEDs 30 to each of pressure sensors 5 (not shown in Figure 2). An output fibre 14 returns light from each pressure sensor 5 (not shown in Figure 2) to photodetector 33. Photodetector 33 preferably comprises an array of

- 9 -

photo-diodes, with each receiving fibre 14 being associated with a specific photo-diode.

[0058] Microprocessor 32 provides control signals 38 that cause photodetector 33 to output an analog signal 39 corresponding to the light intensities received from pressure sensors 5. In the illustrated embodiment, control signals 38 are used to coordinate the signals being sent from the individual elements of photodetector 33 to microprocessor 32 when photodetector 33 comprises an array of photo-diodes or other sensors. Alternatively, photodetector 33 could be configured to provide a separate analog signal 39 to microprocessor 32 from each element of photodetector 33. In the further alternative, monitoring system 7 could include a signal concentrator (not shown) which combines signals from two or more pressure sensors 5 and provides microprocessor 32 with a signal indicating a property of the combined signals, for example a signal containing information about an average pressure exerted on the two or more pressure sensors 5. The signals may be combined optically, for example by detecting light from multiple pressure sensors 5 at a single light detector, or may be combined electronically after having been detected.

[0059] Optionally, analog signal 39 may be amplified, filtered, or otherwise conditioned by analog circuitry 34. Analog signal 39 is then converted into digital form by Analog-to-Digital converter 35, and the sampled signal is read by micro-processor 32. Microprocessor 32 implements any necessary signal processing, as described below, and produces output signals 40 via appropriate driver circuitry 36. Driver circuitry 36 may optionally comprise well known electronic interfaces such as RS-232, RS-485, Ethernet, Universal Serial Bus, or the like, or a digitally controlled driver. Output signal 40 may be passed to an indicator device 3 (not shown in Figure 2), a remote monitoring station, an automated alarm system, or the like.

[0060] Monitoring system 7 may be used to monitor various indications of health of bed occupant 6, including the pulmonary and/or heart activity of bed occupant 6. Referring again to Figure 2, interface electronics 2 may produce an output signal 40 representative of any of the following parameters: the sum of the time derivative of all pressure signals; the sum of the time derivative of the squared pressure signals; or, the sum of the time derivative of the absolute values of the pressure signals. Output signal 40 may comprise a digital, analog or optical signal. The inventors have found that the pulmonary activity, heart activity, and bodily movement of the bed occupant can be determined from these computed parameters.

[0061] Figure 3 shows one possible arrangement of functional characteristics of interface electronics 2. Photodetector 33 provides pressure signals to signal processor 42. Signal processor 42 amplifies, takes the time derivative, or otherwise processes the pressure signals, and passes them to threshold circuitry 44, and optionally also to indicator device 3. Threshold circuitry 44 preferably comprises threshold comparer 45, threshold crossing detector 46, and timer 47. Threshold comparer 45 is configured to produce a signal indicating when the pressure signals indicate a pressure below a predetermined threshold. Threshold crossing detector 46 is configured to reset timer 47 when the pressure signals cross the threshold. Timer 47 is configured to produce a high output if allowed to run without for a predetermined time period without being reset. AND gate 48 is configured to trigger alarm signal generator 49 when it receives high outputs from both threshold comparer 45 and timer 47. Threshold circuitry 44 may be configured to monitor a number of different thresholds, as described below.

[0062] Figure 4 is a typical graph 50 of the sum of the derivatives of the absolute value of the pressure signals generated by a bed occupant lying in a bed equipped with a monitoring system according to the invention, plotted against time. Graph 50 is an idealized representation of pressure signals generated by a pressure sensitive member 1 located on top of support member 4. The variations in the pressure signals are typically less pronounced when the signals are generated by a pressure sensitive member 1 located within or below support member 4, and as such it may be difficult to determine the heart rate of bed occupant 6, although pulmonary activity and movement may still be detected, as described below. It is to be understood that a graph of actual pressure signals may include more noise than illustrated, but the noise may be minimized by any suitable noise reduction techniques.

[0063] In graph 50, time is indicated from left to right, along axis 51. Peaks 53 and 54 correspond to inhaling and exhaling respectively. The smaller more frequent peaks 55 correspond to heart beats. The large disturbance 56 corresponds to bodily movement (for example, when the bed occupant shifts his weight). Movement signals 56 are typically on the order of ten times larger than pulmonary signals 53 and 54, which are in turn typically on the order of ten times larger than heart beat signals 55. The pressure signals will only remain constant if the bed occupant's heart stops beating, the bed occupant leaves the bed, or there is a malfunction.

Interface electronics 2 may be configured to generate an alarm signal if the pressure signals remain below a heart beat threshold for a predetermined period of time selected according to an expected heart beat frequency, or if the pressure signals

remain constant for a predetermined period of time. Further signal processing can optionally be performed by signal processing means in interface electronics 2 to measure the precise rate of respiration and/or the rate of heart beat from the signal shown in Figure 4. The signal processing means may comprise microprocessor 32,
5 a digital signal processor, and/or noise reduction circuitry.

[0064] In one embodiment of the invention, a pulmonary threshold 57 may be set such that if the signal remains below pulmonary threshold 57 for a predetermined period of time, output signal 40 includes a pulmonary alarm which indicates the suspension of pulmonary activity. The predetermined amount of time for the
10 pulmonary alarm may be set according to an expected respiratory frequency. Pulmonary threshold 57 may be determined adaptively by microprocessor 32 based on the pattern of measured pressure signals, or may be preset when monitoring system 7 is manufactured and calibrated. Optionally, a user interface (not shown) may be provided to allow pulmonary threshold 57 and the time period for the
15 pulmonary alarm to be adjusted to allow for differences in weights and breathing patterns of different bed occupants.

[0065] In another embodiment, a bodily movement threshold 58 can be set such that if the signal remains below movement threshold 58 for a predetermined period of time, output signal 40 includes a pulmonary alarm which indicates the suspension of
20 pulmonary activity. The predetermined time period for the movement alarm is set so that the alarm will sound before bed occupant 6 has remained motionless for so long as to be at risk for bed sores. Movement threshold 58 may be determined adaptively by microprocessor 32 based on the pattern of measured pressure signals, or may be preset when monitoring system 7 is manufactured and calibrated.
25 Optionally, a user interface (not shown) may be provided to allow movement threshold 58 and the time period for the movement alarm to be adjusted to allow for differences in weights and movement patterns of different bed occupants.

[0066] Figure 5 is a flowchart illustrating a method of monitoring a bed occupant according to one embodiment of the invention. At block 100, pressure signals are
30 measured by photodetector 33. At block 102, the measured signals are processed by signal processor 42. At block 104, the signals are compared to a threshold by threshold comparer 45. If the signals are not below the threshold (block 104 NO output), the method returns to block 100. If the signals are below the threshold (block 104 YES output), the method continues to block 106. At block 106,
35 threshold crossing detector 46 determines whether the signals have just crossed the threshold. If they have (block 106 YES output), timer 47 is reset at block 108 and the method returns to block 100. If they have not (block 106 NO output) the

- 12 -

method continues to block 110. At block 110, if timer 47 has been running for a predetermined period since it was last reset (block 110 YES output), an alarm signal is generated at block 112. If not, (block 110 NO output), the method returns to block 100.

5 [0067] Figures 6, 7(a) and 7(b) illustrate a pressure sensitive member 1 according to one embodiment of the invention. Pressure sensitive member 1 comprises a plurality of Kinotex™ pressure sensors 5 sandwiched between two layers 9, 10 of a compressible material. The compressible material may comprise foam, and preferably comprises a soft polyurethane foam. Preferably, several bundles of
10 plastic optical fibres 8 deliver and retrieve the light energy from interface electronics 2 to pressure sensors 5. The bundles of fibre 8 are preferably gathered and optionally passed through a protective sleeve 12 that terminates at the interface electronics 2. The bundles of fibre 8 preferably each comprise a plurality of fibre pairs 14,15. An area of adhesive 11 is preferably used to secure each fibre pair 14,
15 15 to the layers 9, 10 above and below each pressure sensor 5. In embodiments wherein pressure sensitive member is to be located at the top of or within support member 4, as shown in Figures 9(a)-(c), fibre bundles 8 are preferably arranged sinusoidally between layers 9, 10 and not adhered along their length so as to provide some flexibility and resilience to pressure sensitive member 1. In
20 embodiments wherein pressure sensitive member 1 is to be located at the bottom of support member 4, as shown in Figure 9(d)-(e), fibre bundles 8 may be adhered along their entire length, as pressure sensitive member 1 will preferably be adjacent to or mounted on a rigid surface.

[0068] Top layer 9 and bottom layer 10 are preferably constructed from material
25 chosen to be suitable with the specific characteristics of pressure sensors 5. Materials well suited for use with Kinotex™ pressure sensors are structurally self-supporting, compressible, at least partially transmissive of light, and optionally elastically resilient. The inventors have determined that white or natural-coloured low density polyurethane foam are suitable materials for use with Kinotex™ pressure
30 sensors. Such foam is available from, among others, Lendell Manufacturing Inc. of St. Charles, Michigan, product code HSS. The inventors have also determined that most standard bed mattress foam materials can be used as top layer 9 and/or bottom layer 10. It will be understood that many different foam materials provide similar characteristics and the present invention is not limited to a specific material. A
35 covering material (not shown) which is opaque at wavelengths used by pressure sensors 5 is preferably provided to keep ambient light from disturbing the Kinotex™ pressure sensors. The opaque covering material preferably comprises a two-tone

- 13 -

flexible plastic cover that is black on the inside and white on the outside, which envelops pressure sensitive member 1.

5 [0069] In an alternative embodiment, pressure sensitive member 1 comprises an area of the mattress in which pressure sensors 5 are formed. Figure 8 illustrates a section of mattress 13 with input and output fibres 15, 14 inserted therein. The compressible material of mattress 13, in addition to supporting bed occupant 6 (not shown in Figure 8), reflects incident wave energy received from input fibre 15 to output fibre 14, and thus forms pressure sensors 5. The Figure 8 embodiment is particularly advantageous for equipping an existing bed with a bed occupant monitoring system 7 according to the invention, as one may do so by simply inserting optical fibres into the mattress.

10 [0070] Pressure sensitive member 1 is preferably flexible and soft. Pressure sensitive member 1 can be placed on a support member 4, which may comprise a bed mattress, underneath the sheets and coverings upon which bed occupant 6 lies. The inventors have determined that, where soft sensors such as Kinotex™-type sensors are used, pressure sensitive member 1 can be made to be essentially undetectable to a bed occupant 6. In some embodiments, the deformable material of sensors 5 has an elastic modulus which is substantially the same as that of the material surrounding sensors 5.

20 [0071] It must be understood that Figure 1 is a schematic representation of one possible embodiment of the invention. Many variations in the physical locations and sizes of the elements are possible. For example, among other things, the pressure sensitive member 1 may be located in-between occupant 6 and support member 4, or it may be embedded in support member 4. Some of the possible positions for pressure sensitive member 1 are shown in Figures 9(a)-(e). Figures 9(a) to 9(e) illustrate various embodiments of the invention with pressure sensitive member 1 placed in different positions with respect to support member 4. Figure 9(a) illustrates an embodiment wherein pressure sensitive member 1 is on top of support member 4. Figure 9(b) illustrates an embodiment wherein pressure sensitive member 1 is placed in a recess 17 near the top of support member 4 so that the top of member 1 is flush with the top surface of support member 4. Figure 9(c) illustrates an embodiment wherein support member 4 is made of at least two layers laminated together, between which is sandwiched pressure sensitive member 1 within a cavity 18. Figure 9(d) illustrates an embodiment wherein pressure sensitive member 1 is located in a recess 19 near the bottom of support member 4 so that the bottom of member 1 is flush with the bottom surface of support member

- 14 -

4. Figure 9(e) illustrates an embodiment wherein pressure sensitive member 1 is attached to the bottom of support member 4.

5 [0072] The wide dynamic range of Kinotex™-type sensors permits such sensors to pick up usable signals even when pressure sensitive member 1 is located under or within a mattress.

10 [0073] Although many arrangements of pressure sensors 5 are possible, pressure sensors 5 may conveniently be arranged in a rectangular array extending across the width of support member 4. Pressure sensors 5 may be spaced approximately 2 cm to 10 cm apart. Depending on the intended application, the array of pressure sensors 5 may extend the entire length of support member 4 or some portion of the length. For example, to monitor the bed occupant's respiration, the inventors have found that a 60-sensor array approximately 90cm wide by 30cm in length is sufficient. A larger device with correspondingly more sensors may be used for larger occupants.

15 [0074] Figure 10 illustrates a pressure sensitive member 20 according to an embodiment of the invention wherein pressure sensors 5 are arranged into three groups 21, 22 and 23. Pressure sensitive member 20 of Figure 10 is dimensioned so that it spans the width of support member 4, with side groups 21 and 23 adjacent to the edges of support member 4. The responses of all of the pressure sensors 5 within the central group 22 are summed by interface electronics 2 by using a single photo-sensor (not shown in Figure 5) to detect their light output simultaneously. Pressure applied to any pressure sensor 5 within central group 22 will result in a change in an output signal from interface electronics 2 which is representative of the average pressure on the sensors of central group 22. In a similar manner, the signals from pressure sensors 5 in side groups 21 and 23 are summed using a second photo-sensor (not shown). This results in two output signals: one representing the total pressure applied within central group 22, and another representing the pressure applied within side groups 21 and 23.

20
25
30
35 [0075] Interface electronics 2 may also comprise further analog electronics to compare these signals to produce a third signal that is derived therefrom. The third signal indicates three possible states: 1) there is no occupant in the bed (determined by both first and second signals being below a threshold); 2) the bed occupant is in the central region (determined by the first signal being above a first threshold and the second signal being below a second threshold); 3) the bed occupant is near the edge of the bed (determined by the second signal being above the second threshold). Interface electronics can be used to active an audible alarm or an attendant call

- 15 -

system depending on which of the three states is indicated by the third signal, and on predetermined monitoring parameters.

[0076] As will be apparent to those skilled in the art in the light of the foregoing disclosure, many alterations and modifications are possible in the practice of this invention without departing from the scope thereof. Accordingly, the scope of the invention is to be construed in accordance with the substance defined by the following claims.

- 16 -

WHAT IS CLAIMED IS:

1. A bed occupant monitoring system comprising:
 - 5 (a) a pressure sensitive member coupled to a support member for supporting a bed occupant, the pressure sensitive member comprising a plurality of pressure sensors, each of the pressure sensors configured to provide an optical pressure signal having an intensity which varies with a pressure applied thereto;
 - 10 (b) at least one wave energy source coupled to the plurality of pressure sensors for providing wave energy to the plurality of pressure sensors; and,
 - (c) at least one wave energy detector coupled to the plurality of pressure sensors for converting the optical pressure signals into electrical pressure signals.
- 15 2. A bed occupant monitoring system according to claim 1 comprising interface electronics with threshold circuitry for comparing the electrical pressure signals to a predetermined threshold.
- 20 3. A bed occupant monitoring system according to claim 2 wherein the threshold circuitry comprises a threshold comparer for determining if the electrical pressure signals are below the predetermined threshold.
- 25 4. A bed occupant monitoring system according to claim 3 wherein the threshold circuitry further comprises a threshold crossing detector configured to reset a timer when the electrical pressure signals cross the predetermined threshold.
- 30 5. A bed occupant monitoring system according to claim 4 further comprising an alarm signal generator coupled to the timer and the threshold comparer by means of an AND gate, the alarm signal generator configured to generate an alarm signal if the timer is not reset for a predetermined time period and the electrical pressure signals are below the predetermined threshold.
- 35 6. A bed occupant monitoring system according to claim 1 comprising a signal concentrator connected to receive a plurality of the electrical pressure signals and to output a combined signal indicative of a property of said plurality of the electrical pressure signals.

- 17 -

7. A bed occupant monitoring system according to claim 1 comprising a signal concentrator connected to receive a plurality of the optical pressure signals and to output a combined optical signal indicative of a property of said plurality of the optical pressure signals to the at least one wave energy detector.
- 5
8. A bed occupant monitoring system according to claim 1 wherein the pressure sensitive member comprises a top foam layer and a bottom foam layer, and wherein each pressure sensor comprises a pair of optical fibres having ends between the top foam layer and the bottom foam layer, each pair of optical fibres comprising an input fibre coupled to the wave energy source and an output fibre coupled to the wave energy detector.
- 10
9. A bed occupant monitoring system according to claim 1 wherein the pressure sensitive member is constructed from a compressible material, and wherein each pressure sensor comprises a pair of optical fibres having ends within the compressible material, each pair of optical fibres comprising an input fibre coupled to the wave energy source and an output fibre coupled to the wave energy detector.
- 15
10. A bed occupant monitoring system according to claim 9 wherein the support member is constructed from a compressible material having an elastic modulus which is substantially the same as an elastic modulus of the compressible material of the pressure sensitive member.
- 20
11. A bed occupant monitoring system according to claim 1 wherein the pressure sensitive member comprises an area of a mattress constructed from a compressible material, and wherein each pressure sensor comprises a pair of optical fibres having ends within the compressible material, each pair of optical fibres comprising an input fibre coupled to the wave energy source and an output fibre coupled to the wave energy detector.
- 25
- 30
12. A bed occupant monitoring system according to claim 1 wherein each of the pressure sensors is responsive to pressure in a range of 1 to 15 mmHg.
- 35

- 18 -

13. A bed occupant monitoring system according to claim 1 wherein the wave energy source is coupled to the plurality of pressure sensors by means of optical fibres.
- 5 14. A bed occupant monitoring system according to claim 1 wherein the wave energy detector is coupled to the plurality of pressure sensors by means of optical fibres.
- 10 15. A bed occupant monitoring system according to claim 1 comprising an indicator device.
16. A bed occupant monitoring system according to claim 1 wherein the wave energy detector comprises a photodetector.
- 15 17. A bed occupant monitoring system according to claim 16 wherein the photodetector comprises an array of photo-diodes, and wherein each of the photo-diodes is coupled to one of the plurality of pressure sensors by means of an optical fibre.
- 20 18. A bed occupant monitoring system according to claim 1 wherein the support member comprises a mattress, and the pressure sensitive member is positioned atop the mattress.
- 25 19. A bed occupant monitoring system according to claim 1 wherein the support member comprises a mattress, and the pressure sensitive member is positioned below the mattress.
20. A bed occupant monitoring system according to claim 1 wherein the support member comprises a mattress, and the pressure sensitive member is positioned within a cavity in the mattress.
- 30 21. A bed occupant monitoring system according to claim 1 wherein the support member comprises a mattress, and the pressure sensitive member is positioned in a recess near a top of the mattress, such that a top surface of the pressure sensitive member is flush with a top surface of the mattress.
- 35

22. A bed occupant monitoring system according to claim 1 wherein the support member comprises a mattress, and the pressure sensitive member is positioned in a recess near a bottom of the mattress, such that a bottom surface of the pressure sensitive member is flush with a bottom surface of the mattress.
23. A bed occupant monitoring system according to claim 1 wherein the plurality of pressure sensors are arranged in an array across a width of the support member, comprising signal processing means for determining a position of the occupant on the support member.
24. A bed occupant monitoring system according to claim 23 wherein the plurality of pressure sensors are arranged into a central group and two side groups, with the side groups positioned adjacent to edges of the support member and the central group positioned therebetween, and wherein the signal processing means are configured to calculate a total applied pressure for each group.
25. A bed occupant monitoring system according to claim 1 further comprising an opaque covering material for shielding the pressure sensors from ambient light.
26. A bed occupant monitoring system according to any one of claims 8 to 11, 13, 14 or 17, further comprising a protective sheath covering the optical fibres between the pressure sensitive member and the interface electronics.
27. A method of monitoring a bed occupant occupying a bed with a pressure sensitive member coupled thereto, the pressure sensitive member comprising a plurality of pressure sensors, each of the pressure sensors configured to provide a reflected wave energy pressure signal by reflecting incident wave energy with an intensity which varies with a pressure applied thereto, the method comprising:
- (a) applying wave energy to the pressure sensors; and,
 - (b) measuring pressure signals received from the pressure sensitive member.

- 20 -

28. A method according to claim 27 comprising processing the measured pressure signals by taking a sum of a time derivative of the absolute values of the pressure signals.
- 5 29. A method according to claim 27 comprising processing the measured pressure signals by taking a sum of a time derivative of the pressure signals.
30. A method according to claim 27 comprising processing the measured pressure signals by taking a sum of a time derivative of the squared pressure signals.
- 10
31. A method according to claim 27 comprising comparing the measured pressure signals to a predetermined threshold.
- 15 32. A method according to claim 31 comprising generating an alarm signal if the measured pressure signals remain below the predetermined threshold for a predetermined time period.
- 20 33. A method according to claim 32 wherein the predetermined threshold and predetermined time period is set in relation to an expected heart beat pressure signal.
34. A method according to claim 32 wherein the predetermined threshold is set in relation to an expected pulmonary pressure signal.
- 25 35. A method according to claim 32 wherein the predetermined threshold is set in relation to an expected bodily movement pressure signal.
36. A method according to claim 27 comprising computing a heart rate of the bed occupant from the measured pressure signals.
- 30 37. A method according to claim 27 comprising computing a respiration rate of the bed occupant from the measured pressure signals.
- 35 38. A bed occupant monitoring system comprising:

- 21 -

- 5
- (a) a pressure sensitive member coupled to a support member for supporting a bed occupant, the pressure sensitive member comprising a plurality of pressure sensors;
 - (b) interface electronics coupled to the pressure sensors for producing at least one pressure signal; and,
 - (c) threshold circuitry for comparing the pressure signals to a predetermined threshold.
- 10
39. Any and all apparatus comprising a novel and inventive feature, combination of features, subcombination of features as described or clearly inferred from the description above.
- 15
40. Any and all methods comprising a novel and inventive act, combination of acts, subcombination of acts, step, combination of steps, subcombination of steps as described or clearly inferred from the description above.

20

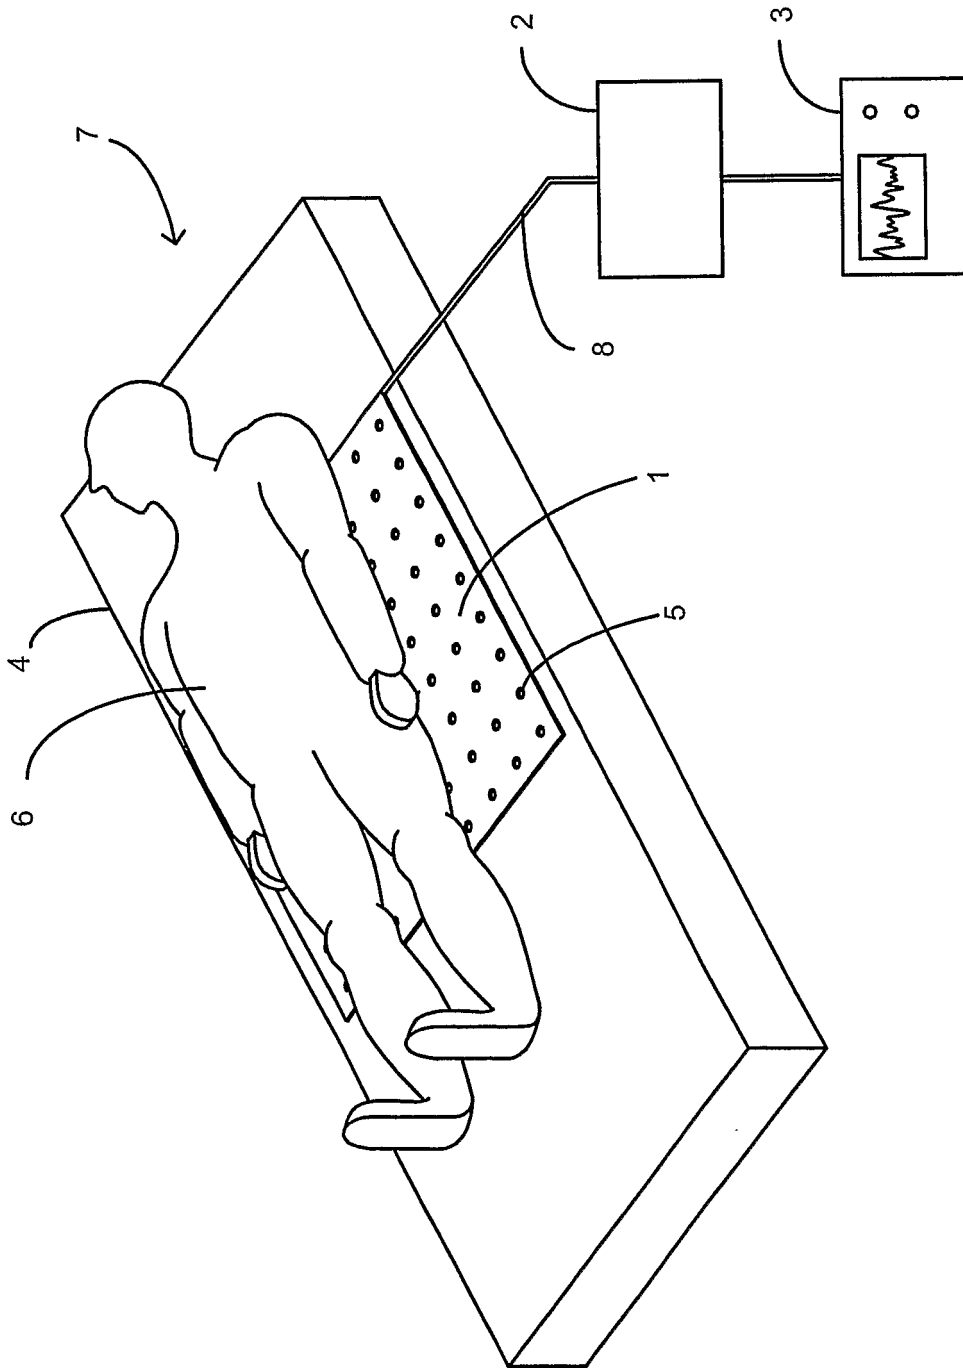


FIGURE 1

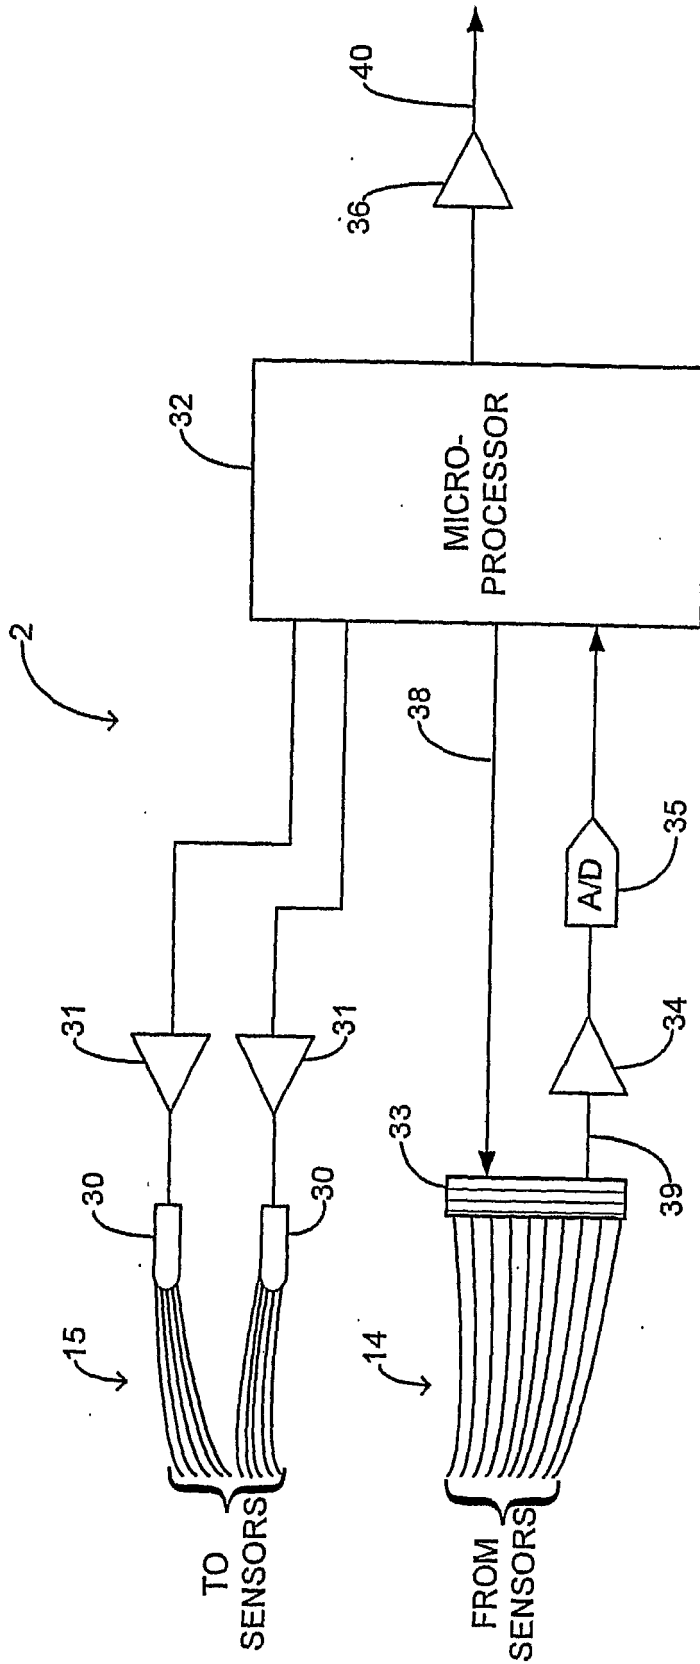


FIGURE 2

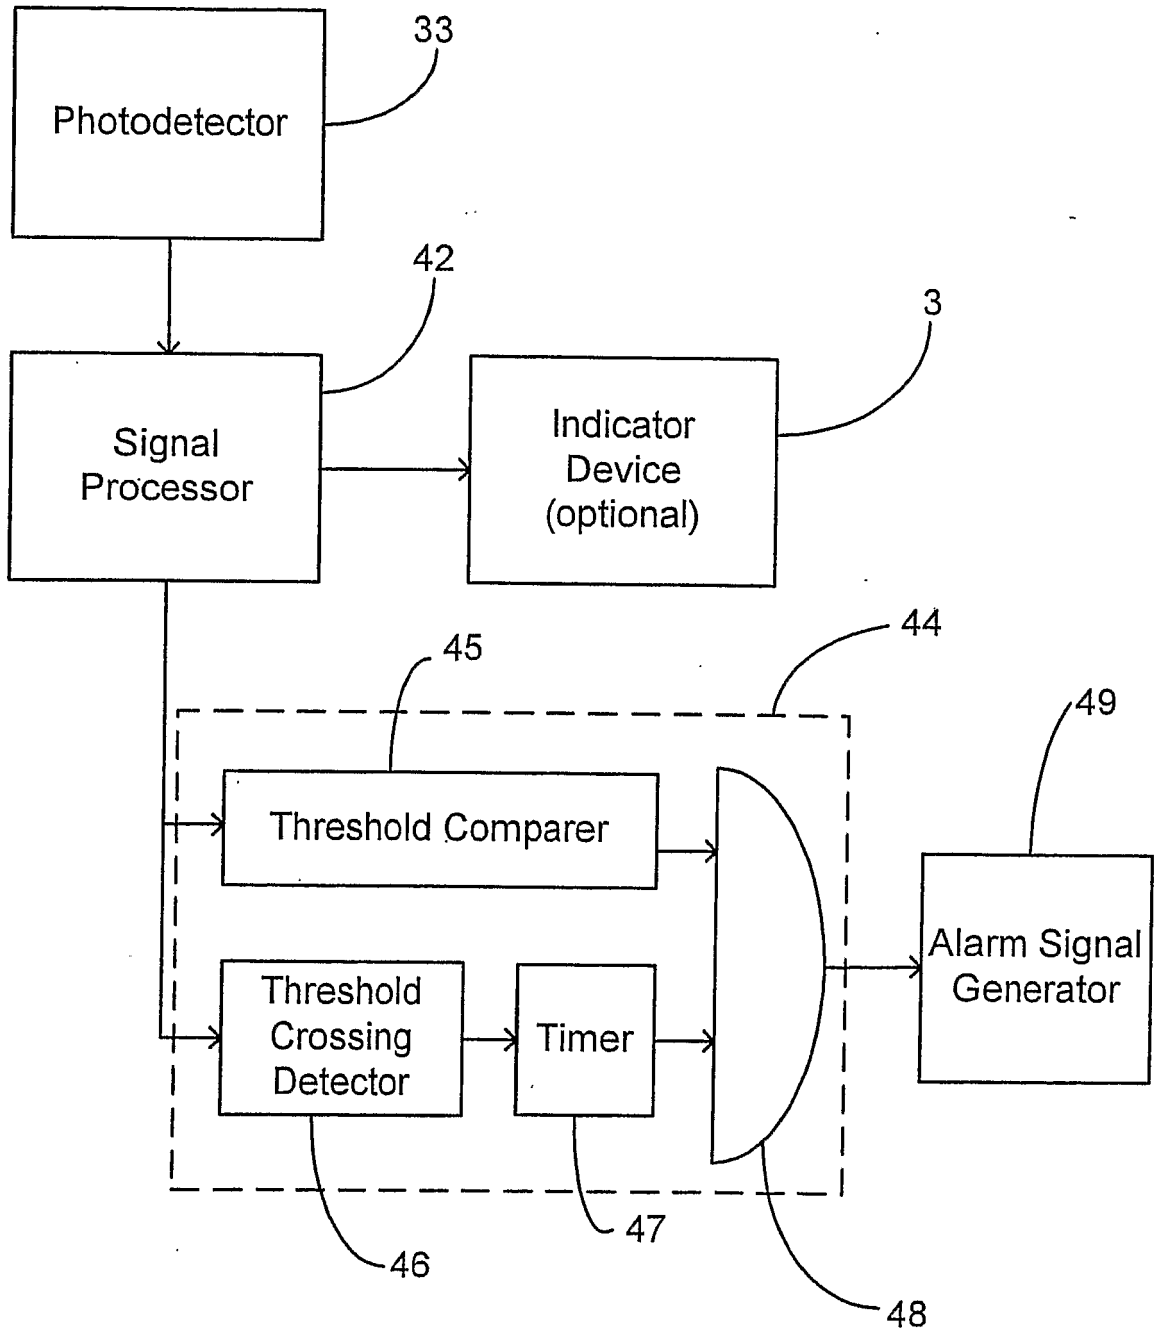


FIGURE 3

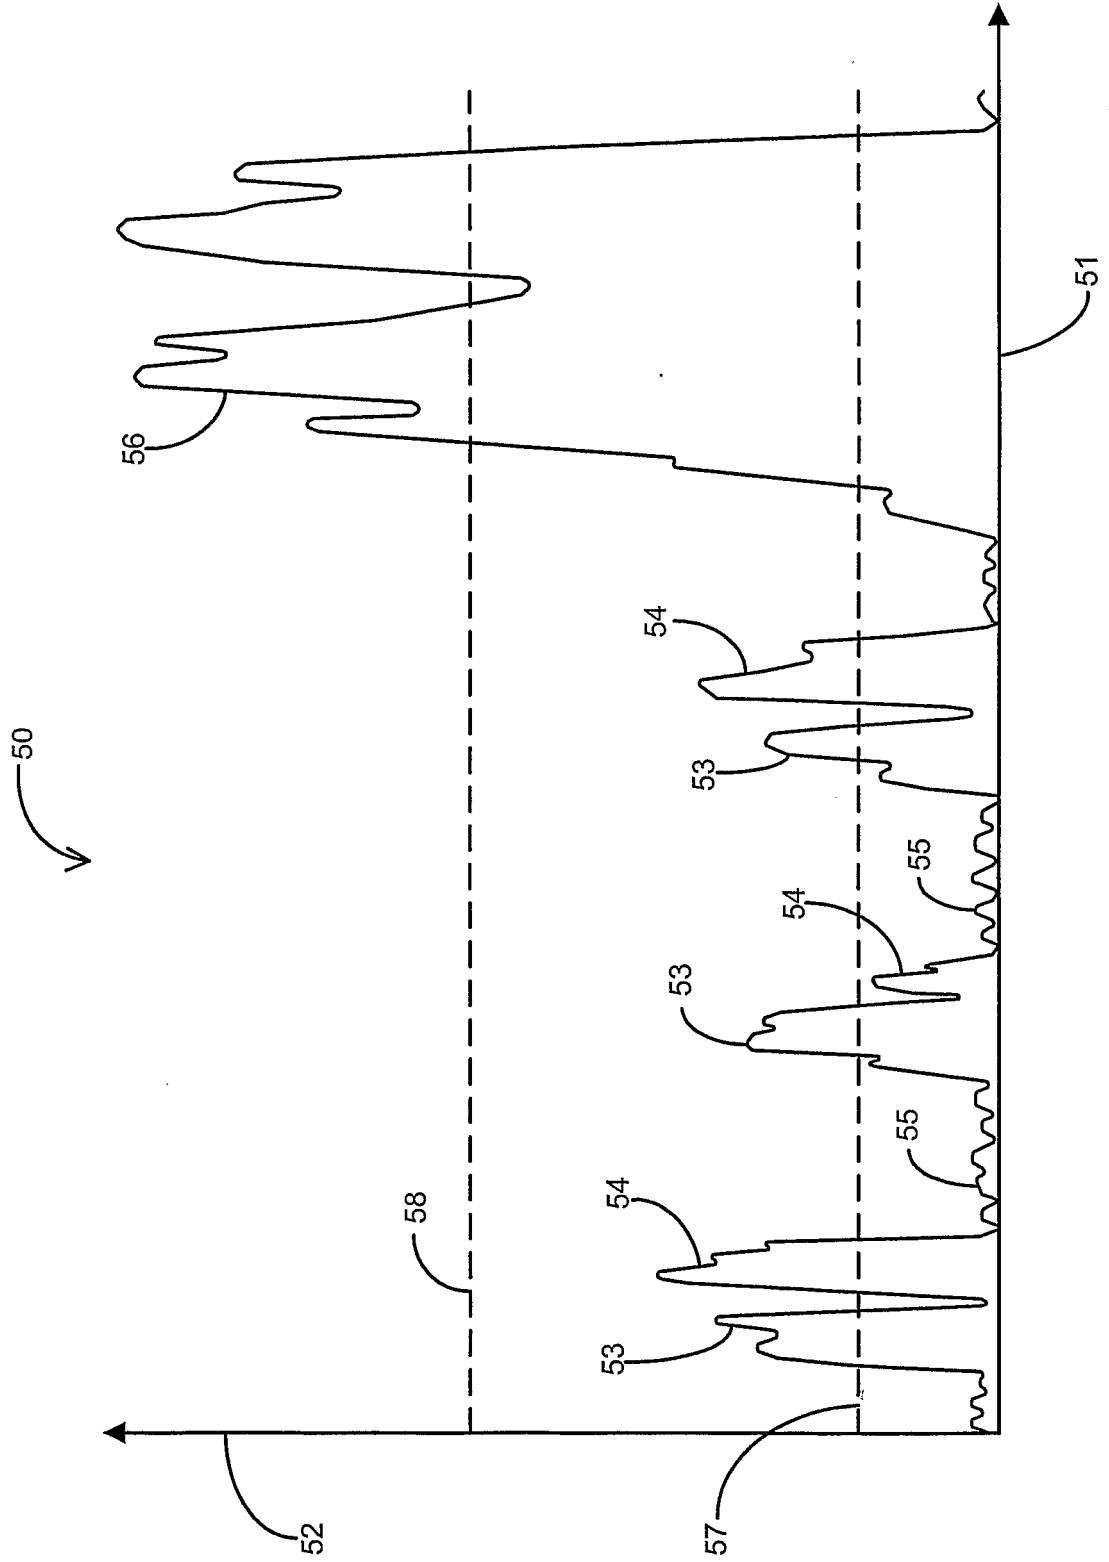


FIGURE 4

5/10

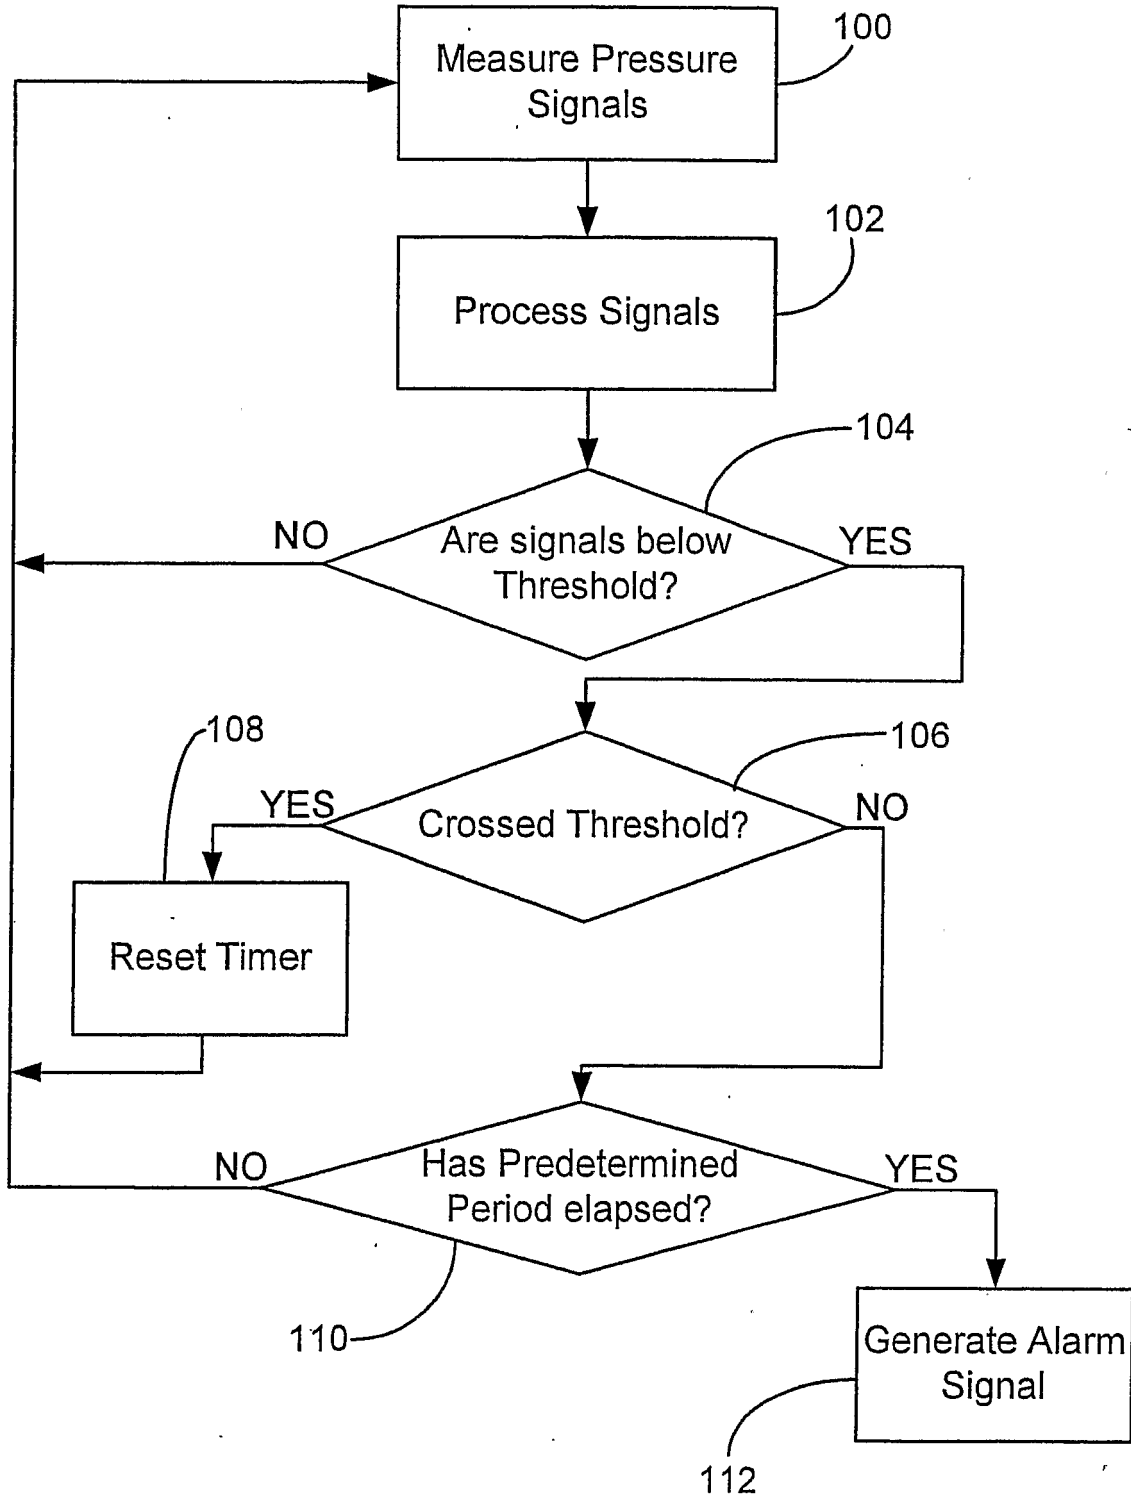


FIGURE 5

6/10

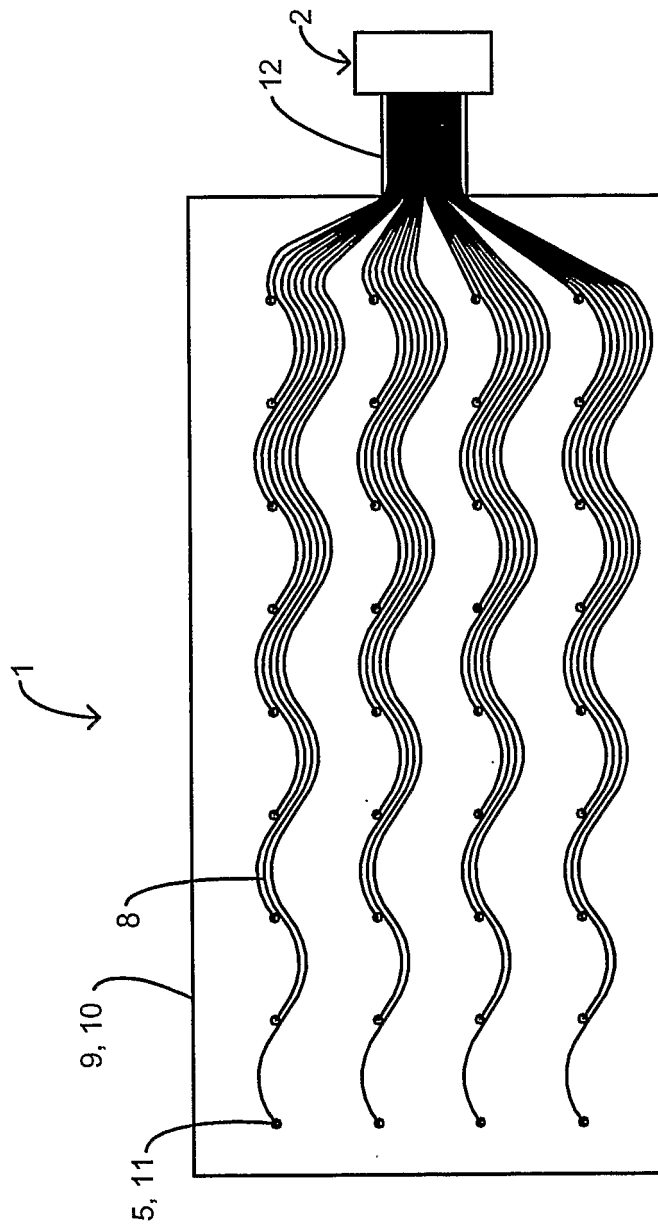


FIGURE 6

7/10

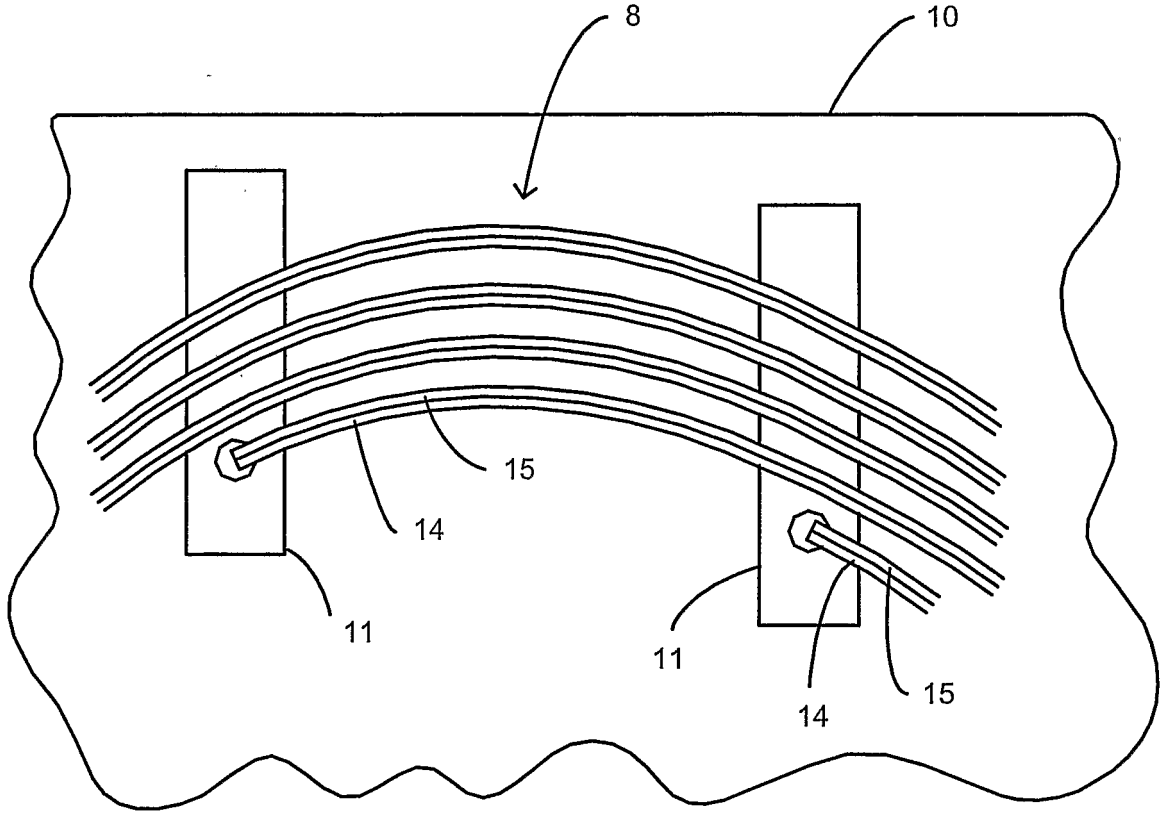


FIGURE 7(a)

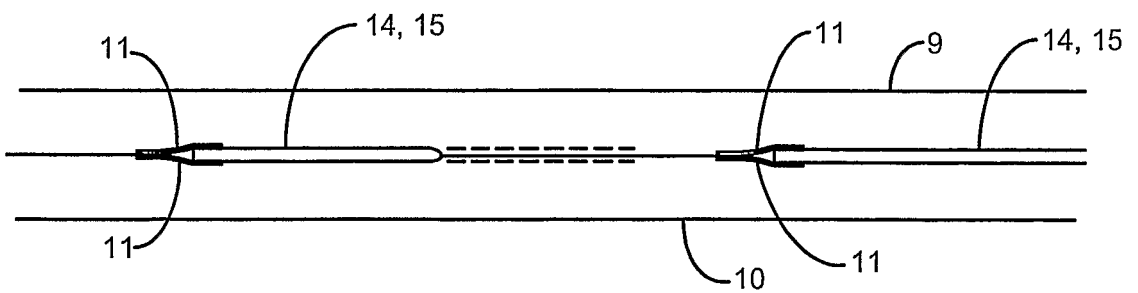


FIGURE 7(b)

8/10



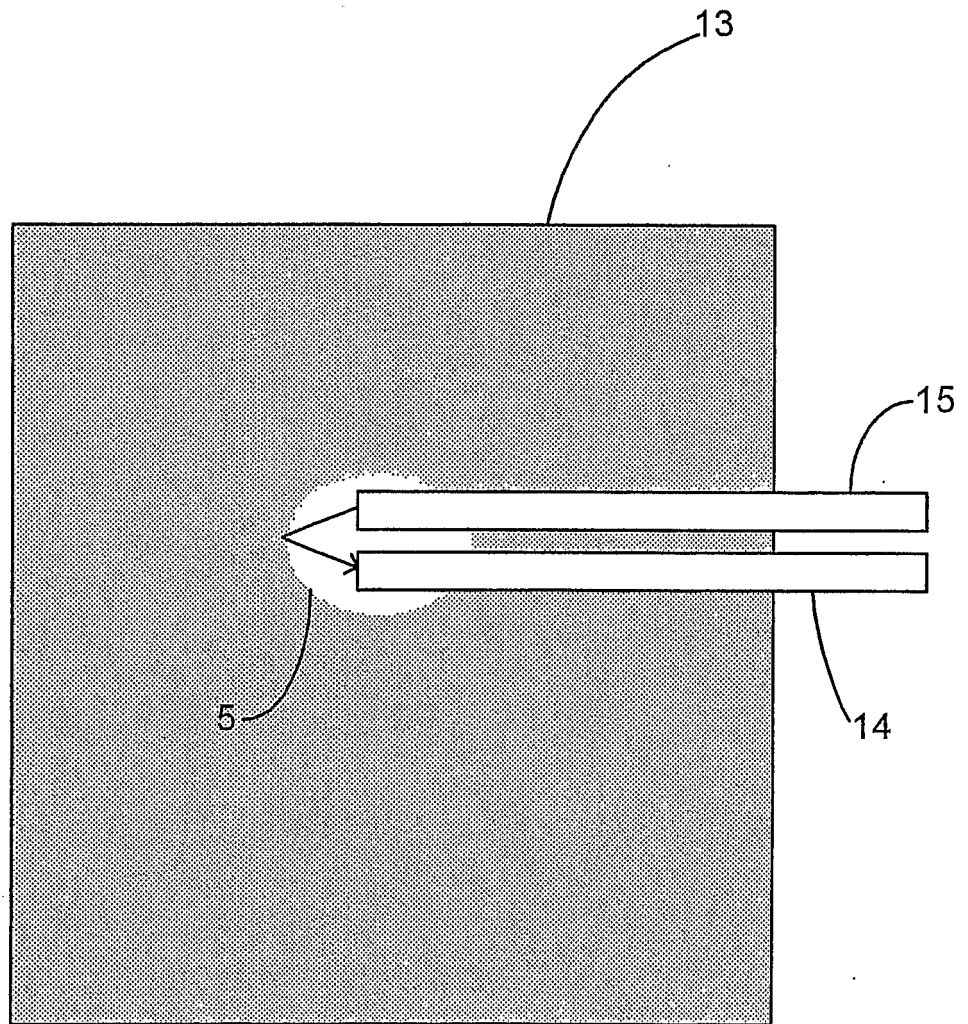


FIGURE 8


9/10

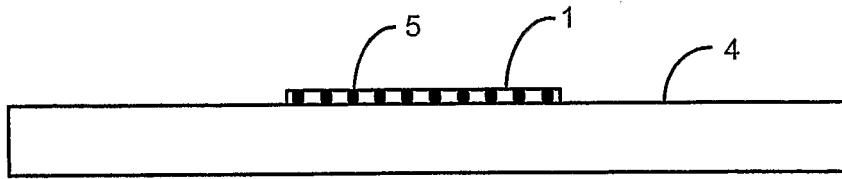


(a)

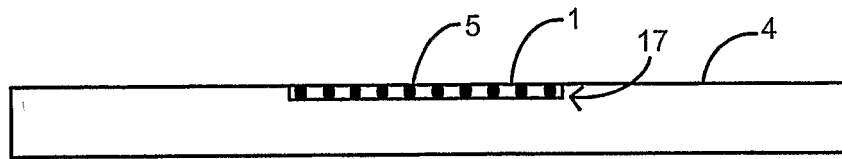


(b)

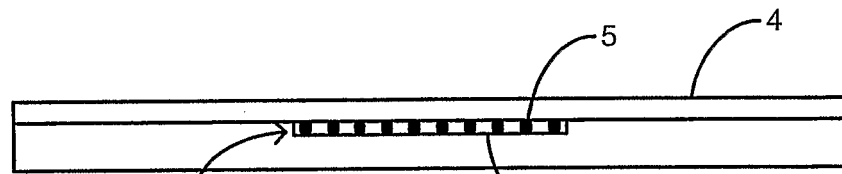

(c)

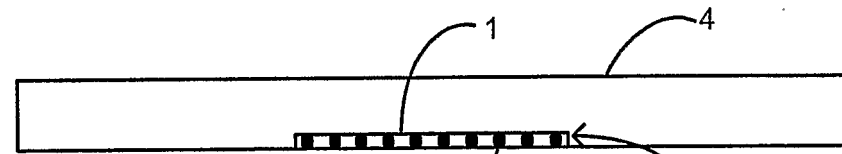

(d)

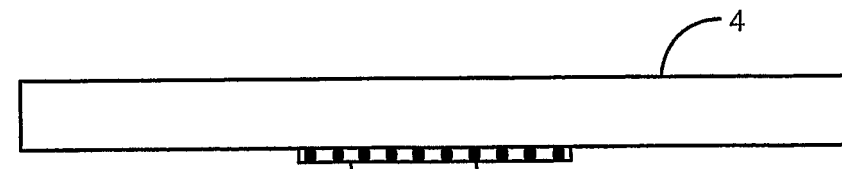

(e)

FIGURE 9

10/10

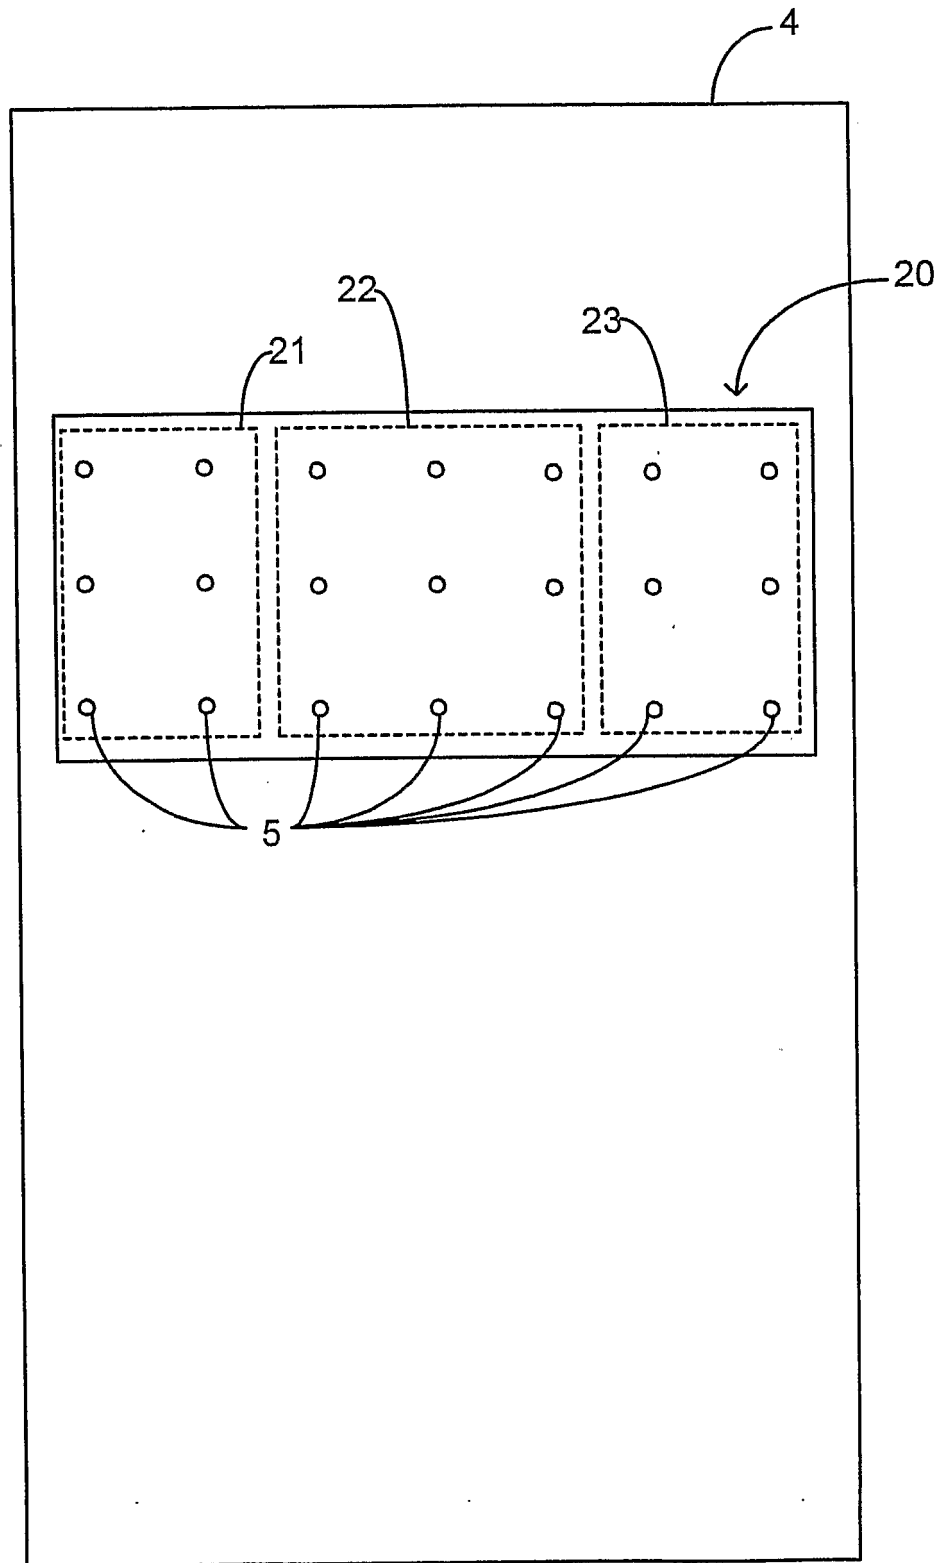


FIGURE 10

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/CA 03/01081

A. CLASSIFICATION OF SUBJECT MATTER
 IPC 7 A61B5/11 G08B21/22

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
 IPC 7 A61B G08B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 917 180 A (DANISCH LEE ET AL) 29 June 1999 (1999-06-29) cited in the application	1,8-10, 12-14, 16,17, 23,25
Y	column 8, line 61 -column 9, line 60 column 11, line 26 -column 12, line 2; figures	2-5,11, 15, 18-23,27
Y	US 4 633 237 A (SORENSEN MARTIN N ET AL) 30 December 1986 (1986-12-30) cited in the application column 3, line 21 -column 5, line 22; figures	11,15, 18-23,27
	--- -/--	

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

° Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

* & * document member of the same patent family

Date of the actual completion of the international search

16 October 2003

Date of mailing of the international search report

22/10/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
 NL - 2280 HV Rijswijk
 Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
 Fax: (+31-70) 340-3016

Authorized officer

Manschot, J

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/CA 03/01081

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 448 996 A (DINGWALL ROBERT P. ET AL) 12 September 1995 (1995-09-12)	38
Y A	column 3, line 21 -column 5, line 11; claims 1,4,5	2-5 31-37
X A	US 2001/001235 A1 (MENKEDICK DOUGLAS J ET AL) 17 May 2001 (2001-05-17) paragraphs '0060!-'0068! paragraph '0076! paragraphs '0084!-'0088!	38 1,18-24
X	US 6 280 392 B1 (HARADA TATUYA ET AL) 28 August 2001 (2001-08-28) the whole document	38
A	US 5 479 932 A (EVERBACH E. CARR ET AL) 2 January 1996 (1996-01-02) the whole document	1,31-35

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

Continuation of Box I.2

Claims Nos.: 39,40

Claims 39 and 40 refer to the description such that the scope of the claims is unclear. (see Article 6 PCT and Rule 6.2.(a) PCT).

The applicant's attention is drawn to the fact that claims, or parts of claims, relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure.

INTERNATIONAL SEARCH REPORT

International application No.
PCT/CA 03/01081

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.: ~~39, 40~~
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
see FURTHER INFORMATION sheet PCT/ISA/210

3. Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No.

PCT/CA 03/01081

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 5917180	A	29-06-1999	AT 225032 T	15-10-2002
			AU 8329298 A	10-02-1999
			BR 9811502 A	26-09-2000
			CA 2226137 A1	16-01-1999
			WO 9904234 A1	28-01-1999
			CN 1264467 T	23-08-2000
			DE 69808293 D1	31-10-2002
			DE 69808293 T2	28-05-2003
			EP 0990126 A1	05-04-2000
			ES 2184298 T3	01-04-2003
			JP 2002507279 T	05-03-2002
US 4633237	A	30-12-1986	NONE	
US 5448996	A	12-09-1995	NONE	
US 2001001235	A1	17-05-2001	US 6208250 B1	27-03-2001
			US 2002080037 A1	27-06-2002
			AU 3509400 A	21-09-2000
			BR 0008746 A	11-06-2002
			CA 2362788 A1	08-09-2000
			EP 1169001 A2	09-01-2002
			JP 2002537901 A	12-11-2002
			WO 0051541 A2	08-09-2000
US 6280392	B1	28-08-2001	JP 2001070256 A	21-03-2001
US 5479932	A	02-01-1996	NONE	

专利名称(译)	床位乘员监控系统		
公开(公告)号	EP1538984A1	公开(公告)日	2005-06-15
申请号	EP2003763555	申请日	2003-07-17
[标]申请(专利权)人(译)	TACTEX CONTROLS		
申请(专利权)人(译)	TACTEX CONTROLS INC.		
当前申请(专利权)人(译)	TACTEX CONTROLS INC.		
[标]发明人	LOKHORST DAVID M INKSTER D ROBERT		
发明人	LOKHORST, DAVID, M. INKSTER, D., ROBERT		
IPC分类号	A61B5/00 A61B5/0205 A61B5/08 A61B5/11 A61B5/113 A61G7/05 G08B21/02 G08B21/04 G08B21/22 G08B25/04		
CPC分类号	A61B5/6892 A61B5/0205 A61B5/11 A61B5/1102 A61B5/113 A61B5/447 A61B5/7239 A61B2562/0233 A61B2562/0247 A61B2562/046 A61B2562/223 G08B21/0446 G08B21/0453 G08B21/0461 G08B21/22		
代理机构(译)	EISENFÜHR, SPEISER & PARTNER		
优先权	2393880 2002-07-17 CA		
外部链接	Espacenet		

摘要(译)

本发明提供一种床乘员监视系统，其包括附接到支撑构件的压敏构件，用于支撑床乘员，压敏构件包括多个压力传感器。每个压力传感器配置成通过反射入射波能量来提供反射波能量压力信号，该强度随施加到传感器的压力而变化。一对光纤耦合到每个压力传感器，每对光纤包括输入光纤和输出光纤。光纤耦合到接口电子器件，接口电子器件包括耦合到每对光纤的输入光纤的波能源，用于提供所施加的光能；以及波能探测器，耦合到每对光纤的输出光纤，用于将散射的光能转换成电信号。