



(11)

**EP 2 294 973 A2**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**16.03.2011 Bulletin 2011/11**

(51) Int Cl.:  
**A61B 5/00** (2006.01)

(21) Application number: **10010532.9**

(22) Date of filing: 10.10.2002

(84) Designated Contracting States:  
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR  
IE IT LI LU MC NL PT SE SK TR

- O'Neil, Michael Patrick  
California, 94086 (US)
- Chin, Rodney  
California, 94611 (US)
- Adnan, Merchant  
California, 94539 (US)

(30) Priority: 12.10.2001 US 328924 P

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:  
**02801052.8 / 1 435 834**

(74) Representative: **Kinsler, Maureen Catherine et al**  
**Marks & Clerk LLP**  
**Aurora**  
**120 Bothwell Street**  
**Glasgow**  
**G2 7JS (GB)**

(71) Applicant: **Nelcor Puritan Bennett LLC**  
**Pleasanton, CA 94588 (US)**


- (72) Inventors:
- **Hannula, Don**  
**California, 93401 (US)**
  - **Coakley, Joseph**  
**California, 94588 (US)**
  - **Mannheimer, Paul D.**  
**California, 94506 (US)**

## Remarks:

This application was filed on 24-09-2010 as a divisional application to the application mentioned under INID code 62.

(54) **Stacked adhesive optical sensor**

(57) A sensor comprising: a sensor body; and an emitter and a detector coupled to the sensor body, wherein the sensor body is configured to hold the emitter and the detector at a substantially fixed distance relative to one another when the sensor is applied to a patient.

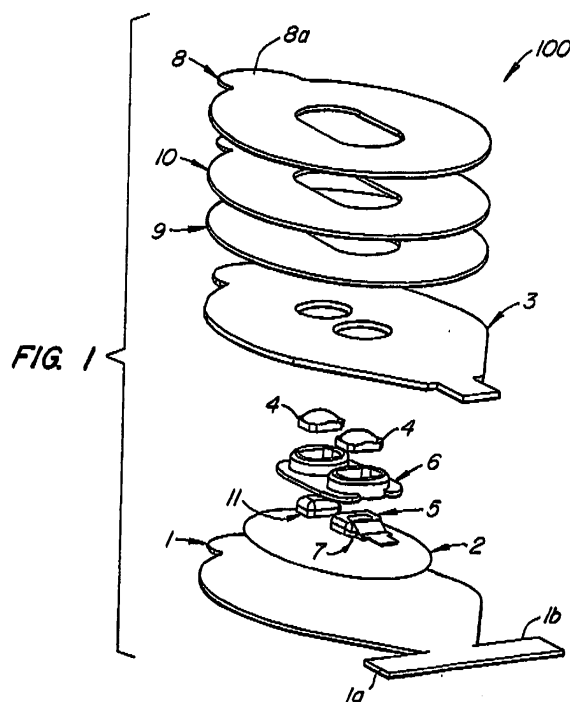

## Description

### CROSS-REFERENCE TO RELATED APPLICATION

**[0001]** The present application claims priority to U.S. Provisional Patent Application No. 60/328,924, filed October 12, 2001, the teachings of which are incorporated herein by reference for all purposes.

### BACKGROUND OF THE INVENTION

**[0002]** The present invention relates to optical sensors, and in particular to pulse oximeter sensors.

**[0003]** Many types of optical sensors are used to measure physiological characteristics of a patient. Typically, an optical sensor provides emitted light which is then scattered through a portion of a patient's tissue and detected. Various characteristics of a patient can be determined from analyzing such light, such as oxygen saturation, pulse rate, tissue bilirubin, etc.

**[0004]** Pulse oximetry is typically used to measure various blood flow characteristics including, but not limited to, the blood-oxygen saturation of hemoglobin in arterial blood, the volume of individual blood pulsations supplying the tissue, and the rate of blood pulsations corresponding to each heartbeat of a patient. Measurement of these characteristics has been accomplished by use of a non-invasive sensor which scatters light through a portion of the patient's tissue where blood perfuses the tissue, and photoelectrically senses the absorption of light in such tissue. The amount of light absorbed is then used to calculate the amount of blood constituent being measured.

**[0005]** The light scattered through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of transmitted light scattered through the tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption. For measuring blood oxygen level, such sensors have typically been provided with a light source that is adapted to generate light of at least two different wavelengths, and with photodetectors sensitive to both of those wavelengths, in accordance with known techniques for measuring blood oxygen saturation.

**[0006]** Known non-invasive sensors include devices that are secured to a portion of the body, such as a finger, an ear or the scalp. In animals and humans, the tissue of these body portions is perfused with blood and the tissue surface is readily accessible to the sensor.

**[0007]** Certain types of optical sensors are applied to a patient's external tissue by way of an adhesive attachment, enabled by an adhesive layer on the sensor. During the monitoring of a patient, there is a need to remove the sensor to perform a site check of the tissue location, and this removal typically damages the adhesive layer. Furthermore, adhesive type sensors are often used with dis-

posable type sensors where the photo emitter and the detector are mounted on a backing without the benefit of a rigid optical mount to maintain the emitter and detector's separation relatively fixed, and thus the sensor is subject to motion induced artifacts that may adversely affect measurement accuracy.

**[0008]** There is therefore a need to improve the functionality of adhesive-type optical sensors.

### BRIEF SUMMARY OF THE INVENTION

**[0009]** The present invention provides an optical sensor having a cover layer, an emitter disposed on a first side of the cover, a detector disposed on the first side of said cover, and a plurality of stacked independent adhesive layers disposed on the same first side of the cover, wherein the top most exposed adhesive layer is attached to a patient's skin. Thus, when the sensor is removed to perform a site check of the tissue location, one of the adhesive layers may also be removed and discarded, exposing a fresh adhesive surface below for re-attachment to a patient's skin. The independent pieces of the adhesive layers can be serially used to extend the useful life of the product.

**[0010]** One aspect of the present invention is directed towards using a generally annulus-shaped adhesive layer that surround the emitter and the detector and thus avoids having any adhesive present between the emitter and the detector to minimize optical shunt, which is known to adversely affect measurement accuracy.

**[0011]** Another aspect of the present invention is directed towards using optical lenses made from a soft or compliant material such as an optically transparent PVC material to minimize tissue necrosis.

**[0012]** Another aspect of the invention is directed towards the use of a semi-rigid optical mount structure to hold the emitter and the detector in place to maintain the separation between the electro-optics (emitter and detector) relatively fixed and yet allow a certain minimal amount of torque and twisting to occur as the sensor is applied. The semi-rigid optical mount, by maintaining the separation relatively fixed reduces motion induced artifacts in the detected electro-optic signals, which may adversely interfere with measurement accuracy. For a further understanding of the nature and advantages of the present invention, reference should be made to the following description in conjunction with the accompanying drawings.

### BRIEF DESCRIPTION OF THE DRAWINGS

**[0013]** Fig. 1 is a perspective disassembled view of the sensor according to an embodiment of the present invention.

**[0014]** Fig. 2 is a perspective view of the sensor according to an embodiment of the present invention.

**[0015]** Fig. 3 is a top view of the embodiment of Fig. 2.

**[0016]** Fig. 4 is a sectional view "A-A" of Fig. 3.

**[0017]** Fig. 5 is a perspective view of an alternate embodiment of the sensor of the present invention having a hinged lid.

**[0018]** Fig. 6 is a diagram showing the sensor of Fig. 5 positioned on a patient during a site check.

## DETAILED DESCRIPTION OF THE INVENTION

**[0019]** Fig. 1 is a perspective disassembled view of the sensor 100 according to an embodiment of the present invention. The sensor includes a sensor top 1 or cover layer which is exposed to the ambient environment when the sensor is attached to a patient's skin. In one embodiment, the cover layer 1 is fabricated of a common PVC foam. Alternately, the cover layer 1 is fabricated of a urethane foam material and particularly, an open cell breathable urethane foam such as, for example, the PORON™ family of urethanes commercially available from the Rogers corporation of Connecticut. A mask layer 2 preferably including a metalized plastic film is adhesively attached to the cover layer 1. In a preferred embodiment, the metalized mask layer 2 is an aluminized polypropylene film with a synthetic adhesive layer for attachment to the cover layer 1. The metalized mask layer 2 is so placed to prevent, minimize or reject secondary light from interfering with the photodetector 7. As used herein, secondary light includes all light that originates from sources other than the emitter 11, and which may have originated from sources including ambient or surgical light sources. An emitter 11 is placed above the mask layer 2. The emitter 11 is configured to direct light at predetermined wavelengths at a patient's skin. The light directed to the patient's skin is scattered through the patient's tissue and is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of blood constituent present in the body. A photo detector 7 is also placed above the mask layer 2 and adjacent to the emitter 11 to detect the amount of light that has been diffused through the patient's tissue. The amount of light that has diffused through the patient's tissue will vary in accordance with the changing amount of blood constituent in the tissue and the related light absorption.

**[0020]** For measuring blood oxygen level, the emitter is adapted to generate light of at least two different wavelengths, in accordance with known techniques for measuring blood oxygen saturation. The sensor, when adapted for blood oxygen saturation is useable for not only adult patients, but may also be adapted for use for neonatal and pediatric patients. Adaptations for neonatal and pediatric use may include accommodations of size and/or adhesive materials more compatible with the geometry and skin characteristics of those patients. Further, the sensor may optionally use emitters of different wavelengths and hence may use emitter and detector combinations that lead to more accurate readings at low blood oxygen saturations, which is the case for some patients. Light sources which are optimized for low oxygen satu-

ration ranges are described in United States Patent No. 5,782,237, entitled: "Pulse Oximeter and Sensor Optimized for Low Saturation," assigned to the assignee herein, the disclosure of which is hereby incorporated by reference herein in its entirety.

**[0021]** A Faraday shield 5 is placed in front of photodetector 7 to reduce the effect of extrinsic electrical fields that could adversely affect the electrical signal from the photodetector. A semi-rigid optical mount 6 is placed above the mask layer 2, and which surrounds and holds the emitter 11 and the detector 7 in a manner to maintain the separation between the emitter 11 and the detector 7 fixed and yet allow a certain minimal amount of flexing and twisting to occur as the sensor is applied to a patient. Without the semi-rigid optical mount in place, torque can often cause orientation changes between the emitter 11 and the detector 7 which can interfere with the accuracy of the measurements obtained by the sensor through changes in calibration and motion-induced artifact. Furthermore, the semi-rigid optical mount 6 substantially reduces the flex and the twist which may also create significant motion artifact, which is also known to adversely affect measurement accuracy. In one embodiment, the semi-rigid optical mount 6 is manufactured from a black polypropylene material. The black color of the optical mount also reduces the potential for optical shunt between the emitter and the detector, which can also cause measurement inaccuracies. Windows or lenses 4 are attached or bonded using a suitable adhesive (e.g., an ultraviolet cure adhesive process), one each to the detector and the emitter to assist in coupling the light emitted from the emitter 11 into the tissue, and collected from the tissue and directed towards the detector 7. In one embodiment, the lenses 4 are made of an optically transparent plastic material to minimize optical attenuation. In an alternate embodiment, the lenses 4 are made of a compliant material such as a transparent PVC, urethanes, or room temperature vulcanized (RTV) material, and so on. The choice of selecting a compliant material for the lenses is driven by the desire to prevent the possibility of necrosis of the skin, when the sensor is applied to the patient. Preferably, the compliant material has a hardness of less than 60 on a Shore A durometer scale. Alternately, or in addition to the lenses, the emitter and/or the detector arrangements may also include optical diffusers. The advantage of using optical diffusers is that the sensor would have less sensitivity to tissue heterogeneity, and thus provide more uniform and more accurate results.

**[0022]** A mask layer 3 is adhesively connected with the parts below it. The mask layer 3 has openings therein that fit over and surround the optical mount 6 placed below it (the mask layer 3). The mask layer 3 serves as a substantially flat platform for the subsequent attachment of the stack of adhesive layers. In one embodiment, the mask layer is fabricated from a cellular urethane foam such as the PORON™ family of urethane foams, and is attached to the cover layer 1 using a pressure sensitive

adhesive. Lastly, a stack of adhesive layers 8, 9, and 10 are placed above the mask layer 3. The lower most adhesive layer 9 is attached to the mask layer 3 using an acrylic transfer adhesive. While in one embodiment a stack of three adhesive layers is placed above the mask layer 3, other multiple stacked adhesive layers are also within the scope of the embodiments of the present invention.

**[0023]** In one embodiment, the adhesive layers are in a ring shape so that no adhesive is present between the photo emitter 11 and the photo detector 7, thereby minimizing optical shunt between the photo emitter and the photo detector, which is known to lead to measurement inaccuracies. The adhesive layers or rings may be manufactured of a polyethylene film having an acrylic adhesive on one side for attachment to the patient's tissue. Alternately, the adhesive layers or rings may have an adhesive layers on both sides, in which case the adhesive layers are separated from one another by release layers (e.g. release paper). Preferably, the adhesive layers include a non-adhesive tab portion (e.g. 8a), arranged stacked or in a fanned-out array, to enable the clinician to easily grab and remove the used adhesive layer to expose the layer below. The tab portions may be non-adhesive colored tabs (e.g., green, yellow, red, lavender, oranges) to enable the easy removal of the adhesive rings. Additionally, another release layer (not shown) is placed above the stack of adhesive layers to cover the very first adhesive layer while it is in storage.

**[0024]** In certain embodiments, the adhesive rings are black to minimize reflected light, which is known to impact the accuracy of optical-based measurements. In certain embodiments, the adhesive rings are thermally stable, so that the adhesion between the rings is not compromised as a result of exposure to heat. Additionally, the adhesive rings may include a release agent, such as, for example, a low molecular weight silicone oil on the back side of the ring, in order to minimize or prevent adjacent rings from sticking to one another. Various alternate ring construction may be employed, including a continuous 0.001 inch thick polyethylene film with acrylic pressure sensitive adhesive on one side. The continuous film can be made of other materials such as polyester, polyimide or Teflon, to achieve specific strength, release and temperature stability requirements. The adhesives used on the surface of the film can be acrylic, synthetic rubber, natural rubber (e.g., latex) or other non-toxic adhesive. The ring may include a paper with a release agent on one side as the carrier film. This allows printing on each release liner, user information such as "adhesive layer #1" or can be inked black to control optical shunt.

**[0025]** Alternately, the adhesive rings need not be in a ring shape, but may be continuous adhesive surface, with a black strip between the emitter and detector in order to minimize optical shunt.

**[0026]** The pre-attached stacks of adhesive layers enables the extended use of a disposable adhesive-type sensor. A desired feature for sensors is the ability to

check the sensor site periodically (e.g. once every 12 hours), and remain capable of continuous use for multiple days. In prior disposable sensors which were adhesively attached to a patient's skin, multiple cycles of repositioning the sensor was not possible due to the degradation of the adhesive and the sloughing nature of the tissue beneath the sensor attachment location. This failed reattachment would necessitate the replacement of the sensor in its entirety, which would increase the overall cost of the patient monitoring procedure. However, with the use of a stack of pre-attached adhesive rings, when the sensor is removed to perform a site check, one of the adhesive layers may also be removed exposing a fresh adhesive surface below. Thus, having several independent pieces of adhesive layers that can be serially used, extends the useful life of the product and reduces the overall costs of the patient monitoring procedure.

**[0027]** Fig. 2 is a perspective view of the assembled sensor 100. This figure (Fig. 2) shows the top most adhesive layer 8, and lenses 4 covering the photo emitter 11 and photo detector 7. Furthermore, Fig. 2 shows cable 14 attached to the sensor 100. Tab portions 1a and 1b (shown in Fig. 1) wrap around the cable 14 to hold the cable and the sensor in a stable manner. Cable 14 attaches to the photo emitter 11 and detector 7 via traces or wires (not shown).

**[0028]** Fig. 3 is a top view of the embodiment of Fig. 2. Fig. 3 also shows the top most adhesive layer 8, and lenses 4 covering the photo emitter 11 and photo detector 7. Furthermore, Fig. 2 shows cable 14 attached to the sensor 100. Fig. 4 shows sectional view "A-A" of Fig. 3. Fig. 4 shows the cover layer 1, the top most adhesive layer 8 and lenses 4 which are placed above the photo emitter 11 and photo detector 7. As can be seen from Fig. 4, the sensor 100 is substantially flat, while the lenses 4 protrude outward from a plane of the sensor. Thus, when attached, the lenses push on the patient's tissue location (e.g. forehead) to enhance light coupling and the depth of optical penetration by pressing mildly into the skin. Since the lenses protrude outward from the sensor plane, the adjacent adhesive layers necessarily lie in a plane which is offset or away from the patient's tissue location, thus "pulling" the lenses into the skin during use. This assures good optical contact between sensor and tissue, and reduces the potential contribution of light shunting.

**[0029]** Fig. 5 is a perspective view of an alternate embodiment of the sensor 200 of the present invention having a hinged lid. The sensor 200 includes a ring-shaped layer 202 having an adhesive side, which is configured to be attached to a patient during monitoring. The sensor 200 also includes a hinged lid 204 which holds the necessary electro-optics including a photo emitter and a photo detector (not shown) as described above. The hinged lid 204 is coupled to the ring-shaped adhesive layer 202 by a hinged connection 208 that enables the lifting and the checking of the sensor site without the need to remove the sensor from the patient. Cable 210 provides

the leads or wires connected with the photo detector and photo emitter for the proper operation of the sensor. A clasp 206 secures the hinged lid 204 in a position effective for patient monitoring. The clasp 206 is also used by a clinician to lift the hinged lid 204 for checking the sensor site. In one embodiment, the clasp 206 adhesively engages the ring-shaped layer 202. In an alternate embodiment, the clasp 206 engages the ring-shaped layer via a mechanical clasp-type connection. The ring-shaped layer 202 may also incorporate a stacked adhesive arrangement as described above to enable the repeated removal and re-attachment of the sensor to the patient.

**[0030]** Fig. 6 is a diagram showing the sensor of Fig. 5 positioned on a patient during a site check. As can be seen from this figure (Fig. 6), the ring-shaped layer 202 is adhesively attached to a patient, while the hinged lid 204 containing the photo emitter 212 and photo detector 214 is lifted from the patient's forehead to enable the checking of the tissue location underneath the sensor site. Cable 210 provides the leads or wires connected with the photo detector and photo emitter for the proper operation of the sensor.

**[0031]** The multiple stacked adhesive layer embodiments and the hinged lid embodiments of the present invention may be also be used to improve the operation of any disposable sensor and particularly disposable oximeter sensors. These disposable sensors include sensors based on the reflectance of light from tissue to the detector (as described above with the emitter and the detector placed on the same side of the tissue) as well as transmissive type sensors, where the emitter and the detector are placed on opposite sides of a tissue site being probed. Examples of sensors that can incorporate the multiple stacked adhesive layer embodiments or the hinged-lid embodiments include the adhesive, and reusable sensors for use at various tissue locations, including the finger tip, foot, nose, and forehead locations such as the D-20, D-25, N-25, I-20, R-15, as well as the A, N, I, and P series of sensors manufactured by the assignee herein.

**[0032]** Furthermore, the multiple stacked adhesive layer embodiments and the hinged lid embodiments of the present invention are not only useable for adult patients, but are also useable with patients on whom it is sometimes preferable to use a soft gel adhesive to minimize the occurrence of tearing of the skin. Such patients include geriatric, pediatric or neonatal patients. The inclusion of a soft gel in an optical sensor is described in United States Patent No. 5,830,136, entitled: "Gel Pad Optical Sensor," assigned to the assignee herein, the disclosure of which is hereby incorporated herein in its entirety. An alternate embodiment of a soft gel adhesive includes only a single adhesive layer (not stacked), since some gel materials can be cleaned with water or other liquid agents to refresh the adhesive properties. As such, the use of multiple layers of gel adhesive may not be required for limited but multiple sensor placements on an individual patient.

**[0033]** As will be understood by those skilled in the art, the present invention may be embodied in other specific forms without departing from the essential characteristics thereof. For example, the disposable sensor may be a forehead or a nasal sensor, the sensor may be configured for use on an adult, pediatric or neonatal patient, the sensor may use several possible arrangements of adhesive layers arranged in an stacked manner, or the sensor may use suitable materials other than those described above. These other embodiments are intended to be included within the scope of the present invention, which is set forth in the following claims. The following clauses are included and form part of the specification:

Clause 1. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer.

Clause 2. The sensor of clause 1 wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector.

Clause 3. The sensor of clause 1 further comprising a first lens disposed above said emitter, and a second lens disposed above said detector, wherein said first and said second lenses are made of an optically transparent and compliant material.

Clause 4. The sensor of clause 3 wherein said compliant material is an optically transparent material selected from the group of materials consisting of PVC, urethane, RTV and combinations thereof.

Clause 5. The sensor of clause 3 wherein said compliant material is optically transparent and has a durometer hardness of approximately less than 60 Shore A.

Clause 6. The sensor of clause 1 wherein said sensor comprises a substantially flat surface and wherein said emitter and said detector protrude outward from said substantially flat surface.

Clause 7. The sensor of clause 1 wherein said sensor comprises a curved surface configured to fit the curvature of a patient's forehead and wherein said emitter and said detector protrude outward from said curved surface.

Clause 8. The sensor of clause 7 wherein said curved surface is configured to fit the curvature of the forehead of a neonatal or pediatric patient.

Clause 9. The sensor of claim 1 further comprising a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively. 5 10

Clause 10. The sensor of clause 1 further comprising an optically opaque layer disposed between said cover layer and said detector. 15

Clause 11. The sensor of clause 1 wherein said sensor is an oximeter sensor,

Clause 12. A sensor comprising: 20

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
and a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector. 25 30

Clause 13. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a first lens disposed above said emitter; a second lens disposed above said detector, wherein said first and said second lenses are made of a compliant material; and a plurality of stacked independent adhesive layers disposed on said first side of said cover layer. 35 40 45

Clause 14. The sensor of clause 13 wherein said soft material is an optically transparent material selected from the group of materials consisting of PVC, urethane, RTV and combinations thereof. 50

Clause 15. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer; and 55

a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein said sensor comprises a substantially flat surface and wherein said emitter and said detector protrude outward from said substantially flat surface.

Clause 16. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer.

Clause 17. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer; a detector disposed on said first side of said cover layer;  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer; and  
an optically opaque layer disposed between said cover layer and said detector.

Clause 18. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector.

Clause 19. A sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;

a detector disposed on said first side of said cover layer; a first lens disposed above said emitter; a second lens disposed above said detector, wherein said first and said second lenses are made of a compliant material, wherein said soft material is an optically transparent PVC; 5  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; 10  
and a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector. 15

Clause 20. A sensor as in any one of clauses 9-15 wherein said sensor is an oximeter sensor. 20

Clauses 21. An oximeter sensor comprising:

a cover layer; 25  
an emitter disposed on a first side of said cover layer; a detector disposed on said first side of said cover layer; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer. 30

Clause 22. An oximeter sensor comprising:

a cover layer; 35  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector. 40

Clause 23. An oximeter sensor comprising: 45

a cover layer; 50  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; and 55  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer,

wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector.

Clause 24. An oximeter sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a first lens disposed above said emitter;  
a second lens disposed above said detector, wherein said first and said second lenses are made of a compliant material, wherein said soft material is an optically transparent PVC;  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; and  
a plurality of stacked independent adhesive layers disposed on said first side of said cover layer, wherein each of said adhesive layers is a ring shaped layer surrounding said emitter and said detector, and wherein no adhesive is present between said emitter and said detector.

Clause 25. A sensor comprising:

a generally annulus-shaped base, said base configured for attachment with a tissue location on a patient;  
a lid hingedly connected at its near end with a near end of said base;  
an emitter disposed on a first side of said lid;  
a detector disposed on said first side of said lid; and  
a clasp connected with a far end of said lid and configured to engage a far end of said base.

Clause 26. The sensor of clause 25 further comprising an adhesive layer disposed on a first side of said generally annulus-shaped base for attachment with a tissue location on a patient.

Clause 27. The sensor of clause 25 further comprising a plurality of stacked independent adhesive layers disposed on a first side of said generally annulus-shaped base for attachment with a tissue location on a patient.

Clause 28. The sensor of clause 25 wherein said sensor is configured to operate in a first mode and a second mode, wherein in said first mode said clasp engages said base, and said lid and said base together form a substantially flat sensor, and wherein

in said second mode, said clasp is disengaged from said base and said lid is lifted from said tissue location.

Clause 29. The sensor of clause 25 wherein said sensor is an oximeter sensor.

Clause 30. An oximeter sensor comprising:

a cover layer;  
an emitter disposed on a first side of said cover layer;  
a detector disposed on said first side of said cover layer;  
a substantially rigid optical mount disposed on said cover layer, said optical mount having first and second apertures therein, wherein said first and said second apertures surround said emitter and said detector respectively; and  
a soft gel adhesive layer disposed on said first side of said cover layer, wherein said gel adhesive layer is a ring-shaped layer surrounding said emitter and said detector, and wherein no gel is present between said emitter and said detector.

Clause 31. The sensor of clause 30 wherein said gel adhesive layer is comprised of two or more separable layers.

## Claims

1. A sensor comprising: a sensor body; and an emitter and a detector coupled to the sensor body, wherein the sensor body is configured to hold the emitter and the detector at a substantially fixed distance relative to one another when the sensor is applied to a patient.
2. The sensor of claim 1, wherein the sensor body comprises a semi-rigid optical mount configured to hold the emitter and the detector at the substantially fixed distance.
3. The sensor of claim 2, wherein the semi-rigid optical mount comprises a first aperture and a second aperture, and wherein the emitter and the detector are disposed in the first aperture and the second aperture, respectively.
4. The sensor of claim 2 or claim 3, wherein the semi-rigid optical mount comprises a polypropylene material.
5. The sensor of any of claims 2 to 4 wherein the semi-rigid optical mount is black,
6. The sensor of any of the preceding claims, wherein the sensor comprises a pulse oximetry sensor or a reflectance-type sensor.
7. The sensor of any of the preceding claims, wherein the emitter and the detector are coupled to a patient contact side of the sensor body, and wherein the sensor comprises a plurality of stacked independent adhesive layers disposed on the patient contact side of the sensor body, the plurality of stacked independent adhesive layers being configured to adhere to a tissue location on a patient.
8. The sensor of any of the preceding claims, comprising a sensor base having an opening therein, and wherein the sensor body is configured to be disposed in the sensor base, and wherein one end of the sensor body is pivotally connected to the sensor base.
9. The sensor of claim 8 comprising a clasp connected with another end of the sensor body, and wherein the clasp is configured to engage the sensor base.
10. The sensor of any of the preceding claims, comprising an adhesive layer disposed on a patient contact side of the sensor base, the adhesive layer configured to adhere to a tissue location on a patient.
11. The sensor of any of the preceding claims wherein the emitter and the detector protrude beyond a patient contact side of the sensor body.
12. A method comprising: fixing the distance between an optical emitter and a photodetector of a sensor relative to one another when the sensor is applied to a patient such that patient movement does not alter the distance.
13. The method of claim 12, wherein fixing the distance between the emitter and the detector comprises:
  - coupling a semi-rigid optical mount to the sensor body and/or
  - holding the emitter and the detector at a fixed distance relative to one another with at least the semi-rigid optical mount and/or
  - surrounding the emitter and the detector with a semi-rigid optical mount comprising a first aperture and a second aperture, wherein the emitter and the detector are sized to be disposed in the first aperture and the second aperture, respectively.
14. A method of manufacturing a pulse oximetry sensor, comprising:
  - providing a sensor body to which an emitter and a detector are coupled, wherein the sensor body



is configured to hold the emitter and the detector at a substantially fixed distance relative to one another.

15. The method of claim 14 comprising: providing a semi-rigid optical mount, wherein the semi-rigid optical mount is configured to hold the emitter and the detector at the substantially fixed distance. 5
16. The method of claim 14 comprising: coupling the semi-rigid optical mount to the sensor body. 10
17. The method of claim 14 comprising: surrounding the emitter and the detector with the semi-rigid optical mount, wherein the semi-rigid optical mount comprises a first aperture and a second aperture, wherein the emitter and the detector are sized to be disposed in the first aperture and the second aperture, respectively. 15

20

25

30


35


40

45


50

55

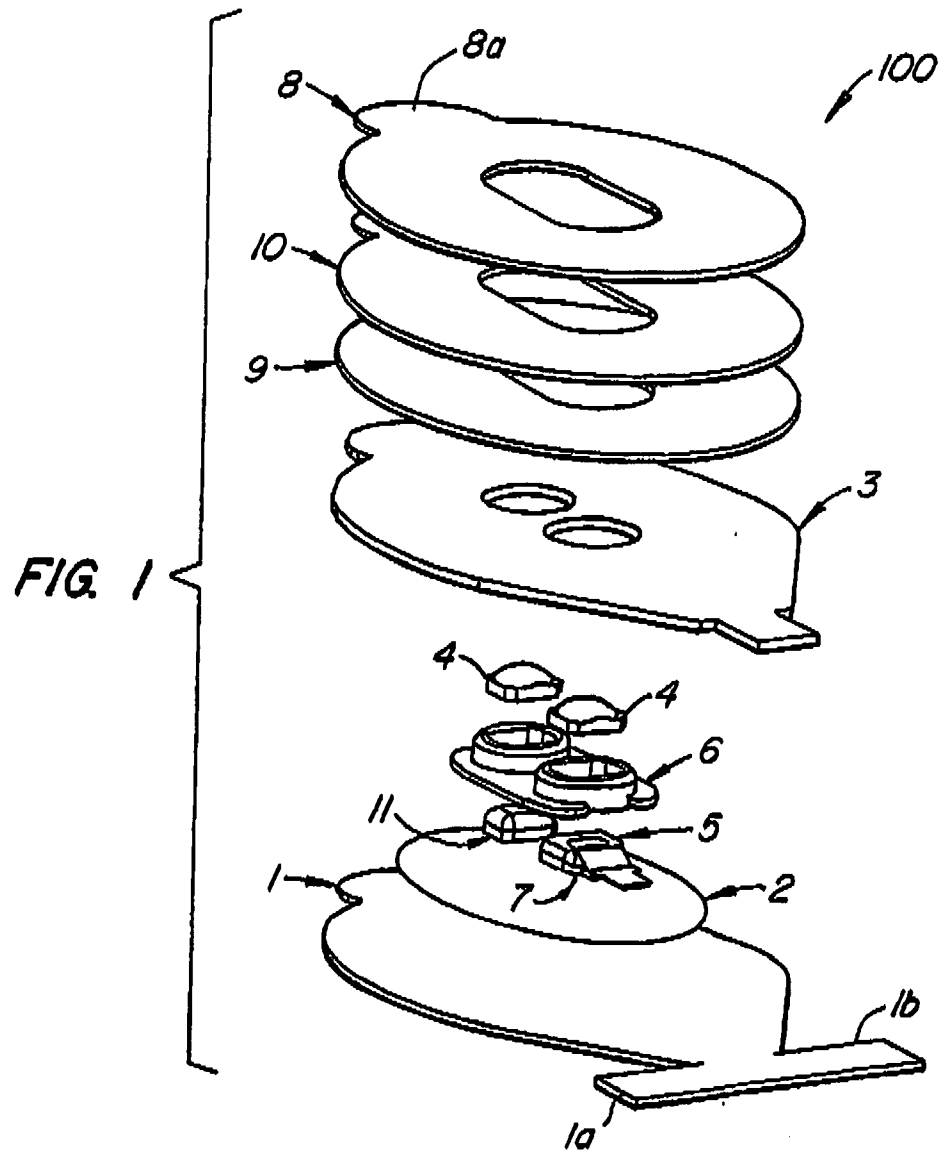


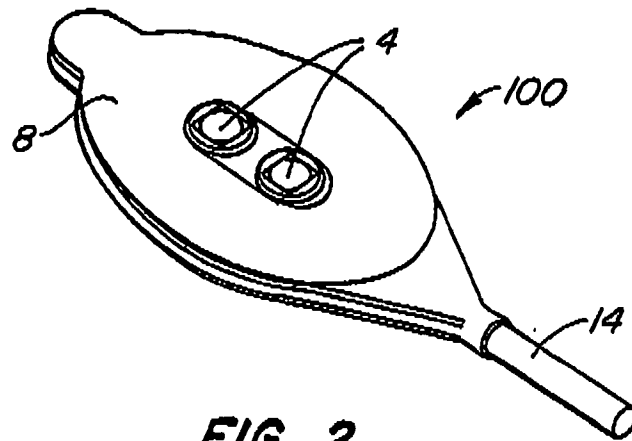


**FIG. 2**

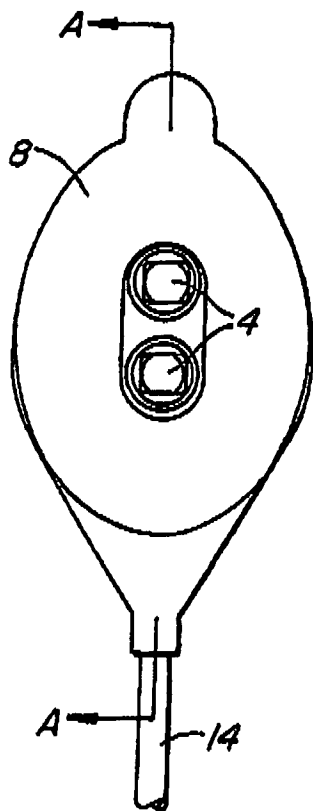


**FIG. 3**

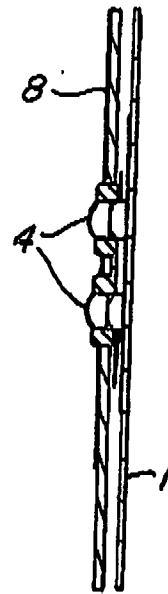

**FIG. 4**

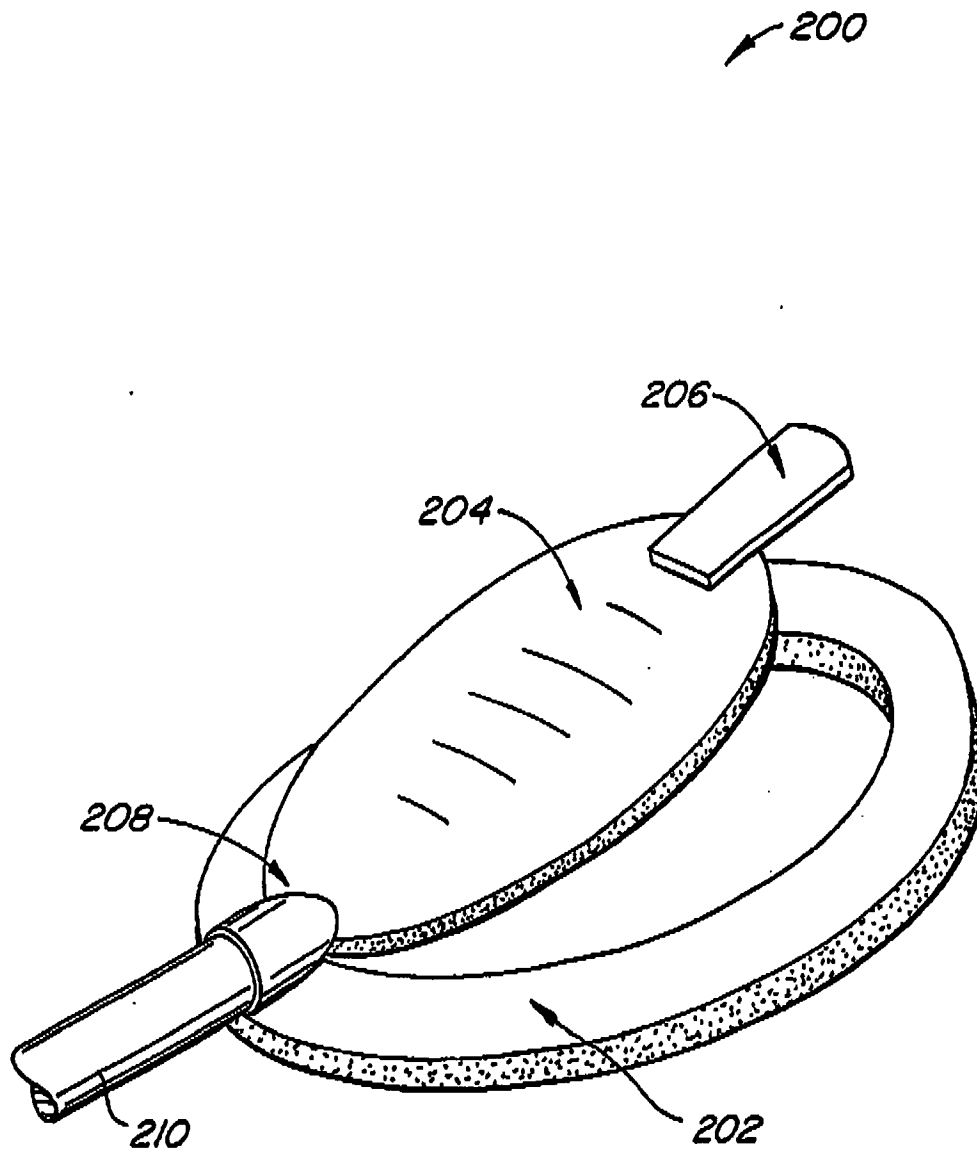

**FIG. 5**

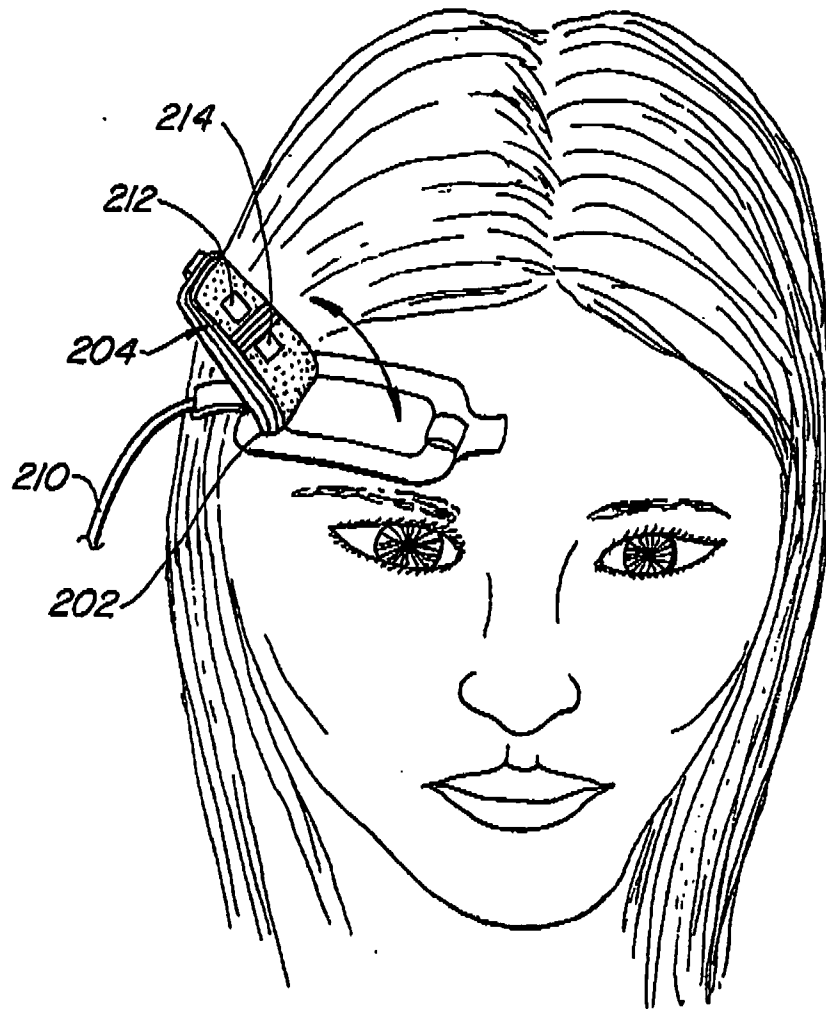

**FIG. 6**

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 32892401 P [0001]
- US 5782237 A [0020]
- US 5830136 A [0032]

专利名称(译)	堆叠式粘合剂光学传感器		
公开(公告)号	<a href="#">EP2294973A2</a>	公开(公告)日	2011-03-16
申请号	EP2010010532	申请日	2002-10-10
[标]申请(专利权)人(译)	内尔科尔普里坦贝内特公司		
申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
当前申请(专利权)人(译)	NELLCOR PURITAN BENNETT LLC		
[标]发明人	HANNULA DON COAKLEY JOSEPH MANNHEIMER PAUL D ONEIL MICHAEL PATRICK CHIN RODNEY ADNAN MERCHANT		
发明人	HANNULA, DON COAKLEY, JOSEPH MANNHEIMER, PAUL D. O'NEIL, MICHAEL PATRICK CHIN, RODNEY ADNAN, MERCHANT		
IPC分类号	A61B5/00 G01N21/17 A61B5/024 A61B5/026 A61B5/145 A61B5/1455 G01N21/31 G01N21/47		
CPC分类号	A61B5/68335 A61B5/0205 A61B5/02427 A61B5/14551 A61B5/14552 A61B5/6814 A61B5/6819 A61B5/6826 A61B5/6829 A61B5/6833 A61B5/6838 A61B5/6841 A61B2562/0233 A61B2562/043 A61B2562/146 A61B2562/164 G01N21/49 G01N2021/3144 Y10T29/49826		
优先权	60/328924 2001-10-12 US		
其他公开文献	EP2294973A3		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

一种传感器，包括：传感器主体；发射器和检测器耦合到传感器主体，其中传感器主体被配置为当传感器应用于患者时将发射器和检测器相对于彼此保持在基本固定的距离。

