

(19)



(11)

EP 3 011 900 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
27.04.2016 Bulletin 2016/17

(51) Int Cl.:
A61B 5/0408 (2006.01) A61B 5/00 (2006.01)

(21) Application number: **14190353.4**

(22) Date of filing: **24.10.2014**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(71) Applicant: **Quickels Systems AB**
114 19 Stockholm (SE)

(72) Inventors:
• **Sjöberg, Krister**
113 61 STOCKHOLM (SE)
• **Sjöberg, Göran**
196 30 STOCKHOLM (SE)

(74) Representative: **Platt, Timothy Nathaniel**
IPQ IP Specialists AB
Docketing
PO Box 42
683 21 Hagfors (SE)

(54) **Electrode module, suction system and tool for biopotential monitoring**

(57) A vacuum hose ECG electrode module has a disposable vacuum electrode unit (5), which can be snapped into a re-usable electrode module housing (2). The disposable electrode unit (5) has a more rigid vacuum chamber dish (7) and a pliable skin-contacting lip ring (8) permanently fixed to the rim of said dish (7).

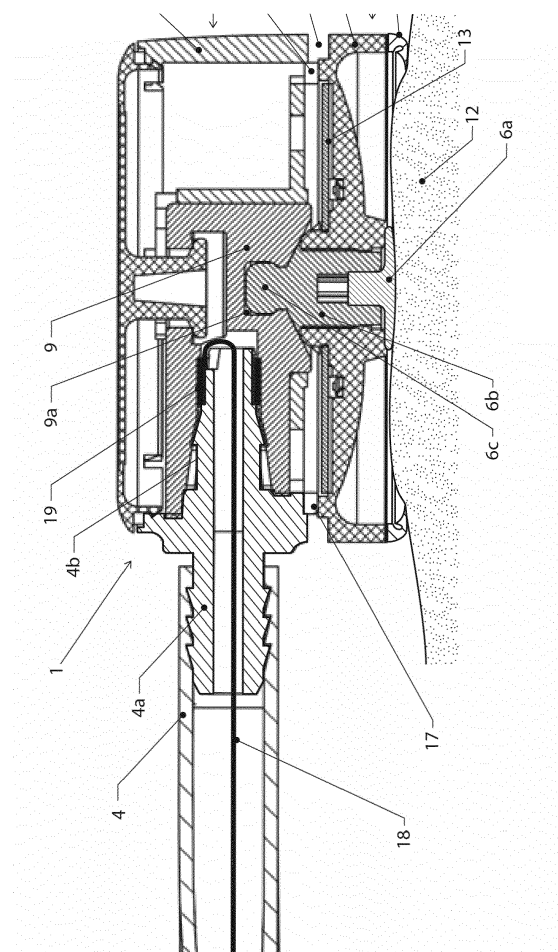


Fig. 1

EP 3 011 900 A1

Description

BACKGROUND

[0001] The present invention relates in general to electrode modules for biopotential monitoring, and in particular electrocardiogram (ECG) monitoring of the heart's electrical activity through the skin at various points on the torso, ankles and wrists.

RELATED ART

[0002] US 8 406 843 describes a disposable stick-on ECG monitoring electrode which does not use vacuum suction. It proposes a way to deal with problems which it describes in the fourth paragraph of column 1: "The strength and accuracy of the signals from the ECG electrodes to the monitor is dependent on motion artifacts caused by the movement of the patient's skin relative to the electrode. This movement can cause extraneous signals, shifting the desired signal baseline. Abrading the skin reduces the electrical potential and minimizes the impedance of the patient's skin, thereby reducing motions artifacts and improving the biopotential electrical signal. Typically, the patient's skin is prepared prior to applying the electrode. Preparatory abrasion removes a portion of the epidermis or external skin layer and is usually performed by rubbing the patient's skin with a rough surfaced material followed by cleaning the abraded area with alcohol. If the electrical potential of one or more electrodes is too great and the signal is not adequate, the electrode(s) must be removed, the site further abraded, and the electrodes (s) reapplied. This procedure is not only time consuming, but may be painful to the patient. The processes may also cause emotional distress to the patient as the patient views the skin abrading procedure. The proposed solution according to this prior art document US 8 406 843 is that the disposable electrode have an abrasive surface, used to sand off and prep the skin of the patient by twisting the electrode back and forth. The abrasive electrode can also be infused with gel which will spread over the abraded skin and decrease the impedance between the skin and the electrode surface. The proposed prior art solution also includes using adhesive patch to keep the electrode in place. Any procedure which requires abrasion of multiple skin locations and the use of gel and adhesive is naturally not optimal.

[0003] In addition to stick-on disposable electrodes, various suction modules are known in the art which are connected via suction hoses to a central vacuum unit and a recording and analysis unit for the electrical signals. Suction electrodes have the advantage of being easy to apply and remove and do not require abrasion of the skin or the use of adhesives.

[0004] One presently known suction cup module is described in WO 2011 /046490 having a housing which can be coupled to a hose for transmitting vacuum and electrical signals. A disposable electrode disc or cup has a

central metal electrode, which has a flat skin-contacting surface and a knob for attachment to/detachment from a block in the module, and is surrounded by a plastic disc portion with a flexible skirt to create a vacuum chamber and seal against the skin of the patient.

[0005] However, none of the related art discloses or hints at how to achieve the solutions provided by the present invention.

10 OBJECT OF THE INVENTION

[0006] A complex of difficult-to-reconcile interrelated problems has up to now not been successfully addressed by the prior art devices.

1. Hygiene: Medical protocols increasingly require sterilization or disposal of electrodes before an ECG unit is used for a new patient. Sterilization is time-consuming and thus expensive and there is a temptation for medical personnel to skip this step under pressure to perform many ECGs during a work session. Replacing entire sets of vacuum electrode modules for every new patient is prohibitively expensive. The disposable electrodes should be removable and safely discardable without the medical personnel ever touching any part of the used electrode. It is also hygienically problematic to replace, on suction units, HEPA (*high-efficiency particulate air*) filter which trap virus and bacteria, which should, ideally, be trapped as close to the patient as possible to avoid contamination of non-disposable parts of the suction unit.

2. ECG units without vacuum suction require the use of gels, adhesives as well as skin-prepping abrasion to make the disposable electrodes stick to the skin during measurement.

3. Vacuum suction ECG units are preferred by many cardiology professionals for ease of attachment and detachment and because no gel, adhesives or abrasion is needed. Only an electrolyte spray is used.

4. ECG "stress tests", of crucial importance in cardiology, usually involving cycling on an exercise bike or running on a treadmill, present significant problems because the hoses or leads can pull on the electrodes and cause them to become detached or give rise to "motion artifacts" in the ECG reading, i. e. measurement anomalies clouding the medical analysis.

5. Hair or uneven skin can break the vacuum holding the electrode in place. A disposable disc or cup made very pliable to always seal over hair or uneven skin will be susceptible to motion artifacts during ECG stress tests as the hoses unavoidably pull on the electrode modules.

SUMMARY

[0007] Disturbances giving rise to "motion artifacts" in

the ECG readings are explainable with reference to the Helmholtz double layer model where in an electrolyte such as skin moisture or a gel, two layers of opposite polarity are formed at the interface between the electrode surface and the electrolyte. Any tipping of this double layer, for example by uneven lateral forces on the electrode module when pulling on the hose, will cause a change in the capacitance and the chemical equilibrium of ions making up the Helmholtz double layer and distort the reading of the true electrical activity of the heart.

[0008] The entire complex of problems listed above finds its solution in the invention as defined in the appended main patent claim.

BRIEF DESCRIPTION OF DRAWINGS

[0009] Embodiments of the invention will now be described in more detail with reference to the appended drawings, wherein:

Fig. 1 shows a vacuum electrode module according to the present invention in cross section.

Fig. 2 shows the same vacuum electrode module as in Fig. 1 adhering to an uneven area of skin.

Fig. 3 illustrates the effect of pulling on the hose attached to the vacuum electrode module.

Figs. 4(a)-(c) shows different views of the entire vacuum electrode module.

Figs. 5(a)-(c) show an exploded view and two cross sectional views of a disposable electrode unit.

Figs. 6-8 show the detacher tool and its use.

DETAILED DESCRIPTION

[0010] With reference to Fig. 1 a vacuum electrode module 1 is shown for use in a suction system together with an ECG monitor. Usually up to ten such vacuum electrode modules are coupled to the same suction system for ECG monitoring, each via an individual electrically conducting vacuum hose 4, which is slipped over the outer part of the nipple 4a. The nipple is part of the peripheral plastic shell 18. The inner nipple 4b is forced into the central conductive polymer block 9 in the vacuum electrode module housing 2. A disposable electrode unit 5 has a central electrode sensor element 6a-c, comprising a skin-contacting biopotential transducer sensor 6a and a snap connector 6b with a knob 6c which is snapped into a socket 9a in the electrically conducting block 9. An electrical signal conducting wire 18 within the hose 4 is connected to a contact ring 19 which is in electrical contact with the conductive polymer block 9.

[0011] When mounted, there is a peripheral groove 16 between the module housing 2 and the disposable elec-

trode unit 5. The sealing rim 17 retains the vacuum within the electrode module housing 2 and the disposable electrode unit 5. Surrounding said electrode sensor element 6a-c is a vacuum chamber dish 7 which is made of relatively rigid plastic, in this embodiment of injection molded polypropylene thermosetting resin. Extending from the periphery of said vacuum chamber dish 7 is a circumferential lip 8 of a flexible and resilient plastic or rubber, in this embodiment of thermoplastic elastomer which has been injection molded to be permanently attached to the dish 7, which is still warm when the thermoplastic lip is molded thereto.

[0012] This construction prevents tugging on the hose 4 and/or unevenness in the skin area from causing the chemical equilibrium of the double layer interface where the electrode sensor element meets the skin surface, to be disturbed, giving rise to motion artifacts in the ECG monitoring record.

[0013] Fig. 2 shows such a situation where the skin area is uneven. The lip 8a on one side is fully compressed by the skin and the force generated by the vacuum, whereas the lip 8b on its other side is only very slightly compressed where it meets the skin, preserving the vacuum suction all around, without ever disturbing the chemical equilibrium interface where the electrode sensor element meets the skin. Also clearly visible is the peripheral groove 16 between the module housing 2 and the disposable electrode 5, the importance of which will be described below with reference to Figs. 6, 7 and 8. The lip 8 also has an interior groove 8c which facilitates folding of the lip as can be seen at 8c in Fig. 2.

[0014] Fig. 3 shows a typical situation where, during an exercise cycle or treadmill running stress test, the vacuum hose 4 is tugged in the direction of the arrow A. By virtue of the reinforced rigidity of the vacuum chamber dish 7 together with the electrode module housing 2, the force, propagated by this pulling, at the interface between the skin-contacting electrode sensor element 6a, will be lateral in the direction of the arrow B, pulling the skin laterally, without any change in the Helmholtz double layer at said interface.

[0015] The novel construction of the disposable electrode disc unit 5 with a stabilizing more rigid portion (the vacuum chamber dish 7) and a softer, flexible and resilient lip portion 8 prevents any tipping of the biopotential transducer sensor 6a in relation to the skin 12 and at the same time ensures a complete and reliable vacuum seal around the vacuum chamber. The forces transmitted via the hose being pulled will act coplanar to the interface between the electrode surface 6a and the skin 12. If both the vacuum chamber dish 7 and the circumferential lip 8 were made in one piece of the same flexible pliable material, pulling on the vacuum hose 4 would cause the entire module to tip changing the contact between the biopotential transducer sensor 6a and the skin 12 and giving rise to motion artifacts. If, on the other hand, both the vacuum chamber dish 7 and the pliable circumferential lip 8 were made in the same more rigid material the

vacuum seal risks being broken due to movement or due to hair or uneven skin, which will also distort the ECG measurements or even lead to the electrode module falling off.

[0016] Fig. 4 (a)-(c) shows the entire coupled vacuum electrode module in three views: (a) a perspective view from above, (b) with the disposable electrode unit 2 detached from the vacuum electrode module housing 2 and (c) a view from below of the coupled module showing the vacuum chamber dish 7 with stabilizing and reinforcing ribs 15 and vacuum holes 14 to transmit suction from the hose 4. In another embodiment said ribs have been replaced by vacuum distribution channels.

[0017] Fig. 5(a)-(c) showing the disposable electrode unit by itself in three views: (a) an exploded view showing the skin-contacting biopotential transducer sensor 6a of the electrode sensor element, the electrically conducting snap connector 6b with knob 6c. On top of the vacuum chamber dish 7 is, in this embodiment, a HEPA filter which will trap almost all particles, which can carry virus and bacteria. Fig. 5(b) shows a cross-section bisecting the reinforcing and stabilizing ribs 15. Fig. 5(c) shows a cross-section along a plane perpendicular thereto.

[0018] Figs. 6, 7 and 8 show the use of a specifically designed detacher tool 20 for separating the disposable electrode unit 5 from the vacuum electrode module housing 2 and disposal of the used electrode unit 5 without the medical personnel ever having to touch the used electrode unit 5. Fig. 6 shows the detacher tool 20 which has two rails 21 spaced the width of the disposable electrode unit. As can be seen in Figs. 7 and 8, the rails 21 each have a ridge 23 extending inwardly the depth of the groove 16 between the module 2 and the disposable electrode 5. To detach the used disposable electrode unit from the module housing 2, the medical worker, pushes the vacuum hose 4 and the module housing 2 between the rails in the direction of the arrow C in Fig. 7. The ridges increase in thickness gradually from the entrance in the direction of the arrow C. The ridges act as ramps to pry the disposable electrode unit 5 from the module housing 2 without having to touch it, and when it detaches it will fall through the hole 22 and into a medical waste container onto which the detacher tool is mounted via a bracket 24.

Claims

1. Electrode module of vacuum suction type, suitable for biopotential monitoring, for example for use with an electrocardiographic monitor, comprising: a. a vacuum electrode module housing (2) with connector means (4a) suitable for receiving a hose (4) conducting vacuum and electrical signals, b. a replaceable electrode unit (5) having a central electrode sensor element (6) coaxial to a surrounding vacuum chamber dish (7), **characterized in that** from the periphery of said vacuum chamber dish (7) there ex-

tends a circumferential skin-contact lip (8) of substantially more pliable material than the material of said vacuum chamber dish (7).

2. Electrode module according to Claim 1, **characterized in that** said vacuum chamber dish (7) is made of polypropylene (PP) and said circumferential skin-contact lip (8) is made of thermoplastic elastomer (TPE).
3. Electrode module according to Claim 2, **characterized in that** said lip (8) is made of TPE having a hardness of between 30 and 60 ShoreA.
4. Electrode module according to one of the preceding claims, **characterized in that** said circumferential lip (8) is provided with an interior groove (8c).
5. Electrode module according to one of the preceding claims, **characterized in that** said replaceable electrode unit comprises a porous air filter disc 13.
6. Electrode module according to Claim 5, **characterized in that** said porous air filter disc 13 is sealed to the vacuum chamber dish (7) at its central hole (13a) and at its periphery (13b, 17).
7. Electrode module according to one of the preceding claims, **characterized in that** said module housing (2) includes a block (9) of electrically conductive polymeric material, with a nipple 4a for receiving a hose (4) and a central electrode (6a-c).
8. Suction system for use in conjunction with an apparatus for biopotential monitoring, comprising a plurality of electrode modules according to one of claims 1-7, and for each electrode module an individual hose, containing a conducting wire for biopotential signals, each hose leading to a vacuum generating unit.
9. Tool suitable for use with an electrode module as defined in one of Claims 1-7, for detaching said interchangeable electrode unit (5) from said module housing (2), **characterized in that** said tool comprises two parallel rails (21) spaced the diameter of the vacuum chamber dish (7), an entrance opening for said electrode module into the space between the two rails (21), from which two ridges (23) extend the depth of a circumferential groove (16) formed between the module housing (2) and the electrode unit (5), wherein said ridges (23) have a thickness which increases gradually from a thickness, at said entrance opening, less than the height of said circumferential groove, to a thickness greater than the height of said groove.
10. Tool according to Claim 9, **characterized in that**

said tool has a mounting bracket (24) suitable for mounting said tool above a medical waste container and wherein said tool has a disposal hole (22) between said rails and disposed remote from said entrance opening for receiving a disposable electrode unit (5) as it is detached from its module housing (2).

10

15

20

25

30

35

40

45

50

55

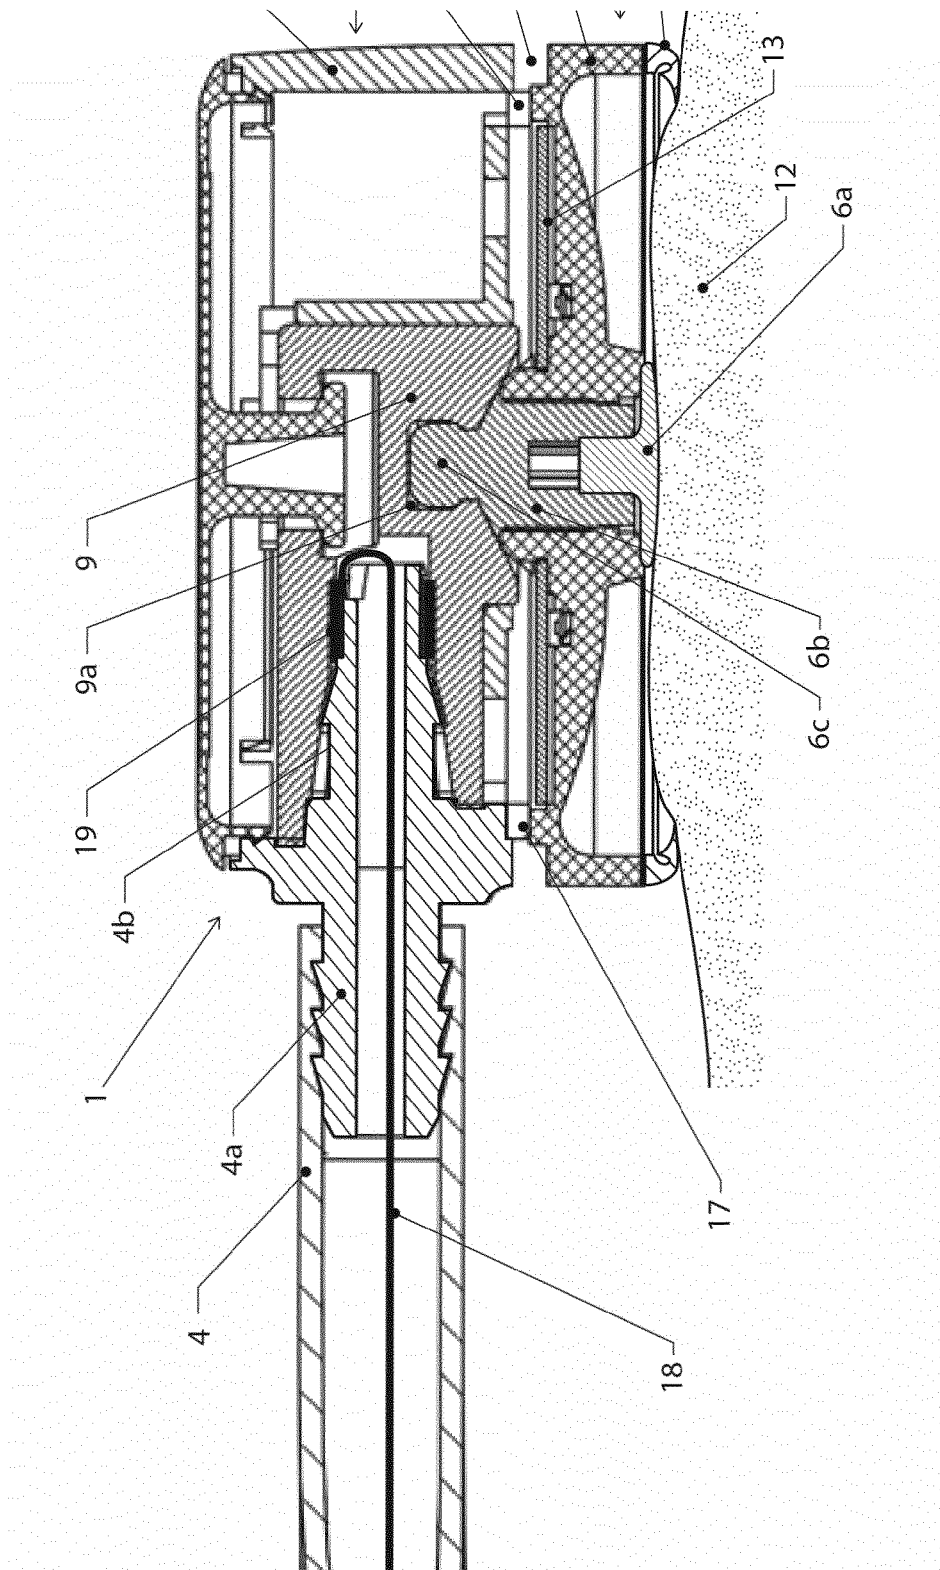


Fig. 1

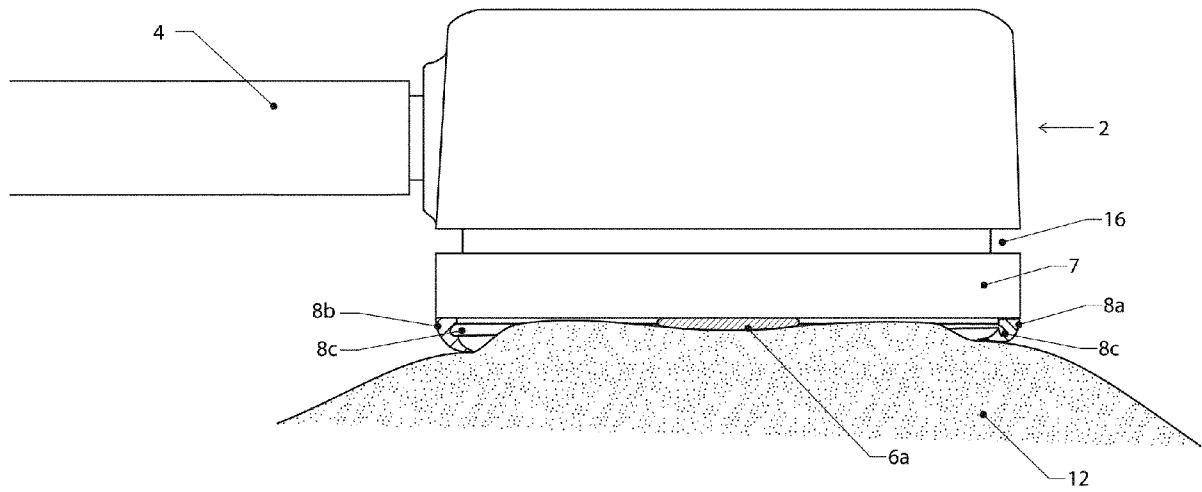


Fig. 2

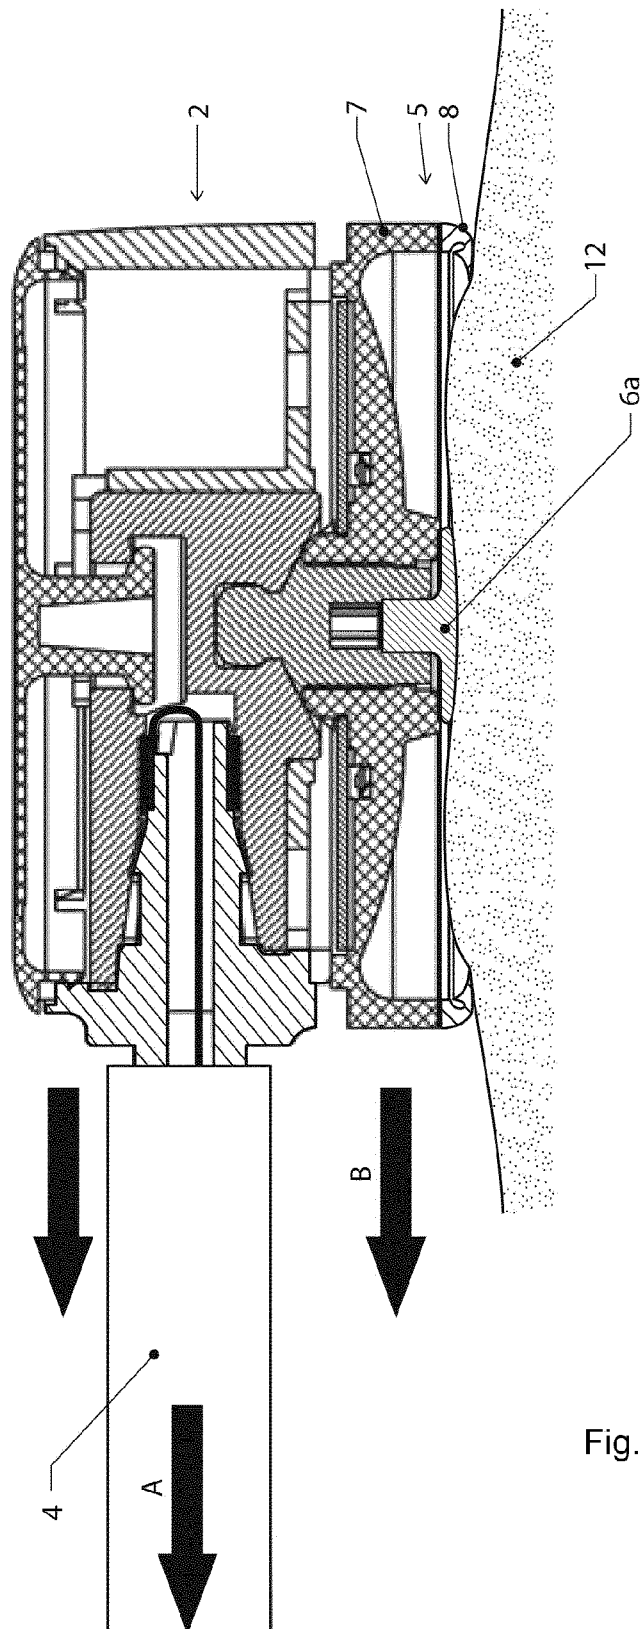


Fig. 3

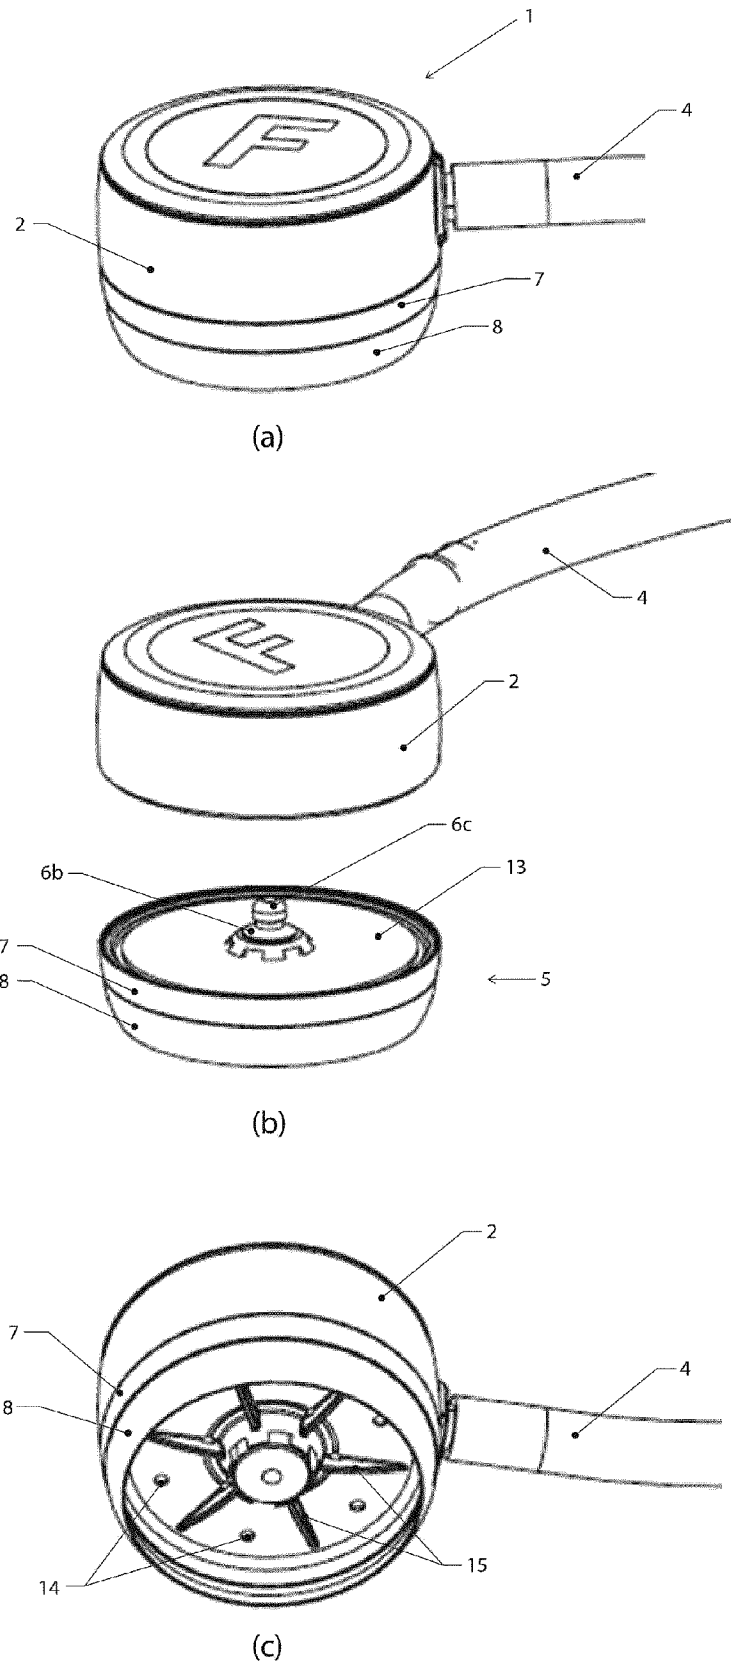


Fig. 4 (a-c)

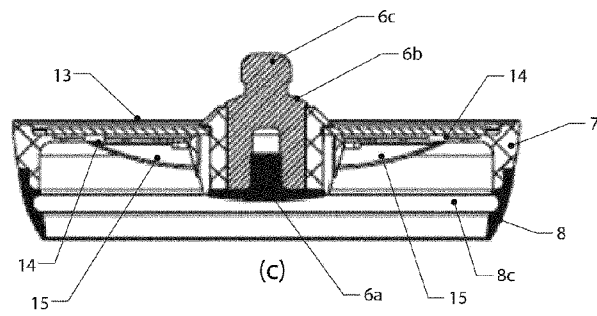
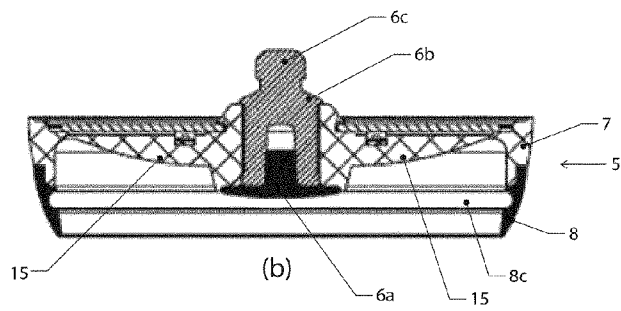
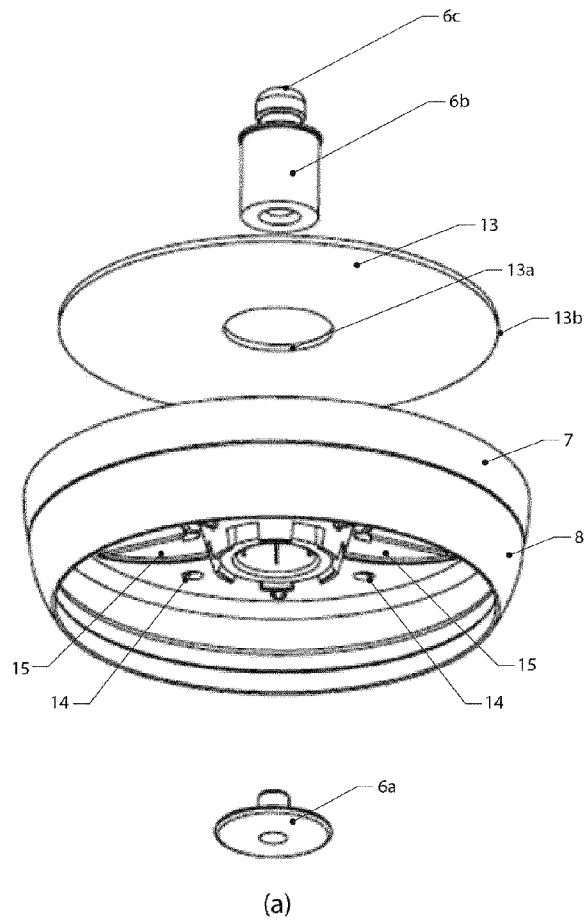


Fig. 5 (a-c)

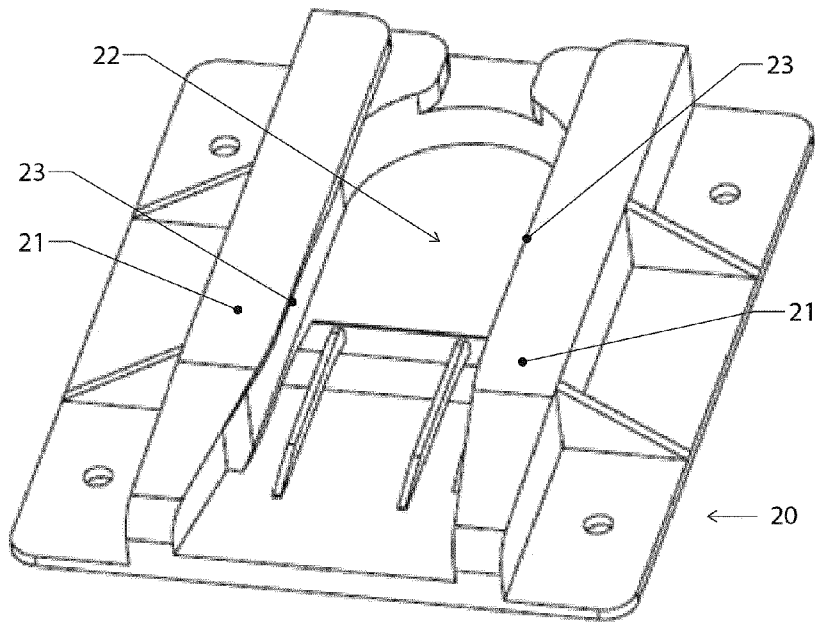


Fig. 6

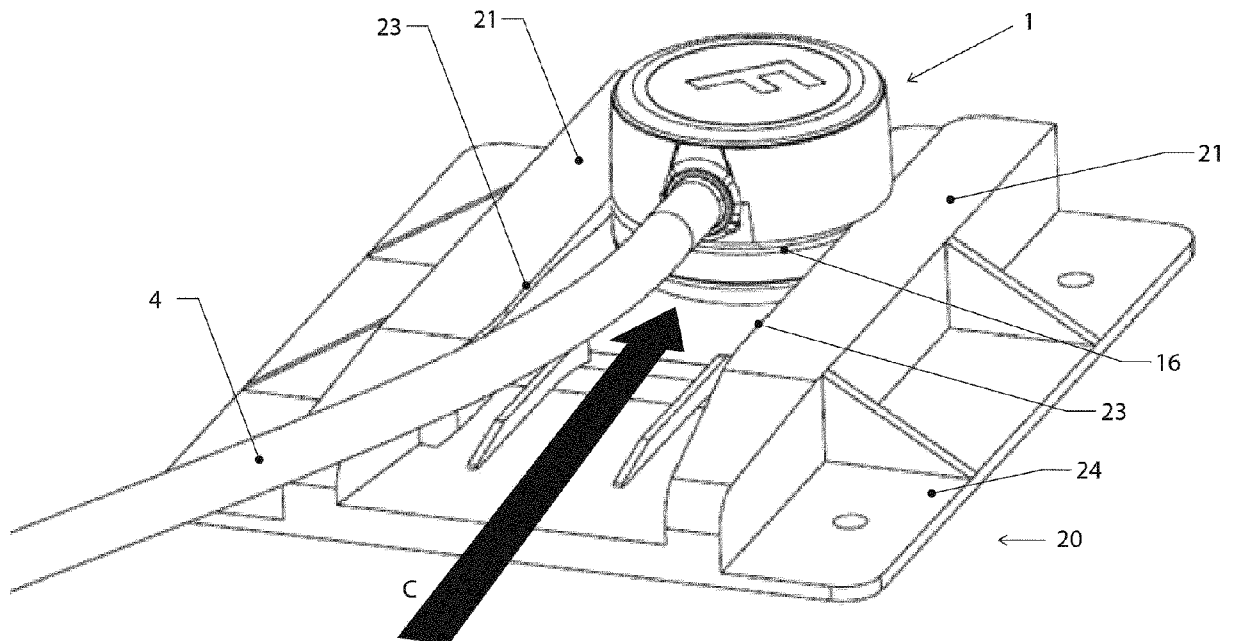


Fig. 7

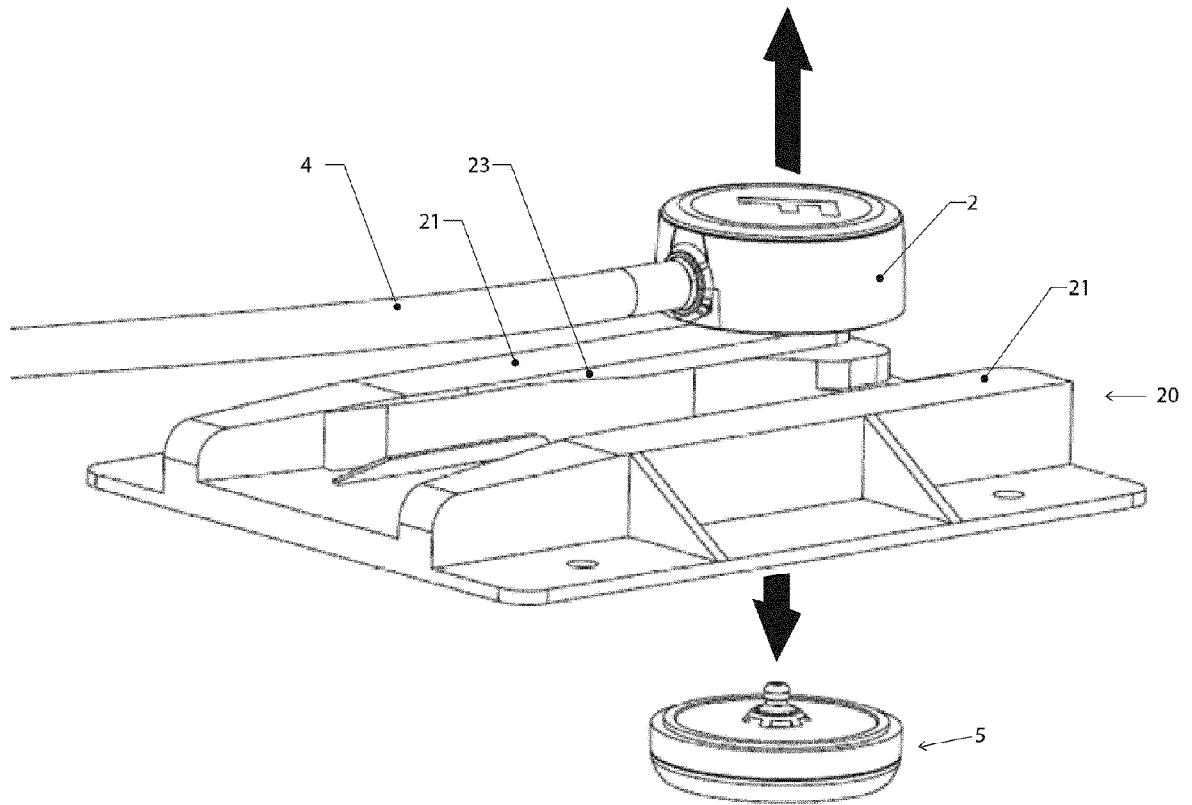


Fig. 8



EUROPEAN SEARCH REPORT

Application Number
EP 14 19 0353

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	WO 95/21568 A1 (HUMANTEKNIK AB [SE]; LUNDBAECK STIG [SE]) 17 August 1995 (1995-08-17) * abstract; claim 1; figures 1,2,5, 5A * * page 3, line 27 - line 36 * * page 4, line 15 - page 5, line 12 * * the whole document *	1-8	INV. A61B5/0408 A61B5/00
X	US 2005/139040 A1 (CRUDGINGTON CLEVELAND B JR [US] CRUDGINGTON JR CLEVELAND BENED [US]) 30 June 2005 (2005-06-30) * figures 5-7, 10-11 * * paragraphs [0033] - [0036] *	9,10	
A	US 5 732 700 A (LUNDBAECK STIG [SE]) 31 March 1998 (1998-03-31) * abstract; figures 1-9 * * column 7, line 1 - line 2 * * the whole document *	1-8	
A,D	WO 2011/046490 A1 (QUICKELS SYSTEMS AB [SE]; AABERG JERKER [SE]) 21 April 2011 (2011-04-21) * the whole document * * figure 1 *	1-8	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	WO 2005/053530 A1 (DEEPBREEZE LTD [IL]; KUSHNIR IGAL [IL]; BOTBOL MEIR [IL]) 16 June 2005 (2005-06-16) * page 7, line 7 - line 17 *	1-3	
A	EP 0 143 761 A1 (ASTRA TECH AB [SE]) 5 June 1985 (1985-06-05) * page 4, line 11 - line 15; claim 1 * * the whole document *	1-8	
A	US 2008/083301 A1 (MESSINA SHARON C [US]) 10 April 2008 (2008-04-10) * figure 1 *	9,10	
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 8 April 2015	Examiner Furlan, Stéphane
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03/82 (P04C01)



Application Number

EP 14 19 0353

CLAIMS INCURRING FEES

The present European patent application comprised at the time of filing claims for which payment was due.

☐ Only part of the claims have been paid within the prescribed time limit. The present European search report has been drawn up for those claims for which no payment was due and for those claims for which claims fees have been paid, namely claim(s):

☐ No claims fees have been paid within the prescribed time limit. The present European search report has been drawn up for those claims for which no payment was due.

LACK OF UNITY OF INVENTION

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

see sheet B

☒ All further search fees have been paid within the fixed time limit. The present European search report has been drawn up for all claims.

☐ As all searchable claims could be searched without effort justifying an additional fee, the Search Division did not invite payment of any additional fee.

☐ Only part of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the inventions in respect of which search fees have been paid, namely claims:

☐ None of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims, namely claims:

☐ The present supplementary European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims (Rule 164 (1) EPC).



**LACK OF UNITY OF INVENTION
SHEET B**

Application Number
EP 14 19 0353

5

10

15

20

25

30

35

40

45

50

55

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

1. claims: 1-8

Electrode module of vacuum suction type

2. claims: 9, 10

Detacher tool

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 14 19 0353

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

08-04-2015

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9521568 A1	17-08-1995	AU 1828295 A	29-08-1995
		CA 2182944 A1	17-08-1995
		CN 1140401 A	15-01-1997
		DE 69533219 D1	05-08-2004
		DE 69533219 T2	07-07-2005
		EP 0744911 A1	04-12-1996
		JP 3434299 B2	04-08-2003
		JP H09508830 A	09-09-1997
		US 5722404 A	03-03-1998
		WO 9521568 A1	17-08-1995

US 2005139040 A1	30-06-2005	NONE	

US 5732700 A	31-03-1998	AT 185956 T	15-11-1999
		AU 680814 B2	14-08-1997
		BR 9305925 A	26-08-1997
		CA 2129360 A1	21-08-1993
		CZ 9401993 A3	18-01-1995
		DE 69326884 D1	02-12-1999
		DE 69326884 T2	28-12-2000
		DK 0626820 T3	25-04-2000
		EP 0626820 A1	07-12-1994
		ES 2140451 T3	01-03-2000
		JP 3329459 B2	30-09-2002
		JP H07503874 A	27-04-1995
		TW 239071 B	21-01-1995
		US 5553612 A	10-09-1996
		US 5732699 A	31-03-1998
		US 5732700 A	31-03-1998
		US 5842985 A	01-12-1998
		WO 9316633 A1	02-09-1993

WO 2011046490 A1	21-04-2011	SE 0901333 A1	17-04-2011
		WO 2011046490 A1	21-04-2011

WO 2005053530 A1	16-06-2005	NONE	

EP 0143761 A1	05-06-1985	AU 574397 B2	07-07-1988
		AU 3466684 A	02-05-1985
		BR 8405422 A	03-09-1985
		CA 1258694 A1	22-08-1989
		CS 274755 B2	15-10-1991
		DD 228170 A5	09-10-1985
		DE 3438788 A1	09-05-1985
		DE 3469847 D1	21-04-1988
		DK 504484 A	29-04-1985

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 14 19 0353

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

08-04-2015

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 0143761 A1	05-06-1985
		ES 8602386 A1	16-03-1986
		FI 844193 A	29-04-1985
		GB 2148719 A	05-06-1985
		GB 2160107 A	18-12-1985
		GR 80751 A1	22-02-1985
		HU 189435 B	28-07-1986
		IE 55695 B1	19-12-1990
		IL 73297 A	12-07-1990
		IN 162242 A1	23-04-1988
		JP H0472539 B2	18-11-1992
		JP S60111632 A	18-06-1985
		MX 157470 A	23-11-1988
		NO 844221 A	29-04-1985
		NZ 209986 A	30-08-1988
		PH 21743 A	10-02-1988
		PL 250211 A1	27-08-1985
		PT 79422 A	01-11-1984
		RO 90230 A	30-09-1986
		SE 454941 B	13-06-1988
		SU 1475475 A3	23-04-1989
		US 4646747 A	03-03-1987
		YU 181184 A	31-12-1986
		ZA 8408269 A	26-06-1985

US 2008083301	A1	10-04-2008	NONE

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 8406843 B [0002]
- WO 2011046490 A [0004]

专利名称(译)	电极模块，抽吸系统和用于生物电位监测的工具		
公开(公告)号	EP3011900A1	公开(公告)日	2016-04-27
申请号	EP2014190353	申请日	2014-10-24
[标]申请(专利权)人(译)	QUICKELS SYST		
申请(专利权)人(译)	QUICKELS系统公司		
当前申请(专利权)人(译)	QUICKELS系统公司		
[标]发明人	SJOBERG KRISTER SJOBERG GORAN		
发明人	SJÖBERG, KRISTER SJÖBERG, GÖRAN		
IPC分类号	A61B5/0408 A61B5/00		
CPC分类号	A61B5/04082 A61B5/6834		
审查员(译)	他stÉphane		
外部链接	Espacenet		

摘要(译)

真空软管ECG电极模块具有一性真空电极单元 (5)，其可以卡入可重复使用的电极模块壳体 (2) 中。一性电极单元 (5) 具有更刚性的真空室盘 (7) 和柔韧的皮肤接触唇环 (8)，其永久地固定到所述盘 (7) 的边缘。

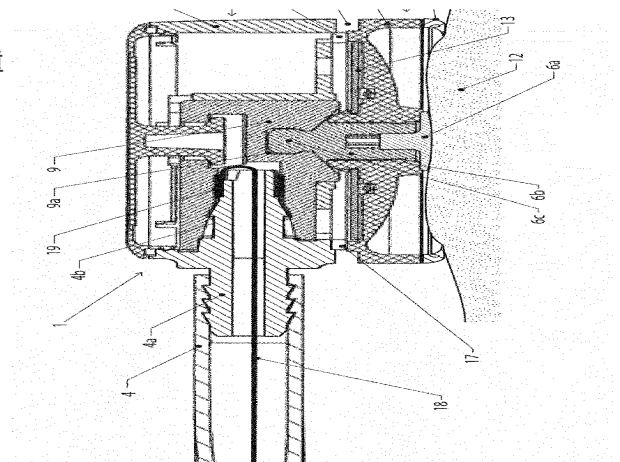


Fig. 1