

(19)



(11)

EP 3 457 934 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

25.12.2019 Bulletin 2019/52

(51) Int Cl.:

A61B 5/05 (2006.01)

A61B 5/00 (2006.01)

(86) International application number:

PCT/GB2017/051380

(21) Application number: **17725735.9**

(22) Date of filing: **17.05.2017**

(87) International publication number:

WO 2017/199029 (23.11.2017 Gazette 2017/47)

(54) **A MEDICAL IMAGING SYSTEM AND METHOD**

SYSTEM UND VERFAHREN ZUR MEDIZINISCHEN BILDGEBUNG

SYSTÈME ET PROCÉDÉ D'IMAGERIE MÉDICALE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **17.05.2016 GB 201608687**

(43) Date of publication of application:

27.03.2019 Bulletin 2019/13

(73) Proprietor: **Micrima Limited**

Bristol BS2 0EL (GB)

(72) Inventors:

- **BANNISTER, Peter Romilly**
Bristol BS2 0EL (GB)

- **THOMAS, Kevin Leslie**
Bristol BS2 0EL (GB)

(74) Representative: **Haseltine Lake Kempner LLP**

Redcliff Quay
120 Redcliff Street
Bristol BS1 6HU (GB)

(56) References cited:

WO-A2-98/38919 WO-A2-2014/149183
DE-A1-102009 007 255 RU-C1- 2 578 298
US-A1- 2006 058 606

EP 3 457 934 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The invention relates to a medical imaging system and method.

[0002] Breast cancer is the most common cancer in women. X-ray mammography is currently the most effective detection technique and is used for screening, however it suffers from relatively high missed- and false-detection rates, involves uncomfortable compression of the breast and also entails exposure to ionizing radiation.

[0003] Microwave imaging and detection of breast tumours is a potential non-ionising alternative. One such approach is to employ a densely packed conformal antenna array, which also stabilises the breast position with a minimum of coupling fluid.

[0004] WO 2014/149183, RU 2578298, DE 102009007255 and WO98/38919 describe a number of medical imaging systems that are known in the art.

[0005] The invention seeks to provide additional functionality to a microwave imaging system.

[0006] The invention is defined in the attached independent claims to which reference should now be made. Further, optional features may be found in the sub-claims appended thereto.

[0007] In accordance with an aspect of the invention, there is provided a medical imaging system comprising: a microwave antenna array comprising a transmitting antenna and a plurality of receiving antennae, wherein the transmitting antenna is configured to transmit microwave signals and the receiving antennae are configured to receive the microwave signals following scattering; a marker configured to scatter the microwave signals; and a processor configured to process the scattered microwave signals and generate an image of the marker.

[0008] The marker may be a passive antenna having a resonant slot.

[0009] The marker may be formed of a metal foil which conforms to the shape of the body part.

[0010] The marker may be a non-linear antenna which scatters the microwave signal at a frequency which is different to the frequency of the received microwave signal.

[0011] The non-linear antenna may be a harmonic antenna.

[0012] The marker may comprise a contrast agent.

[0013] The transmitting antenna may be configured to transmit microwave signals so as to illuminate a body part of a patient and the receiving antennae may be configured to receive the microwave signals following scattering within the body part. The marker may be configured to overlie the surface of the skin of the body part. The processor may be configured to process the scattered microwave signals and generate an image of the internal structure of the body part and the marker so as to identify a region of interest within the body part relative to the position of the marker.

[0014] The processor may be configured to calibrate the medical imaging system based on the marker. The

processor may be configured to calibrate the medical imaging system based on the scattering characteristics of the marker. For example, based on a known reference scattering response from the marker it may be possible to calibrate or adjust the measured scattering from the body part. The scattering characteristics could be brightness, intensity, spectrum (e.g. colour), and directionality.

[0015] The marker may be configured to be applied to the surface of the skin. The marker may be provided with an adhesive for adhering the marker to the surface of the skin. The marker may be provided with a backing material, such as a non-porous layer. This may prevent skin moisture from affecting the dielectric properties of the marker.

[0016] The marker may be attached to a component which is arranged to be fixed in position. The component may comprise a cup or insert, for example. The marker could be adhered to or otherwise attached to the component. For example, it could be embedded within the component. The component may be configured to be in contact with at least a portion of a body part. The component may be configured to receive at least a portion of a body part.

[0017] In accordance with another aspect there is provided a medical imaging method comprising: providing a marker w; illuminating the marker with microwave signals emitted by a transmitting antenna of a microwave antenna array; receiving the microwave signals following scattering by the marker at a plurality of receiving antennae of the microwave antenna array; processing the scattered microwave signals to generate an image of the marker.

[0018] The method may further comprise performing image registration between a plurality of images by correlating the position of the marker in each image.

[0019] The images may be produced using different imaging modalities.

[0020] The method may further comprise adjusting the spatial image reconstruction to correct for spatial distortion by comparing the position of the marker within the image with its known reference position.

[0021] The method may further comprise adjusting reconstruction parameters based on a known reference position of the marker.

[0022] The marker may be provided such that it overlies the surface of the skin of a body part of a patient. The marker and the body part may be illuminated with microwave signals, Microwave signals may be received following scattering within the body part and by the marker. The scattered microwave signals may be processed to generate an image of the body part showing an internal structure of the body part and the marker so as to identify a region of interest within the body part relative to the position of the marker.

[0023] The images may be taken at different instances by reapplying the marker to the same position on the skin.

[0024] The method may further comprise using the known scattering characteristics of the marker as a ref-

erence to adjust the measured scattering from the body part.

[0025] The marker may be affixed to the surface of the skin. The marker may be adhered to the surface of the skin.

[0026] The method may further comprise calibrating a medical imaging system based on the marker. The method may further comprise calibrating the medical imaging system based on the scattering characteristics of the marker.

[0027] The marker may be attached to a component which is fixed in position. The component may comprise a cup. At least a portion of the body part may be received within the cup.

[0028] For a better understanding of the invention, and to show more clearly how it may be carried into effect, reference will now be made, by way of example, to the accompanying drawings, in which:-

Figure 1 is a schematic view of a medical imaging system;

Figure 2 is a front view of a marker for use with the medical imaging system;

Figure 3 is a front view of the marker affixed to a model of a breast;

Figure 4 shows image plots from various directions for the model of the breast; and

Figure 5 is a schematic view of another example of a marker.

[0029] Figure 1 shows a medical imaging system 2 which comprises a microwave antenna array 6. The antenna array 6 comprises a plurality N of antennae 16 which are arranged over the surface of, or within, a shell substrate 18. The shell 18 has a curved profile as shown. In particular, the shell 18 is part or hemi-spherical and is configured to approximate the shape of a breast. The antennae 16 are arranged over the shell 18 such that they all point to a common focal point.

[0030] The antennae 16 are each electrically connected to a switching matrix 20. The switching matrix 20 is in turn connected to both a transmit path and a receive path. The transmit path comprises a signal generator 22 coupled to an amplifier 24. The receive path comprises an amplifier 26 coupled to a detector 28 and a processor 4.

[0031] The switching matrix 20 selectively couples each of the antennae 16 to either the transmit path or the receive path.

[0032] The antenna array 6 is operated in a multi-static fashion. Specifically, the switching matrix 20 is controlled so as to connect one of the antennae 16 to the transmit path and the remaining antennae 16 to the receive path. The signal generator 22 generates a stepped frequency continuous wave (CW), Ultra Wide-Band (UWB) signal

which is amplified by the amplifier 24 and then transmitted by the antenna 16 connected to the transmit path. The stepped frequency continuous wave signal is a sequential series of pulses of continuous wave energy, where each pulse has its frequency stepped up across a range of frequencies, typically within the 3-8 GHz range. The other antennae 16 receive the transmitted signal and the received signal is detected and then recorded by the processor 4.

[0033] The shell 18 receives a cup 30. The cup 30 has a complementary shape to the shell 18 such that it fits snugly within the shell 18.

[0034] The outside of the cup 30 and the inside of the shell 18 may have threaded portions to enable a threaded engagement between the cup 30 and the shell 18. The threaded engagement between the cup 30 and the shell 18 may be used to translate the antenna array 6 relative to the breast 36, as described previously.

[0035] A layer of coupling fluid (dielectric constant controlled fluid) may be inserted in the gap 31 between the shell 18 and the cup 30 so as to improve the coupling between the antennae 16 and the cup 30 in order to minimise signal loss and thus improve transmission of the microwave signal.

[0036] In use, a patient lies in a prone position such that their breast 36 sits in the cup 30. A layer of coupling fluid may also be provided in the gap 35 between the cup 30 and the breast 36 in order to improve coupling between the antennae 16 and the breast 36.

[0037] Although not shown, one or more inserts may be placed inside the cup 30 so as to enable a better fit between the internal surface of the cup 30 and the breast 36. For example, a plurality of such inserts may be provided, each having different shapes and sizes, to enable the system to be better adapted to breasts of different shapes and sizes. The inserts may be made from the same material as the cup (e.g. ceramic).

[0038] The antenna 16 connected to the transmit path illuminates the breast 36 with the microwave signal. The signal is scattered by the breast tissue and the scattered signal is received at each of the non-transmitting antennae 16 where it is detected and recorded. This process is repeated for each antenna 16, as described previously.

[0039] The processor 4 may record the relative difference between the measured phase and amplitude of the transmitted signal as compared to the phase and amplitude of the scattered signal, recorded as a complex number (having real and imaginary parts).

[0040] The signal detected at each antenna 16 will generally comprise three components: a component arising from mutual coupling between the transmitting and receiving antennas 16; a component arising from radiation which reflects off the skin of the breast 36; and a component arising from radiation which reflects off structures within the breast (such as tumours). Tumours can generate identifiable reflections as they exhibit much higher dielectric properties than adipose tissues due to their significant water content. The mutual and skin reflection

components may be removed or at least mitigated from the data set in order to improve the detectability of reflections resulting from the presence of tumours within the breast.

[0041] The acquired data set may be used by the processor 4 to construct an image of the internal structure of the breast 36. Data reconstruction may be performed using Phased Array (frequency domain), Delay and Sum (DAS - time domain) techniques or any other suitable technique. From this, the processor 4 is able to identify (possibly, with additional user input or confirmation) a region of interest (if present) in which a possible tumour or other pathology may exist.

[0042] The precise position of the breast within the antenna array 6 and insert is likely to vary each time the breast is imaged due to variations in the fitting procedure. The positional relationship between the array 6 and the anatomy of the breast cannot usually be readily determined since there is no direct optical access to the array 6. This also makes it difficult to make a visual comparison between imaging modalities for the purposes of breast screening, cancer diagnosis (including image guided biopsy), tumour staging, treatment monitoring and surgical planning.

[0043] A marker 32, as shown in Figure 2, may be used to provide registration between the breast 36 and the array 6. The marker 32 may be formed by a rectangular sheet of thin aluminium foil with a resonant slot 34 extending into the body of the marker 32 midway along one of the sides. The marker 32 therefore has a substantially C or U-shaped profile formed by a pair of legs 38a, 38b either side of the resonant slot 34 and a base portion 40 joining the legs 38a, 38b.

[0044] In an example, the marker 32 may have a width of 5.5mm across the base portion 40 and a length of 9mm. The resonant slot 34 may have a length of 5.5mm (the length of the legs 36a, 36b) and a width of 1.5mm such that the legs 38a, 38b each have a width of 2mm.

[0045] In another example, the marker 32 may have a width of 8.0mm across the base portion 40 and a length of 9mm. The resonant slot 34 may have a length of 4.5mm (the length of the legs 38a, 38b) and a width of 1.5mm such that the legs 38a, 38b each have a width of 3.25mm.

[0046] The ratio of the length of the resonant slot 34 to the length of the marker 32 may be approximately 0.5-0.7. The ratio of the width of the resonant slot 34 to the width of the marker 32 may be approximately 0.1-0.3. However, other dimensions may be used.

[0047] As shown in Figure 3, the marker 32 is affixed to the surface of the skin of the breast 36. The marker 32 may be affixed to the skin using any suitable medical adhesive or the like. The thin aluminium foil of the marker 32 is able to conform to the contours of the breast and so has a low-profile enabling it to fit against the array 6. The aluminium foil used for the marker 32 is both low cost and hypo-allergenic. In another arrangement, as opposed to attaching the marker 32 directly to the skin, the marker 32 is fixed to the cup 30 or the insert. This may

allow the marker 32 to be in a fixed, known position, which may assist in the calibration of the system 2. If the marker 32 is attached to the cup 30 or the insert, in use, the marker 32 may overlie the skin without being in direct contact with the skin. The marker 32 could be adhered to an inner or outer surface of the cup 30 or insert, or it could be embedded within the cup 30 or insert substrate.

[0048] The marker 32 exhibits well defined microwave scattering characteristics such that it can be distinguished from the tissue of the breast 36. The dimensions of the resonant slot 34 may be configured to provide the marker 32 with resonant properties within the UWB region which provides for an enhanced radar cross-section at a particular frequency while having a reduced cross-section outside the resonant region. A range of markers 32 could also be fabricated with different resonant frequencies so as to allow them to be distinguished from one another.

[0049] As shown in Figure 4, the position of the marker 32 is easily identifiable in the images of the breast 36 generated by the system.

[0050] The marker 32 described above is a passive marker which provides a linear response to the microwave signal. In other words, the signal scattered/reflected by the marker 32 and received by the antennae 16 generally has the same frequency as the signal transmitted by the antennae 16. The response of the marker 32 is therefore similar to the tissue of the breast 36 which is a generally linear medium.

[0051] Figure 5 shows an example of a non-linear marker 132. The marker 132 may be a harmonic transponder formed by an antenna coupled to a diode, such as a Schottky diode.

[0052] The marker 132 receives the microwave signal at a certain fundamental frequency and converts this signal to a harmonic response signal at frequency that is an integer multiple of the fundamental frequency. In particular, the harmonic response signal may be the second harmonic frequency which provides optimum conversion efficiency. The diode of the marker 132 therefore effectively serves as a frequency doubler.

[0053] Other forms of non-linear transponder may also be used in which the response signal is modified through nonlinearities in the transponder. Active markers that contain an integrated circuit and/or power source may also be used which generate more complex scattering responses.

[0054] The use of a non-linear marker allows the marker to be easily distinguished from other scattering sources. This therefore provides improved performance when in the presence of strong environmental clutter. For example, if the marker simply responds back at the interrogation frequency in an environment with strong clutter, its response could be obscured by reflections. By using a non-linear response signal, it is easier to conclude that the observed response is caused by the marker rather than the surroundings. This is due to the fact that most natural objects do not display nonlinear properties at typ-

ical power levels used in microwave radar and therefore are not able to reflect back at frequencies which are different to the incoming frequency.

[0055] The use of one or more markers during the imaging process enables the image data to be easily related to the actual anatomy of the patient after imaging has taken place. This may be particularly useful where the images are used for subsequent breast biopsy or surgery with the markers on the skin of the breast providing guidance.

[0056] The marker(s) may be attached to the patient in standardised and predefined positions which will allow the physician to relate the visual position of the marker to the imaged position of the marker and the imaged positions of associated structures within the patient so that the physician can visualise the position of these structures by referring to the visual localisation marker.

[0057] The marker(s) may be located in standardised and well-defined position(s) such that images taken at different times can be compared against one another. The markers may be returned to the same positions for each image using a digital imaging system.

[0058] The marker(s) may be identifiable in additional, complementary imaging modalities beyond microwave imaging. In particular, the marker(s) may be utilised also during Magnetic Resonance Imaging (MRI). The different imaging techniques may be used to refine the diagnosis of a lesion. It will be appreciated that the position of the breast in such other imaging modalities may be very different and the use of common markers which can be viewed in each modality thus provides registration between the images.

[0059] The marker may incorporate a contrast agent sealed within a chamber in a container formed from a solid material. The contrast agent is selected to produce a change in signal intensity under MRI. The contrast agent may also be directly visible by microwave radar. Alternatively, an additional marker may be sealed within the chamber to provide visibility to microwave radar imaging.

[0060] The markers may also be compatible with other modalities, including, for example, X-rays, computed tomographic (CT) X-ray imaging, ultrasound, electrical impedance tomography (EIT), magnetic source imaging (MSI), magnetic resonance spectroscopy (MRS), magnetic resonance mammography (MRM), magnetic resonance angiography (MRA), magneto-electro-encephalography (MEG), laser optical imaging, electric potential tomography (EPT), and nuclear medicine modalities such as positron emission tomography (PET) and single photon emission computed tomography (SPECT).

[0061] The electromagnetic properties of the marker are stable over time and are accurately quantified. This enables the marker to act as a reference in the microwave imaging system without the requirement to use a phantom. Microwave scattering parameter data can change over time due to electronics drift, change in switching characteristics and cable effects and the use of the mark-

er as a reference marker thus allows these changes to be accounted for.

[0062] Microwave scattering parameter data that includes a reference marker can be used to create quantitative data sets relating to breast dielectric properties rather than relative normalized values. Quantitative data sets can be compared over time to observe changes in the breast for screening and for monitoring neoadjuvant therapy.

[0063] The quality of image reconstruction is also dependent on certain assumptions and system parameters that can change over time. A reference marker or markers can be used to improve the quality of image reconstruction, for example focusing, as the marker has known scattering characteristics, size and position relative to the conformal antenna array 6.

[0064] The radar cross-section of the reference markers may be configured so that they shine at a predefined brightness. This allows a reference level of scattering to be defined within the image, so that other images can be defined in their brightness by comparison with the reference marker. The reference markers can therefore provide a quantifiable measure for clutter reduction in the obtained images.

[0065] Markers can be designed with specific known RF scattering characteristics, and so can provide standard references to quantify and adjust measured scattering by comparison against the references. 'RF scattering characteristics' may include brightness, spectrum ('colour'), and directionality. In one embodiment, the medical imaging system may image the marker without a body part. The image of the marker may be used to calibrate the medical imaging system. For example, if the marker has a known characteristic (e.g. a known brightness) then subsequently the measured scattering of microwave signals by a body part may be corrected or adjusted based on the known response of the marker.

[0066] Markers can be placed at known spatial positions, and so can provide spatial reference points against which the spatial image reconstruction can be adjusted by comparing the reconstructed marker position against the known reference position in order to correct for spatial distortion.

[0067] Markers can be placed at known spatial positions and so can provide spatial reference points against which reconstruction parameters including for instance refractive index may be adjusted to optimally focus (autofocus). The process of autofocus by adjusting reconstruction parameters also provides estimates of those actual parameters, thus providing an extra measurement.

[0068] Although the system has been described with reference to the imaging of a breast, it will be appreciated that it may be adapted for other areas of the body.

[0069] In other arrangements, the cup of the antenna array may be dispensed with or integrated into the shell in which the antennae are located.

[0070] The system may employ multiple transmit and receive paths, such that data can be recorded from mul-

tiple antennas simultaneously, and may even comprise a number of transmit and receive paths corresponding to the number of antennas, such that data can be recorded from all antennas simultaneously. In an alternative topology, the switching matrix could be removed thus allowing each antenna to be connected to a transmitting/receiving device.

[0071] Alternatively, more than one antenna may be operated at a time in a frequency multiplexed operation. Multiplexed operation may have significant advantages where high speed tracking of the needle is required.

[0072] To avoid unnecessary duplication of effort and repetition of text in the specification, certain features are described in relation to only one or several aspects or embodiments of the invention. However, it is to be understood that, where it is technically possible, features described in relation to any aspect or embodiment of the invention may also be used with any other aspect or embodiment of the invention.

[0073] The invention is not limited to the embodiments described herein, and may be modified or adapted without departing from the scope of the present invention, which is defined by the appended claims.

Claims

1. A medical imaging system (2) comprising:

a microwave antenna array (6) comprising a transmitting antenna (16) and a plurality of receiving antennae (16), wherein the transmitting antenna (16) is configured to transmit microwave signals so as to illuminate a body part of a patient and the receiving antennae (16) are configured to receive the microwave signals following scattering within the body part;
a marker (32) configured to scatter the microwave signals; and
a processor (4); **characterized in that** the marker (32) is configured to overlie the surface of the skin of the body part, and the processor (4) is configured to generate an image of the internal structure of the body part and the marker (32) by processing the scattered microwave signals so as to identify a region of interest within the body part relative to the position of the marker.

2. A medical imaging system as claimed in claim 1, wherein the marker is a passive antenna having a resonant slot.

3. A medical imaging system as claimed in claim 1 or 2, wherein the marker is formed of a metal foil which conforms to the shape of the body part.

4. A medical imaging system as claimed in any preceding claim, wherein the marker is a non-linear antenna

which scatters the microwave signal at a frequency which is different to the frequency of the received microwave signal;
wherein optionally the non-linear antenna is a harmonic antenna.

5. A medical imaging system as claimed in any preceding claim, wherein the marker comprises a contrast agent.

6. A medical imaging system according to any preceding claim, wherein the processor is configured to calibrate the medical imaging system based on the marker;
wherein optionally the processor is configured to calibrate the medical imaging system based on the scattering characteristics of the marker.

7. A medical imaging system according to any preceding claim, wherein the marker is configured to be applied to the surface of the skin;
wherein optionally the marker is provided with an adhesive for adhering the marker to the surface of the skin.

8. A medical imaging system according to any of claims 1 to 6, wherein the marker is attached to a component which is arranged to be fixed in position;
wherein optionally the component comprises a cup.

9. A medical imaging system according to claim 8, wherein the component is configured to:

be in contact with at least a portion of a body part; and/or
receive at least a portion of a body part.

10. A medical imaging method comprising:

providing a marker (32) such that it overlies the surface of the skin of a body part;
illuminating the marker (32) and the body part with microwave signals emitted by a transmitting antenna (16) of a microwave antenna array (6);
receiving the microwave signals following scattering within the body part and by the marker (32) at a plurality of receiving antennae (16) of the microwave antenna array (6);
generating an image of the body part showing an internal structure of the body part and the marker (32) by processing the scattered microwave signals, so as to identify a region of interest within the body part relative to the position of the marker (32).

11. A medical imaging method as claimed in claim 10, further comprising: performing image registration between a plurality of images by correlating the po-

sition of the marker in each image; and optionally: generating an image of the marker using a different imaging modality including at least one of: X-rays, computed tomographic (CT) X-ray imaging, ultrasound, electrical impedance tomography (EIT), magnetic source imaging (MSI), magnetic resonance spectroscopy (MRS), magnetic resonance mammography (MRM), magnetic resonance angiography (MRA), magnetoencephalography (MEG), laser optical imaging, electric potential tomography (EPT), and nuclear medicine modalities such as positron emission tomography (PET) and single photon emission computed tomography (SPECT).

12. A medical imaging method as claimed in any of claims 10 or 11, further comprising adjusting the spatial image reconstruction to correct for spatial distortion by comparing the position of the marker within the image with its known reference position.
13. A medical imaging method as claimed in any of claims 10 to 12, further comprising adjusting reconstruction parameters based on a known reference position of the marker; wherein optionally the images are taken at different instances by reapplying the marker to the same position on the skin.
14. A medical imaging method as claimed in claim 13, further comprising using the known scattering characteristics of the marker as a reference to adjust the measured scattering from the body part.
15. A medical imaging method according to any of claims 10 to 14, further comprising calibrating a medical imaging system based on the marker; and optionally: calibrating the medical imaging system based on the scattering characteristics of the marker.

Patentansprüche

1. Medizinisches Bildgebungssystem (2), umfassend:

ein Mikrowellenantennenarray (6), umfassend eine Sendeantenne (16) und mehrere Empfangsantennen (16), wobei die Sendeantenne (16) ausgebildet ist zum Übertragen von Mikrowellensignalen, um einen Körperteil eines Patienten zu beleuchten, und die Empfangsantennen (16) ausgebildet sind zum Empfangen der Mikrowellensignale nach der Streuung innerhalb des Körperteils; einen Marker (32), der ausgebildet ist zum Streuen der Mikrowellensignale; und einen Prozessor (4);
dadurch gekennzeichnet, dass der Marker

(32) so ausgebildet ist, dass er über der Oberfläche der Haut des Körperteils liegt und der Prozessor (4) so ausgebildet ist, dass er ein Bild der internen Struktur des Körperteils und des Markers (32) generiert, indem die gestreuten Mikrowellensignale so verarbeitet werden, dass ein interessierendes Gebiet innerhalb des Körperteils relativ zu der Position des Markers identifiziert wird.

2. Medizinisches Bildgebungssystem nach Anspruch 1, wobei der Marker eine passive Antenne mit einem Resonanzschlitz ist.
3. Medizinisches Bildgebungssystem nach Anspruch 1 oder 2, wobei der Marker aus einer Metallfolie ausgebildet ist, die der Form des Körperteils entspricht.
4. Medizinisches Bildgebungssystem nach einem vorhergehenden Anspruch, wobei der Marker eine nichtlineare Antenne ist, die das Mikrowellensignal bei einer Frequenz streut, die von der Frequenz des empfangenen Mikrowellensignals verschieden ist; wobei die nichtlineare Antenne optional eine Oberflächenantenne ist.
5. Medizinisches Bildgebungssystem nach einem vorhergehenden Anspruch, wobei der Marker ein Kontrastmittel umfasst.
6. Medizinisches Bildgebungssystem nach einem vorhergehenden Anspruch, wobei der Prozessor so ausgebildet ist, dass er das medizinische Bildgebungssystem auf Basis des Markers kalibriert; wobei der Prozessor optional so ausgebildet ist, dass er das medizinische Bildgebungssystem auf Basis der Streucharakteristika des Markers kalibriert.
7. Medizinisches Bildgebungssystem nach einem vorhergehenden Anspruch, wobei der Marker so ausgewählt ist, dass er auf der Oberfläche der Haut angebracht wird; wobei der Marker optional mit einem Kleber versehen ist, damit der Marker an der Oberfläche der Haut haftet.
8. Medizinisches Bildgebungssystem nach einem der Ansprüche 1 bis 6, wobei der Marker an einer Komponente angebracht ist, die ausgelegt ist, um an ihrer Position fixiert zu werden; wobei die Komponente optional eine Tasse umfasst.
9. Medizinisches Bildgebungssystem nach Anspruch 8, wobei die Komponente ausgebildet ist: um mit mindestens einem Abschnitt eines Körperteils in Kontakt zu sein und/oder um mindestens einen Abschnitt eines Körperteils aufzunehmen.

10. Medizinisches Bildgebungsverfahren, umfassend:

Bereitstellen eines Markers (32), so dass er über der Oberfläche der Haut eines Körperteils liegt; Beleuchten des Markers (32) und des Körperteils mit durch eine Sendeantenne (16) eines Mikrowellenantennenarrays (6) emittierten Mikrowellensignalen; Empfangen der Mikrowellensignale nach dem Streuen innerhalb des Körperteils und durch den Marker (32) an mehreren Empfangsantennen (16) des Mikrowellenantennenarrays (6); Generieren eines Bilds des Körperteils, das eine interne Struktur des Körperteils und den Marker (32) zeigt, durch Verarbeiten der gestreuten Mikrowellensignale, so dass ein interessierendes Gebiet innerhalb des Körperteils relativ zu der Position des Markers (32) identifiziert wird.

11. Medizinisches Bildgebungsverfahren nach Anspruch 10, weiterhin umfassend: Durchführen einer Bildregistrierung zwischen mehreren Bildern durch Korrelieren der Position des Markers in jedem Bild; und optional:

Generieren eines Bilds des Markers unter Verwendung einer anderen Bildgebungsmodalität beinhal- tend mindestens eines von: Röntgenstrahlen, computertomographische (CT) Röntgenbildgebung, Ultraschall, elektrische Impedanz-Tomographie (EIT), Magnetquellenbildgebung (MSI), Magnetresonanzspektroskopie (MRS), Magnetresonanzmammographie (MRM), Magnetresonanzangiographie (MRA), Magnetelektroecephalographie (MEG), laseroptische Bildgebung, elektrische Potentialtomographie (EPT) und Nuklearmedizinmodalitäten wie etwa Positronenemissionstomographie (PET) und Einzelphotonen-Emissionscomputertomographie (SPECT).

12. Medizinisches Bildgebungsverfahren nach einem der Ansprüche 10 oder 11, weiterhin umfassend das Verstellen der Raumbildrekonstruktion, um eine räumliche Verzerrung durch Vergleichen der Position des Markers innerhalb des Bilds mit seiner bekannten Referenzposition zu korrigieren.

13. Medizinisches Bildgebungsverfahren nach einem der Ansprüche 10 bis 12, weiterhin umfassend das Verstellen von Rekonstruktionsparametern auf Basis einer bekannten Referenzposition des Markers; wobei optional die Bilder bei verschiedenen Instanzen aufgenommen werden, indem der Marker wieder auf der gleichen Position auf der Haut angebracht wird.

14. Medizinisches Bildgebungsverfahren nach Anspruch 13, weiterhin umfassend das Verwenden der bekannten Streucharakteristika des Markers als ei-

ne Referenz zum Verstellen der gemessenen Streuung von dem Körperteil.

15. Medizinisches Bildgebungsverfahren nach einem der Ansprüche 10 bis 14, weiterhin umfassend das Kalibrieren eines medizinischen Bildgebungssystems auf Basis des Markers; und optional: Kalibrieren des medizinischen Bildgebungssystems auf Basis der Streucharakteristika des Markers.

Revendications

1. Système d'imagerie médicale (2) comprenant :

un réseau d'antennes micro-ondes (6) comprenant une antenne émettrice (16) et une pluralité d'antennes réceptrices (16), dans lequel l'antenne émettrice (16) est conçue pour émettre des signaux micro-ondes de façon à éclairer une partie corporelle d'un patient et les antennes réceptrices (16) sont conçues pour recevoir les signaux micro-ondes après diffusion dans la partie corporelle ;

un marqueur (32) configuré pour diffuser les signaux micro-ondes ; et

un processeur (4) ; **caractérisé en ce que** le marqueur (32) est configuré pour recouvrir la surface de la peau de la partie corporelle, et le processeur (4) est configuré pour générer une image de la structure interne de la partie corporelle et du marqueur (32) en traitant les signaux micro-ondes diffusés de façon à identifier une région d'intérêt dans la partie corporelle par rapport à la position du marqueur.

2. Système d'imagerie médicale selon la revendication 1, dans lequel le marqueur est une antenne passive possédant une fente résonante.

3. Système d'imagerie médicale selon la revendication 1 ou 2, dans lequel le marqueur est fait en feuille métallique qui épouse la forme de la partie corporelle.

4. Système d'imagerie médicale selon l'une quelconque des revendications précédentes, dans lequel le marqueur est une antenne non linéaire qui diffuse le signal micro-ondes à une fréquence qui est différente de la fréquence du signal micro-ondes reçu ; dans lequel éventuellement l'antenne non linéaire est une antenne harmonique.

5. Système d'imagerie médicale selon l'une quelconque des revendications précédentes, dans lequel le marqueur comprend un agent de contraste.

6. Système d'imagerie médicale selon l'une quelcon-

- que des revendications précédentes, dans lequel le processeur est configuré pour étalonner le système d'imagerie médicale sur la base du marqueur ; dans lequel éventuellement le processeur est configuré pour étalonner le système d'imagerie médicale sur la base des caractéristiques de diffusion du marqueur.
7. Système d'imagerie médicale selon l'une quelconque des revendications précédentes, dans lequel le marqueur est conçu pour être appliqué à la surface de la peau ; dans lequel éventuellement le marqueur est doté d'un adhésif pour faire adhérer le marqueur à la surface de la peau.
8. Système d'imagerie médicale selon l'une quelconque des revendications 1 à 6, dans lequel le marqueur est fixé à un composant qui est conçu pour être fixé en position ; dans lequel éventuellement le composant comprend une coupe.
9. Système d'imagerie médicale selon la revendication 8, dans lequel le composant est conçu pour :
- être en contact avec au moins une partie d'une partie corporelle ; et/ou
accueillir au moins une partie d'une partie corporelle.
10. Procédé d'imagerie médicale consistant à :
- fournir un marqueur (32) de sorte qu'il recouvre la surface de la peau d'une partie corporelle ; éclairer le marqueur (32) et la partie corporelle avec des signaux micro-ondes émis par une antenne émettrice (16) d'un réseau (6) d'antennes micro-ondes ; recevoir les signaux micro-ondes après diffusion dans la partie corporelle et par le marqueur (32) au niveau d'une pluralité d'antennes réceptrices (16) du réseau (6) d'antennes micro-ondes ; générer une image de la partie corporelle montrant une structure interne de la partie corporelle et du marqueur (32) en traitant les signaux micro-ondes diffusés, de façon à identifier une région d'intérêt dans la partie corporelle par rapport à la position du marqueur (32).
11. Procédé d'imagerie médicale selon la revendication 10, consistant en outre à : réaliser un alignement d'images entre de multiples images en mettant en corrélation la position du marqueur dans chaque image ; et éventuellement : générer une image du marqueur à l'aide d'une modalité d'imagerie différente comprenant au moins un
- parmi : des rayons X, une tomodesitométrie (TDM), une échographie, une tomographie d'impédance électrique (TIE), une imagerie par source magnétique (ISM), une spectroscopie par résonance magnétique (SRM), une mammographie par résonance magnétique (MRM), une angiographie par résonance magnétique (ARM), une magnétoélectro-encéphalographie (MEG), une imagerie optique laser, une tomographie à potentiel électrique (TPE), et des modalités de médecine nucléaire telles que la tomographie par émission de positons (TEP) et la tomographie d'émission à photon unique (TEPU).
12. Procédé d'imagerie médicale selon l'une quelconque des revendications 10 et 11, consistant en outre à ajuster la reconstruction d'images spatiales pour corriger la distorsion spatiale en comparant la position du marqueur dans l'image avec sa position de référence connue.
13. Procédé d'imagerie médicale selon l'une quelconque des revendications 10 à 12, consistant en outre à ajuster des paramètres de reconstruction sur la base d'une position de référence connue du marqueur ; dans lequel éventuellement les images sont prises à des occurrences différentes en réappliquant le marqueur à la même position sur la peau.
14. Procédé d'imagerie médicale selon la revendication 13, consistant en outre à utiliser les caractéristiques de diffusion connues du marqueur en tant que référence pour ajuster la diffusion mesurée provenant de la partie corporelle.
15. Procédé d'imagerie médicale selon l'une quelconque des revendications 10 à 14, consistant en outre à étalonner un système d'imagerie médicale sur la base du marqueur ; et éventuellement à : étalonner le système d'imagerie médicale sur la base des caractéristiques de diffusion du marqueur.

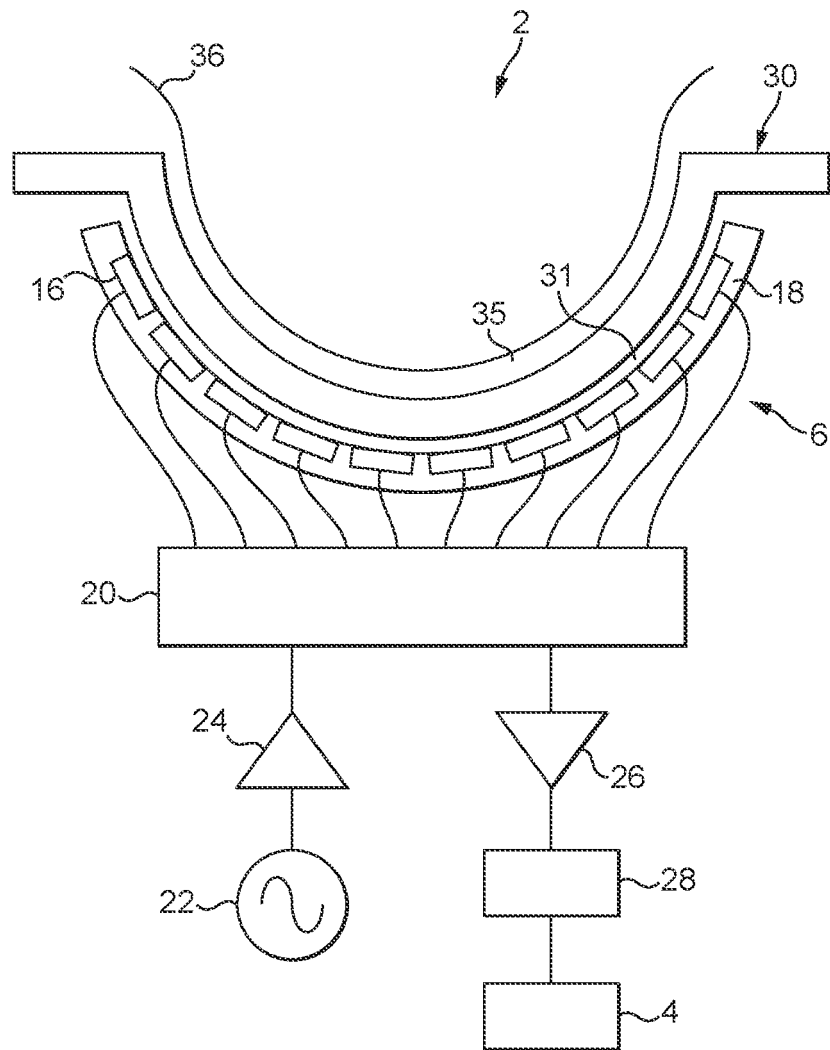


FIG. 1

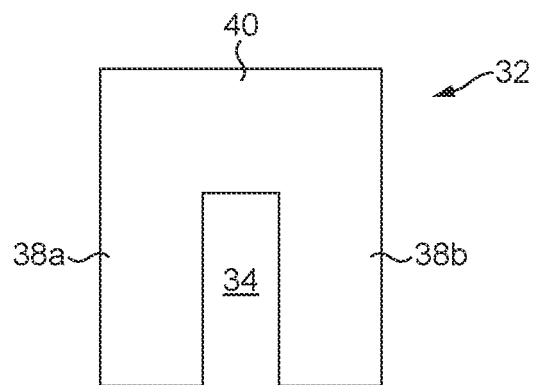


FIG. 2

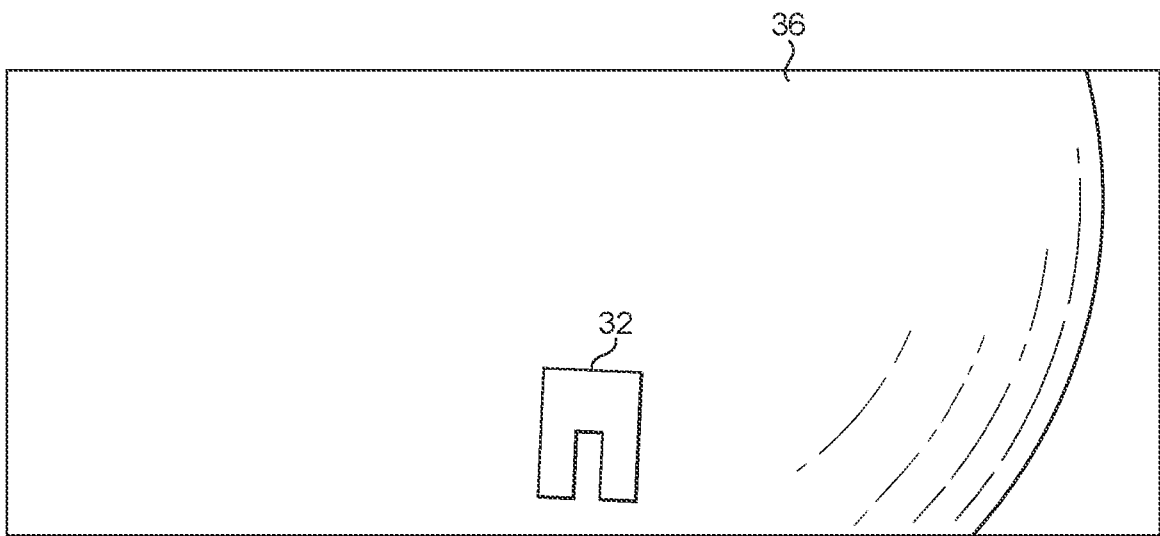


FIG. 3

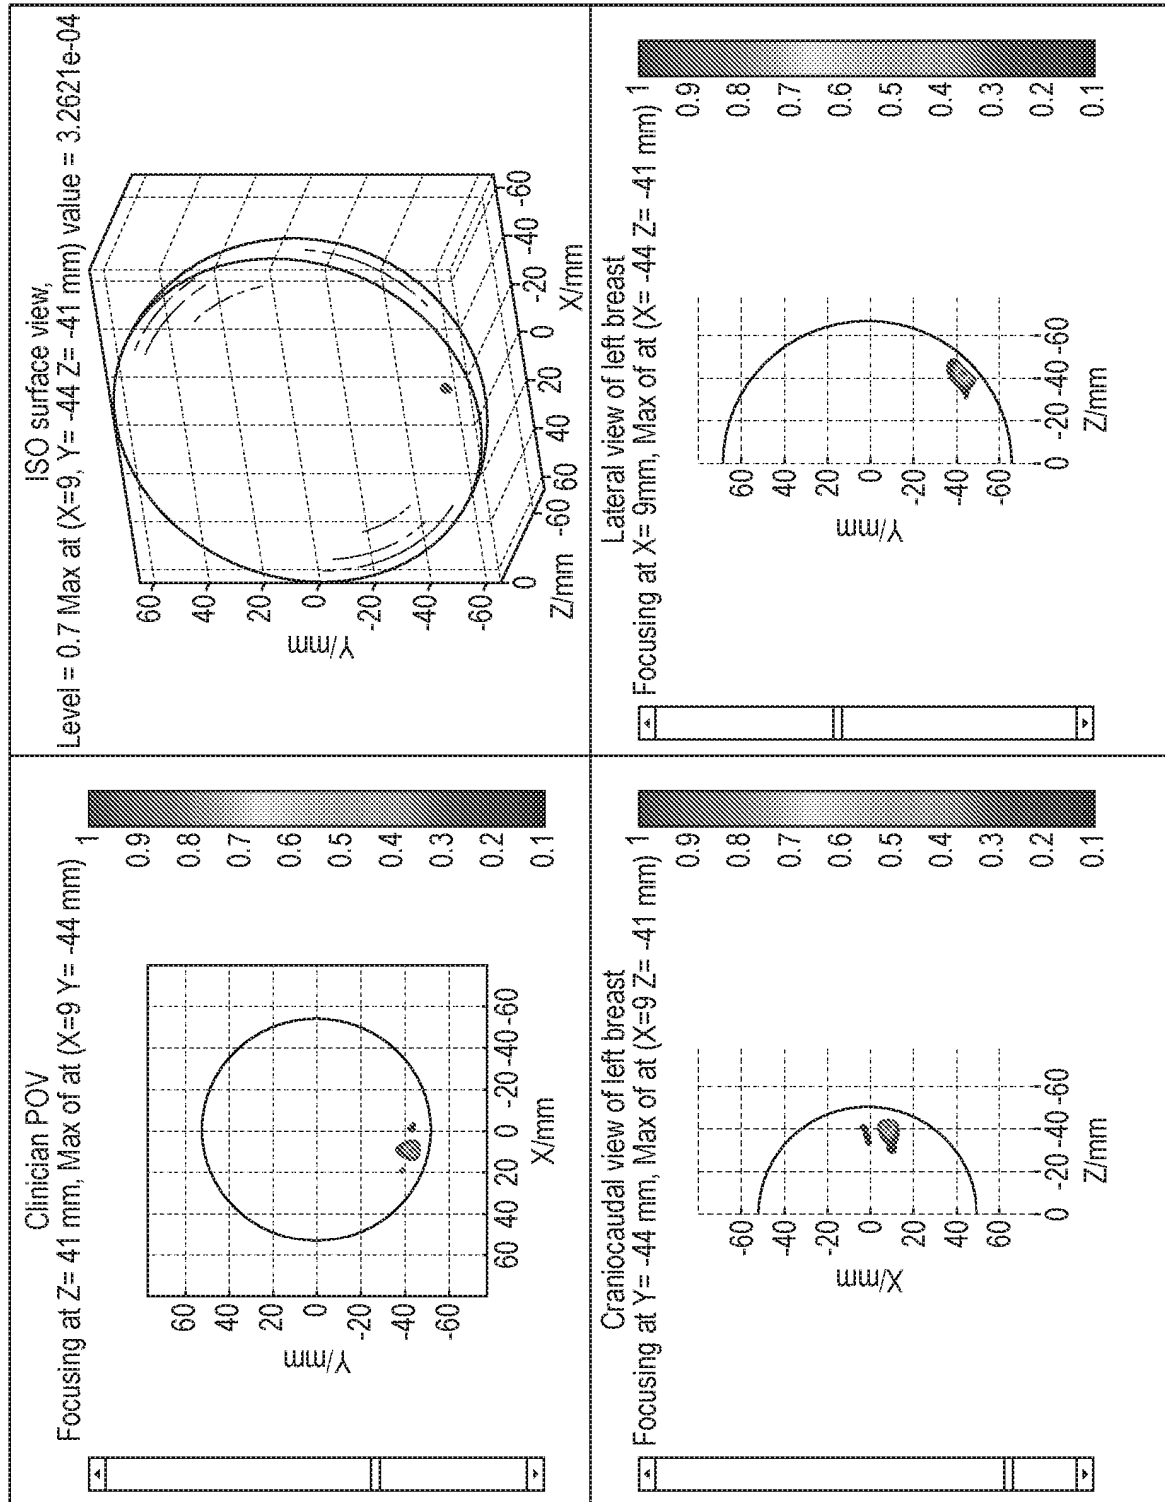


FIG. 4

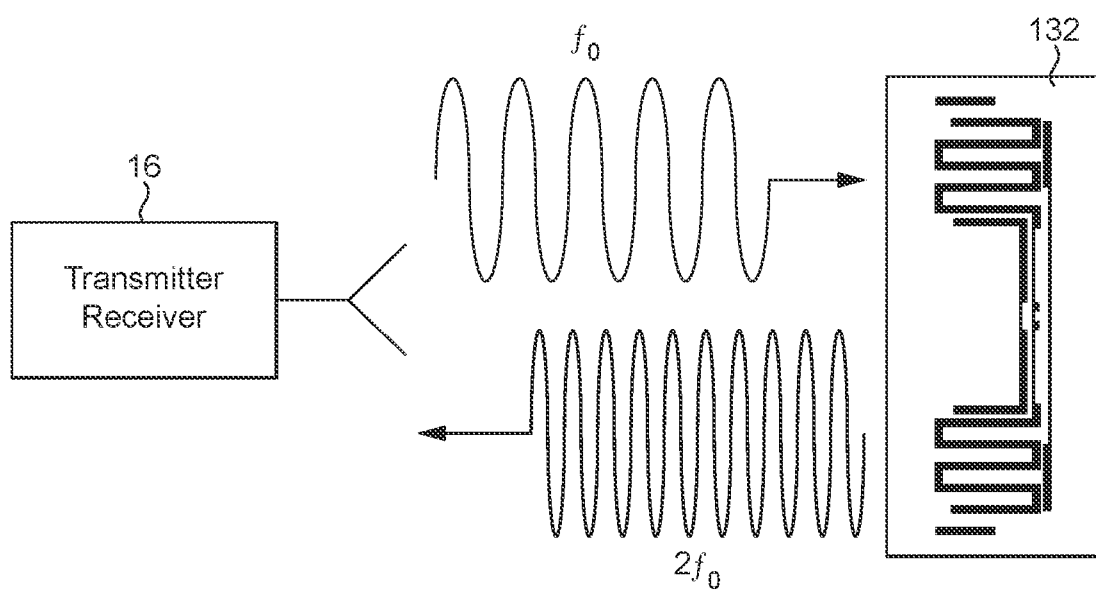


FIG. 5

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 2014149183 A [0004]
- RU 2578298 [0004]
- DE 102009007255 [0004]
- WO 9838919 A [0004]

专利名称(译)	医学成像系统和方法		
公开(公告)号	EP3457934A1	公开(公告)日	2019-03-27
申请号	EP2017725735	申请日	2017-05-17
[标]申请(专利权)人(译)	MICRIMA		
申请(专利权)人(译)	MICRIMA有限公司		
当前申请(专利权)人(译)	MICRIMA有限公司		
[标]发明人	BANNISTER PETER ROMILLY THOMAS KEVIN LESLIE		
发明人	BANNISTER, PETER ROMILLY THOMAS, KEVIN LESLIE		
IPC分类号	A61B5/05 A61B5/00		
CPC分类号	A61B5/0507 A61B5/4312 A61B5/6823 A61B2090/3908 A61B2090/3937 A61B2090/3954 A61B2090/397 A61B2090/3995 A61B90/37 A61B90/39		
代理机构(译)	慧智林LLP		
优先权	2016008687 2016-05-17 GB		
其他公开文献	EP3457934B1		
外部链接	Espacenet		

摘要(译)

描述了一种医学成像系统和方法。该系统包括：微波天线阵列，其包括发射天线和多个接收天线，其中，发射天线被配置为发射微波信号以便照亮患者的身体部位，并且接收天线被配置为接收微波信号。在身体内部散射之后；标记物，其被配置为应用于身体部位的皮肤表面并散射微波信号；处理器，被配置为处理散射的微波信号并生成身体部位和标记物的内部结构的图像，以便识别相对于标记物位置的身体部位内的感兴趣区域。