



US007072701B2

(12) **United States Patent**
Chen et al.

(10) **Patent No.:** **US 7,072,701 B2**
(45) **Date of Patent:** **Jul. 4, 2006**

- (54) **METHOD FOR SPECTROPHOTOMETRIC BLOOD OXYGENATION MONITORING**
4,510,938 A 4/1985 Jobsis et al.
4,570,638 A 2/1986 Stoddart et al.
4,621,643 A 11/1986 New, Jr. et al.
- (75) Inventors: **Bo Chen**, Derby, CT (US); **Paul B. Benni**, Stamford, CT (US)
4,690,492 A 9/1987 Beard
4,700,708 A 10/1987 New, Jr. et al.
4,725,147 A 2/1988 Stoddart
- (73) Assignee: **CAS Medical Systems, Inc.**, Branford, CT (US)
4,768,516 A 9/1988 Stoddart et al.
4,770,179 A 9/1988 New, Jr. et al.
4,805,623 A 2/1989 Jöbsis

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 185 days.

(Continued)

Primary Examiner—Eric F. Winakur

(74) Attorney, Agent, or Firm—O’Shea, Getz & Kosakowski, P.C.

(21) Appl. No.: **10/628,068**

(22) Filed: **Jul. 24, 2003**

(57) **ABSTRACT**

(65) **Prior Publication Data**

US 2004/0024297 A1 Feb. 5, 2004

Related U.S. Application Data

(60) Provisional application No. 60/407,277, filed on Aug. 30, 2002, provisional application No. 60/398,937, filed on Jul. 26, 2002.

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.** **600/331**

(58) **Field of Classification Search** **600/323, 600/331, 336; 250/339.09, 341.1, 341.5; 356/41, 319**

See application file for complete search history.


(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,638,640 A 2/1972 Shaw
- 3,674,008 A 7/1972 Johnson
- 4,105,021 A 8/1978 Williams et al.
- 4,206,764 A 6/1980 Williams
- 4,223,680 A 9/1980 Jobsis
- 4,281,645 A 8/1981 Jobsis
- 4,321,930 A 3/1982 Jobsis et al.
- 4,380,240 A 4/1983 Jobsis et al.

A method and apparatus for non-invasively determining the blood oxygen saturation level within a subject’s tissue is provided that utilizes a near infrared spectrophotometric (NIRS) sensor capable of transmitting a light signal into the tissue of a subject and sensing the light signal once it has passed through the tissue via transmittance or reflectance. The method includes the steps of: (1) transmitting a light signal into the subject’s tissue, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength; (2) sensing a first intensity and a second intensity of the light signal, along the first, second, and third wavelengths after the light signal travels through the subject at a first and second predetermined distance; (3) determining an attenuation of the light signal for each of the first, second, and third wavelengths using the sensed first intensity and sensed second intensity of the first, second, and third wavelengths; (4) determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength; and (5) determining the blood oxygen saturation level within the subject’s tissue using the difference in attenuation between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength.

50 Claims, 3 Drawing Sheets

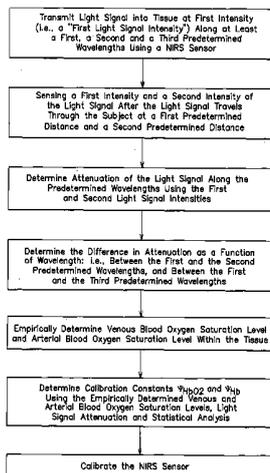

U.S. PATENT DOCUMENTS					
			5,529,065 A	6/1996	Tsuchiya
4,817,623 A	4/1989	Stoddart et al.	5,542,421 A	8/1996	Erdman
4,848,901 A	7/1989	Hood, Jr.	5,584,296 A	12/1996	Cui et al.
4,865,038 A	9/1989	Rich et al.	5,632,273 A	5/1997	Suzuki
4,907,876 A	3/1990	Suzuki et al.	5,661,302 A	8/1997	Evans et al.
4,913,150 A	4/1990	Cheung et al.	5,676,142 A	10/1997	Miwa et al.
4,942,877 A	7/1990	Sakai et al.	5,694,931 A	12/1997	Tsuchiya
5,054,488 A	10/1991	Muz	5,697,367 A	12/1997	Lewis et al.
5,057,695 A *	10/1991	Hirao et al. 600/310	5,720,284 A	2/1998	Aoyagi et al.
5,058,588 A	10/1991	Kaestle	5,729,333 A	3/1998	Osten et al. 356/39
5,080,098 A	1/1992	Willett et al.	5,746,206 A	5/1998	Mannheimer
5,088,493 A	2/1992	Giannini et al.	5,752,914 A	5/1998	Delonzor et al.
5,139,025 A	8/1992	Lewis et al.	5,758,644 A	6/1998	Diab et al.
5,140,989 A	8/1992	Lewis et al.	5,770,454 A	6/1998	Essenpreis et al.
5,153,669 A	10/1992	DeGroot	5,782,755 A	7/1998	Chance et al.
5,217,013 A	6/1993	Lewis et al.	5,795,292 A	8/1998	Lewis et al.
5,218,962 A	6/1993	Mannheimer et al.	5,803,909 A	9/1998	Maki et al.
5,277,181 A	1/1994	Mendelson et al.	5,853,370 A	12/1998	Chance et al.
5,349,961 A	9/1994	Stoddart et al.	5,879,294 A	3/1999	Anderson et al.
5,353,791 A	10/1994	Tamura et al.	5,902,235 A	5/1999	Lewis et al.
5,421,329 A	6/1995	Casciani et al.	5,987,351 A	11/1999	Chance
5,465,714 A	11/1995	Scheuing	6,192,260 B1	2/2001	Chance 600/310
5,477,853 A	12/1995	Farkas et al.	6,615,065 B1	9/2003	Barrett et al.
5,482,034 A	1/1996	Lewis et al.	2005/0119542 A1	6/2005	Stoddart et al.
5,517,987 A	5/1996	Tsuchiya			
5,520,177 A	5/1996	Ogawa et al.			
5,524,617 A	6/1996	Mannheimer			

* cited by examiner

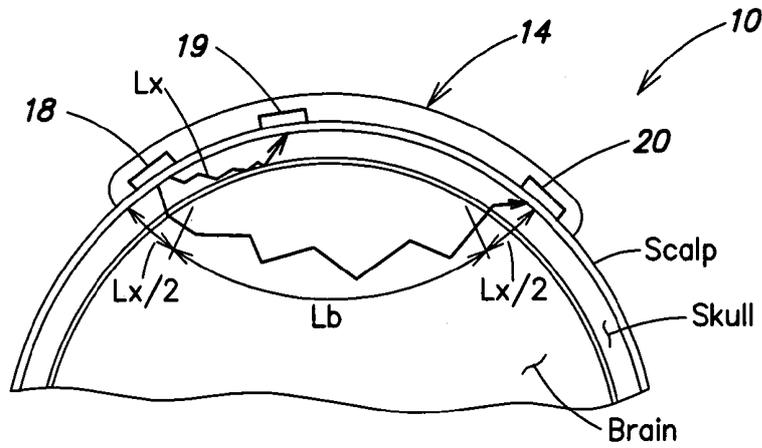


FIG. 1

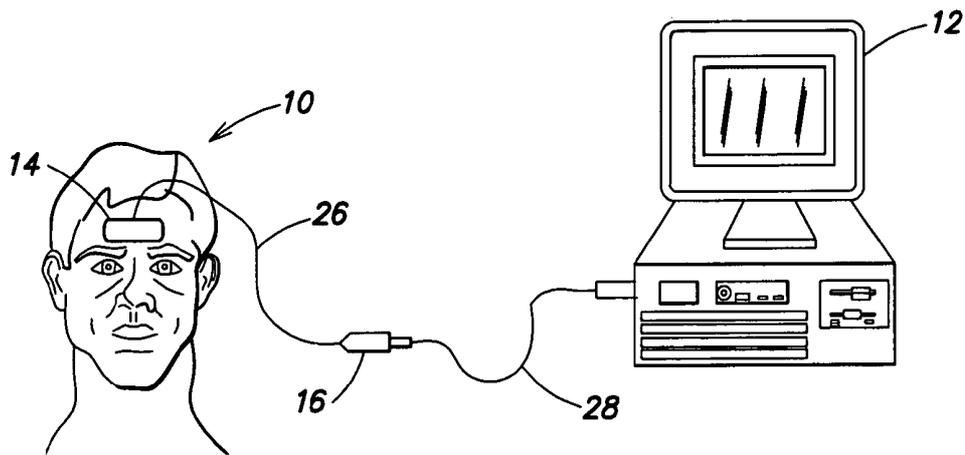


FIG. 2

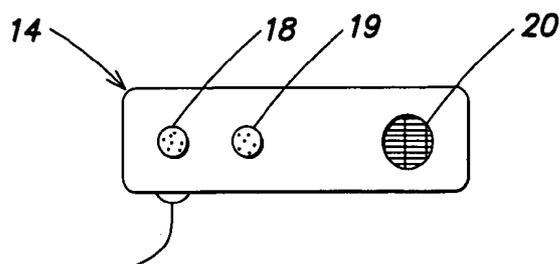
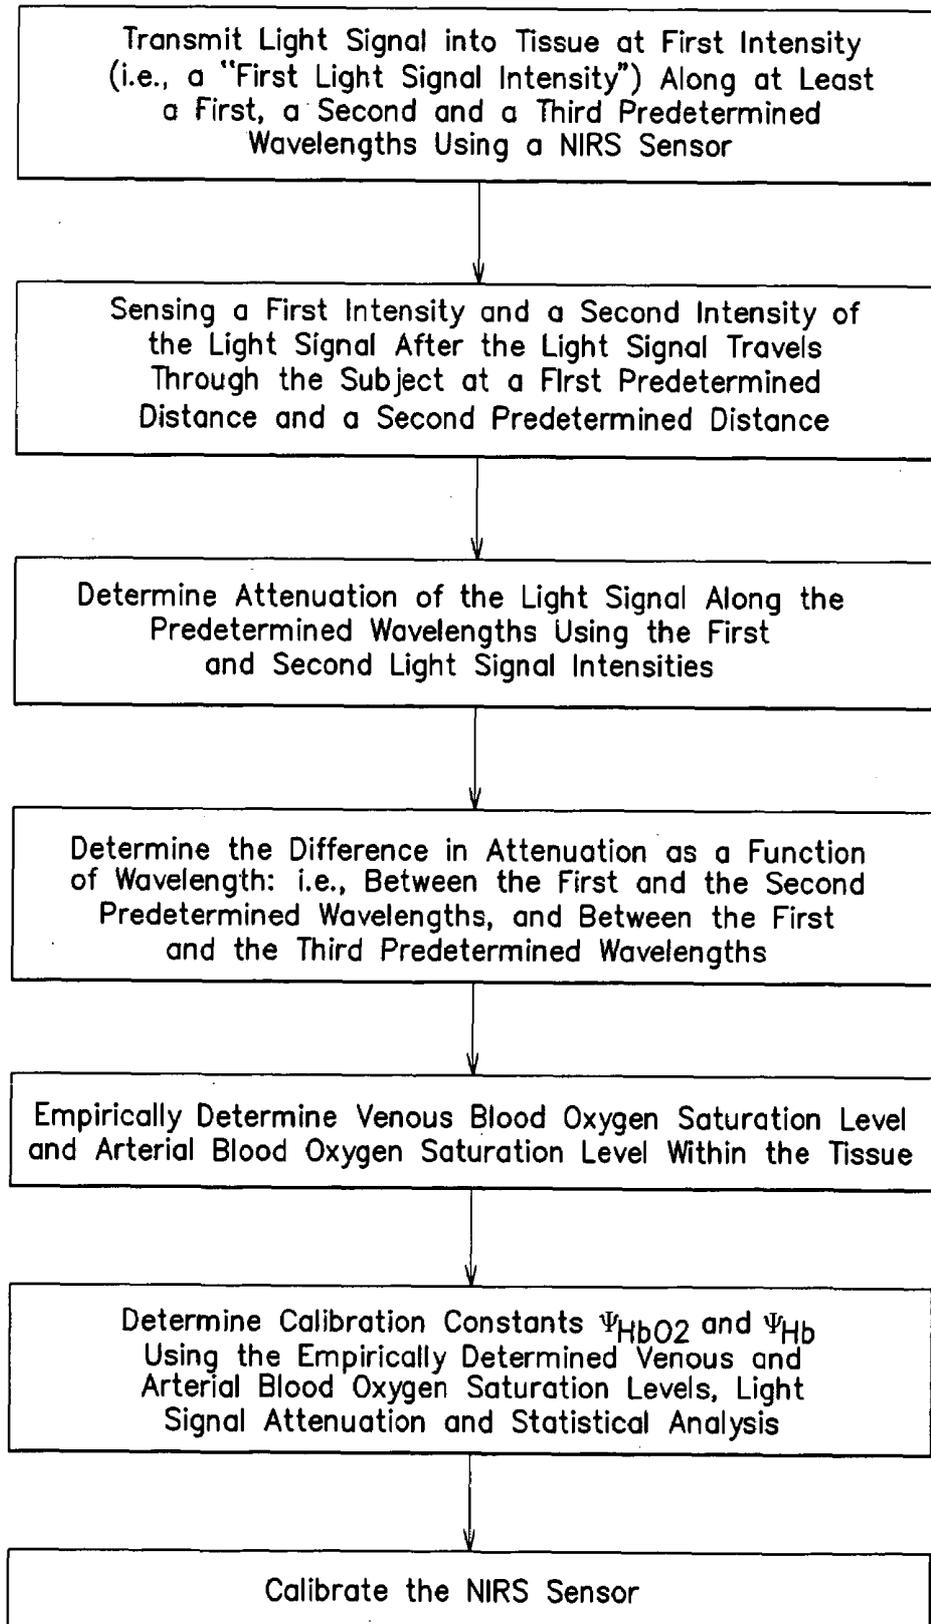


FIG. 3

**FIG. 4**

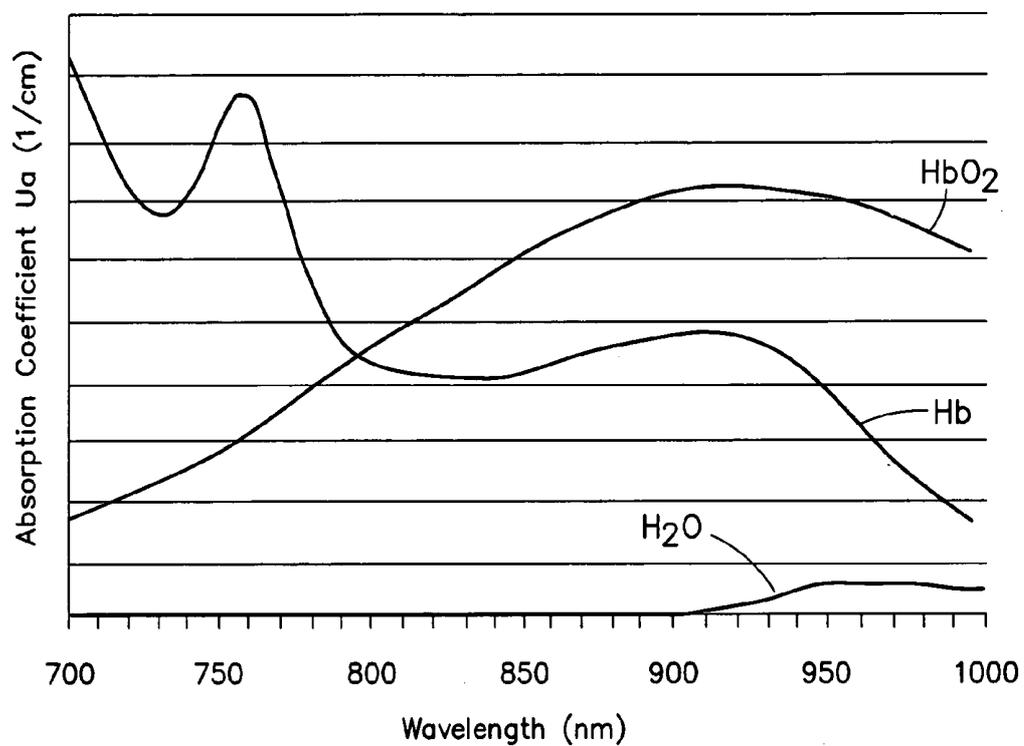


FIG. 5

METHOD FOR SPECTROPHOTOMETRIC BLOOD OXYGENATION MONITORING

This application claims the benefit of the filing date of U.S. Provisional Applications 60/398,937, filed Jul. 26, 2002, and 60/407,277 filed Aug. 30, 2002.

This invention was made with Government support under Contract No. 1R43NS045488-01 awarded by the Department of Health & Human Services. The Government has certain rights in the invention.

BACKGROUND OF THE INVENTION

1. Technical Field

This invention relates to methods for non-invasively determining biological tissue oxygenation in general, and to non-invasive methods utilizing near-infrared spectroscopy (NIRS) techniques in particular.

2. Background Information.

The molecule that carries the oxygen in the blood is hemoglobin. Oxygenated hemoglobin is called oxyhemoglobin (HbO₂) and deoxygenated hemoglobin is deoxyhemoglobin (Hb). Total hemoglobin is the summation of the two states of hemoglobin (Total Hb=HbO₂+Hb), and is proportional to relative blood volume changes, provided that the hematocrit or hemoglobin concentration of the blood is unchanged. The mammalian cardiovascular system consists of a blood pumping mechanism (the heart), a blood transportation system (blood vessels), and a blood oxygenation system (the lungs). Blood oxygenated by the lungs passes through the heart and is pumped into the arterial vascular system. Under normal conditions, oxygenated arterial blood consists predominately of HbO₂. Large arterial blood vessels branch off into smaller branches called arterioles, which profuse throughout biological tissue. The arterioles branch off into capillaries, the smallest blood vessels. In the capillaries, oxygen carried by hemoglobin is transported to the cells in the tissue, resulting in the release of oxygen molecules (HbO₂→Hb). Under normal conditions, only a fraction of the HbO₂ molecules give up oxygen to the tissue, depending on the cellular metabolic need. The capillaries then combine together into venuoles, the beginning of the venous circulatory system. Venuoles then combine into larger blood vessels called veins. The veins further combine and return to the heart, and then venous blood is pumped to the lungs. In the lungs, deoxygenated hemoglobin Hb collects oxygen becoming HbO₂ again and the circulatory process is repeated.

Oxygen saturation is defined as:

$$\text{O}_2 \text{ saturation \%} = \frac{\text{HbO}_2}{(\text{HbO}_2 + \text{Hb})} * 100\% \quad (\text{Eqn. 1})$$

In the arterial circulatory system under normal conditions, there is a high proportion of HbO₂ to Hb, resulting in an arterial oxygen saturation (defined as SaO₂ %) of 95–100%. After delivery of oxygen to tissue via the capillaries, the proportion of HbO₂ to Hb decreases. Therefore, the measured oxygen saturation of venous blood (defined as SvO₂ %) is lower and may be about 70%.

One spectrophotometric method, called pulse oximetry, determines arterial oxygen saturation (SaO₂) of peripheral tissue (i.e. finger, ear, nose) by monitoring pulsatile optical attenuation changes of detected light induced by pulsatile arterial blood volume changes in the arteriolar vascular

system. The method of pulse oximetry requires pulsatile blood volume changes in order to make a measurement. Since venous blood is not pulsatile, pulse oximetry cannot provide any information about venous blood.

Near-infrared spectroscopy (NIRS) is an optical spectrophotometric method of continually monitoring tissue oxygenation that does not require pulsatile blood volume to calculate parameters of clinical value. The NIRS method is based on the principle that light in the near-infrared range (700 to 1,000 nm) can pass easily through skin, bone and other tissues where it encounters hemoglobin located mainly within micro-circulation passages; e.g., capillaries, arterioles, and venuoles. Hemoglobin exposed to light in the near infra-red range has specific absorption spectra that varies depending on its oxidation state; i.e., oxyhemoglobin (HbO₂) and deoxyhemoglobin (Hb) each act as a distinct chromophore. By using light sources that transmit near-infrared light at specific different wavelengths, and measuring changes in transmitted or reflected light attenuation, concentration changes of the oxyhemoglobin (HbO₂) and deoxyhemoglobin (Hb) can be monitored. The ability to continually monitor cerebral oxygenation levels is particularly valuable for those patients subject to a condition in which oxygenation levels in the brain may be compromised, leading to brain damage or death.

The apparatus used in NIRS analysis typically includes a plurality of light sources, one or more light detectors for detecting reflected or transmitted light, and a processor for processing signals that represent the light emanating from the light source and the light detected by the light detector. Light sources such as light emitting diodes (LEDs) or laser diodes that produce light emissions in the wavelength range of 700–1000 nm at an intensity below that which would damage the biological tissue being examined are typically used. A photodiode or other light source detector is used to detect light reflected from or passed through the tissue being examined. The processor takes the signals from the light sources and the light detector and analyzes those signals in terms of their intensity and wave properties.

It is known that relative changes of the concentrations of HbO₂ and Hb can be evaluated using apparatus similar to that described above, including a processor programmed to utilize a variant of the Beer-Lambert Law, which accounts for optical attenuation in a highly scattering medium like biological tissue. The modified Beer-Lambert Law can be expressed as:

$$A_\lambda = -\log(I/I_0)_\lambda = \alpha_\lambda * C * d * B_\lambda + G \quad (\text{Eqn.2})$$

wherein “A_λ” represents the optical attenuation in tissue at a particular wavelength λ (units: optical density or OD); “I₀” represents the incident light intensity (units: W/cm²); “I” represents the detected light intensity; “α_λ” represents the wavelength dependent absorption coefficient of the chromophore (units: OD*cm⁻¹*μM⁻¹); “C” represents the concentration of chromophore (units: μM); “d” represents the light source to detector (optode) separation distance (units: cm); “B_λ” represents the wavelength dependent light scattering differential pathlength factor (unitless); and “G” represents light attenuation due to scattering within tissue (units: OD). The product of “d*B_λ” represents the effective pathlength of photon traveling through the tissue.

Absolute measurement of chromophore concentration (C) is very difficult because G is unknown or difficult to ascertain. However, over a reasonable measuring period of several hours to days, G can be considered to remain constant, thereby allowing for the measurement of relative changes of

chromophore from a zero reference baseline. Thus, if time t_1 marks the start of an optical measurement (i.e., a base line) and time t_2 is an arbitrary point in time after t_1 , a change in attenuation (ΔA) between t_1 and t_2 can be calculated, and variables G and I_o will cancel out providing that they remain constant.

The change in chromophore concentration ($\Delta C=C(t_2)-C(t_1)$) can be determined from the change in attenuation ΔA , for example using the following equation derived from the modified Beer-Lambert Law:

$$\Delta A_{\lambda} = -\log(I_2/I_1)_{\lambda} = \alpha_{\lambda} * \Delta C * d * B_{\lambda} \quad (\text{Eqn.3})$$

Presently known NIRS algorithms that are designed to calculate the relative change in concentration of more than one chromophore use a multivariate form of Equation 2 or 3. To distinguish between, and to compute relative concentration changes in, oxyhemoglobin (ΔHbO_2) and deoxyhemoglobin (ΔHb), a minimum of two different wavelengths are typically used. The concentration of the HbO_2 and Hb within the examined tissue is determined in $\mu\text{moles per liter}$ of tissue (μM).

The above-described NIRS approach to determining oxygenation levels is useful, but it is limited in that it only provides information regarding a change in the level of oxygenation within the tissue. It does not provide a means for determining the absolute value of oxygen saturation within the biological tissue.

At present, information regarding the relative contributions of venous and arterial blood within tissue examined by NIRS is either arbitrarily chosen or is determined by invasive sampling of the blood as a process independent from the NIRS examination. For example, It has been estimated that NIRS examined brain tissue comprising about 60 to 80% blood venous and about 20 to 40% arterial blood. Blood samples from catheters placed in venous drainage sites such as the internal jugular vein, jugular bulb, or sagittal sinus have been used to evaluate NIRS measurements. Results from animal studies have shown that NIRS interrogated tissue consists of a mixed vascular bed with a venous-to-arterial ratio of about 2:1 as determined from multiple linear regression analysis of sagittal sinus oxygen saturation ($SssO_2$) and arterial oxygen saturation (SaO_2). An expression representing the mixed venous/arterial oxygen saturation ($SmvO_2$) in NIRS examined tissue is shown by the equation:

$$SmvO_2 = K_v * SvO_2 + K_a * SaO_2 \quad (\text{Eqn.4})$$

where " SvO_2 " represents venous oxygen saturation; " SaO_2 " represents arterial oxygen saturation; and K_v and K_a are the weighted venous and arterial contributions respectively, with $K_v + K_a = 1$. The parameters K_v and K_a may have constant values, or they may be a function of SvO_2 and SaO_2 . Determined oxygen saturation from the internal jugular vein ($SjvO_2$), jugular bulb ($SjbO_2$), or sagittal sinus ($SssO_2$) can be used to represent SvO_2 . Therefore, the value of each term in Equation 4 is empirically determined, typically by discretely sampling or continuously monitoring and subsequently evaluating patient arterial and venous blood from tissue that the NIRS sensor is examining, and using regression analysis to determine the relative contributions of venous and arterial blood independent of the NIRS examination.

To non-invasively determine oxygen saturation within tissue at certain depth, it is necessary to limit the influence from the superficial tissues. For example, to determine brain oxygen saturation of adult human with NIRS technology, the

contamination from extracranial tissue (scalp and skull) must be eliminated or limited.

What is needed, therefore, is a method for non-invasively determining the level of oxygen saturation within biological tissue that can determine the absolute oxygen saturation value rather than a change in level; a method that provides calibration means to account for energy losses (i.e. light attenuation) due to light scattering within tissue, other background absorption losses from biological compounds, and other unknown losses including measuring apparatus variability; and a method that can non-invasively determine oxygen saturation within tissue at certain depth by limiting the influence from the superficial tissues.

DISCLOSURE OF THE INVENTION

It is, therefore, an object of the present invention to provide a method for non-invasively determining the absolute oxygen saturation value within biological tissue.

It is a further object of the present invention to provide a method that provides calibration means to account for energy losses due to scattering as well as other background absorption from biological compounds.

It is a still further object of the present invention to provide a method that can non-invasively determine oxygen saturation within tissue at certain depth that limits the influence from the superficial tissues.

According to the present invention, a method and apparatus for non-invasively determining the blood oxygen saturation level within a subject's tissue is provided that utilizes a near infrared spectrophotometric (NIRS) sensor capable of transmitting a light signal into the tissue of a subject and sensing the light signal once it has passed through the tissue via transmittance or reflectance. The method includes the steps of: (1) transmitting a light signal into the subject's tissue, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength; (2) sensing a first intensity and a second intensity of the light signal, along the first, second, and third wavelengths after the light signal travels through the subject at a first and second predetermined distance; (3) determining an attenuation of the light signal for each of the first, second, and third wavelengths using the sensed first intensity and sensed second intensity of the first, second, and third wavelengths; (4) determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength; and (5) determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength.

The present method makes it possible to account for energy losses (i.e. light attenuation) due to light scattering within tissue, other background absorption losses from biological compounds, and other unknown losses including measuring apparatus variability. By determining differential attenuation as a function of wavelength, the energy losses due to scattering as well as other background absorption from biological compounds are cancelled out or minimized relative to the attenuation attributable to deoxyhemoglobin, and attenuation attributable to oxyhemoglobin.

In order to account for the resulting minimized differential attenuation attributable to tissue light scattering characteristics, fixed light absorbing components, and measuring apparatus characteristics, each of the parameters must be measured or calibrated out. Since direct measurement is

difficult, calibration to empirically determined data combined with data developed using the NIRS sensor is performed by using regression techniques. The empirically determined data is collected at or about the same time the data is developed with the NIRS sensor. Once the calibration parameters associated with attenuation attributable to tissue light scattering characteristics, fixed light absorbing components, and measuring apparatus characteristics have been determined, the NIRS sensor can be calibrated.

The calibrated sensor can then be used to accurately and non-invasively determine the total oxygen saturation level in the original subject tissue or other subject tissue. In addition, if effective pathlength of photon traveling through the tissue is known, for example, the separation distance (“d”) between the light source to the light detector is known or is determinable, and the value of “ B_λ ”, which represents the wavelength dependent light scattering differential pathlength factor, then the total amount of concentrations of deoxyhemoglobin (Hb) and oxyhemoglobin (HbO₂) within the examined tissue can be determined using the present method and apparatus.

The calibrated sensor can be used subsequently to calibrate similar sensors without having to invasively produce a blood sample. Hence, the present method and apparatus enables a non-invasive determination of the blood oxygen saturation level within tissue. For example, an operator can create reference values by sensing a light signal or other reference medium using the calibrated sensor. The operator can then calibrate an uncalibrated sensor by sensing the same light signal or reference medium, and subsequently adjusting the uncalibrated sensor into agreement with the calibrated sensor. Hence, once a reference sensor is created, other similar sensors can be calibrated without the need for invasive procedure.

There are, therefore, several advantages provided by the present method and apparatus. Those advantages include: 1) a practical non-invasive method and apparatus for determining oxygen saturation within tissue that can be used to determine the total blood oxygen saturation within tissue as opposed to a change in blood oxygen saturation; 2) a calibration method that accounts for energy losses (e.g., light attenuation) due to light scattering within tissue, other background absorption losses from biological compounds, and other unknown losses including measuring apparatus variability; 3) a practical non-invasive method and apparatus for determining oxygen saturation within tissue that can distinguish between the contribution of oxygen saturation attributable to venous blood and that saturation attributable to arterial blood; and 4) a practical non-invasive method and apparatus for determining oxygen saturation within tissue at certain depth that limits the influence from the superficial tissues.

In an alternative embodiment, aspects of the above-described methodology are combined with pulse oximetry techniques to provide a noninvasive method of distinguishing between blood oxygen saturation within tissue that is attributable to venous blood and that which is attributable to arterial blood. Pulse oximetry is used to determine arterial oxygen saturation, and the arterial oxygen saturation is, in turn, used to determine the venous oxygen saturation.

These and other objects, features, and advantages of the present invention method and apparatus will become apparent in light of the detailed description of the invention provided below and the accompanying drawings. The methodology and apparatus described below constitute a preferred embodiment of the underlying invention and do not, therefore, constitute all aspects of the invention that will or

may become apparent by one of skill in the art after consideration of the invention disclosed overall herein.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a diagrammatic representation of a NIRS sensor. FIG. 2 is a diagrammatic representation of a NIRS sensor placed on a subject’s head.

FIG. 3 is a diagrammatic view of a NIRS sensor.

FIG. 4 is a block diagram of the present methodology for calibrating a NIRS sensor.

FIG. 5 is a graph showing an exemplary plot of absorption coefficient vs. wavelength.

DETAILED DESCRIPTION THE INVENTION

The present method of and apparatus for non-invasively determining the blood oxygen saturation level within a subject’s tissue is provided that utilizes a near infrared spectrophotometric (NIRS) sensor that includes a transducer capable of transmitting a light signal into the tissue of a subject and sensing the light signal once it has passed through the tissue via transmittance or reflectance. The present method and apparatus can be used with a variety of NIRS sensors. The present method is not limited to use with this preferred NIRS sensor, however.

Referring to FIGS. 1–5, the preferred NIRS sensor includes a transducer portion 10 and processor portion 12. The transducer portion 10 includes an assembly housing 14 and a connector housing 16. The assembly housing 14, which is a flexible structure that can be attached directly to a subject’s body, includes one or more light sources 18 and light detectors 19, 20. A disposable adhesive envelope or pad is used for mounting the assembly housing 14 easily and securely to the subject’s skin. Light signals of known but different wavelengths from the light sources 18 emit through a prism assembly 22. The light sources 18 are preferably laser diodes that emit light at a narrow spectral bandwidth at predetermined wavelengths. In one embodiment, the laser diodes are mounted within the connector housing 16. The laser diodes are optically interfaced with a fiber optic light guide to the prism assembly 22 that is disposed within the assembly housing 14. In a second embodiment, the light sources 18 are mounted within the assembly housing 14. A first connector cable 26 connects the assembly housing 14 to the connector housing 16 and a second connector cable 28 connects the connector housing 16 to the processor portion 12. The light detector 20 includes one or more photodiodes. The photodiodes are also operably connected to the processor portion 12 via the first and second connector cables 26, 28. The processor portion 12 includes a processor for processing light intensity signals from the light sources 18 and the light detectors 19, 20.

The processor utilizes an algorithm that characterizes a change in attenuation as a function of the difference in attenuation between different wavelengths. The present method advantageously accounts for but minimizes the effects of pathlength and parameter “E”, which represent energy losses (i.e. light attenuation) due to light scattering within tissue (G), other background absorption losses from biological compounds (F), and other unknown losses including measuring apparatus variability (N). $E=G+F+N$.

Refer to FIG. 1, the absorption $A_{b,\lambda}$ detected from the deep light detector 20 comprises attenuation and energy loss from both the deep and shallow tissue, while the absorption $A_{s,\lambda}$ detected from the shallow light detector 19 comprises attenuation and energy loss from shallow tissue only.

Absorptions $A_{b\lambda}$ and $A_{x\lambda}$ can be expressed in the form of Equation 5 and Equation 6 below which is a modified version of Equation 2 that accounts for energy losses due to "E":

$$A_{b\lambda} = -\log(I_b/I_o)_\lambda = \alpha_\lambda * C_b * L_b + \alpha_\lambda * C_x * L_x + E_\lambda \quad (\text{Eqn.5})$$

$$A_{x\lambda} = -\log(I_x/I_o)_\lambda = \alpha_\lambda * C_x * L_x + E_{x\lambda} \quad (\text{Eqn.6})$$

Substituting Equation 6, into Equation 5 yields A'_λ , which represents attenuation and energy loss from deep tissue only:

$$A'_\lambda = A_{b\lambda} - A_{x\lambda} = \alpha_\lambda * C_b * L_b + (E_\lambda - E_{x\lambda}) = -\log\left(\frac{I_b}{I_x}\right)_\lambda \quad (\text{Eqn. 7})$$

Where L is the effective pathlength of the photon traveling through the deep tissue and A'_1 and A'_2 are the absorptions of two different wavelengths. Let $E'_\lambda = E_\lambda - E_{x\lambda}$, therefore:

$$A'_1 - A'_2 = \Delta A'_{12} \quad (\text{Eqn.8})$$

Substituting Equation 7 into Equation 8 for A'_1 and A'_2 , $\Delta A'_{12}$ can be expressed as:

$$\Delta A'_{12} = \alpha_{\lambda 12} * C_b * L_b + \Delta E'_{12} \quad (\text{Eqn.9})$$

and rewritten Equation 9 in expanded form:

$$\begin{aligned} \Delta A'_{12} &= (\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b L_b + (E'_1 - E'_2) \quad (\text{Eqn. 10}) \\ &= (\Delta\alpha_{r12} * [Hb]_b * L_b) + (\Delta\alpha_{o12} * [HbO_2]_b * L_b) + \Delta E'_{12} \end{aligned}$$

where:

$(\Delta\alpha_{r12} * [Hb]_b * L_b)$ represents the attenuation attributable to Hb;

$(\Delta\alpha_{o12} * [HbO_2]_b * L_b)$ represents the attenuation attributable to HbO₂; and

$\Delta E'_{12}$ represents energy losses (i.e. light attenuation) due to light scattering within tissue, other background absorption losses from biological compounds, and other unknown losses including measuring apparatus variability.

The multivariate form of Equation 10 is used to determine $[HbO_2]_b$ and $[Hb]_b$ with three different wavelengths:

$$\begin{bmatrix} \Delta A'_{12} - \Delta E'_{12} \\ \Delta A'_{13} - \Delta E'_{13} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} \Delta\alpha_{r12} & \Delta\alpha_{o12} \\ \Delta\alpha_{r13} & \Delta\alpha_{o13} \end{bmatrix} \begin{bmatrix} [Hb]_b \\ [HbO_2]_b \end{bmatrix} \quad (\text{Eqn. 11})$$

Rearranging and solving for $[HbO_2]_b$ and $[Hb]_b$, simplifying the $\Delta\alpha$ matrix into $[\Delta\alpha']$:

$$\begin{bmatrix} \Delta A'_{12} \\ \Delta A'_{13} \end{bmatrix} [\Delta\alpha']^{-1} (L_b)^{-1} - \begin{bmatrix} \Delta E'_{12} \\ \Delta E'_{13} \end{bmatrix} [\Delta\alpha']^{-1} (L_b)^{-1} = \begin{bmatrix} [Hb]_b \\ [HbO_2]_b \end{bmatrix} \quad (\text{Eqn. 12})$$

Then combined matrices $[\Delta A']$ $[\Delta\alpha']^{-1} = [A_c]$ and $[\Delta E']$ $[\Delta\alpha']^{-1} = [\Psi_c]$:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} [Hb]_b \\ [HbO_2]_b \end{bmatrix} \quad (\text{Eqn. 13})$$

The parameters A_{Hb} and A_{HbO_2} represent the product of the matrices $[(\Delta A_\lambda)]$ and $[\Delta\alpha']^{-1}$ and the parameters Ψ_{Hb} and Ψ_{HbO_2} represent the product of the matrices $[\Delta E'_\lambda]$ and $[\Delta\alpha']^{-1}$. To determine the level of cerebral blood oxygen saturation (SnO₂), Equation 13 is rearranged using the form of Equation 1 and is expressed as follows:

$$SnO_2 \% = \frac{(A_{HbO_2} - \Psi_{HbO_2})}{(A_{HbO_2} - \Psi_{HbO_2} + A_{Hb} - \Psi_{Hb})} * 100\% \quad (\text{Eqn. 14})$$

Note that the effective pathlength L_b cancels out in the manipulation from Equation 13 to Equation 14.

The value for SnO₂ is initially determined from SmvO₂ using Equation 4 and the empirically determined values for SvO₂ and SaO₂. The empirically determined values for SvO₂ and SaO₂ are based on data developed by discrete sampling or continuous monitoring of the subject's blood performed at or about the same time as the sensing of the tissue with the sensor. The temporal and physical proximity of the NIRS sensing and the development of the empirical data helps assure accuracy. The initial values for Kv and Ka within Equation 4 are clinically reasonable values for the circumstances at hand. The values for A_{HbO_2} and A_{Hb} are determined mathematically using the values for $I_{b\lambda}$ and $I_{x\lambda}$ for each wavelength sensed with the NIRS sensor (e.g., using Equation 5 and 6). The calibration parameters Ψ_{Hb} and Ψ_{HbO_2} , which account for energy losses due to scattering as well as other background absorption from biological compounds, are then determined using Equation 14 and non-linear regression techniques by correlation to different weighted values of SvO₂ and SaO₂; i.e., different values of Ka and Kv. Statistically acceptable values of Kv and Ka and Ψ_{Hb} and Ψ_{HbO_2} are converged upon using the non-linear regression techniques. Experimental findings show that after proper selection of Ka and Kv, the calibration parameters Ψ_{Hb} and Ψ_{HbO_2} are constant within a statistically acceptable margin of error for an individual NIRS sensor used to monitor brain oxygenation on different human subjects. In other words, once the sensor is calibrated it can be used on various human subjects and produce accurate information for each human subject. The same is true for animal subjects.

In an alternative method of determining the absolute oxygen saturation value Equation 7 is rewritten:

$$A'_\lambda - E'_\lambda = \quad (\text{Eqn. 15})$$

$$-\log\left(\frac{I_b}{I_x}\right)_\lambda - E'_\lambda = \alpha_\lambda * C * L_b = (\alpha_{r\lambda} [Hb]_b + \alpha_{o\lambda} [HbO_2]_b) L_b$$

For a two wavelength system, let "R" be a calibration index parameter:

$$R = \frac{A'_1 - E'_1}{A'_2 - E'_2} = \frac{(\alpha_{r1} [Hb]_b + \alpha_{o1} [HbO_2]_b) L_b}{(\alpha_{r2} [Hb]_b + \alpha_{o2} [HbO_2]_b) L_b} \quad (\text{Eqn. 16})$$

-continued

$$\frac{\alpha_{r1} + \alpha_{o1} \frac{[HbO_2]_b}{[Hb]_b}}{\alpha_{r2} + \alpha_{o2} \frac{[HbO_2]_b}{[Hb]_b}} = \frac{\alpha_{r1} + \alpha_{o1} \frac{SnO_2}{1 - SnO_2}}{\alpha_{r2} + \alpha_{o2} \frac{SnO_2}{1 - SnO_2}}$$

Canceling out L_b and substituting:

$$\frac{[HbO_2]_b}{[Hb]_b} = \frac{SnO_2}{1 - SnO_2} \text{ form } SnO_2 = \frac{[HbO_2]_b}{[HbO_2]_b + [Hb]_b}$$

the following expression for SnO_2 is obtained:

$$SnO_2 = \frac{\alpha_{r1} - \alpha_{r2}R}{(\alpha_{r1} - \alpha_{o1}) + (\alpha_{r2} - \alpha_{r2}R)} \quad (\text{Eqn. 17})$$

The value of A_1' and A_2' are determined by measuring I_b and I_x for each wavelength. The parameters E'_1 and E'_2 can be considered as empirically determined calibration coefficients derived from the “best-fit” combinations of the weighted ratios of venous and arterial blood-oxygen saturation of the brain. By using non-linear regression techniques, the values of E'_1 and E'_2 are determined by correlating to different combinations of venous and arterial oxygen saturation weighted values to find the “best-fit” relationship of “R” as a function of A_1' , A_2' , E'_1 and E'_2 (Equation 17) to a specific ratio of venous and arterial saturation weighted values.

In the determination of the SnO_2 percentage, the effective photon pathlength L_b cancels out. If, however, the photon pathlength is known or estimated, then the determination of the total value of Hb and/or HbO_2 is possible. For example, if a value for pathlength L_b is input into Equation 13 along with the calibration values Ψ_{Hb} and Ψ_{HbO_2} , then the total value of Hb and/or HbO_2 can be calculated. According to Equation 2, pathlength L can be estimated from the product of “B*d”. The light source to detector separation (optode) distance parameter “d” in the pathlength calculation is a measurable value and can be made constant by setting a fixed distance between light source to detector in the NIRS sensor design. Alternatively, the parameter “d” can be measured once the optodes are placed on the subject by use of calipers, ruler, or other distance measurement means. The pathlength differential factor “B” is more difficult LU measure and requires more sophisticated equipment. From a large data set of measured neonatal and adult head differential pathlength factor values, an estimation of the value of “B” can be determined within a statistically acceptable margin of error. Substitution of these predetermined values of “B” into Equation 13 results in the determination of the total values of Hb and HbO_2 .

An alternative method of determining total values of Hb and HbO_2 combines Equation 3 and Equation 13 together. The multivariate form of Equation 3 is shown below:

$$5 \quad \begin{bmatrix} -\log(I_{t2}/I_{t1})_{\lambda 1} / L_{\lambda 1} \\ -\log(I_{t2}/I_{t1})_{\lambda 2} / L_{\lambda 2} \\ -\log(I_{t2}/I_{t1})_{\lambda 3} / L_{\lambda 3} \end{bmatrix} = \begin{bmatrix} \alpha_{Hb\lambda 1} & \alpha_{HbO_2\lambda 1} \\ \alpha_{Hb\lambda 2} & \alpha_{HbO_2\lambda 2} \\ \alpha_{Hb\lambda 3} & \alpha_{HbO_2\lambda 3} \end{bmatrix} * \begin{bmatrix} \Delta Hb \\ \Delta HbO_2 \end{bmatrix} \quad (\text{Eqn. 18})$$

At time $t=t_1$, the values of ΔHb and ΔHbO_2 are zero. Applying Equation 13, and knowing the calibration values of Ψ_{Hb} and Ψ_{HbO_2} at a predetermined differential pathlength factor “B” and optode separation “d”, the total absolute values of Hb and HbO_2 are determined at time $t=t_1$, which are represented by $[Hb]_{t1}$ and $[HbO_2]_{t1}$ respectively. At time $t=t_2$, the values of ΔHb and ΔHbO_2 are then determined using Equation 18. The total values of Hb and HbO_2 are then determined at time $t=t_2$ using the following equations:

$$[Hb]_{t2} = \Delta Hb(t_2) + [Hb]_{t1} \quad (\text{Eqn.19})$$

$$[HbO_2]_{t2} = \Delta HbO_2(t_2) + [HbO_2]_{t1} \quad (\text{Eqn.20})$$

Equations 19 and 20 are valid only if all the shared parameters in Equations 13 and 18 are exact. Reduced to practice, the advantage of combining Equations 13 and 18 result in improved signal to noise ratio (SNR) in the calculation of the total values for Hb and HbO_2 . Conversely, improved SNR in the calculation of SnO_2 is also obtained from the following expression:

$$SnO_2 \% = \frac{HbO_2}{HbO_2 + Hb} * 100\% \quad (\text{Eqn. 21})$$

After the calibration parameters Ψ_{Hb} and Ψ_{HbO_2} are determined using the above-described methodology for an individual NIRS sensor, this particular sensor is said to be calibrated. A calibrated NIRS sensor affords accurate measurement of total tissue oxygen saturation, SnO_2 , by non-invasive means. The calibrated sensor can be used thereafter on any human patient, including adults and neonates. The same is true for animal subject if the sensor was calibrated on animals. Although the present method is described above in terms of sensing blood oxygenation within cerebral tissue, the present method and apparatus are not limited to cerebral applications and can be used to determine blood oxygenation within tissue found elsewhere within the subject’s body.

According to an additional aspect of the present invention, the above-described method can also be used to establish a calibrated “reference” sensor that can be used to calibrate similar sensors through the use of a phantom sample (also referred to as a “reference sample”). The phantom sample has optical characteristics that are similar to the tissue being examined by the NIRS sensor. The calibrated reference NIRS sensor is used to sense the phantom sample and produce reference values. Similar, but uncalibrated, NIRS sensors can thereafter be calibrated by sensing the same phantom sample and adjusting either the hardware of the uncalibrated sensor or the output of the uncalibrated sensor until the output of the uncalibrated sensor agrees with the reference values produced by the calibrated reference sensor. Therefore, the calibration parameters Ψ_{Hb} and Ψ_{HbO_2} for the uncalibrated sensor would be determined from the phantom sample. This technique makes it unnecessary to calibrate each new sensor in the manner described above,

and thereby provides a relatively quick and cost effective way to calibrate NIRS sensors.

Besides Hb and HbO₂, other biological constituents of interest (e.g., cytochrome aa₃, etc.) could be determined using the multivariate forms of equations 2, 3, 6 or 7. For each additional constituent to be determined, an additional measuring wavelength will be needed.

In an alternative embodiment, the above-described methodology can be combined with pulse oximetry techniques to provide an alternative noninvasive method of distinguishing between oxygen saturation attributable to venous blood and that attributable to arterial blood. As demonstrated by Equation 4, SmvO₂ is determined by the ratio of venous oxygen saturation SvO₂ and arterial oxygen saturation SaO₂. A calibrated NIRS sensor affords accurate measurement of total tissue oxygen saturation, SnO₂, by using regression techniques by correlation to mixed venous oxygen saturation SmvO₂. Therefore, the following expression will result:

$$SnO_2 = SmvO_2 = K_v * SvO_2 + K_a * SaO_2 \quad (\text{Eqn. 22})$$

Non-invasive pulse oximetry techniques can be used to determine the arterial oxygen saturation (SaO₂) of peripheral tissue (i.e. finger, ear, nose) by monitoring pulsatile optical attenuation changes of detected light induced by pulsatile arterial blood volume changes in the arteriolar vascular system. Arterial blood oxygen saturation determined by pulse oximetry is clinically denoted as SpO₂. If NIRS monitoring and pulse oximetry monitoring are done simultaneously and SpO₂ is set equal to SaO₂ in Equation 23, then venous oxygen saturation can be determined from the following expression:

$$SvO_2 = \frac{SnO_2 - (K_a * SpO_2)}{K_v} \quad (\text{Eqn. 23})$$

For the brain, venous oxygen saturation SvO₂ would be determined from internal jugular vein (SijvO₂), jugular bulb (SjbO₂), or sagittal sinus (SssO₂) and the parameters Ka and Kv would be empirically determined during the calibration of the NIRS sensor. Under most physiological conditions, SpO₂ is representative of brain arterial oxygen saturation SaO₂. Therefore, depending on which venous saturation parameter was used to calibrate the NIRS sensor, this clinically important parameter (i.e., SijvO₂, SjbO₂, or SssO₂) can be determined by Equation 24 by non-invasive means.

Since many changes and variations of the disclosed embodiment of the invention may be made without departing from the inventive concept, it is not intended to limit the invention otherwise than as required by the appended claims.

The invention claimed is:

1. A method for non-invasively determining a blood oxygen saturation level within a subject's tissue using a near infrared spectrophotometric sensor, said method comprising the steps of:

transmitting a light signal into the subject's tissue using the sensor, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a first intensity and a second intensity of the light signal, using the sensor, along the first, second, and third wavelengths after the light signal travels through

the subject at a first predetermined distance and a second predetermined distance;

wherein the sensor is calibrated using empirical data that relates to the subject's tissue that is sensed by the sensor to account for light signal attenuation resulting from light signal scattering within the subject's tissue; determining an attenuation of the light signal for each of the first, second, and third wavelengths using the sensed first intensity and sensed second intensity of the first, second, and third wavelengths;

determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength;

determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength.

2. The method of claim 1, wherein the sensor is calibrated using the equation:

$$SmvO_2 = K_v * SvO_2 + K_a * SaO_2.$$

3. The method of claim 2, wherein the sensor is calibrated by using empirical data to determine a first calibration constant and a second calibration constant.

4. The method of claim 3, wherein the step of determining the blood oxygen saturation level within the subject's tissue utilizes the equation:

$$SnO_2 \% = \frac{(A_{HbO_2} - \Psi_{HbO_2})}{(A_{HbO_2} - \Psi_{HbO_2} + A_{Hb} - \Psi_{Hb})} * 100 \%$$

where Ψ_{HbO_2} represents the first calibration constant, Ψ_{Hb} represents the second calibration constant, A_{HbO_2} represents a difference in attenuation of light signal attributable to oxyhemoglobin, and A_{Hb} represents a difference in attenuation of light signal attributable to deoxyhemoglobin.

5. The method of claim 4, further comprising the steps of: determining a photon pathlength L_b ; and

determining a concentration of oxyhemoglobin and a concentration of deoxyhemoglobin within the subject's tissue using the first and second calibration constants.

6. The method of claim 5, wherein the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue are determined using the equation:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} [Hb]_b \\ [HbO_2]_b \end{bmatrix}.$$

7. The method of claim 6, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{12} &= A'_1 - A'_2 = -\log(I_b / I_s)_1 + \log(I_b / I_s)_2 \\ &= \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) \\ &= (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned}$$

13

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} &= A'_1 - A'_3 = -\log(I_b / I_x)_1 + \log(I_b / I_x)_3 \\ &= \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) \\ &= (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned}$$

8. The method of claim 7, wherein the step of determining an attenuation of the light signal utilizes the equation:

$$\begin{aligned} A'_\lambda &= -\log(I_b / I_x)_\lambda = (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + E'_\lambda \\ &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda \end{aligned}$$

for one or more of the first, second, and third wavelengths.

9. The method of claim 1, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{12} &= A'_1 - A'_2 = -\log(I_b / I_x)_1 + \log(I_b / I_x)_2 \\ &= \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) \\ &= (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned}$$

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} &= A'_1 - A'_3 = -\log(I_b / I_x)_1 + \log(I_b / I_x)_3 \\ &= \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) \\ &= (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned}$$

10. The method of claim 9, wherein the step of determining an attenuation of the light signal of a wavelength λ utilizes the equation:

$$\begin{aligned} A'_\lambda &= -\log(I_b / I_x)_\lambda = (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L'_b + E'_\lambda \\ &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda. \end{aligned}$$

11. A method for determining a blood oxygen saturation level within a subject's tissue using a near infrared spectrophotometric sensor attached to the skin of the subject, said method comprising the steps of:

transmitting a light signal into the subject's tissue, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a first intensity and a second intensity of the light signal, using the sensor, along the first, second, and third wavelengths after the light signal travels through the subject at a first predetermined distance and a second predetermined distance;

14

determining an attenuation of the light signal for each of the first, second, and third wavelengths using the first intensity and the sensed second intensity of the first, second, and third wavelengths;

5 determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength;

10 determining a first calibration constant and a second calibration constant using empirical data developed from the subject at or about the same time as when the sensing occurs;

determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength, and the first calibration constant and the second calibration constant.

20 12. The method of claim 11 wherein the empirical data is collected by discretely sampling a venous blood source and an arterial blood source from the subject.

13. The method of claim 11 wherein the empirical data is collected by continuously monitoring a venous blood source and an arterial blood source from the subject.

14. The method of claim 11, wherein the sensor is calibrated using the equation:

$$SmvO_2 = Kv * SvO_2 + Ka * SaO_2.$$

15. The method of claim 14, wherein the step of determining the blood oxygen saturation level within the subject's tissue utilizes the equation:

$$SnO_2\% = \frac{(A_{HbO_2} - \Psi_{HbO_2})}{(A_{HbO_2} - \Psi_{HbO_2} + A_{Hb} - \Psi_{Hb})} * 100\%$$

where Ψ_{HbO_2} represents the first calibration constant, Ψ_{Hb} represents the second calibration constant, A_{HbO_2} represents a difference in attenuation of light signal attributable to oxyhemoglobin, and A_{Hb} represents a difference in attenuation of light signal attributable to deoxyhemoglobin.

16. The method of claim 15, further comprising the steps of:

determining a photon pathlength L_b ; and
determining the concentration of oxyhemoglobin and deoxyhemoglobin within the subject's tissue using the first and second calibration constants.

17. The method of claim 16, wherein the concentration of oxyhemoglobin and deoxyhemoglobin within the subject's tissue are determined using the equation:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} Hb \\ HbO_2 \end{bmatrix}.$$

18. The method of claim 17, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\Delta A'_{12} = A'_1 - A'_2 = -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_2 =$$

-continued

$$\begin{aligned} & \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) = \\ & (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned} \quad 5$$

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} = A'_1 - A'_3 &= -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_3 = \\ & \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) = \\ & (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned} \quad 15$$

19. The method of claim 18, wherein the step of determining an attenuation of the light signal utilizes the equation:

$$\begin{aligned} A'_\lambda = -\log(I_b / I_x)_\lambda &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + E'_\lambda . \\ &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda \end{aligned} \quad 25$$

for one or more of the first, second, and third wavelengths.

20. The method of claim 11, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{12} = A'_1 - A'_2 &= -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_2 = \\ & \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) = \\ & (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned} \quad 40$$

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} = A'_1 - A'_3 &= -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_3 = \\ & \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) = \\ & (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned} \quad 45$$

21. The method of claim 20, wherein the step of determining an attenuation of the light signal utilizes the equation:

$$\begin{aligned} A'_\lambda = -\log(I_b / I_x)_\lambda &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + E'_\lambda . \\ &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda \end{aligned} \quad 55$$

for one or more of the first, second, and third wavelengths.

22. The method of claim 11, wherein the step of determining the blood oxygen saturation level within the subject's tissue utilizes the equation:

$$SnO_2\% = \frac{(A_{HbO_2} - \Psi_{HbO_2})}{(A_{HbO_2} - \Psi_{HbO_2} + A_{Hb} - \Psi_{Hb})} * 100\%$$

where Ψ_{HbO_2} represents the first calibration constant, Ψ_{Hb} represents the second calibration constant, A_{HbO_2} represents a difference in attenuation of light signal attributable to oxyhemoglobin, and A_{Hb} represents a difference in attenuation of light signal attributable to deoxyhemoglobin.

23. The method of claim 22, further comprising the steps of:

determining a photon pathlength L_b , and

determining the concentration of oxyhemoglobin and deoxyhemoglobin within the subject's tissue using the first and second calibration constants.

24. The method of claim 23, wherein the concentration of oxyhemoglobin and deoxyhemoglobin within the subject's tissue are determined using the equation:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} Hb \\ HbO_2 \end{bmatrix}.$$

25. The method of claim 24, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{12} = A'_1 - A'_2 &= -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_2 = \\ & \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) = \\ & (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned} \quad 50$$

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} = A'_1 - A'_3 &= -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_3 = \\ & \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) = \\ & (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned} \quad 55$$

26. The method of claim 25, wherein the step of determining an attenuation of the light signal utilizes the equation:

$$\begin{aligned} A'_\lambda = -\log(I_b / I_x)_\lambda &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + E'_\lambda . \\ &= (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda \end{aligned} \quad 60$$

for one or more of the first, second, and third wavelengths.

27. A method for calibrating a near infrared spectrophotometric sensor for use in determining the blood oxygen saturation level within a subject's tissue, said method comprising the steps of:

transmitting a light signal into the subject's tissue, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a first intensity and a second intensity of the light signal, using the sensor, along the first, second, and third wavelengths after the light signal travels through the subject at a first and second predetermined distances;

determining an attenuation of the light signal for each of the first, second, and third wavelengths using the first intensity and the sensed second intensity of the first, second, and third wavelengths;

determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength;

determining a first calibration constant and a second calibration constant using empirical data developed from the subject at or about the same time as when the sensing occurs; and

calibrating the sensor using the first calibration constant and the second calibration constant.

28. The method of claim 27, wherein the empirical data is collected by discretely sampling a venous blood source and an arterial blood source from the subject.

29. The method of claim 27, wherein the empirical data is collected by continuously monitoring a venous blood source and an arterial blood source from the subject.

30. The method of claim 27, wherein the sensor is calibrated using the equation:

$$SmvO_2 = Kv * SvO_2 + Ka * SaO_2.$$

31. The method of claim 27, wherein the step of determining a difference in attenuation of the light signal between the first wavelength and the second wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{12} = A'_{\lambda 1} - A'_{\lambda 2} = -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_2 = \\ \{(\alpha_{r1} - \alpha_{r2})[Hb]_b + (\alpha_{o1} - \alpha_{o2})[HbO_2]_b\}L_b + (E'_1 - E'_2) = \\ (\Delta\alpha_{r12}[Hb]_b + \Delta\alpha_{o12}[HbO_2]_b)L_b + \Delta E_{12} \end{aligned}$$

and the step of determining a difference in attenuation of the light signal between the first wavelength and the third wavelength utilizes the equation:

$$\begin{aligned} \Delta A'_{13} = A'_{\lambda 1} - A'_{\lambda 3} = -\log\left(\frac{I_b}{I_x}\right)_1 + \log\left(\frac{I_b}{I_x}\right)_3 = \\ \{(\alpha_{r1} - \alpha_{r3})[Hb]_b + (\alpha_{o1} - \alpha_{o3})[HbO_2]_b\}L_b + (E'_1 - E'_3) = \\ (\Delta\alpha_{r13}[Hb]_b + \Delta\alpha_{o13}[HbO_2]_b)L_b + \Delta E_{13}. \end{aligned}$$

32. The method of claim 31, wherein the step of determining an attenuation of the light signal utilizes the equation:

$$\begin{aligned} A'_\lambda = -\log(I_b / I_x)_\lambda = (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + E'_\lambda \\ = (\alpha_{r\lambda}[Hb]_b + \alpha_{o\lambda}[HbO_2]_b)L_b + (E - E_x)_\lambda \end{aligned}$$

for one or more of the first, second, and third wavelengths.

33. A method for calibrating a NIRS sensor, said method comprising the steps of:

transmitting a first light signal from a calibrated NIRS sensor into a reference sample, wherein the transmitted first light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a first intensity and a second intensity of the first light signal with the calibrated NIRS sensor along the first, second, and third wavelengths after the first light signal travels through the reference sample;

determining a first attenuation of the first light signal for each of the first, second, and third wavelengths using the first intensity and the second intensity of the first light signal sensed with the calibrated NIRS sensor;

transmitting a second light signal from an uncalibrated second NIRS sensor into the reference sample at a predetermined first intensity, wherein the transmitted second light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a second intensity of the second light signal with the uncalibrated second NIRS sensor along the first, second, and third wavelengths after the second light signal travels through the subject;

determining a second attenuation of the second light signal for each of the first, second, and third wavelengths using the predetermined first intensity and the second intensity of the first, second, and third wavelengths sensed with the uncalibrated second NIRS sensor;

adjusting the uncalibrated second NIRS sensor so that the second attenuation substantially agrees with the first attenuation.

34. A method for non-invasively determining a concentration of oxyhemoglobin and a concentration of deoxyhemoglobin within a subject's tissue using a near infrared spectrophotometric sensor, said method comprising the steps of:

(a) determining a blood oxygen saturation level with the subject's tissue by

transmitting a light signal into the subject's tissue from a NIRS sensor, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength;

sensing a first intensity and a second intensity of the light signal, using the sensor, along the first, second, and third wavelengths after the light signal travels through the subject at a first and second predetermined distances;

wherein the sensor is calibrated using empirical data that relates to the subject's tissue that is sensed by the sensor to account for light signal attenuation resulting from light signal scattering within the subject's tissue;

determining an attenuation of the light signal for each of the first, second, and third wavelengths using the first intensity and the sensed second intensity of the first, second, and third wavelengths;

determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength;

determining a first calibration constant and a second calibration constant using empirical data developed from the subject at or about the same time as when the sensing occurs;

determining the blood oxygen saturation level within the subject's tissue using the difference in attenua-

tion between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength, and the first calibration constant and the second calibration constant;

- (b) determining a photon pathlength L_b , and
- (c) determining the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue using the first and second calibration constants.

35. The method of claim 34, wherein the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue are determined using the equation:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} Hb \\ HbO_2 \end{bmatrix}$$

where Ψ_{HbO_2} represents the first calibration constant, Ψ_{Hb} represents the second calibration constant, A_{HbO_2} represents a difference in attenuation of light signal attributable to oxyhemoglobin, and A_{Hb} represents a difference in attenuation of light signal attributable to deoxyhemoglobin.

36. A method for non-invasively determining a concentration of oxyhemoglobin and a concentration of deoxyhemoglobin within a subject's tissue at an initial time t_1 and a subsequent time t_2 using a near infrared spectrophotometric sensor, said method comprising the steps of:

- (a) determining a blood oxygen saturation level with the subject's tissue by
 - transmitting a light signal into the subject's tissue from a NIRS sensor, wherein the transmitted light signal includes a first wavelength, a second wavelength, and a third wavelength;
 - sensing a first intensity and a second intensity of the light signal, using the sensor, along the first, second, and third wavelengths after the light signal travels through the subject at a first and second predetermined distances;
 - wherein the sensor is calibrated using empirical data that relates to the subject's tissue that is sensed by the sensor to account for light signal attenuation resulting from light signal scattering within the subject's tissue;
 - determining an attenuation of the light signal for each of the first, second, and third wavelengths using the first intensity and the sensed second intensity of the first, second, and third wavelengths;
 - determining a difference in attenuation of the light signal between the first wavelength and the second wavelength, and between the first wavelength and the third wavelength;
 - determining a first calibration constant and a second calibration constant using empirical data developed from the subject at or about the same time as when the sensing occurs;
 - determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and the second wavelength, and the difference in attenuation between the first wavelength and the third wavelength, and the first calibration constant and the second calibration constant;

- (b) determining a photon pathlength L_b ;
- (c) determining the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue at the initial time t_1 using the equation:

$$\begin{bmatrix} A_{Hb} \\ A_{HbO_2} \end{bmatrix} (L_b)^{-1} - \begin{bmatrix} \Psi_{Hb} \\ \Psi_{HbO_2} \end{bmatrix} (L_b)^{-1} = \begin{bmatrix} Hb \\ HbO_2 \end{bmatrix}$$

where Ψ_{HbO_2} represents the first calibration constant, Ψ_{Hb} represents the second calibration constant, A_{HbO_2} represents a difference in attenuation of light signal attributable to oxyhemoglobin, and A_{Hb} represents a difference in attenuation of light signal attributable to deoxyhemoglobin; and

- (d) determining a change in the concentration of oxyhemoglobin and a change in the concentration of deoxyhemoglobin from the initial time t_1 to a subsequent second time t_2 , determined using the equation:

$$\begin{bmatrix} -\log\left(\frac{I_2}{I_1}\right)_{\lambda_1} / L_{\lambda_1} \\ -\log\left(\frac{I_2}{I_1}\right)_{\lambda_2} / L_{\lambda_2} \\ -\log\left(\frac{I_2}{I_1}\right)_{\lambda_3} / L_{\lambda_3} \end{bmatrix} = \begin{bmatrix} \alpha_{Hb\lambda_1} & \alpha_{HbO_2\lambda_1} \\ \alpha_{Hb\lambda_2} & \alpha_{HbO_2\lambda_2} \\ \alpha_{Hb\lambda_3} & \alpha_{HbO_2\lambda_3} \end{bmatrix} * \begin{bmatrix} \Delta Hb \\ \Delta HbO_2 \end{bmatrix}$$

- ; and
- (e) determining the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue at the subsequent time t_2 using the equations:

$$[Hb]_{t_2} = \Delta Hb(t_2) + [Hb]_{t_1} \text{ and}$$

$$[HbO_2]_{t_2} = \Delta HbO_2(t_2) + [HbO_2]_{t_1}.$$

37. A method for non-invasively determining a blood oxygen saturation level within a subject's tissue using a near infrared spectrophotometric sensor, said method comprising the steps of:

- transmitting a light signal into the subject's tissue using the sensor;
- sensing a first intensity and a second intensity of the light signal, using the sensor, along three or more selectively chosen wavelengths after the light signal travels through the subject at a first and second predetermined distances;
- wherein the sensor is calibrated using empirical data that relates to the subject's tissue that is sensed by the sensor to account for light signal attenuation resulting from light signal scattering within the subject's tissue;
- determining an attenuation of the light signal for at least "n" number of the selectively chosen wavelengths using the first intensity and the sensed second intensity of the selectively chosen wavelengths, where "n" is an integer equal to or greater than three;
- determining a difference in attenuation of the light signal between a first wavelength and each of "n" number of the selectively chosen wavelengths;
- determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and each of the "n" number of other selectively chosen wavelengths.

38. A method for determining a blood oxygen saturation level within a subject's tissue using a near infrared spectrophotometric sensor attached to the skin of the subject, said method comprising the steps of:

- transmitting a light signal into the subject's tissue;
- sensing a first intensity and a second intensity of the light signal, using the sensor, along three or more selectively chosen wavelengths after the light signal travels through the subject at a first and second predetermined distances;
- determining an attenuation of the light signal for at least "n" number of the selectively chosen wavelengths using the first intensity and the sensed second intensity of the selectively chosen wavelengths, where "n" is an integer equal to or greater than three;
- determining a difference in attenuation of the light signal between a first wavelength and each of "n" number of the selectively chosen wavelengths;
- determining a first calibration constant and a second calibration constant using empirical data developed from the subject at or about the same time as when the sensing occurs;
- determining the blood oxygen saturation level within the subject's tissue using the difference in attenuation between the first wavelength and each of "n" number of the selectively chosen wavelengths, and the first calibration constant and the second calibration constant.

39. A method for non-invasively determining a blood oxygen saturation level within a subject's tissue using a near infrared spectrophotometric sensor, said method comprising the steps of:

- transmitting a light signal into the subject's tissue using the sensor, wherein the transmitted light signal includes a first wavelength, and a second wavelength;
- sensing a first intensity and a second intensity of the light signal, using the sensor, along the first wavelength, after the light signal travels through the subject at a first and a second predetermined distances;
- sensing a third intensity and a fourth intensity of the light signal, using the sensor, along the second wavelength, after the light signal travels through the subject at said first and said second predetermined distances;
- wherein the sensor is calibrated using empirical data that relates to the subject's tissue that is sensed by the sensor to account for light signal attenuation resulting from light signal scattering within the subject's tissue;
- determining a first attenuation of the light signal for the first wavelength using said first intensity and said second intensity;
- determining a second attenuation of the light signal for the second wavelength using said third intensity and said fourth intensity;
- determining a ratio of said first and said second attenuations of the light signal for the first, and second wavelengths;
- determining the blood oxygen saturation level within the subject's tissue using said ratio.

40. The method of claim 39, wherein the sensor is calibrated using the equation:

$$S_{mv}O_2 = K_1 * S_1 * O_2 + K_2 * S_2 * O_2.$$

41. The method of claim 40, wherein the sensor is calibrated by using empirical data to determine a first calibration constant and a second calibration constant.

42. The method of claim 41, wherein the step of determining the ratio R of attenuations of the light signal for the first, and second wavelengths utilizes the equation:

$$R = \frac{A'_1 - E'_1}{A'_2 - E'_2}$$

where E₁' represents the first calibration constant, E₂' represents the second calibration constant, A₁' represents the first attenuation of light signal of the first wavelength, and A₂' represents the second attenuation of light signal of the second wavelength.

43. The method of claim 42, wherein the step of determining the first attenuation of the first wavelength utilizes the equation:

$$-\log(I_b/I_x)_1 = (\alpha_{r1}[Hb]_b + \alpha_{o1}[HbO_2]_b)L_b + (E - E_x)_1,$$

and the step of determining the second attenuation of the second wavelength utilizes the equation:

$$-\log(I_b/I_x)_2 = (\alpha_{r2}[Hb]_b + \alpha_{o2}[HbO_2]_b)L_b + (E - E_x)_2.$$

44. The method of claim 40, wherein the step of determining the blood oxygen saturation level within the subject's tissue utilizes the equation:

$$S_{n}O_2 \% = \frac{\alpha_{r1} - \alpha_{r2}R}{(\alpha_{r1} - \alpha_{o1}) + (\alpha_{o2} - \alpha_{r2})R} 100\%$$

where R represents the ratio of attenuations of the light signal for each of the first, and second wavelengths.

45. The method of claim 44, wherein the step of determining the ratio R of attenuations of the light signal for the first, and second wavelengths utilizes the equations:

$$R = \frac{A'_1 - E'_1}{A'_2 - E'_2}$$

where E₁' represents the first calibration constant, E₂' represents the second calibration constant, A₁' represents the first attenuation of light signal of the first wavelength, and A₂' represents the second attenuation of light signal of the second wavelength.

46. The method of claim 45, wherein the step of determining the first attenuation of the first wavelength utilizes the equation:

$$-\log(I_b/I_x)_1 = (\alpha_{r1}[Hb]_b + \alpha_{o1}[HbO_2]_b)L_b + (E - E_x)_1,$$

and the step of determining the second attenuation of the second wavelength utilizes the equation:

$$-\log(I_b/I_x)_2 = (\alpha_{r2}[Hb]_b + \alpha_{o2}[HbO_2]_b)L_b + (E - E_x)_2.$$

47. The method of claim 40, wherein the step of determining the blood oxygen saturation level within the subject's tissue comprising the steps of:

- determining the attenuation ratio R of the light signal for each of the first, and second wavelengths;
- determining the blood oxygen saturation level utilizing an empirical obtained calibration curve defining the relationship between the said attenuation ratio R with blood oxygen saturation.

23

48. The method of claim 47, wherein the step of determining the first attenuation of the first wavelength utilizes the equation:

$$A'_1 = -\log(I_b/I_x)_1 = (\alpha_{r1}[Hb]_b + \alpha_{o1}[HbO_2]_b)L_b + E'_1$$

and the step of determining the second attenuation of the second wavelength utilizes the equation:

$$A'_2 = -\log(I_b/I_x)_2 = (\alpha_{r2}[Hb]_b + \alpha_{o2}[HbO_2]_b)L_b + E'_2$$

49. The method of claim 48, wherein the concentration of oxyhemoglobin and the concentration of deoxyhemoglobin within the subject's tissue are determined using the equation:

24

$$\begin{bmatrix} A'_1 \\ A'_2 \end{bmatrix} \begin{bmatrix} \alpha_{r1} & \alpha_{o1} \\ \alpha_{r2} & \alpha_{o2} \end{bmatrix}^{-1} (L_b)^{-1} - \begin{bmatrix} E'_1 \\ E'_2 \end{bmatrix} \begin{bmatrix} \alpha_{r1} & \alpha_{o1} \\ \alpha_{r2} & \alpha_{o2} \end{bmatrix}^{-1} (L_b)^{-1} = \begin{bmatrix} [Hb]_b \\ [HbO_2]_b \end{bmatrix}$$

5

50. The method of claim 40, further comprising the steps of:

determining a photon pathlength L_b ; and

determining a concentration of oxyhemoglobin and a concentration of deoxyhemoglobin within the subject's tissue using the first and second calibration constants.

10

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 7,072,701 B2
APPLICATION NO. : 10/628068
DATED : July 4, 2006
INVENTOR(S) : Chen et al.

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Column 9, line 56, please delete "pathiength" and insert "pathlength".

Column 11, line 42, please delete "physiological" and insert "physiological."

Signed and Sealed this

Twenty-ninth Day of August, 2006

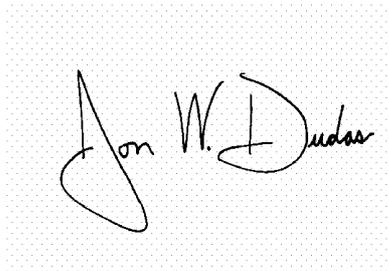A handwritten signature in black ink on a light gray dotted background. The signature reads "Jon W. Dudas" in a cursive style.

JON W. DUDAS

Director of the United States Patent and Trademark Office

专利名称(译)	分光光度法血氧监测方法		
公开(公告)号	US7072701	公开(公告)日	2006-07-04
申请号	US10/628068	申请日	2003-07-24
申请(专利权)人(译)	CAS医疗系统, INC.		
当前申请(专利权)人(译)	CAS医疗系统, INC.		
[标]发明人	CHEN BO BENNI PAUL B		
发明人	CHEN, BO BENNI, PAUL B.		
IPC分类号	A61B5/00 G01N21/17 A61B A61B5/145 A61B5/1455 A61B5/1495 G01N21/35		
CPC分类号	A61B5/14553		
优先权	60/407277 2002-08-30 US 60/398937 2002-07-26 US		
其他公开文献	US20040024297A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于非侵入性地确定受试者组织内的血氧饱和度水平的方法和装置, 其利用近红外分光光度 (NIRS) 传感器, 其能够将光信号传输到受试者的组织中并且一旦感测到光信号就感测到该信号。通过透射率或反射率穿过组织。该方法包括以下步骤: (1) 将光信号传输到受试者组织中, 其中透射光信号包括第一波长, 第二波长和第三波长; (2) 在光信号以第一和第二预定距离通过对象之后, 沿第一, 第二和第三波长感测光信号的第一强度和第二强度; (3) 使用感测到的第一, 第二和第三波长的第一强度和感测的第二强度, 确定第一, 第二和第三波长中的每一个的光信号的衰减; (4) 确定第一波长和第二波长之间以及第一波长和第三波长之间的光信号衰减的差异; (5) 利用第一波长和第二波长之间的衰减差以及第一波长和第三波长之间的衰减差来确定受试者组织内的血氧饱和度。

