





US 20020095093A1

(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2002/0095093 A1**
Au et al. (43) **Pub. Date: Jul. 18, 2002**(54) **HAND-HELD SURFACE ECG AND RF
APPARATUS INCORPORATED WITH A
MEDICAL DEVICE****Related U.S. Application Data**(63) Non-provisional of provisional application No.
60/192,943, filed on Mar. 29, 2000.(76) Inventors: **Nelson Au**, Foster City, CA (US);
Mark Brecht, Imperial Beach, CA
(US); **Marion Buchenau**, San
Francisco, CA (US); **Thomas Crowley**,
Lino Lakes, MN (US); **David**
Karshmer, Menlo Park, CA (US);
Chester G. Nelson, Maple Grove, MN
(US); **Nick Oakley**, Portland, OR (US);
Edwin M. Pearce JR., San Francisco,
CA (US); **Nancy Perry Pool**,
Minnetonka, MN (US); **Richard M.**
Powell, Southport, NC (US); **Elisha**
Tal, (US)**Publication Classification**(51) **Int. Cl.⁷** **A61B 5/0404**
(52) **U.S. Cl.** **600/509**(57) **ABSTRACT**

A hand-holdable structure implementing electrodes to enable good skin-electrode contact to acquire ECG readings is disclosed. Specifically, the structure is shaped to enable patients to apply a simple gentle grip to have a reliable skin-electrode contact and to automatically commence ECG tracing transmission to a patient monitoring station. In one embodiment the structure incorporates an RF telemetry head to simultaneously transfer IMD stored data in conjunction with the ECG tracings. The structure independently or in combination with the RF telemetry head is adaptable to a system of data communications with a programmer or equivalent instrument to transfer ECG and IMD data to a remotely located physician station or patient data storage server. The system is also adaptable for use with a web-enabled network such as, without limitation, the Internet, intranet, World Wide Web, extranet or equivalent.

Correspondence Address:

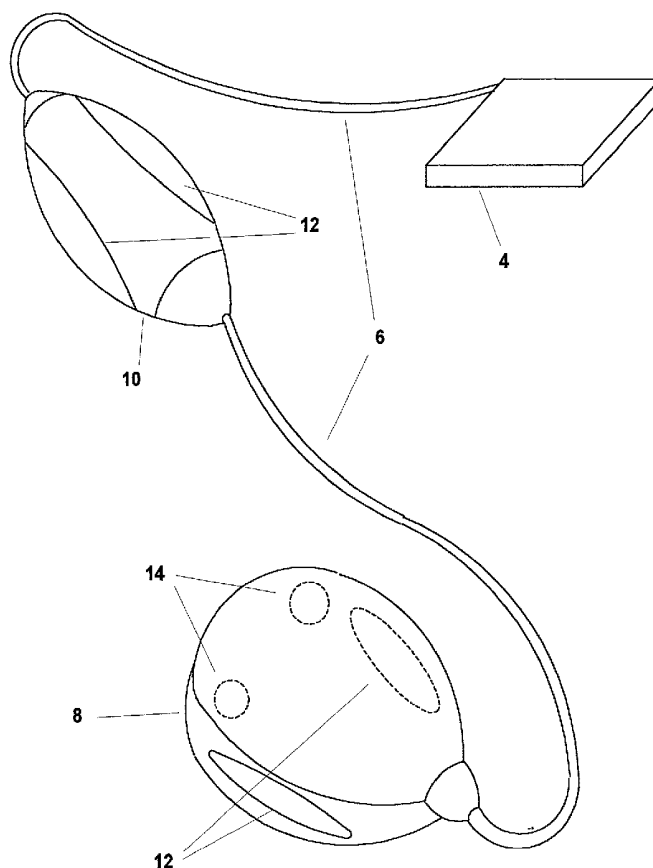Girma Wolde-Michael
MEDTRONIC, INC., MS 301
7000 Central Avenue N.E.
Minneapolis, MN 55432 (US)
(21) Appl. No.: **09/821,201**(22) Filed: **Mar. 29, 2001**

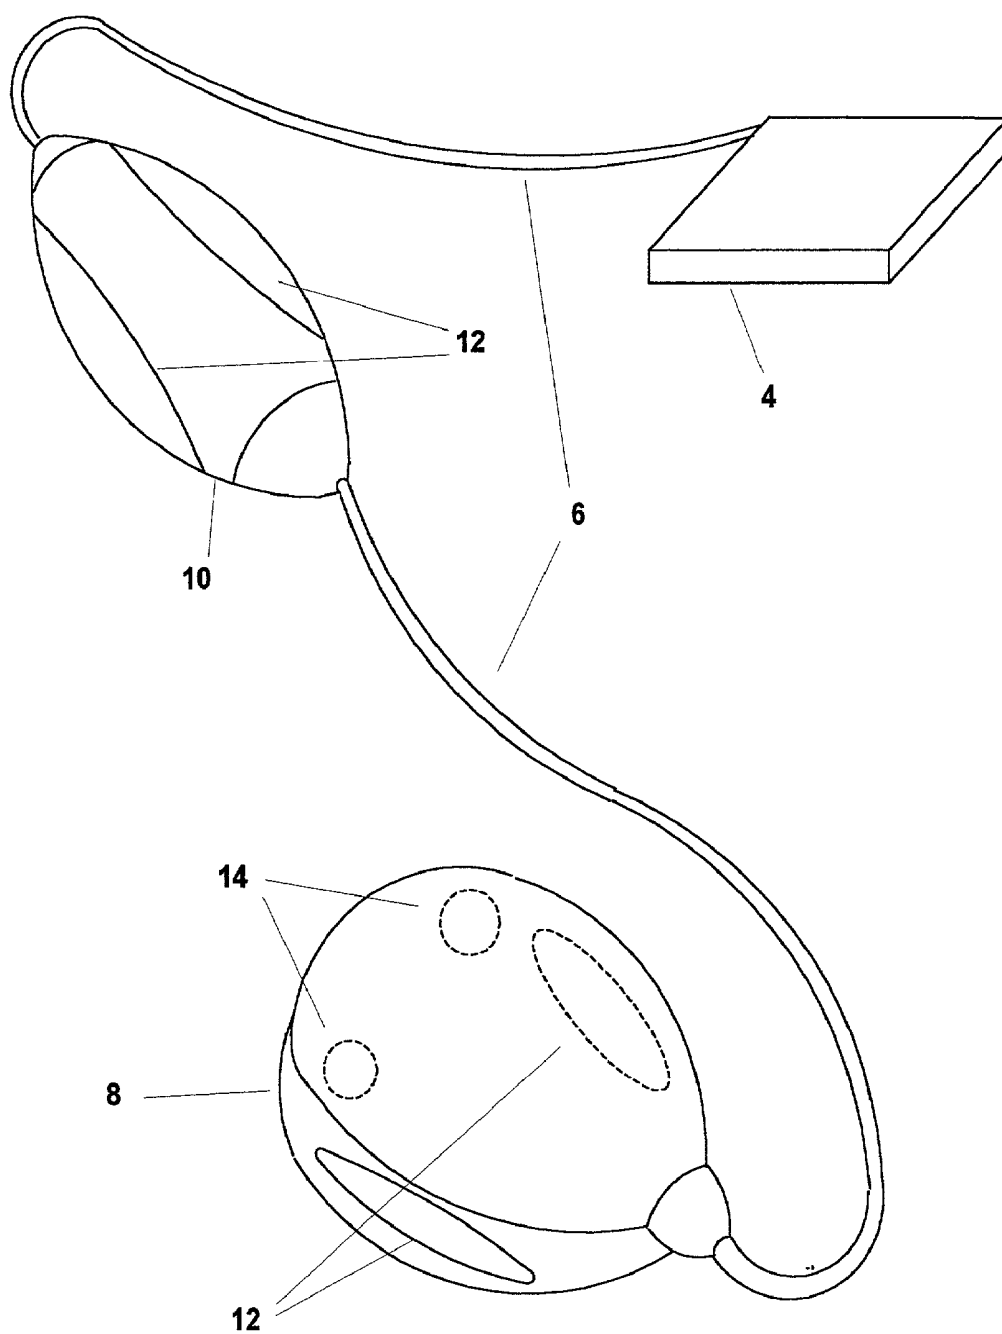**Figure 1**

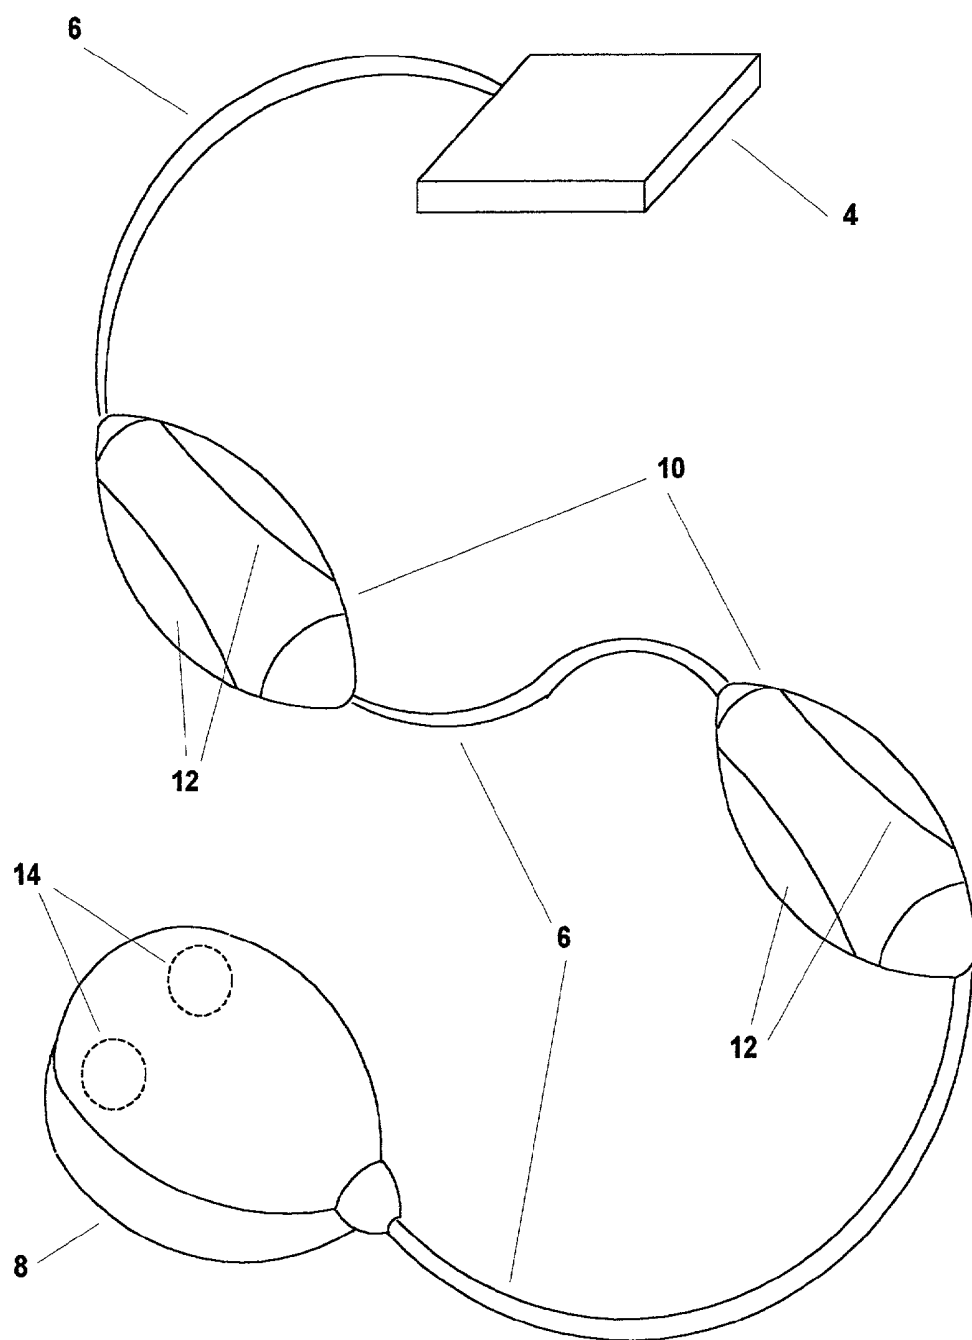
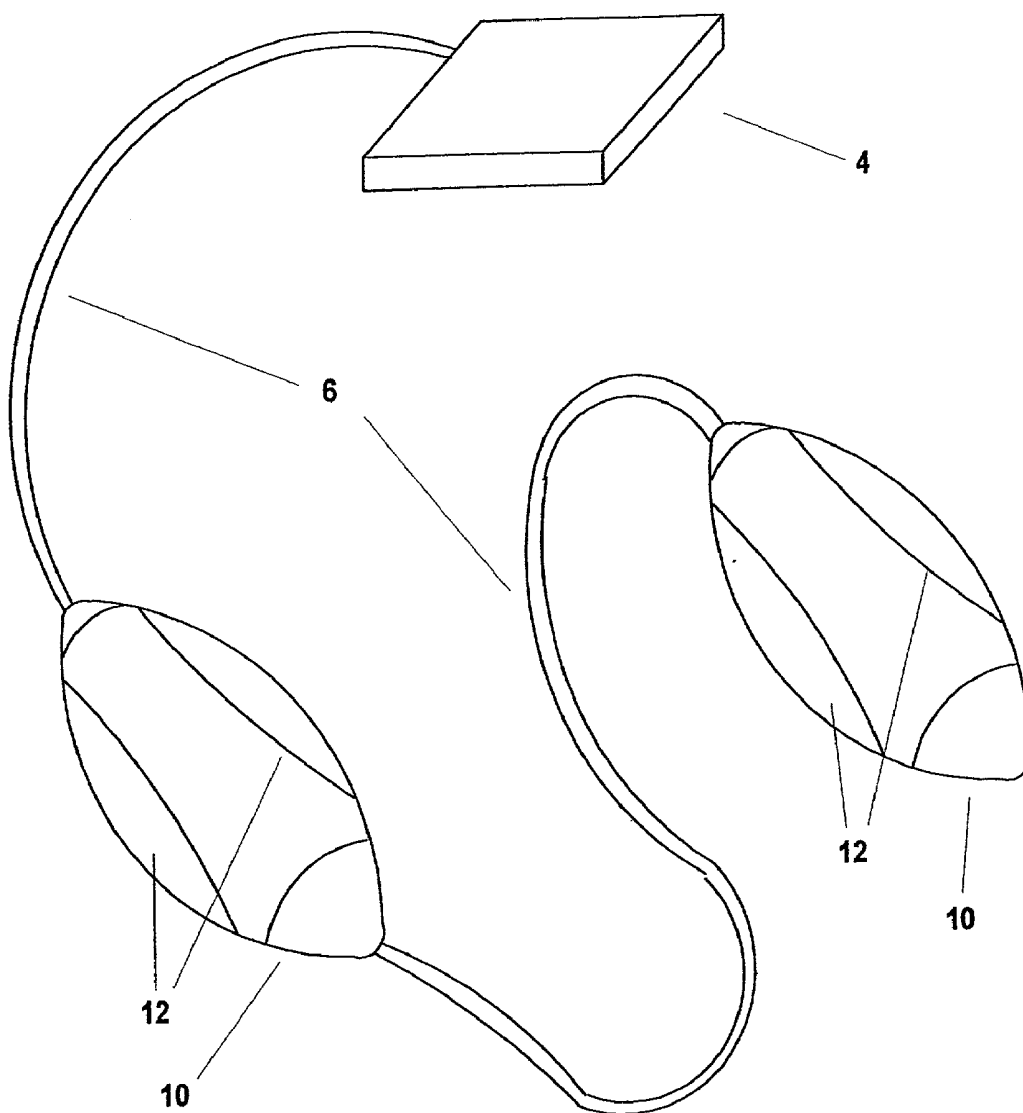


Figure 2

**Figure 3A**

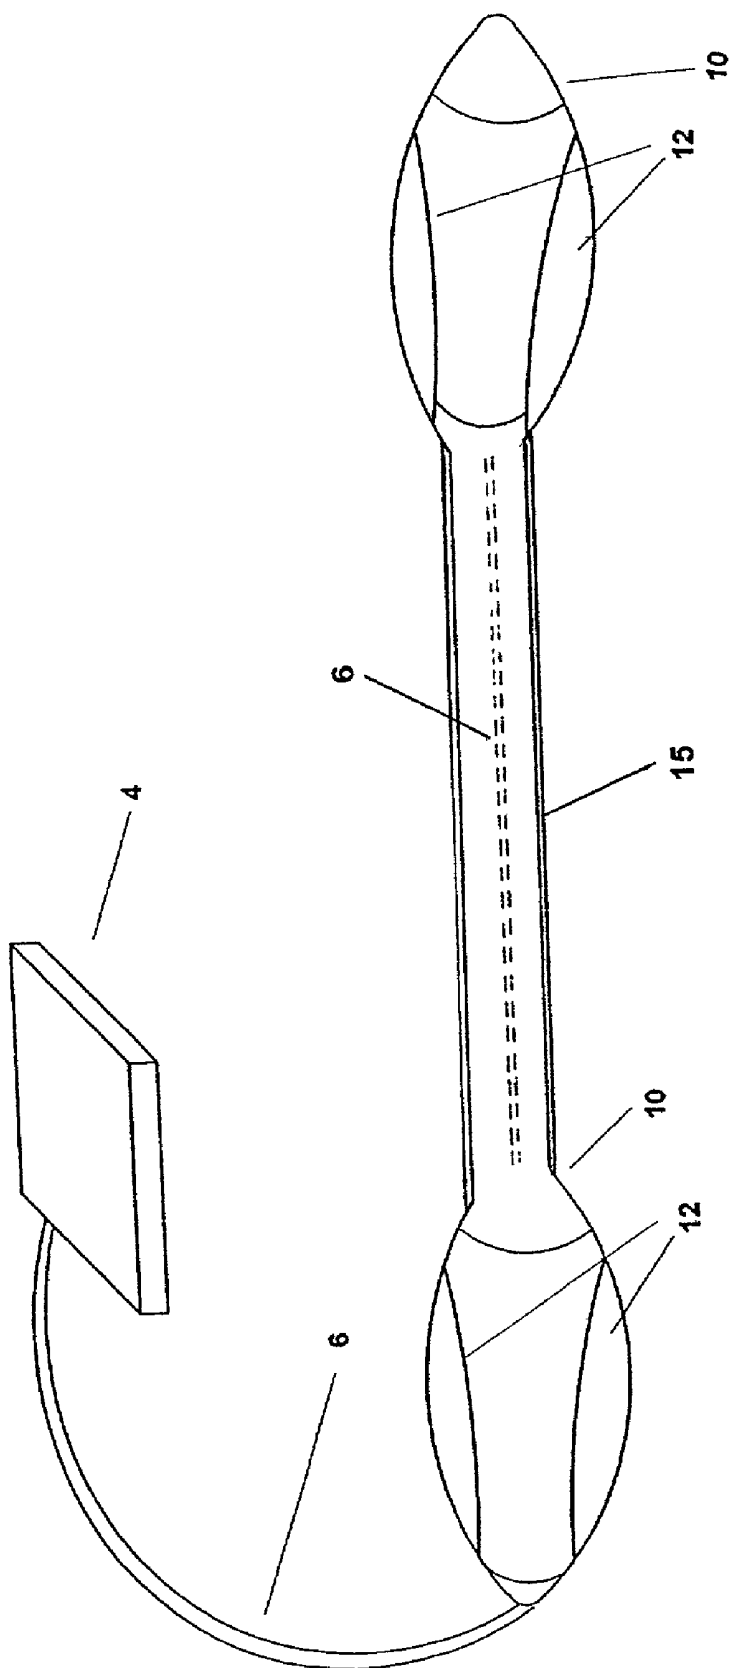


Figure 3B

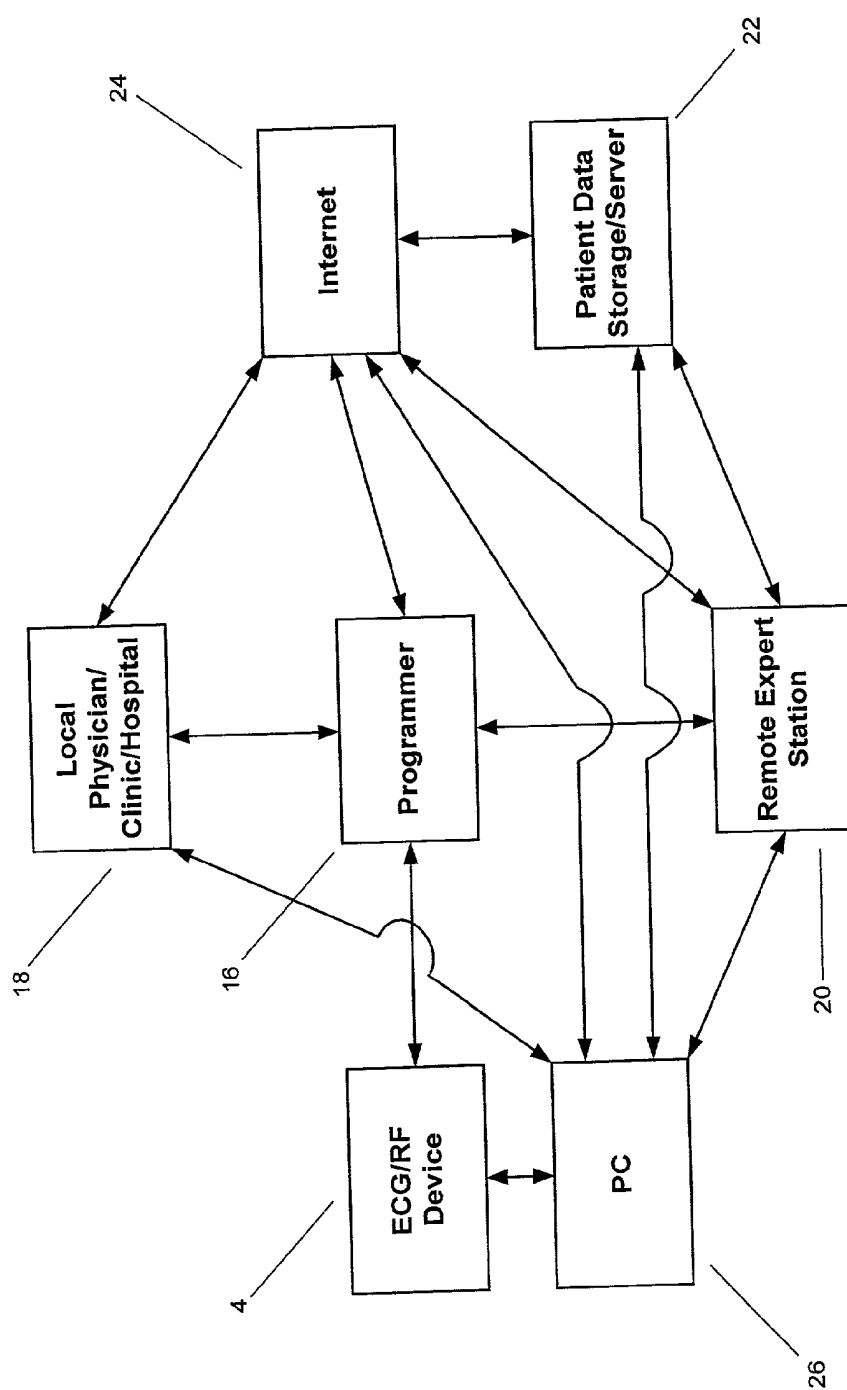


Figure 4

HAND-HELD SURFACE ECG AND RF APPARATUS INCORPORATED WITH A MEDICAL DEVICE

FIELD OF THE INVENTION

[0001] This invention generally relates to a method and apparatus for detecting cardiac depolarizations for remote monitoring of electrocardiograms (ECGs) from patients with an implanted medical device (IMD). More particularly, this invention pertains to hand-held electrodes for recording and transmitting ECG data to a remote site for analysis by a physician, clinician, or diagnostician.

BACKGROUND OF THE INVENTION

[0002] Cardiac muscle is an excitable tissue and includes electrically excitable cardiac muscle cells. Typically, upon intrinsic or artificial supra-threshold electrical excitation, cardiac muscle cells generate a depolarization wave that triggers a delayed contraction. Cardiac muscle cells are electrically coupled enabling the flow of depolarization waves between them. Normally, a group of pacemaker cells located at the Sino-Atrial node in the right atrium originates the depolarization wave that then spreads rapidly to the rest of the heart, first to the atria and then to the ventricles. An ECG is the record of the cardiac depolarizations. A physician uses ECGs to determine a patient's cardiac conduction condition. Depending on the patient's medical condition, it may be needed to document the patient's status at times other than the patient's clinic visit or hospital stay. Typically and prior to the advent of remote monitoring capability, an ECG reading is taken only in a clinical or hospital environment.

[0003] Since a patient's skin exhibits voltage differences due to electrical depolarizations of the heart's muscle cells, ECG signal acquisition involves the use of two or more electrodes placed on a patient's skin. In a clinic, ECGs are recorded via a number of sensing electrodes. An individual electrode usually includes a metal contact that attaches to the patient's skin with an adhesive bandage on which a conductive gel is placed. When paired with other electrode(s), electrode pairs detect changes in electrical potential across the patient's skin. These signals represent cardiac depolarizations and are fed to a recorder that may store them or print them out on a roll of paper as ECG tracings. The ECG electrodes are also capable of detecting artifacts from IMDs such as those indicating a pacing output pulse and printing these on the resultant tracing.

[0004] As the technology associated with IMDs advanced, it soon became clear that it was necessary to have a remote ECG monitoring capability. Transtelephonic ECG monitoring soon became routine for patients with IMDs. Typically, such monitoring is short-term, and involves the patient contacting the physician by phone, and employing an ECG transmitter of the type described in U.S. Pat. No. 4,151,513, issued to Menken et al. Use of such a device, however, typically requires the patient to apply ECG electrodes to the body, and subsequently to couple the monitoring device to their telephone to allow for a brief period of monitoring.

[0005] Alternatively, U.S. Pat. No. 5,503,158 issued to Cuppock, et al describes an ambulatory ECG monitor with a number of sensors placed on the patient's skin to generate an ECG. An amplifier is connected to the sensors to generate an amplified signal. A remote processor is equipped with a

receiver and is connected to the amplifier to receive and process the amplified signal to obtain the patient's electrocardiogram.

[0006] Other methods have also been described, for example, attaching electrodes to the wrist in U.S. Pat No. 5,289,824, issued to Mills et al, or one of the fingers of each hand. In the '824 patent, incorporated herein by reference in its entirety, a wrist-worn monitor is provided that, without external connections of any kind, enables local, multiple event ECG data recording and telecommunication to a remote site. The monitor is housed in a compact and lightweight housing and is operable whenever the patient simply places his/her hand over a portion of the monitor's face to contact an upper skin electrode. Circuitry is provided to drive an integral speaker for the telecommunication of the ECG signal or cardiac event data via telephone lines to a remote site for so-called "over-read", diagnosis and archival recording. The monitor's housing includes dual, integral dry skin electrodes located on a wrist contacting, inner or rear base plate and on an outer or front surface contactable by the palm of the patient's other hand.

[0007] Because the average age of the patients who receive an IMD is generally over seventy, the application and use of ECG electrodes often poses various operational and implementation issues. For example, in the '158 patent, multiple electrodes are placed on the patient's upper torso and remain there over a period of time. These attached electrodes may irritate the skin and make it difficult to take a shower. The wrist electrode, described in the '824 patent, eliminates the permanent application of electrodes while maintaining the ability to have a connection to a remote monitor as disclosed in the '158 patent. The wrist electrode, however, is not without its own problems. For example, an elderly patient may have arthritis and find it quite difficult to attach wrist electrodes or, due to very thin wrists, keep them in close contact with the skin.

[0008] Other types of electrodes, especially those intended for direct application to the skin, such as stick-on electrodes that require a conductive gel, are quite difficult for any patient to apply regardless of his or her age. Removing these types of electrodes can cause extreme skin irritation to a patient of any age, but especially to an elderly patient whose skin may likely be quite thin. Finally, positioning such electrodes requires training in order to acquire an adequate signal that result in an ECG of diagnostic quality.

[0009] Transtelephonic systems, known in the art, seem to require a number of connecting cables to attach the sensing electrodes to the monitoring device. The number of cables may increase when a separate RF head is provided to detect and transmit simultaneous data from the IMD. The responsibility to ensure an adequate connection of these cables to the monitor should not be left to patients. This is partly because patients may forget and, in most cases, may not be comfortable operating electronic equipment.

[0010] Accordingly, current patient management and follow-up require a nurse, clinician/technician call or inform the patient of the need for an ECG tracing when, for example, a physician may ask for one. This call may serve as a reminder to the patient that the appointment is scheduled for some time in the future. Such reminders are important because scheduled monitoring often occur infrequently, for example, at three or six month intervals.

[0011] Following the reminder, the patient must locate the equipment some time prior to the actual start of the scheduled monitoring. After connecting or applying the ECG electrodes, the patient must connect them to the monitoring device. If the monitoring device is a transtelephonic device, that device must also be plugged into a wall socket. The patient waits for the call from the nurse/technician and then begins to transmit the ECG, when instructed to do so. If the ECG electrodes do not have adequate contact with the skin or improperly positioned, the patient is instructed to reposition the ECG electrodes to try another transmission. The nurse/technician on the other end of the line can only hope the patient will reposition the electrodes properly. At times, many attempts are made without much success. In such cases, the only option is to schedule a clinic visit to ensure the acquisition of a diagnostic quality ECG tracing.

SUMMARY OF THE INVENTION

[0012] The present invention, inter alia, overcomes the various limitations of the prior art and simplifies the steps required to collect reliable medical data. Specifically, the present invention includes a cable onto which are attached two or three objects, at least two of which are hand-holdable structures that the patient grasps in the hand in addition to any optional lightweight RF telemetry head. The holdable structure incorporates ECG electrodes. These electrodes ensure good skin-electrode contact to detect cardiac depolarizations. The RF telemetry head is implemented to detect ECGs via electrodes and also downlink with an IMD if needed. When arranged in this manner, the RF telemetry head serves a dual role by detecting ECGs and/or collecting and transmitting data from the IMD. Specifically, when the telemetry head is used to detect depolarization potentials, surface ECG electrodes are incorporated into the telemetry head are used. In the alternative, the head could be used to collect data from the IMD, while simultaneously collecting depolarization data via the electrodes.

[0013] In another embodiment, the lightweight telemetry head may be used solely as a means of collecting IMD data. Generally, the head may collect continuous data from the holdable structures or stored data from the IMD. Preferably, a shielded cable RF/telemetry unit connects the holdable structures to the telemetry head. The RF/telemetry unit transmits ECGs and/or collected IMD data via any one of several means, hard-wired, RF telemetry, infra-red connectivity, BlueTooth or Home RF technology, transtelephonic, or other standard connector known in the art. The RF telemetry of the present invention is similar to telemetry systems disclosed in commonly assigned U.S. Pat. Nos. 6,167,310 to Grevious; 5,752,977 to Grevious et al. and 5,350,411 to Ryan et al. which patents are incorporated herein by reference in their entirety.

[0014] Because of the relatively advanced age of the average IMD patients, it is preferred to offer a system that takes into account the potential for some disability (e.g., arthritis) in addition to being user friendly. The present invention addresses such issues. Further, the present invention the use of gels by incorporating ECG electrodes in the holdable structure and/or telemetry head. These electrodes require only dry skin contact.

[0015] The present invention implements a hand holdable structure that allows an easy, natural grip to enable patients

to apply a simple gentle grip on the structure to record ECGs. There is no need to use a band or other means to ensure a tight or forced grip. The design takes into account the possibility that an individual patient might have an impaired grip and may be unable to exert a tight grip around the structure. The total weight of the structure and associated cable(s) and devices have been kept very light. Preferably, the cable weighs less than 2 pounds, to accommodate those patients who find it difficult to lift and support heavy weights.

[0016] Collection of ECG tracings automatically begins when the patient grasps the structure and the lightweight telemetry head maintains a good skin-electrode contact. When the telemetry head is in use to collect medical device data, grasping the structure with good skin-electrode contact automatically activates both ECG acquisition and data collection. Subsequently, as soon as the patient breaks skin-electrode contact, ECG acquisition and is terminated.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] FIG. 1 is an illustration of a first embodiment, including a hand holdable structure connected to a lightweight telemetry head with both elements connected together by cable and then by cable to an ECG/RF telemetry unit.

[0018] FIG. 2 is an illustration of a second embodiment, with two hand holdable structures connected to a lightweight telemetry head all connected to a cable and an ECG/RF telemetry unit.

[0019] FIG. 3A is an illustration of the third embodiment, that is, with the hand holdable structures connected together by cable and to an ECG/RF telemetry unit.

[0020] FIG. 3B is an alternate embodiment in which the hand-holdable structure is implemented with a rigid connector.

[0021] FIG. 4 is a simplified block diagram showing ECG/RF signals for distribution, transfer and management across various medium.

DETAILED DESCRIPTION OF THE DRAWINGS

[0022] FIG. 1 depicts a first embodiment of the present invention, wherein the patient is able to grasp structure 10 in one hand and lightweight telemetry head 8 in the other. Skin contact with one or more conductive, non-oxidizing electrodes 12 located on structure 10 and telemetry head 8 is achieved by virtue of a substantially ovoid bulb geometry of structure 10. More specifically, structure 10 is designed to provide ease of grasp and also enable intimate contact with a patient's hand to record and transmit ECG data. Telemetry head 8 is adapted to a size and weight to fit comfortably in the hand of the patient. The patient's fingers or other parts of the hand will make contact with electrodes 12 on either side of structure 10 and telemetry head 8. Cable 6 serially connects telemetry head 8, structure 10, and telemetry unit 4. Telemetry unit 4 transmits ECGs and/or collected IMD data via any one of several data transmission systems, including but not limited to a modem, RF telemetry, infra-red connectivity, Blue Tooth, Home RF technology, transtelephonic systems or equivalent systems known in the art. Cable 6 is shielded in such a way that the RF data signals do not interfere with the ECG signals collected at structure 10.

Cable 6 also has one connector with a sufficient number of pins to transfer both types of signals without interference.

[0023] Further referring to FIG. 1, the patient will usually be transmitting ECG signals as well as data from the IMD. Telemetry head 8 includes sensors 14 to enable data transmission from the IMD. Specifically, the patient positions telemetry head 8 over the IMD to initiate an uplink session in which stored data from the IMD is transmitted via telemetry 4. Similarly, ECG signals will be transmitted when structure 10 and 8 are properly positioned with good skin contact in the patient's hand.

[0024] Referring to structure 10 in more detail, the shape of electrodes 12 and the design of structure 10 may vary. Specifically, the substantially ovoid bulbous shape of structure 10 depicted herein is only a representative sample of the many hand-holdable shapes and structures contemplated by the present invention. For example, the bulbous shape of structure 10 could be circular or may take the shape of any other geometry that can be fabricated to fit easily and comfortably into a patient's grasp or on/over the hand. Similarly the oblong shape of electrodes 12 could be varied to cover the whole surface of ovoid structure 10. Telemetry head 8, in this embodiment, may also be fabricated in other geometric shapes. The present invention serves to transmit ECGs and IMD data while making such transmission as easy and as comfortable for the patient as possible. To date, the ovoid shape of structure 10 fulfills, inter alia, these requirements.

[0025] FIG. 2 is an illustration of a second embodiment of this invention. In this embodiment, preferably a plurality of structure 10, attached in tandem by cable 6, with one or more conductive non-oxidizing electrodes 12 on their surfaces are shown. To use this device a patient would simply grasp structure 10, one in each hand, and when good skin-electrode contact occurs ECG transmission would begin. Telemetry head 8, is used exclusively to detect and transmit data from the IMD. Telemetry head 8 preferably has no ECG electrodes, only sensors 14. Telemetry head 8 would be held in close proximity to the IMD by an attachment method, such as a pouch or modified sling (not shown). RF transmission of the data via telemetry 4 would begin immediately upon the start of ECG transmission, as described above. Telemetry head 8 could have various shapes and does not need to conform to a grasp because it need not be held by the patient during transmission.

[0026] FIG. 3A illustrates a third embodiment of the present invention in which two of structure 10 are arranged attached in tandem by cable 6 with one or more conductive, non-oxidizing electrodes 12 on their surface. This embodiment is dedicated to acquire ECG tracings via structure 10 and electrodes 12. If data from the IMD were desired, a separate telemetry head (similar to FIG. 1 or 2) would be required.

[0027] FIG. 3B is an alternate embodiment in which structures 10 are connected by rigid connector 15 with cable 6 running therethrough.

[0028] Referring to FIG. 4, the ECG tracing and RF data from the IMD is transmitted from ECG/RF telemetry unit 4 to programmer 16 by any one of several means: hard-wired, RF telemetry, infra-red connectivity, fiberoptics network, Blue Tooth or Home RF technology, transtelephonic, or

equivalent. Transmission of the signal from programmer 16 can be via internet/modem connection, telephone landline, satellite telemetry, fiberoptics, laser, or other means as generally described in U.S. Pat. No. 5,752,976 issued to Duffin, et al. and incorporated herein in its totality.

[0029] Functionally, an operator at programmer 16 may initiate remote contact. Programmer 16 is adapted too downlink to ECG/RF device 4. Generally, an operator is not needed to operate programmer 16. In fact, uplink from ECG/RF device 4 may be initiated by ECG/RF device 4 and transmission made by any one means as described above. For example, programmer 16 may contain a telemetry transmitter and receiver to uplink and downlink to ECG/RF device 4, a modem, a landline telephone receiver, or equivalent. In any case, signal transmission to programmer 16 may occur remotely, that is, from the patient's home, or within the larger confines of a clinic or hospital, e.g., from a waiting room to the room in which the programmer(s) 16 reside. Programmer 16 is preferably of the type disclosed in U.S. Pat. No. 5,345,362 issued to Winkler, et al., incorporated herein in its totality.

[0030] Communication between programmer 16 and remote expert station 20 is executed via wave units, as described in the '976 patent. Remote expert station 20 includes a plurality of high speed network web-based or web-compatible communication systems. Preferably, in the context of the present invention, remote expert station 20 is in wireless communication with programmer 16. However, the means of communication between expert station 20 and programmer 16 may be selected from one or a combination of several cable and wireless systems, as mentioned above.

[0031] Remote expert station 20 includes software that can identify a noteworthy medical events on the ECG tracing. If such an event is identified, the software determines whether a medical warning is required. If so, warning is immediately issued and transmitted to local physician/clinic/hospital 18 either directly through programmer 16 or indirectly via Internet 24. The event is also recorded in patient data storage 22. In addition, a software in remote expert station 20 analyzes the stored device data and, if necessary, makes a suggestion about programming changes to device parameters. This programming change may be coupled to the medical event that merited a warning. In the alternate, it may be solely based on analysis of stored diagnostic data. For example, if the patient had not attained a normal rate distribution, remote expert station may suggest a change in rate response parameters.

[0032] Programmer 16 is also in direct communication with local physician/clinic/hospital 18. As usually practiced, programmer 16 is located within the confines of a "pacing clinic" to use this therapy as an example. The physician may or may not be present at this clinic. If not, the ECG tracings and data may be sent directly to physician 18, responsible for a specific patient..

[0033] On the other hand, if, for example, the patient's physician is otherwise occupied at the time of ECG/data acquisition, clinic, or hospital 18 may access remote expert station 20 via Internet 24. If contact by physician/clinic/hospital 18 is further delayed, for example, until the next day, the patient's ECG and other medical data will have already been downloaded to patient data storage 22. In this case, physician/clinic/hospital 18 may access patient data storage 22 via Internet 24.

[0034] Patient data storage 22 is a highly interactive component of the system. User identification is required prior to admission. When admitted, the physician 18 may, for example, review the previously mentioned stored suggestions for reprogramming from remote expert station 20. If approved, these programming commands may be routed back to programmer 16 for down linking to the IMD via other methods that are not in the scope of this patent. If not approved, the physician may call for further data that may be obtained by the use of this invention or requesting that the patient come in for a clinic visit.

[0035] In one embodiment PC 26 is implemented to transmit/record ECG and IMD data from ECG/RF device 4. PC 26 is adapted to be in data communication with local physician/clinic/hospital 18, remote expert station 20, storage/server 22 and Internet 24.

[0036] The preceding specific embodiments are illustrative of the practice of the invention. It is to be understood, therefore, that other expedients known to those of skill in the art or disclosed herein may be employed without departing from the invention or the scope of the appended claim. It is therefore to be understood that the invention may be practiced otherwise than is specifically described, without departing from the scope of the present invention. As to every element, it may be replaced by any one of infinite equivalent alternatives, only some of which are disclosed in the specification.

What is claimed is:

1. A hand-holdable device to establish reliable skin-electrode contact for physiological signal acquisition, the hand-holdable device comprising:

- a first structure with at least one electrode shaped to be easily graspable to establish said skin-electrode contact in one hand;
- a second structure with at least one electrode shaped to be easily graspable to establish said skin-electrode contact in another hand; and
- a telemetry unit having operable data communications link with said first and said second structure,

said first structure being connected to said second structure wherein the physiological signal created across said first and said second structures is transmitted to said telemetry unit via said data communication link.

2. The device of claim 1 wherein said first and second structure include a substantially ovoid shape conforming to a human grasp.

3. The device of claim 1 wherein a headless RF telemetry is incorporated in one of said first and second structures to uplink to an IMD.

4. The device of claim 2 wherein said at least one electrode is shaped to conform to said ovoid shape.

5. The device of claim 4 wherein said at least one electrode substantially covers major surfaces of said ovoid shape.

6. The device of claim 1 wherein said telemetry unit includes a communication link to transmit medical data collected by said device to one of and all of a programmer, a PC, a remote station, a data server.

7. The device of claim 6 wherein said medical data includes medical data collected from at least one IMD in a patient using said device.

8. A hand-held surface ECG and RF system for detecting cardiac depolarizations for remote monitoring of ECGs from a patient with an IMD, the system comprising:

a structure shaped to conform to a grasp of the patient; electrodes incorporated in the said structures to enable reliable skin-electrode contact at said grasp of the patient;

a data communication link between said structure and said RF system to enable transmission of ECG tracing from the structure.

9. The system of claim 8 wherein said structure includes substantially ovoid shapes forming a first end and second end rigidly spread apart by a connecting member.

10. The system of claim 9 wherein said connecting member includes means for routing a data communications cable between said first end and said second end.

* * * * *

专利名称(译)	手持式表面ECG和RF装置与医疗装置结合		
公开(公告)号	US20020095093A1	公开(公告)日	2002-07-18
申请号	US09/821201	申请日	2001-03-29
[标]申请(专利权)人(译)	AU NELSON BRECHT MARK BUCHENAU MARION CROWLEY THOMAS KARSHMER DAVID NELSON CHESTER 摹 OAKLEY NICK PEARCE EDWIN 中号 PERRY POOL NANCY 鲍威尔 RICHARD 中号 TAL ELISHA		
申请(专利权)人(译)	AU NELSON BRECHT MARK BUCHENAU MARION CROWLEY THOMAS KARSHMER DAVID NELSON CHESTER G. OAKLEY NICK PEARCE EDWIN M. PERRY POOL NANCY 鲍威尔 理查德 M. TAL ELISHA		
当前申请(专利权)人(译)	美敦力公司, INC.		
[标]发明人	AU NELSON BRECHT MARK BUCHENAU MARION CROWLEY THOMAS KARSHMER DAVID NELSON CHESTER G OAKLEY NICK PEARCE EDWIN M JR PERRY POOL NANCY POWELL RICHARD M TAL ELISHA		
发明人	AU, NELSON BRECHT, MARK BUCHENAU, MARION CROWLEY, THOMAS KARSHMER, DAVID NELSON, CHESTER G. OAKLEY, NICK PEARCE, EDWIN M. JR. PERRY POOL, NANCY POWELL, RICHARD M. TAL, ELISHA		

IPC分类号	A61B5/00 A61B5/0404
CPC分类号	A61B5/0006 A61B5/0404 A61B2560/0468
优先权	60/192943 2000-03-29 US
其他公开文献	US6748260
外部链接	Espacenet USPTO

摘要(译)

本发明公开了一种手持式结构，其实现电极以实现良好的皮肤 - 电极接触以获取ECG读数。具体地，该结构被成形为使得患者能够应用简单的轻柔抓握以具有可靠的皮肤 - 电极接触并且自动开始ECG跟踪传输到患者监测站。在一个实施例中，该结构包括RF遥测头，以同时传输IMD存储的数据以及ECG描记。独立地或与RF遥测头组合的结构适用于与编程器或等效仪器的数据通信系统，以将ECG和IMD数据传送到远程定位的医师站或患者数据存储服务器。该系统还适用于支持web的网络，例如但不限于因特网，内联网，万维网，外联网或等同物。

