



US007254430B2

(12) **United States Patent**
Cho et al.

(10) **Patent No.:** **US 7,254,430 B2**
(45) **Date of Patent:** ***Aug. 7, 2007**

(54) **MEASURING APPARATUS FOR
MEASURING A METABOLIC
CHARACTERISTIC IN A HUMAN BODY**

(75) Inventors: **Ok-Kyung Cho**, Schwerte (DE);
Yoon-Ok Kim, Schwerte (DE)

(73) Assignee: **Hitachi, Ltd.**, Tokyo (JP)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 134 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **11/169,777**

(22) Filed: **Jun. 30, 2005**

(65) **Prior Publication Data**

US 2005/0251000 A1 Nov. 10, 2005

Related U.S. Application Data

(63) Continuation of application No. 10/620,689, filed on Jul. 17, 2003.

(30) **Foreign Application Priority Data**

May 7, 2003 (JP) 2003-129020

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.** **600/316; 600/365; 600/326**

(58) **Field of Classification Search** **600/310, 600/316, 322, 323, 326, 365, 549**

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,306,569 A	12/1981	Weil
4,333,803 A	6/1982	Seger
4,509,531 A	4/1985	Ward
4,750,140 A	6/1988	Asano
4,802,489 A	2/1989	Nitzan
5,551,422 A	9/1996	Simonsen
5,676,143 A	10/1997	Simonsen
5,725,480 A	3/1998	Oosta
5,732,711 A	3/1998	Fitzpatrick
5,743,262 A	4/1998	Lepper, Jr.
5,769,784 A	6/1998	Barnett
5,795,305 A	8/1998	Cho
5,857,966 A	1/1999	Clawson

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0 387 630 9/1990

(Continued)

OTHER PUBLICATIONS

Hillson, R.M., "Facial and Sublingual Temperature Changes Following Intravenous Glucose Injection in Diabetics", *Diabete & Metabolisme (Paris)* 1982, vol. 8, pp. 15-19.

(Continued)

Primary Examiner—Eric F Winakur


(74) *Attorney, Agent, or Firm*—Antonelli, Terry, Stout & Kraus, LLP.

(57) **ABSTRACT**

Blood sugar levels are non-invasively measured based on temperature measurements. Blood sugar levels obtained by non-invasive measurements of temperatures are corrected by blood oxygen saturation and the volume of blood flow so that the measurement data can be stabilized.

See application file for complete search history.

22 Claims, 8 Drawing Sheets

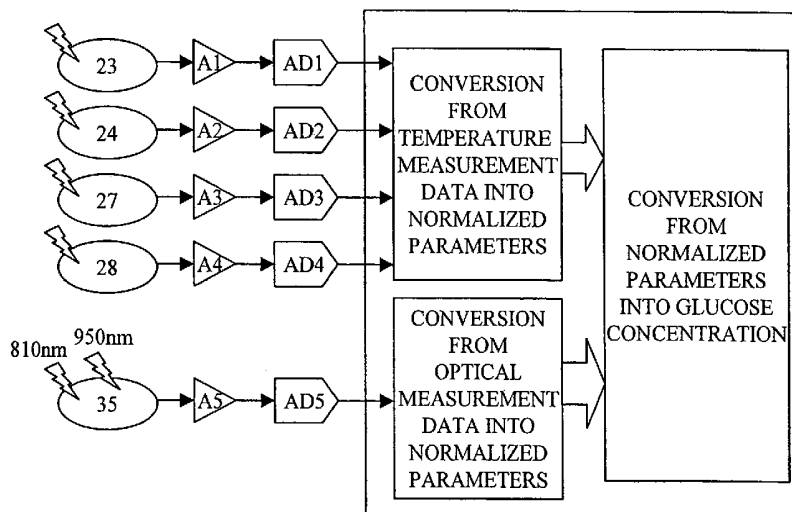

U.S. PATENT DOCUMENTS

5,899,855	A	5/1999	Brown
5,924,996	A	7/1999	Cho
6,226,089	B1	5/2001	Hakamata
6,240,306	B1	5/2001	Rohrscheib
6,269,314	B1	7/2001	Iitawaki et al.
6,270,455	B1	8/2001	Brown
6,280,381	B1	8/2001	Malin
6,353,226	B1	3/2002	Khalil
6,551,276	B1	4/2003	Mann et al.
6,615,061	B1	9/2003	Khalil
2002/0183646	A1	12/2002	Stivoric et al.
2003/0010898	A1	1/2003	MacKenzie
2003/0152133	A1	8/2003	Ellenz
2003/0214655	A1	11/2003	Weiss et al.
2004/0009100	A1	1/2004	Simons et al.

FOREIGN PATENT DOCUMENTS

EP	0 778 000	A1	6/1997
GB	1502056		2/1978
JP	06-317566		11/1994
JP	7-71945		3/1995
JP	08-322821		12/1996
JP	9-641151		12/1996
JP	10-33512		2/1998
JP	10-108857		4/1998

JP	11-505451		5/1999
JP	11-155840		6/1999
JP	11-230901		8/1999
JP	11-318872		11/1999
JP	2000-074829		3/2000
JP	2000-506048		5/2000
JP	2000-258343		9/2000
JP	2002-535023		10/2002
JP	2003-510556		3/2003
WO	01/28417		4/2001
WO	01/28414		4/2001
WO	03/010510		2/2003

OTHER PUBLICATIONS

Scott, A.R., "Diabetes Mellitus and Thermoregulation¹", *Can. J. Physiol. Pharmacol.*, vol. 65, 1987, pp. 1365-1376.

Journal of the Medical Association of Thailand, vol. 69, No. 3, 1986, pp. 153-157 (abstract).

Delayed Metabolic and Thermogenic Response to a Mixed Meal in Normoglycemic European Woman with Previous Gestational Diabetes, *The Journal of Clinical Endocrinology & Metabolism*, pp. 3407-3412, Kousta et al, Mar. 25, 2005.

Metabolic Factors Contributing to Increased Resting Metabolic Rate and Decreased Insulin-Induced Thermogenesis During the Development of Type 2 Diabetes, Weyer, et al., *Diabetes*, vol. 48, Aug. 1999, pp. 1607-1614.

FIG.1

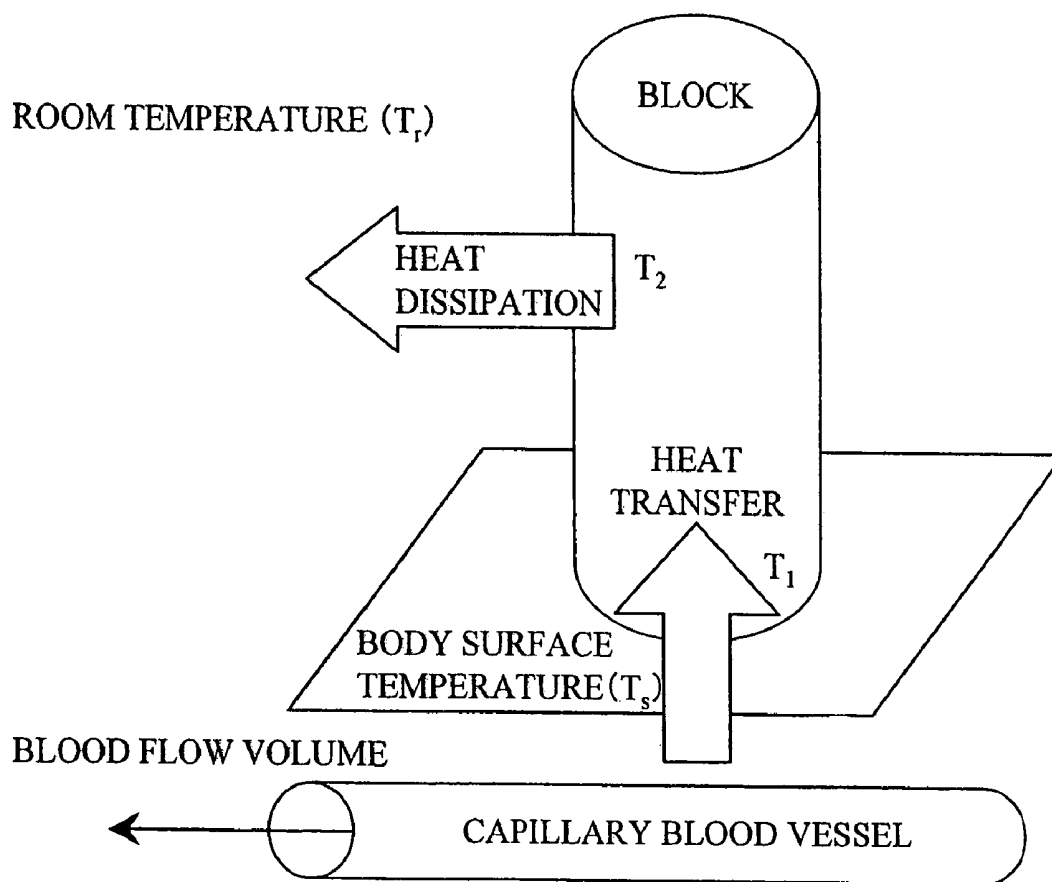


FIG.2

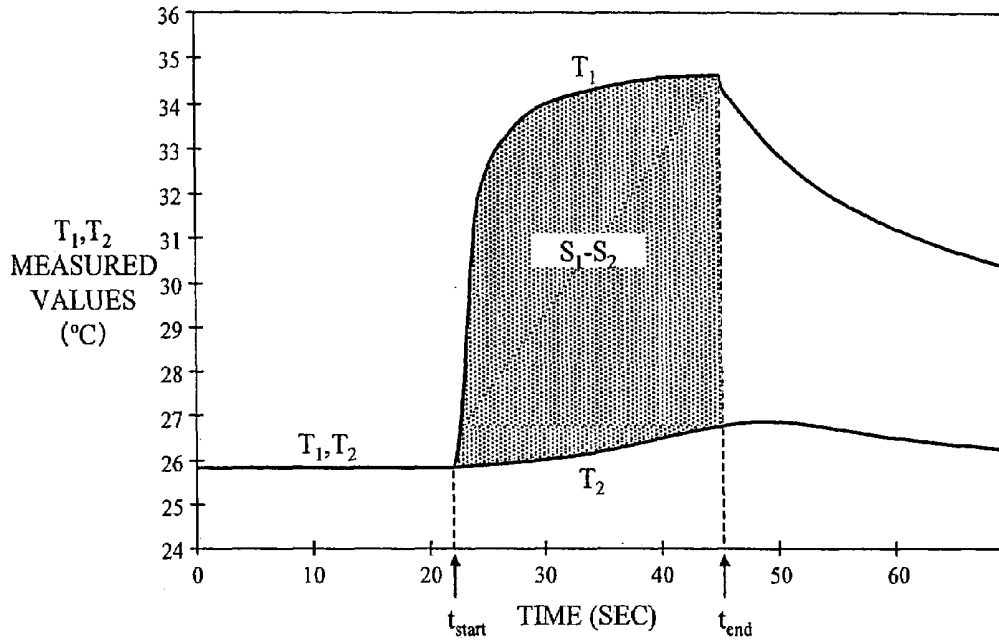


FIG.3

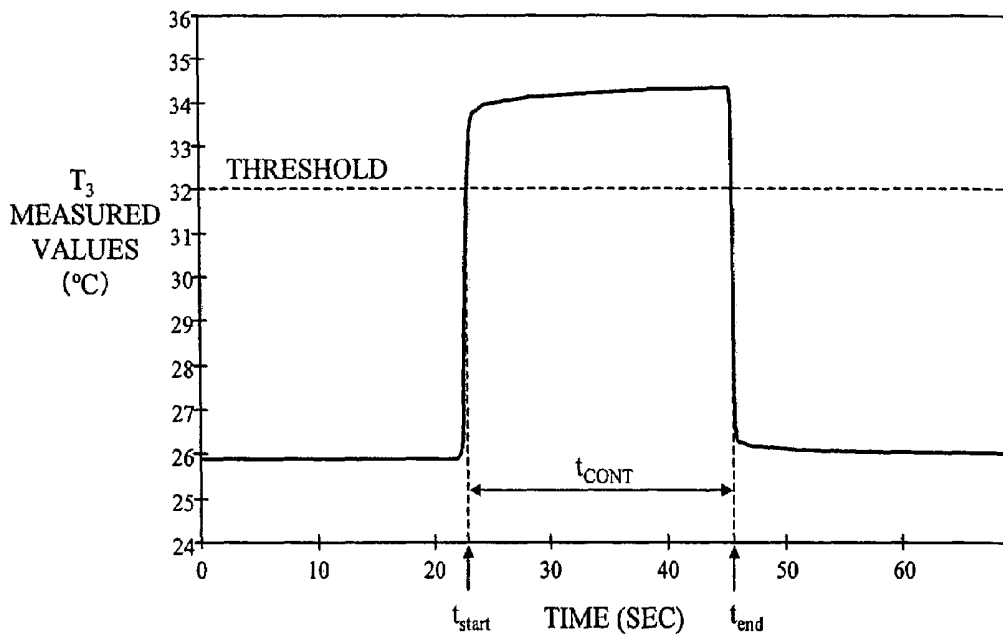


FIG.4

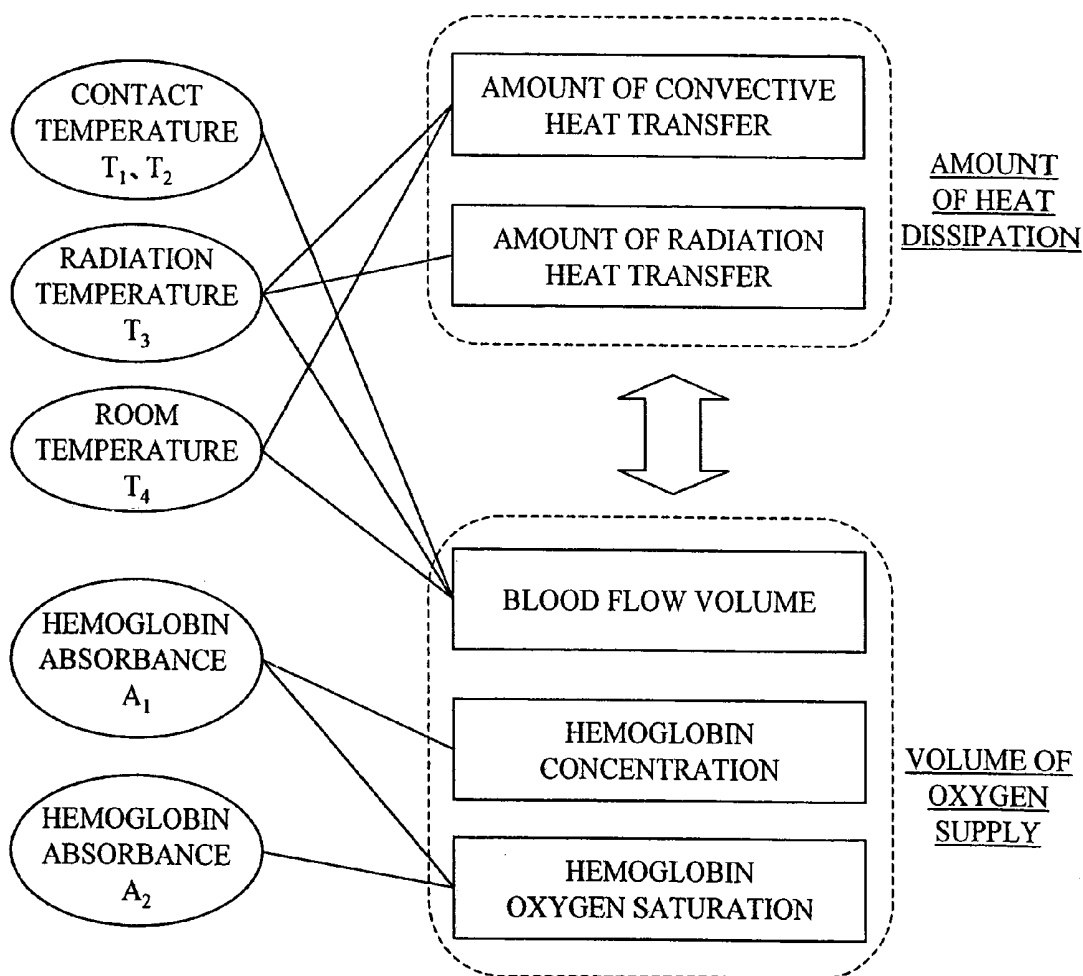


FIG.5

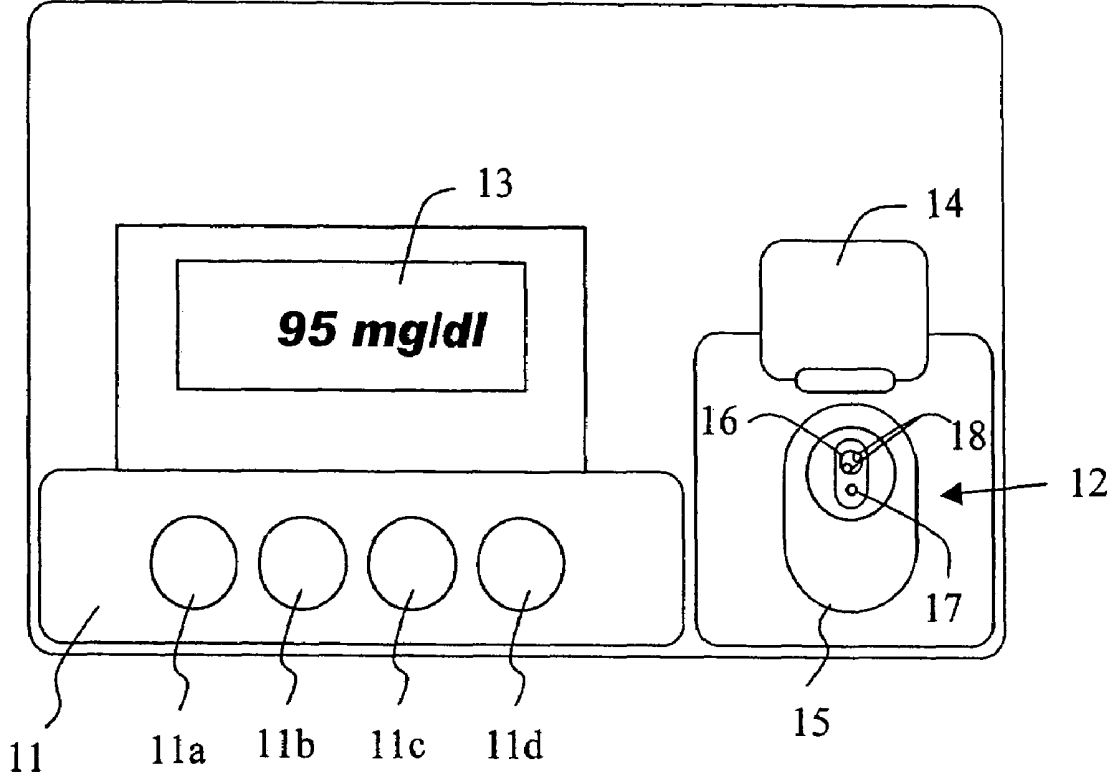


FIG.6

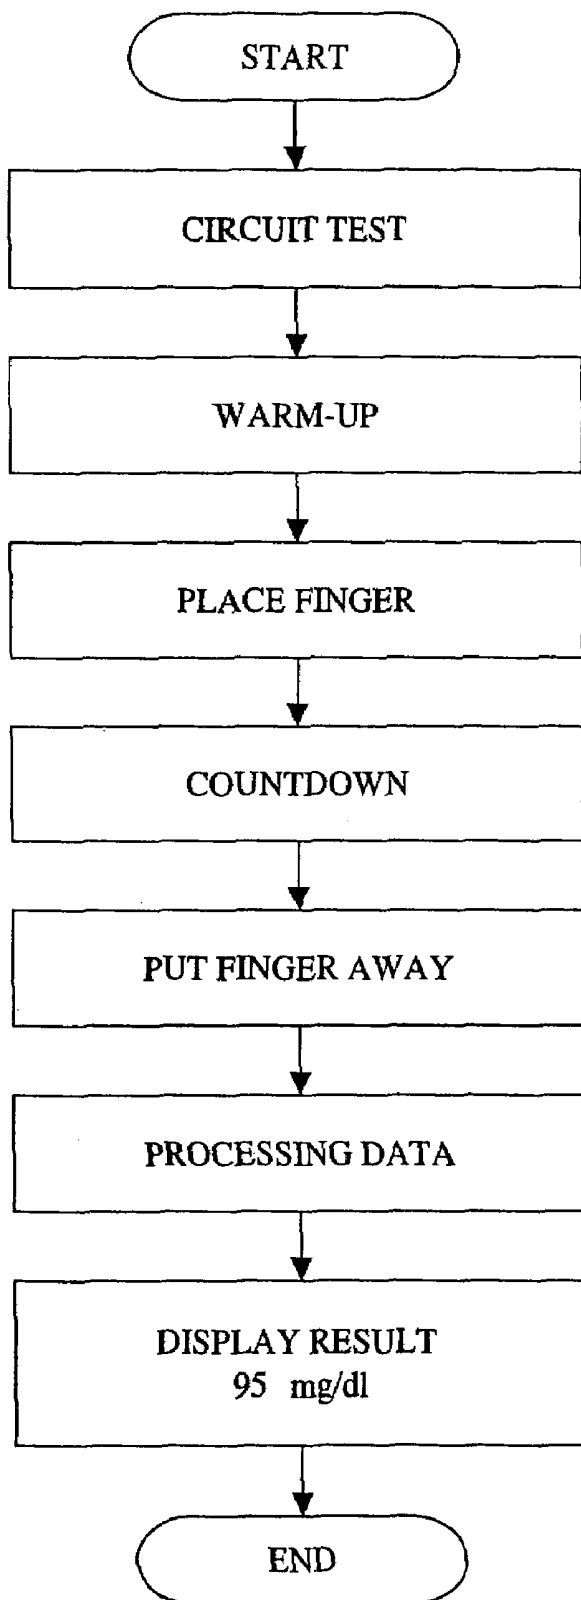


FIG.7(a)

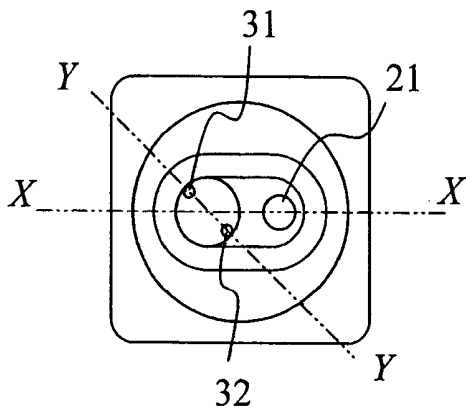


FIG.7(b)

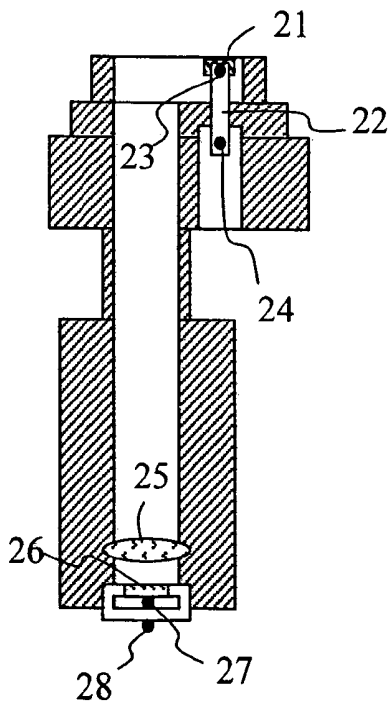


FIG.7(c)

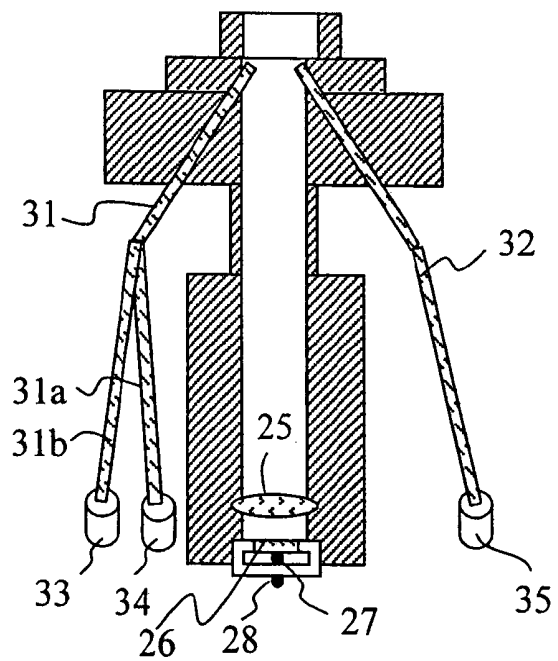


FIG.8


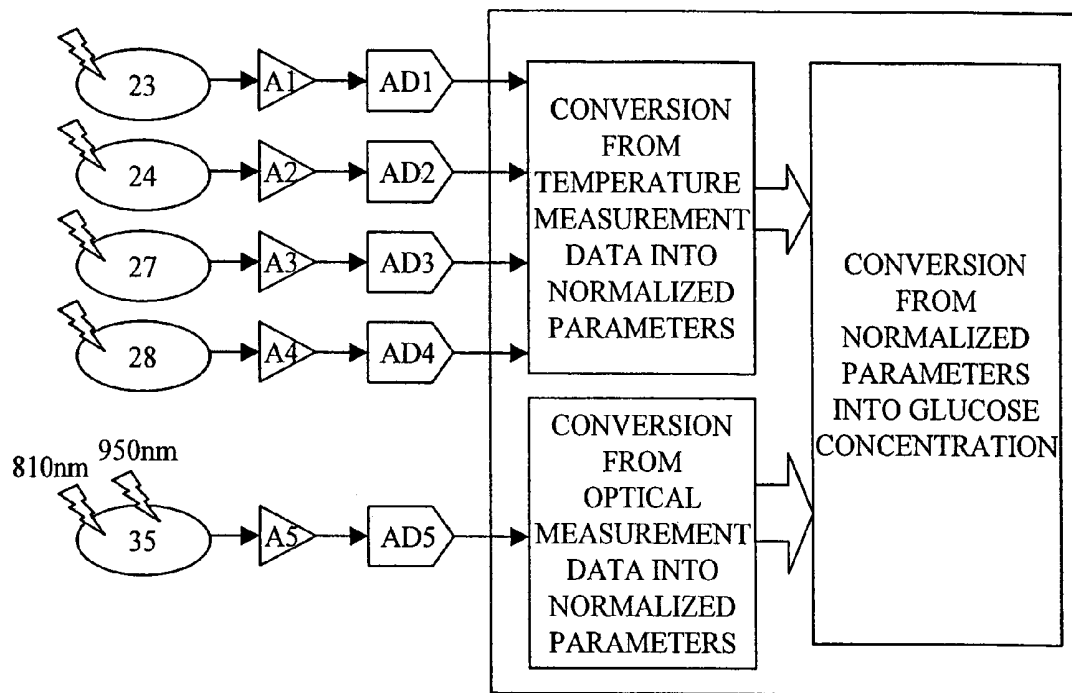


FIG.9

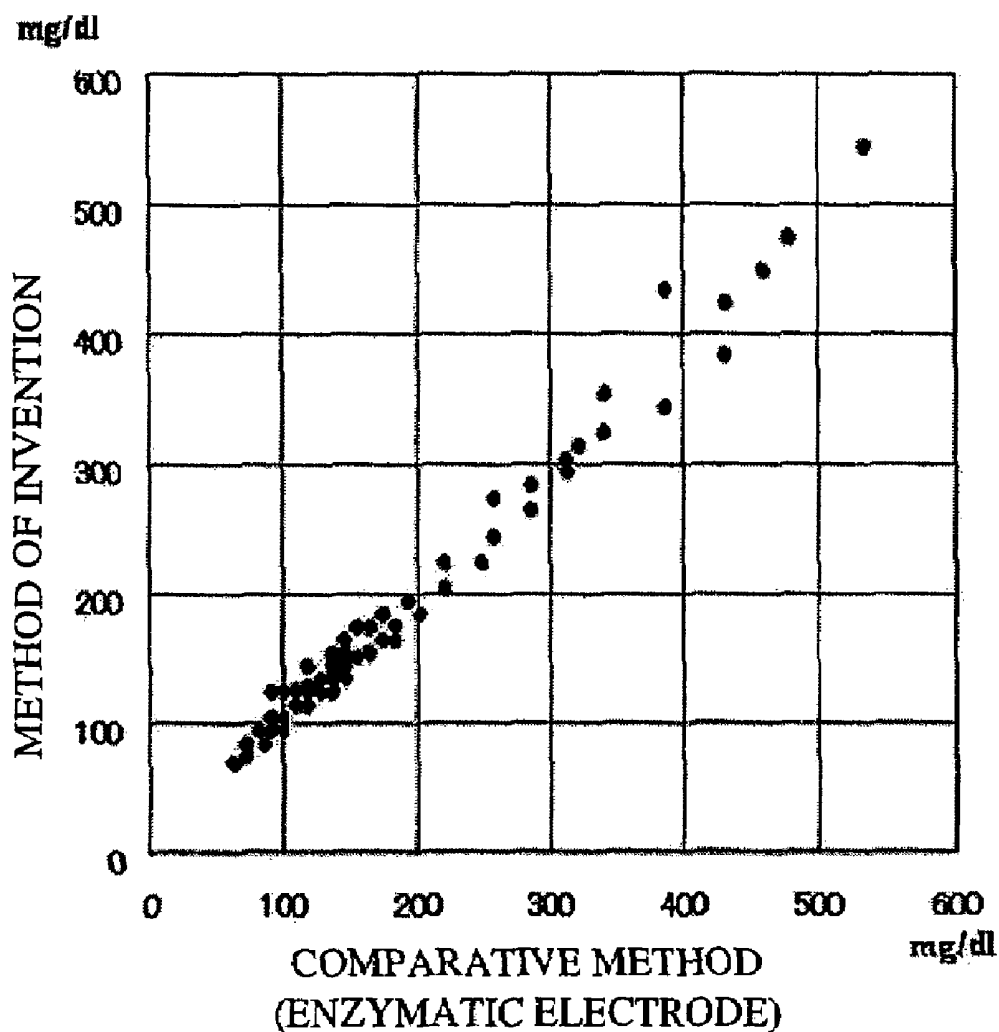

**MEASURING APPARATUS FOR
MEASURING A METABOLIC
CHARACTERISTIC IN A HUMAN BODY**

BACKGROUND OF THE INVENTION

This application is a continuation application of Ser. No. 10/620,689 filed Jul. 17, 2003.

1. Field of the Invention

The present invention relates to a method and apparatus for non-invasively measuring glucose concentration in a living body without blood sampling.

2. Background Art

Hilson et al. report facial and sublingual temperature changes in diabetics following intravenous glucose injection (non-patent literature 1). Scott et al. discuss the issue of diabetes mellitus and thermoregulation (non-patent literature 2). Based on such researches, Cho et al. suggests a method and apparatus for determining blood glucose concentration by temperature measurement without requiring the collection of a blood sample (patent literature 1 and 2).

Various other attempts have been made to determine glucose concentration without blood sampling. For example, a method has been suggested (patent literature 3) whereby a measurement site is irradiated with near-infrared light of three wavelengths, and the intensity of transmitted light as well as the temperature of the living body is detected. Then, representative values of the second-order differentiated values of absorbance are calculated, and the representative values are corrected in accordance with the difference of the living body temperature from a predetermined reference temperature. The blood sugar level corresponding to the thus corrected representative values is then determined. An apparatus is also provided (patent literature 4) whereby a measurement site is heated or cooled while monitoring the living body temperature. The degree of attenuation of light based on light irradiation is measured at the moment of temperature change so that the glucose concentration responsible for the temperature-dependency of the degree of light attenuation can be measured. Further, an apparatus is reported (patent literature 5) whereby an output ratio between reference light and the light transmitted by an irradiated sample is taken, and then the glucose concentration is calculated by a linear expression of the logarithm of the output ratio and the living body temperature.

(Non-patent Literature 1)

R. M. Hilson and T. D. R. Hockaday, "Facial and sublingual temperature changes following intravenous glucose injection in diabetics," *Diabete & Metabolisme*, 8, pp. 15-19: 1982

(Non-patent Literature 2)

A. R. Scott, T. Bennett, I. A. MacDonald, "Diabetes mellitus and thermoregulation," *Can. J. Physiol. Pharmacol.*, 65, pp. 1365-1376: 1987

(Patent Literature 1)

U.S. Pat. No. 5,924,996

(Patent Literature 2)

U.S. Pat. No. 5,795,305

(Patent Literature 3)

JP Patent Publication (Kokai) No. 2000-258343 A

(Patent Literature 4)

JP Patent Publication (Kokai) No. 10-33512 A (1998)

(Patent Literature 5)

JP Patent Publication (Kokai) No. 10-108857 A (1998)

Glucose (blood sugar) in the blood is used for glucose oxidation reaction in cells to produce necessary energy for the maintenance of living bodies. In the basal metabolism

state, in particular, most of the produced energy is converted into heat energy for the maintenance of body temperature. Thus, it can be expected that there is some relationship between blood glucose concentration and body temperature. However, as is evident from the way sicknesses cause fever, the body temperature also varies due to factors other than blood glucose concentration. While methods have been proposed to determine blood glucose concentration by temperature measurement without blood sampling, they lack sufficient accuracy.

SUMMARY OF THE INVENTION

It is the object of the invention to provide a method and apparatus for determining blood glucose concentration with high accuracy based on temperature data of subjects without blood sampling.

Blood sugar is delivered to the cells in the entire human body via the blood vessel system, particularly the capillary blood vessels. In the human body, complex metabolic pathways exist. Glucose oxidation is a reaction in which, fundamentally, blood sugar reacts with oxygen to produce water, carbon dioxide, and energy. Oxygen herein refers to the oxygen delivered to the cells via blood. The volume of oxygen supply is determined by the blood hemoglobin concentration, the hemoglobin oxygen saturation, and the volume of blood flow. On the other hand, the heat produced in the body by glucose oxidation is dissipated from the body by convection, heat radiation, conduction, and so on. On the assumption that the body temperature is determined by the balance between the amount of energy produced in the body by glucose burning, namely heat production, and heat dissipation such as mentioned above, we set up the following model:

- (1) The amount of heat production and the amount of heat dissipation are considered equal.
- (2) The amount of heat production is a function of the blood glucose concentration and the volume of oxygen supply.
- (3) The volume of oxygen supply is determined by the blood hemoglobin concentration, the blood hemoglobin oxygen saturation, and the volume of blood flow in the capillary blood vessels.
- (4) The amount of heat dissipation is mainly determined by heat convection and heat radiation.

According to this model, we achieved the present invention after realizing that blood sugar levels can be accurately determined on the basis of the results of measuring the temperature of the body surface and measuring parameters relating to the blood oxygen concentration and measuring parameter relating to the blood flow volume. The parameters can be measured from a part of the human body, such as the fingertip. The parameters relating to convection and radiation can be determined by carrying out thermal measurements on the fingertip. The parameters relating to the blood hemoglobin concentration and the blood hemoglobin oxygen saturation can be determined by spectroscopically measuring the blood hemoglobin and then finding the ratio between the hemoglobin bound with oxygen and the hemoglobin not bound with oxygen. The parameter relating to the volume of blood flow can be determined by measuring the amount of heat transfer from the skin.

In one aspect, the invention provides a blood sugar level measuring apparatus comprising:

a heat amount measuring unit for measuring a plurality of temperatures derived from a body surface in order to obtain information used for calculating the amount of convective

heat transfer and the amount of radiation heat transfer concerning the dissipation of heat from the body surface;

an oxygen volume measuring unit for obtaining information concerning the volume of blood oxygen;

a storage unit for storing the relationships between blood sugar levels and individual parameters corresponding to both the multiple temperatures and blood oxygen volume;

a computing unit for converting the measurement values provided by the heat amount measuring unit and the oxygen volume measuring unit into parameters, and computing a blood sugar level by applying the parameters to the relationships stored in the storage unit; and

a display unit for displaying the blood sugar level computed by the computing unit.

Preferably, the heat amount measuring unit may comprise an ambient temperature detector for measuring the ambient temperature, and a radiation temperature detector for measuring the radiation heat from the body surface.

Preferably, the oxygen volume measuring unit may comprise a blood flow volume measuring unit for obtaining information concerning the volume of blood flow, and an optical measuring unit for obtaining blood hemoglobin concentration and hemoglobin oxygen saturation.

In another aspect, the invention provides a blood sugar level measuring apparatus comprising:

a temperature measuring unit for measuring a plurality of temperatures from a body surface;

a blood flow volume measuring unit for obtaining information concerning the volume of blood flow based on the results of measurement by the temperature measuring unit;

an oxygen volume measuring unit for determining the volume of blood oxygen based on the result of measurement by the blood flow volume measuring unit;

a storage unit for storing the relationships between blood sugar levels and individual parameters corresponding to the multiple temperatures, the volume of blood oxygen and the volume of blood flow;

a computing unit for converting the measurement values provided by the temperature measuring unit, the blood flow volume measuring unit and the oxygen volume measuring unit into parameters, and computing a blood sugar level by applying the parameters to the relationships stored in the storage unit; and

a display unit for displaying the blood sugar level computed by the computing unit.

In yet another aspect, the invention provides a blood sugar level measuring apparatus comprising:

an ambient temperature measuring unit for measuring the ambient temperature;

a body-surface contact unit to be brought into contact with a body surface;

a radiation heat detector for measuring the radiation heat from the body surface;

a heat conducting member disposed in contact with the body-surface contact unit;

an indirect temperature detector disposed adjacent the heat conducting member and away from the body-surface contact unit for detecting the temperature at a position distanced away from the body-surface contact unit;

a light source for irradiating the body-surface contact unit with light of at least two different wavelengths;

a photodetector for detecting reflected light produced as the light from the light source is reflected by the body surface;

a computing unit comprising a converting portion and a processing portion, wherein the converting portion converts the outputs of the indirect temperature detector, the ambient

temperature measuring unit, the radiation heat detector, and the photodetector into individual parameters, and wherein the processing portion stores the relationships between the parameters and blood sugar levels in advance and computes a blood sugar level by applying the parameters to the stored relationships; and

a display unit for displaying the blood sugar level produced by the computing unit.

In yet another aspect, the invention provides a blood sugar level measuring apparatus comprising:

an ambient temperature measuring unit for measuring the ambient temperature;

a body-surface contact unit to be brought into contact with a body surface;

a heat conducting member disposed in contact with a first region of the body-surface contact unit;

an indirect temperature detector disposed adjacent the heat conductive member and away from the body-surface contact unit for detecting the temperature at a position distanced away from the body-surface contact unit;

a cylindrical member disposed in contact with a second region of the body-surface contact unit and having an opening on one end thereof;

a radiation heat detector disposed adjacent the other end of the cylindrical member for measuring the radiation heat from the body surface;

a light source for irradiating the one end of the cylindrical member with light of at least two different wavelengths;

a photodetector for detecting reflected light produced by the reflection of the light by the body surface;

a computing unit comprising a converting portion and a processing portion, wherein the converting portion converts the outputs of the indirect temperature detector, the ambient temperature measuring unit, the radiation temperature detector, and the photodetector into individual parameters, and wherein the processing portion stores the relationships between the parameters and blood sugar levels in advance and computes a blood sugar level by applying the parameters to the relationships; and

a display unit for displaying the blood sugar level produced by the computing unit.

In accordance with the invention, blood sugar levels can be determined non-invasively with an accuracy similar to that according to the invasive methods according to the prior art.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a model of heat transfer from the body surface to a block.

FIG. 2 plots the measurement values of temperatures T_1 and T_2 as they change with time.

FIG. 3 shows an example of measuring the chronological change in temperature T_3 .

FIG. 4 shows the relationships between measurement values provided by various sensors and the parameters derived therefrom.

FIG. 5 shows an upper plan view of a non-invasive blood sugar level measuring apparatus according to the present invention.

FIG. 6 shows the operating procedure for the apparatus.

FIGS. 7(a) to 7(c) show the measuring unit in detail.

FIG. 8 shows a conceptual chart illustrating the flow of data processing in the apparatus.

FIG. 9 shows the plots of the glucose concentration values calculated according to the present invention and the glucose concentration values measured by the enzymatic electrode method.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

The invention will now be described by way of preferred embodiments thereof with reference made to the drawings.

Initially, the above-mentioned model will be described in more specific terms. Regarding the amount of heat dissipation, convective heat transfer, which is one of the main causes of heat dissipation, is related to temperature difference between the ambient (room) temperature and the body-surface temperature. The amount of heat dissipation due to radiation, another main cause of dissipation, is proportional to the fourth power of the body-surface temperature according to the Stefan-Boltzmann law. Thus, it can be seen that the amount of heat dissipation from the human body is related to the room temperature and the body-surface temperature. Another major factor related to the amount of heat production, oxygen supply, is expressed as the product of hemoglobin concentration, hemoglobin oxygen saturation, and blood flow volume.

The hemoglobin concentration can be measured by the absorbance at the wavelength at which the molar absorbance coefficient of the oxi-hemoglobin is equal to that of the deoxy-hemoglobin (equal-absorbance wavelength). The hemoglobin oxygen saturation can be measured by measuring the absorbance at the equal-absorbance wavelength and the absorbance of at least one different wavelength at which the ratio between the molar absorbance coefficient of the oxi-hemoglobin and that of the deoxy-hemoglobin is known, and then solving simultaneous equations. Namely, the hemoglobin concentration and the hemoglobin oxygen saturation can be obtained by measuring absorbance of at least two wavelengths.

The rest is the blood flow volume, which can be measured by various methods. One example will be described below.

FIG. 1 shows a model for the description of the transfer of heat from the body surface to a solid block having a certain heat capacity when the block is brought into contact with the body surface for a certain time and then separated. The block is made of resin such as plastic or vinyl chloride. In the illustrated example, attention will be focused on the chronological variation of the temperature T_1 of a portion of the block in contact with the body surface, and the chronological variation of the temperature T_2 of a point on the block away from the body surface. The blood flow volume can be estimated by monitoring mainly the chronological variation of the temperature T_2 (of a point on the spatially separated block). The details will be described later.

Before the block comes into contact with the body surface, the temperatures T_1 and T_2 at the two points of the block are equal to the room temperature T_r . When a body-surface temperature T_s is higher than the room temperature T_r , the temperature T_1 swiftly rises due to the transfer of heat from the skin as the block contacts the body surface, and it approaches the body-surface temperature T_s . On the other hand, the temperature T_2 is less than the temperature T_1 as the heat conducted through the block is dissipated from the block surface, and it rises more gradually than the temperature T_1 . The chronological variation of the temperatures T_1 and T_2 depends on the amount of heat transferred from the body surface to the block, which in turn depends on the blood flow volume in the capillary blood vessels under the

skin. If the capillary blood vessels are regarded as a heat exchanger, the heat transfer coefficient from the capillary blood vessels to the surrounding cell tissues is given as a function of the blood flow volume. Thus, by measuring the amount of heat transfer from the body surface to the block by monitoring the chronological variation of the temperatures T_1 and T_2 , the blood flow volume can be estimated. Accordingly, by monitoring the temperature changes in the T_1 and T_2 chronologically, and thus measuring the amount of heat transfer from the body surface to the block, the amount of heat transfer from the capillary blood vessels to the cell tissues can be estimated, so that the blood flow volume can be estimated.

FIG. 2 shows the chronological variation of the measured values of the temperature T_1 at the portion of the block in contact with the body surface and the temperature T_2 at the position on the block away from the body-surface contact position. As the block comes into contact with the body surface, the T_1 measured value swiftly rises, and it gradually drops as the block is brought out of contact.

FIG. 3 shows the chronological variation of the measured value of the temperature T_3 measured by a radiation temperature detector. As the detector detects the temperature due to the radiation from the body surface, it is more sensitive to temperature changes than other sensors. Because radiation heat propagates as an electromagnetic wave, it can transmit temperature changes instantaneously. Thus, by locating the radiation temperature detector near where the block contacts the body surface, as shown in FIG. 7(a) to 7(c) which will be described later, the time of start of contact t_{start} between the block and the body surface, and the time of end of contact t_{end} can be detected by changes in the temperature T_3 . For example, a temperature threshold value is set as shown in FIG. 3. The contact start time t_{start} is when the temperature threshold value is exceeded. The contact end time t_{end} is when the temperature T_3 drops below the threshold. The temperature threshold is set at 32° C., for example.

Then, the T_1 measured value between t_{start} and t_{end} is approximated by an S curve, such as a logistic curve. A logistic curve is expressed by the following equation:

$$T = \frac{b}{1 + c \times \exp(-a \times t)} + d$$

where T is temperature, and t is time.

The measured value can be approximated by determining factors a , b , c , and d by the non-linear least-squares method. For the resultant approximate expression, T is integrated between time t_{start} and time t_{end} to obtain a value S_1 .

Similarly, an integrated value S_2 is calculated from the T_2 measured value. The smaller $(S_1 - S_2)$, the larger the amount of transfer of heat from the finger surface to the position of T_2 . $(S_1 - S_2)$ becomes larger with increasing finger contact time $t_{cont}(=t_{end} - t_{start})$. Thus, $a_5 / (t_{cont} \times (S_1 - S_2))$ is designated as a parameter X_5 indicating the volume of blood flow, where a_5 is a proportionality coefficient.

Thus, it will be seen that the measured data necessary for the determination of blood glucose concentration by the above-described model are the room temperature (ambient temperature), body surface temperature changes, temperature changes in the block brought into contact with the body surface, the temperature due to radiation from the body surface, and the absorbance of at least two wavelengths.

FIG. 4 shows the relationships between the measured values provided by various sensors and the parameters

derived therefrom. A block is brought into contact with the body surface, and chronological change in two kinds of temperatures T_1 and T_2 are measured by two temperature sensors provided at two locations of the block. A radiation temperature T_3 on the body surface and the room temperature T_4 are separately measured. Absorbance A_1 and A_2 are measured at at least two wavelengths related to the absorbance of hemoglobin. The temperatures T_1 , T_2 , T_3 , and T_4 provide parameters related to the volume of blood flow. The temperature T_3 provides a parameter related to the amount of heat transferred by radiation. The temperatures T_3 and T_4 provide parameters related to the amount of heat transferred by convection. The absorbance A_1 provides a parameter related to the hemoglobin concentration. The absorbance A_1 and A_2 provide parameters related to the hemoglobin oxygen saturation.

Hereafter, an example of apparatus for non-invasively measuring blood sugar levels according to the principle of the invention will be described.

FIG. 5 shows a top plan view of the non-invasive blood sugar level measuring apparatus according to the invention. While in this example the skin on the ball of the finger tip is used as the body surface, other parts of the body surface may be used.

On the top surface of the apparatus are provided an operation unit **11**, a measuring unit **12** where the finger to be measured is to be placed, and a display unit **13** for displaying the state of the apparatus, measured values, and so on. The operation unit **11** includes four push buttons **11a** to **11d** for operating the apparatus. The measuring unit **12** has a cover **14** which, when opened (as shown), reveals a finger rest **15** with an oval periphery. The finger rest **15** accommodates an opening end **16** of a radiation temperature sensor, a contact temperature sensor **17**, and an optical sensor unit **18**.

FIG. 6 shows the procedure for operating the apparatus. As one of the buttons on the operation unit is depressed and the apparatus is turned on, an indication "Warming up" is displayed on the LCD while the electronic circuits in the apparatus are being warmed up. At the same time, a check program is activated to automatically check the electric circuits. As the warm-up phase is over, an indication "Place your finger" appears on the LCD. As the user places his or her finger on the finger rest, counting down begins on the LCD. When the countdown is over, an indication "Put your finger away" appears on the LCD. As the user follows the instruction, the LCD indicates "Processing data." Thereafter, the display shows the blood sugar level, which is then stored in an IC card together with the date and time. As the user took notes of the displayed blood sugar level, he or she pushes another button on the operation unit. About one minute later, the apparatus displays a message "Place your finger" on the LCD, thus indicating that the apparatus is ready for the next cycle of measurement.

FIGS. 7(a) to 7(c) show the measuring unit in detail. FIG. 7(a) is a top plan view, FIG. 7(b) is a cross section along line X-X of FIG. 7(a), and FIG. 7(c) is a cross section along line Y-Y of FIG. 7(a).

First, the process of measuring temperature by the non-invasive blood sugar level measuring apparatus according to the invention will be described. In the portion of the measuring unit where the object of measurement (ball of the finger) is to come into contact, a thin plate **21** of a highly heat-conductive material, such as gold, is placed. A bar-shaped heat-conductive member **22** made of material such as polyvinylchloride whose heat conductivity is lower than that of the plate **21** is thermally connected to the plate **21** and extends into the apparatus. The temperature sensors include

a thermistor **23** for measuring the temperature of the plate **21** and acting as an adjacent temperature detector with respect to the measured object. There is also a thermistor **24** for measuring the temperature of the heat-conducting member away from the plate **21** by a certain distance and acting as an indirect temperature detector with respect to the measured object. An infrared lens **25** is disposed inside the apparatus at such a position that the measured object (ball of the finger) placed on the finger rest **15** can be seen through the lens. Below the infrared lens **25** is disposed a pyroelectric detector **27** via an infrared radiation-transmitting window **26**. Another thermistor **28** is disposed near the pyroelectric detector **27**.

Thus, the temperature sensor portion of the measuring unit has four temperature sensors, and they measure four kinds of temperatures as follows:

- (1) Temperature on the finger surface (thermistor **23**): T_1
- (2) Temperature of the heat-conducting member (thermistor **24**): T_2
- (3) Temperature of radiation from the finger (pyroelectric detector **27**): T_3
- (4) Room temperature (thermistor **28**): T_4

The optical sensor unit **18** measures the hemoglobin concentration and the hemoglobin oxygen saturation necessary for the determination of the oxygen supply volume. In order to measure the hemoglobin concentration and the hemoglobin oxygen saturation, absorbance must be measured at at least two wavelengths. FIG. 7(c) shows a configuration for carrying out the two-wavelength measurement using two light sources **33** and **34** and one detector **35**.

The optical sensor unit **18** includes the ends of two optical fibers **31** and **32**. The optical fiber **31** is for optical irradiation, and the optical fiber **32** is for receiving light. As shown in FIG. 7(c), the optical fiber **31** connects to branch fibers **31a** and **31b** that are provided with light-emitting diodes **33** and **34** at the respective ends thereof. The other end of the light-receiving optical fiber **32** is provided with a photodiode **35**. The light-emitting diode **33** emits light with a wavelength of 810 nm, while the light-emitting diode **34** emits light with a wavelength of 950 nm. The wavelength 810 nm is the equal-absorbance wavelength at which the molar absorbance coefficient of the oxy-hemoglobin is equal to that of the deoxy-hemoglobin. The wavelength 950 nm is the wavelength at which the difference between the molar absorbance coefficient of the oxy-hemoglobin and that of the deoxy-hemoglobin is large.

The two light-emitting diodes **33** and **34** emit light in a time-sharing manner such that the finger of the subject is irradiated with the light emitted by the light-emitting diodes **33** and **34** via the irradiating optical fiber **31**. The light shone on the finger is reflected by the skin, enters the light-receiving optical fiber **32**, and is eventually detected by the photodiode **35**. Part of the light reflected by the skin of the finger penetrates the skin and enters into the tissues and is then absorbed by the hemoglobin in the blood flowing in the capillary blood vessels. The measurement data provided by the photodiode **35** has reflectance R , and the absorbance can be approximately calculated by $\log(1/R)$. The finger is thus irradiated with light with the wavelengths of 810 nm and 950 nm, and R is measured for each and also $\log(1/R)$ is calculated for each. Thus, absorbance A_1 and A_2 for wavelengths 810 nm and 950 nm, respectively, are measured.

When the deoxy-hemoglobin concentration is $[Hb]$ and the oxy-hemoglobin concentration is $[HbO_2]$, absorbance A_1 and A_2 are expressed by the following equations:

$$\begin{aligned}
 A_1 &= a \times ([\text{Hb}] \times A_{\text{Hb}}(810 \text{ nm}) + [\text{HbO}_2] \times A_{\text{HbO}_2}(810 \text{ nm})) \\
 &= a \times ([\text{Hb}] + [\text{HbO}_2]) \times A_{\text{HbO}_2}(810 \text{ nm}) \\
 A_2 &= a \times ([\text{Hb}] \times A_{\text{Hb}}(950 \text{ nm}) + [\text{HbO}_2] \times A_{\text{HbO}_2}(950 \text{ nm})) \\
 &= a \times ([\text{Hb}] + [\text{HbO}_2]) \times \left(\left(1 - \frac{[\text{HbO}_2]}{[\text{Hb}] + [\text{HbO}_2]} \right) \times \right. \\
 &\quad \left. A_{\text{Hb}}(950 \text{ nm}) + \frac{[\text{HbO}_2]}{[\text{Hb}] + [\text{HbO}_2]} \times A_{\text{HbO}_2}(950 \text{ nm}) \right)
 \end{aligned}$$

$A_{\text{Hb}}(810 \text{ nm})$ and $A_{\text{Hb}}(950 \text{ nm})$, and $A_{\text{HbO}_2}(810 \text{ nm})$ and $A_{\text{HbO}_2}(950 \text{ nm})$ are the molar absorbance coefficients of the deoxy-hemoglobin and the oxy-hemoglobin, respectively, and are known at the respective wavelengths. The term a is a proportionality coefficient. The hemoglobin concentration $[\text{Hb}] + [\text{HbO}_2]$, and the hemoglobin oxygen saturation $[\text{HbO}_2]/([\text{Hb}] + [\text{HbO}_2])$ can be determined from the above equations as follows:

$$\begin{aligned}
 [\text{Hb}] + [\text{HbO}_2] &= \frac{A_1}{a \times A_{\text{HbO}_2}(810 \text{ nm})} \\
 \frac{[\text{HbO}_2]}{[\text{Hb}] + [\text{HbO}_2]} &= \frac{A_2 \times A_{\text{HbO}_2}(810 \text{ nm}) - A_1 \times A_{\text{Hb}}(950 \text{ nm})}{A_1 \times (A_{\text{HbO}_2}(950 \text{ nm}) - A_{\text{Hb}}(950 \text{ nm}))}
 \end{aligned}$$

In the present example, the hemoglobin concentration and the hemoglobin oxygen saturation are measured by measuring absorbance at two wavelengths. Preferably, however, absorbance may be measured at more than two wavelengths so that the influence of interfering components can be reduced and measurement accuracy can be improved.

FIG. 8 shows the concept of how data is processed in the apparatus. The apparatus according to the present example is equipped with five sensors, namely thermistor 23, thermistor 24, pyroelectric detector 27, thermistor 28, and photodiode 35. The photodiode 35 measures absorbance at wavelengths 810 nm and 950 nm. Thus, the apparatus is supplied with six kinds of measurement values.

The five kinds of analog signals are supplied via individual amplifiers A_1 to A_5 to analog/digital converters AD_1 to AD_5 , where they are converted into digital signals. Based on the digitally converted values, parameters x_i ($i=1, 2, 3, 4, 5$) are calculated. The following are specific descriptions of x_i (where a_1 to a_5 are proportionality coefficients):

Parameter proportional to heat radiation

$$x_1 = a_1 \times (T_3)^4$$

Parameter proportional to heat convection

$$x_2 = a_2 \times (T_4 - T_3)$$

Parameter proportional to hemoglobin concentration

$$x_3 = a_3 \times \left(\frac{A_1}{a \times A_{\text{HbO}_2}(810 \text{ nm})} \right)$$

Parameter proportional to hemoglobin oxygen saturation

$$x_4 = a_4 \times \left(\frac{A_2 \times A_{\text{HbO}_2}(810 \text{ nm}) - A_1 \times A_{\text{Hb}}(950 \text{ nm})}{A_1 \times (A_{\text{HbO}_2}(950 \text{ nm}) - A_{\text{Hb}}(950 \text{ nm}))} \right)$$

Parameter proportional to blood flow volume

$$x_5 = a_5 \times \left(\frac{1}{t_{\text{CONT}} \times (S_1 - S_2)} \right)$$

Then, normalized parameters are calculated from mean values and standard deviations of x_i obtained by actual data pertaining to large numbers of able-bodied people and diabetic patients. A normalized parameter X_i (where $i=1, 2, 3, 4, 5$) is calculated from each parameter x_i according to the following equation:

$$X_i = \frac{x_i - \bar{x}_i}{SD(x_i)}$$

where

x_i : parameter

\bar{x}_i : mean value of the parameter

$SD(x_i)$: standard deviation of the parameter

Using the above five normalized parameters, calculations are conducted for conversion into glucose concentration to be eventually displayed. A program necessary for the processing calculations is stored in a ROM in the microprocessor built inside the apparatus. The memory area required for the processing calculations is ensured in a RAM similarly built inside the apparatus. The results of calculation are displayed on the LCD.

The ROM stores, as a constituent element of the program necessary for the processing calculations, a function for determining glucose concentration C in particular. The function is defined as follows. C is expressed by the below-indicated equation (1), where a_i ($i=0, 1, 2, 3, 4, 5$) is determined from a plurality of pieces of measurement data in advance according to the following procedure:

- (1) A multiple regression equation that indicates the relationship between the normalized parameter and the glucose concentration C is created.
- (2) A normalized equation (simultaneous equation) relating to the normalized parameter is obtained from an equation obtained by the least-squares method.
- (3) Values of coefficient a_i ($i=0, 1, 2, 3, 4, 5$) are determined from the normalized equation and then substituted into the multiple regression equation.

Initially, the regression equation (1) indicating the relationship between the glucose concentration C and the normalized parameters $X_1, X_2, X_3, X_4,$ and X_5 is formulated.

$$\begin{aligned}
 C &= f(X_1, X_2, X_3, X_4, X_5) \\
 &= a_0 + a_1 X_1 + a_2 X_2 + a_3 X_3 + a_4 X_4 + a_5 X_5
 \end{aligned} \tag{1}$$

Then, the least-squares method is employed to obtain a multiple regression equation that would minimize the error with respect to a measured value C_i of glucose concentration according to an enzyme electrode method. When the sum of squares of the residual is D , D is expressed by the following equation (2):

$$\begin{aligned}
 D &= \sum_{i=1}^n d_i^2 \\
 &= \sum_{i=1}^n (C_i - f(X_{i1}, X_{i2}, X_{i3}, X_{i4}, X_{i5}))^2 \\
 &= \sum_{i=1}^n (C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5}))^2
 \end{aligned}
 \tag{2}$$

Because the sum of squares of the residual D becomes minimum when partial differentiation of equation (2) with respect to a_0, a_2, \dots, a_5 gives zero. Thus, we have the following equations:

$$\begin{aligned}
 \frac{\partial D}{\partial a_0} &= -2 \sum_{i=1}^n \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0 \\
 \frac{\partial D}{\partial a_1} &= -2 \sum_{i=1}^n X_{i1} \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0 \\
 \frac{\partial D}{\partial a_2} &= -2 \sum_{i=1}^n X_{i2} \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0 \\
 \frac{\partial D}{\partial a_3} &= -2 \sum_{i=1}^n X_{i3} \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0 \\
 \frac{\partial D}{\partial a_4} &= -2 \sum_{i=1}^n X_{i4} \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0 \\
 \frac{\partial D}{\partial a_5} &= -2 \sum_{i=1}^n X_{i5} \{C_i - (a_0 + a_1 X_{i1} + a_2 X_{i2} + a_3 X_{i3} + a_4 X_{i4} + a_5 X_{i5})\} = 0
 \end{aligned}
 \tag{3}$$

When the mean values of C and X_1 to X_5 are C_{mean} and X_{1mean} to X_{5mean} , respectively, since $X_{imean}=0$ ($i=1$ to 5), equation (4) can be obtained from equation (1) thus:

$$\begin{aligned}
 a_0 &= C_{mean} - a_1 X_{1mean} - a_2 X_{2mean} - \\
 &\quad a_3 X_{3mean} - a_4 X_{4mean} - a_5 X_{5mean} \\
 &= C_{mean}
 \end{aligned}
 \tag{4}$$

The variation and covariation between the normalized parameters are expressed by equation (5). Covariation between the normalized parameter X_i ($i=1$ to 5) and C is expressed by equation (6).

$$\begin{aligned}
 S_{ij} &= \sum_{k=1}^n (X_{ki} - X_{imean})(X_{kj} - X_{jmean}) \\
 &= \sum_{k=1}^n X_{ki} X_{kj} \quad (i, j = 1, 2, \dots, 5) \\
 S_{iC} &= \sum_{k=1}^n (X_{ki} - X_{imean})(C_k - C_{mean}) \\
 &= \sum_{k=1}^n X_{ki}(C_k - C_{mean}) \quad (i = 1, 2, \dots, 5)
 \end{aligned}
 \tag{5}$$

Substituting equations (4), (5), and (6) into equation (3) and rearranging yields simultaneous equation (normalized equation) (7). Solving equation (7) yields a_1 to a_5 .

$$\begin{aligned}
 a_1 S_{11} + a_2 S_{12} + a_3 S_{13} + a_4 S_{14} + a_5 S_{15} &= S_{1C} \\
 a_1 S_{21} + a_2 S_{22} + a_3 S_{23} + a_4 S_{24} + a_5 S_{25} &= S_{2C} \\
 a_1 S_{31} + a_2 S_{32} + a_3 S_{33} + a_4 S_{34} + a_5 S_{35} &= S_{3C} \\
 a_1 S_{41} + a_2 S_{42} + a_3 S_{43} + a_4 S_{44} + a_5 S_{45} &= S_{4C} \\
 a_1 S_{51} + a_2 S_{52} + a_3 S_{53} + a_4 S_{54} + a_5 S_{55} &= S_{5C}
 \end{aligned}
 \tag{7}$$

Constant term a_0 is obtained by means of equation (4). The thus obtained a_i ($i=0, 1, 2, 3, 4, 5$) is stored in ROM at the time of manufacture of the apparatus. In actual mea-

surement using the apparatus, the normalized parameters X_1 to X_5 obtained from the measured values are substituted into regression equation (1) to calculate the glucose concentration C.

Hereafter, an example of the process of calculating the glucose concentration will be described. The coefficients in equation (1) are determined in advance based on large data obtained from able-bodied persons and diabetic patients. The ROM in the microprocessor stores the following formula for the calculation of glucose concentration:

$$C = 99.4 + 18.3 \times X_1 - 20.2 \times X_2 - 23.7 \times X_3 - 22.0 \times X_4 - 25.9 \times X_5$$

X_1 to X_5 are the results of normalization of parameters x_1 to x_5 . Assuming the distribution of the parameters is normal, 95% of the normalized parameter takes on values between -2 to $+2$.

In the case of an able-bodied person, substituting exemplary measurement values in the above equation such that $X_1=-0.06$, $X_2=+0.04$, $X_3=+0.05$, $X_4=-0.12$, and $X_5=+0.10$ yields $C=96$ mg/dl. In the case of a diabetic patient, substituting exemplary measurement values in the equation such that $X_1=+1.15$, $X_2=-1.02$, $X_3=-0.83$, $X_4=-0.91$, and $X_5=-1.24$ yields $C=213$ mg/dl.

Hereafter, the results of measurement by the conventional enzymatic electrode method and those by the method of the invention will be compared. In the enzymatic electrode method, a blood sample is reacted with a reagent and the amount of resultant electrons is measured to determine glucose concentration. When the glucose concentration for

an able-bodied person was 89 mg/dl according to the enzymatic electrode method, the normalized parameters obtained by measurement at the same time according to the invention were $X_1=-0.06$, $X_2=+0.04$, $X_3=+0.05$, $X_4=-0.12$, and $X_5=+0.10$. Substituting these values into the above equation yields $C=96$ mg/dl. On the other hand, when the glucose concentration for a diabetic patient was 238 mg/dl according to the enzymatic electrode method, the normalized parameters obtained by measurement at the same time according to the invention were $X_1=+1.15$, $X_2=-1.02$, $X_3=-0.83$, $X_4=-0.91$, and $X_5=-1.24$. Substituting these values into the above equation yields $C=213$ mg/dl. The results thus indicated that the method according to the invention can provide highly accurate glucose concentration.

FIG. 9 shows the plot of glucose concentration for a plurality of patients. The calculated values of glucose concentration according to the invention are shown on the vertical axis, and the measured values of glucose concentration according to the enzymatic electrode method are shown on the horizontal axis. It will be seen that a good correlation can be obtained by measuring the oxygen supply volume and the blood flow volume according to the method of the invention (correlation coefficient=0.9324).

Thus, the invention can provide a highly accurate non-invasive blood sugar level measuring apparatus and method. What is claimed is:

1. A measuring apparatus for measuring a metabolic characteristic in a human body comprising:

a heat amount measuring unit for measuring a plurality of temperatures derived from the body surface in order to obtain information used for calculating the amount of convective heat transfer and the amount of radiation heat transfer concerning the dissipation of heat from the body surface;

an oxygen volume measuring unit for obtaining information concerning the volume of blood oxygen;

a storage unit for storing the relationships between a metabolic characteristic and the individual parameters corresponding to both the multiple temperatures and blood oxygen volume;

a computing unit for converting the measurement values provided by the heat amount measuring unit and the oxygen volume measuring unit into parameters, and computing the metabolic characteristic by applying the parameters to the relationships stored in the storage unit; and

a display unit for displaying the result computed by the computing unit.

2. The measuring apparatus according to claim 1, wherein the oxygen volume measuring unit comprises a blood flow volume measuring unit for obtaining information concerning the volume of blood flow, and an optical measuring unit for obtaining blood hemoglobin concentration and hemoglobin oxygen saturation.

3. A measuring apparatus for measuring a metabolic characteristic in a human body comprising:

a heat amount measuring unit for measuring a plurality of temperatures derived from the body surface in order to obtain information used for calculating the amount of convective heat transfer and the amount of radiation heat transfer concerning the dissipation of heat from the body surface;

an oxygen volume measuring unit for obtaining information concerning the volume of blood oxygen, wherein volume measuring unit comprises a blood flow volume measuring unit for obtaining information concerning the volume of blood flow, and an optical measuring unit

for obtaining blood hemoglobin concentration and hemoglobin oxygen saturation, wherein the blood flow volume measuring unit comprises a body-surface contact unit; an indirect temperature detector for detecting the temperature at a position distanced away from the body-surface contact unit; and a heat conducting member connecting the body-surface contact unit and the indirect temperature detector

a storage unit for storing the relationships between a metabolic characteristic and the individual parameters corresponding to both the multiple temperatures and blood oxygen volume;

a computing unit for converting the measurement values provided by the heat amount measuring unit and the oxygen volume measuring unit into parameters, and computing the metabolic characteristic by applying the parameters to the relationships stored in the storage unit; and

a display unit for displaying the result computed by the computing unit.

4. The measuring apparatus according to claim 3, wherein the blood flow volume measuring unit further comprises an adjacent temperature detector disposed adjacent the body-surface contact unit.

5. The measuring apparatus according to claim 3, wherein the optical measuring unit comprises:

a light source for generating light of at least two different wavelengths;

an optical system for irradiating the body surface with light emitted by the light source; and

a photodetector for detecting the light reflected by the body surface.

6. The measuring apparatus according to claim 5, wherein the results of detection by the photodetector are used for computing blood hemoglobin concentration and hemoglobin oxygen saturation.

7. The measuring apparatus according to claim 3, wherein the heat amount measuring unit comprises:

an ambient temperature detector for measuring the ambient temperature; and

a radiation temperature detector for measuring the radiation heat from the body surface.

8. A non-invasive metabolic characteristic measuring apparatus comprising:

a temperature measuring unit for measuring a plurality of temperatures from a body surface;

a blood flow volume measuring unit for obtaining information concerning the volume of blood flow based on the results of measurement by the temperature measuring unit;

an oxygen volume measuring unit for determining the volume of blood oxygen based on the result of measurement by the blood flow volume measuring unit;

a storage unit for storing the relationships between a metabolic characteristic and individual parameters corresponding to the multiple temperatures, the volume of blood oxygen and the volume of blood flow;

a computing unit for converting the measurement values provided by the temperature measuring unit, the blood flow volume measuring unit and the oxygen volume measuring unit into parameters, and computing the metabolic characteristic by applying the parameters to the relationships stored in the storage unit; and

a display unit for displaying the result computed by the computing unit.

15

9. The measuring apparatus according to claim 8, wherein the blood flow volume measuring unit comprises:

- a body-surface contact unit;
- an adjacent temperature detector disposed adjacent the body-surface contact unit;
- an indirect temperature detector for detecting the temperature at a position distanced away from the body-surface contact unit; and
- a heat conducting member connecting the body-surface contact unit and the indirect temperature detector.

10. The measuring apparatus according to claim 8, further comprising an optical measuring unit, the oxygen volume measuring unit comprising:

- a light source for generating light of at least two different wavelengths;
- an optical system for irradiating the body surface with light emitted by the light source; and
- a photodetector for detecting the light reflected by the body surface, wherein the oxygen volume measuring unit further employs the result of detection by the photodetector in determining the volume of blood oxygen.

11. The measuring apparatus according to claim 10, wherein the result of detection by the photodetector is used in calculating the blood hemoglobin concentration and hemoglobin oxygen saturation.

12. A measuring apparatus for measuring a metabolic characteristic in a human body comprising:

- an ambient temperature measuring unit for measuring the ambient temperature;
- a body-surface contact unit to be brought into contact with a body surface;
- a radiation heat detector for measuring the radiation heat from the body surface;
- a heat conducting member disposed in contact with the body-surface contact unit;
- an indirect temperature detector disposed adjacent the heat conducting member and away from the body-surface contact unit for detecting the temperature at a position distanced away from the body-surface contact unit;
- a computing unit comprising a converting portion and a processing portion, wherein the converting portion converts the outputs of the indirect temperature detector, the ambient temperature measuring unit, and the radiation heat detector into individual parameters, and wherein the processing portion stores the relationships between the parameters and the metabolic characteristic in advance and computes the metabolic characteristic by applying the parameters to the stored relationships; and
- a display unit for displaying the result produced by the computing unit.

13. A measuring apparatus according to claim 12, further comprising a light source for irradiating the body-surface contact unit with light of at least two different wavelengths; a photodetector for detecting reflected light produced as the light from the light source is reflected by the body surface;

- and the converting portion converts outputs of the indirect temperature detector, the ambient temperature measuring unit, the radiation heat detector, and the photodetector into individual parameters.

14. The measuring apparatus according to claim 13, wherein the light is used for measuring the blood hemoglobin concentration and hemoglobin oxygen saturation.

16

15. The measuring apparatus according to claim 13, further comprising:

- a first optical fiber connecting the light source and the body-surface contact unit; and
- a second optical fiber connecting the body-surface contact unit and the photodetector, wherein the body surface is irradiated with the light from the light source transmitted via the first optical fiber, and the reflected light is guided to the photodetector via the second optical fiber.

16. The measuring apparatus according to claim 12, further comprising:

- a plate adapted to cover an opening end of the heat conducting member in contact with the body-surface contact unit; and
- an adjacent temperature detector for detecting the temperature of the plate, wherein the output of the adjacent temperature detector is converted into a parameter by the converter unit.

17. The measuring apparatus according to claim 16, wherein the thermal conductivity of the plate is higher than that of the heat conducting member.

18. The measuring apparatus according to claim 12, further comprising an infrared lens disposed between the body-surface contact unit and the indirect temperature detector.

19. A measuring apparatus for measuring a metabolic characteristic in a human body comprising:

- an ambient temperature measuring unit for measuring the ambient temperature;
- a body-surface contact unit to be brought into contact with a body surface;
- a heat conducting member disposed in contact with a first region of the body-surface contact unit;
- an indirect temperature detector disposed adjacent the heat conductive member and away from the body-surface contact unit for detecting the temperature at a position distanced away from the body-surface contact unit;
- a cylindrical member disposed in contact with a second region of the body-surface contact unit and having an opening on one end thereof;
- a radiation heat detector disposed adjacent the other end of the cylindrical member for measuring the radiation heat from the body surface;
- a light source for irradiating the one end of the cylindrical member with light of at least two different wavelengths;
- a photodetector for detecting reflected light produced by the reflection of the light by the body surface;
- a computing unit comprising a converting portion and a processing portion, wherein the converting portion converts the outputs of the indirect temperature detector, the ambient temperature measuring unit, the radiation temperature detector, and the photodetector into individual parameters, and wherein the processing portion stores the relationships between the parameters and a metabolic characteristic in advance and computes the metabolic characteristic by applying the parameters to the relationships; and
- a display unit for displaying the result produced by the computing unit.

20. The measuring apparatus according to claim 19, wherein the first and the second regions are disposed adjacent to each other.

17

21. The measuring apparatus according to claim 19, further comprising:

a first optical fiber connecting the light source and the one end of the cylindrical member; and

a second optical fiber connecting the one end and the photodetector, wherein

the light emitted by the light source is guided through the first optical fiber and is then shone on the body surface,

18

and the reflected light is guided through the second optical fiber onto the photodetector.

22. The measuring apparatus according to claim 19, further comprising an infrared lens disposed between the second region and the indirect temperature detector.

* * * * *

专利名称(译)	用于测量人体内代谢特征的测量装置		
公开(公告)号	US7254430	公开(公告)日	2007-08-07
申请号	US11/169777	申请日	2005-06-30
[标]申请(专利权)人(译)	CHO OK KYUNG 金伦		
申请(专利权)人(译)	CHO OK-KYUNG 金润玉		
当前申请(专利权)人(译)	HITACHI, LTD.		
[标]发明人	CHO OK KYUNG KIM YOON OK		
发明人	CHO, OK-KYUNG KIM, YOON-OK		
IPC分类号	A61B5/00 G01N33/48 A61B5/01 A61B5/026 A61B5/028 A61B5/145 A61B5/1455 G01N21/27 G01N33/66		
CPC分类号	A61B5/14532 A61B5/01 A61B5/0261 A61B5/1455		
优先权	2003129020 2003-05-07 JP		
其他公开文献	US20050251000A1		
外部链接	Espacenet USPTO		

摘要(译)

基于温度测量，非侵入性地测量血糖水平。通过血液氧饱和度和血流量校正通过无创测量温度获得的血糖水平，从而可以稳定测量数据。

