


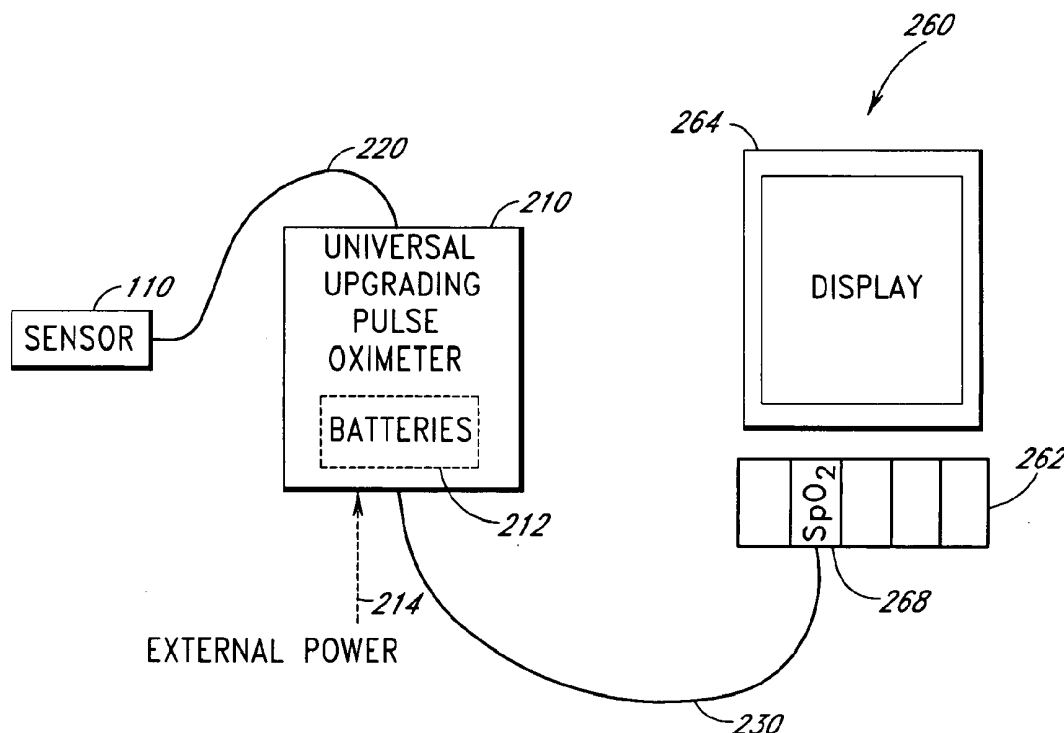

US 20110288384A1

(19) **United States**(12) **Patent Application Publication**  
**Ali et al.**(10) **Pub. No.: US 2011/0288384 A1**(43) **Pub. Date: Nov. 24, 2011**(54) **SYSTEMS AND METHODS FOR ACQUIRING  
CALIBRATION DATA USABLE IN A PULSE  
OXIMETER**(75) Inventors: **Ammar Al Ali**, San Juan  
Capistrano, CA (US); **Don**  
**Carothers**, Mission Viejo, CA  
(US); **David Dalke**, Irvine, CA  
(US); **Mohamed K. Diab**, Ladera  
Ranch, CA (US); **Julian Goldman**,  
Irvine, CA (US); **Massi E. Kiani**,  
Laguna Niguel, CA (US); **Michael**  
**Lee**, Aliso Viejo, CA (US); **Jerome**  
**Novak**, Aliso Viejo, CA (US);  
**Robert Smith**, Lake Forest, CA  
(US); **Val E. Vaden**, Hillsborough,  
CA (US)(73) Assignee: **MASIMO CORPORATION**,  
Irvine, CA (US)(21) Appl. No.: **13/196,732**(22) Filed: **Aug. 2, 2011****Related U.S. Application Data**(63) Continuation of application No. 11/431,151, filed on  
May 8, 2006, now Pat. No. 7,991,446, which is acontinuation of application No. 10/420,994, filed on  
Apr. 22, 2003, now Pat. No. 7,428,432, which is a  
continuation of application No. 10/153,263, filed on  
May 21, 2002, which is a continuation of application  
No. 09/516,110, filed on Mar. 1, 2000, now Pat. No.  
6,584,336, which is a continuation of application No.  
09/491,175, filed on Jan. 25, 2000, now abandoned.(60) Provisional application No. 60/117,097, filed on Jan.  
25, 1999, provisional application No. 60/161,565,  
filed on Oct. 26, 1999.**Publication Classification**(51) **Int. Cl.**  
**A61B 5/00** (2006.01)(52) **U.S. Cl.** ..... **600/301; 600/300**(57) **ABSTRACT**

The present disclosure includes a pulse oximeter attachment having an accessible memory. In one embodiment, the pulse oximeter attachment stores calibration data, such as, for example, calibration data associated with a type of a sensor, a calibration curve, or the like. The calibration data is used to calculate physiological parameters of pulsing blood.



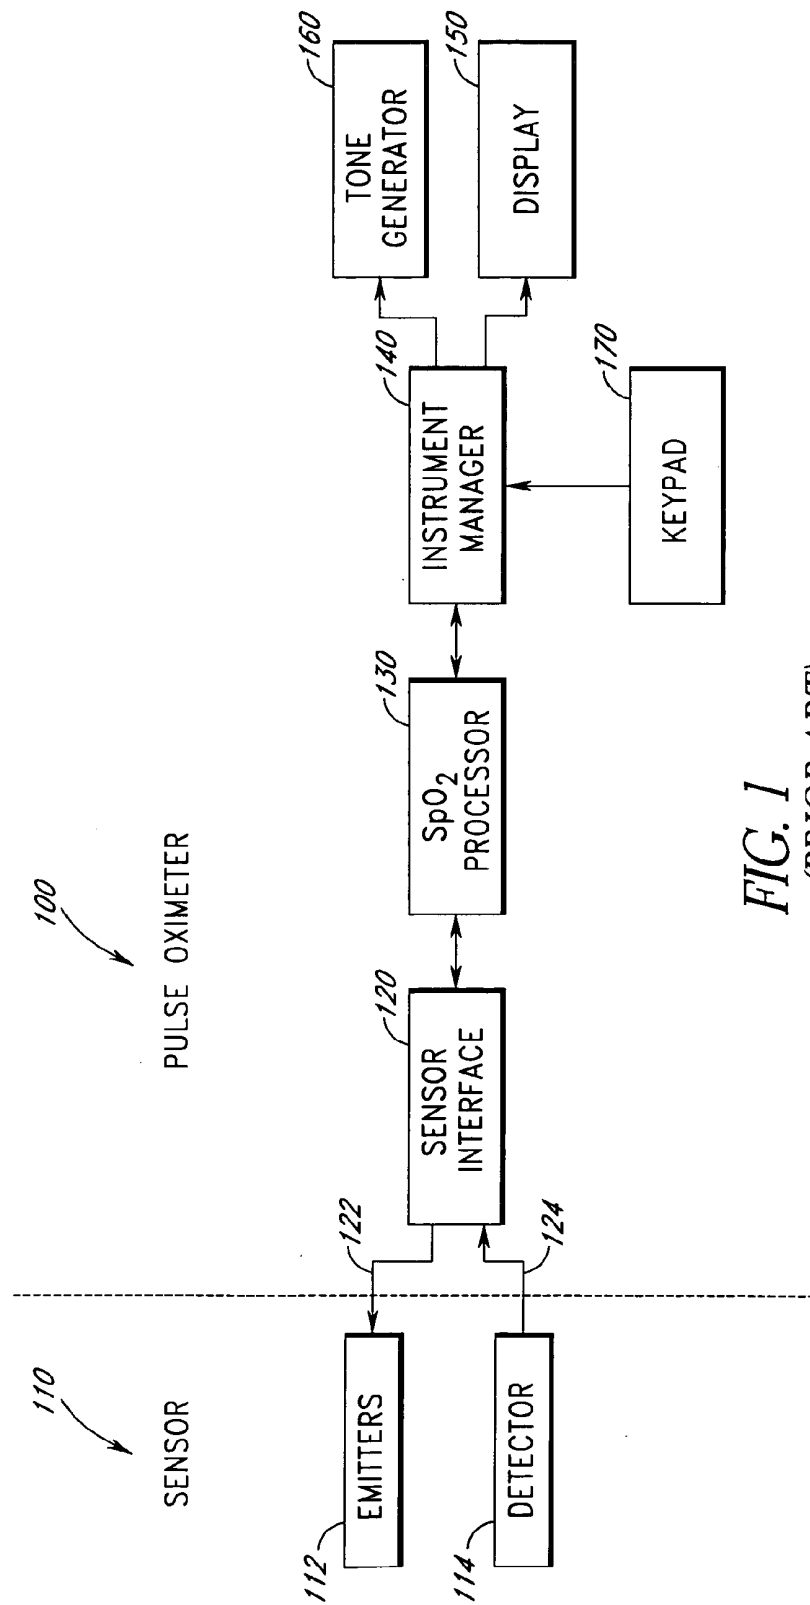


FIG. 1  
(PRIOR ART)

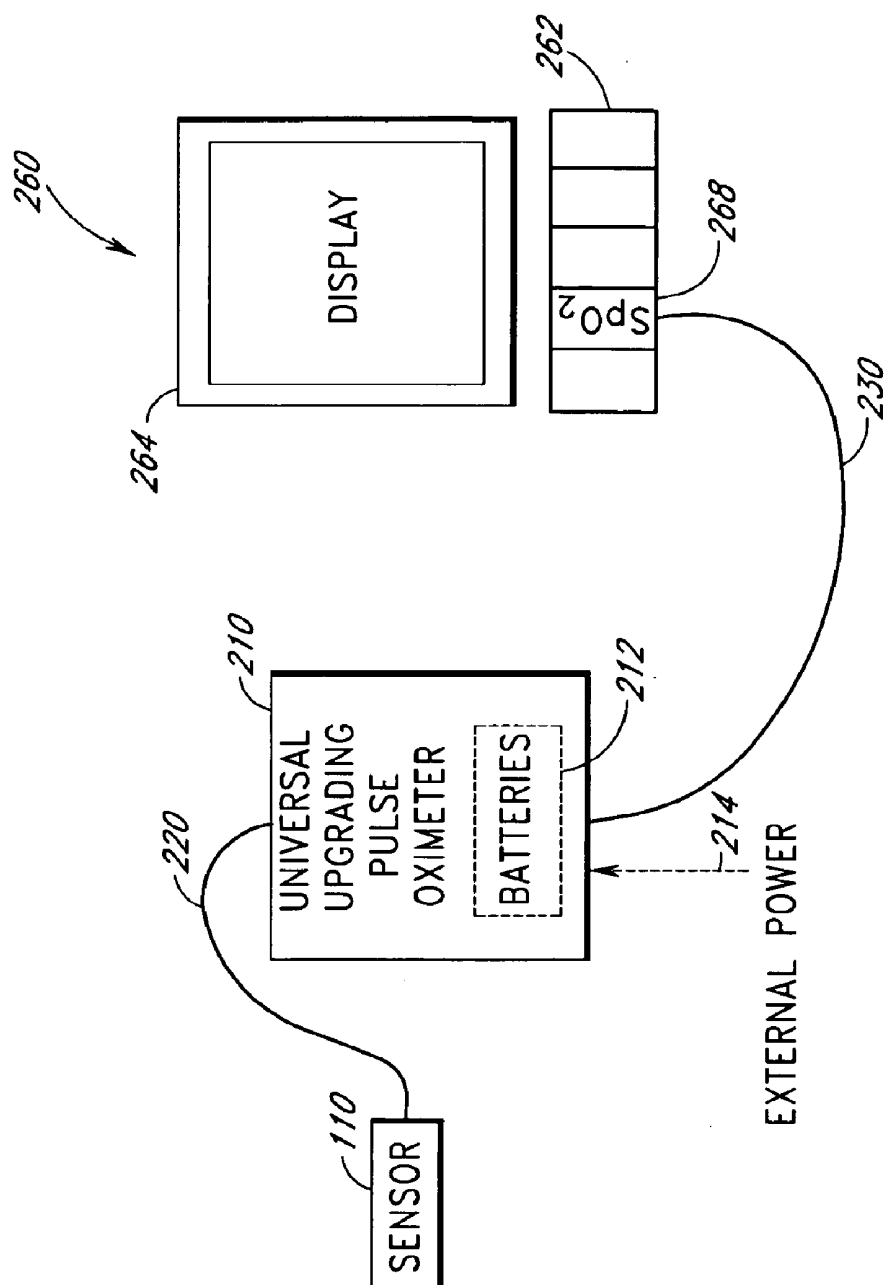


FIG. 2

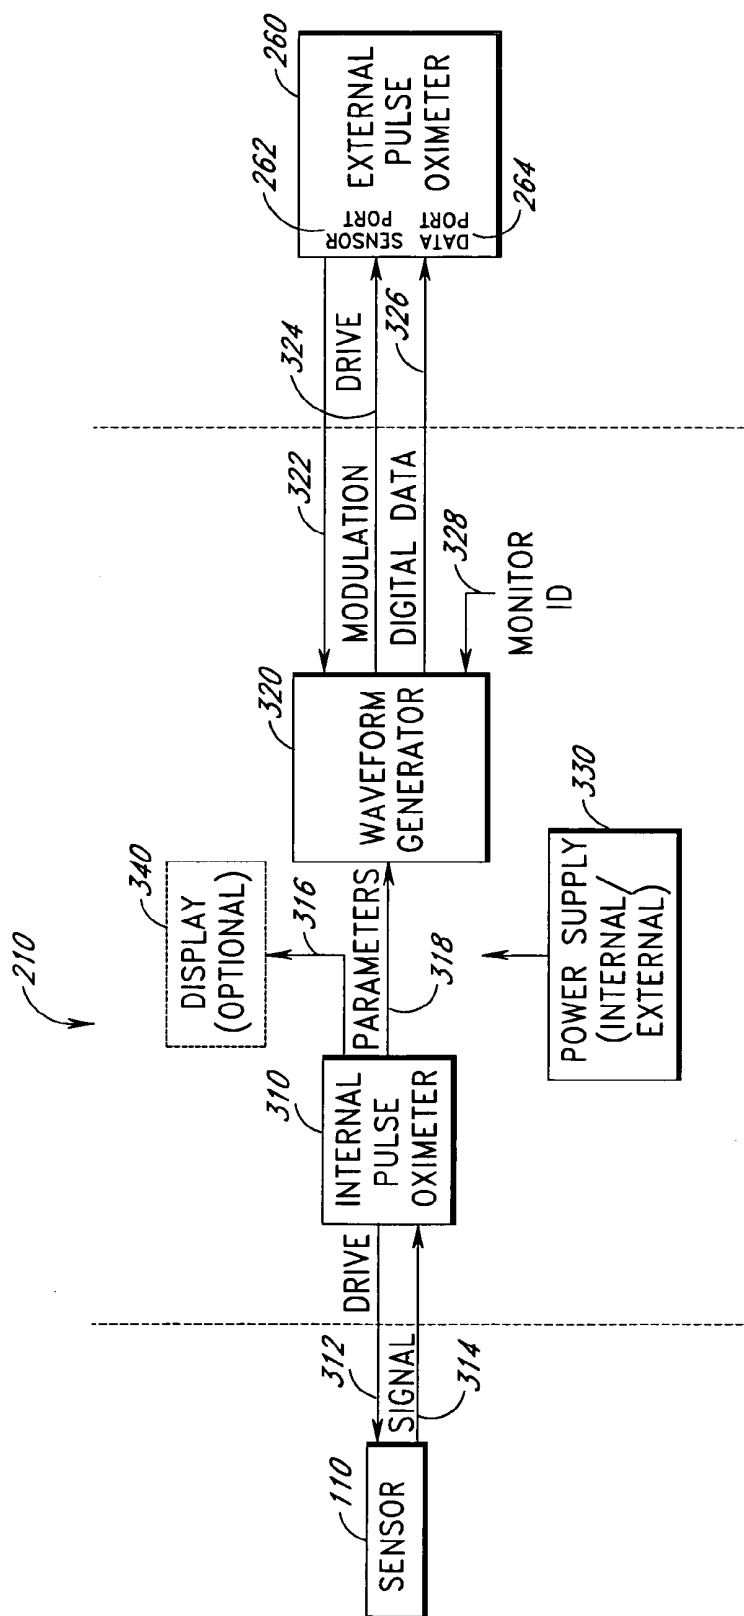


FIG. 3

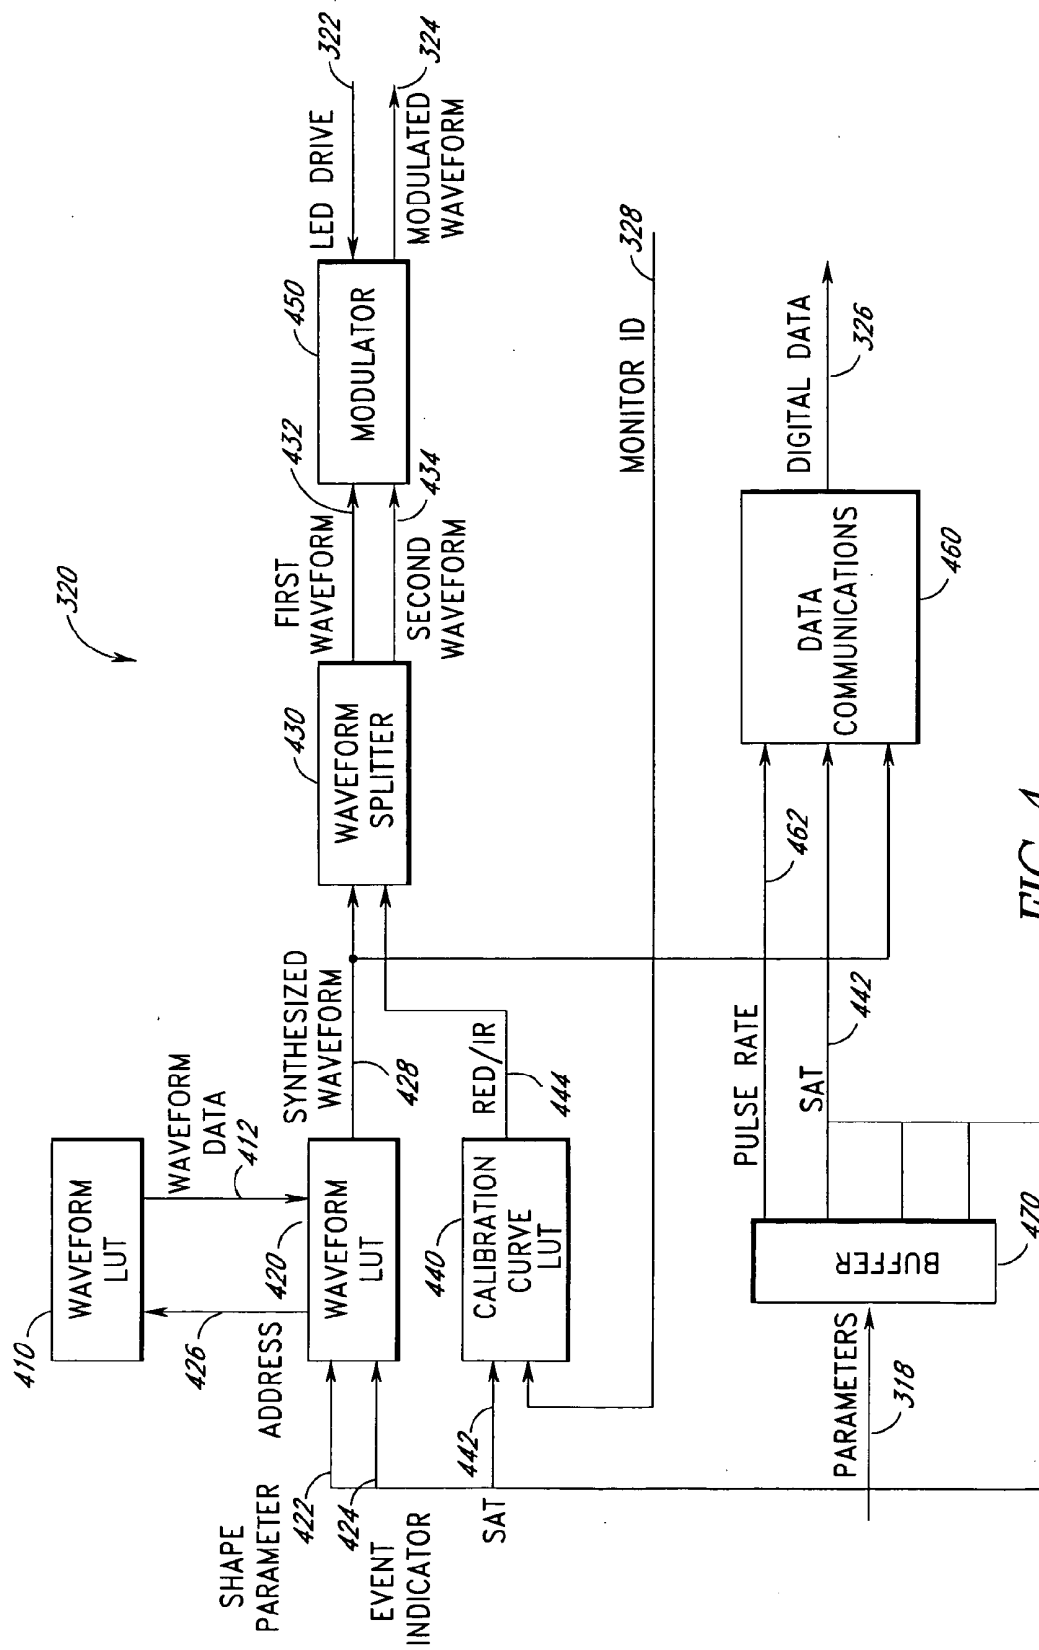


FIG. 4

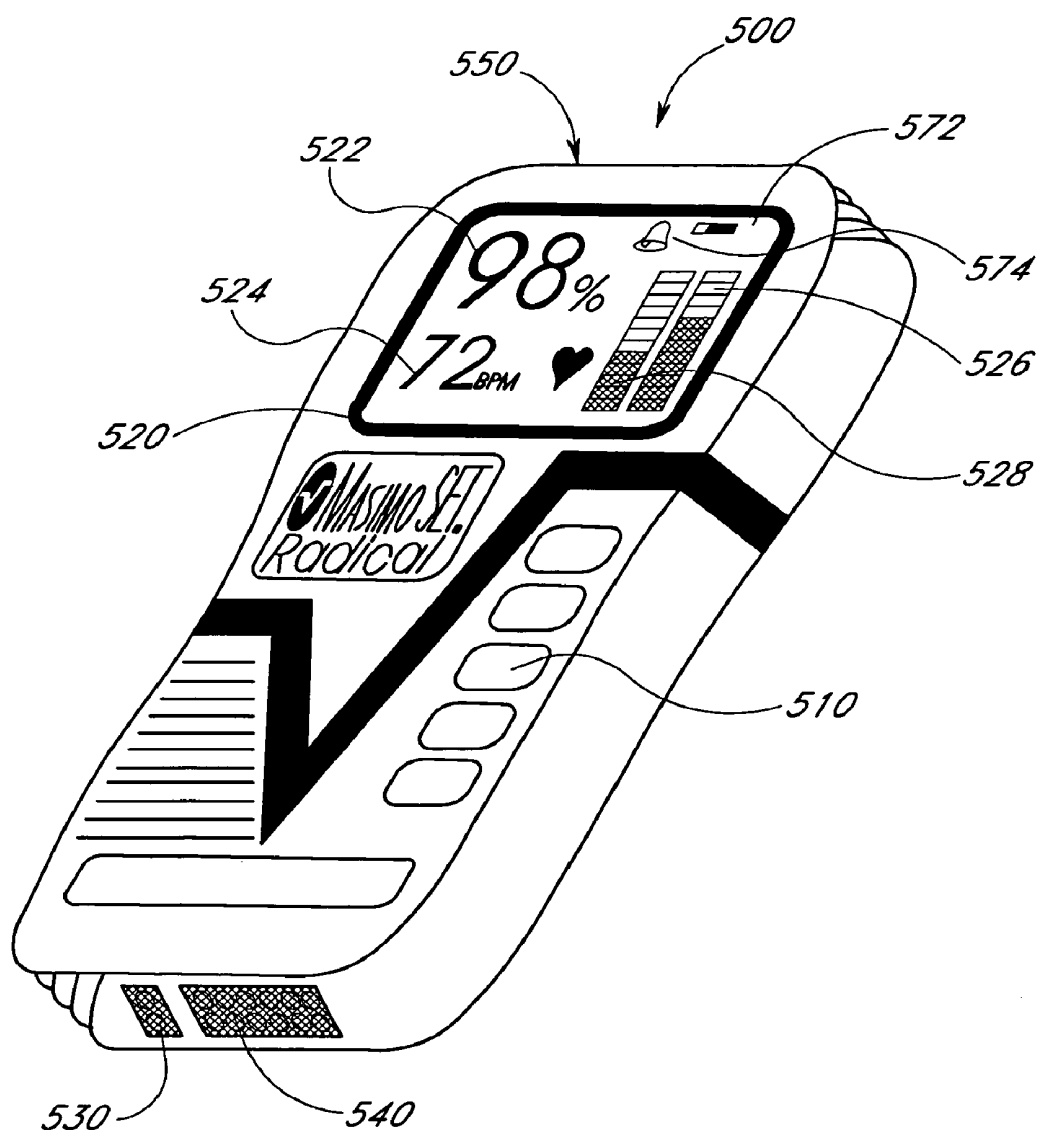


FIG. 5

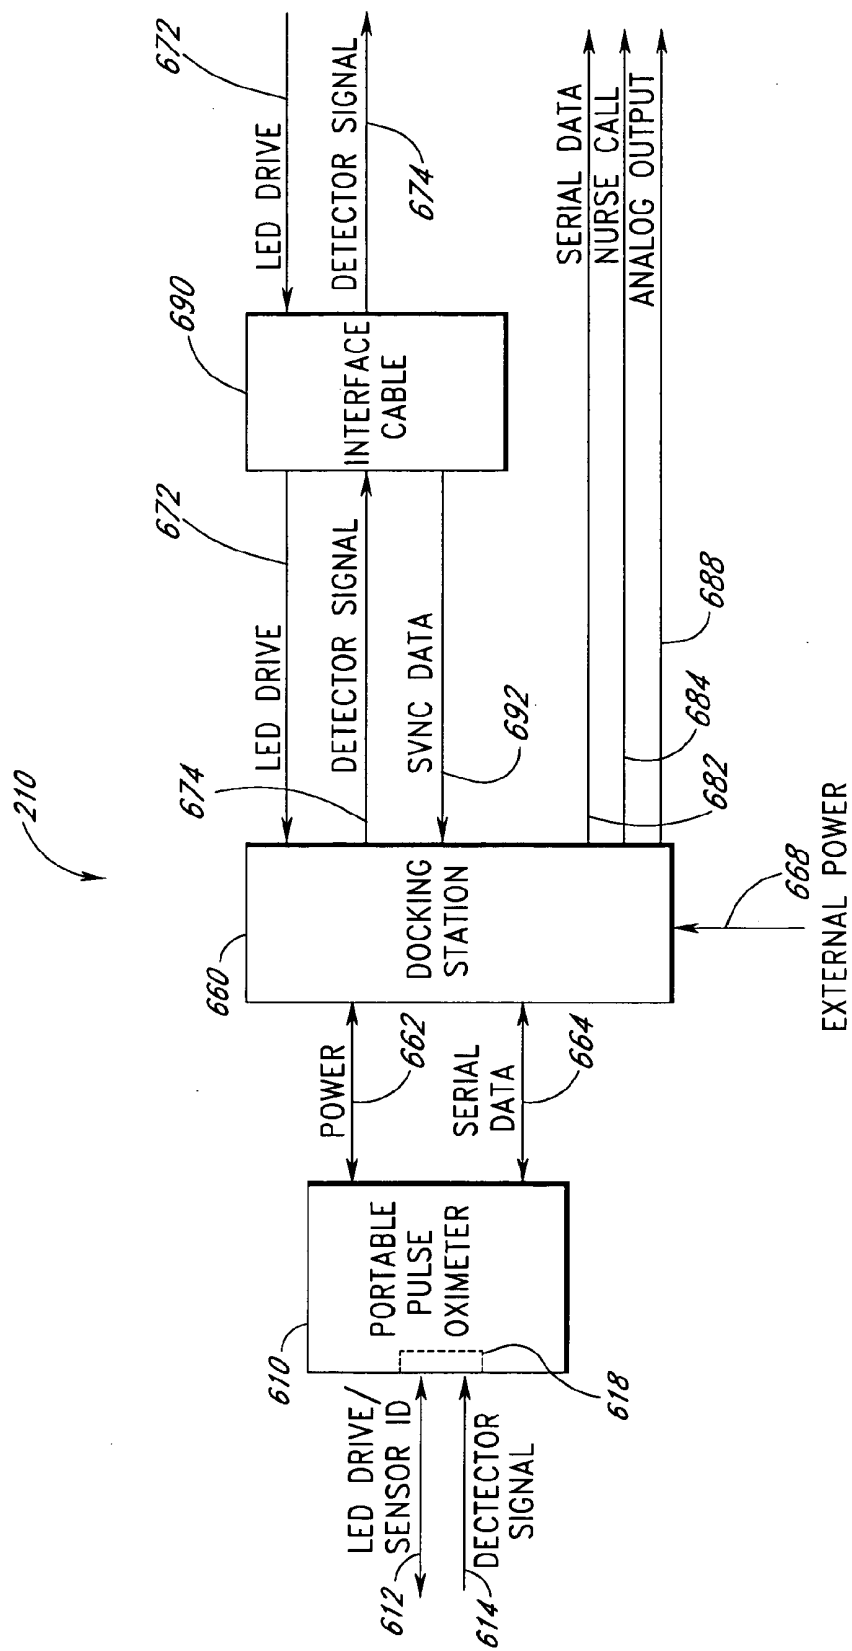


FIG. 6

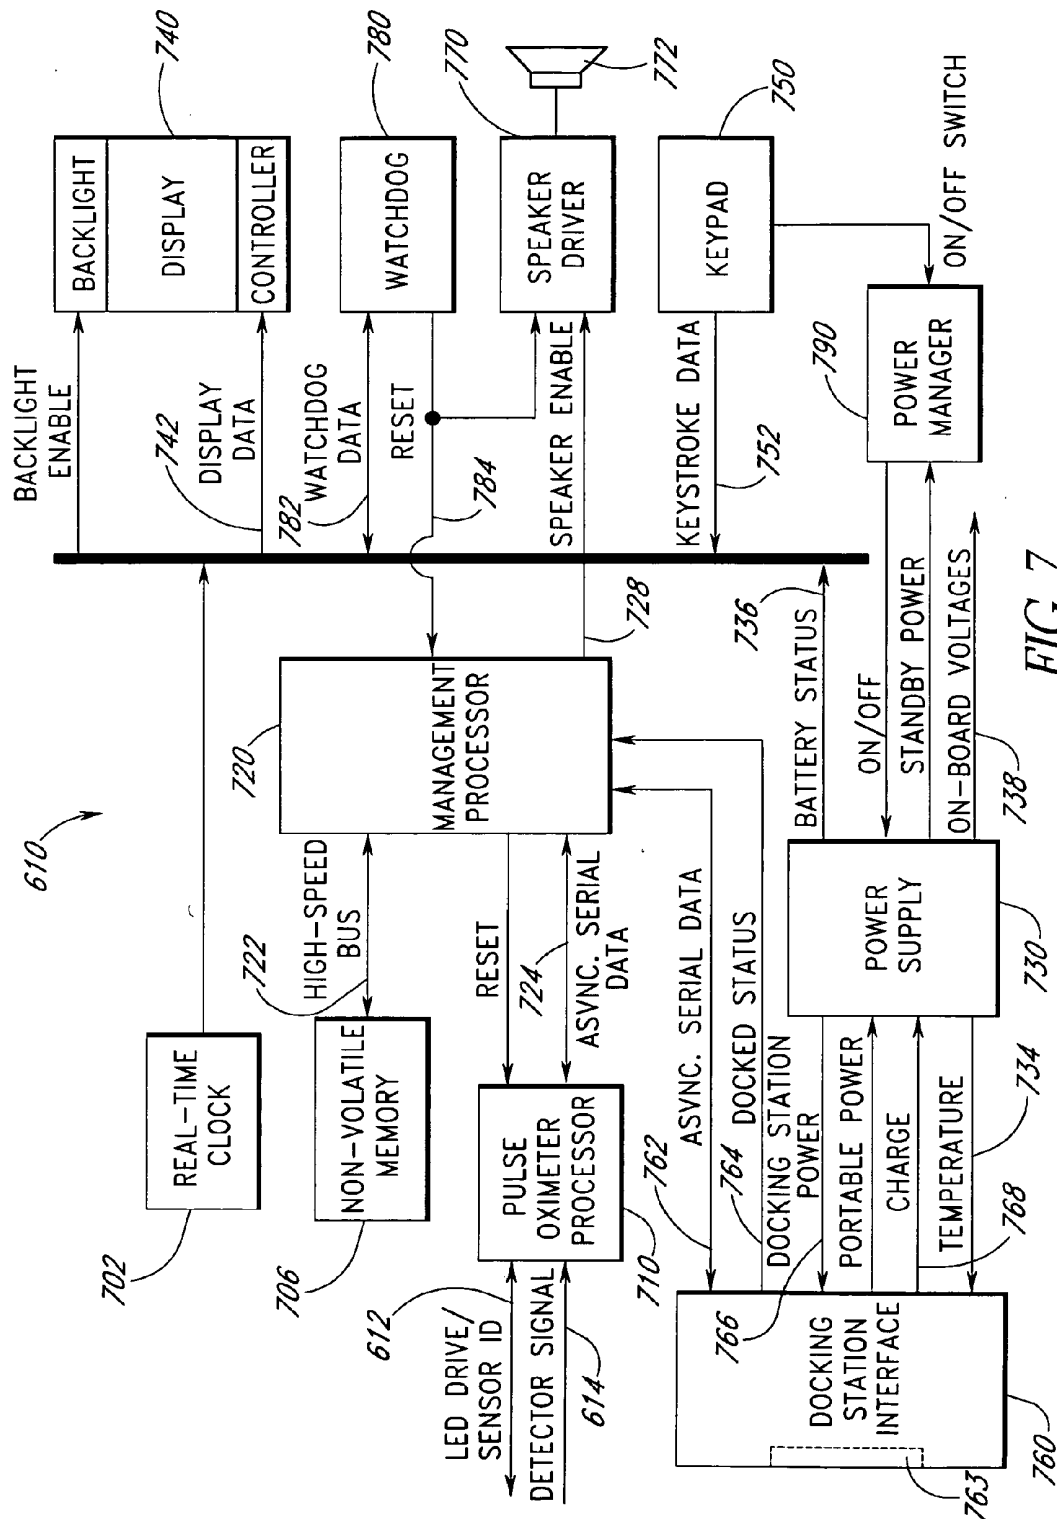


FIG. 7



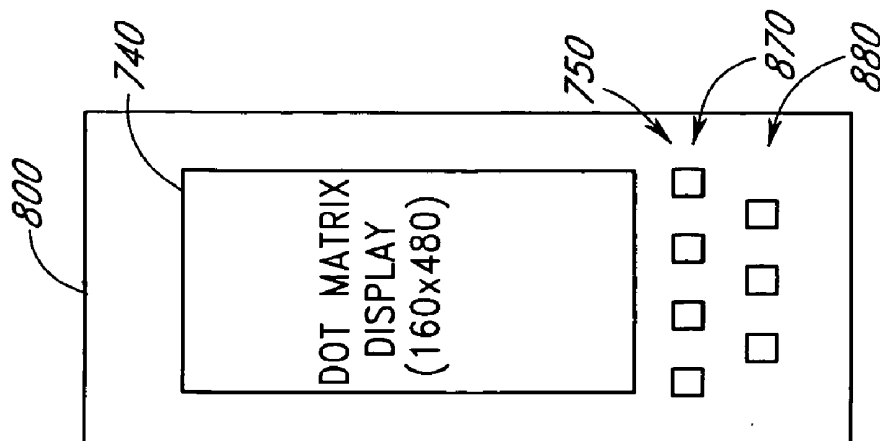


FIG. 8A

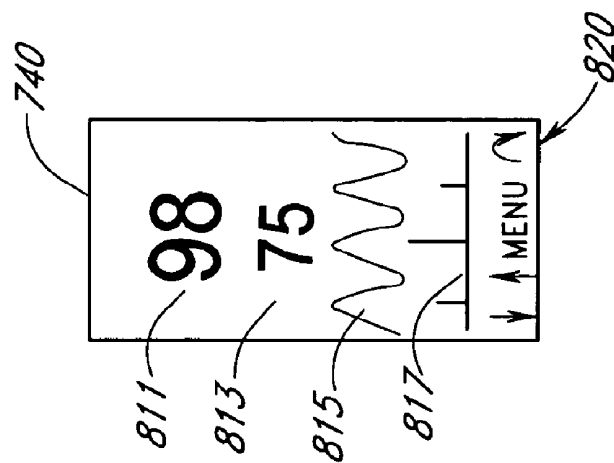


FIG. 8B

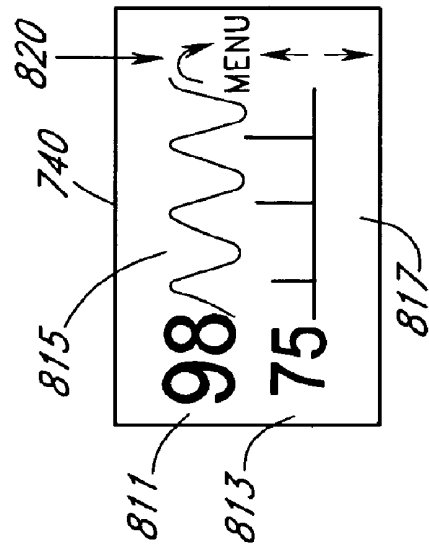


FIG. 8C

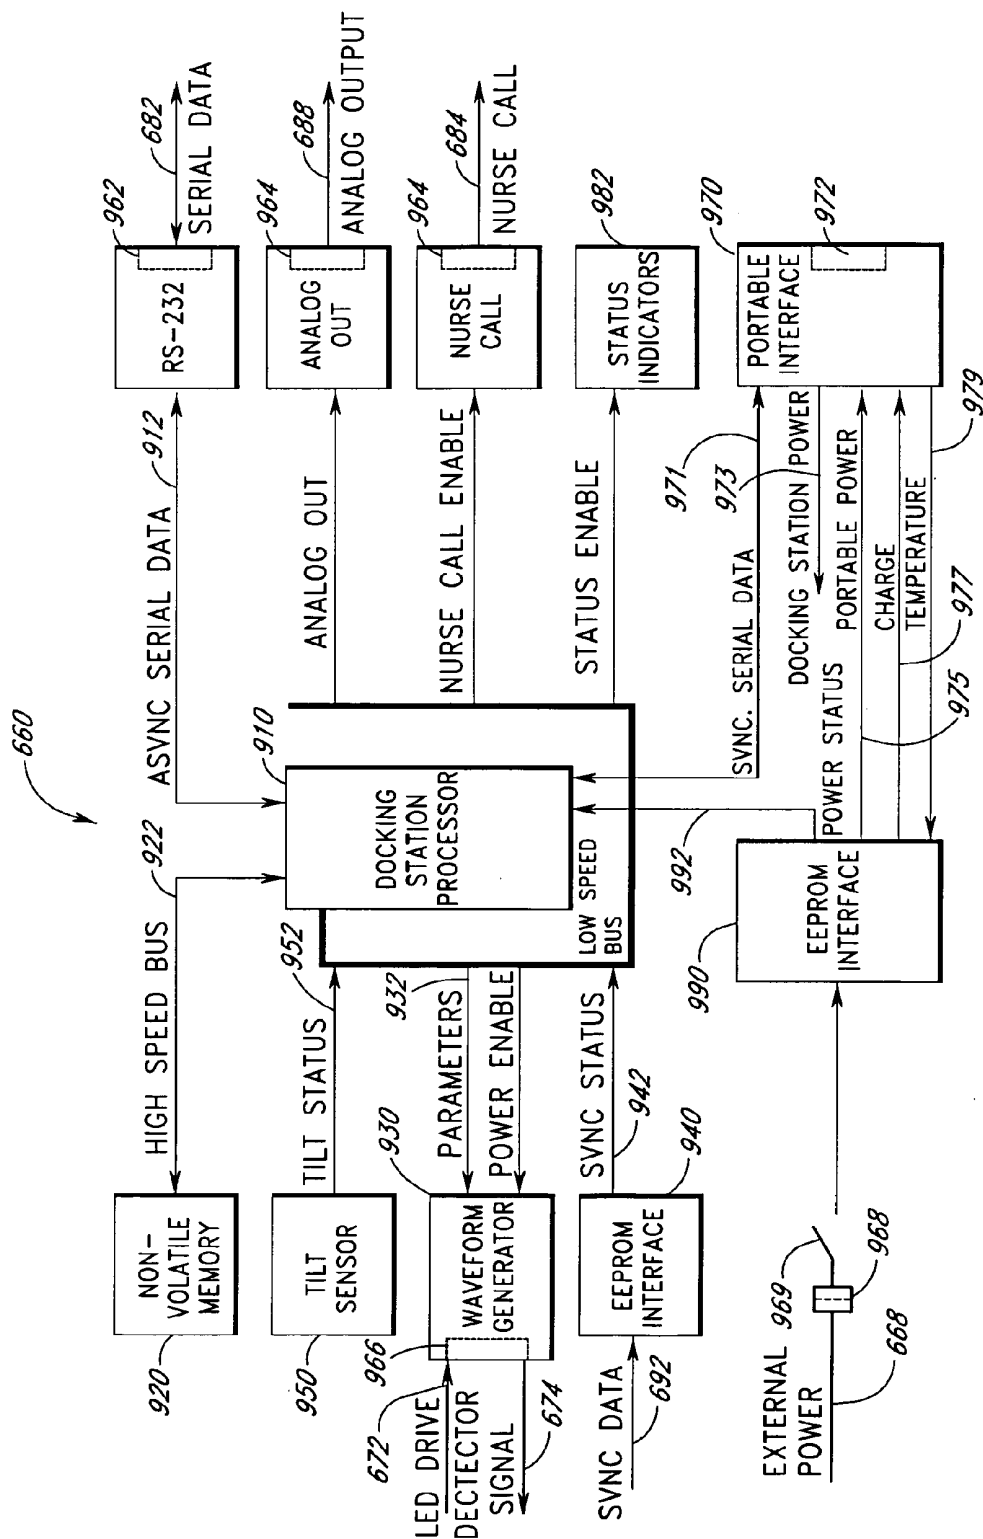


FIG. 9

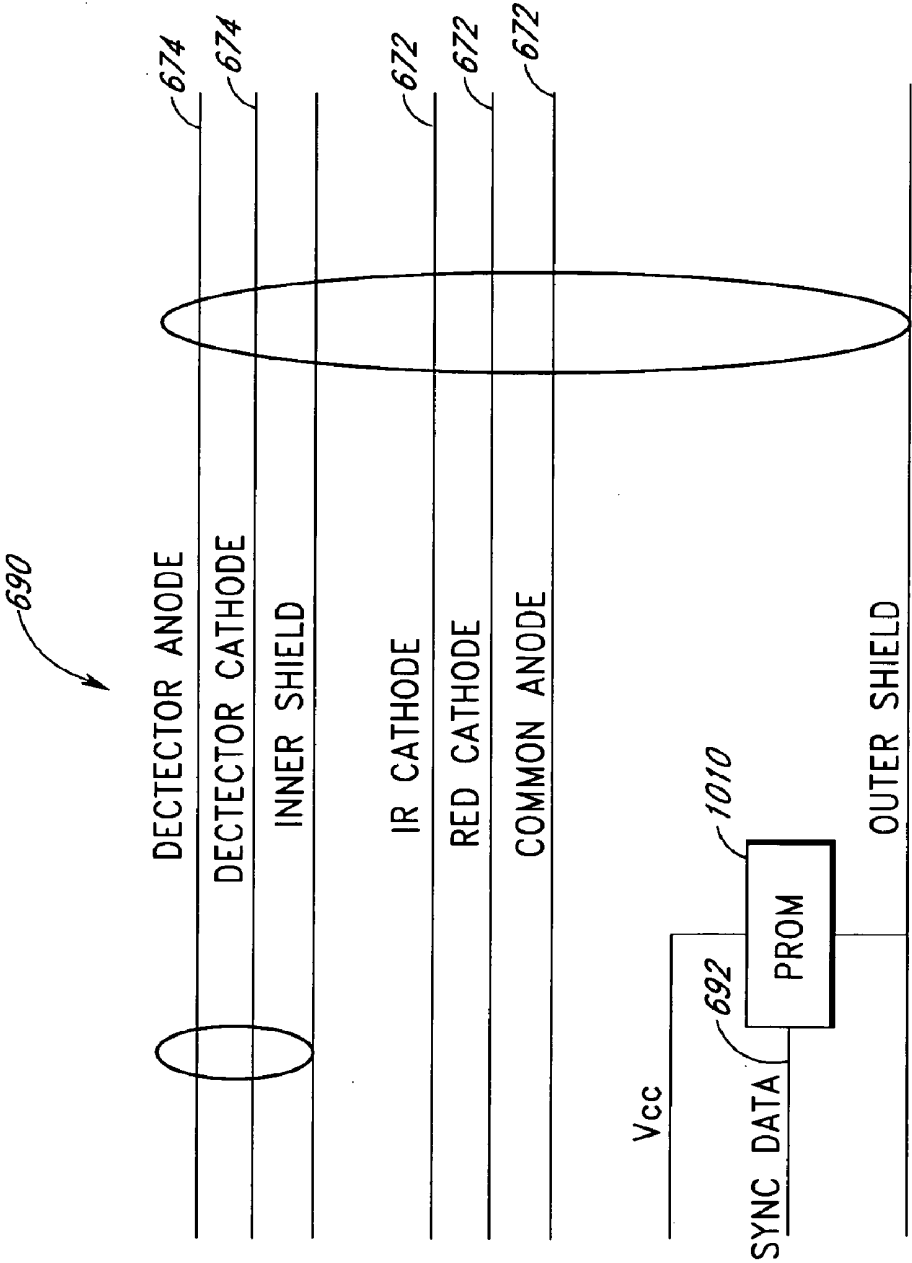


FIG. 10

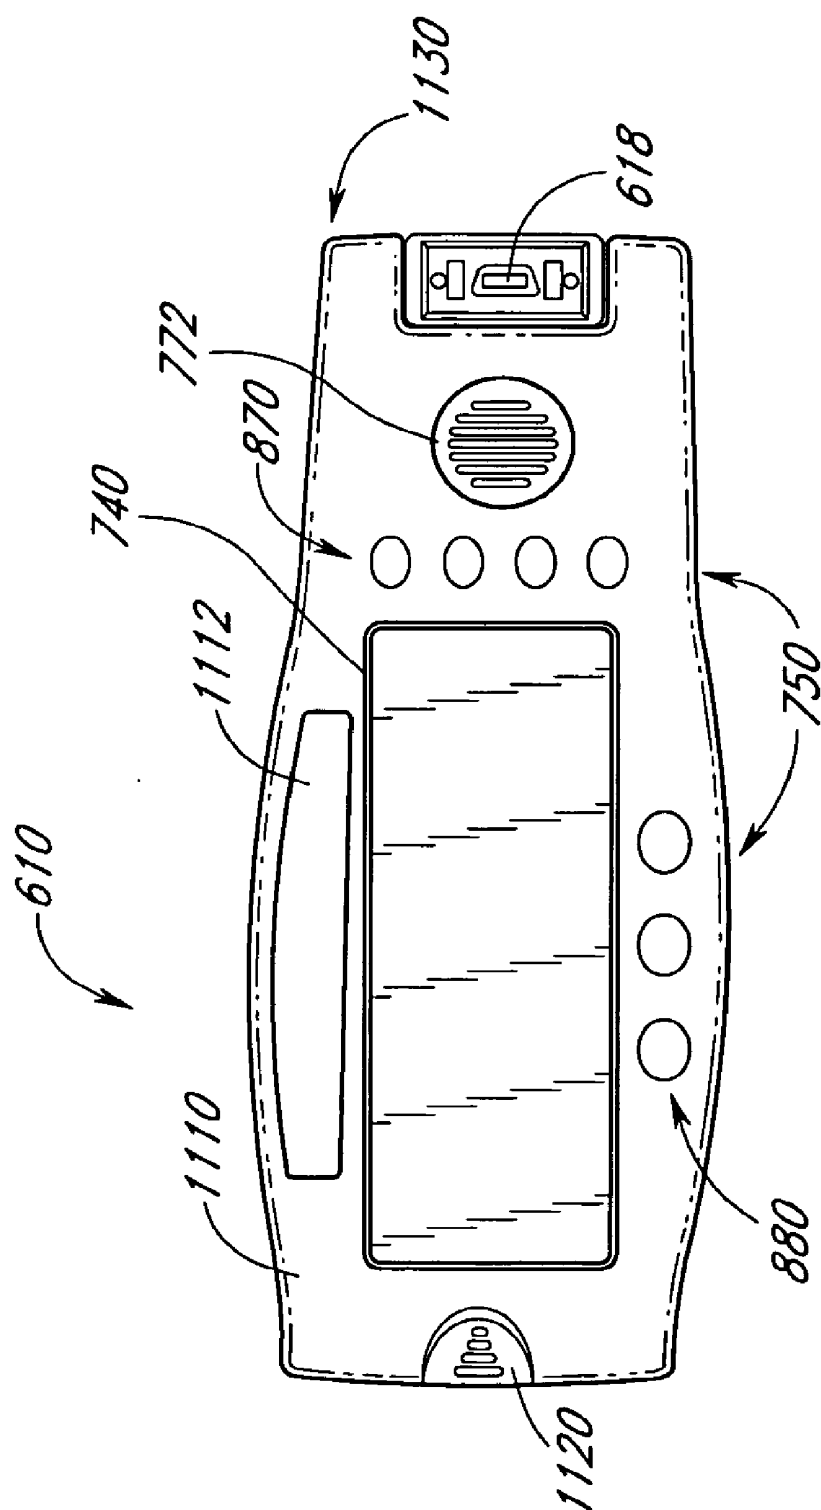


FIG. 11A

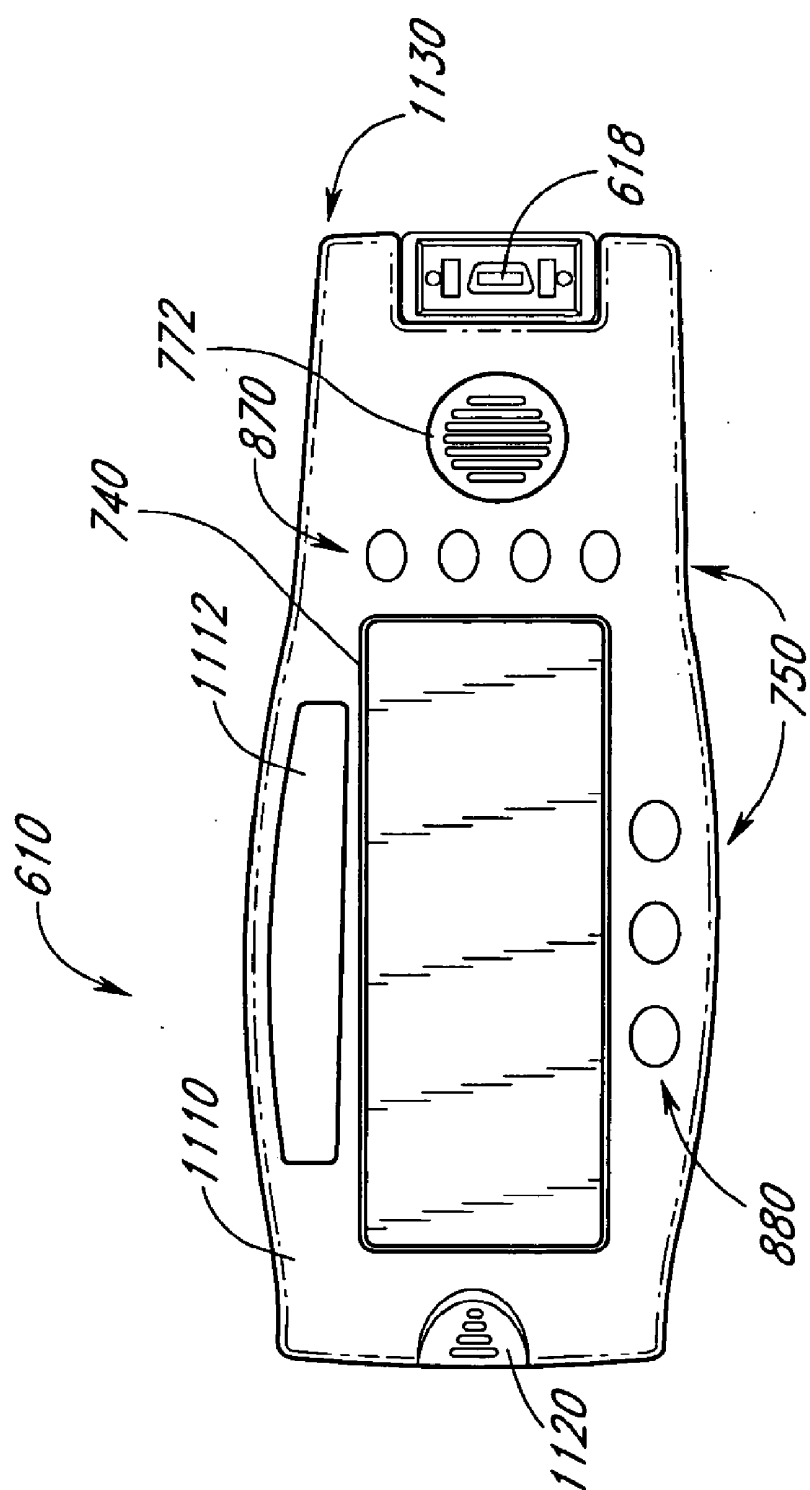


FIG. 11B

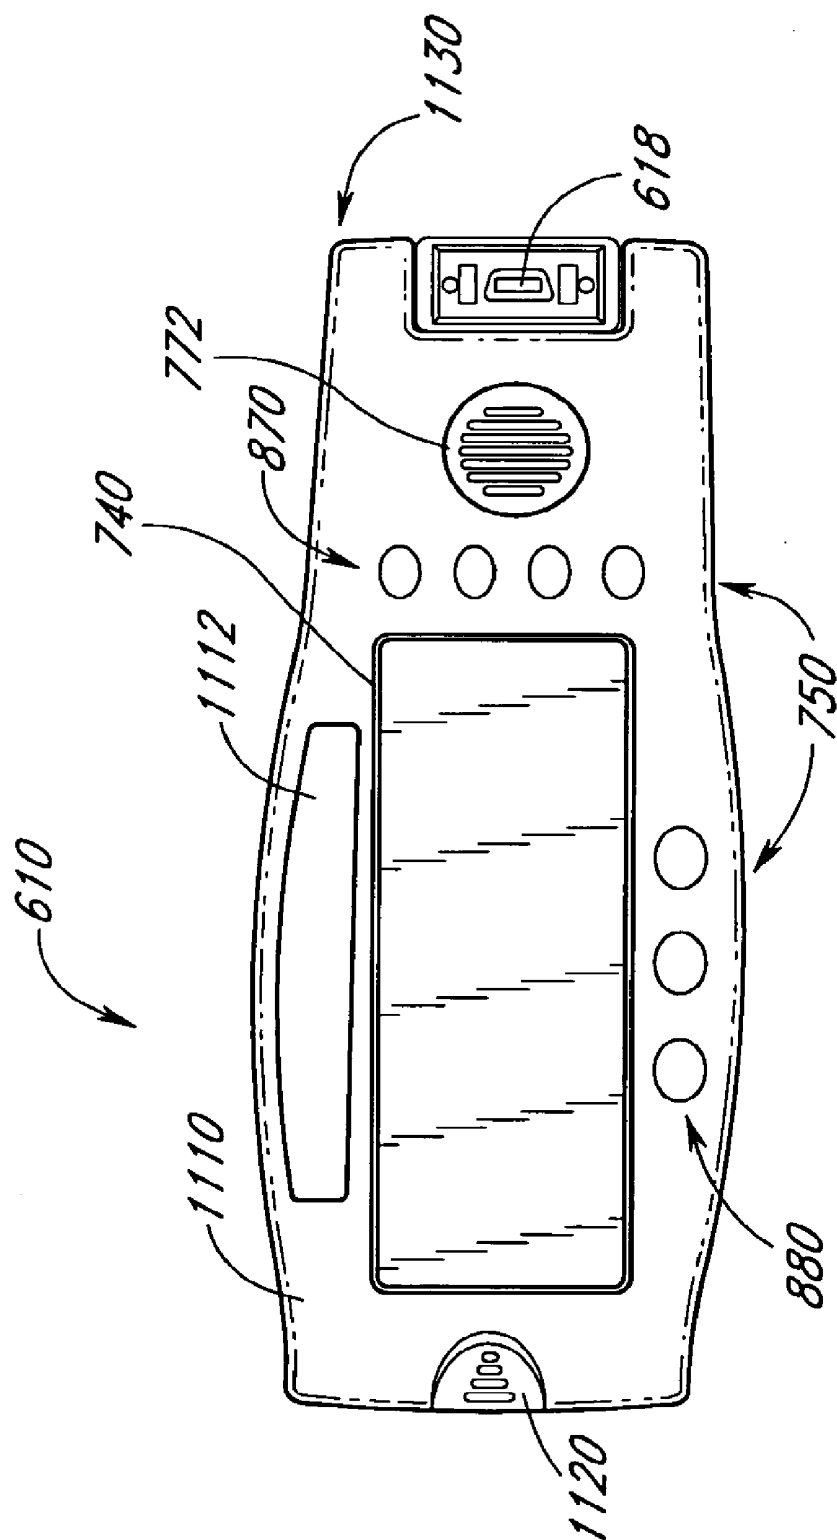


FIG. 12A

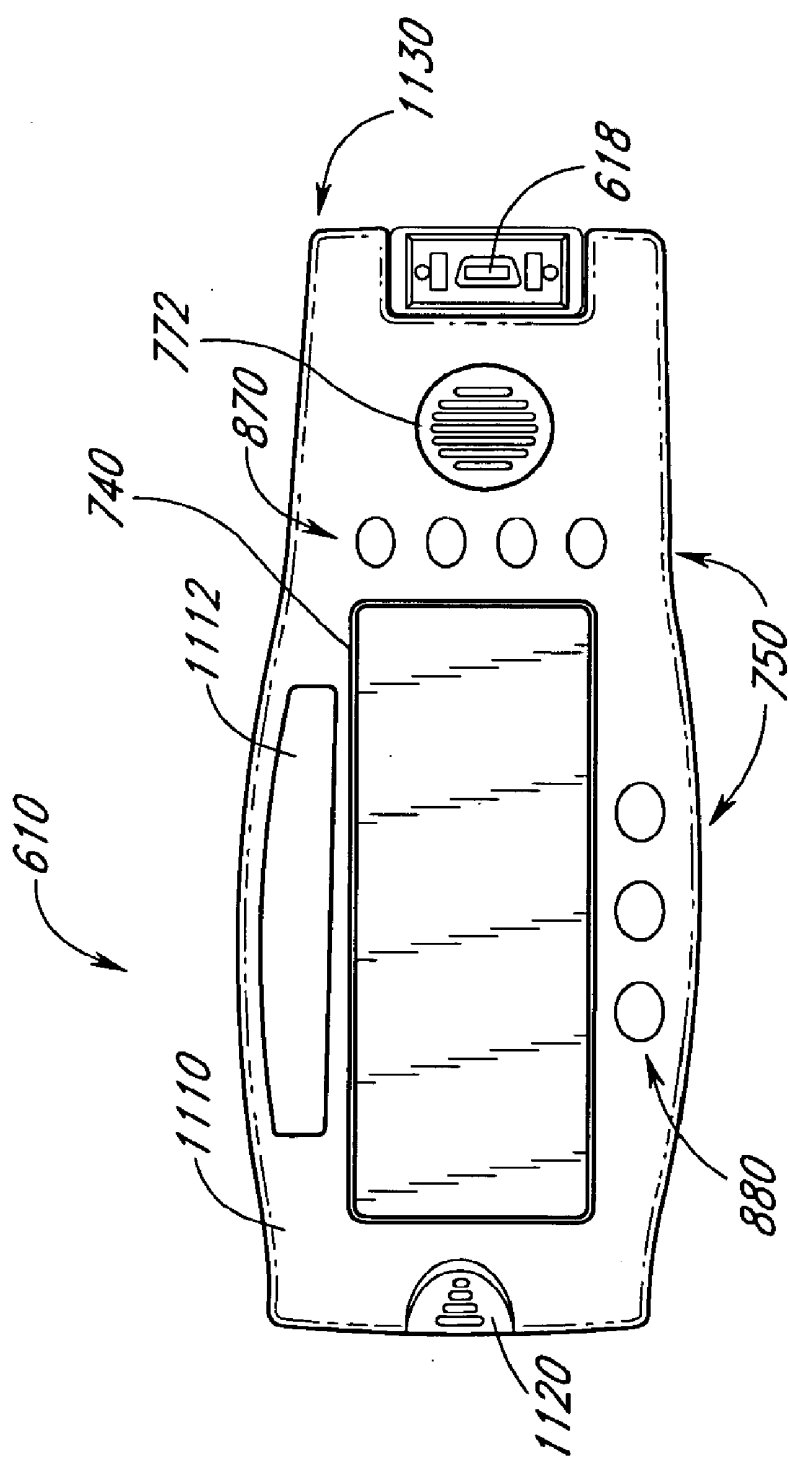


FIG. 12B


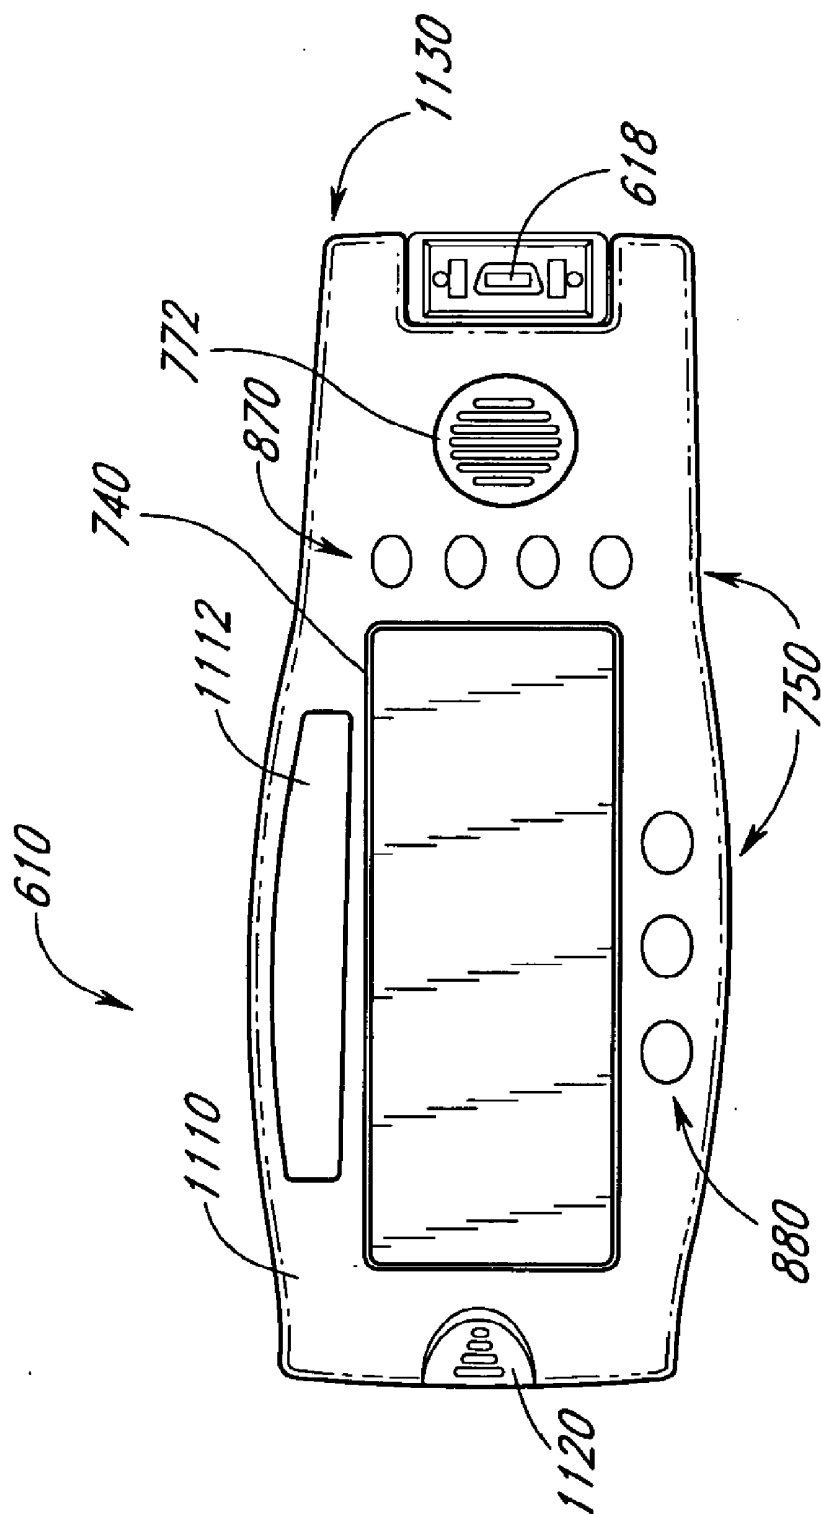


FIG. 13



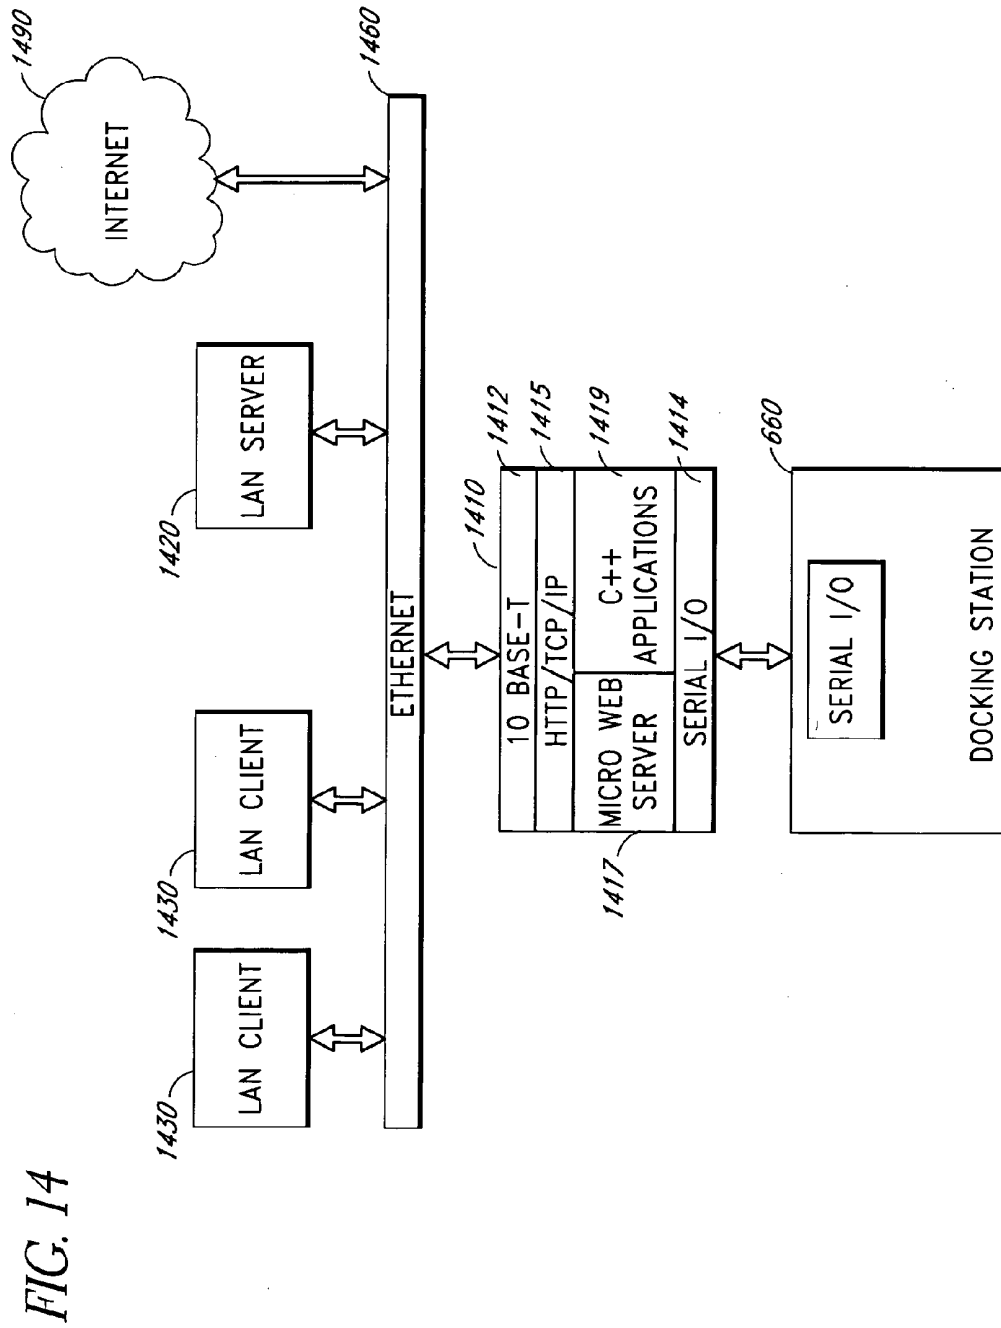

# SYSTEMS AND METHODS FOR ACQUIRING CALIBRATION DATA USABLE IN A PULSE OXIMETER

## CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 11/431,151, filed May 8, 2006, entitled "Systems and Methods for Acquiring Calibration Data Usable In A Pulse Oximeter" which is a continuation of U.S. patent application Ser. No. 10/420,994 filed Apr. 22, 2003, entitled "Systems and Methods for Acquiring Calibration Data Usable In A Pulse Oximeter," now U.S. Pat. No. 7,428,432, which is a continuation of U.S. patent application Ser. No. 10/153,263, filed May 21, 2002, entitled "System And Method For Altering A Display Mode Based On A Gravity-Responsive Sensor," which is a continuation of U.S. patent application Ser. No. 09/516,110, filed Mar. 1, 2000, entitled "Universal/Upgrading Pulse Oximeter," now U.S. Pat. No. 6,584,336, which is a continuation of U.S. patent application Ser. No. 09/491,175, filed Jan. 25, 2000, entitled "Universal/Upgrading Pulse Oximeter," now abandoned, which claims the benefit of U.S. Provisional application No. 60/161,565, filed Oct. 26, 1999, entitled "Improved Universal/Upgrading Pulse Oximeter, and application No. 60/117,097, filed Jan. 25, 1999, entitled "Universal/Upgrading Pulse Oximeter." Each of the foregoing applications is incorporated by reference herein.

## BACKGROUND OF THE INVENTION

[0002] Oximetry is the measurement of the oxygen level status of blood. Early detection of low blood oxygen level is critical in the medical field, for example in critical care and surgical applications, because an insufficient supply of oxygen can result in brain damage and death in a matter of minutes. Pulse oximetry is a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of oxygen supply. A pulse oximetry system consists of a sensor applied to a patient, a pulse oximeter, and a patient cable connecting the sensor and the pulse oximeter.

[0003] The pulse oximeter may be a standalone device or may be incorporated as a module or built-in portion of a multiparameter patient monitoring system, which also provides measurements such as blood pressure, respiratory rate and EKG. A pulse oximeter typically provides a numerical readout of the patient's oxygen saturation, a numerical readout of pulse rate, and an audible indicator or "beep" that occurs in response to each pulse. In addition, the pulse oximeter may display the patient's plethysmograph, which provides a visual display of the patient's pulse contour and pulse rate.

## SUMMARY OF THE INVENTION

[0004] FIG. 1 illustrates a prior art pulse oximeter 100 and associated sensor 110. Conventionally, a pulse oximetry sensor 110 has LED emitters 112, typically one at a red wavelength and one at an infrared wavelength, and a photodiode detector 114. The sensor 110 is typically attached to an adult patient's finger or an infant patient's foot. For a finger, the sensor 110 is configured so that the emitters 112 project light through the fingernail and through the blood vessels and capillaries underneath. The LED emitters 112 are activated by drive signals 122 from the pulse oximeter 100. The detector

114 is positioned at the fingertip opposite the fingernail so as to detect the LED emitted light as it emerges from the finger tissues. The photodiode generated signal 124 is relayed by a cable to the pulse oximeter 100.

[0005] The pulse oximeter 100 determines oxygen saturation (SpO<sub>2</sub>) by computing the differential absorption by arterial blood of the two wavelengths emitted by the sensor 110. The pulse oximeter 100 contains a sensor interface 120, an SpO<sub>2</sub> processor 130, an instrument manager 140, a display 150, an audible indicator (tone generator) 160 and a keypad 170. The sensor interface 120 provides LED drive current 122 that alternately activates the sensor red and IR LED emitters 112. The sensor interface 120 also has input circuitry for amplification and filtering of the signal 124 generated by the photodiode detector 114, which corresponds to the red and infrared light energy attenuated from transmission through the patient tissue site. The SpO<sub>2</sub> processor 130 calculates a ratio of detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on that ratio. The instrument manager 140 provides hardware and software interfaces for managing the display 150, audible indicator 160 and keypad 170. The display 150 shows the computed oxygen status, as described above. The audible indicator 160 provides the pulse beep as well as alarms indicating desaturation events. The keypad 170 provides a user interface for such things as alarm thresholds, alarm enablement, and display options.

[0006] Computation of SpO<sub>2</sub> relies on the differential light absorption of oxygenated hemoglobin, HbO<sub>2</sub>, and deoxygenated hemoglobin, Hb, to determine their respective concentrations in the arterial blood. Specifically, pulse oximetry measurements are made at red and IR wavelengths chosen such that deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin, for example 660 nm (red) and 905 nm (IR).

[0007] To distinguish between tissue absorption at the two wavelengths, the red and IR emitters 112 are provided drive current 122 so that only one is emitting light at a given time. For example, the emitters 112 may be cycled on and off alternately, in sequence, with each only active for a quarter cycle and with a quarter cycle separating the active times. This allows for separation of red and infrared signals and removal of ambient light levels by downstream signal processing. Because only a single detector 114 is used, it responds to both the red and infrared emitted light and generates a time-division-multiplexed ("modulated") output signal 124. This modulated signal 124 is coupled to the input of the sensor interface 120.

[0008] In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site might also comprise skin, muscle, bone, venous blood, fat, pigment, etc., each of which absorbs light. It is assumed that the background absorption due to these surrounding tissues is invariant and can be ignored. Thus, blood oxygen saturation measurements are based upon a ratio of the time-varying or AC portion of the detected red and infrared signals with respect to the time-invariant or DC portion:

$$RD/IR = (Red_{AC}/Red_{DC}) / (IR_{AC}/IR_{DC}).$$

**[0009]** The desired  $\text{SpO}_2$  measurement is then computed from this ratio. The relationship between RD/IR and  $\text{SpO}_2$  is most accurately determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. In a pulse oximeter device, this empirical relationship can be stored as a "calibration curve" in a read-only memory (ROM) look-up table so that  $\text{SpO}_2$  can be directly read-out of the memory in response to input RD/IR measurements.

**[0010]** Pulse oximetry is the standard-of-care in various hospital and emergency treatment environments. Demand has lead to pulse oximeters and sensors produced by a variety of manufacturers. Unfortunately, there is no standard for either performance by, or compatibility between, pulse oximeters or sensors. As a result, sensors made by one manufacturer are unlikely to work with pulse oximeters made by another manufacturer. Further, while conventional pulse oximeters and sensors are incapable of taking measurements on patients with poor peripheral circulation and are partially or fully disabled by motion artifact, advanced pulse oximeters and sensors manufactured by the assignee of the present invention are functional under these conditions. This presents a dilemma to hospitals and other caregivers wishing to upgrade their patient oxygenation monitoring capabilities. They are faced with either replacing all of their conventional pulse oximeters, including multiparameter patient monitoring systems, or working with potentially incompatible sensors and inferior pulse oximeters manufactured by various vendors for the pulse oximetry equipment in use at the installation.

**[0011]** Hospitals and other caregivers are also plagued by the difficulty of monitoring patients as they are transported from one setting to another. For example, a patient transported by ambulance to a hospital emergency room will likely be unmonitored during the transition from ambulance to the ER and require the removal and replacement of incompatible sensors in the ER. A similar problem is faced within a hospital as a patient is moved between surgery, ICU and recovery settings. Incompatibility and transport problems are exacerbated by the prevalence of expensive and non-portable multiparameter patient monitoring systems having pulse oximetry modules as one measurement parameter.

**[0012]** The Universal/Upgrading Pulse Oximeter (UPO) according to the present invention is focused on solving these performance, incompatibility and transport problems. The UPO provides a transportable pulse oximeter that can stay with and continuously monitor the patient as they are transported from setting to setting. Further, the UPO provides a synthesized output that drives the sensor input of other pulse oximeters. This allows the UPO to function as a universal interface that matches incompatible sensors with other pulse oximeter instruments. Further, the UPO acts as an upgrade to existing pulse oximeters that are adversely affected by low tissue perfusion and motion artifact. Likewise, the UPO can drive a  $\text{SpO}_2$  sensor input of multiparameter patient monitoring systems, allowing the UPO to integrate into the associated multiparameter displays, patient record keeping systems and alarm management functions.

**[0013]** One aspect of the present invention is a measurement apparatus comprising a sensor, a first pulse oximeter and a waveform generator. The sensor has at least one emitter and an associated detector configured to attach to a tissue site. The detector provides an intensity signal responsive to the oxygen content of arterial blood at the tissue site. The first pulse

oximeter is in communication with the detector and computes an oxygen saturation measurement based on the intensity signal. The waveform generator is in communication with the first pulse oximeter and provides a waveform based on the oxygen saturation measurement. A second pulse oximeter is in communication with the waveform generator and displays an oxygen saturation value based on the waveform. The waveform is synthesized so that the oxygen saturation value is generally equivalent to the oxygen saturation measurement.

**[0014]** In another aspect of the present invention, a measurement apparatus comprises a first sensor port connectable to a sensor, an upgrade port, a signal processor and a waveform generator. The upgrade port is connectable to a second sensor port of a physiological monitoring apparatus. The signal processor is configured to compute a physiological measurement based on a signal input to the first sensor port. The waveform generator produces a waveform based on the physiological measurement, and the waveform is available at the upgrade port. The waveform is adjustable so that the physiological monitoring apparatus displays a value generally equivalent to the physiological measurement when the upgrade port is attached to the second sensor port.

**[0015]** Yet another aspect of the present invention is a measurement method comprising the steps of sensing an intensity signal responsive to the oxygen content of arterial blood at a tissue site and computing an oxygen saturation measurement based on the intensity signal. Other steps are generating a waveform based on the oxygen saturation measurement and providing the waveform to the sensor inputs of a pulse oximeter so that the pulse oximeter displays an oxygen saturation value generally equivalent to the oxygen saturation measurement.

**[0016]** An additional aspect of the present invention is a measurement method comprising the steps of sensing a physiological signal, computing a physiological measurement based upon the signal, and synthesizing a waveform as a function of the physiological measurement. A further step is outputting the waveform to a sensor input of a physiological monitoring apparatus. The synthesizing step is performed so that the measurement apparatus displays a value corresponding to the physiological measurement.

**[0017]** A further aspect of the present invention is a measurement apparatus comprising a first pulse oximeter for making an oxygen saturation measurement and a pulse rate measurement based upon an intensity signal derived from a tissue site. Also included is a waveform generation means for creating a signal based upon the oxygen saturation measurement and the pulse rate measurement. In addition, there is a communication means for transmitting the signal to a second pulse oximeter.

**[0018]** Another aspect of the present invention is a measurement apparatus comprising a portable portion having a sensor port, a processor, a display, and a docking connector. The sensor port is configured to receive an intensity signal responsive to the oxygen content of arterial blood at a tissue site. The processor is programmed to compute an oxygen saturation value based upon the intensity signal and to output the value to the display. A docking station has a portable connector and is configured to accommodate the portable so that the docking connector mates with the portable connector. This provides electrical connectivity between the docking station and the portable. The portable has an undocked position separate from the docking station in which the portable functions as a handheld pulse oximeter. The portable also has

a docked position at least partially retained within the docking station in which the combination of the portable and the docking station has at least one additional function compared with the portable in the undocked position.

**[0019]** A further aspect of the present invention is a measurement apparatus configured to function in both a first spatial orientation and a second spatial orientation. The apparatus comprises a sensor port configured to receive a signal responsive to a physiological state. The apparatus also has a tilt sensor providing an output responsive to gravity. In addition, there is a processor in communication with the sensor port and the tilt sensor output. The processor is programmed to compute a physiological measurement value based upon the signal and to determine whether the measurement apparatus is in the first orientation or the second orientation based upon the tilt sensor output. A display has a first mode and a second mode and is driven by the processor. The display shows the measurement value in the first mode when the apparatus is in the first orientation and shows the measurement value in the second mode when the apparatus is in the second orientation.

**[0020]** Another aspect of the present invention is a measurement method comprising the steps of sensing a signal responsive to a physiological state and computing physiological measurement based on the signal. Additional steps are determining the spatial orientation of a tilt sensor and displaying the physiological measurement in a mode that is based upon the determining step.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0021]** FIG. 1 is a block diagram of a prior art pulse oximeter;

**[0022]** FIG. 2 is a diagram illustrating a patient monitoring system incorporating a universal/upgrading pulse oximeter (UPO) according to the present invention;

**[0023]** FIG. 3 is top level block diagram of a UPO embodiment;

**[0024]** FIG. 4 is a detailed block diagram of the waveform generator portion of the UPO embodiment shown in FIG. 3;

**[0025]** FIG. 5 is an illustration of a handheld embodiment of the UPO;

**[0026]** FIG. 6 is a top level block diagram of another UPO embodiment incorporating a portable pulse oximeter and a docking station;

**[0027]** FIG. 7 is a detailed block diagram of the portable pulse oximeter portion of FIG. 6;

**[0028]** FIG. 8A is an illustration of the portable pulse oximeter user interface, including a keyboard and display;

**[0029]** FIGS. 8B-C are illustrations of the portable pulse oximeter display showing portrait and landscape modes, respectively;

**[0030]** FIG. 9 is a detailed block diagram of the docking station portion of FIG. 6;

**[0031]** FIG. 10 is a schematic of the interface cable portion of FIG. 6;

**[0032]** FIG. 11A is a front view of an embodiment of a portable pulse oximeter;

**[0033]** FIG. 11B is a back view of a portable pulse oximeter;

**[0034]** FIG. 12A is a front view of an embodiment of a docking station;

**[0035]** FIG. 12B is a back view of a docking station;

**[0036]** FIG. 13 is a front view of a portable docked to a docking station; and

**[0037]** FIG. 14 is a block diagram of one embodiment of a local area network interface for a docking station.

#### DETAILED DESCRIPTION

**[0038]** FIG. 2 depicts the use of a Universal/Upgrading Pulse Oximeter ("UPO") **210** to perform patient monitoring. A pulse oximetry sensor **110** is attached to a patient (not illustrated) and provides the UPO **210** with a modulated red and IR photo-plethysmograph signal through a patient cable **220**. The UPO **210** computes the patient's oxygen saturation and pulse rate from the sensor signal and, optionally, displays the patient's oxygen status. The UPO **210** may incorporate an internal power source **212**, such as common alkaline batteries or a rechargeable power source. The UPO **210** may also utilize an external power source **214**, such as standard 110V AC coupled with an external step-down transformer and an internal or external AC-to-DC converter.

**[0039]** In addition to providing pulse oximetry measurements, the UPO **210** also separately generates a signal, which is received by a pulse oximeter **268** external to the UPO **210**. This signal is synthesized from the saturation calculated by the UPO **210** such that the external pulse oximeter **268** calculates the equivalent saturation and pulse rate as computed by the UPO **210**. The external pulse oximeter **268** receiving the UPO signal may be a multiparameter patient monitoring system (MPMS) **260** incorporating a pulse oximeter module **268**, a standalone pulse oximeter instrument, or any other host instrument capable of measuring SpO<sub>2</sub>. The MPMS **260** depicted in FIG. 2 has a rack **262** containing a number of modules for monitoring such patient parameters as blood pressure, EKG, respiratory gas, and SpO<sub>2</sub>. The measurements made by these various modules are shown on a multiparameter display **264**, which is typically a video (CRT) device. The UPO **210** is connected to an existing MPMS **260** with a cable **230**, advantageously integrating the UPO oxygen status measurements with other MPMS measurements. This allows the UPO calculations to be shown on a unified display of important patient parameters, networked with other patient data, archived within electronic patient records and incorporated into alarm management, which are all MPMS functions convenient to the caregiver.

**[0040]** FIG. 3 depicts the major functions of the UPO **210**, including an internal pulse oximeter **310**, a waveform generator **320**, a power supply **330** and an optional display **340**. Attached to the UPO **210** are a sensor **110** and an external pulse oximeter **260**. The internal pulse oximeter **310** provides the sensor **110** with a drive signal **312** that alternately activates the sensor's red and IR LEDs, as is well-known in the art. A corresponding detector signal **314** is received by the internal pulse oximeter **310**. The internal pulse oximeter **310** computes oxygen saturation, pulse rate, and, in some embodiments, other physiological parameters such as pulse occurrence, plethysmograph features and measurement confidence. These parameters **318** are output to the waveform generator **320**. A portion of these parameters may also be used to generate display drive signals **316** so that patient status may be read from, for example, an LED or LCD display module **340** on the UPO.

**[0041]** The internal pulse oximeter **310** may be a conventional pulse oximeter or, for upgrading an external pulse oximeter **260**, it may be an advanced pulse oximeter capable of low perfusion and motion artifact performance not found in conventional pulse oximeters. An advanced pulse oximeter for use as an internal pulse oximeter **310** is described in U.S.

Pat. No. 5,632,272 assigned to the assignee of the present invention and incorporated herein by reference. An advanced pulse oximetry sensor for use as the sensor **110** attached to the internal pulse oximeter **310** is described in U.S. Pat. No. 5,638,818 assigned to the assignee of the present invention and incorporated herein by reference. Further, a line of advanced Masimo SET® pulse oximeter OEM boards and sensors are available from the assignee of the present invention.

**[0042]** The waveform generator **320** synthesizes a waveform, such as a triangular waveform having a sawtooth or symmetric triangle shape, that is output as a modulated signal **324** in response to an input drive signal **322**. The drive input **322** and modulation output **324** of the waveform generator **320** are connected to the sensor port **262** of the external pulse oximeter **260**. The synthesized waveform is generated in a manner such that the external pulse oximeter **260** computes and displays a saturation and a pulse rate value that is equivalent to that measured by the internal pulse oximeter **310** and sensor **110**. In the present embodiment, the waveforms for pulse oximetry are chosen to indicate to the external pulse oximeter **260** a perfusion level of 5%. The external pulse oximeter **260**, therefore, always receives a strong signal. In an alternative embodiment, the perfusion level of the waveforms synthesized for the external pulse oximeter can be set to indicate a perfusion level at or close to the perfusion level of the patient being monitored by the internal pulse oximeter **310**. As an alternative to the generated waveform, a digital data output **326**, is connected to the data port **264** of the external pulse oximeter **260**. In this manner, saturation and pulse rate measurements and also samples of the unmodulated, synthesized waveform can be communicated directly to the external pulse oximeter **260** for display, bypassing the external pulse oximeter's signal processing functions. The measured plethysmograph waveform samples output from the internal pulse oximeter **310** also may be communicated through the digital data output **326** to the external pulse oximeter **260**.

**[0043]** It will be understood from the above discussion that the synthesized waveform is not physiological data from the patient being monitored by the internal pulse oximeter **310**, but is a waveform synthesized from predetermined stored waveform data to cause the external pulse oximeter **260** to calculate oxygen saturation and pulse rate equivalent to or generally equivalent (within clinical significance) to that calculated by the internal pulse oximeter **310**. The actual physiological waveform from the patient received by the detector is not provided to the external pulse oximeter **260** in the present embodiment. Indeed, the waveform provided to the external pulse oximeter will usually not resemble the plethysmographic waveform of physiological data from the patient being monitored by the internal pulse oximeter **260**.

**[0044]** The cable **230** (FIG. 2) attached between the waveform generator **320** and external pulse oximeter **260** provides a monitor ID **328** to the UPO, allowing identification of predetermined external pulse oximeter calibration curves. For example, this cable may incorporate an encoding device, such as a resistor, or a memory device, such as a PROM **1010** (FIG. 10) that is read by the waveform generator **320**. The encoding device provides a value that uniquely identifies a particular type of external pulse oximeter **260** having known calibration curve, LED drive and modulation signal characteristics. Although the calibration curves of the external pulse oximeter **260** are taken into account, the wavelengths of the

actual sensor **110**, advantageously, are not required to correspond to the particular calibration curve indicated by the monitor ID **328** or otherwise assumed for the external pulse oximeter **260**. That is, the wavelength of the sensor **110** attached to the internal pulse oximeter **310** is not relevant or known to the external pulse oximeter **260**.

**[0045]** FIG. 4 illustrates one embodiment of the waveform generator portion **320** of the UPO **210** (FIG. 3). Although this embodiment is illustrated and described as hardware, one of ordinary skill will recognize that the functions of the waveform generator may be implemented in software or firmware or a combination of hardware, software and firmware. The waveform generator **320** performs waveform synthesis with a waveform look-up table ("LUT") **410**, a waveform shaper **420** and a waveform splitter **430**. The waveform LUT **410** is advantageously a memory device, such as a ROM (read only memory) that contains samples of one or more waveform portions or segments containing a single waveform. These stored waveform segments may be as simple as a single period of a triangular waveform, having a sawtooth or symmetric triangle shape, or more complicated, such as a simulated plethysmographic pulse having various physiological features, for example rise time, fall time and dicrotic notch.

**[0046]** The waveform shaper **420** creates a continuous pulsed waveform from the waveform segments provided by the waveform LUT **410**. The waveform shaper **420** has a shape parameter input **422** and an event indicator input **424** that are buffered **470** from the parameters **318** output from the internal pulse oximeter **310** (FIG. 3). The shape parameter input **422** determines a particular waveform segment in the waveform LUT **410**. The chosen waveform segment is specified by the first address transmitted to the waveform LUT **410** on the address lines **426**. The selected waveform segment is sent to the waveform shaper **420** as a series of samples on the waveform data lines **412**.

**[0047]** The event indicator input **424** specifies the occurrence of pulses in the plethysmograph waveform processed by the internal pulse oximeter **310** (FIG. 3). For example, the event indicator may be a delta time from the occurrence of a previously detected falling pulse edge or this indicator could be a real time or near real time indicator of the pulse occurrence. The waveform shaper **420** accesses the waveform LUT **410** in a manner to create a corresponding delta time between pulses in the synthesized waveform output **428**. In one embodiment, the waveform shaper is clocked at a predetermined sample rate. From a known number of samples per stored waveform segment and the input delta time from the event indicator, the waveform shaper **420** determines the number of sequential addresses to skip between samples and accesses the waveform LUT **410** accordingly. This effectively "stretches" or "shrinks" the retrieved waveform segment so as to fit in the time between two consecutive pulses detected by the UPO.

**[0048]** The waveform splitter **430** creates a first waveform **432** corresponding to a first waveform (such as a red wavelength) expected by the external pulse oximeter **260** (FIG. 3) and a second waveform (such as infrared) **434** expected by the external pulse oximeter **260**. The relative amplitudes of the first waveform **432** and second waveform **434** are adjusted to correspond to the ratio output **444** from a calibration curve LUT **440**. Thus, for every value of measured oxygen saturation at the sat input **442**, the calibration curve LUT **440** provides a corresponding ratio output **444** that results in the first waveform **432** and the second waveform **434** having an

amplitude ratio that will be computed by the external pulse oximeter 260 (FIG. 3) as equivalent to the oxygen saturation measured by the internal pulse oximeter 310 (FIG. 3).

[0049] As described above, one particularly advantageous aspect of the UPO is that the operating wavelengths of the sensor 110 (FIG. 3) are not relevant to the operating wavelengths required by the external pulse oximeter 260 (FIG. 3), i.e. the operating wavelengths that correspond to the calibration curve or curves utilized by the external pulse oximeter. The calibration curve LUT 440 simply permits generation of a synthesized waveform as expected by the external oximeter 260 (FIG. 3) based on the calibration curve used by the external pulse oximeter 260 (FIG. 3). The calibration curve LUT 440 contains data about the known calibration curve of the external pulse oximeter 260 (FIG. 3), as specified by the monitor ID input 328. In other words, the waveform actually synthesized is not a patient plethysmographic waveform. It is merely a stored waveform that will cause the external pulse oximeter to calculate the proper oxygen saturation value and pulse rate values. Although this does not provide a patient plethysmograph on the external pulse oximeter for the clinician, the calculated values, which is what is actually sought, will be accurate.

[0050] A modulator 450 responds to an LED drive input 322 to generate a modulated waveform output 324 derived from the first waveform 432 and second waveform 434. Also, a data communication interface 460 transmits as a digital data output 326 the data obtained from the sat 442, pulse rate 462 and synthesized waveform 428 inputs.

[0051] FIG. 5 depicts a handheld UPO 500 embodiment. The handheld UPO 500 has keypad inputs 510, an LCD display 520, an external power supply input 530, an output port 540 for connection to an external pulse oximeter and a sensor input 550 at the top edge (not visible). The display 520 shows the measured oxygen saturation 522, the measured pulse rate 524, a pulsating bar 526 synchronized with pulse rate or pulse events, and a confidence bar 528 indicating confidence in the measured values of saturation and pulse rate. Also shown are low battery 572 and alarm enabled 574 status indicators.

[0052] The handheld embodiment described in connection with FIG. 5 may also advantageously function in conjunction with a docking station that mechanically accepts, and electrically connects to, the handheld unit. The docking station may be co-located with a patient monitoring system and connected to a corresponding SpO<sub>2</sub> module sensor port, external power supply, printer and telemetry device, to name a few options. In this configuration, the handheld UPO may be removed from a first docking station at one location to accompany and continuously monitor a patient during transport to a second location. The handheld UPO can then be conveniently placed into a second docking station upon arrival at the second location, where the UPO measurements are displayed on the patient monitoring system at that location.

[0053] FIG. 6 shows a block diagram of a UPO embodiment, where the functions of the UPO 210 are split between a portable pulse oximeter 610 and a docking station 660. The portable pulse oximeter 610 ("portable") is a battery operated, fully functional, stand-alone pulse oximeter instrument. The portable 610 connects to a sensor 110 (FIG. 2) through a UPO patient cable 220 (FIG. 2) attached to a patient cable connector 618. The portable 610 provides the sensor 110 with a drive signal 612 that alternately activates the sensor's red and IR LEDs, as is well-known in the art. The portable also

receives a corresponding detector signal 614 from the sensor. The portable can also input a sensor ID on the drive signal line 612, as described in U.S. Pat. No. 5,758,644 entitled Manual and Automatic Probe Calibration, assigned to the assignee of the present invention and incorporated herein by reference.

[0054] The portable 610 can be installed into the docking station 660 to expand its functionality. When installed, the portable 610 can receive power 662 from the docking station 660 if the docking station 660 is connected to external power 668. Alternately, with no external power 668 to the docking station 660, the portable 610 can supply power 662 to the docking station 660. The portable 610 communicates to the docking station with a bi-directional serial data line 664. In particular, the portable 610 provides the docking station with SpO<sub>2</sub>, pulse rate and related parameters computed from the sensor detector signal 614. When the portable 610 is installed, the docking station 660 may drive a host instrument 260 (FIG. 2) external to the portable 610. Alternatively, the portable 610 and docking station 660 combination may function as a stand-alone pulse oximeter instrument, as described below with respect to FIG. 13.

[0055] In one embodiment, the docking station 660 does not perform any action when the portable 610 is not docked. The user interface for the docking station 660, i.e. keypad and display, is on the portable 610. An indicator LED on the docking station 660 is lit when the portable is docked. The docking station 660 generates a detector signal output 674 to the host instrument 260 (FIG. 2) in response to LED drive signals 672 from the host instrument and SpO<sub>2</sub> values and related parameters received from the portable 610. The docking station 660 also provides a serial data output 682, a nurse call 684 and an analog output 688.

[0056] An interface cable 690 connects the docking station 660 to the host instrument patient cable 230 (FIG. 2). The LED drive signals 672 and detector signal output 674 are communicated between the docking station 660 and the host instrument 260 (FIG. 2) via the interface cable 690. The interface cable 690 provides a sync data output 692 to the docking station 660, communicating sensor, host instrument (e.g. monitor ID 328, FIG. 3) and calibration curve data. Advantageously, this data allows the docking station 660 to appear to a particular host instrument as a particular sensor providing patient measurements.

[0057] FIG. 7 provides further detail of the portable 610. The portable components include a pulse oximeter processor 710, a management processor 720, a power supply 730, a display 740 and a keypad 750. The pulse oximeter processor 710 functions as an internal pulse oximeter, interfacing the portable to a sensor 110 (FIG. 2) and deriving SpO<sub>2</sub>, pulse rate, a plethysmograph and a pulse indicator. An advanced pulse oximeter for use as the pulse oximeter processor 710 is described in U.S. Pat. No. 5,632,272, referenced above. An advanced pulse oximetry sensor for use as the sensor 110 (FIG. 2) attached to the pulse oximeter processor 710 is described in U.S. Pat. No. 5,638,818, also referenced above. Further, a line of advanced Masimo SET® pulse oximeter OEM boards and sensors are available from the assignee of the present invention. In one embodiment, the pulse oximeter processor 710 is the Masimo SET® MS-3L board or a low power MS-5 board.

[0058] The management processor 720 controls the various functions of the portable 610, including asynchronous serial data communications 724 with the pulse oximeter processor 710 and synchronous serial communications 762 with the

docking station 660 (FIG. 6). The physical and electrical connection to the docking station 660 (FIG. 6) is via a docking station connector 763 and the docking station interface 760, respectively. The processor 720 utilizes a real-time clock 702 to keep the current date and time, which includes time and date information that is stored along with SpO<sub>2</sub> parameters to create trend data. The processor of the portable 610 and the docking station 660 (FIG. 6) can be from the same family to share common routines and minimize code development time.

[0059] The processor 720 also controls the user interface 800 (FIG. 8A) by transferring data 742 to the display 740, including display updates and visual alarms, and by interpreting keystroke data 752 from the keypad 750. The processor 720 generates various alarm signals, when required, via an enable signal 728, which controls a speaker driver 770. The speaker driver 770 actuates a speaker 772, which provides audible indications such as, for example, alarms and pulse beeps. The processor 720 also monitors system status, which includes battery status 736, indicating battery levels, and docked status 764, indicating whether the portable 610 is connected to the docking station 660 (FIG. 6). When the portable 610 is docked and is on, the processor 720 also decides when to turn on or off docking station power 732.

[0060] Advantageously, the caregiver can set (i.e. configure or program) the behavior of the portable display 740 and alarms when the docked portable 610 senses that an interface cable 690 has connected the docking station 660 to an external pulse oximeter, such as a multiparameter patient monitoring system. In one user setting, for example, the portable display 740 stops showing the SpO<sub>2</sub> 811 (FIG. 8) and pulse rate 813 (FIG. 8) values when connected to an external pulse oximeter to avoid confusing the caregiver, who can read equivalent values on the patient monitoring system. The display 740, however, continues to show the plethysmograph 815 (FIG. 8) and visual pulse indicator 817 (FIG. 8) waveforms. For one such user setting, the portable alarms remain active.

[0061] Another task of the processor 720 includes maintenance of a watchdog function. The watchdog 780 monitors processor status on the watchdog data input 782 and asserts the :P reset output 784 if a fault is detected. This resets the management processor 720, and the fault is indicated with audible and visual alarms.

[0062] The portable 610 gets its power from batteries in the power supply 730 or from power 766 supplied from the docking station 660 (FIG. 6) via the docking station interface 760. A power manager 790 monitors the on/off switch on the keypad 750 and turns-on the portable power accordingly. The power manager 790 turns off the portable on command by the processor 720. DC/DC converters within the power supply 730 generate the required voltages 738 for operation of the portable 610 and docking station power 732. The portable batteries can be either alkaline rechargeable batteries or another renewable power source. The batteries of the power supply 730 supply docking station power 732 when the docking station 660 (FIG. 6) is without external power. A battery charger within the docking station power supply provides charging current 768 to rechargeable batteries within the power supply 730. The docking station power supply 990 (FIG. 9) monitors temperature 734 from a thermistor in the rechargeable battery pack, providing an indication of battery charge status.

[0063] A non-volatile memory 706 is connected to the management processor 720 via a high-speed bus 722. In the present embodiment, the memory 706 is an erasable and field re-programmable device used to store boot data, manufacturing serial numbers, diagnostic failure history, adult SpO<sub>2</sub> and pulse rate alarm limits, neonate SpO<sub>2</sub> and pulse rate alarm limits, SpO<sub>2</sub> and pulse rate trend data, and program data. Other types of non-volatile memory are well known. The SpO<sub>2</sub> and pulse rate alarm limits, as well as SpO<sub>2</sub> related algorithm parameters, may be automatically selected based on the type of sensor 110 (FIG. 2), adult or neonate, connected to the portable 610.

[0064] The LCD display 740 employs LEDs for a backlight to increase its contrast ratio and viewing distance when in a dark environment. The intensity of the backlight is determined by the power source for the portable 610. When the portable 610 is powered by either a battery pack within its power supply 730 or a battery pack in the docking station power supply 990 (FIG. 9), the backlight intensity is at a minimum level. When the portable 610 is powered by external power 668 (FIG. 6), the backlight is at a higher intensity to increase viewing distance and angle. In one embodiment, button on the portable permits overriding these intensity settings, and provides adjustment of the intensity. The backlight is controlled in two ways. Whenever any key is pressed, the backlight is illuminated for a fixed number of seconds and then turns off, except when the portable is docked and derives power from an external source. In that case, the backlight is normally on unless deactivated with a key on the portable 610.

[0065] FIG. 8A illustrates the portable user interface 800, which includes a display 740 and a keypad 750. In one embodiment, the display 740 is a dot matrix LCD device having 160 pixels by 480 pixels. The display 740 can be shown in portrait mode, illustrated in FIG. 8B, or in landscape mode, illustrated in FIG. 8C. A tilt sensor 950 (FIG. 9) in the docking station 660 (FIG. 6) or a display mode key on the portable 610 (FIG. 6) determines portrait or landscape mode. The tilt sensor 950 (FIG. 9) can be a gravity-activated switch or other device responsive to orientation and can be alternatively located in the portable 610 (FIG. 6). In a particular embodiment, the tilt sensor 950 (FIG. 9) is a non-mercury tilt switch, part number CW 1300-1, available from Comus International, Nutley, N.J. ([www.comus-intl.com](http://www.comus-intl.com)). The tilt sensor 950 (FIG. 9) could also be a mercury tilt switch.

[0066] Examples of how the display area can be used to display SpO<sub>2</sub> 811, pulse rate 813, a plethysmographic waveform 815, a visual pulse indicator 817 and soft key icons 820 in portrait and landscape mode are shown in FIGS. 8B and 8C, respectively. The software program of the management processor 720 (FIG. 7) can be easily changed to modify the category, layout and size of the display information shown in FIGS. 8B-C. Other advantageous information for display is SpO<sub>2</sub> limits, alarm, alarm disabled, exception messages and battery status.

[0067] The keypad 750 includes soft keys 870 and fixed keys 880. The fixed keys 880 each have a fixed function. The soft keys 870 each have a function that is programmable and indicated by one of the soft key icons 820 located next to the soft keys 870. That is, a particular one of the soft key icons 820 is in proximity to a particular one of the soft keys 870 and has a text or a shape that suggests the function of that particular one of the soft keys 870. In one embodiment, the button

portion of each key of the keypad **750** is constructed of fluorescent material so that the keys **870**, **880** are readily visible in the dark.

**[0068]** In one embodiment, the keypad **750** has one row of four soft keys **870** and one row of three fixed keys **880**. Other configurations are, of course, available, and specific arrangement is not significant. The functions of the three fixed keys **880** are power, alarm silence and light/contrast. The power function is an on/off toggle button. The alarm silence function and the light/contrast function have dual purposes depending on the duration of the key press. A momentary press of the key corresponding to the alarm silence function will disable the audible alarm for a fixed period of time. To disable the audible alarm indefinitely, the key corresponding to the alarm silence function is held down for a specified length of time. If the key corresponding to the alarm silence function is pressed while the audible alarm has been silenced, the audible alarm is reactivated. If the key corresponding to the light/contrast function is pressed momentarily, it is an on/off toggle button for the backlight. If the key corresponding to the light/contrast function is held down, the display contrast cycles through its possible values.

**[0069]** In this embodiment, the default functions of the four soft keys **870** are pulse beep up volume, pulse beep down volume, menu select, and display mode. These functions are indicated on the display by the up arrow, down arrow, "menu" and curved arrow soft key icons **820**, respectively. The up volume and down volume functions increase or decrease the audible sound or "beep" associated with each detected pulse. The display mode function rotates the display **740** through all four orthogonal orientations, including portrait mode (FIG. **8B**) and landscape mode (FIG. **8C**), with each press of the corresponding key. The menu select function allows the functionality of the soft keys **870** to change from the default functions described above. Examples of additional soft key functions that can be selected using this menu feature are set SpO<sub>2</sub> high/low limit, set pulse rate high/low limit, set alarm volume levels, set display to show trend data, print trend data, erase trend data, set averaging time, set sensitivity mode, perform synchronization, perform rechargeable battery maintenance (deep discharge/recharge to remove battery memory), and display product version number.

**[0070]** FIG. **9** provides further details of the docking station **660**, which includes a docking station processor **910**, a non-volatile memory **920**, a waveform generator **930**, a PROM interface **940**, a tilt sensor **950**, a portable interface **970** and associated connector **972**, status indicators **982**, a serial data port **682**, a nurse call output **684**, an analog output **688** and a power supply **990**. In one embodiment, the docking station **660** is intended to be associated with a fixed (non-transportable) host instrument, such as a multiparameter patient monitoring instrument in a hospital emergency room. In a transportable embodiment, the docking station **660** is movable, and includes a battery pack within the power supply **990**.

**[0071]** The docking station processor **910** orchestrates the activity on the docking station **660**. The processor **910** provides the waveform generator **930** with parameters **932** as discussed above for FIGS. **3** and **4**. The processor **910** also provides asynchronous serial data **912** for communications with external devices and synchronous serial data **971** for communications with the portable **610** (FIG. **6**). In addition, the processor **910** determines system status including sync status **942**, tilt status **952** and power status **992**. The portable management processor **720** (FIG. **7**) performs the watchdog

function for the docking station processor **910**. The docking station processor **910** sends watchdog messages to the portable processor **720** (FIG. **7**) as part of the synchronous serial data **972** to ensure the correct operation of the docking station processor **910**.

**[0072]** The docking station processor **910** accesses non-volatile memory **920** over a high-speed bus **922**. The non-volatile memory **920** is re-programmable and contains program data for the processor **910** including instrument communication protocols, synchronization information, a boot image, manufacturing history and diagnostic failure history.

**[0073]** The waveform generator **930** generates a synthesized waveform that a conventional pulse oximeter can process to calculate SpO<sub>2</sub> and pulse rate values or exception messages, as described above with respect to FIG. **4**. However, in the present embodiment, as explained above, the waveform generator output does not reflect a physiological waveform. It is merely a waveform constructed to cause the external pulse oximeter to calculate the correct saturation and pulse rate. In an alternative embodiment, physiological data could be provided to the external pulse oximeter, but the external pulse oximeter would generally not be able to calculate the proper saturation values, and the upgrading feature would be lost. The waveform generator **930** is enabled if an interface cable **690** (FIG. **6**), described below with respect to FIG. **10**, with valid synchronization information is connected. Otherwise, the power to the waveform generator **930** is disabled.

**[0074]** The status indicators **982** are a set of LEDs on the front of the docking station **660** used to indicate various conditions including external power (AC), portable docked, portable battery charging, docking station battery charging and alarm. The serial data port **682** is used to interface with either a computer, a serial port of conventional pulse oximeters or serial printers via a standard RS-232 DB-9 connector **962**. This port **682** can output trend memory, SpO<sub>2</sub> and pulse rate and support the system protocols of various manufacturers. The analog output **688** is used to interface with analog input chart recorders via a connector **964** and can output "real-time" or trend SpO<sub>2</sub> and pulse rate data. The nurse call output **684** from a connector **964** is activated when alarm limits are exceeded for a predetermined number of consecutive seconds. In another embodiment, data, including alarms, could be routed to any number of communications ports, and even over the Internet, to permit remote use of the upgrading pulse oximeter.

**[0075]** The PROM interface **940** accesses synchronization data **692** from the PROM **1010** (FIG. **10**) in the interface cable **690** (FIGS. **6**, **10**) and provides synchronization status **942** to the docking station processor **910**. The portable interface **970** provides the interconnection to the portable **610** (FIG. **6**) through the docking station interface **760** (FIG. **7**).

**[0076]** As shown in FIG. **9**, external power **668** is provided to the docking station **660** through a standard AC connector **968** and on/off switch **969**. When the docking station **660** has external power **668**, the power supply **990** charges the battery in the portable power supply **730** (FIG. **7**) and the battery, if any, in the docking station power supply **990**. When the portable **610** (FIG. **6**) is either removed or turned off, the docking station power **973** is removed and the docking station **660** is turned off, except for the battery charger portion of the power supply **990**. The docking station power **973** and, hence, the docking station **660** turn on whenever a docked portable



**610** (FIG. 6) is turned on. The portable **610** (FIG. 6) supplies power for an embodiment of the docking station **660** without a battery when external power **668** is removed or fails.

[0077] FIG. 10 provides further detail regarding the interface cable **690** used to connect between the docking station **660** (FIG. 6) and the patient cable **230** (FIG. 2) of a host instrument **260** (FIG. 2). The interface cable **690** is configured to interface to a specific host instrument and to appear to the host instrument as a specific sensor. A PROM **1010** built into the interface cable **690** contains information identifying a sensor type, a specific host instrument, and the calibration curve of the specific host instrument. The PROM information can be read by the docking station **660** (FIG. 6) as synchronization data **692**. Advantageously, the synchronization data **692** allows the docking station **660** (FIG. 6) to generate a waveform to the host instrument that causes the host instrument to display SpO<sub>2</sub> values equivalent to those calculated by the portable **610** (FIG. 6). The interface cable **690** includes an LED drive path **672**. In the embodiment shown in FIG. 10, the LED drive path **672** is configured for common anode LEDs and includes IR cathode, red cathode and common anode signals. The interface cable **690** also includes a detector drive path **674**, including detector anode and detector cathode signals.

[0078] A menu option on the portable **610** (FIG. 6) also allows synchronization information to be calculated in the field. With manual synchronization, the docking station **660** (FIG. 6) generates a waveform to the host instrument **260** (FIG. 2) and displays an expected SpO<sub>2</sub> value. The user enters the SpO<sub>2</sub> value displayed on the host instrument using the portable keypad **750** (FIG. 7). These steps are repeated until a predetermined number of data points are entered and the SpO<sub>2</sub> values displayed by the portable and the host instrument are consistent.

[0079] FIGS. 11A-B depict an embodiment of the portable **610**, as described above with respect to FIG. 6. FIGS. 12A-B depict an embodiment of the docking station **660**, as described above with respect to FIG. 6. FIG. 13 depicts an embodiment of the UPO **210** where the portable **610** is docked with the docking station **660**, also as described above with respect to FIG. 6.

[0080] FIG. 11A depicts the portable front panel **1110**. The portable **610** has a patient cable connector **618**, as described above with respect to FIG. 6. Advantageously, the connector **618** is rotatably mounted so as to minimize stress on an attached patient cable (not shown). In one embodiment, the connector **618** can freely swivel between a plane parallel to the front panel **1110** and a plane parallel to the side panel **1130**. In another embodiment, the connector **618** can swivel between, and be releasably retained in, three locked positions. A first locked position is as shown, where the connector is in a plane parallel to the front panel **1110**. A second locked position is where the connector **618** is in a plane parallel to the side panel **1130**. The connector **618** also has an intermediate locked position 45° between the first and the second locked positions. The connector **618** is placed in the first locked position for attachment to the docking station **660**.

[0081] Shown in FIG. 11A, the portable front panel **1110** also has a speaker **772**, as described with respect to FIG. 7. Further, the front panel **1110** has a row of soft keys **870** and fixed keys **880**, as described above with respect to FIG. 8. In addition, the front panel **1110** has a finger actuated latch **1120** that locks onto a corresponding catch **1244** (FIG. 12A) in the docking station **660**, allowing the portable **610** to be releas-

ably retained by the docking station **660**. An OEM label can be affixed to a recessed area **1112** on the front panel **1110**.

[0082] FIG. 11B depicts the portable back panel **1140**. The back panel **1140** has a socket **763**, a pole clamp mating surface **1160**, and a battery pack compartment **1170**. The socket **763** is configured to mate with a corresponding docking station plug **972** (FIG. 12A). The socket **763** and plug **972** (FIG. 12A) provide the electrical connection interface between the portable **610** and the docking station **660** (FIG. 12A). The socket **763** houses multiple spring contacts that compress against plated edge-connector portions of the docking station plug **972** (FIG. 12A). A conventional pole clamp (not shown) may be removably attached to the mating surface **1160**. This conveniently allows the portable **610** to be held to various patient-side or bedside mounts for hands-free pulse oximetry monitoring. The portable power supply **730** (FIG. 7) is contained within the battery pack compartment **1170**. The compartment **1170** has a removable cover **1172** for protection, insertion and removal of the portable battery pack. Product labels, such as a serial number identifying a particular portable, can be affixed with the back panel indent **1142**.

[0083] FIG. 12A depicts the front side **1210** of the docking station **660**. The front side **1210** has a docking compartment **1220**, a pole clamp recess **1230**, pivots **1242**, a catch **1244**, a plug connector **972** and LED status indicators **982**. The docking compartment **1220** accepts and retains the portable **610** (FIGS. 11A-B), as shown in FIG. 13. When the portable **610** (FIGS. 11A-B) is docked in the compartment **1220**, the pole clamp recess **1230** accommodates a pole clamp (not shown) attached to the portable's pole clamp mating surface **1160** (FIG. 11B), assuming the pole clamp is in its closed position. The portable **610** (FIGS. 11A-B) is retained in the compartment **1220** by pivots **1242** that fit into corresponding holes in the portable's side face **1130** and a catch **1244** that engages the portable's latch **1120** (FIG. 11A). Thus, the portable **610** (FIGS. 11A-B) is docked by first attaching it at one end to the pivots **1242**, then rotating it about the pivots **1242** into the compartment **1220**, where it is latched in place on the catch **1244**. The portable **610** (FIGS. 11A-B) is undocked in reverse order, by first pressing the latch **1120** (FIG. 11A), which releases the portable from the catch **1244**, rotating the portable **610** (FIGS. 11A-B) about the pivots **1242** out of the compartment **1220** and then removing it from the pivots **1242**. As the portable is rotated into the compartment, the docking station plug **972** inserts into the portable socket **763** (FIG. 11B), providing the electrical interface between the portable **610** and the docking station **660**. The status indicators **982** are as described above with respect to FIG. 9.

[0084] FIG. 12B depicts the back side **1260** of the docking station **660**. The back side **1260** has a serial (RS-232 or USB) connector **962**, an analog output and nurse call connector **964**, an upgrade port connector **966**, an AC power plug **968**, an on/off switch **969** and a ground lug **1162**. A handle **1180** is provided at one end and fan vents **1170** are provided at the opposite end. A pair of feet **1190** are visible near the back side **1260**. A corresponding pair of feet (not visible) are located near the front side **1210** (FIG. 12A). The feet near the front side **1210** extend so as to tilt the front side **1210** (FIG. 12A) upward, making the display **740** (FIG. 13) of a docked portable **610** (FIG. 13) easier to read.

[0085] FIG. 13 illustrates both the portable **610** and the docking station **660**. The portable **610** and docking station **660** constitute three distinct pulse oximetry instruments. First, the portable **610** by itself, as depicted in FIGS. 11A-B,

is a handheld pulse oximeter applicable to various patient monitoring tasks requiring battery power or significant mobility, such as ambulance and ER situations. Second, the portable **610** docked in the docking station **660**, as depicted in FIG. **13**, is a standalone pulse oximeter applicable to a wide-range of typical patient monitoring situations from hospital room to the operating room. Third, the portable **610** docked and the upgrade port **966** (FIG. **12B**) connected with an interface cable to the sensor port of a conventional pulse oximeter module **268** (FIG. **2**) within a multiparameter patient monitoring instrument **260** (FIG. **2**) or other conventional pulse oximeter, is a universal/upgrading pulse oximeter (UPO) instrument **210**, as described herein. Thus, the portable **610** and docking station **660** configuration of the UPO **210** advantageously provides a three-in-one pulse oximetry instrument functionality.

**[0086]** Another embodiment of the docking station **660** incorporates an input port that connects to a blood pressure sensor and an output port that connects to the blood pressure sensor port of a multiparameter patient monitoring system (MPMS). The docking station **660** incorporates a signal processor that computes a blood pressure measurement based upon an input from the blood pressure sensor. The docking station **660** also incorporates a waveform generator connected to the output port that produces a synthesized waveform based upon the computed measurement. The waveform generator output is adjustable so that the blood pressure value displayed on the MPMS is equivalent to the computed blood pressure measurement. Further, when the portable **610** is docked in the docking station **660** and the blood pressure sensor is connected to the input port, the portable displays a blood pressure value according to the computed blood pressure measurement. Thus, in this embodiment, the docking station **660** provides universal/upgrading capability for both blood pressure and SpO<sub>2</sub>.

**[0087]** Likewise, the docking station **660** can function as an universal/upgrading instrument for other vital sign measurements, such as respiratory rate, EKG or EEG. For this embodiment, the docking station **660** incorporates related sensor connectors and associated sensor signal processors and upgrade connectors to an MPMS or standalone instrument. In this manner, a variety of vital sign measurements can be incorporated into the docking station **660**, either individually or in combination, with or without SpO<sub>2</sub> as a measurement parameter, and with or without the portable **610**. In yet another embodiment, the docking station **660** can be configured as a simple SpO<sub>2</sub> upgrade box, incorporating a SpO<sub>2</sub> processor and patient cable connector for a SpO<sub>2</sub> sensor that functions with or without the portable **610**.

**[0088]** Unlike a conventional standalone pulse oximeter, the standalone configuration shown in FIG. **13** has a rotatable display **740** that allows the instrument to be operated in either a vertical or horizontal orientation. A tilt sensor **950** (FIG. **9**) indicates when the bottom face **1310** is placed along a horizontal surface or is otherwise horizontally-oriented. In this horizontal orientation, the display **740** appears in landscape mode (FIG. **8C**). The tilt sensor **950** (FIG. **9**) also indicates when the side face **1320** is placed along a horizontal surface or is otherwise horizontally oriented. In this vertical orientation, the display **740** appears in portrait mode (FIG. **8B**). A soft key **870** on the portable **610** can override the tilt sensor, allowing the display to be presented at any 90° orientation, i.e. portrait, landscape, "upside-down" portrait or "upside-down" landscape orientations. The handheld configuration (FIG.

**11A**), can also present the display **740** at any 90° orientation using a soft key **870**. In the particular embodiment described above, however, the portable **610** does not have a tilt sensor and, hence, relies on a soft key **870** to change the orientation of the display when not docked.

**[0089]** FIG. **14** illustrates the docking station **660** incorporated within a local area network (LAN). The LAN shown is Ethernet-based **1460**, using a central LAN server **1420** to interconnect various LAN clients **1430** and other system resources such as printers and storage (not shown). An Ethernet controller module **1410** is incorporated with the docking station **660**. The controller module **1410** can be incorporated within the docking station **660** housing or constructed as an external unit. In this manner, the UPO, according to the present invention, can communicate with other devices on the LAN or over the Internet **1490**.

**[0090]** The Ethernet controller module **1410** can be embedded with web server firmware, such as the Hewlett-Packard (HP) BFOOT-10501. The module **1410** has both a 10 Base-T Ethernet interface for connection to the Ethernet **1460** and a serial interface, such as RS-232 or USB, for connection to the docking station **660**. The module firmware incorporates HTTP and TCP/IP protocols for standard communications over the World Wide Web. The firmware also incorporates a micro web server that allows custom web pages to be served to remote clients over the Internet, for example. Custom C++ programming allows expanded capabilities such as data reduction, event detection and dynamic web page configuration.

**[0091]** As shown in FIG. **14**, there are many applications for the docking station **660** to Ethernet interface. Multiple UPOs can be connected to a hospital's LAN, and a computer on the LAN could be utilized to upload pulse rate and saturation data from the various UPOs, displaying the results. Thus, this Ethernet interface could be used to implement a central pulse oximetry monitoring station within a hospital. Further, multiple UPOs from anywhere in the world can be monitored from a central location via the Internet. Each UPO is addressable as an individual web site and downloads web pages viewable on a standard browser, the web pages displaying oxygen saturation, pulse rate and related physiological measurements from the UPO. This feature allows a caregiver to monitor a patient regardless of where the patient or caregiver is located. For example a caregiver located at home in one city or at a particular hospital could download measurements from a patient located at home in a different city or at the same or a different hospital. Other applications include troubleshooting newly installed UPOs or uploading software patches or upgrades to UPOs via the Internet. In addition alarms could be forwarded to the URL of the clinician monitoring the patient.

**[0092]** The UPO may have other configurations besides the handheld unit described in connection with FIG. **5** or the portable **610** and docking station **660** combination described in connection with FIGS. **11-13**. The UPO may be a module, with or without a display, that can be removably fastened to a patient via an arm strap, necklace or similar means. In a smaller embodiment, this UPO module may be integrated into a cable or connector used for attaching a sensor to a pulse oximeter. The UPO may also be a circuit card or module that can externally or internally plug into or mate with a standalone pulse oximeter or multiparameter patient monitoring system. Alternatively, the UPO may be configured as a simple standalone upgrade instrument.

**[0093]** Further, although a universal/upgrading apparatus and method have been mainly described in terms of a pulse oximetry measurement embodiment, the present invention is equally applicable to other physiological measurement parameters such as blood pressure, respiration rate, EEG and ECG, to name a few. In addition, a universal/upgrading instrument having a single physiological measurement parameter or a multiple measurement parameter capability and configured as a handheld, standalone, portable, docking station, module, plug-in, circuit card, to name a few, is also within the scope of the present invention.

**[0094]** The UPO has been disclosed in detail in connection with various embodiments of the present invention. These embodiments are disclosed by way of examples only and are not to limit the scope of the present invention, which is defined by the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications within the scope of this invention.

What is claimed is:

1. A method for communicating a physiological waveform indicative of a physiological condition to a patient monitor, the method comprising:

obtaining a sensor signal indicative of a physiological parameter;  
calculating a first physiological measurement using a first processor;  
communicating the physiological measurement to a second processor;  
constructing an output signal indicative of the physiological measurement; and  
communicating the output signal to the sensor input of a patient monitoring device.

2. The method of claim 1, further comprising displaying the calculated physiological measurement on a first display associated with the first processor.

3. The method of claim 1, wherein the physiological measurement comprises at least one of blood oxygen levels, blood pressure, ECG, and pulse rate.

4. The method of claim 1, wherein the output signal is configured to cause a patient monitor not associated with the first processor to calculate a second physiological measurement substantially equivalent to the first physiological measurement.

5. The method of claim 1, wherein the second processor comprises a waveform generator.

6. The method of claim 1, wherein the second processor is comprised within a docking station.

7. A system for communicating a physiological waveform indicative of a physiological condition to a patient monitor, the system comprising:

a sensor input configured to obtain a sensor signal indicative of a physiological parameter;  
a first processor configured to calculate a first physiological measurement;  
a second processor in communication with the first processor;

wherein the second processor is configured to construct an output signal indicative of the physiological measurement; and

an output configured to communicate the output signal to a patient monitoring device.

8. The method of claim 7, further comprising a first display in communication with the first processor, wherein the display is configured to display the calculated physiological measurement.

9. The method of claim 7, wherein the physiological measurement comprises at least one of blood oxygen levels, blood pressure, ECG, and pulse rate.

10. The method of claim 7, wherein the output signal is configured to cause a patient monitor not associated with the first processor to calculate a second physiological measurement substantially equivalent to the first physiological measurement.

11. A method for communicating a physiological waveform indicative of a physiological condition to a patient monitor, the method comprising:

obtaining a sensor signal indicative of a physiological parameter;  
displaying information about the sensor signal on a first display;  
constructing an output signal indicative of the sensor signal and  
communicating the output signal to a patient monitoring device, wherein the patient monitoring device communicates with a second display.

12. The method of claim 11, further comprising calculating a first physiological measurement using a first processor.

13. The method of claim 12, further communicating the first physiological measurement to a second processor.

14. The method of claim 12, further comprising displaying the physiological measurement on the first display.

15. The method of claim 11, wherein information comprises a power on indication.

16. The method of claim 11, wherein information comprises signal quality information.

17. The method of claim 11, wherein information comprises a physiological measurement.

18. A system for communicating a physiological waveform indicative of a physiological condition to a patient monitor, the system comprising:

a sensor input configured to obtain a sensor signal indicative of a physiological parameter;  
a first display configured to display information about the sensor signal;  
a processor configured to construct an output signal indicative of the sensor signal; and  
an output configured to communicate the output signal to a patient monitoring device, wherein the patient monitoring device communicates with a second display.

\* \* \* \* \*

专利名称(译)	用于获取可在脉搏血氧计中使用的校准数据的系统和方法		
公开(公告)号	<a href="#">US20110288384A1</a>	公开(公告)日	2011-11-24
申请号	US13/196732	申请日	2011-08-02
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	ALI AMMAR AL CAROTHERS DON DALKE DAVID DIAB MOHAMED K GOLDMAN JULIAN KIANI MASSI E LEE MICHAEL NOVAK JEROME SMITH ROBERT VADEN VAL E		
发明人	ALI, AMMAR AL CAROTHERS, DON DALKE, DAVID DIAB, MOHAMED K. GOLDMAN, JULIAN KIANI, MASSI E. LEE, MICHAEL NOVAK, JEROME SMITH, ROBERT VADEN, VAL E.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/0002 A61B5/14551 A61B5/1495 A61B5/742 A61B2560/0271 A61B5/7278 A61B2562/085 A61B5/743 A61B5/0205 A61B5/0402 A61B2560/0456		
优先权	60/117097 1999-01-25 US 60/161565 1999-10-26 US		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

本公开包括具有可访问存储器的脉冲血氧计附件。在一个实施例中，脉冲血氧计附件存储校准数据，例如，与传感器类型相关的校准数据，校准曲线等。校准数据用于计算脉冲血液的生理参数。

