



US 20020017299A1

(19) **United States**(12) **Patent Application Publication**  
**Hickle**(10) **Pub. No.: US 2002/0017299 A1**(43) **Pub. Date: Feb. 14, 2002**(54) **APPARATUS AND METHOD FOR  
PROVIDING A CONSCIOUS PATIENT  
RELIEF FROM PAIN AND ANXIETY  
ASSOCIATED WITH MEDICAL OR  
SURGICAL PROCEDURES****Publication Classification**(51) **Int. Cl.<sup>7</sup>** ..... **A61N 1/30**; A61M 15/00;  
A61M 16/10; A62B 7/00;  
A61M 16/00; F16K 31/02;  
A62B 18/02(76) **Inventor: Randall S. Hickle, Lubbock, TX (US)**(52) **U.S. Cl.** ..... **128/204.21**; 128/203.12; 128/205.25;  
604/19


Correspondence Address:


**Celine Jimenez Crowson****Hogan & Hartson L.L.P.****555 13th Street, N.W.****Washington, DC 20004 (US)**(21) **Appl. No.: 09/909,782**(22) **Filed: Jul. 23, 2001****Related U.S. Application Data**

(60) Division of application No. 09/324,759, filed on Jun. 3, 1999, which is a non-provisional of provisional application No. 60/087,841, filed on Jun. 3, 1998.

(57) **ABSTRACT**

A care system and associated methods are provided for alleviating patient pain, anxiety and discomfort associated with medical or surgical procedures. The system comprises: at least one patient health monitor device generating a signal reflecting at least one physiological condition of a patient; a drug delivery controller supplying one or more drugs to the patient; a memory device storing a safety data set reflecting parameters of at least one patient physiological condition; and an electronic controller interconnected between the patient health monitor, the drug delivery controller and the safety data set. A method of electronically tracking recurring revenues generated by the use of the care system where the system is at the location of its user is also provided. Additional embodiments of the system and methods are directed to alleviating patient pain or discomfort while enabling safe patient controlled drug delivery in correlation with the monitoring of patient health conditions.

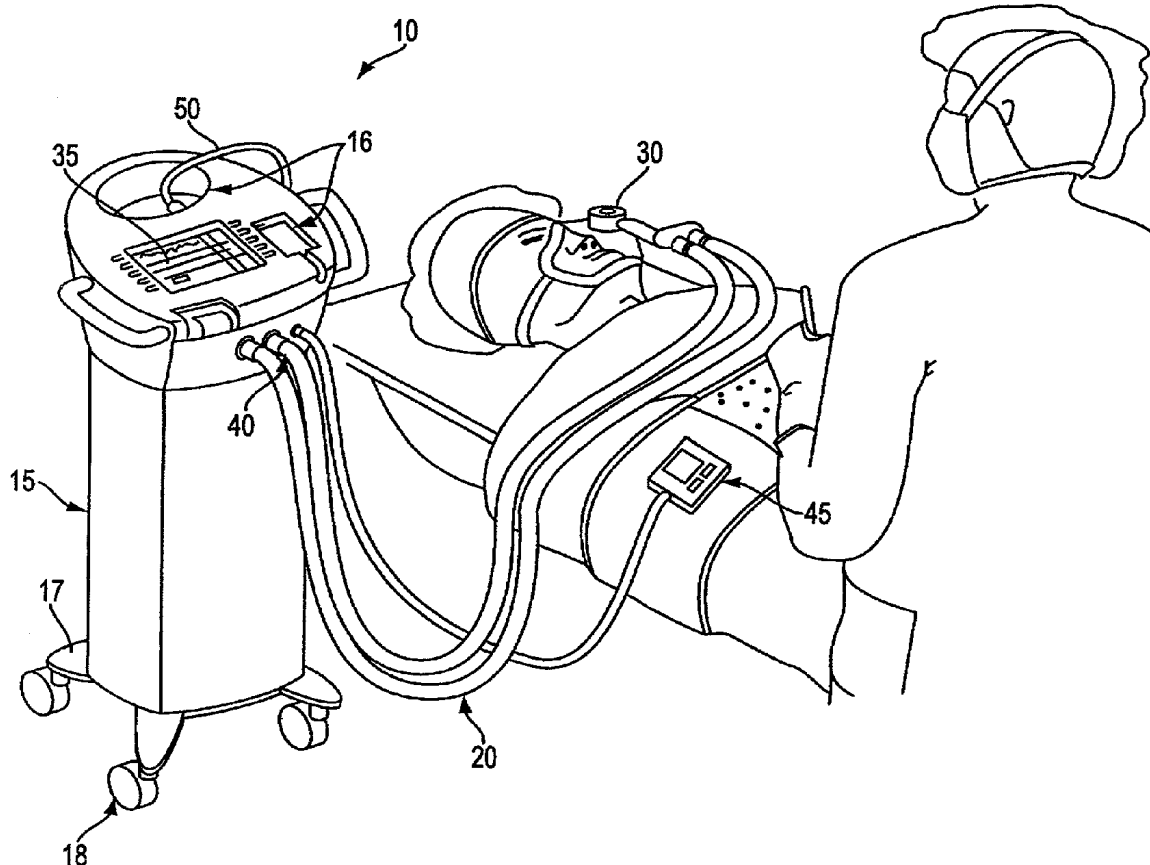

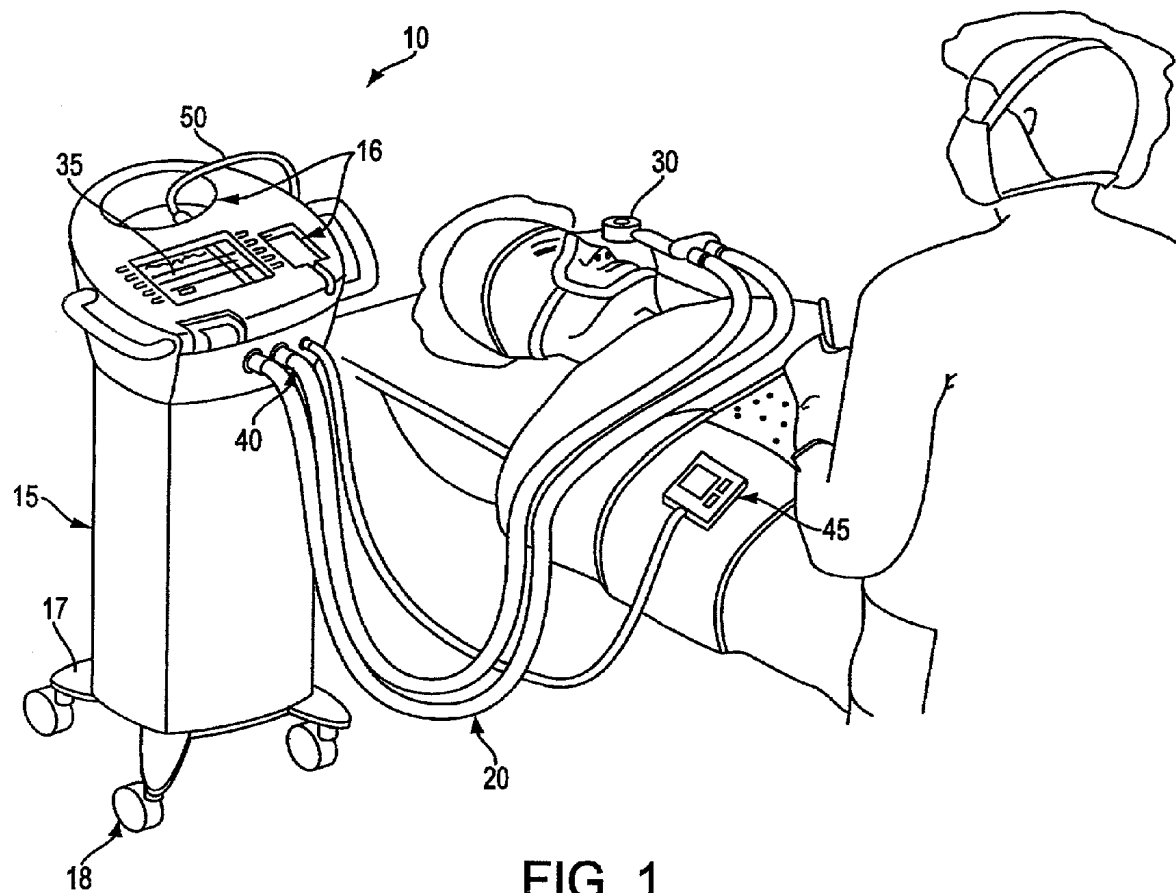

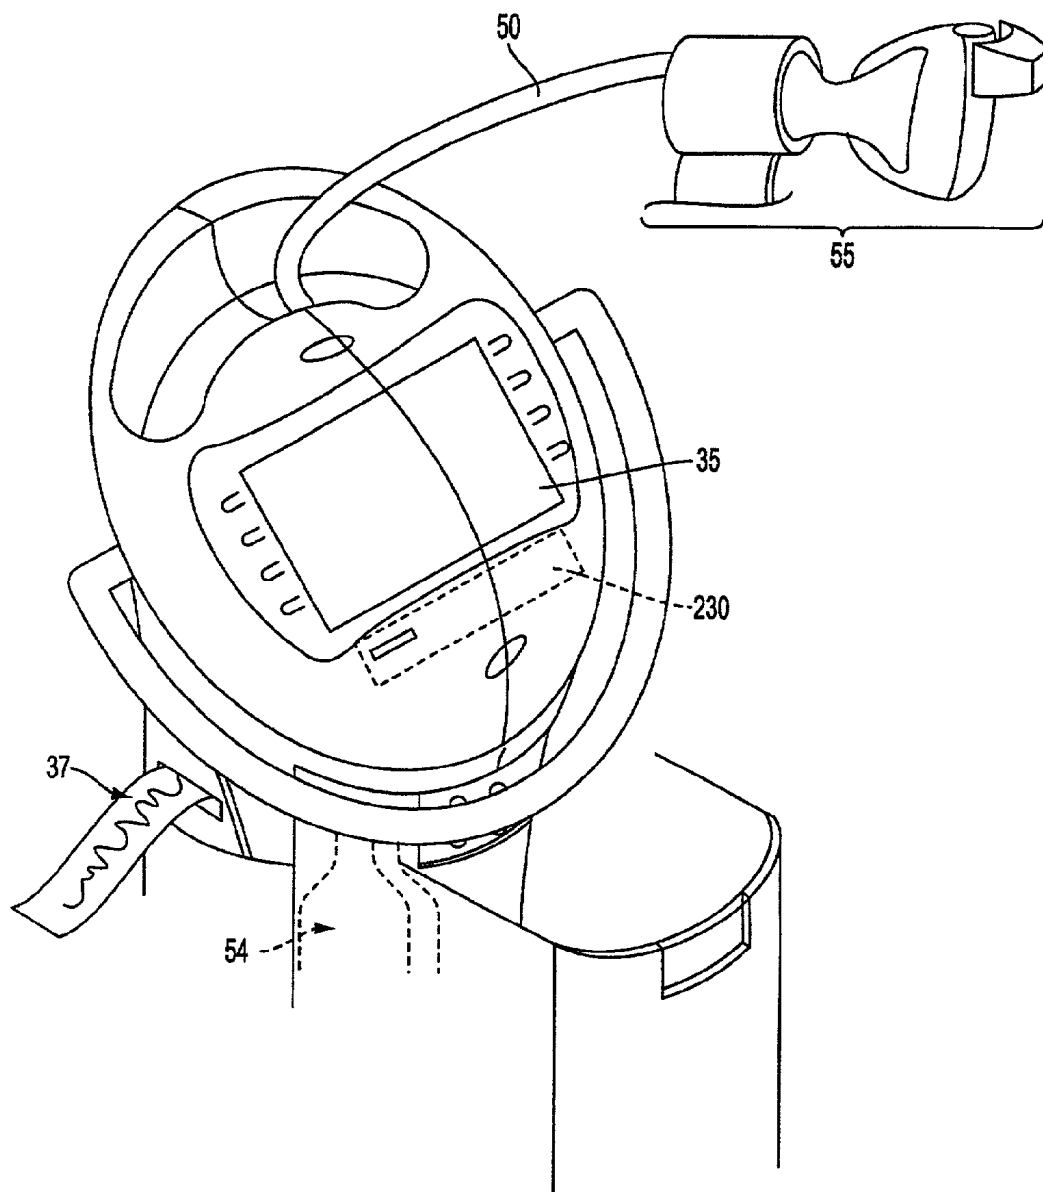


FIG. 2

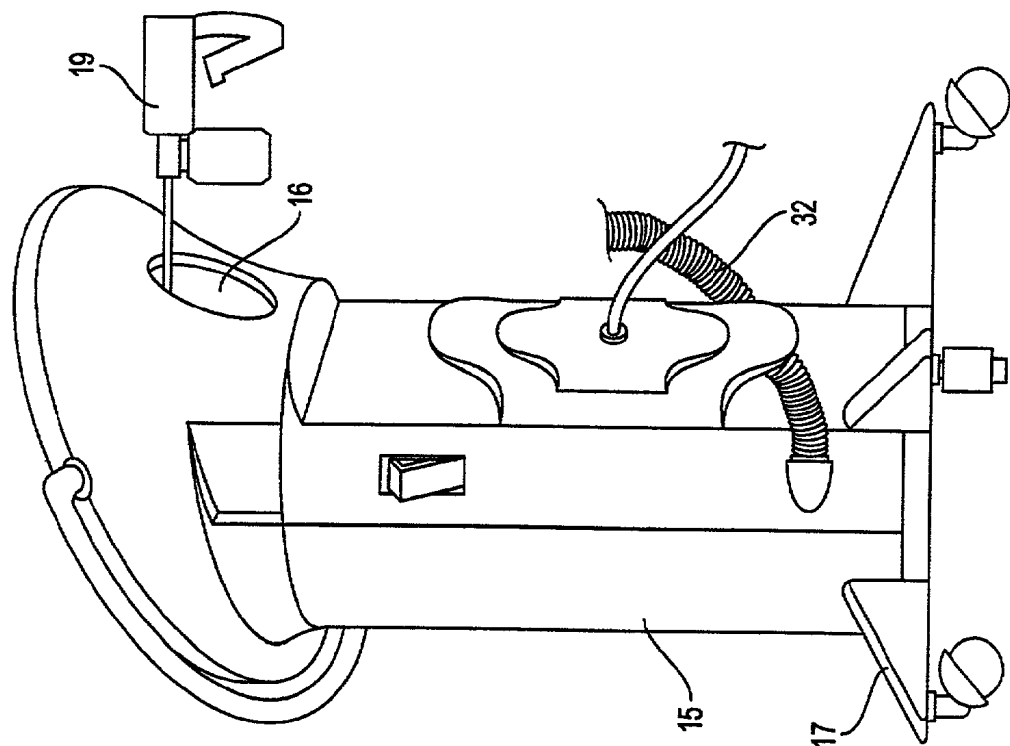


FIG. 3B

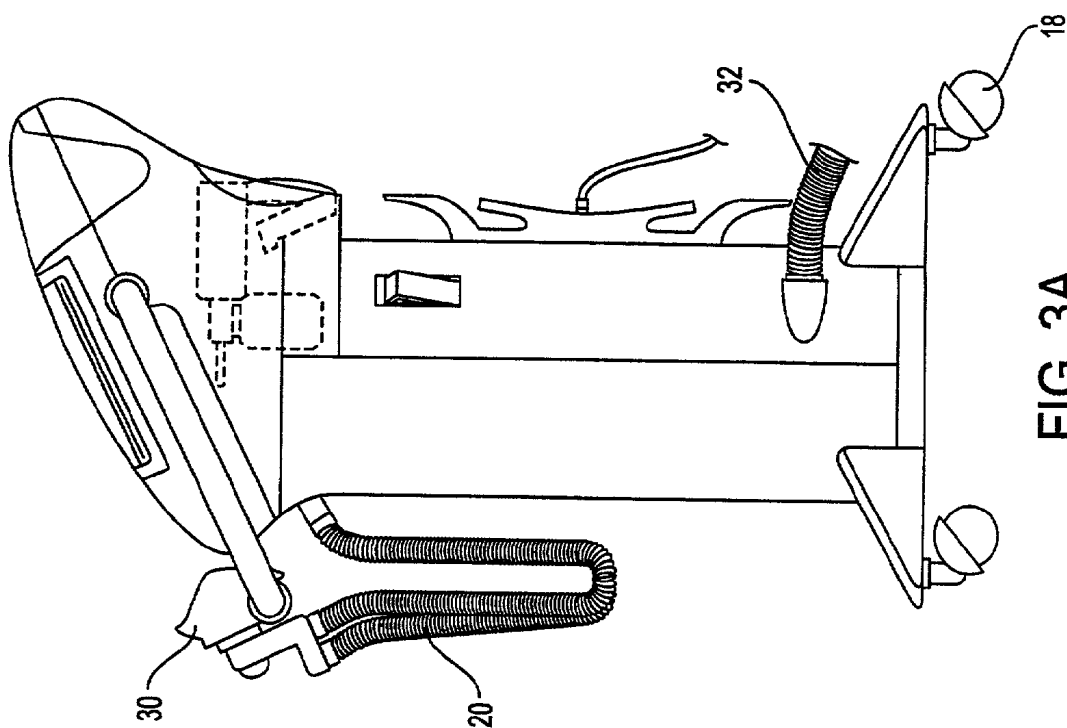


FIG. 3A

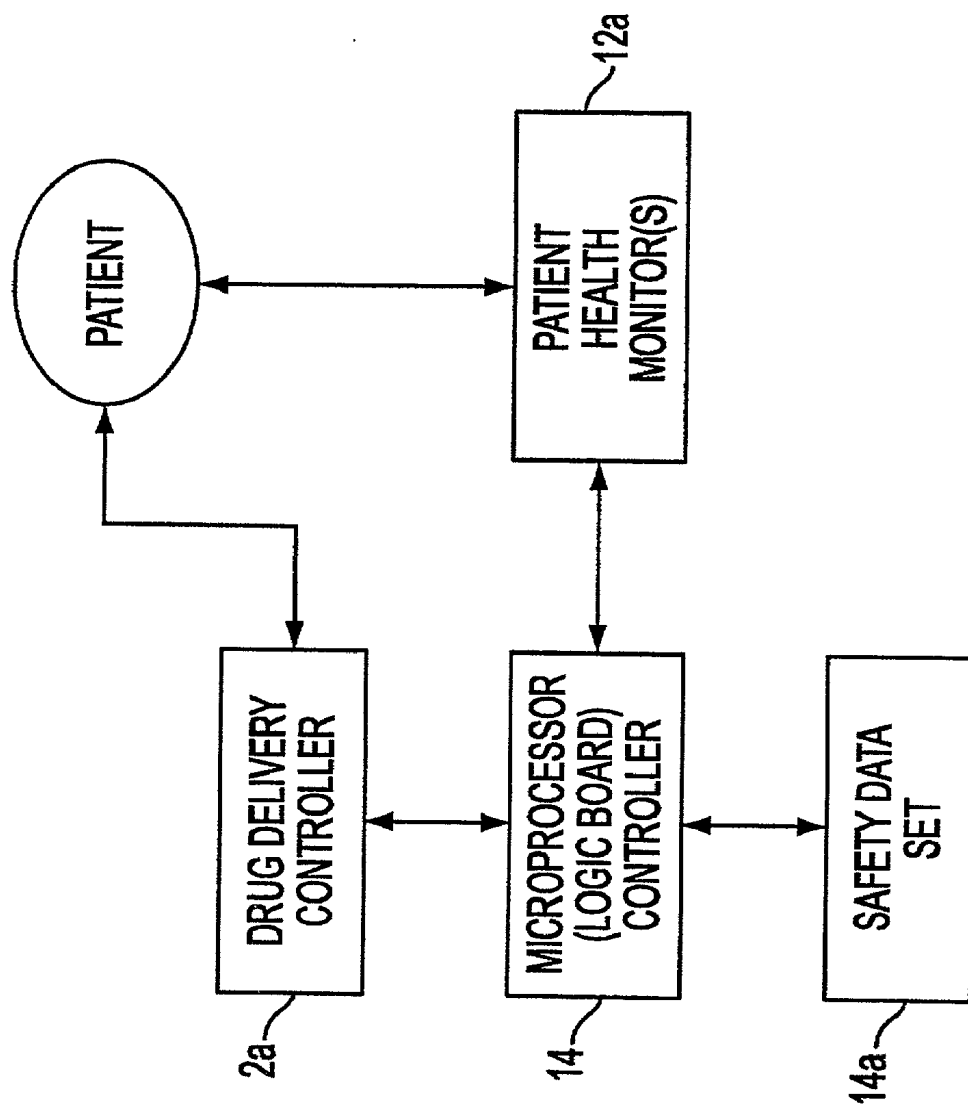


FIG. 4A

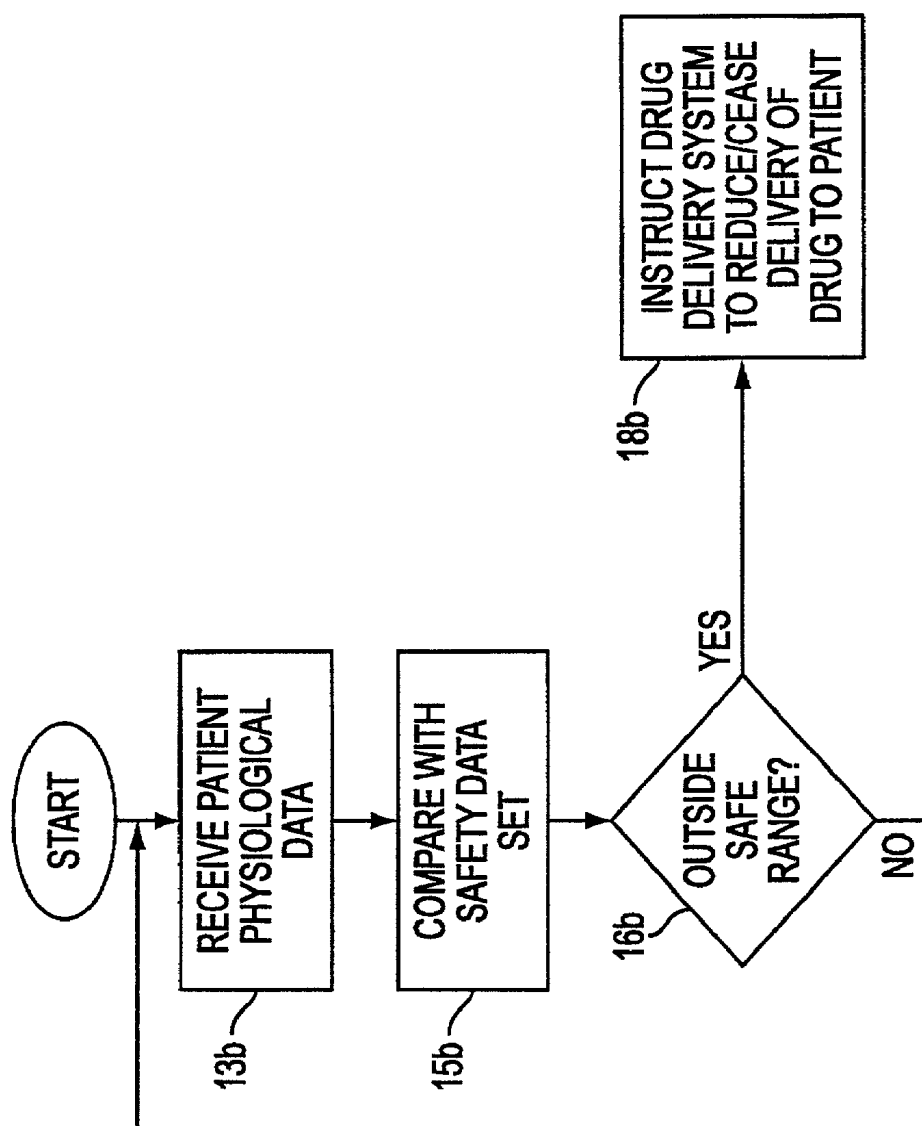


FIG. 4B

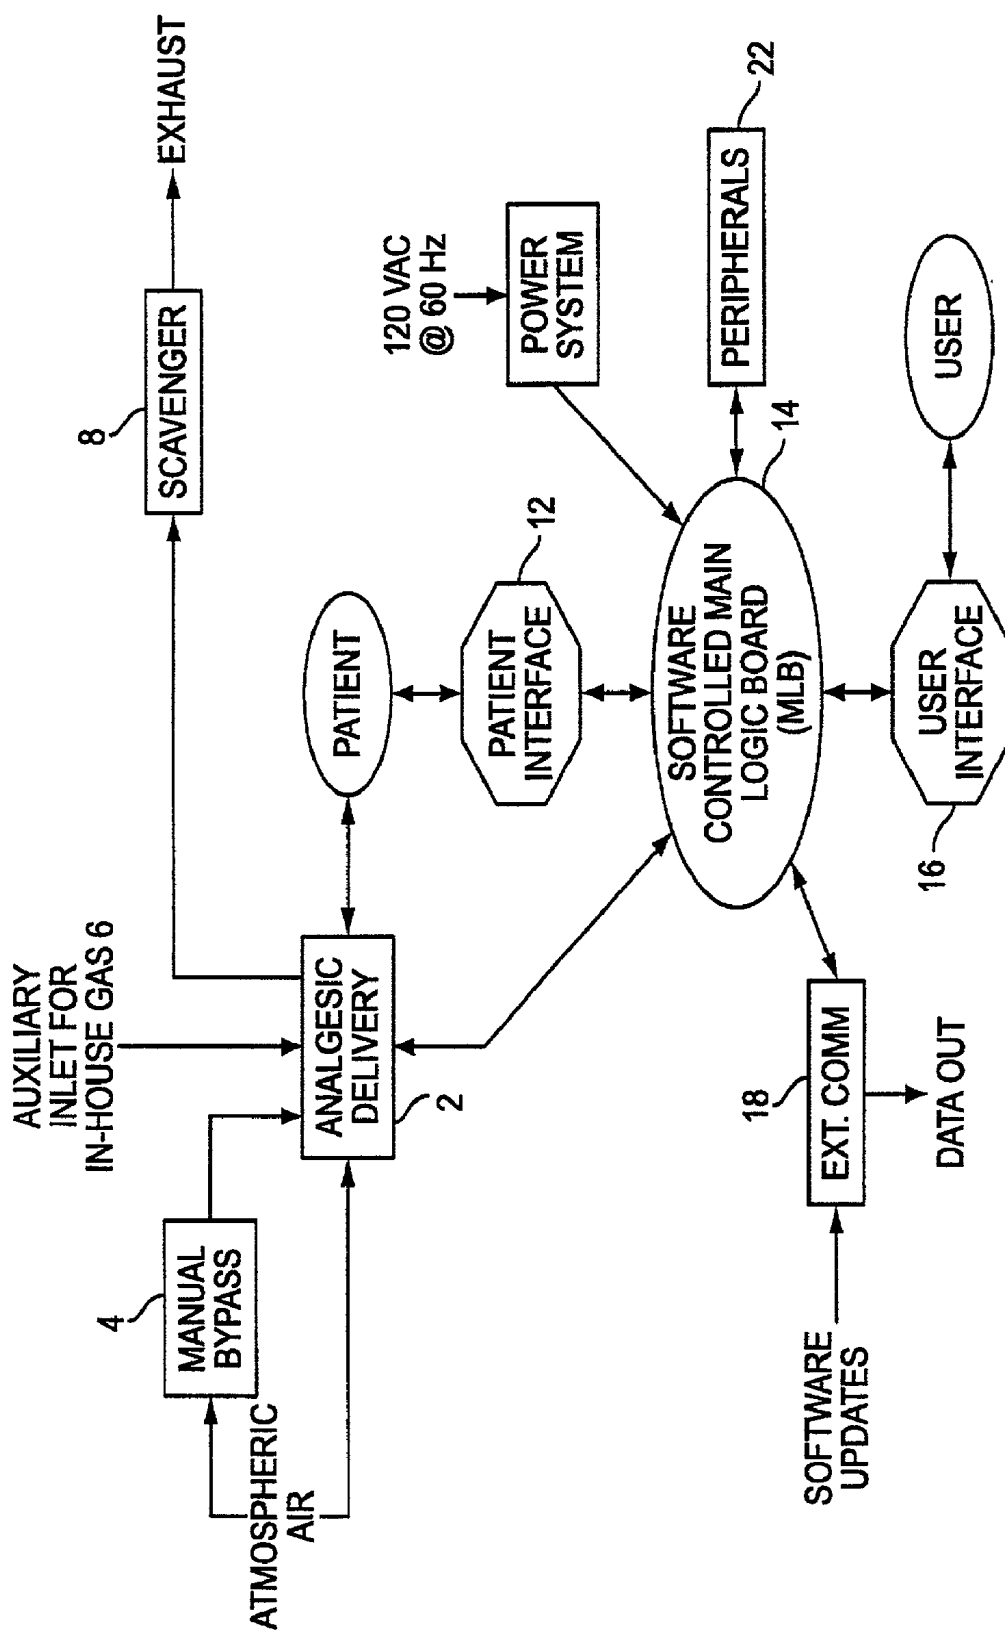


FIG. 5

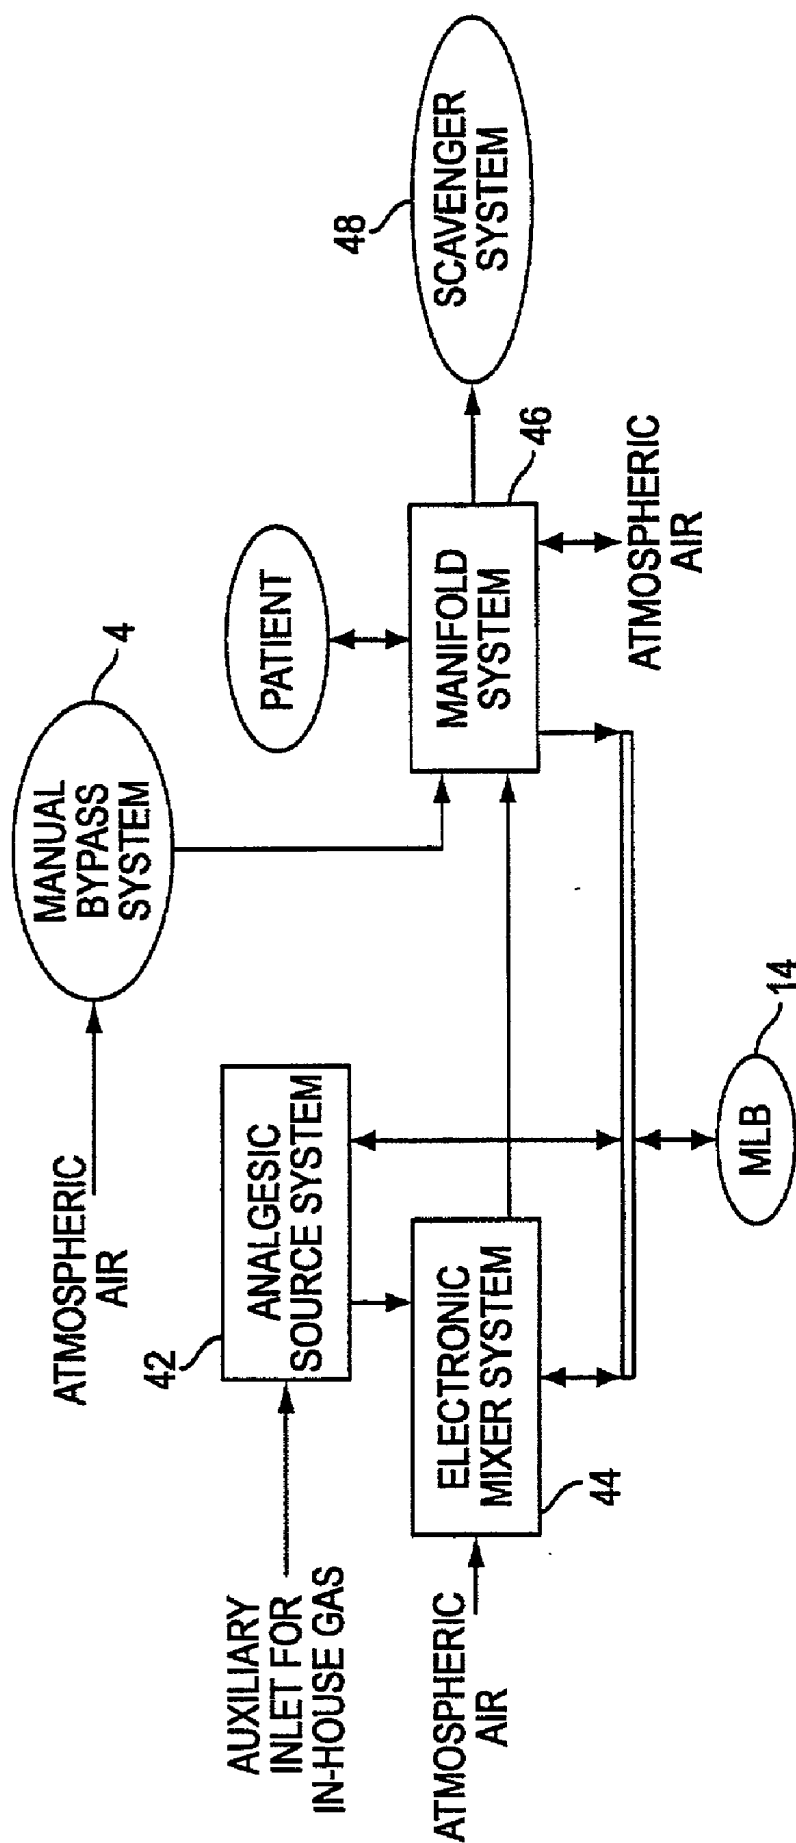


FIG. 6

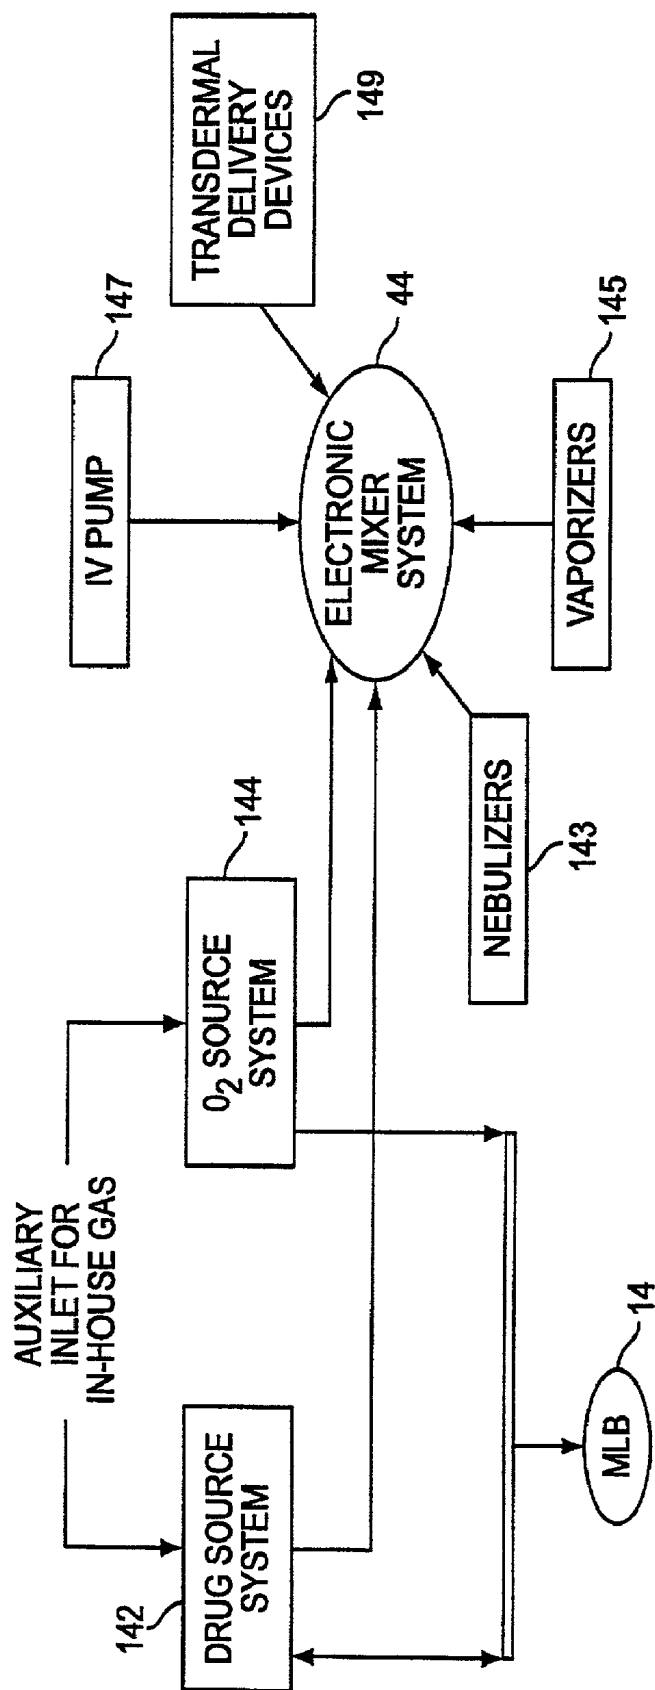


FIG. 7A

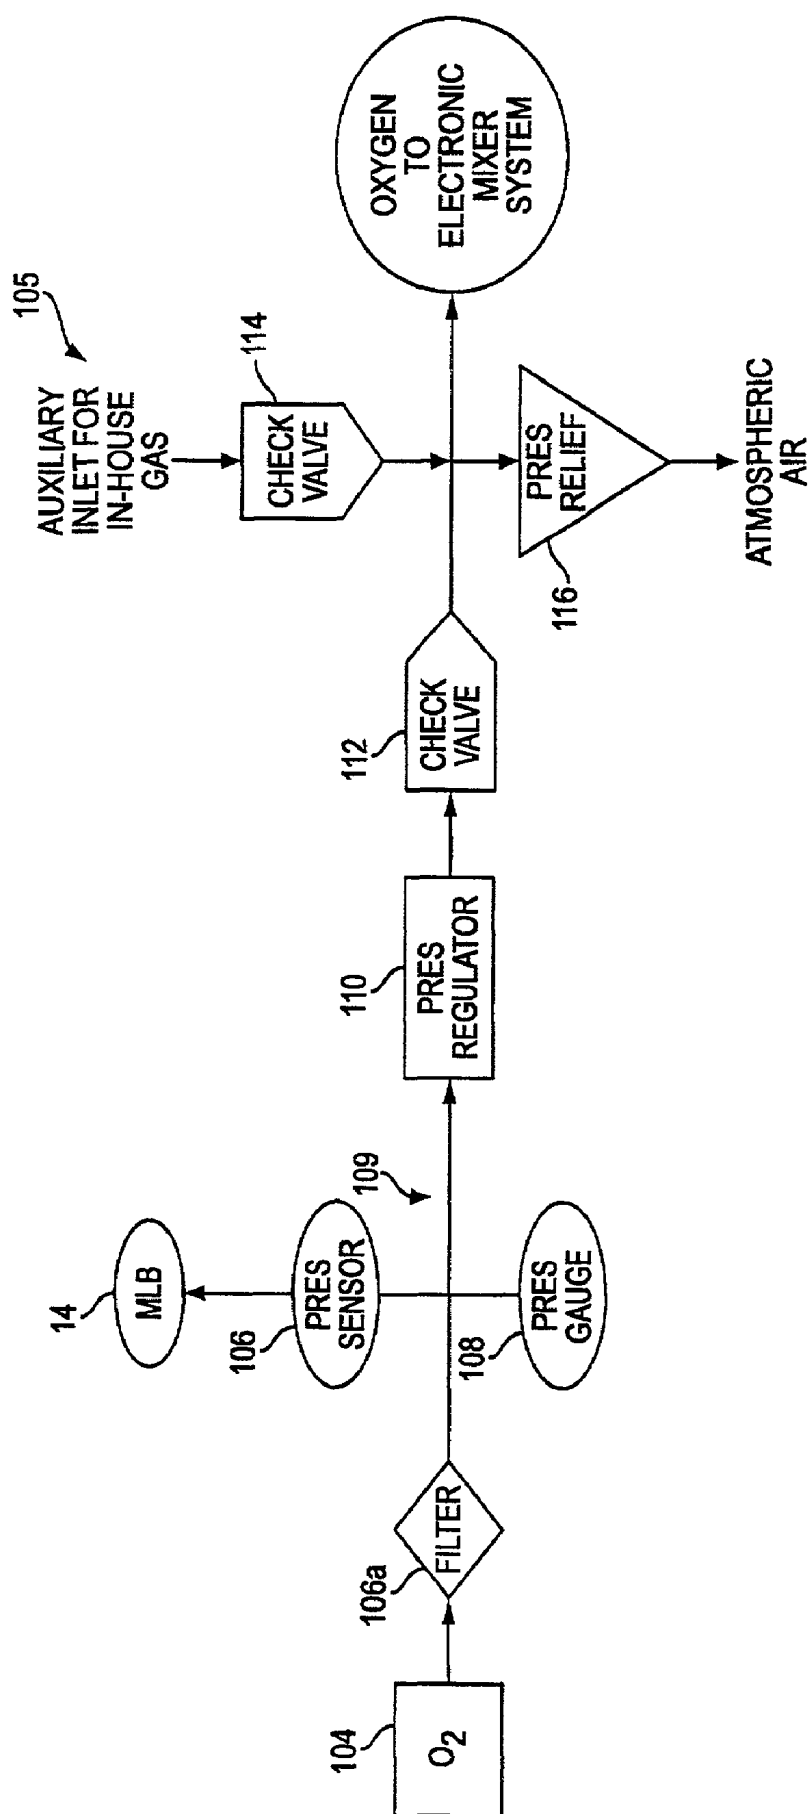


FIG. 7B

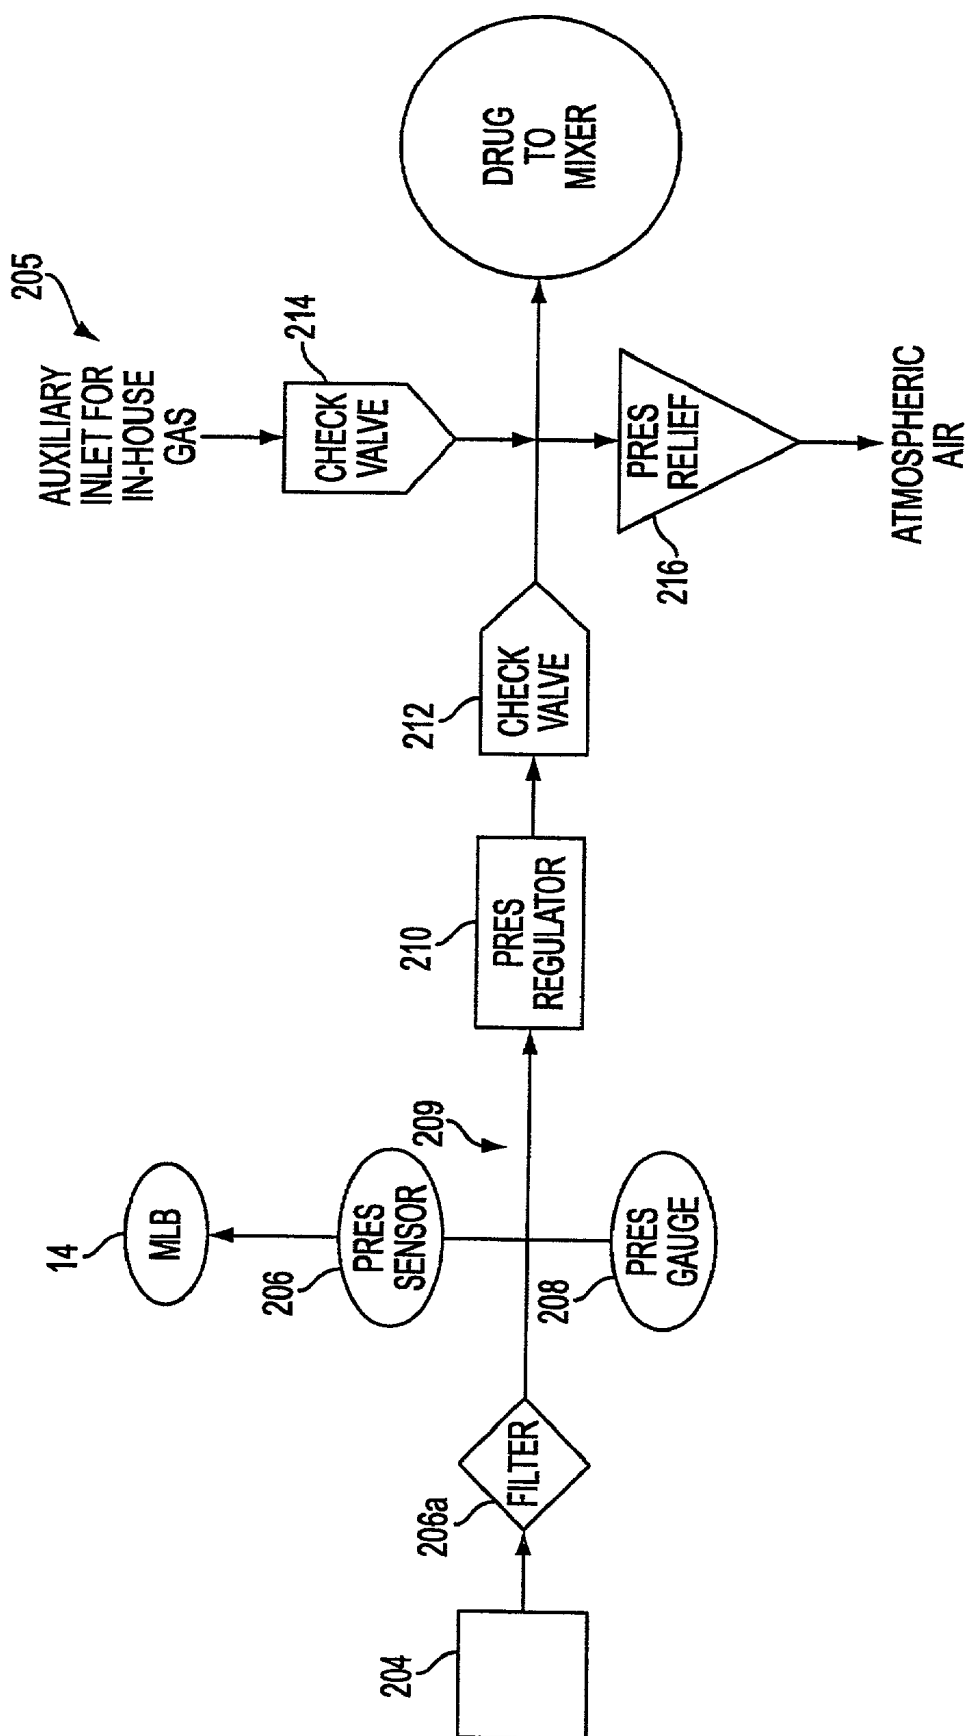


FIG. 7C

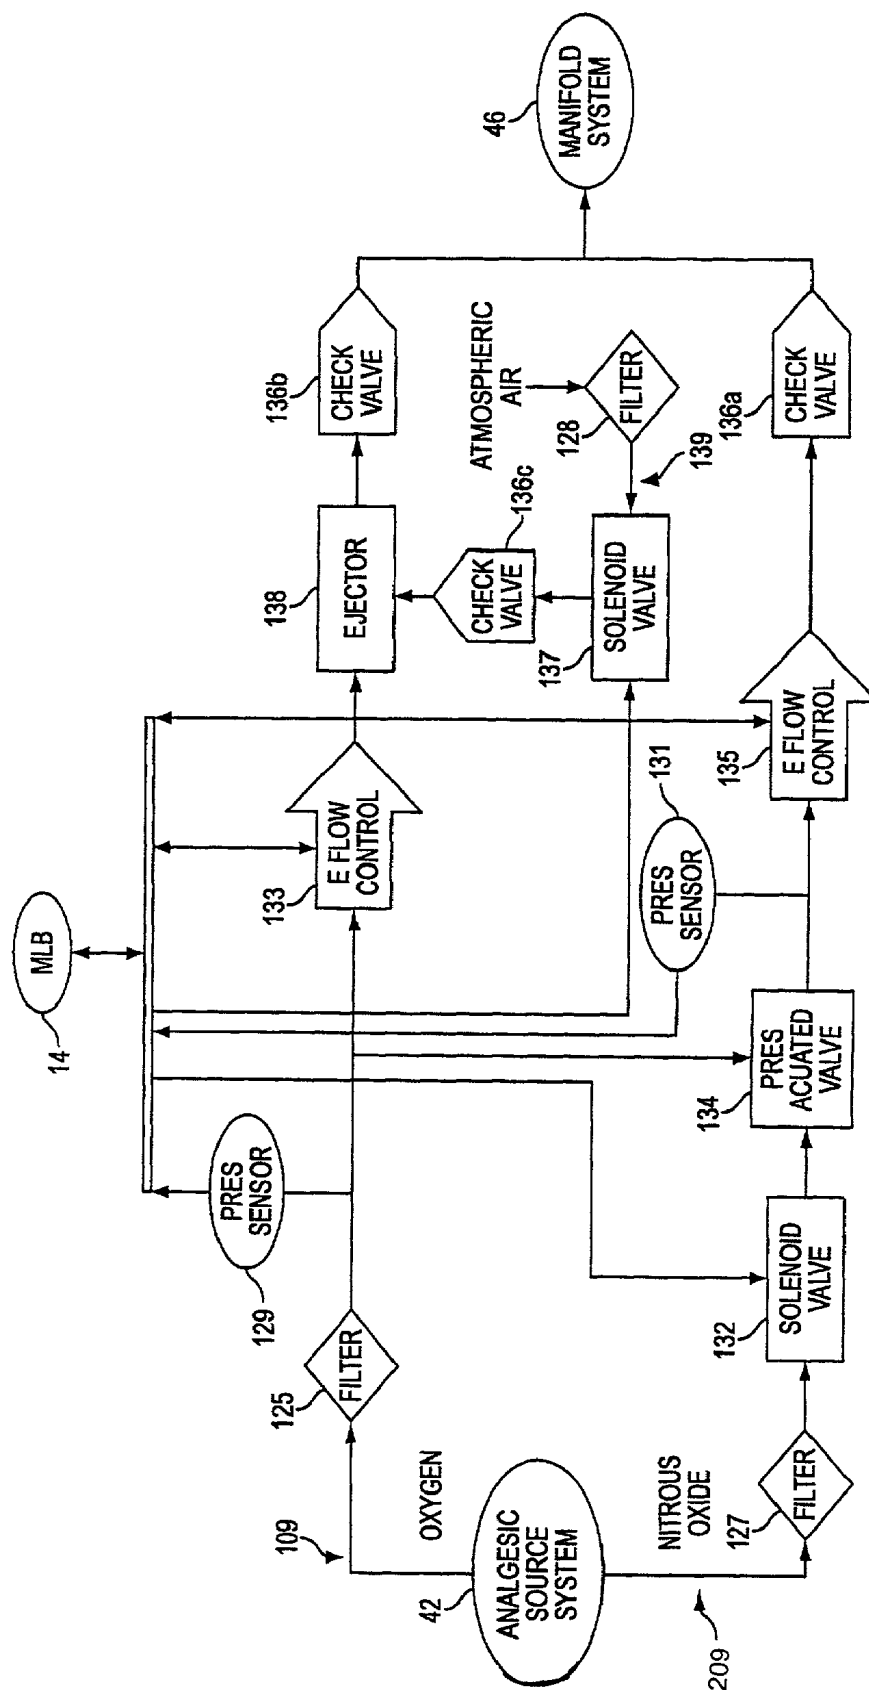


FIG. 8

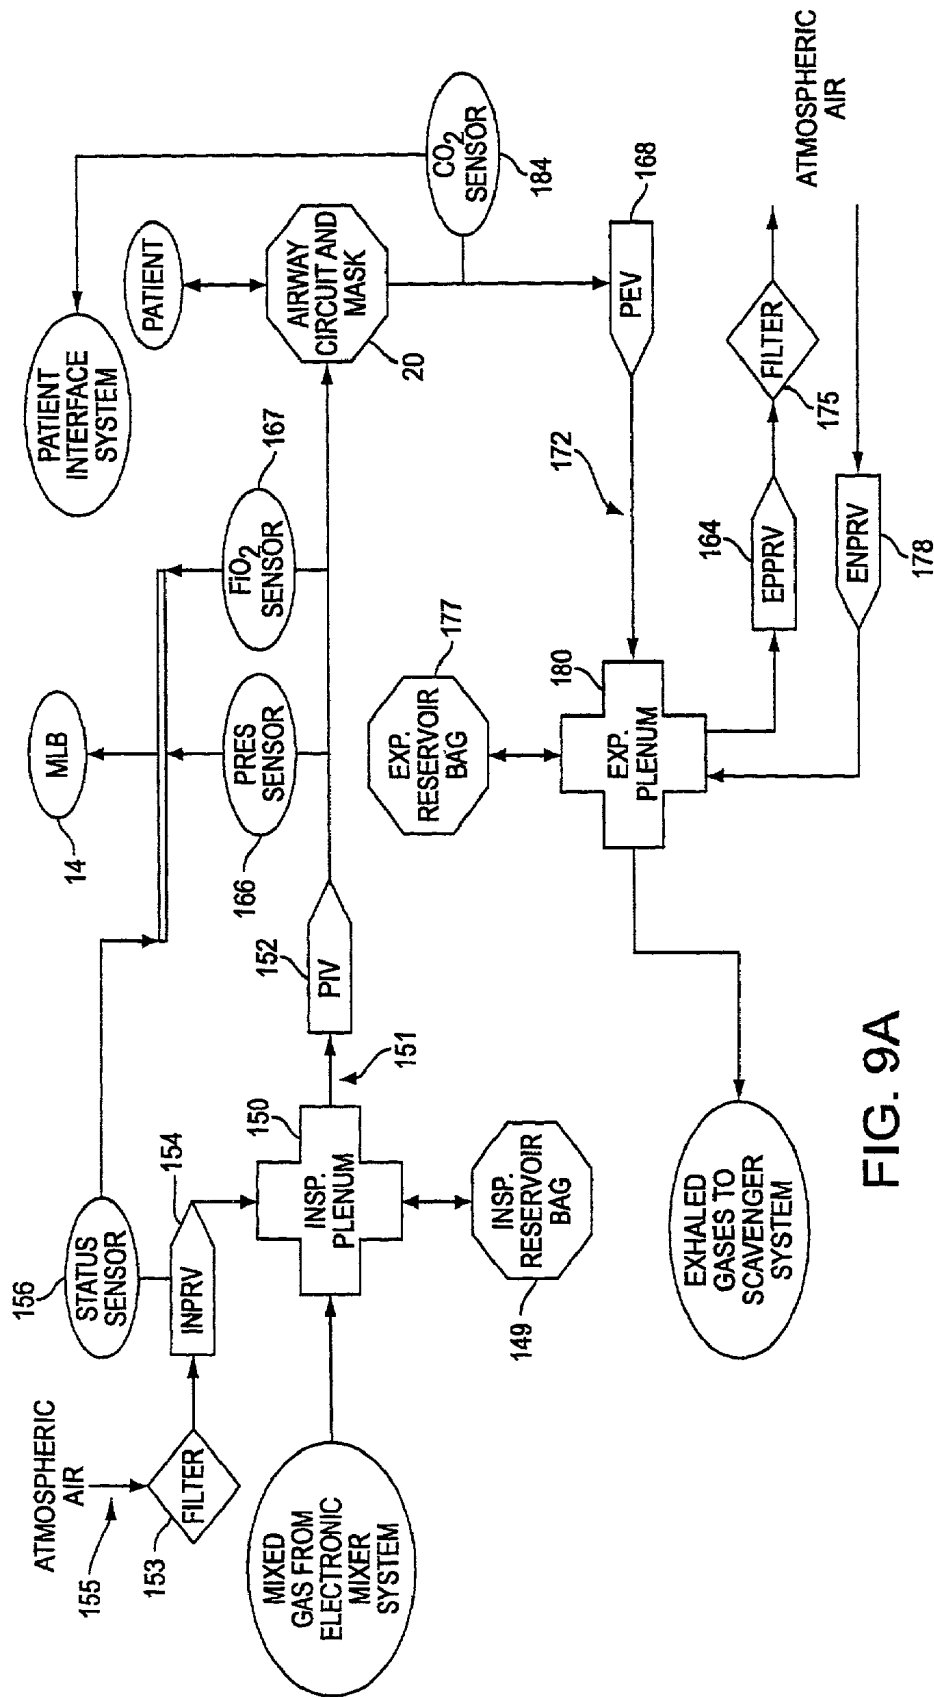


FIG. 9A

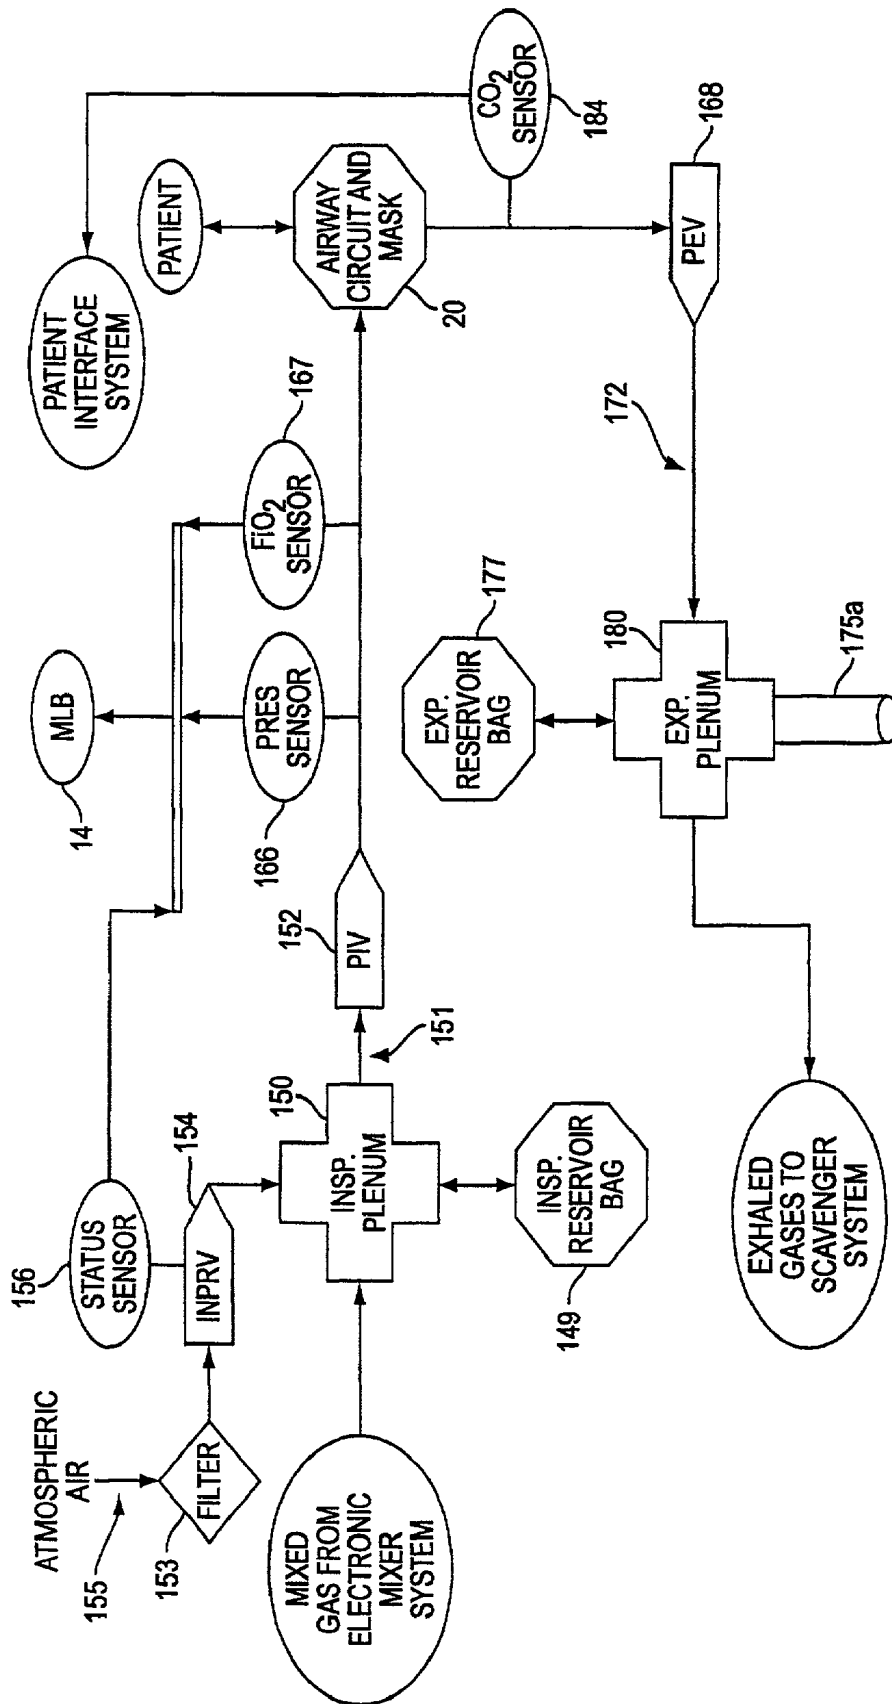


FIG. 9B

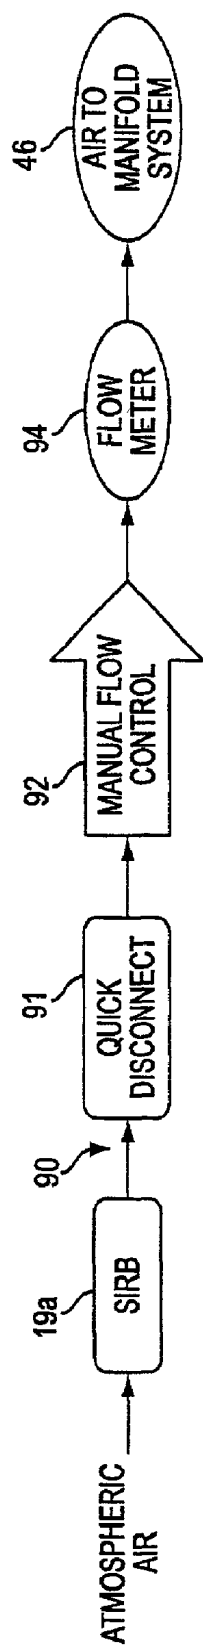


FIG. 10A

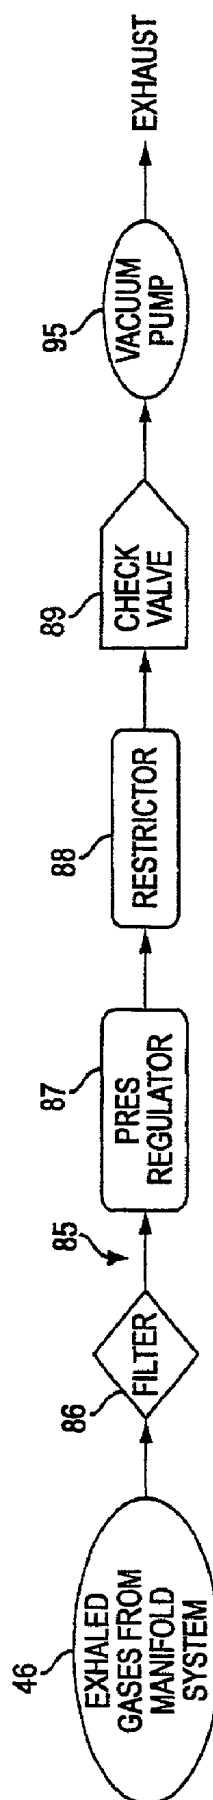


FIG. 10B

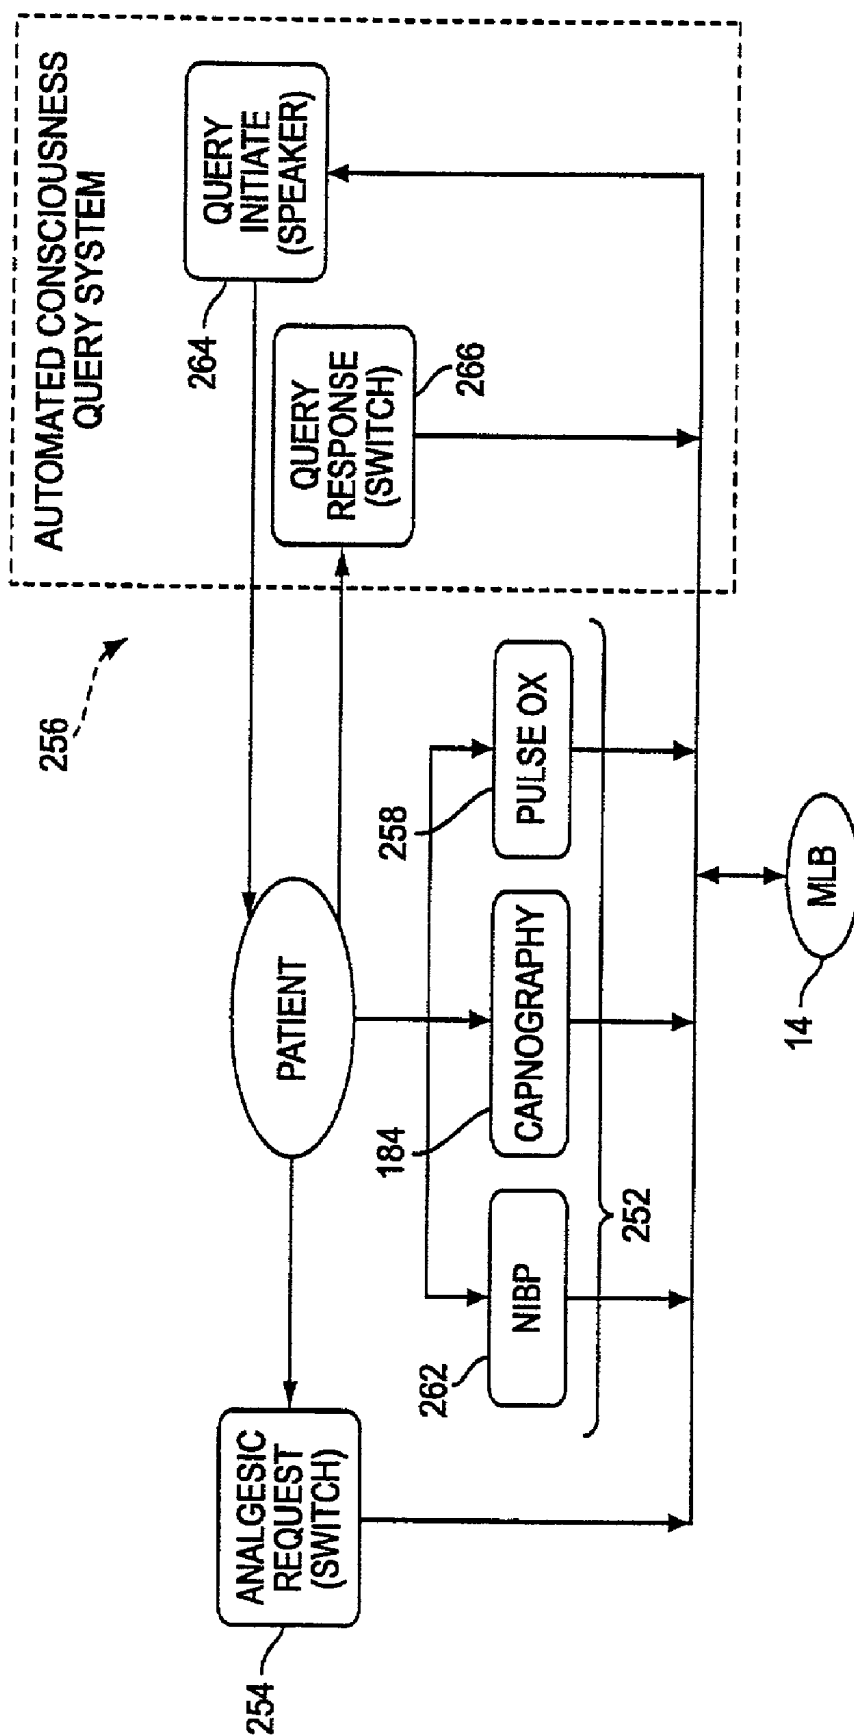
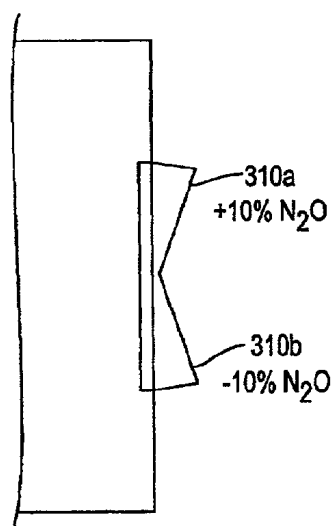
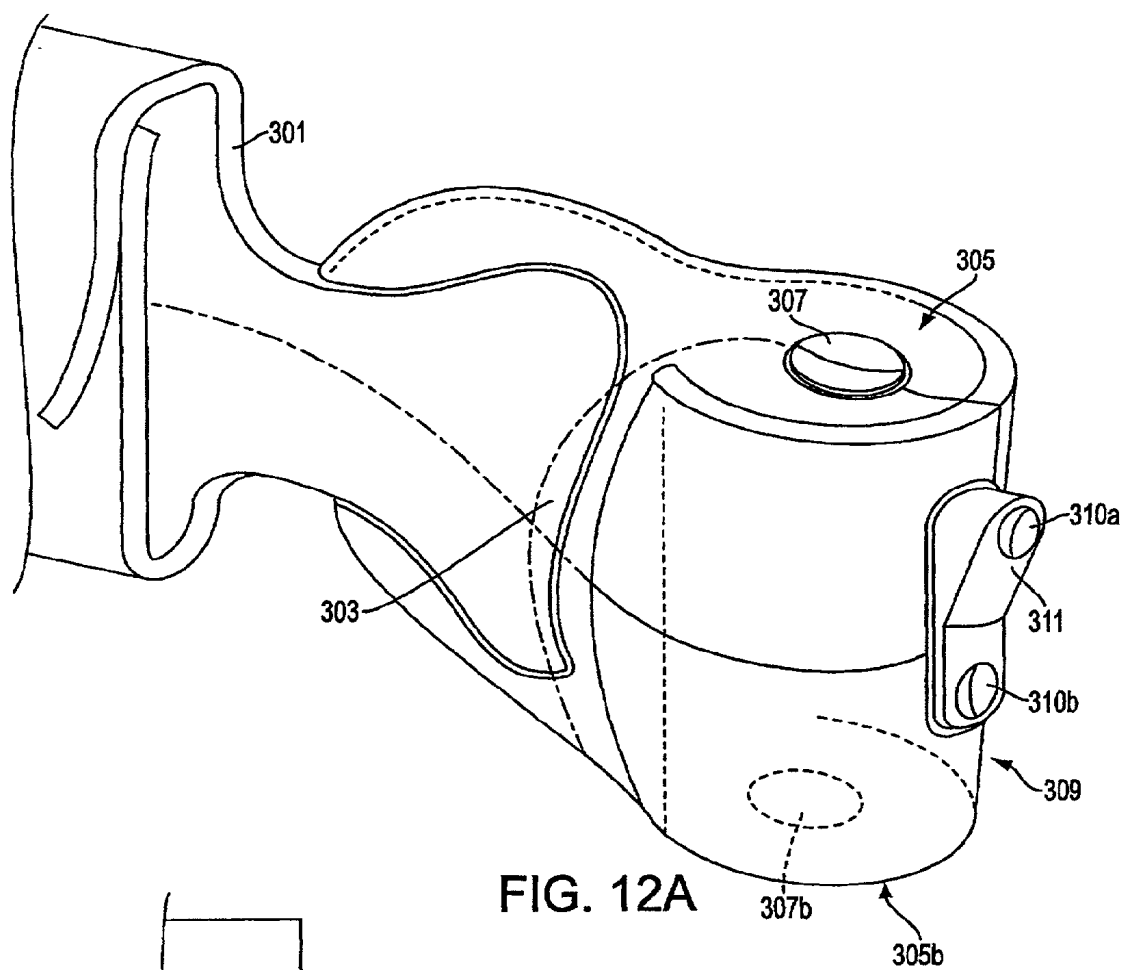


FIG. 11



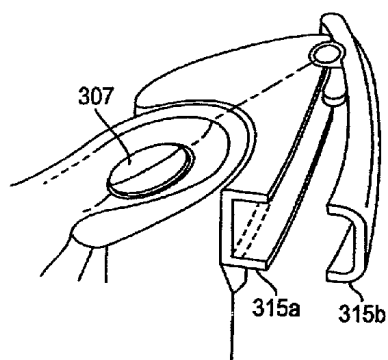


FIG. 13B

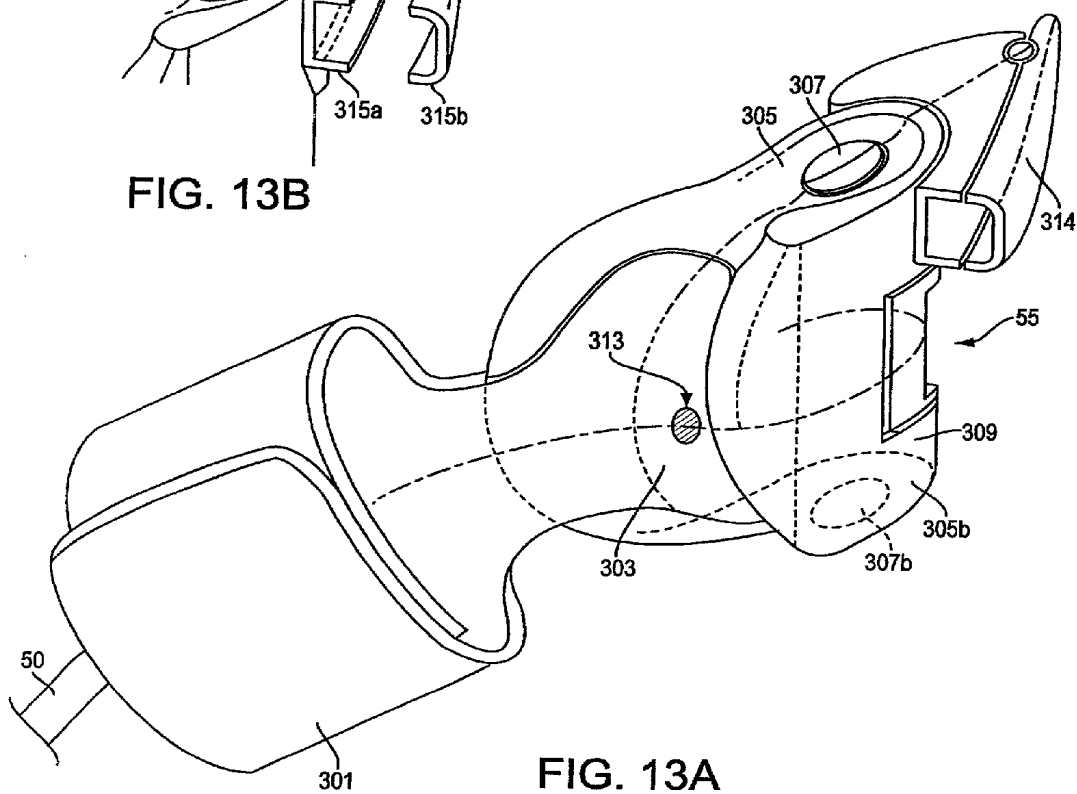


FIG. 13A

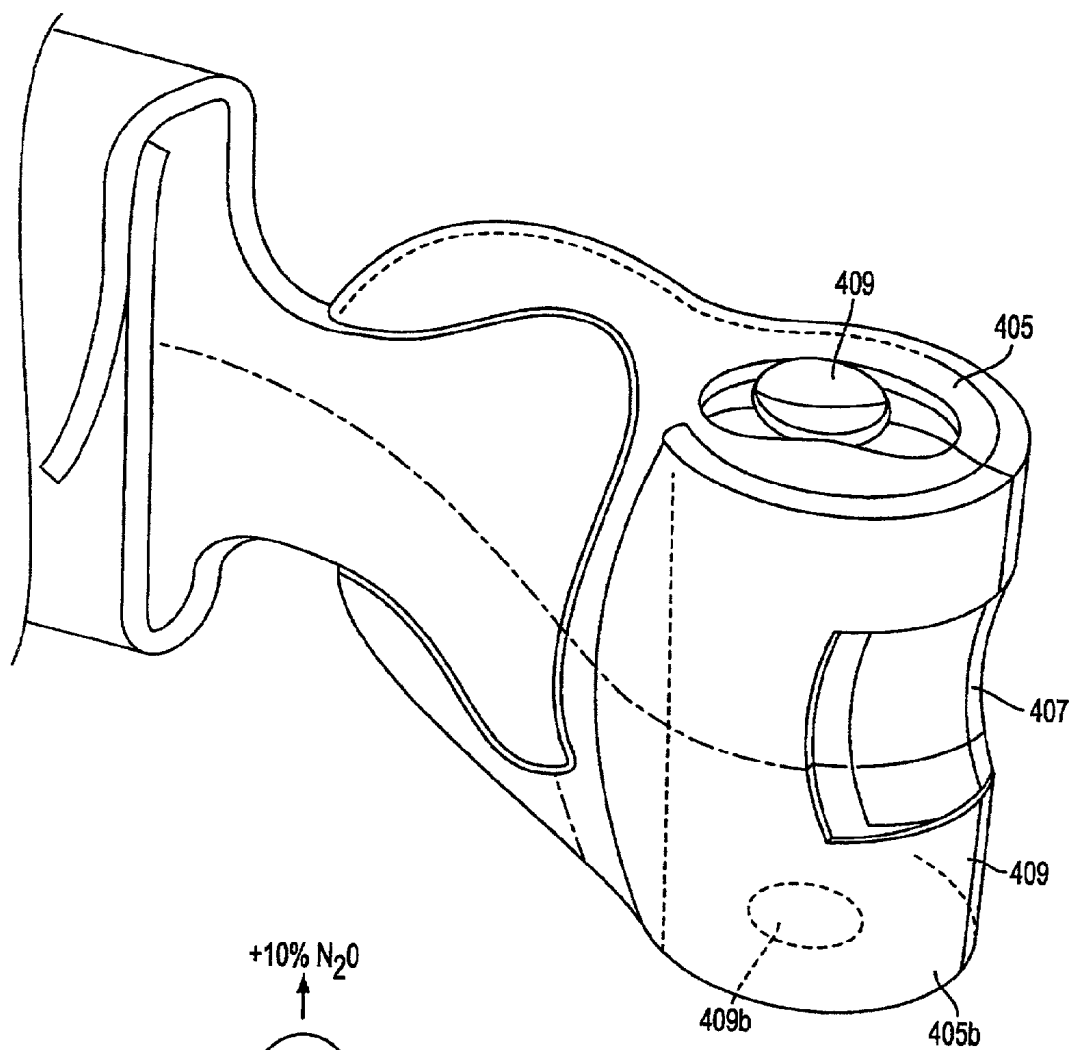


FIG. 14A

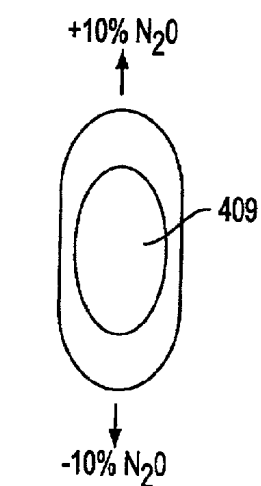


FIG. 14B

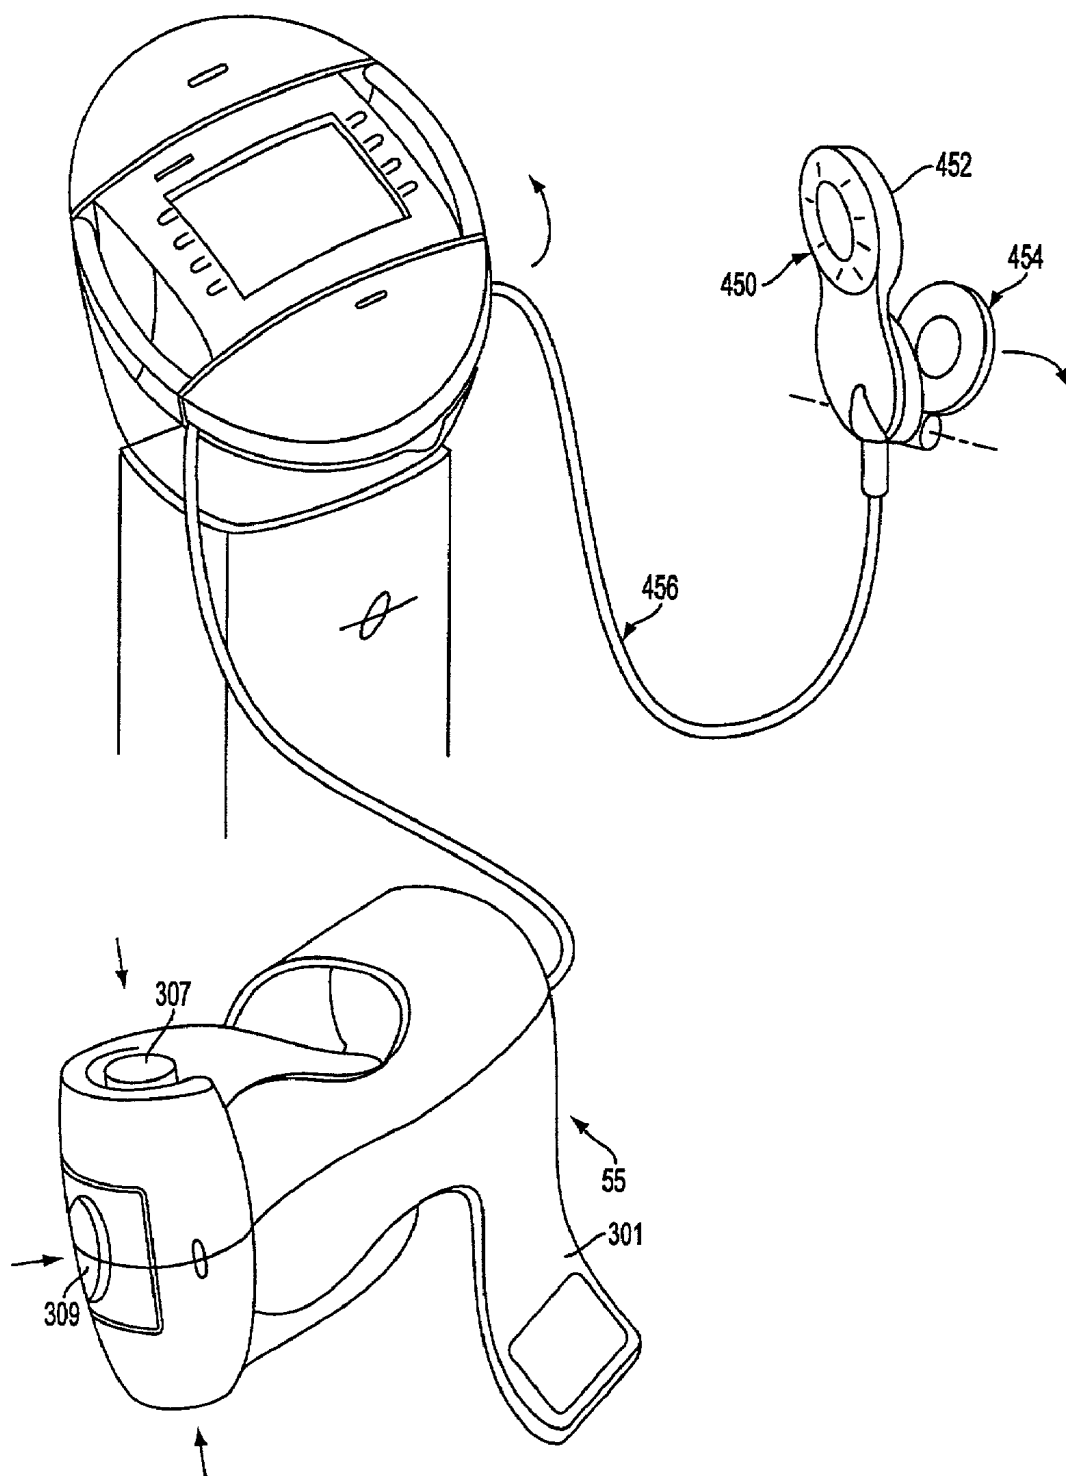


FIG. 15

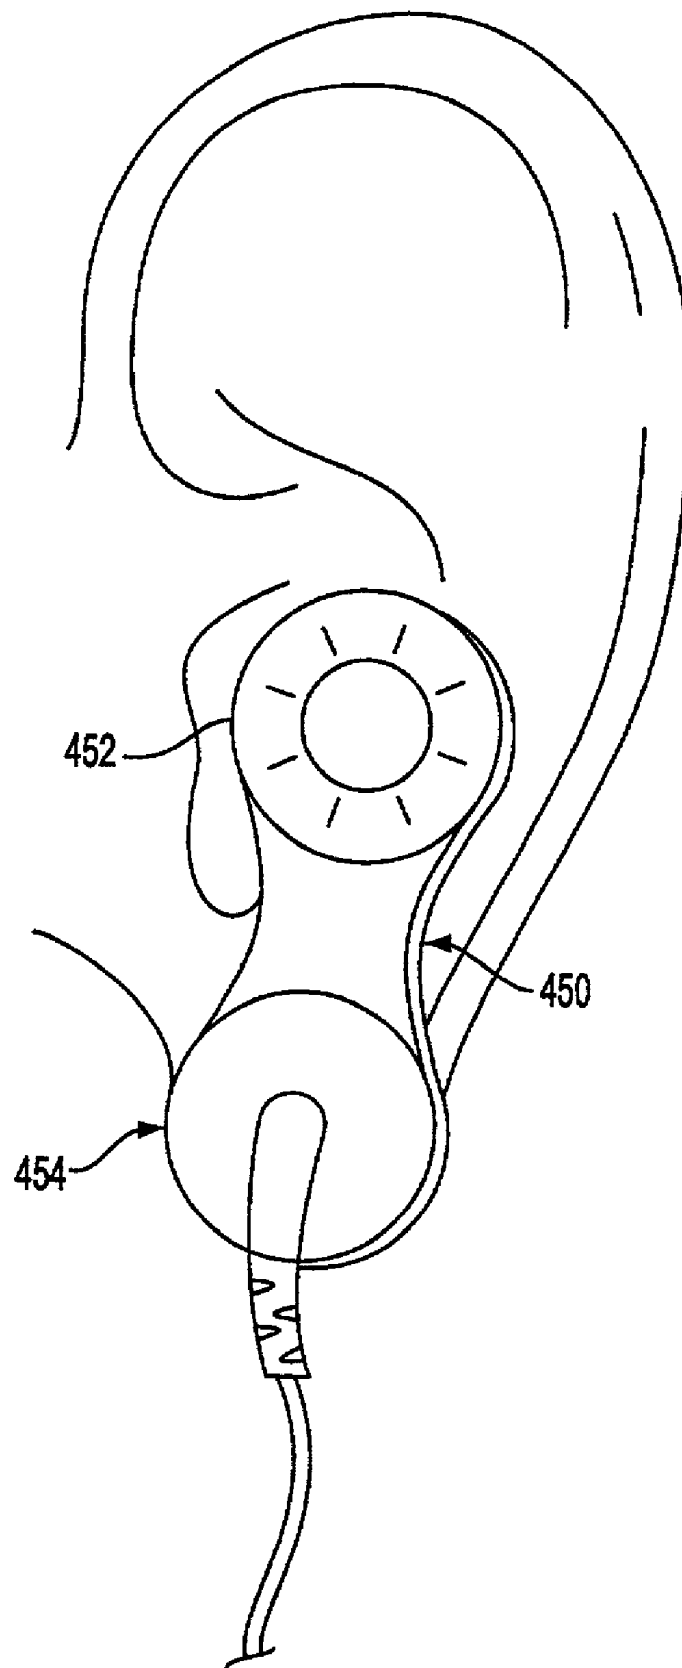


FIG. 16

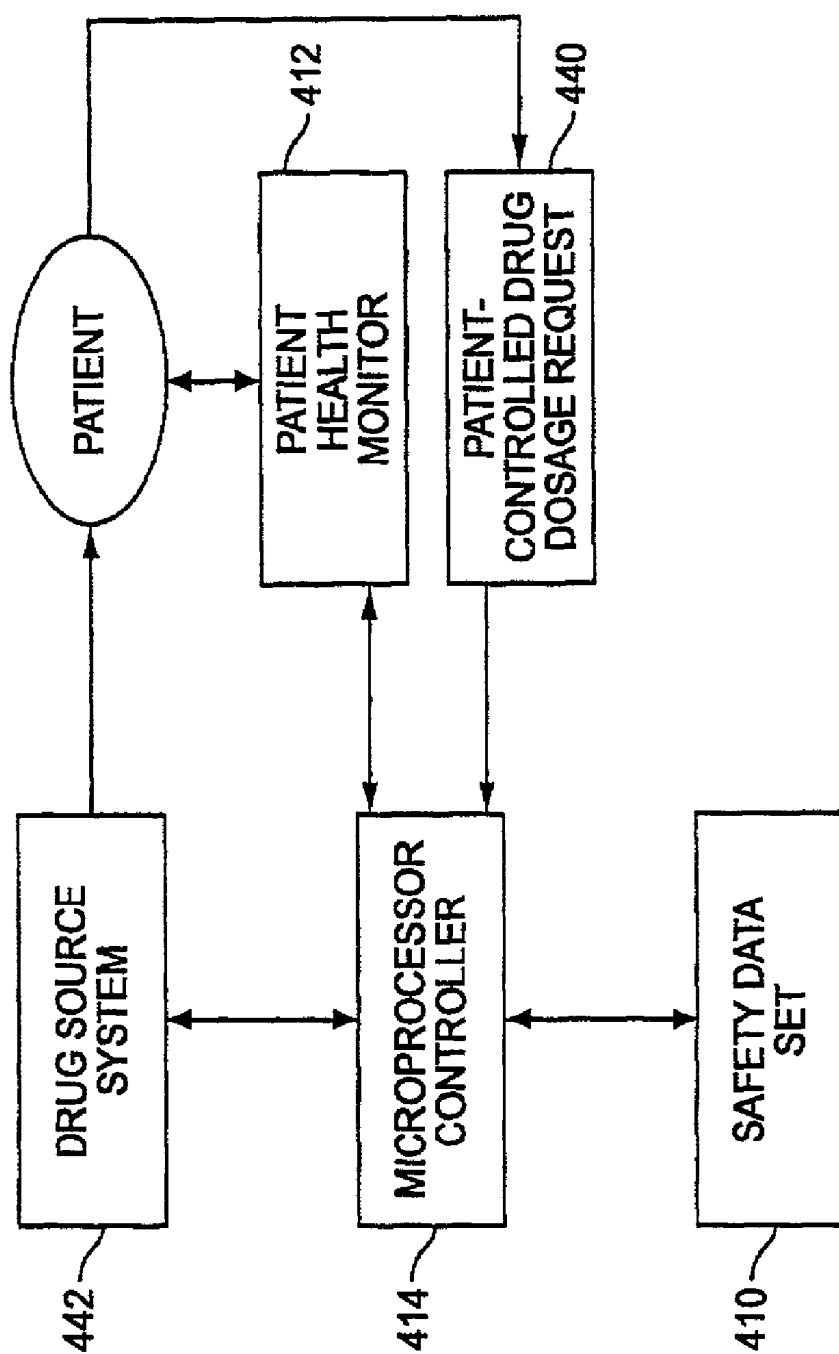


FIG. 17

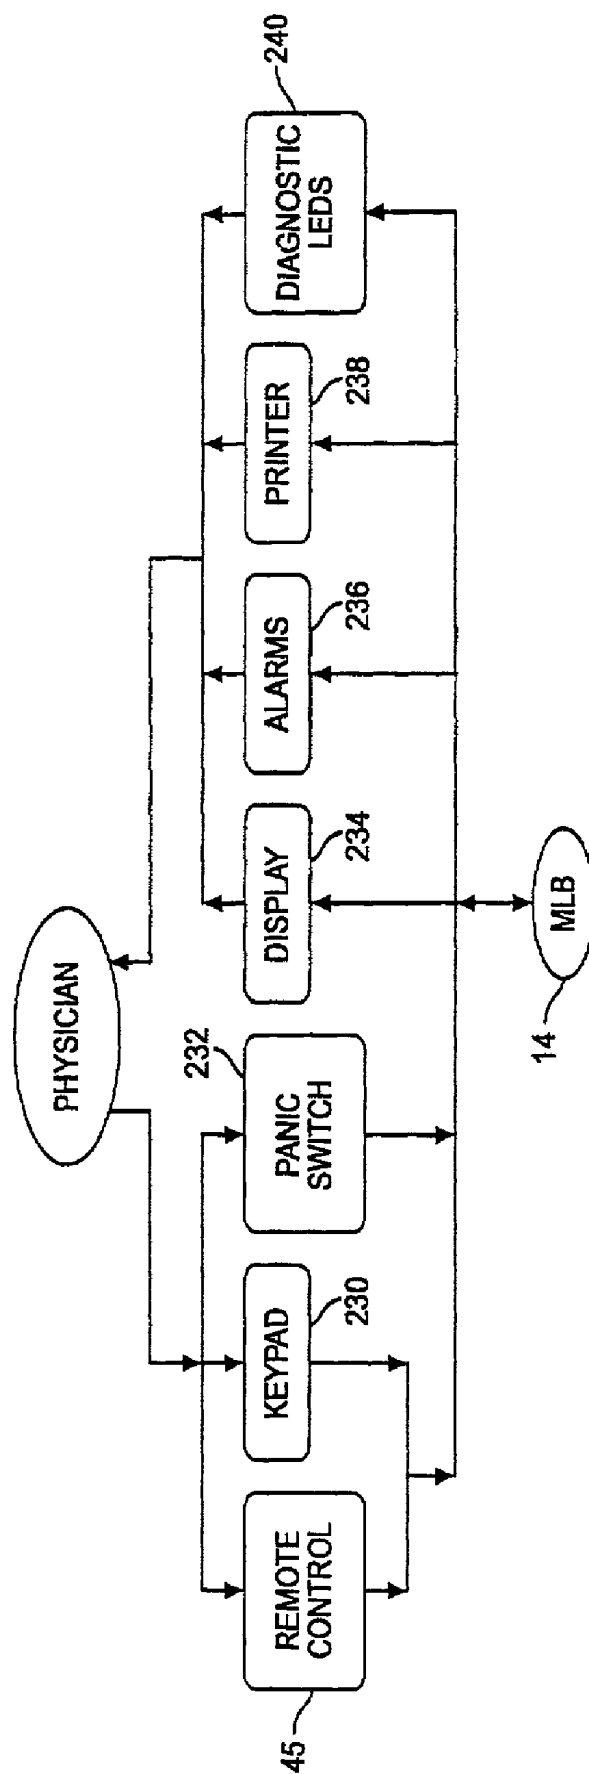


FIG. 18

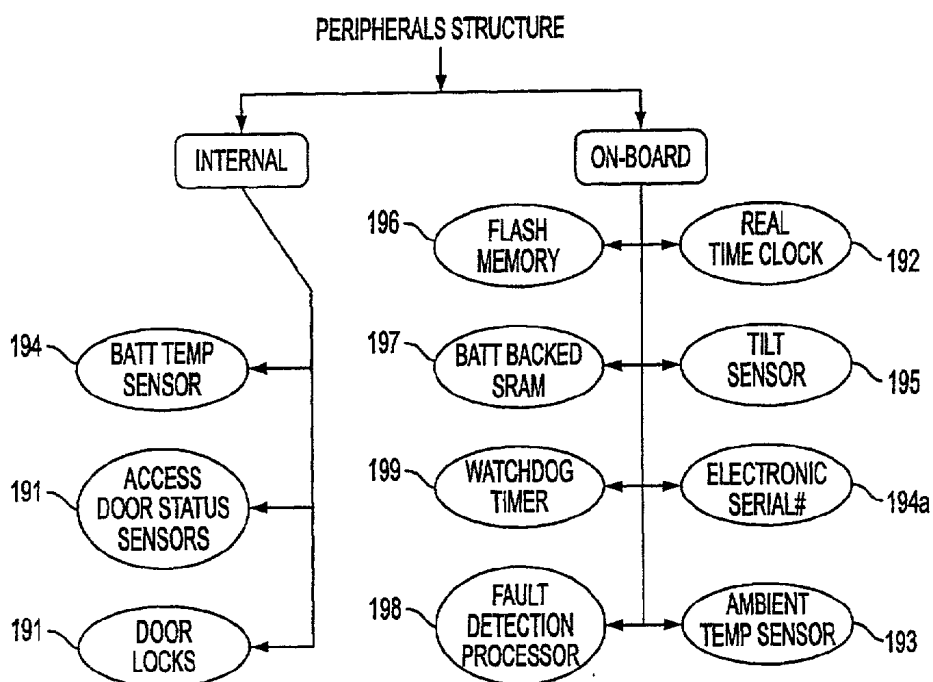


FIG. 19A

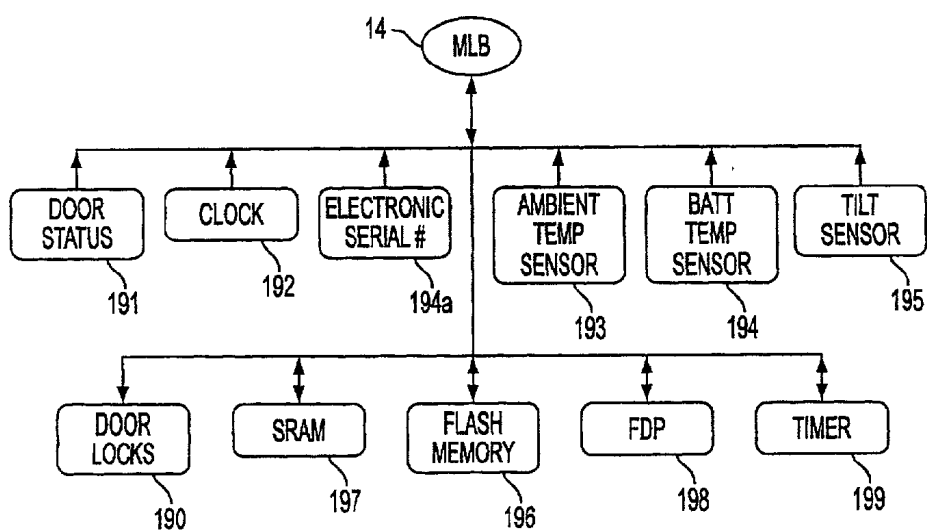


FIG. 19B

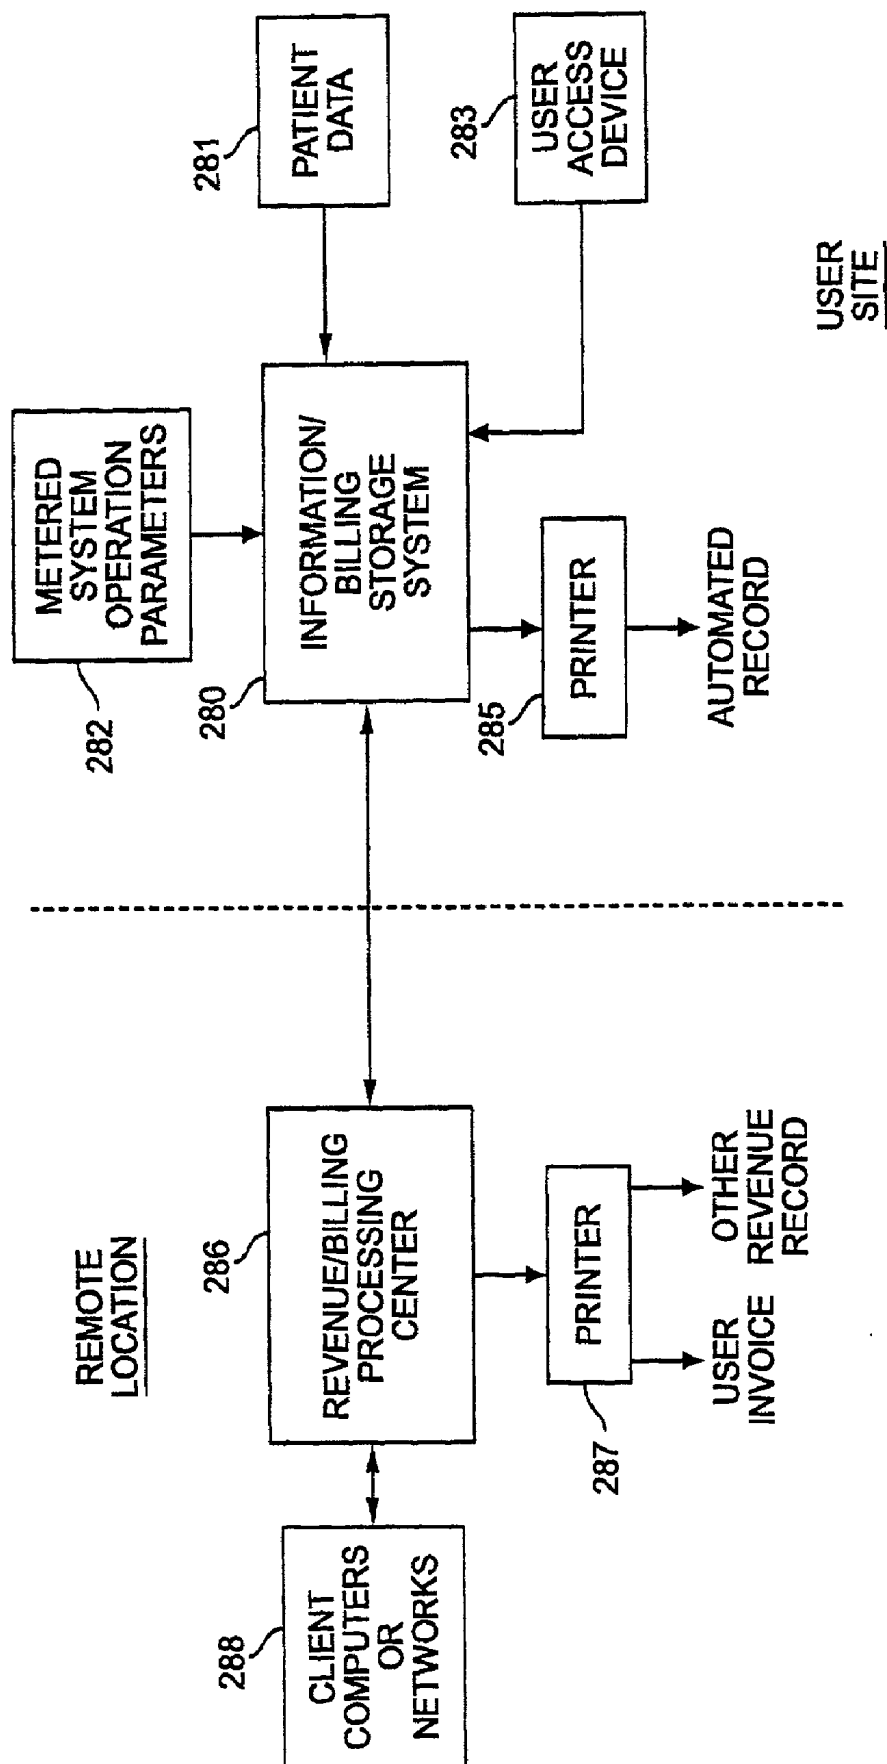


FIG. 20

| PATIENT MONITOR           | MONITOR READING                                                      | ACTION                                                                                                                                                                                                                                                |
|---------------------------|----------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| O <sub>2</sub> SATURATION | ≥ 90%                                                                | NONE                                                                                                                                                                                                                                                  |
|                           | < 90%, ≥ 85%                                                         | ALARM 1 SOUNDS FOR 15 S. IF SILENCED MANUALLY, NO FURTHER ACTION IF NOT SILENCED, N <sub>2</sub> O IS REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10%. SIMILAR ALGORITHMS FOR SEVOFLURANE AND IV INFUSIONS TO BE SPECIFIED. |
|                           | < 85%, ≥ 80%                                                         | ALARM 2 SOUNDS, N <sub>2</sub> O REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10% IMMEDIATELY                                                                                                                                |
|                           | < 80%                                                                | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |
| PULSE RATE                | ≥ 45/min.                                                            | NONE                                                                                                                                                                                                                                                  |
|                           | < 45/min.,<br>≥ 35/min.                                              | ALARM 1 SOUNDS FOR 15 S. IF SILENCED MANUALLY, NO FURTHER ACTION. IF NOT SILENCED, N <sub>2</sub> O IS REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10%                                                                      |
|                           | < 35/min.                                                            | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |
| CO <sub>2</sub> MAXIMUM   | ≤ 50 mm Hg                                                           | NONE                                                                                                                                                                                                                                                  |
|                           | > 50 mm Hg,<br>≤ 55 mm Hg                                            | ALARM 1 SOUNDS FOR 15 S. IF SILENCED MANUALLY, NO FURTHER ACTION. IF NOT SILENCED, N <sub>2</sub> O IS REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10%                                                                      |
|                           | > 55 mm Hg,<br>≤ 60 mm Hg                                            | ALARM 2 SOUNDS, N <sub>2</sub> O REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10% IMMEDIATELY                                                                                                                                |
|                           | < 60 mm Hg                                                           | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |
| RESPIRATION RATE          | APNEA < 1 min.                                                       | NONE                                                                                                                                                                                                                                                  |
|                           | APNEA ≥ 1 min.                                                       | ALARM 2 SOUNDS, N <sub>2</sub> O REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10% IMMEDIATELY                                                                                                                                |
|                           | ALARM 2 AND<br>APNEA ≥ 30 s.                                         | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |
| SYSTOLIC BP               | > 70 mm Hg                                                           | NONE                                                                                                                                                                                                                                                  |
|                           | ≤ 70 mm Hg,<br>> 65 mm Hg                                            | ALARM 1 SOUNDS FOR 15 S. IF SILENCED MANUALLY, NO FURTHER ACTION. IF NOT SILENCED, N <sub>2</sub> O IS REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10%                                                                      |
|                           | ≤ 65 mm Hg,<br>> 60 mm Hg                                            | ALARM 2 SOUNDS, N <sub>2</sub> O REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10% IMMEDIATELY                                                                                                                                |
|                           | ≤ 60 mm Hg                                                           | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |
| CONSCIOUSNESS MONITOR     | PATIENT RESPONDS                                                     | NONE                                                                                                                                                                                                                                                  |
|                           | PATIENT DOES NOT RESPOND                                             | ALARM 1 SOUNDS FOR 15 S. IF SILENCED MANUALLY, NO FURTHER ACTION. IF NOT SILENCED, N <sub>2</sub> O IS REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10%                                                                      |
|                           | ALARM 1 AND<br>PATIENT DOES NOT RESPOND<br>TO STIMULUS<br>30 s LATER | ALARM 2 SOUNDS, N <sub>2</sub> O REDUCED TO THE LESSER CONCENTRATION OF 45% OR CURRENT CONCENTRATION - 10% IMMEDIATELY                                                                                                                                |
|                           | ALARM 2 AND<br>PATIENT DOES NOT RESPOND<br>TO STIMULUS<br>30 s LATER | ALARM 3 SOUNDS, N <sub>2</sub> O REDUCED TO 0%                                                                                                                                                                                                        |

FIG. 21

| MONITOR                               | UNIT         | TRANSITION REQUIREMENT     | VALUE        |                                                                                            |                                                |
|---------------------------------------|--------------|----------------------------|--------------|--------------------------------------------------------------------------------------------|------------------------------------------------|
| O <sub>2</sub> TANK PRESSURE          | PSI          | LOW TANK PRESSURE          | > SETPOINT   | < SETPOINT                                                                                 | N/A                                            |
| O <sub>2</sub> INTERRUPTION FAIL-SAFE | LOGICAL      | O <sub>2</sub> INTERRUPTED | FALSE        | N/A                                                                                        | TRUE                                           |
| TOTAL GAS FLOW                        | LITERS / MIN | LOW GAS FLOW               | > SETPOINT   | < SETPOINT                                                                                 | N/A                                            |
| N <sub>2</sub> O TANK PRESSURE        | PSI          | LOW TANK PRESSURE          | > SETPOINT   | < SETPOINT                                                                                 | N/A                                            |
| FiO <sub>2</sub>                      | %            | LOW FiO <sub>2</sub>       | >= 30        | N/A                                                                                        | < 30                                           |
| VACUUM PUMP                           | LOGICAL      | INSUFFICIENT VACUUM PUMP   | OK           | FAIL                                                                                       | N/A                                            |
| POWER                                 | LOGICAL      | INTERRUPTION IN POWER      | OK           | N/A                                                                                        | FAIL                                           |
|                                       |              | NORMAL                     | NO CHANGE    | START ALARM 1                                                                              | START ALARM 2<br>REDUCE N <sub>2</sub> O TO 0% |
|                                       |              |                            | NORMAL       | ALARM 1                                                                                    | ALARM 2                                        |
|                                       |              | ALARM 1                    | STOP ALARM 1 | IF DURATION > 15 SEC AND NOT SILENCED THEN REDUCE N <sub>2</sub> O TO 45% OR CURRENT - 10% | START ALARM 2<br>REDUCE N <sub>2</sub> O TO 0% |
|                                       |              |                            | NORMAL       | ALARM 1                                                                                    | ALARM 2                                        |
|                                       |              | ALARM 2                    | STOP ALARM 2 | GO TO ALARM 1                                                                              | NO CHANGE                                      |
|                                       |              |                            | NORMAL       | ALARM 1                                                                                    | ALARM 2                                        |
|                                       |              |                            | NORMAL       | ALARM 1                                                                                    | ALARM 2                                        |

FIG. 21A

2230

2238 2239

2242 SEDATION

2244

2240

2241

2243

2246

2248

2250

2255

2236

2234

2233

2232

2231

2230

2229

2228

2227

2226

2225

2224

2223

2222

2221

2220

2219

2218

2217

2216

2215

2214

2213

2212

2211

2210

2209

2208

2207

2206

2205

2204

2203

2202

2201

2200

2199

2198

2197

2196

2195

2194

2193

2192

2191

2190

2189

2188

2187

2186

2185

2184

2183

2182

2181

2180

2179

2178

2177

2176

2175

2174

2173

2172

2171

2170

2169

2168

2167

2166

2165

2164

2163

2162

2161

2160

2159

2158

2157

2156

2155

2154

2153

2152

2151

2150

2149

2148

2147

2146

2145

2144

2143

2142

2141

2140

2139

2138

2137

2136

2135

2134

2133

2132

2131

2130

2129

2128

2127

2126

2125

2124

2123

2122

2121

2120

2119

2118

2117

2116

2115

2114

2113

2112

2111

2110

2109

2108

2107

2106

2105

2104

2103

2102

2101

2100

2099

2098

2097

2096

2095

2094

2093

2092

2091

2090

2089

2088

2087

2086

2085

2084

2083

2082

2081

2080

2079

2078

2077

2076

2075

2074

2073

2072

2071

2070

2069

2068

2067

2066

2065

2064

2063

2062

2061

2060

2059

2058

2057

2056

2055

2054

2053

2052

2051

2050

2049

2048

2047

2046

2045

2044

2043

2042

2041

2040

2039

2038

2037

2036

2035

2034

2033

2032

2031

2030

2029

2028

2027

2026

2025

2024

2023

2022

2021

2020

2019

2018

2017

2016

2015

2014

2013

2012

2011

2010

2009

2008

2007

2006

2005

2004

2003

2002

2001

2000

1999

1998

1997

1996

1995

1994

1993

1992

1991

1990

1989

1988

1987

1986

1985

1984

1983

1982

1981

1980

1979

1978

1977

1976

1975

1974

1973

1972

1971

1970

1969

1968

1967

1966

1965

1964

1963

1962

1961

1960

1959

1958

1957

1956

1955

1954

1953

1952

1951

1950

1949

1948

1947

1946

1945

1944

1943

1942

1941

1940

1939

1938

1937

1936

1935

1934

1933

1932

1931

1930

1929

1928

1927

1926

1925

1924

1923

1922

1921

1920

1919

1918

1917

1916

1915

1914

1913

1912

1911

1910

1909

1908

1907

1906

1905

1904

1903

1902

1901

1900

1899

1898

1897

1896

1895

1894

1893

1892

1891

1890

1889

1888

1887

1886

1885

1884

1883

1882

1881

1880

1879

1878

1877

1876

1875

1874

1873

1872

1871

1870

1869

1868

1867

1866

1865

1864

1863

1862

1861

1860

1859

1858

1857

1856

1855

1854

1853

1852

1851

1850

1849

1848

1847

1846

1845

1844

1843

1842

1841

1840

1839

1838

1837

1836

1835

1834

1833

1832

1831

1830

1829

1828

1827

1826

1825

1824

1823

1822

1821

1820

1819

1818

1817

1816

1815

1814

1813

1812

1811

1810

1809

1808

1807

1806

1805

1804

1803

1802

1801

1800

1799

1798

1797

1796

1795

1794

1793

1792

1791

1790

1789

1788

1787

1786

1785

1784

1783

1782

1781

1780

1779

1778

1777

1776

1775

1774

1773

1772

1771

1770

1769

1768

1767

1766

1765

1764

1763

1762

1761

1760

1759

1758

1757

1756

1755

1754

1753

1752

1751

1750

1749

1748

1747

1746

1745

1744

1743

1742

1741

1740

1739

1738

1737

1736

1735

1734

1733

1732

1731

1730

1729

1728

1727

1726

1725

1724

1723

1722

1721

1720

1719

1718

1717

1716

1715

1714

1713

1712

1711

1710

1709

1708

1707

1706

1705

1704

1703

1702

1701

1700

1699

1698

1697

1696

1695

1694

1693

1692

1691

1690

1689

1688

1687

1686

1685

1684

1683

1682

1681

1680

1679

1678

1677

1676

1675

1674

1673

1672

1671

1670

1669

1668

1667

1666

1665

1664

1663

1662

1661

1660

1659

1658

1657

1656

1655

1654

1653

1652

1651

1650

1649

1648

1647

1646

1645

1644

1643

1642

1641

1640

1639

1638

1637

1636

1635

1634

1633

1632

1631

1630

1629

1628

1627

1626

1625

1624

1623

1622

1621

1620

1619

1618

1617

1616

1615

1614

1613

1612

1611

1610

1609

1608

1607

1606

1605

1604

1603

1602

1601

1600

1599

1598

1597

1596

1595

1594

1593

1592

1591

1590

1589

1588

1587

1586

1585

1584

1583

1582

1581

1580

1579

1578

1577

1576

1575

1574

1573

1572

1571

1570

1569

1568

1567

1566

1565

1564

1563

1562

1561

1560

1559

1558

1557

1556

1555

1554

1553

1552

1551

1550

1549

1548

1547

1546

1545

1544

1543

1542

1541

1540

1539

1538

1537

1536

1535

1534

1533

1532

1531

1530

1529

1528

1527

1526

1525

1524

1523

1522

1521

1520

1519

1518

1517

1516

1515

1514

1513

1512

1511

1510

1509

1508

1507

1506

1505

1504

1503

1502

1501

1500

1499

1498

1497

1496

1495

1494

1493

1492

1491

1490

1489

1488

1487

1486

1485

1484

1483

1482

1481

1480

1479

1478

1477

1476

1475

1474

1473

1472

1471

1470

1469

1468

1467

1466

1465

1464

1463

1462

1461

1460

1459

1458

1457

1456

1455

1454

1453

1452

1451

1450

1449

1448

1447

1446

1445

1444

1443

1442

1441

1440

1439

1438

1437

1436

1435

1434

1433

1432

1431

1430

1429

1428

1427

1426

1425

1424

1423

1422

1421

1420

1419

1418

1417

1416

1415

1414

1413

1412

1411

1410

1409

1408

1407

1406

1405

1404

1403

1402

1401

1400

1399

1398

1397

1396

1395

1394

1393

1392

1391

1390

1389

1388

1387

1386

1385

1384

1383

1382

1381

1380

1379

1378

1377

1376

1375

1374

1373

1372

1371

1370

1369

1368

1367

1366

1365

1364

1363

1362

1361

1360

1359

1358

1357

1356

1355

1354

1353

1352

1351

1350

1349

1348

1347

1346

1345

1344

1343

1342

1341

1340

1339

1338

1337

1336

1335

1334

1333

1332

1331

1330

1329

1328

1327

1326

1325

1324

1323

1322

1321

1320

1319

1318

1317

1316

1315

1314

1313

1312

1311

1310

1309

1308

1307

1306

1305

1304

1303

1302

1301

1300

1299

1298

1297

1296

1295

1294

1293

1292

1291

1290

1289

1288

1287

1286

1285

1284

1283

1282

1281

1280

1279

1278

1277

1276

1275

1274

1273

1272

1271

1270

1269

1268

1267

1266

1265

1264

1263

1262

1261

1260

1259

1258

1257

1256

1255

1254

1253

1252

1251

1250

1249

1248

1247

1246

1245

1244

1243

1242

1241

1240

1239

1238

1237

1236

1235

1234

1233

1232

1231

1230

1229

1228

1227

1226

1225

1224

1223

1222

1221

1220

1219

1218

1217

1216

1215

1214

1213

1212

1211

1210

1209

1208

1207

1206

1205

1204

1203

1202

1201

1200

1199

1198

1197

1196

1195

1194

1193

1192

1191

1190

1189

1188

1187

1186

1185

1184

1183

1182

1181

1180

1179

1178

1177

1176

1175

1174

1173

1172

1171

1170

1169

1168

1167

1166

1165

1164

1163

1162

1161

1160

1159

1158

1157

1156

1155

1154

1153

1152

1151

1150

1149

1148

1147

1146

1145

1144

1143

1142

1141

1140

1139

1138

1137

1136

1135

1134

1133

1132

1131

1130

1129

1128

1127

1126

1125

1124

1123

1122

1121

1120

1119

1118

1117

1116

1115

1114

1113

1112

1111

1110

1109

1108

1107

1106

1105

1104

1103

1102

1101

1100

1099

1098

1097

1096

1095

1094

1093

1092

1091

1090

1089

1088

1087

1086

1085

1084

1083

1082

1081

1080

1079

1078

1077

1076

1075

1074

1073

1072

1071

1070

1069

1068

1067

1066

1065

1064

1063

1062

1061

1060

1059

1058

1057

1056

1055

1054

1053

1052

1051

1050

1049

1048

1047

1046

1045

1044

1043

1042

1041

1040

1039

1038

1037

1036

1035

1034

1033

1032

1031

1030

1029

1028

1027

1026

1025

1024

1023

1022

1021

1020

10

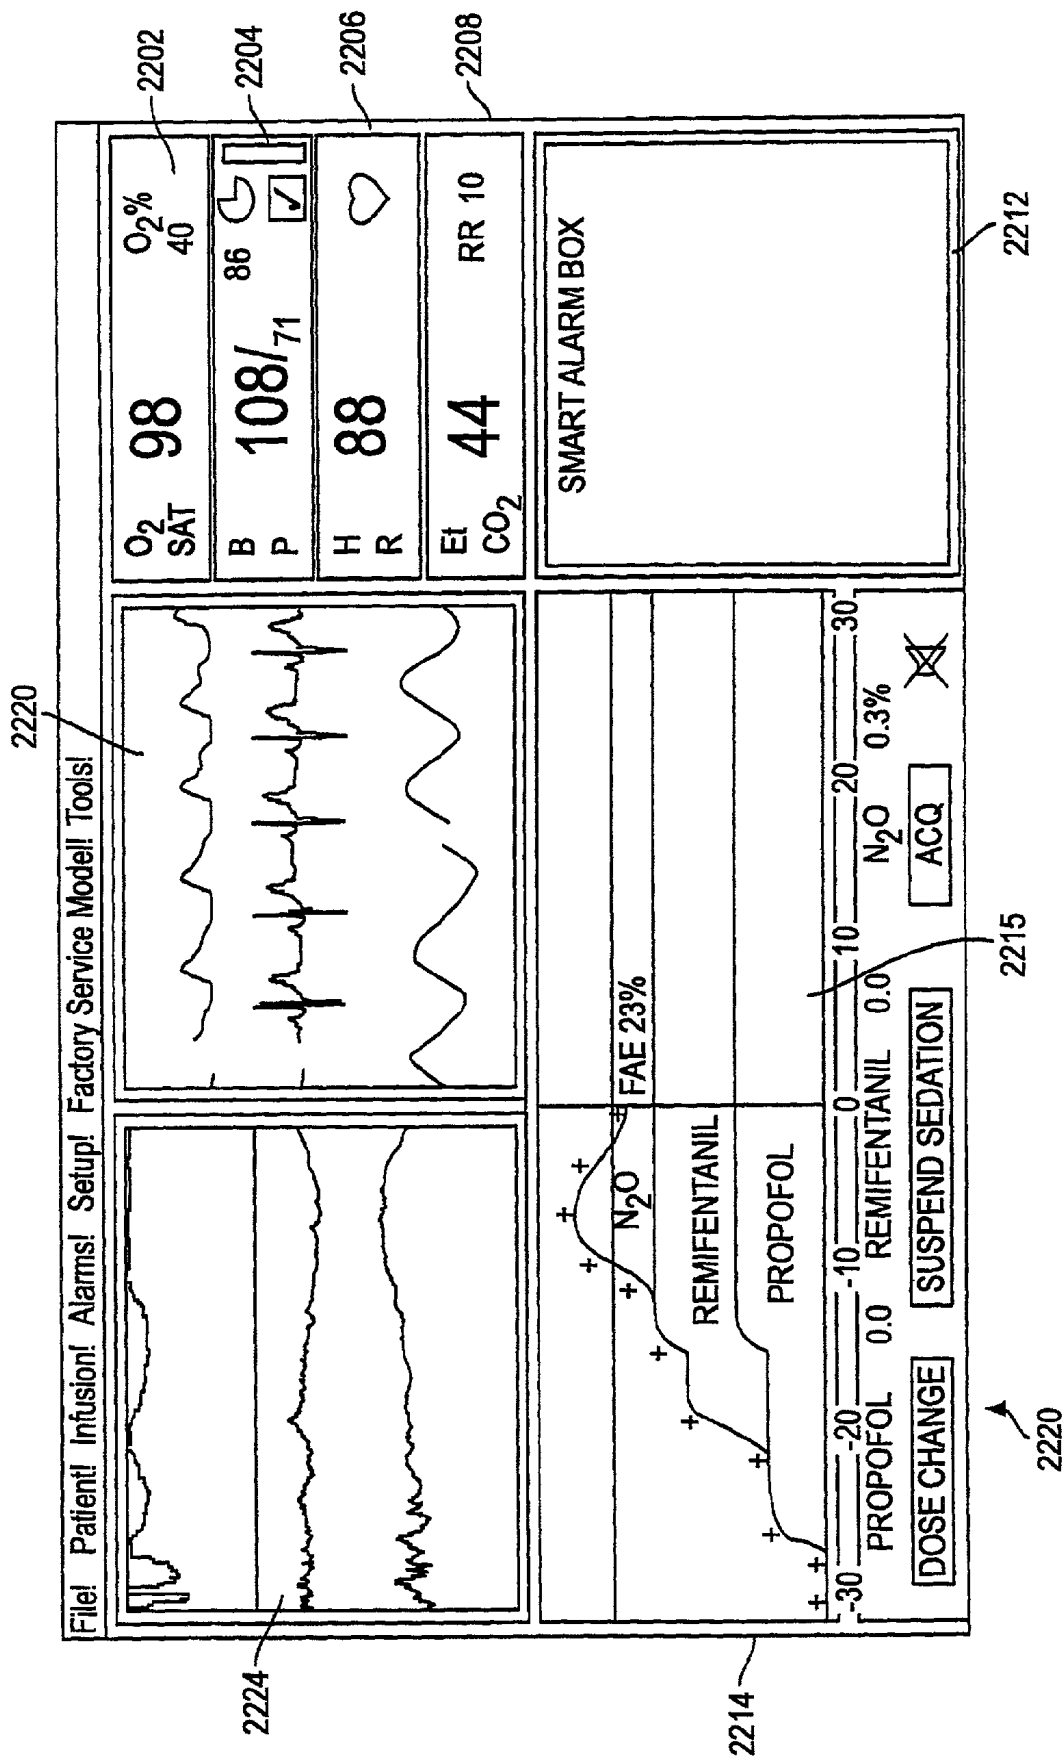


FIG. 22A

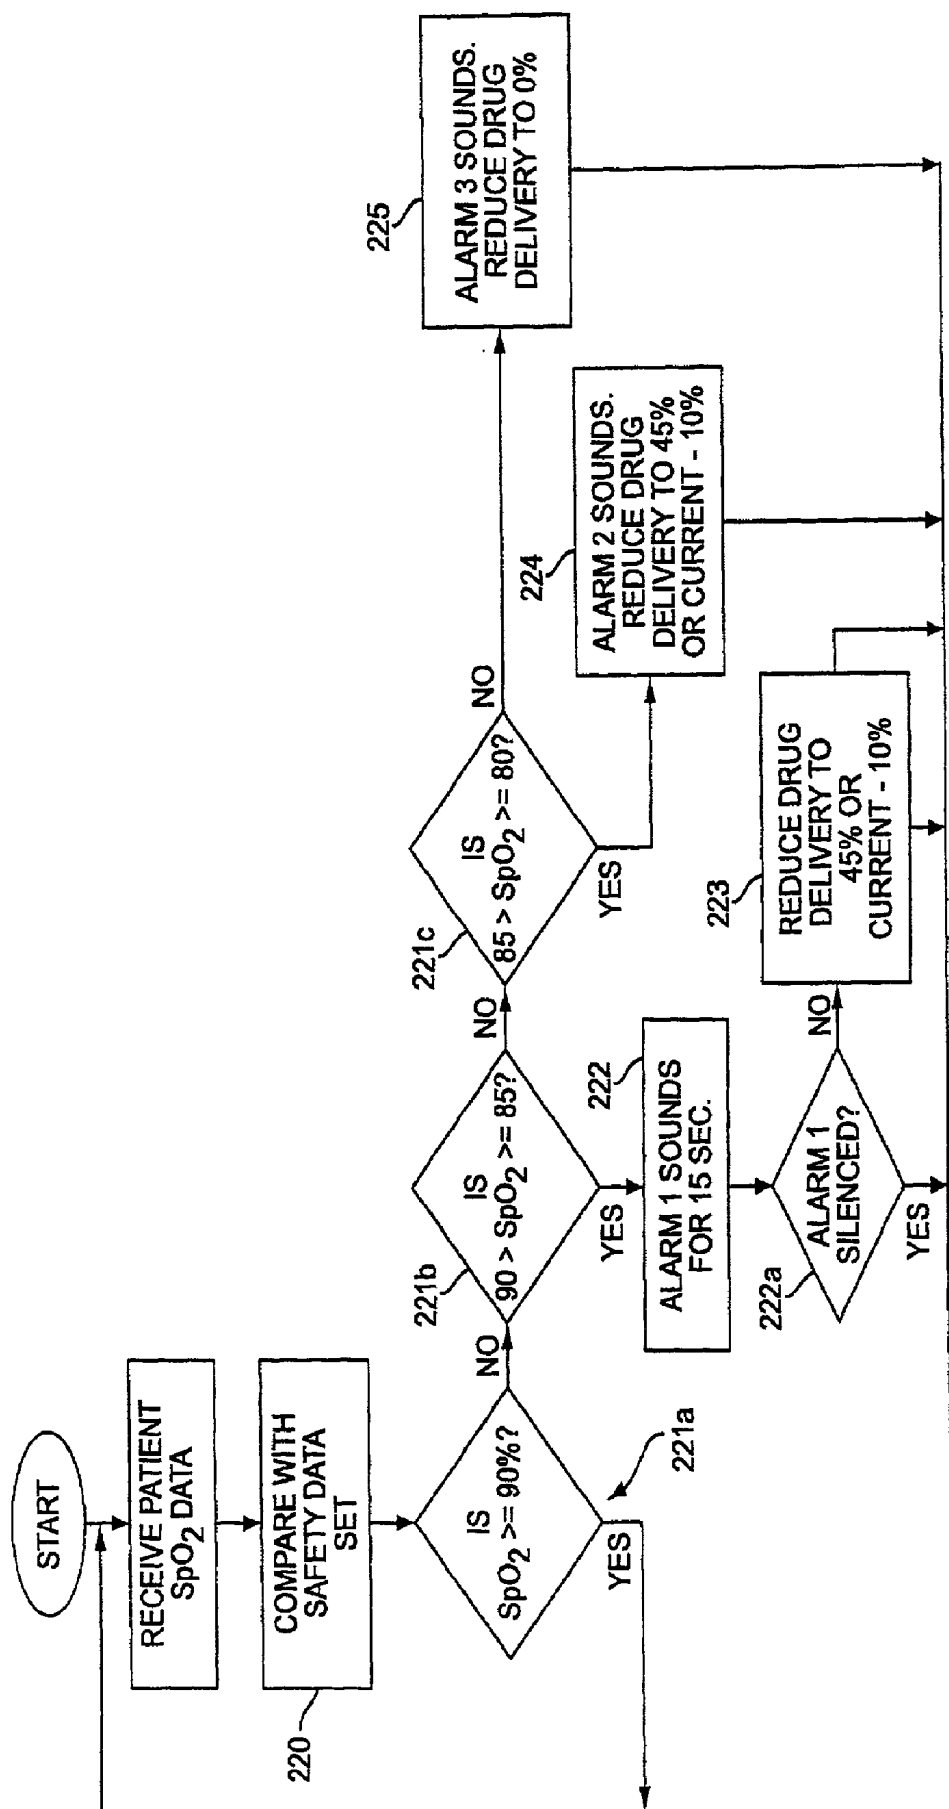


FIG 23

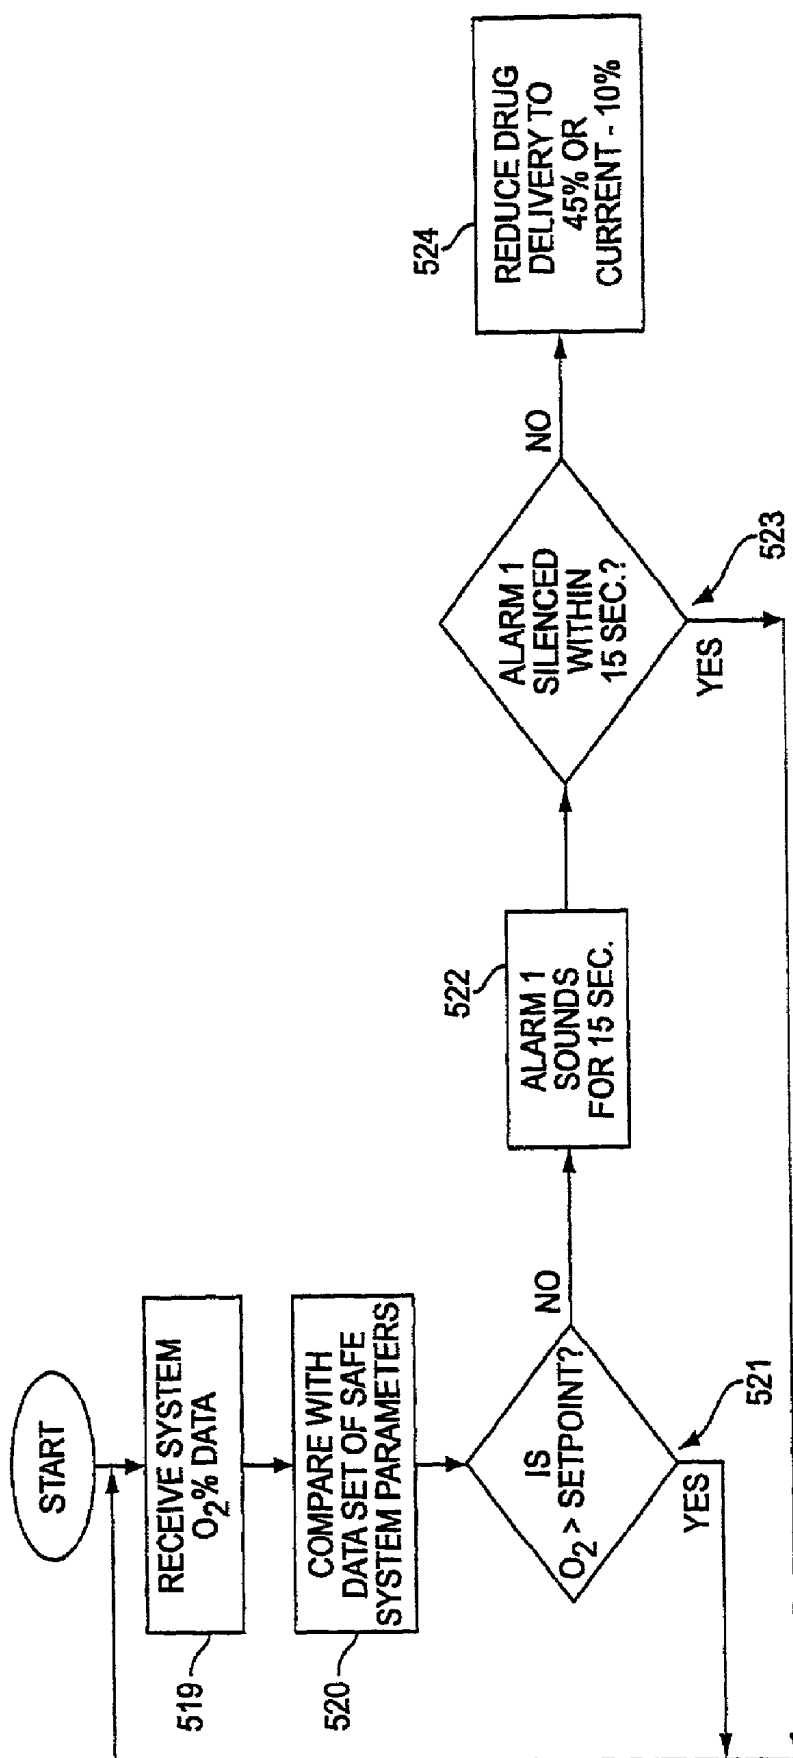


FIG 23A

# APPARATUS AND METHOD FOR PROVIDING A CONSCIOUS PATIENT RELIEF FROM PAIN AND ANXIETY ASSOCIATED WITH MEDICAL OR SURGICAL PROCEDURES

## BACKGROUND OF THE INVENTION

[0001] This invention is directed to providing a conscious patient who is undergoing a painful, uncomfortable or otherwise frightening (anxiety-inspiring) medical or surgical procedure, or who is suffering from post-procedural or other pain or discomfort, with safe, effective and cost-effective relief from such pain and/or anxiety. Focuses of the invention include, but are not limited to, enabling the provision of sedation (inducement of a state of calm), analgesia (insensitivity to pain) and/or amnesia to a conscious patient (sometimes referred to collectively as "conscious sedation") by a nonanesthetist practitioner, i.e., a physician or other clinician who is not an anesthesiologist (M.D.A.) or certified nurse anesthetist (C.R.N.A.), in a manner that is safe, effective and cost-effective; the provision of same to patients in ambulatory settings such as hospital laboratories, ambulatory surgical centers, and physician's offices; and the provision of patient post-operative or other pain relief in remote medical care locations or in home care environments. To those ends, the invention mechanically integrates through physical proximity and incorporation into an overall structural system and electronically integrates through conservative, decision-making software management, the delivery of one or more sedative, analgesic or amnestic drugs to the patient with the electronic monitoring of one or more patient physiological conditions.

[0002] In traditional operating rooms, anesthesiologists provide patients relief from pain, fear and physiological stress by providing general anesthesia. "Anesthesia" is typically used (and is so used herein) interchangeably with the state of "unconsciousness." Over a billion painful and anxiety-inspiring medical and surgical procedures, however, are performed worldwide each year without anesthesia. Thus, outside the practice of anesthesiology there are currently a large number of patients who, while conscious, undergo medical or surgical procedures that produce considerable pain, profound anxiety, and/or physiological stress. Such medical or surgical procedures are often performed by procedural physicians (nonanesthetists) in hospital laboratories, in physicians' offices, and in ambulatory surgical centers. For example, physician specialists perform painful procedures on conscious patients such as pacemaker placement, colonoscopies, various radiological procedures, microlaparoscopy, fracture reduction, wound dressing changes in burn units, and central and arterial catheter insertion in pediatric patients, in hospital laboratory settings. Primary care physicians perform such procedures as flexible sigmoidoscopies, laceration repairs, bone marrow biopsies and other procedures in physicians' offices. Many surgical specialists perform painful procedures such as anterior segment repairs by ophthalmologists, plastic procedures by cosmetic surgeons, foreign body removal, transurethral procedures, incisions of neck and axilla nodes, and breast biopsies in their offices or in ambulatory surgical centers. The needs of patients for safe and effective pain and anxiety relief during and after such procedures are currently unmet.

[0003] Conscious sedation techniques currently available for use by procedural physicians (nonanesthetists) during

medical or surgical procedures such as those described above include sedatives and opioids given orally, rectally or intramuscularly; sedatives and analgesics administered intravenously; and local anesthetics. Often, however, such techniques are less than satisfactory.

[0004] In the case of oral, rectal or intra-muscular administration of sedatives and opioids by procedural physicians during the provision of conscious sedation, there are currently no effective means available to assure that the effects of those drugs can be readily controlled to meet patient need. This is due in part to the variable interval between administration and the onset and dissipation of drug effect. Unreliable sedation and analgesia can result because of mismatches between the dosage administered and the patient's needs which can vary depending on the condition of the patient and the type of procedure performed. Such administration of sedation can also produce an unconscious patient at risk for developing airway obstruction, emesis with pulmonary aspiration or cardiovascular instability. To attempt to avoid these complications, procedural physicians often administer sedatives and analgesics sparingly. This may reduce the risk of major complications, but may also mean that few patients receive adequate relief from pain and/or anxiety during medical and surgical procedures outside the practice of anesthesiology.

[0005] The use of intravenous administration of sedatives and analgesics to conscious patients by procedural physicians in settings such as hospital laboratories, physicians' offices and other ambulatory settings is also less than satisfactory. With respect to intravenous bolus administration, plasma concentrations vary considerably when drugs are injected directly into the blood stream. This can result in initially excessive (potentially toxic) levels followed by sub-therapeutic concentrations. Although intravenously administered drugs can be titrated to the patient's need, doing so safely and effectively usually requires the full-time attention of a trained care giver, e.g., an anesthesiologist. Costs and scheduling difficulties among other things typically preclude this option.

[0006] Due to the difficulties described above involving administration of sedatives and opioids, many procedural physicians rely on local anesthetics for pain relief. However, local anesthetics alone usually provide inadequate analgesia (insensitivity to pain) for most medical and surgical procedures and the injections themselves are often relatively painful.

[0007] In short, current methods commonly available to procedural physicians for providing effective pain relief to conscious patients outside the practice of anesthesiology typically fall short of the objective. Moreover, there are currently no clear standards of practice for nonanesthetists to guide the relief of pain and anxiety for conscious patients. There is not adequate training for such practitioners in the diagnosis and treatment of complications that may arise or result from the provision of sedation and analgesia to conscious patients. Procedures or mechanisms for ongoing quality management of the care of conscious patients undergoing painful and anxiety-inspiring medical or surgical procedures and the devices and methods employed in that care are inadequate.

[0008] An additional focus of this invention is the electronic monitoring of a conscious patient's physiological

condition during drug delivery, and the electronic management of drug delivery by conservative decision-making software that integrates and correlates drug delivery with electronic feedback values representing the patient's physiological condition, thereby ensuring safe, cost-effective, optimized care. Significantly, in many cases involving conscious sedation, the patient's physiological condition is inadequately monitored or not electronically monitored at all during drug delivery and recovery therefrom. That is, there is often no electronic monitoring of basic patient vital signs such as blood pressure, blood oxygen saturation (oximetry) nor of carbon dioxide levels in a patient's inhaled and exhaled gases (capnometry). For example, patients undergoing painful procedures in dentists' offices may receive nitrous oxide ( $\text{N}_2\text{O}$ ) gas to relieve pain, but that drug delivery is often not accompanied by electronic monitoring of a patient's physiological condition, and currently there are no devices available to nonanesthetists which safely and effectively integrate electronic patient monitoring with such drug delivery mechanisms.

[0009] In other circumstances involving the provision of conscious sedation and analgesia by the procedural physician, such as a cardiologist's performing a catheterization procedure in a hospital laboratory, electronic patient monitors are sometimes used, but again, there are no devices currently available to the nonanesthetist which safely and effectively integrate both mechanically (through close, physical proximity and incorporation into a structural system), and electronically (through conservative software management), electronic patient monitors with mechanisms for drug delivery.

[0010] One aspect of the invention of this application is directed to the simplification of drug delivery machines for relieving patient pain and anxiety by eliminating features of those machines that complicate the provision of patient pain and anxiety relief, and by including those features that enable nonanesthetists to provide safe, cost-effective, optimized conscious sedation and analgesia. More specifically, current anesthesia machines used by anesthesiologists to provide general anesthesia and a form of conscious sedation administered by the anesthesiologist known as "monitored anesthesia care" (MAC) include various complex features such as oxygen ( $\text{O}_2$ ) flush valves which are capable of providing large amounts of oxygen to the patient at excessive pressures, and carbon dioxide ( $\text{CO}_2$ ) absorbent material which absorbs  $\text{CO}_2$  from a patient's exhaled gases. In addition, anesthesia machines typically deliver halogenated anesthetic gases which can trigger malignant hyperthermia. Malignant hyperthermia is a rare, but highly critical condition requiring the advanced training and skills of an anesthesiologist for rapid diagnosis and therapy. The airway circuit in current anesthesia machines is circular in nature and self-contained in that the patient inhales an oxygen/anesthetic gas mixture, exhales that mixture which is then passed through  $\text{CO}_2$  absorbent material, re-inhales the filtered gas mixture (supplemented by additional anesthetic and oxygen), and repeats the process.

[0011] These aspects of anesthesia machines, among others, carry attendant risks for the patient such that anesthesia machines require operation by a professional trained through a multi-year apprenticeship (e.g., an anesthesiologist or C.R.N.A.) in detecting and correcting failure modes in the technology. For example, an oxygen flush valve can cause

oxygen to enter a patient's stomach thereby causing vomiting; and carbon dioxide absorbent material can fail in which case the patient could receive too much carbon dioxide if the failure was not promptly detected and corrected. Moreover, the use of the self-contained, circular airway circuit could result in a circumstance whereby if the supply of  $\text{O}_2$  suddenly ceased, a patient would only be breathing the finite supply of oxygen with no provision for administration of additional requirements for  $\text{O}_2$  or atmospheric air. Such features, among others, make anesthesia machines unusable by nonanesthetists. Therefore, a focal point of this aspect of the invention is the simplification of a drug delivery apparatus by selecting and incorporating the appropriate features to facilitate the rendition of safe and effective conscious sedation by nonanesthetists.

[0012] Certain aspects of this invention also focus on ensuring maintenance of patient consciousness to prevent airway difficulties, including monitoring the level of patient consciousness during the delivery of one or more sedative, analgesic and/or amnestic drugs to a conscious, non-intubated, spontaneously-ventilating patient to prevent airway difficulties. For patients not intubated on a ventilator, monitoring the level of patient consciousness is important to provide information about the likelihood of depressed airway reflexes and respiratory drive to breathe, the ability to maintain a patent airway, and the likelihood of cardiovascular instability. Despite the importance of monitoring and maintaining adequate levels of consciousness in certain medical settings, there is no currently available device for ensuring maintenance of patient consciousness by integrating mechanically and electronically such monitoring of a patient's level of consciousness with a drug delivery system. The invention of this application is directed to this unmet need, as well.

[0013] This invention is also directed to providing conscious patients relief from pain and/or anxiety in a manner that is cost-effective and time efficient. Current solutions for relieving patient pain and anxiety by drug delivery and electronic monitoring of a patient's physiological condition are expensive and require a great deal of time to set-up and take down. Also, the current requirement or desire for the presence of an anesthesiologist during some medical or surgical procedures increases costs, especially if that desire requires in-patient care as opposed to care in an ambulatory setting. To the extent medical procedures are performed on conscious patients without adequate sedation and analgesia due to the current unavailability of appropriate methods and devices for providing such care (e.g., wound dressing changes in burn wards), such procedures may need to be conducted on numerous occasions, but over short periods of time (due to a patient's inability to tolerate the level of pain), as opposed to conducting a fewer number of more definitive procedures. The requirement of multiple sessions of care also typically involves increased costs. This invention addresses such cost-effectiveness concerns and provides solutions to problems such as those described.

[0014] The invention is further directed to the provision of relief from post-operative or other post-procedural pain and discomfort in remote medical care locations and home care type settings. Current devices may permit certain patients in, for example, a home care type setting, to provide themselves with an increased dosage of analgesic through the use of a patient-controlled drug delivery device, e.g., a device that

permits a patient to press a button or toggle a switch and receive more analgesic (often intravenously or transdermally). This practice is sometimes called "PCA" or patient-controlled analgesia. Known commercially available PCA-type devices do not electronically integrate and conservatively manage delivery of analgesics in accord with the electronic monitoring of a patient's physiological condition. This invention focuses on this unmet need, as well.

[0015] An additional aspect of this invention is directed to the integration of a billing/information system for use with an apparatus providing sedation, analgesia and/or amnesia to conscious patients in physician's offices, hospital laboratory or other ambulatory settings or remote medical care locations. Current techniques for automated billing and invoice generating provide inadequate and inefficient methods for tracking recurring revenues derived from repeated use of medical devices such as the apparatus of this invention.

[0016] Other focuses of the invention are apparent from the below detailed description of preferred embodiments.

#### DESCRIPTION OF RELATED ART

[0017] Known machines or methods administered by the nonanesthetist for providing conscious, non-intubated, spontaneously-ventilating patients with sedation and analgesia are unreliable, not cost-effective or are otherwise unsatisfactory. No commercially available devices reliably provide such patients with safe and cost-effective sedation, analgesia and amnesia to conscious patients by integrating and correlating the delivery of sedative, analgesic and/or amnestic drugs with electronic monitoring of a patient's physiological condition. Available drug delivery systems do not incorporate a safety set of defined data parameters so as to permit drug delivery to be conservatively managed electronically in correlation with the patient's physiological conditions, including vital signs, to effectuate safe, cost-effective and optimized drug delivery to a patient. Available drug delivery systems do not incorporate alarm alerts that safely and reliably free the nonanesthetist practitioner from continued concern of drug delivery effects and dangers to permit the nonanesthetist to focus on the intended medical examination and procedure. Moreover, there are no known patient-controlled analgesia devices that mechanically and electronically integrate and correlate (through conservative software management) patient requests for adjustments to drug dosage and electronic monitoring of patient physiological conditions.

[0018] Known techniques have focused on the delivery of sedation and analgesia to conscious patients with inadequate or no electronic monitoring of patient physiological conditions, including vital signs, and no electronic integration or correlation of such patient monitoring with drug delivery. Other techniques have focused on the provision of anesthesia to unconscious patients with the requirement of an anesthesiologist to operate a complicated, failure-intensive anesthesia machine.

[0019] Presently known nitrous oxide delivery systems such as those manufactured by Matrux Medical, Inc., Accutron, Inc., and others are used primarily in dental offices for providing conscious sedation only. Such devices contain sources of nitrous oxide and oxygen, a gas mixing device and system monitors, but no mechanical or electrical integration of patient physiological condition monitors with

drug delivery mechanisms. Similarly, other known drug delivery systems (e.g., intravenous infusion or intramuscular delivery mechanisms) for providing sedatives and analgesics to conscious patients used, for example, in hospital laboratories, do not include mechanical or electronic integration of patient physiological condition monitors with drug delivery mechanisms.

[0020] Anesthesia machines used by anesthesiologists to provide general anesthesia or MAC, such as, by way of example, the NARKOMED line of machines manufactured by North American Drager and EXCEL SE ANESTHESIA SYSTEMS manufactured by Ohmeda Inc., mechanically integrate electronic patient monitors in physical proximity to drug delivery mechanisms. These machines, however, employ features such as O<sub>2</sub> flush valves, malignant hyperthermia triggering agents, CO<sub>2</sub> absorbent material, as well as circular airway circuits, among others, thereby requiring operation by an M.D.A. (or C.R.N.A.) to avoid the occurrence of life-threatening incidents. These devices do not provide for the electronic integration or management of drug delivery in correlation with the monitoring of a patient's physiological condition, much less such electronic management through conservative, decision-making software or logic incorporating established safe data-defining parameters.

[0021] U.S. Pat. No. 2,888,922 (Bellville) discloses a servo-controlled drug delivery device for automatic and continuous maintenance of the level of unconsciousness in a patient based on voltages representative of the patient's cortical activity obtained by means of an electroencephalograph (EEG). The device continuously and automatically increases or decreases in robotic fashion the flow of anesthetic gas (or I.V. infusion) in response to selected frequencies of brain potential to maintain a constant level of unconsciousness.

[0022] U.S. Pat. No. 4,681,121 (Kobal) discloses a device for measuring a patient's sensitivity to pain during the provision of anesthesia, by applying a continuous, painful stimulus to the nasal mucosa and regulating the level of anesthesia in response to EEG signals indicating the patient's response to the nasal pain stimulus, with the goal of maintaining a sufficient level of unconsciousness.

[0023] Among other things, none of the above-described known devices manages drug delivery to conscious patients employing conservative decision-making software or logic which correlates the drug delivery to electronic patient feedback signals and an established set of safety data parameters.

#### SUMMARY OF THE INVENTION

[0024] The invention provides apparatuses and methods to safely and effectively deliver a sedative, analgesic, amnestic or other pharmaceutical agent (drug) to a conscious, non-intubated, spontaneously-ventilating patient. The invention is directed to apparatuses and methods for alleviating a patient's pain and anxiety before and/or during a medical or surgical procedure and for alleviating a patient's post-operative or other post-procedural pain or discomfort while simultaneously enabling a physician to safely control or manage such pain and/or anxiety. The costs and time loss often associated with traditional operating room settings or other requirements or desires for the presence of anesthetists may thus be avoided.

[0025] A care system in accordance with the invention includes at least one patient health monitor which monitors a patient's physiological condition integrated with a drug delivery controller supplying an analgesic or other drug to the patient. A programmable, microprocessor-based electronic controller compares the electronic feedback signals generated from the patient health monitor and representing the patient's actual physiological condition with a stored safety data set reflecting safe and undesirable parameters of at least one patient physiological condition and manages the application or delivery of the drug to the patient in accord with that comparison. In a preferred embodiment, the management of drug delivery is effected by the electronic controller via conservative, decision-making software accessing the stored safety data set.

[0026] In another aspect the invention also includes at least one system state monitor which monitors at least one operating condition of the care system, the system state monitor being integrated with a drug delivery controller supplying drugs to the patient. In this aspect, an electronic controller receives instruction signals generated from the system monitor and conservatively controls (i.e., curtails or ceases) drug delivery in response thereto. In a preferred embodiment, this is accomplished through software control of the electronic controller whereby the software accesses a stored data set reflecting safe and undesirable parameters of at least one operating condition of the care system, effects a comparison of the signal generated by the system state monitor with the stored data set of parameters and controls drug delivery in accord with same, curtailing or ceasing drug delivery if the monitored system state is outside of a safe range. The electronic controller may also activate attention-commanding devices such as visual or audible alarms in response to the signal generated by the system state monitor to alert the physician to any abnormal or unsafe operating state of the care system apparatus.

[0027] The invention is further directed to an apparatus which includes a drug delivery controller, which delivers drugs to the patient, electronically integrated with an automated consciousness monitoring system which ensures the consciousness of the patient and generates signal values reflecting patient consciousness. An electronic controller is also included which is interconnected to the drug delivery controller and the automated consciousness monitor and manages the delivery of the drugs in accord with the signal values reflecting patient consciousness.

[0028] In another aspect, the invention includes one or more patient health monitors such as a pulse oximeter or capnometer and an automated consciousness monitoring system, wherein the patient health monitors and consciousness monitoring system are integrated with a drug delivery controller supplying an analgesic or other drug to the patient. A microprocessor-based electronic controller compares electronic feedback signals representing the patient's actual physiological condition including level of consciousness, with a stored safety data set of parameters reflecting patient physiological conditions (including consciousness level), and manages the delivery of the drug in accord with that comparison while ensuring the patient's consciousness. In additional aspects of the invention the automated consciousness monitoring system includes a patient stimulus or query device and a patient initiate response device.

[0029] The invention also provides apparatuses and methods for alleviating post-operative or other post-procedural pain or discomfort in a home care-type setting or remote medical care location. Here the care system includes at least one patient health monitor integrated with patient-controlled drug delivery. An electronic controller manages the patient-controlled drug delivery in accord with electronic feedback signals from the patient health monitors. In a preferred embodiment the electronic controller is responsive to software effecting conservative management of drug delivery in accord with a stored safety data set.

#### DESCRIPTION OF THE DRAWINGS

[0030] Other objects and many of the intended advantages of the invention will be readily appreciated as they become better understood by reference to the following detailed description of preferred embodiments of the invention considered in connection with the accompanying drawings, wherein:

[0031] **FIG. 1** is a perspective view of a preferred embodiment of a care system apparatus constructed in accordance with this invention, depicting the provision of sedation, analgesia and/or amnesia to a conscious patient by a nonanesthetist.

[0032] **FIG. 2** is a perspective view of a preferred embodiment of a care system apparatus constructed in accordance with this invention depicting user interface and patient interface devices.

[0033] **FIGS. 3A and 3B** are side-elevational views of a preferred embodiment of an apparatus constructed in accordance with this invention.

[0034] **FIG. 4A** is a block diagram overview of the invention.

[0035] **FIG. 4B** is an overview data-flow diagram depicting the drug delivery management aspect of the invention.

[0036] **FIG. 5** depicts a preferred embodiment of the invention.

[0037] **FIG. 6** depicts a preferred embodiment of a drug delivery system in accordance with the invention.

[0038] **FIGS. 7A-7C** depict the details of a preferred embodiment of the drug source system in accordance with the invention.

[0039] **FIG. 8** depicts a preferred embodiment of an electronic mixer system in accordance with the invention.

[0040] **FIG. 9A** depicts one embodiment of a manifold system in accordance with the invention.

[0041] **FIG. 9B** depicts a second embodiment of a manifold system in accordance with the invention.

[0042] **FIG. 10A** depicts a preferred embodiment of a manual bypass system in accordance with the invention.

[0043] **FIG. 10B** depicts a preferred embodiment of a scavenger system in accordance with the invention.

[0044] **FIG. 11** depicts a preferred embodiment of a patient interface system in accordance with the invention.

[0045] **FIGS. 12A and 12B** are a front perspective view and a side-elevational view, respectively, of a preferred embodiment of hand cradle device constructed in accordance with the invention.

[0046] **FIGS. 13A and 13B** are rear perspective views of a preferred embodiment of hand cradle device constructed in accordance with the invention.

[0047] **FIGS. 14A and 14B** are, respectively, a front perspective view of an alternative embodiment of a hand cradle device constructed in accordance with this invention and a top plan view of a patient drug dosage request device in accordance with the invention.

[0048] **FIG. 15** shows a perspective view of a preferred embodiment of the invention, including a hand cradle device and an ear piece combination oximeter/auditory query device.

[0049] **FIG. 16** is a side-elevational view of an ear piece placed within a patient's ear containing a pulse oximetry sensor and an auditory query in accordance with the present invention.

[0050] **FIG. 17** depicts an alternative preferred embodiment of a care system apparatus constructed in accordance with the invention.

[0051] **FIG. 18** depicts a user interface system in accordance with a preferred embodiment of the invention.

[0052] **FIGS. 19A and 19B** depict the various peripheral devices included in a preferred embodiment of the invention.

[0053] **FIG. 20** depicts a preferred embodiment of a patient information/billing system in accordance with the invention.

[0054] **FIG. 21** depicts examples of drug delivery management protocols for 3-stage alarm states reflecting monitored patient parameters in accordance with the invention.

[0055] **FIG. 21A** depicts examples of drug delivery management protocols for 2-stage alarm states reflecting monitored system state parameters in accordance with the invention.

[0056] **FIG. 22** depicts a first embodiment of a user interface screen display in accordance with the invention.

[0057] **FIG. 22A** depicts a second embodiment of a user interface screen display in accordance with the invention.

[0058] **FIG. 23** is a data-flow diagram depicting an example of the steps performed by the drug delivery management software or logic responsive to patient health monitors in accordance with the invention.

[0059] **FIG. 23A** is a data-flow diagram depicting an example of the steps performed by the drug delivery management software or logic responsive to system state monitors in accordance with the invention.

#### DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

[0060] The embodiments illustrated below are not intended to be exhaustive or to limit the invention to the precise forms disclosed. The embodiments are chosen and described in order to explain the principles of the invention

and its applications and uses, and thereby enable others skilled in the art to make and utilize the invention.

[0061] **FIG. 1** shows a care system **10** constructed in accordance with this invention, providing sedative, analgesic and/or amnestic drugs to a conscious, non-intubated, spontaneously-ventilating patient undergoing a medical or surgical procedure by a procedural physician. The system **10** has a generally columnar housing **15** with various storage compartments **16** therein for storage of user and patient interface devices, and a base **17** supported on castor wheels **18**. A drug delivery system **40** delivers a mixture of one or more gaseous sedative, analgesic or amnestic drugs in combination with oxygen ( $O_2$ ) gas to a patient, and includes a one-way airway circuit **20** connected at one end to a face mask **30** and at the other end to a manifold valving system contained within housing **15**. **FIGS. 3A and 3B** show from a side-elevation perspective, airway circuit **20**, face mask **30**, and exhaust hose **32** through which scavenged patient exhaled gases are exhausted to a safe location.

[0062] Referring to **FIG. 2**, lead **50** connects one or more patient interface devices (e.g., **55**) to a microprocessor-based electronic controller or computer (sometimes also referred to herein as main logic board, **MLB**) located within housing **15**. The electronic controller or main logic board may be comprised of combinations of available programmable-type microprocessors and other "chips," memory devices and logic devices on various board(s) such as those manufactured by Texas Instruments (e.g., **XK21E**) and National Semiconductor (e.g., **HKL 72**, among others). Patient interface devices **55** can include one or more patient health monitors that monitor a patient's physiological condition, such as known pulse oximeter, capnometer (not shown), non-invasive blood pressure monitors; EKG, EEG, acoustical monitors (not shown), and others; an automated consciousness monitoring system, including query initiate and response devices in accordance with the invention (described below); and patient drug dosage request devices (also described below). The main logic board electronically manages operation of the apparatus **10** by means of conservative, decision-making software that integrates and correlates patient feedback signals received from the one or more patient health monitors with drug delivery.

[0063] Also shown in **FIGS. 1 and 2** are various user interface devices, including a display device **35** integrated into the top surface of apparatus **10** which displays patient and system parameters and operation status of the apparatus, a printer **37** which prints, for example, a hard copy of patient parameters indicating the patient's physiological condition and the status of various system alarms with time stamps, and a remote control device **45** which permits a physician to interact with apparatus **10**. The various patient and user interface devices are described in more detail below.

[0064] It should be recognized that although certain embodiments of the invention show the analgesic delivery system **40** in a form for delivering one or more sedative, analgesic or amnestic drugs in gaseous form, the invention also specifically includes embodiments where such drugs are delivered intravenously, in nebulized, vaporized or other inhaled form, and/or transdermally such as by using known ion-transfer principles. Drugs that may be delivered by the care system include, but are not limited to, nitrous oxide,

propofol, remifentanyl, dexmedetomidine, epibatidine and sevoflurane. Alternative embodiments are described in more detail herein.

[0065] FIG. 4A is a block diagram overview of a preferred embodiment of the invention. FIG. 4B is an overview data flow diagram depicting the drug delivery management steps performed by the software/logic control of microprocessor controller 14 in a preferred embodiment of the invention. In FIG. 4A, one or more patient health monitors 12a (which may include one or more known patient physiological condition monitors such as pulse oximeters, capnometers, other ventilatory monitors, noninvasive blood pressure monitors, EKG, EEG and others, as well as a patient consciousness monitoring system, are electronically coupled, through suitable A-D converters where appropriate, to electronic controller 14, described above. Patient health monitors 12a generate electronic feedback signals representing actual patient physiological data which are converted to electronic signals and then provided to controller 14. Now referring to FIG. 4B, electronic controller 14, e.g., through appropriate software and/or logic, compares the received electronic patient feedback signals 13b with the safety data set 15b stored in a memory device (such as an EPROM device).

[0066] The stored safety data set 14a (FIG. 4A) contains at least one set of data parameters representing safe and undesirable patient physiological conditions. Based on the comparison of the actual monitored patient physiological data 13b with the safety data set 14a, controller 14 determines whether the monitored patient physiological data is outside of a safe range (FIG. 4B, 16b). If the monitored patient data is outside of a safe range, electronic controller 14 sends instruction commands (signals) to drug delivery controller 2a (FIG. 4A) instructing drug delivery controller 2a to conservatively manage (e.g., reduce or cease) drug delivery (FIG. 4B, 18b). Drug delivery controller 2a may be a standard solenoid valve-type electronic flow controller known to those skilled in the art.

[0067] As is described below, additional embodiments of the invention also contemplate provision of electronic feedback signals representing patient-controlled drug dosage increase or decrease requests to controller 14 and electronic management of drug delivery in consideration of such patient requests vis-a-vis the patient's physiological parameters and/or the state of the care system.

[0068] A block diagram of a preferred embodiment of a care system in accordance with the invention is depicted in FIG. 5. Analgesic delivery system 2 of FIG. 5 delivers a mixture of gaseous sedative, analgesic and/or amnestic drugs (such as nitrous oxide, sevoflurane or nebulized narcotics) and oxygen gas to the patient. Manual bypass circuit 4 (shown in further detail in FIG. 6 and FIG. 10A) is coupled to the manifold system portion of analgesic delivery system 2 and bypasses the source of analgesia enabling the manual control of delivery of atmospheric air to the patient. An auxiliary inlet 6 is provided to analgesic delivery system 2 and enables the provision of in-house supply of gaseous drug or oxygen to the delivery system 2. Scavenger system 8 (shown in detail in FIG. 10B) is coupled to analgesic delivery system 2 and collects exhaled gases from the patient and exhausts them to a safe location through exhaust hose 32 (FIG. 3B).

[0069] Patient interface system 12 includes one or more patient health monitors (these can be known vital sign monitors, such as non-invasive blood pressure monitors, or known pulse oximeters, capnometers, EKGs, etc.); means for monitoring the level of a patient's consciousness; and/or means for the patient to communicate with system 10 (FIG. 1), such as by requesting an increase or decrease in the dosage of drugs. One or more of these patient monitoring and request devices are electronically coupled to and, through A-D converters, provide feedback signals representing the patient's actual physiological condition and drug dosage requests to electronic controller 14. Controller 14 compares this electronic feedback received with data stored in a memory device, said data representing sets of one or more safe and undesirable patient physiological condition parameters (e.g., safe and undesirable O<sub>2</sub> saturation conditions, end tidal CO<sub>2</sub> levels and/or levels of patient consciousness). These sets of parameters are collectively referred to as a safety data set.

[0070] Based on the comparison, controller 14 commands conservative application of drug delivery in accord with said parameters at safe, cost-effective optimized values.

[0071] Still referring to FIG. 5, user interface system 16 (described in more detail in FIGS. 18 and 22) displays electronic signal values stored in or provided to electronic controller 14, such values reflecting the status of one or more of the patient's physiological state, the patient's level of consciousness, and/or the status of various care system parameters. User interface system 16 includes devices that permit the nonanesthetist to interact with the care system via controller 14 (e.g., input patient information, pre-set drug dosages, silence alarms) such as keyboard 230 (FIG. 2) and/or remote control unit 45 (FIG. 1). Patient and care system information is displayed by means of graphical and numeric display devices, e.g., 35 (FIG. 1), LEDs incorporated into housing 15 (FIG. 1) and/or on remote control unit 45.

[0072] External communication devices 18 (also described in FIGS. 19A and 19B) enable the sending and/or receiving of electronic information signals to and from electronic controller 14 and external computers at remote locations or on local networks. Peripheral devices 22 such as door and temperature sensors, among others, communicate electronically with controller 14 to ensure the proper, safe and secure operation of care system 10.

[0073] The above systems overviewed in FIG. 5 are now described in more detail.

[0074] FIG. 6 shows in further detail an overview of a preferred drug delivery system 2 (FIG. 5) which provides a mixture of one or more sedative, analgesic and/or amnestic drugs in gaseous form; oxygen; and atmospheric air to a patient, the provision of each being independently adjustable (manually and via electronic controller 14) by the physician. The drug delivery system is comprised of a drug source system 42, an electronic mixer system 44 and a manifold system 46.

[0075] Drug source system 42 contains sources of one or more gaseous drugs and oxygen and is coupled through pneumatic lines to electronic mixer system 42. Drug source system 42 is also electronically coupled to electronic controller 14, and as is described below, contains sensors

monitoring one or more operating states of drug source system 42 (e.g., whether the drug is flowing). Such monitored system information is converted to appropriate electronic signals and fed back to electronic controller 14 via the electronic coupling.

[0076] Electronic mixer 44 receives the one or more gaseous drugs, O<sub>2</sub> and atmospheric air through the pneumatic lines and electronically mixes same. Electronic mixer 44 is also electronically coupled to electronic controller 14 and also contains sensors that provide electronic feedback signals reflecting system operation parameters of mixer 44 to electronic controller 14. Mixer 44 includes electronic flow controllers with solenoid valves which receive flow control instruction signals from controller 14.

[0077] Manifold system 46 is coupled through pneumatic lines to and receives the one or more gaseous drugs, O<sub>2</sub> and air mixture from electronic mixer 44 and delivers the mixture to the patient via airway circuit 20 (FIG. 1) and face mask 30 (FIG. 1). Manifold system 46 is also electronically coupled to electronic controller 14 and includes sensors that provide electronic feedback signals reflecting manifold-system 46 operation parameters to controller 14. Manifold 46 delivers patient exhaled gases to a scavenging system 48 for exhaust to a safe location via exhaust hose 32 (FIG. 3B).

[0078] Drug source system 42 is shown in further detail in FIGS. 7A-7C. Referring to FIG. 7A, analgesic source system includes drug source system 142 which provides a source of one or more sedative, analgesic and/or amnestic drugs; and an oxygen source system 144 which provides a source of oxygen. In aspects of this invention where the drugs are in gaseous form, the sources of drugs and oxygen provide the gases at low pressure, and can be tanks contained within housing 15 (FIG. 1) such as those shown at numeral 54 in FIG. 2 or an in-house source. The ability to use alternative sources increases the useability of the care system of the invention because the system can function as a source-dependent unit within rooms with access to in-house gas supplies or as a self-contained unit within rooms that do not have in-house gas connections.

[0079] In additional aspects of the invention, drug source system 42 can include one or more of the following: known nebulizers 143 which enable the delivery of aerosolized drugs, such as morphine, meperidine, fentanyl and others; known vaporizers 145 which enable the delivery of halogenated agents, such as sevoflurane; known infusion pump-type drug delivery devices 147 or known transdermal-type drug delivery devices 149 (including ion transfer based devices) to enable the delivery of drugs such as propofol, remifentanyl, and other infusible drugs by continuous or bolus administration.

[0080] FIG. 7B details the oxygen source system and shows an oxygen tank or other source of oxygen 104 and a pneumatic line 109 for delivering oxygen gas to electronic mixer system 44 (FIG. 7A). Filter 106a in oxygen line 109 removes contaminants within the oxygen stream from oxygen source 104. Pressure sensor 106 (which may be of a type known and currently available) in oxygen line 109 monitors the pressure in oxygen source 104 generating a signal reflecting same and thereby indirectly measuring the amount of oxygen remaining. Pressure sensor 106 is electronically coupled to electronic controller 14 and forwards signals reflecting the measure of pressure in the oxygen source to

controller 14. In a preferred embodiment, electronic controller 14 receives the signal from pressure sensor 106 and through software accesses data parameters stored in a memory device. The parameters reflect one or more set-points establishing safe and undesirable operating conditions of O<sub>2</sub> operating pressure. Controller 14 compares the actual O<sub>2</sub> pressure to the stored parameter set point data. If the comparison reveals that the O<sub>2</sub> pressure is outside of an established safe range as established by the stored data, an alarm or other attention-commanding device activates and if same is not manually deactivated, electronic controller 14 instructs the flow of drug delivery to reduce to a pre-set safe amount (or cease). The operation of the software control vis-a-vis system state monitors is described in more detail in connection with FIGS. 21A and 23A.

[0081] The signal obtained from oxygen source pressure sensor 106 can be related to the user via display devices (e.g., 35, FIG. 2) in terms of the time remaining under present use so that the user can ascertain if the procedure can be completed. The user is immediately notified if the pressure falls out of the normal operating conditions by an alarm, display device or other suitable attention-commanding device. Pressure gauges 108 visually display to the user the oxygen source pressure obtained by sensor 106. Pressure regulator 110, which may be of a known solenoid type currently available or other suitable regulator, enables the reduction of pressure in oxygen source 104 to a reasonable operating pressure to provide flow of O<sub>2</sub> to the patient. Check valve 112 (check valves may be of a standard one-way type), in oxygen line 109 downstream of regulator 110 prohibits backward flow of the patient's exhalations and ensures that such back-flow does not damage or contaminate regulator 110 and oxygen source 104. In systems where an in-house oxygen source 105 is used, remote check valve 114 ensures that back-flow from the patient's exhalations does not damage or contaminate in-house oxygen source 105. Pressure relief valve 116 exhausts oxygen to the atmosphere if the pressure in oxygen line 109 exceeds safe operating values pre-programmed into electronic controller 14.

[0082] FIG. 7C details the drug source system and in a preferred embodiment includes a tank or other source of drug 204 and a pneumatic line 209 for delivering gaseous drugs to electronic mixer 44. Filter 206a in drug line 209 removes contaminants within the drug stream from drug source 204. Pressure sensor 206 (which may be of a type known and currently available) in drug line 209 monitors the pressure in drug source 204 generating a signal reflecting same and thereby indirectly measuring the amount of drug. Pressure sensor 206 is electronically coupled to electronic controller 14 and forwards signals reflecting the measure of pressure in the drug source to controller 14. As is described above in connection with oxygen source pressure sensor 106 and in FIGS. 21A and 23A, in a preferred embodiment controller 14 receives the signal from sensor 206 and through software accesses stored data parameters reflecting safe and undesirable operating conditions of drug source pressure and conservatively controls drug delivery in accord with said stored parameters.

[0083] The signal obtained from the drug source pressure sensor 206 can be related to the user via display devices (e.g., 35, FIG. 2) in terms of the time remaining under present use so that the user can ascertain if the procedure can be completed. The user is immediately notified via an alarm,

display device or other suitable attention-commanding device if the pressure falls out of the normal operating conditions. Pressure gauges **208** visually display to the user the drug source pressure obtained by sensor **206**. Pressure regulator **210**, which may be of a known solenoid type currently available, enables the reduction of pressure in drug source **204** to a reasonable operating pressure to provide flow of drug to the patient. Check valve **212** in drug line **209** downstream of regulator **210** prohibits backward flow of the patient's exhalations and ensures that back-flow from the patient's exhalations does not damage or contaminate regulator **210** and drug source **204**. In systems where an in-house drug source **205** is used, remote check valve **214** ensures that back-flow from the patient's exhalations does not damage or contaminate in-house drug source **205**. Pressure relief valve **216** exhausts the drug to the atmosphere if the pressure in drug line **209** exceeds safe operating values pre-programmed into electronic controller **14**.

[0084] To increase safety, the known pin indexed safety system (P.I.S.S.) and/or diameter indexed safety system (D.I.S.S.) may be used for all O<sub>2</sub> source and line fittings where appropriate for tank and/or in-house sources. This ensures, for example, that oxygen source **104** is not mistakenly attached to the drug line **209** and vice versa.

[0085] FIG. 8 details a preferred electronic gas mixer system which electronically mixes gaseous drugs and oxygen so that the precise flow rate of gaseous drug and oxygen is delivered to the patient. The use of the electronic mixer system of this invention increases the operational safety of the apparatus of the invention because, as described below, the volume of drug delivery can be electronically controlled in closed-loop fashion by currently available electronic flow controllers which include solenoid type valves which, in response to command signals from electronic controller **14**, halt or reduce the flow of drugs to the patient in the event of an occurrence of unsafe patient or system conditions. Specifically, pneumatic oxygen line **109** and drug line **209** from analgesic source system **42** deliver gaseous drugs and oxygen to filters **125** and **127** in lines **109** and **209**, respectively, which filter contaminants from lines **109** and **209**. System state monitors, namely, pressure sensors **129**, **131**, monitor the oxygen and gaseous drug line pressures, respectively, and transmit signals reflecting said pressures to electronic controller **14**, which conservatively controls drug delivery in accord with a stored data set containing parameters reflecting one or more safe and undesirable system operation states as described above and in FIGS. 21A and 23A. Also, if any of the pressures fall out of the norm, electronic controller **14** immediately alerts the user, for example, by means of signaling an alarm device.

[0086] Electronic flow controllers **133**, **135**, which may be of a known type currently available including solenoid valves, are electronically coupled to and receive instruction signals from electronic controller **14** which has been programmed with and/or calculates a desired flow rate of oxygen and drug. Programmed flow rates may be those input by the physician user employing traditional choices regarding drug administration amounts and rates, including in IV embodiments, target controlled infusion principles, among others. Calculated flow rates may be arrived at through conservative decision-making software protocols including comparison of actual patient physiological condition feedback values with stored data representing safe and undesir-

able patient physiological conditions. Drug delivery is effected at the rates calculated in a closed, control-loop fashion (described in more detail below) by flow controllers **133**, **135**. Drug administration may be a combination of one or more physician inputs and/or electronic flow rate calculations based on patient and system state parameters; flow controllers may respond to instruction signals initiated by electronic controller **14** or by the physician.

[0087] Flow controllers **133**, **135** receive instruction signals from controller **14** reflecting the electronic output of both system state monitors (such as pressure sensors **106**, **206** described above) and patient state monitors. Flow controllers **133**, **135**, in response to instruction signals from controller **14**, may curtail or cease flow of drug delivery when system state and/or patient health monitors indicate to controller **14** that failures in the operation of care system **10** have occurred, that system **10** is otherwise operating outside of an established safe state, or that a patient's physiological state (e.g., vital signs or consciousness level) has deteriorated to an unsafe condition.

[0088] As the invention includes both intravenous and gaseous, among other forms of drug delivery, such embodiments may also include known electronic flow controllers coupled to electronic controller **14** and responsive to instruction signals from controller **14** reflecting both patient and system states.

[0089] Referring again to FIG. 8, solenoid valve **132** is electronically coupled to electronic controller **14** and must be activated by same before drug will flow through line **209**. In the event of system power failure, drug delivery will be halted due to the fail-closed nature of solenoid valve **132**. This is described, for example, in FIG. 21A which shows that if a system state monitor indicates power failure, alarm type "2" sounds to alert the nonanesthetist and drug delivery is halted (i.e., reduced to 0%).

[0090] Moreover, pressure actuated valve **134** in drug line **209** responds to the amount of pressure in O<sub>2</sub> line **109** and permits flow of gaseous drug only if sufficient oxygen flows through oxygen line **109**. Check valve **136a** in drug line **209** ensures that the flow of gaseous drug to manifold system **46** is one-way and that there is no back-flow. Check valve **136b** in oxygen line **109** ensures one-way flow of O<sub>2</sub> to manifold system **46** with no back-flow.

[0091] In atmospheric air line **139**, air inlet solenoid valve **137** is electronically coupled to and activated by electronic controller **14** and if activated permits atmospheric air to be mixed with the oxygen gas by means of air ejector **138**. Air ejector **138** injects a fixed ratio of atmospheric air into oxygen line **109**. Filter **128** removes contaminants from air line **139** and check valve **136c** ensures one-way flow of air from solenoid valve **137** to ejector **138** with no back-flow.

[0092] Referring to FIG. 9A which details one embodiment of manifold system **46** (FIG. 6), the drug/O<sub>2</sub> gas mixture from electronic mixer system **44** (FIG. 6) enters manifold system **46** and flows into inspiratory plenum **150** from which it proceeds through inspiratory line **151** to primary inspiratory valve (PIV) **152** and eventually to airway circuit **20** and mask **30** (FIG. 1). Primary inspiratory valve **152** permits one-way flow of said gas mixture and ensures that exhaled gases from the patient do not enter the inspiratory side of manifold system **46** (FIG. 6), thereby

guarding against possible contamination. Atmospheric air may be permitted to enter inspiratory line 151 through an inspiratory negative pressure relief valve (INPRV) 154 which allows one-way flow of atmospheric air to reach the patient if a significant negative vacuum is drawn on the inspiratory side of manifold system 46 (e.g., the patient inhales and receives no or insufficient oxygen). INPRV 154 thereby essentially permits air on demand by the patient. INPRV filter 153 removes particulates which may be in air line 155 or present in the atmosphere. INPRV status sensor 156 (which may be of a known pressure, temperature, infra-red or other suitable type) monitors the extent of open/close status of INPRV 154 and generates a signal which is converted to an appropriate electronic (digital) signal and communicates the status of INPRV 154 to electronic controller 14. During the exhalation phase of the patient's breathing cycle, inspiratory reservoir bag 149 collects the drug/O<sub>2</sub>/air mixture which the patient will draw on the next inhalation phase.

[0093] Still referring to FIG. 9A, pressure sensor 166 measures pressure in airway circuit 20 (FIG. 1) and is used to indicate airway flow, i.e., if the primary inspiratory valve (PIV) 152 or the primary expiratory valve (PEV) 168 is occluded. For example, if sensor 166 reads a high pressure that indicates that PEV 168 is blocked, whereas a low pressure indicates PIV 152 is blocked. Airway circuit 20 (FIG. 1) also contains a fraction of inspired oxygen (FIO<sub>2</sub>) sensor 167 (which may be of a known type currently available) which measures the oxygen percentage of gas contained in the mixture delivered to the patient, and thus guards against the possibility of delivering a hypoxic mixture to the patient (i.e., a drug/O<sub>2</sub> mixture that does not provide enough O<sub>2</sub> to the patient). INPRV status sensor 156, pressure/airway flow sensor 166, and FIO<sub>2</sub> sensor 167 are electronically coupled to and provide electronic feedback signals reflecting system state parameters to electronic controller 14. As described in FIGS. 21A and 23A, controller 14, through software and/or logic, effects a comparison of the signals generated by these system monitors with a stored data set of system parameters established by setpoints and/or logic-type data reflecting safe and undesirable system operating states, and conservatively controls (e.g., reduces or halts) drug delivery if the comparison determines that care system 10 is operating outside of a safe range.

[0094] Airway circuit and mask (20, FIG. 9) interface with the patient to provide a closed circuit for the delivery of drug/O<sub>2</sub> gas mixture to the patient. It should be recognized that embodiments of the subject invention in which the drugs are delivered in a form other than compressed gas, such as intravenously or transdermally, may not include face masks, airway circuit features and other aspects associated with delivery of drugs in gaseous form. Where the drug is delivered in gaseous form and an airway circuit and face mask are employed, such face mask and attendant airway circuitry and other features such as the scavenging system may be in the form of that described in U.S. Pat. No. 5,676,133 issued to Hickie et al. and entitled Expiratory Scavenging Method and Apparatus and Oxygen Control System for Post-Anesthesia Care Patients. (With respect to such embodiments, the specification of Hickie et al. is incorporated herein by reference.)

[0095] In preferred embodiments the mask is disposable and contains means for sampling the CO<sub>2</sub> content of the

patient's respiratory airstream and, optionally, means for also measuring the flow of the patient's airstream and/or means for acoustical monitoring. The sampling of the CO<sub>2</sub> in the patient's airstream may be done by means of a capnometer or a lumen mounted within the mask through a port in the mask, and placed close to the patient's airway. A second lumen similarly mounted within the mask could be used to measure the airflow in the patient's airstream. This airflow measurement could be accomplished by a variety of currently available devices, including for example, devices that measure the pressure drop in the airstream over a known resistance element and thereby calculate the airflow by known formula. The means for acoustical monitoring may be a lumen placed within the mask with a microphone affixed within that lumen. The microphone would permit recording, transducing and playing out through an amplifier the audible sound of the patient's breathing. It is noted that the lumen for acoustical monitoring could be a separate lumen or could be combined with the lumen for calculating the flow of the patient's airstream. It is further noted that it is important to place the lumens, especially the CO<sub>2</sub> sampling lumen, close to the patient's open airway and to ensure such lumens remain close to the patient's airway.

[0096] Referring again to FIG. 9A, primary expiratory valve (PEV) 168 in expiratory line 172 ensures one-way flow of a patient's exhaled gases to scavenger pump system 48, thus, prohibiting any back-flow from gases exhaled to the scavenger system from reaching the patient. Importantly, PEV 168 guards against the re-breathing of exhaled carbon dioxide. As is easily seen, the manifold 46 and airway circuit 20 of a preferred embodiment of this invention permit one-way airway flow only. That is, unlike prior devices that employ circular airway circuits (which require CO<sub>2</sub> absorbent material to permit re-breathing of exhaled air), there is no re-breathing of exhaled gases in this embodiment of the invention.

[0097] In the embodiment of the invention shown in FIG. 9A, expiratory positive pressure relief valve (EPPRV) 164 in expiratory line 172 allows exhaled gases to escape to the atmosphere if sufficient positive pressure develops on the expiratory side of the manifold system. This could happen, for example, if the patient is exhaling, but scavenger system 48 (FIG. 6) is occluded or otherwise not working properly. EPPRV filter 175 downstream of EPPRV 164 filters contaminants from the expiratory stream flowing through EPPRV 164 prior to the stream entering the atmosphere. Expiratory negative pressure relief valve (ENPRV) 178 is a one-way valve that allows atmospheric air to be drawn into expiratory plenum 180 and then on to scavenger system 48 if sufficient vacuum pressure is drawn on the expiratory side of manifold system 46. This could happen, for example, if the vacuum pump of scavenger system 48 is set too high or PEV 168 is blocked. Expiratory reservoir bag 177 collects exhaled gases from the patient during exhalation via expiratory plenum 180. These gases will be exhausted by scavenger system 48 during the next patient inhalation phase. As is described in detail below, patient vital sign monitor, such as a capnometer 184, monitors the amount of CO<sub>2</sub> in the patient's exhaled gases and provides electronic feedback signals reflecting the level of CO<sub>2</sub> in the patient's exhalations to controller 14. Other types of ventilatory monitors such as an airflow measure, IPG device or an acoustical monitor could also be used to provide electronic feedback signals reflecting patient health parameters to controller 14.

[0098] In an alternative preferred embodiment shown in FIG. 9B, ENPRV 164, filter 175 and ENPRV 178 are eliminated. A long pipe or similar conduit 175a, interconnected with reservoir bag 177 and opening to atmospheric air, is substituted therefor. The elimination of the valves 164 and 175 provides for a more cost efficient and simple system, while the substituting of the pipe 175a still ensures that if the scavenger system 48 is occluded, is set too high, is otherwise not working or if PEV 168 is blocked, that there is still access to atmospheric air, and the patient may breathe into the room or air may come into the system. A highly compliant reservoir bag 179 also assists in catching excess flow of exhaled air. In this simplified embodiment, there are essentially only three valves, PIV 152, PEV 168 and INPRV 154.

[0099] As is described above, system valves PIV 152 and PEV 168 ensure one-way flow of inspired and expired gases. The patient cannot re-breathe exhaled gases and no contaminants are allowed to enter the source system. The valve system INPRV 154, EPPRV 164, and ENPRV 178 (or the alternate INPRV 154 and pipe) provides a system fail-safe. If analgesic source system 42 (FIG. 6) or scavenging system 48 (FIG. 6) is functioning improperly, the valves will open and allow the patient to breath without significant effort. The system state sensors 156, 166 and 167 monitor system operation such as INPRV valve status, gas pressure and fraction of inspired oxygen, and electronically feed back signals reflecting the operating status of those operations to microprocessor controller 14 to ensure safe operation of the apparatus.

[0100] It is noted that the valves and sensors between INPRV 154 and ENPRV 178 in a preferred embodiment of manifold system 46 can be considered a system state monitoring system because there are no valves controlled by the software of electronic controller 14. At this point in the care system 10, the gas has already been mixed and the volume determined by the flow controllers 133, 135 (FIG. 8). Manifold system 46 (FIG. 6) provides at least two basic services, sensor inputs for  $\text{FiO}_2$  and  $\text{CO}_2$  (167, 184 of FIG. 9) and flow status derived from flow sensor 166 (FIG. 9).

[0101] The determination of appropriate drug delivery/flow percentages by controller 14 can be accomplished through a variety of methods. Initial drug administration amounts and rates may be selected and input by the physician employing traditional methods. Physicians may also employ pharmacokinetic/pharmacodynamic modeling to predict resulting drug concentrations and their effect based on physician choices, but not permit automatic changes to drug concentrations without instructions from the physician. In intravenous embodiments known target-controlled infusion techniques may be employed where the physician selects a desired (targeted) blood serum or brain effective site concentration based on such patient parameters as height, weight, gender and/or age.

[0102] During operation of the system when an internal or external event occurs, such as the activation of a system or patient health monitor alarm or a physician or patient request for increased drug, electronic controller 14 determines the desired amount of intravenous drug (or fractional amount of  $\text{O}_2$ , gaseous drug and air in the total gas flow) as the function of such event. The actual IV drug concentrations (or gaseous drug/ $\text{O}_2$ /air fractions) are then calculated. These actual calculated amounts will not always be the same as those

requested (e.g., by the user, patient or system) because of the often complex relationship between drug or drug and gas mixtures. In sum, drug mix fractions are typically calculated when, for example, an alarm levels change, alarm time-outs occur (e.g., there is no silencing of an initial alarm by the user), a user requests a change, the patient requests a change, when a procedure begins (system resorts to default values) and when a controller clock triggers.

[0103] In a preferred embodiment of the invention delivering gaseous drugs, flow controllers in mixer 44 (detailed in FIG. 8) determine the total fresh gas flow (FGF) which is the sum of the volumes of each gas being controlled, namely, the gaseous drug, oxygen and atmospheric air. Solenoid valves are opened proportionally to achieve the desired FGF and fractional amount of each gas. Flow controllers 133, 135 close the feedback loop on the gas fractions by measuring the  $\text{FiO}_2$  and fraction of inspired gaseous drug in the manifold system 46 and adjusting the mixer solenoid valves accordingly.

[0104] In one aspect of the invention, the flow controllers 133, 135 match the FGF with patient minute ventilation rates. The minute ventilation rate is the volume of breath one inhales and then exhales (e.g., in cubic centimeters or milliliters) in one minute. A patient's respiratory physiology is balanced at this minute ventilation. The care system optimizes FGF rates by matching gas delivery to patient minute ventilation rates. This conserves gas supplies, minimizes the release of anesthesia gases into the operating environment, and helps balance respiratory function. For example, if the FGF is less than the minute ventilation, INPRV 154 will open to supplement the air flow (INPRV-154 being a mechanical system not under electronic control).

[0105] In an additional aspect of the invention, the care system will not only measure and monitor minute ventilation as described above, but also "effective minute ventilation" and thereby improve the quantitative information about patient physiology considered by the system. "Effective minute ventilation" is a term used herein to mean the amount of gas that is actually involved in respiratory gas exchange between the alveolar sacs of the lungs and the capillary blood surrounding those sacs (as opposed to simply the volume of gas one inhales and then exhales, "tidal volume"). This measure may be arrived at by subtracting the volume of anatomical space imposed between the air source (edgy, mouth) and the transfer of gas at the alveolar sacs (estimated from the patient's height and weight), from the tidal volume of gas to arrive at "effective tidal volume." The effective tidal volume is then multiplied by respiratory rate to arrive at "effective minute ventilation."

[0106] FIG. 10A details manual bypass system 4 (FIG. 5) which is coupled to manifold system 46. The bypass system 4 includes a self-inflating resuscitation bag (SIRB) 19a (also shown in FIG. 3B) which is a manual pump with which the user can provide air intermittently to the patient through a bypass air line 90. A quick disconnect type fitting 91 (such as that disclosed in Hickie above) couples SIRB 19a with manifold system 46 and provides rapid attachment thereto. A manual flow control valve 92 opens or closes bypass air line 90. When line 90 is open, manual flow control valve 92 can be adjusted to provide the necessary air flow. A flow meter 94 placed in bypass air line 90 provides a visual

display to the user of the status of air flowing through the bypass air line 90. The above-described manual bypass system 4 provides the patient with manually-controlled flow of air and thus enables air delivery in the case of an oxygen source system 144 (FIG. 7A) failure.

[0107] FIG. 10B details scavenger pump system 48 (FIG. 6) which is integrated into the care system and vacuums exhaled gases from manifold system 46 through a scavenging line 85. A filter 86 in scavenging line 85 removes contaminants from the gases which have been exhaled from the patient and which are flowing through the scavenger line 85. Pressure regulator 87 receives the filtered gases and ensures that the vacuum pressure is maintained in vacuum pump 95 downstream at a reasonable working level. Flow restrictor 88 sets the flow rate through the vacuum 95 for a given vacuum pressure. Check valve 89 downstream of flow restrictor 88 provides one-way flow of scavenged gases, and thus ensures that back-flow does not inadvertently flow into scavenger system 48 from the vacuum pump 95 downstream. vacuum pump 95 provides the vacuum pressure necessary for scavenging of exhaled gases from the patient. The pump may be of an electrical type that can be powered by office standard AC current. As the vacuum pump is integrated into the care system, a wall vacuum source (such as that typically in an OR) is not required. Once the gases are vacuumed off, they are exhausted via exhaust hose 32 (FIG. 3B) to an appropriate area. The benefit of scavenging system 48 is at least two-fold in that the system helps assist the patient in the work of breathing and work environment safety is increased.

[0108] In a preferred embodiment, an emesis aspirator 19 (FIG. 3B) is integrated into system 10 and may be stored within housing 15. Emesis aspirator 19 is a manually operated device used to suction a patient's airway in the event of vomiting. Emesis aspirator 19 does not require an external vacuum source (e.g., wall suctioning) or electrical power for operation.

[0109] To enhance the safety of the invention, housing 15 may include structure integrated adjacent or otherwise near where emesis aspirator 19 is stored within housing 15 (FIG. 3B) to hold and prominently display containers of drugs capable of reversing the effects of various sedatives/analgesics. These "reversal drugs," such as naloxone, remazicon and others may be immediately administered to the patient in the event of an overdose of sedative, analgesic and/or amnestic.

[0110] Referring to FIG. 11, a preferred embodiment of the invention includes an integrated patient interface system which combines one or more patient health monitors 252 (additional health monitors to those shown are also contemplated by the invention) with additional automated patient feedback devices including a patient drug dosage increase or decrease request device 254 and an automated consciousness query system 256 for monitoring a patient's level of consciousness. These health monitors 252 and automated patient feedback devices 254, 256 are electronically coupled to electronic controller 14 via leads (e.g., 50, FIG. 2) and provide electronic feedback values (signals) representing the patient's physiological condition to controller 14. Generally, if any monitored patient parameter falls outside a normal range (which may be preset by the user or otherwise preprogrammed and stored in memory device as described

above), the nonanesthetist is immediately alerted, for example, by an alarm, display or other attention-commanding device. The information obtained from patient health monitors 252 is displayed on a display device 35 (FIG. 2), in, for example, continuous wave form or numerics on LEDs, thus allowing the procedural physician to immediately gain useful information by reviewing the display device. Preferred embodiments of displays contemplated by the invention are described in more detail below.

[0111] A preferred embodiment of one aspect of the invention integrates drug delivery with one or more basic patient monitoring systems. These systems interface with the patient and obtain electronic feedback information regarding the patient's physiological condition. Referring to FIG. 11, a first patient monitoring system includes one or more patient health monitors 252 which monitor a patient's physiological conditions. Such monitors can include a known pulse oximeter 258 (e.g., an Ohmeda 724) which measures a patient's arterial oxygen saturation and heart rate via an infra-red diffusion sensor; a known capnometer 184 (e.g., a Nihon Kohden Sjsi2) which measures the carbon dioxide levels in a patient's inhalation/exhalation stream via a carbon dioxide sensor and also measures respiration rate; and a known non-invasive blood pressure monitor 262 (e.g., a Criticon First BP) which measures a patient's systolic, diastolic and mean arterial blood pressure and heart rate by means of an inflatable cuff and air pump. A care system constructed in accordance with this invention may include one or more of such patient health monitors. Additional integrated patient health monitors may also be included, such as, for example, a measure of the flow in a patient's airstream, IPG ventilatory monitoring, a standard electrocardiogram (EKG) which monitors the electrical activity in a patient's cardiac cycle, an electroencephalograph (EEG) which measures the electrical activity of a patient's brain, and an acoustical monitor whose audio signals may be processed and provided to controller 14 and amplified and played audibly.

[0112] A second patient monitoring system monitors a patient's level of consciousness by means of an automated consciousness query (ACQ) system 256 in accordance with the invention. ACQ system 256 comprises a query initiate device 264 and a query response device 266. ACQ system 256 operates by obtaining the patient's attention with query initiate device 264 and commanding the patient to activate query response device 266. Query initiate device 264 may be any type of a stimulus such as a speaker which provides an auditory command to the patient to activate query response device 266 and/or a vibrating mechanism which cues the patient to activate query response device 266. The automated pressurization of the blood pressure cuff employed in the patient health monitoring system may also be used as a stimulus. Query response device 266 can take the form of, for example, a toggle or rocker switch or a depressible button or other moveable member hand held or otherwise accessible to the patient so that the member can be moved or depressed by the patient upon the patient's receiving the auditory or other instruction to respond. In a preferred embodiment, the query system has multiple levels of auditory stimulation and/or vibratory or other sensory stimulation to command the patient to respond to the query. For example, an auditory stimulus would increase in loudness or urgency if a patient does not respond immediately or a vibratory stimulus may be increased in intensity.

[0113] After the query is initiated, ACQ system 256 generates signals to reflect the amount of time it took for the patient to activate response device 266 in response to query initiate device 264 (i.e., this amount of time is sometimes referred to as the "latency period"). ACQ system 256 is electronically coupled to electronic controller 14 and the signals generated by ACQ system 256 are suitably converted (e.g., employing an A-D converter) and thereby provided to controller 14. If the latency period is determined by controller 14, which employs software to compare the actual latency period with stored safety data set parameters reflecting safe and undesirable latency period parameters, to be outside of a safe range, the physician is notified, for example, by means of an alarm or other attention-commanding device. If no action is taken by the physician within a pre-set time period, controller 14 commands the decrease in level of sedation/analgesia/amnesia by control and operation on electronic flow controllers 133, 135 of FIG. 8. The values of the signals reflecting the latency period are displayed on display device 35 (or on LED devices located on housing 15 or on remote control device 45, FIG. 1) and the physician may thus increase or decrease drug delivery based on the latency period.

[0114] The patient interface system of FIG. 11 also includes a drug dosage request device 254 which allows the patient direct control of drug dosage. This is accomplished by the patient activating a switch or button to request electronic controller 14 to command the increase or decrease in the amount of drug he or she is receiving. For example, if a patient experiences increased pain he or she may activate the increase portion of the switch 254, whereas, if a patient begins to feel nauseous, disoriented or otherwise uncomfortable, he or she may request a decrease in drug dosage. In embodiments where drug delivery is intravenous, such delivery can be by continuous infusion or bolus. A feedback signal from analgesic request 254 representing the patient's increase or decrease in drug dosage request is electronically communicated to controller 14 which employs conservative, decision-making software, including comparison of monitored patient conditions with stored safety parameters reflecting patient physiological conditions, to effect safe, optimized drug delivery in response to patient requests. The amount of increase or decrease administered by controller 14 can be pre-set by the physician through user access devices such as keyboard 230, FIG. 2. For example, where the drug being delivered is nitrous oxide, the approved increase or decrease may be in increments of  $\pm 10\%$ . When not activated by the patient, drug request device 254 remains in a neutral position. The invention thus integrates and correlates patient-controlled drug delivery with electronic monitoring of patient physiological conditions.

[0115] In an alternative embodiment, the physician is notified via user interface system 16 (display device 30 or LEDs remote control device 45), FIG. 1 of the patient request to increase or decrease drug dosage and can approve the requested increase or decrease taking into account the patient's present vital signs and other monitored physiological conditions, including consciousness level status as obtained from the various patient interface system monitors 252, 256 (FIG. 11).

[0116] In a preferred embodiment of the invention, the patient controlled drug dosage request system 254 has lock-out capabilities that prevent patient self-administration

of drugs under certain circumstances. For example, access to self-administration will be prevented by electronic controller 14 under circumstances where patient physiology parameters or machine state parameters are or are predicted to be outside of the stored safety data set parameters. Access to self-administration of drugs could also be inhibited at certain target levels or predicted target levels of drugs or combined levels of drugs. For example, if it were predicted that the combined effect of requested drugs would be too great, drug delivery in response to patient requests would be prohibited. It is noted that such predictive effects of drugs could be determined through the use of various mathematical modeling, expert system type analysis or neural networks, among other applications. In short, the invention is designed to dynamically change drug administration and amount variables as a function of patient physiology, care system state and predictive elements of patient physiology.

[0117] Additionally, it is contemplated that patient self-administration of drugs could be prohibited at times when drug levels are changing rapidly. For example, if a patient is experiencing pain and that is apparent to the physician, the physician may increase the target level of drug while at the same time the patient requests additional drug. The subject invention will sequentially address the physician and patient requests for drug increases and will lock out any patient-requested increases that are beyond programmed parameters.

[0118] In an additional aspect of the invention, a patient may be stimulated or reminded to administer drugs based on electronic feedback from the patient physiology monitoring systems. For example, if there is an underdosing of analgesics and the patient is suffering pain evidenced by a high respiratory rate or high blood pressure reflected in electronic feedbacks to the electronic controller, the controller can prompt the patient to self-administer an increase in drugs. This could be accomplished by, for example, an audio suggestion in the patient's ear. Thus, it is contemplated that the invention will have an anticipatory function where it will anticipate the patient's needs for increased drugs.

[0119] In a preferred embodiment of the invention, one or more patient vital sign monitoring devices 252, ACQ system devices 256, and a drug dosage request device 254 are mechanically integrated in a cradle or gauntlet device 55 (FIG. 2) constructed to accommodate and otherwise fit around a patient's hand and wrist. FIG. 2 shows generally hand cradle device 55 electronically coupled by lead 50 to care system 10. One embodiment of a hand cradle device in accordance with this invention is shown in more detail in FIGS. 12A and 12B.

[0120] FIG. 12A shows blood pressure cuff 301 capable of being wrapped around a patient's wrist and affixed to itself such that it can be held in place. Cuff 301 is affixed to palm support portion 303. Alternatively, the cuff may be separated from palm support portion 303 and placed on the upper arm at the physician's discretion. A recessed, generally elliptical or rounded portion 305 is supported by the top edge of palm support portion 303 and is capable of receiving and supporting the bottom surface of a patient's thumb. Depressible query response switch 307 is located within thumb support portion 305 such that switch 307 is capable of being depressed by the patient's thumb. The thumb support portion 305 may be constructed so as to have a

housing, frame, raised walls or other guide so that a patient's thumb may more easily be guided to depress or move buttons or switches within portion **305** (here, switch **307**), or so that any significant patient thumb movement toward the switch will activate same. Supporting thumb support portion **305** and abutting palm portion **303** is finger support portion **309** for receiving in a wrapable fashion the patient's fingers. Drug dosage request switch **311** is integrated into finger support portion **309** and is in the form of a rocker switch whereby depressing the top portion **310a** of said switch will effect an increase in the delivery of sedative, analgesic and/or amnestic whereas depressing the bottom portion **310b** of said rocker switch will effect a decrease in drug delivery at an appropriate set percentage (e.g., +10%, **FIG. 12B**). Rocker switch **311** is constructed so as to remain in a neutral position when not being actuated by the patient.

[0121] **FIGS. 13A and 13B** show an additional embodiment of the hand cradle device of this invention. Specifically, a pulse oximetry sensor **314** is mechanically affixed to and electronically coupled to hand cradle device **55** abutting the upper end of finger support portion **309**, and being generally planar vis-a-vis the outer edge of thumb support portion **305**. Pulse oximeter **314** is constructed as a clip which can be placed on a patient's finger. The transmitter and receiver portions of sensor **314** are contained in the opposite sides **315a**, **315b** (**FIG. 13B**) of the finger clip **314** such that when placed on a finger, infra-red radiation travels through the finger; through spectral analysis the percentage of oxygenated hemoglobin molecules is determined. In this embodiment of hand cradle device **55** the query initiate device **313** is in the form of a small vibrator located in palm support portion **303**. Alternatively, to enhance patient attentiveness to the query initiate device and to increase patient accuracy in depressing the response switch, the vibrator may be located adjacent the query response switch **307** or, in the embodiment of **FIG. 14A**, adjacent response switch **407**.

[0122] In an alternative embodiment of hand cradle device **55**, now referring to **FIGS. 14A and 14B**, drug dosage request device **409** is located within thumb portion **405** and is in the form of a slidable member **409** wherein sliding member **409** forward effects an increase in analgesic dosage and sliding portion **409** backward effects a decrease in analgesic dosage (**FIG. 14B**). In this embodiment of the invention, query response device **407** is a depressible portion integrated within finger support portion **409**.

[0123] All embodiments of hand cradle device **55** are constructed so as to be ambidextrous in nature, namely, they accommodate and are workable by a patient's right or left hand. For example, in **FIGS. 12A and 13A**, a second query response switch **307b** is located within a symmetrically opposed thumb portion **305b** affixed to the opposite end of finger portion **309**. Similarly the device of **FIG. 14A** is also constructed with a symmetrically opposed thumb portion **405b** and drug dosage request device **409b**. The pulse oximeter clip **314** is affixed to finger support portion **309** so as to be mechanically and electronically quick releasable to permit reversibility when used on the opposite hand. It should also be recognized that the pulse oximeter clip **314** may be tethered to hand cradle device **55** rather than mechanically affixed thereto, or blood pressure cuff **301** and oximeter clip **314** may be mechanically separate from cradle device **55** and electronically coupled to controller **14** with flexible leads.

[0124] Referring to **FIG. 15**, an additional alternative embodiment of the invention is shown in which hand cradle device **55** includes mechanically integrated blood pressure cuff **301**, query response device **307** and analgesic request device **309** similar to that described above. This embodiment, however, includes an ear clip device **450** capable of being clipped to the lobe of a patient's ear and being electronically coupled to electronic controller **14** via lead **456**. Referring additionally to **FIG. 16**, ear clip **450** comprises a query initiate device **452** in the form of a speaker which provides an audible command to patient to activate the response switch. Such speaker may also command a patient to self-administer drugs or play music to a patient during a procedure. Pulse oximeter **454** is a clip capable of being affixed to a patient's ear lobe. One side of the clip being a transmitter and the other side of the clip being a receiver to effect the infra-red spectral analysis of the level of oxygen saturation in the patient's blood.

[0125] In an additional aspect of the invention, it is contemplated that the care system's automated monitoring of one patient health conditions is synchronized with the monitoring of one or more other patient health conditions. For example, in a preferred embodiment, if the controller **14**, receives low O<sub>2</sub> saturation, low heart rate or a low perfusion index feedback information from the pulse oximeter (e.g., the actual parameter received is in the undesirable range of the stored safety data set for those parameters), such feedback will trigger controller **14** to automatically inflate the blood pressure cuff and check the patient's blood pressure. (This is because low O<sub>2</sub> saturation can be caused by low blood pressure; and low heart rate can cause low blood pressure and vice versa, etc.) Therefore, under normal operating conditions the preferred embodiment of the invention will automatically check the patient blood pressure every 3 to 5 minutes, and whenever there is a change in other patient parameters such as blood O<sub>2</sub> saturation or heart rate. In another example, the electronic checking of blood pressure is synchronized with the automated consciousness query because the activation of the cuff may arouse a patient and affect query response times. Thus the invention contemplates an "orthogonal redundancy" among patient health monitors to ensure maximum safety and effectiveness.

[0126] As described above, one aspect of a preferred embodiment of the invention includes the electronic management of drug delivery via software/logic controlled electronic controller **14** to integrate and correlate drug delivery with electronic feedback signals from system monitors, one or more patient monitor/interface devices and/or user interface devices. Specifically, electronic signal values are obtained from care system state monitors; from patient monitor/interface devices (which can include one or more vital sign or other patient health monitors **252**, ACQ system **256**, and/or patient drug dosage request device **254**, **FIG. 11**); and in some instances from one or more user interface devices. All are electronically coupled to, through standard A-D converters where appropriate, electronic controller **14**. The controller **14** receives the feedback signal values and, via software and programmed logic, effects a comparison of these values representing the patient's monitored physiological conditions with known stored data parameters representing safe and undesirable patient physiological conditions (a safety data set). Controller **14** then generates an instruction in response thereto to maintain or decrease the level of sedation, analgesia, and/or amnesia being provided

to the conscious patient thereby managing and correlating drug delivery to safe, cost-effective and optimized values (**FIG. 2B**. Controller **14** is operatively, electronically coupled to electronic flow controllers **133**, **135** (**FIG. 8**) of electronic mixer **44** which (via solenoid valves) adjust flow of gaseous drug and O<sub>2</sub> in a closed-loop fashion as described above. In intravenous embodiments such flow controllers would adjust the flow of one or more combination of IV drugs. It should be recognized that the electronic values provided to microprocessor controller **14** to effect management and correlation of drug delivery, could include one or more signals representing patient vital signs and other health conditions such as pulse oximetry, without necessarily including signal(s) representing level of patient consciousness, and vice versa.

[0127] As also indicated above, the software effecting electronic management of drug delivery by controller **14** employs "conservative decision-making" or "negative feedback" principles. This means, for example, that the electronic management of drug delivery essentially only effects an overall maintenance or decrease in drug delivery (and does not increase drugs to achieve overall increased sedation/analgesia). For example, if ACQ system **256** (**FIG. 11**) indicates a latency period outside of an acceptable range, controller **14** may instruct electronic flow controller **133** (**FIG. 8**) to increase the flow of oxygen and/or instruct flow controller **135** to decrease the flow of gaseous drug to manifold system **48**.

[0128] In another example of such electronic management of drug delivery by conservative decision-making principles, if ACQ system **256** (**FIG. 11**) indicates a latency period in response to a patient query given every 3 minutes outside of an acceptable range, electronic controller **14** may immediately cease drug delivery, but at the same time, increase the frequency of times that the patient is queried, e.g., to every 15 seconds. When the patient does respond to the query, the drug delivery is reinitiated, but at a lower overall dose such as 20% less than the original concentration of drug that had been provided.

[0129] A further example of the invention's electronic management of drug delivery through conservative, decision-making software instruction employs known target-controlled infusion software routines to calculate an appropriate dosage of IV drug based on patient physical parameters such as age, gender, body weight, height, etc. Here, a practitioner provides the patient physiological parameters through the user interface system, the electronic controller **14** calculates the appropriate drug dosage based on those parameters, and drug delivery begins, for example, as a bolus and is then brought to the pre-calculated target level of infusion. If later there is a significant change in a patient monitored parameter, e.g., pulse oximetry or latency period falls outside of a desired range, controller **14** effects a decrease in overall drug delivery as described above.

[0130] One concern that the invention addresses with respect to the target controlled infusion of IV drugs is the nature and speed at which the care system reaches the steady state target level of drug. For example, an important consideration for the physician is, once drug administration begins, when is the patient sufficiently medicated (e.g., sedated or anesthetized), so that the physician can begin the procedure. It is frequently desirable that the patient reach the

steady state target level of drug as rapidly as possible so that the procedure can begin as soon as possible. It has been determined that one way of reaching a suitable level of drug effectiveness quickly is to initially overshoot the ultimate steady state target drug level. This shortens the time between the beginning of drug delivery and the onset of clinical drug effectiveness so that the procedure may begin. Typically, predicted target levels have an error of plus or minus 20%, therefore, one approach of reaching the clinical effectiveness state quickly is to attempt to reach at least 80% of the ultimate target level, but initially overshoot that 80% level by giving a 15% additional increase of drug infusion beyond the 80% target. One method of accomplishing this is to use currently available PDI controllers which employ an error state (here the difference between predicted drug levels in the blood stream and the target level) to arrive at an infusion rate. Other control systems, however, that allow some initial overshoot of the target blood level of the drug to get to a clinical effectiveness level quicker would also be appropriate.

[0131] **FIG. 17** is a schematic of an alternative embodiment of an apparatus constructed in accordance with the invention which is particularly suitable for remote medical care locations and home care-type settings for indications such as post-operative or other post-procedural pain and/or discomfort, including, for example, nausea secondary to oncology chemotherapy. In this embodiment, drug source system **442** delivers drugs to the patient (which may be drugs such as propofol, morphine, remifentanyl and others) intravenously by, for example, use of a known syringe pump-type device capable of being worn or otherwise affixed to the patient, or delivers such drugs transdermally by, for example, use of known ion transfer-type devices, among others. The drug delivery may be continuous or by drug bolus and without an integrated supply of O<sub>2</sub>. If necessary, oxygen may be supplied to the patient from separate tanks or an in-house, on-site oxygen source. The resulting apparatus is simplified—there is no requirement for an integrated O<sub>2</sub> source, electronic mixer, manifold, or the airway circuit and face mask devices described above.

[0132] One or more patient health monitors **412** such as known pulse oximeters, blood pressure cuffs, CO<sub>2</sub> end tidal monitors, EKG, and/or consciousness monitors, or other monitors such as those indicated herein, monitor the patient's physiological condition. Drug dosage may be pre-set by a physician prior to or during application of drug delivery and/or also patient controlled thereafter by means of a patient drug dosage increase or decrease request devices generally of the type of that described above. It should also be understood that the intravenous delivery of drugs may be by continuous infusion, target-controlled infusion, pure bolus, patient-elected bolus or combinations thereof.

[0133] Still referring to **FIG. 17**, electronic management of drug delivery in this embodiment of the invention is provided by electronic controller **414** which may be of a type described above. Controller **414** employs conservative decision-making software and/or logic devices to integrate and correlate drug delivery by drug source system **442** (which may include known solenoid type or other electronic flow controllers) with electronic feedback values from one or more patient health monitors **412**. The values (signals) from patient health monitors **412** represent one or more actual patient monitored physiological conditions. Controller **414**,

through software employing comparison protocols such as those described herein, accesses stored safety data set **410** which contains data reflecting safe and undesirable patient physiological conditions, and compares the signals reflecting actual patient monitored conditions with same. As described above, safety data set **410** may be stored in a memory device such as an EPROM. Based on the result of the comparison, controller **414** either instructs no change in drug delivery or generates a signal instructing the drug flow controllers of drug source system **442** to manage application of the drug to safe, optimized levels.

[0134] In certain aspects of the invention, controller **414** may also access, through software, pre-set parameters stored in a memory device representing initial or target drug dosages and lock-outs of patient drug administration requests as described above. In these circumstances, instruction signals generated by controller **414** would also account for and control drug delivery in accord with these pre-set parameters.

[0135] This embodiment of the invention would also typically include system state monitors, such as electronic sensors which indicate whether power is being supplied to the system or which measure the flow of drugs being delivered. Such system state monitors are electronically coupled to controller **414** and provide feedback signals to same—the control of drug delivery by controller **414** electronically coupled to drug source system **442** in response to said feedback signals is similar to that as described herein with respect to other embodiments.

[0136] In another aspect of the invention, electronic controller **414** is located on a remote computer system and electronically manages on-site drug delivery integrating and correlating same with on-site monitoring of patient physiological conditions and care system status as described above, but here with instructions signals generated from a remote location. It is contemplated that controller **414** may, in some embodiments, effect transmission via modem or electronic pager or cellular-type or other wired or wireless technologies of electronic alarm alerts to remote locations if a monitored patient parameter such as the percentage of oxygen absorbed into the blood ( $S_pO_2$ ) falls outside of a safe established value or range of values as established by the stored safety data set. Such remote locations could thereby summon an ambulance or other trained caregiver to respond to the alarm alert.

[0137] FIG. 18 details the user interface system of a preferred embodiment of the invention. This system enables the physician to safely and efficaciously deliver one or more of sedation, analgesia or amnesia to a patient while concurrently performing multiple tasks. The user interface permits the physician to interact with the care system and informs the user of the patient's and system's status in passive display devices and a variety of active audio/visual alarms thereby enhancing the safety and enabling immediate response time (including the "conservative" responses, e.g., detailed drug delivery discussed above) to abnormal situations.

[0138] Specifically, a keypad and/or touch screen **230** (FIGS. 2 and 18) allows the physician to interact with electronic controller **14**, inputting patient background and setting drug delivery and oxygen levels. A remote control device **45** (FIGS. 1 and 18) provides the physician with

remote interaction with the care system **10** allowing him or her to remotely control the functions of the system. Remote control device **45** may be removably integrated into the top surface of housing **15** and capable of being clipped onto material close to the physician and/or patient. In one aspect of the invention, the remote control device **45** itself contains display devices such as LEDs to advise the physician of patient and system parameters. A panic switch **232** (FIG. 18), which may be on-board housing **15** (FIG. 1) or contained in remote control device **45** and electronically coupled to controller **14** allows the physician to shut down care system **10** and maintains it in a safe state pre-programmed into controller **14**.

[0139] Visual display devices **234** (FIG. 2, 35) display actual and predictive or target patient and system parameters and the overall operation status of the care system.

[0140] One version of a preferred embodiment of visual display **234** is shown in FIG. 22. The display **2230** includes a first portion of the display **2234** which is devoted to displaying to the user the current status of the system operation and monitored patient conditions, including the status of any alarm caused by a change in monitored system or patient condition. For example, if a patient's timed response to a consciousness query (latency period) is outside an established range and an alarm is thus activated, that query latency period is displayed in this first portion **2234** of the visual display, thereby enabling the physician to immediately understand the cause of the alarm.

[0141] The visual display device **2230** of this embodiment also includes a second portion of the display **2236** which is devoted to displaying the actions taken or soon to be taken by the care system. For example, if in response to an alarm indicating a latency period outside of an established safe range the apparatus will decrease the flow of drug to the patient, this second portion **2236** displays the percentage decrease in drug dosage to be effected.

[0142] Visual display **2230** facilitates the physician's interaction with the apparatus by walking the physician through various system operation software subprograms. Such subprograms may include system start-up where a variety of system self-checks are run to ensure that the system is fully functional; and a patient set-up. To begin the procedure, the care system monitors are placed on the patient and the physician activates the system by turning it on and entering a user ID (it is contemplated that such user ID would only be issued to physicians who are trained and credentialed). Next, the visual display would prompt the physician to begin a pre-op assessment, including inputting patient ID information and taking a patient history and/or physical. In the pre-op assessment, the physician poses to the patient a series of questions aimed at determining appropriate drug dosage amounts (such as age, weight, height and gender), including factors indicative of illness or high sensitivity to drugs. The responses to such questions would be inputted into the care system and employed by the system to assist the physician in selecting the appropriate dose amount. For example, the care system may make available to the physician one range of dosage units for a healthy person and a narrower range of dosage units for a sick or older person. The physician would have to make an explicit decision to go above the recommended range.

[0143] In addition to the pre-op assessment performed by the physician described above, it is also contemplated that

the care system is capable of performing an automated pre-op assessment of the patient's physiology. For example, with the monitors in place, the care system will assess such parameters as the oxygenation function of the patient's lungs and/or the ventilatory function of the patient's lungs. The oxygenation function could be determined, for example, by considering the A-a gradient, namely, the alveolar or lung level of oxygen compared to the arteriolar or blood level of oxygen. The ventilatory function of the lungs could be determined from pulmonary function tests (PFTs), among other things, which are measurements of the amount of air and the pressure at which that air is moved in and out of the lungs with each breath or on a minute basis. (It is contemplated that these assessments are performed before the procedure begins and during the procedure as a dynamic intra-operative assessment as well.) Also during the pre-op (or as a continuous intra-operative) assessment, heart function may be assessed by viewing the output of an EKG to determine whether there is evidence of ischemia or arrhythmias. Alternatively, automated algorithms could be applied to the EKG signals to diagnose ischemia or arrhythmias. Additional automated patient health assessments could also be made.

[0144] During patient set-up, current patient and system parameters may also be assessed and displayed, and the consciousness-query system and patient drug increase/decrease system tested and baselined. A set drug subprogram allow for the selection of drugs and/or mixture of drugs (or drug, oxygen and air), allows for picking target levels of drugs, and/or permits enabling of the patient's self-administration of drugs within certain ranges. The invention also contemplates during the pre-op assessment determining a sedation threshold limit for the given patient in the unstimulated state. This could be done as a manual check, i.e., by simply turning up the drug levels and watching the patient manually or the procedure could be automated where the drugs are increased and the safety set parameters such as those for latency (consciousness queries) are tested as the concentration at the drug effect site is increased.

[0145] The system and patient status and system action may be displayed during, for example, a sedation subprogram. Visual display device 2230 may include graphical and numeric representations of patient monitored conditions such as patient respiratory and ventilatory status, consciousness, blood O<sub>2</sub> saturation, heart rate and blood pressure (2238); an indication of elapsed time from the start of drug delivery (2239); drug and/or O<sub>2</sub> concentrations (2241); and indications of patient requests for increases or decreases in drug (2243). The actual fraction of inspired oxygen calculated may also be displayed. Command "buttons" are included to mute alarms (2240), change concentration of drug delivered (2242), turn on or off the mixing of an oxygen stream with atmospheric air (2244), and to turn on or off or make other changes to the automated consciousness query system (2246). Command buttons may also be included to place the apparatus in a "recovery" mode once the procedure is completed (patient parameters are monitored, but drug delivery is disabled) (2248), and to end the case and start a new case (2250) or shut-down the system.

[0146] An alternate version of a preferred embodiment of the visual display portion of the invention is shown in FIG. 22A. Portions 2202, 2204, 2206 and 2208 of display device 2200 show current patient O<sub>2</sub> saturation, blood pressure,

heart rate, and end tidal CO<sub>2</sub> levels, respectively. These portions displaying patient physiological state are uniquely color coded. Smart alarm box portion 2212 which may be coded in an attention getting color such as red, displays to the physician the particular alarm that has sounded. For example, if the patient O<sub>2</sub> blood saturation level falls below safe levels, the O<sub>2</sub> saturation alarm will sound and the O<sub>2</sub> saturation level will appear in smart alarm box portion 2212 where it can be easily seen by the physician. In short, whatever parameter has alarmed is moved to the smart alarm box portion; the specific alarm indicator is moved to the same place every time an alarm sounds. Also, the level of criticality of the alarm which, as described below, in a preferred embodiment may be indicated by either yellow or red color, is displayed in the patient physiological parameter portion of the display. For example, if a red level O<sub>2</sub> saturation alarm sounds, the background portion of the O<sub>2</sub> saturation portion 2202 will appear in red.

[0147] Portion 2214 of display 2200 shows the past, present and predicted levels (2215) of drug administration (the drug levels shown in FIG. 22A are the levels of nitrous oxide remifentanyl and propofol). In a preferred embodiment target controlled infusion past, present and predicted levels are shown graphically beginning with the past thirty minutes and going thirty minutes into the future. The invention also contemplates bracketing a range of accuracy of target controlled infusion levels (not shown).

[0148] Display portions 2220 and 2224 depict graphical representations of patient health parameters such as the A-a gradient (oxygenation function) for the lungs, the results of pulmonary function tests, electrocardiogram, blood O<sub>2</sub> saturation, among others.

[0149] In another aspect of the invention, visual display 35 (FIG. 1) may be removably integrated into the top surface of housing 15 and capable of being removed from housing 15 and affixed to a frame near the patient, such as a gurney rail or examination table. Alternatively, or in addition thereto, a heads-up type visual display device is provided to facilitate a nonanesthetist's involvement in the medical or surgical procedure while simultaneously being able to view the status of system and patient monitored values and the details of alarm states. In this case, the display device is miniaturized and mounted onto a wearable headset or eyeglass-type mount or mounted on an easily viewed wall display.

[0150] Referring again to FIG. 18, in a preferred embodiment, audible alarms 236 alert the physician when patient or system parameters are outside of the normal range. In preferred embodiments, the alarms may be two or three stages with different tones to indicate different levels of concern or criticality. As is described above, when an alarm sounds, the user is able to immediately view the cause of the alarm because the smart alarm box portion 2212 of the visual display 2200 shows the value of the monitored system or patient parameter that caused the alarm to activate.

[0151] FIG. 21 shows examples of drug delivery management protocols for three-stage alarms responsive to patient monitors, namely, alarms "1," "2" and "3," in accordance with a preferred embodiment of one aspect of the invention. These alarms may have different tones or other indicators to denote different levels of concern or criticality. The dataflow diagram of FIG. 23 depicts one example of the steps

performed by the drug delivery managing software or logic for one such protocol, namely, one where electronic controller **14** described above receives an electronic feedback signal from a pulse oximeter monitoring the actual amount of oxygen saturation in a patient's blood (the value indicated by "SpO<sub>2</sub>"). As is shown, the SpO<sub>2</sub> value is compared with stored safety data set **220** containing a parameter value or range of parameters values reflecting safe and undesirable patient blood oxygen saturation conditions. If the SpO<sub>2</sub> value is greater than or equal to stored parameter 90%, no alarm sounds and no adjustment to drug delivery is effected (**221a**). If the SpO<sub>2</sub> value is less than 90%, but greater than 85% (**221b**), alarm **1** sounds for 15 seconds (**222**). If alarm **1** is silenced manually (**222a**), no further action is taken by the system. If alarm **1** is not silenced, the amount of drug being delivered (in this example gaseous N<sub>2</sub>O) is reduced to the lesser of a concentration of 45% or the current concentration minus 10% (**223**). The software/logic procedure would operate in a similar fashion for intravenous and nebulized forms of drugs and the instructions provided (e.g., as in **223**) would be specified for safe dosages of such drugs.

[**0152**] Further, if the value of oxygen saturation (SpO<sub>2</sub>) is less than 85%, but greater than or equal to 80% (**221c**), alarm **2** sounds and the amount of N<sub>2</sub>O being delivered is immediately reduced to the lesser of a concentration of 45% or the current concentration minus 10% (**224**). If the feedback value SpO<sub>2</sub> from the pulse oximeter indicates that the oxygen saturation in the blood is less than 80%, alarm **3** sounds and the amount of N<sub>2</sub>O being delivered would be immediately reduced to 0% (**225**).

[**0153**] Similar protocols are described in **FIG. 21** for electronic feedback signals from patient health monitors indicating pulse rate, amount of carbon dioxide in a patient's end tidal exhalations, respiration rate, systolic blood pressure, and feedback from the automated consciousness monitoring system constructed in accordance with the invention. These protocols are effected with software (and/or logic) operating in similar fashion to that described in the dataflow diagram of **FIG. 23**. That is, the protocol shown in **FIG. 23** is one example employing one patient monitored parameter, but the operation of the invention would be similar to effect the remaining protocols of **FIG. 21**.

[**0154**] It should be understood that the system responses to alarms (described above in terms of decreases or cessation of drug concentration) could also include institution and/or increases in administration of oxygen in accord with patient and system state parameters as described above. In circumstances where drugs are halted and pure oxygen (or an O<sub>2</sub> atmospheric mix) is provided, e.g., where feedback signals indicate the patient has a low blood O<sub>2</sub> saturation, a preferred system is designed to operate in a LIFO ("last-in-first-out") manner. This means that when controller **14** receives feedback signaling an adverse patient or machine state and instructs flow controllers to turn on the oxygen, the very next breath the patient takes will be of pure O<sub>2</sub> (and/or atmospheric air) rather than of a drug/air mixture. This may be accomplished, for example, by supplying O<sub>2</sub> for air directly to PIV **152** (**FIG. 9A**) and bypassing reservoir bag **149**.

[**0155**] **FIG. 21A** shows examples of drug delivery management protocols for two-stage alarms responsive to system state monitors, namely, alarms "1" and "2," in accor-

dance with a preferred embodiment of one aspect of the invention. The alarms may have different tones or other indicators to note different levels of concern or criticality. The dataflow diagram of **FIG. 23A** depicts one example of the steps performed by the drug delivery managing software and/or logic for one such protocol, namely, one where electronic controller **14** (e.g., **FIG. 2A**) receives an electronic feedback value from an O<sub>2</sub> tank pressure sensor (**519**) indirectly measuring the amount of oxygen remaining in an on-board oxygen tank (the value indicated by "O<sub>2</sub> remaining"). As is shown, the O<sub>2</sub> remaining value is compared with an established data set of safe system parameters stored in a memory device as described above, said data set containing a "setpoint" reflecting known safe and undesirable oxygen tank pressure conditions (**520**). If the oxygen pressure is greater than the setpoint, no alarm sounds and no adjustment to drug delivery is effected (**521**). If the O<sub>2</sub>% value is less than the setpoint, alarm "1" sounds (**522**). If alarm "1" is silenced manually within 15 seconds, no further action is taken by the system (**523**). If alarm "1" is not silenced within 15 seconds, the amount of drug being delivered (in this example gaseous N<sub>2</sub>O) is reduced to the lesser of the concentration of 45% or the current concentration minus 10% (**524**). The software or logic procedure would operate in a similar fashion for intravenous and nebulized forms of drugs and the instructions provided (e.g., as in **524**), would be specified for safe dosages of such drugs.

[**0156**] In another example of **FIG. 21A** involving a system state monitor which indicates whether power is being supplied to apparatus **10**, a logic operation determines whether power has been interrupted. If the system state monitor for power signals that power has been interrupted, alarm "2" sounds and the delivery of drug is reduced to 0%.

[**0157**] Similar protocols are described in **FIG. 21A** for system state monitors indicating O<sub>2</sub> interruption fail safe, total gas flow, drug tank pressure, fraction of inspired oxygen (FIO<sub>2</sub>), and operation of the vacuum pump for scavenging system **48** (**FIG. 6**). These protocols are effected with software (and/or logic) operating in similar fashion to that described in the dataflow diagram of **FIG. 23A**. That is, the protocol shown in **FIG. 23A** is one example employing one system state monitor stored parameters, but the operation would be similar to effect the remaining protocols of **FIG. 21A**.

[**0158**] In the above examples, involving response to patient physiological state, there is a time lapse between the alarm's sounding and any decrease in drug delivery to the patient. In alternate protocols contemplated by the invention, electronic controller **14** will immediately cease or curtail drug administration upon the sounding of an alarm. For less critical ("yellow") alarms, drug delivery may be decreased to 80% levels upon the sounding of the alarm; for more critical ("red") alarms, drug delivery would cease upon the sounding of the alarm. In either case, the physician will then be given time, for example, thirty seconds, to instruct controller **14** to restart the drug delivery (e.g., the physician will need to override the curtailing of drug delivery). If the physician does override controller **14**, drugs are reinitiated, for example, by a bolus amount. This method prevents against a patient's deteriorating while a physician waits to respond to an alarm at current drug levels, and also avoids underdosing by permitting the physician sufficient time to reinitiate drug delivery.

[0159] Referring again to **FIGS. 2 and 18**, a printer **238** (**FIG. 2, 37**) provides an on-site hard copy of monitored patient health parameters (e.g., the feedback values from the one or more patient health monitors), as well as alarm states with time stamps indicating which type of alarms sounded, why and when. Diagnostic LEDs **240** affixed to the exterior of apparatus **10** (e.g., **FIG. 1**) and electronically coupled to controller **14** permit the physician typically involved in the procedure to ascertain system states at a glance; LEDs coupled to microprocessor controller **14** also permit service technicians to assess fault states.

[0160] A preferred embodiment of the invention includes a variety of peripheral electronic devices, one group internal to or integrated within housing **15** of apparatus **10** (e.g., **FIG. 1**) and a second group on-board electronic controller **14**. These electronic devices ensure proper operation of various aspects of system **10**, including providing hardware status feedback through sensors to ensure that the apparatus is operating within its desired parameters. **FIGS. 19A and 19B** describe various peripheral devices in accordance with the invention, such devices may be of a known, off-the-shelf types currently available. Specifically, internal solenoid-type activated door locks **190** restrict access to the interior of apparatus **10**. Door locks **190** are located within housing **15** (**FIG. 1**) and are electronically coupled to and controlled by controller **14** by means of software that includes protocols for password protection. Access to the interior of apparatus **10** is thus restricted to authorized personnel with passwords. This is intended to, among other things, minimize chances of "recreational" abuse of the pharmaceuticals (e.g.,  $N_2O$ ) contained therein. Internal door status sensors **191** located within housing **15** and electronically coupled to controller **14** generate signals indicating if an access door to the interior of apparatus **10** is open or closed. Real-time clock **192** on-board controller **14** enables said controller **14** to provide time stamps for overall system and patient activities and thereby enables creation of an accurate log of the operation of care system **10**. On-board ambient temperature sensor **193** monitors the exterior temperature signaling same to controller **14** which through software comparison type protocols confirms that apparatus **10** is being operated under desired conditions with respect to surrounding temperature. Internal battery temperature sensor **194** located within housing **15** and electronically coupled to controller **14** generates signals to same indicating whether the back-up battery power system is functioning correctly and not overcharging. Tilt sensor **195** located on-board controller **14** signals same if the apparatus **10** is being operated at an angle beyond its designed conditions.

[0161] In a preferred embodiment, the software control processes of electronic controller **14** are stored in a standard flash memory **196** and SRAM type battery-backed memory **197** stores system, patient and other status information in the event of an AC power loss. On-board fault detection processor (FDP) **198** signals failures to controller **14** and is a secondary microprocessor based computing system which relieves controller **14** of its control duties if a fault is detected in operation. On-board watch dog timer **199** indicates to controller **14** that the apparatus **10** is functioning and resets controller **14** if system **10** fails to respond.

[0162] A preferred embodiment of the invention also includes a standard serial port interface, such as an RS-232C serial port, for data transfer to and from electronic controller

**14**. The port enables, for example, downloading software upgrades to and transfer of system and patient log data from controller **14**. An interface such as a PC Type III slot is also provided to enable the addition of computer support devices to system **10**, such as modems or a LAN, to be used, for example, to transfer billing information to a remote site; or to permit diagnosis of problems remotely thereby minimizing the time required for trouble-shooting and accounting.

[0163] It should be understood that the care system of the invention may be modular in nature with its functions divided into separable, portable, plug-in type units. For example, electronic controller **14**, display devices (**FIG. 2, 35**) and one or more patient health monitors would be contained in one module, the pneumatic systems (flow controllers, pressure regulators, manifold) in a second module, and the base (**FIG. 3B, 17**), oxygen and drug tanks (**FIG. 2, 54**), scavenger system and vacuum pump (**FIG. 3B, 32**) in a third module. Additionally, the patient health monitors or drug delivery aspects of the system may each be their own plug-in type modules. The system, for example, may provide for a pluggable ventilator type module. This modularity enables the system not only to be more easily portable, but also enables use of certain features of the system (such as certain patient health monitors), while not requiring use of others.

[0164] **FIG. 20** depicts a preferred embodiment of a patient information and billing system capable of being interfaced with care system **10** (**FIG. 1**) to allow billing or other gathering of patient information to take place locally at the place of use or remotely at a billing office. Specifically, information/billing storage system **280**, which may be of a known type microprocessor-based computing system controlled by software, collects and stores patient data **281** such as the patient's name, address and other account information, as well as metered system operation data **282** generated during operation of apparatus **10** and stored in controller **14** such as start time, time of use, frequency of use, duration of patient monitoring, amount of gases expended, and other such parameters. User access device **283** which may be of a standard keyboard type permits the physician to interact with information/billing storage system **280** to input additional data such as pre-determined treatment or billing parameters or to read the status of same (e.g., to read the status of metered system operation parameters **282**). Preferably, a password is provided to permit access to information/billing system **280**.

[0165] At the termination of a medical or surgical procedure or at some other desired period, information/billing storage system **280** processes the received data and transmits same to revenue/billing processing center **286** at a remote location. Revenue/billing processing center **286** may be of a known, mainframe-type computing system such as that manufactured by International Business Machines (IBM) or a known client-server type computer network system. At the remote location a patient invoice is generated by printer **287** as may be other revenue records used for payment to vendors, etc.

[0166] The invention also contemplates that an automated record of the system operation details will be printed at the user site on printer **285** which is preferably located on-board apparatus **10** (**FIG. 1**). Such system operation details may include, for example, all alarm and actual system operation

states, drug flow rates and/or monitored actual patient physiological conditions as supplied by electronic controller 14. A modem or LAN may be used to send and receive billing and other information remotely and to communicate with remote client/server or other networks 288 as described above.

I claim:

1. A care system for alleviating patient pain, anxiety and discomfort associated with medical or surgical procedures said system comprising:

- a patient health monitor device coupled to a patient and generating a signal reflecting at least one physiological condition of the patient;
  - a drug delivery controller supplying one or more drugs to the patient;
  - a memory device storing a safety data set reflecting safe and undesirable parameters of at least one patient physiological condition;
  - an electronic controller interconnected between the patient health monitor, the drug delivery controller and the safety data set; wherein said electronic controller manages the application of the drugs in accord with the safety data set.
2. A care system as recited in claim 1 wherein said drugs are one or more sedatives, analgesics or amnestics.
3. A care system as recited in claim 1 wherein said drug is delivered in gaseous form.
4. A care system as recited in claim 1 wherein said system also includes airway circuitry providing a drug and oxygen mixture to the patient.
5. A care system as recited in claim 4 wherein said system also includes a scavenging vacuum pump which exhausts patient exhalations.
6. A care system as recited in claim 4 wherein said system also includes a disposable face mask coupled to said airway circuitry and engaging the patient's face.
7. A care system as recited in claim 6 wherein said face mask includes a mask base with a pliable outer edge and adhesive for sealingly engaging the patient's face and a quick release mechanism which allows rapid removal of the mask for emergency access to the patient's face.
8. A care system as recited in claim 6 wherein said face mask includes a monitoring device which monitors a patient's end tidal CO<sub>2</sub> levels in the patient's exhaled air stream.
9. A care system as recited in claim 6 wherein said face mask includes a monitoring device which monitors the acoustical levels of a patient's breathing.
10. A care system as recited in claim 6 wherein said face mask includes an airstream flow measurement device.
11. A care system as recited in claim 1 wherein said system includes means for delivering at least one of the drugs intravenously.
12. A care system as recited in claim 1 wherein said electronic controller includes logic for receiving the signal reflecting the at least one physiological condition and comparing said signal with the safety data set and managing the application of the drug to the patient in accord with the safety data set.
13. A care system as recited in claim 1 wherein said electronic controller is controlled by software which accesses the safety data set.

14. A care system as recited in claim 1 wherein said patient health monitor device comprises a pulse oximeter that monitors the oxygen level in the patient's blood.

15. A care system as recited in claim 14 wherein said system includes a second health monitor device coupled to a patient and generating values reflecting a second physiological condition of a patient; and wherein the safety data set also reflects safe and undesirable parameters of said second patient physiological condition and said electronic controller is interconnected with said second patient health monitor and manages application of the drug in accord with said safety data set.

16. A care system as recited in claim 15 wherein said second health monitor device comprises a capnometer that monitors the carbon dioxide level in the patient's inhaled and exhaled gases.

17. A care system as recited in claim 15 wherein said second health monitor device comprises an EKG device that monitors a patient's heart activity.

18. A care system as recited in claim 15 wherein said second health monitor device comprises an acoustical monitoring device that monitors the acoustical characteristics of a patient's inhaled and exhaled breaths.

19. A care system as recited in claim 1 wherein at least one of said drugs is propofol.

20. A care system as recited in claim 1 wherein at least one of said drugs is sevoflurane.

21. A care system as recited in claim 1 wherein at least one of said drugs is nitrous oxide.

22. A care system as recited in claim 1 wherein at least one of said drugs is a narcotic delivered as an intravenous infusion.

23. A care system as recited in claim 1 wherein at least one of said drugs is delivered as a nebulized aerosol to be inhaled.

24. A care system as recited in claim 1 wherein said system includes means for delivery of at least one of said drugs transdermally.

25. A care system as recited in claim 1 wherein at least one of said drugs is dexmedetomidine.

26. A care system as recited in claim 1 wherein at least one of said drugs is epibatidine.

27. A care system as recited in claim 15 wherein said second health monitor device is a patient consciousness monitor.

28. A care system as recited in claim 27 wherein said patient consciousness monitor includes an automated patient query and response system.

29. A care system as recited in claim 1 wherein said drug delivery controller comprises a patient-controlled drug dosage device coupled to the patient and interconnected to the electronic controller.

30. A care system as recited in claim 29 wherein said electronic controller is programmed with lock-out parameters that prevent activation of said patient-controlled drug dosage device.

31. A care system as recited in claim 1 wherein said system includes at least one alarm device that sounds when said signal is determined to fall within said undesirable parameters of said safety data set.

32. A care system as recited in claim 31 wherein said electronic controller curtails drug delivery upon the sounding of said alarm device.

**33.** A care system as recited in claim 31 wherein said electronic controller increases the delivery of oxygen to the patient upon the sounding of said alarm device.

**34.** A care system as recited in claim 4 wherein said system includes a LIFO oxygen delivery mechanism.

**35.** A care system according to claim 31, wherein said system also includes a display device with an alarm box portion which displays a representation of the patient physiological condition associated with the sounded alarm in that alarm box portion.

**36.** A care system as recited in claim 1 wherein said apparatus includes a display device showing data reflecting predicted concentration levels of drugs.

**37.** A care system as recited in claim 14 wherein activation of said first and second monitors are synchronized with one another.

**38.** A care system as recited in claim 1 wherein said system includes a display device showing data reflecting the patient's A-a gradient.

**39.** A care system as recited in claim 1 wherein said system includes a display device having portions showing patient physiological parameters and wherein said portions are color coded.

**40.** A care system for facilitating a nonanesthetist's safely and efficaciously providing conscious sedation to a patient undergoing a medical or surgical procedure, said system comprising:

- a patient health monitor device coupled to a patient and generating a value reflecting at least one physiological condition of the patient;
- a drug delivery controller supplying one or more drugs to a patient;
- a means for monitoring the consciousness of the patient coupled to the patient and generating a value representing the level of patient consciousness;
- a memory device storing a safety data set reflecting safe and undesirable parameters of at least one patient physiological condition and of patient consciousness level;
- an electronic controller interconnected between the patient health monitor, the drug delivery controller, and the safety data set; wherein said electronic controller manages application of the drugs to the patient in accord with the safety data set.

**41.** A method for alleviating pain and anxiety in connection with medical and surgical procedures, said method comprising the steps of:

- a) connecting to a patient a drug delivery device having a drug delivery controller supplying one or more drugs, said drug delivery controller being coupled to an electronic controller which controls the delivery of the drugs to the patient;
- b) attaching at least one patient health monitor device to a patient, which health monitor device generates a value reflecting at least one physiological condition of a patient and is coupled to said electronic controller;
- c) accessing a memory device which stores a safety data set reflecting parameters of at least one patient physiological condition;

d) delivering the drugs to the patient in accord with the safety data set.

**42.** A method as recited in claim 41 in which said drug delivery device is a patient-controlled drug dosage device.

**43.** A method as recited in claim 41, wherein the method also includes the step of performing an automated assessment of the patient's physiological state.

**44.** A method as recited in claim 43, wherein the automated assessment is performed pre-operatively.

**45.** A method as recited in claim 44 in which the pre-op assessment includes determining a patient sedation threshold limit.

**46.** A method as recited in claim 43 in which the electronic controller manages drug delivery in accord with the automated assessment.

**47.** A method as recited in claim 41 in which the drug is propofol.

**48.** A method as recited in claim 41 in which the drug is sevoflurane.

**49.** A method as recited in claim 41 in which the delivering of the drugs step is accomplished by target-controlled infusion.

**50.** A method as recited in claim 49 in which the drug is initially delivered in an amount overshooting a steady state target drug level.

**51.** A method as recited in claim 41 in which the patient health monitor device is a pulse oximeter and the application of drug is managed in accord with the oxygen level of the patient's blood.

**52.** An apparatus for delivering drugs to a conscious patient, said apparatus comprising:

- a drug delivery controller delivering a drug to a patient;
- an electronic controller connected to the drug delivery controller for varying the rate of delivery of drug to a patient;
- an automated consciousness monitoring system which ensures the consciousness of a patient and generates a signal reflecting the consciousness level of a patient; and wherein said electronic controller is capable of varying the delivery of drug to the patient in accord with said signal.

**53.** An apparatus as recited in claim 52 wherein said automated consciousness monitoring system comprises a stimulator device which commands a patient; and a response device for activation by the patient in response to the stimulator device; said response device generating signals having values reflecting the time it takes for the patient to activate the response device in response to the stimulator device, and providing said signals to and to the electronic controller.

**54.** An apparatus as recited in claim 53 wherein said stimulator device has multiple urgency or intensity levels.

**55.** An apparatus as recited in claim 53 in which the stimulator device comprises a speaker that provides an auditory instruction to a patient.

**56.** An apparatus as recited in claim 53 in which the stimulator device comprises a vibrator.

**57.** An apparatus as recited in claim 53 wherein the stimulator device is located in close proximity to the response device.

**58.** An apparatus as recited in claim 52, wherein said apparatus also includes at least one patient health monitor

device which generates a signal reflecting at least one physiological condition of a patient.

**59.** An apparatus as recited in claim 42 wherein said drug delivery controller comprises a patient-controlled drug administration device.

**60.** An apparatus as recited in claim 42 wherein said apparatus also includes a display device displaying the value of the signal reflecting the consciousness level of the patient.

**61.** A method for relieving patient pain or anxiety, said method comprising the steps of:

- a) monitoring at least one physiological condition of a patient with at least one electronic health monitor device;
- b) electronically monitoring the level of consciousness of a patient; and
- c) electronically managing the delivery of pain or anxiety relieving drugs to a patient in accord with the at least one physiological condition of a patient and the level of consciousness of a patient.

**62.** A method as recited in claim 61 in which the electronic health monitor device is a pulse oximeter and the delivery of drugs is electronically managed in accord with the level of oxygen in the patient's blood.

**63.** A method as recited in claim 61 in which the monitoring of the level of consciousness of a patient further comprises the steps of:

- a) automatically commanding the attention of the patient with a stimulus;
- b) electronically receiving the patient's response to the stimulus;
- c) generating a signal having a value reflecting the level of consciousness of a patient as a function of the time it took for the patient to respond to the stimulus.

**64.** A method as recited in claim 61 in which the delivery of drugs is accomplished through target controlled intravenous infusion.

**65.** A method as recited in claim 61 in which the delivery of drugs is accomplished by a patient-controlled drug delivery device.

**66.** An integrated patient interface apparatus for use with a drug delivery and patient monitoring system, said system including an electronic controller which electronically manages the delivery of drugs to a patient, said patient interface apparatus comprising:

- a portion for receiving a patient's hand;
- a patient-controlled drug dosage request device integrated into said portion and having a movable member capable of being activated by the patient to request a change in dosage of drug; and wherein said drug dosage request device is electronically coupled to said electronic controller; and
- a patient health monitor device electronically coupled to said electronic controller.

**67.** An apparatus as recited in claim 66 in which said patient health monitor is a consciousness monitor.

**68.** An apparatus as recited in claim 66 in which said patient health monitor is a pulse oximeter.

**69.** An apparatus as recited in claim 66 which also includes a patient response device integrated into said hand cradle and having a movable member capable of being

activated by a patient in response to a stimulus; and wherein said patient response device is electronically coupled to said electronic controller and produces a value reflecting the level of consciousness of the patient, providing said value to said electronic controller.

**70.** An apparatus as recited in claim 68 wherein said pulse oximeter is mounted on said portion for receiving the patient's hand.

**71.** An apparatus as recited in claim 66, wherein said patient health monitor includes a blood pressure monitor mounted on said portion for receiving a patient's hand and removably attachable to the patient.

**72.** An apparatus as recited in claim 66 wherein said patient health monitor includes a blood pressure cuff.

**73.** A method for electronically tracking recurring revenues generated by use of a conscious sedation care system at the location of the user, said method comprising the steps of:

- a) providing a medical apparatus at the location of the user, said apparatus having a user access device, and a memory device storing data representing metered system operation values and patient informational data;
- b) providing a password to said apparatus enabling access to said memory device;
- c) reading said metered system operation values and patient informational data and transmitting said values and data to a remote location;
- d) calculating a revenue based on said system operation values; and
- e) providing a record at the remote location reflecting said revenue and patient informational data.

**74.** A method as recited in claim 73 wherein said method includes the step of printing a record of said revenues at the remote location.

**75.** A method as recited in claim 73 wherein said method includes the step of printing a patient invoice at the remote location.

**76.** A method as recited in claim 73 wherein said medical apparatus includes a printer providing an automated record of said system operation values and patient informational data at the location of the user.

**77.** An apparatus as recited in claim 52, wherein said apparatus further includes an attention-commanding device which receives said signal reflecting the consciousness level of the patient and notifies the nonanesthetist in the event said consciousness level changes to a level outside an acceptable range.

**78.** An apparatus as recited in claim 77 wherein said attention-commanding device is an audible alarm.

**79.** An apparatus as recited in claim 77 wherein said apparatus further includes a display device which displays the value reflecting the consciousness level of the patient upon the activation of said attention-commanding device and visually displays an action to be taken by said electronic controller in the event said consciousness level is outside of an acceptable range.

**80.** A care system as recited in claim 4 wherein said drug and oxygen mixture is provided to the patient in accord with the respiratory rate of the patient.

**81.** A care system as recited in claim 4 wherein said drug and oxygen mixture is provided to the patient in accord with the effective minute ventilation of the patient.

**82.** An apparatus as recited in claim 35 wherein said display device is a heads-up type device mounted on a support and capable of being viewed by the practitioner at eye level.

**83.** An apparatus as recited in claim 66 wherein said patient health monitor is a pulse oximeter mounted on an earpiece removably attachable to the patient.

**84.** A care system as recited in claim 2 wherein said system includes at least one drug dosage container mounted on said apparatus containing at least one dosage of drug capable of reversing the effect of the one or more sedatives, analgesics or anesthetics delivered to the patient.

**85.** A care system for alleviating pain or discomfort in a conscious patient while simultaneously enabling safe patient control of said pain or discomfort, said apparatus comprising:

- a patient health monitor device coupled to the patient and generating a value reflecting at least one physiological condition of the patient;
- a memory device storing a safety data set reflecting parameters of the at least one patient physiological condition;
- a patient-controlled drug dosage request device which generates a signal indicating the patient's request for an adjustment in drug dosage and having a drug delivery controller;
- an electronic controller interconnected between the patient health monitor, the patient-controlled drug dosage increase/decrease request device, and the safety data set; wherein said electronic controller manages the application of the drugs in accord with the safety data set.

**86.** A care system as recited in claim 85 wherein said memory device also stores programmed parameters indicating desired drug dosages;

**87.** An apparatus as recited in claim 85 wherein said patient health monitor device is a pulse oximeter.

**88.** A care system as recited in claim 85 wherein said safety data set reflects safe and undesirable of at least one

patient physiological condition, and said electronic controller manages the application of the drugs in response to said signal generated by patient-controlled drug dosage request device in accord with the stored parameters in said memory device.

**89.** An apparatus as recited in claim 85 wherein said electronic controller is programmed with lock-out parameters that prevent patient self-administration of drugs at specified levels of drugs.

**90.** An apparatus as recited in claim 85 wherein said electronic controller is programmed with lock-out parameters that prevent patient self-administration of drugs at specified rates of changes in drug levels.

**91.** An apparatus as recited in claim 88 wherein said apparatus includes at least one attention commanding device which activates when said patient physiological condition value falls within the undesirable range of said safety data set.

**92.** A care system as recited in claim 1 wherein said system includes at least one system state monitor which generates a signal reflecting the state of at least one operating condition of the system and which is coupled to the electronic controller; and wherein said safety data set also reflects safe and undesirable parameters of at least one operating condition of the apparatus.

**93.** A care system as recited in claim 92 wherein said system state monitor is an oxygen source pressure sensor that measures the flow of oxygen to the patient.

**94.** A care system as recited in claim 92 wherein said system state monitor indicates whether there has been a power failure in the system.

**95.** A care system as recited in claim 92 wherein said electronic controller activates an attention-commanding device in response to said signal reflecting the state of at least one operating condition of the apparatus.

**96.** A care system as recited in claim 92 wherein said system state monitor is a drug source flow sensor that measures flow of drug to the patient.

\* \* \* \* \*

|                |                                                                                                                                                                                                                                                                                                                                                                                                           |         |            |
|----------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 用于提供有意识的患者免于与医疗或外科手术相关的疼痛和焦虑的装置和方法                                                                                                                                                                                                                                                                                                                                                                        |         |            |
| 公开(公告)号        | <a href="#">US20020017299A1</a>                                                                                                                                                                                                                                                                                                                                                                           | 公开(公告)日 | 2002-02-14 |
| 申请号            | US09/909782                                                                                                                                                                                                                                                                                                                                                                                               | 申请日     | 2001-07-23 |
| [标]申请(专利权)人(译) | HICKLE RANDALL 小号                                                                                                                                                                                                                                                                                                                                                                                         |         |            |
| 申请(专利权)人(译)    | HICKLE RANDALL S.                                                                                                                                                                                                                                                                                                                                                                                         |         |            |
| 当前申请(专利权)人(译)  | HICKLE RANDALL S.                                                                                                                                                                                                                                                                                                                                                                                         |         |            |
| [标]发明人         | HICKLE RANDALL S                                                                                                                                                                                                                                                                                                                                                                                          |         |            |
| 发明人            | HICKLE, RANDALL S.                                                                                                                                                                                                                                                                                                                                                                                        |         |            |
| IPC分类号         | A61B5/00 A61B5/11 A61B5/145 A61B5/16 A61B19/00 A61G12/00 A61K9/22 A61M5/00 A61M16/00 A61M16/01 A61M21/02 G06F19/00 G06Q50/22 G06Q50/24 G16H10/60 A61N1/30 A61M15/00 A61M16/10 A62B7/00 F16K31/02 A62B18/02                                                                                                                                                                                                |         |            |
| CPC分类号         | A61B5/1106 Y10T428/24355 A61B5/417 A61B5/4821 A61M16/0051 A61M16/0078 A61M16/009 A61M16/01 A61M2016/0036 A61M2205/3561 A61M2209/084 A61M2230/205 A61M2230/43 A61M2230/432 G06Q50/22 G06Q50/24 G06F19/3468 A61M16/0084 A61M19/00 A61M2205/18 A61M2205/276 A61M2205/3303 A61M2205/3379 A61B5/162 A61M16/0093 A61M16/026 A61M16/1015 A61M16/107 A61M2016/0027 A61M2016/1025 A61M2205/505 G16H20/17 G16H40/63 |         |            |
| 优先权            | 60/087841 1998-06-03 US                                                                                                                                                                                                                                                                                                                                                                                   |         |            |
| 其他公开文献         | US6986347                                                                                                                                                                                                                                                                                                                                                                                                 |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>                                                                                                                                                                                                                                                                                                                                                           |         |            |

# 摘要(译)

提供护理系统和相关方法，用于减轻与医疗或外科手术相关的患者疼痛，焦虑和不适。该系统包括：至少一个患者健康监测装置，其产生反映患者的至少一种生理状况的信号；药物输送控制器向患者提供一种或多种药物；存储装置，存储反映至少一个患者生理状况参数的安全数据集；以及在患者健康监测器，药物输送控制器和安全数据集之间互连的电子控制器。还提供了一种电子跟踪由使用护理系统产生的经常性收入的方法，其中系统位于其用户的位置。该系统和方法的另外的实施方案涉及减轻患者疼痛或不适，同时与患者健康状况的监测相关联地实现安全的患者控制的药物递送。

