



US008932217B2

(12) **United States Patent**
Gibson et al.

(10) **Patent No.:** **US 8,932,217 B2**
(45) **Date of Patent:** **Jan. 13, 2015**

(54) **VITAL SIGNS MONITOR**

(75) Inventors: **Grant S. Gibson**, Portland, OR (US);
Cory R. Gondek, Tigard, OR (US);
Richard A. Sunderland, Aloha, OR
(US); **Steven D. Baker**, Beaverton, OR
(US); **Robert T. Lewis**, Beaverton, OR
(US); **Braxton L. Lathrop**, Lake
Oswego, OR (US); **Christopher L.**
Dunn, Lake Oswego, OR (US); **Omer**
Kotzer, Portland, OR (US)

(73) Assignee: **Welch Allyn, Inc.**, Skaneateles Falls, NY
(US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 1700 days.

(21) Appl. No.: **11/795,301**

(22) PCT Filed: **Jan. 13, 2006**

(86) PCT No.: **PCT/US2006/001093**

§ 371 (c)(1),

(2), (4) Date: **Apr. 10, 2008**

(87) PCT Pub. No.: **WO2006/076498**

PCT Pub. Date: **Jul. 20, 2006**

(65) **Prior Publication Data**

US 2008/0281168 A1 Nov. 13, 2008

Related U.S. Application Data

(60) Provisional application No. 60/643,636, filed on Jan.
13, 2005.

(51) **Int. Cl.**

G06F 19/00 (2011.01)

A61B 5/00 (2006.01)

A61B 5/024 (2006.01)

A61B 5/0205 (2006.01)

A61B 5/0424 (2006.01)

A61B 5/1455 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/02438** (2013.01); **G06F 19/3406**
(2013.01); **A61B 5/7275** (2013.01); **A61B**

5/746 (2013.01); **A61B 5/0205** (2013.01);
A61B 5/0424 (2013.01); **A61B 5/14551**
(2013.01); **A61B 5/6843** (2013.01); **A61B**
5/6887 (2013.01); **A61B 5/742** (2013.01);
A61B 5/7475 (2013.01); **A61B 5/002**
(2013.01); **A61B 5/0022** (2013.01); **A61B**
2560/0276 (2013.01); **A61B 2560/0456**
(2013.01)

USPC **600/301**; **600/300**

(58) **Field of Classification Search**

None

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,996,928 A	12/1976	Marx
4,026,278 A	5/1977	Ricketts et al.
4,051,522 A	9/1977	Healy et al.
4,090,505 A	5/1978	Mortara
4,121,574 A	10/1978	Lester
4,129,125 A	12/1978	Lester et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO9625877 A1 * 8/1996 A61B 5/0404

OTHER PUBLICATIONS

Extended European Search Report for EP Application No. 06 718
193.3; Mailed Jul. 29, 2009; 8 pages.

Primary Examiner — William Thomson


Assistant Examiner — Davin K Sands

(74) *Attorney, Agent, or Firm* — Hiscock & Barclay, LLP

(57) **ABSTRACT**

A multi-parametric vital signs monitoring device configured for use as an ambulatory and a bedside monitor wherein the device can be patient-wearable and is battery powered. The monitoring device can be used with a charging cradle to provide power to the device in lieu of the battery as a power source for bedside applications, in which the cradle further serves as an intermediary device to enable a data link with a PC or other peripheral device. The monitoring device can include a wireless radio to enable bi-directional transfer of patient-related data to a separate remote station.

18 Claims, 35 Drawing Sheets

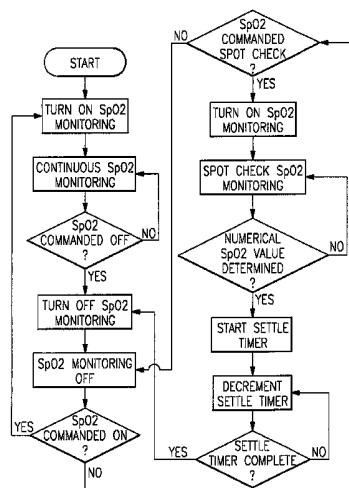

(56)

References Cited

U.S. PATENT DOCUMENTS

4,270,547 A	6/1981	Steffen et al.	5,566,676 A	10/1996	Rosenfeldt et al.
4,276,888 A	7/1981	Smith et al.	5,573,012 A	11/1996	McEwan et al.
4,308,870 A	1/1982	Arkans	5,579,001 A	11/1996	Dempsey et al.
4,347,851 A	9/1982	Jundanian	5,579,775 A *	12/1996	Dempsey et al. 600/483
4,383,534 A	5/1983	Peters	5,594,786 A	1/1997	Chaco et al.
4,411,267 A	10/1983	Heyman	5,600,108 A	2/1997	Newham
4,494,553 A	1/1985	Sciarra et al.	5,614,887 A	3/1997	Buchbinder
4,522,213 A	6/1985	Wallroth et al.	5,633,910 A	5/1997	Cohen
4,526,176 A	7/1985	Bremer et al.	5,640,953 A	6/1997	Bishop et al.
4,583,553 A	4/1986	Shah et al.	5,649,535 A	7/1997	Voith
4,705,048 A	11/1987	Pfohl	5,650,770 A	7/1997	Schlager et al.
4,712,562 A	12/1987	Ohayon et al.	5,662,105 A	9/1997	Tien
4,715,385 A	12/1987	Cudahy et al.	5,664,270 A	9/1997	Bell et al.
4,724,844 A	2/1988	Rafelson	5,666,958 A	9/1997	Rothenberg et al.
4,803,625 A	2/1989	Fu et al.	5,685,314 A	11/1997	Geheb et al.
4,827,943 A	5/1989	Bornn et al.	5,687,717 A	11/1997	Halpern et al.
4,835,372 A	5/1989	Gombrich et al.	5,687,734 A	11/1997	Dempsey et al.
4,852,571 A	8/1989	Gadsby	5,689,229 A	11/1997	Chaco et al.
4,860,759 A	8/1989	Kahn et al.	5,689,242 A	11/1997	Sims et al.
4,889,131 A	12/1989	Salem et al.	5,704,364 A	1/1998	Saltzstein et al.
4,889,132 A	12/1989	Hutcheson et al.	5,713,350 A	2/1998	Yokota et al.
4,889,839 A	12/1989	Chu et al.	5,715,451 A	2/1998	Marlin
4,895,161 A	1/1990	Cudahy et al.	D393,072 S	3/1998	Rogler
4,909,260 A	3/1990	Salem et al.	5,724,025 A	3/1998	Tavori
4,916,441 A	4/1990	Gombrich	5,732,074 A	3/1998	Spaur et al.
4,951,678 A	8/1990	Joseph et al.	5,740,001 A	4/1998	Flachslaender et al.
4,958,636 A	9/1990	Blandino et al.	5,746,697 A *	5/1998	Swedlow et al. 600/323
4,958,638 A	9/1990	Sharpe et al.	5,748,103 A	5/1998	Flach et al.
4,981,139 A	1/1991	Pfohl	5,749,374 A	5/1998	Schneider, Sr.
5,003,984 A	4/1991	Muraki et al.	5,749,907 A	5/1998	Mann
5,010,890 A	4/1991	Pfohl et al.	5,752,917 A	5/1998	Fuchs
5,022,404 A	6/1991	Hafner	5,766,208 A	6/1998	McEwan
5,025,808 A	6/1991	Hafner	5,767,791 A	6/1998	Stoop et al.
5,036,869 A	8/1991	Inahara	5,785,650 A	7/1998	Akasaka et al.
5,038,800 A	8/1991	Oba	5,788,644 A *	8/1998	Donehoo et al. 600/509
5,131,399 A	7/1992	Sciarra	5,801,755 A	9/1998	Echerer
D328,645 S	8/1992	Rogler et al.	5,819,741 A	10/1998	Karlsson et al.
5,140,519 A	8/1992	Friesdorf et al.	5,822,544 A	10/1998	Chaco et al.
5,181,521 A	1/1993	Lemelson	5,827,180 A	10/1998	Goodman
5,187,641 A	2/1993	Muskatello et al.	5,832,448 A	11/1998	Brown
5,188,108 A	2/1993	Secker et al.	5,840,036 A	11/1998	Voith
5,205,294 A	4/1993	Flach et al.	5,855,550 A	1/1999	Lai et al.
5,215,087 A	6/1993	Anderson et al.	5,860,176 A	1/1999	Norberg
5,285,783 A	2/1994	Secker et al.	5,865,733 A	2/1999	Malinouskas
5,285,784 A	2/1994	Seeker	5,867,688 A	2/1999	Simmon et al.
5,285,792 A	2/1994	Sjoquist et al.	5,882,300 A	3/1999	Malinouskas et al.
5,309,908 A	5/1994	Friedman et al.	5,902,234 A	5/1999	Webb
5,319,363 A	6/1994	Welch et al.	5,907,291 A	5/1999	Chen et al.
5,331,549 A	7/1994	Crawford, Jr.	5,919,141 A	7/1999	Money et al.
5,333,617 A	8/1994	Hafner	5,924,074 A	7/1999	Evans
5,339,810 A	8/1994	Ivers et al.	5,924,979 A	7/1999	Swedlow et al.
5,343,869 A	9/1994	Pross et al.	5,931,791 A	8/1999	Saltzstein et al.
5,355,893 A	10/1994	Mick et al.	5,936,539 A	8/1999	Fuchs
5,361,755 A	11/1994	Schraag et al.	5,944,659 A	8/1999	Flach et al.
5,375,604 A	12/1994	Kelly et al.	5,947,907 A	9/1999	Duich
5,396,224 A	3/1995	Dukes et al.	5,959,611 A	9/1999	Smailagic et al.
5,410,471 A	4/1995	Alyfuku et al.	5,961,446 A	10/1999	Beller et al.
D357,982 S	5/1995	Dahl et al.	5,967,993 A	10/1999	Maruyama et al.
5,413,099 A	5/1995	Schmidt et al.	6,004,312 A	12/1999	Finneran et al.
5,413,102 A	5/1995	Schmidt et al.	6,005,658 A *	12/1999	Kaluza et al. 356/39
5,417,222 A	5/1995	Dempsey et al.	6,011,989 A	1/2000	Sugo et al.
5,446,548 A	8/1995	Gerig et al.	6,016,445 A	1/2000	Baura
5,456,261 A	10/1995	Luczyk	6,021,351 A	2/2000	Kadhiresan et al.
5,458,123 A	10/1995	Unger	6,049,731 A	4/2000	Ochiai et al.
5,458,124 A	10/1995	Stanko et al.	6,057,758 A	5/2000	Dempsey et al.
5,469,844 A	11/1995	Rogler	6,062,902 A	5/2000	Buckles et al.
5,473,536 A	12/1995	Wimmer	6,067,462 A	5/2000	Diab et al.
5,494,051 A	2/1996	Schneider, Sr.	6,077,082 A	6/2000	Gibson et al.
5,513,406 A	5/1996	Foster et al.	6,083,156 A	7/2000	Lisiecki
5,526,287 A	6/1996	French	6,083,171 A	7/2000	Ono et al.
5,529,073 A	6/1996	Kielbasiewicz	6,093,146 A	7/2000	Filangeri
5,537,289 A	7/1996	Dahl	6,102,856 A	8/2000	Groff et al.
5,544,661 A	8/1996	Davis et al.	6,104,941 A	8/2000	Huey et al.
5,553,113 A	9/1996	Weedon	6,106,457 A	8/2000	Perkins et al.
5,558,638 A	9/1996	Evers et al.	6,122,543 A	9/2000	Ochiai et al.
			6,150,951 A	11/2000	Olejniczak
			6,157,855 A	12/2000	Sjöholm
			6,157,935 A	12/2000	Tran et al.
			6,160,478 A	12/2000	Jacobsen et al.


(56)

References Cited

U.S. PATENT DOCUMENTS

6,161,036	A	12/2000	Matsumura et al.	6,551,252	B2	4/2003	Sackner et al.
6,167,258	A	12/2000	Schmidt et al.	6,556,630	B1	4/2003	Brinsfield et al.
6,171,237	B1	1/2001	Avitall et al.	6,558,321	B1	5/2003	Burd et al.
6,176,826	B1	1/2001	Shimura et al.	6,572,545	B2	6/2003	Knobbe et al.
6,183,417	B1	2/2001	Geheb et al.	6,575,905	B2	6/2003	Knobbe et al.
6,185,454	B1	2/2001	Thompson	6,577,901	B2	6/2003	Thompson
6,185,460	B1	2/2001	Thompson	6,579,231	B1	6/2003	Phipps
6,188,407	B1	2/2001	Smith et al.	6,579,232	B2	6/2003	Sakamaki et al.
6,198,390	B1	3/2001	Schlager et al.	6,579,242	B2	6/2003	Bui et al.
6,198,394	B1	3/2001	Jacobsen et al.	6,584,336	B1	6/2003	Ali et al.
6,206,829	B1	3/2001	Iliff	6,585,645	B2	7/2003	Hutchinson
6,210,301	B1	4/2001	Abraham-Fuchs et al.	6,589,170	B1	7/2003	Flach et al.
6,213,942	B1	4/2001	Flach et al.	6,591,135	B2	7/2003	Palmer et al.
6,221,012	B1 *	4/2001	Maschke et al. 600/301	6,593,528	B2	7/2003	Franklin-Lees et al.
6,223,080	B1	4/2001	Thompson	6,594,146	B2	7/2003	Frangesch et al.
6,224,549	B1	5/2001	Drongelen	6,595,918	B2	7/2003	Gopinathan et al.
6,234,964	B1	5/2001	Iliff	6,595,929	B2	7/2003	Stivoric et al.
6,241,682	B1	6/2001	Ochiai et al.	6,600,421	B2	7/2003	Freeman
6,246,992	B1	6/2001	Brown	6,602,191	B2	8/2003	Quy
6,247,674	B1	6/2001	Jawidzik	6,610,010	B2	8/2003	Sjöqvist
6,248,064	B1	6/2001	Gopinathan et al.	6,611,705	B2	8/2003	Hopman et al.
6,252,531	B1	6/2001	Gordon et al.	6,616,598	B2	9/2003	Kaushansky et al.
6,259,355	B1	7/2001	Chaco et al.	6,616,606	B1	9/2003	Petersen et al.
6,259,944	B1	7/2001	Margulis et al.	6,616,613	B1	9/2003	Goodman
6,263,222	B1	7/2001	Diab et al.	6,629,937	B2	10/2003	Watrous
6,263,235	B1	7/2001	Kaiser et al.	6,631,281	B1	10/2003	Kästle
6,267,722	B1	7/2001	Anderson et al.	6,638,218	B2	10/2003	Bulat
6,267,723	B1	7/2001	Matsumura et al.	6,640,145	B2	10/2003	Hoffberg et al.
6,282,440	B1	8/2001	Brodnick et al.	6,641,533	B2 *	11/2003	Causey et al. 600/300
6,287,252	B1	9/2001	Lugo	6,647,280	B2	11/2003	Bahr et al.
6,309,342	B1	10/2001	Blazey et al.	6,647,287	B1	11/2003	Peel, III et al.
6,319,200	B1	11/2001	Lai et al.	6,648,820	B1	11/2003	Screl
6,322,502	B1	11/2001	Schoenberg et al.	6,656,125	B2	12/2003	Mischynski et al.
6,336,900	B1	1/2002	Alleckson et al.	6,657,976	B1	12/2003	Larghi
6,339,715	B1	1/2002	Bahr et al.	6,661,379	B2	12/2003	Stilp et al.
6,352,504	B1	3/2002	Ise et al.	6,669,630	B1	12/2003	Joliat et al.
6,353,445	B1	3/2002	Babula et al.	6,671,563	B1	12/2003	Engelson et al.
6,364,834	B1	4/2002	Reuss et al.	6,676,600	B1	1/2004	Conero et al.
6,370,423	B1	4/2002	Guerrero et al.	6,705,990	B1	3/2004	Gallant et al.
6,375,614	B1	4/2002	Braun et al.	6,716,165	B1	4/2004	Flanders et al.
6,377,223	B1	4/2002	Clapp et al.	6,721,178	B1	4/2004	Clark et al.
6,389,308	B1	5/2002	Shusterman	6,723,045	B2	4/2004	Cosentino et al.
6,394,952	B1	5/2002	Anderson et al.	6,726,634	B2	4/2004	Freeman
6,398,727	B1	6/2002	Bui et al.	6,731,989	B2	5/2004	Engleson et al.
6,401,138	B1	6/2002	Judge et al.	6,733,447	B2	5/2004	Lai et al.
6,402,691	B1	6/2002	Peddico et al.	6,733,464	B2	5/2004	Olbrich et al.
6,405,076	B1	6/2002	Taylor et al.	6,738,798	B1	5/2004	Ploetz et al.
6,405,083	B1	6/2002	Rockwell et al.	6,740,033	B1	5/2004	Olejniczak et al.
6,406,426	B1	6/2002	Reuss et al.	6,741,887	B1	5/2004	Gleeson
6,407,335	B1	6/2002	Franklin-Lees et al.	6,745,036	B1	6/2004	Dunne et al.
6,409,659	B1	6/2002	Warner et al.	6,746,403	B2	6/2004	Kolluri et al.
6,409,662	B1	6/2002	Lloyd et al.	6,749,566	B2	6/2004	Russ
6,412,980	B1	7/2002	Lounsbury et al.	6,751,650	B1	6/2004	Finch, II et al.
6,416,471	B1	7/2002	Kumar et al.	6,755,795	B2	6/2004	Marmaropoulos et al.
6,418,346	B1	7/2002	Nelson et al.	6,763,260	B2	7/2004	Kohls
6,434,572	B2	8/2002	Derzay et al.	6,770,028	B1 *	8/2004	Ali et al. 600/300
RE37,852	E	9/2002	Aso et al.	6,773,396	B2	8/2004	Flach et al.
6,454,708	B1	9/2002	Ferguson et al.	6,783,501	B2	8/2004	Takahashi et al.
6,454,718	B1	9/2002	Clift	6,790,178	B1	9/2004	Mault et al.
6,471,087	B1	10/2002	Shusterman	6,792,396	B2	9/2004	Inda et al.
6,491,647	B1	12/2002	Bridger et al.	6,795,688	B1	9/2004	Plasson et al.
6,493,220	B1	12/2002	Clark et al.	6,801,802	B2	10/2004	Sitzman et al.
6,493,568	B1	12/2002	Bell et al.	6,816,266	B2	11/2004	Varshneya et al.
6,505,067	B1	1/2003	Lee et al.	6,826,419	B2	11/2004	Diab et al.
6,516,073	B1	2/2003	Schulz et al.	6,870,484	B1	3/2005	Brinsfield et al.
6,520,073	B1	2/2003	Sorensen	6,896,661	B2	5/2005	Dekker
6,524,240	B1	2/2003	Thede	6,907,283	B2	6/2005	Carter et al.
6,537,214	B1	3/2003	Hood et al.	7,130,671	B2 *	10/2006	Baker et al. 600/310
6,537,225	B1	3/2003	Mills	2002/0013518	A1 *	1/2002	West et al. 600/300
6,539,249	B1	3/2003	Kadhiresan et al.	2002/0072660	A1 *	6/2002	Diab et al. 600/323
6,540,673	B2	4/2003	Gopinathan	2002/0137995	A1 *	9/2002	Heckel 600/323
6,544,173	B2	4/2003	West et al.	2003/0055309	A1	3/2003	Kaushansky et al.
6,544,174	B2	4/2003	West et al.	2003/0139656	A1 *	7/2003	Kiani et al. 600/322
6,547,740	B2	4/2003	Sugo et al.	2003/0236100	A1 *	12/2003	Fujieda et al. 455/550.1
6,551,243	B2	4/2003	Bocionek et al.	2004/0147818	A1 *	7/2004	Levy et al. 600/300
				2004/0186357	A1	9/2004	Soderberg et al.
				2005/0065417	A1 *	3/2005	Ali et al. 600/323
				2005/0197586	A1 *	9/2005	Pearlman 600/509

* cited by examiner

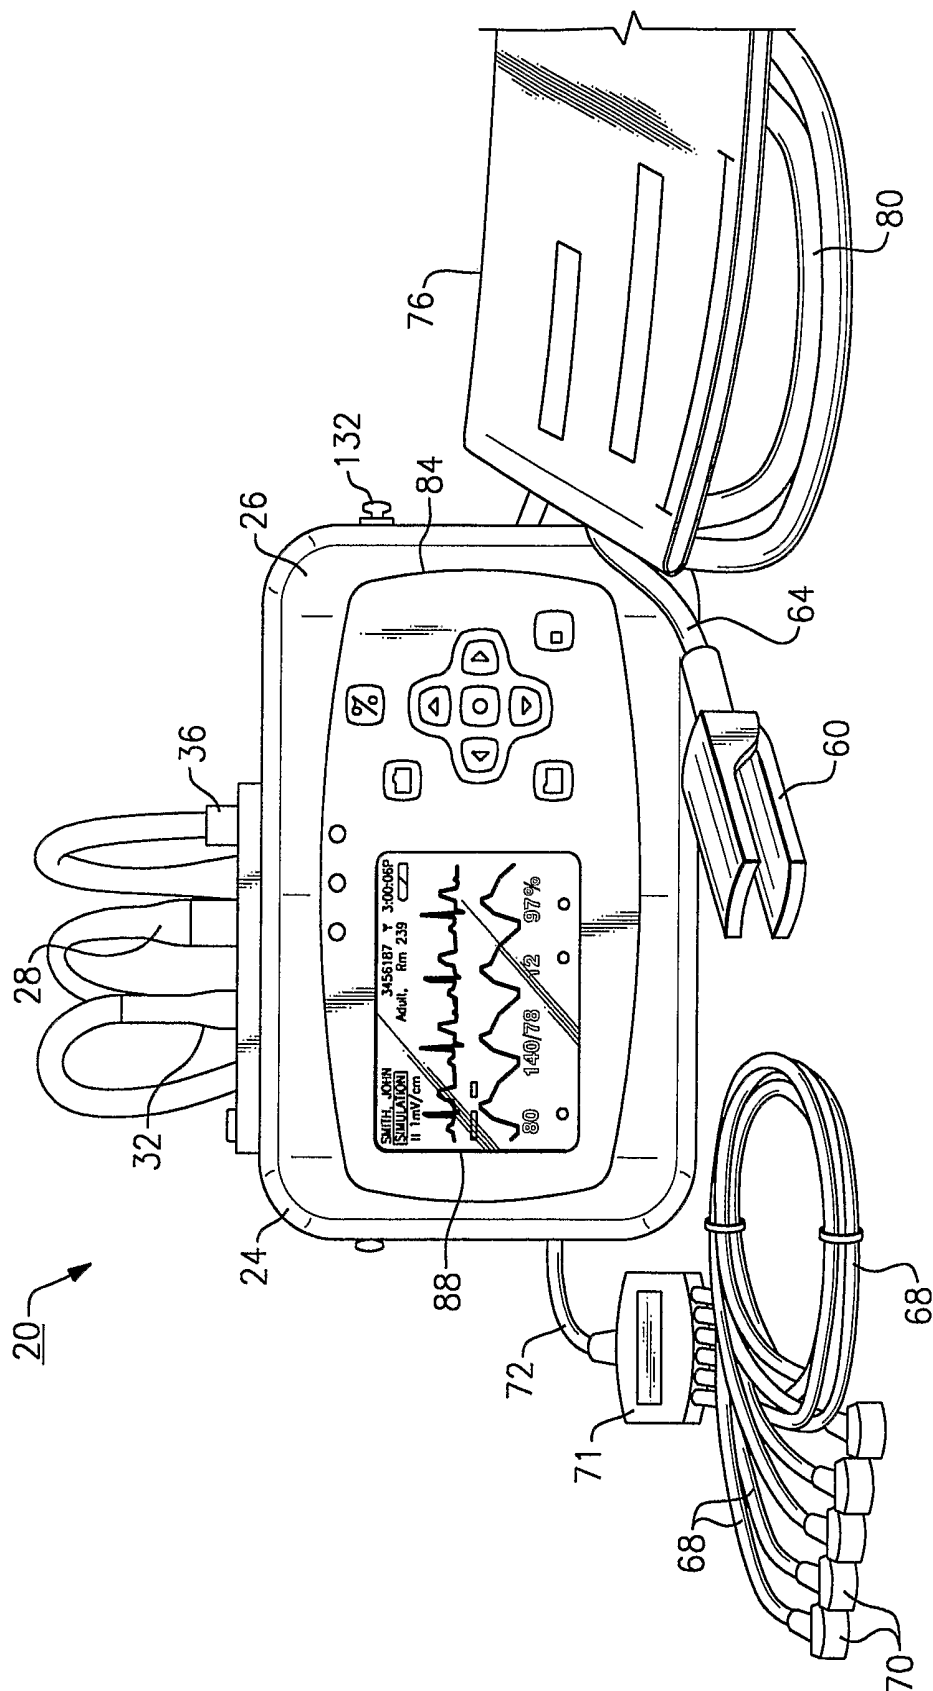

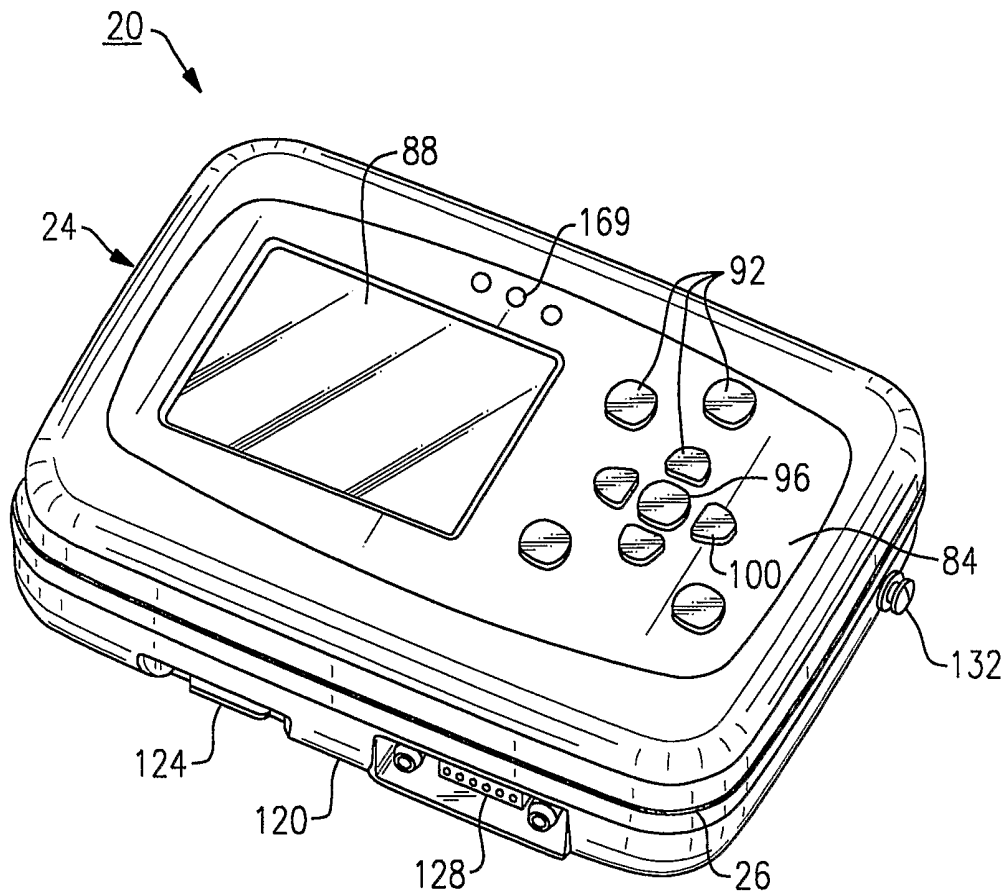


FIG. 2

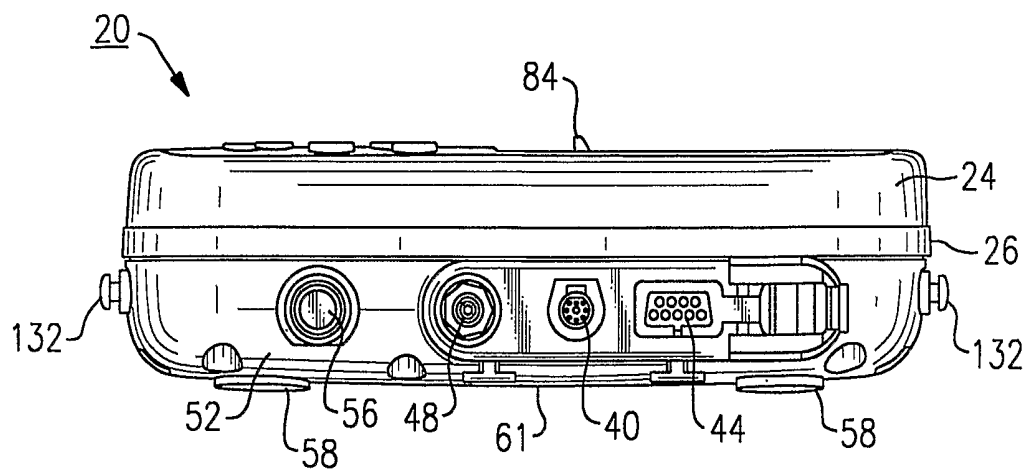
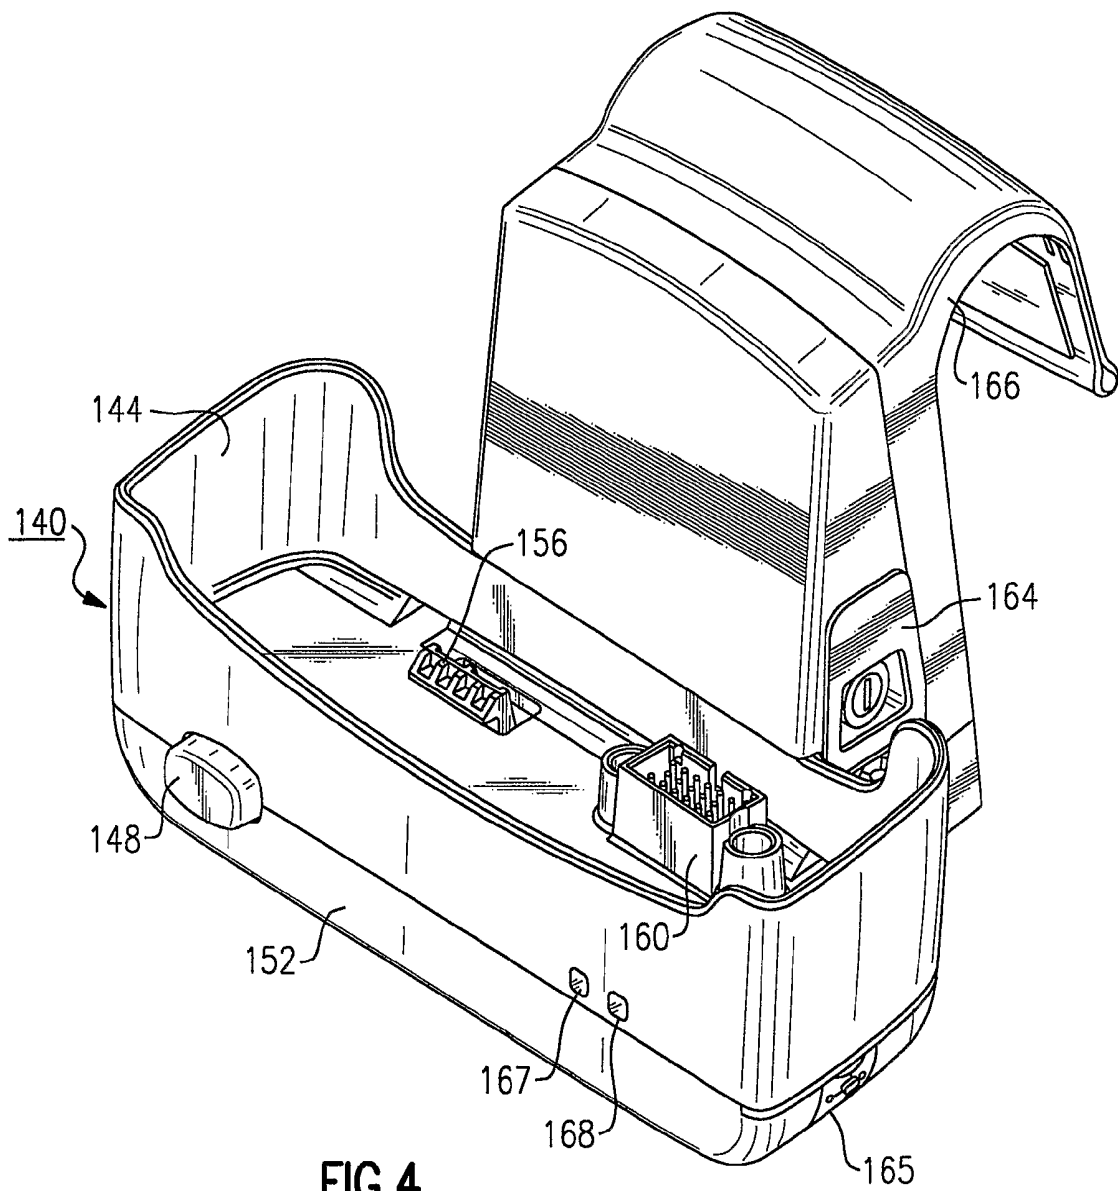


FIG. 3

**FIG. 4**

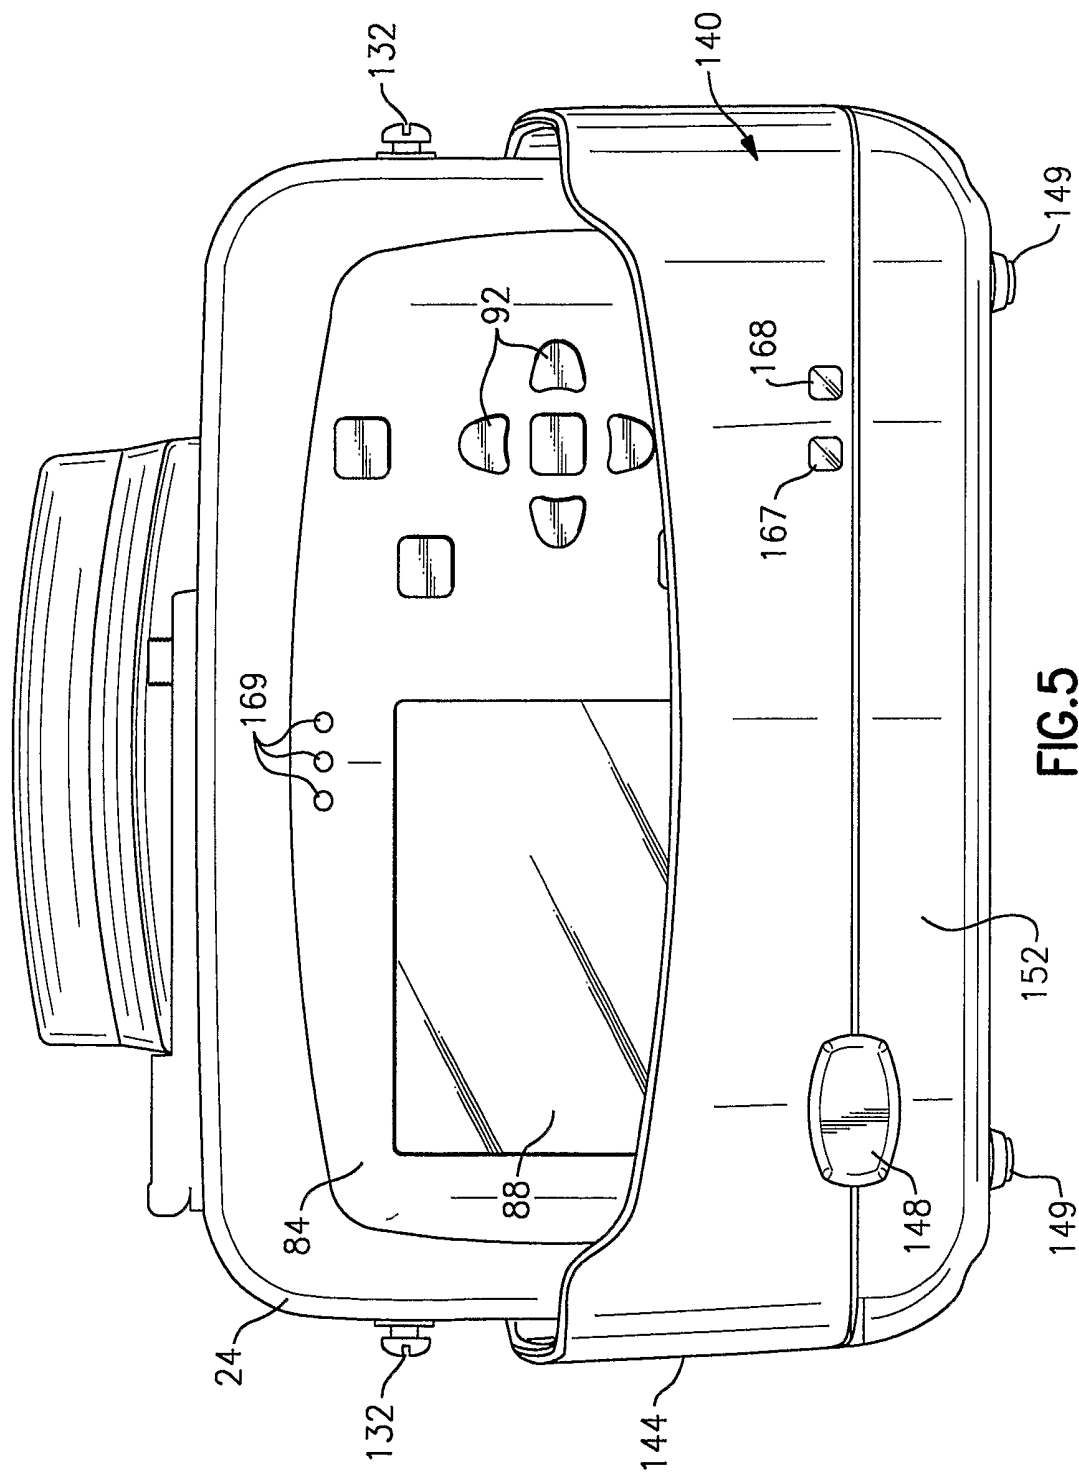


FIG. 5

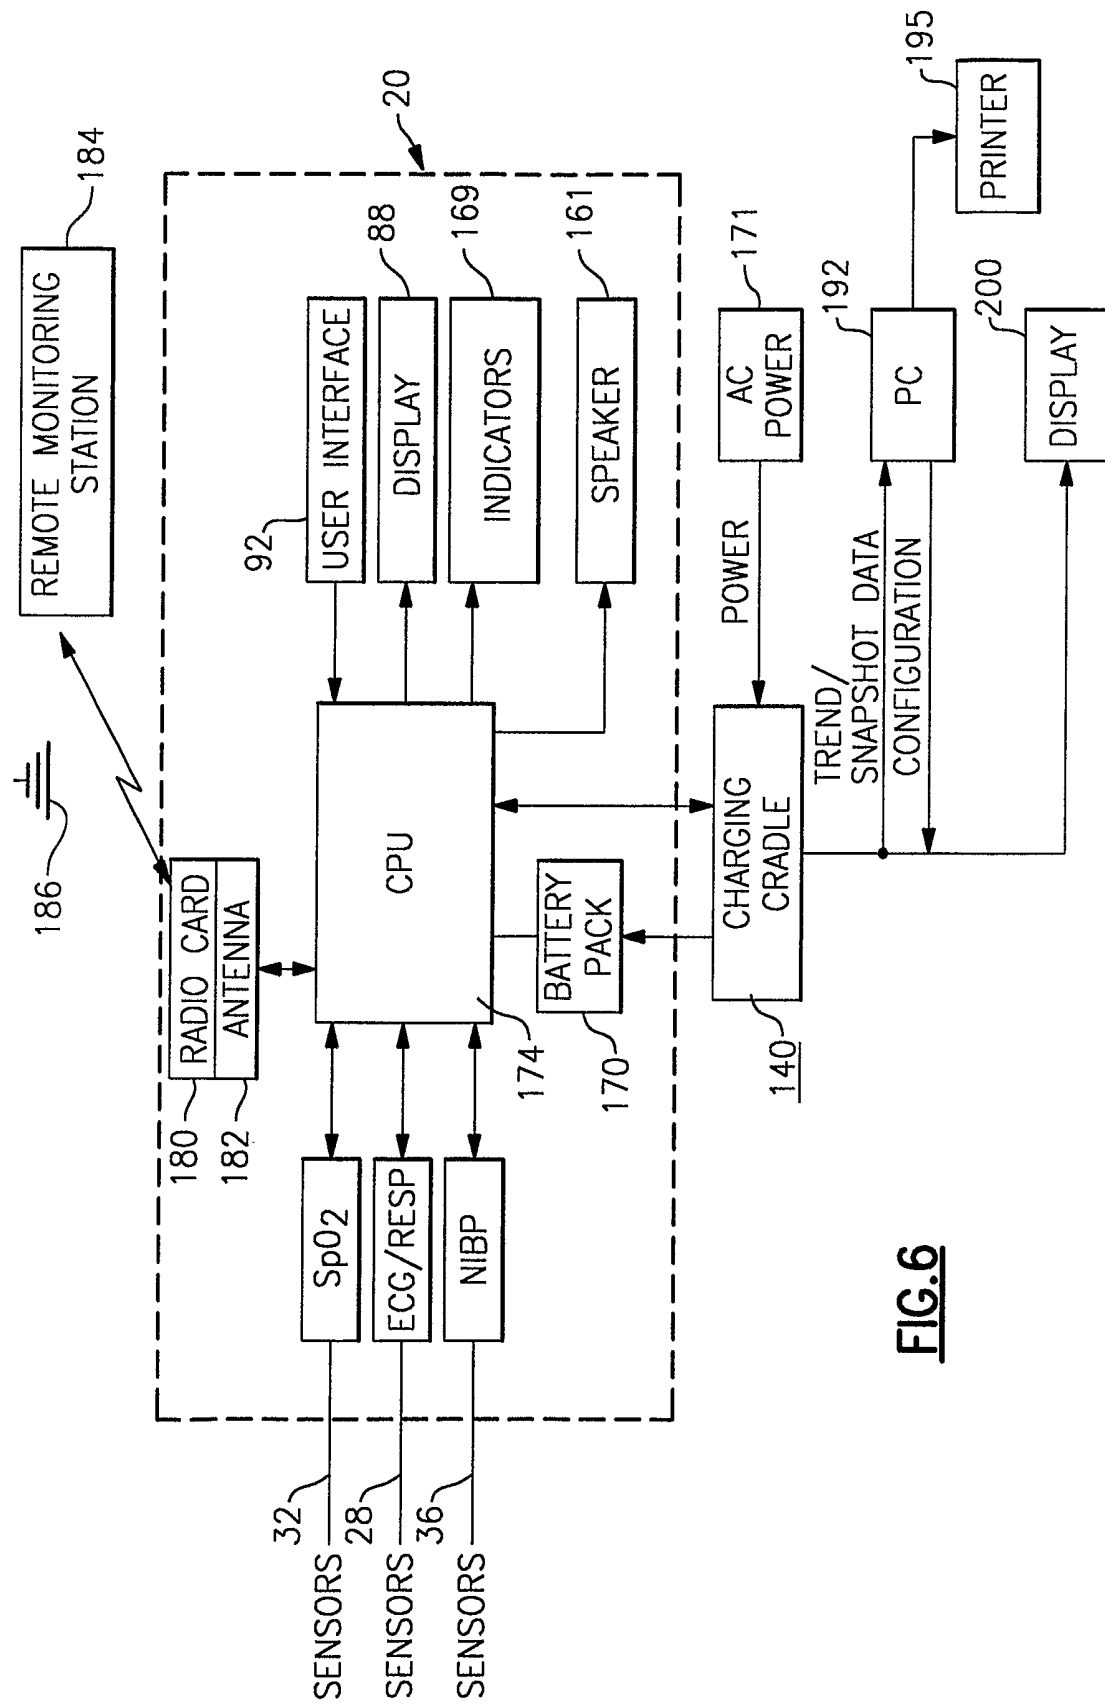


FIG. 6

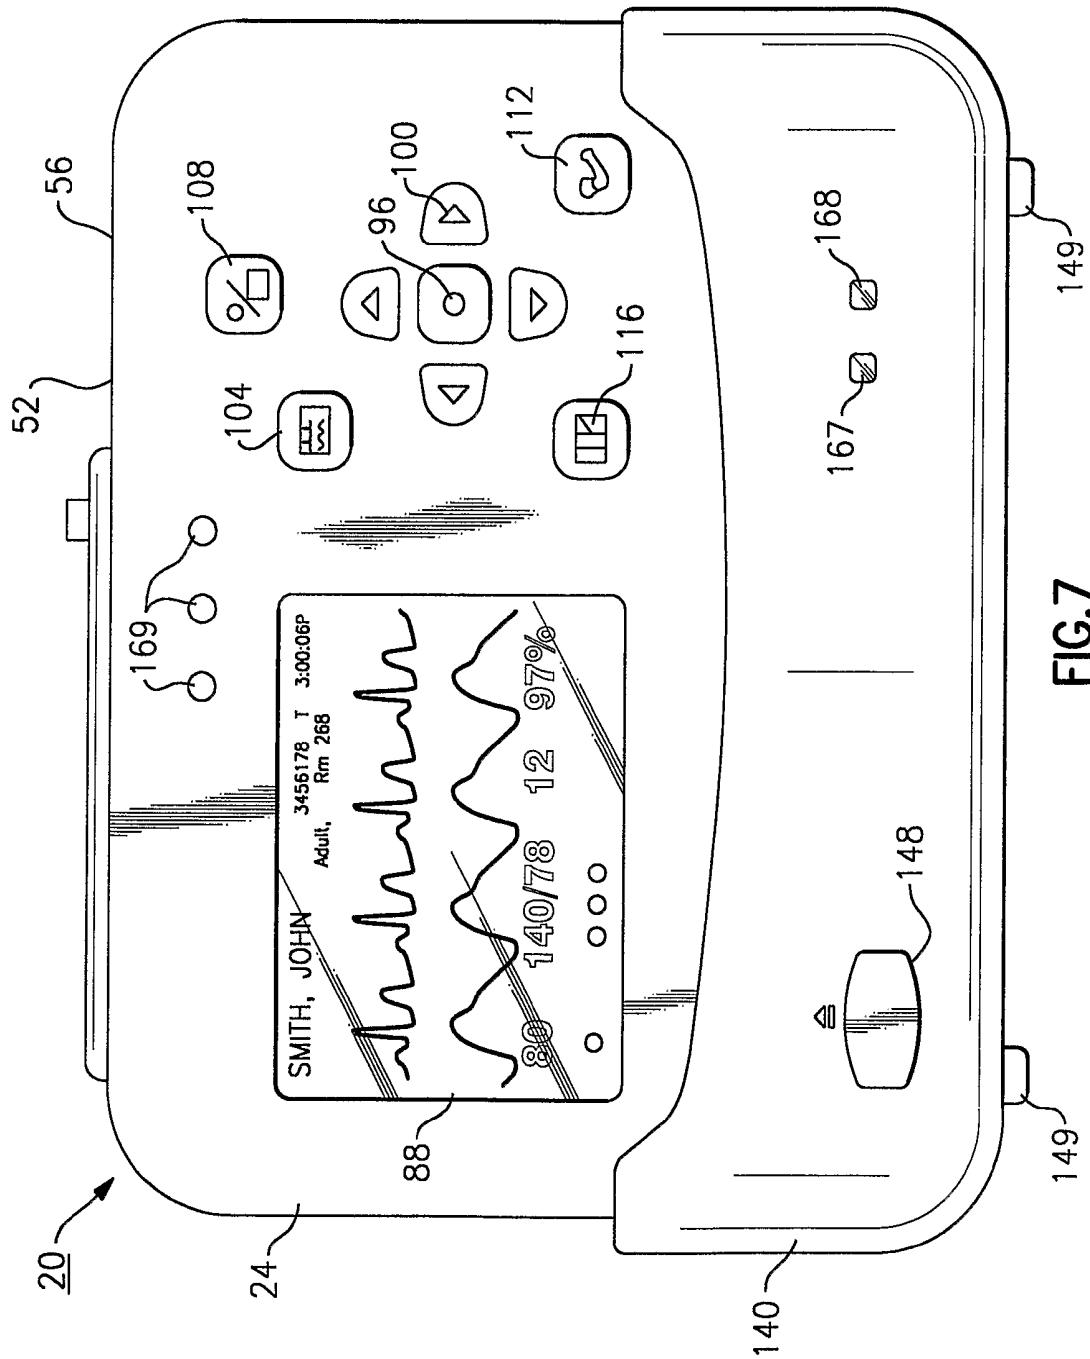


FIG. 7

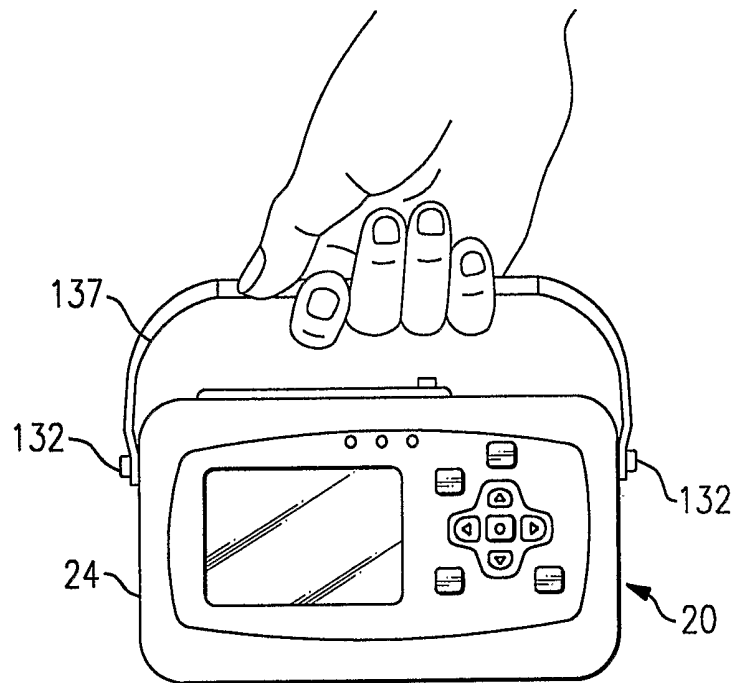


FIG. 8

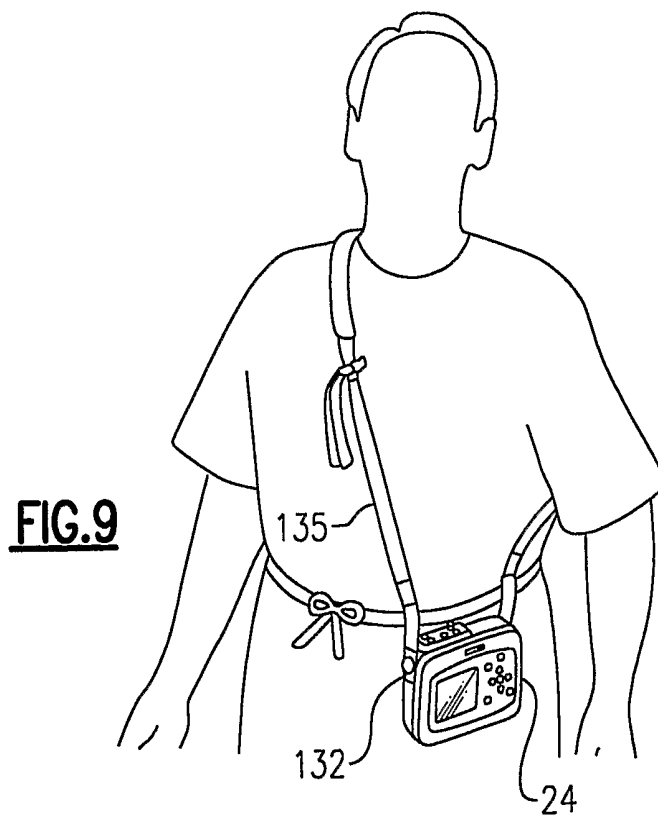


FIG. 9

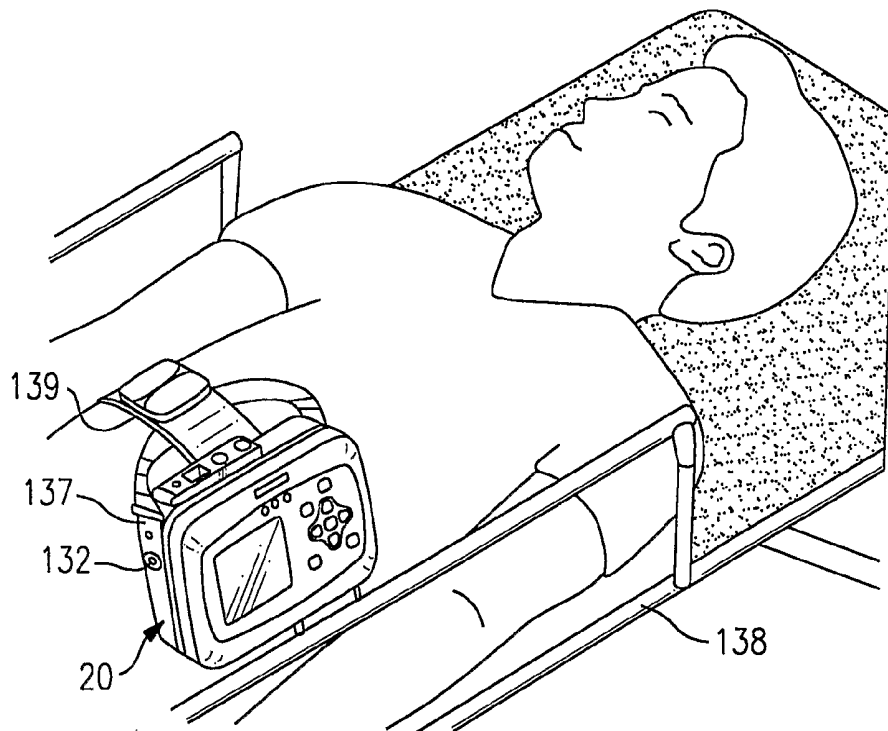


FIG. 10

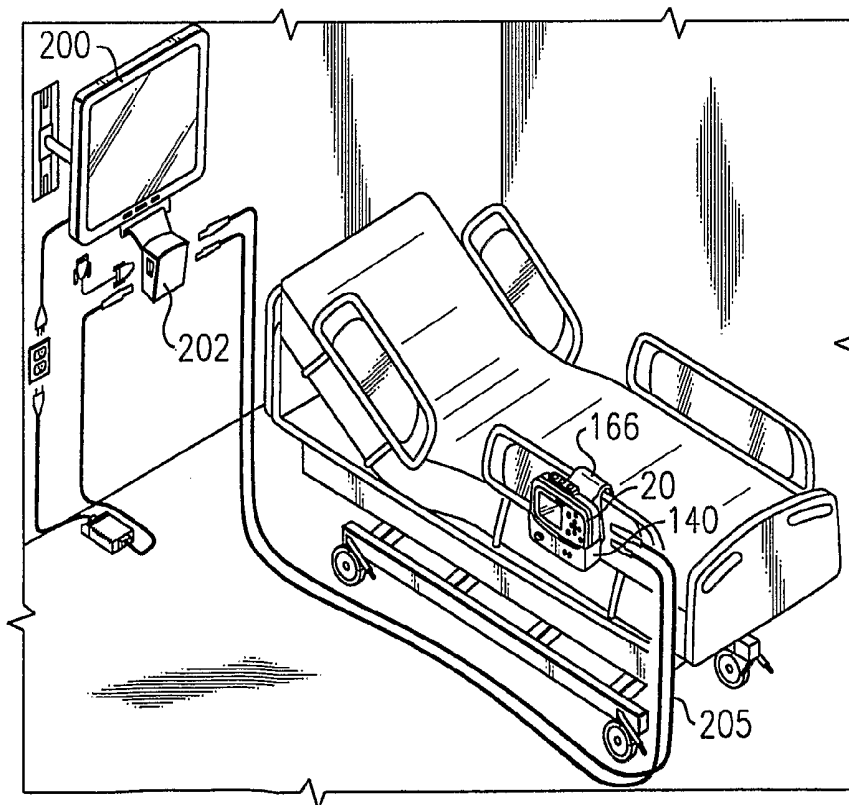
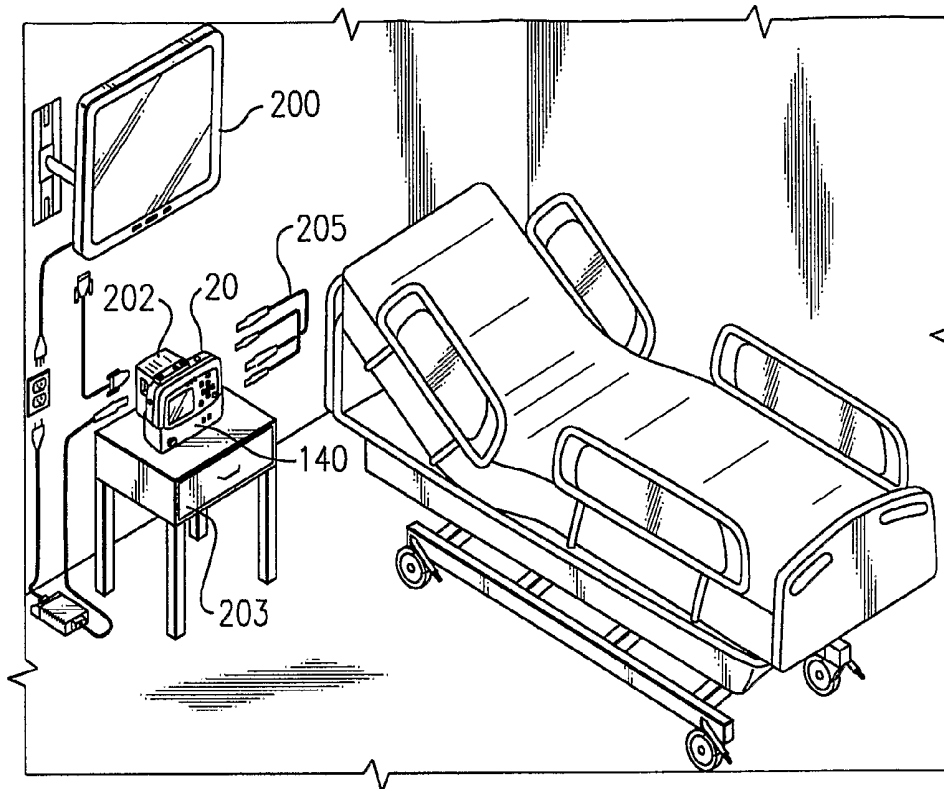
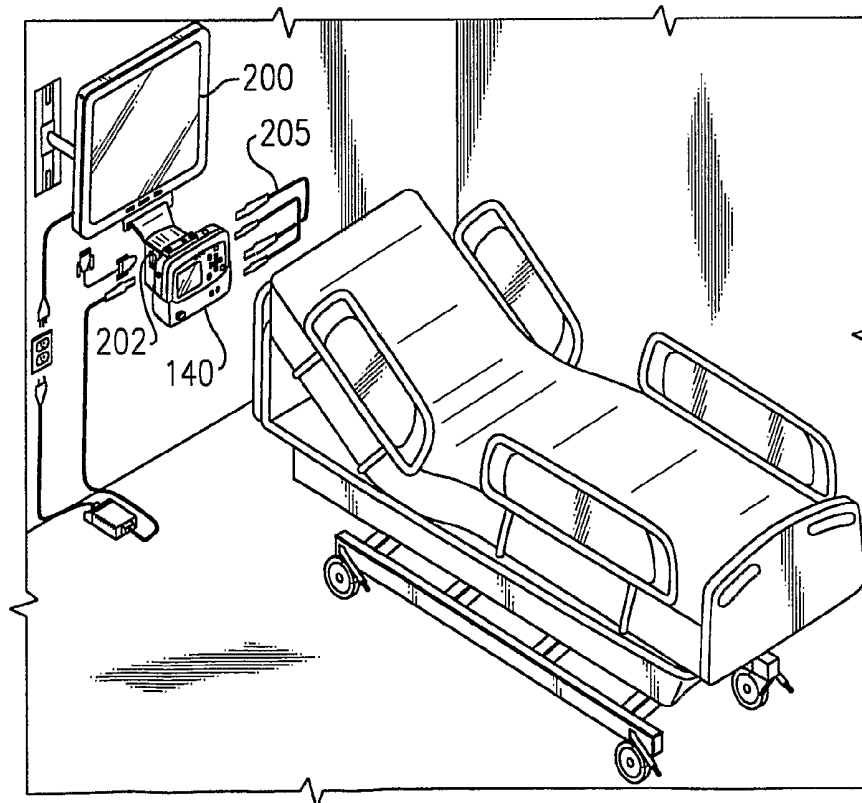


FIG. 11

FIG. 12FIG. 13

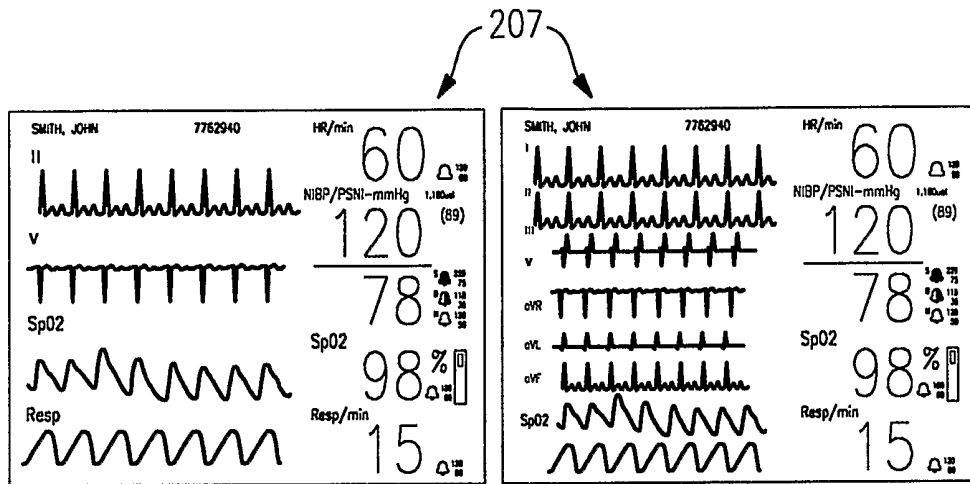


FIG. 14

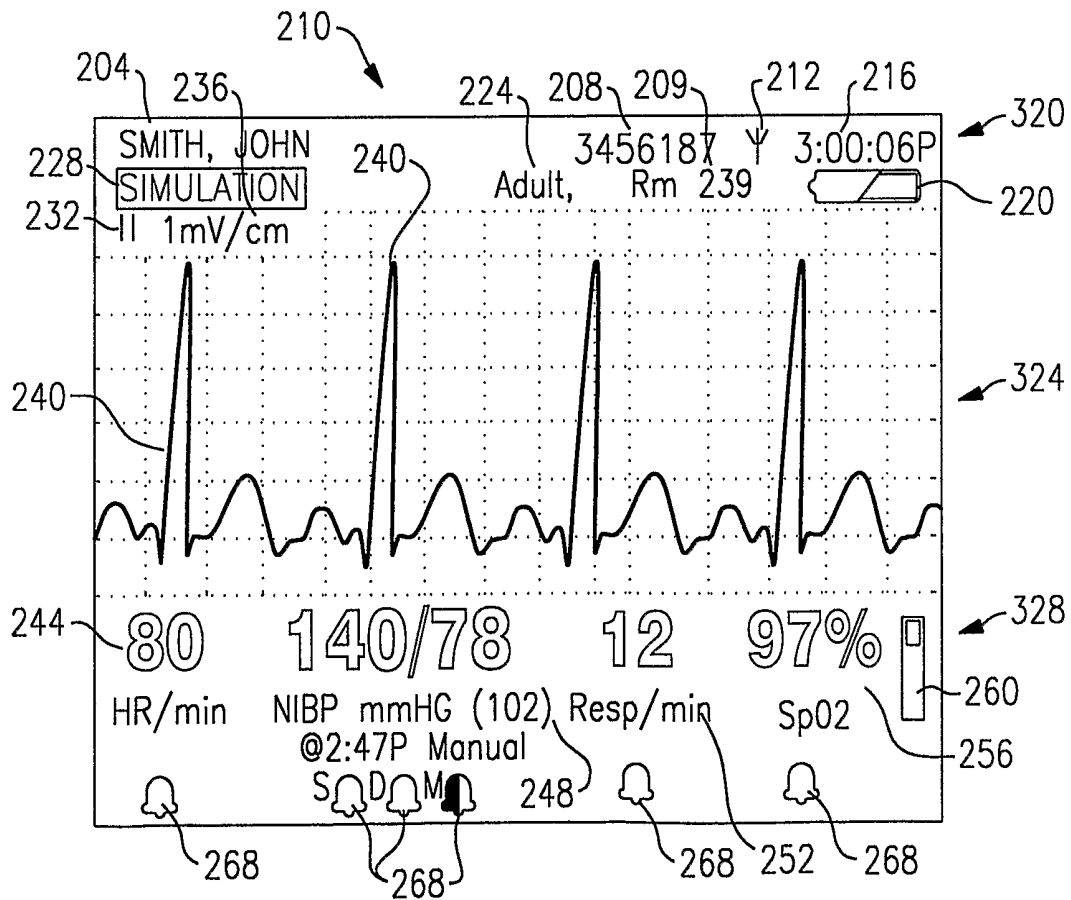


FIG. 15

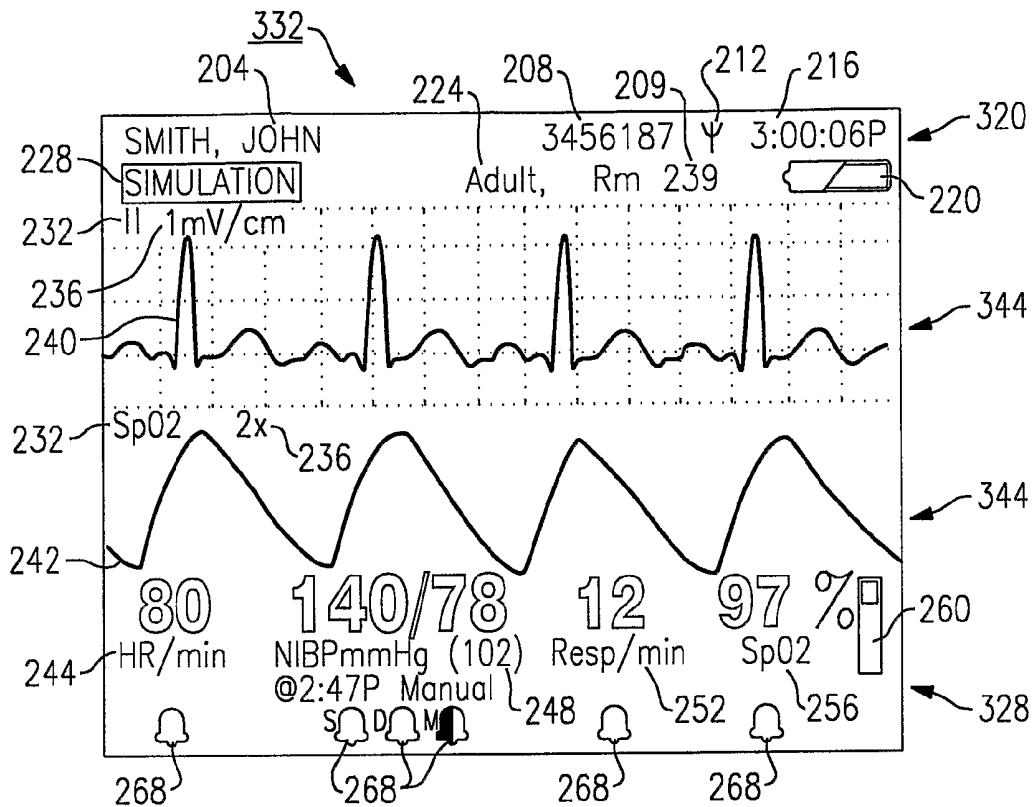


FIG. 16

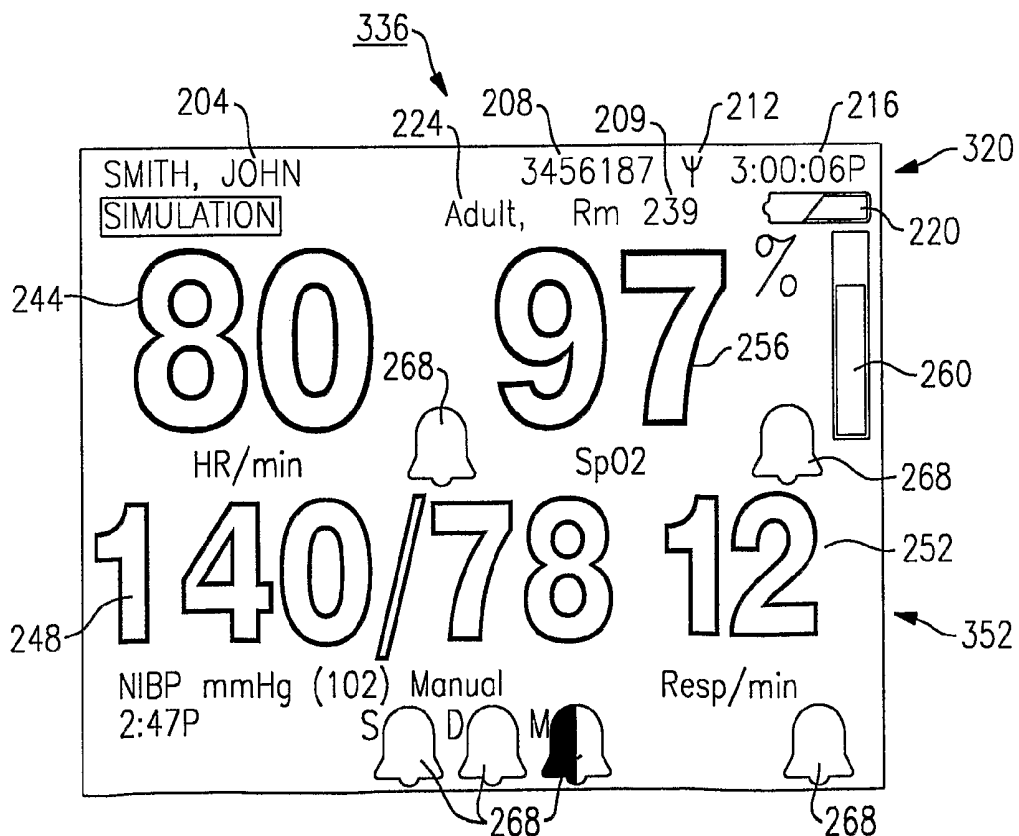


FIG. 17

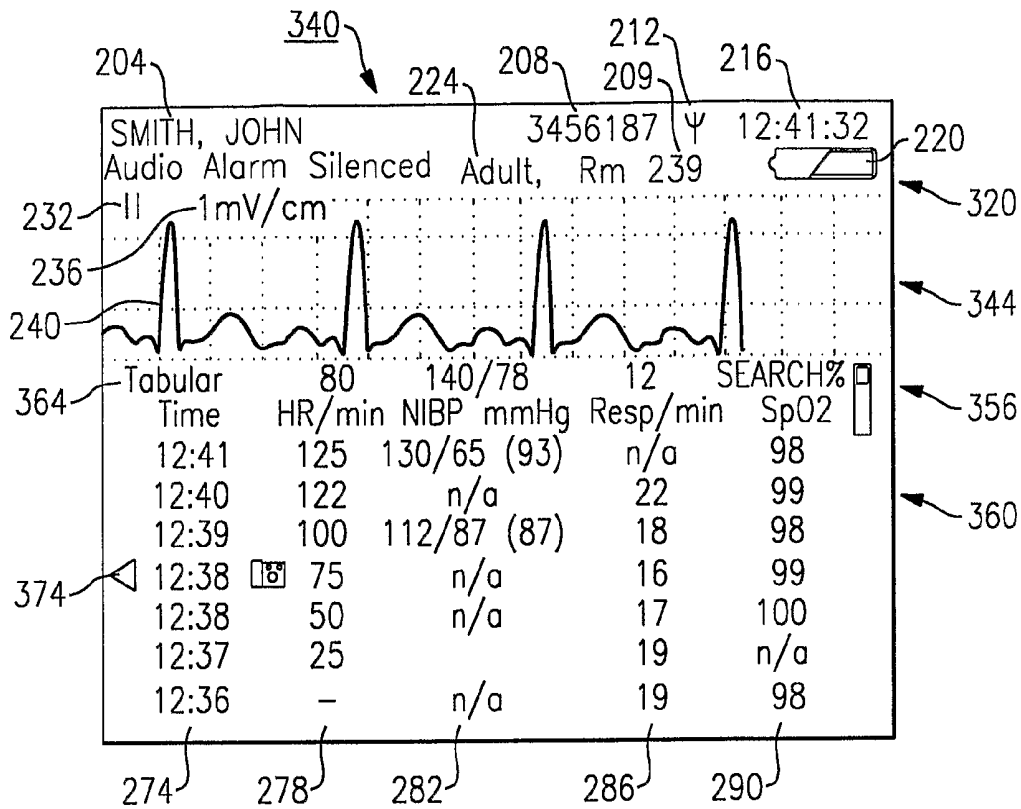


FIG. 18

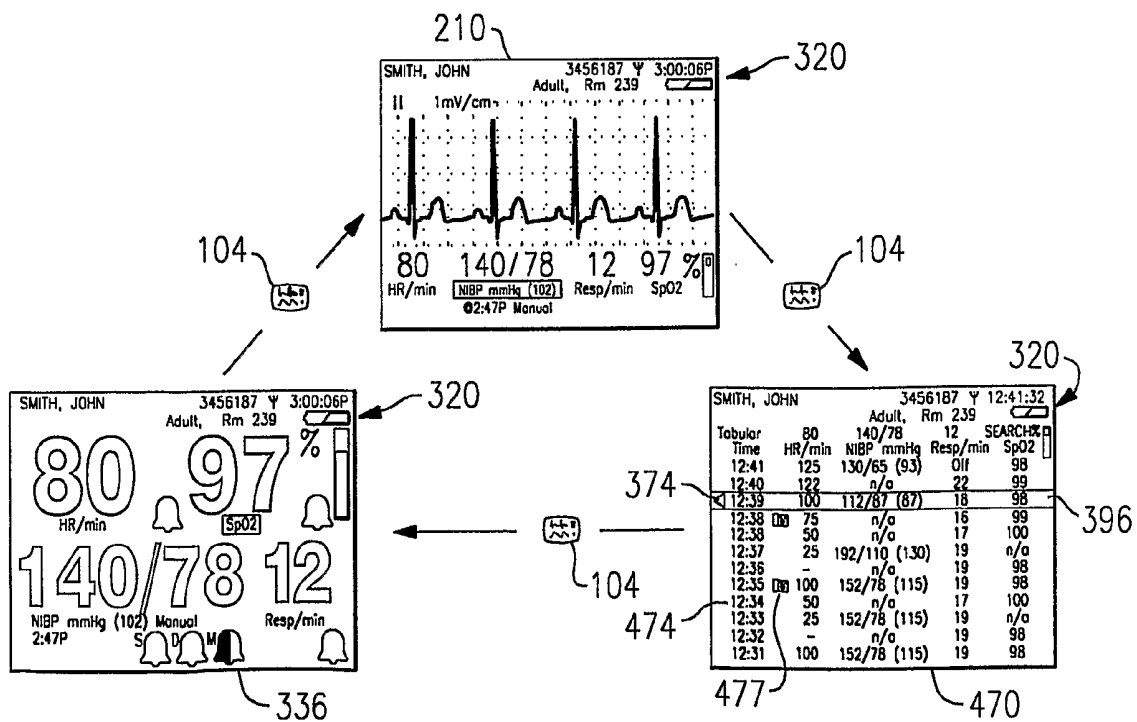
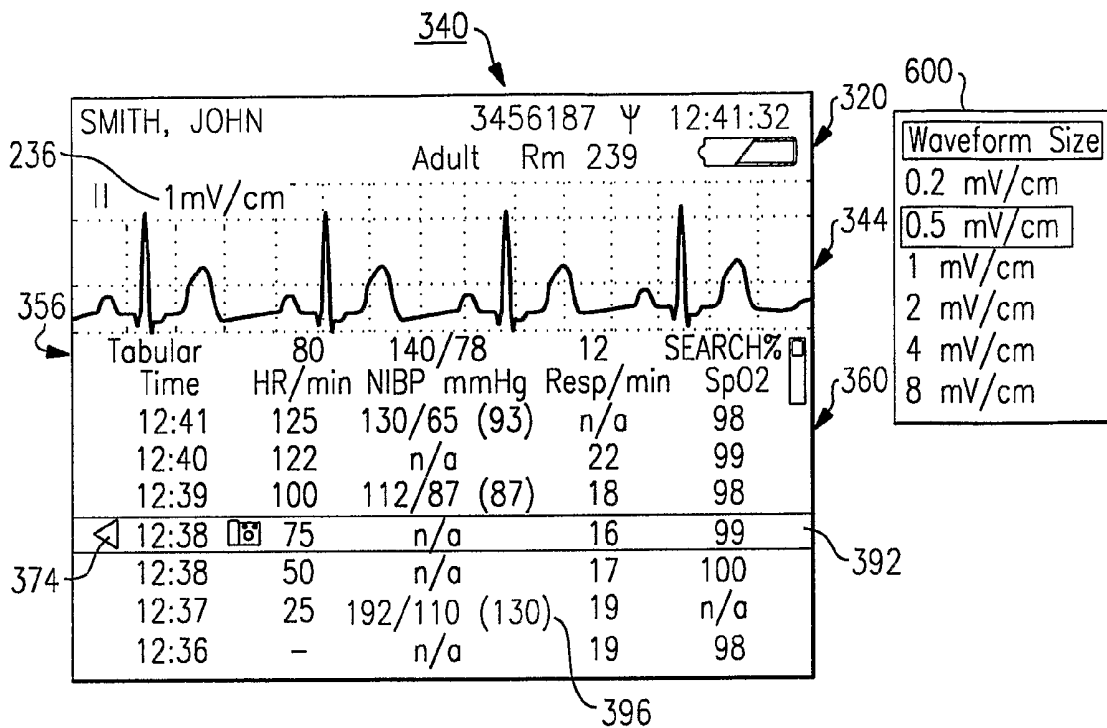
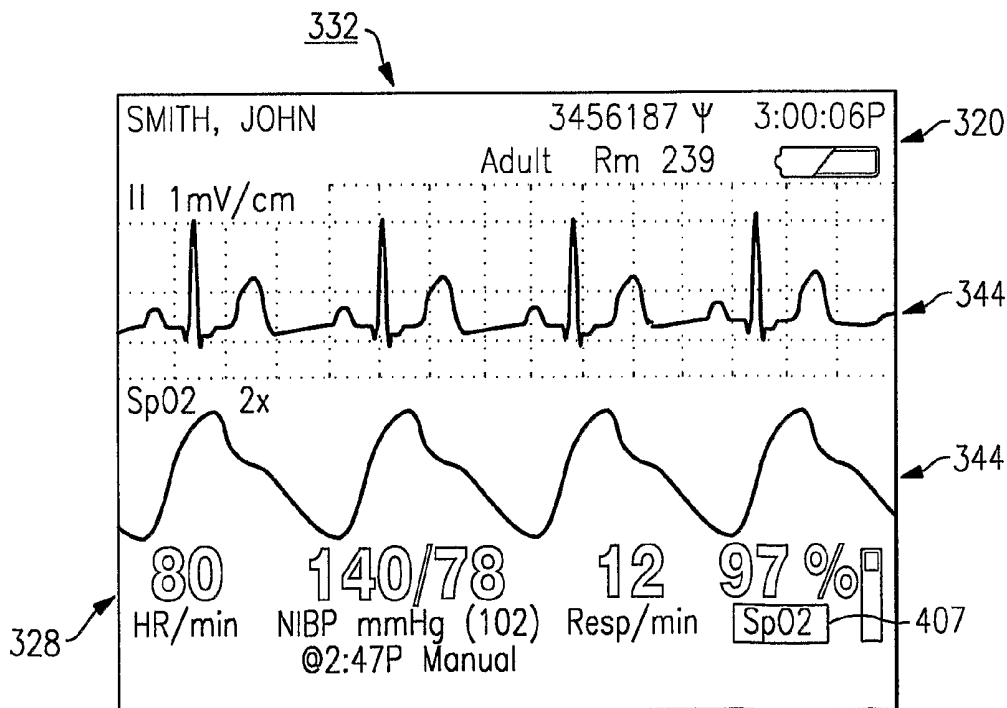
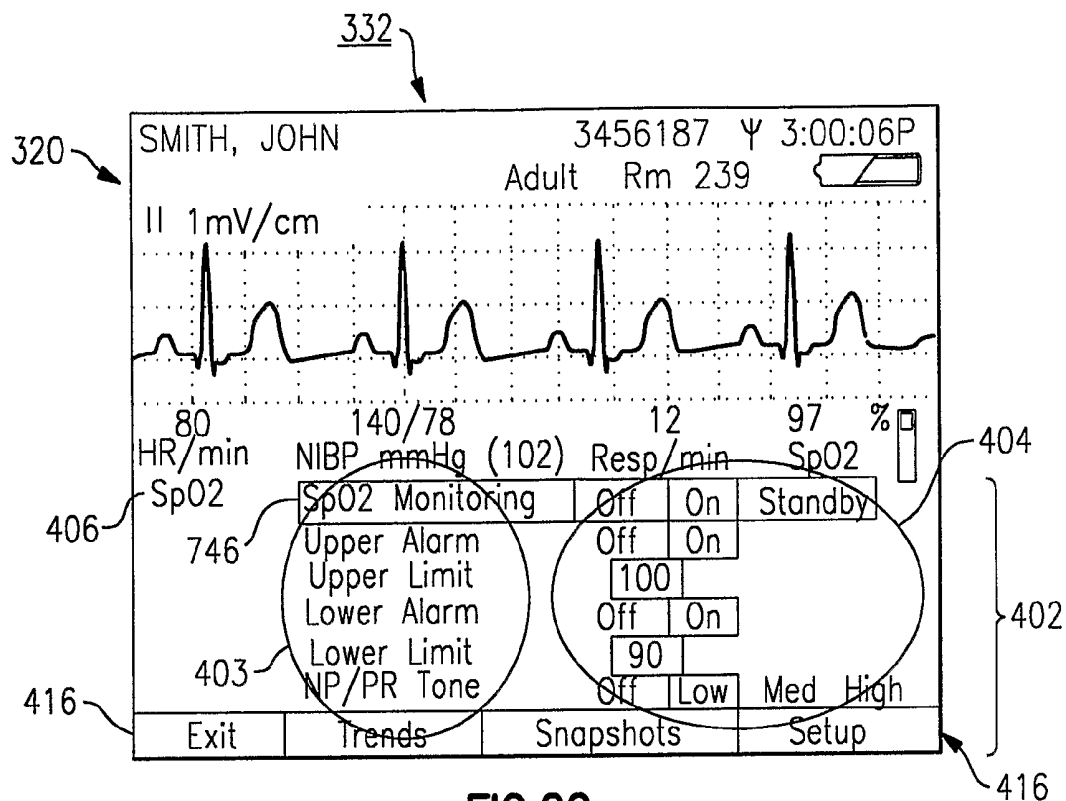
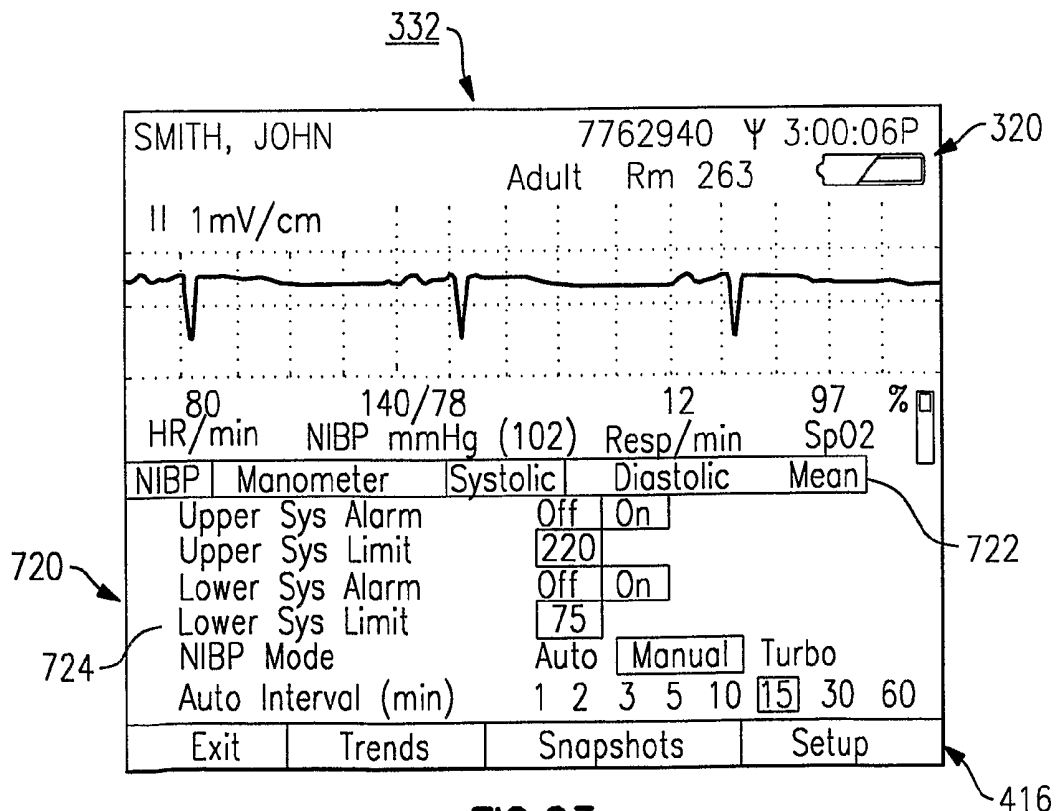


FIG. 19

**FIG. 20****FIG. 21**

**FIG.22****FIG.23**







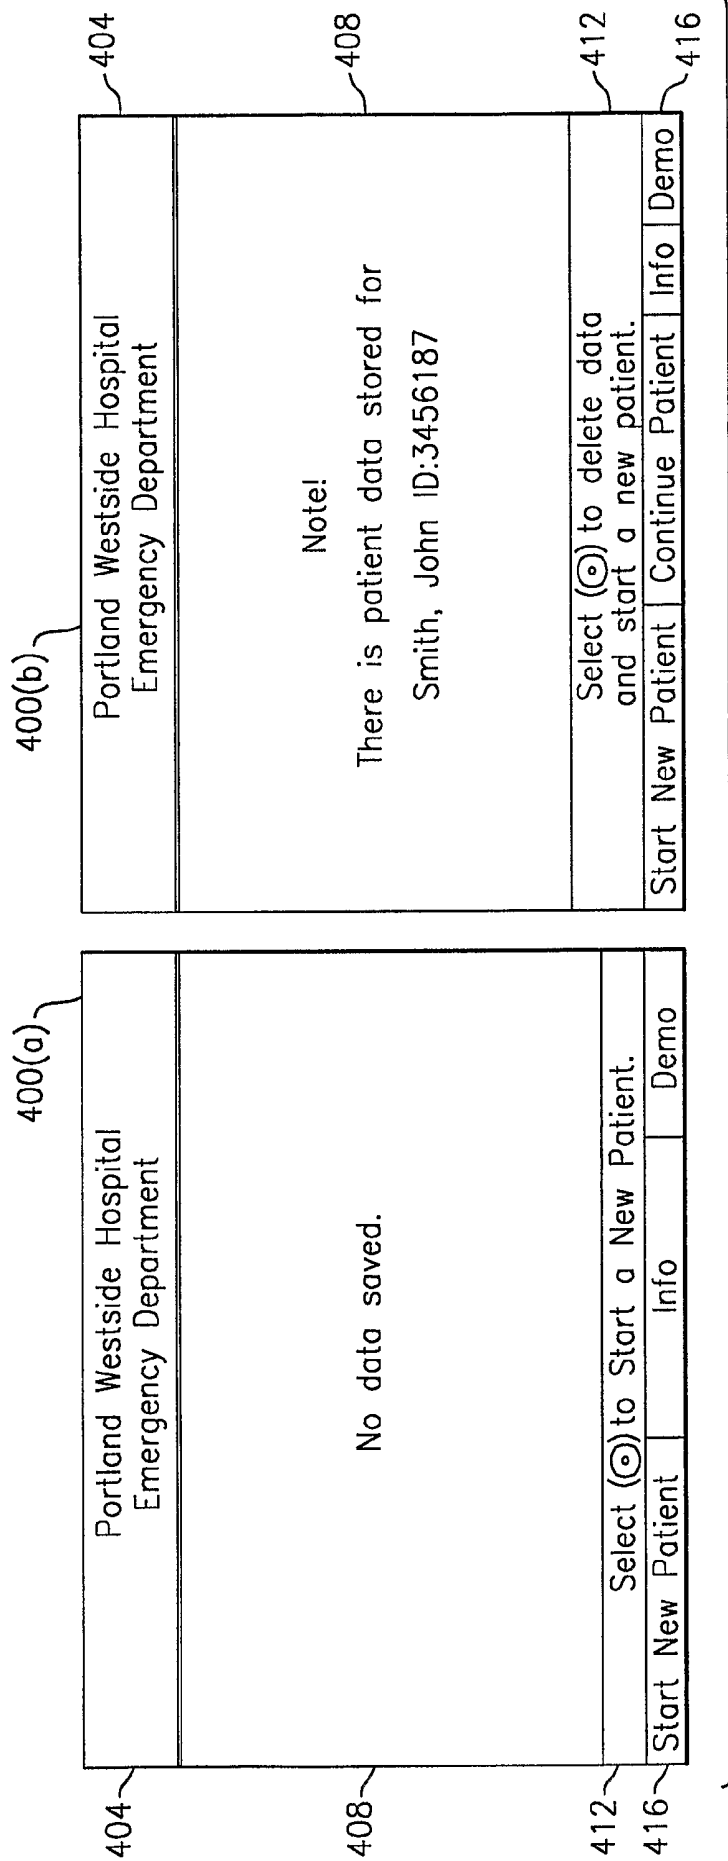


FIG. 24

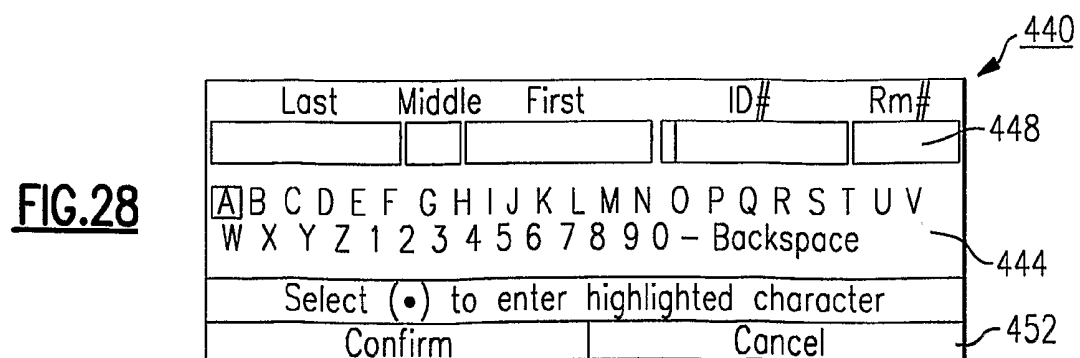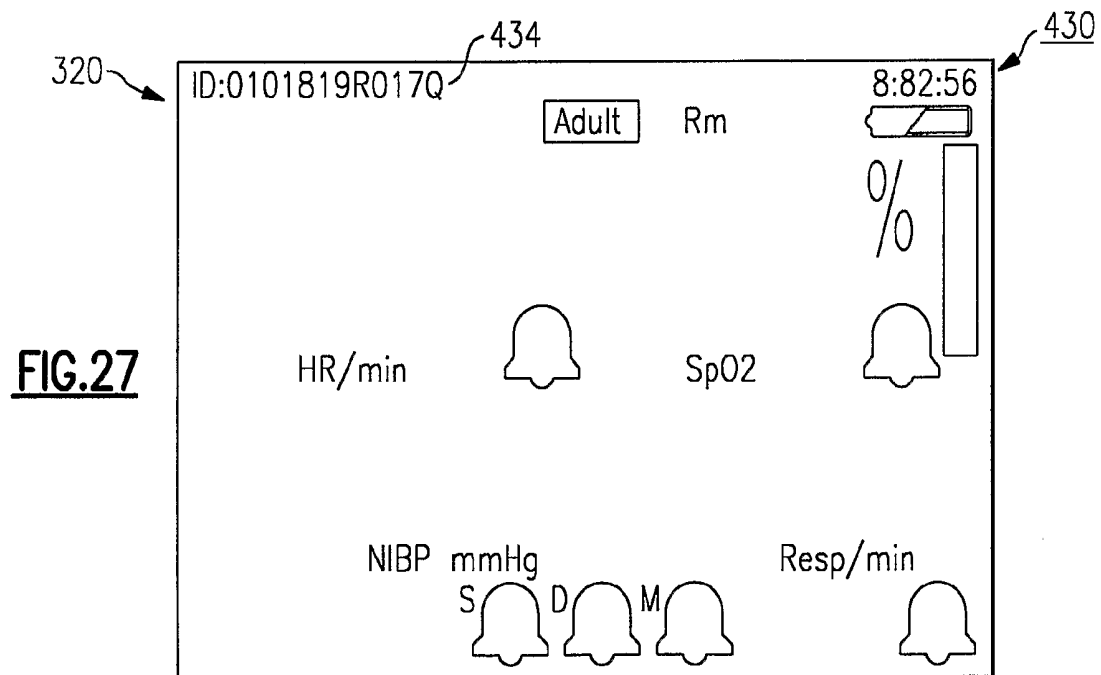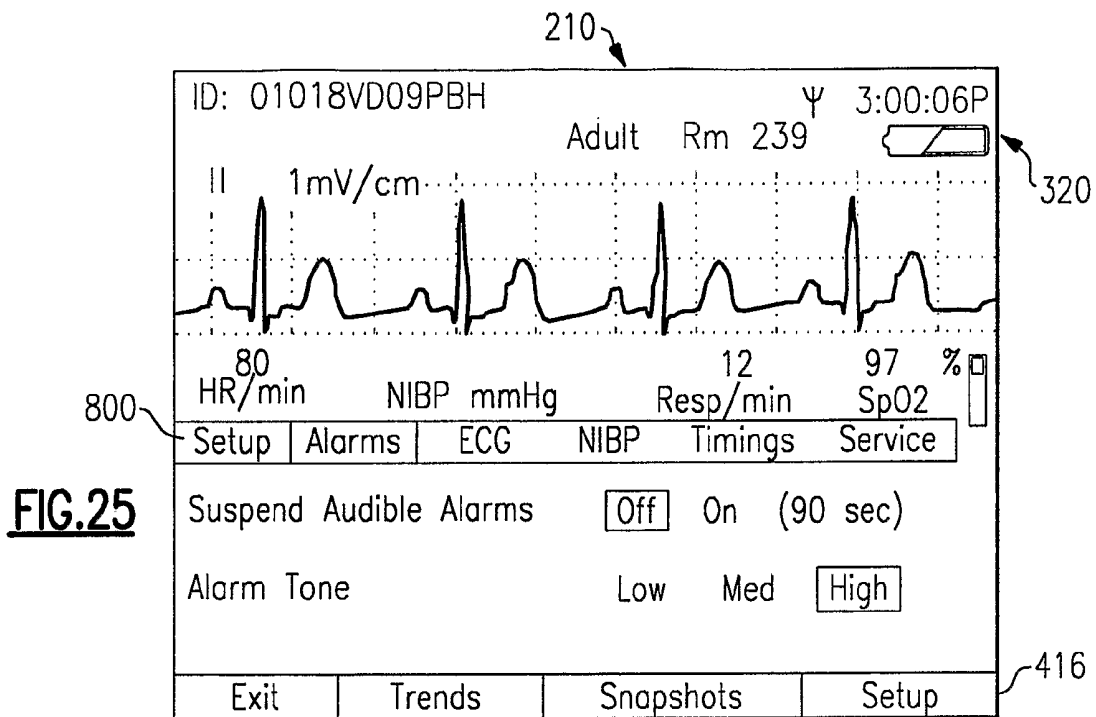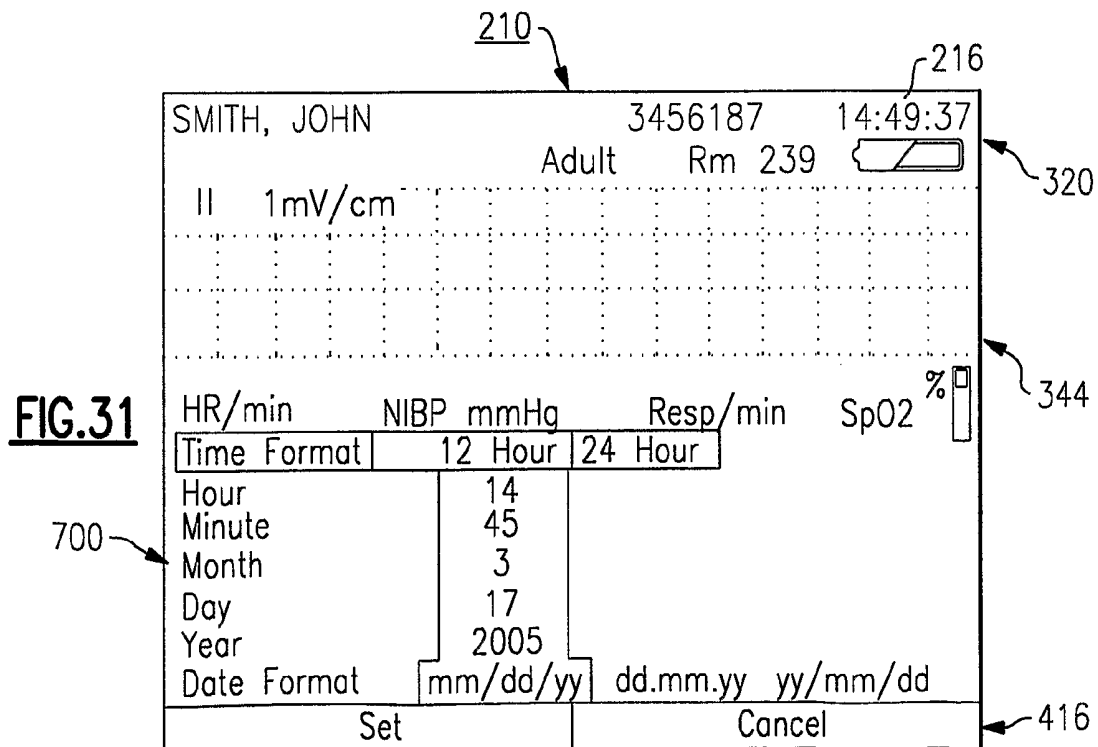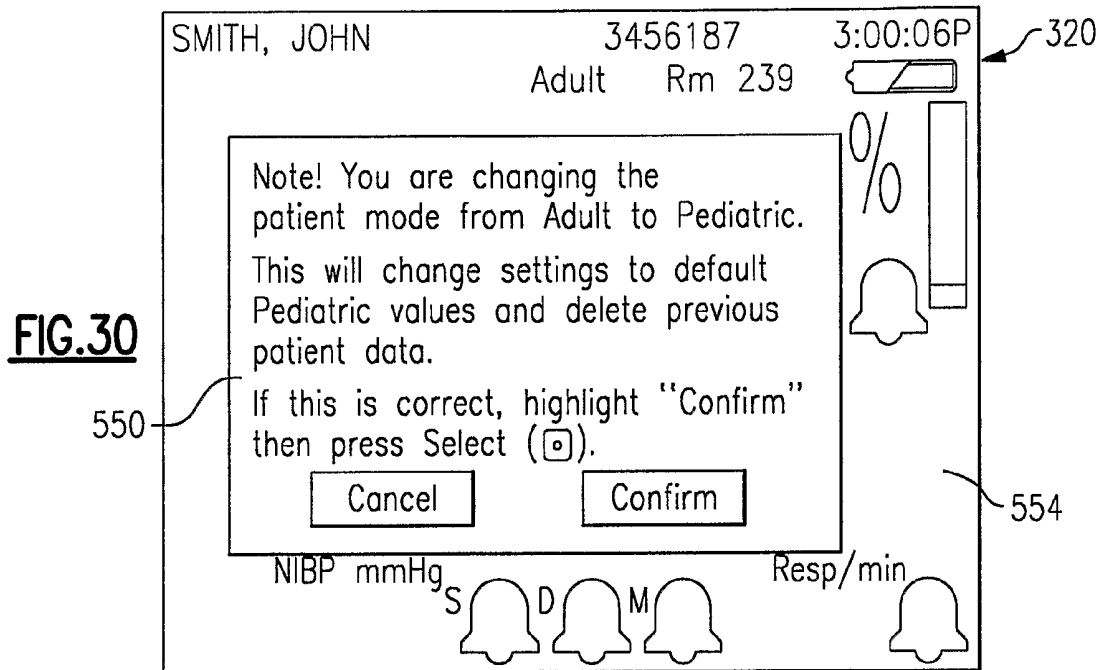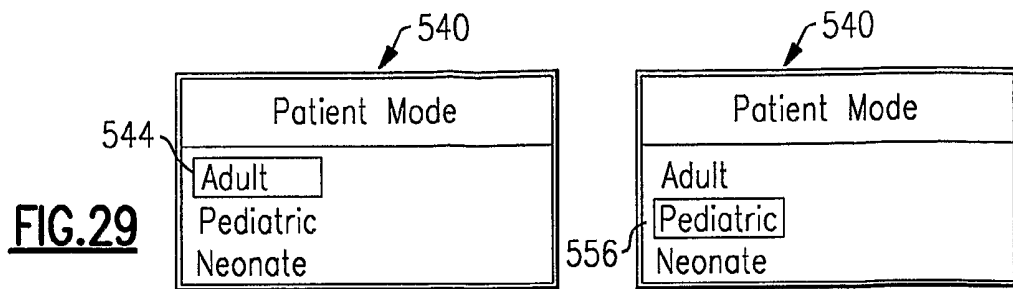

422 Welch Allyn Propaq 802LTRN SERIAL#F82C0DD5 V1.00.00	422 Welch Allyn Propaq 802LTON SERIAL#AB72383-1 V1.00.00
424 Portland Westside Emergency Department PtIdWstsdED10Jun05.mnt Ann Jones, MD 503-530-0101 X9999 Patient Mode Adult Wireless Communications Enabled	424 Portland Westside Emergency Department PtIdWstsdED10Jun05.mnt Ann Jones, MD 503-530-0101 X9999 Patient Mode Adult Wireless Communications Disabled
416	416
Start New Patient	Start New Patient
Info	Info
Demo	Demo

FIG.26



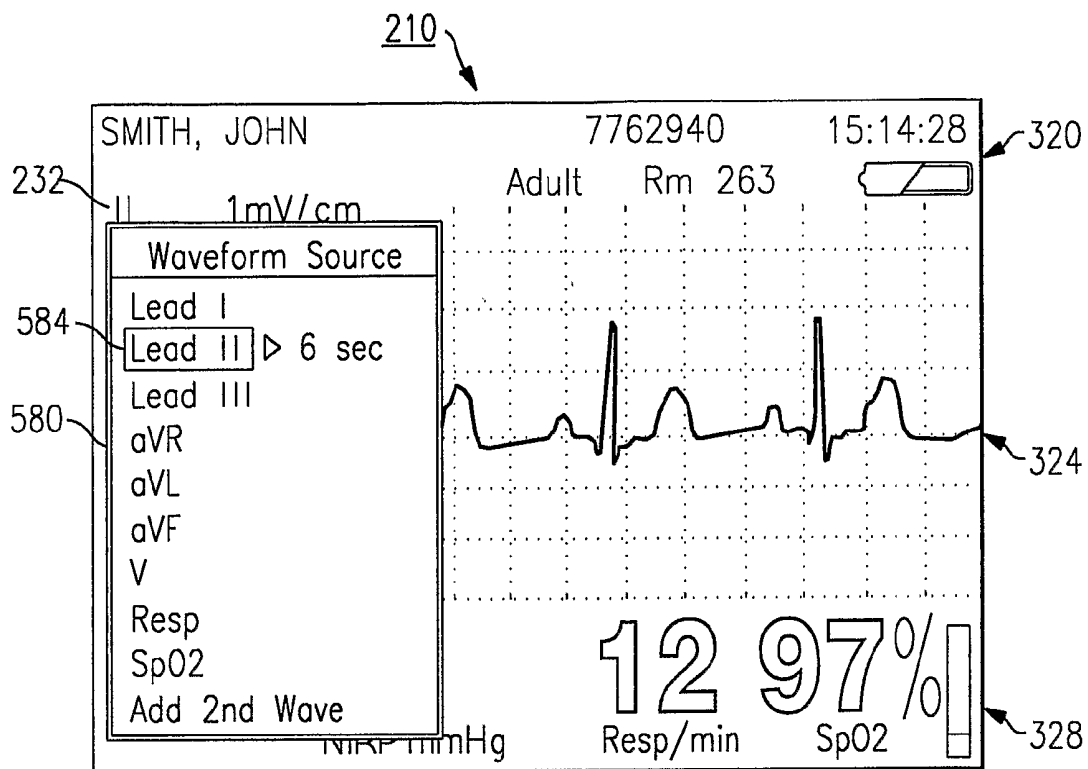


FIG.32

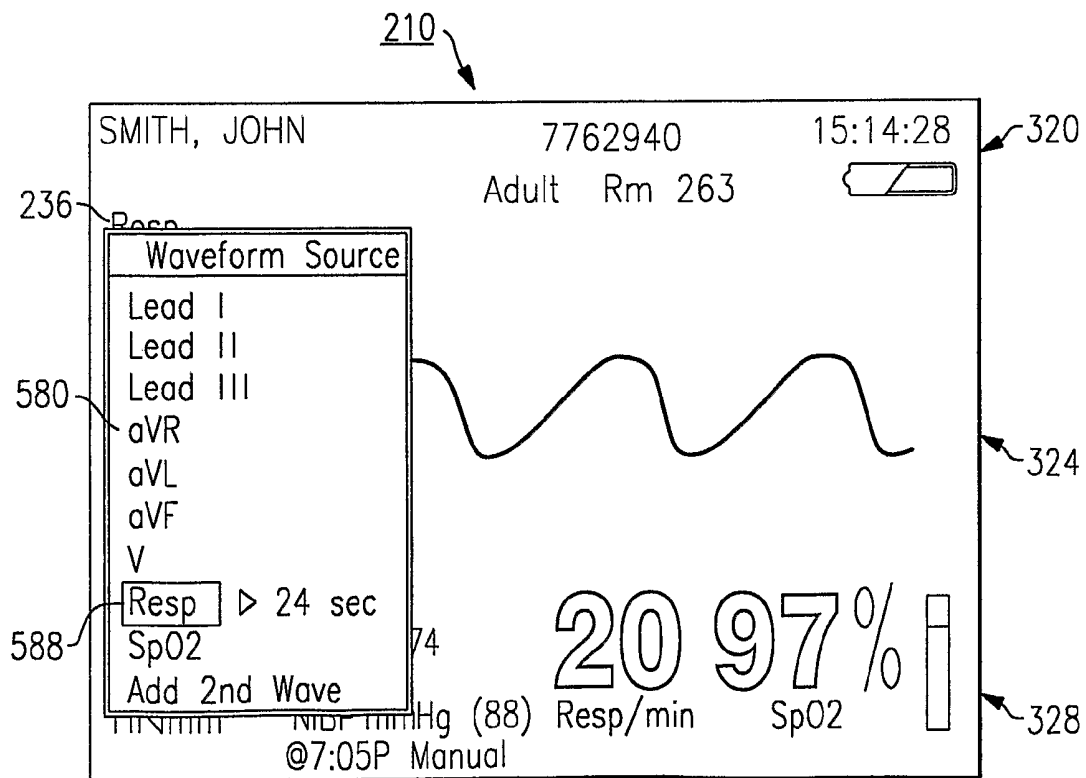


FIG.33

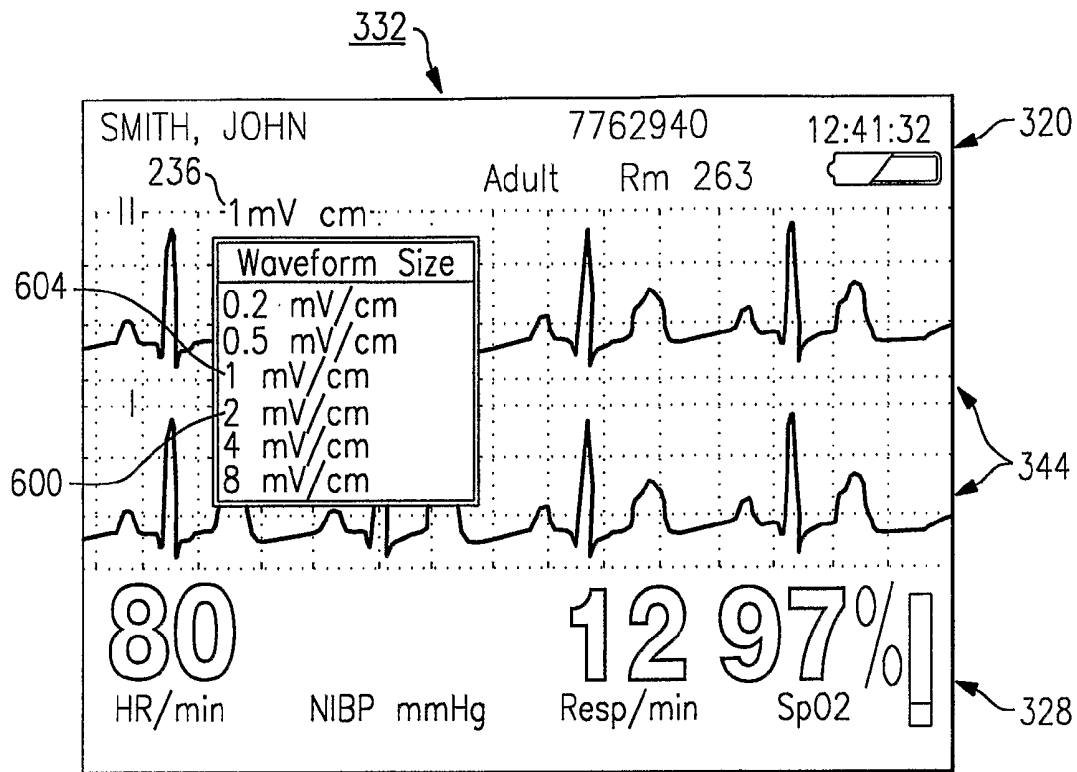
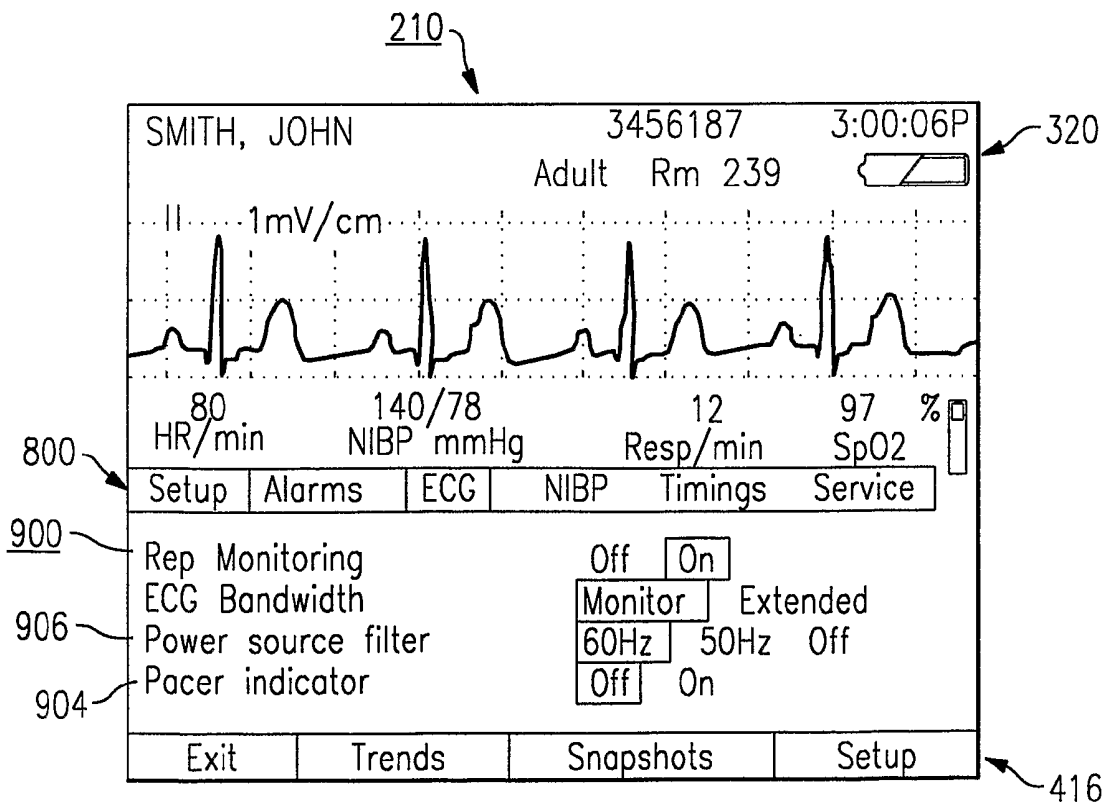
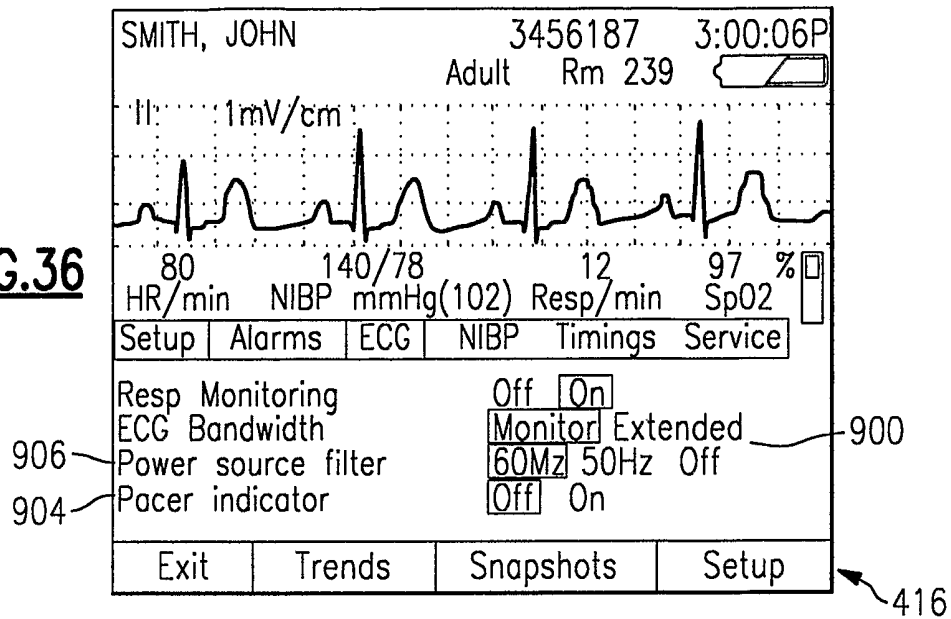
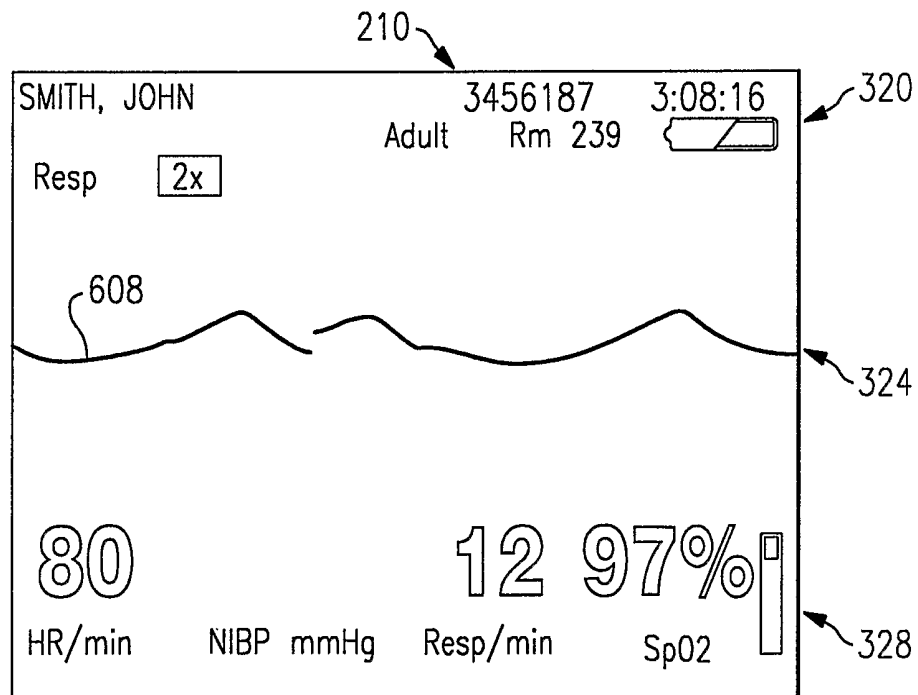
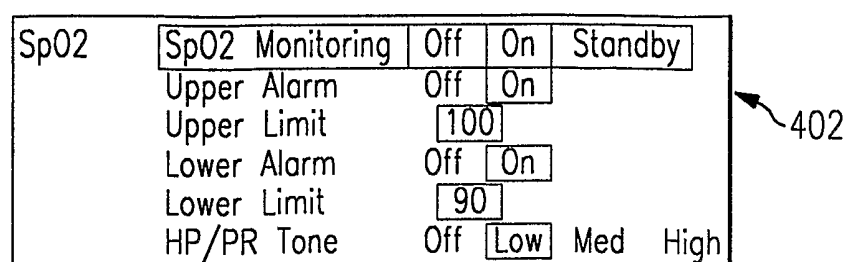
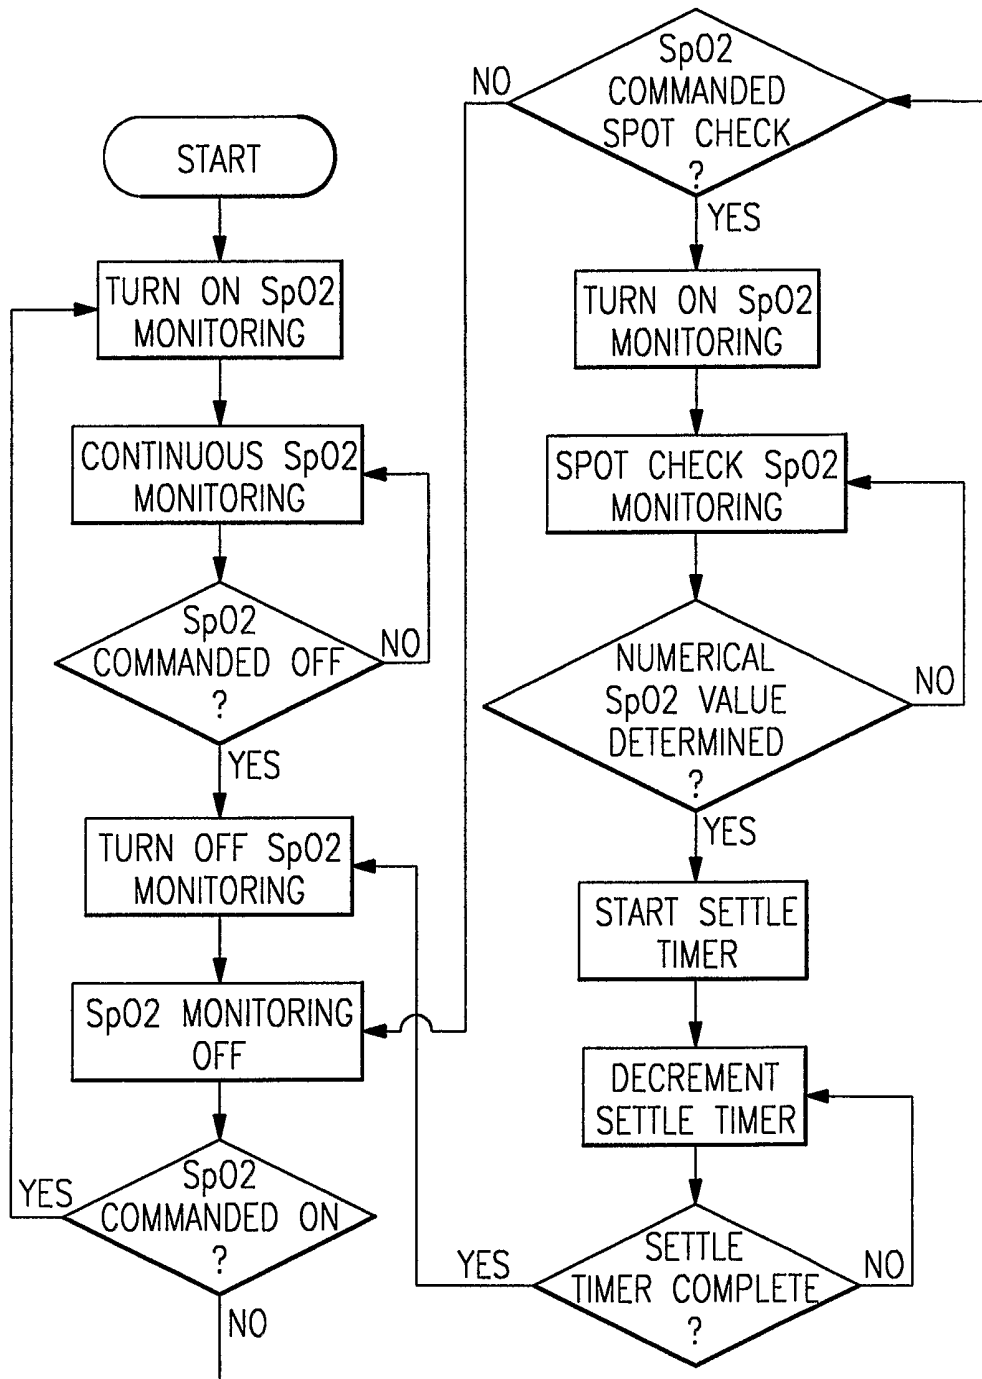
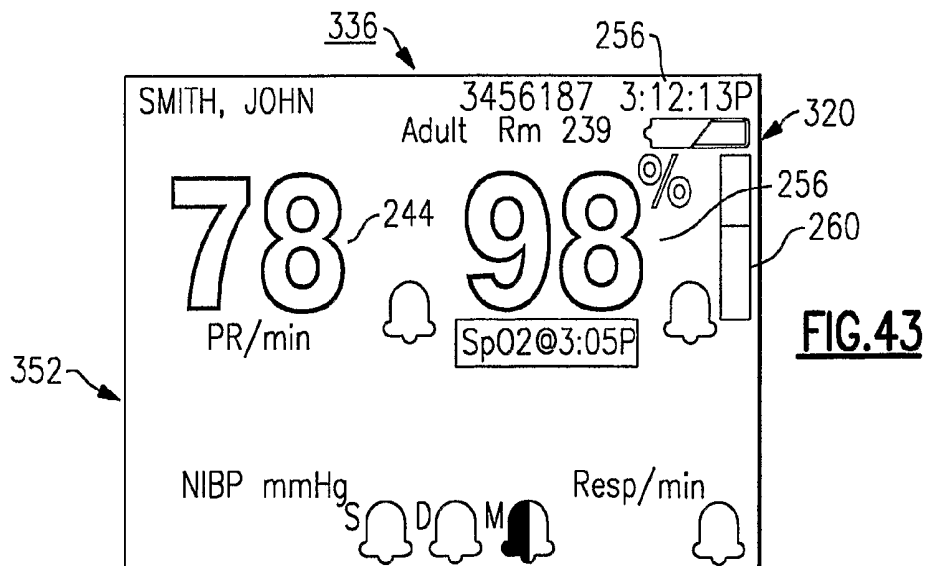
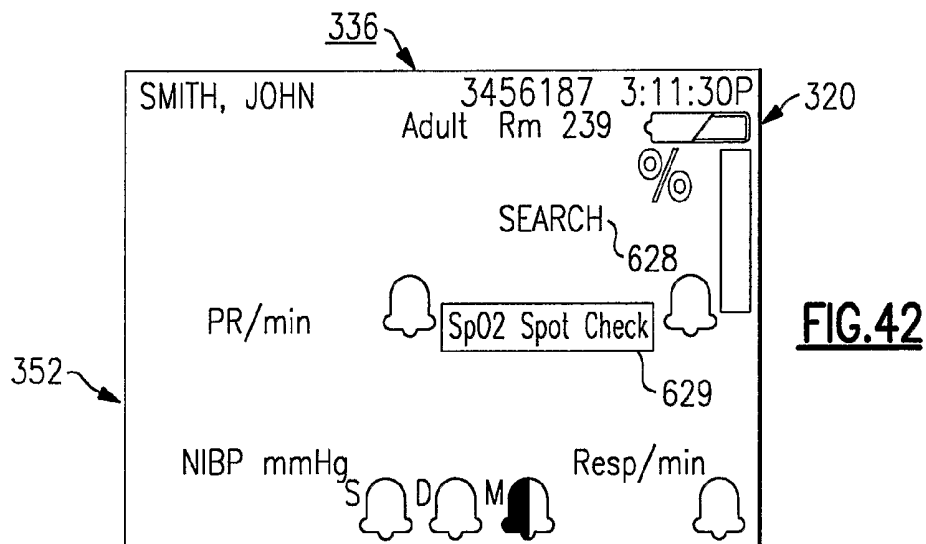
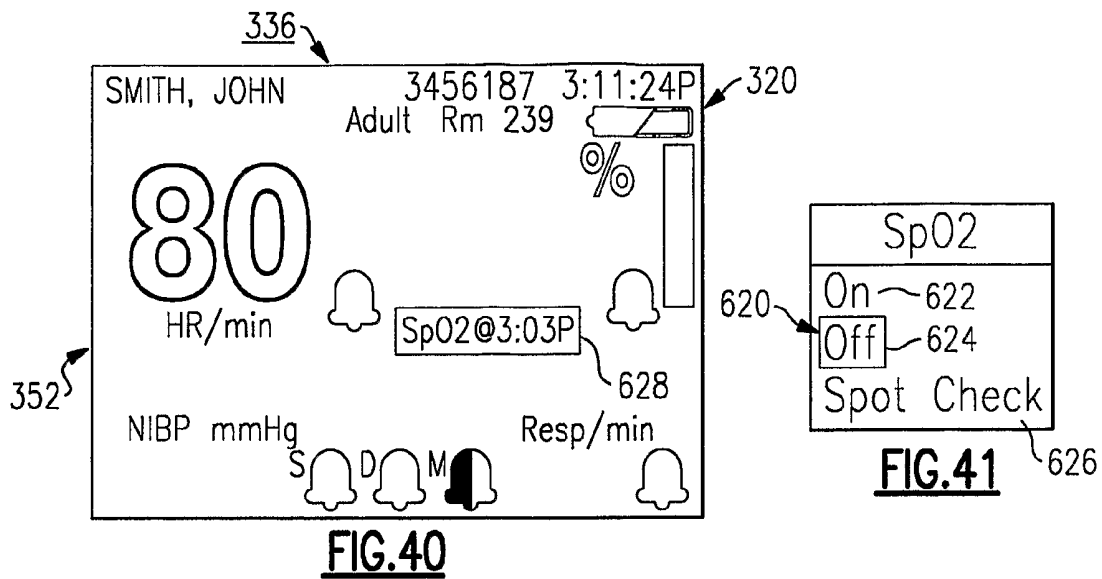
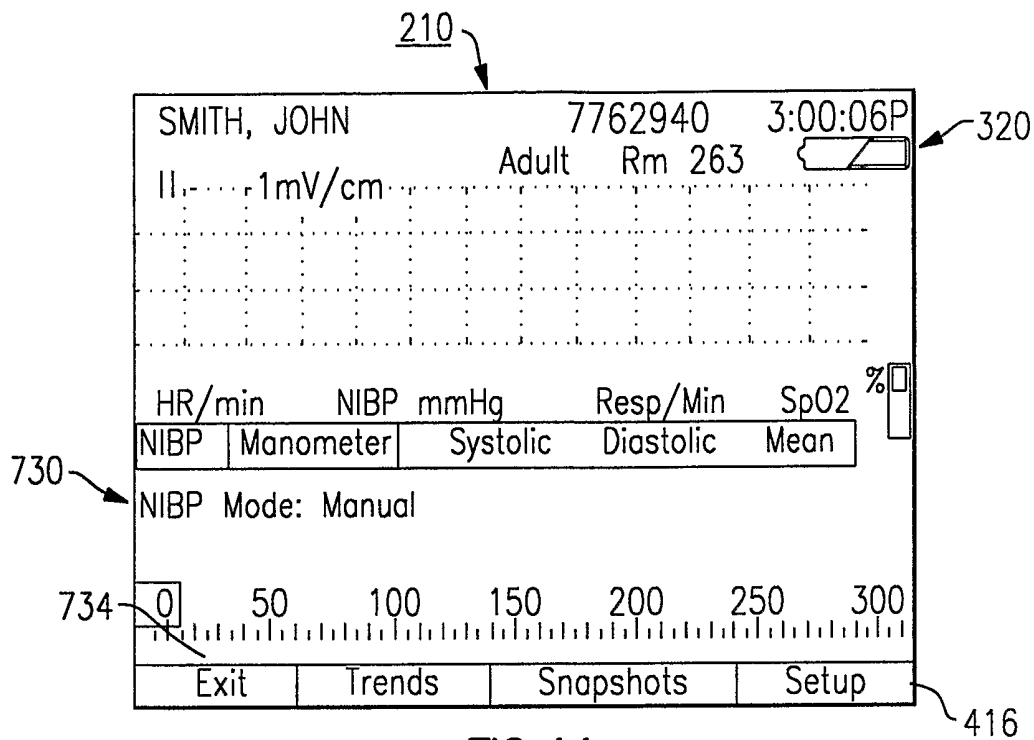
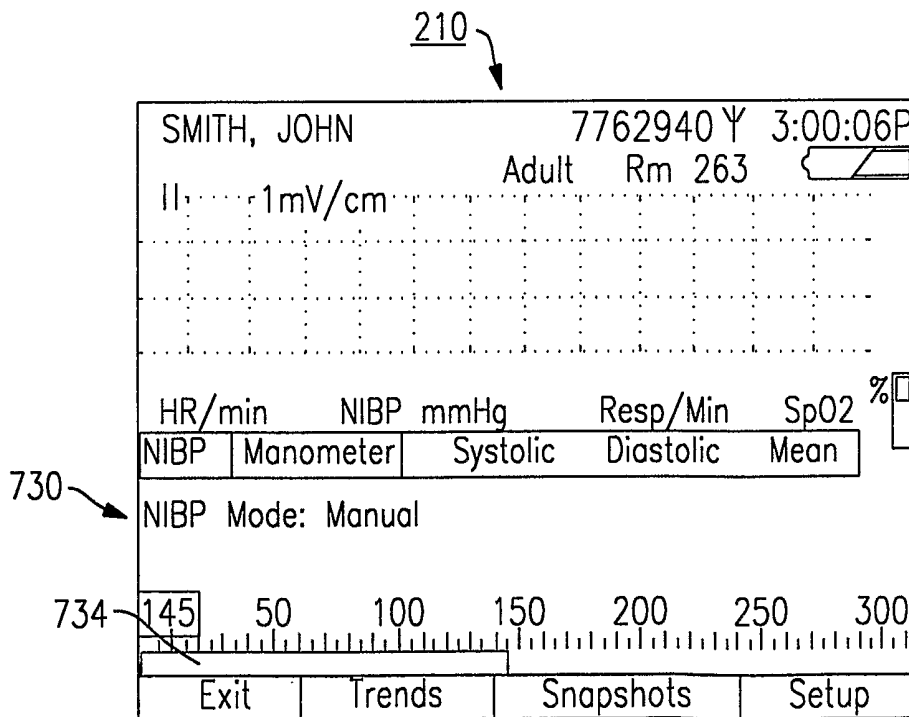
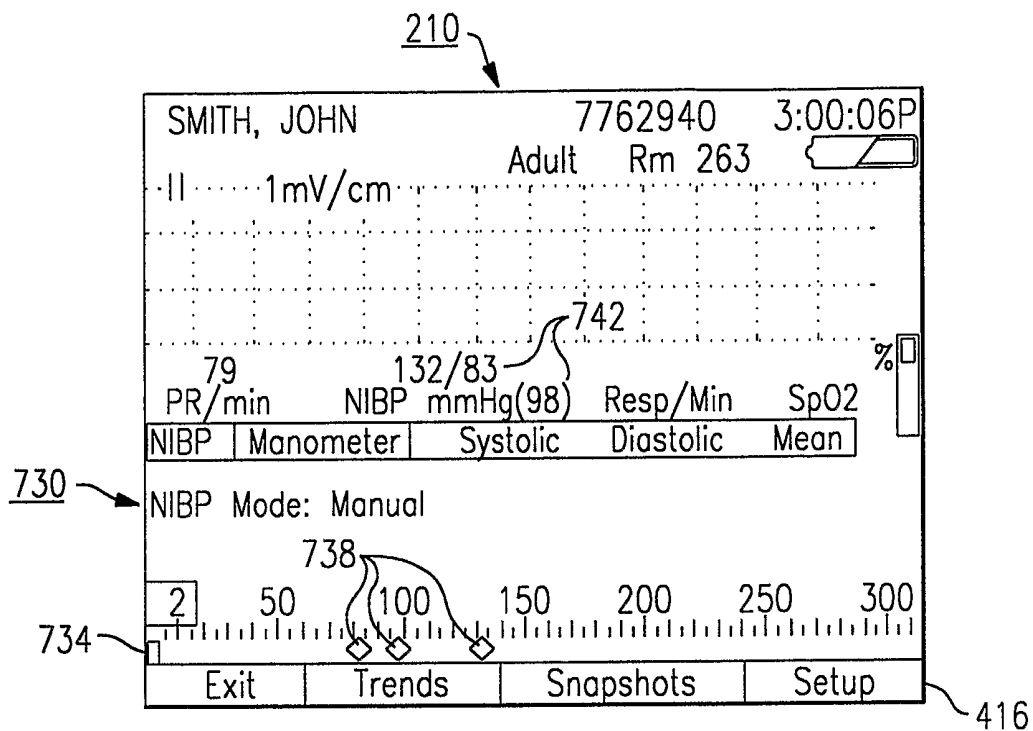
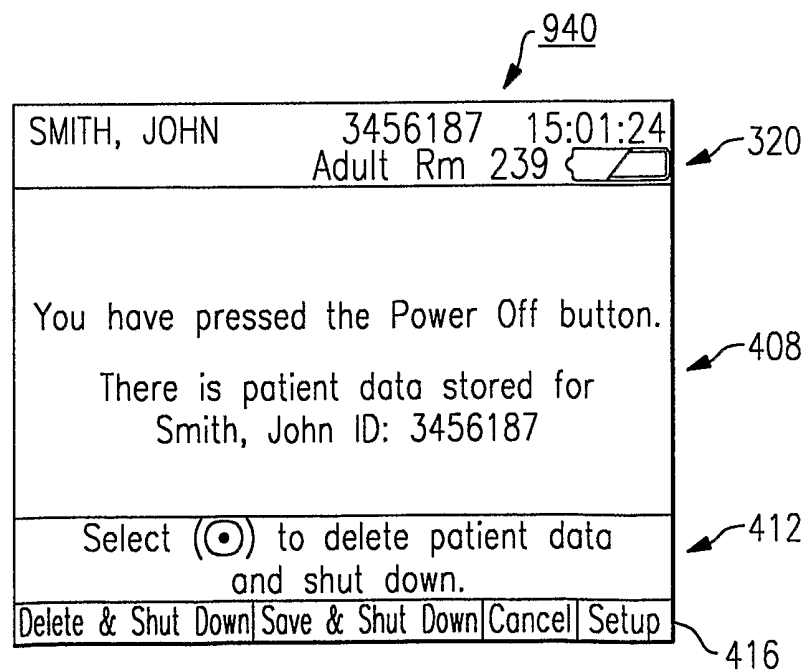
**FIG.34****FIG.35**

FIG.36**FIG.37****FIG.38**

**FIG.39**



**FIG. 44****FIG. 45**

**FIG. 46****FIG. 47**

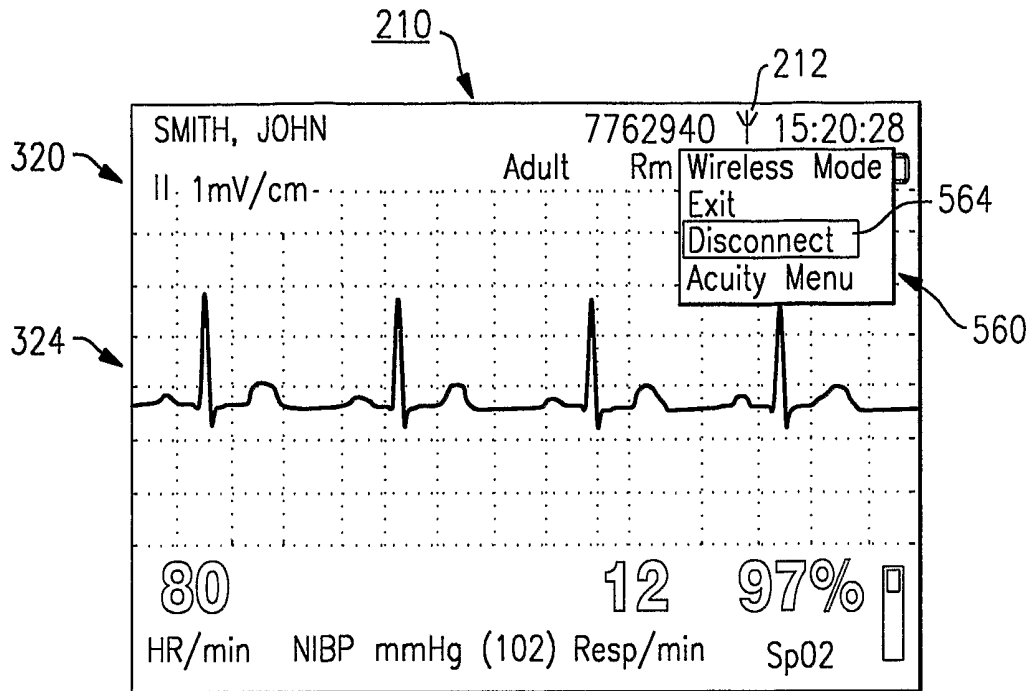


FIG. 48

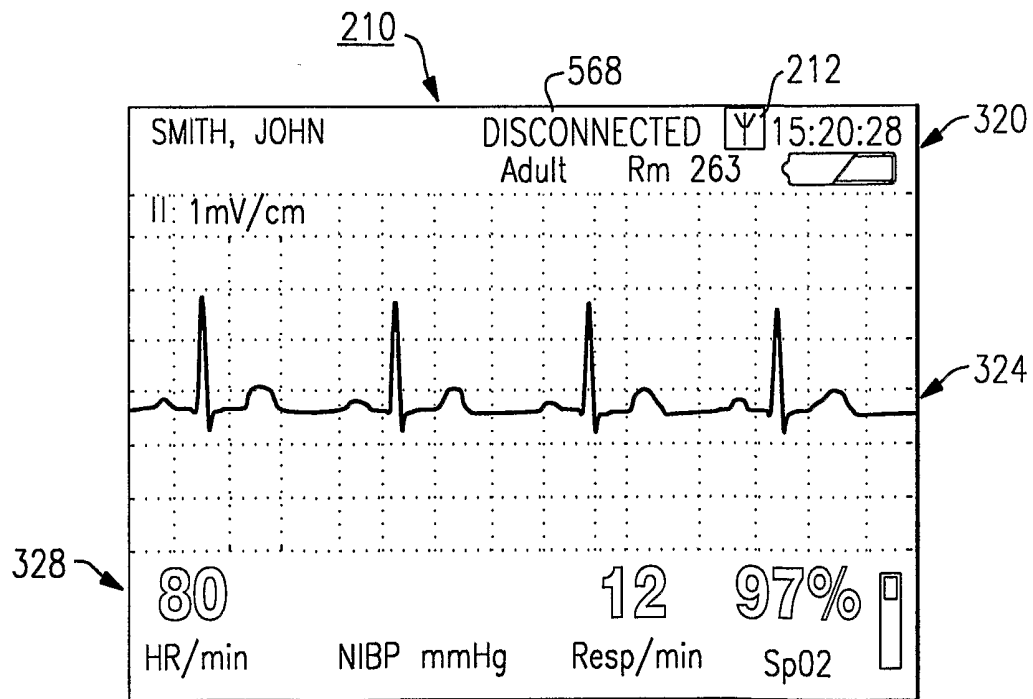


FIG. 49

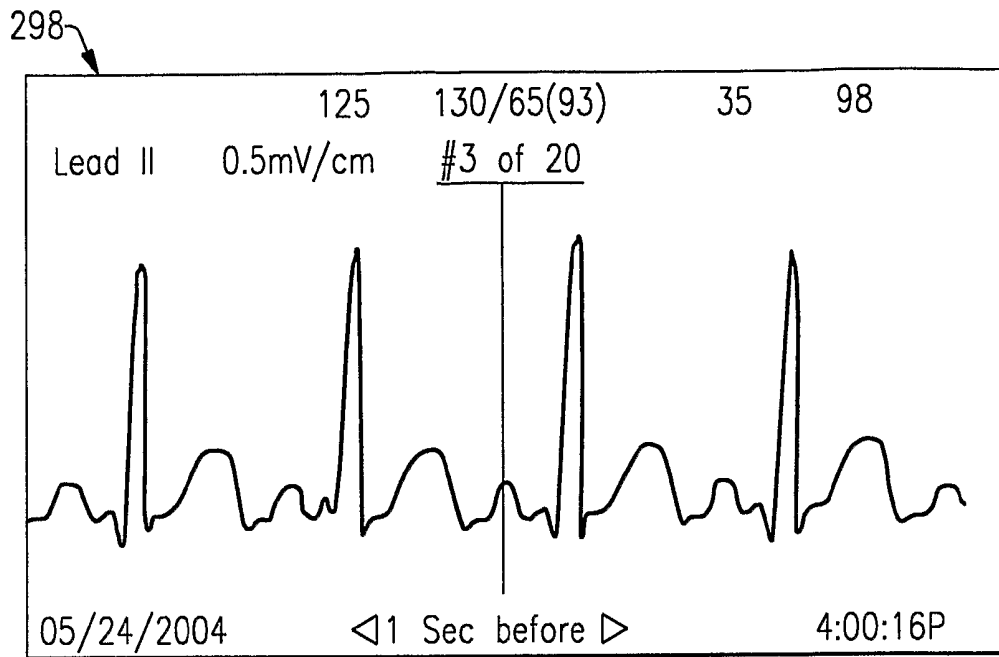


FIG.50

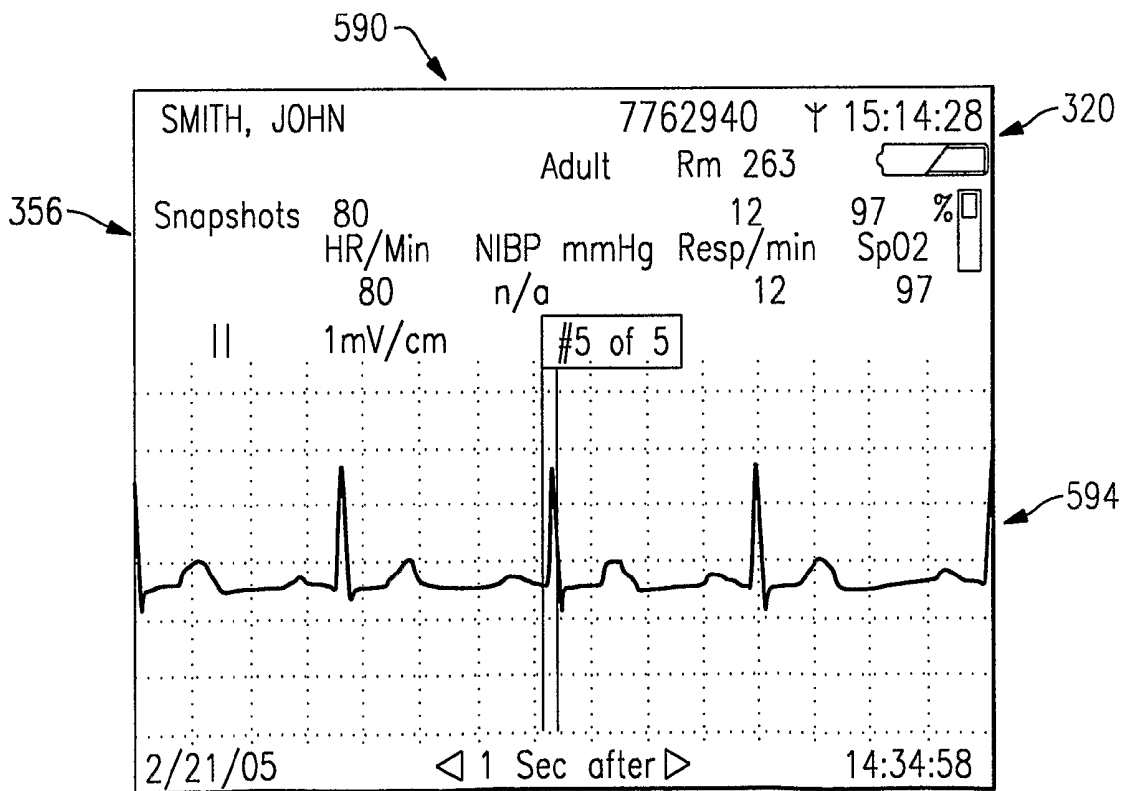


FIG.51

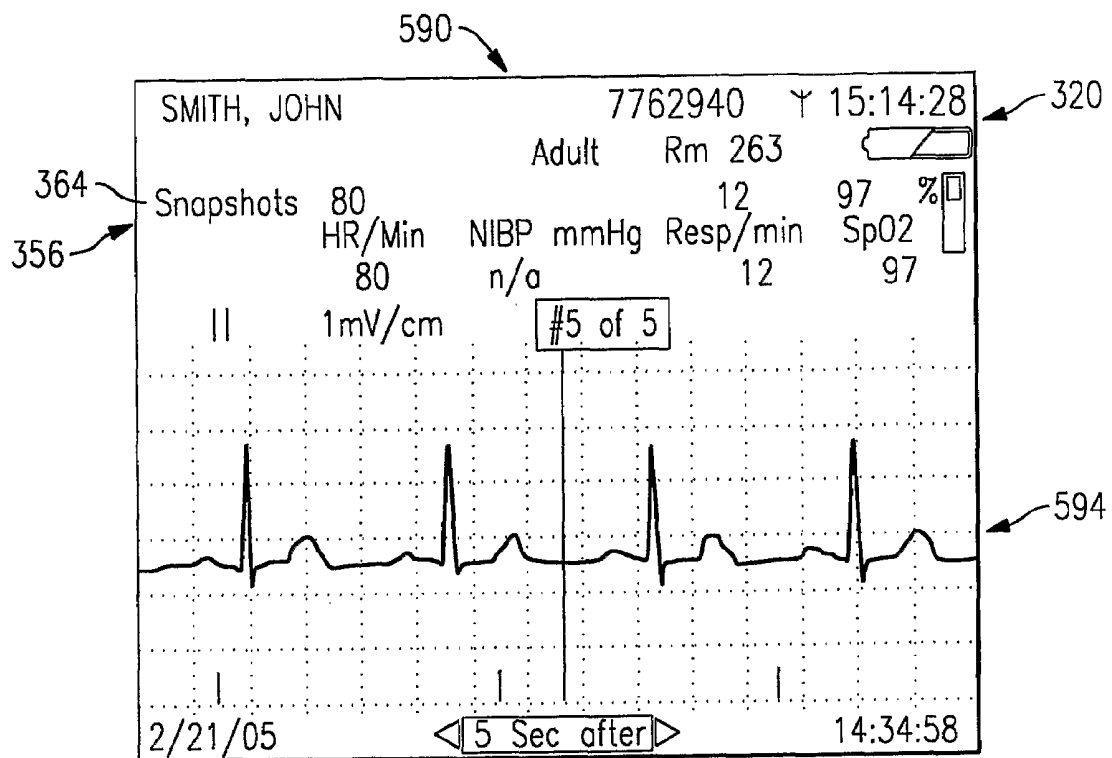


FIG. 52

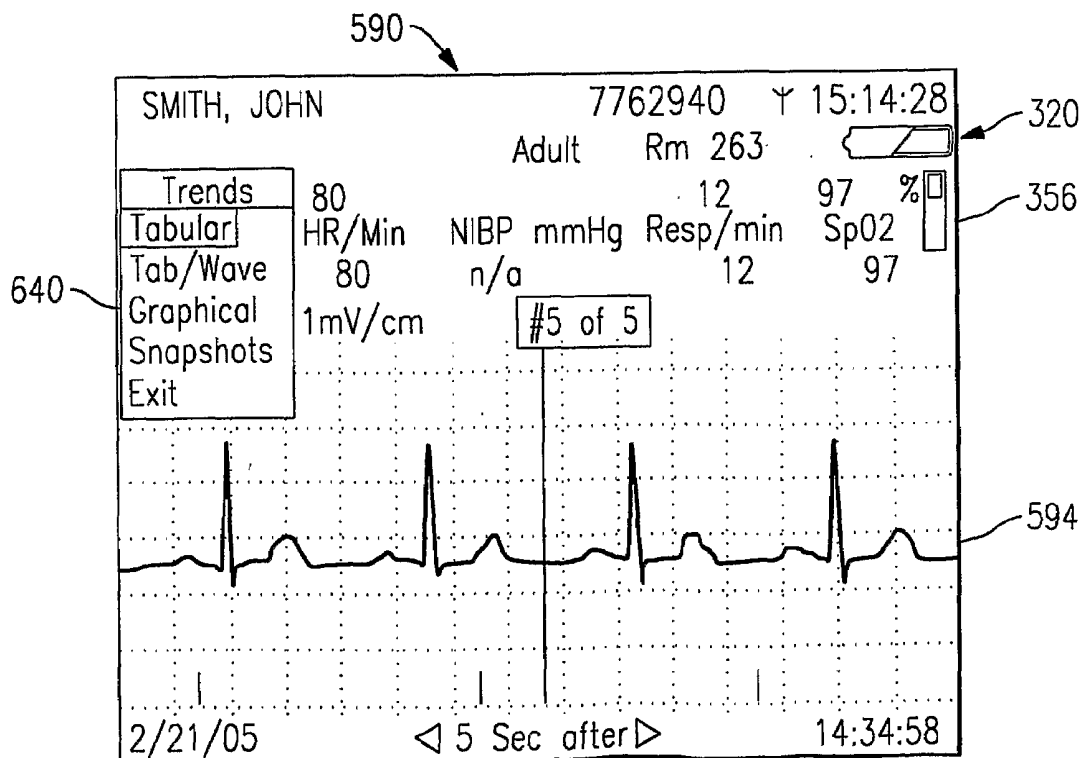


FIG. 53

470

SMITH, JOHN 7762940 Y 04:45:10P 320

Adult Rm 263

356 Tabular 59 120/72(88) 14 98 %

476 Time HR/Min NIBPmmHg Resp/min SpO2

474

477

4:42P	60	121/73(89)	14	99
4:41P	58	119/72(88)	13	98
4:40P	59	120/72(88)	14	98
4:40P	59	120/72(88)	14	99
4:39P	60	118/71(87)	13	98
4:39P	60	118/71(87)	14	98
4:38P	59	120/71(88)	14	98
4:37P	60	119/71(87)	14	99
4:36P	60	117/70(86)	13	98
4:35P	60	120/72(88)	14	98
4:35P	60	120/72(88)	13	99
4:34P	59	119/72(88)	13	98

FIG.54

470

SMITH, JOHN

7762940 Y 04:45:12P

Adult Rm 263

Tabular 59

120/72(88)

14

98

%

View Interval in

NIBPmmHg

Resp/min

SpO2

1 min

121/73(89)

14

99

5 min

119/72(88)

13

98

10 min

120/72(88)

14

98

15 min

120/72(88)

14

99

30 min

118/71(87)

13

98

60 min

118/71(87)

14

98

4:38P 59

120/71(88)

14

98

4:37P 60

119/71(87)

14

99

4:36P 60

117/70(86)

13

98

4:35P 60

120/72(88)

14

98

4:35P 60

120/72(88)

13

99



4:34P 59

119/72(88)

13

98

FIG.55

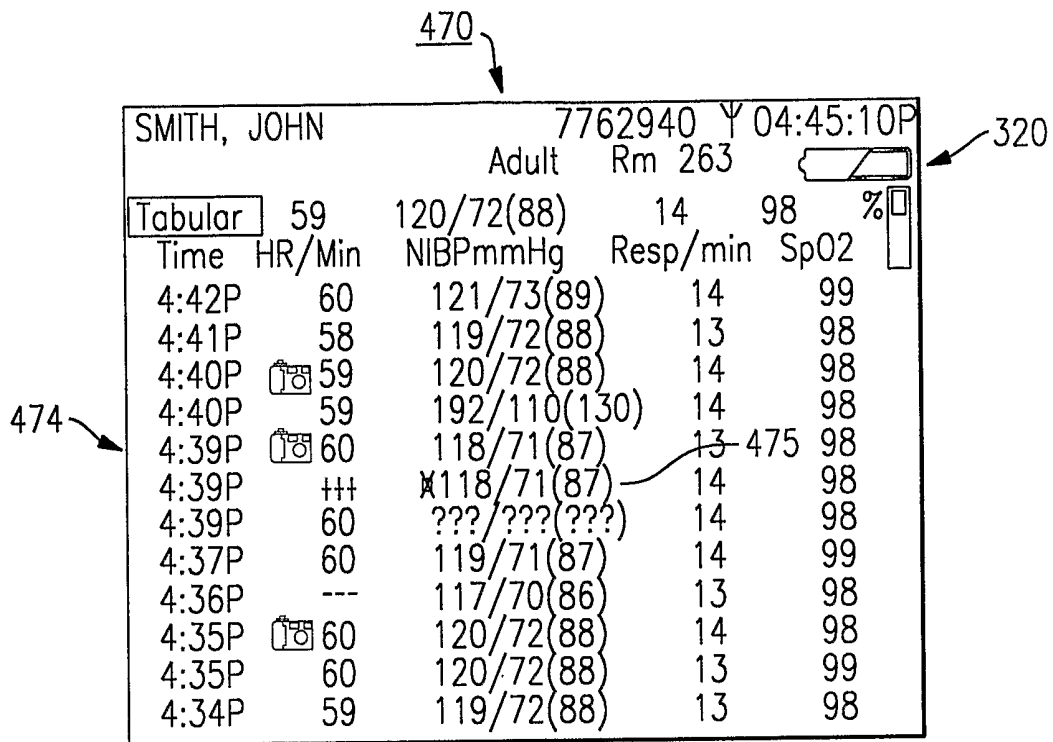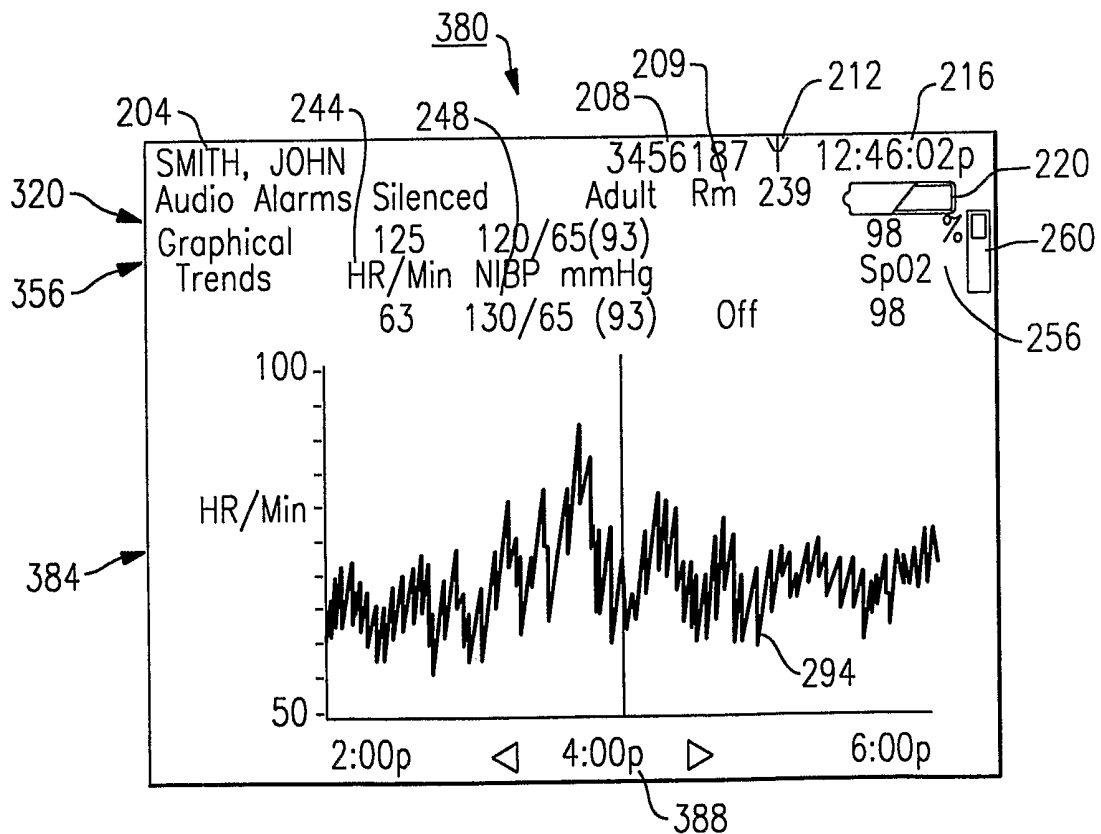**FIG.56****FIG.57**

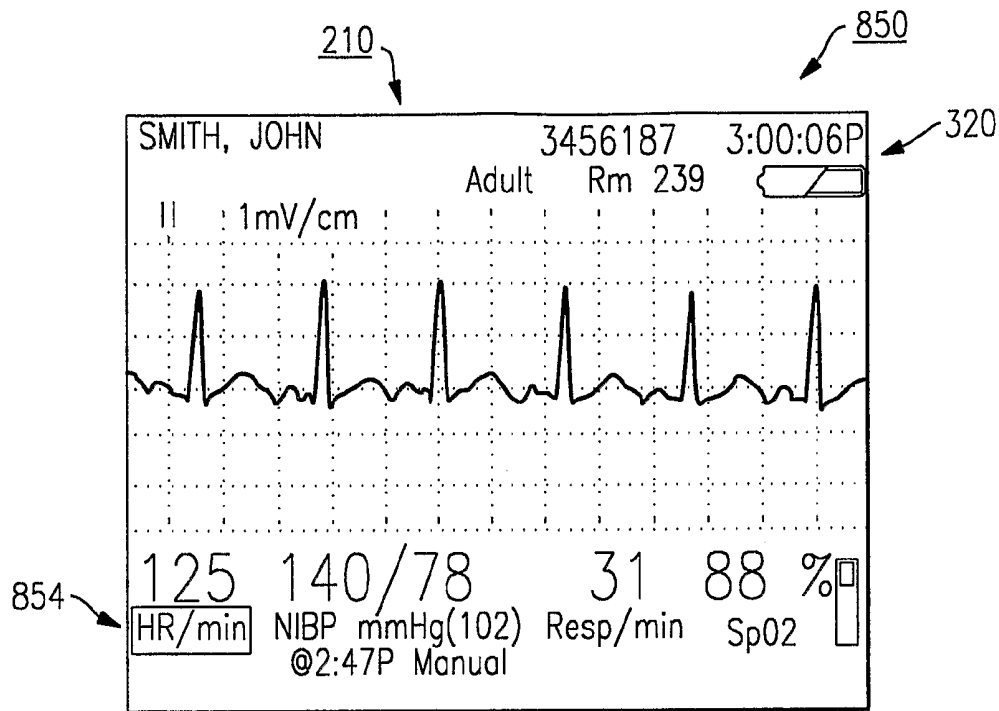


FIG. 58

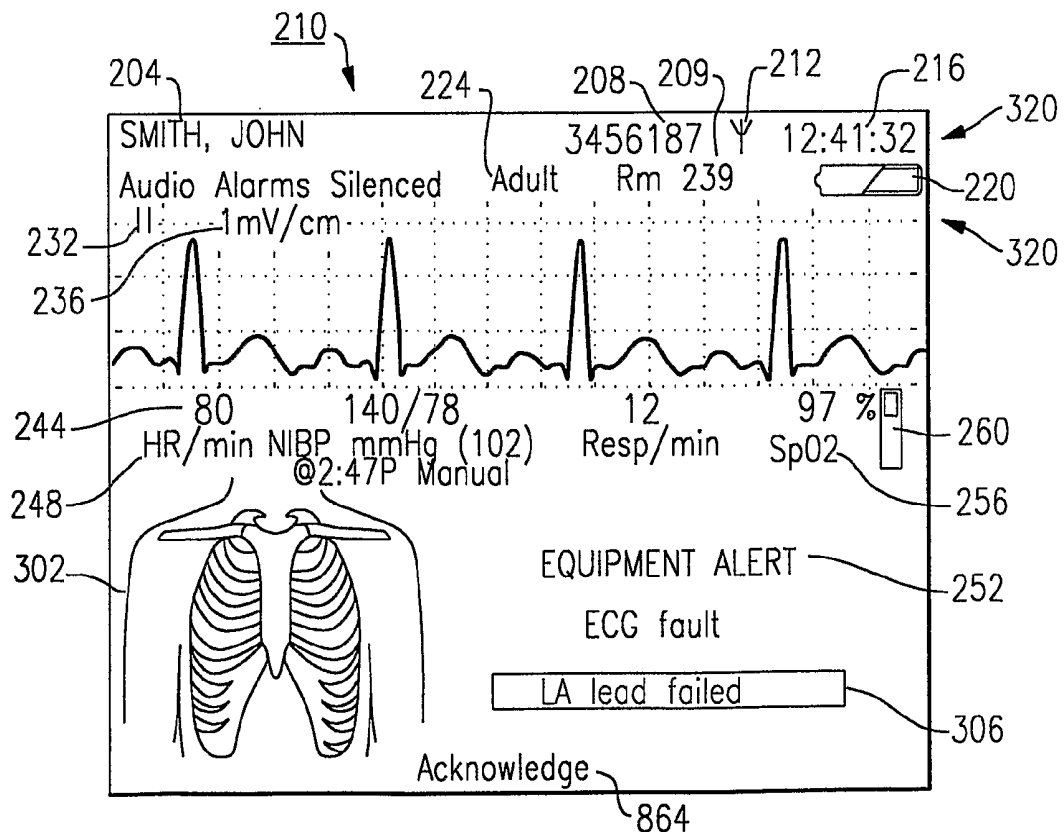
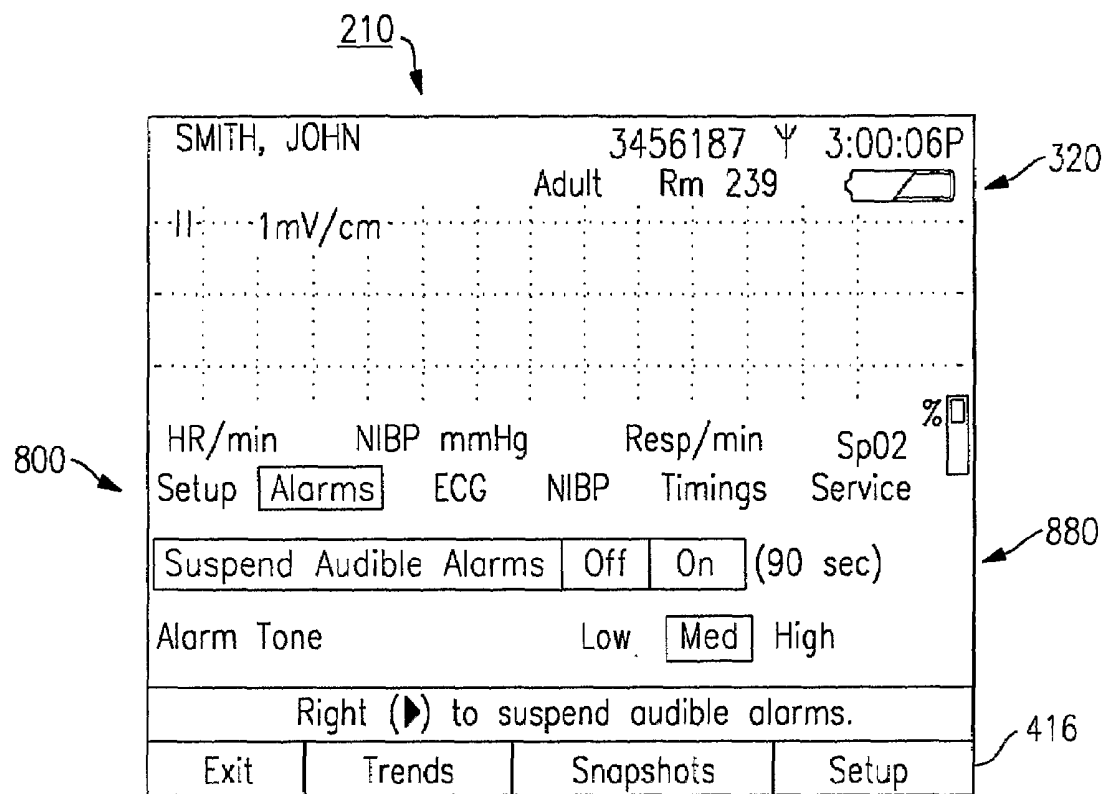
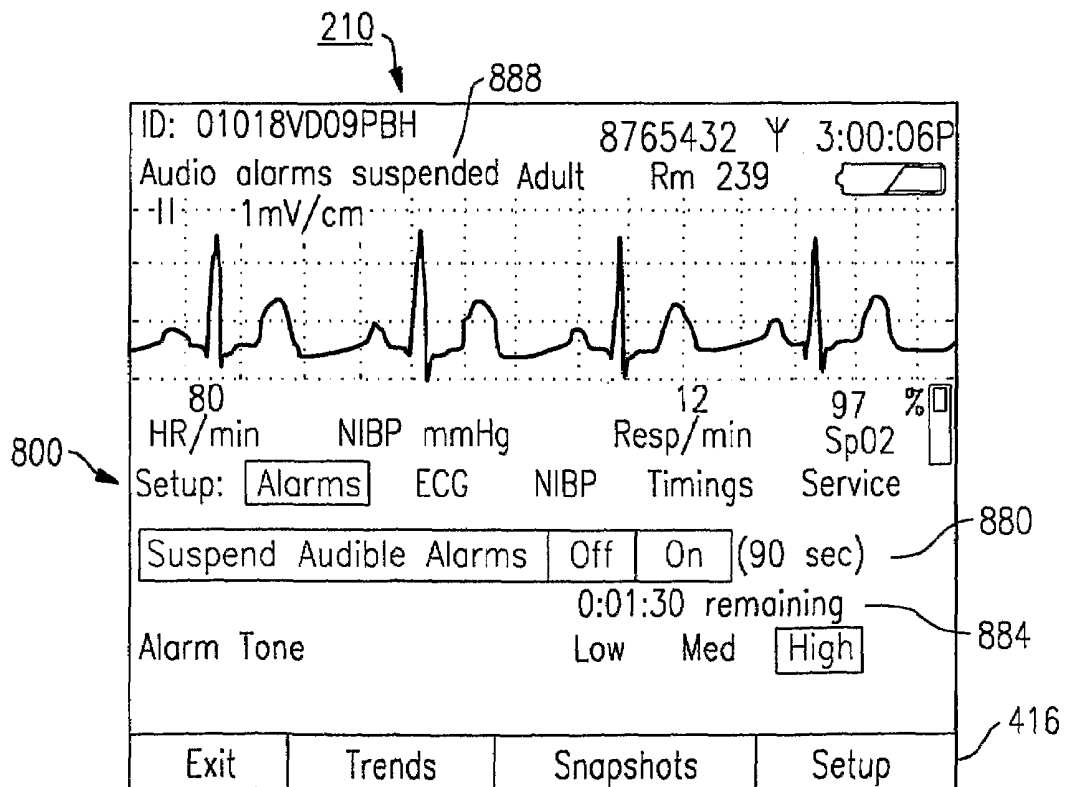


FIG. 59

**FIG. 60****FIG. 61**

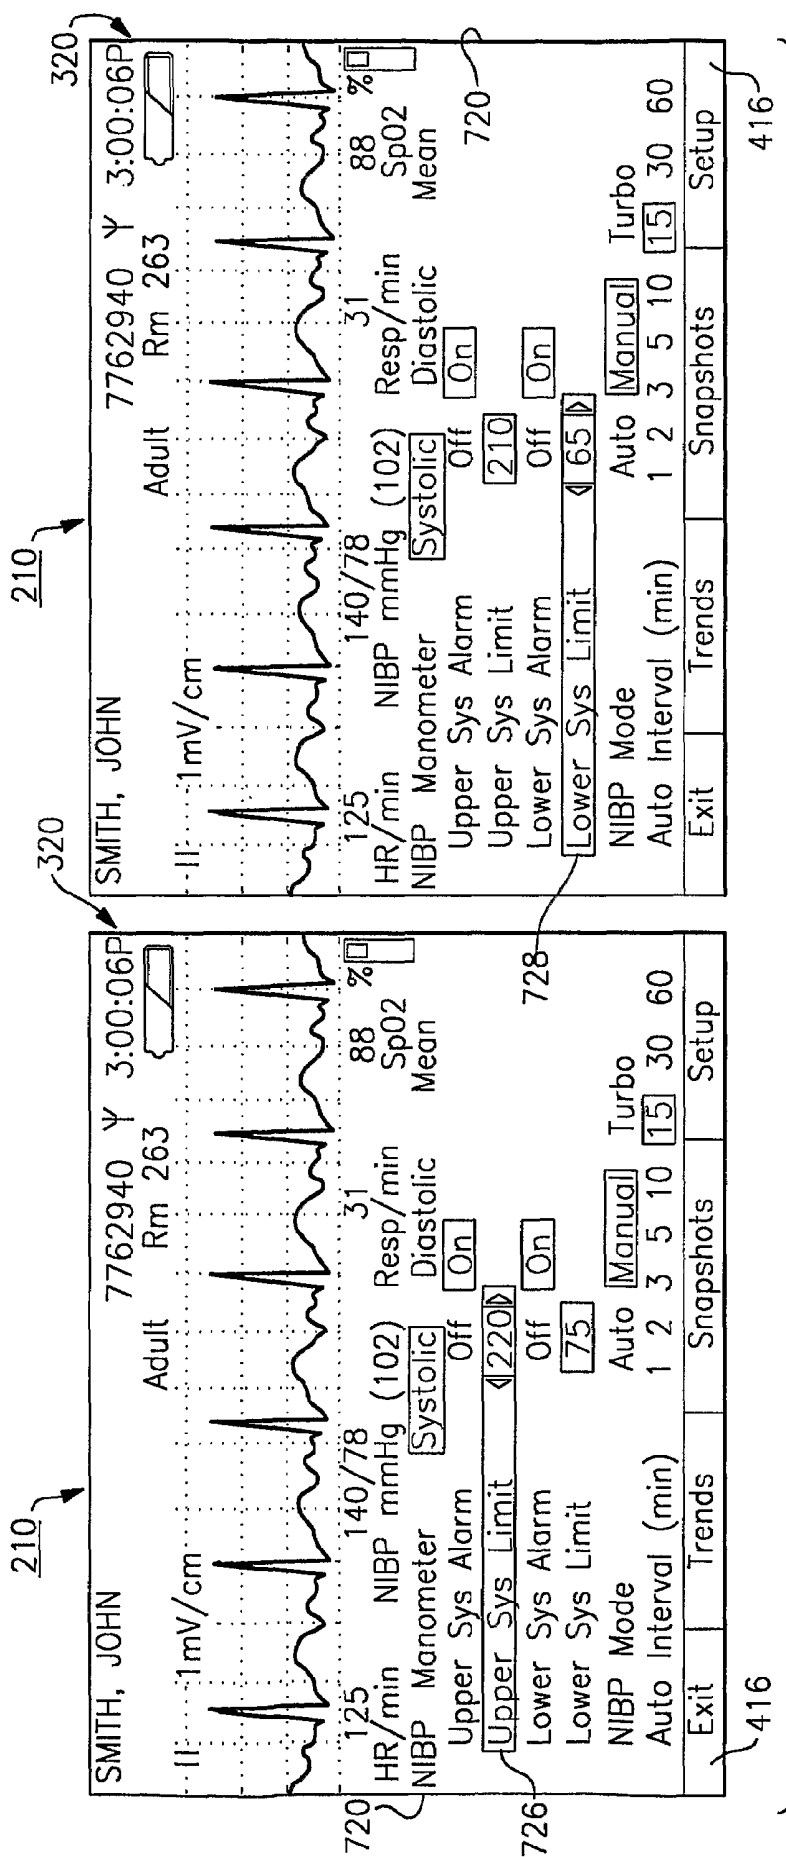


FIG. 62

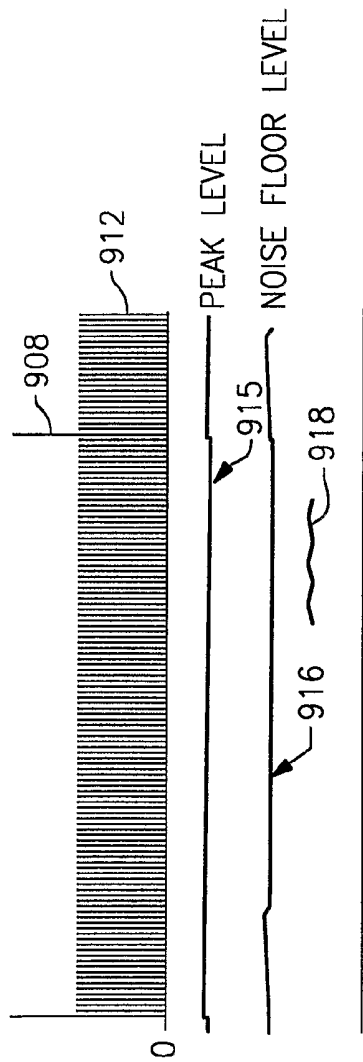


FIG. 63

950 ↗

PARAMETER	ALARMING LEVEL	ALARM LIMIT (PARAMSET =5%)	ALARM LIMIT (PARAMSET =10%)	ALARM LIMIT (PARAMSET =15%)	ALARM LIMIT (PARAMSET =20%)	ALARM LIMIT (PARAMSET =25%)	
HR/PR	UPPER	90	94	99	104	108	113
	LOWER	60	57	54	51	48	45
NIBP	UPPER	140	147	154	161	168	175
	SYSTOLIC LOWER	100	95	90	85	80	75
NIBP	UPPER	90	94	99	104	108	113
	DIASTOLIC LOWER	60	57	54	51	48	45
NIBP MAP	UPPER	107	112	118	123	128	134
	LOWER	73	69	66	62	58	55
SpO2	UPPER	100	100	100	100	100	100
	LOWER	90	86	81	77	72	68
RESP	UPPER	20	21	22	23	24	25
	LOWER	12	11	11	10	10	9

FIG. 65

198

8.1 ParamSet Enable

Do you want to enable ParamSet?

197 ☒ (Yes)
☐ (No)Note If you select ☐ (No), disregards the rest of the ParamSet settings.

8.2 ParamSet % for Upper HR/PR

ParamSet increases the Upper HP/PR limit ____%. (5, 10, 15, **20**, 25)

8.3 ParamSet % for Lower HR/PR

ParamSet decreases the Lower HP/PR limit ____%. (5, 10, 15, **20**, 25)

199

8.4 ParamSet % for Upper NIBP Systolic

ParamSet increases the Upper NIBP Systolic limit by ____%. (5, 10, **15**, 20, 25)

8.5 ParamSet % for Lower NIBP Systolic

ParamSet decreases the Lower NIBP Systolic limit by ____%. (5, 10, **15**, 20, 25)

8.6 ParamSet % for Lower NIBP Diastolic

ParamSet increases the Upper NIBP Diastolic limit by ____%. (5, 10, **15**, 20, 25)

8.7 ParamSet % for Lower NIBP Diastolic

ParamSet decreases the Lower NIBP Diastolic limit by ____%. (5, 10, **15**, 20, 25)

8.8 ParamSet % for Upper NIBP Mean

ParamSet increases the Upper NIBP Mean limit by ____%. (5, **10**, 15)

8.9 ParamSet % for Lower NIBP Mean

ParamSet decreases the Lower NIBP Mean limit by ____%. (5, **10**, 15)8.10 ParamSet % for Upper SpO₂ParamSet increases the Upper SpO₂ limit by ____%. (**5**, 10)8.11 ParamSet % for Lower SpO₂ParamSet decreases the Lower SpO₂ limit by ____%. (**5**, 10)

8.12 ParamSet % for Upper Resp

ParamSet increases the Upper Resp limit by ____%. (**5**, 10, 15, 20, 25)

8.13 ParamSet % for Lower Resp

ParamSet decreases the Lower Resp limit by ____%. (**5**, 10, 15, 20, 25)**FIG.64**

VITAL SIGNS MONITOR**CROSS REFERENCE TO RELATED APPLICATIONS**

The following patent application is a national stage application based upon PCT/US/2006/001093, entitled: Vital Signs Monitor, filed Jan. 13, 2006, claiming priority of U.S. Ser. No. 60/643,636, filed Jan. 13, 2005, the entire contents of each above noted application being herein incorporated by reference in its entirety.

FIELD OF THE INVENTION

The invention relates to the field of medical diagnostic instruments and in particular to a portable, battery powered, multi-parametric, vital signs monitoring device that can be used for both ambulatory and transport applications as well as bedside monitoring. The device can be used with an optional charging cradle that supplies power and charges the contained battery. The charging cradle can additionally serve to provide an isolated data link to an interconnected portable computer allowing snapshot and trended data from the monitoring device to be printed automatically and also allowing default configuration settings to be downloaded to the monitoring device. The monitoring device is capable of use as a stand-alone unit as well as part of a bi-directional wireless communications network that includes at least one remote monitoring station.

BACKGROUND OF THE INVENTION

A number of vital signs monitoring devices are known that are capable of measuring multiple physiologic parameters of a patient wherein various sensor output signals are transmitted either wirelessly or by means of a wired connection to at least one remote site, such as a central monitoring station. U.S. Pat. No. 5,319,363 describes a wired version of such a device and network, while U.S. Pat. Nos. 6,544,173 and 6,544,174 each describe a multi-parametric vital signs monitoring device that is linked by means of a bi-directional wireless communications network with at least one central monitoring station, usually located at a nurse's station on a hospital floor or Intensive Care Unit (ICU). Such monitoring systems have dramatically improved the manner in which patients can be monitored during a hospital stay. However, there is a perceived need in the field to provide a patient monitoring device that is truly versatile, such that the device can be selectively used for bedside as well as ambulatory applications in order to more effectively cover the varied number of situations a monitored patient may encounter, but without a loss in device (e.g., monitoring) connection with that patient or in obtaining required physiologic data.

There are additional concerns that exist in the field of patient vital signs monitoring. For example, the nature of monitoring devices that continuously monitor SpO₂ (blood oxygen saturation) levels of a patient can cause false or nuisance alarms, particularly those patients who are of lower acuity or are ambulatory. Traditional continuous monitors of this type are found in ICU, OR, ED, PACU and other specialty beds, for the most part. The majority of hospital beds, on the other hand, are found in medical-surgical and/or general care areas in which non-continuous, spot-checking monitoring devices are primarily used. It is believed that present hospital healthcare dynamics, such as the general shortage of nurses, has increased pressure for regulatory compliance, rising costs, and higher acuity in patient census. The latter, it is

further believed, could cause a convergence of continuous monitoring and spot-checking to the un-monitored beds of the hospital. A very large challenge or barrier to this trend is that clinical staff members on medical surgical floors are generally ill-trained or adequately skilled in the use of continuous medical monitoring devices.

There is yet another general need in the field of patient vital signs monitoring to improve the level of alarm management with regard to existing physiologic monitoring devices. Most known devices of this type include at least one visual and/or audible alarm that is produced, typically both at the monitoring device (e.g., bedside) as well as at the central monitoring station. According to one currently known monitoring system, the preset upper and lower alarm limits for all physiologic parameters can be automatically changed simultaneously a single time by a user simultaneously by a specified percentage (e.g., 20 percent). While this form of management/updates is often suitable for certain parameters, such as heart rate, it is not practicable for other parameters (e.g., SpO₂). Though some monitoring devices further permit manual adjustment of alarm limits, this adjustment can be a somewhat time consuming and tedious process. As a result, there is a general desire to improve alarm management over presently known patient monitoring devices.

Additionally, there are also a number of patient monitoring devices that can indicate when an electrode assembly, such as those used for ECG electrode assemblies, has already reached failure or has become detached from the patient, such as those described by U.S. Pat. No. 5,819,741 to Karlsson et al. It would be even more desirable, however, to provide a patient monitoring device that can in addition to the above features proactively detect the onset of failure in at least one leadwire/electrode such that the at least one electrode or leadwire could be retrofitted in advance of having the ECG electrode assembly fail during examination or during rounds.

It is a desirable function of any cardiac monitoring device to provide sufficient information so that a clinician can discern if an implanted cardiac pacemaker is operating properly. Basically, it is desirable to include in the ECG waveform a highly visible indication each time the pacemaker fires. As the technology for implanted pacemakers and implanted pacing electrodes has evolved, the magnitude and duration of the pulses that result at the body surface have reduced, making these pulses more difficult to detect. Furthermore, the observed pacer pulse amplitude is smaller in some ECG vectors than in others. Which ECG vectors have the strongest pacer pulse signals is dependent on body surface ECG electrode placement and the location of the implanted pacemaker electrodes, and therefore the detection issues vary from patient to patient. Making the pacer pulse detector in an ECG monitoring device be able to detect smaller amplitude, shorter duration spikes unfortunately causes the detector to trigger more often on the electrical noise spikes that often occur in the patient's vicinity. Faulty incandescent light dimmers, fluorescent lights, electronic power supplies, and other assemblies generate electromagnetic interference (EMI) and other sources of electronic noise may generate such noise spikes, these spikes occurring at a rate that is twice the frequency of the power line. If a pacer pulse detector is triggered this rapidly, it is extremely difficult for the monitoring device to calculate an accurate heart rate. The extent to which these noise spikes affect a pacer pulse detector is further affected by the contact impedance of the body surface ECG electrodes—higher impedance connections make it more likely that these noise spikes will trigger the pacer pulse detector. For each of the foregoing reasons it is therefore desirable to be able to select as an input to a monitor's pacer detector, an ECG vector

that contains real pacer pulses whose amplitude is sufficiently above the detection threshold, and which also contains environmental noise spikes whose amplitudes are sufficiently below the detection threshold. To that end, it would be desirable to be able to identify localized areas or sources of electrical noise, in order to permit the clinician to move the patient and/or noise source and thereby avoid instances of premature alerts or other similar situations.

It is yet another general desire in the field of remote monitoring to provide a multiple physiologic parameter monitoring device that is more user-friendly than previous devices of this type; that is, a device that can be more easily and effectively used by staff of varying skill levels.

Still further, there is a general need to provide a more rugged and durable patient monitoring device, given that such devices are finding increased uses, for example, in military field applications, requiring devices of this type to be much more tolerant to shock and environmental loads than those found in classical hospital environments.

SUMMARY OF THE INVENTION

According to an aspect of the present invention, there is herein described a portable, lightweight and battery powered vital signs monitoring device that is capable of being used as an ambulatory or transport monitor and which is optionally patient-wearable. In spite of its lightweight design defined by a compact profile for ease of transport and handheld use, the device is defined by a rugged design that is intended to withstand shock, impact and/or other loads that could be present in literally any patient-related setting or application.

The herein-described monitoring device can also be used in connection with a charging cradle, permitting use of same as a bedside monitor, wherein the charging cradle provides power for the monitoring device in lieu of the contained battery and provides charging for same. In addition, the monitoring device and cradle further permit mounting of same, for example, to either a bed rail and/or a fluid (IV) pole, as needed, or to a large display connected as a peripheral to the device as mounted in the cradle with the cradle having a data port permitting the pass through of data.

The monitoring device further optionally includes an integrated wireless transceiver and antenna, permitting communication bi-directionally with at least one remote station, such as a central monitoring station, over a wireless network. The monitoring device can operate to transmit patient data whether the device is connected to the charging cradle or while in use as a stand-alone unit.

The charging cradle according to one aspect of the present invention further can permit a data-link connection between the monitoring device and a portable computer (PC). According to one version of the invention, the PC can be equipped with configuration utility software and used in order to custom configure the monitoring device for specified usage in a hospital or facility; for example, a neonatal ward. According to another version, the monitoring device is storing "snapshot" data and trended data to be manually or automatically transmitted for printing using the PC with the connected charging cradle acting as an intermediary or pass through device. Alternatively, the charging cradle permits the monitoring device to transmit patient data in a real-time fashion, such as to a large display via the serial connection.

The monitoring device according to another aspect of the present invention is connectable to a plurality of physiologic sensor assemblies wherein multiple patient parameters can be measured, including, for example, blood pressure, SpO₂, ECG, pulse/heart rate and respiration. The monitoring device

includes an integrated display to indicate the status of the measured physiologic parameters, as well as a user interface, including a keypad, that permits the user to selectively display various output or display modes, including both tabular and graphical data trending of at least one monitored physiologic parameter, as well as to view status of the monitoring device, including connectivity with the wireless network, available power to operate the monitoring device, and other features.

According to yet another aspect of the present invention, the user interface of the monitoring device permits navigation using a series of embedded menus using the keypad (user interface), thereby minimizing the time required for the clinician to obtain relevant data and further permitting highly skilled as well as less skilled clinical staff to equally and effectively utilize the monitoring device. The device further includes security features wherein the buttons of the user interface and/or the display can be locked out or disabled in order to prevent any unauthorized use and power-saving features wherein the display is automatically powered down based on a lack of activity or in which certain assemblies are made inoperative (i.e., NIBP) when a low battery condition exists. In addition and in a wireless version in which the herein described monitoring device is out of range, the wireless data transmission feature can selectively be deactivated until the device is again in range of the network.

According to still another version of the present invention, the user interface is additionally configured to assist the user in terms of alarm management. According to this version of the present invention, upper and/or lower alarm settings or limits for specified measured parameters can be selectively incremented by preset percentage amounts, as needed, during the occurrence of an existing alarm. Additionally, all parameters can be similarly adjusted simultaneously, as needed.

According to yet another aspect of the present invention, the monitoring device permits continuous measurement of certain physiologic parameters, including pulse oximetry. The device, however, can be selectively configured by the user such that the remaining physiologic parameters, such as ECG, can continue to be monitored in the usual manner while SpO₂ readings of a patient can be selectively random or spot checked by the user of the monitoring device.

An advantage of the present invention is that a multi-parametric monitoring device is provided that can be used in literally any patient setting, allowing the device to be used for monitoring a patient on hospital medical-surgical, telemetry and intermediate floors, hospital emergency departments, transport, emergency medical services and/or other health-care applications. As such, the herein described monitoring device can be used for and/or between bedside, ambulatory, transport or other similar applications seamlessly.

Moreover, the rugged construction, compact design and adaptability between various bedside and transport applications make the herein described monitoring device extremely useful for military and other similar purposes.

Another advantage of the present invention is that the herein described monitoring device can be custom configured to enable the device to be used in a specific facility. The device can also be temporarily configured for a current patient, wherein settings can be selectively retained for the patient or deleted along with stored data upon power down of the device, thereby facilitating use between patients.

These and other aspects, features and advantages will become readily apparent from the following Detailed Description as well as the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a front view of a vital signs monitoring device in accordance with an embodiment of the present invention;

FIG. 2 is a front perspective view of the vital signs monitoring device of FIG. 1;

FIG. 3 is a top plan view of the vital signs monitoring device of FIGS. 1 and 2;

FIG. 4 is a front perspective view of a charging cradle that is used in connection with the vital signs monitoring device of FIGS. 1-3;

FIG. 5 is a front view of the vital signs monitoring device of FIGS. 1-3 as mounted in the charging cradle of FIG. 4;

FIG. 6 is a schematic block diagram of a patient monitoring system including the vital signs monitoring device of FIGS. 1-3 and the charging cradle of FIG. 4;

FIG. 7 is another front view of the vital signs monitoring device of FIGS. 1-3 as mounted in the charging cradle of FIGS. 4 and 5, illustrating the user interface thereof;

FIG. 8 is a front view of the vital signs monitoring device of FIGS. 1-3 with an attached strap permitting hand-held operation thereof;

FIG. 9 is an alternative view of the vital signs monitoring device of FIGS. 1-3 using a patient-wearable harness;

FIG. 10 depicts the vital signs monitoring device of FIGS. 1-3, as used in a patient transport application;

FIG. 11 depicts the vital signs monitoring device of FIGS. 1-3 as mounted to a bed rail and attached to a large display;

FIG. 12 depicts the vital signs monitoring device of FIG. 11 as attached to a charging cradle and an interface housing for the large display;

FIG. 13 depicts the vital signs monitoring device of FIGS. 11 and 12 as mounted in a charging cradle and directly attached to the large display;

FIG. 14 illustrates two sample display screens indicative of the information that can be captured by the vital signs monitoring device of FIGS. 1-3 and displayed by the large display;

FIG. 15 illustrates an example of a display screen of the vital signs monitoring device of FIGS. 1-3 according to one display mode;

FIG. 16 depicts another example of a display screen of the vital signs monitoring device according to another display mode for the vital signs monitoring device of FIGS. 1-3;

FIG. 17 depicts yet another exemplary display screen according to yet another display mode for the vital signs monitoring device of FIGS. 1-3;

FIG. 18 depicts yet another example of a display screen according to yet another display mode for the vital signs monitoring device of FIGS. 1-3 showing trended tabular data;

FIG. 19 depicts the toggling between various display modes using the vital signs monitoring device;

FIG. 20 illustrates another display screen showing how the display cursor is used to highlight a displayed item to permit navigation;

FIG. 21 illustrates another example of a display screen of the vital signs monitoring device of the present invention and illustrating how the SELECT button is used to select a highlighted item for navigation;

FIG. 22 is an exemplary control menu accessed through selection of the highlighted item of the display screen of FIG. 21;

FIG. 23 depicts another exemplary control menu for the vital signs monitoring device in accordance with the present invention;

FIG. 24 depicts side by side examples of display screens presented to a user of the vital signs monitoring device upon powering up of the device, depending upon whether patient-related data and settings have been previously stored by the device;

FIG. 25 is an exemplary set-up menu for the vital signs monitoring device;

FIG. 26 is an exemplary set of information display windows for the vital signs monitoring device;

FIG. 27 is a configured data display screen of the vital signs monitoring device in which patient information is being entered;

FIG. 28 is another display screen depicting a patient information entry panel of the display screen of FIG. 27;

FIG. 29 depicts an exemplary change patient mode menu for the display screen of the vital signs monitoring device of FIGS. 1-3;

FIG. 30 depicts a confirmation display screen that is displayed by the vital signs monitoring device in accordance with the invention when a patient mode is changed by the user;

FIG. 31 is an exemplary display screen of the vital signs monitoring device of the present invention including a time/date control menu;

FIG. 32 is an exemplary display screen of the vital signs monitoring device of the present invention including a waveform source menu;

FIG. 33 is another exemplary display screen of the vital signs monitoring device depicting a different waveform source;

FIG. 34 is another exemplary display screen of the vital signs monitoring device including a waveform size menu;

FIG. 35 is a display screen of the vital signs monitoring device depicting an ECG set-up menu in accordance with an aspect of the present invention;

FIG. 36 is another example of a function performed in the ECG set-up menu of FIG. 35;

FIG. 37 is an exemplary respiration waveform as displayed by the vital signs monitoring device;

FIG. 38 depicts a portion of an exemplary display screen of the monitoring device and in particular an SpO₂ control menu;

FIG. 39 is a flow chart relating to a SpO₂ spot checking feature of the vital signs monitoring device of FIGS. 1-3;

FIG. 40 is an exemplary display screen of the vital signs monitoring device of the present invention, including a primary vital signs display screen with the SpO₂ icon highlighted after SpO₂ has been turned off;

FIG. 41 is a drop down pulse oximeter spot check menu accessed through the window navigation of FIG. 40;

FIG. 42 is an exemplary display screen detailing portions of the SpO₂ spot-check feature in accordance with the present invention;

FIG. 43 is a later version of the display screen of FIG. 42 illustrating pulse oximetry data;

FIG. 44 is an exemplary display screen of the vital signs monitoring device illustrating a digital manometer feature;

FIG. 45 is the display screen of FIG. 44 at a later time during an NIBP reading, in progress;

FIG. 46 is the display screen of FIGS. 44 and 45 at a later time following the NIBP measurement including depicting markers/indicators for the user with respect to systolic, diastolic and mean pressure values;

FIG. 47 is an exemplary Power Off display screen of the vital signs monitoring device;

FIG. 48 is an exemplary display screen of the vital signs monitoring device depicting in part, a wireless mode drop-down menu;

FIG. 49 is a display screen accessed and displayed by the vital signs monitoring device when the device is disconnected from the wireless network;

FIGS. 50-52 depict examples of an exemplary display screen according to yet another display mode for the vital

signs monitoring device of FIGS. 1-3 illustrating snapshots of vitals signs data captured by the device;

FIG. 53 depicts a snapshot display screen similar to FIGS. 50-52, but further including a trends data selection menu;

FIGS. 54-56 depict various exemplary display screens of tabular trended patient data as displayed by the vital signs monitoring device of the present invention;

FIG. 57 depicts yet another example of a display screen according to yet another display mode for the vital signs monitoring device of FIGS. 1-3, showing trended graphical data;

FIG. 58 depicts an exemplary alarm display screen of the vital signs monitoring device of FIGS. 1-3;

FIG. 59 depicts an exemplary equipment alert display screen of the vital signs monitoring device of FIGS. 1-3;

FIGS. 60 and 61 illustrate exemplary display screens for the vital signs monitoring device, including an alarms set-up menu in which audible alarms can be enabled or disabled;

FIG. 62 illustrates examples of display screens in accordance with the present invention, including a parameter control menu wherein alarm limits can be temporarily customized for an individual patient;

FIG. 63 is a signal output indicating how electrical noise can be discriminated from pacer signals as detected by the device from a selected ECG vector; and

FIGS. 64 and 65 depict portions of an exemplary configuration worksheet used for configuring individual alarm limit settings to predetermined percentage amounts for the monitoring device in accordance with one version of the invention.

DETAILED DESCRIPTION

The following description relates to a specific embodiment for a multi-parametric, vital signs monitoring device that can be used universally for a number of different patient-related applications, including ambulatory, bedside, transport, procedure, and handheld operations. It will be readily apparent, however, from the discussion that follows to those of sufficient skill that numerous variations and modifications are possible within the intended scope of the invention. In addition and throughout the text, a number of terms are used in order to provide a suitable frame of reference with regard to the accompanying drawings, including "top", "bottom", "front", "rear", "back", and the like. These terms are not intended to be over limiting of the present invention, except in those instances where specifically indicated.

Referring to FIG. 1, the herein described patient monitoring device 20 is defined by a housing 24 that receives input from a plurality of sensors, each forming part of physiologic sensor assemblies 28, 32 and 36, in this instance ECG, SpO₂ (pulse oximetry) and blood pressure (NIBP) assemblies. The housing 24 includes a display 88 for vital sign numerics, waveforms and other patient data, as well as a user interface 92, FIG. 2, that permits operation of the monitoring device 20.

Referring to FIGS. 1-3, the display 88 is provided on a front facing side of the housing 24, as well as a plurality of adjacent actuable buttons defining the user interface 92. According to the present embodiment, the display 88 is a quarter (QVGA) color display, the display according to this embodiment being approximately 3.5 inches (measured diagonally). More particularly and according to this embodiment, the display 88 is an LCD having a pixel count of 240 by 320. The herein described display 88 preferably includes a backlight (not shown) to improve readability of the display under low ambient light conditions.

As to the profile of the herein described device 20, the housing 24 according to this specific embodiment is approxi-

mately 5.3 inches in height, 7.5 inches in width, and 2.0 inches in depth. In spite of the lightweight design, however, the herein described monitoring device 20 is extremely durable and rugged wherein the device is equipped to handle various loads that may be encountered in a patient-related setting. For example, the housing 24 includes a center or intermediate rubberized bladder 26 disposed between a front housing half and a rear housing half that is disposed peripherally therebetween about the device housing 24 in order to assist in cushioning the monitoring device 20 from impact or shock loads and to retain the interior of the device from dust or other contaminants. To further assist in cushioning the monitoring device 20, each of the corners of the housing 24 are curved to provide an effective contour. A battery compartment (not shown) is also formed within the housing 24, the cover of the battery compartment being essentially flush with the rear facing side 61 of the housing such the compartment does not protrude from the overall profile of the monitoring device 20. The rear facing side 61 of the housing 24 further includes a set of rubberized pads or feet 58, enabling the monitoring device 20 to be placed on a flat surface, as needed. In addition, each of the buttons comprising the user interface 92, discussed in greater detail below, are elastomerized to aid in the overall durability and ruggedness of the monitoring device 20, the buttons being positioned so as not to overly protrude from the facing surface 84 of the housing 24 and allowing the device to maintain a relatively compact profile.

The compact profile of the device housing 24 enables the monitoring device 20 to be patient wearable. A pair of tabs 132, FIG. 2, provided on opposing lateral sides of the device housing 24 enable the monitoring device 20 to be secured to a patient-wearable harness 135, such as shown in FIG. 9, or alternatively a strap 137 can be attached to the side tabs 132, as shown in FIG. 8, permitting hand-held and portable operation of the monitoring device 20. The strap 137 can be used additionally for transport operations along with a transport belt 139, such as shown in FIG. 10, with respect to a gurney 138 or other transport apparatus. Otherwise and as noted above, the herein described monitoring device 20 can be suitably positioned upon a table or other flat surface using the rubberized pads 58 provided on the rear facing side 61 of the device housing 24.

In addition to being compact and durable, the herein described monitoring device 20 is extremely lightweight. The entire assemblage shown in FIG. 1 weighs approximately two pounds.

As noted above and according to this embodiment, a plurality of physiologic sensor assemblies are tethered to the housing 24, including an ECG sensor assembly 28, an SpO₂ sensor assembly 32 and a non-invasive blood pressure (hereinafter NIBP) sensor assembly 36, respectively, the sensor assemblies being shown in FIG. 1 only for the sake of clarity.

A brief treatment of each tethered physiologic sensor assembly 28, 32, 36 is now provided for the sake of completeness. More particularly and in brief, the SpO₂ sensor assembly 32 is used to noninvasively measure oxygen saturation of arteriolar hemoglobin of a peripheral measurement site of a patient, such as the wrist, a finger, a toe, forehead, earlobe or other area. Reusable or disposable sensor probes can be used. In this instance, a finger clamp 60 is shown in FIG. 1, the clamp having a light emitter and a light detector that can be used to detect pulse/heart rate as well as blood oxygen saturation through pulse oximetry. The finger clamp 60 is tethered by means of a cable 64 extending to a pinned connector that mates with a corresponding female connecting port 44, FIG. 3, that is provided on the exterior of the device housing 24.

The concepts relating to pulse oximetry in general are commonly known in the field and do not form an inventive part of the present invention.

In brief, the ECG sensor or monitoring assembly **28** includes a lead wire assembly, wherein either a three-lead or a five-lead ECG can be utilized according to the present embodiment. More particularly and by way of example, the herein pictured ECG sensor assembly **28** of FIG. **1** comprises a set of lead wires **68**, each having electrodes **70** at the ends thereof to permit attachment, in a conventionally known manner, to the body of a patient, the lead wire assembly comprising a harness **71** that is attached to a connection cable **72** having a connector which is matingly attachable to the connection port **40** of the device housing **24**. The ECG sensor assembly **28** is further utilized herein with respect to a respiration channel of the herein-described monitoring device **20** in order to determine the rate or absence (apnea) of respiration effort through the determination of ac impedance between selected terminals of ECG electrodes **70**, thereby determining the respiration rate of a patient using impedance pneumography based upon movements of the chest wall using a designated reference lead wire. Heart rate according to the present embodiment is detected for the herein described device **20** using the ECG sensor assembly **28**.

The ECG sensor assembly **32** creates a waveform (ECG vector) for each lead and further includes a QRS detector that can be adjusted depending upon the patient mode selected. The ECG sensor assembly **28** is further configured to determine heart/pulse rate, if selected, according to the present embodiment as well as mark pacer spikes in the resulting ECG waveforms by way of a pacer detection circuit. The ECG sensor assembly **28** according to the present embodiment further includes selectable notch filters of 50 Hz and 100 Hz, 60 Hz and 120 Hz, respectively.

In brief, the NIBP sensor assembly **36** according to this embodiment indirectly measures arterial pressure using an inflatable cuff or sleeve **76**, which is attached to the limb (arm or leg) of a patient (not shown). The remaining end of a connected hose **80** includes an attachment end that can be screwed into a fitted air connector fitting **48** that is provided on the top facing side of the housing **24**. The air connector fitting **48** is connected to a pump (not shown) disposed within the monitoring device housing **24** in order to selectively inflate and deflate the cuff **76** to a specified pressure, depending on the type of patient, using the oscillometric method. Pressure changes are detected by means of circuitry in order to determine systolic, diastolic and mean arterial pressure (MAP). The NIBP sensor assembly **36** according to this embodiment is capable of performing manual, automatic and a turbo mode of operation, as described in greater detail below. The assembly **36** can also be equipped, in this embodiment, when ECG is also being monitored, with a motion artifact filter if ECG is also being monitored. The filter according to the present embodiment employs a software algorithm that can be used to automatically synchronize the process of NIBP measurement to the occurrences of the R-wave of the ECG waveform, thereby increasing accuracy in cases of extreme artifact and diminished pulses. An example of a suitable NIBP artifact filter is described in U.S. Pat. No. 6,405,076 B1, the entire contents of which are herein incorporated by reference. Examples of NIBP and ECG sensor assemblies useful for incorporation into the herein described monitoring device **20** are manufactured by Welch Allyn Inc., of Skaneateles Falls, N.Y., among others. With regard to each, the form of sensor assembly can be varied depending on the type of patient, (i.e., adult, pediatric, neonatal) by selective attachment to the connection ports **40**, **48** that are provided on

the monitoring device **20**. Each of the foregoing sensor assemblies according to the present embodiment further include electrosurgery interference suppression. As noted, pulse rate can be detected from either the SpO₂ or the NIBP channels of the monitoring device **20**.

It is contemplated for purposes of the present invention, however, that other means for connecting the above-noted sensor assemblies **28**, **32** to the monitoring device **20** other than through the connection ports **40**, **44**, including wireless means, such as for example, IR, optical, RF, and other non-tethered connections could also be employed for purposes of the present invention. It should be further noted that the number of types of physiologic sensor assemblies used with the herein described device **20** can be varied and that those shown are intended to only be exemplary of the present invention. The invention contemplates both multiple and single physiologic parameter monitoring of a patient using the monitoring device **20** and therefore such variation is purposely intended.

Referring to FIGS. **1** and **6**, each of the above physiologic sensor assemblies **28**, **32**, **36** according to this embodiment are internally connected electrically to a CPU **174** that is contained within the housing **24** of the monitoring device **20**. According to this embodiment, signal processing for each of the physiologic sensor assemblies **28**, **32**, **36** is performed internally through resident processing circuitry; for example, the SpO₂ sensor assembly **32** of the present embodiment utilizes the Nellcor Puritan MP506 architecture while the NIBP sensor assembly **36** is based upon a design, such as those used presently in the Micropaq and Propaq vital signs monitors, including, for example, an NIBP Module, Part 007-0090-01, manufactured and sold by Welch Allyn, Inc. Though not shown in FIG. **6**, the resident circuitry for each of the sensor assemblies **28**, **32**, **36** are all integrated into a single logic board wherein the ECG and respiration parameters utilize a common processor, such as a Motorola MPC 823 processor of the CPU **174**. Despite being integrated into a single logic board, the remaining physiologic parameters (SpO₂ and NIBP) are implemented in a more modular fashion, as shown in FIG. **6**, and utilize their own processors. It should be readily apparent, however, that the electronic packaging of the various processing elements of the physiologic sensor assemblies **28**, **32**, **36** of the monitoring device **20** can easily assume various configurations for purposes of the present invention and other versions could easily be contemplated.

Still referring to the schematic diagram of FIG. **6**, the contained battery pack **170** is interconnected to the CPU **174**, the latter including a microprocessor, memory, and resident circuitry, wherein each are connected to the tethered sensor assemblies **28**, **32**, **36** in order to enable processing storage and selective display of the signals provided therefrom as well as perform power conversion between the charging circuit of an optional charging cradle **140** and the contained battery pack, including circuitry to prevent overcharging of the contained battery pack **170** (i.e., 12 volts to 5 volts), as described in greater detail below. The CPU **174** according to this embodiment includes available volatile and non-volatile storage for patient data, in the form of Flash memory and SRAM, though other form as are also possible, the CPU **174** being further connected to the display **88**. As noted above, the CPU **174** according to this embodiment is presented on a single logic board along with the processors for the physiologic sensor assemblies **28**, **32**, **36**. The CPU **174** is intended to handle device-specific aspects, such as alarm limits, display generation, and enabling and disabling of certain features, wherein the physiologic sensor assemblies **28**, **32**, **36** predominantly only relate data for use by the CPU **174**. It

should be noted that portions of the processing function, for example, the ECG processing algorithms, can also reside in CPU 174, though this can be varied appropriately depending, for example, on the extent of processing power required or packaging concerns. The CPU 174, predominantly controls the operation of the device 20, including patient modes, pressures, voltages and the like, either as a factory default setting, or configured, as described below either through the user interface 92, a remote monitoring station 184, FIG. 6, and/or a connected PC 192, FIG. 6.

In addition to the preceding, the monitoring device 20 as schematically represented in FIG. 6 further optionally includes a wireless radio card/transceiver 180, enabling bi-directional wireless communication with at least one remote monitoring station 184, such as, for example, the Acuity Monitoring Station manufactured and sold by Welch Allyn Inc., using the radio card as inserted in an internal PCMCIA expansion slot (not shown). The radio card 180 according to this embodiment is an IEEE 802.11 compliant radio card that connects to an antenna 182 that is also disposed within the housing 24 of the monitoring device 20 for transmission over a 2.4 GHz frequency hopping spread spectrum (FHSS) wireless local area network (WLAN) using access points 186. Additional details relating to an exemplary wireless interconnection, including networking therewith, is provided in U.S. Pat. No. 6,544,174, the entire contents of which are herein incorporated by reference. Additional discussion of device-specific details relating to the wireless connection of the herein described monitoring device 20 is provided in a later portion of this description.

As most clearly shown in FIG. 2, a lower or bottom facing surface 120 of the device housing 24 includes a latching member 124, FIG. 2, as well as an electrical port 128, FIG. 2, each of which are used in conjunction with an optional charging cradle 140, FIG. 4, described in greater detail below. As previously noted, the battery pack 170, only shown schematically in FIG. 6, is contained in the rear of the device housing 24 within a rear compartment (not shown). The battery pack 170 provides portable power for the monitoring device 20 wherein the battery life is dependent upon certain operational modes of the device, as described below. The battery pack 170 is rechargeable by means of charging circuitry contained within the optional charging cradle 140, FIGS. 4, 5. According to this embodiment, the battery pack 170 includes at least one rechargeable lithium-ion battery, such as those manufactured by Sanyo Corporation. In this instance, the battery pack 170 includes two rechargeable batteries. According to the present embodiment, the monitoring device 20 is capable of operation in a stand-alone mode using the contained battery 170 as a power source, the battery according to this embodiment having an average runtime of up to approximately 24 hours, depending on the usage of the device.

Referring to FIGS. 4-6, details relating to the charging cradle 140 and its optional connection with the monitoring device 20 are herein described. The charging cradle 140 permits DC power from a wall adapter 171, shown only schematically in FIG. 6, or other source to be supplied to the contained rechargeable battery pack 170 through charging circuitry contained in the cradle and power conversion circuitry contained in the monitoring device. The use of the optional charging cradle 140 permits the monitoring device 20 to be operated regardless of the status of the contained battery (i.e., charged or uncharged), therefore enabling use of the monitoring device 20 as a stand-alone or networked bedside monitor. That is, the foregoing operation can permit both

the internal display of patient data as well as wireless transmission of stored patient data to the central monitoring station 184.

Structurally, the charging cradle 140, according to the present embodiment, is defined by an open-topped receptacle 144 having a molded or otherwise defined internal cavity that is sized to receive the lower half of the monitoring device 20. The receptacle 144 is designed to allow operation of the monitoring device 20 via the user interface 92, as shown in the attached view of FIG. 5, when the device is attached thereto. A monitor release button 148 is provided on a front facing side 152 of the receptacle 144. The monitoring device 20 is engaged by aligning the bottom facing surface 120, FIG. 2, of the device housing 24 with the internal cavity of the receptacle 144 and more specifically aligning the latching member 124 provided thereupon with a pivotally movable locking or latching element 156 that is disposed within the bottom of the internal cavity of the receptacle 144. A pinned electrical connector 160 adjacent the latching element 156 mates with the corresponding electrical connector 128, FIG. 2, provided on the bottom facing side 120, FIG. 2, of the device housing 24, FIG. 2, and thereby provides electrical connection between the monitoring device 20 and the charging cradle 140, as schematically shown in FIG. 6. Engagement of the latching member 124 with the latching element 156 locks the monitoring device 20 in place wherein depression of the monitor release button 148 causes the latching element 156 to be pivoted out of contact with the latching member 124, allowing release of the monitoring device 20 from the charging cradle 140.

A rear engagement portion 164 of the charging cradle 140 includes a curved hanging bracket 166, permitting the charging cradle and attached monitoring device 20 to be attached to a bedrail, as shown, for example, in FIG. 11. Alternatively, the hanging bracket 166 can further include at least one other mount (not shown) that permits attachment to separate apparatus, such as a fluid-IV pole (not shown). In one version, the hanging bracket 166 can include both attachment modes (bedrail, IV pole). The hanging bracket 166 is separably removable by way of threaded fasteners (not shown) or other means from the rear engagement portion 164 to permit other attachment arrangements, such as those discussed below with reference to FIGS. 11-13. The bottom surface of the charging cradle 140 according to this embodiment further includes a plurality of support feet 149, FIG. 5. According to this embodiment, the support feet 149 are provided at each corner of the bottom surface in order to permit placement onto a flat surface, such as a table 203, FIG. 12.

A pair of indicators 167, 168 are provided on the front facing side 152 of the charging cradle 140 wherein according to this embodiment indicator 167 is a status indicator and indicator 168 is a power indicator. The power indicator 168, in this instance, a green LED, indicates that power is connected to the charging cradle 140. The status indicator 167, in this instance, a multi-colored LED, is used to indicate the charging status of the monitoring device 20. For example and if the monitoring device 20 is in the charging cradle 140 and power is properly connected to the charging cradle from the wall adapter 171, FIG. 6, the status indicator 167 will be illuminated (e.g., either green or yellow) or will be off. When the status indicator 167 is green, charging is proceeding normally. The status indicator 167 is turned off when the battery pack 170 reaches full charge. When the status indicator 167 is yellow, the indicator indicates that a fault has occurred and the battery pack 170 is not charging properly. Such faults may occur, for example, as those caused by a severe discharge of the battery 170, a cradle logic fault, incorrect seating of the

monitoring device 20 within the charging cradle 140, improper engagement of the connectors or other similar anomaly.

In spite of most charging faults, as noted above, power will not be interrupted to the monitoring device 20. That is, the power indicator 168 may be illuminated (e.g., green), indicating power is capable of being delivered to the monitoring device 20 in spite of the fact that a charging fault (yellow) has occurred. Each time the monitoring device 20 is placed into the charging cradle 140 according to this embodiment, the cradle attempts to charge the contained battery pack 170. If the battery pack 170 is fully charged when the monitoring device 20 is inserted into the charging cradle 140, the status indicator 167 turns green momentarily and upon sensing of a full charge, the indicator is turned off. In the instance that the battery is overcharged at the device 20, however, no power for charging the battery pack 170 will be delivered to the device.

Typically, the herein described monitoring device 20 is shipped to a user/facility with a preset factory configuration for each setting and behavior of the device. It is desirable for most facilities to reconfigure any received patient monitoring device 20 to conform the device to local protocol and adapt the device to the clinical environment to which the device will be used. For example, the monitoring device 20 might be used in a neonatal unit although the factory calibration/configuration is preset for adult patients. Although the user could custom configure the monitoring device 20 upon each use to allow the device to be used for neonatal patients, as described in greater detail herein, it may be preferable to have neonatal mode installed as the default patient mode for a monitoring device.

According to the present invention, a PC 192, FIG. 6, can be used in conjunction with the charging cradle 140 to download a new configuration file to the monitoring device(s) 20 prior to use in a facility for service. According to the present embodiment, the charging cradle includes a USB data port 165, FIG. 4, provided on the exterior of the charging cradle 140 that provides an isolated serial data-link connection between the attached monitoring device 20 and the personal computer (PC) 192, FIG. 6, through a USB cable.

Using a configuration utility supplied through the data link with the PC 192, the charging cradle 140 serves as an intermediary or pass through to the monitoring device 20 to configure the monitoring device prior to use in a facility by creating a configuration file that includes a plurality of setting choices that can be completed, for example, by the bioengineer of the hospital, to adapt onto or to replace pre-existing factory settings initially provided with the device 20 that are stored or programmed within the CPU 174. According to this embodiment, the PC 192 includes utility software that enables the creation of a utility configuration worksheet into which default settings and limits can be entered. The worksheet is then converted into the new configuration file that is downloaded into the CPU 174 of the monitoring device 20 through the intermediary charging cradle 140. As many as approximately 60-70 different settings, depending on the device, can be preset using the downloaded configuration file wherein some of these features, if not enabled, cannot be controlled by the clinician/user. These settings can include, for example, the default language of the monitoring device 20, the default patient mode of device operation, forms of display available to the user and/or their ordering, the enablement of device specific features, such as, for example, lockout of the user interface 92 and display 88, time limits on alarms and alerts, data trending, and the enablement of alarm and alert tones. All or certain of the factory settings can be adjusted by appropriate entries provided on the configuration

worksheet created at the PC 192 and communicated through the data link between the CPU 174 and the PC 192. Therefore, this PC configuration results in a set of revised default settings and monitoring device behaviors.

A portion of an exemplary configuration worksheet is shown in FIGS. 64 and 65 with regard to one specific feature that can be enabled with regard to alarm management. Specifics relating to this feature are described in greater detail in a later section. The worksheet 198 shown is a paper version that is completed by a user in advance to using the configuration utility, the latter providing a PC worksheet version that provides similar entries. The user completes the paper configuration worksheet 198, FIG. 64, to organize the features for configuration or can directly input selections into the utility worksheet provided at the PC 192, FIG. 6. Once all entries have been made, the configuration file is created with instructions to override the factory settings when the file is downloaded to the monitoring device 20 through the serial data link provided by the charging cradle 140.

As will be described in greater detail below, the PC 192, FIG. 6, also permits stored data to be printed automatically when the monitoring device 20 is activated and attached to the charging cradle 140, also using the associated USB data port 165, FIG. 4. In this instance and referring to FIG. 6, the PC 192 is connected to a suitable peripheral printer, in this instance, a laser printer 195, also schematically shown in FIG. 6, wherein the monitoring device 20 and PC are programmed to automatically permit data transfer to occur. According to this embodiment, the data that is stored is in the form of trended data and "snapshots", the latter term referring to numeric and waveform data covering a predetermined time period that is electively taken by a user using the snapshot button 116. Pressing the snapshots button 116, FIG. 7, located on the device housing 24, FIG. 2, causes data occurring a predetermined time period prior to pressing the button and a predetermined time period after pressing the button to be stored by the CPU 174. Details relating to stored trend and snapshot data are provided in a later portion of this description.

Referring to FIGS. 6 and 11-14, the charging cradle 140 can alternatively serve to provide an intermediary interconnection between the herein described monitoring device 20 and a large display 200. This form of interconnection permits all processed data in the monitoring device 20 to be transmitted in real time in order to permit viewing of the data substantially as though users were at the central monitoring station 184, as opposed to the smaller and constricted device display 88. That is, a series of waveforms can be displayed for viewing, for example, as shown in FIG. 14. The large display 200 according to this embodiment includes a VGA card and suitable attachment bracketry in the form of an interface box or housing 202. Several embodiments for interconnection of the monitoring device/charging cradle assembly to the large display 200 through the interface box 202 are illustrated in FIGS. 11-13. In each embodiment, the monitoring device 20 is already attached to the charging cradle 140 in the manner described above. According to FIG. 11, the charging cradle 140 is attached to a bedrail using the hanging bracket 166. A VGA cable 205 is then connected from the USB data port 165, FIG. 4, to connectors that are provided on the interface box 202. As such, the charging cradle 140 serves as an intermediary for data transfer from the patient monitoring device 20. As shown in FIG. 12, the curved bracket 166, FIG. 4, can be removed from the rear engagement portion 166, FIG. 4, of the charging cradle 140 and the monitoring device 20/charging cradle 140 can be placed on a table 203 adjacent the large display 200, the latter being attached in each instance to a

wall. In the latter example, the interface box **202** is directly attached to the rear of the charging cradle **140**. Finally and as shown in FIG. **13**, the monitoring device **20** and charging cradle **140** can be attached to the interface box **202** directly on the large display **200** through the display bracketry and bracketry that is provided on the charging cradle **140**, respectively. A sample data output of the large display **200** is shown in FIG. **14**, this output substantially replicating that seen by the remote monitoring station **184**, FIG. **6**, and considerably an increased amount of data than is viewable on the integrated display **88**.

It is further contemplated within the spirit and scope of the present invention that the charging cradle **140** can include additional features to provide a level of adaptability for a system incorporating the herein described monitoring device **20**. For example, an additional physiologic parameter assembly could be attached to the charging cradle **140** in lieu of or in addition to the monitoring device **20** wherein physiologic data could still be uploaded to the monitoring device **20** when the device is attached to the charging cradle for wireless transmission to the central monitoring station **184**, FIG. **6**. Similar configurations should be readily apparent. For example, the charging cradle **140** can be equipped with at least one physiologic sensor assembly (not shown) wherein data collected by the at least one sensor assembly can be inputted to the CPU **174** of the monitoring device **20** for display and transmission.

With regard to running time available on the monitoring device **20** when the device is not mounted in the charging cradle **140**, the life of the battery pack **170** is highly dependent on the use mode of the device. As noted above and according to this embodiment, about 24 hours of runtime is possible. The level of battery charge is displayed by the monitoring device **20** according to this embodiment, as described below.

Referring to FIG. **7**, the user interface **92**, FIG. **2**, according to this specific embodiment includes five (5) closely arranged buttons forming a keypad. In brief, a center button, referred to throughout as a SELECT button **96**, is generally used to select a highlighted item that is displayed by the device, as discussed in greater detail below, or to confirm a choice. Four buttons **100** immediately surrounding the SELECT button **96** are generally used (up, down, left or right) in order to directionally guide a display cursor in order to highlight an item, for example, or to increase or decrease a selected parameter value. A number of additional actuatable buttons are also provided, according to this embodiment, on the front facing side **84** of the housing **24**, these buttons being used for specified or dedicated purposes, including a display button **104**, permitting the user to cycle between a plurality of varied display formats, such as those shown in FIGS. **15-19**, an alarm silence/resume button **108** permitting the user to temporarily and manually silence or resume an existing patient alert/alarm tone, an NIBP start/stop button **112** for manually starting or stopping an NIBP measurement, and finally the above referred to snapshots button **116** that automatically stores a predetermined time period of vitals-signs data in both tabular and waveform format, an exemplary snapshot display screen being shown in FIG. **50**. Each of the above-described buttons further include a visual representation of their function for ease of use by the clinician; for example, the directional control buttons **100** include specific directional arrow indicators, the display button **104** includes a display icon, the NIBP start/stop button **112** includes a depiction of a blood pressure cuff, the snapshots button **116** includes a camera icon and the SELECT button **96** depicts a circle thereupon. Additional details concerning the functions defined by each of the above-listed buttons, and the implementation and operation of the

user interface **92** of the herein described monitoring device **20** will be described in greater detail in a succeeding section of this description.

Referring to FIGS. **2**, **5** and **7** and in addition to the above user interface **92**, a series of visual status indicators are also provided on the front facing side **84** of the monitoring device **20**. Three status indicators **169** are arranged in linear fashion above the display **88** at the center of the front facing side **84** of the device housing **24**, and are electrically connected to the CPU **174**, FIG. **6**. Among the purposes of the visual status indicators **169** according to this embodiment are to apprise the user of the operational status of the monitoring device **20**; that is, whether the monitoring device **20** is operating normally, confirmation of the connection of the monitoring device **20** and the proper patient being connected to a network or to a remote monitoring station **184**, FIG. **6**, and/or whether the herein monitoring device **20** is subject to an alarm and/or alert condition. It should be readily apparent that the number and location of these indicators can be suitably varied.

More specifically and according to the present embodiment, each of the status indicators **169** are illuminated with a specific colored light (e.g., red, yellow or amber, and green), indicating an alarm condition, an alert condition, and normal operation of the monitoring device **20**, respectively. For purposes of definition herein, an "alarm" is indicative of a patient condition, such as vital signs reading(s) that is outside of acceptable limits. When an alarm condition occurs, for example, the red indicator **169** is illuminated. An "alert" condition, by comparison, is not as serious as an "alarm" condition and is typically indicative of a device-operational problem, such as a low or discharged battery or a detached lead. The yellow status indicator **169** is illuminated when this type of condition is indicated. Normal operation is signified by illumination of the green indicator **169**. The status indicators **169** can further either illuminate steadily or flash in order to indicate the severity of the problem. For example and according to this embodiment, this severity can be defined between an equipment alert and an alarm condition. The monitoring device **20** further includes a speaker **161**, shown only schematically in FIG. **6**, for signifying audible tones, as needed, for example, that may be sounded during an alarm or alert condition. Additional details relating to alarm and alert management using the herein described monitoring device **20** are described in a later portion.

Each of the tethered sensor assemblies **28**, **32**, **36** provide physiologic parameter data in the form of analog signals and the like to the CPU **174** of the monitoring device **20**. The herein described monitoring device **20** is capable of continuously monitoring each of the physiologic parameters (NIBP, pulse rate, 3 and 5 lead ECG, respiration, SpO₂) depending on the number and type of sensor assemblies that are connected therewith.

As depicted in the operational block diagram of FIG. **6** and as previously noted herein, each of the SpO₂ sensor assembly **32** and the blood pressure (NIBP) sensor assembly **36** according to this embodiment include their own individual processors contained within the monitoring device **20** that operate the sensor assemblies with regard to the acquisition of and processing of data (that is, each of the above sensor assemblies include appropriate algorithms and resident circuitry for processing the acquired signals). The ECG/respiration sensor assembly **28** according to this embodiment includes attendant circuitry within the CPU **174**. As previously noted, any or all of the sensor assemblies can include modular processors or the processing can be carried out within a single integrated logic/CPU board. The signals then being processed are stored into the memory of the CPU **174** for display and for wireless

transmission using the contained transceiver **180** and antenna **182** to the central monitoring station **184** using the communications network, as described in the previously incorporated U.S. Pat. No. 6,544,174. Additional data, such as patient demographics, can be added for storage and display by the user, as discussed below, or may alternately be uploaded to the monitoring device **20** from a list of available patients from the remote station **184**. The monitoring device **20** can transmit patient information, once configured with the network, for display of all stored parametric data at the remote monitoring station **184**. The monitoring device **20** is also connectable through the USB port **165**, FIG. 4, of the charging cradle **140**, enabling operation as a bedside monitor in which serial attachment to the PC **192** through the USB port **165** enables interconnectivity to a peripheral device, such as a printer **195**, as previously described or alternatively, to the larger display **200**. In the meantime, the monitoring device **20** can also transmit wirelessly to the remote monitoring station **184** using the connected radio **180** and antenna **182**.

The versatility of the herein described monitoring device **20** therefore provides a number of distinct advantages. First, the herein described monitoring device **20** can be used as a transport monitor in that the device is battery powered. Second, the use of the rubberized back feet or pads **58**, the rear interior loading of the battery pack **170** and general packaging and compactness of the profile of the monitoring device **20** present a lightweight and extremely versatile unit that allows for both wired and wireless connectivities enabling the device to work in either a stand-alone or a networked capacity. The charging cradle **140**, FIG. 4, permits the monitoring device **20** to be used for bedside applications by providing a source of power for the contained battery pack **170** as needed and for charging same. In addition and through use of the data port, the charging cradle **140** serves as an intermediary device that enables data transfer to either a large display **200** or printing to a locally connected computer **192**. The locally connected computer **192** can also be used to selectively modify factory programmed configuration settings of a monitoring device **20** through new default settings that can be downloaded to the monitoring device **20**.

The following discussion relates to the operational aspects of the monitoring device **20**. Reference is made throughout to numerous exemplary display screens that are generated by the CPU **174** of the herein described monitoring device **20**. Each display screen is defined by a stored preformatted template consisting of a number of discrete panels with each panel including a number of elements that are defined by various combinations of textual, numeric, waveform, graphical and/or other forms of data, as described herein that are obtained from the CPU **174** and generated onto display **88**.

Upon powering up the herein described monitoring device **20** using the Power On/Off button **56**, an audible tone from the contained speaker **61**, FIG. 6, is sounded. With each activation of the monitoring device **20** according to this embodiment, a self-diagnostic or operational test is initiated. If the self test is unsuccessful, at least one of the status indicators **169** of the monitoring device **20** is illuminated, depending on the error. In terms of a general overview and if the self test is successful and following this diagnostic, a start-up display screen **400(a)**, **400(b)**, FIG. 24, appears on the display **88**, FIG. 1, with the display screen having user-selectable options to continue monitoring a patient (in the event patient data has been saved), start monitoring a new patient, obtain system information, or enter a demonstration mode.

Referring to FIG. 24, the stored template format of each of the generated start-up screens **400(a)**, **400(b)** is similar whether or not patient data has previously been stored by the

monitoring device **20**. That is, each start-up display screen **400(a)**, **400(b)** commonly includes a customer ID panel **404**, a notice panel **408**, a bottom message panel **412** and a context menu panel **416**, respectively, as read from the top of the display screen. In the instance that no patient data has previously been saved by the monitoring device **20**, the notice panel **408** of start-up display screen **400(a)** indicates by way of a textual message that no data has been saved. The notice panel **408** of the other version of the display screen **400(b)**, on the other hand, indicates that specific patient data has been previously stored by the monitoring device **20**. In the instance that a patient's data was stored prior to the time the monitoring device **20** was last turned off, monitoring can be resumed for that patient when the monitoring device **20** is powered up again. When the patient data is saved by the monitoring device **20**, the settings of the monitoring device **20** are also saved into the nonvolatile memory of the CPU **174**. In this instance, a decision must be made by the user as to whether the data is to be saved and monitoring will continue with the same patient or whether the stored patient data should be deleted and a new patient monitoring mode should be initiated.

The customer ID panel **404** provides information about the facility and device that have been previously entered and stored in an information screen, such as shown in FIG. 26, shown as **420(a)**, **420(b)**. The information screen **420(a)**, **420(b)** can be accessed from the Info option of the context menu panel **416**. Each of the information screens **420(a)**, **420(b)** also include a context menu panel **416** at the bottom thereof, including the same options as the start-up screens **400(a)**, **400(b)**, respectively. Typically, this information can be added to the memory of the device **20**, such as during the creation and downloading of the configuration file using PC **192**, FIG. 6, as described previously.

In general, the context menu panels **416** provide a means for navigation between various control screens of the herein-described monitoring device **20**. Each context menu contains a number of menu options disposed along the length of the panel **416**. The user interface **92** and in particular, the directional buttons **100** and the SELECT button **96** are used to highlight and select a highlighted option by movement of the display cursor. To that end, selection of one of the context menu options executes a new mode of the monitoring device **20** or creates a new display screen, as described in greater detail below. The content and options available in context menus vary depending on the display screen which utilizes them. Examples of various context menus **416** that are used in the operation of the monitoring device **20** are provided in FIGS. 25, 28 and 47, each of which are detailed in a later portion of this description.

Referring back to FIG. 24, and to the specifics of the context menu panel **416** of the start-up display screens—in the instance in which no previous patient data has been stored by the monitoring device **20**, the context menu panel **416** indicates the following available user-selectable options; namely, a Start New Patient option, an Info option, and a Demo option. The Start New Patient option permits the user to enter a patient monitoring mode. The Info option reverts the user to an information screen, such as either **420(a)**, **420(b)** shown in FIG. 26, while selection of the Demo menu option provides access to a demonstration mode for the monitoring device **20**.

In the instance that patient data has been saved by the monitoring device **20**, the above three (3) user-selectable options are provided in the context menu panel **416** of display screen **400(b)**, as well as a Continue Patient option. To resume monitoring on the same patient and upon powering up the

monitoring device **20**, the “patient data stored” display screen, **400(b)**, FIG. **24**, is displayed. The user then verifies that the displayed name and patient ID match that of the current patient and upon verification, and highlights the Continue Patient option in the context menu panel **416** at the bottom of the display screen **400(b)**. If the latter option is selected through use of the directional arrow buttons **100** and pressing the SELECT button **96**, then any stored data is loaded and the monitoring device **20** is ready for monitoring, including the continued implementation of any previous custom configuration settings that are particular to the patient.

If, however, the Start New Patient option (onto which the display cursor is highlighted in the display screen **400(b)**) is elected and the SELECT button **96** is pressed, then all previous data (and custom configuration settings) are deleted and a new patient monitoring mode is initiated.

Upon election of the Start New Patient option, a first configured data display screen **430** appears, as shown in FIG. **27**. In this data display screen **430**, a unique auto ID is provided in a status panel **320**, and more specifically in a device ID field **434** that is highlighted using the SELECT button **96**, accessing a Patient Information Entry screen **440**, as shown in FIG. **28**, the latter consisting of a table of alphanumeric characters **444** that can be highlighted and sequentially entered into the proper field **448** to create entries. The name of the new patient is then entered as well as the patient ID and the patient room number. Alternatively, this data can be entered using the remote monitoring station **184**, FIG. **6**, through an enabled wireless connection as opposed to the above-described local entry of information. When all of the above information is entered, a Confirm option provided in the context menu panel **416** of the display screen **440** is highlighted and the SELECT button **96** is pressed. All information entered is then stored into memory of the CPU **174** and is used by the device in various display screens throughout the operation of the monitoring device **20**. The mode of the patient is then confirmed and the sensor assemblies **28**, **32**, **36** are attached to the patient and the monitoring device **20** (if not already attached to the device). The monitoring device **20** is now ready to begin monitoring wherein readings are displayed on a formatted default data display screen, such as shown in FIG. **27**, in predetermined fields on a display screen adjacent to text identifiers that are preformatted on the generated screen template. The screen format shown in FIG. **27** is that of a large numerics display screen, discussed in greater detail below.

For purposes of the following discussion, it is assumed that each of the sensor assemblies **28**, **32**, **36** have been suitably attached to a patient (not shown) and the monitoring device **20** and that the patient has been monitored for an extended period of time by the device. A number of specifically configured display screen template formats are stored in memory of the CPU **174** and are available for viewing at the user's option, these templates including associated vital signs data in the form of either current or trended data. An exemplary default display screen **210**, FIG. **15**, for purposes of this discussion is enabled by way of the configuration settings of the monitoring device **20**, this screen being the current display screen displayed to the user during monitoring. The format of this particular display screen **210** includes a status panel **320**, a large waveform panel **324** and a parameter panel **328**, respectively, as read from the top of the display screen.

The displayed data that is shown in FIG. **15** as contained in the various fields of the status panel **320** includes the following elements: the patient's name, if available, shown as **204**, the patient ID **208**, and the patient room number **209**. Each of the preceding elements were manually added to the internal memory of the monitoring device **20** and added at start-up as

previously described above with regard to FIGS. **27** and **28** by the clinician or alternatively in the case of a network-enabled monitoring device **20**, by the remote monitoring station **184**, FIG. **6**, prior to monitoring of the patient over a wireless communications link. In the former instance, this information as entered in the Patient Entry Information display screen **440**, FIG. **28**, by the CPU **174** is used to populate the status panel **320** of each display screen of the herein described monitoring device **20** for the patient currently being monitored, for so long as power is maintained to the device, unless the user elects to specifically maintain these settings prior to turning the device off, as described in greater detail below.

Referring to FIG. **15** and in addition to the patient information, the status panel **320** further includes a communication status icon **212** (if the device includes a wireless transceiver **180**, FIG. **6**, and antenna **182**, FIG. **6**) and a time display **216**, as well as a battery status indicator or icon **220**, the latter providing an indication of available battery power. The battery status icon **220** can provide an indication as to whether the contained battery pack **170** is full, partially full indicating that the battery is not fully charged, but not fully discharged, partially full and charging, low battery wherein the battery has approximately 30 minutes of runtime remaining, low battery and charging, very low battery wherein the battery has approximately 5 minutes of run time remaining and very low battery but charging. In the instances in which low battery is indicated by the icon **220** (as indicated by a depiction of a half-filled battery) and in addition to the icon, an alert (not shown) can be provided by the monitoring device **20**. The battery status icon **220** would remain after acknowledgement of the alert. Alerts and their management are discussed in a later portion of this description.

According to this embodiment, the CPU **174** is programmed to automatically disable the NIBP sensor assembly **36** upon a low battery indication being determined wherein a status message is displayed to the user if the manual NIBP start/stop button **112** is pressed. If the monitoring device **20** is charging in the charging cradle **140** and a low battery and charging indication appears via icon **220**, then the NIBP sensor assembly **36** is enabled.

In addition to the above, the mode (adult, neonatal, pediatric) of the patient **224**, as well as the mode of the device **228** (simulation, monitoring) are each applied within separate fields that are provided in the status panel **320** of the display screen **210**. Each of the foregoing are typically based upon default settings of the herein described monitoring device **20**, unless modified by the user, as described in greater detail below.

With regard to the waveform panel **324**, the depicted waveform **240** is current and can originate from a number of sources. The panel **324** further provides text identifiers relating to the specific waveform source **232** and waveform size (display scale) **236**. In this example, a waveform representative of an ECG vector is represented. The waveform depicted, including its size and source as displayed, are also typically based upon a default setting of the monitoring device **20**, wherein each setting may be changed locally by the user or remotely by the remote monitoring station **184**, as described below.

Beneath the waveform panel **324** and in the formatted parameter numerics panel **328**, current or live parameter numeric values are displayed for heart rate/pulse rate **244**, respiration rate **252**, and pulse oximetry **256**, as well as a separate dynamic indicator for the pulse amplitude of the pulse oximeter sensor in the form of a blip bar **260**. Text identifiers are also provided beneath each above-noted parameter. In addition, the most recent NIBP measurement

248 is also displayed, with a corresponding text identifier and time stamp, the pressure measurement being displayed in terms of systolic over diastolic numerics with mean pressure being expressed in parenthetical terms. Since each of these physiologic parameters, except NIBP, are continuously monitored, their numeric values will change and be updated with stored data being trended by the CPU **174**, FIG. **6**. Finally, a series of alarm status indicators **268** are also represented in the parameter numerics panel **328** at the bottom of the display screen **210** for each listed parameter. These alarm indicators **268**, represented herein by bell icons indicate whether the upper and lower limits for each physiologic parameter are on, the upper alarm limit is on but the lower alarm limit is off, the upper limit is off but the lower limit is on, or all alarms are off through an appropriate representation of an alarm symbol, whether in blank or solid, and combinations thereof. Alarms are described in greater detail in a later portion of this description.

Each of FIGS. **16-19** depict additional exemplary display screens that can be selectively displayed by the user in addition to the single waveform display screen **210** depicted in FIG. **15**. Each of these additional display screens include a specifically defined template format that is stored into memory for generation by the CPU **174** onto the display **88**. According to this specific embodiment, these additional user-selectable display screens include a dual waveform display screen **332**, shown in FIG. **16**, a large numeric display screen **336**, shown in FIG. **17**, which is similar to that shown also in FIG. **27**, and a single waveform with tabular trended data display screen **340**, as shown in FIG. **18**. For purposes of discussion herein, each of the same reference numerals are used to label similar data and symbology herein for the sake of convenience and clarity. The above-noted display screens permit live monitoring of vital sign numerics, waveforms and/or trend information in various user-selectable formats as now described.

The dual waveforms display **332** screen of FIG. **16** is a variation upon the single waveform display screen **210** of FIG. **15**. This display screen **332** provides patient and monitoring device information as well as two waveforms and available parameter numerics. To that end, the defined format of this display screen **332** includes a status panel **320** that includes each of the elements of the single waveform display screen **210** referred to above including patient name **204**, patient ID **208**, patient room number **209**, communication status indicator **212**, time display **216**, battery status indicator **220**, patient mode indicator **224**, and display mode indicator **228**. Two small waveform panels **344** are provided in lieu of the single panel of the display screen **210**, FIG. **15**, the display screen further including a live or current parameters numerics panel **328**, similar to that of the single waveform display screen **210**, FIG. **15**. Each of the waveform panels **344** are smaller than that of the single waveform data display screen **210**, but contain similar information including waveform source **232** and size indicia **236**. The waveforms presented in the panels **344** can be from two different sources or can be provided alternatively as a cascaded waveform from one source that is presented on two adjacent waveform panels. In the example shown in FIG. **16**, separate ECG and SpO₂ waveform **240**, **242**, respectively, are depicted. The live parameter numerics panel **328** like the preceding includes a heart rate/pulse rate numeric and text identifier **244**, the most recently taken NIBP numeric **248** including the systolic/diastolic and mean (parentheses) numerics and text identifiers as well as a corresponding time stamp, a respiration numeric and text identifier **252**, and an SpO₂ numeric and text identifier **256** including a dynamic blip bar **260** showing pulse

amplitude. Alarm icons **268**, in the forms of bell icons, are also provided for each of the preceding parameters in this panel **328**.

The large numerics display screen **336** shown in FIG. **17** is similar to that depicted in FIG. **27**, labeled as **430** (but without data or patient information entered). This display screen **336** is defined by a format that includes a status panel **320**, also similar to that described for the display screens of FIGS. **15** and **16**, and a large numerics panel **352** provided in lieu of waveform panels. The large numerics panel **352** contains the same information provided in the panel **348** discussed with regard to FIG. **16** other than that the icons and associated text identifiers are significantly larger and disposed in differently assigned fields in the display screen **336**. More specifically, the live or current parameters panel for this display screen includes a large HR/PR numeric element **244** as well as a text element and an alarm icon **268**, a large SpO₂ numeric element **256** along with an associated text element, alarm icon **268** and blip bar **260**, a large NIBP numeric element **248** representative of the most recent measurement as well as a text element and time stamp of measurement and alarm icon **268** and a large respiration numeric element **252** along with an associated text element and alarm icon **268**. With regard to the alarm icons **268**, these provide an indication of those alarms that are currently enabled and those alarms that are currently disabled. For purposes of this discussion, the left half of each alarm icon **268** relates to the lower alarm limit and the right hand side of the icon refers to the upper alarm limit. A solid bell, shown herein as white, indicates that the alarm is enabled while a blackened portion of the bell indicates that the alarm is disabled. Alarms are provided (upper and lower limits) for each of heart rate/pulse rate, respiration, NIBP (systolic, diastolic and mean) and SpO₂. As seen in the depicted example, the lower limit of the mean NIBP is currently disabled while the remaining alarm limits are each currently enabled. The alarm icons **268** further permit the user to access menus, as described in greater detail below, by which the alarms can be enabled or disabled, upper and lower limits can be set, and volume controls for audible tones can be adjusted.

The herein described monitoring device **20** can not only display current or recent numerics and waveforms, but is also storing data for trend analysis. To that end, several display formats relate to trended data, wherein this data can be reproduced either graphically or tabularly. Snapshot data is also stored in addition to any periodic or randomly taken measurement data and data stored by the device **20** based upon continuous monitoring. To that end, FIG. **18** illustrates a combination waveform/tabular trend display screen **340**. In this example, a waveform as well as live parameter numerics and tabular list of trend data are depicted in a generated template format on the display **88** pertaining to a monitored patient. The pre-defined format of this display screen **340** includes a status panel **320**, similar to that described with regard to FIG. **15**, a single waveform panel **344** including a waveform and text identifiers relating to the waveform source **232** and size **236**, respectively, similar to those described in FIG. **16**, a trends live numeric panel **356** and a trends data panel **360**, respectively.

The trends live numerics panel **356** includes a data display header **364** relating the form of data presented (tabular, graphical, or other) followed by a linear set of current heart rate, respiration and SpO₂ parameter numerics and the most recent NIBP measurement, as well as text identifiers beneath each corresponding parameter numeric and the current blip bar **260** for SpO₂. A "Time" table heading is also provided beneath the data display header **364**.

The trends data panel **360** of this display screen **340** includes a tabular (in this instance) arrangement of stored numerics arranged in a table, allowing the user to navigate through a predetermined period (e.g., 24 hours) of stored trends with entries for time, heart rate/pulse rate, NIBP, respiration and pulse oximetry provided beneath each corresponding text identifier. According to this embodiment, trend data is listed in one minute intervals for each of time, heart rate/pulse rate, respiration, and SpO₂, respectively, when any NIBP readings are successfully made using the NIBP start/stop button **112** or through automated mode, or when an SpO₂ spot check reading is made. Each of the latter features are described in a later portion herein. As will also be detailed in a later portion of this description, the time interval between trend entries is a configuration setting of the monitoring device **20** that can be selectively adjusted by the user, for example, depending on the patient.

The exemplary display screen **340** is configured to list seven (7) entries in the display panel **360** according to the present example, although this parameter can be varied. For example, and as shown in FIGS. **19** and **54-56**, a twelve (12) entry table is provided on a tabular trend data display screen **470**. No waveform data is provided on this screen **470**, which is defined by a status panel **320**, a trends live numerics panel **356**, similar to that shown in FIG. **18**, and a trends data panel **474**. As noted, up to 24 hours or other predetermined time period of trend data can be stored into memory. A scrolling navigation icon **374** is also provided next to the time listing in order to permit the user to access any of the stored data, as needed.

In addition to tabular data, the herein described device **20** can display trended data in a graphical form. An exemplary graphical trend data display screen **380** is shown in FIG. **57**. This display screen **380** is defined by a format that includes a status panel **320**, as described above, a live trends numerics panel **356**, and a graphics display panel **384** with graphical trend data **294** having a time scroll **388** at the bottom thereof. The data shown pertains to a single parameter (in this example, heart rate), wherein the parameter data being displayed can be varied, as described in greater detail below.

Referring to FIGS. **18**, **19** and **56**, user-captured snapshots are identified separately in the tabular listing of trend data with a camera icon **477**. A sample snapshots viewing screen **298** is shown in FIG. **50**. Reviewing of snapshot data is discussed in a later portion of this description.

The display button **104** according to the herein described embodiment is used to cycle through the configured display formats. As shown in FIG. **19**, the display modes can be toggled between large numeric display screens, waveform/numeric display screens, and trend data display screens. According to this example, pressing the display button **104** allows the user of the monitoring device **20** to toggle between a large numerics display screen **336**, a single waveform display screen **210**, and a tabular trend display screen **470**, respectively. Depending on the configuration settings of the herein described monitoring device **20**, the display button **104** could be used to navigate between each of the display screens shown in FIGS. **15**, **17** and **18**, respectively, wherein a default version of each type of display screen can be determined.

In terms of overall navigation with regard to any of the above primary display screens and in general according to this embodiment, the display cursor, as referred to above, is always highlighted. Referring to FIG. **21**, and looking at an exemplary display screen, in this case a dual waveform display screen **332**, each and every display screen according to this embodiment includes a single element—the current con-

text—labeled herein as **407**, that is shown by a first colored field (e.g., blue) in order to highlight the element.

Using the user interface **92** of the herein described monitoring device **20**, pressing the SELECT button **96** causes the monitoring device **20** to replace the current display screen with another display screen that is related to the current context. By way of example, if the SpO₂ text identifier is highlighted in the display screen **332** of FIG. **21**, and the SELECT button **96** is pressed, the monitoring device **20** is programmed to then display a SpO₂ control menu **402**, having a specified format and shown in FIG. **22**, onto the primary display screen. The directional buttons **100** can be used to scroll the display cursor in order to highlight the item to be selected by the user.

In addition, there are at least some display screens that also contain elements—parameter values—that are highlighted by a second colored field (e.g., green). In the case of the second color highlighted areas, the current values of multiple parameters are identified within a given context. For example and in the control menu display screen of FIG. **22**, the current context of the SpO₂ monitoring menu option **403** is highlighted in the primary or first color (e.g., blue), while the current settings **404** of the SpO₂ parameters according to this embodiment are highlighted in the second color (e.g., green). Control menus and other menus are discussed in a later portion of this description.

In passing, other forms of indications can be provided on a display screen to a user using various colors or are provided with separate indicators in accordance with this embodiment. For example, items listed in red as shown in the display screen of FIG. **20** indicate readings **396** that exceeded a given alarm limit (either an upper or a lower limit) in addition to the current context **392**, for example. Other examples are provided. For example, the trend tabular display screen **470** presented in FIG. **56** depicts a number of readings **475** that have been compared to known limits and have been suitably identified.

In addition to the display button **104**, the herein described monitoring device includes a set of embedded menus that are used for at least two purposes. First, certain menus (e.g., context menus) permit the user to navigate between various modes of the monitoring device **20**. Second, other menus permit adjustments to be made to the monitoring device **20**. These adjustments are intended to be temporary and typically relate to the specific patient being monitored. As previously noted, device settings are typically configured through factory default settings. A technique using a configuration file using the charging cradle **140** as an intermediary relative to a portable computer **192**, FIG. **6**, has also been discussed as an option to permit at least some of the factory settings to be overridden. The monitoring device **20** further permits custom configuration at the user level using a variety of display menus that can be accessed through the user interface **92**. For purposes of explanation herein, two (2) main types of menus can be accessed, pop-up (also referred to throughout the discussion as drop-down) menus and control menus. Each of these menus will now be described with regard to the present embodiment. Other menus assist in navigation through and between various display screens in addition to the herein described display button **112**. These menus have been alluded to with regard to the start-up display screens, FIG. **24**, and information screens, FIG. **27**, noted above and are referred to as context menus.

First, pop-up or drop down menus are provided to allow a user to temporarily make configuration settings for the herein described monitoring device **20** as well as to vary certain formats, for example, for display. The menus also affect various modes of the device, among other features, as will now be

described. In brief, the display cursor is used to highlight an item in any primary display screen **210**, **332**, such as shown in FIGS. **15**, **16**, using the directional buttons **100** of the user interface **92** and the SELECT button **96** is pressed to access a corresponding drop-down menu. As shown, for example, in FIG. **53**, the resulting pop-up or drop down menu appears as an overlay onto the primary display screen **590** wherein the format of each corresponding menu includes a header text and a plurality of listed menu items or options. According to this embodiment, there are at least ten (10) drop down menus available for the herein described monitoring device **20**, each of which enable certain settings of the device to be temporarily altered for a particular patient.

A patient mode drop down menu **540**, FIG. **29**, is accessible by highlighting the displayed patient mode field **224** as provided on any primary vital signs display screen **210**, FIG. **15**, in the status panel **320** thereof and pressing the SELECT button **96**. The current or default patient mode **544**, in this case, an Adult mode, is highlighted and the directional arrow buttons **100** of the user interface **92**, FIG. **2**, enable the mode to be changed to pediatric mode, shown as **556**. When a patient mode is changed according to this embodiment, all stored vital signs data, including any snapshot and trended data, for the patient is deleted automatically from the CPU **174** and all monitoring device settings revert to the default settings for the new patient mode that is selected. Therefore and when changing a patient mode, a confirmation screen **550**, see FIG. **30**, appears as an overlay on the display screen, shown herein as **554**, indicating that parameter values will be changed to default settings for the mode now selected and further indicating that all stored information will be lost if the patient mode is changed. Confirmation is then required before any new mode selection can be implemented by the user wherein confirmation changes the patient mode and removes the confirmation message panel **550** from the display screen **554**. The resulting display screen (not shown) then indicates pediatric in the patient mode field **224** thereof.

As noted previously and referring to FIG. **6**, the monitoring device **20** includes a wireless RF radio card **180** and internal antenna **182** which when enabled, automatically establishes a wireless communications link between the monitoring device **20** and the central monitoring station **184**. While within the confines of a wireless LAN (Local Area Network), this connection is suitable within range of a suitable access point **186**. The communication status indicator or icon **212** located on the status panel **320** of any primary display screen **210**, such as those shown in FIG. **15**, is configured to provide an indication of the status of the wireless connection with the remote monitoring station **184**, which is limited, for example, given the distance between the monitoring device **20** and an access point **186** on the network. For example, if the status indicator **212** is blank, according to this embodiment, then the monitoring device **20** is not enabled for communication with the remote monitoring station **184**. This status indicator **212** can provide certain information concerning the connection as follows according to this embodiment: If the communication status indicator **212** flashes, this is an indication that the monitoring device **20** is associated with an access point **186**, but the device is not communicating with the remote monitoring station **184**. If the communication status indicator **212** has a line appearing through it, the indicator being presented as shown in FIGS. **15-18** as an antenna symbol, then the monitoring device **20** is not communicating with an access point **186**, FIG. **6**, and is not communicating with the remote monitoring station **184**. As previously noted, the communication status indicator **212** according to this embodiment is located at the upper right hand corner of the status panel **320**

in any primary display screen. Similar indications can be made using the status indicator **212** when the monitoring device **20** is communicating with a PC **192** and not with the network, and whether the monitoring device is associated with the network and is communicating with the remote monitoring station **184**.

Due to battery constraints it is desirable when the monitoring device **20** moves out of range of the access point **186**, that the user can selectively disconnect the monitoring device **20** from the wireless network and place the device in a disconnected wireless mode. This selective disconnection is highly desirable given the considerable drain to the battery resources that occur when attempting to restore communications with the remote monitoring station **184**, FIG. **6**, as the device would continue to attempt to restore communications even when the device is out of range. According to one version according to the present invention, this selective disconnection is achieved through software wherein the user highlights the communications status indicator **212** of primary display screen **210**, FIG. **15**, or any display screen having a status panel **320** using one of the directional arrow buttons **100** pressing the SELECT button **96**.

According to this embodiment and referring to FIGS. **48** and **49**, a disconnected wireless icon popup or drop-down menu **560** (if the device is enabled with a wireless transceiver **180** and antenna **182**) is accessed by which the user is permitted to selectively toggle into and out of a disconnected wireless mode.

The pop-up menu **560** includes a set of menu options, including a disconnect option **564** which the user can elect to disconnect the monitoring device **20** from the wireless network by scrolling using the appropriate directional arrow buttons **100** and highlighting the disconnect menu option. This election is further indicated to the user by one of the status indicators **169**, FIG. **2**, provided on the front facing side **84** of the monitoring device **20**. During the time that the monitoring device **20** is disconnected from the network, the device provides only local respiration, NIBP, HR/PR and SpO₂ alarms or equipment alerts. During that time, a Disconnect message **568** is also displayed to the user next to the communication status indicator **212** on the display screen **210**, the latter having a symbol indication of disconnection, as shown in FIG. **49**. The use of the disconnect feature provides an advantage in that battery/device power is conserved while the monitoring device **20** is out of range. During the time the above wireless disconnect feature is utilized, trended vital signs data continues to be stored within the memory of the CPU **174**, as per normal operation.

When the monitoring device **20** is again within range of the network, the communication status indicator **212**, FIG. **15**, provides a signal that the monitoring device **20** is within range and network connection can be restored by again highlighting the communication status indicator **212** to access the wireless mode menu **560**, highlighting a Reconnect menu option (not shown), and pressing the SELECT button **96**. This selection automatically causes a prompt that is displayed to the user for information concerning the patient and the network. A similar message is displayed at the remote monitoring station **184**. Reconfiguration and handshaking of the herein described monitoring device **20** with the wireless network is as described in the previously incorporated U.S. Pat. No. 6,544, 174. At the time network connection is restored, all trended data stored during the time the monitoring device **20** was disconnected is transmitted to the remote monitoring station **184**, FIG. **6**, over the wireless network.

While the wireless version of the herein described monitoring device **20** is connected over the network, patient data

gathered by the monitoring device is continuously stored at the remote monitoring station **184**. At the remote monitoring station **184**, patient information can be accessed and administrative functions can be performed including admitting, transferring and discharging the patient from the remote central monitoring station unit, editing the patient description (name, primary care physician), and reviewing and printing patient data, including trends and waveforms.

Other pop-up or drop-down menus are provided according to this embodiment for temporarily configuring other settings of the monitoring device **20** include a waveform source popup menu **580**, see FIGS. **32**, **33**, that provides user selections for determining which waveform is being displayed (e.g., resp, ECG including choice of vector) and for switching, for example, between a single waveform display screen **210** and a dual waveforms display screen **332**, FIG. **16**. This latter menu **580** is accessed by the user by highlighting the waveform source field **232** on the display screen **210** and pressing the SELECT button **96**. According to the present embodiment and for all waveforms, except respiration, the monitoring device **20** further includes means for cascading a display in order to sweep a single waveform through two panels, thereby showing or presenting a waveform covering a 2× time period (e.g., 6 seconds to 12 seconds). FIG. **32** illustrates an example ECG waveform having a default menu option **584**, with FIG. **33** depicting a user option **588** for a respiration waveform using the menu **580**.

Similarly, a waveform size drop-down menu **600**, FIG. **34**, permits user selection relating to the size of displayed ECG, SpO₂ or respiration waveforms relative to any display screen **332** by highlighting the waveform size text identifier **236**, located in the waveform panel **344** and selecting a menu option **604**. A sample respiration waveform **608**, FIG. **37**, is shown that is augmented by this size menu.

A trend display pop-up menu **640**, FIG. **53**, permits selection between various forms of trended data (tabular, waveform, snapshot) by highlighting the data display header **364**, FIG. **52**, in the trends live numerics panel **356**, FIG. **52**, of a trended display screen, in this instance, a snapshots display screen **590**. As previously noted, tabular screens are shown in FIGS. **54-56** and a graphical trend display screen **380** is depicted in FIG. **57**.

Similarly, a trend view interval popup menu **660**, FIG. **55**, is accessed by highlighting the Time heading in the data display panel **474**, the menu permitting the time intervals between trended data listed to be selectively varied by the user.

Additional pop-up menus according to this embodiment include a snapshot waveform source popup menu, a graphical source pop-up menu and a snapshot selection pop-up menu. Each of these embedded menus are similarly accessed by highlighting the appropriate text identifier and pressing the SELECT button **96** to affect temporary configuration setting changes for the device **20**. In addition, an SpO₂ spot check or random pop-up menu **620**, FIG. **41**, is also provided, details being provided for this latter feature in a succeeding section.

A "control" menu for purposes of this embodiment includes a topic name for the current context (for example, SpO₂, in FIG. **22**), each menu being defined by a stored formatted template comprising a first display panel having a column of parameters with one of the parameters highlighted (for example, SpO₂ Monitoring), and a column of options, with one item in the set of options being highlighted (for example, Standby, On, **100**, On, **90**, Low). The primary (e.g., blue) highlighted item indicates the parameter that is currently enabled for modification, while secondary (e.g., green) highlighted items indicate each of the current settings for all

parameters in the control menu. Each control menu further includes a context menu at the bottom of the control panel in order to enable navigation as well as permit confirmation or cancellation of a choice/option selected by the user, such as in the instance of the start-up display screens **400(a)**, **400(b)**, FIG. **24**. Presently, the monitoring device **20** described herein includes at least nine (9) control menus that are accessible by the user.

As noted, each control menu can provide customization of the configuration of the monitoring device **20** for the current patient and to confirm choices. As in the preceding, each control menu can be accessed using the directional arrow buttons **100** to locate and highlight the item to be controlled and pressing the SELECT button **96**, as previously described. It will be readily apparent that the number and arrangement of these menus is exemplary and that other variations and modifications are possible within the intended ambits of the invention. Additionally, it should further be noted that each of the following controls can be similarly modified from the remote monitoring station **184** over the wireless connection with the monitoring device **20**.

First, a time setup control menu **700**, FIG. **31**, allows the time, date and time format used by the monitoring device **20** to be locally modified by the user. More particularly and according to this embodiment, the time format (12 hour/24 hour), hour, minute, month, day, year, year and year format can be selectively adjusted by the user. The time and date can also be confirmed for correctness as the monitoring device **20** is capable of displaying time in either 12 hour (AM/PM) or 24 hour format, and displays the date in either a month/day/year, day/month/year, or other suitable format. According to this embodiment, the date does not appear in the primary display screens but does appear in both a snapshot list and associated snapshot data, details of which are described below. Highlighting the time display **216** (located in the upper right corner of a primary vital signs display screen **210** or any display screen having a status panel **320**) and pressing the SELECT button **96** to accesses the Time/Date control menu **700**, the screen allowing changes to be made and stored into memory by the monitoring device **20**.

Additionally, a number of parameter control menus are accessible, including an NIBP control menu, an SpO₂ control menu, a HR/PR control menu and a respiration control menu, respectively. Each of these parameter control menus can be accessed by either selecting the parameter text identifier in any primary display screen such as **210**, FIG. **15**, or by selecting the alarm bell icon **268**.

More specifically, the NIBP control menu permits the setting of upper and lower alarm limits for each of the systolic, diastolic and mean pressures as well as the selection of a digital manometer, the selection of a specific NIBP mode and the time interval used when an automatic mode is enabled. An exemplary NIBP control menu **720** is shown in FIG. **23**. The NIBP control menu **720** is defined by three panels according to the present embodiment. The uppermost panel **722** includes a listing of menu options that can be elected by the user. The second field **724** includes a listing of submenu options associated with each menu option from the first panel **722**. The third panel is a context menu panel **416** that includes a series of navigational options.

More specifically with regard to the herein described monitoring device **20**, NIBP measurements can be taken through a user-selected automatic mode in which blood pressure readings are taken at prescribed time intervals. Following the correct positioning of a proper sized cuff **76**, FIG. **1**, on a patient, and screwing the hose end into the NIBP air connector fitting **48**, FIG. **3**, provided on the top facing side **52** of the

device housing 24, FIG. 3, the automatic NIBP mode can be enabled by highlighting the NIBP text identifier in the primary vital signs display screen 210, FIG. 15, and pressing the SELECT button 96. The above selection accesses the NIBP control menu 720, shown in FIG. 23, wherein the NIBP Mode option is scrolled to and the Auto menu suboption in the second panel 724 is selected using the directional control buttons 100 to highlight the desired mode and pressing the SELECT button 96. An appropriate time interval can then be selected by highlighting the Auto Time Interval (min) suboption in the panel 724 that will provide automatic blood pressure measurements at the prescribed intervals (e.g., 3 min, 5 min, 15 min, 30 min, 60 min, etc). It should be noted that the incorrect placement or failure to place the cuff 76 on the patient will still enable automated mode, but an equipment alert will be sounded by the monitoring device 20.

The automatic NIBP mode can be disabled by highlighting the NIBP text identifier on the primary vital signs display screen 210 using the directional control buttons 100, pressing the SELECT button 96 to access the NIBP control menu, FIG. 23, and then highlighting NIBP mode from the NIBP control menu 720 and selecting the Manual menu option using the appropriate directional control buttons 100.

Otherwise, any blood pressure reading can be taken manually after positioning the correct cuff 76, FIG. 1, and hose 80, FIG. 1, relative to the patient, screwing the hose end into the NIBP air connector fitting 48, FIG. 3, provided on the top facing side 52, FIG. 3, of the housing 24 and pressing the NIBP start/stop button 112. As previously noted, all manual and other NIBP mode measurements are stored as trended data by the monitoring device 20.

In addition, an enhanced blood pressure measurement mode (herein referred to as "Turbo" mode) is provided in which the monitoring device 20 automatically initiates a blood pressure measurement reading in a conventional manner and then takes as many readings as is possible within a predetermined time period (e.g., 5 minutes), provided this option is enabled by way of default configuration settings such as through the downloaded configuration file. Turbo mode, as defined herein, can be set through the user interface 92 by highlighting the NIBP text identifier in any primary vital signs display screen 210 and pressing the SELECT button 96 to access the NIBP control menu 720, FIG. 23, as previously described. The NIBP Mode menu option can then be highlighted with the Turbo suboption then being selected using the appropriate arrow button 100. Selecting the NIBP start/stop button 112 or highlighting the NIBP Mode Manual menu option from the NIBP control menu 720 will restore the monitoring device 20 to a manual NIBP measurement mode.

As noted generally above, the patient monitoring device 20 according to the present embodiment further includes a digital manometer that can be selectively displayed for the user during a blood pressure measurement procedure. This feature is enabled through the NIBP control menu 720 which is accessed in the manner previously described above from any of the primary vital signs display screens. In the NIBP control menu 720, FIG. 23, the Manometer option listed therein in the top panel 722 is highlighted using the directional arrow buttons 100. Pressing the SELECT button 96 causes a manometer menu 730 to appear as an overlay on the display screen 210, as shown in FIG. 44. Pressing the NIBP start/stop button 112 starts the NIBP measurement cycle as previously described. When the attached cuff 76, FIG. 1, is inflated, a manometer pressure indicator bar 734 located at the bottom of the display screen 210 dynamically displays the pressure reading, as shown in FIG. 45. When the blood pressure measurement cycle is completed, measurement numerics 742

appear below the waveform grid of the display screen 210 and each of the systolic, diastolic and MAP values for the measurement are displayed as markers 738, if valid readings are obtained for each along a defined manometer scale, as shown in FIG. 46.

Adjustment and enablement of the alarm limits and the remaining options on the control menu 720 are selected in the same manner described above. As to the context menu panel 416 options for parameter control menus and referring for example to FIG. 44, the Exit menu option, if selected by the SELECT button 96, reverts the user back to the previous primary vital signs display screen, the Trends option changes the display screen to a trends viewer screen that causes a tabular or waveform history to be displayed, the Snapshots menu option causes a series of 21-second waveform snapshots of the current patient's vital signs to be selectively viewable, and the Setup menu option accesses the setup control menu.

The SpO₂ control menu 402, FIG. 22, permits setting of either continuous or a random (herein also commonly referred to as a spot-check) SpO₂ measurements, the setting of alarm limits and setting of the pulse tone. According to the present embodiment, continuous measurement of at least one physiologic parameter other than SpO₂, such as ECG, is enabled through the CPU 174 and the tethered physiologic parameter sensor assemblies, while permitting the user, by means of the user interface 92, to manually "spot check" SpO₂. That is to say, SpO₂ can be periodically or randomly checked on the patient (not shown) while simultaneously maintaining continuous monitoring of at least one other physiologic parameter.

When continuous SpO₂ is enabled, an alert is generated each time that SpO₂ readings are interrupted, such as when the sensor is disconnected from the patient after the monitoring device 20 has begun to take SpO₂ readings. Using the random monitoring or "spot check" feature, any number of randomly taken readings can be taken, attaching and detaching the sensor repeatedly without generating any alarms.

Referring to FIG. 39, a flowchart generally describes the herein referred to random or spot checking monitoring feature. Initially, the SpO₂ monitoring function of the monitoring device 20 is turned off. The user can turn the continuous SpO₂ monitoring function off manually with the user interface 92 by scrolling to the primary vital signs display screen, FIG. 21, and highlighting the SpO₂ text identifier 407 and pressing the SELECT button 96. The preceding accesses the SpO₂ control menu 402, FIG. 22. This control menu 402 is defined by two panels; a first panel 746 that includes a list of menu options and suboptions and a context menu panel 416 permitting navigation out of the spot-check mode. Highlighting the SpO₂ Monitoring menu option 403, using the left arrow button 100 to highlight the Off suboption and pressing the SELECT button 96 then turns off the continuous monitoring function and turns the spot checking feature.

When the SpO₂ monitoring function has been deactivated, it can then be reactivated by the user, either for continuous monitoring or for a one-time spot check reading. When a spot check is desired according to this embodiment, the pulse oximeter sensor 60, FIG. 1, is attached to the monitoring device 20 and to the patient. The user then highlights SpO₂ on the primary vital signs display screen, FIG. 40, and presses the SELECT button 96. Upon pressing same, the user then highlights SpO₂ @ XX:XX and presses the SELECT button 96 accessing a SpO₂ drop-down menu 620, FIG. 41. This menu 620 that appears as an overlay onto the display screen (not shown in this view) includes On, Off and Spot Check options. The On option 622 permits the user to reenale the

continuous SpO₂ monitoring feature. The Off option **624** disables the continuous monitoring feature and enables spot checks. The Spot check option **626** is highlighted in this instance, since the SpO₂ continuous monitoring function has already been disabled. The spot checking feature of the herein described monitoring device **20** is controlled through logic contained within the monitoring device **20** that allows the SpO₂ hardware to first initiate the sensor assembly **32**, FIG. **1**, and acquire a stable SpO₂ measurement from the patient as sensed by the apparatus. According to this embodiment and referring to FIG. **42**, the primary vital signs display indicates SpO₂ Spot Check with a text identifier "SEARCH" **628** displayed above a Spot Check text identifier **629** to indicate that the monitoring device **20** is waiting for pulse oximetry data from the patient. After a few seconds, the SpO₂ indicator (if SpO₂ is used to determine pulse rate begins to display pulses and after approximately 30 seconds, the SEARCH text identifier **628** disappears and a pulse oximetry reading **256** appears, FIG. **43**. Once a stable measurement has been acquired, the SpO₂ subsystem is powered down automatically. The stable SpO₂ reading that has been obtained is then displayed for a predetermined period of time or until a new spot check reading of SpO₂ is acquired. For additional spot checking, the preceding steps are then repeated wherein the SpO₂ sensor assembly **28** is initiated; a stable reading is acquired and then displayed for a predetermined period of time. In the meantime, any other parameters that are continuously monitored, such as ECG, are unaffected by the spot-checking functionality feature.

Each of the HR/PR and respiration control menus as well as the NIBP and pulse oximeter control menus permit the setting of upper and lower alarm limits. The HR/PR control menu (not shown) further permits adjustment of volume or enablement of the heart tone, and the preferred source (either SpO₂ or ECG) for heart rate wherein the current source is also highlighted. The respiration control menu (not shown) also permits the selection of the reference leadwire used from the ECG monitoring assembly.

In addition to the above parameter control menus and the time setup control menu, set-up control menus are also provided to the user in order to define the behavior of the herein described monitoring device **20**. A typical set-up menu can be accessed according to this embodiment from any main display screen, such as those depicted in FIGS. **15-19**, by performing the steps of: highlighting the battery indicator icon **220**, HR/PR text identifier, SpO₂ text identifier, NIBP text identifier, respiration text identifier or the alarm icon **268**; pressing the SELECT button **96** thereby accessing a parameter control menu; highlighting the setup option located in the context menu panel **416** at the bottom of the display screen **210**; and pressing the SELECT button **96** again.

Among the items that can be configured in the respective set-up control menus according to this embodiment are the suspension and enablement of the audible alarms and adjustment of alarm tones, permitting management of same in a patient context. As previously noted, an "alarm" warns of a patient condition, such as a vital-sign reading that is outside of acceptable limits. When an "alarm condition" occurs according to the present embodiment, the red light status indicator **169**, FIG. **2**, on the front facing side **84** of the monitoring device **20** flashes and the numerics of the violating alarm limits shown on the display **88** turn red, such as depicted in FIG. **20**. In addition, the display cursor moves automatically to the displayed item that caused the alarm and if not suspended, an audible alarm tone also may sound. A sample alarm condition **850** is shown in FIG. **58** in a single waveform display screen **210**. In this instance, the heart rate

for the monitored patient has exceeded a predetermined limit, as highlighted by **854**. In addition to the above and in the instance that the monitoring device **20** is connected to a remote monitoring station **184**, FIG. **6**, notification of the alarm condition may also be transmitted to the remote monitoring station. Pressing the alarm silence/resume button **112** will silence current alarm tone for a predetermined period of time (e.g., 90 seconds).

An "alert" refers to an equipment or device condition, such as a low battery or a detached lead. When an "alert condition" occurs, the yellow light indicator **169** on the monitoring device **20** flashes and a message describing the condition appears on the display **88** in a message panel. An example of an equipment alert, in this instance, the disconnection of an ECG lead, is shown by the display screen of FIG. **59**. Equipment alerts, according to this device embodiment, are indicated by a flashing yellow indicator **169** as well as a highlighted (e.g., yellow) alert message **306** provided conspicuously on the display screen of the monitoring device **20** and repeated sounding of an alert tone, in the instance that the alert is not acknowledged or the cause of the alert is not alleviated. The knowledge is made through a context menu located at the alert window screen. Preferably, an alert tone will be distinguishable from an alarm tone to a user. In this specific instance, the depicted equipment alert is an ECG lead failure. Therefore and in addition, a diagram **302** is illustrated with an indication (in this instance a circled X) to indicate at least one disconnected lead. Alarm and alert conditions can also be detected by the remote monitoring station **184**, FIG. **6**, via the wireless network.

Examples of alert conditions detected by the herein described monitoring device **20** include, but are not limited to, the following: ECG Faults which can include Lead failure (single, multiple), excessive offset, or detection of unplugged ECG cable; NIBP Faults that can include an air leak, kinked hose, overpressure cuff condition, weak pulses to determine systolic/diastolic pressure, no pulses detected, detection of artifact prevents valid reading, or low battery; Network Communication Faults including the detection of a network communication problem, detection in attachment to charging cradle, low battery, or no SpO₂ detected; and respiration channel faults, such as a noisy signal or lead failure. Still referring to FIG. **59**, acknowledgement of the alert by the user is made by highlighting the acknowledge option **864** at the bottom of the display screen and pressing the SELECT button **96**, FIG. **2**. Acknowledgement will remove the message panel and revert the display **88** to the previous display screen format.

Equipment faults for those situations in which the herein-described monitoring device **20** is operating on battery power as opposed to being mounted in the charging cradle have been discussed previously. In low battery conditions in which less than approximately 30 minutes of battery runtime remains, NIBP functions are disabled and the monitoring device **20** displays an appropriate message to the user that NIBP is disabled. Any attempt to press the NIBP start/stop button **112** or otherwise initiate a blood pressure measurement during a low battery condition will display an equipment alert with an appropriate message. However, placing the monitoring device **20** into the charging cradle **140** during a low battery condition will immediately enable all blood pressure monitoring features.

There are two techniques according to the present embodiment in order temporarily silence an alarm tone. The first technique is through pressing the alarm/silence button **108**, which will silence any current alarm(s) for a predetermined period of time (e.g., 90 seconds). It should be noted, that silencing the audible tone does not affect the remaining alarm

or alert indicators. The alarm tone can also, according to this particular device embodiment, be suspended for all parameters, thereby preventing the alarm tone from sounding if an alarm condition occurs while monitoring a patient. Suspension is done by the user through accessing an alarms suspend menu **880** that is provided in the set up controls menu **800**, as shown in FIGS. **60**, **61**. If an alarm condition occurs while the alarm tones are suspended, the monitoring device **20** presents visual alarm indicators, but does not sound an audible tone.

As opposed to the interval for silencing an alarm tone, the suspension period of the alarm tone can be set during configuration of the monitoring device **20** to disable the tone for a predetermined period (i.e., 90 seconds-60 minutes). In addition, the monitoring device **20** can be so preconfigured such that the alarm tone cannot be suspended by the user, for example, through use of the configuration file that is uploaded to replace the factory settings of the monitoring device using the PC **192**, FIG. **6**, as previously described.

Referring to FIGS. **60**, **61**, and if the suspend feature is not disabled for the present monitoring device **20**, the user can access the set-up control menu **800** by highlighting the text identifier of the parameter that is highlighted by the alarm. Once in the set-up control menu **800**, the user can highlight the Alarms option, thereby accessing the Alarms set-up menu **880**. As shown in FIG. **60** and upon accessing the Alarms setup menu **880**, the display cursor highlights the Off menu option wherein a message panel appears in the display screen **210** to use the directional right arrow button **100** in order to highlight the On suboption. Once suspension has commenced, FIG. **61**, a count-down timer **884** appears below the line in the set-up menu **880** as well as a highlighted indicator **888** in the upper portion of the display screen **210**. When the suspension period expires, the alarm tone is again enabled. The alarms set up menu **880** further permits the volume of the alarm tone to be selectively adjusted by the user.

Typically, each medical facility defines the patient alarm limits for adult, pediatric and neonatal patients and then configures the monitoring device **20** with those alarm limits prior to putting the monitoring device into service. As previously noted herein, it was noted that the user can locally or custom adjust certain configuration settings of the herein described monitoring device **20**.

According to another feature of the herein described patient monitoring device **20** and referring to FIG. **62**, upper and lower alarm limits can be temporarily customized for an individual patient while the monitoring device **20** is in use. This temporary customization feature can be implemented by the user by highlighting any vital sign of interest from a primary vitals signs display screen and pressing the SELECT button **96** so as to access the control menu for that parameter; in this instance, NIBP, **720**. Upper and lower alarm limits can then be selected by highlighting the current value and using the left and right directional arrow buttons **100** to set the new alarm limit(s), **726**, **728**. These new limit values are then stored in volatile memory of the CPU **174**, FIG. **6**, of the monitoring device **20** and are erased when the monitoring device is powered down unless the user specifically maintains them as part of the current patient. Alternatively, however, the device could be configured to allow a user such that the settings could be retained by the user irrespective of the patient. The monitoring device **20** is further configured to permit alarm limits to be customized for a particular patient from the remote monitoring station **184**, FIG. **6**, over the bidirectional wireless network using the radio card **180** and antenna **182** to receive new limit values.

In addition to the above features, the herein described monitoring device can be further configured such that the user

can perform alarm management on the monitoring device **20** by permitting the user to actuate a feature provided on the user interface **92** that creates a predetermined percentage change to the alarm limits for a single parameter each time the SELECT button **96** is depressed at the time of an existing alarm. The initialization and initial percentage settings for each of the alarm parameter settings is performed according to this specific embodiment as part of the configuration of the monitoring device **20** prior to use of the monitoring device **20** through the PC **192** using the configuration file to override factory configuration settings, the new settings being stored by the CPU **174**. A portion of a sample worksheet **198** is shown in FIGS. **64**, **65** in which factory settings **199**, shown in bold, can be adjusted for specific parameters, as listed in FIG. **64**. Completing the worksheet **198** through the utility thereby provides means for completing the configuration file and assigning preset percentage amounts for adjusting alarm limits for any single parameter during a current alarm(s). The worksheet includes a menu choice **197** for enabling the alarm limit percentage option herein, also referred to as ParamSet. In essence, the user of this selective alarm management setting feature permits both upper and lower alarm limits to be preset accordingly and then used selectively by the clinician/nurse.

In summary, four (4) techniques are now provided in the present monitoring device **20** for handling or managing an existing alarm: First, the user can temporarily silence an alarm through use of the alarm silence/resume button **108** provided on the user interface **92**. Turning the alarm off temporarily, however, in and of itself, does not change the limit. Therefore, if the patient's physiologic parameters are unchanged, the alarm will go off again momentarily depending on the default settings of the monitoring device **20** (e.g., 90 seconds). Second, the user can suspend the alarm tone for a patient for a predetermined period of time in the manner described above using the control menus **800**. This feature also does not change any alarm limits. Third, the user can temporarily change or customize any of the alarm limits individually through features provided on the user interface **92**, using the set-up control menus, as described above, such as **720** or other menu. As noted, this third technique can be accomplished by accessing the control menu for a specific parameter to highlight a specified parameter indicator (such as HR/min or NIBP, for example) and pressing the SELECT button **96**. The corresponding parameter control menu, FIG. **62**, is then displayed, permitting the user using the directional left and right cursor control buttons **100** to set appropriate alarm limits for the patient, the user then highlighting Exit to leave the menu window. Using the same pop-up menu or a similar menu, a fourth technique is provided by means of the presently described vital signs monitoring device **20** in which the user can also now automatically and selectively change a parameter alarm limit by a prescribed amount. Rather than incrementally changing the alarm limits, the user can change the alarm limits by a prescribed percentage amount each time the SELECT button **96** for this option is actuated as entered using worksheet **198**, FIG. **64**, via the configuration file. The latter feature can be accessed only during a current alarm(s). For example, upper and lower alarm limits for HR/PR can initially be set to alarm at an upper rate of 90 and a lower rate of 60. Using the latter feature, each time the SELECT button **96** is actuated for the above feature in the control menu, the alarm limits can be incremented by a predetermined percentage (e.g., 5 percent, 10 percent, or other). For example, if a five percent change were configured for the herein described monitoring device **20**, the alarm limits would change to **94** (upper)/**57** (lower) the first time the SELECT button **96** is

depressed, **99** (upper)/**54** (lower) the second time the button is depressed, and so forth. Similarly, NIBP (systolic pressure, diastolic pressure and mean pressure), SpO₂ and respiration rate limits can be similarly adjusted wherein the amount from factory (default) preset value alarm limit values can be adjusted, depending on the patient mode, for individual parameters as part of the pre-configuration routine using the PC **192**. A tabular listing **950** is shown in FIG. **65** for appropriate percentage changes to the alarm limits according to one example.

The ECG monitoring sensor assembly **28**, FIG. **1**, of the present embodiment includes a respiration circuit provided in the form of an ASIC, wherein breath signals using impedance pneumography supports measurement of respiration rate as well as central apnea. The herein described monitoring device **20** can monitor heart signs (ECG) and respiration rate using either a 3-lead or a 5-lead ECG cable. Using a 3-lead ECG cable, one signal waveform for lead I, II, or III can be displayed. Using a 5-lead ECG cable, either one or two signal waveforms can be displayed by the monitoring device **20** for leads I, II, III, V, and if enabled in the configuration, aVR, aVL, or aVF. The SpO₂ or Resp waveform can also be displayed in place of the ECG waveform.

To monitor ECG, the appropriate ECG cable is plugged into the device housing **24** and appropriate electrode sites are selected on the body of the patient. This selection process is commonly known and does not form a significant part of the present invention. At least three (3) electrode connections are required for ECG/Resp monitoring. The monitoring device **20** provides a graphic display **302**, FIG. **59**, of a three or five lead ECG attachment with fixed locations being indicated. The locations of the circles shown in the diagram **302** in FIG. **59** do not indicate the exact placement of the electrodes on the patient.

The monitoring device **20** is adapted to indicate whether some lead wires are not connected and to indicate an "ECG Fault" equipment alert and a chest diagram such as shown in FIG. **59**, indicating the general location of the disconnected lead or leads. If the disconnected lead(s) indicate that the waveform source (Lead) used for HR determination, then the monitoring device **20** automatically reassigns, if possible, the Lead used for heart rate (HR). If the reassignment succeeds, the monitoring device **20** then displays another equipment alert with the message "ECG Lead changed".

When all leads are properly connected, returning to the primary vital signs display screen will confirm that an ECG waveform is being displayed as well as heart rate and other patient data. The waveform source can be changed, for example, from Lead I to Lead II by highlighting the waveform source selection icon using the cursor control buttons **100** and pressing the SELECT button **96**. The latter will access the waveform source menu **580**, FIG. **32**, wherein the appropriate option **584** can be highlighted. In passing and by scrolling to the bottom of the waveform source choice menu, a second waveform can be added (or deleted). The waveform size can also be suitably varied by the user by highlighting the current waveform scale and pressing the SELECT button **96**. The waveform size pop-up menu **600**, FIG. **34**, is accessed through the latter selection and a desired scaling factor can be highlighted.

Respiration rate is also monitored using the ECG monitoring circuit, as noted above, based on impedance pneumography, wherein respirations can be sensed from the ECG electrodes. The respiration numeric is displayed in the lower right corner of the display screen. To view the respiration waveform, the waveform source identifier **232**, FIG. **15**, is highlighted and the SELECT button **96** is pressed in order to

access the waveform source pop-up menu **580**, FIG. **33**. Respiration as a menu option **588** is then highlighted and selected. Waveform size can be adjusted in the same manner described previously for the ECG waveforms.

In addition to monitoring the presence of the ECG waveform, the monitoring device **20** also detects the periodic signals emanating from an implanted pacemaker device. To that end, according to the present embodiment and referring to FIG. **35**, if the patient being monitored has an implanted pacemaker device, the monitoring device **20** can indicate the occurrence of pacemaker or pacer signals by activation of the Pacer Indicator option **904** from the ECG set-up control menu **900**, FIG. **36**, if not already configured. When activated, the Pacer Indicator displays and prints vertical dashed lines to indicate pacemaker signals. If the Pacer Indicator option **904** is not enabled, the monitoring device **20** according to this embodiment continues to detect the pacemaker signals, but does not display or print the pacer markers. If the pacer signal is sufficiently strong, the monitoring device **20** displays this signal as a waveform spike, whether the Pacer Indicator option **904** is enabled or not. The present ECG circuit also detects when pacer signals/EMI pulses are occurring too frequently (outside of the periodicity of realistic pacer signals).

As previously noted, the detection of these pacer signals is commonly affected by electronic noise (such as EMI—Electromagnetic Interference) triggered, for example, from overhead lights that can hinder the ability to adequately detect a pacer signal from an implanted patient device (i.e., a pacemaker). Electrical noise from a power source can also cause an unclear or noisy waveform. According to one aspect, the invention provides the ability to select amongst the various ECG vectors, each of which has been processed for pacer pulse detection of both polarities and feeds both the pacer pulse detector and a peak/noise floor detector. An example is shown in FIG. **63**. The latter detector generally captures a value **908** that is representative of the peak amplitude of real pacer pulses, and also captures a second value **912** that is representative of the peak amplitude of rapidly repetitive noise spikes, as shown in FIG. **63**. Means allow selection of available ECG vectors and after obtaining a peak and noise floor level signal from each, shown as **915**, **916**, respectively, then picking an optimum ECG vector to continue feeding the pacer pulse detector. If the noise floor signal is made available to the user, the user can observe how the magnitude of the noise floor signal changes while moving the monitoring device **20** about in the vicinity of a possible noise source, the latter being shown magnified as **918**. The reported signal level will generally increase as the monitoring device **20** is moved closer to the noise source and hence serves a directional aid in locating the source of electrical noise. Since it is already known at what level the noise spikes **912** would begin to trigger the pacer pulse detector, it may thus be determined whether a noise source was sufficiently large to cause false pulse detections. The principles described herein can be implemented by hardware, software or a combination of hardware and software.

The above circuit can further be used to validate a measurement in order to assess lead wire and electrode integrity for an ECG monitoring assembly. This measurement capability provides means for monitoring electrode performance as well as providing a means for proactively changing electrodes, as needed. As a matter of background and when lead wires of an ECG monitoring assembly are attached to a patient, the hardware drives a small current through each connected lead wire. This current is directed through the patient to a reference lead wire, also extending from the

patient. As a result, each lead wire produces an offset voltage (with respect to the reference lead) based on Ohm's Law.

According to a variant of the present invention, each lead wire's offset voltage delta (that is, the voltage difference between each of its lead wires) can be determined, thereby providing a means for qualitatively "ranking" each of the lead wires and electrode assemblies. Software included within the monitoring device can then be utilized in order to provide an assessment of the electrodes and the lead wires based on the computed deltas, at least to determine the "qualitative state" of the electrodes, (e.g., if one lead wire has a much higher offset than the remaining leads, the most likely cause is an electrode contact issue such as a dry electrode or loss of contact with the patient). By comparing ratios of these voltage differentials, it is therefore possible to anticipate or become proactive relative to the life of portions of the ECG monitoring assembly.

In addition to the above, the monitoring device **20** also includes a power source filter that can be enabled from the ECG set-up control menu **900**, FIG. **36**. The settings for the power source filter should be applied depending on the power source in the facility. To that end, the power source filter option **906** according to this embodiment includes settings of 60 Hz and 50 Hz.

Many factors can adversely affect a blood pressure (NIBP) measurement including cardiac arrhythmias, sudden changes in blood pressure, patient motion such as convulsions or shivering, sudden cuff movement, vibration, vehicle motion, or a weak pulse, among others. According to the present embodiment, and when NIBP and ECG are each being monitored with regard to a patient, the herein described monitoring device **20** can be further equipped with the selective use of a motion artifact filter, such as the Smartcuf artifact filter manufactured by Welch Allyn, Inc., in order to increase the measurement accuracy in the presence of moderate motion artifacts or diminished pulses. Specific details relating to the specific motion artifact filter utilized by this device are described in U.S. Pat. No. 6,405,076 B1, the entire contents of which have been previously incorporated by reference.

Enablement of an artifact filter feature would include the steps of mounting each of the ECG and NIBP assemblies to the monitoring device **20** and to the patient respectively and as previously described, and then simultaneously monitoring the patient using each of the above physiologic sensor assemblies. The set-up control menu **800** would be accessed in the manner described above from a primary vital signs display screen. Upon accessing the set-up control menu **800**, the NIBP menu option would be highlighted to access the NIBP setup control menu and then a Smartcuf suboption (not shown) would be highlighted and selected. Under some conditions in which the artifact filter feature is enabled and motion artifacts are too severe that measurement accuracy is still affected, the blood pressure measurement could be marked with an identifiable symbol on the display screen and on printouts. During certain types of arrhythmias and other situations in which a valid ECG signal cannot be obtained, the motion artifact filter could also be selectively disabled by accessing the control menu in the same manner described above, highlighting the NIBP option and disabling the Smartcuf sub-option.

The buttons of the user interface **96** and the display and/or backlight of the herein described monitoring device **20** can be locked out to prevent unauthorized access or use. This lock out feature can be accomplished in several different ways. According to one technique and if the feature is initially enabled using the PC configuration utility, the user can simultaneously hold down the left arrow, the right arrow and the up

button simultaneously for a continuous period of time (e.g., 5 seconds). All buttons, including the Power ON/Off button **56** are locked. The buttons are automatically unlocked when an alert or an alarm condition occurs. Similarly, the display **88** and/or backlight can also be locked out by the user using a selective combination of buttons if no operator activity (e.g., no buttons are pressed) has occurred for a predetermined amount of time. The backlight lockout and the display lockout features would again be disabled immediately after an alarm or alert condition occurs.

The remaining set up control menus that are available to the user according to this specific embodiment include that relating to the Demo Mode (Disabled, Low, High). In addition to the set-up control menus, the monitoring device **20** incorporates additional control menus according to this embodiment including a Device Status Control Menu; and a Message Control Menu. The Device Status Control Menu permits the user to see a displayed information screen **420(a)**, **420(b)**, such as shown in FIG. **26**. The information screen **420(a)**, **420(b)** includes separate panels **422**, **424** including the facility name, department name, and other associated information. The Message Control Menu is used, for example, with regard to changing of ECG leads in the event of a lead failure, requiring the reassignment of channels. At the bottom of each of the control menus are context menu panels **416**, allowing the user to navigate, the context menus for the set-up control menus being identical to those of the parameter control menus.

A more specific example of using a control menu is now herein described with reference to the display screen depicted in FIG. **22**. In this example, it is desired to alter (i.e., raise) the SpO₂ lower alarm limit to **95** and to shut off the HR/PR tone. To perform the first step and with "SpO₂" highlighted, the down arrow button **100** is used to scroll to highlight Lower Limit and the right arrow button **100** is then pressed as many times as necessary in order to increment the limit to the intended limit value; in this instance **95**. It should be pointed out the herein described monitoring device **20** is programmed such that the upper alarm limit cannot be decreased to a level that is lower than the lower alarm limit for the parameter. Similarly, a lower alarm limit cannot be raised to a level that is greater than or equal to the upper alarm limit.

To adjust the HR/PR tone, the down arrow button **100** is pressed to scroll down to the HR/PR Tone field and the left or right arrow button is pressed as many times as is necessary in order to highlight OFF. Pressing the SELECT button or the display button **104** will exit the control menu screen and return the display to the previous vital signs display screen.

When the control menu is exited, the values that are displayed at the time the menu is exited are the new default values for the monitoring device **20**. If a parameter is changed therefore, a decision must be made by the user prior to leaving the display screen whether or not to keep the previous setting values. If so, these parameters must be returned prior to exiting the control menu.

In summary and for purposes of menu and display navigation of the herein described monitoring device **20**, the directional arrow buttons **100** are therefore used to perform any of the following functions: highlight an item on display, selection of options from a control menu, set-up menu or displayed "pop-up" menu, and changing the values of numeric parameters.

According to this embodiment, the display button **104** in addition to cycling through the configured display formats as shown in FIG. **19** can also be used to return to a primary vital signs display screen from a control menu and for closing a "pop-up" menu.

Finally, the SELECT button **96** is used to perform the following operations: display the control menu for a primary highlighted item, return from a control menu to a primary vital signs display screen, provide access to a set up menu when setup is highlighted by the display cursor, display of tabular and graphical trends when trends is highlighted, display of snapshots when snapshot is highlighted, turn on the display or the back light if either has been turned off by a power save feature of the monitoring device **20**, and displaying a pop-up menu.

The herein described monitoring device **20** in addition to displaying current numerics and waveforms and the most recent measurements also stores a predetermined amount of patient data. According to this specific embodiment, up to 24 hours (at one-minute intervals) of trends (graphical and/or numeric) information for the patient being monitored can be stored, as well as NIBP and SpO₂ "spot checks" and "snapshots", as taken selectively by the user in connection with the patient and accessible from the Trends option of the context menu of any control menu, as described below. When data storage is at capacity, the data from each new reading overwrites the data from the oldest data stored. The features relating to the taking of SpO₂ and NIBP spot checks have previously been discussed at length.

As previously noted, a snapshot request is made by pressing the snapshot button **116**, FIG. 7, which is provided on the front facing side **84** of the device housing **24**. Upon depression of the snapshots button **116**, the CPU **174** is programmed to provide a graphical display **298** of a default waveform (ECG, respiration) for a selected lead for a predetermined time period along with additional information, such as shown in the exemplary display screen of FIG. 50. In the sample snapshot display screen depicted in FIG. 50 and according to this embodiment, for example, 21 seconds of stored ECG data (7 seconds after the snapshot button **116** is pressed and 14 seconds before the snapshot button is pressed) is presented along with a time and data stamp for each waveform, the waveform source detected, the waveform scale (size) used and the corresponding number of the snapshot. According to the present embodiment, up to twenty (20) snapshots can be stored by the monitoring device **20** wherein any new snapshots overwrite the oldest stored versions thereof. It should be readily apparent that the number of snapshots can be suitably varied.

This data can be reviewed at the monitoring device **20**. To review a snapshot and from any primary vital signs display screen, the user highlights any of the parameter text identifiers (HR/PR, SpO₂, etc) and then accesses a control menu for that parameter. The user then highlights the context menu panel **416** for that control menu and selects the snapshots option and confirms the selection by pressing the SELECT button **96**. Highlighting the Snapshots option causes a Snapshots display screen to be displayed, examples of which is depicted in FIG. 51-53. Each of the up to twenty snapshots can then be viewed by the user. In the example shown in FIGS. 51-53, five (5) snapshots were taken. The snapshot display screen **590** includes a status panel **320** at the top of the display screen, a live numerics panel **356** and a snapshot display panel **594**, respectively. The snapshot display panel **594** displays the stored snapshot for viewing and includes controls for selecting the snapshot file, the data source, the scale of the display and scroll controls. A vertical line indicates the center of the display. The waveform and numeric vital signs data during the 21 seconds can be viewed by the user by highlighting time interval provided at the bottom of the display screen **590** and using the directional (left/right) cursor buttons **100** to scroll the display to the desired time. An

example is shown in FIG. 52, for five seconds after the trigger point of the snapshot as opposed to FIG. 51, which is taken one second following the trigger point. The waveform source and size of the snapshot can also be selectively changed by the user for any captured snapshot by highlighting the appropriate icon on the display screen and accessing an associated drop-down menu **580**, **600**, as shown in FIG. 32, 33. In this example, the user can optionally switch to another type of display or can exit and return to a primary vital signs display screen by highlighting Snapshots in the upper left corner of the display screen and pressing the SELECT button **96**. The preceding accesses a Trends menu **640**, FIG. 53, wherein highlighting the appropriate option allows the user to navigate to another display screen.

As noted, the monitoring device **20** also stores trend data that is viewable in a plurality of user selectable formats. Trend data can be reviewed in a manner similar to that of waveform data by highlighting any parameter icon from any primary vital signs display screen, FIG. 53, and pressing the SELECT button **96**. Highlighting Trends from the resulting pop-up menu and pressing the SELECT button **96** accesses the Trends display screen **470**, an example of which is shown in FIG. 54. The trends display screen **470** displays tabular trend data as well as live numerics for the monitored patient, the screen having a format consisting of a status panel **320**, a trends live numerics panel **356** and trends panel **474**, respectively. The status panel **320** is similar to that previously described with respect to FIG. 15 and the live numerics panel is similar to that depicted in FIG. 18. The trends panel **474** includes a tabular listing taken at one minute intervals with current vital sign readings for the monitored patient at the top of the display screen above the tabular list. As shown in this example, the reading time, HR/min, blood pressure (systolic/diastolic/mean), Respiration rate/min, and pulse oximeter (SpO₂) readings are provided. The user can scroll through the displayed tabular list using the directional (up/down) cursor buttons **100**. The listing can include indications to show those readings that have already been captured in terms of snapshots, and any readings (if any) that are outside of permissible limits. Referring to FIG. 54, the user can selectively change the time interval for the displayed trend data by highlighting the Time text identifier **476** in the display screen **470** and accessing a view interval "pop-up" menu **660**, permitting the user to selectively change the time (e.g., 5 minutes, 15 minutes, 30 minutes, 60 minutes) as needed by highlighting same and pressing the SELECT button **96**.

FIG. 56 represents a sample display screen similar to FIG. 54, but indicating readings that have either exceeded alarm limits or appear suspect.

When attached to the charging cradle **140** and the PC **192**, as shown in FIG. 6, all captured snapshots are caused to be automatically printed, if the monitoring device **20** is on for subsequent printing by the printer **195** through the USB data link with the PC **192** and the charging cradle **140**. The data is uploaded to the PC **192**, either manually or automatically through software loaded into the PC. According to the one version, all stored patient data is automatically printed when a powered monitoring device **20** is placed into a charging cradle **140**. If the monitoring device **20** is off when placed in the charging cradle **140**, then the autoprint feature is disabled. To enable the autoprint feature, the user must power up the monitoring device **20** and select Continue Patient in the start-up display screen **400(b)**, FIG. 24. Tabular trend data and snapshots stored within the monitoring device **20** are printed.

Pressing the Power On/Off button **56** accesses a Power Off display screen as shown in FIG. 47. The format of the Power-Off display screen **940** includes a status panel **320**, a notice

41

panel 408, a short message panel 412 and a context menu panel 416, as read from the top of the display screen. If there is an intent to monitor the same patient when the monitoring device 20 is turned on again, then it may be desired to save the stored vitals signs data and monitoring device settings. As such, two options are provided in the context menu panel 416 at the bottom of the display screen 940—to either delete the stored data and settings and shut down or to save the stored data and shut down. Highlighting either of these options using the directional arrow buttons 100 and pressing the SELECT button 96 will cause the monitoring device 20 to shut down and either save or delete the stored data and settings. Alternatively, if the Power Off button 56 is pressed and the user wishes to continue monitoring the same patient, then a Cancel option is also provided in the Context menu panel 416 of the display screen 940. Failure to act within a predetermined time period according to this embodiment, as measured by an internal timer, will revert the display screen 940 to the previous screen or the default display screen as configured by the monitoring device 20.

Variations of the herein described monitoring device and associated hardware and software are possible within the intended scope of the inventive concepts in accordance with the following claims.

What is claimed is:

1. A multi-parametric patient monitoring device comprising:

a device housing that retains a portable power supply, a CPU, and a display for permitting the monitoring device to operate in a first stand-alone mode wherein a plurality of physiological sensors are attached to said device housing and in which parameter data received from said sensors is processed by said CPU within said device housing;

a wireless transceiver enabling said monitoring device to operate in a second mode in which patient-related data is transmitted to a remote station and in which said monitoring device is further configured to be separately operated in a separate charging mode wherein said device can still operate simultaneously in the second remote wireless transmitting mode while in said charging mode, said device further including a wired transceiver to permit patient-related data transfer remotely in said charging mode, and in which said device simultaneously transfers data over each of said wired and said wireless transceivers,

wherein a plurality of physiological parameters are continuously monitored by said monitoring device, said monitoring device further comprising a pulse oximeter assembly in which said monitoring device is programmed to continuously monitor at least one of said plurality of physiological parameters while said pulse oximeter assembly is enabled to selectively operate in each of a continuous monitoring mode and a spot-check monitoring mode and in which the at least one of said plurality of physiological parameters is continuously monitored independent of the monitoring mode selected for the pulse oximeter assembly.

2. A device according to claim 1, in which the monitoring device is placed in a charging cradle in the charging mode, the charging cradle including a data port to permit communication between said patient monitoring device and at least one peripheral device.

42

3. A device as recited in claim 1, wherein said monitoring device is patient wearable in said first and second modes.

4. A device as recited in claim 2, in which the peripheral device is a large display wherein patient-related data is further transmitted in real time to said display in said charging mode using said data port.

5. A device as recited in claim 2, in which the peripheral device is a computing device.

6. A device as recited in claim 5, in which the computing device sends a configuration file to the patient monitoring device providing default settings for said monitoring device.

7. A device as recited in claim 5, in which said computing device automatically receives stored data from said patient monitoring device when said monitoring device is attached to said charging cradle.

8. A device as recited in claim 2, wherein said CPU includes memory for storing and trending patient-related data, said device further including a user interface that permits snapshots of data to be selectively taken, wherein all trended data and snapshot data is automatically transmitted when said patient monitoring device is attached to said charging cradle.

9. A device as recited in claim 1, including a user interface defined on said housing having a plurality of user-actuable buttons for operating said device, and in which said buttons can selectively be locked out.

10. A device as recited in claim 1, including a display having a backlight, and in which said display and the backlight can be selectively powered off to prevent unauthorized access.

11. A device as recited in claim 10, wherein at least one of the display and the backlight can be powered down based on inactivity of said device.

12. A device as recited in claim 1, including an ECG assembly, said ECG assembly including a pacer detection circuit for determining pacer spikes.

13. A device as recited in claim 12, wherein said ECG assembly determines an appropriate ECG vector for electrical noise detection using pacer spikes from the pacer detection circuit.

14. A device as recited in claim 1, wherein the wireless transceiver can be selectively powered down if the transceiver is out of range of an access point.

15. A device as recited in claim 9, wherein said user interface includes a plurality of buttons that are used with a display screen to navigate using drop-down menus that are accessed through the user interface.

16. A device as recited in claim 15, wherein said user interface can access a disconnected wireless mode menu in which the device can be selectively switched between a disconnected wireless mode and said wireless mode.

17. A device as recited in claim 1, wherein enabling said monitoring device in said spot-check monitoring mode permits a sensor of said pulse oximeter assembly to be continually removed and attached from a patient without alarm generation.

18. A device as recited in claim 17, wherein enabling said monitoring device in said continuous monitoring mode generates an alert each time said sensor of said pulse oximeter assembly is removed from the patient.

* * * * *

专利名称(译)	生命体征监测		
公开(公告)号	US8932217	公开(公告)日	2015-01-13
申请号	US11/795301	申请日	2006-01-13
[标]申请(专利权)人(译)	伟伦公司		
申请(专利权)人(译)	伟伦 , INC.		
当前申请(专利权)人(译)	伟伦 , INC.		
[标]发明人	GIBSON GRANT S GONDEK CORY R SUNDERLAND RICHARD A BAKER STEVEN D LEWIS ROBERT T LATHROP BRAXTON L DUNN CHRISTOPHER L KOTZER OMER		
发明人	GIBSON, GRANT S. GONDEK, CORY R. SUNDERLAND, RICHARD A. BAKER, STEVEN D. LEWIS, ROBERT T. LATHROP, BRAXTON L. DUNN, CHRISTOPHER L. KOTZER, OMER		
IPC分类号	G06F19/00 A61B5/00 A61B5/0205 A61B5/024 A61B5/0424 A61B5/1455		
CPC分类号	A61B5/0205 A61B5/02438 A61B5/0424 A61B5/14551 A61B5/6843 A61B5/6887 A61B5/742 A61B5/7475 A61B5/002 A61B5/0022 G06F19/3406 A61B5/7275 A61B5/746 A61B2560/0276 A61B2560/0456 G06F19/00 G16H40/63 A61B5/021 A61B5/024 A61B5/04012 A61B5/0402 A61B5/0816 H02J7/0042		
审查员(译)	THOMSON , WILLIAM		
优先权	60/643636 2005-01-13 US		
其他公开文献	US20080281168A1		
外部链接	Espacenet USPTO		

摘要(译)

一种多参数生命体征监测装置，被配置为用作门诊和床边监测器，其中所述装置可以是患者可佩戴的并且是电池供电的。监视设备可以与充电支架一起使用以向设备提供电力而不是作为床边应用的电源的电池，其中支架还用作中间设备以实现与PC或其他外围设备的数据链接。设备。监视设备可以包括无线电台，以实现将患者相关数据双向传输到单独的远程站。

