



US007787938B2

(12) **United States Patent**
Pompei

(10) **Patent No.:** **US 7,787,938 B2**
(45) **Date of Patent:** ***Aug. 31, 2010**

(54) **TEMPORAL ARTERY TEMPERATURE DETECTOR**

(75) Inventor: **Francesco Pompei**, Boston, MA (US)

(73) Assignee: **Exergen Corporation**, Watertown, MA (US)

2,710,559 A	6/1955	Heitmuller et al.
3,273,395 A	9/1966	Schwarz
3,282,106 A	11/1966	Barnes
3,374,354 A	3/1968	Hood
3,392,282 A	7/1968	Astheimer
3,491,596 A	1/1970	Dean

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1 day.

(Continued)

This patent is subject to a terminal disclaimer.

FOREIGN PATENT DOCUMENTS

DE 19 14 468 B2 11/1970

(21) Appl. No.: **12/011,467**

(Continued)

(22) Filed: **Jan. 25, 2008**

OTHER PUBLICATIONS

(65) **Prior Publication Data**

US 2008/0200830 A1 Aug. 21, 2008

"Surface Temperature Scanner STS-100-F/C & 101-C," Omega Medical Corporation, pamphlet, 2 pages, Circa 1987.

(Continued)

Related U.S. Application Data

(63) Continuation of application No. 10/684,818, filed on Oct. 14, 2003, now Pat. No. 7,346,386, which is a continuation of application No. 09/923,240, filed on Aug. 3, 2001, now abandoned, which is a continuation of application No. 09/151,482, filed on Sep. 11, 1998, now Pat. No. 6,292,685.

Primary Examiner—Long V Le

Assistant Examiner—Jacqueline Cheng

(74) *Attorney, Agent, or Firm*—Hamilton, Brook, Smith & Reynolds, P.C.

(57) **ABSTRACT**

(51) **Int. Cl.**

A61B 6/00 (2006.01)

A61B 5/00 (2006.01)

G01K 1/00 (2006.01)

G01K 13/12 (2006.01)

Body temperature measurements are obtained by scanning a thermal radiation sensor across the side of the forehead over the temporal artery. A peak temperature measurement is processed to compute an internal temperature of the body as a function of ambient temperature and the sensed surface temperature. The function includes a weighted difference of surface temperature and ambient temperature, the weighting being varied with target temperature through a minimum in the range of 96° F. and 100° F. The radiation sensor views the target surface through an emissivity compensating cup which is spaced from the skin by a circular lip of low thermal conductivity.

(52) **U.S. Cl.** **600/474; 600/549; 374/100**

(58) **Field of Classification Search** **600/474, 600/459; 374/100, 104, 121, 126, 129**


See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,658,390 A 11/1953 Machler

67 Claims, 4 Drawing Sheets

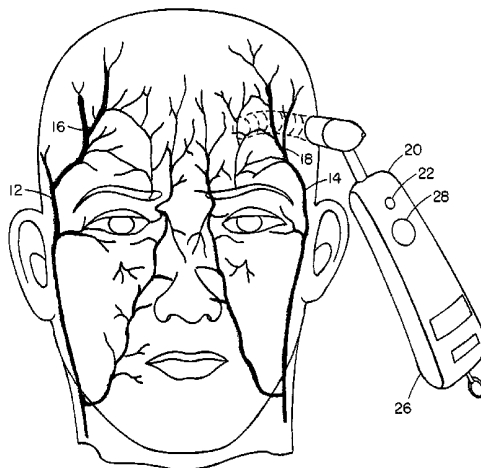

U.S. PATENT DOCUMENTS

3,526,135 A 9/1970 Wortz
 3,581,570 A 6/1971 Wortz
 3,614,892 A 10/1971 Offenstein
 3,719,838 A 3/1973 Peduto et al.
 3,777,568 A 12/1973 Risgin et al.
 3,781,837 A 12/1973 Anderson et al.
 3,933,045 A 1/1976 Fox et al.
 4,005,605 A 2/1977 Michael
 4,133,700 A 1/1979 Hollander et al.
 4,141,149 A 2/1979 George et al.
 4,198,861 A 4/1980 Mung-Kuen Luk
 4,204,120 A 5/1980 Riboulet et al.
 4,302,971 A 12/1981 Luk
 4,317,998 A 3/1982 Dore
 4,372,690 A 2/1983 Berman et al.
 4,420,265 A 12/1983 Everest et al.
 4,428,382 A 1/1984 Walsall et al.
 4,456,390 A 6/1984 Junkert et al.
 4,456,919 A 6/1984 Tomita
 4,494,881 A 1/1985 Everest
 4,566,808 A 1/1986 Pompei
 4,602,642 A 7/1986 O'Hara et al.
 4,623,266 A 11/1986 Kielb
 4,626,686 A 12/1986 Pompei et al.
 4,634,294 A 1/1987 Christol et al.
 4,636,091 A 1/1987 Pompei et al.
 4,691,713 A 9/1987 Suzuki
 4,722,612 A 2/1988 Junkert et al.
 4,726,688 A 2/1988 Ruel
 4,784,149 A 11/1988 Berman et al.
 4,790,324 A 12/1988 O'Hara et al.
 4,797,840 A 1/1989 Fraden
 4,831,258 A 5/1989 Paulk et al.
 4,843,577 A 6/1989 Muramoto
 4,846,583 A 7/1989 Yamamoto
 4,895,164 A 1/1990 Wood
 4,932,789 A 6/1990 Egawa et al.
 4,993,419 A 2/1991 Pompei et al.
 5,012,813 A 5/1991 Pompei et al.
 5,017,018 A 5/1991 Iuchi et al.
 5,017,019 A 5/1991 Pompei
 5,018,872 A 5/1991 Suszynski et al.
 5,024,533 A 6/1991 Egawa et al.
 5,050,612 A 9/1991 Matsumura
 5,056,929 A 10/1991 Watanae et al.
 5,150,969 A 9/1992 Goldberg et al.
 5,159,936 A 11/1992 Yelderman et al.
 5,167,235 A * 12/1992 Seacord et al. 600/474
 5,178,464 A 1/1993 Fraden
 5,187,943 A 2/1993 Taniguchi et al.
 5,199,436 A 4/1993 Pompei et al.
 5,229,612 A 7/1993 Pompei et al.
 5,232,284 A 8/1993 Egawa et al.
 5,271,407 A 12/1993 Pompei et al.
 RE34,507 E 1/1994 Egawa et al.
 5,325,863 A 7/1994 Pompei
 5,333,784 A 8/1994 Pompei
 5,368,038 A 11/1994 Fraden
 5,381,796 A 1/1995 Pompei
 5,441,476 A 8/1995 Kitado et al.
 5,445,158 A 8/1995 Pompei
 5,469,855 A 11/1995 Pompei et al.
 5,626,139 A 5/1997 Szeles et al.
 5,626,147 A 5/1997 Lackey
 RE35,554 E 7/1997 Pompei et al.
 5,653,238 A 8/1997 Pompei
 5,695,283 A 12/1997 Johnson
 5,725,308 A * 3/1998 Smith et al. 374/169
 5,743,644 A 4/1998 Kobayashi et al.
 5,818,044 A 10/1998 Sodickson et al.
 5,872,362 A 2/1999 Pompei

5,874,736 A 2/1999 Pompei
 5,893,833 A 4/1999 Pompei et al.
 5,924,996 A 7/1999 Cho et al.
 5,924,998 A 7/1999 Cornelius et al.
 6,001,066 A * 12/1999 Canfield et al. 600/559
 6,030,342 A 2/2000 Amano et al.
 6,047,205 A 4/2000 Pompei
 6,056,435 A 5/2000 Pompei
 6,059,452 A 5/2000 Smith et al.
 6,287,262 B1 9/2001 Amano et al.
 6,292,685 B1 9/2001 Pompei
 6,299,347 B1 10/2001 Pompei
 6,499,877 B2 12/2002 Pompei
 7,346,386 B2 3/2008 Pompei

FOREIGN PATENT DOCUMENTS

EP 0 411 121 A1 6/1991
 EP 0 446 788 A1 9/1991
 EP 0 845 241 A1 6/1998
 GB 1 226 540 3/1971
 JP 55037917 3/1980
 JP 02-045719 2/1990
 JP 2035322 A 2/1990
 JP 06-117882 A 4/1994
 JP 06-341906 12/1994
 JP 7140008 A 6/1995
 JP 8254467 A 10/1995
 JP 08-275924 A 10/1996
 JP 11-155826 6/1999
 WO WO 81/00764 3/1981
 WO WO 86/06163 10/1986
 WO WO 93/03666 3/1993
 WO WO 97/47239 12/1997
 WO WO 98/01730 1/1998
 WO WO 98/08431 5/1998
 WO WO 99/39166 8/1999

OTHER PUBLICATIONS

"Sensor Touch Temporal Artery Thermometer—The Noninvasive Thermometer You Can Trust," 5 page brochure, Exergen Corporation, 1999.
 Wei, D., et al., "Optimal Design of a Thermistor Probe for Surface Measurement of Cerebral Blood Flow," Transactions on Biomedical Engineering, 37(12):1159-1172, 1990.
 Database WPI, Section PQ, Week 9505, Derwent Publications Ltd., London, GB, May 15, 1994, Abstract.
 Omega Medical Surface Temperature Scanner STS-100-F/C & 101-C, 2 pages.
 Det Tronics, Optical Calibration, Oct. 1987.
 Model 1M Thermopile Detector, Dexter Research Center, Technical Description, Oct. 1980.
 Fraden, Jacob, "Application of Piezo/Pyroelectric Films in Medical Transducers," *J. Clinical Engineering*, 13(3):133-138 (1988).
 Houdas, Y. And Ring, E.F.J., "Human Body Temperature, Its Measurement and Regulation," Plenum Press, N.Y., pp. 83, 1982.
 Looney, Jr., Joseph M. and Pompei, Francisco, "Ear Thermometry," *Medical Electronics*, Jun. 1989.
 Surface Temperature Scanner, Models: STS100-F/C, STS-101-C, User Manual, 9 pages.
 Proceedings of the Eighth Annual Conference of the IEEE/Engineering in Medicine and Biology Society, vol. 3 of 3, Nov. 7-10, 1986.
 Ryan, Marybeth, "The Equine Infrared Thermographic Scanner: Assuring Performance of the Equine Athlete," Exergen Corporation, 4 pages, 1989.
 Pompei, Marybeth, "Temperature Assessment via the Temporal Artery: Validation of a New Method," Exergen Corporation, 1999.
 Sketch of Radiation Detector Manufactured by IR-ONICS Corporation and distributed by Dermatherm Corporation, pre 1983.
 Kuzucu, Etham Y., "Measurement of Temperature," *Int. Anesthesiol Clin.* 3(3):435-449 (1965).
 PET™, Physician's Electronic Thermometer, Phillips Bio-Medical, Inc., Specifications, 2 pgs.

- FirstTemp Intelligent Medical Systems, Model 2000A, Operation Manual, 8 pages.
- ComforTemp All-Family Instant Underarm Thermometer, Quick Start Instructions, 6 pages.
- FirstTemp Clinical Thermometer, Technical Manual, 24 pages.
- Notification of Reason(s) for Rejection mailed May 7, 2009 for JP Application No. 2000-570539.
- Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States Court of Appeal for the Federal Circuit, 2006-1491, 2007-1180.
- Notification of Reason(s) for Rejection mailed: Aug. 25, 2009 for JP Application No. 2000-570539 (with English Translation attached).
- Communication Pursuant to Article 96(2) EPC mailed: Jan. 15, 2003 for European Application No. 99 945 647.8.
- Communication Pursuant to Article 115(2) EPC mailed: Sep. 24, 2003 for European Application No. 99 945 647.8.
- Communication Pursuant to Article 96(2) EPC mailed: Jan. 24, 2006 for European Application No. 99 945 647.8.
- Communication Pursuant to Article 94(3) EPC mailed: Apr. 16, 2008 for European Application No. 99 945 647.8.
- Communication Pursuant to Article 94(3) EPC mailed: Mar. 25, 2009 for European Application No. 99 945 647.8.
- Pompei & Pompei, *Physicians Reference Handbook on Temperature: Vital Sign Assessment with Infrared Thermometry*, Exergen Corporation, Boston, MA (entire book enclosed).
- Marybeth Pompei, Letter dated Jun. 13, 1997 to Jeffrey Blummer, MD.
- Marybeth Pompei, Letter dated Jun. 15, 1997 to Jeffrey Blummer, MD.
- Marybeth Pompei, Letter dated Jul. 20, 1997 to Jeffrey Blummer, MD.
- Marybeth Pompei, Letter dated Aug. 10, 1997 to William Walsh, MD.
- Francesco Pompei, *Non-Invasive Arterial Thermometry: from Physics and Physiology to Physicians and Nurses*, Sep. 16, 1997.
- "Tecnimed SRL's Preliminary Invalidity Disclosures," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 1:08-CV-11416-DPW, May 6, 2009.
- "Exergen's Responses to Tecnimed's Preliminary Invalidity Contentions," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 08-CV-11416-DPW, Jun. 8, 2009.
- "Tecnimed's Preliminary Identification of Claim Terms and Proposed Construction," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 1:08-CV-11416-DPW, Aug. 14, 2009.
- "Plaintiff Exergen Corporation's Supplemental Proposed Claim Constructions," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 08-CV-11416-DPW, Jan. 26, 2010.
- "Tecnimed's Updated Identification of Claim Terms and Proposed Constructions," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 1:08-CV-11416-DPW, Feb. 19, 2010.
- "Deposition of Francesco Pompei," (Redacted), including Exhibits 3, 4 and 6, *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 1:08-CV-11416-DPW, Aug. 27, 2009.
- "Expert Witness Report of Jack Goldberg," *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jan. 17, 2003.
- "Disclosure of Expert Rebuttal Testimony of Dr. Francesco Pompei," *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Mar. 3, 2009.
- "Supplemental Expert Witness Report of Jack Goldberg," *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jan. 21, 2005.
- "Second Supplemental Expert Witness Report of Jack Goldberg," *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jan. 21, 2005.
- Transcript of Jury Trial Day 5, *Exergen Corporation v. S.A.A.T. Systems Application of Advanced Technology Ltd., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jun. 17, 2005.
- Transcript of Jury Trial Day 13, *Exergen Corporation v. S.A.A.T. Systems Application of Advanced Technology Ltd., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jul. 5, 2005.
- Transcript of Jury Trial Day 14, *Exergen Corporation v. S.A.A.T. Systems Application of Advanced Technology Ltd., et al.*, United States District Court for District of Massachusetts, Case No. 01-CV-11306-RCL, Jul. 6, 2005.
- Benzinger, T.H., "Heat Regulation: Homeostasis of Central Temperature in Man," *Physiological Reviews*, 49(4): 671-759 (Oct. 1969).
- Castle, S.C., et al., "The Equivalency of Infrared Tympanic Membrane Thermometry with Standard Thermometry in Nursing Home Residents," Abstract, Erratum and Comment in *J. Am. Geriatr. Soc.* 41(7): 781-782 (Jul. 1993).
- Houdas, Y. and E.F.J. Ring, "Human Body Temperature It's Measurement and Regulation," *Plenum Press*, p. 83 (date not available).
- Looney, J.M., Jr., and F. Pompei, "Ear Thermometry," *Medical Electronics*, EXE037469-EXE037474 (Jun. 1989).
- Benzinger, M., "Tympanic Thermometry in Surgery and Anesthesia," *JAMA*, 209(8): 1207-1211 (Aug. 1969).
- Nadel, E.R. and S.M. Horvath, "Comparison of Tympanic Membrane and Deep Body Temperature in Man," *Life Sciences*, 9(1): 869-875 (Jun. 1970).
- "Memorandum and Order on Defendants' Motion for Partial Summary Judgment and on Plaintiff's Motion for Summary Judgment on S.A.A.T.'s Counterclaims," *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, United States District Court of Massachusetts, Case No. 01-CV-10436-RCL, Jul. 14, 2004.
- Pompei, F. and M. Pompei, "Arterial Thermometry Via Heat Balance at the Ear," *Medical Electronics*, (Oct. 1996).
- Benzinger, T.H., "Tympanic Clinical Temperature," *Biology and Medicine*, 192: 2089-2102 (date not available).
- "Deposition of Francesco Pompei, Ph.D.," *Exergen v. Wal-Mart*, Dec. 7, 2002 (Filed Under Seal).
- "Deposition of Francesco Pompei, Ph.D.," *Exergen v. Wal-Mart*, Dec. 8, 2002 (Filed Under Seal).
- Defendant's Trial Brief, *Exergen v. Wal-Mart*, Jun. 8, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).
- Judgment in a Civil Case, *Exergen v. CVS Corporation, et al.*, Aug. 4, 2005, Civil Action No. 01-11306-RCL and 02-10436-RCL.
- Verdict Form, *Exergen v. S.A.A.T. Systems Application of Advanced Technology LTD. Daiwa Products, Inc., and CVS Corporation*, Jul. 11, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).
- Transcript of Jury Trial Day 15, *Exergen v. S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and CVS Corporation*, Jul. 7, 2005, Civil Action No. 01-11306-RCL.
- Memorandum in Support of Defendants' Motion for Judgment as a Matter of Law that Defendants' Motion for Judgment as a Matter of Law that Defendants do not Infringe the '813, '205, and '685 Patents as to the Safety 1st Device, the CVS Device, and the Thermotek Device, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 6, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).
- Memorandum in Support of Defendants' Motion for Judgment as a Matter of Law that Defendant SAAT does not Infringe the '813, '205, and '685 Patents, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 6, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).
- Memorandum in Support of Defendants' Motion for Judgment as a Matter of Law that Claims 1-5 of the '205 Patent are Invalid as Anticipated by the O'Hara Patent, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa*

Products, Inc., and Hana Microelectronics Co, Ltd., Jul. 6, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Motion for Judgment as a Matter of Law that Defendants do not Infringe the '813, '205 and '685 Patents as to the Safety 1st Device, the CVS Device, and the Thermotek Device, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jun. 30, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Motion for Judgment as a Matter of Law that Defendant SAAT does not Infringe the '813, '205, and '685 Patents, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jun. 30, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Motion for Judgment as a Matter of Law that Claims 1-5 of the '205 Patent are Invalid as Anticipated by the O'Hara Patent, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jun. 30, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Opposition to Plaintiff's Motion for Judgment as a Matter of Law that Defendants Infringe all Asserted Claims and are Liable for Lost Profits, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 21, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Opposition to Plaintiff's Motion for Judgment as a Matter of Law that Defendants have Failed to Prove that any Patent Claim is Invalid, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 21, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Memorandum in Support of Exergen's Motion for Judgment as a Matter of Law that Defendants have Failed to Prove that any Patent Claim is Invalid, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 7, 2005, Civil Action No. 01-CV-11306-RCL, Civil Action No. 02-CV-10436-RCL.

Exergen's Motion for Judgment as a Matter of Law that Defendants Infringe the Patents-in-Suit and that Defendants are Liable for Exergen's Lost Profits, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 7, 2005, Civil Action No. 01-CV-11306-RCL, Civil Action No. 02-CV-10436-RCL.

Exergen's Motion for Judgment as a Matter of Law that Defendants have Failed to Prove that any Patent Claim is Invalid, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jul. 7, 2005, Civil Action No. 01-CV-11306-RCL, Civil Action No. 02-CV-10436-RCL.

Defendant's Motion *in Limine* (No. 5) to Exclude any Evidence or Argument Relying Upon an Incorrect Construction of the Claim Term "Internal Temperature", *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, May 31, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Plaintiff Exergen's Opposition to Defendants' Motions in Limine Nos. 3, 4, 5, 6 and 7, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Jun. 10, 2005, Civil Action No. 01-CV-11306-RCL and Civil Action No. 02-CV-10436-RCL.

Memorandum in Support of Defendants' Renewed Motion for Judgment as a Matter of Law that Claims 1-5 of the '205 Patent are Invalid as Anticipated by the O'Hara Patent, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Memorandum in Support of Defendants' Renewed Motion for Judgment as a Matter of Law that Defendant SAAT did not Infringe the '813, '205, and '685 Patents, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Memorandum of Points and Authorities in Support of Defendants' Renewed Motion for Judgment as a Matter of Law that Defendants do not Infringe the '813, '205, and '685 Patents as to the Safety 1st Device, the CVS Device, and the Thermotek Device, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Renewed Motion for Judgment as a Matter of Law that Defendants do not Infringe the '813, '205, and '685 Patents as to the Safety 1st Device, the CVS Device, and the Thermotek Device and Request for Oral Argument, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Renewed Motion for Judgment as a Matter of Law that Defendant SAAT did not Infringe the '813, '205, and '685 Patents and Request for Oral Argument, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Defendants' Renewed Motion for Judgment as a Matter of Law that Claims 1-5 of the '205 Patent are Invalid as Anticipated by the O'Hara Patent and Request for Oral Argument, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Aug. 18, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Reply Brief in Support of Defendants' Motions for Judgment as a Matter of Law, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Sep. 16, 2005, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Exergen's Opposition to Defendants' Motions for Judgment as a Matter of Law, *Exergen v. CVS Corporation, S.A.A.T. Systems Application of Advanced Technology Ltd., and Daiwa Products, Inc.*, Sep. 6, 2005, Civil Action No. 01-CV-11306-RCL and Civil Action No. 02-CV-10436-RCL.

Defendants' Motion for Partial Summary Judgment of Noninfringement and Request for Oral Argument, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Apr. 15, 2003, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Memorandum of Points and Authorities in Support of Defendants' Motion for Partial Summary Judgment of Noninfringement, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, Apr. 15, 2003, Civil Action No. 01-CV-11306-RCL (consolidated with Civil Action No. 02-CV-10436-RCL).

Exergen's Opposition to Motion for Partial Summary Judgment of Non-Infringement, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, May 14, 2003, Civil Action No. 01-CV-11306-RCL, Civil Action No. 02-CV-10436-RCL.

Memorandum and Order on Defendants' Motion for Partial Summary Judgment and on Plaintiff's Motion for Summary Judgment on S.A.A.T.'s Counterclaims, *Exergen v. Wal-Mart Stores Inc., S.A.A.T. Systems Application of Advanced Technology Ltd., Daiwa Products, Inc., and Hana Microelectronics Co, Ltd.*, *Exergen v. CVS Corporation*, Jul. 14, 2004, Case No. 01 CV 11306-RCL, Case No. 02-CV-10436-RCL.

Brief of Defendants-Appellants S.A.A.T. Systems Application of Advanced Technology, Ltd. and Daiwa Products, Inc., *Exergen v. Wal-Mart Stores Inc., et al.*, Dec. 5, 2008, Case No. 011-CV-11306RCL.

Brief of Plaintiff- Exergen Corporation, *Exergen v. Wal-Mart Stores Inc., et al.*, Jan. 30, 2009, Case No. 011-CV-11306RCL.

Response and Reply Brief of Defendants-Appellants S.A.A.T. Systems Application of Advanced Technology, Ltd. and Daiwa Products, Inc., *Exergen v. Wal-Mart Stores Inc., et al.*, Mar. 16, 2009, Case No. 011-CV-11306RCL.

Reply Brief for Plaintiff-Cross Appellant Exergen Corporation, *Exergen v. Wal-Mart Stores Inc., et al.*, Apr. 1, 2009, Case No. 011-CV-11306RCL.

Decision of U.S. Court of Appeals for the Federal Circuit, *Exergen v. Wal-Mart Stores Inc., et al.*, Aug. 4, 2009, Case No. 011-CV-11306RCL.

"Exhibit 3: Claim Terms and Proposed Construction," *Exergen Corporation v. Kidz-Med, Inc., et al.*, Case No. 1:08-CV-11416-DPW United States District Court for District of Massachusetts, Feb. 11, 2010.

T.K. Bergersen, "A Search for Arteriovenous Anastomoses in Human Skin Using Ultrasound Doppler," *Acta Physiol Scand*, 147: 195-201 (Feb. 1993).

Tecnimcd SRL's Supplemental Preliminary Invalidity Disclosures, *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for the District of Massachusetts, Civil Action No. 1:08-cv-11416-DPW, Filed May 21, 2010.

"Exhibit A- Tecnimcd SRL's Supplemental Invalidity Disclosures," *Exergen Corporation v. Kidz-Med, Inc., et al.*, United States District Court for the District of Massachusetts, Civil Action No. 1:08-cv-11416-DPW, Filed May 21, 2010.

Newburgh, L.H., M.D., et al., "Physiology of Heat Regulation and The Science of Clothing," *Div. of Med. Sciences, Nat'l Research Council*, Preface, Chapters 2 and 3 of Part 1 (Oct. 1949).

Expert Witness Report of Jack Goldberg, *Exergen Corporation v. Wal-Mart Stores, Inc., et al.*, Civil Action No. 01-CV-11306-RCL (Jan. 17, 2003).

Symposium, "Temperature: Its Measurement and Control In Science an Industry," *American Institute of Physics, National Bureau of Standards and National Research Council*, pp. 446-452 and 537-543 (Nov. 1941).

Nadel, Ethan R., et al., "Comparison of Tympanic Membrane and Deep Body Temperature in Man," *Institute of Environmental Stress*, University of California -Santa Barbara (Jun. 1970).

* cited by examiner

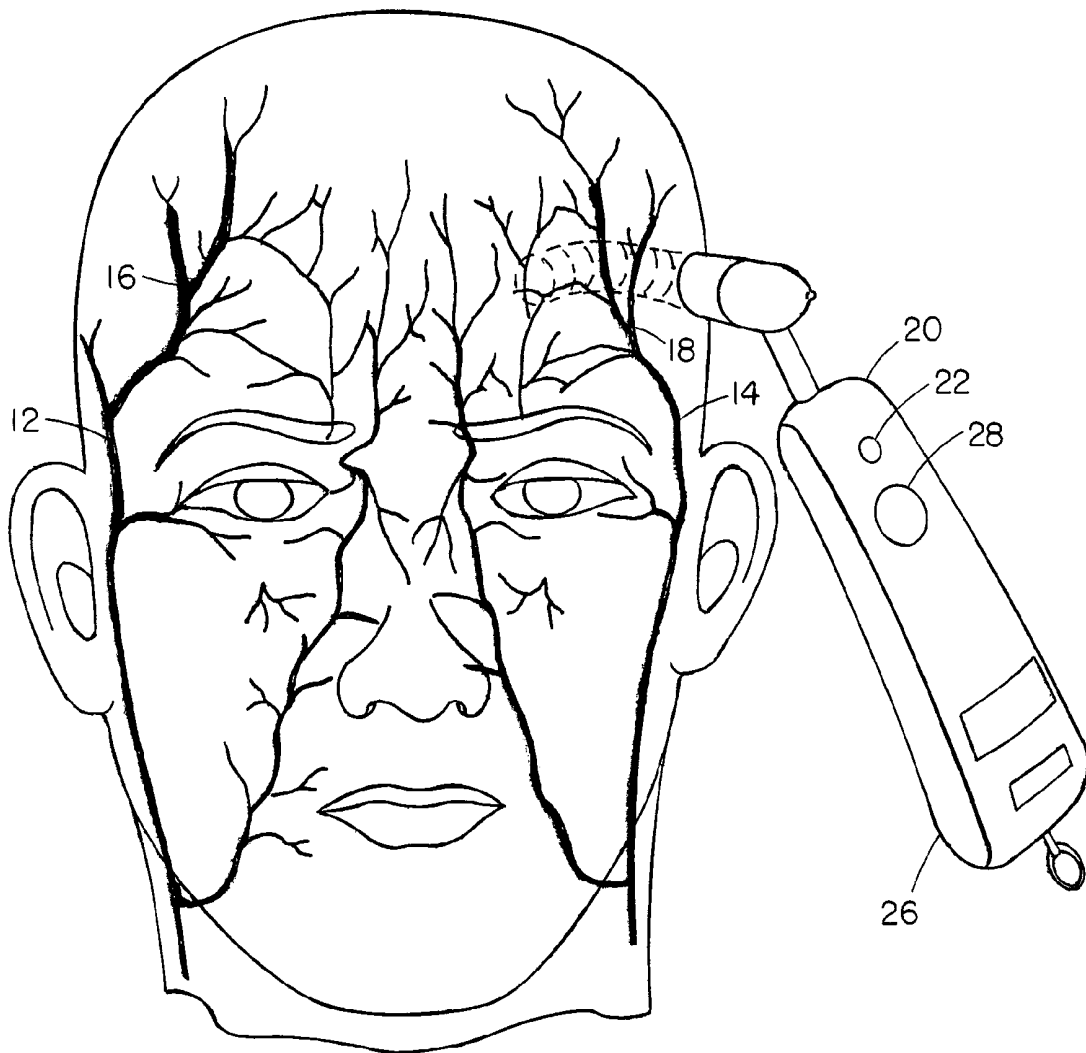


FIG. 1

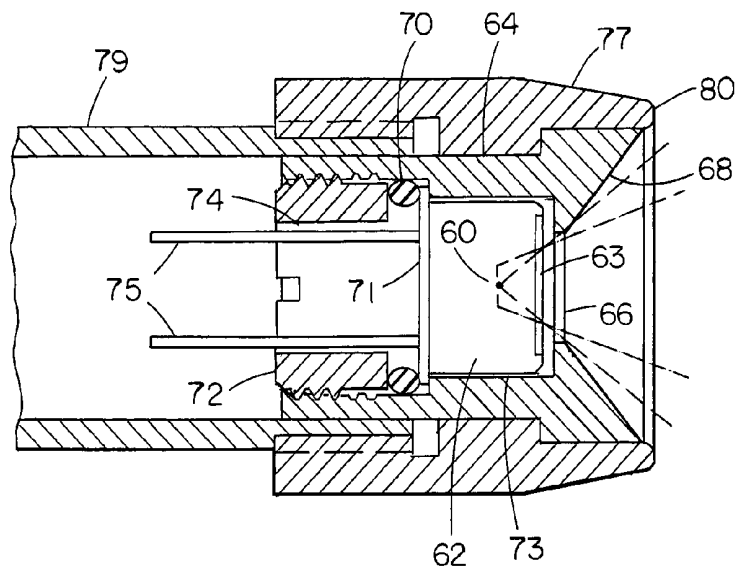


FIG. 2A

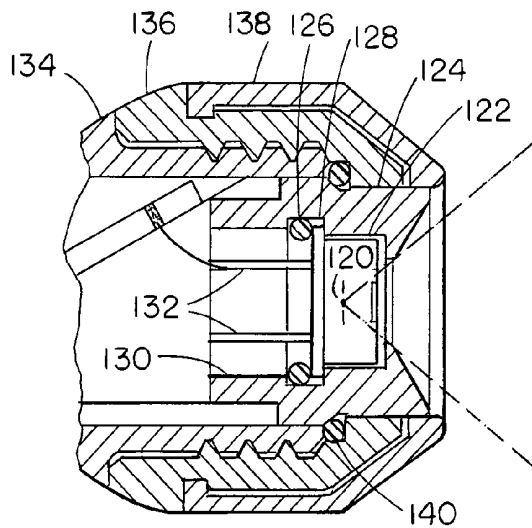


FIG. 2B

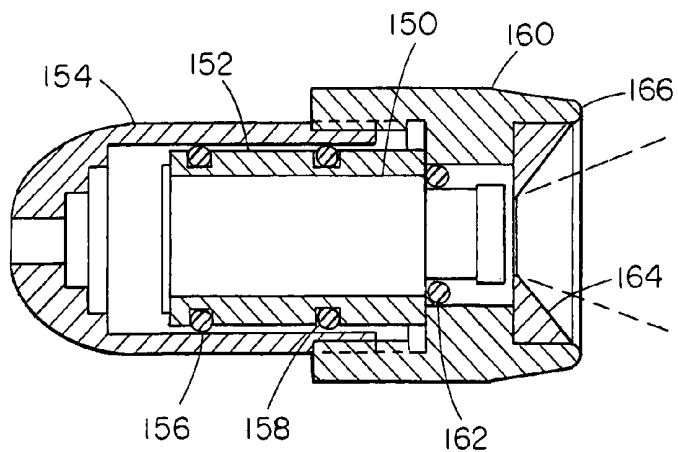


FIG. 2C

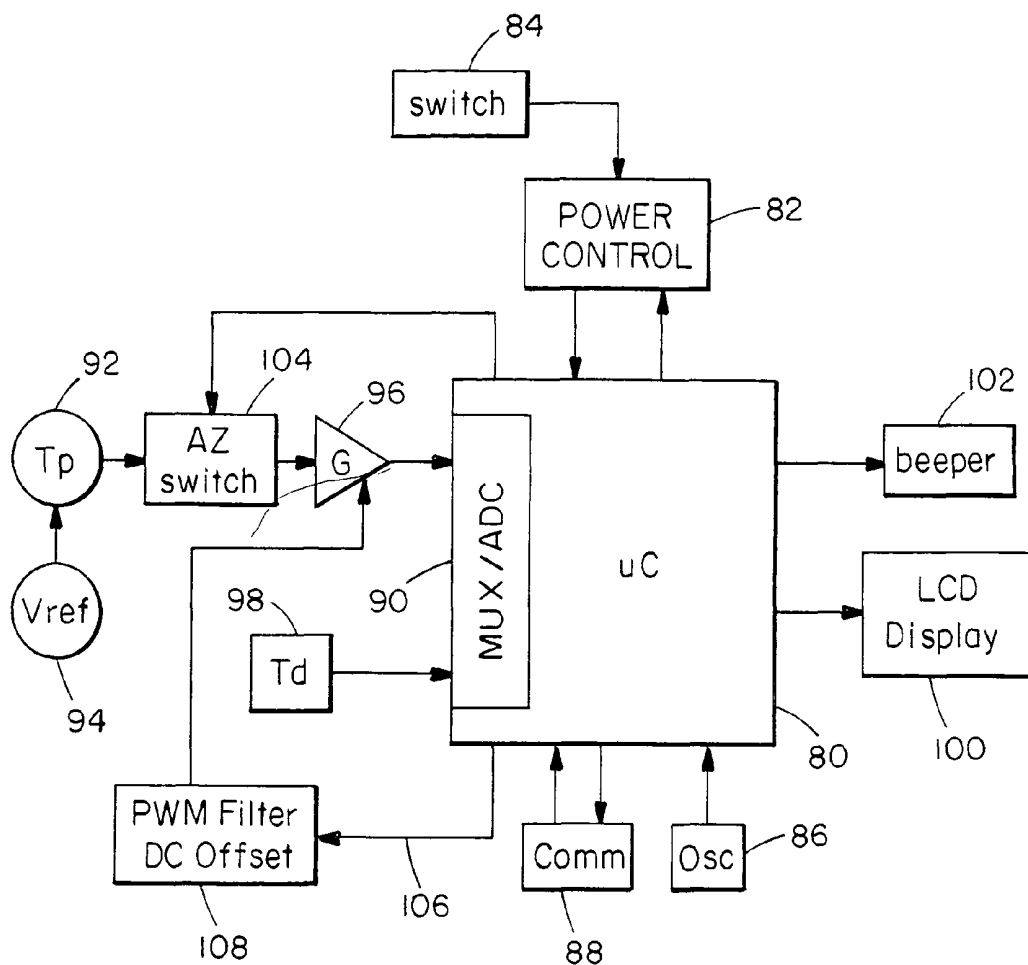


FIG. 3

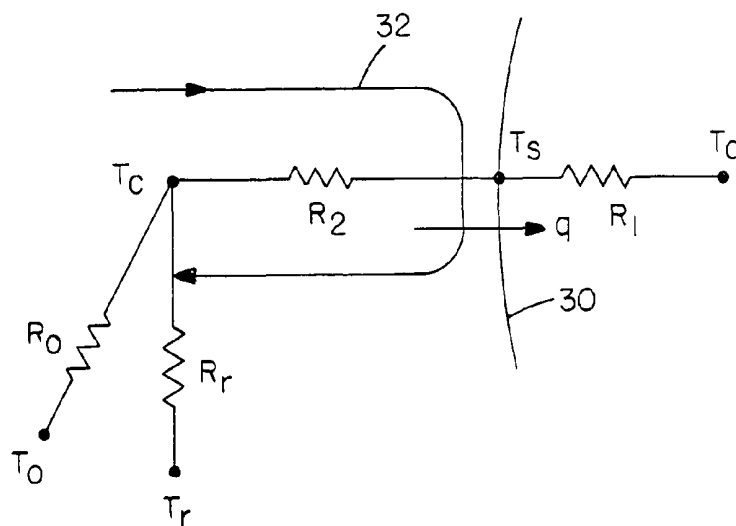


FIG. 4

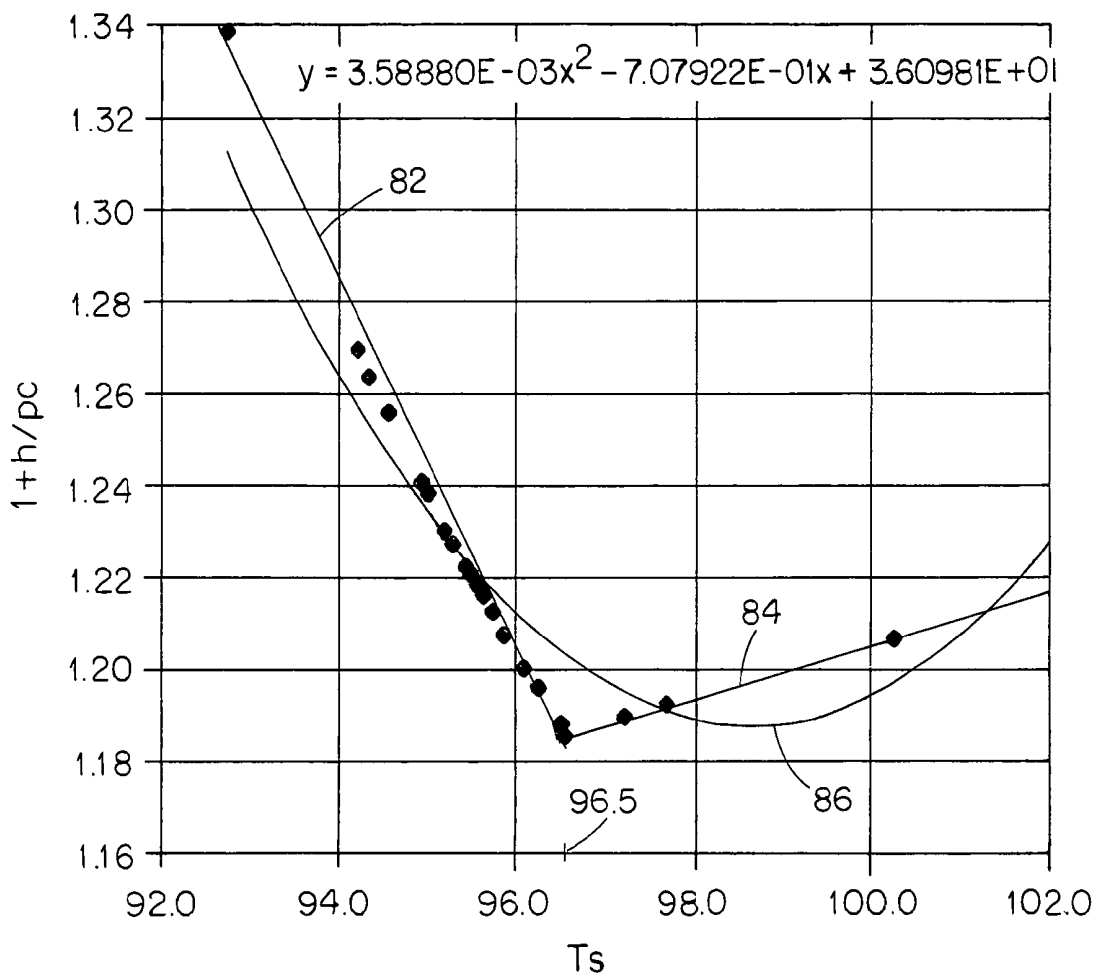


FIG. 5

TEMPORAL ARTERY TEMPERATURE DETECTOR

RELATED APPLICATIONS

This application is a continuation of application Ser. No. 10/684,818, filed Oct. 14, 2003, now U.S. Pat. No. 7,346,386, which is a continuation of application Ser. No. 09/923,240, filed Aug. 3, 2001, now abandoned which is a continuation of application Ser. No. 09/151,482, filed Sep. 11, 1998, now U.S. Pat. No. 6,292,685. The entire teachings of the above applications are incorporated herein by reference.

BACKGROUND OF THE INVENTION

In recent years, infrared thermometers have come into wide use for detection of temperature of adults. For core temperature readings, infrared thermometers which are adapted to be inserted into the patient's ear have been very successful. Early infrared thermometers were adapted to extend into the ear canal in order to view the tympanic membrane and provide an uncorrected, direct reading of tympanic temperature which correlates with pulmonary artery temperature. More recently, however, to provide for greater comfort and ease of use, ear thermometers have been designed to provide corrected readings of the generally cooler distal ear canal. Such thermometers measure temperature of distal ear canal tissue and calculate arterial core temperature via heat balance.

Core temperature is a term used to describe deep body temperature and is approximated by oral, rectal, ear, pulmonary artery, esophageal and bladder temperatures and the like. Of those temperatures, pulmonary artery temperature is the most precise definition of core temperature since it is closest to the heart and its blood is supplied to all tissues. Calculations of arterial core temperature via heat balance provide approximations of the pulmonary artery temperature, and unless otherwise indicated, core temperature refers to the pulmonary artery temperature.

The arterial heat balance approach is based on a model of heat flow through series thermal resistances from the arterial core temperature to the ear skin temperature and from the ear skin temperature to ambient temperature. Accordingly, after sensing both the skin temperature and ambient temperature, the arterial core temperature can be calculated. The thermal resistance model also allows for computation of equivalent oral and rectal temperatures with the mere adjustment of a weighting factor in the computation. Infrared ear thermometers using the arterial heat balance are disclosed in U.S. Pat. Nos. 4,993,419; 5,012,813; 5,199,436; 5,381,796; 5,445,158; 5,653,238 and 5,271,407, the entire teachings of which are incorporated herein by reference.

To avoid clinical difficulties in using ear thermometers, particularly with neonates, axillary (underarm) infrared thermometers have been introduced. Infrared thermometers designed for axillary temperature measurements are presented in U.S. patent application Ser. Nos. 08/469,484, 08/738,300 and 08/881,891, the entire teachings of which are incorporated herein by reference. In each of those devices, an infrared detector probe extends from a temperature display housing and may easily slide into the axilla to lightly touch the apex of the axilla and provide an accurate infrared temperature reading in as little as one-half second. The axillary thermometer also relies on the arterial heat balance approach to provide arterial, oral or rectal temperature.

The axillary infrared thermometer has found great utility not only with neonates but as a screening tool in general, and

especially for small children where conventional temperature measurements such as a thermometer under the tongue or a rectal thermometer are difficult.

In ear and neonate axillary thermometry, the difference between skin temperature and ambient temperature has been weighted by a coefficient approximating h/pc , where h is an empirically determined coefficient which includes a radiation view factor between the skin tissue and ambient, p is perfusion rate and c is blood specific heat. In ear and neonate axillary thermometry, that coefficient was found empirically to be about 0.09 and 0.05, respectively, with only minor variations. However, with greater exposure for heat transfer and higher vasomotor functions, that coefficient has been determined empirically for the adult axillary region to be about 0.13 with much more significant variations according to the patient's temperature.

SUMMARY OF THE INVENTION

The present invention provides for particularly convenient temperature readings of neonate, child and adult temperatures by detecting the temperature of the forehead directly over the superficial temporal artery.

Because arteries receive blood directly from the heart, they are a good choice for detecting core temperature, but an artery at the extremities of the body, such as those felt as pulse points at the wrist or ankle, are highly subject to vasoconstriction. This means, for example, that when an individual is extremely sick, in shock, or even just cold or nervous, the arteries constrict to reduce the flow of blood to that area as a means of retaining heat, or as in the case of shock, in an effort to redirect the blood to more critical areas of the body. This can result in a large temperature change at the artery which is a local artifact only and not representative of core temperature.

Ruling out those arteries located in the extremities, in attempting to replicate the temperature at the source (the heart), we find, in the temporal artery, an artery as short a distance from the heart as possible, with a high and relatively constant blood flow, and that is readily accessible on all individuals. The heart, the lungs and the brain are vital to our very existence, so the supply of blood is high to these organs and continues as high as possible even through, in the face of grave illness, other areas may shut down to accommodate.

Originating in the heart is the aorta, the main trunk of the arterial system. A direct extension of the aorta is the common carotid artery, a robust artery which runs upward in the neck and divides into the internal and external carotids. But, the carotids, even the external carotid, are at best partially embedded, and at worst completely embedded in the skull, and therefore are not accessible at the skin. Extending directly from the carotid is the temporal artery, again an artery dividing internally and externally. We look to the external branch which travels in front of the ear and up into the soft temple area, terminating in a fork directly between the skin and the skull adjoining the eyebrow.

Demonstrably, the temporal artery is very easily accessible; in fact in most individuals, it is usually quite visible. Terminating in a two-prong fork, it easily doubles the assurance of measuring the correct area. Touching it does not present a risk of injury. There are no mucous membranes present, thus eliminating the risk of contaminates such as those found in the mouth and rectum. And, despite lying so close to the skin surface, the temporal artery perfusion, which is the flow of blood per unit volume of tissue, remains relatively constant and so ensures the stability of blood flow required for our measurement.

In accordance with one aspect of the invention, a temperature sensor is scanned across the forehead, preferably in the vicinity of the temporal artery, and a peak temperature reading is provided from the scan. At least three readings per second should be made during the scan, preferably about ten readings per second. The method can be extended to other arteries near the skin such as in the axilla. The preferred radiation sensor is a radiation sensor which views a target surface of the forehead through a reflective cup. The cup has a large open diameter close to the target surface and a window at the base of the cup through which the radiation sensor views the target, the cup being out of the field of view of the sensor. The reflective cup is spaced from the target surface by a smooth lip of low thermal conductivity material.

As in prior ear and axillary thermometers, internal core temperature can be computed from the function

$$T_c = (1 + (h/pc))(T_s - T_a) + T_a \quad (1)$$

where T_s and T_a are the skin and ambient temperatures. The function can be seen to include a weighted difference of surface temperature and ambient temperature with a weighting coefficient h/pc .

In accordance with another aspect of the invention, electronics in the detector compute an internal temperature of the body as a function of ambient temperature and sensed surface temperature. The function includes a weighted difference of surface temperature and ambient temperature, the weighting being varied with target temperature. The weighting varies with target temperature through a minimum in the range of 96° F. to 100° F., the weighting increasing above and below the minimum. In particular, the weighting is an approximation of h/pc at the forehead artery where h is a heat transfer coefficient between the target surface and ambient, p is perfusion rate and c is blood specific heat. In a preferred embodiment, the weighting is a linear approximation having a minimum between 96° F. and 97° F. The approximation of h/pc at the minimum is about 0.19. In another embodiment, the weighting includes a polynomial approximation of $1 + h/pc = k_1 T_s^2 - k_2 T_s + k_3$ where h is a heat transfer coefficient between the target surface and ambient, p is perfusion rate, c is blood specific heat T_s is skin temperature, k_1 is approximately 0.00359, k_2 is approximately 0.708 and k_3 is approximately 36.1.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other objects, features and advantages of the invention will be apparent from the following more particular description of preferred embodiments of the invention, as illustrated in the accompanying drawings in which like reference characters refer to the same parts throughout the different views. The drawings are not necessarily to scale, emphasis instead being placed upon illustrating the principles of the invention.

FIG. 1 illustrates an infrared thermometer scanning the temporal artery in the forehead in accordance with the present invention.

FIGS. 2A, B and C are cross-sectional views of three embodiments of the radiation sensor assembly of the invention.

FIG. 3 is an electrical block diagram of the electronics of the thermometer of FIG. 1.

FIG. 4 illustrates the arterial heat balance model.

FIG. 5 illustrates the change in weighting coefficient $(1 + h/pc)$ with change in skin temperature.

DETAILED DESCRIPTION OF THE INVENTION

A description of preferred embodiments of the invention follows.

As illustrated in FIG. 1, the temporal arteries **12** and **14** extend upwardly toward the side of the human face and bifurcate at **16** and **18** in the forehead region. In that region, the temporal artery passes over the skull bone very close to the skin and is thus termed the superficial temporal artery. The superficial temporal artery is, therefore, particularly accessible for providing temperature readings and, as an artery, has a temperature close to the heart temperature. Further, there are no known arterial/venous anastomoses, that is, shunts between the artery and veins for regulation of skin temperature. Accordingly, the blood flow is relatively stable, varying a maximum of only 50% as opposed to as much as 500% in other areas of the skin.

To locate the temporal artery, a temperature detector, preferably a radiation detector **20**, is scanned across the side of the forehead over the temporal artery while electronics in the detector search for the peak reading which indicates the temporal artery. Preferably, that temperature reading is then further processed in accordance with an algorithm specific to the temporal artery for providing a display temperature which may, for example, correspond to core, oral or rectal temperature.

The temperature detector **20** provides an audible beep with each peak reading. A display **26** provides the temperature reading resulting from the electronic processing discussed below, updated to each new peak reading. A button **28** enables the user to activate the temperature detector. In one embodiment, an LED **22** which flashes with each peak reading can be observed when someone other than the patient performs the reading, and another LED on the other side of the housing can be observed by the patient, particularly when taking his own temperature.

FIG. 2A illustrates one sensor assembly for the radiation detector of FIG. 1. The assembly is similar to that presented in application Ser. No. 08/881,891. A thermopile radiation sensor **60** is mounted within a can **62** in conventional fashion. For high stability the thermopile may be a vapor deposited thermopile surrounded with xenon gas, but for reduced cost it may be a semiconductor thermopile surrounded with air. An infrared radiation transparent window **63** is provided over a viewing opening in the can. The can **62** is set within a bore within a heat sink **64**. A shoulder defines an aperture **66** at the base of a conical emissivity compensating cup **68** through which the thermopile views the target. The cup is preferably of low emissivity in order to provide emissivity compensation as disclosed in U.S. Pat. No. 4,636,091. Preferably, the heat sink **64** in which the cup is formed is of aluminum. Alternatively, the heat sink may be of brass, nickel plated in the cup region.

An elastomeric o-ring **70** is positioned behind the can **62**. A plug **72** is threaded into the bore in the heat sink **64** to press the ring **70** against the rear flange **71** of the can and thus press the flange against a shoulder in the heat sink bore. With the flange pressed against the shoulder and having a close tolerance with the larger diameter of the bore, an air gap **73** is maintained about the side and front of the can. This arrangement provides for good thermal contact between the can and the heat sink **64** at the rear and also makes the thermopile highly resistant to mechanical shock since the shock is only transferred through the thin flange past the shock absorbing elastomer. If the flange were rigidly clamped between metal parts, there would be a danger of shock breaking the gas seal of the can. An opening **74** is provided through the center of the plug **72** for

access of electrical leads **75** to the thermopile can. The heat sink **64** is press fit in a plastic cap **77** which is threaded on to the tubular head **79** of the detector.

The plastic cap **77** in which the sensor assembly is mounted is of low thermal conductivity, preferably less than one hundredth that of aluminum. The housing thermally isolates the heat sink **64** from the surrounding environment to minimize heat flow to the heat sink. Further, the heat sink **64** is of significant thermal mass. Accordingly, the RC time constant for change in temperature of the radiation sensor, with change in temperature to which the housing is exposed, can be made large for a more stable temperature reading. The thermal resistance is made high by the low conductivity housing, and the thermal capacitance is made high by the large mass of the heat sink **64**. That RC time constant should be at least 5 minutes and is preferably about 25 minutes.

Past designs of infrared thermometers, such as presented in U.S. Pat. No. 4,993,419, have relied on a massive thermopile can which also served as the heat sink. That design assured a high RC time constant for thermal conduction through the external thermal barrier to the heat sink relative to a thermal RC time constant for temperature response of the cold junction to heat transferred to the heat sink. The latter low RC time constant was obtained by assuring a low thermal resistance to the cold junction using expensive high conductivity material in a specially designed can/heat sink. In the present device, a design goal is to use a conventional low cost thermopile mounted in a light weight can which does not provide the low thermal resistance of the prior design. Accordingly, it is important that the can be mounted to assure that all heat conduction to the thermopile be through the rear of the can which serves as the thermal ground to the thermopile. That objective is obtained by making thermal contact to the can through the rear flange and assuring an air space about the sides and front of the can.

Forming the emissivity compensating cup **68** in the heat sink reduces the cost of the assembly and also improves the thermal characteristics. Although the emissivity of the cup is ideally zero, it is in fact about 0.1. With the cup formed as part of the heat sink, it is at the temperature to which the can is grounded. Accordingly, any thermal emissions from the surface of cup **68** will be at substantially the same temperature as the cold junction and thus not be seen. The electronics can also be calibrated to compensate for the loss of reflectance due to non-ideal emissivity, but that calibration is affected by the temperature of the reflective surface. By assuring that the surface of cup **68** is at the temperature to which the thermopile can is grounded, the temperature of the surface is generally known and compensation can be made temperature dependent.

When adapted to household use, concerns for patient cross-contamination associated with clinical temperature detectors is not so significant. Further, at the forehead, evaporation of moisture is not as significant as in the ear and axillary applications. Accordingly, the disposable radiation transparent covers used in prior infrared thermometers, such as in Ser. No. 08/469,484 and Ser. No. 08/738,300 is less desirable. However, in the clinical environment, the transparent cover is still preferred to prevent cross contamination.

During the scanning of the radiation detector across the forehead, contact of the housing **78** with the skin can cause cooling of the skin. To minimize that cooling, a circular lip **80** protrudes axially beyond the tip of the heat sink **64**. The lip has a thin radius of 0.02 to 0.05 inch, preferably about 0.03 inch, to minimize the thermal conductance through the insulation material. The heat sink **64** is recessed 0.02 to 0.05 inch,

preferably about 0.03 inch, behind the tip of the lip. For comfort during scanning, the lip has a smooth curve.

Another embodiment of the radiation sensor assembly is presented in FIG. 2B. As in the prior embodiment, the thermopile **120** is positioned within a can **122**. The can is retained in a heat sink **124** by an o-ring **126** which presses against the flange **128** of the can and is set within a circumferential groove in the bore **130** of the heat sink. As before, wires **132** extend through that bore. The housing **134** of the detector head is a split tube formed of two parts which meet along longitudinal seams. The two tube parts are held together by a nut **136** to which a plastic cap **138** is snap fit. The heat sink is retained in the assembly by an o-ring **140** which is seated within a groove in the heat sink and a groove in the nut **136**. As before, the cap **138** has a curved lip which extends beyond the tip of the heat sink **124**. Cap **138** is of soft material for the comfort of the patient.

In the embodiment of FIG. 2C, the thermopile is positioned within a can **150** of high thermal mass similar to that disclosed in U.S. Pat. No. 5,012,813. The can is set within a sleeve **152** which is retained in the head housing **154** by o-rings **156** and **158**. A plastic cap **160** is threaded onto the head **154**, and the can **150** is centered within the cap by an additional o-ring **162**. A low emissivity cup **164** is press fit within the cap **160** and, as before, is recessed behind a smooth lip **166**.

An electrical block diagram for the radiation detector is presented in FIG. 3. A microprocessor **80** is at the heart of the circuit. A power control circuit **82** responds to activation of the button switch **84** by the user to apply power to the microprocessor and other elements of the circuit. That power is maintained until the microprocessor completes the measurement cycle and signals the power control **82** to power down. The microprocessor is clocked by an oscillator circuit **86** and may communicate with an external source for programming and calibration through communication conductors **88**. The temperature determined by the microprocessor is displayed on the liquid crystal display **100**, and detection of peaks during the temperature processing is indicated by a beeper **102**. Peaks are detected from readings taken at least three times per second, and preferably about ten times per second, for rapid scan across the forehead to avoid cooling of the forehead through the detector. During the measurement process, the microprocessor takes readings through a multiplexer/analog-to-digital converter **90**. The preferred microprocessor **80** is a PIC16C74 which includes an internal 8-bit A-D converter. To minimize expense, the circuit is designed to rely solely on that A-D converter.

Thermopile **92** provides a voltage output signal equal to the fourth power difference between target temperature and the temperature of the thermopile cold junction, offset by voltage reference **94**. The voltage output from the thermopile is amplified by an amplifier **96**, having a gain in the order of 1000, which also provides an offset determined by a pulse width modulated filter **108** controlled by the microprocessor. Through operation of the multiplexer, the microprocessor provides an analog-to-digital conversion of the amplified sensor output and of the detector temperature T_d provided by temperature sensor **98**. The temperature sensor **98** is positioned to sense the substantially uniform temperature of the thermopile cold junction, can and heat sink. An auto zero switch **104** is included to allow for isolation of the amplifier **96** from the thermopile **92** during a calibration sequence as discussed in prior U.S. application Ser. No. 08/738,300.

It is well known that the output of the thermopile is proportional to $(T_s^4 - T_d^4)$ where T_s is the target skin temperature viewed by the radiation detector and T_d is the temperature of the detector measured by sensor **98**. From that relationship,

T_s can be computed. It is also known that, based on the determined skin temperature and the ambient temperature to which the skin is exposed, an internal core temperature can be computed using the arterial heat balance approach illustrated in FIG. 4. Heat flux q from the internal core temperature T_c passes through the skin **30** to the ambient environment at temperature T_a . The skin is thus held at some intermediate temperature T_s .

The heat loss of skin, such as at the forehead, the external ear canal or axilla, to the environment can be calculated with the following well-known equation:

$$q = hA(T_s - T_a) \tag{2}$$

where q is heat flow, A is surface area, T_s and T_a the skin and ambient temperatures, respectively, and h is an empirically determined coefficient which includes a radiation view factor between the skin tissue and ambient. The equation takes the linear form for simplicity. Although the exact form of the equation is fourth-power due to the radiation exchange, the linearized form provides excellent accuracy over the range of interest of about 900 to 105° F.

Heat flow from the core arterial source to the skin is via blood circulation **32**, which is many times more effective than tissue conduction. Thermal transport via the circulation can be described with the following equation:

$$q = wc(T_c - T_s) \tag{3}$$

where q again is heat flow, w is blood mass flow rate, c is blood specific heat, and T_c and T_s are core and skin temperatures, respectively.

Accordingly, the skin can be viewed thermally as tissue being warmed by its blood supply as governed by equation 3, balanced by radiating heat to ambient as governed by equation 2.

Equating:

$$hA(T_s - T_a) = wc(T_c - T_s) \tag{4}$$

Simplifying by dividing by surface area A :

$$h(T_s - T_a) = pc(T_c - T_s) \tag{5}$$

where p is blood flow per unit area, also termed perfusion rate.

Equation 5 then provides a method to calculate core temperature T_c when skin temperature T_s and ambient temperature T_a are known, and the coefficients (or their ratio) have been empirically determined.

Solving for T_c :

$$T_c = (h/pc)(T_s - T_a) + T_s \tag{6}$$

where h/pc , the weighting coefficient which weights the difference of surface temperature and ambient temperature, is empirically determined on a statistical basis over a range of patients and clinical situations.

An alternative method of calculating is to employ an electrical analog technique, since equations 2 and 3 have the identical form of a simple voltage/current relationship. The method employs the convention that electrical current is analogous to heat flow and voltage differential is analogous to temperature differential.

Accordingly, equations 2 and 3 may be written as:

$$q = (1/R_1)(T_s - T_a) \tag{7}$$

$$q = (1/R_2)(T_c - T_s) \tag{8}$$

and the electrical circuit can be drawn, with resistances R_1 and R_2 and with T_c and T_a as constant temperature (voltage)

reservoirs (FIG. 4). A third equation with a more convenient form can be written as:

$$q = (1/(R_1 + R_2))(T_c - T_a) \tag{9}$$

Using equations 7 and 9 and solving for T_c :

$$T_c = ((R_1 + R_2)/R_1)(T_s - T_a) + T_a \tag{10}$$

and finally:

$$T_c = k(T_s - T_a) + T_a \tag{11}$$

which is the precise form of the heat balance equation programmed into arterial heat balance instruments, with $(R_1 + R_2)/R_1$ expressed as the k -Factor.

The k Factor can be rewritten as follows:

$$k = \frac{R_1 + R_2}{R_1} = 1 + \frac{R_2}{R_1} = 1 + (h/pc) \tag{12}$$

Accordingly, in either form, equation 6 or 11, it can be seen that the weighting coefficient h/pc is applied to the difference of surface and ambient temperature.

In the ear temperature and neonatal axillary temperature measurements, the perfusion rate is also generally constant, resulting in h/pc of about 0.09 for adult ears and 0.05 for neonates. For a normal adult, the perfusion rate of the axilla is such that the weighting coefficient h/pc is about 0.13. Further, the perfusion rate varies according to the condition of the patient. In particular, with a fever, the perfusion rate can become much higher. Similarly, in the forehead, perfusion rate varies with skin temperature.

In both the ear and axilla, the coefficient h is relatively constant. The forehead has greater exposure to the ambient environment, and the radiation heat loss increases with increased skin temperature. Thus, where the weighting coefficient h/pc decreased for all increasing skin temperatures in the ear and axilla temperature measurements, it has been found that, as illustrated in FIG. 5, the weighting coefficient reaches a minimum at near normal body temperature and then, due to the increasing value of h , increases. Empirical data suggests that the value h/pc decreases linearly 82 to a value of about 0.19 and a temperature of about 96-97° F. The coefficient then increases linearly with skin temperature but at a lesser slope at **84**. The linear approximations illustrated in FIG. 5 are used in the computations in the clinical model. However, in the consumer model, those linear approximations are replaced by a single polynomial approximation **86**:

$$1 + h/pc = .0035888 T_s^2 - .707922 T_s + 36.0981$$

Since all body site temperatures of interest arise from the arterial temperature source, the arterial heat balance can be applied to any site. Accordingly, based on the Thevenin equivalents theorem, oral and rectal diagnostic equivalents T_o and T_r , of arterial temperature can be calculated by appropriate selection of k -Factor, empirically taking into consideration resistances R_o and R_r .

Individual aspects of the radiation detector which make it particularly suited to providing temperature readings from the temporal artery and other arteries can be found in applicant's prior designs. However, none of those designs provide the unique combination of elements which enable consistent

measurements of core temperature by scanning across a superficial artery. Specifically, the Exergen D501 Industrial Temperature Detector used in emissivity compensating cup and provided a peak temperature based on about ten temperature readings per second. However, that device did not perform a heat balance computation and was thus not suited to measurement of core temperature. The emissivity compensating cup was utilized in the axillary temperature detector with a heat balance computation, but that unit was not adapted to be scanned across the target surface. The detected peak in that device used to indicate when the reading had stabilized and could be relied upon. That peak detection was based on only one reading per second. Applicant's prior ear temperature detectors have obtained a peak temperature from ten readings per second but with pivoting of the detector rather than with lateral scan across the target surface. There was no emissivity compensating cup.

While this invention has been particularly shown and described with references to preferred embodiments thereof, it will be understood by those skilled in the art that various changes in form and details may be made therein without departing from the spirit and scope of the invention as defined by the appended claims.

The invention claimed is:

1. A method of detecting human body temperature comprising moving a radiation detector to scan across skin over an artery and measure radiation as target skin surface over the artery is viewed, and electronically determining a body temperature approximation, distinct from skin surface temperature, from the radiation detector as the target skin surface over the artery is viewed.

2. The method of claim 1 wherein the body temperature approximation corresponds to an oral measurement.

3. The method of claim 1 wherein the body temperature approximation corresponds to a rectal measurement.

4. The method of claim 1 further comprising determining the body temperature approximation based on an ambient temperature to which the human body is exposed.

5. The method of claim 1 further comprising evaluating a plurality of radiation readings to determine the body temperature approximation.

6. The method of claim 1 further comprising displaying the body temperature approximation.

7. The method of claim 1 further comprising sounding an audible signal upon completion of the measurement.

8. The method of claim 1 further comprising measuring radiation emitted in at least three readings per second.

9. The method of claim 8 further comprising providing a peak temperature reading.

10. The method of claim 1 wherein the artery has relatively constant blood flow.

11. The method of claim 1 wherein the body temperature approximation is based on heat flow from the body to ambient.

12. The method of claim 1 wherein the artery is a temporal artery.

13. The method of claim 1 wherein the artery is a forehead artery.

14. A method of detecting human body temperature comprising making at least three radiation readings per second while moving a radiation detector to scan across a region of skin over an artery to electronically determine a body temperature approximation, distinct from skin surface temperature.

15. The method of claim 14 wherein the body temperature approximation corresponds to an oral measurement.

16. The method of claim 14 wherein the body temperature approximation corresponds to a rectal measurement.

17. The method of claim 14 further comprising determining the body temperature approximation based on ambient temperature to which the human body is exposed.

18. The method of claim 14 further comprising evaluating a plurality of radiation readings to determine the body temperature approximation.

19. The method of claim 14 further comprising displaying the body temperature approximation.

20. The method of claim 14 further comprising sounding an audible signal upon completion of the measurement.

21. The method of claim 14 further comprising determining the body temperature approximation from a peak temperature reading.

22. The method of claim 14 wherein the artery has relatively constant blood flow.

23. The method of claim 14 wherein the body temperature approximation is based on heat flow from the body to ambient.

24. The method of claim 14 wherein the artery is a temporal artery.

25. The method of claim 14 wherein the artery is a forehead artery.

26. A method of detecting human body temperature comprising, with a radiation detector, measuring radiation as target skin surface over an artery is viewed, the artery having a relatively constant blood flow, and electronically determining a body temperature approximation, distinct from skin surface temperature, from the radiation detector as the target skin surface over the artery is viewed.

27. The method of claim 26 wherein the body temperature approximation corresponds to an oral measurement.

28. The method of claim 26 wherein the body temperature approximation corresponds to a rectal measurement.

29. The method of claim 26 further comprising determining the body temperature approximation based on ambient temperature to which the human body is exposed.

30. The method of claim 26 further comprising evaluating a plurality of radiation readings to determine the body temperature approximation.

31. The method of claim 26 further comprising displaying the body temperature approximation.

32. The method of claim 26 further comprising sounding an audible signal upon completion of the measurement.

33. The method of claim 26 further comprising moving the radiation detector to scan the region of the skin over the artery.

34. The method of claim 33 further comprising measuring radiation emitted in at least three readings per second.

35. The method of claim 34 further comprising providing a peak temperature reading.

36. The method of claim 26 wherein the body temperature approximation is determined based on heat flow from the body to ambient.

37. The method of claim 26 wherein the artery is a temporal artery.

38. The method of claim 26 wherein the artery is a forehead artery.

39. A body temperature detector comprising:
a radiation detector;
electronics that measure radiation from at least three readings per second of the radiation detector as target skin surface over an artery is viewed and that process the detected radiation to provide a body temperature approximation based on heat flow from an internal body temperature to ambient.

11

40. The body temperature detector claimed in claim 39 wherein the body temperature corresponds to an oral measurement.

41. The body temperature detector as claimed in claim 39 wherein the body temperature corresponds to a rectal measurement.

42. The body temperature detector claimed in claim 39 wherein the electronics determine body temperature based on ambient temperature to which the body is exposed.

43. The body temperature detector as claimed in claim 39 further comprising a display of the body temperature approximation.

44. The body temperature detector as claimed in claim 39 further comprising an audible signal that sounds upon completion of a measurement.

45. The body temperature detector as claimed in claim 39 wherein the electronics provide the body temperature approximation from a peak reading.

46. The body temperature detector of claim 39 wherein the artery is a temporal artery.

47. The body temperature detector claimed in claim 39 wherein the artery is a forehead artery.

48. A body temperature detector comprising:

a radiation detector; and

electronics that measure radiation from at least three readings per second of the radiation detector as a target skin surface over an artery is viewed, the artery having a relatively constant blood flow, and that process the measured radiation to provide a body temperature approximation, distinct from skin surface temperature, based on detected radiation.

49. The body temperature detector of claim 48 wherein the artery is a temporal artery.

50. The body temperature detector of claim 48 wherein the artery is a forehead artery.

51. A method of detecting human body temperature comprising:

measuring temperature of a region of skin of the forehead; and

processing the measured temperature to provide a body temperature approximation based on heat flow from an internal body temperature to ambient temperature.

52. The method of claim 51 wherein the region of the skin is over an artery.

53. The method of claim 51 wherein the region of the skin is over a temporal artery.

54. A method of detecting human body temperature comprising:

measuring radiation as target skin surface of the forehead is viewed, and

12

processing the measured radiation to provide a body temperature approximation based on heat flow from an internal body temperature to ambient temperature.

55. The method of claim 54 wherein the region of the skin is over an artery.

56. The method of claim 54 wherein the region of the skin is over a temporal artery.

57. A method of detecting human body temperature comprising:

moving a temperature detector to scan across skin of a region of a forehead; and

providing a body temperature approximation from a peak temperature reading from plural readings taken from plural locations during the scan.

58. A method as claimed in claim 57 wherein the temperature detector comprises a radiation sensor which views a target surface area of the forehead.

59. A method as claimed in claim 58 wherein the radiation sensor views the target surface area through a reflective cup, the cup having a large open diameter close to the target surface area and a window at the base of the cup through which the radiation sensor views the target surface area, the cup being out of the field of view of the sensor.

60. A method as claimed in claim 57 further comprising providing a body temperature approximation based on ambient temperature to which the human body is exposed and the peak temperature reading.

61. A method as claimed in claim 60 wherein the body temperature approximation corresponds to an oral temperature.

62. A method as claimed in claim 60 wherein the body temperature approximation corresponds to a rectal temperature.

63. A method as claimed in claim 60 wherein the function includes a weighted difference of surface temperature and ambient temperature, the weighting including an approximation of h/pc at a forehead artery where h is a heat transfer coefficient between a target surface of the forehead and ambient, p is perfusion rate and c is blood specific heat.

64. A method as claimed in claim 60 wherein the temperature detector comprises a radiation sensor which views a target surface area of the forehead.

65. A method as claimed in claim 57 wherein the scan is over an artery.

66. A method as claimed in claim 57 wherein the scan is over a temporal artery.

67. A method of claim 57 wherein the temperature detector makes at least three readings per second as it is moved.

* * * * *

专利名称(译)	颞动脉温度探测器		
公开(公告)号	US7787938	公开(公告)日	2010-08-31
申请号	US12/011467	申请日	2008-01-25
申请(专利权)人(译)	的Exergen CORPORATION		
当前申请(专利权)人(译)	的Exergen CORPORATION		
[标]发明人	POMPEI FRANCESCO		
发明人	POMPEI, FRANCESCO		
IPC分类号	A61B6/00 G01K1/00 A61B5/00 G01K13/12 G01J5/02 A61B5/01 G01J5/00 G01J5/04 G01J5/10 G01K13/00		
CPC分类号	A61B5/015 G01J5/0022 G01J5/0025 G01J5/02 G01J5/026 G01J5/04 G01J5/06 G01J5/16 A61B5/01 A61B5/742		
其他公开文献	US20080200830A1		
外部链接	Espacenet USPTO		

摘要(译)

通过在颞动脉上方的前额侧扫描热辐射传感器来获得体温测量值。处理峰值温度测量以计算作为环境温度和感测的表面温度的函数的身体的内部温度。该功能包括表面温度和环境温度的加权差，加权随目标温度变化，最小值在96°F和100°F之间。辐射传感器通过发射率补偿杯观察目标表面。通过低导热率的圆形唇缘与皮肤隔开。

