



US 20060200018A1

(19) **United States**

(12) **Patent Application Publication**  
**Al-Ali**

(10) **Pub. No.: US 2006/0200018 A1**

(43) **Pub. Date: Sep. 7, 2006**

(54) **RESPOSABLE PULSE OXIMETRY SENSOR**

**Publication Classification**

(76) Inventor: **Ammar Al-Ali**, Tustin, CA (US)

(51) **Int. Cl.**  
**A61B 5/00** (2006.01)

Correspondence Address:  
**KNOBBE MARTENS OLSON & BEAR LLP**  
**2040 MAIN STREET**  
**FOURTEENTH FLOOR**  
**IRVINE, CA 92614 (US)**

(52) **U.S. Cl.** ..... **600/344; 600/310**

(57) **ABSTRACT**


(21) Appl. No.: **11/415,600**

(22) Filed: **May 2, 2006**

A pulse oximeter sensor has both a reusable and a disposable portion. The reusable portion of the sensor preserves the relatively long-lived and costly emitter, detector and connector components. The disposable portion of the sensor is the relatively inexpensive adhesive tape component that is used to secure the sensor to a measurement site, typically a patient's finger or toe. The disposable portion of the sensor is removably attached to the reusable portion in a manner that allows the disposable portion to be readily replaced when the adhesive is expended or the tape becomes soiled or excessively worn. The disposable portion may also contain an information element useful for sensor identification or for security purposes to insure patient safety.

**Related U.S. Application Data**

(63) Continuation of application No. 10/741,777, filed on Dec. 19, 2003, now Pat. No. 7,039,449, which is a continuation of application No. 10/128,721, filed on Apr. 23, 2002, now Pat. No. 6,725,075, which is a continuation of application No. 09/456,666, filed on Dec. 9, 1999, now Pat. No. 6,377,829.

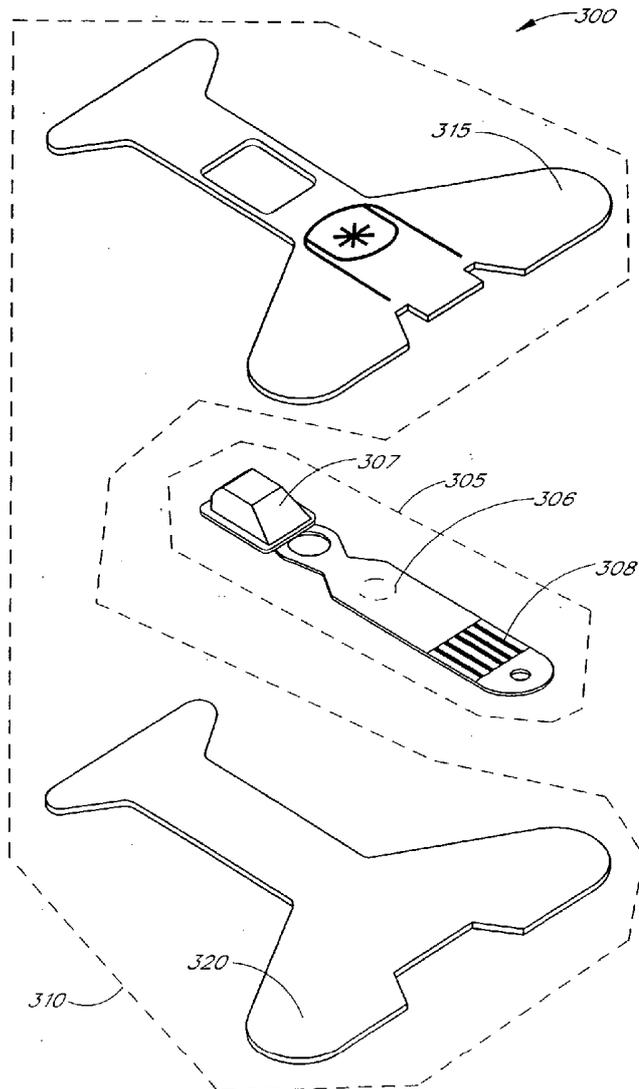

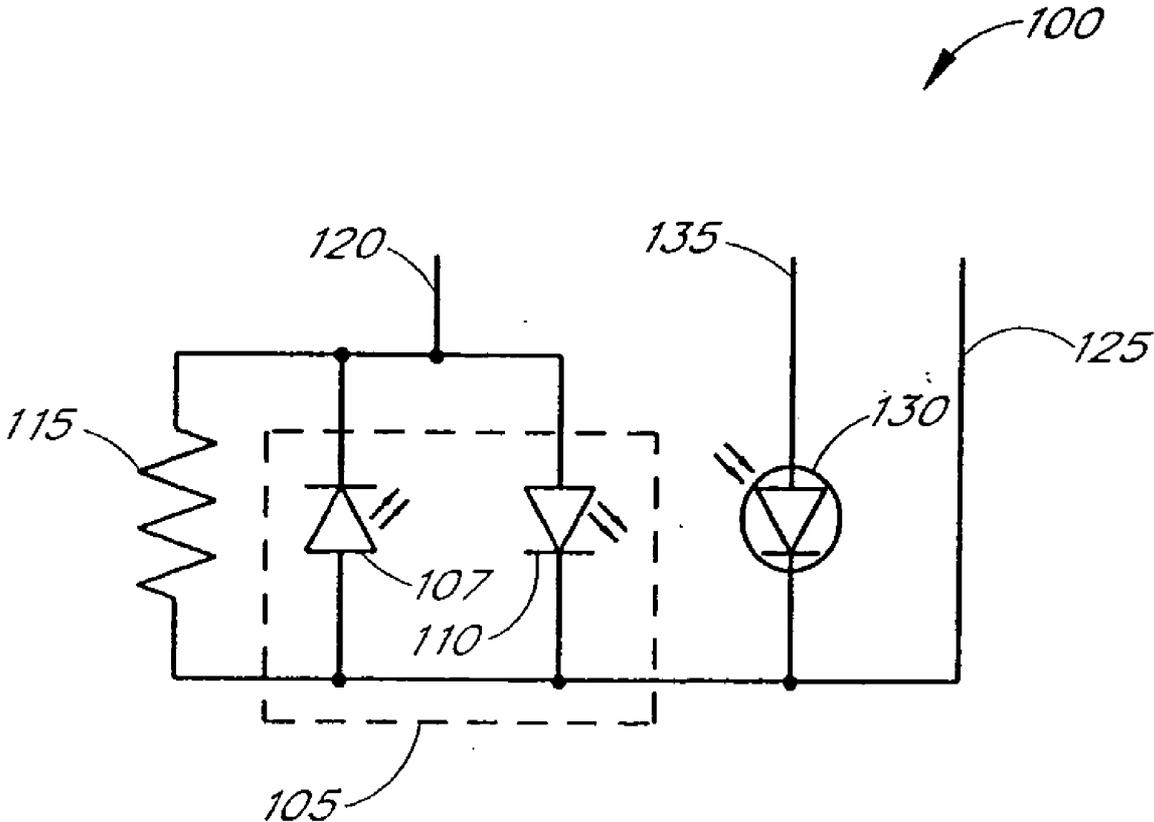
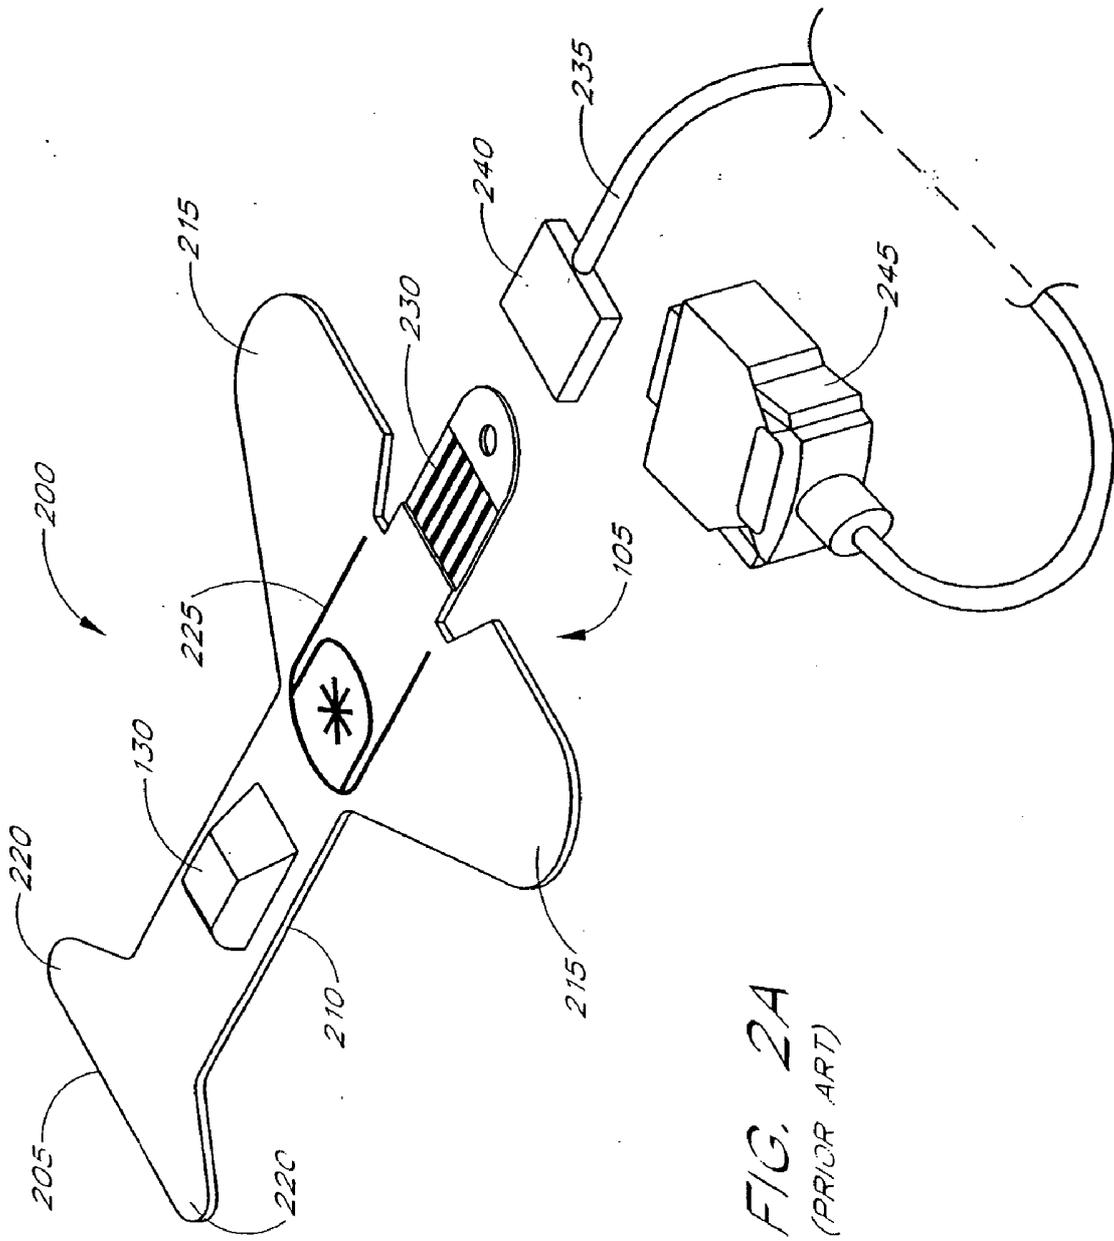


FIG. 1



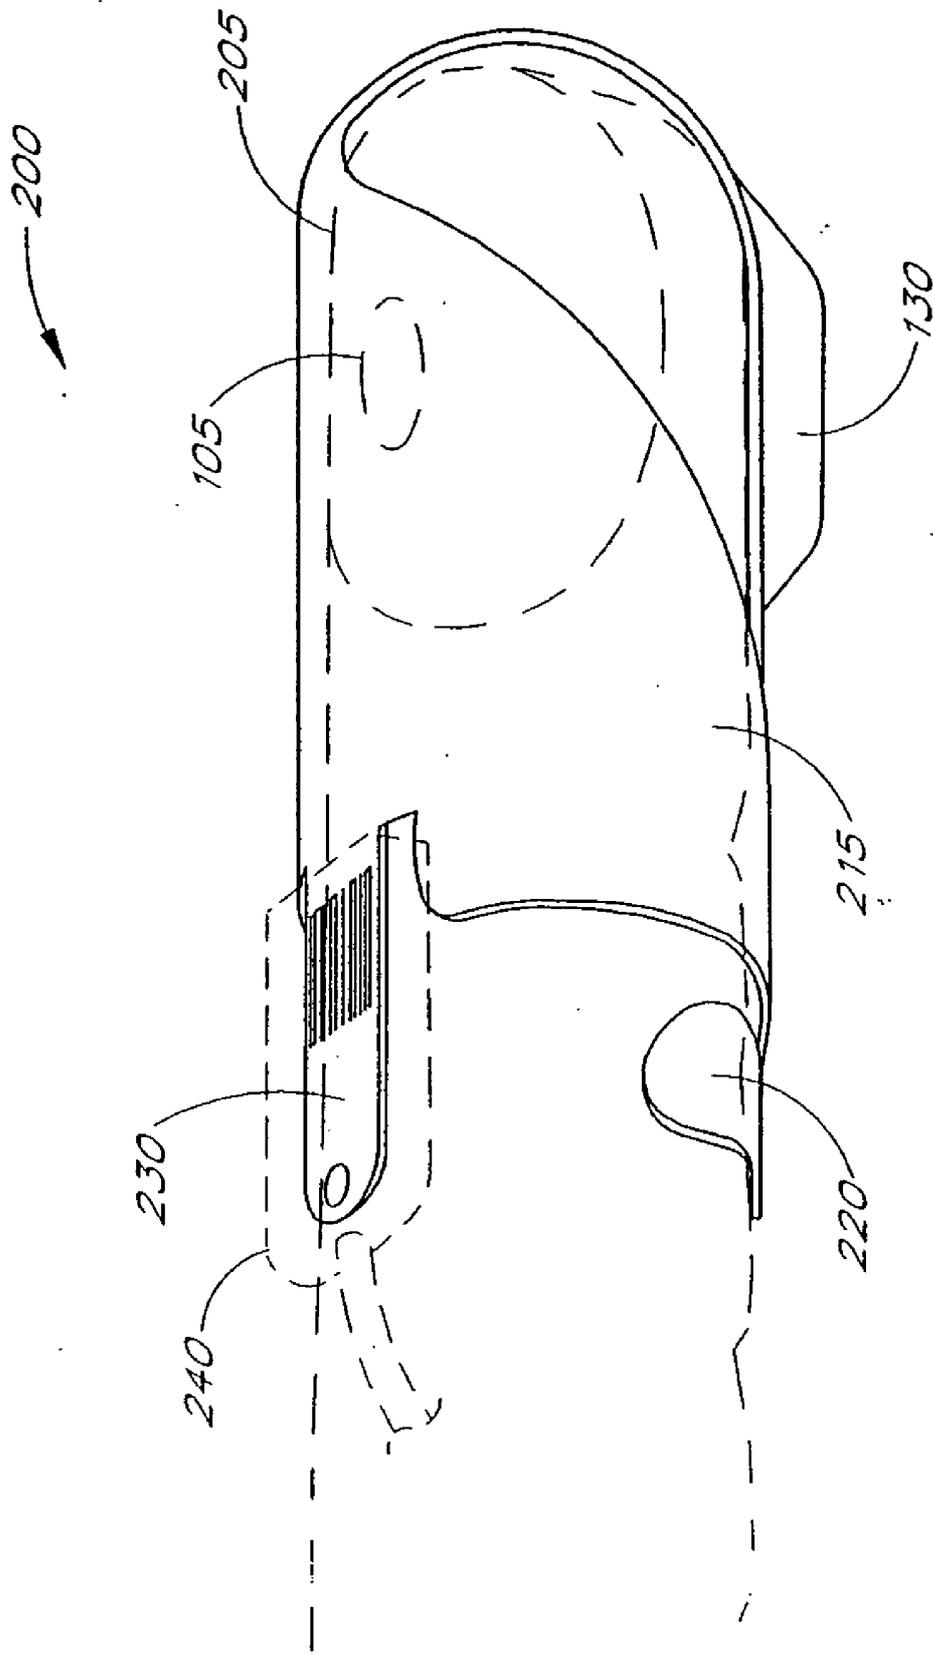


FIG. 2B  
(PRIOR ART)

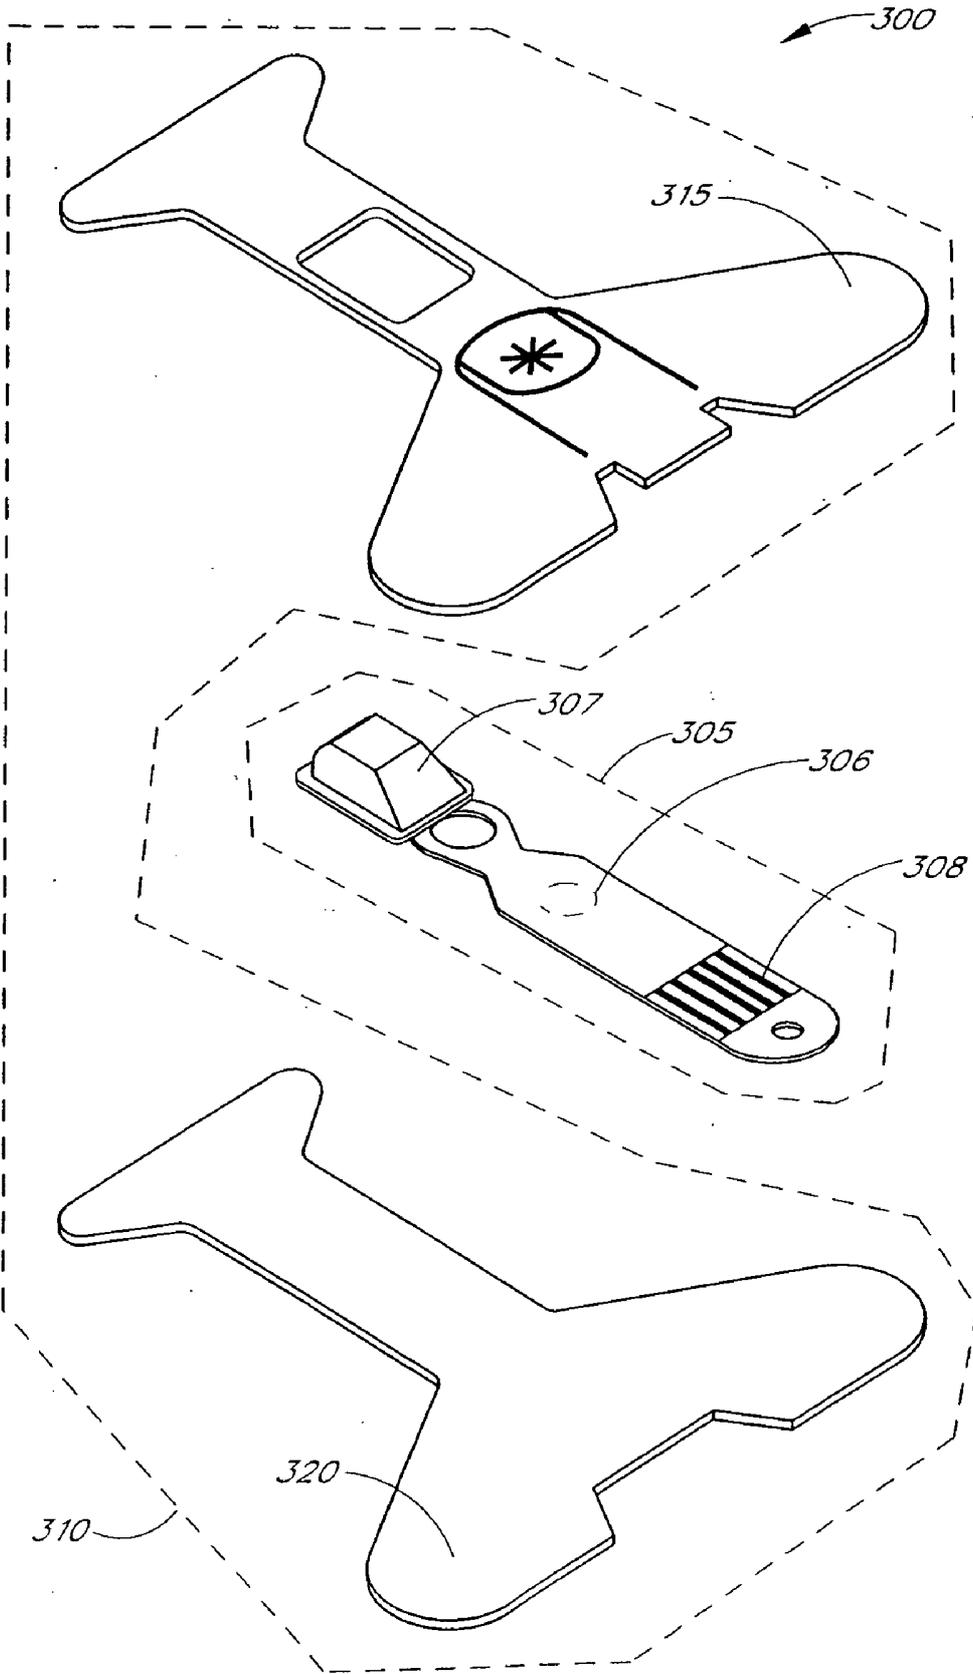


FIG. 3

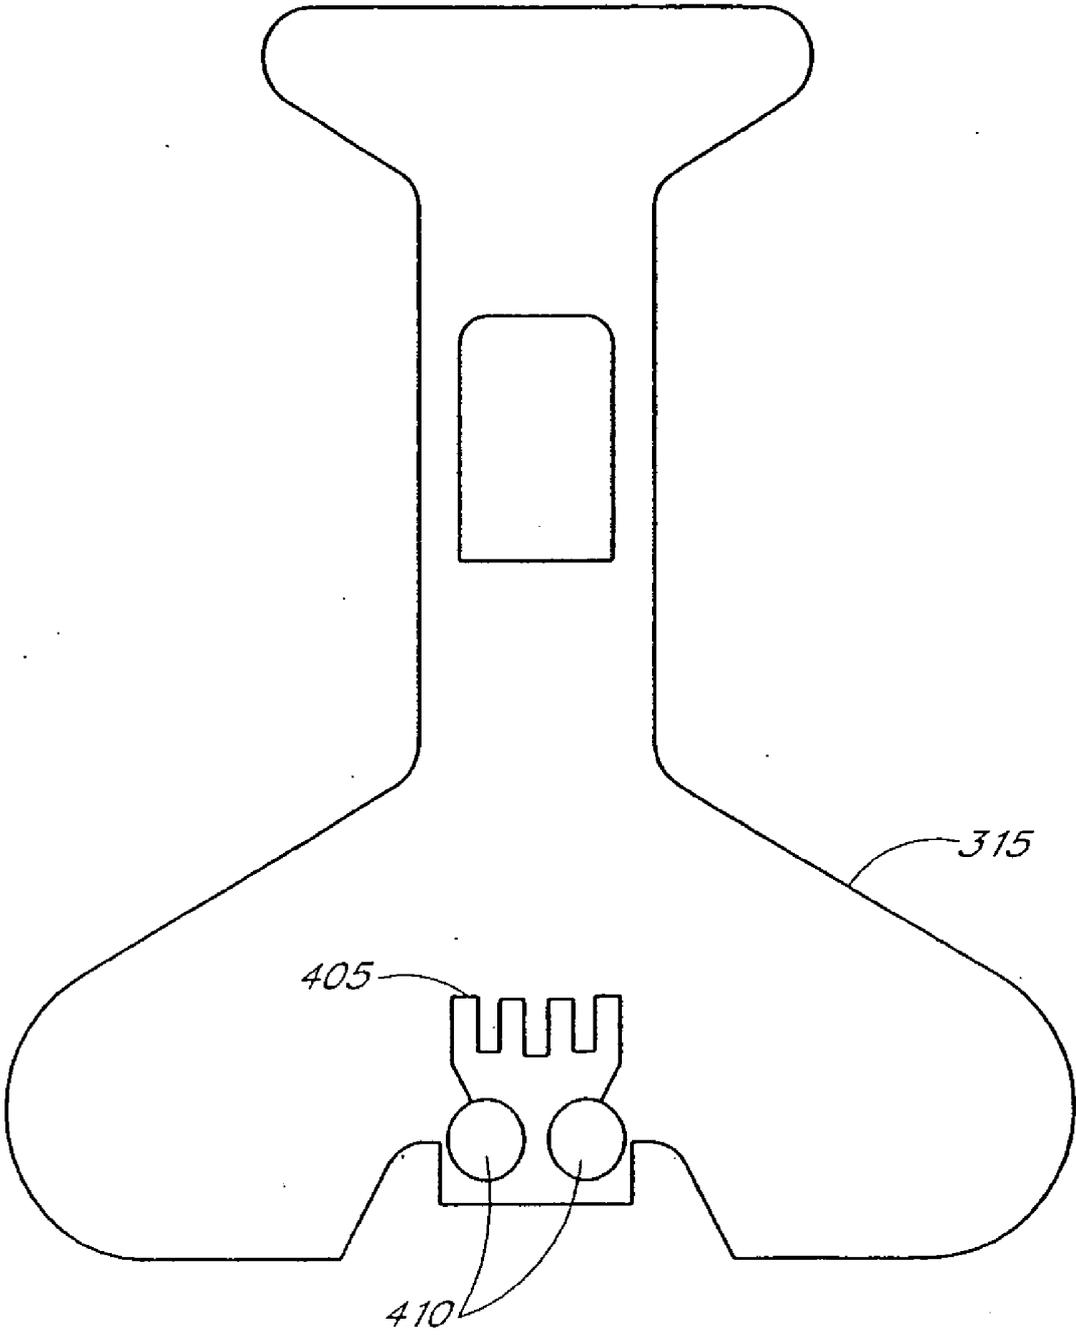


FIG. 4

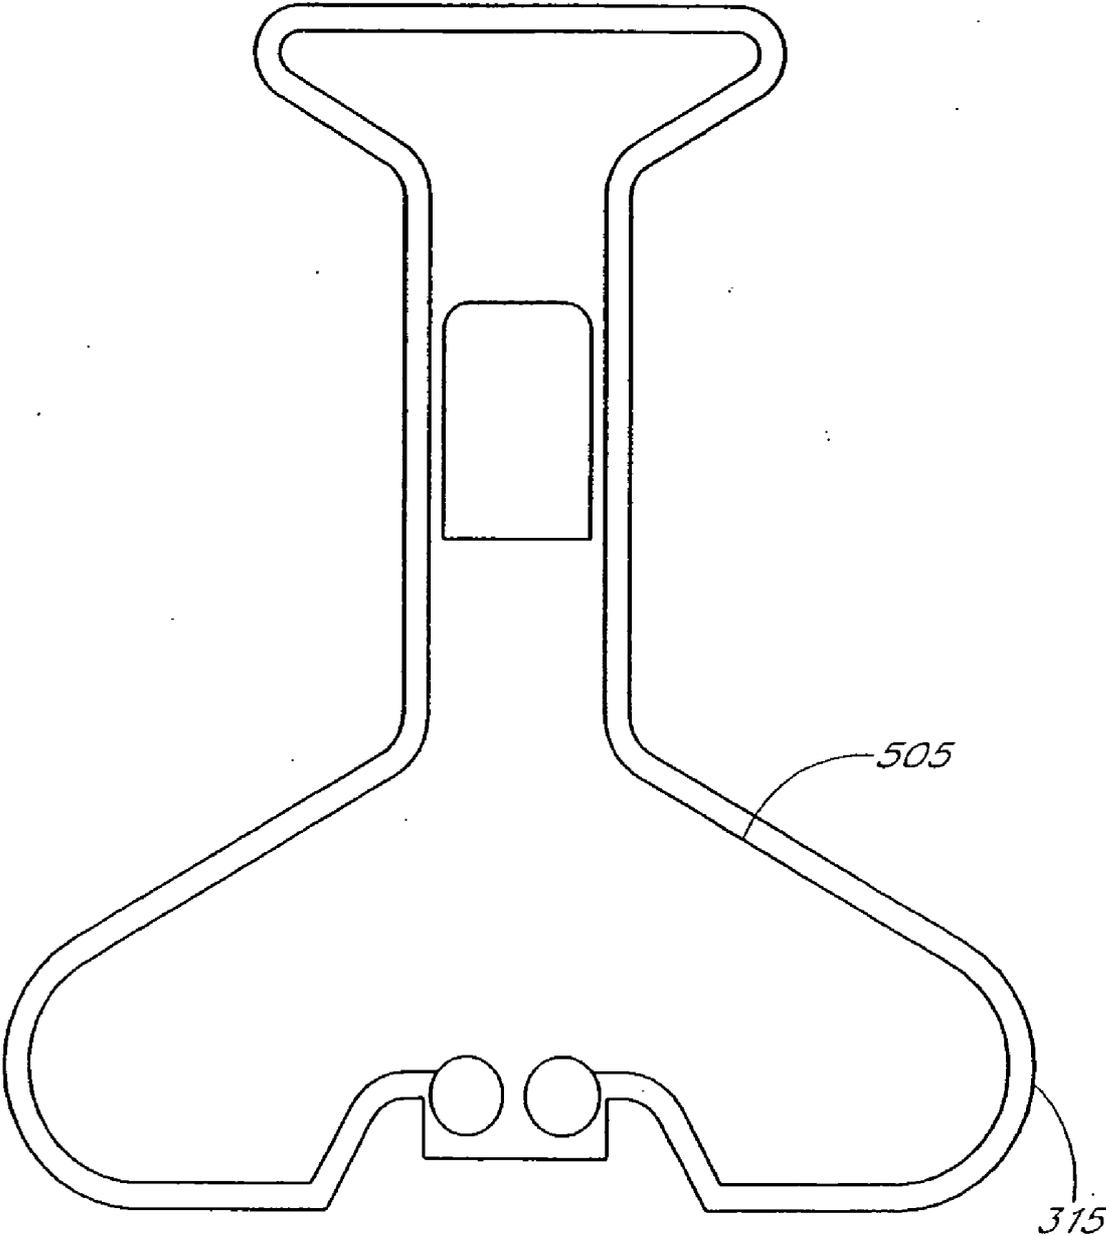


FIG. 5

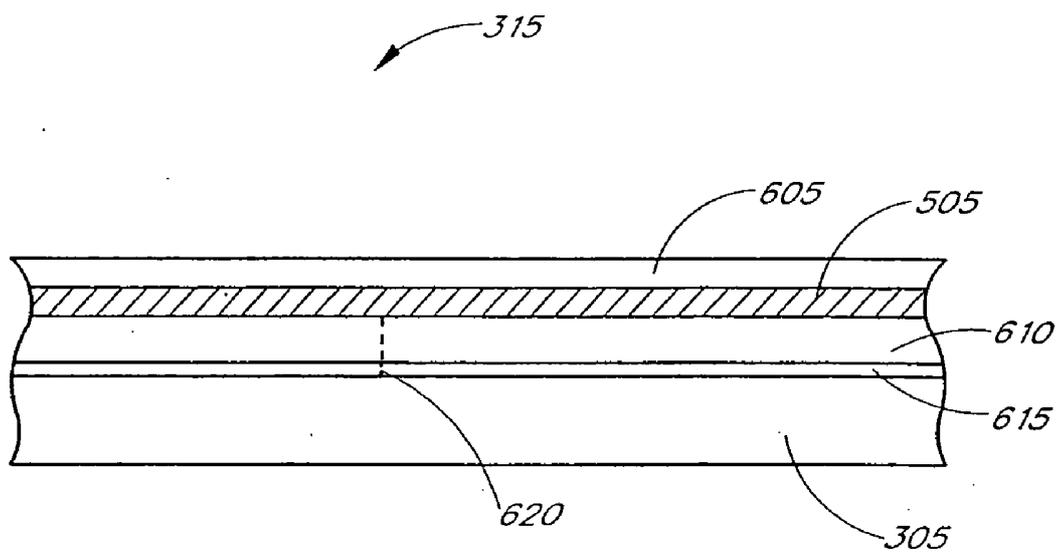


FIG. 6A

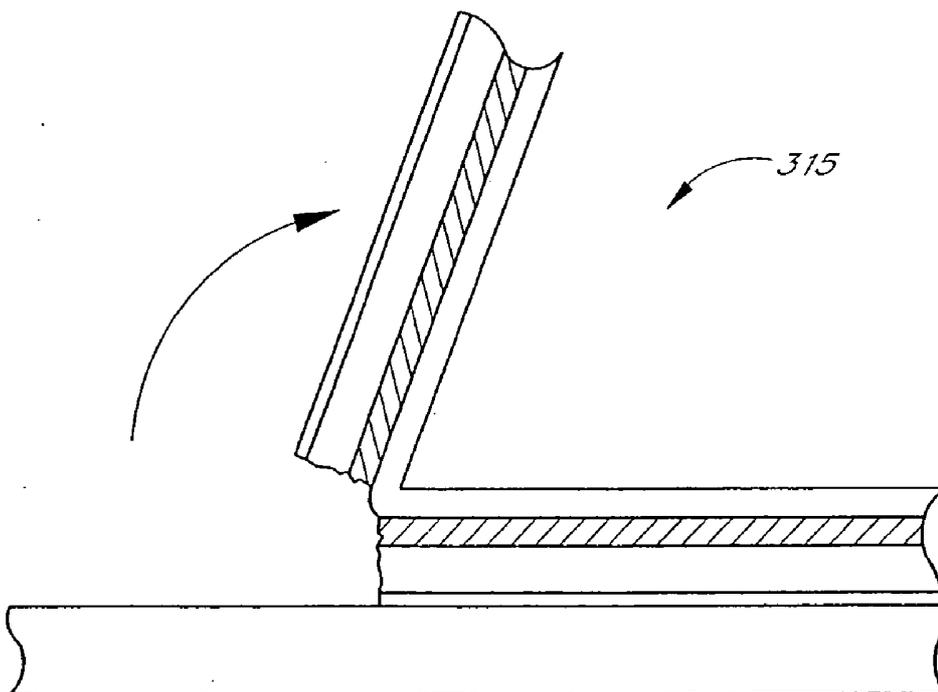


FIG. 6B

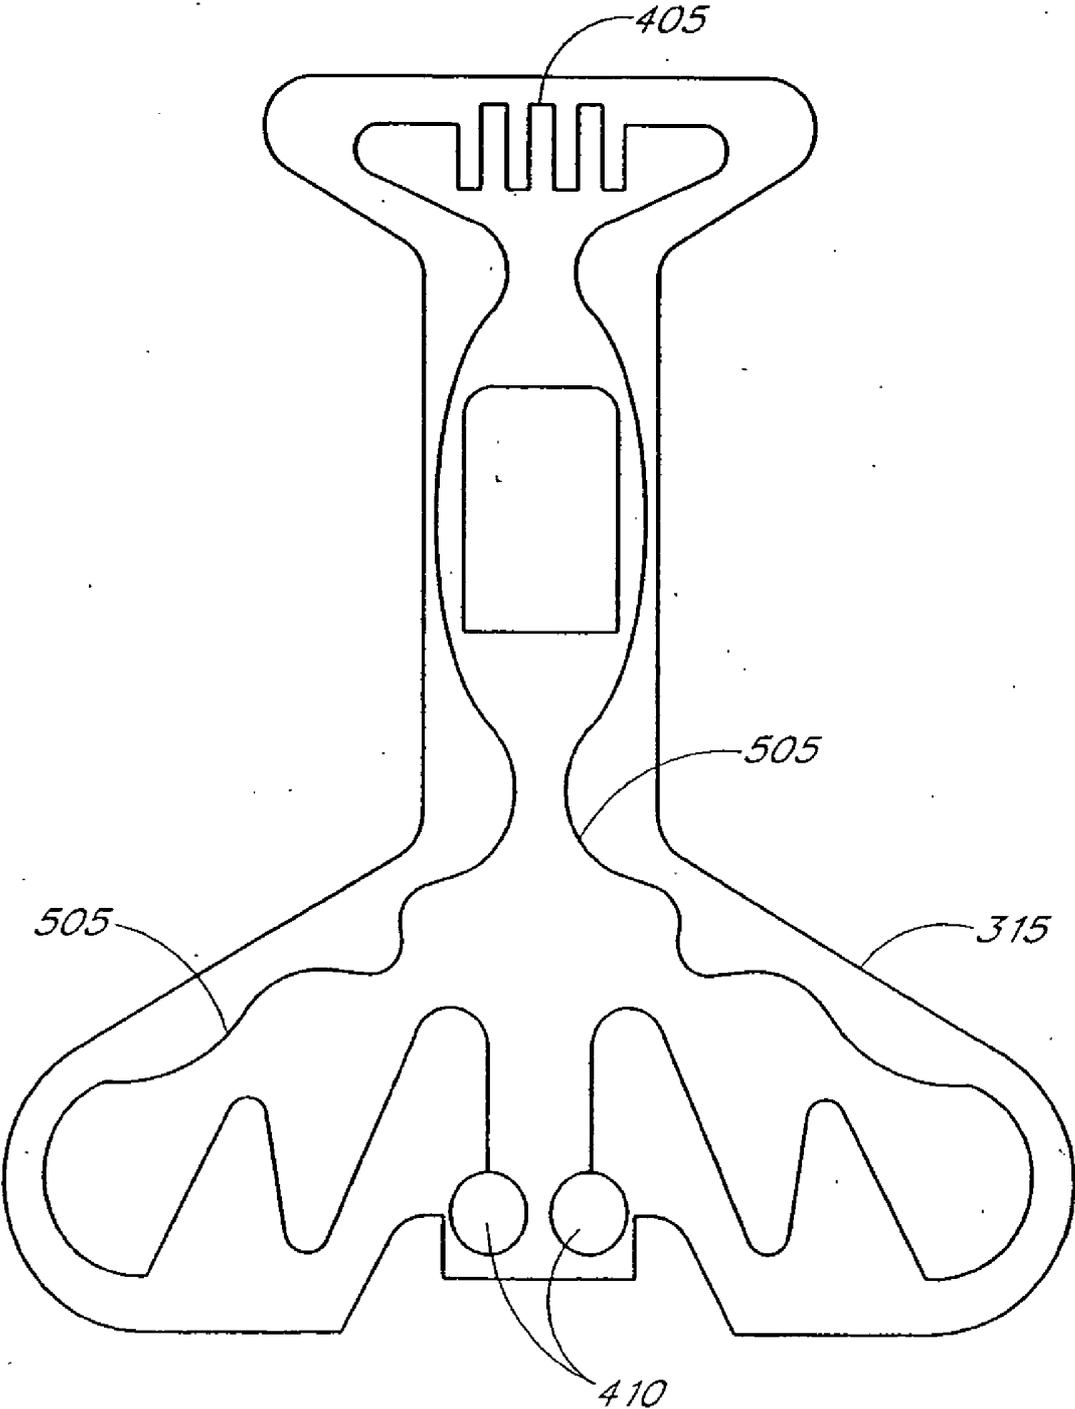


FIG. 7

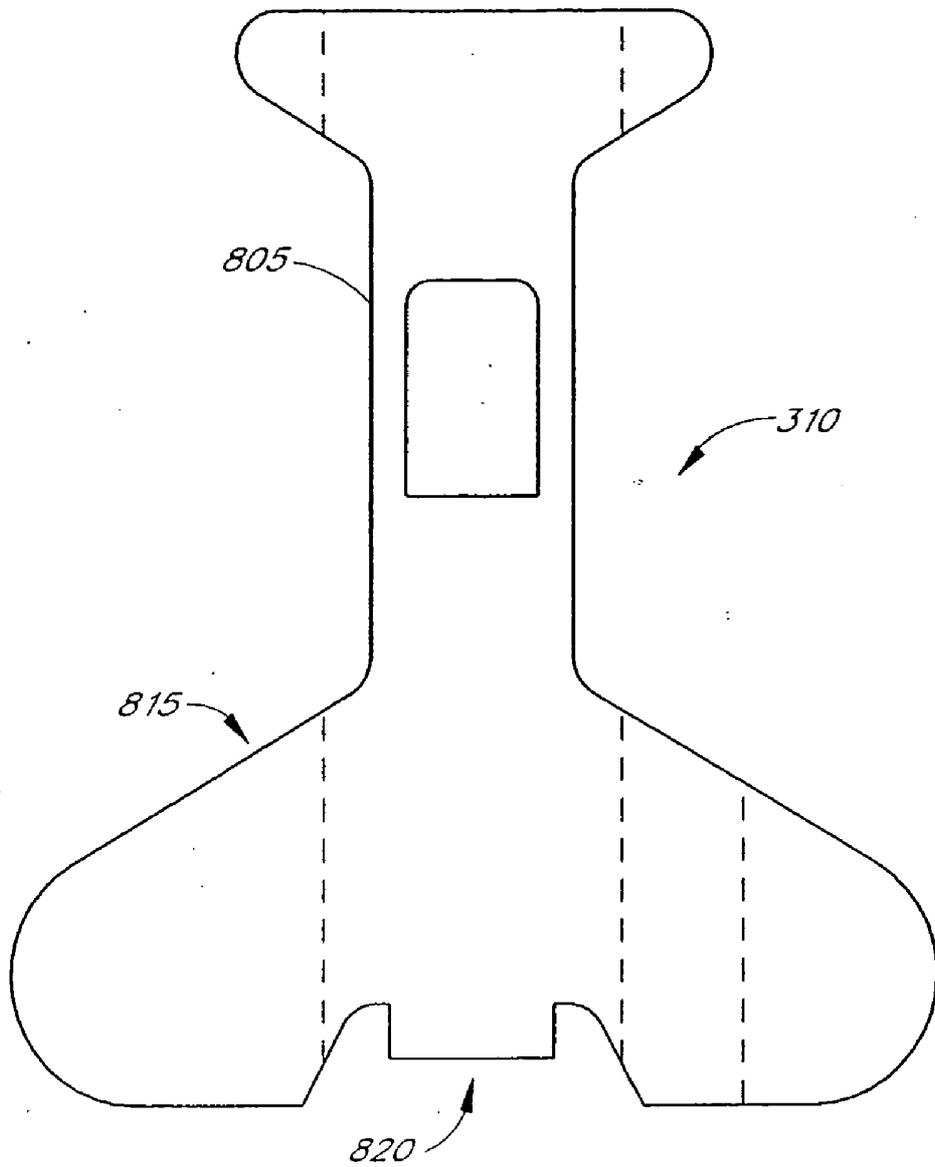


FIG. 8A

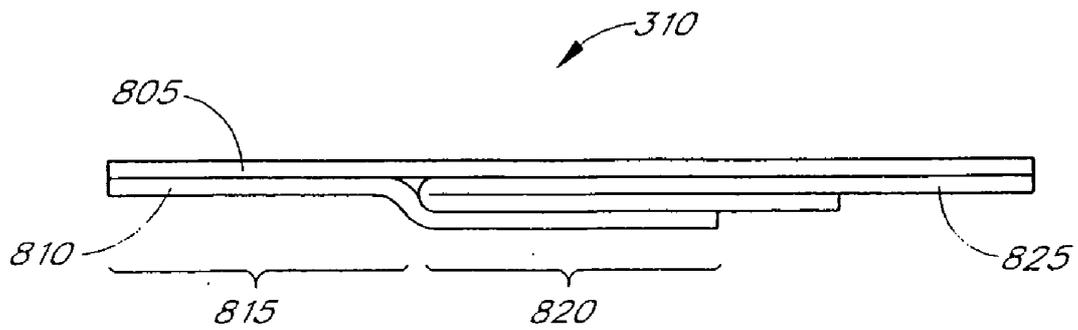


FIG. 8B

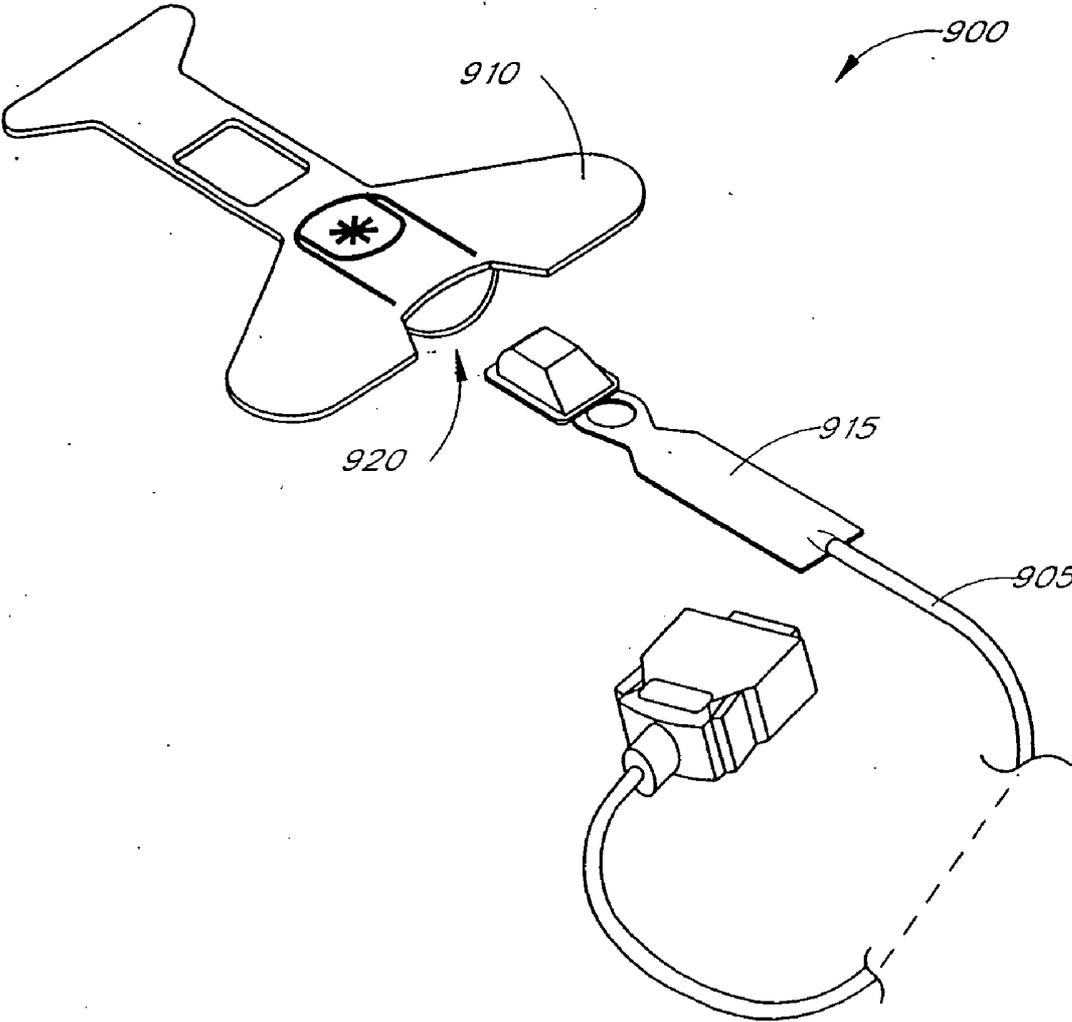


FIG. 9A

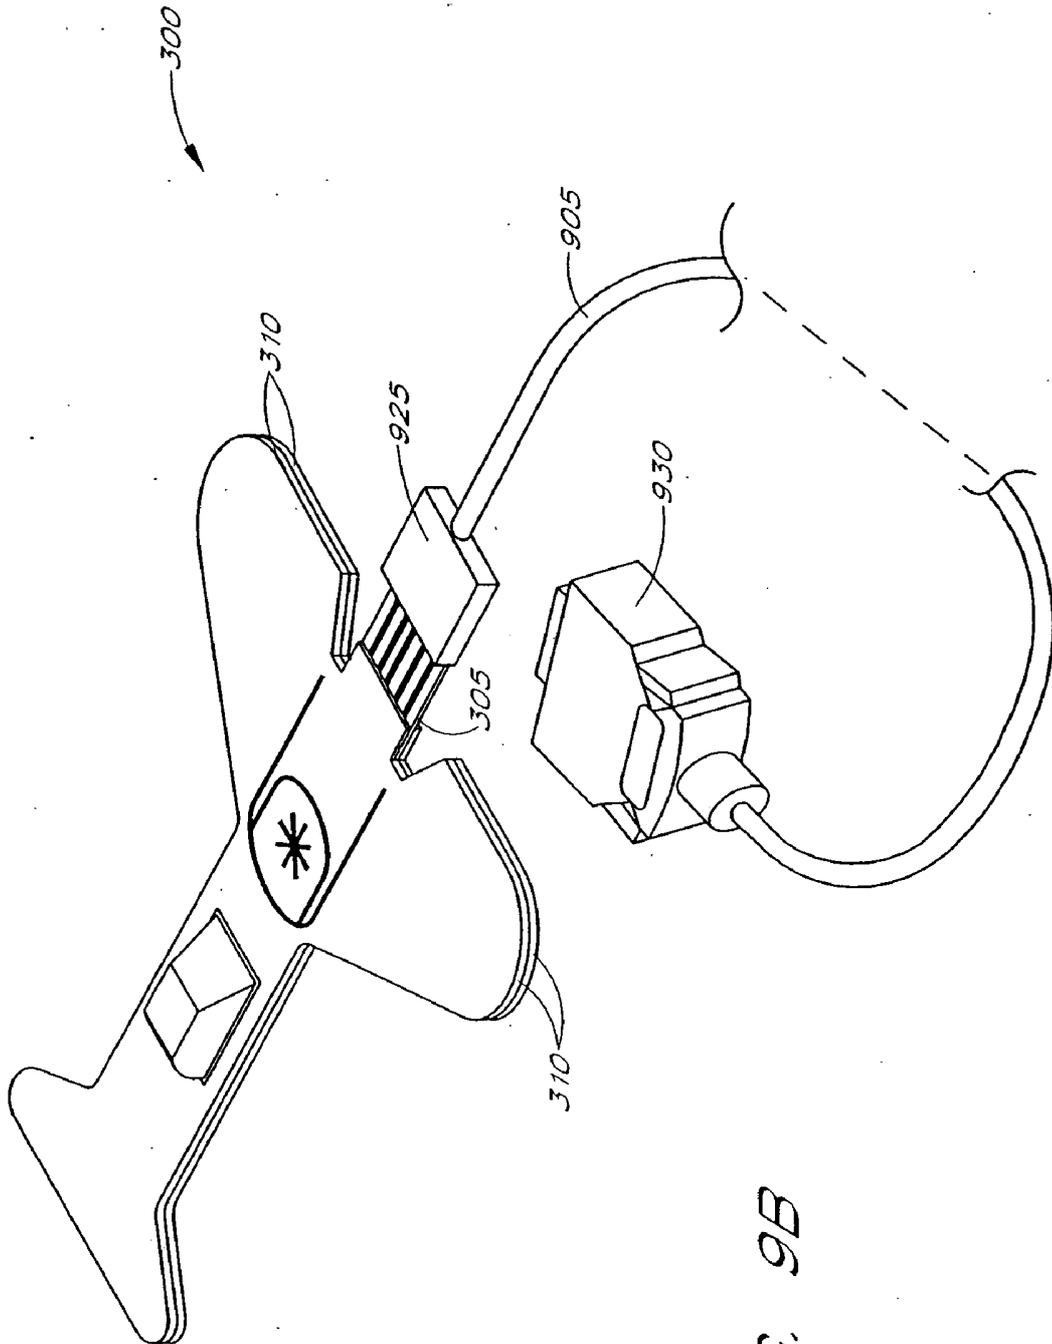


FIG. 9B

## RESPONSABLE PULSE OXIMETRY SENSOR

### PRIORITY CLAIM TO RELATED APPLICATIONS

[0001] The present application is a continuation of U.S. patent application Ser. No. 10/741,777, filed on Dec. 19, 2003, entitled "Responsible Pulse Oximetry Sensor," now U.S. Pat. No. 7,039,449, which is a continuation of U.S. patent application Ser. No. 10/128,721, filed on Apr. 23, 2002, entitled "Responsible Pulse Oximetry Sensor," which is a continuation of U.S. Patent No. U.S. patent application Ser. No. 09/456,666, filed Dec. 12, 1999, entitled "Responsible Pulse Oximetry Sensor," now U.S. Pat. No. 6,377,829. The present application incorporates the foregoing disclosures herein by reference.

### FIELD OF THE INVENTION

[0002] The present invention relates in general to sensors for measuring oxygen content in the blood, and, in particular, relates to responsible (reusable/disposable) sensors having an information element contained therein.

### BACKGROUND

[0003] Early detection of low blood oxygen is critical in a wide variety of medical applications. For example, when a patient receives an insufficient supply of oxygen in critical care and surgical applications, brain damage and death can result in just a matter of minutes. Because of this danger, the medical industry developed oximetry, a study and measurement of the oxygen status of blood. One particular type of oximetry, pulse oximetry, is a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of the oxygen status of the blood. A pulse oximeter relies on a sensor attached to a patient in order to measure the blood oxygen saturation.

[0004] Conventionally, a pulse oximeter sensor has a red emitter, an infrared emitter, and a photodiode detector. The sensor is typically attached to a patient's finger, earlobe, or foot. For a finger, the sensor is configured so that the emitters project light through the outer tissue of the finger and into the blood vessels and capillaries contained inside. The photodiode is positioned at the opposite side of the finger to detect the emitted light as it emerges from the outer tissues of the finger. The photodiode generates a signal based on the emitted light and relays that signal to an oximeter. The oximeter determines blood oxygen saturation by computing the differential absorption by the arterial blood of the two wavelengths (red and infrared) emitted by the sensor.

[0005] Conventional sensors are either disposable or reusable. A disposable sensor is typically attached to the patient with an adhesive wrap, providing a secure contact between the patient's skin and the sensor components. A reusable sensor is typically a clip that is easily attached and removed, or reusable circuitry that employs a disposable attachment mechanism, such as an adhesive tape or bandage.

[0006] The disposable sensor has the advantage of superior performance due to conformance of the sensor to the skin and the rejection of ambient light. However, repeated removal and reattachment of the adhesive tape results in deterioration of the adhesive properties and tearing of the tape. Further, the tape eventually becomes soiled and is a

potential source of cross-patient contamination. The disposable sensor must then be thrown away, wasting the long-lived emitters, photodiode and related circuitry.

[0007] On the other hand, the clip-type reusable sensor has the advantage of superior cost savings in that the reusable pulse sensor does not waste the long-lived and expensive sensor circuitry. However, as mentioned above, the clip-type reusable sensor does not conform as easily to differing patient skin shape, resulting in diminished sensitivity and increased ambient light.

[0008] Similar to the clip-type reusable sensor, the circuit-type reusable sensor advantageously does not waste the sensor circuitry. On the other hand, the circuit-type reusable sensor fails to provide quality control over the attachment mechanism. Much like the disposable sensors, the attachment mechanism for the circuit-type reusable sensor may become soiled or damaged, thereby leading to cross-patient contamination or improper attachment. Moreover, because the reusable circuit is severable from the attachment mechanism, operators are free to use attachment mechanisms that are either unsafe or improper with regard to a particular type of reusable circuitry.

[0009] Based on the foregoing, significant and costly drawbacks exist in conventional disposable and reusable oximetry sensors. Thus, a need exists for an oximetry sensor that incorporates the advantages found in the disposable and reusable sensors, without the respective disadvantages.

### SUMMARY OF THE INVENTION

[0010] Accordingly, one aspect of the present invention is to provide a reusable/disposable (responsible) sensor having a disposable adhesive tape component that can be removed from other reusable sensor components. This hybrid sensor combines the longevity and associated cost advantages of the reusable sensor with the performance features of the disposable.

[0011] In one embodiment of the responsible sensor, the disposable tape includes an information element along with a mechanism for the electrical connection of the information element to the emitters. The information element provides an indication to an attached oximeter of various aspects of the sensor.

[0012] According to another embodiment, the information element provides an indication of the sensor type. According to yet another embodiment, the information element provides an indication of the operating characteristics of the sensor. In yet another embodiment, the information element provides security and quality control. For instance, the information element advantageously indicates that the sensor is from an authorized supplier.

[0013] According to yet another embodiment, the information element is advantageously located in the disposable portion and configured to be in communication with the reusable portion via a breakable conductor. The breakable conductor is also located within the disposable portion such that excessive wear of the disposable portion results in isolation of the information element, thereby indicating that the disposable portion should be replaced. Moreover, the information element may comprise one or more passive or active components, ranging from a single coding resistor to

an active circuit, such as a transistor network, a memory device, or a central processing component.

[0014] Therefore, one aspect of the present invention is a pulse oximetry sensor including a reusable portion having an emitter configured to transmit light through tissue, a detector configured to receive light from tissue, a first contact, an external connector configured to attach to a monitor, and electrical circuitry configured to provide electrical communications to and from the external connector, the emitter, the detector and the first contact. The pulse oximetry sensor also includes a disposable portion configured to attach the reusable portion to the tissue. The disposable portion has an information element, a breakable conductor, and a second contact electrically connecting the information element and the breakable conductor, the second contact configured to create an electrical connection to the first contact when the disposable portion is combined with the reusable portion.

[0015] Another aspect of the present invention is a responsible sensor for noninvasively measuring a physiological parameter in tissue. The responsible sensor includes a reusable portion and a disposable portion. The disposable portion has at least one of an information element and a conductor electrically connected to the reusable portion. Moreover, the disposable portion is configured to secure the reusable portion to a measurement site.

[0016] Another aspect of the present invention is a method of providing disposable oximeter sensor elements. The method includes forming a disposable housing configured to receive a reusable electronic circuit. The method also includes forming at least one of an information element and a conductor associated with the disposable housing and configured to be disconnected from the reusable electronic circuit when the disposable housing is damaged, overused, or repeatedly attached.

[0017] Another aspect of the present invention is a method of providing reusable oximeter sensor elements. This includes forming a reusable electronic circuit configured to electrically connect with electronic components of a disposable housing and to employ the disposable housing for attachment to a measurement site.

[0018] Another aspect of the present invention is a method of measuring a tissue characteristic. This method includes creating a sensor through combining reusable electronic circuitry with a first disposable material such that an electrical connection is made between the reusable electronic circuitry and electronic components associated with the first disposable material. Moreover, the method includes attaching the sensor to a measurement site, removing the sensor, separating the reusable electronic circuitry from the first disposable material, and recombining the reusable electronic circuitry with a second disposable material.

[0019] Another aspect of the present invention is a pulse oximeter having a sensor including a reusable portion and a disposable portion. The disposable portion includes an information element electrically connected to the reusable portion through a breakable conductor. The breakable conductor is configured to electrically disconnect the information element from the reusable portion in the event of overuse, damage, or excessive reattachment of the disposable portion. Moreover, the pulse oximeter includes a monitor, and a cable for connecting the sensor to the monitor.

[0020] Yet another aspect of the present invention is a pulse oximeter sensor element having a disposable material that incorporates electronic components. The disposable material is configured to removably receive reusable oximeter sensor elements such that the electronic components electrically connect with the reusable oximeter sensor elements. Moreover, the disposable material is configured to secure the reusable oximeter sensor elements to a measurement site.

[0021] Another aspect of the present invention is a pulse oximeter sensor element including reusable electronic circuitry configured to electrically connect with electronic components of a disposable material and to employ the disposable material for attachment to a measurement site.

[0022] Another aspect of the present invention is a responsible sensor for measuring a tissue aspect. The responsible sensor includes a face tape, a base tape removably attached to the face tape, and reusable measurement circuitry removably secured between the face tape and the base tape. The reusable measurement circuitry is also configured to connect to an external monitor and configured to measure an aspect of tissue at a measurement site. Moreover, the face tape includes at least one of an information element and a breakable conductor connected to the reusable measurement circuitry when the reusable measurement circuitry is secured to the face tape.

[0023] Another aspect of the present invention is a responsible sensor having a reusable emitter and detector removably connected to a patient cable. The responsible sensor also includes a replaceable envelope having electronic circuitry configured to attach to the reusable emitter and detector such that the electronic circuitry monitors at least one characteristic of the responsible sensor. Moreover, the replaceable envelope is configured to removably receive the reusable emitter and detector and configured to secure the reusable emitter and detector to a measurement site.

[0024] Yet another aspect of the present invention is a pulse oximetry sensor having an emitter, a detector and a connector. The emitter is configured to transmit light through tissue and the detector is configured to receive light from tissue to measure a physiological parameter. Further, the connector is configured to provide electrical communications between the detector and emitter and a monitor. The pulse oximetry sensor includes a reusable portion having the emitter, the detector, the connector and a first contact in communication with the connector. Moreover, the sensor includes a disposable portion having a second contact, an information element and a conductive element disposed on an adhesive substrate configured to secure the reusable portion to a measurement site. The disposable portion removably attaches to the reusable portion in a first position such that the first contact contacts the second contact. The disposable portion detaches from the reusable portion in a second position. Also, the conductive element has a continuity condition connecting the information element to the second contact so that the information element is in communication with the connector. The conductive element has a discontinuity condition isolating the information element from the second contact and the connector. The discontinuity condition results from use of the disposable portion substantially beyond a predetermined amount.

## BRIEF DESCRIPTION OF THE DRAWINGS

[0025] **FIG. 1** illustrates a circuit diagram of a conventional disposable sensor having an information element.

[0026] **FIGS. 2A and 2B** illustrate perspective views of the conventional disposable sensor.

[0027] **FIG. 3** illustrates an exploded view of a resposable sensor having two disposable tape layers, according to one embodiment of the invention.

[0028] **FIG. 4** illustrates a top view of one of the disposable tape layers of **FIG. 3** incorporating an information element.

[0029] **FIG. 5** illustrates a top view of one of the disposable tape layers of **FIG. 3** incorporating a breakable conductor.

[0030] **FIGS. 6A and 6B** illustrate cross-sectional views of a portion of the disposable tape player of **FIG. 5**.

[0031] **FIG. 7** illustrates a top view of one of the disposable tape layers of **FIG. 3** incorporating the information element with a breakable conductor.

[0032] **FIGS. 8A and 8B** illustrate a top view and a side view, respectively, of one of the disposable layers of **FIG. 3** configured as a fold-over tape.

[0033] **FIG. 9A** illustrates a perspective view of a resposable sensor having a disposable portion configured as a tape sleeve and a reusable portion directly attached to a patient cable, according to another embodiment of the invention.

[0034] **FIG. 9B** illustrates a perspective view of a resposable sensor having a reusable portion removably attached to a patient cable, according to another embodiment of the invention.

## DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0035] The configuration of an information element for an oximeter sensor and method of reading an information element with an attached oximeter is described in U.S. Pat. No. 5,758,644, assigned to the assignee of the current application, and incorporated by reference herein. Accordingly, the configuration and the implementation of an information element will be greatly summarized as follows.

[0036] **FIG. 1** illustrates a conventional oximeter sensor circuit **100**. The oximeter sensor circuit **100** includes an emitter **105** comprising a first LED **107** and a second LED **110**. The oximeter sensor circuit further includes an information element comprising a resistor **115**. The first LED **107**, the second LED **110** and the resistor **115** are connected in parallel. The parallel connection has a common input electrical connection **120** and a common return **125**. The oximeter sensor circuit **100** also includes a photodetector **130** having an input electrical connection **135** connected to one end and having the common return **125** connected to the other end.

[0037] As mentioned, the resistor **115** is provided as an information element that can be read by an attached oximeter. In order to read the resistor **115**, the oximeter drives the oximeter sensor circuit **100** at a level where the emitter **105** draws effectively insignificant current. As is well understood in the art, the emitter **105** becomes active only if driven at

a voltage above a threshold level. Thus, at this low level, significantly all of the current through the input electrical connection **120** flows through the resistor **115**. By reducing the drive voltage across the input electrical connection **120** and common return **125** to a low enough level to not activate the emitter **105**, the emitter **105** is effectively removed from the oximeter sensor circuit **100**. Thus, the oximeter can determine the value of the resistor **115**.

[0038] The value of the resistor **115** can be preselected to indicate, for example, the type of sensor (e.g., adult, pediatric, or neonatal), the operating wavelength, or other parameters about the sensor. The resistor **115** may also be utilized for security and quality control purposes. For example, the resistor **115** may be used to ensure that the oximeter sensor circuit **100** is configured properly for a given oximeter. For instance, the resistor **115** may be utilized to indicate that the oximeter sensor circuit **100** is from an authorized supplier.

[0039] An information element other than the resistor **115** may also be utilized. The information element need not be a passive device. Coding information may also be provided through an active circuit, such as a transistor network, memory chip, or other identification device.

[0040] Furthermore, it will be understood by a skilled artisan that a number of different circuit configurations can be implemented that allow the oximeter sensor circuit **100** to include an information element. For example, the emitter **105** and the information element may each have individual electrical connections.

[0041] As mentioned above, the resistor **115** is preselected such that at low drive voltages, it is the only circuit element sensed by the oximeter. On the other hand, the resistor **115** can also be preselected be of a sufficiently high value that when the drive voltage rises to a level sufficient to drive the emitter **105**, the resistor **115** is effectively removed from the oximeter sensor circuit **100**. Thus, the resistor **115** does not affect normal operations of the emitter **105**. In summary, an information element may form an integral part of the oximeter sensor circuit **100** by providing valuable information to the attached oximeter.

[0042] **FIGS. 2A and 2B** illustrate a conventional disposable sensor **200**. The disposable sensor **200** includes an adhesive substrate **205** having an elongated center portion **210** with front and rear flaps, **215** and **220**, extending outward from the elongated center portion **210**. The adhesive substrate **205** may also have an image **225** superimposed on the adhesive substrate **205** so as to indicate proper use.

[0043] The elongated center portion **210** includes the oximeter sensor circuit **100** of **FIG. 1**. For example, the emitter **105** is housed on an underside of the elongated center portion **210** approximately beneath the superimposed image **225**. Thus, as shown in **FIG. 2A**, the emitter **105** may be housed approximately beneath the asterisk superimposed on the image of a fingernail. On the other hand, the photodetector **130** is housed on the topside of the elongated center portion **210** in proximity with the rear flaps **220**.

[0044] The elongated center portion **210** further includes an electrical connector **230** to drive the emitter **105** and to receive an output from the photodetector **130**. The electrical connector **230** is preferably configured to attach to a connector cable **235** via a sensor connector **240**. Also, the

connector cable **235** attaches to or connects with an oximeter via an oximeter connector **245**.

[0045] **FIG. 2B** illustrates an example of how the disposable sensor **200** wraps the front and rear flaps **215** and **220** around a finger such that the adhesive substrate **205** provides a secure contact between the patient's skin, the emitter **105** and the photodetector **130**. **FIG. 2B** also illustrates an example of the sensor connector **240** (shown in broken lines) encompassing the electrical connector **230**.

[0046] As shown in **FIGS. 1-2B**, the conventional disposable sensor **200** integrates the components of the conventional oximeter sensor circuit **100** such that disposal of the disposable sensor **200** includes disposal of the longer lasting, expensive circuitry found therein.

[0047] **FIG. 3** illustrates an exploded view of one embodiment of a reusable (reusable/disposable) sensor **300** according to the present invention. In this embodiment, the reusable sensor **300** includes a reusable portion **305** having an emitter **306**, a photodetector **307** and an electrical connector **308**. The reusable sensor also includes a disposable portion **310** having a face tape layer **315** and a clear base tape layer **320**. As shown in **FIG. 3**, the disposable portion **310** attaches to the reusable portion **305** by sandwiching the reusable portion **305** between a face tape layer **315** and a clear base tape layer **320**.

[0048] According to this embodiment, conventional adhesives or other attaching methodology may be used to removably attach the face tape layer **315** to the clear base tape layer **320**. Furthermore, the adhesive properties associated with the base of the conventional disposable sensor **200** may be the same as the adhesive properties on the base of the clear base tape layer **320**, as both portions are provided to attach to the patient's skin.

[0049] As mentioned, the disposable portion **310** removably attaches to the reusable portion **305** in, for example, a sandwich or layered style. After removably attaching the disposable portion **310** to the reusable portion **305**, the reusable sensor **300** functions similar to the disposable sensor **200**, i.e., the reusable sensor **300** wraps flaps around a patient's tissue such that the emitter **306** and the photodetector **307** align on opposite sides of the tissue. However, in contrast to the disposable sensor **200**, the reusable sensor **300** provides for reuse of the reusable portion **305**. For example, when the disposable portion **310** becomes contaminated, worn, or defective, rather than discarding the entire reusable sensor **300**, the disposable portion **310** is removed such that the reusable portion **305** may be re-removably attached to a new disposable portion **310**. The discarding of the disposable portion **310** completely avoids cross-contamination through the reuse of adhesive tapes between patients without wasting the more costly and longer lasting sensor circuitry of the reusable portion **305**. Note that optional sterilization procedures may be advantageously performed on the reusable portion **305** before reattachment to either the new disposable portion **310** or to the patient, in order to further ensure patient safety.

[0050] **FIG. 4** illustrates a top view of an embodiment of the face tape layer **315** of the disposable portion **310** of the reusable sensor **300**. According to this embodiment, the face tape layer **315** further includes an information element **405** as an integral part of the face tape layer **315**. In this

embodiment, the information element **405** is a resistive element made by depositing a conductive ink trace having a predetermined length and width. As is known in the art, the length, width and conductivity of the conductive ink trace determines the resistance of the resistive element. The information element **405** is deposited between contacts **410** that are also implemented with conductive ink. It will be understood by a skilled artisan that a variety of methods can be used for mating the contacts **410** with the electrical circuitry of the reusable portion **305**. For example, the contacts **410** may advantageously physically touch the leads or the electrical connector **308** such that the reusable portion **305** is electrically configured to include the information element **405**. Such a configuration employs the oximeter sensor circuit **100** of **FIG. 1**, having elements thereof distributed in both the reusable portion **305** and the disposable portion **310** of the reusable sensor **300**.

[0051] In the foregoing embodiment, the disposable portion **310** comprises the information element **405** along with the face tape layer **315** and the clear base layer **320**. As mentioned, the disposable portion **310** is removably attached to the reusable portion **305** and is employed in a similar manner as the disposable sensor **200**. In contrast to the disposable sensor **200**, when the disposable portion **310** of the reusable sensor **300** becomes worn, the disposable portion **310** and the information element **405** are discarded and the reusable portion **305** is saved. By discarding the information element, the attached oximeter can perform quality control. For example, if the reusable portion **305** is reattached to a patient using either a simple adhesive or any other non-authorized disposable mechanism, the reusable sensor **300** will not include the information element **405**. As mentioned above, an attached oximeter can recognize the absence of the information element **405** and create an appropriate response indicating inappropriate use of the reusable portion **305** of the reusable sensor **300**.

[0052] **FIG. 5** illustrates a top view of yet another embodiment of the face tape layer **315** of the disposable portion **310** of the reusable sensor **300**. In this embodiment, the face tape layer **315** includes a breakable conductor **505** comprising a conductive ink trace located approximately along the periphery of the face tape layer **315**. This location ensures that a tear along the periphery of the face tape layer **315** results in a tear, or electrical discontinuity, in the breakable conductor **505**. For example, **FIGS. 6A** and **6B** illustrate the face tape layer **315** in which the breakable conductor **505** is layered between a tape stock **605** and a tape base **610**. The reusable portion **305** of the reusable sensor **300** then attaches to the tape base **610** through a pressure sensitive adhesive (PSA) **615**. The PSA **615**, the conductor **505** and the tape base **610** include a score **620** such that multiple attachment and removal of the reusable sensor **300** will result in a peripheral tear, or electrical discontinuity, in the breakable conductor **505**, as illustrated in **FIG. 6B**.

[0053] Thus, like the information element **405**, the breakable conductor **505** also provides security and quality control functions. In particular, repeated use of the disposable portion **305** of the reusable sensor **300** advantageously severs at least one part of the breakable conductor **505**. An attached oximeter can detect such severance and initiate an appropriate notification to, for example, monitoring medical personnel. Providing security and quality control through a breakable conductor advantageously assists in controlling

problems with patient contamination or improper attachment due to weakened adhesives.

[0054] FIG. 7 illustrates yet another embodiment of the face tape layer 315. In this embodiment, the face tape layer 315 combines the breakable conductor 505 and the information element 405. In this embodiment, the breakable conductor 505 is printed in a serpentine pattern to further increase the probability of a discontinuity upon the tearing of any portion of the face tape layer 315. This combination of the information element 405 and the breakable conductor 505 advantageously adds significant safety features. For example, in this embodiment, the information element 405 is connected serially with the breakable conductor 505 and in parallel with the emitter 306 of the reusable portion 305. Therefore, any discontinuity or tear in the breakable conductor 505 separates the information element 405 from the circuitry of the reusable portion 305.

[0055] According to the foregoing embodiment, the attached oximeter receives an indication of both overuse and misuse of the responsible sensor 300. For example, overuse is detected through the tearing and breaking of the breakable conductor 505, thereby removing the information element 405 from the responsible sensor 300 circuitry. In addition, misuse through employment of disposable portions 310 from unauthorized vendors is detected through the absence of the information element 405. Moreover, misuse from purposeful shorting of the contacts 410 is detected by effectively removing the emitter 306 from the circuit, thereby rendering the responsible sensor 300 inoperative. Therefore, the responsible sensor 300 of this embodiment advantageously provides a multitude of problem indicators to the attached oximeter. By doing so, the responsible sensor 300 advantageously prevents the likelihood of contamination, adhesive failure, and misuse. The responsible sensor 300 also advantageously maintains the likelihood of quality control.

[0056] A skilled artisan will recognize that the concepts of FIGS. 3-7 may be combined in total or in part in a wide variety of devices. For example, either or both of the breakable conductor 505 and the information element 405 may advantageously be traced into the clear base tape layer 320 rather than into the face tape layer 315.

[0057] FIGS. 8A and 8B illustrate yet another embodiment of the disposable portion 310 of the responsible sensor 300 according to the present invention. As shown in this embodiment, the disposable portion 310 includes a face tape layer 805 and a clear base tape layer 810. According to this embodiment, the clear base tape layer 810 includes a pre-attached section 815 and a fold over section 820. The preattached section 815 attaches approximately one third of the face tape layer 805 to the clear base tape layer 810. On the other hand, the fold over section 820 forms a flap configured to create a cavity between the face tape layer 805 and the clear base tape layer 810. The cavity is configured to receive the reusable portion 305 of the responsible sensor 300. According to one embodiment, a release liner 825 fills the cavity and separates the face tape layer 805 from the clear base tape layer 810. When the release liner 825 is removed, newly exposed adhesive on the fold over section 820 and the face tape layer 805 removably attaches the reusable portion 305 between the face tape layer 805 and fold over section 820 of the clear base tape layer 810.

[0058] According to another embodiment, the cavity is so formed that adhesive is not needed. For example, the fold over section 820 may comprise resilient material that can form a friction fit relationship so as to fix the reusable portion 305 in an appropriate position relative to the disposable portion 310. On the other hand, the fold over section 820 may also comprise material having other than resilient or adhesive properties, but still allow for proper placement of the reusable portion 305 and disposable portion 310 on the patient. For example, hook-and-loop type materials like VELCRO® may be used.

[0059] It will be understood that a skilled artisan would recognize that the fold over embodiment of the responsible sensor 300 may employ the properties discussed in relation to FIGS. 3-7, such as the information element 405 and the breakable wire 505.

[0060] FIG. 9A illustrates an embodiment of a responsible sensor 900 integrated with an attached patient cable 905, according to another embodiment of the invention. In this embodiment, a disposable portion 910 is attached to a reusable portion 915 by removably inserting the reusable portion 915 into a tape envelope 920 formed in the disposable portion 910.

[0061] A skilled artisan will recognize that the disposable portion 910 may include the information element 405, the breakable wire 505, or both. Inclusion of one or both of these electronic components in the responsible sensor 900 advantageously provides the security, quality control, and safety features described in the foregoing embodiments.

[0062] FIG. 9B illustrates an embodiment of a responsible sensor 300 of FIG. 3, according to another embodiment of the invention. According to this embodiment, the responsible sensor 300 removably attaches to the patient cable 905 via a sensor connector 925. The patient cable 905 then attaches to an oximeter via an oximeter connector 930. Use of the sensor connector 925 enables the replacement of both the reusable portion 305 of the responsible sensor 300 without replacement of the sensor connector 925 or patient cable 905. In such an embodiment, the disposable portion 310 would follow a different, more frequent, replacement schedule than that of the reusable portion 305.

[0063] A skilled artisan will recognize that the variety of configurations described above that include the information element 405, the breakable wire 505, or both, may be incorporated into the embodiment of FIG. 9B.

[0064] Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art. For example, select aspects of FIGS. 3-9B may be combined. For example, the envelope configured disposable portion 910 of FIG. 9A may be combined with the reusable portion 305 of FIG. 3.

[0065] Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the reaction of the preferred embodiments, but is to be defined by reference to the appended claims.

What is claimed is:

1. A disposable component of an optical probe comprising:

a disposable attachment mechanism including an adhesive side capable of removably securing a reusable component of an optical probe to a measurement site on body tissue, wherein the reusable component includes a light emitting source capable of emitting light at different wavelengths, a light detector capable of detecting the light after it has been attenuated by the body tissue, and a plurality of conductors; and

an information element; and

an electrical connection electrically connecting the information element to ones of the plurality of conductors in the reusable component when the reusable component and the disposable attachment mechanism are combined to form an optical probe, wherein the information element provides information about the optical probe.

2. The disposable component of claim 1; wherein the information element comprises a resistor.

3. The disposable component of claim 1, wherein the information element comprises a memory chip.

4. The disposable component of claim 1, wherein the information element comprises an identification device.

5. The disposable component of claim 1, wherein the information element comprises a transistor network.

6. The disposable component of claim 1, wherein the information element comprises an active circuit.

7. A noninvasive optical probe including a disposable portion and a reusable portion, the optical probe comprising:

a reusable portion including a light emitting source, a detector, and a plurality of electrical wires; and

a disposable portion including an information element electrically communicating with ones of the plurality of electrical wires.

8. The noninvasive optical probe of claim 7, wherein the information element comprises a resistor.

9. The noninvasive optical probe of claim 7, wherein the information element comprises a memory chip.

10. The noninvasive optical probe of claim 7, wherein the information element comprises an identification device.

11. The noninvasive optical probe of claim 7, wherein the information element comprises a transistor network.

12. The noninvasive optical probe of claim 7, wherein the information element comprises an active circuit.

13. A method of electrically connecting an information element to conductors of a reusable circuit of an optical probe, the method comprising:

providing a reusable circuit including a light emitting source capable of emitting light at different wavelengths, a light detector capable of detecting the light after it has been attenuated by body tissue, and a plurality of conductors;

providing a disposable tape adapted to position the reusable circuit on the body tissue, the disposable tape including an information element; and

removably combining the reusable circuit with the disposable tape including making an electrical connection between the information element and ones of the plurality of conductors.

14. The method of claim 13, comprising reading information from the information element over the ones of the plurality of conductors.

15. The method of claim 14, comprising configuring a patient monitor based on the information.

16. The method of claim 13, wherein the information element comprises a resistor.

17. The method of claim 13, wherein the information element comprises a memory chip.

18. The method of claim 13, wherein the information element comprises an identification device.

19. The method of claim 13, wherein the information element comprises a transistor network.

20. The method of claim 13, wherein the information element comprises an active circuit.

\* \* \* \* \*

专利名称(译)	一次性脉搏血氧饱和度传感器		
公开(公告)号	<a href="#">US20060200018A1</a>	公开(公告)日	2006-09-07
申请号	US11/415600	申请日	2006-05-02
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	摩根大通银行, NATIONAL ASSOCIATION		
[标]发明人	AL ALI AMMAR		
发明人	AL-ALI, AMMAR		
IPC分类号	A61B5/00 A61B5/145 A61B5/1455		
CPC分类号	A61B5/14552 A61B5/6826 A61B5/6838 Y10T137/4478		
其他公开文献	US8000761		
外部链接	<a href="#">Espacenet</a>	<a href="#">USPTO</a>	

摘要(译)

脉冲血氧计传感器具有可重复使用部分和一次性部分。传感器的可重复使用部分保留了相对长寿命且昂贵的发射器,探测器和连接器组件。传感器的一次性部分是相对便宜的胶带组件,其用于将传感器固定到测量部位,通常是患者的手指或脚趾。传感器的一次性部分可拆卸地连接到可再用部分上,使得当粘合剂消耗或者带弄脏或过度磨损时,一次性部分可以容易地更换。一次性部分还可以包含用于传感器识别或用于安全目的的信息元件,以确保患者安全。

