




US 20040122301A1

(19) **United States**(12) **Patent Application Publication****Kiani et al.**(10) **Pub. No.: US 2004/0122301 A1**(43) **Pub. Date:****Jun. 24, 2004**(54) **PARAMETER COMPENSATED PULSE
OXIMETER****Publication Classification**(51) **Int. Cl.⁷** **A61B 5/00**(52) **U.S. Cl.** **600/336; 600/300**(76) Inventors: **Massl E. Kiani**, Laguna Niguel, CA
(US); **Mohamed Diab**, Mission Viejo,
CA (US); **Ammar Al-Ali**, Tustin, CA
(US); **Walter M. Weber**, Laguna Hills,
CA (US)(57) **ABSTRACT**

Correspondence Address:

KNOBBE MARTENS OLSON & BEAR LLP
2040 MAIN STREET
FOURTEENTH FLOOR
IRVINE, CA 92614 (US)(21) Appl. No.: **10/671,179**(22) Filed: **Sep. 25, 2003****Related U.S. Application Data**(60) Provisional application No. 60/413,494, filed on Sep.
25, 2002.

A monitor has a primary input responsive to a first property of a tissue site. An uncompensated measurement is determinable from the primary input. A parameter input is responsive to a second property associated with the tissue site, where the first property is dependent upon the second property. The monitor also has a compensation relationship of the primary input, the parameter input and a compensated measurement. A processor is configured to output a compensated measurement from the primary input and the parameter input utilizing the compensation relationship, where the compensated measurement more accurately represents the first property than the uncompensated measurement.

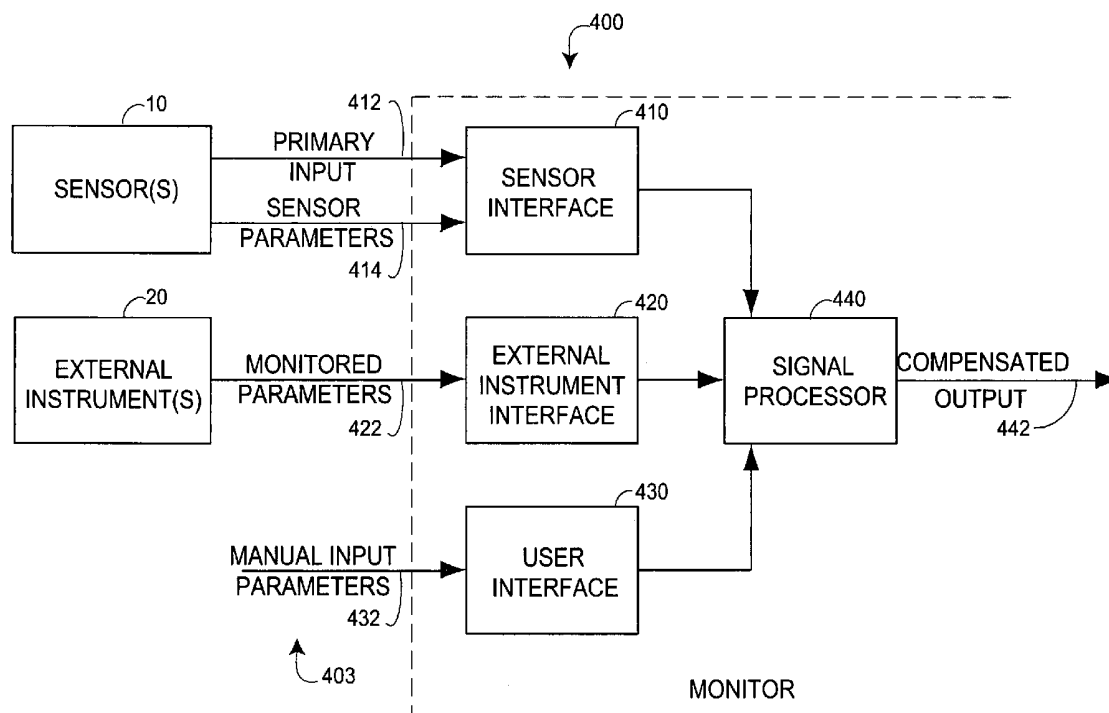

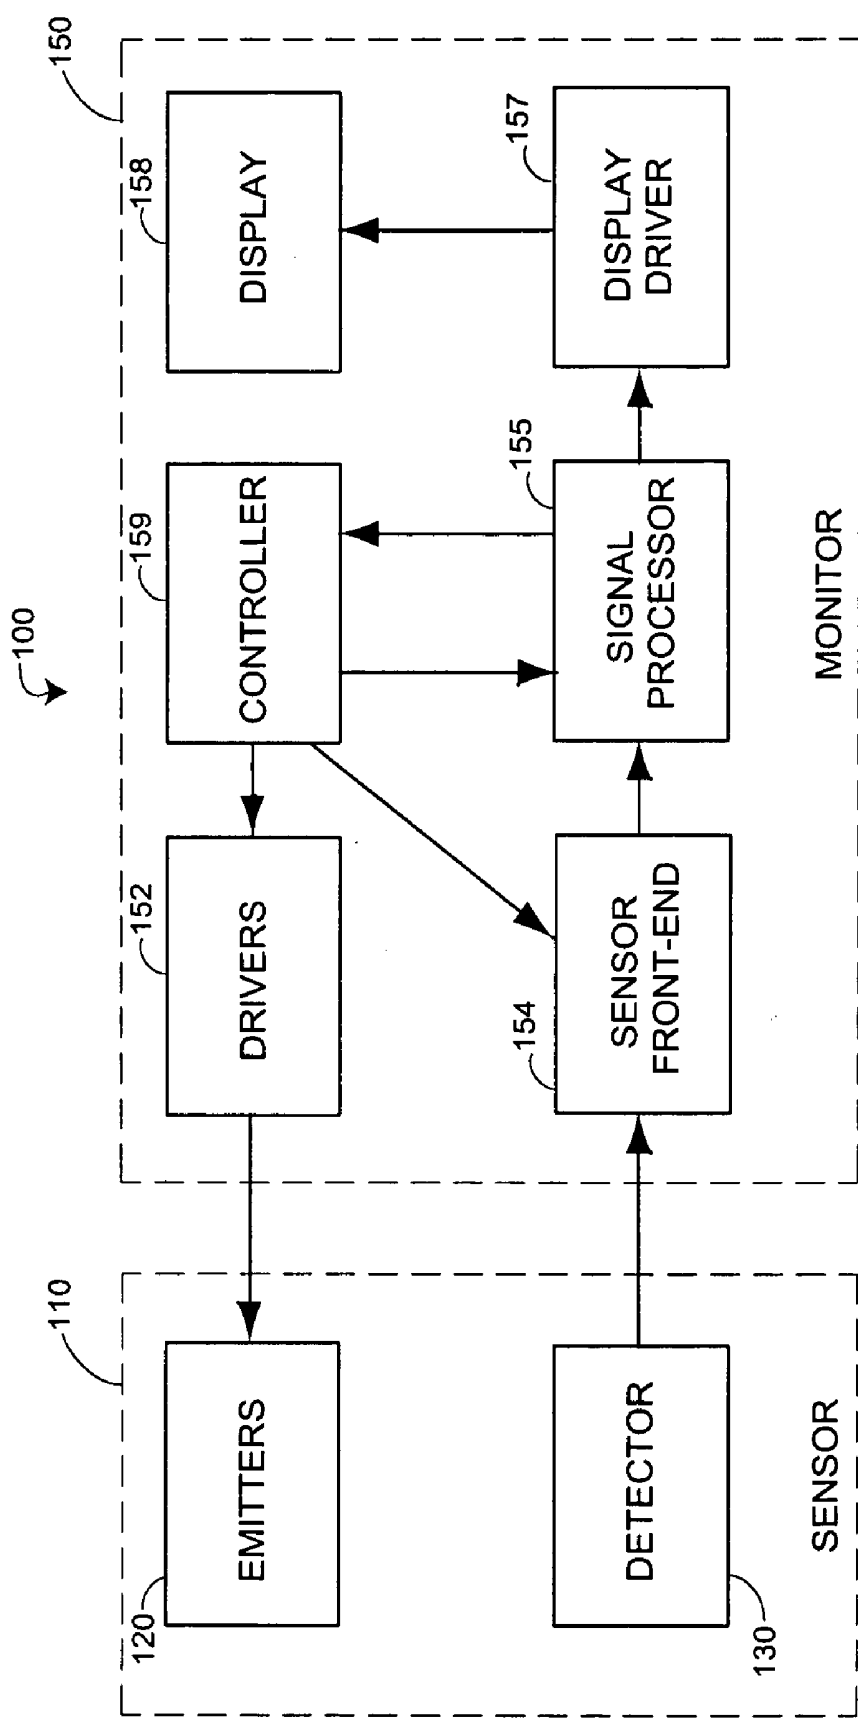
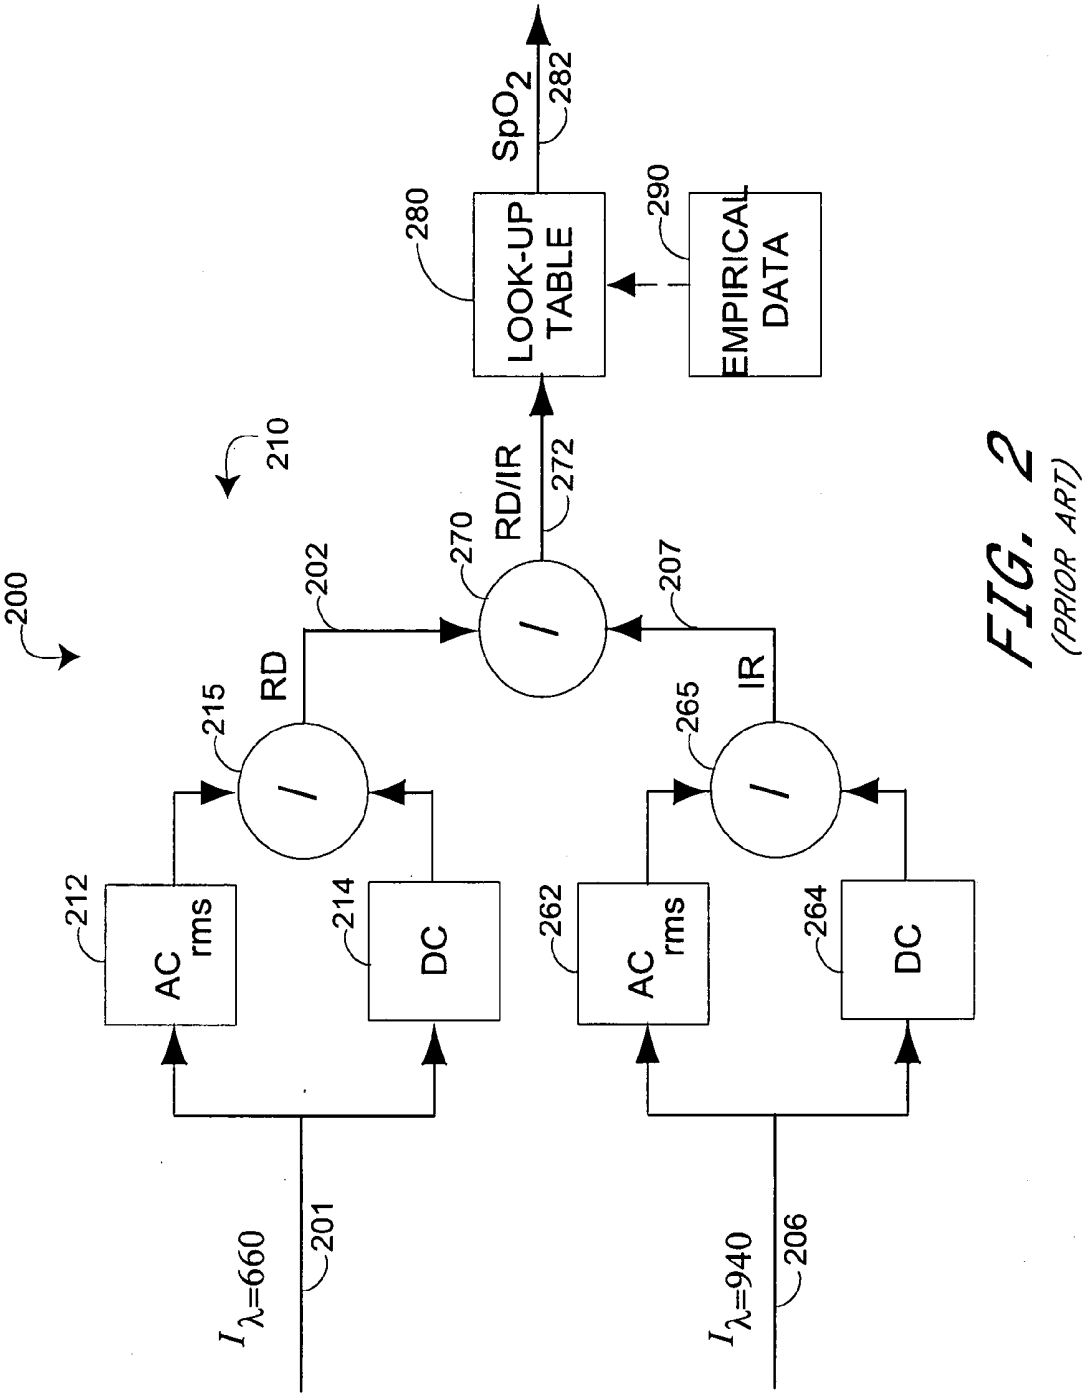


FIG. 1
(PRIOR ART)



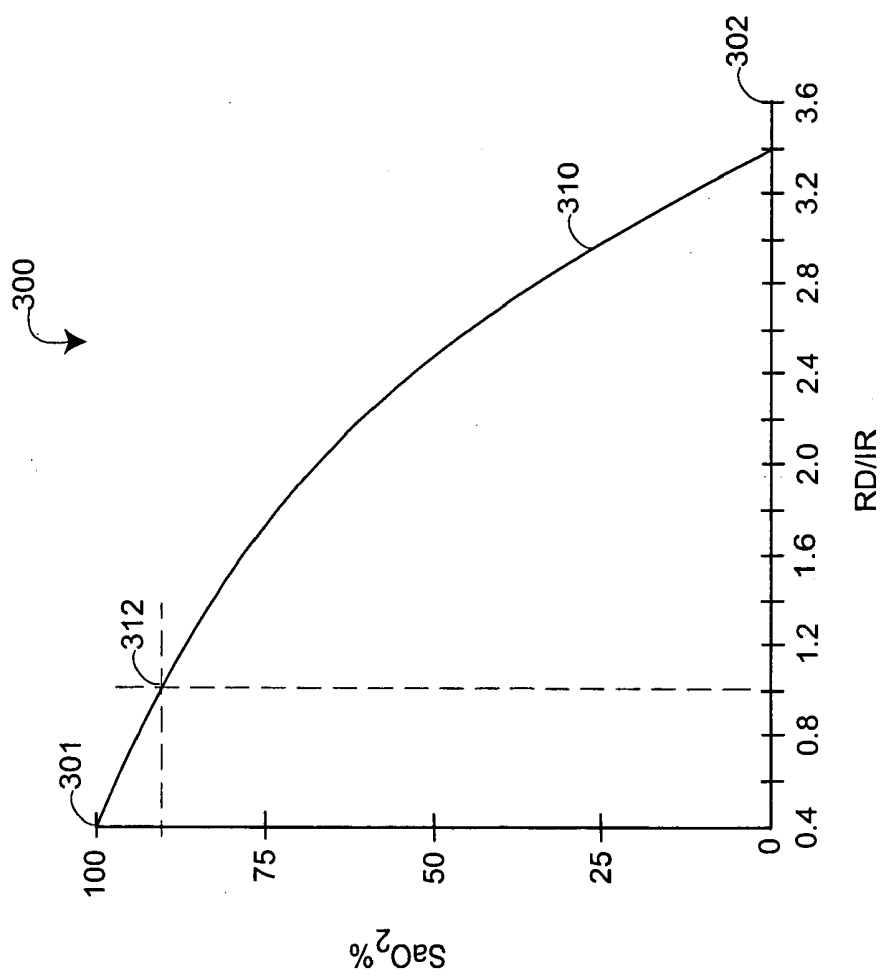


FIG. 3
(PRIOR ART)

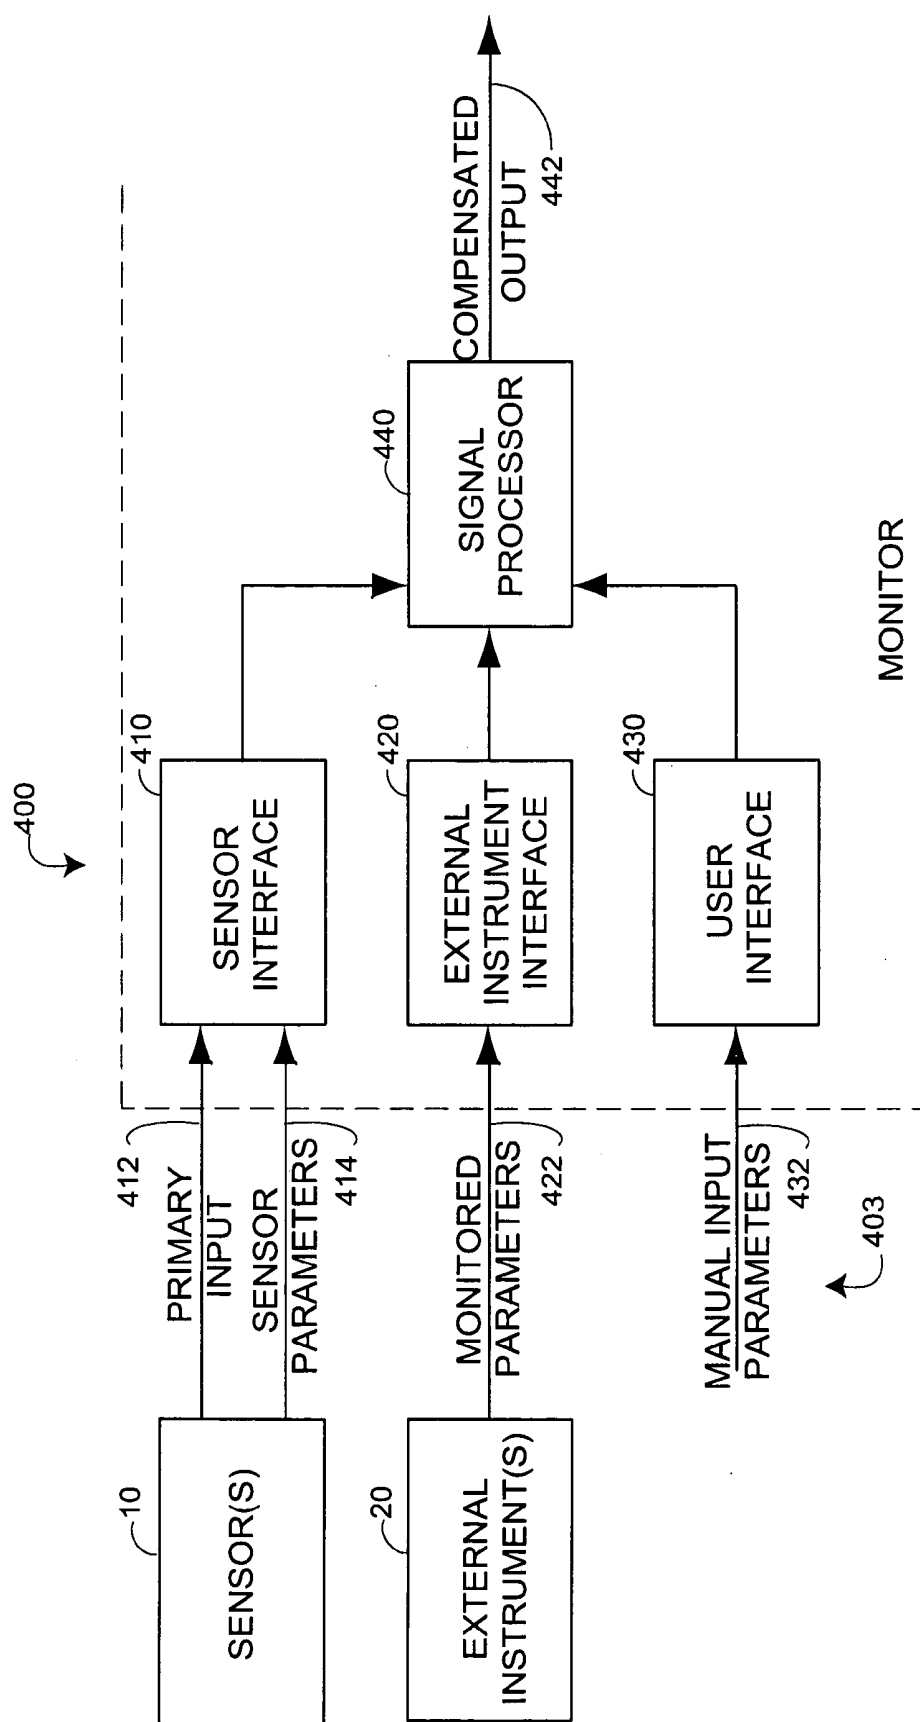


FIG. 4

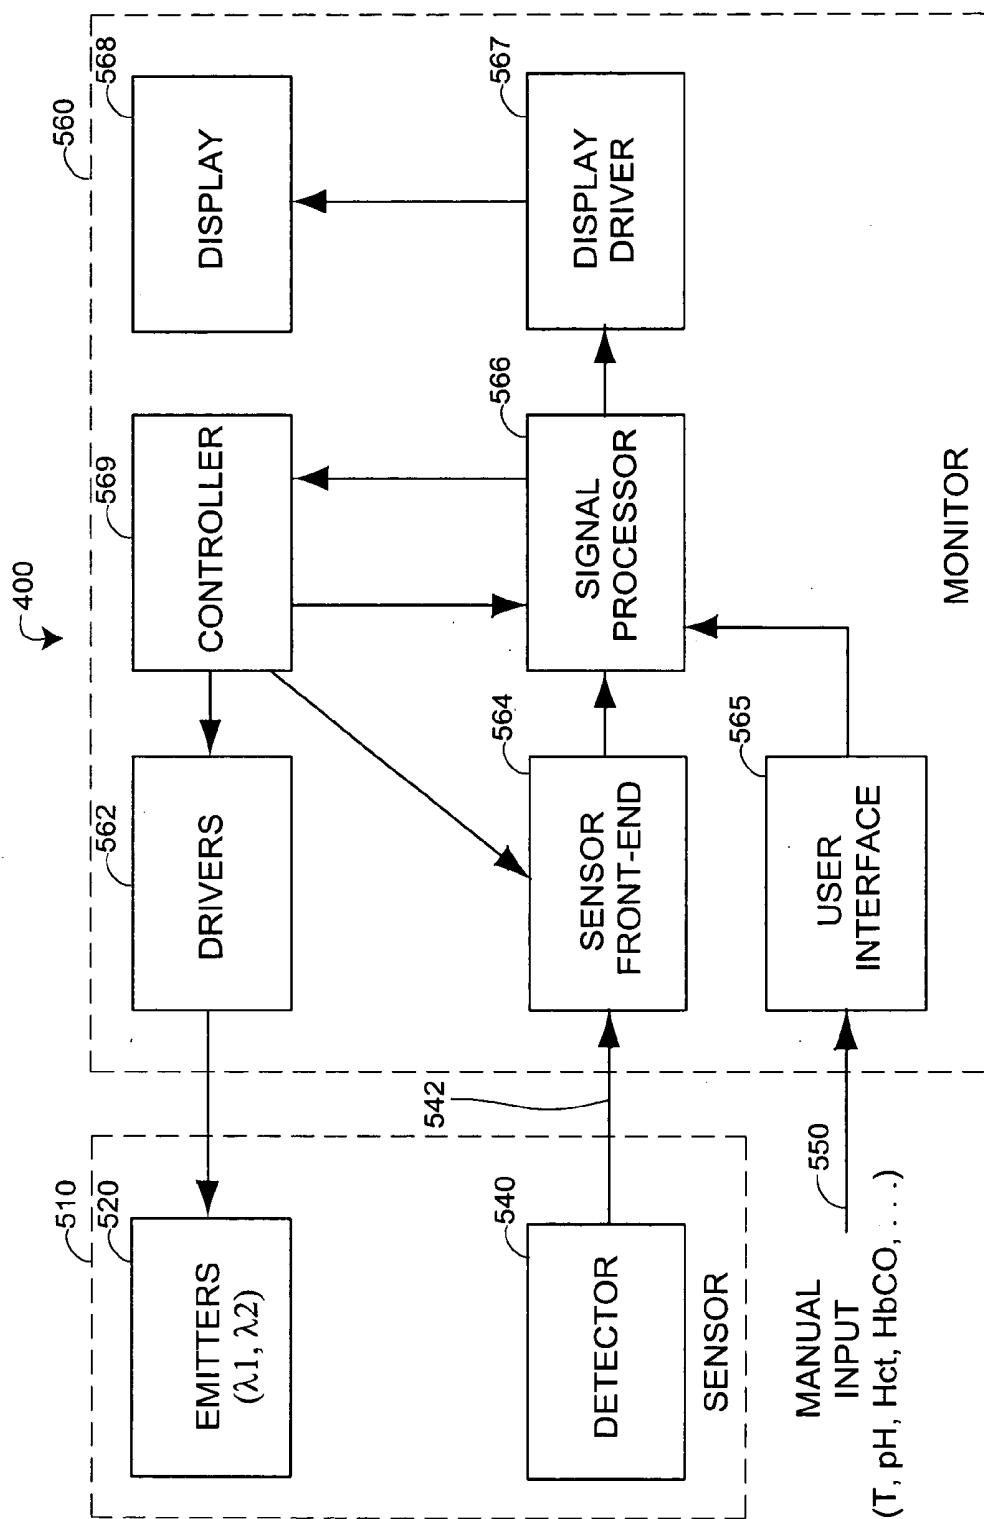


FIG. 5

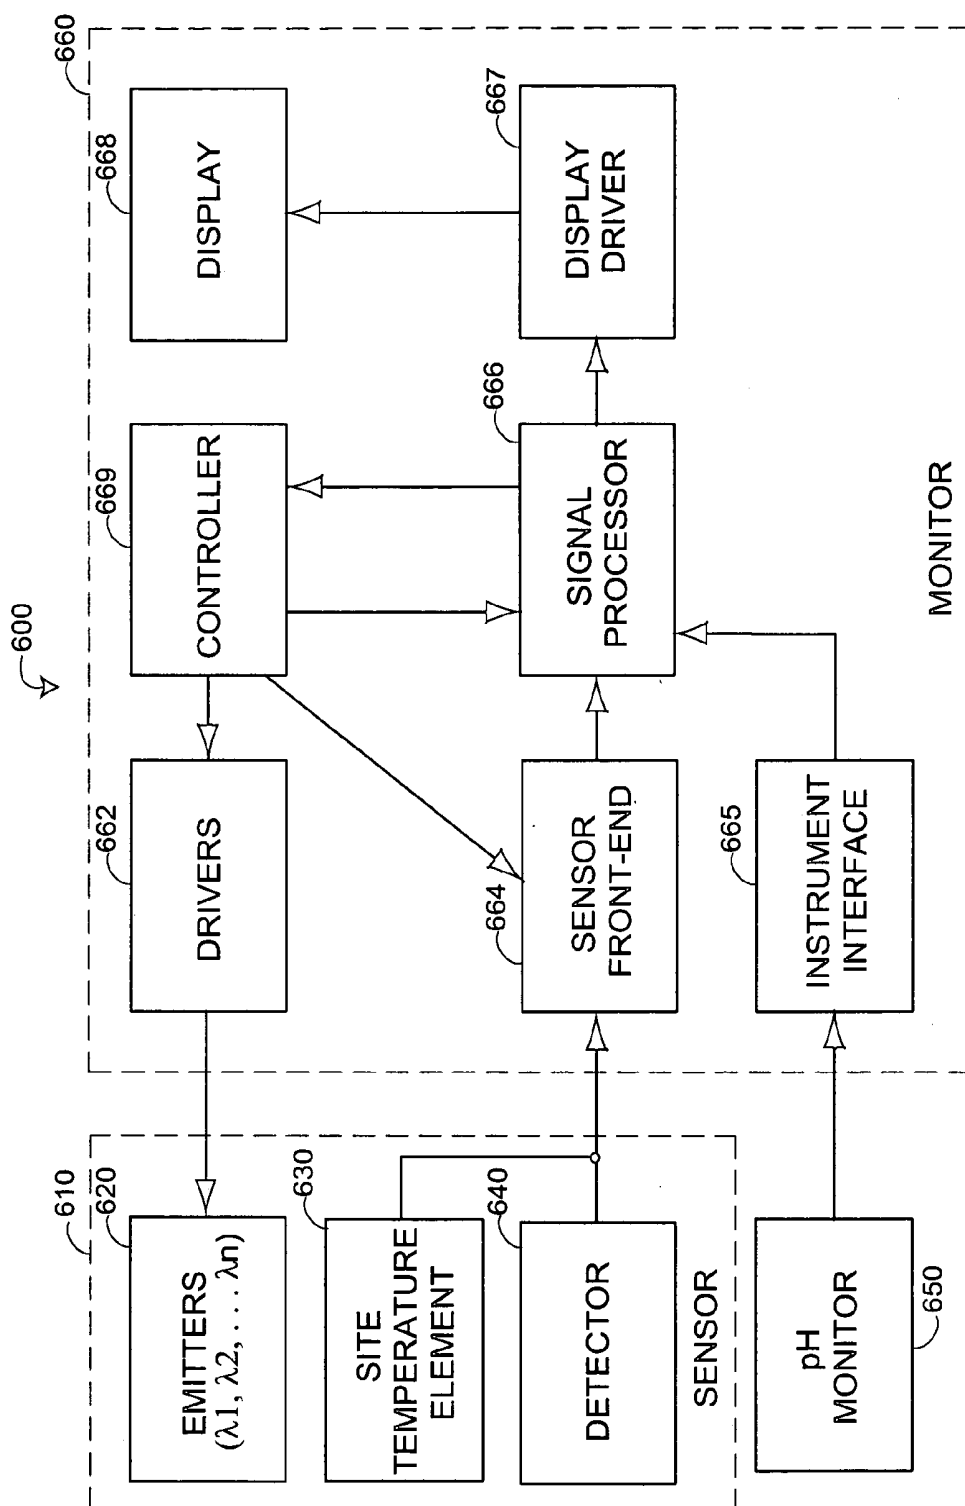


FIG. 6

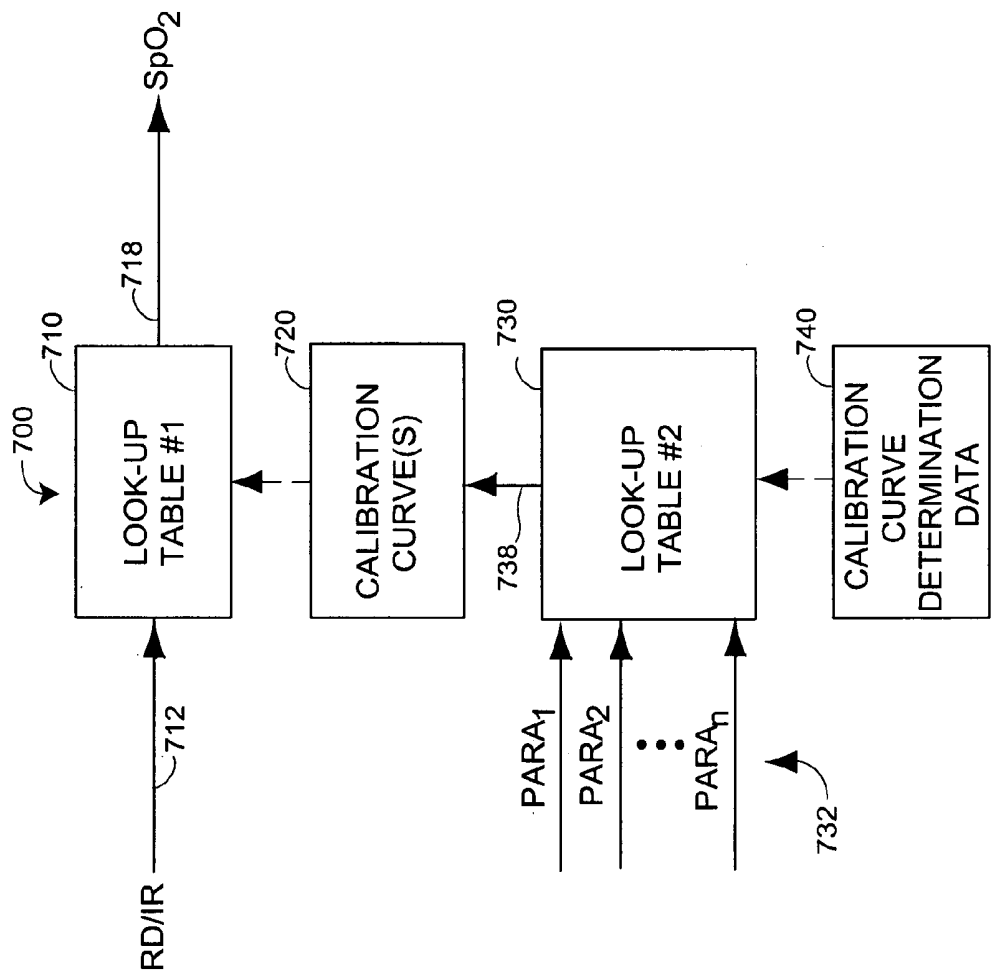


FIG. 7

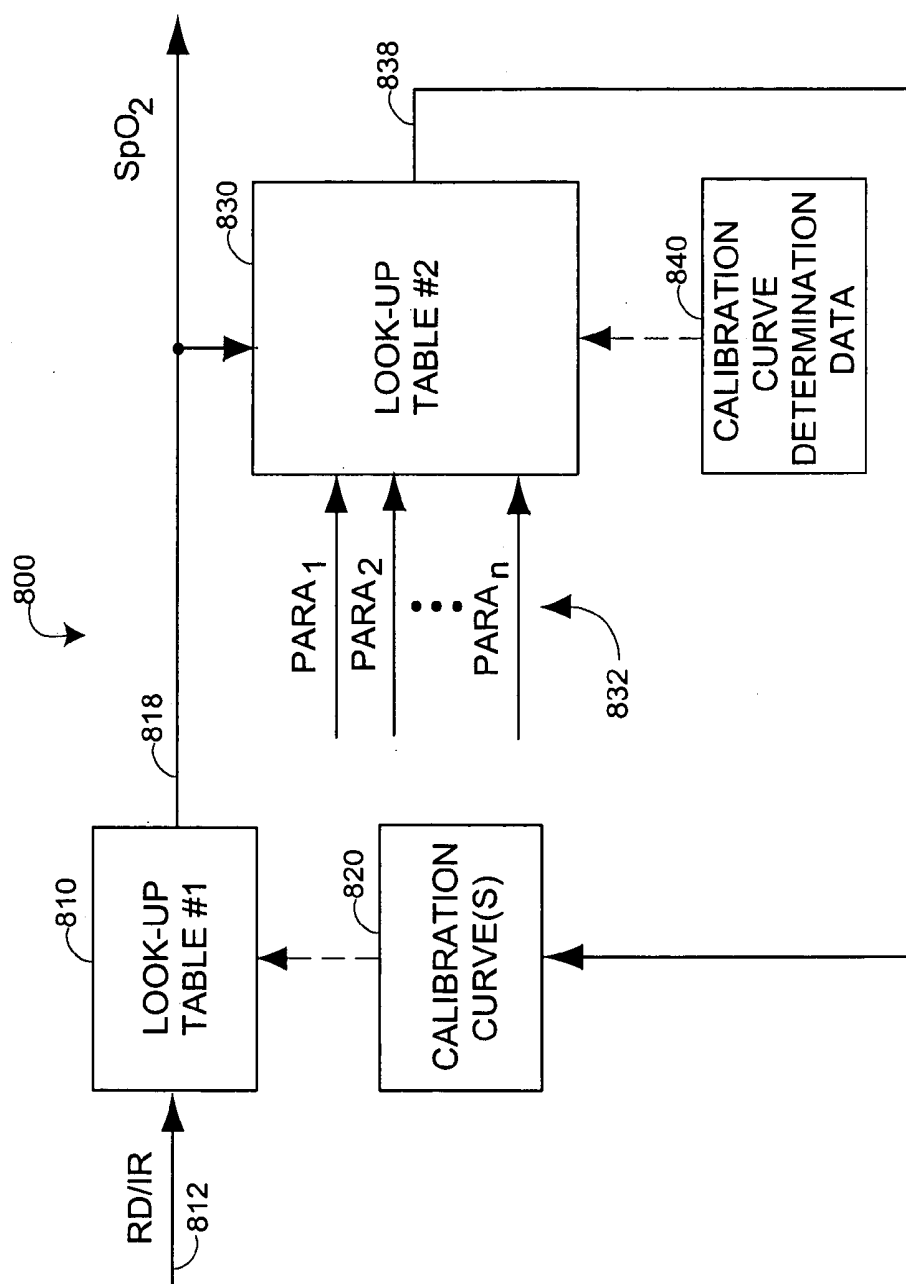


FIG. 8

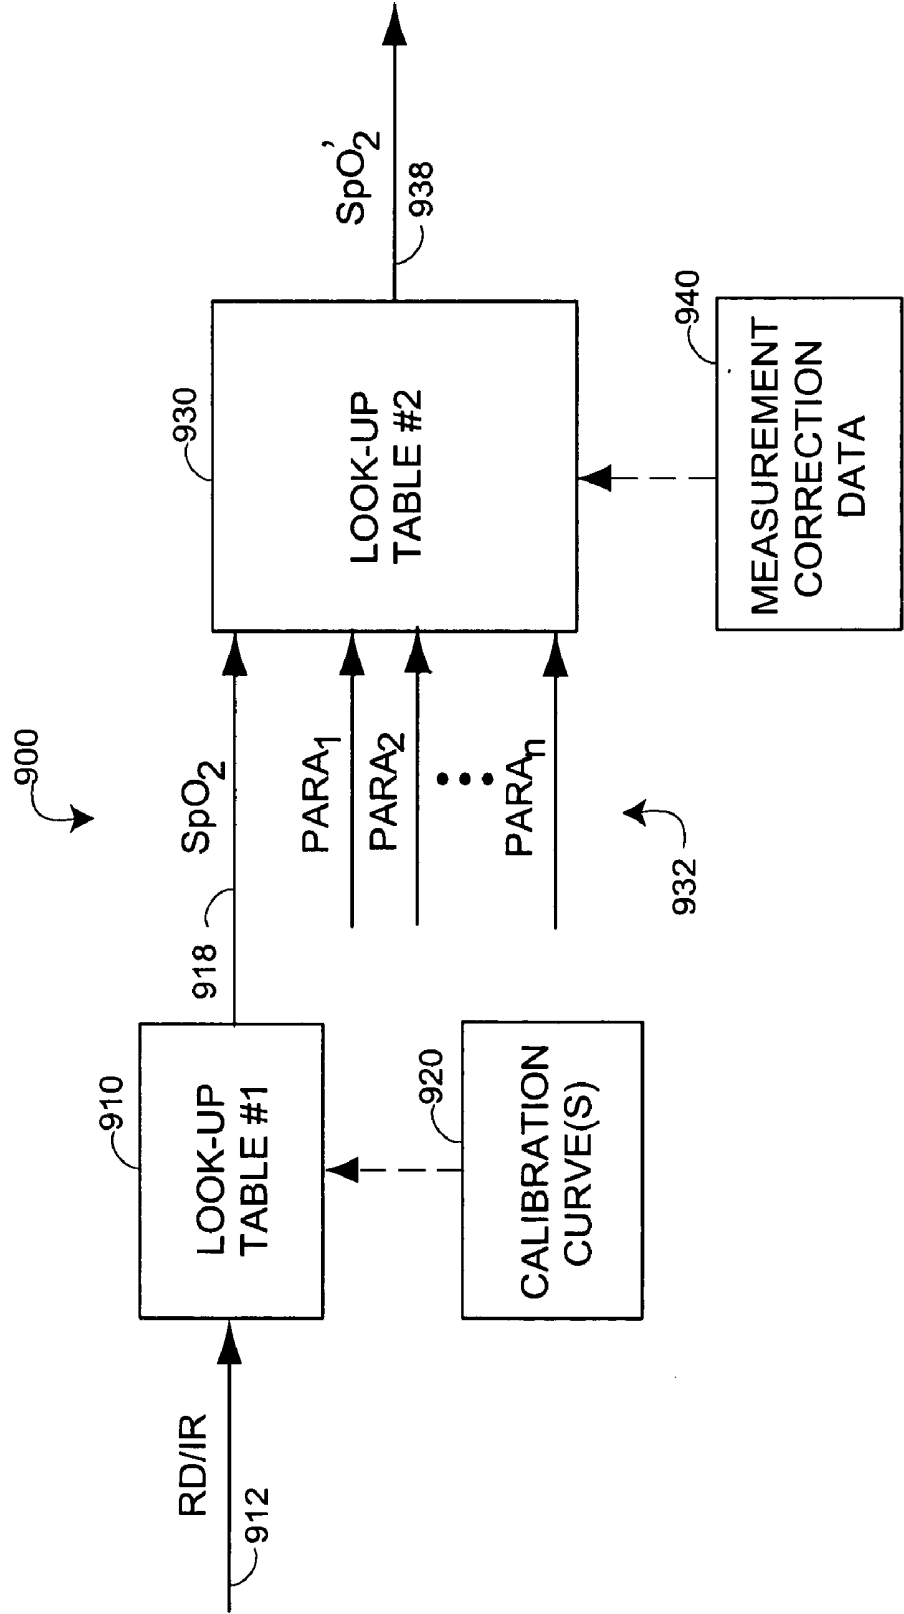


FIG. 9

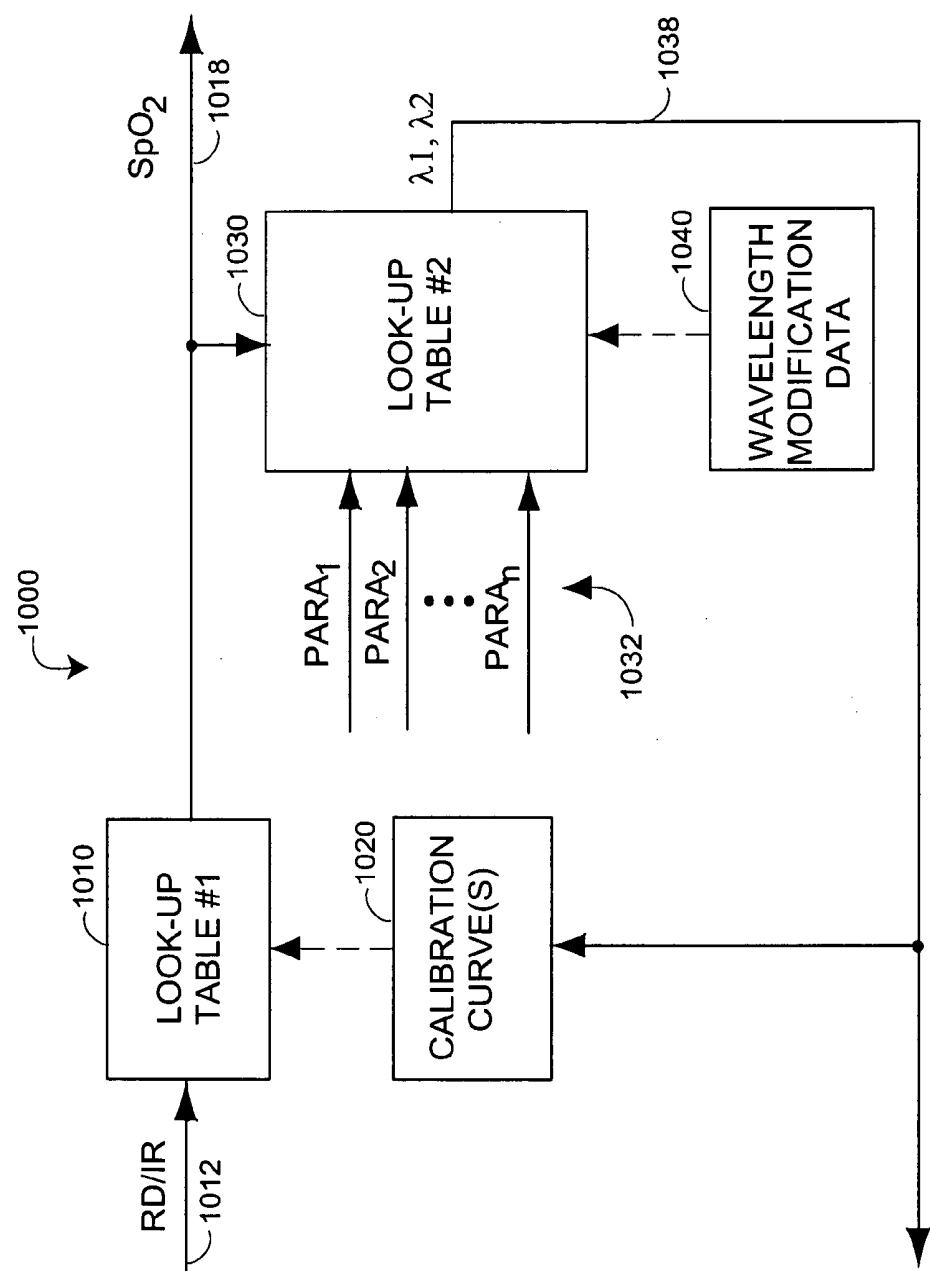


FIG. 10

PARAMETER COMPENSATED PULSE OXIMETER

[0006]

REFERENCE TO RELATED APPLICATIONS

[0001] The present application claims priority benefit under 35 U.S.C. §119(e) from U.S. Provisional Application No. 60/413,494, filed Sep. 25, 2002, entitled "Parameter Compensated Pulse Oximeter," which is incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] Pulse oximetry is a noninvasive, easy to use, inexpensive procedure for measuring the oxygen saturation level of arterial blood. Pulse oximeters perform a spectral analysis of the pulsatile component of arterial blood in order to determine the relative concentration of oxygenated hemoglobin, the major oxygen carrying constituent of blood, and deoxygenated (depleted) hemoglobin. These instruments have gained rapid acceptance in a wide variety of medical applications, including surgical wards, intensive care units, general wards and home care by providing early detection of decreases in the arterial oxygen supply, which reduces the risk of accidental death and injury.

[0003] FIG. 1 illustrates a pulse oximetry system 100 having a sensor 110 and a monitor 150. The sensor 110 has emitters 120 and a detector 130. The emitters 120 typically consist of a red LED (light emitting diode) and an infrared LED that project light through blood vessels and capillaries underneath a tissue site, such as a fingernail bed. The detector 130 is typically a photodiode positioned opposite the LEDs so as to detect the emitted light as it emerges from the tissue site. A pulse oximetry sensor is described in U.S. Pat. No. 6,088,607 entitled "Low Noise Optical Probe," which is assigned to Masimo Corporation, Irvine, Calif. and incorporated by reference herein.

[0004] Also shown in FIG. 1, the monitor 150 has drivers 152, a sensor front-end 154, a signal processor 155, a display driver 157, a display 158 and a controller 159. The drivers 152 alternately activate the emitters 120 as determined by the controller 159. The front-end 154 conditions and digitizes the resulting current generated by the detector 130, which is proportional to the intensity of the detected light. The signal processor 155 inputs the conditioned detector signal and determines oxygen saturation based upon the differential absorption by arterial blood of the two wavelengths projected by the emitters 120. Specifically, a ratio of detected red and infrared intensities is calculated by the signal processor 155, and an arterial oxygen saturation value is empirically determined based on the ratio obtained, as described with respect to FIGS. 2-3, below. The display driver 157 and associated display 158 indicate a patient's oxygen saturation along with pulse rate.

[0005] The Beer-Lambert law provides a simple model that describes a tissue site response to pulse oximetry measurements. The Beer-Lambert law states that the concentration c_i of an absorbent in solution can be determined by the intensity of light transmitted through the solution, knowing the pathlength d_λ , the intensity of the incident light $I_{0,\lambda}$, and the extinction coefficient $\epsilon_{i,\lambda}$ at a particular wavelength λ . In generalized form, the Beer-Lambert law is expressed as:

$$I = I_{0,\lambda} e^{-d_\lambda / \mu_{a,\lambda}} \quad (1)$$

$$\mu_{a,\lambda} = \sum_{i=1}^n \epsilon_{i,\lambda} \cdot c_i \quad (2)$$

[0007] where $\mu_{a,\lambda}$ is the bulk absorption coefficient and represents the probability of absorption per unit length. The Beer-Lambert law assumes photon scattering in the solution is negligible. The minimum number of discrete wavelengths that are required to solve EQS. 1-2 are the number of significant absorbers that are present in the solution.

[0008] FIG. 2 illustrates top-level computation functions for the signal processor 155 (FIG. 1), described above. For pulse oximetry, it is assumed that wavelengths are chosen such that there are only two significant absorbers, which are oxygenated hemoglobin (HbO₂) and deoxygenated hemoglobin (Hb). In particular, pulse oximetry measurements are conventionally made at a red wavelength corresponding to 660 nm and an infrared wavelength corresponding to 940 nm. At these wavelengths, deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin.

[0009] In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site also comprises skin, muscle, bone, venous blood, fat, pigment, etc., each of which absorbs light. It is assumed that the background absorption due to these surrounding tissues is invariant and can be ignored. That is, the sensor signal generated by the pulse-added arterial blood is isolated from the signal generated by other layers including tissue, venous blood and baseline arterial blood.

[0010] As shown in FIG. 2, to isolate the pulsatile arterial blood, the signal processor 155 (FIG. 1) computes ratios 215, 265 of the AC portions 212, 262 of the detected red (RD) 201 and infrared (IR) 206 signals with respect to the DC portions 214, 264 of the detected signals 201, 206. Computations of these AC/DC ratios 215, 265 provide relative absorption measures that compensate for variations in both incident light intensity and background absorption and, hence, are responsive only to the hemoglobin in the arterial blood. Further, a ratio of the normalized absorption at the red wavelength over the normalized absorption at the infrared wavelength is computed:

$$RD/IR = (Red_{AC}/Red_{DC}) / (IR_{AC}/IR_{DC}) \quad (3)$$

[0011] The desired oxygen saturation (SpO₂) 282 is then computed empirically from this "red-over-infrared, ratio-of-ratios" (RD/IR) 272. That is, the RD/IR output 272 is input to a look-up table 280 containing empirical data 290 relating RD/IR to SpO₂, as described with respect to FIG. 3, below.

[0012] FIG. 3 shows a graph 300 depicting the relationship between RD/IR and SpO₂. This relationship can be approximated from Beer-Lambert's Law, described above. However, it is most accurately determined by statistical

regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. The result can be depicted as a curve **310**, with measured values of RD/IR shown on a x-axis **302** and corresponding saturation values shown on a y-axis **301**. In a pulse oximeter device, this empirical relationship can be stored in a read-only memory (ROM) for use as a look-up table **280** (**FIG. 2**) so that SpO₂ can be directly read-out from an input RD/IR measurement. For example, an RD/IR value of 1.0 corresponding to a point **312** on the calibration curve **310** indicates a resulting SpO₂ value of approximately 85%.

SUMMARY OF THE INVENTION

[0013] Saturation measurements from a conventional pulse oximeter depend on a predictable, empirical correlation between RD/IR and SpO₂. Tissue optical properties, i.e. RD absorbance as compared with IR absorbance, however, vary with other patient dependent parameters such as site temperature, pH and total hematocrit (Hct), to name a few, that are not accounted for in the conventional photon absorbance model. A compensated pulse oximeter advantageously utilizes measurements of one or more parameters that are missing from a conventional pulse oximeter to derive a more accurate SpO₂ measurement. Parameter measurements may be derived from multiple parameter sensors, from additional sensors and/or instruments and from manual inputs. A compensated pulse oximeter accounts for these parameters by calibration curve selection, modification or derivation, by measurement output corrections and by dynamic sensor wavelength modification.

BRIEF DESCRIPTION OF THE DRAWINGS

[0014] **FIG. 1** is a block diagram of a prior art pulse oximeter;

[0015] **FIG. 2** is a top-level functional diagram of conventional pulse oximetry signal processing;

[0016] **FIG. 3** is an exemplar graph of a conventional calibration curve;

[0017] **FIG. 4** is a top-level block diagram of a parameter compensated pulse oximeter portion having sensor, external instrument and manual parameter inputs;

[0018] **FIG. 5** is a detailed block diagram of a pulse oximeter having manual parameter inputs;

[0019] **FIG. 6** is a detailed block diagram of a pulse oximeter having a multi-wavelength and site temperature sensor in addition to an external pH monitor input;

[0020] **FIG. 7** is a functional block diagram of parameter compensated signal processing incorporating one embodiment of calibration curve determination;

[0021] **FIG. 8** is a functional block diagram of parameter compensated signal processing incorporating another embodiment of calibration curve determination;

[0022] **FIG. 9** is a functional block diagram of parameter compensated signal processing incorporating measurement output correction; and

[0023] **FIG. 10** is functional block diagram of parameter compensated signal processing incorporating sensor wavelength modification.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0024] Overview

[0025] Parameter compensated pulse oximetry is described below with respect to monitor interface architectures (**FIGS. 4-6**) and monitor signal processing functions (**FIGS. 7-10**). **FIG. 4** illustrates a general interface architecture including a primary sensor input for deriving SpO₂ and parameter inputs from sensors, external instruments and manual entry for deriving a more accurate SpO₂. **FIG. 5** illustrates a two-wavelength sensor along with manual parameter inputs. **FIG. 6** illustrates a multiple wavelength sensor for a derived parameter input, a sensor temperature element for a site temperature parameter input, and an external instrument parameter input.

[0026] **FIGS. 7-8** illustrate a compensated SpO₂ computed from RD/IR utilizing a parameter determined calibration curve. **FIG. 9** illustrates a compensated SpO₂ computed from parameter dependent correction of an uncompensated SpO₂. **FIG. 10** illustrates a compensated SpO₂ resulting from parameter dependent sensor wavelength modification.

[0027] The interface architectures according to **FIGS. 4-6** may each support signal processing functions according to **FIGS. 7-10**. As just one of many examples and embodiments, a pulse oximeter has a manual input compensation parameter, such as described with respect to **FIG. 5**. The manual input may be, say, a blood gas derived parameter, such as HbCO or MetHb to name just a few. This parameter is utilized to select, modify, derive or otherwise determine a calibration curve so as to compute a more accurate measure of SpO₂.

[0028] Parameter Compensation Architecture

[0029] **FIG. 4** illustrates a parameter compensated pulse oximeter **400** having a sensor interface **410**, an external instrument interface **420** and a user interface **430**. The sensor interface **410** connects to one or more tissue site sensors **10**, which may be optical or non-optical devices configured to provide invasive or noninvasive measurements of tissue site properties. The sensor interface **410** has a primary input **412** and one or more sensor parameter inputs **414**. The primary input **412** is adapted to provide tissue site properties via sensor elements. A sensor parameter input **414** is also adapted to provide tissue site related properties, which include optical or nonoptical properties. In one embodiment, the primary input **412** is a detector response to at least two emitter wavelengths after transmission through or reflection from a tissue site, from which the pulse oximeter may derive at least a conventional measure of oxygen saturation, as described with respect to **FIGS. 1-3** above. An example of this embodiment is described with respect to **FIG. 5**, below. In another embodiment, the sensor **10** utilizes more than two wavelengths so that the pulse oximeter **400** may derive the concentrations of other blood constituents in addition to oxygen saturation, such as total hematocrit (Hct), carboxy-hemoglobin (HbCO) and methemoglobin (MetHb), to name a few. An example of this is described with respect to **FIG. 6**, below. The same sensor or a different sensor provides a measure of tissue site temperature on a sensor parameter input **414**, such as described with respect to **FIG. 6**, below.

[0030] Also shown in **FIG. 4**, an external instrument interface **620** connects to one or more external instruments

20, which may monitor optical or non-optical properties, invasively or noninvasively, from the sensor tissue site or from other portions of a patient or a patient's immediate environment. In one embodiment, the external instrument 20 is a pH monitor, as described with respect to FIG. 6, below.

[0031] Further shown in FIG. 4, a user interface 430 accepts one or more manual input parameters 432. As an example, the user interface 430 may be a keyboard input operating in conjunction with a user display, which may range from a small character display to a CRT providing a computer-generated graphical user interface (GUI). The manual inputs may be any information related to a patient or a patient's immediate environment. In one embodiment, a manual input of blood gas measurements, such as are obtainable from a CO-oximeter, is provided. Blood gas measurements may include arterial oxygen saturation (SaO_2), Hct, HbCO, MetHb to name a few.

[0032] Additionally shown in FIG. 4, the sensor interface 410, external instrument interface 420 and user interface 430 each provide inputs to the signal processor 440. The signal processor utilizes the primary input 412 and one or more parameter inputs 403 to generate a compensated output 442. In one embodiment, the output 442 is an SpO_2 measurement that is derived from both the primary input 412 and the parameter inputs 403.

[0033] FIG. 5 illustrates one embodiment of a parameter compensated pulse oximeter 500 having a sensor 510 and manual inputs to a monitor 560. In particular, drivers 562 activate emitters 520 that project two wavelengths into a tissue site, and a detector 540 responsive to the emitters 520 provides a primary input 542 to a sensor front-end 564, as described above. A user interface 565 accepts manual inputs such as temperature (T), pH, Hct, HbCO and MetHb to name a few, the values of which a user may obtain from separate instruments. The sensor front-end 564 and user interface 565 output to the signal processor 566 a detector signal along with the manually input parameters. The signal processor 566 computes a compensated SpO_2 measurement from the detector signal and these parameters, as described with respect to FIGS. 7-10, below. The compensated SpO_2 measurement is then displayed 567, 568 in a manner similar to that described above with respect to FIG. 1.

[0034] FIG. 6 illustrates another embodiment of a parameter compensated pulse oximeter 600 having a sensor 610 and an external pH monitor 650 providing inputs to a pulse oximetry monitor 660. The sensor 610 has multiple wavelength emitters 620 and a site temperature element 630. Multiple wavelengths may be achieved, for example, by utilizing multiple LEDs each manufactured for a specific wavelength according to the number of wavelengths desired. Alternatively, one or more LEDs having drive current dependent wavelengths may be utilized, where the drive current is controlled to shift between multiple wavelengths. The site temperature element 630 provides a site temperature parameter input to the sensor front-end 664. In one embodiment, the site temperature element 630 is a thermistor located on the sensor 610 proximate the emitters 620 or proximate the detector 640. The detector 640 provides a multiple wavelength signal output that is combined with a site temperature output to a sensor front-end 664. An instrument interface 665 is adapted to input pH readings from the pH monitor 650. The sensor drivers 662 provide multiplexed

activation of the multiple emitters 620 as determined by the controller 669. The signal processor 666 accepts outputs from the sensor front-end 664 and the instrument interface 665. In addition, the signal processor 666 computes an SpO_2 measurement from the detector signal along with other blood constituents, utilizing the multiple wavelength signal from the detector 640. Further, the signal processor 666 derives a compensated SpO_2 measurement from the input parameters, as described with respect to FIGS. 7-10, below. The compensated SpO_2 measurement is then displayed 667, 668 in a manner similar to that described above.

[0035] As shown in FIG. 6, a pulse oximetry sensor 610 may be improved for use in conjunction with a parameter compensated pulse oximeter by increasing the number of wavelengths projected by the emitters 620, which allows the resolution of more than two blood constituents, as described above. Further, the sensor 610 may be improved by adding the capability to measure various parameters, such as site temperature. Alternatively, as shown in FIG. 5, pulse oximeter performance can be improved at reduced costs by utilizing simple sensors in conjunction with other instrumentation and/or manual inputs to provide additional input parameters.

[0036] The sensor 610 may also have an information element (not shown) that describes information regarding the sensor. In one embodiment, the information element provides the monitor 660 with information regarding available wavelengths for the emitters 620 and/or information regarding the temperature element 630, such as the resistance-temperature characteristics of a thermistor. An information element is described in U.S. Pat. No. 6,011,986 entitled "Manual And Automatic Probe Calibration," assigned to Masimo Corporation, Irvine, Calif. and incorporated by referenced herein.

[0037] Parameter Compensation Signal Processing

[0038] FIG. 7 illustrates a calibration curve determination function 700 having a first look-up table 710, an associated calibration curve or curves 720, a second look-up table 730 and a calibration curve determination data set 740. The calibration curve determination function 700 advantageously selects, modifies, derives or otherwise determines a calibration curve 720 so as to generate a compensated SpO_2 output 718. The first look-up table 710 has an RD/IR input 712 and generates a SpO_2 output 718 utilizing a calibration curve 720, such as described with respect to FIGS. 2-3, above. The second look-up table 730 has one or more compensation parameter inputs 732, such as temperature, pH, Hct, HbCO and MetHb to name a few, and provides a calibration curve control output 738 according to calibration curve determination data 740. The control output 738 determines the calibration curve 720 utilized by the first look-up table 710, according to the compensation parameters 732. In one embodiment, the control output 738 selects one of a family of calibration curves 720. In another embodiment, the control output 738 determines the direction and amount of shift in a calibration curve 720 or a selected one of a family of calibration curves 720. In yet another embodiment, the control output 738 modifies a calibration curve or a selected one of a family of calibration curves 720, such as by rotating a calibration curve around a selected point on the curve. In an additional embodiment, the control output 738 specifies one or more points from which a calibration curve 720 is

derived. The calibration curves **720** and calibration curve determination data **740** define a relationship between the primary input **712**, the parameter inputs **732** and the compensated output **718**. The calibration curve or curves **720** and associated curve determination data **740** may be determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation and associated parameters. All or part of the first look-up table **710**, calibration curves **720**, second look-up table **730** and calibration curve determination data set **740** may be replaced by or combined with a mathematical formula or algorithm, theoretically or experimentally derived, that derives a calibration curve or curves or directly computes an SpO_2 output from RD/IR and parameter inputs.

[0039] FIG. 8 illustrates a calibration curve determination function **800** having a first look-up table **810**, a calibration curve or curves **820**, a second look-up table **830** and associated calibration curve modification data **840**. The calibration curve determination function **800** functions as described with respect to FIG. 7, but has, as input to the second look-up table **830**, the compensated SpO_2 output **818**. In particular, the first look-up table **810** has an RD/IR input **812** and generates a SpO_2 output **818** utilizing a calibration curve **820**. The second look-up table **830** has one or more compensation parameter inputs **832** and has, as an input, the SpO_2 output **818**. The second look-up table **830** provides a calibration curve control output **838** according to calibration curve determination data **840**. The control output **838** determines the calibration curve **820** utilized by the first look-up table **810**, according to the compensation parameters **832** and the SpO_2 output **818**. As described above with respect to FIG. 7, the control output **838** may select one of a family of calibration curves **820**, may determine the direction and amount of shift in a calibration curve **820** or a selected one of a family of calibration curves **820**, may modify a calibration curve or a selected one of a family of calibration curves **820**, such as by rotating a calibration curve around a selected point on the curve, or may specify one or more points from which a calibration curve **820** is derived or may cause a combination of these actions. The calibration curve or curves **820** and associated curve determination data **840** may be determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation and associated parameters.

[0040] In one advantageous embodiment, there is a single parameter input **832** comprising one or more blood gas measurements of SaO_2 . According to these SaO_2 measurements, a calibration curve **820** is selected, modified, such as by shifting or rotating a calibration curve, or otherwise derived so that subsequently derived SpO_2 measurements are consistent with blood gas measurements. In a particular embodiment, so as to reduce sensitivity, multiple blood gas input values are taken over a range of saturation values and are evaluated for consistency within a tolerance range before the current calibration curve is replaced or modified.

[0041] FIG. 9 illustrates a parameter compensation function **900** for an uncompensated SpO_2 measurement having a first look-up table **910**, a calibration curve or curves **920**, a second look-up table **930** and associated correction data **940**. The parameter compensation function **900** differs from the calibration determination function **700** (FIG. 7) described

above in that, as shown in FIG. 9, an uncompensated SpO_2 value **918** is calculated and corrected to yield a compensated SpO_2 value **938**. This contrasts with a compensated SpO_2 value being directly derived from RD/IR, as described with respect to FIG. 7, above. In one embodiment, the parameter compensation function **900** advantageously upgrades the results of a conventional pulse oximeter. The first look-up table **910** and calibration curve **920** may be as described with respect to FIGS. 2-3, above. The second look-up table **930** and associated correction data **940** may be as described with respect to FIG. 7, above, except that an uncompensated value of SpO_2 **918** is an input to the look-up table **930** rather than RD/IR **912**. As above, the correction data set **940** may be determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation and associated parameters or may be replaced by or combined with a mathematical formula or algorithm that directly computes a compensated SpO_2 output from uncompensated SpO_2 and parameter inputs.

[0042] In one advantageous embodiment, a blood gas measurement of HbCO and/or MetHb is manually entered into a pulse oximeter and utilized to generate a compensated value of SpO_2 . As described above, conventional pulse oximetry utilizes two wavelengths, assuming that Hb and HbO_2 are the only significant absorbers. However, carboxy-hemoglobin (HbCO) and methemoglobin (MetHb) may also be significant absorbers at RD and IR wavelengths. The presence of significant concentrations of HbCO and MetHb have different effects on a conventional pulse oximeter estimate of oxygen saturation. HbO_2 and HbCO have similar extinctions at the RD wavelength, as do MetHb and Hb. At the IR wavelength, HbCO is relatively transparent whereas MetHb has greater extinction than the other hemoglobins. The two wavelength assumption has the effect of lumping HbO_2 and HbCO together, i.e. HbCO is counted as an oxygen carrying form of hemoglobin, causing a conventional pulse oximeter to overestimate oxygen saturation. As MetHb increases, RD/IR tends to unity and SpO_2 to a constant (e.g. 85%) regardless of oxygen saturation. A manually entered value of HbCO and/or MetHb is used as a parameter in conjunction with the functions described above with respect to any of FIGS. 7-9, so as to distinguish these hemoglobin species from HbO_2 and Hb, providing a more accurate, HbCO and/or MetHb compensated, value of SpO_2 .

[0043] FIG. 10 illustrates a wavelength modification function **1000** having a first look-up table **1010**, a calibration curve or curves **1020**, a second look-up table **1030** and associated wavelength modification data **1040**. The wavelength modification function **1000** advantageously changes sensor wavelength to generate a compensated SpO_2 output **1018**. The first look-up table **1010** has an RD/IR input **1012** and generates an SpO_2 output **1018** utilizing conventional calibration curves **1020**. The wavelength control output **1038** provides a calibration curve input for selecting a wavelength dependent calibration curve **1020**. The second look-up table **1030** has SpO_2 **1018** and parameter **1032** inputs and provides a sensor wavelength control output **1038** according to associated wavelength modification data **1040**. As above, the look-up tables may be replaced by or combined with mathematical formulas or algorithms. The wavelength control output **1038** is a feedback path to a controller **669** (FIG. 6) and/or drivers **662** (FIG. 6). In one advanta-

geous embodiment, there are no parameter inputs **1032**, and the wavelength control output **1038** is dependent on SpO_2 . In this manner, sensor wavelength can be dynamically adjusted based upon saturation levels, e.g. a first red and/or IR wavelength may be used in low saturation conditions and a second red and/or IR wavelength may be used in normal saturation conditions.

[0044] A parameter compensated pulse oximeter has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications.

What is claimed is:

1. A monitor comprising:

- a primary input responsive to a first property of a tissue site;
- an uncompensated measurement determinable from said primary input;
- a parameter input responsive to a second property associated with said tissue site, said first property being dependent upon said second property;
- a compensation relationship of said primary input, said parameter input and a compensated measurement; and
- a processor configured to output said compensated measurement from said primary input and said parameter input utilizing said compensation relationship, wherein

said compensated measurement more accurately represents said first property than said uncompensated measurement.

2. A monitoring method comprising the steps of:

determining a relationship between a first property of a tissue site, a second property associated with said tissue site and a compensated measurement of said tissue site;

reading a primary input responsive to said first property and a parameter input responsive to said second property; and

processing said primary input and said parameter input according to said relationship so as to output said compensated measurement.

3. A monitor comprising:

an first input means for determining a first property value associated with a tissue site;

a second input means for determining a second property value associated with a tissue site;

a compensation means for determining a relationship between compensated measurement values, first property values and second property values; and

a processor means for deriving a compensated measurement of said first property from said first input means, said second input means and said compensation means.

* * * * *

专利名称(译)	参数补偿脉搏血氧仪		
公开(公告)号	US20040122301A1	公开(公告)日	2004-06-24
申请号	US10/671179	申请日	2003-09-25
[标]申请(专利权)人(译)	Kiani曾MASSLé 戴铂MOHAMED AL ALI AMMAR WEBER WALTER中号		
申请(专利权)人(译)	Kiani曾MASSL E. 戴铂MOHAMED AL-ALI AMMAR WEBER WALTER M.		
当前申请(专利权)人(译)	摩根大通银行，NATIONAL ASSOCIATION		
[标]发明人	KIANI MASSL E DIAB MOHAMED AL ALI AMMAR WEBER WALTER M		
发明人	KIANI, MASSL E. DIAB, MOHAMED AL-ALI, AMMAR WEBER, WALTER M.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/01 A61B5/14551 A61B5/14535		
优先权	60/413494 2002-09-25 US		
其他公开文献	US7274955		
外部链接	Espacenet USPTO		

摘要(译)

监视器具有响应于组织部位的第一属性的主要输入。可以从主输入确定未补偿的测量。参数输入响应于与组织部位相关联的第二属性，其中第一属性取决于第二属性。监视器还具有主输入，参数输入和补偿测量的补偿关系。处理器被配置为利用补偿关系从主输入和参数输入输出补偿测量，其中补偿测量比未补偿测量更准确地表示第一属性。

