



US008498684B2

(12) **United States Patent**
Weber et al.

(10) **Patent No.:** **US 8,498,684 B2**
(45) **Date of Patent:** **Jul. 30, 2013**

(54) **SINE SATURATION TRANSFORM**

(75) Inventors: **Walter M. Weber**, Laguna Hills, CA (US); **Ammar Al-Ali**, San Juan Capistrano, CA (US); **Lorenzo Cazzoli**, Barcelona (ES)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 158 days.

(21) Appl. No.: **13/043,421**

(22) Filed: **Mar. 8, 2011**

(65) **Prior Publication Data**

US 2011/0160552 A1 Jun. 30, 2011

Related U.S. Application Data

(63) Continuation of application No. 12/336,419, filed on Dec. 16, 2008, now Pat. No. 7,904,132, which is a continuation of application No. 11/894,648, filed on Aug. 20, 2007, now Pat. No. 7,467,002, which is a continuation of application No. 11/417,914, filed on May 3, 2006, now Pat. No. 7,377,099, which is a continuation of application No. 11/048,232, filed on Feb. 1, 2005, now Pat. No. 7,373,194, which is a continuation of application No. 10/184,032, filed on Jun. 26, 2002, now Pat. No. 6,850,787.

(60) Provisional application No. 60/302,438, filed on Jun. 29, 2001.

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/024 (2006.01)

(52) **U.S. Cl.**
USPC **600/324; 600/323; 600/502; 702/190**

(58) **Field of Classification Search**

USPC 600/310, 322, 323, 324, 336, 500, 600/502; 702/189, 190
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,188,108 A	2/1993	Secker
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO	WO 98/42250	10/1998
WO	WO 02/47582 A3	6/2002

OTHER PUBLICATIONS

Office Action of Japanese Patent Application No. 2003-508244 dated Mar. 26, 2008 and English Translation of same in 35 pages.

(Continued)


Primary Examiner — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A transform for determining a physiological measurement is disclosed. The transform determines a basis function index from a physiological signal obtained through a physiological sensor. A basis function waveform is generated based on basis function index. The basis function waveform is then used to determine an optimized basis function waveform. The optimized basis function waveform is used to calculate a physiological measurement.

19 Claims, 14 Drawing Sheets

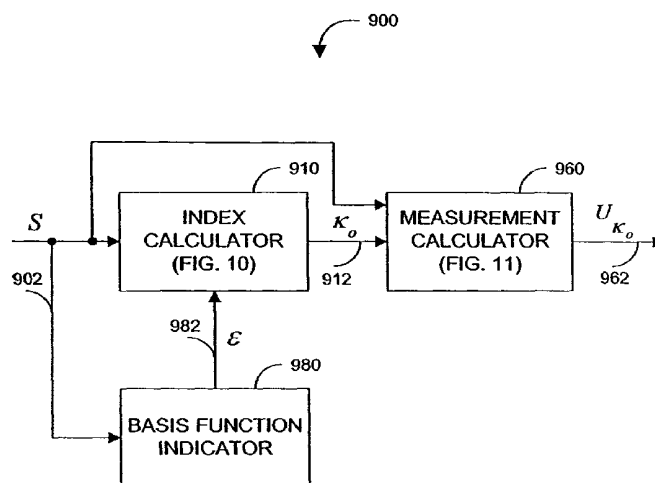



US008498684B2

(12) **United States Patent**
Weber et al.

(10) **Patent No.:** **US 8,498,684 B2**
(45) **Date of Patent:** **Jul. 30, 2013**

(54) **SINE SATURATION TRANSFORM**

(75) Inventors: **Walter M. Weber**, Laguna Hills, CA (US); **Ammar Al-Ali**, San Juan Capistrano, CA (US); **Lorenzo Cazzoli**, Barcelona (ES)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 158 days.

(21) Appl. No.: **13/043,421**

(22) Filed: **Mar. 8, 2011**

(65) **Prior Publication Data**

US 2011/0160552 A1 Jun. 30, 2011

Related U.S. Application Data

(63) Continuation of application No. 12/336,419, filed on Dec. 16, 2008, now Pat. No. 7,904,132, which is a continuation of application No. 11/894,648, filed on Aug. 20, 2007, now Pat. No. 7,467,002, which is a continuation of application No. 11/417,914, filed on May 3, 2006, now Pat. No. 7,377,099, which is a continuation of application No. 11/048,232, filed on Feb. 1, 2005, now Pat. No. 7,373,194, which is a continuation of application No. 10/184,032, filed on Jun. 26, 2002, now Pat. No. 6,850,787.

(60) Provisional application No. 60/302,438, filed on Jun. 29, 2001.

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/024 (2006.01)

(52) **U.S. Cl.**
USPC **600/324; 600/323; 600/502; 702/190**

(58) **Field of Classification Search**

USPC 600/310, 322, 323, 324, 336, 500, 600/502; 702/189, 190
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,188,108 A	2/1993	Secker
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.

(Continued)

FOREIGN PATENT DOCUMENTS

WO	WO 98/42250	10/1998
WO	WO 02/47582 A3	6/2002

OTHER PUBLICATIONS

Office Action of Japanese Patent Application No. 2003-508244 dated Mar. 26, 2008 and English Translation of same in 35 pages.

(Continued)


Primary Examiner — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A transform for determining a physiological measurement is disclosed. The transform determines a basis function index from a physiological signal obtained through a physiological sensor. A basis function waveform is generated based on basis function index. The basis function waveform is then used to determine an optimized basis function waveform. The optimized basis function waveform is used to calculate a physiological measurement.

19 Claims, 14 Drawing Sheets

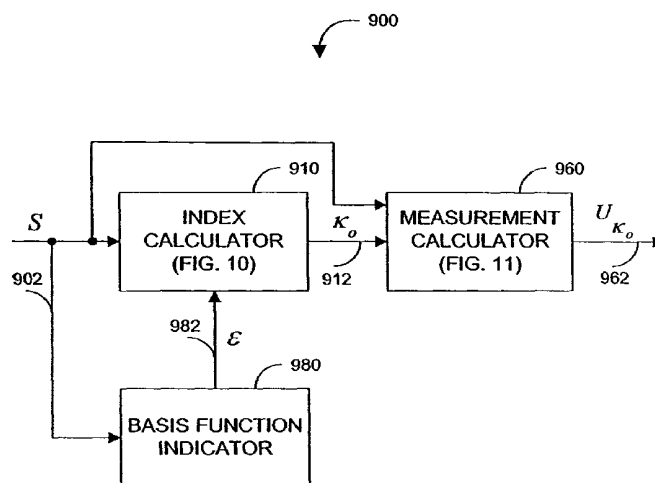

U.S. PATENT DOCUMENTS

D353,196 S	12/1994	Savage et al.	6,321,100 B1	11/2001	Parker
5,377,676 A	1/1995	Vari et al.	6,325,761 B1	12/2001	Jay
D359,546 S	6/1995	Savage et al.	6,334,065 B1	12/2001	Al-Ali et al.
5,431,170 A	7/1995	Mathews	6,343,224 B1	1/2002	Parker
D361,840 S	8/1995	Savage et al.	6,349,228 B1	2/2002	Kiani et al.
D362,063 S	9/1995	Savage et al.	6,360,114 B1	3/2002	Diab et al.
5,452,717 A	9/1995	Branigan et al.	6,368,283 B1	4/2002	Xu et al.
D363,120 S	10/1995	Savage et al.	6,371,921 B1	4/2002	Caro et al.
5,456,252 A	10/1995	Vari et al.	6,377,829 B1	4/2002	Al-Ali
5,479,934 A	1/1996	Imran	6,388,240 B2	5/2002	Schulz et al.
5,482,036 A	1/1996	Diab et al.	6,397,091 B2	5/2002	Diab et al.
5,490,505 A	2/1996	Diab et al.	6,430,437 B1	8/2002	Marro
5,494,043 A	2/1996	O'Sullivan et al.	6,430,525 B1	8/2002	Weber et al.
5,533,511 A	7/1996	Kaspari et al.	6,463,311 B1	10/2002	Diab
5,534,851 A	7/1996	Russek	6,470,199 B1	10/2002	Kopotic et al.
5,561,275 A	10/1996	Savage et al.	6,501,975 B2	12/2002	Diab et al.
5,562,002 A	10/1996	Lalin	6,505,059 B1	1/2003	Kollias et al.
5,590,649 A	1/1997	Caro et al.	6,515,273 B2	2/2003	Al-Ali
5,602,924 A	2/1997	Durand et al.	6,519,487 B1	2/2003	Parker
5,632,272 A	5/1997	Diab et al.	6,525,386 B1	2/2003	Mills et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	6,526,300 B1	2/2003	Kiani et al.
5,638,818 A	6/1997	Diab et al.	6,541,756 B2	4/2003	Schulz et al.
5,645,440 A	7/1997	Tobler et al.	6,542,764 B1	4/2003	Al-Ali et al.
5,685,299 A	11/1997	Diab et al.	6,580,086 B1	6/2003	Schulz et al.
D393,830 S	4/1998	Tobler et al.	6,584,336 B1	6/2003	Ali et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,595,316 B2	7/2003	Cybulski et al.
5,758,644 A	6/1998	Diab et al.	6,597,932 B2	7/2003	Tian et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,597,933 B2	7/2003	Kiani et al.
5,769,785 A	6/1998	Diab et al.	6,606,511 B1	8/2003	Ali et al.
5,782,757 A	7/1998	Diab et al.	6,632,181 B2	10/2003	Flaherty et al.
5,785,659 A	7/1998	Caro et al.	6,639,668 B1	10/2003	Trepagnier
5,791,347 A	8/1998	Flaherty et al.	6,640,116 B2	10/2003	Diab
5,810,734 A	9/1998	Caro et al.	6,643,530 B2	11/2003	Diab et al.
5,823,950 A	10/1998	Diab et al.	6,650,917 B2	11/2003	Diab et al.
5,830,131 A	11/1998	Caro et al.	6,654,624 B2	11/2003	Diab et al.
5,833,618 A	11/1998	Caro et al.	6,658,276 B2	12/2003	Kianl et al.
5,853,364 A	12/1998	Baker et al.	6,661,161 B1	12/2003	Lanzo et al.
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,671,531 B2	12/2003	Al-Ali et al.
5,890,929 A	4/1999	Mills et al.	6,678,543 B2	1/2004	Diab et al.
5,904,654 A	5/1999	Wohlmann et al.	6,684,090 B2	1/2004	Ali et al.
5,919,134 A	7/1999	Diab	6,684,091 B2	1/2004	Parker
5,934,925 A	8/1999	Tobler et al.	6,697,656 B1	2/2004	Al-Ali
5,940,182 A	8/1999	Lepper, Jr. et al.	6,697,657 B1	2/2004	Shehada et al.
5,995,855 A	11/1999	Kiani et al.	6,697,658 B2	2/2004	Al-Ali
5,997,343 A	12/1999	Mills et al.	RE38,476 E	3/2004	Diab et al.
6,002,952 A	12/1999	Diab et al.	6,699,194 B1	3/2004	Diab et al.
6,011,986 A	1/2000	Diab et al.	6,714,804 B2	3/2004	Al-Ali et al.
6,027,452 A	2/2000	Flaherty et al.	RE38,492 E	4/2004	Diab et al.
6,036,642 A	3/2000	Diab et al.	6,721,582 B2	4/2004	Trepagnier et al.
6,045,509 A	4/2000	Caro et al.	6,721,585 B1	4/2004	Parker
6,067,462 A	5/2000	Diab et al.	6,725,075 B2	4/2004	Al-Ali
6,081,735 A	6/2000	Diab et al.	6,728,560 B2	4/2004	Kollias et al.
6,083,172 A	7/2000	Baker, Jr. et al.	6,735,459 B2	5/2004	Parker
6,088,607 A	7/2000	Diab et al.	6,745,060 B2	6/2004	Diab et al.
6,110,522 A	8/2000	Lepper, Jr. et al.	6,760,607 B2	7/2004	Al-Ali
6,119,026 A	9/2000	McNulty et al.	6,770,028 B1	8/2004	Ali et al.
6,124,597 A	9/2000	Shehada	6,771,994 B2	8/2004	Kiani et al.
6,128,521 A	10/2000	Marro et al.	6,792,300 B1	9/2004	Diab et al.
6,129,675 A	10/2000	Jay	6,813,511 B2	11/2004	Diab et al.
6,144,868 A	11/2000	Parker	6,816,741 B2	11/2004	Diab
6,151,516 A	11/2000	Kiani-Azarbayjany et al.	6,822,564 B2	11/2004	Al-Ali
6,152,754 A	11/2000	Gerhardt et al.	6,826,419 B2	11/2004	Diab et al.
6,157,850 A	12/2000	Diab et al.	6,830,711 B2	12/2004	Mills et al.
6,165,005 A	12/2000	Mills et al.	6,850,787 B2	2/2005	Weber et al.
6,184,521 B1	2/2001	Coffin, IV et al.	6,850,788 B2	2/2005	Al-Ali
6,206,830 B1	3/2001	Diab et al.	6,852,083 B2	2/2005	Caro et al.
6,229,856 B1	5/2001	Diab et al.	6,861,639 B2	3/2005	Al-Ali
6,232,609 B1	5/2001	Snyder et al.	6,898,452 B2	5/2005	Al-Ali et al.
6,236,872 B1	5/2001	Diab et al.	6,920,345 B2	7/2005	Al-Ali et al.
6,241,683 B1	6/2001	Macklem et al.	6,931,268 B1	8/2005	Kiani-Azarbayjany et al.
6,253,097 B1	6/2001	Aronow et al.	6,934,570 B2	8/2005	Kiani et al.
6,256,523 B1	7/2001	Diab et al.	6,939,305 B2	9/2005	Flaherty et al.
6,263,222 B1	7/2001	Diab et al.	6,943,348 B1	9/2005	Coffin, IV
6,278,522 B1	8/2001	Lepper, Jr. et al.	6,950,687 B2	9/2005	Al-Ali
6,280,213 B1	8/2001	Tobler et al.	6,961,598 B2	11/2005	Diab
6,285,896 B1	9/2001	Tobler et al.	6,970,792 B1	11/2005	Diab
6,301,493 B1	10/2001	Marro et al.	6,979,812 B2	12/2005	Al-Ali
6,317,627 B1	11/2001	Ennen et al.	6,985,764 B2	1/2006	Mason et al.
			6,993,371 B2	1/2006	Kiani et al.

6,996,427 B2	2/2006	Ali et al.	7,467,002 B2	12/2008	Weber et al.
6,999,904 B2	2/2006	Weber et al.	7,469,157 B2	12/2008	Diab et al.
7,003,338 B2	2/2006	Weber et al.	7,471,969 B2	12/2008	Diab et al.
7,003,339 B2	2/2006	Diab et al.	7,471,971 B2	12/2008	Diab et al.
7,015,451 B2	3/2006	Dalke et al.	7,483,729 B2	1/2009	Al-Ali et al.
7,024,233 B2	4/2006	Ali et al.	7,483,730 B2	1/2009	Diab et al.
7,027,849 B2	4/2006	Al-Ali	7,489,958 B2	2/2009	Diab et al.
7,030,749 B2	4/2006	Al-Ali	7,496,391 B2	2/2009	Diab et al.
7,039,449 B2	5/2006	Al-Ali	7,496,393 B2	2/2009	Diab et al.
7,041,060 B2	5/2006	Flaherty et al.	D587,657 S	3/2009	Al-Ali et al.
7,044,918 B2	5/2006	Diab	7,499,741 B2	3/2009	Diab et al.
7,067,893 B2	6/2006	Mills et al.	7,499,835 B2	3/2009	Weber et al.
7,096,052 B2	8/2006	Mason et al.	7,500,950 B2	3/2009	Al-Ali et al.
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,509,154 B2	3/2009	Diab et al.
7,132,641 B2	11/2006	Schulz et al.	7,509,494 B2	3/2009	Al-Ali
7,142,901 B2	11/2006	Kiani et al.	7,510,849 B2	3/2009	Schurman et al.
7,149,561 B2	12/2006	Diab	7,526,328 B2	4/2009	Diab et al.
7,186,966 B2	3/2007	Al-Ali	7,530,942 B1	5/2009	Diab
7,190,261 B2	3/2007	Al-Ali	7,530,949 B2	5/2009	Al-Ali et al.
7,215,984 B2	5/2007	Diab	7,530,955 B2	5/2009	Diab et al.
7,215,986 B2	5/2007	Diab	7,563,110 B2	7/2009	Al-Ali et al.
7,221,971 B2	5/2007	Diab	7,596,398 B2	9/2009	Al-Ali et al.
7,225,006 B2	5/2007	Al-Ali et al.	7,618,375 B2	11/2009	Flaherty
7,225,007 B2	5/2007	Al-Ali	D606,659 S	12/2009	Kiani et al.
RE39,672 E	6/2007	Shehada et al.	7,647,083 B2	1/2010	Al-Ali et al.
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	D609,193 S	2/2010	Al-Ali et al.
7,245,953 B1	7/2007	Parker	D614,305 S	4/2010	Al-Ali et al.
7,254,429 B2	8/2007	Schurman et al.	RE41,317 E	5/2010	Parker
7,254,431 B2	8/2007	Al-Ali	7,729,733 B2	6/2010	Al-Ali et al.
7,254,433 B2	8/2007	Diab et al.	7,734,320 B2	6/2010	Al-Ali
7,254,434 B2	8/2007	Schulz et al.	7,761,127 B2	7/2010	Al-Ali et al.
7,272,425 B2	9/2007	Al-Ali	7,761,128 B2	7/2010	Al-Ali et al.
7,274,955 B2	9/2007	Kiani et al.	7,764,982 B2	7/2010	Dalke et al.
D554,263 S	10/2007	Al-Ali	D621,516 S	8/2010	Kiani et al.
7,280,858 B2	10/2007	Al-Ali et al.	7,791,155 B2	9/2010	Diab
7,289,835 B2	10/2007	Mansfield et al.	7,801,581 B2	9/2010	Diab
7,292,883 B2	11/2007	De Felice et al.	7,822,452 B2	10/2010	Schurman et al.
7,295,866 B2	11/2007	Al-Ali	RE41,912 E	11/2010	Parker
7,328,053 B1	2/2008	Diab et al.	7,844,313 B2	11/2010	Kiani et al.
7,332,784 B2	2/2008	Mills et al.	7,844,314 B2	11/2010	Al-Ali
7,340,287 B2	3/2008	Mason et al.	7,844,315 B2	11/2010	Al-Ali
7,341,559 B2	3/2008	Schulz et al.	7,865,222 B2	1/2011	Weber et al.
7,343,186 B2	3/2008	Lamego et al.	7,873,497 B2	1/2011	Weber et al.
D566,282 S	4/2008	Al-Ali et al.	7,880,606 B2	2/2011	Al-Ali
7,355,512 B1	4/2008	Al-Ali	7,880,626 B2	2/2011	Al-Ali et al.
7,356,365 B2	4/2008	Schurman	7,891,355 B2	2/2011	Al-Ali et al.
7,371,981 B2	5/2008	Abdul-Hafiz	7,894,868 B2	2/2011	Al-Ali et al.
7,373,193 B2	5/2008	Al-Ali et al.	7,899,507 B2	3/2011	Al-Ali et al.
7,373,194 B2	5/2008	Weber et al.	7,899,518 B2	3/2011	Trepagnier et al.
7,376,453 B1	5/2008	Diab et al.	7,904,132 B2	3/2011	Weber et al.
7,377,794 B2	5/2008	Al-Ali et al.			
7,377,899 B2	5/2008	Weber et al.			
7,383,070 B2	6/2008	Diab et al.			
7,415,297 B2	8/2008	Al-Ali et al.			
7,428,432 B2	9/2008	Ali et al.			
7,438,683 B2	10/2008	Al-Ali et al.			
7,440,787 B2	10/2008	Diab			
7,454,240 B2	11/2008	Diab et al.			

OTHER PUBLICATIONS

PCT International Search Report, App. No. PCT/US 02/20674, App. Dates: Jun. 28, 2002, 5 pages.

Smith, Steven W., "The Scientist and Engineer's Guide to Digital Signal Processing", Section 8, 1st Edition, 1997, California Technical Publishing.

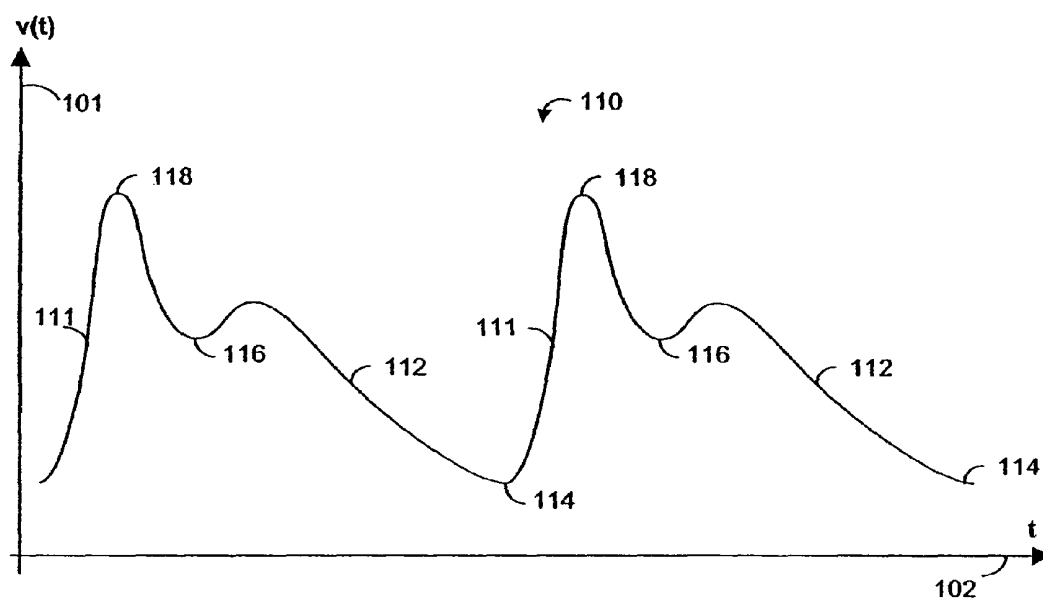


FIG. 1A

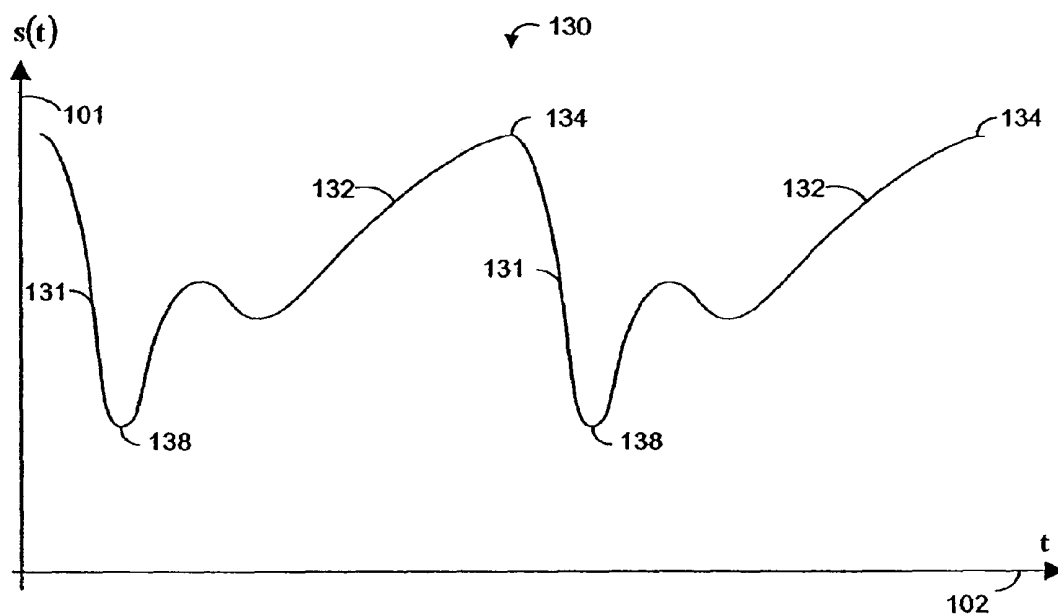


FIG. 1B

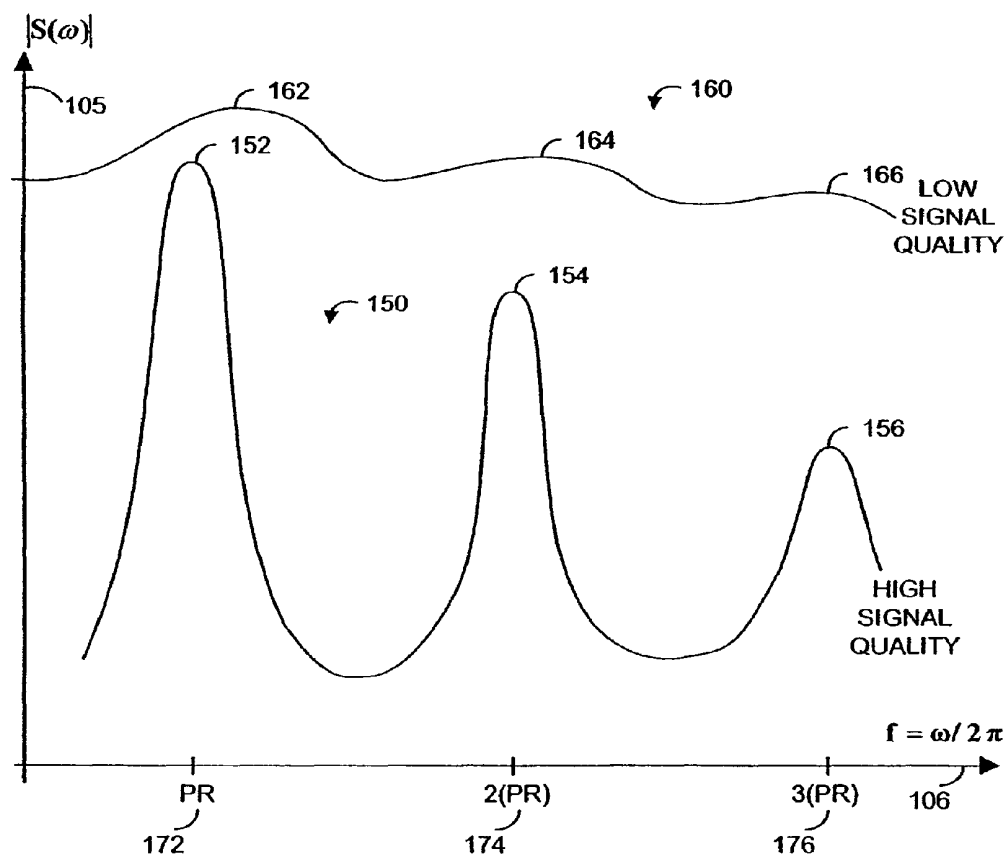


FIG. 1C

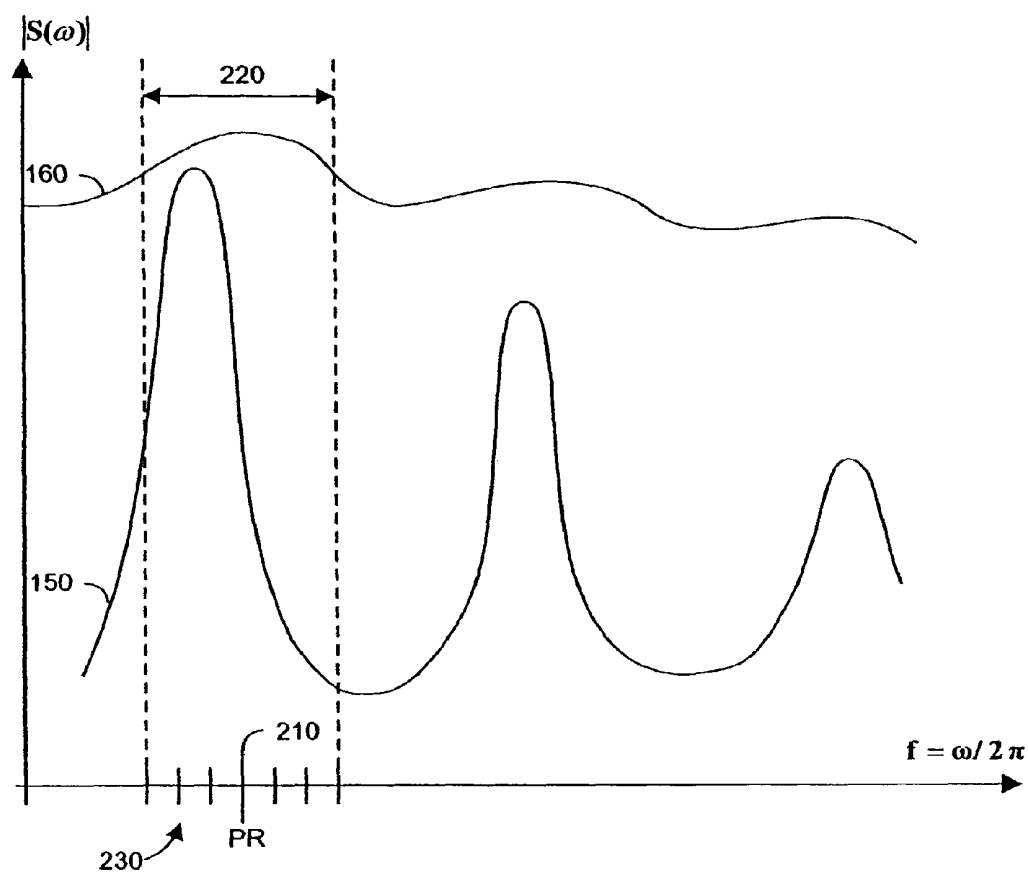


FIG. 2

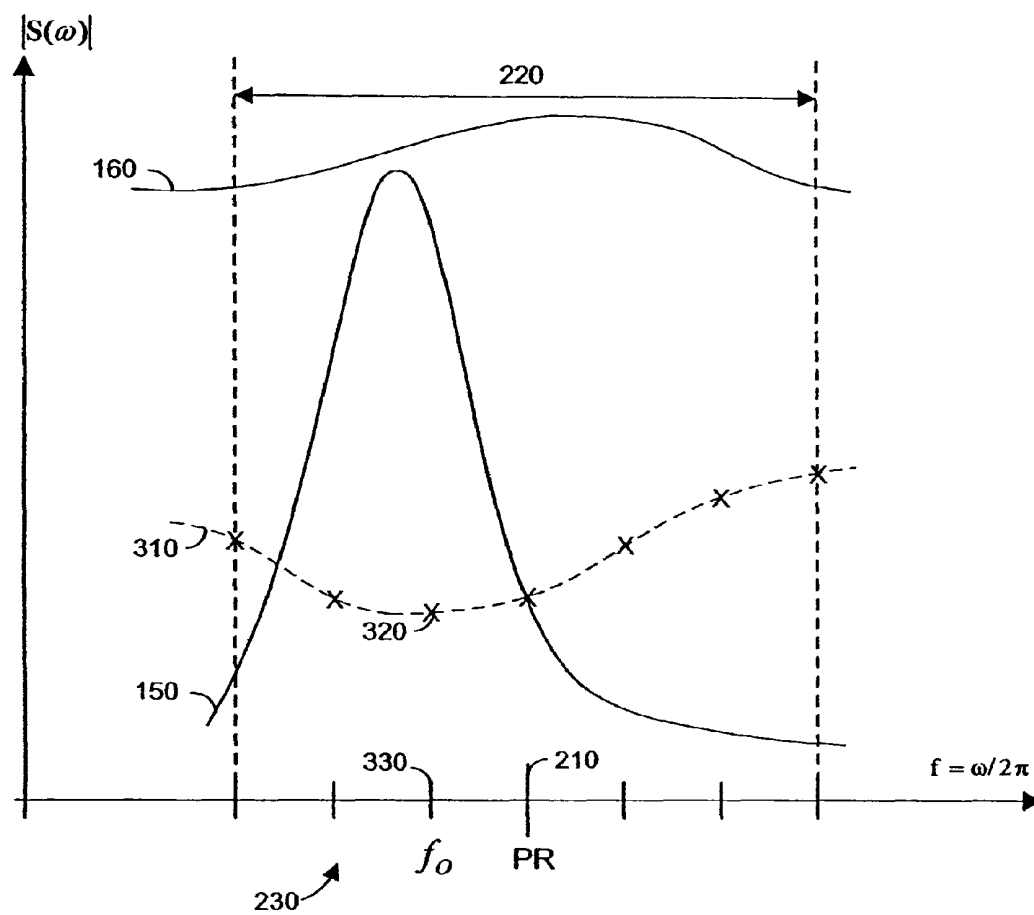


FIG. 3

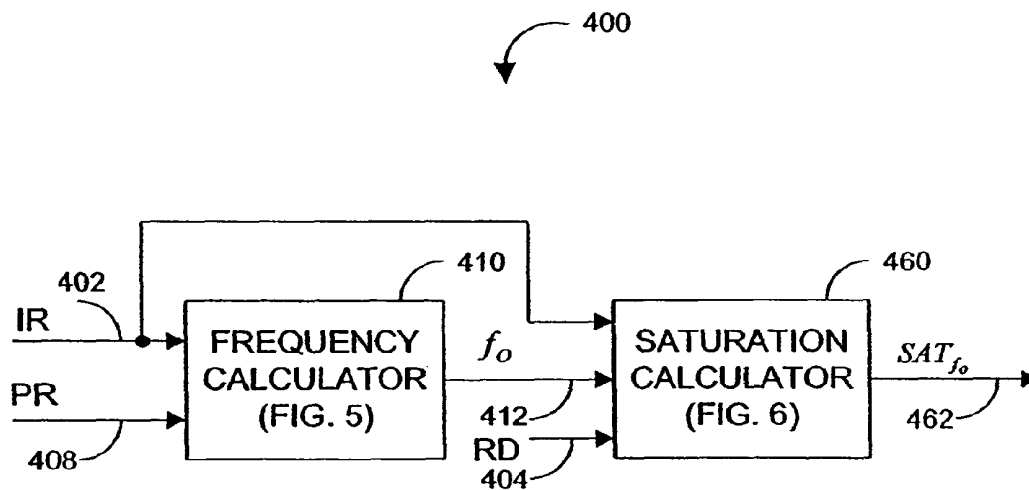


FIG. 4

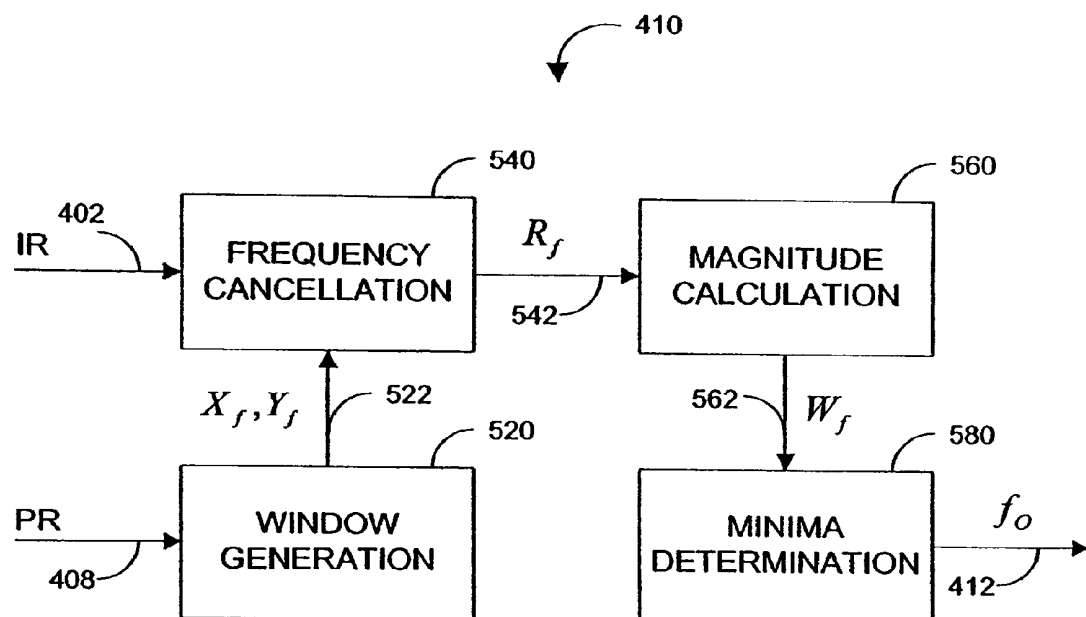


FIG. 5

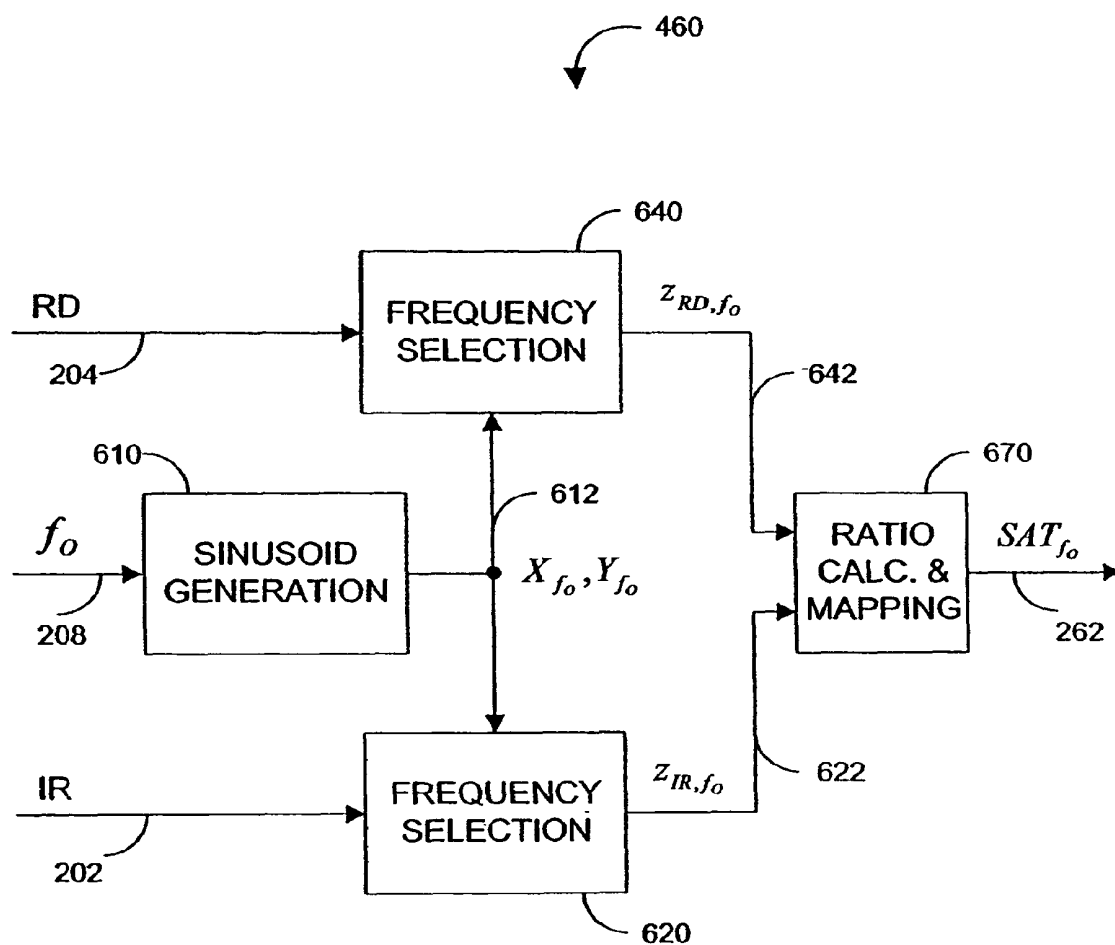


FIG. 6

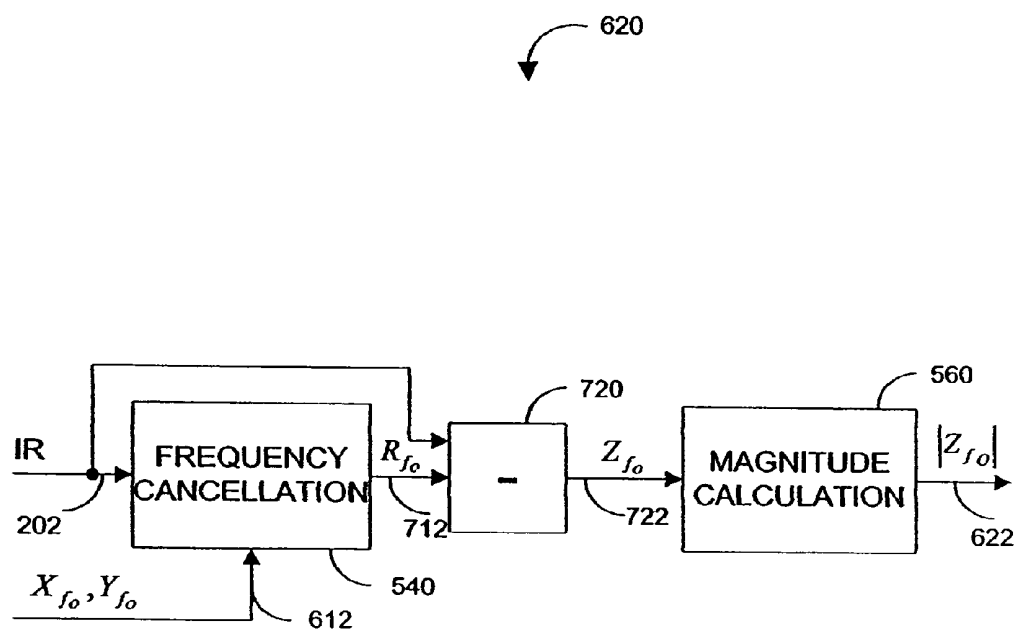


FIG. 7

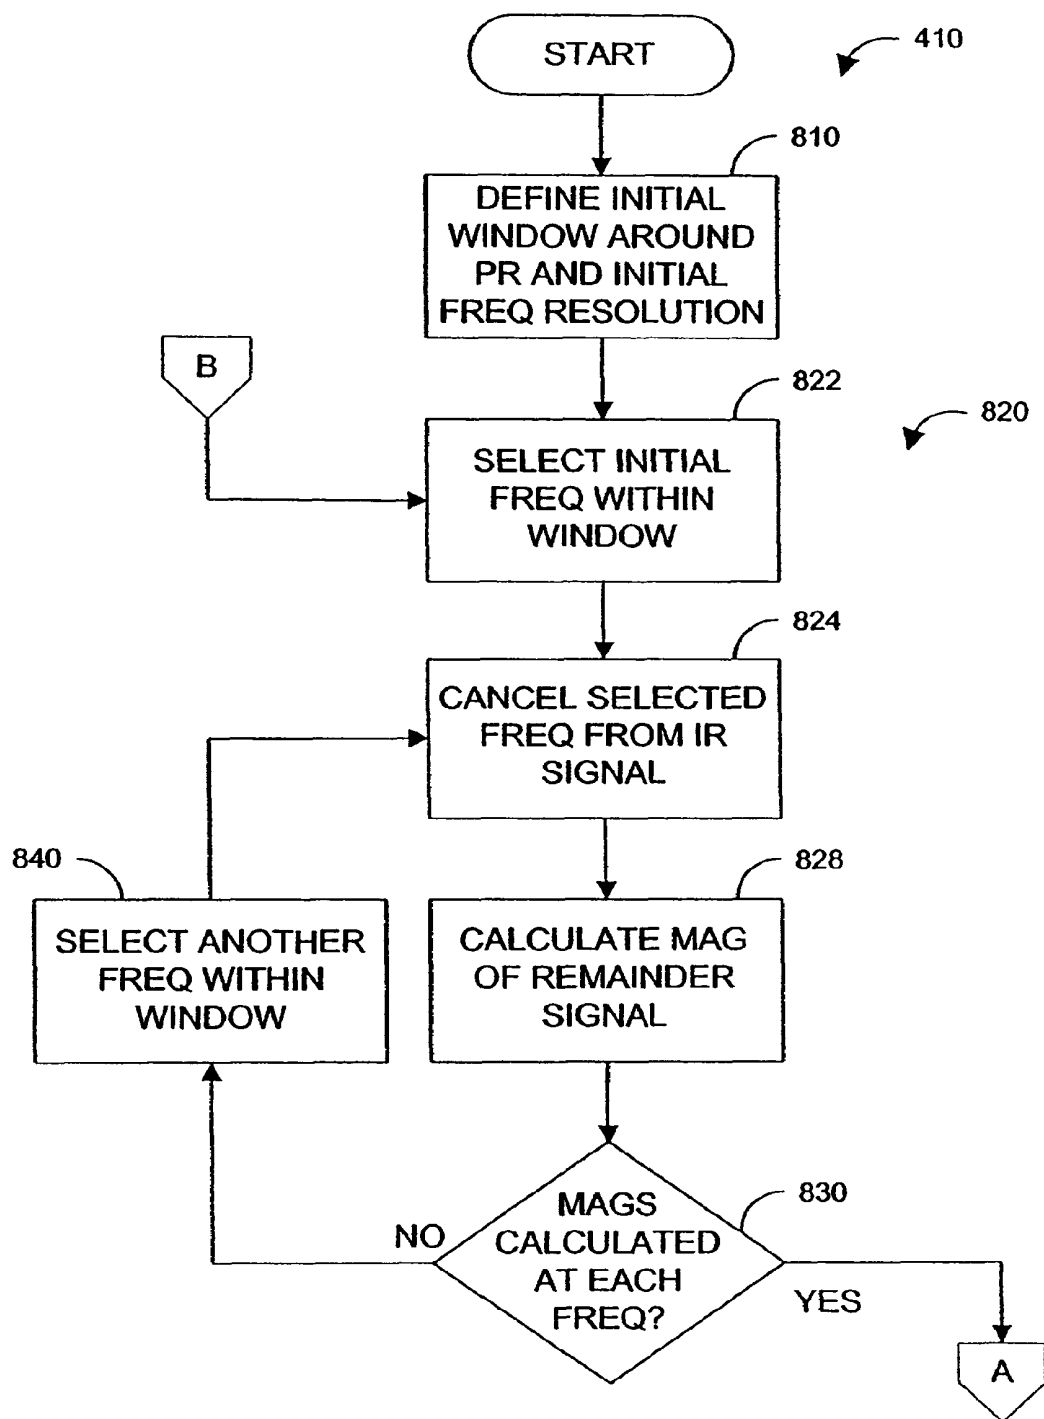


FIG. 8A

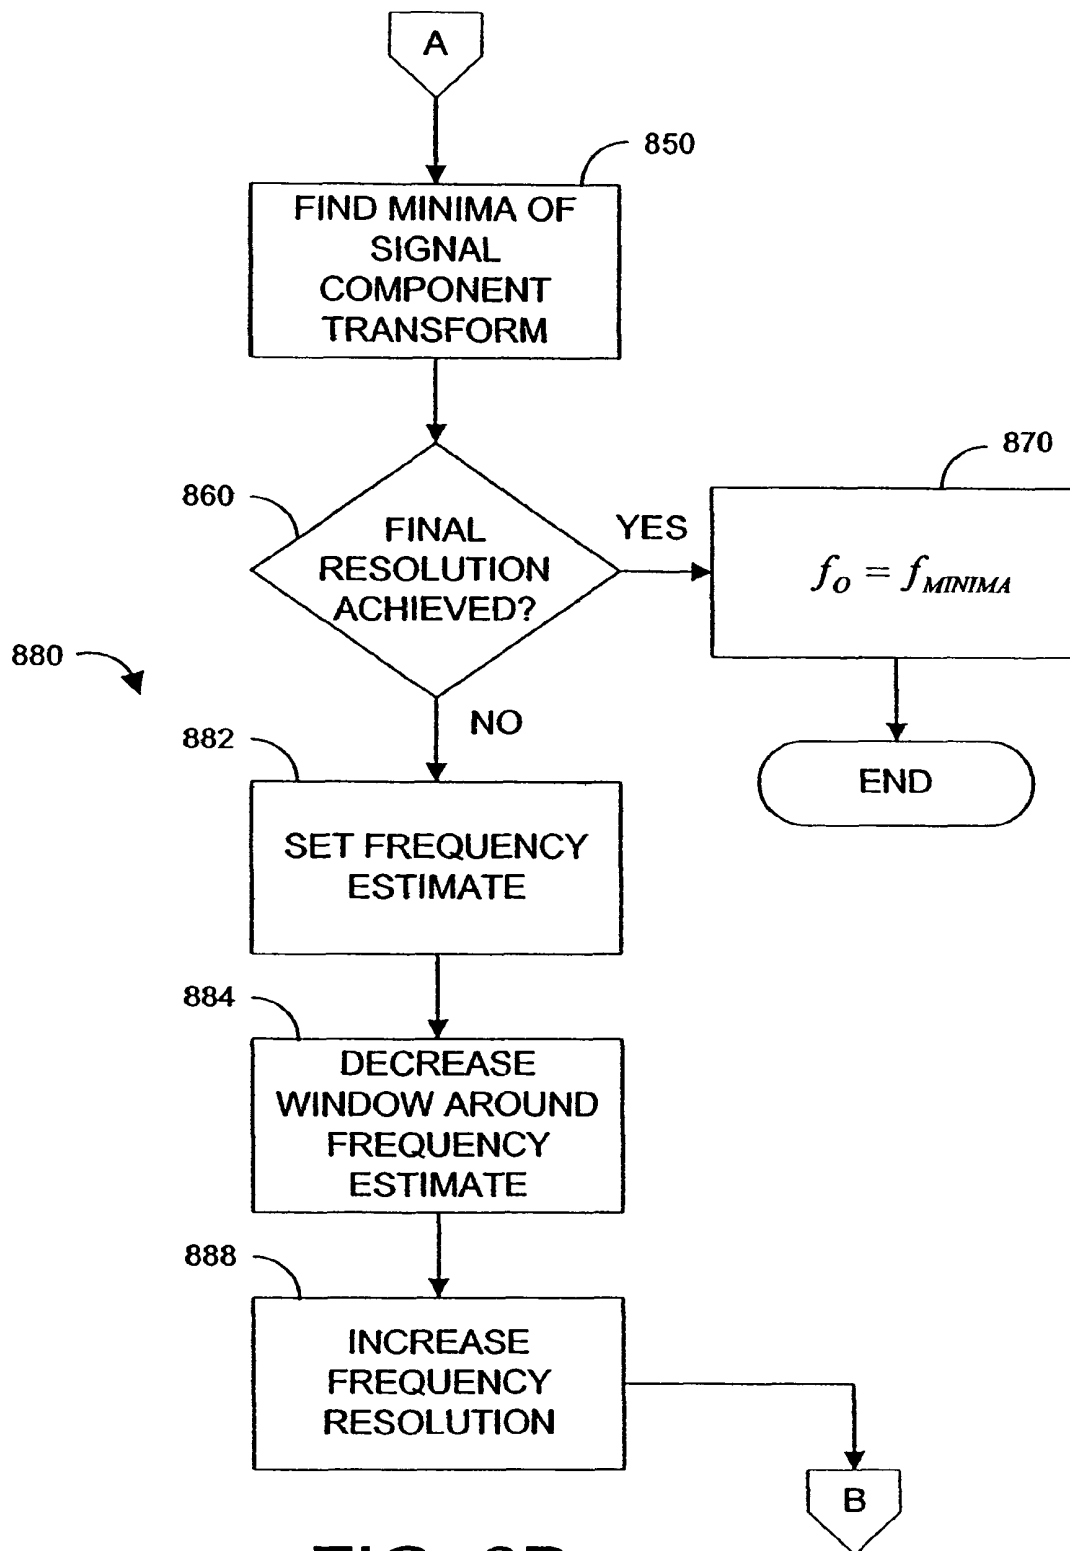


FIG. 8B

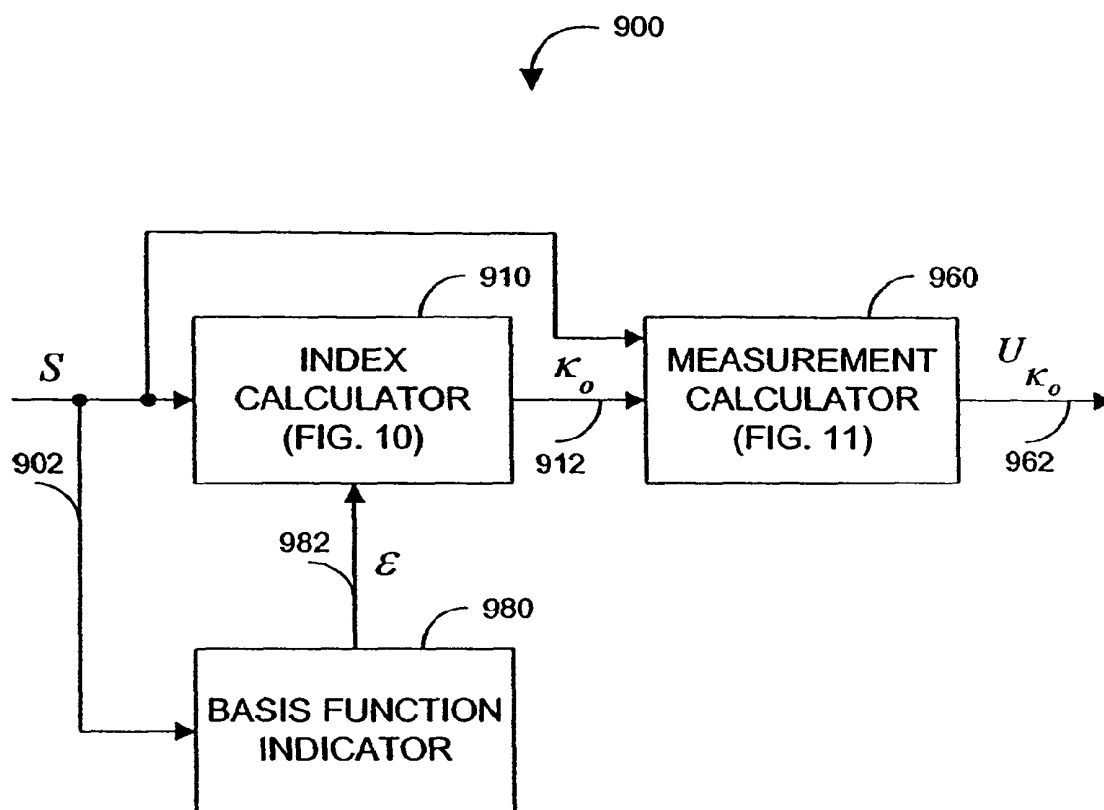


FIG. 9

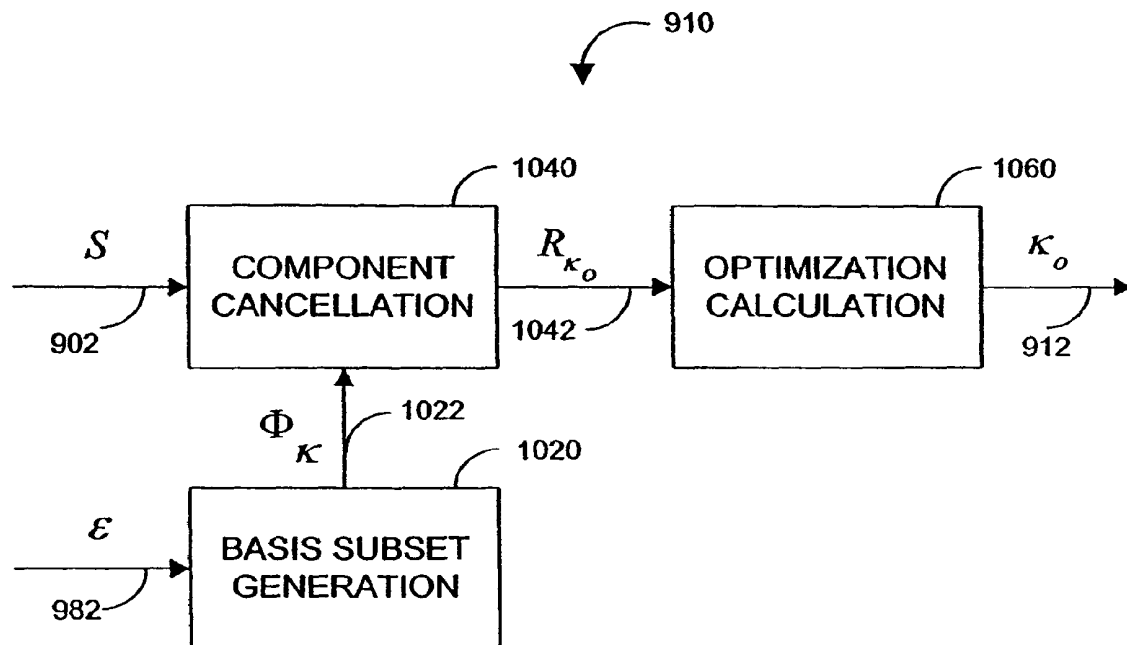


FIG. 10

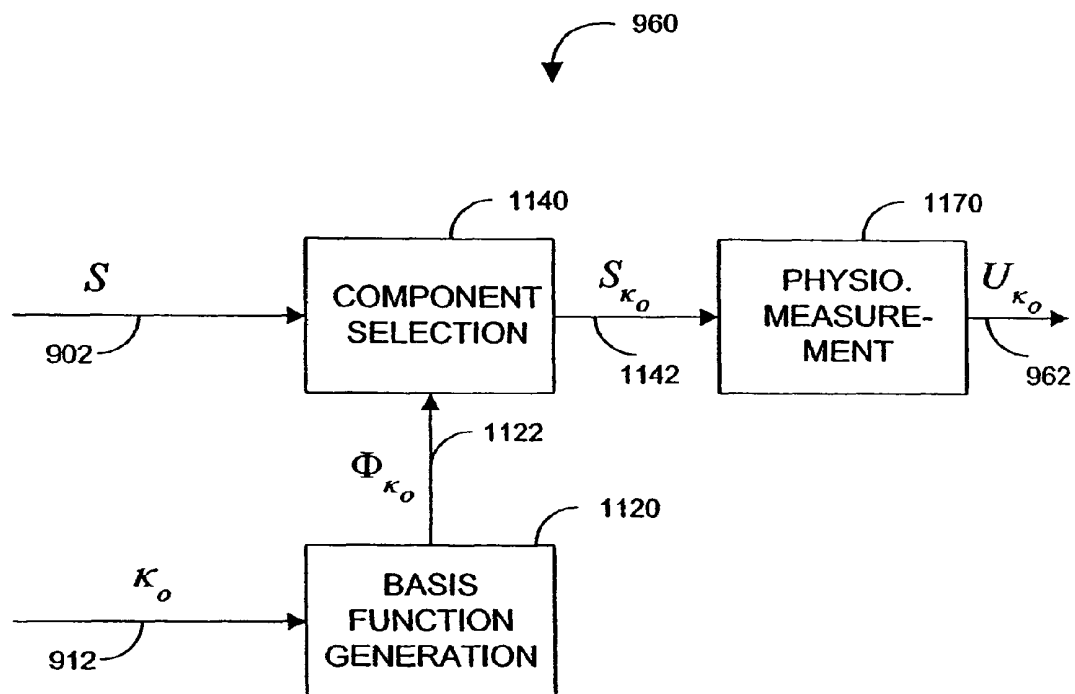


FIG. 11

SINE SATURATION TRANSFORM

CROSS-REFERENCE TO RELATED APPLICATIONS

The present application claims priority benefit under 35 U.S.C. §120 to, and is a continuation of U.S. patent application Ser. No. 12/336,419, filed Dec. 16, 2008 entitled "Sine Saturation Transform," which is a continuation of, U.S. patent application Ser. No. 11/894,648, filed Aug. 20, 2007 entitled "Sine Saturation Transform," now U.S. Pat. No. 7,467,002 which is a continuation of U.S. patent application Ser. No. 11/417,914, filed May 3, 2006, entitled "Sine Saturation Transform," now U.S. Pat. No. 7,377,899, which is a continuation of, U.S. patent application Ser. No. 11/048,232, filed Feb. 1, 2005, entitled "Signal Component Processor," now U.S. Pat. No. 7,373,194 which is a continuation of U.S. patent application Ser. No. 10/184,032, filed Jun. 26, 2002, entitled "Signal Component Processor," now U.S. Pat. No. 6,850,787, which claims priority benefit under 35 U.S.C. §119(e) from U.S. Provisional Application No. 60/302,438, filed Jun. 29, 2001, entitled "Signal Component Processor." The present application also incorporates the foregoing disclosures herein by reference.

BACKGROUND OF THE INVENTION

Early detection of low blood oxygen is critical in the medical field, for example in critical care and surgical applications, because an insufficient supply of oxygen can result in brain damage and death in a matter of minutes. Pulse oximetry is a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of oxygen supply. A pulse oximeter typically provides a numerical readout of the patient's oxygen saturation and pulse rate. A pulse oximetry system consists of a sensor attached to a patient, a monitor, and a cable connecting the sensor and monitor. Conventionally, a pulse oximetry sensor has both red (RD) and infrared (IR) light-emitting diode (LED) emitters and a photodiode detector. The pulse oximeter measurements are based upon the absorption by arterial blood of the two wavelengths emitted by the sensor. The pulse oximeter alternately activates the RD and IR sensor emitters and reads the resulting RD and IR sensor signals, i.e. the current generated by the photodiode in proportion to the detected RD and IR light intensity, in order to derive an arterial oxygen saturation value, as is well-known in the art. A pulse oximeter contains circuitry for controlling the sensor, processing the sensor signals and displaying the patient's oxygen saturation and pulse rate.

SUMMARY OF THE INVENTION

FIG. 1A illustrates a plethysmograph waveform **110**, which is a display of blood volume, shown along the ordinate **101**, over time, shown along the abscissa **102**. The shape of the plethysmograph waveform **110** is a function of heart stroke volume, pressure gradient, arterial elasticity and peripheral resistance. Ideally, the waveform **110** displays a short, steep inflow phase **111** during ventricular systole followed by a typically three to four times longer outflow phase **112** during diastole. A dicrotic notch **116** is generally attributed to closure of the aortic valve at the end of ventricular systole.

FIG. 1B illustrates a corresponding RD or IR sensor signal $s(t)$ **130**, such as described above. The typical plethysmograph waveform **110** (FIG. 1A), being a function of blood

volume, also provides a light absorption profile. A pulse oximeter, however, does not directly detect light absorption and, hence, does not directly measure the plethysmograph waveform **110**. However, IR or RD sensor signals are 180° out-of-phase versions of the waveform **110**. That is, peak detected intensity **134** occurs at minimum absorption **114** and minimum detected intensity **138** occurs at maximum absorption **118**.

FIG. 1C illustrates the corresponding spectrum of $s(t)$, which is a display of signal spectral magnitude $|S(\omega)|$, shown along the ordinate **105**, versus frequency, shown along the abscissa **106**. The plethysmograph spectrum is depicted under both high signal quality **150** and low signal quality **160** conditions. Low signal quality can result when a pulse oximeter sensor signal is distorted by motion-artifact and noise. Signal processing technologies such as described in U.S. Pat. No. 5,632,272, assigned to the assignee of the present invention and incorporated by reference herein, allow pulse oximetry to function through patient motion and other low signal quality conditions.

Ideally, plethysmograph energy is concentrated at the pulse rate frequency **172** and associated harmonics **174**, **176**. Accordingly, motion-artifact and noise may be reduced and pulse oximetry measurements improved by filtering out sensor signal frequencies that are not related to the pulse rate. Under low signal quality conditions, however, the frequency spectrum is corrupted and the pulse rate fundamental **152** and harmonics **154**, **156** can be obscured or masked, resulting in errors in the computed pulse rate. In addition, a pulse rate, physiologically, is dynamic, potentially varying significantly between different measurement periods. Hence, maximum plethysmograph energy may not correspond to the computed pulse rate except under high signal quality conditions and stable pulse rates. Further, an oxygen saturation value calculated from an optical density ratio, such as a normalized red over infrared ratio, at the pulse rate frequency can be sensitive to computed pulse rate errors. In order to increase the robustness of oxygen saturation measurements, therefore, it is desirable to improve pulse rate based measurements by identifying sensor signal components that correspond to an optimization, such as maximum signal energy.

One aspect of a signal component processor comprises a physiological signal, a basis function index determined from the signal, a basis function waveform generated according to the index, a component derived from the sensor signal and the waveform, and a physiological measurement responsive to the component. In one embodiment, the component is responsive to the inner product of the sensor signal and the waveform. In another embodiment, the index is a frequency and the waveform is a sinusoid at the frequency. In that embodiment, the signal processor may further comprise a pulse rate estimate derived from the signal wherein the frequency is selected from a window including the pulse rate estimate. The physiological measurement may be an oxygen saturation value responsive to a magnitude of the component.

Another aspect of a signal component processor comprises a signal input, a basis function indicator derived from the signal input, a plurality of basis functions generated according to the indicator, a plurality of characteristics of the signal input corresponding to the basis functions and an optimization of the characteristics so as to identify at least one of said basis functions. In one embodiment, the indicator is a pulse rate estimate and the processor further comprises a window configured to include the pulse rate estimate, and a plurality of frequencies selected from within the window. In another embodiment, the characteristic comprises a plurality of signal remainders corresponding to the basis functions and a plural-

ity of magnitudes of the signal remainders. In that embodiment, the optimization comprises a minima of the magnitudes. In a further embodiment, the characteristic comprises a plurality of components corresponding to the basis functions and a plurality of magnitudes of the components. In this embodiment, the optimization comprises a maxima of the magnitudes.

An aspect of a signal component processing method comprises the steps of receiving a sensor signal, calculating an estimated pulse rate, determining an optimization of the sensor signal proximate the estimated pulse rate, defining a frequency corresponding to the optimization, and outputting a physiological measurement responsive to a component of the sensor signal at the frequency. In one embodiment the determining step comprises the substeps of transforming the sensor signal to a frequency spectrum encompassing the estimated pulse rate and detecting an extrema of the spectrum indicative of the frequency. The transforming step may comprise the substeps of defining a window including the estimated pulse rate, defining a plurality of selected frequencies within the window, canceling the selected frequencies, individually, from the sensor signal to generate a plurality of remainder signals and calculating a plurality of magnitudes of the remainder signals. The detecting step may comprise the substep of locating a minima of the magnitudes.

In another embodiment, the outputting step comprises the substeps of inputting a red (RD) portion and an infrared (IR) portion of the sensor signal, deriving a RD component of the RD portion and an IR component of the IR portion corresponding to the frequency and computing an oxygen saturation based upon a magnitude ratio of the RD component and the IR component. The deriving step may comprise the substeps of generating a sinusoidal waveform at the frequency and selecting the RD component and the IR component utilizing the waveform. The selecting step may comprise the substep of calculating the inner product between the waveform and the RD portion and the inner product between the waveform and the IR portion. The selecting step may comprise the substeps of canceling the waveform from the RD portion and the IR portion, leaving a RD remainder and an IR remainder, and subtracting the RD remainder from the RD portion and the IR remainder from the IR portion.

A further aspect of a signal component processor comprises a first calculator means for deriving an optimization frequency from a pulse rate estimate input and a sensor signal, and a second calculator means for deriving a physiological measurement responsive to a sensor signal component at the frequency. In one embodiment, the first calculator means comprises a signal component transform means for determining a plurality of signal values corresponding to a plurality of selected frequencies within a window including the pulse rate estimate, and a detection means for determining a particular one of the selected frequencies corresponding to an optimization of the sensor signal. The second calculator means may comprise a waveform means for generating a sinusoidal signal at the frequency, a frequency selection means for determining a component of the sensor signal from the sinusoidal signal and a calculator means for deriving a ratio responsive to the component.

BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A-C are graphical representations of a pulse oximetry sensor signal;

FIG. 1A is a typical plethysmograph illustrating blood volume versus time;

FIG. 1B is a pulse oximetry sensor signal illustrating detected light intensity versus time;

FIG. 1C is a pulse oximetry sensor signal spectrum illustrating both high signal quality and low signal quality conditions;

FIGS. 2-3 are magnitude versus frequency graphs for a pulse oximetry sensor signal illustrating an example of signal component processing;

FIG. 2 illustrates a frequency window around an estimated pulse rate; and

FIG. 3 illustrates an associated signal component transform;

FIGS. 4-7 are functional block diagrams of one embodiment of a signal component processor;

FIG. 4 is a top-level functional block diagram of a signal component processor;

FIG. 5 is a functional block diagram of a frequency calculator;

FIG. 6 is a functional block diagram of a saturation calculator; and

FIG. 7 is a functional block diagram of one embodiment of a frequency selection;

FIGS. 8A-B are flowcharts of an iterative embodiment of a frequency calculator; and

FIGS. 9-11 are functional block diagrams of another embodiment of a signal component processor;

FIG. 9 is a top-level functional block diagram of a signal component processor;

FIG. 10 is a functional block diagram of an index calculator; and

FIG. 11 is a functional block diagram of a measurement calculator.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

FIGS. 2 and 3 provide graphical illustration examples of signal component processing. Advantageously, signal component processing provides a direct method for the calculation of saturation based on pulse rate. For example, it is not necessary to compute a frequency transform, such as an FFT, which derives an entire frequency spectrum. Rather, signal component processing singles out specific signal components, as described in more detail below. Further, signal component processing advantageously provides a method of refinement for the calculation of saturation based on pulse rate.

FIG. 2 illustrates high and low signal quality sensor signal spectrums 150, 160 as described with respect to FIG. 1C, above. A frequency window 220 is created, including a pulse rate estimate PR 210. A pulse rate estimate can be calculated as disclosed in U.S. Pat. No. 6,002,952, entitled "Signal Processing Apparatus and Method," assigned to the assignee of the present invention and incorporated by reference herein. A search is conducted within this window 220 for a component frequency f_o at an optimization. In particular, selected frequencies 230, which include PR, are defined within the window 220. The components of a signal $s(t)$ at each of these frequencies 230 are then examined for an optimization indicative of an extrema of energy, power or other signal characteristic. In an alternative embodiment, the components of the signal $s(t)$ are examined for an optimization over a continuous range of frequencies within the window 220.

FIG. 3 illustrates an expanded portion of the graph described with respect to FIG. 2, above. Superimposed on the high signal quality 150 and low signal quality 160 spectrums is a signal component transform 310. In one embodiment, a

5

signal component transform **310** is indicative of sensor signal energy and is calculated at selected signal frequencies **230** within the window **220**. A signal component transform **310** has an extrema **320** that indicates, in this embodiment, energy optimization at a particular one **330** of the selected frequencies **230**. The extrema **320** can be, for example, a maxima, minima or inflection point. In the embodiment illustrated, each point of the transform **310** is the magnitude of the signal remaining after canceling a sensor signal component at one of the selected frequencies. The extrema **320** is a minima, which indicates that canceling the corresponding frequency **330** removes the most signal energy. In an alternative embodiment, not illustrated, the transform **310** is calculated as the magnitude of signal components at each of the selected frequencies **230**. In that embodiment, the extrema is a maxima, which indicates the largest energy signal at the corresponding frequency. The result of a signal component transform **310** is identification of a frequency f_O **330** determined from the frequency of a signal component transform extrema **320**. Frequency f_O **330** is then used to calculate an oxygen saturation. A signal component transform and corresponding oxygen saturation calculations are described in additional detail with respect to FIGS. 4-8, below. Although signal component processing is described above with respect to identifying a particular frequency within a window including a pulse rate estimate PR, a similar procedure could be performed on 2PR, 3PR etc. resulting in the identification of multiple frequencies f_{O1}, f_{O2} etc., which could be used for the calculation of oxygen saturation as well.

Advantageously, a signal component transform **310** is calculated over any set of selected frequencies, unrestricted by the number or spacing of these frequencies. In this manner, a signal component transform **310** differs from a FFT or other standard frequency transforms. For example, a FFT is limited to N evenly-distributed frequencies spaced at a resolution of f_s/N , where N is the number of signal samples and f_s is the sampling frequency. That is, for a FFT, a relatively high sampling rate or a relatively large record length or both are needed to achieve a relatively high resolution in frequency. Signal component processing, as described herein, is not so limited. Further, a signal component transform **310** is advantageously calculated only over a range of frequencies of interest. A FFT or similar frequency transformation may be computationally more burdensome than signal component processing, in part because such a transform is computed over all frequencies within a range determined by the sampling frequency, f_s .

FIGS. 4-7 illustrate one embodiment of a signal component processor. FIG. 4 is a top-level functional block diagram of a signal component processor **400**. The signal component processor **400** has a frequency calculator **410** and a saturation calculator **460**. The frequency calculator **410** has an IR signal input **402**, a pulse rate estimate signal PR input **408** and a component frequency f_O output **412**. The frequency calculator **410** performs a signal component transform based upon the PR input **408** and determines the f_O output **412**, as described with respect to FIGS. 2-3, above. The frequency calculator **410** is described in further detail with respect to FIG. 5, below.

In an alternative embodiment, the frequency calculator **410** determines f_O **412** based upon a RD signal input substituted for, or in addition to, the IR signal input **402**. Similarly, one of ordinary skill in the art will recognize that f_O can be determined by the frequency calculator **410** based upon one or more inputs responsive to a variety of sensor wavelengths.

The saturation calculator **460** has an IR signal input **402**, a RD signal input **404**, a component frequency f_O input **412** and

6

an oxygen saturation output, SAT_{f_O} **462**. The saturation calculator **460** determines values of the IR signal input **402** and the RD signal input **404** at the component frequency f_O **412** and computes a ratio of those values to determine SAT_{f_O} **462**, as described with respect to FIG. 6, below. The IR signal input **402** and RD signal input **404** can be expressed as:

$$IR = \begin{bmatrix} IR_0 \\ \vdots \\ IR_{N-1} \end{bmatrix}; RD = \begin{bmatrix} RD_0 \\ \vdots \\ RD_{N-1} \end{bmatrix} \quad (1)$$

where N is the number of samples of each signal input.

FIG. 5 shows one embodiment of the frequency calculator **410**. In this particular embodiment, the frequency calculator functions are window generation **520**, frequency cancellation **540**, magnitude calculation **560** and minima determination **580**. Window generation **520**, frequency cancellation **540** and magnitude calculation **560** combine to create a signal component transform **310** (FIG. 3), as described with respect to FIG. 3, above. Minima determination **580** locates the signal component transform extrema **320** (FIG. 3), which identifies f_O **412**, also described with respect to FIG. 3, above.

As shown in FIG. 5, window generation **520** has a PR input **408** and defines a window **220** (FIG. 3) about PR **210** (FIG. 3) including a set of selected frequencies **230** (FIG. 3)

$$\{f_m; m = 0, \dots, M-1\}; f = \begin{bmatrix} f_0 \\ \vdots \\ f_{M-1} \end{bmatrix} \quad (2)$$

where M is the number of selected frequencies **230** (FIG. 3) within the window **220** (FIG. 3). Window generation **520** has a sinusoidal output X_f, Y_f **522**, which is a set of sinusoidal waveforms $x_{n,f}, y_{n,f}$ each corresponding to one of the set of selected frequencies **230** (FIG. 3). Specifically

$$X_f = \begin{bmatrix} x_{0,f} \\ \vdots \\ x_{N-1,f} \end{bmatrix}; Y_f = \begin{bmatrix} y_{0,f} \\ \vdots \\ y_{N-1,f} \end{bmatrix} \quad (3a)$$

$$x_{n,f} = \sin(2\pi f n); y_{n,f} = \cos(2\pi f n) \quad (3b)$$

Also shown in FIG. 5, the frequency cancellation **540** has IR **402** and X_f, Y_f **522** inputs and a remainder output R_f **542**, which is a set of remainder signals $r_{n,f}$ each corresponding to one of the sinusoidal waveforms $x_{n,f}, y_{n,f}$. For each selected frequency f **230** (FIG. 3), frequency cancellation **540** cancels that frequency component from the input signal IR **402** to generate a remainder signal $r_{n,f}$. In particular, frequency cancellation **540** generates a remainder R_f **542**

$$R_f = \begin{bmatrix} r_{0,f} \\ \vdots \\ r_{N-1,f} \end{bmatrix} \quad (4a)$$

$$R_f = IR - \frac{IR \cdot X_f}{|X_f|^2} X_f - \frac{IR \cdot Y_f}{|Y_f|^2} Y_f \quad (4b)$$

Additionally, as shown in FIG. 5, the magnitude calculation **560** has a remainder input R_{f_o} **542** and generates a magnitude output W_{f_o} **562**, where

$$W_{f_o} = |R_{f_o}| = \sqrt{\sum_{n=0}^{N-1} r_{n,f_o}^2} \quad (5)$$

Further shown in FIG. 5, the minima determination **580** has the magnitude values W_{f_o} **562** as inputs and generates a component frequency f_o output. Frequency f_o is the particular frequency associated with the minimum magnitude value

$$W_{f_o} = \min\{W_f\} \quad (6)$$

FIG. 6 shows that the saturation calculator **460** functions are sinusoid generation **610**, frequency selection **620**, **640** and ratio calculation **670**. Sinusoid generation has a component frequency f_o input **208** and a sinusoidal waveform X_{f_o} , Y_{f_o} output **612**, which has a frequency of f_o . Frequency selection **620**, **640** has a sensor signal input, which is either an IR signal **202** or a RD signal **204** and a sinusoid waveform X_{f_o} , Y_{f_o} input **612**. Frequency selection **620**, **640** provides magnitude outputs z_{IR,f_o} **622** and z_{RD,f_o} **642** which are the frequency components of the IR **202** and RD **204** sensor signals at the f_o frequency. Specifically, from equation 3(a)

$$X_{f_o} = \begin{bmatrix} x_{0,f_o} \\ \vdots \\ x_{N-1,f_o} \end{bmatrix}; Y_{f_o} = \begin{bmatrix} y_{0,f_o} \\ \vdots \\ y_{N-1,f_o} \end{bmatrix} \quad (7)$$

Then, referring to equation 1

$$z_{IR,f_o} = \frac{|IR \cdot X_{f_o}|}{|X_{f_o}|^2} X_{f_o} + \frac{|IR \cdot Y_{f_o}|}{|Y_{f_o}|^2} Y_{f_o} \quad (8a)$$

$$= \sqrt{\frac{(IR \cdot X_{f_o})^2}{|X_{f_o}|^2} + \frac{(IR \cdot Y_{f_o})^2}{|Y_{f_o}|^2}}$$

$$z_{RD,f_o} = \frac{|RD \cdot X_{f_o}|}{|X_{f_o}|^2} X_{f_o} + \frac{|RD \cdot Y_{f_o}|}{|Y_{f_o}|^2} Y_{f_o} \quad (8b)$$

$$= \sqrt{\frac{(RD \cdot X_{f_o})^2}{|X_{f_o}|^2} + \frac{(RD \cdot Y_{f_o})^2}{|Y_{f_o}|^2}}$$

For simplicity of illustration, EQS. 8a-b assume that the cross-product of X_{f_o} and Y_{f_o} is zero, although generally this is not the case. The ratio calculation and mapping **670** has z_{IR,f_o} **622** and z_{RD,f_o} **642** as inputs and provides SAT_{f_o} **262** as an output. That is

$$SAT_{f_o} = g\{z_{RD,f_o}/z_{IR,f_o}\} \quad (9)$$

where g is a mapping of the red-over-IR ratio to oxygen saturation, which may be an empirically derived lookup table, for example.

FIG. 7 illustrates an alternative embodiment of frequency selection **620** (FIG. 6), as described above. In this embodiment, frequency cancellation **540** and magnitude calculation **560**, as described with respect to FIG. 5, can also be used, advantageously, to perform frequency selection. Specifically, frequency cancellation **540** has IR **202** and X_{f_o} , Y_{f_o} **612** as inputs and generates a remainder signal R_{f_o} **712** as an output, where

$$R_{f_o} = IR - \frac{IR \cdot X_{f_o}}{|X_{f_o}|^2} X_{f_o} - \frac{IR \cdot Y_{f_o}}{|Y_{f_o}|^2} Y_{f_o} \quad (10)$$

The remainder R_{f_o} **712** is subtracted **720** from IR **202** to yield

$$Z_{f_o} = IR - \left[IR - \frac{IR \cdot X_{f_o}}{|X_{f_o}|^2} X_{f_o} - \frac{IR \cdot Y_{f_o}}{|Y_{f_o}|^2} Y_{f_o} \right] \quad (11)$$

$$= \frac{IR \cdot X_{f_o}}{|X_{f_o}|^2} X_{f_o} + \frac{IR \cdot Y_{f_o}}{|Y_{f_o}|^2} Y_{f_o}$$

where z_{f_o} **722** is the component of IR **202** at the f_o frequency. The magnitude calculation **560** has z_{f_o} **722** as an input and calculates

$$|Z_{f_o}| = \left| \frac{IR \cdot X_{f_o}}{|X_{f_o}|^2} X_{f_o} + \frac{IR \cdot Y_{f_o}}{|Y_{f_o}|^2} Y_{f_o} \right| \quad (12)$$

$$= \sqrt{\frac{(IR \cdot X_{f_o})^2}{|X_{f_o}|^2} + \frac{(IR \cdot Y_{f_o})^2}{|Y_{f_o}|^2}}$$

which is equivalent to equation 8a, above.

FIGS. 8A-B illustrate an iterative embodiment of the frequency calculator **410** (FIG. 4) described above. An iterative frequency calculator **410** has an initialization **810**, a signal component transform **820**, an extrema detection **850**, a resolution decision **860** and a resolution refinement **880** and provides a component frequency f_o **870**. Initialization **810** defines a window around the pulse rate estimate PR and a frequency resolution within that window.

As shown in FIG. 8A, a signal component transform **820** has an initial frequency selection **822**, a frequency cancellation **824** and an magnitude calculation **828**. A decision block **830** determines if the magnitude calculation **828** has been performed at each frequency within the window. If not, the loop of frequency cancellation **824** and magnitude calculation **828** is repeated for another selected frequency in the window. The frequency cancellation **824** removes a frequency component from the IR sensor signal, as described with respect to FIG. 5, above. The magnitude calculation **828** determines the magnitude of the remainder signal, also described with respect to FIG. 5, above. If the decision block **830** determines that the remainder signal magnitudes have been calculated at each of the selected frequencies, then the signal component transform loop **820** is exited to the steps described with respect to FIG. 8B.

As shown in FIG. 8B, the extrema detector **850** finds a minima of a signal component transform **820** and a resolution decision block **860** determines if the final frequency resolution of a signal component transform is achieved. If not, resolution refinement **880** is performed. If the final resolution is achieved, the component frequency output f_o is equated to the frequency of the minima **870**, i.e. a signal component transform minima determined by the extrema detector **850**.

Further shown in FIG. 8B, the resolution refinement **880** has a set frequency estimate **882**, a window decrease **884** and a frequency resolution increase **888**. Specifically, the frequency estimate **882** is set to a signal component transform minima, as determined by the extrema detector **850**. The window decrease **884** defines a new and narrower window around the frequency estimate, and the frequency resolution

increase **888** reduces the spacing of the selected frequencies within that window prior to the next iteration of a signal component transform **820**. In this manner, a signal component transform **820** and the resulting frequency estimate are refined to a higher resolution with each iteration of signal component transform **820**, extrema detection **850**, and resolution refinement **880**.

In a particular embodiment, the component calculation requires three iterations. A frequency resolution of 4 beats per minute or 4 BPM is used initially and a window of five or seven selected frequencies, including that of the initial pulse rate estimate PR, is defined. That is, a window of either 16 BPM or 24 BPM centered on PR is defined, and a signal component transform is computed for a set of 5 or 7 selected frequencies evenly spaced at 4 BPM. The result is a frequency estimate f_1 . Next, the frequency resolution is reduced from 4 BPM to 2 BPM and a 4 BPM window centered on f_1 is defined with three selected frequencies, i.e. $f_1 - 2$ BPM, f_1 , and $f_1 + 2$ BPM. The result is a higher resolution frequency estimate f_2 . On the final iteration, the frequency resolution is reduced to 1 BPM and a 2 BPM window centered on f_2 is defined with three selected frequencies, i.e. $f_2 - 1$ BPM, f_2 , and $f_2 + 1$ BPM. The final result is the component frequency f_o determined by a signal component transform to within a 1 BPM resolution. This component frequency f_o is then used to calculate the oxygen saturation, SAT_{f_o} , as described above.

The signal component processor has been described above with respect to pulse oximetry and oxygen saturation measurements based upon a frequency component that optimizes signal energy. The signal component processor, however, is applicable to other physiological measurements, such as blood glucose, carboxy-hemoglobin, respiration rate and blood pressure to name a few. Further, the signal component processor is generally applicable to identifying, selecting and processing any basis function signal components, of which single frequency components are one embodiment, as described in further detail with respect to FIG. 9, below.

FIGS. 9-11 illustrate another embodiment of a signal component processor **900**. As shown in FIG. 9, the processor **900** has an index calculator **910** and a measurement calculator **960**. The index calculator has a sensor signal input **S 902** and outputs a basis function index κ_o **912**, as described with respect to FIG. 10, below. The measurement calculator **960** inputs the basis function index κ_o **912** and outputs a physiological measurement U_{κ_o} **962**, as described with respect to FIG. 11, below. The processor **900** also has a basis function indicator **980**, which is responsive to the sensor signal input **S 902** and provides a parameter ϵ **982** that indicates a set of basis functions to be utilized by the index calculator **910**, as described with respect to FIG. 10, below.

As shown in FIG. 10, the functions of the index calculator **910** are basis subset generation **1020**, component cancellation **1040** and optimization calculation **1060**. The basis subset generation **1020** outputs a subset Φ_{κ} **1022** of basis function waveforms corresponding to a set of selected basis function indices κ . The basis functions can be any complete set of functions such that

$$S = \sum_{\kappa} \alpha_{\kappa} \Phi_{\kappa} \quad (13)$$

For simplicity of illustration purposes, these basis functions are assumed to be orthogonal

$$\langle \vec{\Phi}_{\gamma}, \vec{\Phi}_{\eta} \rangle = 0; \gamma \neq \eta \quad (14)$$

where $\langle \rangle$ denotes an inner product. As such

$$\alpha_{\kappa} = \langle S, \Phi_{\kappa} \rangle / \langle \Phi_{\kappa}, \Phi_{\kappa} \rangle \quad (15)$$

$$S_{\kappa} = \alpha_{\kappa} \Phi_{\kappa} \quad (16)$$

In general, the basis functions may be non-orthogonal. The subset of basis functions generated is determined by an input parameter ϵ **982**. In the embodiment described with respect to FIG. 5, above, the basis functions are sinusoids, the indices are the sinusoid frequencies and the input parameter ϵ **982** is a pulse rate estimate that determines a frequency window.

As shown in FIG. 10, the component cancellation **1040** generates a remainder output R_{κ} **1042**, which is a set of remainder signals corresponding to the subset of basis function waveforms Φ_{κ} **1022**. For each basis function waveform generated, component cancellation removes the corresponding basis function component from the sensor signal **S 902** to generate a remainder signal. In an alternative embodiment, component cancellation **1040** is replaced with a component selection that generates a corresponding basis function component of the sensor signal **S 902** for each basis function generated. The optimization calculation **1060** generates a particular index κ_o **912** associated with an optimization of the remainders R_{κ} **1042** or, alternatively, an optimization of the selected basis function signal components.

As shown in FIG. 11, the functions of the measurement calculator **960** are basis function generation **1120**, component selection **1140**, and physiological measurement calculation **1170**. The component selection **1140** inputs the sensor signal **S 902** and a particular basis function waveform Φ_{κ_o} **1122** and outputs a sensor signal component S_{κ_o} **1142**. The physiological measurement **1170** inputs the sensor signal component S_{κ_o} **1142** and outputs the physiological measurement U_{κ_o} **962**, which is responsive to the sensor signal component S_{κ_o} **1142**. In the embodiment described with respect to FIG. 6, above, the basis functions Φ_{κ} are sinusoids and the index κ_o is a particular sinusoid frequency. The basis function generation **1120** creates sine and cosine waveforms at this frequency. The component selection **1140** selects corresponding frequency components of the sensor signal portions, RD and IR. Also, the physiological measurement **1170** computes an oxygen saturation based upon a magnitude ratio of these RD and IR frequency components.

The signal component processor has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications.

What is claimed is:

1. A method of determining of a physiological parameter of a monitored patient attached to a noninvasive optical sensor, the method including electronically processing signals indicative of attenuation by body tissue of the patient, the method comprising:

receiving one or more signals indicative of light attenuated by body tissue of pulsing blood in said monitored patient, said one or more signals usable to determine measurements for one or more physiological parameters of said monitored patient;
electronically determining at least one basis function index based on said one or more signals;

11

electronically generating at least one basis function waveform based on said at least one basis function index;
 electronically optimizing said at least one basis function waveform and said one or more signals to determine an optimized basis function index;
 electronically generating an optimized basis function waveform based on said optimized basis function index;
 and
 electronically processing said one or more signals and said optimized basis function waveform to determine an output measurement of one or more of said one or more physiological parameters.

2. The method of claim 1, comprising generating one or more sinusoidal waves as the at least one basis function waveform.

3. The method of claim 2, comprising individually canceling the generated sinusoidal waves from said one or more signals.

4. The method of claim 1, wherein said optimizing includes determining a frequency corresponding to the sinusoidal waveform which produces an extrema.

5. The method of claim 4, wherein the extrema comprises a minima.

6. The method of claim 1, comprising sending said output measurement to a display.

7. The method of claim 6, comprising displaying said output measurement.

8. The method of claim 1, wherein said one or more physiological parameters comprises oxygen saturation.

9. The method of claim 1, wherein said at least one basis function corresponds to an estimated pulse rate.

10. The method of claim 1, wherein said at least one basis function waveform comprises two or more basis function waveforms.

11. A signal processing system for determining a physiological parameter of a monitored patient attached to a non-invasive optical sensor, electronically processing signals indicative of attenuation by body tissue of the patient, the system comprising:

- at least one input configured to receive one or more signals indicative of light attenuated by body tissue of pulsing blood in said monitored patient, said one or more signals usable to determine measurements for one or more physiological parameters of said monitored patient;
- at least one basis function indicator configured to determine at least one basis function index based on said one or more signals;
- at least one basis subset generator configured to generate at least one basis function waveform based on said at least one basis function index;
- at least one optimization calculator configured to optimize said one or more signals and said one or more basis function waveforms to determine an optimized basis function index;
- at least one basis function generator configured to generate an optimized basis function waveform based on said optimized basis function index; and

12

at least one physiological measurement calculator configured to process said one or more signals and said optimized basis function waveform to determine a physiological measurement.

12. The system of claim 11, comprising at least one component calculator configured to combine said at least one basis function waveform with said one or more of said signals to produce a remainder signal response.

13. The system of claim 11, comprising at least one component selection calculator configured to process said one or more signals and said second basis function waveform to determine a sensor signal component.

14. The system of claim 11, wherein said one or more physiological parameters comprises two or more physiological parameters.

15. The method of claim 11, wherein said at least one basis function corresponds to an estimated pulse rate.

16. The method of claim 11, wherein said at least one basis function waveform comprises two or more basis function waveforms.

17. A signal processing system for determining a physiological parameter of a monitored patient attached to a non-invasive optical sensor, electronically processing signals indicative of attenuation by body tissue of the patient, the method comprising:

- an input capable of accepting at least one physiological signal;

- a first waveform generator configured to generate a plurality of waveforms based on an estimated pulse rate from said at least one physiological signal;

- a frequency optimization calculator configured to: process said at least one signal with said plurality of waveforms to determine one or more remainder waveforms;

- determine one or more magnitudes based on said one or more remainder waveforms;

- determine an optimized component frequency based on said one or more magnitudes;

- a second waveform generator configured to generate a component waveform corresponding to said optimized component frequency; and

- a physiological measurement calculator configured to: process said at least one signal based on said component waveform to determine frequency components of said at least one signal;
- determine a physiological measurement based on said frequency components.

18. The system of claim 17, wherein said at least one physiological signal comprises an IR signal input and an RD signal input.

19. The system of claim 18, wherein the physiological measurement calculator determines frequency components of said IR signal input and said RD signal input corresponding to said component frequency.

* * * * *

专利名称(译)	正弦饱和变换		
公开(公告)号	US8498684	公开(公告)日	2013-07-30
申请号	US13/043421	申请日	2011-03-08
[标]申请(专利权)人(译)	WEBER WALTER中号 AL ALI AMMAR CAZZOLI LORENZO		
申请(专利权)人(译)	WEBER , WALTER M. AL-ALI , AMMAR CAZZOLI , LORENZO		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	WEBER WALTER M AL ALI AMMAR CAZZOLI LORENZO		
发明人	WEBER, WALTER M. AL-ALI, AMMAR CAZZOLI, LORENZO		
IPC分类号	A61B5/1455 A61B5/024 A61B5/02 A61B5/00 A61B5/145		
CPC分类号	A61B5/024 A61B5/14551 A61B5/1455 A61B5/14532 A61B5/02433 A61B5/14552 A61B5/7282		
优先权	11/894648 2008-12-16 US 11/417914 2008-05-27 US 11/048232 2008-05-13 US 10/184032 2005-02-01 US 60/302438 2001-06-29 US		
其他公开文献	US20110160552A1		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种用于确定生理测量的变换。变换根据通过生理传感器获得的生理信号确定基函数指数。基于基函数索引生成基函数波形。然后使用基函数波形来确定优化的基函数波形。优化的基函数波形用于计算生理测量。

