



US008670812B2

(12) **United States Patent**
Gonopolskiy et al.

(10) **Patent No.:** **US 8,670,812 B2**
(45) **Date of Patent:** **Mar. 11, 2014**

(54) **PHYSIOLOGICAL SENSOR HAVING A WAIST**

(75) Inventors: **Oleg Gonopolskiy**, West Bloomfield, MI (US); **Arik Anderson**, Birmingham, MI (US); **Melissa Muto**, Royal Oak, MI (US); **Richard Morbito**, Grosse Ile, MI (US); **Matthew Stimpson**, Macomb, MI (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 666 days.

(21) Appl. No.: **12/842,801**

(22) Filed: **Jul. 23, 2010**

(65) **Prior Publication Data**

US 2011/0021893 A1 Jan. 27, 2011

Related U.S. Application Data

(60) Provisional application No. 61/228,086, filed on Jul. 23, 2009.

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.**
USPC **600/323**

(58) **Field of Classification Search**
USPC 600/323
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,519,484	B1 *	2/2003	Lovejoy et al.	600/323
6,745,061	B1 *	6/2004	Hicks et al.	600/344
2005/0197550	A1 *	9/2005	Al-Ali et al.	600/323
2005/0251004	A1 *	11/2005	Istvan et al.	600/395
2006/0084852	A1 *	4/2006	Mason et al.	600/344
2006/0089585	A1 *	4/2006	Takemura et al.	602/58
2007/0197886	A1 *	8/2007	Naganuma et al.	600/322
2008/0242958	A1 *	10/2008	Al-Ali et al.	600/323
2009/0143657	A1 *	6/2009	Diab et al.	600/344
2009/0182209	A1 *	7/2009	Benni	600/323
2010/0049018	A1 *	2/2010	Duffy et al.	600/323
2012/0046530	A1 *	2/2012	Al-Ali et al.	600/310


* cited by examiner



Primary Examiner — Rodney Fuller



(57) **ABSTRACT**

An exemplary sensor includes a sensor pad having a first portion and a second portion separated by a waist portion. The waist portion is narrower than the first portion and the second portion. A light source that is disposed on the first portion is configured to generate near-infrared light and transmit the near-infrared light through part of a patient's body. A light detector that is disposed on the second portion is configured to detect near-infrared light that has traveled through the part of the patient's body. The near-infrared light detected indicates an amount of oxygen in the part of the patient's body through which the near-infrared light traveled.

22 Claims, 2 Drawing Sheets

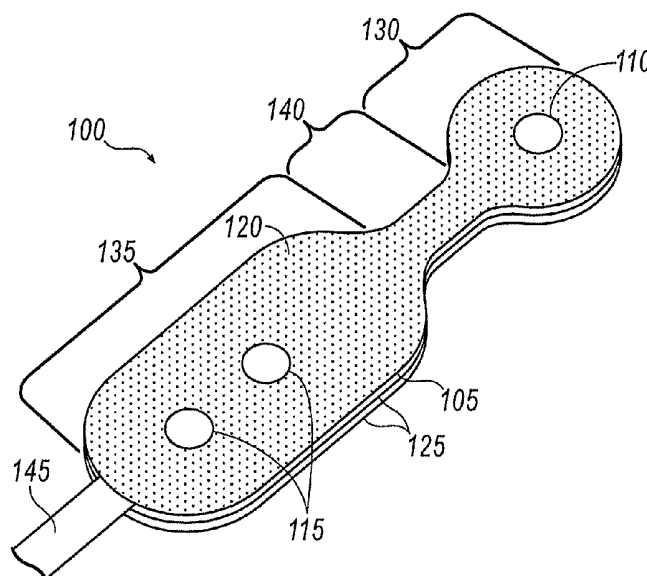

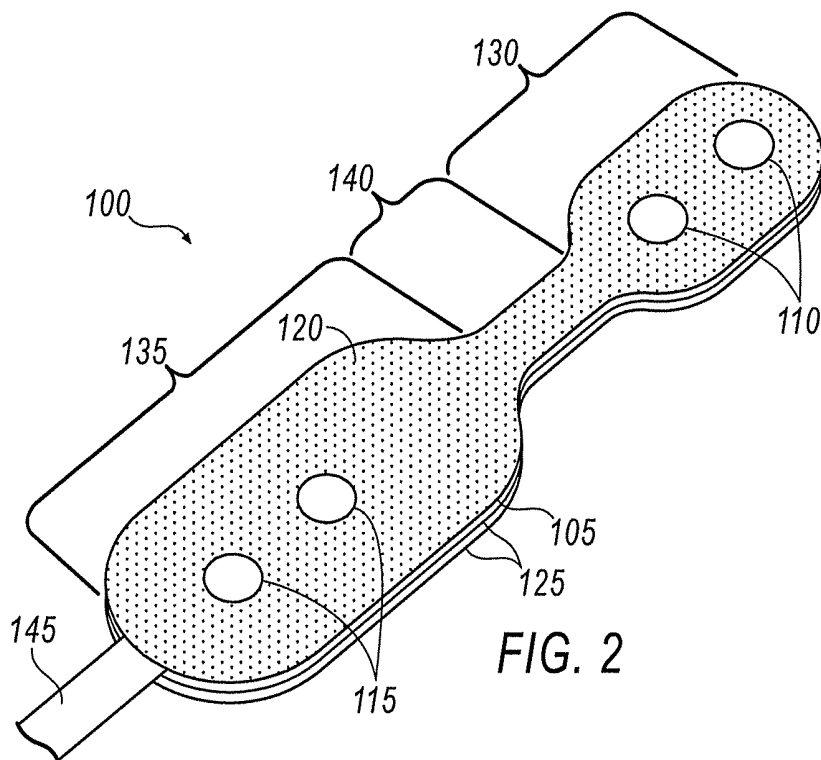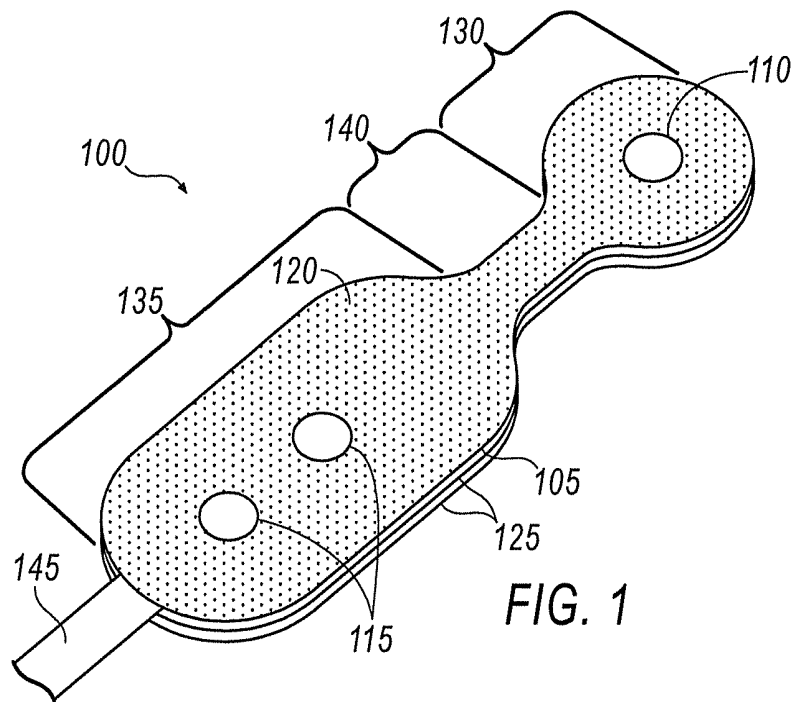

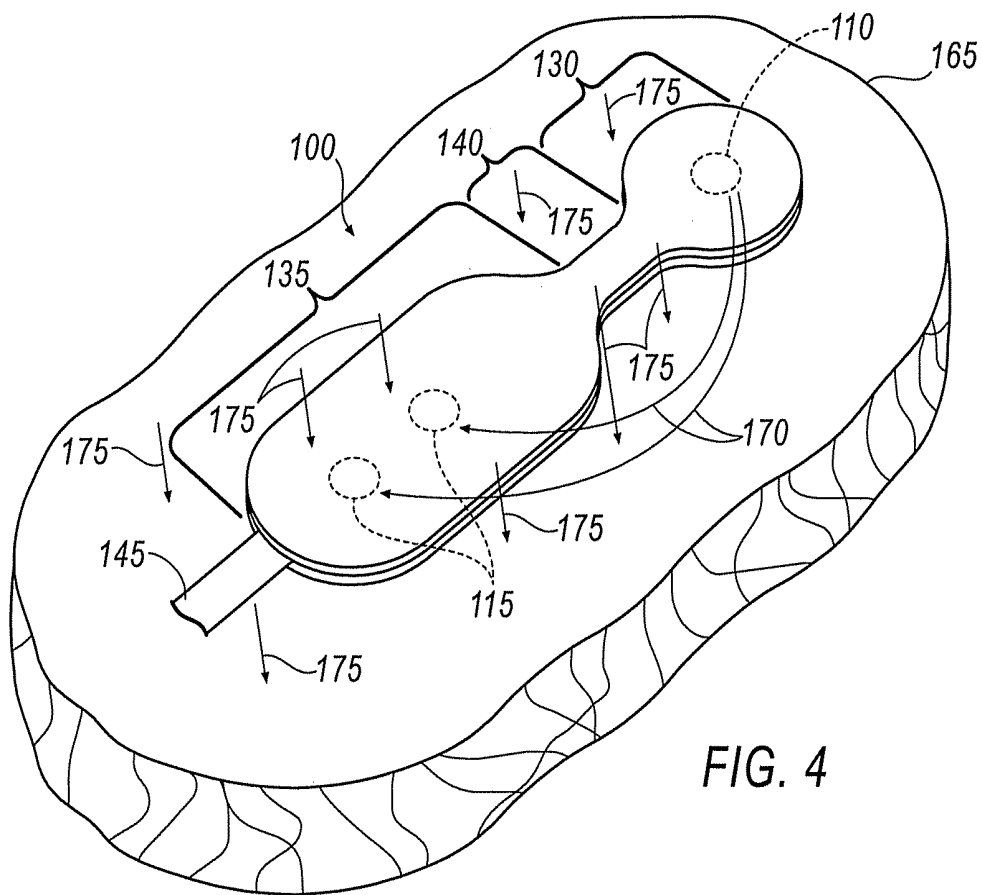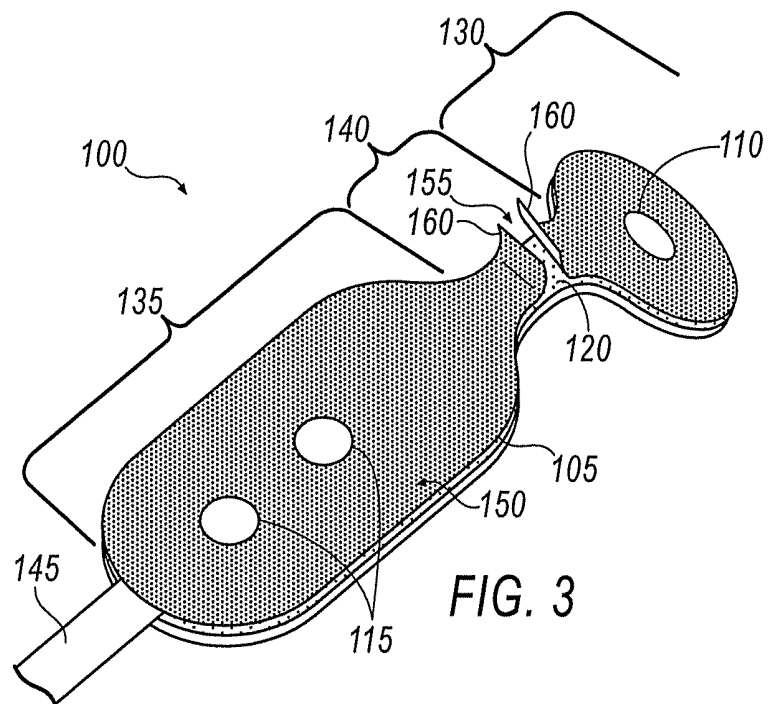

1

PHYSIOLOGICAL SENSOR HAVING A WAIST

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority to U.S. Ser. No. 61/228,086 filed Jul. 23, 2009, which is incorporated herein by reference in its entirety.

BACKGROUND

Near-infrared sensors are used in the medical industry to measure the amount of oxygen saturation in a patient's blood or tissue. These sensors work by detecting light after it has traveled through a portion of the patient's body. However, ambient or other light may interfere with the sensor, providing medical personnel with false readings that may lead to missed diagnoses and incorrect treatments. Existing solutions to blocking ambient light results in sensors that are bulky and expensive to manufacture. Moreover, these bulky sensors are not very flexible and cannot always conform to the contours of a patient's body. Accordingly, a physiological sensor is needed that protects against interference from ambient and other forms of light but is flexible enough to conform to the contours of the patient's body.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates an exemplary sensor having a sensor pad with a waist portion.

FIG. 2 illustrates an exemplary sensor having another sensor pad with a waist portion.

FIG. 3 illustrates an exemplary sensor having a liner disposed on the sensor pad.

FIG. 4 illustrates the exemplary sensor of FIG. 1 disposed on a patient.

DETAILED DESCRIPTION

An exemplary physiological sensor that blocks interfering light and provides sufficient flexibility includes a sensor pad having a first portion and a second portion separated by a waist portion. The waist portion is narrower than the first portion and the second portion. A light source disposed on the first portion is configured to generate near-infrared light and transmit the near-infrared light through part of a patient's body. A light detector disposed on the second portion is configured to detect near-infrared light that has traveled through the part of the patient's body. The near-infrared light detected indicates an amount of oxygen in the part of the patient's body through which the near-infrared light traveled.

FIG. 1 illustrates an exemplary sensor **100** that conforms to the contours of a patient's body and is able to prevent interference from ambient light. The sensor **100** may take many different forms and include multiple and/or alternate components and facilities. While an exemplary sensor **100** is shown in FIG. 1, the exemplary components illustrated in the figures are not intended to be limiting. Indeed, additional or alternative components and/or implementations may be used.

As illustrated in FIG. 1, the sensor **100** includes a sensor pad **105** housing a light source **110** and a light detector **115**. Of course, the sensor pad **105** may house any number of light sources **110** and light detectors **115**. Indeed, one light source **110** and two light detectors **115** are illustrated in FIG. 1. FIG. 2 illustrates a sensor **100** with two light sources **110** and two light detectors **115**. As illustrated in FIGS. 1 and 2, the sensor

2

100 may further include an adhesive **120** disposed on the sensor pad **105** and a connector **145**.

The sensor pad **105** may be formed from any material configured to house the light source **110** and light detector **115**. For instance, the sensor pad **105** may be formed from two or more layers **125** of a flexible material that sandwich one or more circuit boards (not shown) with the light source **110**, the light detector **115**, or both. At least one of the layers **125** may include a light blocking material. That is, one of the layers **125** may be opaque to ambient and other types of light that may interfere with the light detector **115**. When placed on a patient, one layer **125** is disposed on the patient's skin while the other layer **125** is spaced from the patient's skin. In one exemplary approach, the layer **125** spaced from the patient's skin includes the light blocking material. Of course, both layers **125** may include the light blocking material and the layer **125** disposed on the patient's skin may define openings in line with the light source **110** and light detector **115**. Further, one or both of the layers **125** may include a flexible material so that the sensor **100** may bend to fit the contours of the patient's body.

The sensor pad **105** may define a first portion **130** that may house the light source **110** and/or the light detector **115**, a second portion **135** that may house the light source **110** and/or the light detector **115**, and a waist portion **140** that separates the first portion **130** and the second portion **135**. The first portion **130**, the second portion **135**, and the waist portion **140** may be integrally formed with one another from the layers **125** of the sensor pad **105**. Additionally, the first portion **130**, the second portion **135**, the waist portion **140**, or any combination thereof, may include the light blocking material and/or the flexible material. In one exemplary approach, only the second portion **135** includes the light blocking material and only the waist portion **140** includes the flexible material. However, in the interest of reducing manufacturing complexity, each of the first portion **130**, the second portion **135**, and the waist portion **140** may include both the light blocking material and the flexible material.

The second portion **135** may have a larger surface area than the first portion **130** and the waist portion **140**. The larger surface area helps the sensor pad **105** block interfering light, such as ambient light. With the larger surface area, it is less likely that the light detector **115** will receive interfering light and provide false oximetry readings. Since the light source **110** does not need protection against interfering light, manufacturing the sensor **100** so that the first portion **130** has a smaller surface area than the second portion **135** results in reduced material costs. Alternatively, however, the second portion **135** and the first portion **130** may have the same surface area.

The waist portion **140** may be narrower than the first portion **130** and the second portion **135** to provide the sensor **100** with additional flexibility to fit the contours of the patient. In one exemplary implementation, the first portion **130** and the second portion **135** may gradually taper to the width of the waist portion **140**, thus providing a smooth transition between the first portion **130**, the waist portion **140**, and the second portion **135**. Alternatively, one or both of the first portion **130** and the second portion **135** may transition to the waist portion **140** more abruptly.

The light source **110** may include any device that is able to generate near-infrared light. For instance, the light source **110** may include a light emitting diode (LED) or a laser diode. Of course, the light source **110** may include additional or alternative devices. Further, the sensor **100** may include any num-

ber of light sources **110**. For example, as illustrated in FIG. **2**, the sensor **100** includes two light sources **110** within the first portion **130**.

The light detector **115** may include any device configured to detect near-infrared light. The light detector **115**, therefore, may include a photodiode. Any number of light detectors **115** may be disposed on the sensor pad **105**. As illustrated in FIGS. **1** and **2**, the sensor pad **105** houses two light detectors **115**.

The adhesive **120** is disposed on the layer **125** of the sensor pad **105** that will be disposed on the patient while the sensor **100** is in use. The adhesive **120** may include any adhesive **120** that is able to hold the sensor pad **105** in place relative to the patient's body. For example, the adhesive **120** may include a pressure sensitive adhesive **120**.

The connector **145** may extend from the sensor pad **105** and be used to control the light source **110** and light detector **115**. Moreover, the connector **145** may transmit signals representing the light received by the light detector **115** to a controller (not shown) for further processing.

FIG. **3** illustrates an exemplary sensor **100** having a liner **150** disposed on the adhesive **120**. The liner **150** may, for example, prevent the adhesive **120** from adhering the sensor pad **105** to unintended objects until the sensor **100** is ready to be placed on a patient. The liner **150** may be formed from any material that adheres to the adhesive **120** but will not significantly remove the adhesive **120** when the liner **150** is removed. The liner **150** may be formed from one or more pieces. For instance, in the exemplary approach of FIG. **3**, the liner **150** is formed from two pieces.

The liner **150** defines a slit **155** over the waist portion **140**. The slit **155** and flexibility of the waist portion **140** may allow a user of the sensor **100** to easily remove the liner **150**. For instance, the user may bend the waist portion **140** as illustrated in FIG. **3** to expose two tabs **160**. The user may further pull each tab **160** to remove each piece of the liner **150** from the sensor **100**. Removing the liner **150** exposes the adhesive **120**. With the liner **150** removed, the user may adhere the sensor **100** to the patient.

FIG. **4** illustrates the sensor **100** disposed on a patient. As illustrated, the near-infrared light **170** from the light source **110** is transmitted through blood or tissue and is received by the light detector **115**. The light detector **115** generates a signal that indicates the oxygen saturation of the blood or tissue through which the light **170** traveled. The second portion **135** of the sensor pad **105** has a larger surface area than the first portion **130**. While some interfering light **175** such as ambient light may travel through the tissue, the large surface area of the second portion **135** reduces the amount of interfering light **175** that is received by the sensor **100**. FIG. **4** further illustrates the waist portion **140** that is narrower than the first portion **130** and the second portion **135**. This gives the sensor **100** additional flexibility to fit the contours of the patient's body.

With regard to the processes, systems, methods, heuristics, etc. described herein, it should be understood that, although the steps of such processes, etc. have been described as occurring according to a certain ordered sequence, such processes could be practiced with the described steps performed in an order other than the order described herein. It further should be understood that certain steps could be performed simultaneously, that other steps could be added, or that certain steps described herein could be omitted. In other words, the descriptions of processes herein are provided for the purpose of illustrating certain embodiments, and should in no way be construed so as to limit the claimed invention.

Accordingly, it is to be understood that the above description is intended to be illustrative and not restrictive. Many embodiments and applications other than the examples provided would be apparent upon reading the above description. The scope of the invention should be determined, not with reference to the above description, but should instead be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled. It is anticipated and intended that future developments will occur in the technologies discussed herein, and that the disclosed systems and methods will be incorporated into such future embodiments. In sum, it should be understood that the invention is capable of modification and variation.

All terms used in the claims are intended to be given their broadest reasonable constructions and their ordinary meanings as understood by those knowledgeable in the technologies described herein unless an explicit indication to the contrary is made herein. In particular, use of the singular articles such as "a," "the," "said," etc. should be read to recite one or more of the indicated elements unless a claim recites an explicit limitation to the contrary.

The invention claimed is:

1. A sensor comprising:

an integrated sensor pad having a first portion and a second portion separated by a waist portion, wherein the waist portion is narrower than the first portion and the second portion, and wherein said sensor pad is configured to be adhered to a patient's body by an adhesive disposed directly on an underside of said sensor pad;

a light source at least partially housed within said sensor pad and configured to generate near-infrared light and transmit the near-infrared light through part of a patient's body; and

a light detector at least partially housed within said sensor pad and configured to detect near-infrared light that has traveled through the part of the patient's body, wherein the near-infrared light detected indicates an amount of oxygen in the part of the patient's body through which the near-infrared light traveled.

2. A sensor as set forth in claim 1, wherein the second portion is configured to substantially prevent the light detector from receiving interfering light.

3. A sensor as set forth in claim 1, wherein at least one of the first portion, the waist portion, and the second portion includes a light blocking material.

4. A sensor as set forth in claim 1, further comprising a liner disposed on the adhesive.

5. A sensor as set forth in claim 4, wherein the liner defines a slit.

6. A sensor as set forth in claim 5, wherein the slit is located over the waist portion to facilitate removal of the liner.

7. A sensor as set forth in claim 1, wherein at least one of the first portion, the second portion, and the waist portion includes a flexible material.

8. A sensor as set forth in claim 1, wherein the light detector is disposed on the second portion and wherein the second portion has a larger surface area than the first portion.

9. A sensor as set forth in claim 1, wherein the sensor pad is formed from multiple layers having generally the same size and shape and forming the first portion, the second portion, and the waist portion.

10. A sensor pad comprising:

a first portion configured to house a light source that generates near-infrared light and transmits the near-infrared light through a part of a patient's body;

a second portion configured to house a light detector that detects near-infrared light after the near-infrared light

5

has traveled through a part of the patient's body, wherein the light received indicates oxygen saturation of the part of the patient's body through which the light traveled; and

a waist portion disposed between the first portion and the second portion, wherein the surface area of the second portion is larger than the surface area of the first portion and the waist portion is narrower than the first portion and the second portion.

11. A sensor pad as set forth in claim 10, wherein the second portion includes a light blocking material that substantially prevents the light detector from receiving interfering light.

12. A sensor pad as set forth in claim 10, wherein at least one of the first portion and the waist portion include a light blocking material.

13. A sensor pad as set forth in claim 10, wherein the waist portion includes a flexible material.

14. A sensor pad as set forth in claim 10, wherein at least one of the first portion and the second portion includes a flexible material.

15. A sensor pad as set forth in claim 10, further comprising an adhesive disposed on an underside of the first portion and the second portion.

16. A sensor pad as set forth in claim 15, further comprising a liner disposed on the adhesive.

17. A sensor pad as set forth in claim 16, wherein the liner defines a slit located over the waist portion to facilitate removal of the liner.

18. A sensor pad as set forth in claim 10, wherein said sensor pad comprises a plurality of layers and each of the layers is substantially the same size and shape.

6

19. A sensor comprising:

an integrated sensor pad assembly having a plurality of layers having generally the same size and shape and forming a first portion and a second portion separated by a waist portion, wherein the waist portion is narrower than the first portion and the second portion, the second portion including a light blocking material and the waist portion including a flexible material;

a light source disposed on the first portion and configured to generate near-infrared light and transmit the near-infrared light through a part of a patient's body;

a light detector disposed on the second portion and configured to detect near-infrared light that has traveled through part of the patient's body to identify an amount of oxygen in the part of the patient's body through which the near-infrared light traveled, and wherein the second portion substantially prevents the light detector from receiving interfering light;

an adhesive disposed directly on the sensor pad; and a liner disposed on the adhesive and defining a slit located near or over the waist portion.

20. A sensor as set forth in claim 19, wherein at least one of the first portion, the second portion, and the waist portion includes a flexible material.

21. A sensor as set forth in claim 19, wherein the second portion of the sensor pad assembly has a larger surface area than the first portion.

22. A sensor as set forth in claim 19, wherein said first portion has a surface area that is smaller than the surface area of the second portion.

* * * * *

专利名称(译)	具有腰部的生理传感器		
公开(公告)号	US8670812	公开(公告)日	2014-03-11
申请号	US12/842801	申请日	2010-07-23
[标]申请(专利权)人(译)	GONOPOLSKIY OLEG 阿里克·安德森 MUTO MELISSA MORBITO RICHARD 斯廷普森MATTHEW		
申请(专利权)人(译)	GONOPOLSKIY OLEG 阿里克·安德森 MUTO MELISSA MORBITO RICHARD 斯廷普森MATTHEW		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	GONOPOLSKIY OLEG ANDERSON ARIK MUTO MELISSA MORBITO RICHARD STIMPSON MATTHEW		
发明人	GONOPOLSKIY, OLEG ANDERSON, ARIK MUTO, MELISSA MORBITO, RICHARD STIMPSON, MATTHEW		
IPC分类号	A61B5/00		
CPC分类号	A61B2562/164 A61B5/14552 A61B5/6833		
优先权	61/228086 2009-07-23 US		
其他公开文献	US20110021893A1		
外部链接	Espacenet USPTO		

摘要(译)

示例性传感器包括传感器垫，该传感器垫具有由腰部分开的第一部分和第二部分。腰部比第一部分和第二部分窄。设置在第一部分上的光源被配置为产生近红外光并通过患者身体的一部分传输近红外光。设置在第二部分上的光检测器被配置为检测已经穿过患者身体的一部分的近红外光。检测到的近红外光表示近红外光通过的患者身体部位的氧气量。

