



US006813511B2

(12) **United States Patent**
Diab et al.(10) **Patent No.: US 6,813,511 B2**(45) **Date of Patent: Nov. 2, 2004**(54) **LOW-NOISE OPTICAL PROBES FOR
REDUCING AMBIENT NOISE**(75) Inventors: **Mohamed Diab**, Mission Viejo, CA
(US); **Esmail Kiani-Azarbayjany**,
Laguna Niguel, CA (US); **David R.**
Tobler, Westminster, CO (US);
Thomas J. Gerhardt, Littleton, CO
(US); **Eugene E. Mason**, Boulder, CO
(US); **Mike A. Mills**, Golden, CO (US)(73) Assignee: **Masimo Corporation**, Irvine, CA (US)(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.(21) Appl. No.: **10/260,049**(22) Filed: **Sep. 27, 2002**(65) **Prior Publication Data**

US 2003/0045785 A1 Mar. 6, 2003

Related U.S. Application Data(63) Continuation of application No. 09/898,990, filed on Jul. 3,
2001, which is a continuation of application No. 09/094,202,
filed on Jun. 9, 1998, now Pat. No. 6,256,523, which is a
continuation of application No. 08/543,789, filed on Oct. 16,
1995, now Pat. No. 5,782,757, which is a continuation-in-
part of application No. 08/333,132, filed on Nov. 1, 1994,
now Pat. No. 5,638,818, which is a continuation-in-part of
application No. 07/672,890, filed on Mar. 21, 1991, now
abandoned.(51) **Int. Cl.⁷** **A61B 5/00**(52) **U.S. Cl.** **600/344; 600/310**(58) **Field of Search** 600/310, 322,
600/323, 340, 344(56) **References Cited****U.S. PATENT DOCUMENTS**2,567,926 A 9/1951 Dunkelberger
3,103,214 A 9/1963 Smith
3,463,142 A 8/1969 Harte3,482,565 A 12/1969 Gowen
3,704,706 A 12/1972 Herczfeld et al.
4,129,124 A 12/1978 Thalmann
4,321,930 A 3/1982 Jobsis et al.
4,334,544 A 6/1982 Hill et al.
4,350,165 A 9/1982 Striese
4,380,240 A 4/1983 Jobsis et al.
4,406,289 A 9/1983 Wesseling et al.
4,528,986 A 7/1985 Arundel et al.
4,621,643 A 11/1986 New, Jr. et al.
4,685,464 A 8/1987 Goldberger et al.
4,700,708 A 10/1987 New, Jr. et al.
4,824,242 A 4/1989 Frick et al.
4,825,872 A 5/1989 Tan et al.
4,825,879 A 5/1989 Tan et al.
4,830,014 A 5/1989 Goodman et al.
4,859,057 A 8/1989 Taylor et al.
4,865,038 A 9/1989 Rich et al.
4,867,165 A 9/1989 Noller

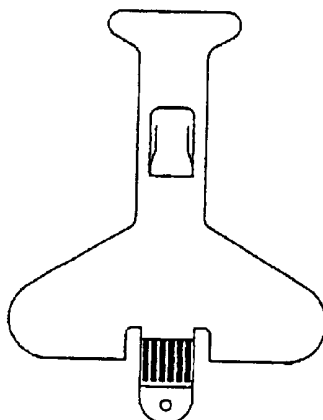
(List continued on next page.)

FOREIGN PATENT DOCUMENTSEP 074428 3/1983
EP 89/105503 8/1983
EP 104772 4/1984
EP 404562 12/1990
WO 01894 3/1992
WO 92/01894 6/1992**OTHER PUBLICATIONS**

US 4,928,691, 5/1990, Nicolson et al. (withdrawn)

Primary Examiner—Eric F. Winakur(74) *Attorney, Agent, or Firm*—Knobbe, Martens, Olson &
Bear, LLP(57) **ABSTRACT**

An optical probe, which is particularly suited to reduce noise
in measurements taken on an easily compressible material,
such as a finger, a toe, a forehead, an earlobe, or a lip,
measures characteristics of the material. A neonatal and
adult disposable embodiment of the probe include adhesive
coated surfaces to securely affix the probe onto the patient.
In addition, the surface of the probe is specially constructed
to reduce the effect of ambient noise.

41 Claims, 34 Drawing Sheets

U.S. PATENT DOCUMENTS

4,880,304 A	11/1989	Jaeb et al.	6,036,642 A	3/2000	Diab et al.
4,907,594 A	3/1990	Muz	6,067,462 A	5/2000	Diab et al.
4,913,150 A	4/1990	Cheung et al.	6,081,735 A	6/2000	Diab et al.
4,927,264 A	5/1990	Shiga et al.	6,088,607 A	7/2000	Diab et al.
4,938,218 A	7/1990	Goodman et al.	6,110,522 A	8/2000	Lepper, Jr. et al.
4,964,408 A	10/1990	Hink et al.	6,151,516 A	11/2000	Kiani-Azarbayjany et al.
4,974,591 A	12/1990	Awazu et al.	6,152,754 A	11/2000	Gerhardt et al.
5,031,608 A	7/1991	Weinstein	6,157,850 A	12/2000	Diab et al.
5,058,588 A	10/1991	Kaestle	6,165,005 A	12/2000	Mills et al.
5,080,098 A	1/1992	Willett et al.	6,184,521 B1	2/2001	Coffin, IV et al.
5,086,229 A	2/1992	Rosenthal et al.	6,206,830 B1	3/2001	Diab et al.
5,099,842 A	3/1992	Mannheimer et al.	6,229,856 B1	5/2001	Diab et al.
5,109,848 A	5/1992	Thomas et al.	6,236,872 B1	5/2001	Diab et al.
5,109,849 A	5/1992	Goodman et al.	6,256,523 B1	7/2001	Diab et al.
5,125,403 A	6/1992	Culp	6,263,222 B1	7/2001	Diab et al.
5,170,786 A	12/1992	Thomas et al.	6,278,522 B1	8/2001	Lepper, Jr. et al.
5,217,013 A	6/1993	Lewis et al.	6,280,213 B1	8/2001	Tobler et al.
5,224,478 A	7/1993	Sakai et al.	6,285,896 B1	9/2001	Tobler et al.
5,226,417 A *	7/1993	Swedlow et al. 600/322	6,334,065 B1	12/2001	Al-Ali et al.
5,246,003 A	9/1993	DeLonzor	6,349,228 B1	2/2002	Kiani et al.
5,337,744 A	8/1994	Branigan	6,360,114 B1	3/2002	Diab et al.
5,390,670 A	2/1995	Centa et al.	6,371,921 B1	4/2002	Caro et al.
5,452,717 A	9/1995	Branigan et al.	6,377,829 B1	4/2002	Al-Ali
5,469,845 A	11/1995	DeLonzor et al.	6,388,240 B2	5/2002	Schulz et al.
5,482,036 A	1/1996	Diab et al.	6,397,091 B2	5/2002	Diab et al.
5,490,505 A	2/1996	Diab et al.	6,430,525 B1	8/2002	Weber et al.
5,520,177 A	5/1996	Ogawa et al.	6,470,199 B1	10/2002	Kopotic et al.
5,584,296 A	12/1996	Cui et al.	6,501,975 B2	12/2002	Diab et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	6,515,273 B2	2/2003	Al-Ali
5,638,818 A	6/1997	Diab et al.	6,525,386 B1	2/2003	Mills et al.
5,645,440 A	7/1997	Tobler et al.	6,526,300 B1	2/2003	Kiani et al.
5,685,299 A	11/1997	Diab et al.	6,541,756 B2	4/2003	Schulz et al.
D393,830 S	4/1998	Tobler et al.	6,542,764 B1	4/2003	Al-Ali et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,580,086 B1	6/2003	Schulz et al.
5,758,644 A	6/1998	Diab et al.	6,584,336 B1	6/2003	Ali et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,597,933 B2	7/2003	Kiani et al.
5,769,785 A	6/1998	Diab et al.	6,606,511 B1	8/2003	Ali et al.
5,782,757 A	7/1998	Diab et al.	6,632,181 B2	10/2003	Flaherty et al.
5,823,950 A	10/1998	Diab et al.	6,640,116 B2	10/2003	Diab
RE36,000 E	12/1998	Swedlow et al.	6,643,530 B2	11/2003	Diab et al.
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,650,917 B2	11/2003	Diab et al.
5,890,929 A	4/1999	Mills et al.	6,654,624 B2	11/2003	Diab et al.
5,919,134 A	7/1999	Diab	6,658,277 B2	12/2003	Diab et al.
5,934,925 A	8/1999	Tobler et al.	6,671,531 B2	12/2003	Al-Ali et al.
5,940,182 A	8/1999	Lepper, Jr. et al.	6,678,543 B2	1/2004	Diab et al.
5,995,855 A	11/1999	Kiani et al.	6,684,090 B2	1/2004	Ali et al.
5,997,343 A	12/1999	Mills et al.	6,697,656 B1	2/2004	Al-Ali
6,002,952 A	12/1999	Diab et al.	6,697,658 B2	2/2004	Al-Ali
6,011,986 A	1/2000	Diab et al.	6,699,194 B1	3/2004	Diab et al.

* cited by examiner

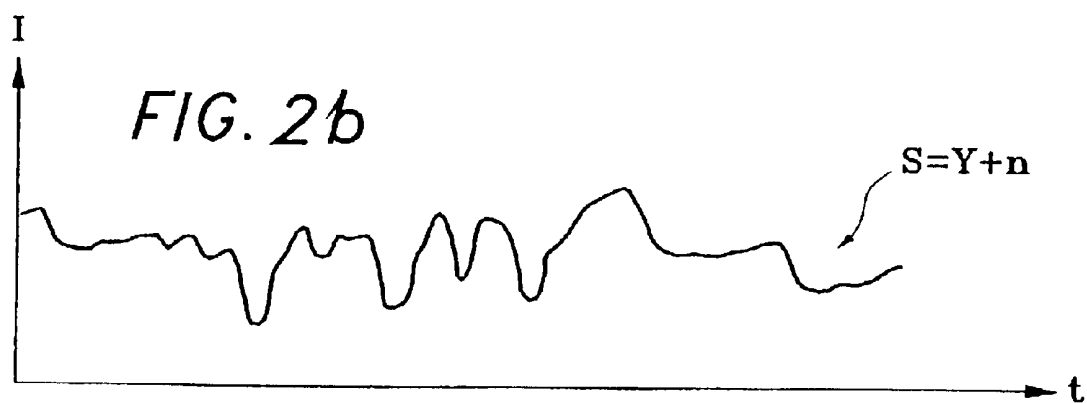
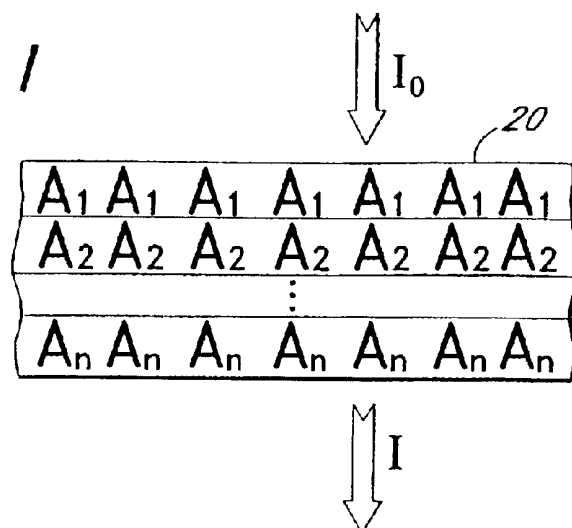
FIG. 1

FIG. 3

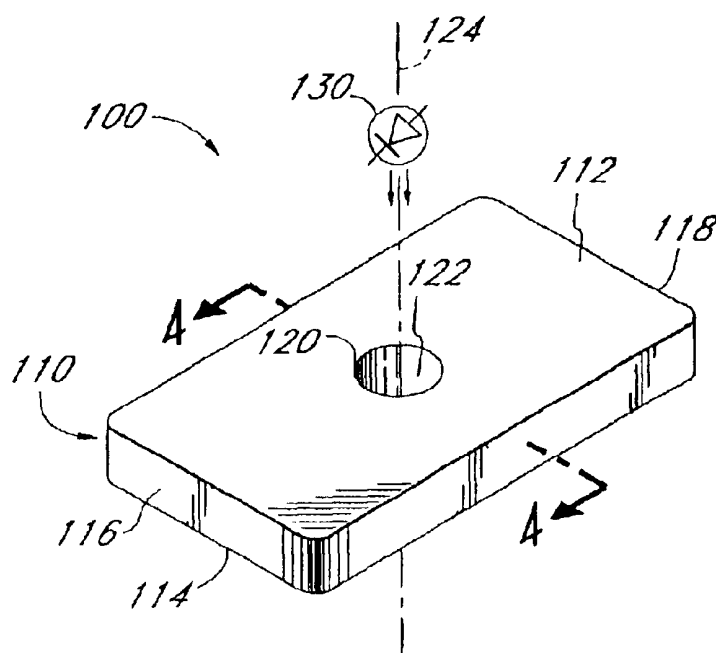


FIG. 4

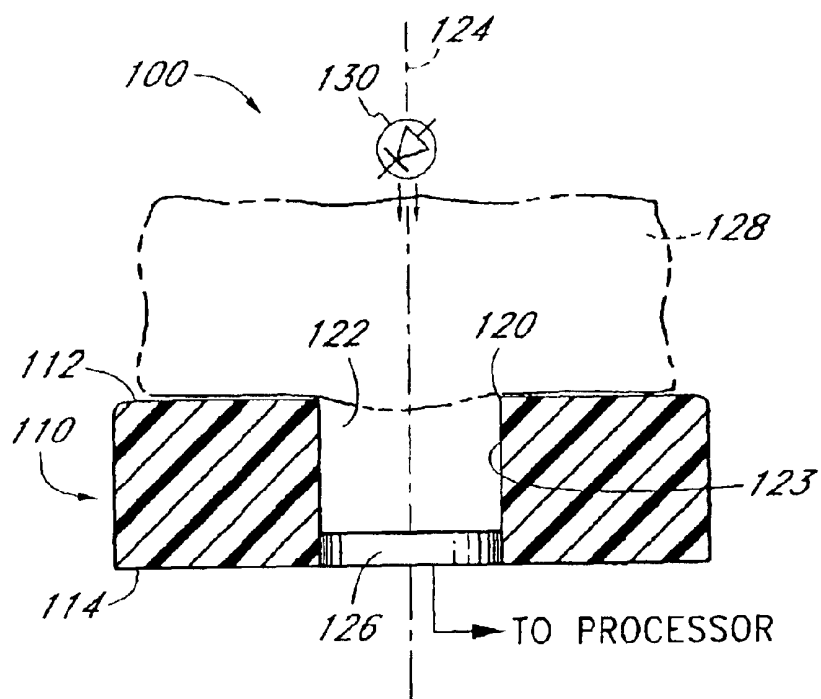


FIG. 5

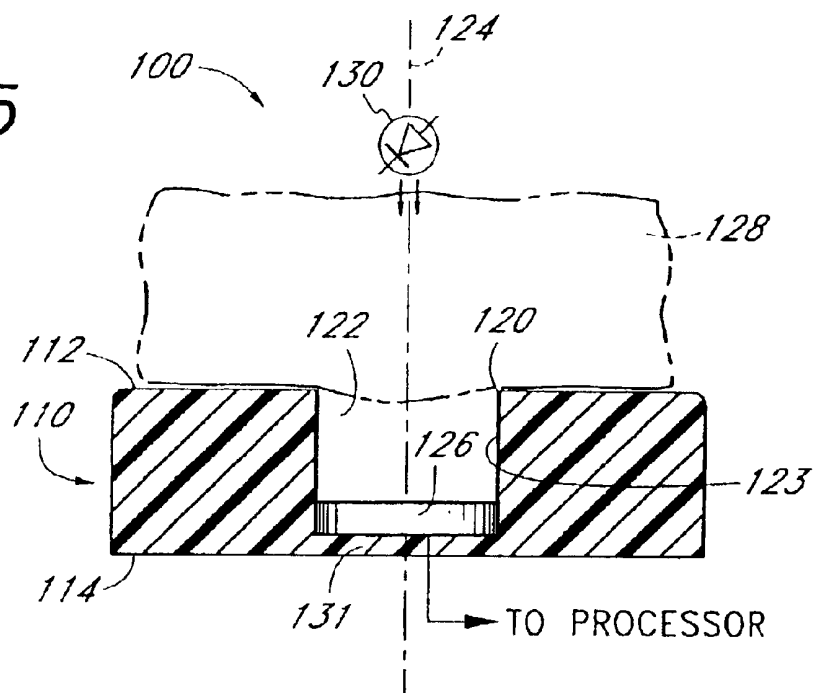
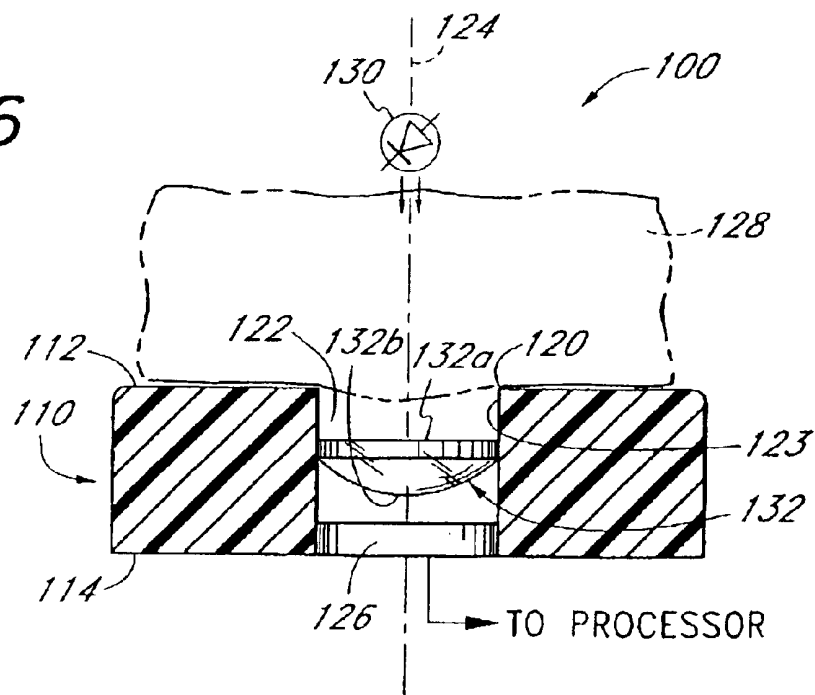


FIG. 6



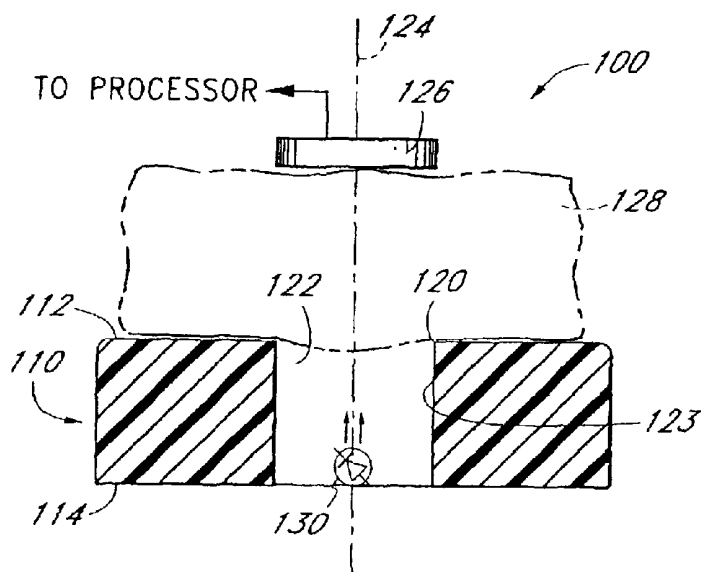


FIG. 7

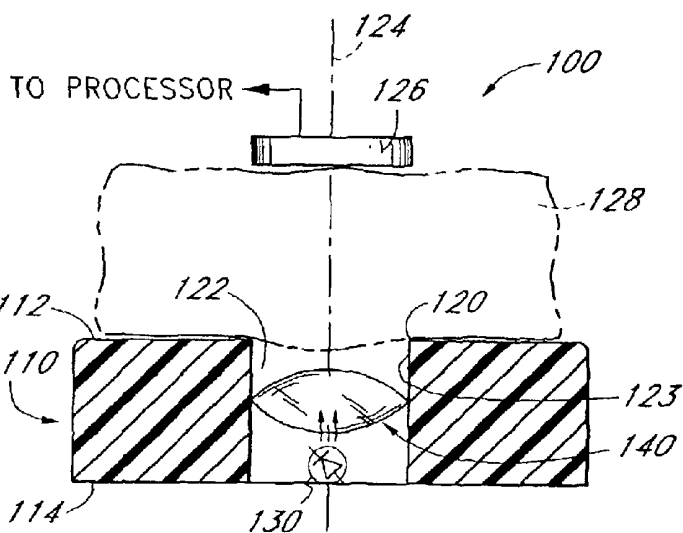
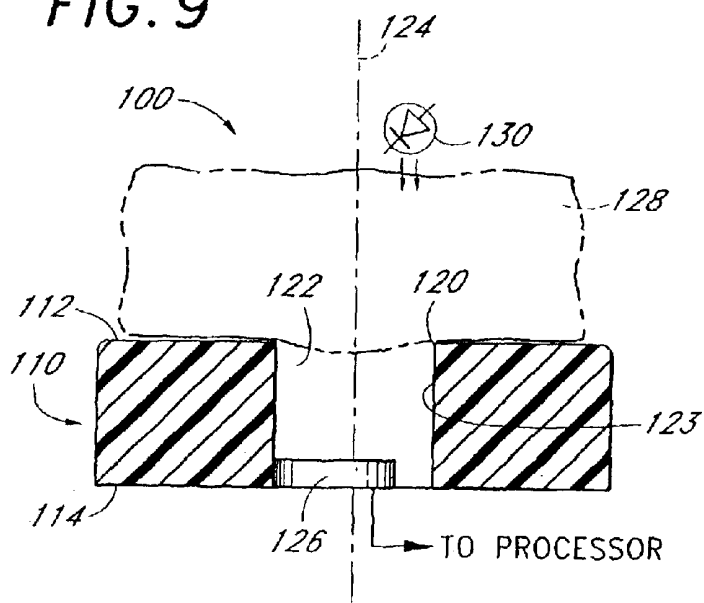


FIG. 8



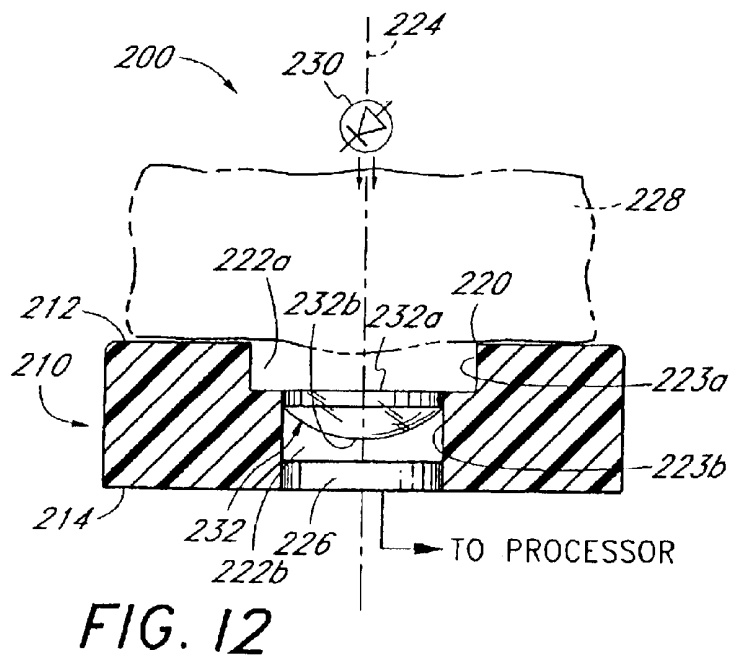
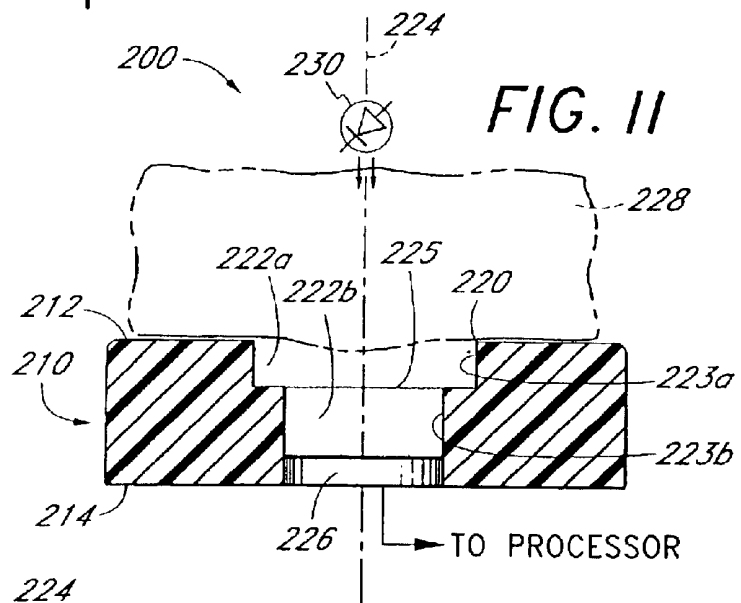
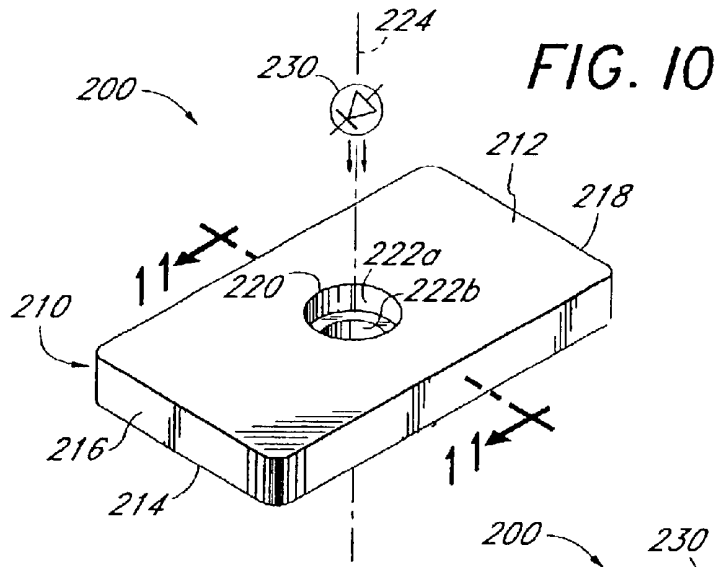


FIG. 13

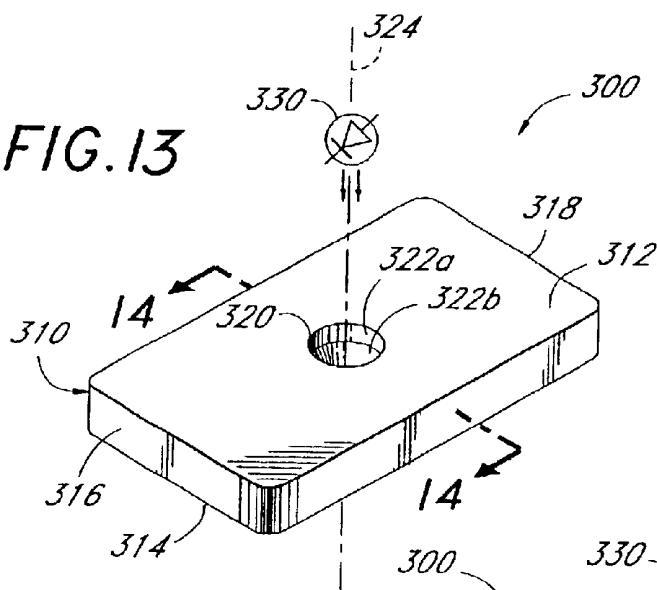


FIG. 14

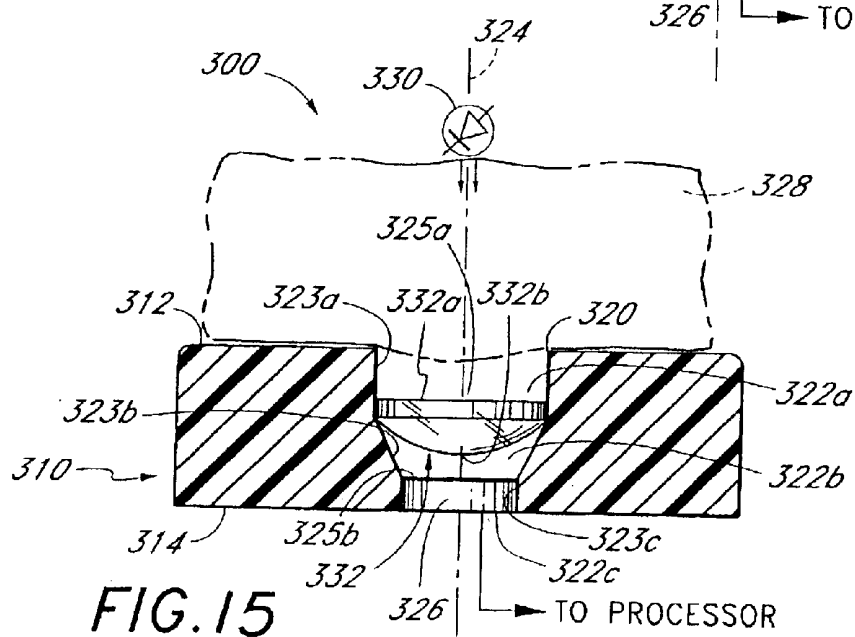
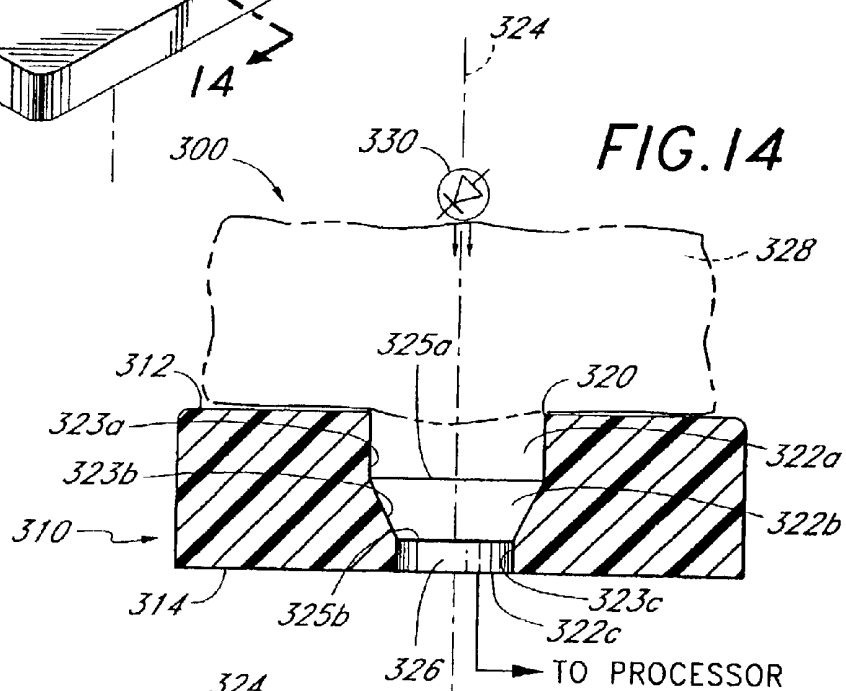


FIG. 16

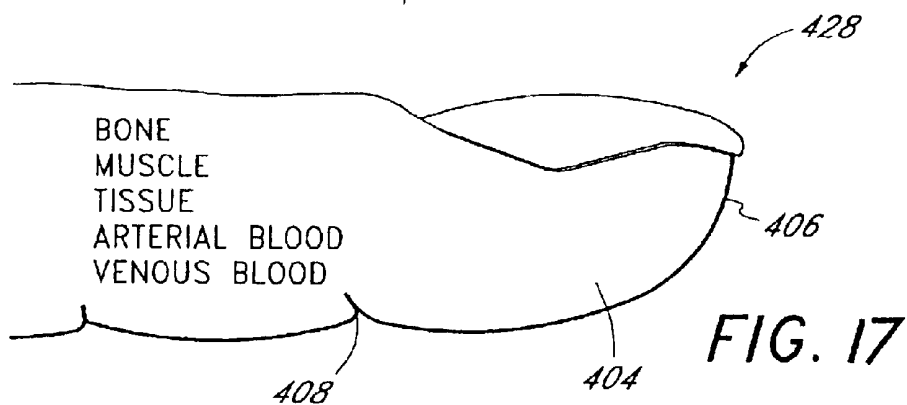
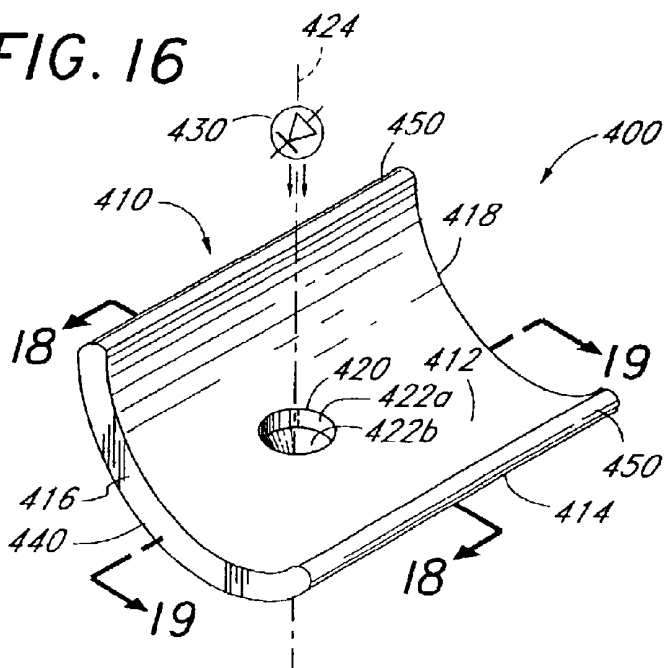


FIG. 17

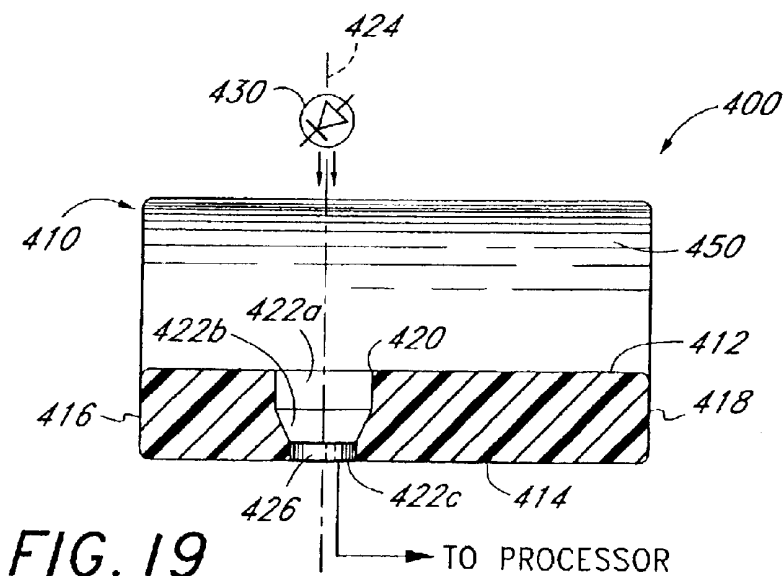


FIG. 19

FIG. 18

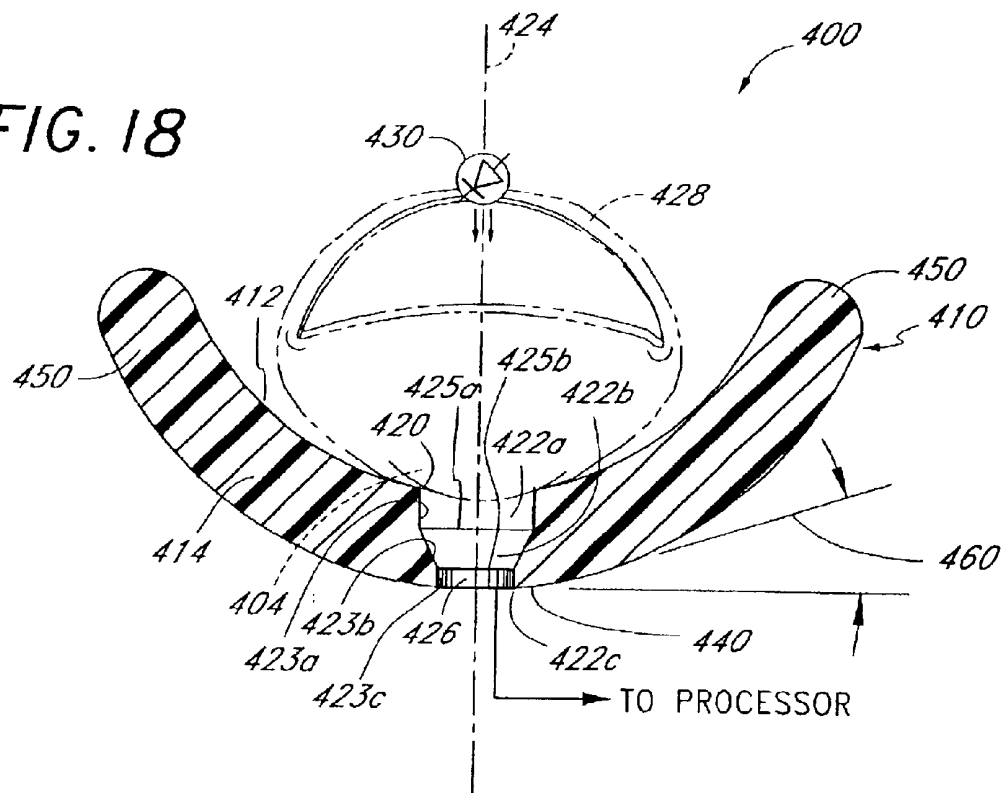


FIG. 20

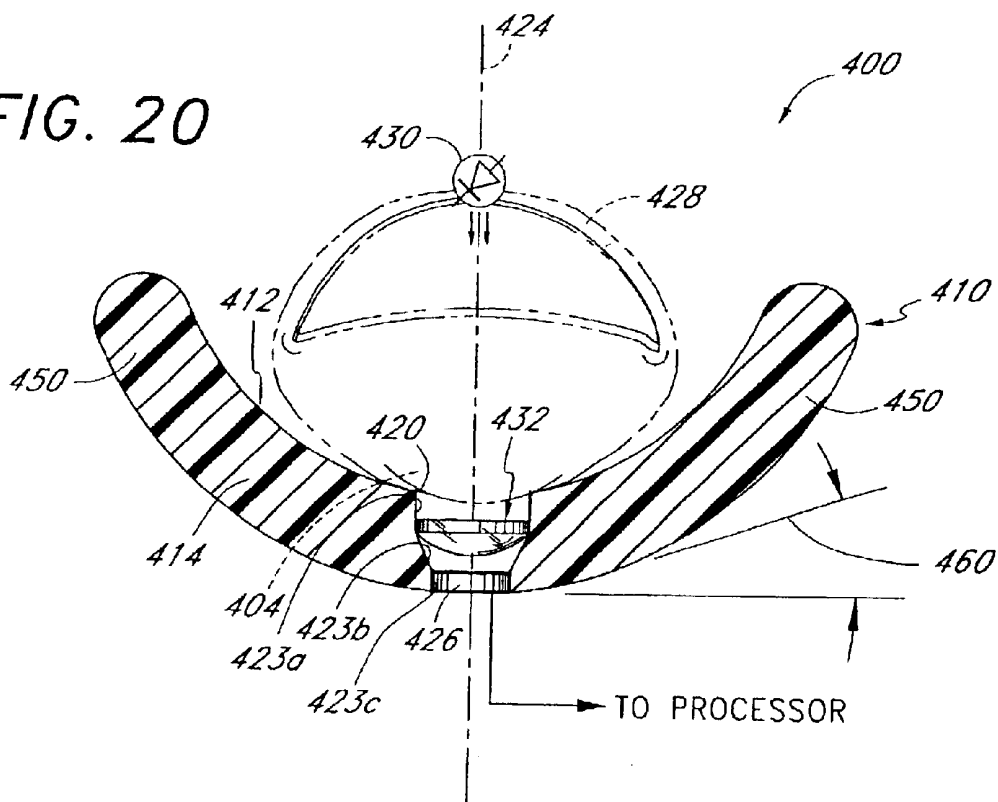


FIG. 21

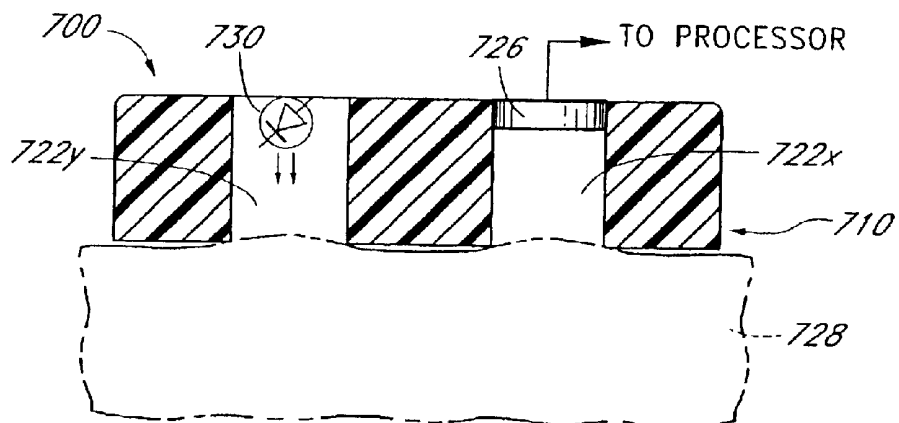


FIG. 22

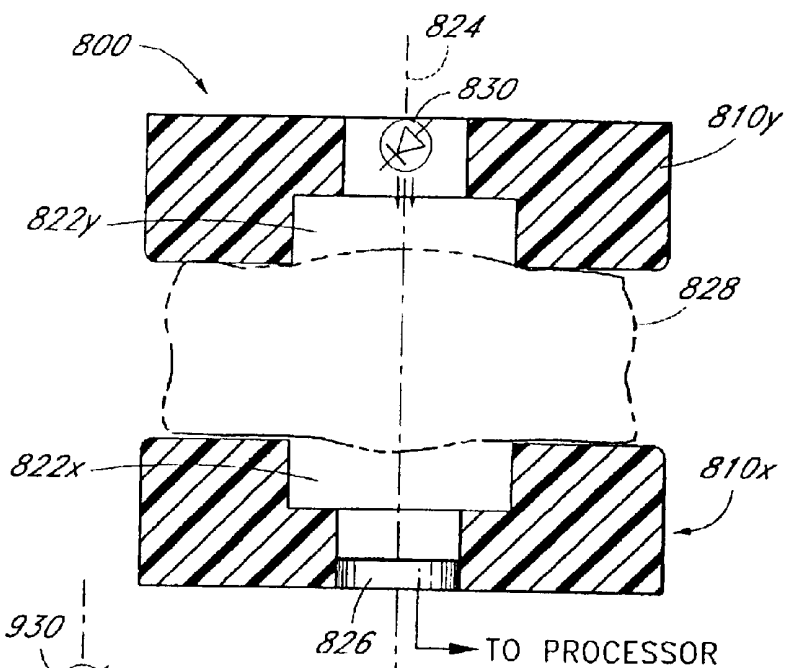
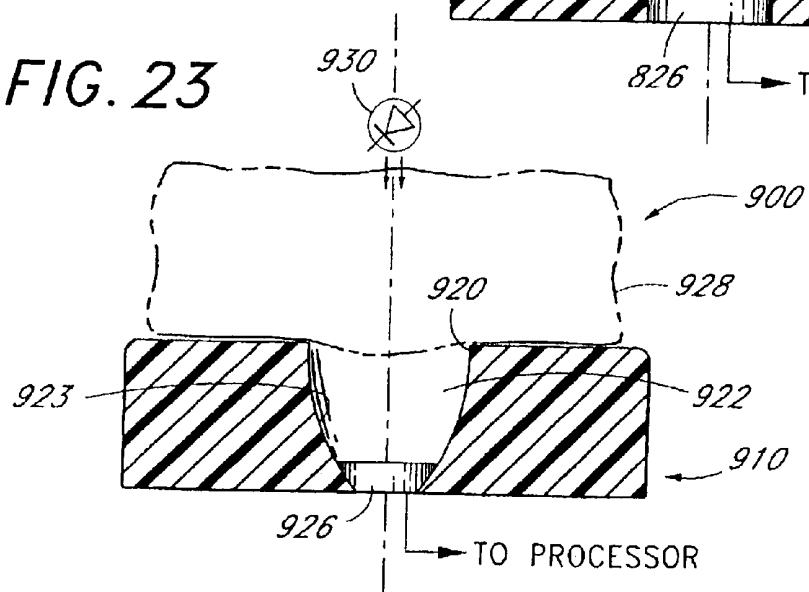
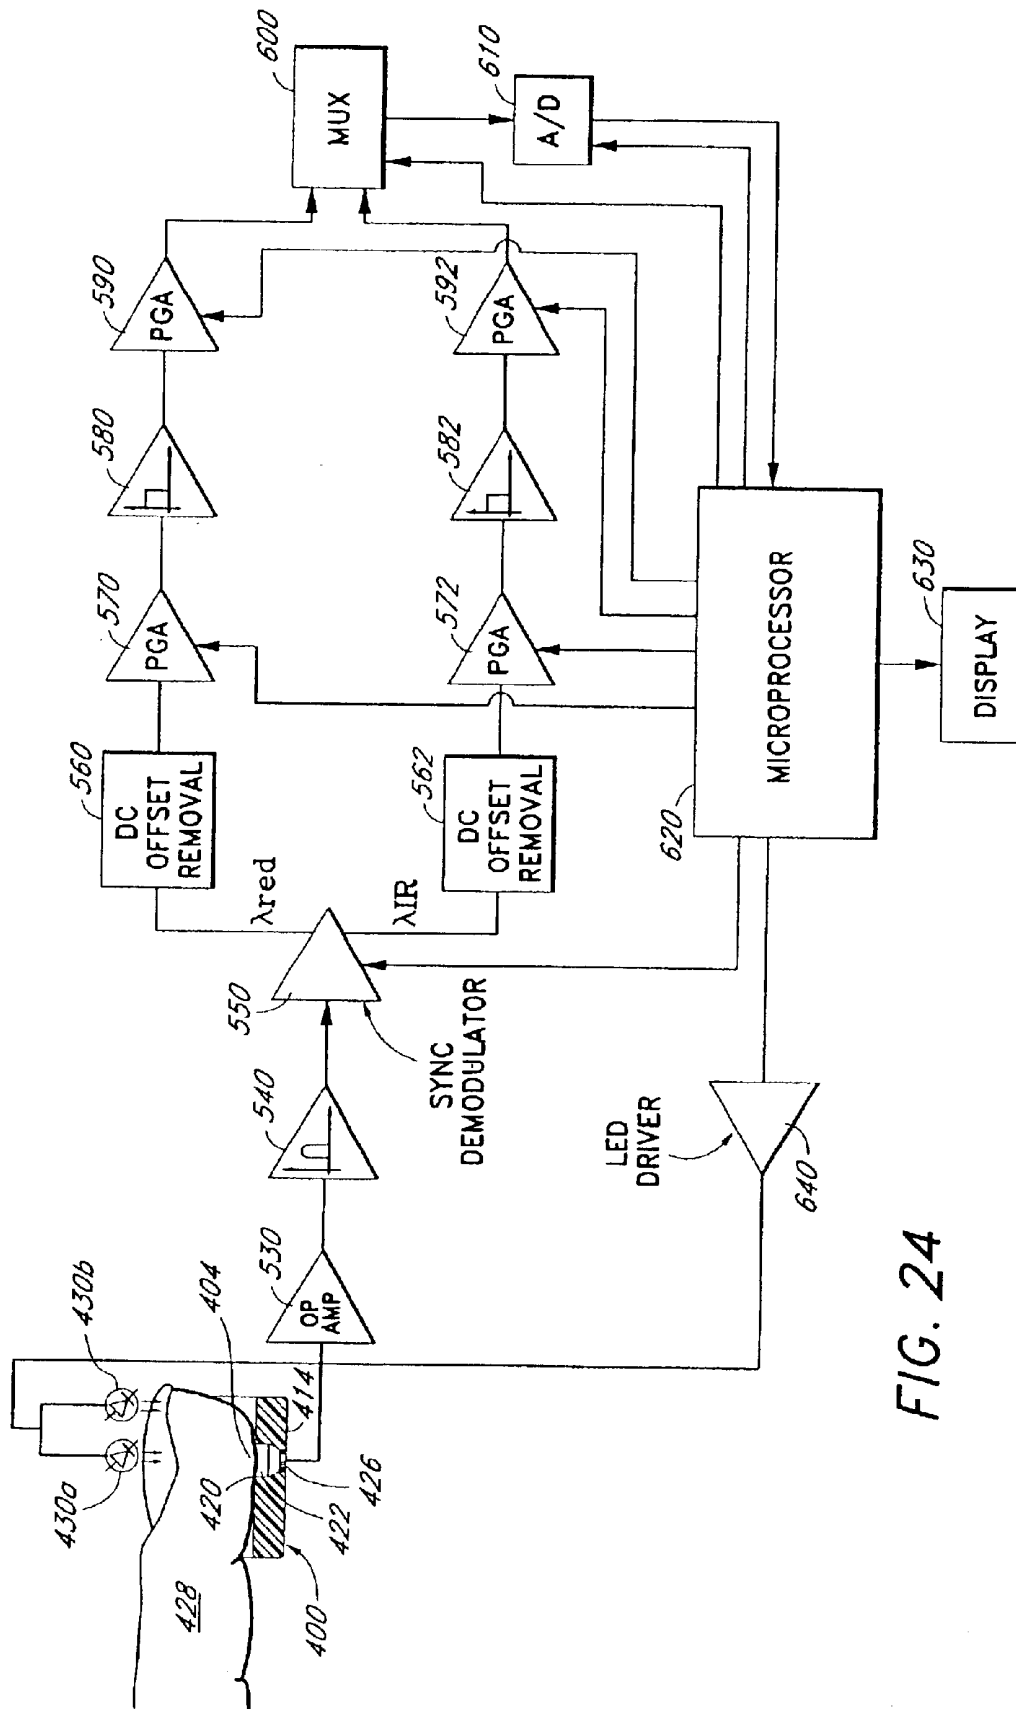


FIG. 23





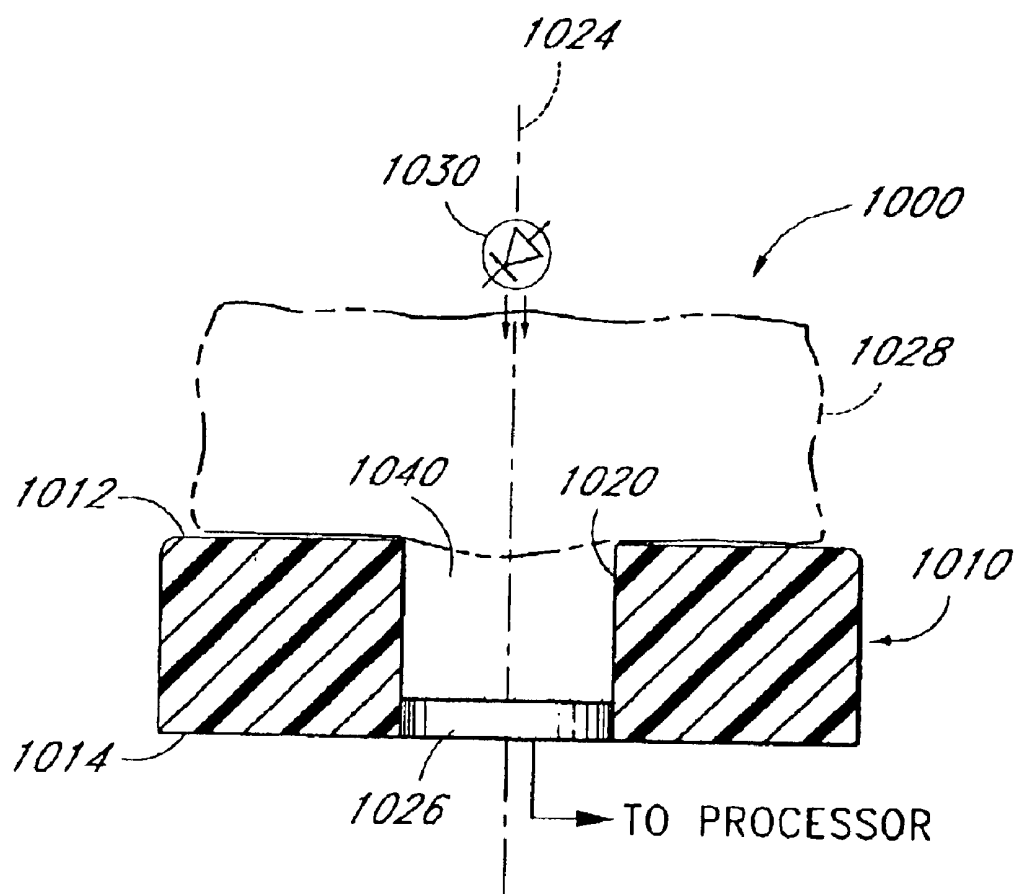
*FIG. 25*

FIG. 26

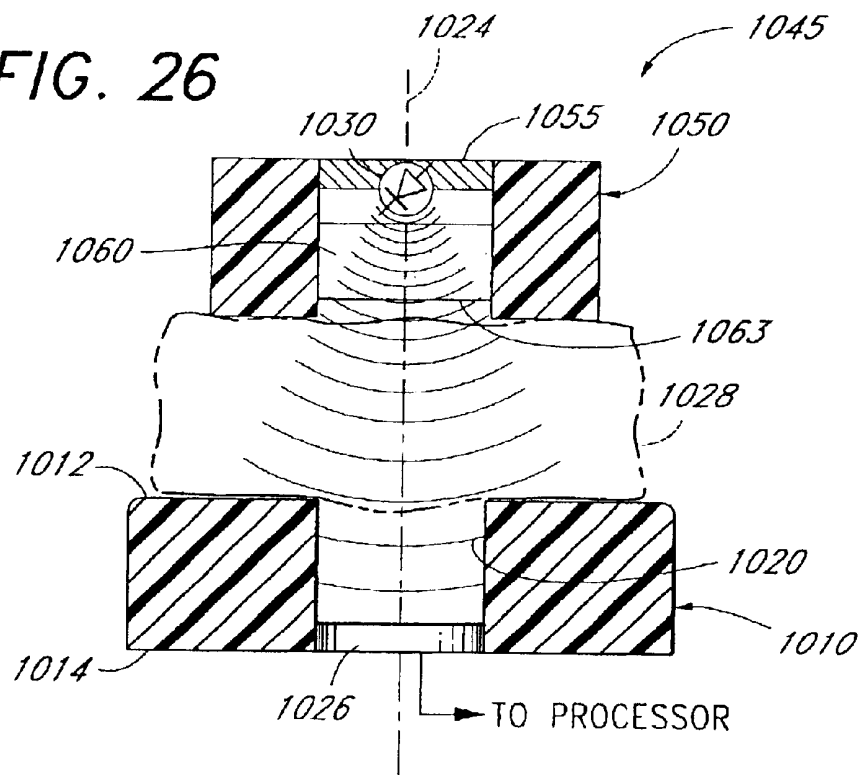
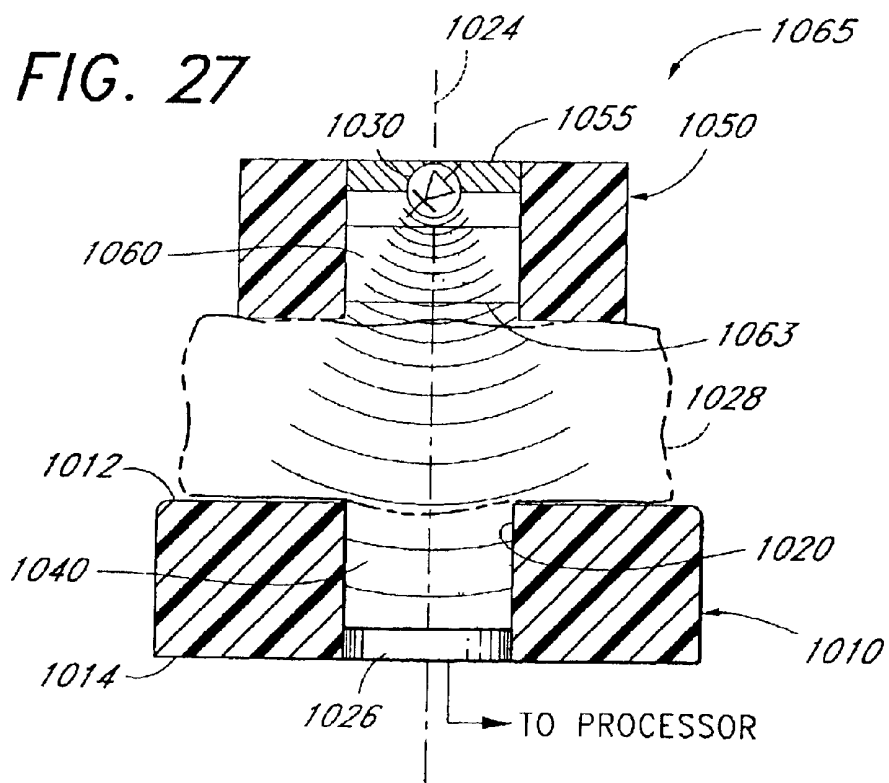


FIG. 27



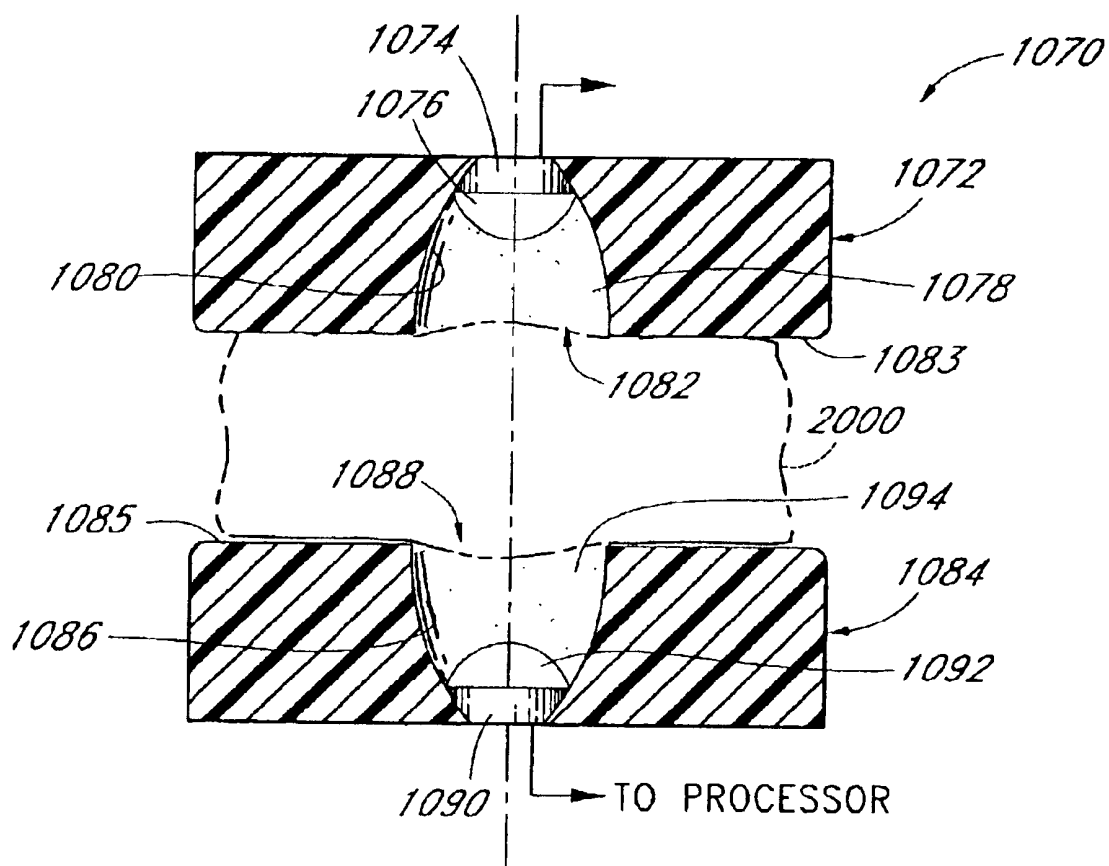


FIG. 28

FIG. 29A

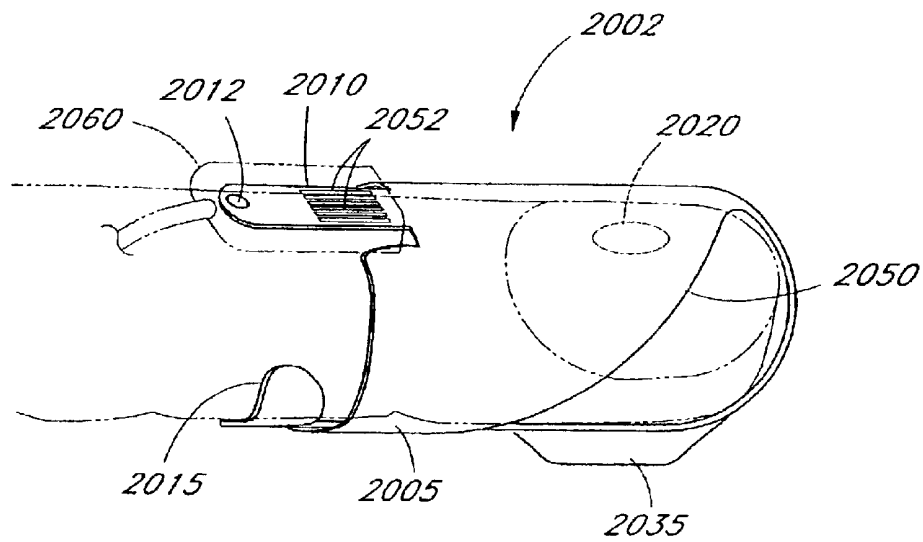
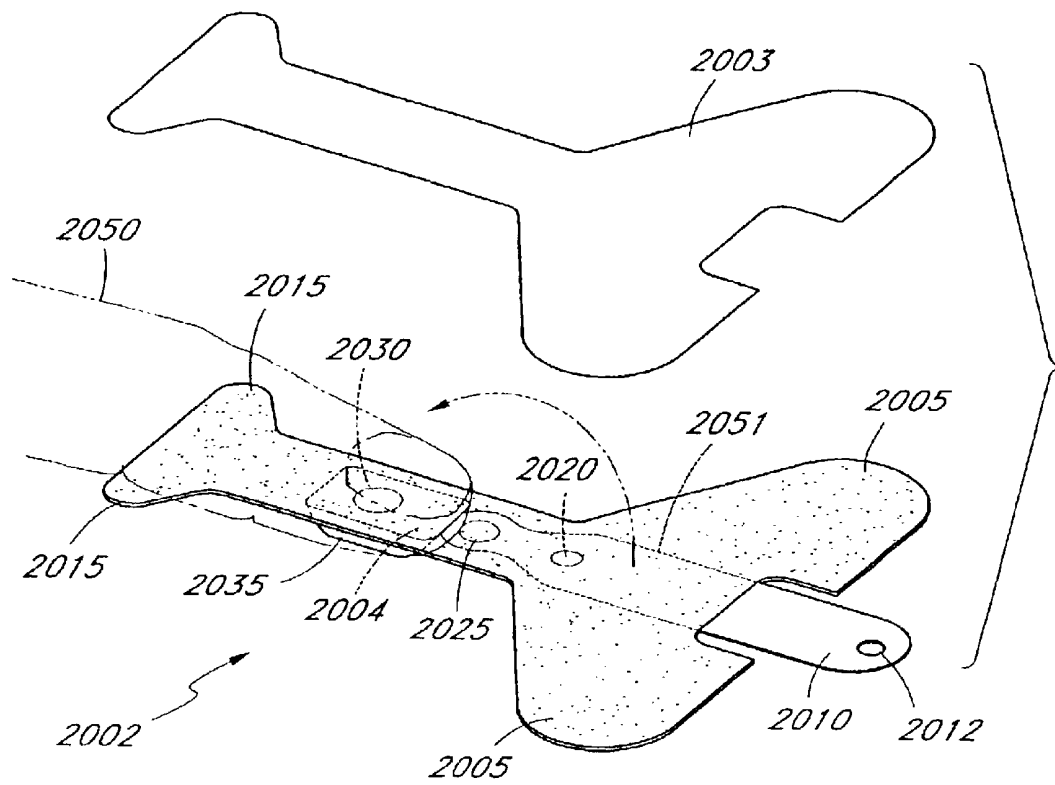


FIG. 29B

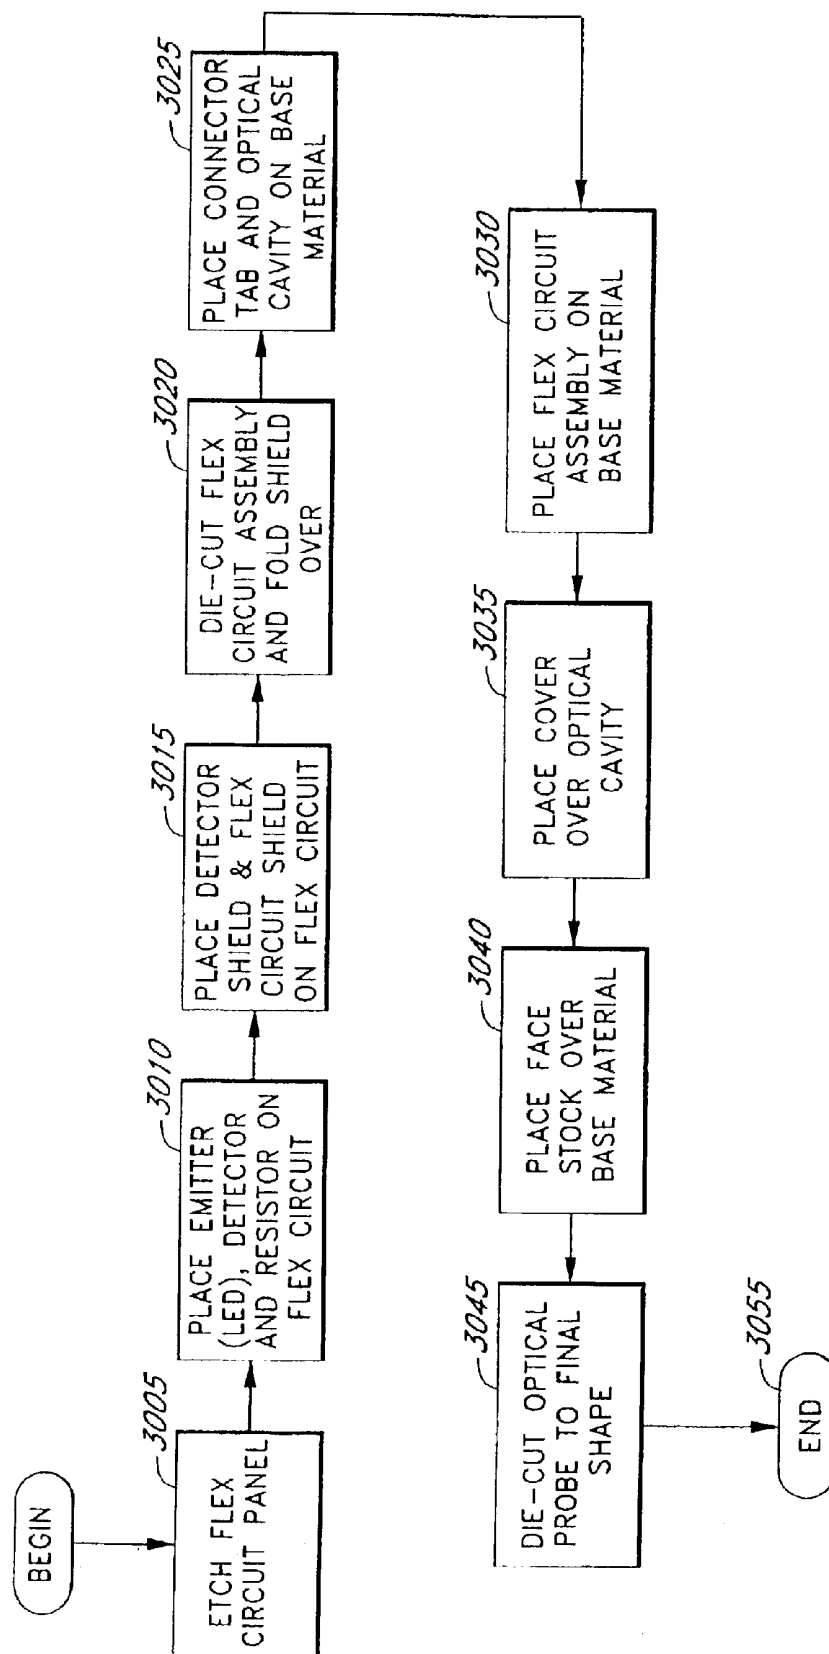


FIG. 30

FIG. 31A

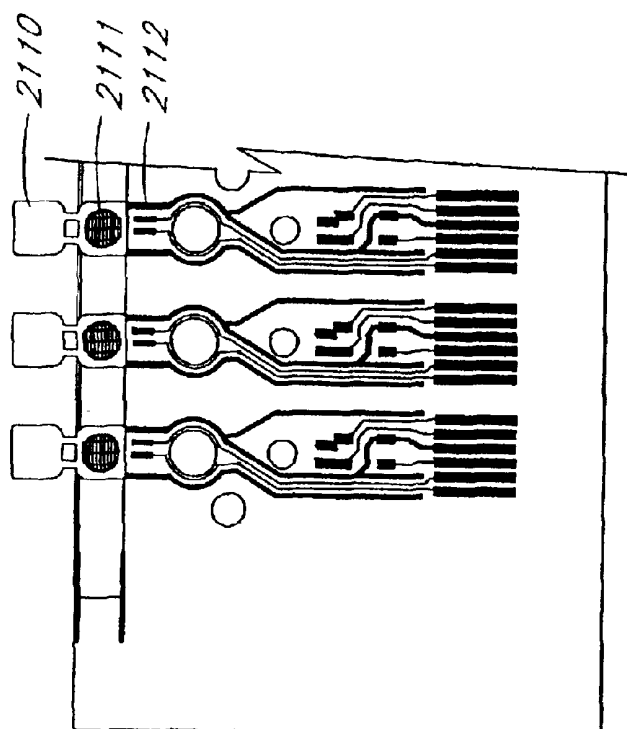


FIG. 31

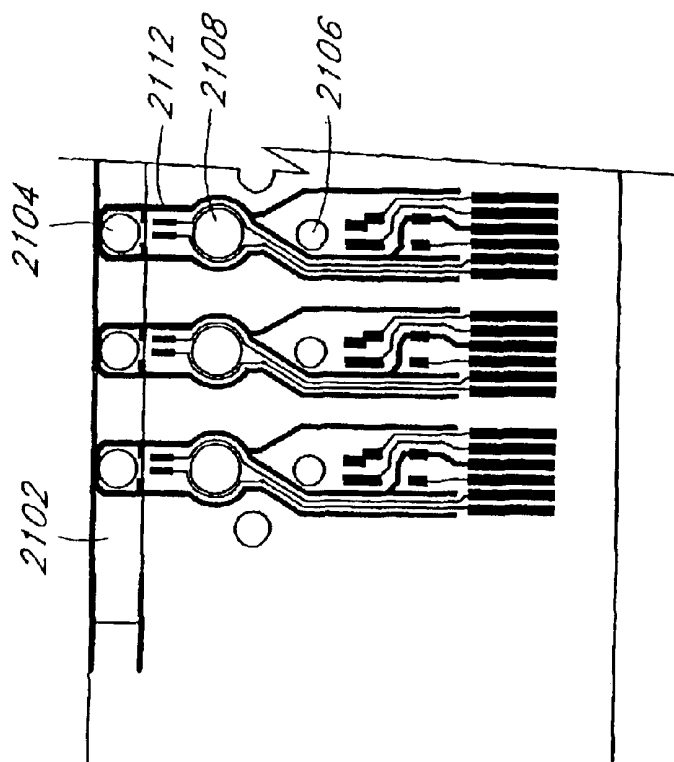
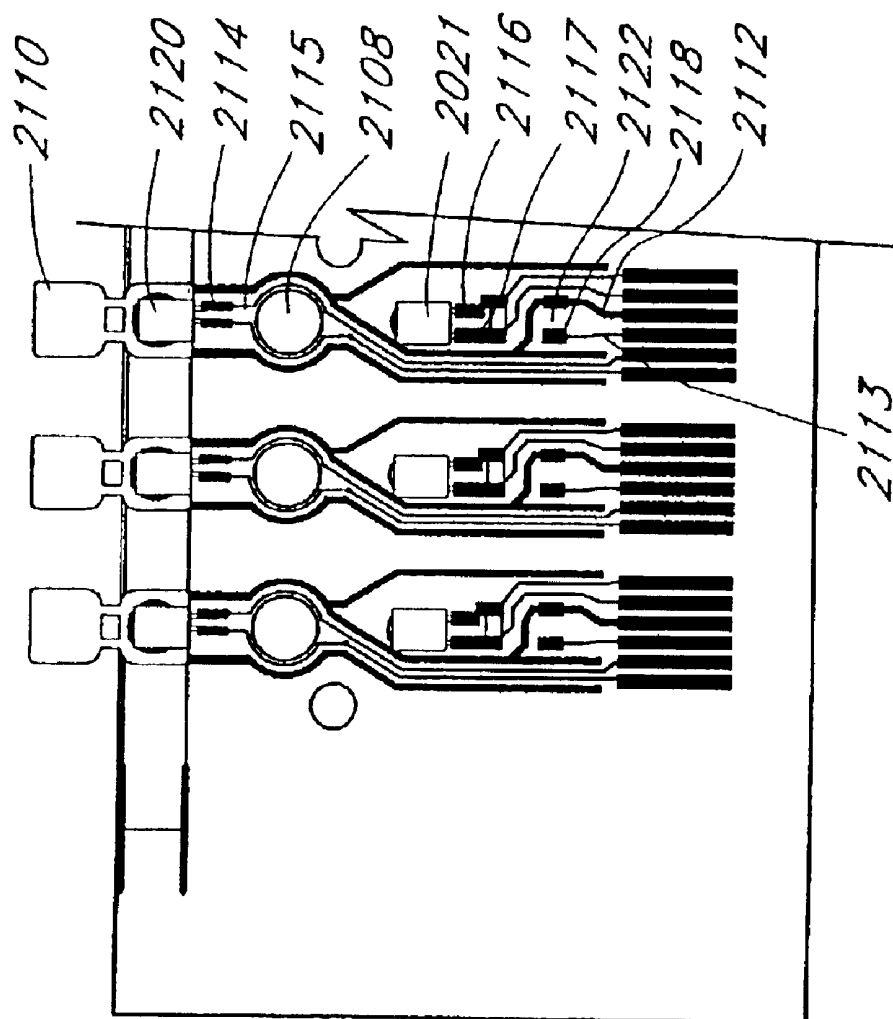
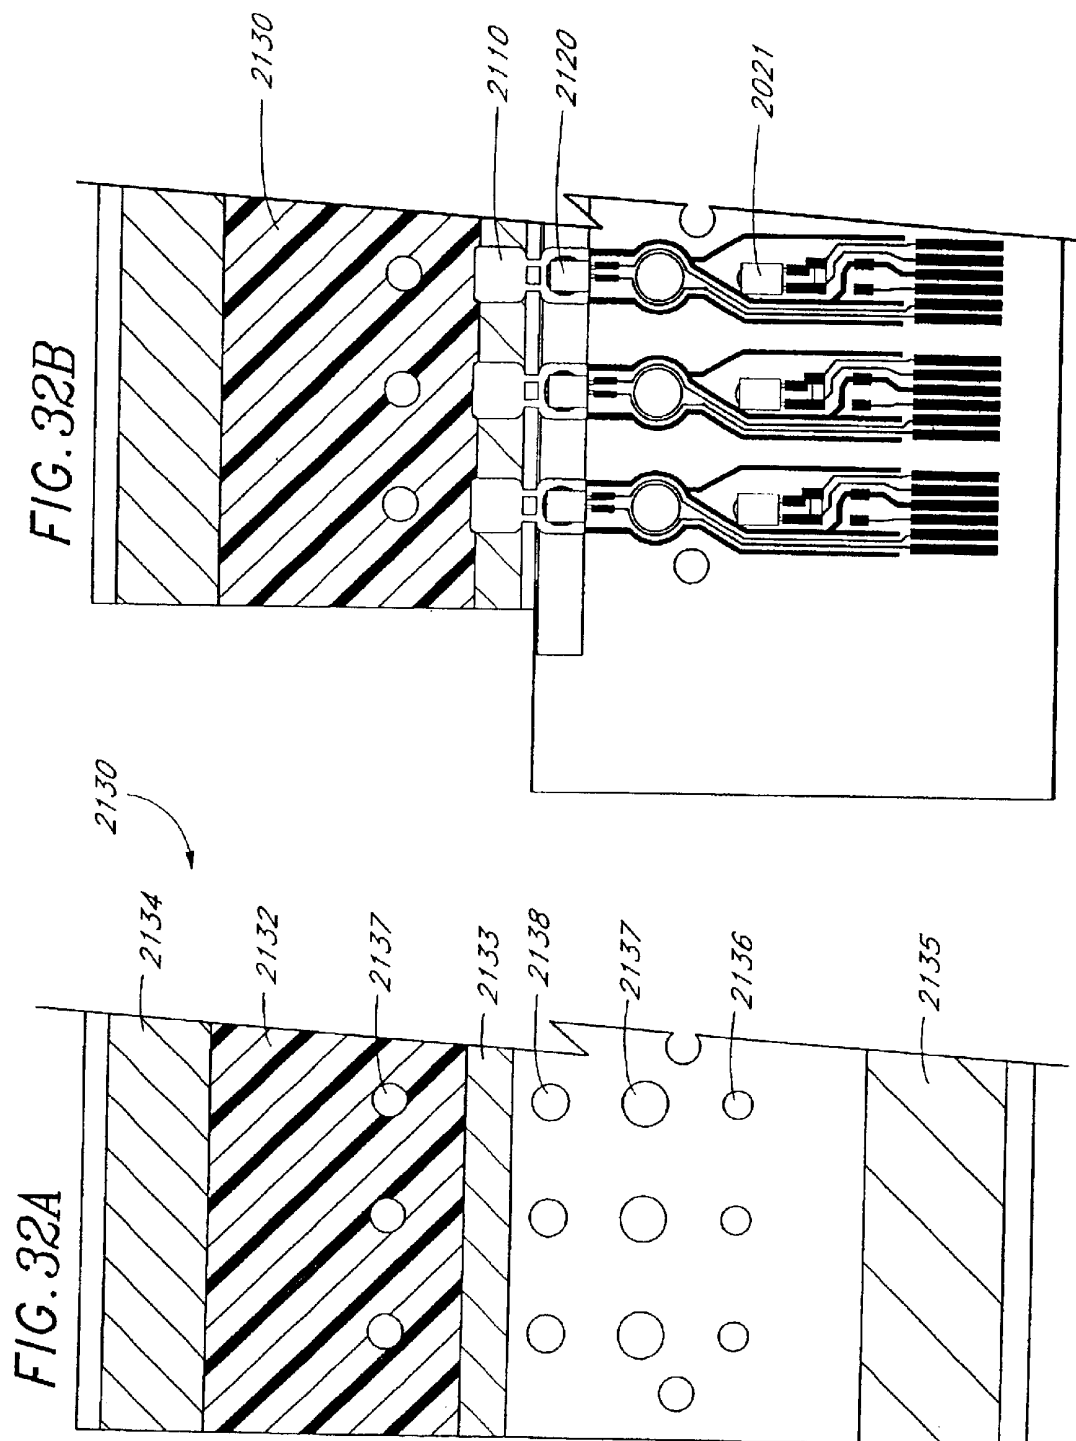


FIG. 31B





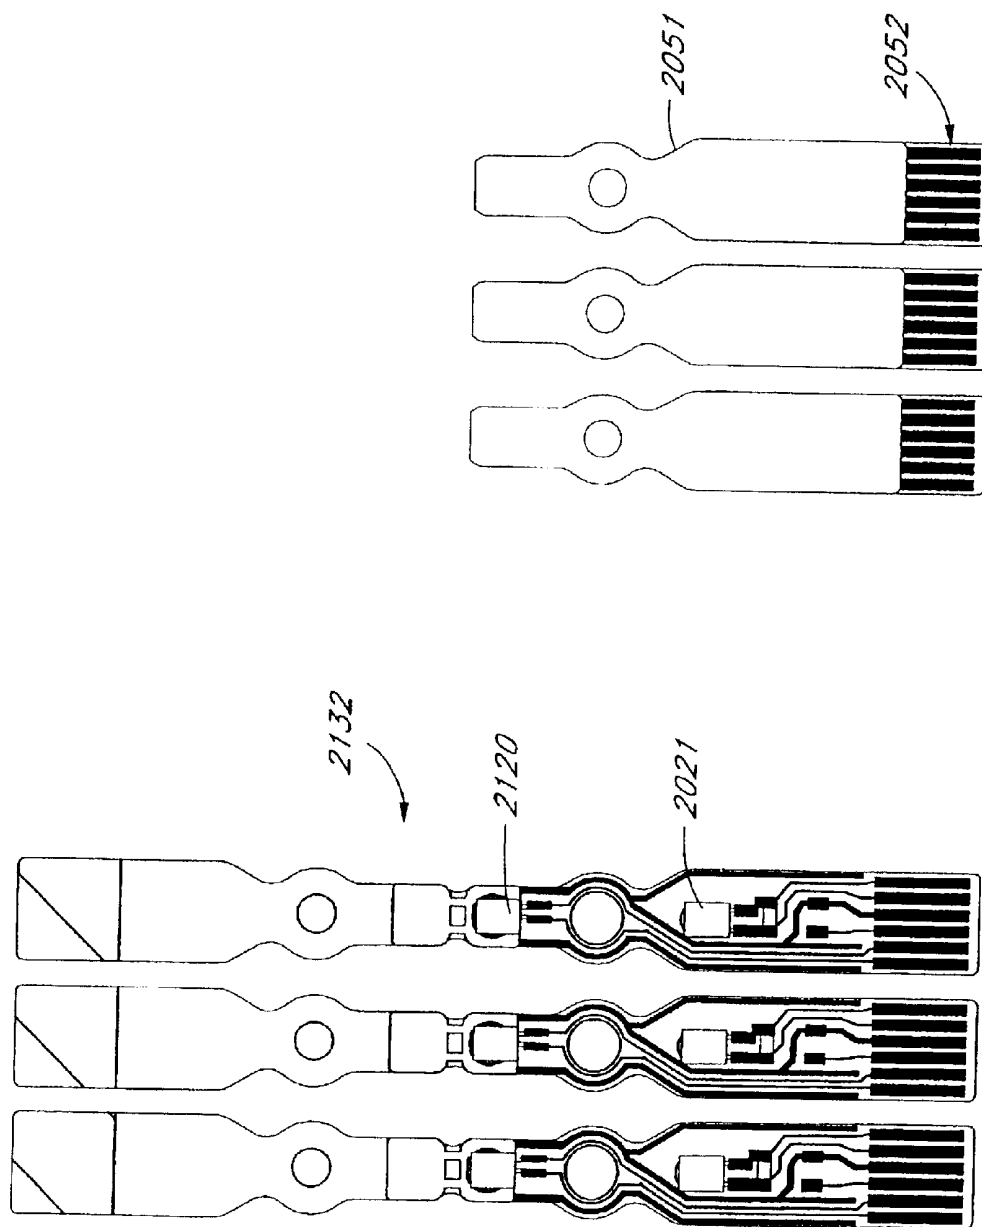


FIG. 33A

FIG. 33B

FIG. 34

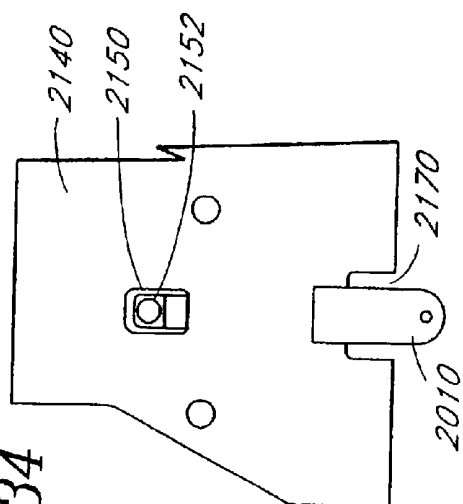


FIG. 35

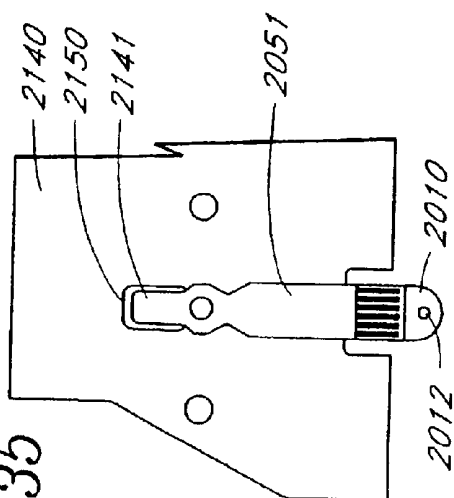


FIG. 36

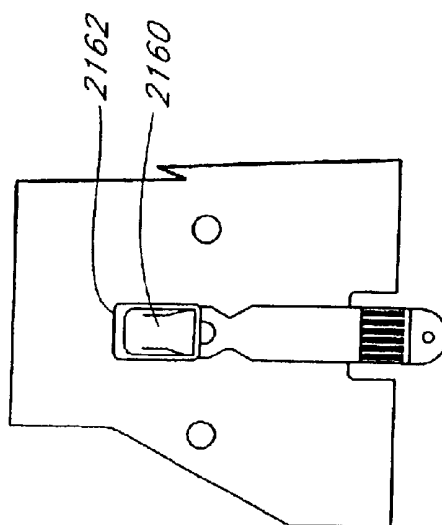


FIG. 37

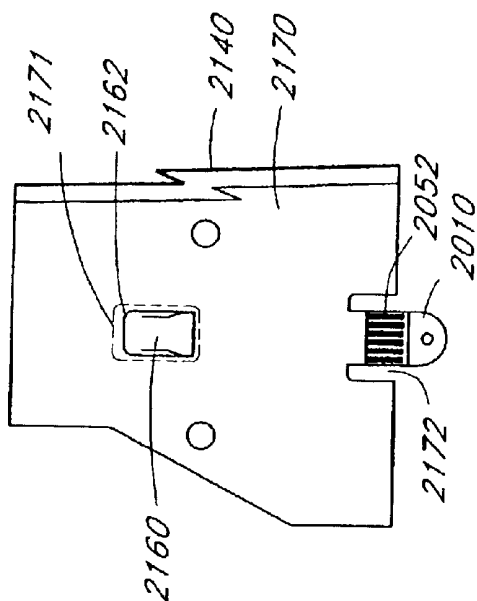
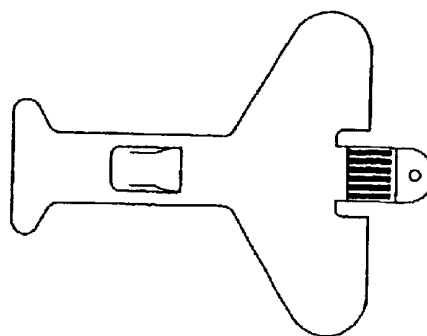
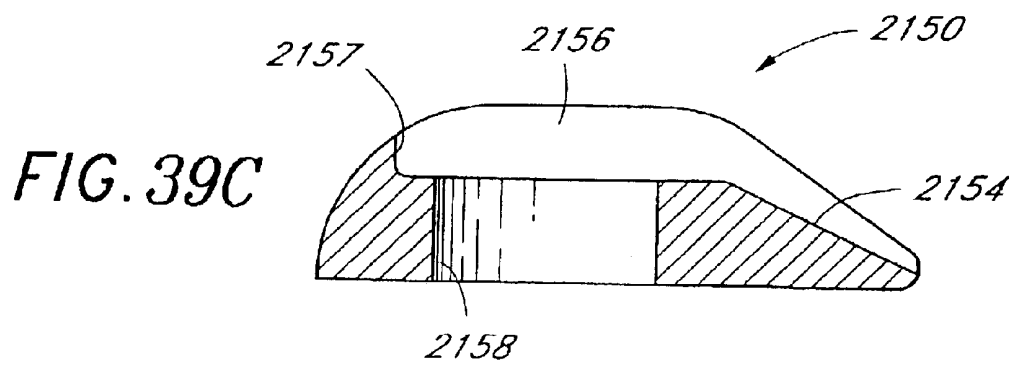
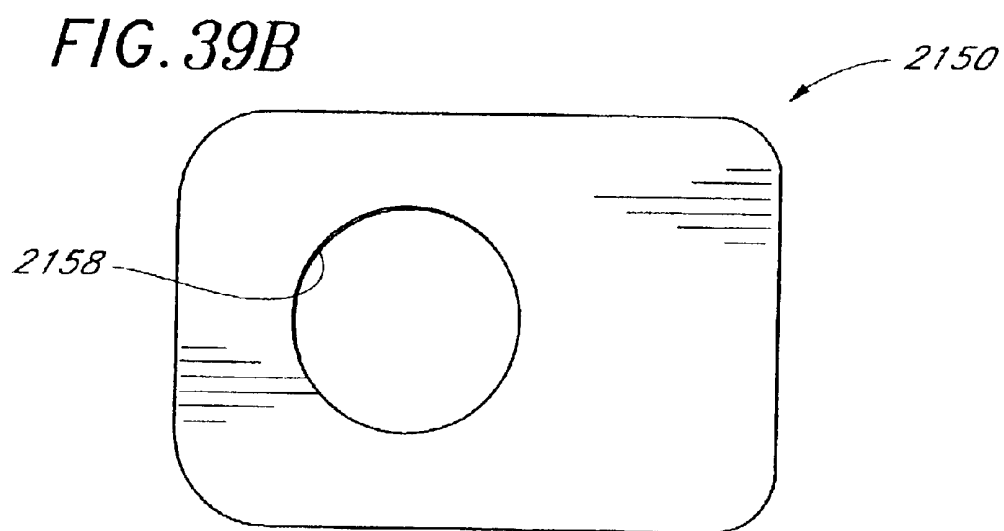
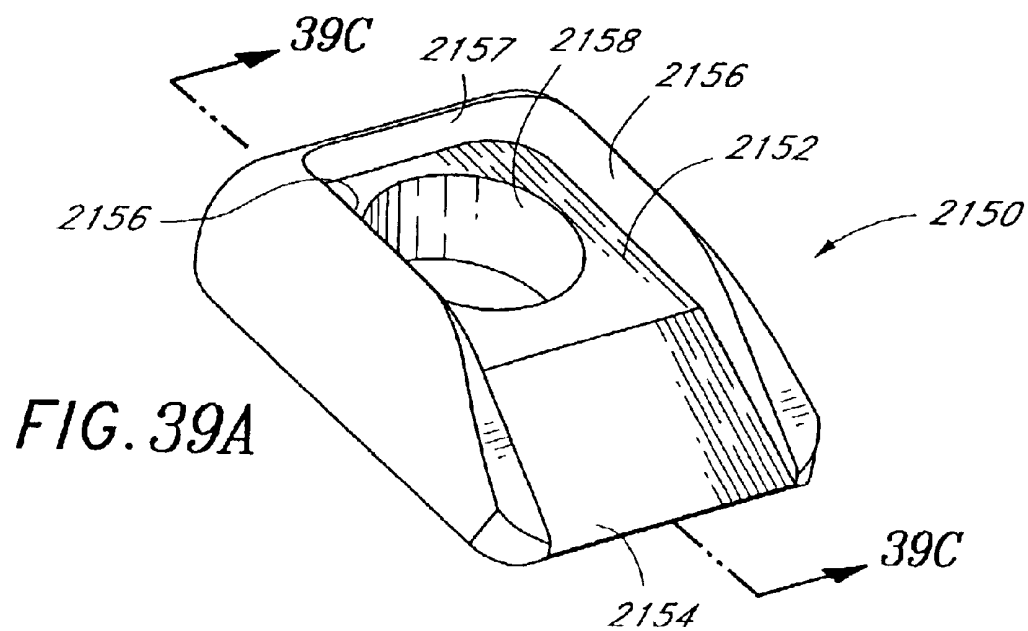


FIG. 38





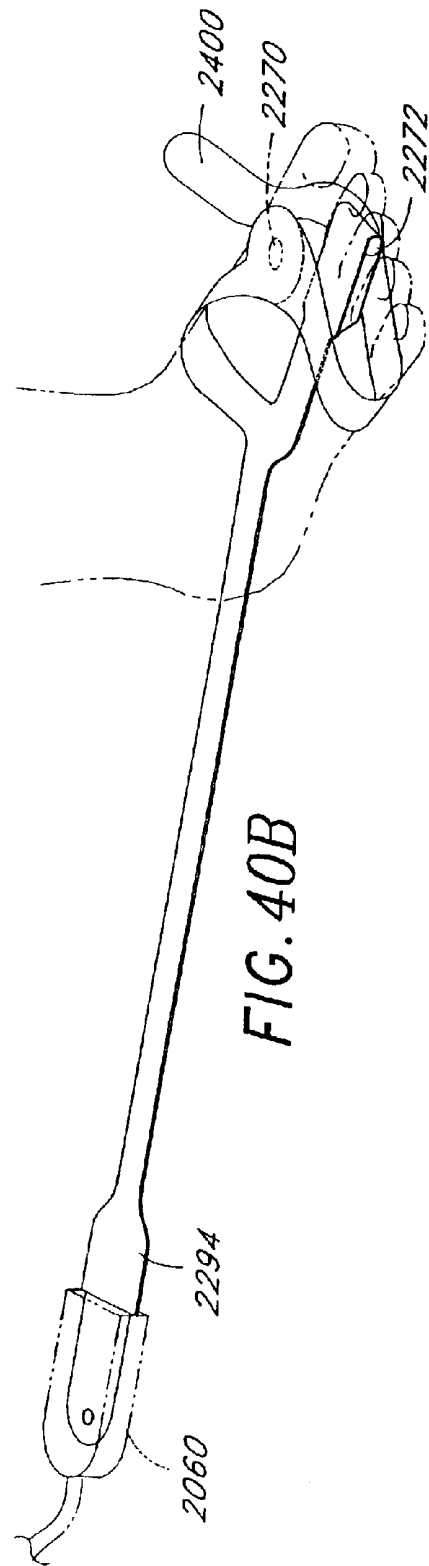
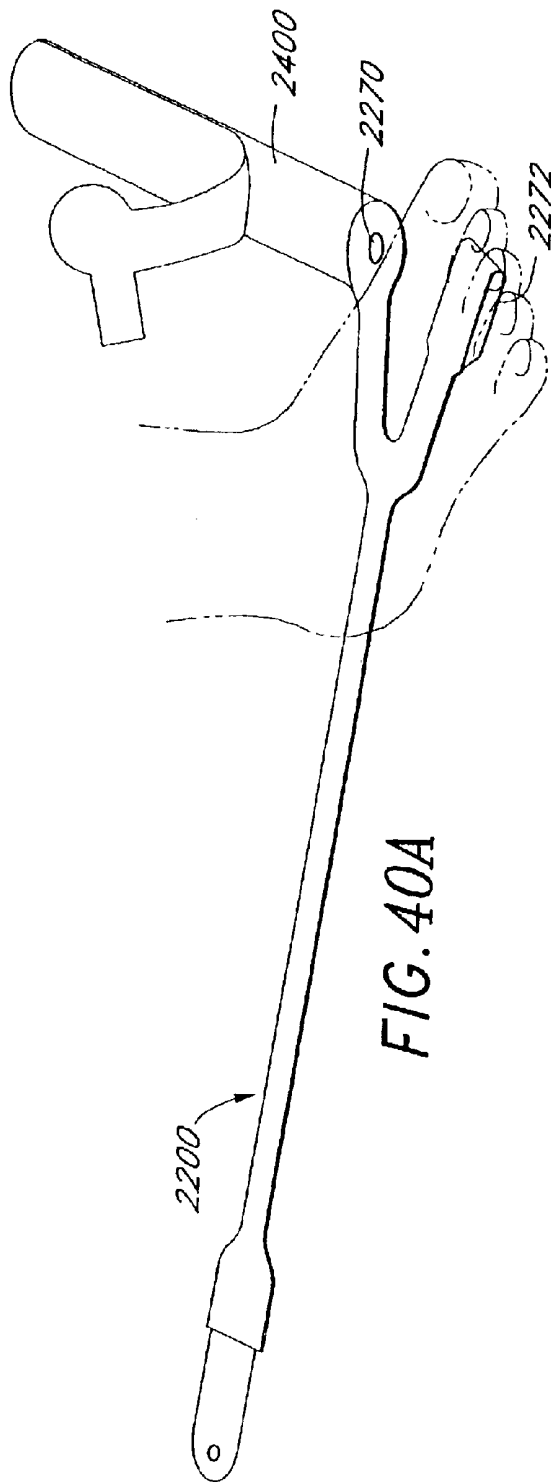


FIG. 41

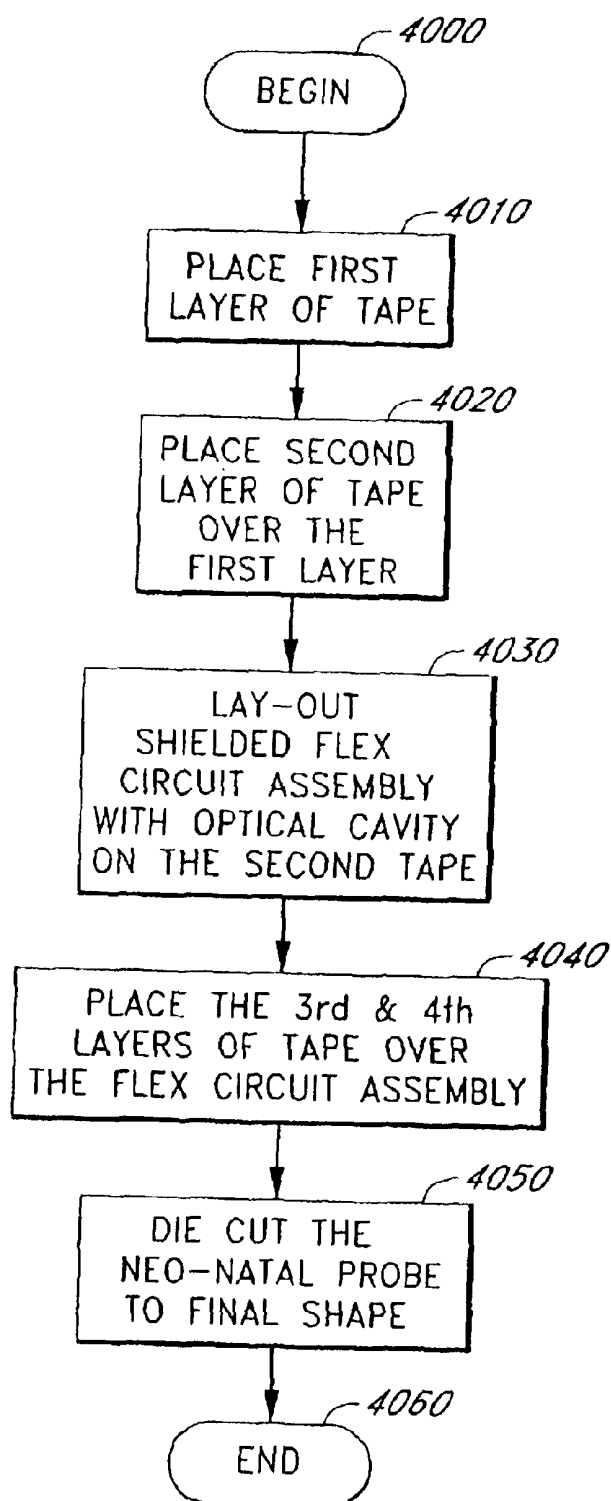


FIG. 42

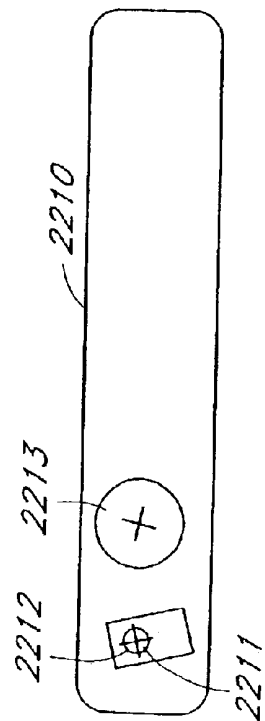
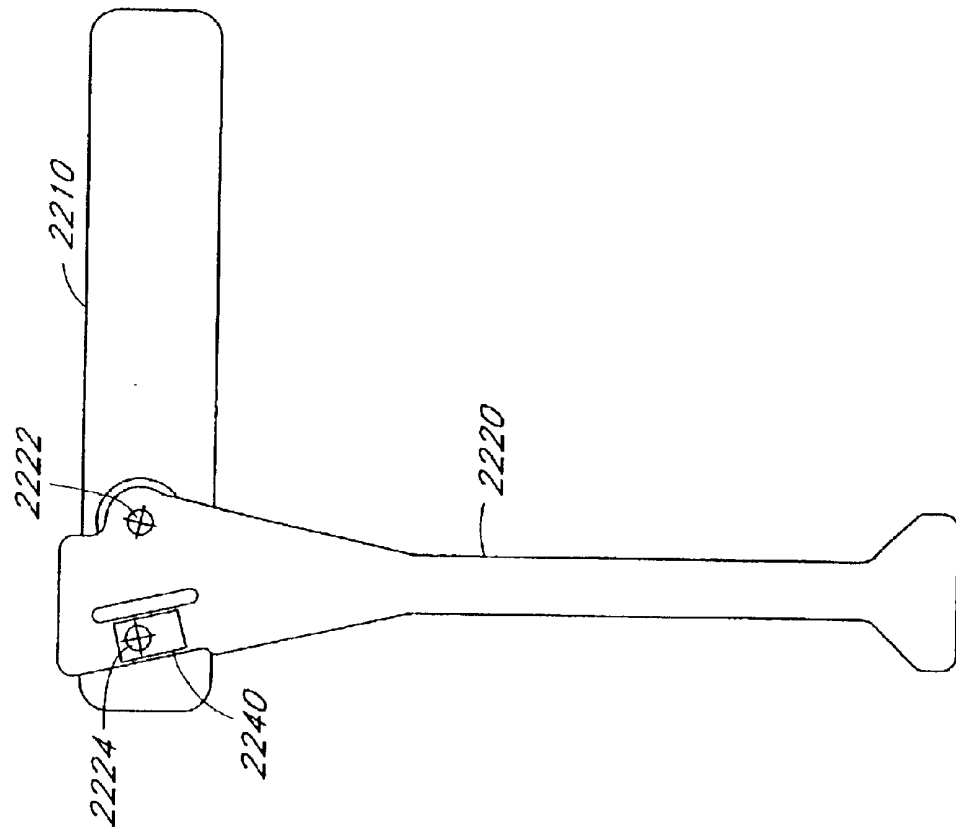


FIG. 43



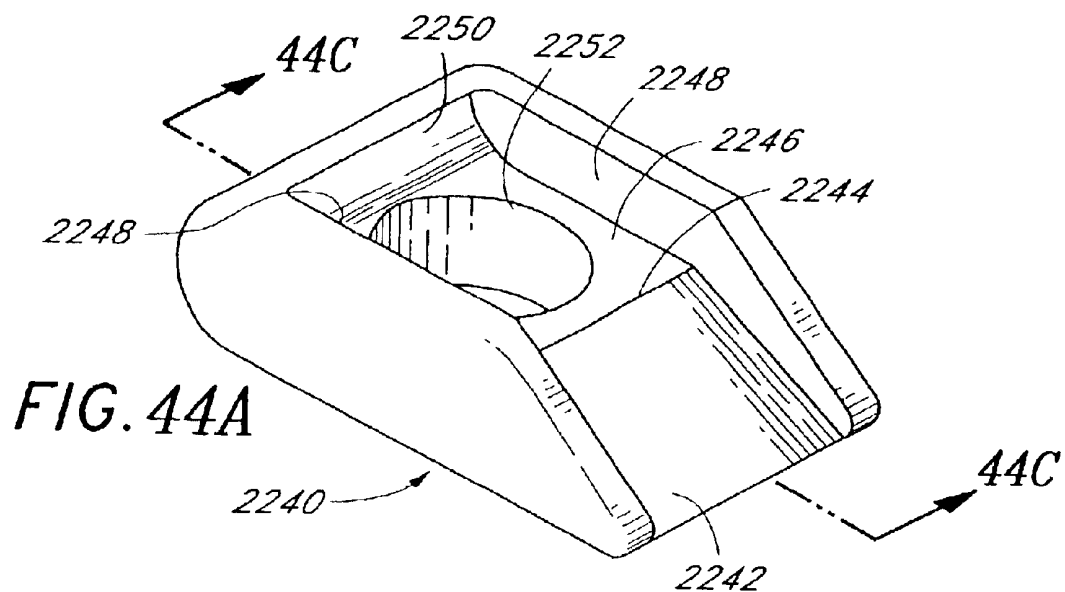
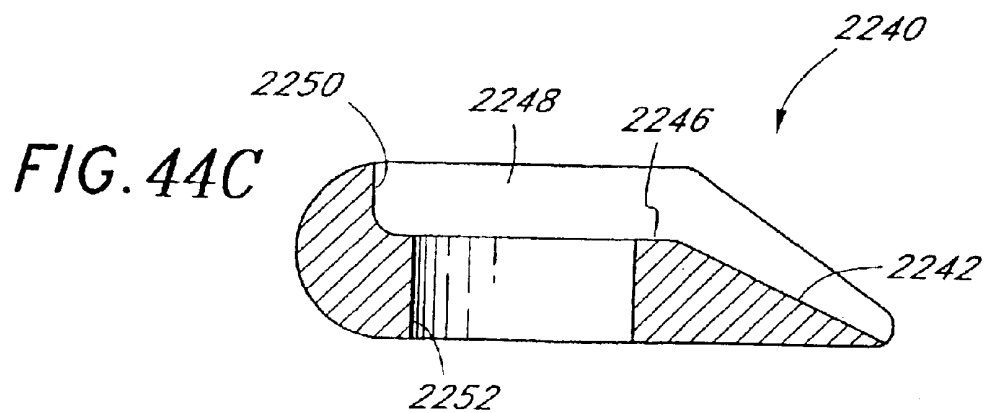
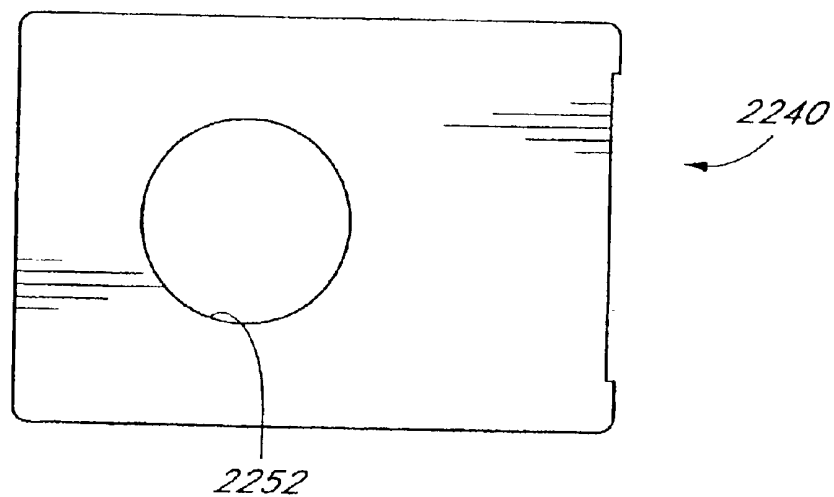


FIG. 44B



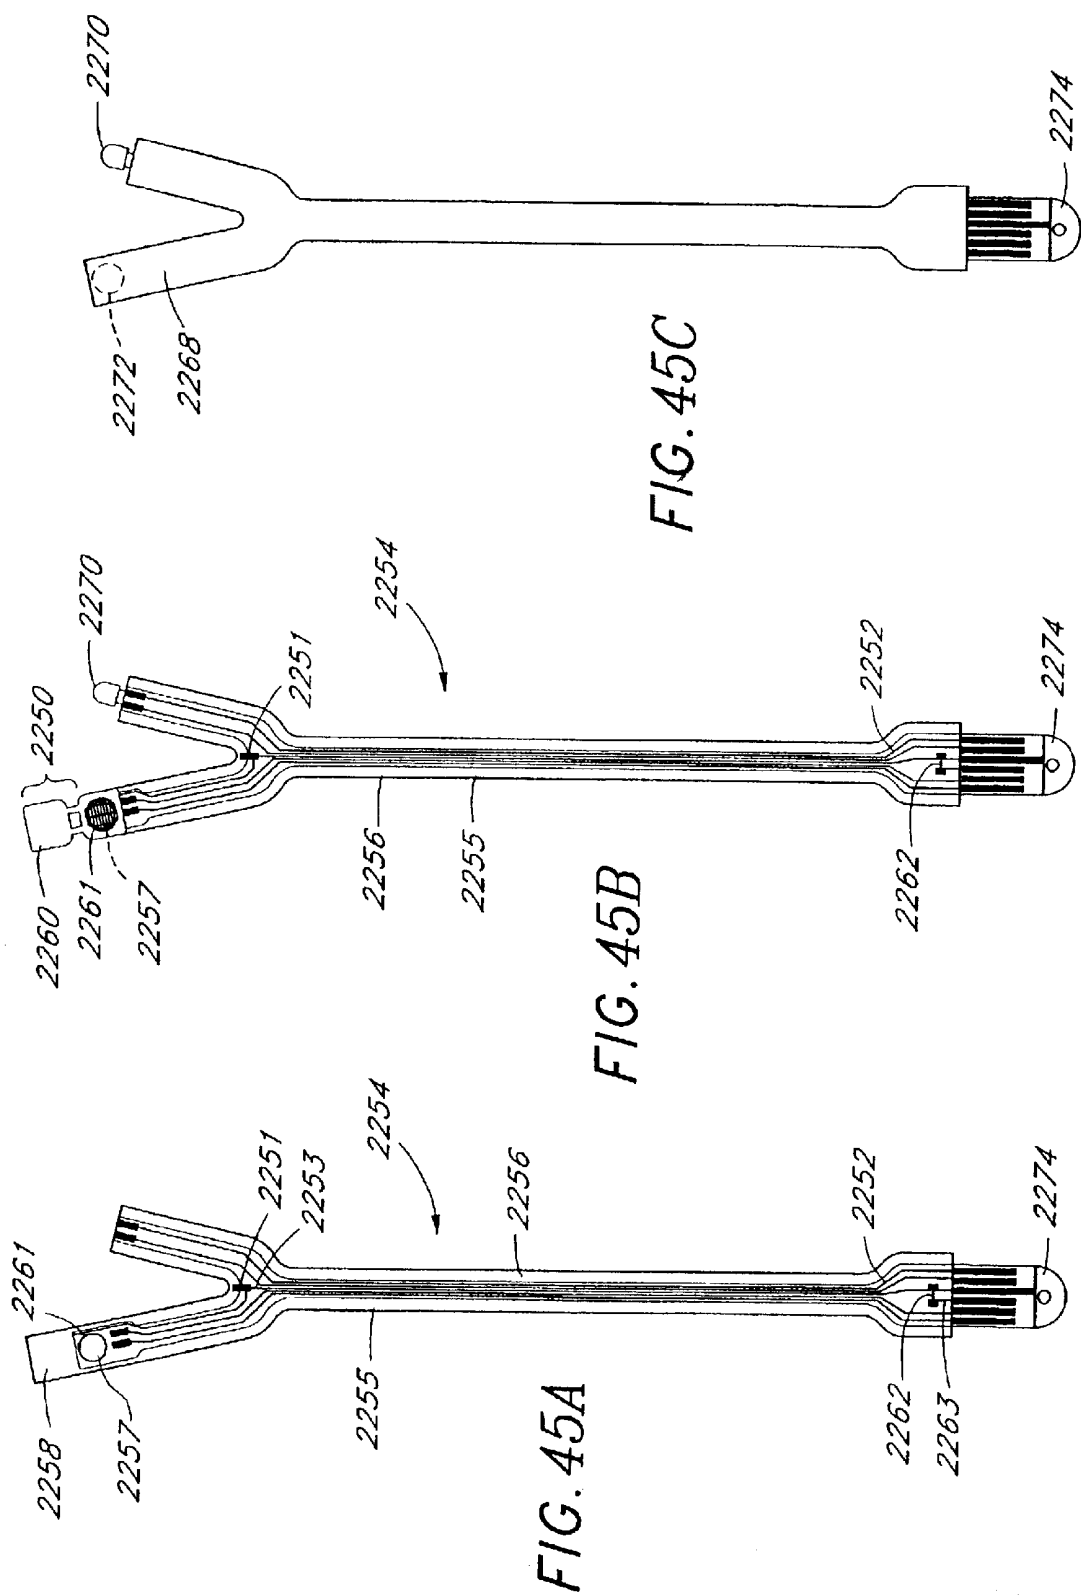


FIG. 47

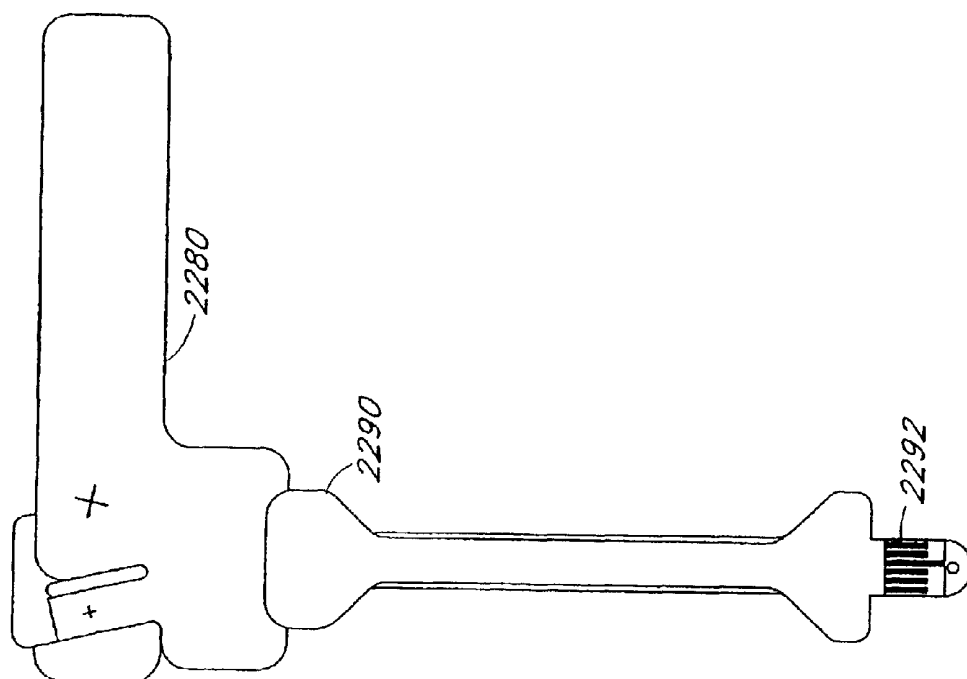


FIG. 46

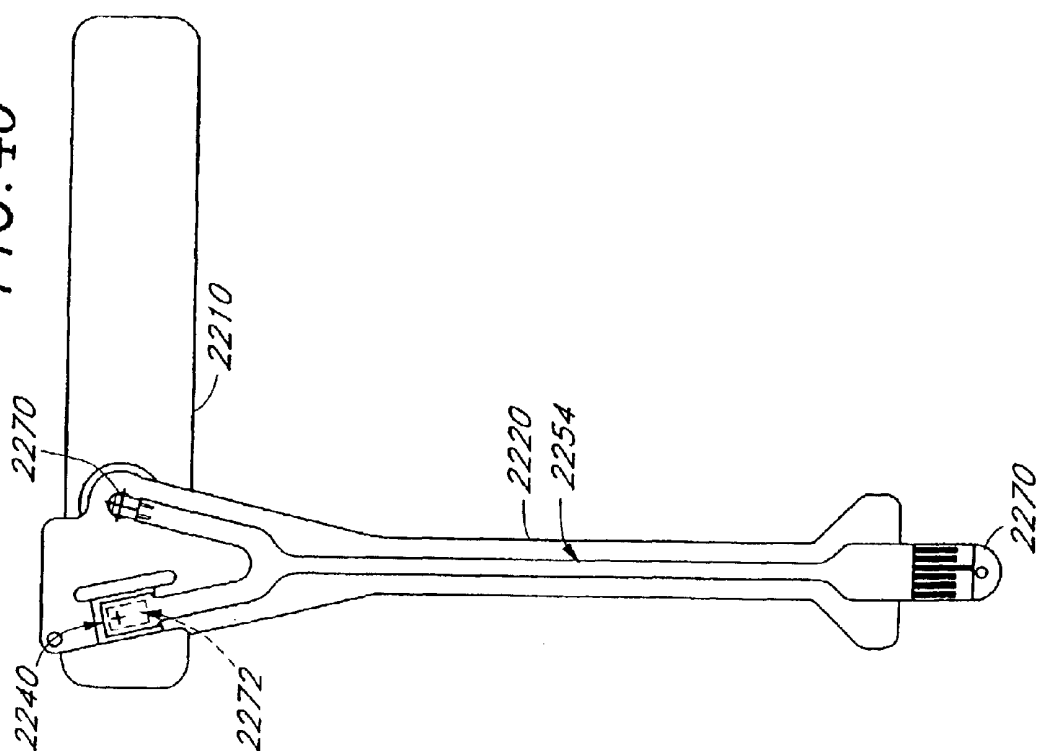
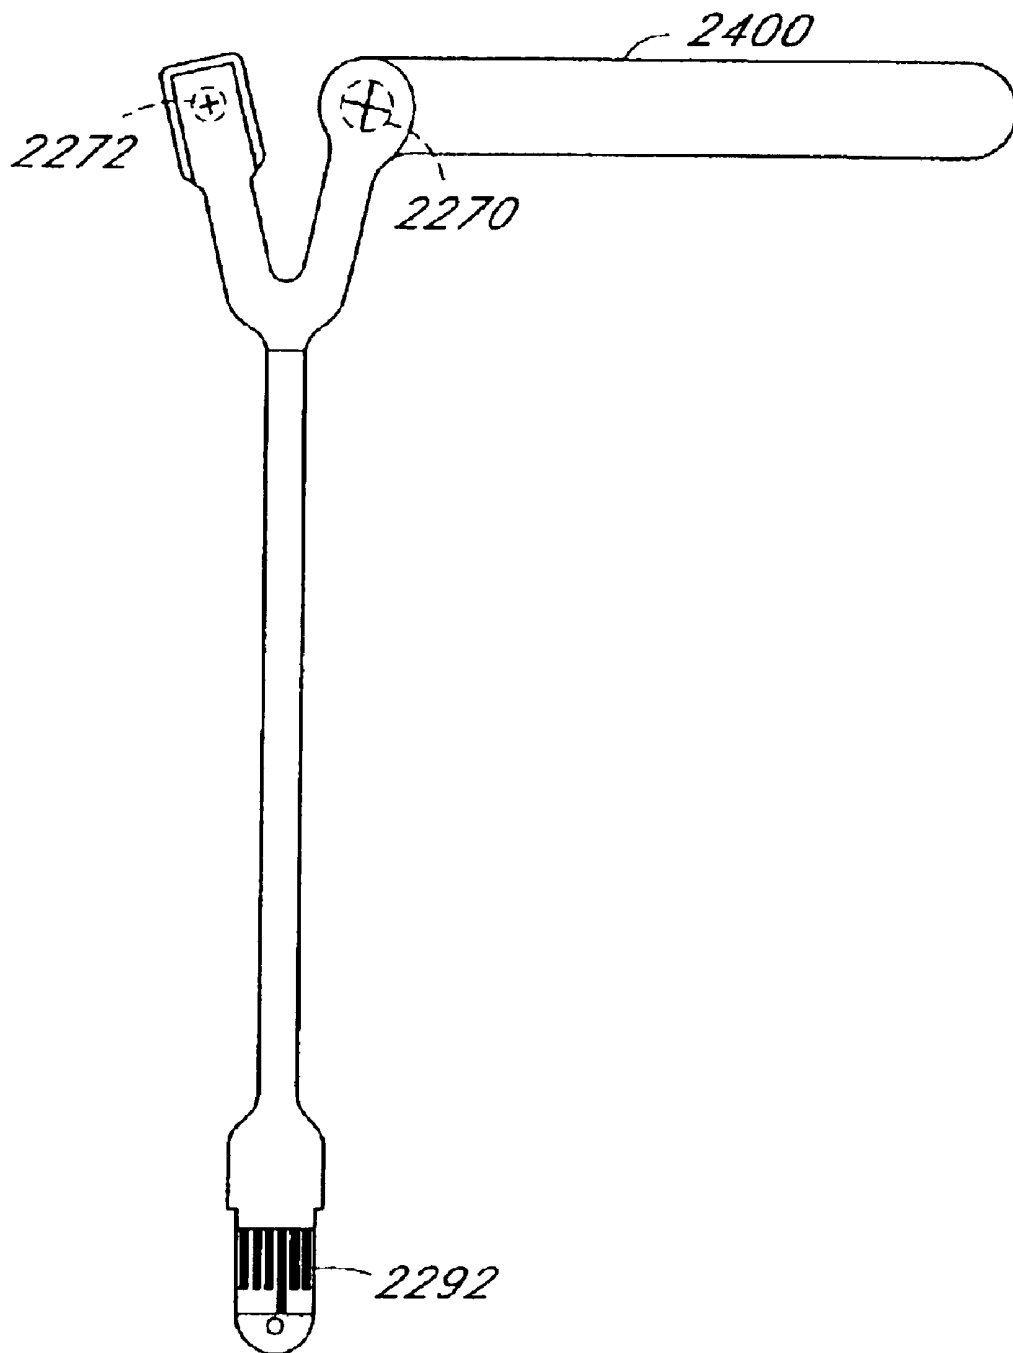
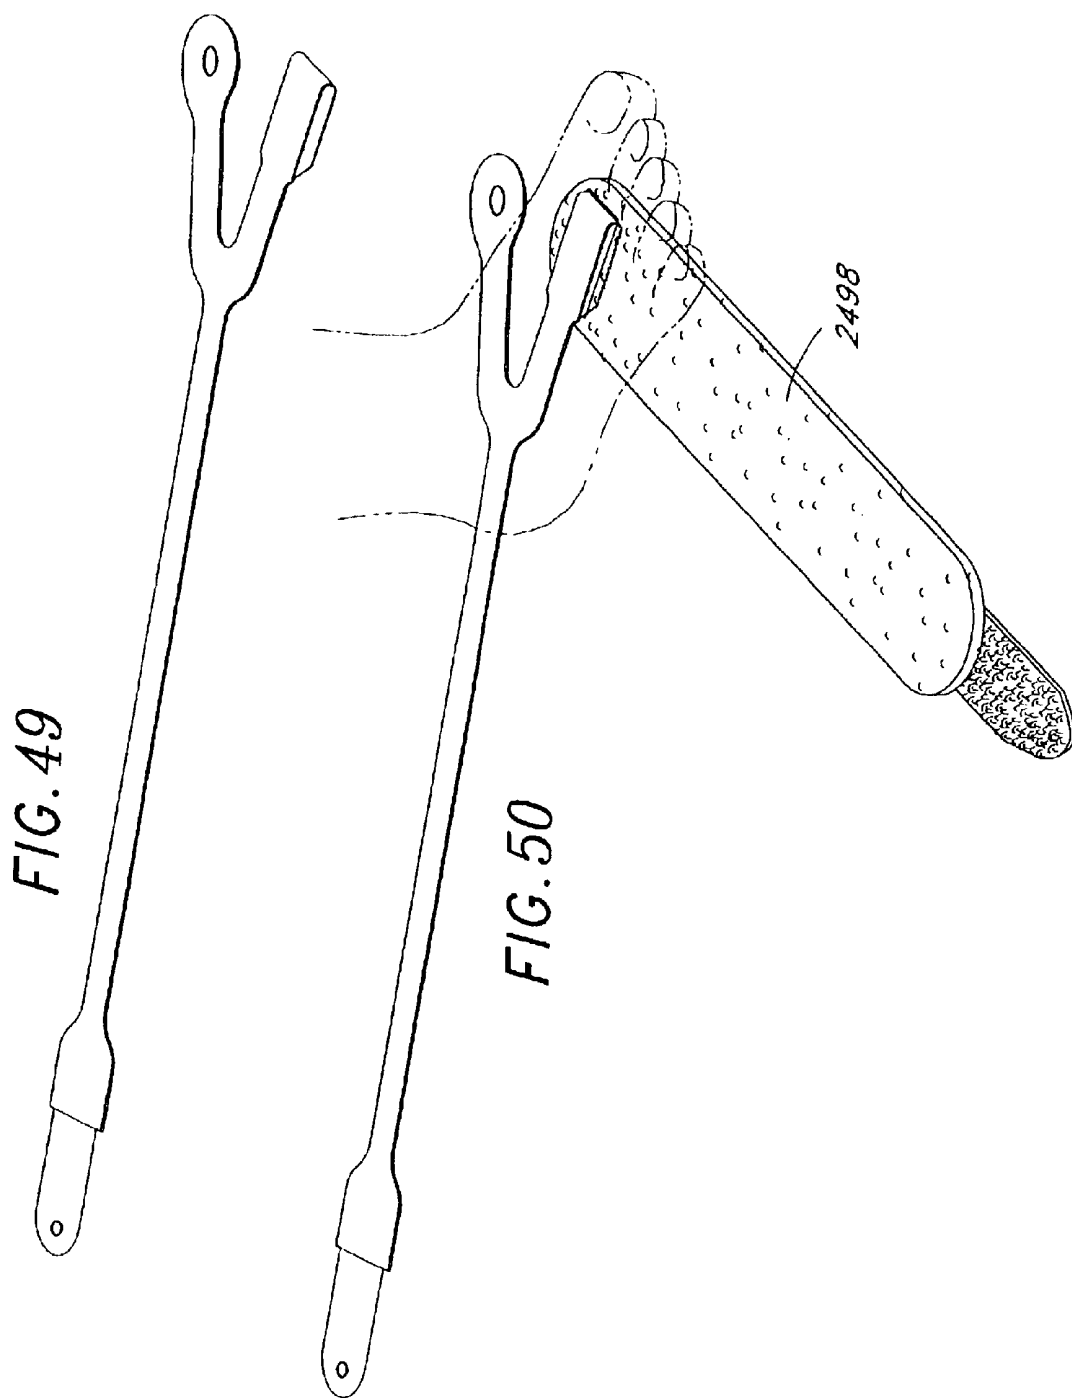


FIG. 48



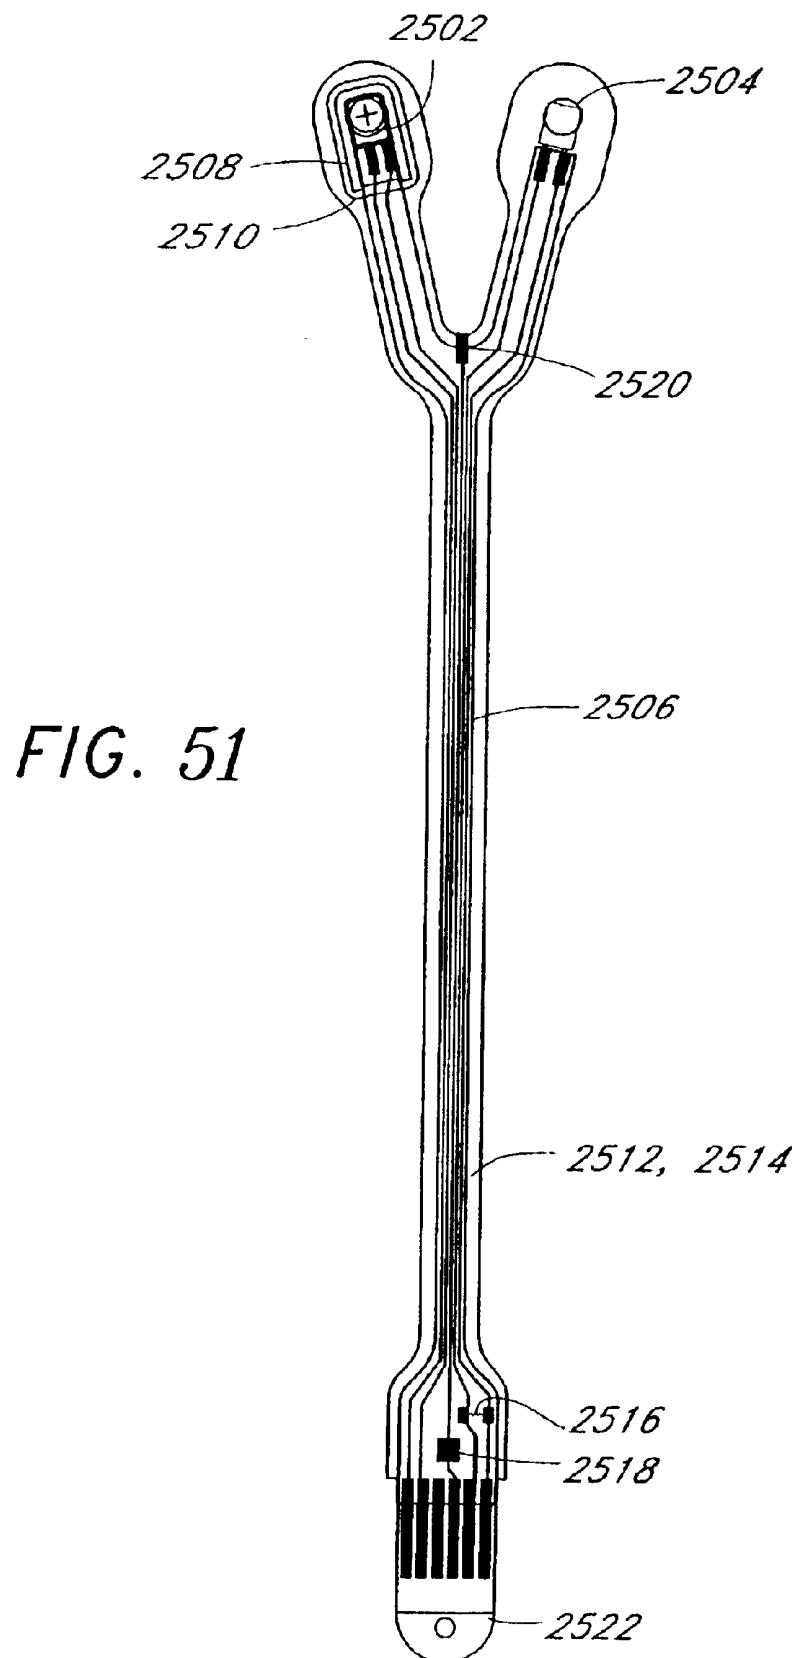


FIG. 52A

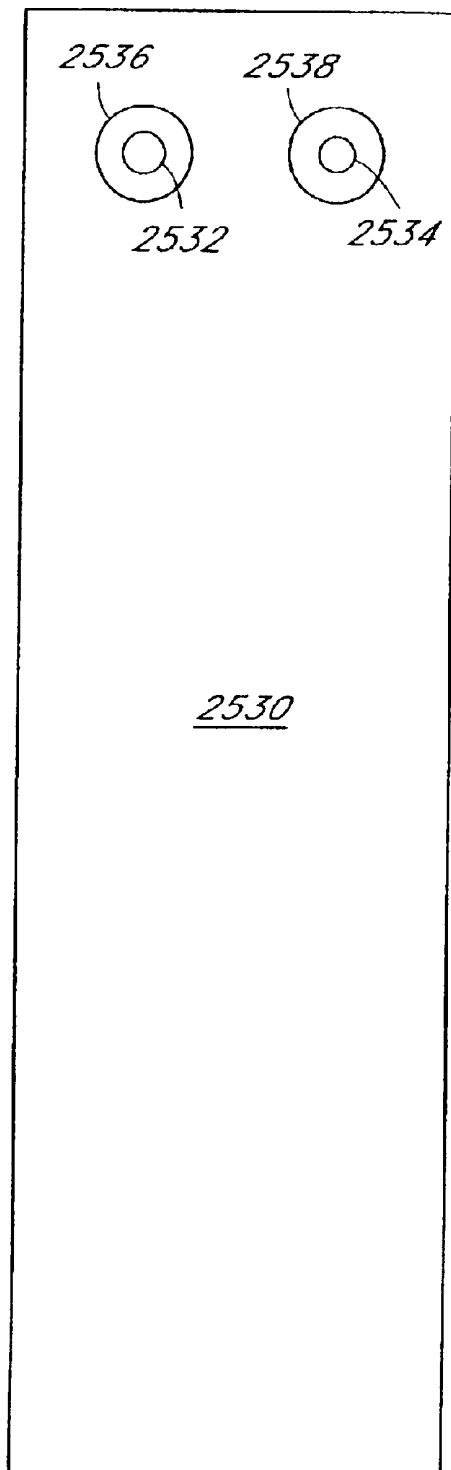


FIG. 52B

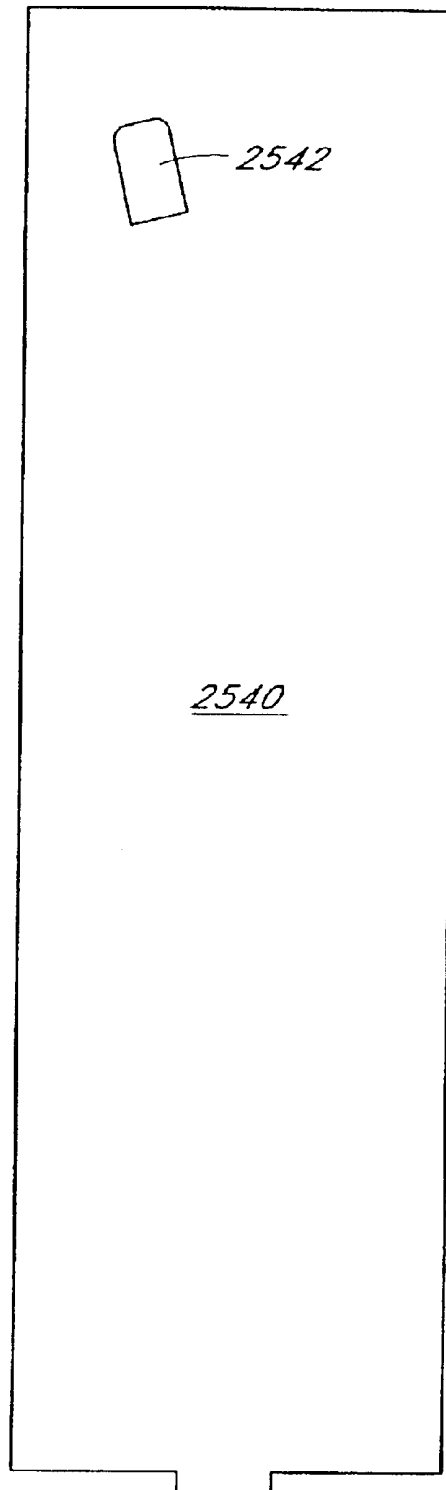


FIG. 53A

FIG. 53B

FIG. 54

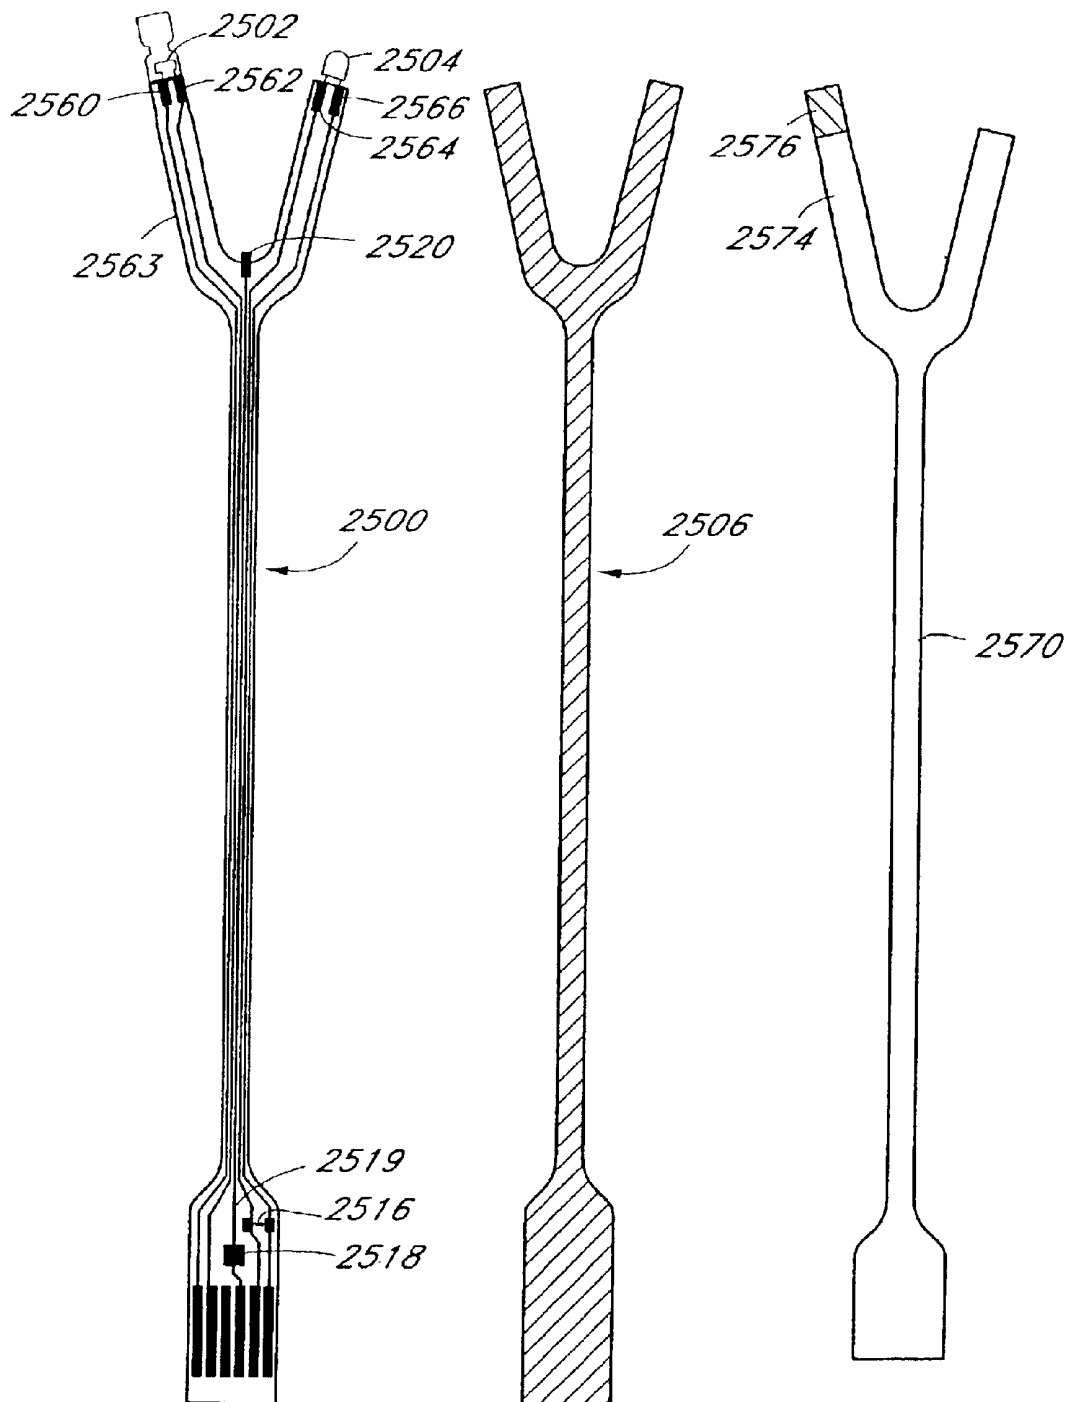


FIG. 55A

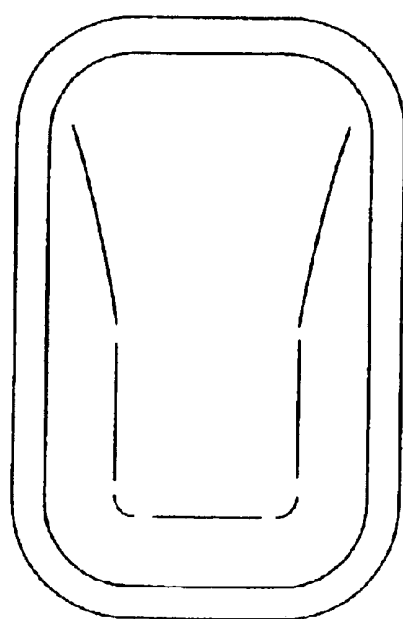


FIG. 55B

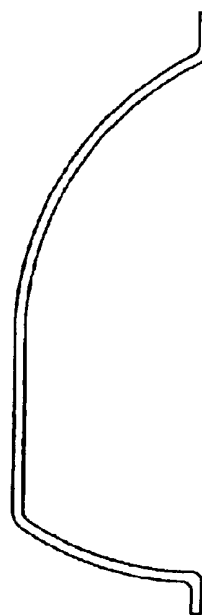
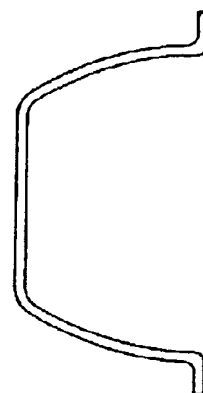
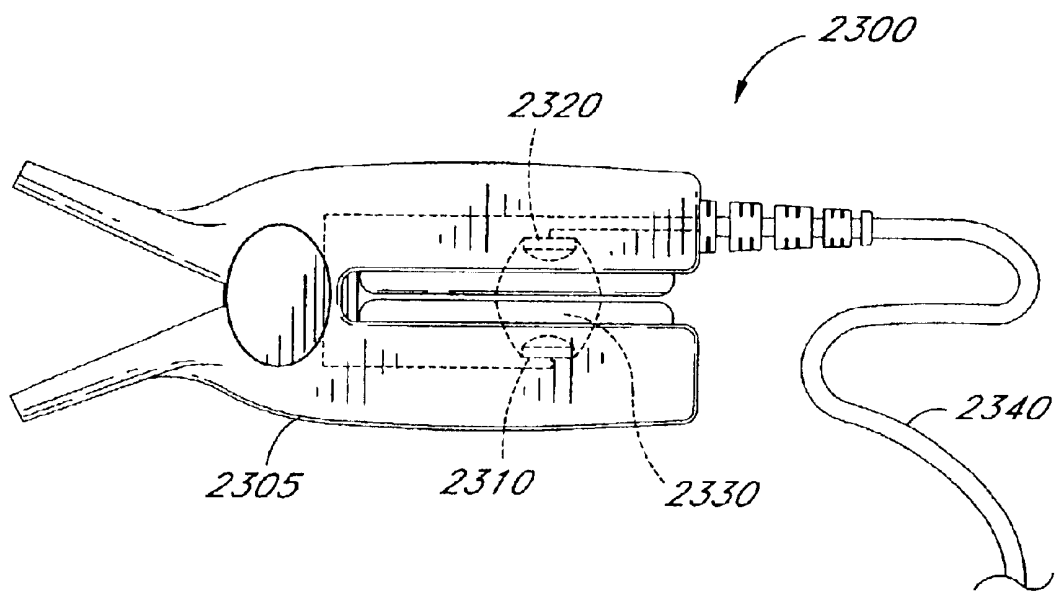


FIG. 55C



*FIG. 56*

LOW-NOISE OPTICAL PROBES FOR REDUCING AMBIENT NOISE

REFERENCE TO RELATED APPLICATIONS

This application is a continuation of application Ser. No. 09/898,990, filed Jul. 3, 2001, which is a continuation of application Ser. No. 09/094,202, filed Jun. 9, 1998, now U.S. Pat. No. 6,256,523, which is a continuation of application Ser. No. 08/543,789, now U.S. Pat. No. 5,782,757, filed Oct. 16, 1995, which is a continuation-in-part of application Ser. No. 08/333,132, filed Nov. 1, 1994, now U.S. Pat. No. 5,638,818, which is a continuation-in-part of application Ser. No. 07/672,890, filed Mar. 21, 1991, now abandoned.

FIELD OF THE INVENTION

The present invention relates to low-noise, disposable and reusable optical probes which may be used to sense optical energy passed through a medium to determine the characteristics of the medium.

BACKGROUND OF THE INVENTION

Energy is often transmitted through or reflected from a medium to determine characteristics of the medium. For example, in the medical field, instead of extracting material from a patient's body for testing, light or sound energy may be caused to be incident on the patient's body and transmitted (or reflected) energy may be measured to determine information about the material through which the energy has passed. This type of non-invasive measurement is more comfortable for the patient and can be performed more quickly.

Non-invasive physiological monitoring of bodily function is often required. For example, during surgery, blood pressure and the body's available supply of oxygen, or the blood oxygen saturation, are often monitored. Measurements such as these are often performed with non-invasive techniques where assessments are made by measuring the ratio of incident to transmitted (or reflected) light through a portion of the body, for example a digit such as a finger, or an earlobe, or a forehead.

Transmission of optical energy as it passes through the body is strongly dependent on the thickness of the material through which the light passes, or the optical path length. Many portions of a patient's body are typically soft and compressible. For example, a finger comprises skin, muscle, tissue, bone, blood, etc. Although the bone is relatively incompressible, the tissue, muscle, etc. are easily compressible with pressure applied to the finger, as often occurs when the finger moves. Thus, if optical energy is made incident on a finger and the patient moves in a manner which distorts or compresses the finger, the optical path length changes. Since a patient generally moves in an erratic fashion, the compression of the finger is erratic. This causes the change in optical path length to be erratic, making the absorption erratic, resulting in a difficult to interpret measured signal.

Many types of non-invasive monitoring devices have been developed to try to produce a clear and discernable signal as energy is transmitted through a medium, such as a finger or other part of the body. In typical optical probes a light emitting diode (LED) is placed on one side of the medium while a photodetector is placed on an opposite side of the medium. Many prior art optical probes are designed for use only when a patient is relatively motionless since, as discussed above, motion induced noise can grossly corrupt the measured signal. Typically, probes are designed to

maximize contact between the LED and the medium and the photodetector and the medium to promote strong optical coupling between the LED, the medium, and the photodetector, thereby generating a strong output signal intensity. In this way, a strong, clear signal can be transmitted through the medium when the patient is generally motionless.

For example, U.S. Pat. No. 4,880,304 to Jaeb, et al. discloses an optical probe for a pulse oximeter, or blood oxygen saturation monitor, comprising a housing with a flat lower face containing a central protrusion in which a plurality of light emitting diodes (LEDs) and an optical detector are mounted. When the probe is placed on the patient's tissue, the protrusion causes the LEDs and the detector to press against the tissue to provide improved optical coupling of the sensor to the skin. In another embodiment (FIGS. 4a and 4b in the Jaeb patent), the LEDs and the detector are arranged within a central chamber, generally horizontal with respect to the tissue on which the probe is placed. A set of mirrors or prisms causes light to be directed from the LEDs onto the tissue through a polymer sealant within the chamber, the sealant providing a contact with the tissue for good optical coupling with the tissue.

U.S. Pat. No. 4,825,879 to Tan, et al. discloses an optical probe wherein a T-shaped wrap, having a vertical stem and a horizontal cross bar, is utilized to secure a light source and an optical sensor in optical contact with a finger. The light source is located in a window on one side of the vertical stem while the sensor is located in a window on the other side of the vertical stem. The finger is aligned with the stem and the stem is bent such that the light source and the sensor lie on opposite sides of the finger. Then, the cross bar is wrapped around the finger to secure the wrap, thereby ensuring that the light source and the sensor remain in contact with the finger to produce good optical coupling.

U.S. Pat. No. 4,380,240 to Jöbssis, et al. discloses an optical probe wherein a light source and a light detector are incorporated into channels within a slightly deformable mounting structure which is adhered to a strap. Annular adhesive tapes are placed over the source and the detector. The light source and detector are firmly engaged with a bodily surface by the adhesive tapes and pressure induced by closing the strap around a portion of the body. An alternative embodiment provides a pressurized seal and a pumping mechanism to cause the body to be sucked into contact with the light source and detector.

U.S. Pat. No. 4,865,038 to Rich, et al. discloses an optical probe having an extremely thin cross section such that it is flexible. A die LED and a die photodetector are located on a flexible printed circuit board and encapsulated by an epoxy bead. A spacer, having circular apertures positioned in alignment with the LED and photodetector, is placed over the exposed circuit board. A transparent top cover is placed over the spacer and is sealed with a bottom cover placed under the circuit board, thereby sealing the probe from contaminants. A spine may be added to strengthen the device. The flexibility of the device allows it to be pinched onto the body causing the epoxy beads over the LED and the photodetector to protrude through the apertures in the spacer and press against the top cover such that good optical contact is made with the body.

U.S. Pat. No. 4,907,594 to Muz discloses an optical probe wherein a dual wall rubberized sheath is fit over a finger. A pump is located at the tip of the finger such that a pressurized chamber may be formed between the two walls, thereby causing an LED and a photodetector located in the inner wall to be in contact with the finger.

Each of the above described optical probes is designed to cause a strong measured signal at the photodetector by optimizing contact between the LED, the patient, and the probe. However, this optimization forces compressible portions of the patient's body to be in contact with surfaces which compress these portions of the patient's body when the patient moves. This can cause extreme changes in the thickness of material through which optical energy passes, i.e., changes in the optical path length and changes due to scattering as a result of venous blood movement during motion. Changes in the optical path length can produce enough distortion in the measured signal to make it difficult or impossible to determine desired information.

Furthermore, demand has increased for disposable and reusable optical probes which are suitably constructed to provide low-noise signals to be output to a signal processor in order to determine the characteristics of the medium. Many difficulties relating to motion-induced noise have been encountered in providing such an optical probe inexpensively. Furthermore, such probes tend to be difficult to use in certain applications, such as applications where a patient's finger may move or shift during measurement, or, in a more extreme case, when the optical probe is employed on small children who typically do not sit still during the measurement process.

Thus, a need exists for a low-cost, low-noise optical probe which is easy to use under adverse conditions, and for a method of manufacturing such a probe. More specifically, a need exists for a probe which reduces motion induced noise, or motion artifacts, during measurement of a signal while still generating a transmitted or reflected signal of sufficient intensity to be measured by a detector.

SUMMARY OF THE INVENTION

The present invention involves a probe for use in non-invasive energy absorption (or reflection) measurements. One aspect of the present embodiment involves an optical probe for non-invasive measurement of characteristics of a medium, wherein the probe has an emitter which transmits optical radiation and a detector configured to detect the optical radiation transmitted by the emitter. The probe also has a flexible circuit assembly having circuit paths for connection with the emitter and the detector. A substrate forms a surface of the flex circuit assembly between the detector and the emitter. The substrate is constructed to minimize light piping from the emitter to the detector.

In one embodiment, the probe further has a flexible backing supporting the flex circuit, the flexible backing being configured to attach the optical probe to the medium. Advantageously, an optical cavity is provided for the detector.

In one advantageous embodiment, the flexible circuit assembly is sufficiently flexible to provide spring action to minimize optical decoupling between the emitter and the detector due to perturbations of the medium. Advantageously, a flexible backing supporting the flex circuit is configured to affix the optical probe to the medium. Also, in one preferred embodiment, the flex circuit has an optical obstruction between the emitter and the detector.

In one preferred embodiment, the optical obstruction comprising an aperture through the flex circuit configured to receive a fingertip when the optical probe is affixed to a finger. The aperture stabilizes the finger within the probe so as to reduce optical decoupling between the emitter and the detector.

Preferably, the probe has an optical cavity containing the detector. In one advantageous embodiment, the optical cavity

containing the detector is coated with a material which absorbs ambient light or the cavity is made from an ambient light absorptive material.

A further aspect of the present invention involves an probe for the non-invasive measurement of characteristics of a medium. According to this aspect, the optical probe has an emitter which transmits optical radiation and a detector configured to detect the optical radiation after attenuation through the medium. Again, a flexible circuit assembly extending between the emitter and the detector has electrical circuit paths for the detector and the emitter. A cushion positioned between the detector and the emitter along the flexible circuit is also provided. The cushion is preferably formed in the flexible circuit between the emitter and the detector so that the cushion abuts a patient's fingertip when the optical probe is attached to the fingertip.

Another aspect of the present invention involves an optical probe for the non-invasive measurement of characteristics of a medium, wherein the probe has a substrate which forms a surface for the probe such that the substrate is constructed to have a V-configuration with the emitter and detector positioned on opposite branches of the V-configuration. This configuration is advantageous for use with a newborn baby.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates a schematic medium comprising N different constituents.

FIG. 2a illustrates an ideal plethysmographic signal that would be measured by the optical probe of the present invention when utilized for pulse oximetry.

FIG. 2b illustrates a realistic signal measured by the optical probe of the present invention when utilized for pulse oximetry.

FIG. 3 is a perspective view of a probe of the present invention having a single segment chamber.

FIG. 4 is a cross-sectional view of an optical probe of the present invention illustrating a single segment chamber having a detector within it.

FIG. 5 is a cross-sectional view of a probe of the present invention having a detector resting on a shell of base material.

FIG. 6 is a cross-sectional view of a probe of the present invention incorporating a light collecting lens.

FIG. 7 is a cross-sectional view of a probe of the present invention illustrating a single segment chamber having an LED within it.

FIG. 8 is a cross-sectional view of a probe of the present invention incorporating a collimating lens assembly.

FIG. 9 is a cross-section view of a probe of the present invention wherein the LED and the detector are not aligned along the central axis of the chamber.

FIG. 10 is a perspective view of another embodiment of a probe of the present invention having a two segment chamber.

FIG. 11 is a cross-sectional view of another embodiment of the probe of FIG. 10 incorporating a two segment chamber having a detector within it.

FIG. 12 is a cross-sectional view of another embodiment of the probe of FIG. 10 incorporating a light collecting lens in a two segment chamber.

FIG. 13 is a perspective view of a probe of the present invention having a three segment chamber.

FIG. 14 is a cross-sectional view of the probe of FIG. 13 incorporating a three segment chamber having a detector within it.

FIG. 15 is a cross-sectional view of another embodiment of the probe of FIG. 13 incorporating a light collimating lens.

FIG. 16 is a perspective view of a probe of the present invention specifically designed to be used with a digit.

FIG. 17 illustrates a schematic finger comprising fingernail, skin, bone, tissue, muscle, blood, etc.

FIG. 18 is a cross-section view of the probe of FIG. 16.

FIG. 19 is a longitudinal cross-sectional view of the probe of FIG. 16.

FIG. 20 is a cross-sectional view of another embodiment of the probe of FIG. 16 incorporating a light collecting lens.

FIG. 21 is a cross-sectional view of a probe of the present invention designed to be utilized for reflectance measurements.

FIG. 22 is a cross-sectional view of a probe which is advantageously used for non-invasive measurements when a material is compressible on more than one side. The probe has two bases, each with a chamber to house a detector or an energy source and thereby reduce motion artifacts.

FIG. 23 is a cross-sectional view of a probe having a generally cone-shaped chamber with a reflective surface which advantageously causes energy to be concentrated, or "funneled," onto the surface of a detector within the chamber, improving the measured signal.

FIG. 24 is a schematic of one system which may advantageously employ a probe of the present invention.

FIG. 25 is a cross-sectional view of a probe wherein the aperture is filled with a compressible scattering medium.

FIG. 26 is a cross-sectional view of a probe wherein the LED is spaced from the material to be measured by a transmission assembly having a scattering medium interposed between the LED and the material.

FIG. 27 is a cross-sectional view of a probe wherein a scattering medium is interposed between the LED and the material as well as between the material and the photodetector.

FIG. 28 is a cross-sectional view of a preferred embodiment of a probe in accordance with the present invention having an immersion lens for the photodetector and for the LED and having scattering medium interposed between the LED and the test material as well as between the test material and the photodetector.

FIGS. 29A–29B are perspective views illustrating the use of one embodiment of the disposable optical probe of the present invention to measure the characteristics of a human fingertip.

FIG. 30 is a flow chart which details a method of manufacturing the low-noise optical probe shown in FIGS. 29–29B.

FIG. 31 depicts a first step of the manufacturing process, wherein multiple rows of flex circuit panels are etched onto a flex circuit panel comprising, for example, copper/MYLAR™, copper/CAPTAN™, or conductive ink/MYLAR™.

FIG. 31A depicts the placement of detector shields on pressure sensitive adhesive at detector end of the flex circuit.

FIG. 31B illustrates a second step in the manufacturing process, wherein components are placed and soldered onto the flex circuits of FIG. 31.

FIGS. 32A and 32B illustrate a third step in the manufacturing process, wherein the flex circuits are placed onto a strip of flex circuit shield material.

FIGS. 33A and 33B depict a fourth step of the manufacturing process, wherein the flex circuit assemblies are die cut

and the shields are folded over the flex circuits to provide the completed flex circuit assemblies.

FIG. 34 illustrates a fifth step of the manufacturing process, wherein a connector tab and a detector cavity are placed onto a sheet of base material.

FIG. 35 depicts a sixth stage of the manufacturing process, wherein the flex circuit assembly is positioned on the base material.

FIG. 36 illustrates a seventh step in the manufacturing process, wherein a cover is placed over the detector cavity.

FIG. 37 illustrates an eighth step of the manufacturing process, wherein face stock is placed over the flex circuit assembly on the base material.

FIG. 38 illustrates a ninth step of the manufacturing process, wherein the optical probe is die cut to the final shape shown in FIG. 29a.

FIGS. 39A–39C illustrate an optical cavity in detail.

FIGS. 40A and 40B illustrate the application of the a neonatal probe made in accordance with the present invention.

FIG. 41 is a flow chart which details the general method used for manufacturing a neonatal disposable optical probe in accordance with a second embodiment of the present invention.

FIG. 42 illustrates a first step of the manufacturing process for a neonatal embodiment of the low-noise optical probe, wherein a first layer of tape is laid out.

FIG. 43 illustrates a second step in the manufacturing process for the neonatal probe, wherein a second elongated layer of tape is laid out over the first layer of FIG. 41.

FIGS. 44A–44C illustrate an optical cavity in detail.

FIGS. 45A–45C illustrate the manufacture of the neonate flex circuit assembly.

FIG. 46 illustrates a third step in the manufacturing process for the neonatal probe, wherein the flex circuit is laid out with a connector as well as an optical probe onto the second layer of tape.

FIG. 47 illustrates a fourth step in the manufacturing process of the neonatal probe, wherein the third and fourth layers of tape are laid over the flex circuit.

FIG. 48 illustrates a fifth step in the manufacturing process wherein the neonatal probe is die-cut to the final shape.

FIGS. 49 and 50 depict an alternative embodiment of the neonatal probe wherein a soft, hospital wrap is used to affix the probe to a newborn's foot.

FIGS. 51–54 illustrate an alternative method of manufacturing the neonate probe.

FIGS. 55A–55C depict a cover which is affixed over the optical cavity.

FIG. 56 depicts a clip-on version of the optical probe.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Examination of a material is often advantageous, especially when it is difficult or expensive to procure and test a sample of the material. For example, in physiological measurements, it is often desirable to monitor a patient without drawing of blood or tissue from the patient. The known properties of energy absorption as energy propagates through a material may be used to determine information about the material through which the energy has passed. Energy is made incident on a material, and a measurement is made of energy either transmitted by or reflected from the material.

The amplitude of the measured signal is highly dependent on the thickness of the material through which the energy passes, or the optical path length, as well as other properties such as the erratic movement of venous blood during motion. A schematic medium **20** comprising N different constituents A_i through A_N is shown in FIG. 1. Energy transmitted through the medium **20** is approximately attenuated according to the equation:

$$I \approx I_0 e^{-\sum_{i=1}^N \epsilon_i c_i x_i} \quad (1)$$

where ϵ_i is the absorption coefficient of the i^{th} constituent; x_i is the thickness of the i^{th} constituent through which light energy passes, or the optical path length of the i^{th} ; and c_i is the concentration of the i^{th} constituent in thickness x_i .

Since energy absorption is strongly dependent on the thicknesses of the constituents A_i through A_N which make up the medium **20** through which the energy passes, when the thickness of the medium **20** changes, due to motion for example, the thicknesses of the individual constituents A_i through A_N change. This causes the absorption characteristics of the medium **20** to change.

Often a medium **20** is under random or erratic motion. For example, if the medium **20** is an easily compressible portion of a patient's body, such as a digit, and the patient moves, the medium **20** compresses erratically causing the individual thicknesses X_i through X_N of the constituents A_i through A_N to vary erratically. This erratic variation may cause large excursions in the measured signal and can make it extremely difficult to discern a desired signal, as would be present without motion induced noise, or motion artifacts.

For example, FIG. 2a illustrates an ideal desired signal waveform, labeled Y, measured in one application of the present invention, namely pulse oximetry. FIG. 2b illustrates a more realistic measured waveform S, also measured in a pulse oximetry application, comprising the ideal desired signal waveform Y plus motion induced noise, n, i.e. $S=Y+n$. It is easily seen how motion artifacts obscure the desired signal portion Y.

FIG. 3 is a perspective view of one embodiment of an optical probe **100** of the present invention which greatly diminishes the effects of motion artifacts on the measured signal. FIG. 4 shows a cross-sectional view of the optical probe **100** of the present invention taken along line 4—4 in FIG. 3. For clarity in the perspective view of FIG. 3, a material **128** on which measurements are to be taken is not shown placed adjacent the probe **100**. However, the material **128** on which measurements are to be made is shown in FIG. 4. As illustrated in FIGS. 3 and 4, a base **110**, having a top **112**, a bottom **114**, a forward end **116**, and a rear end **118**, is made of a material which is preferably rigid and opaque. It will be understood, however, that the probe **100** may be made of materials which may be rigid, resilient, opaque, or transparent, for example.

An aperture **120** is formed in the top **112** of the base **110**. Typically, the aperture **120** is located at a point between one-quarter and one-half of the length of the base **100**. The aperture **120** may be of any shape, including but not limited to circular, square, or triangular. The aperture **120** forms the opening to a chamber **122** which may also be of any shape. In one embodiment, a lateral cross-section (not shown) of the chamber **122** is the same shape as the aperture. A central axis **124** of the chamber **122** is defined by a line aligned perpendicular to the aperture **120** and extending generally through a central portion of the aperture **120**.

In the embodiment of FIG. 4, a light source **130**, typically a light emitting diode (LED), is affixed adjacent the material

128, aligned along the central axis **124** of the chamber **122** opposite the chamber **122**. Typically, an adhesive such as medical tape is used to affix the LED **130** to the material **128**. A detector **126**, such as a photodetector, is placed within the chamber **122**. A central portion of the photodetector **126** is generally aligned with the central axis **124** of the chamber **122**, typically at the bottom **114** of the chamber **122**. The photodetector **126** may be fixed within the chamber **122** according to a number of different methods, including but not limited to adhesive, a press fit, or clear epoxy resin which transmits light over a range of wavelengths of interest. Typically, no matter how the photodetector **126** is held within the chamber **122**, the bottom surface **114** of the chamber **122** is made opaque either via the press fit or via paint or tape, for example.

It is often the case that materials **128** on which absorption measurements are performed are, at least in part, easily compressible. Easily compressible portions of the material **128** are placed directly adjacent (i.e., above) the chamber **122**. The area surrounding the aperture **120** supports the material covering the chamber **122**. The chamber **122** is wide enough that any compressible portion of the material **128** located above the aperture **120** may intrude into the chamber **122**. Thus, the material **122** may rest above or penetrate slightly into the chamber **122** and is thereby shielded from perturbations which compress the material **128**, such as pressure caused when the material **128** is touched.

In the present embodiment, the depth of the chamber **122** may range from 0.5 mm to 10 mm in depth, with 2–4 mm preferred, and 3–4 mm more preferred. Similarly, the diameter of the aperture **120** may, in the present embodiment, range from 3 mm to 20 mm, as required by the specific application. For instance, the aperture would be smaller for neonates than for adults. These sizes have been found to be effective in reducing perturbations and compression of the material **128**, when the material is human skin.

The chamber **122** is deep enough that the photodetector **126** and the bottom **114** of the chamber **122** do not come into contact with the easily compressible portion of the material **128**, even when the material **128** is caused to move. Thus, along the central axis **124** of the chamber **122** nothing comes into physical contact with the easily compressible portion of the material **128** and causes it to compress. With little or no compression of the material **128** in this region, the thickness of the material **128**, or the optical path length of light energy propagating through the material **128**, is substantially stabilized in the field of view of the photodetector. The movement of venous blood due to compression is also minimized in the field of view of the photodetector.

The LED **130** emits light at a known wavelength. The light propagates through the material **128** and an attenuated signal is transmitted into the chamber **122** to be received by the photodetector **126**. As light from the LED **130** propagates through the material **128**, it is scattered by the material **128** and is thus transmitted into the chamber **122** over a broad range of angles in a very complex manner. Thus, some of the light is caused to be incident on the opaque walls **123** of the chamber **122** and is absorbed. Although the signal travels through a greater optical distance to reach the photodetector **126** at the bottom **114** of the chamber **122** than if the photodetector **126** were immediately adjacent the material **128**, thus eliminating direct coupling between the photodetector **126** and the material **128**, the resulting degradation to signal intensity is compensated for by the stabilization of the optical path length and the resultant reduction of noise in the measured signal. The photodetector

126 produces an electrical signal indicative of the intensity of light energy incident on the photodetector 126. The electrical signal is input to a processor which analyzes the signal to determine characteristics of the media 128 through which the light energy has passed.

The opaque quality of the base 110 absorbs ambient light which can interfere with the signal measured at the photodetector 126. This further improves signal quality. Further, the opaque bottom 114 of the chamber 122 protects the photodetector 126 from ambient light which can obscure the desired signal measured at the photodetector 126. Thus, an accurate measurement of the intensity of the attenuated signal may be made at the photodetector 126.

An alternative embodiment of the chamber 122 is shown in frontal cross-section in FIG. 5. A shell 131 of base 110 material covers the bottom 114 of the chamber 122. The photodetector 126 is mounted on the shell 131, within the chamber 122, generally aligned with the LED 130. The photodetector 126 is electrically connected to a processor through a small hole (not shown) in the shell 131. The shell 131 shields the photodetector 126 from ambient light which can seriously degrade the signal-to-noise ratio of the signal measured at the photodetector 126. It will be understood that the bottom 114 of the chamber 122 may be formed with or without the shell in any embodiment of the probe of the present invention.

FIG. 6 shows a frontal cross sectional view of another embodiment of the probe 100 of the present invention wherein a light collecting lens 132 is placed within the chamber 122, between the material 128 which rests above or enters into the chamber 122 and the photodetector 126. The lens 132 has one generally planar surface 132a aligned parallel to the aperture 120 in the top 112 of the base 110, located deep enough within the chamber 122 that any material 128 which intrudes into the chamber 122 does not contact the planar surface 132a of the lens 132. Another surface 132b of the lens 132 is generally convex having its apex directed toward the photodetector 126 in the bottom 114 of the chamber 122. The lens 132 may be held in the chamber 122 by a number of means, including but not limited to optical adhesive, a lens retaining ring, or a press fit. The chamber 122 functions in the same manner as described above to stabilize the optical path length and reduce motion artifacts. The light collecting lens 132 gathers much of the light which was scattered as it was transmitted through the material 128 and causes it to be incident on the photodetector 126. This produces a stronger measured signal.

FIG. 7 shows another embodiment of the probe 100 of the present invention wherein the positions of the photodetector 126 and the LED 130 are interchanged. The LED 130 is placed within the chamber 122, typically at the bottom 114 of the chamber 122, generally aligned with the central axis 124 of the chamber 122. The LED 130 may be fixed within the chamber 122 according to a number of different methods, including but not limited to a press fit, adhesive, or clear epoxy resin which transmits light over a range of wavelengths of interest, such as around the wavelength which the LED emits. Again, a material 128 is placed on the base 110 having a compressible portion of the material 128 located directly above the chamber 122. The photodetector 126 is attached to the material 128, opposite the LED 130, such that the LED 130, the photodetector 126, and the chamber 122 are aligned along the central axis 124 of the chamber 122. The photodetector 126 is typically attached by an opaque material. For example, the photodetector 126 may be attached to the material 128 with opaque tape, thereby

limiting signal degradation caused by ambient light. The photodetector 126 is, again, electrically connected to a processor.

The probe 100 of this embodiment functions substantially identically to the embodiment of the probe 100 having the photodetector 126 housed in the chamber 122. The chamber 122 stabilizes the optical path length by allowing easily compressible portions of the material 128 to rest above or intrude into the chamber 122, thereby stabilizing the optical path length and substantially reducing motion artifacts. This is true regardless of whether the photodetector 126 or the LED 130 is housed within the chamber 122.

FIG. 8 shows a cross-sectional view of another embodiment of the probe 100 of the present invention wherein the LED 130 is located within the chamber 122. A collimating lens assembly 140 is placed within the chamber 122, between the material 128 which rests above or enters into the chamber 122 and the LED 130. Collimating lens assemblies 140 are well known in the art and, thus, the lens assembly 140 is represented schematically in the FIG. 8. The collimating lens assembly 140 is located deep enough within the chamber 122 that any material 128 which intrudes into the chamber 122 does not contact the lens assembly 140. The lens assembly 140 may be held in the chamber 122 by a number of means, including but not limited to optical adhesive, a lens retaining ring, or a press fit. The chamber 122 functions in the same manner as described above to stabilize the optical path length and reduce motion artifacts. The collimating lens assembly 140 causes light from the LED 130 to be focused on the material 128 above the chamber 122, thus providing a less scattered signal transmitted onto the photodetector 126 surface, thereby utilizing the photodetector 126 more effectively.

FIG. 9 shows another embodiment of the probe 100 of the present invention wherein the LED 130 and the photodetector 126 are not aligned along the central axis 124 of the chamber 122. Light is scattered within the material 128, causing at least a portion of the light emitted by the LED 130 to reach the photodetector 126 for measurement. As long as light emitted by the LED 130 and scattered by the material 128 reaches the photodetector 126 with great enough intensity to be measured, the LED 130 and the photodetector 126 need not be aligned. While alignment of the LED 130 and the photodetector 126 along the same axis causes the light emitted by the LED 130 to reach the photodetector 126 more directly, it is not necessary for operation of the probe of the present invention. In some applications, misalignment may even be advantageous. It will be understood that this is true for any embodiment of the probe of the present invention. Additionally, it will be understood that a photodetector 126 which fills the width of the chamber 122 is advantageous in that more of the light directed into the chamber 122 will be incident on the surface of the photodetector 126, resulting in a stronger measured signal. However, any size photodetector 126 which acquires enough energy to produce an adequately strong measured signal is acceptable. It will be understood that this is true for any embodiment of the probe of the present invention.

A perspective view of another embodiment of a probe 200 of the present invention comprising a multi-segment chamber 222 is shown in FIG. 10. FIG. 11 shows a cross-sectional view of the probe 200 of the present invention taken along line 11—11 in FIG. 10. For clarity in the perspective view of FIG. 10, a material 228 on which measurements are to be taken is not shown placed adjacent the probe 200. However, the material 228 is shown adjacent the probe 200 in FIG. 11.

As illustrated in FIGS. 10 and 11, a base 210, having a top 212, a bottom 214, a forward end 216, and a rear end 218,

is made of a material which is preferably rigid and opaque. It will be understood, however, that the probe **200** may be made of materials which may be rigid, resilient, opaque, or transparent, for example. An aperture **220** of any shape is formed in the base **210**, similar to the aperture **120** described above in conjunction with the probe **100** of FIGS. **3** through **9**. The aperture **220** forms the opening to a stabilizing segment **222a** of the multiple segment chamber **222**. A lateral cross-section (not shown) of the stabilizing segment **222a** of the chamber **222** is typically the same shape as the aperture **220**. Walls **223a** of the stabilizing segment **222a** are generally perpendicular to the aperture **220**. A central axis **224** of the chamber **222** is defined by a line aligned generally perpendicular to the aperture **220** and extending generally through a central portion of the aperture **220** and the chamber **222**.

A mounting segment **222b** is located directly adjacent and below the stabilizing segment **222b**, connected to the stabilizing segment **222b** by a border **225**. The mounting segment **222b** shares the central axis **224** of the stabilizing segment **222a** and is typically of smaller width. Walls **223b** of the mounting segment **222b** are generally parallel to the central axis **224**. The mounting segment **222b** may extend through the bottom **214** of the base **210**, as shown in FIG. **11**, or the mounting segment **222b** may extend to just above the bottom **214** of the base **210**, leaving a shell (not shown) of base **210** material at the bottom **214** of the chamber **222**.

A photodetector **226** is placed in the mounting segment **222b** of the chamber **222**, typically at the bottom **214** of the mounting segment **222b**, having a central portion of the photodetector **226** generally aligned with the central axis **224** of the chamber **222**. The mounting segment **222b** of the chamber **222** is deep enough that the photodetector **226** does not penetrate into the stabilizing segment **222** of the chamber **222**. The photodetector **226** may be fixed within the chamber **222** according to a number of different methods, including but not limited to adhesive, a press fit, or a clear epoxy resin which transmits light over a range of wavelengths of interest. In this embodiment, the bottom **214** of the chamber **222** is made opaque via paint or tape, for example, or by leaving a shell (not shown) of base **210** material at the bottom **214** of the chamber **222** when the chamber **222** is formed. The photodetector **226** is electrically connected to a processor, similarly to the photodetector **126** in the previous embodiment of the probe **100** of the present invention.

An energy absorbing material **228** (the material under test) is placed over the base **210** as shown in the cross section of FIG. **11**. A portion of the material **228** may rest above the chamber **222**. Additionally, the stabilizing segment **222a** of the chamber **222** is wide enough that any easily compressible portion of the material **228** may intrude into the stabilizing segment **222a** of the chamber **222**. The stabilizing segment **222a** of the chamber **222** is deep enough that the portion of the material **228** which enters into the stabilizing segment **222a** does not contact matter within the stabilizing segment **222a** which might cause compression, even when the material **228** is caused to move.

A light emitting diode (LED) **230** is affixed adjacent to the material **228**, opposite the aperture **220**. The LED **230** is advantageously aligned along the central axis **224** to optimize the amount of light incident directly through the material **228** onto the photodetector **226**. However, it will be understood that the positions of the photodetector **226** and the LED **230** could be interchanged as discussed in conjunction with FIG. **7**. Additionally, a collimating lens assembly (not shown) could be added to the chamber **222** as

discussed in conjunction with FIG. **8**. The collimating lens assembly may be held in the chamber **222** similarly to a light collecting lens **232** discussed below. Further, it will be understood that the LED **230** and the photodetector **226** could be unaligned, as discussed in conjunction with FIG. **9**.

As light from the LED **230** propagates through the material **228**, it is scattered by the material **228** and is thus transmitted into the chamber **222** over a broad range of angles. Thus, some of the light is caused to be incident on the opaque walls **223a** and **223b** of the chamber **222** and is absorbed. However, the advantageous alignment of the photodetector **226** and the LED **230** along the central axis **224** causes a large percentage of the light to be incident on the surface of the photodetector **226**. Since the material **228** remains substantially uncompressed above and within the stabilizing segment **222a**, the thickness through which the light travels, or the optical path length, is substantially stabilized. Thus, the signal-to-noise ratio of the measured signal is improved by the suppression of motion artifacts due to the chamber **222**.

In another embodiment of the probe **200**, a light collecting lens **232** is inserted within the chamber **222**, as shown in cross-section in FIG. **12**. The lens **232** is advantageously supported at the border **225** between the stabilizing segment **222a** and the mounting segment **222b**. The lens may be held in place by a number of means, including but not limited to an optical adhesive, a lens retaining ring, or a press fit. The lens **232** has a generally planar surface **232a** aligned with the border **225** between the stabilizing segment **222a** and the mounting segment **222b** and a generally convex surface **232b** extending into the mounting segment **222b** of the chamber **222**. The stabilizing segment **222a** of the chamber **222** is deep enough that the lens **232** does not contact any of the compressible material **228** which may have intruded into the chamber **222**.

The lens **232** collects light which is incident on the planar surface **232a**. Much of the light which is incident on this surface **232a** at angles which would be absorbed by the walls **223a** and **223b** of the chamber **222** if the lens were not present is now directed toward the photodetector **226**. Thus, a greater percentage of the light transmitted through the material **228** is caused to be incident on the photodetector **226**, resulting in a stronger measured signal.

A perspective view of another embodiment of the probe **300** of the present invention which incorporates a chamber **322** having three segments **322a**, **322b**, and **322c** is shown in FIG. **13**. The probe **300** has a base **310** with a top **312**, a bottom **314**, a forward end **316**, and a rear end **318**. The base **310** is typically made of rigid opaque material. However, it will be understood that the base **310** may be made of other materials which may be rigid, resilient, opaque, or transparent, for example. A cross-sectional view of the chamber **322** of this embodiment is shown in FIG. **14**. For clarity in the perspective view of FIG. **13**, a material **328** on which measurements are to be taken is not shown placed adjacent the probe **300**. However, the material **328** is shown in the cross section of FIG. **13**. An aperture **320** of any shape is formed in the base **310**, similar to the apertures **120** and **220** described above. The aperture **320** forms the opening to a stabilizing segment **322a** of a three segment chamber **322**. A lateral cross-section (not shown) of the stabilizing segment **322a** of the chamber **322** is typically the same shape as the aperture **320**. Walls **323a** of the stabilizing segment **322a** are generally perpendicular to the aperture **320**. A central axis **324** of the chamber **322** is defined by a line aligned perpendicular to the aperture **320** and extending generally through a central portion of the aperture **320** and the chamber **322**.

A second, transitional segment **322b** of the chamber **322** is adjacent the stabilizing segment **322a** of the chamber **322**. A top border **325a** is formed between the transitional segment **322b** and the stabilizing segment **322a** of the chamber **322**. The transitional segment **322b** shares the same central axis **324** as the stabilizing segment **322a**. Walls **323b** of the transitional segment **322b** are angled inwardly such that a bottom border **325b** of the transitional segment **322b** is of smaller dimension than the top border **325a** of the transitional segment **322b**.

The bottom border **325b** of the transitional segment **322b** leads into a mounting segment **322c** of the chamber **322**. The mounting segment **322c** shares the same central axis **324** of the stabilizing and transitional segments **322a** and **322b** and is typically of smaller width than the stabilizing and transitional segments **322a** and **322b**. Walls **323c** of the mounting segment **322c** are generally parallel to the central axis **324**. Thus, any cross-section of the mounting segment **322c** cut perpendicular to the central axis **324** of the chamber **322** is typically of approximately the same shape as the bottom border **325b** of the transitional segment **322b** of the chamber **322**. The mounting segment **322c** may extend through the bottom **314** of the base **310**, as shown. Alternatively, the mounting segment **322c** may extend to just above the bottom **314** of the base **310**, leaving a shell (not shown) of base **310** material at the bottom **314** of the three segment chamber **322**.

A photodetector **326** is placed within the mounting segment **322c** of the chamber **322**, at the bottom **314** of the chamber **322** in the present embodiment. A central portion of the photodetector **326** is aligned with the central axis **324** of the chamber **322**. The mounting segment **322c** of the chamber **322** is deep enough that the photodetector **326** does not penetrate into the stabilizing segment **322** of the chamber **322**. The photodetector **326** may be fixed within the chamber **322** according to a number of different methods, including but not limited to adhesive, a press fit, or a clear epoxy resin which transmits light over a range of wavelengths of interest. In this embodiment, the bottom **314** of the chamber **322** is made opaque via the press fit, paint, or tape, for example. The photodetector **326** is electrically connected to a processor, similarly to the photodetectors **126** and **226** in the previous embodiments of the probe of the present invention.

When a portion of an energy absorbing material **328** is placed over the probe **300**, as shown in the cross-section of FIG. **14**, it may rest above the chamber **322**. Additionally, the stabilizing segment **322a** of the chamber **322** is wide enough that easily compressible portions of the material **328** may enter into the stabilizing segment **322a** of the chamber **322**. The stabilizing segment **322a** of the chamber **322** is deep enough that the easily compressible portion of the material **328** which intrudes into the stabilizing segment **322a** does not contact matter within the stabilizing segment **322a** which might cause compression of the material **328**, even when the material **328** is caused to move. The chamber **322** shields the compressible material **328** from contact which might cause compression of the material **328** and thereby change the optical path length through the material **328**.

An LED **330** is affixed to the material **328**, opposite the aperture **320**. The LED **330** is advantageously aligned along the central axis **324** to optimize the amount of light incident directly through the material **328** onto the photodetector **326**. It will be understood that the positions of the photodetector **326** and the LED **330** could be interchanged as discussed in conjunction with FIG. **7**. Additionally, a collimating lens assembly (not shown) could be added to the

chamber **322** as discussed in conjunction with FIG. **8**. The collimating lens assembly may be held in the chamber **322** similarly to a light collecting lens **332** discussed below. Further, it will be understood that the LED **330** and the photodetector **326** could be unaligned, as discussed in conjunction with FIG. **9**.

As light from the LED **330** propagates through the material **328**, it is scattered by the material **328** and is thus transmitted into the chamber **322** over a broad range of angles. Thus, some of the light is caused to be incident on the opaque walls **323a**, **323b**, and **323c** of the chamber **322** and is absorbed. However, the advantageous alignment of the photodetector **326** and the LED **330** along the central axis **324** of the chamber **322** causes a large percentage of the light to be incident on the surface of the photodetector **326**. Since the material **328** remains substantially uncompressed above and within the stabilizing segment **322a**, the thickness through which the light travels, or the optical path length, is substantially stabilized. Thus, the signal-to-noise ratio of the measured signal is improved by the suppression of motion artifacts. Additionally helping to improve the signal to noise ratio of the measured signal is the opaque bottom **314** of the mounting segment **322c** which shelters the photodetector **326** from ambient light.

In another embodiment of the probe **300** of the present invention, a light collecting lens **332** is added to the transitional segment **322b** of the chamber **322**, as shown in a cross sectional view in FIG. **15**. The lens **332** is supported in the transitional segment **322b** and may be held in the transitional segment **322b** by a number of means, including but not limited to optical adhesive, a lens retaining ring, or a press fit. The lens has a generally planar surface **332a** aligned with the top border **325a** of the transitional segment **322b** of the chamber **322** and a generally convex surface **325b** extending into the transitional segment **322b** of the chamber **322**. The stabilizing segment **322a** of the chamber **322** is deep enough that the lens **332** does not contact the easily compressible material **328** which rests above or has intruded into the chamber **322**.

The lens **332** collects light which is incident on the planar surface **332a**. Much of the light which is incident on this surface **332a** at angles which would have been absorbed by the walls **323a**, **323b** and **323c** of the chamber **322** if the lens **332** were not present is now directed toward the photodetector **326**. Thus, a greater percentage of the light transmitted through the material **328** is caused to be incident on the photodetector **326**, resulting in a stronger measured signal.

It will be understood that the walls **323b** of the transitional segment **322b** in each of the above described embodiments need not be sloped to achieve transition from larger width in the stabilizing segment **322a** to smaller width in the mounting segment **322c**. The walls **323b** of the transitional segment **322b** could be aligned generally parallel to the central axis **324**, arranged at a distance which would cause the width of the transitional segment **322b** to be less than the width of the stabilizing segment **322a** and greater than the width of the mounting segment **322c**.

FIG. **16** shows a perspective view of another probe **400** of the present invention specifically designed for use with a digit, such as a finger or a toe. For ease of illustration, the present example will pertain to a finger, though it will be understood that the present example could equally well pertain to any digit. FIG. **17** illustrates a schematic finger **428** comprising nail, skin, bone, tissue, muscle, blood, etc. Constituents in the finger's pad **404**, such as fat and tissue, are easily compressible with motion of a patient. Even slight motion of the finger **428** can cause the thickness of con-

stituents within the finger 428 to change greatly, thereby causing large motion induced excursions to occur in a measured signal, often obscuring a desired portion of the measured signal from which information about the patient can be determined.

As depicted in FIG. 16, base 410 of the finger probe 400, called a saddle 410 in this embodiment, is generally semi-cylindrical and preferably is made of a rigid or semi-rigid, opaque material such as black plastic. It will be understood, however, that the saddle 410 may be made of other materials, including those which are rigid, resilient, opaque, and transparent, for example. The saddle 410 has a top 412, a bottom 414, a forward end 416, a rear end 418, a ridge 440, and sidewalls 450 which curve upwardly from the ridge 440 to form a U-shape in cross-section, as shown in FIG. 18.

As illustrated in FIGS. 16 and 18, an aperture 420 forms the entrance to a chamber 422, located between one-quarter to one-half of the length of the saddle 410 from the forward end 416 of the saddle 410, as shown in the longitudinal cross-section of FIG. 19. The aperture 420 can be of any shape, including but not limited to circular, square, or triangular. The aperture 420 is the entrance to a chamber 422, as described previously in conjunction with other embodiments 100, 200, and 300 of the probe of the present invention. The chamber 422 may also be of any shape, including but not limited to circular, square, or triangular in cross-section.

The chamber 422 may have one or more segments, as described previously. Although the chamber 422 shown in this embodiment is a three segment chamber 422, having a stabilizing segment 422a, a sloped-wall transitional segment 422b, and a mounting segment 422c aligned on a common central axis 424, it will be understood that any chamber 422 which protects from compression, a compressible portion of the finger 428 through which light energy passes during absorption measurements, is a viable alternative. It will further be understood that a shell (not shown) of saddle 410 material could cover the bottom 414 of the chamber 422, as described previously with respect to the embodiment of the probe shown in FIG. 5.

A photodetector 426 is placed within the chamber 422, typically at the bottom 414 of the mounting segment 422c of the chamber 422. The photodetector 426 may be in place by adhesive, a press fit, or a clear epoxy resin which transmits light over a range of wavelengths of interest, for example. Typically, the bottom 414 of the chamber 422 is made opaque via tape or paint, for example, such that ambient light does not affect the photodetector 426.

The finger 428 is placed on the saddle 410, the finger pad 404 directly adjacent the aperture 420 and chamber 422. Additionally, the finger pad 404 may rest above the chamber 422. The aperture 420 and stabilizing segment 422a of the chamber 422 are wide enough that any easily compressible portion of the finger 428, such as a portion of the finger pad 404, may intrude into the chamber 422. The stabilizing segment 422a of the chamber 422 is deep enough that any portion of the finger 428 which does penetrate into the stabilizing segment 422a does not contact any matter within the stabilizing segment 422a which might cause compression of the finger 428, even when the finger 428 is caused to move.

An LED 430 is affixed to the finger 428, generally opposite the aperture 420. The LED 430 is typically attached to the finger 428 via adhesive, such as medical tape. The LED 430 is advantageously aligned along the central axis 424 to optimize the amount of light transmitted directly through the finger 428 onto the photodetector 426. However,

it will be understood that the positions of the photodetector 426 and the LED 430 could be interchanged as discussed in conjunction with FIG. 7. Additionally, a collimating lens assembly (not shown) could be added to the chamber 422 as discussed in conjunction with FIG. 8. The collimating lens assembly may be held in the chamber 422 similarly to a light collecting lens 432 discussed below. Further, it will be understood that the LED 430 and the photodetector 426 could be unaligned, as discussed in conjunction with FIG. 9.

The LED 430 emits a light energy signal which propagates through the finger 428 and is transmitted into the chamber 422. The chamber 422 shields from compression the portion of the finger 428 through which light energy passes. Thus, the optical path length of the light through the finger 428 is substantially stabilized and motion artifacts are substantially reduced in the measured signal. It will be understood that a single segment chamber as described in conjunction with FIGS. 3 through 9 or a two segment chamber as described in conjunction with FIGS. 10 through 12 could equally well be used in the finger probe 400 of the present invention to shield the compressible portion of the finger 428 from compression and thereby reduce motion artifacts.

FIGS. 16, 18, and 19 illustrate a perspective view, a frontal cross-sectional view, and a longitudinal cross-sectional view, respectively, of one embodiment of the finger probe 400. The curvature of the saddle 410 is correlated to the average curvature of the finger 428 such that the sidewalls 450 form a semi-circular splint-type support for the finger 428. The saddle 410 is approximately 25 mm long between the forward end 416 and the rear end 418, such that a portion of the finger 428 between its tip 406 and approximately its first knuckle 408 (shown in FIG. 17) fits between the front 416 and the rear 418 ends of the probe 400. The curvature of the saddle 410 is generally defined by a line 460 (shown in FIG. 18) which is tangent to a sidewall 450 at an angle between 30°E and 50°E from horizontal.

The placement of the aperture 420 at a point between one-third and one-half of the length of the saddle 410, causes the thickest section of the compressible portion of the finger 428, or the finger pad 404, to rest above and within the chamber 422. Thus, the portion of the finger 428 with the greatest amount of compressible material is safeguarded from compression by the chamber 422.

In the embodiment of the finger probe 400 shown in FIGS. 16, 18, 19, and 20, the aperture 420 is generally circular and the chamber 422 has three segments 422a, 422b, and 422c, as shown in the cross-sectional view of FIG. 18. Advantageously employed dimensions for the finger probe 400 illustrated in FIGS. 16, 18, 19, and 20 include the stabilizing segment 422a of the chamber 422 being generally cylindrical and having a diameter of approximately seven millimeters. Additionally, the stabilizing segment 422a of the chamber 422 is deep enough that any portion of the finger 428 which penetrates into the chamber remains substantially free of perturbation, even when the finger 428 moves. An advantageous depth for the stabilizing segment 422a is thus approximately two millimeters deep. The mounting segment 422c of the chamber 422 is also cylindrical, having a diameter of approximately five millimeters. The transitional segment 422b of the chamber 422 is of varying diameter, having sloped walls 423b, such that a top border 425a is approximately seven millimeters in diameter and a bottom border 425b is approximately five millimeters in diameter. A detector 426 having up to a 5 millimeter diameter is positioned in the bottom 416 of the mounting segment 422c of the chamber 422.

In another embodiment of the finger probe **400**, a light collecting lens **432** may be added to the finger probe **400** of the present invention, as shown in FIG. **20**. The saddle **410** and the chamber **422** function as discussed above. The lens **432** functions as described above in conjunction with FIGS. **6**, **12**, and **15** to collect light incident on the lens **432** which would be absorbed by the walls **423a**, **423b** and **423c** of the chamber **422** if the lens **432** were not present. Thus, a greater percentage of the light transmitted through the finger **428** is directed onto the photodetector **426**, resulting in a stronger measured signal.

Other embodiments of the probe of the present invention may be specifically designed and manufactured for use with an earlobe or other thin section of the body, such as a nostril or a lip, using the principles described herein. Also, embodiments of the probe of the present invention utilizing the properties of attenuation as energy is reflected from a medium, rather than transmitted through a medium, may be made using similar principles.

A probe **700** specifically designed to measure reflected energy is shown in cross-section in FIG. **21**. A base **710** is placed adjacent a material **728** on which reflectance measurements are to be made. A photodetector **726** and an LED **730** are located within the base **710**. In the embodiment shown in FIG. **21**, the photodetector **726** is positioned within a chamber **722x** and the LED **730** is positioned within a chamber **722y**. Although single segment chambers **722x** and **722y** are illustrated, the chambers **722x** and **722y** may be of any suitable shape and size. The chambers **722x** and **722y** function to stabilize the optical path length, as discussed previously, by shielding from compression any compressible portion of a material which rests above or intrudes into the chambers **722x** and **722y**.

A light collecting lens (not shown) may be added to the chamber **722x** having the photodetector **726** within it, as discussed previously in conjunction with FIGS. **6**, **12** and **15**. Additionally, a collimating lens assembly (not shown) may be added to the chamber **722y** having the LED **730** in it, as discussed previously in conjunction with FIG. **8**. The chambers **722x** and **722y** may be formed with or without a shell (not shown) of base **710** material, as discussed previously in conjunction with FIG. **5**.

It will be understood that in other embodiments (not shown) of the reflectance probe **700**, the photodetector **726** could protrude from the base **710** and the LED **730** be located within a chamber **722y** or the LED **730** could be protrude from the base **710** and the photodetector **726** could be located within a chamber **722x**. Additionally, the photodetector **726** and the LED **730** could be located within a single chamber **722**. In any embodiment the chamber(s) **722** may have any number of segments of any suitable shape.

The type of probe **700** which relies on reflection may be advantageously utilized on materials where a photodetector **726** and an LED **730** cannot be placed on opposite sides of the material **728**, such as with the forehead. However, a reflectance probe **700** can be used anywhere a non-invasive measurement needs to be taken, such as a lip, an earlobe, or a finger, for example.

FIG. **22** shows a cross-sectional view of another probe **800** of the present invention wherein two bases **810x** and **810y** are placed adjacent to a material **828** on which measurements are to be made. The bases **810x** and **810y** are located on opposite sides of the material **828**. A photodetector **826** is placed in a chamber **822x** in the base **810x**. An LED **830** is placed in a chamber **822y** in the base **810y**. The photodetector **826** and the LED **830** are aligned substantially along a central axis **824**. Although two segment chambers

822x and **822y** are illustrated, the chambers **822x** and **822y** may be of any suitable shape and size. Independent of which shape of chamber is utilized, the chambers **822x** and **822y** function to stabilize the optical path length and thereby reduce the effects of motion artifacts on the measured signals.

As discussed previously, the probe **800** may be modified slightly with a light collecting lens (not shown) added to the chamber **822x** with the photodetector **826** in it. A collimating lens assembly (not shown) may be added to the chamber **822y** with the LED **830** in it. Additionally, the chambers **822x** and **822y** may be formed with or without a shell (not shown) of base **810x** and **810y** material. The probe **800** is particularly advantageous when a material **828** is compressible on more than one side since each chamber **822x** and **822y** supports and shields from compression any compressible portion of a material **828** which rests above or intrudes into the chambers **822x** and **822y**, respectively.

FIG. **23** shows a cross-sectional view of another probe **900** of the present invention wherein a chamber **922** having walls **923** is formed to concentrate, or "funnel," energy onto the surface of a photodetector **926**. An aperture **920** is formed in a base **910**, the aperture **920** leading to a generally cone-shaped chamber **922**. The base **910** is placed adjacent a material **928** on which measurements are to be made, the chamber **922** being placed directly adjacent any easily compressible portion of the material **928**. The photodetector **926** is placed within the chamber **922**, typically at the bottom of the chamber **928**. A light emitting diode **930** is placed on the material **928**, generally opposite and aligned with the photodetector **926**.

As discussed previously, a portion of the material **928** is supported by the area surrounding the aperture **920**. Additionally, the aperture **920** and chamber **922** are wide enough that any easily compressible portion of the material **928** may intrude into the chamber **922** without being compressed, thereby shielding this portion of the material **928** from compression, even during motion of the material **928**. This substantially stabilizes the optical path length and improves the signal to noise ratio of the signal measured at the photodetector **926**.

Further improving the signal to noise ratio of measurements made with the probe **900**, reflective material, such as a highly reflective metal, covers the walls **923** of the chamber **922**. This causes light scattered by the material **928** and made incident on the walls of the chamber **922** to be reflected. The cone shape causes the light to be concentrated generally on the photodetector **926**.

Depending upon the shape of the photodetector **926**, the chamber **922** may be advantageously contoured to maximize the funneling of light onto the photodetector **926**. If the photodetector **926** is flat, the chamber is most advantageously shaped having a generally hyperbolic cross-section. However, if the photodetector **926** is spherical or slightly curved, as is often the case due to manufacturing processes, the chamber is most advantageously shaped having a cone-shaped cross-section with uncurved walls **923**.

As discussed previously in conjunction with other embodiments of the probe of the present invention, the probe **900** may be modified to include a light collecting lens (not shown). Alternatively, an LED **930** could be placed within the chamber **922** instead of the photodetector **926**. With the LED in the chamber **922**, a collimating lens assembly (not shown) could be placed within the chamber **922**. Two bases **910** with two generally cone-shaped chambers could be utilized on one or either side of a material **928**. A single base **910** with two generally cone-shaped chambers **922** located

side by side could also be used for reflective measurements. Additionally, the photodetector 926 and the LED 930 need not be aligned along the central axis 924.

FIG. 24 depicts one embodiment of a probe constructed in accordance with the present invention coupled to an oximeter. The oximeter could be any oximeter known in the art which utilizes light attenuation measurements. A block diagram of one possible oximeter is depicted in FIG. 24. The oximeter shown in FIG. 24 is a pulse oximeter wherein the finger probe 400 is employed and two measured signals at different wavelengths, one of which is typically red and the other of which is typically infrared, are alternately passed through the finger 428. Signals measured at the photodetector 426 are then processed to determine the amount of oxygen available to the body. This is evaluated by finding the saturation of oxygenated hemoglobin in blood comprising both oxygenated and deoxygenated hemoglobin.

Two LEDs 430a and 430b, one LED 430a emitting red wavelengths and another LED 430b emitting infrared wavelengths, are placed adjacent the finger 428. The finger probe 400 is placed underneath the finger 428, the aperture 420 and chamber 422 located directly adjacent the finger pad 404. The photodetector 426 in the bottom 414 of the chamber 422 is connected to a single channel of common processing circuitry including an amplifier 530 which is in turn connected to a band pass filter 540. The band pass filter 540 passes signal into a synchronized demodulator 550 which has a plurality of output channels. One output channel is for signals corresponding to visible wavelengths and another output channel is for signals corresponding to infrared wavelengths.

The output channels of the synchronized demodulator 550 for signals corresponding to both the visible and infrared wavelengths are each connected to separate paths, each path comprising further processing circuitry. Each path includes a DC offset removal element 560 and 562, such as a differential amplifier, a programmable gain amplifier 570 and 572 and a low pass filter 580 and 582. The output of each low pass filter 580 and 582 is amplified in a second programmable gain amplifier 590 and 592 and then input to a multiplexer 600.

The multiplexer 600 is connected to an analog-to-digital converter 610 which is in turn connected to a microprocessor 620. Control lines between the microprocessor 620 and the multiplexer 600, the microprocessor 620 and the analog-to-digital converter 610, and the microprocessor 620 and each programmable gain amplifier 570, 572, 590, and 592 are formed. The microprocessor 620 has additional control lines, one of which leads to a display 630 and the other of which leads to an LED driver 640 situated in a feedback loop with the two LEDs 430a and 430b.

Each of the LEDs 430a and 430b alternately emits energy which is absorbed by the finger 428 and received by the photodetector 426. The photodetector 426 produces an electrical signal which corresponds to the intensity of the light energy striking the photodetector 426 surface. The amplifier 530 amplifies this electrical signal for ease of processing. The band pass filter 540 then removes unwanted high and low frequencies. The synchronized demodulator 550 separates the electrical signal into electrical signals corresponding to the red and infrared light energy components. A predetermined reference voltage, V_{ref} , is subtracted by the DC offset removal element 560 and 562 from each of the separate signals to remove substantially constant absorption which corresponds to absorption when there are no motion artifacts. Then the first programmable gain amplifiers 570 and 572 amplify each signal for ease of manipulation. The

low pass filters 580 and 582 integrate each signal to remove unwanted high frequency components and the second programmable gain amplifiers 590 and 592 amplify each signal for further ease of processing.

The multiplexer 600 acts as an analog switch between the electrical signals corresponding to the red and the infrared light energy, allowing first a signal corresponding to the red light to enter the analog-to-digital converter 610 and then a signal corresponding to the infrared light to enter the analog-to-digital converter 610. This eliminates the need for multiple analog-to-digital converters 610. The analog-to-digital converter 610 inputs the data into the microprocessor 620 for calculation of the saturation of oxygen according to known methods, such as those described in U.S. patent application Ser. No. 07/666,060 filed Mar. 7, 1991, and abandoned in favor of continuation U.S. patent application Ser. No. 08/249,690, entitled "SIGNAL PROCESSING APPARATUS AND METHOD," filed May 26, 1994, both assigned to MASIMO CORPORATION, the same assignee as the present patent, and incorporated herein by reference. U.S. patent application Ser. No. 08/320,154, entitled Signal Processing Apparatus, filed on Oct. 7, 1994 is also incorporated by reference herein. The microprocessor 620 centrally controls the multiplexer 600, the analog-to-digital converter 610, and the first and second programmable gain amplifiers 570, 590, 572, and 592 for both the red and the infrared channels. Additionally, the microprocessor 620 controls the intensity of the LEDs 430a and 430b through the LED driver 640 in a servo loop to keep the average intensity received at the photodetector 426 within an appropriate range.

As explained above, the probe of the present invention could be used with a variety of oximeter systems. A recent embodiment of an oximeter by the assignee of the present application is described in detail in U.S. patent application Ser. No. 08/320,154, entitled "Signal Processing Apparatus," and filed Oct. 7, 1994, which patent application is also incorporated herein by reference.

FIGS. 25–28 depict alternative embodiments of the present invention wherein an improved signal to noise ratio is observed in the received signal due to optical scattering effects. A probe 1000, shown in cross-section in FIG. 25, includes a base 1010, having a top 1012, a bottom 1014, and a forward and a rear end (not shown in FIG. 25). The base 1010 is preferably rigid and opaque to the wavelengths used in the probe 1000. An aperture 1020 is formed in the top 1012 of the base 1010. The aperture 1020 may be cylindrical (as shown in FIG. 25), conical, rectangular, or other shapes as called for by the specific application. The depth of the aperture 1020 may, for example, range from 0.5 mm to 10 mm, and is preferably in the range of 2–4 mm in depth in one embodiment, and more preferably in the range of 3–4 mm. Furthermore, the diameter of the aperture 1020 may range from 3 mm to 20 mm, as called for by the specific application. It has been found by the inventors that an aperture less than 0.5 mm in diameter does not obtain the benefits of the present invention.

A light source 1030 (e.g., one or more light emitting diodes) is affixed adjacent to material 1028 (e.g., an earlobe, finger, or other fleshy material), aligned along a central axis 1024 which passes substantially through the center of a photodetector 1026. The aperture 1020 is filled wholly, or in part, by a scattering medium 1040, which may, for example, comprise 2.2 pound polyurethane reticulated foam (although conformable plastic or scattering gels may also be employed). In general, the scattering medium may comprise one of a number of fixotropic materials (i.e., materials

having two or more mixed materials which are conducive to scattering). Ideally, the scattering medium **1040** scatters but does not significantly absorb optical radiation at the operational red (e.g., 660 nm) and infrared (e.g., 940 nm) wavelengths for the oximeter. In other words, the material is clear to optical absorption, but still scatters light.

In operation, the light source **1030** (e.g., two LEDs in the present embodiment) emits optical radiation (e.g., in the red or infra-red spectrum range) which passes through the material under test **1028**. The optical radiation is received by the photodetector **1026** after passing through the scattering medium **1040**. The received optical radiation is scattered by the scattering medium **1040**.

The scattering of the optical radiation within the scattering medium **1040** has been found to increase the signal-to-noise ratio of the received signal. It is believed that the signal-to-noise ratio is improved because there appears to be a reduced effect on the signal from any particular local region of the material **1028** (e.g., flesh). That is, by scattering the signal either prior to or posterior to the material interface, the signal is effectively spread over a larger area of the material **1028**. Thus, perturbations of a locality within the area of exposure will have less effect with a scattered beam over a large area than with a more concentrated signal passing through that same locality. In this way, the effect of perturbations on the average signal is reduced. Also, the foam and plastic cover reduce optical decoupling and geometric variation in the optical light path during motion.

The scattering medium **1040** or plastic cover should be soft (i.e., highly compressible) so that the material **1028** does not significantly compress when the material **1028** presses against the scattering medium **1040**. Compression of the scattering medium **1040** does not significantly alter the amplitude of the measured signal since the scattering medium is not highly absorptive of the optical radiation. Although conformable plastic covers may be used, reticulated foams provide improved optical coupling with flesh. This is because the reticulated foam provides contact in spots rather than across large areas of the flesh. If contact is made across large areas of flesh, microscopic droplets of perspiration or oil can form a layer between the flesh and the scattering medium **1040**. This layer creates an impedance mismatch interface which is absorptive of the optical radiation. Of course, gels may also be used in accordance with the present invention. Such gels should not contain significant amounts of metal salts or silica because these materials absorb light.

The teachings of the present invention depart from conventional methods of improving optical signal-to-noise ratios. Commonly, lens assemblies which focus optical radiation are used to improve the signal-to-noise ratios of optical signals. However, oximetry by means of transmission or reflection is a non-imaging method of optical detection. Thus, the form of the image is not important for detection purposes. For this reason, scattering may be used as a method of improving optical signal quality; whereas, since scattering was thought to degrade signal-to-noise ratios of optical signals, previous methods have not employed optical scattering techniques.

FIGS. **26** and **27** depict further alternative embodiments of the present invention wherein optical scattering is provided prior to the flesh interface, and both prior and posterior to the flesh interface, respectively. In FIG. **26**, an oximetry probe **1045** further has a transmission assembly **1050** which secures the LED **1030** in place within a backing **1055**. A scattering medium **1060**, having a face **1063**, is interposed between the LED **1030** and the material **1028**. In the

embodiment depicted in FIG. **26**, the scattering medium **1060** does not contact the LED **1030**; however, it should be understood that the scattering medium **1060** may contact one or both of the LED **1030** and the material **1028**.

The scattering medium **1060** diffuses the optical radiation emitted by the LED **1030** over a wider area. Thus, the LED **1030**, which is essentially a point source, is transformed into an evenly distributed source of light over the entire area of the face **1063** of the scattering medium **1060**. The diffusion of the light over a wider area provides an improved signal-to-noise ratio.

As seen in FIGS. **26–28**, the light is scattered. This is represented by the energy intensity contours rather than light path indicators. As recognized by the present inventors, the particular light path is not significant. The important aspect is the intensity of the light and the field of view of the photodetector and the light source. This will be explained further in connection with the embodiment of FIG. **28** utilizing an immersion lens.

The operation of a probe **1065** shown in FIG. **27** is essentially the same as that of the probe **1045**, with the exception that the scattering medium **1040** is provided within the aperture **1020**. It has been found that by providing a scattering medium on both sides of the material **1028**, an improved signal-to-noise ratio is observed over the probes having a scattering medium on only one side of the material **1028**.

FIG. **28** depicts a preferred embodiment of a probe **1070** in accordance with the present invention. As depicted in FIG. **28**, the probe **1070** comprises a transmission assembly **1072**, having a light source **1074**, an immersion lens **1076**, scattering medium **1078**, a chamber **1080** defining an aperture **1082** along a support surface **1083** of the transmission assembly. A detector assembly **1084** is similarly configured with a support surface **1085**, a chamber **1086** defining an aperture **1088** along the support surface **1085**, a photodetector **1090**, an immersion lens **1092** and scattering medium **1094**. FIG. **28** further depicts a test material **2000** such as a human tissue (e.g., a finger or earlobe) interposed between the light source assembly **1072** and the detector assembly **1084**.

Several advantages are obtained from the particular configuration shown in FIG. **28**. First, it should be understood that an economical way to fabricate the light source in the photodetector is to utilize small semiconductor LEDs and photodetectors. Such devices are very small, and therefore, have a very small field of view. The inventors have recognized that it is advantageous to improve the field of view of the photodetector and the LED because the surface of the tissue material **2000** at the aperture of the support surfaces is large compared to the surface of the semiconductor photodetector and LED. Thus, without enlarging the field of view of the photodetector and/or LED, much of the tissue material interface at the apertures is not utilized. As explained above, scattering of the light improves the received signal quality. An immersion lens for the photodetector and/or LED increases the field of view of the semiconductor photodetector and LEDs such that a substantial portion of the tissue material covering the apertures is within the field of view of the photodetector and/or LED.

Because imaging optics are not required due to the advantages of scattering, a significantly advantageous configuration is to utilize epoxy placed directly over the photodetector and/or over the LED in the form of a partial sphere which performs suitably as an immersion lens in the present embodiment. In one embodiment, the index of refraction of the epoxy is advantageously 1.56 in the present

embodiment. The epoxy also acts to protect the photodetector and/or LED. The immersion lens can be formed by placing a bump of epoxy over the photodetector and the LED.

The immersion lens formed by a bump of epoxy over the photodetector and/or LED expands the field of view for the photodetector and LED in order to disperse the transmitted light energy over the tissue surface area at the apertures which is large relative to the surface of the optical elements. This assists in minimizing the effects of the relatively small optical details of the test materials (e.g., pores, fingerprint lines, sweat glands).

In the advantageous embodiment of FIG. 28, the scattering material **1080**, **1086** is also placed in the chambers **1080**, **1086** in order to enhance scattering of the light as explained above.

The cone shaped chambers **1080**, **1086** depicted in FIG. 28 are also advantageous when the walls of the chambers are coated with a highly reflective material which does not absorb the light from the LED. The cone shape assists in reflecting the light energy away from the LED and toward the photodetector. All of these elements in combination form a particularly advantageous probe which can maximize the signal-to-noise ratio of the probe and minimize the effects of motion artifact on the received signal.

It should be understood that in alternative embodiments of the probe **1070** depicted in FIG. 28, elements could be removed and still obtain significant benefit. For instance, the detector assembly **1084** could remain the same with the light source assembly **1072** simply becoming an LED with no support surface and no chamber. Alternatively, the scattering media **1078**, **1086** could be removed from either the chamber **1080** in the light source assembly **1072** or the chamber **1086** in the detector assembly **1082**.

The light collecting lens, or other optical elements, could also be added to the chamber in any optical probe of the present invention to direct light onto the photodetector. However, the immersion lens provides better performance. The location of the photodetector and the LED may be interchanged in any of the above described probes. The bottom of any chamber formed in a base of an optical probe of the present invention can remain exposed, be covered by a material such as opaque tape, or be covered by a shell of base material without affecting the reduction of motion artifacts brought about by the chamber. Additionally, reflective measurements could be made with the probes of the present invention by mounting both the photodetector and LED on the base of the probe. Also, a plurality of LEDs or photodetectors could be mounted in the chamber or affixed to the material such that more than one signal may be measured at a time. Furthermore, any material having a chamber, with a detector or an LED mounted within the chamber, will reduce the effects of motion artifacts in non-invasive absorption (or reflection) measurements, according to the present invention.

FIGS. 29A–29B depict one embodiment of a disposable, optical probe **2002**, and the attachment of the optical probe **2002** on the fingertip **2050** of an adult patient. As shown in FIGS. 29A–B, the disposable optical probe **2002** is designed to fit comfortably onto a patient's fingertip. Advantageously, the optical probe **2002** is also configured to provide one or more of the following features: (i) minimization of undesirable movement with respect to the tissue under test (e.g., due to motion by the patient or contact of the probe **2002** with an object or surface); (ii) minimization or prevention of "light piping" (transmission) directly from the light source (e.g., light emitting diode) to the detector (e.g.,

photodetector), (iii) minimization of the detector and LED decoupling from the test site during motion, and (iv) the low noise chamber configuration described above.

As illustrated in FIG. 29A, the probe **2002** includes a central portion **2004**, a pair of adhesive flanges **2005** extending from the central portion **2004**, a connector portion **2010** situated between the flanges **2005**, and a pair of smaller adhesive flaps **2015** extending from the central portion **2004** on the end of the optical probe **2002** opposite from the connector **2010**. The probe **2002** further includes a connection aperture **2012** formed in the connector tab **2010**, an emitter aperture **2020** with an emitter (e.g., a light-emitting diode) positioned within the central portion **2004** close to the connector portion **2010**. A flex pocket **2025** is located within the central portion between the emitter aperture **2020** and a detector aperture **2030** which allows light to pass through the detector aperture **2030** to a detector assembly **2035**. An adult fingertip **2050** is shown in phantom in FIG. 29A to illustrate the position at which the fingertip **2050** would be placed when the probe **2002** is to be fastened onto the fingertip **2050** for use.

Although not depicted specifically in FIGS. 29A–29B, the probe **2002** is fabricated from multiple layers, including a flex circuit layer, a MYLAR™ layer, a face stock tape layer, and other tape layers, depicted further in FIGS. 31–39.

FIG. 29B illustrates the probe **2002** fastened onto the fingertip **2050**. As shown in FIG. 29B, the probe **2002** folds at the location of the flex pocket **2025** over the fingertip **2050** such that the flex pocket **2025** aligns with the very end of the fingertip and such that adhesive flaps **2005** fold downward (in the illustration of FIG. 29B) to wrap around the fingertip **2050** while the adhesive flaps **2015** fold upward (in the illustration of FIG. 29B) about a portion of the circumference of the fingertip **2050** to provide support. As shown in FIG. 29B, when the probe **2002** is folded about the fingertip **2050**, the emitter located within the probe is spaced opposite the detector assembly **2035** such that light from the emitter passes through the emitter aperture **2020**, through the finger **2050** and is incident upon the detector assembly **2035** through the detector aperture **2030**.

Advantageously, when the probe **2002** is attached to the finger, the flex pocket **2025** is aligned at the tip of the finger **2050** so as to provide alignment of the probe **2002** on the fingertip **2050**. The flex pocket **2025** also provides a highly flexible portion, thus providing for reduced movement of the detector and LED assembly with respect to the finger **2050** if the fingertip comes into contact with another object. This provides a more stable probe with increased motion resistance. In other words, the flex pocket also assists in minimizing perturbations in the detected signal due to movement of the detector and emitter with respect to the test tissue (e.g., the finger). Furthermore, the flex pocket **2025** reduces light piping since light is diverted around the circumference of the pocket.

In one embodiment, the flex pocket **2025** is formed to include an air cushion or other cushion material to further absorb contact of the probe **2002** with objects. In this manner, jarring of the probe **2002** in the event the fingertip **2050** moves slightly or in the event of contact of the probe to another surface is minimized.

The probe **2002** includes an internal flex circuit **2051** which acts as a spring-like shock absorber for the disposable probe. The flex circuit **2051** also assists in reducing shifting between the emitter **2021** and the detector assembly **2035** due to contact or motion by the patient. Thus, the internal flex circuit **2051**, together with the flex pocket **2025** act to minimize the decoupling of the detector assembly.

FIG. 29B depicts a receiving connector portion 2060 which engages with contacts 2052 on the connector 2010 to provide an electrical connection between the optical probe 2002 and digital signal processing circuitry (not shown in FIG. 29C). The digital signal processing circuitry may be used to analyze the output of the detector within the assembly 2035. In one advantageous embodiment, the aperture 2012 catches onto a tab (not shown) within the connector 2060 to firmly secure the connector 2060 with the optical probe 2002. Once the optical probe 2002 is securely fastened to the fingertip 2050 and the connector provides an electrical connection between the optical probe 2002 and digital signal processing circuitry, signals are detected from the detector 2035 and transmitted to the processing circuitry via the connector 2060. Further details of the receiving connector portion 2060 are described in a patent application entitled "Patient Cable Connector" filed on the same date as the present application and assigned to the assignee of the present application, which application is incorporated herein by reference as if fully set forth.

FIG. 30 is a flow chart which illustrates the general steps in accordance with the present invention to manufacture a first embodiment of the disposable, optical probe 2002 depicted in FIGS. 29A–29C. A flex circuit is formed on a flex circuit panel as represented by an activity block 3005. In one advantageous embodiment, the flex circuit panel comprises a copper/MYLAR™ or copper/CAPTON™ laminant, or, alternatively, is formed by depositing a conductive ink on MYLAR™. For example, FIG. 31 depicts three etched flex circuits on a flexible circuit panel material. The flex circuits have been formed by etching in one preferred embodiment, and are comprised of one-ounce copper (approximately 1.3 mils) over 1 mil of MYLAR™ or CAPTON™.

After the flex circuit has been etched in an appropriate copper coated MYLAR™ substrate material, conductive pressure sensitive adhesive (PSA) 2102 is applied to the end of the flex circuits where the detector will be placed (hereinafter, the "detector end"), as depicted in FIG. 31. After the conductive PSA (made by 3M in the present embodiment, part No. 9703) is applied, a detector component window 2104 is cut through the conductive PSA 2102 and the flex circuit MYLAR™ base. An emitter component window 2106 is also cut through the flex circuit MYLAR™ base. A flex pocket hole 2108 is also cut through the flexible circuit MYLAR™ base. Next, detector shields 2110 are placed on the PSA at the end of the detector end of the flex circuit, as depicted in FIG. 31A.

In one embodiment, the detector shields are etched copper shields made of copper sheet. A grating 2111, which is about 80% open, is etched through the shields to allow light from the light source (e.g., LED) to transmit through the shield to a detector. The resultant shield has a frame of approximately 4 mils thickness and a grating of approximately 2 mils thickness. The shields provide a Faraday Shield for the detector.

The diffraction grating aligns with the detector component window 2104 in the flex circuit and, when the probe is assembled, with the detector aperture 2030 (FIG. 29A). The conductive PSA 2102 makes electrical connection between a flex circuit ground trace 2112 and the detector shield 2110 to connect the detector shield 2110 to ground.

In one preferred embodiment, low temperature solder paste is dispensed on contacts 2114, 2115, for the detector connections (FIG. 31B), on contacts 2116, 2117 for the emitter connections and on resistor pad 2118 for an identifying resistor. The emitter (LED) 2021, a detector 2120 and

a resistor 2122 are placed and soldered in the appropriate positions on the flex circuits as depicted in FIG. 31B, and represented in an activity block 3010 (FIG. 30). The solder operation is preferably performed through a direct heat reflow of the low temperature solder. The emitter 2021 and detector 2120 are placed such that the transmission and detection field of view are through the detector and emitter windows 2104 and 2106 (FIG. 31).

In one embodiment, the resistor 2122 advantageously is connected to the ground trace on one end and a resistor signal trace 2113 at the other end. In another embodiment, the resistor 2122 is connected in parallel with the emitter 2021. The advantages of this parallel connection are explained in detail in copending application Ser. No. 08/478,493 entitled Manual and Automatic Probe Calibration, which is incorporated herein by reference as if fully set forth.

In one embodiment, the resistor 2122 provides a company identifier. In other words, the resistor 2122 can provide a value that specifically identifies that the probe is made by or for a particular patient monitoring company. As explained in copending application Ser. No. 08/478,493 the resistor can be read by lowering the voltage across the LED to a point where the LED is effectively off, thereby removing the LED from the circuit as a current draw.

As mentioned above, and as seen in FIG. 31B, the flex circuit has the aperture 2108 which is the aperture in the flex circuit forming a portion of the flex pocket 2025 of the probe 2002. In addition to the advantages of the high flexibility, this aperture 2108 through the flex circuit prevents a direct line of transmission between the emitter 2021 and the detector 2120. In other words, in use, light from the emitter 2021 which reaches the detector 2130 should pass through the medium under test (e.g., the finger or other tissue). Direct transmission of stray light from the emitter directly to the detector 2120 along a light conductive surface can cause erroneous readings, especially during motion. This direct transmission of light between the transmitter and detector is referred to herein as "light piping." That is, if the probe between the emitter 2021 and the detector 2120 has optical transmission properties, due to the construction or the material of the probe, stray light from the emitter may channel along the probe directly to the detector, without passing through the tissue material under test. Light piping is a heretofore unrecognized cause of noise and invalid signals from such optical probes. The aperture 2108 minimizes or prevents this "light piping" by preventing or minimizing a direct line of transmission from the emitter 2021 to the detector 2120 along the flexible circuit. Thus, the aperture 2108 provides benefits in the present invention of providing a highly flexible portion of the flex circuit, which reduces decoupling of the LED 2021 and the detector 2120 during motion (due, for example, to tapping on the finger tip), and preventing light piping between the emitter and the detector.

Once the appropriate circuit elements are placed and soldered onto the flex circuit, a flex circuit shield 2130, as depicted in FIG. 32A, is attached to the flex circuit panel as represented in an activity block 3015. The placement of the flex circuit shield 2130 with the flex circuit is depicted in FIGS. 32A and 32B. The flex circuit shield 2130 is advantageously constructed from MYLAR™ laminated with a thin conductive layer such as copper. In the present embodiment, the laminated MYLAR™ is made by ACUTEK.

In the present embodiment, the flex circuit shield 2130 has an insulator film 2132 depicted in double-cross hatching (made by Coating Sciences, part number P-341 in the

present embodiment), a flex circuit shield conductive PSA strip **2133** (made by 3M, part no. 9703 in the present embodiment) and two non-conductive PSA strips **2134**, **2135**. As seen in FIG. 32A, the flex circuit shield **2130** has an emitter aperture **2136**, two flex pocket apertures **2137**, and a detector aperture **2138**.

When the flex circuit shield **2130** is applied to the flex circuit, the insulator strip **2132** insulates the signal traces of the flex circuit from the metallization of the flex circuit shield **2130** to prevent short circuits. As further depicted in FIGS. 32A and 32B, when the flex circuit shield **2130** is positioned such that the apertures align with corresponding apertures on the flex circuit, the PSA strip **2135** provides bonding with the back of the flex circuit, the conductive PSA strip **2133** provides for bonding of one tab of the detector shield **2110** with the flex circuit shield **2130**. The conductive PSA strip **2133** also provides connection of the flex circuit shield with the ground via the detector shield tab.

With the flex circuit shield in position, the flex circuit assembly **2132** (including the flex circuit, the emitter **2021**, the detector **2120**, the resistor **2122**, and the shields **2110**, **2130**), are die-cut, as depicted in FIG. 33A. The flex circuit shield **2130**, along with the detector shield **2110**, is folded over the flex circuit as represented in an activity block **3020**. The final flex circuit assembly **2051** is depicted in FIG. 33B.

Once folded, the insulator film **2132** prevents contact from the flex circuit traces to the metallization in the flex circuit shield **2130**. The PSA strip **2135** bonds the flex circuit shield to the signal circuit side of the flex circuit. As depicted in FIG. 33B, the contact fingers **2052** remain exposed.

As illustrated in FIG. 34, a base material **2140** also forms a layer of the probe **2002**. In one embodiment, the base material comprises Avery 3044 base material. Each side of the base material is coated with PSA adhesive (Coating Sciences, Inc., P-341 in the present embodiment). The back side (in reference to the illustration of FIG. 34) of the base material **214** is provided with the thin release liner **2003** (see FIG. 29A, not shown in FIG. 34), preferably made from a paper release liner or the like, as is well understood in the art.

In the present embodiment, the base material is transparent to the wavelength of the emitter **2021**. The connector tab **2010** and an optical cavity **2150**, are placed onto a first adhesive side of the base material **2140**, as represented within an activity block **3025**, and depicted in FIG. 34. The connector tab **2010** is advantageously formed of ABS styrene, and has the aperture **2012**. The optical cavity **2150** may, for example, have the configuration for its walls in the shape of any of the above-disclosed bases (e.g., the bases **110**, **1010**, etc.) having a chamber formed therein. As depicted in FIG. 34, the optical cavity has a rectangular receiving receptacle **2152** adapted to receive the detector end of the completed flex circuit assemblies.

Additional detail of the optical cavity of the present embodiment of the probe **2002** is depicted in FIGS. 39A–39C. FIG. 39A depicts a perspective view of the optical cavity **2150** for the probe **2002**. FIG. 39B depicts a bottom view of the optical cavity **2150** and FIG. 39C depicts a cross sectional view along 39C–39C of FIG. 39A. The optical cavity **2150** is made from styrene in one embodiment. In one preferred embodiment, the optical cavity is coated with an optical coating that is opaque to ambient light. This can be on the inside walls of the optical cavity or over the exterior walls of the optical cavity, or the entire optical cavity can be coated. The opaque coating advantageously prevents or minimizes the transmission of ambient light from the surrounding environment which could be incident on the detector if the optical cavity is not opaque to

ambient light. As an alternative to an opaque coating, the optical cavity can be made from a material that is opaque to ambient light.

Advantageously, the optical cavity **2150** has a wedge shape ramp **2154** as part of the rectangular receptacle **2152**. As briefly mentioned above, the rectangular receptacle **2152** is adapted to receive the detector end of the flex circuit **2051**. The wedge shaped ramp **2154** of the optical cavity **2150** provides a ramp for a smooth transition for the flex circuit **2051** between the surface of the base material to the rectangular receptacle table **2152**.

Further illustrated in FIG. 40A are two side walls **2156** that runs along the side border of the rectangular receptacle **2152** and an end wall **2157** that runs between the two side walls **2156**. These walls hold the flex circuit **2051** in position such that the detector **2120** aligns properly with an aperture **2158** in the optical cavity. Preferably, the flex circuit fits snugly between the side walls **2156** and against the end wall **2157**.

In a preferred embodiment, the aperture **2158** has the configuration of the cavities describe above (e.g., cone-shaped, cylindrical in shape, or conical in shape, etc.).

Preferably, the PSA on the first adhesive side (FIG. 34) of the base material **2140** allows simple attachment of the optical cavity **2150** and the connector tab **2010** through the application of pressure.

After the connector tab **2010** and the optical cavity **2150** have been placed on the base material **2140**, the flex circuit assembly **2051** is placed on top of the base material **2140**, the connector tab **2010** and the optical cavity **2150** as depicted in FIG. 35 on one end. The detector end **2141** of the completed flex circuit assembly **2051** seats within the rectangular receptacle **2152** of the optical cavity **2150**, as depicted in FIG. 35. Mounting of the completed flex circuit assemblies **2051** is represented in an activity block **3030** (FIG. 30).

With the detector end **2141** of the flex circuit assembly **2051** seated in the receptacle **2152** of the optical cavity **2150**, the photodetector mounted to the flex circuit assembly **2151** is positioned to aligned with the aperture **2158** of the optical cavity **2150**. In one embodiment, a hole, corresponding to the emitter aperture **2020** and the detector aperture **2030**, is cut in the base material to correspond to the emitter **2021** and the detector **2120**. However, in the present embodiment, the base material is transparent to the wavelength of the emitter **2021**; therefore, holes are not provided through the base material **2140** for the detector and emitters.

As explained above in general, one of the advantages of the optical cavity **2150** is that fleshy tissue can enter the cavity without significant perturbation in the area of the field of view of the detector. Even if no hole is cut in the base material, if the base material chosen is very flexible, perturbation of the fleshy tissue in the field of view of the detector **2100** will be minimal due to the optical cavity aperture **2158**, with the added benefit of not creating optical geometrical changes if the base material is not removed over the cavity.

A cover **2160** is placed over the optical cavity **2150** as represented in an activity block **3035**, and shown in FIG. 36. The cover is advantageously a vacuum formed, cup-shaped cover. In the present embodiment, the cover is made from polypropylene. In one advantageous embodiment, the cover is opaque to ambient light. The opaque characteristic can be obtained from a coating or from the material of construction. The cover has flange **2162** which serves as a bonding surface with the base material. Advantageously, PSA on the base material provides the appropriate bond between the flange **2162** of the cover and the base material **2140**.

A face stock **2170**, advantageously constructed from a non-woven, flexible material, is placed over the base material **2140**. In an alternative embodiment, a woven, flexible material is acceptable. In the present embodiment, the face stock **2170** comprises 3M part no. 9908. The face stock preferably has an aperture **2171** to allow the cup portion of the cover **2160** to protrude through the face stock. The face stock **2170** covers the flange portion **2162** (shown in dotted lines in FIG. **37**) of the cover **2160**. This assists in holding the cover **2160** firmly in place. Because the base material has PSA on the side to which the face stock is applied, pressure applied to the face stock bonds the face stock with the base material. In the present embodiment, the face stock **2170** also has PSA on one side (side down in FIG. **37**). The face stock is cut such that the connector tab **2010** and the connector traces **2052** of the flex circuit remain exposed. This manufacturing step is represented in an activity block **3040** and is depicted in FIG. **37**.

In addition, to a cutout **2172** in the face stock **2170** and the base material **2140** provide a slot on each side of the connector tab **2010** and the connection traces end of the flex circuit assembly **2051**. These slots are adapted to receive walls of the connector receptacle **2060** (see FIG. **29B**) for stability.

Finally, the optical probe is die-cut to a final shape as depicted in FIG. **38** and represented in an activity block **3045** (FIG. **30**). The manufacturing method is complete, as represented within an activity block **3055**. Removal of the release liner **2003** on the base material **2140** allows for placement on the digit of a pediatric or adult patient as depicted in FIGS. **29A–29B**.

Another embodiment of a low noise optical probe **2200** is depicted in FIG. **40A**. This embodiment is advantageous for use with neonates, as will be further described below. FIG. **41** is a flow chart which details the general method used for manufacturing a neonatal disposable optical probe **2200** in accordance with this second embodiment of the present invention.

As with the previous embodiment, the neonatal probe **2200** is constructed of several layers. A first tape layer **2210** is laid out as represented in an activity block **4010**, and depicted in FIG. **42**. Advantageously, the first tape layer **2210** is constructed from release liner material. The first tape layer **2210** has adhesive portions on one side for adhesion to the tissue material under test, as will be further understood below. In the present embodiment, the release liner is a conventional paper type release liner for the medical industry.

In a preferred embodiment, the first tape layer **2210** has a first portion of adhesive **2212** and a second portion of adhesive **2213** which provide adhesion in the area of the detector and emitters. In the present embodiment, the adhesive portions **2212**, **2213** are made from 3M part number MED 3044, which is a medical quality two-sided PSA material. This material is transparent to the wavelength of the emitter in the probe **2200**, and therefore, a thru hole is not required. However, a thru hole, such as the thru hole **2211** could be provided in one embodiment.

A second tape layer **2220** is placed over the first tape layer as represented in an activity block **4020**, and depicted in FIG. **43**. The second tape layer **2220** includes an emitter aperture (thru hole) **2222** and a detector aperture **2224**, which provide windows for the detector and emitters. In the present embodiment, the second tape layer is made from a non-woven face stock material, with PSA on one side. In the present embodiment, the second tape layer **2220** comprises part number **9908**, made by 3M. In the illustration of FIG. **43**, the adhesive side is up.

An optical cavity **2240** is placed onto the second tape as shown in FIG. **43** and represented in an activity block **4030**. One preferred embodiment of the optical cavity **2240** is illustrated in additional detail in FIGS. **44A–C**. FIG. **44A** depicts a perspective view of the optical cavity **2240**. FIG. **44B** depicts a bottom plan view of the optical cavity **2240**, and FIG. **44C** depicts a side cross-sectional view through **44C–44C** of FIG. **44A**. As with the embodiment of FIGS. **39A–C**, the optical cavity **2240** is made from styrene or ABS or the like in one embodiment. In one preferred embodiment, the optical cavity **2140** is coated with an optical coating that is opaque to ambient light. This can be on the inside walls of the optical cavity or over the exterior walls of the optical cavity, or the entire optical cavity can be coated. The opaque coating advantageously prevents or minimizes the transmission of ambient light from the surrounding environment which could be incident on the detector if the optical cavity is not opaque to ambient light. As an alternative to an opaque coating, the optical cavity can be made from a material that is opaque to ambient light.

Advantageously, the optical cavity **2240** has a wedge-shaped ramp **2242** as part of a rectangular receptacle **2244**. The rectangular receptacle **2244** is adapted to receive the detector end of a flex circuit, as further explained below. The wedge-shaped ramp **2242** of the optical cavity **2240** provides a ramp for a smooth transition for the flex circuit between the surface of the second tape layer **2220** to a rectangular receptacle table **2246**.

Further illustrated in FIG. **44A** are two side walls **2248** that extend along the side border of the rectangular receptacle **2244** and an arcuate end wall **2250** that extends between the two side walls **2248**. These walls hold the flex circuit in position such that the detector aligns properly with an aperture **2252** in the optical cavity **2240**. Preferably, the flex circuit fits snugly between the side walls **2248**.

In a preferred embodiment, the aperture **2252** has the configuration of the cavities describe above in general (e.g., cone-shaped, cylindrical in shape, conical in shape, etc.)

A flex circuit **2254** is depicted in detail in FIGS. **45A–B**. As depicted in FIG. **45A**, a flex circuit is formed on a flexible substrate **2255**. In the present embodiment, the flexible substrate advantageously comprises 3 Mil polyester (e.g., MYLAR™) with copper coating on 1 side. In the present embodiment, the copper coating is ½ OZ. copper coating. The circuit pattern is etched such that the circuit traces of copper remain on a signal side of the flex circuit **2254** after etching. From this etching standpoint, the flex circuit **2254** is made in the same fashion as the flex circuit assembly **2051** of the adult probe **2002**.

Once the circuit is etched, it is placed on a bottom shielding layer **2256**, depicted in FIG. **45A**. In one embodiment, the shielding comprises a metallized MYLAR™ shield, with one side metallized. The metallic side is positioned against the back side of the flex circuit substrate **2255**. Conductive PSA bonds the flex circuit substrate **2252** with the bottom shielding layer **2256** through connection **2251** connects the bottom shield metallization to ground from the ground trace **2253**. The bottom shielding layer **2256** has an emitter aperture corresponding to the emitter aperture **2252** in the optical cavity **2240** and the emitter aperture **2257** in the flex circuit **2254**. The bottom shielding layer **2256** extends (extension labeled **2258** in FIG. **45A**) beyond the detector end of the flex circuit **2250**. In an alternative embodiment, the back side of the flex circuit **2254** has a metal coating, such as copper. This provides appropriate shielding. Thus, the first shielding layer could be eliminated in an alternative embodiment.

A detector shield **2260**, such as the detector shield **2110** of the probe **2002** (FIG. **32**), is bonded to the signal trace side of flex circuit **2254**, as depicted in FIG. **45B**. Next, a detector **2272** is placed using low temperature solder, as with the previous embodiment, such that the detector field of view is through the grating **2261** in the detector shield **2260**. The detector shield **2260** is then folded over the detector in order to provide a Faraday shield, as with the previous embodiment.

The extension **2258** of the first shielding layer **2256** is then folded over and conductive PSA is used to bond the metallized side of the bottom shielding layer **2256** to the detector shield **2260**. This connects the detector shield to ground. The emitter **2270** is also placed using the low temperature solder.

In one advantageous embodiment, a resistor **2262** is also placed either in parallel with the emitter or is provided with its own connection trace. The embodiment of FIG. **45A** depicts an embodiment with a separate connection trace **2263** for the resistor **2262**.

A top shielding layer **2268** is placed to shield the signal side of the flex circuit, as depicted in FIG. **45C**. In the present embodiment, this second shielding layer **2268** comprises the same material as the first shielding layer **2256**. The second shielding layer **2268** is bonded to the detector shield **2260** using conductive PSA which couples the second shielding layer **2268** to ground. The second shielding layer **2268** covers the entire flex circuit and is bonded to the flex circuit **2254** using PSA.

The flex circuit assembly **2254** of FIG. **45** used in the neonatal probe **2200** is constructed with a unique V-configuration. The emitter **2270** is at the tip of one branch, a detector **2272** is at the tip of the other branch, and a connector tab **2274** (substantially the same as the connector tab **2010**) is attached at the base of the "V."

The optical cavity **2240** is substantially the same as the optical cavity **2150**. In addition, the detector **2272** and the emitter **2270** are substantially the same as the detector **2120** and the emitter **2021**.

Once the shielded flex circuit assembly **2254** is completed, the completed flex circuit assembly is placed onto the second tape **2220**, as depicted in FIG. **46**. The flex circuit **2250** is positioned such that the emitter **2270** and the detector **2272** have a field of view through the respective apertures **2222**, **2224** in the second tape layer **2220**.

Once the flex circuit assembly is placed, third and fourth layers of tape **2280**, **2290** are placed over the flex circuit assembly **2254** as represented within an activity block **4040** and depicted in FIG. **47**. The third and fourth tape layers **2280**, **2290** are made from the non-woven face material such as that made by 3M as part number 9908. The third and fourth tape layers **2280**, **2290** have PSA on the side which bonds to the assembly made up of the first tape layer **2210**, the second tape layer **2220** and the flex circuit assembly **2254**. As depicted in FIG. **47**, the fourth tape layer **2290** is configured to allow connection traces **2292** of the flex circuit to remain exposed.

Finally, the neonatal disposable probe **2200** is die-cut to a final shape as represented within activity block **4050** and depicted in FIG. **48**. The manufacturing method is then complete as represented within an activity block **4060**.

FIGS. **40A** and **40B** illustrate the neonatal probe being attached to a baby's foot (shown in phantom). The finger is placed on the detector branch of the probe **2200**. The emitter branch is then positioned so that the emitter **2270** is directly above the detector **2272** with the foot in-between. An adhesive strap **2400** (which was die-cut from the first tape

layer **2210** and the third tape layer **2280**) is then wrapped around the foot to secure the relative position of the emitter **2270** and detector **2272**. It should be appreciated that the adhesive material selected to coat the adhesive strap should not be so strong as to tear or bruise the skin of a newborn baby. The connector **2060** subsequently establishes electrical connection between the probe **2200** and digital signal processing circuitry via the connector tab **2294**.

The unique V-configuration of the neonatal probe embodiment of the present invention (e.g., as displayed in FIG. **49**) is particularly advantageous for use in applications where the optical probe is used on neonates. The V-configuration allows the probe to be used on many different sizes of monitoring sites (e.g., feet, hands, etc.) for a neonate. With conventional wrap-around embodiments, the spacing of the detector and emitter is fixed, thus making the use of the probe for different sized monitoring sites more difficult. In addition, the V-shaped design allows for the use of the probe on various body parts. For instance, the probe **2200** could be attached to the nose or ear of the neonate. The probe **2200** could also be used as a reflectance probe with the probe attached to the forehead of the neonate, or other relatively flat skin surface. Thus, the V-design provides for the adaptation of the probe for many different places on the neonate body.

An alternative embodiment of the V-configuration is depicted in FIG. **49**. In the embodiment depicted in FIG. **49**, the adhesive extension **2400** (FIG. **48**) is not provided. In this embodiment, the probe can be used with conventional medical tape or the like, or can be provided such that the adhesive **2212**, **2213** (FIG. **42**) in the area of the detector and emitter hold the probe in place. Alternatively, a soft, spongy, hospital wrap (e.g., a POSEY wrap) **2498** can be configured to firmly hold the probe to a digit as depicted in FIG. **50**.

Another embodiment of the method of making the neonatal probe is illustrated in FIGS. **51–55**. An X-ray type view of the alternative embodiment **2500** is depicted in FIG. **51**. As illustrated in FIG. **51**, the probe **2500** has a detector **2502**, an emitter **2504**, a flex circuit **2506**, a low noise cavity **2508** and a cover **2510** for the optical cavity **2508**, top and base tapes **2512**, **2514**, an identification resistor **2516**, thru connections **2518**, **2520**, and a connection tab **2522**. This embodiment of the probe is depicted without the tape extension, such as the extension **2400** (FIG. **48**), but could include a tape extension in one embodiment. The overall configuration of the finished probe **2500** is nearly identical to the probe of FIG. **49**. However, the shielding is different, the optical cavity has a cover, and the probe **2500** is constructed using two tapes instead of four. The construction of this embodiment of the probe **2500** is similar to the adult probe from the standpoint of the tape-up.

FIGS. **52A** and **52B** illustrate a base tape **2530** and the top tape **2540**. The base tape **2530** has a detector component window **2532** and an emitter component window **2534**. Advantageously, the component windows form apertures through the base tape **2530**. Therefore, in one preferred embodiment, clear (i.e., transparent to the emitter wavelengths) window material portions **2536**, **2538** are provided as a cover to the component windows **2532**, **2534**. In one embodiment, the clear window material is made from the 3M, Med **3044** described above. The MED **3044** is attached to the back-side (with reference to the illustration in FIG. **52A**) of the base tape **2530** in order to provide adhesion to the tissue material under test. Alternatively, the window material **2536**, **2538** is non-adhesive, and can be mounted to the up-side (with reference to the illustration in FIG. **53A**) of the base tape.

In the present embodiment, the base tape **2530** is formed of a laminate formed of a first layer of non-woven face stock, such as that made by 3M as part number 9908, and a second film, such as single-sided PSA film sold by Coating Sciences, Inc. as P-341. The face stock has PSA on one side. In the illustration of FIG. **52A**, the PSA for the face stock is up. The second film of material is laminated to the first layer of non-woven face stock. In the present embodiment, the second layer also has one side with PSA. In the illustration of FIG. **52A**, the PSA side of the second film is up. Accordingly, the side of the base tape **2530** depicted in FIG. **52A** has PSA from the second film. In the present embodiment, the second film comprises a 1 Mil layer of Coating Sciences part number P-341. The use of two layers provides improved isolation to the flex circuit.

FIG. **52B** illustrates the top tape **2540**, which is also formed of the two layers of material as with the base tape. In the illustration of FIG. **52B**, the adhesive side of the top tape is down and the face stock side of the top tape **2540** is up. For the present embodiment, the top tape has a cutout **2542** for the cover **2510** to the optical cavity **2508**. The optical cavity **2508** has the same configuration as the optical cavity **2240** FIG. **44**.

An appropriate cover **2510** is depicted in detail in FIG. **55A–C**. The cover is cup-shaped to fit snugly about the optical cavity **2508**. FIG. **55A** depicts a top view of the optical cover **2510**. FIG. **55B** depicts a side cross sectional view through B—B in FIG. **55A**. FIG. **55C** depicts an end cross-sectional view through **55C—55C** in Figure **55A**. In the present embodiment, the cover **2510** is vacuum formed from styrene, and is coated with a light absorbing paint, such as black paint to reduce the effects of ambient light.

FIGS. **53A** illustrates the signal side of an appropriate flex circuit **2506** and FIG. **53B** illustrates the back side (i.e., shield side in the this embodiment) of the flex circuit **2506**. As depicted in FIG. **54B**, the signal side of the flex circuit **2506** has signal traces, the identification resistor **2516**, and the two through connections **2518**, **2520**. The flex circuit also has connection pads **2560**, **2562** for the detector **2502** and connection pads **2564**, **2556** for the emitter **2504**. As with the previous embodiments, the signal side of the flex circuit **2506** has traces formed by etching away the metallic coating. The flex circuit is formed of the same materials as described for the previous embodiments of flex circuits.

FIG. **53B** depicts the shield side of the flex circuit **2506**. In this embodiment, the flex circuit **2506** is a two-sided circuit, with the shield side coated, substantially in its entirety, with metal, such as copper. By providing a metallic shield side, a separate shielding layer is not needed for the back of the flex circuit **2506**. The through connections **2518**, **2520** connect the shield side metal to the ground trace **2510**.

FIG. **54** illustrates a top shield **2570** for the flex circuit **2506**. In the present embodiment, the top shield **2570** is formed from a metallized MYLAR™, as with the shields for the previous embodiment. Prior to application of the top shield **2570**, the detector **2502** and the emitter **2504** are soldered to the connection pads **2560**, **2562**, **2564**, **2566**. Then one end of a detector shield **2572**, having the same configuration as the detector shield **2260** (FIG. **45B**) is connected to the shield side of the flex circuit **2506**. In one embodiment, the connection is made with solder or conductive PSA.

The top shield **2570** is applied to the signal side of the flex circuit **2506** (with the non-metallized side against the signal side of the flex circuit) with PSA. The detector branch **2574** of the top shield **2570** is longer than a detector branch **2563** of the flex circuit **2506**. Thus, the detector branch **2574** is

positioned such that the end of the detector branch **2574** covers the detector **2502**. Conductive PSA **2576** is applied to the end of the metallized side of the detector branch **2574**. The detector shield **2272** is folded over the top shield **2570** and connection is made via the conductive PSA **2576**. In this manner, top shield **2570** is coupled to ground via the connection detector shield **2572** which is connected to ground via its connection to the shield side of the flex circuit **2506**.

Once the flex circuit assembly **2506** is completed, it is placed on the base tape **2530**, with the detector **2502** and the emitter **2504** aligned with the detector window **2532** and the emitter window **2534**, respectively. The detector **2502** also is positioned in the rectangular receptacle table of the optical cavity **2508**. The optical cavity cover **2510** is then placed over the optical cavity **2508**. Finally, the top tape **2540** is placed over the entire assembly with the cut-out for the optical cavity cover aligned with the cover **2510**. The entire assembly is pressed to set the PSA adhesive on the base tape **2530** and the top tape **2540**. The assembly is then die cut to the shape depicted in FIG. **51**.

This embodiment of the probe **2506** has the advantage of fewer assembly steps, and therefore reduced cost. The use of the cover **2510** also allows for further isolation of the detector from ambient light. As discussed above, the cover, as well as the optical cavity, can be made opaque to ambient light, either through coatings or pigmented or otherwise impregnated materials.

In accordance with another embodiment of the invention, a reusable, low-noise, optical probe **2300** is constructed as depicted in FIG. **56**. The probe **2300** comprises a padded, clip-on bracket **2305** which comfortably secures the probe **2300** onto a patient's fingertip (not shown in FIG. **56**). The probe further includes a detector **2310** (shown in phantom) which detects optical radiation emitted by an emitter **2320** (also shown in phantom). An aperture **2330**, which is substantially similar to the aperture **1020**, is formed in the probe **2300** to provide the advantages enumerated above with respect to the aperture **1020**. Power to activate the LED **2320**, is provided via a connector cable **2340**. The cable **2340** also provides a return path for signals output by the detector **2310**. Advantageously, the reusable probe **2300** can have a connector with a similar configuration as the connector for the disposable probes, such that the instrument connector can be the same for use with disposable and reusable probes.

The probe of the present invention may be employed in any circumstance where a measurement of transmitted or reflected energy is to be made, including but not limited to measurements taken on a finger, an earlobe, a lip, or a forehead. Thus, there are numerous other embodiments including, but not limited to, changes in the shape of the probe, changes in the materials out of which the probe is made including rigid and resilient materials, and changes in the shape, dimensions, and location of the chamber. Moreover, the chamber(s) may be coated, in whole or in part, with reflective material to help direct energy onto the detector. Furthermore, the probe of the present invention may be employed in measurements of other types of energy. Depending upon the type of energy which is most advantageously utilized in a measurement, the type of transmitter or receiver of energy may be changed. The invention may be embodied in other specific forms without departing from its spirit or essential characteristics. The described embodiments are to be considered in all respects only as illustrative and not restrictive. The scope of the invention is, therefore, indicated by the appended claims rather than by the fore-

going description. All changes which come within the meaning and range of equivalency of the claims are to be embraced within their scope.

What is claimed is:

1. disposable optical probe comprising:
 - a disposable adhesive base material;
 - a disposable face material;
 - a circuit assembly, at least a portion of which is fixedly attached above said base material and below said face material, said circuit assembly including an emitter which transmits optical radiation into a medium and a detector receives said optical radiation attenuated by said medium, wherein said base material is adapted to removably attach said circuit assembly to a medium; and
 - a shield, at least a portion of which is positioned above said detector, wherein said shield reduces degradation of said optical radiation attenuated by said medium caused by ambient light.
2. The disposable optical probe according to claim 1, wherein said shield reduces degradation of said optical radiation attenuated by said medium caused by electromagnetic interference.
3. The disposable optical probe according to claim 1, wherein said shield comprises material substantially opaque to ambient light.
4. The disposable optical probe according to claim 1, wherein said shield includes an opaque tape.
5. The disposable optical probe according to claim 1, wherein said shield includes an opaque cover.
6. The disposable optical probe according to claim 1, wherein said shield comprises a metallic shield.
7. The disposable optical probe according to claim 1, wherein said medium comprises tissue of one of an adult patient, a pediatric patient, an infant patient, and a neonatal patient.
8. The disposable optical probe according to claim 7, wherein the tissue comprises one of a nose, a forehead, a digit, a heel, an foot, and an ear.
9. disposable optical probe comprising:
 - an disposable adhesive base material;
 - a disposable face material;
 - a circuit assembly, at least a portion of which is fixedly attached above said base material and below said face material, said circuit assembly including an emitter which transmits optical radiation into a medium and a detector receives said optical radiation attenuated by said medium, wherein said base material is adapted to removably attach said circuit assembly to a medium; and
 - a shield, at least a portion of which is positioned above said detector
- wherein said shield includes a flange portion and said face material secures at least said flange portion.
10. A disposable optical probe comprising:
 - an disposable adhesive base material;
 - a disposable face material;
 - a circuit assembly, at least a portion of which is fixedly attached above said base material and below said face material, said circuit assembly including an emitter which transmits optical radiation into a medium and a detector receives said optical radiation attenuated by said medium, wherein said base material is adapted to removably attach said circuit assembly to a medium; and

a shield, at least a portion of which is positioned above said detector

wherein said base material is transparent.

11. A method of shielding a detector of a disposable optical probe from ambient light, the method comprising:
 - providing a disposable detector configured to detect attenuated optical radiation;
 - providing disposable light blocking material proximate to said detector to limit degradation of said attenuated optical radiation, wherein said degradation is caused by noise; and
 - providing a disposable optical probe by fixedly attaching said detector, said light blocking material, and an emitter between a disposable adhesive first tape layer and a disposable second tape layer, wherein said emitter is configured to transmit optical radiation into a medium and said detector is adapted to receive said attenuated optical radiation from said medium when said first tape layer removably attaches the disposable optical probe to the medium.
12. The method according to claim 11, wherein the providing the disposable light blocking material limits degradation caused by noise.
13. The method according to claim 12, wherein the noise comprises ambient light.
14. The method according to claim 12, wherein the noise comprises electromagnetic interference.
15. The method according to claim 11, wherein the providing the disposable light blocking material includes providing an opaque cover.
16. The method according to claim 11, wherein the providing the disposable light blocking material includes providing a metallic material.
17. The method according to claim 11, wherein said medium comprises tissue of one of an adult patient, a pediatric patient, an infant patient, and a neonatal patient.
18. The method according to claim 17, wherein the tissue comprises one of a nose, a forehead, a digit, a heel, an foot, and an ear.
19. A disposable optical probe comprising:
 - a disposable electronic circuit comprising at least one emitter and a detector;
 - a disposable noise blocking layer capable of blocking noise comprising ambient light; and
 - a disposable flexible attachment mechanism adhesively housing said electronic circuit proximate to said noise blocking layer so as to materially reduce an effect of noise on said detector, wherein said attachment mechanism is configured to removably attach said electronic circuit to a measurement site.
20. The disposable optical probe according to claim 19, wherein the noise blocking layer comprises a cover.
21. The disposable optical probe according to claim 20, wherein the cover is opaque.
22. The disposable optical probe according to claim 21, wherein the cover is metallic and the noise further comprises electromagnetic interference.
23. The disposable optical probe according to claim 19, further comprising a face stock layer including a non-woven, flexible face stock disposed over at least a portion of said noise blocking layer so as to hold said noise blocking layer in lace with respect to said detector.
24. The disposable optical probe according to claim 19, wherein said measurement site comprises tissue of one of an adult patient, a pediatric patient, an infant patient, and a neonatal patient.

25. The disposable optical probe according to claim 24, wherein the tissue comprises one of a nose, a forehead, a digit, a heel, an foot, and an ear.

26. A disposable optical probe comprising:

an adhesive base material;

a circuit assembly having an emitter and a detector, said assembly fixedly attached to said base material, said base material adapted to removably attach said circuit assembly to a medium so that said emitter transmits optical radiation into said medium and said detector receives said optical radiation attenuated by said medium; and

a cover being opaque to ambient light, said cover placed over said detector and attached to said base material so as to shield said detector from ambient light.

27. The disposable optical probe according to claim 26, further comprising a face stock adapted to assist holding said cover in place.

28. The disposable optical probe according to claim 27, wherein said cover has a flange portion and said face stock covers said flange portion.

29. The disposable optical probe according to claim 26, wherein said cover is an opaque tape.

30. A disposable optical probe comprising:

an adhesive base material;

a circuit assembly having an emitter and a detector, said assembly fixedly attached to said base material, said base material adapted to removably attach said circuit assembly to a medium so that said emitter transmits optical radiation into said medium and said detector receives said optical radiation attenuated by said medium; and

a cover being opaque to ambient light, said cover placed over said detector and attached to said base material so as to shield said detector from ambient light

wherein said base material is transparent to an emitter wavelength.

31. A disposable optical probe method comprising the steps of:

fixedly attaching a detector and an emitter to an adhesive base layer;

removably attaching said adhesive base layer to a medium so as to transmit optical radiation from said emitter into said medium and to receive at said detector a corresponding attenuated optical radiation from said medium;

generating a signal from said detector in response to said attenuated optical radiation; and

shielding said detector with a cover that is opaque to ambient light placed over said detector so as to limit degradation of said signal due to ambient light.

32. The disposable optical probe method according to claim 31, comprising the further step of placing a face stock over at least a portion of said cover so as to assist holding said cover in place.

33. A disposable optical probe comprising:

an adhesive first layer;

a cover adapted to be opaque to ambient light;

a circuit assembly having a detector and an emitter disposed on a flexible substrate, said circuit assembly fixedly attached between said cover and said first layer; said first layer configured to removably affix said circuit assembly to a medium so that said emitter and said detector measure a characteristic of said medium; and

said cover placed over said detector so as to shield said detector from ambient light.

34. A disposable optical probe comprising:

an adhesive first layer;

a cover adapted to be opaque to ambient light;

a circuit assembly having a detector and an emitter disposed on a flexible substrate, said circuit assembly fixedly attached between said cover and said first layer; said first layer configured to removably affix said circuit assembly to a medium so that said emitter and said detector measure a characteristic of said medium, and said cover placed over said detector so as to shield said detector from ambient light; and

an adhesive second layer, said circuit assembly and said cover disposed between said first layer and said second layer.

35. The disposable optical probe according to claim 34, wherein said second layer covers a flange portion of said cover so as to assist in holding said cover in place.

36. A disposable optical probe comprising:

an adhesive first layer;

a cover adapted to be opaque to ambient light;

a circuit assembly having a detector and an emitter disposed on a flexible substrate, said circuit assembly fixedly attached between said cover and said first layer; said first layer configured to removably affix said circuit assembly to a medium so that said emitter and said detector measure a characteristic of said medium; and said cover placed over said detector so as to shield said detector from ambient light, and wherein said first layer is transparent to the wavelengths of said emitter.

37. A disposable optical probe comprising:

an adhesive first layer;

a cover adapted to be opaque to ambient light;

a circuit assembly having a detector and an emitter disposed on a flexible substrate, said circuit assembly fixedly attached between said cover and said first layer; said first layer configured to removably affix said circuit assembly to a medium so that said emitter and said detector measure a characteristic of said medium; and said cover placed over said detector so as to shield said detector from ambient light, and wherein said cover is attached to said first layer.

38. A disposable optical probe comprising:

a flexible substrate having a front side and a second side and defining an LED aperture and a detector aperture, said front side supporting an LED and a detector adapted so that, when said substrate is attached to a tissue site, said LED transmits optical radiation through said LED aperture and into said tissue site and said detector receives optical radiation through said detector aperture from said tissue site;

an opaque cover disposed proximate said front side and fitted over said detector so as to limit detector signal degradation caused by ambient light; and

a base layer having a back side and a front side, each of said sides coated with adhesive so that said front side is fixedly attached to said substrate and said back side is adapted to removably attach said substrate to said tissue site, said base layer transparent to the wavelengths of said LED.

39. The disposable optical probe according to claim 38, further comprising a non-woven, flexible face stock disposed over at least a portion of said cover so as to hold said cover in place.

39

40. A disposable optical probe comprising:
 a flexible substrate having a first side and a second side;
 a circuit assembly disposed on said first side;
 a base layer disposed on said second side;
 an opaque cover located proximate said first side and
 distal said second side, said cover disposed over a
 detector portion of said circuit assembly; and
 a face stock placed over at least a portion of said cover so
 that said cover is held in place between said base layer
 and said face stock.
41. A disposable oximeter probe, comprising:
 means for emitting optical radiation;
 means for detecting attenuated optical radiation;

40

means proximate to said means for detecting, for limiting
 degradation of said attenuated optical radiation,
 wherein said degradation is caused by ambient light;
 and
 means for fixedly attaching said means for detecting, said
 means for limiting, and means for emitting, between an
 adhesive first tape layer and a second tape layer,
 wherein said first tape layer is adapted to removably
 attach to a medium so as to transmit the optical radia-
 tion from said means for emitting into said medium and
 to receive at said means for detecting said attenuated
 optical radiation from said medium.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 6,813,511 B2
APPLICATION NO. : 10/260049
DATED : November 2, 2004
INVENTOR(S) : Mohamed Diab et al.

Page 1 of 2

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

At Page 2, Column 2, delete “6,658,277” and insert -- 6,658,276 --, therefore.

At column 3, line 50, after “Advantageously,” delete “a”.

At column 4, line 4, delete “an” and insert -- a --, therefore.

At column 5, line 52 (Approx.), delete “29-29B” and insert -- 29A-29B --, therefore.

At column 6, line 19, after “the” delete “a”.

At column 7, line 13 (Approx.), after “constituent,” delete “X_i” and insert -- X_i --, therefore.

At column 7, line 15 (Approx.), after “and” delete “C_i” and insert -- C_i --, therefore.

At column 7, line 16 (Approx.), after “thickness” delete “X_i” and insert -- X_i --, therefore.

At column 19, line 12, delete “arc” and insert -- are --, therefore.

At column 30, line 8, delete “FIGS.” and insert -- FIG. --, therefore.

At column 30, line 34, delete “a” and insert -- an --, therefore.

At column 33, line 35, after “side in” delete “the”.

At column 35, line 5, in Claim 1, before “disposable” insert -- A --.

At column 35, line 31, in Claim 5, after “includes” delete “a” and insert -- an --, therefore.

At column 35, line 40, in Claim 8, delete “an foot” and insert -- a foot --, therefore.

At column 35, line 41, in Claim 9, before “disposable” insert -- A --.

At column 35, line 42, in Claim 9, delete “an disposable” and insert -- a disposable --, therefore.

At column 35, line 54 (Approx.), in Claim 9, after “detector” insert -- , --.

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 6,813,511 B2
APPLICATION NO. : 10/260049
DATED : November 2, 2004
INVENTOR(S) : Mohamed Diab et al.

Page 2 of 2

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

At column 35, line 58, in Claim 10, delete "an disposable" and insert -- a disposable --, therefore.

At column 36, line 2, in Claim 10, after "detector" insert -- , --.

At column 36, line 31 (Approx.), in Claim 15, after "an" delete "a".

At column 36, line 39, in Claim 18, delete "an foot" and insert -- a foot --, therefore.

At column 36, line 56, in Claim 22, delete "claim 21" and insert -- claim 20 --, therefore.

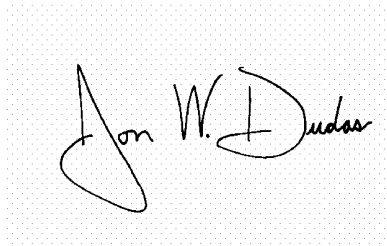
At column 36, line 63, in Claim 23, delete "lace" and insert -- place --, therefore.

At column 37, line 3, in Claim 25, delete "an foot" and insert -- a foot --, therefore.

At column 37, line 36, in Claim 30, after "light" insert -- , --.

Signed and Sealed this

Nineteenth Day of June, 2007

A handwritten signature in black ink on a light gray dotted background. The signature reads "Jon W. Dudas" in a cursive, stylized script. The first name "Jon" is written with a large, sweeping initial 'J'. The last name "Dudas" is written with a large, circular 'D' and a trailing flourish.

JON W. DUDAS

Director of the United States Patent and Trademark Office

专利名称(译)	低噪声光学探头，用于降低环境噪音		
公开(公告)号	US6813511	公开(公告)日	2004-11-02
申请号	US10/260049	申请日	2002-09-27
[标]申请(专利权)人(译)	戴铂MOHAMED Kiani曾AZARBAYJANY ESMAIEL TOBLER戴维r GERHARDT托马斯· MASON EUGENEê MILLS迈克		
申请(专利权)人(译)	戴铂MOHAMED Kiani曾-AZARBAYJANY ESMAIEL TOBLER DAVID R. GERHARDT托马斯J. MASON EUGENE E. MILLS MIKE A.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	DIAB MOHAMED KIANI AZARBAYJANY ESMAIEL TOBLER DAVID R GERHARDT THOMAS J MASON EUGENE E MILLS MIKE A		
发明人	DIAB, MOHAMED KIANI-AZARBAYJANY, ESMAIEL TOBLER, DAVID R. GERHARDT, THOMAS J. MASON, EUGENE E. MILLS, MIKE A.		
IPC分类号	A61B5/00 A61B5/024 H05K1/18 A61B5/022 A61B5/0245 A61B5/145 A61B5/1455 G01N21/17 G01N21/59		
CPC分类号	A61B5/6829 A61B5/6826 A61B5/6838 A61B5/02427 A61B5/14552 H05K1/189 Y10T29/49826 A61B2562/08 A61B2562/12		
优先权	61/898990 2001-07-03 US		
其他公开文献	US20030045785A1		
外部链接	Espacenet USPTO		

摘要(译)

光学探针特别适合于降低在易于压缩的材料（例如手指，脚趾，前额，耳垂或唇部）上进行的测量中的噪声，测量材料的特性。探针的新生儿和成人一次性实施方案包括涂有粘合剂的表面，以将探针牢固地固定在患者身上。此外，探头表面经过特殊构造，可减少环境噪音的影响。

