




US 20020049394A1

(19) **United States**(12) **Patent Application Publication**
Roy et al.(10) **Pub. No.: US 2002/0049394 A1**(43) **Pub. Date: Apr. 25, 2002**(54) **APPARATUS AND METHOD FOR
ASSESSING LOADS ON ADJACENT BONES****Related U.S. Application Data**(63) Non-provisional of provisional application No.
60/228,166, filed on Aug. 25, 2000.(75) Inventors: **Shuvo Roy**, Cleveland, OH (US);
Aaron J. Fleischman, University
Heights, OH (US); **Edward C. Benz**,
Gates Mills, OH (US); **Lisa Ferrara**,
Cleveland Heights, OH (US)**Publication Classification**(51) **Int. Cl.⁷** **A61B 5/103**; **A61F 2/44**(52) **U.S. Cl.** **600/594**; **623/17.11**(57) **ABSTRACT**

An apparatus (10) that utilizes microelectromechanical systems (MEMS) technology to provide an in vivo assessment of loads on adjacent bones (24 and 26) comprises a body (34) for insertion between the adjacent bones. At least one sensor (42) is associated with the body (34). The sensor (42) generates an output signal in response to and indicative of a load being applied to the body (34) through the adjacent bones (24 and 26). A telemetric device (40) is operatively coupled with the sensor (42). The telemetric device (40) is operable to receive the output signal from the sensor (42) and to transmit an EMF signal dependent upon the output signal. According to various aspects of the invention, the sensor comprises a pressure sensor (42), a load cell (320), and/or at least one strain gauge (142).

Correspondence Address:

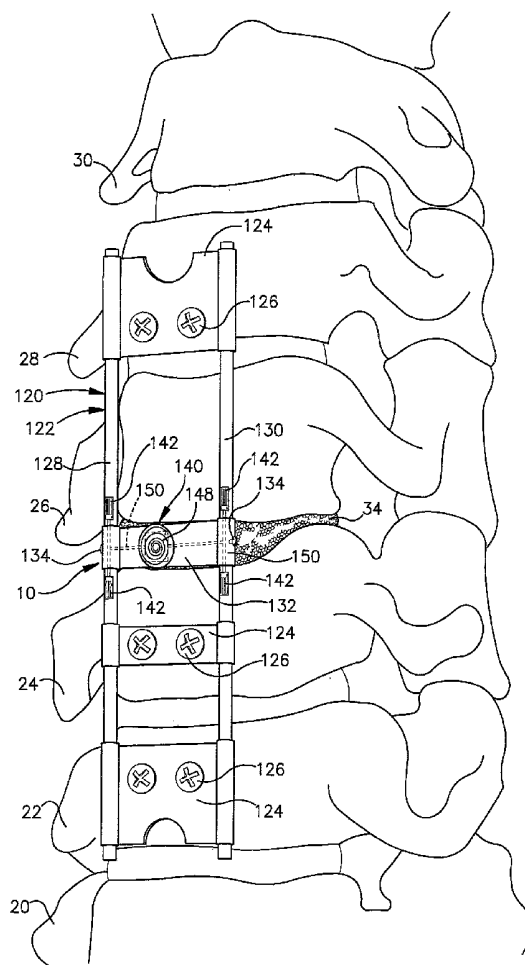**TAROLLI, SUNDHEIM, COVELL,
TUMMINO & SZABO L.L.P.**
1111 LEADER BUILDING
CLEVELAND, OH 44114 (US)(73) Assignee: **The Cleveland Clinic Foundation**(21) Appl. No.: **09/939,331**(22) Filed: **Aug. 24, 2001**

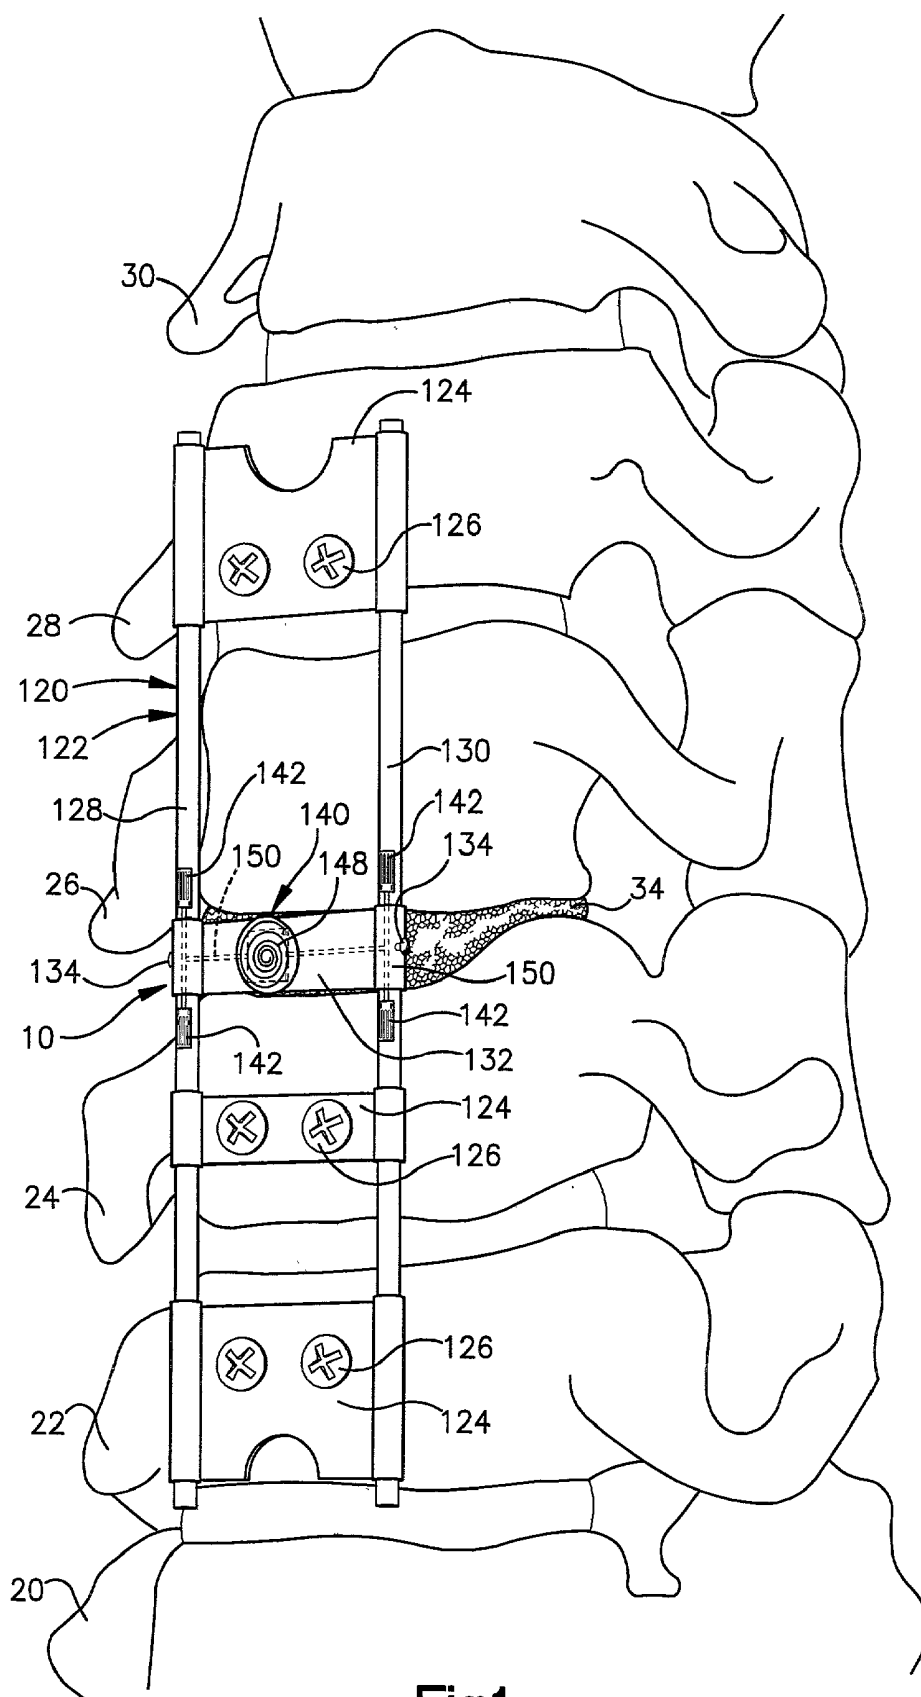
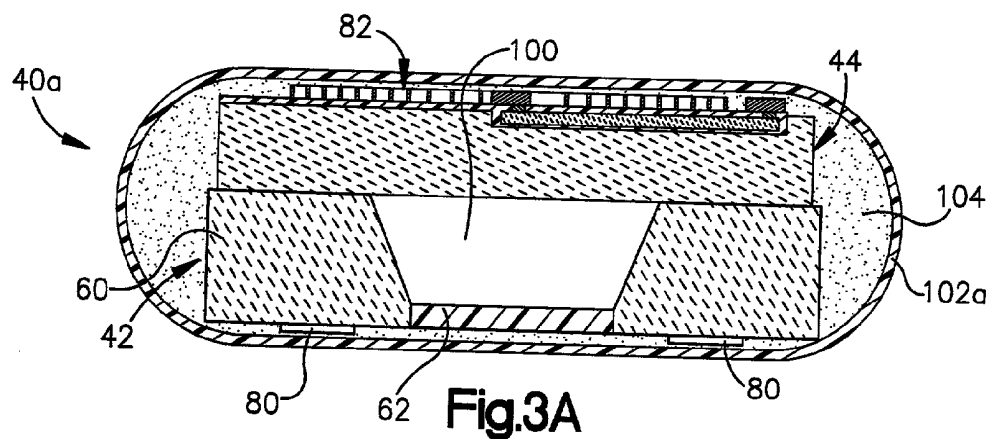
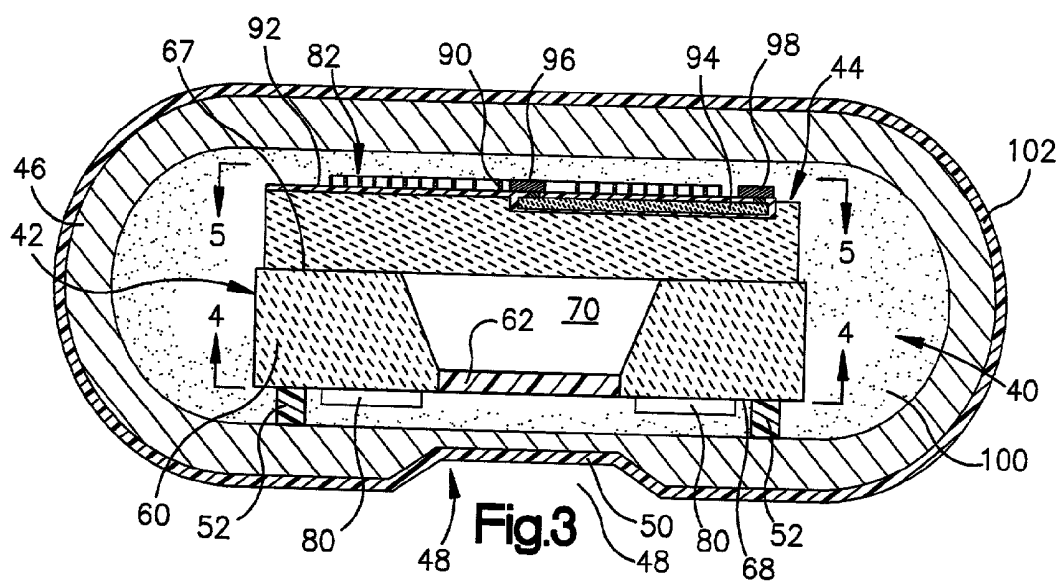
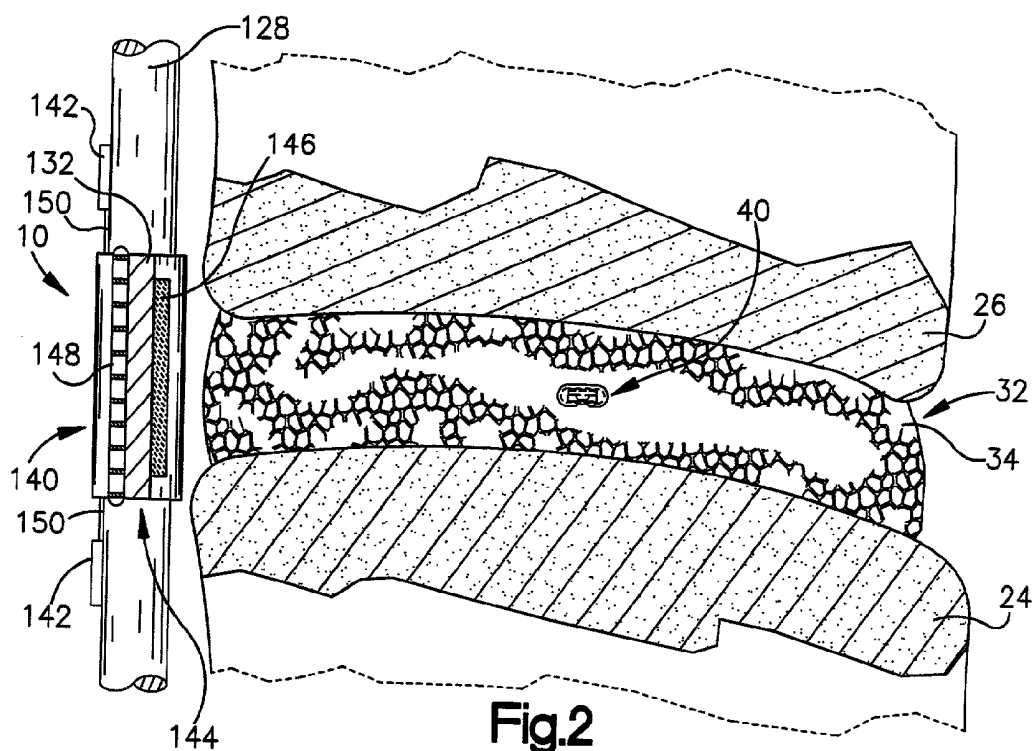
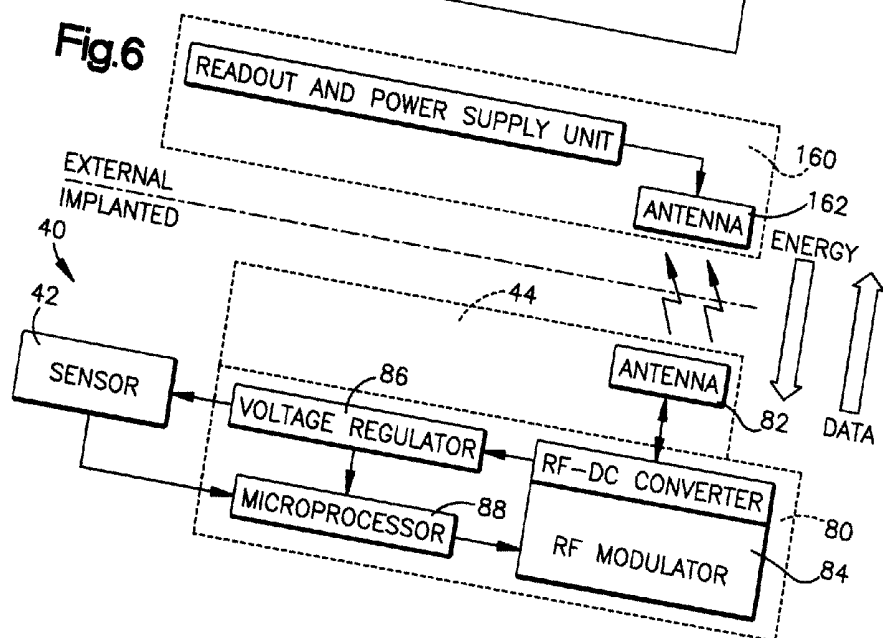
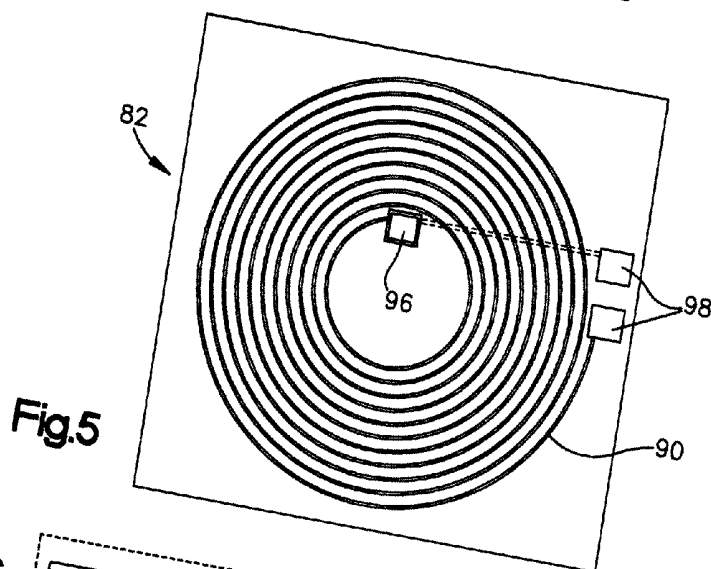
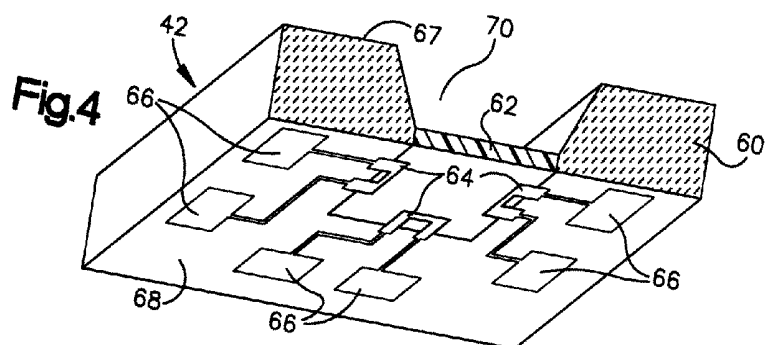
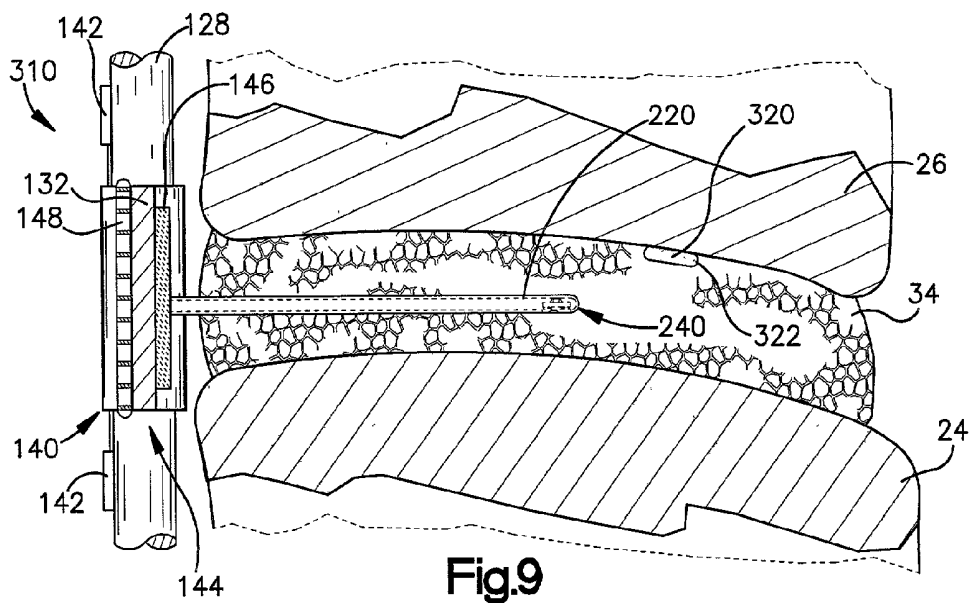
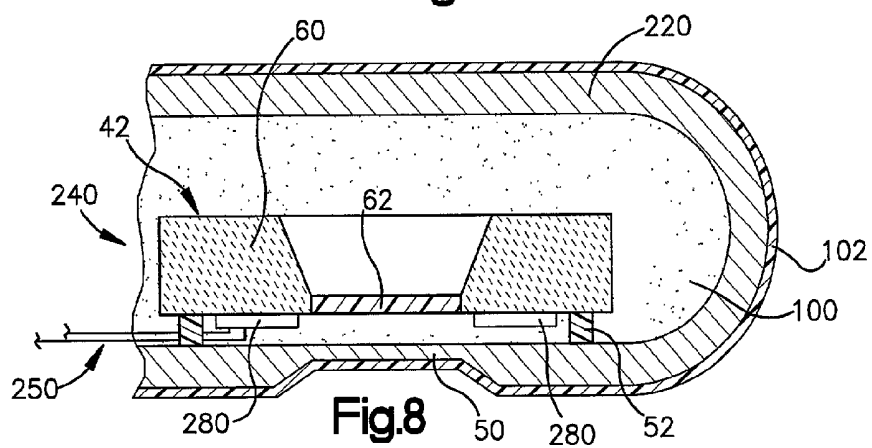
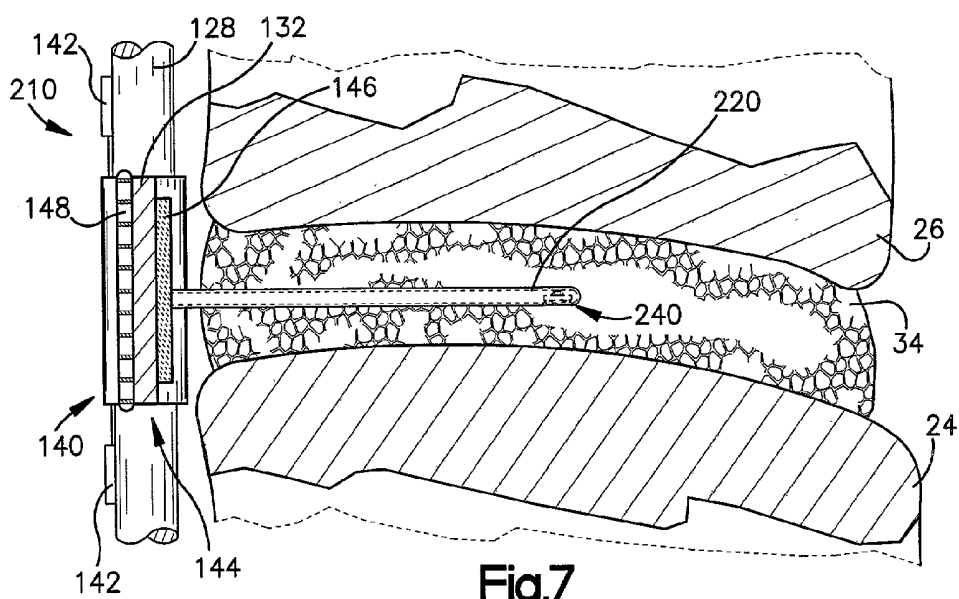
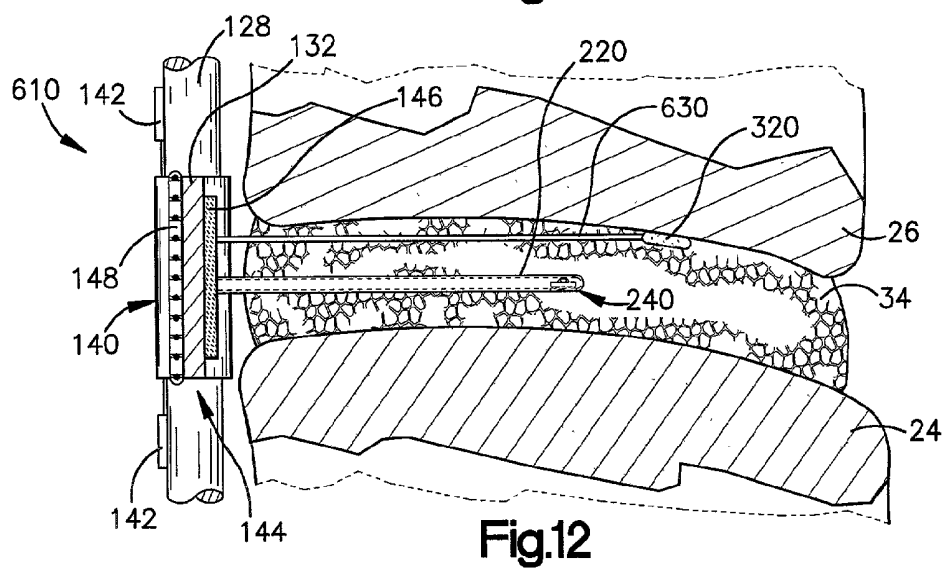
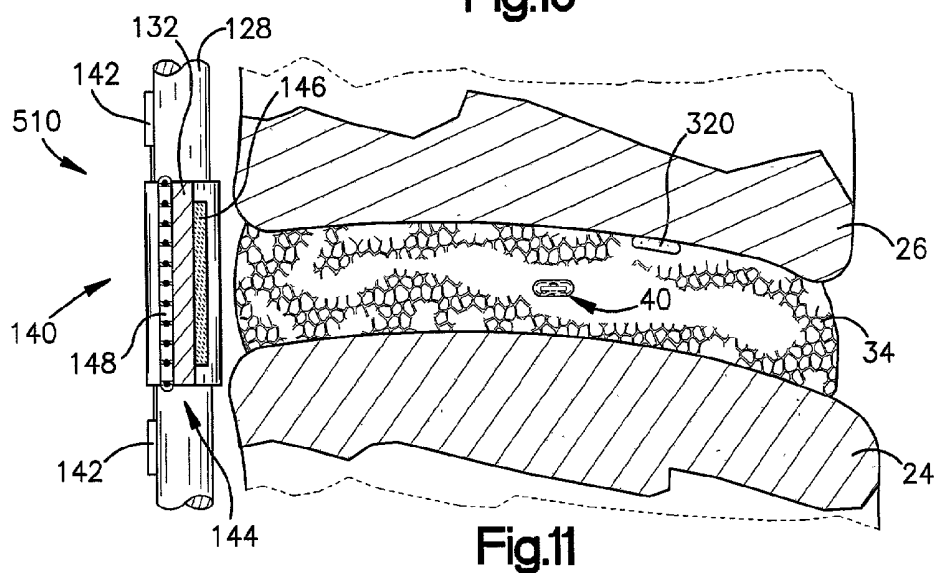
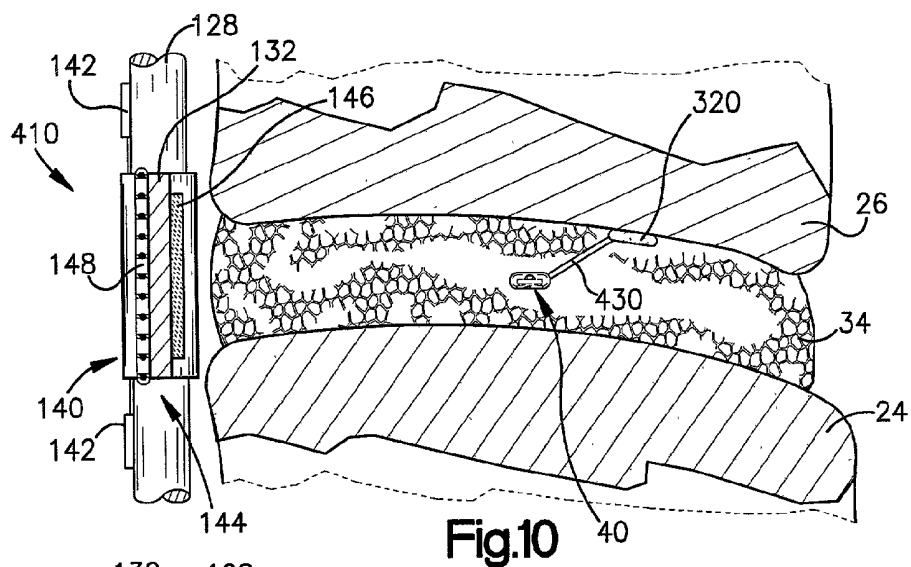




Fig.1









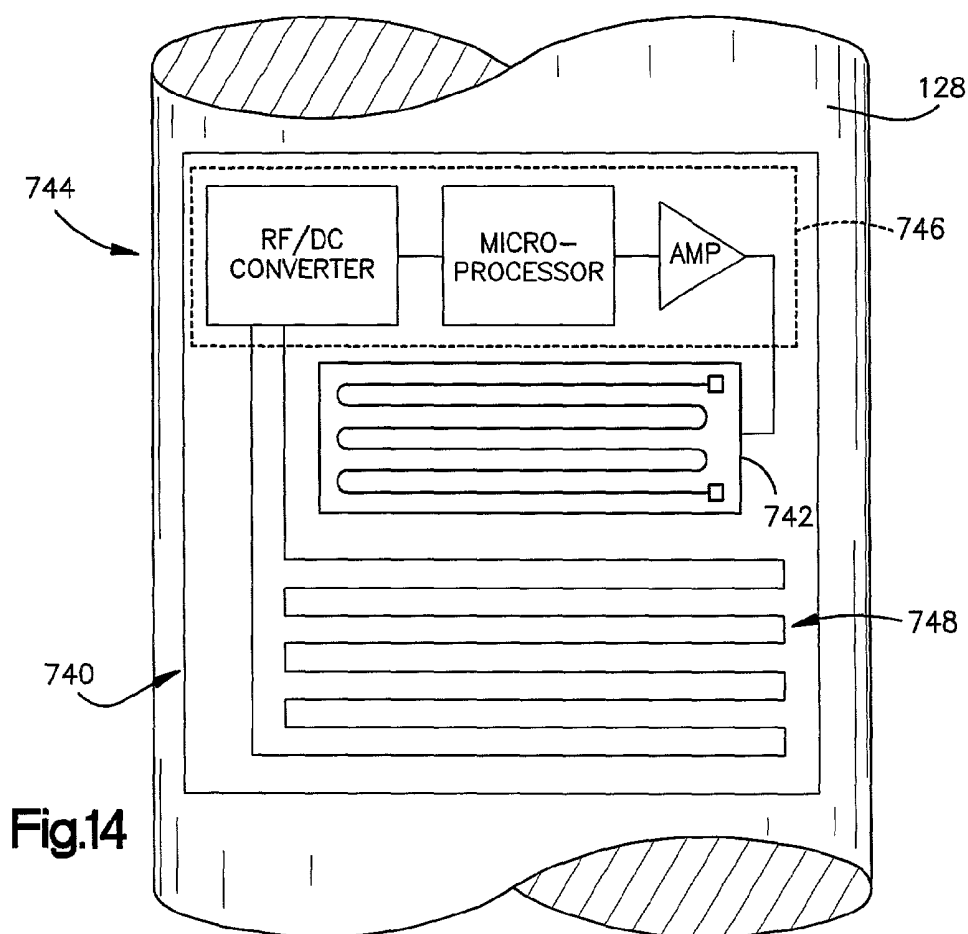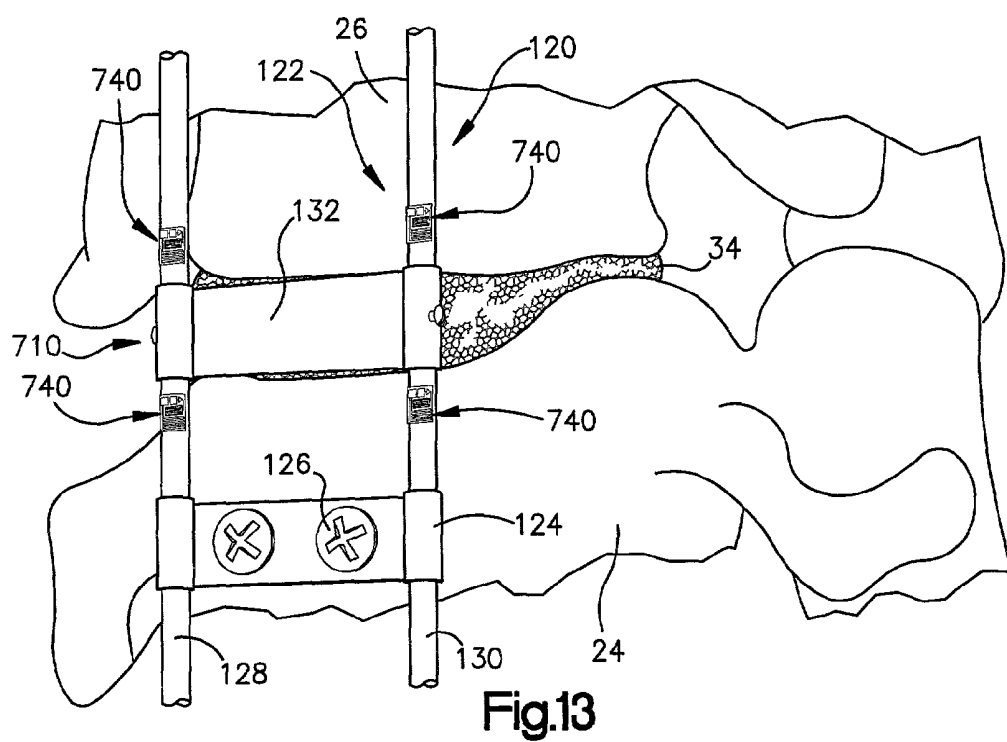

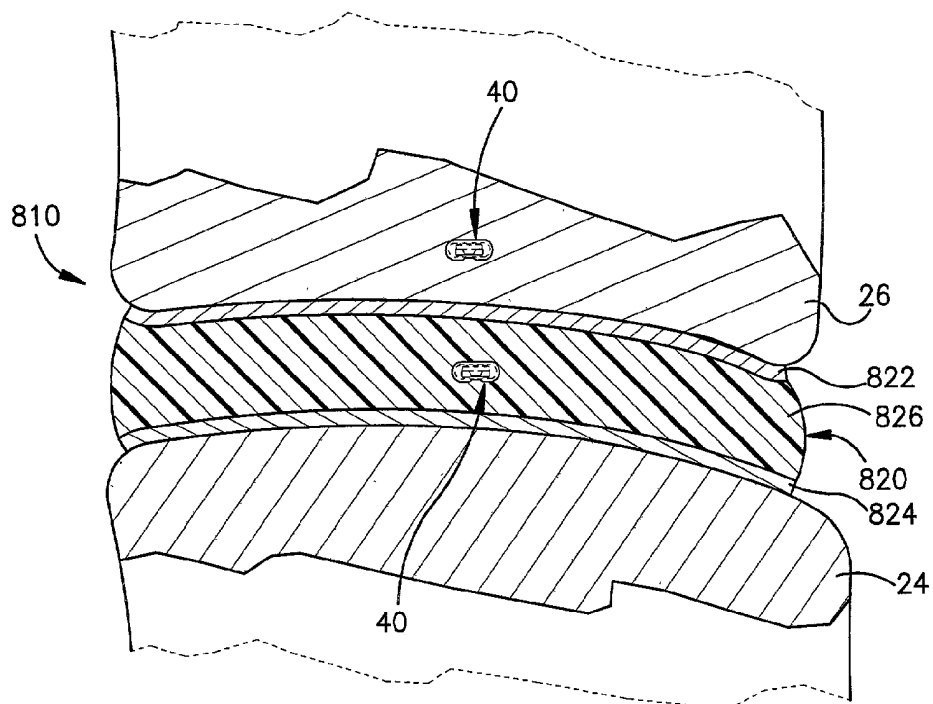


Fig.15



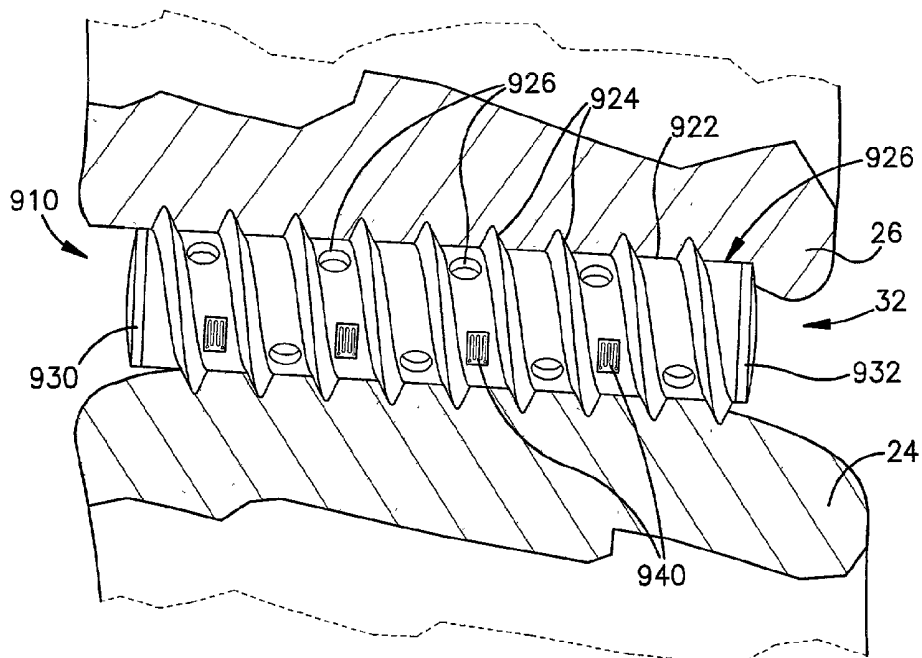


Fig.16

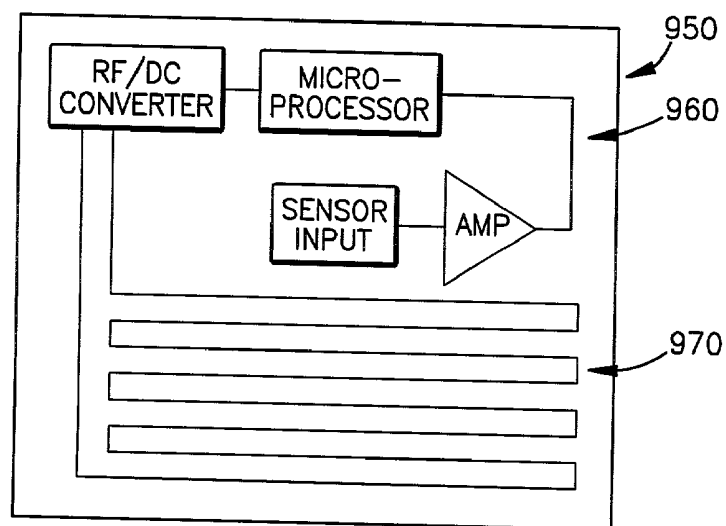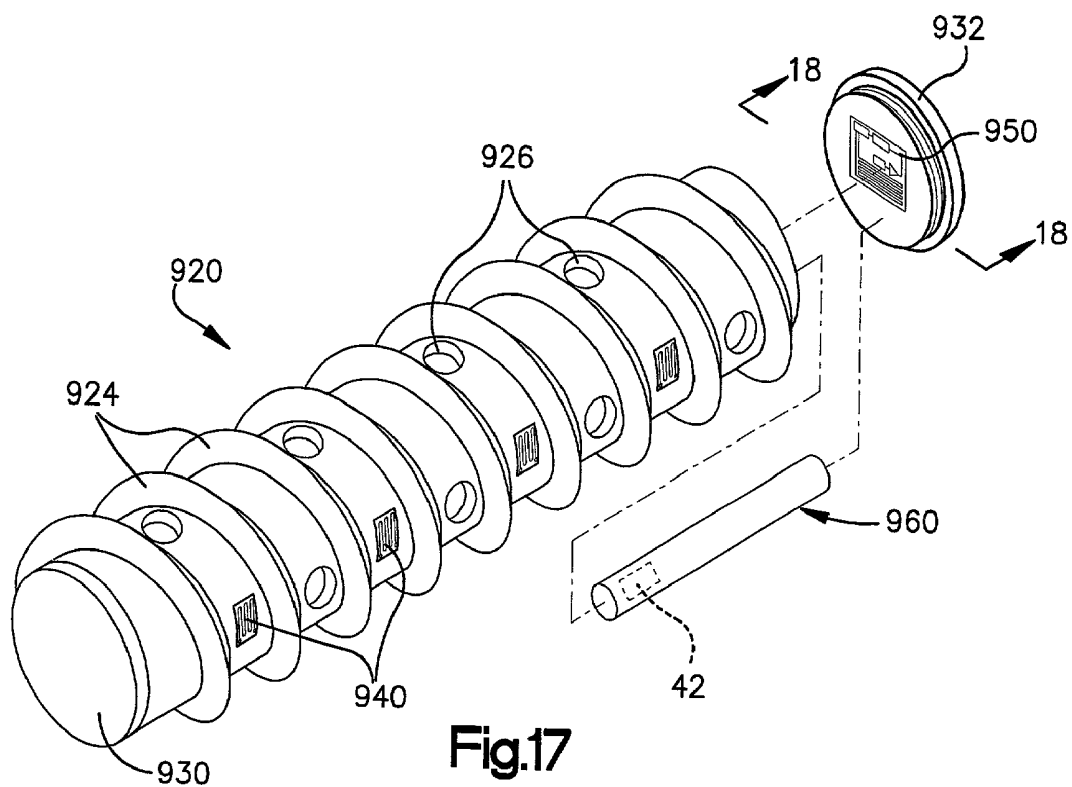

APPARATUS AND METHOD FOR ASSESSING LOADS ON ADJACENT BONES

TECHNICAL FIELD

[0001] The present invention relates to an apparatus and method for assessing loads on adjacent bones, and is particularly directed to an apparatus and method for providing an in vivo assessment of loads on adjacent bones to be fused together.

BACKGROUND OF THE INVENTION

[0002] It is known to use surgical procedures to stabilize a fractured bone or repair a problematic interaction of adjacent bones. For example, spinal surgery is frequently performed to stabilize a problematic portion of the spine and relieve pain. Often, the vertebrae in the problematic portion of the spine are fused together with a bone graft in order to achieve the stabilization. Because the bone fusion takes time (six months or more on average), spinal implants (often referred to as fixation instrumentation), such as rods, clamps, and plates, are typically implanted and used to secure the vertebrae while the fusion of the bone graft takes place.

[0003] During the months while the arthrodesis is occurring, it is desirable to monitor the progress of the bony incorporation, or bone-ingrowth, of the graft. Known methods for examining the bony incorporation include radiographic evaluation, magnetic resonance imaging, and computerized tomography. All of these techniques provide a snapshot of the progress of the bony incorporation, but do not provide accurate, continuous, real-time information to the patient and physician. Without the ability to accurately and continuously assess the bony incorporation, pseudoarthrosis (non-healed bone fusion) may occur unbeknownst to the physician. Such pseudoarthrosis may cause post-operative pain for the patient and necessitate additional surgery. If the fusion progress could be assessed continuously or on-demand during the post-operative period by assessing the loads on the fixation instrumentation, it may be possible to appropriately time additional surgery or even avoid additional surgery.

[0004] In a related manner, it is also desirable to assess the biomechanical performance of implanted spinal fixation instrumentation during the post-operative period while bone fusion is occurring. Both in vitro and in vivo biomechanical testing of fixation instrumentation has been done in the past, but with limited success. Current in vitro testing of fixation instrumentation typically subjects cadaveric vertebrae and implantable instrumentation to various axial and torsional loading parameters on a hydraulic testing apparatus. Unfortunately, the use of nonliving cadaveric tissue can introduce significant error into the test data.

[0005] Previous attempts at in vivo biomechanical testing of spinal fixation instrumentation have been done primarily using animals (quadrupeds), but some limited testing has been done with humans. In one of the in vivo human tests performed to date, sensors that were placed on the implanted spinal instrumentation utilized wires to carry data percutaneously (through the skin) from the sensors to a data monitoring unit outside the human body. The use of wires or other type of electrical or optical connection extending

through the skin provides a significant risk of infection and is not suitable for long-term testing as there is a high risk of wire breakage.

[0006] Another problem encountered with the in vivo testing that has been done is failure of a sensor, such as a strain gauge, or the sensor wiring which has been known to break, corrode, or debond within four months of in vivo implantation. While attempts have been made to use telemetry to transmit data from sensors implanted in transcranial applications to an external monitoring device, a need exists for an implantable, telemetered sensor arrangement for spinal or other orthopedic applications that could survive a minimum of a year.

[0007] Microelectromechanical systems, or MEMS, refers to a class of miniature electromechanical components and systems that are fabricated using techniques originally used in the fabrication of microelectronics. MEMS devices, such as pressure sensors and strain gauges, manufactured using microfabrication and micromachining techniques can exhibit superior performance compared to their conventionally built counterparts and are resistant to failure due to corrosion, etc. Further, due to their extremely small size, MEMS devices can be utilized to perform functions in unique applications, such as the human body, that were not previously feasible using conventional devices.

SUMMARY OF THE INVENTION

[0008] The present invention is an apparatus for providing an in vivo assessment of loads on adjacent bones. The apparatus comprises a body for insertion between the adjacent bones. At least one sensor is associated with the body. The at least one sensor generates an output signal in response to and indicative of a load being applied to the body through the adjacent bones. At least one telemetric device is operatively coupled with the at least one sensor. The least one telemetric device is operable to receive the output signal from the at least one sensor and to transmit an electromagnetic field (EMF) signal dependent upon the output signal.

[0009] In accordance with one embodiment of the invention, the body comprises an implant for helping the adjacent bones to fuse together. The implant comprises a bone graft. In accordance with another embodiment of the invention, the body comprises a fusion cage for insertion between an adjacent pair of vertebrae. In accordance with yet another embodiment, the body comprises a prosthetic device for preserving motion between adjacent bones.

[0010] According to various features of the invention, the at least one sensor comprises a pressure sensor, a load cell, and/or at least one strain gauge.

[0011] According to another aspect of the present invention, an apparatus for providing an in vivo assessment of loads on adjacent bones comprises a body for insertion between the adjacent bones and sensor means for sensing a load being applied to the body through the adjacent bones. The sensor means generates a corresponding output signal in response to and indicative of a sensed load. First circuit means is operatively coupled with the sensor means for receiving the output signal from the sensor means. The first circuit means includes antenna means for receiving energy to power the first circuit means and the sensor means and for transmitting an EMF signal dependent upon the output signal.

[0012] In according with another feature of the invention, the apparatus further comprises second circuit means for transmitting energy to power the first circuit means and the sensor means and for receiving the EMF signal. The second means is disposed remote from the first circuit means.

[0013] According to yet another aspect of the present invention, an apparatus for providing an in vivo assessment of loads on and motion of one or more bones comprises a member for placement adjacent a bone and at least one sensor associated with the member. The at least one sensor generates an output signal in response to and indicative of a load being applied to the member through the bone. At least one telemetric device is operatively coupled with the at least one sensor. The at least one telemetric device is operable to receive the output signal from the at least one sensor and to transmit an EMF signal dependent upon the output signal.

[0014] According to various embodiments of the present invention, the member comprises an implant for helping adjacent bones fuse together, such as a fusion cage, a fixation plate, and/or a bone graft. Alternatively, the member comprises a prosthetic device for preserving motion between adjacent bones.

[0015] According to still another aspect of the present invention, an apparatus for providing an in vivo assessment of loads on and motion of one or more bones comprises at least one sensor attached to a bone. The at least one sensor generates an output signal in response to and indicative of a load on the bone. At least one telemetric device is operatively coupled with the at least one sensor. The at least one telemetric device is operable to receive the output signal from the at least one sensor and to transmit an EMF signal dependent upon the output signal.

[0016] The present invention also provides a method for in vivo assessing the loads on adjacent bones to be fused together. According to the inventive method, a body for insertion between the adjacent bones is provided. The body is instrumented with at least one sensor for sensing a load on the body and for generating an output signal indicative of a sensed load. At least one telemetric device is operatively coupled with the at least one sensor to receive the output signal and to transmit an EMF signal dependent upon the output signal. The body is implanted between the adjacent bones. The EMF signal from the at least one telemetric device is then monitored.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] The foregoing and other features of the present invention will become apparent to those skilled in the art to which the present invention relates upon reading the following description with reference to the accompanying drawings, in which:

[0018] **FIG. 1** is a perspective view of a portion of a human spine illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones in accordance with the present invention;

[0019] **FIG. 2** is a side view, taken in section, illustrating the apparatus of **FIG. 1**;

[0020] **FIG. 3** is a sectional view of a component of the apparatus shown in **FIG. 2**;

[0021] **FIG. 3A** is a view similar to **FIG. 3** illustrating an alternate construction of the component;

[0022] **FIG. 4** is a perspective view taken along line 4-4 in **FIG. 3**;

[0023] **FIG. 5** is a plan view taken along line 5-5 in **FIG. 3**;

[0024] **FIG. 6** is a schematic block diagram of the apparatus for providing an in vivo assessment of loads on adjacent bones;

[0025] **FIG. 7** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a second embodiment of the present invention;

[0026] **FIG. 8** is a sectional view, similar to **FIG. 3**, showing a component of the apparatus of **FIG. 7**;

[0027] **FIG. 9** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a third embodiment of the present invention;

[0028] **FIG. 10** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a fourth embodiment of the present invention;

[0029] **FIG. 11** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a fifth embodiment of the present invention;

[0030] **FIG. 12** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a sixth embodiment of the present invention;

[0031] **FIG. 13** is a perspective view, similar to **FIG. 1**, of a portion of a human spine illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones in accordance with a seventh embodiment of the present invention;

[0032] **FIG. 14** is an enlarged view illustrating a component of the apparatus of **FIG. 13**;

[0033] **FIG. 15** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with an eighth embodiment of the present invention;

[0034] **FIG. 16** is a side view, similar to **FIG. 2**, illustrating an apparatus for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a ninth embodiment of the present invention;

[0035] **FIG. 17** is a perspective view of a component of the apparatus of **FIG. 16**; and

[0036] **FIG. 18** is a schematic block diagram of another component of the apparatus of **FIG. 16**.

DESCRIPTION OF EMBODIMENTS

[0037] The present invention relates to an apparatus and method for providing an in vivo assessment of loads on adjacent bones. As representative of the present invention, **FIG. 1** illustrates several cervical vertebrae in a human spine

and an apparatus **10** for providing an in vivo assessment of loads on adjacent cervical vertebrae to be fused together. It should be understood that the apparatus **10** could be used to assess loads and motion in other regions of the human spine. Further, it should also be understood that basic concept of the apparatus **10** could be used to assess loads on and motion of bones in other areas of the human body such as, for example, hip and knee joints, as well as loads on and motion of cartilage, muscles, ligaments, and tendons associated with various bones.

[0038] Cervical vertebrae C2-C7, identified by reference numbers **20-30**, respectively, are shown in FIG. 1. A discectomy has been performed to remove a problematic intervertebral disc (not shown) between two vertebrae (indicated by reference numbers **24** and **26**). The removal of the disc leaves an intervertebral space **32** (FIG. 2) between the vertebrae **24** and **26**. The intervertebral space **32** is to be filled with a body of bone graft material. In the illustrated embodiment, the body of bone graft material is an autograft **34** harvested from the patient undergoing the discectomy, but the body of bone graft material could alternatively be an allograft, heterograft, or a graft made of a synthetic, bio-compatible material.

[0039] Prior to insertion of the autograft **34** into the space **32** between the vertebrae **24** and **26**, a small passage (not shown) is drilled into the cancellous bone in the interior of the autograft. A transducer assembly **40** placed into the interior of the autograft **34** through a small cannula (not shown). To place the transducer assembly **40** into the autograft **34**, the transducer assembly is first loaded into one end of the cannula, and the end of the cannula is then inserted into the passage in the autograft. Morselized cancellous bone may also be placed into the cannula to protect the transducer assembly **40** and to assist in moving the transducer assembly from the end of the cannula into the interior of the autograft **34**. Following placement of the transducer assembly **40** inside the autograft **34**, the cannula is removed. The passage may then be filled with additional morselized cancellous bone to close and seal the passage.

[0040] The transducer assembly **40** comprises a pressure sensor **42** and a telemetric device **44**. The transducer assembly **40** is encased in a shell **46** made of a biocompatible metal, such as titanium, or other suitable biocompatible material. As may be seen in FIG. 3, a portion of the shell **46** has a recess **48** defining a thin wall section **50** that is responsive to external pressure. Inside the shell **46**, a pair of spacers **52** separate the transducer assembly **40** from the shell.

[0041] The illustrated pressure sensor **42** is of a known configuration and is made using known micromachining processes, microfabrication processes, or other suitable MEMS fabrication techniques. Pressure sensors of this type are commercially available from Motorola, Inc. of Schaumburg, Ill. and TRW Novasensor of Fremont, Calif. It should be understood that any pressure sensor that meets the biocompatibility and size requirements (less than two mm³) may be used.

[0042] The illustrated pressure sensor **42** is a piezoresistive device, but it should be understood that other types of pressure sensors, such as a piezoelectric and capacitive sensors, could be substituted. As best seen in FIG. 4, the pressure sensor **42** comprises a substrate **60**, a sensing

diaphragm **62**, a plurality of patterned resistors **64**, and a plurality of bond pads **66**, two of which are associated with each of the resistors.

[0043] The substrate **60** has upper and lower surfaces **67** and **68**, respectively, and is made of silicon, but could alternatively be made of another suitable material. The substrate **60** has a well region **70** that extends between the upper and lower surfaces **67** and **68** and that is formed using a conventional microfabrication and bulk micromachining processes including lithography and etching. The sensing diaphragm **62**, which extends across the well region **70**, is also made of silicon and is defined by the lithography and etching processes. The resistors **64** and the bond pads **66** are formed from a metal layer that is deposited, patterned, and etched in a known manner on the lower surface **68** of the substrate **60**. The resistors **64** could also be formed by doping the silicon using boron, phosphorus, arsenic, or another suitable material to make it highly conductive. The resistors **64** are positioned along the edges of the sensing diaphragm **62** to detect strain in the sensing diaphragm caused by pressure differentials.

[0044] The telemetric device **44** in the transducer assembly **40** comprise an electronics module **80** (FIG. 3) and an antenna **82**. The electronics module **80** is operatively coupled to the pressure sensor **42** by the bond pads **66** in a manner not shown. As shown in the block diagram of FIG. 6, the electronics module **80** comprises an integrated circuit. It is contemplated that an application specific integrated circuit (ASIC) could be designed to incorporate the electronics module **80** and the antenna **82**.

[0045] The integrated circuit includes an RF-DC converter/modulator **84** and a voltage regulator **86** operatively coupled between the antenna **82** and the pressure sensor **42**. The integrated circuit further includes a microprocessor **88** operatively coupled between the pressure sensor **42** and the RF-DC converter/modulator **84**. To protect the circuitry of the electronics module **80**, the electronics module may be coated with a soft polymeric film, such as parylene or polydimethylsiloxane (PDMS), or a biocompatible epoxy.

[0046] The antenna **82** may be fabricated on the substrate of the pressure sensor **42** using known micromachining or microfabrication techniques, or may alternatively be fabricated separately and joined with the pressure sensor. The antenna **82** comprises a spiral-shaped coil **90** (FIG. 5) of metal deposited over an oxide layer **92** (FIG. 3). A layer of doped polysilicon **94** underneath the oxide layer establishes an electrical connection between a contact **96** in the center of the coil **90** and one of two contacts **98** outside the coil. The contacts **98** of the antenna **82** outside of the coil **90** are operatively coupled with the electronics module **80** in a manner not shown. For protection purposes, the antenna **82** may be coated with a soft polymeric film, such as parylene or PDMS, or a biocompatible epoxy.

[0047] Before the shell **46** of the transducer assembly **40** is sealed shut, in a manner not shown, to encapsulate the transducer assembly, the interior of the shell is filled with a silicone gel **100**, sol-gel, or other suitable material that is dielectric and biocompatible. The properties of the gel **100** allow it to transmit pressure exerted against the thin section **50** of the shell **46** uniformly against the sensing diaphragm **62** of the pressure sensor **42**, while isolating the electrical components and circuitry of the transducer assembly **40** from any corrosive media.

[0048] The shell 46 containing the transducer assembly 40 is then packaged within a biomolecular coating 102. Exposing the shell 46 to solutions containing desired biomolecules, such as collagen or hyaluronan, leads to monolayer coating of the outer surface of the shell 46. Alternatively, the outer surfaces of the shell 46 may be coated with thin layers of a soft biocompatible material, such as parylene or PDMS.

[0049] FIG. 3A illustrates an alternate configuration for the transducer assembly 40, indicated by the suffix "a". The difference between the transducer assembly 40 of FIG. 3 and the transducer assembly 40a of FIG. 3A is that the shell 46 has been omitted. The transducer assembly 40a is simply coated with a biocompatible polymeric film 104, such as parylene or PDMS, or a biocompatible epoxy. The transducer assembly may then also be packaged within a biomolecular coating 102a, as described above.

[0050] Returning now to the first embodiment of the present invention, when the transducer assembly 40 is positioned inside the autograft 34 as described above, the autograft is ready to be inserted into the intervertebral space 32 between the vertebrae 24 and 26. Insertion of the autograft 34 into the intervertebral space 32 involves a distraction procedure known in the art.

[0051] After the autograft 34 has been inserted between the vertebrae 24 and 26, a spinal fixation implant 120 (FIG. 1) is connected to the cervical vertebrae 22, 24, and 28 to stabilize the vertebrae 20-30 while the autograft 34 fuses the adjacent vertebrae 24 and 26 together. According to the illustrated embodiment, the implant 120 comprises a modified version of the DOC™ Ventral Cervical Stabilization System (hereinafter referred to as the "DOC™ system 122"), available from the DePuy/AcroMed division of Johnson & Johnson, described in U.S. Pat. Nos. 5,843,082 and 6,036,693. It should, however, be understood that the implant 120 could be any type of implanted orthopedic instrumentation or device.

[0052] The DOC™ system 122 includes a plurality of plates 124 that are anchored to the vertebrae by screws 126 and interconnected by first and second rods 128 and 130. A platform 132 also extends between the rods 128 and 130 and is secured to the rods by setscrews 134. The platform 132 is positioned over the inserted autograft 34.

[0053] A second transducer assembly 140, comprising a plurality of strain gauges 142 and a second telemetric device 144, is mounted to the DOC™ system. The second telemetric device 144 is constructed like the telemetric device described above and comprises a second electronics module 146 and a second antenna 148, both of which are shown only schematically in FIG. 2. The second electronics module 146 is located on a first side of the platform 132 facing toward the autograft 34, while the second antenna 148 is located on an oppositely disposed second side of the platform 132.

[0054] The second electronics module 146 has the basic construction as the electronics module 80 in the transducer assembly 40 illustrated in FIG. 6. The second electronics module 146 comprises an integrated circuit that is operatively coupled to the second antenna 148 on the second side of the platform 132 in manner not shown. To protect its circuitry, the second electronics module 146 may be coated with a soft polymeric film, such as parylene or PDMS, or a biocompatible epoxy.

[0055] As may be seen in FIG. 1, the second antenna 148 is larger in overall size than the antenna 82 in the transducer assembly 40, but has the same basic configuration and construction. The second antenna 148 may be fabricated using known MEMS fabrication or micromachining techniques, or any other conventional microelectronic fabrication process. The second antenna 148 comprises a spiral-shaped coil of metal deposited over an oxide layer. A layer of doped polysilicon underneath the oxide player establishes an electrical connection between a contact in the center of the coil and a contact outside the coil. For protection purposes, the antenna 82 may be coated with a soft polymeric film, such as parylene or PDMS, or a biocompatible epoxy.

[0056] In accordance with the apparatus 10, the first and second rods 128 and 130 of the DOC™ system 122 are instrumented with the plurality of strain gauges 142. The strain gauges 142 may be commercially available devices, such as those produced by microelectronics suppliers such as Vishay Inc. and MicroMeasurements Inc., or may be custom-fabricated by a foundry. Two of the strain gauges 142 are secured to the first rod 128 above and below, respectively, the platform 132. The strain gauges 142 are operatively coupled to the second electronics module 146 by electrical leads in the form of metal traces 150 deposited on the surface of an insulating film (not shown) covering the first rod 128 and the side of the platform 132. Alternatively, the electrical ends could be insulated wires threaded through the inside of the rod 128 to make contact. For protection purposes, the strain gauges 142 and the electrical traces 150 may be coated with a soft polymeric film, such as parylene or PDMS, a biocompatible epoxy, or a monolayer of biomolecular coating.

[0057] Similarly, another two strain gauges 142 are secured to the second rod 130 above and below, respectively, the platform 132. These two strain gauges 142 are also operatively coupled to the second electronics module 146 by electrical leads in the form of metal traces 150 deposited on the surface of the second rod 130 and the side of the platform 132. Again, the strain gauges 142 and the electrical traces 150 associated with the second rod 130 may be coated with a soft polymeric film, such as parylene or PDMS, or a biocompatible epoxy.

[0058] The apparatus 10 further includes an external (meaning it is located outside of and/or remote from the patient's body) readout/power supply unit 160 (FIG. 6) having an integrated antenna 162. The readout/power supply unit 160 contains circuitry known in the art and therefore not described in any detail. The readout/power supply unit 160 may be a hand-held device or a larger piece of equipment found at a physician's office. The readout/power supply unit 160 could also be a device worn by the patient.

[0059] The readout/power supply unit 160 is operable to transmit electrical energy and receive data through the antenna 162 as described further below. Further, the readout/power supply unit 160 is able to display and store the received data.

[0060] Following implantation of the instrumented autograft 34 and the instrumented DOC™ system 122 into the spine as described above, the apparatus 10 can be used to provide an in vivo assessment of the bony incorporation of the autograft, and thus the fusion of the autograft and the

vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system. The readout/power supply unit **160** transmits electrical energy in the form of an electromagnetic field (EMF) signal, or more specifically a radio frequency (RF) signal, through the antenna **162** to the transducer assembly **40** in the autograft **34** and to the transducer assembly **140** on the platform **132**. The RF signal is received through the antennas **82** and **148** in each of the transducer assemblies **40** and **140**, respectively, and is converted into a DC signal to energize the circuitry in the sensor assemblies, including the pressure sensor **42** and the strain gauges **142**.

[0061] The pressure sensor **42** in the autograft **34** detects changes in electrical resistance caused by deformation and strain on the sensing diaphragm **62**. The changes in resistance detected by the pressure sensor **42** correspond to applied pressure and a data signal dependent upon the sensed condition is generated by the electronics module **80**. The data signal is then transmitted percutaneously from the antenna **82** to the antenna **162** in the readout/power supply unit **160**. The data signal transmitted is a pulse-width-modulated (PWM) signal that has an RF carrier frequency. It should be understood that other signal types (e.g., frequency modulation (FM) or frequency shift key (FSK)) could also be used.

[0062] The antenna **162** in the readout/power supply unit **160** receives the data signal from the transducer assembly **40**, processes the data signal, and displays pressure data based on the data signal that correspond to the pressure sensed by the pressure sensor **42**. The pressure data may be displayed in any number of formats, such as absolute values or plots. The pressure data may also be stored by the readout/power supply unit **160**.

[0063] While the readout/power supply unit **160** is providing electrical power to and receiving data from the transducer assembly **40** in the autograft **34**, the readout/power supply unit **160** is also doing the same with the second transducer assembly **140** on the DOC™ system **122**. The implanted strain gauges **142** detect changes in strain on the rods **128** and **130**. The electronics module **146** on the platform **132** generates data signals dependent upon the sensed changes in strain. These data signals are then transmitted percutaneously from the antenna **148** to the antenna **162** in the readout/power supply unit **160**. As above, the data signals transmitted are a pulse-width-modulated (PWM) signals that have an RF carrier frequency, but could be other signal types (e.g., frequency modulation (FM) or frequency shift key (FSK)).

[0064] The antenna **162** in the readout/power supply unit **160** receives the data signals from the second transducer assembly **140**, processes the data signals, and displays strain data based on the data signals that correspond to the strain on the rods **128** and **130**. The strain data may be displayed in any number of formats, and may also be stored by the readout/power supply unit **160**.

[0065] The pressure data and the strain data received by the readout/power supply unit **160** provide an in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**. For example, an expected pattern of loads detected by the pressure sensor **42** will initially involve

pressure oscillations that dampen over time, with an overall increase in applied pressure indicative of bone incorporation of the autograft **34**. On the other hand, an expected pattern of strain detected by the strain gauges **142** will initially involve large axial forces that will decrease over time as the DOC™ system **122** shares more of the load with the vertebrae **24** and **26** that are being fused by the autograft **34**. If the data from the pressure sensor **42** and the strain gauges **142** follows or deviates from the expected patterns, conclusions can be drawn about progress of the fusion between the autograft **34** and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**.

[0066] The apparatus **10** described above provides the ability to continuously, or on-demand, monitor fusion progress and biomechanical performance during the post-operative period by assessing the loads on the autograft **34** and on the spinal fixation instrumentation. Because of this ability to continuously or on-demand monitor fusion progress and biomechanical performance, it may be possible to appropriately time, or even avoid, additional surgery. Further, information gathered from such in vivo assessments can lead to improvements in surgical techniques and spinal implant design.

[0067] FIGS. 7 and 8 illustrate an apparatus **210** for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a second embodiment of the present invention. In the second embodiment of FIGS. 7 and 8, reference numbers that are the same as those used in the first embodiment of FIGS. 1-6 designate components that are the same as components in the first embodiment.

[0068] According to the second embodiment, a tube **220** replaces the shell **46** and encapsulates a transducer assembly **240**. The tube **220** is made of metal, such as titanium, and is fixedly attached to the platform **132** of the DOC™ system in a manner not shown. The transducer assembly **240** is positioned inside the end of the tube **220** and coated inside the tube with a dielectric gel as described above. The tube **220** is inserted into the passage drilled into the autograft **34** so that the transducer assembly **240** is located approximately in the middle of the autograft.

[0069] The tube **220** containing the transducer assembly **240** may be packaged within a biomolecular coating. Exposing the tube **220** to solutions containing desired biomolecules, such as collagen or hyaluronan, leads to monolayer coating of the outer surface of the tube. Alternatively, the outer surfaces of the tube **220** may be coated with thin layers of a soft biocompatible material, such as parylene or PDMS.

[0070] The transducer assembly **240** comprises the pressure sensor **42** described above, but could alternatively utilize another suitable type of micromachined/microfabricated sensor. Unlike the transducer assembly **40** described above, the transducer assembly **240** does not include an antenna. Rather, wires **250** (FIG. 8) extend through the tube **220** to electrically connect the electronics module **146** on the platform **132** to an electronics module **280** in the transducer assembly **240**. The wires **250** carry electrical power from the second transducer assembly **140** to the transducer assembly **240** in the autograft **34**. The wires **250** also carry data signals from the pressure sensor **42** back to the second transducer assembly **140** for transmission over the antenna **148** on the platform **132**.

[0071] The apparatus **210** according to the second embodiment functions in the same manner as the apparatus of the

first embodiment to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system.

[0072] FIG. 9 illustrates an apparatus **310** for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a third embodiment of the present invention. In the third embodiment of FIG. 9, reference numbers that are the same as those used in FIGS. 1-8 designate components that are the same as components shown in FIGS. 1-8.

[0073] According to the third embodiment, the apparatus **310** includes a load cell **320**. The load cell **320** is counter-sunk into the upper surface (as viewed in the Figures) of the autograft **34** facing the vertebrae **26**. It should be understood, however, that the load cell **320** could be positioned in any number of locations in the autograft **34**. Further, it is contemplated that more than one load cell **320** could be positioned in the autograft **34**.

[0074] Like the transducer assembly **40** illustrated in FIG. 3, the load cell **320** includes a sensing element (not shown) and an integral telemetry device (not shown) constructed using MEMS and/or microelectronic fabrication techniques. The telemetry device includes an electronics package and an antenna. The sensing element in the load cell **320** may be a piezoresistive device, a piezoelectric device, a capacitive device, a strain gauge-based device, or any other suitable device. Using an RF carrier signal, the load cell **320** is inductively powered and interrogated for data in the same manner as the transducer assembly **40** described in the first embodiment.

[0075] The load cell **320** has an outer housing **322** that may be packaged within a biomolecular coating. Exposing the outer housing **322** of the load cell **320** to solutions containing desired biomolecules, such as collagen or hyaluronan, leads to monolayer coating of the surface of the outer housing **322**. Alternatively, the outer housing **322** of the load cell **320** may be coated with thin layers of a soft biocompatible material, such as parylene or PDMS.

[0076] The apparatus **310** according to the third embodiment functions in a similar manner to the apparatus **10** of the first embodiment to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**. The addition of the load cell **320** in the apparatus provides additional data for the physician to assess the bone in-growth and biomechanical performance of the implant.

[0077] FIG. 10 illustrates an apparatus **410** for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a fourth embodiment of the present invention. In the fourth embodiment of FIG. 10, reference numbers that are the same as those used in FIGS. 1-9 designate components that are the same as components shown in FIGS. 1-9.

[0078] According to the fourth embodiment, the apparatus **410** includes the first and second transducer assemblies **40** and **140**, as well as the load cell **320**. A tube **430** extends between the transducer assembly **40** in the autograft **34** and

the load cell **320** in the upper surface of the autograft. As above, it should be understood that the load cell **320** could be positioned in any number of locations in the autograft **34**.

[0079] Unlike the load cell **320** described above in the third embodiment, the load cell **320** does not include an antenna. Rather, wires (not shown) extend through the tube **430** to electrically connect any electronics module (not shown) in the load cell **320** to the electronics module **80** in the transducer assembly **40**. The wires carry electrical power from the transducer assembly **40** to the load cell **320**. The wires also carry data signals from the load cell **320** back to the transducer assembly **40** for RF transmission to the readout/power supply device **160**.

[0080] It should be apparent that a variant of the fourth embodiment would be that a telemetry device, including an electronics module and an antenna, be located in the load cell **320** rather than in the transducer assembly **40**. Further, it should also be apparent that another variant of the fourth embodiment would be to use the transducer assembly **240** of FIG. 9, which does not include an electronics module nor an antenna, and the tube **220** that houses wires for exchanging signals.

[0081] The apparatus **410** according to the fourth embodiment functions in the same manner as the apparatus **310** of the third embodiment to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**.

[0082] In FIG. 11, an apparatus **510** constructed in accordance with a fifth embodiment of the present invention is illustrated. The fifth embodiment of FIG. 11 is nearly identical to the fourth embodiment of FIG. 10, except that both the transducer assembly **40** and the load cell **320** have integral telemetry devices. As such, the readout/power supply unit **160** thus separately inductively powers and collects data from the load cell **320**, the transducer assembly **40** in the autograft **34**, and the transducer assembly **140** on the DOC™ system **122**. Accordingly, the apparatus **510** functions in the same basic manner as the apparatus **310** of the third embodiment **310** to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**.

[0083] FIG. 12 illustrates an apparatus **610** constructed in accordance with a sixth embodiment of the present invention. The sixth embodiment of FIG. 12 is similar to the third embodiment of FIG. 9, except that in FIG. 12 a second tube **630** connects the load cell **320** to the transducer assembly **140** on the platform **132**. This is because the load cell **320** does not have an integral telemetry device and thus wires (not shown) are run through the second tube **630** to carry electrical power and data to and from, respectively, the load cell **320**. As such, all of the data from the load cell **320**, the pressure sensor **42**, and the strain gauges **142** is transmitted over the antenna **148** on the platform **132**. Other than this difference, the apparatus **610** according to the sixth embodiment functions in the same basic manner as the apparatus **310** of the third embodiment to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the

vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**.

[0084] FIGS. **13** and **14** illustrate an apparatus **710** for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a seventh embodiment of the present invention. In the seventh embodiment of FIGS. **13** and **14**, reference numbers that are the same as those used above designate components that are the same as components described above.

[0085] According to the seventh embodiment, the apparatus **710** comprises a plurality of transducer assemblies **740** mounted to the rods **128** and **130** of the DOC™ system **122**. Additional transducer assemblies may be located in the autograft **34** as described above, but are omitted from FIGS. **13** and **14** for clarity. Each transducer assembly **740** includes a sensor, such as a strain gauge **742**, and an integral telemetry device **744** constructed using MEMS and/or microelectronic fabrication techniques. As best seen in the schematic diagram of FIG. **14**, each telemetry device **744** includes an electronics package **746** and an antenna **748**. Hence, there are no electronics present on the platform **132**. Using RF carrier signals, each strain gauge **742** is inductively powered and interrogated for data in the same manner as the transducer assembly **40** described in the first embodiment.

[0086] The apparatus **710** according to the seventh embodiment functions to provide a continuous or on-demand in vivo assessment of the bony incorporation of the autograft **34**, and thus the fusion of the autograft and the vertebrae **24** and **26**, as well as the biomechanical performance of the DOC™ system **122**.

[0087] FIG. **15** illustrates an apparatus **810** for providing an in vivo assessment of loads on and motion of a bone in accordance with an eighth embodiment of the present invention. In the eighth embodiment of FIG. **15**, reference numbers that are the same as those used above designate components that are the same as components described above.

[0088] In accordance with the eighth embodiment, an artificial disc **820** is inserted between the vertebrae **24** and **26** in place of a problematic disc. The artificial disc **820** is intended to carry the loads on the vertebrae **24** and **26** and also preserve the motion of the vertebrae. The artificial disc **820** illustrated in FIG. **15** has upper and lower plates **822** and **824** spaced apart by a flexible polymeric core **826**. It should, however, be understood that other configurations of artificial discs could also be used.

[0089] Prior to insertion of the artificial disc **820** between the vertebrae **24** and **26**, a transducer assembly such as the transducer assembly **40** described in the first embodiment, is positioned within the artificial disc. Additional transducer assemblies (not shown) may also be located in the artificial disc **820**. Further, as shown in FIG. **15**, it is contemplated that a transducer assembly **40** can be positioned in the interior of a vertebrae, such as the vertebrae **26**, by inserting the transducer assembly into a passage drilled in the vertebrae. The apparatus **810** according to the eighth embodiment functions to provide a continuous or on-demand in vivo assessment of the loads on the vertebrae **26** and on the artificial disc **820**, as well as provide an assessment of the motion of the artificial disc relative to the vertebrae **24** and **26**.

[0090] It should be understood that the apparatus **810** could be used in any number of different applications in the human body where it is desirable to assess the loads on one or more bones or on an orthopedic implant. Furthermore, it should also be understood that the apparatus **810** could be used to assess motion of, or between, adjacent bones and/or orthopedic implants. Such additional applications of the apparatus **810** would include most joints in the human body.

[0091] FIGS. **16-18** illustrate an apparatus **910** for providing an in vivo assessment of loads on adjacent bones constructed in accordance with a ninth embodiment of the present invention. In the ninth embodiment of FIGS. **16-18**, reference numbers that are the same as those used above designate components that are the same as components described above.

[0092] According to the ninth embodiment, another different type of implant is inserted into the intervertebral space **32** following a discectomy. The implant is an interbody fusion cage **920** known in the art. The fusion cage **920** has a cylindrical outer surface **922** with external threads **924**. The fusion cage **920** is screwed into place in the intervertebral space **32** so that the threads **924** bite into the surfaces (also known as endplates) of the vertebrae **24** and **26**. As is known in the art, the fusion cage **920** has a plurality of openings **926** that extend through the outer surface **922** and into an interior chamber (not numbered). After the fusion cage **920** is implanted in the vertebrae **24** and **26**, the interior chamber is filled with bone graft material, such as bone chips or a synthetic material to promote bone growth. Removable end caps **930** and **932** close the interior chamber after the bone graft material has been placed inside the fusion cage **920**. Over time, bone in-growth occurs and the fusion cage **920** fuses the vertebrae **24** and **26** together. The openings **926** in the fusion cage **920** help to facilitate the bone in-growth, and thus, the fusion process.

[0093] Prior to implantation of the fusion cage **920**, a plurality of strain gauges **940** are installed on the fusion cage. The strain gauges **940** are located in the groove that lies between the threads **924** on the outer surface **922** of the fusion cage **920**. The strain gauges **940** may be commercially available devices or custom-fabricated by a foundry. The strain gauges **940** are operatively coupled to a telemetry device **950** located on the end cap **932** by electrical leads in the form of metal traces (not shown) deposited on an insulating film (not shown) or the inside surface of the fusion cage. The traces make electrical contact with traces (not shown) on the end cap **932** when the end cap is attached to the fusion cage **920**. Alternatively, the electrical leads could be insulated wires. For protection purposes, the strain gauges **940** and the electrical traces may be coated with a soft polymeric film, such as parylene or PDMS, a biocompatible epoxy, or a monolayer biomolecular coating. Alternatively, each strain gauge **940** could have an integral telemetry device constructed using MEMS and/or microelectronic fabrication techniques.

[0094] A metal tube **960** is attached, in a manner not shown, to the end cap **932** and extends into the interior chamber of the fusion cage **920**. A pressure sensor, such as the pressure sensor **42** described above, is positioned inside the end of the tube **960** and coated with a dielectric gel as described above. Wires (not shown) extend through the tube **960** to electrically connect the pressure sensor to the telem-

etry device **950**. The tube **960** containing the pressure sensor **42** may be packaged within a biomolecular coating or coated with thin layers of a soft biocompatible material, such as parylene or PDMS.

[0095] As shown in **FIG. 18**, the telemetry device **950** on the end cap **932** of the fusion cage **920** includes an electronics module **960** and an antenna **970**. In the same manner as described above with regard to the previous embodiments, the telemetry device **950** is inductively powered by the readout/power supply unit **160** and is operable to transmit data from the strain gauges **940** and pressure sensor **42** via an RF carrier signal out to the readout/power supply unit.

[0096] The apparatus **910** according to the ninth embodiment of the present invention functions to provide a continuous or on-demand in vivo assessment of bony incorporation, and thus the fusion of the fusion cage **920** and the vertebrae **24** and **26**, as well as the biomechanical performance of the fusion cage.

[0097] In addition to the telemetry schemes described above, it is contemplated that an alternative telemetry scheme using a tank circuit (not shown) could be employed with each of the aforementioned embodiments of the present invention. It is known that a change in capacitance or inductance on a sensor, such as a pressure sensor or a strain gauge, can be detected using a tank circuit. Such a tank circuit has either a variable capacitance and a fixed inductance, or a variable inductance and a fixed capacitance.

[0098] If the tank circuit has a variable capacitance, the capacitance will change as the pressure or strain, depending on the type of sensor, changes. This change in capacitance leads to changes in resonant frequency that can be detected. The capacitance changes can then be calculated using the following equation: $f_0 = 1/2\pi(LC)^{1/2}$, where L is the inductance and C is the capacitance. This same equation is also used to calculate inductance changes if the capacitance of the tank circuit is fixed. In the embodiments discussed above where there are multiple sensors, each sensor is designed to operate within a specific resonant frequency band. The tank circuit is then swept over range of frequencies so that the individual resonant frequency of each sensor, which corresponds to the output of each sensor, can be identified.

[0099] In the present invention, the tank circuit telemetry scheme could be employed in several different ways. The circuitry of the tank circuit could be added to the electronics module associated with each of the implanted sensors. Alternatively, the implanted sensors could be capacitive sensors having an integral tank circuitry. Finally, the conventional tank circuit described above (variable capacitance or variable inductance) could be configured such that the variable capacitor and one half of the inductor are fabricated on the same sensing diaphragm. The other half of the inductor is combined with a fixed electrode of the capacitor such that when the sensing diaphragm moves, the capacitance and the inductance increase or decrease together.

[0100] From the above description of the invention, those skilled in the art will perceive improvements, changes and modifications. For example, it is contemplated that the EMF signals exchanged between the readout/power supply unit and the transducer assemblies could be infrared transmissions rather than RF transmissions. Such improvements, changes and modifications within the skill of the art are intended to be covered by the appended claims.

Having described the invention, we claim:

1. An apparatus for providing an in vivo assessment of loads on adjacent bones, said apparatus comprising:

a body for insertion between the adjacent bones;

at least one sensor associated with said body, said at least one sensor for generating an output signal in response to and indicative of a load being applied to said body through the adjacent bones; and

at least one telemetric device operatively coupled with said at least one sensor, said at least one telemetric device being operable to receive said output signal from said at least one sensor and to transmit an EMF signal dependent upon said output signal.

2. The apparatus of claim 1 wherein said body comprises an implant for helping the adjacent bones to fuse together.

3. The apparatus of claim 2 wherein said implant comprises a fusion cage for insertion between an adjacent pair of vertebrae, said fusion cage having an interior chamber for receiving bone graft material.

4. The apparatus of claim 1 wherein said body comprises a bone graft.

5. The apparatus of claim 1 wherein said at least one sensor comprises a pressure sensor.

6. The apparatus of claim 1 wherein said at least one sensor further comprises a load cell.

7. The apparatus of claim 1 further comprising an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together.

8. The apparatus of claim 7 further comprising at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to a load being applied to said implant, said at least one strain gauge being electrically connected with said at least one telemetric device.

9. The apparatus of claim 1 wherein said body comprises a prosthetic device for preserving motion between adjacent bones.

10. An apparatus for providing an in vivo assessment of loads on adjacent bones to be fused together, said apparatus comprising:

a graft for insertion between the adjacent bones;

at least one sensor associated with said graft, said at least one sensor for generating an output signal in response to and indicative of a load being applied to said graft through the adjacent bones; and

at least one telemetric device operatively coupled with said at least one sensor, said at least one telemetric device being operable to receive said output signal from said at least one sensor and to transmit an EMF signal dependent upon said output signal.

11. The apparatus of claim 10 further comprising an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together.

12. The apparatus of claim 10 wherein said at least one sensor comprises a pressure sensor.

13. The apparatus of claim 12 further comprising an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together.

14. The apparatus of claim 13 further comprising at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to a load being applied to said implant, said at least one strain gauge being electrically connected with said at least one telemetric device.

15. The apparatus of claim 12 wherein said at least one sensor further comprises a load cell.

16. The apparatus of claim 15 further comprising an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together.

17. The apparatus of claim 15 further comprising at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to and indicative of a load being applied to said implant, said at least one strain gauge being electrically connected with said at least one telemetric device.

18. The apparatus of claim 10 wherein said at least one sensor comprises a load cell.

19. The apparatus of claim 18 further comprising an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together.

20. The apparatus of claim 19 further comprising at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to and indicative of a load being applied to said implant, said at least one strain gauge being electrically connected with said at least one telemetric device.

21. An apparatus for providing an in vivo assessment of loads on adjacent vertebrae to be fused together, the adjacent vertebrae being separated by an intervertebral space created by the removal of an intervertebral disc, said apparatus comprising:

a bone graft for insertion into the intervertebral space;

at least one sensor associated with said bone graft, said at least one sensor for generating an output signal in response to and indicative of a load being applied to said bone graft through the adjacent pair of vertebrae; and

at least one telemetric device operatively coupled with said at least one sensor, said at least one telemetric device being operable to receive said output signal from said at least one sensor and to transmit an EMF signal dependent upon said output signal.

22. The apparatus of claim 21 wherein said at least one sensor comprises a pressure sensor.

23. The apparatus of claim 22 wherein said pressure sensor is positioned in an interior portion of said bone graft.

24. The apparatus of claim 22 wherein said at least one sensor further comprises at least one load cell.

25. The apparatus of claim 24 wherein said at least one load cell is countersunk into a surface of said bone graft that faces one of the adjacent bones.

26. The apparatus of claim 21 wherein said at least one sensor comprises at least one load cell.

27. The apparatus of claim 19 further comprising:

an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together; and

at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to and indicative of a load being applied to said implant, said at least one strain gauge being electrically connected with said at least one telemetric device.

28. The apparatus of claim 27 wherein said at least one telemetric device is mounted on said implant and operatively coupled to said at least one sensor.

29. The apparatus of claim 27 wherein said at least one telemetric device and said at least one sensor are formed on a silicon substrate and secured within said bone graft, said at least one telemetric device being operatively coupled to said at least one strain gauge.

30. An apparatus for providing an in vivo assessment of loads on adjacent bones to be fused together, said apparatus comprising:

a bone graft for insertion between the adjacent bones;

a pressure sensor associated with said bone graft, said pressure sensor for generating a first output signal in response to and indicative of a load being applied to said bone graft through the adjacent bones; and

a load cell associated with said bone graft, said load cell for generating a second output signal in response to and indicative of the load being applied to said bone graft through the adjacent bones.

31. The apparatus of claim 30 wherein said pressure sensor is positioned in an interior portion of said bone graft.

32. The apparatus of claim 30 wherein said pressure sensor is coated with a film of biomolecules to protect said pressure sensor.

33. The apparatus of claim 30 wherein said pressure sensor is coated with monolayers of biomolecules to protect said pressure sensor.

34. The apparatus of claim 30 wherein said pressure sensor is coated with thin layers of biocompatible materials to protect said pressure sensor.

35. The apparatus of claim 30 wherein said load cell is countersunk into a surface of said bone graft that faces one of the adjacent bones.

36. The apparatus of claim 30 wherein said load cell is coated with a film of biomolecules to protect said load cell.

37. The apparatus of claim 30 wherein said load cell is coated with monolayers of biomolecules to protect said load cell.

38. The apparatus of claim 30 wherein said load cell is coated with thin layers of biocompatible materials to protect said load cell.

39. The apparatus of claim 30 further comprising at least one telemetric device operatively coupled with said pressure sensor and with said load cell, said at least one telemetric device being operable to receive said first and second output signals and to transmit EMF signals dependent upon said output signals.

40. The apparatus of claim 39 further comprising:

an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones fuse together; and

at least one strain gauge mounted on said implant, said at least one strain gauge for generating a third output signal in response to and indicative of the load being

applied to said implant, said at least one strain gauge being operatively coupled with said at least one telemetric device.

41. An apparatus for providing an in vivo assessment of loads on adjacent bones to be fused together, said apparatus comprising:

- a graft for insertion between the adjacent bones;
- at least one sensor associated with said graft, said at least one sensor for generating a first output signal in response to and indicative of a load being applied to said graft;
- an implant connected with the adjacent bones for helping to stabilize the adjacent bones while the adjacent bones are fusing together; and
- at least one strain gauge mounted on said implant, said at least one strain gauge for generating a second output signal in response to and indicative of the load being applied to said implant.

42. The apparatus of claim 41 wherein said at least one sensor comprises a pressure sensor.

43. The apparatus of claim 41 wherein said at least one sensor further comprises a load cell.

44. The apparatus of claim 41 wherein said implant includes a platform and at least one rod, said at least one strain gauge being mounted to one of said platform and said at least one rod.

45. The apparatus of claim 41 further comprising at least one telemetric device operatively coupled with said at least one sensor and with said at least one strain gauge, said at least one telemetric device being operable to receive said first and second output signals and to transmit EMF signals dependent upon said output signals percutaneously.

46. The apparatus of claim 45 further comprising an external monitoring unit for receiving said EMF signals transmitted percutaneously.

47. An apparatus for providing an in vivo assessment of loads on adjacent bones to be fused together, said apparatus comprising:

- a body for insertion between the adjacent bones;
- sensor means for sensing a load being applied to said body through the adjacent bones and for generating a corresponding output signal in response to and indicative of a sensed load; and
- first circuit means operatively coupled with said sensor means for receiving said output signal from said sensor means, said first circuit means including antenna means for receiving energy to power said first circuit means and said sensor means and for transmitting an EMF signal dependent upon said output signal.

48. The apparatus of claim 47 wherein said first circuit means includes signal processing means and telemetry means.

49. The apparatus of claim 47 wherein said first circuit means further includes an RF-DC converter/modulator and a voltage regulator operatively coupled between said antenna means and said at least one sensor, said RF-DC converter/modulator and said voltage regulator providing electrical energy received by said antenna means to said at least one sensor.

50. The apparatus of claim 49 wherein said first circuit means further includes a microprocessor operatively

coupled between said at least one sensor and said RF-DC converter/modulator, said microprocessor and said RF-DC converter/modulator receiving said output signal from said at least one sensor and converting said output signal into said EMF signal for percutaneous transmission via said antenna means.

51. The apparatus of claim 47 further comprising second circuit means for transmitting energy to power said first circuit means and said sensor means and for receiving said data signal, said second means being disposed remote from said first circuit means.

52. An apparatus for providing an in vivo assessment of loads on and motion of one or more bones, said apparatus comprising:

- a member for placement adjacent a bone;
- at least one sensor associated with said member, said at least one sensor for generating an output signal in response to and indicative of a load being applied to said member through the bone; and

at least one telemetric device operatively coupled with said at least one sensor, said at least one telemetric device being operable to receive said output signal from said at least one sensor and to transmit an EMF signal dependent upon said output signal.

53. The apparatus of claim 52 wherein said member comprises an implant for helping adjacent bones fuse together.

54. The apparatus of claim 53 wherein said implant comprises a fusion cage for insertion between an adjacent pair of vertebrae.

55. The apparatus of claim 52 wherein said member comprises a bone graft.

56. The apparatus of claim 52 wherein said member comprises a prosthetic device for preserving motion between adjacent bones.

57. The apparatus of claim 56 wherein said prosthetic device comprises an artificial disc.

58. An apparatus for providing an in vivo assessment of loads on and motion of one or more bones, said apparatus comprising:

- at least one sensor attached to a bone, said at least one sensor for generating an output signal in response to and indicative of a load on the bone; and
- at least one telemetric device operatively coupled with said at least one sensor, said at least one telemetric device being operable to receive said output signal from said at least one sensor and to transmit an EMF signal dependent upon said output signal.

59. The apparatus of claim 58 wherein said at least one sensor comprises a pressure sensor.

60. The apparatus of claim 59 wherein said pressure sensor is positioned in an interior portion of a vertebrae.

61. A method for in vivo assessing the loads on adjacent vertebrae to be fused together, said method comprising the steps of:

- harvesting a bone graft;
- removing an intervertebral disc between the adjacent vertebrae;

instrumenting the bone graft with at least one sensor for sensing a load on the bone graft and for generating an output signal indicative of a sensed load;

operatively coupling at least one telemetric device with the at least one sensor to receive the output signal and to transmit an EMF signal dependent upon the output signal;

implanting the bone graft between the adjacent vertebrae; and

monitoring the EMF signal from the least one telemetric device.

62. The method of claim 61 further wherein said step of instrumenting the bone graft with at least one sensor comprises securing a pressure sensor to the bone graft.

63. The method of claim 61 further comprising the step of coating the pressure sensor with thin layers of a biocompatible material.

64. The method of claim 61 further comprising the step of coating the pressure sensor with monolayers of biomolecules.

65. The method of claim 61 further comprising the step of coating the pressure sensor with a film of biomolecules.

66. The method of claim 61 further wherein said step of instrumenting the bone graft with at least one sensor further comprises securing a load cell to the bone graft.

67. The method of claim 66 further comprising the step of coating the load cell with thin layers of a biocompatible material.

68. The method of claim 66 further comprising the step of coating the load cell with monolayers of biomolecules.

69. The method of claim 66 further comprising the step of coating the load cell with a film of biomolecules.

70. The method of claim 61 further comprising the step of attaching an implant to the adjacent vertebrae to help stabilize the vertebrae while fusing together.

71. The method of claim 70 further comprising the steps of:

mounting at least one strain gauge to the implant; and

operatively coupling the at least one strain gauge to the least one telemetric device.

72. The method of claim 61 further comprising the step of inductively energizing the at least one sensor and the least one telemetric device.

73. A method for in vivo assessing the loads on adjacent bones to be fused together, said method comprising the steps of:

providing a body for insertion between the adjacent bones;

instrumenting the body with at least one sensor for sensing a load on the body and for generating an output signal indicative of a sensed load;

operatively coupling at least one telemetric device with the at least one sensor to receive the output signal and to transmit an EMF signal dependent upon the output signal;

implanting the body between the adjacent bones; and

monitoring the EMF signal from the least one telemetric device.

74. The method of claim 73 wherein said step of providing a body comprises providing a prosthetic implant for helping the adjacent bones to fuse together.

75. The method of claim 74 further comprising the step of filling the interior of the prosthetic implant with bone graft material following implantation of the prosthetic implant.

76. The method of claim 73 wherein said step of providing a body comprises harvesting a bone graft.

77. A method for in vivo assessing of loads on and motion of one or more bones, said method comprising the steps of:

providing a member for placement adjacent a bone;

instrumenting the member with at least one sensor for generating an output signal in response to and indicative of a load being applied to the member through the bone;

operatively coupling at least one telemetric device with the at least one sensor to receive the output signal from the at least one sensor and to transmit an EMF signal dependent upon the output signal;

inserting the member adjacent the bone; and

monitoring the EMF signal from the least one telemetric device.

* * * * *

专利名称(译)	用于评估相邻骨骼上的负载的装置和方法		
公开(公告)号	US20020049394A1	公开(公告)日	2002-04-25
申请号	US09/939331	申请日	2001-08-24
[标]申请(专利权)人(译)	克里夫兰诊所基金会		
申请(专利权)人(译)	克利夫兰诊所基金会		
当前申请(专利权)人(译)	克利夫兰诊所基金会，		
[标]发明人	ROY SHUVO FLEISCHMAN AARON J BENZEL EDWARD C FERRARA LISA		
发明人	ROY, SHUVO FLEISCHMAN, AARON J. BENZEL, EDWARD C. FERRARA, LISA		
IPC分类号	A61B5/00 A61B5/03 A61B5/103 A61B17/70 A61F2/02 A61F2/28 A61F2/30 A61F2/44 A61F2/46		
CPC分类号	A61B5/0031 A61F2250/0002 A61B5/4504 A61B17/7044 A61B2562/0247 A61B2562/0261 A61B2562/028 A61F2/30744 A61F2/442 A61F2/446 A61F2002/2835 A61F2002/30563 A61F2002/3067 A61F2002/30772 A61F2002/3085 A61F2002/4666 A61B5/036		
优先权	60/228166 2000-08-25 US		
其他公开文献	US6706005		
外部链接	Espacenet USPTO		

摘要(译)

利用微机电系统 (MEMS) 技术来提供相邻骨骼 (24和26) 上的负载的体内评估的装置 (10) 包括用于插入相邻骨骼之间的主体 (34) 。至少一个传感器 (42) 与主体 (34) 相关联。传感器 (42) 响应于并指示通过相邻骨 (24和26) 施加到主体 (34) 的负载而产生输出信号。遥测设备 (40) 可操作地与传感器 (42) 耦合。遥测设备 (40) 可操作以接收来自传感器 (42) 的输出信号并根据输出信号发送EMF信号。根据本发明的各个方面，传感器包括压力传感器 (42) ，测力传感器 (320) 和/或至少一个应变仪 (142) 。

