



US008515509B2

(12) **United States Patent**
Bruinsma et al.

(10) **Patent No.:** **US 8,515,509 B2**
(45) **Date of Patent:** **Aug. 20, 2013**

(54) **MULTI-STREAM EMITTER FOR
NONINVASIVE MEASUREMENT OF BLOOD
CONSTITUENTS**

(75) Inventors: **Johannes Bruinsma**, Mission Viejo, CA (US); **Marcelo Lamego**, Coto De Caza, CA (US); **Sean Merritt**, Lake Forest, CA (US); **Cristiano Dalvi**, Mission Viejo, CA (US); **Hung Vo**, Garden Grove, CA (US); **Jeroen Poeze**, Mission Viejo, CA (US); **Ferdyan Lesmana**, Irvine, CA (US); **Massi Joe E. Kiani**, Laguna Niguel, CA (US)

(73) Assignee: **Cercacor Laboratories, Inc.**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 792 days.

(21) Appl. No.: **12/534,825**

(22) Filed: **Aug. 3, 2009**

(65) **Prior Publication Data**

US 2010/0030041 A1 Feb. 4, 2010

Related U.S. Application Data

(60) Provisional application No. 61/086,060, filed on Aug. 4, 2008, provisional application No. 61/086,108, filed on Aug. 4, 2008, provisional application No. 61/086,063, filed on Aug. 4, 2008, provisional application No. 61/086,057, filed on Aug. 4, 2008, provisional application No. 61/091,732, filed on Aug. 25, 2008.

(51) **Int. Cl.**
A61B 5/00 (2006.01)

(52) **U.S. Cl.**
USPC 600/322

(58) **Field of Classification Search**
USPC 600/322
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,114,604 A 9/1978 Shaw et al.
4,258,719 A 3/1981 Lewyn

(Continued)

FOREIGN PATENT DOCUMENTS

EP 419223 3/1991
WO WO93/12712 7/1993
WO WO 00/25112 5/2000

OTHER PUBLICATIONS

International Search Report and Written Opinion for PCT/US2009/049638, mailed Jan. 7, 2010.

(Continued)

Primary Examiner — Clayton E LaBalle


Assistant Examiner — Dennis Hancock

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson & Bear, LLP

(57) **ABSTRACT**

The present disclosure relates to an emitter that is suitable for a noninvasive blood constituent sensor. The emitter is configured as a point optical source that comprises a plurality of LEDs that emit a sequence of pulses of optical radiation across a spectrum of wavelengths. In some embodiments, the plurality of sets of optical sources may each comprise at least one top-emitting LED and at least one super luminescent LED. In some embodiments, the emitter comprises optical sources that transmit optical radiation in the infrared or near-infrared wavelengths suitable for detecting glucose. In order to achieve the desired SNR for detecting analytes like glucose, the emitter may be driven using a progression from low power to higher power. In addition, the emitter may have its duty cycle modified to achieve a desired SNR.

36 Claims, 65 Drawing Sheets

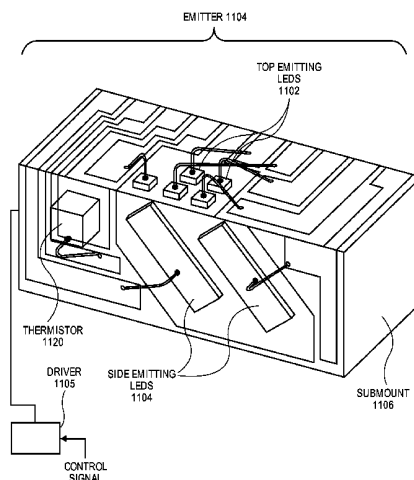

(56)

References Cited

U.S. PATENT DOCUMENTS

4,267,844 A	5/1981	Yamanishi	
4,444,471 A	4/1984	Ford et al.	
4,655,225 A *	4/1987	Dahne et al.	600/316
4,755,676 A	7/1988	Gaalema et al.	
4,781,195 A	11/1988	Martin	
4,805,623 A	2/1989	Jöbssis	
4,880,304 A	11/1989	Jaeb et al.	
4,960,128 A	10/1990	Gordon et al.	
4,964,408 A	10/1990	Hink et al.	
5,028,787 A	7/1991	Rosenthal et al.	
5,035,243 A	7/1991	Muz	
5,041,187 A	8/1991	Hink et al.	
5,069,213 A	12/1991	Polczynski	
5,069,214 A	12/1991	Samaras et al.	
5,077,476 A	12/1991	Rosenthal	
D326,715 S	6/1992	Schmidt	
5,131,391 A	7/1992	Sakai et al.	
5,137,023 A	8/1992	Mendelson et al.	
5,163,438 A	11/1992	Gordon et al.	
5,222,496 A	6/1993	Clarke et al.	
5,249,576 A	10/1993	Goldberger et al.	
5,278,627 A	1/1994	Aoyagi et al.	
5,297,548 A	3/1994	Pologe	
5,319,355 A	6/1994	Russek	
5,337,744 A	8/1994	Branigan	
5,337,745 A	8/1994	Benaron	
5,341,805 A	8/1994	Stavridi et al.	
5,362,966 A	11/1994	Rosenthal et al.	
D353,195 S	12/1994	Savage et al.	
D353,196 S	12/1994	Savage et al.	
5,377,676 A	1/1995	Vari et al.	
D356,870 S	3/1995	Ivers et al.	
D359,546 S	6/1995	Savage et al.	
5,431,170 A	7/1995	Mathews	
D361,840 S	8/1995	Savage et al.	
5,437,275 A	8/1995	Amundsen et al.	
5,441,054 A	8/1995	Tsuchiya	
D362,063 S	9/1995	Savage et al.	
5,452,717 A	9/1995	Branigan et al.	
D363,120 S	10/1995	Savage et al.	
5,456,252 A	10/1995	Vari et al.	
5,479,934 A	1/1996	Imran	
5,482,034 A	1/1996	Lewis et al.	
5,482,036 A	1/1996	Diab et al.	
5,490,505 A	2/1996	Diab et al.	
5,494,043 A	2/1996	O'Sullivan et al.	
5,511,546 A	4/1996	Hon	
5,533,511 A	7/1996	Kaspari et al.	
5,534,851 A	7/1996	Russek	
5,553,615 A	9/1996	Carim et al.	
5,553,616 A *	9/1996	Ham et al.	600/316
5,561,275 A	10/1996	Savage et al.	
5,562,002 A	10/1996	Lalin	
5,590,649 A	1/1997	Caro et al.	
5,602,924 A	2/1997	Durand et al.	
D378,414 S	3/1997	Allen et al.	
5,632,272 A	5/1997	Diab et al.	
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	
5,638,818 A	6/1997	Diab et al.	
5,645,440 A	7/1997	Tobler et al.	
5,676,143 A	10/1997	Simonsen et al.	
5,685,299 A	11/1997	Diab et al.	
D390,666 S	2/1998	Lagerlof	
D393,830 S	4/1998	Tobler et al.	
5,743,262 A	4/1998	Lepper, Jr. et al.	
5,750,927 A	5/1998	Baltazar	
5,752,914 A	5/1998	Delonzor et al.	
5,758,644 A	6/1998	Diab et al.	
5,760,910 A	6/1998	Lepper, Jr. et al.	
5,769,785 A	6/1998	Diab et al.	
5,782,757 A	7/1998	Diab et al.	
5,785,659 A	7/1998	Caro et al.	
5,791,347 A	8/1998	Flaherty et al.	
5,792,052 A	8/1998	Isaacson et al.	
5,810,734 A	9/1998	Caro et al.	
5,823,950 A	10/1998	Diab et al.	
5,826,885 A	10/1998	Helgeland	
5,830,131 A	11/1998	Caro et al.	
5,833,618 A	11/1998	Caro et al.	
D403,070 S	12/1998	Maeda et al.	
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	
5,890,929 A	4/1999	Mills et al.	
5,902,235 A	5/1999	Lewis et al.	
5,904,654 A	5/1999	Wohltmann et al.	
5,919,134 A	7/1999	Diab	
5,934,925 A	8/1999	Tobler et al.	
5,940,182 A	8/1999	Lepper, Jr. et al.	
D414,870 S	10/1999	Saltzstein et al.	
5,995,855 A	11/1999	Kiani et al.	
5,997,343 A	12/1999	Mills et al.	
6,002,952 A	12/1999	Diab et al.	
6,011,986 A	1/2000	Diab et al.	
6,027,452 A	2/2000	Flaherty et al.	
6,036,642 A	3/2000	Diab et al.	
6,045,509 A	4/2000	Caro et al.	
6,049,727 A *	4/2000	Crothall	600/310
6,067,462 A	5/2000	Diab et al.	
6,081,735 A	6/2000	Diab et al.	
6,088,607 A	7/2000	Diab et al.	
6,110,522 A	8/2000	Lepper, Jr. et al.	
6,124,597 A	9/2000	Shehada	
6,128,521 A	10/2000	Marro et al.	
6,129,675 A	10/2000	Jay	
6,144,866 A	11/2000	Miesel et al.	
6,144,868 A	11/2000	Parker	
6,151,516 A	11/2000	Kiani-Azarbayjany et al.	
6,152,754 A	11/2000	Gerhardt et al.	
6,157,850 A	12/2000	Diab et al.	
6,165,005 A	12/2000	Mills et al.	
6,172,743 B1	1/2001	Kley et al.	
6,181,958 B1	1/2001	Steuer et al.	
6,184,521 B1	2/2001	Coffin, IV et al.	
6,206,830 B1	3/2001	Diab et al.	
6,223,063 B1	4/2001	Chaiken et al.	
6,229,856 B1	5/2001	Diab et al.	
6,232,609 B1	5/2001	Snyder et al.	
6,236,872 B1	5/2001	Diab et al.	
6,241,683 B1	6/2001	Macklem et al.	
6,253,097 B1	6/2001	Aronow et al.	
6,256,523 B1	7/2001	Diab et al.	
6,263,222 B1	7/2001	Diab et al.	
6,278,522 B1	8/2001	Lepper, Jr. et al.	
6,278,889 B1 *	8/2001	Robinson	600/322
6,280,213 B1	8/2001	Tobler et al.	
6,285,896 B1	9/2001	Tobler et al.	
6,301,493 B1	10/2001	Marro et al.	
6,317,627 B1	11/2001	Ennen et al.	
6,321,100 B1	11/2001	Parker	
D452,012 S	12/2001	Phillips	
6,334,065 B1	12/2001	Al-Ali et al.	
6,343,224 B1	1/2002	Parker	
6,345,194 B1	2/2002	Nelson et al.	
6,349,228 B1	2/2002	Kiani et al.	
6,353,750 B1	3/2002	Kimura et al.	
6,360,113 B1	3/2002	Dettling	
6,360,114 B1	3/2002	Diab et al.	
6,360,115 B1	3/2002	Greenwald et al.	
D455,834 S	4/2002	Donars et al.	
6,368,283 B1	4/2002	Xu et al.	
6,371,921 B1	4/2002	Caro et al.	
6,377,829 B1	4/2002	Al-Ali	
6,388,240 B2	5/2002	Schulz et al.	
6,397,091 B2	5/2002	Diab et al.	
6,430,437 B1	8/2002	Marro	
6,430,525 B1	8/2002	Weber et al.	
D463,561 S	9/2002	Fukatsu et al.	
6,463,311 B1	10/2002	Diab	
6,470,199 B1	10/2002	Kopotic et al.	
6,501,975 B2	12/2002	Diab et al.	
6,505,059 B1	1/2003	Kollias et al.	
6,515,273 B2	2/2003	Al-Ali	
6,519,487 B1	2/2003	Parker	
6,525,386 B1	2/2003	Mills et al.	
6,526,300 B1	2/2003	Kiani et al.	

6,541,756	B2	4/2003	Schulz et al.	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,542,764	B1	4/2003	Al-Ali et al.	7,132,641	B2	11/2006	Schulz et al.
6,580,086	B1	6/2003	Schulz et al.	7,142,901	B2	11/2006	Kiani et al.
6,584,336	B1	6/2003	Ali et al.	7,149,561	B2	12/2006	Diab
6,595,316	B2	7/2003	Cybulski et al.	D535,031	S	1/2007	Barrett et al.
6,597,932	B2	7/2003	Tian et al.	D537,164	S	2/2007	Shigemori et al.
6,597,933	B2	7/2003	Kiani et al.	7,186,966	B2	3/2007	Al-Ali
6,606,509	B2	8/2003	Schmitt	7,190,261	B2	3/2007	Al-Ali
6,606,511	B1	8/2003	Ali et al.	7,215,984	B2	5/2007	Diab
D481,459	S	10/2003	Nahm	7,215,986	B2	5/2007	Diab
6,632,181	B2	10/2003	Flaherty et al.	7,221,971	B2	5/2007	Diab
6,636,759	B2	10/2003	Robinson	7,225,006	B2	5/2007	Al-Ali et al.
6,639,668	B1	10/2003	Trepagnier	7,225,007	B2	5/2007	Al-Ali
6,640,116	B2	10/2003	Diab	RE39,672	E	6/2007	Shehada et al.
6,643,530	B2	11/2003	Diab et al.	D547,454	S	7/2007	Hsieh
6,650,917	B2	11/2003	Diab et al.	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,654,624	B2	11/2003	Diab et al.	7,245,953	B1	7/2007	Parker
6,658,276	B2	12/2003	Kianl et al.	D549,830	S	8/2007	Behar et al.
6,661,161	B1	12/2003	Lanzo et al.	7,254,429	B2	8/2007	Schurman et al.
6,671,531	B2	12/2003	Al-Ali et al.	7,254,431	B2	8/2007	Al-Ali
6,678,543	B2	1/2004	Diab et al.	7,254,433	B2	8/2007	Diab et al.
6,684,090	B2	1/2004	Ali et al.	7,254,434	B2	8/2007	Schulz et al.
6,684,091	B2	1/2004	Parker	D550,364	S	9/2007	Glover et al.
6,697,656	B1	2/2004	Al-Ali	D551,350	S	9/2007	Lorimer et al.
6,697,657	B1	2/2004	Shehada et al.	7,272,425	B2	9/2007	Al-Ali
6,697,658	B2	2/2004	Al-Ali	7,274,955	B2	9/2007	Kiani et al.
RE38,476	E	3/2004	Diab et al.	D553,248	S	10/2007	Nguyen
6,699,194	B1	3/2004	Diab et al.	D554,263	S	10/2007	Al-Ali
6,714,804	B2	3/2004	Al-Ali et al.	7,280,858	B2	10/2007	Al-Ali et al.
RE38,492	E	4/2004	Diab et al.	7,289,835	B2	10/2007	Mansfield et al.
6,721,582	B2	4/2004	Trepagnier et al.	7,292,883	B2	11/2007	De Felice et al.
6,721,585	B1	4/2004	Parker	7,295,866	B2	11/2007	Al-Ali
6,725,075	B2	4/2004	Al-Ali	D562,985	S	2/2008	Brefka et al.
6,728,560	B2	4/2004	Kollias et al.	7,328,053	B1	2/2008	Diab et al.
6,735,459	B2	5/2004	Parker	7,332,784	B2	2/2008	Mills et al.
6,745,060	B2	6/2004	Diab et al.	7,340,287	B2	3/2008	Mason et al.
6,760,607	B2	7/2004	Al-Ali	7,341,559	B2	3/2008	Schulz et al.
6,770,028	B1	8/2004	Ali et al.	7,343,186	B2	3/2008	Lamego et al.
6,771,994	B2	8/2004	Kiani et al.	D566,282	S	4/2008	Al-Ali et al.
6,792,300	B1	9/2004	Diab et al.	D567,125	S	4/2008	Okabe et al.
6,813,511	B2	11/2004	Diab et al.	7,355,512	B1	4/2008	Al-Ali
6,816,241	B2	11/2004	Grubisic	7,356,365	B2	4/2008	Schurman
6,816,741	B2	11/2004	Diab	D569,001	S	5/2008	Omaki
6,822,564	B2	11/2004	Al-Ali	D569,521	S	5/2008	Omaki
6,826,419	B2	11/2004	Diab et al.	7,371,981	B2	5/2008	Abdul-Hafiz
6,830,711	B2	12/2004	Mills et al.	7,373,193	B2	5/2008	Al-Ali et al.
6,850,787	B2	2/2005	Weber et al.	7,373,194	B2	5/2008	Weber et al.
6,850,788	B2	2/2005	Al-Ali	7,376,453	B1	5/2008	Diab et al.
6,852,083	B2	2/2005	Caro et al.	7,377,794	B2	5/2008	Al-Ali et al.
D502,655	S	3/2005	Huang	7,377,899	B2	5/2008	Weber et al.
6,861,639	B2	3/2005	Al-Ali	7,383,070	B2	6/2008	Diab et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,415,297	B2	8/2008	Al-Ali et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,428,432	B2	9/2008	Ali et al.
D508,862	S	8/2005	Behar et al.	7,438,683	B2	10/2008	Al-Ali et al.
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,440,787	B2	10/2008	Diab
6,934,570	B2	8/2005	Kiani et al.	7,454,240	B2	11/2008	Diab et al.
6,939,305	B2	9/2005	Flaherty et al.	7,467,002	B2	12/2008	Weber et al.
6,943,348	B1	9/2005	Coffin, IV	7,469,157	B2	12/2008	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,471,969	B2	12/2008	Diab et al.
D510,625	S	10/2005	Widener et al.	7,471,971	B2	12/2008	Diab et al.
6,961,598	B2	11/2005	Diab	7,483,729	B2	1/2009	Al-Ali et al.
6,970,792	B1	11/2005	Diab	7,483,730	B2	1/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	7,489,958	B2	2/2009	Diab et al.
6,985,764	B2	1/2006	Mason et al.	7,496,391	B2	2/2009	Diab et al.
6,993,371	B2	1/2006	Kiani et al.	7,496,393	B2	2/2009	Diab et al.
D514,461	S	2/2006	Harju	D587,657	S	3/2009	Al-Ali et al.
6,996,427	B2	2/2006	Ali et al.	7,499,741	B2	3/2009	Diab et al.
6,999,904	B2	2/2006	Weber et al.	7,499,835	B2	3/2009	Weber et al.
7,003,338	B2	2/2006	Weber et al.	7,500,950	B2	3/2009	Al-Ali et al.
7,003,339	B2	2/2006	Diab et al.	7,509,154	B2	3/2009	Diab et al.
7,015,451	B2	3/2006	Dalke et al.	7,509,494	B2	3/2009	Al-Ali
7,024,233	B2	4/2006	Ali et al.	7,510,849	B2	3/2009	Schurman et al.
7,027,849	B2	4/2006	Al-Ali	7,526,328	B2	4/2009	Diab et al.
7,030,749	B2	4/2006	Al-Ali	7,530,942	B1	5/2009	Diab
7,039,449	B2	5/2006	Al-Ali	7,530,949	B2	5/2009	Al Ali et al.
7,041,060	B2	5/2006	Flaherty et al.	7,530,955	B2	5/2009	Diab et al.
7,044,918	B2	5/2006	Diab	7,563,110	B2	7/2009	Al-Ali et al.
7,067,893	B2	6/2006	Mills et al.	7,596,398	B2	9/2009	Al-Ali et al.
7,096,052	B2	8/2006	Mason et al.	7,606,606	B2	10/2009	Laakkonen

D603,966 S	11/2009	Jones et al.	2002/0091322 A1 *	7/2002	Chaiken et al.	600/476
7,618,375 B2	11/2009	Flaherty	2002/0115918 A1 *	8/2002	Crowley	600/310
D606,659 S	12/2009	Kiani et al.	2004/0039272 A1	2/2004	Abdul-Hafiz et al.	
7,647,083 B2	1/2010	Al-Ali et al.	2004/0049237 A1	3/2004	Larson et al.	
D609,193 S	2/2010	Al-Ali et al.	2004/0054269 A1 *	3/2004	Rantala et al.	600/322
7,657,294 B2	2/2010	Eghbal et al.	2004/0054291 A1	3/2004	Schulz et al.	
7,657,295 B2	2/2010	Coakley et al.	2005/0162761 A1	7/2005	Hargis et al.	
7,657,296 B2	2/2010	Raridan et al.	2006/0167347 A1 *	7/2006	Xu et al.	600/310
D614,305 S	4/2010	Al-Ali et al.	2006/0189859 A1	8/2006	Kiani et al.	
RE41,317 E	5/2010	Parker	2006/0208191 A1 *	9/2006	Kessler et al.	250/339.13
7,729,733 B2	6/2010	Al-Ali et al.	2006/0211924 A1 *	9/2006	Dalke et al.	600/310
7,734,320 B2	6/2010	Al-Ali	2006/0258922 A1	11/2006	Mason et al.	
7,761,127 B2	7/2010	Al-Ali et al.	2007/0149865 A1	6/2007	Laakkonen	
7,761,128 B2	7/2010	Al-Ali et al.	2007/0165218 A1	7/2007	Qing et al.	
7,764,982 B2	7/2010	Dalke et al.	2007/0197886 A1 *	8/2007	Naganuma et al.	600/322
D621,516 S	8/2010	Kiani et al.	2007/0293792 A1	12/2007	Sliwa et al.	
7,791,155 B2	9/2010	Diab	2008/0036855 A1	2/2008	Heenan	
7,801,581 B2	9/2010	Diab	2008/0071154 A1 *	3/2008	Hausmann et al.	600/323
7,822,452 B2	10/2010	Schurman et al.	2008/0130232 A1	6/2008	Yamamoto	
RE41,912 E	11/2010	Parker	2008/0139908 A1	6/2008	Kurth	
7,844,313 B2	11/2010	Kiani et al.	2008/0208006 A1	8/2008	Farr	
7,844,314 B2	11/2010	Al-Ali	2009/0043180 A1	2/2009	Tschautscher et al.	
7,844,315 B2	11/2010	Al-Ali	2009/0105565 A1	4/2009	Xu	
7,865,222 B2	1/2011	Weber et al.	2009/0163775 A1	6/2009	Barrett et al.	
7,873,497 B2	1/2011	Weber et al.	2009/0259114 A1	10/2009	Johnson et al.	
7,880,606 B2	2/2011	Al-Ali	2010/0004518 A1	1/2010	Vo et al.	
7,880,626 B2	2/2011	Al-Ali et al.	2010/0049018 A1	2/2010	Duffy et al.	
7,891,355 B2	2/2011	Al-Ali et al.	2010/0090118 A1	4/2010	Rozenfeld	
7,894,868 B2	2/2011	Al-Ali et al.				
7,899,507 B2	3/2011	Al-Ali et al.				
7,899,518 B2	3/2011	Trepagnier et al.				
7,904,132 B2	3/2011	Weber et al.				
7,909,772 B2	3/2011	Popov et al.				
7,910,875 B2	3/2011	Al-Ali				
7,919,713 B2	4/2011	Al-Ali et al.				
7,937,128 B2	5/2011	Al-Ali				
7,937,129 B2	5/2011	Mason et al.				
7,937,130 B2	5/2011	Diab et al.				
7,941,199 B2	5/2011	Kiani				
7,951,086 B2	5/2011	Flaherty et al.				
7,957,780 B2	6/2011	Lamego et al.				
7,962,188 B2	6/2011	Kiani et al.				
7,962,190 B1	6/2011	Diab et al.				
7,976,472 B2	7/2011	Kiani				
7,988,637 B2	8/2011	Diab				
7,990,382 B2	8/2011	Kiani				
7,991,446 B2	8/2011	Ali et al.				
8,000,761 B2	8/2011	Al-Ali				
8,008,088 B2	8/2011	Bellott et al.				
RE42,753 E	9/2011	Kiani-Azarbayjany et al.				
8,019,400 B2	9/2011	Diab et al.				
8,028,701 B2	10/2011	Al-Ali et al.				
8,029,765 B2	10/2011	Bellott et al.				
8,036,728 B2	10/2011	Diab et al.				
8,046,040 B2	10/2011	Ali et al.				
8,046,041 B2	10/2011	Diab et al.				
8,046,042 B2	10/2011	Diab et al.				
8,048,040 B2	11/2011	Kiani				
8,050,728 B2	11/2011	Al-Ali et al.				
RE43,169 E	2/2012	Parker				
8,118,620 B2	2/2012	Al-Ali et al.				
8,126,528 B2	2/2012	Diab et al.				
8,128,572 B2	3/2012	Diab et al.				
8,130,105 B2	3/2012	Al-Ali et al.				
8,145,287 B2	3/2012	Diab et al.				
8,150,487 B2	4/2012	Diab et al.				
8,175,672 B2	5/2012	Parker				
8,180,420 B2	5/2012	Diab et al.				
8,182,443 B1	5/2012	Kiani				
8,185,180 B2	5/2012	Diab et al.				
8,190,223 B2	5/2012	Al-Ali et al.				
8,190,227 B2	5/2012	Diab et al.				
8,203,438 B2	6/2012	Kiani et al.				
8,203,704 B2	6/2012	Merritt et al.				
8,224,411 B2	7/2012	Al-Ali et al.				
8,228,181 B2	7/2012	Al-Ali				
8,229,533 B2	7/2012	Diab et al.				
2002/0016536 A1	2/2002	Benni				
2002/0052547 A1	5/2002	Toida				

OTHER PUBLICATIONS

Burritt, Mary F.; Current Analytical Approaches to Measuring Blood Analytes; vol. 36; No. 8(B); 1990.

Hall, et al., Jeffrey W.; Near-Infrared Spectrophotometry: A New Dimension in Clinical Chemistry; vol. 38; No. 9; 1992.

Kuenstner, et al., J. Todd; Measurement of Hemoglobin in Unlysed Blood by Near-Infrared Spectroscopy; vol. 48; No. 4, 1994.

Manzke, et al., B.; Multi Wavelength Pulse Oximetry in the Measurement of Hemoglobin Fractions; vol. 2676.

Naumenko, E. K.; Choice of Wavelengths for Stable Determination of Concentrations of Hemoglobin Derivatives from Absorption Spectra of Erythrocytes; vol. 63; No. 1; pp. 60-66 Jan.-Feb. 1996; Original article submitted Nov. 3, 1994.

Schmitt, Joseph M.; Simple Photon Diffusion Analysis of the Effects of Multiple Scattering on Pulse Oximetry; Mar. 14, 1991; revised Aug. 30, 1991.

Schmitt, et al., Joseph M.; Measurement of Blood Hematocrit by Dual-Wavelength near-IR Photoplethysmography; vol. 1641; 1992.

Schnapp, et al., L.M.; Pulse Oximetry. Uses and Abuses.; Chest 1990; 98; 1244-1250 DOI 10.1378/Chest.98.5.1244.

International Search Report issued in Application No. PCT/US2009/052756, mailed Feb. 10, 2009 in 14 pages.

International Preliminary Report on Patentability and Written Opinion of the International Searching Authority issued in Application No. PCT/US2009/052756, mailed Feb. 8, 2011 in 8 pages.

International Preliminary Report on Patentability and Written Opinion of the International Searching Authority issued in Application No. PCT US2009/049638, mailed Jan. 5, 2011 in 9 pages.

PCT International Search Report, App. No. PCT/US2010/047899, Date of Actual Completion of Search: Jan. 26, 2011, 4 pages.

<http://www.masimo.com/rainbow/pronto.htm> Noninvasive & Immediate Hemoglobin Testing, printed on Aug. 20, 2009.

<http://www.masimo.com/pulseOximeter/Rad5.htm>; Signal Extraction Pulse Oximeter, printed on Aug. 20, 2009.

http://blogderoliveira.blogspot.com/2008_02_01_archive.html; Ricardo Oliveira, printed on Aug. 20, 2009.

<http://www.masimo.com/rad-57/>; Noninvasive Measurement of Methemoglobin, Carboxyhemoglobin and Oxyhemoglobin in the blood. Printed on Aug. 20, 2009.

<http://amivital.ugr.es/blog/?tag=spo2>; Monitorizacion de la hemoglobina . . . y mucho mas, printed on Aug. 20, 2009.


<http://www.masimo.com/spco/>; Carboxyhemoglobin Noninvasive > Continuous > Immediate, printed on Aug. 20, 2009.


<http://www.masimo.com/PARTNERS/WELCHALLYN.htm>; Welch Allyn Expands Patient Monitor Capabilities with Masimo Pulse Oximetry Technology, printed on Aug. 20, 2009.


<http://www.masimo.com/pulseOximeter/PPO.htm>; Masimo Personal Pulse Oximeter, printed on Aug. 20, 2009.
<http://www.masimo.com/generalFloor/system.htm>; Masimo Patient SafetyNet System at a Glance, printed on Aug. 20, 2009.
<http://www.masimo.com/partners/GRASEBY.htm>; Graseby Medical Limited, printed on Aug. 20, 2009.


European Office Action issued in application No. 10763901.5 on Jan. 11, 2013.


* cited by examiner

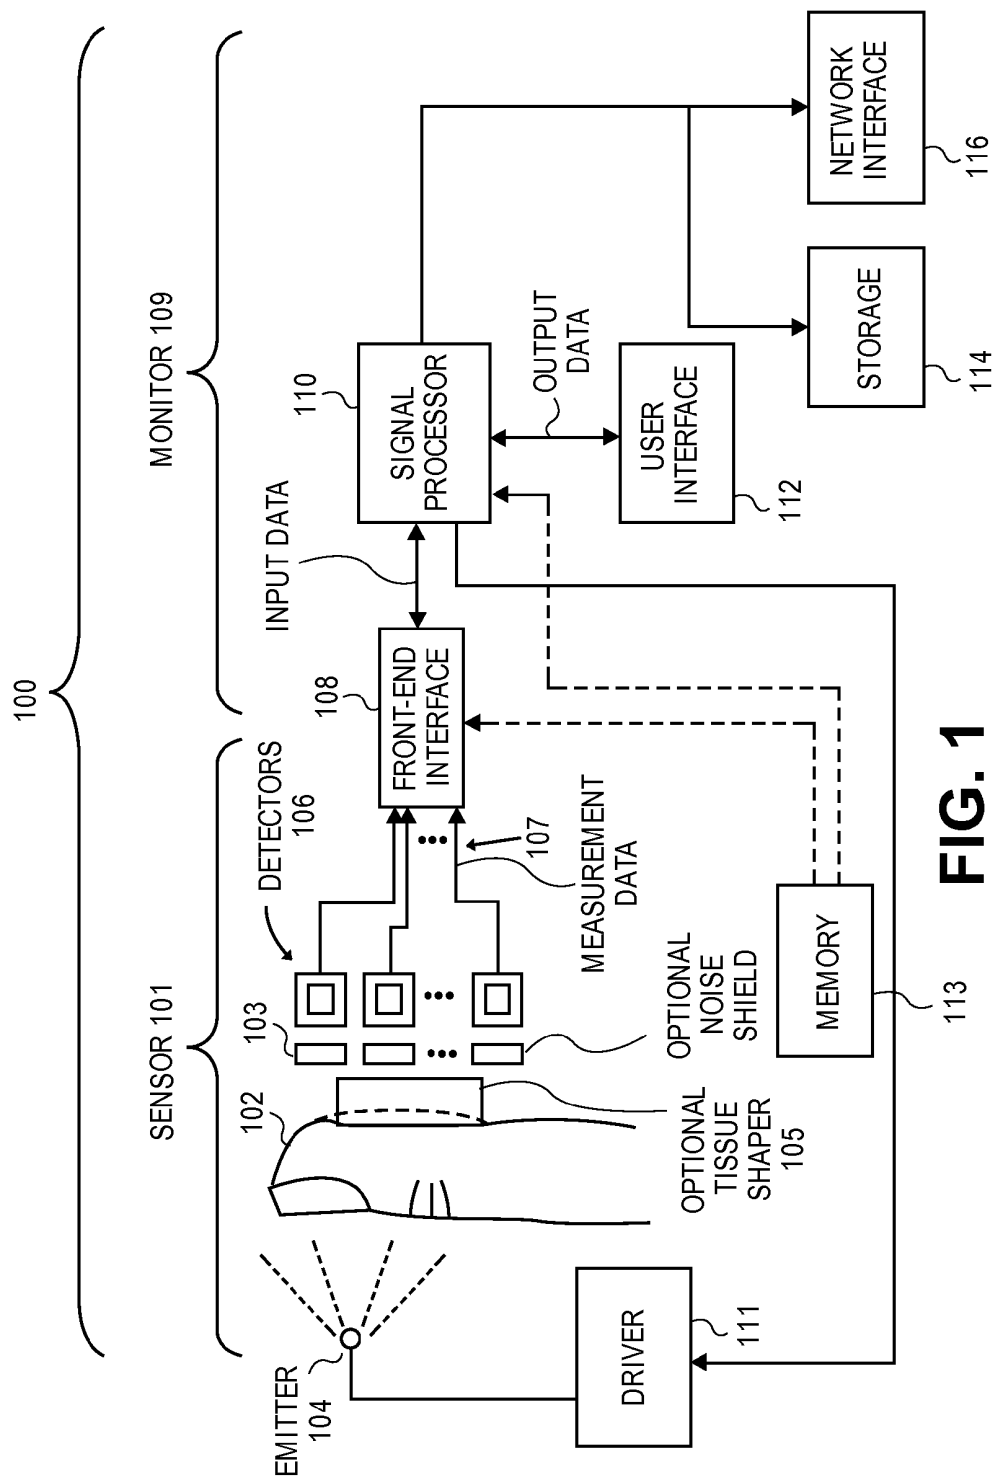**FIG. 1**

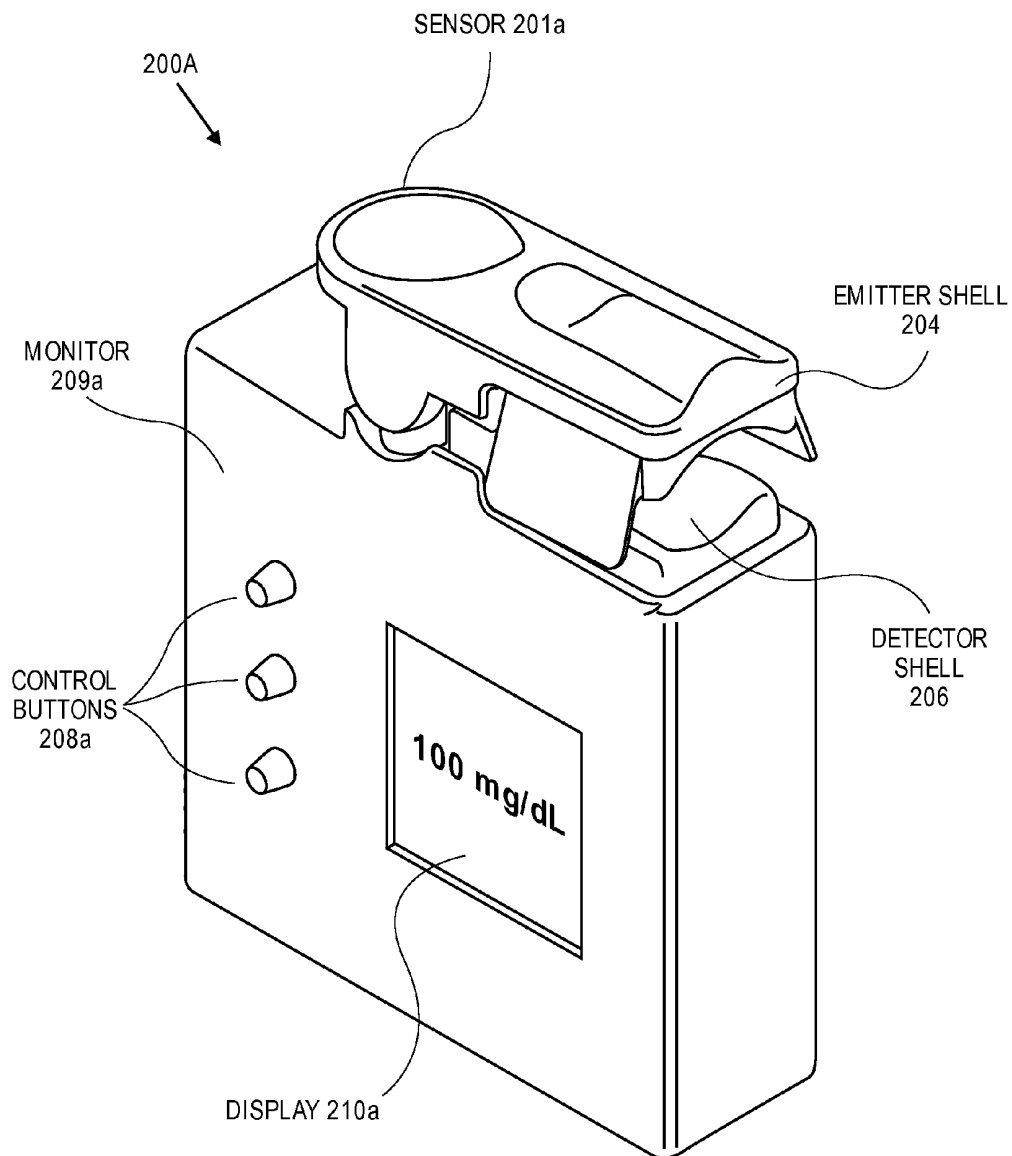**FIG. 2A**

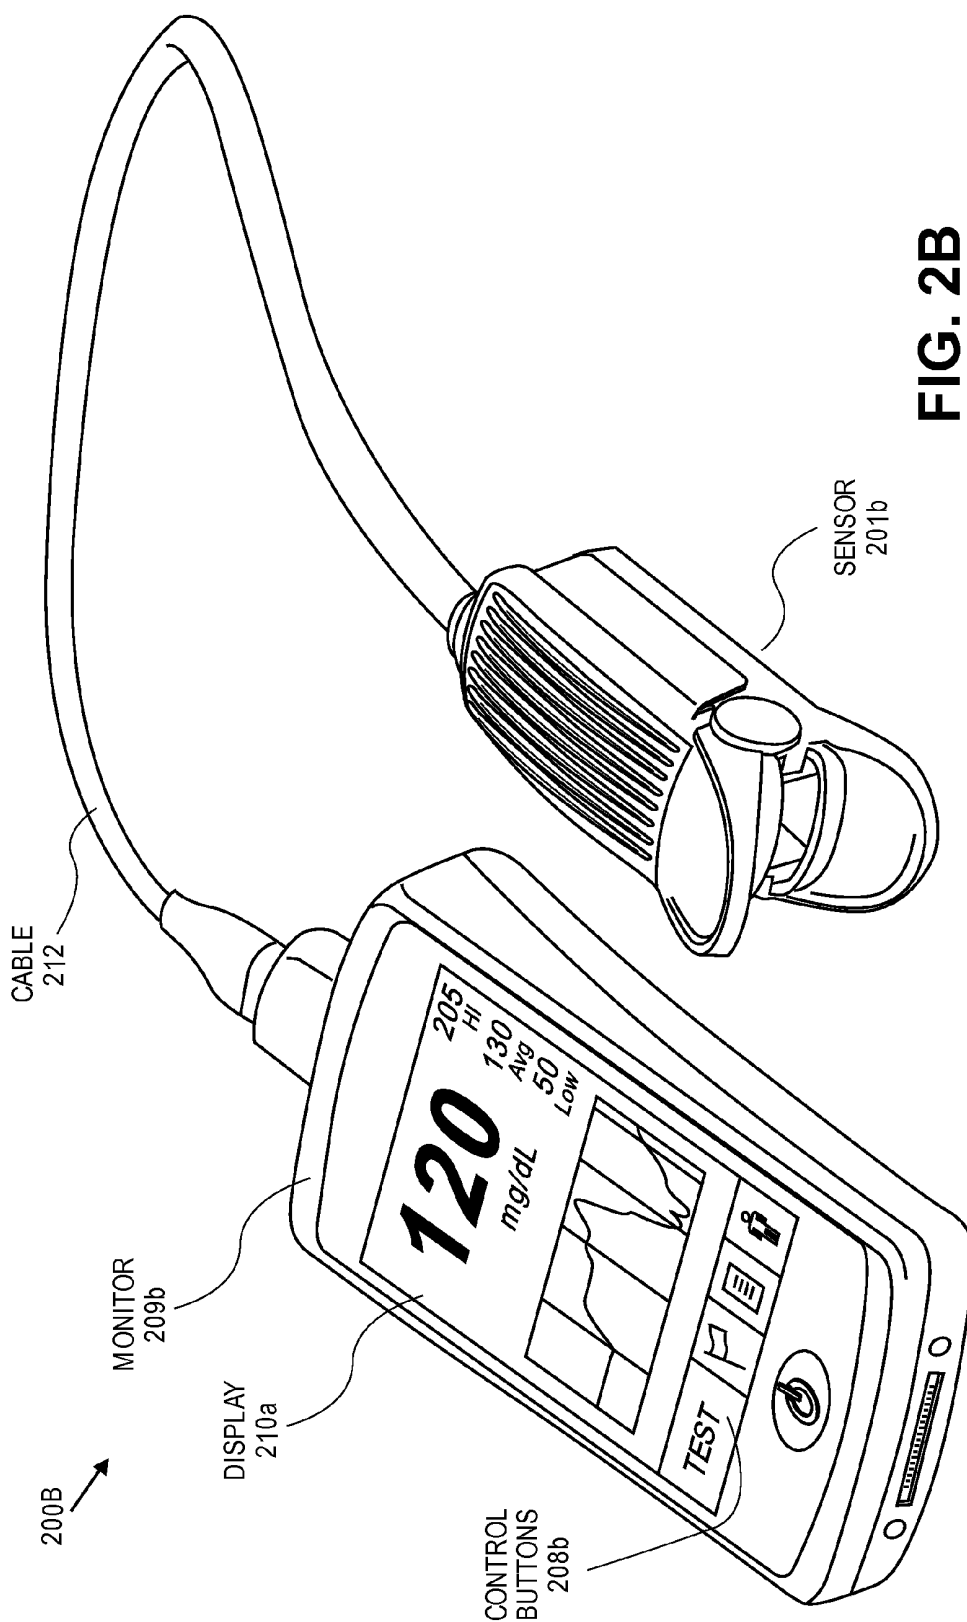

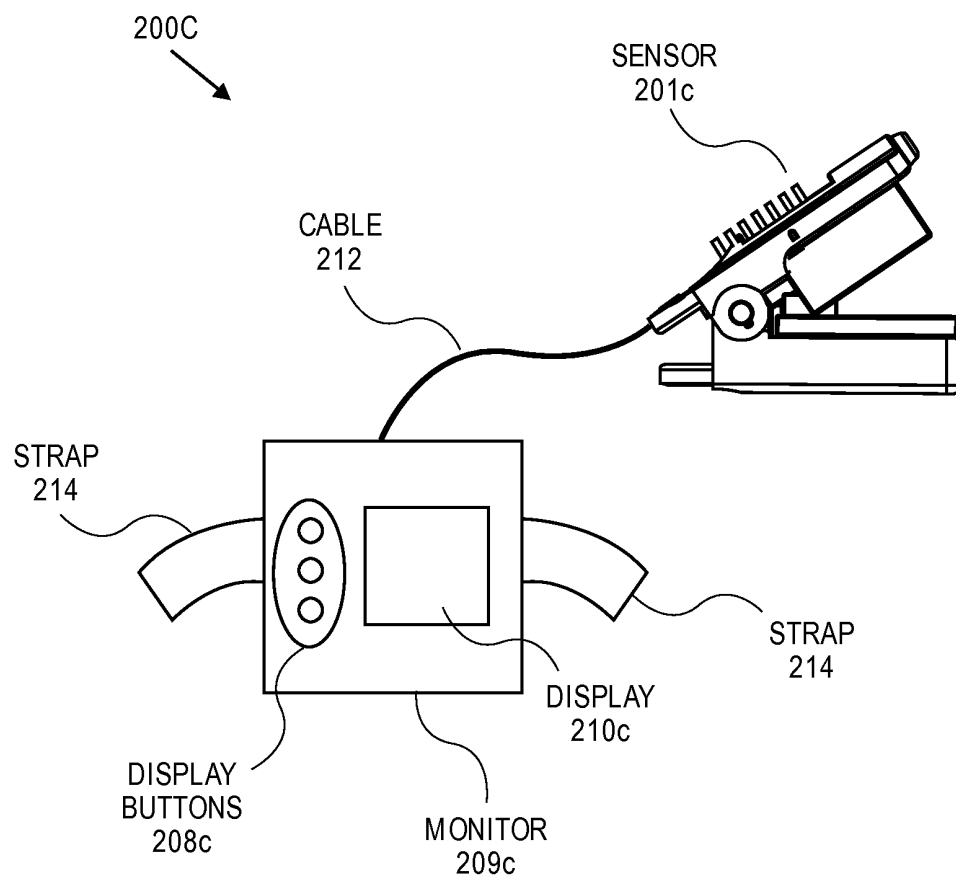**FIG. 2C**

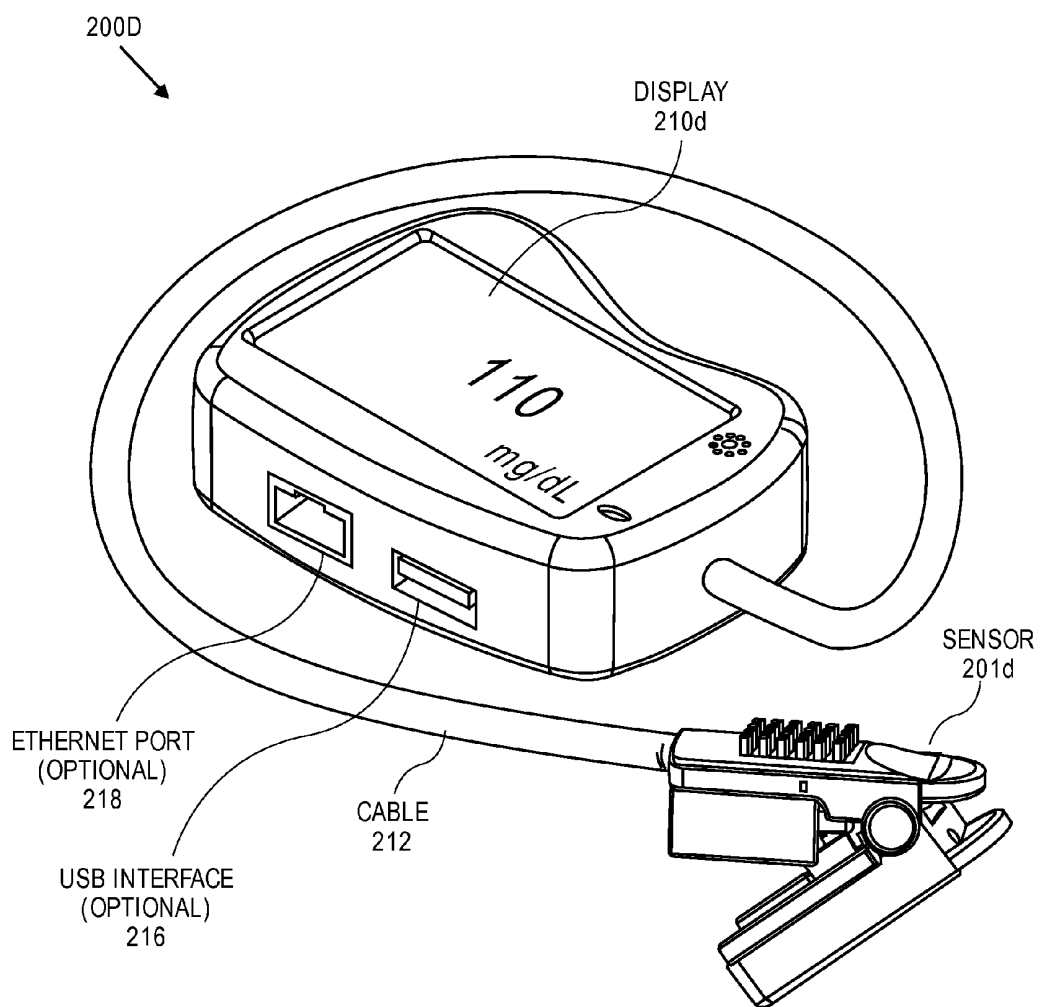**FIG. 2D**

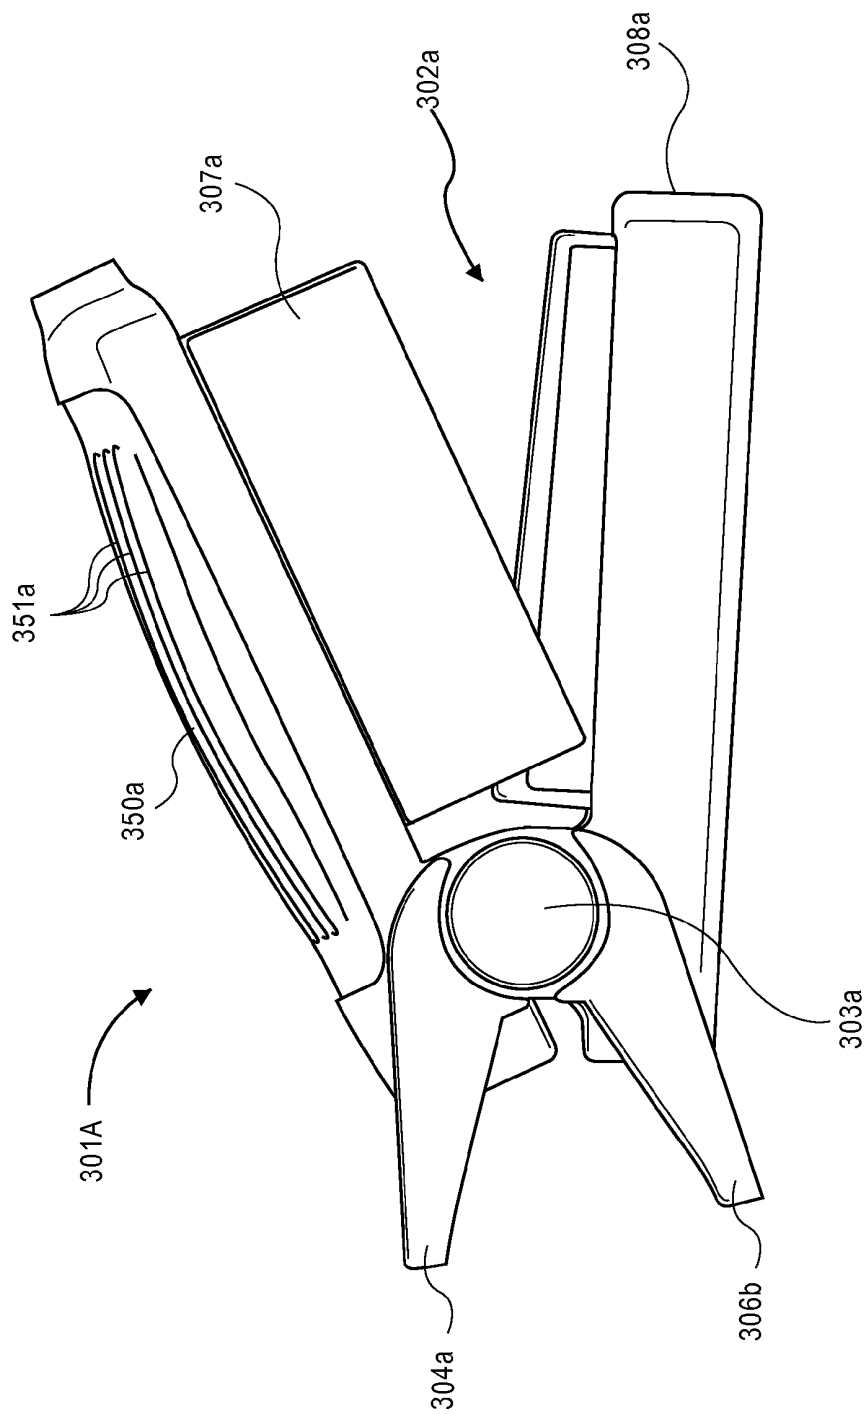
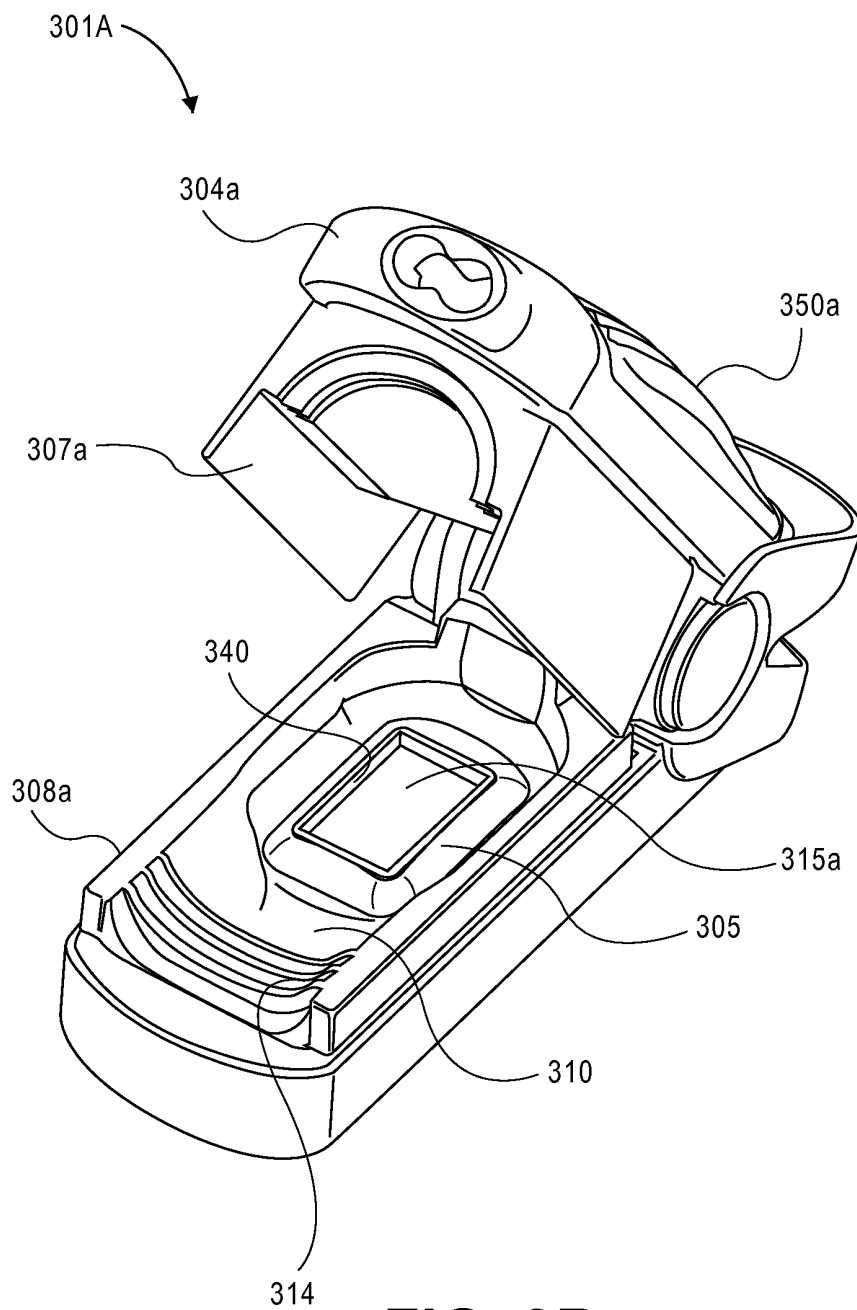


FIG. 3A

**FIG. 3B**

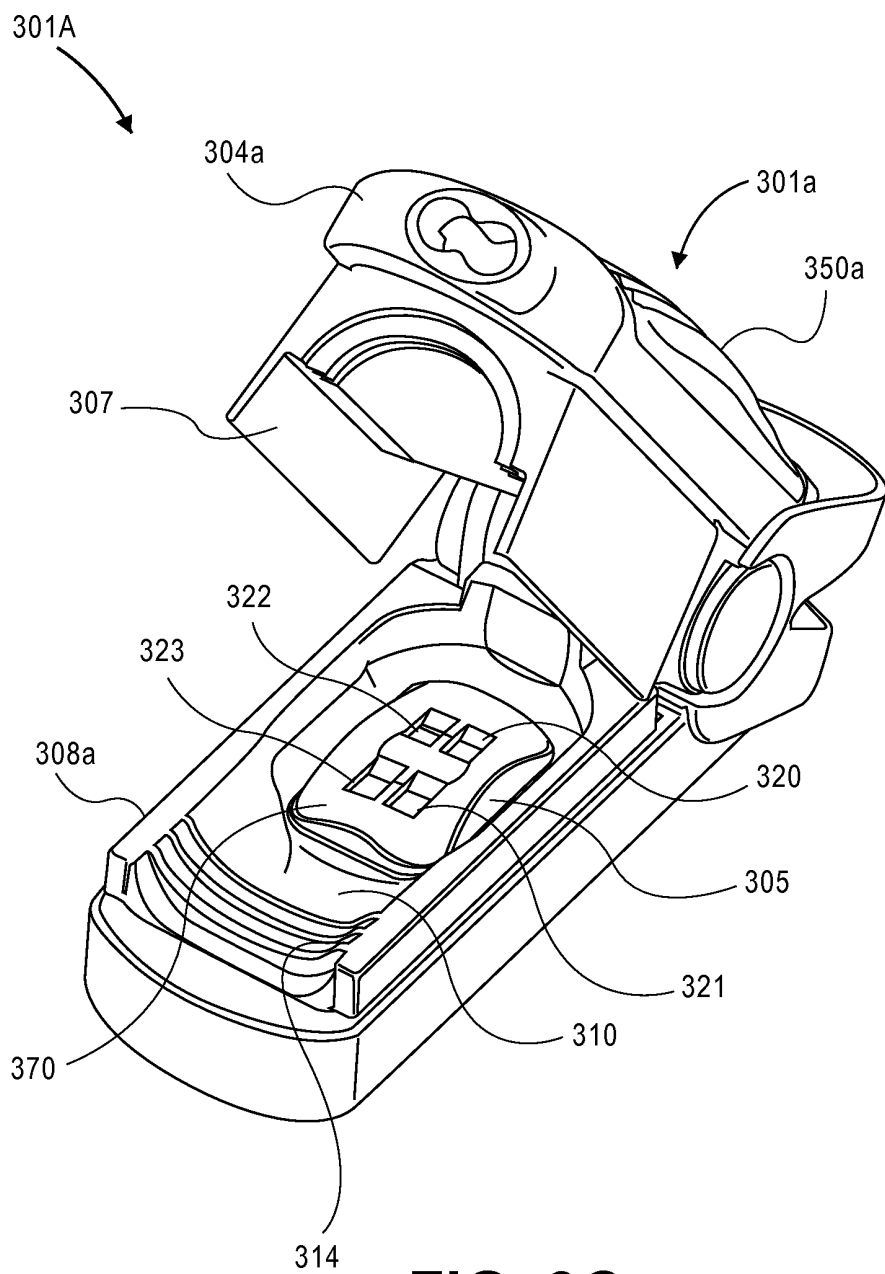
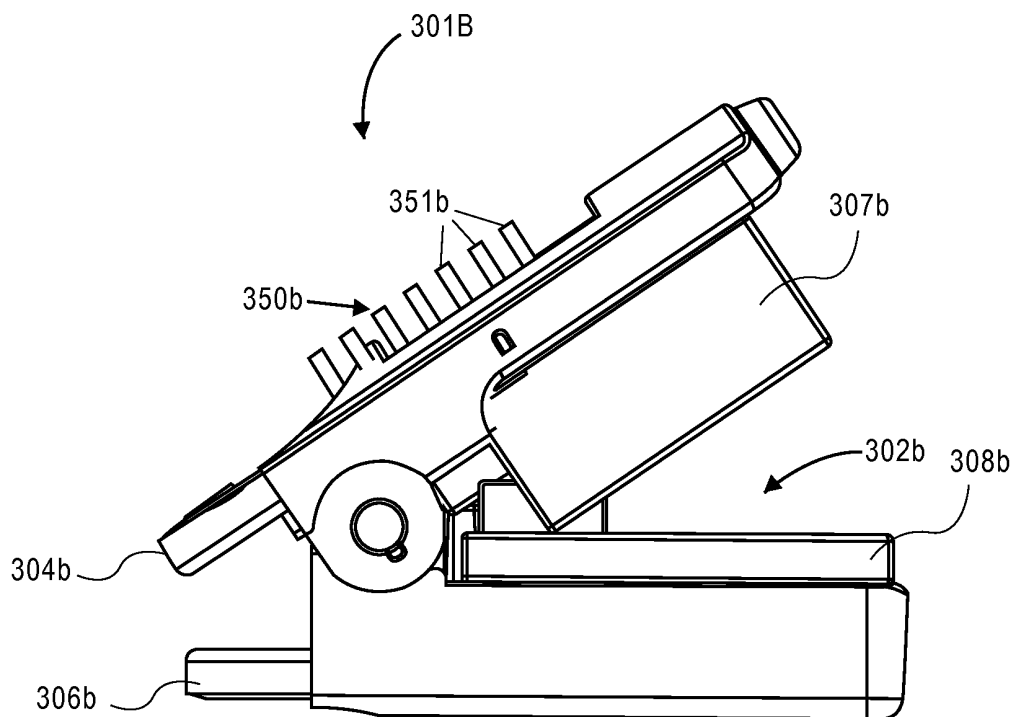
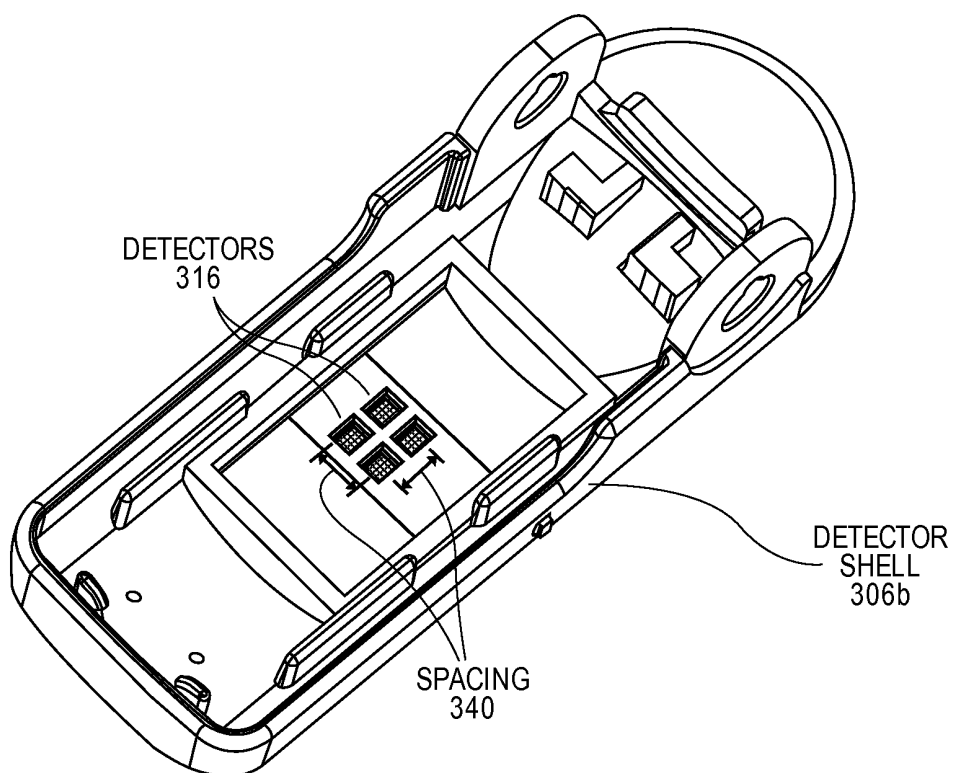


FIG. 3C

**FIG. 3D**

**FIG. 3E**

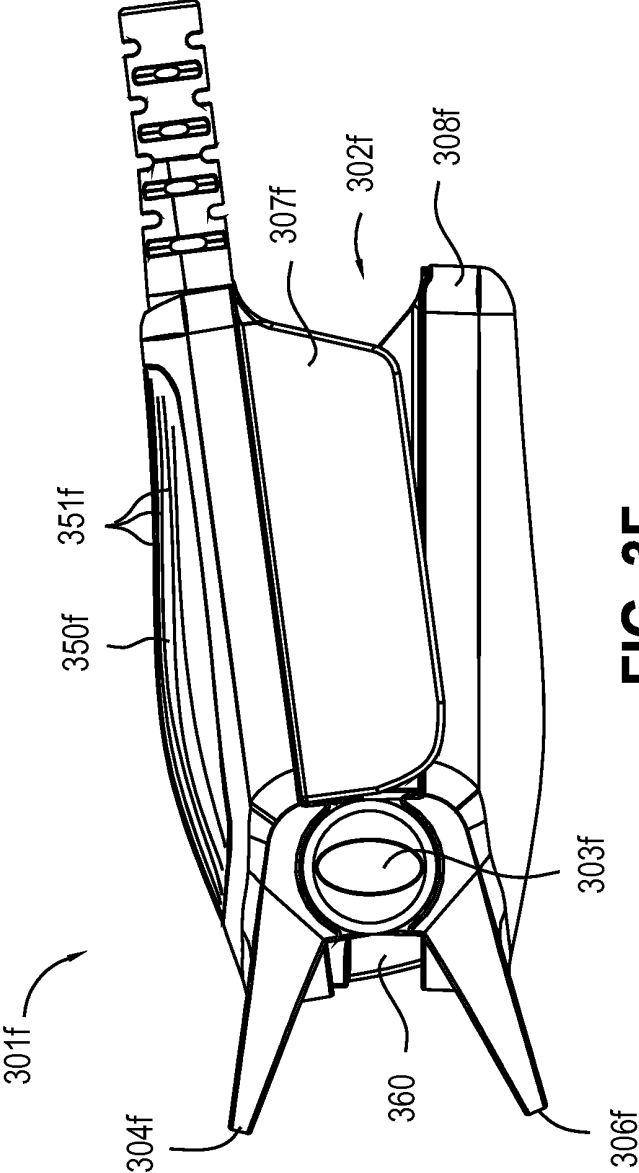


FIG. 3F

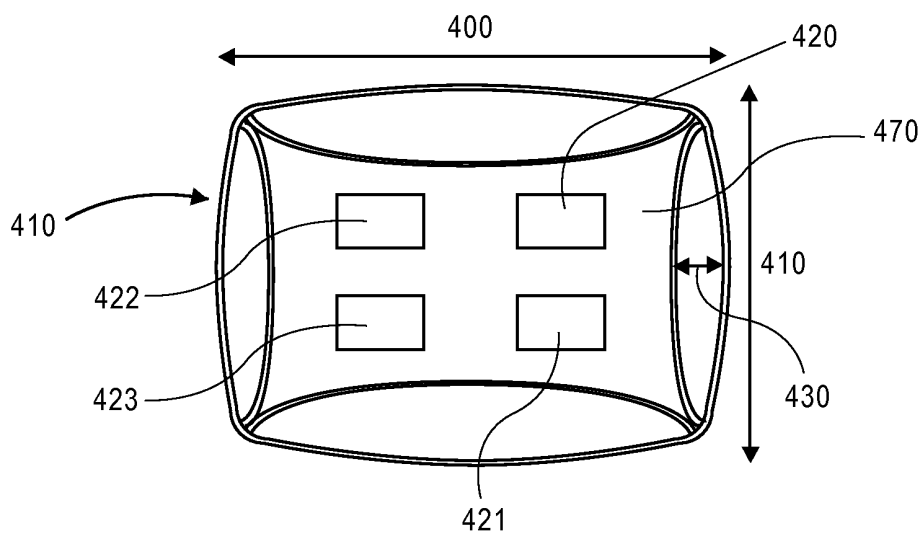


FIG. 4A

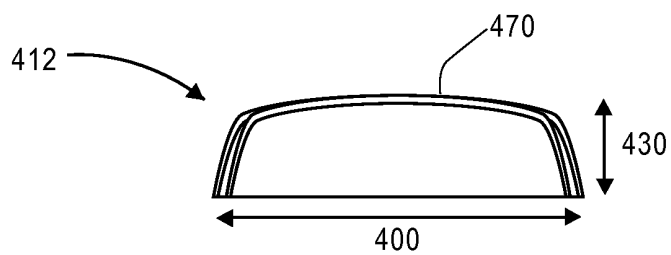


FIG. 4B

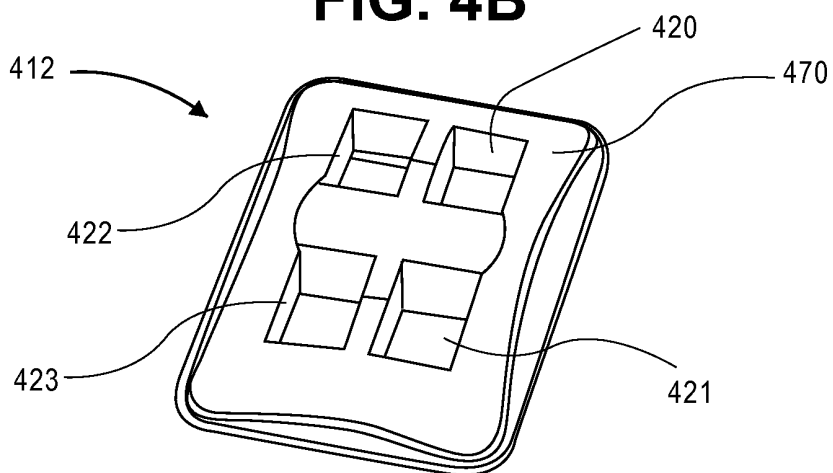


FIG. 4C

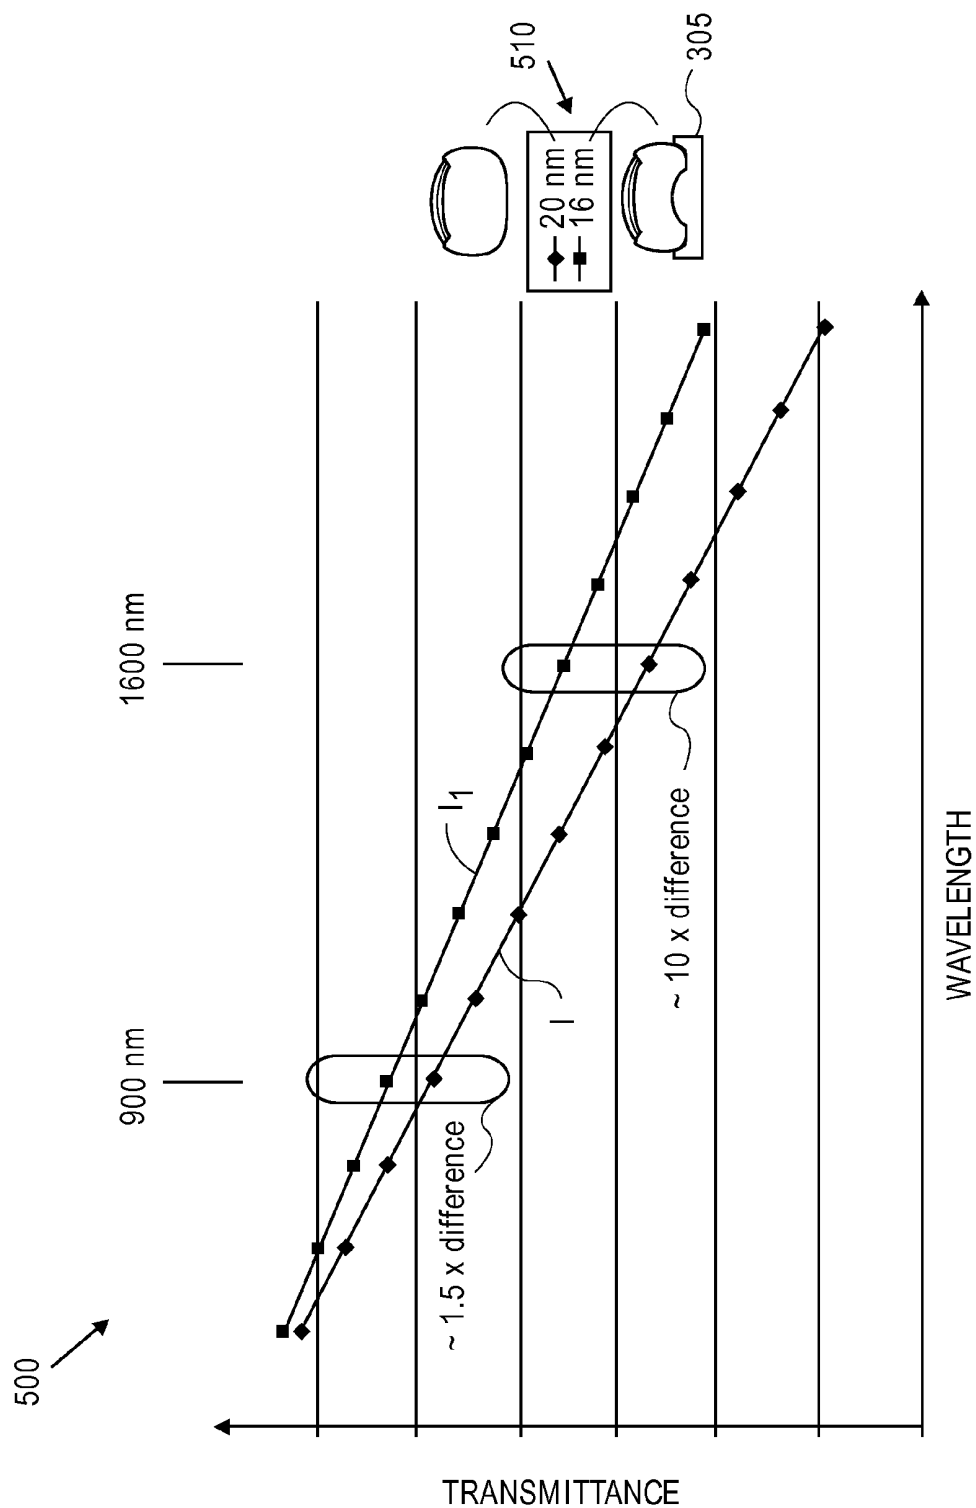


FIG. 5

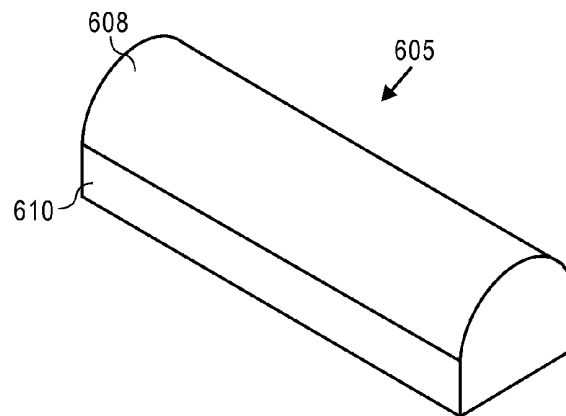


FIG. 6A




FIG. 6B

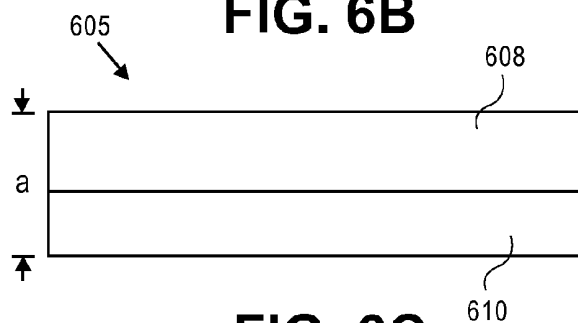


FIG. 6C

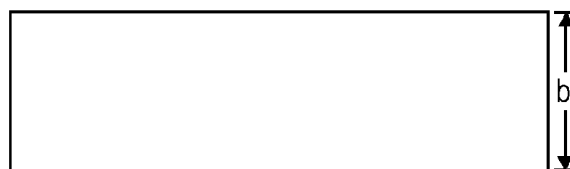


FIG. 6D

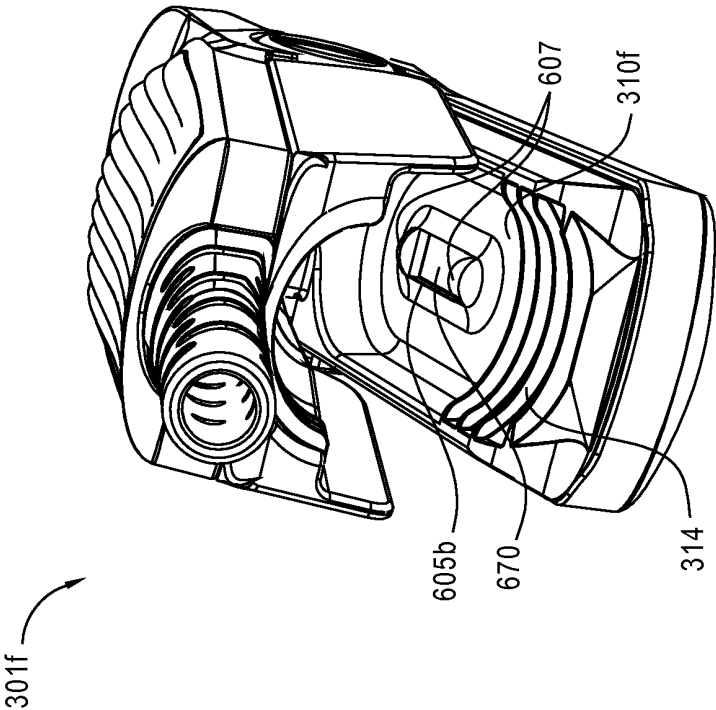
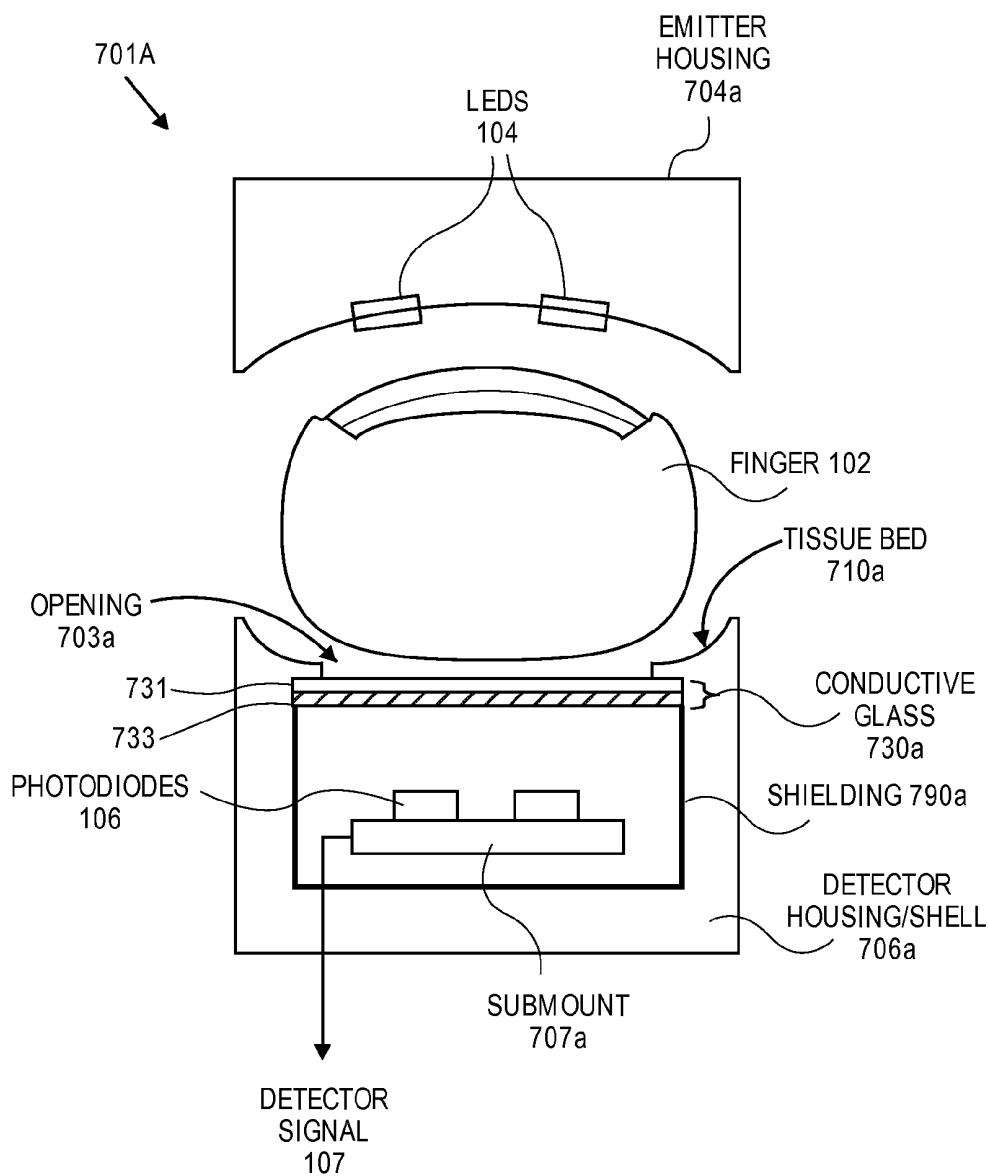
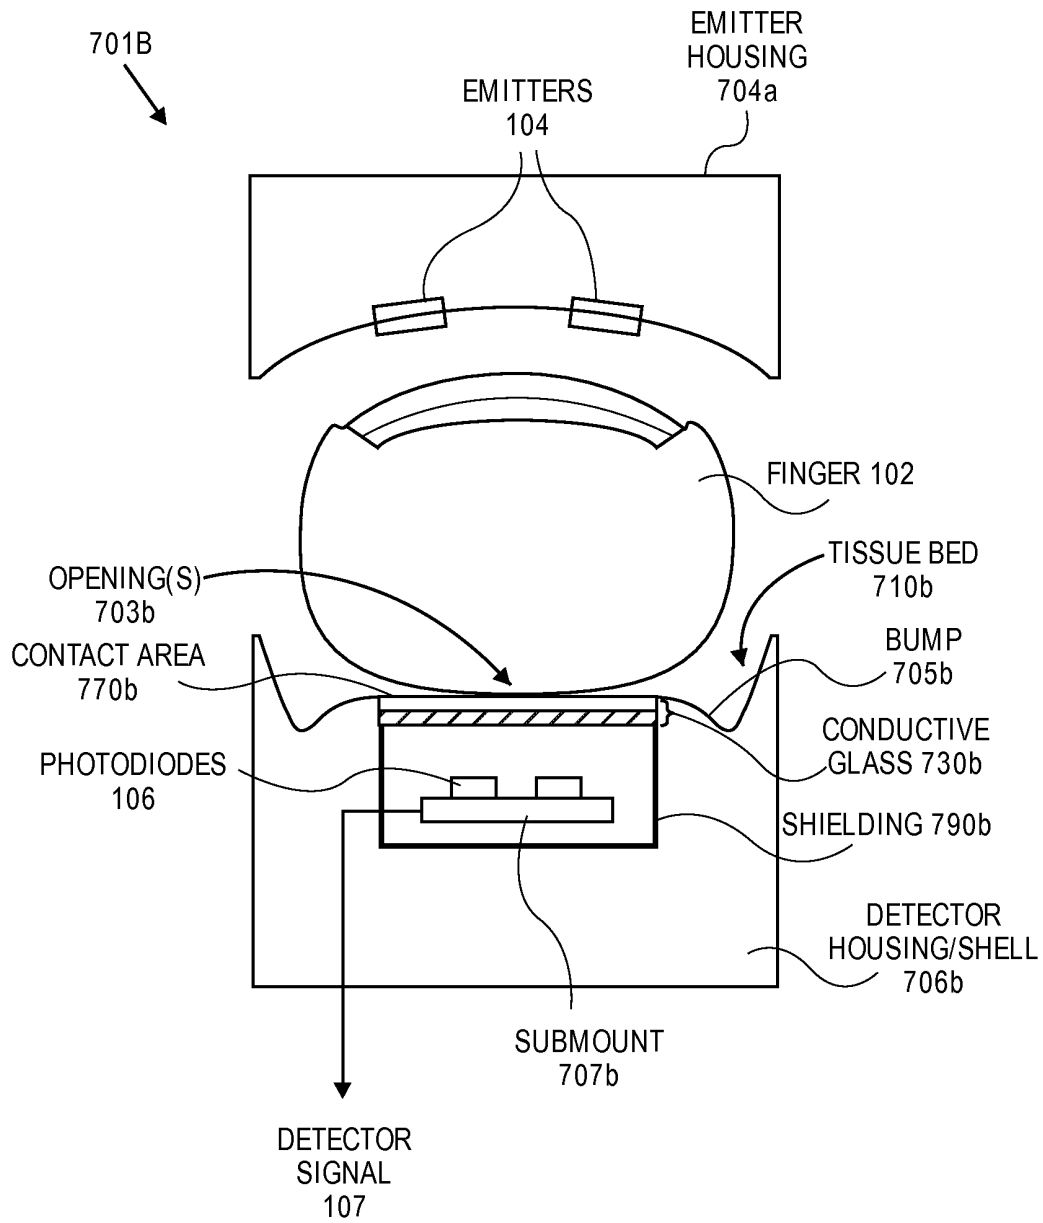


FIG. 6E

**FIG. 7A**

**FIG. 7B**

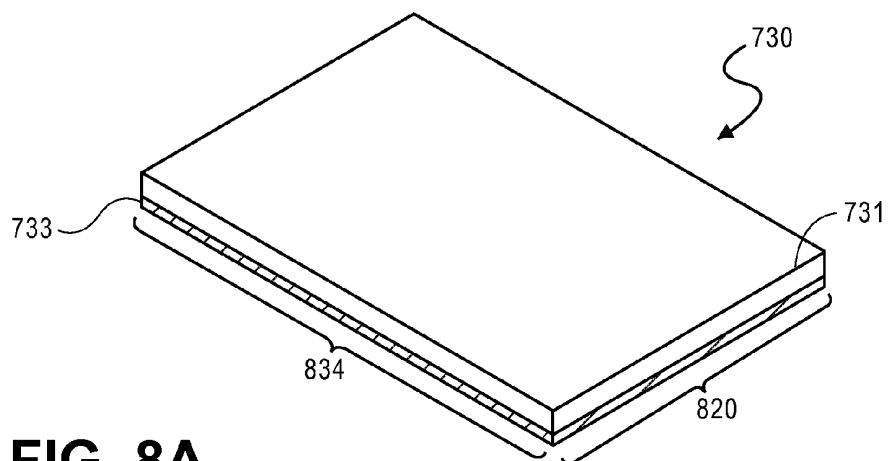


FIG. 8A

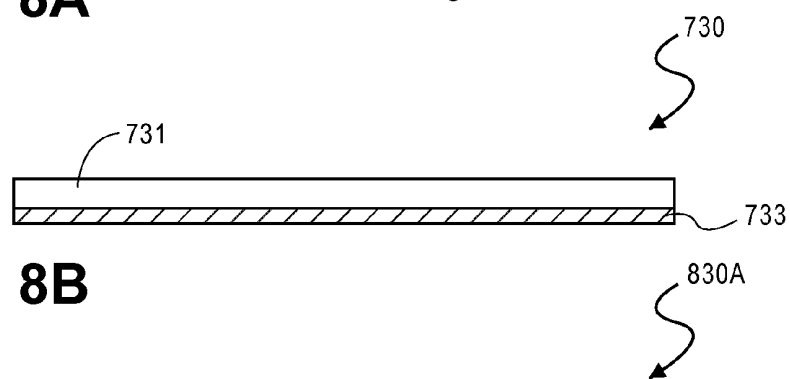


FIG. 8B




FIG. 8C

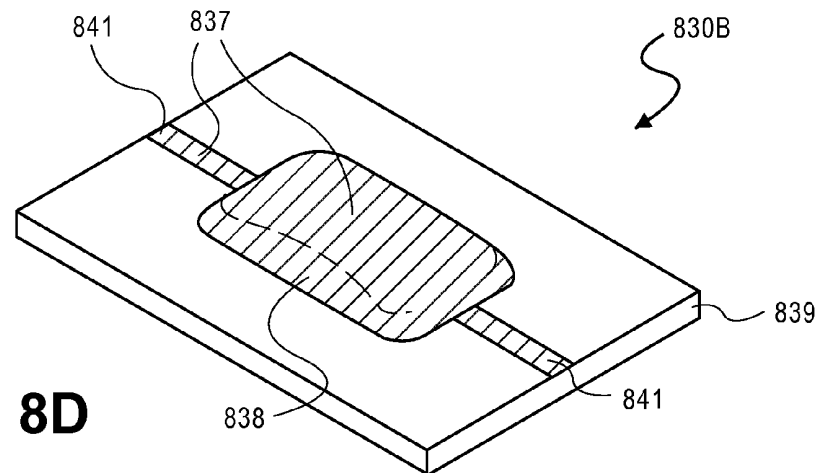


FIG. 8D

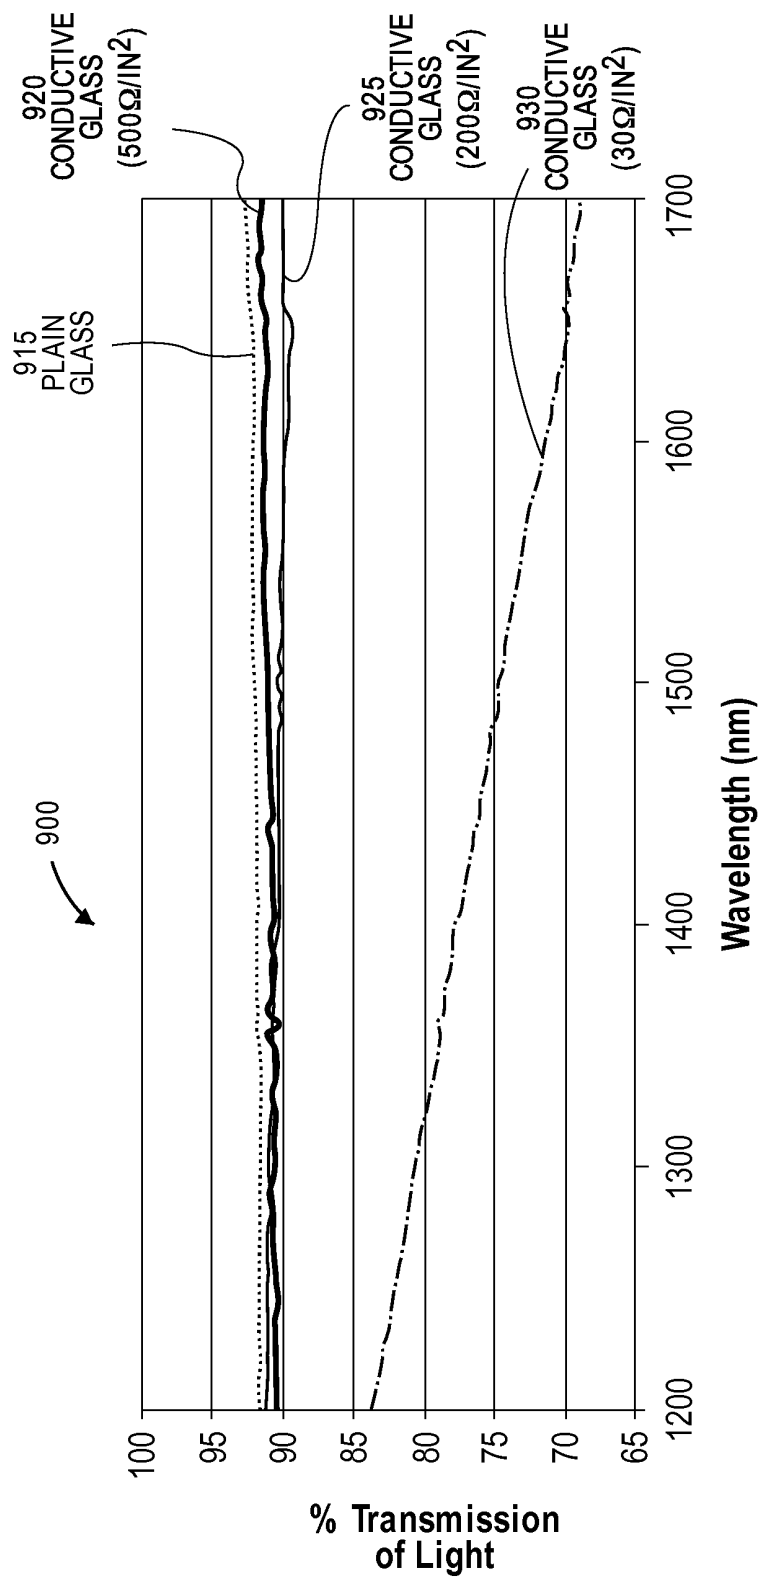


FIG. 9

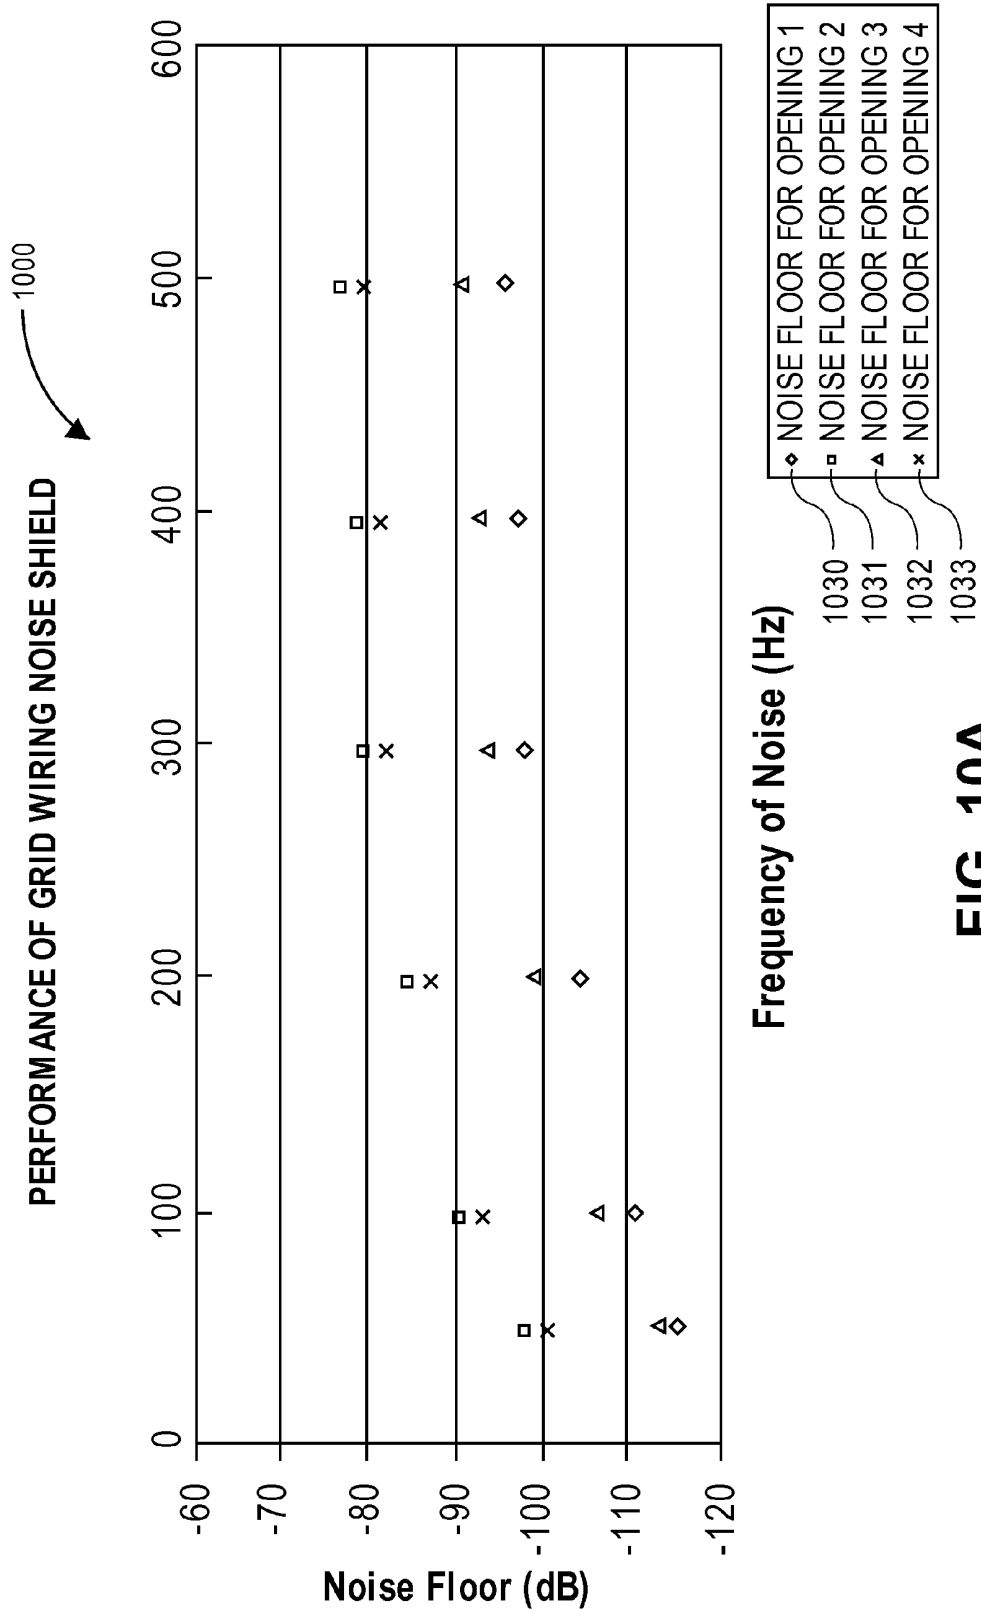


FIG. 10A



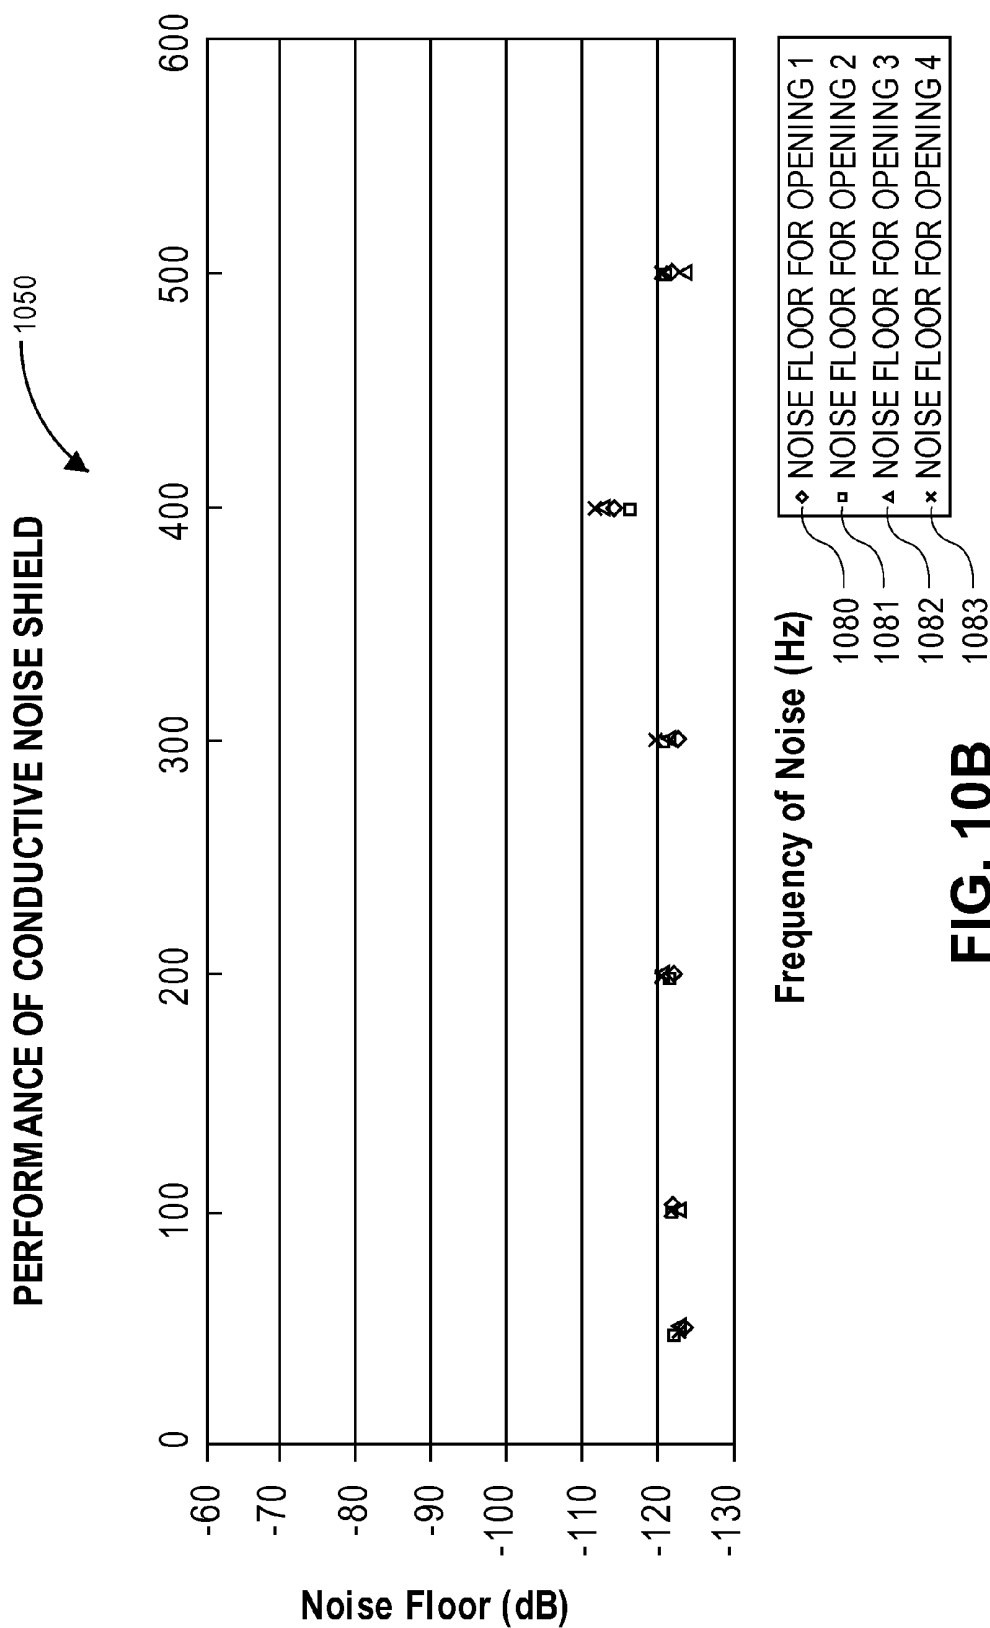


FIG. 10B

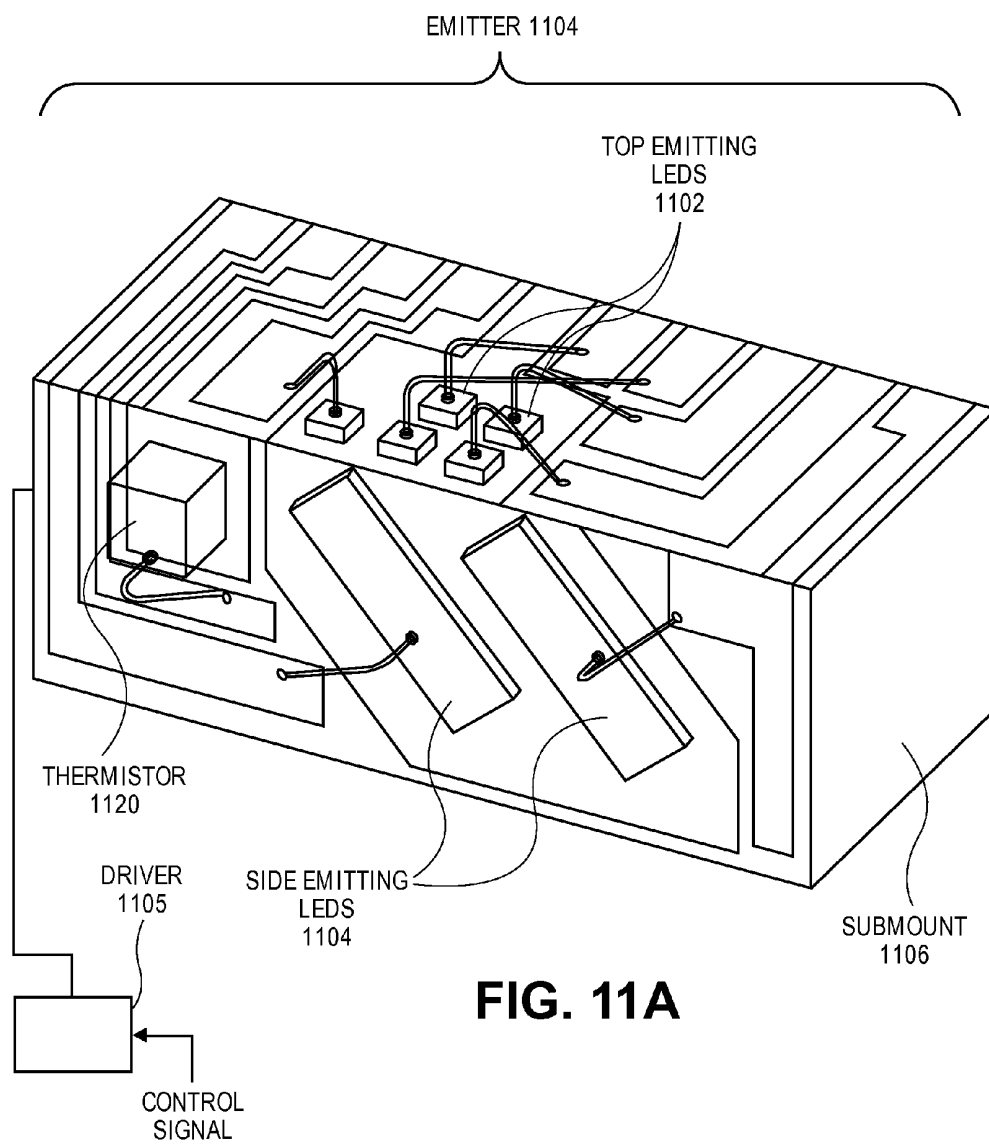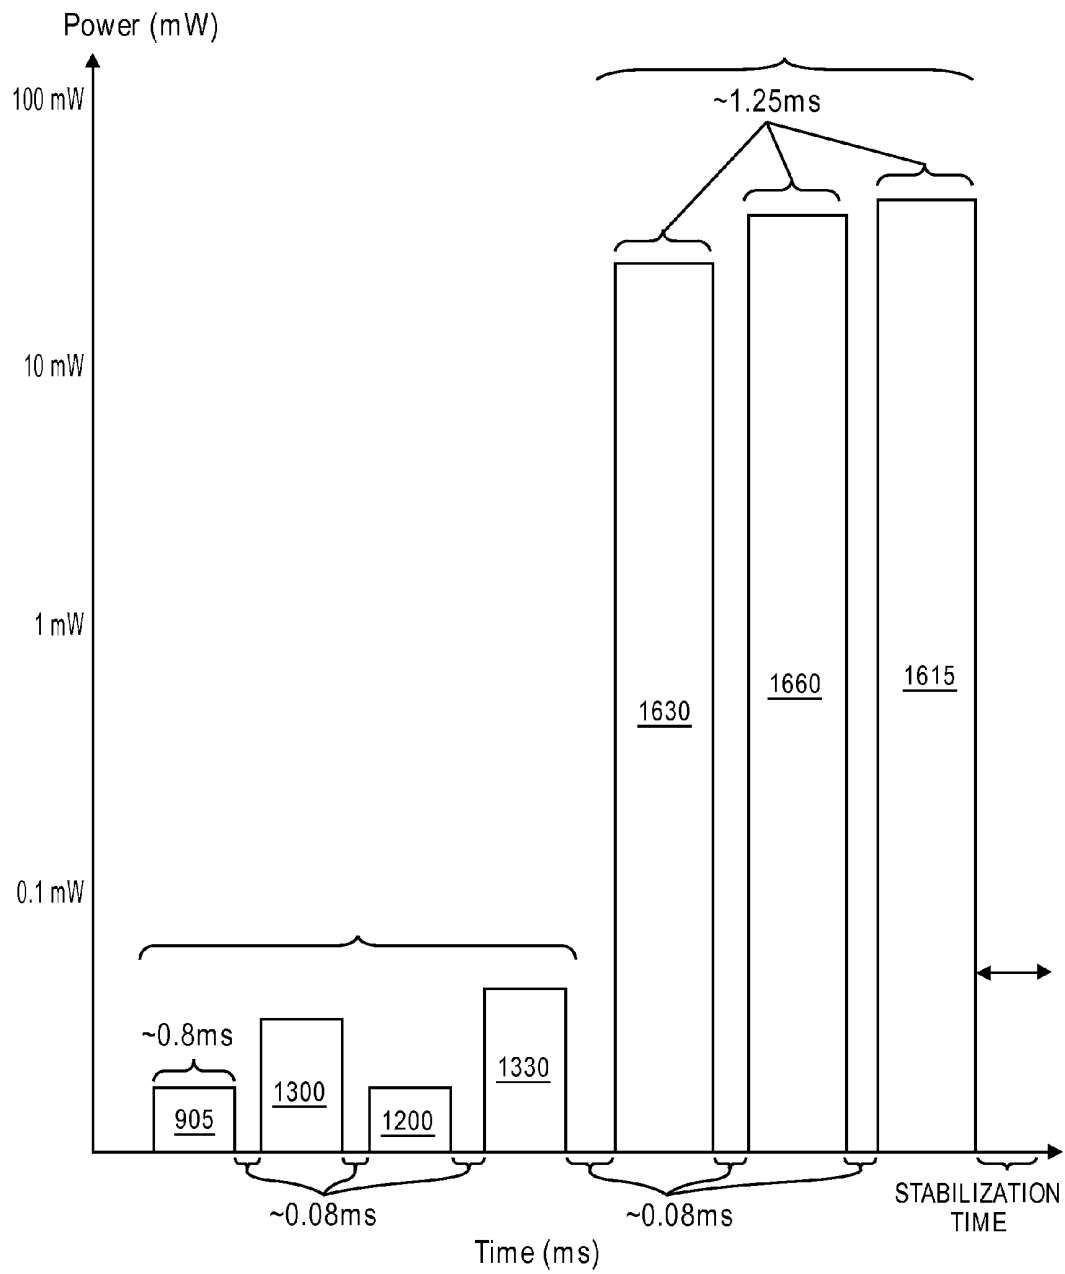

**FIG. 11B**

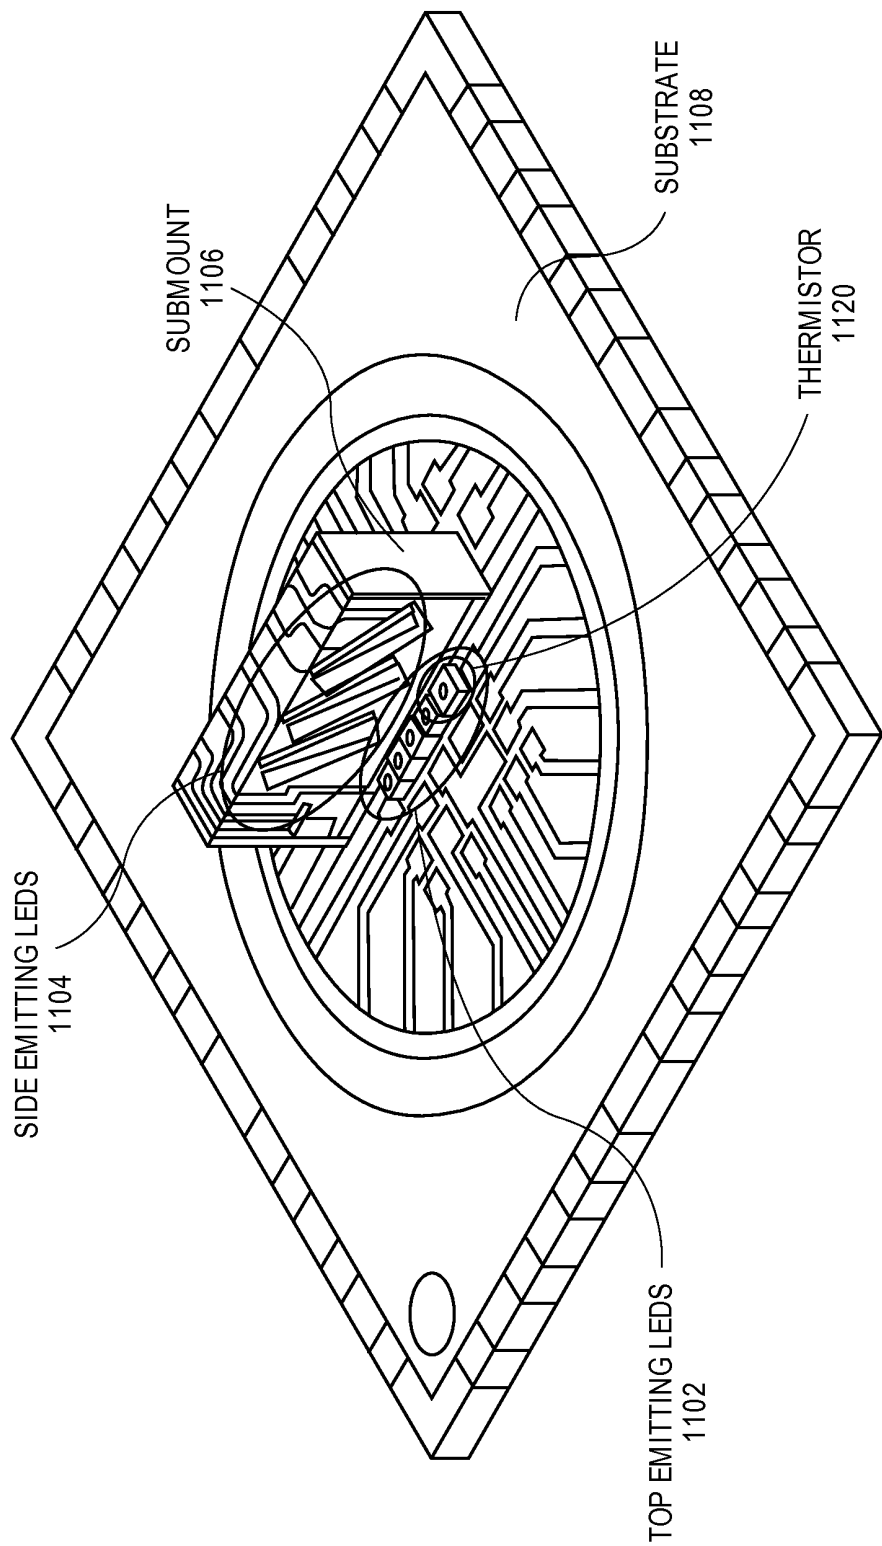


FIG. 11C

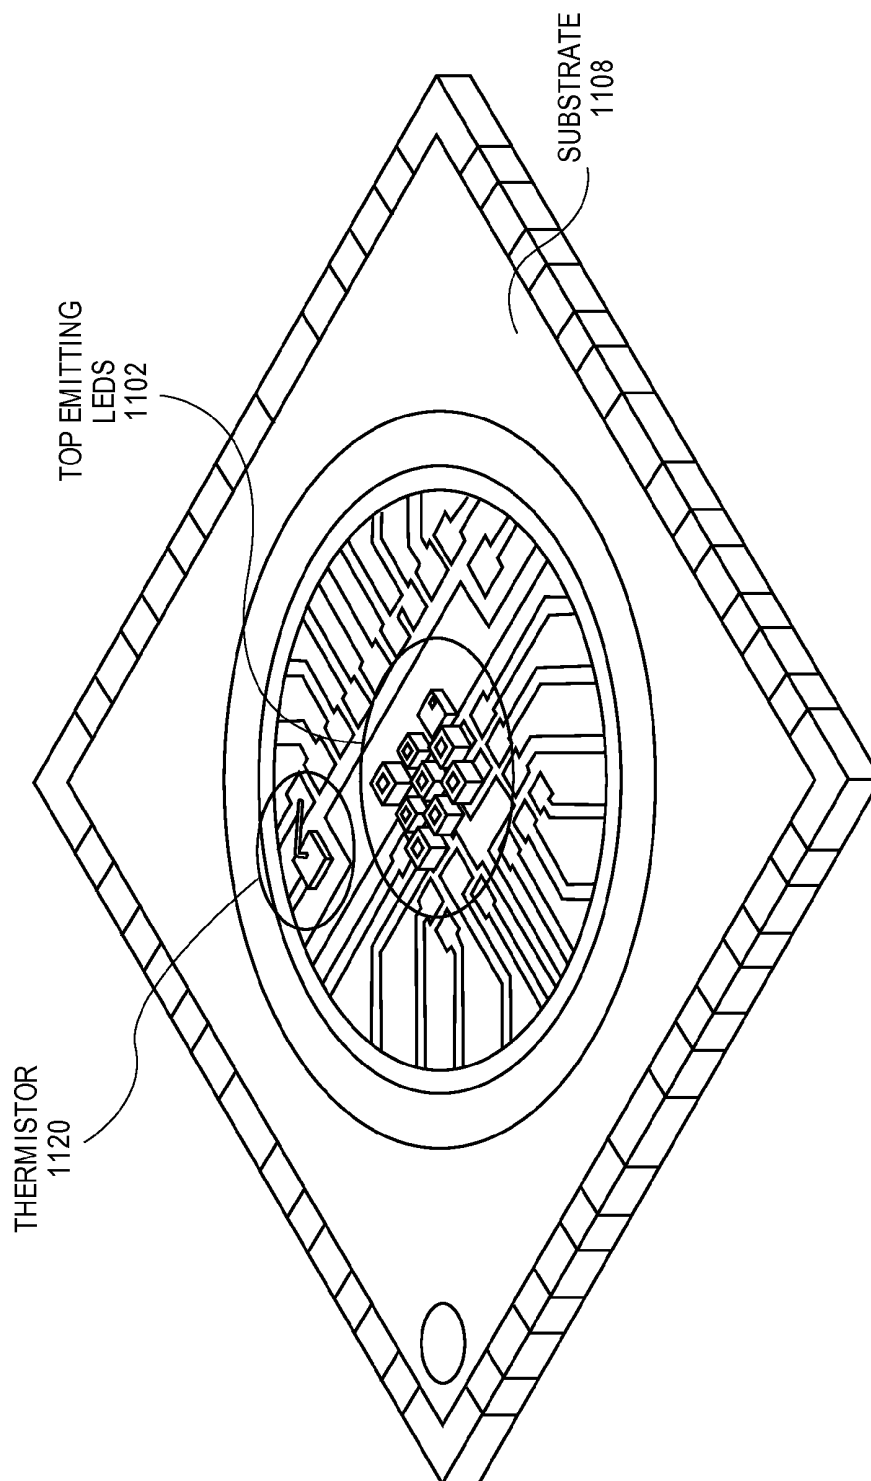
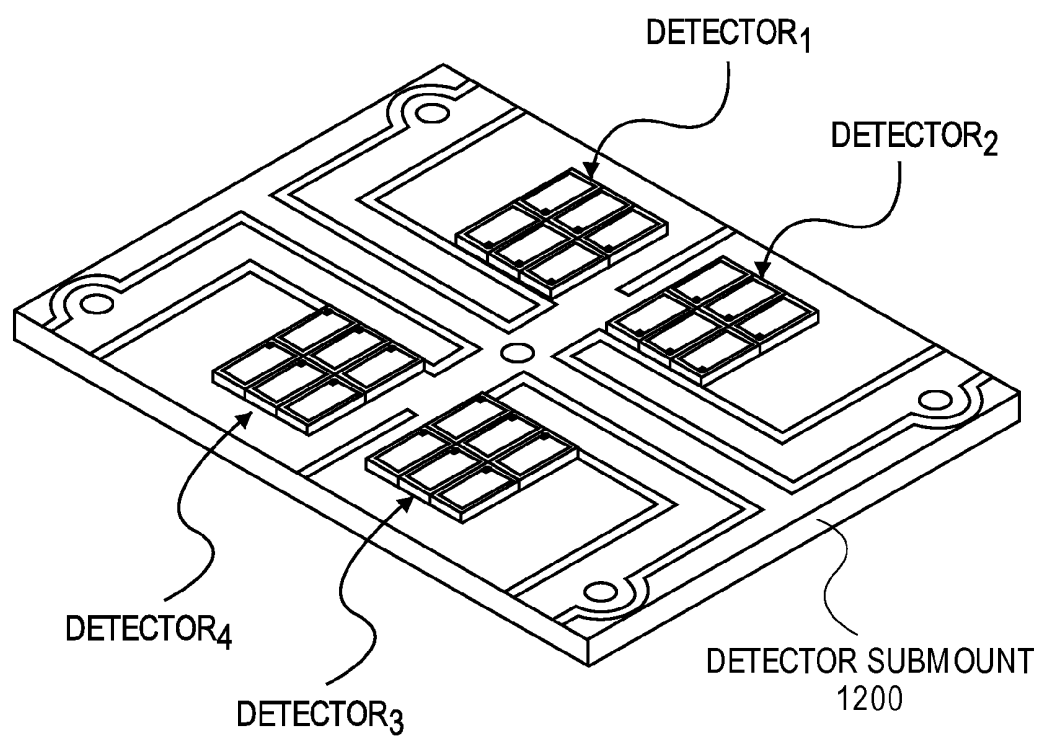


FIG. 11D

**FIG. 12A**

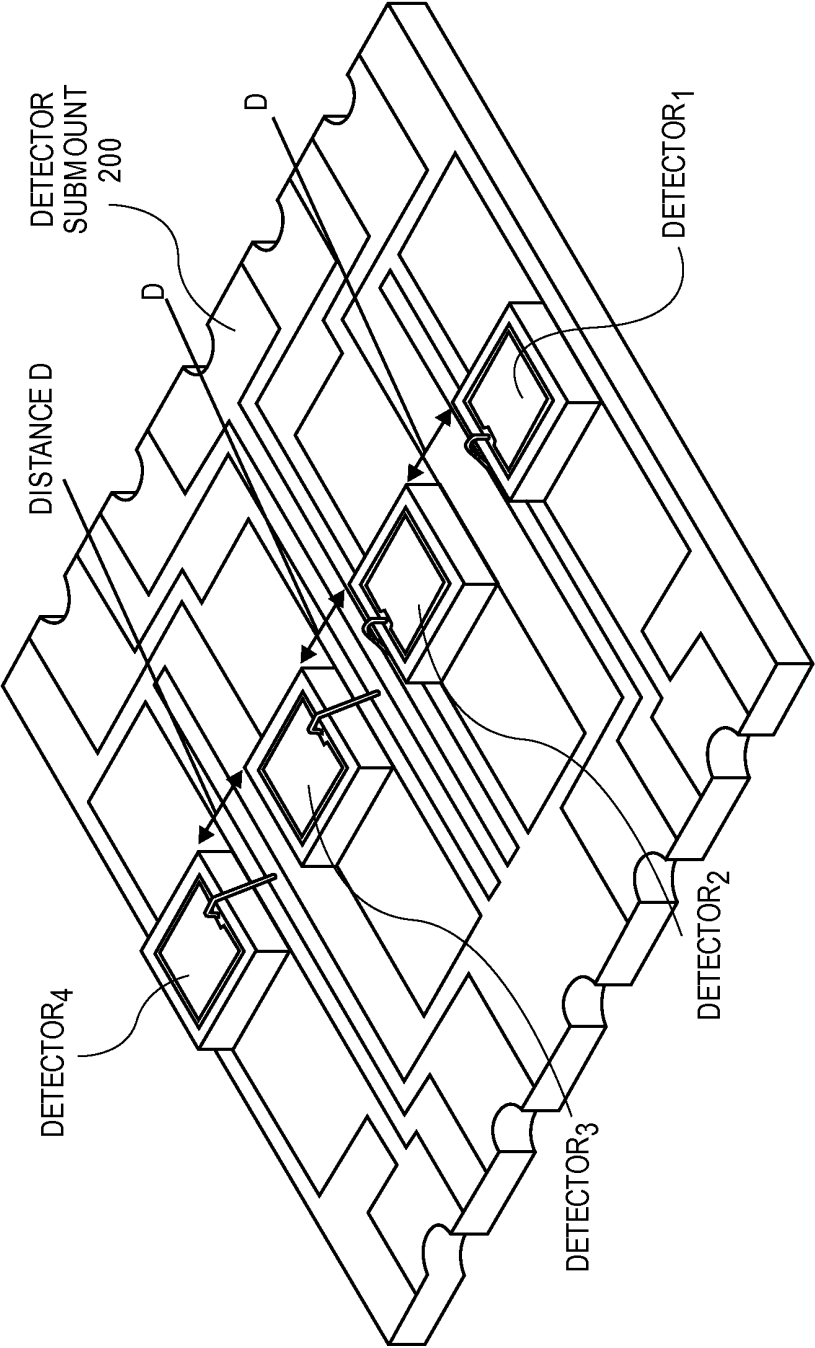
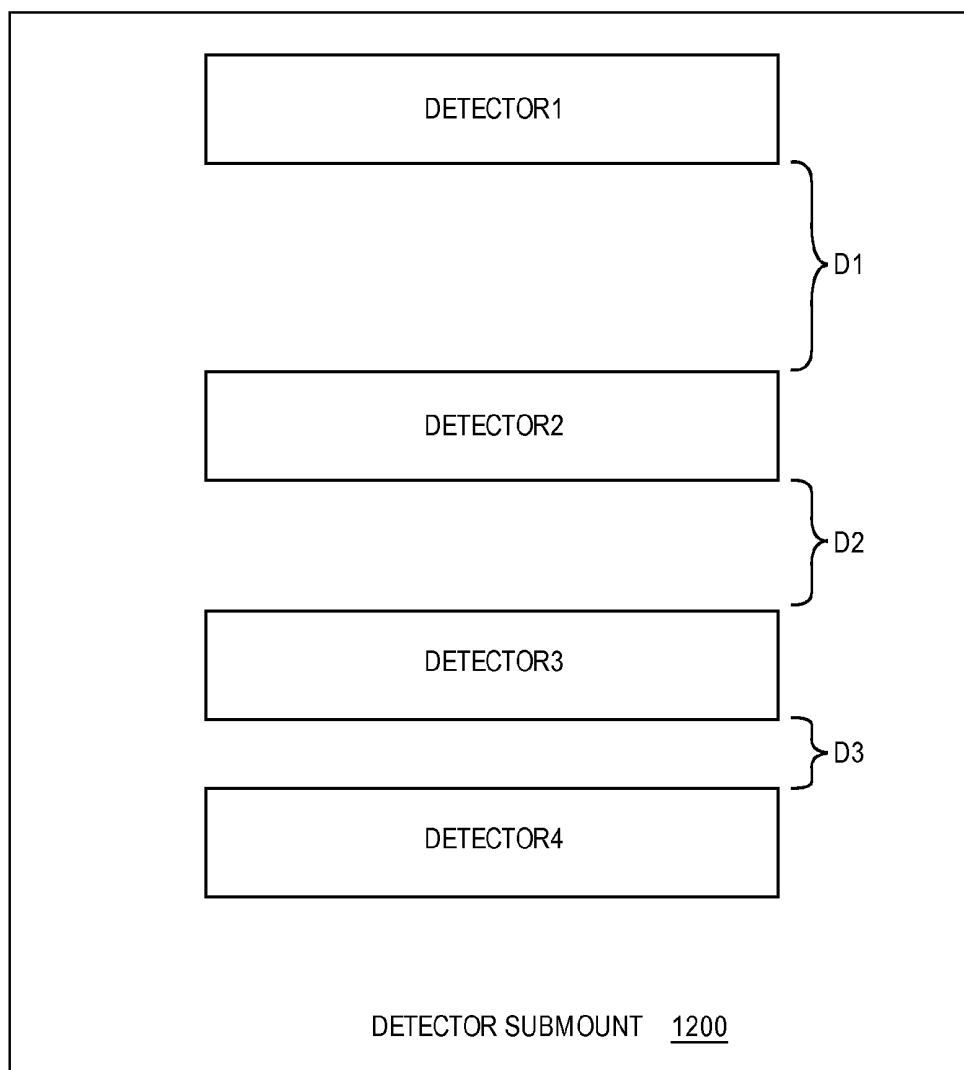
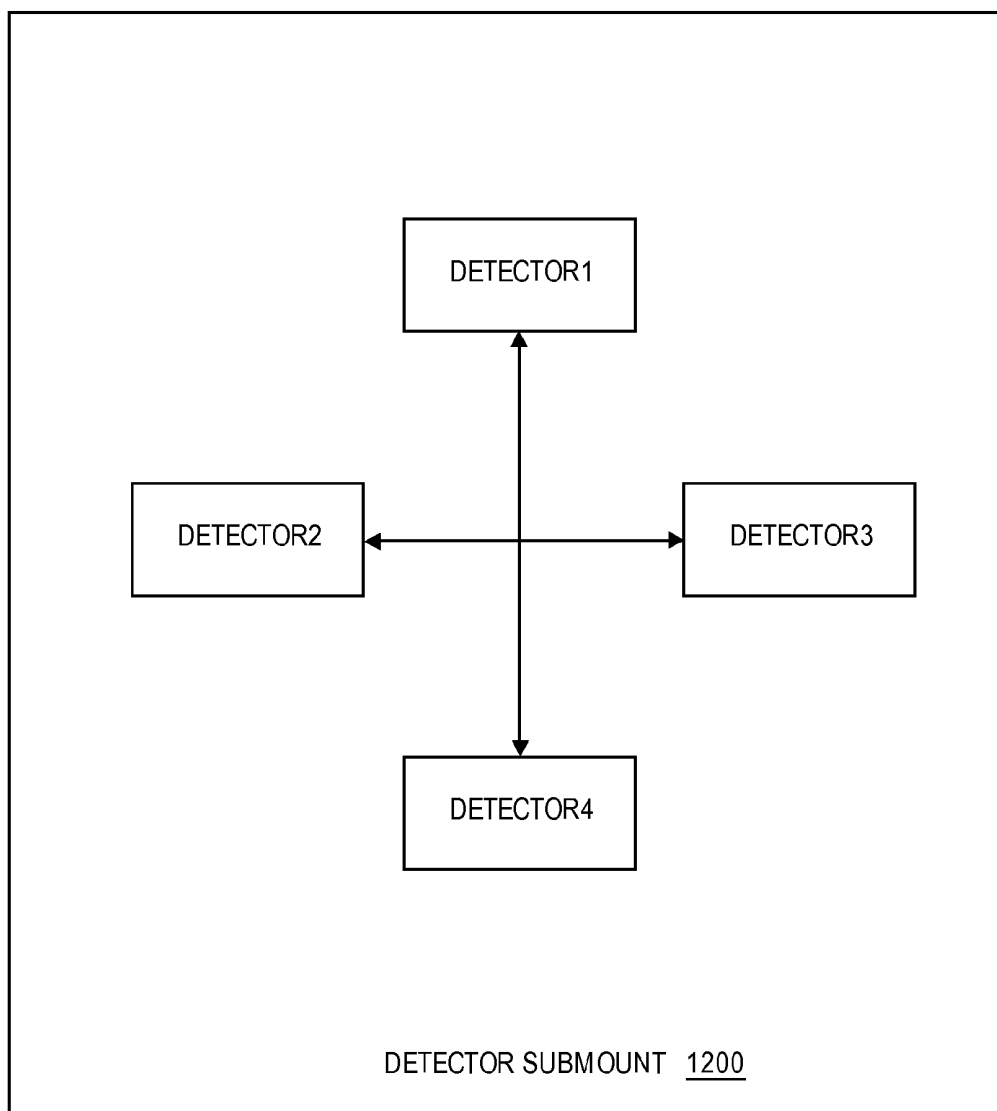
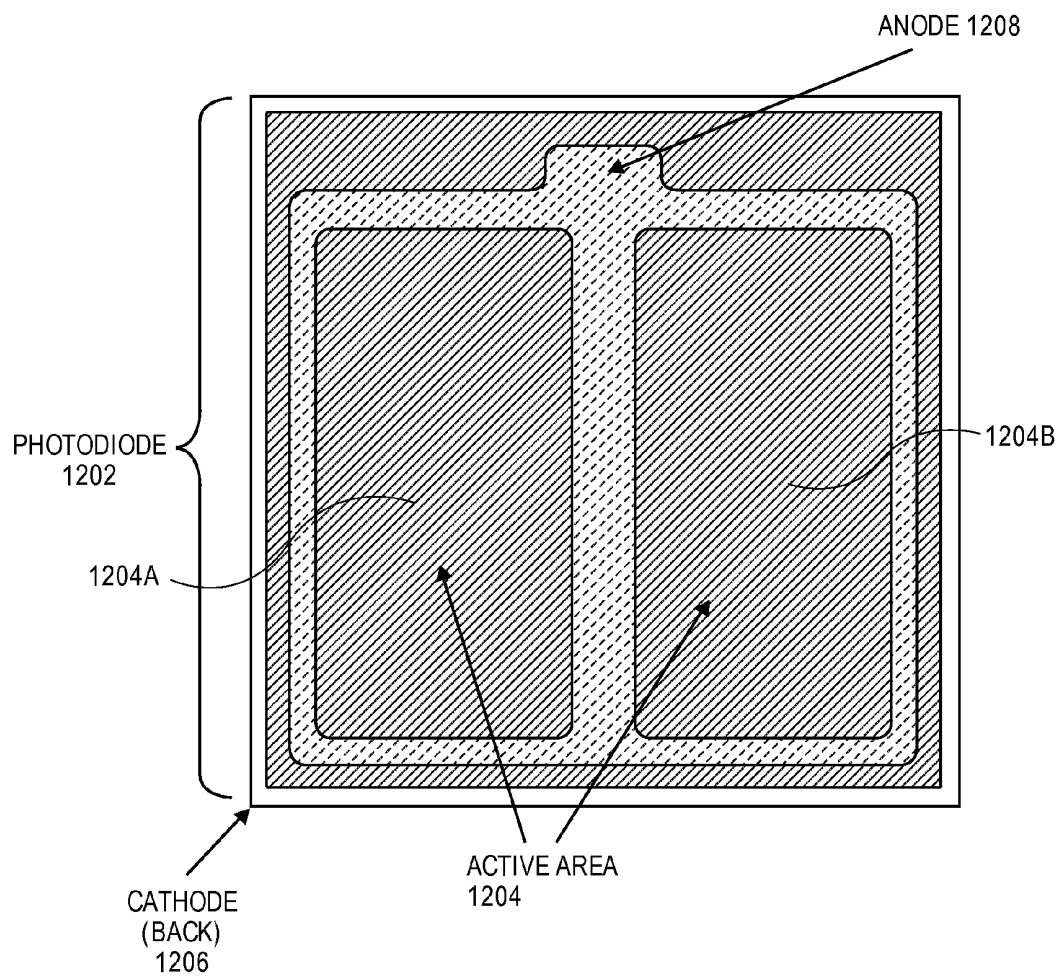
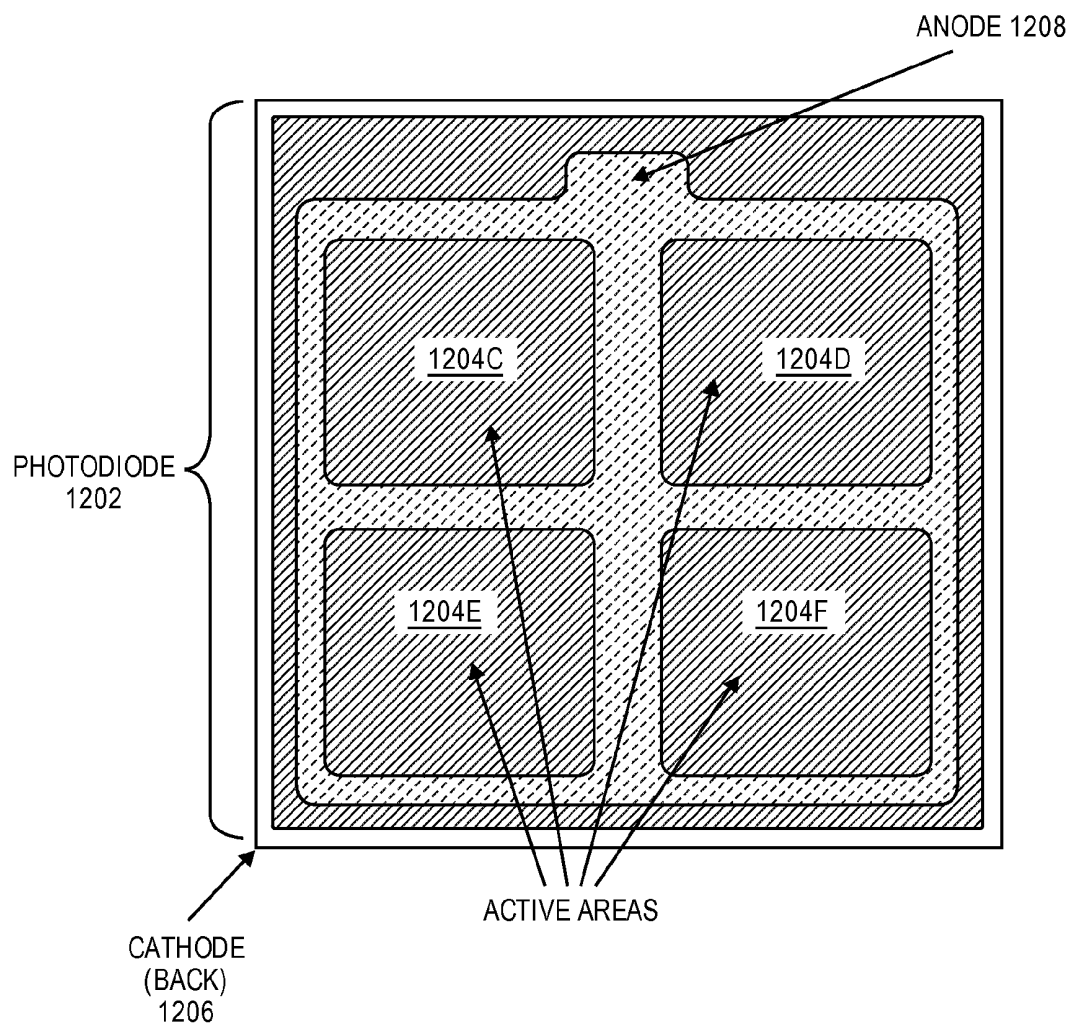



FIG. 12B


**FIG. 12C**


**FIG. 12D**


**FIG. 12E**

**FIG. 12F**

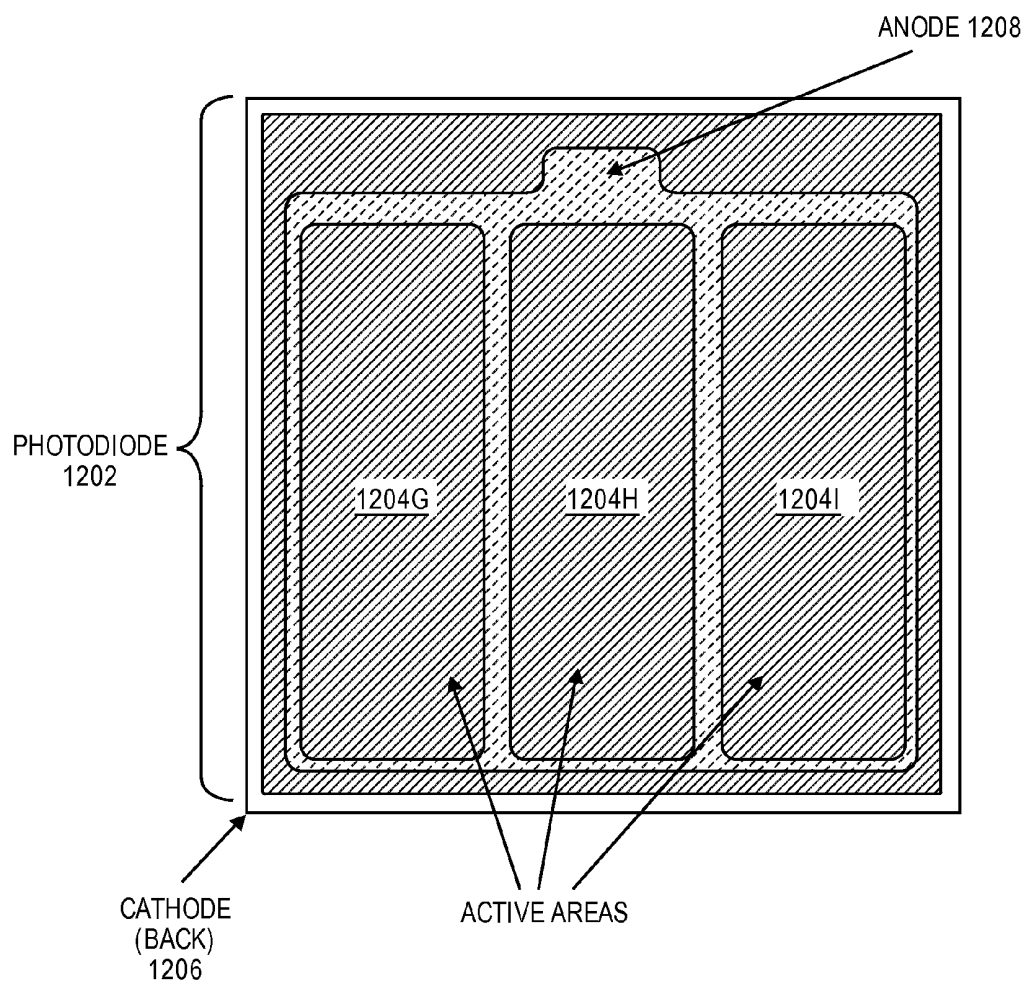**FIG. 12G**

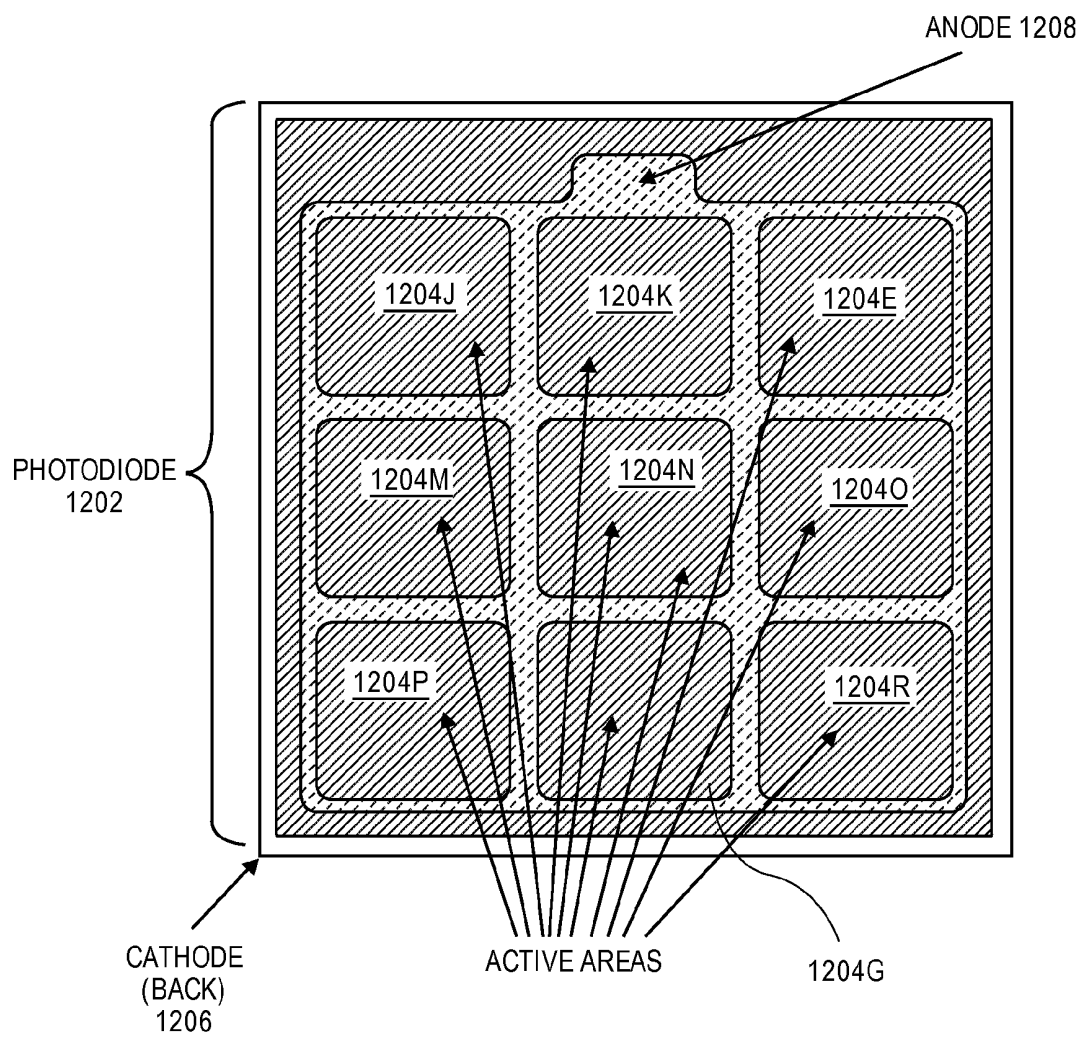**FIG. 12H**

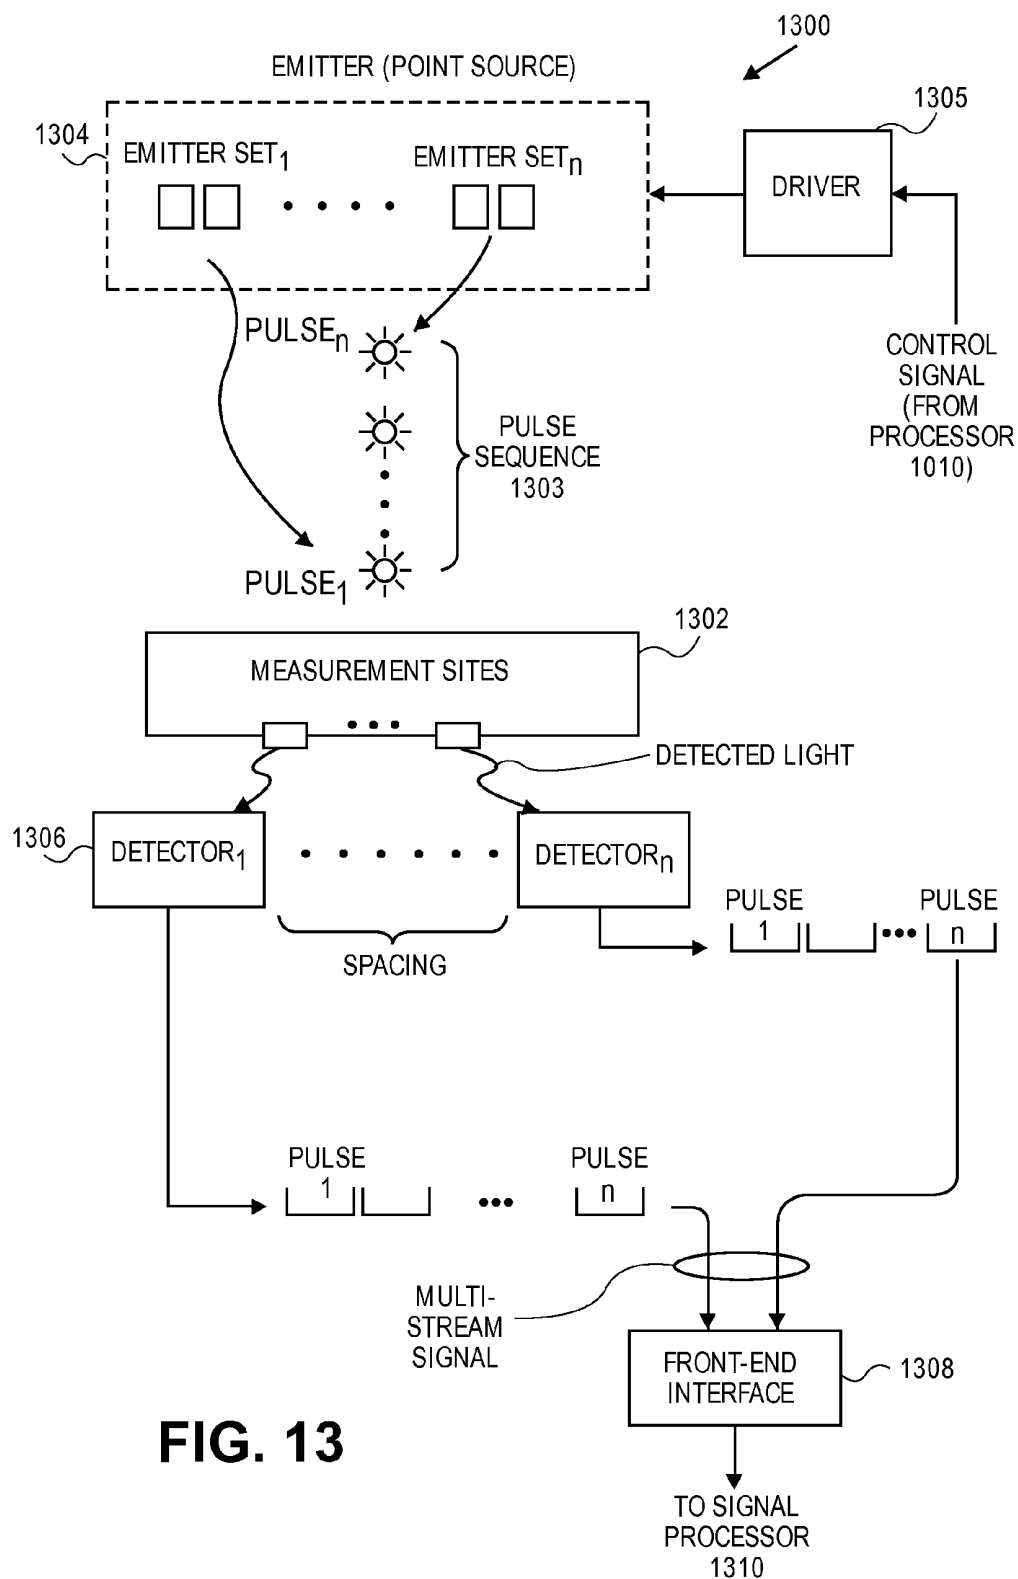

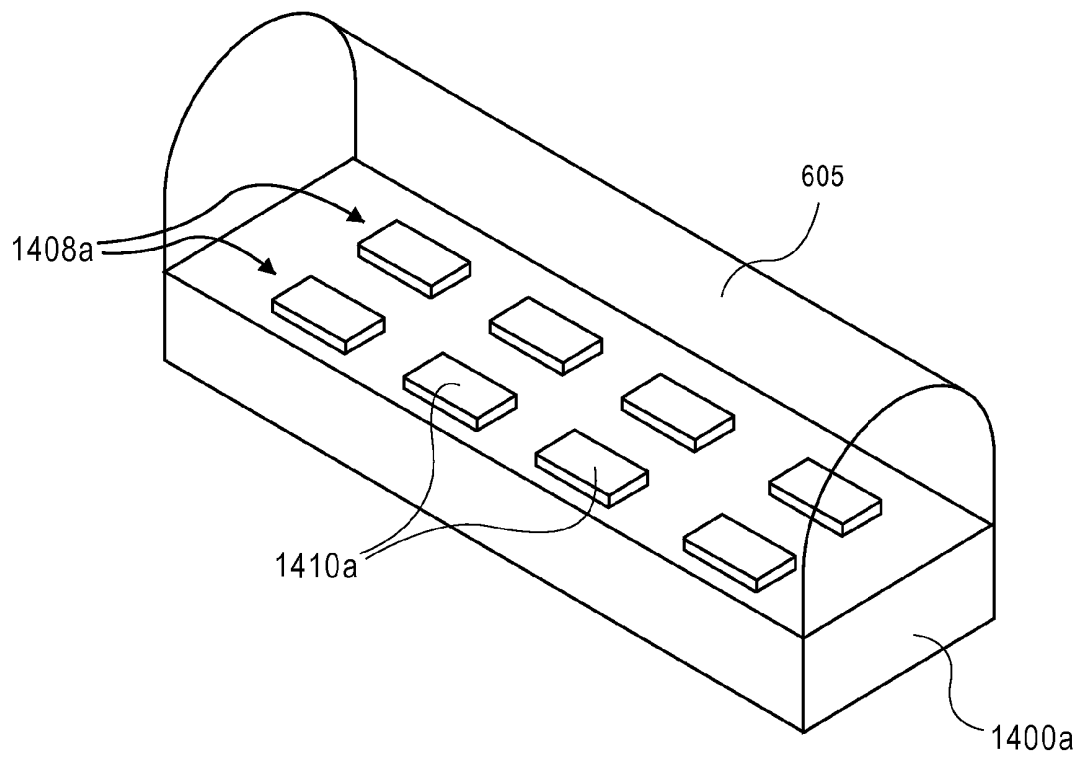**FIG. 14A**

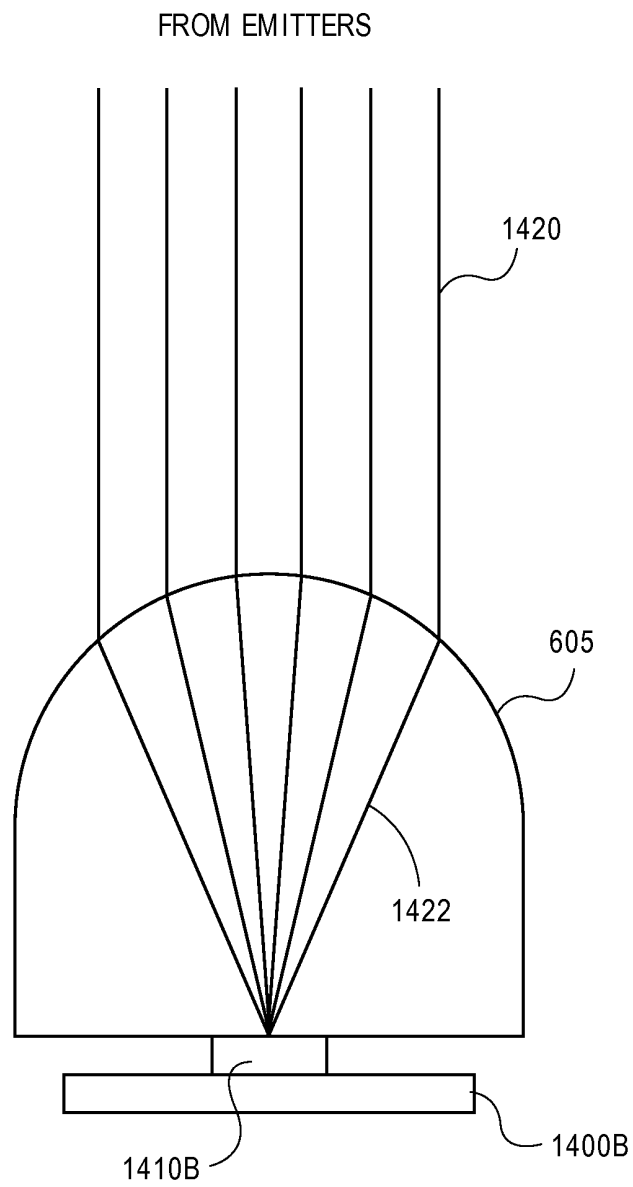
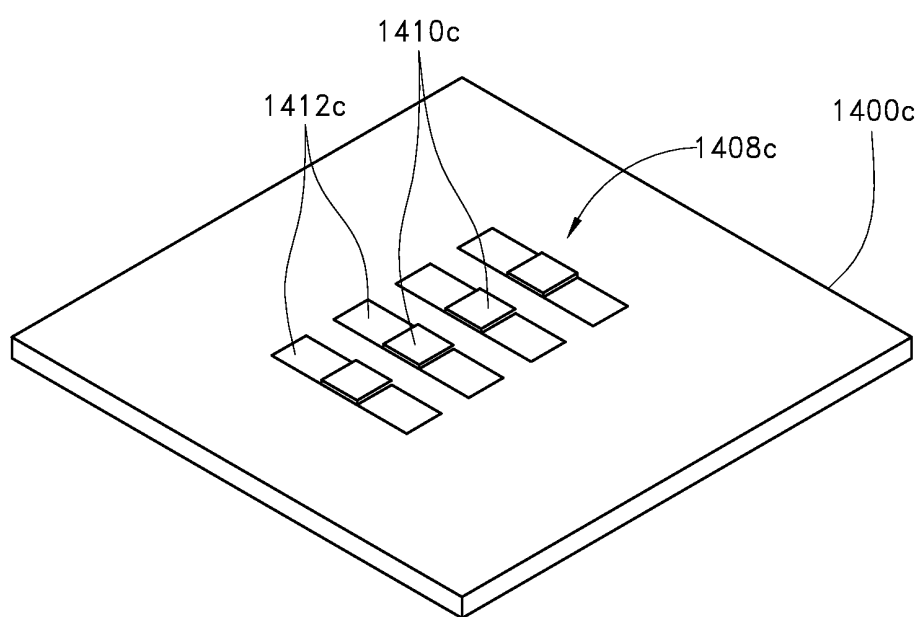
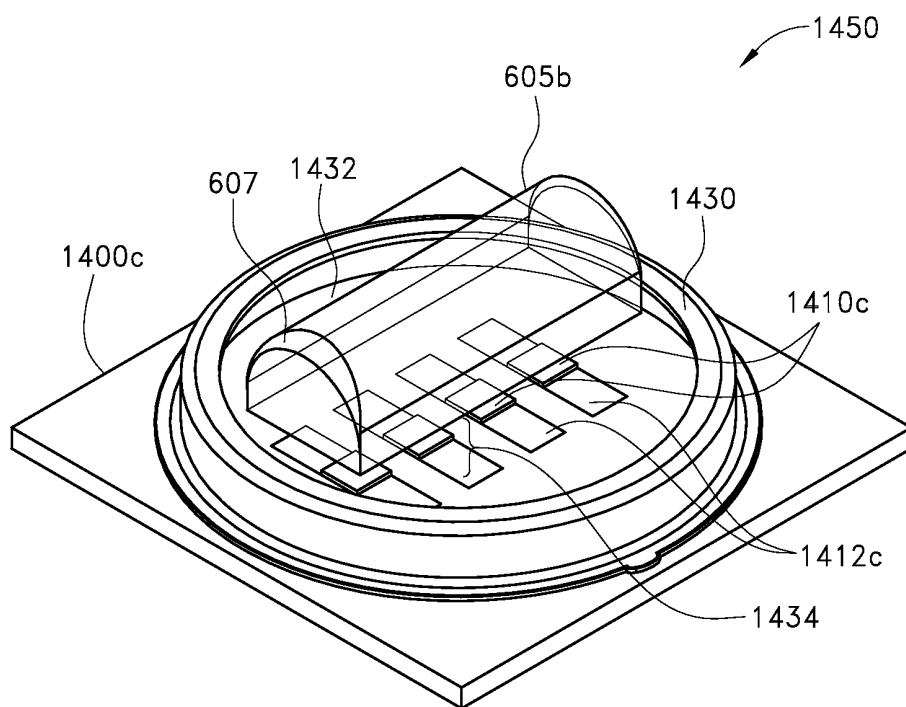


FIG. 14B

**FIG. 14C**

**FIG. 14D**

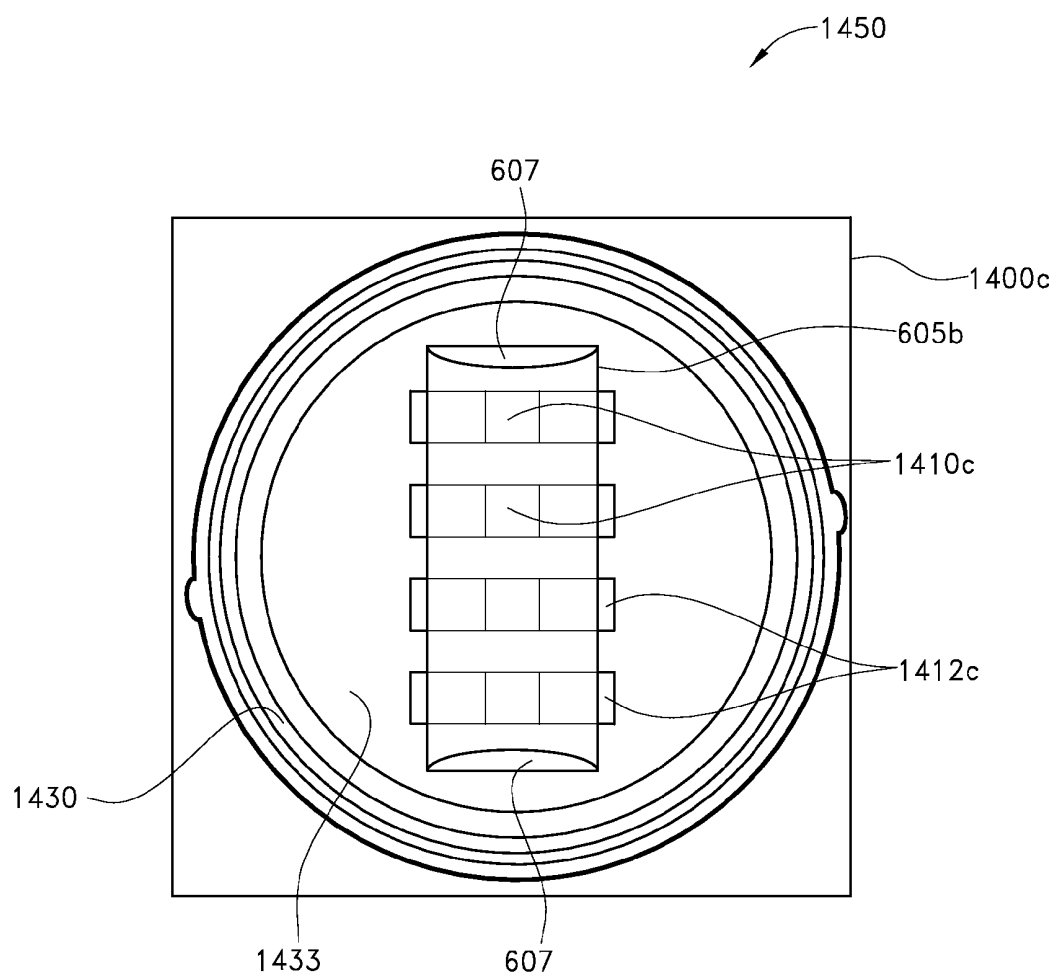
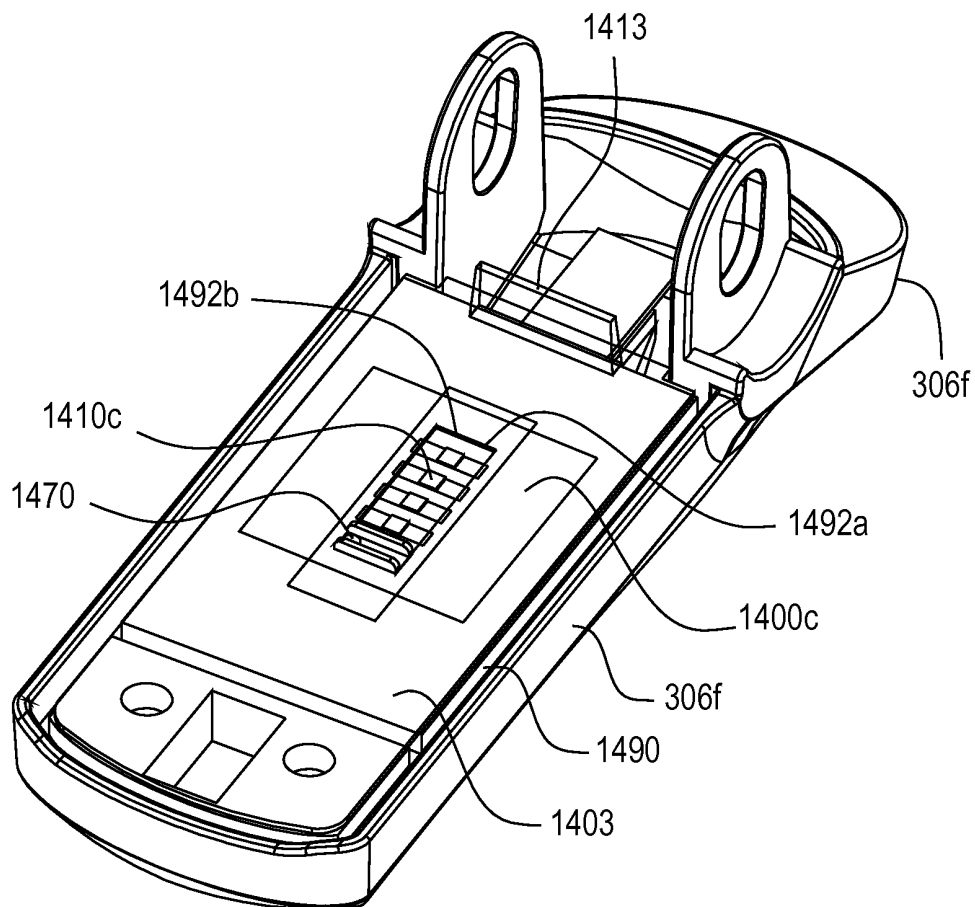


FIG. 14E

**FIG. 14F**

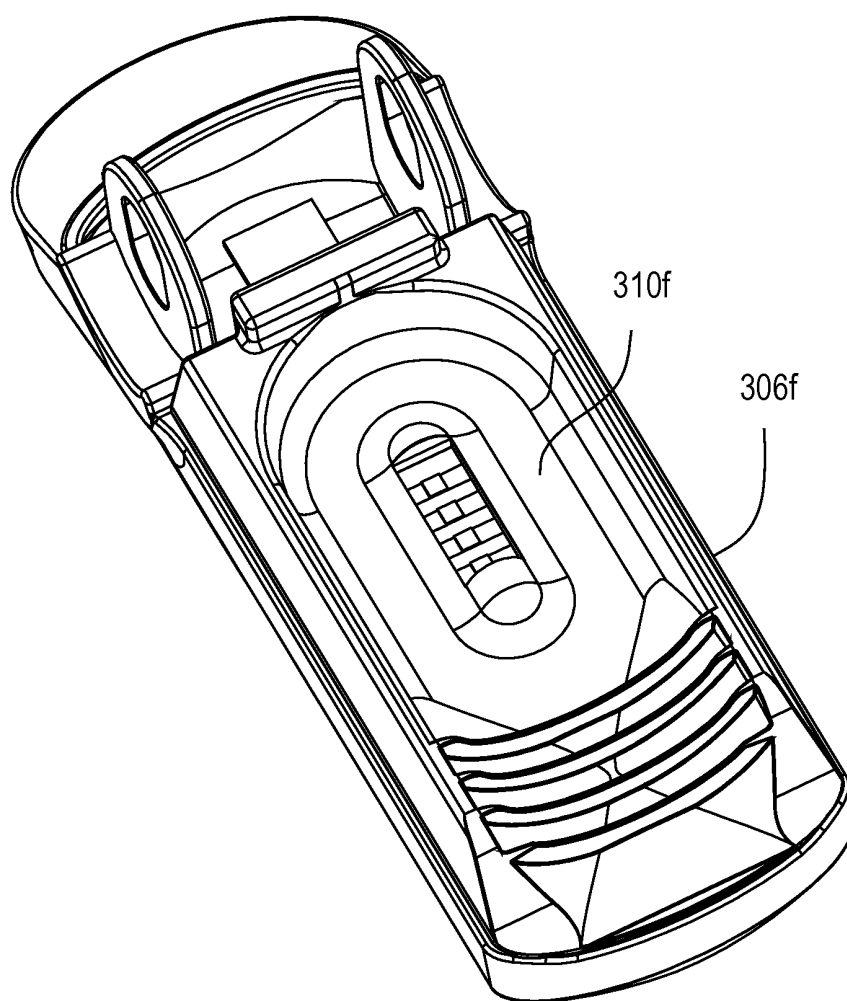


FIG. 14G

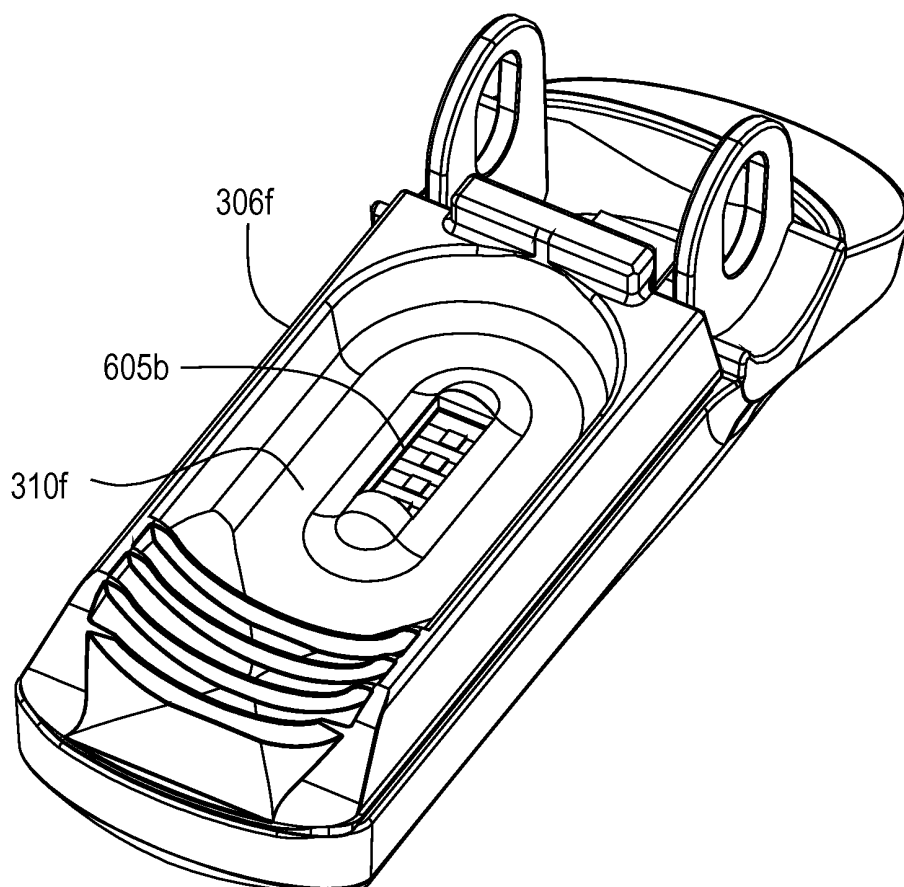
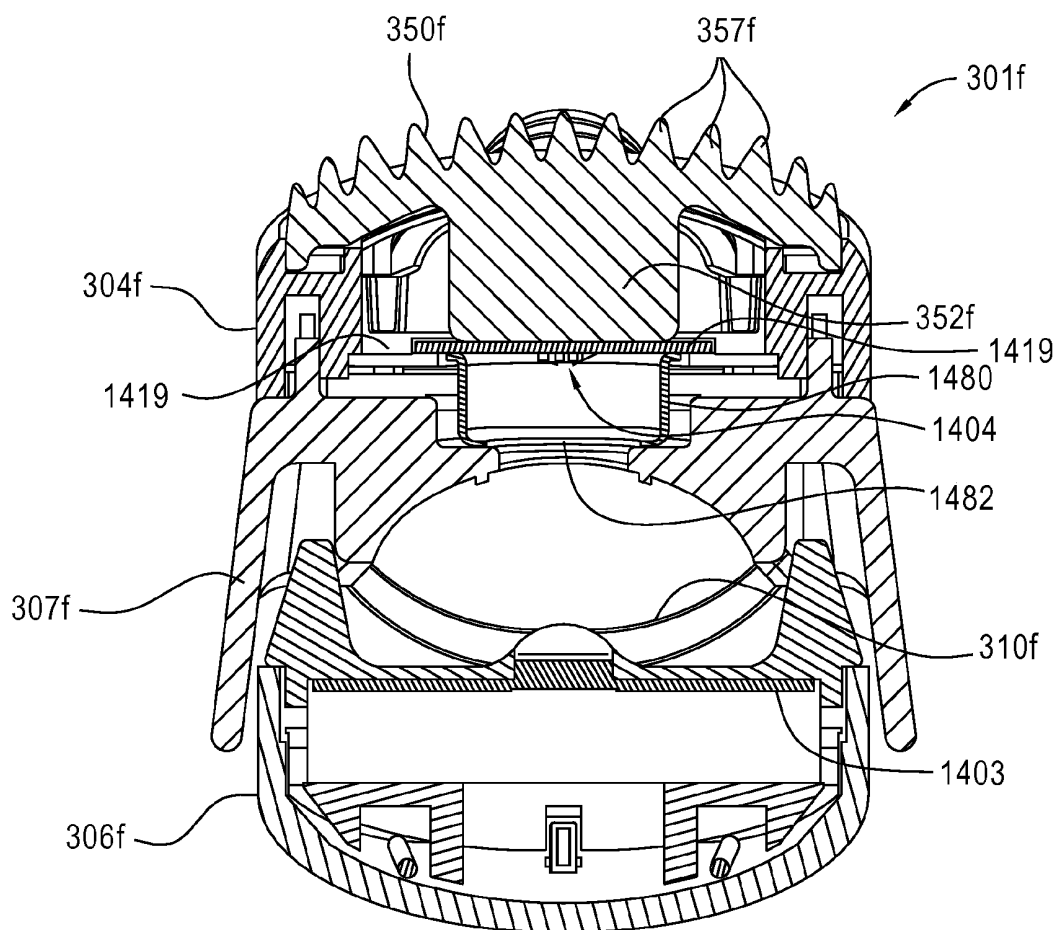


FIG. 14H

**FIG. 14I**

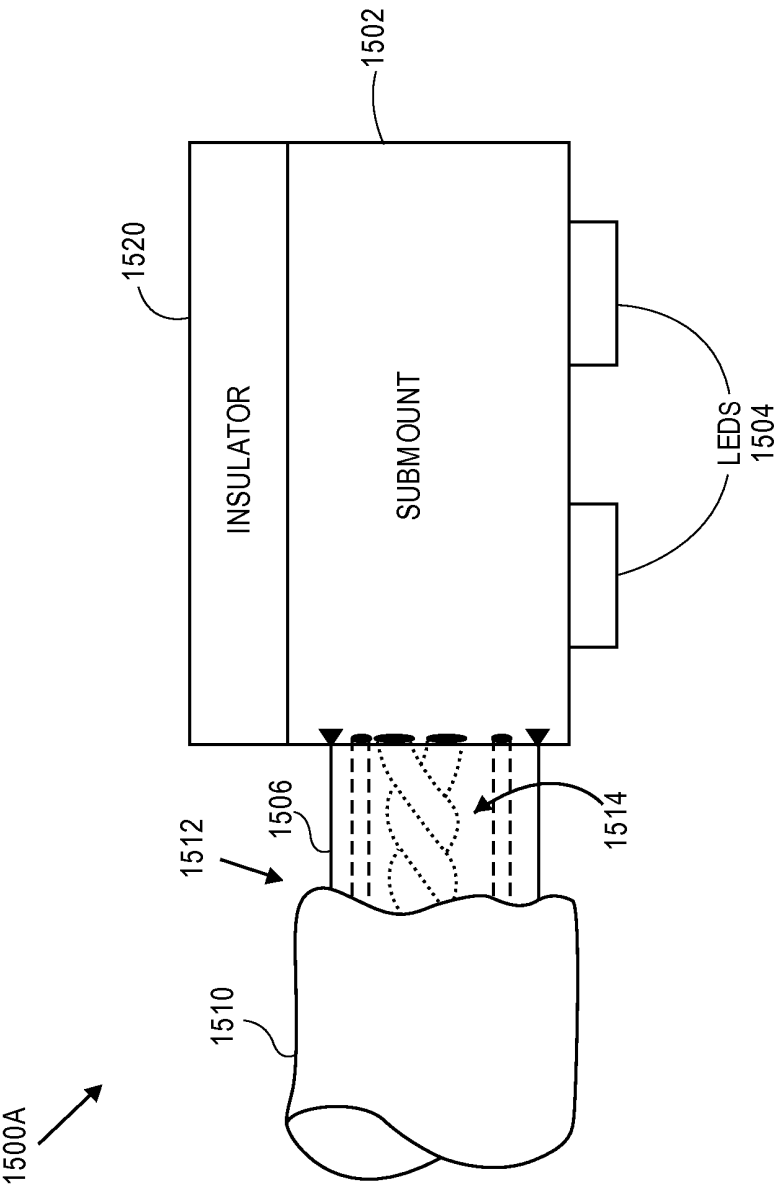


FIG. 15A

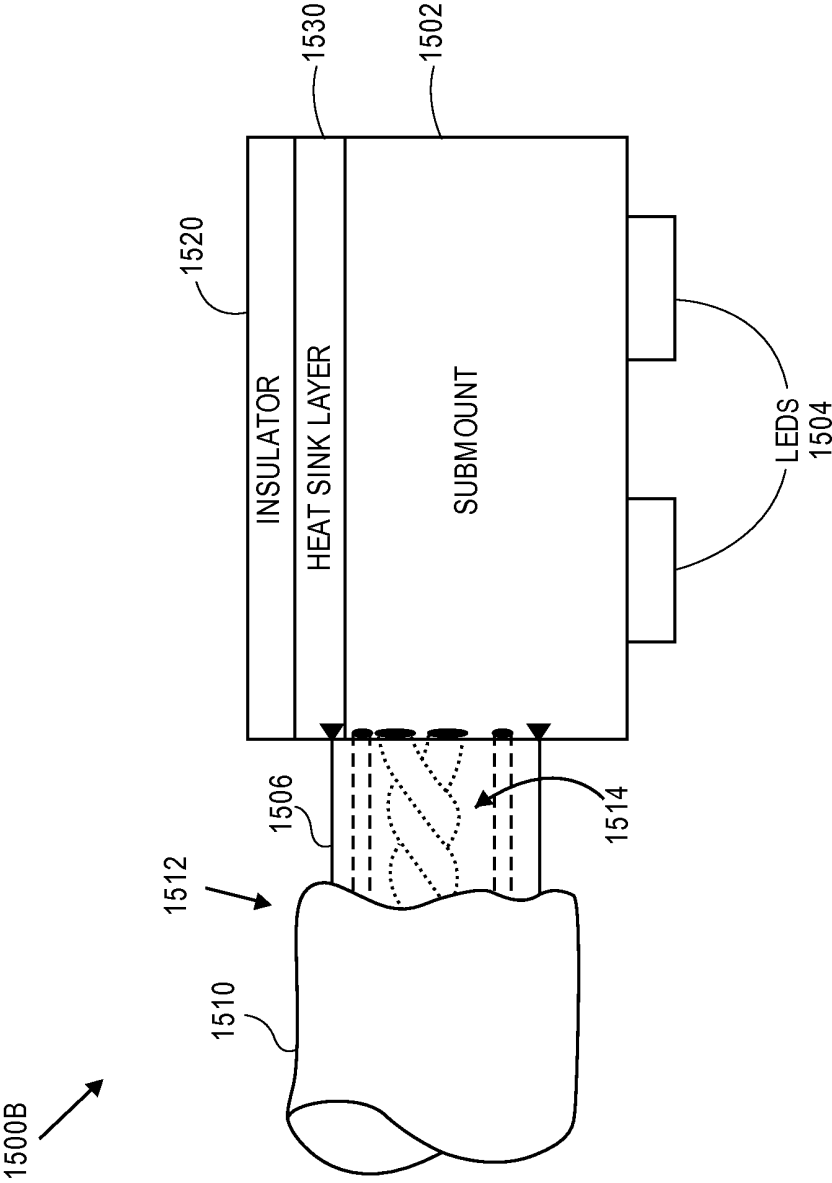


FIG. 15B

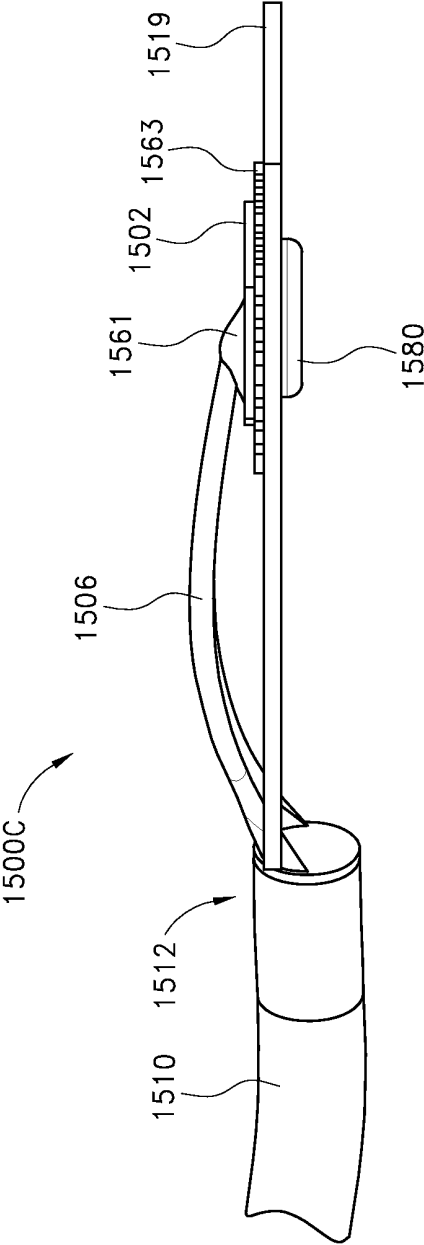


FIG. 15C

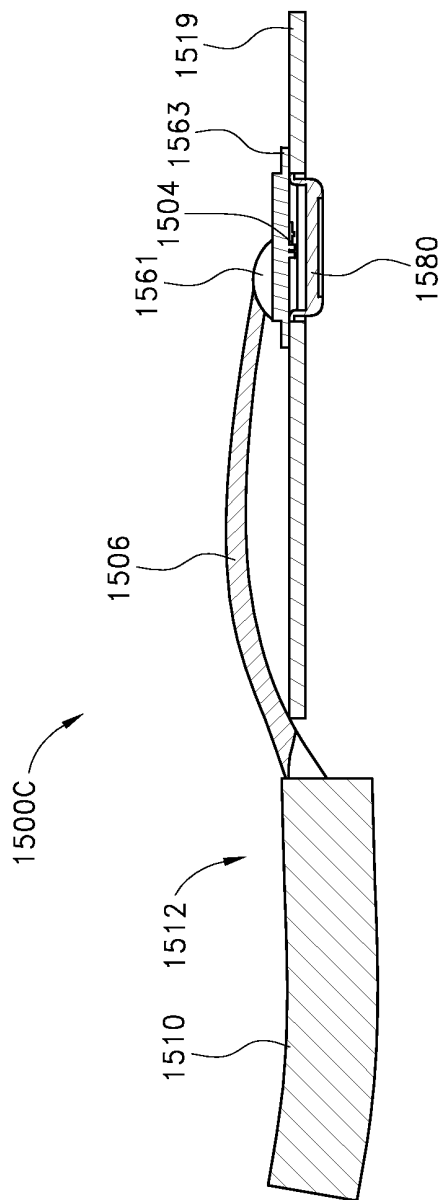


FIG. 15D

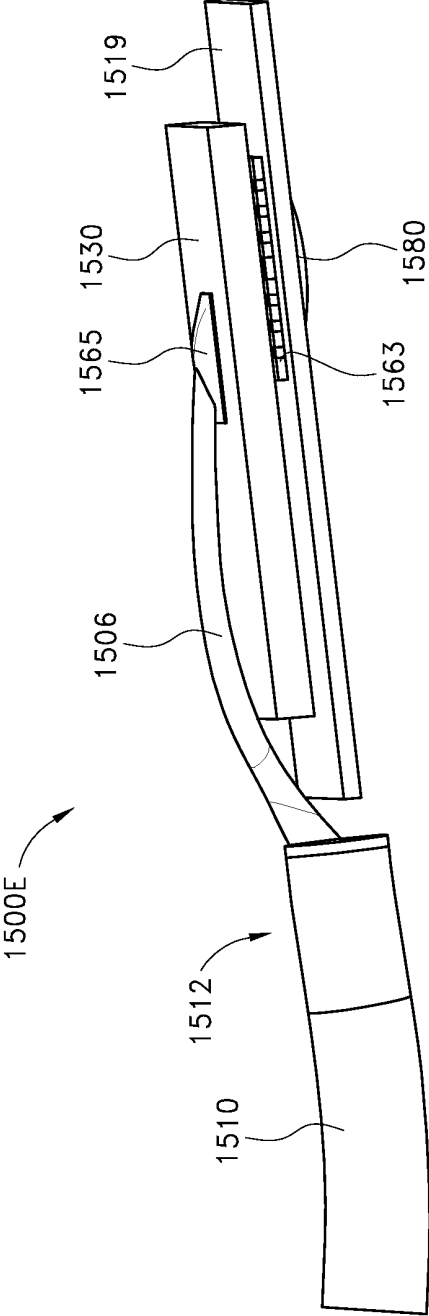


FIG. 15E

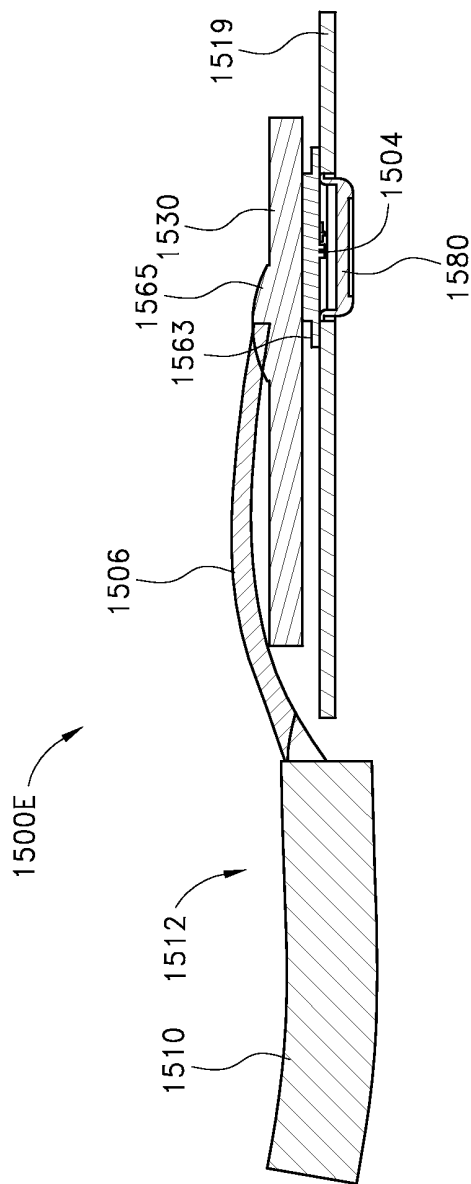


FIG. 15F

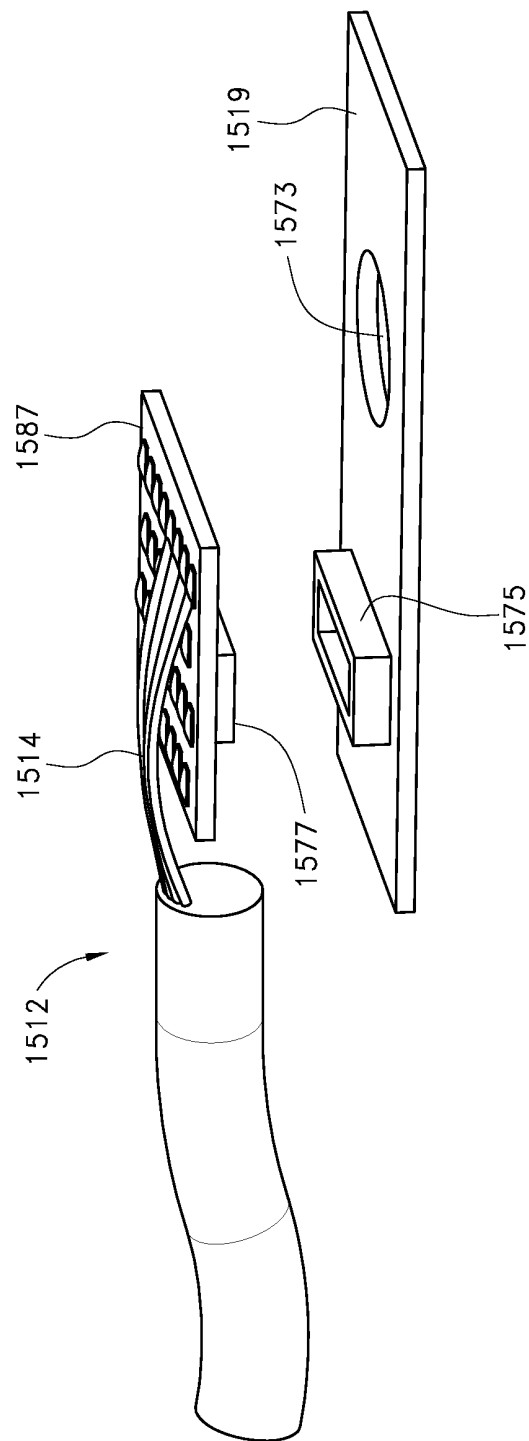


FIG. 15G

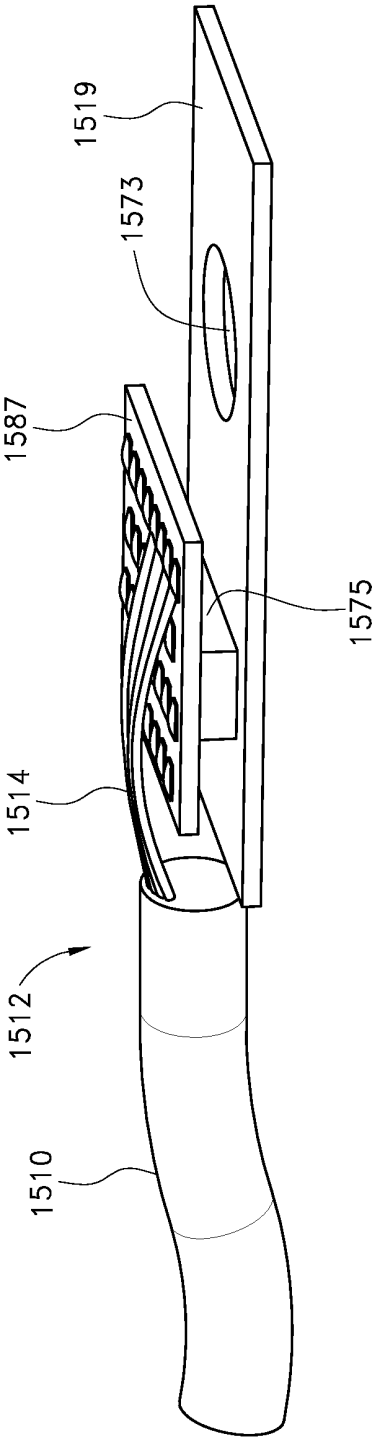


FIG. 15H



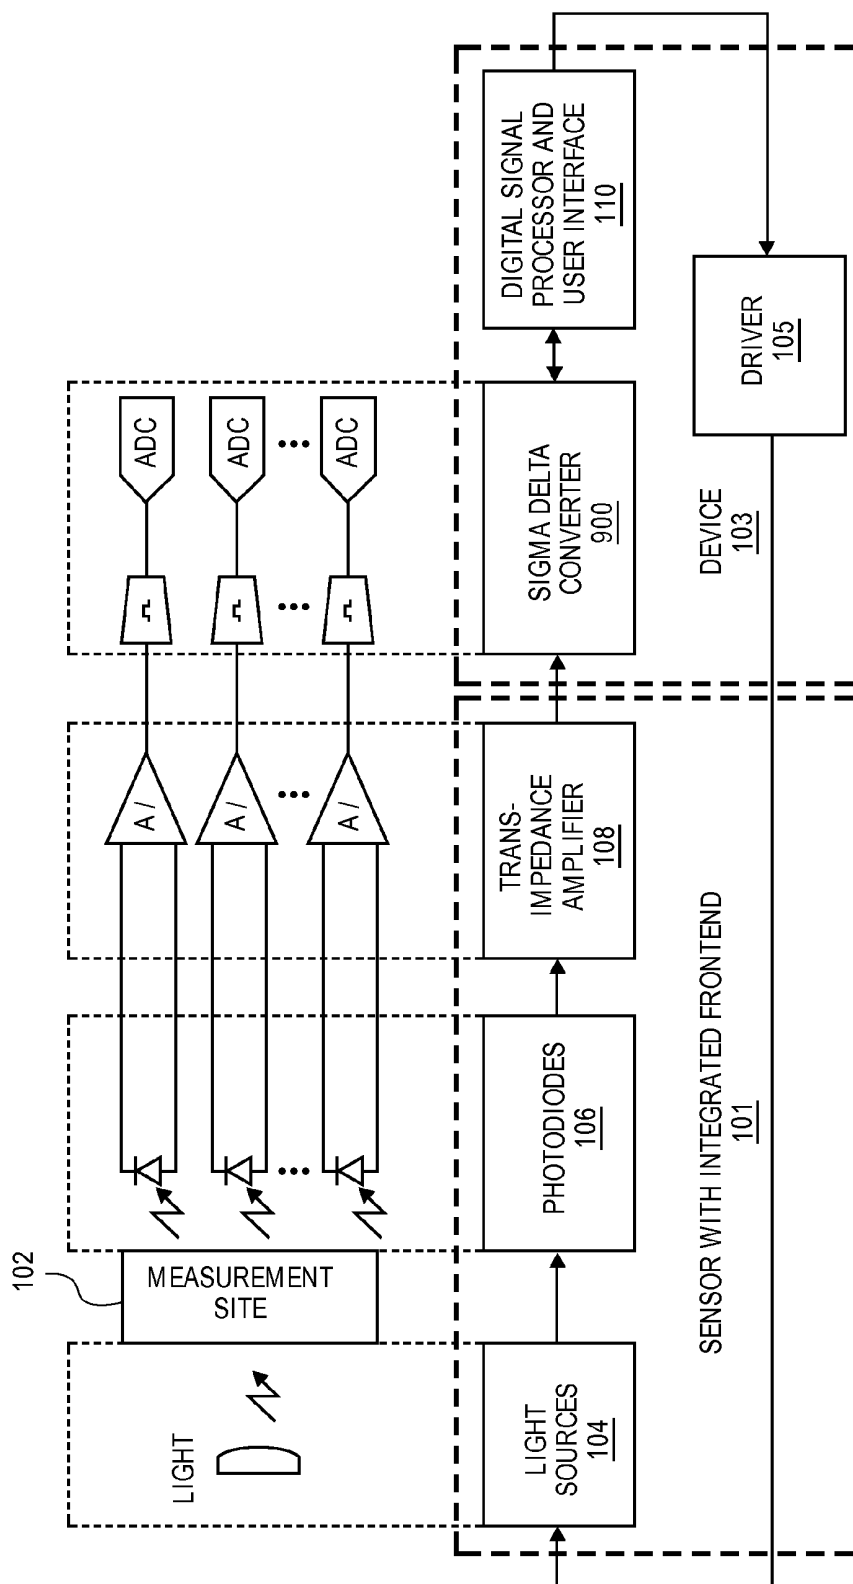


FIG. 15I

**FIG. 15J**

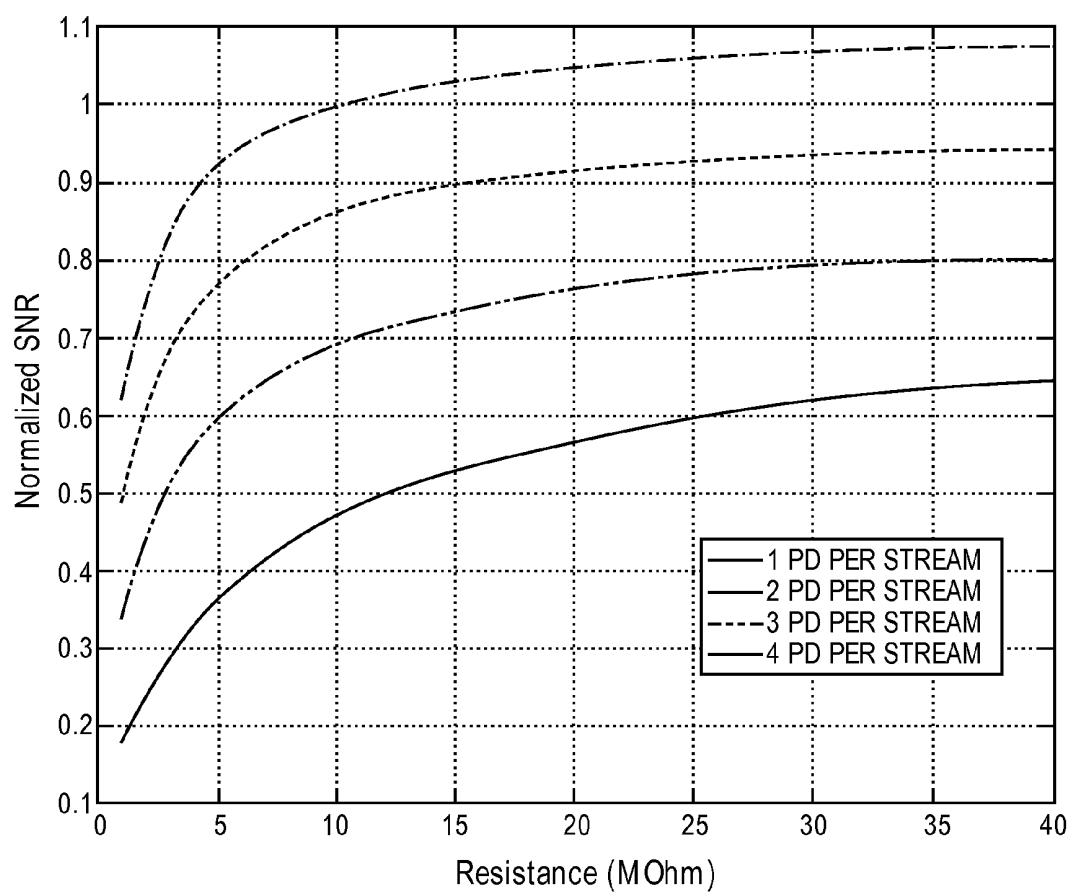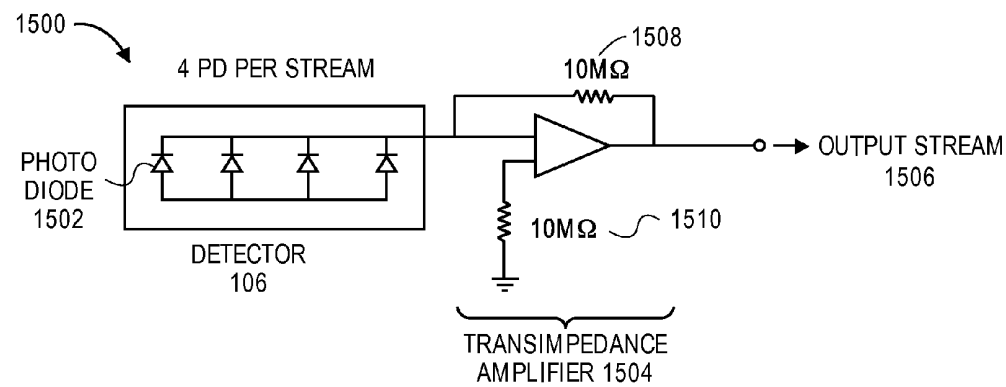

VS.

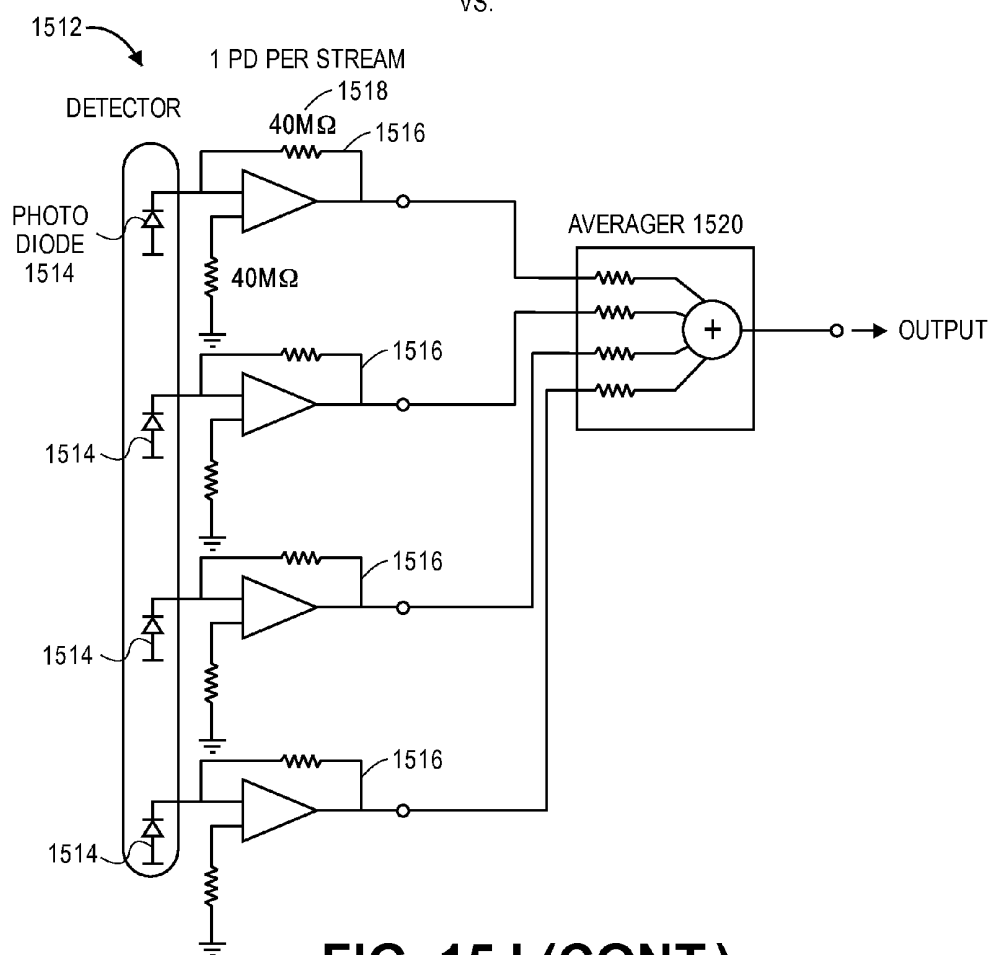


FIG. 15J (CONT.)

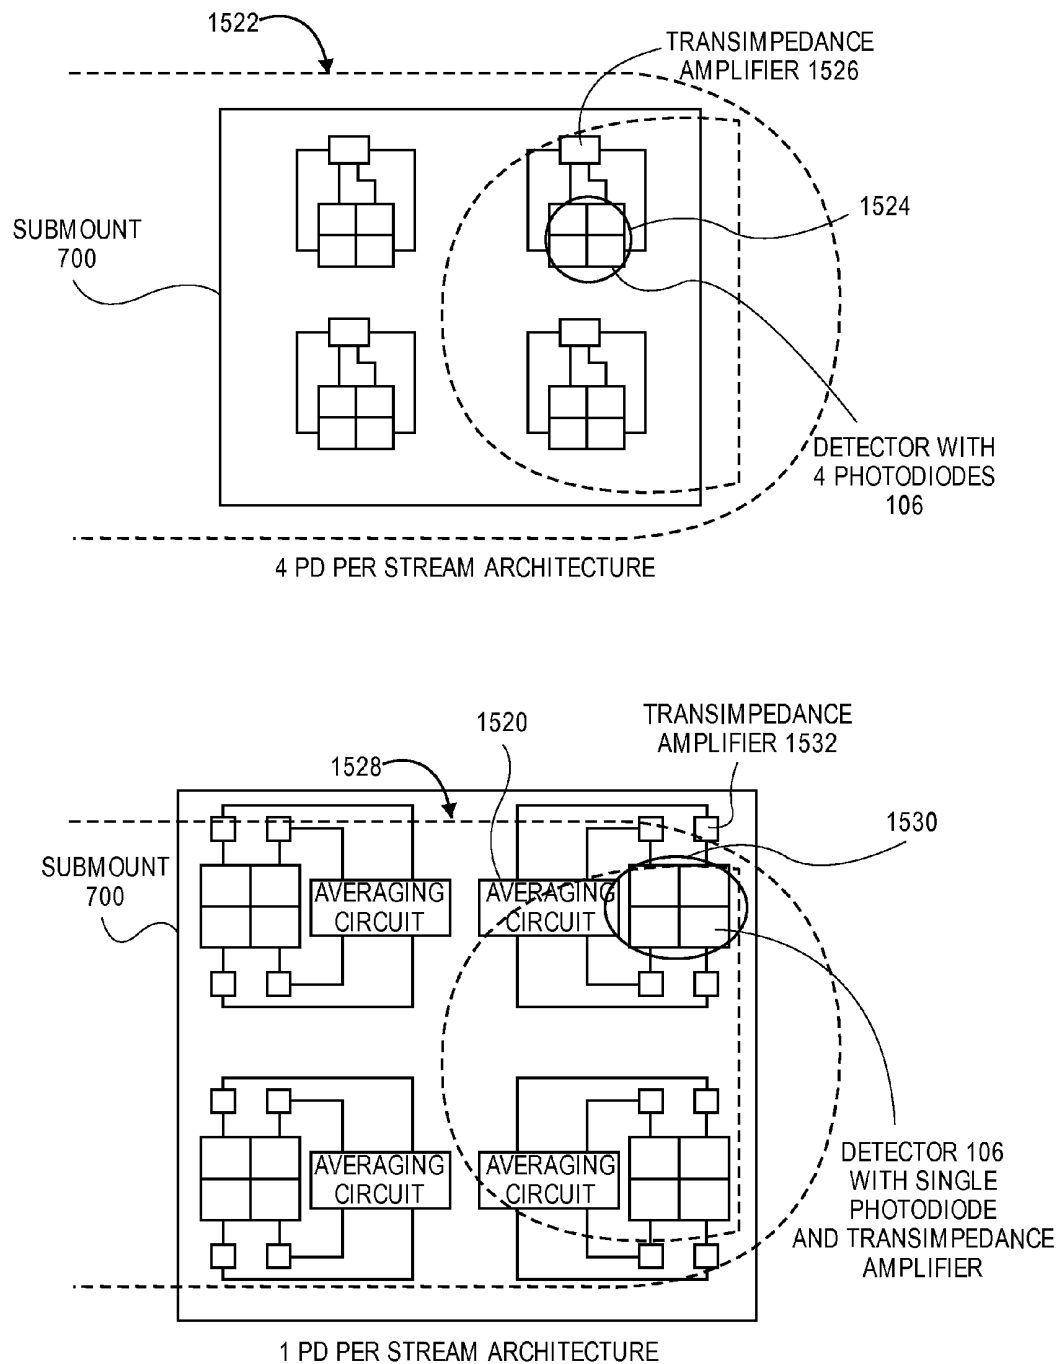
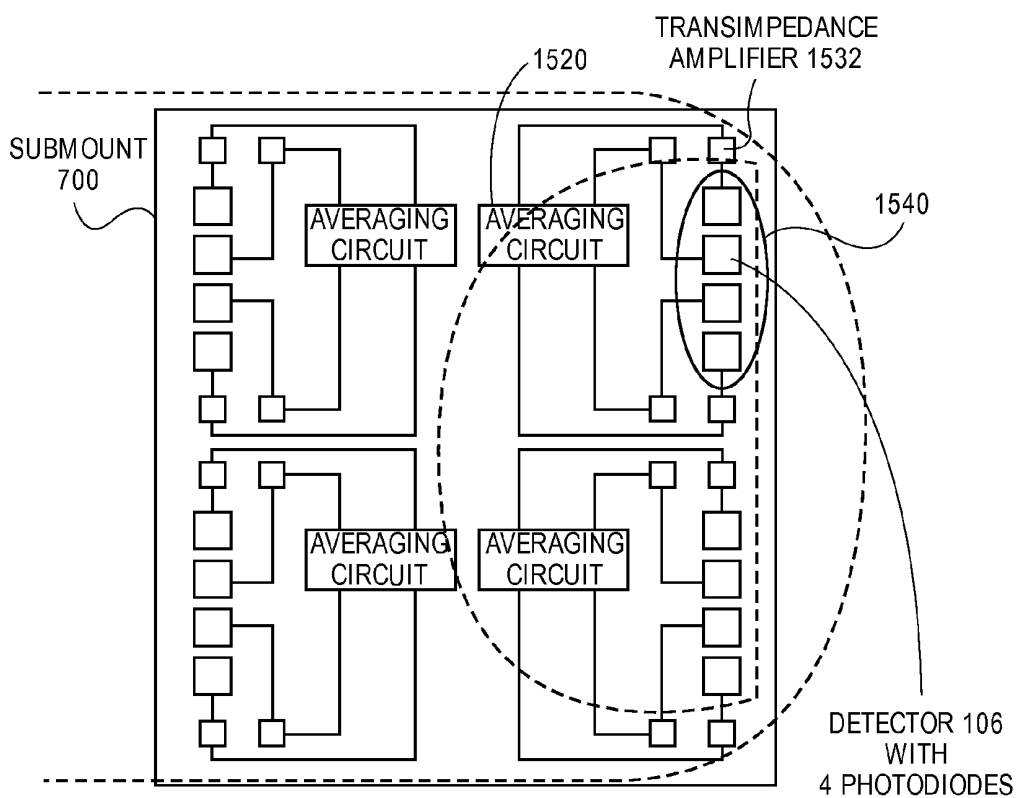
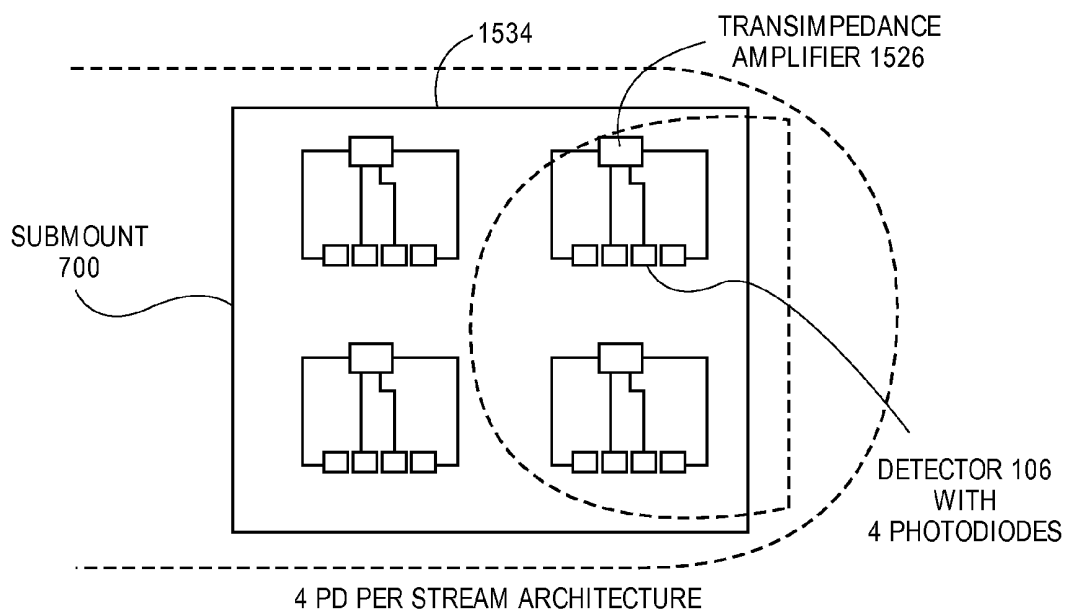
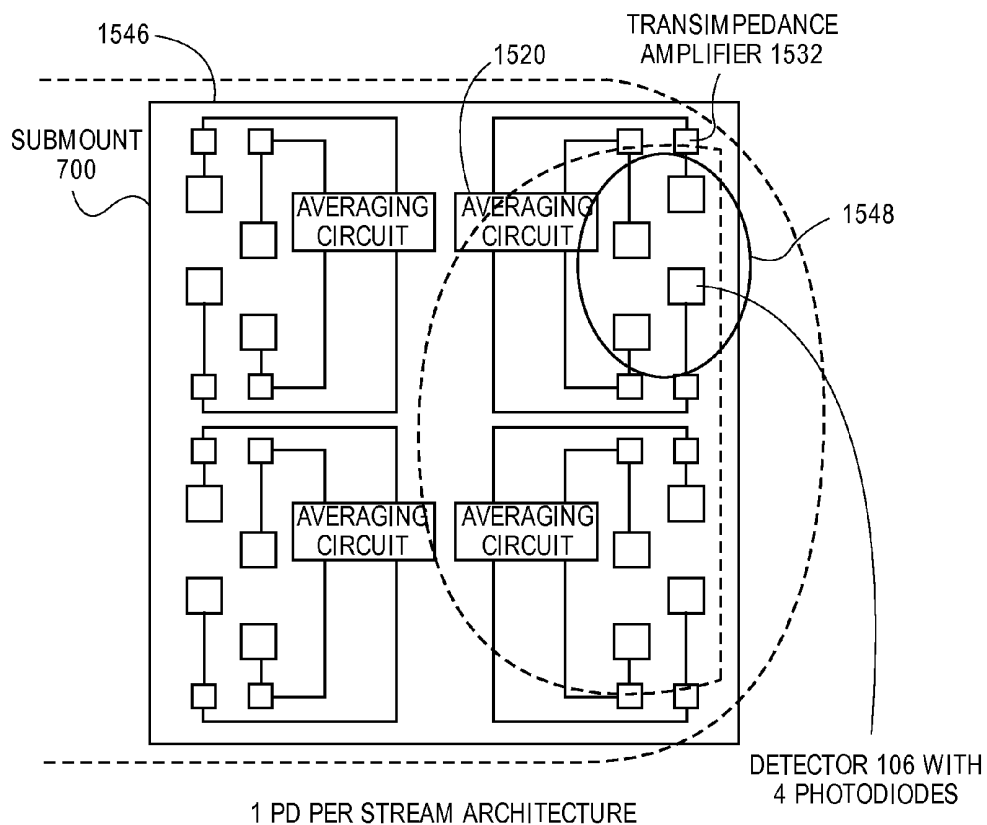
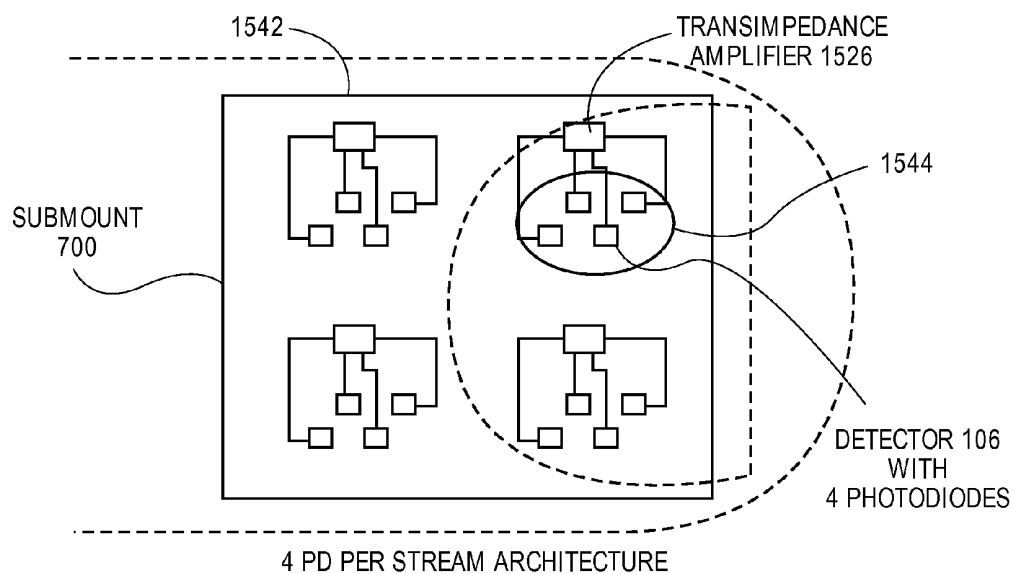


FIG. 15K

**FIG. 15K (CONT.)**

**FIG. 15K (CONT.)**






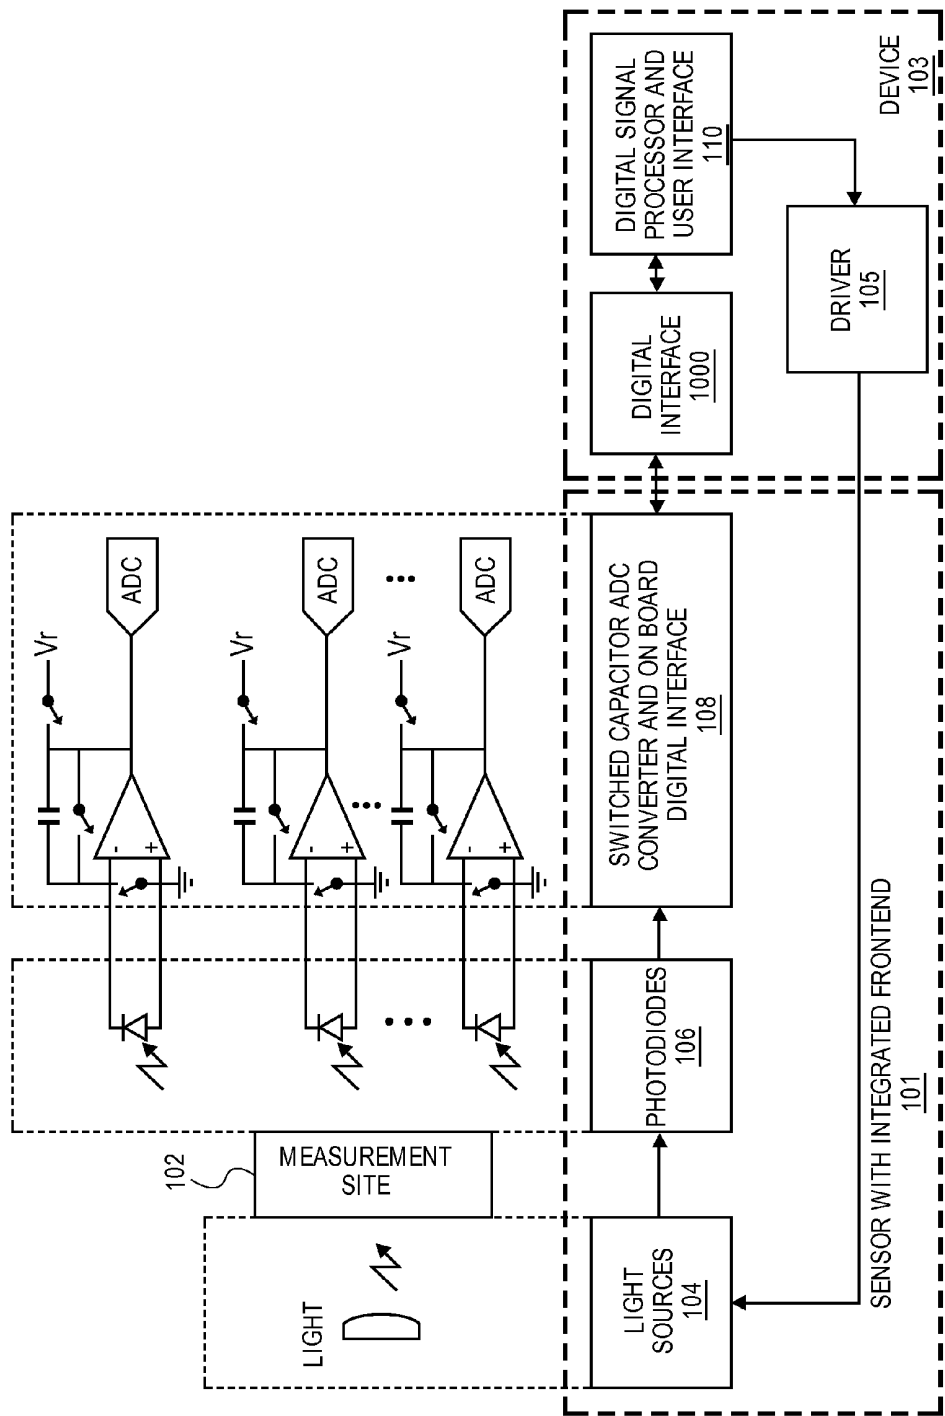



FIG. 15L

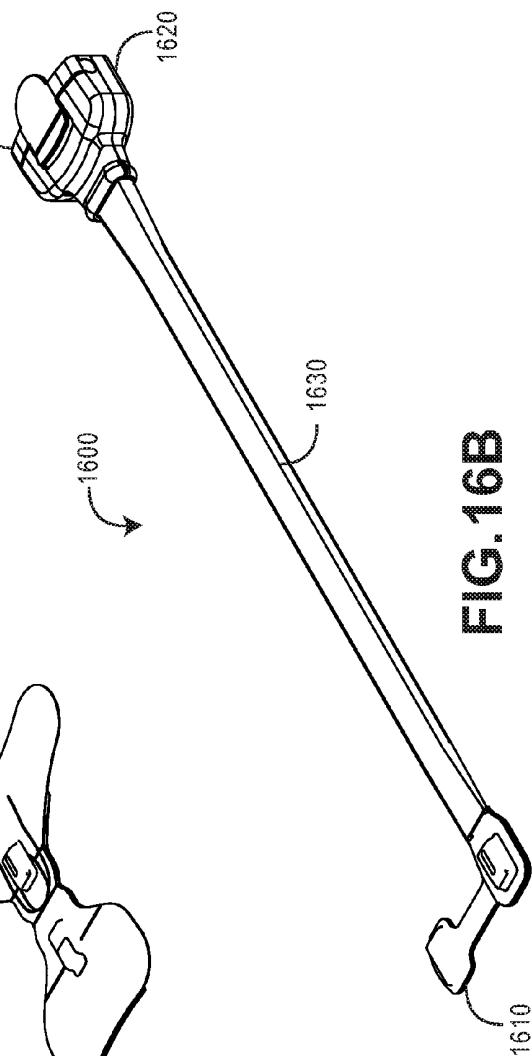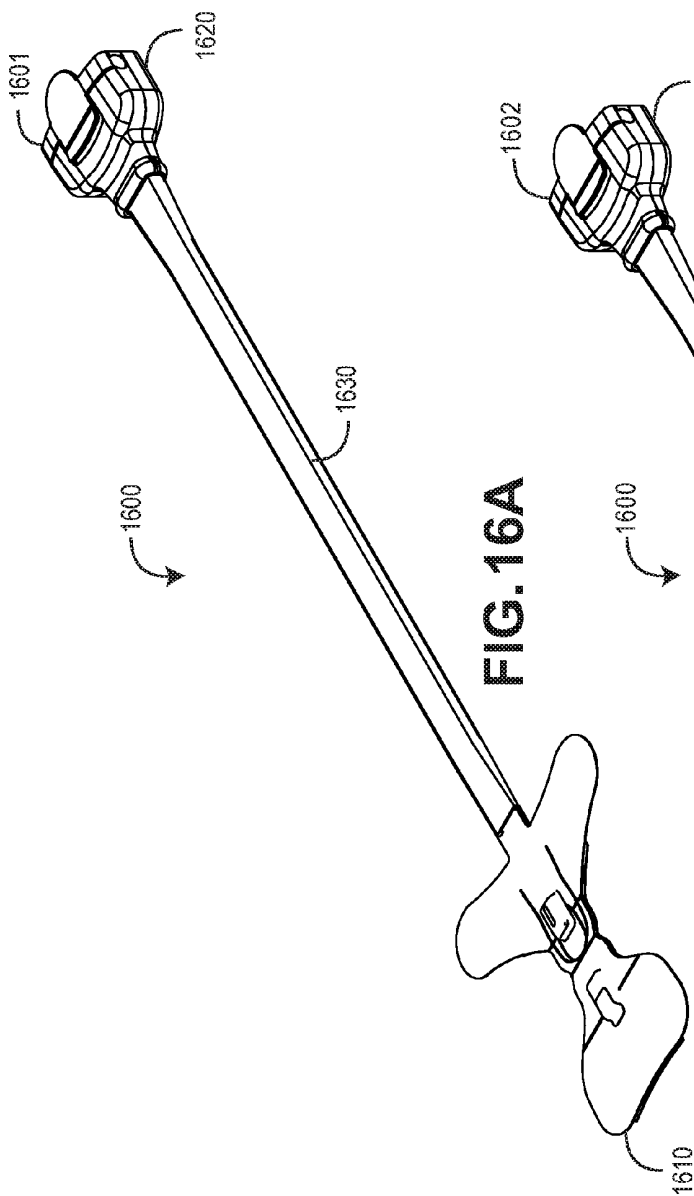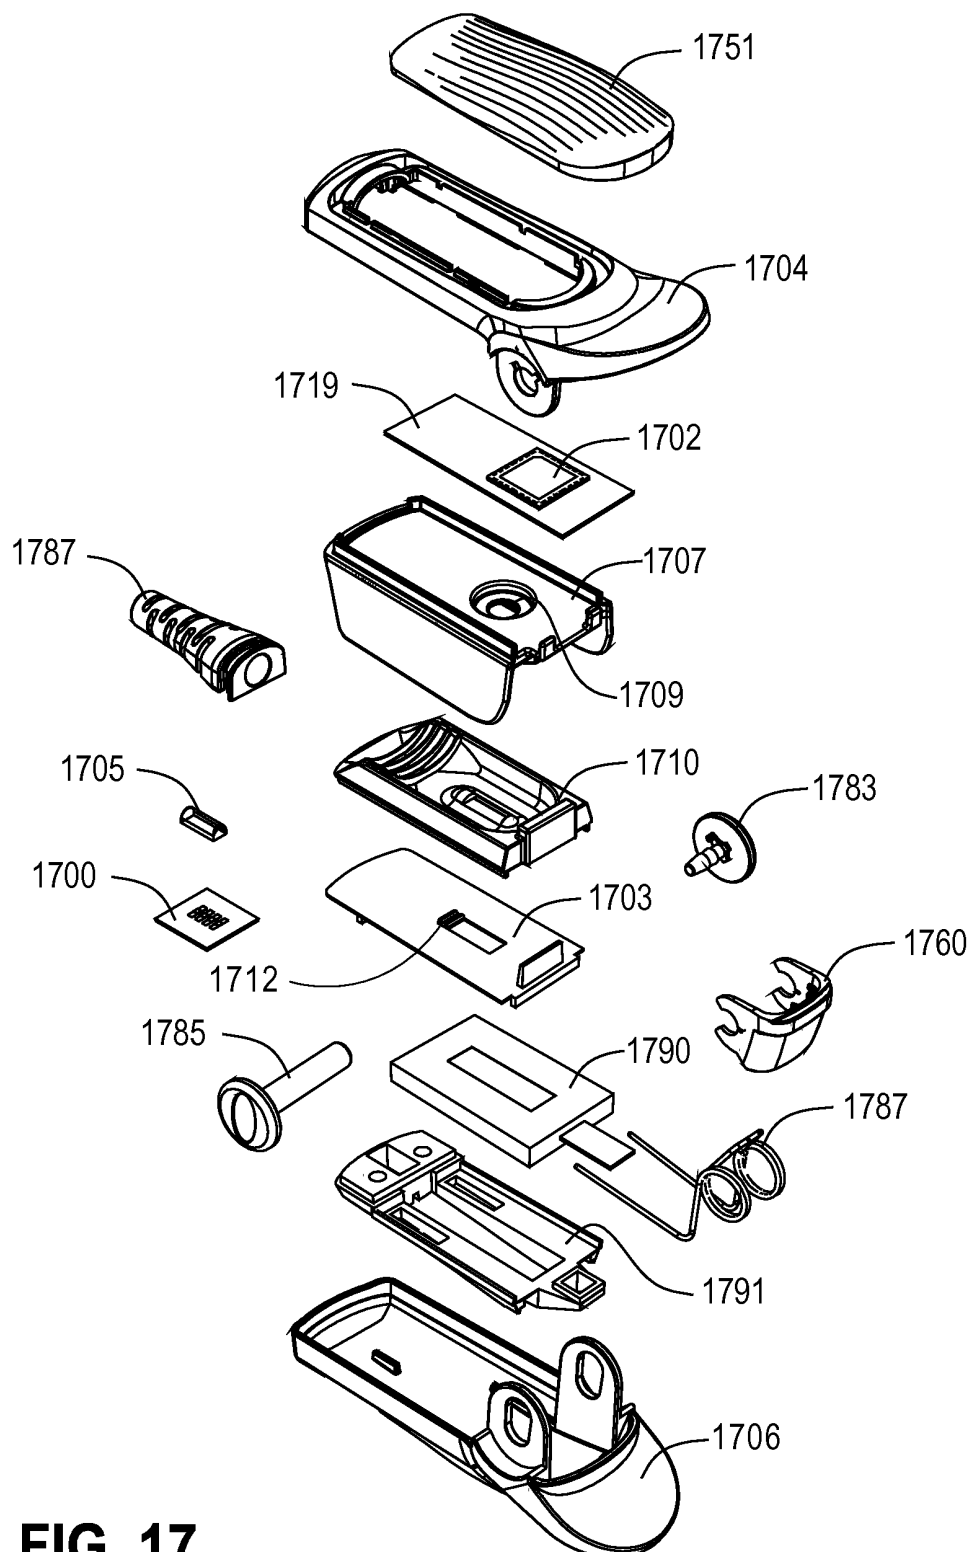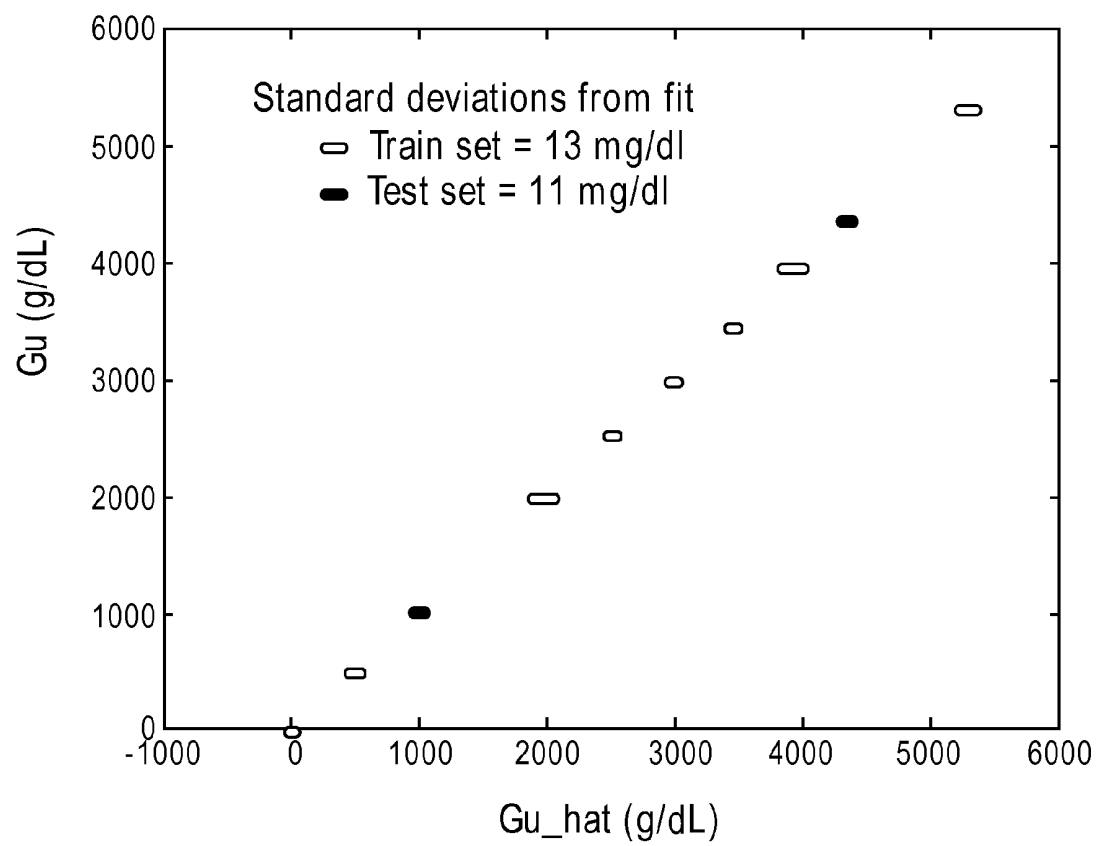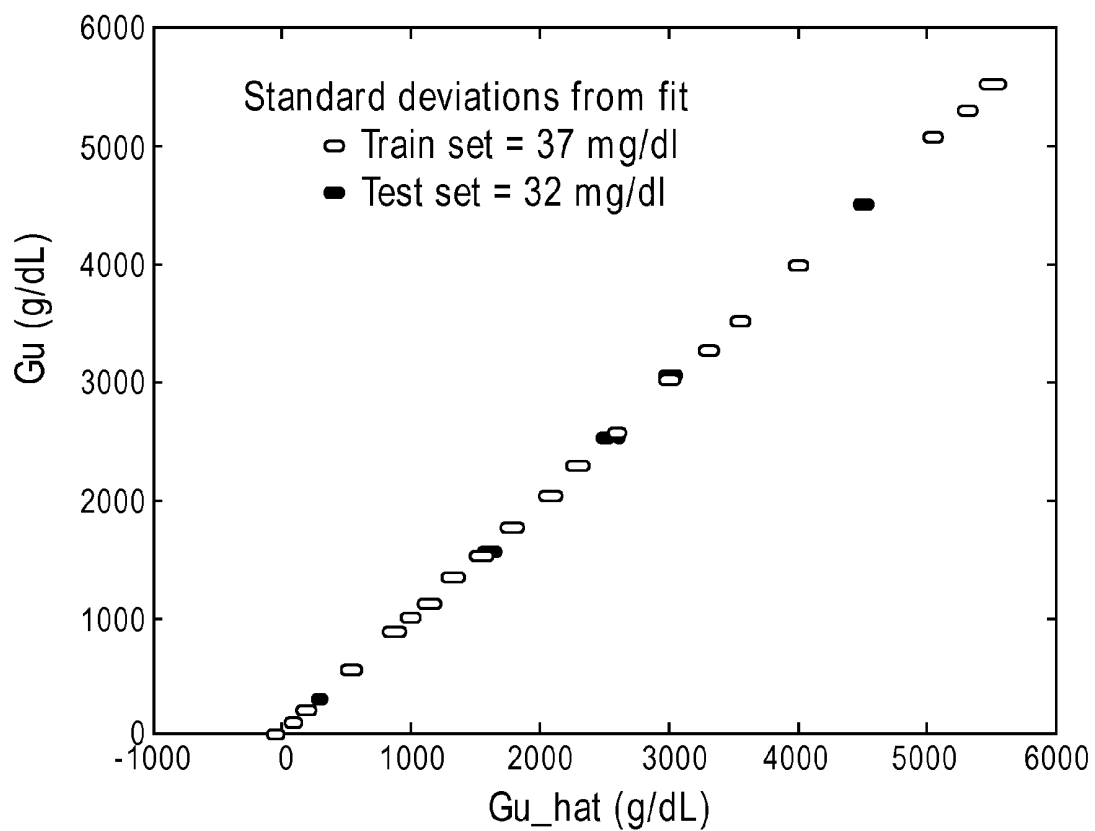



**FIG. 17**

**FIG. 18**

**FIG. 19**

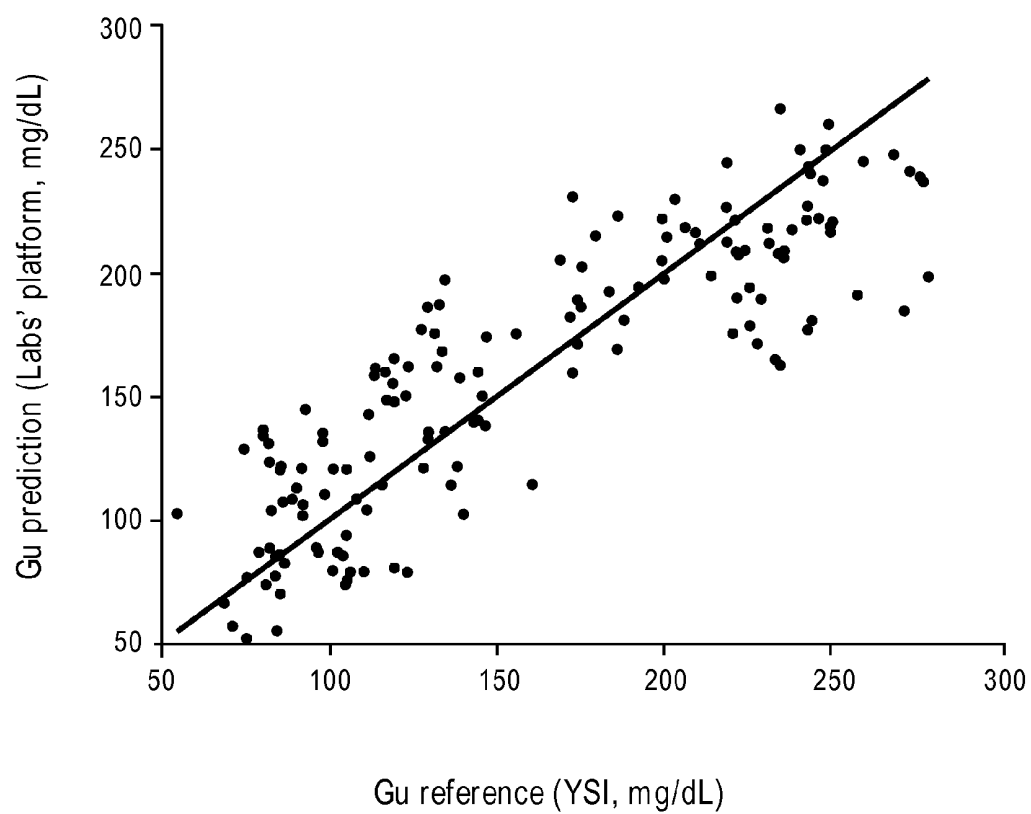**FIG. 20**

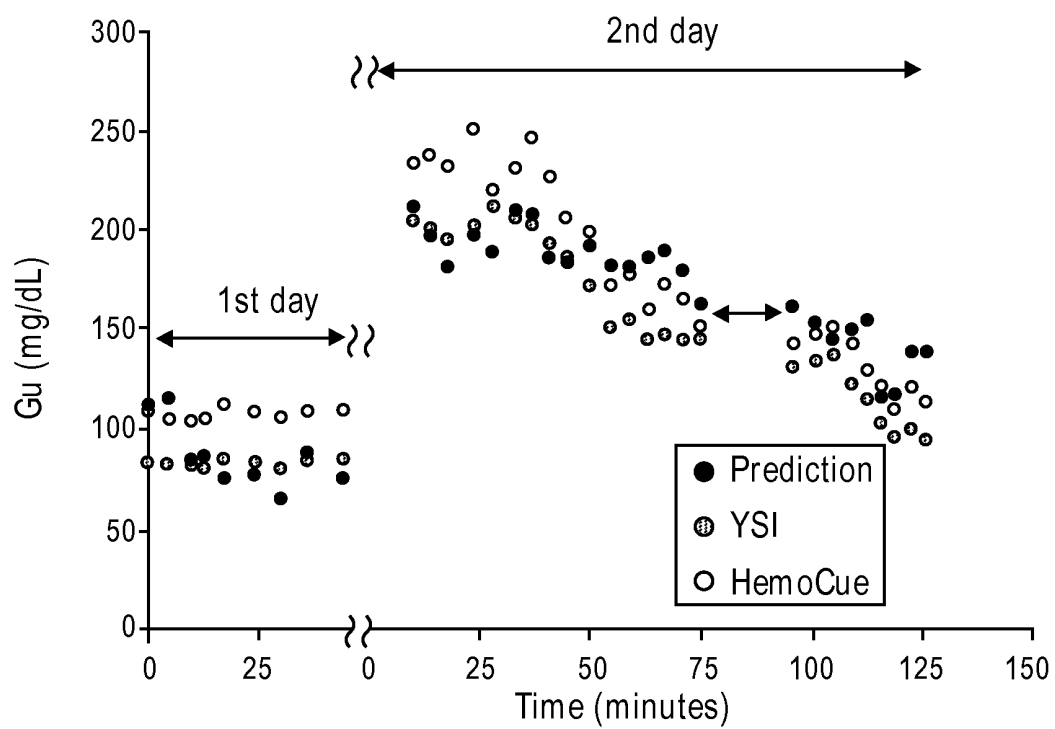**FIG. 21**

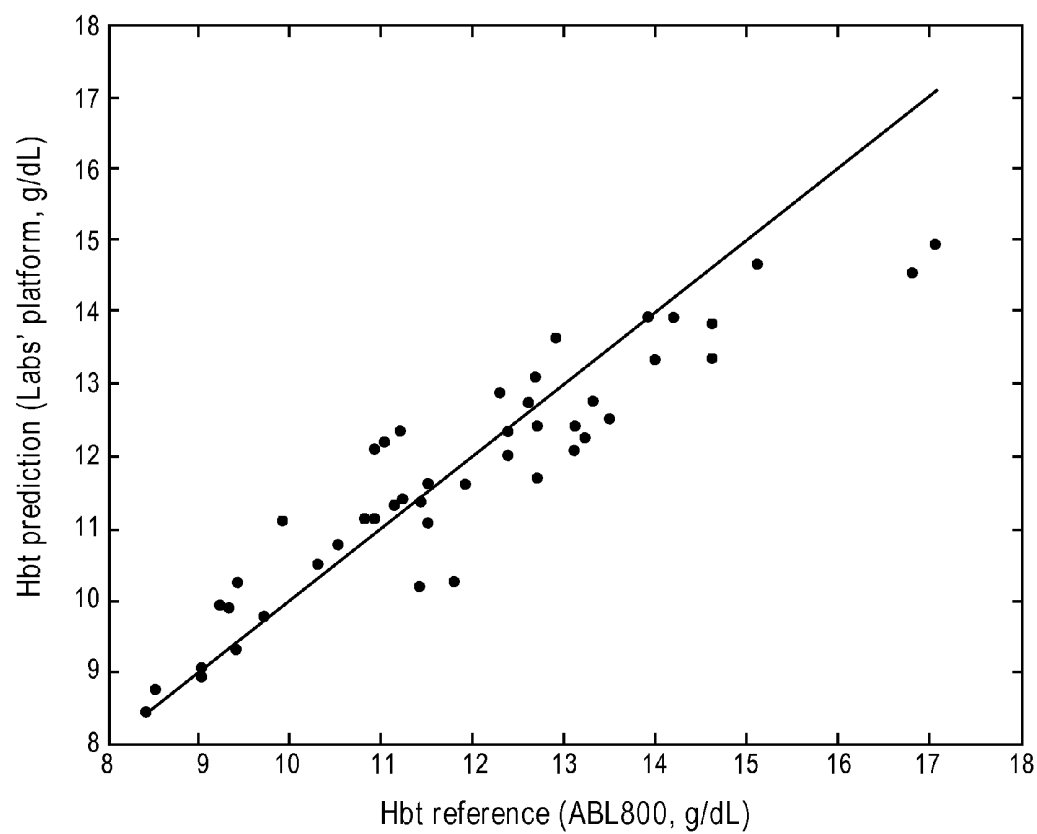**FIG. 22**

1

MULTI-STREAM EMITTER FOR NONINVASIVE MEASUREMENT OF BLOOD CONSTITUENTS

RELATED APPLICATIONS

This application claims the benefit of priority under 35 U.S.C. §119(e) of the following U.S. Provisional Patent Applications:

App. No.	Filing Date	Title	Attorney Docket
61/086,060	Aug. 4, 2008	Multi-Stream Data Collection System For Non-Invasive Measurement of Glucose and Other Analytes	MLHUM.002PR
61/086,108	Aug. 4, 2008	Multi-Stream Sensor Front Ends for Noninvasive Measurement of Glucose and Other Analytes	MLHUM.003PR
61/086,063	Aug. 4, 2008	Multi-Stream Detector For Noninvasive Measurement Of Glucose And Other Analytes	MLHUM.004PR
61/086,057	Aug. 4, 2008	Multi-Stream Emitter For Noninvasive Measurement Of Glucose And Other Analytes	MLHUM.005PR
61/091,732	Aug. 25, 2008	Sensor For Improving Measurement Of Blood Constituents	MLHUM.011PR

This application is related to the following U.S. patent applications:

App. No.	Filing Date	Title	Attorney Docket
12/497,528	Jul. 2, 2009	Noise Shielding for Noninvasive Device Contoured Protrusion for Improving Spectroscopic Measurement of Blood Constituents	MLHUM.006A
12/497,523	Jul. 2, 2009	Heat Sink for Noninvasive Medical Sensor	MLHUM.007A
12/498,506	Jul. 2, 2009	Multi-Stream Data Collection System for Non-Invasive Measurement of Blood Constituents	MLHUM.011A
Unknown	Herewith	Multi-Stream Sensor Front Ends for Non-Invasive Measurement of Blood Constituents	MLHUM.002A
Unknown	Herewith	Multi-Stream Sensor for Non-Invasive Measurement of Blood Constituents	MLHUM.003A
Unknown	Herewith	Multi-Stream Sensor for Non-Invasive Measurement of Blood Constituents	MLHUM.004A

The foregoing applications are hereby incorporated by reference in their entirety.

BACKGROUND

The standard of care in caregiver environments includes patient monitoring through spectroscopic analysis using, for example, a pulse oximeter. Devices capable of spectroscopic analysis generally include a light source(s) transmitting optical radiation into or reflecting off a measurement site, such as, body tissue carrying pulsing blood. After attenuation by tissue and fluids of the measurement site, a photodetection device(s) detects the attenuated light and outputs a detector signal(s) responsive to the detected attenuated light. A signal processing device(s) process the detector(s) signal(s) and outputs a measurement indicative of a blood constituent of inter-

2

est, such as glucose, oxygen, met hemoglobin, total hemoglobin, other physiological parameters, or other data or combinations of data useful in determining a state or trend of wellness of a patient.

In noninvasive devices and methods, a sensor is often adapted to position a finger proximate the light source and light detector. For example, noninvasive sensors often include

a clothespin-shaped housing that includes a contoured bed conforming generally to the shape of a finger.

SUMMARY

The present disclosure relates to noninvasive methods, devices, and systems for measuring a blood analyte, such as glucose. In the present disclosure, blood analytes are measured noninvasively based on multi-stream infrared and near-infrared spectroscopy. In some embodiments, an emitter may include one or more sources that are configured as a point optical source. In addition, the emitter may be operated in a manner that allows for the measurement of an analyte like glucose. In embodiments, the emitter may comprise a plurality of LEDs that emit a sequence of pulses of optical radiation across a spectrum of wavelengths. In addition, in order to achieve the desired SNR for detecting analytes like glucose, the emitter may be driven using a progression from low power to higher power. The emitter may also have its duty cycle modified to achieve a desired SNR.

In an embodiment, a multi-stream emitter for a noninvasive, physiological device configured to transmit optical

radiation in a tissue site comprises: a set of optical sources arranged as a point optical source; and a driver configured to drive the at least one light emitting diode and at least one optical source to transmit near-infrared optical radiation at sufficient power to measure an analyte in tissue that responds to near-infrared optical radiation.

In an embodiment, an emitter for a noninvasive, physiological device configured to transmit optical radiation in a tissue site comprises: a point optical source comprising an optical source configured to transmit infrared and near-infrared optical radiation to a tissue site; and a driver configured to drive the point optical source at a sufficient power and noise tolerance to effectively provide attenuated optical radiation from a tissue site that indicates an amount of glucose in the tissue site.

In an embodiment, a method of transmitting a stream of pulses of optical radiation in a tissue site is provided. At least one pulse of infrared optical radiation having a first pulse width is transmitted at a first power. At least one pulse of near-infrared optical radiation is transmitted at a power that is higher than the first power.

In an embodiment, a method of transmitting a stream of pulses of optical radiation in a tissue site is provided. At least one pulse of infrared optical radiation having a first pulse width is transmitted at a first power. At least one pulse of near-infrared optical radiation is then transmitted, at a second power that is higher than the first power.

For purposes of summarizing the disclosure, certain aspects, advantages and novel features of the inventions have been described herein. It is to be understood that not necessarily all such advantages can be achieved in accordance with any particular embodiment of the inventions disclosed herein. Thus, the inventions disclosed herein can be embodied or carried out in a manner that achieves or optimizes one advantage or group of advantages as taught herein without necessarily achieving other advantages as can be taught or suggested herein.

BRIEF DESCRIPTION OF THE DRAWINGS

Throughout the drawings, reference numbers can be re-used to indicate correspondence between referenced elements. The drawings are provided to illustrate embodiments of the inventions described herein and not to limit the scope thereof.

FIG. 1 illustrates a block diagram of an example data collection system capable of noninvasively measuring one or more blood analytes in a monitored patient, according to an embodiment of the disclosure;

FIGS. 2A-2D illustrate an exemplary handheld monitor and an exemplary noninvasive optical sensor of the patient monitoring system of FIG. 1, according to embodiments of the disclosure;

FIGS. 3A-3C illustrate side and perspective views of an exemplary noninvasive sensor housing including a finger bed protrusion and heat sink, according to an embodiment of the disclosure;

FIG. 3D illustrates a side view of another example noninvasive sensor housing including a heat sink, according to an embodiment of the disclosure;

FIG. 3E illustrates a perspective view of an example noninvasive sensor detector shell including example detectors, according to an embodiment of the disclosure;

FIG. 3F illustrates a side view of an example noninvasive sensor housing including a finger bed protrusion and heat sink, according to an embodiment of the disclosure;

FIGS. 4A through 4C illustrate top elevation, side and top perspective views of an example protrusion, according to an embodiment of the disclosure;

FIG. 5 illustrates an example graph depicting possible effects of a protrusion on light transmittance, according to an embodiment of the disclosure;

FIGS. 6A through 6D illustrate perspective, front elevation, side and top views of another example protrusion, according to an embodiment of the disclosure;

FIG. 6E illustrates an example sensor incorporating the protrusion of FIGS. 6A through 6D, according to an embodiment of the disclosure;

FIGS. 7A through 7B illustrate example arrangements of conductive glass that may be employed in the system of FIG. 1, according to embodiments of the disclosure.

FIGS. 8A through 8D illustrate an example top elevation view, side views, and a bottom elevation view of the conductive glass that may be employed in the system of FIG. 1, according to embodiments of the disclosure;

FIG. 9 shows example comparative results obtained by an embodiment of a sensor;

FIGS. 10A and 10B illustrate comparative noise floors of various embodiments of the present disclosure;

FIG. 11A illustrates a block diagram of some of the components that may include an embodiment of a sensor, according to an embodiment of the disclosure;

FIG. 11B illustrates a configuration of emitting optical radiation into a measurement site for measuring blood constituents, according to an embodiment of the disclosure;

FIG. 11C illustrates another exemplary emitter that may be employed in the sensor according to an embodiment of the disclosure;

FIG. 11D illustrates another exemplary emitter that may be employed in the sensor according to an embodiment of the disclosure.

FIG. 12A illustrates an example detector portion that may be employed in an embodiment of a sensor, according to an embodiment of the disclosure;

FIGS. 12B through 12D illustrate exemplary arrangements of detectors that may be employed in an embodiment of the sensor, according to some embodiments of the disclosure;

FIGS. 12E through 12H illustrate exemplary structures of photodiodes that may be employed in embodiments of the detectors, according to some embodiments of the disclosure;

FIG. 13 illustrates an example multi-stream operation of the system of FIG. 1, according to an embodiment of the disclosure;

FIG. 14A illustrates another example detector portion having a partially cylindrical protrusion that can be employed in an embodiment of a sensor, according to an embodiment of the disclosure;

FIG. 14B depicts a front elevation view of the partially cylindrical protrusion of FIG. 14A;

FIGS. 14C through 14E illustrate embodiments of a detector submount;

FIGS. 14F through 14H illustrate embodiment of portions of a detector shell;

FIG. 14I illustrates a cutaway view of an embodiment of a sensor;

FIGS. 15A through 15F illustrate embodiments of sensors that include heat sink features;

FIGS. 15G and 15H illustrate embodiments of connector features that can be used with any of the sensors described herein;

FIG. 15I illustrates an exemplary architecture for a transimpedance-based front-end that may be employed in any of the sensors described herein;

FIG. 15J illustrates an exemplary noise model for configuring the transimpedance-based front-ends shown in FIG. 15I;

FIG. 15K shows different architectures and layouts for various embodiments of a sensor and its detectors;

FIG. 15L illustrates an exemplary architecture for a switched-capacitor-based front-end;

FIGS. 16A and 16B illustrate embodiments of disposable optical sensors;

FIG. 17 illustrates an exploded view of certain components of an example sensor; and

FIGS. 18 through 22 illustrate various results obtained by an exemplary sensor of the disclosure.

DETAILED DESCRIPTION

The present disclosure generally relates to non-invasive medical devices. A sensor can include photocommunicative components, such as an emitter, a detector, and other components. The emitter is configured as a point optical source that comprises a plurality of LEDs that emit a sequence of pulses of optical radiation across a spectrum of wavelengths. In some embodiments, the plurality of sets of optical sources may each comprise at least one top-emitting LED and at least one super luminescent LED. In some embodiments, the emitter comprises optical sources that transmit optical radiation in the infrared or near-infrared wavelengths suitable for detecting blood analytes like glucose. In order to achieve the desired SNR for detecting analytes like glucose, the emitter may be driven using a progression from low power to higher power. In addition, the emitter may have its duty cycle modified to achieve a desired SNR.

The emitter may be constructed of materials, such as aluminum nitride and may include a heat sink to assist in heat dissipation. A thermistor may also be employed to account for heating effects on the LEDs. The emitter may further comprise a glass window and a nitrogen environment to improve transmission from the sources and prevent oxidative effects.

Detectors can then detect optical radiation from the measurement site. The optical sources and optical radiation detectors can operate at any appropriate wavelength, including, as discussed herein, infrared, near infrared, visible light, and ultraviolet. In addition, the optical sources and optical radiation detectors can operate at any appropriate wavelength, and such modifications to the embodiments desirable to operate at any such wavelength will be apparent to those skilled in the art.

In certain embodiments, multiple detectors are employed and arranged in a spatial geometry. This spatial geometry provides a diversity of path lengths among at least some of the detectors and allows for multiple bulk and pulsatile measurements that are robust. Each of the detectors can provide a respective output stream based on the detected optical radiation, or a sum of output streams can be provided from multiple detectors. In some embodiments, the sensor can also include other components, such as one or more heat sinks and one or more thermistors.

The sensor can be coupled to one or more monitors that process and/or display the sensor's output. The monitors can include various components, such as a sensor front end, a signal processor, a display, etc.

The sensor can be integrated with a monitor, for example, into a handheld unit including the sensor, a display and user controls. In other embodiments, the sensor can communicate with one or more processing devices. The communication can be via wire(s), cable(s), flex circuit(s), wireless technologies, or other suitable analog or digital communication methodolo-

gies and devices to perform those methodologies. Many of the foregoing arrangements allow the sensor to be attached to the measurement site while the device is attached elsewhere on a patient, such as the patient's arm, or placed at a location near the patient, such as a bed, shelf or table. The sensor or monitor can also provide outputs to a storage device or network interface.

Reference will now be made to the Figures to discuss embodiments of the present disclosure.

FIG. 1 illustrates an example of a data collection system 100. In certain embodiments, the data collection system 100 noninvasively measure a blood analyte, such as oxygen, carbon monoxide, methemoglobin, total hemoglobin, glucose, proteins, glucose, lipids, a percentage thereof (e.g., saturation) or for measuring many other physiologically relevant patient characteristics. The system 100 can also measure additional blood analytes and/or other physiological parameters useful in determining a state or trend of wellness of a patient.

The data collection system 100 can be capable of measuring optical radiation from the measurement site. For example, in some embodiments, the data collection system 100 can employ photodiodes defined in terms of area. In an embodiment, the area is from about 1 mm²-5 mm² (or higher) that are capable of detecting about 100 nanoamps (nA) or less of current resulting from measured light at full scale. In addition to having its ordinary meaning, the phrase "at full scale" can mean light saturation of a photodiode amplifier (not shown). Of course, as would be understood by a person of skill in the art from the present disclosure, various other sizes and types of photodiodes can be used with the embodiments of the present disclosure.

The data collection system 100 can measure a range of approximately about 2 nA to about 100 nA full scale. The data collection system 100 can also include sensor front-ends that are capable of processing and amplifying current from the detector(s) at signal-to-noise ratios (SNRs) of about 100 decibels (dB) or more, such as about 120 dB in order to measure various desired analytes. The data collection system 100 can operate with a lower SNR if less accuracy is desired for an analyte like glucose.

The data collection system 100 can measure analyte concentrations, including glucose, at least in part by detecting light attenuated by a measurement site 102. The measurement site 102 can be any location on a patient's body, such as a finger, foot, ear lobe, or the like. For convenience, this disclosure is described primarily in the context of a finger measurement site 102. However, the features of the embodiments disclosed herein can be used with other measurement sites 102.

In the depicted embodiment, the system 100 includes an optional tissue thickness adjuster or tissue shaper 105, which can include one or more protrusions, bumps, lenses, or other suitable tissue-shaping mechanisms. In certain embodiments, the tissue shaper 105 is a flat or substantially flat surface that can be positioned proximate the measurement site 102 and that can apply sufficient pressure to cause the tissue of the measurement site 102 to be flat or substantially flat. In other embodiments, the tissue shaper 105 is a convex or substantially convex surface with respect to the measurement site 102. Many other configurations of the tissue shaper 105 are possible. Advantageously, in certain embodiments, the tissue shaper 105 reduces thickness of the measurement site 102 while preventing or reducing occlusion at the measurement site 102. Reducing thickness of the site can advantageously reduce the amount of attenuation of the light because there is less tissue through which the light must travel. Shaping the

tissue in to a convex (or alternatively concave) surface can also provide more surface area from which light can be detected.

The embodiment of the data collection system **100** shown also includes an optional noise shield **103**. In an embodiment, the noise shield **103** can be advantageously adapted to reduce electromagnetic noise while increasing the transmittance of light from the measurement site **102** to one or more detectors **106** (described below). For example, the noise shield **103** can advantageously include a conductive coated glass or metal grid electrically communicating with one or more other shields of the sensor **101** or electrically grounded. In an embodiment where the noise shield **103** includes conductive coated glass, the coating can advantageously include indium tin oxide. In an embodiment, the indium tin oxide includes a surface resistivity ranging from approximately 30 ohms per square inch to about 500 ohms per square inch. In an embodiment, the resistivity is approximately 30, 200, or 500 ohms per square inch. As would be understood by a person of skill in the art from the present disclosure, other resistivities can also be used which are less than about 30 ohms or more than about 500 ohms. Other conductive materials transparent or substantially transparent to light can be used instead.

In some embodiments, the measurement site **102** is located somewhere along a non-dominant arm or a non-dominant hand, e.g., a right-handed person's left arm or left hand. In some patients, the non-dominant arm or hand can have less musculature and higher fat content, which can result in less water content in that tissue of the patient. Tissue having less water content can provide less interference with the particular wavelengths that are absorbed in a useful manner by blood analytes like glucose. Accordingly, in some embodiments, the data collection system **100** can be used on a person's non-dominant hand or arm.

The data collection system **100** can include a sensor **101** (or multiple sensors) that is coupled to a processing device or physiological monitor **109**. In an embodiment, the sensor **101** and the monitor **109** are integrated together into a single unit. In another embodiment, the sensor **101** and the monitor **109** are separate from each other and communicate one with another in any suitable manner, such as via a wired or wireless connection. The sensor **101** and monitor **109** can be attachable and detachable from each other for the convenience of the user or caregiver, for ease of storage, sterility issues, or the like. The sensor **101** and the monitor **109** will now be further described.

In the depicted embodiment shown in FIG. 1, the sensor **101** includes an emitter **104**, a tissue shaper **105**, a set of detectors **106**, and a front-end interface **108**. The emitter **104** can serve as the source of optical radiation transmitted towards measurement site **102**. As will be described in further detail below, the emitter **104** can include one or more sources of optical radiation, such as LEDs, laser diodes, incandescent bulbs with appropriate frequency-selective filters, combinations of the same, or the like. In an embodiment, the emitter **104** includes sets of optical sources that are capable of emitting visible and near-infrared optical radiation.

In some embodiments, the emitter **104** is used as a point optical source, and thus, the one or more optical sources of the emitter **104** can be located within a close distance to each other, such as within about a 2 mm to about 4 mm. The emitters **104** can be arranged in an array, such as is described in U.S. Publication No. 2006/0211924, filed Sep. 21, 2006, titled "Multiple Wavelength Sensor Emitters," the disclosure of which is hereby incorporated by reference in its entirety. In particular, the emitters **104** can be arranged at least in part as described in paragraphs [0061] through [0068] of the afore-

mentioned publication, which paragraphs are hereby incorporated specifically by reference. Other relative spatial relationships can be used to arrange the emitters **104**.

For analytes like glucose, currently available non-invasive techniques often attempt to employ light near the water absorbance minima at or about 1600 nm. Typically, these devices and methods employ a single wavelength or single band of wavelengths at or about 1600 nm. However, to date, these techniques have been unable to adequately consistently measure analytes like glucose based on spectroscopy.

In contrast, the emitter **104** of the data collection system **100** can emit, in certain embodiments, combinations of optical radiation in various bands of interest. For example, in some embodiments, for analytes like glucose, the emitter **104** can emit optical radiation at three (3) or more wavelengths between about 1600 nm to about 1700 nm. In particular, the emitter **104** can emit optical radiation at or about 1610 nm, about 1640 nm, and about 1665 nm. In some circumstances, the use of three wavelengths within about 1600 nm to about 1700 nm enable sufficient SNRs of about 100 dB, which can result in a measurement accuracy of about 20 mg/dL or better for analytes like glucose.

In other embodiments, the emitter **104** can use two (2) wavelengths within about 1600 nm to about 1700 nm to advantageously enable SNRs of about 85 dB, which can result in a measurement accuracy of about 25-30 mg/dL or better for analytes like glucose. Furthermore, in some embodiments, the emitter **104** can emit light at wavelengths above about 1670 nm. Measurements at these wavelengths can be advantageously used to compensate or confirm the contribution of protein, water, and other non-hemoglobin species exhibited in measurements for analytes like glucose conducted between about 1600 nm and about 1700 nm. Of course, other wavelengths and combinations of wavelengths can be used to measure analytes and/or to distinguish other types of tissue, fluids, tissue properties, fluid properties, combinations of the same or the like.

For example, the emitter **104** can emit optical radiation across other spectra for other analytes. In particular, the emitter **104** can employ light wavelengths to measure various blood analytes or percentages (e.g., saturation) thereof. For example, in one embodiment, the emitter **104** can emit optical radiation in the form of pulses at wavelengths about 905 nm, about 1050 nm, about 1200 nm, about 1300 nm, about 1330 nm, about 1610 nm, about 1640 nm, and about 1665 nm. In another embodiment, the emitter **104** can emit optical radiation ranging from about 860 nm to about 950 nm, about 950 nm to about 1100 nm, about 1100 nm to about 1270 nm, about 1250 nm to about 1350 nm, about 1300 nm to about 1360 nm, and about 1590 nm to about 1700 nm. Of course, the emitter **104** can transmit any of a variety of wavelengths of visible or near-infrared optical radiation.

Due to the different responses of analytes to the different wavelengths, certain embodiments of the data collection system **100** can advantageously use the measurements at these different wavelengths to improve the accuracy of measurements. For example, the measurements of water from visible and infrared light can be used to compensate for water absorbance that is exhibited in the near-infrared wavelengths.

As briefly described above, the emitter **104** can include sets of light-emitting diodes (LEDs) as its optical source. The emitter **104** can use one or more top-emitting LEDs. In particular, in some embodiments, the emitter **104** can include top-emitting LEDs emitting light at about 850 nm to 1350 nm.

The emitter **104** can also use super luminescent LEDs (SLEDs) or side-emitting LEDs. In some embodiments, the emitter **104** can employ SLEDs or side-emitting LEDs to emit

optical radiation at about 1600 nm to about 1800 nm. Emitter 104 can use SLEDs or side-emitting LEDs to transmit near infrared optical radiation because these types of sources can transmit at high power or relatively high power, e.g., about 40 mW to about 100 mW. This higher power capability can be useful to compensate or overcome the greater attenuation of these wavelengths of light in tissue and water. For example, the higher power emission can effectively compensate and/or normalize the absorption signal for light in the mentioned wavelengths to be similar in amplitude and/or effect as other wavelengths that can be detected by one or more photodetectors after absorption. However, the embodiments of the present disclosure do not necessarily require the use of high power optical sources. For example, some embodiments may be configured to measure analytes, such as total hemoglobin (tHb), oxygen saturation (SpO₂), carboxyhemoglobin, methemoglobin, etc., without the use of high power optical sources like side emitting LEDs. Instead, such embodiments may employ other types of optical sources, such as top emitting LEDs. Alternatively, the emitter 104 can use other types of sources of optical radiation, such as a laser diode, to emit near-infrared light into the measurement site 102.

In addition, in some embodiments, in order to assist in achieving a comparative balance of desired power output between the LEDs, some of the LEDs in the emitter 104 can have a filter or covering that reduces and/or cleans the optical radiation from particular LEDs or groups of LEDs. For example, since some wavelengths of light can penetrate through tissue relatively well, LEDs, such as some or all of the top-emitting LEDs can use a filter or covering, such as a cap or painted dye. This can be useful in allowing the emitter 104 to use LEDs with a higher output and/or to equalize intensity of LEDs.

The data collection system 100 also includes a driver 111 that drives the emitter 104. The driver 111 can be a circuit or the like that is controlled by the monitor 109. For example, the driver 111 can provide pulses of current to the emitter 104. In an embodiment, the driver 111 drives the emitter 104 in a progressive fashion, such as in an alternating manner. The driver 111 can drive the emitter 104 with a series of pulses of about 1 milliwatt (mW) for some wavelengths that can penetrate tissue relatively well and from about 40 mW to about 100 mW for other wavelengths that tend to be significantly absorbed in tissue. A wide variety of other driving powers and driving methodologies can be used in various embodiments.

The driver 111 can be synchronized with other parts of the sensor 101 and can minimize or reduce jitter in the timing of pulses of optical radiation emitted from the emitter 104. In some embodiments, the driver 111 is capable of driving the emitter 104 to emit optical radiation in a pattern that varies by less than about 10 parts-per-million.

The detectors 106 capture and measure light from the measurement site 102. For example, the detectors 106 can capture and measure light transmitted from the emitter 104 that has been attenuated or reflected from the tissue in the measurement site 102. The detectors 106 can output a detector signal 107 responsive to the light captured or measured. The detectors 106 can be implemented using one or more photodiodes, phototransistors, or the like.

In addition, the detectors 106 can be arranged with a spatial configuration to provide a variation of path lengths among at least some of the detectors 106. That is, some of the detectors 106 can have the substantially, or from the perspective of the processing algorithm, effectively, the same path length from the emitter 104. However, according to an embodiment, at least some of the detectors 106 can have a different path length from the emitter 104 relative to other of the detectors

106. Variations in path lengths can be helpful in allowing the use of a bulk signal stream from the detectors 106. In some embodiments, the detectors 106 may employ a linear spacing, a logarithmic spacing, or a two or three dimensional matrix of spacing, or any other spacing scheme in order to provide an appropriate variation in path lengths.

The front end interface 108 provides an interface that adapts the output of the detectors 106, which is responsive to desired physiological parameters. For example, the front end interface 108 can adapt a signal 107 received from one or more of the detectors 106 into a form that can be processed by the monitor 109, for example, by a signal processor 110 in the monitor 109. The front end interface 108 can have its components assembled in the sensor 101, in the monitor 109, in connecting cabling (if used), combinations of the same, or the like. The location of the front end interface 108 can be chosen based on various factors including space desired for components, desired noise reductions or limits, desired heat reductions or limits, and the like.

The front end interface 108 can be coupled to the detectors 106 and to the signal processor 110 using a bus, wire, electrical or optical cable, flex circuit, or some other form of signal connection. The front end interface 108 can also be at least partially integrated with various components, such as the detectors 106. For example, the front end interface 108 can include one or more integrated circuits that are on the same circuit board as the detectors 106. Other configurations can also be used.

The front end interface 108 can be implemented using one or more amplifiers, such as transimpedance amplifiers, that are coupled to one or more analog to digital converters (ADCs) (which can be in the monitor 109), such as a sigma-delta ADC. A transimpedance-based front end interface 108 can employ single-ended circuitry, differential circuitry, and/or a hybrid configuration. A transimpedance-based front end interface 108 can be useful for its sampling rate capability and freedom in modulation/demodulation algorithms. For example, this type of front end interface 108 can advantageously facilitate the sampling of the ADCs being synchronized with the pulses emitted from the emitter 104.

The ADC or ADCs can provide one or more outputs into multiple channels of digital information for processing by the signal processor 110 of the monitor 109. Each channel can correspond to a signal output from a detector 106.

In some embodiments, a programmable gain amplifier (PGA) can be used in combination with a transimpedance-based front end interface 108. For example, the output of a transimpedance-based front end interface 108 can be output to a PGA that is coupled with an ADC in the monitor 109. A PGA can be useful in order to provide another level of amplification and control of the stream of signals from the detectors 106. Alternatively, the PGA and ADC components can be integrated with the transimpedance-based front end interface 108 in the sensor 101.

In another embodiment, the front end interface 108 can be implemented using switched-capacitor circuits. A switched-capacitor-based front end interface 108 can be useful for, in certain embodiments, its resistor-free design and analog averaging properties. In addition, a switched-capacitor-based front end interface 108 can be useful because it can provide a digital signal to the signal processor 110 in the monitor 109.

As shown in FIG. 1, the monitor 109 can include the signal processor 110 and a user interface, such as a display 112. The monitor 109 can also include optional outputs alone or in combination with the display 112, such as a storage device 114 and a network interface 116. In an embodiment, the signal processor 110 includes processing logic that deter-

mines measurements for desired analytes, such as glucose, based on the signals received from the detectors **106**. The signal processor **110** can be implemented using one or more microprocessors or subprocessors (e.g., cores), digital signal processors, application specific integrated circuits (ASICs), field programmable gate arrays (FPGAs), combinations of the same, and the like.

The signal processor **110** can provide various signals that control the operation of the sensor **101**. For example, the signal processor **110** can provide an emitter control signal to the driver **111**. This control signal can be useful in order to synchronize, minimize, or reduce jitter in the timing of pulses emitted from the emitter **104**. Accordingly, this control signal can be useful in order to cause optical radiation pulses emitted from the emitter **104** to follow a precise timing and consistent pattern. For example, when a transimpedance-based front end interface **108** is used, the control signal from the signal processor **110** can provide synchronization with the ADC in order to avoid aliasing, cross-talk, and the like. As also shown, an optional memory **113** can be included in the front-end interface **108** and/or in the signal processor **110**. This memory **113** can serve as a buffer or storage location for the front-end interface **108** and/or the signal processor **110**, among other uses.

The user interface **112** can provide an output, e.g., on a display, for presentation to a user of the data collection system **100**. The user interface **112** can be implemented as a touch-screen display, an LCD display, an organic LED display, or the like. In addition, the user interface **112** can be manipulated to allow for measurement on the non-dominant side of patient. For example, the user interface **112** can include a flip screen, a screen that can be moved from one side to another on the monitor **109**, or can include an ability to reorient its display indicia responsive to user input or device orientation. In alternative embodiments, the data collection system **100** can be provided without a user interface **112** and can simply provide an output signal to a separate display or system.

A storage device **114** and a network interface **116** represent other optional output connections that can be included in the monitor **109**. The storage device **114** can include any computer-readable medium, such as a memory device, hard disk storage, EEPROM, flash drive, or the like. The various software and/or firmware applications can be stored in the storage device **114**, which can be executed by the signal processor **110** or another processor of the monitor **109**. The network interface **116** can be a serial bus port (RS-232/RS-485), a Universal Serial Bus (USB) port, an Ethernet port, a wireless interface (e.g., WiFi such as any 802.1x interface, including an internal wireless card), or other suitable communication device(s) that allows the monitor **109** to communicate and share data with other devices. The monitor **109** can also include various other components not shown, such as a microprocessor, graphics processor, or controller to output the user interface **112**, to control data communications, to compute data trending, or to perform other operations.

Although not shown in the depicted embodiment, the data collection system **100** can include various other components or can be configured in different ways. For example, the sensor **101** can have both the emitter **104** and detectors **106** on the same side of the measurement site **102** and use reflectance to measure analytes. The data collection system **100** can also include a sensor that measures the power of light emitted from the emitter **104**.

FIGS. 2A through 2D illustrate example monitoring devices **200** in which the data collection system **100** can be housed. Advantageously, in certain embodiments, some or all of the example monitoring devices **200** shown can have a

shape and size that allows a user to operate it with a single hand or attach it, for example, to a patient's body or limb. Although several examples are shown, many other monitoring device configurations can be used to house the data collection system **100**. In addition, certain of the features of the monitoring devices **200** shown in FIGS. 2A through 2D can be combined with features of the other monitoring devices **200** shown.

Referring specifically to FIG. 2A, an example monitoring device **200A** is shown, in which a sensor **201a** and a monitor **209a** are integrated into a single unit. The monitoring device **200A** shown is a handheld or portable device that can measure glucose and other analytes in a patient's finger. The sensor **201a** includes an emitter shell **204a** and a detector shell **206a**. The depicted embodiment of the monitoring device **200A** also includes various control buttons **208a** and a display **210a**.

The sensor **201a** can be constructed of white material used for reflective purposes (such as white silicone or plastic), which can increase the usable signal at the detector **106** by forcing light back into the sensor **201a**. Pads in the emitter shell **204a** and the detector shell **206a** can contain separated windows to prevent or reduce mixing of light signals, for example, from distinct quadrants on a patient's finger. In addition, these pads can be made of a relatively soft material, such as a gel or foam, in order to conform to the shape, for example, of a patient's finger. The emitter shell **204a** and the detector shell **206a** can also include absorbing black or grey material portions to prevent or reduce ambient light from entering into the sensor **201a**.

In some embodiments, some or all portions of the emitter shell **204a** and/or detector shell **206a** can be detachable and/or disposable. For example, some or all portions of the shells **204a** and **206a** can be removable pieces. The removability of the shells **204a** and **206a** can be useful for sanitary purposes or for sizing the sensor **201a** to different patients. The monitor **209a** can include a fitting, slot, magnet, or other connecting mechanism to allow the sensor **201c** to be removably attached to the monitor **209a**.

The monitoring device **200a** also includes optional control buttons **208a** and a display **210a** that can allow the user to control the operation of the device. For example, a user can operate the control buttons **208a** to view one or more measurements of various analytes, such as glucose. In addition, the user can operate the control buttons **208a** to view other forms of information, such as graphs, histograms, measurement data, trend measurement data, parameter combination views, wellness indications, and the like. Many parameters, trends, alarms and parameter displays could be output to the display **210a**, such as those that are commercially available through a wide variety of noninvasive monitoring devices from Masimo® Corporation of Irvine, Calif.

Furthermore, the controls **208a** and/or display **210a** can provide functionality for the user to manipulate settings of the monitoring device **200a**, such as alarm settings, emitter settings, detector settings, and the like. The monitoring device **200a** can employ any of a variety of user interface designs, such as frames, menus, touch-screens, and any type of button.

FIG. 2B illustrates another example of a monitoring device **200B**. In the depicted embodiment, the monitoring device **200B** includes a finger clip sensor **201b** connected to a monitor **209b** via a cable **212**. In the embodiment shown, the monitor **209b** includes a display **210b**, control buttons **208b** and a power button. Moreover, the monitor **209b** can advantageously include electronic processing, signal processing, and data storage devices capable of receiving signal data from said sensor **201b**, processing the signal data to determine one or more output measurement values indicative of one or more

physiological parameters of a monitored patient, and displaying the measurement values, trends of the measurement values, combinations of measurement values, and the like.

The cable **212** connecting the sensor **201b** and the monitor **209b** can be implemented using one or more wires, optical fiber, flex circuits, or the like. In some embodiments, the cable **212** can employ twisted pairs of conductors in order to minimize or reduce cross-talk of data transmitted from the sensor **201b** to the monitor **209b**. Various lengths of the cable **212** can be employed to allow for separation between the sensor **201b** and the monitor **209b**. The cable **212** can be fitted with a connector (male or female) on either end of the cable **212** so that the sensor **201b** and the monitor **209b** can be connected and disconnected from each other. Alternatively, the sensor **201b** and the monitor **209b** can be coupled together via a wireless communication link, such as an infrared link, radio frequency channel, or any other wireless communication protocol and channel.

The monitor **209b** can be attached to the patient. For example, the monitor **209b** can include a belt clip or straps (see, e.g., FIG. 2C) that facilitate attachment to a patient's belt, arm, leg, or the like. The monitor **209b** can also include a fitting, slot, magnet, LEMO snap-click connector, or other connecting mechanism to allow the cable **212** and sensor **201b** to be attached to the monitor **209b**.

The monitor **209b** can also include other components, such as a speaker, power button, removable storage or memory (e.g., a flash card slot), an AC power port, and one or more network interfaces, such as a universal serial bus interface or an Ethernet port. For example, the monitor **209b** can include a display **210b** that can indicate a measurement for glucose, for example, in mg/dL. Other analytes and forms of display can also appear on the monitor **209b**.

In addition, although a single sensor **201b** with a single monitor **209b** is shown, different combinations of sensors and device pairings can be implemented. For example, multiple sensors can be provided for a plurality of differing patient types or measurement sites or even patient fingers.

FIG. 2C illustrates yet another example of monitoring device **200C** that can house the data collection system **100**. Like the monitoring device **200B**, the monitoring device **200C** includes a finger clip sensor **201c** connected to a monitor **209c** via a cable **212**. The cable **212** can have all of the features described above with respect to FIG. 2B. The monitor **209c** can include all of the features of the monitor **200B** described above. For example, the monitor **209c** includes buttons **208c** and a display **210c**. The monitor **209c** shown also includes straps **214c** that allow the monitor **209c** to be attached to a patient's limb or the like.

FIG. 2D illustrates yet another example of monitoring device **200D** that can house the data collection system **100**. Like the monitoring devices **200B** and **200C**, the monitoring device **200D** includes a finger clip sensor **201d** connected to a monitor **209d** via a cable **212**. The cable **212** can have all of the features described above with respect to FIG. 2B. In addition to having some or all of the features described above with respect to FIGS. 2B and 2C, the monitoring device **200D** includes an optional universal serial bus (USB) port **216** and an Ethernet port **218**. The USB port **216** and the Ethernet port **218** can be used, for example, to transfer information between the monitor **209d** and a computer (not shown) via a cable. Software stored on the computer can provide functionality for a user to, for example, view physiological data and trends, adjust settings and download firmware updates to the monitor **209b**, and perform a variety of other functions. The USB port **216** and the Ethernet port **218** can be included with the other monitoring devices **200A**, **200B**, and **200C** described above.

FIGS. 3A through 3C illustrate more detailed examples of embodiments of a sensor **301a**. The sensor **301a** shown can include all of the features of the sensors **100** and **200** described above.

Referring to FIG. 3A, the sensor **301a** in the depicted embodiment is a clothespin-shaped clip sensor that includes an enclosure **302a** for receiving a patient's finger. The enclosure **302a** is formed by an upper section or emitter shell **304a**, which is pivotably connected with a lower section or detector shell **306a**. The emitter shell **304a** can be biased with the detector shell **306a** to close together around a pivot point **303a** and thereby sandwich finger tissue between the emitter and detector shells **304a**, **306a**.

In an embodiment, the pivot point **303a** advantageously includes a pivot capable of adjusting the relationship between the emitter and detector shells **304a**, **306a** to effectively level the sections when applied to a tissue site. In another embodiment, the sensor **301a** includes some or all features of the finger clip described in U.S. Publication No. 2006/0211924, incorporated above, such as a spring that causes finger clip forces to be distributed along the finger. Paragraphs [0096] through [0105], which describe this feature, are hereby specifically incorporated by reference.

The emitter shell **304a** can position and house various emitter components of the sensor **301a**. It can be constructed of reflective material (e.g., white silicone or plastic) and/or can be metallic or include metalized plastic (e.g., including carbon and aluminum) to possibly serve as a heat sink. The emitter shell **304a** can also include absorbing opaque material, such as, for example, black or grey colored material, at various areas, such as on one or more flaps **307a**, to reduce ambient light entering the sensor **301a**.

The detector shell **306a** can position and house one or more detector portions of the sensor **301a**. The detector shell **306a** can be constructed of reflective material, such as white silicone or plastic. As noted, such materials can increase the usable signal at a detector by forcing light back into the tissue and measurement site (see FIG. 1). The detector shell **306a** can also include absorbing opaque material at various areas, such as lower area **308a**, to reduce ambient light entering the sensor **301a**.

Referring to FIGS. 3B and 3C, an example of finger bed **310** is shown in the sensor **301b**. The finger bed **310** includes a generally curved surface shaped generally to receive tissue, such as a human digit. The finger bed **310** includes one or more ridges or channels **314**. Each of the ridges **314** has a generally convex shape that can facilitate increasing traction or gripping of the patient's finger to the finger bed. Advantageously, the ridges **314** can improve the accuracy of spectroscopic analysis in certain embodiments by reducing noise that can result from a measurement site moving or shaking loose inside of the sensor **301a**. The ridges **314** can be made from reflective or opaque materials in some embodiments to further increase SNR. In other implementations, other surface shapes can be used, such as, for example, generally flat, concave, or convex finger beds **310**.

Finger bed **310** can also include an embodiment of a tissue thickness adjuster or protrusion **305**. The protrusion **305** includes a measurement site contact area **370** (see FIG. 3C) that can contact body tissue of a measurement site. The protrusion **305** can be removed from or integrated with the finger bed **310**. Interchangeable, different shaped protrusions **305** can also be provided, which can correspond to different finger shapes, characteristics, opacity, sizes, or the like.

Referring specifically to FIG. 3C, the contact area **370** of the protrusion **305** can include openings or windows **320**, **321**, **322**, and **323**. When light from a measurement site

passes through the windows **320**, **321**, **322**, and **323**, the light can reach one or more photodetectors (see FIG. 3E). In an embodiment, the windows **320**, **321**, **322**, and **323** mirror specific detector placements layouts such that light can impinge through the protrusion **305** onto the photodetectors. Any number of windows **320**, **321**, **322**, and **323** can be employed in the protrusion **305** to allow light to pass from the measurement site to the photodetectors.

The windows **320**, **321**, **322**, and **323** can also include shielding, such as an embedded grid of wiring or a conductive glass coating, to reduce noise from ambient light or other electromagnetic noise. The windows **320**, **321**, **322**, and **323** can be made from materials, such as plastic or glass. In some embodiments, the windows **320**, **321**, **322**, and **323** can be constructed from conductive glass, such as indium tin oxide (ITO) coated glass. Conductive glass can be useful because its shielding is transparent, and thus allows for a larger aperture versus a window with an embedded grid of wiring. In addition, in certain embodiments, the conductive glass does not need openings in its shielding (since it is transparent), which enhances its shielding performance. For example, some embodiments that employ the conductive glass can attain up to an about 40% to about 50% greater signal than non-conductive glass with a shielding grid. In addition, in some embodiments, conductive glass can be useful for shielding noise from a greater variety of directions than non-conductive glass with a shielding grid.

Turning to FIG. 3B, the sensor **301a** can also include a shielding **315a**, such as a metal cage, box, metal sheet, perforated metal sheet, a metal layer on a non-metal material, or the like. The shielding **315a** is provided in the depicted embodiment below or embedded within the protrusion **305** to reduce noise. The shielding **315a** can be constructed from a conductive material, such as copper. The shielding **315a** can include one or more openings or windows (not shown). The windows can be made from glass or plastic to thereby allow light that has passed through the windows **320**, **321**, **322**, and **323** on an external surface of the protrusion **305** (see FIG. 3C) to pass through to one or more photodetectors that can be enclosed or provided below (see FIG. 3E).

In some embodiments, the shielding cage for shielding **315a** can be constructed in a single manufactured component with or without the use of conductive glass. This form of construction may be useful in order to reduce costs of manufacture as well as assist in quality control of the components. Furthermore, the shielding cage can also be used to house various other components, such as sigma delta components for various embodiments of front end interfaces **108**.

In an embodiment, the photodetectors can be positioned within or directly beneath the protrusion **305** (see FIG. 3E). In such cases, the mean optical path length from the emitters to the detectors can be reduced and the accuracy of blood analyte measurement can increase. For example, in one embodiment, a convex bump of about 1 mm to about 3 mm in height and about 10 mm² to about 60 mm² was found to help signal strength by about an order of magnitude versus other shapes. Of course other dimensions and sizes can be employed in other embodiments. Depending on the properties desired, the length, width, and height of the protrusion **305** can be selected. In making such determinations, consideration can be made of protrusion's **305** effect on blood flow at the measurement site and mean path length for optical radiation passing through openings **320**, **321**, **322**, and **323**. Patient comfort can also be considered in determining the size and shape of the protrusion.

In an embodiment, the protrusion **305** can include a pliant material, including soft plastic or rubber, which can some-

what conform to the shape of a measurement site. Pliant materials can improve patient comfort and tactility by conforming the measurement site contact area **370** to the measurement site. Additionally, pliant materials can minimize or reduce noise, such as ambient light. Alternatively, the protrusion **305** can be made from a rigid material, such as hard plastic or metal.

Rigid materials can improve measurement accuracy of a blood analyte by conforming the measurement site to the contact area **370**. The contact area **370** can be an ideal shape for improving accuracy or reducing noise. Selecting a material for the protrusion **305** can include consideration of materials that do not significantly alter blood flow at the measurement site. The protrusion **305** and the contact area **370** can include a combination of materials with various characteristics.

The contact area **370** serves as a contact surface for the measurement site. For example, in some embodiments, the contact area **370** can be shaped for contact with a patient's finger. Accordingly, the contact area **370** can be sized and shaped for different sizes of fingers. The contact area **370** can be constructed of different materials for reflective purposes as well as for the comfort of the patient. For example, the contact area **370** can be constructed from materials having various hardness and textures, such as plastic, gel, foam, and the like.

The formulas and analysis that follow with respect to FIG. 5 provide insight into how selecting these variables can alter transmittance and intensity gain of optical radiation that has been applied to the measurement site. These examples do not limit the scope of this disclosure.

Referring to FIG. 5, a plot **500** is shown that illustrates examples of effects of embodiments of the protrusion **305** on the SNR at various wavelengths of light. As described above, the protrusion **305** can assist in conforming the tissue and effectively reduce its mean path length. In some instances, this effect by the protrusion **305** can have significant impact on increasing the SNR.

According to the Beer Lambert law, a transmittance of light (I) can be expressed as follows: $I = I_0 * e^{-m * b * c}$, where I_0 is the initial power of light being transmitted, m is the path length traveled by the light, and the component " $b * c$ " corresponds to the bulk absorption of the light at a specific wavelength of light. For light at about 1600 nm to about 1700 nm, for example, the bulk absorption component is generally around 0.7 mm⁻¹. Assuming a typical finger thickness of about 12 mm and a mean path length of 20 mm due to tissue scattering, then $I = I_0 * e^{(-20 * 0.7)}$.

In an embodiment where the protrusion **305** is a convex bump, the thickness of the finger can be reduced to 10 mm (from 12 mm) for some fingers and the effective light mean path is reduced to about 16.6 mm from 20 mm (see box **510**). This results in a new transmittance, $I_1 = I_0 * e^{(-16.6 * 0.7)}$. A curve for a typical finger (having a mean path length of 20 mm) across various wavelengths is shown in the plot **500** of FIG. 5. The plot **500** illustrates potential effects of the protrusion **305** on the transmittance. As illustrated, comparing I and I_1 results in an intensity gain of $e^{(-16.6 * 0.7) / e^{(-20 * 0.7)}}$, which is about a 10 times increase for light in the about 1600 nm to about 1700 nm range. Such an increase can affect the SNR at which the sensor can operate. The foregoing gains can be due at least in part to the about 1600 nm to about 1700 nm range having high values in bulk absorptions (water, protein, and the like), e.g., about 0.7 mm⁻¹. The plot **500** also shows improvements in the visible/near-infrared range (about 600 nm to about 1300 nm).

Turning again to FIGS. 3A through 3C, an example heat sink **350a** is also shown. The heat sink **350a** can be attached to, or protrude from an outer surface of, the sensor **301a**,

thereby providing increased ability for various sensor components to dissipate excess heat. By being on the outer surface of the sensor **301a** in certain embodiments, the heat sink **350a** can be exposed to the air and thereby facilitate more efficient cooling. In an embodiment, one or more of the emitters (see FIG. 1) generate sufficient heat that inclusion of the heat sink **350a** can advantageously allows the sensor **301a** to remain safely cooled. The heat sink **350a** can include one or more materials that help dissipate heat, such as, for example, aluminum, steel, copper, carbon, combinations of the same, or the like. For example, in some embodiments, the emitter shell **304a** can include a heat conducting material that is also readily and relatively inexpensively moldable into desired shapes and forms.

In some embodiments, the heat sink **350a** includes metallicized plastic. The metallicized plastic can include aluminum and carbon, for example. The material can allow for improved thermal conductivity and diffusivity, which can increase commercial viability of the heat sink. In some embodiments, the material selected to construct the heat sink **350a** can include a thermally conductive liquid crystalline polymer, such as CoolPoly® D5506, commercially available from Cool Polymers®, Inc. of Warwick, R.I. Such a material can be selected for its electrically non-conductive and dielectric properties so as, for example, to aid in electrical shielding. In an embodiment, the heat sink **350a** provides improved heat transfer properties when the sensor **301a** is active for short intervals of less than a full day's use. In an embodiment, the heat sink **350a** can advantageously provide improved heat transfers in about three (3) to about four (4) minute intervals, for example, although a heat sink **350a** can be selected that performs effectively in shorter or longer intervals.

Moreover, the heat sink **350a** can have different shapes and configurations for aesthetic as well as for functional purposes. In an embodiment, the heat sink is configured to maximize heat dissipation, for example, by maximizing surface area. In an embodiment, the heat sink **350a** is molded into a generally curved surface and includes one or more fins, undulations, grooves, or channels. The example heat sink **350a** shown includes fins **351a** (see FIG. 3A).

An alternative shape of a sensor **301b** and heat sink **350b** is shown in FIG. 3D. The sensor **301b** can include some or all of the features of the sensor **301a**. For example, the sensor **301b** includes an enclosure **302b** formed by an emitter shell **304b** and a detector shell **306b**, pivotably connected about a pivot **303a**. The emitter shell **304b** can also include absorbing opaque material on one or more flaps **307b**, and the detector shell **306b** can also include absorbing opaque material at various areas, such as lower area **308b**.

However, the shape of the sensor **301b** is different in this embodiment. In particular, the heat sink **350b** includes comb protrusions **351b**. The comb protrusions **351b** are exposed to the air in a similar manner to the fins **351a** of the heat sink **350a**, thereby facilitating efficient cooling of the sensor **301b**.

FIG. 3E illustrates a more detailed example of a detector shell **306b** of the sensor **301b**. The features described with respect to the detector shell **306b** can also be used with the detector shell **306a** of the sensor **301a**.

As shown, the detector shell **306b** includes detectors **316**. The detectors **316** can have a predetermined spacing **340** from each other, or a spatial relationship among one another that results in a spatial configuration. This spatial configuration can purposefully create a variation of path lengths among detectors **316** and the emitter discussed above.

In the depicted embodiment, the detector shell **316** can hold multiple (e.g., two, three, four, etc.) photodiode arrays that are arranged in a two-dimensional grid pattern. Multiple

photodiode arrays can also be useful to detect light piping (e.g., light that bypasses measurement site **102**). In the detector shell **316**, walls can be provided to separate the individual photodiode arrays to prevent or reduce mixing of light signals from distinct quadrants. In addition, the detector shell **316** can be covered by windows of transparent material, such as glass, plastic, or the like, to allow maximum or increased transmission of power light captured. In various embodiments, the transparent materials used can also be partially transparent or translucent or can otherwise pass some or all of the optical radiation passing through them. As noted, this window can include some shielding in the form of an embedded grid of wiring, or a conductive layer or coating.

As further illustrated by FIG. 3E, the detectors **316** can have a spatial configuration of a grid. However, the detectors **316** can be arranged in other configurations that vary the path length. For example, the detectors **316** can be arranged in a linear array, a logarithmic array, a two-dimensional array, a zig-zag pattern, or the like. Furthermore, any number of the detectors **316** can be employed in certain embodiments.

FIG. 3F illustrates another embodiment of a sensor **301f**. The sensor **301f** can include some or all of the features of the sensor **301a** of FIG. 3A described above. For example, the sensor **301f** includes an enclosure **302f** formed by an upper section or emitter shell **304f**, which is pivotably connected with a lower section or detector shell **306f** around a pivot point **303f**. The emitter shell **304f** can also include absorbing opaque material on various areas, such as on one or more flaps **307f**, to reduce ambient light entering the sensor **301f**. The detector shell **306f** can also include absorbing opaque material at various areas, such as a lower area **308f**. The sensor **301f** also includes a heat sink **350f**, which includes fins **351f**.

In addition to these features, the sensor **301f** includes a flex circuit cover **360**, which can be made of plastic or another suitable material. The flex circuit cover **360** can cover and thereby protect a flex circuit (not shown) that extends from the emitter shell **304f** to the detector shell **306f**. An example of such a flex circuit is illustrated in U.S. Publication No. 2006/0211924, incorporated above (see FIG. 46 and associated description, which is hereby specifically incorporated by reference). The flex circuit cover **360** is shown in more detail below in FIG. 17.

In addition, sensors **301a-f** has extra length—extends to second joint on finger—Easier to place, harder to move due to cable, better for light piping

FIGS. 4A through 4C illustrate example arrangements of a protrusion **405**, which is an embodiment of the protrusion **305** described above. In an embodiment, the protrusion **405** can include a measurement site contact area **470**. The measurement site contact area **470** can include a surface that molds body tissue of a measurement site, such as a finger, into a flat or relatively flat surface.

The protrusion **405** can have dimensions that are suitable for a measurement site such as a patient's finger. As shown, the protrusion **405** can have a length **400**, a width **410**, and a height **430**. The length **400** can be from about 9 to about 11 millimeters, e.g., about 10 millimeters. The width **410** can be from about 7 to about 9 millimeters, e.g., about 8 millimeters. The height **430** can be from about 0.5 millimeters to about 3 millimeters, e.g., about 2 millimeters. In an embodiment, the dimensions **400**, **410**, and **430** can be selected such that the measurement site contact area **470** includes an area of about 80 square millimeters, although larger and smaller areas can be used for different sized tissue for an adult, an adolescent, or infant, or for other considerations.

The measurement site contact area **470** can also include differently shaped surfaces that conform the measurement

site into different shapes. For example, the measurement site contact area 470 can be generally curved and/or convex with respect to the measurement site. The measurement site contact area 470 can be other shapes that reduce or even minimize air between the protrusion 405 and or the measurement site. Additionally, the surface pattern of the measurement site contact area 470 can vary from smooth to bumpy, e.g., to provide varying levels of grip.

In FIGS. 4A and 4C, openings or windows 420, 421, 422, and 423 can include a wide variety of shapes and sizes, including for example, generally square, circular, triangular, or combinations thereof. The windows 420, 421, 422, and 423 can be of non-uniform shapes and sizes. As shown, the windows 420, 421, 422, and 423 can be evenly spaced out in a grid like arrangement. Other arrangements or patterns of arranging the windows 420, 421, 422, and 423 are possible. For example, the windows 420, 421, 422, and 423 can be placed in a triangular, circular, or linear arrangement. In some embodiments, the windows 420, 421, 422, and 423 can be placed at different heights with respect to the finger bed 310 of FIG. 3. The windows 420, 421, 422, and 423 can also mimic or approximately mimic a configuration of, or even house, a plurality of detectors.

FIGS. 6A through 6D illustrate another embodiment of a protrusion 605 that can be used as the tissue shaper 105 described above or in place of the protrusions 305, 405 described above. The depicted protrusion 605 is a partially cylindrical lens having a partial cylinder 608 and an extension 610. The partial cylinder 608 can be a half cylinder in some embodiments; however, a smaller or greater portion than half of a cylinder can be used. Advantageously, in certain embodiments, the partially cylindrical protrusion 605 focuses light onto a smaller area, such that fewer detectors can be used to detect the light attenuated by a measurement site.

FIG. 6A illustrates a perspective view of the partially cylindrical protrusion 605. FIG. 6B illustrates a front elevation view of the partially cylindrical protrusion 605. FIG. 6C illustrates a side view of the partially cylindrical protrusion 605. FIG. 6D illustrates a top view of the partially cylindrical protrusion 605.

Advantageously, in certain embodiments, placing the partially cylindrical protrusion 605 over the photodiodes in any of the sensors described above adds multiple benefits to any of the sensors described above. In one embodiment, the partially cylindrical protrusion 605 penetrates into the tissue and reduces the path length of the light traveling in the tissue, similar to the protrusions described above.

The partially cylindrical protrusion 605 can also collect light from a large surface and focus down the light to a smaller area. As a result, in certain embodiments, signal strength per area of the photodiode can be increased. The partially cylindrical protrusion 605 can therefore facilitate a lower cost sensor because, in certain embodiments, less photodiode area can be used to obtain the same signal strength. Less photodiode area can be realized by using smaller photodiodes or fewer photodiodes (see, e.g., FIG. 14). If fewer or smaller photodiodes are used, the partially cylindrical protrusion 605 can also facilitate an improved SNR of the sensor because fewer or smaller photodiodes can have less dark current.

The dimensions of the partially cylindrical protrusion 605 can vary based on, for instance, a number of photodiodes used with the sensor. Referring to FIG. 6C, the overall height of the partially cylindrical protrusion 605 (measurement "a") in some implementations is about 1 to about 3 mm. A height in this range can allow the partially cylindrical protrusion 605 to penetrate into the pad of the finger or other tissue and reduce the distance that light travels through the tissue. Other

heights, however, of the partially cylindrical protrusion 605 can also accomplish this objective. For example, the chosen height of the partially cylindrical protrusion 605 can be selected based on the size of the measurement site, whether the patient is an adult or child, and so on. In an embodiment, the height of the protrusion 605 is chosen to provide as much tissue thickness reduction as possible while reducing or preventing occlusion of blood vessels in the tissue.

Referring to FIG. 6D, the width of the partially cylindrical protrusion 605 (measurement "b") can be about 3 to about 5 mm. In one embodiment, the width is about 4 mm. In one embodiment, a width in this range provides good penetration of the partially cylindrical protrusion 605 into the tissue to reduce the path length of the light. Other widths, however, of the partially cylindrical protrusion 605 can also accomplish this objective. For example, the width of the partially cylindrical protrusion 605 can vary based on the size of the measurement site, whether the patient is an adult or child, and so on. In addition, the length of the protrusion 605 could be about 10 mm, or about 8 mm to about 12 mm, or smaller than 8 mm or greater than 12 mm.

In certain embodiments, the focal length (f) for the partially cylindrical protrusion 605 can be expressed as:

$$f = \frac{R}{n-1},$$

where R is the radius of curvature of the partial cylinder 608 and n is the index of refraction of the material used. In certain embodiments, the radius of curvature can be between about 1.5 mm and about 2 mm. In another embodiment, the partially cylindrical protrusion 605 can include a material, such as nBK7 glass, with an index of refraction of around 1.5 at 1300 nm, which can provide focal lengths of between about 3 mm and about 4 mm.

A partially cylindrical protrusion 605 having a material with a higher index of refraction such as nSF11 glass (e.g., n=1.75 at 1300 nm) can provide a shorter focal length and possibly a smaller photodiode chip, but can also cause higher reflections due to the index of refraction mismatch with air. Many types of glass or plastic can be used with index of refraction values ranging from, for example, about 1.4 to about 1.9. The index of refraction of the material of the protrusion 605 can be chosen to improve or optimize the light focusing properties of the protrusion 605. A plastic partially cylindrical protrusion 605 could provide the cheapest option in high volumes but can also have some undesired light absorption peaks at wavelengths higher than 1500 nm. Other focal lengths and materials having different indices of refraction can be used for the partially cylindrical protrusion 605.

Placing a photodiode at a given distance below the partially cylindrical protrusion 605 can facilitate capturing some or all of the light traveling perpendicular to the lens within the active area of the photodiode (see FIG. 14). Different sizes of the partially cylindrical protrusion 605 can use different sizes of photodiodes. The extension 610 added onto the bottom of the partial cylinder 608 is used in certain embodiments to increase the height of the partially cylindrical protrusion 605. In an embodiment, the added height is such that the photodiodes are at or are approximately at the focal length of the partially cylindrical protrusion 605. In an embodiment, the added height provides for greater thinning of the measurement site. In an embodiment, the added height assists in deflecting light piped through the sensor. This is because light piped around the sensor passes through the side walls of the

added height without being directed toward the detectors. The extension **610** can also further facilitate the protrusion **605** increasing or maximizing the amount of light that is provided to the detectors. In some embodiments, the extension **610** can be omitted.

FIG. 6E illustrates another view of the sensor **301f** of FIG. 3F, which includes an embodiment of a partially cylindrical protrusion **605b**. Like the sensor **301A** shown in FIGS. 3B and 3C, the sensor **301f** includes a finger bed **310f**. The finger bed **310f** includes a generally curved surface shaped generally to receive tissue, such as a human digit. The finger bed **310f** also includes the ridges or channels **314** described above with respect to FIGS. 3B and 3C.

The example of finger bed **310f** shown also includes the protrusion **605b**, which includes the features of the protrusion **605** described above. In addition, the protrusion **605b** also includes chamfered edges **607** on each end to provide a more comfortable surface for a finger to slide across (see also FIG. 14D). In another embodiment, the protrusion **605b** could instead include a single chamfered edge **607** proximal to the ridges **314**. In another embodiment, one or both of the chamfered edges **607** could be rounded.

The protrusion **605b** also includes a measurement site contact area **670** that can contact body tissue of a measurement site. The protrusion **605b** can be removed from or integrated with the finger bed **310f**. Interchangeable, differently shaped protrusions **605b** can also be provided, which can correspond to different finger shapes, characteristics, opacity, sizes, or the like.

FIGS. 7A and 7B illustrate block diagrams of sensors **701** that include example arrangements of conductive glass or conductive coated glass for shielding. Advantageously, in certain embodiments, the shielding can provide increased SNR. The features of the sensors **701** can be implemented with any of the sensors **101**, **201**, **301** described above. Although not shown, the partially cylindrical protrusion **605** of FIG. 6 can also be used with the sensors **701** in certain embodiments.

For example, referring specifically to FIG. 7A, the sensor **701a** includes an emitter housing **704a** and a detector housing **706**. The emitter housing **704a** includes LEDs **104**. The detector housing **706a** includes a tissue bed **710a** with an opening or window **703a**, the conductive glass **730a**, and one or more photodiodes for detectors **106** provided on a sub-mount **707a**.

During operation, a finger **102** can be placed on the tissue bed **710a** and optical radiation can be emitted from the LEDs **104**. Light can then be attenuated as it passes through or is reflected from the tissue of the finger **102**. The attenuated light can then pass through the opening **703a** in the tissue bed **710a**. Based on the received light, the detectors **106** can provide a detector signal **107**, for example, to the front end interface **108** (see FIG. 1).

In the depicted embodiment, the conductive glass **730** is provided in the opening **703**. The conductive glass **730** can thus not only permit light from the finger to pass to the detectors **106**, but it can also supplement the shielding of the detectors **106** from noise. The conductive glass **730** can include a stack or set of layers. In FIG. 7A, the conductive glass **730a** is shown having a glass layer **731** proximate the finger **102** and a conductive layer **733** electrically coupled to the shielding **790a**.

In an embodiment, the conductive glass **730a** can be coated with a conductive, transparent or partially transparent material, such as a thin film of indium tin oxide (ITO). To supplement electrical shielding effects of a shielding enclosure **790a**, the conductive glass **730a** can be electrically coupled to

the shielding enclosure **790a**. The conductive glass **730a** can be electrically coupled to the shielding **704a** based on direct contact or via other connection devices, such as a wire or another component.

The shielding enclosure **790a** can be provided to encompass the detectors **106** to reduce or prevent noise. For example, the shielding enclosure **790a** can be constructed from a conductive material, such as copper, in the form of a metal cage. The shielding or enclosure **a** can include an opaque material to not only reduce electrical noise, but also ambient optical noise.

In some embodiments, the shielding enclosure **790a** can be constructed in a single manufactured component with or without the use of conductive glass. This form of construction may be useful in order to reduce costs of manufacture as well as assist in quality control of the components. Furthermore, the shielding enclosure **790a** can also be used to house various other components, such as sigma delta components for various embodiments of front end interfaces **108**.

Referring to FIG. 7B, another block diagram of an example sensor **701b** is shown. A tissue bed **710b** of the sensor **701b** includes a protrusion **705b**, which is in the form of a convex bump. The protrusion **705b** can include all of the features of the protrusions or tissue shaping materials described above. For example, the protrusion **705b** includes a contact area **370** that comes in contact with the finger **102** and which can include one or more openings **703b**. One or more components of conductive glass **730b** can be provided in the openings **703**. For example, in an embodiment, each of the openings **703** can include a separate window of the conductive glass **730b**. In an embodiment, a single piece of the conductive glass **730b** can use for some or all of the openings **703b**. The conductive glass **730b** is smaller than the conductive glass **730a** in this particular embodiment.

A shielding enclosure **790b** is also provided, which can have all the features of the shielding enclosure **790a**. The shielding enclosure **790b** is smaller than the shielding enclosure **790a**; however, a variety of sizes can be selected for the shielding enclosures **790**.

In some embodiments, the shielding enclosure **790b** can be constructed in a single manufactured component with or without the use of conductive glass. This form of construction may be useful in order to reduce costs of manufacture as well as assist in quality control of the components. Furthermore, the shielding enclosure **790b** can also be used to house various other components, such as sigma delta components for various embodiments of front end interfaces **108**.

FIGS. 8A through 8D illustrate a perspective view, side views, and a bottom elevation view of the conductive glass described above with respect to the sensors **701a**, **701b**. As shown in the perspective view of FIG. 8A and side view of FIG. 8B, the conductive glass **730** includes the electrically conductive material **733** described above as a coating on the glass layer **731** described above to form a stack. In an embodiment where the electrically conductive material **733** includes indium tin oxide, surface resistivity of the electrically conductive material **733** can range approximately from 30 ohms per square inch to 500 ohms per square inch, or approximately 30, 200, or 500 ohms per square inch. As would be understood by a person of skill in the art from the present disclosure, other resistivities can also be used which are less than 30 ohms or more than 500 ohms. Other transparent, electrically conductive materials can be used as the material **733**.

Although the conductive material **733** is shown spread over the surface of the glass layer **731**, the conductive material **733** can be patterned or provided on selected portions of the glass

layer **731**. Furthermore, the conductive material **733** can have uniform or varying thickness depending on a desired transmission of light, a desired shielding effect, and other considerations.

In FIG. **8C**, a side view of a conductive glass **830a** is shown to illustrate an embodiment where the electrically conductive material **733** is provided as an internal layer between two glass layers **731**, **835**. Various combinations of integrating electrically conductive material **733** with glass are possible. For example, the electrically conductive material **733** can be a layer within a stack of layers. This stack of layers can include one or more layers of glass **731**, **835**, as well as one or more layers of conductive material **733**. The stack can include other layers of materials to achieve desired characteristics.

In FIG. **8D**, a bottom perspective view is shown to illustrate an embodiment where a conductive glass **830b** can include conductive material **837** that occupies or covers a portion of a glass layer **839**. This embodiment can be useful, for example, to create individual, shielded windows for detectors **106**, such as those shown in FIG. **3C**. The conductive material **837** can be patterned to include an area **838** to allow light to pass to detectors **106** and one or more strips **841** to couple to the shielding **704** of FIG. **7**.

Other configurations and patterns for the conductive material can be used in certain embodiments, such as, for example, a conductive coating lining periphery edges, a conductive coating outlaid in a pattern including a grid or other pattern, a speckled conductive coating, coating outlaid in lines in either direction or diagonally, varied thicknesses from the center out or from the periphery in, or other suitable patterns or coatings that balance the shielding properties with transparency considerations.

FIG. **9** depicts an example graph **900** that illustrates comparative results obtained by an example sensor having components similar to those disclosed above with respect to FIGS. **7** and **8**. The graph **900** depicts the results of the percentage of transmission of varying wavelengths of light for different types of windows used in the sensors described above.

A line **915** on the graph **900** illustrates example light transmission of a window made from plain glass. As shown, the light transmission percentage of varying wavelengths of light is approximately 90% for a window made from plain glass. A line **920** on the graph **900** demonstrates an example light transmission percentage for an embodiment in which a window is made from glass having an ITO coating with a surface resistivity of 500 ohms per square inch. A line **925** on the graph **900** shows an example light transmission for an embodiment in which a window is made from glass that includes a coating of ITO oxide with a surface resistivity of 200 ohms per square inch. A line **930** on the graph **900** shows an example light transmission for an embodiment in which a window is made from glass that includes a coating of ITO oxide with a surface resistivity of 30 ohms per square inch.

The light transmission percentage for a window with currently available embedded wiring can have a light transmission percentage of approximately 70%. This lower percentage of light transmission can be due to the opacity of the wiring employed in a currently available window with wiring. Accordingly, certain embodiments of glass coatings described herein can employ, for example, ITO coatings with different surface resistivity depending on the desired light transmission, wavelengths of light used for measurement, desired shielding effect, and other criteria.

FIGS. **10A** through **10B** illustrate comparative noise floors of example implementations of the sensors described above. Noise can include optical noise from ambient light and elec-

tromagnetic noise, for example, from surrounding electrical equipment. In FIG. **10A**, a graph **1000** depicts possible noise floors for different frequencies of noise for an embodiment in which one of the sensors described above included separate windows for four (4) detectors **106**. One or more of the windows included an embedded grid of wiring as a noise shield. Symbols **1030-1033** illustrate the noise floor performance for this embodiment. As can be seen, the noise floor performance can vary for each of the openings and based on the frequency of the noise.

In FIG. **10B**, a graph **1050** depicts a noise floor for frequencies of noise **1070** for an embodiment in which the sensor included separate openings for four (4) detectors **106** and one or more windows that include an ITO coating. In this embodiment, a surface resistivity of the ITO used was about 500 ohms per square inch. Symbols **1080-1083** illustrate the noise floor performance for this embodiment. As can be seen, the noise floor performance for this embodiment can vary less for each of the openings and provide lower noise floors in comparison to the embodiment of FIG. **10A**.

FIG. **11A** illustrates an example structure for configuring the set of optical sources of the emitters described above. As shown, an emitter **104** can include a driver **1105**, a thermistor **1120**, a set of top-emitting LEDs **1102** for emitting red and/or infrared light, a set of side-emitting LEDs **1104** for emitting near infrared light, and a submount **1106**.

The thermistor **1120** can be provided to compensate for temperature variations. For example, the thermistor **1120** can be provided to allow for wavelength centroid and power drift of LEDs **1102** and **1104** due to heating. In addition, other thermistors (not shown) can be employed, for example, to measure a temperature of a measurement site. The temperature can be displayed on a display device and used by a caregiver. Such a temperature can also be helpful in correcting for wavelength drift due to changes in water absorption, which can be temperature dependent, thereby providing more accurate data useful in detecting blood analytes like glucose. In addition, using a thermistor or other type of temperature sensitive device may be useful for detecting extreme temperatures at the measurement site that are too hot or too cold. The presence of low perfusion may also be detected, for example, when the finger of a patient has become too cold. Moreover, shifts in temperature at the measurement site can alter the absorption spectrum of water and other tissue in the measurement site. A thermistor's temperature reading can be used to adjust for the variations in absorption spectrum changes in the measurement site.

The driver **1105** can provide pulses of current to the emitter **1104**. In an embodiment, the driver **1105** drives the emitter **1104** in a progressive fashion, for example, in an alternating manner based on a control signal from, for example, a processor (e.g., the processor **110**). For example, the driver **1105** can drive the emitter **1104** with a series of pulses to about 1 milliwatt (mW) for visible light to light at about 1300 nm and from about 40 mW to about 100 mW for light at about 1600 nm to about 1700 nm. However, a wide number of driving powers and driving methodologies can be used. The driver **1105** can be synchronized with other parts of the sensor and can minimize or reduce any jitter in the timing of pulses of optical radiation emitted from the emitter **1104**. In some embodiments, the driver **1105** is capable of driving the emitter **1104** to emit an optical radiation in a pattern that varies by less than about 10 parts-per-million; however other amounts of variation can be used.

The submount **1106** provides a support structure in certain embodiments for aligning the top-emitting LEDs **1102** and the side-emitting LEDs **1104** so that their optical radiation is

transmitted generally towards the measurement site. In some embodiments, the submount **1106** is also constructed of aluminum nitride (AlN) or beryllium oxide (BEO) for heat dissipation, although other materials or combinations of materials suitable for the submount **1106** can be used.

FIG. **11B** illustrates a configuration of emitting optical radiation into a measurement site for measuring a blood constituent or analyte like glucose. In some embodiments, emitter **104** may be driven in a progressive fashion to minimize noise and increase SNR of sensor **101**. For example, emitter **104** may be driven based on a progression of power/current delivered to LEDs **1102** and **1104**.

In some embodiments, emitter **104** may be configured to emit pulses centered about 905 nm, about 1050 nm, about 1200 nm, about 1300 nm, about 1330 nm, about 1610 nm, about 1640 nm, and about 1665 nm. In another embodiment, the emitter **104** may emit optical radiation ranging from about 860 nm to about 950 nm, about 950 nm to about 1100 nm, about 1100 nm to about 1270 nm, about 1250 nm to about 1350 nm, about 1300 nm to about 1360 nm, and about 1590 nm to about 1700 nm. Of course, emitter **104** may be configured to transmit any of a variety of wavelengths of visible, or near-infrared optical radiation.

For purposes of illustration, FIG. **11B** shows a sequence of pulses of light at wavelengths of around 905 nm, around 1200 nm, around 1300 nm, and around 1330 nm from top emitting LEDs **1102**. FIG. **11B** also shows that emitter **104** may then emit pulses centered at around 1630 nm, around 1660 nm, and around 1615 nm from side emitting LEDs **1104**. Emitter **104** may be progressively driven at higher power/current. This progression may allow driver circuit **105** to stabilize in its operations, and thus, provide a more stable current/power to LEDs **1102** and **1104**.

For example, as shown in FIG. **11B**, the sequence of optical radiation pulses are shown having a logarithmic-like progression in power/current. In some embodiments, the timing of these pulses is based on a cycle of about 400 slots running at 48 kHz (e.g. each time slot may be approximately 0.02 ms or 20 microseconds). An artisan will recognize that term "slots" includes its ordinary meaning, which includes a time period that may also be expressed in terms of a frequency. In the example shown, pulses from top emitting LEDs **1102** may have a pulse width of about 40 time slots (e.g., about 0.8 ms) and an off period of about 4 time slots in between. In addition, pulses from side emitting LEDs **1104** (e.g., or a laser diode) may have a pulse width of about 60 time slots (e.g., about 1.25 ms) and a similar off period of about 4 time slots. A pause of about 70 time slots (e.g. 1.5 ms) may also be provided in order to allow driver circuit **1105** to stabilize after operating at higher current/power.

As shown in FIG. **11B**, top emitting LEDs **1102** may be initially driven with a power to approximately 1 mW at a current of about 20-100 mA. Power in these LEDs may also be modulated by using a filter or covering of black dye to reduce power output of LEDs. In this example, top emitting LEDs **1102** may be driven at approximately 0.02 to 0.08 mW. The sequence of the wavelengths may be based on the current requirements of top emitting LEDs **502** for that particular wavelength. Of course, in other embodiments, different wavelengths and sequences of wavelengths may be output from emitter **104**.

Subsequently, side emitting LEDs **1104** may be driven at higher powers, such as about 40-100 mW and higher currents of about 600-800 mA. This higher power may be employed in order to compensate for the higher opacity of tissue and water in measurement site **102** to these wavelengths. For example, as shown, pulses at about 1630 nm, about 1660 nm, and about

1615 nm may be output with progressively higher power, such as at about 40 mW, about 50 mW, and about 60 mW, respectively. In this embodiment, the order of wavelengths may be based on the optical characteristics of that wavelength in tissue as well as the current needed to drive side emitting LEDs **1104**. For example, in this embodiment, the optical pulse at about 1615 nm is driven at the highest power due to its sensitivity in detecting analytes like glucose and the ability of light at this wavelength to penetrate tissue. Of course, different wavelengths and sequences of wavelengths may be output from emitter **104**.

As noted, this progression may be useful in some embodiments because it allows the circuitry of driver circuit **1105** to stabilize its power delivery to LEDs **1102** and **1104**. Driver circuit **1105** may be allowed to stabilize based on the duty cycle of the pulses or, for example, by configuring a variable waiting period to allow for stabilization of driver circuit **1105**. Of course, other variations in power/current and wavelength may also be employed in the present disclosure.

Modulation in the duty cycle of the individual pulses may also be useful because duty cycle can affect the signal noise ratio of the system **100**. That is, as the duty cycle is increased so may the signal to noise ratio.

Furthermore, as noted above, driver circuit **1105** may monitor temperatures of the LEDs **1102** and **1104** using the thermistor **1120** and adjust the output of LEDs **1102** and **1104** accordingly. Such a temperature may be to help sensor **101** correct for wavelength drift due to changes in water absorption, which can be temperature dependent.

FIG. **11C** illustrates another exemplary emitter that may be employed in the sensor according to an embodiment of the disclosure. As shown, the emitter **104** can include components mounted on a substrate **1108** and on submount **1106**. In particular, top-emitting LEDs **1102** for emitting red and/or infrared light may be mounted on substrate **1108**. Side emitting LEDs **1104** may be mounted on submount **1106**. As noted, side-emitting LEDs **1104** may be included in emitter **104** for emitting near infrared light.

As also shown, the sensor of FIG. **11C** may include a thermistor **1120**. As noted, the thermistor **1120** can be provided to compensate for temperature variations. The thermistor **1120** can be provided to allow for wavelength centroid and power drift of LEDs **1102** and **1104** due to heating. In addition, other thermistors (not shown) can be employed, for example, to measure a temperature of a measurement site. Such a temperature can be helpful in correcting for wavelength drift due to changes in water absorption, which can be temperature dependent, thereby providing more accurate data useful in detecting blood analytes like glucose.

In some embodiments, the emitter **104** may be implemented without the use of side emitting LEDs. For example, certain blood constituents, such as total hemoglobin, can be measured by embodiments of the disclosure without the use of side emitting LEDs. FIG. **11D** illustrates another exemplary emitter that may be employed in the sensor according to an embodiment of the disclosure. In particular, an emitter **104** that is configured for a blood constituent, such as total hemoglobin, is shown. The emitter **104** can include components mounted on a substrate **1108**. In particular, top-emitting LEDs **1102** for emitting red and/or infrared light may be mounted on substrate **1108**.

As also shown, the emitter of FIG. **11D** may include a thermistor **1120**. The thermistor **1120** can be provided to compensate for temperature variations. The thermistor **1120** can be provided to allow for wavelength centroid and power drift of LEDs **1102** due to heating.

FIG. 12A illustrates a detector submount **1200** having photodiode detectors that are arranged in a grid pattern on the detector submount **1200** to capture light at different quadrants from a measurement site. One detector submount **1200** can be placed under each window of the sensors described above, or multiple windows can be placed over a single detector submount **1200**. The detector submount **1200** can also be used with the partially cylindrical protrusion **605** described above with respect to FIG. 6.

The detectors include photodiode detectors **1-4** that are arranged in a grid pattern on the submount **1200** to capture light at different quadrants from the measurement site. As noted, other patterns of photodiodes, such as a linear row, or logarithmic row, can also be employed in certain embodiments.

As shown, the detectors **1-4** may have a predetermined spacing from each other, or spatial relationship among one another that result in a spatial configuration. This spatial configuration can be configured to purposefully create a variation of path lengths among detectors **106** and the point light source discussed above.

Detectors may hold multiple (e.g., two, three, four, etc.) photodiode arrays that are arranged in a two-dimensional grid pattern. Multiple photodiode arrays may also be useful to detect light piping (i.e., light that bypasses measurement site **102**). As shown, walls may separate the individual photodiode arrays to prevent mixing of light signals from distinct quadrants. In addition, as noted, the detectors may be covered by windows of transparent material, such as glass, plastic, etc., to allow maximum transmission of power light captured. As noted, this window may comprise some shielding in the form of an embedded grid of wiring, or a conductive layer or coating.

FIGS. 12B through 12D illustrate a simplified view of exemplary arrangements and spatial configurations of photodiodes for detectors **106**. As shown, detectors **106** may comprise photodiode detectors **1-4** that are arranged in a grid pattern on detector submount **1200** to capture light at different quadrants from measurement site **102**.

As noted, other patterns of photodiodes may also be employed in embodiments of the present disclosure, including, for example, stacked or other configurations recognizable to an artisan from the disclosure herein. For example, detectors **106** may be arranged in a linear array, a logarithmic array, a two-dimensional array, and the like. Furthermore, an artisan will recognize from the disclosure herein that any number of detectors **106** may be employed by embodiments of the present disclosure.

For example, as shown in FIG. 12B, detectors **106** may comprise photodiode detectors **1-4** that are arranged in a substantially linear configuration on submount **1200**. In this embodiment shown, photodiode detectors **1-4** are substantially equally spaced apart (e.g., where the distance *D* is substantially the same between detectors **1-4**).

In FIG. 12C, photodiode detectors **1-4** may be arranged in a substantially linear configuration on submount **1200**, but may employ a substantially progressive, substantially logarithmic, or substantially semi-logarithmic spacing (e.g., where distances $D1 > D2 > D3$). This arrangement or pattern may be useful for use on a patient's finger and where the thickness of the finger gradually increases.

In FIG. 12D, a different substantially grid pattern on submount **1200** of photodiode detectors **1-4** is shown. As noted, other patterns of detectors may also be employed in embodiments of the present invention.

FIGS. 12E through 12H illustrate several embodiments of photodiodes that may be used in detectors **106**. As shown in

these figures, a photodiode **1202** of detector **106** may comprise a plurality of active areas **1204**. These active areas **204** may be coupled together via a common cathode **1206** or anode **1208** in order to provide a larger effective detection area.

In particular, as shown in FIG. 12E, photodiode **1202** may comprise two (2) active areas **1204a** and **1204b**. In FIG. 12F, photodiode **1202** may comprise four (4) active areas **1204c-f**. In FIG. 12G, photodiode **1202** may comprise three (3) active areas **1204g-i**. In FIG. 12H, photodiode **1202** may comprise nine (9) active areas **1204j-r**. The use of smaller active areas may be useful because smaller active areas can be easier to fabricate and can be fabricated with higher purity. However, one skilled in the art will recognize that various sizes of active areas may be employed in the photodiode **1202**.

FIG. 13 illustrates an example multi-stream process **1300**. The multi-stream process **1300** can be implemented by the data collection system **100** and/or by any of the sensors described above. As shown, a control signal from a signal processor **1310** controls a driver **1305**. In response, an emitter **1304** generates a pulse sequence **1303** from its emitter (e.g., its LEDs) into a measurement site or sites **1302**. As described above, in some embodiments, the pulse sequence **1303** is controlled to have a variation of about 10 parts per million or less. Of course, depending on the analyte desired, the tolerated variation in the pulse sequence **1303** can be greater (or smaller).

In response to the pulse sequence **1300**, detectors **1** to *n* (*n* being an integer) in a detector **1306** capture optical radiation from the measurement site **1302** and provide respective streams of output signals. Each signal from one of detectors **1-n** can be considered a stream having respective time slots corresponding to the optical pulses from emitter sets **1-n** in the emitter **1304**. Although *n* emitters and *n* detectors are shown, the number of emitters and detectors need not be the same in certain implementations.

A front end interface **1308** can accept these multiple streams from detectors **1-n** and deliver one or more signals or composite signal(s) back to the signal processor **1310**. A stream from the detectors **1-n** can thus include measured light intensities corresponding to the light pulses emitted from the emitter **1304**.

The signal processor **1310** can then perform various calculations to measure the amount of glucose and other analytes based on these multiple streams of signals. In order to help explain how the signal processor **1310** can measure analytes like glucose, a primer on the spectroscopy employed in these embodiments will now be provided.

Spectroscopy is premised upon the Beer-Lambert law. According to this law, the properties of a material, e.g., glucose present in a measurement site, can be deterministically calculated from the absorption of light traveling through the material. Specifically, there is a logarithmic relation between the transmission of light through a material and the concentration of a substance and also between the transmission and the length of the path traveled by the light. As noted, this relation is known as the Beer-Lambert law.

The Beer-Lambert law is usually written as:

Absorbance $A = m * b * c$, where:

m is the wavelength-dependent molar absorptivity coefficient (usually expressed in units of $M^{-1} cm^{-1}$);
b is the mean path length; and
c is the analyte concentration (e.g., the desired parameter).

In spectroscopy, instruments attempt to obtain the analyte concentration (c) by relating absorbance (A) to transmittance (T). Transmittance is a proportional value defined as:

$$T = I/I_o, \text{ where:}$$

I is the light intensity measured by the instrument from the measurement site; and

I_o is the initial light intensity from the emitter.

Absorbance (A) can be equated to the transmittance (T) by the equation:

$$A = -\log T$$

Therefore, substituting equations from above:

$$A = -\log(I/I_o)$$

In view of this relationship, spectroscopy thus relies on a proportional-based calculation of $-\log(I/I_o)$ and solving for analyte concentration (c).

Typically, in order to simplify the calculations, spectroscopy will use detectors that are at the same location in order to keep the path length (b) a fixed, known constant. In addition, spectroscopy will employ various mechanisms to definitively know the transmission power (I_o), such as a photodiode located at the light source. This architecture can be viewed as a single channel or single stream sensor, because the detectors are at a single location.

However, this scheme can encounter several difficulties in measuring analytes, such as glucose. This can be due to the high overlap of absorption of light by water at the wavelengths relevant to glucose as well as other factors, such as high self-noise of the components.

Embodiments of the present disclosure can employ a different approach that in part allows for the measurement of analytes like glucose. Some embodiments can employ a bulk, non-pulsatile measurement in order to confirm or validate a pulsatile measurement. In addition, both the non-pulsatile and pulsatile measurements can employ, among other things, the multi-stream operation described above in order to attain sufficient SNR. In particular, a single light source having multiple emitters can be used to transmit light to multiple detectors having a spatial configuration.

A single light source having multiple emitters can allow for a range of wavelengths of light to be used. For example, visible, infrared, and near infrared wavelengths can be employed. Varying powers of light intensity for different wavelengths can also be employed.

Secondly, the use of multiple-detectors in a spatial configuration allow for a bulk measurement to confirm or validate that the sensor is positioned correctly. This is because the multiple locations of the spatial configuration can provide, for example, topology information that indicates where the sensor has been positioned. Currently available sensors do not provide such information. For example, if the bulk measurement is within a predetermined range of values, then this can indicate that the sensor is positioned correctly in order to perform pulsatile measurements for analytes like glucose. If the bulk measurement is outside of a certain range or is an unexpected value, then this can indicate that the sensor should be adjusted, or that the pulsatile measurements can be processed differently to compensate, such as using a different calibration curve or adjusting a calibration curve. This feature and others allow the embodiments to achieve noise cancellation and noise reduction, which can be several times greater in magnitude than what is achievable by currently available technology.

In order to help illustrate aspects of the multi-stream measurement approach, the following example derivation is provided. Transmittance (T) can be expressed as:

$$T = e^{-m \cdot b \cdot c}$$

In terms of light intensity, this equation can also be rewritten as:

$$I/I_o = e^{-m \cdot b \cdot c}$$

Or, at a detector, the measured light (I) can be expressed as:

$$I = I_o \cdot e^{-m \cdot b \cdot c}$$

As noted, in the present disclosure, multiple detectors (1 to n) can be employed, which results in $I_1 \dots I_n$ streams of measurements. Assuming each of these detectors have their own path lengths, $b_1 \dots b_n$, from the light source, the measured light intensities can be expressed as:

$$I_n = I_o \cdot e^{-m \cdot b_n \cdot c}$$

The measured light intensities at any two different detectors can be referenced to each other. For example:

$$I_1/I_n = (I_o \cdot e^{-m \cdot b_1 \cdot c}) / (I_o \cdot e^{-m \cdot b_n \cdot c})$$

As can be seen, the terms, I_o , cancel out and, based on exponent algebra, the equation can be rewritten as:

$$I_1/I_n = e^{-m(b_1 - b_n)c}$$

From this equation, the analyte concentration (c) can now be derived from bulk signals $I_1 \dots I_n$ and knowing the respective mean path lengths b_1 and b_n . This scheme also allows for the cancelling out of I_o , and thus, noise generated by the emitter **1304** can be cancelled out or reduced. In addition, since the scheme employs a mean path length difference, any changes in mean path length and topological variations from patient to patient are easily accounted. Furthermore, this bulk-measurement scheme can be extended across multiple wavelengths. This flexibility and other features allow embodiments of the present disclosure to measure blood analytes like glucose.

For example, as noted, the non-pulsatile, bulk measurements can be combined with pulsatile measurements to more accurately measure analytes like glucose. In particular, the non-pulsatile, bulk measurement can be used to confirm or validate the amount of glucose, protein, etc. in the pulsatile measurements taken at the tissue at the measurement site(s) **1302**. The pulsatile measurements can be used to measure the amount of glucose, hemoglobin, or the like that is present in the blood. Accordingly, these different measurements can be combined to thus determine analytes like blood glucose.

FIG. **14A** illustrates an embodiment of a detector submount **1400a** positioned beneath the partially cylindrical protrusion **605** of FIG. **6** (or alternatively, the protrusion **605b**). The detector submount **1400a** includes two rows **1408a** of detectors **1410a**. The partially cylindrical protrusion **605** can facilitate reducing the number and/or size of detectors used in a sensor because the protrusion **605** can act as a lens that focuses light onto a smaller area.

To illustrate, in some sensors that do not include the partially cylindrical protrusion **605**, sixteen detectors can be used, including four rows of four detectors each. Multiple rows of detectors can be used to measure certain analytes, such as glucose or total hemoglobin, among others. Multiple rows of detectors can also be used to detect light piping (e.g., light that bypasses the measurement site). However, using more detectors in a sensor can add cost, complexity, and noise to the sensor.

Applying the partially cylindrical protrusion **605** to such a sensor, however, could reduce the number of detectors or

rows of detectors used while still receiving the substantially same amount of light, due to the focusing properties of the protrusion 605 (see FIG. 14B). This is the example situation illustrated in FIG. 14—two rows 1408a of detectors 1410a are used instead of four. Advantageously, in certain embodiments, the resulting sensor can be more cost effective, have less complexity, and have an improved SNR, due to fewer and/or smaller photodiodes.

In other embodiments, using the partially cylindrical protrusion 605 can allow the number of detector rows to be reduced to one or three rows of four detectors. The number of detectors in each row can also be reduced. Alternatively, the number of rows might not be reduced but the size of the detectors can be reduced. Many other configurations of detector rows and sizes can also be provided.

FIG. 14B depicts a front elevation view of the partially cylindrical protrusion 605 (or alternatively, the protrusion 605b) that illustrates how light from emitters (not shown) can be focused by the protrusion 605 onto detectors. The protrusion 605 is placed above a detector submount 1400b having one or more detectors 1410b disposed thereon. The submount 1400b can include any number of rows of detectors 1410, although one row is shown.

Light, represented by rays 1420, is emitted from the emitters onto the protrusion 605. These light rays 1420 can be attenuated by body tissue (not shown). When the light rays 1420 enter the protrusion 605, the protrusion 605 acts as a lens to refract the rays into rays 1422. This refraction is caused in certain embodiments by the partially cylindrical shape of the protrusion 605. The refraction causes the rays 1422 to be focused or substantially focused on the one or more detectors 1410b. Since the light is focused on a smaller area, a sensor including the protrusion 605 can include fewer detectors to capture the same amount of light compared with other sensors.

FIG. 14C illustrates another embodiment of a detector submount 1400c, which can be disposed under the protrusion 605b (or alternatively, the protrusion 605). The detector submount 1400c includes a single row 1408c of detectors 1410c. The detectors are electrically connected to conductors 1412c, which can be gold, silver, copper, or any other suitable conductive material.

The detector submount 1400c is shown positioned under the protrusion 605b in a detector subassembly 1450 illustrated in FIG. 14D. A top-down view of the detector subassembly 1450 is also shown in FIG. 14E. In the detector subassembly 1450, a cylindrical housing 1430 is disposed on the submount 1400c. The cylindrical housing 1430 includes a transparent cover 1432, upon which the protrusion 605b is disposed. Thus, as shown in FIG. 14D, a gap 1434 exists between the detectors 1410c and the protrusion 605b. The height of this gap 1434 can be chosen to increase or maximize the amount of light that impinges on the detectors 1410c.

The cylindrical housing 1430 can be made of metal, plastic, or another suitable material. The transparent cover 1432 can be fabricated from glass or plastic, among other materials. The cylindrical housing 1430 can be attached to the submount 1400c at the same time or substantially the same time as the detectors 1410c to reduce manufacturing costs. A shape other than a cylinder can be selected for the housing 1430 in various embodiments.

In certain embodiments, the cylindrical housing 1430 (and transparent cover 1432) forms an airtight or substantially airtight or hermetic seal with the submount 1400c. As a result, the cylindrical housing 1430 can protect the detectors 1410c and conductors 1412c from fluids and vapors that can cause corrosion. Advantageously, in certain embodiments, the

cylindrical housing 1430 can protect the detectors 1410c and conductors 1412c more effectively than currently-available resin epoxies, which are sometimes applied to solder joints between conductors and detectors.

In embodiments where the cylindrical housing 1430 is at least partially made of metal, the cylindrical housing 1430 can provide noise shielding for the detectors 1410c. For example, the cylindrical housing 1430 can be soldered to a ground connection or ground plane on the submount 1400c, which allows the cylindrical housing 1430 to reduce noise. In another embodiment, the transparent cover 1432 can include a conductive material or conductive layer, such as conductive glass or plastic. The transparent cover 1432 can include any of the features of the noise shields 790 described above.

The protrusion 605b includes the chamfered edges 607 described above with respect to FIG. 6E. These chamfered edges 607 can allow a patient to more comfortably slide a finger over the protrusion 605b when inserting the finger into the sensor 301f.

FIG. 14F illustrates a portion of the detector shell 306f, which includes the detectors 1410c on the substrate 1400c. The substrate 1400c is enclosed by a shielding enclosure 1490, which can include the features of the shielding enclosures 790a, 790b described above (see also FIG. 17). The shielding enclosure 1490 can be made of metal. The shielding enclosure 1490 includes a window 1492a above the detectors 1410c, which allows light to be transmitted onto the detectors 1410c.

A noise shield 1403 is disposed above the shielding enclosure 1490. The noise shield 1403, in the depicted embodiment, includes a window 1492a corresponding to the window 1492a. Each of the windows 1492a, 1492b can include glass, plastic, or can be an opening without glass or plastic. In some embodiments, the windows 1492a, 1492b may be selected to have different sizes or shapes from each other.

The noise shield 1403 can include any of the features of the conductive glass described above. In the depicted embodiment, the noise shield 1403 extends about three-quarters of the length of the detector shell 306f. In other embodiments, the noise shield 1403 could be smaller or larger. The noise shield 1403 could, for instance, merely cover the detectors 1410c, the submount 1400c, or a portion thereof. The noise shield 1403 also includes a stop 1413 for positioning a measurement site within the sensor 301f. Advantageously, in certain embodiments, the noise shield 1403 can reduce noise caused by light piping.

A thermistor 1470 is also shown. The thermistor 1470 is attached to the submount 1400c and protrudes above the noise shield 1403. As described above, the thermistor 1470 can be employed to measure a temperature of a measurement site. Such a temperature can be helpful in correcting for wavelength drift due to changes in water absorption, which can be temperature dependent, thereby providing more accurate data useful in detecting blood analytes like glucose.

In the depicted embodiment, the detectors 1410c are not enclosed in the cylindrical housing 1430. In an alternative embodiment, the cylindrical housing 1430 encloses the detectors 1410c and is disposed under the noise shield 1403. In another embodiment, the cylindrical housing 1430 encloses the detectors 1410c and the noise shield 1403 is not used. If both the cylindrical housing 1430 and the noise shield 1403 are used, either or both can have noise shielding features.

FIG. 14G illustrates the detector shell 306f of FIG. 14F, with the finger bed 310f disposed thereon. FIG. 14H illustrates the detector shell 306f of FIG. 14G, with the protrusion 605b disposed in the finger bed 310f.

FIG. 14I illustrates a cutaway view of the sensor 301f. Not all features of the sensor 301f are shown, such as the protrusion 605b. Features shown include the emitter and detector shells 304f, 306f; the flaps 307f; the heat sink 350f and fins 351f; the finger bed 310f; and the noise shield 1403.

In addition to these features, emitters 1404 are depicted in the emitter shell 304f. The emitters 1404 are disposed on a submount 1401, which is connected to a circuit board 1419. The emitters 1404 are also enclosed within a cylindrical housing 1480. The cylindrical housing 1480 can include all of the features of the cylindrical housing 1430 described above. For example, the cylindrical housing 1480 can be made of metal, can be connected to a ground plane of the submount 1401 to provide noise shielding, and can include a transparent cover 1482.

The cylindrical housing 1480 can also protect the emitters 1404 from fluids and vapors that can cause corrosion. Moreover, the cylindrical housing 1480 can provide a gap between the emitters 1404 and the measurement site (not shown), which can allow light from the emitters 1404 to even out or average out before reaching the measurement site.

The heat sink 350f, in addition to including the fins 351f, includes a protuberance 352f that extends down from the fins 351f and contacts the submount 1401. The protuberance 352f can be connected to the submount 1401, for example, with thermal paste or the like. The protuberance 352f can sink heat from the emitters 1404 and dissipate the heat via the fins 351f.

FIGS. 15A and 15B illustrate embodiments of sensor portions 1500A, 1500B that include alternative heat sink features to those described above. These features can be incorporated into any of the sensors described above. For example, any of the sensors above can be modified to use the heat sink features described below instead of or in addition to the heat sink features of the sensors described above.

The sensor portions 1500A, 1500B shown include LED emitters 1504; however, for ease of illustration, the detectors have been omitted. The sensor portions 1500A, 1500B shown can be included, for example, in any of the emitter shells described above.

The LEDs 1504 of the sensor portions 1500A, 1500B are connected to a substrate or submount 1502. The submount 1502 can be used in place of any of the submounts described above. The submount 1502 can be a non-electrically conducting material made of any of a variety of materials, such as ceramic, glass, or the like. A cable 1512 is attached to the submount 1502 and includes electrical wiring 1514, such as twisted wires and the like, for communicating with the LEDs 1504. The cable 1512 can correspond to the cables 212 described above.

Although not shown, the cable 1512 can also include electrical connections to a detector. Only a portion of the cable 1512 is shown for clarity. The depicted embodiment of the cable 1512 includes an outer jacket 1510 and a conductive shield 1506 disposed within the outer jacket 1510. The conductive shield 1506 can be a ground shield or the like that is made of a metal such as braided copper or aluminum. The conductive shield 1506 or a portion of the conductive shield 1506 can be electrically connected to the submount 1502 and can reduce noise in the signal generated by the sensor 1500A, 1500B by reducing RF coupling with the wires 1514. In alternative embodiments, the cable 1512 does not have a conductive shield. For example, the cable 1512 could be a twisted pair cable or the like, with one wire of the twisted pair used as a heat sink.

Referring specifically to FIG. 15A, in certain embodiments, the conductive shield 1506 can act as a heat sink for the LEDs 1504 by absorbing thermal energy from the LEDs 1504

and/or the submount 1502. An optional heat insulator 1520 in communication with the submount 1502 can also assist with directing heat toward the conductive shield 1506. The heat insulator 1520 can be made of plastic or another suitable material. Advantageously, using the conductive shield 1506 in the cable 1512 as a heat sink can, in certain embodiments, reduce cost for the sensor.

Referring to FIG. 15B, the conductive shield 1506 can be attached to both the submount 1502 and to a heat sink layer 1530 sandwiched between the submount 1502 and the optional insulator 1520. Together, the heat sink layer 1530 and the conductive shield 1506 in the cable 1512 can absorb at least part of the thermal energy from the LEDs and/or the submount 1502.

FIGS. 15C and 15D illustrate implementations of a sensor portion 1500C that includes the heat sink features of the sensor portion 1500A described above with respect to FIG. 15A. The sensor portion 1500C includes the features of the sensor portion 1500A, except that the optional insulator 1520 is not shown. FIG. 15D is a side cutaway view of the sensor portion 1500C that shows the emitters 1504.

The cable 1512 includes the outer jacket 1510 and the conductive shield 1506. The conductive shield 1506 is soldered to the submount 1502, and the solder joint 1561 is shown. In some embodiments, a larger solder joint 1561 can assist with removing heat more rapidly from the emitters 1504. Various connections 1563 between the submount 1502 and a circuit board 1519 are shown. In addition, a cylindrical housing 1580, corresponding to the cylindrical housing 1480 of FIG. 14I, is shown protruding through the circuit board 1519. The emitters 1504 are enclosed in the cylindrical housing 1580.

FIGS. 15E and 15F illustrate implementations of a sensor portion 1500E that includes the heat sink features of the sensor portion 1500B described above with respect to FIG. 15B. The sensor portion 1500E includes the heat sink layer 1530. The heat sink layer 1530 can be a metal plate, such as a copper plate or the like. The optional insulator 1520 is not shown. FIG. 15F is a side cutaway view of the sensor portion 1500E that shows the emitters 1504.

In the depicted embodiment, the conductive shield 1506 of the cable 1512 is soldered to the heat sink layer 1530 instead of the submount 1502. The solder joint 1565 is shown. In some embodiments, a larger solder joint 1565 can assist with removing heat more rapidly from the emitters 1504. Various connections 1563 between the submount 1502 and a circuit board 1519 are shown. In addition, the cylindrical housing 1580 is shown protruding through the circuit board 1519. The emitters 1504 are enclosed in the cylindrical housing 1580.

FIGS. 15G and 15H illustrate embodiments of connector features that can be used with any of the sensors described above with respect to FIGS. 1 through 15F. Referring to FIG. 15G, the circuit board 1519 includes a female connector 1575 that mates with a male connector 1577 connected to a daughter board 1587. The daughter board 1587 includes connections to the electrical wiring 1514 of the cable 1512. The connected boards 1519, 1587 are shown in FIG. 15H. Also shown is a hole 1573 that can receive the cylindrical housing 1580 described above.

Advantageously, in certain embodiments, using a daughter board 1587 to connect to the circuit board 1519 can enable connections to be made more easily to the circuit board 1519. In addition, using separate boards can be easier to manufacture than a single circuit board 1519 with all connections soldered to the circuit board 1519.

FIG. 15I illustrates an exemplary architecture for front-end interface 108 as a transimpedance-based front-end. As noted,

front-end interfaces **108** provide an interface that adapts the output of detectors **106** into a form that can be handled by signal processor **110**. As shown in this figure, sensor **101** and front-end interfaces **108** may be integrated together as a single component, such as an integrated circuit. Of course, one skilled in the art will recognize that sensor **101** and front-end interfaces **108** may comprise multiple components or circuits that are coupled together.

Front-end interfaces **108** may be implemented using transimpedance amplifiers that are coupled to analog to digital converters in a sigma delta converter. In some embodiments, a programmable gain amplifier (PGA) can be used in combination with the transimpedance-based front-ends. For example, the output of a transimpedance-based front-end may be output to a sigma-delta ADC that comprises a PGA. A PGA may be useful in order to provide another level of amplification and control of the stream of signals from detectors **106**. The PGA may be an integrated circuit or built from a set of micro-relays. Alternatively, the PGA and ADC components in converter **900** may be integrated with the transimpedance-based front-end in sensor **101**.

Due to the low-noise requirements for measuring blood analytes like glucose and the challenge of using multiple photodiodes in detector **106**, the applicants developed a noise model to assist in configuring front-end **108**. Conventionally, those skilled in the art have focused on optimizing the impedance of the transimpedance amplifiers to minimize noise.

However, the following noise model was discovered by the applicants:

$$\text{Noise} = \sqrt{aR + bR^2}, \text{ where:}$$

aR is characteristic of the impedance of the transimpedance amplifier; and

bR^2 is characteristic of the impedance of the photodiodes in detector and the number of photodiodes in detector **106**.

The foregoing noise model was found to be helpful at least in part due to the high SNR required to measure analytes like glucose. However, the foregoing noise model was not previously recognized by artisans at least in part because, in conventional devices, the major contributor to noise was generally believed to originate from the emitter or the LEDs. Therefore, artisans have generally continued to focus on reducing noise at the emitter.

However, for analytes like glucose, the discovered noise model revealed that one of the major contributors to noise was generated by the photodiodes. In addition, the amount of noise varied based on the number of photodiodes coupled to a transimpedance amplifier. Accordingly, combinations of various photodiodes from different manufacturers, different impedance values with the transimpedance amplifiers, and different numbers of photodiodes were tested as possible embodiments.

In some embodiments, different combinations of transimpedance to photodiodes may be used. For example, detectors **1-4** (as shown, e.g., in FIG. **12A**) may each comprise four photodiodes. In some embodiments, each detector of four photodiodes may be coupled to one or more transimpedance amplifiers. The configuration of these amplifiers may be set according to the model shown in FIG. **15J**.

Alternatively, each of the photodiodes may be coupled to its own respective transimpedance amplifier. For example, transimpedance amplifiers may be implemented as integrated circuits on the same circuit board as detectors **1-4**. In this embodiment, the transimpedance amplifiers may be grouped into an averaging (or summing) circuit, which are known to those skilled in the art, in order to provide an output stream from the detector. The use of a summing amplifier to combine

outputs from several transimpedance amplifiers into a single, analog signal may be helpful in improving the SNR relative to what is obtainable from a single transimpedance amplifier. The configuration of the transimpedance amplifiers in this setting may also be set according to the model shown in FIG. **15J**.

As yet another alternative, as noted above with respect to FIGS. **12E** through **12H**, the photodiodes in detectors **106** may comprise multiple active areas that are grouped together. In some embodiments, each of these active areas may be provided its own respective transimpedance. This form of pairing may allow a transimpedance amplifier to be better matched to the characteristics of its corresponding photodiode or active area of a photodiode.

As noted, FIG. **15J** illustrates an exemplary noise model that may be useful in configuring transimpedance amplifiers. As shown, for a given number of photodiodes and a desired SNR, an optimal impedance value for a transimpedance amplifier could be determined.

For example, an exemplary "4 PD per stream" sensor **1502** is shown where detector **106** comprises four photodiodes **1502**. The photodiodes **1502** are coupled to a single transimpedance amplifier **1504** to produce an output stream **1506**. In this example, the transimpedance amplifier comprises 10 M Ω resistors **1508** and **1510**. Thus, output stream **1506** is produced from the four photodiodes (PD) **1502**. As shown in the graph of FIG. **15J**, the model indicates that resistance values of about 10 M Ω may provide an acceptable SNR for analytes like glucose.

However, as a comparison, an exemplary "1 PD per stream" sensor **1512** is also shown in FIG. **15J**. In particular, sensor **1512** may comprise a plurality of detectors **106** that each comprises a single photodiode **1514**. In addition, as shown for this example configuration, each of photodiodes **1514** may be coupled to respective transimpedance amplifiers **1516**, e.g., 1 PD per stream. Transimpedance amplifiers are shown having 40 M Ω resistors **1518**. As also shown in the graph of FIG. **15J**, the model illustrates that resistance values of 40 M Ω for resistors **1518** may serve as an alternative to the 4 photodiode per stream architecture of sensor **1502** described above and yet still provide an equivalent SNR.

Moreover, the discovered noise model also indicates that utilizing a 1 photodiode per stream architecture like that in sensor **1512** may provide enhanced performance because each of transimpedance amplifiers **1516** can be tuned or optimized to its respective photodiodes **1518**. In some embodiments, an averaging component **1520** may also be used to help cancel or reduce noise across photodiodes **1518**.

For purposes of illustration, FIG. **15K** shows different architectures (e.g., four PD per stream and one PD per stream) for various embodiments of a sensor and how components of the sensor may be laid out on a circuit board or substrate. For example, sensor **1522** may comprise a "4 PD per stream" architecture on a submount **700** in which each detector **106** comprises four (4) photodiodes **1524**. As shown for sensor **1522**, the output of each set of four photodiodes **1524** is then aggregated into a single transimpedance amplifier **1526** to produce a signal.

As another example, a sensor **1528** may comprise a "1 PD per stream" architecture on submount **700** in which each detector **106** comprises four (4) photodiodes **1530**. In sensor **1528**, each individual photodiode **1530** is coupled to a respective transimpedance amplifier **1532**. The output of the amplifiers **1532** may then be aggregated into averaging circuit **1520** to produce a signal.

As noted previously, one skilled in the art will recognize that the photodiodes and detectors may be arranged in differ-

ent fashions to optimize the detected light. For example, sensor **1534** illustrates an exemplary “4 PD per stream” sensor in which the detectors **106** comprise photodiodes **1536** arranged in a linear fashion. Likewise, sensor **1538** illustrates an exemplary “1 PD per stream” sensor in which the detectors

comprise photodiodes **1540** arranged in a linear fashion. Alternatively, sensor **1542** illustrates an exemplary “4 PD per stream” sensor in which the detectors **106** comprise photodiodes **1544** arranged in a two-dimensional pattern, such as a zig-zag pattern. Sensor **1546** illustrates an exemplary “1 PD per stream” sensor in which the detectors comprise photodiodes **1548** also arranged in a zig-zag pattern.

FIG. **15L** illustrates an exemplary architecture for a switched-capacitor-based front-end. As shown, front-end interfaces **108** may be implemented using switched capacitor circuits and any number of front-end interfaces **108** may be implemented. The output of these switched capacitor circuits may then be provided to a digital interface **1000** and signal processor **110**. Switched capacitor circuits may be useful in system **100** for their resistor free design and analog averaging properties. In particular, the switched capacitor circuitry provides for analog averaging of the signal that allows for a lower smaller sampling rate (e.g., 2 KHz sampling for analog versus 48 KHz sampling for digital designs) than similar digital designs. In some embodiments, the switched capacitor architecture in front end interfaces **108** may provide a similar or equivalent SNR to other front end designs, such as a sigma delta architecture. In addition, a switched capacitor design in front end interfaces **108** may require less computational power by signal processor **110** to perform the same amount of decimation to obtain the same SNR.

FIGS. **16A** and **16B** illustrate embodiments of disposable optical sensors **1600**. In an embodiment, any of the features described above, such as protrusion, shielding, and/or heat sink features, can be incorporated into the disposable sensors **1600** shown. For instance, the sensors **1600** can be used as the sensors **101** in the system **100** described above with respect to FIG. **1**. Moreover, any of the features described above, such as protrusion, shielding, and/or heat sink features, can be implemented in other disposable sensor designs that are not depicted herein.

The sensors **1600** include an adult/pediatric sensor **1610** for finger placement and a disposable infant/neonate sensor **1602** configured for toe, foot or hand placement. Each sensor **1600** has a tape end **1610** and an opposite connector end **1620** electrically and mechanically interconnected via a flexible coupling **1630**. The tape end **1610** attaches an emitter and detector to a tissue site. Although not shown, the tape end **1610** can also include any of the protrusion, shielding, and/or heat sink features described above. The emitter illuminates the tissue site and the detector generates a sensor signal responsive to the light after tissue absorption, such as absorption by pulsatile arterial blood flow within the tissue site.

The sensor signal is communicated via the flexible coupling **1630** to the connector end **1620**. The connector end **1620** can mate with a cable (not shown) that communicates the sensor signal to a monitor (not shown), such as any of the cables or monitors shown above with respect to FIGS. **2A** through **2D**. Alternatively, the connector end **1620** can mate directly with the monitor.

FIG. **17** illustrates an exploded view of certain of the components of the sensor **301**/described above. A heat sink **1751** and a cable **1781** attach to an emitter shell **1704**. The emitter shell attaches to a flap housing **1707**. The flap housing **1707** includes a receptacle **1709** to receive a cylindrical housing **1480/1580** (not shown) attached to an emitter submount **1702**, which is attached to a circuit board **1719**.

A spring **1787** attaches to a detector shell **1706** via pins **1783**, **1785**, which hold the emitter and detector shells **1704**, **1706** together. A support structure **1791** attaches to the detector shell **1706**, which provides support for a shielding enclosure **1790**. A noise shield **1713** attaches to the shielding enclosure **1790**. A detector submount **1700** is disposed inside the shielding enclosure **1790**. A finger bed **1710** provides a surface for placement of the patient’s finger. Finger bed **1710** may comprise a gripping surface or gripping features, which may assist in placing and stabilizing a patient’s finger in the sensor. A partially cylindrical protrusion **1705** may also be disposed in the finger bed **1710**. As shown, finger bed **1710** attaches to the noise shield **1703**. The noise shield **1703** may be configured to reduce noise, such as from ambient light and electromagnetic noise. For example, the noise shield **1703** may be constructed from materials having an opaque color, such as black or a dark blue, to prevent light piping.

Noise shield **1703** may also comprise a thermistor **1712**. The thermistor **1712** may be helpful in measuring the temperature of a patient’s finger. For example, the thermistor **1712** may be useful in detecting when the patient’s finger is reaching an unsafe temperature that is too hot or too cold. In addition, the temperature of the patient’s finger may be useful in indicating to the sensor the presence of low perfusion as the temperature drops. In addition, the thermistor **1712** may be useful in detecting a shift in the characteristics of the water spectrum in the patient’s finger, which can be temperature dependent.

Moreover, a flex circuit cover **1706** attaches to the pins **1783**, **1785**. Although not shown, a flex circuit can also be provided that connects the circuit board **1719** with the submount **1700** (or a circuit board to which the submount **1700** is connected). A flex circuit protector **1760** may be provided to provide a barrier or shield to the flex circuit (not shown). In particular, the flex circuit protector **1760** may also prevent any electrostatic discharge to or from the flex circuit. The flex circuit protector **1760** may be constructed from well known materials, such as a plastic or rubber materials.

FIG. **18** shows the results obtained by an exemplary sensor **101** of the present disclosure that was configured for measuring glucose. This sensor **101** was tested using a pure water ex-vivo sample. In particular, ten samples were prepared that ranged from 0-55 mg/dL. Two samples were used as a training set and eight samples were then used as a test population. As shown, embodiments of the sensor **101** were able to obtain at least a standard deviation of 13 mg/dL in the training set and 11 mg/dL in the test population.

FIG. **19** shows the results obtained by an exemplary sensor **101** of the present disclosure that was configured for measuring glucose. This sensor **101** was tested using a turbid ex-vivo sample. In particular, 25 samples of water/glucose/Lyposin were prepared that ranged from 0-55 mg/dL. Five samples were used as a training set and 20 samples were then used as a test population. As shown, embodiments of sensor **101** were able to obtain at least a standard deviation of 37 mg/dL in the training set and 32 mg/dL in the test population.

FIGS. **20** through **22** shows other results that can be obtained by an embodiment of system **100**. In FIG. **20**, 150 blood samples from two diabetic adult volunteers were collected over a 10-day period. Invasive measurements were taken with a YSI glucometer to serve as a reference measurement. Noninvasive measurements were then taken with an embodiment of system **100** that comprised four LEDs and four independent detector streams. As shown, the system **100** obtained a correlation of about 85% and Arms of about 31 mg/dL.

In FIG. 21, 34 blood samples were taken from a diabetic adult volunteer collected over a 2-day period. Invasive measurements were also taken with a glucometer for comparison. Noninvasive measurements were then taken with an embodiment of system 100 that comprised four LEDs in emitter 104 and four independent detector streams from detectors 106. As shown, the system 100 was able to attain a correlation of about 90% and Arms of about 22 mg/dL.

The results shown in FIG. 22 relate to total hemoglobin testing with an exemplary sensor 101 of the present disclosure. In particular, 47 blood samples were collected from nine adult volunteers. Invasive measurements were then taken with a CO-oximeter for comparison. Noninvasive measurements were taken with an embodiment of system 100 that comprised four LEDs in emitter 104 and four independent detector channels from detectors 106. Measurements were averaged over 1 minute. As shown, the testing resulted in a correlation of about 93% and Arms of about 0.8 mg/dL.

Conditional language used herein, such as, among others, “can,” “could,” “might,” “may,” “e.g.,” and the like, unless specifically stated otherwise, or otherwise understood within the context as used, is generally intended to convey that certain embodiments include, while other embodiments do not include, certain features, elements and/or states. Thus, such conditional language is not generally intended to imply that features, elements and/or states are in any way required for one or more embodiments or that one or more embodiments necessarily include logic for deciding, with or without author input or prompting, whether these features, elements and/or states are included or are to be performed in any particular embodiment.

While certain embodiments of the inventions disclosed herein have been described, these embodiments have been presented by way of example only, and are not intended to limit the scope of the inventions disclosed herein. Indeed, the novel methods and systems described herein can be embodied in a variety of other forms; furthermore, various omissions, substitutions and changes in the form of the methods and systems described herein can be made without departing from the spirit of the inventions disclosed herein. The claims and their equivalents are intended to cover such forms or modifications as would fall within the scope and spirit of certain of the inventions disclosed herein.

What is claimed is:

1. A multi-stream emitter for a noninvasive, physiological device configured to transmit optical radiation in a tissue site, said emitter comprising:

a set of optical sources comprising:

a top-emitting diode affixed to a first surface, and

a side-emitting diode affixed to a second surface, wherein the first surface is approximately perpendicular to the second surface; and

a driver configured to:

drive the top-emitting diode to transmit first infrared optical radiation at a first power into a tissue site of a patient, wherein the top-emitting diode is configured to emit the first infrared optical radiation in a first direction substantially perpendicular to the first surface; and

drive the side-emitting diode to transmit second infrared optical radiation at a second power into the tissue site of the patient, wherein the side-emitting diode is configured to emit the second infrared optical radiation in a second direction substantially parallel to the second surface, and wherein the second power is greater than the first power; enabling measurement of an analyte in the tissue site of the patient.

2. The emitter of claim 1, wherein the side-emitting diode comprises a super luminescent light emitting diode.

3. The emitter of claim 1, wherein the side-emitting diode comprises a laser diode.

4. The emitter of claim 1 further comprising a submount that configures the set of optical sources as a single point source.

5. The emitter of claim 4 wherein the submount is configured to position the set of optical sources within a diameter of about 2 mm of each other.

6. The emitter of claim 4 wherein the submount is configured to position the set of optical sources within a diameter of about 4 mm of each other.

7. The emitter of claim 1, wherein the top-emitting diode is configured to emit the first infrared optical radiation at a wavelength of approximately 900 to approximately 1350 nm.

8. The emitter of claim 1, wherein the side-emitting diode is configured to emit the second infrared optical radiation at wavelengths of approximately 1600 to approximately 1800 nm.

9. The emitter of claim 1, further comprising a heat sink thermodynamically coupled to the set of optical sources.

10. The emitter of claim 1, further comprising at least one thermistor.

11. The emitter of claim 10, wherein the at least one thermistor is configured to detect a temperature of at least one of the optical sources.

12. The emitter of claim 10, wherein the at least one thermistor is configured to detect a temperature of the tissue site.

13. The emitter of claim 1, wherein the set of optical sources comprises a plurality of side-emitting diodes.

14. The emitter of claim 1, wherein the set of optical sources comprises a plurality of top-emitting diodes.

15. An emitter of a noninvasive optical sensor, the emitter configured to transmit optical radiation into a tissue site to be detected after attenuation by said tissue site and processed to determine one or more physiological parameters of a patient, said emitter comprising:

an optical source; including:

a top-emitting diode having a first surface connected to an electrical contact, and

a side-emitting diode having a second surface connected to an electrical contact; and

a driver:

configured to drive the top-emitting diode to transmit light at a first wavelength into the tissue site, wherein the top-emitting diode is configured to transmit light at the first wavelength in a first direction substantially perpendicular to the first surface; and

configured to drive the side-emitting diode to transmit light at a second wavelength into the tissue site, wherein the side-emitting diode is configured to transmit light at the second wavelength in a second direction substantially parallel to the second surface.

16. The emitter of claim 15, wherein the second wavelength is between approximately 1650 nm and approximately 1800 nm.

17. The emitter of claim 15, wherein the driver is configured to deliver a progression of about 1 mW for emitting the light at the first wavelength and about 40 to about 100 mW for emitting the light at the second wavelength.

18. The emitter of claim 15, wherein the driver is configured to:

drive the top-emitting diode at a first power; and

drive the side-emitting diode at a second power, wherein the second power is greater than the first power.

19. The emitter of claim 15, wherein the top-emitting diode and the side-emitting diode are placed on orthogonal planes.

20. The emitter of claim 15, wherein the top-emitting diode and the side-emitting diode do not face the same plane.

21. A method of transmitting a stream of pulses of optical radiation in a tissue site, said method comprising:

transmitting with a top-emitting diode affixed to a first surface, at a first power, at least one pulse of first infrared optical radiation having a first pulse width, wherein the top-emitting diode is configured to transmit light at the first infrared optical radiation in a first direction substantially perpendicular to the first surface; and

transmitting with a side-emitting diode affixed to a second surface not parallel to the first surface, at a second power, at least one pulse of second infrared optical radiation, wherein the side-emitting diode is configured to transmit light at the second infrared optical radiation in a second direction substantially parallel to the second surface.

22. The method of claim 21, further comprising waiting for an idle period before transmitting at the second power.

23. The method of claim 21, further comprising waiting for a stabilization period between transmitting at the second power and repeating transmission at the first power.

24. The method of claim 21, further comprising adjusting the pulse widths of the at least one pulse of the first or the second infrared optical radiation.

25. The method of claim 21, further comprising: monitoring a temperature of sources of the first or the second infrared optical radiation; and

adjusting transmission of the at least one pulse of the first or the second infrared optical radiation based on the temperature.

26. The method of claim 21, further comprising: monitoring a temperature of the tissue site; and adjusting transmission of the at least one pulse of the first or the second infrared optical radiation based on the temperature.

27. The method of claim 21, further comprising synchronizing transmission of the pulses of the first and the second infrared optical radiation with a sampling frequency at a detector detecting optical radiation from the tissue site.

28. The method of claim 21, wherein the stream of optical pulses are transmitted by optical sources that are within about a 2 mm diameter of each other.

29. The method of claim 21, wherein the stream of optical pulses are transmitted by the top-emitting diode and the side-emitting diode that are within about a 4 mm diameter of each other.

30. The method of claim 21, transmitting the at least one pulse of the first infrared optical radiation comprises transmitting at a wavelength of approximately 900 to approximately 1350 nm.

31. The method of claim 21, transmitting the at least one pulse of the second infrared optical radiation comprises transmitting at a wavelength of approximately 1650 to approximately 1800 nm.

32. A light source for a noninvasive, physiological device configured to transmit optical radiation in a tissue site, said light source comprising:

a set of optical sources, the set of optical sources comprising:

a first emitting diode affixed to a first surface, and a side emitting diode affixed to a second surface, said second surface being in a non-parallel plane to said first surface; and

a driver configured to:

drive the first emitting diode to transmit first optical radiation into a tissue site of a patient, wherein the first emitting diode is configured to emit the first optical radiation in a first direction, and

drive the second emitting diode to transmit second optical radiation into the tissue site of the patient, wherein the second emitting diode is configured to emit the second optical radiation in the first direction;

wherein the first direction is generally toward the tissue site of the patient, wherein the first optical radiation is emitted at a first intensity and the second optical radiation is emitted at a second intensity, the second intensity be substantially greater than the first intensity.

33. The light source of claim 32, wherein the second emitting diode is configured to transmit optical radiation at wavelengths of approximately 1650 to approximately 1800 nm.

34. The light source of claim 32, wherein the driver is configured to deliver a progression of about 1 mW for emitting the first optical radiation and about 40 to about 100 mW for emitting the second optical radiation.

35. The light source of claim 32, wherein the first surface is approximately perpendicular to the second surface.

36. The light source of claim 32, wherein the first emitting diode comprises one or more top-emitting diodes and the second emitting diode comprises one or more side-emitting diodes.

* * * * *

专利名称(译)	多流发射器，用于无创测量血液成分		
公开(公告)号	US8515509	公开(公告)日	2013-08-20
申请号	US12/534825	申请日	2009-08-03
[标]申请(专利权)人(译)	MASIMO LAB		
申请(专利权)人(译)	MASIMO实验室，INC.		
当前申请(专利权)人(译)	CERCACOR LABORATORIES，INC.		
[标]发明人	BRUINSMA JOHANNES LAMEGO MARCELO MERRITT SEAN DALVI CRISTIANO VO HUNG POEZE JEROEN LESMANA FERDYAN KIANI MASSI JOE E		
发明人	BRUINSMA, JOHANNES LAMEGO, MARCELO MERRITT, SEAN DALVI, CRISTIANO VO, HUNG POEZE, JEROEN LESMANA, FERDYAN KIANI, MASSI JOE E.		
IPC分类号	A61B5/00		
CPC分类号	A61B5/14532 A61B5/14546 A61B5/1455 A61B5/14552 A61B5/6816 A61B5/6829 A61B5/6838 A61B5/6843 A61B5/6826 A61B2562/146 A61B2562/0233 A61B2562/046 A61B2562/04		
助理审查员(译)	汉考克，DENNIS		
优先权	61/086060 2008-08-04 US 61/086108 2008-08-04 US 61/086063 2008-08-04 US 61/086057 2008-08-04 US 61/091732 2008-08-25 US		
其他公开文献	US20100030041A1		
外部链接	Espacenet USPTO		

摘要(译)

本发明涉及一种适用于非侵入性血液成分传感器的发射器。发射器被配置为点光源，其包括多个LED，这些LED发射跨越波长谱的光辐射脉冲序列。在一些实施例中，多组光源可各自包括至少一个顶部发光LED和至少一个超级发光LED。在一些实施例中，发射器包括传输适合于检测葡萄糖的红外或近红外波长的光辐射的光源。为了实现用于检测诸如葡萄糖的分析物的期望SNR，可以使用从低功率到更高功率的进展来驱动发射器。另外，发射器可以修改其占空比以实现期望的SNR。

