



US006934573B1

(12) **United States Patent**
Glukhovsky et al.

(10) **Patent No.:** **US 6,934,573 B1**
(45) **Date of Patent:** **Aug. 23, 2005**

(54) **SYSTEM AND METHOD FOR CHANGING TRANSMISSION FROM AN IN VIVO SENSING DEVICE**

6,438,405 B1 * 8/2002 Mooney et al. 600/427
6,546,276 B1 * 4/2003 Zanelli 600/424
6,587,711 B1 * 7/2003 Alfano et al. 600/476

(75) Inventors: **Arkady Glukhovsky**, Santa Clarita, CA (US); **Baruch Erlich**, Qiryat Tivon (IL)

FOREIGN PATENT DOCUMENTS

DE 34 40 177 5/1986
JP 4109927 4/1992
JP 5015515 1/1993
WO WO 01/08548 2/2001
WO WO 01/50941 7/2001
WO WO 01/65995 9/2001

(73) Assignee: **Given Imaging Ltd.**, Yoqneam (IL)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 104 days.

OTHER PUBLICATIONS

(21) Appl. No.: **10/200,548**

The Radio Pill, Rowlands, et al., British Communications and Electronics, Aug. 1960, pp. 598-601.

(22) Filed: **Jul. 23, 2002**

Wellesley company sends body monitors into space, Crum, Apr. 1998.

Related U.S. Application Data

Wireless transmission of a color television moving image from the stomach using a miniature CCD camera, light source and microwave transmitter. Swain CP, Gong F, Mills TN. Gastrointest Endosc 1997;45:AB40.

(60) Provisional application No. 60/306,872, filed on Jul. 23, 2001.

(51) **Int. Cl.**⁷ **A61B 5/05**; A61B 17/00

(Continued)

(52) **U.S. Cl.** **600/407**; 606/1

Primary Examiner—Daniel Robinson

(58) **Field of Search** 600/407, 410, 600/437, 372; 607/1, 2; 250/363.01, 363.02, 250/363.03, 363.04; 606/1, 2

(74) *Attorney, Agent, or Firm*—Pearl Cohen Zedek Latzer, LLP

(56) **References Cited**


(57) **ABSTRACT**

U.S. PATENT DOCUMENTS

3,971,362 A 7/1976 Pope et al.
4,278,077 A 7/1981 Mizumoto
4,689,621 A 8/1987 Kleinberg
4,844,076 A 7/1989 Lesho et al.
5,279,607 A 1/1994 Schentag et al.
5,477,858 A * 12/1995 Norris et al. 600/441
5,604,531 A * 2/1997 Iddan et al. 348/76
5,819,736 A 10/1998 Avny et al.
5,928,159 A * 7/1999 Eggers et al. 600/547
6,240,312 B1 5/2001 Alfano et al.

A device, system and method enables obtaining data such as in vivo images from within body lumens or cavities, such as images of the gastrointestinal (GI) tract. A device may include an imaging system and a radio frequency (RF) transmitter for transmitting signals from an imaging device to a receiving system. The signal strength of the transmitter may be varied or changed to account for, for example, the amount of signal attenuation resulting from body tissues.

31 Claims, 2 Drawing Sheets

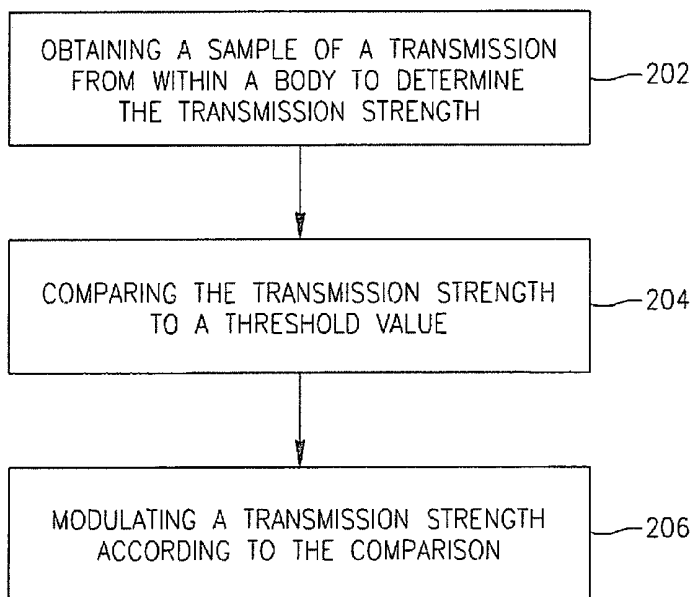

OTHER PUBLICATIONS

BBC News Online—Pill camera to ‘broadcast from the gut’,
Feb. 21, 2000, www.news.bbc.co.uk.

Biomedical Telemetry, R Stewart McKay, John Wiley and
Sons, 1970, p244-245.

* cited by examiner

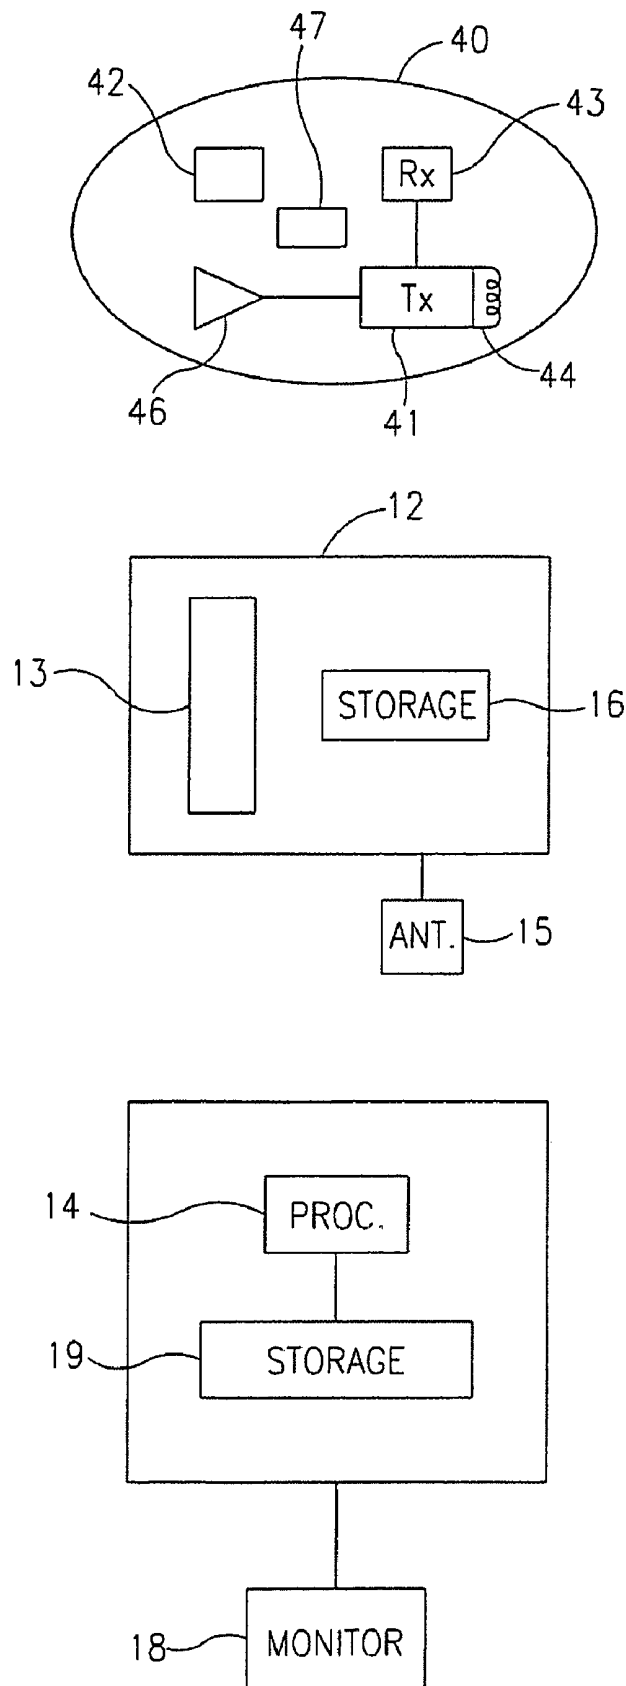


FIG. 1

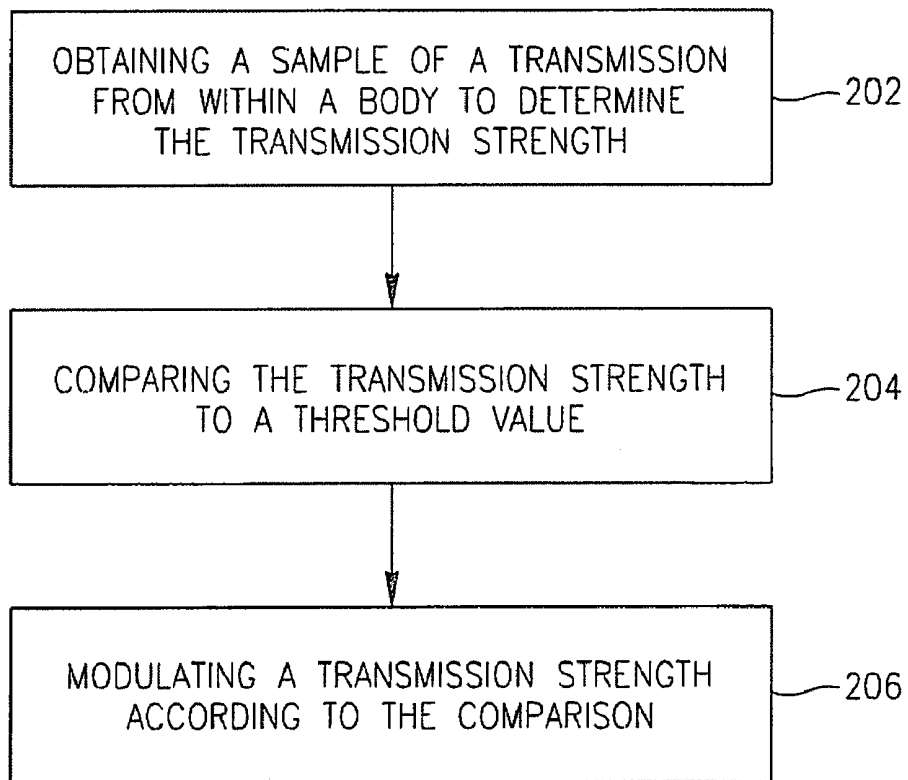


FIG. 2

SYSTEM AND METHOD FOR CHANGING TRANSMISSION FROM AN IN VIVO SENSING DEVICE

PRIOR PROVISIONAL APPLICATION

The present application claims benefit from prior U.S. provisional application No. 60/306,872 entitled "VARIABLE SIGNAL STRENGTH IMAGING DEVICE" and filed on Jul. 23, 2001.

FIELD OF THE INVENTION

The present invention relates to an in vivo sensing device, system and method such as for imaging the digestive tract; more specifically, to an in vivo sensing device utilizing a device, system and method whereby the transmission signal strength may be varied.

BACKGROUND OF THE INVENTION

Devices and methods for sensing of passages or cavities within a body, and for gathering information (e.g., image data, pH data, temperature information, pressure information), are known in the art. Such devices may include, inter alia, various endoscopic imaging systems and devices for performing imaging in various internal body cavities. Some devices transmit the collected data to an external receiving unit.

An in-vivo imaging device may include, for example, an imaging system for obtaining images from inside a body cavity or lumen, such as the gastrointestinal (GI) tract. The imaging system may include, for example, an illumination unit, such as a set of light emitting diodes (LEDs), or other suitable light sources. The device may include an imaging sensor and an optical system, which focuses the images onto the imaging sensor. A transmitter and antenna may be included for transmitting the images signals. A receiver/recorder, for example worn by the patient, may record transmitted image data and store image and other data. The recorded data may then be downloaded from the receiver/recorder to a computer or workstation for display and analysis.

A signal transmitted from an in vivo sensor may be attenuated while passing through the body tissues, due to the fact that tissues have electrical conductance. Continuous high-level transmission, which might overcome the attenuation, may require a continuous supply of high energy, may be inefficient and may be in conflict with regulatory considerations.

Therefore, there is a need for an in-vivo sensing device, such as an imaging device, which may transmit data at efficient power levels.

SUMMARY OF THE INVENTION

An embodiment of the device, system and method of the present invention enables obtaining in vivo images from within body lumens or cavities, such as images of the gastrointestinal (GI) tract. One embodiment of the invention provides a device including an imaging system and a radio frequency (RF) transmitter for transmitting signals from an imaging device to a receiving system. In one embodiment of such an imaging system, the signal strength of the transmitter may be varied or changed to account for, for example, the amount of signal attenuation resulting from body tissues.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a schematic diagram of an in vivo imaging system according to one embodiment of the present invention; and

FIG. 2 shows a block diagram of a method for changing data transmitted from an in vivo sensing device, according to an embodiment of the invention.

DETAILED DESCRIPTION OF THE INVENTION

In the following description, various aspects of the present invention will be described. For purposes of explanation, specific configurations and details are set forth in order to provide a thorough understanding of the present invention. However, it will also be apparent to one skilled in the art that the present invention may be practiced without the specific details presented herein. Furthermore, well known features may be omitted or simplified in order not to obscure the present invention.

The device, system and method of the present invention may be used with an imaging system or device such as that described in WO 01/65995 entitled "A Device And System For In Vivo Imaging", published on 13 Sep. 2001, which is hereby incorporated by reference. However, the device, system and method according to the present invention may be used with any device providing data from a body lumen or cavity. For example, the device, system and method of the present invention may be used with imaging devices using cameras other than CMOS imaging cameras. In alternate embodiments, a known imaging camera of another type such as a CCD may be used. A further example of an imaging system and device with which the system and method of the present invention may be used is described in U.S. Pat. No. 5,604,531 entitled "In Vivo Video Camera System," which is incorporated herein by reference. In further embodiments, the system and method of the present invention may be used with devices and systems capturing information other than image information within the human body; for example, pressure or pH information, information on the location of a transmitting device, or other information.

Reference is made to FIG. 1, which shows a schematic diagram of an in vivo sensor according to one embodiment of the present invention. In an exemplary embodiment, the system includes a device **40** having an image sensor **46**, for capturing images, an optical system (not shown), an illumination source **42** (which may be, for example, one or more LEDs, although any suitable illumination source), for illuminating the body lumen, and a transmitter **41** and antenna **44**, for transmitting image and possibly other information to a receiving device. Typically, the device **40** is an ingestible capsule capturing images, but may be another sort of device and may collect information other than image information. An optical system (not shown), including, for example, lenses or mirrors, may aid in focusing reflected light onto the image sensor **46**. The device **40** typically includes a power source **47** which may be, for example, one or more batteries or other power sources.

The device **40** may be swallowed or otherwise ingested by a patient and typically traverses the patient's GI tract. In one embodiment, transmitter **41** provides control and possibly other processing capability for the device **40**. Thus, transmitter **41** may include or be associated with circuitry such as an ASIC, a microcontroller, or a "computer on a chip." In alternate embodiments, a separate control and/or processing unit may be provided.

In one embodiment, the imager **46** is a complementary metal oxide semiconductor (CMOS) imaging camera. The CMOS imager is typically an ultra low power imager, has a low sensitivity to the red spectrum, and is provided in chip scale packaging (CSP). One suitable CMOS camera is, for example, a “camera on a chip” CMOS imager specified by Given Imaging Ltd. of Israel and designed by Photobit Corp. of California, USA, with integrated active pixel and post processing circuitry. Other types of CMOS imagers may be used. In another embodiment, another imager may be used, such as a CCD imager, or another imager.

In one embodiment, transmitter **41** includes at least a modulator for receiving an image signal from the imager **46**, a radio frequency (RF) amplifier, an impedance matcher and an antenna. The modulator converts the input image signal having a cutoff frequency f_c of less than 5 MHz to an RF signal having a carrier frequency f_r , typically in the range of 1 GHz. While in one embodiment, the signal is an analog signal, the modulating signal may be digital rather than analog. The carrier frequency may be in other bands, e.g. a 400 MHz band. The modulated RF signal has a bandwidth of ft. The impedance matcher matches the impedance of the circuit to that of the antenna. Other transmitters or arrangements of transmitter components may be used. For example, alternate embodiments may not include a matched antenna or may include a transmitter without a matching circuit. In alternate embodiments, the device **40** may have different configurations and include other sets of components. Other frequencies may be used. In yet further embodiments sensors other than image sensors may be used, such as pH meters, temperature sensors, pressure sensors, etc. and input RF signals other than image signals may be used.

According to one embodiment, while the device **40** traverses a patient’s GI tract, the device **40** transmits image and possibly other data to components located outside the patient’s body, which receive and process the data. Typically, located outside the patient’s body in one or more locations, are an image receiver **12**, typically including an antenna **15** or antenna array, an image receiver storage unit **16**, a data processor **14**, a data processor storage unit **19**, and an image monitor **18**, for displaying, inter alia, the images transmitted by the device **40** and recorded by the image receiver **12**. According to one embodiment, the image receiver **12** and image receiver storage unit **16** are small and portable, and are worn on the patient’s body during recording of the images. Typically, data processor **14**, data processor storage unit **19** and monitor **18** are part of a personal computer or workstation, which includes standard components such as processor **14**, a memory, a disk drive, and input-output devices, although alternate configurations are possible.

In alternate embodiments, the data reception and storage components may be of another configuration. Further, image and other data may be received in other manners, by other sets of components. Typically, in operation, image data is transferred to the data processor **14**, which, in conjunction with, for example, a central processing unit and software, stores, possibly processes, and displays the image data on monitor **18**. Other systems and methods of storing and/or displaying collected image data may be used.

Typically, the device **40** transmits image information in discrete portions. Each portion typically corresponds to an image or frame. Other transmission methods are possible. For example, the device **40** may capture an image once every half second, and, after capturing such an image, transmit the image. Other capture rates are possible. Typically, the image data recorded and transmitted is digital color

image data, although in alternate embodiments other image formats (e.g., black and white image data) may be used. In one embodiment, each frame of image data includes 256 rows of 256 pixels each, each pixel including data for color and brightness, according to known methods. For example, in each pixel, color may be represented by a mosaic of four sub-pixels, each sub-pixel corresponding to primaries such as red, green, or blue (where one primary is represented twice). The brightness of the overall pixel may be recorded by, for example, a one byte (i.e., 0–255) brightness value. Other data formats may be used.

The receiver **12** typically detects a signal having the carrier frequency f_r and the bandwidth f_c described hereinabove. The receiver **12** may be similar to those found in televisions or it may be one similar to those described on pages 244–245 of the book Biomedical Telemetry by R. Stewart McKay and published by John Wiley and Sons, 1970. The receiver may be digital or analog. In alternate embodiments, other receivers may be used.

The location of the imaging device **40** inside the body and its orientation relative to the antenna(s) **15** change as the device **40** traverses the GI tract. At times the device **40** may be located close to the body surface, and at other times it may be located deeper inside the body. The signal transmitted from the device **40** may be attenuated while passing through the body tissues, due to the fact that tissues have electrical conductance. The level of attenuation may be affected by, inter alia, the amount and types of body tissue that the signal passes through, and on the transmission frequency. Attenuation typically increases logarithmically with the frequency. In one embodiment of such an imaging device **40**, transmission occurs at a frequency of 434 MHz, using Phase Shift Keying (PSK); the body tissue attenuation at this frequency is approximately 2.5–3 dB/cm. In alternate embodiments, other transmission frequencies and other methods (such as AM or FM) may be used.

One method for maintaining a reliable communication channel for practically all possible (or likely) locations of the device **40** inside the body is to set the transmission power of the transmitter **41** in the device **40** to some maximum amount such that proper transmission between the device **40** and the antenna **15** or antenna array is achieved for all locations. For example, assuming that the maximal depth in the body, of which the device **40** is to traverse (e.g., the GI tract) is 25 cm, the transmitter **41** transmission output should be higher than the minimum power level required by the receiver **12** by, for example, 3 dB/cm * 25 cm = 75 dB; the total power level required is the minimum required level of the receiver **12** plus 75 dB. The minimum required level is a typically empirical value which depends, inter alia, on the sensitivity of the receiver **12**, on the modulation technique being used as well as on the specific design of the receiver **12**. In such an “open loop” embodiment, high-level transmission levels occur continually, even when lower power transmission may be satisfactory. High power transmission requires the transmitter **41** to consume high levels of power; if the system operates on batteries, the batteries are emptied faster. Further, government regulatory considerations may limit transmission levels.

In one embodiment of the device, system and method of the present invention, a “closed loop” is used, with feedback from the receiver **12** or another module altering the power transmission level of the transmitter **41** in the device **40** in order to ensure that the power level is high enough, but not higher than necessary, or not significantly higher than necessary, to allow for acceptable transmission quality. Typically, the receiver **12** measures the power level of the

5

received signal from the imaging or other device **40**. Various known methods of measuring the strength of the received signal may be used. In one embodiment, at the start of the transmission of an image frame or other unit of transmission, a blank or dummy section is sent. During the transmission of this section, the receiver **12** samples signals from each of typically multiple antennas in the antenna array **15**, and determines which antenna is receiving and is the source of the strongest signal. This antenna is used to receive the image frame, and the strength of this signal determines the signal strength. In alternate embodiments, only one antenna may be used, and this antenna is then used to determine signal strength. Embodiments of the present invention may be used with devices or systems not transmitting "frames" of data, and may be used with systems transmitting data continuously.

In one embodiment, to regulate the signal strength of the transmitter **41**, if the receiver **12** determines that the signal strength is below a lower threshold which will result in clear transmission, it determines that the signal strength of the transmitter **41** should be increased, and if the image receiver **12** determines that the signal strength is above an upper threshold, it determines that the signal strength of the transmitter **41** should be decreased. In alternate embodiments, other methods of controlling the signal strength may be used. For example, after each frame is received, the received signal strength may be evaluated and the signal strength of the transmitter **41** may be adjusted. A blank frame need not be used.

A power level transmitter **13** within the receiver **12**, typically a simple transmitter (e.g., a transmitter transmitting a relatively small amount of information using simple modulation or Frequency Shift Keying (FSK), using a relatively low frequency signal), transmits a signal to the device **40** regarding the power level of the received signal. In the imaging or other device **40** a typically simple power level receiver **43** (e.g., a simple RF receiver, such as a receiver in the alarm of a car) may be used to receive and decode power level information, and the output power of the transmitter within the device **40** is changed accordingly.

Typically, the power level transmitter **13** may transmit a command from a pre-determined set of commands. The receiver **43** may receive and decode the command, and transfer it to the transmitter **41**, in order to set the output power level. In alternate embodiments, other power level information may be used; for example, a signal to raise or lower the power level by a certain amount, or a signal indicating the power level or signal quality. In further embodiments, processing capability may be included in the device **40** for adjusting the power level based on such signals. According to one embodiment a processing unit may be included in the device **40** for processing the power level data received from the power level transmitter **13** and for commanding the transmitter **41** to adjust the transmission level. In one embodiment, transmitter **41** may provide processing unit capabilities, thus transmitter **41** may adjust its own power levels. According to alternate embodiments a processing unit may be included in the receiver **12** for processing the signal received from transmitter **41** and for regulating the signal transmitted from power level transmitter **13**. The transmitter **41** may include circuitry, which may enable it to change the level of the output signal, i.e. the level of the signal that is transmitted through the antenna. The level of the transmitted signal may be determined by dif-

6

ferent methods, e.g. it may be set constant, or may be changed after receiving a command by the power level receiver **43**.

In alternate embodiments, the power level transmitter **13** and power level receiver **43** need not be simple devices. In further embodiments, a device other than the receiver **12**, which may include a power level receiver, may provide feedback to the device **40**.

In yet further embodiments the power level transmitter **13** may be used to transmit a constant, typically, periodical and known signal to be received by the power level receiver **43**. The signal is typically attenuated (e.g., by the passage through the body tissues) such that the received signal contains information regarding the attenuation. As such, the received signal may provide indication of the transmission strength required from transmitter **41**. According to embodiments of the invention the device **40** may include a processor, typically, for computing the transmission strength of a transmitted signal based on a received signal, for example, a signal received from the power level transmitter **13**.

According to one embodiment two image frames are transmitted from the device **40** every second, and with the transmission of each frame, the signal strength is measured by the receiver **12** and a power level feedback signal is provided to the device **40**. In alternate embodiments, other rates of imaging and other rates of feedback may be used. For example, feedback may be provided once every several frames or periodically, per a fixed time period.

Reference is now made to FIG. 2, which shows a block diagram of a method for changing data transmission from an in vivo sensing device. According to one embodiment the method includes the steps of obtaining a transmission from within a body and in response to the transmission, changing a transmission strength. According to an embodiment of the invention, the method includes the steps of obtaining a sample of a transmission from within a body (**202**) to determine the transmission strength; comparing the transmission strength to a threshold value (**204**); and changing (for example, decreasing or increasing) a transmission strength according to the comparison (**206**). According to one embodiment one transmission event is sampled, for example, by measuring the transmission strength of a blank or dummy portion of the transmission, and the same transmission event is changed. According to another embodiment one transmission event is sampled and another transmission event is changed, for example, transmission n is sampled and the transmission strength of n is determined and compared to a threshold. Transmission n+1 is then changed according to the comparison. Other sampling methods or frequencies may be used.

According to an embodiment of the invention a method for controlling image data transmission from an in vivo capsule is provided. The method according to an embodiment may include receiving a transmission having a signal strength; evaluating the signal strength; and altering a capsule transmission power level.

Accordingly, lower average power consumption in the device **40** may be achieved, prolonging battery life (if a battery is used). Furthermore, in situations where the estimated maximum power level is not enough to achieve reliable communication, the power level can be increased by the closed loop system, allowing for more reliable communication.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly

shown and described hereinabove. Alternate embodiments are contemplated which fall within the scope of the invention.

What is claimed is:

1. A system for obtaining in vivo data, the system comprising:
 - a swallowable capsule; and
 - a receiving unit;
 - said swallowable capsule comprising at least one in vivo sensor, at least one signal transmitter and at least one power level receiver to receive a command to adjust the power level of said at least one signal transmitter; and said receiving unit comprising at least one receiver and at least one power level transmitter.
2. The system according to claim 1 wherein the power level transmitter is configured to transmit data regarding the power level of a signal transmitted from the signal transmitter and wherein the power level receiver is configured to receive a signal from the power level transmitter.
3. The system according to claim 1 wherein the swallowable capsule further comprises a processing unit.
4. The system according to claim 3 wherein the processing unit is configured to process power level data received from the power level transmitter.
5. The system according to claim 3 wherein the processing unit is configured to command the signal transmitter to change a transmission power level.
6. The system according to claim 1 wherein the signal transmitter includes an RF transmitter.
7. The system according to claim 1 wherein the power level transmitter includes an RF transmitter.
8. The system according to claim 1 wherein the receiving unit comprises at least one antenna.
9. The system according to claim 1 wherein the receiver comprises a plurality of antennas.
10. The system according to claim 9 wherein the receiving unit is configured to determine which antenna is receiving the strongest signal and is configured to sample transmission from the antenna receiving the strongest signal for data regarding power level of a signal transmitted from the signal transmitter.
11. The system according to claim 1 wherein the receiving unit is portable.
12. The system according to claim 1 wherein at least one in vivo sensor includes an image sensor.
13. The system according to claim 12 wherein the swallowable capsule further comprises at least one illumination source.
14. The system according to claim 1 wherein the at least one in vivo sensor is selected from a group consisting of: a temperature sensor, a pH meter, and a pressure sensor.
15. The system according to claim 1 wherein the swallowable capsule is an ingestible imaging capsule.
16. The system according to claim 1 wherein the power level receiver includes an RF receiver.
17. A method for changing data transmission from a swallowable capsule, the method comprising the steps of:
 - obtaining a data transmission from within a body;
 - in response to the transmission, transmitting a command to adjust a power level of data transmission and changing a data transmission strength.
18. The method of claim 17 comprising comparing the data transmission strength to a threshold value, wherein the change is according to a comparison.

19. The method according to claim 17 wherein the step of obtaining a data transmission comprises determining signal strength.

20. The method according to claim 17 wherein the step of obtaining a data transmission comprises measuring the signal strength of a blank portion of the transmission.

21. The method according to claim 17 wherein the step of changing comprises raising or lowering the transmission strength.

22. The method according to claim 17 wherein the step of changing comprises raising or lowering the transmission strength by a predetermined value.

23. The method according to claim 17 wherein the step of obtaining a data transmission comprises obtaining a sample of a data transmission and wherein the step of changing a transmission strength comprises changing the strength of the same transmission.

24. The method according to claim 17 wherein the step of obtaining a data transmission comprises obtaining a sample of a data transmission and wherein the step of changing a transmission strength comprises changing the strength of a subsequent transmission.

25. The method according to claim 17, wherein the data transmission includes image data.

26. The method of claim 17, wherein the swallowable capsule is an imaging capsule.

27. The method according to claim 17 wherein the step of determining the transmission strength comprises the steps of:

- determining a strongest signal source; and
- obtaining a data transmission from the strongest signal source.

28. A method for controlling image data transmission from a swallowable capsule, the method comprising:

- receiving a data transmission having a signal strength;
- evaluating the signal strength;
- transmitting a command to adjust a power level of data transmission; and
- altering a capsule data transmission power level.

29. A method for changing image data transmission from a swallowable capsule, the method comprising the steps of:

- obtaining a sample of a data transmission of image data from within a body to determine the transmission strength;
- comparing the data transmission strength to a threshold value;
- transmitting a command to adjust a power level of data transmission; and
- changing a data transmission strength according to the comparison.

30. The method according to claim 29 comprising initial steps of:

- obtaining images from a body lumen; and
- transmitting image data.

31. The method according to claim 29 wherein the step of obtaining images is performed by an ingestible imaging capsule.

专利名称(译)	用于改变来自体内传感装置的传输的系统和方法		
公开(公告)号	US6934573	公开(公告)日	2005-08-23
申请号	US10/200548	申请日	2002-07-23
[标]申请(专利权)人(译)	基文影像公司		
申请(专利权)人(译)	基文影像有限公司.		
当前申请(专利权)人(译)	基文影像有限公司.		
[标]发明人	GLUKHOVSKY ARKADY ERLICH BARUCH		
发明人	GLUKHOVSKY, ARKADY ERLICH, BARUCH		
IPC分类号	A61B17/00 A61B5/00 A61B5/07 H04B7/005 A61B5/05		
CPC分类号	A61B1/00036 A61B1/041 A61B5/0031 A61B5/073 A61B5/14539 H04W52/06 A61B1/00016 A61B5/01 A61B2017/00137 A61B2560/0209 H04W52/08 H04W52/10		
审查员(译)	ROBINSON , DANIEL		
优先权	60/306872 2001-07-23 US		
外部链接	Espacenet USPTO		

摘要(译)

装置，系统和方法使得能够从体腔或腔内获得诸如体内图像的数据，例如胃肠（GI）道的图像。设备可以包括成像系统和射频（RF）发射器，用于将信号从成像设备发送到接收系统。可以改变或改变发射器的信号强度，以解决例如由身体组织引起的信号衰减量。

