



US006939313B2

(12) **United States Patent**
Saadat et al.

(10) **Patent No.:** **US 6,939,313 B2**
(45) **Date of Patent:** **Sep. 6, 2005**

(54) **DEVICE FOR SENSING PARAMETERS OF A HOLLOW BODY ORGAN**

(76) Inventors: **Vahid Saadat**, 12679 Kane Dr., Saratoga, CA (US) 95070; **Ross Tsugita**, 1653 Gretel La., Mountain View, CA (US) 94040-3706

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 281 days.

(21) Appl. No.: **10/146,014**

(22) Filed: **May 14, 2002**

(65) **Prior Publication Data**

US 2003/0088187 A1 May 8, 2003

Related U.S. Application Data

(63) Continuation-in-part of application No. 09/904,212, filed on Jul. 12, 2001, now abandoned.

(51) **Int. Cl.**⁷ **A61B 5/103**; A61B 5/117

(52) **U.S. Cl.** **600/587**

(58) **Field of Search** 600/585, 433, 600/434, 435, 474, 481, 505, 549, 1; 374/141, 148, 166, 179; 606/41, 194, 32, 49; 604/530, 913, 95.01; 607/122, 99; 378/44

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,215,275 A	7/1980	Wickersheim	
4,301,023 A	11/1981	Schuberth et al.	
RE32,204 E	7/1986	Halvorsen	
4,699,147 A	10/1987	Chilson et al.	
4,777,955 A	10/1988	Brayton et al.	
4,862,887 A	9/1989	Weber et al.	
4,883,459 A	11/1989	Calderon	
4,884,573 A *	12/1989	Wijay et al.	606/194
4,952,033 A	8/1990	Davis	
4,958,642 A	9/1990	Christian et al.	
4,995,398 A	2/1991	Turnidge	

(Continued)

FOREIGN PATENT DOCUMENTS

WO	WO 97/10748 A1	3/1997
WO	WO 01/13603 A1	3/2000
WO	WO 00/27278 A1	5/2000
WO	WO 01/74263 A1	10/2001

OTHER PUBLICATIONS

Pasterkamp, G. et al. (Jul. 2000). "Techniques Characterizing the Coronary Atherosclerotic Plaque: Influence on Clinical Decision Making?" *J. Am. Coll. Cardiol.* 36(1):13-21.
 Stefanadis, C. et al. (Apr. 1999). "Thermal Heterogeneity Within Human Atherosclerotic Coronary Arteries Detected In Vivo," *Circulation* 99:1965-1971.

Bolz, Ray E. and Tuve, George L. (eds) (1973) Chapter 10 Transducers and Measurement Techniques, *CRC Handbook of Tables for Applied Engineering Science*, 2nd edition, CRC Press, pp. 975-978.

Brochure from Parker (May 1992) Compumotor Digiplan, Positioning Control Systems and Drives, Parker, Catalog 8000, Engineering Reference and Application Solutions, Table of Contents and A77 A80 (Glossary of Terms).

Inflammation Hypothesis, Vulnerable Plaque, Milestones in Vulnerable Plaque and Atherosclerosis Research, located at <<http://www.vp.org/Milestones/Milestones.htm>> visited on Jun. 30, 2002, 2 pages, see under # 1856.

Primary Examiner—Max F. Hindenburg


Assistant Examiner—Brian Szmal

(57)

ABSTRACT

A device for sensing the profile of a hollow body organ includes a hollow guidewire or probe carrying a sensor. The hollow probe includes a distal coiled end tube with a tip bent at an angle between about 10° to 90° relative to the probe longitudinal axis and having a torque response of no more than about 0.4 ozf in. The flexural rigidity of the distal end tube relative to the mid and proximal end tubes forming the probe is generally in the range of about 1:(4 to 4,400):(110 to 13,000), respectively. An actuator is detachably secured to the probe and includes one or several motors which allow the sensor to travel in a rotational and axial path through the body organ.

45 Claims, 27 Drawing Sheets

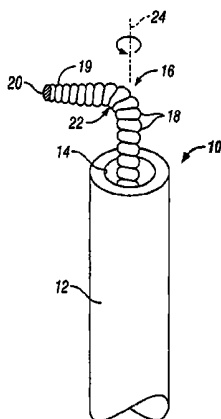


US 6,939,313 B2

Page 2

U.S. PATENT DOCUMENTS

5,054,501 A	10/1991	Chuttani et al.	5,938,624 A	8/1999	Akerfeldt et al.
5,069,226 A	12/1991	Yamauchi et al.	5,980,563 A	11/1999	Tu et al.
5,124,819 A	6/1992	Davis	5,989,242 A	11/1999	Saadat et al.
5,178,159 A	1/1993	Christian	6,010,476 A	1/2000	Saadat
5,237,996 A	8/1993	Waldman et al.	6,071,277 A	6/2000	Farley et al.
5,279,299 A	1/1994	Imran	6,090,052 A	7/2000	Akerfeldt et al.
5,304,194 A	4/1994	Chee et al.	6,106,486 A	8/2000	Tenerz et al.
5,342,300 A	8/1994	Stefanadis et al.	6,142,958 A	11/2000	Hammarström et al.
5,623,940 A	4/1997	Daikuzono	6,156,046 A	12/2000	Passafaro et al.
5,657,764 A	8/1997	Coulter et al.	6,167,763 B1	1/2001	Tenerz et al.
RE35,648 E	11/1997	Tenerz et al.	6,196,980 B1	3/2001	Akerfeldt et al.
5,701,905 A	12/1997	Esch	6,197,021 B1	3/2001	Panescu et al.
5,730,741 A	3/1998	Horzewski et al.	6,245,026 B1	6/2001	Campbell et al.
5,733,739 A	3/1998	Zakim et al.	6,267,746 B1	7/2001	Bumbalough
5,741,214 A	4/1998	Ouchi et al.	6,267,781 B1	7/2001	Tu
5,769,846 A	6/1998	Edwards et al.	6,312,425 B1	11/2001	Simpson et al.
5,771,895 A	6/1998	Slager	6,371,928 B1	4/2002	Mcfann et al.
5,782,741 A	7/1998	Bradshaw et al.	6,406,442 B1	6/2002	McFann et al.
5,871,449 A	2/1999	Brown	6,786,905 B2 *	9/2004	Swanson et al. 606/32
5,910,101 A	6/1999	Andrews et al.	2001/0053882 A1	12/2001	Haddock et al.
5,924,997 A	7/1999	Campbell	2002/0067754 A1	6/2002	Werneth
5,935,075 A	8/1999	Casscells et al.	2003/0055307 A1 *	3/2003	Elmaleh et al. 600/1

* cited by examiner

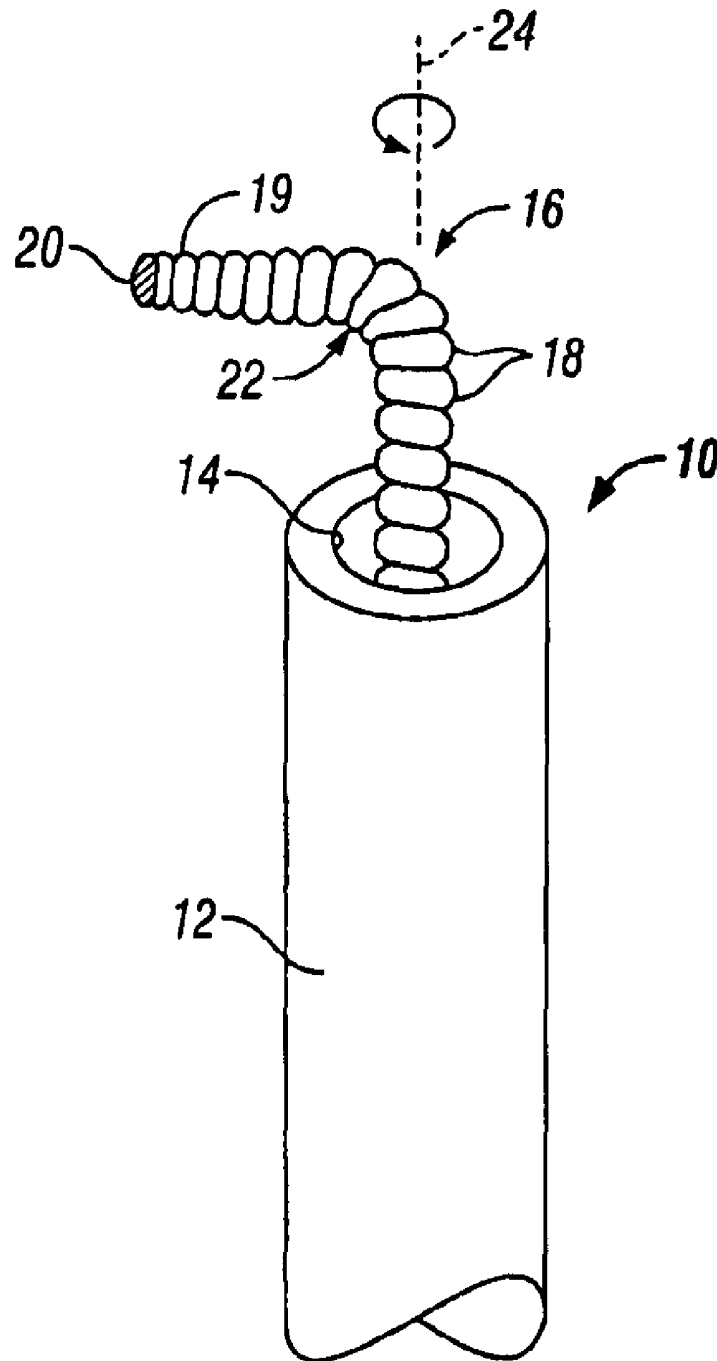**FIG. 1**

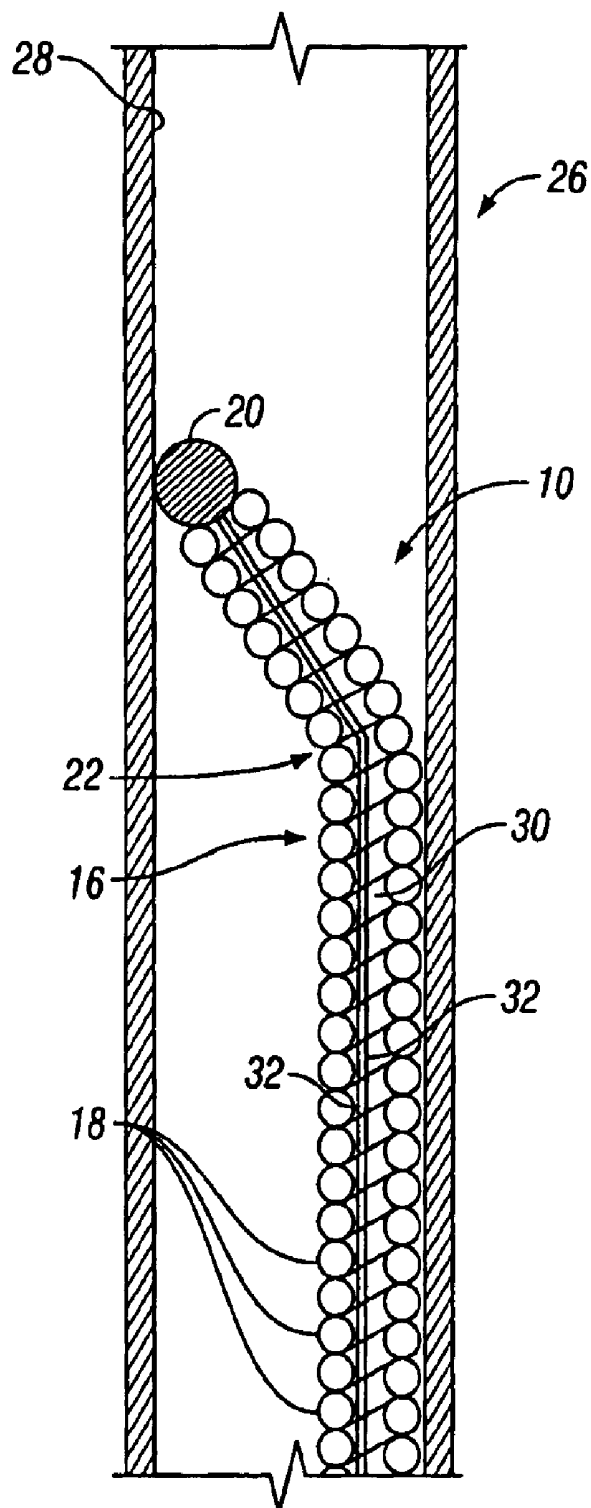


FIG. 2

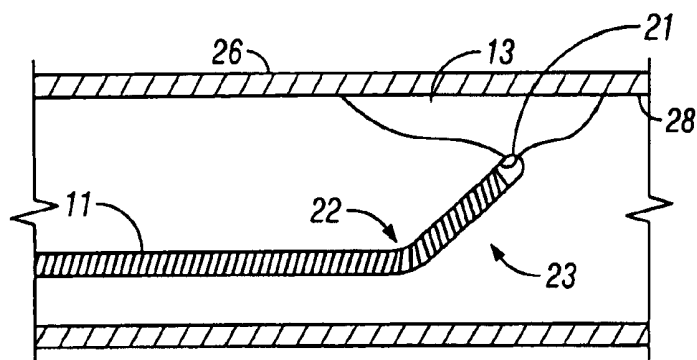


FIG. 3A

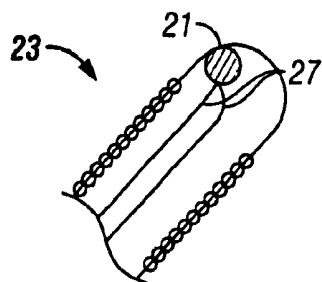


FIG. 3B

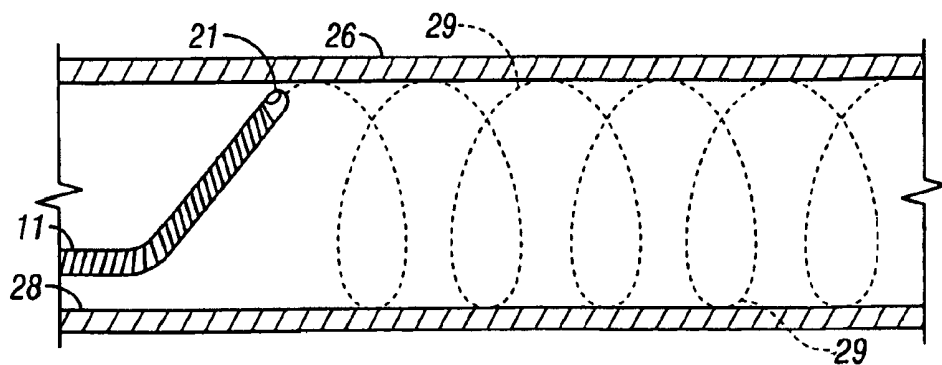


FIG. 4A

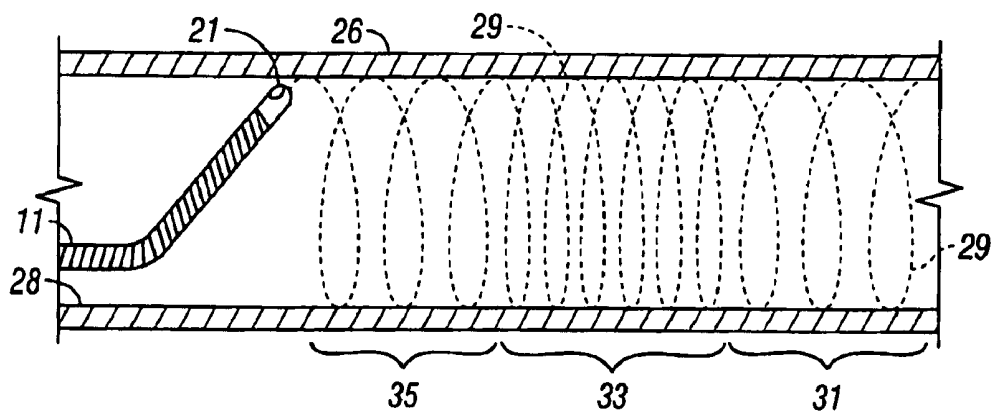
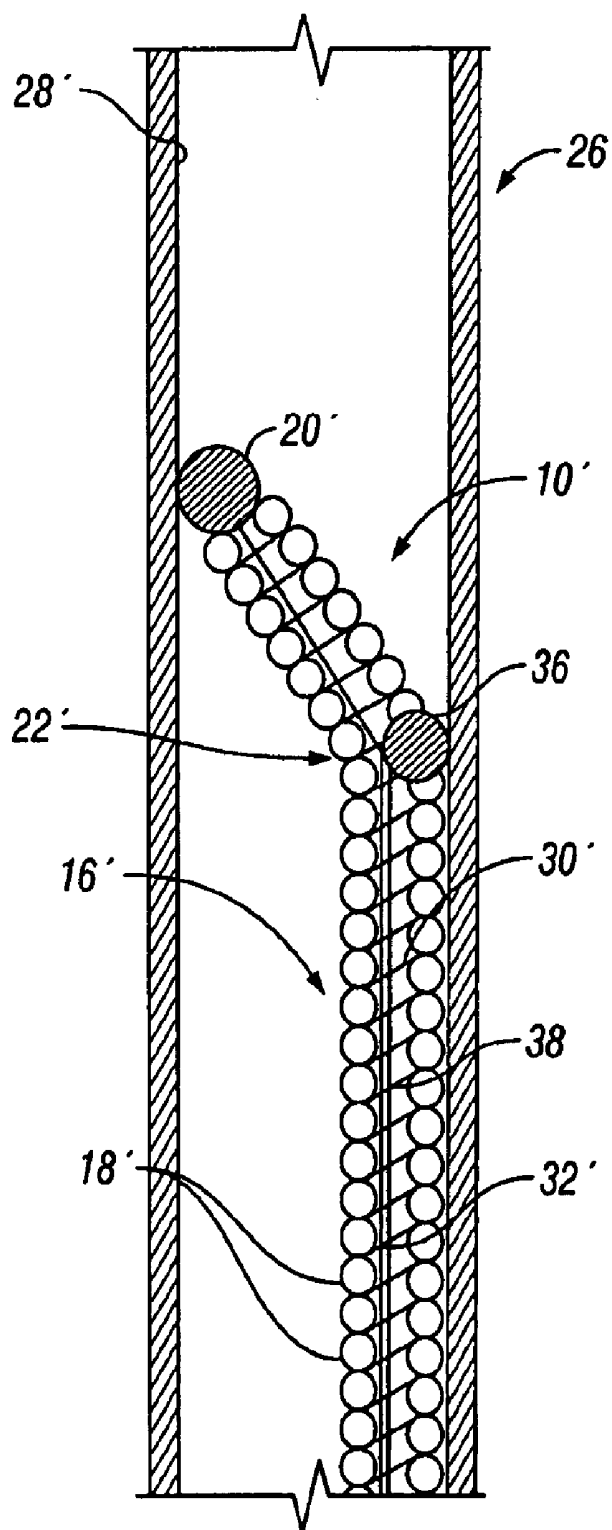


FIG. 4B

**FIG. 5**

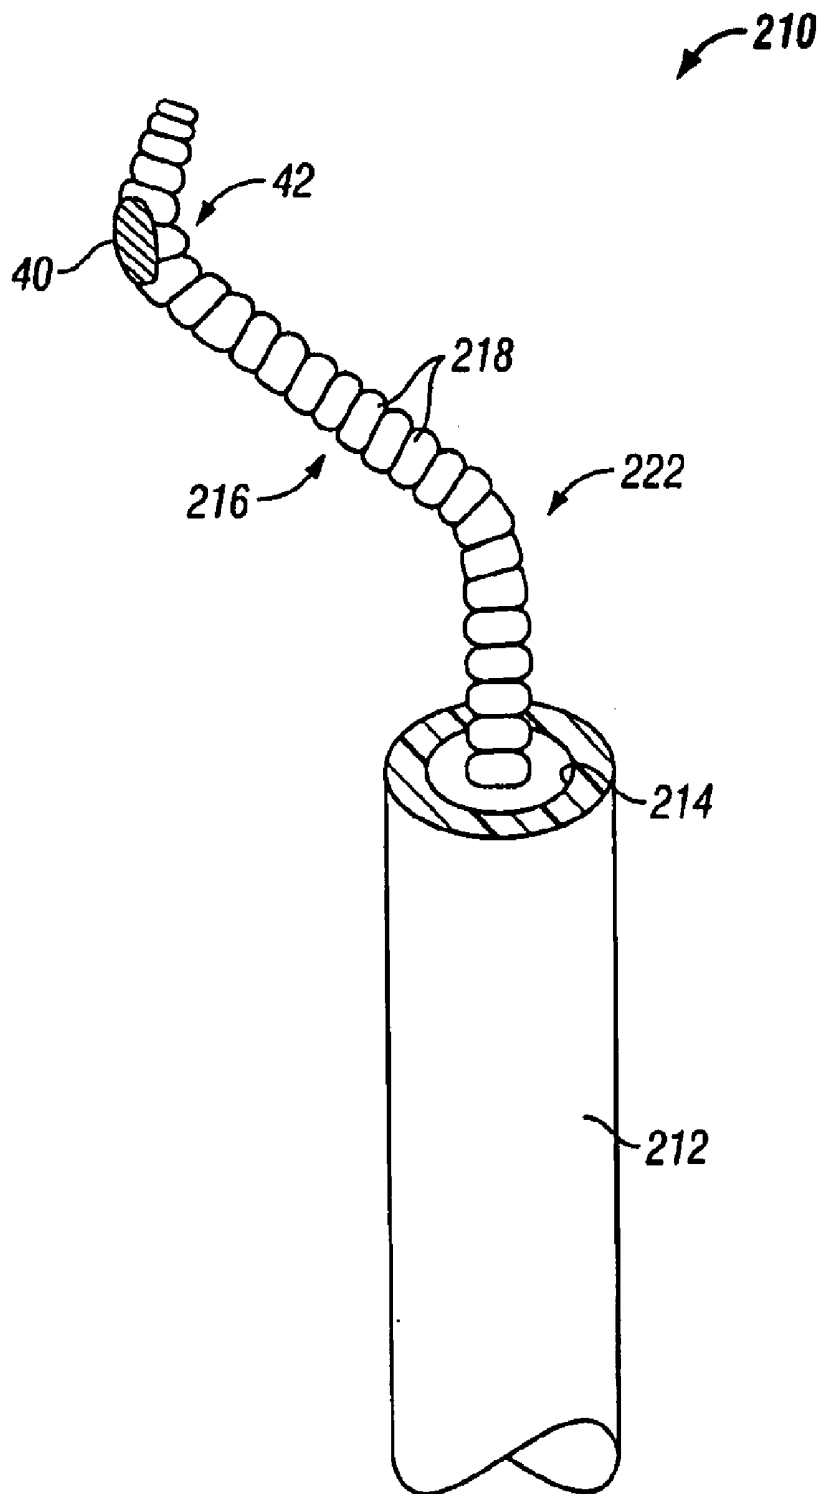
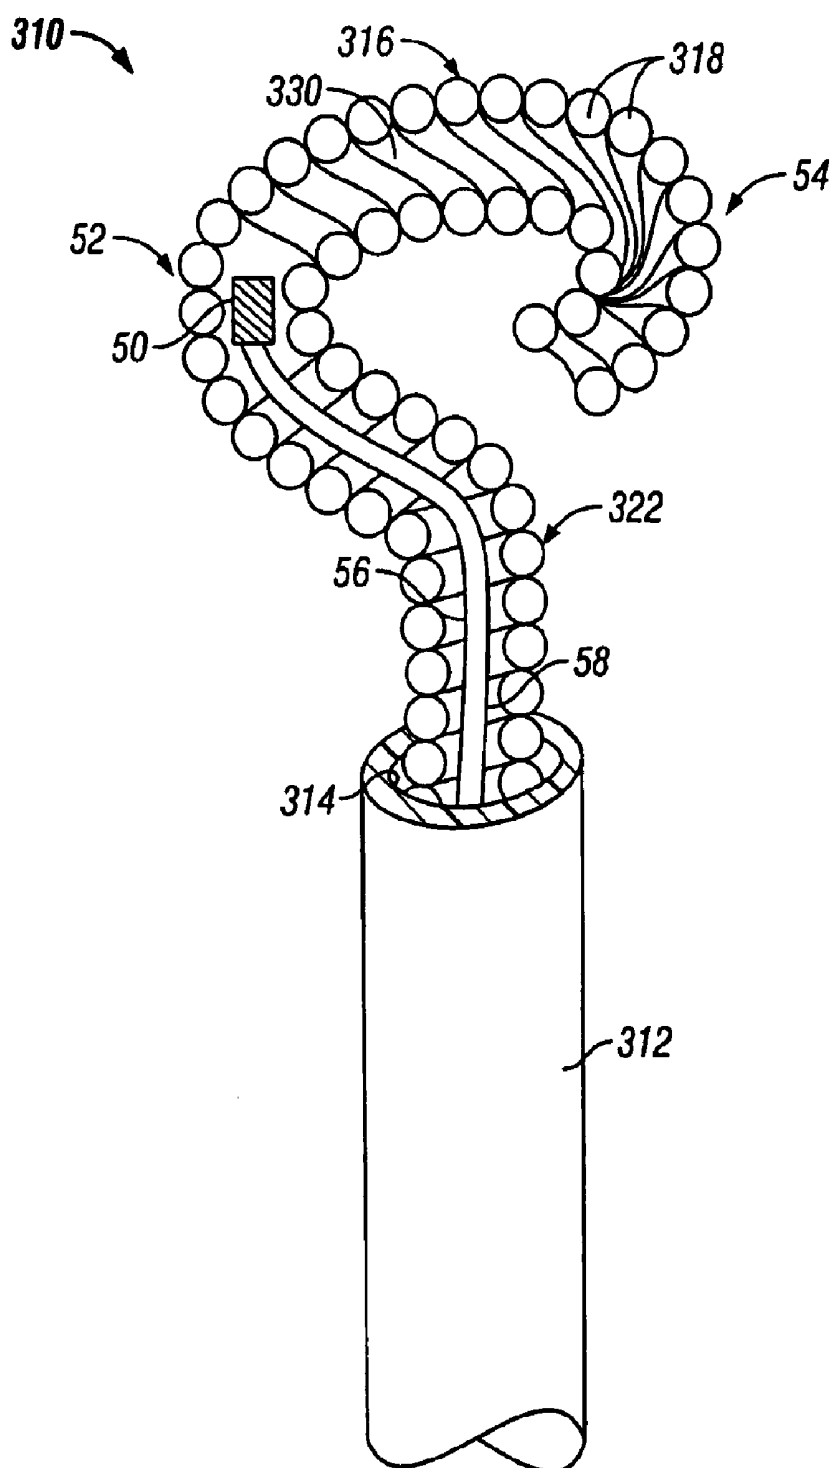
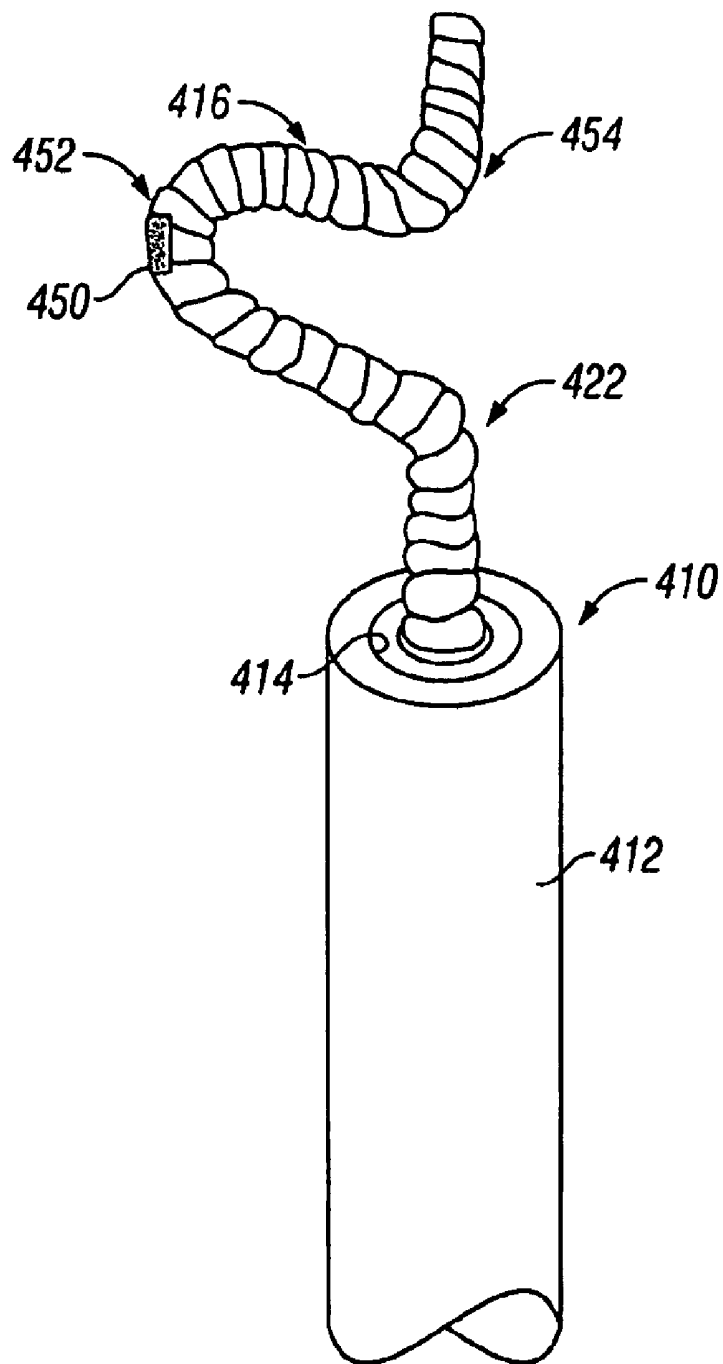


FIG. 6

**FIG. 7**

**FIG. 8**

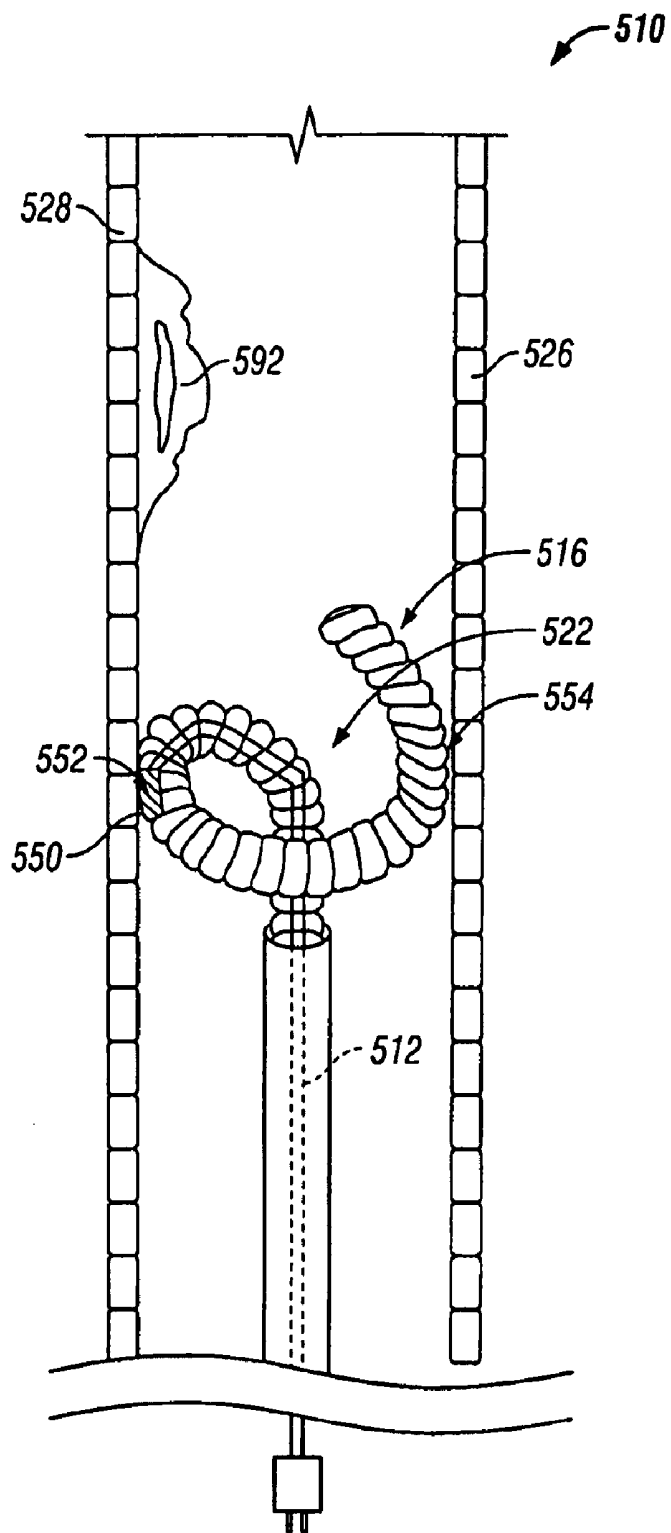


FIG. 9

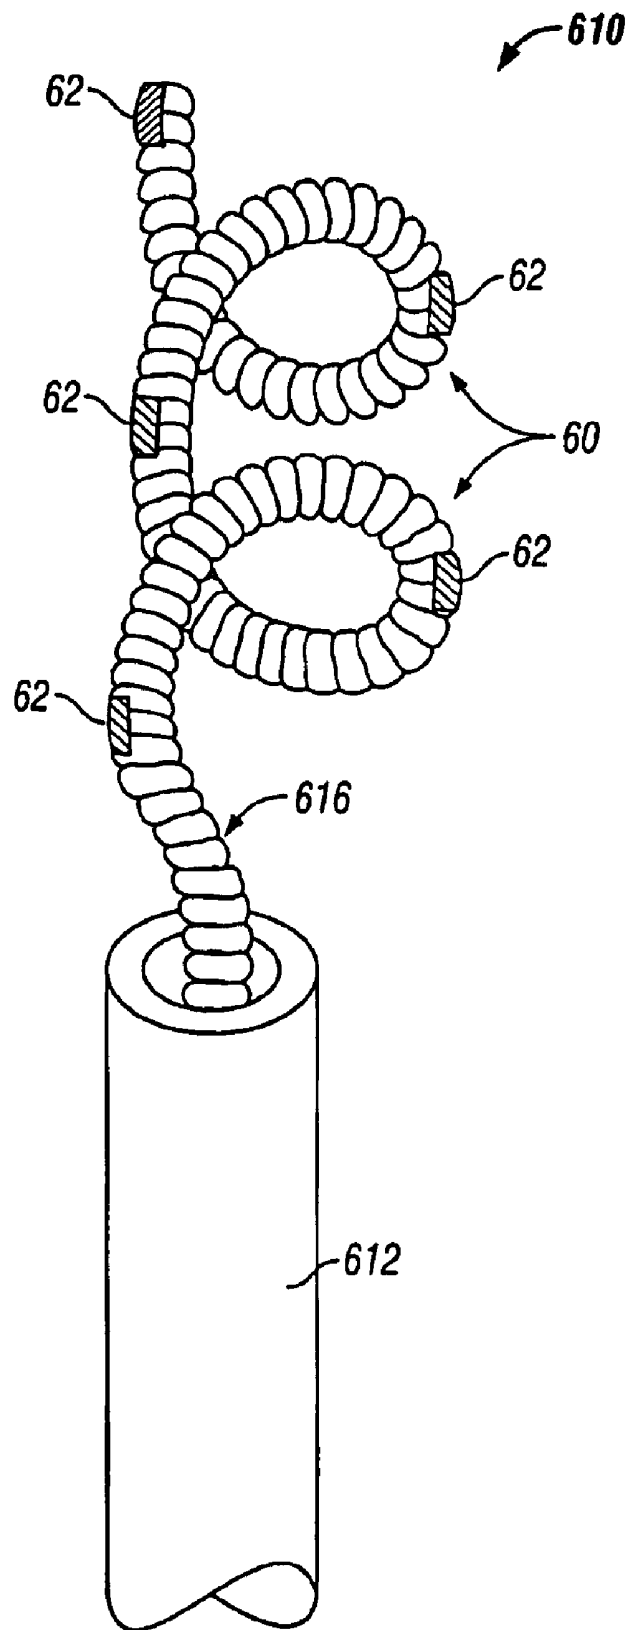


FIG. 10

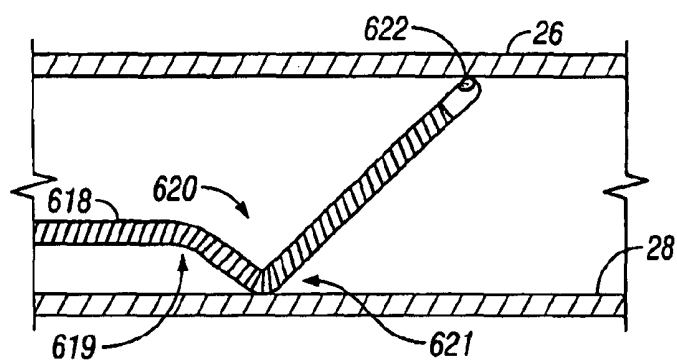


FIG. 11

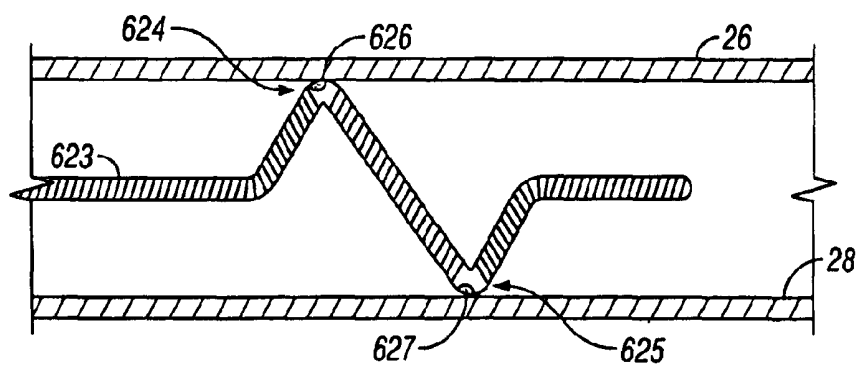


FIG. 12

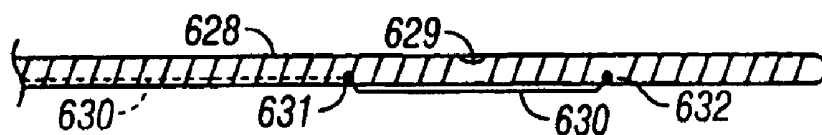


FIG. 13A

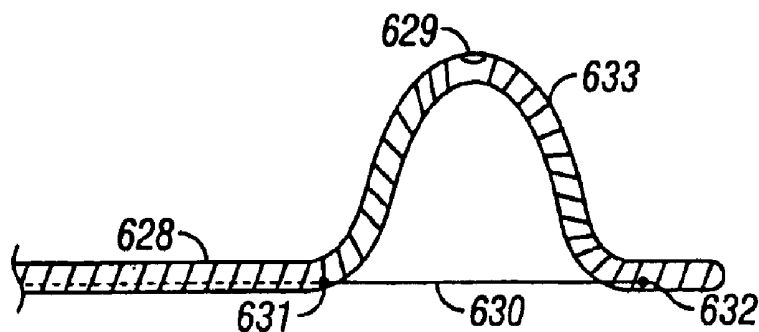


FIG. 13B




FIG. 14A

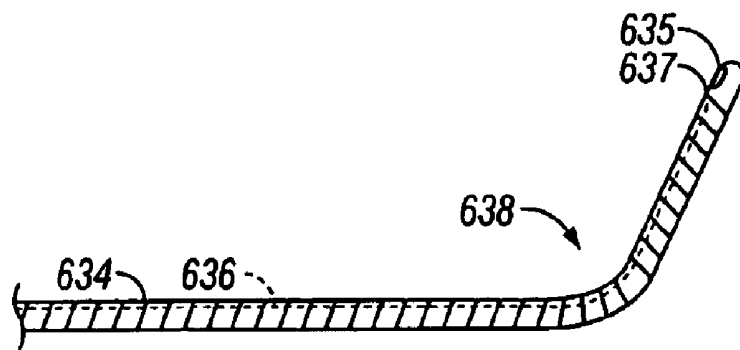


FIG. 14B

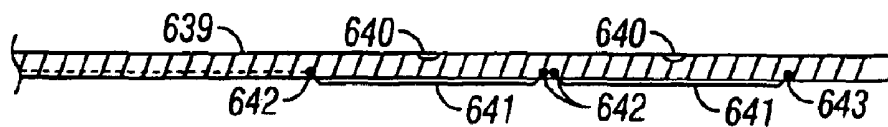


FIG. 15A

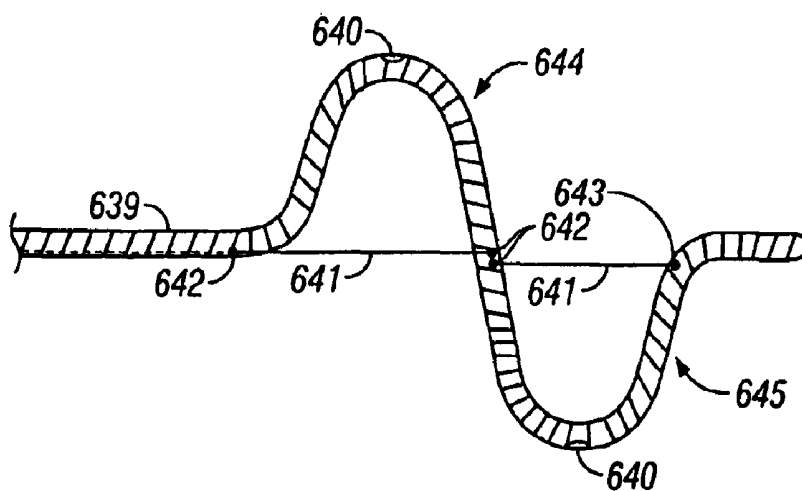


FIG. 15B

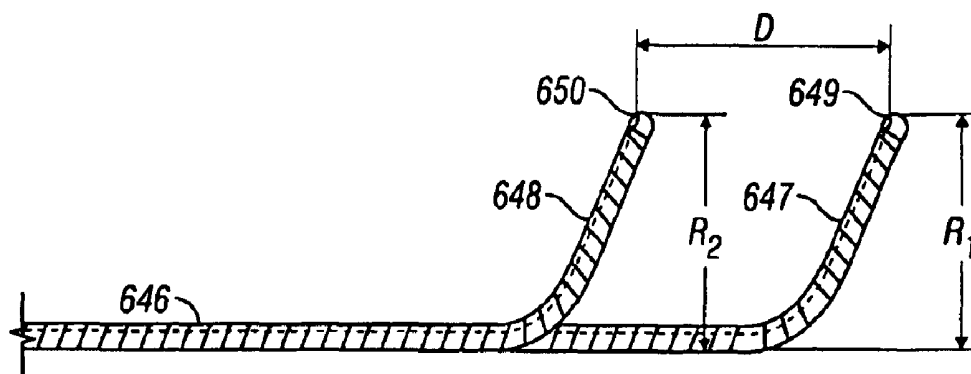


FIG. 16

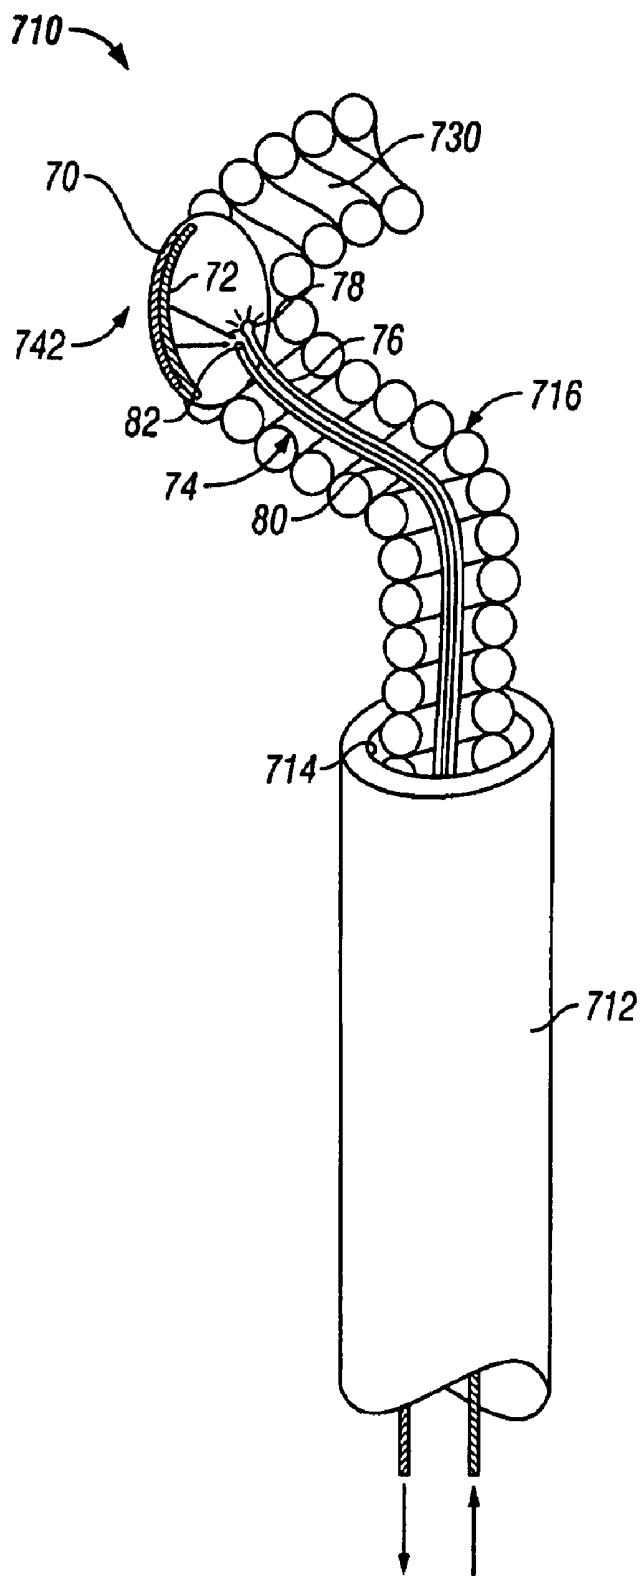


FIG. 17

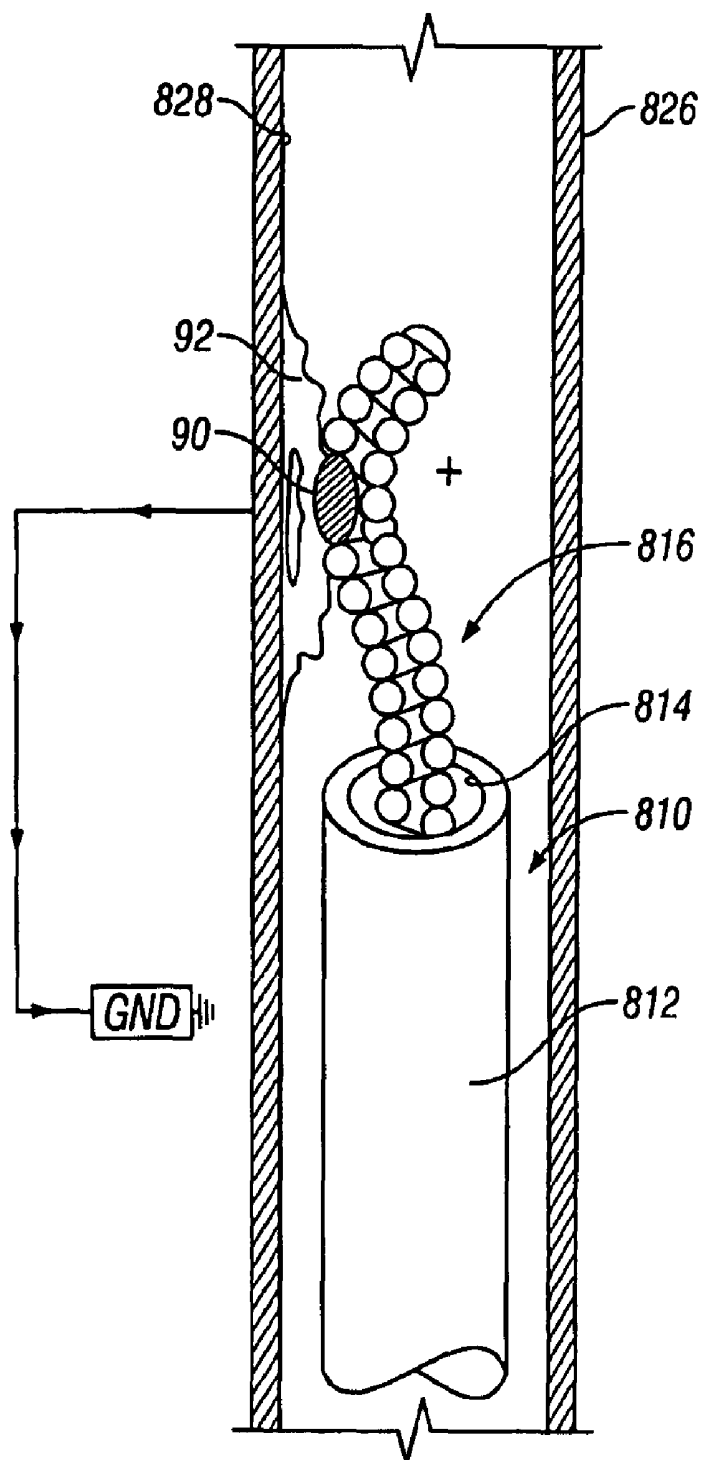


FIG. 18

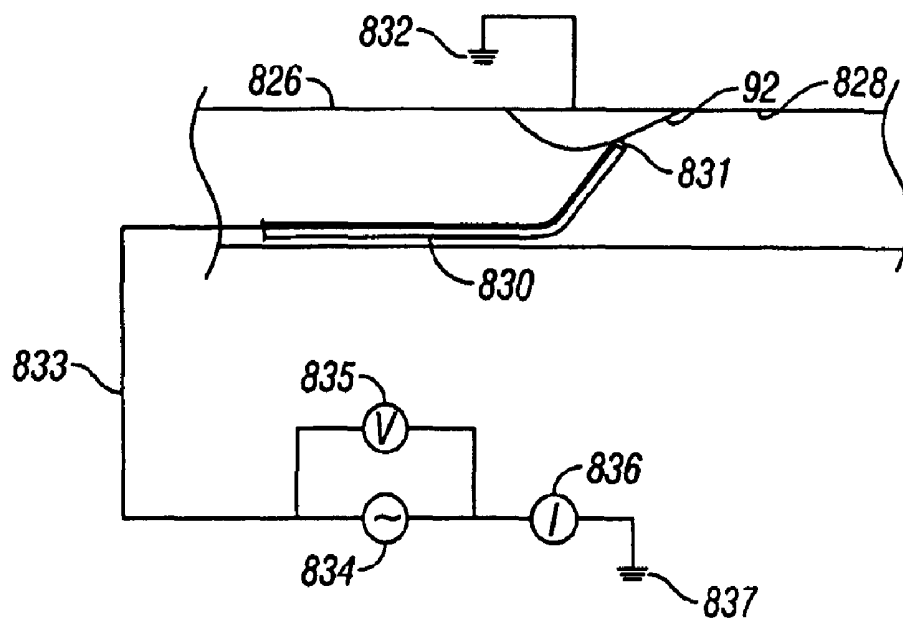


FIG. 19

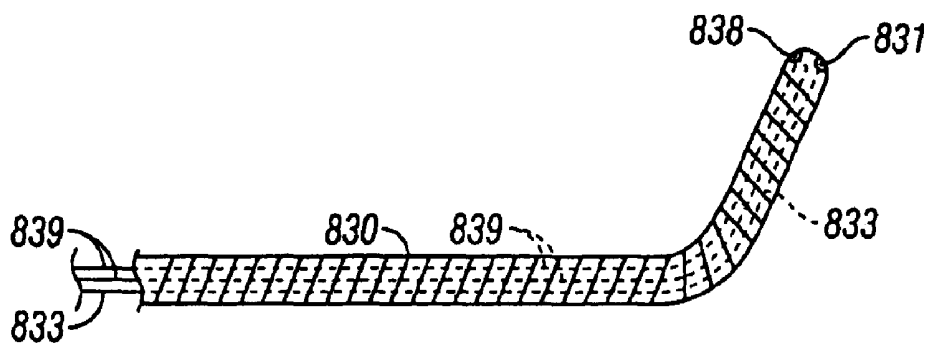


FIG. 20

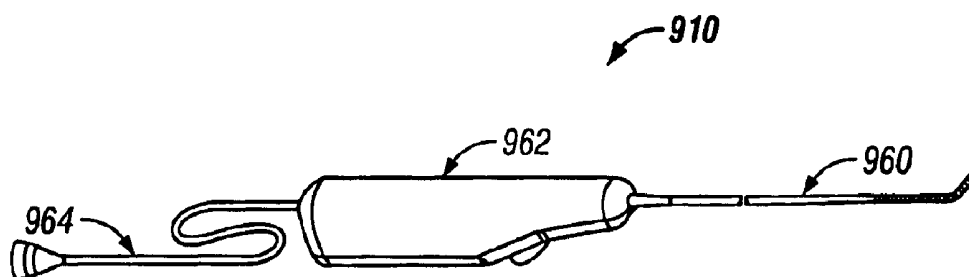


FIG. 21A

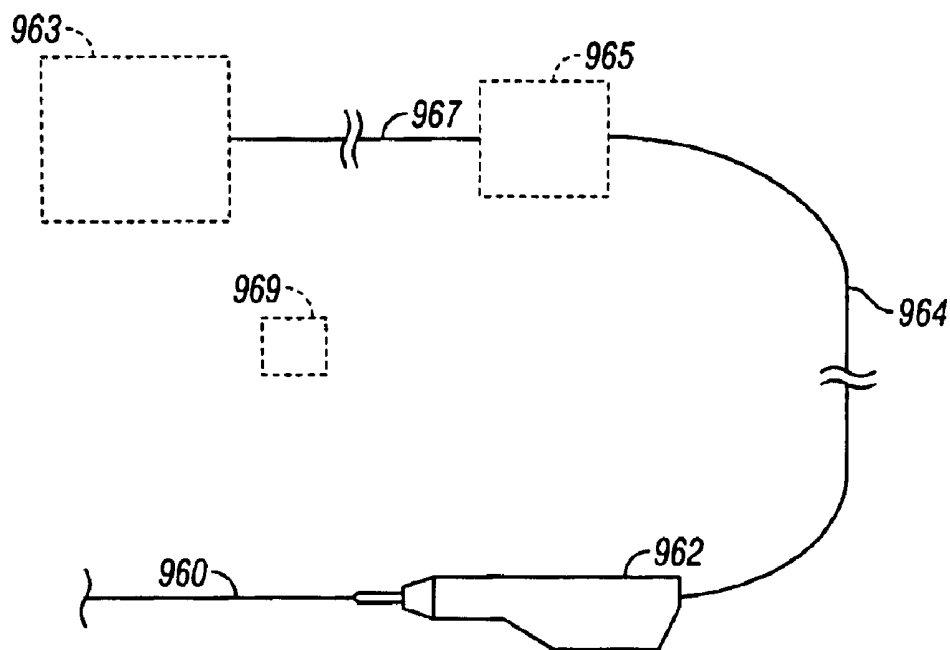


FIG. 21B

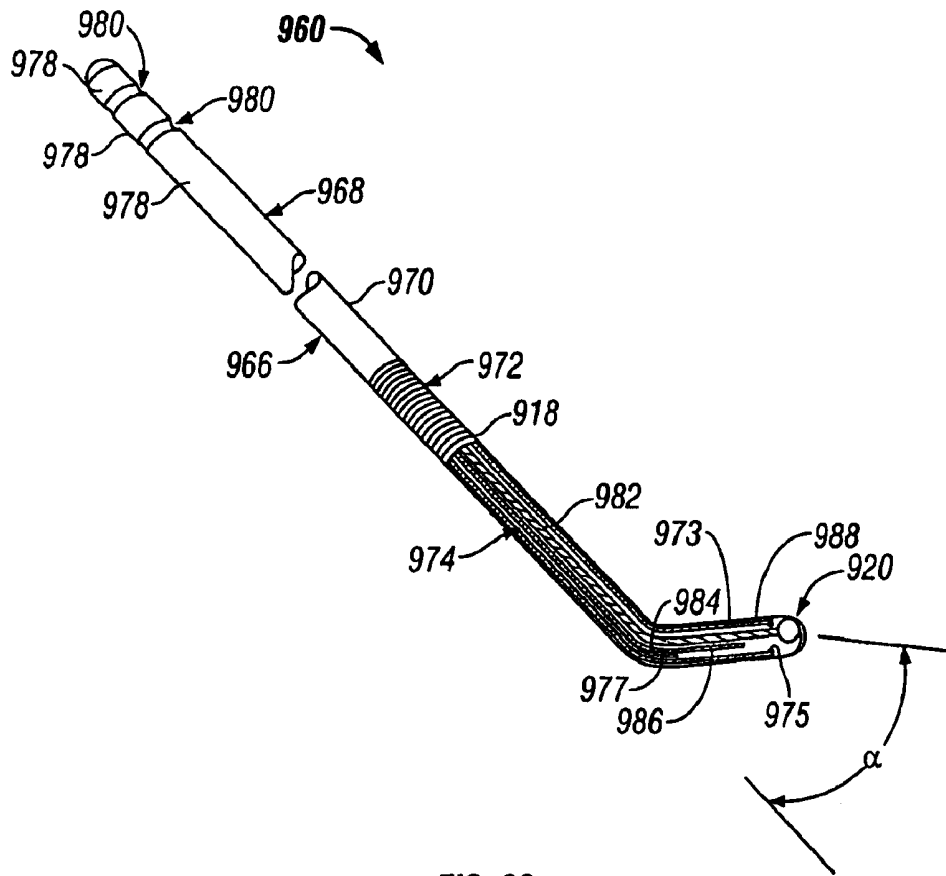


FIG. 22

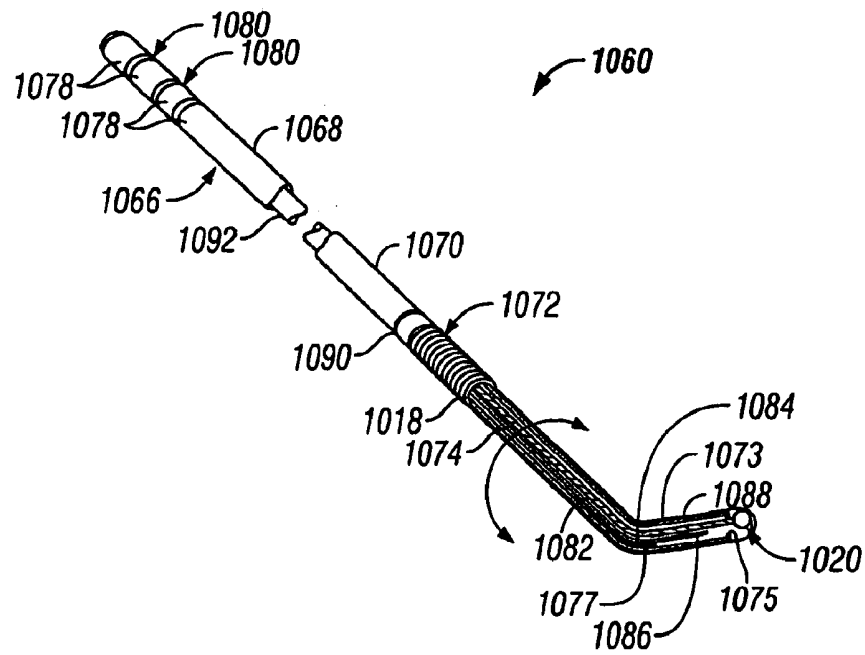


FIG. 23

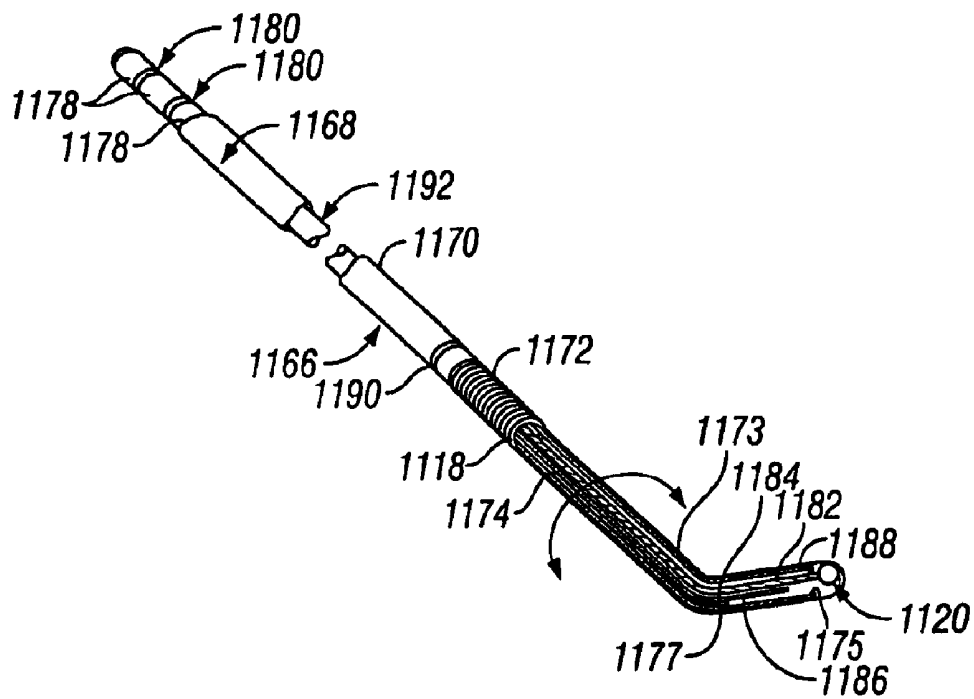


FIG. 24

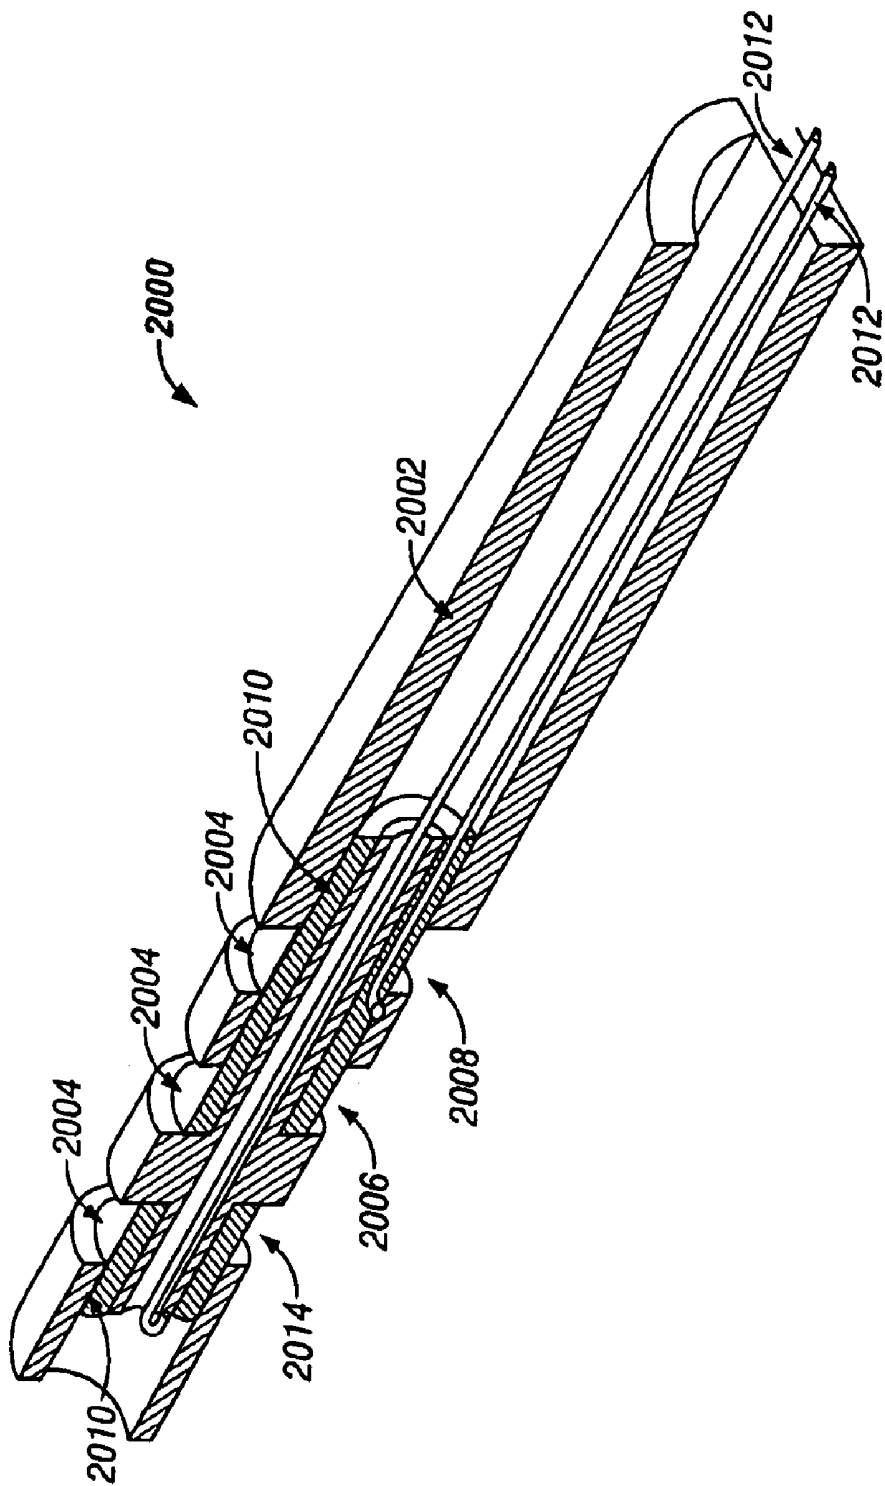


FIG. 25A

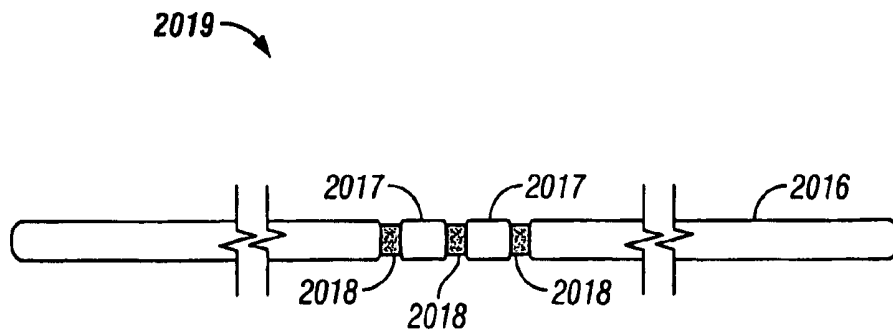


FIG. 25B

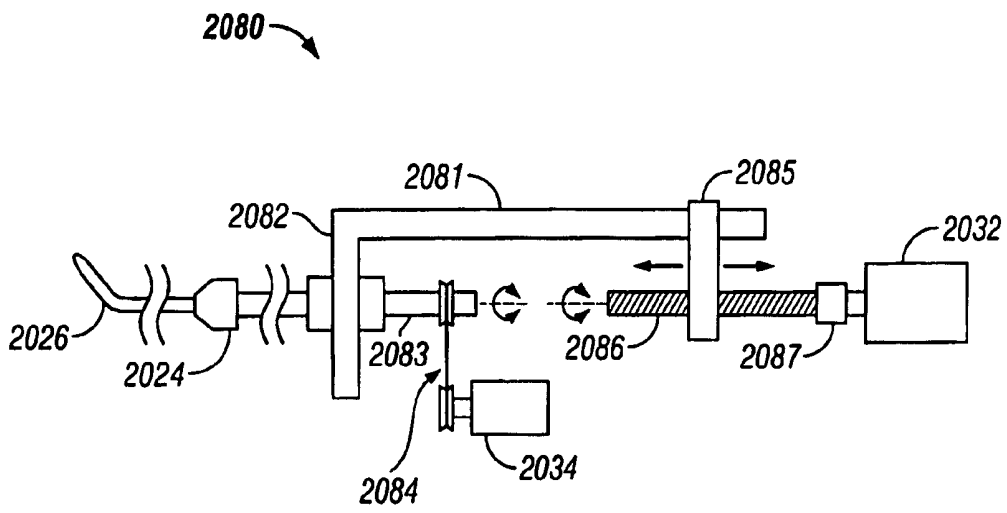


FIG. 26

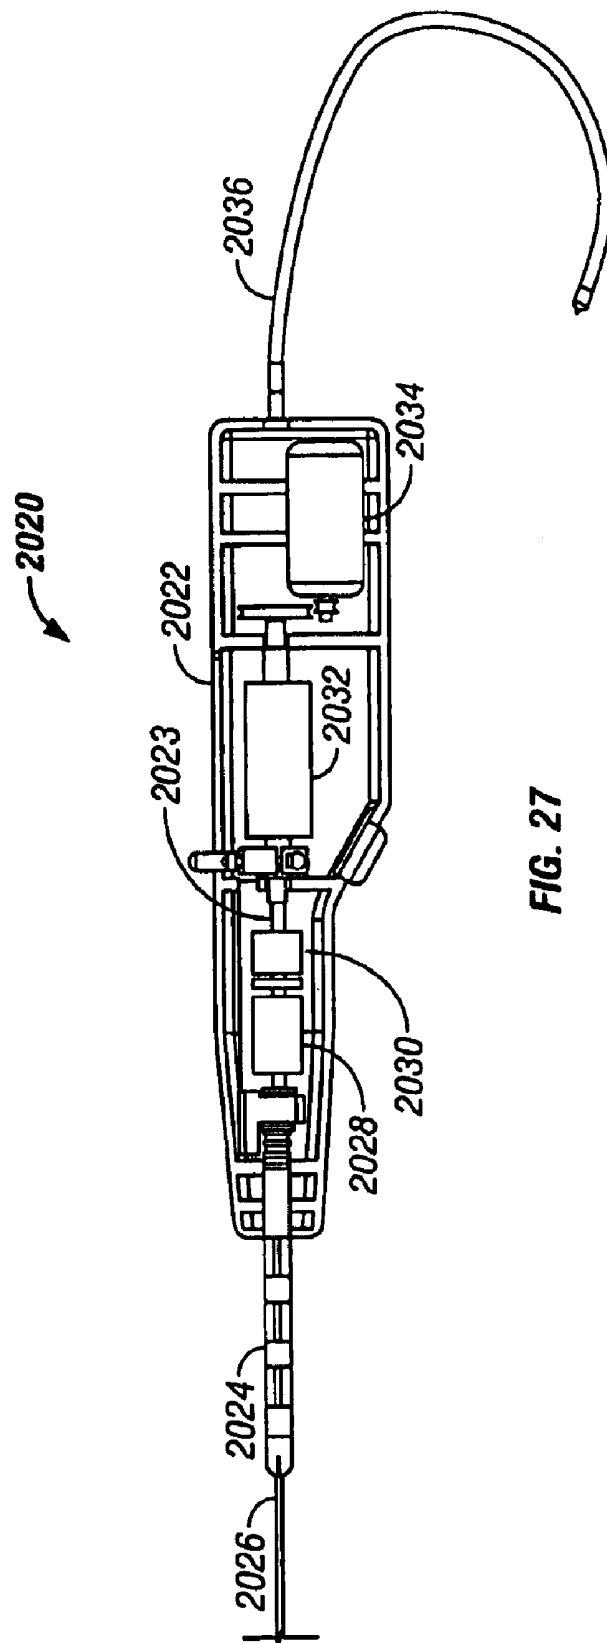
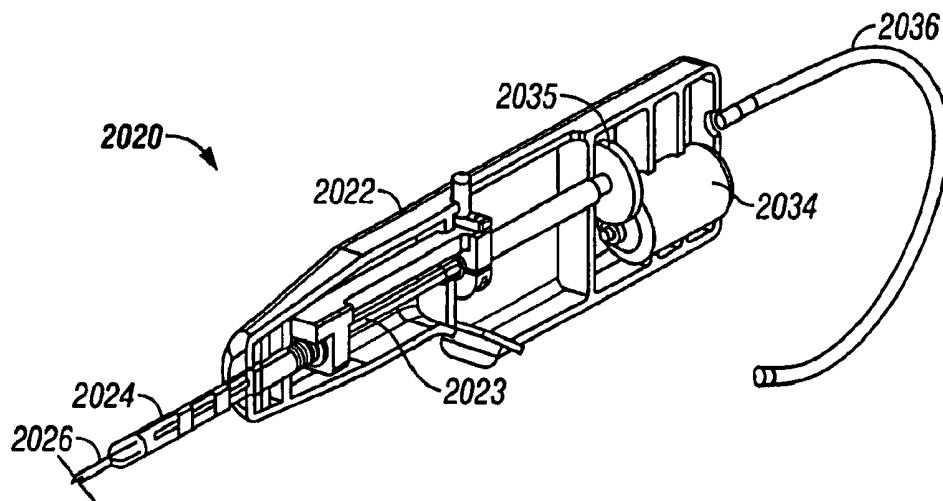


FIG. 27

**FIG. 28**

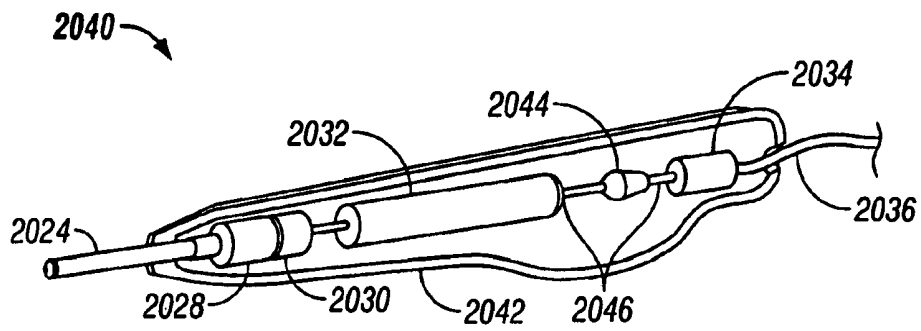


FIG. 29

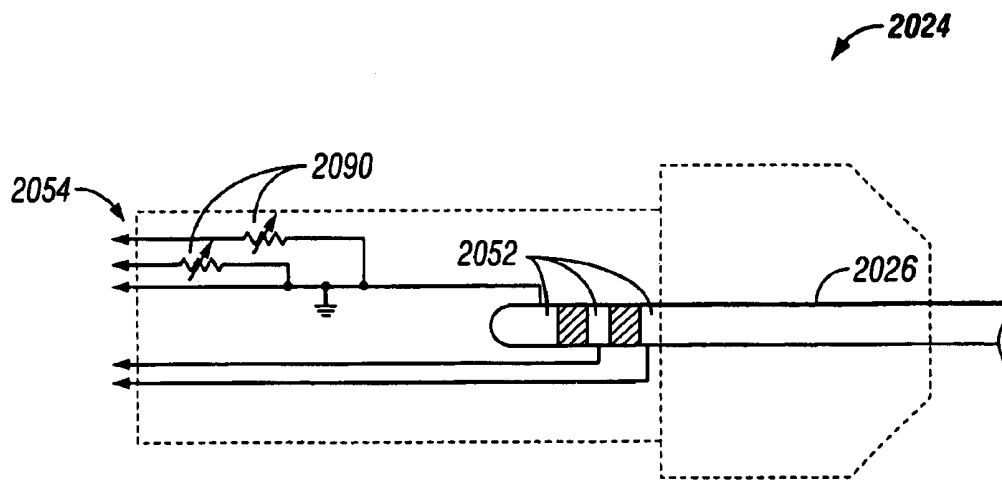


FIG. 30B

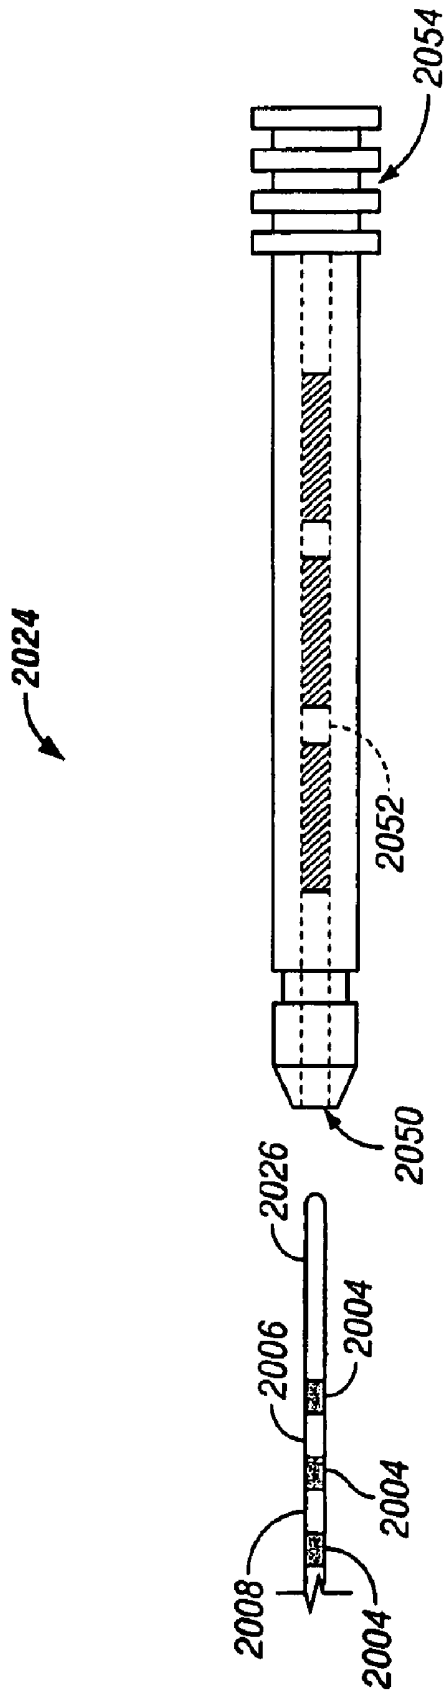
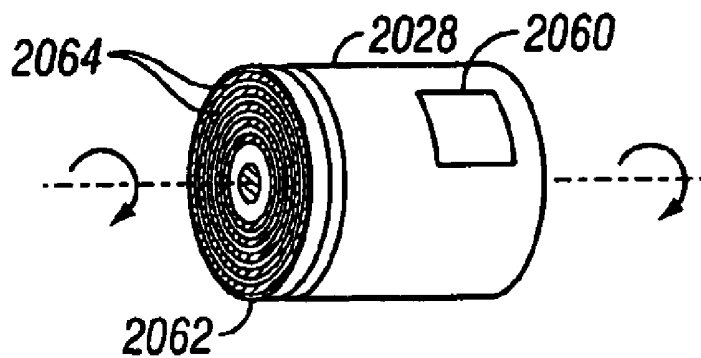
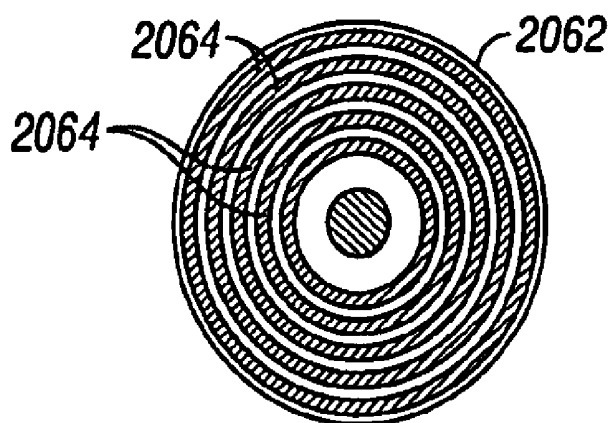


FIG. 30A

**FIG. 31A****FIG. 31B**

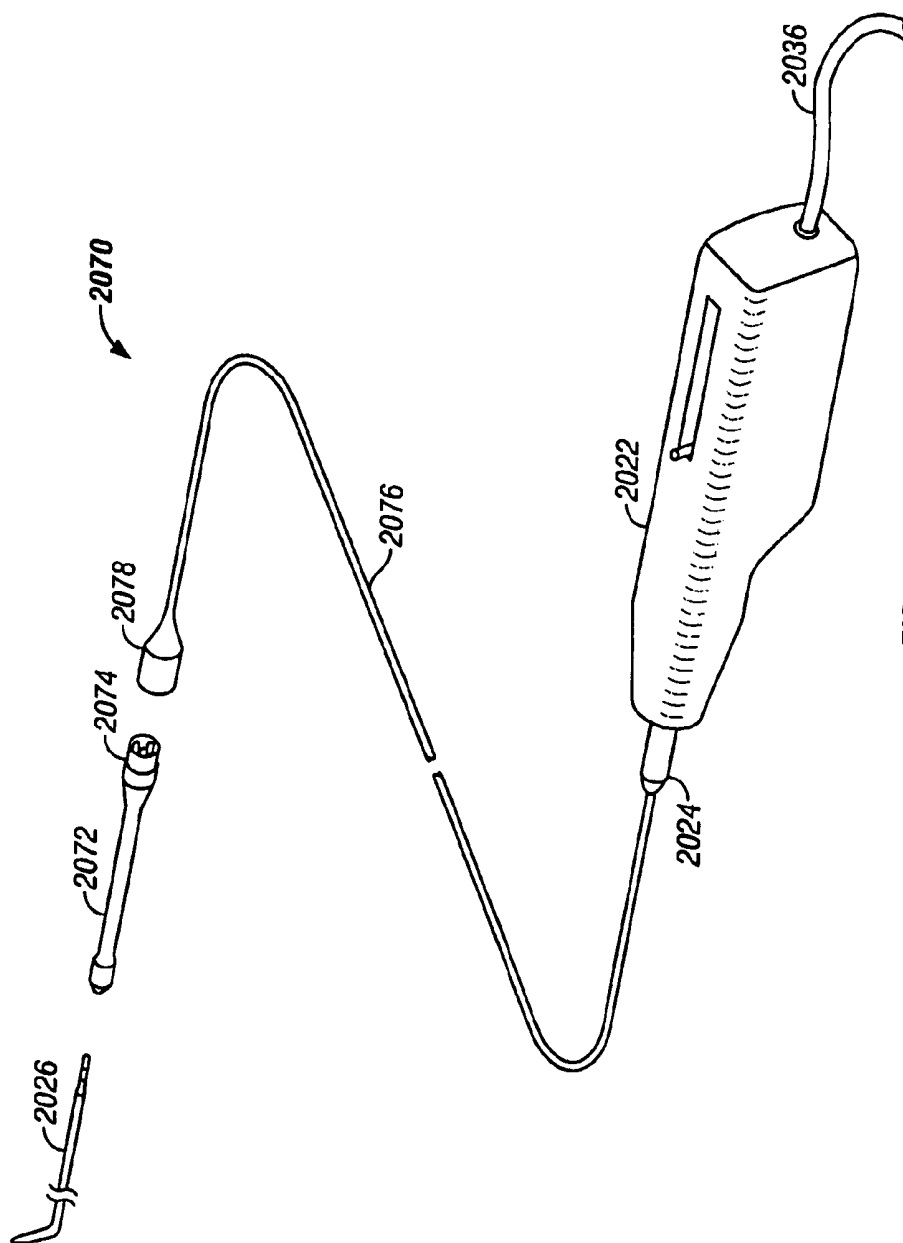


FIG. 32

DEVICE FOR SENSING PARAMETERS OF A HOLLOW BODY ORGAN

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part of U.S. patent application Ser. No. 09/904,212, filed on Jul. 12, 2001 (now abandoned).

TECHNICAL FIELD OF THE INVENTION

This invention relates generally to invasive medical devices and more particularly to devices for sensing the profile of the interior wall of a hollow body organ such as a blood vessel.

BACKGROUND OF THE INVENTION

Acute ischemic syndromes involving arterial blood vessels, such as myocardial infarction, or heart attack, and stroke, frequently occur when atherosclerotic plaque ruptures, triggering the formation of blood clots, or thrombosis. Plaque that is inflamed is particularly unstable and vulnerable to disruption, with potentially devastating consequences. Therefore, there is a strong need to detect and locate this type of plaque so that treatment can be initiated before the plaque undergoes disruption and induces subsequent life-threatening clotting.

Various procedures are known for detecting and locating plaque in a blood vessel. Angiography is one such procedure in which X-ray images of blood vessels are generated after a radio-opaque dye is injected into the blood stream. This procedure is capable of locating plaque in an artery, but is not capable of revealing whether the plaque is the inflamed, unstable type.

Researchers, acting on the theory that inflammation is a factor in the development of atherosclerosis, have discovered that local variations of temperature along arterial walls can indicate the presence of inflamed plaque. The temperature at the site of inflammation, i.e., the unstable plaque, is elevated relative to adjacent plaque-free arterial walls.

Using a tiny thermal sensor at the end of a catheter, the temperature at multiple locations along an arterial wall were measured in people with and without atherosclerotic arteries. In people free of heart disease, the temperature was substantially homogeneous wherever measured: an average of 0.65 degrees F. above the oral temperature. In people with stable angina, the temperature of their plaques averaged 0.19 degrees F. above the temperature of their unaffected artery walls. The average temperature increase in people with unstable angina was 1.23 degrees F. The increase was 2.65 degrees F. in people who had just suffered a heart attack. Furthermore, temperature variation at different points at the plaque site itself was found to be greatest in people who had just had a heart attack. There was progressively less variation in people with unstable angina and stable angina.

The temperature heterogeneity discussed above can be exploited to detect and locate inflamed, unstable plaque through the use of cavity wall profiling apparatus. Typically, cavity wall profiling apparatus are comprised of temperature indicating probes such as thermocouples, thermistors, fluorescence lifetime measurement systems, resistance thermal devices and infrared measurement devices.

One problem with conventional cavity wall profiling apparatus is that they usually exert an undue amount of force on the region of interest. If the region of interest cannot withstand these forces, it may be damaged. The inside walls

of a healthy human artery are vulnerable to such damage. Furthermore, if inflamed, unstable plaque is present it may be ruptured by such forces.

Another problem with conventional cavity wall profiling apparatus is that they can only measure the temperature at one specific location. In order to generate a map of the cavity temperature variation, one would need to move the temperature indicating probe from location to location. This can be very tedious, can increase the risk of damaging the vessel wall or rupturing vulnerable plaque, and may not resolve temporal characteristics of the profile with sufficient resolution. An array of probes could be employed but that could be very big and heavy.

BRIEF SUMMARY OF THE INVENTION

According to one aspect of the invention, a device is provided for sensing the temperature profile of a hollow body organ. The device includes a hollow guidewire, a temperature sensor disposed on or within the guidewire, and an optional catheter through which the guidewire may be delivered. The guidewire has a relaxed configuration externally of the catheter that is formed to provide contact with the wall of the hollow body organ. The guidewire also has a contracted configuration internally of the catheter and is of a lesser diameter than the catheter.

According to another aspect of the invention, the device is used by contracting the guidewire elastically and constraining the guidewire within the catheter. The catheter and guidewire are advanced to a region of interest in a hollow body organ. The catheter is withdrawn to expose the distal portion of the guidewire which may then reconfigure into a relaxed configuration to make contact with the hollow body organ. Alternatively, the catheter may be held stationary relative to the hollow body organ and the guidewire may be advanced until the distal portion of the guidewire is exposed to reconfigure. The guidewire is moved longitudinally and rotated, continuously or continually, to sense the temperature of the hollow body organ at multiple locations.

Alternatively, the catheter may be omitted entirely from the deployment procedure. Rather than using a catheter or sheath to restrain the distal portion of the guidewire during deployment, the guidewire may simply be inserted and advanced within the hollow body organ to the tissue region of interest while in its relaxed configuration. For instance, an introducer and/or guide catheter may be positioned percutaneously through the skin into the body of a patient and the guidewire may simply be inserted without the use of a separate catheter directly into, e.g., the vasculature, via the introducer. During insertion, the guidewire may be inserted into the body while the probe is in its relaxed configuration. Except when initially introduced or withdrawn through the introducer into the body, the probe may remain in its relaxed configuration.

In accordance with yet another aspect of the present invention, the probe or guidewire includes a hollow, flexible, elongate stem having proximal and mid portions and a distal end portion which terminates in a coil having at least a tip segment thereof biased away from the rotational axis of the probe at an angle between approximately 30° to 75° relative to the stem longitudinal axis, and more preferably between approximately 40° to 60°, and having a torque response of no more than about 0.4 ozf in. Moreover, a transducer is mounted to the coil, a connector is located at the proximal end portion of the stem, and at least one conductor connects the transducer to the connector. An elongate mandrel having a bent tip extends through the coil and provides the coil with its bent configuration.

The probe may be configured such that the coil rotates about the proximal end portion of the stem in response to the rotation of an actuation shaft extending through the proximal end portion of the stem. The proximal end portion of the stem can also define a sheath slidable on the actuation shaft and operably coupled to the coil for allowing the axial reciprocal movement of the coil. An actuator may surround the proximal end portion of the stem and be adapted to provide both rotational and axial or longitudinal movement to the stem to allow the sensor to travel in a helical path through the desired body organ.

Moreover, and depending upon the particular desired application, the materials and/or shapes of the proximal, mid and distal end portions of the stem may be varied to provide a flexural rigidity ratio between the coil and the mid portion and the proximal end portion in the range of about 1:(4 to 4,400):(110 to 13,000), respectively, and more preferably 1:400:1200, respectively.

To ensure contact between the probe and the vessel wall, various impedance measurement devices or sensors may also be provided in addition to the thermal sensors or transducers mounted in the tip segment.

The actuator which controls the rotational and axial movement of the probe may be constructed as a handle. The probe may be attached via an optionally removable chuck to the handle and both the chuck and the probe may be electrically connected to an amplifier positioned within the handle. The amplifier is preferably configured to rotate while maintaining electrical contact with the probe. Moreover, various motors under the control of a motor controller, are used to control both the rotational and axial movement of the probe. A processor, e.g., a computer, is used to not only track/control the positioning and movement of the probe, but is also used to process the signals acquired by the probe. During the measurement or scanning process, the rate and pitch at which the vessel walls are scanned may be automatically varied by the processor to increase the measured sampling resolution upon the determination of a threshold measurement value being exceeded.

While the processor and/or controller may be used to control the movement of the probe, an alternative embodiment may incorporate an intervening chuck and connector cable to allow for the manual manipulation of the probe. This embodiment utilizes a separate chuck which is used to receive the probe. The chuck may then be connected to the probe actuator via the connector cable. During normal operation, the intervening chuck and connector cable may remain attached to the probe actuator or they may be connected when manual manipulation is desired. To accomplish the manipulation, the physician or surgeon may simply rotate and/or axially move the probe via the intervening chuck while maintaining the sterility of the probe and probe actuator. Alternatively, the intervening chuck may be omitted altogether and the probe may simply be attached to a connector cable which is configured to directly receive the probe connector.

Further aspects and advantages of the present invention are apparent from the following description of the preferred embodiments referring to the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

In the drawings,

FIG. 1 is a perspective view of an embodiment of the present invention;

FIG. 2 is a longitudinal sectional view of an arterial hollow body organ in which the embodiment of FIG. 1, also shown in longitudinal section, is deployed;

FIG. 3A is a longitudinal sectional view of a guidewire probe variation in which the sensor is positioned off-center or off-axis;

FIG. 3B is a cross-sectioned detail view of the probe of FIG. 3A;

FIG. 4A is a longitudinal sectional view showing an example of a mapping or scanning path in which the rotational and withdrawal rates are constant;

FIG. 4B is a longitudinal sectional view showing an example of a mapping or scanning path in which the rotational and/or withdrawal rates may be varied to provide for regions of higher and lower measurement resolution;

FIG. 5 is a longitudinal sectional view of an arterial hollow body organ in which another preferred embodiment of the present invention, also shown in longitudinal section, is deployed;

FIG. 6 is a perspective view of yet another preferred embodiment of the present invention;

FIG. 7 is a perspective view, partially in section, of a further preferred embodiment of the present invention;

FIG. 8 is a perspective view of yet another preferred embodiment of the present invention;

FIG. 9 is a longitudinal sectional view of an arterial hollow body organ in which another preferred embodiment of the present invention, shown in perspective, is deployed;

FIG. 10 is a perspective view of a further preferred embodiment of the present invention;

FIG. 11 is a longitudinal sectional view showing another variation of a guidewire having at least two bends;

FIG. 12 is a longitudinal sectional view showing another variation of a guidewire having multiple bends and at least two sensors;

FIGS. 13A and 13B are longitudinal views showing alternative embodiments in which a guidewire probe may be reconfigured by active actuation into a shape having a bend portion;

FIGS. 14A and 14B are longitudinal views showing alternative embodiments in which a guidewire probe may be reconfigured by active actuation into a shape having a radially extended portion;

FIGS. 15A and 15B are longitudinal views showing alternative embodiments in which a guidewire probe may be reconfigured by active actuation into a shape having at least two bend portions;

FIG. 16 is a longitudinal view showing another embodiment in which guidewire probe may have at least two radially extended probes linearly spaced apart from one another;

FIG. 17 is a perspective view of another preferred embodiment of the present invention;

FIG. 18 is a longitudinal sectional view of an arterial hollow body organ in which yet another preferred embodiment of the present invention, shown in perspective, is deployed;

FIG. 19 is a longitudinal sectional view showing a variation in which impedance measurements may be taken to determine whether sufficient contact exists between the guidewire and the vessel wall;

FIG. 20 is a detailed view of the probe of FIG. 19 showing a variation on the dual-sensor location;

FIG. 21A is a perspective view of another device embodiment of the present invention;

FIG. 21B is a schematic representation of a variation of a signal processor and controller connected to a probe actuator;

FIG. 22 is an exploded, broken perspective view of the probe of the device of FIG. 21A;

FIG. 23 is an exploded, broken perspective view of an alternate embodiment of the probe of the device of FIG. 21A;

FIG. 24 is an exploded, broken perspective view of yet another alternate embodiment of the probe of the device of FIG. 21A;

FIG. 25A is a cross-sectioned perspective view of a proximal end of a probe;

FIG. 25B is a side view of a variation on the probe in which the connector region is positioned near the mid-section of the wire;

FIG. 26 is a schematic illustration of one variation of an actuator assembly which may be used to provide the rotational and axial movement for the probe;

FIG. 27 is a side view of one embodiment of the probe actuator with the cover partially removed;

FIG. 28 is a perspective view of the probe actuator of FIG. 27 with some components removed for clarity;

FIG. 29 is a perspective view of an alternate embodiment of the probe actuator with the cover partially removed;

FIG. 30A is a side view of an embodiment of the probe chuck;

FIG. 30B is an electrical schematic showing one variation of the chuck from FIG. 30A which may be self-calibrated;

FIGS. 31A and 31B are perspective and end views, respectively, of an embodiment of a rotatable amplifier; and

FIG. 32 is a perspective view of an alternate embodiment having a manually manipulatable assembly.

DETAILED DESCRIPTION OF THE INVENTION

FIG. 1 shows a device 10 for profiling the wall of a hollow body organ. Device 10 includes a lumened catheter 12 having a central lumen 14, a hollow guidewire 16 that defines a conduit comprising a metal wire 18 or the like in the shape of a coil defining a central lumen (not shown), and a thermal sensor 20 disposed at the terminal end of the distal portion of guidewire 16. Conventional conductors or other signal carrying structures (not shown) are provided to convey signals from the thermal sensor 20 along guidewire 16 and out of the proximal portion of guidewire 16 for connection to appropriate signal processing apparatus that converts the signals to a temperature indication. Thermal sensor 20 can be, e.g., a thermocouple, a thermistor, an infrared radiation sensor, fiberoptic oxygen sensor, ultrasonic transducer, impedance sensor, pH sensor, mechanical force sensor (e.g., strain gauge), etc., for example, and is secured by appropriate mechanical or adhesive means to the terminal end of guidewire 16. Moreover, radio-opaque materials, e.g., platinum, gold, etc., may be formed in epoxy materials which may be used to attach sensor 20 to guidewire 16. Alternatively, one or several radio-opaque marker bands 19, preferably made of biocompatible materials such as those listed above, may be formed proximally of sensor 20 along guidewire 16 to assist in denoting the location of sensor 20 during a measurement procedure. Typical thermocouples which can be used may include T-type thermocouples (Copper and Constantan) having thermoelectric conversion coefficients of about 40.3 $\mu\text{V}/^\circ\text{C}$.

Hollow guidewire 16 is made of thin wire 18 wound, for example around a mandrel, into small helical coils of desired diameter that lie tightly adjacent one another to form a

hollow tube having a central passageway or lumen there-through. Guidewire 16 may have an outer diameter which is uniform along its length; alternatively, the diameter may be varied, e.g., having diameter decrease proximally along the length of guidewire 16 or having sections of differing guidewire 16 diameters along the length. Guidewire 16 has an outer diameter somewhat less than the inner diameter of catheter 12 to permit guidewire 16 to slide freely within the lumen 14 of catheter 12. In addition, guidewire 16, in its relaxed configuration, is shaped in the form of a bend 22 at the distal portion thereof, the bend 22 being spaced from the terminal end of guidewire 16 at which thermal sensor 20 is disposed. Consequently, thermal sensor 20 is displaced radially from the longitudinal axis 24 of guidewire 16 and catheter 12 when guidewire 16 is in the relaxed, bent configuration. Through external manipulation, guidewire 16 in the relaxed, bent configuration can be made to rotate about axis 24, continuously or continually, depending on the response time for the sensor, thereby causing thermal sensor 20 to traverse a circumferential or helical path about axis 24 while providing temperature information. Guidewire 16 can be deformed elastically into a substantially straight configuration, i.e., without bend 22, under force. When the force is removed, guidewire 16 returns to the relaxed, bent configuration.

Guidewire 16 can be constructed of spring steel that can be deformed into a relatively straight configuration when withdrawn into catheter 12, but which springs back to its bent configuration when extruded from catheter 12 and released from constraint. Another way is to construct guidewire 16 of superelastic nitinol and take advantage of the martensitic transformation properties of nitinol. Guidewire 16 can be inserted into catheter 12 in its straight form and kept cool within the catheter by the injection of cold saline through catheter 12 and over guidewire 16. Upon release of guidewire 16 into the bloodstream, it will warm up and change to its austenite memory shape based on the well-known martensitic transformation by application of heat and putting the material through its transformation temperature.

Guidewire 16 can also be made out of a composite such as a nitinol tube within the guidewire structure. In this fashion, the martensitic or superelastic properties of nitinol can be combined with the spring steel characteristics of the spring and lead to a desirable composition. Other suitable materials for guidewire 16 include copper, constantin, chromel or alumel.

FIG. 2 shows device 10 deployed in a hollow body organ comprising an arterial blood vessel 26 having an endothelium 28 forming the inner wall thereof. Only the distal portion of guidewire 16 that extends beyond catheter 12 is shown. Electrical conductors 32 extend through lumen 30 of guidewire 16. Conductor 32 is electrically insulated from the coils 18 of guidewire 16 so that guidewire 16 comprises one conductor and conductor 32 comprises another conductor or lead of the thermal sensor 20 which can be a thermocouple or thermistor. The conductors convey signals from the thermal sensor 20 to the proximal end of guidewire 16 for connection to appropriate signal processing apparatus that converts the received signals to a temperature indication.

Although thermal sensor 20 is shown as extending along the center of the distal end of guidewire 16, sensor 20 is preferably positioned off-center or off-axis from the longitudinal axis of the guidewire. As shown in FIG. 3A, as guidewire 11 traverses along wall 28 within vessel 26, a lesion or obstruction 13 may force distal portion 23 to bend radially inward towards the longitudinal axis along bend 22.

Placement of thermal sensor **21** off-axis may allow for continuous contact and/or sensing between sensor **21** and wall **28** or lesion **13** despite having the center tip of distal portion **23** bent inwardly. FIG. 3B shows a cross-sectioned detail view of distal portion **23** where sensor **21**, connected to conductors **27**, is positioned off-axis near the distal tip.

In one use, the guidewire **16** and thermal sensor **20** of device **10**, as shown in FIGS. 1 and 2, are inserted into the lumen **14** of catheter **12** from the proximal end, thereby constraining guidewire **16** in a substantially straight configuration with the thermal sensor **20** near the distal end of catheter **12**. Using conventional percutaneous insertion techniques, access to the blood vessel **26** is obtained surgically. Catheter **12**, with guidewire **16** and thermal sensor **20** disposed within, is advanced through the blood vessel **26** to the region of interest.

Catheter **12** is slowly withdrawn while guidewire **16** is secured against movement relative to the patient such that guidewire **16** emerges from the distal end of catheter **12** and reverts to the relaxed, bent configuration within the blood vessel **26**. Alternatively, catheter **12** may be secured against movement relative to the patient and guidewire **16** may be advanced distally until it emerges from the distal end of catheter **12**. Guidewire **16** remains substantially fixed in the axial direction relative to the blood vessel **26** as catheter **12** is withdrawn, with the re-formed bent distal portion of guidewire **16** springing gently radially outwardly into contact with the vessel wall **28**.

In another use, catheter **12** may be omitted entirely from the deployment procedure. Rather, guidewire **16** may simply be inserted into the patient while in its relaxed configuration and advanced within the hollow body organ to the tissue region of interest. With catheter **12** omitted, the guidewire **16** may be advanced in its relaxed configuration, as mentioned, or it may be inserted within the patient in its substantially straightened configuration and be allowed to reconfigure itself by heating up while being advanced.

With guidewire **16** exposed and thermal sensor **20** lying in contact with the wall **28** of blood vessel **26**, the thermal sensor **20** senses the localized temperature of the vessel wall **26** at the region where the thermal sensor **20** is situated. By slowly withdrawing guidewire **16**, either into catheter **12** or simply withdrawing distally, while simultaneously rotating guidewire **16** about its longitudinal axis, thermal sensor **25** can be made to traverse a helical path around the inner wall **28** of the blood vessel **26**, permitting temperature measurements to be taken at intervals of different regions of the vessel wall **28**. Depending upon the response time of thermal sensor **20**, which is preferably on the order of milliseconds, e.g., between 10 to 100 msec. and preferably less than 50 msec., rotation can be intermittent or continuous, as needed. By withdrawing and rotating the guidewire **16** at constant rates, e.g., at a scanning rate of about 50 mm/min with a linear or pull-back rate of between 0.3 to 10 mm/sec. and preferably 1 mm/sec. and at a rotational rate of between 1 to 100 rpm, and preferably between 10 to 100 rpm, and more preferably about 25 rpm, the location of the thermal sensor **20** relative to the distal end of the catheter **12** can be determined as a function of time, so that a temperature profile of the blood vessel **26** can be mapped, provided the response time of the thermal sensor is relatively short.

One variation of a mapping procedure is shown in FIG. 4A where the rotational and withdrawal rates are maintained constant. The mapping or scanning path **29**, i.e., the path traced by sensor **21** against vessel wall **28** as guidewire **11** is rotated and withdrawn, may be formed at a uniform rate.

To provide higher resolution measurements, the pitch of mapping or scanning path **29** may be tightened or shortened to provide for closer measurement readings, thereby producing a higher resolution profile. Yet to optimize the scanning profile and minimize the time involved in profiling a region of tissue, the device may be configured to automatically provide for lower resolution readings in non-critical areas and higher resolution readings in critical areas, e.g., where the temperature readings are elevated. One method of configuring the device may be to detect when a threshold temperature difference value between set variables, e.g., 0.05° to 0.5° C., is detected. When this threshold difference value is exceeded, this may be an indication of a lesion present within the tissue and the scanning path **29** of guidewire **11** may accordingly be tightened to produce the higher resolution profile.

For example, during a mapping procedure as shown in FIG. 4B, the guidewire **11** may be rotated and withdrawn at an initial constant pitch. During this sensing period, scanning path **29** may provide for a relatively lower resolution temperature profile along region **31**. When a temperature of the vessel wall **28** is measured by sensor **21** to exceed the predetermined threshold temperature difference, the pitch of scanning path **29** may be automatically reduced via a connected processor to produce the tightened scanning profile and thereby result in a higher resolution along region **33**. As the scanning path **29** progresses, once the measured or sensed temperature difference value falls below the preselected threshold value, guidewire **11** may be configured to then automatically resume a lower resolution profile, as seen along region **35**.

Once the mapping is completed, the guidewire **16** may be withdrawn fully into catheter **12**, re-sheathed and constrained in a substantially straight configuration, if catheter **12** is utilized. Catheter **12** or guidewire **16** alone can then either be withdrawn from the blood vessel **26** or repositioned to another region of interest within the hollow body organ for further mapping of the temperature profile at that region.

FIG. 5 shows a second preferred embodiment of a device **10'** for profiling the wall of a hollow body organ. Device **10'** can be deployed in a hollow body organ in a manner similar to the embodiment of device **10** shown in FIGS. 1 and 2 and described above with respect to structure and use. Components of device **10'** that are similar in structure and function to corresponding components of device **10** of FIGS. 1 and 2 are designated by like primed numerals. The description of device **10** above applies also to device **10'** unless described otherwise below.

Device **10'** includes a second thermal sensor **36** disposed at the outside of bend **22'** and exposed for contact with the inner wall **28'** of vessel **26'**. A second electrical conductor **38** is electrically insulated the conductor **32'** and from the wire **18'** of guidewire **16'** so that guidewire **16'** comprises one conductor and conductor **38** comprises another conductor of the thermocouple or thermistor of thermal sensor **36** for conveying signals from the thermal sensor **36** to the proximal end of guidewire **16** for connection to appropriate signal processing apparatus that converts the signals to a temperature indication. Wire **18'** of guidewire **16'** is a conductor common to thermal sensors **20'** and **36**.

Device **10'** of FIG. 5 can be used in a manner substantially similar to the manner of use described above with respect to the devices above, except that thermistors **20'** and **38** simultaneously traverse intertwined helical paths in contact with the inner wall **28'** of hollow body organ **26'**. Consequently, the temperature profile of the inner wall **28'** can be mapped

more quickly because data can be gathered from different locations simultaneously.

FIG. 6 shows yet another preferred embodiment of a device 210 for profiling the wall temperature of a hollow body organ. Device 210 can be deployed in a hollow body organ in the manner described above with respect to the embodiments described above. Components of device 210 that are similar in structure and function to corresponding components of the devices above are designated by like reference numerals in the 200 series but having the same last two digits. The description of device 10 above applies also to device 210 unless described otherwise below.

Device 210 of FIG. 6 includes one thermal sensor 40 disposed at the outside of a dogleg bend 42 that is spaced distally from bend 222 and from the terminal end of guidewire 216. Thermal sensor 40 is exposed for contact with the inner wall 228 of vessel 226. An electrical conductor (not shown) is electrically insulated from the wire 218 of guidewire 216 so that guidewire 216 comprises one conductor and the electrical conductor comprises another conductor of the thermocouple or thermistor of thermal sensor 40 for conveying signals from the thermal sensor 40 to the proximal end of guidewire 216 for connection to appropriate signal processing apparatus that converts the signals to a temperature indication. Unlike the embodiments of the devices of FIGS. 1 to 5, device 210 includes only a thermistor at bend 42 and no thermistor at the terminal end of guidewire 216 or at bend 222.

Device 210 of FIG. 6 can be used in a manner substantially similar to the manner of use described above with respect to the devices of FIGS. 1 to 5.

FIG. 7 shows a further preferred embodiment of a device 310 for profiling the wall temperature of a hollow body organ. Device 310 can be deployed in a hollow body organ in the manner described above with respect to the embodiments of the devices described above. Components of device 310 that are similar in structure and function to corresponding components of the above-described devices are designated by like reference numerals. The description of device 10 above applies also to device 310 unless described otherwise below.

Device 310 of FIG. 7, rather than having externally exposed thermal sensors as in the embodiments above, includes a thermal sensor 50 disposed within the lumen 330 of hollow guidewire 316 and in thermal contact with the coiled wire 318 that comprises guidewire 316. Thermal sensor 50 is located at bend 52 that is spaced between bend 322 and the distal end of guidewire 316. Guidewire 316 also includes bend 54 between bend 52 and the distal end of guidewire 316. Bends 322, 52 and 54 together cause the distal portion of guidewire 316 to assume the shape of a question mark when in a relaxed configuration. In such a configuration, bend 52 and bend 54 contact opposite sides of the inner wall of the hollow body organ. The spring nature of guidewire 316 urges bend 52 in contact with the hollow body organ. Insulated electrical conductors 56 and 58 are operatively connected to the thermocouple or thermistor of thermal sensor 50 for conveying signals from the thermal sensor 50 to the proximal end of guidewire 316 for connection to appropriate signal processing apparatus that converts the signals to a temperature indication.

Device 310 of FIG. 7 can be used in a manner substantially similar to the manner of use described above with respect to the devices.

FIG. 8 shows another embodiment of a device 410 for profiling the wall temperature of a hollow body organ.

Device 410 is an alternative configuration of the device 310 of FIG. 7, in which bend 454 extends in a direction opposite to that of bend 54, such that the terminal end portion of guidewire 416 extends axially away from catheter 412. Bend 454 serves a purpose similar to that of bend 54 of device 310 of FIG. 7, i.e., to assure that bend 452, at which thermal sensor 450 is located, remains in contact with the inner wall of the hollow body organ when deployed therein.

FIG. 9 shows yet another embodiment of the present invention. Temperature sensing device 510 is carried by hollow guidewire 516 which extends outwardly from the distal end of catheter 512 and includes thermal sensor 550, e.g., a thermistor at bend 552 spaced from bend 522 which is situated between the sensor-carrying bend 552 and the distal end portion of catheter 512. The distal end portion of guide wire 516 terminates in a generally crescent-shaped loop and is rotatable, continuously or continually, as desired, to sense the temperature of the endothelium 528 lining the wall of blood vessel 526 in the vicinity of plaque deposit 592.

FIG. 10 shows a further embodiment of a device 610 for profiling the wall temperature of a hollow body organ. Device 610 comprises another alternative configuration of the device 310 of FIG. 7, in which guidewire 616 is shaped as a plurality of loops 60 with a plurality of thermal sensors 62 located within guidewire 616 at each location along the loops 60 that would contact the wall of the hollow body organ when disposed therein.

FIG. 11 shows another embodiment of guidewire 618 which has two bends disposed within vessel 26. Guidewire 618 may be formed into a device which is configured to securely place the distal sensing tip against vessel wall 28. A contact region 621 is formed between guidewire 618 and vessel wall 28 by first bend 619. Guidewire 619 may then be configured with second bend 620 to extend sensor 622 against wall 28. With this variation, sensor 622 may be placed securely against wall 28 during rotation and withdrawal.

FIG. 12 shows a similar variation in guidewire 623 which may form first and second contact regions 624, 625 between first and second sensors 626, 627, respectively, against vessel wall 28. This variation may have at least two sensors 626, 627 formed to simultaneously detect opposite sides of wall 28 during a sensing procedure. This configuration may also allow for guidewire 623 to ensure contact between wall 28 and sensors 626, 627 since the two opposing contact regions 624, 625 may press in opposing directions against wall 28 with a gentle force.

The following FIGS. 13A to 15B show alternative embodiments in which the guidewire probes may be configured to form their sensing configurations by active actuation alone or in addition to any reshaping which may occur by shape memory characteristics of the guidewires. As seen in FIGS. 13A and 13B, guidewire 628 may be formed in a straightened configuration with sensor 629 positioned at some location proximal of the distal tip. Pullwire 630 may be disposed within guidewire 628 along its length and exposed exteriorly of guidewire 628 between exit port 631 and anchor region 632. Sensor 629 is preferably positioned along guidewire 628 near the center portion between exit port 631 and anchor region 632. Guidewire 628 may be inserted into, e.g., the vasculature, in its straightened configuration and placed near the tissue region to be examined. Prior to examination, pullwire 630 may be pulled at its proximal end, preferably manipulated outside the body of the patient, such that a bend portion 633 is formed between

exit port **631** and anchor region **632**. As bend portion **633** is formed, sensor **629** is preferably extended radially relative to the longitudinal axis of guidewire **628** such that contact between sensor **629** and the vessel wall may occur. To help ensure that sensor **629** is extended on the outer curvature of bend portion **633**, exit port **631** and anchor region **632** are preferably defined on guidewire **628** opposite to where sensor **629** is located.

FIGS. **14A** and **14B** show another alternative embodiment in guidewire **634**. Sensor **635** may be located near or at the distal end of guidewire **634** and pullwire **636** may be disposed within the length of guidewire **634** and anchored at anchor region **637** proximally of sensor **635**. Prior to examination of the tissue region of interest, pullwire **636** may be manipulated to reconfigure the distal end of guidewire **634** to radially extend at bend region **638**. At the end of the examination procedure, pullwire **636** may be relaxed and guidewire **634** may also be relaxed to reconfigure into its straightened shape.

FIGS. **15A** and **15B** show an embodiment which is similar to that shown in FIG. **12** above. Guidewire **639** may be formed to have at least two sensors **640** spaced apart relative to one another along guidewire **639**. Pullwire **641** may be disposed within the length of guidewire **639** and exposed exteriorly preferably between exit ports **642** and anchored to guidewire **639** at anchor region **643**. As above, sensors **640** are preferably located near the central portions between the exit ports **642** and anchor region **643** and pullwire **641** is preferably located along guidewire **639** oppositely of sensors **640**. Prior to examination, pullwire **641** may similarly be manipulated at its proximal end to reconfigure guidewire **639** into first and second bend regions **644**, **645**, respectively. Sensors **640** are preferably located along the outer curvatures of bend regions **644**, **645** so guidewire **639** may undergo a torquing about its longitudinal axis to align sensors **640** accordingly as pullwire **641** is pulled.

FIG. **16** shows another alternative embodiment in guidewire **646** which has linearly spaced probes separated by a distance D . As shown, first probe **647** has a distally located first sensor **649** at a first distance or radius R_1 relative to the guidewire **646** longitudinal axis and second probe **648** has a distally located second sensor **650** at a second distance R_2 . Although this embodiment shows two probes, any number of linearly spaced probes may be used as practicable. Probes **647**, **648** are preferably parallel with one another to ensure complete coverage during the scanning process, but they may alternatively be located at various angles relative to one another in the same plane or within different plane depending upon the desired configuration and application. The distance D between the probes **647**, **648** may also be varied depending upon the desired coverage during scanning. Moreover, the radii may likewise be varied to suit the application. For instance, the radii shown has $R_1=R_2$; however, they may be varied such that $R_1<R_2$ or $R_1>R_2$ depending upon the scanning profile and the geometry of the tissue to be examined.

FIG. **17** shows yet another embodiment of a device **710** for profiling the wall temperature of a hollow body organ. Device **710** includes a lumened catheter **712** and a hollow guidewire **716**. The inner surface of lumen **730** of guidewire **716**, at a bend **742** similar to bend **42** of device **210** of FIG. **6**, is lined with a layer of black paint **70** which is in turn lined with a thermochromic material **72** that is sensitive to a change of temperature of the guidewire **716**. The color of the thermochromic material **716** varies as a function of temperature.

Disposed within lumen **730** of guidewire **716**, inwardly of thermochromic material **72**, is an optical probe **74** including

an illuminating optical fiber **76** having a radially emitting diffuser **78** at the distal end thereof, and a sensing optical fiber **80** having a conically beveled distal end **82** for collecting light. An illuminating electromagnetic radiation source connected to the proximal end of illuminating optical fiber **76** provides illuminating radiation that is guided by optical fiber **76** to the region of interest within the hollow body organ, and diffused radially by diffuser **78** to illuminate the interior of lumen **730**, particularly thermochromic material **72**. The illuminating radiation can be in the visible, infrared or ultraviolet portions of the spectrum. Radiation from diffuser **78** is differentially absorbed and reflected by thermochromic material **72**, according to the color of material **72** which is indicative of the temperature of guidewire **716** in contact with the wall of the hollow body organ in the region of interest.

The light reflected from thermochromic material **72**, having wavelengths indicative of the color thereof, is collected by distal end **82** and directed toward the proximal end of sensing optical fiber **80**. An appropriate optical reflectance spectrometry device connected to the proximal end of sensing optical fiber **80** generates an electrical signal indicative of the color, and therefore temperature, of thermochromic material **72**.

FIG. **18** shows yet another embodiment of a device **810** suitable for profiling the impedance of the wall of a hollow body organ. Device **810** includes a catheter **812** within which is disposed a guidewire **816** having a bend in the distal portion thereof. Device **810** is similar in configuration to the embodiment of device **210** of FIG. **6**, and like components are indicated by like reference numerals in the **800** series but having the same last two digits. Unlike device **210** of FIG. **6**, device **810** does not employ thermal sensing, but rather employs impedance sensing for profiling the wall of a hollow body organ. An electrode **90** at the outside of the bend of guidewire **816** is in electrical contact with guidewire **816** and in electrical contact with the inner wall **828** of the hollow body organ **826**. Guidewire **816** comprises a conductor operatively connected to an external impedance measuring device that has a ground terminal electrically connected to the body in which the hollow body organ is located. A small electrical current is applied via guidewire **816** and electrode **90** to the inner wall **828** at the region of contact therebetween. The impedance of the electrical path through the body, including through the region of interest in the hollow body organ **826**, can be measured and recorded. By moving guidewire **816** relative to the hollow body organ **826** as described above with respect to other embodiments, the impedance of the wall of the vessel **826** can be mapped. Any change of impedance along the wall **828** indicates the presence of an anomaly in the wall, such as a plaque **92**.

Aside from detecting anomalies in the wall of the vessel, impedance measurements may also be used to provide real-time feedback for contact between the guidewire probe and the vessel wall. For instance, when the impedance value rises above a preselected threshold, this may be an indication of lost contact against the vessel wall **828** since the surrounding fluids, e.g., blood, and/or tissue will likely have a higher impedance than the tissue being examined. One variation using impedance measurements for ensuring contact against the vessel wall is shown in FIGS. **19** and **20**. Similarly to FIG. **18** above, contact between guidewire **830** and plaque **92** or inner wall **828** may be ensured by monitoring the measured impedance. In this variation, an impedance sensor **831** may be disposed within the distal tip of guidewire **830** in communication with power source **834** via connection **833**. Connection **833** may be any conventional

electrical conductor or optical fiber if optical sensors are utilized. Power source **834** may be any type of power supply preferably capable of generating AC power.

In operation, a first voltage may be applied through the body or vessel **826**, which is typically connected to electrical ground **832** either directly through, e.g., grounding straps, or indirectly through natural contact via the body of the patient. This first voltage, V_1 , may be measured at voltage measurement location **835** and the resulting first current, I_1 , may be measured at current measurement location **836**, which is preferably taken between power source **834** and electrical ground **837**. A second voltage at a second current may be applied through the body or vessel **826** and the resulting voltage, V_2 , and current, I_2 , may be measured at voltage and current measurement locations **835**, **836**, respectively. The ratio between the differences of the respective voltages and currents can then be calculated to give an impedance value, i.e., impedance $Z = \Delta V / \Delta I = (V_1 - V_2) / (I_1 - I_2)$. If contact were maintained between impedance sensor **831** and plaque **92** or vessel wall **828**, a consistent impedance value may be maintained and used as an indicator of contact between the two. Yet if contact were broken, then the impedance value will vary and this may be used as an indicator of lost contact between guidewire **830** and the tissue.

One detailed example of a dual-sensor probe is shown in FIG. **20** which may be used for impedance measurement. As shown, the distal end portion of guidewire **830** may have the thermal sensor **838** in the distal tip, as described above, in communication with a proximally located detector and processor via conductors **839**. A second sensor, impedance sensor **831**, may be disposed adjacent or near thermal sensor **838**, and connected via connection **833** as shown. Impedance sensor **831** may detect contact via electrical impedance, as described above, but it may also detect via alternative methods, e.g., ultrasound, infrared, laser light, electrical conductivity, etc. If impedance sensor **831** were configured to detect electrical impedance or conductivity, connection **833** will be conductors, but if sensor **831** were configured to detect via optical methods, e.g., infrared or laser light, optical fibers may accordingly be used as connection **833** to detect and transmit the optical signals. The methods for impedance detection of FIGS. **19** and **20** may be used with any of the various guidewire embodiments described herein.

FIG. **21A** shows a device embodiment **910** where a probe or guidewire **960** is adapted to be coupled to a detachable probe actuator **962** which, in turn, includes a cable **964** adapted to be coupled to a signal processing unit or the like. FIG. **21B** shows schematically an example of an overall system for temperature sensing. As seen, probe actuator **962** may be connected via cable **964** directly to either the signal processor unit **963** or to the controller **965**. The example shows the probe actuator **962** connected to controller **965**, which may be used to control and/or record the advancement or withdrawal of the motors or actuators contained within probe actuator **962** (discussed below in further detail) used for manipulating the guidewire **960**. Controller **965** may be connected via cable **967** to processor **963**, e.g., a computer, which may be used to process and display signals received from guidewire **960** as well as to control the movement of guidewire **960** within the vasculature.

Prior to temperature acquisition, the probe system is preferably calibrated. The calibration may be performed through various methods. One example includes having two separate sensors for real-time calibration directly by a patient prior to use. One sensor may be placed in an orifice, e.g., the mouth, of the patient and an offset may be added to the measured value to estimate the core body temperature.

The other sensor may be within the guidewire and used to acquire the temperature from the tissue region of interest.

Alternatively, the system may be calibrated in the factory and a programmed calibration factor may be provided to the physician or technician for final calibration prior to use by the patient. Another alternative may be to provide a calibration slug or pod **969** along with the system. Such a slug **969** may be made from a material, e.g., plastics or polymers, which may be consistently and uniformly heated or cooled to a predetermined temperature, e.g., 37° C., preferably within a protective case prior to calibration. Slug **969** is preferably configured to define a channel or station for receiving and holding the guidewire after the slug **969** has been heated to the desired temperature. The guidewire may then be calibrated prior to each use as the slug **969** may be preferably reused multiple times to generate a consistent calibration temperature.

FIG. **22** shows the structure of the probe or guidewire **960** which includes a stem **966** having a proximal end portion in the form of a hollow, elongate flexible proximal hypotube **968**, a mid portion in the form of a hollow, elongate, flexible mid hypotube **970** unitary with the tube **968**, and a distal end portion unitary with the tube **970** and being in the form of a hollow coiled end tube **972** which has a bent tip portion or segment **973** and is composed of thin wire **918** which has been wound into small helical coils in a manner similar to that described with respect to the coiled guidewire **16** of the device **10** shown in FIG. **2**. A transducer **920** is disposed within the interior of the terminal tip **973** of the distal coiled end tube **972**. As described above with reference to the device **10** of FIG. **2**, the transducer **920** can take the form of a thermal sensor such as a thermocouple, thermistor, or a radiation sensor. The transducer **920** can also, however, take the form of an instrument adapted to respond to inputs other than temperature or radiation such as, for example, displacement or force. A radiopaque marker band **975** in the tip **973** of the distal end tube **972** allows the exact location of the probe **960** to be tracked during use. Moreover, it is understood that the bent tip **973** of the distal end coiled tube **972** can be made of a material which is more radio-opaque than the material forming the remainder of the tube **972** to allow better visibility of the probe **960** as it is advanced through a blood vessel.

The distal coiled end tube **972** includes an elongate shaping mandrel **974** extending through the interior thereof generally between the distal end of the mid tube **970** and the transducer **920**. The mandrel **974** comprises an elongate strip of metal or the like material having a distal tip portion **977** bent at an angle, α , generally between 10° to 90° relative to the longitudinal axis of the stem **966**. In accordance with the preferred embodiment of the probe **960**, the distal tip portion **977** of the mandrel **974** is bent at an angle, α , generally between 30° to 70° and more preferably between 40° to 60° relative to the longitudinal axis of the stem **966**. The bent configuration of the mandrel **974** is, of course, imparted to the distal coiled end tube **972** of the stem **966**. It has also been determined that the guidewire **16** disclosed in FIG. **2** should preferably also be bent at the same angles as described above with respect to the mandrel **974**.

Although the mandrel **974** of FIG. **22** is permanently bent into its angled configuration, it is understood that the mandrel **974** can be constructed from the same types of shape memory materials described above with respect to the guidewire **16** of FIG. **2** including, for example, spring steel or superelastic nitinol, so as to allow the mandrel **974** to move between straight and bent configurations in response to, for example, a change in temperature or the withdrawal of the coiled end tube **972** from a catheter **12** as shown in FIG. **2**.

15

Although not shown in FIG. 22, it is also understood that the mandrel 974 can alternatively take the shape of any of the coils described and shown herein. Additionally, it is understood that the present invention encompasses any one of several different mandrel embodiments depending upon the desired application of the device. For example, in applications where a soft and flexible tip portion 973 is desired, the length of the mandrel 974 can be shortened such that it terminates short of the tip portion 973. Moreover, in applications where the tip portion 973 must have a particular stiffness or in applications where it would be desirable to be able to bend or flex the tip portion 973 to help direct the probe into tight openings, the distal tip 977 of the mandrel 974 can be flattened and/or made of a material different than the remainder of the mandrel 974.

A plurality of spaced-apart parallel bands or rings of electrical connectors 978 surround the proximal tube 968 adjacent the proximal terminus thereof. The connectors 978 are separated from each other by a plurality of spaced-apart parallel bands or rings of insulative material 980. In accordance with one embodiment of the invention, the rings of connectors 978 and insulative material 980 respectively are flush with the outer surface of the tube 968 to assist in the alignment of the contacts 978 with cooperating contacts (not shown) in the actuator 962. Although not shown, it is also understood that the proximal tube 968 may incorporate a reduced diameter segment defining a groove in the proximal tube 968 and that the connector rings 978 can surround the reduced diameter segment to further assist in the alignment of the contacts with cooperating contacts in the actuator 962.

Also, an elongate conductive wire 982 extends through the stem 966 between and in contact with the connectors 978 at one end and the transducer 920 at the opposite end for conveying appropriate signals from the transducer 920 to the connectors 978 and thereafter through the actuator 962 and the cable 964 and into the appropriate signal processing apparatus (not shown). An elongate strip of insulative material 984 extending through the stem 966 insulates the conductive wire 982 from the coils 918 and the tubes 968 and 970. Moreover, an elongate strip of insulative material 986 insulates the mandrel 974 from the coils 918 and the tubes 968 and 970. Another elongate strip of insulative material 988 insulates the mandrel 984 from the conductive wire 982.

FIG. 23 depicts another probe embodiment 1060 which is similar in structure to the probe 960 of FIG. 22. Components of probe or guidewire 1060 which are similar in structure and function to corresponding components of probe 960 are designated by like numerals in the 1000 series but have the same last two digits. The description of the probe 960 above applies equally to the probe 1060 unless described otherwise.

Specifically, the probe 1060 incorporates structure which allows the distal coiled tube 1072 to rotate relative to the mid-tube 1070. Particularly, the distal coiled tube 1072 is adapted to rotate about a rotary seal 1090 which separates the coiled tube 1072 from the mid-tube 1070, and the proximal and mid-tubes 1068 and 1072 respectively include an elongate actuation shaft 1092 extending therethrough and having a distal terminus (not shown) operably coupled for rotation to the proximal terminus (not shown) of the distal coiled tube 1072. Additionally, it is understood that the proximal terminus of proximal tube 1068 is adapted to be removably secured within the distal terminus of the actuator 962 shown in FIG. 21A and further that the actuator 962 incorporates motors therein (as described below) which is operably coupled to the proximal end of the shaft 1092 and

16

adapted to impart a rotary and/or linear motion thereto which, in turn, is transferred to the distal coiled tube 1072. This, of course, allows the transducer 1020 in the bent tip portion 1073 of stem 1066 to traverse a circular path around the inner wall of the blood vessel in a manner similar to that described with respect to the earlier embodiment.

FIG. 24 depicts a further probe embodiment 1160 which is similar in structure to the probes 960 and 1060. Components of probe 1160 which are similar in structure and function to corresponding components of probes 900 and 1060 are designated by like numerals in the 1100 series but having the same last two digits. The description of probes 960 and 1060 above applies equally unless described otherwise. Specifically, the stem 1166 is mounted for axial sliding back and forth movement about the actuator shaft 1192 extending therethrough. Moreover, in the probe 1160, the actuator shaft 1192 is hollow and, although not shown, it is understood that the elongate conductive wire 1182 extends through the distal coiled tube 1172 and then through the interior of the shaft 1192.

The probe 1160 also includes a plurality of spaced-apart, parallel bands or rings of electrical connectors 1178 surrounding the proximal end portion of the shaft 1192. The connectors 1178 are separated from each other by a plurality of spaced-apart parallel bands or rings of insulative material 1180. The connectors 1178 and bands of insulative material 1180 are flush with the outer surface of the rotating shaft 1192, and although not shown, it is understood that the proximal end of the conductive wire 1182 is connected to the connectors 1178.

It is understood that the probe 1160 and, more particularly, the proximal end portions of the shaft 1192 and the proximal tube 1168 are adapted to be removably fitted within the distal end of the actuator 962 (FIG. 21A) and further that the actuator 962 is adapted to incorporate, e.g., one or several motor-actuated screw drives, operably associated with the shaft 1192 and the stem 1166 to provide the combined rotational and axial probe movement which allows the transducer 1120 to traverse a helical path about the longitudinal stem axis in response to the activation of the actuator 962 to permit measurements to be taken at intervals of different regions of a vessel wall in the manner as described above with respect to the device 10 and FIG. 2.

Although not shown, it is also understood that each of the probe or guidewire embodiments described herein must be sufficiently flexible to be insertable within, for example, a blood vessel through a femoral artery access introducer and threaded into the coronary arteries and further that the various probe and guidewire embodiments must also have sufficient rigidity to ensure the rotation of the distal coiled tubes thereof in response to the rotation of the proximal end tubes thereof. In addition, the various probe and guidewire embodiments must provide support, i.e., directional control, for a catheter such as the catheter 12 shown in FIG. 2.

For example, because the balance between flexibility and rigidity is important to the effective operation of the various probe embodiments, it has been determined that the probe and guidewire embodiments herein should preferably be constructed such that the bent distal coiled end tubes thereof preferably incorporate a torque response of no more than about 0.4 ounce force inches (ozf in), and more preferably no more than 0.3 ozf in, in response to the torque which is applied to the proximal end tubes of the respective probe and guidewire embodiments. This particular distal coiled end tube torque response can be achieved by varying the profile and/or material and/or coating of any one of the tube sections or the mandrel.

Additionally, the stiffness or flexibility of the various guidewire or probe embodiments can be adjusted or varied also by changing the shape, profile and/or material of any one of the tube sections or mandrel. Depending upon the desired performance requirements, the tubes **968** and **970** of the device **910** may, for example, be made from either nitinol or stainless steel and the tube **972** can be shaped into either a flat ribbon or a flat wide ribbon to obtain the desired stiffness ratio.

For example, where a probe **910** with a soft and flexible coiled distal end tube **972** is desired, it has been determined that the tubes **968**, **970** and **972** should be of a shape and/or material resulting in a relative stiffness ratio between the distal coiled tube **972**, the mid-tube **970**, and the proximal tube **968** of about 1:4,400:13,000, respectively. It has also been determined that in applications where a probe with a stiff distal coiled tube is desired, the tubes **968**, **970** and **972** should have such a shape and/or be constructed of such material sufficient to provide a ratio of about 1:4:110 between the distal, mid and proximal tubes **968**, **970**, and **972**, respectively. Moreover, testing has revealed that the preferred stiffness ratio between the respective distal, mid and proximal tubes forming the probe should be about 1:400:1200 to provide the desired distal end coiled tube torque response of no more than about 0.4 ounce force inches.

An example of the proximal end of a probe or guidewire, as shown in the various embodiments of FIGS. 22–24, is shown in FIG. 25A. The proximal end of the probe, which has been cross-sectioned for clarity, preferably comprises a connector assembly **2000** which comprises shaft **2002** having multiple contacts near the proximal end, e.g., proximal contact **2006** and distal contact **2008**, which may be separated by indexing grooves **2004**.

The sensor leads **2012** which extend down shaft **2002** to the sensor at the distal coiled tube, preferably terminate at each respective contact **2006**, **2008**. The proximal ends of the sensor leads **2012** may be electrically separated by any conventional insulative coating **2010** which may extend into indexing grooves **2004** to maintain the electrical separation. Indexing grooves **2004** may be formed such that they are non-coextensive with an outer surface of shaft **2002**, i.e., grooves **2004** are formed such that they have diameters which are different, e.g., preferably less in diameter, than a diameter of shaft **2002**. The probe may further extend proximally with a proximal extension **2014** to any desired length.

Proximal extension **2014** may be extended a short distance as shown in FIGS. 22–24. However, another embodiment of the connector may include a probe having a length much longer than the lengths as shown in the figures above. As seen in FIG. 25B, probe **2016** may have a length with a mid-portion **2019** within which contacts **2017** and insulation **2018** may be situated. Contacts **2017** may be placed along the probe **2016** away from either the distal or proximal ends, and preferably near or at the mid-portion **2019** of probe **2016**. Placement of the contacts **2017** within mid-portion **2019** may then allow for a probe **2016** having a length much longer, e.g., twice the normal length, than a length typically used. The additional length may then allow for the use of rapid-exchange type catheters to be guided over the body of probe **2016** for advancement through the vasculature.

Probe actuator **962**, discussed above, may not only provide for rotational movement of the guidewire probe, but it may also provide for longitudinal movement. A schematic illustration of a variation of actuator **2080** is shown in FIG.

26. Rail guide or frame **2081** may provide an internal frame for supporting the various components within the handle of actuator **962**. At a distal end of frame **2081**, rotational shaft **2083** may be supported through interface **2082**. Chuck **2024**, to which probe **2026** may be connected, may be rotatably connected to the distal end of rotational shaft **2083**. The proximal end of rotational shaft **2083** may be connected to motor **2034**, e.g., DC motor, which may provide the rotational torquing force to rotate chuck **2024** and probe **2026** about its longitudinal axis through, e.g., a pulley and cable assembly **2084**, rotational gear assemblies, worm screw assemblies, etc.

At a proximal end of frame **2081**, a second motor, e.g., stepper motor **2032**, may be rotatably connected via coupler **2087** to lead screw **2086**, or any other device which can translate rotational motion into linear motion, e.g., worm screw assemblies, rack or internal gear and pinion assemblies, etc. Coupler **2087** may comprise any conventional coupling device which can transmit the rotational torque from a motor with minimal loss to another device such as lead screw **2086**. A carriage assembly **2085** which is preferably connected to a proximal end of frame **2081** is preferably configured to receive lead screw **2086**. Lead screw **2086** is preferably received through carriage **2085** within a threaded hole such that rotation of lead screw **2086** in a first rotational direction translates carriage **2085** and frame **2081** in a first linear direction and rotation of lead screw **2086** in a second opposite rotational direction translates carriage **2085** and frame **2081** in a second opposite linear direction. Thus, a controlled linear motion of probe **2026** may be provided by controlled rotation of motor **2032**. Control of motors **2032**, **2034** may be provided by a processor and/or controller as described above.

Although the actuators are shown as motors, e.g., DC or stepper motors, alternative actuators may include any type of practicable device which can be used to convert mechanical energy into rotational or longitudinal motion for the probes. For instance, screws or thumbscrews may be used to manually impart motion to the probe and guidewire apparatus. Alternatively, lead screw **2086**, rotational shaft **2083**, or chuck **2024**, or any other component, may be manually manipulated to actuate movement of the probe without having to resort to the use of motors.

FIGS. 27 to 29 show various embodiments which may incorporate actuator variation **2080**, or various embodiments thereof, to effect motion. Various features may be omitted from the figures only for clarity. FIG. 27 shows a side view of one variation on probe actuator **2020** with the cover removed for clarity. Probe actuator **2020** comprises handle **2022** having an optionally detachable probe or guidewire chuck **2024**. Guidewire chuck **2024**, which is discussed in further detail below, is configured for mechanically and electrically receiving the proximal connection end of probe **2026** and chuck **2024** itself is in electrical communication with amplifier **2028**. Probe **2026** is configured to rotate about its longitudinal axis, and accordingly, chuck **2024** is also configured to rotate about its longitudinal axis. Because chuck **2024** rotates, amplifier **2028** is also configured to rotate about the same axis as chuck **2024** while remaining in electrical contact to receive the signals from sensor leads **2012** during probe **2026** rotation.

As amplifier **2028** rotates, it is preferably electrically attached to a non-rotating platform **2030** having a plurality of concentric contacts for transmitting the signals to an externally located processor, e.g., processor **963** in FIG. 21B. An optional motor, e.g., stepper motor **2032**, may be used to distally advance or proximally withdraw probe **2026**

through a known longitudinal distance using, e.g., actuator variation **2080** above. The distance traveled may be controlled and/or recorded via processor **963** and controller **965** of FIG. **21B**. Probe actuator **2020** may also contain within the handle **2022** a separate motor, e.g., DC motor **2034**, used for the rotational control of probe **2026**. The motor **2034** may rotate, e.g., in this variation the central shaft **2023**, which may also connect the chuck **2024** with probe **2026**. Each of the motors may have encoders (not shown) to determine both the rotational and axial position of the probe. Motor **2034** may also be controlled via the processor **963** and/or controller **965** through signal cable **2036**.

FIG. **28** shows an isometric view of probe actuator **2020** of FIG. **27** with various components removed for clarity. Motor **2034** may be seen connected to the rotational shaft **2023** via a rotational gear **2035**. Shaft **2023** may also be seen optionally extending from the motor **2034** to the probe or guidewire chuck **2024**.

FIG. **29** shows an isometric view of an alternative probe actuator **2040** which has had the cover partially removed for clarity. As shown, handle **2042** may contain the components as described above, e.g., chuck **2024**, amplifier **2028**, stepper motor **2032**, DC motor **2034**, etc. The variation **2040** seen has the DC motor **2034** positioned in-line with the other components in a collinear arrangement. Thus, motor **2034** may be aligned and mechanically connected via coupler **2044** to transfer the rotational motion via shafts **2046** to chuck **2024**. This arrangement allows for the compact packaging of the components within an ergonomically designed handle **2042**.

The chuck **2024** which acts as the interface between the probe actuator and the probe itself is preferably removable as a separate unit from the probe actuator and may optionally be disposable. It may be provided as a package with the probe or guidewire for use with different probe actuators to maintain the sterility of the probe and the chuck between different patients. FIG. **30A** shows a side view of a chuck **2024** which has been removed from the probe actuator. As seen by the dashed lines, a probe insertion lumen **2050** is defined within the chuck **2024** for receiving the proximal end of the probe **2026**. Within the insertion lumen **2050**, there may be one or several contacts **2052** which are complementary to the contacts **2006**, **2008** located on probe **2026**.

Chuck **2024** may also be configured such that probe **2026** is mechanically seated securely within the insertion lumen **2050**. Ensuring a secure mechanical fit can ensure good signal transfer between probe **2026** and the amplifier **2028**. Moreover, the processor **963** may be configured whereby if the probe **2026** is not securely seated, any temperature readings will default to a null value or alternatively to a predetermined value which is well beyond normal readings to indicate a faulty connection in the system.

Moreover, the insertion lumen **2050** may further define a stop or a barrier within for halting the insertion of the probe **2026** within the lumen **2050** at the desirable position such that the contacts are fittingly aligned with one another. When the contacts are desirably aligned, the electrical signals taken by the probe **2026** may be transferred through the chuck **2024** with minimal noise and interference. The proximal end of the chuck **2024** may define an attachment **2054** for connection to the probe actuator in which the attachment region **2054** defines several contact regions. These regions are configured to allow for the transfer of signals from contacts **2052** to an electrically connected amplifier while chuck **2024** rotates about its own longitudinal axis during signal acquisition.

FIG. **30B** shows one variation of an electrical schematic of chuck **2024** from FIG. **30A** which may be self-calibrated. As seen, with probe **2026** seated within chuck **2024**, electrical contact may be made between contacts **2052** and probe **2026**. Chuck **2024** may be configured to have variable resistors **2090**, which may also be discrete resistors, in electrical communication between probe **2026** and attachment region **2054**. Variable resistors **2090** can be used to determine a calibration factor for a given probe which may be provided along with a chuck calibrated to the probe. For example, a resistor value of, e.g., 1 to 1000 Ω , can be selected to have 1000 discrete values. An arbitrary resistor value of, e.g., 500 Ω , may be selected as a neutral point and any probe having calibration errors above this neutral point may be used with a resistor having a value above 500 Ω and any probe having calibration errors below this neutral point may be used with a resistor having a value below 500 Ω . Variable resistors **2090** in any chuck **2024** may simply be adjusted accordingly to account for the calibration errors.

The amplifier **2028** of FIGS. **27** and **29** are shown in isometric and end views in FIGS. **31A** and **31B**, respectively. The amplifier **2028** is used to amplify the acquired signals taken from the tissue by the probe while rotating about a longitudinal axis as seen by the rotational arrows in FIG. **31A**. As signals are electrically received by the amplifier circuitry **2060**, they may be transferred via a rotating platform **2062** which is in electrical communication with amplifier **2028**. The platform **2062**, which is preferably circular in shape but may also be formed into other shapes, may have a plurality of contacts **2064** formed on one side of the platform **2062**. The contacts **2064** may be formed into any number of concentric circles depending upon the number of contacts needed to transfer the signal. When the amplifier **2028** and the platform **2062** rotate during signal acquisition, the received signals may be transmitted through the contacts **2064** to brushes in corresponding contact without having to stop for signal transfer.

Signal processing and probe manipulation are preferably done by processor **963** and/or controller **965**. However, manual operation of the probe may sometimes be desirable. To allow for easy manual manipulation, an intervening chuck assembly, an intervening connector cable, or a combination of both may be utilized. As seen in FIG. **32**, an isometric view of a manually actuated probe assembly **2070** is illustrated with an optional intervening chuck **2072**. The intervening chuck **2072** may be used to receive the probe **2026** in the same manner as described above and the chuck **2072** may have an optional connector **2074** for attachment to the intervening cable connector **2078**. The intervening connector cable **2076** is preferably made of a polymeric material which is flexible enough to assume various curves but is stiff enough to transmit a torquing force along the length of the connector cable **2076**. This can be accomplished through any variety of methods in constructing the connector cable **2076**; for instance, metallic braids, reinforcing braids, or strands may be used in the construction of the cable. Alternatively, thermoset or thermoplastic polymers having a sufficient shear strength may be used alone or in combination with the various reinforcing methods.

The intervening chuck **2072** and connector cable **2076** may be used merely as an extension of the chuck **2024** in normal operation. When manual manipulation is desired, however, the physician or surgeon may manipulate the intervening chuck **2072** by hand to impart a rotational or longitudinal motion to the probe **2026** as necessary or desired. The intervening chuck assembly **2072** may be integrated directly with connector cable **2076**. Alternatively,

the chuck 2072 may be maintained as a separate device, as currently shown in FIG. 32, and attached separately to cable connector 2078 to maintain the sterility of the connector 2076 and handle 2022 prior to its use. Moreover, chuck 2072 may be omitted entirely and cable connector 2078 may be configured to receive and hold probe 2026 directly. Manual manipulation of probe 2026 may, in this case, be accomplished by rotating cable 2076, connector 2078 or probe 2026 directly.

Although the present invention has been described in detail in terms of preferred embodiments, no limitation on the scope of the invention is intended. The scope of the subject matter in which an exclusive right is claimed is defined in the appended claims.

What is claimed is:

1. A diagnostic probe suitable for insertion into a blood vessel comprising:

an elongate stem including a proximal end portion and a distal end portion terminating in a coil and having at least a segment thereof biased away from the rotational axis of the probe and having a torque response of no more than about 0.4 ozf in.;

a transducer mounted to the coil;

a connector at the proximal end portion of the stem; and at least one conductor connecting the transducer to the connector.

2. The diagnostic probe of claim 1 wherein an elongate shaping mandrel extends through the coil.

3. The diagnostic probe of claim 1 wherein the coil is rotatable relative to the proximal end portion of the stem and the probe further comprises a rotatable actuation shaft extending through the proximal end portion of the stem and operably associated with the coil.

4. The diagnostic probe of claim 3 further comprising an actuator adapted for coupling to the proximal end portion of the stem and including a motor operably coupled to the actuation shaft.

5. The diagnostic probe of claim 3 wherein the proximal end portion of the stem defines a sheath slidable on the actuation shaft and operably coupled to the coil for allowing the axial reciprocal movement of the coil.

6. The diagnostic probe of claim 1 wherein the coil is biased at an angle between about 10° to 90° relative to the longitudinal axis of the stem.

7. The diagnostic probe of claim 6 wherein the coil is biased at an angle between about 40° to 60° relative to the longitudinal axis of the stem.

8. The diagnostic probe of claim 6 wherein the coil is biased away from the longitudinal axis of the stem.

9. The diagnostic probe of claim 6 wherein the coil is biased towards the longitudinal axis of the stem.

10. The diagnostic probe of claim 1 wherein the stem includes a mid portion between the proximal end portion and the coil and the flexural rigidity ratio between the proximal end portion and the mid portion and the coil is about 1 to 4,400 to 13,000, respectively.

11. The diagnostic probe of claim 1 further comprising a sensor mounted to the coil adjacent to the transducer for measuring an impedance against the blood vessel.

12. The diagnostic probe of claim 1 wherein the transducer is adapted to have a measurement response time between about 10 to 100 msec.

13. The diagnostic probe of claim 1 wherein the probe is adapted to be withdrawn longitudinally through the blood vessel at a rate of 0.3 to 10 mm/sec.

14. The diagnostic probe of claim 1 wherein the probe is adapted to rotate about a longitudinal axis defined by the elongate stem at a rate of between 1 to 100 rpm.

15. A device for sensing the profile of a hollow body organ, comprising:

a hollow guidewire having a relaxed bent configuration defining an angle between about 10° to 90° relative to a longitudinal axis of the guidewire, and a contracted configuration; and

a sensor connected to the guidewire and moveable therewith, the sensor being displaceable laterally relative to the longitudinal axis of the guidewire when the guidewire is in the relaxed configuration.

16. The device of claim 15 further comprising a catheter having a longitudinal axis wherein the hollow guidewire is slidably disposable therewithin.

17. The device of claim 16 wherein the guidewire has the relaxed bent configuration when disposed externally of the catheter and the contracted configuration when disposed internally of the catheter.

18. The device of claim 15 wherein the guidewire is bent at an angle between about 40° to 60° relative to the longitudinal axis of the guidewire.

19. A diagnostic probe suitable for insertion into a blood vessel comprising a stem including a proximal end portion, a distal end portion and a mid portion therebetween, the ratio of the flexural rigidity of the distal end portion relative to the mid portion and the proximal end portion in the range of 1:(4 to 4,400):(110 to 13,000), respectively.

20. The diagnostic probe of claim 19 wherein the ratio of the flexural rigidity of the distal end portion relative to the mid portion and the proximal end portion is 1:4:110, respectively.

21. The diagnostic probe of claim 19 wherein the ratio of the flexural rigidity of the distal end portion relative to the mid portion and the proximal end portion is 1:400:1200, respectively.

22. The diagnostic probe of claim 19 wherein the ratio of the flexural rigidity of the distal end portion relative to the mid portion and the proximal end portion is 1:4,400:13,000, respectively.

23. The system of claim 1 wherein the transducer is a type selected from the group consisting of thermocouples, thermistors, radiation sensors, oxygen sensors, ultrasonic transducers, impedance sensors, pH sensors, and mechanical force sensors.

24. A system for determining the profile of a hollow body organ comprising:

an elongate stem including a proximal end portion having a connector mounted thereto and a distal end portion having a detector mounted thereto, wherein at least a segment of the distal end portion is biased away from a rotational axis of the stem when in a relaxed configuration;

a conductor extending through the stem between the detector and the connector;

a processor in communication with the connector; and an amplifier in electrical communication with the proximal end portion of the stem, the amplifier being adapted to rotate about the rotational axis of the stem while amplifying signals received from the detector.

25. The system of claim 24 wherein the detector comprises a transducer.

26. The system of claim 24 wherein the connector comprises a plurality of spaced-apart bands of conductive material extending along the proximal end portion of the stem and separated therefrom by a plurality of bands of insulative material.

27. The system of claim 26 wherein the stem includes an outer surface and the respective bands of conductive and insulative material are flush with the outer surface of the stem.

23

28. The system of claim 24 further comprising at least one actuator attachable to the proximal end portion of the stem and adapted to provide rotational, axial, or both rotational and axial movement to the stem.

29. The system of claim 28 wherein the actuator comprises at least one motor coupled to the stem for providing a torquing force for rotating the stem about the rotational axis.

30. The system of claim 29 wherein the actuator is adapted to rotate about a longitudinal axis defined by the elongate stem at a rate of between 1 to 100 rpm.

31. The system of claim 29 wherein a rotatable shaft extends at least partially through the actuator between the motor and the proximal end portion which is operably coupled to the shaft for rotation therewith.

32. The system of claim 31 wherein the proximal end portion defines a sheath which is slidable axially in response to the activation of the shaft and is operably coupled to the distal end portion for allowing the axial movement of the distal end portion.

33. The system of claim 28 wherein the actuator includes at least one additional motor coupled to the stem for providing an axial force for moving the stem axially.

34. The system of claim 33 wherein the actuator is adapted to proximally withdraw the stem at a rate of 0.3 to 10 mm/sec.

35. The system of claim 24 further comprising a rotatable chuck member having a proximal end which is adapted to be in communication with the processor, the chuck member defining a lumen at least partially therethrough for receiving the proximal end portion of the stem.

36. The system of claim 35 further comprising an intervening connector having a first end and a second end with a length therebetween, wherein the first end is adapted for attachment to the proximal end of the chuck member and the second end is adapted to be in communication with the

24

processor, and wherein the length is adapted to transmit a rotational movement to the stem.

37. The system of claim 24 further comprising an intervening connector having a first end and a second end with a length therebetween, wherein the first end is adapted for attachment to the proximal end portion of the stem and the second end is adapted to be in communication with the processor, and wherein the length is adapted to transmit a rotational movement to the stem.

38. The system of claim 24 further comprising a controller for controlling the rotational and axial movement of the stem, the controller being in electrical communication with the processor and the connector.

39. The system of claim 24 further comprising a pod which is adapted to be uniformly heated or cooled to a predetermined temperature for calibrating the system, the pod being further adapted to receive the detector during the calibration.

40. The system of claim 24 wherein the processor comprises a computer.

41. The system of claim 24 wherein the processor is in electrical communication with the connector.

42. The system of claim 24 wherein the processor is in optical communication with the connector.

43. The system of claim 24 further comprising a sensor mounted to the coil adjacent to the detector for measuring an impedance against the hollow body organ.

44. The system of claim 24 wherein the detector is adapted to have a measurement response time between about 10 to 100 msec.

45. The system of claim 24 wherein the detector is a type selected from the group consisting of thermocouples, thermistors, radiation sensors, oxygen sensors, ultrasonic transducers, impedance sensors, pH sensors, and mechanical force sensors.

* * * * *

专利名称(译)	用于感测中空身体器官的参数的装置		
公开(公告)号	US6939313	公开(公告)日	2005-09-06
申请号	US10/146014	申请日	2002-05-14
[标]申请(专利权)人(译)	萨达特瓦希德 TSUGITA ROSS		
申请(专利权)人(译)	萨达特瓦希德 TSUGITA ROSS		
当前申请(专利权)人(译)	萨达特，瓦希德		
[标]发明人	SAADAT VAHID TSUGITA ROSS		
发明人	SAADAT, VAHID TSUGITA, ROSS		
IPC分类号	A61B5/00 A61B5/01 A61B5/103 A61B5/107 A61B5/117		
CPC分类号	A61B5/015 A61B5/0538 A61B5/1076 A61B5/1077 A61M2025/09116		
优先权	09/904024 2001-07-12 US		
其他公开文献	US20030088187A1		
外部链接	Espacenet USPTO		

摘要(译)

一种用于感测中空身体器官的轮廓的装置包括中空导丝或携带传感器的探针。中空探针包括远端盘绕的端管，其具有相对于探针纵轴以约10°至90°之间的角度弯曲并且具有不大于约0.4ozf in的扭矩响应的尖端。远端的抗弯刚度。相对于形成探针的中间和近端管的管通常分别在约1：(4至4,400)：(110至13,000)的范围内。致动器可拆卸地固定到探头上，并包括一个或多个马达，这些马达允许传感器以旋转和轴向路径行进通过身体器官。

