



US007850676B2

(12) **United States Patent**
Wood, Jr.

(10) **Patent No.:** **US 7,850,676 B2**
(45) **Date of Patent:** ***Dec. 14, 2010**

(54) **SYSTEM WITH A RESERVOIR FOR
PERFUSION MANAGEMENT**

(75) Inventor: **Lowell L. Wood, Jr.**, Livermore, CA
(US)

(73) Assignee: **The Invention Science Fund I, LLC**,
Bellevue, WA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 1270 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **10/827,572**

(22) Filed: **Apr. 19, 2004**

(65) **Prior Publication Data**

US 2005/0234398 A1 Oct. 20, 2005

(51) **Int. Cl.**

A61M 25/00 (2006.01)

A61M 37/00 (2006.01)

(52) **U.S. Cl.** **604/528**; 604/288.04; 604/523;
604/264; 604/93.01

(58) **Field of Classification Search** 604/93.01,
604/164.01, 187, 194–196, 239, 264, 272,
604/288.04, 523, 528; 600/101–183; 606/107
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,391,697 A 7/1968 Greatbatch
3,837,339 A 9/1974 Aisenberg et al.
4,585,652 A 4/1986 Miller et al.
4,628,928 A 12/1986 Lowell
4,714,460 A 12/1987 Calderon
4,763,667 A 8/1988 Manzo
4,771,772 A 9/1988 DeWitt
4,817,601 A 4/1989 Roth et al.
4,871,351 A 10/1989 Feingold

4,905,689 A 3/1990 Stack et al.
4,944,659 A * 7/1990 Labbe et al. 417/413.2
4,994,071 A 2/1991 MacGregor
5,019,372 A 5/1991 Folkman et al.
5,153,827 A 10/1992 Coutre et al.
5,176,638 A 1/1993 Don Michael
5,188,111 A 2/1993 Yates et al.
5,234,457 A 8/1993 Andersen
5,269,303 A 12/1993 Wernicke et al.
5,279,607 A 1/1994 Schentag et al.
5,310,404 A 5/1994 Gyory et al.
5,314,451 A 5/1994 Mulier
5,335,657 A 8/1994 Terry, Jr. et al.
5,337,732 A 8/1994 Grundfest et al.
5,338,625 A 8/1994 Bates et al.
5,339,051 A 8/1994 Koehler et al.
5,353,807 A 10/1994 DeMarco

(Continued)

FOREIGN PATENT DOCUMENTS

EP 1 245 201 A1 10/2002

(Continued)

OTHER PUBLICATIONS

U.S. Appl. No. 11/651,946, Ferren et al.


(Continued)

Primary Examiner—Nicholas D Lucchesi
Assistant Examiner—Victoria P Campbell

(57) **ABSTRACT**

A system for perfusion management that monitors, main-
tains, diagnoses, or treats perfusion deficiencies.

37 Claims, 5 Drawing Sheets

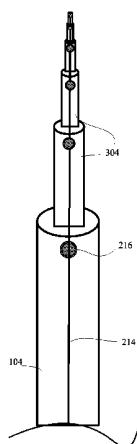

U.S. PATENT DOCUMENTS

5,386,741	A	2/1995	Rennex	6,337,997	B1	1/2002	Rise
5,395,390	A	3/1995	Simon et al.	6,372,248	B1	4/2002	Qin et al.
5,398,670	A	3/1995	Ortiz et al.	6,383,162	B1	5/2002	Sugarbaker
5,403,311	A	4/1995	Abele et al.	6,384,741	B1 *	5/2002	O'Leary, Sr. 340/937
5,411,551	A	5/1995	Winston et al.	6,385,472	B1	5/2002	Hall et al.
5,437,660	A	8/1995	Johnson et al.	6,398,280	B1	6/2002	Parker et al.
5,476,450	A	12/1995	Ruggio	6,402,678	B1	6/2002	Fischell et al.
5,497,147	A	3/1996	Arms et al.	6,409,674	B1	6/2002	Brockway et al.
5,522,394	A	6/1996	Zurbrugg	6,436,120	B1	8/2002	Meglin
5,551,953	A	9/1996	Lattin et al.	6,442,413	B1	8/2002	Silver
5,554,914	A	9/1996	Miyazawa	6,450,937	B1	9/2002	Mercereau et al.
5,569,968	A	10/1996	Lal et al.	6,464,687	B1	10/2002	Ishikawa et al.
5,574,347	A	11/1996	Neubauer	6,475,639	B2	11/2002	Shahinpoor et al.
5,593,434	A	1/1997	Williams	6,490,483	B2	12/2002	Willis
5,599,324	A	2/1997	McAlister et al.	6,497,714	B1	12/2002	Ishikawa et al.
5,610,488	A	3/1997	Miyazawa	6,500,174	B1	12/2002	Maguire et al.
5,624,398	A	4/1997	Smith et al.	6,512,949	B1	1/2003	Combs et al.
5,632,754	A	5/1997	Farley et al.	6,512,950	B2	1/2003	Li et al.
5,643,296	A	7/1997	Hundertmark et al.	6,514,237	B1	2/2003	Maseda
5,662,587	A	9/1997	Grundfest et al.	6,530,950	B1	3/2003	Alvarado et al.
5,669,874	A	9/1997	Feiring	6,547,825	B1	4/2003	Shimizu et al.
5,674,276	A	10/1997	Andersen et al.	6,548,982	B1	4/2003	Papanikolopoulos et al.
5,688,269	A	11/1997	Newton et al.	6,554,798	B1	4/2003	Mann et al.
5,695,457	A	12/1997	St. Goar et al.	6,575,969	B1	6/2003	Rittman, III et al.
5,697,967	A	12/1997	Dinh et al.	6,585,763	B1	7/2003	Keilman et al.
5,702,432	A	12/1997	Chen et al.	6,591,137	B1	7/2003	Fischell et al.
5,705,293	A	1/1998	Hobson	6,592,567	B1	7/2003	Levin et al.
5,728,089	A	3/1998	Lal et al.	6,597,954	B1	7/2003	Pless et al.
5,737,279	A	4/1998	Carter	6,607,553	B1	8/2003	Healy et al.
5,782,798	A	7/1998	Rise	6,616,676	B2	9/2003	Bashiri et al.
5,804,563	A	9/1998	Still et al.	6,623,519	B2	9/2003	Edwin et al.
5,807,395	A	9/1998	Mulier et al.	6,632,216	B2	10/2003	Houzeago et al.
5,819,736	A	10/1998	Avny et al.	6,638,273	B1	10/2003	Farley et al.
5,830,179	A	11/1998	Mikus et al.	6,648,908	B2	11/2003	Dobak, III et al.
5,830,207	A	11/1998	Leeb et al.	6,666,860	B1	12/2003	Takahashi
5,831,012	A	11/1998	Nilsson et al.	6,669,683	B2	12/2003	Santini, Jr. et al.
5,843,139	A	12/1998	Goedeke et al.	6,673,042	B1	1/2004	Samson et al.
5,855,801	A	1/1999	Lin et al.	6,673,363	B2	1/2004	Luo et al.
5,873,835	A	2/1999	Hastings et al.	6,679,893	B1	1/2004	Tran
5,908,027	A	6/1999	Butterfield et al.	6,709,388	B1	3/2004	Mosse et al.
5,947,119	A	9/1999	Reznick	6,711,423	B2	3/2004	Colvin, Jr.
5,951,600	A	9/1999	Lemelson	6,712,835	B2	3/2004	Mazzocchi et al.
5,954,675	A	9/1999	Dellagatta	6,719,684	B2	4/2004	Kim et al.
5,964,773	A	10/1999	Greenstein	6,735,474	B1	5/2004	Loeb et al.
6,004,269	A	12/1999	Crowley et al.	6,735,475	B1	5/2004	Whitehurst et al.
6,016,449	A	1/2000	Fischell et al.	6,743,211	B1	6/2004	Prausnitz et al.
6,022,316	A	2/2000	Eppstein et al.	6,754,536	B2	6/2004	Swoyer et al.
6,053,873	A	4/2000	Govari et al.	6,755,802	B2	6/2004	Bell
6,086,528	A *	7/2000	Adair 600/104	6,755,803	B1	6/2004	Le et al.
6,102,845	A	8/2000	Woodard et al.	6,764,441	B2	7/2004	Chiel et al.
6,111,520	A	8/2000	Allen et al.	6,773,429	B2	8/2004	Sheppard, Jr. et al.
6,128,538	A	10/2000	Fischell et al.	6,797,522	B1	9/2004	Still et al.
6,134,474	A	10/2000	Fischell et al.	6,802,811	B1	10/2004	Slepian
6,159,230	A	12/2000	Samuels	6,824,508	B2	11/2004	Kim et al.
6,164,284	A	12/2000	Schulman et al.	6,824,510	B2	11/2004	Kim et al.
6,170,488	B1	1/2001	Spillman, Jr. et al.	6,824,561	B2	11/2004	Soykan et al.
6,179,789	B1	1/2001	Tu et al.	6,849,183	B2	2/2005	Gorsuch et al.
6,185,452	B1	2/2001	Schulman et al.	6,855,115	B2	2/2005	Fonseca et al.
6,186,986	B1	2/2001	Berg et al.	6,860,867	B2	3/2005	Seward et al.
6,187,599	B1	2/2001	Asher et al.	6,861,001	B2	3/2005	Lee et al.
6,197,013	B1	3/2001	Reed et al.	6,890,303	B2	5/2005	Fitz
6,219,577	B1	4/2001	Brown, III et al.	6,898,464	B2	5/2005	Edell et al.
6,221,099	B1	4/2001	Andersen et al.	6,911,004	B2	6/2005	Kim et al.
6,240,312	B1	5/2001	Alfano et al.	6,911,496	B2	6/2005	Rhee et al.
6,248,345	B1	6/2001	Goldenheim et al.	6,920,359	B2	7/2005	Meadows et al.
6,249,076	B1	6/2001	Madden et al.	6,921,413	B2	7/2005	Mahadevan-Jansen et al.
6,255,361	B1	7/2001	Rajagopalan et al.	6,925,357	B2	8/2005	Wang et al.
6,278,379	B1	8/2001	Allen et al.	6,929,636	B1	8/2005	Von Alten
6,295,990	B1	10/2001	Lewis et al.	6,936,003	B2	8/2005	Iddan
6,296,638	B1 *	10/2001	Davison et al. 606/41	6,939,290	B2	9/2005	Iddan
6,322,532	B1	11/2001	D'Sa et al.	6,939,376	B2	9/2005	Shulze et al.
				6,950,707	B2	9/2005	Whitehurst
				6,953,589	B1	10/2005	Trautman et al.

6,958,034	B2	10/2005	Iddan	2005/0079132	A1	4/2005	Wang et al.
6,959,215	B2	10/2005	Gliner et al.	2005/0107870	A1	5/2005	Wang et al.
6,960,227	B2	11/2005	Jones et al.	2005/0113460	A1	5/2005	Glick
6,963,792	B1	11/2005	Green	2005/0121411	A1	6/2005	Cohen
6,991,617	B2	1/2006	Hektner et al.	2005/0126916	A1	6/2005	Lockard et al.
7,003,352	B1	2/2006	Whitehurst	2005/0149170	A1	7/2005	Van Tassel et al.
7,013,177	B1	3/2006	Whitehurst et al.	2005/0151524	A1	7/2005	Sae-Ueng et al.
7,037,343	B2	5/2006	Imran	2005/0177223	A1	8/2005	Palmaz
7,042,184	B2	5/2006	Oleynikov et al.	2005/0182482	A1	8/2005	Wang et al.
7,101,386	B2	9/2006	Dobak, III	2005/0203613	A1	9/2005	Arney et al.
7,115,109	B2	10/2006	Gerdts et al.	2005/0216074	A1	9/2005	Sahatjian et al.
7,125,382	B2	10/2006	Zhou et al.	2005/0221529	A1	10/2005	Bang et al.
7,131,979	B2	11/2006	DiCarlo et al.	2005/0228259	A1	10/2005	Glukhovsky et al.
7,160,258	B2	1/2007	Imran et al.	2005/0234393	A1	10/2005	Wood, Jr.
7,245,954	B2	7/2007	Glukhovsky	2005/0234440	A1	10/2005	Wood, Jr.
7,297,113	B1	11/2007	Russell et al.	2005/0238689	A1	10/2005	Carpenter et al.
7,341,577	B2	3/2008	Gill	2005/0272806	A1	12/2005	Falotico et al.
7,365,509	B2	4/2008	Park et al.	2005/0272974	A1	12/2005	Iddan
7,383,071	B1	6/2008	Russell et al.	2005/0277839	A1	12/2005	Alderman et al.
2001/0029348	A1	10/2001	Willis	2005/0278020	A1	12/2005	Wang et al.
2001/0051766	A1	12/2001	Gazdzinski	2006/0004395	A1	1/2006	Chiel et al.
2002/0065509	A1 *	5/2002	Lebel et al. 604/892.1	2006/0009810	A1	1/2006	Mann et al.
2002/0068080	A1	6/2002	Lerner	2006/0015146	A1	1/2006	Girouard et al.
2002/0090388	A1	7/2002	Humes et al.	2006/0074479	A1	4/2006	Bailey et al.
2002/0116029	A1	8/2002	Miller et al.	2006/0119304	A1	6/2006	Farritor et al.
2002/0116034	A1	8/2002	Miller et al.	2006/0167339	A1	7/2006	Gilad et al.
2002/0147480	A1	10/2002	Mamayek	2007/0010868	A1	1/2007	Ferren et al.
2002/0156462	A1 *	10/2002	Stultz 604/891.1	2007/0066929	A1	3/2007	Ferren et al.
2002/0165592	A1	11/2002	Glukhovsky et al.	2007/0088334	A1	4/2007	Hillis et al.
2002/0169436	A1	11/2002	Gurm et al.	2007/0225634	A1	9/2007	Ferren et al.
2002/0188323	A1	12/2002	Penner et al.	2008/0063703	A1	3/2008	Gross et al.
2002/0193679	A1	12/2002	Malave et al.	2008/0103440	A1	5/2008	Ferren et al.
2002/0193874	A1	12/2002	Crowley				
2002/0198470	A1	12/2002	Imran et al.				
2002/0198521	A1	12/2002	Maguire				
2002/0198604	A1	12/2002	Schulman et al.				
2003/0024534	A1	2/2003	Silvestri et al.				
2003/0040704	A1	2/2003	Dorros et al.				
2003/0065358	A1	4/2003	Freckner et al.				
2003/0069475	A1	4/2003	Banik et al.				
2003/0069523	A1	4/2003	Williams et al.				
2003/0151524	A1	8/2003	Clark				
2003/0152823	A1	8/2003	Heller				
2003/0158584	A1	8/2003	Cates et al.				
2003/0163177	A1	8/2003	Eggers et al.				
2003/0167000	A1	9/2003	Mullick et al.				
2003/0214579	A1	11/2003	Iddan				
2003/0220556	A1	11/2003	Porat et al.				
2004/0008853	A1	1/2004	Pelrine et al.				
2004/0018508	A1	1/2004	Friedman				
2004/0019374	A1	1/2004	Hojeibane et al.				
2004/0064093	A1	4/2004	Hektner et al.				
2004/0073177	A1	4/2004	Hickle				
2004/0073190	A1	4/2004	Deem et al.				
2004/0097819	A1	5/2004	Duarte				
2004/0098030	A1	5/2004	Makower et al.				
2004/0133147	A1	7/2004	Woo				
2004/0147939	A1	7/2004	Rabkin et al.				
2004/0148034	A1	7/2004	Kagan et al.				
2004/0162469	A1	8/2004	Imran				
2004/0162501	A1	8/2004	Imran				
2004/0176664	A1	9/2004	Iddan				
2004/0199246	A1	10/2004	Chu et al.				
2004/0225325	A1	11/2004	Bonutti				
2004/0225326	A1	11/2004	Weiner et al.				
2004/0260391	A1	12/2004	Santini, Jr. et al.				
2004/0267240	A1	12/2004	Gross et al.				
2005/0004553	A1 *	1/2005	Douk 604/523				
2005/0021023	A1	1/2005	Guglielmi et al.				
2005/0027236	A1 *	2/2005	Douk 604/40				
2005/0058701	A1	3/2005	Gross et al.				
2005/0065592	A1	3/2005	Holzer				
2005/0069925	A1	3/2005	Ford et al.				

FOREIGN PATENT DOCUMENTS

EP	1 618 831	A2	1/2006
EP	2 163 206	A1	3/2010
GB	99810271.7		10/2001
JP	2005-74229		3/2005
WO	WO 96/39999		12/1996
WO	WO 98/14243		4/1998
WO	WO 99/20335		4/1999
WO	WO 99/44665		9/1999
WO	WO 00/69515		11/2000
WO	WO 03/072157	A1	9/2003
WO	WO 03/090618	A2	11/2003
WO	WO 03/106966	A2	12/2003
WO	WO 2004/028335	A2	4/2004
WO	WO 2004/058041	A2	7/2004
WO	WO 2004/086958	A1	10/2004
WO	WO 2005/082248	A1	9/2005

OTHER PUBLICATIONS

U.S. Appl. No. 11/645,358, Ferren et al.
U.S. Appl. No. 11/645,357, Ferren et al.
U.S. Appl. No. 11/485,619, Hillis et al.
U.S. Appl. No. 11/478,368, Ferren et al.
U.S. Appl. No. 11/417,898, Hillis et al.
U.S. Appl. No. 11/403,230, Ferren et al.
U.S. Appl. No. 10/949,186, Hillis et al.
UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0706802.6; bearing a date of Dec. 1, 2008; pp. 1-2.
PCT International Search Report; International App. No. PCT/US05/13349; Apr. 28, 2008; pp. 1-2.
PCT International Search Report; International App. No. PCT/US2007/008993; Sep. 29, 2008; pp. 1-3.
PCT International Search Report; International App. No. PCT/US07/10819; Aug. 27, 2008; pp. 1-3.
PCT International Search Report; International App. No. PCT/US07/10824; Aug. 21, 2008; pp. 1-3.
PCT International Search Report; International App. No. PCT/US07/10942; Aug. 15, 2008; pp. 1-3.

- PCT International Search Report; International App. No. PCT/US07/10936; Jul. 24, 2008; pp. 1-3.
- PCT International Search Report; International App. No. PCT/US07/10857; Jul. 21, 2008; pp. 1-2.
- PCT International Search Report; International App. No. PCT/US07/10969; Nov. 10, 2008; pp. 1-2.
- PCT International Search Report; International App. No. PCT/US2007/008993; Sep. 29, 2008; pp. 1-3.
- "001_08 Comparison of Capsule Cameras: M2A (Given Imaging) vs. NORIKA3 (RF System lab)" RF System lab; bearing dates of 2001-2004; pp. 1-2; http://www.rfnorika.com/eng/system/sys_008.html; printed on May 4, 2006.
- "A Hydrogel-based CO₂ sensor"; BIOS—The lab on a chip group; bearing a date of Aug. 29, 2005; pp. 1-2; <http://bios.ewi.utwente.nl/research/analysissystemssensors/ahydrogelbased.doc/index.html>; printed on Apr. 25, 2006; University of Twente; the Netherlands.
- Agarwal, Abhishek K.; Atencia, Javier; Beebe, David J.; Jiang, Hongrui; "Magnetically-driven temperature-controlled microfluidic actuators"; pp. 1-5; http://www.unl.im.dendai.ac.jp/INSS2004/INSS2004_papers/OralPresentations/C2.pdf.
- "Agile new plastics change shape with heat"; MIT News Office; Nov. 20, 2006; pp. 1-4; Massachusetts Institute of Technology; printed on Nov. 22, 2006; <http://web.mit.edu/newsoffice/2006/triple-shape.html>.
- "Agile new plastics change shape with heat"; MIT Tech Talk; Nov. 22, 2006; p. 5 (1 page).
- Ananthaswamy, Anil; "First robot moved by muscle power"; bearing a date of Feb. 27, 2004; pp. 1-3; New Scientist; <http://www.newscientist.com/article.ns?id=dn4714>; printed on Sep. 12, 2006.
- Asari, Vijayan K.; Kumar, Sanjiv; Kassim, Irwan M.; "A Fully Autonomous Microrobotic Endoscopy System"; Journal of Intelligent and Robotic Systems; bearing a date of 2000; pp. 325-341; vol. 28; Kluwer Academic Publishers.
- Behkam, Bahareh; Sitti, Metin; "Towards Hybrid Swimming Microrobots: Bacteria Assisted Propulsion of Polystyrene Beads"; Proceedings of the 28th IEEE EMBS Annual International Conference; bearing dates of Aug. 30, 2006-Sep. 3, 2006 and 2006; pp. 2421-2424; IEEE.
- Berlinger, Norman T.; "Robotic Surgery—Squeezing into Tight Places"; New England Journal of Medicine; bearing dates of May 17, 2006, May 18, 2006, and 2006; pp. 2099-2101; Massachusetts Medical Society; www.nejm.org.
- Bezrouk, A.; Hanuš, J.; Záhora, J.; "Temperature Characteristics of Nitinol Spiral Stents"; Scripta Medica (BRNO); bearing dates of Aug. 2005, Oct. 2005; pp. 219-226; vol. 78, No. 4.
- Bialek, William; Rieke, Fred; De Ruyter Van Steveninck, Rob R.; Warland, David; "Reading a Neural Code"; Science; bearing a date of Jun. 28, 1991; pp. 1854-1857; vol. 252.
- Bucher, Volker; Graf, Michael; Stelzle, Martin; Nisch, Wilfried; "Low-Impedance Thin-Film Polycrystalline Silicon Microelectrodes for Extracellular Stimulation and Recording"; Biosensors and Bioelectronics; bearing a date of 1999; pp. 639-649; vol. 14; Elsevier Science S.A.; www.elsevier.com/locate/bios.
- Butson, Christopher R.; McIntyre, Cameron C.; "Role of Electrode Design on the Volume of Tissue Activated During Deep Brain Stimulation"; Journal of Neural Engineering; bearing a date of 2006; vol. 3; pp. 1-8; IOP Publishing Ltd.
- Chang, Suk Tai; Paunov, Vesselin N.; Petsev, Dimitar N.; Velev, Orlin D.; "Articles: Remotely Powered Self-Propelling Particles and Micropumps Based on Miniature Diodes"; Nature Materials; bearing a date of 2007; pp. 1-6; Nature Publishing Group; www.nature.com/naturematerials.
- Chen, Haitao; Ebner, Armin D.; Ritter, James A.; Kaminski, Michael D.; Rosengart, Axel J.; "Sequestration of Blood-Borne Magnetic Drug Carrier Particles Using Magnetizable Intravascular Stents"; Collaborative Investigators for Applied Nanotechnology in Medicine; pp. 1; Chicago, Illinois.
- Chen, Ting; Barton, Scott Calabrese, Binyamin, Gary; Gao, Zhiqiang; Zhang, Yongchao, Kim, Hyug-Han; Heller, Adam; "A Miniature Biofuel Cell"; Journal of the American Chemical Society; Aug. 11, 2001; pp. 8630-8631; vol. 123; 2001 American Chemical Society.
- Christensen, Bill; "Musclebot: Microrobot with a Heart"; Technovelgy.com; pp. 1-2; bearing a date of Feb. 27, 2004; <http://technovelgy.com/ct/Science-Fiction-News.asp?NewsNum=46>; printed on Sep. 12, 2006.
- Christensen, Bill; "Propulsion System for 'Fantastic Voyage' Robot"; Technovelgy.com; pp. 1-4; Technovelgy.com; <http://www.technovelgy.com/ct/Science-Fiction-News.asp?NewsNum=811>; printed on Jan. 4, 2007.
- Costamagna; Guido M.D.; "PillCam™ SB Capsule Endoscopy"; Given Imaging.com; bearing dates of 2001-2006; pp. 1-4; <http://www.givenimaging.com/Cultures/en-US/Given/English/Products/CapsuleEndoscopy/>; printed on May 4, 2006.
- Cui, Xinyan; Hetke, Jammie F.; Wiler, James A.; Anderson, David J.; Martin, David C.; "Electrochemical Deposition and Characterization of Conducting Polymer Polypyrrole/PPS on Multichannel Neural Probes"; Sensors and Actuators A Physical; bearing a date of 2001; pp. 8-18; vol. 93; Elsevier Science B.V.; www.elsevier.com/locate/sna.
- Dario, P.; Carrozza, M.C.; Lencioni, L.; Magnani, B.; D'Atanasio, S.; "A Micro Robotic System for Colonoscopy"; Proceedings of the 1997 IEEE International Conference on Robotics and Automation; bearing dates of Apr. 1997 and 1997; pp. 1567-1572; IEEE.
- Dillier, Norbert; Lai, Wai Kong; Almqvist, Bengt; Frohne, Carolin; Müller-Deile, Joachim; Stecker, Matthias; Von Wallenberg, Ernst; "Measurement of the Electrically Evoked Compound Action Potential Via a Neural Response Telemetry System"; Annals Of Otolaryngology and Laryngology; bearing a date of May 2002; pp. 407-414; vol. 111, No. 5; Annals Publishing Company.
- Dongxiang, Chi; Guozheng, Yan; "An earthworm based miniature robot for intestinal inspection"; Proceedings of SPIE; bearing dates of Nov. 7, 2001-Nov. 9, 2001; pp. 396-400; vol. 4601; SPIE.
- Donoghue, John P.; "Review: Connecting Cortex to Machines: Recent Advances in Brain Interfaces"; Nature Neuroscience Supplement; bearing a date on Nov. 2002; pp. 1085-1088; vol. 5; Nature Publishing Group; <http://www.nature.com/natureneuroscience>.
- Fang, Zi-Ping; Mortimer, J. Thomas; "Selective Activation of Small Motor Axons by Quasitrapezoidal Current Pulses"; IEEE Transactions on Biomedical Engineering; bearing a date of Feb. 1991; pp. 168-174; vol. 38, No. 2; IEEE.
- Fiaccabrino, G.C.; Tang, X.-M.; Skinner, N.; De Rooij, N.F.; Koudelka-Hep, M.; "Electrochemical Characterization of Thin-Film Carbon Interdigitated Electrode Arrays"; Analytica Chimica Acta; bearing a date of 1996; pp. 155-160; vol. 326; Elsevier Science B.V.
- Freitas Jr., Robert A.; "8.2.1.2 Arteriocenous Microcirculation"; "9.4.3.5 Legged Ambulation"; "9.4.3.6 Tank-Tread Rolling"; "9.4.3.7 Amoeboid Locomotion"; "9.4.3.8 Inchworm Locomotion"; "Nanomedicine vol. I: Basic Capabilities"; bearing a date of 1999; pp. 211-214, pp. 316-318; Landes Bioscience; Georgetown, Texas, USA.
- Gitter, Alfred H.; Fromm, Michael; Schulzke, Jörg-Dieter; "Impedance Analysis for the Determination of Epithelial and Subepithelial Resistance in Intestinal Tissues"; Journal of Biochemical and Biophysical Methods; bearing a date of 1998; pp. 35-46; vol. 37; Elsevier Science B.V.
- Goda, Yukiko; Colicos, Michael A.; "Protocol: Photoconductive Stimulation of Neurons Cultured on Silicon Wafers"; Nature Protocols; bearing a date of 2006; pp. 461-467; vol. 1, No. 1; Nature Publishing Group; <http://www.nature.com/natureprotocols>.
- Gozani, Shai N.; Miller, John P.; "Optimal Discrimination and Classification of Neuronal Action Potential Waveforms from Multiunit, Multichannel Recordings Using Software-Based Linear Filters"; IEEE Transactions on Biomedical Engineering; bearing a date of Apr. 1994; pp. 358-372; vol. 41, No. 4; IEEE.
- Gray, Charles M.; Maldonado, Pedro E.; Wilson, Mathew; McNaughton, Bruce; "Tetodes Markedly Improve the Reliability and Yield of Multiple Single-Unit Isolation from Multi-Unit Recordings in Cat Striate Cortex"; Journal of Neuroscience Methods; bearing a date of 1995; pp. 43-54; vol. 63; Elsevier Science B.V.
- Hagleitner, C.; Hierlemann, A.; Lange, D.; Kummer, A.; Kerness, N.; Brand, O.; Baltes, H.; "Smart single-chip gas sensor microsystem"; Nature; Nov. 15, 2001; pp. 293-296; vol. 414; Macmillan Magazines Ltd.; www.nature.com.

- Hanna, Darrin M.; Oakley, Barbara A.; Stryker, Gabrielle A.; "Using a System-on-Chip Implantable Device to Filter Circulating Infected Cells in Blood or Lymph"; IEEE Transactions on Biomedical Engineering; bearing dates of Jan. 25, 2003, Mar. 2003; pp. 6-13; vol. 2, No. 1; IEEE.
- Hodgkin, A.L.; Huxley, A.F.; "A Quantitative Description of Membrane Current and its Application to Conduction and Excitation in Nerve"; Journal of Physiology; bearing a date of 1952; pp. 500-544; vol. 117.
- Høeg, H.D.; Slatkin, A.B.; Burdick, J.W.; Grundfest, Dr. Warren S.; "Biomechanical Modeling of the Small Intestine as Required for the Design and Operation of a Robotic Endoscope"; Proceedings ICRA '00 IEEE International Conference on Robotics and Automation; Apr. 24, 2000-Apr. 28, 2000; pp. 1-8; vol. 2.
- Hofmann, U.G.; Folkers, A.; Mösch, F.; Höhl, D.; Kindlundh, M.; Norlin, P.; "A 64(128)-Channel Multisite Neuronal Recording System"; bearing a date of 2002; pp. 1-4.
- Ikeuchi, K.; Yoshinaka, K.; Hashimoto, S.; Tomita, N.; "Locomotion of Medical Micro Robot with Spiral Ribs Using Mucus"; Seventh International Symposium on Micro Machine and Human Science; bearing a date of 1996; pp. 217-222; IEEE.
- Inmann, Andreas; Haugland, Morten; Haase, Jens; Biering-Sørensen, Finn; Sinkjaer, Thomas; "NeuroReport: Signals from Skin Mechanoreceptors used in Control of a Hand Grasp Neuroprosthesis"; Motor Systems; bearing a date of Sep. 17, 2001; pp. 2817-2819; vol. 12, No. 13; Lippincott Williams & Wilkins.
- Janders, M.; Egert, U.; Stelze, M.; Nisch, W.; "Novel Thin Film Titanium Nitride Micro-Electrodes with Excellent Charge Transfer Capability for Cell Stimulation and Sensing Applications"; IEEE Engineering in Medicine and Biology Society; bearing a date of 1996; pp. 245-247; IEEE.
- "Japanese Researchers Unveil Medical Mini Robot"; Yahoo! News; bearing a date of Mar. 8, 2007; pp. 1-2; Yahoo! Inc.; http://news.yahoo.com/s/afp/20070308/hl_afp/afplifestyleshealthscience; printed on Mar. 8, 2007.
- Ji, Jin; Najafi, Khalil; Wise, Kensall D.; "A Low-Noise Demultiplexing System for Active Multichannel Microelectrode Arrays"; IEEE Transactions on Biomedical Engineering; bearing a date of Jan. 1991; pp. 77-81; vol. 38, No. 1; IEEE.
- Kassim, Irwan; Phee, Louis; Ng, Wan S.; Gong, Feng; Dario, Paolo; Mosse, Charles A.; "Locomotion Techniques for Robotic Colonoscopy"; IEEE Engineering in Medicine and Biology Magazine; bearing dates of May/Jun. 2006 and 2006; pp. 49-56; IEEE.
- Kennedy, P.R.; Bakay, R.A.E.; Moore, M.M.; Adams, K.; Goldwraith, J.; "Direct Control of a Computer from the Human Central Nervous System"; IEEE Transactions on Rehabilitation Engineering; bearing a date of Jun. 2000; pp. 198-202; vol. 8, No. 2; IEEE.
- Kobetic, Rudi; Triolo, Ronald J.; Uhlir, James P.; Bieri, Carole; Wibowo, Michael; Polando, Gordie; Marsolais, E. Byron; Davis Jr., John A.; Ferguson, Kathleen A.; Sharma, Mukut; "Implanted Functional Electrical Stimulation System for Mobility in Paraplegia: A Follow-Up Case Report"; IEEE Transactions on Rehabilitation Engineering; bearing a date of Dec. 1999; pp. 390-398; vol. 7, No. 4; IEEE.
- Krueger, Curtis; "New light on blood testing"; Oct. 20, 2006; pp. 1-2; St. Petersburg Times; printed on Oct. 24, 2006; http://www.sptimes.com/2006/10/20news_pf/Tampabay/New_light_on_blood_te.shtml.
- Langer, Robert; Peppas, Nicholas A.; Advances in Biomaterials, Drug Delivery, and Bionanotechnology; AICHE Journal—Bioengineering, Food, and Natural Products; Dec. 2003; pp. 2990-3006; vol. 49, No. 12.
- Loeb, G.E.; Peck, R.A.; Martyniuk, J.; "Toward the Ultimate Metal Microelectrode"; Journal of Neuroscience Methods; bearing a date of 1995; pp. 175-183; vol. 63; Elsevier Science B.V.
- Loeb, Gerald E.; Peck, Raymond A.; Moore, William H.; Hood, Kevin; "BION System for Distributed Neural Prosthetic Interfaces"; Medical Engineering and Physics; bearing a date of 2001; pp. 9-18; vol. 23; Elsevier Science Ltd.; www.elsevier.com/locate/medengphy.
- Lu, Zhao; Martel, Sylvain; "Preliminary Investigation of Bio-carriers Using Magnetotactic Bacteria"; Proceedings of the 28th IEEE EMBS Annual International Conference; bearing dates of Aug. 30, 2006-Sep. 3, 2006 and 2006; pp. 3415-3418; IEEE.
- Mangan, Elizabeth V.; Kingsley, Dan A.; Quinn, Roger D.; Chiel, Hillel J.; "Development of a Peristaltic Endoscope"; IEEE International Conference on Robotics & Automation 2002; pp. 1-6; http://biorobots.cwru.edu/publications/ICRA02_Mangan_Endoscope.pdf.
- Marks, William B.; Loeb, Gerald E.; "Action Currents, Internodal Potentials, and Extracellular Records of Myelinated Mammalian Nerve Fibers Derived from Node Potentials"; Biophysical Journal; 1976; pp. 655-668; vol. 16.
- Martel, Sylvain; "Fundamentals of high-speed piezo-actuated three-legged motion for miniature robots designed for nanometer-scale operations"; pp. 1-8.
- Martel, Sylvain; "Towards MRI-Controlled Ferromagnetic and MC-1 Magnetotactic Bacterial Carriers for Targeted Therapies in Arteriolo-capillary Networks Stimulated by Tumoral Angiogenesis"; Proceedings of the 28th IEEE EMBS Annual International Conference; bearing dates of Aug. 30, 2006-Sep. 3, 2006 and 2006; pp. 3399-3402; IEEE.
- Martel, Sylvain; Mathieu, Jean-Baptiste; Felfoul, Ouajdi; Chanu, Arnaud; Aboussouan, Eric; Tamaz, Samer; Pouponneau, Pierre; "Automatic Navigation of an Untethered Device in the Artery of a Living Animal using a Conventional Clinical Magnetic Resonance Imaging System"; Applied Physics Letters; 2007; pp. 114105-1-114105-3; vol. 90, No. 114105; American Institute of Physics.
- Mathieu, J-B.; Martel, S.; Yahia, L'H.; Soulez, G.; Beaudoin, G.; "MRI Systems as a Mean of Propulsion for a Microdevice in Blood Vessels"; bearing a date of 2003; pp. 3419-3422; IEEE.
- Matsui, Takemi; Matsumura, Kouji; Hagiwara, Kousuke; Ishihara, Masayuki; Ishizuka, Toshiaki; Suzuki, Minoru; Kurita, Akira; Kikuchi, Makoto; "A Novel Ferromagnetic Thermo-Stent for Plaque Stabilization That Self-Regulates the Temperature"; IEEE Transactions on Biomedical Engineering; bearing dates of Jun. 2002 and 2002; pp. 621-623; vol. 49, No. 6; IEEE.
- McNeal, Donald R.; "Analysis of a Model for Excitation of Myelinated Nerve"; IEEE Transactions on Biomedical Engineering; bearing a date of Jul. 1976; pp. 329-337; vol. BME-23, No. 4.
- Meier, P.; Oberthür, S.; Lang, M.; "Development of a compliant device for minimally invasive surgery"; Proceedings of the 28th IEEE EMBS Annual International Conference; bearing dates of Aug. 30, 2006-Sep. 3, 2006 and 2006; pp. 331-334; IEEE.
- "MEMS at the cutting edge®; Patent Pending"; VERIMETRA; pp. 1-2; <http://www.verimetra.com/flow.htm>; printed on May 4, 2006.
- Menciassi, A.; Park, Jong H.; Lee, S.; Gorini, S.; Dario, P.; Park, Jong-Oh; "Robotic Solutions and Mechanisms for a Semi-Autonomous Endoscope"; Proceedings of the 2002 IEEE/RSJ International Conference on Intelligent Robots and Systems; bearing a date of 2002; pp. 1379-1384; IEEE.
- Mohseni, Kamran; "Biomimetic & Bio-Inspired Aerial and Underwater Vehicles"; bearing a date of Sep. 23, 2006; pp. 1-10; printed on Jan. 4, 2007; <http://enstrophy.colorado.edu/~mohseni/MicroVehicles1.html#UUV1#UUV1>.
- Mosse, Charles; Mills, Tim; Appleyard, Mark; Swain, Paul; "Electrostimulation to move endoscopes in the small bowel"; Proceedings of SPIE; bearing a date of 2001; pp. 24-28; vol. 4158.
- Murthy, S. Narasimha; Hiremath, Shobha Rani R.; "Physical and Chemical Permeation Enhancers in Transdermal Delivery of Terbutaline Sulphate"; AAPS PharmSciTech; bearing a date of 2001; pp. 1-5; vol. 2(1); Technical Note 1; <http://www.pharmscitech.com/>.
- Nakayama, Yasuhide; Ji-Youn, Kim; Nishi, Shogo; Ueno, Hikaru; Matsuda, Takehisa; "Development of high-performance stent: gelatinous photogel-coated stent that permits drug delivery and gene transfer"; J Biomed Mater Res; bearing dates of Nov. 13, 2000, Apr. 23, 2001, May 10, 2001 and 2001; pp. 559-566; vol. 57; John Wiley & Sons, Inc.
- Naqvi, Nasir H.; Rudrauf, David; Damasio, Hanna; Bechara, Antoine; "Damage to the Insula Disrupts Addiction to Cigarette Smoking"; Science; bearing a date of Jan. 26, 2007; pp. 531-534; vol. 315, No. 531; www.sciencemag.org; printed on Jan. 25, 2007.
- Neto, A.M. Figueiredo; Godinho, M.H.; Toth-Katona, T.; Palfy-Muhoray, P.; "Optical, Magnetic and Dielectric Properties of Non-

- Liquid Crystalline Elastomers Doped with Magnetic Colloids"; *Brazilian Journal of Physics*; Bearing a date of Mar. 2005; pp. 184-189; vol. 35, No. 1.
- "New Medical Device Combines Wireless and MEMS Technology"; Georgia Institute of Technology; pp. 1-4; PhysOrg.com; <http://www.physorg.com/printnews.php?newsid=10533>; printed on Feb. 20, 2006.
- Nieuwenhuizen-Berkovits, P., "Lubrelastic medical appliances"; *Lubrelastic Medical Appliances*; pp. 1-4; <http://www.xs4all.nl/~plien070/caeng.html>; printed on Feb. 20, 2006.
- Nyitrai, Zsolt; Illyefalvi-Vitéz, Zsolt; Pinkola, János; "Preparing Stents with Masking & Etching Technology"; 26th International Spring Seminar on Electronics Technology; bearing dates of May 8, 2003-May 11, 2003 and 2003; pp. 321-324; IEEE.
- Olsson III, R.H.; Gulari, M.N.; Wise, K.D.; "Poster 114: Silicon Neural Recording Arrays with On-Chip Electronics for In-Vivo Data Acquisition"; *Microtechnologies in Medicine and Biology*; bearing dates of May 2, 2002-May 4, 2002; pp. 237-240; IEEE.
- Oweiss, Karim G.; Anderson, David J.; "A New Technique for Blind Source Separation Using Subband Subspace Analysis in Correlated Multichannel Signal Environments"; bearing a date of 2001; pp. 2813-2816; IEEE.
- Patronik, N.A.; Ota, T.; Zenati, M.A.; Riviere, C.N.; "Improved Traction for a Mobile Robot Traveling on the Heart"; *Proceedings of the 28th IEEE EMBS Annual International Conference*; bearing dates of Aug. 30, 2006-Sep. 3, 2006 and 2006; pp. 339-342; IEEE.
- PCT International Search Report App. No. PCT/US05/33475; dated Sep. 5, 2006; pp. 1-2.
- Peckham, P. Hunter; Knutson, Jayme S.; "Functional Electrical Stimulation for Neuromuscular Applications"; *Annual Review Biomedical Engineering*; bearing a date of 2005; pp. 327-360; vol. 7; *Annual Reviews*.
- Rattay, F.; "The Basic Mechanism for the Electrical Stimulation of the Nervous System"; *Neuroscience*; 1999; pp. 335-346; vol. 98. No. 2; Elsevier Science Ltd; printed on Mar. 15, 2007.
- Rattay, Frank; Aberham, Matthias; "Modeling Axon Membranes from Functional Electrical Stimulation"; *IEEE Transactions on Biomedical Engineering*; bearing a date of Dec. 1993; pp. 1201-1209; vol. 40, No. 12; IEEE.
- Rattay, Frank; "Analysis of Models for Extracellular Fiber Stimulation"; *IEEE Transactions on Biomedical Engineering*; bearing a date of Jul. 1989; pp. 676-682; vol. 36, No. 7; IEEE.
- "Remote-Control Electrostimulation Capsule"; *Popular Science*; bearing dates of 2002 and 2003; pp. 1-2; <http://www.popsci.com/popsci/brown/2003/article/0,18881,537028,00.html>; printed on May 4, 2006.
- "Researchers: Squid-Inspired Vortex Generators Could Mean Better Propulsion for Unmanned Underwater Vehicles"; *UnderwaterTimes.com*; Dec. 12, 2006; pp. 1-2; *UnderwaterTimes.com*; printed on Jan. 4, 2007; http://www.underwatertimes.com/print.php?article_id=51030782641.
- Rice, Mike; "Implantable Neurostimulation Device Market Poised for Explosive Growth"; *Future Fab International*; Jan. 7, 2006; pp. 1-4; printed on Oct. 6, 2006; http://www.future-fab.com/documents.asp?d_ID=3725.
- Rice, Mike; "New Products, Emphasis on Miniaturization Driving Medical Device Innovation"; bearing a date Aug. 23, 2006; pp. 1-3; *Advantage Business Media*; <http://www.mdtmag.com/scripts/ShowPR.asp?PUBCODE=046&ACCT=0006109&ISSUE=0603&RELTYPE=PR&PRODCODE=0790&PRODLETT=A>; printed on Aug. 23, 2006.
- Riedmüller, J.; Bolz, A.; Rebling, H.; Schaldach, M.; "Improvement of Stimulation and Sensing Performance of Bipolar Pacemaker Leads"; *IEEE Eng. Med. Biol. Soc.*; 1992; pp. 2364-2365; IEEE.
- Robinson, David A.; "The Electrical Properties of Metal Microelectrodes"; *Proceedings of the IEEE*; bearing a date of Jun. 1968; pp. 1065-1071; vol. 56, No. 6.
- Rousche, Patrick J.; Pellinen, David S.; Pivin, David P.; Williams, Justin C.; Vetter, Rio J.; Kipke, Daryl R.; "Flexible Polyimide-Based Intracortical Electrode Arrays with Bioactive Capability"; *IEEE Transactions on Biomedical Engineering*; bearing a date Mar. 2001; pp. 361-371; vol. 48, No. 3; IEEE.
- Rutten, Wim; Mouveroux, Jean-Marie; Buitenweg, Jan; Heida, Ciska; Ruurdij, Teun; Marani, Enrico; Lakke, Egbert; "Neuroelectronic Interfacing with Cultured Multielectrode Arrays Toward a Cultured Probe"; *Proceedings of the IEEE*; bearing a date of Jul. 2001; pp. 1013-1029; vol. 89, No. 7; IEEE.
- Saltzman, John R.; "Endoscopic Advances—A View Toward the Future"; bearing dates of May 4, 2006, May 17, 2005, and 2005; pp. 1-4; *Medscape*; <http://www.medscape.com/viewarticle/505100>; printed on May 4, 2006.
- Schmidt, W.; Behrens, P.; Behrend, D.; Schmitz, K.-P.; Andresen, R.; "Experimental Study of Peripheral, Balloon-expandable Stent Systems"; *Progress in Biomedical Research*; bearing a date of May 2001; pp. 246-255.
- Schoonhoven, R.; Stegeman, D.F.; "Models and Analysis of Compound Nerve Action Potentials"; *Critical Reviews in Biomedical Engineering*; bearing a date of 1991; pp. 47-111; vol. 19, No. 1; CRC Press, Inc.
- Senel, Sevda; Hincal, A. Atilla; "Drug permeation enhancement via buccal route: possibilities and limitations"; *Journal of Controlled Release*; bearing a date of 2001; pp. 133-144; vol. 72 (2001); Elsevier; www.elsevier.com/locate/jconrel.
- Serruya, Mijail D.; Hatsopoulos, Nicholas G.; Paninski, Liam; Fellows, Matthew R.; Donoghue, John P.; "Brief Communications: Instant Neural Control of a Movement Signal"; *Nature*; bearing a date of Mar. 14, 2002; pp. 141-142; vol. 416; Macmillan Magazines Ltd; www.nature.com.
- Serruys, Patrick W.; Kutryk, Michael J.B.; Ong, Andrew T.L.; "Coronary-Artery Stents"; *The New England Journal of Medicine*; bearing dates of Feb. 2, 2006 and Feb. 15, 2006; pp. 483-495; vol. 354;5; Massachusetts Medical Society.
- Shabalovskaya, Svetlana, A.; "Surface, corrosion and biocompatibility aspects of Nitinol as an implant material"; *Bio-Medical Materials and Engineering*; bearing dates of Apr. 4, 2001, and 2002; pp. 69-109; vol. 12; IOS Press.
- Shahinpoor, Mohsen; Kim, Kwang J.; Ionic polymer-metal composites: IV. Industrial and medical applications; *Smart Materials and Structures*; 2005; pp. 197-214; vol. 14; Institute of Physics Publishing.
- Smith, Michael; "PAS: Nasal Spray Flu Vaccine Seems Safe and Effective in Young"; May 2, 2006; pp. 1-2; *MedPage Today, LLC*; bearing dates of 2004-2006; printed on May 4, 2006; <http://www.medpagetoday.com/tbprint.cfm?tbid=3213>.
- Snoek, G.J.; Ijzerman, M.J.; In 't Groen, Fag; Stoffers, T.S.; Zilvold, G.; "Use of the NESS Handmaster to Restore Handfunction in Tetraplegia: Clinical Experiences in Ten Patients"; *Spinal Cord*; bearing a date of 2000; pp. 244-249; vol. 38; International Medical Society of Paraplegia.
- Snow, E.S.; Perkins, F.K.; Houser, E.J.; Badescu, S.C.; Reinecke, T. L.; "Chemical Detection with a Single-Walled Carbon Nanotube Capacitor"; *Science*; Mar. 25, 2005; pp. 1942-1945; vol. 307; www.sciencemag.org.
- Stoeckel, Dieter; Pelton, Alan; Duerig, Tom; "Self-expanding nitinol stents: material and design considerations"; *European Radiology*; bearing dates of Jan. 28, 2003, May 22, 2003, Jul. 1, 2003, Sep. 3, 2003, Feb. 2004 and 2004; pp. 292-301(1-2); vol. 14, No. 2; Springer-Verlag GmbH-SpringerLink—Article; [http://www.springerlink.com/\(1begg455gtgjfseqqptyb43m\)/app/home/contribution.asp?referrer=parent&backto=issue,17,26;journal,27,147;browsepublicationsresults,444,1551](http://www.springerlink.com/(1begg455gtgjfseqqptyb43m)/app/home/contribution.asp?referrer=parent&backto=issue,17,26;journal,27,147;browsepublicationsresults,444,1551); printed on Feb. 22, 2006.
- Strauss, Bradley H., M.D.; Li, Chris, M.D.; Whittingham, Heather A., M.Sc.; Tio, Fermin O., M.D.; Kutryk, Michael J.B., M.D.; Ph.D.; Janicki, Christian, Ph.D.; Sparkes, John, D., M.Sc.; Turnlund, Todd, B.Sc.; Sweet, William L., M.D.; "Late Effects of Low-Energy Gamma-Emitting Stents in a Rabbit Iliac Artery Model"; *Int. J. Radiation Oncology Biol. Phys.*; bearing dates of Oct. 23, 2001, May 13, 2002 and May 15, 2002 and 2002; pp. 551-561; vol. 54, No. 2; Elsevier Science Inc.
- Struijk, Johannes Jan; "The Extracellular Potential of a Myelinated Nerve Fiber in an Unbounded Medium and in Nerve Cuff Models"; *Biophysical Journal*; bearing a date of Jun. 1997; pp. 2457-2469; vol. 72; Biophysical Society.

- Taylor, Dawn M.; Helms Tillery, Stephen I.; Schwartz, Andrew B.; "Research Article: Direct Cortical Control of 3D Neuroprosthetic Devices"; Science; bearing a date of Jun. 7, 2002; pp. 1829-1832; vol. 296; www.sciencemag.org.
- "Tiny Robot Reduces Need for Surgery"; Pink Tentacle; bearing a date of Feb. 26, 2007; p. 1; <http://www.pinktentacle.com/2007/02/tiny-robot-reduces-need-for-surgery/>; printed on Mar. 8, 2007.
- "Trying to control pain can be a double-edged sword, say scientists"; PhysOrg.com; printed on Nov. 2, 2006; pp. 1-2; <http://www.physorg.com/printnews.php?newsid=81599312>.
- Tummala, R. Lal; Mukherjee, R.; Aslam, D.; Xi, Ning; Mahadevan, S.; Weng, J.; "Reconfigurable Adaptable Micro-robot"; IEEE; bearing a date of 1999; pp. 687-691.
- Twardoch, U.M.; "Integrity of Ultramicro-Stimulation Electrodes Determined from Electrochemical Measurements"; Journal of Applied Electrochemistry; bearing a date of 1994; pp. 835-857; vol. 24; Chapman & Hall.
- Warland, David K.; Reinagel, Pamela; Meister, Markus; "Decoding Visual Information from a Population of Retinal Ganglion Cells"; bearing a date of 1997; pp. 2336-2350; The American Physiological Society.
- Weis, Rolf; Müller, Bernt; Fromherz, Peter; "Neuron Adhesion on a Silicon Chip Probed by an Array of Field-Effect Transistors"; Physical Review Letters; bearing a date of Jan. 8, 1996; pp. 327-330; vol. 76, No. 2; The American Physical Society.
- Wessberg, Johan; Stambaugh, Christopher R.; Kralik, Jerald D.; Beck, Pamela D.; Laubach, Mark; Chapin, John K.; Kim, Jung; Biggs, S. James; Srinivasan, Mandayam A.; Nicolelis, Miguel A.L.; "Letters to Nature: Real-Time Prediction of Hand Trajectory by Ensembles of Cortical Neurons in Primates"; Nature; bearing a date of Nov. 16, 2000; pp. 361-365; vol. 408; Macmillan Magazines Ltd; www.nature.com.
- White, Dave; "Mini Robot Explores, Gives you Medicine from Within"; Mobile Magazine; bearing a date of Feb. 27, 2007; p. 1; <http://www.mobilemag.com/content/100/313/C11869/>; printed on Mar. 8, 2007.
- Yusa, Go; Muraki, Koji; Takashina, Kei; Hashimoto, Katsushi; Hirayama, Yoshiro; "Controlled multiple quantum coherences of nuclear spins in a nanometre-scale device"; Nature; Apr. 21, 2005; pp. 1001-1005; vol. 434; 2005 Nature Publishing Group; www.nature.com/nature.
- "Zyvex NanoEffector Microgrippers"; Nanotechnology at Zyvex; printed on Dec. 7, 2006; pp. 1-2; http://www.zyvex.com/Products/Grippers_Features.html.
- "Zyvex NanoEffector Microgrippers"; Zyvex.com; bearing a date of 2006; pp. 1-2; Zyvex Corporation.
- U.S. Appl. No. 12/075,480, Hillis et al.
- U.S. Appl. No. 11/891,573, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/891,371, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/891,356, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/891,355, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/891,334, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/891,333, Wood, Jr., Lowell L.
- U.S. Appl. No. 11/726,031, Ferren et al.
- U.S. Appl. No. 11/726,025, Ferren et al.
- U.S. Appl. No. 11/725,982, Ferren et al.
- UK Intellectual Property Office Examination Report Under Section 18(3), App. No. GB0821523.8; Jul. 2, 2009; pp. 1-2.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821519.6; Nov. 12, 2009; pp. 1-4.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821526.1; Nov. 11, 2009; pp. 1-5.
- UK Examination Report Under Section 18(3); App. No. GB0821524.6; bearing a date of May 6, 2010; pp. 1-3.
- UK Intellectual Property Examination Report Under Section 18(3); App. No. GB0706802.6; Nov. 23, 2009; pp. 1-2.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821526.1; bearing a date of Jul. 15, 2010; pp. 1-2.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821524.6; Aug. 9, 2010 (received by our Agent on Aug. 10, 2010); pp. 1-2.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821519.6; Aug. 9, 2010 (received by our Agent on Aug. 10, 2010); pp. 1-3.
- UK Intellectual Property Office Examination Report Under Section 18(3); App. No. GB0821530.3; Aug. 27, 2010 (received by our Agent on Sep. 3, 2010); pp. 1-6.

* cited by examiner

FIG. 1

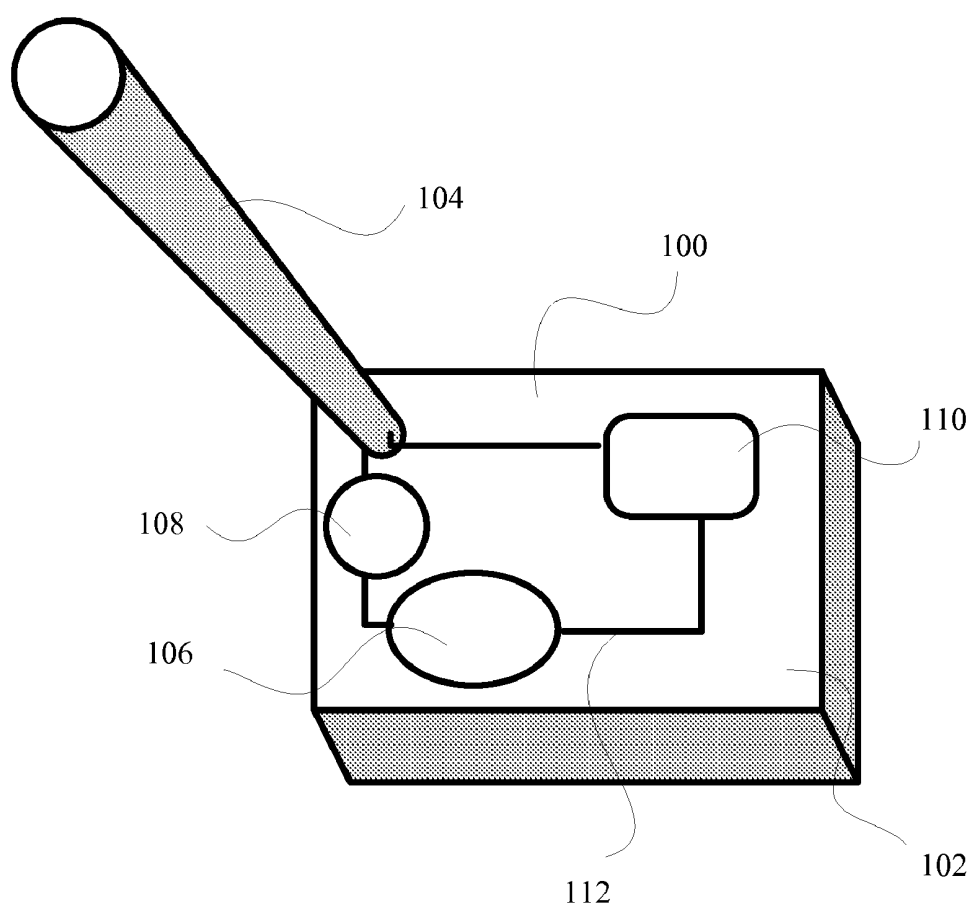
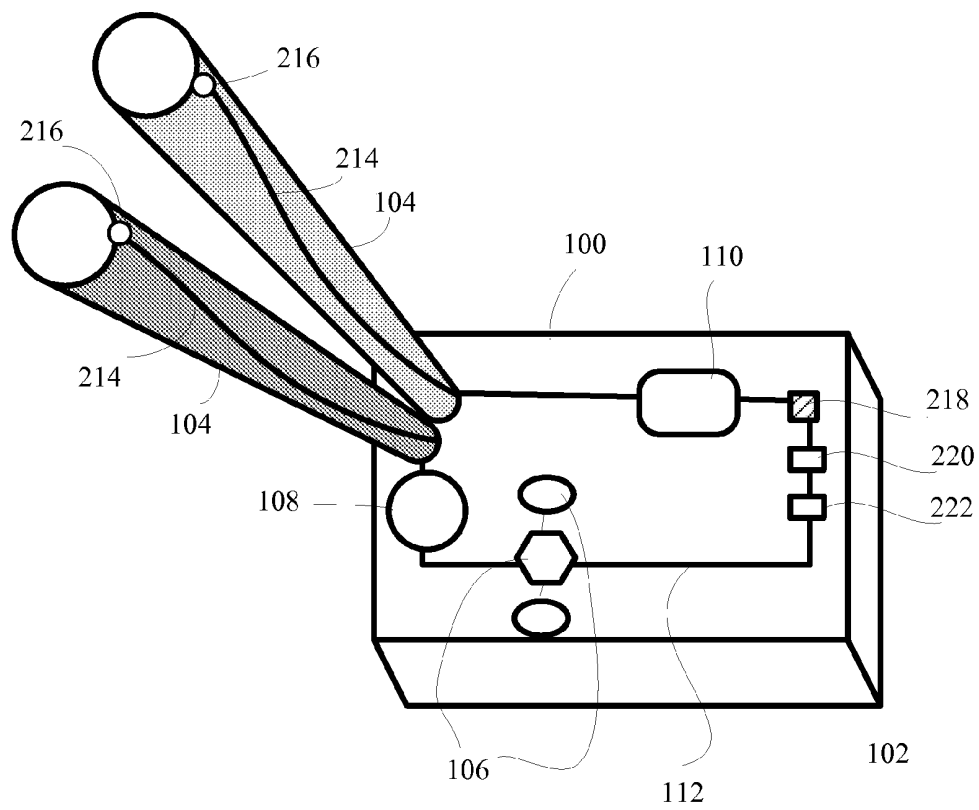


FIG. 2



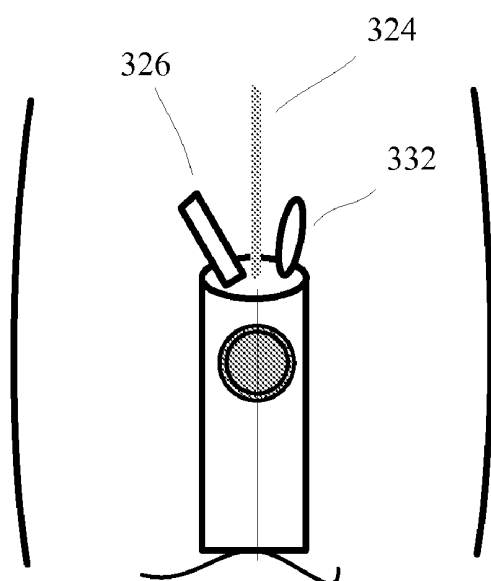


FIG. 3A

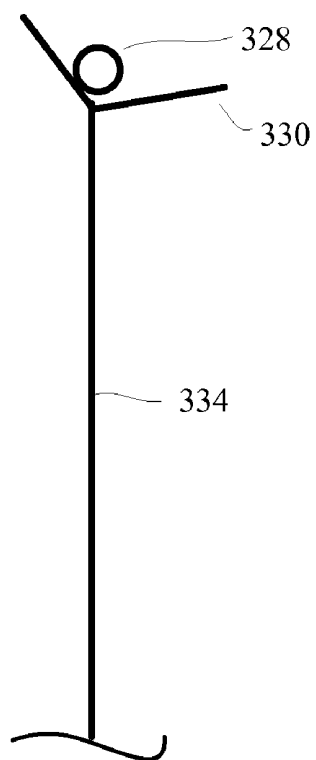


FIG. 3B

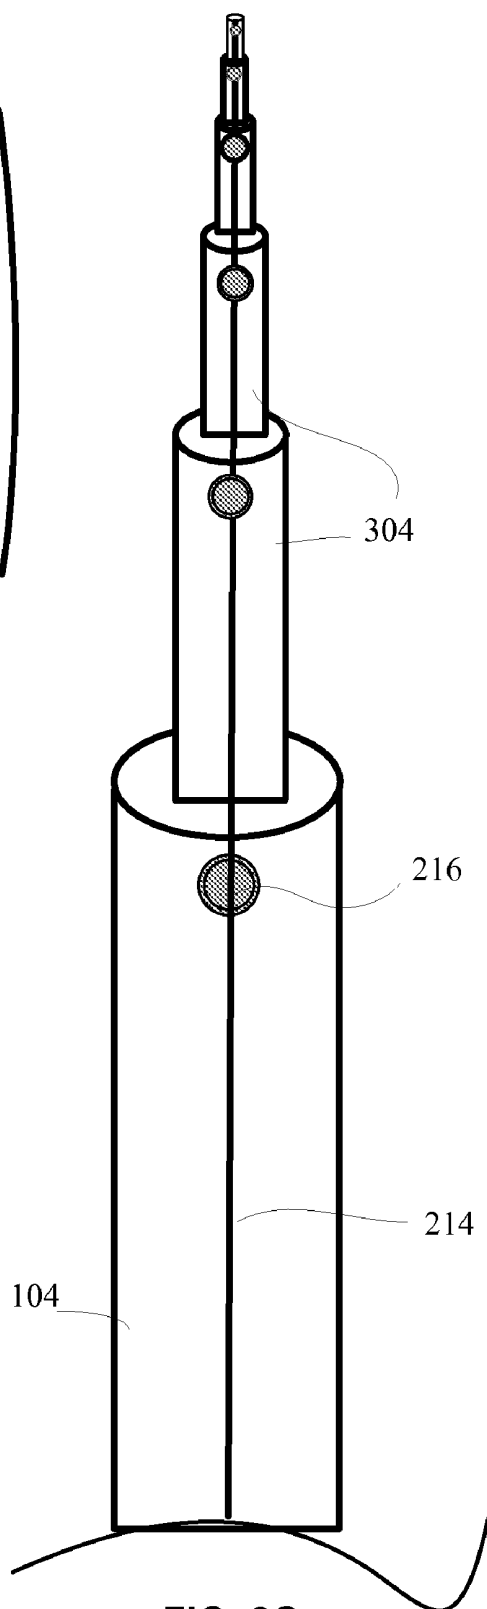


FIG. 3C

FIG. 4


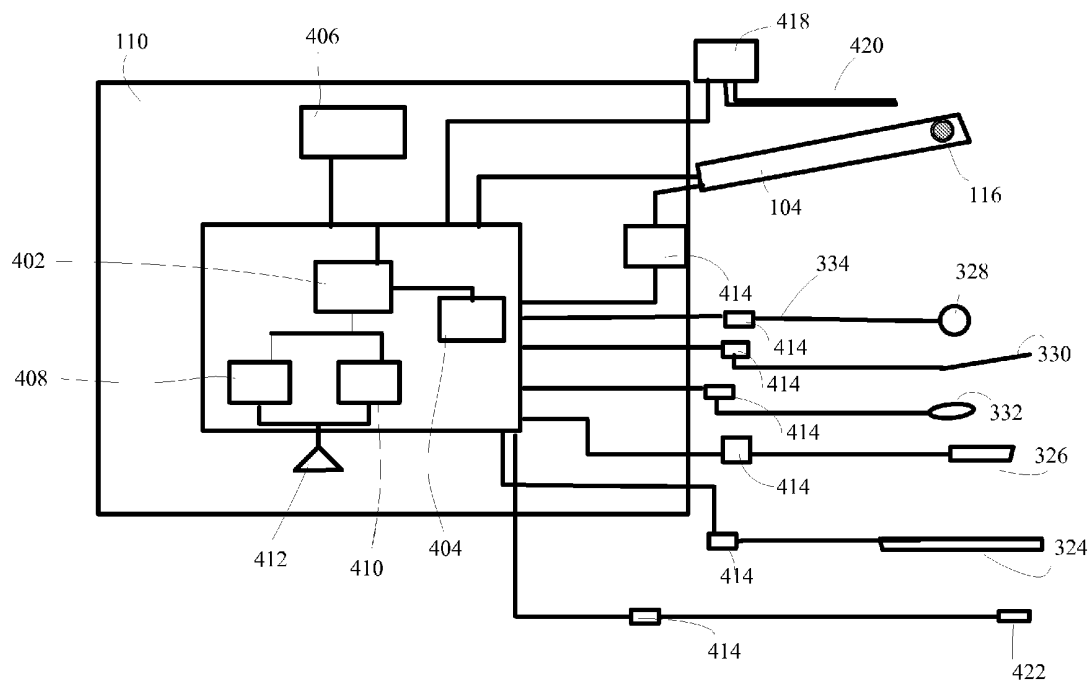


FIG. 5

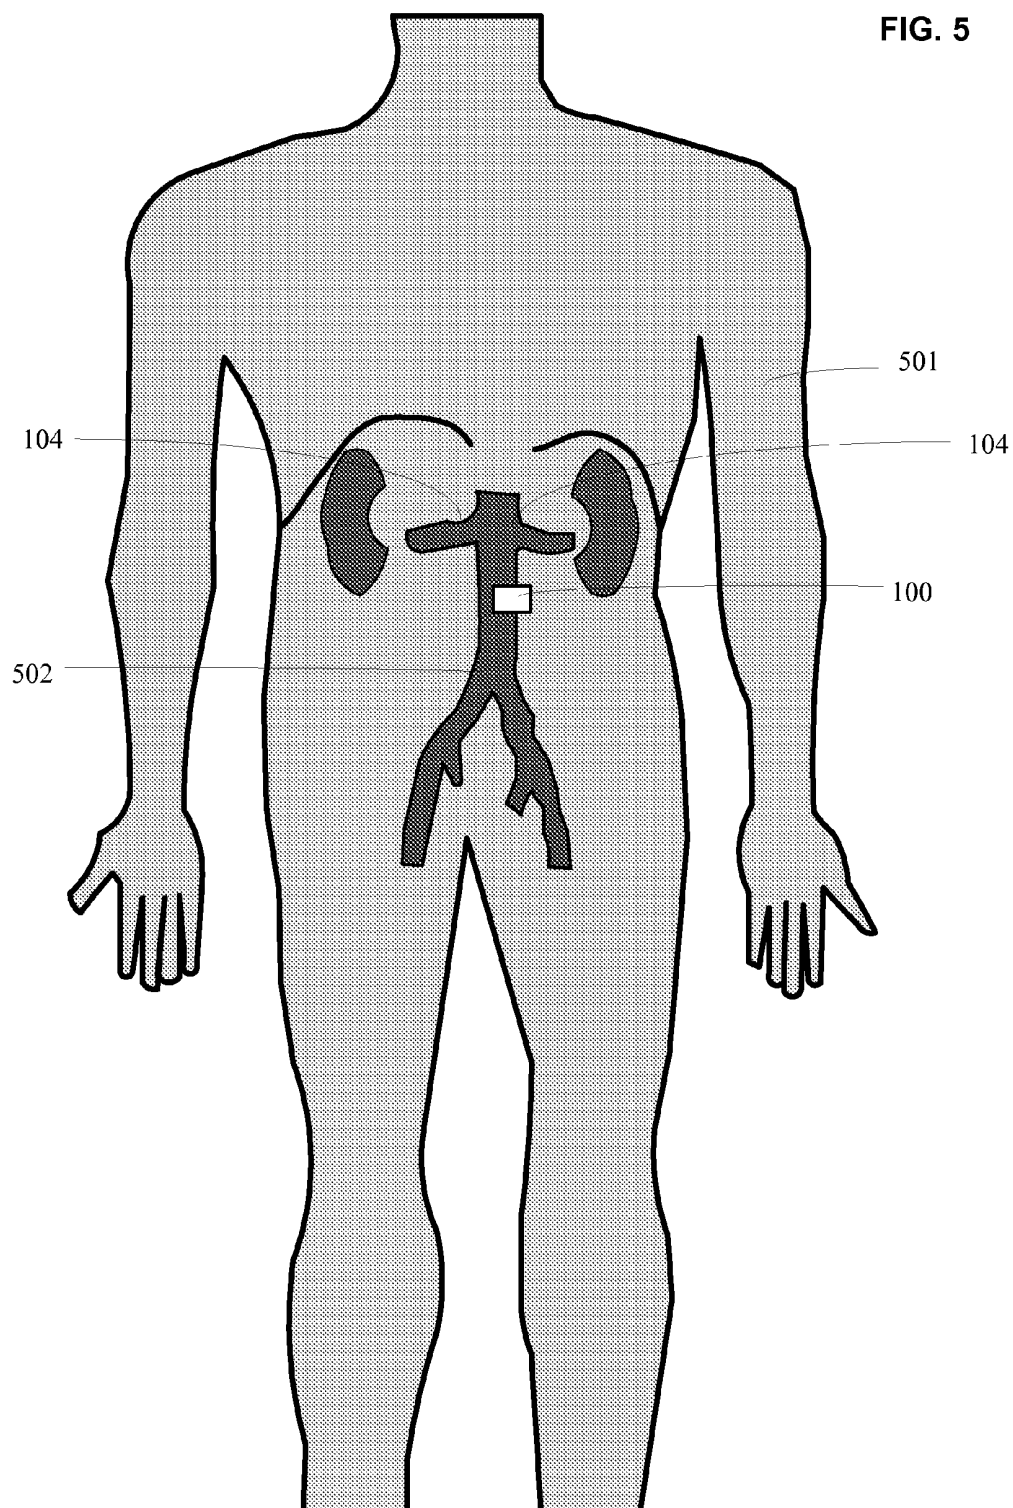

SYSTEM WITH A RESERVOIR FOR PERFUSION MANAGEMENT

CROSS-REFERENCE TO RELATED APPLICATIONS

The present application is related to, claims the earliest available effective filing date(s) from the following listed application(s) (the "Related Applications") (e.g., claims earliest available priority dates for other than provisional patent applications or claims benefits under 35 USC §119(e) for provisional patent applications), and incorporates by reference in its entirety all subject matter of the following listed application(s); the present application also claims the earliest available effective filing date(s) from, and also incorporates by reference in its entirety all subject matter of any and all parent, grandparent, great-grandparent, etc. applications of the "Related Application(s)."

RELATED APPLICATIONS

1. For purposes of the USPTO extra-statutory requirements, the present application constitutes a continuation-in-part of U.S. patent application Ser. No. 10/827,576, entitled A SYSTEM FOR PERFUSION MANAGEMENT, naming Lowell L. Wood Jr. as inventor, filed 19 Apr. 2004, which is currently co-pending, or is an application of which a currently co-pending application is entitled to the benefit of the filing date.
2. For purposes of the USPTO extra-statutory requirements, the present application constitutes a continuation-in-part of U.S. patent application Ser. No. 10/827,578, entitled A SYSTEM WITH A SENSOR FOR PERFUSION MANAGEMENT, naming Lowell L. Wood Jr. as inventor, filed 19 Apr. 2004, which is currently co-pending, or is an application of which a currently co-pending application is entitled to the benefit of the filing date.
3. For purposes of the USPTO extra-statutory requirements, the present application constitutes a continuation-in-part of U.S. patent application Ser. No. 10/827,390, entitled A TELESCOPING PERFUSION MANAGEMENT SYSTEM, naming Lowell L. Wood, Jr. as inventor, filed 19 Apr. 2004, which is currently co-pending, or is an application of which a currently co-pending application is entitled to the benefit of the filing date.

The United States Patent Office (USPTO) has published a notice to the effect that the USPTO's computer programs require that patent applicants reference both a serial number and indicate whether an application is a continuation or continuation-in-part. Stephen G. Kunin, *Benefit of Prior-Filed Application*, USPTO Official Gazette Mar. 18, 2003. The present Applicant Entity (hereinafter "Applicant") has provided above a specific reference to the application(s) from which priority is being claimed as recited by statute. Applicant understands that the statute is unambiguous in its specific reference language and does not require either a serial number or any characterization, such as "continuation" or "continuation-in-part," for claiming priority to U.S. patent applications. Notwithstanding the foregoing, Applicant understands that the USPTO's computer programs have certain data entry requirements, and hence Applicant is designating the present application as a continuation-in-part of its parent applications as set forth above, but expressly points out that such designations are not to be construed in any way as any type of commentary and/or admission as to whether or not the present application contains any new matter in addition to the matter of its parent application(s).

All subject matter of the Related Applications and of any and all parent, grandparent, great-grandparent, etc. applications of the Related Applications is incorporated herein by reference to the extent such subject matter is not inconsistent herewith.

TECHNICAL FIELD

The present application relates, in general, to detection and/or treatment.

SUMMARY

In one aspect, a system includes but is not limited to: a body portion; at least one extensible finger coupled to said body portion; at least one reservoir in communication with said extensible finger; and a control circuitry coupled to said extensible finger, or said body portion. In addition to the foregoing, other system aspects are described in the claims, drawings, and text forming a part of the present application.

In one aspect, a method includes but is not limited to: fabricating a device by forming a cavity for storing a receivable; coupling a flexible conduit to said cavity, the conduit being configured to extend from said cavity to a target location in an animal's body; and coupling said flexible conduit and said cavity to a monitoring system, said monitoring system including logic or software configured for directing said receivable from said cavity to said target location. In addition to the foregoing, other method aspects are described in the claims, drawings, and text forming a part of the present application.

In another aspect, a method includes but is not limited to: storing a receivable in an implanted storage medium; extending a flexible conduit between said storage medium and a target location; and transmitting said receivable from said storage medium to said target location. In addition to the foregoing, other method aspects are described in the claims, drawings, and text forming a part of the present application.

In one or more various aspects, related systems include but are not limited to circuitry and/or programming for effecting the herein-referenced method aspects; the circuitry and/or programming can be virtually any combination of hardware, software, and/or firmware configured to effect the herein-referenced method aspects depending upon the design choices of the system designer.

In addition to the foregoing, various other method and or system aspects are set forth and described in the text (e.g., claims and/or detailed description) and/or drawings of the present application.

The foregoing is a summary and thus contains, by necessity, simplifications, generalizations and omissions of detail; consequently, those skilled in the art will appreciate that the summary is illustrative only and is NOT intended to be in any way limiting. Other aspects, inventive features, and advantages of the devices and/or processes described herein, as defined solely by the claims, will become apparent in the non-limiting detailed description set forth herein.

BRIEF DESCRIPTION OF THE FIGURES

FIG. 1 is a front-plan view of a device for perfusion management 100.

FIG. 2 is a front-plan view of another aspect of the device for perfusion management 100.

FIGS. 3A, 3B, and 3C show exploded views of various aspects of the device of FIG. 1 including an extensible finger 104.

FIG. 4 is a schematic view of the control circuit 110 and devices in communication with the control circuit 110.

FIG. 5 illustrates an example wherein the device for perfusion management 100 is placed in a selected location in a human body 501.

The use of the same symbols in different drawings typically indicates similar or identical items.

DETAILED DESCRIPTION

The present application uses formal outline headings for clarity of presentation. However, it is to be understood that the outline headings are for presentation purposes, and that different types of subject matter may be discussed throughout the application (e.g., device(s)/structure(s) may be described under the process(es)/operations heading(s) and/or process(es)/operations may be discussed under structure(s)/process(es) headings). Hence, the use of the formal outline headings is not intended to be in any way limiting.

1. Perfusion Management Device(s) and/or Process(es).

With reference now to FIG. 1, shown is a front plan view illustrative of various exemplary perfusion management device(s) and/or process(es). Accordingly, the present application first describes certain specific exemplary structures of FIG. 1; thereafter, the present application illustrates certain specific exemplary processes. Those having skill in the art will appreciate that the specific devices and processes described herein are intended as merely illustrative of their more general counterparts.

A. Structure(s) and or Device(s)

With reference to the figures, and with reference now to FIG. 1, shown is a front-plan view of a device for perfusion management 100. The device for perfusion management 100 includes a body portion 102 from which at least one extensible finger 104 projects. At least one reservoir 106 within the body portion 102 contains a fluid, for example, a fluid for treatment. A controllable valve 108 provides a path through which the fluid may travel to the at least one extensible finger 104. A control circuit 110 provides a control signal that may open or close the control valve 108.

Referring now to FIG. 2, depicted is an aspect of the device for perfusion management 100 which includes a body portion 102 from which a set of extensible fingers projects. In one aspect, at least one of the extensible finger 104 of the set of extensible fingers has a sensor 216 at the distal end of the at least one of the extensible finger 104. Additionally, a sense line 214 connects the control circuit 110 to the sensor 216 at the distal end of the extensible finger 104. The control circuit 110 may be connected to a sense line 214 that allows it to monitor the fluid levels within the at least one reservoir 106.

Continuing to refer to FIG. 2, in one aspect, each of the extensible finger 104 of the set of extensible fingers is in fluid communication with at least one of a respective reservoir 106 filled with a different fluid for delivery. In another approach, the at least one reservoir 106 may be coupled to a mixing chamber where the fluid contents of the at least one reservoir 106 are present for mixing and the mixed contents enter the extensible finger 104 for delivery to a selected location. The choice of the fluid in the at least one reservoir 106 may depend, for example, on the purpose of the device, for example, treatment of colon cancer, treatment of breast cancer, or treatment of an arterial disease. The choice of fluid in the reservoir 106 includes, but is not limited to, for example, a chemical, a chemical compound, a protein, a lipoprotein, a glycoprotein, a sugar, a lipid, an antigen, an antibody, a cytokine, a peptide, a neurotransmitter, a hormone, an ion, a messenger molecule, a nucleic acid, an engineered nucleic acid,

a nucleic acid vector, a drug, a cell, a cell fragment, a cell organelle, a liposome, a pharmaceutical agent, a biological material, or a biological fraction. The reservoir 106 may also be utilized for storage and disposal of operational fluids. Also, although the exemplary embodiment described herein focuses primarily on fluid delivery, one skilled in the art will understand that fluid-like substances, such as gels, and fluidizable substances or non-fluid type substances, such as small solid particles, may be delivered in accordance with the invention. It will also be appreciated by those having skill in the art that the nature of the fluid in the reservoir 206 includes, for example, and is not limited to, a liquid, a solution, a mixture, a gel, a colloid, a colloid of a suitable viscosity, a suspension, an emulsion, or any material of low shear-strength for delivery to a site.

In one aspect one or more fluids are delivered to one or more of selected locations by the device for perfusion management 100. The selected location may be, for example, in proximity to or within a tumor, a circulatory system, an aorta, a vena cava, a site of therapy, or a site of investigation in an animal.

Continuing to refer to FIG. 2, a pump 218 provides fluid at a controlled flow rate for delivery to a site from the reservoir 106. It will be appreciated by those skilled in the art that the type of pump is not critical to the invention and may include, for example, a mechanical pump, a piezoelectric pump, an osmotic pump, a source of pressure, or a device for maintaining a positive flow of fluid through the device. Additionally, fluid flow may be further modulated with micro valves and self-pressurizing fluidic reservoirs. Moreover, in some applications, the fluid may be delivered without a pump. For example, fluid delivery may be controlled using a pressurized bladder, controlled dissolution or dilution of a material, a drip or gravity type of approach, or any other suitable approach to deliver the appropriate amount or an appropriate delivery-rate of the fluid.

With reference now to FIG. 3, depicted is an exploded view of the extensible finger 104 showing a plurality of telescoping segments 304 with the sensor 216 at the distal end of each of the telescoping segments 304. In one aspect of the invention, the sensor 216 is an array of sensors, deployed from one or more portholes, at the distal end of each of the telescoping segments 304. In one approach, the portholes are sized and shaped to provide access through which the sensors 216 may be deployed. The portholes may include seals, stress relief or other features appropriate for proper mechanical deployment. In one approach, one or more of the portholes can be controllably opened or closed to provide communication exterior to the extensible finger or main body. The sensor 216 may be retracted within the port hole and deployed through the porthole. Where the porthole can be opened and closed, the porthole can close to limit communication and can be opened for deployment. The array of sensors may include, but is not limited to, for example, sensors for detecting pressure, temperature, chemical, gas, electrolyte, flow, volume, composition, or concentration. In an alternate aspect of the invention, microelectrodes, such as, for example, solid-state microelectrodes are sensitized with an agent for detecting a relevant interactor. Examples of the agent include, but are not limited to, for example, agonists of angiogenesis. The choice of sensor 216 depends on the physiological variable being monitored, treated, or controlled. The term "physiological variable" refers to any and all measurements relating to the functioning of a living organism under normal, sub-normal, or abnormal states.

Continuing to refer to FIG. 3 and referring now to FIG. 4, an operative tool 324 is coupled to the distal most telescoping

segment **304**, or deployed from the porthole, or carried by the extensible finger **104**, further including a carrying line **334** in communication with the control circuit **110**. The operative tool **324** includes, but is not limited to, for example, one or more of a combination of, a tool positioner, an ablation device, a laser, a vacuum, a siphon **326**, an evacuation device, a fluid dispenser **328**, a cauterizer **330**, a stent **332**, a tissue-liquefying device, or a source of an electric or an electromagnetic charge **422**. The vacuum or the siphon is employed for removing a cell, a mass of cells, a tissue, a fluid, a gel, a sample, a debris, a contaminant, or other material for which removal is desired or appropriate. The ablation device operates for perturbing or reducing the structural integrity or viability of a cell, a mass of cells, an assembly of biological materials exhibiting shear strength, or a tissue. The assembly of biological materials includes, for example, blood clots, cartilage, or bone. The source of an electric or electromagnetic charge **422** includes, but is not limited to, for example, steady state electric currents, time-varying electric currents, alternating electric currents, radio waves, microwaves, ultraviolet rays, infra-red rays, optical rays, terahertz beams, and the like.

Continuing to refer to FIG. 3, it will be appreciated by those having skill in the art that the operative tool **324** may include a set of devices having general or "multi-purpose" utility. The operative tool **324** may include, but is not limited to, for example, a combination of the fluid dispenser **328**, the siphon **326**, and the ablation device. In this example the operative tool combination, for example, delivers the fluid or gel, ablates cells, and removes debris.

Continuing to refer to FIG. 3, the plurality of telescoping segments **304** may themselves be hollow forming a conduit for delivery of the fluid to a site, or for housing a circuitry coupling the control circuit **110** to the operative tool **324**, or for housing a mechanism that guides the arm **104** or the plurality of telescoping segments **304**.

With reference now to FIG. 4, illustrated is a schematic view of the control circuit **110** and devices in communication with the control circuit **110**. The device for perfusion management **100** shows a data transmitter **410**, and a data receiver **408** coupled to the control circuit **110**. An antenna **412** may be used for transmitting data to the exterior wirelessly. The antenna **412** is shown diagrammatically, but may be a structure, such as a strip antenna, that may be integrated in a manner that does not impair or significantly perturb system performance. The control circuit **110** is depicted as having a processor **402** coupled to a memory **404** that provides data storage and retrieval capability, and a power source **406**. Feedback circuitry or logic circuitry provides communication between the control circuit **110** and devices in communication with it. In some applications, a software program providing instructions may be stored in the memory **404** to control operation of the control circuitry or to store data gathered under control of the control circuitry. Additionally, the control circuit **110** may have components for system integrated digital data gathering, processing, storage, compression and transmission. These can provide data control capabilities and operation control capabilities. For example, the transmission components may communicate through the antenna **412** to a person, system, computer, or device exterior to the body. This communication can allow data gathered by the sensors to be displayed, stored or otherwise processed in the external environment. Additionally, this communication may allow for the processed data or a plurality of new data to be received from the exterior by the device for perfusion management **100**. Data compression can allow the control circuitry to store data

representing larger amounts of data to be stored in the memory **404** or to be transmitted to the exterior environment in a more efficient manner.

Continuing to refer to FIG. 4, one or more of the operative tools **324** are mounted on an actuator **414** which allows for the independent movement of each tool. Alternatively, one or more operative tools **324** may be mounted as a unit on one actuator **414** and moved as a group, for example, forming an aspirating-dispensing unit. For example, the fluid dispenser **328** and the siphon **326** may be mounted together as a group. The actuator **414** may be a motor, a piezo electrically driven actuator, a micromechanical or electrical effector, or the like.

Continuing to refer to FIG. 4, the extensible finger **104** may include an imaging device deployed from the porthole or from the distal end of the extensible finger **104** or carried by a carrying line **334**. The term "imaging device" being used herein to designate in general those components, circuits, assemblies and sub-assemblies comprising electrical, optical, or opto-electronic components. In one aspect, the control circuit **110** is coupled to the imaging device that includes a laser **418**, or a source of light or scene-illuminating radiation, coupled to an optical feed line **420** to illuminate an area. A charge coupled device is positioned to capture data from the illuminated area and provides an electronic signal indicative of the area imaged. Conventional circuitry then produces a digital representation that may be displayed, stored in the memory **404**, or otherwise processed. The displayed image may serve, for example, for guiding the extensible finger **104** to the selected location or for determining the efficacy of a treatment or a procedure. One skilled in the art will recognize that the imaging device described herein is exemplary of imaging devices and that other imaging devices, including for example, raster and line-scanning imagers, nonvisible spectral imagers, and fluorescence imagers, may be included.

With reference now to FIG. 5, the device for perfusion management **100** is depicted implanted in an aorta **502** with the extensible finger **104** traveling a blood vessel in a human body **501**. Additionally, the device for perfusion management **100** is configured for full or partial placement in the human body **501**. The configuration may incorporate a combination of the following criteria, including but not limited to, dimensions, composition, shape, power dissipation level, or texture. In one aspect, the body portion **102** is sized for implantation in proximity to the aorta **502** or the vena cava and the extensible finger **104** is sized for traveling a blood vessel in an animal, for example, the human body **501**. In this aspect, if the vasculature decreases two-fold, each of the telescoping segments **304** has about a two-fold decrease in diameter. The length of the extensible finger **104**, for example, depends upon the distance between the selected location and the location of the body portion **102**, and the route traveled by the extensible finger **104** to arrive at the selected location. It will be appreciated by those having skill in the art that the extensible finger **104** including the one or more of the operative tools **324** is of a size, dimension or shape operable for traveling one or more blood vessel of decreasing or increasing luminal diameter. It will also be appreciated by those having skill in the art that the extensible finger **104** and the one or more operative tool **324** may pass through the wall of the lumen, or trans-luminally, to the surrounding tissue for detecting, delivery of a treatment, or for sampling. It will also be appreciated by those having skill in the art that the trans-luminal mode described is not limited to blood vessels and includes the space or cavity of an organ or structure.

It will also be appreciated by those having skill in the art that the device for perfusion management **100** and its components, such as, for example, the extensible finger **104**, the

plurality of telescoping segments **304**, or one or more operative tools **324**, has a size, dimension, shape, material, and properties of flexion, retraction, and extension to allow for the steering, guiding, or positioning of the components of the device for perfusion management **100**. For example, the extensible finger **104** may need to be steered around an occlusion or a fork in the vasculature. In this example, the extensible finger **104** may need to be retracted, repositioned and then extended in a new direction. Extending, retracting or repositioning of the extensible finger **104** may be accomplished by techniques known in the art, for example, by using a guide wire or a by employing a shape polymer. In another aspect, the extensible finger may be retracted and then "punched through" an occlusion to dislodge it. In this example, lasers, shears, or a drug may be employed to degrade the occlusion. In this example, subsequent to the dislodgement and degradation of the occlusion, the siphon **326** or an evacuation device is employed to evacuate any debris, before the extensible finger **104** continues traveling the circulatory system. It will also be appreciated by those skilled in the art that the device for perfusion management **100** is not restricted to traveling the circulatory system but may be implanted in any tissue, such as, for example, nerve, epithelial, dermal, subdermal, connective, or muscle tissue. Additionally, the device for perfusion management **100** may be implanted in inter-tissue spaces, or inter-organ spaces, for example, those found within a body cavity.

In one aspect the device for perfusion management **100** includes an array of sensors **116** positioned across the plurality of telescoping segments **304** for monitoring, tracking, or mapping a gradient of temperature, pressure, flow, or material concentration in one or more locations. The one or more location may be, for example, a tissue, an artery, or a vein. In another aspect the device for perfusion management **100** has an auto-correct feature for correcting a sub-normal or abnormal gradient of temperature, pressure, flow concentration, or material concentration.

The device for perfusion management **100** may be composed of materials known in the art, for example, a metal, a ceramic, a glass, a plastic, a polymer, a biologically compatible material, or a combination. For example, the device for perfusion management **100** may be made of helically-coiled stainless steel wire and coated with a polymer, such as, Teflon™. In another example, the device for perfusion management **100** may be made of helically-coiled stainless steel wire and coated with a polymer and impregnated with one or more of a biological material, for example, including but not limited to, anti coagulants, or inhibitors.

B. Operation(s) and/or Process(es)

Those having skill in the art will appreciate that some or all of the components of the device for perfusion management **100** may be present ex-vivo. In one implementation, the device for perfusion management **100** is placed in proximity to the location on the animal, for example, the human body **501**, and the extensible finger **104** directed to the selected location and an effective agent delivered in proximity to the selected location. The extensible finger **104** may be retracted after such a delivery, leaving the device for perfusion management **100** in place at the location, until time for a future delivery of the effective agent or another operation. In this implementation, the majority of the device for perfusion management **100** is ex vivo while the extensible finger **104** alternates between ex vivo and in vivo states.

In another aspect, some or all the components of the device for perfusion management **100** are present in vivo. In one implementation, the device for perfusion management **100** is placed in proximity to the location within the animal, for

example, the human body **501**, and the extensible finger **104** directed to a selected location and an effective agent delivered in proximity to the selected location. The extensible finger **104** may be retracted after such a delivery, leaving the device for perfusion management **100** in place at the location, until time for a future delivery or another operation. In this implementation, the majority of the device for perfusion management **100** is in-vivo while the extensible finger **104** alternates between retracted, partially retracted or unretracted states.

In one implementation, the device for perfusion management **100** is operable by a person. The person monitors, guides, positions, and performs other actions/operations or manages a response consistent with the device for perfusion management **100** being managed by the person. In such an implementation a separate display device can present imagery to aid the person. The imagery may be captured as described above with reference to FIG. 4, may be computer generated or may be captured by a separate imaging device internal to or external to the animal, for example, the human body **501**. Actions may be performed under control of the person who may be on site or may be linked from a remote location, or the device for perfusion management **100** may be programmed to perform some or all functions automatically. For example, the device for perfusion management **100** may be programmed to perform functions, such as, lumen clearance, lumen maintenance, monitoring of concentrations, sending of alerts, delivery of one or more of the effective agent at timed intervals or locations, self-check, and self-diagnosis. It will be appreciated by those of skill in the art that the device for perfusion management **100** may be programmed for complete automatic operation of one or more functions.

C. Variation(s), and/or Implementation(s)

Those having skill in the art will recognize that the present application teaches modifications of the devices, structures, and/or processes within the spirit of the teaching herein. For example, the device for perfusion management **100** need not be limited to managing perfusion. The device provides a mechanism for exploring one or more regions and/or reaching a location within an animal, obtaining information, communicating this information, performing operations, performing procedures, and providing treatment. In another example, the device for perfusion management **100** may find utility in the management of physiological functions, the detection or elimination of pathological functions or conditions, and/or treatment of diseases of non-human animals. Other modifications of the subject matter herein will be appreciated by one of skill in the art in light of the teachings herein.

The foregoing described aspects depict different components contained within, or connected with, different other components. It is to be understood that such depicted architectures are merely exemplary, and that in fact many other architectures can be implemented which achieve the same functionality. In a conceptual sense, any arrangement of components to achieve the same functionality is effectively "associated" such that the desired functionality is achieved. Hence, any two components herein combined to achieve a particular functionality can be seen as "associated with" each other such that the desired functionality is achieved, irrespective of architectures or intermedial components. Likewise, any two components so associated can also be viewed as being "operably connected", or "operably coupled", to each other to achieve the desired functionality.

While particular aspects of the present subject matter described herein have been shown and described, it will be obvious to those skilled in the art that, based upon the teachings herein, changes and modifications may be made without

departing from this subject matter described herein and its broader aspects and, therefore, the appended claims are to encompass within their scope all such changes and modifications as are within the true spirit and scope of this subject matter described herein. Furthermore, it is to be understood that the invention is defined solely by the appended claims. It will be understood by those within the art that, in general, terms used herein, and especially in the appended claims (e.g., bodies of the appended claims) are generally intended as "open" terms (e.g., the term "including" should be interpreted as "including but not limited to," the term "having" should be interpreted as "having at least," the term "includes" should be interpreted as "includes but is not limited to," etc.). It will be further understood by those within the art that if a specific number of an introduced claim recitation is intended, such an intent will be explicitly recited in the claim, and in the absence of such recitation no such intent is present. For example, as an aid to understanding, the following appended claims may contain usage of the introductory phrases "at least one" and "one or more" to introduce claim recitations. However, the use of such phrases should not be construed to imply that the introduction of a claim recitation by the indefinite articles "a" or "an" limits any particular claim containing such introduced claim recitation to inventions containing only one such recitation, even when the same claim includes the introductory phrases "one or more" or "at least one" and indefinite articles such as "a" or "an" (e.g., "a" and/or "an" should typically be interpreted to mean "at least one" or "one or more"); the same holds true for the use of definite articles used to introduce claim recitations. In addition, even if a specific number of an introduced claim recitation is explicitly recited, those skilled in the art will recognize that such recitation should typically be interpreted to mean at least the recited number (e.g., the bare recitation of "two recitations," without other modifiers, typically means at least two recitations, or two or more recitations), etc.

What is claimed is:

1. A device for perfusion management, comprising:
a body portion;
at least one extensible finger coupled to said body portion, the extensible finger being composed of a plurality of retractable segments, the plurality of retractable segments of the extensible finger configured to controllably telescopically extend from the body portion;
at least one reservoir in communication with said extensible finger;
a control circuitry coupled to said extensible finger, and/or said body portion;
and an array of sensors distributed among the plurality of retractable segments and configured to deploy from controllably openable and/or closable portholes.
2. The device for perfusion management according to claim 1, further comprising a device for data gathering, data processing, data storage, and/or data transmission.
3. The device for use in perfusion management according to claim 1, wherein the array of sensors comprise an imager, a pressure sensor, a temperature sensor, a chemical sensor, a gas sensor, an electrolyte sensor, a composition sensor, a concentration sensor, and/or a flow sensor coupled to said extensible finger.
4. The device for perfusion management according to claim 1, further comprising a pump, and/or a source of pressure coupled to said extensible finger.
5. The device for perfusion management according to claim 1, further comprising a motor and/or an actuator coupled to said extensible finger.

6. The device for perfusion management according to claim 1, further comprising a wireless data transmitter, coupled to said extensible finger and/or said control circuitry.

7. The device for perfusion management according to claim 1, further comprising a wireless data receiver, and/or a wireless data controller coupled to said extensible finger and/or said control circuit.

8. The device according to claim 1, wherein said at least one extensible finger is coupled to a source of a chemical, a chemical compound, a protein, a lipoprotein, a glycoprotein, a sugar, a lipid, an antigen, an antibody, a cytokine, a peptide, a neurotransmitter, a hormone, an ion, a messenger molecule, a nucleic acid, an engineered nucleic acid, a nucleic acid vector, a drug, a cell, a cell fragment, a cell organelle, a liposome, a pharmaceutical agent, a biological material, and/or a biological fraction internal and/or external to said reservoir.

9. The device according to claim 1, wherein said at least one extensible finger is coupled to a source of two or more of a chemical, a chemical compound, a protein, a lipoprotein, a glycoprotein, a sugar, a lipid, an antigen, an antibody, a cytokine, a peptide, a neurotransmitter, a hormone, an ion, a messenger molecule, a nucleic acid, an engineered nucleic acid, a nucleic acid vector, a drug, a cell, a cell fragment, a cell organelle, a liposome, a pharmaceutical agent, a biological material, and/or a biological fraction internal and/or external to said reservoir.

10. The device for perfusion management according to claim 1, further comprising an operative tool in communication with said extensible finger.

11. The device for perfusion management according to claim 10, wherein said operative tool comprises a tool positioner.

12. The device for perfusion management according to claim 10, wherein said operative tool comprises a device for ablating and/or degrading and/or liquefying a cell, a mass of cells, a tissue, and/or an assembly of biological materials exhibiting shear strength.

13. The device for perfusion management according to claim 10, wherein said control circuitry is operative to guide said operative tool.

14. The device for perfusion management according to claim 1, wherein said extensible finger includes a source of an electric charge and/or electromagnetic radiation coupled and/or carried by said extensible finger.

15. The device for perfusion management according to claim 1, wherein the plurality of retractable segments are configured to articulate at joints of adjacent segments.

16. The device for perfusion management according to claim 1, wherein said plurality of retractable segments are hollow.

17. The device for perfusion management according to claim 1, wherein said extensible finger further comprises a device for fully or partially blocking and/or shunting a liquid flow.

18. The device for perfusion management according to claim 1, further comprising a device for evacuating a target coupled to said extensible finger.

19. The device for perfusion management according to claim 1, further comprising a device for cauterizing and/or sealing a cell, a mass of cells, a tissue, and/or an assembly of biological materials exhibiting shear strength carried by said extensible finger.

20. The device for perfusion management according to claim 1, further comprising a fluid dispenser operative to provide a fluid at a controlled rate.

11

21. The device for perfusion management according to claim 20, wherein said fluid dispenser is carried by said extensible finger.

22. The device for perfusion management according to claim 1, wherein said extensible finger comprises a stent.

23. The device for perfusion management according to claim 1, wherein said control circuitry is coupled to control said extensible finger.

24. The device for perfusion management according to claim 1, wherein said control circuitry is operative to guide said extensible finger.

25. The device for perfusion management according to claim 1, wherein said control circuitry comprises a processor, a feedback circuit, and/or a logic circuit.

26. The device for perfusion management according to claim 1, wherein said control circuitry is a processor further comprising a stored software and/or firmware program cooperative with said processor.

27. The device according to claim 1, wherein said device is of a size, a composition, a power dissipation level, and/or a shape configured for full or partial placement in vivo.

28. The device for perfusion management according to claim 1, wherein said device is configured for implantation in an animal.

29. The device for perfusion management according to claim 28, wherein said animal is human.

30. The device for perfusion management according to claim 29, wherein said device is configured for placement in

12

a selected location in said human corresponding to at least one physiological variable to be monitored and/or treated.

31. The device for perfusion management according to claim 30, wherein said selected location is in a circulatory system, an aorta and/or a vena cava.

32. The device for perfusion management according to claim 1, wherein said device is operative to provide and/or monitor a treatment and/or a response in a patient.

33. The device for perfusion management according to claim 32, wherein said treatment comprises delivering a medicinal agent, a pharmaceutical agent, a therapeutic device and/or assembly to a location in said patient.

34. The device for perfusion management according to claim 1, wherein said device communicates exterior to said patient.

35. The device for perfusion management according to claim 1, wherein the plurality of retractable segments are configured to slidably collapse against adjacent segments and/or within an interior of adjacent segments of larger diameter.

36. The device for perfusion management according to claim 1, wherein a length of the at least one extensible finger is controllably adjustable.

37. The device for perfusion management according to claim 1, wherein articulation of the at least one extensible finger is controllably adjustable.

* * * * *

专利名称(译)	具有用于灌注管理的储液器的系统		
公开(公告)号	US7850676	公开(公告)日	2010-12-14
申请号	US10/827572	申请日	2004-04-19
[标]申请(专利权)人(译)	SEARETE LLC ALIMITED责任特拉华州		
申请(专利权)人(译)	SEARETE有限责任公司，特拉华州的ALIMITED责任公司		
当前申请(专利权)人(译)	齿轮箱有限责任公司		
[标]发明人	WOOD JR LOWELL L		
发明人	WOOD, JR., LOWELL L.		
IPC分类号	A61M25/00 A61M37/00 A61B5/00 A61B5/07 A61B18/14 A61B18/18 A61B18/24 A61F2/02 A61K31/19 A61M1/00 A61M3/00 A61M29/00 A61M31/00		
CPC分类号	A61B5/0031 A61B5/076 A61B5/145 A61B5/14546 A61B5/4839 A61B5/6876 A61M1/0058 A61B1/00016 Y10T29/49826 A61B5/7232 A61B18/1492 A61B18/18 A61B18/24 A61B2562/028 A61F2250/0002 A61M2205/3561 A61M2205/3592 A61M2209/084 A61B1/041		
其他公开文献	US20050234398A1		
外部链接	USPTO		

摘要(译)

用于灌注管理的系统，其监测，维持，诊断或治疗灌注缺陷。

