



US008131564B2

(12) **United States Patent**
Dicks et al.

(10) **Patent No.:** **US 8,131,564 B2**
(45) **Date of Patent:** ***Mar. 6, 2012**

(54) **METHOD FOR MEDICAL DATA
COLLECTION AND TRANSMISSION**

(75) Inventors: **Kent Dicks**, Scottsdale, AZ (US); **Ralph Kent**, Scottsdale, AZ (US); **Robert Tripp**, Fountain Hills, AZ (US); **Terry Bartlett**, Cave Creek, AZ (US); **Thomas Crosley**, Gilbert, AZ (US)

(73) Assignee: **MedApps, Inc.**, Scottsdale, AZ (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **12/938,187**

(22) Filed: **Nov. 2, 2010**

(65) **Prior Publication Data**

US 2011/0093283 A1 Apr. 21, 2011

Related U.S. Application Data

(63) Continuation of application No. 11/923,013, filed on Oct. 24, 2007, now abandoned, and a continuation of application No. 11/877,994, filed on Oct. 24, 2007, and a continuation of application No. 11/877,966, filed on Oct. 24, 2007, and a continuation of application No. 11/877,946, filed on Oct. 24, 2007, and a continuation of application No. 11/877,930, filed on Oct. 24, 2007, and a continuation of application No. 11/877,582, filed on Oct. 23, 2007, and a continuation of application No. 11/877,550, filed on Oct. 23, 2007, and a continuation of application No. 11/877,541, filed on Oct. 23, 2007, and a continuation of application No. 11/877,525, filed on Oct. 23, 2007, now abandoned, and a continuation of application No. 11/876,732, filed on Oct. 22, 2007, and a continuation of application No. 11/876,744, filed on Oct. 22, 2007, and a continuation of application No. 11/876,725, filed on Oct. 22, 2007, and a continuation of application No. 11/876,719, filed on Oct. 22, 2007, and a continuation of application No. 11/876,713, filed on Oct. 22, 2007, and a continuation of application No. 11/876,711, filed on Oct. 22, 2007, and a continuation

of application No. 11/876,708, filed on Oct. 22, 2007, and a continuation of application No. 11/876,695, filed on Oct. 22, 2007, and a continuation of application No. 11/876,689, filed on Oct. 22, 2007.

(60) Provisional application No. 60/862,743, filed on Oct. 24, 2006.

(51) **Int. Cl.**
G06F 3/00 (2006.01)
G06Q 50/00 (2012.01)
A61B 5/00 (2006.01)

(52) **U.S. Cl.** **705/2; 705/3; 710/15; 710/16; 600/300**

(58) **Field of Classification Search** **705/2-3; 710/15-16; 600/300**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,006,699 A 4/1991 Felkner et al.
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2002100889 6/2003
(Continued)

OTHER PUBLICATIONS

“WHMS—Wearable Health Monitoring Systems” <http://www.ece.uah.edu/~jovanov/whrms/>; stored May 15, 2006 at archive.org; retrieved Nov. 15, 2011.*

(Continued)

Primary Examiner — Lena Najarian


Assistant Examiner — Minnah Seoh

(74) *Attorney, Agent, or Firm* — Snell & Wilmer LLP

(57) **ABSTRACT**

An exemplary method according to various aspects of the present invention includes receiving data from a medical device and transmitting a message including at least a portion of the received data to a provided medical data server. This exemplary method further includes receiving a command from the medical data server.

15 Claims, 27 Drawing Sheets

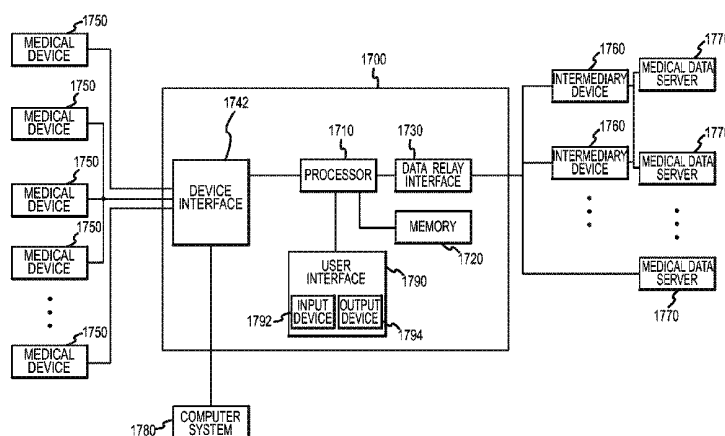

U.S. PATENT DOCUMENTS

5,673,692 A 10/1997 Schulze et al.
 5,721,780 A 2/1998 Ensor et al.
 5,772,586 A 6/1998 Heinonen et al.
 5,891,180 A 4/1999 Greeninger et al.
 5,936,523 A 8/1999 West
 6,024,699 A 2/2000 Surwit et al.
 6,034,963 A 3/2000 Minami et al.
 6,093,146 A 7/2000 Filangeri
 6,302,844 B1 10/2001 Walker et al.
 6,336,900 B1 1/2002 Alleckson et al.
 6,416,471 B1 7/2002 Kumar et al.
 6,443,890 B1 9/2002 Schulze et al.
 6,443,891 B1 9/2002 Grevious
 6,478,736 B1 11/2002 Mault
 6,485,418 B2 11/2002 Yasushi et al.
 6,579,231 B1 6/2003 Phipps
 6,580,948 B2 6/2003 Hauptert
 6,598,084 B1 7/2003 Edwards et al.
 6,625,642 B1 9/2003 Naylor et al.
 6,790,178 B1 9/2004 Mault et al.
 6,804,558 B2 10/2004 Haller et al.
 6,807,965 B1 10/2004 Hickie
 6,893,396 B2 5/2005 Schulze et al.
 6,903,657 B2 6/2005 Kwoen
 6,915,267 B2 7/2005 Jackson et al.
 6,957,107 B2 10/2005 Rogers et al.
 6,978,182 B2 12/2005 Mazar et al.
 7,039,810 B1 5/2006 Nichols
 7,044,911 B2 5/2006 Drinan et al.
 7,129,836 B2 10/2006 Lawson et al.
 7,134,996 B2 11/2006 Bardy
 7,154,398 B2 12/2006 Chen et al.
 7,156,808 B2 1/2007 Quy
 7,161,484 B2 1/2007 Tsoukalis
 7,181,017 B1 2/2007 Nagel et al.
 7,231,258 B2 6/2007 Moore et al.
 7,265,676 B2 9/2007 Gordon et al.
 7,311,666 B2 12/2007 Stupp et al.
 7,761,261 B2 7/2010 Shmueli et al.
 2001/0005772 A1 6/2001 Kisakibaru
 2001/0051787 A1 12/2001 Haller et al.
 2002/0029157 A1 3/2002 Marchosky
 2002/0072933 A1 6/2002 Vonk et al.
 2002/0128804 A1 9/2002 Geva
 2003/0009088 A1 1/2003 Korth et al.
 2003/0018742 A1 1/2003 Imago
 2003/0050539 A1 3/2003 Naghavi et al.
 2003/0072424 A1 4/2003 Evans
 2003/0088295 A1 5/2003 Cox
 2003/0088441 A1 5/2003 McNerney
 2003/0095675 A1 5/2003 Marlow et al.
 2003/0149593 A1 8/2003 Mok et al.
 2003/0216625 A1 11/2003 Phillips
 2004/0015132 A1 1/2004 Brown
 2004/0078220 A1 4/2004 Jackson
 2004/0097796 A1 5/2004 Berman et al.
 2004/0100376 A1 5/2004 Lye et al.
 2004/0102683 A1 5/2004 Khanuja et al.
 2004/0122488 A1 6/2004 Mazar et al.
 2004/0127775 A1 7/2004 Miyazaki et al.
 2004/0152961 A1 8/2004 Carlson et al.
 2004/0199056 A1 10/2004 Husemann et al.
 2004/0210458 A1 10/2004 Evans
 2005/0004700 A1 1/2005 DiMaggio
 2005/0021370 A1 1/2005 Riff et al.
 2005/0038680 A1 2/2005 McMahon
 2005/0060187 A1 3/2005 Gottesman
 2005/0065815 A1 3/2005 Mazar et al.
 2005/0070767 A1 3/2005 Maschke
 2005/0119580 A1 6/2005 Eveland
 2005/0137465 A1 6/2005 Cuddihy et al.
 2005/0171410 A1 8/2005 Hjelt et al.
 2005/0171762 A1 8/2005 Ryan et al.
 2005/0192649 A1 9/2005 Shehadeh et al.
 2005/0197545 A1 9/2005 Hoggie
 2005/0203775 A1 9/2005 Chesbrough
 2005/0234307 A1 10/2005 Heinonen et al.
 2005/0240111 A1 10/2005 Chung

2006/0020302 A1 1/2006 Torgerson et al.
 2006/0026118 A1 2/2006 Jung et al.
 2006/0035669 A1 2/2006 Chuprun et al.
 2006/0036134 A1 2/2006 Tarassenko et al.
 2006/0063980 A1 3/2006 Hwang et al.
 2006/0064320 A1 3/2006 Postrel
 2006/0089542 A1 4/2006 Sands
 2006/0111079 A1 5/2006 Tischer et al.
 2006/0116744 A1 6/2006 Von Arx et al.
 2006/0135858 A1 6/2006 Nidd et al.
 2006/0142648 A1 6/2006 Banet et al.
 2006/0161222 A1 7/2006 Haubrich et al.
 2006/0167346 A1 7/2006 Sarel
 2006/0200007 A1 9/2006 Brockway et al.
 2006/0202816 A1 9/2006 Crump et al.
 2006/0205564 A1 9/2006 Peterson
 2006/0212316 A1 9/2006 Jackson et al.
 2006/0218011 A1 9/2006 Walker et al.
 2006/0235280 A1 10/2006 Vonk et al.
 2006/0242295 A1 10/2006 Husemann et al.
 2006/0253301 A1 11/2006 Simms et al.
 2006/0293607 A1 12/2006 Alt et al.
 2007/0002791 A1 1/2007 Kasprzyk et al.
 2007/0004969 A1 1/2007 Kong et al.
 2007/0015974 A1 1/2007 Higgins et al.
 2007/0016450 A1 1/2007 Bhora et al.
 2007/0033072 A1 2/2007 Bildirici
 2007/0055552 A1 3/2007 St. Clair et al.
 2007/0061167 A1 3/2007 Brown
 2007/0073266 A1 3/2007 Chmeil et al.
 2007/0078497 A1 4/2007 Vandanacker
 2007/0083246 A1 4/2007 Mazar et al.
 2007/0135855 A1 6/2007 Foshee et al.
 2007/0188323 A1 8/2007 Sinclair et al.
 2007/0239229 A1 10/2007 Masoud et al.
 2007/0250130 A1 10/2007 Ball et al.
 2007/0253380 A1 11/2007 Jollota et al.
 2008/0059239 A1 3/2008 Gerst et al.
 2008/0065412 A1 3/2008 Vallone
 2008/0126131 A1 5/2008 Lou

FOREIGN PATENT DOCUMENTS

WO 0049549 8/2000
 WO 02058307 7/2002
 WO 2005079667 9/2005
 WO 2005101279 10/2005
 WO 2006006159 1/2006
 WO 2006060669 6/2006

OTHER PUBLICATIONS

USPTO; Office Action dated Apr. 14, 2010 in U.S. Appl. No. 11/876,689.
 USPTO; Final Office Action dated Dec. 22, 2010 in U.S. Appl. No. 11/876,689.
 USPTO; Advisory Action dated Apr. 1, 2011 in U.S. Appl. No. 11/876,689.
 USPTO; Office Action dated Apr. 1, 2010 in U.S. Appl. No. 11/876,695.
 USPTO; Final Office Action dated Dec. 21, 2010 in U.S. Appl. No. 11/876,695.
 USPTO; Office Action dated Apr. 28, 2010 in U.S. Appl. No. 11/876,708.
 USPTO; Final Office Action dated Dec. 22, 2010 in U.S. Appl. No. 11/876,708.
 USPTO; Office Action dated May 26, 2010 in U.S. Appl. No. 11/876,713.
 USPTO; Final Office Action dated Dec. 22, 2010 in U.S. Appl. No. 11/876,713.
 USPTO; Office Action dated Mar. 29, 2010 in U.S. Appl. No. 11/876,719.
 USPTO; Office Action dated Dec. 22, 2010 in U.S. Appl. No. 11/876,719.
 USPTO; Office Action dated Sep. 15, 2010 in U.S. Appl. No. 11/876,725.
 USPTO; Office Action dated Apr. 1, 2010 in U.S. Appl. No. 11/876,744.

- USPTO; Final Office Action dated Dec. 21, 2010 in U.S. Appl. No. 11/876,744.
- USPTO; Office Action dated Sep. 3, 2010 in U.S. Appl. No. 11/876,732.
- USPTO; Office Action dated Jan. 26, 2011 in U.S. Appl. No. 12/951,957.
- USPTO; Office Action dated Jul. 29, 2010 in U.S. Appl. No. 11/877,493.
- USPTO; Final Office Action dated Mar. 18, 2011 in U.S. Appl. No. 11/877,493.
- USPTO; Office Action dated Jan. 26, 2011 in U.S. Appl. No. 11/877,541.
- USPTO; Office Action dated Aug. 31, 2010 in U.S. Appl. No. 11/877,545.
- USPTO; Office Action dated Feb. 9, 2011 in U.S. Appl. No. 11/877,550.
- USPTO; Office Action dated Jan. 27, 2011 in U.S. Appl. No. 11/877,573.
- USPTO; Office Action dated Jul. 1, 2010 in U.S. Appl. No. 11/877,582.
- USPTO; Final Office Action dated Mar. 2, 2011 in U.S. Appl. No. 11/877,582.
- USPTO; Office Action dated Aug. 9, 2010 in U.S. Appl. No. 11/877,930.
- USPTO; Final Office Action dated Mar. 14, 2011 in U.S. Appl. No. 11/877,930.
- USPTO; Office Action dated Apr. 13, 2010 in U.S. Appl. No. 11/877,946.
- USPTO; Final Office Action dated Dec. 21, 2010 in U.S. Appl. No. 11/877,946.
- USPTO; Office Action dated Apr. 15, 2010 in U.S. Appl. No. 11/877,966.
- USPTO; Final Office Action dated Dec. 21, 2010 in U.S. Appl. No. 11/877,966.
- USPTO; Office Action dated Sep. 1, 2010 in U.S. Appl. No. 11/877,994.
- USPTO; Office Action dated Jan. 21, 2011 in U.S. Appl. No. 12/952,009.
- EP; Examination Report dated Jan. 18, 2011 in Application No. 7844567.3.
- CN; Office Action dated Dec. 2010 in Application No. 200780048044.X.
- CN; Office Action dated Mar. 2011 in Application No. 200780048064.7.
- CN; Office Action dated Mar. 2011 in Application No. 200780048047.3.
- PCT; International Search Report and Written Opinion dated May 14, 2008 in Application No. PCT/US2007/082161.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082161.
- PCT; International Search Report and Written Opinion dated Oct. 10, 2008 in Application No. PCT/US2007/082253.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082253.
- PCT; International Search Report and Written Opinion dated Jan. 15, 2009 in Application No. PCT/US2007/082284.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082284.
- PCT; International Search Report and Written Opinion dated Nov. 6, 2008 in Application No. PCT/US2007/082158.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082158.
- PCT; International Search Report and Written Opinion dated Feb. 18, 2008 in Application No. PCT/US2007/082351.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082351.
- PCT; International Search Report and Written Opinion dated May 27, 2008 in Application No. PCT/US2007/082358.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082358.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082288.
- PCT; International Preliminary Report on Patentability dated Apr. 28, 2009 in Application No. PCT/US2007/082292.
- USPTO; Final Office Action dated May 24, 2011 in U.S. Appl. No. 11/876,725.
- USPTO; Final Office Action dated May 11, 2011 in U.S. Appl. No. 11/877,545.
- USPTO; Final Office Action dated May 11, 2011 in U.S. Appl. No. 11/877,994.
- Blount et al., "Remote health-care monitoring using Personal Care Connect", IBM Systems Journal, vol. 46, No. 1, pp. 95-113, (2007).
- Milenkovic et al., "Wireless sensor networks for personal health monitoring: Issues and an implementation", Computer Communications, 13 pages (2006).
- Setton et al., "Bluetooth sensors for wireless home and hospital healthcare monitoring", Cyberfab, 6 pages, date unknown, 2007.
- Korhonen et al., "Health Monitoring in the Home of the Future", IEEE Engineering in Medicine and Biology Magazine, pp. 66-73 (May/Jun. 2003).
- "WHIMS—Wearable Health Monitoring Systems", Electrical and Computer Engineering, The University of Alabama in Huntsville, <http://www.ece.uah.edu/~jovanov/whrms/>, 13 pages, 2006.
- Hung et al., "Implementation of a WAP-Based Telemedicine System for Patient Monitoring", IEEE Transactions of Information Technology in Biomedicine, vol. 7, No. 2, pp. 101-107 (Jun. 2003).
- Lee et al., "Design and Implementation of a Mobile-Care System over Wireless Sensor Network for Home Healthcare Applications", Proceedings of the 28th IEEE EMBS Annual International Conference, pp. 6004-6007 (Aug./Sep. 2006).
- Chen et al., "An i-Mode Portable Healthcare Monitor", Proceedings of the Second Joint EMBS/BMES Conference, IEEE, pp. 1851-1852 (2002).
- Kuo et al., "Design and Implementation of Internet-Based In-House Healthcare and Home Automation Systems", IEEE, pp. 2944-2949 (2003).
- Jovanov et al., "Stress Monitoring Using a Distributed Wireless Intelligent Sensor System", IEEE Engineering in Medicine and Biology Magazine, pp. 49-55 (May/Jun. 2003).
- Lubrin et al., "Wireless Remote Healthcare Monitoring with Motes", Proceedings of the International Conference on mobile Business, IEEE Computer Society, 7 pages (2005).
- Princeton University Wordnet; <http://wordnetweb.princeton.edu/perl/webwn?s=event>; accessed Dec. 19, 2010.
- Guo et al., "Implementing a wireless portable healthcare monitoring system for physiological signals", The Institute of Engineering and Technology, 1 page (2007).
- Otto et al., "System Architecture of a Wireless Body Area Sensor Network for Ubiquitous Health Monitoring", Journal of Mobile Multimedia, vol. 1, No. 4, pp. 307-326 (2006).
- Yu et al., "A Wireless Physiological Signal Monitoring System with Integrated Bluetooth and WiFi Technologies", Proceedings of the 2005 IEEE Engineering in Medicine and Biology 27th Annual Conference pp. 2203-2206 (2005).
- "Body Area Networks—A 'Healthy Aims' Projects", Zarlink Semiconductor Inc., 1 page (2007).
- "Bionformatics" downloaded from webpage <http://en.wikipedia.org/wiki/Bioinformatics> on Aug. 2, 2007 (9 pages).
- Mintz, "Microsoft Launches Health Records Site," downloaded from webpage http://bz.yahoo.com/ap/071004/microsoft_healthvault.html?_v=1 on Dec. 18, 2007 (3 pages).
- "Bluetooth Sig Aims to Improve Healthcare Experience Through Interoperability," downloaded from webpage http://www.bluetooth.com/Bluetooth/Press/SIG/BLUETOOTH_SIG_AIMS_TO_IMPROVE_HEALTHCARE_EXPERIENCE_THROUGH_INTEROPERABILITY.htm (2 pages), May 22, 2006.
- How PGP Works, <http://www.pgpi.org/doc/pgpintro/>, 2010.

* cited by examiner

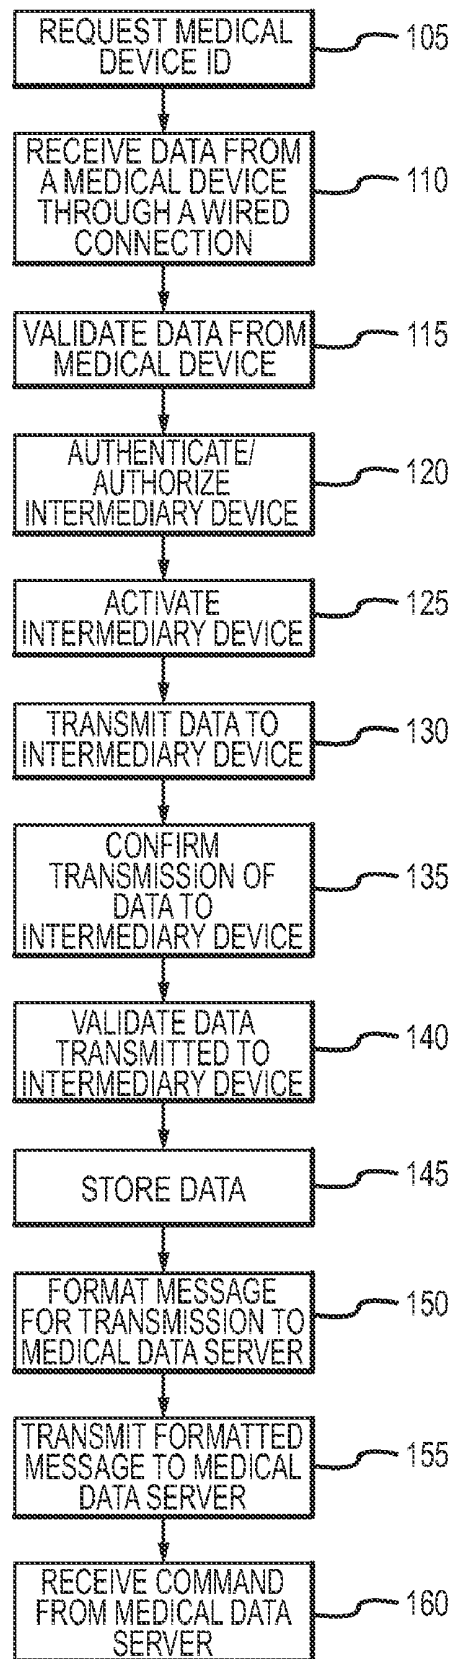


FIGURE 1

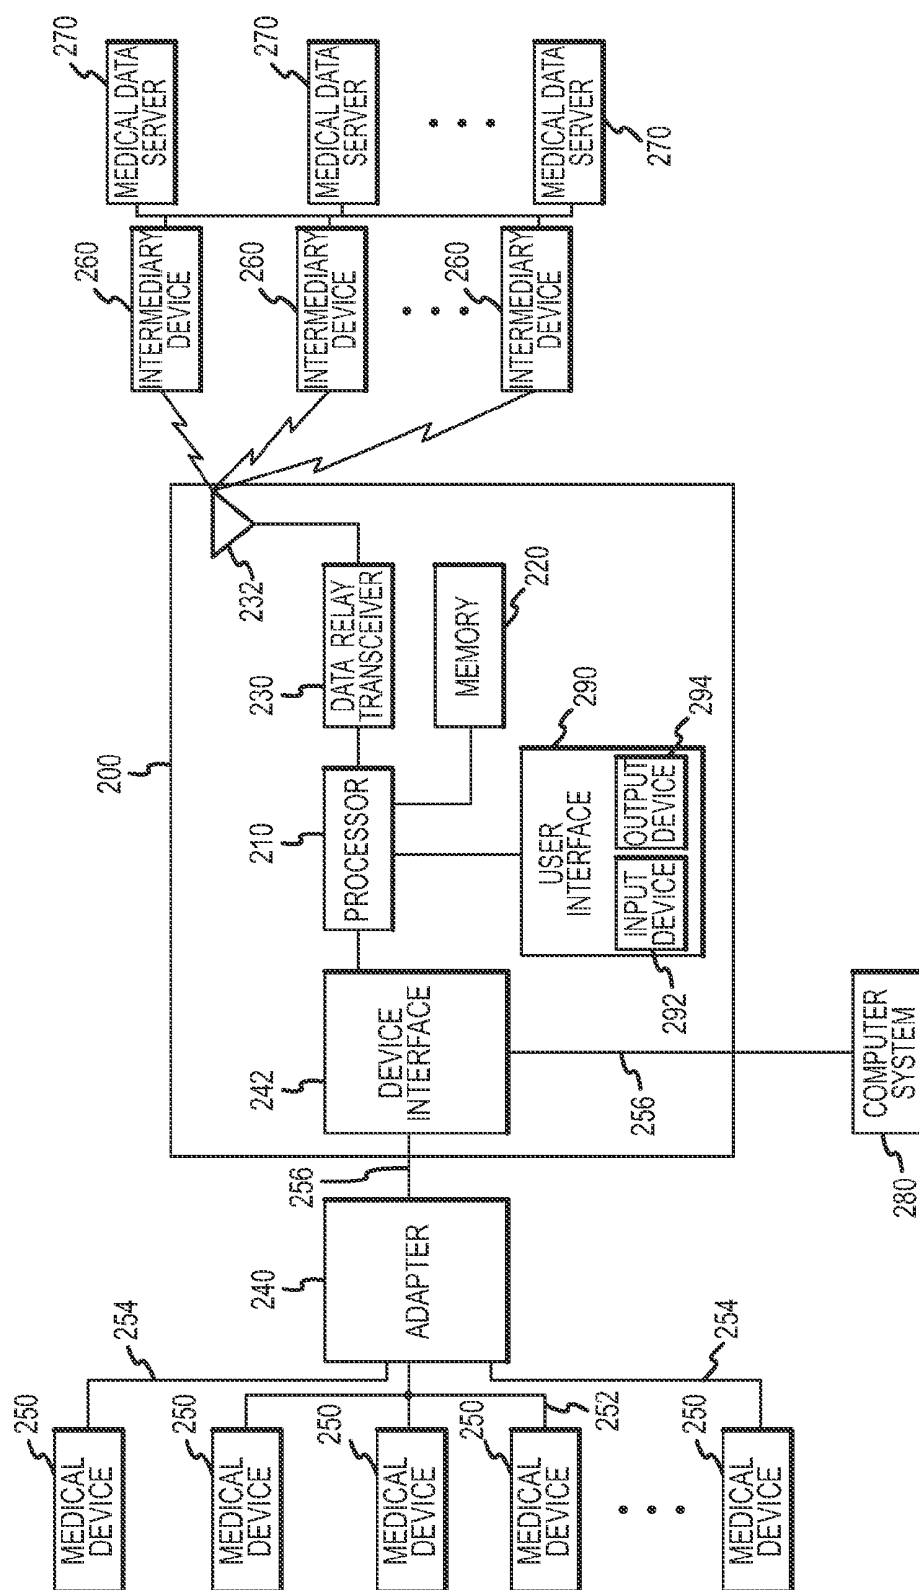


FIGURE 2A

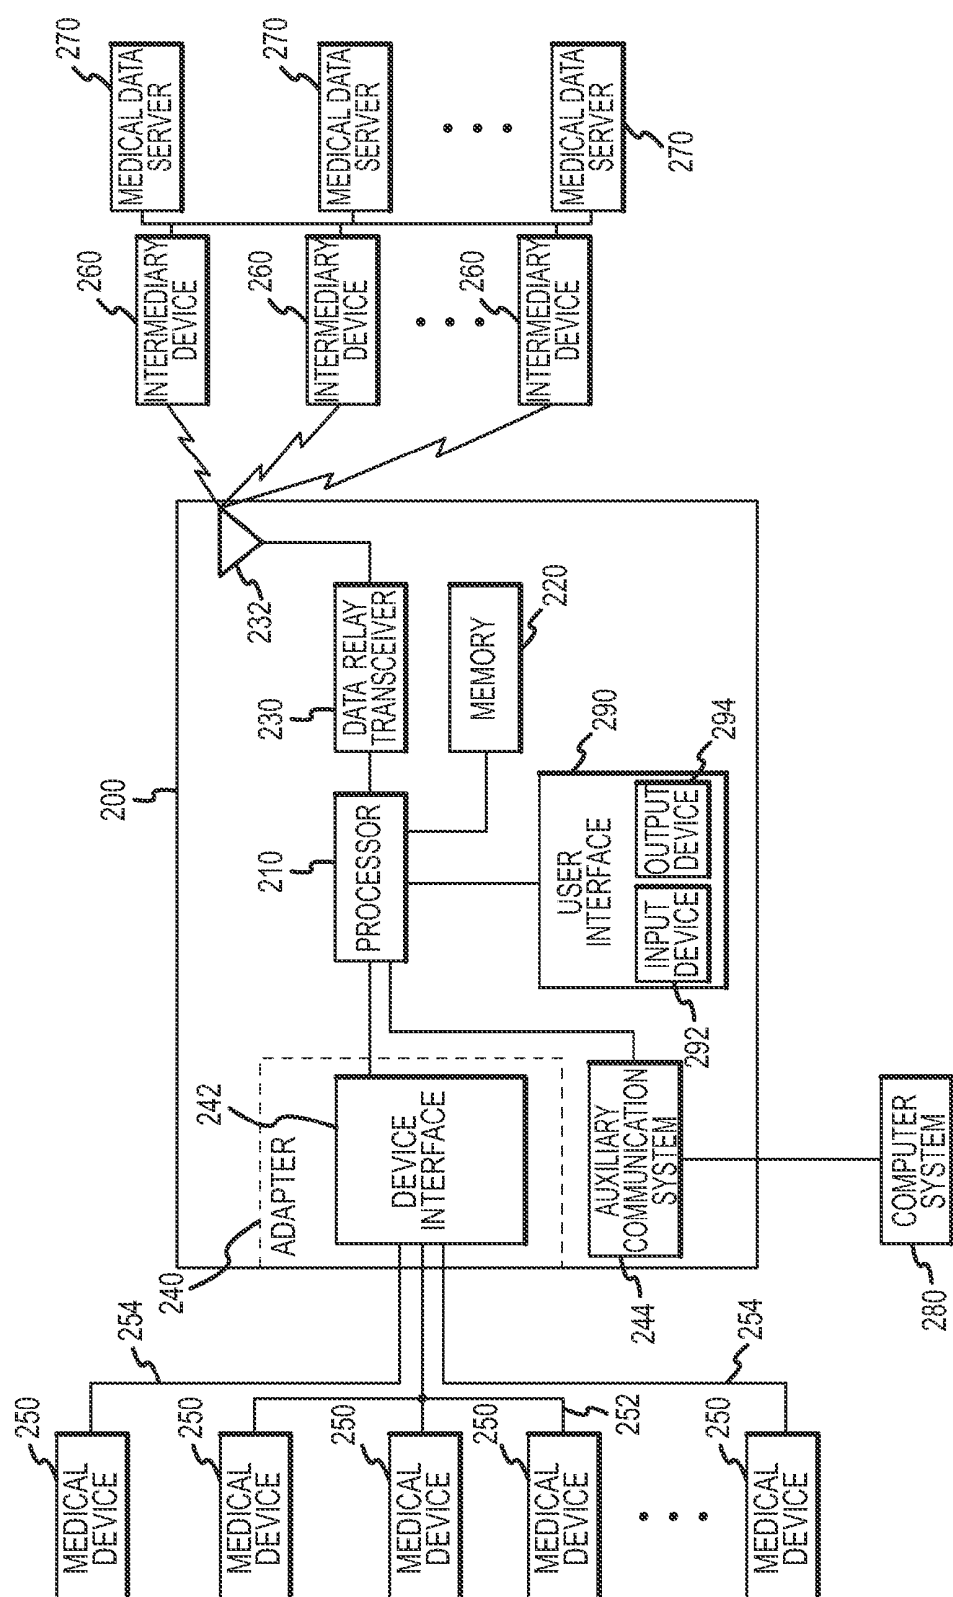


FIGURE 2B

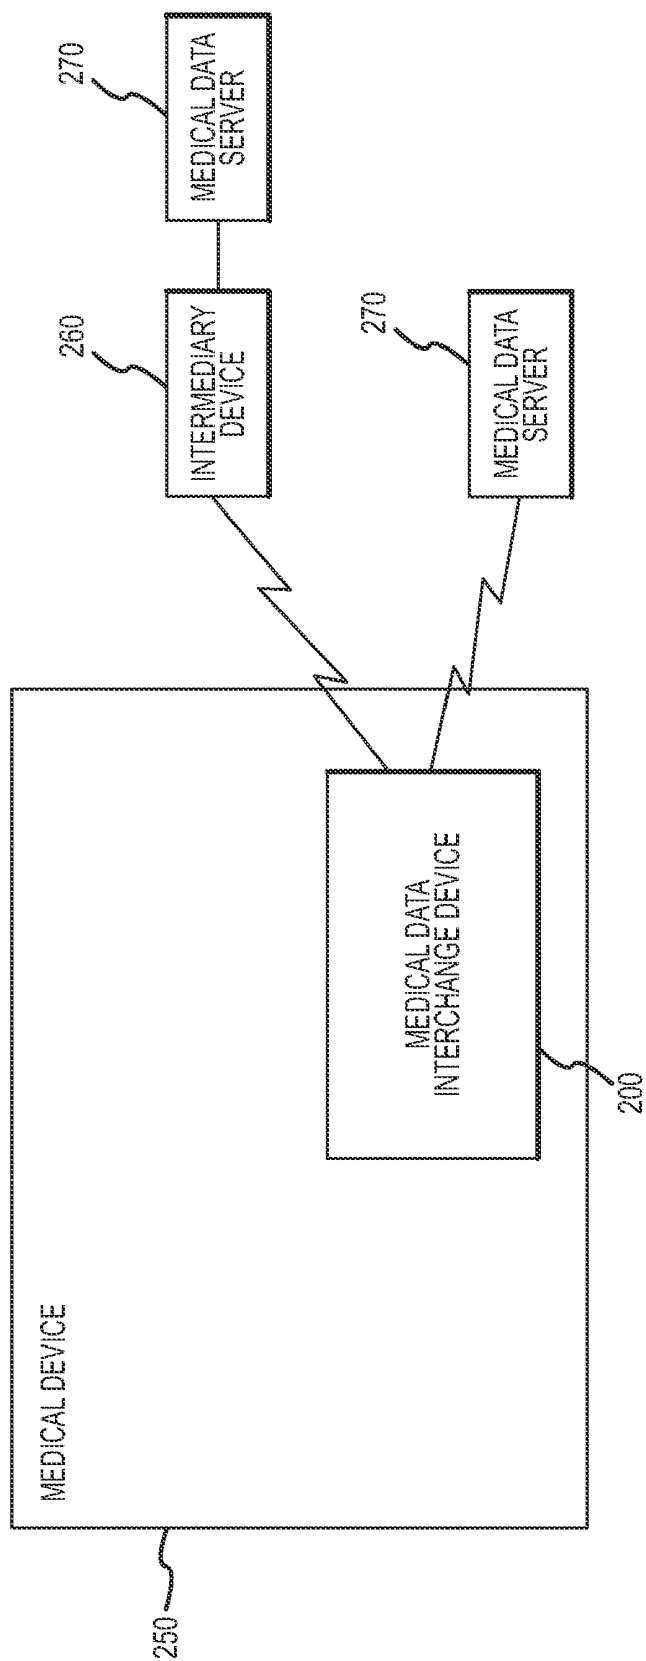


FIGURE 2C

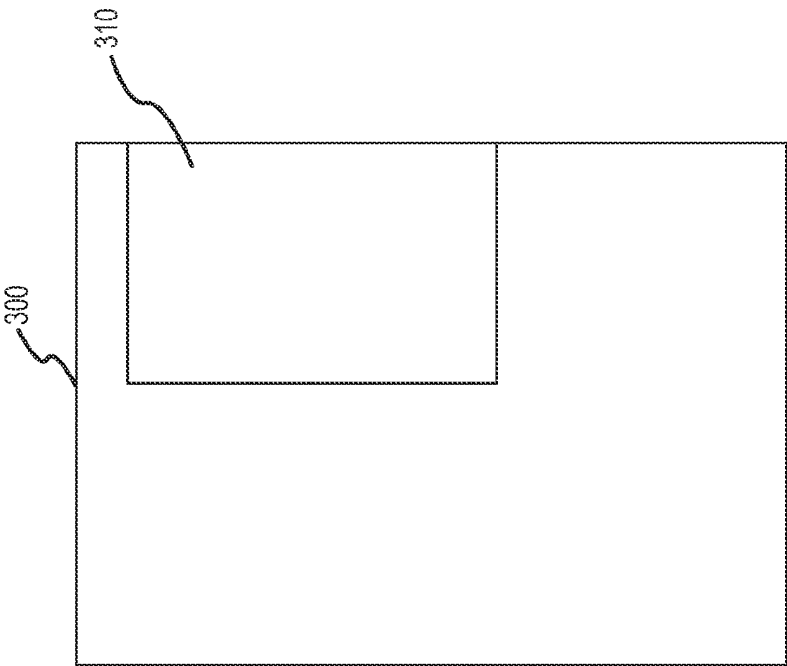


FIGURE 3A

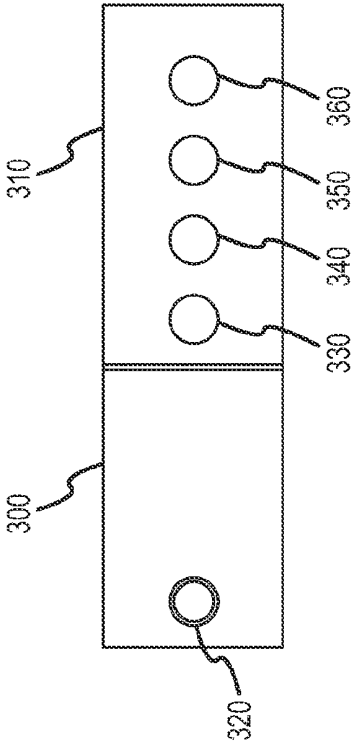


FIGURE 3B

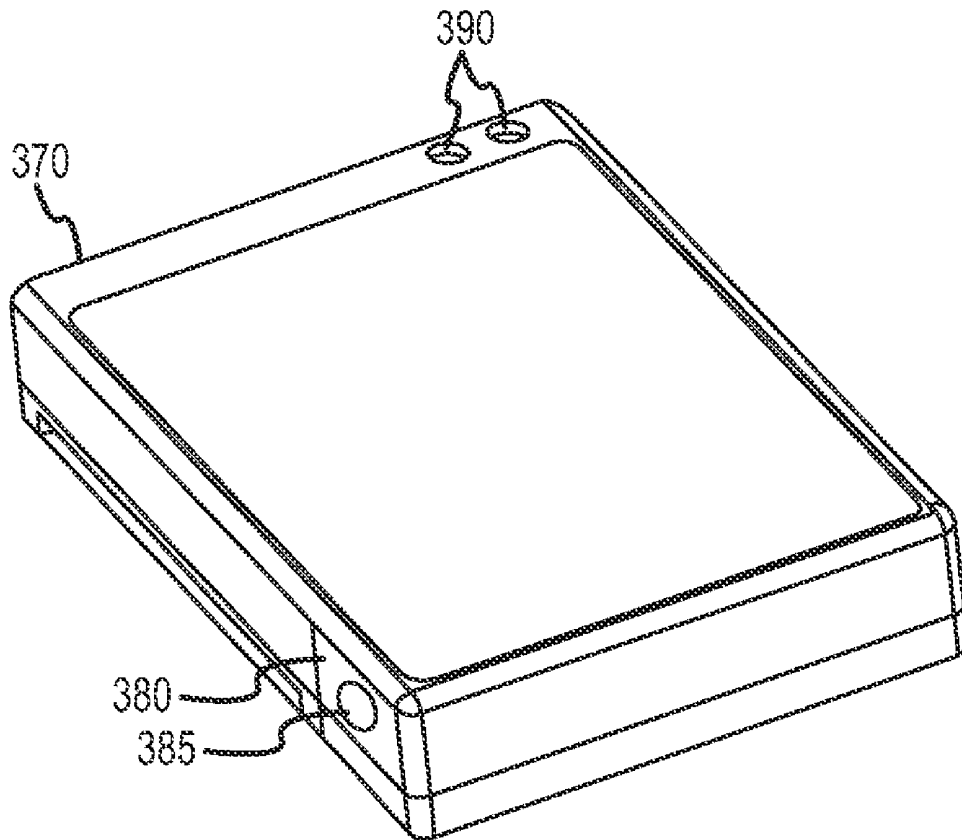


FIG. 3C

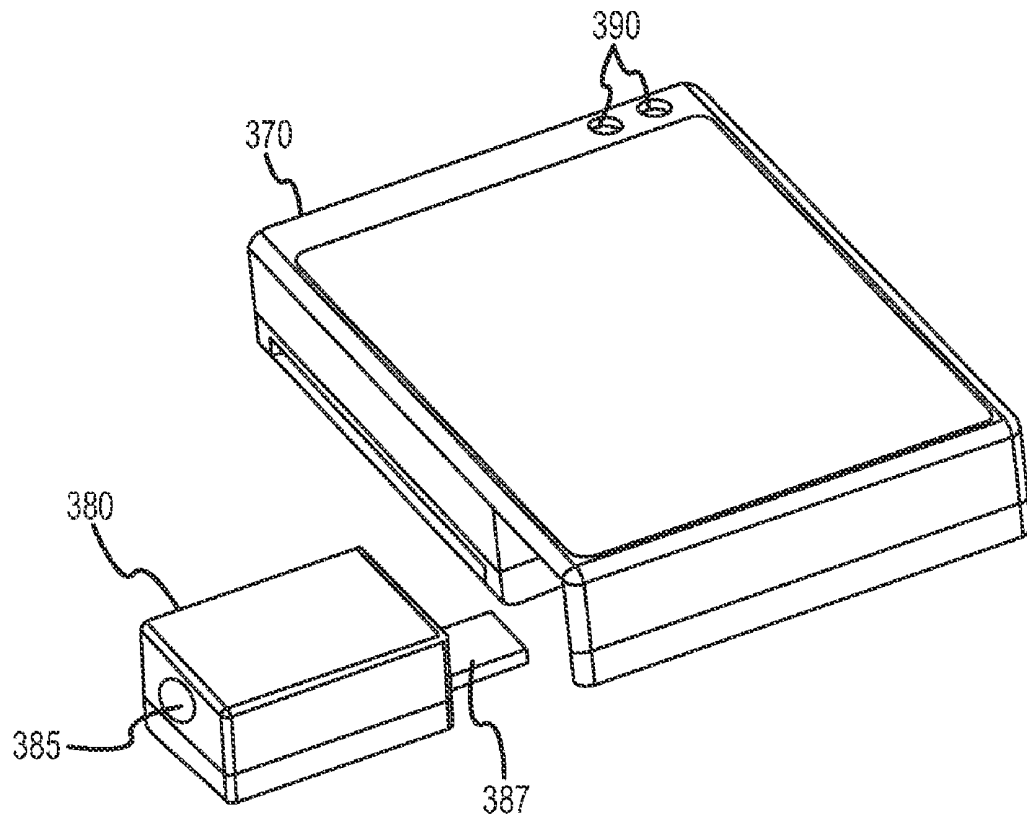


FIG.3D

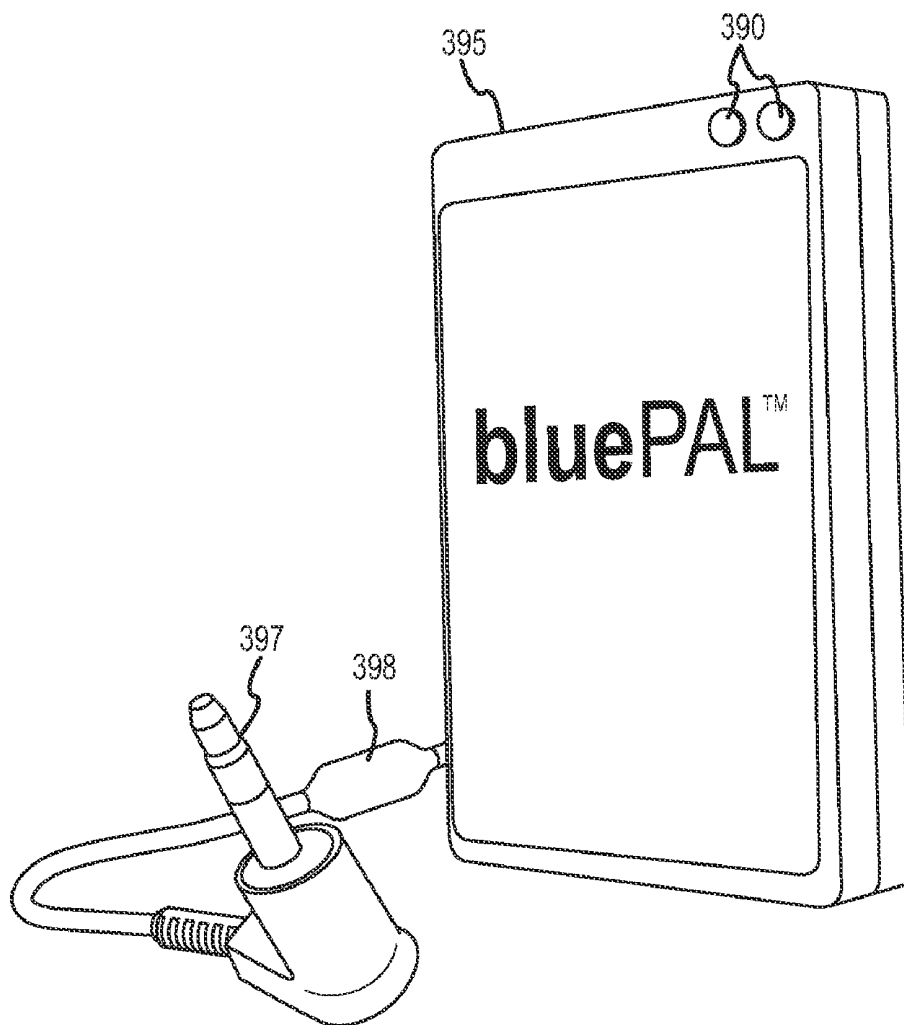


FIG. 3E

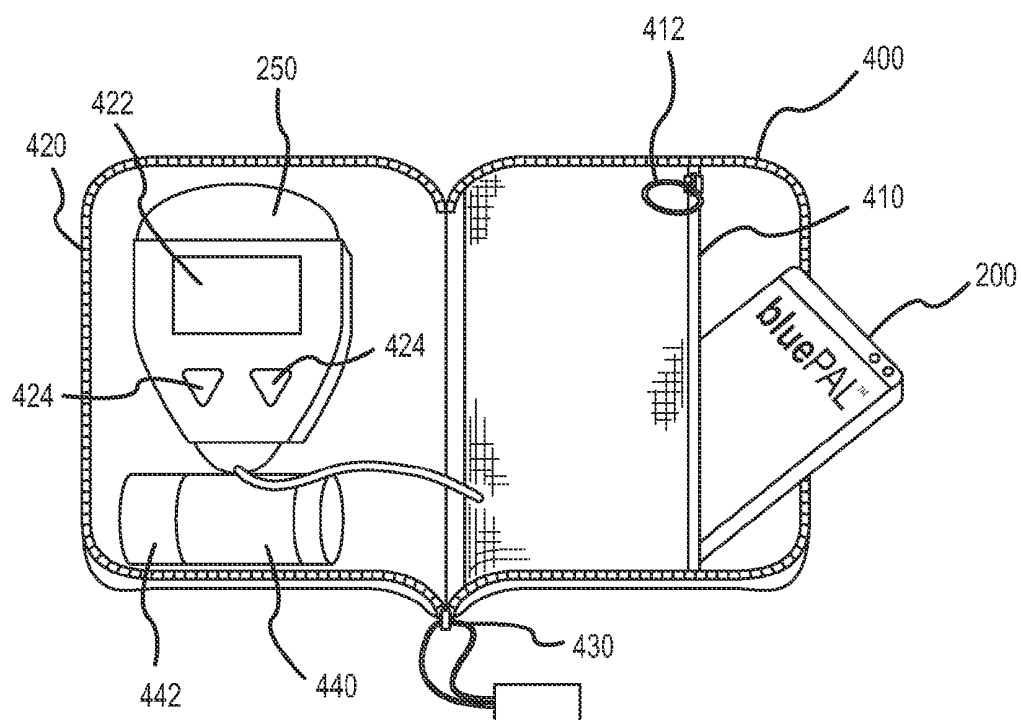


FIG.4

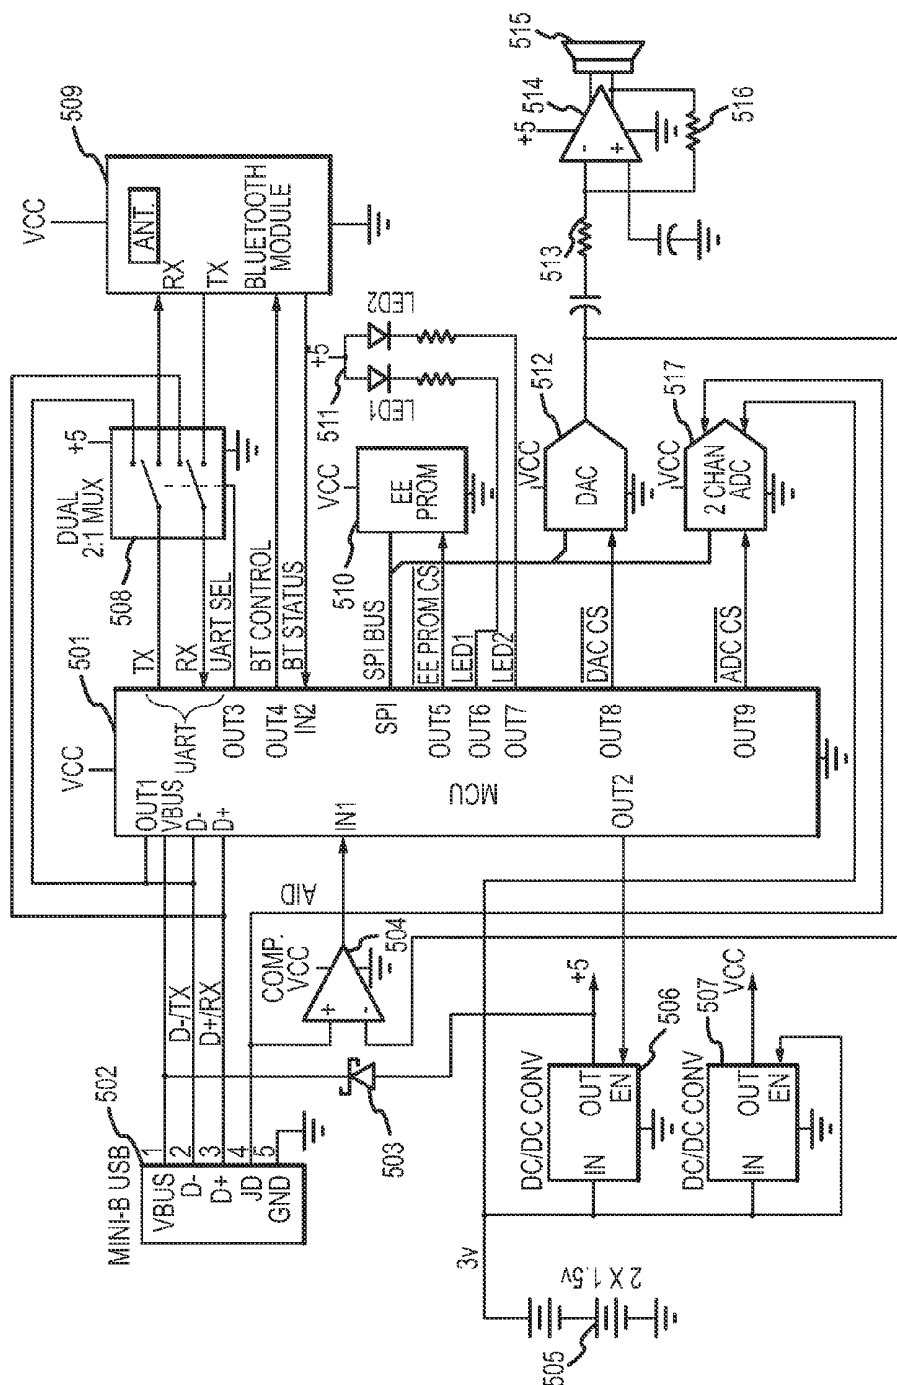


FIGURE 5A

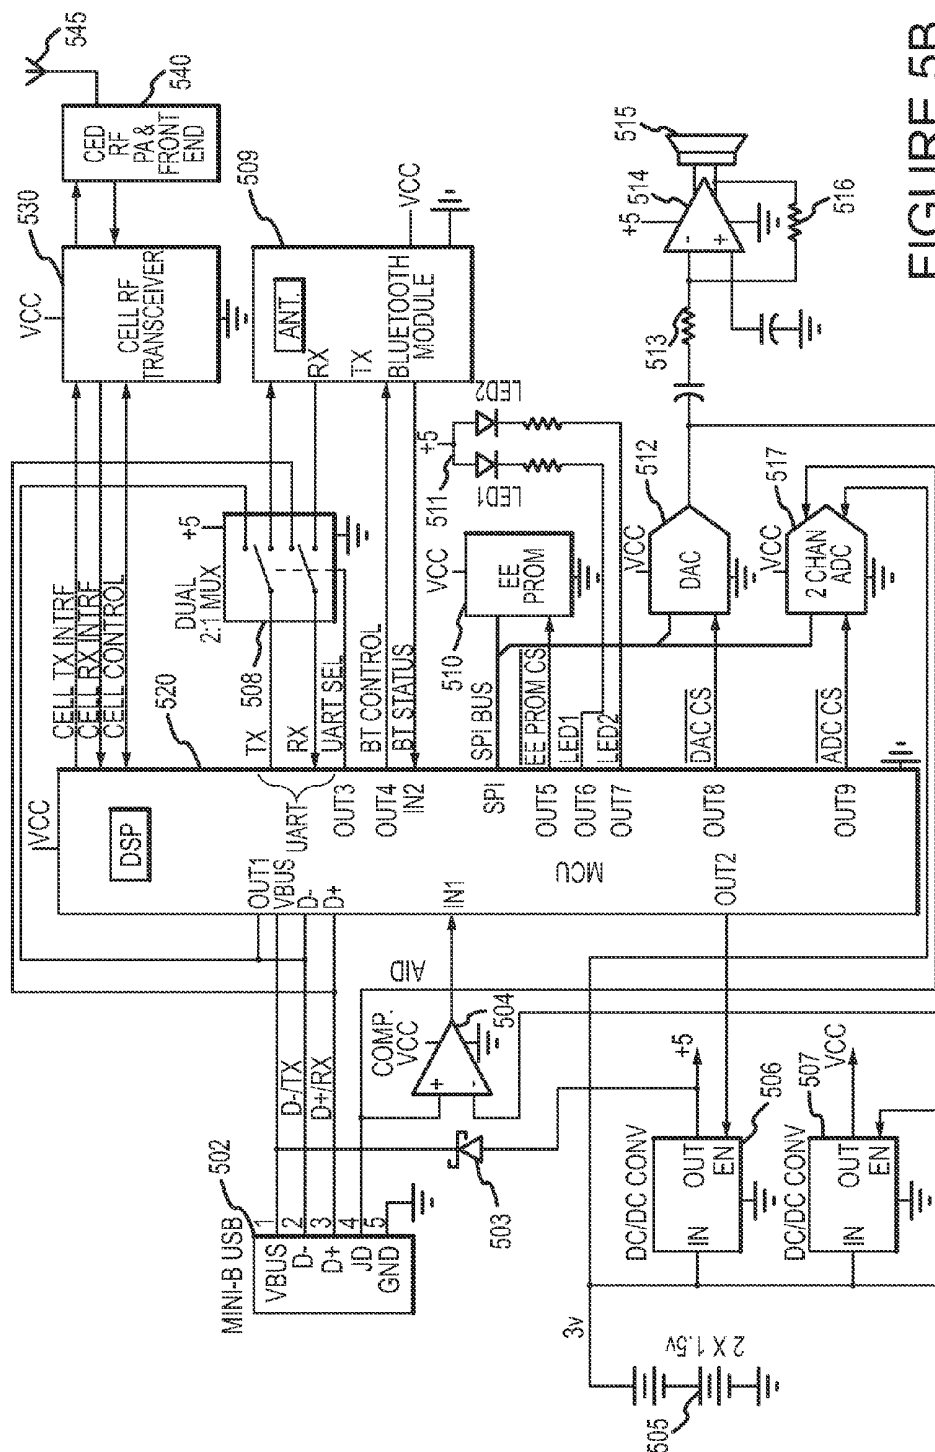
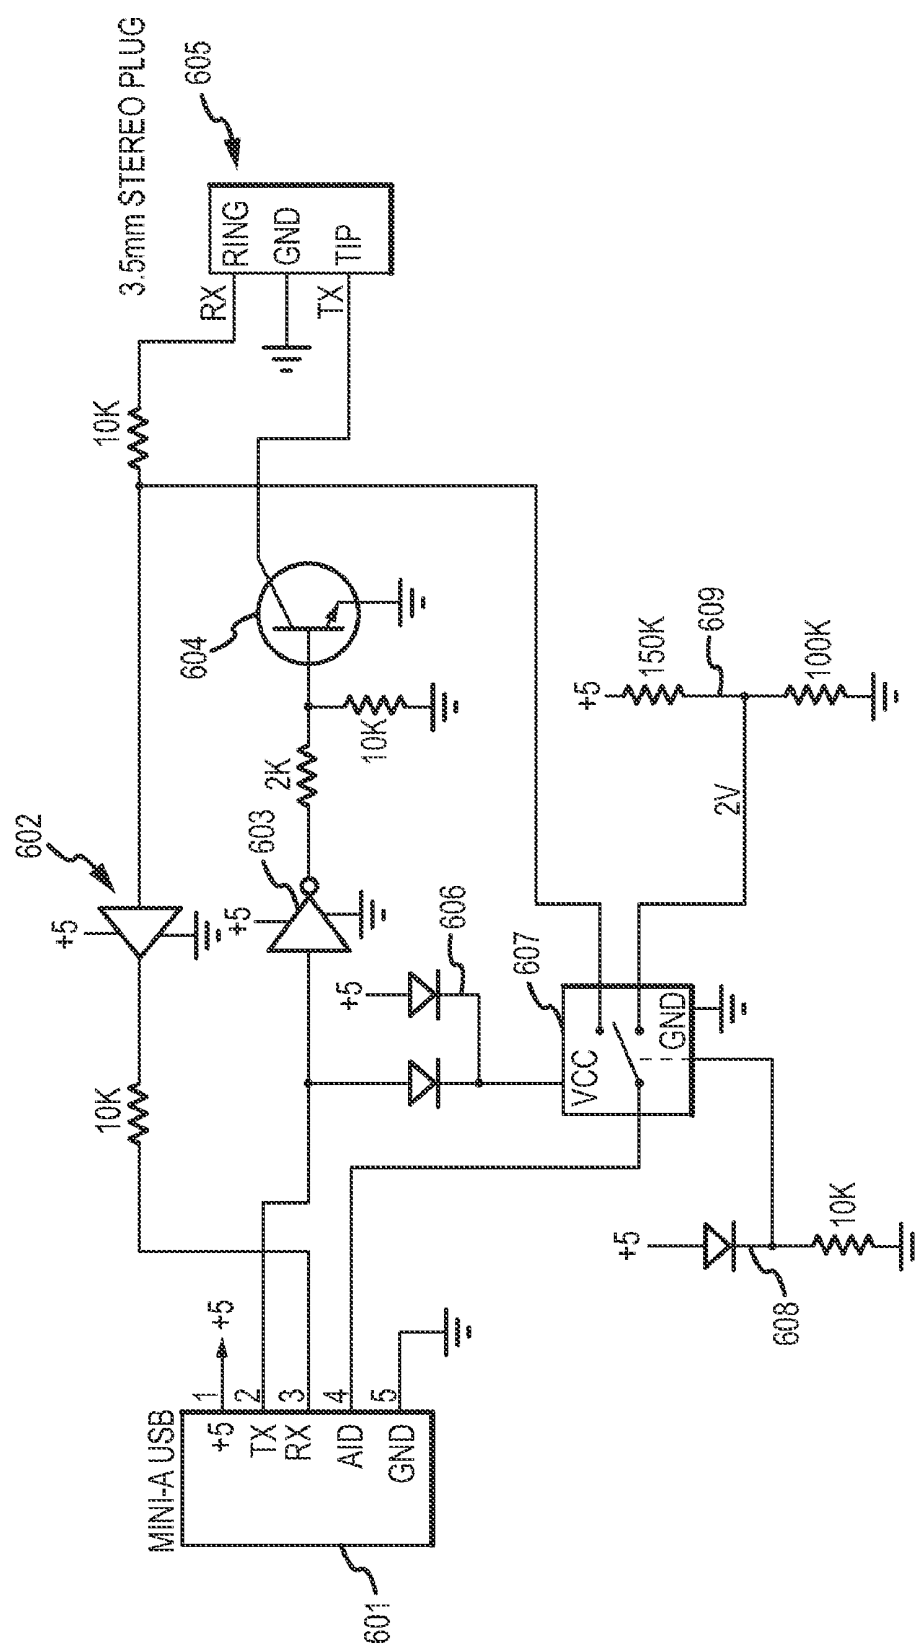


FIGURE 5B





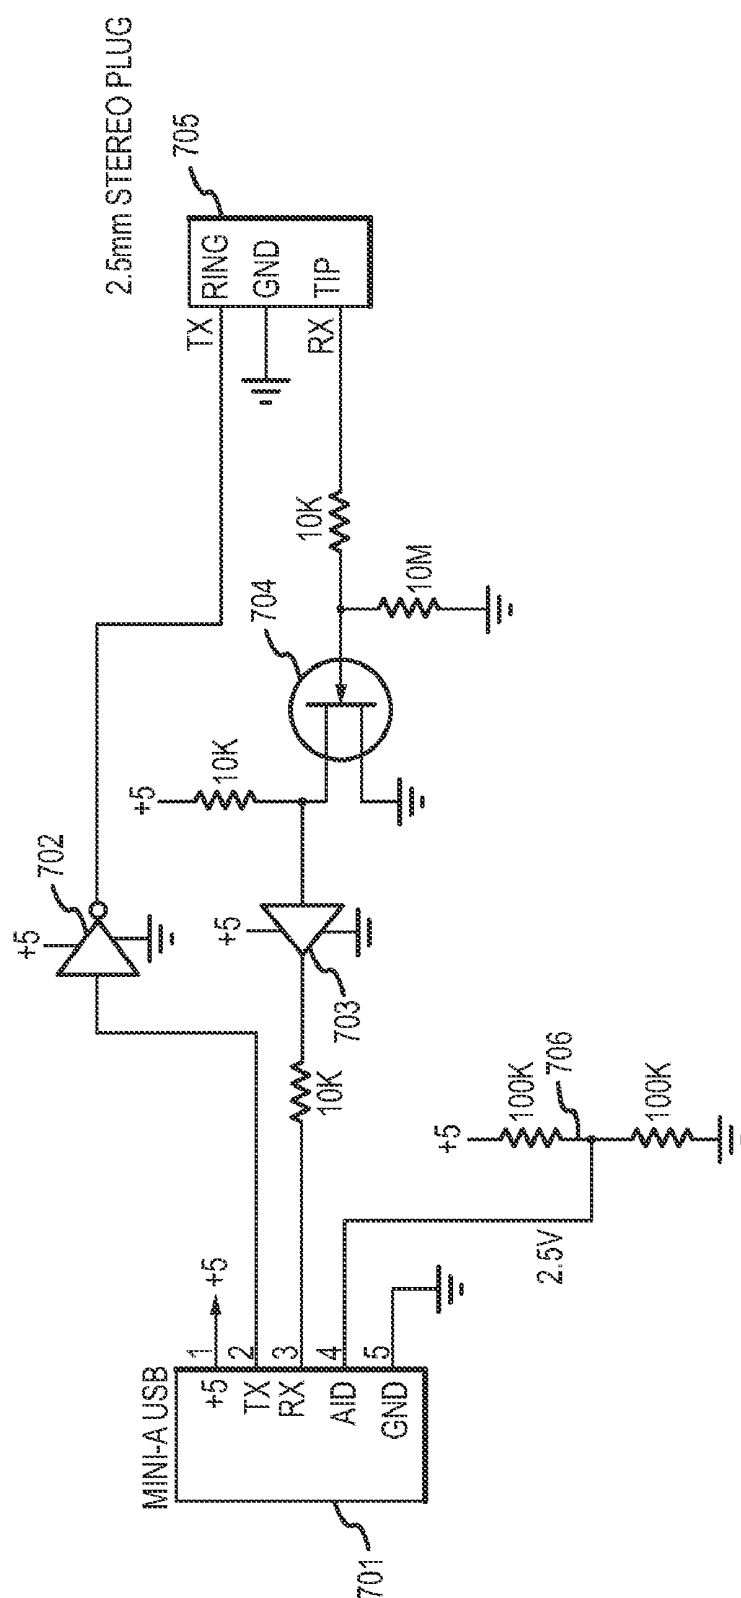


FIGURE 7

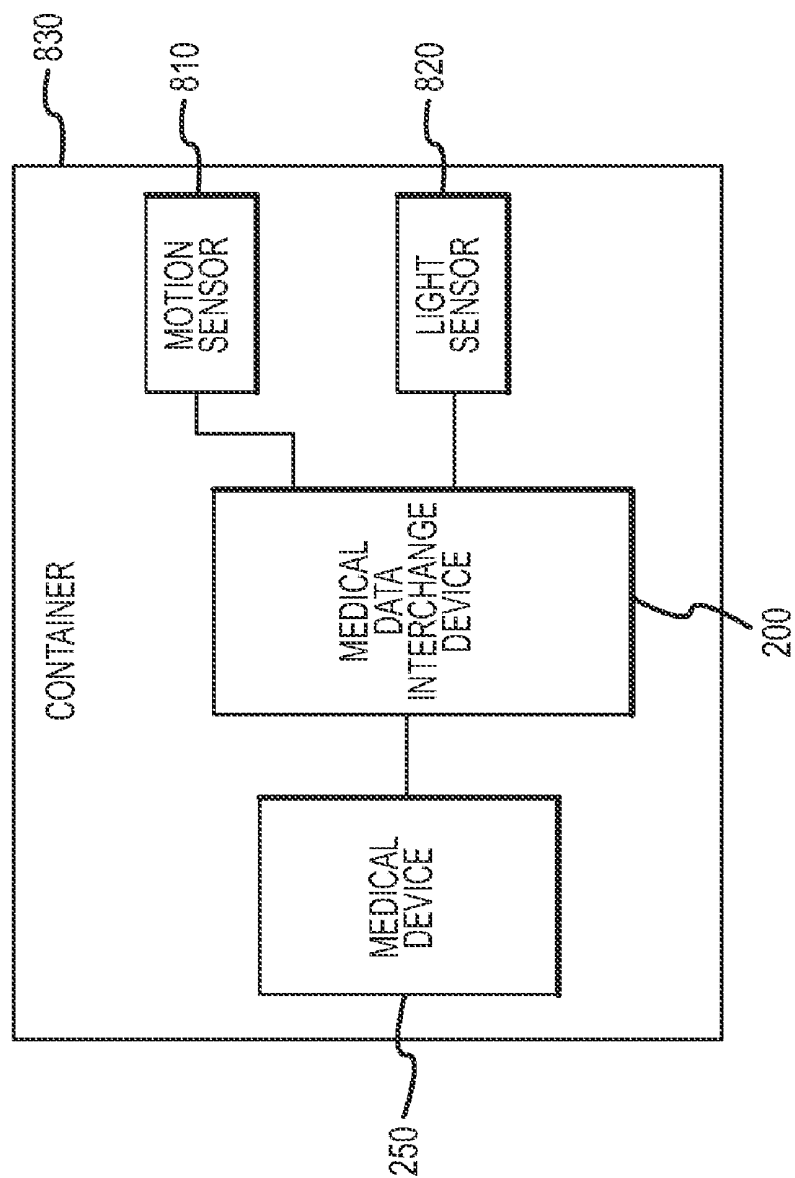


FIGURE 8

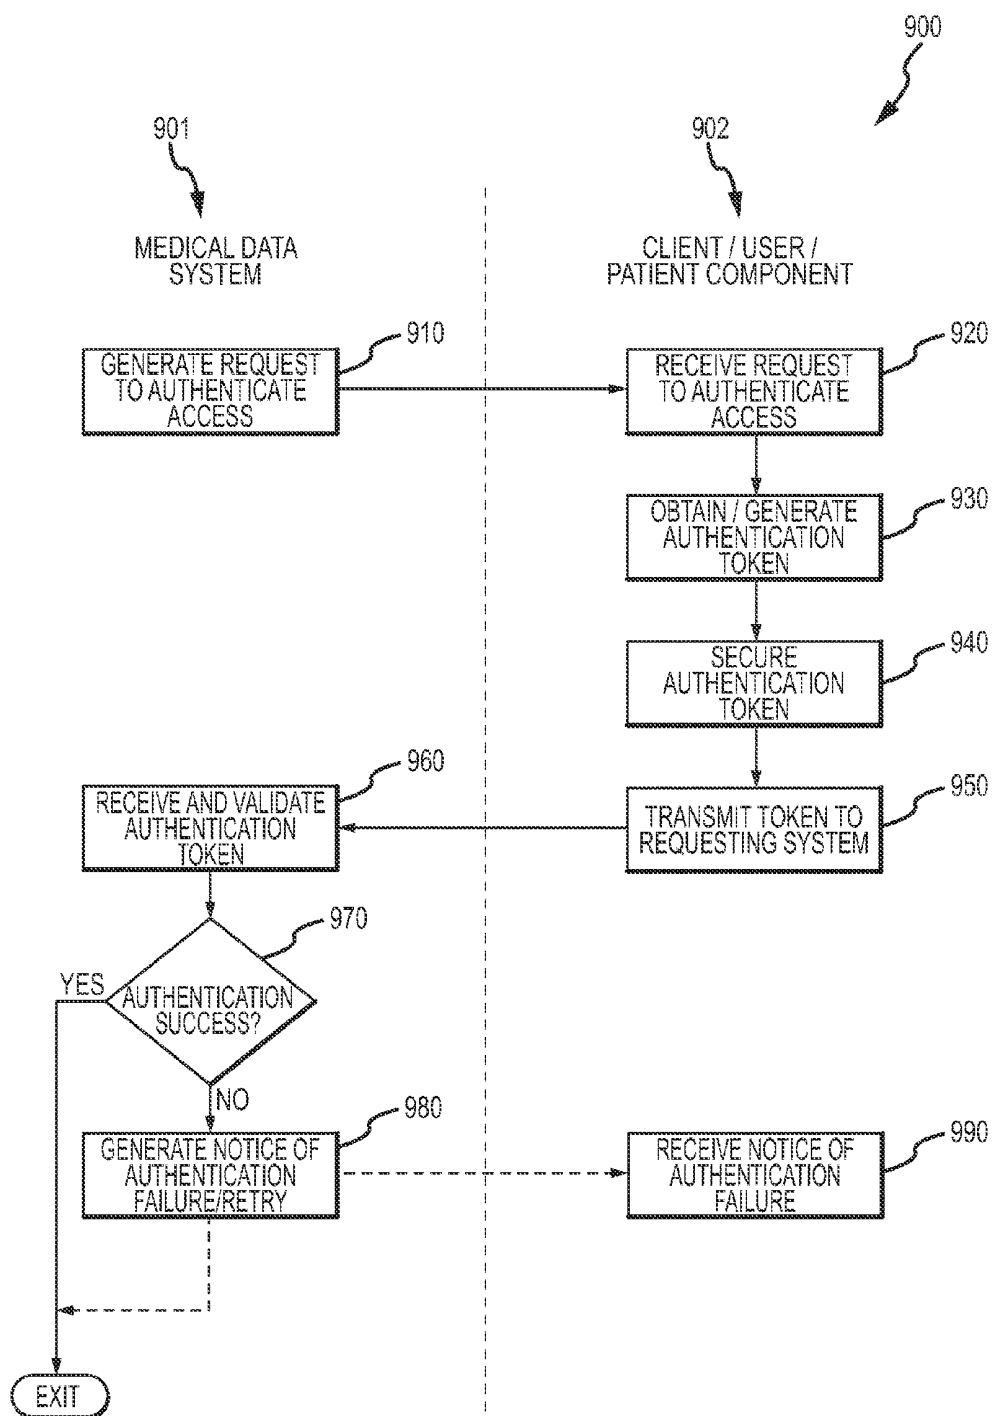


FIGURE 9

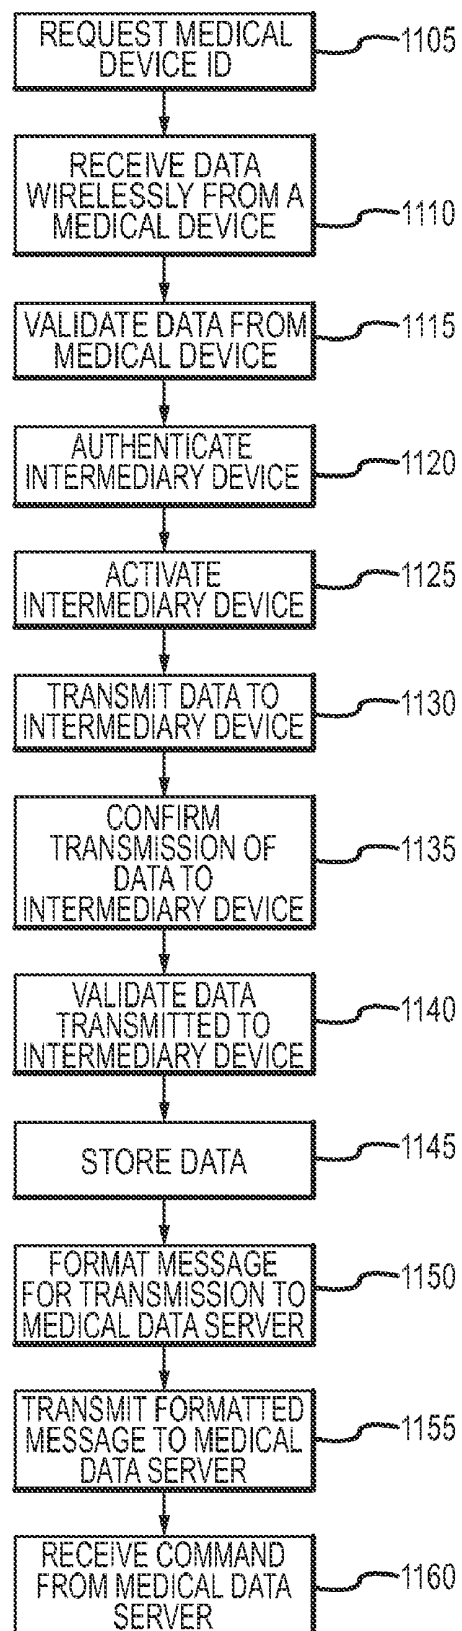


FIGURE 10

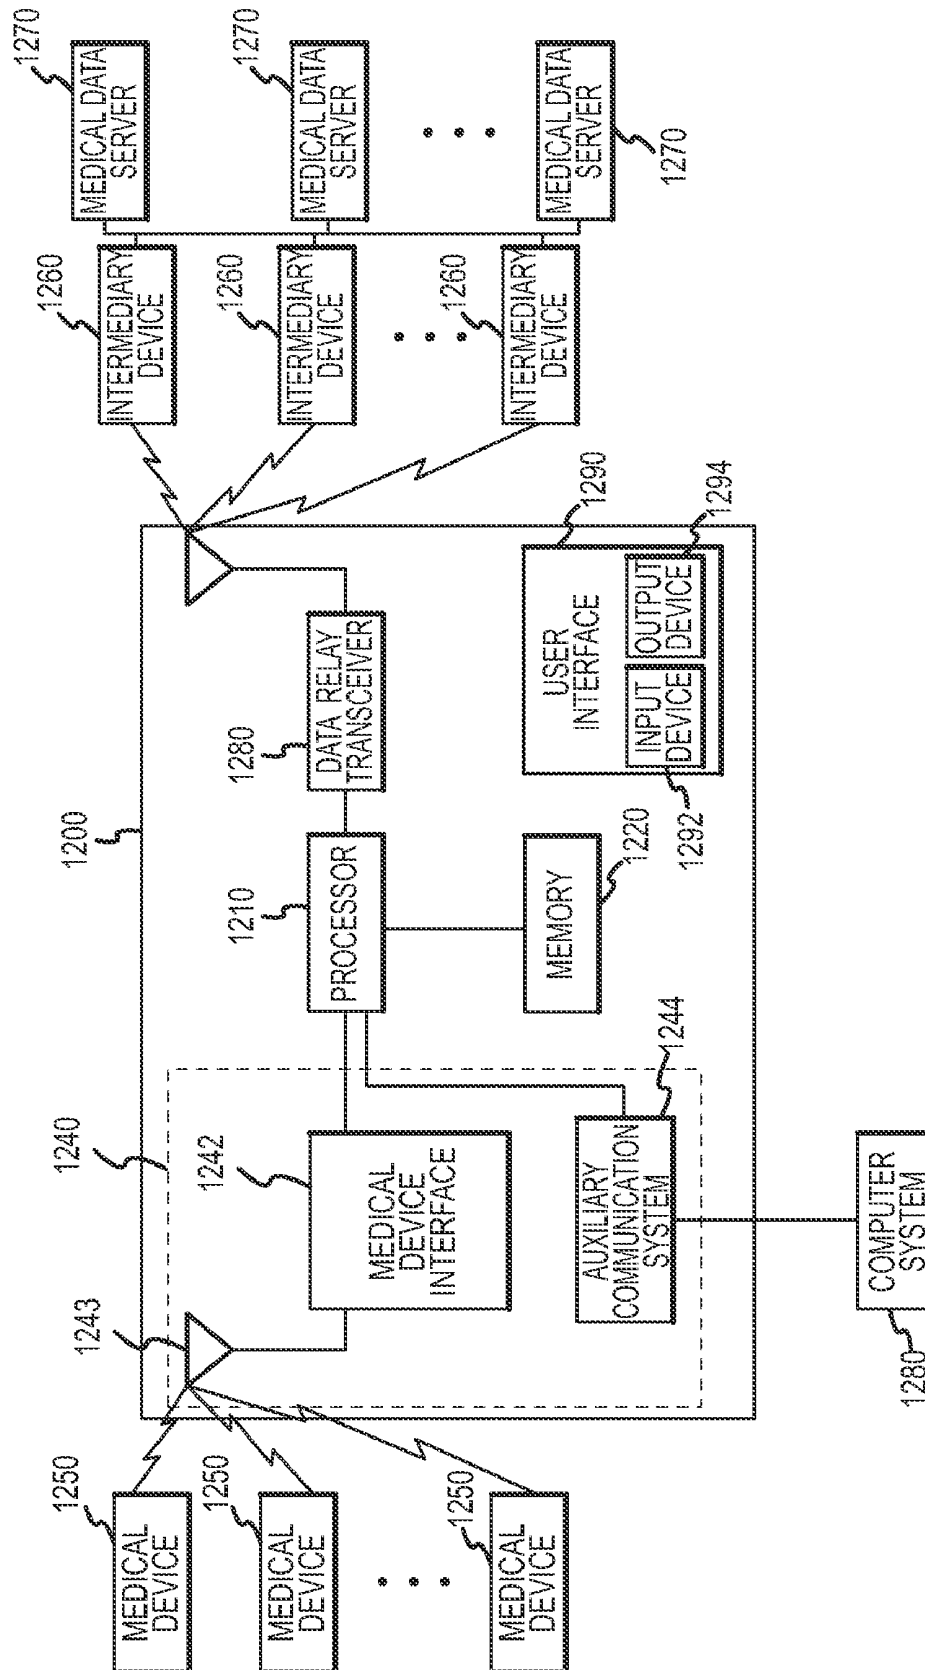


FIGURE 11

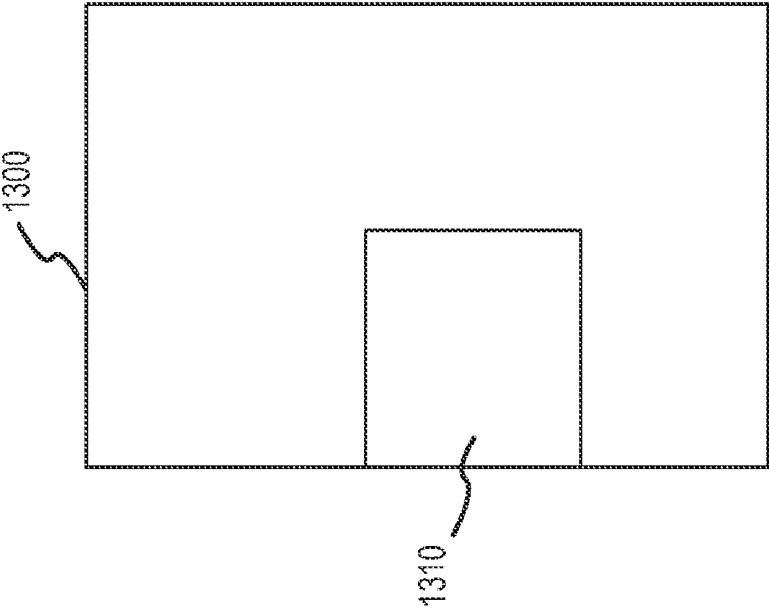


FIGURE 12A

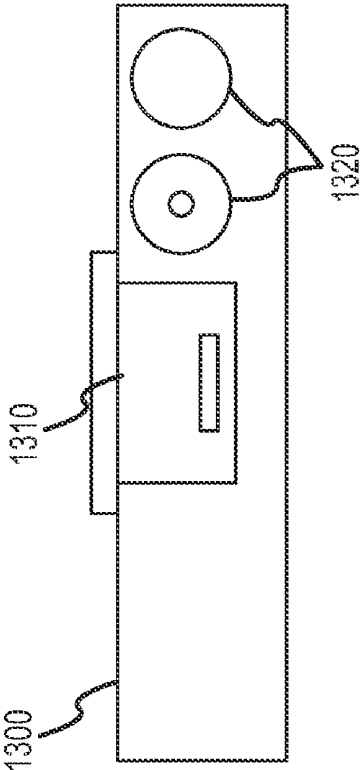


FIGURE 12B

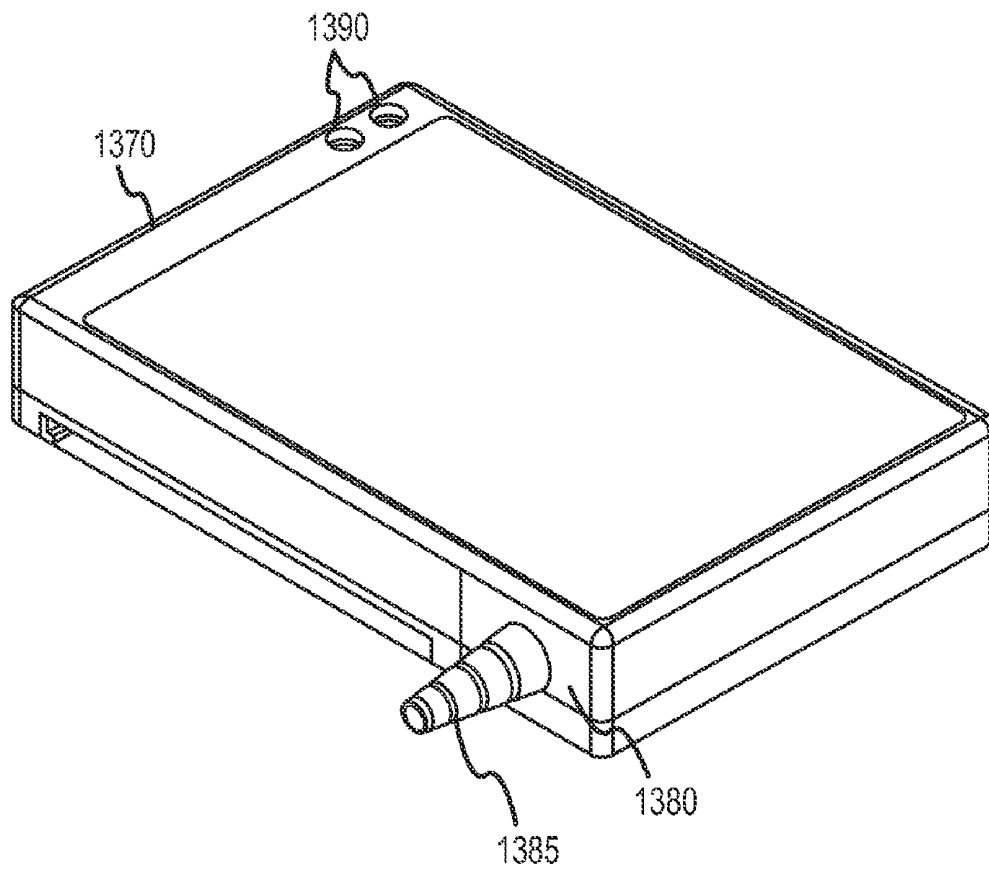


FIGURE 12C

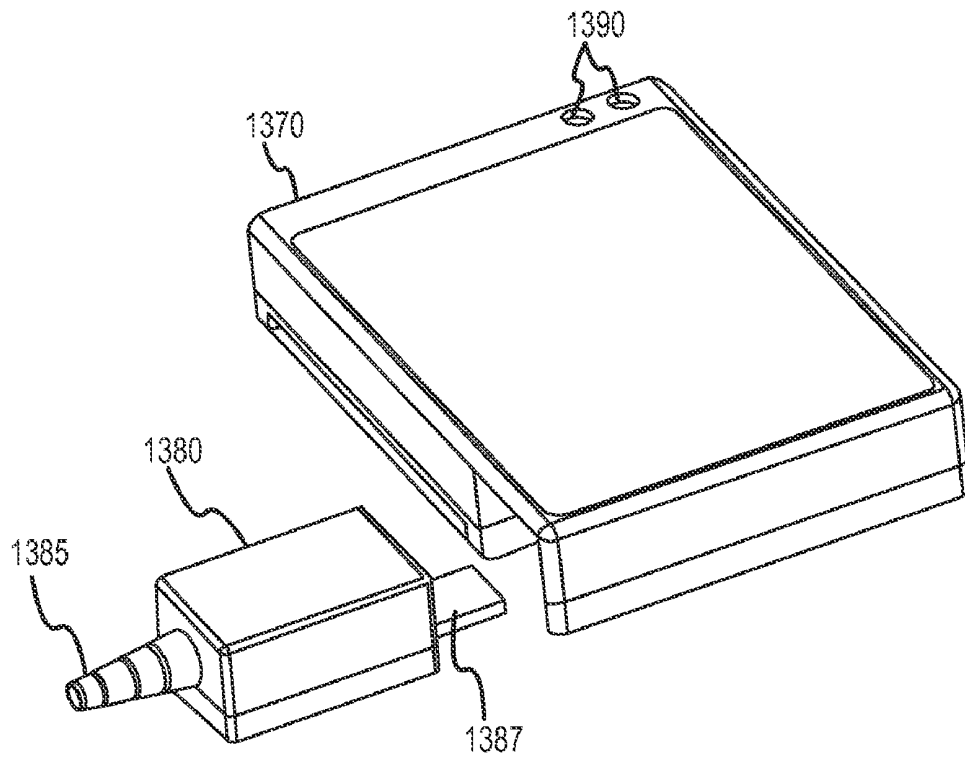


FIGURE 12D

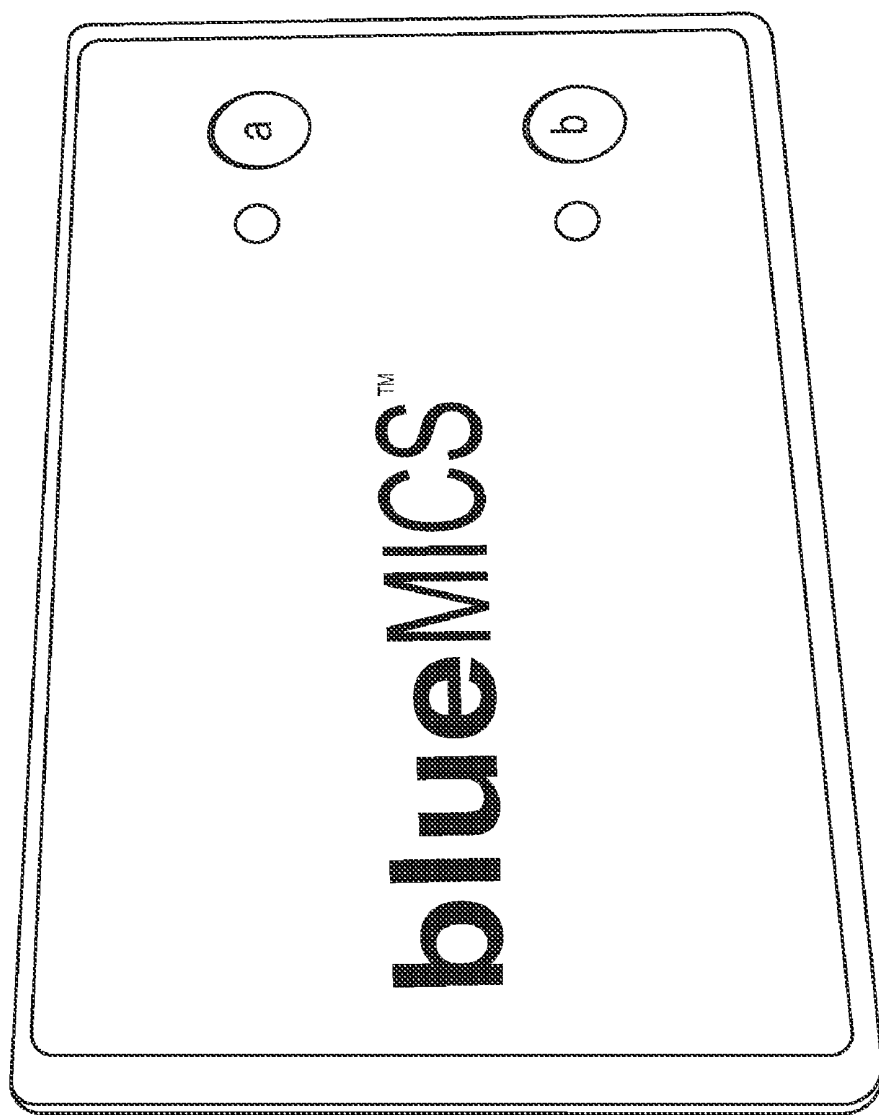


FIGURE 12E

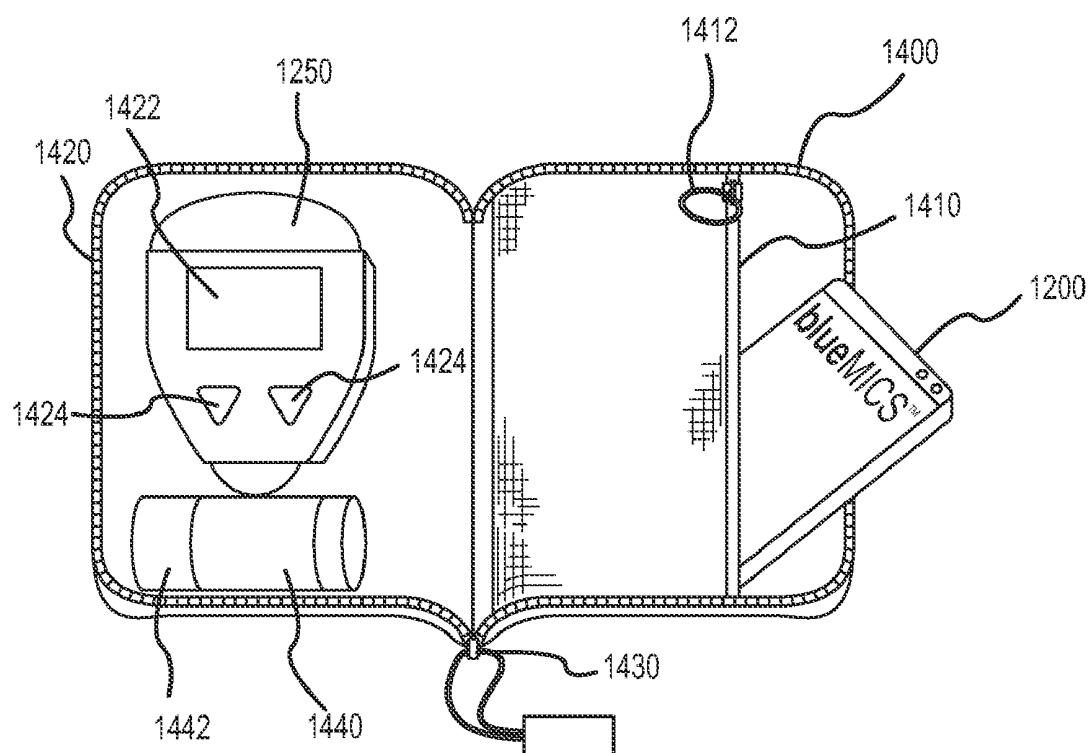


FIGURE 13

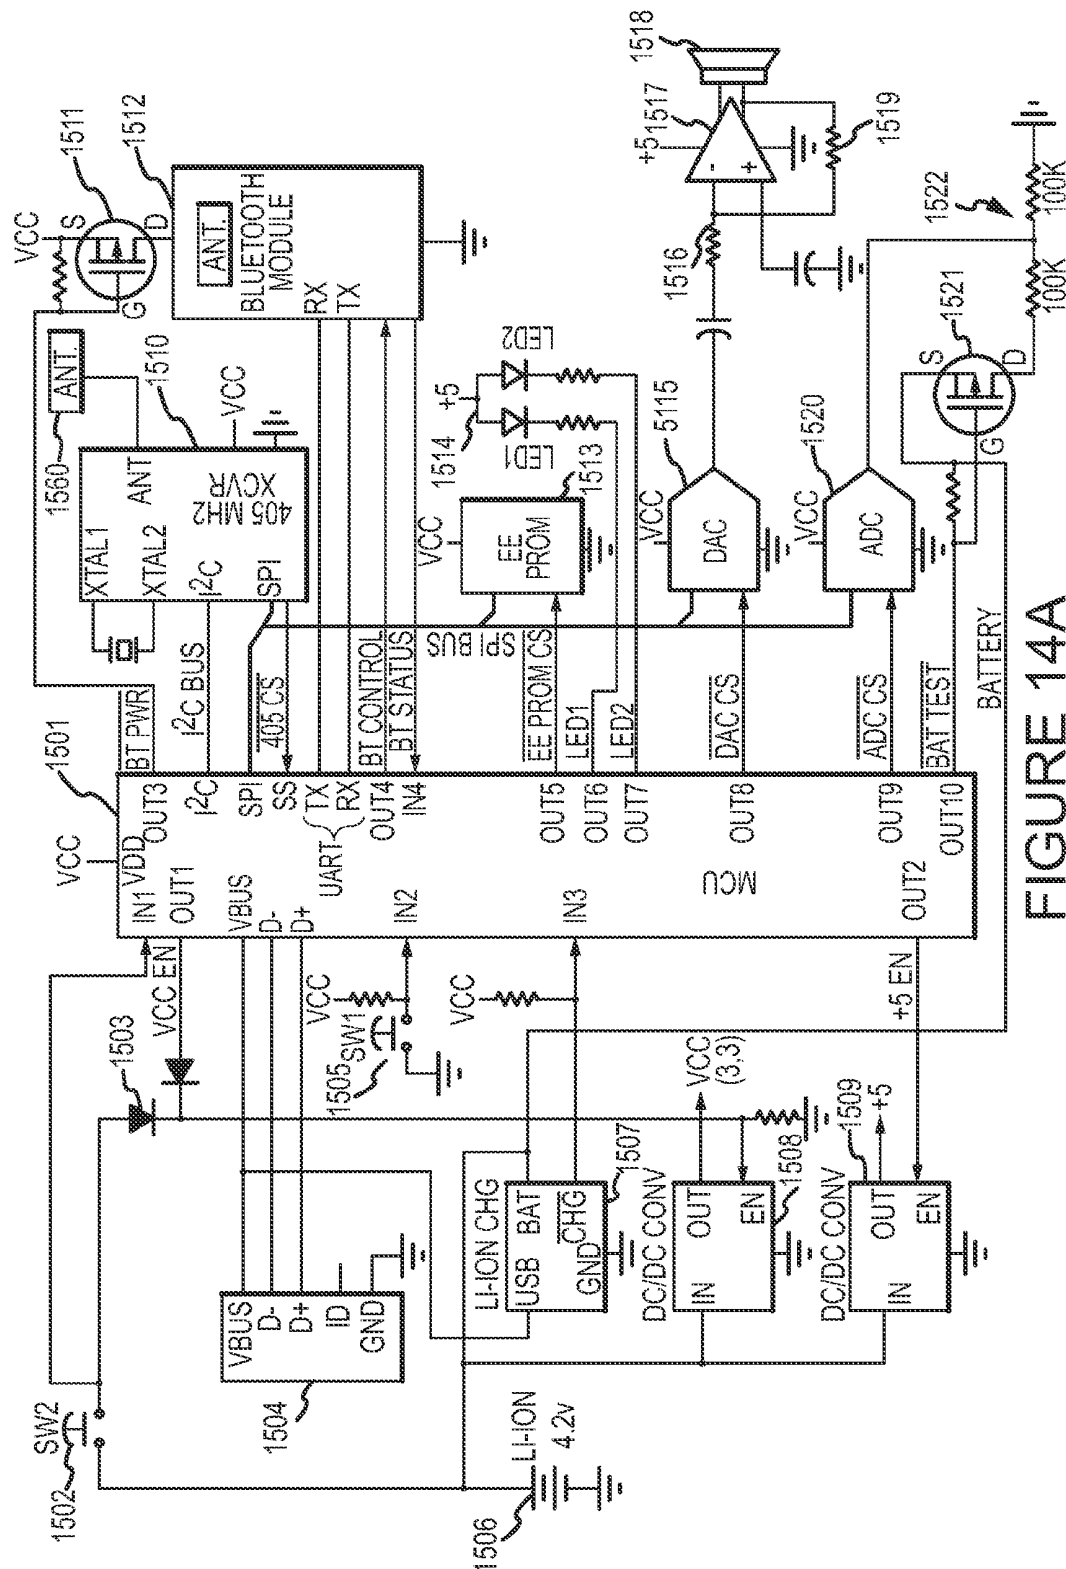


FIGURE 14A

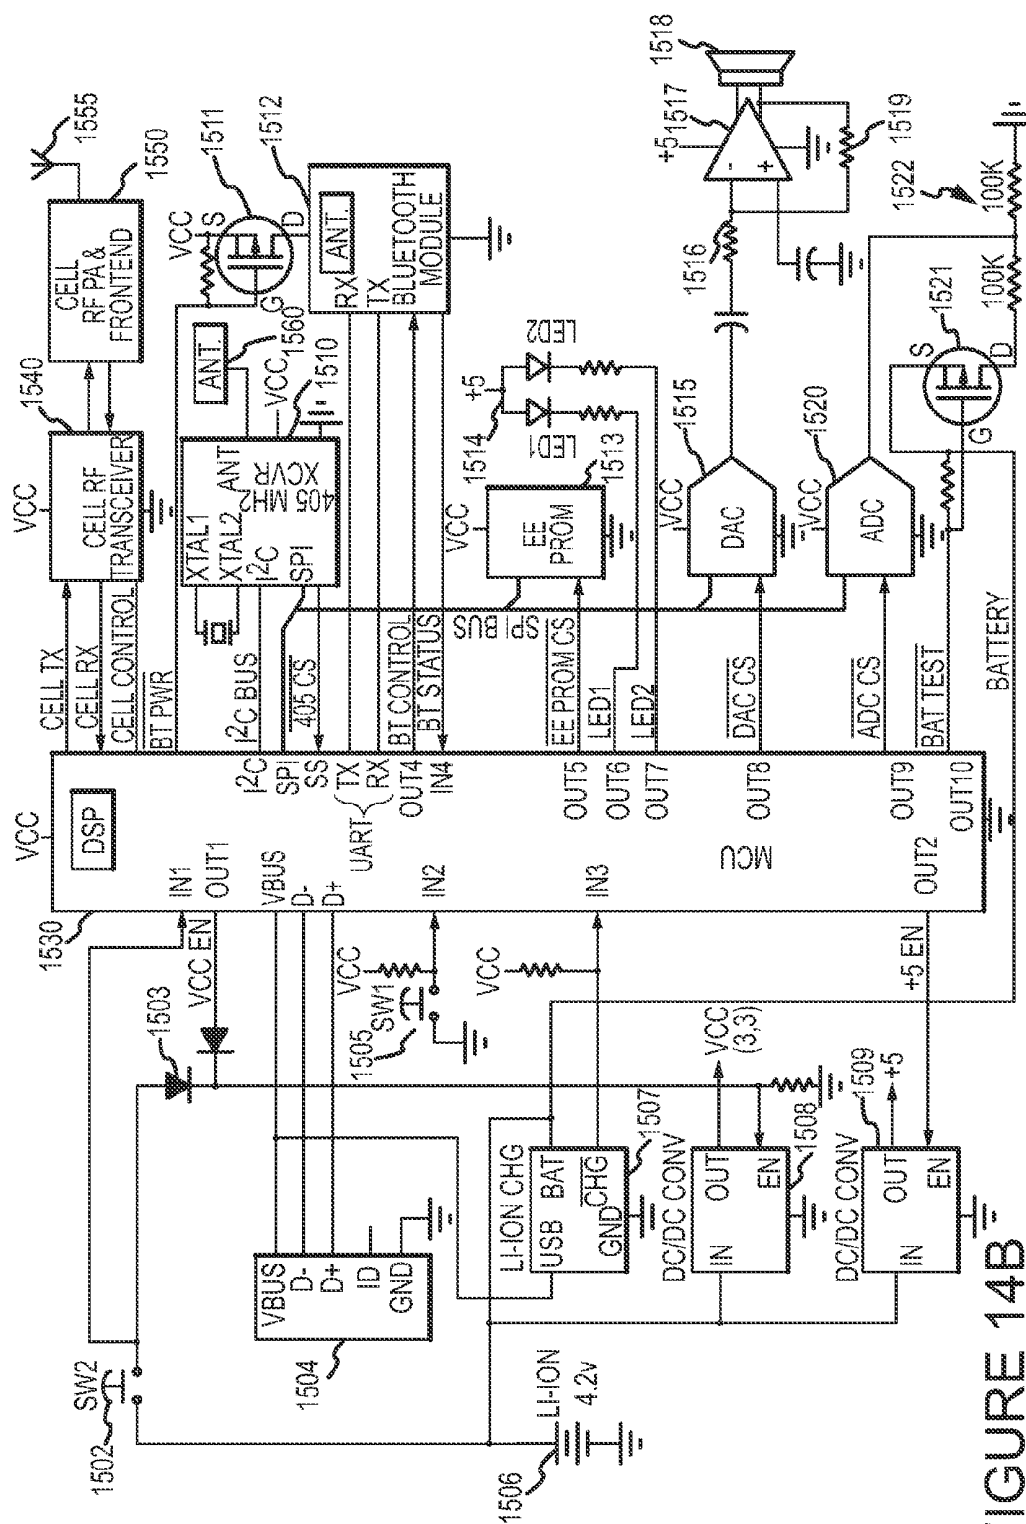


FIGURE 14B

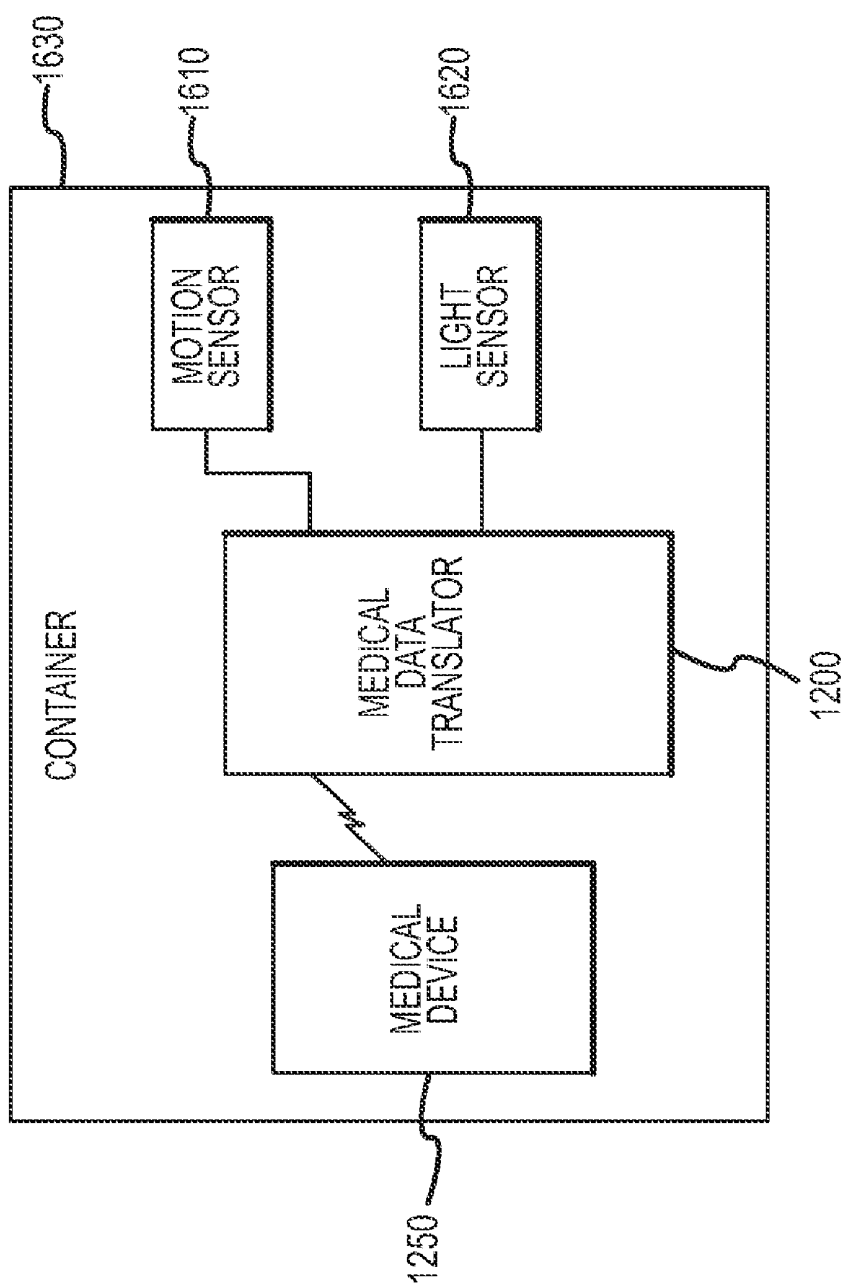


FIGURE 15

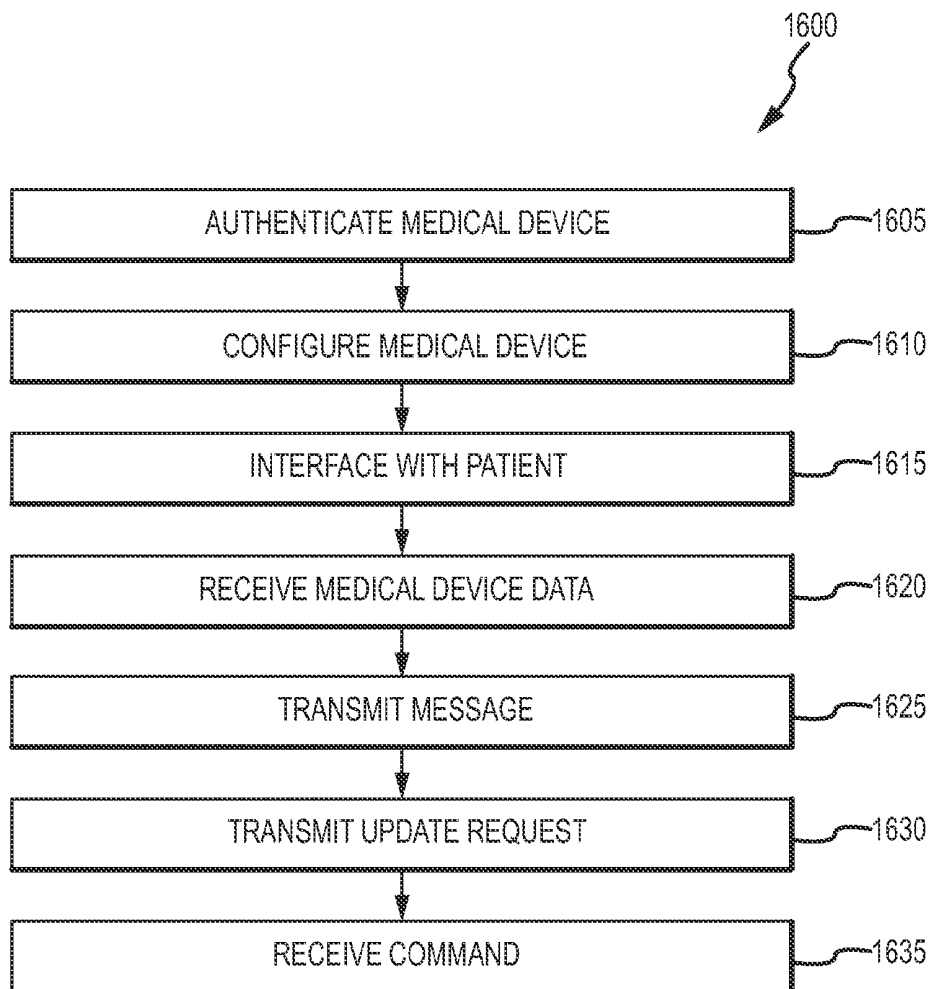


FIGURE 16

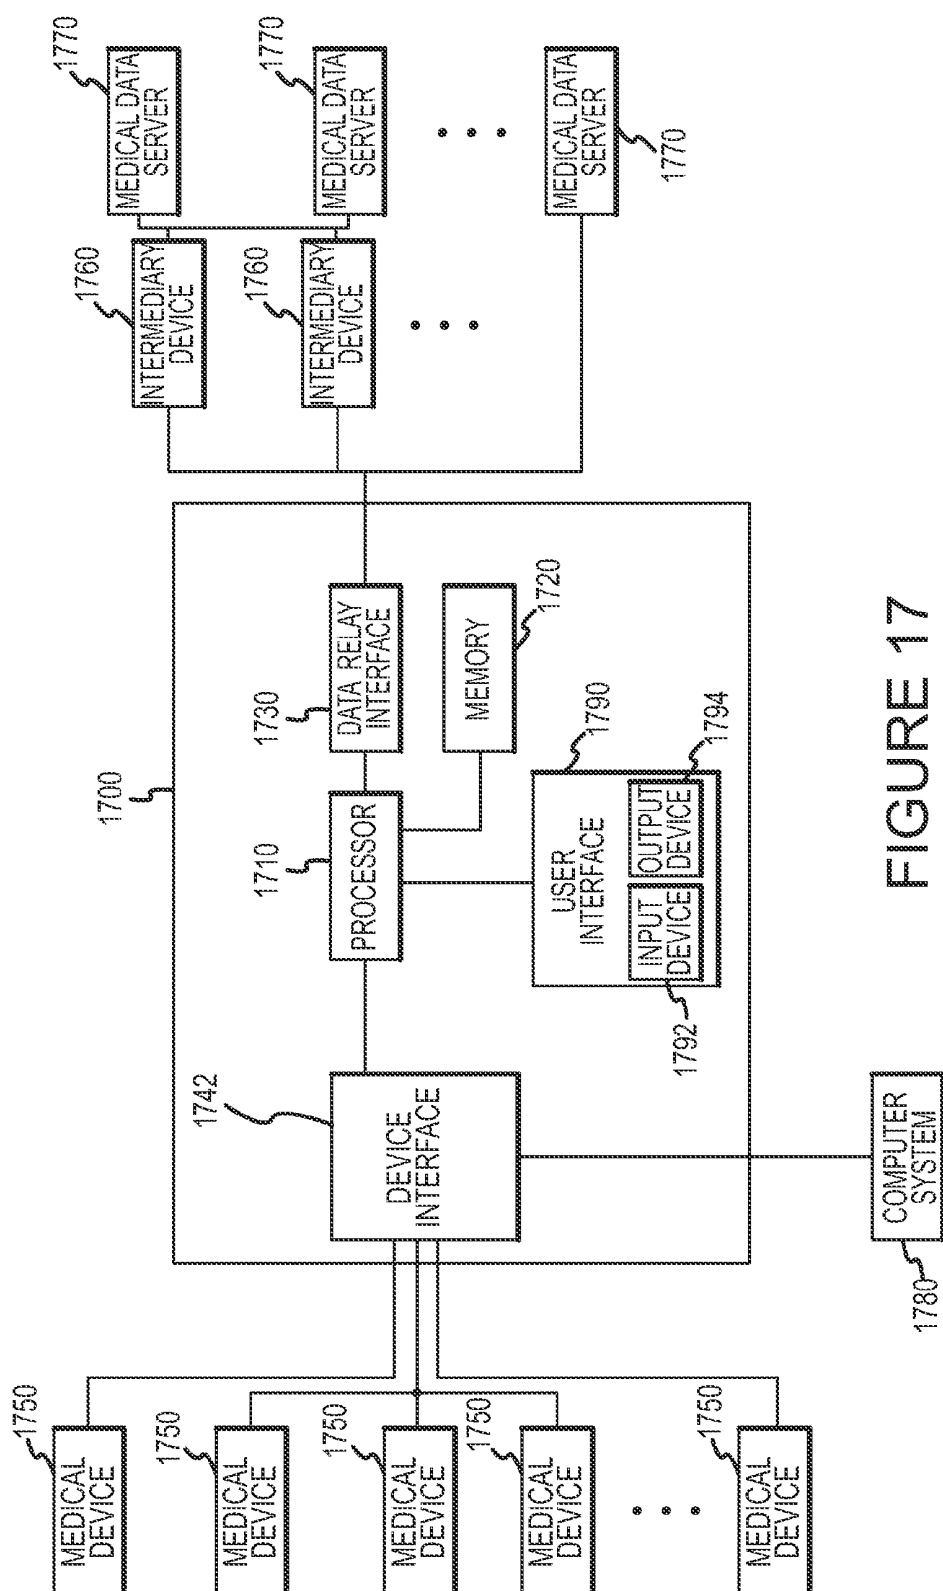


FIGURE 17

METHOD FOR MEDICAL DATA COLLECTION AND TRANSMISSION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application claims priority to U.S. Provisional Patent Application Ser. No. 60/862,743, filed Oct. 24, 2006; and claims priority to and is a continuation of: U.S. Patent Publication No. 20080097908 filed as U.S. Utility patent application Ser. No. 11/876,689 on Oct. 22, 2007; U.S. Patent Publication No. 20080097909 filed as U.S. Utility patent application Ser. No. 11/876,695 on Oct. 22, 2007; U.S. Patent Publication No. 20080097551 filed as U.S. Utility patent application Ser. No. 11/876,708 on Oct. 22, 2007; U.S. Patent Publication No. 20080103554 filed as U.S. Utility patent application Ser. No. 11/876,711 on Oct. 22, 2007; U.S. Patent Publication No. 20080103370 filed as U.S. Utility patent application Ser. No. 11/876,713 on Oct. 22, 2007; U.S. Patent Publication No. 20080097910 filed as U.S. Utility patent application Ser. No. 11/876,719 on Oct. 22, 2007; U.S. Patent Publication No. 20080215360 filed as U.S. Utility patent application Ser. No. 11/876,725 on Oct. 22, 2007; U.S. Patent Publication No. 20080097911 filed as U.S. Utility patent application Ser. No. 11/876,744 on Oct. 22, 2007; U.S. Patent Publication No. 20080097552 filed as U.S. Utility patent application Ser. No. 11/876,732 on Oct. 22, 2007; U.S. Patent Publication No. 20080097917 filed as U.S. Utility patent application Ser. No. 11/877,525 on Oct. 23, 2007 now abandoned; U.S. Patent Publication No. 20080103555 filed as U.S. Utility patent application Ser. No. 11/877,541 on Oct. 23, 2007; U.S. Patent Publication No. 20080218376 filed as U.S. Utility patent application Ser. No. 11/877,550 on Oct. 23, 2007; U.S. Patent Publication No. 20080224852 filed as U.S. Utility Patent application Ser. No. 11/877,582 on Oct. 23, 2007; U.S. Patent Publication No. 20080097550 filed as U.S. Utility patent application Ser. No. 11/877,930 on Oct. 24, 2007; U.S. Patent Publication No. 20080183502 filed as U.S. Utility patent application Ser. No. 11/877,946 on Oct. 24, 2007; U.S. Patent Publication No. 20090234672 filed as U.S. Utility patent application Ser. No. 11/877,966 on Oct. 24, 2007; U.S. Patent Publication No. 20080097793 filed as U.S. Utility patent application Ser. No. 11/877,994 on Oct. 24, 2007; and U.S. Patent Publication No. 20090112769 filed as U.S. Utility patent application Ser. No. 11/923,013 on Oct. 24, 2007 now abandoned; the disclosures of which are incorporated by reference in their entirety for all purposes.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

Not applicable.

NOTICE OF INCLUDED COPYRIGHTED MATERIAL

A portion of the disclosure of this patent document contains material which is subject to copyright protection. The copyright owner has no objection to the facsimile reproduction by anyone of the patent document or the patent disclosure, as it appears in the Patent and Trademark Office patent file or records, but otherwise reserves all copyright rights whatsoever. All trademarks and service marks identified herein are owned by the applicant.

DESCRIPTION OF THE INVENTION

1. Field of the Invention

The present invention relates to medical data collection and transmission.

2. Background of the Invention

Historically, patient medical care was often provided for in the patient's home or some other environment apart from a clinical setting. Physicians, midwives, or other healthcare providers would make house calls, observe patient symptoms, formulate diagnoses, and provide treatment. As the state of the art of health care evolved over time, the number of house calls made by healthcare professionals diminished. In large part, health care providers conducted fewer and fewer house calls because it became impractical to bring bulky medical diagnosis and test equipment to the patient. Likewise, it was not cost effective or intellectually feasible for patients to purchase and operate the complicated and expensive medical machines in a home setting. Therefore, the health care model changed dramatically, emphasizing patient visits to health care facilities where an assortment of state-of-the-art test equipment would be available to assist doctors in more accurately assessing and treating patients. This meant that patients were now expected to come to the doctor, rather than the other way around.

Innovations in electronics in the last twenty years have made available a large number of more affordable and patient-operable medical devices that obviated, at least in part, the need for the patient to go to a facility each time a medical test or device checkup was required. Size and expense were not the only factors making this possible; since the new devices provided sophisticated processing in smaller form factors, the technical complexity required to operate the devices were reduced to a level that would not overwhelm a layperson's knowledge. Unfortunately, although portable medical devices such as blood glucose meters now allow patients to perform tests outside the context of medical facilities, patients still need to meet with health care providers to discuss the results obtained.

Some medical devices include ports to allow the communication of data to and from the medical device through a cable or other wired connection. Medical devices that communicate through such wired connections allow healthcare providers to monitor the operation of the medical device, as well as to optionally monitor a patient's biological and biometric information, the patient's behavior, and other information pertinent to the treatment of the patient. However, the manner in which medical devices communicate data varies depending on the type and manufacturer of the device, and therefore, proprietary equipment has been designed to communicate with medical devices only using a specific type of wired connection based on the type of medical device being used.

Medical devices can communicate through a wide range of wired connections. In the context of this application, "wired connection" generally refers to any physical connection that a medical device can communicate through. For example, "wired connections" can also refer to a waveguide, such as an optical fiber. Other wired connections that can be used by various medical devices include various sizes of tip and sleeve (TS), tip, ring, and sleeve (TRS), and tip, ring, ring, and sleeve (TRRS) connections. Such connections are also commonly referred to as "RCA plugs," "phone plugs," and "stereo jacks" and commonly include plug diameters of 2.5 mm and 3.5 mm when used with medical devices. Other wired connections, such as serial peripheral interface bus (SPI) connections, universal serial bus (USB) connections, RS-232 serial

connections, Firewire (IEEE 1394) and Ethernet connections may also be used. A wired connection can also include any soldered electrical connection, trace on a circuit board, or other physical connection. Each of these connections vary not only in the physical structure of the connection, but also in the communication protocols used to transfer data. It would thus be desirable to have the capability to communicate with a variety of medical devices regardless of the specific wired connection they use.

Some medical devices include wireless transmitters for the communication of data to and from the medical device. For medical devices implanted in a patient, such as a pacemaker, wireless communication allows a healthcare provider to monitor the operation of the medical device, and to optionally monitor a patient's biological and biometric information, the patient's behavior, and other information pertinent to the treatment of the patient. However, the manner in which medical devices communicate data varies depending on the type and manufacturer of the device, and therefore, proprietary equipment has been designed to wirelessly communicate with medical devices only on a specific frequency and using a particular data communication protocol based on the type of medical device being used.

In the United States, medical devices can broadcast on a wide range of frequencies. For example, older implantable devices use frequencies ranging from 32 KHz to 175 KHz. The Federal Communications Commission (FCC) has allocated three frequency bands for use with wireless medical device communication, known as the Wireless Medical Telemetry System (WMTS). The WMTS frequency bands include the frequency ranges of 608-614 MHz, 1395-1400 MHz, and 1427-1432 MHz. Additionally, the FCC has allocated a band specifically for use by implanted medical devices. This band is known as the Medical Implant Communication Service (MICS) and includes the 402-405 MHz frequency band. It would be desirable to have the capability to communicate with medical devices using any of these frequency bands using a wide variety of wireless protocols that might be broadcast by the devices.

To make patient monitoring more convenient, Remote Patient Monitoring (RPM) was developed. Remote Patient Monitoring (RPM) generally refers to monitoring one or more conditions of a patient without requiring the patient to visit a hospital, doctor's office, or other healthcare facility. RPM can increase the efficiency and effectiveness of providing care to patients while reducing costs. RPM can be particularly useful when a patient has a long-term or chronic disease that would otherwise require frequent visits to a healthcare facility and/or where a patient's treatment regimen should be modified based on changed patient conditions that are monitored by one or more medical devices, such as a pacemaker or glucose meter. For example, Type-I Diabetes patients (a lifelong condition) use glucose meters to monitor their blood sugar level to assist in determining when to take insulin—it would be desirable if such information could be quickly, easily, and effectively relayed to a health care provider for review and analysis.

Conventional RPM generally involves the use of a specific monitoring device installed in a patient's home. The device collects data concerning the patient's condition and relays the data to a healthcare provider. Some conventional systems require a patient to manually enter the data. For example, a diabetes patient using a conventional system for RPM may be required to sample their blood sugar level using a glucose meter, take note of the reading, and then manually enter the level in the conventional system. There are drawbacks with these conventional devices. Because of their complexity and

proprietary interfaces, many are very expensive, which reduces the cost-savings benefit of RPM. Additionally, they often require a land-line connection (such as phone or VPN) to transmit data and/or are physically bulky/heavy and therefore difficult to transport. Furthermore, conventional systems are often unable to provide data to healthcare providers quickly where data must be manually entered by a patient, which can reduce the level of benefit the patient receives from RPM. The present invention addresses these and other issues.

SUMMARY OF THE INVENTION

Methods and systems according to the present invention may operate in conjunction with any wired or wireless connection, including those described herein, and may operate in conjunction with multiple wired or wireless connections. In exemplary embodiments, methods and systems according to the present invention may be configured to receive medical device data transmitted in any format and from any medical device.

An exemplary method according to various aspects of the present invention includes receiving data from a medical device and transmitting a message including at least a portion of the received data to a provided medical data server. This exemplary method further includes receiving a command from the medical data server.

Both the foregoing summary and the following detailed description are exemplary and explanatory only and are not restrictive of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

A more complete understanding of the present invention may be derived by referring to the detailed description and claims when considered in connection with the following illustrative figures.

FIG. 1 is a flow diagram depicting an exemplary process for medical data interchange according to various aspects of the present invention.

FIG. 2A is a block diagram depicting an exemplary system for medical data interchange according to various aspects of the present invention.

FIG. 2B is a block diagram depicting another exemplary system for medical data interchange according to various aspects of the present invention.

FIG. 2C is a block diagram depicting yet another exemplary system for medical data interchange according to various aspects of the present invention.

FIGS. 3A and 3B depict top and rear views, respectively, of an external casing for a medical data interchange device according to various aspects of the present invention.

FIGS. 3C and 3D depict perspective views of another embodiment of an external casing for a medical data interchange device according to various aspects of the present invention.

FIG. 3E depicts a perspective view of yet another embodiment of an external casing for a medical data interchange device according to various aspects of the present invention.

FIG. 4 depicts the interior of an exemplary container for holding a medical device and medical data interchange device according to various aspects of the present invention.

FIGS. 5A and 5B are circuit diagrams depicting elements of an exemplary medical data interchange device according to various aspects of the present invention.

FIG. 6 is a circuit diagram illustrating elements of an exemplary embodiment of a smart cable with ID and wake-up capability.

FIG. 7 is a circuit diagram illustrating elements of an alternate exemplary embodiment of a smart cable with ID capability.

FIG. 8 is a block diagram depicting a container including light and motion sensors for activating a medical data interchange device in accordance with various aspects of the present invention.

FIG. 9 is a flow diagram showing an exemplary process for authenticating access to a system component of the present invention.

FIG. 10 is a flow diagram depicting an exemplary process for medical device monitoring according to various aspects of the present invention.

FIG. 11 is a block diagram depicting an exemplary system for medical device monitoring according to various aspects of the present invention.

FIGS. 12A and 12B depict top and side views, respectively, of an external casing for a medical data translator device according to various aspects of the present invention.

FIGS. 12C and 12D depict perspective views of another embodiment of an external casing for a medical data translator according to various aspects of the present invention.

FIG. 12E depicts a perspective view of yet another embodiment of an external casing for a medical data translator according to various aspects of the present invention.

FIG. 13 depicts the interior of an exemplary container for holding a medical device and medical data translator according to various aspects of the present invention.

FIGS. 14A and 14B are circuit diagrams depicting elements of exemplary medical data translators according to various aspects of the present invention.

FIG. 15 is a block diagram depicting a container including light and motion sensors for activating a medical data translator in accordance with various aspects of the present invention.

FIG. 16 is a flow diagram illustrating an exemplary method in accordance with various aspects of the present invention.

FIG. 17 is a block diagram depicting an exemplary system for medical data collection and transmission.

DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS

Exemplary Method Using Wired Communication

An exemplary method according to an aspect of the present invention is depicted in FIG. 1. In this method, an identifier is requested from a medical device (105), and data from the medical device is received (110) and validated (115) through a wired connection. An intermediary device such as a mobile phone or personal digital assistant is authenticated (120) and activated (125). The data is transmitted by the medical device to the intermediary device (130) and the transmission to the intermediary device is confirmed (135) and validated (140). The data is stored (145) in the intermediate device. A message is formatted (150) and transmitted to a medical data server (155). Optionally, a command can be received from the medical data server (160) and optionally relayed from the intermediary device. Any combination and/or subset of the elements of the method depicted in FIG. 1 may be practiced in any suitable order and in conjunction with any system, device, and/or process. The method shown in FIG. 1 can be implemented in any suitable manner, such as through software operating on one or more computer systems. Exemplary systems for performing elements of the method shown in FIG. 1 are discussed later in this description.

Request Medical Device ID

In the exemplary process according to aspects of the present invention depicted in FIG. 1, an identifier is requested from a medical device providing the data to be monitored (105). Any suitable identifier may be provided, such as the serial number of the medical device and/or a numeric, alphabetic, alphanumeric, or symbolic identifier. The medical device identifier can be used to determine whether the correct medical device is being monitored. The medical device identifier can also be used to determine the manufacturer, model, type, characteristics, or other information pertinent to the medical device and/or the patient(s) it monitors. The medical device identifier may be received passively, such as from a medical device that automatically includes its identifier as part of its telemetry broadcast. Alternatively, the medical device can be polled to request the medical device identifier. The medical device identifier need not be requested from the medical device each time the medical device is being monitored. For example, the medical device identifier may be stored in a storage medium for future reference.

Receive Data from a Medical Device Through a Wired Connection

In the exemplary method shown in FIG. 1, data is received through a wired connection from the medical device (110). As stated previously, a "wired connection" in the context of this application refers generally to any physical connection that allows communication between two devices. Wired connections thus include, without limitation: tip and sleeve (TS), tip, ring, and sleeve (TRS), and tip, ring, ring, and sleeve (TRRS) connections; serial peripheral interface bus (SPI) connections; universal serial bus (USB) connections; RS-232 serial connections, Ethernet connections, optical fiber connections, and Firewire connections. Data from a medical device may be received using any number and combinations of such connections, as well as any other type of connection. Additionally, medical device may communicate data through a wired connection using any suitable format and communications protocol.

Systems implementing the method depicted in FIG. 1 are preferably small, light, and portable, allowing patients monitored by medical devices to lead active lifestyles without being forced to remain close to a non-portable system receiving the data from the medical device. Data can be received from any medical device, such as a blood glucose meter, a pacemaker, a blood pressure monitor, an insulin pump, a pulse oximeter, a holter monitor, an electrocardiograph, an electroencephalograph, a blood alcohol monitor, an alcohol breathalyzer, an alcohol ignition interlock, a respiration monitor, an accelerometer, a skin galvanometer, a thermometer, a patient geolocation device, a scale, an intravenous flow regulator, patient height measuring device, a biochip assay device, a sphygmomanometer, a hazardous chemical agent monitor, an ionizing radiation sensor, a monitor for biological agents, a loop recorder, a spirometer, an event monitor, a prothrombin time (PT) monitor, an international normalized ratio (INR) monitor, a tremor sensor, a defibrillator, or any other medical device.

A medical device that includes a combination of different medical devices (such as those listed previously) may be monitored in accordance with the present invention. The medical device can be partially or completely implanted in a patient, such as in the case of a pacemaker. Data from the medical device can be received through any number of other relay devices, such as routers, hubs, bridges, switches, and modems. Where the medical device is completely implanted in the patient, such relay devices can receive data from the medical device wirelessly and retransmit the data through a

wired connection. The medical device may also be located externally to a patient. The medical device may be connected to a patient (for example, through one or more electrodes), or operate independent of any coupling to a patient, such as a scale. The medical device may also operate in conjunction with a temporary interfacing with a patient, such as the case of the cuff of a blood pressure monitor encompassing the arm of a patient to take a reading.

The medical device data can be received by any person, system, device, or other suitable recipient. The exemplary method in FIG. 1 may be practiced manually by a human being, automatically by a device, or a combination of the two. Exemplary devices for performing the method illustrated in FIG. 1 are depicted in FIGS. 2A, 2B, and 2C, and are discussed in detail below.

Data can be received directly from a medical device. For example, some medical devices such as glucose meters have ports that allow data to be communicated through a cable. As mentioned previously, a medical device can also provide data using another device, system, or other entity. In one embodiment of the present invention, for example, a medical device provides data through a serial port (a wired connection) to a computing device. The computing device is in turn connected to an Ethernet router or hub. The data can thus be received through an Ethernet connection from the router or hub. In another exemplary embodiment of the present invention, a human patient retrieves data from the medical device and then provides the data through a keypad, microphone, or other suitable input device.

The medical device data can be received from a plurality of different medical devices, where each medical device may perform any combination of functions. For example, data from a glucose meter, blood pressure monitor, and combination scale/height measuring device each transmitting data in different formats and through different wired connections may each be received in accordance with the present invention. In the case where a plurality of medical devices transmits data in response to a request for data, each device in the plurality of devices can be sent such a request separately. Alternatively, a plurality of medical devices automatically transmitting data in the same format, and potentially at the same time (such as in the case of multiple devices of the same type and/or from the same manufacturer) can be received in accordance with the present invention by, for example, using separate wired connections. When data has been received from a plurality of medical devices, in one embodiment, a list of the medical devices may be displayed on a user interface, and optionally, the user may be prompted to select one, all, or none of the plurality medical devices, whose data is desired to be transmitted to the medical data server. The data for the selected set of medical devices is then relayed as described with alternate embodiments as described herein. Any other suitable method for receiving data from a plurality of medical devices may also be used in conjunction with the present invention.

Any type of data may be received from a medical device. For example, the data may include information regarding a patient, such as the patient's biological and biometric information, the patient's behaviors, results of analysis of physical patient parameters, and information regarding the patient's environment. For example, a medical device such as a glucose meter could provide data regarding a patient's current (or last measured) blood glucose level, the date and time the patient last used the glucose meter, and the current temperature or other environmental factors that might affect a glucose test. Other possible environmental parameters that may be included in the data received from a medical device include a

battery charge level, a temperature, a barometric pressure, a code relating to an accessory for the medical device, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, and a quality of service (QoS), and combinations thereof. Data received from a medical device may also include any other suitable information, such as diagnostic information regarding the medical device.

The medical device data may provide data relating to a single patient or multiple patients. In the case where a single medical device provides data regarding multiple patients, the data can be identified with an individual patient either in the data received by medical device (such as by using a patient identifier) or through processing in accordance with the present invention.

The medical device can provide the data in any format. Different medical devices from different manufacturers often use different formats for providing data. For example, data from a glucose meter may be provided in a series of fixed-length data records followed by a terminator indicator (such as a null or other predefined character) and/or a checksum for validating the data. Any type of data may be provided. In the case of a glucose meter, the data may include one or more readings of a patient's blood glucose level and the date and time each reading was taken. The medical device identifier discussed previously may be used to determine a specific data format used by a medical device. Alternatively, a data format may be specified by a user or selected by analyzing the format of the data received and comparing it to a set of known medical device data formats.

Validate Data

In the exemplary process shown in FIG. 1, the data from the medical device is validated (115). The data from the medical device can be validated in any suitable manner to achieve any result. For example, the data from the medical device may be validated to ensure it was transmitted properly and completely. The medical device data may also be validated to ensure it was provided from a specific medical device or particular type of medical device. The data may also be validated to ensure that fields in the data correspond to predetermined values and/or are within certain thresholds or tolerances. Any number, code, value or identifier can be used in conjunction with validating the medical device data. For example, the data can be validated by analyzing a medical device serial number, a medical device identifier, a patient identifier, one or more parity bits, a cyclic redundancy checking code, an error correction code, and/or any other suitable feature.

Authenticate/Authorize Intermediary Device

In the exemplary method depicted in FIG. 1, an intermediary device receiving the data is authenticated (120). In the context of the present invention, the intermediary device includes any type of system or device capable of receiving the medical device data in any manner. Such intermediate devices may include, for example, personal computers, laptops, personal digital assistants, routers, hubs, bridges, switches, modems, and mobile computing devices. The intermediary device may process the data in any manner, and can transmit some or all of the data to another recipient, such as a medical data server. For example, but not by way of limitation, the intermediary device may include a personal computer or a mobile computing device, such as a laptop computer, a mobile wireless telephone, or a personal digital assistant (PDA). In an exemplary embodiment of the present invention, the intermediate device further includes software for receiving the medical device data, formatting a message based on the data, and transmitting the formatted message to a medical

data server. Such software can operate on any suitable mobile computing device and with any computer operating system. The intermediary device may include any number of other systems and devices suitable for receiving data from the medical device, processing the data, and/or transmitting the data to a medical data server. Further discussion regarding exemplary embodiments of intermediary devices is presented later in this description.

The intermediary device can receive the data directly from the medical device, or from one or more other devices. In one exemplary embodiment of the present invention, the intermediary device comprises a mobile computing device and is configured to receive data from one or more medical devices directly through one or more wired connections. In another exemplary embodiment of the present invention, the medical device transmits the data to a first device through a wired connection, which in turn transmits the medical device data to the intermediary device (wirelessly or through a wired connection).

The intermediary device may be authenticated to achieve any result. For example, transmission may be restricted only to authenticated devices operating as part of the present invention. Authentication can also prevent sensitive medical data from being viewed by unintended recipients. The intermediary device may also be authenticated to verify the intermediary device is able to receive, process, and/or transmit the medical device data to a medical data server. During authentication, the authenticated device or devices may also be remotely commanded, and such commands may include steps that configure devices to interoperate with components of the present invention. For example, but not by way of limitation, such steps may include the downloading of software applications, applets, embedded operating code, and/or data.

The intermediary device can be authenticated in any manner. For example, an intermediary device can be authorized to receive data from one or more medical devices using an authorization code. The authorization code can be any number, code, value or identifier to allow the intermediary device to be identified as a valid recipient of the data from the medical device. In one exemplary embodiment of the present invention, an intermediary device stores an authorization code and broadcasts the authorization code in response to a request for authorization. Unless the authorization code matches a code stored by the transmitter of the medical device data (such as the medical device itself or another transmission device), the medical device data is not transmitted to the intermediary device. Transmission of the medical device data to the intermediary device need not necessarily be predicated upon successful authentication of the intermediary device, however. For example, where the medical data is related to a medical emergency, the medical data could be transmitted to any suitable intermediary device within range, whether or not any intermediary device is actually able to be authenticated or authorized to receive the data.

In another exemplary embodiment of the present invention, an intermediary device receiving the medical device data using a wireless network protocol (such as Bluetooth) is authenticated based on whether the intermediary device advertises one or more services. In this context, advertised services reflect functions, utilities, and processes the intermediary device is capable of performing. The intermediary device broadcasts indicators of this functionality, thus "advertising" them to other systems and devices. In the present exemplary embodiment of the invention, unless the intermediary device advertises a service that is identifiable with the operation of the present invention (i.e. a process capable of

broadcasting the medical device data to a medical data server, for example), the intermediary device is not authenticated and thus the medical device data is not transmitted to the intermediary device.

5 Activate Intermediary Device

In the exemplary process depicted in FIG. 1, the intermediary device can be activated (125) prior to transmitting the medical device data to the intermediary device. Many devices, particularly mobile computing devices running on batteries, employ power-saving features to conserve battery life when not in use. In the case where an intermediary device is in a power-saving or standby mode, it may be necessary to activate the intermediary device before it can receive the medical device data. The intermediary device can be activated in any suitable manner. For example, a signal configured to activate the device may be transmitted to prepare the intermediary device to receive the medical device data.

Transmit Data to Intermediary Device

The medical device data is transmitted to the intermediary device (130) in the exemplary process depicted in FIG. 1. The data can be transmitted in any suitable manner. In one exemplary embodiment of the present invention, the medical device data is transmitted to the intermediary device using a wired connection, such as an RS-232 serial cable, USB connector, Firewire connector, or other suitable wired connection. The medical device data can also be transmitted to the intermediary device wirelessly using a wireless transmitter. Any suitable method of wireless communication can be used to transmit the medical device data, such as a Bluetooth connection, infrared radiation, Zigbee protocol, Wibree protocol, IEEE 802.15 protocol, IEEE 802.11 protocol, IEEE 802.16 protocol, and/or ultra-wideband (UWB) protocol. If desired, the medical device data could be transmitted to the intermediary device using both a wired and wireless connection, such as to provide a redundant means of communication, for example.

Any amount of medical device data can be transmitted to the intermediary device in any manner. For example, data from the medical device can be transmitted to the intermediary device in real-time as it is measured, or medical device data can be stored (such as in a memory storage device) for a period of time before being transmitted to the intermediary device. In some cases, for example, it may be more efficient to transmit blocks of medical device data at once rather than initiating communication with an intermediary device each time data is available from the medical device. In other cases, the intermediary device may be out of range or otherwise unavailable to receive the medical device data. The medical device data can also be stored for any desired length of time, and/or until a particular event occurs. For example, the medical device data could be stored until it is verified that the intermediary device and/or the medical data server have received the data, allowing the data to be retransmitted if necessary. Data can also be deleted when a data record exceeds a predetermined storage time, and/or the oldest data record is deleted first after a predetermined storage size limit has been reached.

The medical device data can be transmitted to the intermediary device in any format. For example, the data from the medical device can be transmitted to the intermediary device exactly as it is transmitted from the medical device. This would be the case in embodiments of the present invention where the medical device itself is transmitting the data directly to the intermediary device. Alternatively, in embodiments of the present invention where the data is being received from the medical device and then retransmitted to the intermediary device, the medical device data can be refor-

matted, modified, combined with other data, or processed in any other suitable manner before being transmitted to the intermediary device. For example, the medical device data can be encrypted prior to transmission to the intermediary device, and this encryption may occur at any stage, for instance in the medical device itself or at a stage after being transmitted by the medical device. In cases where the medical device data is being combined with other data and transmitted to the intermediary device, all of the data may be encrypted or simply the medical device data itself. In an alternate embodiment, a digest of the medical data may be encrypted, to digitally "sign" the data contents to verify its authenticity. For example, but not by way of limitation, this digest may be produced by providing the received medical data to a hashing algorithm such as the MD5 or SHA-1 Secure Hashing Algorithm as specified in National Institute of Standards and Technology Federal Information Processing Standard Publication Number 180-1.

Asymmetric encryption algorithms and techniques are well known in the art. See, for example, *RSA & Public Key Cryptography*, by Richard A. Mollin, CRC Press, 2002, and U.S. Pat. No. 4,405,829, issued Sep. 20, 1983, the disclosures of which are fully incorporated by reference herein for all purposes. In an illustrative example, if two parties (for example, "Alice" and "Bob") wish to communicate securely using public key cryptography, each party begins by generating a unique key pair, where one of the keys is a private key that is kept in confidence by that party, and the other key is a public key that may be publicly distributed, published only to a message recipient, or made available through a public key infrastructure. The key generation step need be done by a party only once, provided that the party's private key does not become compromised or known by another party. If Alice wants to send a message confidentially to Bob, she may use Bob's public key to encrypt the message, and once sent, only Bob can decrypt and view the message using Bob's private key. But if Alice also wanted Bob to have assurance that the message was in fact coming from her, she could further encrypt the message with her private key before sending, then when Bob's private key and Alice's public key are used to decrypt the message, Bob knows for certain that he was the intended recipient and that Alice was the one who originated the message, and Alice knows that only Bob will be able to decrypt and read her message.

Asymmetric cryptography may be utilized to enhance security of certain implementations of the present invention. In an alternate embodiment, data transmitted by a medical device 250 is encrypted with a private key of the medical device user (or optionally with the private key of a health care provider that is operating the medical device), or with a public key of the intended recipient system such as the medical data server 270, or with both keys. The private and/or public keys may be delivered to the medical data interchange device 200 through a wired or wireless connection, allowing the medical data interchange device 200 to be configured for secure operation. In one embodiment, the system or medical data server 270 may request that the public key of the medical device be forwarded to enable decryption of any medical information encoded with the user's private key. In this manner, the data may be authenticated as coming from the actual patient that is desired to be monitored, and optionally, the patient may also be assured that only the intended recipient system or medical device server 270 is capable of decrypting and gaining access to the patient's medical device data.

In an alternate embodiment, encrypted or unencrypted data can be transmitted through an encrypted transmission protocol, such as the wireless encryption protocols (WEP, WPA

and WPA2) associated with the IEEE 802.11 wireless protocols or a Bluetooth encryption protocol associated with IEEE 802.15. Any number of other encryption methods can be used to encrypt the medical device data in conjunction with the present invention. The intermediary device may decrypt the medical device data, to allow processing of the data for example. Alternatively, to protect the data from unauthorized viewing, an intermediary device could simply retransmit the encrypted data to the medical data server.

Confirm Transmission of Data to Intermediary Device

The transmission of the medical device data can be confirmed (135) to verify the transmission was successful. The transmission can be confirmed in any suitable manner. For example, the intermediary device can transmit an acknowledgement once the transmission is received, otherwise the transmission can be rebroadcast.

Validate Data Transmitted to Intermediary Device

In the exemplary process shown in FIG. 1, the data transmitted to the intermediary device is validated (115). The data from the medical device can be validated in any suitable manner to achieve any result. For example, the data from the medical device may be validated to ensure it was transmitted properly and completely. The medical device data may also be validated to ensure it was provided from a specific medical device or particular type of medical device. The data may also be validated to ensure that fields in the data correspond to predetermined values and/or are within certain thresholds or tolerances. Any number, code, value or identifier can be used in conjunction with validating the medical device data. For example, the data can be validated by analyzing a medical device serial number, a medical device identifier, a patient identifier, one or more parity bits, a cyclic redundancy checking code, an error correction code, and/or any other suitable feature.

Store Data

The intermediary device may store the medical device data (145). The intermediary device may store the data in any suitable manner, such as by using a memory storage device. Any portion or amount of medical device data (or other forms of information) received or generated by the intermediary device may be stored for any length of time. The data may be stored for a predefined period of time and/or until an event occurs. For example, in one embodiment of the present invention the data is stored by the intermediary device until the data has been transmitted to the medical data server. In another embodiment, data is stored by the intermediary device until a predetermined data transmission record size has been reached, so as to reduce communication charges that may accrue during transmission. In yet another embodiment, the intermediary device stores the data until an acknowledgment from the medical data server is received, where the acknowledgment indicates that the stored data has been received by the medical data server. The medical data may be stored in any desired file format, as well as in an encrypted or decrypted state.

Format Message for Transmission to Medical Data Server

In the exemplary method according to an aspect of the present invention depicted in FIG. 1, a message is formatted for transmission to the medical data server. The message can originate from any entity operating in conjunction with the present invention. For example, the message may be created by the intermediary device, a device transmitting the medical device data to the intermediary device, or the medical device itself. The message can include some or all of the medical device data, as well as any other information useful to the medical data server. Multiple messages can be formatted to include any desired amount of medical device data. For

example, in the case of data from a glucose meter, multiple messages may be formatted to each include a single glucose reading, or a single message could be formatted to include the last ten glucose readings taken by the meter. The message can include any other desired data from any suitable source. For example, real-time data from a medical device may be included in a message along with previously-transmitted data from the stored by the intermediary device creating the message. The message (in whole or in part) may be encrypted to protect the contents of the message from unintended viewers and/or the privacy of the patient being monitored.

The message provides the medical device information to the medical data server in a format the medical data server can recognize and utilize. The message can thus be formatted to only include portions of the medical device data needed by the server and/or additional information about a patient, the medical device, and/or the treatment regimen. The message can be of any desired format. For example, the message can be included in a file having a tokenized format such as standard ASCII text format, or any other suitable standardized file format, such as an MS Word document, MS Excel file, Adobe PDF file, or binary picture file (JPEG, bitmap, etc.). The data within such a file can be ordered in any manner and have any suitable delimiters, notations, or other features. For example, a list of multiple glucose level readings in a text file message could be provided chronologically by when the readings were taken, with comma or tab delimiters to denote the start and end of each reading. The message may also have a unique and/or propriety format.

The format of the message can also be based on the method by which the message is transmitted to the medical data server. For example, where the message is transmitted to the medical data server using a wireless mobile telephone such as a cellular phone, the message can be formatted as an SMS text message. Similarly, the message may be formatted as an XML record, email, and/or facsimile. The message can include multiple formats and/or multiple messages may be formatted having different formats for transmission in a variety of methods or to a variety of recipient medical data servers.

Transmit Formatted Message to Medical Data Server

The message is transmitted to a medical data server (160) to allow the medical device data to be analyzed and processed. The message can be transmitted to a single medical data server, or to a plurality of medical data servers. The medical data server can be any suitable recipient of the medical device data. For example, the medical data server can be a computer system or other device as well as a human recipient (such as a doctor, nurse, or other healthcare provider). The message may be transmitted to the medical data server by any entity operating in conjunction with the present invention, and need not be the same entity that received the medical data or formatted the message. For example, the message may be transmitted to the medical data server by the intermediary device, any device transmitting or receiving the medical device data, or the medical device itself.

The message can be transmitted to the medical data server in any suitable manner. For example, the message can be transmitted to the medical data server through a wired connection, such as a telephone line, fiber optic cable, and/or coaxial cable. The message may also be transmitted wirelessly using any suitable wireless system, such as a wireless mobile telephony network, General Packet Radio Service (GPRS) network, wireless Local Area Network (WLAN), Global System for Mobile Communications (GSM) network, Enhanced Data rates for GSM Evolution (EDGE) network, Personal Communication Service (PCS) network, Advanced

Mobile Phone System (AMPS) network, Code Division Multiple Access (CDMA) network, Wideband CDMA (W-CDMA) network, Time Division-Synchronous CDMA (TD-SCDMA) network, Universal Mobile Telecommunications System (UMTS) network, Time Division Multiple Access (TDMA) network, and/or a satellite communication network. The message may be transmitted using any suitable combination of multiple wired and wireless communication methods. The transmission method selected to transmit the message to the medical data server can be chosen according to any desired criteria. For example, one or more transmission methods can be selected from a plurality of possible transmission methods to send the message based on each method's cost, time required to transmit, reliability, security, or any other suitable factor. Based on such criteria, the message may be stored until there is a suitable opportunity to transmit the message. For example, the message may be stored until an evening or weekend rate is available on a communications network.

Receive a Command from Medical Data Server

In addition to receiving the medical device data, the medical data server can transmit a command (160). The command can be received by the intermediary device, the medical device, and/or any other suitable recipient. Any number of commands of any type may be transmitted by the medical data server. The command can be transmitted using the same variety of wired and wireless methods discussed previously for the transmittal of the formatted message. The command need not be transmitted using the same communication method with which the formatted messages are transmitted to the medical data server.

In one embodiment of the present invention, for example, the medical data server issues a command to reconfigure a software application operating on the intermediary device. In another embodiment, the medical data server issues one or more commands to control the functionality of the medical device. In yet another embodiment, the medical data server issues one or more commands to request that a public encryption key corresponding to the patient using a medical device be forwarded to the medical data server, or that a device associated with the present invention receive a public encryption key corresponding to an intended recipient such as a particular health care service provider or other known destination such as the medical data server. In another embodiment, the medical data server issues one or more commands to cause the medical device to perform a warm reset, a cold restart, or to reset a password.

The commands need not be sent directly to a device they are intended to control. For example, a command could be transmitted to an intermediary device, which in turn retransmits it (unmodified) to the medical device to be controlled. Alternatively, the intermediary device could receive a command from the medical server, analyze the command, and then transmit an appropriately formatted command tailored to the specific medical device to be controlled. In this manner, the medical data server need not be able to generate a command for each and every specific device it wishes to control, rather, it can send a command appropriate to a class of devices (i.e. glucose meters) and the intermediary device will appropriately translate the command to control the medical device. The commands from the medical data server can initiate/run diagnostic programs, download data, request the patient's public encryption key, download the intended recipient's public encryption key, and perform any other suitable function on the intermediary device, medical device, or other devices operating in conjunction with systems and methods of the present invention.

In one embodiment, a user of a medical device may interact with the medical data server, and as a result of such interaction, cause a command to be created by the medical data server and transmitted to the medical device. Such a user may comprise, for example, the patient associated with the medical device or a health care provider that is caring for the patient. In various embodiments, the user may interact with a system that includes the medical data server through a computer interface (e.g. a web browser), a portable digital assistant (PDA), a mobile communication device (such as a cell phone), an emergency medical beacon, a medical data interchange device, an interactive voice response (IVR) function associated with the system, or other suitable interface. In one scenario, for example, the user calls the IVR function through a cellular network or PSTN connection, and in response to guided voice prompts, the user either gives vocal input, button-press inputs such as by DTMF tones, or a combination of methods. Based on the user's inputs to the system, whether by IVR or other means, the medical data server may respond by generating a command that is ultimately transmitted to the medical device or an intermediary device. In one implementation, the medical data server could generate and transmit a command that instructs the medical device to transmit data to the medical data server either directly or through an intermediate device. Such data may represent, for example, medical or historical information regarding a patient or the user of the medical device; medical device diagnostic information; or environmental parameters such as a battery charge level, a temperature, a barometric pressure, a code relating to an accessory for the medical device, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, or a quality of service (QoS) parameter. In one implementation, in response to user input or input associated with analysis of data uploaded to the medical data server, the medical data server causes a command to be transmitted to the medical device that instructs the device to take action that results in the administration of a prescribed dose of medication to the patient, or a prescribed shock to the patient's heart.

A command from a medical data server can be in any appropriate format and may include any suitable information. For example, a command may include data received from one medical device 250 to be delivered to another medical device 250 through the medical data interchange device 200. In this manner, a variety of medical devices can share data whether or not they are in communication with the medical data interchange device 200.

A command can also originate from an intermediary device 260. For example, a command to program or reconfigure one or more software programs on the medical data interchange device 200 depicted in FIGS. 2A, 2B, and 2C can be provided by an intermediary device 260 to the medical data interchange device 200 through the data relay transceiver 230. A command, as discussed above, may include multiple instructions, applets, or data elements to be processed, such as sections of executable code or interpretable scripts. Additionally, a user can program or configure a software program on any device operating in conjunction with the present invention through a suitable user interface, such as the user interface 290 of medical data interchange device 200.

In any system where commands can be sent remotely, security is always a concern, especially when a wireless implementation may provide an entry vector for an interloper to gain access to components, observe confidential patient data, and control health-sensitive components such as pacemakers and insulin pumps. In any digital data network, it is also possible that commands intended for one recipient may

be misrouted to a patient or health care provider that was not the intended recipient of the command. Embodiments of the present invention provide for enhanced security in a remote command system while still allowing flexibility and minimal obtrusiveness.

In one embodiment, a command received by any of the components in FIG. 2A, 2B, or 2C may be authenticated before the command is either acted upon by the destination component, or forwarded to another component in the system. Authentication may be directed to determining (1) whether the command came from a trusted or authorized source and (2) that the recipient is actually the intended recipient of the command. In one implementation, source command authentication is achieved by determining whether the origin of the command is a trusted component or server, and one way to accomplish this determination is analyzing whether a command is properly digitally signed by the originator or some other authentication information is provided that assures the recipient component that the message or command is authentic and the recipient component is actually the intended recipient. In an alternate implementation, destination command authentication is accommodated by examining the contents of the message or an authorization code to determine the intended recipient, or alternatively decrypting the command or a portion of the command to verify the intended recipient.

In one embodiment, when commands are created by a command originator, the originator provides for a means to verify the authenticity and/or validity of the command by at least one of the following methods: (1) encrypting the command with a private key of the command originator; (2) generating a digest of the command (through a method such as a hashing algorithm discussed above) and optionally encrypting the hashed digest with the command originator's private key, or (3) utilizing a symmetric encryption scheme providing an authentication code (such as a cryptographically hashed password) that is compared to previously stored values. Then, when a system component receives the command along with any encrypted or cleartext certification data, the component may determine the command is valid by (1) attempting to decrypt an encrypted command message with the alleged originator's public key, (2) attempting to decrypt an encrypted digest with the alleged originator's public key, and comparing the result to a hashed value of the command, or (3) comparing a cryptographically hashed password for the alleged originator to known pre-stored values, and if a match is found, authorization is granted. As an additional step, if the command were optionally encrypted using the intended patient/provider's public key, then only the recipient is capable of decrypting the command, ensuring that only the truly intended patient's health-care devices were being issued commands, and not an unintended third party. For example, in one embodiment, authenticating the command comprises decrypting at least part of the command using at least one of: a public key associated with the medical data server; a private key associated with a user of the medical device; and a private key associated with the medical device.

Authenticate User Access to Medical Data Server

In another embodiment, in regards to the methods described in regards to FIG. 1, it is desirable to ensure that a party attempting to interface with a system such as a medical data server is actually the party believed to be authorized to do so. Turning to FIG. 9, an embodiment is provided that illustrates a method to authenticate user access to the medical data server. A medical data system component 901 such as a medical data server (FIG. 2, 270) generates 910 a request to authenticate access, either on its own accord or as a result of

a message received by an alleged patient who is enrolled in the medical service provided by the medical data server. The medical data system **901** then sends a request to authenticate access to a user component **902** of the present invention associated with the client, user, or health care provider, and in one implementation, such component may include the medical data interchange device **200**. The user component **902** then receives **920** the request to authenticate access, and generates **930** an authentication token.

In various embodiments, authentication tokens may comprise either simple or complex text strings or data values indicating an account number or other patient identifier that can be matched against an internal patient database by the medical data server. Alternatively, authentication tokens may comprise encoded passwords or other indicia that assert that the entity for whom authentication is requested is genuine. Generation of an authentication token may be accomplished using alternative methods such as entry of a patient identifier, PIN, or password by a patient or healthcare provider after being prompted to do so. Alternatively, a biometric measurement of the patient or healthcare provider could be obtained and the measurement rendered into a digital representation. Once generated, for security purposes the authorization token may be secured **940** by encrypting the token, digesting and encrypting the digest of the token, or cryptographically hashing the token before transmission to the requesting entity such as the medical data system **901** or server. As discussed above in regards to the abovementioned command authentication, in one embodiment, when authentication tokens are created, the originating component of the token may create a certification of validity through at least one of the following methods: (1) encrypting the token with a private key associated with the token originator; (2) encrypting the token with a public key associated with the token requester or destination; (3) generating a digest of the token (through a method such as a hashing algorithm discussed above) and optionally encrypting the hashed digest with the token originator's private key, or (4) providing an authentication code as at least part of the token (such as a cryptographically hashed password) that may be compared to previously stored values. Then, when a medical data system component **901** receives the token along with any encrypted or cleartext certification data, the component may determine the access is valid by (1) attempting to decrypt an encrypted token with the alleged originator's public key; (2) attempting to decrypt an encrypted token with the alleged originator's public key; (3) attempting to decrypt an encrypted digest with the alleged originator's public key, and comparing the result to a hashed value of the token, pin, code, or password, or (4) comparing a cryptographically hashed password for the alleged originator to known pre-stored values, and if a match is found, authorization is granted.

The medical data system component **901** then receives **960** and analyzes **970** the validity of the authentication token as described above. If examination of the authentication token provides that the token is authentic, such as by comparing the analyzed token data to known, pre-stored values such as the patient or the patient's health care provider's pre-stored hashed password or other identity datum, then access is successful and the process terminates. After analyzing the authentication token or a message containing or associated with the token, the medical data system may determine that access is either permitted or denied, and may communicate **980** this status to the originator of the authentication token **902** who then receives notice of the failure **990**. At that point, the system may repeat the process **900**, allowing the token originator to attempt access again.

Exemplary Systems Using Wired Communication

Exemplary systems for use in conjunction with the present invention are depicted in FIGS. **2A**, **2B**, and **2C**. These systems may be used in conjunction with the method described in FIG. **1**, as well as with any subset or combination of the elements thereof. The systems shown in FIGS. **2A**, **2B**, and **2C** may also be used in conjunction with any other suitable embodiments of systems and methods for medical device monitoring according to an aspect of the present invention.

The exemplary system depicted in FIG. **2A** is a medical data interchange device **200** that includes a processor **210** coupled to a memory **220**. A data relay transceiver **230** wirelessly communicates with one or more intermediary devices **260** via antenna **232**, which in turn communicates with one or more medical device servers **270** through either a wired or wireless protocol. An external adapter module **240** communicates with one or more medical devices **250**. The adapter module **240** also communicates with a device interface **242**, as can any number of external devices, such as a computer system **280**. The device interface **242** may include any number of wired or wireless connections such as a universal serial bus (USB) connection, serial connection, parallel connection, Firewire connection (such as IEEE 1394), Ethernet connection, or any other suitable connection. Those of skill in the relevant arts also recognize that computer system **280** may also comprise external storage media such as a FLASH drive or a portable hard drive. The exemplary system shown in FIG. **2B** includes a modular adapter **240** removably attached to the medical data interchange device **200**. In one implementation of this embodiment, the device interface **242** is integrated with the adapter module **240**.

The medical data interchange device **200** may include any suitable power connection for powering the interchange device and/or for recharging an energy storage device such as a battery (not shown). The components of the medical data interchange device **200** may receive electrical power from any other type of power supply.

The device interface **242** may establish unidirectional or bidirectional communications with one or more of the medical devices **250** through the adapter **240**. The adapter **240** may be located internally or externally to the device interface **242** and/or medical data interchange device **200**. In FIG. **2A**, for example, the device interface **242** connects to an adapter **240** that is external to the medical interchange device **200**, while FIG. **2B** depicts the device interface **242** being integrated with the adapter **240**.

FIG. **2C** depicts an exemplary embodiment of the present invention wherein the medical data interchange device **200** is integrated with a medical device **250**. The medical data interchange device **200** can be integrated with the medical device **250** using any number of suitable wired connections (i.e.—soldered connections and/or traces on a printed circuit board) to allow the medical data interchange device **200** to communicate with components in the medical device **250**. As with the medical data interchange devices **200** depicted in FIGS. **2A** and **2B**, the medical data interchange device **200** depicted in FIG. **2C** can communicate with any number of intermediary devices **260** and/or medical data servers **270**.

The functionality of the medical data interchange device **200** can be implemented in any suitable manner, such as through the processor **210** executing software instructions stored in the memory **220**. Functionality may also be implemented through various hardware components storing machine-readable instructions, such as application-specific integrated circuits (ASICs), field-programmable gate arrays (FPGAs) and/or complex programmable logic devices (CPLDs). Systems for medical data interchange according to

an aspect of the present invention may operate in conjunction with any desired combination of software and/or hardware components.

Medical Data Interchange Device 200

Referring to FIGS. 3A and 3B, the medical data interchange device 200 depicted in FIGS. 2A and 2B is shown enclosed within a within a case 300. A case holding a system for medical data interchange according to aspects of the present invention may be of any size, shape and configuration. The system (and case enclosing it) is preferably small enough to be easily portable by a patient or person being monitored. For example, the exemplary case 300 depicted in FIGS. 3A and 3B is 3 inches long, 1 inch wide, and 0.5 inches deep. The top and bottom of the case 300 are 0.05 inches thick, while the sides of the case 300 are 0.075 inches thick. The case may be manufactured from any number of materials, such as plastic, metal, wood, composites, and/or any other suitable material. The case 300 shown in FIGS. 3A and 3B, for example, is manufactured from hard plastic.

The case 300 includes a power connection 320 for powering the interchange device 200 and/or for recharging an energy storage device such as a battery. The case 300 also includes an interface module 310 with four separate ports to accommodate different wired connections to the adapter 240, including a serial port interface (SPI) port 330, an infrared input 340, a mini-jack port 350 (i.e.—a 3.5 mm TRS connector), and a super mini-jack port 360 (i.e.—a 2.5 mm TRS connector). The interface module 310 may include any number and type of wired connection ports.

The interface module 310 may include any suitable portion of the medical data interchange device 200. In one embodiment, referring to FIG. 2B, the interface module 310 is an adapter module 240 that includes the device interface 242. The plurality of wired connection ports (330, 340, 350, and 360) are coupled to the adapter 240, which in turn communicates data to the rest of the medical data interchange device 200 through the device interface 242. In this embodiment, the interface module 310 is removably attached to the case 300 to allow different modules 310 to be interchangeably connected to the case 300 to communicate with different medical devices 250.

In another exemplary embodiment, referring again to FIG. 2A, the interface module 310 contains the device interface 242 that couples to an external adapter 240. In this embodiment, the adapter 240 includes one or more connections to one or more medical devices 250. The connections to the medical devices 250 can be through a common wired connection 252, such as a PCI bus, ISA bus, PCI-E bus, SPI, USB, or other common connection. The connections to the medical devices 250 may also be made through individual wired connections to each medical device 254. The adapter 240 can communicate with any number of medical devices 250 through any combination of common wired connections 252 and individual wired connections 254.

In the exemplary embodiment depicted in FIG. 2A, the adapter 240 also connects to the device interface 242, through one or more wired connections 256. The wired connection 256 between the adapter 240 and the device interface 242 can be a single shared wired connection that communicates data to and from every medical device 250 connected to the adapter 240. The adapter 240 can also communicate with the device interface 242 through a plurality of wired connections 256, wherein each wired connection 256 is dedicated to communicating with a separate medical device 250. The adapter 240 can also communicate with the device interface 242 through any combination of dedicated or shared connections.

The adapter module 310 may be removably attached to the rest of the case 300 to allow different modules with different types of wired connection ports to be interchangeably used, as depicted in FIG. 2B. The adapter module 310 may include any of the elements of the medical data interchange device 200, as well as any other desired systems and devices.

In another exemplary embodiment of the present invention, referring now to FIGS. 3C and 3D, a case 370 includes a removable adapter module 380 that includes a medical device connector 385 for communicating with a medical device through a wired connection. The adapter module 380 connects to the case 370 using plug 387. The plug 387 attaches to a corresponding port on the case 370 (not shown) to hold the adapter module 380 in place and allow the communication of data through the adapter module 380. The connector 385 and plug 387 can use any desired wired connection, and need not use the same type of wired connection. In one embodiment, for example, referring to FIG. 3E, a case 395 includes a 2.5 mm or 3.5 mm stereo plug connector 397 connected to a USB jack on the side of the case 395 (not shown). In this embodiment, the adapter module 380 is implemented in a component 398 that electrically couples the stereo plug connector 397 and USB jack. The component 398 includes circuitry (such as that depicted in FIGS. 6 and 7) to convert and/or redirect the signals from the stereo plug 397 to the USB jack and vice versa.

The adapter module 380 connects to the case 370 using plug 387. The plug 387 attaches to a corresponding port on the case 370 (not shown) to hold the adapter module 380 in place and allow the communication of data through the adapter module 380. The connector 385 and plug 387 can use any desired wired connection, and need not use the same type of wired connection. In the present embodiment, for example, the connector 385 is a 2.5 mm or 3.5 mm stereo jack while plug 387 is a USB plug.

The case can include any other suitable features. For example, the case may include a screen, lights, LEDs, keys, and speaker and microphone grilles to support features of a user interface included in a system for medical data interchange. The exemplary systems for medical data interchange shown in FIGS. 2A, 2B, 3A, 3B, 3C, 3D, and 3E are all configured to fit in a container along with the medical device it communicates with to allow a user to easily transport the medical device and the data interchange device together. In the exemplary system for medical data interchange depicted in FIG. 2C, the medical data interchange device 200 is integrated within the case or packaging of the medical device 250 itself.

Other embodiments of systems for medical data interchange according to aspects of the present invention can be configured to be in small enough to be coupled with or integrated into a medical device 250 or an intermediary device 260. For example, a medical device 250 may be manufactured to include a medical data interchange device 200 within the packaging or housing of the medical device 250. Similarly, a medical data interchange device 200 can be integrated as part of an intermediary device 260 such as a cellular phone, PDA, or other mobile computing device. The intermediary device 260 could thus be configured to both receive data from a medical device 250 through a wired connection, as well as transmit messages regarding the medical device 250 and/or patient to a medical data server 270.

Alternatively, a medical data interchange device 200 can be configured to be physically attached to a medical device 250 or intermediary device 260. For example, where an intermediary device 260 such as a mobile wireless telephone or PDA is used in conjunction with embodiments of the present inven-

tion, one exemplary embodiment of a medical data interchange device **200** and its case **300** is configured to match the size and shape of the intermediary device **260** and attach to the back of the intermediary device **260** using metal or plastic clips that wrap around the face and/or sides of the intermediary device **260**. When attached, the medical data interchange device **200** conforms to the size and shape of the outline of the intermediary device **260**, and is preferably shaped to conform to the dimensions of the back of the intermediary device **260** to avoid unnecessarily impacting the original size of the intermediary device **260**. In this embodiment, the case of the medical data interchange device **200** may also include other desirable features, such as a belt clip to allow the data interchange device/intermediary device combination to be worn by a user.

Turning to FIG. 4, in another exemplary embodiment of the present invention, the medical data interchange device **200** is contained in a flexible, protective container **400** that opens to allow a medical device **250** to be likewise contained therein. The container **400** could also be configured to hold an intermediary device **260** (such as a cellular phone, PDA, or other mobile computing device) to allow a medical data interchange device **200** to be used with a variety of intermediary devices **260**, which may (in some cases) provide a more cost effective approach to integrate the medical data interchange device **200** with an intermediary device **260** or medical device **250**. The medical data interchange device **200** can also be integrated within the protective container **400** itself, with the container **400** acting as the case for the data interchange device **200**.

Alternatively, as depicted in FIG. 4, the medical data interchange device **200** may simply be contained within a pouch **410** or other structure within the container **400**. The exemplary container **400** depicted in FIG. 4 also includes a holder **420** for the medical device **250** formed from clear plastic to allow a user to read a display **422** and/or operate keys **424** on the medical device **250**. The protective container **400** can also be sized to comfortably fit and protect any other desired item, such as a day planner, wallet, notepad, and/or writing utensil or PDA stylus. The protective container **400** can be made from any combination of desired materials, such as leather, plastic, nylon, cordura, or other flexible material. The protective container **400** can be sealed in any manner, such as by using snaps, hook-and-loop closures, buttons, and/or a zipper. The exemplary container **400** depicted in FIG. 4, for example, is sealed using a zipper **430**. The container **400** can be waterproof, heat resistant, and/or include padding to protect the medical data interchange device and other contents from the shock of a fall. The container **400** may include any number of pockets, pouches, or other sub-containers inside or outside the case to hold accessories associated with the medical device **250**, intermediary device **260**, or other item(s) stored within the container **400**.

The exemplary protective container **400** depicted in FIG. 4 is configured to hold a medical device **250** (specifically, a glucose meter) and a medical data interchange device **200** according to an aspect of the present invention. In this exemplary embodiment, the protective container **400** is closed using a zipper **430** that runs along the exterior of the sides of the container **400**. A user unzips the two halves of the container **400** and opens the container **400** to display the glucose meter contained in the holder **420** attached to the interior of one half of the container **400**, while the medical data interchange device **200** is contained in a pouch **410** attached to the interior of the other half of the container **400**. The pouch **410** is formed from a nylon mesh material to allow a user to see and/or interact with user interface features of the medical data

interchange device **200**. The pouch **410** is sealed with a zipper **412**. The container **400** includes a flexible elastic strap **440** to hold a container of blood sugar metering strips **442**. The container **400** may include any number of other pouches or containers on the interior or exterior of the container for storing batteries and/or power cables for the glucose meter and/or medical data interchange device, and other items of use to the patient carrying the container, such as bottles of insulin and needles for use by the patient depending on the outcome of a reading by the glucose meter.

Processor **210**

The processor **210** retrieves and executes instructions stored in the memory **220** to control the operation of the medical data interchange device **200**. Any number and type of processor(s) such as an integrated circuit microprocessor, microcontroller, and/or digital signal processor (DSP), can be used in conjunction with the present invention. Referring now to FIG. 5A, an exemplary medical data interchange device **200** according to an aspect of the present invention is implemented using a microcontroller **501**. In the exemplary system depicted in FIG. 5A, the microcontroller **501** includes a Universal Asynchronous Receiver/Transmitter (UART) and Universal Serial Bus (USB). The microcontroller **520** depicted in FIG. 5B also includes these features, along with a digital signal processor (DSP) for communication with a cellular RF Transceiver **530** as will be discussed in more detail below. The microcontrollers **501**, **520** depicted in FIGS. 5A and 5B, respectively can include any other suitable components and features, such as comparators (**504**), analog-to-digital converters (ADCs) (**517**), and/or digital-to-analog converters (DACs) (**512**), though these components have been shown outside the microcontrollers **501**, **520** for clarity.

Memory **220**

The exemplary systems depicted in FIGS. 2A and 2B include a memory **220**. The memory **220** stores instructions, medical device data, messages transmitted to or received from the medical data server **270**, and any other suitable information. A memory **220** operating in conjunction with the present invention may include any combination of different memory storage devices, such as hard drives, random access memory (RAM), read only memory (ROM), FLASH memory, or any other type of volatile and/or nonvolatile memory.

In the exemplary embodiments depicted in FIGS. 5A and 5B, the microcontroller **501** and **520** each include an on-chip memory. In addition, the microcontroller **501**, **520** is coupled to a flash memory **510**. The flash memory **510** may be of any size to achieve any desired purpose. In this exemplary embodiment, the size of flash memory **510** is selected to adequately store pre-recorded voice recordings to be played through the speaker **515**, discussed below. Any number of memory storage devices of any size and configuration may also be used in conjunction with the present invention.

Power Source

Any number, combination, and type of suitable power sources can be utilized in accordance with aspects of the present invention. The exemplary systems depicted in FIGS. 5A and 5B are powered by a pair of replaceable alkaline AAA 1.5 volt batteries **505**. The positive lead of the series-coupled battery pair **505** is connected to ADC **517** to enable the microcontroller **501**, **520** to monitor the voltage level of the batteries **505**. Any number of other suitable batteries may also be used according to any desired criteria. For example, a rechargeable battery or batteries integrated with the data interchange device may be selected to reduce the overall size of the medical data interchange device **200** and/or provide for the convenience of a user who would not need to replace

batteries. Such rechargeable batteries can be charged through the USB connector **502**, as well as through a dedicated power connector. Any battery of any suitable type and size may be used. Replaceable batteries may be selected to reduce the price of the medical data interchange device. The power supply circuitry shown in FIGS. **5A** and **5B** is exemplary only, and may be implemented by using other conventional power supply approaches. The medical data interchange device **200** and other systems for medical data interchange according to various aspects of the present invention can utilize any appropriate power supply devices, components, circuits, and systems.

In the exemplary circuits shown in FIGS. **5A** and **5B**, voltage from the batteries **505** is supplied to two DC to DC converters **506**, **507** which supply an appropriate voltage level to the various components of the medical data interchange device **200**. DC converter **506** steps up the voltage to 5 volts, while DC converter **507** steps up the voltage to 3.3 volts. Any number of voltage converters or similar components may be used as desired to supply appropriate voltage levels to components of the medical data interchange device **200**.

Data Relay Transceiver **230**

The data relay transceiver **230** communicates with one or more intermediary devices **260**, medical data servers **270**, or other suitable systems. Any suitable communications device, component, system, and method may be used in conjunction with the present invention. In the exemplary circuits shown in FIGS. **5A** and **5B**, the data relay transceiver **230** comprises a Bluetooth transceiver **509** that is in bidirectional communication with microcontroller **501**, **520** through multiplexer **508**. The multiplexer **508** allows the microcontroller **501**, **520** to alternately communicate with the USB port **502** and the Bluetooth transceiver **509** through a single UART on the microcontroller **501**, **520**.

The medical data interchange device **200** may include, or operate in conjunction with, any number of data relay transceivers **230**. In FIG. **5B**, for example the exemplary medical data interchange device **200** further includes a cellular radio frequency (RF) transceiver **530** in communication with microcontroller **520**. In this exemplary embodiment, the microcontroller **520** is a cellular baseband processor that includes a digital signal processor (DSP) which communicates data through a cellular RF power amplifier and front end **540** connected to a cellular antenna **545**. Data is transmitted by the microcontroller **520** on the CELL TX INTRF line and received by the microcontroller on the CELL RX INTRF line. Additionally, the microcontroller **520** can control various features of the RF transceiver **530** via the CELL CONTROL line. The RF power amplifier and front end **540** performs the necessary functions to transmit and receive cellular signals, such as power amplification, power detection, filtering, and input/output matching.

The medical data interchange device **200** depicted in FIG. **5B** may be configured to communicate using any number and type of cellular protocols, such as General Packet Radio Service (GPRS), Global System for Mobile Communications (GSM), Enhanced Data rates for GSM Evolution (EDGE), Personal Communication Service (PCS), Advanced Mobile Phone System (AMPS), Code Division Multiple Access (CDMA), Wideband CDMA (W-CDMA), Time Division-Synchronous CDMA (TD-SCDMA), Universal Mobile Telecommunications System (UMTS), and/or Time Division Multiple Access (TDMA). A medical data interchange device **200** operating in conjunction with the present invention may alternatively (or additionally) include data relay transceiver **230** components to communicate using any other method of wired or wireless communication.

As discussed previously, the medical data interchange device **200** can transmit any data to any entity operating in conjunction with the present invention. For example, the medical data interchange devices **200** depicted in FIGS. **5A** and **5B** may transmit medical data to one or more intermediary devices **260**, as well as to one or more medical data servers **270**.

Adapter Module **240**

Referring again to FIG. **2A**, the exemplary medical data interchange device **200** includes an adapter module **240** for communicating with one or more medical devices **250** as well as other suitable systems. The adapter module **240** can be configured to communicate with any suitable class, type, and/or manufacturer of medical device **250**. The adapter module **240** depicted in FIG. **2A** is an external component that communicates with a device interface **242** in the medical data interchange device **200**. In the exemplary circuits depicted in FIGS. **5A** and **5B**, the USB port **502** is configured to interface with a standard USB connection, as well as with the adapter interfaces **601** and **701** (shown on FIGS. **6** and **7**, respectively) which utilize USB connectors, but not the USB communications protocol. Instead, the adapters depicted in FIGS. **6** and **7** implement a customized protocol tailored to communicating with medical devices **250** through ring/tip connectors **605** and **705**. The microcontroller **501**, **520** is configured to detect and utilize the same communications protocol as an adapter module **240** connected to port **502**.

In accordance with various aspects of the present invention, the adapter module **240** can also be modular and removably attached to the body of the data interchange device **200**, integrated as part of the data interchange device **200**, or a combination of the two. In the exemplary embodiment of the present invention depicted in FIG. **2B**, an adapter module **240** is removably attached to the body of the medical data interchange device **200** and includes the device interface **242** to allow different medical devices **250** to interoperate with the data interchange device **200**. As new medical devices **250** and/or new wired connections are utilized, a modular adapter module **240** configured to communicate with the new device or new frequency can be added to the existing system.

Software running on or operating in conjunction with the adapter module **240** can be configured/updated through the device interface **242**, auxiliary communication system **244**, the user interface **290**, or in response to a communication from an intermediary device **260** or medical data server **270** received through the data relay transceiver **230**. This allows the functionality of the medical data interchange device **200** to be dynamically updated and avoids the expense of having to create custom hardware implementations for every type of medical device to be monitored.

FIG. **6** depicts a circuit diagram of an adapter module **240** that interfaces with the data interchange device **200** through a USB connector **601**. As stated previously, the adapter **240** adjusts the voltage levels of Tx and Rx in order to communicate with a medical device **250** connected to TRS connector **605**. An adapter **240** operating in conjunction with the present invention may use any combination of wired connections and communication protocols.

The adapter module **240** depicted in FIG. **6** is configured to interface with a medical device **250** that sends a wakeup signal. In operation, a signal received from the medical device **250** on the Rx line is provided to the USB connector **601** through a buffer **602** that provides isolation between the medical device **250** and the circuitry of the medical data interchange device **200** depicted in FIGS. **5A** and **5B**. The Rx signal is also provided to switch **607** which places a voltage on the AID pin of the USB connector **601**. Referring back to

FIGS. 5A and 5B, the voltage from the AID pin on connector 601 is provided to the comparator 504 through the ID pin on the USB port 502. The comparator 504 then activates the microcontroller 501, 520 in response. The level of voltage provided on the AID pin can also be used to identify the type of meter and/or adapter connected to the medical data interchange device 200 to the microcontroller 501, 520.

Referring again to FIG. 6, the Tx lead from the USB connector 601 is driven logically high when the UART on the microcontroller 501 is idle. The Tx signal from the USB connector 601 is inverted by inverter 603. When the UART on the microcontroller is idle, the inverter 603 drives the signal low, turning transistor 604 off and allowing the Tx signal to the tip of connector 605 to float at the voltage level from the medical device 250. Alternatively, when the UART on the microcontroller 501 is active, the Tx signal from the USB connector 601 is logically low and the inverter 603 inverts the low signal high to activate transistor 604 and allow the Tx signal from connector 601 to drive the Tx line on the TRS connector 605 to the medical device 250.

FIG. 7 depicts a circuit diagram for another adapter 240 according to various aspects of the present invention. In this exemplary embodiment, USB connector 701 interfaces with USB port 502 shown in FIGS. 5A and 5B. Inverter 702 inverts the logic level of the Tx signal provided by the microcontroller 501 through the USB connector 701 to correspond to the voltage levels used by a medical device 250 connected to TRS connector 705. The Rx signal from a medical device 250 connected to the TRS connector 705 is provided to an N-channel JFET 704. In this exemplary circuit, when the Rx signal from the medical device 250 is marking (a -5.5 volt signal indicative of a logical "1") the JFET 704 is turned off, causing a 5-volt signal to be provided through buffer 703 and to the Rx lead of the UART on the microcontroller 501. Alternatively, when the Rx signal from the medical device 250 is spacing (a 6-volt signal indicative of a logical "0") the JFET 704 is turned on, causing ground to be provided through buffer 703 and to the Rx lead of the UART on the microcontroller 501, 520. The present invention can be configured to operate in conjunction with any other combination of voltages between the microcontroller 501, 520 and the TRS connector 705.

Device Interface 242

The device interface 242 communicates with one or more medical devices 250. The device interface 242 can also communicate with any other system, device or entity. The device interface 242 may include any number and combination of hardware and/or software components. The device interface 242 can communicate with medical devices through an adapter 240, as shown in FIG. 2A. In this exemplary embodiment, the device interface 242 connects to an external adapter 240 configured to couple with one or more medical devices 250. In this way, adapters 240 that allow connections to different medical devices can be used interchangeably with the same medical data interchange device 200. In another exemplary embodiment, referring to FIG. 2B, the device interface 242 is integrated with the adapter 240.

Any number of adapter modules 240 may be used in conjunction with the present invention, for example to communicate with multiple medical devices 250 using different wired connections and/or communication protocols. The present invention may be used in conjunction with any wired connection and communication protocol to communicate with one or more medical devices. For example, the medical data interchange device 200 may be configured to communicate with one or more medical devices using, without limitation: tip and sleeve (TS), tip, ring, and sleeve (TRS), and tip,

ring, ring, and sleeve (TRRS) connections; serial peripheral interface bus (SPI) connections; universal serial bus (USB) connections; RS-232 serial connections, Ethernet connections, optical fiber connections, and Firewire connections.

In the exemplary embodiments depicted in FIGS. 2A and 2B, the device interface 242 and/or adapter 240 can be configured (e.g. through a software program residing in memory 220 and executed by processor 210) to detect and switch to different communication protocols and/or different wired connections to one or more medical devices 250 or other devices (such as the computer system 280), thus providing interoperability between types and manufacturers of a wide variety of devices. The auxiliary communication system 244 depicted in FIG. 2B may similarly be configured.

The medical data interchange device 200 can be configured to automatically request data from one or more medical devices 250 at predetermined times using the device interface 242. Any appropriate date or time setting may be used. The data interchange device 200, medical device 250, or any other device operating in conjunction with the present invention can be configured to automatically request and/or transmit data in any suitable manner. For example, the medical data interchange devices 200 depicted in FIGS. 2A and 2B can be configured through the device interface 242, the user interface 290, and/or from a command issued transmitted by an intermediary device 260 through the data relay transceiver 230. Additionally the medical data interchange device depicted in FIG. 2B can be configured through the auxiliary communication system 244. In the case of a command received through the data relay transceiver 230, the command can be generated by any suitable entity, such as from a medical data server 260 or a user of the intermediary device.

The automatic requesting/transmission of data by a device operating in conjunction with the present invention may be subject to any suitable conditions or rules that dictate whether the data is in fact requested/transmitted. For example, a medical data interchange device 200 programmed to request data from a medical device 250 at a set time may first check to verify that the medical device is within range, that the translator 200 has sufficient battery reserves to send the request and receive the data, whether the translator 200 has sufficient space in the memory 220 to store the data, and/or whether any other suitable condition is met.

Auxiliary Communication System 244

The medical data interchange device 200 depicted in FIG. 2B includes an auxiliary communication system 244 for communicating with additional systems and devices. For example, the auxiliary communication system 244 may be used to communicate with an external personal computer system 280 to upload software to the data interchange device 200, store data, provide or update encryption keys, perform diagnostics, and other appropriate purposes. The auxiliary communication system 244 can be a separate device, system, and/or component, or may be integrated with another component, such as the device interface 242. For example, in one embodiment of the present invention, the device interface 242 includes a USB port for communicating with any device capable of communicating through a USB connection. This allows the medical data interchange device 200 to communicate instructions, software upgrades, medical data, and other information with computing devices, memory storage devices (such as portable USB memory drives), as well as medical devices. The same device interface 242 can thus be used to receive medical data from a medical device 250 as well as to download reports that include the medical data. In one embodiment, medical data received by the medical data interchange device 200 may be formatted by the processor

210 into a ubiquitous data format such as Portable Document Format (PDF), and subsequently transferred to an external device such as a computer system **280** through the auxiliary communication system **244**.

The medical data interchange device **200** or other system operating in conjunction with the present invention can include any suitable circuit, component, device, and system for communicating with any other device. The auxiliary communication system **244** can be used to transfer data to and from the medical data interchange device **200**, as well as for an external computer system **280** to configure or program software and hardware in the data interchange device **200**. In one embodiment of the present invention, for example, a user operating computer system **280** connected to medical data interchange device **200** through the Internet can configure settings for the device interface **242**, adapter **240**, data relay transceiver **230**, and user interface **290**. The computer system **280** can also download data received by the data interchange device **200** from one or more medical devices **250**. Additionally, the computer system **280** may communicate with the medical devices **250** real-time through the medical device transceiver **240**, such as to monitor or control one or more medical devices **250** in real-time.

User Interface **290**

The medical device **250**, medical data interchange device **200**, intermediary device **260**, or other device operating in conjunction with the present invention may include a user interface. Referring to FIGS. **2A** and **2B**, an exemplary user interface **290** of a medical data interchange device **200** in accordance with aspects of the present invention includes an input device **292** and an output device **294**. The input device **292** receives commands, data, and other suitable input from a user. The output device **294** provides the user with data, alerts, and other suitable information from the medical data interchange device **200**.

Any number of input devices may be included in a user interface for one or more devices in the present invention. In one embodiment of the present invention, for example, the user interface **290** includes a touch pad, a touch screen, or an alphanumeric keypad to allow a user to enter instructions and data into the medical data interchange device **200**. One or more buttons on the keypad or touch screen can be programmed or configured to perform specific functions, such as to request data from one or more medical devices. The user interface **290** can also include one or more multifunction switches, keys, or buttons that each allows a user to perform multiple functions.

The user interface may also include a microphone to allow the user to provide such information to the medical data interchange device **200** verbally. In this exemplary embodiment, the medical data interchange device **200** also includes speech recognition software to process verbal input through the user interface **290**. The ability of the medical data interchange device to recognize speech from a patient can be particularly useful for users/patients who have vision problems, arthritis, or other impairments that would inhibit them from using a keypad or other input device. A microphone can be used in conjunction with audible (e.g. through sound waves perceivable by the human ear) data provided through a speaker, as discussed below, to allow a user to interact with any device operating in conjunction with the present invention in a completely auditory manner. In one nonlimiting example, audible input could also be sensed and analyzed by the medical data interchange device **200** that a patient has uttered a command, such as the command to turn on. Bidirectional audible communication, in addition to aiding impaired patients, allows users to operate devices in the

present invention in a hands-free manner which can increase the speed, ease, and efficiency in which a device (such as the medical data interchange device **200**) can be utilized.

Devices operating in conjunction with the present invention may include any number of suitable output devices. Referring to the exemplary medical data interchange device circuits depicted in FIGS. **5A** and **5B**, a user interface **290** including two lights **511** (LED1 and LED2) may be used to indicate the status of the medical data interchange device **200** to the user, as well as other pertinent information. For example, a flashing LED can be used to indicate when data from a medical device is in the process of being transferred, while a solid LED can indicate the transfer of data is complete. The medical data interchange devices **200** depicted in FIGS. **5A** and **5B** also provide auditory output through speaker **515**. The microcontroller **501**, **520** retrieves audio samples, such as recorded speech, from the EEPROM **510** and provides output to DAC **512**, which converts the digital signal from the microcontroller **501**, **520** to an analog signal that can be output on the speaker **515**. The analog signal is provided to an audio amplifier **514** that amplifies the signal. The gain of the amplifier **514** is set by the ratio of resistors **516** and **513**.

Any other suitable user interface features may similarly be included in devices and systems operating in accordance with the present invention. In another exemplary embodiment, for example, the output device **294** includes a display screen to visually display information as well as a speaker (e.g. speaker **515** shown in FIGS. **5A** and **5B**) to provide auditory output. The output device **294** can include multiple transducers such as audio speakers or piezoelectric elements, amplifiers, and other appropriate devices and systems to provide the auditory output. The medical data interchange device **200** may be configured to provide words, phrases, tones, recorded music, or any other type of auditory output to a user.

Any type of information may be communicated through the user interface **290**, such as the biological, biometric, or behavioral information for one or more patients. The user interface can provide/receive any other suitable information, such as environmental information and/or diagnostic data for a medical device, a battery charge level, a temperature, a barometric pressure, a code relating to an accessory for the medical device, a biometric access measurement, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, and a quality of service (QoS), and combinations thereof.

Information provided or received by the user interface **290** may be in any appropriate format. For example, a user interface that communicates information to a user in an auditory format may first provide a data header followed by a data value to identify the data to the user. Similarly, an output device **294** providing information to a user visually may provide a series of measurements in the form of a spreadsheet with headers indicating the source of the measurements. The output device **294** can also provide information in any number of desired languages, regardless of whether the information is provided audibly or visually.

Various features of the user interface can be implemented in hardware, software, or a combination of the two. In the medical data interchange devices **200** depicted in FIGS. **2A** and **2B**, for example, the user interface **290** includes voice interface software stored in the memory **220**, including tables of recorded words and phrases. When executed by the processor **210**, the voice interface software plays the appropriate recorded words and phrases (such as enunciating the medical data) through a speaker such as one included in the output

device **294** to provide information to the user. The voice interface software, like any software operating on the medical data interchange device **200**, can be downloaded and configured through the auxiliary communication system **244** or device interface **242**. As discussed previously, any software program on any device operating in accordance with the present invention can be programmed or configured through any other suitable interface. In the medical data interchange device **200**, for example, the voice interface software could also be downloaded and configured through the data relay transceiver **230** in response from a command from a medical data server **270** and/or intermediary device **260**, as well as from input from the user through the user interface **290**. Accordingly, the voice interface software can be configured to include words and phrases in any number of different languages, and can be updated with new words and phrases as desired, such as to accommodate a new medical device **250** operating with the medical data interchange device **200**. Non-verbal sounds, such as melodies and tones, can also be stored and used by the user interface **294** to provide alerts, indicators, and other information to the user.

The user interface can also provide/receive information to a user in a machine-readable format. In one exemplary embodiment of the present invention, for example, the user interface **290** of a medical data interchange device **200** includes a fixed or retractable USB port to communicate with a thumb drive, memory stick, portable hard drive, an external computer system, or other USB-compatible device. This allows doctors and other healthcare providers to directly access the medical data interchange device **200** directly, without having to retrieve the data from a medical data server. In this exemplary embodiment, the medical data interchange device **200** can be configured to send, receive, and process machine-readable data can in any standard format (such as a MS Word document, Adobe PDF file, ASCII text file, JPEG, or other standard format) as well as any proprietary format. Machine-readable data to or from the user interface may also be encrypted to protect the data from unintended recipients and/or improper use. In an alternate embodiment, a user must enter a passcode to enable use of the USB port, and optionally, after a period of time of non-use, the USB port is automatically disabled. Any other user interface feature may be utilized to allow a human or non-human user to interact with one or more devices operating in conjunction with the present invention.

Power Saving Features

A medical data interchange device, intermediary device, medical device, or other system operating in accordance with aspects of the present invention may include any other suitable features, components, and/or systems. For example, the data interchange device **200** or other device may be configured to preserve the life of its battery by shutting off or going into a low-power mode when it, and/or the medical device it monitors, experiences a predetermined period of non-use, or a change in a measured parameter such as indication that a case holding the translator **200** has been actuated to a closed position. Such devices can also be configured to become active in response to any suitable event, such as receiving a signal from a device (such as a sensor).

In one non-limiting embodiment of the present invention, referring now to FIG. **8**, a medical data interchange device **200** communicates with a motion sensor **810** and a light sensor **820** to determine when a container **830** holding the data interchange device **200** and the medical device **250** it monitors is open or closed. In this exemplary embodiment, the data interchange device **200** can preserve the life of its battery by shutting off or going into a low-power mode when

the container **830** is closed and, therefore, the medical device **250** held in the container **830**, is not in use. Any type of motion sensor can be used in accordance with the present invention, such as an accelerometer, tilt switch, or other device that generates a signal in response to movement. Similarly, any type of light sensor may be used in conjunction with the present invention. The light sensor can be used to detect the amount of light entering a container **830** holding the medical device, medical data interchange device, or other device to activate the device when the sensed amount of light exceeds a predetermined threshold, or if an increase in the amount of incident light exceeds a predetermined threshold. In an alternate embodiment, a microphone may receive audible signals that are analyzed by the medical data interchange device **200** to indicate a command has been uttered that indicates that the medical data interchange device **200** should be shut down or activated from a quiescent or low-power state.

A sensor may be integrated into the medical data interchange device **200**, or operate externally to the data interchange device **200**, communicating with the data interchange device **200** wirelessly or through a wired connection. For example, in the exemplary embodiment depicted in FIG. **8**, the motion sensor **810** and light sensor **820** are integrated into the interior of the container **830** and communicate with a medical data interchange device **200** contained within to indicate when the container **830** is actuated from a closed position to an open position.

Security Measures

Systems and devices operating in accordance with aspects of the present invention may implement one or more security measures to protect data, restrict access, or provide any other desired security feature. For example, any device operating in conjunction with the present invention may encrypt transmitted data and/or protect data stored within the device itself. Such security measures may be implemented using hardware, software, or a combination thereof. Any method of data encryption or protection may be utilized in conjunction with the present invention, such as public/private keyed encryption systems, data scrambling methods, hardware and software firewalls, tamper-resistant or tamper-responsive memory storage devices or any other method or technique for protecting data. Similarly, passwords, biometrics, access cards or other hardware, or any other system, device, and/or method may be employed to restrict access to any device operating in conjunction with the present invention.

Exemplary Method Using Wireless Communication

An exemplary method according to an aspect of the present invention is depicted in FIG. **10**. In this method, an identifier is requested from a medical device (**1105**), and data from the medical device is received (**1110**) and validated (**1115**). An intermediary device such as a mobile phone or personal digital assistant is authenticated (**1120**) and activated (**1125**). The data is transmitted by the medical device to the intermediary device (**1130**) and the transmission to the intermediary device is confirmed (**1135**). The data is stored (**1140**) in the intermediary device. A message is formatted (**1145**) and transmitted to a medical data server (**1150**). Optionally, a command can be received from the medical data server (**1155**) and optionally relayed from the intermediary device. Any combination and/or subset of the elements of the method depicted in FIG. **10** may be practiced in any suitable order and in conjunction with any system, device, and/or process. The method shown in FIG. **10** can be implemented in any suitable manner, such as through software operating on one or more computer systems. Exemplary systems for performing elements of the method shown in FIG. **10** are discussed later in this description.

Request Medical Device Id

In the exemplary process according to aspects of the present invention depicted in FIG. 10, an identifier is requested from a medical device providing the data to be monitored (1105). Any suitable identifier may be provided, such as the serial number of the medical device or a numeric, alphabetic, alphanumeric, or other identifier. The medical device identifier can be used to determine whether the correct medical device is being monitored. The medical device identifier can also be used to determine the manufacturer, model, type, characteristics, or other information pertinent to the medical device and/or the patient(s) it monitors. The medical device identifier may be received passively, such as from a medical device that automatically includes its identifier as part of its telemetry broadcast. Alternatively, the medical device can be polled to request the medical device identifier. The medical device identifier need not be requested from the medical device each time the medical device is being monitored. For example, the medical device identifier may be stored in a storage medium for future reference.

Receive Data Wirelessly from a Medical Device

In the exemplary method shown in FIG. 10, data is received wirelessly from the medical device (1110). Accordingly, any system implementing the method of FIG. 10 does not need to be physically connected to the medical device to receive the data. Patients monitored by medical devices are thus able to lead active lifestyles without being forced to remain close to the system receiving the data from the medical device. Data can be received from any medical device, such as a blood glucose meter, a pacemaker, a blood pressure monitor, an insulin pump, a pulse oximeter, a holter monitor, an electrocardiograph, an electroencephalograph, a blood alcohol monitor, an alcohol breathalyzer, an alcohol ignition interlock, a respiration monitor, an accelerometer, a skin galvanometer, a thermometer, a patient geolocation device, a scale, an intravenous flow regulator, patient height measuring device, a biochip assay device, a sphygmomanometer, a hazardous chemical agent monitor; an ionizing radiation sensor; a monitor for biological agents, a loop recorder, a spirometer, an event monitor, a prothrombin time (PT) monitor, an international normalized ratio (INR) monitor, a tremor sensor, a defibrillator, or any other medical device. A medical device that includes a combination of different medical devices (such as those listed previously) may be monitored in accordance with the present invention. The medical device can be partially or completely implanted in a patient, such as in the case of a pacemaker. The medical device may also be located externally to a patient. The medical device may be connected to a patient (for example, through one or more electrodes), or operate independent of any coupling to a patient, such as a scale. The medical device may also operate in conjunction with a temporary interfacing with a patient, such as the case of the cuff of a blood pressure monitor encompassing the arm of a patient to take a reading.

The medical device data can be received by any person, system, device, or other suitable recipient. The exemplary method in FIG. 10 may be practiced manually by a human being, automatically by a device, or a combination of the two. An exemplary device for performing the method depicted in FIG. 10 is depicted in FIG. 11 and is discussed in detail below.

Data can be received directly from a medical device. For example, some medical devices such as pacemakers and other devices implanted in a patient include wireless transmitters to wirelessly broadcast data. A medical device can also provide data wirelessly using another device. In one embodiment of the present invention, for example, a medical device provides data through a serial port (a wired connection) to a computing

device. The computing device is in turn connected to a wireless router. The data can thus be received wirelessly after being retransmitted from the wireless router.

The medical device may transmit on any frequency using any format and protocol. For example, various medical devices transmit data in the Wireless Medical Telemetry Service (WMTS) frequency bands. There are three WMTS frequency bands, including frequencies from 608 MHz to 614 MHz, 1395 MHz to 1400 MHz, and 1427 MHz to 1432 MHz. In another example, the medical device may transmit using the Medical Implant Communications Service (MICS) frequency band, including frequencies from 402 MHz to 405 MHz. In yet another example a medical device may transmit data in the 32 KHz to 175 KHz range.

The medical device data can be received from a plurality of different medical devices, where each medical device may perform any combination of functions. For example, data from a glucose meter, blood pressure monitor, and combination scale/height measuring device each transmitting data in different formats and on different frequencies may each be received in accordance with the present invention. In the case where a plurality of medical devices transmits data in response to a request for data, each device in the plurality of devices can be sent such a request separately. Alternatively, a plurality of medical devices automatically transmitting data on the same frequency, in the same format, and potentially at the same time (such as in the case of multiple devices of the same type and/or from the same manufacturer) can be received in accordance with the present invention by, for example, using a separate wireless receiver keyed to a unique identifier associated with each medical device. When data has been received from a plurality of medical devices, in one embodiment, a list of the medical devices may be displayed on a user interface, and optionally, the user may be prompted to select one, all, or none of the plurality medical devices, whose data is desired to be transmitted to the medical data server. The data for the selected set of medical devices is then relayed as described with alternate embodiments as described herein. Any other suitable method for receiving data from a plurality of medical devices may also be used in conjunction with the present invention.

Any type of data may be received from a medical device. For example, the data may include information regarding a patient, such as the patient's biological and biometric information, the patient's behaviors, results of analysis of physical patient parameters, and information regarding the patient's environment. For example, a medical device such as a glucose meter could provide data regarding a patient's current (or last measured) blood glucose level, the date and time the patient last used the glucose meter, and the current temperature or other environmental factors that might affect a glucose test. Other possible environmental parameters that may be included in the data received from a medical device include a battery charge level, a temperature, a barometric pressure, a code relating to an accessory for the medical device, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, and a quality of service (QoS), and combinations thereof. Data received from a medical device may also include any other suitable information, such as diagnostic information regarding the medical device.

The medical device data may provide data relating to a single patient or multiple patients. In the case where a single medical device provides data regarding multiple patients, the data can be identified with an individual patient either in the

data received by medical device (such as by using a patient identifier) or through processing in accordance with the present invention.

The medical device can provide the data in any format. Different medical devices from different manufacturers often use different formats for providing data. For example, data from a glucose meter may be provided in a series of fixed-length data records followed by a terminator indicator (such as a null or other predefined character) and/or a checksum for validating the data. Any type of data may be provided. In the case of a glucose meter, the data may include one or more readings of a patient's blood glucose level and the date and time each reading was taken. The medical device identifier discussed previously may be used to determine a specific data format used by a medical device. Alternatively, a data format may be specified by a user or selected by analyzing the format of the data received and comparing it to a set of known medical device data formats.

Validate Data

In the exemplary process shown in FIG. 10, the data from the medical device is validated (1115). The data from the medical device can be validated in any suitable manner to achieve any result. For example, the data from the medical device may be validated to ensure it was transmitted properly and completely. The medical device data may also be validated to ensure it was provided from a specific medical device or particular type of medical device. The data may also be validated to ensure that fields in the data correspond to predetermined values and/or are within certain thresholds or tolerances. Any number, code, value or identifier can be used in conjunction with validating the medical device data. For example, the data can be validated by analyzing a medical device serial number, a medical device identifier, a patient identifier, one or more parity bits, a cyclic redundancy checking code, an error correction code, and/or any other suitable feature.

Authenticate Intermediary Device

In the exemplary method depicted in FIG. 10, an intermediary device receiving the data is authenticated (1120). In the context of the present invention, the intermediary device includes any type of system or device capable of receiving the medical device data in any manner. Such intermediate devices may include, for example, personal computers, laptops, personal digital assistants, and mobile computing devices. The intermediary device may process the data in any manner, and can transmit some or all of the data to another recipient, such as a medical data server. For example, but not by way of limitation, the intermediary device may include a personal computer or a mobile computing device, such as a laptop computer, a mobile wireless telephone, or a personal digital assistant (PDA). In an exemplary embodiment of the present invention, the intermediate device further includes software for receiving the medical device data, formatting a message based on the data, and transmitting the formatted message to a medical data server. Such software can operate on any suitable mobile computing device and with any computer operating system. The intermediary device may also include any number of other systems and devices suitable for receiving data from the medical device, processing the data, and/or transmitting the data to a medical data server. Further discussion regarding exemplary embodiments of intermediary devices is presented later in this description.

The intermediary device can receive the data directly from the medical device, or from one or more other devices. In one exemplary embodiment of the present invention, the intermediary device comprises a mobile computing device including one or more wireless transceivers and is configured to receive

data from the medical device directly. In another exemplary embodiment of the present invention, the medical device transmits the data to a first device, which in turn transmits the medical device data to the intermediary device (wirelessly or through a wired connection).

The intermediary device may be authenticated to achieve any result. For example, the intermediary device may be authenticated to restrict transmission of the data from the medical device to intermediary devices operating as part of the present invention. Authentication can also prevent sensitive medical data from being broadcast and viewed by unintended recipients. The intermediary device may also be authenticated to verify the intermediary device is able to receive, process, and/or transmit the medical device data to a medical data server. During authentication, the authenticated device or devices may also be remotely commanded, and such commands may include steps that configure devices to interoperate with components of the present invention. For example, but not by way of limitation, such steps may include the downloading of software applications, applets, embedded operating code, and/or data.

The intermediary device can be authenticated in any manner. For example, an intermediary device can be authenticated to receive data from one or more medical devices using an authorization code. The authorization code can be any number, code, value or identifier to allow the intermediary device to be identified as a valid recipient of the data from the medical device. In one exemplary embodiment of the present invention, an intermediary device stores an authorization code and broadcasts the authorization code in response to a request for authorization. Unless the authorization code matches a code stored by the transmitter of the medical device data (such as the medical device itself or another transmission device), the medical device data is not transmitted to the intermediary device. Transmission of the medical device data to the intermediary device need not necessarily be predicated upon successful authentication of the intermediary device, however.

In another exemplary embodiment of the present invention, an intermediary device receiving the medical device data using a wireless network protocol (such as Bluetooth) is authenticated based on whether the intermediary device advertises one or more services. In this context, advertised services reflect functions, utilities, and processes the intermediary device is capable of performing. The intermediary device broadcasts indicators of this functionality, thus "advertising" them to other systems and devices. In the present exemplary embodiment of the invention, unless the intermediary device advertises a service that is identifiable with the operation of the present invention (i.e. a process capable of broadcasting the medical device data to a medical data server, for example), the intermediary device is not authenticated and thus the medical device data is not transmitted to the intermediary device.

Activate Intermediary Device

In the exemplary process depicted in FIG. 10, the intermediary device can be activated (1125) prior to transmitting the medical device data to the intermediary device. Many devices, particularly mobile computing devices running on batteries, employ power-saving features to conserve battery life when not in use. In the case where an intermediary device is in a power-saving or standby mode, it may be necessary to activate the intermediary device before it can receive the medical device data. The intermediary device can be activated in any suitable manner. For example, a signal configured to activate the device may be transmitted to prepare the intermediary device to receive the medical device data.

Transmit Data to Intermediary Device

The medical device data is transmitted to the intermediary device (1130). The data can be transmitted in any suitable manner. In one exemplary embodiment of the present invention, the medical device data is transmitted to the intermediary device using a wired connection, such as an RS-232 serial cable, USB connector, Firewire connector, or other suitable wired connection. The medical device data can also be transmitted to the intermediary device wirelessly using a wireless transmitter. Any suitable method of wireless communication can be used to transmit the medical device data, such as a Bluetooth connection, infrared radiation, Zigbee protocol, Wibree protocol, IEEE 802.15 protocol, IEEE 802.11 protocol, IEEE 802.16 protocol, and/or ultra-wideband (UWB) protocol. If desired, the medical device data could be transmitted to the intermediary device using both a wired and wireless connection, such as to provide a redundant means of communication, for example.

Any amount of medical device data can be transmitted to the intermediary device in any manner. For example, data from the medical device can be transmitted to the intermediary device in real-time, or medical device data can be stored (such as in a memory storage device) for a period of time before being transmitted to the intermediary device. In some cases, for example, it may be more efficient to transmit blocks of medical device data at once rather than initiating communication with an intermediary device each time data is available from the medical device. In other cases, the intermediary device may be out of range or otherwise unavailable to receive the medical device data. The medical device data can also be stored for any desired length of time, and/or until a particular event occurs. For example, the medical device data could be stored until it is verified that the intermediary device and/or the medical data server have received the data, allowing the data to be retransmitted if necessary.

The medical device data can be transmitted to the intermediary device in any format. For example, the data from the medical device can be transmitted to the intermediary device exactly as it is transmitted from the medical device. This would be the case in embodiments of the present invention where the medical device itself is transmitting the data directly to the intermediary device. Alternatively, in embodiments of the present invention where the data is being received from the medical device and then retransmitted to the intermediary device, the medical device data can be reformatted, modified, combined with other data, or processed in any other suitable manner before being transmitted to the intermediary device. For example, the medical device data can be encrypted prior to transmission to the intermediary device, and this encryption may occur at any stage, for instance in the medical device itself or at a stage after being transmitted by the medical device. In cases where the medical device data is being combined with other data and transmitted to the intermediary device, all of the data may be encrypted or simply the medical device data itself. In an alternate embodiment, a digest of the medical data may be encrypted, to digitally "sign" the data contents to verify its authenticity. For example, but not by way of limitation, this digest may be produced by providing the received medical data to a hashing algorithm such as the MD5 or SHA-1 Secure Hashing Algorithm as specified in National Institute of Standards and Technology Federal Information Processing Standard Publication Number 180-1.

Asymmetric encryption algorithms and techniques are well known in the art. See, for example, RSA & Public Key Cryptography, by Richard A. Mollin, CRC Press, 2002, and U.S. Pat. No. 4,405,829, issued Sep. 20, 1983, the disclosures

of which are fully incorporated by reference herein for all purposes. In an illustrative example, if two parties (for example, "Alice" and "Bob") wish to communicate securely using public key cryptography, each party begins by generating a unique key pair, where one of the keys is a private key that is kept in confidence by that party, and the other key is a public key that may be publicly distributed, published only to a message recipient, or made available through a public key infrastructure. The key generation step need be done by a party only once, provided that the party's private key does not become compromised or known by another party. If Alice wants to send a message confidentially to Bob, she may use Bob's public key to encrypt the message, and once sent, only Bob can decrypt and view the message using Bob's private key. But if Alice also wanted Bob to have assurance that the message was in fact coming from her, she could further encrypt the message with her private key before sending, then when Bob's private key and Alice's public key are used to decrypt the message, Bob knows for certain that he was the intended recipient and that Alice was the one who originated the message, and Alice knows that only Bob will be able to decrypt and read her message.

Asymmetric cryptography may be utilized to enhance security of certain implementations of the present invention. In an alternate embodiment, data transmitted by a medical device 1250 is encrypted with a private key of the medical device user (or optionally with the private key of a health care provider that is operating the medical device), or with a public key of the intended recipient system such as the medical data server 1270, or with both keys. The private and/or public keys may be delivered to the medical data translator 1200 through a wired or wireless connection, allowing the translator 1200 to be configured for secure operation. In one embodiment, the system or medical data server 1270 may request that the public key of the medical device be forwarded to enable decryption of any medical information encoded with the user's private key. In this manner, the data may be authenticated as coming from the actual patient that is desired to be monitored, and optionally, the patient may also be assured that only the intended recipient system or medical device server 1270 is capable of decrypting and gaining access to the patient's medical device data.

In alternate embodiment, encrypted or unencrypted data can be transmitted through an encrypted transmission protocol, such as the wireless encryption protocols (WEP, WPA and WPA2) associated with the IEEE 802.11 wireless protocols. Any number of other encryption methods can be used to encrypt the medical device data in conjunction with the present invention. The intermediary device may decrypt the medical device data, to allow processing of the data for example. Alternatively, to protect the data from unauthorized viewing, an intermediary device could simply retransmit the encrypted data to the medical data server.

Confirm Transmission of Data to Intermediary Device

The transmission of the medical device data can be confirmed (1135) to verify the transmission was successful. The transmission can be confirmed in any suitable manner. For example, the intermediary device can transmit an acknowledgement once the transmission is received, otherwise the transmission can be rebroadcast.

Validate Data Transmitted to Intermediary Device

In the exemplary process shown in FIG. 10, the data transmitted to the intermediary device is validated (1115). The data from the medical device can be validated in any suitable manner to achieve any result. For example, the data from the medical device may be validated to ensure it was transmitted properly and completely. The medical device data may also

be validated to ensure it was provided from a specific medical device or particular type of medical device. The data may also be validated to ensure that fields in the data correspond to predetermined values and/or are within certain thresholds or tolerances. Any number, code, value or identifier can be used in conjunction with validating the medical device data. For example, the data can be validated by analyzing a medical device serial number, a medical device identifier, a patient identifier, one or more parity bits, a cyclic redundancy checking code, an error correction code, and/or any other suitable feature.

Store Data

The intermediary device may store the medical device data (1145). The intermediary device may store the data in any suitable manner, such as by using a memory storage device. Any portion or amount of medical device data (or other forms of information) received or generated by the intermediary device may be stored for any length of time. The data may be stored for a predefined period of time and/or until an event occurs. For example, in one embodiment of the present invention the data is stored by the intermediary device until the data has been transmitted to the medical data server. In another embodiment, data is stored by the intermediary device until a predetermined data transmission record size has been reached, so as to reduce communication charges that may accrue during transmission. In yet another embodiment, the intermediary device stores the data until an acknowledgment from the medical data server is received, where the acknowledgment indicates that the stored data has been received by the medical data server.

Format Message for Transmission to Medical Data Server

In the exemplary method according to an aspect of the present invention depicted in FIG. 10, a message is formatted for transmission to the medical data server. The message can originate from any system operating in conjunction with the present invention. For example, the message may be created by the intermediary device, a device transmitting the medical device data to the intermediary device, or the medical device itself. The message can include some or all of the medical device data, as well as any other information useful to the medical data server. Multiple messages can be formatted to include any desired amount of medical device data. For example, in the case of data from a glucose meter, multiple messages may be formatted to each include a single glucose reading, or a single message could be formatted to include the last ten glucose readings taken by the meter. The message can include any other desired data from any suitable source. For example, real-time data from a medical device may be included in a message along with previously-transmitted data from the stored by the intermediary device creating the message. The message (in whole or in part) may be encrypted to protect the contents of the message from unintended viewers and/or the privacy of the patient being monitored.

The message provides the medical device information to the medical data server in a format the medical data server can recognize and utilize. The message can thus be formatted to only include portions of the medical device data needed by the server and/or additional information about a patient, the medical device, and/or the treatment regimen. The message can be of desired format. For example, the message can be included in a file having a tokenized format such as standard ASCII text format, or any other suitable standardized file format, such as an MS Word document, MS Excel file, Adobe PDF file, or binary picture file (JPEG, bitmap, etc.). The data within such a file can be ordered in any manner and have any suitable delimiters, notations, or other features. For example, a list of multiple glucose level readings in a text file message

could be provided chronologically by when the readings were taken, with comma or tab delimiters to denote the start and end of each reading. The message may also have a unique and/or propriety format.

The format of the message can also be based on the method by which the message is transmitted to the medical data server. For example, where the message is transmitted to the medical data server using a wireless mobile telephone such as a cellular phone, the message can be formatted as an SMS text message. Similarly, the message may be formatted as an XML record, email, and/or facsimile. The message can include multiple formats and/or multiple messages may be formatted having different formats for transmission in a variety of methods or to a variety of recipient medical data servers.

Transmit Formatted Message to Medical Data Server

The message is transmitted to a medical data server (1155) to allow the medical device data to be analyzed and processed. The message can be transmitted to a single medical data server, or to a plurality of medical data servers. The medical data server can be any suitable recipient of the medical device data. For example, the medical data server can be a computer system or other device as well as a human recipient (such as a doctor, nurse, or other healthcare provider).

The message can be transmitted to the medical data server in any suitable manner. For example, the message can be transmitted to the medical data server through a wired connection, such as a telephone line, fiber optic cable, and/or coaxial cable. The message may also be transmitted wirelessly using any suitable wireless system, such as a wireless mobile telephony network, General Packet Radio Service (GPRS) network, wireless Local Area Network (WLAN), Global System for Mobile Communications (GSM) network, Personal Communication Service (PCS) network, Advanced Mobile Phone System (AMPS) network, and/or a satellite communication network. The message may be transmitted using any suitable combination of multiple wired and wireless communication methods. The transmission method selected to transmit the message to the medical data server can be chosen according to any desired criteria. For example, one or more transmission methods can be selected from a plurality of possible transmission methods to send the message based on each method's cost, time required to transmit, reliability, security, or any other suitable factor.

Receive Command from Medical Data Server

In addition to receiving the medical device data, the medical data server can transmit a command (1160). The command can be received by the intermediary device, the medical device, and/or any other suitable recipient. Any number of commands of any type may be transmitted by the medical data server. The command can be transmitted using the same variety of wired and wireless methods discussed previously for the transmittal of the formatted message. The command need not be transmitted using the same communication method with which the formatted messages are transmitted to the medical data server.

In one embodiment of the present invention, for example, the medical data server issues a command to reconfigure a software application operating on the intermediary device. In another embodiment, the medical data server issues one or more commands to control the functionality of the medical device. In yet another embodiment, the medical data server issues one or more commands to request that a public encryption key corresponding to the patient using a medical device be forwarded to the medical data server, or that a device associated with the present invention receive a public encryption key corresponding to an intended recipient such as a

particular health care service provider or other known destination such as the medical data server.

The commands need not be sent directly to a device they are intended to control. For example, a command could be transmitted to an intermediary device, which in turn retransmits it (unmodified) to the medical device to be controlled. Alternatively, the intermediary device could receive a command from the medical server, analyze it, and then transmit an appropriately formatted command tailored to the specific medical device to be controlled. In this manner, the medical data server need not be able to generate a command for each and every specific device it wishes to control, it can send a command appropriate to a class of devices (i.e. glucose meters) and the intermediary device will appropriately translate the command to control the medical device. The commands from the medical data server can initiate/run diagnostic programs, download data, request the patient's public encryption key, download the intended recipient's public encryption key, and perform any other suitable function on the intermediary device, medical device, or other devices operating in conjunction with systems and methods of the present invention.

A command from a medical data server can be in any appropriate format and may include any suitable information. For example, a command may include data received from one medical device **250** to be delivered to another medical device **250** through the medical data translator **1200**. In this manner, a variety of medical devices can share data whether they are in communication with the medical data translator **1200** or not.

A command can also originate from an intermediary device. For example, a command to program or reconfigure one or more software programs on the medical data translator **1200** depicted in FIG. **11** can be provided by an intermediary device **1260** to the medical data translator **1200** through the data relay transceiver **1230**. A command, as discussed above, may include multiple instructions, applets, or data elements to be processed, such as sections of executable code or interpretable scripts. Additionally, a user can program or configure a software program on any device operating in conjunction with the present invention through a suitable user interface, such as the user interface **1290** of medical data translator **1200**.

In any system where commands can be sent remotely, security is always a concern, especially when a wireless implementation may provide an entry vector for an interloper to gain access to components, observe confidential patient data, and control health-sensitive components such as pacemakers and insulin pumps. In any digital data network, it is also possible that commands intended for one recipient may be misrouted to a patient or health care provider that was not the intended recipient of the command. There are, however, a number of methods to provide for enhanced security in a remote command system while still allowing flexibility and minimal obtrusiveness.

In one embodiment, a command received by any of the components in FIG. **11** may be authenticated before the command is either acted upon by the destination component, or forwarded to another component in the system. Authentication may be directed to determining (1) whether the command came from a trusted or authorized source and (2) that the recipient is actually the intended recipient of the command. In one implementation, source command authentication is achieved by determining whether the origin of the command is a trusted component or server, and one way to accomplish this determination is analyzing whether a command is properly digitally signed by the originator, or some other authentication information is provided that assures the recipient

component that the message or command is authentic and the recipient component is actually the intended recipient. In an alternate implementation, destination command authentication is accommodated by examining the contents of the message or an authorization code to determine the intended recipient, or alternatively decrypting the command or a portion of the command to verify the intended recipient.

In one embodiment, when commands are created by a command originator, the originator provides for a means to verify the authenticity and/or validity of the command by at least one of the following methods: (1) encrypting the command with a private key of the command originator; (2) generating a digest of the command (through a method such as a hashing algorithm discussed above) and optionally encrypting the hashed digest with the command originator's private key, or (3) utilizing a symmetric encryption scheme providing an authentication code (such as a cryptographically hashed password) that is compared to previously stored values. Then, when a system component receives the command along with any encrypted or cleartext certification data, the component may determine the command is valid by (1) attempting to decrypt an encrypted command message with the alleged originator's public key, (2) attempting to decrypt an encrypted digest with the alleged originator's public key, and comparing the result to a hashed value of the command, or (3) comparing a cryptographically hashed password for the alleged originator to known pre-stored values, and if a match is found, authorization is granted. As an additional step, if the command were optionally encrypted using the intended patient/provider's public key, then only the recipient is capable of decrypting the command, ensuring that only the truly intended patient's health-care devices were being issued commands, and not an unintended third party. For example, in one embodiment, authenticating the command comprises decrypting at least part of the command using at least one of: a public key associated with the medical data server; a private key associated with a user of the medical device; and a private key associated with the medical device.

Authenticate User Access to Medical Data Server

In another embodiment, the method described in FIG. **10** may be used in conjunction with the authentication process described above for FIG. **9**.

Exemplary System Using Wireless Communication

An exemplary system for use in conjunction with the present invention is depicted in FIG. **11**. This system may be used in conjunction with the method described in FIG. **10**, as well as with any subset or combination of the elements thereof. The system shown in FIG. **11** may also be used in conjunction with any other suitable embodiments of systems and methods for medical device monitoring according to an aspect of the present invention.

The exemplary system for medical device monitoring depicted in FIG. **11** includes a medical data translator **1200** that includes a processor **1210** coupled to a memory **1220**. A data relay transceiver **230** wirelessly communicates with one or more intermediary devices **1260** via antenna **1232**, which in turn communicates with one or more medical device servers **1270** through either a wired or wireless protocol. An adapter module **1240** communicates with one or more medical devices **1250** via antenna **1243**. The adapter module **140** includes a medical device transceiver **1242** and an auxiliary communication system **1244**, both in communication with the processor **1210**. The auxiliary system **1244** may include any number of wired or wireless connections to one or more computer systems **1280**, such as a universal serial bus (USB) connection, serial connection, parallel connection, Firewire connection, Ethernet connection, or any other suitable con-

nection. The medical data translator **1200** may include any suitable power connection for powering the translator and/or for recharging an energy storage device such as a battery (not shown). The components of the medical data translator **1200** may receive electrical power from any other type of power supply. The medical device transceiver is coupled to an antenna, **1243**, which may establish unidirectional or bidirectional wireless communications with one or more of the medical devices **1250**. The antenna **1243** may be the same antenna as antenna **1232**, or one or more separate antennas. The antenna **1243** may be located internally or externally to the adapter module **1240**, and may be configured in any suitable manner to operate with the medical data translator **1200**. The functionality of the medical data translator **1200** can be implemented in any suitable manner, such as through the processor **1210** executing software instructions stored in the memory **1220**. Functionality may also be implemented through various hardware components storing machine-readable instructions, such as application-specific integrated circuits (ASICs), field-programmable gate arrays (FPGAs) and/or complex programmable logic devices (CPLDs). Systems for medical device monitoring according to an aspect of the present invention may operate in conjunction with any desired combination of software and/or hardware components.

Medical Data Translator **1200**

Referring to FIGS. **12A** and **12B**, the medical data translator **1200** depicted in FIG. **11** is shown enclosed within a within a case **1300**. A case holding a system for medical device monitoring according to aspects of the present invention may be of any size, shape and configuration. The system (and case enclosing it) is preferably small enough to be easily portable by a patient or person being monitored. For example, the exemplary case **300** depicted in FIGS. **12A** and **12B** is 2.5 inches long, 2 inches wide, and 0.5 inches deep. The top and bottom of the case **1300** are 0.05 inches thick, while the sides of the case **300** are 0.075 inches thick. The case may be manufactured from any number of materials, such as plastic, metal, wood, composites, and/or any other suitable material. The case **1300** shown in FIGS. **3A** and **3B**, for example, is manufactured from hard plastic.

The case **1300** includes battery compartments **1320** for powering the data translator **1200**. The case **1300** also includes an interface module **1310** that includes the adapter **1240**. The interface module **1310** may include any suitable portion of the medical data translator **1200**. In the exemplary embodiment depicted in FIG. **11**, the interface module **1310** includes the adapter module **1240** comprising a medical device transceiver **1242** and auxiliary communication system **1244**. In this embodiment, the interface module **1310** is removably attached to the case **1300** to allow different modules **1310** to be interchangeably connected to the case **1300** to communicate with different medical devices **1250**.

In another exemplary embodiment of the present invention, referring now to FIGS. **12C** and **12D**, a case **1370** includes a removable adapter module **1380** that includes an antenna **1385** for communicating with a medical device **1250** through a wireless connection. The adapter module **1380** connects to the case **1370** using plug **1387**. The plug **1387** attaches to a corresponding port on the case **1370** (not shown) to hold the adapter module **1380** in place and allow the communication of data through the adapter module **1380**. The plug **1387** can utilize any desired wired connection, such as a USB connection. The adapter module **1380** connects to the case **1370** using plug **1387**. The plug **1387** attaches to a corresponding

port on the case **1370** (not shown) to hold the adapter module **1380** in place and allow the communication of data through the adapter module **1380**.

The case can include any other suitable features. For example, the case may include a screen, lights, LEDs, keys, speaker, and microphone grille to support features of a user interface included in a system for medical device monitoring. The exemplary systems for medical device monitoring shown in FIGS. **11**, **12A**, **12B**, **12C**, **12D** and **12E** are all configured to fit in a container along with the medical device it communicates with to allow a user to easily transport the medical device and the data translator together.

Other embodiments of systems for medical device monitoring according to aspects of the present invention can be configured to be in small enough to be coupled with or integrated into a medical device **1250** or an intermediary device **1260**. For example, a medical device **1250** may be manufactured to include a medical data translator **1200** within the packaging housing the medical device **1250**. Similarly, a medical data translator **1200** can be integrated as part of an intermediary device **1260** such as a cellular phone, PDA, or other mobile computing device. The intermediary device **1260** could thus be configured to both receive data from a medical device **1250** as well as transmit messages regarding the medical device **1250** and/or patient to a medical data server **1270**.

Alternatively, a medical data translator **1200** can be configured to be physically attached to a medical device **1250** or intermediary device **1260**. For example, where an intermediary device **1260** such as a mobile wireless telephone or PDA is used in conjunction with embodiments of the present invention, one exemplary embodiment of a medical data translator **1200** and its case **1300** is configured to match the size and shape of the of the intermediary device **1260** and attach to the back of the intermediary device **1260** using metal or plastic clips that wrap around the face and/or sides of the intermediary device **1260**. When attached, the medical data translator **1200** conforms to the size and shape of the outline of the intermediary device **1260**, and is preferably shaped to conform to the dimensions of the back of the intermediary device **1260** to avoid unnecessarily impacting the original size of the intermediary device **1260**. In this embodiment, the case of the medical data translator **1200** may also include other desirable features, such as a belt clip to allow the data translator/intermediary device combination to be worn by a user.

Turning to FIG. **13**, in another exemplary embodiment of the present invention, the medical data translator **1200** is contained in a flexible, protective container **400** that opens to allow a medical device **1250** and/or intermediary device **1260** (such as a cellular phone, PDA, or other mobile computing device) to be likewise contained therein. This allows a medical data translator **1200** to be used with a variety of intermediary devices **1260**, and may (in some cases) provide a more cost effective approach to integrate the medical data translator **1200** with an intermediary device **1260** or medical device **1250**. In this embodiment, the medical data translator **1200** can be integrated within the protective container **1400** itself, with the container acting as the case for the data translator **1200**.

Alternatively, as depicted in FIG. **13**, the medical data translator **1200** may simply be contained within a pouch or other structure within the container **1400**. The exemplary container **1400** depicted in FIG. **13** also includes a holder **1420** for the medical device **1250** formed from clear plastic to allow a user to read a display **1422** and/or operate keys **1424** on the medical device **1250**. The protective container **1400** can also be sized to comfortably fit and protect any other

desired item, such as a day planner, wallet, notepad, and/or writing utensil or PDA stylus. The protective container can be made from any desired material, such as leather, plastic, nylon, cordura, or other flexible material. The protective container can be sealed in any manner, such as by using snaps, hook-and-loop closures, buttons, and/or a zipper. The exemplary container **1400** depicted in FIG. **13**, for example, is sealed using a zipper **1430**. The container **1400** can be water-proof, heat resistant, and/or include padding to protect the medical data translator and other contents from the shock of a fall. The container **1400** may include any number of pockets, pouches, or other sub-containers inside or outside the case to hold accessories associated with the medical device **1250**, intermediary device **1260**, or other item(s) stored within the container **1400**.

The exemplary protective container **1400** depicted in FIG. **13** is configured to hold a medical device **1250** (specifically, a glucose meter) and a medical data translator **1200** according to an aspect of the present invention. In this exemplary embodiment, the protective container **1400** is closed using a zipper **1430** that runs along the exterior of the sides of the container **1400**. A user unzips the two halves of the container **1400** and opens the container **1400** to display the glucose meter contained in the holder **1420** attached to the interior of one half of the container **1400**, while the medical data translator **1200** is contained in a pouch **1410** attached to the interior of the other half of the container **1400**. The pouch **1410** is formed from a nylon mesh material to allow a user to see and/or interact with user interface features of the medical data translator **1200**. The pouch **1410** is sealed with a zipper **1412**. The container **1400** includes a flexible elastic strap **1440** to hold a container of blood sugar metering strips **1442**. The container **1400** may include any number of other pouches or containers on the interior or exterior of the container for storing batteries and/or power cables for the glucose meter and/or medical data translator **1200**, and other items of use to the patient carrying the container, such as bottles of insulin and needles for use by the patient depending on the outcome of a reading by the glucose meter.

Processor **1210**

The processor **1210** retrieves and executes instructions stored in the memory **1220** to control the operation of the medical data translator **1200**. Any number and type of processor such as an integrated circuit microprocessor, microcontroller, and/or digital signal processor (DSP), can be used in conjunction with the present invention. Referring now to FIG. **14A**, an exemplary medical data translator **1200** according to an aspect of the present invention is implemented using a microcontroller **1501**. In the exemplary systems depicted in FIGS. **14A** and **14B**, the microcontrollers **1501** and **1530** include a Universal Asynchronous Receiver/Transmitter (UART) and Universal Serial Bus (USB). The microcontroller **1530** depicted in FIG. **14B** additionally includes a digital signal processor (DSP) for communication with a cellular RF Transceiver **1540** as will be discussed in more detail below. The microcontrollers **1501**, **1530** depicted in FIGS. **14A** and **14B**, respectively can include any other suitable components and features, such as analog-to-digital converters (ADCs) (**1520**), and/or digital-to-analog converters (DACs) (**1515**), though these components have been shown outside the microcontrollers **1501**, **1530** for clarity.

Power Source

Any number, combination, and type of suitable power sources can be utilized in accordance with aspects of the present invention. The exemplary systems depicted in FIGS. **14A** and **14B** are powered by a rechargeable 4.2V Lithium Ion battery **1506**. One DC to DC converter **508** is used to steps

down the voltage from the battery **1506** to 3.3V for use by some components in the system, while another DC to DC converter **1509** is used to step up the voltage to 5V for use by other components. The battery **1506** can be recharged through the VBUS lead of the USB connector **1504** and charging circuit **1507**. Both converters **1508**, **1509** can be enabled and disabled via signals from the microcontroller **1501** on OUT1 and OUT2 to save power and extend the life of the battery **1506**. The microcontroller **1501**, **1530** can monitor the voltage of the battery **1506** using ADC **1520**, FET circuit **1521**, and voltage divider **1522**. The voltage divider **1522** is used because the voltage of the battery **1506** when fully charged (4.2V) is greater than the maximum 3.3V input that can be accepted by the ADC **1250**. The FET circuit **1521** connects the battery **1506** to the voltage divider **1522** only when a battery test is being performed (i.e.—when pin OUT10 is grounded) to avoid a constant drain on the battery **1506** when the system is otherwise powered down.

Any other suitable battery may be used according to any desired criteria. For example, a rechargeable battery or batteries integrated with the data translator may be selected to reduce the overall size of the medical data translator **1200** and/or provide for the convenience of a user who would not need to replace batteries. One or more standard replaceable batteries (i.e. alkaline AA or AAA batteries) may be selected to reduce the price of the medical data translator **1200**. The power supply circuitry shown in FIGS. **14A** and **14B** is exemplary only, and may be implemented by using other conventional power supply approaches. The medical data translator **1200** and other systems for medical device monitoring according to various aspects of the present invention can utilize any appropriate power supply devices, components, circuits, and systems.

Memory **1220**

The exemplary system in FIG. **11** includes a memory **1220**. The memory **1220** stores instructions, medical device data, messages transmitted to or received from the medical data server **1270**, and any other suitable information. A memory operating in conjunction with the present invention may include any combination of different memory storage devices, such as hard drives, random access memory (RAM), read only memory (ROM), FLASH memory, or any other type of volatile and/or nonvolatile memory.

In the exemplary embodiments of medical data translators **1200** depicted in FIGS. **13A** and **13B**, the microcontroller **1501** and **1530** each include an on-chip memory. In addition, the microcontroller **1501**, **1530** is coupled to a flash memory **1513**. The flash memory **1513** may be of any size to achieve any desired purpose. In this exemplary embodiment, the size of flash memory **1513** is selected to adequately store pre-recorded voice recordings to be played through the speaker **1518**, discussed below. Any number of memory storage devices of any size and configuration may also be used in conjunction with the present invention.

Data Relay Transceiver **1230**

The data relay transceiver **1230** communicates with one or more intermediary devices **260**, medical data servers **1270**, or other suitable systems. Any suitable communications device, component, system, and method may be used in conjunction with the present invention. In the exemplary circuits shown in FIGS. **14A** and **14B**, the data relay transceiver **1230** comprises a Bluetooth transceiver **1512** that is in bidirectional communication with the microcontroller **1501**, **1530** through the UART interface on the microcontroller **1501**, **1530**.

The medical data translator **1200** may include, or operate in conjunction with, any number of data relay transceivers **1230**. In FIG. **14B**, for example the exemplary medical data trans-

lator **200** further includes a cellular radio frequency (RF) transceiver **1540** in communication with microcontroller **1530**. In this exemplary embodiment, the microcontroller **1530** is a cellular baseband processor that includes a digital signal processor (DSP) which communicates data through a cellular RF power amplifier and front end **1550** connected to a cellular antenna **1555**. Data is transmitted by the microcontroller **1530** on the CELL TX line and received by the microcontroller **1530** on the CELL RX line. Additionally, the microcontroller **1530** can control various features of the RF transceiver **1540** via the CELL CTRL line. The RF power amplifier and front end **1550** performs the necessary functions to transmit and receive cellular signals, such as power amplification, power detection, filtering, and input/output matching.

The medical data translator **1200** depicted in FIG. **14B** may be configured to communicate using any number and type of cellular protocols, such as General Packet Radio Service (GPRS), Global System for Mobile Communications (GSM), Enhanced Data rates for GSM Evolution (EDGE), Personal Communication Service (PCS), Advanced Mobile Phone System (AMPS), Code Division Multiple Access (CDMA), Wideband CDMA (W-CDMA), Time Division-Synchronous CDMA (TD-SCDMA), Universal Mobile Telecommunications System (UMTS), and/or Time Division Multiple Access (TDMA). A medical data translator **1200** operating in conjunction with the present invention may alternatively (or additionally) include data relay transceiver **1230** components to communicate using any other method of wired or wireless communication.

As discussed previously, the medical data translator **1200** can transmit any data to any entity operating in conjunction with the present invention. For example, the medical data translators **1200** depicted in FIGS. **14A** and **14B** may transmit medical data to one or more intermediary devices **1260**, as well as to one or more medical data servers **1270**.

Adapter Module **1240**

Referring again to FIG. **11**, the exemplary medical data translator **1200** includes an adapter module **1240** for communicating with one or more medical devices **1250** as well as other suitable systems. The adapter module **1240** can be configured to communicate with any suitable class, type, and/or manufacturer of medical device **1250**. The adapter module **1240** in this example includes a medical device transceiver **1242** for communicating with one or more medical devices **1250** and an auxiliary communication system **1244** for communicating with an external personal computer system **1280** to upload software to the data translator **1200**, store data, provide or update encryption keys, perform diagnostics, and other appropriate purposes. The adapter module **1240** can be modular and removably attached to the body of the data translator **1200**, integrated as part of the data translator **1200**, or a combination of the two. Antenna **1243** may optionally be included in the adapter module **1240** assembly, or otherwise electrically coupled to the adapter module. In one exemplary embodiment of the present invention, the adapter module **1240** is removably attached to the body of the medical data translator **1200** to allow different medical devices **1250** to interoperate with the data translator **1200**. As new medical devices **1250** and/or new frequencies are utilized, an adapter module **1240** configured to communicate with the new device or new frequency can be added to the existing system. In the exemplary circuits depicted in FIGS. **14A** and **14B**, any of the components used to communicate with other devices, such as the USB connector **1504**, MICS transceiver **1510**, and Blue-

tooth transceiver **1512** can be included in an adapter module **1240** that is removably attached to the body of the medical data translator **1200**.

Software running on or operating in conjunction with the adapter module **1240** can be configured/updated through the auxiliary communication system **1244**, the user interface **1290**, or in response to a communication from an intermediary device **1260** or medical data server **1270** received through the data relay transceiver **1230**. This allows the functionality of the medical data translator **1200** to be dynamically updated and avoids the expense of having to create custom hardware implementations for every type of medical device to be monitored.

Medical Device Transceiver **1242**

The medical device transceiver **1242** wirelessly communicates with one or more medical devices **1250**. The medical device transceiver **1242** may include any number and combination of hardware and/or software components. In the exemplary medical data translator **1200** depicted in FIG. **11**, the medical device transceiver **1242** is integrated with the adapter **1240** and communicates with medical devices **1250** through an antenna **1243**. In this way, adapters **240** that allow connections to different medical devices can be used interchangeably with the same medical data translator **200**.

Any number of transceivers may be used in conjunction with the present invention, for example to communicate with multiple medical devices **1250** using different frequencies and/or communication protocols. The present invention may be used in conjunction with any communication protocol to communicate with one or more medical devices **1250**. For example, the medical data translator **1200** may be configured to communicate with one or more medical devices using (without limit): the WMTS frequency bands (608-614 MHz, 1395-1400 MHz, and 1427-1432 MHz), the MICS frequency band (402-405 MHz), 32 KHz-175 KHz, as well as any other suitable frequency band. The medical data translator **1200** may communicate with medical devices using any other method of communication, such as infrared radiation, Zigbee protocol, Wibree protocol, Bluetooth connection, IEEE 802.11 protocol, IEEE 802.15 protocol, IEEE 802.16 protocol, and/or Ultra-Wideband (UWB) protocol. In alternate embodiments, the medical data translator **1200** may selectively communicate with one or more medical devices by using time division multiple access (TDMA), frequency division multiple access (FDMA), code division multiple access (CDMA), or other multiple access protocols.

In the exemplary embodiment depicted in FIG. **11**, the medical device transceiver **1242** can be configured (e.g. through a software program residing in memory **1220** and executed by processor **1210**) to detect and switch to different frequencies emitted from one or more medical devices **1243**. Take for example, a hypothetical case where a patient has an implanted loop recorder broadcasting data regarding the patient's heart rate and rhythm using a MICS frequency, an implanted pacemaker broadcasting data at 32 KHz, and utilizes an external insulin pump communicating at 175 KHz. Each device could be produced by the same or separate manufacturers. The medical device transceiver **1242** according to various aspects of the present invention can be configured to detect the three devices and switch to the appropriate frequencies to communicate with each, thus providing interoperability between types and manufacturers of a wide variety of medical devices.

The medical data translator **1200** can be configured to automatically request data from one or more medical devices **1250** at predetermined times using the medical device transceiver **1242**. Any appropriate date or time setting may be

used. The data translator **1200**, medical device **1250**, or any other device operating in conjunction with the present invention can be configured to automatically request and/or transmit data in any suitable manner. For example, the medical data translator **1200** depicted in FIG. **11** can be configured through the auxiliary communication system **1244**, the user interface **1290**, and/or from a command issued transmitted by an intermediary device **1260** through the data relay transceiver **1230**. In the case of a command received through the data relay transceiver **1230**, the command can be generated by any suitable entity, such as from a medical data server **1260** or a user of the intermediary device.

The automatic requesting/transmission of data by a device operating in conjunction with the present invention may be subject to any suitable conditions or rules that dictate whether the data is in fact requested/transmitted. For example, a medical data translator **1200** programmed to request data from a medical device **1250** at a set time may first check to verify that the medical device is within range, that the translator **1200** has sufficient battery reserves to send the request and receive the data, whether the translator **1200** has sufficient space in the memory **1220** to store the data, and/or whether any other suitable condition is met.

In the exemplary circuits depicted in FIGS. **14A** and **14B**, the medical data transceiver **1242** comprises a 405 MHz transceiver **1510** in bidirectional communication with the microcontroller **1501**, **1530** through an Inter-Integrated Circuit (I²C) bus interface and a Serial Peripheral Interface (SPI) bus interface. The transceiver **1510** sends and receives signals in the 402-405 MHz MICS band through antenna **1560**. In this exemplary embodiment, the microcontroller **1501**, **1530** can activate the transceiver **1510** periodically to monitor for incoming signals from one or more medical devices **1250**. This mode of operation is useful for collecting data from medical devices **1250** that only broadcast data, but do not have the capability to receive requests for data. For medical devices **1250** that can both send and receive information, the microcontroller **1510**, **1530** can activate the transceiver **1510** to send a request for data to one or more medical devices **1250**. Both modes of operation help reduce the amount of time the transceiver **1510** is activated, and thus reduce the amount of power used by the system.

Auxiliary Communication System **1244**

The adapter module **1240** depicted in FIG. **11** includes an auxiliary communication system **1244** for communicating with additional systems and devices. The medical data translator **1200** or other system operating in conjunction with the present invention can include any suitable circuit, component, device, and system for communicating with any other device. In the exemplary circuits depicted in FIGS. **14A** and **14B**, the auxiliary communication system **1244** comprises a USB connector **1504**.

The auxiliary communication system **1244** can be used to transfer data to and from the medical data translator **1200**, as well as for an external computer system **1280** to configure or program software and hardware in the data translator **1200**. In one embodiment of the present invention, for example, a user operating computer system **1280** connected to medical data translator **1200** through the Internet can configure settings for the adapter module **1240**, data relay transceiver **1230**, and user interface **1290**. The computer system **1280** can also download data received by the data translator **1200** from one or more medical devices **1250**. Additionally, the computer system **1280** may communicate with the medical devices **1250** real-time through the medical device transceiver **1240**, such as to monitor or control one or more medical devices **1250**.

User Interface **1290**

The medical device **1250**, medical data translator **1200**, intermediary device **1260**, or other device operating in conjunction with the present invention may include a user interface. Referring to FIG. **11**, an exemplary user interface **1290** of a medical data translator **1200** in accordance with aspects of the present invention includes an input device **1292** and an output device **1294**. The input device **1292** receives commands, data, and other suitable input from a user. The output device **1294** provides the user with data, alerts, and other suitable information from the medical data translator **1200**.

Any number of input devices may be included in a user interface for one or more devices in the present invention. In one embodiment of the present invention, for example, the user interface **1290** includes a touch pad, a touch screen, or an alphanumeric keypad to allow a user to enter instructions and data into the medical data translator **1200**. One or more buttons on the keypad or touch screen can be programmed or configured to perform specific functions, such as to request data from one or more medical devices. The user interface **1290** can also include one or more multifunction switches, keys, or buttons that each allows a user to perform multiple functions.

The user interface may also include a microphone to allow the user to provide such information to the medical data translator **1200** verbally. In this exemplary embodiment, the medical data translator **1200** also includes speech recognition software to process verbal input through the user interface **1290**. The ability of the medical data translator to recognize speech from a patient can be particularly useful for users/patients who have vision problems, arthritis, or other impairments that would inhibit them from using a keypad or other input device. A microphone can be used in conjunction with audible (e.g. through sound waves perceivable by the human ear) data provided through a speaker, as discussed below, to allow a user to interact with any device operating in conjunction with the present invention in a completely auditory manner. In one nonlimiting example, audible input could also be sensed and analyzed by the medical data translator **1200** that a patient has uttered a command, such as the command to turn on. Bidirectional audible communication, in addition to aiding impaired patients, allows users to operate devices in the present invention in a hands-free manner which can increase the speed, ease, and efficiency in which a device (such as the medical data translator **1200**) can be utilized.

Devices operating in conjunction with the present invention may include any number of suitable output devices. Referring to the exemplary medical data translator circuits depicted in FIGS. **14A** and **14B**, a user interface including two lights **1514** (LED1 and LED2) may be used to indicate the status of the data translator to the user, as well as other pertinent information. For example, a flashing LED can be used to indicate when data from a medical device is in the process of being transferred, while a solid LED can indicate the transfer of data is complete. The medical data translators **1200** depicted in FIGS. **14A** and **14B** also provide auditory output through speaker **1518**. The microcontroller **1501**, **1530** retrieves audio samples, such as recorded speech, from the EEPROM **1513** and provides output to DAC **1515**, which converts the digital signal from the microcontroller **1501**, **1530** to an analog signal that can be output on the speaker **1518**. The analog signal is provided to an audio amplifier **1517** that amplifies the signal. The gain of the amplifier **1517** is set by the ratio of resistors **1516** and **1519**.

Any other suitable user interface features may similarly be included in devices and systems operating in accordance with the present invention. In another exemplary embodiment, for

example, the output device **1294** includes a display screen to visually display information as well as a speaker (e.g. speaker **1518** shown FIGS. **14A** and **14B**) to provide auditory output. The output device **1294** can include multiple transducers such as audio speakers or piezoelectric elements, amplifiers, and other appropriate devices and systems to provide the auditory output. The medical data translator **1200** may be configured to provide words, phrases, tones, recorded music, or any other type of auditory output to a user.

Any type of information may be communicated through the user interface **1290**, such as the biological, biometric, or behavioral information for one or more patients. The user interface can provide/receive any other suitable information, such as environmental information and/or diagnostic data for a medical device, a battery charge level, a temperature, a barometric pressure, a code relating to an accessory for the medical device, a biometric access measurement, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, and a quality of service (QoS), and combinations thereof.

Information provided or received by the user interface **1290** may be in any appropriate format. For example, a user interface that communicates information to a user in an auditory format may first provide a data header followed by a data value to identify the data to the user. Similarly, an output device **1294** providing information to a user visually may provide a series of measurements in the form of a spreadsheet with headers indicating the source of the measurements. The output device **1294** can also provide information in any number of desired languages, regardless of whether the information is provided audibly or visually.

Various features of the user interface can be implemented in hardware, software, or a combination of the two. In the medical data translator **1200** depicted in FIG. **11**, for example, the user interface **1290** includes voice interface software stored in the memory **1220**, including tables of recorded words and phrases. When executed by the processor **1210**, the voice interface software plays the appropriate recorded words and phrases (such as enunciating the medical data) through a speaker such as one included in the output device **1294** to provide information to the user. The voice interface software, like any software operating on the medical data translator **1200**, can be downloaded and configured through the auxiliary communication system **1244**. As discussed previously, any software program on any device operating in accordance with the present invention can be programmed or configured through any other suitable interface. In the medical data translator **1200**, for example, the voice interface software could also be downloaded and configured through the data relay transceiver **1230** in response from a command from a medical data server **1270** and/or intermediary device **1260**, as well as from input from the user through the user interface **1290**. Accordingly, the voice interface software can be configured to include words and phrases in any number of different languages, and can be updated with new words and phrases as desired, such as to accommodate a new medical device **1250** operating with the medical data translator **1200**. Non-verbal sounds, such as melodies and tones, can also be stored and used by the user interface **1294** to provide alerts, indicators, and other information to the user.

The user interface can also provide/receive information to a user in a machine-readable format. In one exemplary embodiment of the present invention, for example, the user interface **1290** of a medical data translator **1200** includes a fixed or retractable USB port to communicate with a thumb drive, memory stick, portable hard drive, an external com-

puter system, or other USB-compatible device. This allows doctors and other healthcare providers to directly access the medical data translator **1200** directly, without having to retrieve the data from a medical data server. In this exemplary embodiment, the medical data translator **1200** can be configured to send, receive, and process machine-readable data in any standard format (such as a MS Word document, Adobe PDF file, ASCII text file, JPEG, or other standard format) as well as any proprietary format. Machine-readable data to or from the user interface may also be encrypted to protect the data from unintended recipients and/or improper use. In an alternate embodiment, a user must enter a passcode to enable use of the USB port, and optionally, after a period of time of non-use, the USB port is automatically disabled. Any other user interface feature may be utilized to allow a human or non-human user to interact with one or more devices operating in conjunction with the present invention.

Power Saving Features

A medical data translator, intermediary device, medical device, or other system operating in accordance with aspects of the present invention may include any other suitable features, components, and/or systems. For example, the data translator **200** or other device may be configured to preserve the life of its battery by shutting off or going into a low-power mode when it, and/or the medical device it monitors, experiences a predetermined period of non-use, or a change in a measured parameter such as indication that a case holding the translator **1200** has been actuated to a closed position. Such devices can also be configured to become active in response to any suitable event, such as receiving a signal from a device (such as a sensor).

In one non-limiting embodiment of the present invention, referring now to FIG. **6**, a medical data translator **1200** communicates with a motion sensor **1610** and a light sensor **1620** to determine when a container **1630** holding the data translator **1200** and the medical device **1250** it monitors is open or closed. In this exemplary embodiment, the data translator **1200** can preserve the life of its battery by shutting off or going into a low-power mode when the container **1630** is closed and, therefore, the medical device **1250** held in the container **1630**, is not in use. Any type of motion sensor can be used in accordance with the present invention, such as an accelerometer, tilt switch, or other device that generates a signal in response to movement. Similarly, any type of light sensor may be used in conjunction with the present invention. The light sensor can be used to detect the amount of light entering a container **1630** holding the medical device **1250**, medical data translator **1200**, or other device to activate the device when the sensed amount of light exceeds a predetermined threshold, or if an increase in the amount of incident light exceeds a predetermined threshold. In an alternate embodiment, a microphone may receive audible signals that are analyzed by the medical data translator **1200** to determine that a command has been uttered, and such a command may include instructions that the medical data translator **1200** should be shut down or activated from a quiescent or low-power state.

A sensor may be integrated into the medical data translator **1200**, or operate externally to the data translator **1200**, communicating with the data translator **1200** wirelessly or through a wired connection. For example, in the exemplary embodiment depicted in FIG. **15**, the motion sensor **1610** and light sensor **1620** are integrated into the interior of the container **1630** and communicate with a medical data translator **1200** contained within to indicate when the container **1630** is actuated from a closed position to an open position.

Security Measures

Systems and devices operating in accordance with aspects of the present invention may implement one or more security measures to protect data, restrict access, or provide any other desired security feature. For example, any device operating in conjunction with the present invention may encrypt transmitted data and/or protect data stored within the device itself. Such security measures may be implemented using hardware, software, or a combination thereof. Any method of data encryption or protection may be utilized in conjunction with the present invention, such as public/private keyed encryption systems, data scrambling methods, hardware and software firewalls, tamper-resistant or tamper-responsive memory storage devices or any other method or technique for protecting data. Similarly, passwords, biometrics, access cards or other hardware, or any other system, device, and/or method may be employed to restrict access to any device operating in conjunction with the present invention.

Exemplary Method for Medical Data Collection and Transmission

FIG. 16 illustrates an exemplary method 1600 for medical data collection and transmission according to various aspects of the present invention. In method 1600, a medical device is authenticated (1605) and configured (1610). An interface with the patient may be established (1615) and data is received from the medical device (1620). A message including some or all of the medical device data is transmitted (1625). A request for a software or firmware update may also be transmitted (1630) and a command received (1635).

A medical device can be authenticated or authorized in any suitable manner, including the authentication methods described above. In one exemplary embodiment, the system 1700 is configured to automatically connect to, and communicate with, a medical device (either directly or through an intermediary device) with little or no action required by a user. The system 1700 can also be configured to automatically change settings on the medical device, as well as to download firmware or software updates to the medical device from a medical data server or other source. In this manner, the present invention allows medical devices to be quickly configured to upload data to the system 1700 without requiring a user (such as a patient or caregiver) to manually set up the medical device to communicate with the system 1700.

Information can be provided to, or received from, a user (such as a patient or healthcare worker) (1615). Information can be provided or received through a user interface of the medical device 1750, user interface 1790 of the system 1700, or user interface of another device operating in conjunction with the present invention. In one exemplary embodiment of the present invention, the user interface 1790 may provide information to a user such as an indicator as to whether a medical device is currently in communication with the system, an indicator that the system has received medical data from a medical device, a survey regarding a treatment for a patient, and/or an indicator regarding the status of an update to a software application operating on a medical device. Any other suitable information can also be provided to a user. A system operating in conjunction with the present invention may also receive any suitable information from a user, including information regarding a treatment for a patient, an indicator that a patient is in need of assistance, and/or a communication from a patient for delivery to a caregiver of the patient.

In the exemplary method 1600, data is received from one or more medical devices (1620). The data can be received by any suitable system or device, such as through the device interface 242, 1242, or 1742 of a medical data interchange device 200,

medical data translator 1200, or medical data collection and transmission system 1700, respectively. The received data may include any suitable information for one or more patients, including a location for a patient, a patient identifier (such as the patient's name or a number associated with the patient), a health status indicator (e.g., an indicator that the patient's medical data is within or outside ordinary levels, the patient needs help, the patient is having a health emergency, the patient needs to take one or more medications, and/or the patient is outside a predetermined boundary), biological information for a patient, biometric information for a patient, behavioral information for a patient, and/or any other suitable information, including the environmental information and diagnostic data for a medical device discussed previously.

Data may be received from a plurality of medical devices. Each of a plurality of medical devices can be associated with a single respective patient, or each medical device can provide data regarding a plurality of patients. Data may be received from one or more medical devices in any desired manner. For example, the data interface 1742 of system 1700 may receive data from any type of wired or wireless connection, including those described above in conjunction with the adapter 240, device interface 242, and device interface 1242.

A message including at least a portion of the medical device data is transmitted to a medical data server (1625). A transmission method may be selected according to any suitable criteria, including those described above for steps 160 and 1160. The message can be transmitted to a medical data server and/or to an intermediary device configured to (e.g., using a software program) retransmit the message to the medical data server. Medical data servers and intermediary devices operating in conjunction with the present invention are described in detail above. The message can be transmitted to a medical data server and/or intermediary device in any suitable manner, such as through the data relay transceiver 230 or 1230 of a medical data interchange device 200 or medical data translator 1200, respectively. Additionally, the message can be transmitted through a wired or wireless connection using the data relay interface 1730 of the system 1700. The message may include some or all of the data received from one or more medical devices. Part or all of the message may be encrypted using, for example, the encryption mechanisms described above.

A request for an update may be transmitted to a medical data server or other system or device (1630). The update request may include any suitable information, including an identifier for a medical device to be updated and/or a current software or firmware version for the medical device. The update request may also be used to obtain an update for the system 1700 itself, as well as any other device that communicates with the system 1700 through the device interface 1742 or data relay interface 1730. The update request can be transmitted through any wired or wireless connection, including those described previously.

In method 1600, a command is received from a medical data server. The command can be transmitted by a medical data server in response to input from a user of the medical data server or a device in communication with the medical data server (e.g., system 1700), such as a request for an update (step 1630 above). The command may be provided for any purpose, including those described above in conjunction with steps 160 and 1160 above. In one exemplary embodiment, a command from the medical data server can be used to reconfigure a software application running on the system 1700, control one or more medical devices 1750, and/or reconfigure a software application on a medical device 1750.

Exemplary System for Medical Data Collection and Transmission

Any of the systems and devices depicted in FIGS. 2A-8 and FIGS. 11-15 can be used to collect and transmit medical data according to various aspects of the present invention, such as the method depicted in FIG. 16.

Additionally, an exemplary system for medical data collection and transmission is depicted in FIG. 17. In this exemplary embodiment, system 1700 includes a processor 1710 in communication with a memory 1720. A data relay interface 1730 communicates with one or more medical device servers 1770 (directly or through one or more intermediary devices 1760) through a wired and/or wireless protocol. A device interface 1742 communicates with one or more medical devices 1750. The device interface 1742 also communicates with any number of other external devices, such as a computer system 1780. The device interface 1742 may support any number of wired or wireless connections, including those described above for device interfaces 242 and 1242.

In one exemplary embodiment, the processor 1710 executes software instructions stored in the memory 1720 of system 1700 to perform the steps of the method in FIG. 16. The device interface 1742 communicates with one or more medical devices 1750 while the data relay interface communicates with one or more intermediary devices 1760 and/or medical data servers 1770. In another exemplary embodiment, the steps of the method in FIG. 16 can be performed by software operating on a medical data interchange device 200 and/or medical data translator 1200.

The system 1700 may include any number and type of processor 1710 and memory 1720, including the processors and memories described above for components 210, 1210, 220, and 1220 above. Medical devices 1750 may include any type of medical device, including the devices described above for medical devices 250 and 1250. A medical device 1750 may communicate with the device interface 1742 in any desired manner, including the wired and wireless communication protocols described above for medical devices 250 and 1250 above.

The data relay interface 1730 communicates with one or more intermediary devices 1760 and/or medical data servers 1770. The intermediary devices 1760 and medical data servers 1770 may include any of the features and functionality described above for intermediary devices 260 and 1260, and medical data servers 270 and 1270, respectively. The data relay interface 1730 may communicate through a wired and/or wireless connection, including any of the wired and wireless connections described above.

A medical data server operating in conjunction with the present invention may include a memory storage device and a processor. The medical data server may include any number and type of processors to retrieve and execute instructions stored in the memory storage device of the medical data server to control its functionality. Any number and type of conventional computer, computer system, computer network, computer workstation, minicomputer, mainframe computer, or computer processor, such as an integrated circuit microprocessor or microcontroller in accordance with the present invention.

The message can be transmitted to, and received by, the medical data server or intermediary device in any suitable manner, including through a wired connection, such as a telephone line, fiber optic cable, and/or coaxial cable. The message may also be transmitted wirelessly using any suitable wireless system, such as a wireless mobile telephony network, General Packet Radio Service (GPRS) network, wireless Local Area Network (WLAN), Global System for

Mobile Communications (GSM) network, Personal Communication Service (PCS) network, Advanced Mobile Phone System (AMPS) network, and/or a satellite communication network. The message may also be transmitted using any suitable combination of multiple wired and wireless communication methods. The transmission method selected to transmit the data to the medical data server can be chosen according to any desired criteria. For example, one or more transmission methods can be selected from a plurality of possible transmission methods to send the data based on each method's cost, time required to transmit, reliability, security, or any other suitable factor. The message may be received in any other manner, such as by an interactive voice response (IVR) system, a mobile computing device, a mobile telecommunication device, a computer system connected to a network, and/or a human operator.

An intermediary device 1760 or medical data server 1770 operating in conjunction with the present invention may include any combination of different memory storage devices, such as hard drives, random access memory (RAM), read only memory (ROM), FLASH memory, or any other type of volatile and/or nonvolatile memory. A medical data server or intermediary device may include an operating system (e.g., Windows NT, 95/98/2000/XP/Vista, OS2, UNIX, Linux, Solaris, MacOS, etc.) as well as various conventional support software and drivers typically associated with computers. Software applications stored in the memory may be entirely or partially served or executed by the processor(s) in performing methods or processes of the present invention.

The medical data server 1770 or intermediary device 1760 may also include a user interface for receiving and providing data to one or more users (such as a doctor, nurse, or patient). The user interface may include any number of input devices such as a keyboard, mouse, touch pad, touch screen, alphanumeric keypad, voice recognition system, or other input device to allow a user or patient to provide instructions and information to the medical data server. Similarly, the user interface may include any number of suitable output devices, such as a monitor, speaker, printer, or other device for providing information to one or more users.

The device interface 1742 communicates with, and receives data directly or indirectly from, one or more medical devices through wired and/or wireless connections, including those previously described. In one embodiment, the device interface 1742 includes an RJ11 connector for connecting to a telephone line. The device interface 1742 can communicate with different medical devices 1750 (or devices relaying/transmitting medical device data) through different connections to allow medical device data to be quickly and efficiently collected by the system 1700. The device interface 1742 can also communicate with other devices, such as one or more computer systems 1780. The system 1700 can track the status of multiple medical devices it is in communication with, and report this information in a message transmitted to a medical data server 1770. The medical data server 1770 can, in turn, provide a command to the system 1700 to configure one or more medical devices according to the specific requirements for one or more patients.

In one exemplary embodiment, the device interface 1742 delivers software and/or firmware updates to medical devices 1750 and/or computer systems 1780 in communication with system 1700. The system 1700 can receive such updates and store them in the memory 1720 (or other storage device in communication with the system 1700) until the appropriate device(s) is in communication with the system 1700 to receive the update. The device interface 1742 may communicate with a device through any of the wired or wireless

connections described above for device interface **242**, **1242**, and adapter **240** or **1240**. Additionally, the device interface **1742** may communicate with a medical device **1750** or other device through a docking connection. A docking connection operating in conjunction with the present invention may be used to supply power to the medical device (e.g., to recharge its battery), establish data and user-interface connections, or provide any other desired function. In one exemplary embodiment, the docking connection is a 30-pin interface configured to connect with a mobile device (e.g., IPOD, IPHONE, IPAD, and other devices). Any other type of docking connection may also be used in conjunction with the present invention.

In one exemplary embodiment, the device interface **1742** includes an interface for communicating with a flash memory card, such as a SECURE DIGITAL (SD) memory card. The SD card can be used to upload information (including software or firmware updates for the system **1700** or a medical device **1750**), as well as to store data (including data from one or more medical devices **1750**). Similarly, the device interface **1742** may also be configured to load data from, and store data to, a portable hard drive or other storage device through a Universal Serial Bus (USB) connection or other suitable connection. Among other things, this allows a nurse or other healthcare provider to load data from one or more systems **1700** and generate reports based on the medical data for one or more patients.

Information can be provided to, or received from, a user (such as a patient or healthcare worker) through the user interface **1790**, which may include any number and type of input devices **1792** and/or output devices **1794**, including any of the input and output devices described previously. In one embodiment, the user interface **1790** includes one or more lights and/or a display to convey information to a user, such as an indicator as to whether a medical device is in communication with (e.g., secured in a docking port of the device interface **1742**) the system **1700**, and/or an indicator that a command (e.g., including a software update) is waiting for retrieval by a medical device and/or user.

A plurality of medical interchange devices **200** (receiving medical data through wired connections), medical data translators **1200** (receiving medical data through wireless connections), and medical data collection and transmission systems **1700** can be used (e.g., either stand-alone or networked together) in a healthcare-related facility, such as a hospital or nursing home, to retrieve data from multiple medical devices and from multiple patients to help monitor groups of patients. Among other things, the present invention allows a patient to upload his or her data from a medical device with little or no action required by the patient. This simplifies the collection of medical data and allows for health care providers to deliver treatments to patients more quickly and efficiently.

The particular implementations shown and described above are illustrative of the invention and its best mode and are not intended to otherwise limit the scope of the present invention in any way. Indeed, for the sake of brevity, conventional data storage, data transmission, and other functional aspects of the systems may not be described in detail. Methods illustrated in the various figures may include more, fewer, or other steps. Additionally, steps may be performed in any suitable order without departing from the scope of the invention. Furthermore, the connecting lines shown in the various figures are intended to represent exemplary functional relationships and/or physical couplings between the various elements. Many alternative or additional functional relationships or physical connections may be present in a practical system.

Changes and modifications may be made to the disclosed embodiments without departing from the scope of the present invention. These and other changes or modifications are intended to be included within the scope of the present invention, as expressed in the following claims.

What is claimed is:

1. A method comprising:

automatically detecting, by a medical data interchange device, a wireless signal from one or more of the plurality of medical devices, wherein the medical data interchange device includes a medical device interface configured to receive data via a wireless connection from a plurality of medical devices, and wherein the signal is received via a medical device interface;

transitioning the medical data interchange device from a quiescent state to an active state in response to the signal to prepare the medical data interchange device to receive data from the plurality of medical devices;

broadcasting, by the medical data interchange device, an authorization code stored in the medical data interchange device in response to a request for authorization, the authorization code for authenticating the medical data interchange device by one or more of the plurality of medical devices;

in response to the detected wireless signal, automatically configuring the medical device interface to communicate using a frequency used by the one or more of the plurality of medical devices and a communication protocol used by the one or more of the plurality of medical devices;

receiving data from the plurality of medical devices via the medical device interface;

transmitting a message including at least a portion of the received data to a medical data server;

receiving a command from the medical data server, wherein the command is appropriate to a class of medical devices of the plurality of medical devices, and wherein the command is for updating a software application on the class of medical devices; and

automatically downloading a software update, based on the command, to one or more of the class of medical devices.

2. The method of claim 1, wherein the data from the plurality of medical devices corresponds to medical data for a plurality of patients.

3. The method of claim 1, wherein the received data includes one or more of:

biological information for a patient;

biometric information for a patient; and

behavioral information for a patient.

4. The method of claim 1, wherein the message is encrypted.

5. The method of claim 1, wherein the data is received through a wireless connection using a protocol selected from the group consisting of a Zigbee protocol, a Wibree protocol, an IEEE 802.11 protocol, an IEEE 802.15 protocol, an IEEE 802.16 protocol, an Ultra-Wideband (UWB) protocol, an Infrared Data Association (IrDA) protocol, a Bluetooth protocol, and combinations thereof.

6. The method of claim 1, wherein the data includes an environmental parameter, wherein the environmental parameter includes at least one of a battery charge level, a temperature, a barometric pressure, a code relating to an accessory for a medical device, a data validity measurement, an elapsed time since a previous reading by the medical device, a test result parameter, a signal-to-noise parameter, and a quality of service (QoS) parameter.

57

7. The method of claim 1, wherein the message is transmitted through a wireless network selected from the group consisting of:

- a cellular network;
- a General Packet Radio Service (GPRS) network;
- a wireless Local Area Network (WLAN);
- a Global System for Mobile Communications (GSM) network;
- a Personal Communication Service (PCS) network;
- an Advanced Mobile Phone System (AMPS) network;
- a satellite communication network; and
- combinations thereof.

8. The method of claim 1, wherein the message is transmitted through a wired connection selected from the group consisting of:

- a universal serial bus (USB) connection;
- a serial connection;
- a telephone connection;
- a parallel connection;
- a Firewire connection;
- an Ethernet connection; and
- combinations thereof.

9. The method of claim 1, further comprising transmitting the message to an intermediary device, wherein the intermediary device is configured to retransmit at least a portion of the message to the medical data server.

10. The method of claim 1, wherein the command is provided by the medical data server in response to input from a user.

58

11. The method of claim 1, wherein the command reconfigures a software application running on a system receiving the medical data and transmitting the message.

12. The method of claim 1, further comprising automatically configuring a medical device of the plurality of medical devices, wherein configuring the medical device is based on information for one or more patients.

13. The method of claim 1, further comprising authenticating the plurality of medical devices before receiving data from the plurality of medical devices.

14. The method of claim 1, further comprising providing information to, and receiving information from, a patient through a user interface, wherein the information provided to the patient includes one or more of:

- an indicator as to whether a medical device is currently in communication with a system coupled to the user interface;
- an indicator that medical data has been received from the medical device;
- a survey regarding a treatment for the patient; and
- an indicator regarding the status of an update to a software application operating on a medical device.

15. The method of claim 14, wherein the information received from a patient includes one or more of:

- information regarding a treatment for the patient;
- an indicator that the patient is in need of assistance; and
- a communication from the patient for delivery to a caregiver of the patient.

* * * * *

专利名称(译)	医疗数据收集和传输的方法		
公开(公告)号	US8131564	公开(公告)日	2012-03-06
申请号	US12/938187	申请日	2010-11-02
[标]申请(专利权)人(译)	DICKS KENT KENT RALPH 特里普ROBERT 巴特利特TERRY 克罗斯利THOMAS		
申请(专利权)人(译)	DICKS KENT KENT RALPH 特里普ROBERT 巴特利特TERRY 克罗斯利THOMAS		
当前申请(专利权)人(译)	MEDAPPS INC.		
[标]发明人	DICKS KENT KENT RALPH TRIPP ROBERT BARTLETT TERRY CROSLEY THOMAS		
发明人	DICKS, KENT KENT, RALPH TRIPP, ROBERT BARTLETT, TERRY CROSLEY, THOMAS		
IPC分类号	G06F3/00 G06Q50/00 A61B5/00		
CPC分类号	A61B5/0022 A61B5/1112 G06F19/3418 G06Q50/22 G06Q50/24 A61B2560/045 G06F19/3406 G06F19/345 G06F19/3456 A61B2505/07 A61B2560/0209 A61B2560/0431 G16H40/63 G16H40/67 G16H50/20		
优先权	60/862743 2006-10-24 US		
其他公开文献	US20110093283A1		
外部链接	Espacenet USPTO		

摘要(译)

根据本发明的各个方面的示例性方法包括从医疗设备接收数据并将包括所接收的数据的至少一部分的消息发送到所提供的医疗数据服务器。该示例性方法还包括从医疗数据服务器接收命令。

