



(19) **United States**

(12) **Patent Application Publication**  
**Okerlund et al.**

(10) **Pub. No.: US 2003/0187358 A1**

(43) **Pub. Date: Oct. 2, 2003**

(54) **METHOD, SYSTEM AND COMPUTER  
PRODUCT FOR CARDIAC  
INTERVENTIONAL PROCEDURE  
PLANNING**

**Publication Classification**

(51) **Int. Cl.<sup>7</sup> ..... A61B 8/00**

(52) **U.S. Cl. .... 600/443; 128/916**

(76) **Inventors: Darin R. Okerlund, Muskego, WI  
(US); Hui David He, Brookfield, WI  
(US); Jerome Knoplioch, Neuilly Sur  
Seine (FR); Jasbir S. Sra, Pewaukee,  
WI (US); Mark E. Woodford,  
Waukesha, WI (US)**


(57) **ABSTRACT**

A method of creating 3D models to be used for cardiac interventional procedure planning. Acquisition data is obtained from a medical imaging system and cardiac image data is created in response to the acquisition data. A 3D model is created in response to the cardiac image data and three anatomical landmarks are identified on the 3D model. The 3D model is sent to an interventional system where the 3D model is in a format that can be imported and registered with the interventional system.

Correspondence Address:  
**CANTOR COLBURN, LLP  
55 GRIFFIN ROAD SOUTH  
BLOOMFIELD, CT 06002**

(21) **Appl. No.: 10/063,064**

(22) **Filed: Mar. 15, 2002**

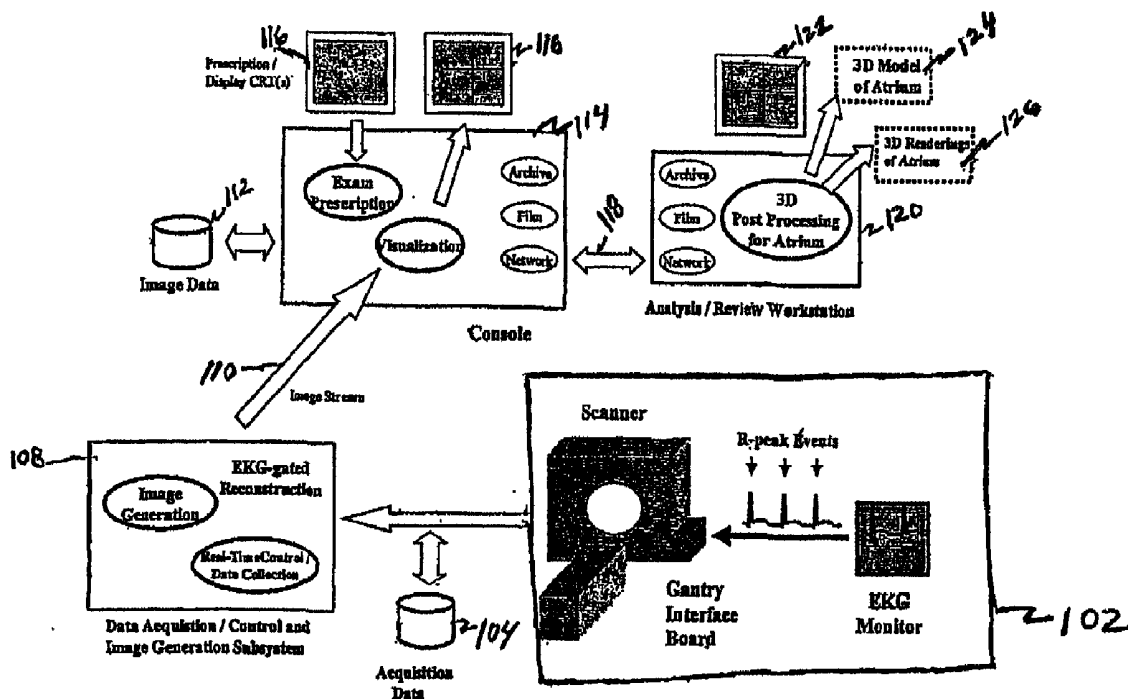

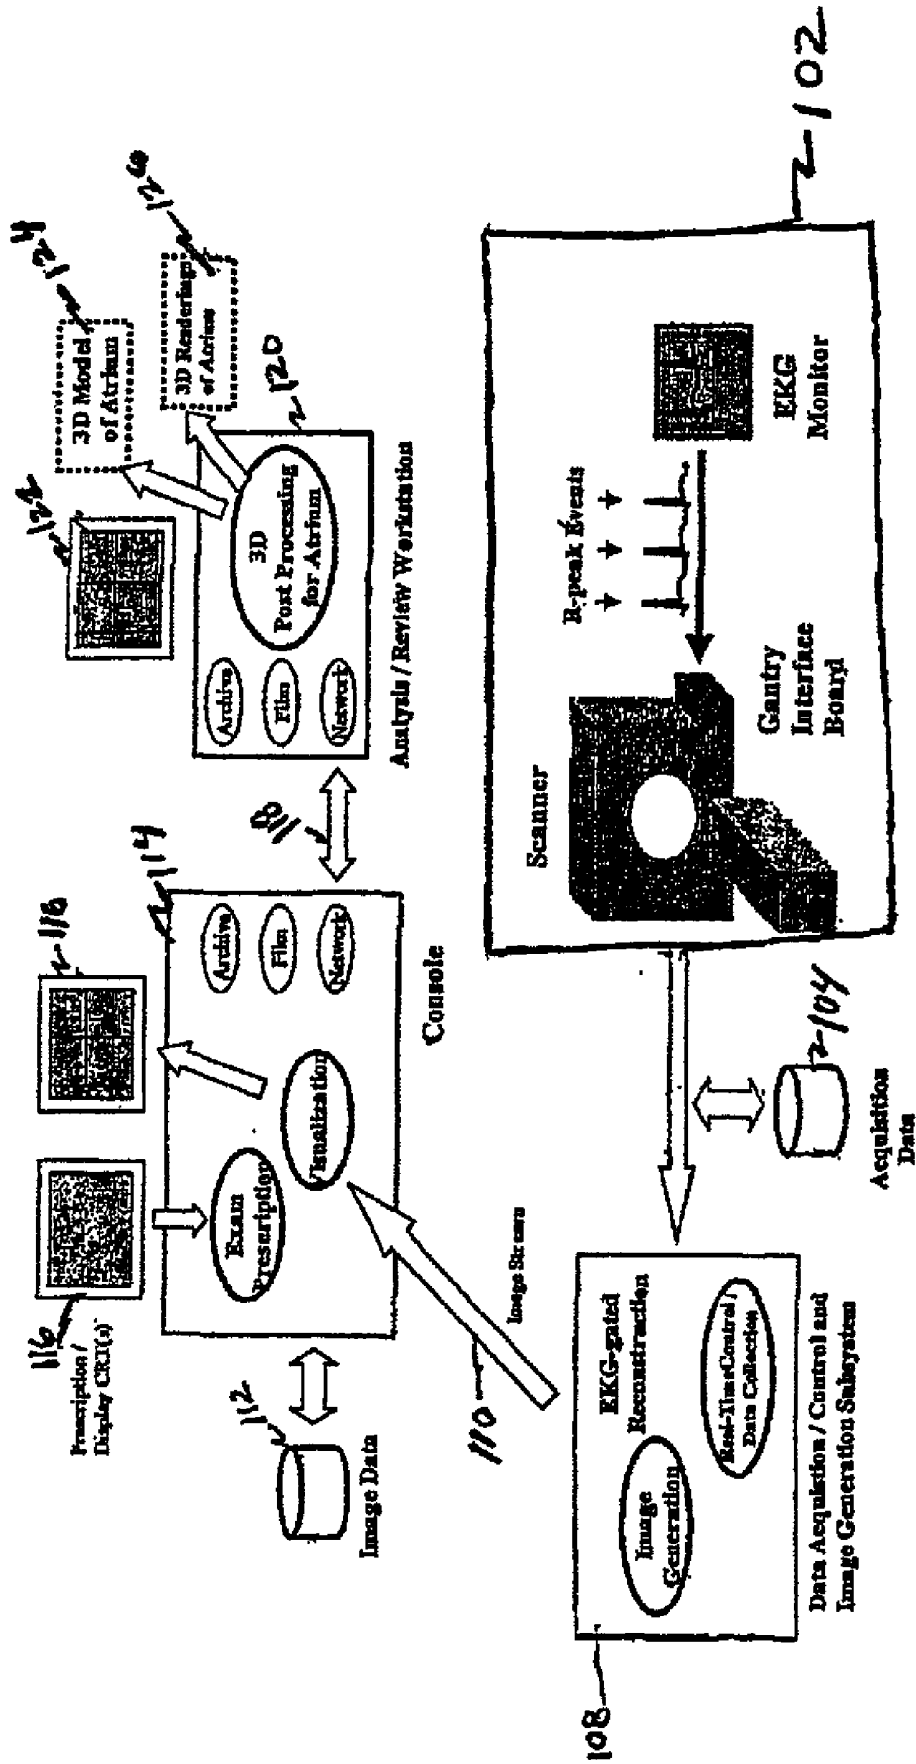


FIG. 1

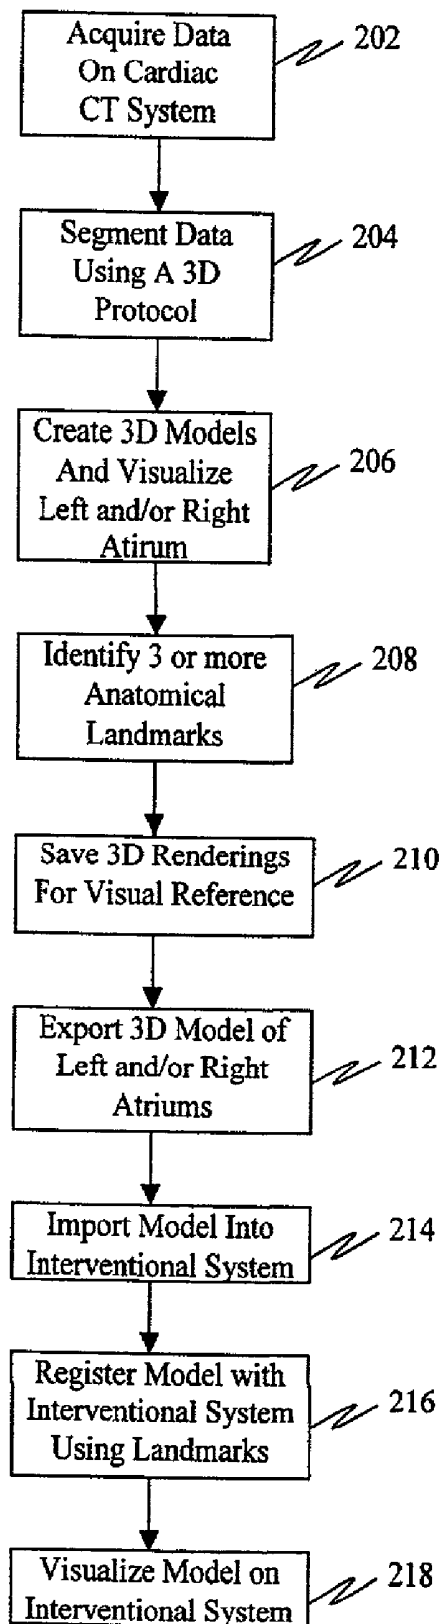


FIG.2

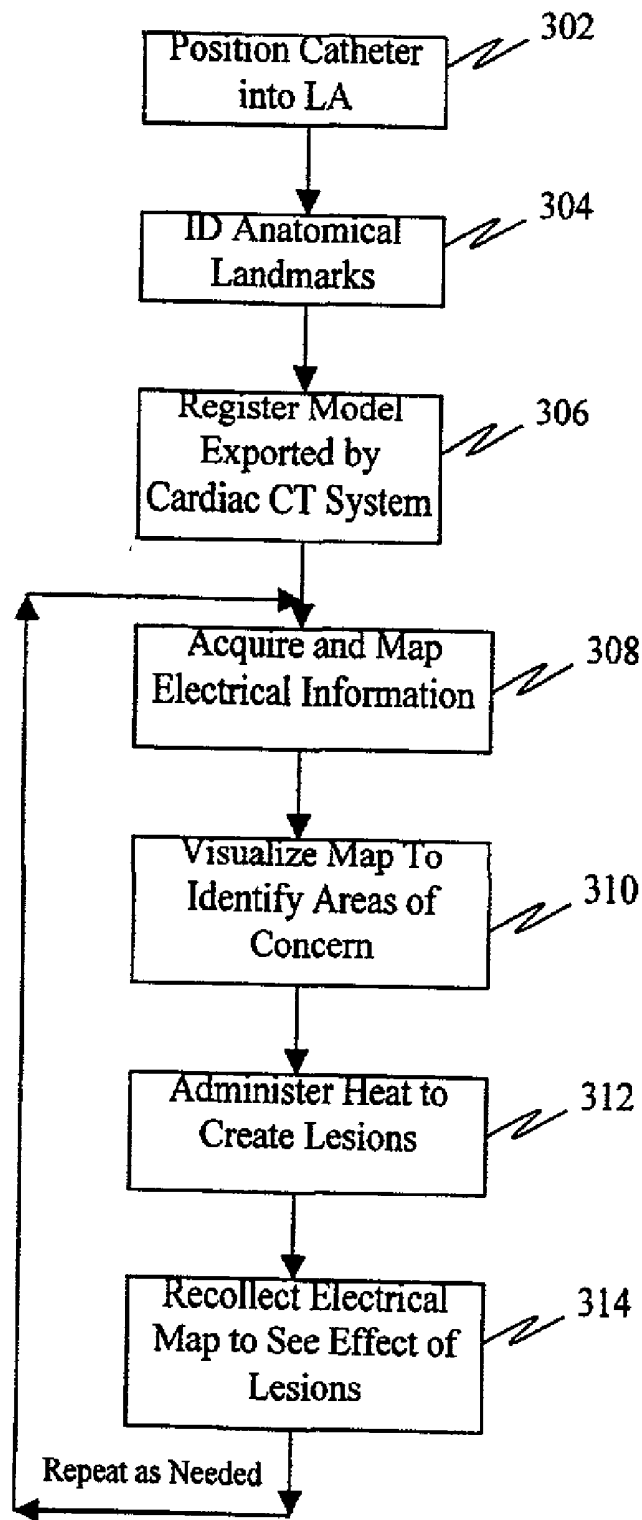


FIG.3

## METHOD, SYSTEM AND COMPUTER PRODUCT FOR CARDIAC INTERVENTIONAL PROCEDURE PLANNING

### BACKGROUND OF INVENTION

[0001] The present disclosure relates generally to a method for the planning of cardiac interventional procedures and in particular, to a method for using data created by a medical imaging system in cardiac interventional procedure planning.

[0002] Medical diagnostic and imaging systems are ubiquitous in modern health care facilities. Such systems provide invaluable tools for identifying, diagnosing and treating physical conditions and greatly reduce the need for surgical diagnostic intervention. In many instances, final diagnosis and treatment proceed only after an attending physician or radiologist has complemented conventional examinations with detailed images of relevant areas and tissues via one or more imaging modalities.

[0003] Currently, a number of modalities exist for medical diagnostic and imaging systems. These include computed tomography (CT) systems, x-ray systems (including both conventional and digital or digitized imaging systems), magnetic resonance (MR) systems, positron emission tomography (PET) systems, ultrasound systems and nuclear medicine systems. In many instances, these modalities complement one another and offer the physician a range of techniques for imaging particular types of tissue, organs, physiological systems, and so forth. Health care institutions often dispose of several such imaging systems at a single or multiple facilities, permitting its physicians to draw upon such resources as required particular patient needs.

[0004] Modern medical diagnostic systems typically include circuitry for acquiring image data and for transforming the data into a useable form which is then processed to create a reconstructed image of features of interest within the patient. The image data acquisition and processing circuitry is often referred to as a "scanner" regardless of the modality, because some sort of physical or electronic scanning often occurs in the imaging process. The particular components of the system and related circuitry, of course, differ greatly between modalities due to their different physics and data processing requirements.

[0005] Medical diagnosis and treatment can also be performed by using an interventional procedure such as atrial fibrillation (AF) intervention. Approximately 2.2 million people in the United States have AF. It is the most common arrhythmia and is the most troublesome. It is currently the number one independent cause of stroke in the United States. The incidences of AF increase with age, rapidly increasing after the age of sixty. In the case of left atrial fibrillation, muscle tissues around any of the four pulmonary veins (PV) which connect to the left atrium (LA) can sometimes generate an extra electrical signal causing AF. One current clinical treatment for this condition is ablation using a special catheter which is positioned into the left atrium to create small lesions by administering heat near the origin of the problematic electrical signal. Ablation therapy is done routinely during open heart surgery in less than one hour, but it is very difficult and timely using the less invasive catheter procedure.

[0006] In the example of ablation therapy, the following procedure is typical. First, a catheter is position into the LA, guided by X-ray fluoro, this takes approximately one hour. Next, a crude 3D geometric representation of the LA and PV ostiums (openings) is acquired using 3D positioning information from a special catheter by attempting to "sweep through" the space of the LA. Acquiring a crude 3D geometric representation typically takes about one hour. The next steps are performed in the following order as many times as necessary. A special catheter is used to acquire electrical information from one or more heart cycles and this electrical information is mapped onto the crude 3D geometric representation using interventional system software. The next step is to visualize this map in order to identify the areas of concern which should be treated with ablation. Heat is then administered to create lesions, as the software keeps track of these locations. The last step is to recollect the electrical map to see the effects of the lesions. If necessary to complete the ablation therapy, the process continues with repeating the previous steps starting with using a special catheter to acquire electrical information. The ablation therapy procedure is lengthy and labor intensive.

### SUMMARY OF INVENTION

[0007] One aspect of the invention is a method of creating 3D models to be used for cardiac interventional procedure planning. Acquisition data is obtained from a medical imaging system and cardiac image data is created in response to the acquisition data. A 3D model is created in response to the cardiac image data and three anatomical landmarks are identified on the 3D model. The 3D model is sent to an interventional system where the 3D model is in a format that can be imported and registered with the interventional system.

[0008] Another aspect of the invention is a method for creating 3D models to be used for cardiac interventional procedure planning. Acquisition data is received from a medical imaging system. Cardiac image data is created in response to the acquisition data and a 3D model is created in response to the cardiac image data. Three anatomical landmarks are identified on the 3D model. The 3D model is registered on the interventional system in response to the three anatomical landmarks and the 3D model is visualized on the interventional system.

[0009] A further aspect of the invention is a system for creating 3D models to be used for cardiac interventional procedure planning. The system comprises a medical imaging system, an acquisition database in communication with the medical imaging system, an image database, a data, transfer mechanism and a processing device. The processing device is in communication with the data transfer mechanism, the acquisition database and the image database. The processing device includes instructions to create 3D models to be used for cardiac interventional procedure planning. The instructions carry out a method to obtain acquisition data from the medical imaging system where the acquisition data is stored in the acquisition database. Cardiac image data is created in response to the acquisition data where the cardiac image data is stored in the image database. A 3D model is created in response to the cardiac image data and three anatomical landmarks are identified on the 3D model. The 3D model is sent to an interventional system, where the 3D model is in a format that can be registered and imported

into the interventional system. The sending is performed using the data transfer mechanism.

[0010] Another aspect of the invention is a system for creating 3D models to be used for cardiac interventional procedure planning. The system comprises a medical imaging system, an acquisition database in communication with the medical imaging system, an image database, a data transfer mechanism, an interventional system in communication with the data transfer mechanism and a processing device. The processing device is in communication with the data transfer mechanism, the acquisition database and the image database. The processing device includes instructions to create 3D models to be used for cardiac interventional procedure planning. The instructions carry out a method to obtain acquisition data from the medical imaging system where the acquisition data is stored in the acquisition database. Cardiac image data is created in response to the acquisition data where the cardiac image data is stored in the image database. A 3D model is created in response to the cardiac image data and three anatomical landmarks are identified on the 3D model. The 3D model is sent to an interventional system, where the 3D model is in a format that can be registered and imported into the interventional system. The sending is performed using the data transfer mechanism. The 3D model is received at the interventional system and registered in response to the three anatomical landmarks. The 3D model is visualized on the interventional system.

[0011] Another aspect of the invention is a computer program product for creating 3D models to be used for cardiac interventional procedure planning. The product includes a storage medium that is readable by a processing circuit and stores instructions for execution by the processing circuit. The instructions for execution include obtaining acquisition data from a medical imaging system and creating cardiac image data in response to the acquisition data. A 3D model is created in response to the cardiac image data and three anatomical landmarks are identified on the 3D model. The 3D model is sent to an interventional system where the 3D model is in a format that can be imported and registered with the interventional system.

[0012] Further aspects of the invention are disclosed herein. The above discussed and other features and advantages of the present invention will be appreciated and understood by those skilled in the art from the following detailed description and drawings.

#### BRIEF DESCRIPTION OF DRAWINGS

[0013] Referring to the exemplary drawings wherein like elements are numbered alike in the several Figures:

[0014] FIG. 1 is an overview of a cardiac computed tomography (CT) system with support for cardiac imaging;

[0015] FIG. 2 is a flow diagram of a process where image data created on a cardiac CT is used by an interventional planning system; and

[0016] FIG. 3 is a flow diagram of a revised process for performing an interventional procedure.

#### DETAILED DESCRIPTION

[0017] FIG. 1 is an overview of an exemplary cardiac computed tomography (CT) system with support for cardiac

imaging. The cardiac CT system is used as an example; other imaging systems known in the art can also be used in an embodiment of the present invention. The scanner portion of the system 102 includes an EKG monitor that outputs Revents into the scanner through a scanner interface board. The scanner interface board can be used to couple the EKG system to the scanner. An example of a scanner interface board is a Gantry interface board. The cardiac CT subsystem 102 includes EKG gated acquisition or image reconstruction capabilities to image the heart free of motion in its diastolic phase. Data is output from the scanner into a subsystem 108 that includes software to perform data acquisition, data control and image generation. In addition, data that is output from the scanner, including R-peak time stamps, is stored in the acquisition database 104. Acquisition is performed according to one or more acquisition protocols that are optimized for imaging the heart and specifically the left and/or right atrium. Image generation is performed using one or more optimized 3D protocols for automated image segmentation of the CT image dataset for the inner surface of the left and/or right atrium.

[0018] Referring to FIG. 1, the image data stream 110 is sent to the operator console 114. The data used by software at the operator console 114 for exam prescription and visualization is stored in an image database 112 along with the data from the image data stream 110. Display screens 116 are provided to the operator of the exam prescription and visualization process. The image data may be archived, put on film or sent over a network to a workstation 120 for analysis and review including 3D post processing. The post processing software depicted in the workstation 120 provides immersible views of the atriums (or ventricle chambers), such that the pulmonary veins can be visualized from the inside of the left atrium, for example. These special views can be saved into a 3D rendering of atrium file 126 and viewed by the interventionalist during the intervention procedure. The post processing software also provides for the export of detailed 3D models 124 of the left and/or right atriums inner surfaces. In the case of the left atrium, the four pulmonary veins are clearly defined in 3D models 124. The 3D models 124 include anatomical landmarks that can be used for 3D registration with the coordinate system of the interventional or therapeutic system. The 3D models 124 can be in exported in one of several formats: a wire mesh geometric model; a set of contours; a segmented volume of binary images; or a DICOM object using the radiation therapy (RT) DICOM object standard or similar object. Other formats known in the art can also be used to store and export the 3D models 124. Additionally, the operator can view the 3D models 124 on a display screen 122. In another embodiment, the interventional system could contain the advanced 3D registration and/or visualization software included by an embodiment of this invention.

[0019] FIG. 2 is a flow diagram of an exemplary process where image data created on a cardiac CT is used by an interventional planning system. The process begins at step 202 when a volume of data is acquired on the cardiac CT system using a protocol that is optimized for the left and/or right atrium. An example of a protocol that could be used is a coronary artery imaging protocol that uses a helical scan acquisition technique with gated reconstruction. In an exemplary embodiment, parameters used by the coronary artery imaging protocol could include 0.5 second Gantry periods with 0.375 helical pitch factors using single or multi-sector

cardiac reconstruction. Parameters could also include 120 kilovolts, 250 milliamps, and 1.25 millimeters on a multi-slice CT scanner. At step **204**, the image dataset is segmented using post processing software that includes a 3D protocol designed to extract the inner surface of the left and/or right atrium. In an exemplary embodiment, post processing software functions can include applying advanced vessel analysis, depositing seeds, using connectivity, and performing region growing techniques. These functions can be performed with a purchased software tool (eg., Advanced Vessel Analysis (AVA)). In an exemplary embodiment, after a tool such as AVA is applied to the image dataset, further processing can include: thresholding, floater filtering, scalping, bridging data, and scalping processing. This automated process, at step **204**, of segmenting data using a 3D protocol may require one or more queues from the operator. In an exemplary embodiment when a queue is required from the operator the operator may be stepped through the process. The 3D protocol includes default views of the volume and processing steps that can be performed on the data in order to do the 3D segmentation and exporting.

[**0020**] Next, at step **206**, the 3D model is created. The left and/or right atrium is visualized using 3D surface and/or volume rendering including an immersible view. A variety of volume rendering software packages are available including Volume Rendering (VR) and Cardiac Image Quality (CARDIQ). At step **208**, the operator identifies three or more specific anatomical landmarks to be used for registration with the interventional system. If rigid registration has been used three anatomical landmarks are required. If nonregistration has been used then more than three anatomical landmarks may be required. In the case of the left atrium, the sinus and two superior pulmonary veins could be used. Landmarks can be visualized in a different color scheme than the inner surface of the heart chamber. Alternatively, explicit geometric markers can be inserted into the volume at the landmarks and the chamber can be visualized in a translucent fashion with opaque geometric landmarks. A volume rendering tool such as the one described previously in reference to step **206** can be used to perform this step. In an exemplary embodiment of the invention the operator will be stepped through the visualization and landmark identification.

[**0021**] At step **210**, specific 3D renderings that are requested for visual reference during the interventional planning procedure are saved. The 3D renderings could be saved in a variety of manners including DICOM images, on film or in a multimedia format. These views could also be blended with the projection image on a fluoroscopy system. A fluoroscopy system can include positioning an x-ray tube on one side of a patient and a detector on the other side of the patient in order to get real time x-ray images. A fluoroscopy system is an example of one way to guide a catheter during a procedure.

[**0022**] At step **212**, a 3D model of the left and/or right atrium is exported using a format of choice. Possible formats include: a wire mesh geometric model; a series of contours; a segmented volume of binary images, and a DICOM object such as the RT DICOM object being used by the radiation therapy DICOM standard. In an exemplary embodiment, all non-relevant data in the binary images are set to zero and the segmented volume of binary images includes only the non-zero information. The value of the voxels correspond to

CT attenuation and the density of a tissue expressed in Hounsfield units makes up the segmented volume of binary images.

[**0023**] At step **214**, the 3D model that has been exported is input to the interventional system. Next, at step **216**, the 3D model is registered with the identical landmarks that were identified in step **208**. The 3D model can be registered in the coordinate system of the interventional system using rigid or non-rigid registration techniques. At step **218**, the model is further visualized on the interventional system and electrical systems are mapped onto the model. The exemplary embodiment described above refers to one 3D model, this could be expanded to any number of 3D models being exported by the cardiac imaging system and imported to the interventional system.

[**0024**] In another embodiment, the process described in **FIG. 2** includes an additional step after the interventional procedure has been completed. This step includes importing into the cardiac imaging system both before and after electrical signals calculated by the interventional system to be displayed and archived in a DICOM format. Additionally, the process described in reference to **FIG. 2** is applicable to any chamber (eg., left or right atrium, left or right ventricle) or vessel (eg., right coronary artery, ascending aorta) of the heart. Likewise, the process is applicable to ablation or any other type of interventional procedure that requires planning using renderings or 3D models generated by an image acquisition system. The process depicted in **FIG. 2** is applicable to other image acquisition systems in addition to a cardiac CT system. For example, if the cardiac images are acquired on an magnetic resonance image (MRI) system, step **204** would include using cardiac segmentation algorithms that are optimized for post processing of magnetic resonance (MR) images.

[**0025**] **FIG. 3** is a flow diagram of an exemplary revised process for performing an interventional procedure using an embodiment of the present invention. The revised process for ablation therapy begins at step **302** with positioning the catheter into the left atrium (LA), guided by the x-ray fluoro. This part of the process typically takes about one hour to perform. Next, at step **304**, three or more anatomical landmarks are identified within the atrium using a positioning catheter and the fluoro system in order to define a plane. At step **306**, the interventional system performs a 3D registration of the 3D model exported by the cardiac CT system such that the model is transformed into the interventional system coordinate system. Steps **304** and **306** replace part of the current interventional procedure described in the background section. Acquiring a crude 3D geometric representation using 3D positioning information from a special catheter by attempting to sweep through the space of the LA is no longer required. Using steps **304** and **306** instead of the current method allows the interventional procedure to be completed in less time.

[**0026**] Next, a loop begins that includes steps **308-314**. At step **308**, electrical information is acquired from one or more heart cycles using a special catheter. The electrical information is mapped onto the detailed geometric model of the atrium using interventional system software. Next, at step **310**, the map is visualized to identify the areas of concern that should be treated with ablation. At step **312**, heat is administered to create lesions and the software keeps track

of these locations. The electrical map is recollected at step 314 to see the effects of the lesion. This loop, including steps 3084, is repeated as many times as needed to complete the interventional procedure.

[0027] The cardiac CT system for atrial fibrillation planning provides information for planning of interventional procedures so that the interventionalist can avoid acquiring a crude 3D geometric representation of the LA and PV ostiums using a special catheter and sweeping through the space of the LA as described in the background section. This can result in the overall duration of the interventional procedure being reduced. Additionally, with a more detailed 3D geometric representation of the LA and PV's than that which could be acquired by a special catheter, fewer iterations of delivering the therapy, steps 308-314 in FIG. 3, are required. The increased accuracy of the geometry can allow the interventionalist to identify the origins of the problematic electrical signals more quickly and with more precision.

[0028] Although the preceding embodiments are discussed with respect to medical imaging, it is understood that the image acquisition and processing methodology described herein is not limited to medical applications, but may be utilized in non-medical applications.

[0029] As described above, the embodiments of the invention may be embodied in the form of computer-implemented processes and apparatuses for practicing those processes. Embodiments of the invention may also be embodied in the form of computer program code containing instructions embodied in tangible media, such as floppy diskettes, CD-ROMs, hard drives, or any other computer-readable storage medium, wherein, when the computer program code is loaded into and executed by a computer, the computer becomes an apparatus for practicing the invention. An embodiment of the present invention can also be embodied in the form of computer program code, for example, whether stored in a storage medium, loaded into and/or executed by a computer, or transmitted over some transmission medium, such as over electrical wiring or cabling, through fiber optics, or via electromagnetic radiation, wherein, when the computer program code is loaded into and executed by a computer, the computer becomes an apparatus for practicing the invention. When implemented on a general-purpose microprocessor, the computer program code segments configure the microprocessor to create specific logic circuits.

[0030] While the invention has been described with reference to exemplary embodiments, it will be understood by those skilled in the art that various changes may be made and equivalents may be substituted for elements thereof without departing from the scope of the invention. In addition, many modifications may be made to adapt a particular situation or material to the teachings of the invention without departing from the essential scope thereof. Therefore, it is intended that the invention not be limited to the particular embodiment disclosed as the best mode contemplated for carrying out this invention, but that the invention will include all embodiments falling within the scope of the appended claims. Moreover, the use of the terms first, second, etc. do not denote any order of importance, but rather the terms first, second, etc. are used to distinguish one element from another.

1. A method of creating 3D models to be used for cardiac interventional procedure planning, the method comprising:

obtaining acquisition data from a medical imaging system;

creating cardiac image data in response to said acquisition data;

creating a 3D model in response to said cardiac image data;

identifying three anatomical landmarks on said 3D model; and

sending said 3D model to an interventional system, wherein said 3D model is in a format that can be imported and registered with said interventional system.

2. The method of claim 1 further comprising receiving from said interventional system before and after electrical signals calculated by said interventional system.

3. The method of claim 2 further comprising storing said before and after electrical signals in a DICOM format.

4. The method of claim 1 further comprising:

receiving said 3D model at said interventional system;

registering said 3D model on said interventional system, wherein said registering is performed in response to said three anatomical landmarks; and

visualizing said 3D model on said interventional system.

5. The method of claim 1 further comprising:

creating 3D renderings for visual reference in response to said cardiac image data; and

sending said 3D renderings to said interventional system.

6. The method of claim 5 wherein said 3D renderings are blended with a projection image on a fluoroscopy system.

7. The method of claim 1 wherein:

said creating cardiac image data is performed using a tool to step an operator through said creating cardiac image data;

said creating a 3D model is performed using a tool to step an operator through said creating a 3D model; and

said identifying is performed using a tool to step an operator through said identifying.

8. The method of claim 1 wherein said creating cardiac image data includes:

segmenting said acquisition data using post processing software that includes a 3D protocol and instructions for extracting an inner surface of the area of interest; and

visualizing said area of interest including creating an immersible view.

9. The method of claim 8 wherein said post processing software further includes instructions for applying advanced vessel analysis.

10. The method of claim 8 wherein said post processing software further includes instructions for depositing seeds.

11. The method of claim 8 wherein said post processing software further includes instructions for using connectivity, thresholding and morphological operators.

12. The method of claim 8 wherein said post processing software further includes instructions for performing region growing techniques.

13. The method of claim 8 wherein said visualizing is performed in a translucent fashion with opaque geometric landmarks.

14. The method of claim 1 wherein said medical imaging system is a cardiac computed tomography system.

15. The method of claim 1 wherein said medical imaging system is a magnetic resonance imaging system.

16. The method of claim 1 wherein said 3D model is in a wire mesh geometric model format.

17. The method of claim 1 wherein said 3D model is in a series of contours format.

18. The method of claim 1 wherein said 3D model is in a segmented volume of binary images format.

19. The method of claim 1 wherein said 3D model is in a DICOM object format.

20. The method of claim 1 wherein said interventional system is an atrial fibrillation intervention system.

21. The method of claim 20 wherein said atrial fibrillation intervention system is used to perform ablation therapy.

22. A method of creating 3D models to be used for cardiac interventional procedure planning, the method comprising:

receiving acquisition data from a medical imaging system at an interventional system;

creating cardiac image data in response to said acquisition data;

creating a 3D model in response to said cardiac image data;

identifying three anatomical landmarks on said 3D model; and

registering said 3D model on said interventional system, wherein said registering is performed in response to said three anatomical landmarks; and

visualizing said 3D model on said interventional system.

23. The method of claim 22 further comprising creating 3D renderings for visual reference in response to said cardiac image data.

24. A system for creating 3D models to be used for cardiac interventional procedure planning, the system comprising:

a medical imaging system;

an acquisition database in communication with said medical imaging system;

an image database;

a data transfer mechanism; and

a processing device in communication with said data transfer mechanism, said acquisition database and said image database and including instructions to create 3D models to be used for cardiac interventional procedure planning, the method comprising:

obtaining acquisition data from said medical imaging system, wherein said acquisition data is stored in said acquisition database;

creating cardiac image data in response to said acquisition data, wherein said cardiac image data is stored in said image database;

creating a 3D model in response to said cardiac image data;

identifying three anatomical landmarks on said 3D model; and

sending said 3D model to an interventional system, wherein said 3D model is in a format that can be imported and registered with said interventional system and said sending is performed using said data transfer mechanism.

25. The system of claim 24 wherein said processing device includes instructions to implement a method further comprising receiving from said interventional system before and after electrical signals calculated by said interventional system.

26. The system of claim 24 wherein said processing device includes instructions to implement a method further comprising:

creating 3D renderings for visual reference in response to said cardiac image data; and

sending said 3D renderings to said interventional system.

27. The system of claim 24 wherein said acquisition database is relational.

28. The system of claim 24 wherein said image database is relational.

29. The system of claim 24 wherein said medical imaging system includes:

an EKG;

an interface board receiving R-peak event data from said EKG; and

a scanner in communication with said interface board.

30. The system of claim 24 wherein said data transfer mechanism is a network.

31. The system of claim 30 wherein said network is the Internet.

32. The system of claim 24 wherein said medical imaging system is a cardiac computed tomography system.

33. The system of claim 24 wherein said medical imaging system is a magnetic resonance imaging system.

34. The system of claim 24 wherein said interventional system is an atrial fibrillation intervention system.

35. A system for creating 3D models to be used for cardiac interventional procedure planning, the system comprising:

a medical imaging system;

an acquisition database in communication with said medical imaging system;

an image database;

a data transfer mechanism;

an interventional system in communication with said data transfer mechanism; and

a processing device in communication with said data transfer mechanism, said acquisition database and said image database and including instructions to create 3D models to be used for cardiac interventional procedure planning, the method comprising:

obtaining acquisition data from said medical imaging system, wherein said acquisition data is stored in said acquisition database;

creating cardiac image data in response to said acquisition data, wherein said cardiac image data is stored in said image database;

creating a 3D model in response to said cardiac image data;

identifying three anatomical landmarks on said 3D model;

sending said 3D model to said interventional system, wherein said 3D model is in a format that can be imported and registered with said interventional system and said sending is performed using said data transfer mechanism;

receiving said 3D model at said interventional system;

registering said 3D model on said interventional system, wherein said registering is performed in response to said three anatomical landmarks; and

visualizing said 3D model on said interventional system.

**36.** The system of claim 35 wherein said processing device, said interventional system and said medical imaging system are physically located in the same geographic location.

**37.** The system of claim 35 wherein said processing device, said interventional system and said medical imaging

system are physically located in more than one geographic location and data is transferred using said data transfer mechanism.

**38.** A computer program product for creating 3D models to be used for cardiac interventional procedure planning, the product comprising:

a storage medium readable by a processing circuit and storing instructions for execution by the processing circuit for:

obtaining acquisition data from a medical imaging system;

creating cardiac image data in response to said acquisition data;

creating a 3D model in response to said cardiac image data;

identifying three anatomical landmarks on said 3D model; and

sending said 3D model to an interventional system, wherein said 3D model is in a format that can be imported and registered with said interventional system.

\* \* \* \* \*

专利名称(译)	用于心脏介入手术计划的方法，系统和计算机产品		
公开(公告)号	<a href="#">US20030187358A1</a>	公开(公告)日	2003-10-02
申请号	US10/063064	申请日	2002-03-15
[标]申请(专利权)人(译)	OKERLUND DARINř 何辉DAVID KNOPLIOCH JEROME SRA JASBIR小号 WOODFORD标志着e		
申请(专利权)人(译)	OKERLUND DARIN R. 何辉DAVID KNOPLIOCH JEROME SRA JASBIR S. WOODFORD MARK E.		
当前申请(专利权)人(译)	OKERLUND DARIN R. 何辉DAVID KNOPLIOCH JEROME SRA JASBIR S. WOODFORD MARK E.		
[标]发明人	OKERLUND DARIN R HE HUI DAVID KNOPLIOCH JEROME SRA JASBIR S WOODFORD MARK E		
发明人	OKERLUND, DARIN R. HE, HUI DAVID KNOPLIOCH, JEROME SRA, JASBIR S. WOODFORD, MARK E.		
IPC分类号	A61B5/00 A61B6/00 A61B17/00 A61B19/00 G06F19/00 A61B8/00		
CPC分类号	A61B5/7285 A61B6/503 A61B6/504 A61B6/541 A61B19/50 A61B19/52 Y10S128/922 G06F19/321 G06F19/3437 G06F19/3481 A61B6/027 Y10S128/92 A61B2017/00243 A61B34/10 A61B90/36 G16H20 /00 G16H30/20 G16H30/40 G16H50/50 G16H70/20		
其他公开文献	US7286866		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

一种创建用于心脏介入手术计划的3D模型的方法。从医学成像系统获得采集数据，并且响应于采集数据创建心脏图像数据。响应于心脏图像数据创建3D模型，并且在3D模型上识别三个解剖标志。将3D模型发送到介入系统，其中3D模型的格式可以导入并向介入系统注册。

