



US009420952B2

(12) **United States Patent**
Paquet et al.

(10) **Patent No.:** **US 9,420,952 B2**
(45) **Date of Patent:** **Aug. 23, 2016**

(54) **TEMPERATURE PROBE SUITABLE FOR
AXILLARY READING**

(75) Inventors: **Pierre Paquet**, Quebec (CA); **Binta Diallo**, Quebec (CA); **Mark Raptis**, Valley Center, CA (US)

(73) Assignee: **CareFusion 303, Inc.**, San Diego, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 558 days.

(21) Appl. No.: **12/844,775**

(22) Filed: **Jul. 27, 2010**

(65) **Prior Publication Data**

US 2012/0029310 A1 Feb. 2, 2012

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61B 5/01 (2006.01)

A61B 5/0205 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/0008** (2013.01); **A61B 5/01** (2013.01); **A61B 5/02055** (2013.01); **A61B 5/6813** (2013.01); **A61B 5/6833** (2013.01); **A61B 2562/0271** (2013.01)

(58) **Field of Classification Search**

USPC 600/549, 301
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,677,261 A 7/1972 Day
3,805,769 A 4/1974 Sessions
3,830,224 A * 8/1974 Vanzetti et al. 600/549
3,845,757 A 11/1974 Weyer
4,121,574 A 10/1978 Lester

4,396,020 A 8/1983 Wolff et al.
4,407,295 A * 10/1983 Steuer A61B 5/02438
600/483

4,490,005 A 12/1984 Hovey
4,527,087 A 7/1985 Taya et al.
4,530,366 A 7/1985 Nessi et al.
4,539,996 A 9/1985 Engel
4,541,734 A 9/1985 Ishizaka
4,554,924 A 11/1985 Engel

(Continued)

FOREIGN PATENT DOCUMENTS

EP 1748289 A2 1/2007
JP 61003019 1/1986

(Continued)

OTHER PUBLICATIONS

Akyldiz, I.F. et al.; "Wireless Multimedia Sensor Networks: A survey." IEEE Wireless Communications. Dec. 2007, p. 32-39.

(Continued)


Primary Examiner — Sean Dougherty

(74) *Attorney, Agent, or Firm* — McDermott Will & Emery LLP

(57) **ABSTRACT**

Systems and methods of monitoring the axillary temperature of a person are disclosed. A portion of a temperature probe is provided within the axilla of the person. The temperature probe includes a wiring portion and a body connection portion and a sensing portion between the wiring and body connection portions. The sensing portion comprises a temperature sensing element. The wiring portion is coupled to a monitoring device and comprises a conductor having a first end and a second end, the first end coupled to the temperature sensing element, and the second end connected to the monitoring device. At least a portion of the body connection portion is attached to a second body portion of the person, such that the sensing portion is retained within the axilla.

18 Claims, 17 Drawing Sheets

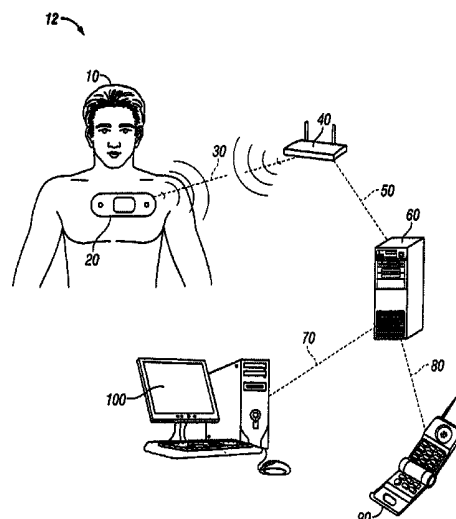

(56)

References Cited

U.S. PATENT DOCUMENTS

4,640,289 A	2/1987	Craighead	
4,686,998 A *	8/1987	Robbins	600/549
4,708,146 A	11/1987	Lane	
4,715,382 A	12/1987	Strand	
4,765,340 A	8/1988	Sakai et al.	
4,771,713 A	9/1988	Kinzenbaw	
4,838,273 A	6/1989	Cartmell	
4,846,185 A	7/1989	Carim	
4,848,353 A	7/1989	Engel	
4,967,765 A	11/1990	Turner et al.	
5,012,810 A	5/1991	Strand et al.	
5,050,612 A *	9/1991	Matsumura	600/483
5,094,545 A *	3/1992	Larsson	G01K 11/06 116/217
5,133,356 A	7/1992	Bryan et al.	
5,153,584 A	10/1992	Engira	
5,215,087 A	6/1993	Anderson et al.	
5,258,577 A	11/1993	Clements	
5,273,036 A	12/1993	Kronberg et al.	
5,285,577 A	2/1994	Carney et al.	
5,344,335 A	9/1994	Scholz et al.	
5,353,793 A *	10/1994	Bornn	600/386
5,401,100 A *	3/1995	Thackston et al.	374/208
5,511,553 A *	4/1996	Segalowitz	600/508
5,544,661 A	8/1996	Davis et al.	
5,803,915 A *	9/1998	Kremenchugsky	A61B 5/01 374/29
5,980,467 A	11/1999	Henry	
6,030,342 A	2/2000	Amano et al.	
6,042,966 A	3/2000	Cheu	
6,090,050 A	7/2000	Constantinides	
6,222,456 B1	4/2001	Tice	
6,270,252 B1	8/2001	Siefert	
6,273,886 B1	8/2001	Edwards et al.	
6,287,252 B1	9/2001	Lugo	
6,324,426 B1	11/2001	Thompson	
6,355,031 B1	3/2002	Edwards et al.	
6,358,245 B1	3/2002	Edwards et al.	
6,416,471 B1	7/2002	Kumar et al.	
6,454,708 B1	9/2002	Ferguson et al.	
6,468,261 B1	10/2002	Small et al.	
6,472,612 B2	10/2002	Fartash et al.	
6,472,614 B1	10/2002	Dupont et al.	
6,494,829 B1 *	12/2002	New et al.	600/300
6,517,497 B2	2/2003	Rymut et al.	
6,636,754 B1	10/2003	Baura et al.	
6,740,049 B2	5/2004	Wallach	
6,740,059 B2	5/2004	Flaherty	
6,950,688 B2	9/2005	Axelgaard et al.	
6,963,772 B2	11/2005	Bloom et al.	
6,980,112 B2	12/2005	Nee	
7,052,472 B1	5/2006	Miller et al.	
7,061,858 B1	6/2006	Di Benedetto et al.	
7,198,600 B2	4/2007	Tamaki et al.	
7,319,895 B2 *	1/2008	Klefstad-Sillonville	A41D 13/1281 600/388
7,355,512 B1	4/2008	Al-Ali	
RE40,470 E	8/2008	Fitzpatrick et al.	
7,434,991 B2	10/2008	Harr et al.	
7,447,526 B2	11/2008	Kim et al.	
7,538,682 B2	5/2009	Trost et al.	
7,542,437 B1	6/2009	Redi et al.	
7,639,352 B2	12/2009	Huber et al.	
7,639,652 B1	12/2009	Amis et al.	
7,645,263 B2	1/2010	Angel et al.	
7,668,588 B2 *	2/2010	Kovacs	600/509
7,924,150 B2	4/2011	Baldus et al.	
7,959,574 B2	6/2011	Bardy	
7,962,188 B2	6/2011	Kiani et al.	
8,007,436 B2 *	8/2011	Katayama	600/301
8,200,320 B2 *	6/2012	Kovacs	600/513
8,226,572 B2	7/2012	Keith et al.	
8,228,188 B2	7/2012	Key et al.	
8,231,542 B2	7/2012	Keith et al.	
8,496,597 B2	7/2013	James et al.	
8,506,480 B2 *	8/2013	Banet et al.	600/301
8,721,562 B2 *	5/2014	Abreu	600/549
2001/0047127 A1 *	11/2001	New et al.	600/300
2002/0007676 A1	1/2002	Ward et al.	
2002/0013538 A1 *	1/2002	Teller	600/549
2002/0045836 A1	4/2002	Alkawwas	
2002/0099277 A1	7/2002	Harry et al.	
2002/0107436 A1	8/2002	Barton et al.	
2002/0109621 A1	8/2002	Khair et al.	
2002/0198519 A1	12/2002	Qin et al.	
2003/0004403 A1	1/2003	Drinan et al.	
2003/0040305 A1	2/2003	Ng et al.	
2003/0069510 A1	4/2003	Semler et al.	
2003/0191445 A1	10/2003	Wallen et al.	
2003/0212319 A1	11/2003	Magill	
2003/0212340 A1	11/2003	Lussier et al.	
2003/0229809 A1	12/2003	Wexler et al.	
2004/0015058 A1	1/2004	Besson et al.	
2004/0030259 A1	2/2004	Dae et al.	
2004/0062133 A1	4/2004	Tsuji	
2004/0073132 A1	4/2004	Maahs et al.	
2004/0116822 A1 *	6/2004	Lindsey	600/549
2004/0165646 A1	8/2004	Shidemantle et al.	
2004/0215098 A1	10/2004	Barton et al.	
2004/0220538 A1 *	11/2004	Panopoulos	A61F 13/42 604/361
2004/0236188 A1	11/2004	Hutchinson et al.	
2005/0085706 A1	4/2005	Perrault et al.	
2005/0101843 A1 *	5/2005	Quinn et al.	600/300
2005/0131288 A1	6/2005	Turner et al.	
2005/0159653 A1	7/2005	Lijima et al.	
2005/0195079 A1	9/2005	Cohen	
2005/0228297 A1	10/2005	Banet et al.	
2005/0228299 A1	10/2005	Banet	
2005/0231350 A1	10/2005	Littrell et al.	
2005/0245831 A1	11/2005	Banet	
2005/0245839 A1	11/2005	Stivoric et al.	
2005/0249263 A1 *	11/2005	Yerlikaya et al.	374/209
2005/0251128 A1	11/2005	Amoah	
2005/0280531 A1	12/2005	Fadem et al.	
2006/0009697 A1	1/2006	Banet et al.	
2006/0045165 A1	3/2006	Chan et al.	
2006/0047987 A1	3/2006	Prabhakaran et al.	
2006/0094971 A1	5/2006	Drew	
2006/0098576 A1	5/2006	Brownrigg et al.	
2006/0155183 A1	7/2006	Kroecker et al.	
2006/0202816 A1	9/2006	Crump et al.	
2006/0224349 A1	10/2006	Butterfield	
2006/0276714 A1	12/2006	Holt et al.	
2007/0032706 A1	2/2007	Kamath et al.	
2007/0041424 A1 *	2/2007	Lev et al.	374/163
2007/0099678 A1	5/2007	Kim et al.	
2007/0116089 A1	5/2007	Bisch et al.	
2007/0123756 A1	5/2007	Kitajima et al.	
2007/0129622 A1	6/2007	Bourget et al.	
2007/0135866 A1	6/2007	Baker et al.	
2007/0142715 A1	6/2007	Banet et al.	
2007/0185660 A1	8/2007	Anderson	
2007/0191728 A1	8/2007	Shennib	
2007/0208233 A1 *	9/2007	Kovacs	600/300
2007/0219434 A1 *	9/2007	Abreu	600/301
2007/0225614 A1	9/2007	Naghavi et al.	
2007/0293781 A1	12/2007	Sims et al.	
2008/0042866 A1	2/2008	Morse et al.	
2008/0091090 A1	4/2008	Guillory et al.	
2008/0097178 A1	4/2008	Banet et al.	
2008/0097422 A1	4/2008	Edwards et al.	
2008/0114220 A1	5/2008	Banet et al.	
2008/0119707 A1	5/2008	Stafford	
2008/0143512 A1	6/2008	Wakisaka et al.	
2008/0183054 A1	7/2008	Kroeger et al.	
2008/0200770 A1	8/2008	Hubinette	
2008/0200774 A1	8/2008	Luo	
2008/0208026 A1	8/2008	Noujaim et al.	
2008/0214949 A1	9/2008	Stivoric et al.	
2008/0221399 A1	9/2008	Zhou et al.	
2008/0234600 A1	9/2008	Marsh	
2008/0275327 A1	11/2008	Faarbaek et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

2008/0294065	A1 *	11/2008	Waldhoff et al.	600/549
2008/0305154	A1	12/2008	Yanaki	
2009/0018409	A1 *	1/2009	Banet et al.	600/301
2009/0054737	A1	2/2009	Magar et al.	
2009/0062670	A1	3/2009	Sterling et al.	
2009/0069642	A1	3/2009	Gao et al.	
2009/0076336	A1 *	3/2009	Mazar	A61B 5/0402 600/300
2009/0076340	A1	3/2009	Libbus et al.	
2009/0076341	A1	3/2009	James et al.	
2009/0076342	A1	3/2009	Amurthur et al.	
2009/0076343	A1	3/2009	James et al.	
2009/0076345	A1	3/2009	Manicka et al.	
2009/0076346	A1	3/2009	James et al.	
2009/0076350	A1	3/2009	Bly et al.	
2009/0076363	A1	3/2009	Bly et al.	
2009/0076364	A1	3/2009	Libbus et al.	
2009/0076405	A1	3/2009	Amurthur et al.	
2009/0076559	A1	3/2009	Libbus et al.	
2009/0105549	A1	4/2009	Smith et al.	
2009/0105605	A1 *	4/2009	Abreu	600/549
2009/0131759	A1	5/2009	Sims et al.	
2009/0131774	A1	5/2009	Sweitzer et al.	
2009/0182204	A1	7/2009	Semler et al.	
2009/0203974	A1	8/2009	Hickle	
2009/0209896	A1	8/2009	Selevan	
2009/0227877	A1	9/2009	Tran	
2009/0259139	A1 *	10/2009	Stepien et al.	600/549
2009/0270744	A1	10/2009	Prstojevich et al.	
2009/0271681	A1	10/2009	Piret et al.	
2009/0306536	A1	12/2009	Ranganathan et al.	
2010/0010319	A1	1/2010	Tivig et al.	
2010/0036212	A1	2/2010	Rieth	
2010/0056886	A1	3/2010	Hurtubise et al.	
2010/0056945	A1	3/2010	Holmes	
2010/0056946	A1	3/2010	Holmes	
2010/0056947	A1	3/2010	Holmes	
2010/0081949	A1	4/2010	Derby, Jr.	
2010/0100004	A1	4/2010	van Someren	
2010/0113894	A1	5/2010	Padiy	
2010/0121217	A1 *	5/2010	Padiy	G01K 1/16 600/549
2010/0160745	A1	6/2010	Hills et al.	
2010/0222688	A1	9/2010	Fischell et al.	
2010/0234716	A1 *	9/2010	Engel	A61B 5/02055 600/391
2010/0286607	A1	11/2010	Saltzstein	
2010/0292605	A1 *	11/2010	Grassl	G01K 1/16 600/549
2010/0298656	A1	11/2010	McCombie et al.	
2010/0298895	A1	11/2010	Ghaffari et al.	
2010/0323634	A1	12/2010	Kimura	
2010/0324548	A1	12/2010	Godara et al.	
2011/0004076	A1	1/2011	Janna et al.	
2011/0060252	A1	3/2011	Simonsen et al.	
2011/0066062	A1	3/2011	Banet et al.	
2011/0077497	A1	3/2011	Oster et al.	
2011/0144470	A1	6/2011	Mazar et al.	
2011/0160601	A1	6/2011	Wang et al.	
2011/0176465	A1	7/2011	Panta et al.	
2011/0182213	A1	7/2011	Forssell et al.	
2011/0224557	A1	9/2011	Banet et al.	
2012/0029300	A1 *	2/2012	Paquet	600/300
2012/0029308	A1 *	2/2012	Paquet	600/301
2012/0029314	A1 *	2/2012	Paquet et al.	600/301
2012/0108920	A1	5/2012	Bly et al.	
2012/0165621	A1 *	6/2012	Grayzel	A61B 5/00 600/301
2012/0238901	A1 *	9/2012	Augustine	G01K 1/165 600/549
2012/0310070	A1	12/2012	Kumar et al.	

FOREIGN PATENT DOCUMENTS

JP	2002-507131	3/2002
JP	2004-503266	2/2004
JP	2005-521453	7/2005
JP	2009-544065	12/2009
KR	20070097725	10/2007
KR	100949150	3/2010
WO	WO90/12606	11/1990

OTHER PUBLICATIONS

Arisha, K. et al. "System-Level Power Optimization for wireless Multimedia Communication." Editors: Ramesh K. and Goodman, D.; Springer US; 2002, p. 21-40.

Cardei, M. et al.; "Improving Wireless Sensor Network Lifetime through Power Aware Organization"; *Wireless Networks* 11, 222-240. 2005.

Davidson, K. G. et al., "Measurement of tidal volume by using transthoracic impedance variations in rats," *J. Appl. Physiol.* 86:759-766, 1999.

Ernst, J.M. et al., "Impedance Penumography: noise as signal in impedance cardiography," *Psychophysiology*, 36 (1999) 333-338.

Freundlich J.J. et al., *Electrical Impedance Pneumography for Simple Nonrestrictive Continuous Monitoring of Respiratory Rate, Rhythm and Tidal Volume for Surgical Patients*, *Chest*, 65, p. 181-184, 1974.

Herman, T. et al.; "A Distributed TDMA Slot Assignment Algorithm for Wireless Sensor Networks"; S. Nikolettseas and J. Rolim (Eds.): *Algosensors 2004*, LNCS 3121, pp. 45-58, 2004, Springer-Verlag Berlin Heidelberg 2004.

Hohlt, B. et al. "Flexible Power Scheduling for Sensor Networks," *IPSN'04*, Apr. 26-27, 2004, Berkeley, California, USA. pp. 1-10.

Kelkar, S. P. et al., "Development of Movement artifact free breathing monitor," *J. Instrum. Soc. India* 38(1) 34-43, 2008.

Lee, W. L.; "Flexible-Schedule-Based TDMA Protocol for Fault-Tolerant and Energy-Efficient Wireless Sensor Networks," *IEEE Transactions on Parallel and Distributed Systems*, vol. 19, No. 6, Jun. 2008; p. 851-864.

Lee, W. L.; "Flexible-Schedule-Based TDMA Protocols for Supporting Fault-Tolerance, On-Demand TDMA Slot Transfer, and Peer-to-Peer Communication in Wireless Sensor Networks," Thesis for the degree of Doctor in Philosophy, University of Western Australia, 2007, p. 1-213.

Loriga, G., et al., "Textile sensing interfaces for cardiopulmonary signs monitoring," *Proceedings of the 2005 IEEE Engineering in Medicine and Biology 27th Annual Conference Shanghai, China*, Sep. 1-4, 2005, p. 7349-7352.

Luo, S. et al., "The electrode system in Impedance-Based Ventilation Measurement," *IEEE Transactions of biomedical Engineering*, vol. 39, No. 11, Nov. 1992, p. 1130-1140.

Matthews, R., et al., "A Wearable Physiological Sensor Suite for Unobtrusive Monitoring of Physiological and Cognitive State," *Proceedings of the 29th Annual International Conference of the IEEE EMBS Cite Internationale, Lyon, France*, Aug. 23-26, 2007, pp. 1-6.

Pacula, A.F. "Impedance Pneumograph, a survey of instrumentation techniques," *Med. & Biol. Engineering*, vol. 4, p. 1-5, 1966.

Pantazis, N.A. et al.; "Energy efficiency in wireless sensor networks using sleep mode TDMA scheduling," *Ad Hoc Networks* 7 (2009) 322-343.

Paradiso, R. et al., "A wearable health care system based on knitted integrated sensors," *IEEE transactions on Information Technology in biomedicine*, vol. 9, No. 3, Sep. 2005, p. 337-344.

Park, et al., "Development of Flexible Self Adhesive Patch for Professional Heat Stress Monitoring Service," *Proceedings of the 2005 IEEE Engineering in Medicine and Biology 27th Annual Conference Shanghai, China*, Sep. 1-4, 2005, pp. 3789-3792.

Rashid, R. A. et al.; "Development of Energy Aware TDMA-Based MAC Protocol for Wireless Sensor Network System," *European Journal of Scientific*, vol. 30 No. 4 (2009), pp. 571-578.

Shaw, G.A. et al., "Warfighter Physiological and Environmental Monitoring: A Study for the U.S. Army Research Institute in Environmental Medicine and the Soldier Systems Center," 2004, Lincoln Laboratory, MIT, pp. 1-141.

(56)

References Cited

OTHER PUBLICATIONS

Zheng, W. W. et al. "Adaptive-frame-based Dynamic Slot Assignment Protocol for Tactical Data Link System," 2009 International Conference of Networks Security, Wireless Communications and Trusted Computing, IEEE, p. 709-714.

Final Office Action, dated Oct. 28, 2012 for U.S. Appl. No. 12/844,771.

Non-Final Office Action, dated Jun. 30, 2014 for U.S. Appl. No. 12/844,796.

Office Actions issued in U.S. Appl. No. 12/844,801, dated Aug. 14, 2014, and U.S. Appl. No. 12/844,794, dated Sep. 26, 2014.

Brown, B.H. et al., "Bipolar and Tetrapolar transfer impedance measurements from volume conductor," *Electronics Letters*, Vol. 35, No. 25, 2000, pp. 2060-2062.

Cooley, W.L. et al. "A new design for an impedance pneumograph," *Journal of Applied Physiology*, vol. 25, No. 4, 1968, pp. 429-432.

Grenvik, A. et al., "Impedance Pneumography," *Chest*, vol. 62, No. 4, Oct. 1972, pp. 439-443.

International Preliminary Report on Patentability in International Application No. PCT/US2011/030088, dated Oct. 27, 2012, 13 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045240, dated Jan. 29, 2013, 6 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045245, dated Jan. 29, 2013, 5 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045249, dated Jan. 29, 2013, 4 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045256, dated Jan. 29, 2013, 4 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045258, dated Jan. 29, 2013, 5 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045337, dated Jan. 9, 2013, 4 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045361, dated Jan. 29, 2013, 6 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045408, dated Jan. 29, 2013, 4 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045414, dated Jan. 29, 2013, 6 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045415, dated Jan. 29, 2013, 4 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045419, dated Jan. 29, 2013, 5 pages.

International Preliminary Report on Patentability in International Application No. PCT/US2011/045425, dated Jan. 29, 2013, 5 pages.

International Search Report and Written Opinion for International Application No. PCT/US2011/045408, dated Feb. 24, 2012, 6 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045361, dated Apr. 6, 2012, 8 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/030088, dated Oct. 31, 2011, 7 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045240, dated Mar. 15, 2012, 8 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045245, dated Mar. 28, 2012, 7 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045249, dated Mar. 12, 2012, 6 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045256, dated Feb. 9, 2012, 12 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045258, dated Apr. 6, 2012, 12 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045337, dated Feb. 9, 2012, 7 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045414, dated Feb. 24, 2012, 9 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045415, dated Feb. 24, 2012, 7 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045419, dated Apr. 6, 2012, 7 pages.

International Search Report and Written Opinion in International Application No. PCT/US2011/045425, dated Apr. 6, 2012, 7 pages.

Kessler, "TCP/IP and tcpdump Pocket reference Guide", Champlain College, 2006.

Murat, B., "Electrical Impedance Plethysmography," *Wiley Encyclopedia of Biomedical Engineering*, 2006, p. 1-10.

Poon, C.S. et al., "Evaluation of two noninvasive techniques for exercise ventilatory measurements," *IEEE Engineering in Medicine and Biology Conference*, 1988, pp. 0823-0824.

Sahakian, A.V. et al., "electrode Motion Artifacts in electrical Impedance Pneumography," *IEEE Transactions in Biomedical Engineering*, vol. BME-32, No. 6, Jun. 1985, pp. 448-451.

Zhihui Chen; Kohkhar, A. "Self organization and energy efficient TDMA MAC protocol by wake up for wireless sensor networks," *Sensor and Ad Hoc Communications and Networks*, 2004. IEEE SECON 2004. 2004 First Annual IEEE Communications Society Conference on, pp. 335-341. Oct. 2004.

Brown, B.H. et al., "Bipolar and Tetrapolar transfer impedance measurements from volume conductor," *Electronics Letters*, vol. 35, No. 25, 2000, pp. 2060-2062.

Cooley, W.L. et al., "A new design for an impedance pneumograph," *Journal of Applied Physiology*, vol. 25, No. 4, 1968, pp. 429-432.

Grenvik, A. et al., "Impedance Pneumography," *Chest*, vol. 62, No. 4, Oct. 1972, pp. 439-443.

Holt, T. et al., "Monitoring and recording of physiological data of the manned space flight program," *Supplement to IEEE Transactions on Aerospace*, Jun. 1965, p. 341-344.

Miller, Matthew J., et al., "On-Demand TDMA Scheduling for Energy Conservation in Sensor Networks," *Technical Report*, Jun. 2004.


Murat, B., "Electrical Impedance Plethysmography," *Wiley Encyclopedia of Biomedical Engineering*, 2006, p. 1-10.


NPL_VitalSense_2006, p. 1-2.

Poon, C. S. et al., "Evaluation of two noninvasive techniques for exercise ventilatory measurements," *IEEE Engineering in Medicine and Biology conference*, 1988, pp. 0823-0824.

Shakian, A. V. et al., "Electrode Motion Artifacts in Electrical Impedance Pneumography," *IEEE Transactions in Biomedical Engineering*, vol. BME-32, No. 6, Jun. 1985, pp. 448-451.

* cited by examiner

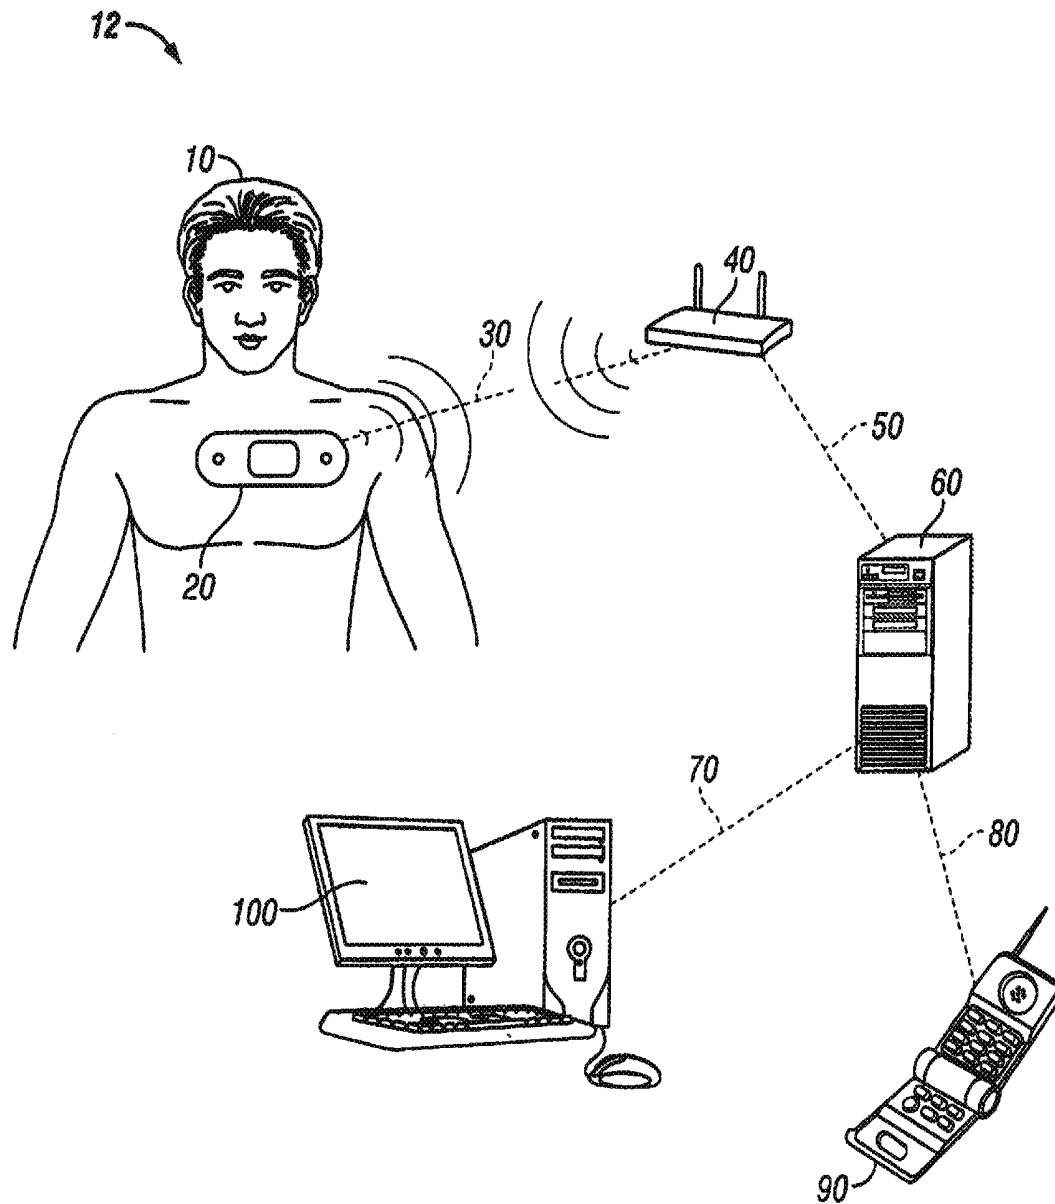**FIG. 1**

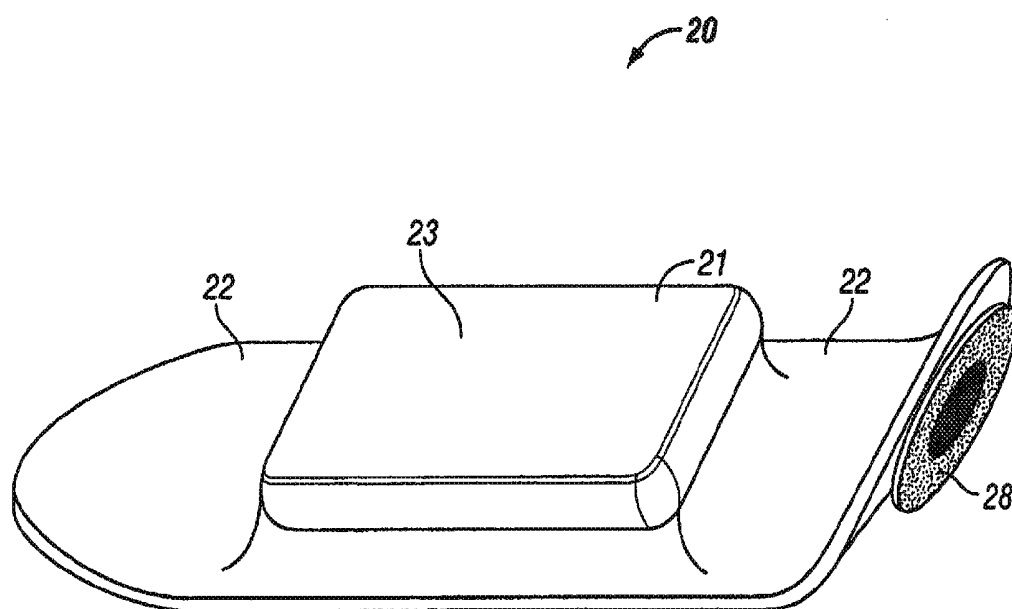**FIG. 2A**

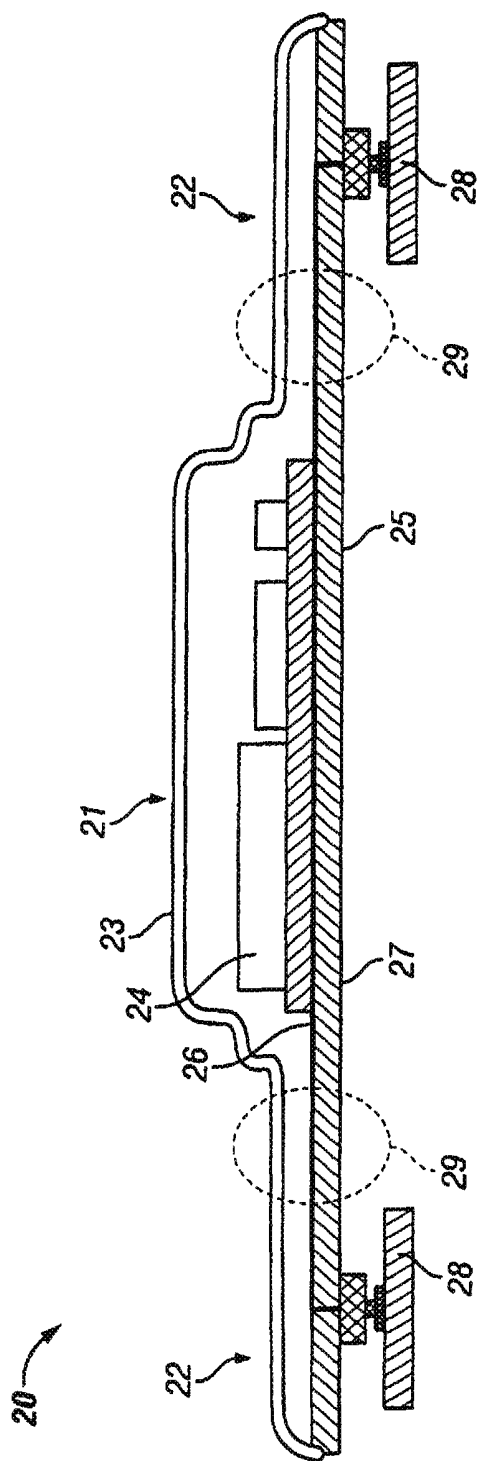
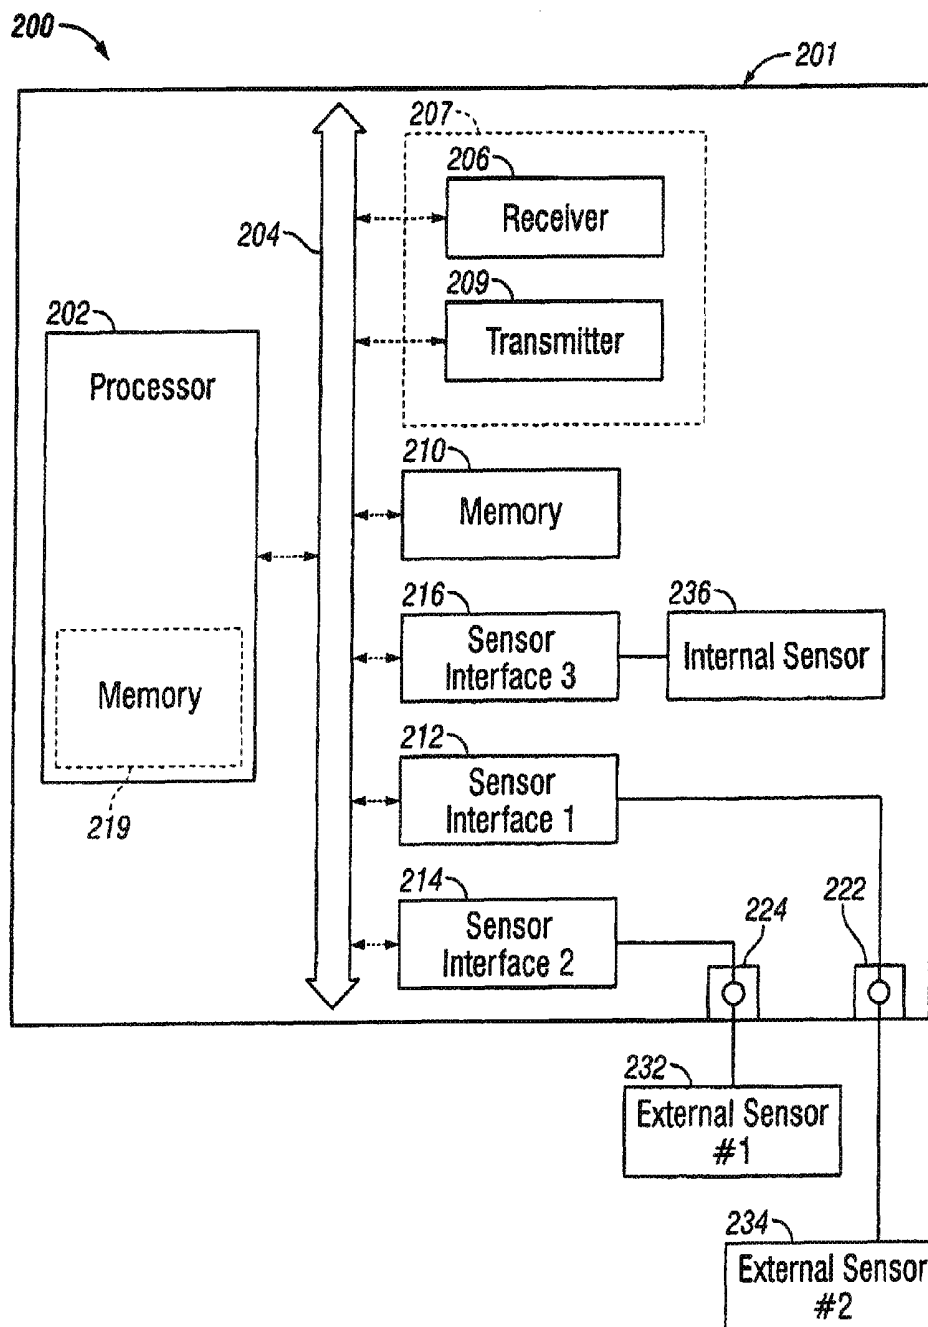
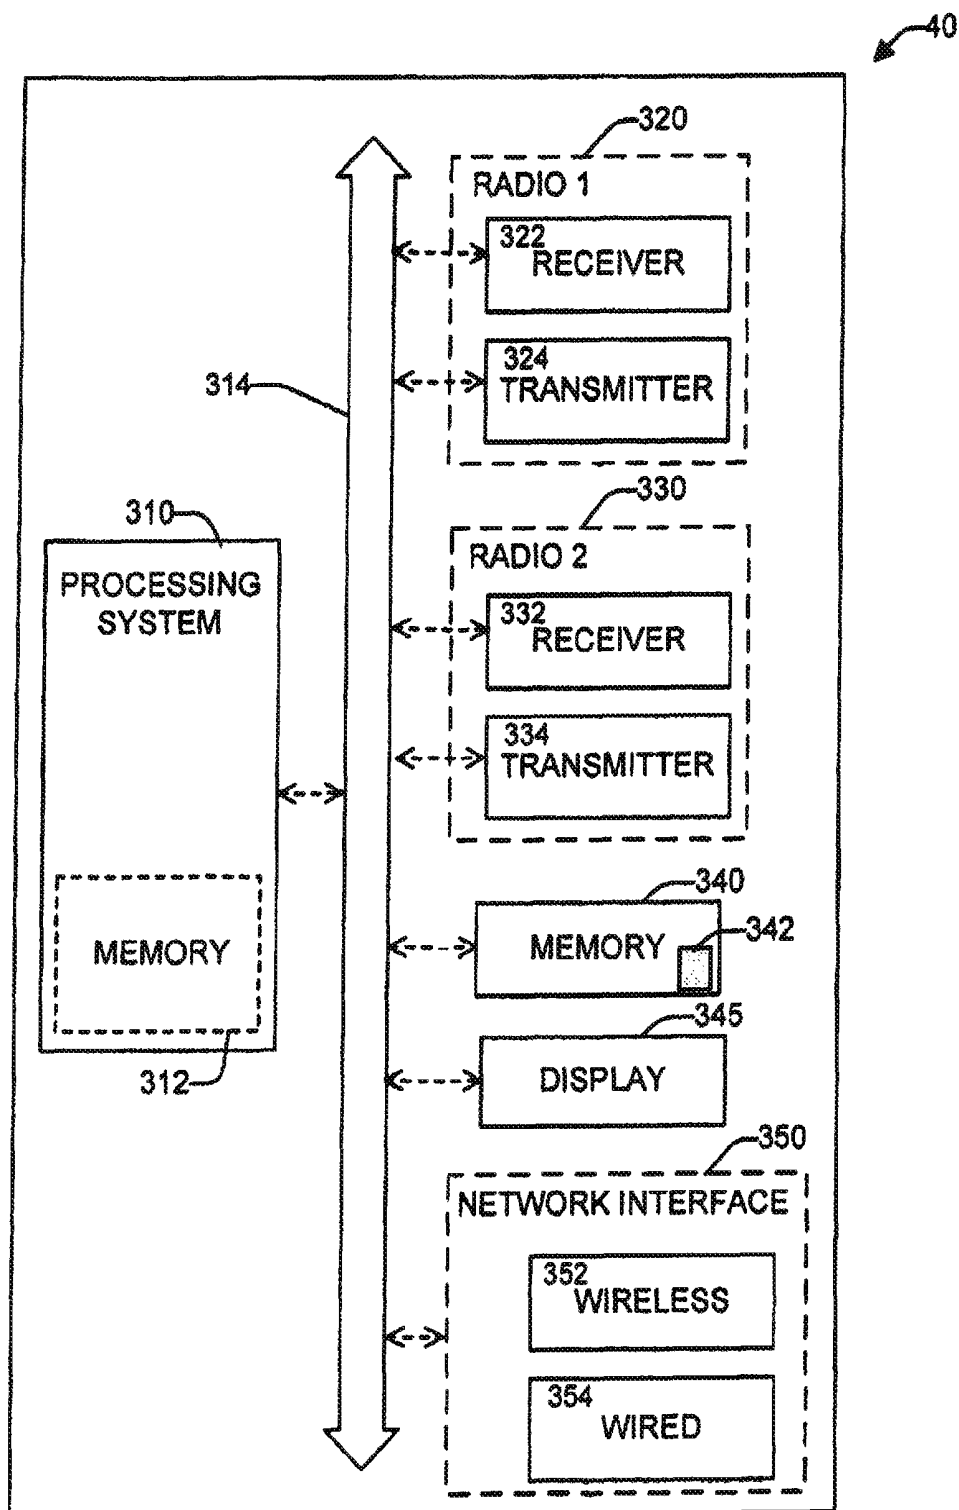
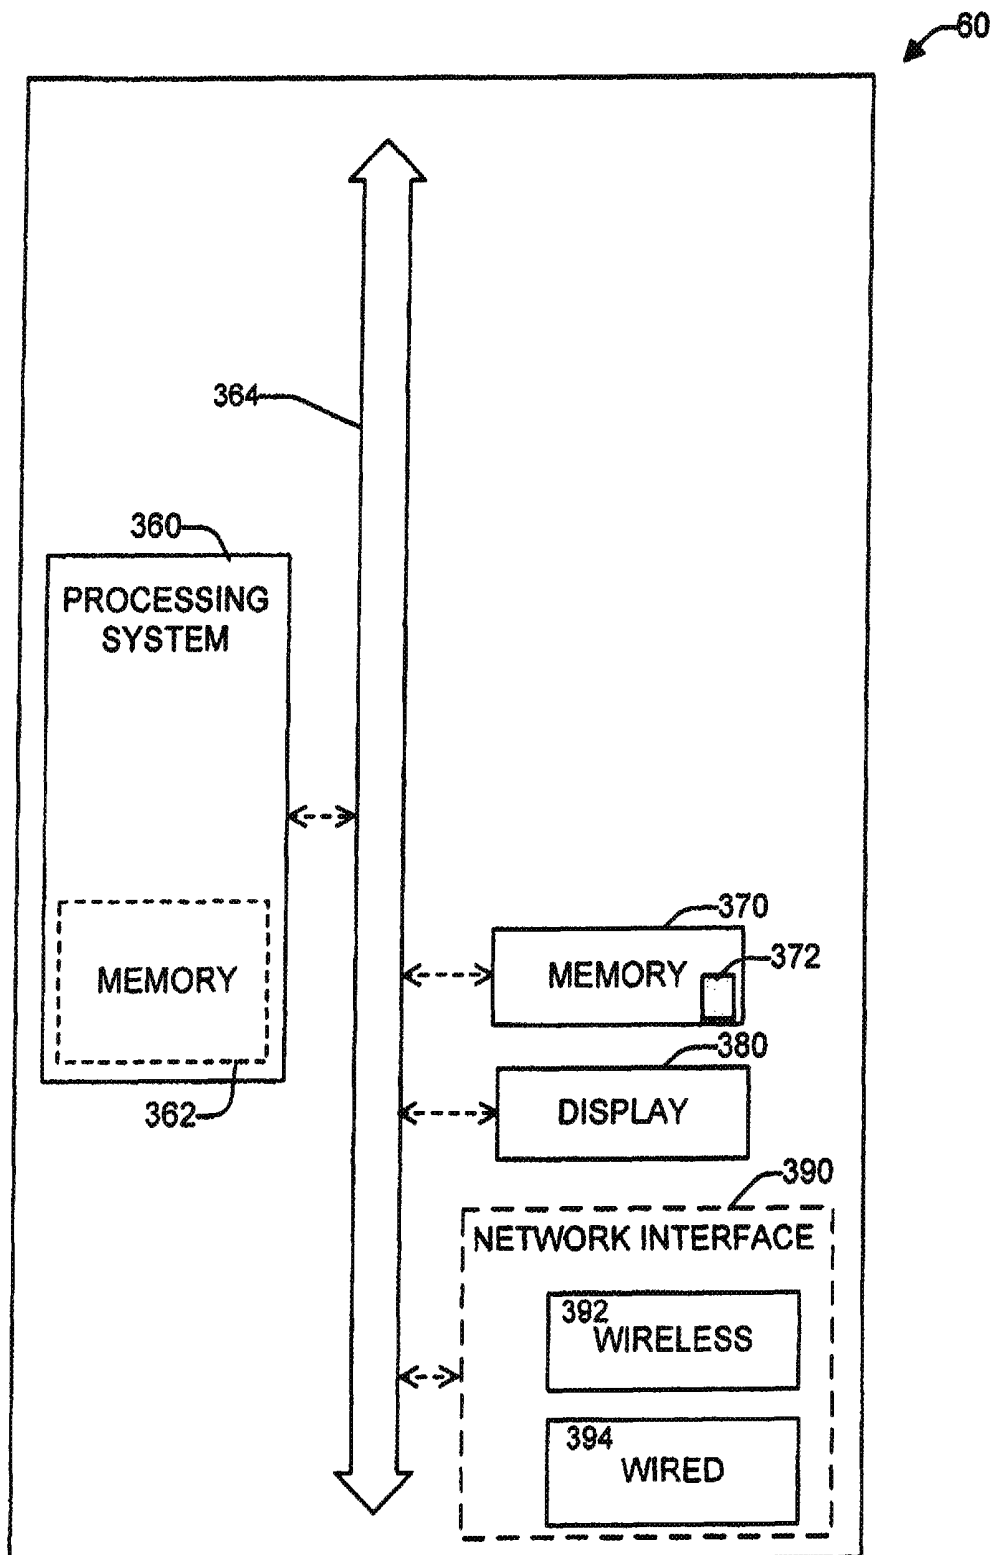
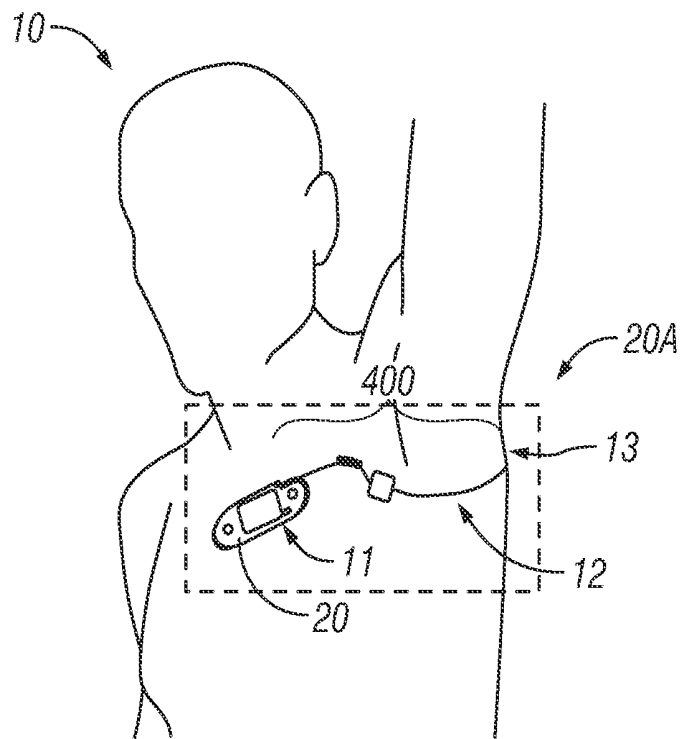


FIG. 2B

**FIG. 2C**

**FIG. 3A**

**FIG. 3B**

**FIG. 4A**

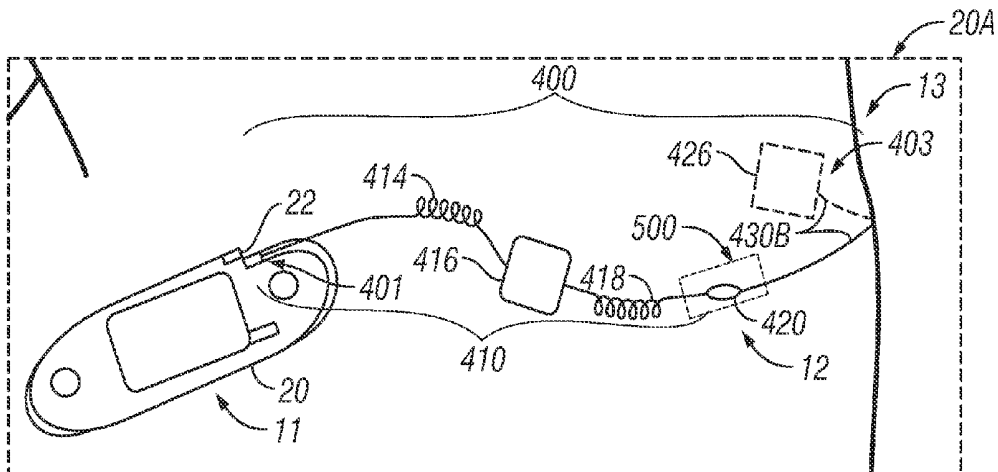


FIG. 4B

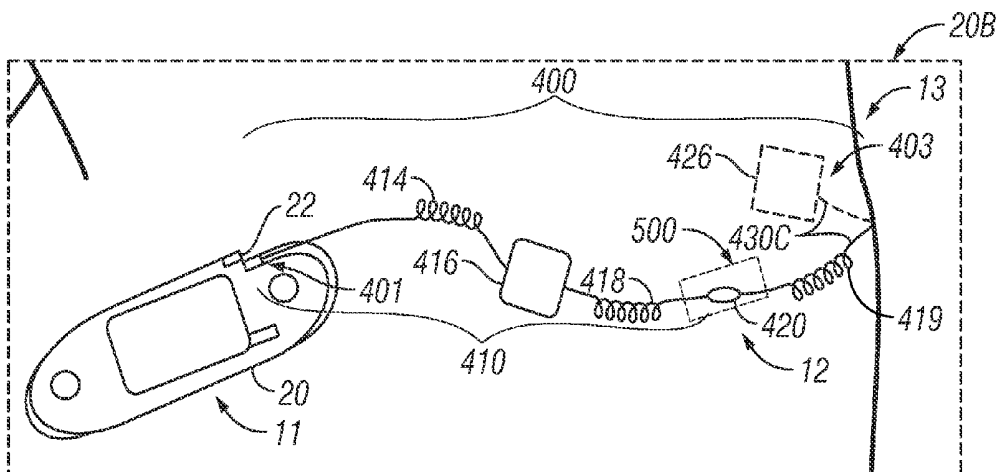


FIG. 4C

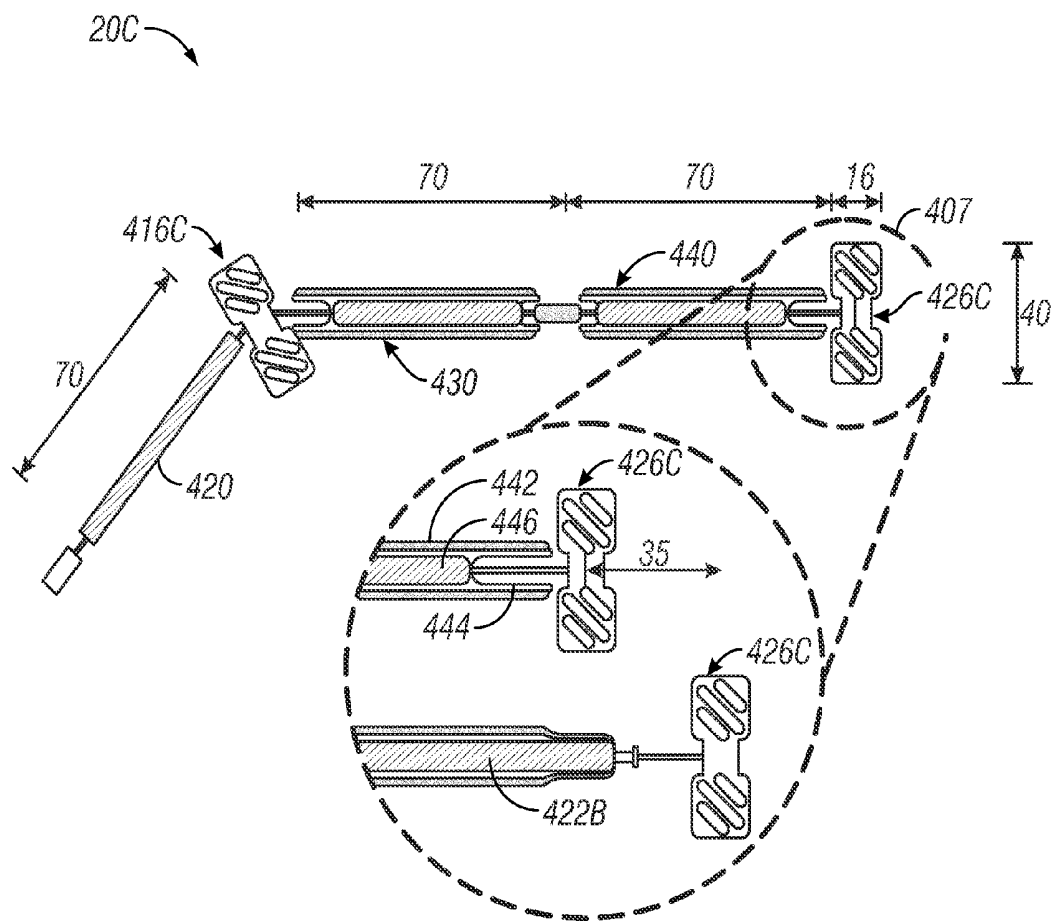
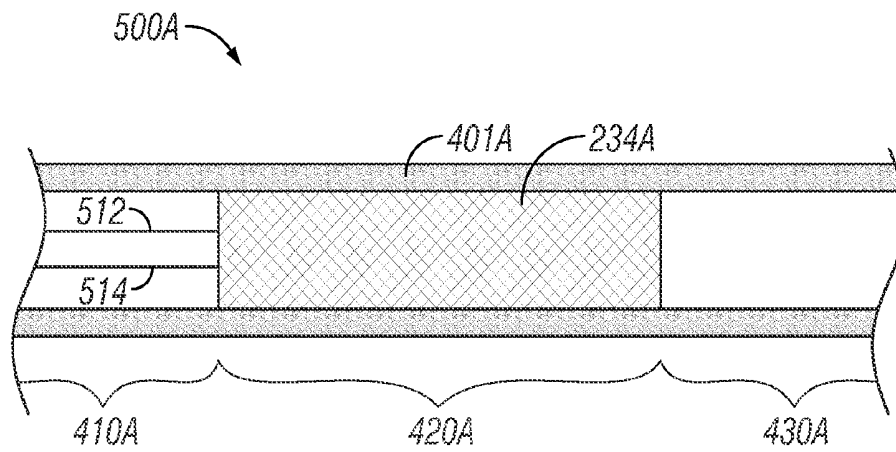
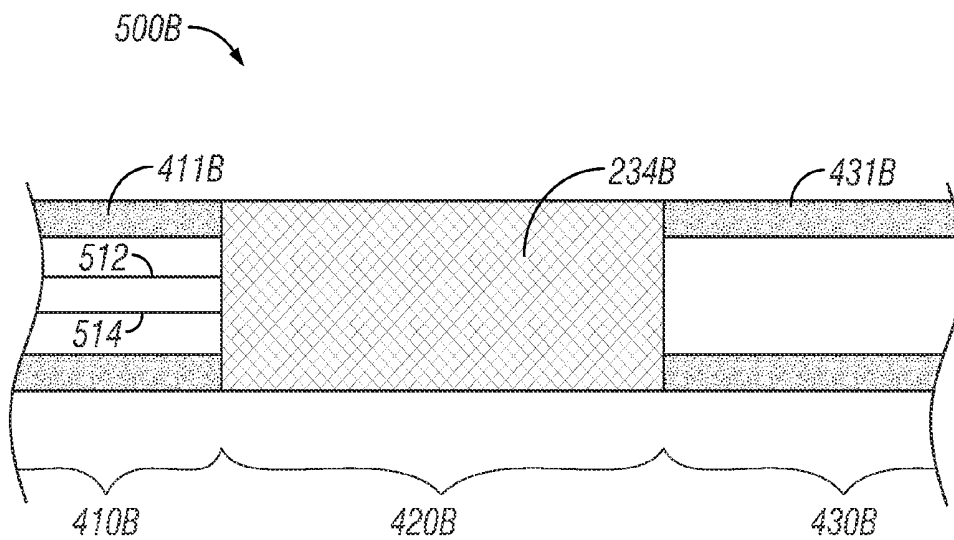
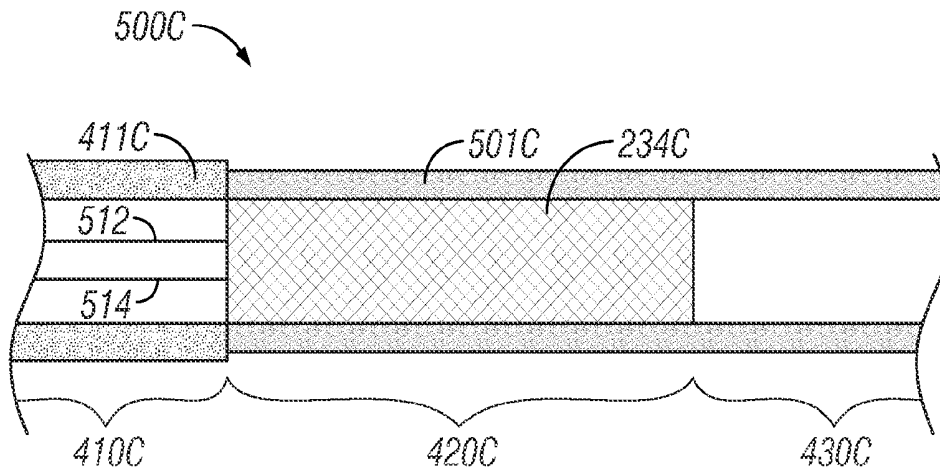
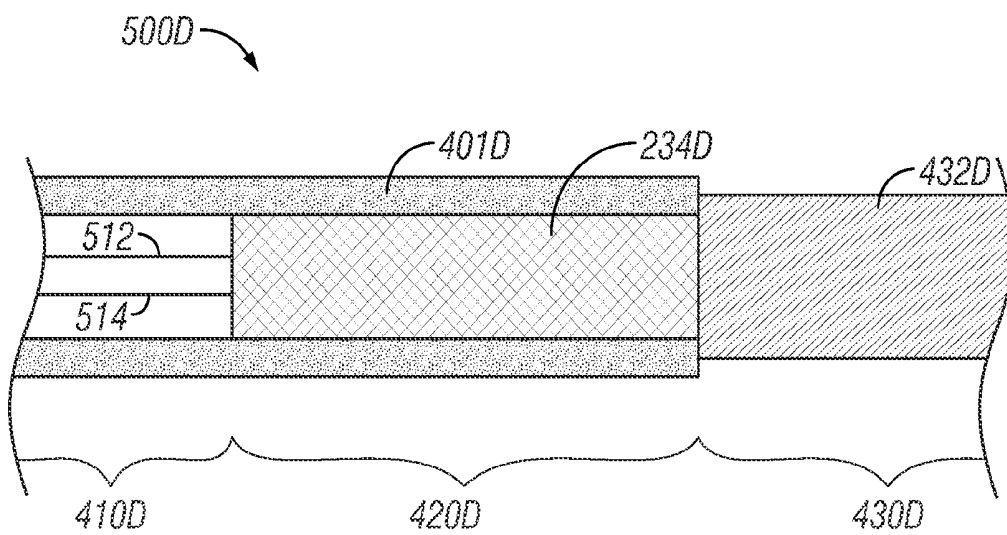


FIG. 4D

**FIG. 5A****FIG. 5B**

**FIG. 5C****FIG. 5D**

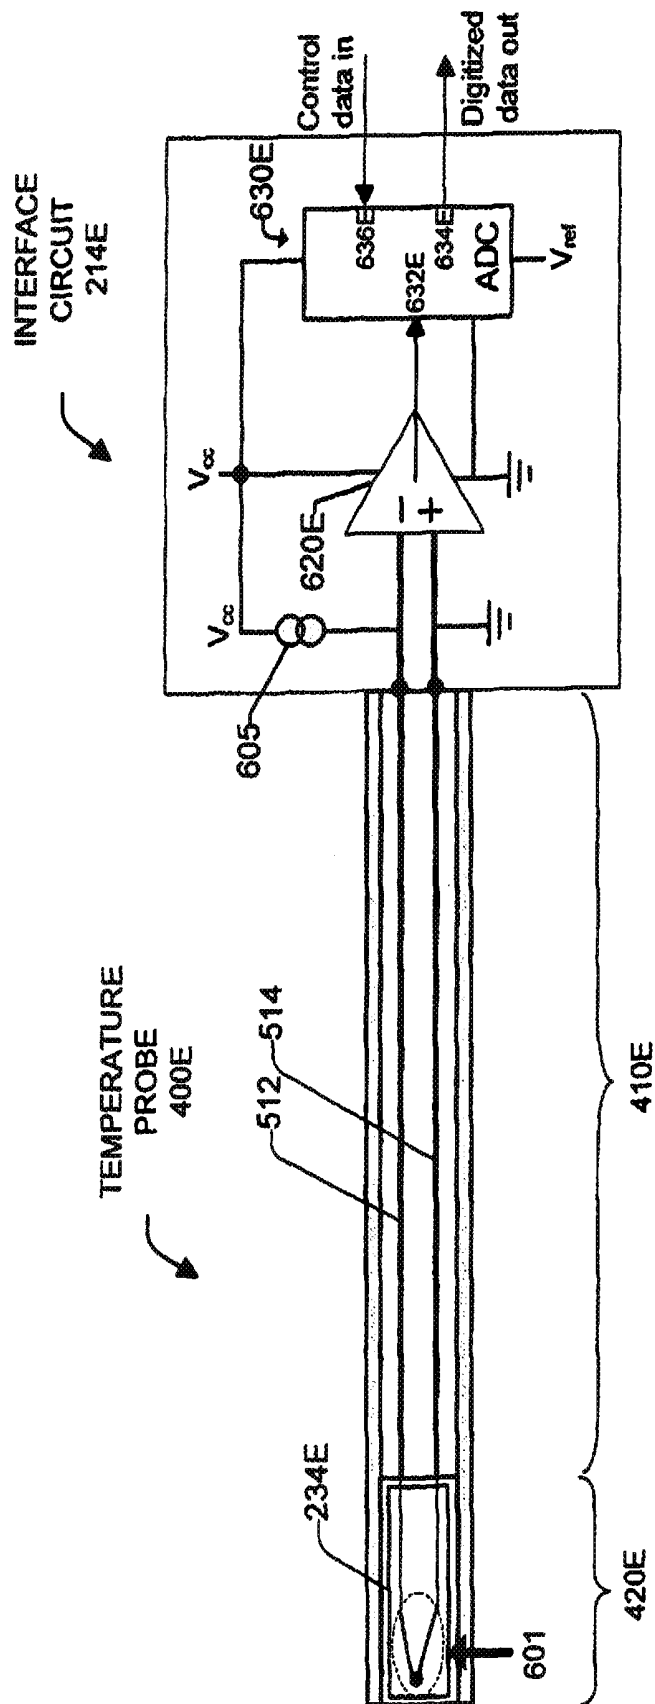


FIG. 6A

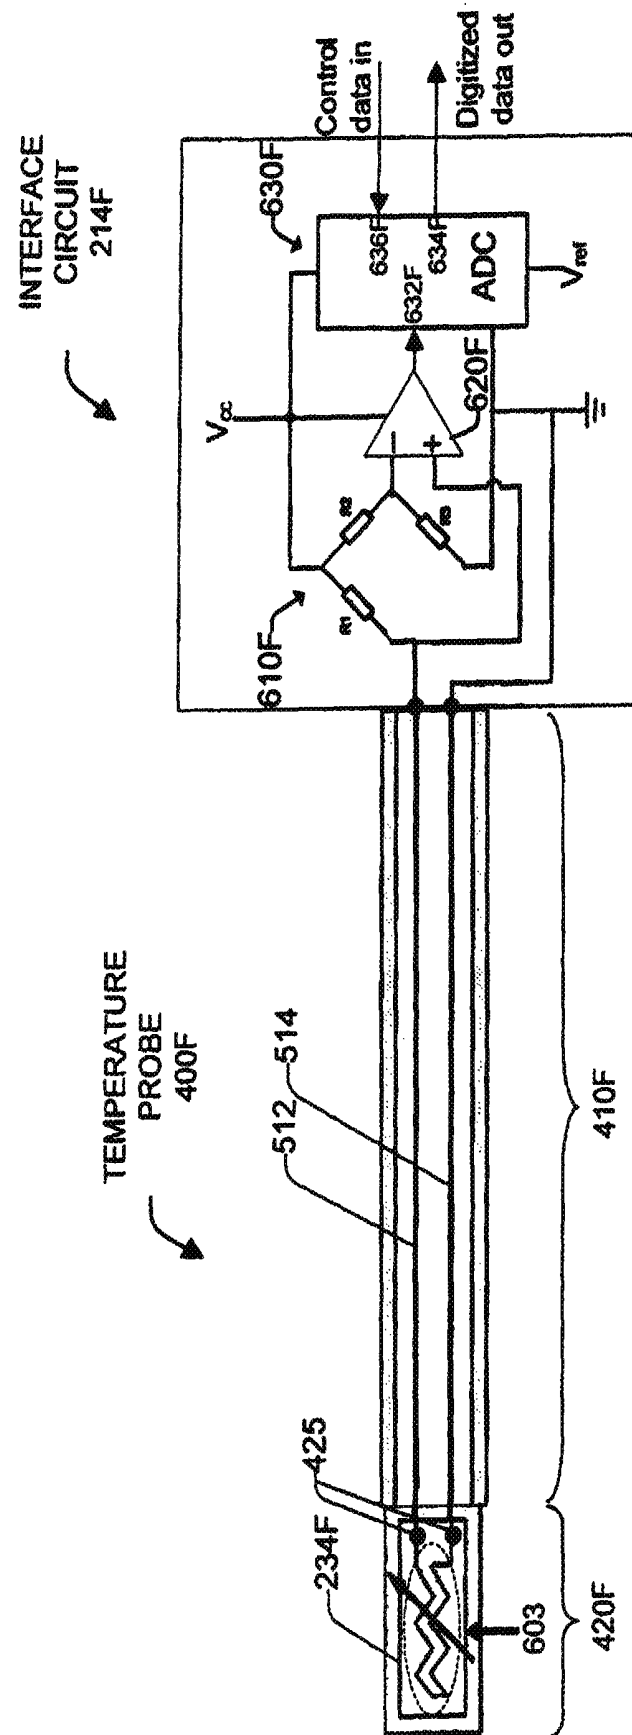


FIG. 6B

BODY-PROBE CONTACT LOSS DETECTION

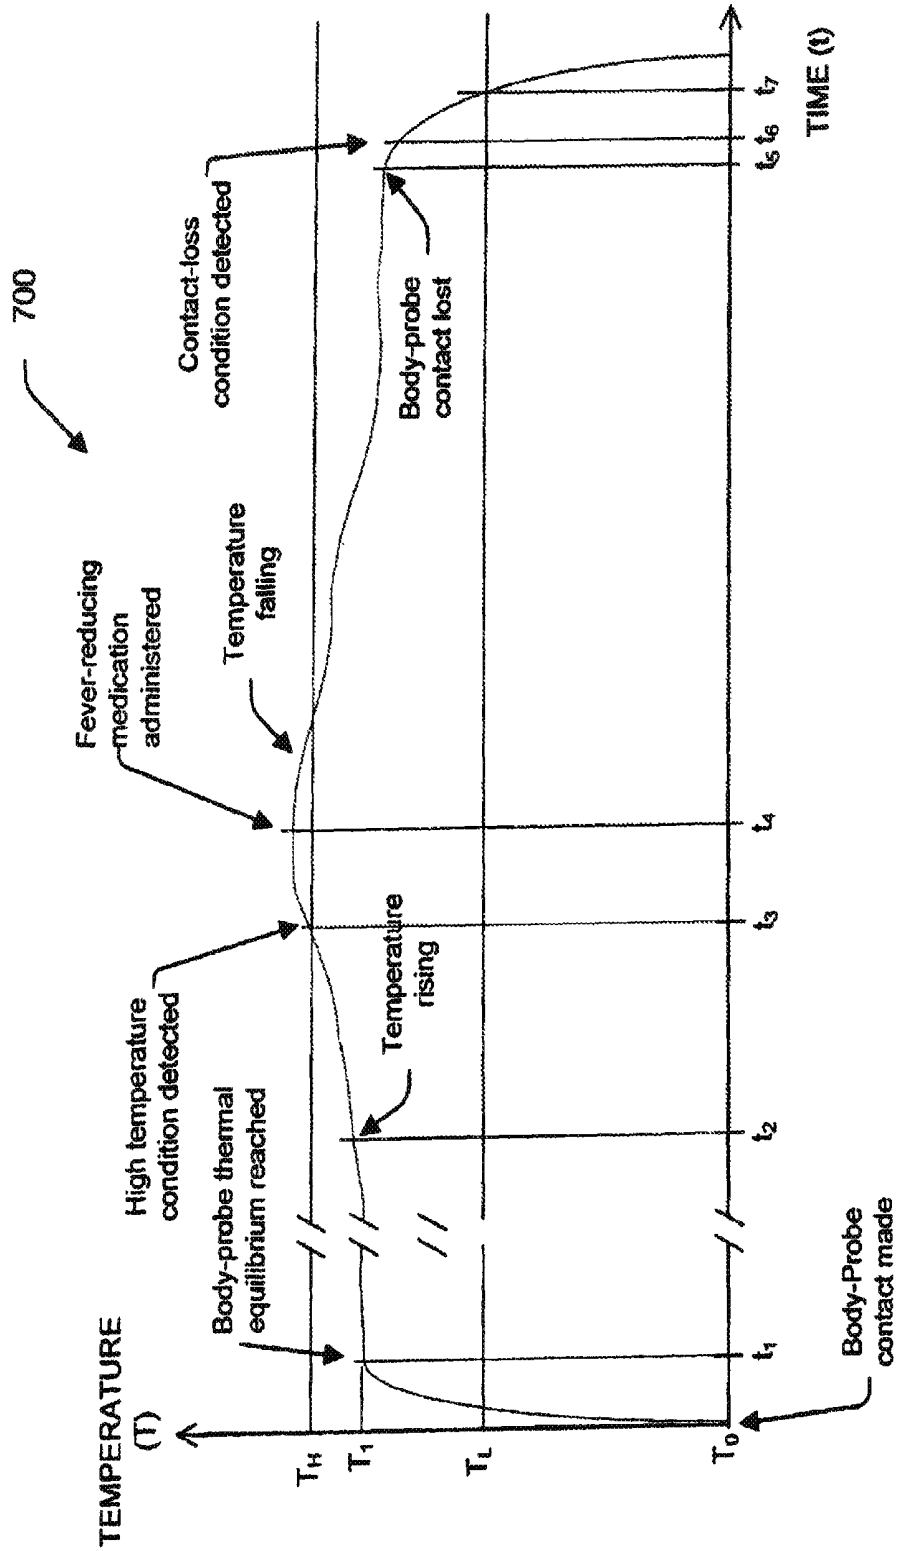
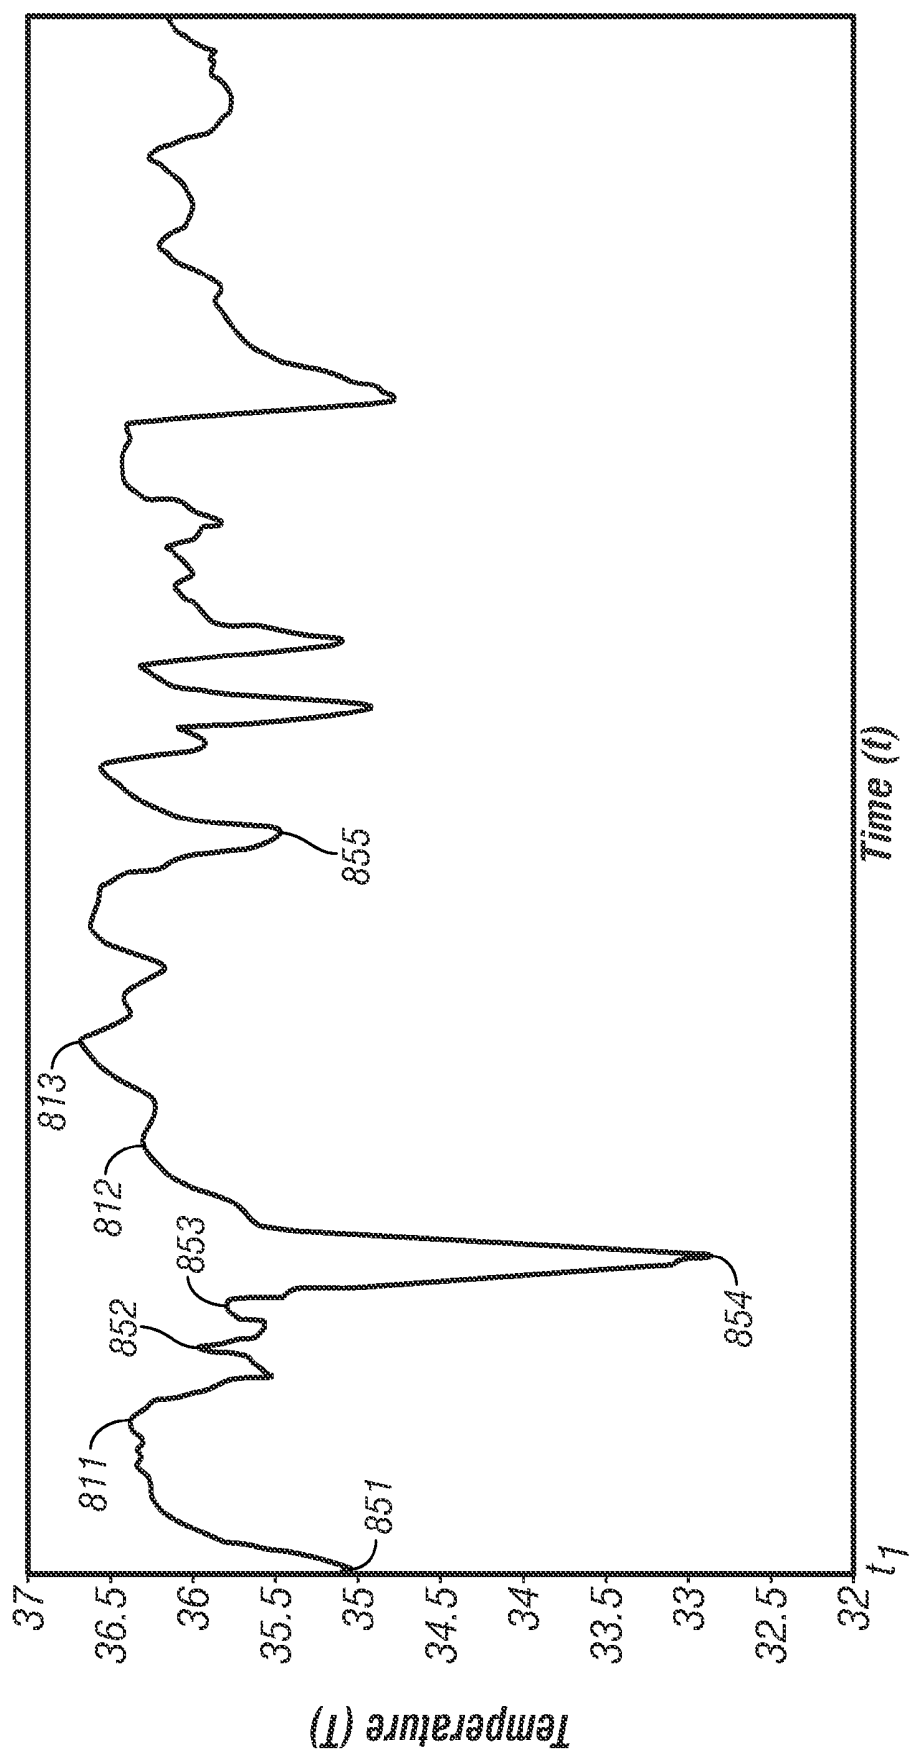


FIG. 7

**FIG. 8A**

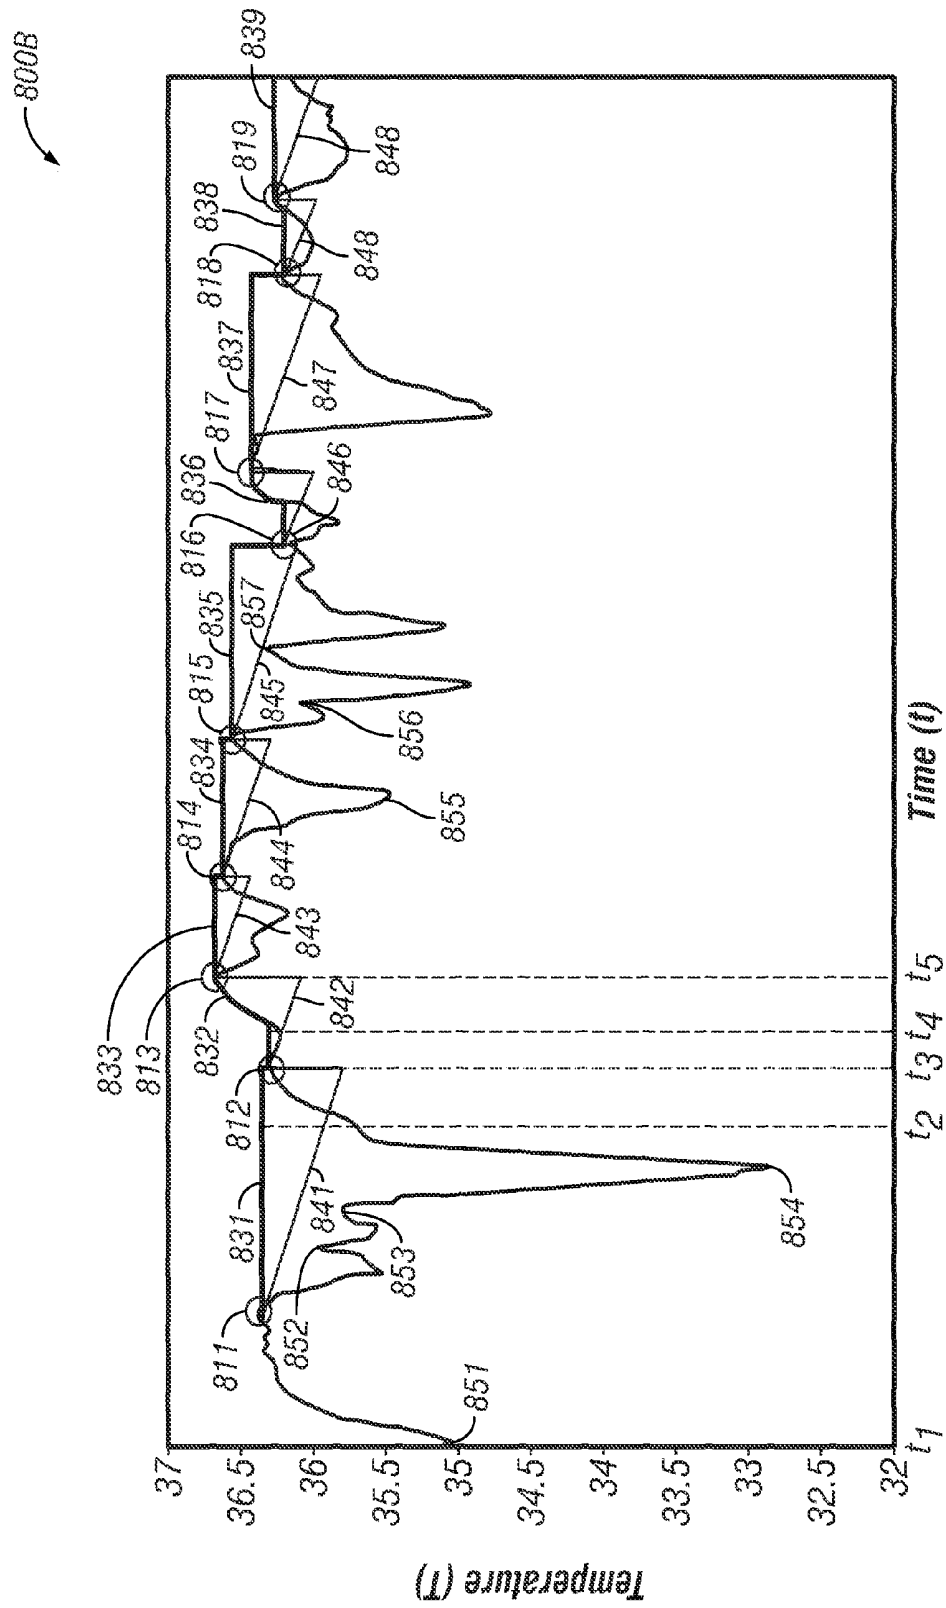


FIG. 8B

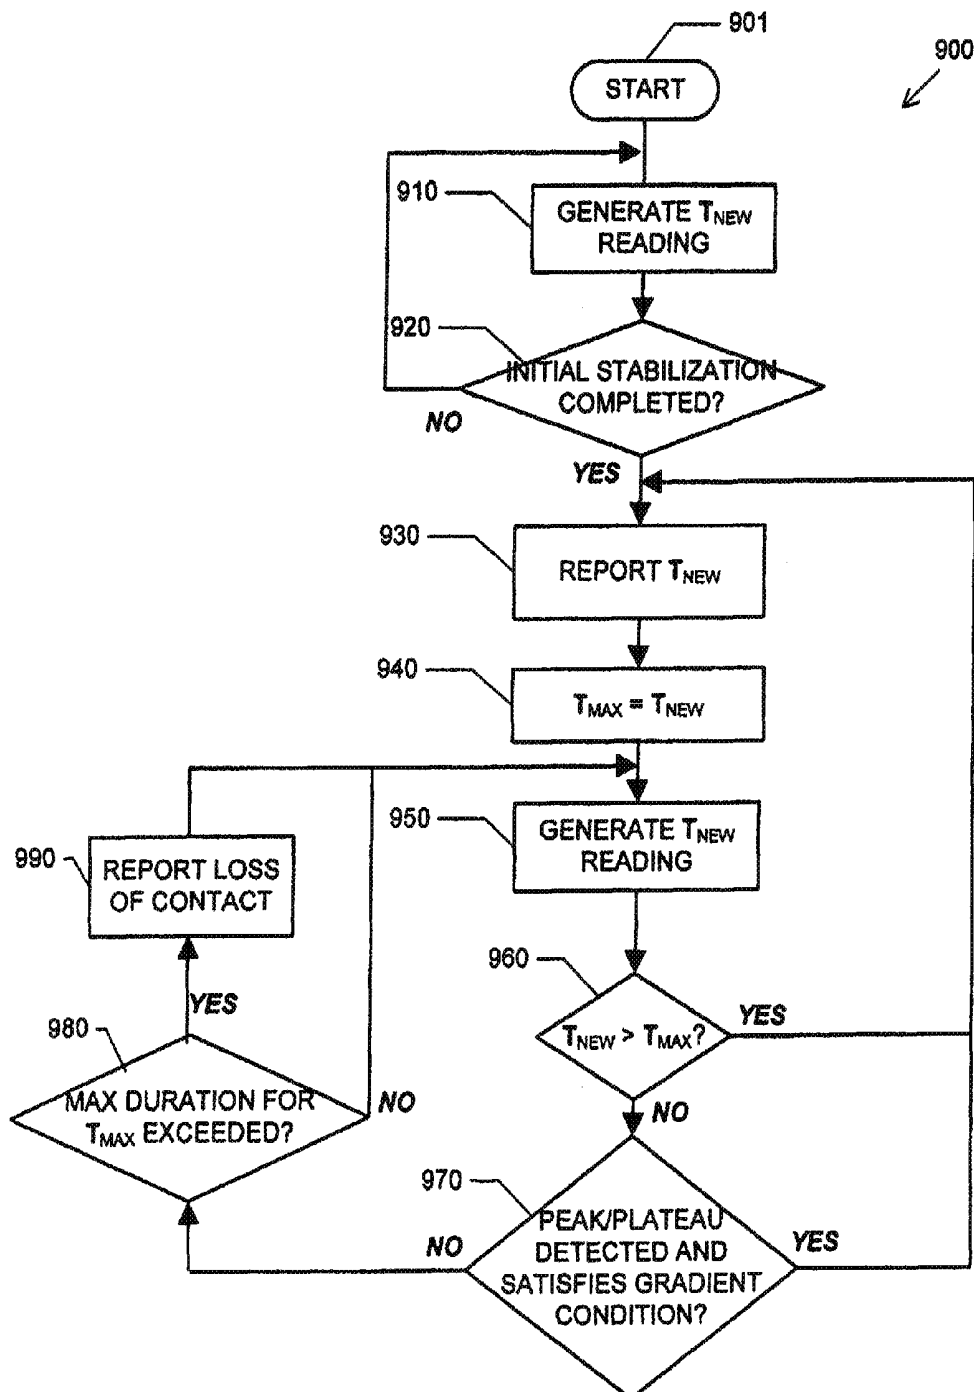


FIG. 9

TEMPERATURE PROBE SUITABLE FOR AXILLARY READING

CROSS-REFERENCES TO RELATED APPLICATIONS

The following applications disclose certain common subject matter with the present application: A Vital-Signs Monitor with Encapsulation Arrangement, U.S. patent application Ser. No. 12/844,766; A Vital-Signs Monitor with Spaced Electrodes, U.S. patent application Ser. No. 12/844,769; A Vital-Signs Patch Having a Strain Relief, U.S. patent application Ser. No. 12/844,774; System and Method for Monitoring Body Temperature of a Person, U.S. patent application Ser. No. 12/844,771; A System and Method for Storing and Forwarding Data from a Vital-Signs Monitor, U.S. patent application Ser. No. 12/844,780; System and Method for Saving Battery Power in a Vital Signs Monitor, U.S. patent application Ser. No. 12/844,789; A System and Method for Conserving Battery Power in a Patient Monitoring System, U.S. patent application Ser. No. 12/844,796; A System and Method for Saving Battery Power in a Patient Monitoring System, U.S. patent application Ser. No. 12/844,801; A System And Method for Tracking Vital-Signs Monitor Patches, U.S. patent application Ser. No. 12/844,788; A System And Method for Reducing False Alarms Associated with Vital-Signs Monitoring, U.S. patent application Ser. No. 12/844,794; A System And Method for Location Tracking of Patients in a Vital-Signs Monitoring System, U.S. patent application Ser. No. 12/844,781; A System And Method for Reducing False Alarms Based on Motion and Location Sensing, U.S. patent application Ser. No. 12/844,765; all of the listed applications filed on Jul. 27, 2010.

FIELD

The present disclosure generally relates to systems and methods of physiological monitoring, and, in particular, relates to a temperature probe suitable for axillary reading.

DESCRIPTION OF THE RELATED ART

Some of the most basic indicators of a person's health are those physiological measurements that reflect basic body functions and are commonly referred to as a person's "vital signs." The four measurements commonly considered to be vital signs are body temperature, pulse rate, blood pressure, and respiratory rate. Some clinicians consider oxygen saturation (S_{O_2}) to be a "fifth vital sign" particularly for pediatric or geriatric cases. Some or all of these measurements may be performed routinely upon a patient when they arrive at a healthcare facility, whether it is a routine visit to their doctor or arrival at an Emergency Room (ER).

Vital signs are frequently taken by a nurse using basic tools including a thermometer to measure body temperature, a sphygmomanometer to measure blood pressure, and a watch to count the number of breaths or the number of heart beats in a defined period of time which is then converted to a "per minute" rate. If a patient's pulse is weak, it may not be possible to detect a pulse by hand and the nurse may use a stethoscope to amplify the sound of the patient's heart beat so that she can count the beats. Oxygen saturation of the blood is most easily measured with a pulse oximeter.

When a patient is admitted to a hospital, it is common for vital signs to be measured and recorded at regular intervals during the patient's stay to monitor their condition. A typical

interval is 4 hours, which leads to the undesirable requirement for a nurse to awaken a patient in the middle of the night to take vital sign measurements.

When a patient is admitted to an ER, it is common for a nurse to do a "triage" assessment of the patient's condition that will determine how quickly the patient receives treatment. During busy times in an ER, a patient who does not appear to have a life-threatening injury may wait for hours until more-serious cases have been treated. While the patient may be reassessed at intervals while awaiting treatment, the patient may not be under observation between these reassessments.

Measuring certain vital signs is normally intrusive at best and difficult to do on a continuous basis. Measurement of body temperature, for example, is commonly done by placing an oral thermometer under the tongue or placing an infrared thermometer in the ear canal such that the tympanic membrane, which shared blood circulation with the brain, is in the sensor's field of view. Another method of taking a body temperature is by placing a thermometer under the arm, referred to as an "axillary" measurement as axilla is the Latin word for armpit. Skin temperature can be measured using a stick-on strip that may contain panels that change color to indicate the temperature of the skin below the strip.

Measurement of respiration is easy for a nurse to do, but relatively complicated for equipment to achieve. A method of automatically measuring respiration is to encircle the upper torso with a flexible band that can detect the physical expansion of the rib cage when a patient inhales. An alternate technique is to measure a high-frequency electrical impedance between two electrodes placed on the torso and detect the change in impedance created when the lungs fill with air. The electrodes are typically placed on opposite sides of one or both lungs, resulting in placement on the front and back or on the left and right sides of the torso, commonly done with adhesive electrodes connected by wires or by using a torso band with multiple electrodes in the strap.

Measurement of pulse is also relatively easy for a nurse to do and intrusive for equipment to achieve. A common automatic method of measuring a pulse is to use an electrocardiograph (ECG or EKG) to detect the electrical activity of the heart. An EKG machine may use 12 electrodes placed at defined points on the body to detect various signals associated with the heart function. Another common piece of equipment is simply called a "heart rate monitor." Widely sold for use in exercise and training, heart rate monitors commonly consist of a torso band, in which are embedded two electrodes held against the skin and a small electronics package. Such heart rate monitors can communicate wirelessly to other equipment such as a small device that is worn like a wristwatch and that can transfer data wirelessly to a PC.

Nurses are expected to provide complete care to an assigned number of patients. The workload of a typical nurse is increasing, driven by a combination of a continuing shortage of nurses, an increase in the number of formal procedures that must be followed, and an expectation of increased documentation. Replacing the manual measurement and logging of vital signs with a system that measures and records vital signs would enable a nurse to spend more time on other activities and avoid the potential for error that is inherent in any manual procedure.

SUMMARY

For some or all of the reasons listed above, there is a need to be able to continuously monitor patients in different set-

tings. In addition, it is desirable for this monitoring to be done with limited interference with a patient's mobility or interfering with their other activities.

Embodiments of the patient monitoring system disclosed herein measure certain vital signs of a patient, which include respiratory rate, pulse rate, blood pressure, body temperature, and, in some cases, oxygen saturation (S_{O_2}), on a regular basis and compare these measurements to defined limits.

In one aspect of the present disclosure, a temperature probe for axillary temperature reading of a person is provided. The temperature probe can comprise a sensing portion configured for placement within the axilla of a person and having a first end and a second end. The sensing portion can comprise a temperature sensing element configured to provide a signal responsive to a change in body temperature of the person. The temperature probe can further comprise a wiring portion having one end connected to the first end of the sensing portion and comprising an electrical conductor, the electrical conductor having a first end configured for coupling to a monitoring device, and a second end connected to the temperature sensing element, the electrical connector configured to carry the signal from the temperature sensing element to the monitoring device. The temperature probe can further comprise a body connection portion having one end connected to the second end of the sensing portion and configured to be attached to another body portion of the person.

In one aspect of the present disclosure, a system for body temperature monitoring of a person through axillary measurement is provided. The system can comprise a temperature probe comprising a cable and a temperature sensing element, configured such that the temperature sensing element is to be retained in the axilla of the person at least during body temperature monitoring. The system can further comprise a monitoring device worn by the person and connected to the cable, the monitoring device receiving signals from the temperature sensing element. The monitoring device can include a wireless communication system to wirelessly transmit readings representative of sensed body temperatures of the person as determined by the monitoring device based on the signals received from the temperature sensing element.

In one aspect of the present disclosure, a method of monitoring the axillary temperature of a person is disclosed. The method can comprise providing a portion of a temperature probe within the axilla of the person, the temperature probe comprising a wiring portion and a body connection portion and a sensing portion between the wiring and body connection portions, the sensing portion comprising a temperature sensing element, the wiring portion coupled to a monitoring device and comprising a conductor having a first end and a second end, the first end coupled to the temperature sensing element, and the second end connected to the monitoring device. The method can further comprise attaching at least a portion of the body connection portion to a second body portion of the person, such that the sensing portion is retained within the axilla.

It is understood that other configurations of the subject technology will become readily apparent to those skilled in the art from the following detailed description, wherein various configurations of the subject technology are shown and described by way of illustration. As will be realized, the subject technology is capable of other and different configurations and its several details are capable of modification in various other respects, all without departing from the scope of the subject technology. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are included to provide further understanding and are incorporated in and constitute a part of this specification, illustrate disclosed embodiments and together with the description serve to explain the principles of the disclosed embodiments. In the drawings:

FIG. 1 is a diagram illustrating an exemplary embodiment of a patient monitoring system according to certain aspects of the present disclosure.

FIG. 2A is a perspective view of the vitals sign monitor patch shown in FIG. 1 according to certain aspects of the present disclosure.

FIG. 2B is a cross-sectional view of the vital signs patch shown in FIGS. 1 and 2A according to certain aspects of the present disclosure.

FIG. 2C is a functional block diagram illustrating exemplary electronic and sensor components of the monitor patch of FIG. 1 according to certain aspects of the present disclosure.

FIG. 3A is a functional schematic diagram of an embodiment of the bridge according to certain aspects of the present disclosure.

FIG. 3B is a functional schematic diagram of an embodiment of the surveillance server according to certain aspects of the present disclosure.

FIG. 4A is a diagram depicting a patient wearing a temperature monitoring system comprising a monitor patch and a temperature probe and configured to measure body temperature of the patient according to certain aspects of the present disclosure.

FIG. 4B is a diagram providing an enlarged view of the temperature monitoring system depicted in FIG. 4A according to certain aspects of the present disclosure.

FIG. 4C is a diagram providing an enlarged view of an alternative monitoring system according to certain aspects of the present disclosure.

FIG. 4D is a diagram depicting another alternative monitoring system according to certain aspects of the present disclosure.

FIGS. 5A-D are diagrams depicting some exemplary embodiments of the temperature probe depicted in FIG. 4B according to alternative aspects of the present disclosure.

FIGS. 6A-B are diagrams depicting two temperature-sensor interface configurations comprising exemplary temperature probes and sensor interfaces according to alternative aspects of the present disclosure.

FIG. 7 is a graph of a measured temperature reading versus time for illustrating an exemplary temperature monitoring scheme according to certain aspects of the present disclosure.

FIG. 8A is a diagram depicting a realistic temperature reading (T) versus time (t) graph associated with a temperature monitoring system according to certain aspects of the present disclosure.

FIG. 8B shows a graph illustrating an exemplary temperature monitoring algorithm based on certain acceptance conditions according to certain aspects of the present disclosure.

FIG. 9 is a flowchart illustrating an exemplary process associated with the exemplary temperature monitoring algorithm of FIG. 8B according to certain aspects of the present disclosure.

DETAILED DESCRIPTION

Periodic monitoring of patients in a hospital is desirable at least to ensure that patients do not suffer an un-noticed sudden deterioration in their condition or a secondary injury during

their stay in the hospital. It is impractical to provide continuous monitoring by a clinician and cumbersome to connect sensors to a patient, which are then connected to a fixed monitoring instrument by wires. Furthermore, systems that sound an alarm when the measured value exceeds a threshold value may sound alarms so often and in situations that are not truly serious that such alarms are ignored by clinicians.

Measuring vital signs is difficult to do on a continuous basis. Accurate measurement of cardiac pulse, for example, can be done using an electrocardiograph (ECG or EKG) to detect the electrical activity of the heart. An EKG machine may use up to 12 electrodes placed at various points on the body to detect various signals associated with the cardiac function. Another common piece of equipment is termed a "heart rate monitor." Widely sold for use in exercise and physical training, heart rate monitors may comprise a torso band in which are embedded two electrodes held against the skin and a small electronics package. Such heart rate monitors can communicate wirelessly to other equipment such as a small device that is worn like a wristwatch and that can transfer data wirelessly to a personal computer (PC).

Monitoring of patients that is referred to as "continuous" is frequently periodic, in that measurements are taken at intervals. In many cases, the process to make a single measurement takes a certain amount of time, such that even back-to-back measurements produce values at an interval equal to the time that it takes to make the measurement. For the purpose of vital sign measurement, a sequence of repeated measurements can be considered to be "continuous" when the vital sign is not likely to change an amount that is of clinical significance within the interval between measurements. For example, a measurement of blood pressure every 10 minutes may be considered "continuous" if it is considered unlikely that a patient's blood pressure can change by a clinically significant amount within 10 minutes. The interval appropriate for measurements to be considered continuous may depend on a variety of factors including the type of injury or treatment and the patient's medical history. Compared to intervals of 4-8 hours for manual vital sign measurement in a hospital, measurement intervals of 30 minutes to several hours may still be considered "continuous."

Certain exemplary embodiments of the present disclosure include a system that comprises a vital-signs monitor patch that is attached to the patient, and a bridge that communicates with monitor patches and links them to a central server that processes the data, where the server can send data and alarms to a hospital system according to algorithms and protocols defined by the hospital.

The construction of the vital-signs monitor patch is described according to certain aspects of the present disclosure. As the patch may be worn continuously for a period of time that may be several days, as is described in the following disclosure, it is desirable to encapsulate the components of the patch such that the patient can bathe or shower and engage in their normal activities without degradation of the patch function. An exemplary configuration of the construction of the patch to provide a hermetically sealed enclosure about the electronics is disclosed.

In the following detailed description, numerous specific details are set forth to provide a full understanding of the present disclosure. It will be apparent, however, to one ordinarily skilled in the art that embodiments of the present disclosure may be practiced without some of the specific details. In other instances, well-known structures and techniques have not been shown in detail so as not to obscure the disclosure.

FIG. 1 discloses a vital sign monitoring system according to certain embodiments of the present disclosure. The vital sign monitoring system 12 includes vital-signs monitor patch 20, bridge 40, and surveillance server 60 that can send messages or interact with peripheral devices exemplified by mobile device 90 and workstation 100.

Monitor patch 20 resembles a large adhesive bandage and is applied to a patient 10 when in use. It is preferable to apply the monitor patch 20 to the upper chest of the patient 10 although other locations may be appropriate in some circumstances. Monitor patch 20 incorporates one or more electrodes (not shown) that are in contact with the skin of patient 10 to measure vital signs such as cardiac pulse rate and respiration rate. Monitor patch 20 also may include other sensors such as an accelerometer, temperature sensor, or oxygen saturation sensor to measure other characteristics associated with the patient. These other sensors may be internal to the monitor patch 20 or external sensors that are operably connected to the monitor patch 20 via a cable or wireless connection. Monitor patch 20 also includes a wireless transmitter that can both transmit and receive signals. This transmitter is preferably a short-range, low-power radio frequency (RF) device operating in one of the unlicensed radio bands. One band in the United States (US) is, for example, centered at 915 MHz and designated for industrial, scientific and medical (ISM) purposes. An example of an equivalent band in the European Union (EU) is centered at 868 MHz. Other frequencies of operation may be possible dependent upon the International Telecommunication Union (ITU), local regulations and interference from other wireless devices.

Surveillance server 60 may be a standard or virtualized computer server connected to the hospital communication network and preferably located in the hospital data center or computer room, although other locations may be employed. The server 60 stores and processes signals related to the operation of the patient monitoring system 12 disclosed herein including the association of individual monitor patches 20 with patients 10 and measurement signals received from multiple monitor patches 20. Hence, although only a single patient 10 and monitor patch 20 are depicted in FIG. 1, the server 60 is able to monitor the monitor patches 20 for multiple patients 10.

Bridge 40 is a device that connects, or "bridges", between monitor patch 20 and server 60. Bridge 40 communicates with monitor patch 20 over communication link 30 operating, in these exemplary embodiments, at approximately 915 MHz and at a power level that enables communication link 30 to function up to a distance of approximately 10 meters. It is preferable to place a bridge 40 in each room and at regular intervals along hallways of the healthcare facility where it is desired to provide the ability to communicate with monitor patches 20. Bridge 40 also is able to communicate with server 60 over network link 50 using any of a variety of computer communication systems including hardwired and wireless Ethernet using protocols such as 802.11a/b/g or 802.3af. As the communication protocols of communication link 30 and network link 50 may be very different, bridge 40 provides data buffering and protocol conversion to enable bidirectional signal transmission between monitor patch 20 and server 60.

While the embodiments illustrated by FIG. 1 employ a bridge 40 to provide communication link between the monitor patch 20 and the server 60, in certain alternative embodiments, the monitor patch 20 may engage in direct wireless communication with the server 60. In such alternative embodiments, the server 60 itself or a wireless modem connected to the server 60 may include a wireless communication system to receive data from the monitor patch 20.

In use, a monitor patch **20** is applied to a patient **10** by a clinician when it is desirable to continuously monitor basic vital signs of patient **10** while patient **10** is, in this embodiment, in a hospital. Monitor patch **20** is intended to remain attached to patient **10** for an extended period of time, for example, up to 5 days in certain embodiments, limited by the battery life of monitor patch **20**. In some embodiments, monitor patch **20** is disposable when removed from patient **10**.

Server **60** executes analytical protocols on the measurement data that it receives from monitor patch **20** and provides this information to clinicians through external workstations **100**, preferably personal computers (PCs), laptops, or smart phones, over the hospital network **70**. Server **60** may also send messages to mobile devices **90**, such as cell phones or pagers, over a mobile device link **80** if a measurement signal exceeds specified parameters. Mobile device link **80** may include the hospital network **70** and internal or external wireless communication systems that are capable of sending messages that can be received by mobile devices **90**.

FIG. **2A** is a perspective view of the vital-signs monitor patch **20** shown in FIG. **1** according to certain aspects of the present disclosure. In the illustrated embodiment, the monitor patch **20** includes component carrier **23** comprising a central segment **21** and side segments **22** on opposing sides of the central segment **21**. In certain embodiments, the central segment **21** is substantially rigid and includes a circuit assembly (**24**, FIG. **2B**) having electronic components and battery mounted to a rigid printed circuit board (PCB). The side segments **22** are flexible and include a flexible conductive circuit (**26**, FIG. **2B**) that connect the circuit assembly **24** to electrodes **28** disposed at each end of the monitor patch **20**, with side segment **22** on the right shown as being bent upwards for purposes of illustration to make one of the electrodes **28** visible in this view.

FIG. **2B** is a cross-sectional view of the vital-signs patch **20** shown in FIGS. **1** and **2A** according to certain aspects of the present disclosure. The circuit assembly **24** and flexible conductive circuit **26** described above can be seen herein. The flexible conductive circuit **26** operably connects the circuit assembly **24** to the electrodes **28**. Top and bottom layers **23** and **27** form a housing **25** that encapsulate circuit assembly **28** to provide a water and particulate barrier as well as mechanical protection. There are sealing areas on layers **23** and **27** that encircle circuit assembly **28** and is visible in the cross-section view of FIG. **2B** as areas **29**. Layers **23** and **27** are sealed to each other in this area to form a substantially hermetic seal. Within the context of certain aspects of the present disclosure, the term 'hermetic' implies that the rate of transmission of moisture through the seal is substantially the same as through the material of the layers that are sealed to each other, and further implies that the size of particulates that can pass through the seal are below the size that can have a significant effect on circuit assembly **24**. Flexible conductive circuit **26** passes through portions of sealing areas **29** and the seal between layers **23** and **27** is maintained by sealing of layers **23** and **27** to flexible circuit assembly **28**. The layers **23** and **27** are thin and flexible, as is the flexible conductive circuit **26**, allowing the side segment **22** of the monitor patch **20** between the electrodes **28** and the circuit assembly **24** to bend as shown in FIG. **2A**.

FIG. **2C** is a functional block diagram **200** illustrating exemplary electronic and sensor components of the monitor patch **20** of FIG. **1** according to certain aspects of the present disclosure. The block diagram **200** shows a processing and sensor interface module **201** and external sensors **232**, **234** connected to the module **201**. In the illustrated example, the module **201** includes a processor **202**, a wireless transceiver

207 having a receiver **206** and a transmitter **209**, a memory **210**, a first sensor interface **212**, a second sensor interface **214**, a third sensor interface **216**, and an internal sensor **236** connected to the third sensor interface **216**. The first and second sensor interfaces **212** and **214** are connected to the first and second external sensors **232**, **234** via first and second connection ports **222**, **224**, respectively. In certain embodiments, some or all of the aforementioned components of the module **201** and other components are mounted on a PCB.

Each of the sensor interfaces **212**, **214**, **216** can include one or more electronic components that are configured to generate an excitation signal or provide DC power for the sensor that the interface is connected to and/or to condition and digitize a sensor signal from the sensor. For example, the sensor interface can include a signal generator for generating an excitation signal or a voltage regulator for providing power to the sensor. The sensor interface can further include an amplifier for amplifying a sensor signal from the sensor and an analog-to-digital converter for digitizing the amplified sensor signal. The sensor interface can further include a filter (e.g., a low-pass or bandpass filter) for filtering out spurious noises (e.g., a 60 Hz noise pickup).

The processor **202** is configured to send and receive data (e.g., digitized signal or control data) to and from the sensor interfaces **212**, **214**, **216** via a bus **204**, which can be one or more wire traces on the PCB. Although a bus communication topology is used in this embodiment, some or all communication between discrete components can also be implemented as direct links without departing from the scope of the present disclosure. For example, the processor **202** may send data representative of an excitation signal to the sensor excitation signal generator inside the sensor interface and receive data representative of the sensor signal from the sensor interface, over either a bus or direct data links between processor **202** and each of sensor interface **212**, **214**, and **216**.

The processor **202** is also capable of communication with the receiver **206** and the transmitter **209** of the wireless transceiver **207** via the bus **204**. For example, the processor **202** using the transmitter and receiver **209**, **206** can transmit and receive data to and from the bridge **40**. In certain embodiments, the transmitter **209** includes one or more of a RF signal generator (e.g., an oscillator), a modulator (a mixer), and a transmitting antenna; and the receiver **206** includes a demodulator (a mixer) and a receiving antenna which may or may not be the same as the transmitting antenna. In some embodiments, the transmitter **209** may include a digital-to-analog converter configured to receive data from the processor **202** and to generate a base signal; and/or the receiver **206** may include an analog-to-digital converter configured to digitize a demodulated base signal and output a stream of digitized data to the processor **202**.

The processor **202** may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory **219**, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in a memory **219** and/or **210**, may be executed by the processor **202** to control and manage the wireless transceiver **207**, the sensor interfaces **212**, **214**, **216**, as well as provide other communication and processing functions.

The processor **202** may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or

a combination of devices that can perform calculations or other manipulations of information.

Information, such as program instructions, data representative of sensor readings, preset alarm conditions, threshold limits, may be stored in a computer or processor readable medium such as a memory internal to the processor **202** (e.g., the memory **219**) or a memory external to the processor **202** (e.g., the memory **210**), such as a Random Access Memory (RAM), a flash memory, a Read Only Memory (ROM), a Programmable Read-Only Memory (PROM), an Erasable PROM (EPROM), registers, a hard disk, a removable disk, or any other suitable storage device.

In certain embodiments, the internal sensor **236** can be one or more sensors configured to measure certain properties of the processing and sensor interface module **201**, such as a board temperature sensor thermally coupled to a PCB. In other embodiments, the internal sensor **236** can be one or more sensors configured to measure certain properties of the patient **10**, such as a motion sensor (e.g., an accelerometer) for measuring the patient's motion or position with respect to gravity.

The external sensors **232**, **234** can include sensors and sensing arrangements that are configured to produce a signal representative of one or more vital signs of the patient to which the monitor patch **20** is attached. For example, the first external sensor **232** can be a set of sensing electrodes that are affixed to an exterior surface of the monitor patch **20** and configured to be in contact with the patient for measuring the patient's respiratory rate, and the second external sensor **234** can include a temperature sensing element (e.g., a thermocouple or a thermistor or resistive thermal device (RTD)) affixed, either directly or via an interposing layer, to skin of the patient **10** for measuring the patient's body temperature. In other embodiments, one or more of the external sensors **232**, **234** or one or more additional external sensors can measure other vital signs of the patient, such as blood pressure, pulse rate, or oxygen saturation.

FIG. 3A is a functional block diagram illustrating exemplary electronic components of bridge **40** of FIG. 1 according to one aspect of the subject disclosure. Bridge **40** includes a processor **310**, radio **320** having a receiver **322** and a transmitter **324**, radio **330** having a receiver **332** and a transmitter **334**, memory **340**, display **345**, and network interface **350** having a wireless interface **352** and a wired interface **354**. In some embodiments, some or all of the aforementioned components of module **300** may be integrated into single devices or mounted on PCBs.

Processor **310** is configured to send data to and receive data from receiver **322** and transmitter **324** of radio **320**, receiver **332** and transmitter **334** of radio **330** and wireless interface **352** and wired interface **354** of network interface **350** via bus **314**. In certain embodiments, transmitters **324** and **334** may include a radio frequency signal generator (oscillator), a modulator, and a transmitting antenna, and the receivers **322** and **332** may include a demodulator and antenna which may or may not be the same as the transmitting antenna of the radio. In some embodiments, transmitters **324** and **334** may include a digital-to-analog converter configured to convert data received from processor **310** and to generate a base signal, while receivers **322** and **332** may include analog-to-digital converters configured to convert a demodulated base signal and sent a digitized data stream to processor **310**.

Processor **310** may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory **312**, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in

memories **312** or **340**, may be executed by the processor **310** to control and manage the transceivers **320**, **330**, and **350** as well as provide other communication and processing functions.

Processor **310** may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or a combination of devices that can perform calculations or other manipulations of information.

Information such as data representative of sensor readings may be stored in memory **312** internal to processor **310** or in memory **340** external to processor **310** which may be a Random Access Memory (RAM), flash memory, Read Only Memory (ROM), Programmable Read Only Memory (PROM), Erasable Programmable Read Only Memory (EPROM), registers, a hard disk, a removable disk, a Solid State Memory (SSD), or any other suitable storage device.

Memory **312** or **340** can also store a list or a database of established communication links and their corresponding characteristics (e.g., signal levels) between the bridge **40** and its related monitor patches **20**. In the illustrated example of FIG. 3A, the memory **340** external to the processor **310** includes such a database **342**; alternatively, the memory **312** internal to the processor **310** may include such a database.

FIG. 3B is a functional block diagram illustrating exemplary electronic components of server **60** of FIG. 1 according to one aspect of the subject disclosure. Server **60** includes a processor **360**, memory **370**, display **380**, and network interface **390** having a wireless interface **392** and a wired interface **394**. Processor **360** may include a general-purpose processor or a specific-purpose processor for executing instructions and may further include a memory **362**, such as a volatile or non-volatile memory, for storing data and/or instructions for software programs. The instructions, which may be stored in memories **362** or **370**, may be executed by the processor **360** to control and manage the wireless and wired network interfaces **392**, **394** as well as provide other communication and processing functions.

Processor **360** may be a general-purpose microprocessor, a microcontroller, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA), a Programmable Logic Device (PLD), a controller, a state machine, gated logic, discrete hardware components, or any other suitable device or a combination of devices that can perform calculations or other manipulations of information.

Information such as data representative of sensor readings may be stored in memory **362** internal to processor **360** or in memory **370** external to processor **360** which may be a Random Access Memory (RAM), flash memory, Read Only Memory (ROM), Programmable Read Only Memory (PROM), Erasable Programmable Read Only Memory (EPROM), registers, a hard disk, a removable disk, a Solid State Memory (SSD), or any other suitable storage device.

Memory **362** or **370** can also store a database of communication links and their corresponding characteristics (e.g., signal levels) between monitor patches **20** and bridges **40**. In the illustrated example of FIG. 3B, the memory **370** external to the processor **360** includes such a database **372**; alternatively, the memory **362** internal to the processor **360** may include such a database.

As indicated above with respect to FIG. 2C, certain embodiments of the monitor patch **20** are configured to operate with external sensors that are in turn configured to produce

a signal representative of one or more vital signs of the patient to whom the monitor patch **20** is attached. For example, the second external sensor **234** can be a temperature probe that includes a temperature sensing element (e.g., a thermocouple or thermistor) affixed, either directly or via an interposing layer, to skin of the patient **10** for measuring the patient's body temperature. FIG. 4A is a diagram depicting a patient **10** wearing a temperature monitoring system **20A** comprising a monitor patch **20** and a temperature probe **400** that is configured to measure body temperature of the patient **10**. In the illustrated example, the temperature probe **400** is configured for axillary temperature sensing of the patient **10** to whom the monitor patch **20** is attached. The monitor patch **20** is attached to the chest **11** of the patient **10**, with a sensing portion of the temperature probe **400** retained in the axilla **12** of the patient **10** during body temperature monitoring.

FIG. 4B is a diagram providing an enlarged view of the monitoring system **20A** depicted in FIG. 4A according to certain aspects of the present disclosure. As indicated above, the monitor patch **20** is attached to the chest **11** of the patient **10** via, e.g., an adhesive backing (not shown). The temperature probe **400** has a proximal end **401** and a distal end **403** and includes a wiring portion **410**, a body connection portion **430B**, and a sensing portion **420** disposed between the wiring and body connection portions **410**, **430B**. The proximal end **401** of the temperature probe **400** is connected to the monitor patch **20** at its connection port **22**. In certain embodiments, the proximal end **401** of the temperature probe **400** is removably attached (e.g., plugged) to the monitor patch **20**. In other embodiments, the proximal end **401** is fixedly attached (e.g., epoxied or fused) to the monitor patch **20**.

The sensing portion **420** of the temperature probe **400** is configured for placement within the axilla **12** of the patient **10** and includes a temperature sensing element (e.g., **234A-D** of FIGS. 5A-D and **234E-F** of FIGS. 6A-B). The wiring portion **410** of the temperature probe **400** includes one or more electrical conductors (**512**, **514** of FIGS. 5A-D and FIGS. 6A-B) for carrying a signal responsive to a change in body temperature of the patient **10** between the temperature sensing element **234** and the monitor patch **20**. In the illustrated example of FIG. 4B, the wiring portion **410** includes a flexible cable comprising a tubing and electrical conductors (e.g., a pair of twisted copper wires) placed within the tubing. The wiring portion **410** includes a first coiled section **414** and a second coiled section **418**. The coiled sections **414**, **418** serve a number of functions including, but not limited to, holding the sensing portion **420** as high as possible in the axilla **12**, accommodating arm movements by reducing the "sawing" effect of a straight wire moving along its axis when the patient's arm is moving, creating a wider surface of contact with the skin, thus increasing patient's comfort, creating a contact surface with the skin that does not tend to cause irritation as much as a straight wire would.

In the illustrated example, the monitoring system **20A** further includes an adhesive element **416** (e.g., a tape) coupled to the cable between the first and second coiled sections **414**, **418** and configured to attach the wiring portion **410** of the cable to the patient's body, e.g., at a point between the chest **11** and the armpit **12** of the patient.

The body connection portion **430B** has one end connected to the sensing portion **420** and is configured to be attached to another body portion of the patient **10** such that the sensing portion **420** of the temperature probe **400** can be retained within the axilla **12** of the patient **10**. In the illustrated example, such attachment is achieved via an adhesive element **426** (e.g., a tape) coupled to the distal end of the body connection portion **430B**. The coupled adhesive element **426**

is then attached to a second body portion **13** (e.g., the back of the patient's arm) of the patient **10**. In the illustrated embodiment of FIG. 4B, the body connection portion **430B** includes an elastic tubing comprising an elastic polymers (elastomers) such as natural rubber, synthetic polyisoprene, butyl rubber, and the like. In such embodiments, the adhesive element **426** is attached to the patient's body while the elastic tubing is in its stretched state such that the restorative ("pulling") tensile force in the stretched tubing helps to hold the temperature sensing portion **420** in place within the axilla **12** of the patient. The adhesive elements **416**, **426** can be pre-attached adhesive tabs with a peel-off backing. Alternatively, the adhesive elements **416**, **426** can be pre-attached fixture tab that allow for the use of a standard medical tape. Openings (holes, slots, etc.) can be present in both cases to allow skin to breathe. The adhesive elements **416**, **426** are preferably positioned at about the same vertical level, high enough so both of the stretchable coiled sections **414**, **418** would pull the sensing portion **420** upward.

FIG. 4C is a diagram providing an enlarged view of an alternative monitoring system **20B** according to certain aspects of the present disclosure. The monitoring system **20B** is substantially the same as the monitoring system **20A**, except an additional (e.g., third) coiled section **419** is provided in body connection portion **430C** in place of the elastic tubing **430B**. The additional coiled section **419** can provide all or some of the pulling force such as the one provided by the elastic tubing in the embodiment of FIG. 4B. In one or more implementations, the coiled section **419** acts as a spring. The remainder of the body connection portion **430C** may include an elastic or inelastic flexible tubing.

FIG. 4D is a diagram depicting another alternative monitoring system **20C** according to certain aspects of the present disclosure. The monitoring system **20C** includes a first stretchable component **420**, a second stretchable component **430**, and a third stretchable component **440**. The monitoring system **20C** further comprises adhesive elements **416C**, **426C**. At least some of the stretchable components (e.g., **440**) include a tubing **442** with a flexible boot **424** at the end thereof as illustrated by an enlarged view of an end section **407** of the stretchable component **440**. The enlarged view shows the stretchable component **440** in its unstretched state (top) and in its stretched state (bottom). The adhesive elements **416C**, **426C** are substantially similar to the adhesive elements **416**, **426** described above with respect to the monitoring system **20A**. The adhesive element **426C** depicted in the enlarged view include slotted holes that allow skin to breathe.

A multitude of modifications and additions to the illustrated embodiments of FIGS. 4B, 4C and 4D are possible without departing from the scope of the disclosure. For example, the body connection portion **430** of the temperature probe **400** can include one or more coiled sections similar to the coiled section **414** of the wiring portion **410**. Any or all of the coiled sections **414**, **418**, **419** in the embodiments of FIGS. 4B and 4C may be replaced with elastic elements (e.g., elastic tubing). The adhesive element **416** may be coupled to the body connection portion **430** at a point different than the distal end of the body connection portion **430**. In certain embodiments, entirely different means of attaching the body connection portion **430** to the patient's body may be used. For example, the body connection portion **430** may itself be in the form of an adhesive tape that can stick to the body of the patient **10** or may include an elastic loop (e.g., a rubber band) to be placed around the patient's arm.

While the temperature probe **400** in the illustrated embodiments of FIGS. 4A-C is shown to be operatively coupled to a vital-sign monitor patch worn by the patient **10**, the tempera-

ture probe **400** may be alternatively operatively coupled to other types of monitoring devices such as a stationary monitoring unit located near the patient's hospital bed. Such a stationary monitoring unit can take readings of the patient's body temperature based on a signal from the temperature probe **400** and send the temperature readings to a surveillance server via a wired or wireless connection and make other decisions such as providing an indication of an alarm condition (e.g., a high body temperature condition or a loss of thermal contact between the temperature probe and the patient).

FIGS. 5A-D are diagrams depicting various exemplary embodiments of the temperature probe according to alternative aspects of the present disclosure. For the purposes of illustration only, without an intent to limit the scope of the present disclosure in any way, the embodiments will be described with references to elements of FIG. 4B. For clarity, each of the diagrams focuses on a region **500A-D** (corresponding to region **500** in FIG. 4B) of the thermocouple **400** where sensing portion **420A-D** interfaces with wiring portion **410A-D** and body connection portions **430A-D**. The figures are not drawn to scale.

In the first exemplary embodiment of the temperature probe **400** depicted in FIG. 5A, the wiring portion **410A**, the sensing portion **420A**, and the body connection portion **430A** comprise a single hollow flexible cable **401A**. The wiring portion **410A** of the flexible cable **401A** includes a first electrical conductor **512** and a second electrical conductor **514**. The sensing portion of the flexible cable **401A** houses a temperature sensing element **234A** that is electrically connected to the first and second electrical conductors **512**, **514**. The temperature sensing element **234A** is configured to make thermal contact with the axilla of the patient **10** through the surrounding flexible cable **401A**. In the illustrated example, the body connection portion **430A** of the flexible cable **401A** is empty inside.

In the second exemplary embodiment of the temperature probe **400** depicted in FIG. 5B, the wiring portion **410B** comprises a first hollow flexible cable **411B** having a first electrical conductor **512** and a second electrical conductor **514**. The sensing portion **420B** includes a temperature sensing element **234B**. In the illustrated example, the temperature sensing element **234B** is mechanically connected (e.g., glued or fused) to an end portion of the first flexible cable **411B** and is electrically connected to the first and second electrical conductors **512**, **514**. The temperature sensing element **234B** is configured to make a direct physical and thermal contact with the axilla **12** of the patient **10** (i.e., not through a flexible cable). The body connection portion **430B** comprises a second hollow flexible cable **431B**. In the illustrated example, the second flexible cable **431B** is empty inside.

In the third exemplary embodiment of the temperature probe **400** depicted in FIG. 5C, wiring portion **410C** comprises a first flexible cable **411C** having a first electrical conductor **512** and a second electrical conductor **514**. The sensing portion **420C** and body connection portion **430C** comprise a second hollow flexible cable **501C**. The second flexible cable **501C** is mechanically connected (e.g., glued or fused) to an end portion of the first flexible cable **411C**. The sensing portion **420C** of the second flexible cable **501C** houses a temperature sensing element **234C** that is electrically connected to the first and second electrical conductors **512**, **514**. The temperature sensing element **234C** is configured to make a thermal contact with the axilla of a patient through the surrounding second flexible cable **501C**. The body connection portion **430C** of the second flexible cable **401C** is empty inside.

In the fourth exemplary embodiment of the temperature probe **400** depicted in FIG. 5D, the wiring portion **410D** and the sensing portion **420D** comprise a first flexible cable **401D**. The wiring portion **410D** of the first flexible cable **401D** includes a first electrical conductor **512** and a second electrical conductor **514**. The sensing portion **420D** of the first flexible cable **401D** houses a temperature sensing element **234D**. The temperature sensing element **234D** is electrically connected to the first and second electrical conductors **512**, **514**. The body connection portion **430D** comprises a flexible tape **432D** that is mechanically connected (e.g., glued or fused) to the sensing portion **420D** at the temperature sensing element **234D** and/or an end portion of the first flexible cable **401D**. In certain embodiments, the flexible tape **432D** includes an adhesive section that can be attached to a body portion (e.g., the back of the patient's arm) so as to retain the sensing portion **420D** of the temperature probe **400** within the axilla **12** of the patient **10**.

The above embodiments of FIGS. 5A-5D are exemplary only, as other embodiments can be employed without departing from the scope of the present disclosure. For example, a modular arrangement in which the cables are snap connectable with the temperature sensing element can be employed, as well as other physical configurations.

FIGS. 6A-B are diagrams depicting two temperature-sensor interface configurations comprising exemplary temperature probes **400E**, **400F** and sensor interfaces **214E**, **214F** according to alternative aspects of the present disclosure. Each of the temperature probes **400E**, **400F** comprises respective wiring portion **410E**, **410F** and sensing portion **420E**, **420F** having temperature sensing element **234E**, **234F**. Each of the sensor interface circuits **214E**, **214F** is connected to the temperature probe **400E**, **400F** and configured to receive a sensor signal from the temperature sensing element **234E**, **234F** via electrical conductors **512**, **514** in the wiring portion **410E**, **410F** of the probe **400E**, **400F**. As described above with respect to FIG. 2, the sensor interface **214E**, **214F** is part of a processing and sensor interface module (e.g., **201**) of a vital-sign monitor patch (e.g., **20**). For simplicity, each of the diagrams shows only a wiring portions **410E**, **410F** and a sensing portion **420E**, **420F** of the temperature probe **400E**, **400F**. The figures are not drawn to scale.

In the first exemplary probe-sensor interface configuration depicted in FIG. 6A, the temperature sensing element **234E** is a thermocouple that comprises a junction **601** between two different metals. The junction **601** produces a voltage difference related to temperature at the junction **601**. The junction is of dissimilar metals including specific alloys such as platinum and platinum-rhodium alloy (Type S) or chromel and alumel (Type K). This embodiment of a thermocouple is exemplary only, as other embodiments may be employed. For example, additional circuits/elements relating to cold junction compensation may be used. In some embodiments, the temperature sensing element may comprise a resistance temperature detector (RTD) based on platinum.

A signal representative of the voltage difference produced at the junction **601** of the thermocouple **234E** is received by the sensor interface **214E** via the first and second electrical conductors **512**, **514** in the wiring portion **410E**. The sensor interface **214E** includes an amplifier **620E**, an analog-to-digital converter (ADC) **630E** and a current source **605**. The current source **605** supplies a constant DC current that flows through the junction and produces a signal representative of the voltage difference across the junction. The signal is received at the minus input of the amplifier **620E**. The received signal is amplified by the amplifier **620E**, and the amplified signal is received by the ADC **630E** at input port

632E. The ADC 630E digitizes the amplified signal and provides a stream of digitized data at output port 634E. The stream of digitized data is passed to a processor (e.g., 202 of FIG. 2) for further processing and/or transmission to a surveillance server (e.g., 60 of FIG. 1) via a bridge (e.g., 40 of FIG. 1). In certain embodiments, the ADC 630E at its control data input port 636E receives from the processor a set of control data that configures one or more functionalities of the ADC 630E including, not limited to, its sampling (digitization) rate and dynamic range.

In the second exemplary probe-sensor interface depicted in FIG. 6B, the temperature sensing element 234F includes a thermistor 603, a type of resistor whose resistance varies with temperature. The thermistor 603 can be made from a material that has a positive temperature coefficient (PTC) (called a "PTC thermistor") or from a material that has a negative temperature coefficient (NTC) (called a "NTC thermistor").

Two electrical contacts 425 of the thermistor 603 are connected to the sensor interface circuit 214F via the first and second electrical conductors 512, 514 in the wiring portion 410F. The sensor interface circuit 214F includes a Wheatstone bridge 610F having three fixed resistors (R1, R2, and R3), an amplifier 620F, and an analog-to-digital converter (ADC) 630F. By the connection provided by the first and second electrical conductors 512, 514, the thermistor 603 functions as a fourth and variable resistor in the Wheatstone bridge 610F such that the bridge 610F outputs a signal that is responsive to a change in the resistance of the thermistor 603, which resistance is in turn responsive to a change in the body temperature of the patient 10. The signal generated at the Wheatstone bridge 610 is received by an amplifier 620F. An amplified signal at the output of the amplifier 620F is received by an input port 632F of the ADC 630F. The ADC 630F digitizes the received signal and provides a stream of digitized data at output port 634F. The stream of digitized data is passed to a processor (e.g., 202 of FIG. 2) for further processing and/or transmission to a surveillance server (e.g., 60 of FIG. 1). In certain embodiments, the ADC 630F at its control data input port 636F receives a set of control data that configures one or more functionalities of the ADC 630F including, not limited to its sampling (digitization) rate and dynamic range.

With references to FIGS. 1, 2 and 4A-B, the monitor patch 20 worn by the patient 10 receives a signal from a temperature sensing element (e.g., a thermocouple and a thermistor) of the temperature probe 400, the signal responsive to a change in body temperature of the patient 10. The signal is amplified and digitized into a stream of data by the sensor interface circuit 214 as explained above with respect to FIGS. 6A-B. The digitized signal is then received by the processor 202. The processor 202 generates a sequence of temperature readings based on the digitized signal. The processor 202 is operatively connected to a wireless communication system (e.g., the wireless transceiver 207) which transmits data indicative of the patient's body temperature to the surveillance server 60 via the bridge 40. In certain embodiments, the processor 202 performs a number of temperature monitoring functions on the temperature readings to determine, inter alia, a high temperature condition and occurrence and loss of thermal contact between the patient 10 and the temperature probe 400.

FIG. 7 is a graph 700 of a measured temperature reading (T) versus time (t) for illustrating an exemplary temperature monitoring scheme according to certain aspects of the present disclosure. The graph 700 shows a low temperature limit (T_L) and a high temperature limit (T_H) that are used in the temperature monitoring scheme. For the purposes of illustration only without an intent to limit the scope of the present dis-

closure in any way, the exemplary temperature monitoring scheme will be described with reference to elements of FIGS. 4A,B. At $t=0$, a body-probe contact between the body of the patient 10 and the temperature probe 400 is made, e.g., by securing the sensing portion 420 of the temperature probe 400 within the axilla 12 of the patient 10. A processor (the processor 202 of FIG. 2) executing a control program in the monitoring device (e.g., the monitor patch 20) can recognize the body-probe contact by a number of different ways. For example, the recognition can be achieved from the temperature reading rising sharply past the low temperature limit (T_L) at a rate exceeding a first threshold rate of rise after having been below T_L at least once.

As seen in FIG. 7, the temperature reading rises from an initial (e.g., open-air) value (T_0) at $t=t_1$ to an equilibrium value (T_1) at $t=t_1$ when the temperature sensing element has reached a thermal equilibrium with the patient's body.

At $t=t_2$, the temperature reading begins to rise, indicating that the patient's body temperature is on the rise. At $t=t_3$, the temperature reading exceeds the high temperature limit (T_H). When this occurs, the processor executing control software in the monitoring device can invoke a high temperature handler routine in the control software and take a number of predetermined actions. For example, the processor can cause the transmitter 209 (FIG. 2) to start sending a signal indicative of the high temperature alarm condition to the surveillance server 60 either directly or via the bridge 40. In response, the surveillance server 60 can send a notification to a hospital system (e.g., the workstation 100 of FIG. 1). The monitor patch 20 can also set off an alarm, e.g., at the monitor patch 20 or at a stand alone monitoring unit or at a hospital system (e.g., the workstation 100 of FIG. 1), thereby notifying a nurse or other caregiver. The monitor patch 20 can enter into an alert operation mode from the normal operation mode and take and transmit the temperature readings (e.g., to the surveillance server 60) at a faster rate. For instance, the monitor patch 20 can take and transmit the temperature reading every 10 minutes during the normal operation mode, but does so every 2 minutes in the alert operation mode. In certain embodiments, the temperature monitoring scheme utilizes two high temperature limits (T_{H1} and T_{H2} , where $T_{H2} > T_{H1}$) and different sets of predetermined actions are performed depending on whether the temperature reading has exceeded only T_{H1} or both T_{H1} and T_{H2} .

In the illustrated example of FIG. 7, it is assumed that at $t=t_4$, a nurse who has been notified of the high temperature condition of the patient 10 has decided to administer a fever-reducing medication to the patient 10. Responding to the fever-reducing medication, the patient's body temperature reading begins to fall gradually and reach a relatively stable level below T_H .

However, at $t=t_5$, the body-probe contact is lost due to, e.g., the patient 10 opening the arm in a manner that causes the sensing portion 420 of the temperature probe 400 to be detached from the axilla 12 of the patient 10, or the temperature probe 400 accidentally falls off the patient's body. The loss of body-probe contact causes the temperature reading to fall towards a lower (e.g., open-air) value at a relatively sharp rate of decline. In certain embodiments of the temperature monitoring system 20A, the processor executing control software in the monitor patch 20 can detect the loss of body-probe contact by computing a rate of decline in the sequence of temperature readings and comparing the computed rate of decline to a threshold rate of decline. If the rate of decline exceeds the threshold rate of decline for a predetermined number of samples (e.g., 1-4), the processor determines that the body-probe contact has been lost and generates an indi-

cation of the loss of contact. In the illustrated example of FIG. 7, the loss of body-probe contact is detected at $t=t_6$. As can be seen from FIG. 7, the detection scheme based on the rate of decline described herein can detect the loss of contact earlier than a scheme relying on the temperature readings falling below the low temperature limit (T_L). The latter scheme would not detect the loss of contact until $t=t_7$.

In certain embodiments, an indication of the loss of contact is wirelessly transmitted to the bridge 40 to be sent to the surveillance server 60, and the surveillance server 60 then provides a notification of the loss of contact to a hospital system (e.g., the workstation 100 of FIG. 1). In other embodiments, in addition or in lieu of the wireless transmission of the indication, the monitor patch 20 itself may sound an alarm indicating the loss of contact to the patient 10 or a nurse or caregiver who is near the patient 10.

In certain embodiments, the monitor patch 20, after providing the indication, enters a sleep mode in which no additional temperature readings are taken. Alternatively, the monitor patch 20 can continue to take additional temperature readings to determine whether a new body-probe contact has been established.

FIG. 8A is diagram depicting a realistic temperature reading (T) versus time (t) graph 800A associated with a temperature monitoring system (e.g., 20) according to certain aspects of the present disclosure. The temperature readings have peaks (e.g., 811, 812) and valleys (e.g., 854, 855). The up-and-down fluctuations in the temperature readings can be caused by movements of a patient's arm (up and down/back and forth), for example. This is because arm movements can affect the quality of thermal contact between the sensing portion 420 of the temperature probe 400 and the axilla 12 of the patient 10. In general, when the temperature readings are rising rapidly as between reading 854 and reading 812, the rise may be attributable to a transition from a relatively poor thermal contact to a good thermal contact, e.g., by armpit closing. On the other hand, when the temperature readings are decreasing rapidly as between reading 853 and reading 854, the decrease may be attributable to a transition from a relatively good thermal contact to a poor thermal contact caused, e.g., by armpit opening up or the temperature probe being detached from the patient 10, thereby partially or fully exposing the sensing portion 420 to ambient air. A reading taken while the quality of thermal contact is poor is likely to be inaccurate, and thus it is desirable to identify occurrence of such a poor thermal contact so that inaccurate readings associated with the poor thermal contact may be rejected, and only valid temperature readings associated with a good thermal contact are reported, e.g., to the surveillance server 60. In addition, a prolonged loss of thermal contact may be detected and reported so that the patient 10 and/or a caregiver can be alerted. As used herein, the term "poor thermal contact" refers to partial or complete loss of contact between a temperature probe and a person to whom the temperature probe is supposed to be attached.

In certain aspects of the present disclosure, the monitoring system 20 achieves these objectives by adopting the following principles:

- 1) Only maximum readings (peaks or plateaus) are considered as potentially valid readings.
- 2) Temperature readings on a downward slope are considered to be associated with a poor thermal contact.
- 3) Given an almost impossible rate of decay of the core body temperature (e.g., -2 C/h), any peak or plateau below this threshold decay rate are rejected.

Applying these principles, a current (new) temperature reading (T_{NEW}) is reported as a new valid temperature reading

and replaces the current maximum temperature reading (T_{MAX}) if T_{NEW} fulfills at least one of the following acceptance conditions:

- Condition 1: Initial stabilization is just completed;
- Condition 2: ($T_{NEW} > T_{MAX}$); or
- Condition 3: ($T_{NEW} < T_{MAX}$) AND a peak/plateau (e.g., a local maximum) is detected AND a gradient condition, namely, the peak/plateau is at or above a threshold decay curve representing the threshold decay rate (e.g., e.g., -2 C/h), is satisfied.

Conversely, if the current temperature reading fails to satisfy all of these conditions, the reading is considered inaccurate and rejected, and the monitoring system 20 retains the current T_{MAX} as the currently effective temperature reading value.

FIG. 8B shows a graph 800B graphically illustrating an exemplary temperature monitoring algorithm based on the above-enumerated acceptance conditions according to certain aspects of the present disclosure. FIG. 9 is a flowchart illustrating an exemplary process 900 associated with the exemplary temperature monitoring algorithm of FIG. 8B according to certain aspects of the present disclosure. Indicated on the graph 800B are peak temperature readings (e.g., in between 811-819) that satisfy at least one of Conditions 1-3 enumerated above. Lines (straight or curvilinear) 831-839 represent currently effective temperature reading values, e.g., the values that the monitoring system 20 considers as the current axillary temperature of the patient 10. Saw-tooth-shaped curves 841-849 represent threshold decay curves generated based on a threshold decay rate (e.g., e.g., -2 C/h) discussed above with respect to Condition 3.

The algorithm 900 begins at start state 901 and proceeds to operation 910 in which a new temperature reading (T_{NEW}) is generated. By way of example, the T_{NEW} reading can be generated by a processor of the monitor patch 20 based on a signal generated by a temperature sensing element (e.g., 234A-D of FIG. 5A-D) of the temperature probe 400. As described above, the sensing element can be a thermocouple (234E of FIG. 6A), thermistor (234F of FIG. 6B) or any another temperature transducer configured to generate a signal responsive to a change in body temperature of a person to whom the temperature probe 400 is attached.

The algorithm 900 proceeds to decision state 920 in which a query is made as to whether an initial stabilization (e.g., a thermal equilibrium) has been completed for the temperature readings, e.g., after an initial attachment of the temperature probe 400 to the patient 10 or after a prolonged loss of thermal contact. This query is designed to determine whether the current T_{NEW} reading satisfies Condition 1, e.g., whether the monitoring has gone through or completed its stabilization phase.

In certain embodiments, the decision state 920 can involve, for example, determining whether the current and recent temperature readings have flattened out after a sharp increase by monitoring a slope (e.g., derivative) or an average of slopes of the temperature readings versus time. In other embodiments, the decision state 920 can involve waiting for a certain period of time (e.g. 15 minutes) before reporting a value, even though some peaks or plateaus might be found. After that stabilization period, the maximum value found will be reported as the first value. The purpose of the stabilization period is to reduce chances of having low peaks of temperature being reported right after system activation because of the fact that the gradient criterion cannot be applied (gradient criterion requires an initial value). For example, if a peak is found after activation, without the gradient criterion to discard it, it would be reported as a valid reading. Waiting 15 minutes and taking the maximum value offers better chances

of starting with a more accurate value. The above examples illustrate simple stabilization algorithms (e.g., waiting Z minutes and taking the maximum peak/plateau value). There can be different methods of obtaining a first reading such as using a predictive algorithm.

If answer to the query at the decision state **920** is NO, (initial stabilization not completed), the process **900** loops back to the operation **910** in which another T_{NEW} reading is generated. On the other hand, if answer to the query at the decision state **920** is YES (initial stabilization completed), the process **900** proceeds to operation **930** in which the new temperature reading (T_{NEW}) is reported, and to operation **940** in which the T_{NEW} reading is assigned to T_{MAX} . In the illustrated example of FIG. 8B, a first temperature reading **851** is taken at time **801**, e.g., after an initial attachment of the temperature probe **400** to the patient **10**, and an initial stabilization is determined to be completed at reading **811**.

The process **900** then proceeds to operation **950** in which another T_{NEW} reading is generated and then to decision state **960** in which a query is made as to whether the T_{NEW} reading obtained at the operation **950** is larger than the current maximum temperature reading (T_{MAX}), which at this point is equal to the value of the initially-stabilized temperature reading **811**. This query is designed to determine whether the current T_{NEW} reading satisfies Condition 2, namely $T_{NEW} > T_{MAX}$. If answer to the query is YES ($T_{NEW} > T_{MAX}$) the process **900** loops back to the operations **930** and **940** in which the current T_{NEW} reading is reported and assigned to T_{MAX} .

On the other hand, if the answer to the query at the decision state **960** is NO ($T_{NEW} \leq T_{MAX}$), the process **900** proceeds to decision states **970** in which a first query is made as to whether the new temperature reading corresponds to a peak (e.g., local maximum) or a plateau (e.g., relatively flat region after a local maximum), and, if so, a second query is made as to whether the peak/plateau satisfies the gradient condition, namely, whether the peak/plateau is at or above a corresponding one of the threshold decay curves **841-849** representing the threshold decay rate (e.g., -2 C/h). The first and second queries of the decision state **970** are designed to determine whether the current T_{NEW} reading satisfies Condition 3. In certain embodiments, the first query relating to the occurrence of a peak/plateau involves obtaining a sequence of temperature readings and retroactively identifying one of the readings corresponding to a local maximum. If the first and second queries of the decision state **970** are both satisfied (YES), the process **900** loops back to the operations **930** and **940** in which the current T_{NEW} reading is reported and assigned to T_{MAX} .

On the other hand, if at least one of the first and second queries is not satisfied (NO), the process **900** proceeds to another decision state **980** in which a query is made as to whether a maximum duration for the current T_{MAX} reading has been exceeded. This query detects a prolonged loss of thermal contact between the temperature probe **420** and the axilla **12** of the patient **10**. In certain exemplary embodiments, the maximum duration is preset at a value between about 10 and 30 minutes. If the query at the decision state **980** is NO (maximum duration not exceeded), the process **900** loops back to the operation **950** where another temperature reading is generated and then to decision state **960** and potentially to decision state **970** where Conditions 2 and 3, respectively, are checked. The algorithm maintains the current T_{MAX} reading, and the monitoring system **20** considers it as the currently effective temperature reading as indicated by the line **831**.

On the other hand, if the answer to the query at the decision state **980** is YES (maximum duration exceeded), the process **900** proceeds to operation **990** in which the loss of thermal

contact is reported (e.g., displayed on hospital system **100**) and then back to operations **950**, where a next T_{NEW} reading is taken.

In the illustrated example of FIG. 8B, temperature readings (e.g., **852, 853**) generated after the reading **811** do not satisfy the combination of first and second queries of the decision state **970**, and the maximum duration for the current T_{MAX} reading is exceeded at t_2 . The monitoring system **20** at or after t_2 reports the prolonged loss of thermal contact to, e.g., a database in the surveillance server **60** or the patient **10** and/or nurse/caregiver at operation **990**. After the reporting at operation **990**, the process **900** loops back to the operations **950**, where a next T_{NEW} reading is taken.

After determining (e.g., identifying) the initially-stabilized T_{NEW} reading **812**, the process **900** detects a series of new peak temperature readings **813-819** that satisfies Condition 2 (**813, 817, 819**) or Condition 3 (**814, 815, 816, 818**). Other T_{NEW} readings, such as readings **852, 853, 856**, however, are rejected because they do not satisfy either Condition 2 (T_{NEW} not greater than the current T_{MAX} **815**) or Condition 3 (T_{NEW} below the threshold decay curve **845**). Valid temperature readings do not always have to be local maxima. For example, after identifying the reading **812**, the algorithm associated with the process **900** can report a series of readings between t_4 and t_5 indicated by the curved line **832** as they satisfy Condition 2.

With reference to FIG. 2C, certain aspects of various temperature monitoring algorithms described herein are performed by the processor **202** (FIG. 2C) executing one or more sequences of one or more instructions using threshold limits contained in an internal machine-readable medium such as the internal memory **219** or the memory **210**. For example, the processor **202** can determine the loss of body-probe thermal contact by executing instructions contained in the internal memory **202** that involve computation of a rate of decline in temperature readings and comparison of the rate of decline to a threshold rate of decline stored in the memory **210** or generation of a threshold decay curve **841-849** based on a threshold decay rate and comparison of the current T_{NEW} reading to the threshold decay curve. The processor **202** may be a microprocessor, a microcontroller, a digital signal processor (DSP), or an application specific integrated circuit (ASIC) capable of executing computer instructions. Such instructions and/or threshold limits may be read into the memory **219, 210** from another machine-readable medium, such as a CD, flash memory, or a wireless transmission. Execution of the sequences of instructions contained in the memory **219** causes the processor **202** to perform the process steps described herein. One or more processors in a multi-processing arrangement may also be employed to execute the sequences of instructions contained in memory **219**. In alternative embodiments, hard-wired circuitry may be used in place of or in combination with software instructions to implement various embodiments. Thus, embodiments are not limited to any specific combination of hardware circuitry and software.

The term "machine-readable medium" as used herein refers to any medium that participates in providing instructions to processor **202** for execution or storing results of or parameters (e.g., variables or constants) for computations such as for the determination of the occurrence and loss of thermal contact between the patient's body and the temperature probe. Such a medium may take many forms, including, but not limited to, non-volatile media, volatile media, and transmission media. Non-volatile media include, for example, optical or magnetic disks, such as data storage device. Volatile media include dynamic memory, such as the

memory **210**. Transmission media include coaxial cables, copper wire, and fiber optics, including the wires that comprise bus **204**. Common forms of machine-readable media include, for example, floppy disk, a flexible disk, hard disk, magnetic tape, any other magnetic medium, a CD-ROM, DVD, any other optical medium, punch cards, paper tape, any other physical medium with patterns of holes, a RAM, a PROM, an EPROM, a FLASH EPROM, any other memory chip or cartridge, a carrier wave, or any other medium from which a computer can read.

In some embodiments, after the processor **202** programmatically generates data such as a sequence of temperature readings or indications of the high temperature condition or the loss of body-probe contact, such values can be either temporarily stored in the machine-readable medium such as the memory **210** until the values are transmitted via the wireless transmitter **209**. Instructions and/or various threshold limits (e.g., the threshold rates of rise and decline, the maximum duration for T_{MAX}) used by the temperature monitoring scheme of the present disclosure may be downloaded into the memory **210**, **219** via wireless transmission from an external device (e.g., the surveillance server **60** via the bridge **40**) via the receiver **206**.

The foregoing description is provided to enable any person skilled in the art to practice the various embodiments described herein. While the foregoing embodiments have been particularly described with reference to the various figures and embodiments, it should be understood that these are for illustration purposes only and should not be taken as limiting the scope of the claims.

The word “exemplary” is used herein to mean “serving as an example or illustration.” Any aspect or design described herein as “exemplary” is not necessarily to be construed as preferred or advantageous over other aspects or designs.

A reference to an element in the singular is not intended to mean “one and only one” unless specifically stated, but rather “one or more.” The term “some” refers to one or more. Underlined and/or italicized headings and subheadings are used for convenience only, do not limit the invention, and are not referred to in connection with the interpretation of the description of the invention. All structural and functional equivalents to the elements of the various embodiments of the invention described throughout this disclosure that are known or later come to be known to those of ordinary skill in the art are expressly incorporated herein by reference and intended to be encompassed by the invention. Moreover, nothing disclosed herein is intended to be dedicated to the public regardless of whether such disclosure is explicitly recited in the above description.

What is claimed is:

1. A temperature probe for measuring a temperature of an axilla of a person, comprising:
 - a first adhesive element;
 - a temperature sensing portion configured for placement within the axilla;
 - a second adhesive element;
 - a coiled electrical conductor coupled between the first adhesive element and the temperature sensing portion and having a length sufficient to extend from the temperature sensing portion to a first location outside of the axilla on a first side of the axilla; and
 - a spring element coupled between the temperature sensing portion and the second adhesive element and having a length sufficient to extend from the temperature sensing portion to a second location outside of the axilla on an opposing second side of the axilla,

wherein the coiled electrical conductor and the spring element are configured to cooperate with the first and second adhesive elements to hold the temperature sensing portion within the axilla when the first and second adhesive elements are attached at the first and second locations outside of the axilla.

2. The temperature probe of claim 1, further comprising:
 - a monitoring device; and
 - a flexible cable coupled between the first adhesive element and the monitoring device.

3. The temperature probe of claim 1, further comprising an electrical conductor configured for coupling between a monitoring device and the temperature sensing portion.

4. The temperature probe of claim 3, wherein the monitoring device is a vital-sign monitoring patch.

5. The temperature probe of claim 1, wherein the spring element comprises at least one coiled section acting as a spring.

6. The temperature probe of claim 1, wherein the temperature sensing element comprises a thermocouple.

7. The temperature probe of claim 1, wherein the temperature sensing element comprises a thermistor.

8. The temperature probe of claim 1, wherein the temperature sensing element comprises a resistance temperature detector (RTD), the RTD comprising platinum.

9. A system for monitoring a temperature of a person having an axilla disposed between a chest and a back, the system comprising:

- a first adhesive element;
- a temperature sensing element;
- a second adhesive element;
- a coiled electrical conductor coupled between the first adhesive element and the temperature sensing element;
- a spring element coupled between the temperature sensing element and the second adhesive element; and
- a monitoring patch comprising an adhesive backing for attachment to the person, the monitoring patch configured to receive signals from the temperature sensing element via the coiled electrical conductor, the monitoring device including a wireless communication system to wirelessly transmit readings based on the received signals; and

wherein the coiled electrical conductor and the spring element each have a sufficient length such that the temperature sensing element is retained in the axilla by the first adhesive element, the second adhesive element, the coiled electrical conductor and the spring element when the first adhesive element is attached to a first point on the person that is external to the axilla on one of the chest and the back of the person and the second adhesive element is attached to a second point on the person that is external to the axilla on the other of the chest and the back of the person.

10. The system of claim 9, wherein the monitoring device is a vital-sign monitor patch, the monitor patch configured to measure body temperature and at least one other vital sign of the person wearing the monitor patch.

11. The system of claim 10, wherein the at least one other vital sign comprises at least one of pulse rate, blood pressure, and respiratory rate.

12. The system of claim 9, further comprising an additional coiled electrical conductor coupled between the monitoring device and the first adhesive element.

13. The system of claim 12 wherein the system is configured to remain attached to the person for a period of time.

14. The system of claim 12, wherein the spring element comprises a coiled section.

15. A method of monitoring a temperature of an axilla of a person, comprising:

placing a sensing portion of a temperature probe within the axilla of the person,

attaching a first adhesive element to the person at a first location on the person, wherein the first location is external to the axilla;

attaching a second adhesive element at a second location on the person, wherein the second location is external to the axilla and on an opposing side of the axilla; and

retaining the sensing portion within the axilla with a coiled electrical conductor coupled between the first adhesive element and the sensing portion and a spring element coupled between the second adhesive element and the sensing portion.

16. The method of claim **15**, further comprising wirelessly transmitting readings representative of sensed body temperatures of the person as determined by a monitoring device based on signals received from the temperature sensing element.

17. The method of claim **16**, wherein the monitoring device is a vital-sign monitoring patch, the monitor patch configured to measure body temperature and at least one other vital sign of the person wearing the monitor patch.

18. The method of claim **17**, wherein the at least one other vital sign comprises at least one of pulse rate, blood pressure, and respiratory rate.

* * * * *

专利名称(译)	温度探头适合腋窝读数		
公开(公告)号	US9420952	公开(公告)日	2016-08-23
申请号	US12/844775	申请日	2010-07-27
申请(专利权)人(译)	CAREFUSION 303 , INC.		
当前申请(专利权)人(译)	CAREFUSION 303 , INC.		
[标]发明人	PAQUET PIERRE DIALLO BINTA RAPTIS MARK		
发明人	PAQUET, PIERRE DIALLO, BINTA RAPTIS, MARK		
IPC分类号	A61B5/00 A61B5/01 A61B5/0205		
CPC分类号	A61B5/0008 A61B5/01 A61B5/02055 A61B5/6813 A61B5/6833 A61B2562/0271		
代理机构(译)	MCDERMOTT WILL & EMERY LLP		
其他公开文献	US20120029310A1		
外部链接	Espacenet USPTO		

摘要(译)

公开了监测人的腋温的系统和方法。温度探针的一部分设置在人的腋窝内。温度探测器包括布线部分和主体连接部分以及布线和主体连接部分之间的感测部分。传感部分包括温度传感元件。布线部分耦合到监控装置并且包括具有第一端和第二端的导体，第一端耦合到温度感测元件，第二端连接到监控装置。主体连接部分的至少一部分附接到人的第二主体部分，使得感测部分保持在腋窝内。

