



US008228181B2

(12) **United States Patent**  
**Al-Ali**

(10) **Patent No.:** **US 8,228,181 B2**  
(45) **Date of Patent:** **\*Jul. 24, 2012**

(54) **PHYSIOLOGICAL TREND MONITOR**

(56) **References Cited**

(75) Inventor: **Ammar Al-Ali**, San Juan Capistrano, CA (US)

U.S. PATENT DOCUMENTS

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **13/018,334**

(22) Filed: **Jan. 31, 2011**

(65) **Prior Publication Data**

US 2011/0124990 A1 May 26, 2011

**Related U.S. Application Data**

(63) Continuation of application No. 12/070,061, filed on Feb. 12, 2008, now Pat. No. 7,880,606, which is a continuation of application No. 11/717,591, filed on Mar. 13, 2007, now Pat. No. 7,355,512, which is a continuation of application No. 11/405,815, filed on Apr. 18, 2006, now Pat. No. 7,190,261, which is a continuation of application No. 10/975,860, filed on Oct. 28, 2004, now Pat. No. 7,030,749, which is a continuation of application No. 10/351,735, filed on Jan. 24, 2003, now Pat. No. 6,822,564.

(60) Provisional application No. 60/351,510, filed on Jan. 24, 2002.

(51) **Int. Cl.**  
**G08B 29/00** (2006.01)

(52) **U.S. Cl.** ..... **340/511**; 340/539.12; 340/573.1;  
600/322; 600/323

(58) **Field of Classification Search** ..... 340/511,  
340/539.12, 573.1; 600/322, 323

See application file for complete search history.

4,960,128 A	10/1990	Gordon et al.
4,964,408 A	10/1990	Hink et al.
5,041,187 A	8/1991	Hink et al.
5,069,213 A	12/1991	Polczynski
5,163,438 A	11/1992	Gordon et al.
5,319,355 A	6/1994	Russek
5,337,744 A	8/1994	Branigan
5,341,805 A	8/1994	Stavridi et al.
D353,195 S	12/1994	Savage et al.
D353,196 S	12/1994	Savage et al.
5,377,676 A	1/1995	Vari et al.
D359,546 S	6/1995	Savage et al.
5,431,170 A	7/1995	Mathews
D361,840 S	8/1995	Savage et al.
D362,063 S	9/1995	Savage et al.
5,452,717 A	9/1995	Branigan et al.
D363,120 S	10/1995	Savage et al.
5,456,252 A	10/1995	Vari et al.
5,479,934 A	1/1996	Imran
5,482,036 A	1/1996	Diab et al.
5,490,505 A	2/1996	Diab et al.
5,494,043 A	2/1996	O'Sullivan et al.
5,533,511 A	7/1996	Kaspari et al.

(Continued)


*Primary Examiner* — John A Tweel, Jr.

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear LLP

(57) **ABSTRACT**

A physiological trend monitor has a sensor signal responsive to multiple wavelengths of light transmitted into a tissue site. The transmitted light is detected after attenuation by pulsatile blood flow within the tissue site. A processor has an input responsive to the sensor signal and a physiological parameter output. Features are extracted from the physiological parameter output. Criteria are applied to the features. An alarm output is generated when the criteria are satisfied.

**14 Claims, 9 Drawing Sheets**

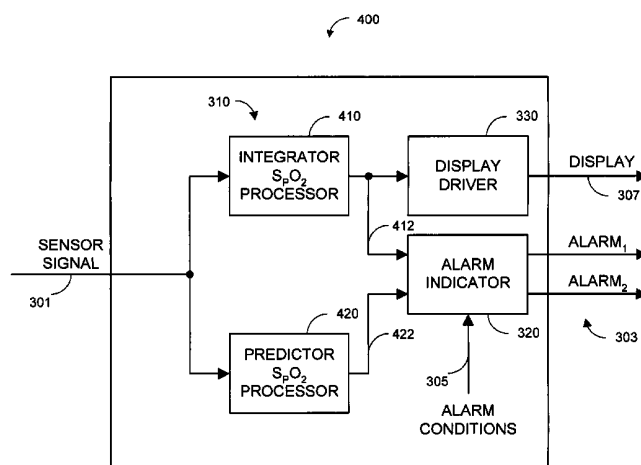

## U.S. PATENT DOCUMENTS

5,534,851	A	7/1996	Russek	6,515,273	B2	2/2003	Al-Ali
5,561,275	A	10/1996	Savage et al.	6,519,487	B1	2/2003	Parker
5,562,002	A	10/1996	Lalin	6,525,386	B1	2/2003	Mills et al.
5,590,649	A	1/1997	Caro et al.	6,526,300	B1	2/2003	Kiani et al.
5,602,924	A	2/1997	Durand et al.	6,541,756	B2	4/2003	Schulz et al.
5,632,272	A	5/1997	Diab et al.	6,542,764	B1	4/2003	Al-Ali et al.
5,638,816	A	6/1997	Kiani-Azarbayjany et al.	6,580,086	B1	6/2003	Schulz et al.
5,638,818	A	6/1997	Diab et al.	6,584,336	B1	6/2003	Ali et al.
5,645,440	A	7/1997	Tobler et al.	6,595,316	B2	7/2003	Cybulski et al.
5,685,299	A	11/1997	Diab et al.	6,597,932	B2	7/2003	Tian et al.
D393,830	S	4/1998	Tobler et al.	6,597,933	B2	7/2003	Kiani et al.
5,743,262	A	4/1998	Lepper, Jr. et al.	6,606,511	B1	8/2003	Ali et al.
5,758,644	A	6/1998	Diab et al.	6,632,181	B2	10/2003	Flaherty et al.
5,760,910	A	6/1998	Lepper, Jr. et al.	6,639,668	B1	10/2003	Trepagnier
5,769,785	A	6/1998	Diab et al.	6,640,116	B2	10/2003	Diab
5,782,757	A	7/1998	Diab et al.	6,643,530	B2	11/2003	Diab et al.
5,785,659	A	7/1998	Caro et al.	6,650,917	B2	11/2003	Diab et al.
5,791,347	A	8/1998	Flaherty et al.	6,654,624	B2	11/2003	Diab et al.
5,810,734	A	9/1998	Caro et al.	6,658,276	B2	12/2003	Kiani et al.
5,823,950	A	10/1998	Diab et al.	6,661,161	B1	12/2003	Lanzo et al.
5,830,131	A	11/1998	Caro et al.	6,671,531	B2	12/2003	Al-Ali et al.
5,833,618	A	11/1998	Caro et al.	6,678,543	B2	1/2004	Diab et al.
5,860,919	A	1/1999	Kiani-Azarbayjany et al.	6,684,090	B2	1/2004	Ali et al.
5,890,929	A	4/1999	Mills et al.	6,684,091	B2	1/2004	Parker
5,904,654	A	5/1999	Wohltmann et al.	6,697,656	B1	2/2004	Al-Ali
5,919,134	A	7/1999	Diab	6,697,657	B1	2/2004	Shehada et al.
5,934,925	A	8/1999	Tobler et al.	6,697,658	B2	2/2004	Al-Ali
5,940,182	A	8/1999	Lepper, Jr. et al.	RE38,476	E	3/2004	Diab et al.
5,995,855	A	11/1999	Kiani et al.	6,699,194	B1	3/2004	Diab et al.
5,997,343	A	12/1999	Mills et al.	6,714,804	B2	3/2004	Al-Ali et al.
6,002,952	A	12/1999	Diab et al.	RE38,492	E	4/2004	Diab et al.
6,011,986	A	1/2000	Diab et al.	6,721,582	B2	4/2004	Trepagnier et al.
6,027,452	A	2/2000	Flaherty et al.	6,721,585	B1	4/2004	Parker
6,036,642	A	3/2000	Diab et al.	6,725,075	B2	4/2004	Al-Ali
6,045,509	A	4/2000	Caro et al.	6,728,560	B2	4/2004	Kollias et al.
6,067,462	A	5/2000	Diab et al.	6,735,459	B2	5/2004	Parker
6,081,735	A	6/2000	Diab et al.	6,745,060	B2	6/2004	Diab et al.
6,088,607	A	7/2000	Diab et al.	6,760,607	B2	7/2004	Al-Ali
6,110,522	A	8/2000	Lepper, Jr. et al.	6,770,028	B1	8/2004	Ali et al.
6,124,597	A	9/2000	Shehada	6,771,994	B2	8/2004	Kiani et al.
6,128,521	A	10/2000	Marro et al.	6,792,300	B1	9/2004	Diab et al.
6,129,675	A	10/2000	Jay	6,813,511	B2	11/2004	Diab et al.
6,144,868	A	11/2000	Parker	6,816,741	B2	11/2004	Diab
6,151,516	A	11/2000	Kiani-Azarbayjany et al.	6,822,564	B2	11/2004	Al-Ali
6,152,754	A	11/2000	Gerhardt et al.	6,826,419	B2	11/2004	Diab et al.
6,157,850	A	12/2000	Diab et al.	6,830,711	B2	12/2004	Mills et al.
6,165,005	A	12/2000	Mills et al.	6,850,787	B2	2/2005	Weber et al.
6,184,521	B1	2/2001	Coffin, IV et al.	6,850,788	B2	2/2005	Al-Ali
6,206,830	B1	3/2001	Diab et al.	6,852,083	B2	2/2005	Caro et al.
6,229,856	B1	5/2001	Diab et al.	6,861,639	B2	3/2005	Al-Ali
6,232,609	B1	5/2001	Snyder et al.	6,898,452	B2	5/2005	Al-Ali et al.
6,236,872	B1	5/2001	Diab et al.	6,920,345	B2	7/2005	Al-Ali et al.
6,241,683	B1	6/2001	Macklem et al.	6,931,268	B1	8/2005	Kiani-Azarbayjany et al.
6,253,097	B1	6/2001	Aronow et al.	6,934,570	B2	8/2005	Kiani et al.
6,256,523	B1	7/2001	Diab et al.	6,939,305	B2	9/2005	Flaherty et al.
6,263,222	B1	7/2001	Diab et al.	6,943,348	B1	9/2005	Coffin, IV
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,950,687	B2	9/2005	Al-Ali
6,280,213	B1	8/2001	Tobler et al.	6,961,598	B2	11/2005	Diab
6,285,896	B1	9/2001	Tobler et al.	6,970,792	B1	11/2005	Diab
6,301,493	B1	10/2001	Marro et al.	6,979,812	B2	12/2005	Al-Ali
6,317,627	B1	11/2001	Ennen et al.	6,985,764	B2	1/2006	Mason et al.
6,321,100	B1	11/2001	Parker	6,993,371	B2	1/2006	Kiani et al.
6,325,761	B1	12/2001	Jay	6,996,427	B2	2/2006	Ali et al.
6,334,065	B1	12/2001	Al-Ali et al.	6,999,904	B2	2/2006	Weber et al.
6,343,224	B1	1/2002	Parker	7,003,338	B2	2/2006	Weber et al.
6,349,228	B1	2/2002	Kiani et al.	7,003,339	B2	2/2006	Diab et al.
6,360,114	B1	3/2002	Diab et al.	7,015,451	B2	3/2006	Dalke et al.
6,368,283	B1	4/2002	Xu et al.	7,024,233	B2	4/2006	Ali et al.
6,371,921	B1	4/2002	Caro et al.	7,027,849	B2	4/2006	Al-Ali
6,377,829	B1	4/2002	Al-Ali	7,030,749	B2	4/2006	Al-Ali
6,388,240	B2	5/2002	Schulz et al.	7,039,449	B2	5/2006	Al-Ali
6,397,091	B2	5/2002	Diab et al.	7,041,060	B2	5/2006	Flaherty et al.
6,430,437	B1	8/2002	Marro	7,044,918	B2	5/2006	Diab
6,430,525	B1	8/2002	Weber et al.	7,067,893	B2	6/2006	Mills et al.
6,463,311	B1	10/2002	Diab	7,096,052	B2	8/2006	Mason et al.
6,470,199	B1	10/2002	Kopotic et al.	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,501,975	B2	12/2002	Diab et al.	7,132,641	B2	11/2006	Schulz et al.
6,505,059	B1	1/2003	Kollias et al.	7,142,901	B2	11/2006	Kiani et al.
				7,149,561	B2	12/2006	Diab

7,186,966 B2	3/2007	Al-Ali	7,471,971 B2	12/2008	Diab et al.
7,190,261 B2	3/2007	Al-Ali	7,483,729 B2	1/2009	Al-Ali et al.
7,215,984 B2	5/2007	Diab	7,483,730 B2	1/2009	Diab et al.
7,215,986 B2	5/2007	Diab	7,489,958 B2	2/2009	Diab et al.
7,221,971 B2	5/2007	Diab	7,496,391 B2	2/2009	Diab et al.
7,225,006 B2	5/2007	Al-Ali et al.	7,496,393 B2	2/2009	Diab et al.
7,225,007 B2	5/2007	Al-Ali	D587,657 S	3/2009	Al-Ali et al.
RE39,672 E	6/2007	Shehada et al.	7,499,741 B2	3/2009	Diab et al.
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,499,835 B2	3/2009	Weber et al.
7,245,953 B1	7/2007	Parker	7,500,950 B2	3/2009	Al-Ali et al.
7,254,429 B2	8/2007	Schurman et al.	7,509,154 B2	3/2009	Diab et al.
7,254,431 B2	8/2007	Al-Ali	7,509,494 B2	3/2009	Al-Ali
7,254,433 B2	8/2007	Diab et al.	7,510,849 B2	3/2009	Schurman et al.
7,254,434 B2	8/2007	Schulz et al.	7,526,328 B2	4/2009	Diab et al.
7,272,425 B2	9/2007	Al-Ali	7,530,942 B1	5/2009	Diab
7,274,955 B2	9/2007	Kiani et al.	7,530,949 B2	5/2009	Al Ali et al.
D554,263 S	10/2007	Al-Ali	7,530,955 B2	5/2009	Diab et al.
7,280,858 B2	10/2007	Al-Ali et al.	7,563,110 B2	7/2009	Al-Ali et al.
7,289,835 B2	10/2007	Mansfield et al.	7,596,398 B2	9/2009	Al-Ali et al.
7,292,883 B2	11/2007	De Felice et al.	7,618,375 B2	11/2009	Flaherty
7,295,866 B2	11/2007	Al-Ali	D606,659 S	12/2009	Kiani et al.
7,328,053 B1	2/2008	Diab et al.	7,647,083 B2	1/2010	Al-Ali et al.
7,332,784 B2	2/2008	Mills et al.	D609,193 S	2/2010	Al-Ali et al.
7,340,287 B2	3/2008	Mason et al.	D614,305 S	4/2010	Al-Ali et al.
7,341,559 B2	3/2008	Schulz et al.	RE41,317 E	5/2010	Parker
7,343,186 B2	3/2008	Lamego et al.	7,729,733 B2	6/2010	Al-Ali et al.
D566,282 S	4/2008	Al-Ali et al.	7,734,320 B2	6/2010	Al-Ali
7,355,512 B1	4/2008	Al-Ali	7,761,127 B2	7/2010	Al-Ali et al.
7,356,365 B2	4/2008	Schurman	7,761,128 B2	7/2010	Al-Ali et al.
7,371,981 B2	5/2008	Abdul-Hafiz	7,764,982 B2	7/2010	Dalke et al.
7,373,193 B2	5/2008	Al-Ali et al.	D621,516 S	8/2010	Kiani et al.
7,373,194 B2	5/2008	Weber et al.	7,791,155 B2	9/2010	Diab
7,376,453 B1	5/2008	Diab et al.	7,801,581 B2	9/2010	Diab
7,377,794 B2	5/2008	Al Ali et al.	7,822,452 B2	10/2010	Schurman et al.
7,377,899 B2	5/2008	Weber et al.	RE41,912 E	11/2010	Parker
7,383,070 B2	6/2008	Diab et al.	7,844,313 B2	11/2010	Kiani et al.
7,415,297 B2	8/2008	Al-Ali et al.	7,844,314 B2	11/2010	Al-Ali
7,428,432 B2	9/2008	Ali et al.	7,844,315 B2	11/2010	Al-Ali
7,438,683 B2	10/2008	Al-Ali et al.	7,865,222 B2	1/2011	Weber et al.
7,440,787 B2	10/2008	Diab	7,873,497 B2	1/2011	Weber et al.
7,454,240 B2	11/2008	Diab et al.	7,880,606 B2 *	2/2011	Al-Ali ..... 340/511
7,467,002 B2	12/2008	Weber et al.			
7,469,157 B2	12/2008	Diab et al.			
7,471,969 B2	12/2008	Diab et al.			

\* cited by examiner

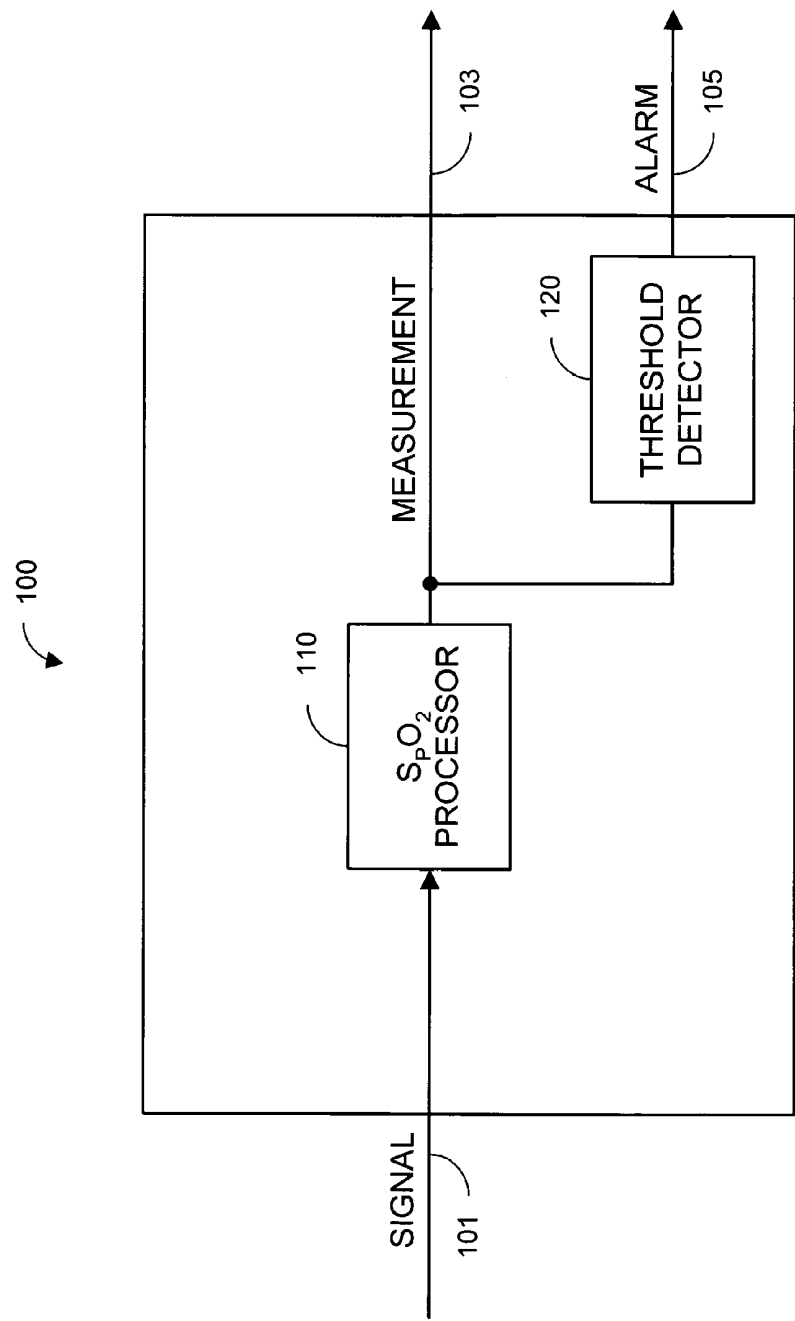


FIG. 1 (Prior Art)

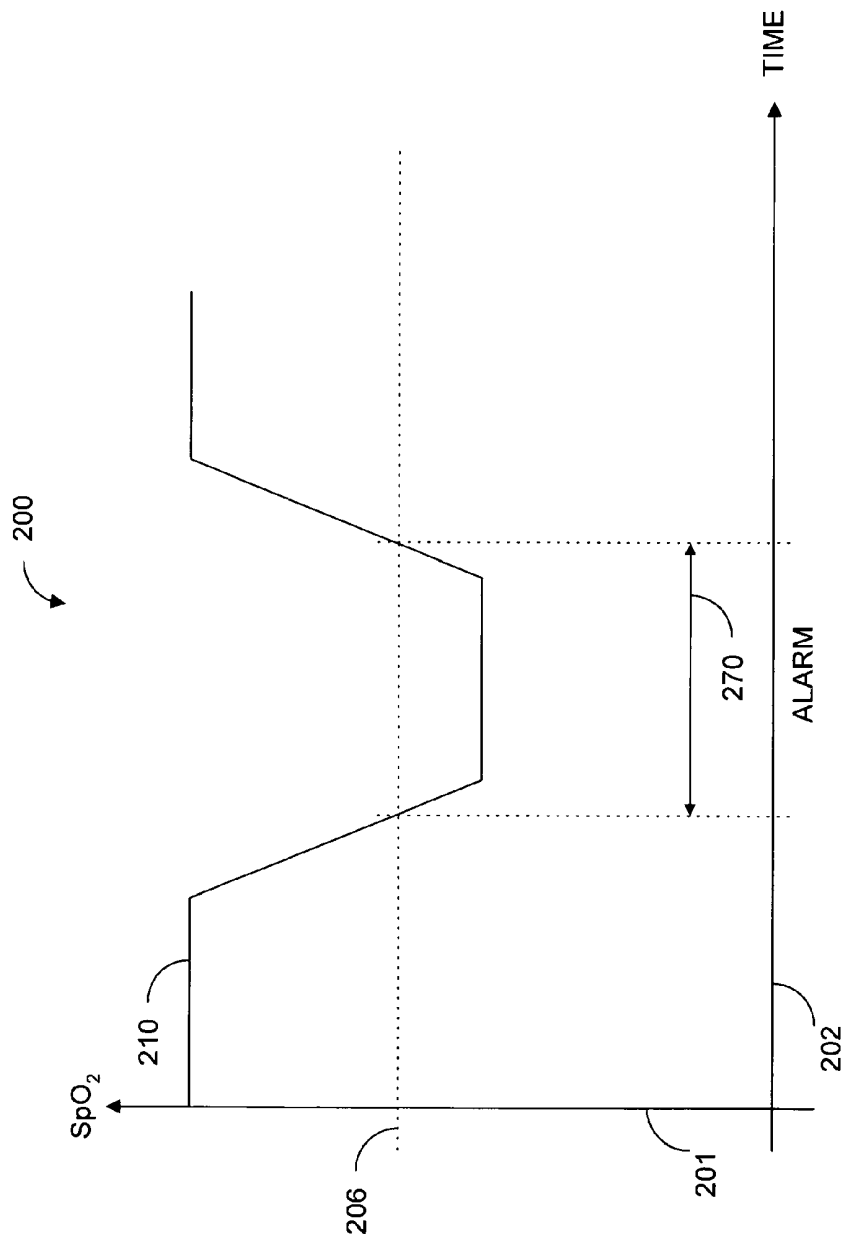


FIG. 2

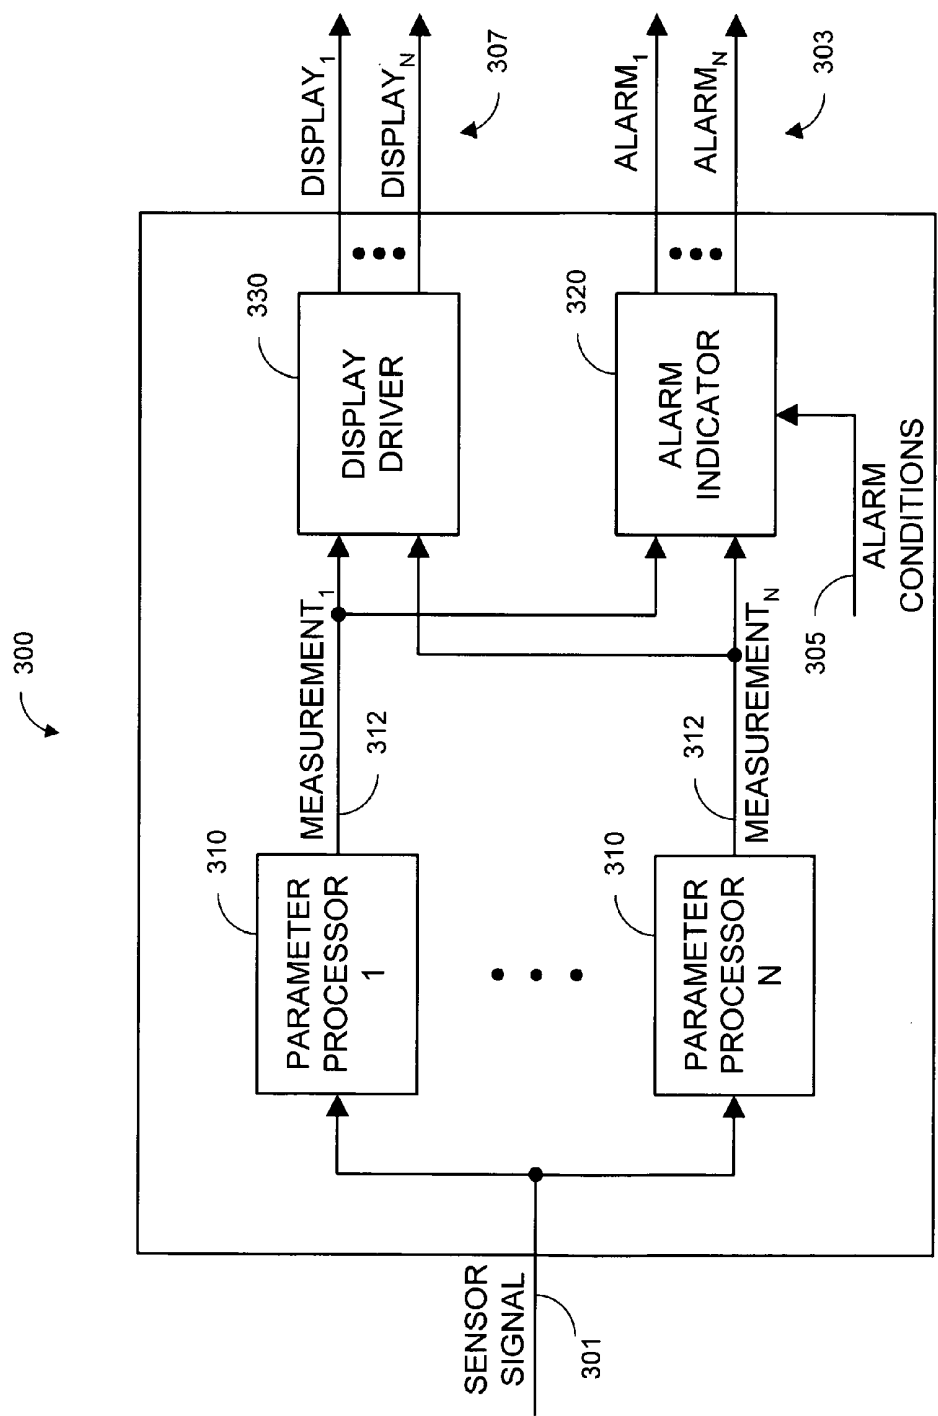


FIG. 3

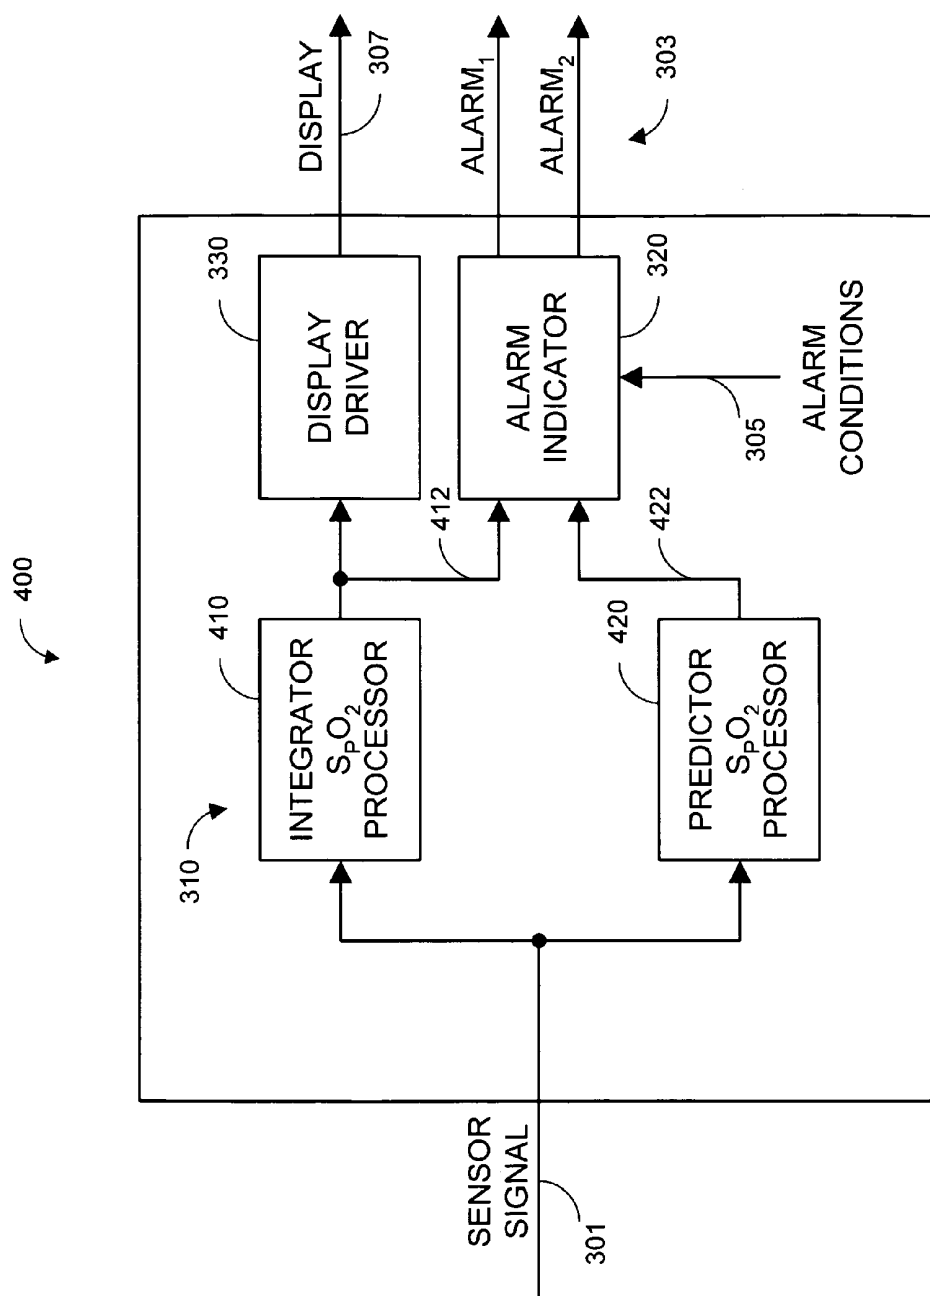


FIG. 4

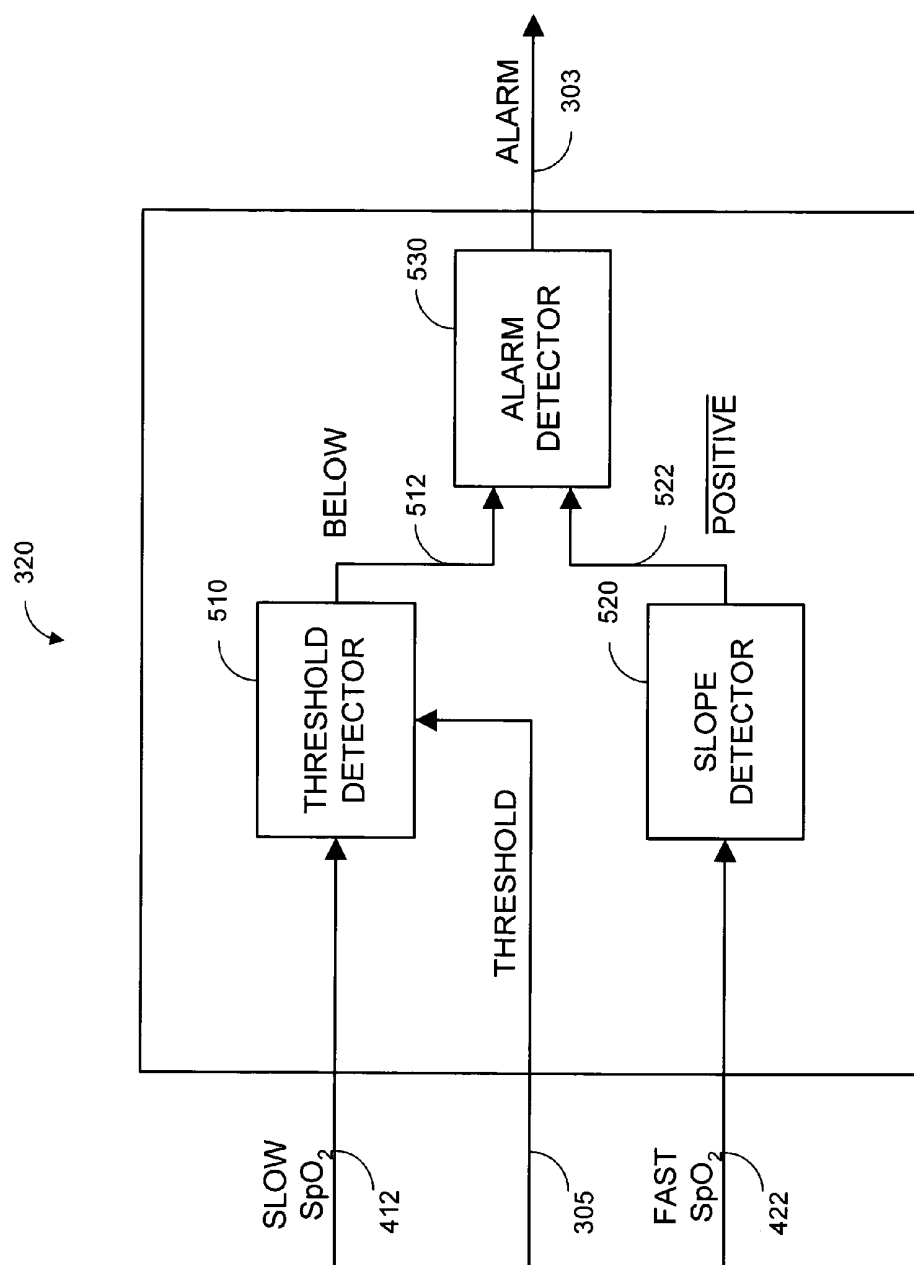


FIG. 5



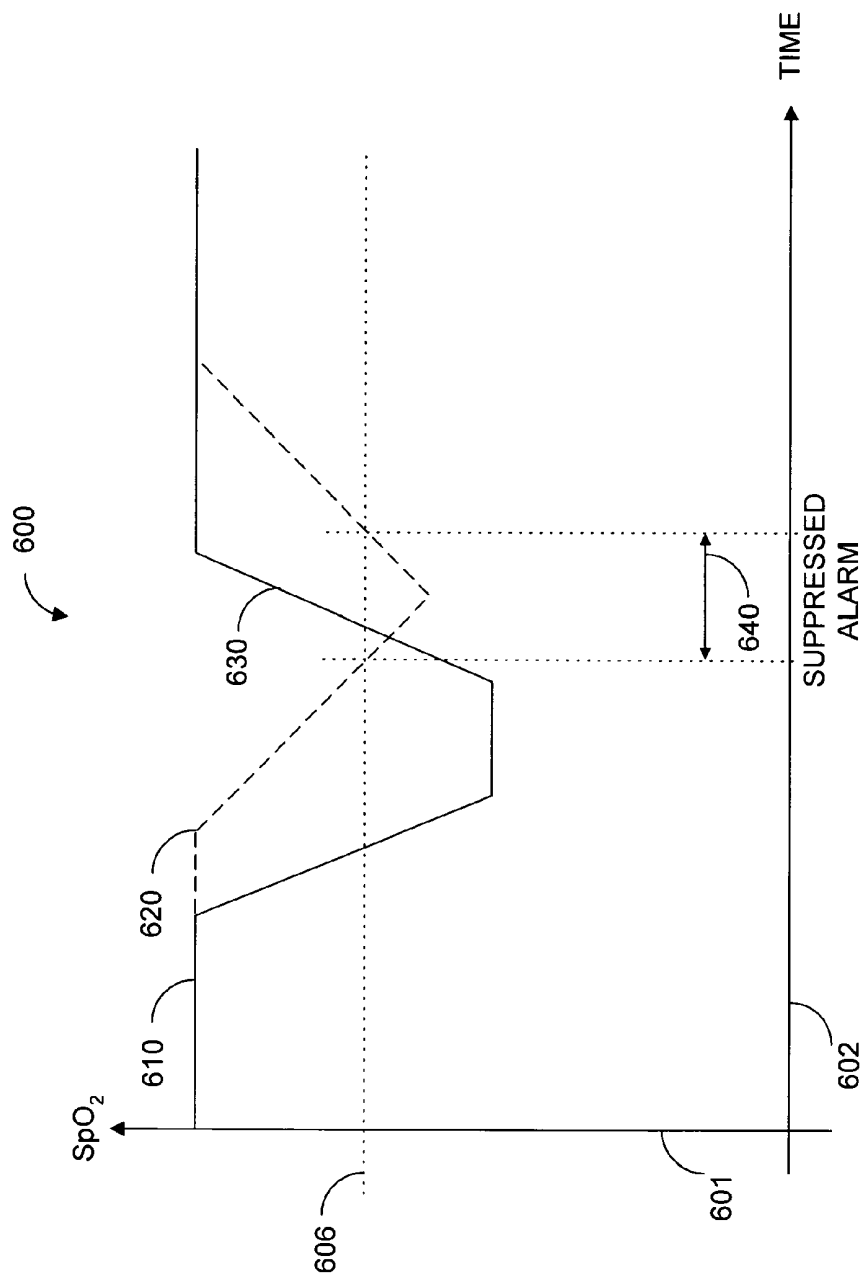


FIG. 6A

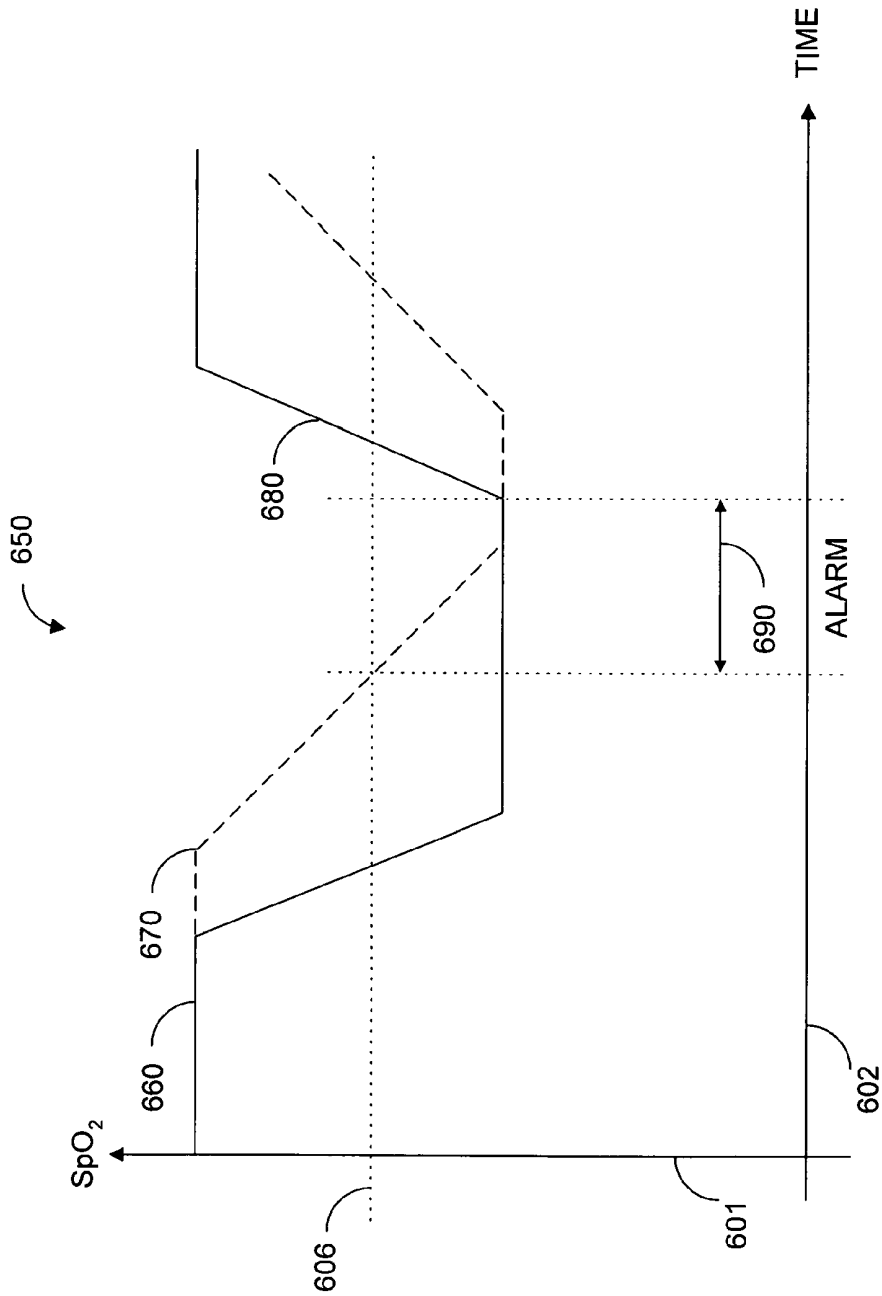


FIG. 6B

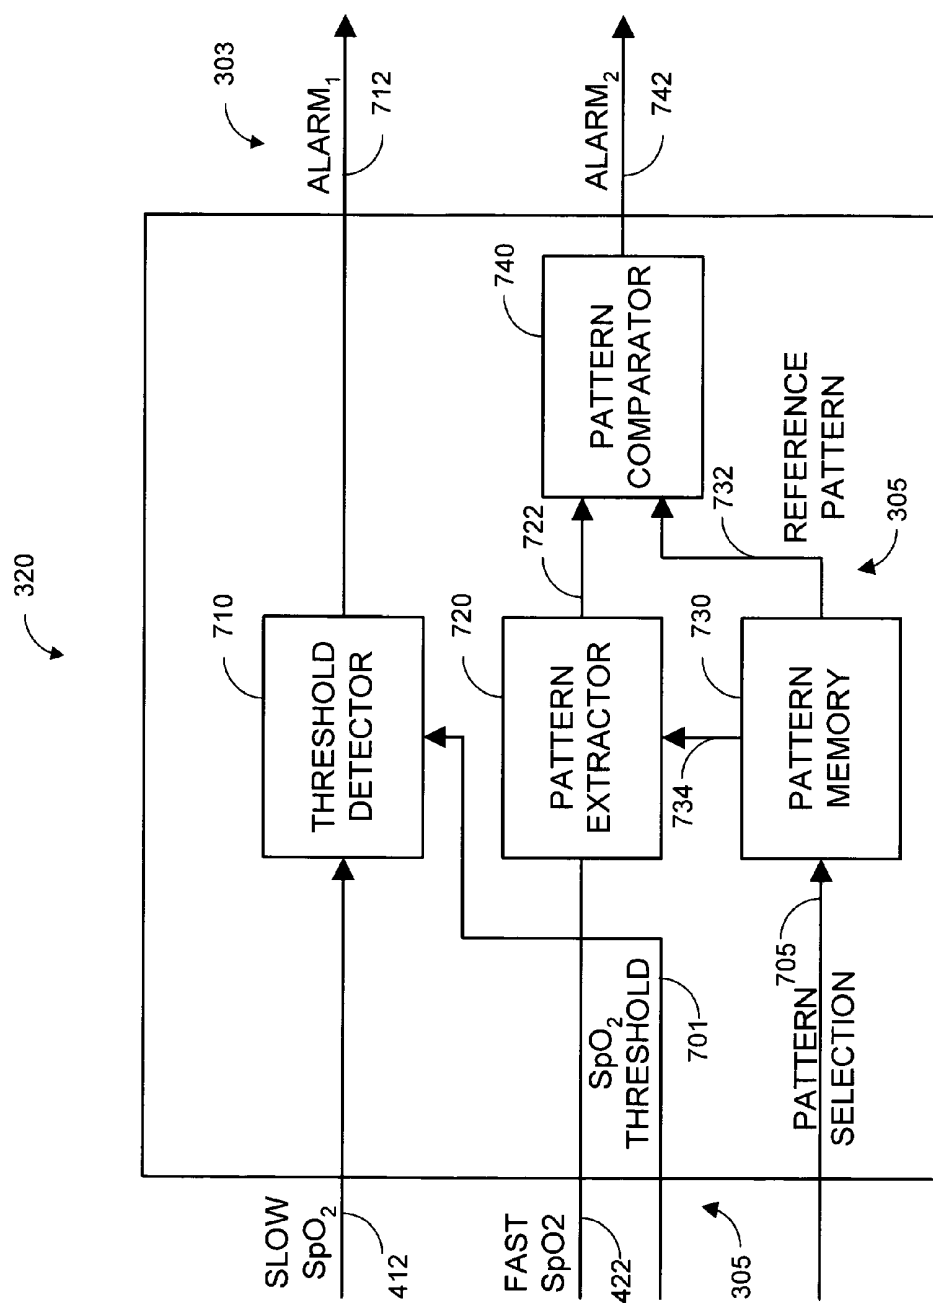


FIG. 7

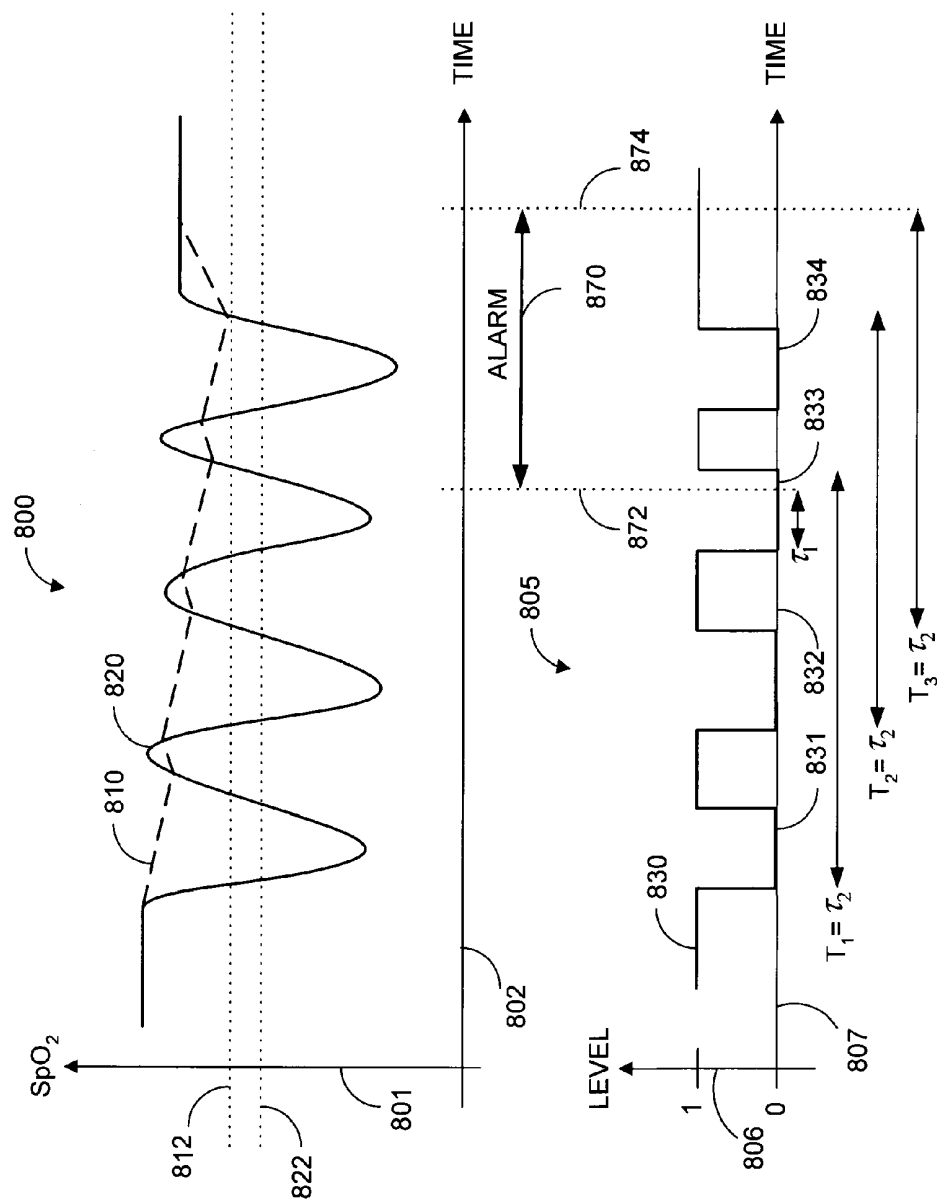


FIG. 8

## PHYSIOLOGICAL TREND MONITOR

## REFERENCE TO RELATED APPLICATIONS

The present application claims priority benefit under 35 U.S.C. §120 to, and is a continuation of, U.S. patent application Ser. No. 12/070,061, filed Feb. 12, 2008, now U.S. Pat. No. 7,880,606, entitled "Physiological Trend Monitor," which is a continuation of U.S. patent application Ser. No. 11/717,591, filed Mar. 13, 2007, now U.S. Pat. No. 7,355,512, entitled "Parallel Alarm Processor," which is a continuation of U.S. patent application Ser. No. 11/405,815, filed Apr. 18, 2006, now U.S. Pat. No. 7,190,261, entitled "Arrhythmia Alarm Processor," which is a continuation of U.S. patent application Ser. No. 10/975,860, filed Oct. 28, 2004, now U.S. Pat. No. 7,030,749, entitled "Parallel Measurement Alarm Processor," which is a continuation of U.S. patent application Ser. No. 10/351,735, filed Jan. 24, 2003, now U.S. Pat. No. 6,822,564, entitled "Parallel Measurement Alarm Processor," which claims priority benefit under 35 U.S.C. §119(e) from U.S. Provisional Application No. 60/351,510, filed Jan. 24, 2002, entitled "Parallel Measurement Alarm Processor." The present application also incorporates the foregoing utility disclosures herein by reference.

## BACKGROUND OF THE INVENTION

Physiological measurement instruments employed in healthcare environments often feature visual and audible alarm mechanisms that alert a caregiver when a patient's vital signs are outside of predetermined limits. One example is a pulse oximeter, which measures the oxygen saturation level of arterial blood, an indicator of oxygen supply. A typical pulse oximeter displays a numerical readout of the patient's oxygen saturation, a numerical readout of pulse rate, and a plethysmograph, which is indicative of a patient's pulse. In addition, a pulse oximeter provides an alarm that warns of a potential desaturation event.

FIG. 1 illustrates a prior art pulse oximeter portion **100** having a signal input **101** and generating an oxygen saturation measurement output **103** and an alarm output **105**. The pulse oximeter portion **100** has an oxygen saturation (SPO.sub.2) processor **110** and an associated threshold detector **120**. The SPO.sub.2 processor **110** derives an oxygen saturation measurement from the signal input **101**. The signal input **101** is typically an amplified, filtered, digitized and demodulated sensor signal. A sensor emits both red and infrared (IR) wavelength light, which is transmitted through a patient's tissue, detected and input to the pulse oximeter. The pulse oximeter calculates a normalized ratio (AC/DC) of the detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on a ratio of these normalized ratios, as is well-known in the art. The oxygen saturation measurement output **103** is typically a digital signal that is then communicated to a display.

FIG. 2 illustrates the operation of a conventional threshold detector **120** (FIG. 1) utilizing a graph **200** of oxygen saturation **201** versus time **202**. The graph **200** displays a particular oxygen saturation measurement **210** corresponding to the measurement output **103** (FIG. 1) and a predetermined alarm threshold **206**. During an alarm time period **270** when the measured oxygen saturation **210** is below the threshold **206**, an alarm output **105** (FIG. 1) is generated, which triggers a caregiver alert. Adjusting the threshold **206** to a lower value of oxygen saturation **201** reduces the probability of an alarm, i.e. reduces the probability of a false alarm and increases the probability of a missed event. Likewise, adjusting the thresh-

old **206** to a higher value of oxygen saturation **201** increases the probability of an alarm, i.e. increases the probability of a false alarm and decreases the probability of a missed event.

## SUMMARY OF THE INVENTION

One aspect of a physiological trend monitor comprises transmitting light into a patient tissue site, generating a sensor signal, detecting a blood parameter trend according to the sensor signal and generating an alarm according to the blood parameter trend. The transmitted light has multiple wavelengths. The sensor signal is responsive to the light after attenuation by pulsatile arterial blood flow within the tissue site. In various embodiments, the detecting comprises deriving a curve-fitting blood parameter measurement. A blood parameter slope is calculated from the blood parameter measurement. The alarm is responsive to a negative value of the blood parameter slope. A smoothed blood parameter measurement is derived. A threshold value is set for the smoothed blood parameter measurement. The alarm is responsive to the smoothed blood parameter measurement crossing the threshold value.

Another aspect of a physiological trend monitor comprises a sensor signal responsive to multiple wavelengths of light transmitted into a tissue site and detected after attenuation by pulsatile blood flow within the tissue site. A processor has an input responsive to the sensor signal and a physiological parameter output. Features are extracted from the physiological parameter output. Criteria are applied to the features. An alarm output is generated when the criteria are satisfied. In various embodiments a pattern memory stores feature values and a comparator compares the features with the stored feature values. The criteria determine a match between the features and the stored feature values so as to trigger the alarm output. At least one of the features relate to the number of threshold crossings over a specified time period. At least one of the features relate to a duration of a threshold crossing by the physiological parameter output. At least one of the features relate to a trend in the physiological parameter and a slope of that trend over a specified time period.

A further aspect of a physiological trend monitor comprises a detector responsive to multiple wavelengths of light transmitted into a tissue site after attenuation by pulsatile blood flow within the tissue site so as to generate a sensor signal. A processor means calculates a physiological measurement in response to the sensor signal. A pattern extractor means identifies features of the physiological measurement. A pattern memory means stores a reference pattern. A pattern comparator means triggers an alarm if the identified features match the reference pattern. In various embodiments, a threshold is input to the pattern extractor. The identified features comprise at least the number of times the physiological measurement crosses the threshold within a predetermined time period. The identified features comprise at least the duration of each time the physiological measurement crosses the threshold. The physiological measurement comprises a predictive oxygen saturation measurement. A second processor means calculates an integrator oxygen saturation measurement.

## BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a block diagram of a prior art pulse oximeter portion;

FIG. 2 is a graph of oxygen saturation versus time illustrating a conventional threshold detector alarm;

FIG. 3 is a block diagram of an alarm processor utilizing parallel measurements of a physiological parameter;

FIG. 4 is a block diagram of a pulse oximeter processor utilizing dual oxygen saturation measurements;

FIG. 5 is a block diagram of a predictive alarm indicator utilizing a threshold detector with a slow oxygen saturation measurement input and a slope detector with a fast oxygen saturation measurement input;

FIGS. 6A-B are graphs of oxygen saturation versus time illustrating operation of the alarm indicator according to FIG. 5;

FIG. 7 is a block diagram of a pattern recognition alarm indicator utilizing a threshold detector with a slow oxygen saturation measurement input and a pattern extractor with a fast oxygen saturation measurement input; and

FIG. 8 is a graph of oxygen saturation versus time illustrating the pattern recognition alarm indicator according to FIG. 7.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

FIG. 3 illustrates a parallel measurement alarm processor 300. The alarm processor 300 has a sensor signal input 301 responsive to a physiological parameter and provides one or more alarm outputs 303 to indicate that the physiological parameter may have exceeded particular limits. The alarm processor 300 also has multiple parameter processors 310, which do not necessarily have the same or similar internal configurations. The multiple parameter processors 310 input the sensor signal 301 and provide parallel measurements 312 of the physiological parameter, each measurement having differing characteristics, such as response time or bandwidth to name a few. The alarm processor 300 further has an alarm indicator 320 that inputs the parallel parameter measurements 312 and generates the alarm outputs 303 based upon alarm conditions 305. The alarm outputs 303 change state to indicate that the parameter may have exceeded one or more limits and to trigger an alarm accordingly. The alarm conditions 305 define particular limits with respect to one or more of the measurements 312. The alarm conditions 305 may be pre-defined, such as by user input, or determined by a separate process, such as a measurement of sensor signal quality or data confidence as described in U.S. patent application Ser. No. 09/858,114 entitled "Pulse Oximetry Data Confidence Indicator," assigned to Masimo Corporation, Irvine, Calif. and incorporated by reference herein. The alarm processor 300 may also have a display driver 330 that processes one or more of the parameter measurements 312 and provides one or more display outputs 307.

FIG. 4 illustrates a pulse oximeter embodiment 400 of the alarm processor 300 (FIG. 3) described above. A pulse oximeter sensor (not shown) provides a signal input 301 that is responsive to arterial oxygen saturation, as described with respect to FIG. 1, above. The alarm processor 400 has dual oxygen saturation processors 310. An integrator oxygen saturation (SpO.sub.2) processor 410 outputs a slow SpO.sub.2 measurement 412, i.e. a measurement having a slow response time to changes in the SpO.sub.2 parameter. A predictor SpO.sub.2 processor 420 outputs a fast SpO.sub.2 measurement 422, i.e. a measurement having a fast response time that tracks changes in the SpO.sub.2 parameter. The slow SpO.sub.2 measurement 412 is input to a display driver 330, which provides an oxygen saturation display output 307. For example, the display output 307 may be input to a digital display that provides a numerical readout of oxygen saturation to a caregiver. Both the slow SpO.sub.2 measurement 412

and the fast SpO.sub.2 measurement 422 are input to an alarm indicator 320 that generates at least one alarm output 303 based upon alarm conditions 305, as described in further detail with respect to FIGS. 5-8, below.

The integrator SpO.sub.2 processor 410, advantageously, provides a smoothed measurement of oxygen saturation suitable for threshold detection. The predictor SpO.sub.2 processor 420, advantageously, provides a curve-fitting or a predictive measurement of oxygen saturation that detects trends in oxygen saturation, as described in further detail with respect to FIG. 5 and FIGS. 6A-B, below. Further, the predictor SpO.sub.2 processor 420 advantageously tracks oxygen saturation details that may signal a critical physiological event, as described in further detail with respect to FIGS. 7-8, below. The integrator SpO.sub.2 processor 410 and predictor SpO.sub.2 processor 420 may be a pulse oximeter as described in U.S. patent application Ser. No. 09/586,845 entitled "Variable Mode Averager," assigned to Masimo Corporation, Irvine, Calif. and incorporated by reference herein.

FIG. 5 illustrates a trend embodiment of an alarm indicator 320, which has a threshold detector 510, a slope detector 520 and alarm detector 530. The threshold detector 510 has a slow SpO.sub.2 measurement 412 and a threshold alarm condition 305 as inputs and a logic output BELOW 512. The slope detector 520 has a fast SpO.sub.2 measurement 422 input and a logic output POSITIVE/522. The alarm detector 530 has BELOW 512 and POSITIVE/522 logic inputs and generates an alarm output 303. The threshold detector 510 is a comparator that asserts BELOW 512 while the slow SpO.sub.2 measurement 412 is less in value than the value of the threshold 305. The slope detector 520 is a differentiator and comparator that asserts POSITIVE/522 while the slope of the fast SpO.sub.2 measurement 422 is non-positive, i.e. while the derivative of the fast SpO.sub.2 measurement 422 is zero or less than zero. The alarm detector 530 performs a logical AND function, asserts the alarm output 303 and indicates an alarm when BELOW 512 and POSITIVE/522 are both asserted. In this manner, an alarm output 303 only changes state when the slow SpO.sub.2 measurement 412 is below a threshold 305 and the fast SpO.sub.2 measurement 422 has not begun to increase in value. Advantageously, the trend recognition alarm indicator 320 reduces false alarms by suppressing a threshold-based alarm on the slow SpO.sub.2 measurement 412 when the fast SpO.sub.2 measurement 422 determines that a patient's oxygen saturation is in recovery, as described in further detail with respect to FIGS. 6A-B, below.

FIGS. 6A-B illustrate operation of the trend recognition alarm indicator 320 (FIG. 5). In FIG. 6A, a graph 600 has an SpO.sub.2 axis 601 and a time axis 602. Shown along the SPO.sub.2 axis 601 is a constant SPO.sub.2 value 606 corresponding to a threshold 305 (FIG. 5). The graph 600 shows a first plot of SPO.sub.2 versus time 610 corresponding to a fast SPO.sub.2 measurement 422 (FIG. 5). The graph 600 also shows a second plot of SpO.sub.2 versus time 620 corresponding to a slow SpO.sub.2 measurement 412 (FIG. 5). A suppressed alarm interval 640 along the time axis 602 corresponds to an alarm that would be indicated by the threshold detector 510 (FIG. 5) but is suppressed as occurring during a positive slope portion 630 of a fast SPO.sub.2 measurement 610. The alarm detector 530 (FIG. 5) would not assert an alarm output 303 (FIG. 5) during this interval.

In FIG. 6B, a graph 650 shows a first plot of SpO.sub.2 versus time 660 corresponding to a fast SpO.sub.2 measurement 422 (FIG. 5). The graph 650 also shows a second plot of SpO.sub.2 versus time 670 corresponding to a slow SpO.sub.2 measurement 412 (FIG. 5). An alarm interval 690 along the time axis 602 corresponds to an alarm period trig-

gered by the alarm output 303 (FIG. 5). This alarm interval 640 occurs while a slow SpO.sub.2 measurement 670 is below the threshold 606 and before a positive slope portion 680 of a fast SpO.sub.2 measurement 660.

FIG. 7 illustrates a pattern recognition embodiment of an alarm indicator 320, having a threshold detector 710, a pattern extractor 720, a pattern memory 730 and a pattern comparator 740. Further, the alarm indicator 320 has slow SpO.sub.2 412 and fast SpO.sub.2 422 measurement inputs in addition to threshold 701 and reference pattern 732 alarm condition inputs 305. The threshold detector 710 has a slow SPO.sub.2 measurement 412 and a SpO.sub.2 threshold 701 as inputs and a first alarm output 712. The threshold detector 710 changes the state of the first alarm output 712 when the value of the slow SpO.sub.2 measurement 412 crosses the SpO.sub.2 threshold 701. For example, the first alarm output 712 changes state to trigger an alarm when the slow SpO.sub.2 measurement 412 becomes less than the SpO.sub.2 threshold 701.

As shown in FIG. 7, the pattern extractor 720 has a fast SpO.sub.2 measurement 422 and a pattern threshold 734 as inputs and an extracted pattern output 722. The pattern extractor 720 identifies features of the fast SpO.sub.2 measurement 422 that may be used for pattern matching. Features may be, for example, the number of times the fast SpO.sub.2 measurement 422 crosses the pattern threshold 734 within a certain time period, or the duration of each time period that the fast SpO.sub.2 measurement 422 is less than the pattern threshold 734, to name a few. The pattern memory 730 has a pattern selection input 705 and a reference pattern output 732. The pattern memory 730 stores values for particular features that are identified by the pattern extractor 720. The reference pattern output 732 transfers these stored values to the pattern comparator 740. The pattern memory 730 may be nonvolatile and one or more patterns may be stored at the time of manufacture or downloaded subsequently via a data input (not shown). One of multiple patterns may be determined via the pattern selection input 705, by a user or by a separate process, for example. The pattern threshold 734 may be generated in response to the pattern selection input 705 or in conjunction with a selected reference pattern 732.

Also shown in FIG. 7, the pattern comparator 740 has the extracted pattern 722 and the reference pattern 732 as inputs and generates a second alarm output 742. That is, the pattern comparator 740 matches extracted measurement features provided by the pattern extractor 720 with selected features retrieved from pattern memory 730, changing the state of the second alarm output 742 accordingly. For example, the second alarm output 742 changes state to trigger an alarm when features of the fast SpO.sub.2 measurement 422 match the reference pattern output 732. Advantageously, the pattern recognition alarm indicator 320 reduces missed events by supplementing the threshold-based first alarm output 712 responsive to the slow SpO.sub.2 measurement 412 with a pattern-based second alarm output 742 responsive to detail in the fast SpO.sub.2 measurement 422. In this manner, if a patient's oxygen saturation is, for example, irregular or intermittent, the second alarm output 742 may trigger a caregiver alert when the first alarm output 712 does not, as described in further detail with respect to FIG. 8, below.

FIG. 8 illustrates operation of a pattern recognition alarm indicator 320 (FIG. 7), as described above. A graph 800 has a SpO.sub.2 axis 801 and a time axis 802. The graph 800 shows a SpO.sub.2 plot versus time 810 corresponding to the slow SPO.sub.2 measurement 412 (FIG. 7). Shown along the time axis 802 is a constant SPO.sub.2 value 812 corresponding to the SPO.sub.2 threshold 701 (FIG. 7). Due to the short dura-

tion of irregular and intermittent drops in SpO.sub.2, the slow SpO.sub.2 measurement 810 does not fall below the SpO.sub.2 threshold 812. Thus, the first alarm output 712 (FIG. 7) does not trigger an alarm in this example.

Also shown in FIG. 8, the graph 800 shows a SpO.sub.2 plot versus time 820 corresponding to the fast SpO.sub.2 measurement 422 (FIG. 7). Shown along the time axis 802 is a constant SPO.sub.2 value 822 corresponding to the pattern threshold 734 (FIG. 7). A corresponding graph 805 has a logic level axis 806 and a time axis 807. The graph 805 shows a logic level plot versus time 830 corresponding to the extracted pattern output 722 (FIG. 7). The logic level plot 830 has a "1" level when the fast SpO.sub.2 plot 820 is above the pattern threshold 822 and a "0" level when the fast SpO.sub.2 plot 820 is below the pattern threshold 822. In this manner, the logic level plot 830 indicates the number and duration of times the fast SpO.sub.2 plot 820 falls below a threshold value 822.

Further shown in FIG. 8, an alarm interval 870 along the time axis 802 corresponds to an alarm period indicated by the pattern comparator 740 (FIG. 7). This alarm interval 870 occurs after a reference pattern 732 (FIG. 7) is detected as matching an extracted pattern 722 (FIG. 7) and ends, correspondingly, when there is no longer a match. For example, assume that the reference pattern output 732 (FIG. 7) has the alarm criteria that at least three below threshold periods of minimum duration  $\tau_{sub.1}$  must occur during a maximum period  $\tau_{sub.2}$ , where the value of  $\tau_{sub.1}$  and  $\tau_{sub.2}$  are illustrated along the time axis 807. The below threshold time periods 831-834 are each greater in duration than  $\tau_{sub.1}$  and a first set of three, below-threshold time periods 831-833 occurs within a time period  $T_{sub.1} = \tau_{sub.2}$ , as illustrated. Thus, the alarm interval beginning 872 is triggered by the second alarm output 742 (FIG. 7). A second set of three, below-threshold time periods 832-834 also occurs within a time period  $T_{sub.2} = \tau_{sub.2}$ , as illustrated. Thus, the alarm interval 870 continues. There is no third set of three, below-threshold time periods. Thus, after the end of the time interval  $T_{sub.3} = \tau_{sub.2}$ , the alarm interval end 874 is triggered. This example illustrates how the pattern recognition alarm indicator 320 (FIG. 7) can trigger an alarm on an event, such as a period of irregular heartbeats, that might be missed by a threshold-based alarm responsive to the slow SpO.sub.2 measurement 412.

Although some alarm processor embodiments were described above in terms of pulse oximetry and oxygen saturation measurements, one of ordinary skill in the art will recognize that an alarm processor as disclosed herein is also applicable to the measurement and monitoring of other blood constituents, for example blood glucose and total hemoglobin concentration to name a few, and other physiological parameters such as blood pressure, pulse rate, respiration rate, and EKG to name a few.

In an embodiment, multiple pattern processors, each including a pattern extractor, pattern memory and pattern comparator, such as described with respect to FIG. 7, above, have as inputs one or more of fast SpO.sub.2 measurements, a pulse oximeter plethysmograph and pulse rate measurements. An arrhythmia alarm is generated based upon irregular heartbeat patterns being matched or otherwise detected in one or more combinations of SpO.sub.2 measurements, a pulse oximeter plethysmograph and pulse rate measurements.

A physiological trend monitor has been disclosed in detail in connection with various embodiments. These embodiments are disclosed by way of examples only and are not to limit the scope of the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications.

What is claimed is:

1. An oximeter, comprising:
  - a plurality of processing modules, each responsive to a noninvasive sensor signal indicative of light attenuated by body tissue, at least one processing module having different characteristics from another processing module, each of said plurality of processing modules outputting a parallel measurement, an alarm;
  - a memory storing criteria indicative of alarm conditions, said criteria including at least a duration of at least one of said parallel measurements crossing a threshold;
  - an alarm indicator receiving said parallel measurements from said plurality of processing modules, extracting features from said parallel measurements, comparing said features to said criteria, and when said features match said criteria, triggering said alarm on said oximeter.
2. The oximeter according to claim 1 wherein said criteria including at least a trend of said parallel measurements and a behavior of a slope of said trend.
3. The oximeter according to claim 1 wherein said criteria including at least a pattern.
4. The oximeter according to claim 1 wherein said criteria including at least a number of times said measurements crossed said threshold.
5. The oximeter according to claim 1 wherein at least one of said parallel measurements comprises a relatively slow measurement and at least one of said parallel measurements comprises a relatively fast measurement.
6. The oximeter according to claim 5, wherein said alarm indicator extracts threshold features from said slow measurement and at least one waveform feature from said fast measurement and said alarm indicator triggers said alarm based on a combination of said threshold and said waveform features.
7. The oximeter according to claim 5, wherein said alarm indicator extracts threshold features from said slow measurement and triggers said alarm based on said threshold features, said alarm indicator also extracting pattern features from said fast measurement and triggers said alarm based on said pattern features.
8. A method of determining when to alert a caregiver during oximeter-based patient monitoring, the method comprising:

- providing a plurality of electronic processing modules, at least one processing module having different characteristics from another processing module;
- providing an alarm;
- providing a memory;
- providing an alarm indicator;
- receiving a noninvasive sensor signal indicative of light attenuated by body tissue;
- electronically processing said sensor signal with said plurality of processing modules;
- outputting a parallel measurement from each of said plurality of processing modules;
- storing criteria indicative of alarm conditions, said criteria including at least a duration of at least one of said parallel measurements crossing a threshold;
- extracting features from said parallel measurements;
- comparing said features to said criteria; and
- when said features match said criteria, triggering said alarm.
9. The method according to claim 8 wherein storing said criteria comprises storing criteria including at least a trend of said parallel measurements and a behavior of a slope of said trend.
10. The method according to claim 8 wherein storing said criteria comprises storing criteria including at least a pattern.
11. The method according to claim 8 wherein storing said criteria comprises storing criteria including at least a number of times said measurements crossed said threshold.
12. The method according to claim 8 wherein outputting said parallel measurement includes outputting a relatively slow measurement and outputting a relatively fast measurement.
13. The method according to claim 12, wherein extracting features includes extracting threshold features from said slow measurement and extracting at least one waveform feature from said fast measurement, and wherein said triggering said alarm includes triggering said alarm based on a combination of said threshold and said waveform features.
14. The method according to claim 12, wherein extracting features includes extracting threshold features from said slow measurement and said triggering said alarm includes triggering said alarm based on said threshold features, and wherein extracting features includes extracting pattern features from said fast measurement and said triggering said alarm includes triggering said alarm based on said pattern features.

\* \* \* \* \*



专利名称(译)	生理趋势监测		
公开(公告)号	<a href="#">US8228181</a>	公开(公告)日	2012-07-24
申请号	US13/018334	申请日	2011-01-31
[标]申请(专利权)人(译)	AL ALI AMMAR		
申请(专利权)人(译)	AL-ALI AMMAR		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR		
发明人	AL-ALI, AMMAR		
IPC分类号	G08B29/00 A61B5/00		
CPC分类号	A61B5/746 A61B5/14551 A61B5/021 A61B5/04018 A61B5/0402 A61B5/0816 A61B5/14532 A61B5/14546		
优先权	60/351510 2002-01-24 US		
其他公开文献	US20110124990A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

生理趋势监测器具有响应于传输到组织部位的多个波长的光的传感器信号。在通过组织部位内的脉动血流衰减后检测透射光。处理器具有响应于传感器信号和生理参数输出的输入。从生理参数输出中提取特征。标准适用于功能。满足条件时生成警报输出。

