



US008657742B2

(12) **United States Patent**
Neumann

(10) **Patent No.:** **US 8,657,742 B2**
(45) **Date of Patent:** **Feb. 25, 2014**

(54) **MEDICAL MEASURING DEVICE**

(75) Inventor: **Rolf Neumann**, Calw (DE)

(73) Assignee: **Koninklijke Philips N.V.**, Eindhoven (NL)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1005 days.

(21) Appl. No.: **10/596,111**

(22) PCT Filed: **Nov. 23, 2004**

(86) PCT No.: **PCT/IB2004/052511**

§ 371 (c)(1),

(2), (4) Date: **Mar. 6, 2007**

(87) PCT Pub. No.: **WO2005/053527**

PCT Pub. Date: **Jun. 16, 2005**

(65) **Prior Publication Data**

US 2008/0039699 A1 Feb. 14, 2008

(30) **Foreign Application Priority Data**

Dec. 2, 2003 (EP) 03104501

(51) **Int. Cl.**

A61B 5/00 (2006.01)

G06F 19/00 (2011.01)

G06F 11/07 (2006.01)

(52) **U.S. Cl.**

CPC **G06F 19/3406** (2013.01); **G06F 11/0784** (2013.01); **A61B 5/7221** (2013.01)

USPC **600/301**

(58) **Field of Classification Search**

USPC 600/300–301; 128/903–905, 920

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,449,745 A	6/1969	Holt	
4,869,253 A *	9/1989	Craig et al.	600/323
5,137,458 A *	8/1992	Ungs et al.	434/262
5,170,791 A	12/1992	Boos et al.	
5,247,932 A	9/1993	Chung et al.	
5,262,944 A	11/1993	Weisner et al.	
5,417,222 A *	5/1995	Dempsey et al.	600/509
5,433,209 A	7/1995	Gallant et al.	
5,501,230 A	3/1996	Laribiere	
5,544,661 A	8/1996	Davis et al.	
5,620,472 A *	4/1997	Rahbari	607/27
5,638,816 A *	6/1997	Kiani-Azarbayjany et al.	600/316
5,704,351 A *	1/1998	Mortara et al.	600/382

(Continued)

FOREIGN PATENT DOCUMENTS

JP	2001078974 A	3/2001
JP	2002351981 A	12/2002

(Continued)

Primary Examiner — Bill Thomson


Assistant Examiner — Bobby Soriano

(57)

ABSTRACT

A medical measuring device or system (10) includes at least one measuring apparatus (12, 14). Each measuring apparatus, in turn, has at least one sensor (16, 18) for generating a measuring signal representing a sensed physiological parameter, e.g. ECG signals, of a patient (20, 22). The measuring apparatuses (12, 14) incorporate the measuring signal into a carrier signal which is transmitted a wireless communication route (24, 26) to a centrally located data detection device (24) which displays graphs (42) or numerical values (40) representing the sensed physiological parameters. The at least one measuring apparatus (12, 14) signals the quality of the measuring signals to a wearing patient (20) via an LED (32, 34) or loudspeaker (28, 30).

12 Claims, 1 Drawing Sheet

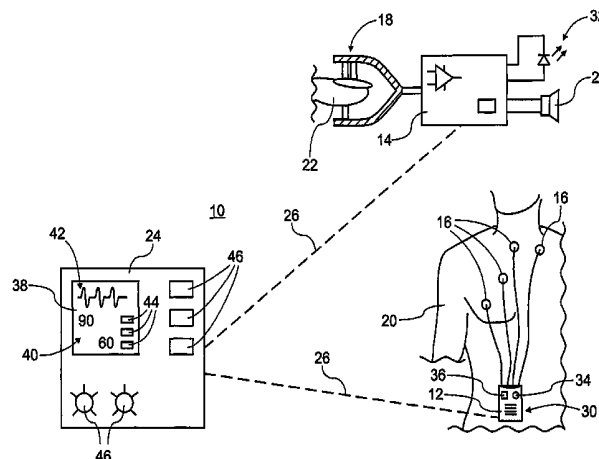

(56)

References Cited

U.S. PATENT DOCUMENTS


5,730,143 A * 3/1998 Schwarzberg 600/523
 5,733,259 A * 3/1998 Valcke et al. 604/66
 5,865,744 A * 2/1999 Lemelson 600/407
 5,931,791 A * 8/1999 Saltzstein et al. 600/513
 6,282,439 B1 * 8/2001 Ruha 600/509
 6,282,440 B1 * 8/2001 Brodnick et al. 600/512
 6,319,200 B1 * 11/2001 Lai et al. 600/300
 6,364,834 B1 * 4/2002 Reuss et al. 600/300
 6,415,166 B1 7/2002 Van Hoy et al.
 6,449,501 B1 9/2002 Reuss
 6,551,252 B2 * 4/2003 Sackner et al. 600/536
 6,658,276 B2 * 12/2003 Kianl et al. 600/322
 6,728,564 B2 * 4/2004 Lahteenmaki 600/383
 6,811,535 B2 * 11/2004 Palti et al. 600/499
 6,850,788 B2 * 2/2005 Al-Ali 600/323
 6,863,652 B2 * 3/2005 Huang et al. 600/300
 6,893,396 B2 * 5/2005 Schulze et al. 600/300
 7,016,707 B2 3/2006 Fujisawa et al.
 7,100,601 B2 * 9/2006 Bruna 128/200.14
 7,115,097 B2 * 10/2006 Johnson 600/538

7,174,206 B2 * 2/2007 Frei et al. 600/544
 7,371,214 B2 * 5/2008 Kouchi et al. 600/300
 8,187,181 B2 * 5/2012 Osorio et al. 600/300
 2002/0035315 A1 3/2002 Ali et al.
 2002/0109621 A1 * 8/2002 Khair et al. 341/174
 2002/0161291 A1 10/2002 Kianl et al.
 2003/0004403 A1 * 1/2003 Drinan et al. 600/301
 2003/0023183 A1 1/2003 Williams
 2003/0120164 A1 6/2003 Nielsen et al.
 2003/0217747 A1 * 11/2003 Hickie et al. 128/203.12
 2004/0030226 A1 * 2/2004 Quy 600/300
 2004/0122295 A1 * 6/2004 Hatlestad et al. 600/300

FOREIGN PATENT DOCUMENTS

JP 2003144394 A 5/2003
 JP 2003264632 A 9/2003
 JP 2003271732 A 9/2003
 WO WO 94/10902 A1 5/1994
 WO 02091918 A2 11/2002
 WO WO 03/009749 A1 2/2003

* cited by examiner

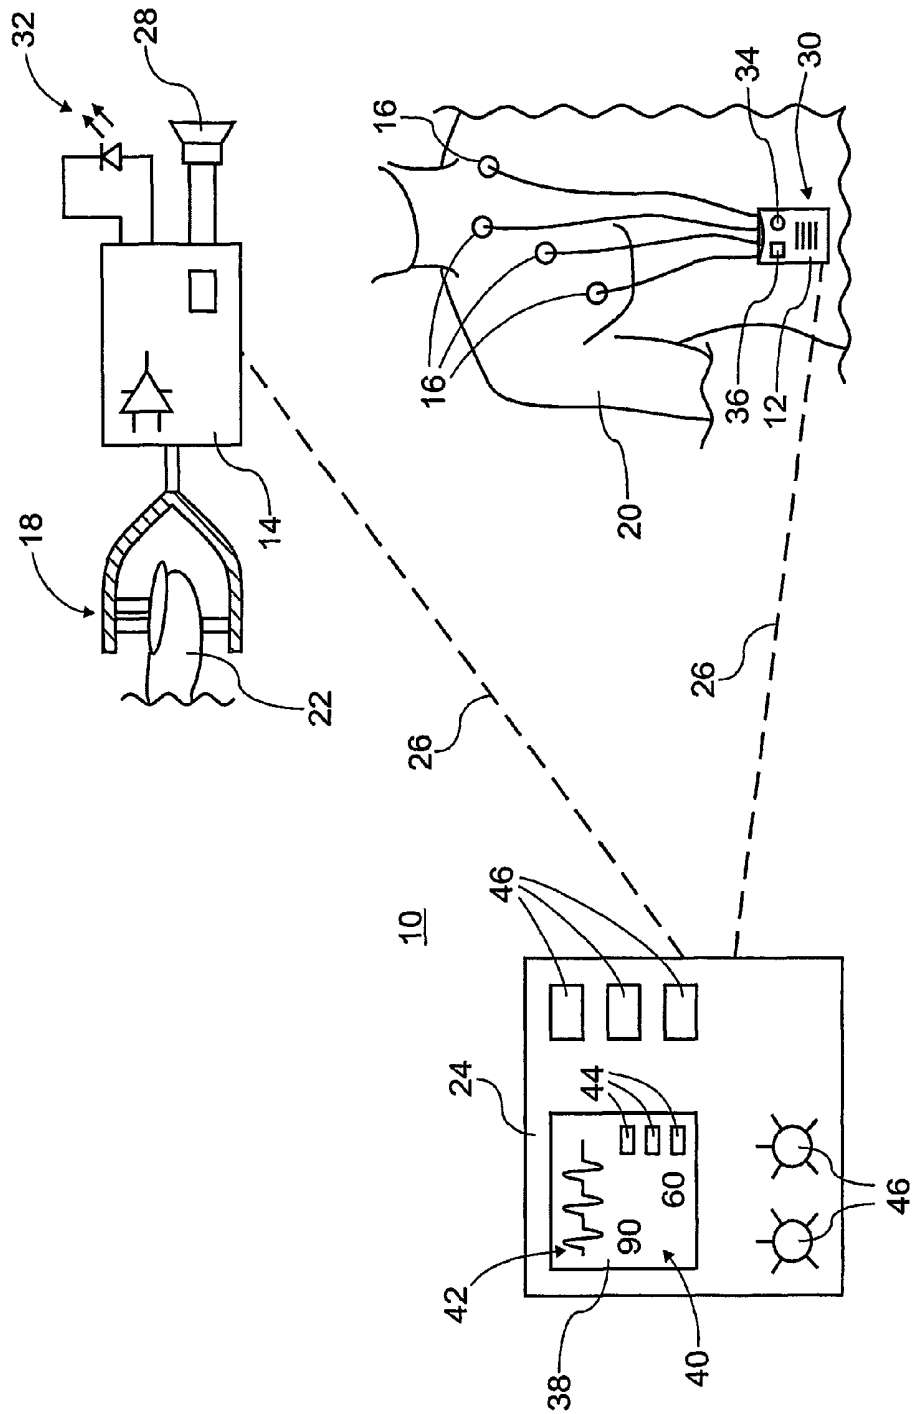

MEDICAL MEASURING DEVICE

The invention relates to a medical measuring device according to claim 1.

Instead of stationary and large measuring apparatuses, small and mobile apparatuses are used more and more frequently in the medical sector, which can be carried by patients and therefore allow greater freedom of movement. An autonomous ECG recorder is known, for example, from U.S. Pat. No. 5,433,209 and is designed as a portable apparatus allowing leads-off detection and alarm actuation on the portable apparatus which is implemented automatically according to a fixed sequence once the apparatus has been switched on.

Mobile devices of this type are generally optimized with respect to a small size and low power consumption. They therefore do not generally have detailed displays, but only small displays designed for the basic functions such as on/off or the battery status.

Devices of this type are increasingly no longer used as autonomous units, but as remote units for measuring data detection in a distributed measuring and measuring data detection system. These units then communicate with a stationary apparatus via a generally wireless communication connection, via which measuring signals are transmitted from a remote unit or a measuring apparatus to the stationary apparatus or the measuring data detection device.

However, when sensors of the remote units are placed on the body of a patient, medical staff cannot generally see a stationary apparatus with its detailed displays located in another room. Therefore they have no information about the correct placing on the body of the patient with respect to good quality of the measuring signals. For this purpose, the staff have to go to the stationary apparatus once the sensors have been placed and check the measuring signal quality. However, this is very time-consuming.

A further problem is that directly after the placing of sensors of a remote unit, the measuring signal quality is frequently very good but some time later deteriorates. It is therefore generally necessary for medical staff to check the measuring signal quality from time to time at the stationary apparatus. However, this is also very time-consuming.

An object of the present invention is therefore to propose a medical measuring device which is easier for medical staff to handle than the devices described at the outset, in particular requiring less time for monitoring.

A patient-worn measuring apparatus is described in which signal quality from a sensor, e.g., electrode, is measured directly at the measuring apparatus. Medical staff are therefore spared the time-consuming checking of the quality of the measuring signals at a central unit like the measuring data detection device.

A medical measuring device has at least one measuring apparatus which has at least one sensor for generating a measuring signal of a patient, and a measuring data detection device, which is designed to exchange the measuring signal with the at least one measuring apparatus via an, in particular, wireless communication route. The at least one measuring apparatus is designed to signal the quality of the measuring signal.

The at least one measuring apparatus is designed, in particular, to signal the quality of the measuring signal acoustically, for example by a short audio signal, when the signal quality is poor. The audio signal can thus be changed depending on the signal quality, for example it may be repeated very

often in the case of very poor signal quality. Typically no audio signal is sounded when the signal quality is adequate or good.

Alternatively or in addition, the at least one measuring apparatus can be designed to signal the quality of the measuring signal optically, for example by a display with LEDs or on an LCD.

The at least one measuring device is preferably a light means with different colors, each color being associated with a predetermined range of a signal quality and activated when the quality of the measuring signal is in the corresponding, predetermined range.

The light means may also be, for example, a three-colored LED, three different colors being provided for a range of poor quality, a range of medium and a range of high quality. Red may be, for example, poor, yellow medium and green good signal quality.

The at least one measuring apparatus is preferably designed to signal the quality of the measuring signal automatically. In this case no activation of a signalization of the measuring signal quality is necessary by medical staff.

The at least one measuring apparatus may be designed, for example, to signal the quality of the measuring signal when it is placed on a patient at another measuring site. In other words, it is triggered automatically when the measuring site is changed and signals the signal quality.

In addition or also alternatively, the at least one measuring apparatus can be designed to signal the quality of the measuring signal, if a substantial change in the quality of the measuring signal is detected, for example when a patient has removed one or more sensors.

The at least one measuring apparatus can also be designed to signal the quality of the measuring signal on demand, for example by pressing a button on the measuring apparatus or by a corresponding demand from the measuring data detection device.

In a simple embodiment, the at least one measuring apparatus is designed to signal the quality of the measuring signal in such a way that falling below a predetermined signal quality is signaled. In other words there is a threshold value in the form of the predetermined signal quality. The falling below of the threshold value can be detected by a comparator in the measuring apparatus and trigger or activate signaling.

For preferred application areas in the medical sector, the at least one measuring apparatus is designed to signal the quality of the measuring signal on the basis of an evaluation of one or more parameters such as the perfusion index, transmission level, interference level, the signal form or the like.

The at least one measuring apparatus is preferably a pulse oximeter, an ECG recorder and/or ultrasound measuring head.

Further advantages of the application possibilities of the present invention emerge from the following description of an embodiment of the invention with the single drawing.

The single FIGURE of the drawing shows a medical measuring device 10 in the form of a distributed medical measuring system with measuring apparatuses 12 and 14 and a central measuring data detection device 24 which is used for storing and displaying medical measuring data and for central control of the measuring apparatus 12 and 14.

The measuring data detection device 24 comprises an LCD display screen 38 for displaying medical measuring data. The medical measuring data comprise, for example, a curve pattern 42, numerical values 40 for measuring values, or other display information 44. The measuring data detection device 24 has various operating elements 46 for adjusting measuring

parameters, the display on the screen **38** and functions of this type of the measuring data detection device **24**.

The measuring device **12** is a portable ECG measuring apparatus which has a plurality of ECG electrodes **16** as sensors. As shown in the FIGURE, a patient **20** carries the ECG measuring apparatus **12** on his upper body, on which the ECG electrodes **16** are fastened. The ECG measuring device **12** has an ECG recorder for recording the ECG signals picked up via the ECG sensor **16**. It also comprises a radio unit, with which it can build up a radio communication connection **26** with the measuring data detection device **24** for transmitting measuring signals.

To facilitate the correct placing of the ECG electrodes **16** on the upper body of the patient **20** for medical staff, the ECG measuring apparatus **12** has a three-colored LED **34** and a loudspeaker **30**. The LED **34** and the loudspeaker **30** are used for optical or acoustic signaling of the quality of measuring signals which are captured via the ECG electrodes **16**.

When the ECG measuring apparatus **12** detects that no measuring signal with adequate quality can be received via the ECG electrodes **16**, it switches the color of the LED **34** to red to display a poor or lesser signal quality. Furthermore, an acoustic signal in the form of a short periodic audio signal sounds over the loudspeaker **30** for as long as the signal quality is not adequate.

The signal quality is checked fully automatically in the ECG measuring apparatus **12**, as soon as it is switched on. It is also possible to start a test of the signal quality by actuating a signal quality test button **36** on the ECG measuring apparatus **12**. This may be carried out, for example, by the patient **20** himself. When the signal quality is adequate, the ECG measuring device **12** transmits measuring signals of the ECG electrodes **16** via the radio communication connection **26** to the measuring data detection device **24** which shows the signals received, for example in the form of the curve pattern **42** on the large LCD display screen **38** and records the course of the measuring signals.

The measuring apparatus **14** is a pulsoximeter and connected to a pulsoximeter sensor **18**, in which one finger **22** of the patient is located. The measuring signals of the sensor **18** are transmitted to the pulsoximeter measuring apparatus **14**. The measuring apparatus comprises a comparator for comparing the signal quality of the measuring signals received with the predetermined threshold value for a predetermined signal quality. When the signal quality received is less than the predetermined threshold value, the comparator output signal activates an LED **32** and an audio signal generator which controls the loudspeaker **28** with an audio signal. In this case, there is therefore optical and acoustic signaling that the quality of the signal of the pulsoximeter sensor **18** is not adequate to ensure reliable recording in the measuring data detection device **24**.

The signal quality can then be changed by the patient or medical staff by changing the position of the pulsoximeter sensor **18** in order to receive an adequate signal quality. When the signal quality is adequate, the measuring signals are transmitted from the pulsoximeter measuring apparatus **14** via a radio communication connection **26** to the measuring data detection device **24** which displays the measuring signals received in the form of numerical values on the screen **38** and records them.

The invention has been described with reference to the preferred embodiments. Modifications and alterations may occur to others upon reading and understanding the preceding detailed description. It is intended that the invention be con-

strued as including all such modifications and alterations insofar as they come within the scope of the appended claims or the equivalents thereof.

LIST OF REFERENCE NUMERALS

10 medical measuring device
12 ECG measuring apparatus
14 pulsoximeter
16 ECG electrodes
18 pulsoximeter sensor
20 patient
22 finger of a patient
24 measuring data detection device
26 radio communication connection
28, 30 loudspeaker
32, 34 LED
36 signal quality test button
38 LCD display screen
40 numerical values
42 curve pattern
46 operating elements

The invention claimed is:

1. A medical measuring system comprising:

one or more patient body mounted sensors which contact a portion of a patient to measure physiological patient data and generate physiological patient data signals indicative of the measured physiological patient data;

a patient body mounted measuring apparatus worn by the patient, the patient body mounted measuring apparatus receives the physiological patient data signals from the one or more sensors, evaluates the measured physiological patient data signals from the one or more sensors for a change in a quality of the physiological patient data signal, and indicates the quality of the physiological patient data signals to the patient wherein the measuring apparatus evaluates the measured medical data signals for one or more of an interference level and a signal form to determine the quality of the physiological patient data signals generated by the sensors as received at the measuring apparatus; and

a measurement display apparatus detached from the patient that displays physiological patient data generated by the one or more sensors, the physiological patient data being wirelessly transferred from the patient body mounted measuring apparatus to the measurement display apparatus; and

wherein the measuring apparatus compares the determined quality with a preselected quality level and transmits the patient data wirelessly to the measurement apparatus in response to the determined quality meeting or exceeding the preselected level and signals the wearer in response to the determined quality falling below the preselected level.

2. The medical measuring system as claimed in claim 1, wherein the measuring apparatus includes an optical indicator which includes:

a light with a plurality of colors, each color being associated with one of a plurality of predetermined ranges of the at least one physiological data signal quality to indicate when the quality of the at least one physiological data measurement signal is in the corresponding one of the plurality of predetermined ranges.

3. The medical measuring system as claimed in claim 1, wherein the measuring apparatus indicates the quality of the

5

physiological data signal in response to one of the sensors being placed on another measuring site of the patient wearing the measuring apparatus.

4. The medical measuring system as claimed in claim 1, wherein the measuring apparatus indicates the quality of physiological data signal in response to a preselected change in the quality of the physiological data signal from the sensor.

5. The medical measuring system as claimed in claim 1, wherein the at least one sensor includes a pulseoximeter, an ECG recorder or ultrasound measuring head.

6. The medical measuring system of claim 1, wherein the measuring apparatus indicates the quality of the physiological patient data signals to the patient in response to the determined quality of the physiological patient data signals being below a threshold and generates at least one of:

- an acoustic signal to the patient to which the measuring apparatus is mounted, and
- an optical signal via a light mounted on the measuring apparatus.

7. The medical measuring system of claim 1, wherein the measuring apparatus does not display the physiological patient data.

8. The medical measuring system of claim 1, wherein the quality is indicated in a manner which is humanly perceivable to the patient locally adjacent the measuring apparatus, wherein the quality is not indicated at the measurement display apparatus.

9. A medical measuring system comprising:

- a data device including a display screen for displaying at least one of medical measurement values and graphs;
- at least one sensor worn by a patient which generates at least one physiological data measurement signal indicative of physiological data of the patient;
- at least one mobile measuring apparatus worn by the patient which (1) receives the at least one physiological data measurement signal from the at least one sensor, (2) evaluates the at least one physiological data measurement signal from the at least one sensor for a change in a quality of the at least one physiological data measurement signal and indicates the quality of the at least one physiological data measurement signal generated by the at least one sensor, and (3) communicates the at least one data measurement signal wirelessly to the data device, wherein the mobile measuring apparatus evaluates a signal form of the at least one physiological data mea-

6

surement signal from the at least one sensor to determine the quality of the at least one physiological data measurement signal; and

wherein the data device is disposed remote from the patient, the wireless communication between the at least one mobile measuring apparatus and the data device enabling the patient to move freely without being tethered to the data device.

10. The medical measuring system as claimed in claim 9, wherein the at least one mobile measuring apparatus includes at least one of an acoustic indicator and an optical indicator which indicates the quality of the at least one physiological data measurement signal to a wearer of the mobile measuring apparatus.

11. The medical measuring system as claimed in claim 9, wherein the at least one measuring apparatus signals the quality of the at least one physiological data measurement signal on demand.

12. A medical measuring system comprising:

- a data device including a display screen for displaying at least one of medical measurement values and graphs;
- at least one sensor worn by the patient which generates at least one physiological data measurement signal indicative of physiological data of a patient; and
- at least one mobile measuring apparatus worn by the patient which (1) receives the at least one physiological data measurement signal from the at least one sensor, (2) automatically evaluates the at least one physiological data measurement signal to determine change in a quality of the at least one physiological data measurement signal and indicates to the patient at least one of the quality and the change in the quality of the at least one physiological data measurement signal generated by the at least one sensor, and (3) communicates the at least one data measurement signal wirelessly to the data device, wherein the mobile measuring apparatus evaluates the physiological data measurement signal based on an interference level;

wherein the data device is disposed remote from the patient, the wireless communication between the at least one mobile measuring apparatus and the data device enabling the patient to move freely without being tethered to the data device.

* * * * *

专利名称(译)	医疗测量设备		
公开(公告)号	US8657742	公开(公告)日	2014-02-25
申请号	US10/596111	申请日	2004-11-23
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	NEUMANN ROLF		
发明人	NEUMANN, ROLF		
IPC分类号	A61B5/00 A61B5/0404 G06F11/07 A61B8/00 G06F19/00		
CPC分类号	A61B5/0404 A61B8/00 A61B5/1455 A61B5/7221 G06F11/0784 A61B5/0002 G06F19/3406 G16H40/63		
优先权	2003104501 2003-12-02 EP		
其他公开文献	US20080039699A1		
外部链接	Espacenet USPTO		

摘要(译)

医学测量装置或系统 (10) 包括至少一个测量装置 (12,14)。每个测量装置又具有至少一个传感器 (16,18)，用于产生表示所感测的生理参数的测量信号，例如，患者的ECG信号 (20,22)。测量装置 (12,14) 将测量信号合并到载波信号中，该载波信号通过无线通信路径 (24,26) 传输到位于中心的数据检测装置 (24)，该装置显示图形 (42) 或数值 (40)。表示感测的生理参数。至少一个测量装置 (12,14) 通过LED (32,34) 或扬声器 (28,30) 向佩戴患者 (20) 发信号通知测量信号的质量。

