



US 20140371554A1

(19) **United States**(12) **Patent Application Publication**
Bake, JR.(10) **Pub. No.: US 2014/0371554 A1**(43) **Pub. Date: Dec. 18, 2014**(54) **METHOD FOR IMPROVED OXYGEN
SATURATION ESTIMATION IN THE
PRESENCE OF NOISE**(71) Applicant: **COVIDIEN LP, MANSFIELD, MA**
(US)(72) Inventor: **Clark R. Bake, JR., Newman, CA (US)**(21) Appl. No.: **14/472,038**(22) Filed: **Aug. 28, 2014****Related U.S. Application Data**(63) Continuation of application No. 12/165,256, filed on
Jun. 30, 2008, now Pat. No. 8,862,194.**Publication Classification**(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 5/1455 (2006.01)(52) **U.S. Cl.**
CPC **A61B 5/7203** (2013.01); **A61B 5/14551**
(2013.01); **A61B 5/7264** (2013.01); **A61B**
5/7282 (2013.01); **A61B 5/7405** (2013.01);
A61B 5/742 (2013.01); **A61B 5/7455** (2013.01)
USPC **600/323**(57) **ABSTRACT**

The present disclosure relates, according to some embodiments, to devices, systems, and methods for estimating a physiological parameter in the presence of noise. For example, the disclosure relates, in some embodiments, to devices, systems, and methods for assessing (e.g., estimating, measuring, calculating) oxygen saturation (SpO₂). Methods of assessing SpO₂ may include assessing a noise metric associated with motion artifact. In some embodiments, a percentage (e.g., an empirically determined percentage) of a noise metric may be simply added to the SpO₂ estimate to produce a corrected SpO₂ estimate. An oximetry algorithm may include, according to some embodiments, combining multiple internal SpO₂ estimates and associated noise and/or signal quality metrics (e.g., using a radial basis neural network) to produce a modified (e.g., corrected) SpO₂ estimate (e.g., rather than merely selecting the estimate from a finite number of candidates). A modified SpO₂ estimate may include little or no movement-based error.

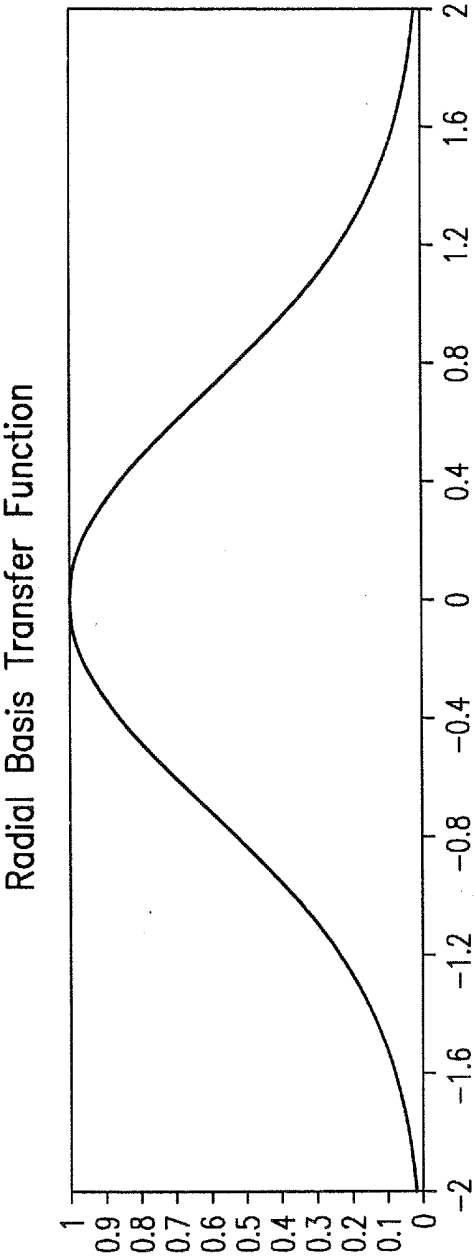


FIG.1

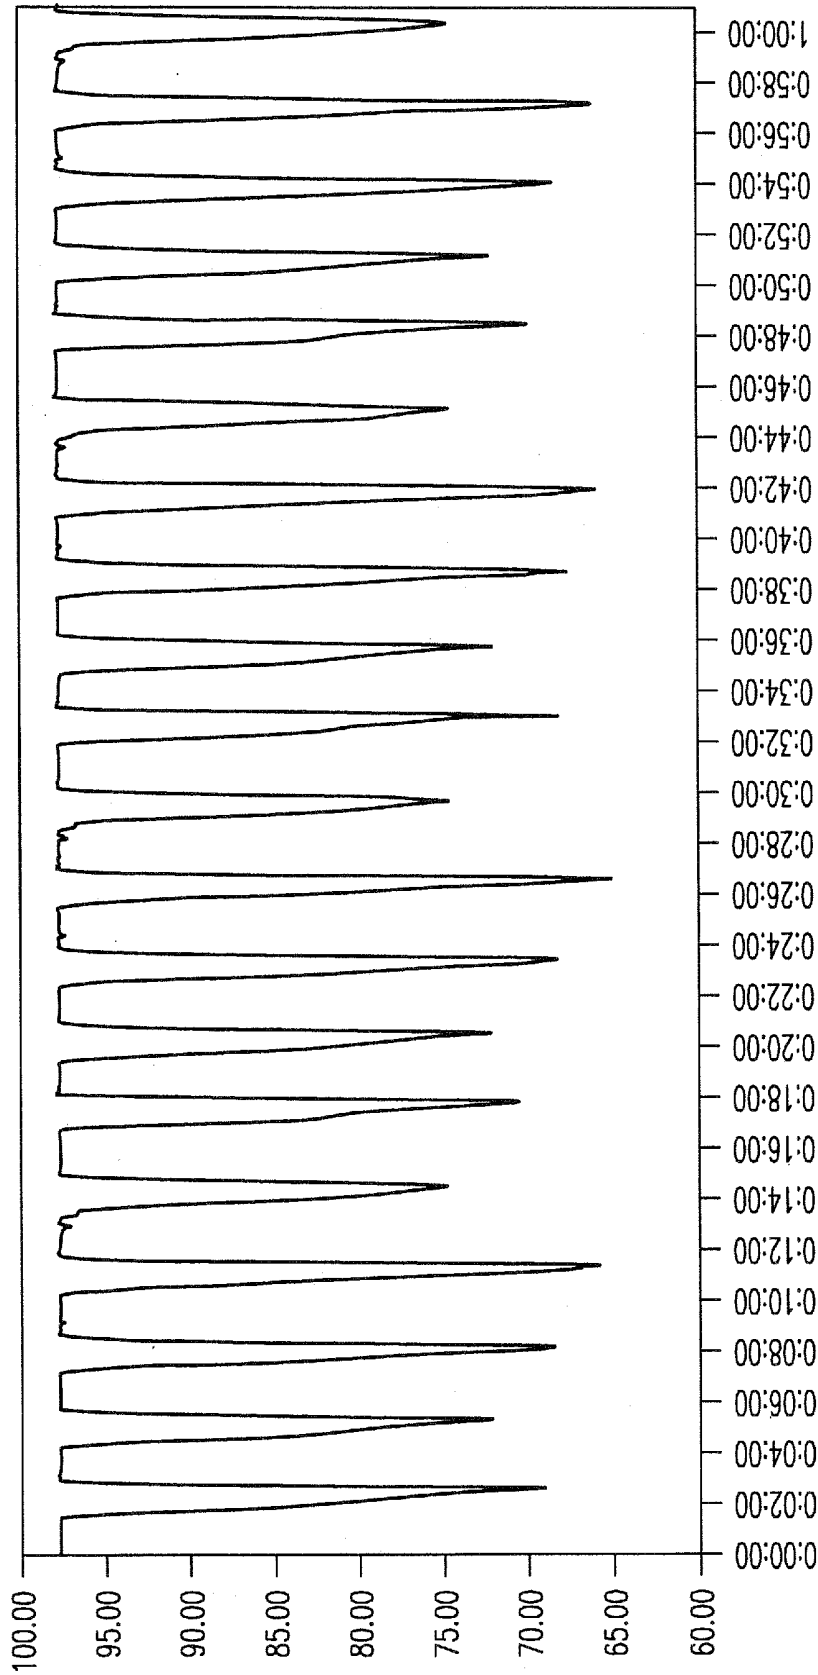


FIG.2

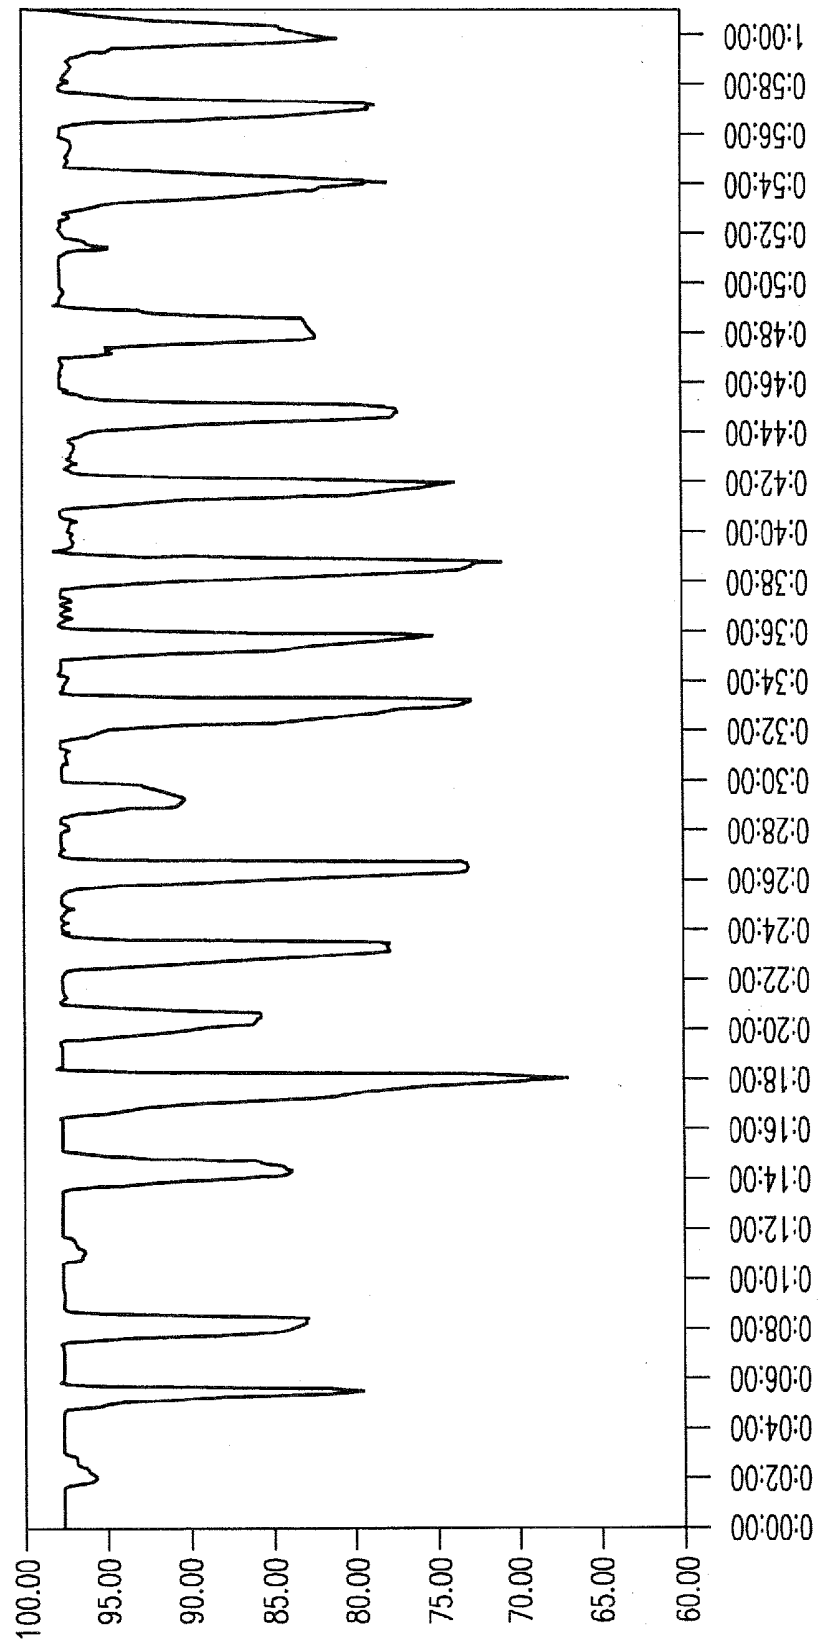


FIG. 3

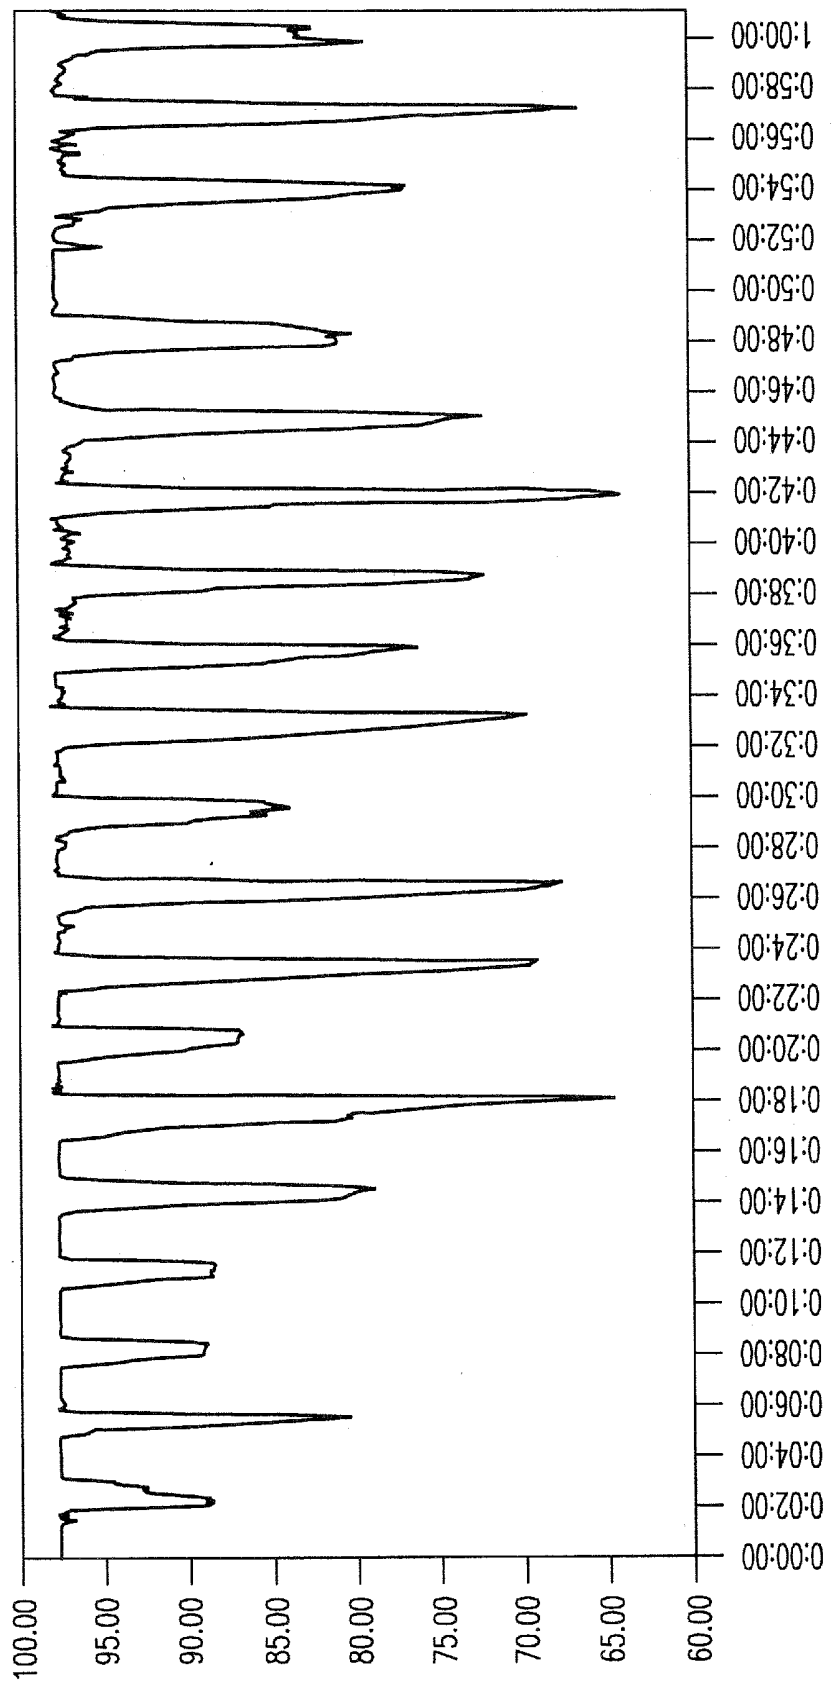


FIG.4

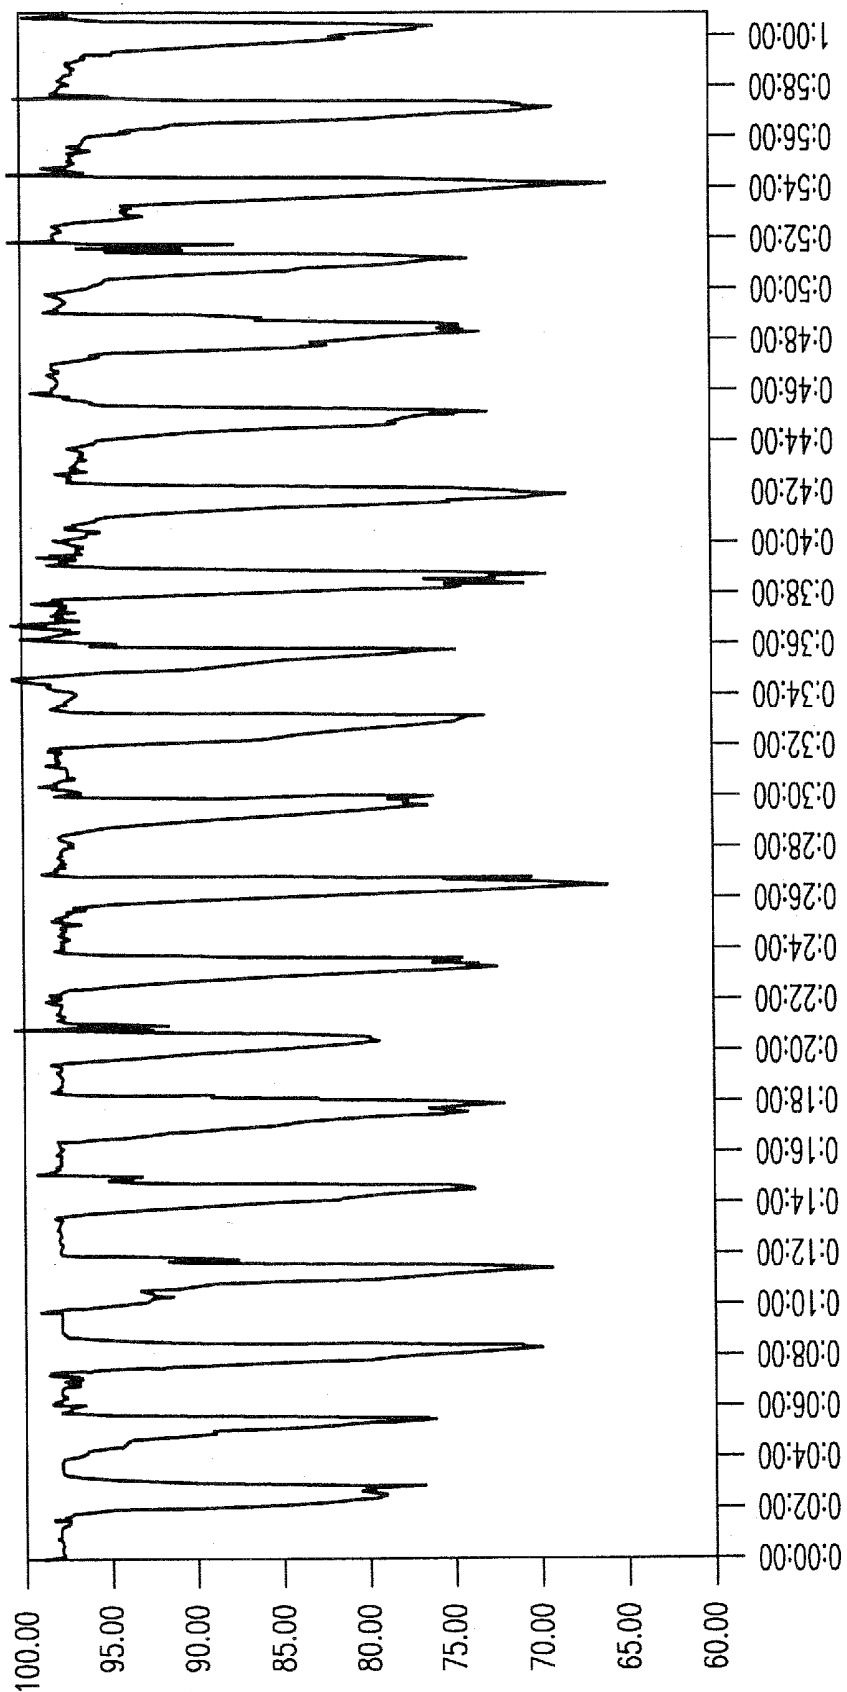


FIG. 5

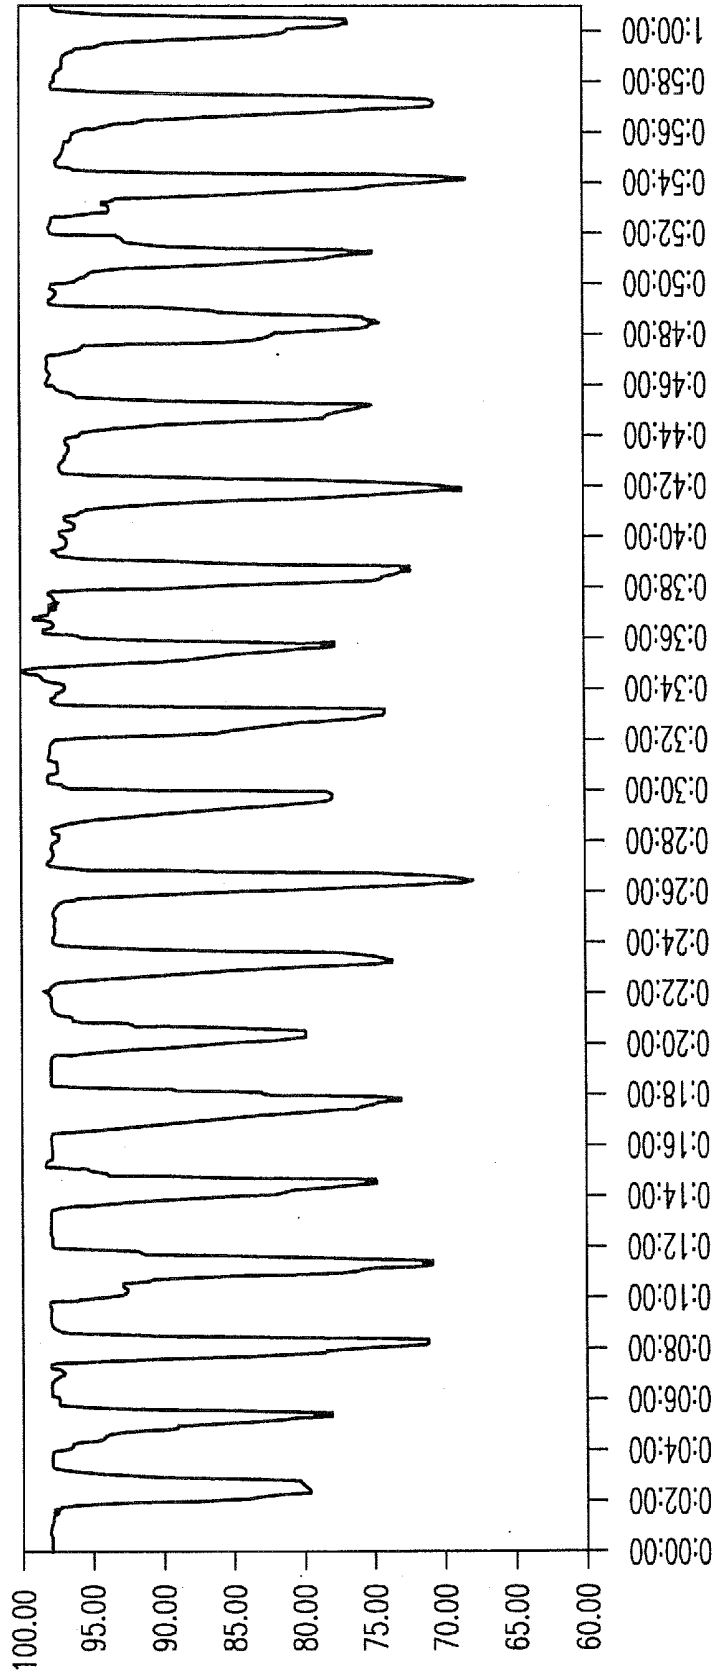


FIG. 6

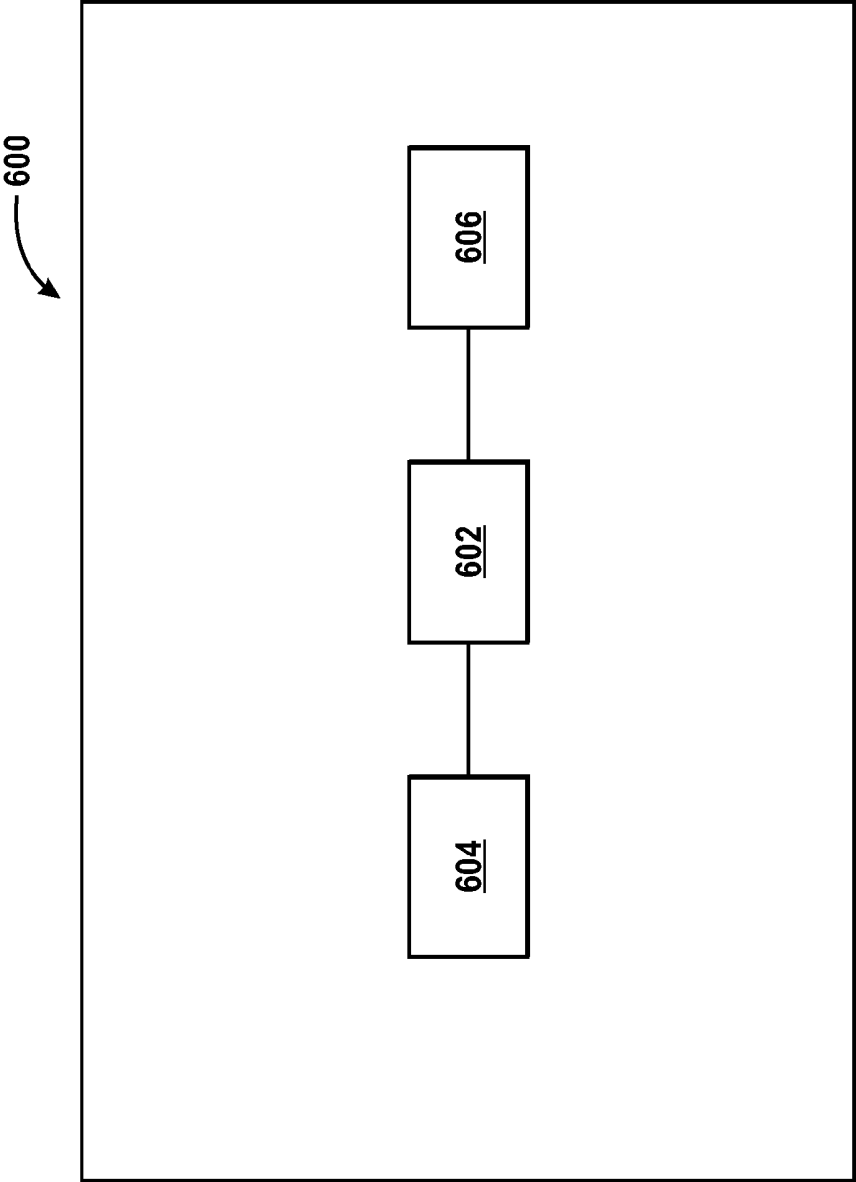


FIG. 7

METHOD FOR IMPROVED OXYGEN SATURATION ESTIMATION IN THE PRESENCE OF NOISE

[0001] This application is a divisional of U.S. patent application Ser. No. 12/165,256, entitled "Method for Improved Oxygen Saturation Estimation in the Presence of Noise," filed Jul. 3, 2008, which is incorporated herein by reference in its entirety.

FIELD OF THE DISCLOSURE

[0002] The present disclosure relates, in some embodiments, to devices, systems, and methods for estimating oxygen saturation (SpO₂).

BACKGROUND OF THE DISCLOSURE

[0003] Pulse oximeters typically measure and display various blood flow characteristics including but not limited to the oxygen saturation of hemoglobin in arterial blood. Oximeters pass light through blood perfused tissue such as a finger or an ear, and photoelectrically sense the absorption of light in the tissue. The amount of light absorbed is then used to calculate the amount of the blood constituent (e.g., oxyhemoglobin) being measured.

[0004] The light passed through the tissue is selected to be of one or more wavelengths that are absorbed by the blood in an amount representative of the amount of the blood constituent present in the blood. The amount of light passed through the tissue varies in accordance with the changing amount of blood constituent in the tissue and the related light absorption.

[0005] The optical signal through the tissue may be degraded by noise or other artifacts. One source of noise is ambient light which reaches the light detector. Another source of noise is electromagnetic coupling from other electronic instruments. Motion of the patient may also introduce noise onto the signal. For example, the contact between the detector and the skin, or the emitter and the skin, may be temporarily disrupted when motion causes either to move away from the skin. In addition, since blood is a fluid, it may respond differently than the surrounding tissue to inertial effects, thus resulting in momentary changes in volume at the point to which the oximeter probe is attached. Noise may degrade a pulse oximetry signal relied upon by a physician, without the physician's awareness.

[0006] An oximetry algorithm may include noise metrics to allow it to quantify artifacts that degrade SpO₂ accuracy. These metrics may be used to reduce the impact of the artifacts on accuracy. For example, these metrics may be used to adapt multiple internal filters and to select from multiple internal SpO₂ estimates. In cases with motion artifact, the noise metrics generally have a significant negative correlation to the SpO₂ level for typical sensor designs. That is, increased motion artifact usually results in a negative SpO₂ bias for transmission-type sensor designs, rather than simply generating zero-mean SpO₂ errors.

SUMMARY

[0007] Accordingly, a need has arisen for improved noise metrics to correct negative SpO₂ bias associated with artifacts (e.g., movement artifacts).

[0008] The present disclosure relates, according to some embodiments, to devices, systems, and methods for estimating a physiological parameter in the presence of noise. For

example, the disclosure relates, in some embodiments, to devices, systems, and methods for assessing (e.g., estimating, measuring, calculating) oxygen saturation (SpO₂). Methods of assessing SpO₂ may include assessing a noise metric associated with motion artifact. In some embodiments, a percentage (e.g., an empirically determined percentage) of a noise metric may be simply added to the SpO₂ estimate to produce a corrected SpO₂ estimate. Indeed, by adding the percentage of the noise metric, the negative SpO₂ bias may be corrected. An oximetry algorithm may include, according to some embodiments, combining multiple internal SpO₂ estimates and associated noise and/or signal quality metrics (e.g., using a radial basis neural network) to produce a modified (e.g., corrected) SpO₂ estimate (e.g., rather than merely selecting the estimate from a finite number of candidates). A modified SpO₂ estimate may include little or no movement-based error.

[0009] One embodiment includes a device for estimating oxygen saturation in the presence of noise. The device may include a processor in communication with a radial basis neural network, wherein the processor is configured to receive optical oximetry data, process the optical oximetry data to produce at least one oxygen saturation estimate, communicate the at least one oxygen saturation estimate to the radial basis neural network, and receive a modified oxygen saturation estimate comprising less noise bias than the at least one oxygen saturation estimate from the radial basis neural network, wherein the radial basis neural network is configured to define the modified oxygen saturation estimate based at least in part on combining the at least one oxygen saturation estimate with corresponding signal quality metrics. The device may also include a display in communication with the processor, wherein the display is operable to display a representation of the modified oxygen saturation estimate.

[0010] One embodiment includes a method for estimating oxygen saturation in the presence of noise. The method may include determining a change in estimated oxygen saturation comprising calculating a difference between a first estimated oxygen saturation value at a first time and a second estimated oxygen saturation value at a second time. Additionally, the method may include determining a change in a saturation noise estimate between a first saturation noise estimate and a second saturation noise estimate, wherein the change in the saturation noise estimate attends the change in estimated oxygen saturation. Further, the method may include displaying either the first estimated oxygen saturation value or the second oxygen saturation value based at least in part on a comparison between the change in the estimated oxygen saturation and the change in the saturation noise estimate.

[0011] One embodiment includes a method for reducing affects of noise in an oxygen saturation estimate. The method may include solving a computer-implemented radial basis neural network using a training set of oxygen saturation estimates, wherein the training set of oxygen saturation estimates include a target saturation estimate from noise-free data, a noise-perturbed saturation estimate, and metrics associated with calculating the noise-perturbed saturation estimate. Further, the method may include processing at least one test oxygen saturation estimate that is biased by noise using the computer-implemented radial basis neural network to produce a modified test oxygen saturation estimate comprising less noise bias than the at least one test oxygen saturation estimate.

[0012] One embodiment includes a method of detecting hypoxia in a subject. The method may include collecting optical oximetry data from a subject, processing the optical oximetry data to produce at least one oxygen saturation estimate, processing the at least one oxygen saturation estimate using a solved, computer-implemented radial basis neural network to produce at least one modified oxygen saturation estimate, and comparing the at least one modified oxygen saturation estimate with a hypoxia oxygen saturation threshold.

BRIEF DESCRIPTION OF THE DRAWINGS

[0013] Some embodiments of the disclosure may be understood by referring, in part, to the present disclosure and the accompanying drawings, wherein:

[0014] FIG. 1 illustrates a transfer function $F(x)$ according to a specific example embodiment of the disclosure;

[0015] FIG. 2 illustrates oxygen saturation in a non-moving finger as a function of time using an example algorithm;

[0016] FIG. 3 illustrates oxygen saturation from moving fingers as a function of time using a prior art algorithm;

[0017] FIG. 4 illustrates oxygen saturation (SpO_2) from moving fingers as a function of time using a prior art algorithm;

[0018] FIG. 5 illustrates oxygen saturation from moving fingers as a function of time using an algorithm according to a specific example embodiment of the disclosure;

[0019] FIG. 6 illustrates oxygen saturation from moving fingers as a function of time using an algorithm according to a specific example embodiment of the disclosure; and

[0020] FIG. 7 is a block diagram of a device or system for estimating oxygen saturation in the presence of motion artifact.

DETAILED DESCRIPTION

[0021] The present disclosure relates, in some embodiments, to devices, systems, and methods for reducing the effects of motion artifact and/or noise on a physiological parameter measurement. For example, methods according to some embodiments of the disclosure may take into account physical limitations on various physiological parameters being monitored when weighting and combining a series of samples and/or measurements. Varying weights may be assigned different measurements. Optionally, measurements may be rejected if unduly corrupt. The averaging period may be adjusted according to the reliability of the measurements in some embodiments. More specifically, a general class of filters may be employed in processing the measurements. These filters may use mathematical models which (a) describe how physiological parameters change in time and/or (b) how these parameters relate to measurement in a noisy environment. The filters may adaptively modify a set of averaging weights and/or averaging times to optimally estimate the physiological parameters.

[0022] The present disclosure relates, in some embodiments, to devices, systems, and methods for estimating oxygen saturation (SpO_2). For example, a method for estimating SpO_2 may comprise (a) collecting optical oximetry data from a subject, and (b) processing the data to produce at least one oxygen saturation estimate. A system, in some embodiments, may take the natural logarithm of the optical oximetry data and then bandpass filter the data to get absorption-like data. A bandpass filter may strongly attenuate data below about 0.5

Hz and/or above about 10 Hz in an attempt to remove out-of-band noise. In other words, the bandpass filter may be designed to filter out frequencies that are not due to a cardiac pulse. This filtered data may be processed through two algorithms: a rate calculator and a saturation calculator. In some embodiments, an oxygen saturation estimate may be further processed to produce a modified saturation estimate (e.g., corrected to improve accuracy). This post-processing may comprise modifying the saturation estimate using a radial basis neural network.

[0023] According to some embodiments, the present disclosure relates to methods for reducing noise effects in a system for measuring a physiological parameter. A plurality of measurements may be generated corresponding to at least one wavelength of electromagnetic energy transmitted through living tissue. Selected measurements may be compared with at least one expected measurement characteristic. A variable weight may be assigned to each of the selected measurements based on the comparison, thereby generating a plurality of differently weighted measurements for each wavelength. A first number of weighted measurements may be averaged to obtain a filtered measurement, the first number varying according to the manner in which weights are assigned to a plurality of successive weighted measurements. A plurality of filtered measurements may be generated for each wavelength. The filtered measurements for each wavelength may be then combined and calculations resulting therefrom may be adaptively filtered using variable weights based on comparing the calculations to an expected calculation. A second number of the weighted calculations may be averaged to obtain a filtered calculation, the second number varying according to the manner in which weights are assigned to a plurality of successive weighted calculations.

[0024] According to some embodiments, a method for estimating SpO_2 may comprise post-processing and/or alarm handling strategies that include using a saturation noise estimate. For example, the saturation noise estimate may be used to correct the saturation estimate. Empirical data includes a number of events where the saturation estimate and saturation noise estimate are mirror images of each other. There are entire cases where the saturation estimate and saturation noise estimate are fairly well correlated. Thus, where this is true across a population, a corrected saturation estimate may be calculated as follows:

$$Sat' = Sat + k(\max(\text{noise} - m, 0)),$$

where k and m are determined empirically so as to minimize the saturation error.

[0025] In some embodiments, a saturation noise estimate may be used to determine whether a change in the saturation estimate is significant. For example, if the saturation noise estimate is high, small changes in the saturation estimate (e.g., changes that are within the range of the saturation noise estimate) may not be significant. On the other hand, if the saturation noise estimate is small, large changes in the saturation estimate (e.g., changes that exceed the saturation noise estimate) may be significant. For example, it may be desirable to show only those changes in the saturation estimate that have a 95% probability of being real. If a change in the saturation estimate is attended by a change in the saturation noise estimate from 2 points to 12 points, then the saturation estimate may be held unless the change in the saturation estimate changed by twice that delta (i.e., $2 \times (12 \text{ points} - 2 \text{ points}) = 20 \text{ points}$). It should be noted that the term "points"

may refer to percent saturation, as oxygen saturation is usually displayed in increments of 1%, from 0% to 100%. In other words, a single point may correspond to 1% oxygen saturation. It may not be desirable to continue to hold a saturation estimate if the saturation noise estimate drops below what it had been when the initial decision was made to hold it. For example, if a saturation estimate changes by 15 points, but the saturation noise estimate increases from 2 points to 12 points, the saturation estimate may be held (i.e., $15 < 20$). However, if the saturation noise estimate subsequently drops to 7 points (now, $2 \times \text{delta} = 10$ points), then the 15-point change in the saturation estimate is more likely to be real. Thus, it may be desirable to discontinue holding the saturation estimate. Alternatively, an assumption may be made that, on average, a held saturation estimate becomes progressively less accurate at a rate of perhaps 0.2 saturation points per second. In such a case, if the saturation noise estimate goes from 2 points to 12 points, the saturation noise estimate may be held for up to 50 seconds (i.e., $10 \text{ points} / 0.2 \text{ points/second} = 50 \text{ seconds}$).

[0026] A saturation noise estimate may be used, according to some embodiments, to determine the likelihood that the saturation has crossed the saturation threshold and exceeded some sat-time integral. The sat-time integral may be defined as the difference between the oxygen saturation value and its associated alarm threshold, integrated over time, such as is described in U.S. Pat. No. 5,865,736, which is incorporated herein by reference. During motion, an alarm may only be raised when the likelihood that the alarm condition has occurred is high. For example, a saturation of 80 may mean that there is a 50% probability that the saturation is above 80 and a 50% probability that it is below 80. In the absence of motion, with a 2 point accuracy spec, the probability that that saturation estimate of 80 is below an alarm threshold of 85 is virtually 100%. But if the saturation noise estimate is 5 points, then that saturation is only one standard deviation below the threshold of 85. There is about an 84 percent probability that the saturation is below the threshold and a 16 percent probability that it is above the threshold. So, a sat-time integral may be incremented only about 68 percent (i.e., the difference between 84% and 16%) as much as in the no motion case. The noisier the saturation estimate becomes, and the closer the saturation estimate gets to the alarm threshold, the slower this alarm integral may be incremented. The alarm integral may be decremented when the saturation estimate goes above the threshold, as this may indicate a greater probability that the physiological saturation is above rather than below the alarm threshold. Furthermore, the alarm integral may be set to zero when the saturation value indicates a very high probability that the physiological saturation is above the alarm threshold (i.e. the difference between the saturation value and the alarm threshold is more than one or two times the estimate of saturation accuracy derived from one or more signal quality or noise metrics indicative of saturation accuracy).

[0027] A radial basis neural network may be used for saturation estimation, according to some embodiments. A radial basis network may be a computer-implemented, single-hidden-layer network with n unique inputs, m nodes in the hidden layer, and a single linear node in the output layer. A unique feature of a radial basis network, in some embodiments, may be the equation used by its hidden nodes. Each node (a) may receive n inputs, (b) may have n associated

weights, and (c) may have a single bias. The equation for a node's output may be:

$$y = F(b * \text{distance}(x_1 \dots x_n, w_1 \dots w_n)),$$

[0028] where $x_1 \dots x_n$ denotes the inputs,

[0029] $w_1 \dots w_n$ denotes the weights,

[0030] b is the bias,

[0031] distance () is the distance between the x and w vectors in an n -dimensional space, and

$$F(x) = e^{-x^2}.$$

[0032] In some embodiments, a transfer function $F(x)$ may only have a high output when its input is near zero. This is shown in FIG. 1. Therefore, the output of each radial basis neuron may be a function of how close $x_1 \dots x_n$ is to the ideal inputs $w_1 \dots w_n$, and the size of the region within which the neuron will output a high value (> 0.5) may be proportional to b . The output of a radial basis network, therefore, may be a function of how close $x_1 \dots x_n$ is to the weights for each hidden neuron. Matrix-based methods for solving (determining) the weights for radial basis networks are known to those skilled in the art of signal processing, and are implemented in commonly used signal processing software, such as MATLAB®. A radial-basis neural network with the previously determined weights may then be implemented in system or apparatus embodying the invention.

[0033] Depending on the desired behavior, one skilled in the art of signal processing may define the value of b , thus controlling how much overlap there will be between the areas in the input space that each neuron is sensitive to. More overlap may be chosen to maximize coverage of the input space with a small network. Less overlap may be chosen if the neural net needed to respond very differently within narrow regions of the input space.

[0034] The ability to solve the weights for a radial basis neural network may pose an advantage over designs that apply some other types of neural networks to the same problem (i.e. accurate estimation of oxygen saturation). For example, training a backpropagation network may undesirably require that its initial weights be initialized to random values, followed by iterative training. Consequently, the weights may converge to very different values in different training sessions on the same data, and these different values may significantly impact the performance of the neural net. In contrast a radial basis neural network presented with the same training data will always have the same weights determined, making its behavior repeatable.

[0035] An engineer skilled in the art of signal processing, in some embodiments, may observe the weights of each hidden neuron to determine the region of data to which a neuron is sensitive. A backpropagation network, in some embodiments, may require a monotonic transfer function that causes a neuron's output to be high over one half of the input space, low in the other half, and changing rapidly over limited region near the boundary. Thus, in some embodiments, a radial basis network may be desirable for input spaces containing many local peaks and a backpropagation network may be desirable for inputs containing many edges.

[0036] In some embodiments, a radial basis neural network may receive an input vector that is well outside of the network's training set. If this circumstance is not otherwise addressed, the output of all the hidden nodes may be virtually zero, and the output layer may output whatever its default value (bias) is. However, where an outlying data set is identified (e.g., by a skilled engineer), an additional node centered

on this data may be specified and added to the hidden layer. This outlying data may then be added to the original training set. The output layer, which is always linear, may then be re-solved for the expanded training set, without having to redefine the rest of the hidden layer.

[0037] The present disclosure relates, according to some embodiments, to devices, systems, and methods for detecting oxygen saturation that crosses a threshold and/or falls within a range. For example, a method may comprise initiating or ending an alarm when an oxygen saturation estimate is below a threshold (e.g., below about 80%) or above a threshold (e.g., above about 95%). A method may comprise initiating or ending an alarm when an oxygen saturation estimate is within a selected and/or desired range. An alarm may include any type of alert that may be perceived by a human and/or a machine including, for example, a visible alert, an audible alert, and/or a tactile alert. Non-limiting examples of a visible alert include the appearance or change in appearance of text or an icon on a display and/or a blinking light (e.g., a red light). Non-limiting examples of an audible alert include an intermittent and/or continuous tone and/or playback of a recorded warning message. Non-limiting examples of a tactile alert include vibration or other movement of an object.

[0038] Embodiments of the present invention may facilitate calculation of corrected saturation values when only a single saturation value is available along with associated signal quality metrics. Further, when multiple saturation estimates and associated signal quality metrics are combined, a corrected saturation value calculated in accordance with present embodiments may not have a value between the multiple saturation estimates. Indeed, present embodiments may result in extrapolation as well as interpolation. It should be noted that, in accordance with present embodiments, the combining of saturation values and associated metrics to reduce bias may be specific to a sensor model or design. For example, combination for a reflectance sensor may differ from combination for a transmission sensor.

[0039] Some specific example embodiments of the disclosure may be illustrated by one or more of the examples provided herein.

EXAMPLE 1

Breathdown Procedure

[0040] Desaturation (hypoxia) was induced by reducing the amount of oxygen in the breathing gas delivered to the subject. Normoxia (resaturation) was restored by reverting to the original breathing gas mixture. Oxygen saturation was assessed on a moving and a non-moving hand.

[0041] Five desaturations and resaturations were caused in quick succession. Simultaneous data was collected from the four fingers of the moving hand and from one finger of the non-moving hand. The non-motion saturations were concatenated from each finger of the non-moving hand to form a target vector containing twenty desaturations (FIG. 2), each of which has a minima below 80 percent. The saturations computed from the moving hand by a prior-art algorithm or an algorithm embodying the present invention may likewise be concatenated (FIGS. 3-6) to form a test set. Thus, an ideal algorithm should report twenty desaturations below 80 percent on both the non-motion and motion data.

EXAMPLE 2

Prior Art Algorithm with Pulse-Synchronous Ensemble Averaging

[0042] A prior art algorithm that computes saturation with and without pulse-synchronous ensemble averaging was tested. FIG. 3 shows the non-pulse-synchronous ensemble averaging saturation computed using the data concatenated from the four moving fingers. Saturations below 80 are calculated (detected) for only 11 of the 20 desaturations. FIG. 4 shows the pulse-synchronous ensemble averaging saturation computed using the same motion data. Saturations below 80 are calculated for only 12 of the 20 desaturations. Different desaturations were missed by the two saturation estimates.

[0043] In addition to these two saturation estimates, the same prior art algorithm also computes two associated error and “saturation age” estimates, wherein each “error” estimate quantifies the degree to which processed two-wavelength photoplethysmographs used to calculate a given saturation estimate are not correlated, and each “saturation age” estimate quantifies the cumulative filtering (i.e. averaging occurring in each of multiple filtering steps) used in the calculation of a given saturation estimate. One of the “saturation age” estimates is highly correlated with its corresponding error estimates, but the other is not. It has been observed that these age or error estimates are sometimes mirror images of the saturation trace. Therefore, the prior art algorithm computes five semi-independent inputs that are correlated to saturations: 2 saturations, 2 error estimates, and 2 rates.

EXAMPLE 3

A Radial Basis Network

[0044] A Radial Basis network with 30 hidden neurons was solved for this training set of 5 inputs X 20 desaturation events, wherein the solving comprised determining the set of weights that minimizes the squared difference between the output of the Radial Basis neural net and the non-motion saturation estimate. The output is shown in FIG. 5.

[0045] Although the tracing in FIG. 5 contains some short-term noise, the network successfully estimated all 20 desaturations below 80. FIG. 6 shows the output of the neural net after further processing by a 20-second median filter to mitigate this noise.

[0046] FIGS. 3 and 4 show two estimates of oxygen saturation calculated with different signal processing, each of which demonstrate unique perturbations due to motion artifact. As the text describes, each trace of oxygen saturations is associated with metrics unique to that trace. FIG. 5 demonstrates that by combining multiple estimates of oxygen saturation, such as those shown in FIGS. 3 and 4, and signal quality metrics uniquely associated with each of the multiple estimates, that embodiments of the present invention may produce a corrected saturation estimate that is significantly more accurate than either of the input saturations by itself. This is apparent when the trace in FIG. 2 is compared with the traces represented in FIGS. 3-5.

[0047] FIG. 7 is a block diagram of a device or system for estimating oxygen saturation in the presence of motion artifact. The system is generally indicated by reference number 600. The system 600 (e.g., a computer) includes a processor 602 (e.g., a microprocessor) and a radial basis neural network 604 in communication with one another. The system 600 also

includes a display 606 in communication with the processor 602. The radial basis neural network 602 may include a single-hidden-layer network and may be computer-implemented. Indeed, the radial basis neural network 604 may be stored within a memory component of the processor 602.

[0048] The processor 602 may be configured to receive optical oximetry data from a patient or from another source (e.g., a database). Further, the processor 602 may be configured to process the optical oximetry data to produce at least one oxygen saturation estimate. Once the processor 602 has produced the at least one oxygen saturation estimate, the processor 602 may be configured to communicate the at least one oxygen saturation estimate to the radial basis neural network 604. The radial basis neural network 604 may be configured to modify the oxygen saturation estimate received from the processor 602 to reduce bias caused by motion artifact. For example, the radial basis neural network 604 may be configured to define a modified oxygen saturation estimate based on combining the at least one oxygen saturation estimate received from the processor 602 with one or more additional oxygen saturation estimates and corresponding signal quality metrics to reduce motion artifact bias. Once the modified oxygen saturation estimate has been established by the radial basis neural network 604, the radial basis neural network 604 may be configured to communicate the modified oxygen saturation estimate to the processor 602, which may be configured to present a representation of the modified oxygen saturation estimate on the display 606, which may be communicatively coupled with the processor 602.

[0049] As will be understood by those skilled in the art who have the benefit of the instant disclosure, other equivalent or alternative compositions, devices, methods, and systems for estimating oxygen saturation can be envisioned without departing from the description contained herein. Accordingly, the manner of carrying out the disclosure as shown and described is to be construed as illustrative only.

[0050] Persons skilled in the art may make various changes in the shape, size, number, and/or arrangement of parts without departing from the scope of the instant disclosure. For example, a device and/or system may include a single computer-implemented network per subject (e.g., patient) or a single computer-implemented network that serves two or more subjects. In addition, the size of a device and/or system may be scaled up or down to suit the needs and/or desires of a practitioner. Also, where ranges have been provided, the disclosed endpoints may be treated as exact and/or approximations as desired or demanded by the particular embodiment. In addition, it may be desirable in some embodiments to mix and match range endpoints. All or a portion of an oxygen saturation device and/or system may be configured and arranged to be disposable, serviceable, interchangeable, and/or replaceable. These equivalents and alternatives along with obvious changes and modifications are intended to be included within the scope of the present disclosure. Accordingly, the foregoing disclosure is intended to be illustrative, but not limiting, of the scope of the disclosure as illustrated by the following claims.

What is claimed is:

1. A device for estimating oxygen saturation in the presence of noise, the device comprising:

a processor in communication with a neural network, wherein the processor is configured to receive oximetry data, process the oximetry data to produce at least one oxygen saturation estimate, communicate the at least

one oxygen saturation estimate to the neural network, and receive a modified oxygen saturation estimate from the neural network comprising less noise bias than the at least one oxygen saturation estimate, wherein the neural network is configured to define the modified oxygen saturation estimate based at least in part on combining the at least one oxygen saturation estimate with corresponding signal quality metrics; and

a display in communication with the processor, wherein the display is configured to display a representation of the modified oxygen saturation estimate.

2. The device of claim 1, wherein the neural network comprises a radial basis neural network.

3. The device of claim 2, wherein the radial basis neural network comprises a single-hidden-layer network.

4. The device of claim 3, wherein the single-hidden-layer network has a plurality of nodes, and each node of the plurality of nodes includes one or more associated weights and a single bias.

5. The device of claim 4, wherein the single bias of at least one node of the plurality of nodes is in the range of about 5% oxygen saturation to about 10% oxygen saturation.

6. The device of claim 4, wherein the single bias of at least one node in the plurality of nodes is in the range of about 1% oxygen saturation to about 5% oxygen saturation.

7. The device of claim 1, wherein the neural network is configured to define the modified oxygen saturation estimate based at least in part on combining the at least one oxygen saturation estimate with one or more additional oxygen saturation estimates.

8. The device of claim 7, wherein the modified oxygen saturation estimate has a value that is not between the values of the at least one oxygen saturation estimate and the one or more additional oxygen saturation estimates.

9. The device of claim 1, wherein the processor is configured to compare the modified oxygen saturation estimate with a hypoxia oxygen saturation threshold and to initiate an alarm if the modified oxygen saturation estimate is less than or equal to the hypoxia oxygen saturation threshold.

10. The device of claim 9, wherein the alarm comprises one or more of a visible alert, an audible alert, a tactile alert, or any combination thereof

11. A method for estimating oxygen saturation in the presence of noise, the method comprising:

generating at least one oxygen saturation estimate using the processor;

communicating the at least one oxygen saturation estimate to a neural network using the processor;

receiving, at the processor, a modified oxygen saturation estimate from the neural network comprising less noise bias than the at least one oxygen saturation estimate, wherein the neural network defines the modified oxygen saturation estimate based at least in part on combining the at least one oxygen saturation estimate with corresponding signal quality metrics; and

presenting, via the processor, a representation of the modified oxygen saturation estimate on a display that is in communication with the processor.

12. The method of claim 11, wherein the neural network comprises a radial basis neural network.

13. The method of the claim 12, wherein the radial basis neural network comprises a single-hidden-layer network.

14. The method of claim **13**, wherein the single-hidden-layer network has a plurality of nodes, and each node of the plurality of nodes includes one or more associated weights and a single bias.

15. The method of claim **11**, wherein the neural network defines the modified oxygen saturation estimate based at least in part on combining the at least one oxygen saturation estimate with one or more additional oxygen saturation estimates.

16. The method of claim **15**, wherein the modified oxygen saturation estimate has a value that is not between the values of the at least one oxygen saturation estimate and the one or more additional oxygen saturation estimates.

17. The method of claim **11**, comprising comparing the modified oxygen saturation estimate with a hypoxia oxygen saturation threshold using the processor and initiating an alarm, via the processor, if the modified oxygen saturation estimate is less than or equal to the hypoxia oxygen saturation threshold.

18. The method of claim **11**, comprising receiving oximetry data from a pulse oximeter at the processor and generating the at least one oxygen saturation estimate based on the received oximetry data, using the processor.

19. A system for estimating oxygen saturation in the presence of noise, the system comprising:

a processor in communication with a radial basis neural network, wherein the processor is configured to process oximetry data to produce at least one oxygen saturation estimate, the radial basis neural network is configured to receive the at least one oxygen saturation estimate from the processor and to modify the at least one oxygen saturation estimate based on corresponding signal quality metrics indicative of an accuracy of the at least one oxygen saturation estimate to define a modified oxygen saturation estimate having less noise bias than the at least one oxygen saturation, and the processor is configured to provide an output indicative of the modified oxygen saturation estimate.

20. The system of claim **19**, wherein the processor is configured to compare the modified oxygen saturation estimate with a hypoxia oxygen saturation threshold and to initiate an alarm if the modified oxygen saturation estimate is less than or equal to the hypoxia oxygen saturation threshold.

* * * * *

专利名称(译)	在存在噪声的情况下改进氧饱和度估计的方法		
公开(公告)号	US20140371554A1	公开(公告)日	2014-12-18
申请号	US14/472038	申请日	2014-08-28
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	BAKE JR CLARK R		
发明人	BAKE, JR., CLARK R.		
IPC分类号	A61B5/00 A61B5/1455		
CPC分类号	A61B5/7203 A61B5/14551 A61B5/7264 A61B5/7455 A61B5/7405 A61B5/742 A61B5/7282 G16H50/20		
外部链接	Espacenet USPTO		

摘要(译)

根据一些实施例，本公开涉及用于在存在噪声的情况下估计生理参数的设备，系统和方法。例如，在一些实施例中，本公开涉及用于评估（例如，估计，测量，计算）氧饱和度（SpO₂）的装置，系统和方法。评估SpO₂的方法可以包括评估与运动伪影相关联的噪声度量。在一些实施例中，可以将噪声度量的百分比（例如，经验确定的百分比）简单地添加到SpO₂估计以产生校正的SpO₂估计。根据一些实施例，血氧测定算法可以包括组合多个内部SpO₂估计和相关联的噪声和/或信号质量度量（例如，使用径向基础神经网络）以产生修改的（例如，校正的）SpO₂估计（例如，而不仅仅是从有限数量的候选人中选择估计数。修改的SpO₂估计可以包括很少或没有基于移动的错误。

