



US 20160100765A1

(19) **United States**(12) **Patent Application Publication**
MUEHLSTEFF et al.(10) **Pub. No.: US 2016/0100765 A1**(43) **Pub. Date: Apr. 14, 2016**(54) **NON-INVASIVE BLOOD PRESSURE
MONITOR AND METHOD OF OPERATING
THE SAME**(52) **U.S. CL.**
CPC **A61B 5/022** (2013.01); **A61B 5/7235**
(2013.01)


(71) Applicant: , EINDHOVEN (NL)

(72) Inventors: **Jens MUEHLSTEFF**, Aachen (DE);
Teun VAN DEN HEUVEL, Eindhoven
(NL); **Erik BRESCH**, Eindhoven (NL);
Lars SCHMITT, Aachen (DE); **Dieter
WOEHRLE**, Waiblingen (DE)(57) **ABSTRACT**

According to an aspect there is provided a method of obtaining a measurement of the blood pressure of a subject using a non-invasive blood pressure, NIBP, monitor and including using a pulse rate sensor and a cuff that is to be placed around a limb of the subject, the method comprising using the pulse rate sensor to obtain information on the pulse rate of the subject; adapting a pressure signal filter according to the obtained information on the pulse rate of the subject; starting inflation of the cuff; obtaining a pressure signal representing the pressure in the cuff as the cuff is inflated; filtering the pressure signal using the adapted pressure signal filter during inflation of the cuff; and processing the filtered pressure signal to obtain a blood pressure measurement for the subject during inflation of the cuff.

(21) Appl. No.: **14/857,883**(22) Filed: **Sep. 18, 2015**(30) **Foreign Application Priority Data**

Oct. 10, 2014 (EP) 14188411.4

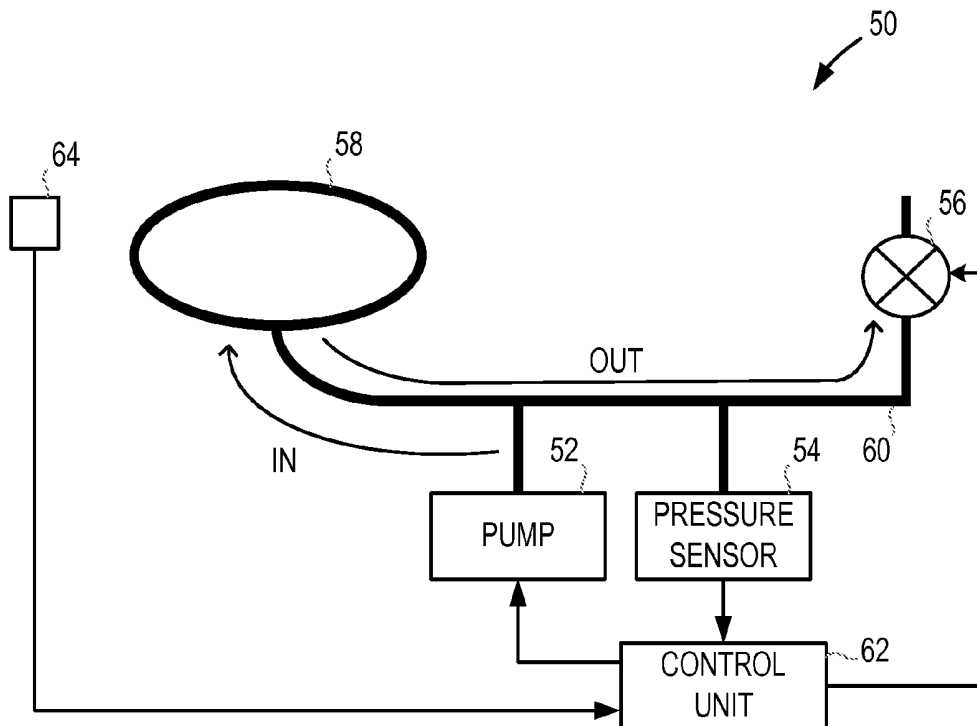Publication Classification(51) **Int. Cl.**
A61B 5/022 (2006.01)
A61B 5/00 (2006.01)

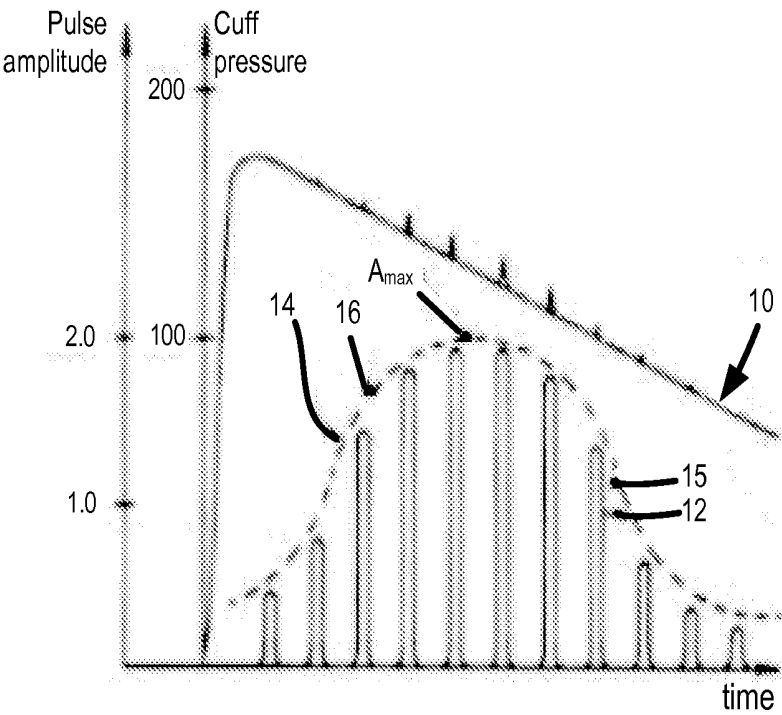


Fig. 1

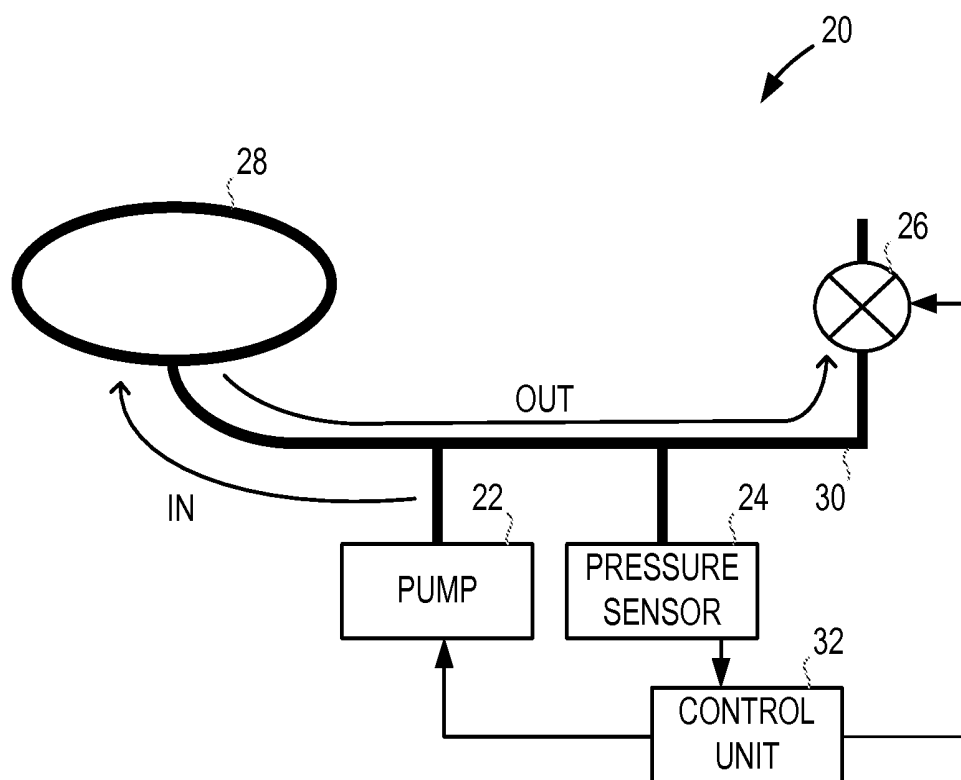


Fig. 2

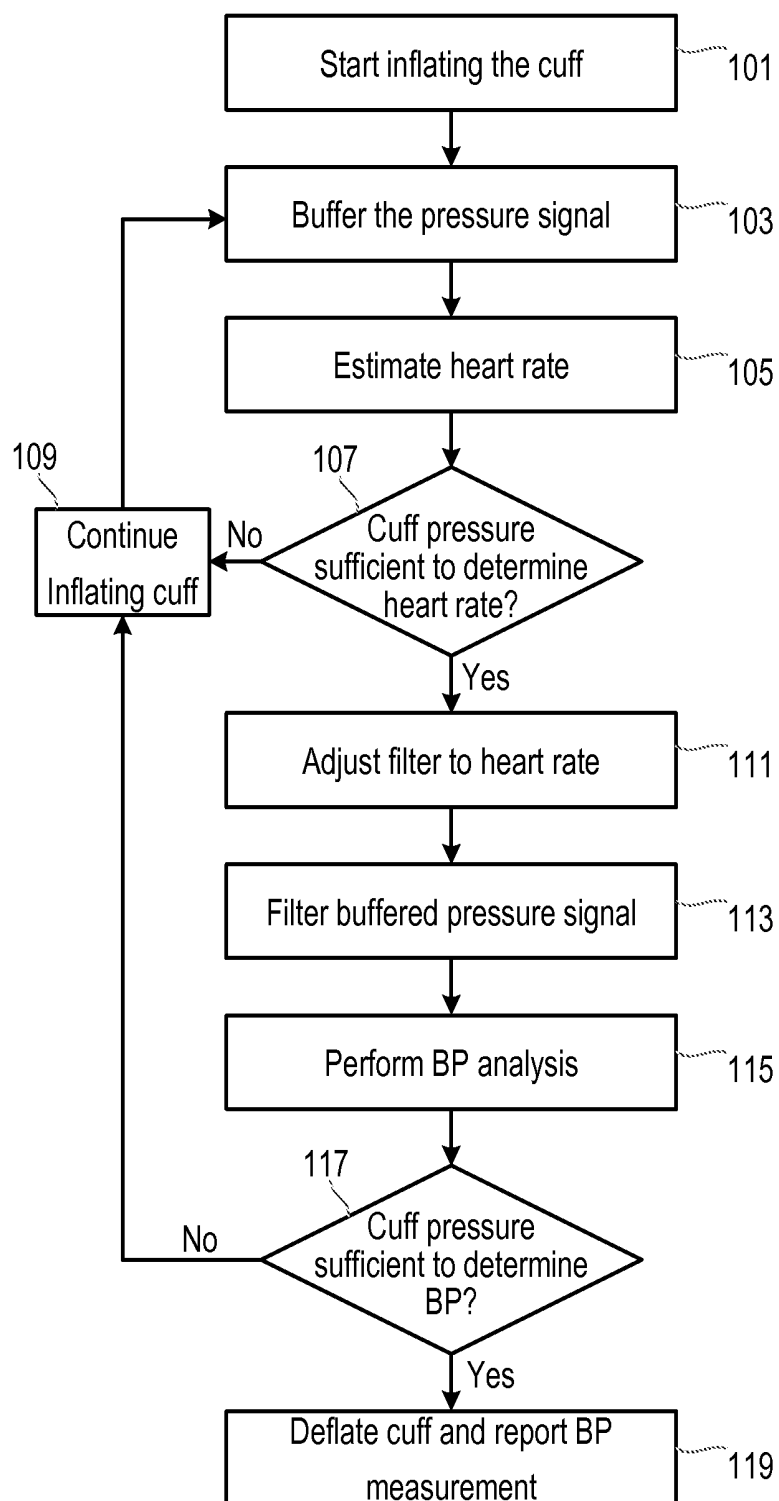


Fig. 3

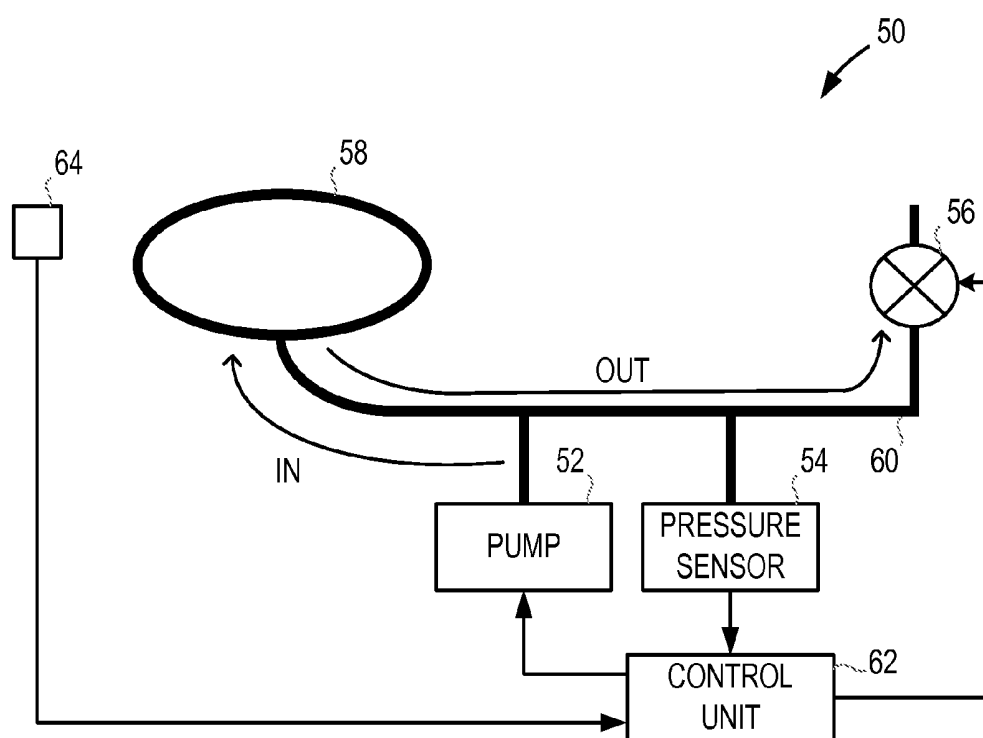


Fig. 4

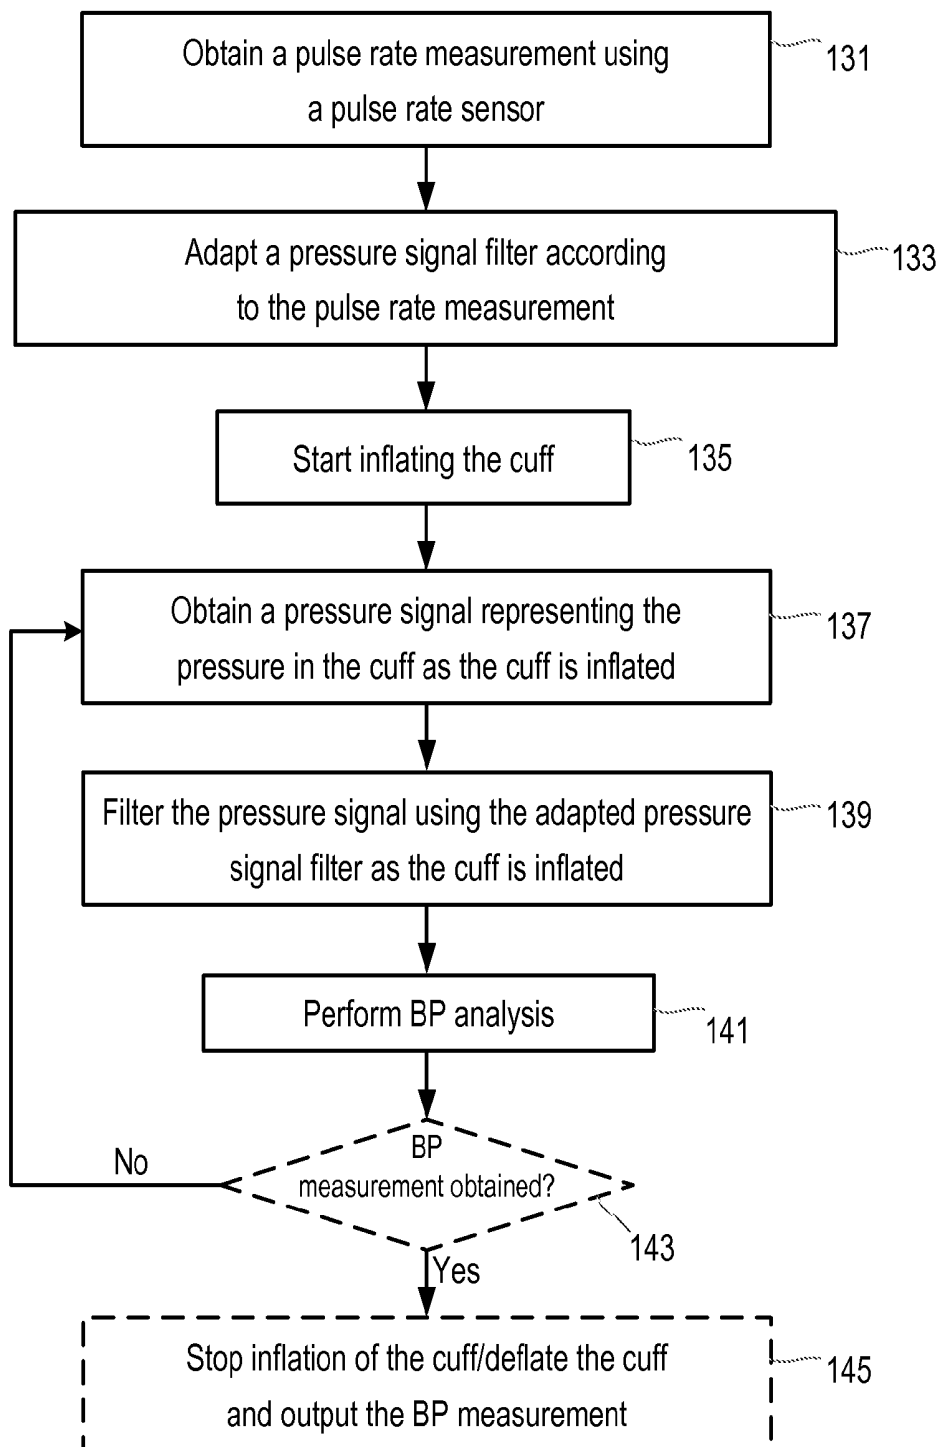


Fig. 5

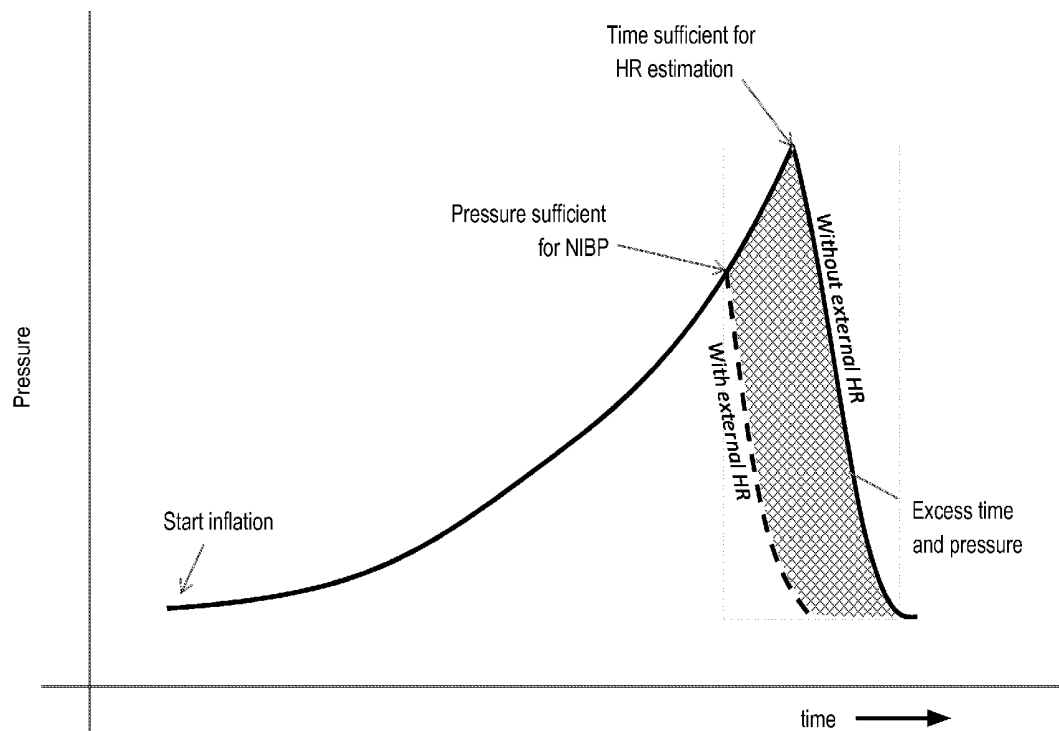


Fig. 6

NON-INVASIVE BLOOD PRESSURE MONITOR AND METHOD OF OPERATING THE SAME

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of EP provisional application serial no. 14188411.4 filed Oct. 10, 2014, which is incorporated herein by reference.

TECHNICAL FIELD OF THE INVENTION

[0002] The invention relates to a non-invasive blood pressure (NIBP) monitor and a method of operating the same, and in particular relates to improving the comfort of the blood pressure measurements obtained by such a monitor.

BACKGROUND TO THE INVENTION

[0003] Arterial blood pressure (BP) is one of the most important vital signs and is widely used in clinical practice. Non-invasive arterial blood pressure (NIBP) is usually measured by slowly varying the pressure in a cuff that is wrapped around the upper arm of a subject. The BP is determined either by measuring sound distal from the cuff (the auscultatory method, based on Korotkoff sounds) or by measuring pressure pulsations in the cuff caused by volume pulsations of the arm and brachial artery and extracting features from the envelope of these pressure pulses (the oscillometric method). The oscillometric method is easily automated and is widely used.

[0004] The principle behind a typical oscillometric method is illustrated by FIG. 1, which shows a graph of cuff pressure 10, and a processed high pass filtered trace 12 of this cuff pressure, versus time. The left-hand y-axis shows pulse amplitude, the right-hand y-axis shows cuff pressure, and the x-axis shows time. To perform a NIBP measurement using the oscillometric method, first the cuff pressure 10 is ramped up until it is sufficiently larger than systolic blood pressure. After ramp up, the cuff is deflated (in FIG. 1 the deflation is done gradually, but step wise deflation is also possible). During the deflation, small oscillations in cuff pressure occur, caused by volume changes in the bladder of the cuff, which are in turn caused by volume changes in the brachial artery. The measured cuff pressure 10 is high pass filtered, and the resulting trace 12 shows the cuff pressure oscillations due to volume changes in the brachial artery. An envelope 14 of the oscillation amplitudes is determined. The maximum A_{max} of this pulse envelope 14 is taken as a reference point for determining the systolic 16 and diastolic pressure 15. The systolic pressure 16 is determined as the cuff pressure where the pressure oscillation is approximately 0.8 times the maximum amplitude A_{max} at a pressure higher than the pressure at the reference point. The diastolic pressure 15 is determined as the cuff pressure where the pressure oscillation is approximately 0.55 times the maximum amplitude A_{max} at a pressure lower than the pressure at the reference point. These ratios are based on empirical values (see, e.g., L A Geddes et. al., *Annals of Biomedical Engineering* 10 pp 271-280. 1982). The exact algorithms that are employed by manufacturers of blood pressure devices to determine systolic and diastolic pressures are usually trade secrets.

[0005] The typical monitor 20 used for acquiring oscillometric NIBP measurements is illustrated in FIG. 2. A pump 22, a pressure sensor 24, and a valve 26 are connected to a cuff

28 by tubing 30. A control unit 32 is connected to the pump 22 and the valve 26 to control the operation of those components, and is also connected to the pressure sensor 24 in order to receive the signal representing the pressure of the gas in the cuff 28 (the 'pressure signal'). The control unit 32 runs the algorithm that controls the pump 22 and valve 26 and processes the pressure signal from the pressure sensor 24 to determine the BP measurement. During execution of the oscillometric method the pump 22 blows air into the cuff 28, thereby inflating it. The pressure sensor 24 measures the gas pressure in the system (and therefore the pressure of the gas in the cuff 28) and outputs a signal representing the pressure in the cuff 28 (referred to as the 'pressure signal'). When a pressure larger than systolic pressure is reached, the pump 22 is disabled or switched off, the valve 26 is opened and slow (or step wise) deflation occurs, during which the cuff pressure is continuously measured and the measurements (pressure signal) stored. The pump 22 and valve 26 are controlled by control unit 32, which also receives the cuff pressure measurements and calculates the pulse envelope and the systolic and diastolic pressure using these measurements. In practice the monitor 20 may comprise multiple sensors and valves for safety reasons.

[0006] The operation of the typical monitor 20 is often uncomfortable for the subject (and in some cases is painful), since the arm is compressed with an external pressure. In a clinical or hospital (or even home) setting where blood pressure measurements need to be obtained through the day and night, the taking of a blood pressure measurement by the monitor 20 will often disturb the sleep of the subject. NIBP monitors originally developed for high acuity subjects (e.g. those in an intensive care unit (ICU)) were optimized for accuracy and precision, but not the comfort of the subject.

[0007] In a home setting, it has been found that NIBP measurements have a relatively low acceptance by subjects (e.g. the subjects do not comply with the required measurement schedule or do not perform the measurements properly), which in some cases is due to the pain caused by the inflation of the cuff (which can relate to the duration that the cuff is inflated for and/or the peak pressure in the cuff), irritation of skin under the cuff (particularly on NIBP monitors that are continuously worn by a subject), haematomas, and disturbance of the sleep of the subject.

[0008] The comfort of the NIBP measurement can be improved in any or all of three areas: the total measurement time (where a reduction is desired), the maximum cuff pressure reached (where a lower maximum pressure is desired) and the integral of cuff pressure over time (where a smaller integral is desired). Of course, this increase in comfort should not come at the expense of the accuracy of the NIBP measurement beyond acceptable limits.

[0009] In addition to the types of monitor described above in which the BP is measured using envelope detection during deflation of the cuff (which can typically take around 45 seconds), monitors have been developed that can measure the BP while the cuff is being inflated. This can reduce the total measurement time (in some cases to around 20 seconds), since the deflation stage can be very quick once the BP measurement has been obtained, and therefore can result in a measurement that is more comfortable for the subject. However, there is further scope for improving the comfort of these inflation-based BP measurements.

[0010] Therefore there is a need for an NIBP monitor and method of operating the same that measures the blood pres-

sure during inflation of the cuff and that is more comfortable for the subject than conventional monitors.

SUMMARY OF THE INVENTION

[0011] According to a first aspect, there is provided a method of obtaining a measurement of the blood pressure of a subject using a non-invasive blood pressure, NIBP, monitor that comprises a pulse rate sensor and a cuff that is to be placed around a limb of the subject, the method comprising using the pulse rate sensor to obtain information on the pulse rate of the subject; adapting a pressure signal filter according to the obtained information on the pulse rate of the subject; starting inflation of the cuff; obtaining a pressure signal representing the pressure in the cuff as the cuff is inflated; filtering the pressure signal using the adapted pressure signal filter during inflation of the cuff; and processing the filtered pressure signal to obtain a blood pressure measurement for the subject during inflation of the cuff.

[0012] In some embodiments the step of using the pulse rate sensor to obtain information on the pulse rate of the subject is performed prior to starting the inflation of the cuff.

[0013] In some embodiments the step of adapting the pressure signal filter is performed prior to starting the inflation of the cuff.

[0014] In some embodiments the steps of using the pulse rate sensor to obtain information on the pulse rate of the subject and adapting the pressure signal filter are also performed during inflation of the cuff.

[0015] In some embodiments the step of adapting the pressure signal filter comprises adapting the frequency characteristics of the filter according to the obtained information on the pulse rate of the subject.

[0016] In some embodiments the method further comprises the step of stopping the inflation of the cuff when a blood pressure measurement has been obtained.

[0017] In some embodiments the method further comprises the step of deflating the cuff once the blood pressure measurement has been obtained.

[0018] In some embodiments the method further comprises the step of performing a measurement of the blood pressure during deflation of the cuff if the step of processing the filtered pressure signal to obtain a blood pressure measurement for the subject does not provide a measurement of the blood pressure or an acceptable measurement.

[0019] In some embodiments the pulse rate sensor is an accelerometer, a photoplethysmograph, PPG, sensor or an electrocardiograph, ECG, sensor.

[0020] In preferred embodiments the pulse rate sensor is a different sensor to the sensor that measures the pressure in the cuff.

[0021] In preferred embodiments the information on the pulse rate of the subject is not obtained from the pressure signal.

[0022] In some embodiments the NIBP monitor further comprises a pump for inflating the cuff.

[0023] According to a second aspect there is provided a computer program product comprising a computer readable medium having computer readable code embodied therein, the computer readable code being configured such that, on execution by a suitable computer, processor or control unit, the computer, processor or control unit is caused to perform any of the methods described above.

[0024] According to a third aspect, there is provided a non-invasive blood pressure, NIBP, monitor for measuring the

blood pressure of a subject, the NIBP monitor comprising a control unit that is configured to obtain information on the pulse rate of the subject from a pulse rate sensor; adapt a pressure signal filter according to the obtained information on the pulse rate of the subject; control a pump to start inflating a cuff; obtain a pressure signal representing the pressure in the cuff as the cuff is inflated; filter the pressure signal using the adapted pressure signal filter during inflation of the cuff; and process the filtered pressure signal to obtain a blood pressure measurement for the subject during inflation of the cuff.

[0025] In some embodiments the NIBP monitor further comprises a pulse rate sensor for measuring the pulse rate of the subject and for providing information on the pulse rate to the control unit.

[0026] In some embodiments the pulse rate sensor is an accelerometer, a photoplethysmograph, PPG, sensor or an electrocardiograph, ECG, sensor.

[0027] In some embodiments the control unit is configured to obtain the information on the pulse rate of the subject prior to controlling the pump to start inflating the cuff.

[0028] In some embodiments the control unit is configured to adapt the pressure signal filter prior to controlling the pump to start inflating the cuff.

[0029] In some embodiments the control unit is further configured to obtain information on the pulse rate of the subject from the pulse rate sensor and to adapt the pressure signal filter during inflation of the cuff.

[0030] In some embodiments the control unit is configured to adapt the pressure signal filter by adapting the frequency characteristics of the filter according to the obtained information on the pulse rate of the subject.

[0031] In some embodiments the control unit is further configured to control the pump to stop the inflation of the cuff when a blood pressure measurement has been obtained.

[0032] In some embodiments the control unit is further configured to deflate the cuff once the blood pressure measurement has been obtained.

[0033] In some embodiments the control unit is further configured to obtain a measurement of the blood pressure during deflation of the cuff if the processing of the filtered pressure signal does not provide a measurement of the blood pressure or an acceptable measurement of the blood pressure.

[0034] In preferred embodiments the pulse rate sensor is a different sensor to the sensor that measures the pressure in the cuff.

[0035] In preferred embodiments the control unit does not obtain the information on the pulse rate of the subject from the pressure signal.

[0036] In some embodiments the NIBP monitor further comprises a cuff; a pump for inflating the cuff; and a pressure sensor for measuring the pressure in the cuff and for outputting a pressure signal representing the pressure in the cuff to the control unit.

BRIEF DESCRIPTION OF THE DRAWINGS

[0037] For a better understanding of the invention, and to show more clearly how it may be carried into effect, reference will now be made, by way of example only, to the accompanying drawings, in which:

[0038] FIG. 1 is a graph of cuff pressure versus time measured using a conventional oscillometric NIBP monitor;

[0039] FIG. 2 shows a block diagram of a conventional oscillatory NIBP monitor;

[0040] FIG. 3 is a flow chart illustrating an exemplary method for performing an inflation-based BP measurement;

[0041] FIG. 4 is a block diagram of an NIBP monitor according to an embodiment of the invention;

[0042] FIG. 5 is a flow chart illustrating a method of operating a NIBP monitor to obtain an inflation-based BP measurement according to an aspect of the invention; and

[0043] FIG. 6 is a graph illustrating the improvements in BP measurements provided by the invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0044] As described above, measuring the blood pressure (BP) of a subject during inflation of a cuff, rather than during deflation of the cuff from a peak pressure that is sufficient to prevent blood flow in the limb, allows the BP measurement to be completed more quickly, which helps to improve the comfort of the BP measurement for the subject.

[0045] The flow chart in FIG. 3 illustrates an exemplary method for performing an inflation-based measurement using the monitor 20 shown in FIG. 2. Briefly, in this method, information about the subject's heart rate is obtained from the pressure signal and used to adapt a filter that is applied to the pressure signal in order to obtain the BP measurement.

[0046] In step 101 inflation of the cuff 28 is started, and the pressure signal representing the pressure in the system is buffered (step 103). In order to obtain a reliable BP measurement, the subject's blood pressure range (diastolic to systolic) needs to be sampled over a certain number of heart cycles (beats). This certain number of heart cycles puts an upper limit on the rate at which the cuff can be inflated from the diastolic pressure to the systolic pressure (since if the cuff is inflated too quickly there will not be enough heart cycles in the signal representing the pressures between diastolic and systolic pressure to obtain a reliable BP measurement). Thus, in step 101 the cuff 28 is inflated at a rate that will allow a sufficient number of heart cycles in the diastolic to systolic range to be measured (typically this rate is set based on an assumption of the lowest possible heart rate in order to ensure that a sufficient number of heart cycles are captured).

[0047] In step 105, the buffered pressure signal is processed to determine the heart rate of the subject. This step typically requires the cuff to be at a certain pressure for the heart rate signal to be observed, and a substantial length or duration of pressure signal (e.g. covering a few heart beats) is required in order to be able to extract the heart rate information. If the pressure in the cuff is not yet sufficient to determine the heart rate (as determined in step 107), then no heart rate will be determined in step 105, and the method passes to step 109 in which inflation of the cuff 28 continues and the pressure signal continues to be buffered (step 103). In some embodiments, step 105 can comprise estimating the autocorrelation function of the buffered pressure signal and then finding a peak in that function that most likely corresponds to the subject's heart rate. In some cases the amplitude of the peak can be compared to a threshold to determine if the peak has a sufficient magnitude to represent the heart rate. If the amplitude of the peak exceeds the threshold, the peak can be used as the estimate of the heart rate.

[0048] If the heart rate can be extracted from the pressure signal in step 105, the method passes to step 111 in which the heart rate is used to adapt a filter that is to be applied to the pressure signal. Once the filter has been adapted to the heart rate of the subject, the buffered pressure signal can be filtered

(step 113) and an analysis of the filtered pressure signal performed to determine the BP (step 115). The filter is a high-pass filter, similar to the high-pass filter used in the traditional oscillometric method. The heart rate (HR) is used to adapt the frequency characteristics of the filter, e.g. the cut-off frequency. In some embodiments, the cut-off frequency can be set to the heart rate (e.g. 60 beats per minute, bpm=1 Hz), but in other embodiments the cut-off frequency may be (slightly) higher or lower than the heart rate (depending on details of the filter design and other processing steps). Generally, the higher the heart rate, the higher the cut-off frequency of the filter (and vice versa). In one example, a basic moving average filter is used, whereby the width of the averaging window is set to correspond to the heart period ($=1/\text{HR}$). Running this filter over the pressure signal returns a low-pass filtered pressure signal, which is then subtracted from the original pressure signal to obtain the high-pass filtered pressure signal.

[0049] If the pressure in the cuff 28 is not yet sufficient to determine the BP (e.g. if the cuff pressure has not yet reached the systolic pressure) then the inflation of the cuff continues (step 109). At this stage, as the heart rate has already been determined, it may not be necessary to continue processing the pressure signal to extract the current heart rate (step 105) and adapt the filter (step 111), so the method can return to step 113 after step 109 and the filter can be applied to newly buffered pressure signal data. In other implementations, the extraction of the heart rate and adaptation of the filter can be a continuous process, in which case the method can return to step 103. If at step 115 a BP measurement is determined from the pressure signal, then the method passes to step 119 in which the inflation of the cuff 28 by the pump 22 is stopped, the cuff 28 is deflated and the BP measurement can be reported to the subject, other operator of the monitor 20 or a remote computer or base unit that collates and stores the BP measurement information for the subject.

[0050] Thus, in this method, obtaining a BP measurement during inflation of the cuff 28 requires information about the subject's heart rate in order to be able to filter the pressure signal appropriately. Since estimating the heart rate from the pressure signal during inflation requires a certain pressure in the cuff for a substantial length of time (e.g. covering a few heart beats), there can be a delay in being able to perform the BP measurement processing while the heart rate information is extracted (and hence a delay in being able to determine that inflation of the cuff 28 can be stopped), by which time the cuff 28 may have been inflated beyond the maximum pressure required to complete the BP measurement. This can cause discomfort for the subject due to excess pressure and duration of the BP measurement.

[0051] Therefore, the invention provides that heart rate information (particularly the pulse rate of the subject) used to adapt the filter applied to the pressure signal is obtained from a different, separate sensor, rather than being derived from the pressure signal itself. This means that heart rate information is available continuously throughout the inflation of the cuff, and the disadvantages with the method in FIG. 3 can be overcome. In particular, the processing of the pressure signal to obtain the BP measurement can start as soon as the inflation of the cuff starts (instead of when a sufficient pressure has been reached in the cuff to enable the heart rate information to be derived), which increases the chances of the inflation of the cuff being stopped at the earliest opportunity (i.e. when the systolic pressure is reached).

[0052] A non-invasive blood pressure (NIBP) monitor according to an embodiment of the invention is shown in FIG. 4. The monitor **50** comprises a pump **52**, a pressure sensor **54**, and a valve **56** that are connected to a cuff **58** by tubing **60**. A control unit **62** is connected to the pump **52** and the valve **56** to control the operation of those components, and is also connected to the pressure sensor **54** in order to receive the signal representing the pressure of the gas in the cuff **58** (the 'pressure signal'). The control unit **62** runs the algorithm that controls the pump **52** and valve **56** and processes the pressure signal from the pressure sensor **54** to determine the BP measurement. The control unit **62** can comprise one or more processors that are configured or programmed to control the operation of the components of the NIBP monitor **50** and obtain the BP measurement.

[0053] As in the conventional monitor, the pump **52** is for blowing air or other gas into the cuff **58** in order to inflate the cuff **58** and prevent blood flow in the limb around which the cuff **58** is placed. The valve **56** is used to allow air or gas out of the system and thus deflate the cuff **58**.

[0054] In accordance with an embodiment of the invention, the monitor **50** further comprises a pulse rate sensor **64** that is for measuring the pulse rate of the subject while the cuff **58** is being inflated. The pulse sensor **64** can be any suitable type of sensor that measures the pulse rate of the subject, and that is able to obtain a pulse rate measurement at any required time (e.g. as required by the BP measurement algorithm).

[0055] In some embodiments, the sensor **64** is a photoplethysmography (PPG) sensor, an accelerometer or an ECG sensor, although those skilled in the art will be aware of other types of heart rate sensor that can be used (such as a camera, radar, impedance cardiogram, heart sound sensor, etc.). In the case of a PPG sensor, accelerometer and/or ECG sensor, the sensor **64** can comprise the appropriate sensing apparatus, e.g. light source and detector for a PPG sensor, accelerometer, and two or more electrodes for an ECG sensor, and the processing of the signals from those sensors to determine the pulse rate can be performed by the control unit **62**. In the case of an accelerometer, the acceleration signal can be processed to extract the movements caused by the beating of the heart/pulses of blood in the circulatory system.

[0056] In use, the pulse rate sensor **64** is attached to or otherwise in contact with the appropriate part of the body of the subject in order to measure the pulse rate. It will be appreciated that in some embodiments, the sensor **64** can be integrated with the cuff **58** so the subject only has to place the cuff around their arm in order to start using the monitor **50**, whereas in other embodiments the sensor **64** can be separate from the cuff **58** and placed separately on the body of the subject. In some embodiments, there can be a wired connection between the sensor **64** and the control unit **62**, whereas in other embodiments, the sensor **64** can communicate with the control unit **62** wirelessly.

[0057] It will be appreciated that FIG. 4 only shows the components required to illustrate this aspect of the invention, and in a practical implementation the NIBP monitor **50** will comprise additional components to those shown. For example, the monitor **50** may comprise multiple pressure sensors **54** and valves **56** for safety reasons, a battery or other power supply for powering the monitor **50**, a memory module for storing program code and/or the BP measurements, a communication module for enabling the BP measurements to be communicated to a base unit for the monitor **50** or a remote computer, and/or one or more user interface components that

allow a user (e.g. the subject or healthcare professional) to interact and control the monitor). Also, in embodiments of the invention the pulse rate sensor **64** need not form part of the monitor **50** as such, with instead the monitor **50** being arranged to obtain information on the pulse rate of the subject from a separately provided pulse rate sensor **64**.

[0058] The flow chart in FIG. 5 illustrates a method of obtaining a measurement of the blood pressure of a subject during inflation of a cuff according to the invention. This method can be implemented by a NIBP monitor **50** as shown in FIG. 4, and it will be appreciated that in some embodiments the NIBP monitor **50** can comprise computer program code for enabling the control unit **62** to perform the method.

[0059] In the first step, step **131**, the pulse rate sensor **64** is used to obtain a measurement of the pulse rate of the subject. This step is first performed at the start of the BP measurement process, preferably just prior to starting the inflation of the cuff **58** by pump **52**, although in some embodiments it can be performed as, or just after, inflation of the cuff **58** is started. In any case, the measurement of the pulse rate is available much earlier in the process than in the exemplary method above in which the pulse rate information has to be derived from the pressure signal.

[0060] Once the measurement of the pulse rate has been obtained, the filter that is applied to the pressure signal as part of the process for determining the BP measurement is adapted according to the pulse rate measurement (step **133**). As in the method of FIG. 3, in step **133** the filter can be a high-pass filter, similar to the high-pass filter used in the traditional oscillometric method. The pulse rate (PR) is used to adapt the frequency characteristics of the filter, e.g. the cut-off frequency. In some embodiments, the cut-off frequency can be set to the heart rate (e.g. 60 beats per minute, bpm=1 Hz), but in other embodiments the cut-off frequency may be set (slightly) higher or lower than the heart rate (depending on details of the filter design and other processing steps). Generally, the higher the heart rate, the higher the cut-off frequency of the filter (and vice versa). In one example, a basic moving average filter is used, whereby the width of the averaging window is set to correspond to the heart period ($=1/PR$). Running this filter over the pressure signal returns a low-pass filtered pressure signal, which is then subtracted from the original pressure signal to obtain the high-pass filtered pressure signal.

[0061] The inflation of the cuff **58** is started (step **135**) and a pressure signal representing the pressure in the cuff **58** is obtained (step **137**).

[0062] Next, this pressure signal is filtered using the adapted filter (step **139**). This filtering is performed during inflation of the cuff **58**, and preferably in real time as the pressure signal is obtained (or as near to real time as is possible). The filtered pressure signal is then analyzed to determine the BP measurement (step **141**). Those skilled in the art will be aware of various techniques for performing this analysis, and therefore further details are not provided herein. Again, this step is performed during inflation of the cuff **58**, and preferably in real time (or as near to real time as is possible).

[0063] If a BP measurement cannot be obtained from the pressure signal (e.g. if the pressure in the cuff **58** has not yet reached the systolic blood pressure in the subject), then following step **143** the inflation of the cuff **58** continues and the method returns to step **137** where the pressure signal continues to be obtained, filtered and analyzed. If a BP measurement

is obtained in step **141**, the method passes to step **145** in which the inflation of the cuff **58** is stopped and the deflation of the cuff **58** is started (e.g. by opening valve **56**). Since the BP measurement has been obtained, the deflation is preferably performed as fast as possible. The deflation is preferably initiated as soon as or immediately after the BP measurement has been obtained. The BP measurement can be reported to the subject, other operator of the monitor **50** or a remote computer or base unit that collates and stores the BP measurement information for the subject.

[0064] The graph in FIG. **6** illustrates the reduction in measurement time and maximum pressure that is possible with an external heart rate (HR)/pulse rate measurement according to the invention shown in FIG. **5**. It can be seen that if the heart rate information is obtained from the pressure signal itself, by the time the heart rate information has been derived, the pressure in the cuff may have already exceeded that required to complete the BP measurement, which leads to a longer measurement time and higher peak pressure in the cuff than is required.

[0065] Instead, by obtaining the heart rate information (particularly the pulse rate of the subject) from a different, separate sensor **64** (and therefore not from the pressure signal), the heart rate information is available continuously throughout the inflation of the cuff **58**, which means that the processing of the pressure signal to obtain the BP measurement can start as soon as the inflation of the cuff **58** starts (and thus always starts before the systolic pressure is reached in the cuff **58**) and therefore the BP measurement can be obtained at the earliest opportunity.

[0066] In some embodiments, since the pulse rate of the subject can change over the course of the BP measurement process, the pulse rate sensor **64** can also be used to obtain measurements of the pulse rate of the subject during inflation of the cuff **58**, and those measurements can be used to adapt the filter to the current pulse rate of the subject. This helps to ensure that the filter is up to date for the current pulse rate of the subject and therefore provide a BP measurement that is as accurate as possible.

[0067] In some embodiments, if for any reason the analysis in step **141** is unable to obtain a BP measurement (or a BP measurement that is reliable), for example if the subject moves during the measurement process or experiences an arrhythmia, the control unit **62** can control the NIBP monitor **50** to perform a conventional deflation-based BP measurement. Thus, when the systolic pressure has been exceeded (or when a preset maximum inflation pressure has been reached without being able to obtain a BP measurement) the control unit **62** can control the pump **52** to stop inflating the cuff **58**, and operate the valve **56** to release pressure from the cuff **58** in a controlled manner. The pressure signal from the pressure sensor **54** obtained while the cuff **58** deflates is analyzed by the control unit **62** using a conventional deflation-based algorithm to determine the blood pressure of the subject.

[0068] There is therefore provided an NIBP monitor and a method of operating the same that measures the blood pressure of a subject during inflation of the cuff and that is more comfortable for the subject than measurements made according to conventional methods or by conventional monitors.

[0069] While the invention has been illustrated and described in detail in the drawings and foregoing description, such illustration and description are to be considered illustrative or exemplary and not restrictive; the invention is not limited to the disclosed embodiments.

[0070] Variations to the disclosed embodiments can be understood and effected by those skilled in the art in practicing the claimed invention, from a study of the drawings, the disclosure and the appended claims. In the claims, the word “comprising” does not exclude other elements or steps, and the indefinite article “a” or an does not exclude a plurality. A single processor or other unit may fulfil the functions of several items recited in the claims. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage. A computer program may be stored/distributed on a suitable medium, such as an optical storage medium or a solid-state medium supplied together with or as part of other hardware, but may also be distributed in other forms, such as via the Internet or other wired or wireless telecommunication systems. Any reference signs in the claims should not be construed as limiting the scope.

1. A method of obtaining a measurement of the blood pressure of a subject using a non-invasive blood pressure, NIBP, monitor and including using a pulse rate sensor, a cuff that is to be placed around a limb of the subject and a pressure sensor for measuring the pressure in the cuff, wherein the pulse rate sensor is a different sensor to the pressure sensor, the method comprising:

- using the pulse rate sensor to obtain information on the pulse rate of the subject;
- adapting a pressure signal filter according to the obtained information on the pulse rate of the subject;
- starting inflation of the cuff;
- obtaining a pressure signal using the pressure sensor, the pressure signal representing the pressure in the cuff as the cuff is inflated;
- filtering the pressure signal using the adapted pressure signal filter during inflation of the cuff; and
- processing the filtered pressure signal to obtain a blood pressure measurement for the subject during inflation of the cuff.

2. A method as claimed in claim **1**, wherein step of using the pulse rate sensor to obtain information on the pulse rate of the subject is performed prior to starting the inflation of the cuff.

3. A method as claimed in claim **2**, wherein the step of adapting the pressure signal filter is performed prior to starting the inflation of the cuff.

4. A method as claimed in claim **2**, wherein the steps of using the pulse rate sensor to obtain information on the pulse rate of the subject and adapting the pressure signal filter are also performed during inflation of the cuff.

5. A method as claimed in claim **1**, the method further comprising the step of deflating the cuff once the blood pressure measurement has been obtained.

6. A method as claimed in claim **1**, the method further comprising the step of performing a measurement of the blood pressure during deflation of the cuff if the step of processing the filtered pressure signal to obtain a blood pressure measurement for the subject does not provide a measurement of the blood pressure or an acceptable measurement.

7. A method as claimed in claim **1**, wherein the step of adapting the pressure signal filter comprises adapting the frequency characteristics of the filter according to the obtained information on the pulse rate of the subject.

8. A computer program product comprising a computer readable medium having computer readable code embodied therein, the computer readable code being configured such

that, on execution by a suitable computer, processor or control unit that is for use with a non-invasive blood pressure, NIBP, monitor and including use of a pulse rate sensor, a cuff that is to be placed around a limb of the subject and a pressure sensor for measuring the pressure in the cuff, wherein the pulse rate sensor is a different sensor to the pressure sensor, the computer, processor or control unit is caused to perform the method of claim 1.

9. A non-invasive blood pressure, NIBP, monitor for measuring the blood pressure of a subject, the NIBP monitor comprising:

a control unit that is configured to:

obtain information on the pulse rate of the subject from a pulse rate sensor;

adapt a pressure signal filter according to the obtained information on the pulse rate of the subject;

control a pump to start inflating a cuff;

obtain a pressure signal using a pressure sensor, the pressure signal representing the pressure in the cuff as the cuff is inflated;

filter the pressure signal using the adapted pressure signal filter during inflation of the cuff; and

process the filtered pressure signal to obtain a blood pressure measurement for the subject during inflation of the cuff;

wherein the pulse rate sensor is a different sensor to the pressure sensor.

10. A NIBP monitor as claimed in claim 9, wherein the NIBP monitor further comprises a pulse rate sensor for measuring the pulse rate of the subject and for providing information on the pulse rate to the control unit.

11. A NIBP monitor as claimed in claim 9, wherein the control unit is configured to obtain the information on the pulse rate of the subject prior to controlling the pump to start inflating the cuff.

12. A NIBP monitor as claimed in claim 11, wherein the control unit is configured to adapt the pressure signal filter prior to controlling the pump to start inflating the cuff.

13. A NIBP monitor as claimed in claim 11, wherein the control unit is further configured to obtain information on the pulse rate of the subject from the pulse rate sensor and to adapt the pressure signal filter during inflation of the cuff.

14. A NIBP monitor as claimed in claim 9, wherein the control unit is configured to adapt the pressure signal filter by adapting the frequency characteristics of the filter according to the obtained information on the pulse rate of the subject.

15. A NIBP monitor as claimed in claim 9, wherein the NIBP monitor further comprises:

a cuff;

a pump for inflating the cuff; and

a pressure sensor for measuring the pressure in the cuff and for outputting a pressure signal representing the pressure in the cuff to the control unit.

* * * * *

专利名称(译)	无创血压监测仪及其操作方法		
公开(公告)号	US20160100765A1	公开(公告)日	2016-04-14
申请号	US14/857883	申请日	2015-09-18
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	MUEHLSTEFF JENS VAN DEN HEUVEL TEUN BRESCH ERIK SCHMITT LARS WOEHRLE DIETER		
发明人	MUEHLSTEFF, JENS VAN DEN HEUVEL, TEUN BRESCH, ERIK SCHMITT, LARS WOEHRLE, DIETER		
IPC分类号	A61B5/022 A61B5/00		
CPC分类号	A61B5/7235 A61B5/022 A61B5/02225 A61B5/024 A61B5/72 A61B5/725		
优先权	2014188411 2014-10-10 EP		
外部链接	Espacenet USPTO		

摘要(译)

根据一个方面，提供了一种使用非侵入性血压，NIBP，监视器获得对象的血压测量的方法，并且包括使用脉搏率传感器和将被放置在肢体周围的袖带。该方法包括使用脉率传感器获得关于受试者脉搏率的信息；根据获得的关于受试者脉搏率的信息调整压力信号滤波器；开始袖带充气；当袖带充气时，获得表示袖带中的压力的压力信号；在袖带充气期间使用适配的压力信号滤波器过滤压力信号；并且处理过滤后的压力信号以在袖带充气期间获得对象的血压测量值。

