



US009622693B2

(12) **United States Patent**
Diab

(10) **Patent No.:** **US 9,622,693 B2**
(45) **Date of Patent:** ***Apr. 18, 2017**

(54) **SYSTEMS AND METHODS FOR DETERMINING BLOOD OXYGEN SATURATION VALUES USING COMPLEX NUMBER ENCODING**

(71) Applicant: **Cercacor Laboratories, Inc.**, Irvine, CA (US)

(72) Inventor: **Mohamed K. Diab**, Ladera Ranch, CA (US)

(73) Assignee: **MASIMO CORPORATION**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/609,841**

(22) Filed: **Jan. 30, 2015**

(65) **Prior Publication Data**

US 2015/0201874 A1 Jul. 23, 2015

Related U.S. Application Data

(63) Continuation of application No. 13/896,731, filed on May 17, 2013, now Pat. No. 8,948,835, which is a (Continued)

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
A61B 5/024 (2006.01)

(52) **U.S. Cl.**
CPC **A61B 5/14551** (2013.01); **A61B 5/02416** (2013.01); **A61B 5/7207** (2013.01); (Continued)

(58) **Field of Classification Search**

CPC A61B 5/14551; A61B 5/1455; A61B 5/14552; A61B 5/7207; A61B 5/7253; A61B 5/743; A61B 5/742; A61B 5/7239
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,051,522 A 9/1977 Healy
4,085,378 A 4/1978 Ryan
(Continued)

FOREIGN PATENT DOCUMENTS

DE 3328862 A1 2/1985
EP 0104771 B1 4/1984
(Continued)

OTHER PUBLICATIONS

US 8,845,543, 09/2014, Diab et al. (withdrawn)
(Continued)

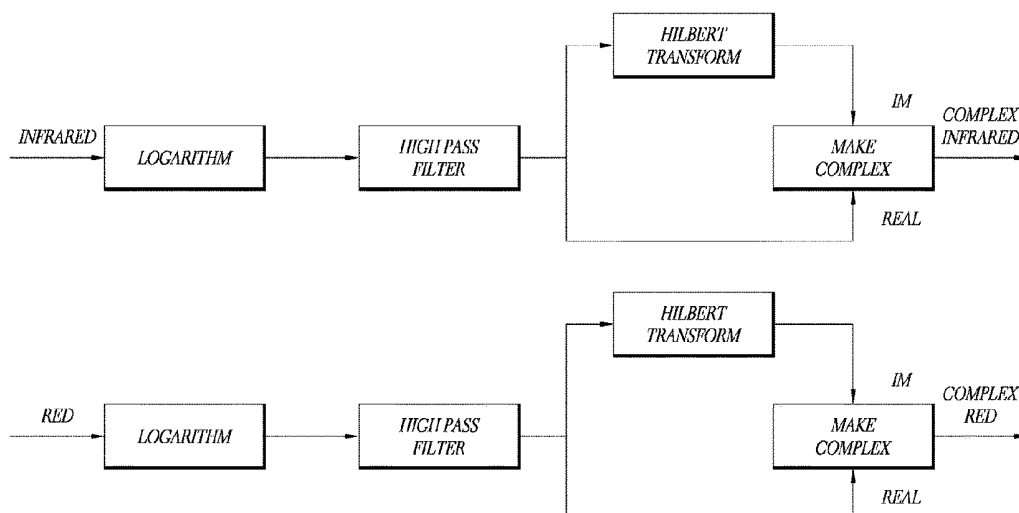
Primary Examiner — Eric Winakur

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

The disclosure includes pulse oximetry systems and methods for determining point-by-point saturation values by encoding photoplethysmographs in the complex domain and processing the complex signals. The systems filter motion artifacts and other noise using a variety of techniques, including statistical analysis such as correlation, or phase filtering.

17 Claims, 28 Drawing Sheets



Related U.S. Application Data

continuation of application No. 12/248,868, filed on Oct. 9, 2008, now Pat. No. 8,447,374, which is a continuation of application No. 11/288,812, filed on Nov. 28, 2005, now Pat. No. 7,440,787, which is a continuation of application No. 10/727,348, filed on Dec. 3, 2003, now Pat. No. 6,970,792.

(60) Provisional application No. 60/430,834, filed on Dec. 4, 2002.

(52) U.S. Cl.

CPC *A61B 5/7253* (2013.01); *A61B 5/7278* (2013.01); *A61B 5/742* (2013.01); *A61B 5/743* (2013.01); *A61B 5/7239* (2013.01)

(56) References Cited

U.S. PATENT DOCUMENTS

4,623,248 A	11/1986	Sperinde	5,448,991 A	9/1995	Polson et al.
4,653,498 A	3/1987	New	5,452,717 A	9/1995	Branigan et al.
4,745,398 A	5/1988	Abel	D363,120 S	10/1995	Savage et al.
4,765,340 A	8/1988	Sakai	5,456,252 A	10/1995	Vari et al.
4,800,495 A	1/1989	Smith	5,479,934 A	1/1996	Imran
4,802,486 A	2/1989	Goodman	5,481,620 A	1/1996	Vaidyanathan
4,863,265 A	9/1989	Flower	5,482,036 A	1/1996	Diab et al.
4,870,588 A	9/1989	Merhav	5,490,505 A	2/1996	Diab et al.
4,911,167 A	3/1990	Corenman	5,494,043 A	2/1996	O'Sullivan et al.
4,934,372 A	6/1990	Corenman et al.	5,503,148 A	4/1996	Pologe
4,942,877 A	7/1990	Sakai	5,533,511 A	7/1996	Kaspari et al.
4,955,379 A	9/1990	Hall	5,534,851 A	7/1996	Russek
4,960,128 A	10/1990	Gordon et al.	5,542,421 A	8/1996	Erdman
4,964,408 A	10/1990	Hink et al.	5,549,111 A	8/1996	Wright et al.
4,965,840 A	10/1990	Subbarao	5,561,275 A	10/1996	Savage et al.
5,003,252 A	3/1991	Nystrom	5,562,002 A	10/1996	Lalin
RE33,643 E	7/1991	Isaacson et al.	5,575,284 A	11/1996	Athan
5,041,187 A	8/1991	Hink et al.	5,588,435 A	12/1996	Weng et al.
5,069,213 A	12/1991	Polczynski	5,590,649 A	1/1997	Caro et al.
5,163,438 A	11/1992	Gordon et al.	5,602,924 A	2/1997	Durand et al.
5,170,791 A	12/1992	Boos et al.	5,608,820 A	3/1997	Vaidyanathan
5,188,108 A	2/1993	Secker	5,610,996 A	3/1997	Eller
5,190,038 A	3/1993	Polson	5,632,272 A	5/1997	Diab et al.
5,193,124 A	3/1993	Subbarao	5,638,816 A	6/1997	Kiani-Azarbayjany et al.
5,218,962 A	6/1993	Mannheimer	5,638,818 A	6/1997	Diab et al.
5,226,417 A	7/1993	Swedlow	5,645,440 A	7/1997	Tobler et al.
5,246,002 A	9/1993	Prosser	5,652,566 A	7/1997	Lambert
5,259,381 A	11/1993	Cheung	5,685,299 A	11/1997	Diab et al.
5,270,942 A	12/1993	Reed	5,720,293 A	2/1998	Quinn
5,307,284 A	4/1994	Brunfeldt et al.	D393,830 S	4/1998	Tobler et al.
5,319,355 A	6/1994	Russek	5,743,262 A	4/1998	Lepper, Jr. et al.
5,331,394 A	7/1994	Shalon et al.	5,758,644 A	6/1998	Diab et al.
5,337,744 A	8/1994	Branigan	5,760,910 A	6/1998	Lepper, Jr. et al.
5,341,805 A	8/1994	Stavridi et al.	5,769,785 A	6/1998	Diab et al.
5,345,510 A	9/1994	Singhi	5,782,237 A	7/1998	Casciani
5,353,356 A	10/1994	Waugh et al.	5,782,757 A	7/1998	Diab et al.
5,355,882 A	10/1994	Ukawa	5,785,659 A	7/1998	Caro et al.
5,357,965 A	10/1994	Hall et al.	5,791,347 A	8/1998	Flaherty et al.
5,368,224 A	11/1994	Richardson	5,810,734 A	9/1998	Caro et al.
D353,195 S	12/1994	Savage et al.	5,820,267 A	10/1998	Baker, Jr. et al.
D353,196 S	12/1994	Savage et al.	5,823,950 A	10/1998	Diab et al.
5,377,676 A	1/1995	Vari et al.	5,830,131 A	11/1998	Caro et al.
5,384,451 A	1/1995	Smith et al.	5,833,618 A	11/1998	Caro et al.
5,398,003 A	3/1995	Heyl et al.	5,842,979 A	12/1998	Jarman
5,404,003 A	4/1995	Smith	5,853,364 A	12/1998	Baker, Jr. et al.
5,406,952 A	4/1995	Barnes	5,860,919 A	1/1999	Kiani-Azarbayjany et al.
D359,546 S	6/1995	Savage et al.	5,865,736 A	2/1999	Baker, Jr. et al.
5,421,329 A	6/1995	Casciani	5,890,929 A	4/1999	Mills et al.
5,431,170 A	7/1995	Mathews	5,891,023 A	4/1999	Lynn
D361,840 S	8/1995	Savage et al.	5,904,654 A	5/1999	Wohlmann et al.
5,438,983 A	8/1995	Falcone	5,919,134 A	7/1999	Diab
5,442,940 A	8/1995	Secker	5,921,921 A	7/1999	Potratz et al.
5,445,156 A *	8/1995	Daft G01S 15/8979	5,934,925 A	8/1999	Tobler et al.
		600/454	5,940,182 A	8/1999	Lepper, Jr. et al.
D362,063 S	9/1995	Savage et al.	5,950,139 A	9/1999	Korycan
			5,987,343 A	11/1999	Kinast
			5,995,855 A	11/1999	Kiani et al.
			5,997,343 A	12/1999	Mills et al.
			6,002,952 A	12/1999	Diab et al.
			6,011,986 A	1/2000	Diab et al.
			6,027,452 A	2/2000	Flaherty et al.
			6,036,642 A	3/2000	Diab et al.
			6,045,509 A	4/2000	Caro et al.
			6,047,203 A	4/2000	Sackner et al.
			6,064,910 A	5/2000	Andersson et al.
			6,067,462 A	5/2000	Diab et al.
			6,081,735 A	6/2000	Diab et al.
			6,083,172 A	7/2000	Baker, Jr. et al.
			6,088,607 A	7/2000	Diab et al.
			6,110,522 A	8/2000	Lepper, Jr. et al.
			6,119,026 A	9/2000	McNulty et al.
			6,122,535 A	9/2000	Kaestle et al.
			6,124,597 A	9/2000	Shehada
			6,128,521 A	10/2000	Marro et al.
			6,129,675 A	10/2000	Jay
			6,135,952 A	10/2000	Coetzee
			6,144,868 A	11/2000	Parker
			6,151,516 A	11/2000	Kiani-Azarbayjany et al.
			6,152,754 A	11/2000	Gerhardt et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,157,850	A	12/2000	Diab et al.	6,792,300	B1	9/2004	Diab et al.
6,165,005	A	12/2000	Mills et al.	6,813,511	B2	11/2004	Diab et al.
6,184,521	B1	2/2001	Coffin, IV et al.	6,816,741	B2	11/2004	Diab
6,188,407	B1	2/2001	Smith et al.	6,822,564	B2	11/2004	Al-Ali
6,206,830	B1	3/2001	Diab et al.	6,826,419	B2	11/2004	Diab et al.
6,229,856	B1	5/2001	Diab et al.	6,830,711	B2	12/2004	Mills et al.
6,232,609	B1	5/2001	Snyder et al.	6,850,787	B2	2/2005	Weber et al.
6,236,872	B1	5/2001	Diab et al.	6,850,788	B2	2/2005	Al-Ali
6,241,683	B1	6/2001	Macklem et al.	6,852,083	B2	2/2005	Caro et al.
6,253,097	B1	6/2001	Aronow et al.	6,861,639	B2	3/2005	Al-Ali
6,256,523	B1	7/2001	Diab et al.	6,898,452	B2	5/2005	Al-Ali et al.
6,263,222	B1	7/2001	Diab et al.	6,920,345	B2	7/2005	Al-Ali et al.
6,278,522	B1	8/2001	Lepper, Jr. et al.	6,931,268	B1	8/2005	Kiani-Azarbayjany et al.
6,280,213	B1	8/2001	Tobler et al.	6,934,570	B2	8/2005	Kiani et al.
6,285,896	B1	9/2001	Tobler et al.	6,939,305	B2	9/2005	Flaherty et al.
6,301,493	B1	10/2001	Marro et al.	6,943,348	B1	9/2005	Coffin, IV
6,317,627	B1	11/2001	Ennen et al.	6,950,687	B2	9/2005	Al-Ali
6,321,100	B1	11/2001	Parker	6,961,598	B2	11/2005	Diab
6,325,761	B1	12/2001	Jay	6,970,792	B1	11/2005	Diab
6,334,065	B1	12/2001	Al-Ali et al.	6,979,812	B2	12/2005	Al-Ali
6,343,224	B1	1/2002	Parker	6,985,764	B2	1/2006	Mason et al.
6,349,228	B1	2/2002	Kiani et al.	6,993,371	B2	1/2006	Kiani et al.
6,360,114	B1	3/2002	Diab et al.	6,996,427	B2	2/2006	Ali et al.
6,368,283	B1	4/2002	Xu et al.	6,999,904	B2	2/2006	Weber et al.
6,371,921	B1	4/2002	Caro et al.	7,003,338	B2	2/2006	Weber et al.
6,377,829	B1	4/2002	Al-Ali	7,003,339	B2	2/2006	Diab et al.
6,388,240	B2	5/2002	Schulz et al.	7,015,451	B2	3/2006	Dalke et al.
6,397,091	B2	5/2002	Diab et al.	7,024,233	B2	4/2006	Ali et al.
6,430,437	B1	8/2002	Marro	7,027,849	B2	4/2006	Al-Ali
6,430,525	B1	8/2002	Weber et al.	7,030,749	B2	4/2006	Al-Ali
6,463,311	B1	10/2002	Diab	7,039,449	B2	5/2006	Al-Ali
6,470,199	B1	10/2002	Kopotic et al.	7,041,060	B2	5/2006	Flaherty et al.
6,501,975	B2	12/2002	Diab et al.	7,044,918	B2	5/2006	Diab
6,505,059	B1	1/2003	Kollias et al.	7,067,893	B2	6/2006	Mills et al.
6,515,273	B2	2/2003	Al-Ali	7,096,052	B2	8/2006	Mason et al.
6,519,486	B1	2/2003	Edgar, Jr. et al.	7,096,054	B2	8/2006	Abdul-Hafiz et al.
6,519,487	B1	2/2003	Parker	7,132,641	B2	11/2006	Schulz et al.
6,525,386	B1	2/2003	Mills et al.	7,142,901	B2	11/2006	Kiani et al.
6,526,300	B1	2/2003	Kiani et al.	7,149,561	B2	12/2006	Diab
6,541,756	B2	4/2003	Schulz et al.	7,186,966	B2	3/2007	Al-Ali
6,542,764	B1	4/2003	Al-Ali et al.	7,190,261	B2	3/2007	Al-Ali
6,580,086	B1	6/2003	Schulz et al.	7,215,984	B2	5/2007	Diab
6,584,336	B1	6/2003	Ali et al.	7,215,986	B2	5/2007	Diab
6,595,316	B2	7/2003	Cybulski et al.	7,221,971	B2	5/2007	Diab
6,597,932	B2	7/2003	Tian et al.	7,225,006	B2	5/2007	Al-Ali et al.
6,597,933	B2	7/2003	Kiani et al.	7,225,007	B2	5/2007	Al-Ali
6,606,511	B1	8/2003	Ali et al.	RE39,672	E	6/2007	Shehada et al.
6,632,181	B2	10/2003	Flaherty et al.	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,639,668	B1	10/2003	Trepagnier	7,245,953	B1	7/2007	Parker
6,640,116	B2	10/2003	Diab	7,254,429	B2	8/2007	Schurman et al.
6,643,530	B2	11/2003	Diab et al.	7,254,431	B2	8/2007	Al-Ali
6,650,917	B2	11/2003	Diab et al.	7,254,433	B2	8/2007	Diab et al.
6,654,624	B2	11/2003	Diab et al.	7,254,434	B2	8/2007	Schulz et al.
6,658,276	B2	12/2003	Kianl et al.	7,272,425	B2	9/2007	Al-Ali
6,661,161	B1	12/2003	Lanzo et al.	7,274,955	B2	9/2007	Kiani et al.
6,671,531	B2	12/2003	Al-Ali et al.	D554,263	S	10/2007	Al-Ali
6,678,543	B2	1/2004	Diab et al.	7,280,858	B2	10/2007	Al-Ali et al.
6,684,090	B2	1/2004	Ali et al.	7,289,835	B2	10/2007	Mansfield et al.
6,684,091	B2	1/2004	Parker	7,292,883	B2	11/2007	De Felice et al.
6,697,656	B1	2/2004	Al-Ali	7,295,866	B2	11/2007	Al-Ali
6,697,657	B1	2/2004	Shehada et al.	7,328,053	B1	2/2008	Diab et al.
6,697,658	B2	2/2004	Al-Ali	7,332,784	B2	2/2008	Mills et al.
RE38,476	E	3/2004	Diab et al.	7,340,287	B2	3/2008	Mason et al.
6,699,194	B1	3/2004	Diab et al.	7,341,559	B2	3/2008	Schulz et al.
6,714,804	B2	3/2004	Al-Ali et al.	7,343,186	B2	3/2008	Lamego et al.
RE38,492	E	4/2004	Diab et al.	D566,282	S	4/2008	Al-Ali et al.
6,721,582	B2	4/2004	Trepagnier et al.	7,355,512	B1	4/2008	Al-Ali
6,721,585	B1	4/2004	Parker	7,356,365	B2	4/2008	Schurman
6,725,075	B2	4/2004	Al-Ali	7,371,981	B2	5/2008	Abdul-Hafiz
6,728,560	B2	4/2004	Kollias et al.	7,373,193	B2	5/2008	Al-Ali et al.
6,735,459	B2	5/2004	Parker	7,373,194	B2	5/2008	Weber et al.
6,745,060	B2	6/2004	Diab et al.	7,376,453	B1	5/2008	Diab et al.
6,760,607	B2	7/2004	Al-Ali	7,377,794	B2	5/2008	Al-Ali et al.
6,770,028	B1	8/2004	Ali et al.	7,377,899	B2	5/2008	Weber et al.
6,771,994	B2	8/2004	Kiani et al.	7,383,070	B2	6/2008	Diab et al.
				7,415,297	B2	8/2008	Al-Ali et al.
				7,428,432	B2	9/2008	Ali et al.
				7,438,683	B2	10/2008	Al-Ali et al.
				7,440,787	B2	10/2008	Diab

(56)

References Cited

U.S. PATENT DOCUMENTS

7,454,240 B2	11/2008	Diab et al.	8,046,042 B2	10/2011	Diab et al.
7,467,002 B2	12/2008	Weber et al.	8,048,040 B2	11/2011	Kiani
7,469,157 B2	12/2008	Diab et al.	8,050,728 B2	11/2011	Al-Ali et al.
7,471,969 B2	12/2008	Diab et al.	RE43,169 E	2/2012	Parker
7,471,971 B2	12/2008	Diab et al.	8,118,620 B2	2/2012	Al-Ali et al.
7,483,729 B2	1/2009	Al-Ali et al.	8,126,528 B2	2/2012	Diab et al.
7,483,730 B2	1/2009	Diab et al.	8,128,572 B2	3/2012	Diab et al.
7,489,958 B2	2/2009	Diab et al.	8,130,105 B2	3/2012	Al-Ali et al.
7,496,391 B2	2/2009	Diab et al.	8,145,287 B2	3/2012	Diab et al.
7,496,393 B2	2/2009	Diab et al.	8,150,487 B2	4/2012	Diab et al.
D587,657 S	3/2009	Al-Ali et al.	8,175,672 B2	5/2012	Parker
7,499,741 B2	3/2009	Diab et al.	8,180,420 B2	5/2012	Diab et al.
7,499,835 B2	3/2009	Weber et al.	8,182,443 B1	5/2012	Kiani
7,500,950 B2	3/2009	Al-Ali et al.	8,185,180 B2	5/2012	Diab et al.
7,509,154 B2	3/2009	Diab et al.	8,190,223 B2	5/2012	Al-Ali et al.
7,509,494 B2	3/2009	Al-Ali	8,190,227 B2	5/2012	Diab et al.
7,510,849 B2	3/2009	Schurman et al.	8,203,438 B2	6/2012	Kiani et al.
7,526,328 B2	4/2009	Diab et al.	8,203,704 B2	6/2012	Merritt et al.
7,530,942 B1	5/2009	Diab	8,224,411 B2	7/2012	Al-Ali et al.
7,530,949 B2	5/2009	Al Ali et al.	8,228,181 B2	7/2012	Al-Ali
7,530,955 B2	5/2009	Diab et al.	8,229,533 B2	7/2012	Diab et al.
7,563,110 B2	7/2009	Al-Ali et al.	8,233,955 B2	7/2012	Al-Ali et al.
7,596,398 B2	9/2009	Al-Ali et al.	8,244,325 B2	8/2012	Al-Ali et al.
7,618,375 B2	11/2009	Flaherty	8,255,026 B1	8/2012	Al-Ali
D606,659 S	12/2009	Kiani et al.	8,255,027 B2	8/2012	Al-Ali et al.
7,647,083 B2	1/2010	Al-Ali et al.	8,255,028 B2	8/2012	Al-Ali et al.
D609,193 S	2/2010	Al-Ali et al.	8,260,577 B2	9/2012	Weber et al.
D614,305 S	4/2010	Al-Ali et al.	8,265,723 B1	9/2012	McHale et al.
RE41,317 E	5/2010	Parker	8,274,360 B2	9/2012	Sampath et al.
7,729,733 B2	6/2010	Al-Ali et al.	8,301,217 B2	10/2012	Al-Ali et al.
7,734,320 B2	6/2010	Al-Ali	8,310,336 B2	11/2012	Muhsin et al.
7,761,127 B2	7/2010	Al-Ali et al.	8,315,683 B2	11/2012	Al-Ali et al.
7,761,128 B2	7/2010	Al-Ali et al.	RE43,860 E	12/2012	Parker
7,764,982 B2	7/2010	Dalke et al.	8,337,403 B2	12/2012	Al-Ali et al.
D621,516 S	8/2010	Kiani et al.	6,970,792 C1	1/2013	Diab
7,791,155 B2	9/2010	Diab	8,346,330 B2	1/2013	Lamego
7,801,581 B2	9/2010	Diab	8,353,842 B2	1/2013	Al-Ali et al.
7,822,452 B2	10/2010	Schurman et al.	8,355,766 B2	1/2013	MacNeish, III et al.
RE41,912 E	11/2010	Parker	8,359,080 B2	1/2013	Diab et al.
7,844,313 B2	11/2010	Kiani et al.	8,364,223 B2	1/2013	Al-Ali et al.
7,844,314 B2	11/2010	Al-Ali	8,364,226 B2	1/2013	Diab et al.
7,844,315 B2	11/2010	Al-Ali	8,374,665 B2	2/2013	Lamego
7,865,222 B2	1/2011	Weber et al.	8,385,995 B2	2/2013	Al-Ali et al.
7,873,497 B2	1/2011	Weber et al.	8,385,996 B2	2/2013	Smith et al.
7,880,606 B2	2/2011	Al-Ali	8,388,353 B2	3/2013	Kiani et al.
7,880,626 B2	2/2011	Al-Ali et al.	8,399,822 B2	3/2013	Al-Ali
7,891,355 B2	2/2011	Al-Ali et al.	8,401,602 B2	3/2013	Kiani
7,894,868 B2	2/2011	Al-Ali et al.	8,405,608 B2	3/2013	Al-Ali et al.
7,899,507 B2	3/2011	Al-Ali et al.	8,414,499 B2	4/2013	Al-Ali et al.
7,899,518 B2	3/2011	Trepagnier et al.	8,418,524 B2	4/2013	Al-Ali
7,904,132 B2	3/2011	Weber et al.	8,423,106 B2	4/2013	Lamego et al.
7,909,772 B2	3/2011	Popov et al.	8,428,967 B2	4/2013	Olsen et al.
7,910,875 B2	3/2011	Al-Ali	8,430,817 B1	4/2013	Al-Ali et al.
7,919,713 B2	4/2011	Al-Ali et al.	8,437,825 B2	5/2013	Dalvi et al.
7,937,128 B2	5/2011	Al-Ali	8,447,374 B2	5/2013	Diab
7,937,129 B2	5/2011	Mason et al.	8,455,290 B2	6/2013	Siskavich
7,937,130 B2	5/2011	Diab et al.	8,457,703 B2	6/2013	Al-Ali
7,941,199 B2	5/2011	Kiani	8,457,707 B2	6/2013	Kiani
7,951,086 B2	5/2011	Flaherty et al.	8,463,349 B2	6/2013	Diab et al.
7,957,780 B2	6/2011	Lamego et al.	8,466,286 B2	6/2013	Bellott et al.
7,962,188 B2	6/2011	Kiani et al.	8,471,713 B2	6/2013	Poeze et al.
7,962,190 B1	6/2011	Diab et al.	8,473,020 B2	6/2013	Kiani et al.
7,976,472 B2	7/2011	Kiani	8,483,787 B2	7/2013	Al-Ali et al.
7,988,637 B2	8/2011	Diab	8,489,364 B2	7/2013	Weber et al.
7,990,382 B2	8/2011	Kiani	8,498,684 B2	7/2013	Weber et al.
7,991,446 B2	8/2011	Al-Ali et al.	8,509,867 B2	8/2013	Workman et al.
8,000,761 B2	8/2011	Al-Ali	8,515,509 B2	8/2013	Bruinsma et al.
8,008,088 B2	8/2011	Bellott et al.	8,523,781 B2	9/2013	Al-Ali
RE42,753 E	9/2011	Kiani-Azarbayjany et al.	8,529,301 B2	9/2013	Al-Ali et al.
8,019,400 B2	9/2011	Diab et al.	8,532,727 B2	9/2013	Ali et al.
8,028,701 B2	10/2011	Al-Ali et al.	8,532,728 B2	9/2013	Diab et al.
8,029,765 B2	10/2011	Bellott et al.	D692,145 S	10/2013	Al-Ali et al.
8,036,728 B2	10/2011	Diab et al.	8,547,209 B2	10/2013	Kiani et al.
8,046,040 B2	10/2011	Ali et al.	8,548,548 B2	10/2013	Al-Ali
8,046,041 B2	10/2011	Diab et al.	8,548,550 B2	10/2013	Al-Ali et al.
			8,560,032 B2	10/2013	Al-Ali et al.
			8,560,034 B1	10/2013	Diab et al.
			8,570,167 B2	10/2013	Al-Ali
			8,570,503 B2	10/2013	Vo et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

8,571,618 B1	10/2013	Lamego et al.	8,948,834 B2	2/2015	Diab et al.
8,571,619 B2	10/2013	Al-Ali et al.	8,948,835 B2	2/2015	Diab
8,577,431 B2	11/2013	Lamego et al.	8,965,471 B2	2/2015	Lamego
8,584,345 B2	11/2013	Al-Ali et al.	8,983,564 B2	3/2015	Al-Ali
8,588,880 B2	11/2013	Abdul-Hafiz et al.	8,989,831 B2	3/2015	Al-Ali et al.
8,600,467 B2	12/2013	Al-Ali et al.	8,996,085 B2	3/2015	Kiani et al.
8,606,342 B2	12/2013	Diab	8,998,809 B2	4/2015	Kiani
8,626,255 B2	1/2014	Al-Ali et al.	9,028,429 B2	5/2015	Telfort et al.
8,630,691 B2	1/2014	Lamego et al.	9,037,207 B2	5/2015	Al-Ali et al.
8,634,889 B2	1/2014	Al-Ali et al.	9,060,721 B2	6/2015	Reichgott et al.
8,641,631 B2	2/2014	Sierra et al.	9,066,666 B2	6/2015	Kiani
8,652,060 B2	2/2014	Al-Ali	9,066,680 B1	6/2015	Al-Ali et al.
7,440,787 C1	3/2014	Diab	9,072,474 B2	7/2015	Al-Ali et al.
8,663,107 B2	3/2014	Kiani	9,078,560 B2	7/2015	Schurman et al.
8,666,468 B1	3/2014	Al-Ali	9,084,569 B2	7/2015	Weber et al.
8,667,967 B2	3/2014	Al-Ali et al.	9,095,316 B2	8/2015	Welch et al.
8,670,811 B2	3/2014	O'Reilly	9,106,038 B2	8/2015	Telfort et al.
8,670,814 B2	3/2014	Diab et al.	9,107,625 B2	8/2015	Telfort et al.
8,676,286 B2	3/2014	Weber et al.	9,107,626 B2	8/2015	Al-Ali et al.
8,682,407 B2	3/2014	Al-Ali	9,113,831 B2	8/2015	Al-Ali
RE44,823 E	4/2014	Parker	9,113,832 B2	8/2015	Al-Ali
RE44,875 E	4/2014	Kiani et al.	9,119,595 B2	9/2015	Lamego
8,690,799 B2	4/2014	Telfort et al.	9,131,881 B2	9/2015	Diab et al.
8,700,112 B2	4/2014	Kiani	9,131,882 B2	9/2015	Al-Ali et al.
8,702,627 B2	4/2014	Telfort et al.	9,131,883 B2	9/2015	Al-Ali
8,706,179 B2	4/2014	Parker	9,131,917 B2	9/2015	Telfort et al.
8,712,494 B1	4/2014	MacNeish, III et al.	9,138,180 B1	9/2015	Coverston et al.
8,715,206 B2	5/2014	Telfort et al.	9,138,182 B2	9/2015	Al-Ali et al.
8,718,735 B2	5/2014	Lamego et al.	9,138,192 B2	9/2015	Weber et al.
8,718,737 B2	5/2014	Diab et al.	9,142,117 B2	9/2015	Muhsin et al.
8,720,249 B2	5/2014	Al-Ali	9,153,112 B1	10/2015	Kiani et al.
8,721,541 B2	5/2014	Al-Ali et al.	9,153,121 B2	10/2015	Kiani et al.
8,721,542 B2	5/2014	Al-Ali et al.	9,161,696 B2	10/2015	Al-Ali et al.
8,723,677 B1	5/2014	Kiani	9,161,713 B2	10/2015	Al-Ali et al.
8,740,792 B1	6/2014	Kiani et al.	9,167,995 B2	10/2015	Lamego et al.
8,754,776 B2	6/2014	Poeze et al.	9,176,141 B2	11/2015	Al-Ali et al.
8,755,535 B2	6/2014	Telfort et al.	9,186,102 B2	11/2015	Bruinsma et al.
8,755,856 B2	6/2014	Diab et al.	2002/0082488 A1	6/2002	Al-Ali
8,755,872 B1	6/2014	Marinow	2002/0161291 A1	10/2002	Kiani
8,761,850 B2	6/2014	Lamego	2003/0000522 A1	1/2003	Lynn
8,764,671 B2	7/2014	Kiani	2003/0018241 A1	1/2003	Mannheimer
8,768,423 B2	7/2014	Shakespeare et al.	2003/0073890 A1	4/2003	Hanna
8,771,204 B2	7/2014	Telfort et al.	2003/0120164 A1	6/2003	Nielsen
8,777,634 B2	7/2014	Kiani et al.	2009/0247984 A1	10/2009	Lamego et al.
8,781,543 B2	7/2014	Diab et al.	2009/0275844 A1	11/2009	Al-Ali
8,781,544 B2	7/2014	Al-Ali et al.	2010/0004518 A1	1/2010	Vo et al.
8,781,549 B2	7/2014	Al-Ali et al.	2010/0030040 A1	2/2010	Poeze et al.
8,788,003 B2	7/2014	Schurman et al.	2011/0001605 A1	1/2011	Kiani et al.
8,790,268 B2	7/2014	Al-Ali	2011/0082711 A1	4/2011	Poeze et al.
8,801,613 B2	8/2014	Al-Ali et al.	2011/0105854 A1	5/2011	Kiani et al.
8,821,397 B2	9/2014	Al-Ali et al.	2011/0208015 A1	8/2011	Welch et al.
8,821,415 B2	9/2014	Al-Ali et al.	2011/0213212 A1	9/2011	Al-Ali
8,830,449 B1	9/2014	Lamego et al.	2011/0230733 A1	9/2011	Al-Ali
8,831,700 B2	9/2014	Schurman et al.	2011/0237911 A1	9/2011	Lamego et al.
8,840,549 B2	9/2014	Al-Ali et al.	2012/0059267 A1	3/2012	Lamego et al.
8,847,740 B2	9/2014	Kiani et al.	2012/0179006 A1	7/2012	Jansen et al.
8,849,365 B2	9/2014	Smith et al.	2012/0209082 A1	8/2012	Al-Ali
8,852,094 B2	10/2014	Al-Ali et al.	2012/0209084 A1	8/2012	Olsen et al.
8,852,994 B2	10/2014	Wojtczuk et al.	2012/0227739 A1	9/2012	Kiani
8,868,147 B2	10/2014	Stippick et al.	2012/0283524 A1	11/2012	Kiani et al.
8,868,150 B2	10/2014	Al-Ali et al.	2012/0296178 A1	11/2012	Lamego et al.
8,870,792 B2	10/2014	Al-Ali et al.	2012/0319816 A1	12/2012	Al-Ali
8,886,271 B2	11/2014	Kiani et al.	2012/0330112 A1	12/2012	Lamego et al.
8,888,539 B2	11/2014	Al-Ali et al.	2013/0023775 A1	1/2013	Lamego et al.
8,888,708 B2	11/2014	Diab et al.	2013/0041591 A1	2/2013	Lamego
8,892,180 B2	11/2014	Weber et al.	2013/0045685 A1	2/2013	Kiani
8,897,847 B2	11/2014	Al-Ali	2013/0046204 A1	2/2013	Lamego et al.
8,909,310 B2	12/2014	Lamego et al.	2013/0060147 A1	3/2013	Welch et al.
8,911,377 B2	12/2014	Al-Ali	2013/0096405 A1	4/2013	Garfio
8,912,909 B2	12/2014	Al-Ali et al.	2013/0096936 A1	4/2013	Sampath et al.
8,920,317 B2	12/2014	Al-Ali et al.	2013/0190581 A1	7/2013	Al-Ali et al.
8,921,699 B2	12/2014	Al-Ali et al.	2013/0197328 A1	8/2013	Diab et al.
8,922,382 B2	12/2014	Al-Ali et al.	2013/0211214 A1	8/2013	Olsen
8,929,964 B2	1/2015	Al-Ali et al.	2013/0243021 A1	9/2013	Siskavich
8,942,777 B2	1/2015	Diab et al.	2013/0253334 A1	9/2013	Al-Ali et al.
			2013/0296672 A1	11/2013	O'Neil et al.
			2013/0317370 A1	11/2013	Dalvi et al.
			2013/0324808 A1	12/2013	Al-Ali et al.
			2013/0331670 A1	12/2013	Kiani

(56)

References Cited

U.S. PATENT DOCUMENTS

2013/0338461	A1	12/2013	Lamego et al.
2014/0034353	A1	12/2013	Al-Ali et al.
2014/0012100	A1	1/2014	Al-Ali et al.
2014/0051953	A1	2/2014	Lamego et al.
2014/0058230	A1	2/2014	Abdul-Hafiz et al.
2014/0066783	A1	3/2014	Kiani et al.
2014/0077956	A1	3/2014	Sampath et al.
2014/0081100	A1	3/2014	Muhsin et al.
2014/0081175	A1	3/2014	Telfort
2014/0094667	A1	4/2014	Schurman et al.
2014/0100434	A1	4/2014	Diab et al.
2014/0114199	A1	4/2014	Lamego et al.
2014/0120564	A1	5/2014	Workman et al.
2014/0121482	A1	5/2014	Merritt et al.
2014/0121483	A1	5/2014	Kiani
2014/0127137	A1	5/2014	Bellott et al.
2014/0129702	A1	5/2014	Lamego et al.
2014/0135588	A1	5/2014	Al-Ali et al.
2014/0142401	A1	5/2014	Al-Ali et al.
2014/0163344	A1	6/2014	Al-Ali
2014/0163402	A1	6/2014	Lamego et al.
2014/0166076	A1	6/2014	Kiani et al.
2014/0171763	A1	6/2014	Diab
2014/0180038	A1	6/2014	Kiani
2014/0180154	A1	6/2014	Sierra et al.
2014/0194709	A1	7/2014	Al-Ali et al.
2014/0194711	A1	7/2014	Al-Ali
2014/0194766	A1	7/2014	Al-Ali et al.
2014/0206963	A1	7/2014	Al-Ali
2014/0213864	A1	7/2014	Abdul-Hafiz et al.
2014/0243627	A1	8/2014	Diab et al.
2014/0266790	A1	9/2014	Al-Ali et al.
2014/0275808	A1	9/2014	Poeze et al.
2014/0275835	A1	9/2014	Lamego et al.
2014/0275871	A1	9/2014	Lamego et al.
2014/0275872	A1	9/2014	Merritt et al.
2014/0275881	A1	9/2014	Lamego et al.
2014/0288400	A1	9/2014	Diab et al.
2014/0303520	A1	10/2014	Telfort et al.
2014/0316228	A1	10/2014	Blank et al.
2014/0323825	A1	10/2014	Al-Ali et al.
2014/0330092	A1	11/2014	Al-Ali et al.
2014/0330098	A1	11/2014	Merritt et al.
2014/0330099	A1	11/2014	Al-Ali et al.
2014/0333440	A1	11/2014	Kiani
2014/0336481	A1	11/2014	Shakespeare et al.
2014/0343436	A1	11/2014	Kiani
2015/0018650	A1	1/2015	Al-Ali et al.

FOREIGN PATENT DOCUMENTS

EP	0352923	1/1990
EP	0645117	3/1995
EP	0659384	6/1995
WO	WO 84/03032	8/1984
WO	WO 92/11803	7/1992
WO	WO 92/15955	9/1992
WO	WO 92/20273	11/1992
WO	WO 95/21567	8/1995
WO	WO 98/43071	10/1998

OTHER PUBLICATIONS

Edward Bedrosian, *The Analytic Signal Representation of Modulating Waveforms* (1962).

Boualem Boashash, *Note on the Use of the Wigner Distribution for Time-Frequency Signal Analysis*, IEEE on Acoustics, Speech and Signal Processing, vol. 36, No. 9 (Sep. 1988).

Boualem Boashash, *Estimating and Interpreting the Instantaneous Frequency of a Signal—Part 1: Fundamentals*, Proceedings of the IEEE, vol. 80, No. 4 (Apr. 1992).

Wukitsch, M.W., BA, et al. Pulse Oximetry: Analysis of Theory, Technology, and Practice, Journal of Clinical Monitoring, vol. 4, (1988), pp. 290-301.

U.S. Appl. No. 90/012,403, filed Jul. 23, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,263,222, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,409, filed Aug. 17, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,699,194, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,463, filed Sep. 5, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,215,984, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,532, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,499,835, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,534, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,962,188, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,538, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,377,899, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,541, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,899,507, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,542, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 8,180,420, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,543, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,850,787, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,546, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,438,683, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,548, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,880,606, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,553, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,024,233, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,555, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,440,787, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,557, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 8,150,487, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,559, filed Sep. 13, 2012, requesting ex parte reexamination of U.S. Pat. No. 8,190,223, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,561, filed Sep. 14, 2012, requesting ex parte reexamination of U.S. Pat. No. 8,019,400, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,562, filed Sep. 14, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,463,311, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,566, filed Sep. 14, 2012, requesting ex parte reexamination of U.S. Pat. No. 7,530,955, including accompanying

(56)

References Cited

OTHER PUBLICATIONS

Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,567, filed Sep. 14, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,684,090, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,568, filed Sep. 14, 2012, requesting ex parte reexamination of U.S. Pat. No. 8,128,572, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 90/012,699, filed Oct. 4, 2012, requesting ex parte reexamination of U.S. Pat. No. 6,002,952, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.510 and 35 U.S.C. § 302.

U.S. Appl. No. 95/002,183, filed Sep. 12, 2012, requesting inter partes reexamination of U.S. Pat. No. 7,530,955, including accompanying Reexam Request, claim charts, and other documentation filed under 37 C.F.R. § 1.913 and 35 U.S.C. § 311.

Blitt, Casey D., *Monitoring in Anesthesia and Critical Care Medicine*, (2d ed. 1990).

Business Wire, "Mallinckrodt Announces the Nellcor N-395 Pulse Oximeter With Oxismart XL and SatSeconds," Oct. 7, 1999.

Hanzo et al., "A Portable Multimedia Communicator Scheme", *Multimedia Technologies and Future Applications: Proceedings of the IEEE International Symposium* (1994).

Maciej Niedzwiecki et al. "Smoothing of Discontinuous Signals: The Competitive Approach," *IEEE Transactions on Signal Processing*, vol. 43, No. 1, Jan. 1995, pp. 1-13.

Steven W. Smith, *The Scientist and Engineer's Guide to Digital Signal Processing*, § 8 (1st ed. 1997).

Declaration of Perry D. Oldham in Support of Masimo Opposition to Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 7,215,984, vol. 1, Doc. 556, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Declaration of Perry D. Oldham in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 7,215,984, vol. 2, Doc. 558, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Masimo Corporation's Answering Brief in Opposition to Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 7,215,984, Doc. 555, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Philip's Opening Brief in Support of Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 7,215,984, Doc. 442, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 21, 2012. (Redacted).

Philip Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 7,215,984, Doc. 394, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 14, 2012.

Reply Brief in Support of Defendants' Motion for Summary Judgment of invalidity and Noninfringement of U.S. Pat. No. 7,216,984, Doc. 609, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 26, 2012. (Redacted).

Declaration of Gail Baura, Ph.D. in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 7,215,984, Doc. 561, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Declaration of Gail Baura, Ph.D. in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 5,632,272, Doc. 554, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Declaration of Perry D. Oldham in Support of Masimo Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 5,632,272, Doc. 553, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Masimo Corporation's Answering Brief in Opposition to Defendant's Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 5,632,272, Doc. 552, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Opening Brief in Support of Defendants' Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 5,632,272, Doc. 444, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 21, 2012. (Redacted).

Defendants' Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 5,632,272, Doc. 402, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 14, 2012.

Reply Brief in Support of Defendants' Motion for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. No. 5,632,272, Doc. 614, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 26, 2012 (Redacted).

Declaration of Mohammed K. Diab in Support of Masimo's Oppositions to Defendants' Motions for Summary Judgment of Invalidity and Noninfringement of U.S. Pat. Nos. 5,632,272 and 7,215,984, Doc. 563, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012 (Redacted).

Declaration of Perry D. Oldham in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 550, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012 (Redacted).

Masimo Corporation's Answering Brief in Opposition to Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 549, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012 (Redacted).

Philip's Opening Brief in Support of Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 413, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 14, 2012.

Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 410, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 14, 2012.

(56)

References Cited

OTHER PUBLICATIONS

Reply Brief in Support of Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 613, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 26, 2012 (Redacted).

Declaration of Gail Baura, Ph.D. in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,263,222, Doc. 551, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

V. Ya. Volkov, "Enhancing the Reliability and Accuracy of Pulse Oximetry with a Built-In Expert System," *Biomedical Engineering*, vol. 27, No. 3 (May-Jun. 1993) (translated from Russian).

Declaration of Gail Baura, Ph.D. in Support of Masimo's Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,699,194, Doc. 508, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 21, 2012.

Opening Brief in Support of Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,699,194, Doc. 445, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 21, 2012. (Redacted).

Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,699,194, Doc. 406, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Aug. 14, 2012.

Reply Brief in Support of Defendants' Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,699,194, Doc. 610, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 26, 2012. (Redacted).

Declaration of Perry D. Oldham in Support of Masimo Opposition to Defendant's Motion for Summary Judgment of Invalidity of U.S. Pat. No. 6,699,194, Doc. 548, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Sep. 28, 2012. (Redacted).

Scharf, "Optimization of Portable Pulse Oximetry Through Fourier Analysis".

Scharf, "Pulse Oximetry Through Spectral Analysis".

Rusch, "Master's Thesis," Graduate School University of South Florida, Tampa, Florida (Dec. 1994).

Philips' Response to Masimo Corporation's Objections to the Report and Recommendation Regarding Claim Construction, Doc. 230, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 24, 2011.

Masimo Corporation's Objections to the Report and Recommendation Regarding Claim Construction, Doc. 219, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 8, 2011.

Defendants' Objections to Magistrate Judge Thyne's Report and Recommendation Regarding Claim Construction, Doc. 218, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 7, 2011. Report and Recommendation Regarding Claim Construction, Doc. 210, *Masimo Corporation v. Philips Electronics North America*

Corporation and Philips Medizin Systeme Bötblingen GMBH, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Feb. 18, 2011.

Memorandum Order Adopting Report and Recommendation Regarding Claim Construction, Doc. 319, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Jan. 17, 2011.

Masimo Corporation's Response to Defendants' Objections to the Report and Recommendation Regarding Claim Construction, Doc. 232, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 24, 2011.

V. Ya. Volkov, "Principles and Algorithms for Determining Blood Oxygenation Level by Pulse Oximetry," *Biomedical Engineering*, vol. 27, No. 1 (Jan.-Feb. 1993) (translated from Russian).

Supplemental Expert Report of Dr. Robert Stone Regarding the invalidity of Masimo's Patents-in-Suit (U.S. Pat. No. 5,632,272, U.S. Pat. No. 6,263,222, U.S. Pat. No. 7,215,984, and U.S. Pat. No. 6,699,194, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 18, 2012.

Appendix for Expert Report of Dr. Robert Stone Regarding the invalidity of Masimo's Patents-in-Suit (U.S. Pat. No. 5,632,272, U.S. Pat. No. 6,263,222, U.S. Pat. No. 7,215,984, and U.S. Pat. No. 6,699,194, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 7, 2012.

Expert Report of Dr. Robert Stone Regarding the invalidity of Masimo's Patents-in-Suit (U.S. Pat. No. 5,632,272, U.S. Pat. No. 6,263,222, U.S. Pat. No. 7,215,984, and U.S. Pat. No. 6,699,194, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 7, 2012.

Revised Expert Report of Dr. Robert Stone Regarding the invalidity of Masimo's Patents-in-Suit (U.S. Pat. No. 5,632,272, U.S. Pat. No. 6,263,222, U.S. Pat. No. 7,215,984, and U.S. Pat. No. 6,699,194, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Mar. 7, 2012.

Wukitsch, et al., "Knowing Your Monitoring Equipment," *Journal of Clinical Monitoring*, vol. 4, No. 4 (Oct. 1998).

Second Amended Complaint for Patent Infringement, Doc. 42, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:11-cv-00742 (LPS/MPT) dated Apr. 25, 2012.


Masimo's Answer to Philips' Counterclaims, Doc. 28, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:11-cv-00742 (LPS/MPT) dated Dec. 30, 2011.

Defendants' Answer and Philips Electronics North America Corp.'s Counterclaims to Masimo's First Amended Complaint, Doc. 11, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:11-cv-00742 (LPS/MPT) dated Nov. 7, 2011.

Masimo's Answer to Philips' Counterclaims to Masimo's Second Amended Complaint, Doc. 358, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:11-cv-00742 (LPS/MPT) dated Jun. 4, 2012.

Defendants' Answer and Philips Electronics North America Corp.'s Counterclaims to Masimo's Second Amended Complaint, Doc. 43, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Bötblingen GMBH*, (District of Delaware, Case No. 1:11-cv-00742 (LPS/MPT) dated May 11, 2012.

* cited by examiner

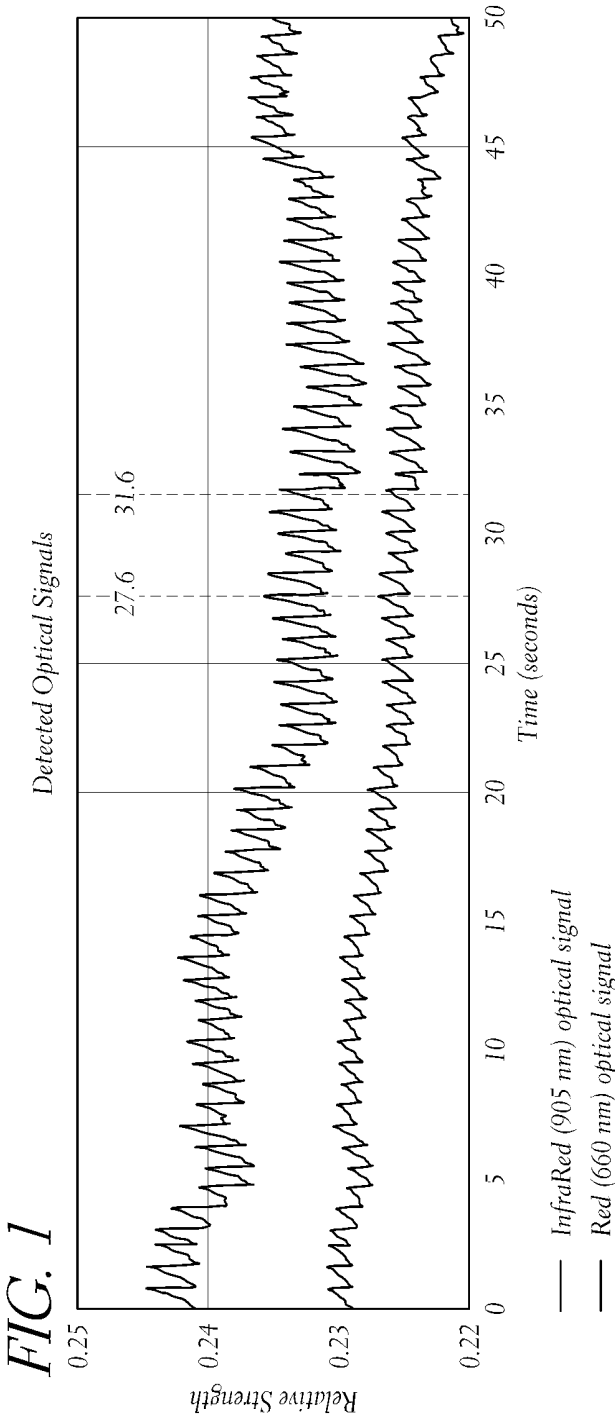




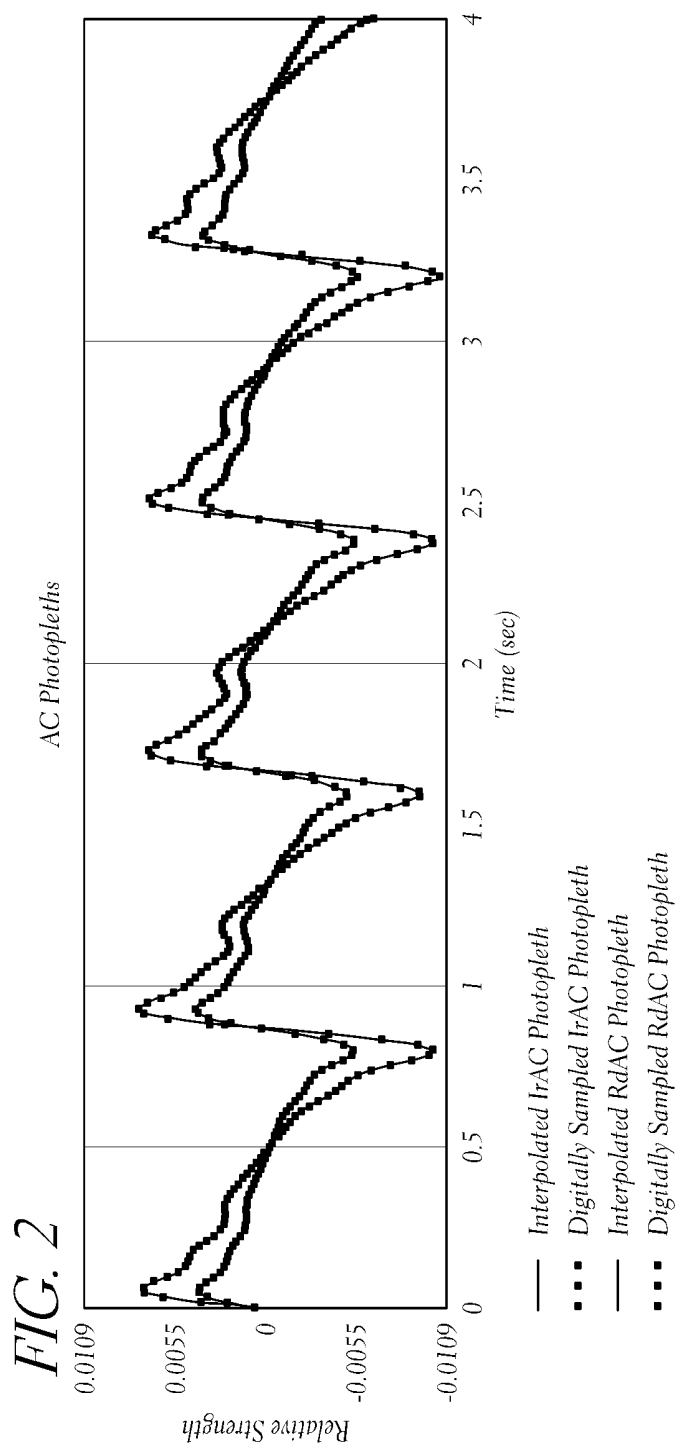


FIG. 3

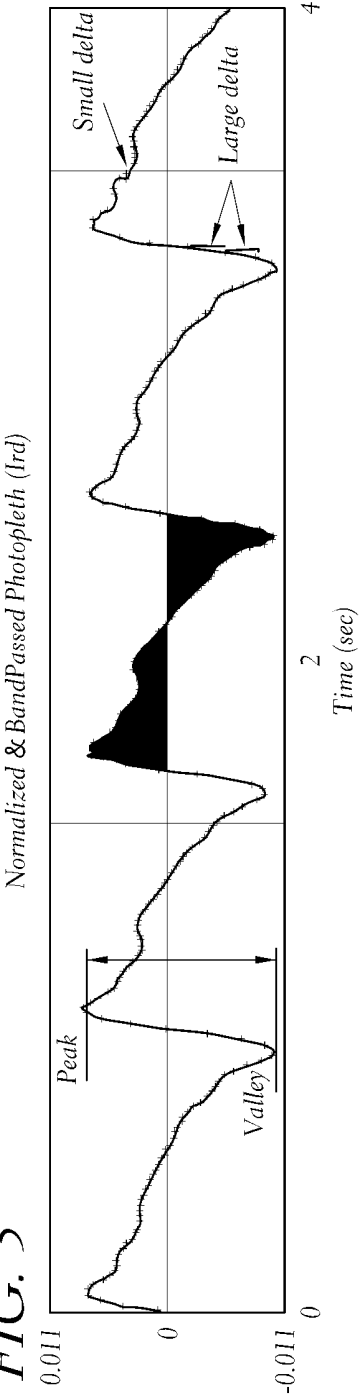

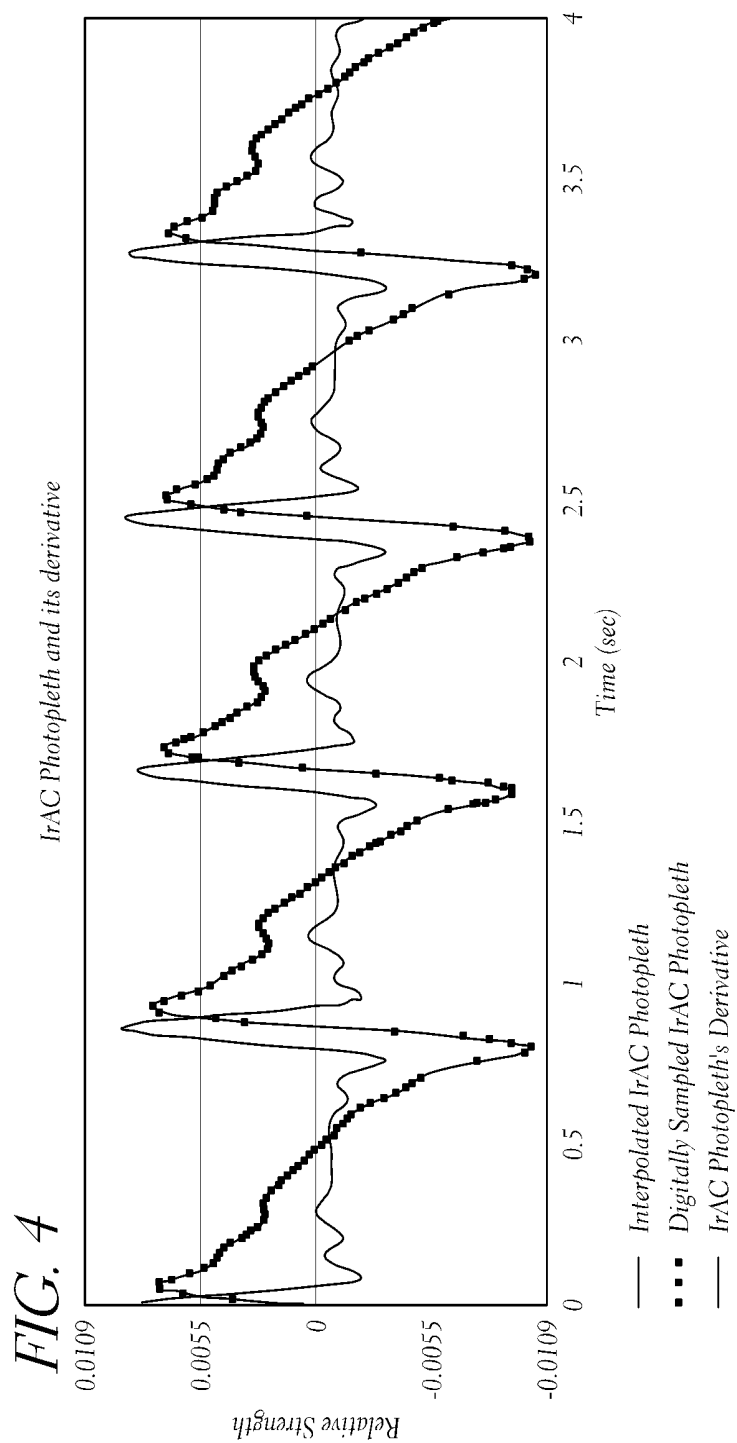

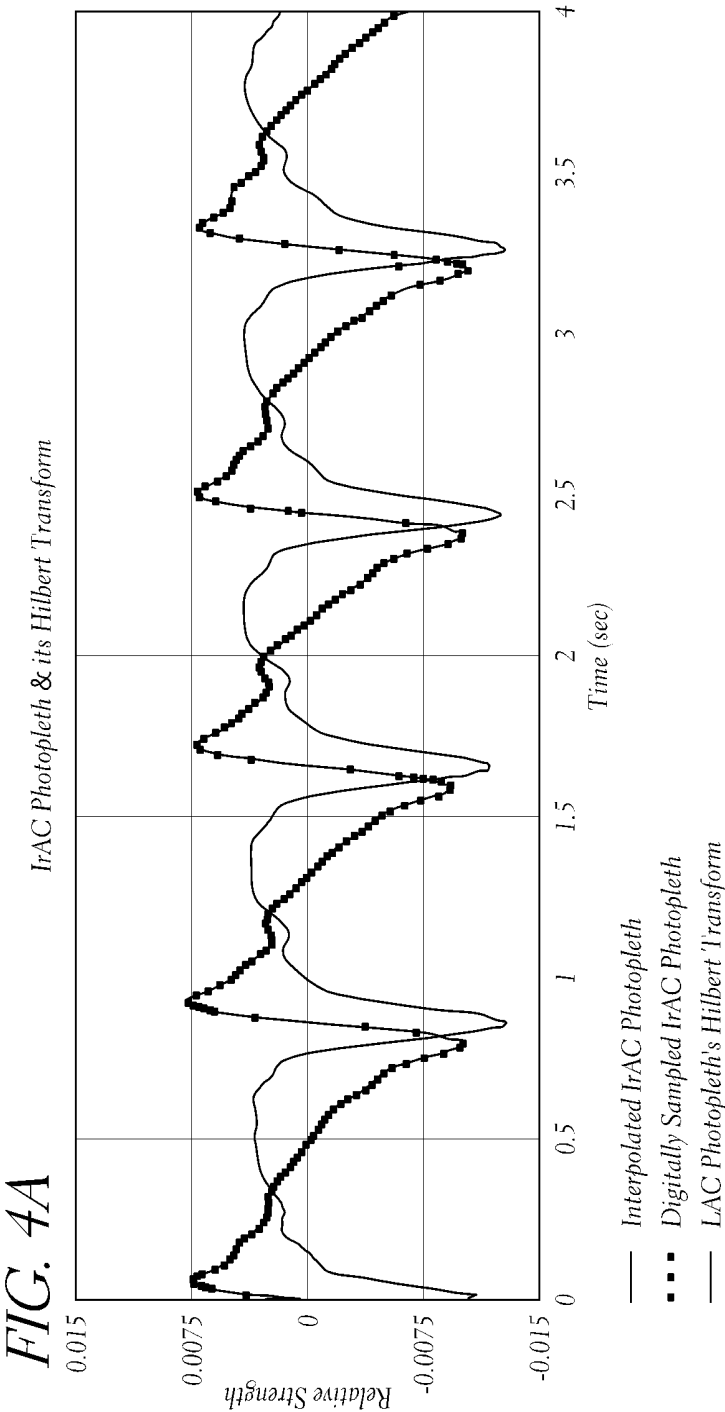

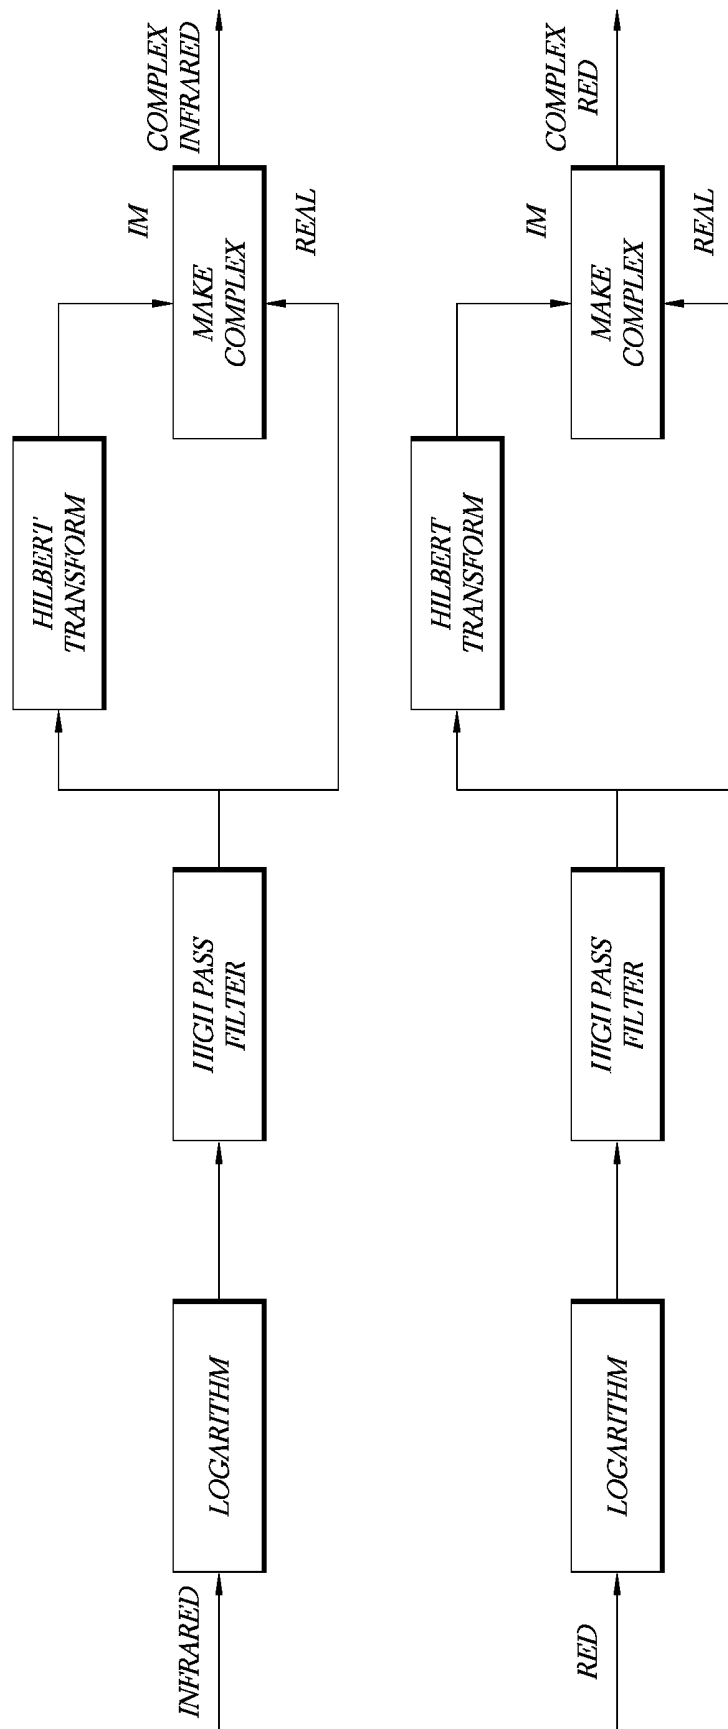


FIG. 5


FIG. 5A

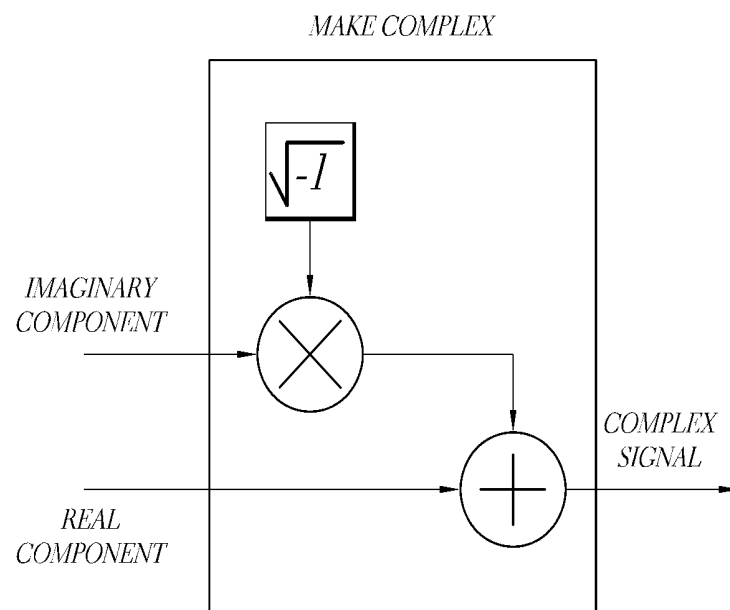FIG. 6


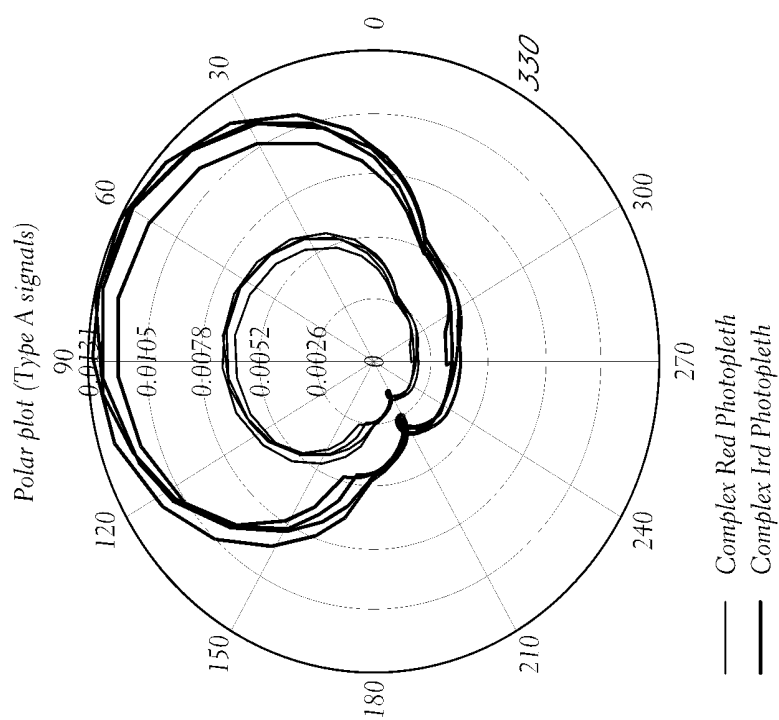


FIG. 7

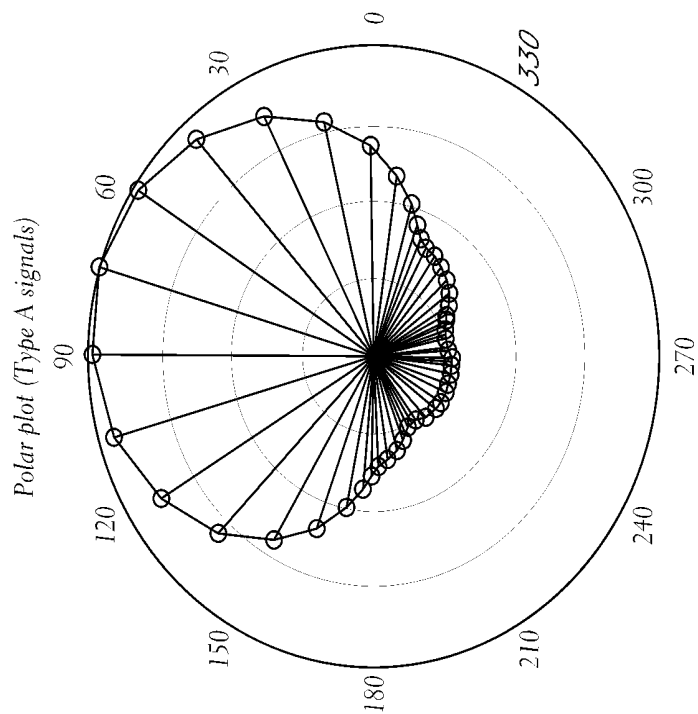

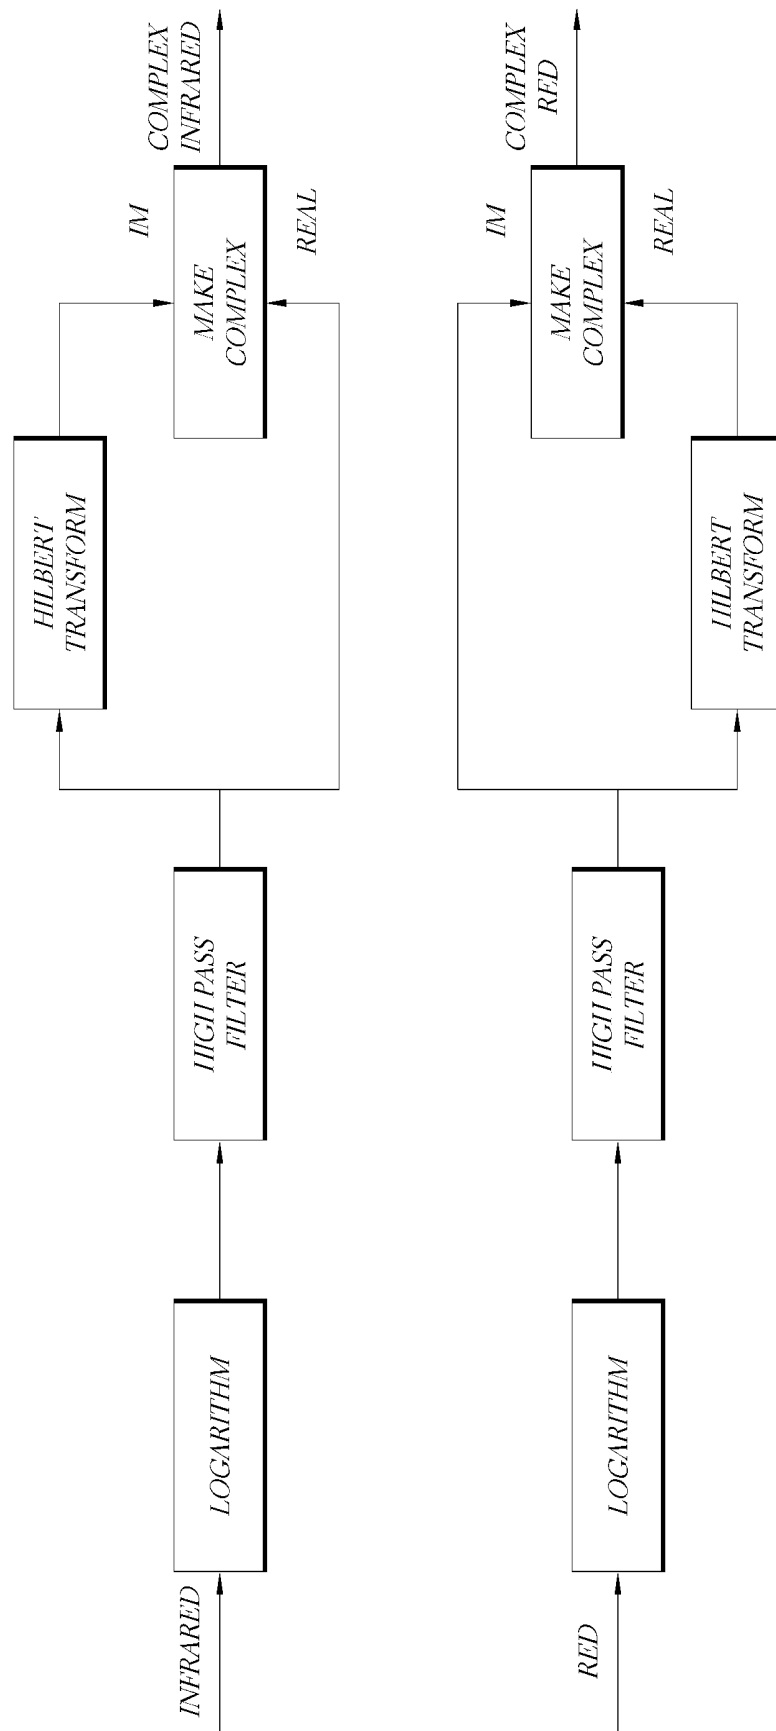


FIG. 8

FIG. 9

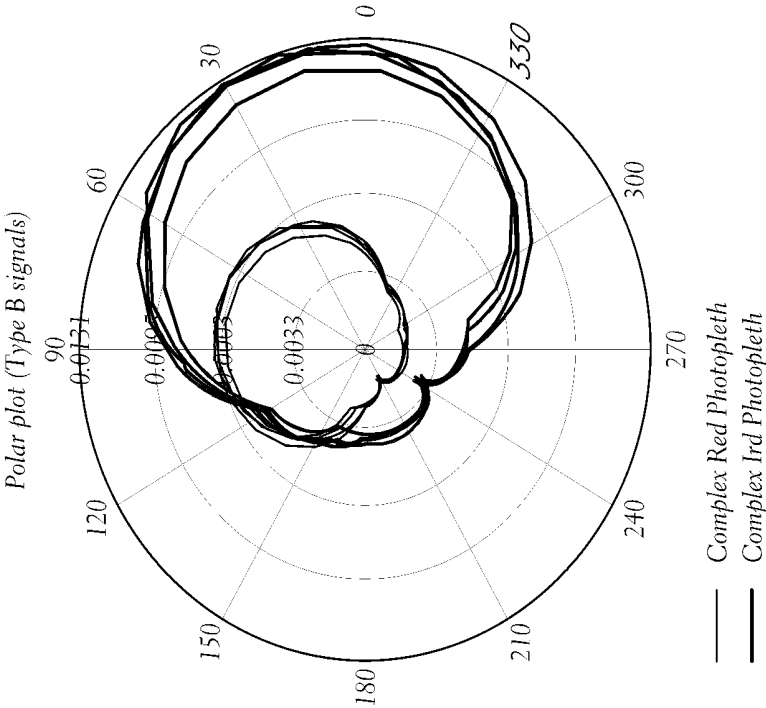


FIG. 10

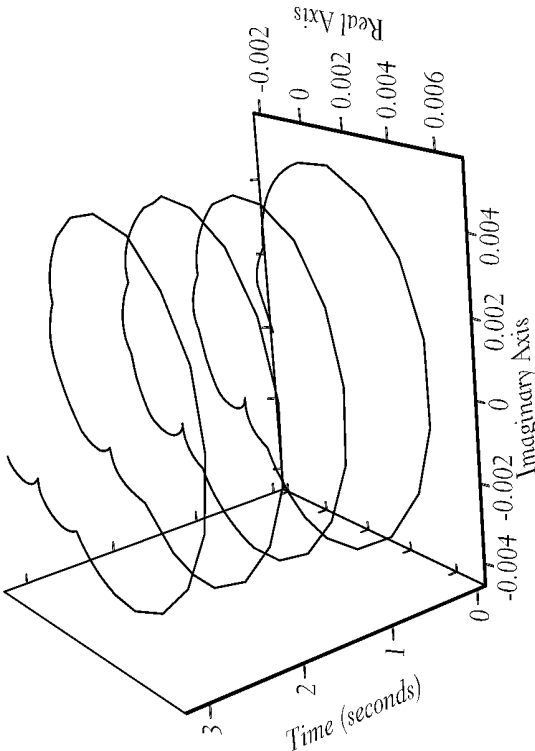


FIG. 11

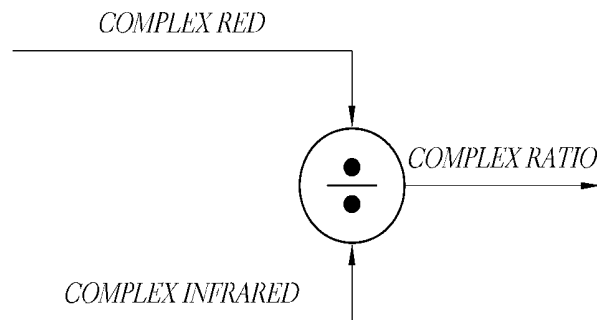


FIG. 12

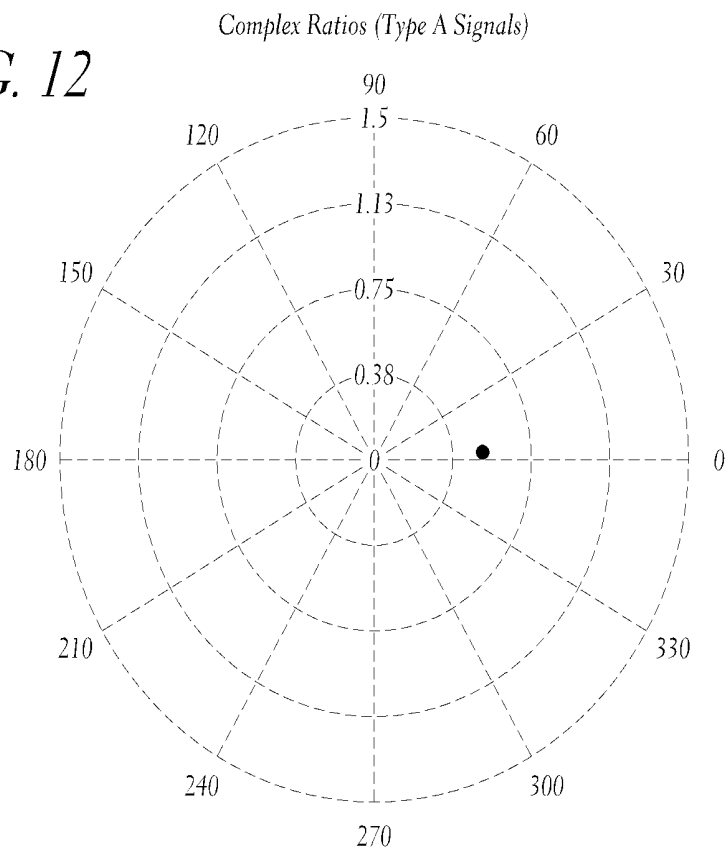
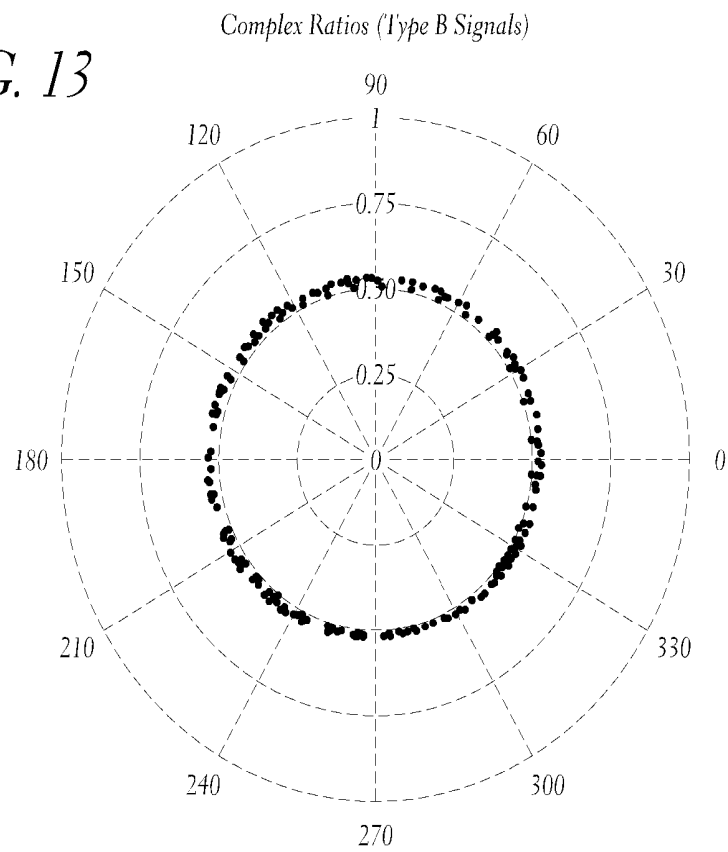
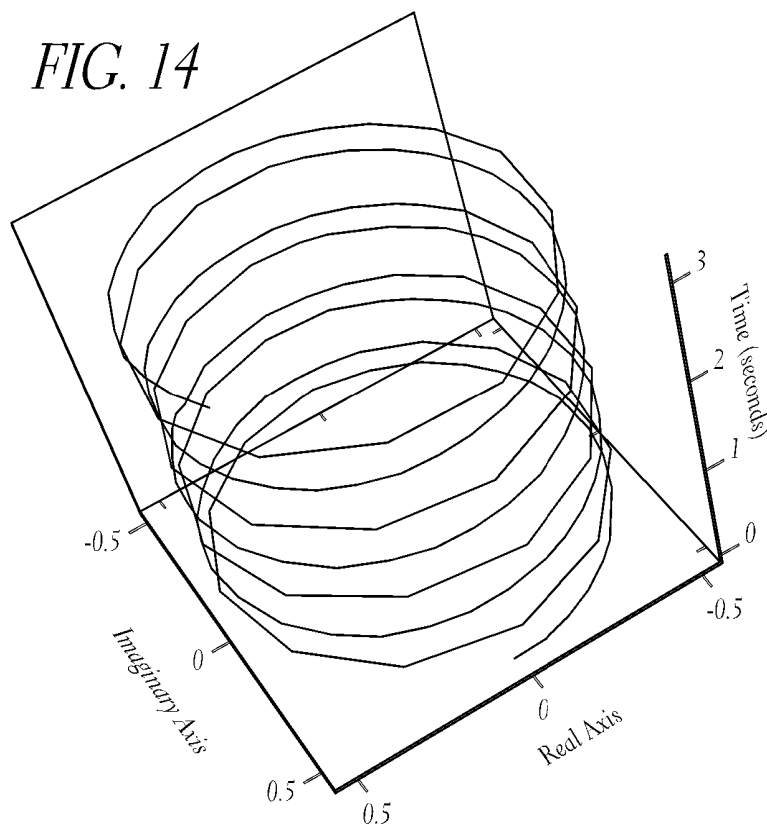


FIG. 13*FIG. 14*

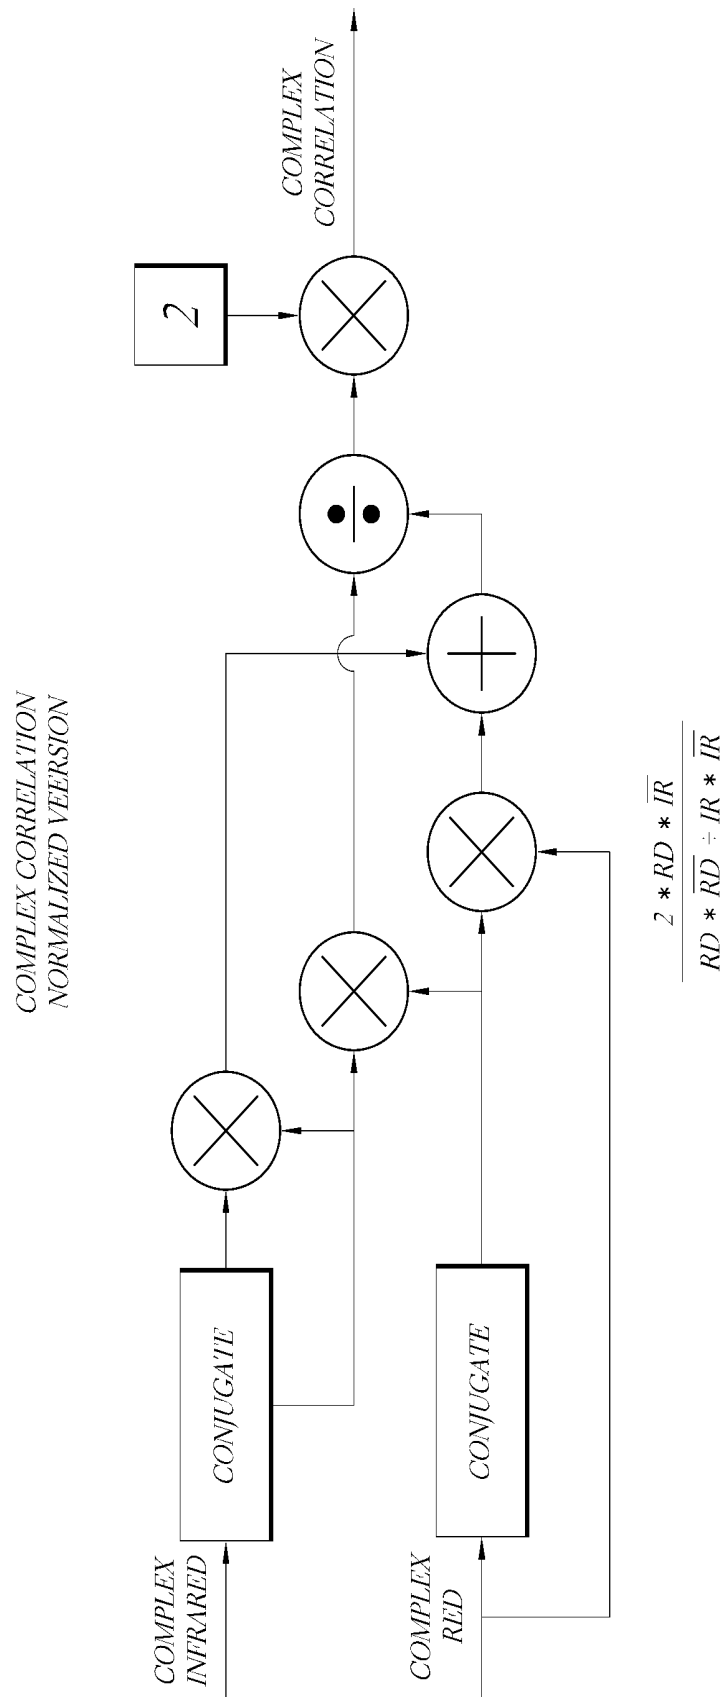


FIG. 15

FIG. 16

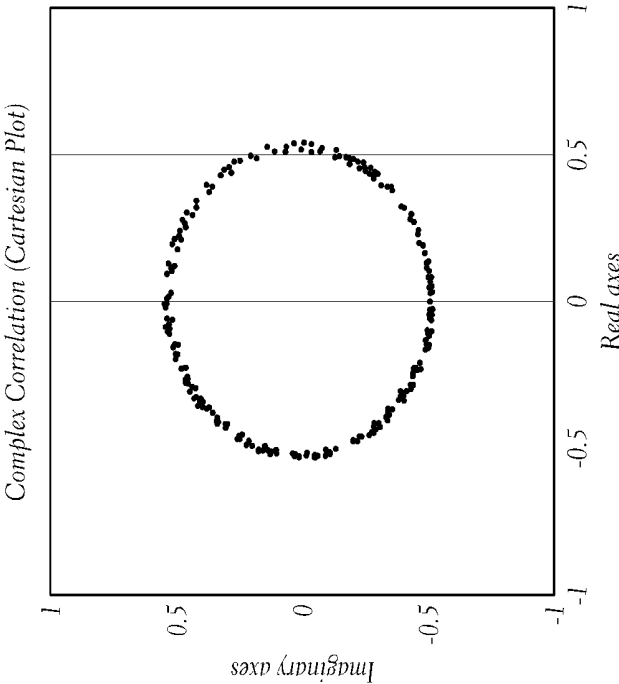


FIG. 17



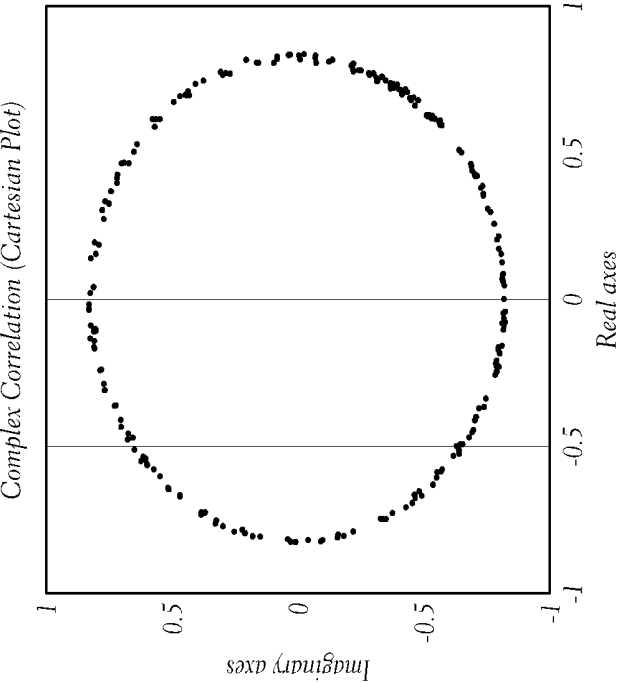


FIG. 18

Correlation vs. Ratio

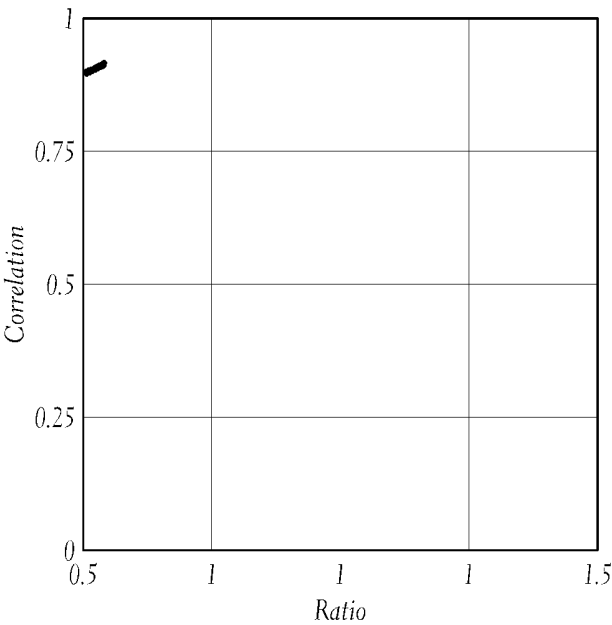

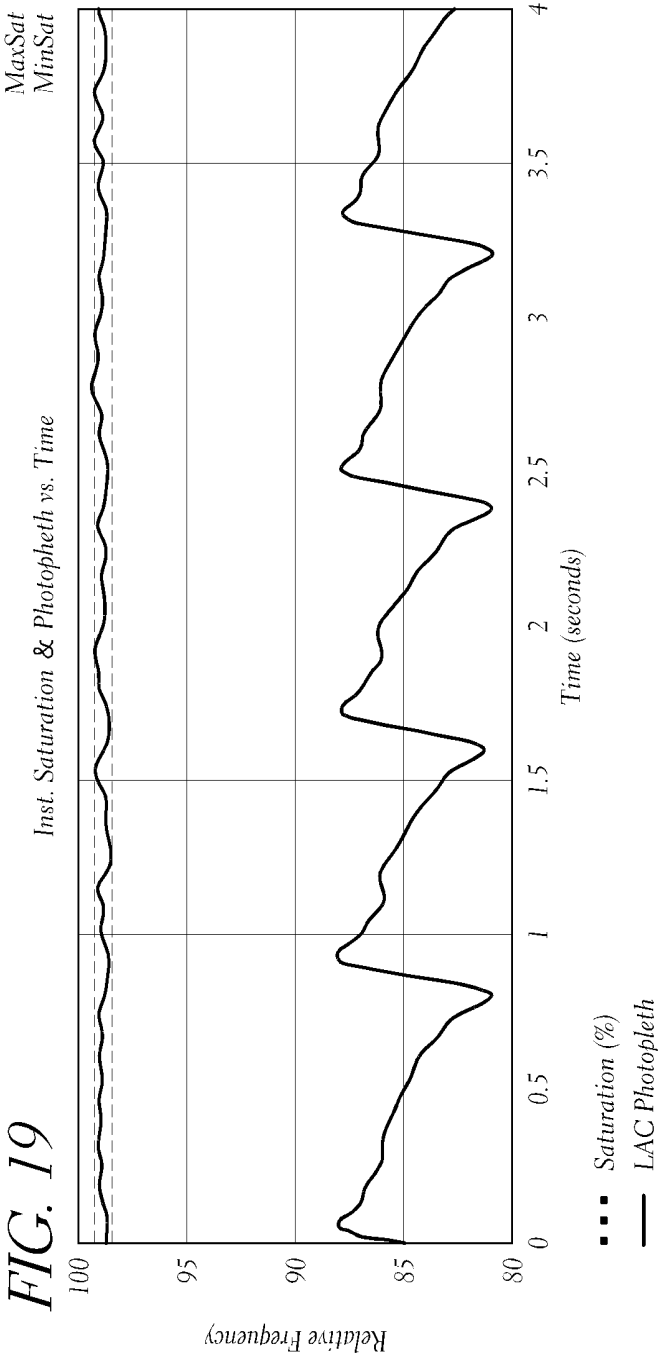



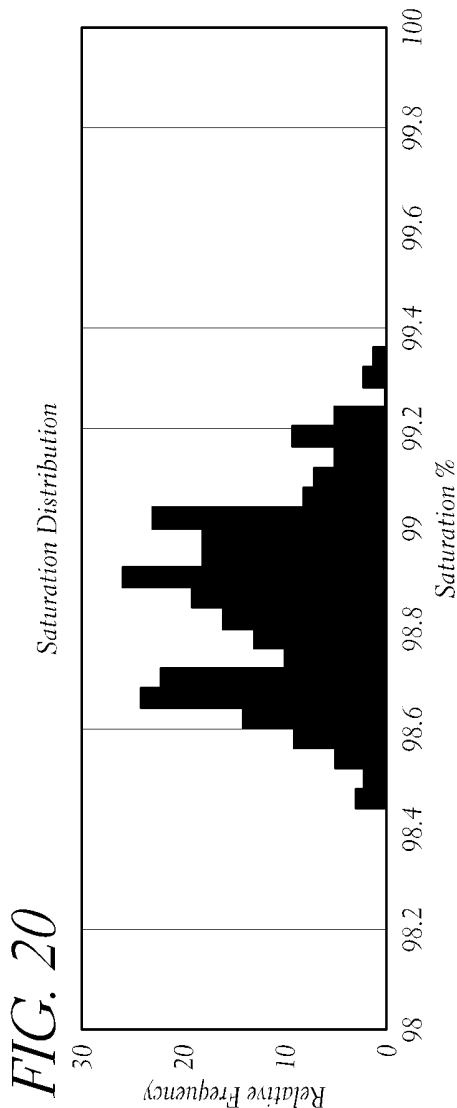
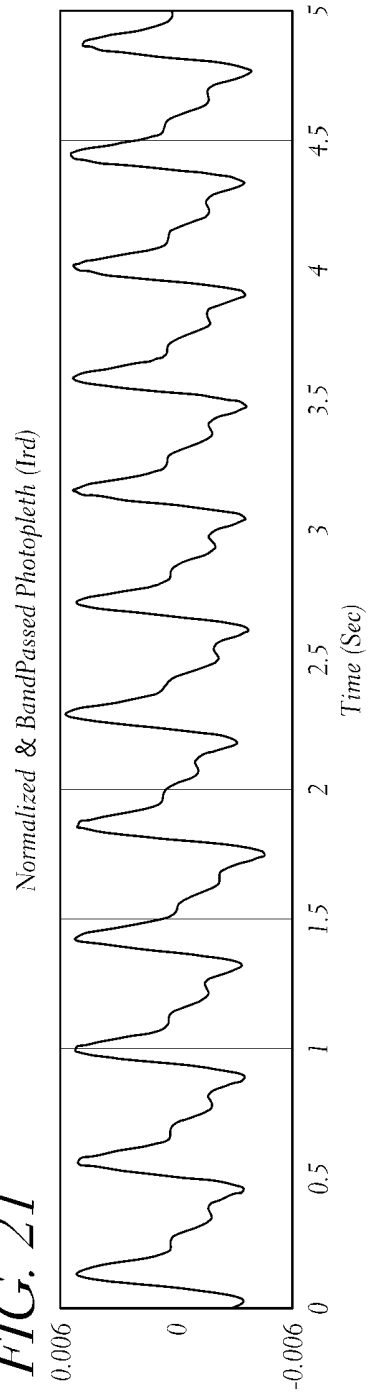
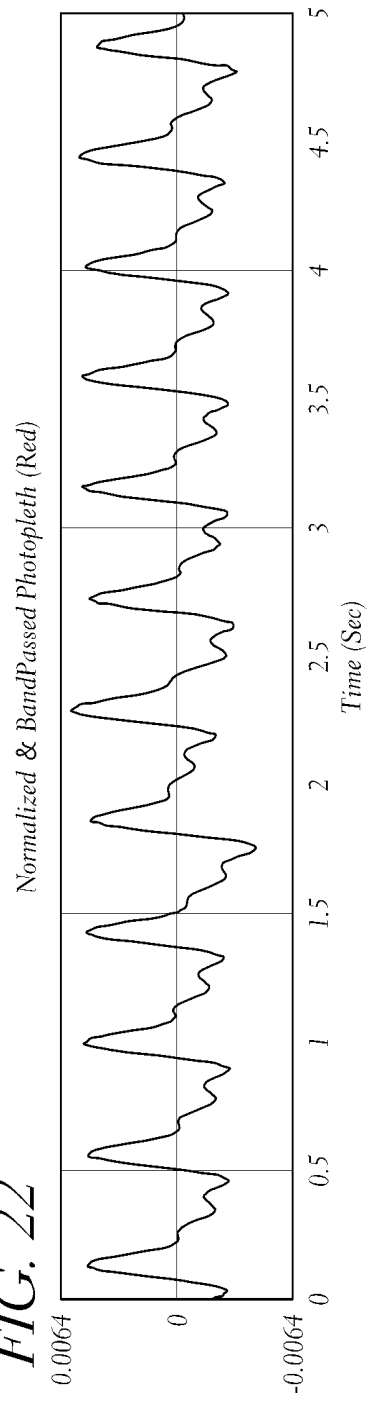


FIG. 21**FIG. 22**

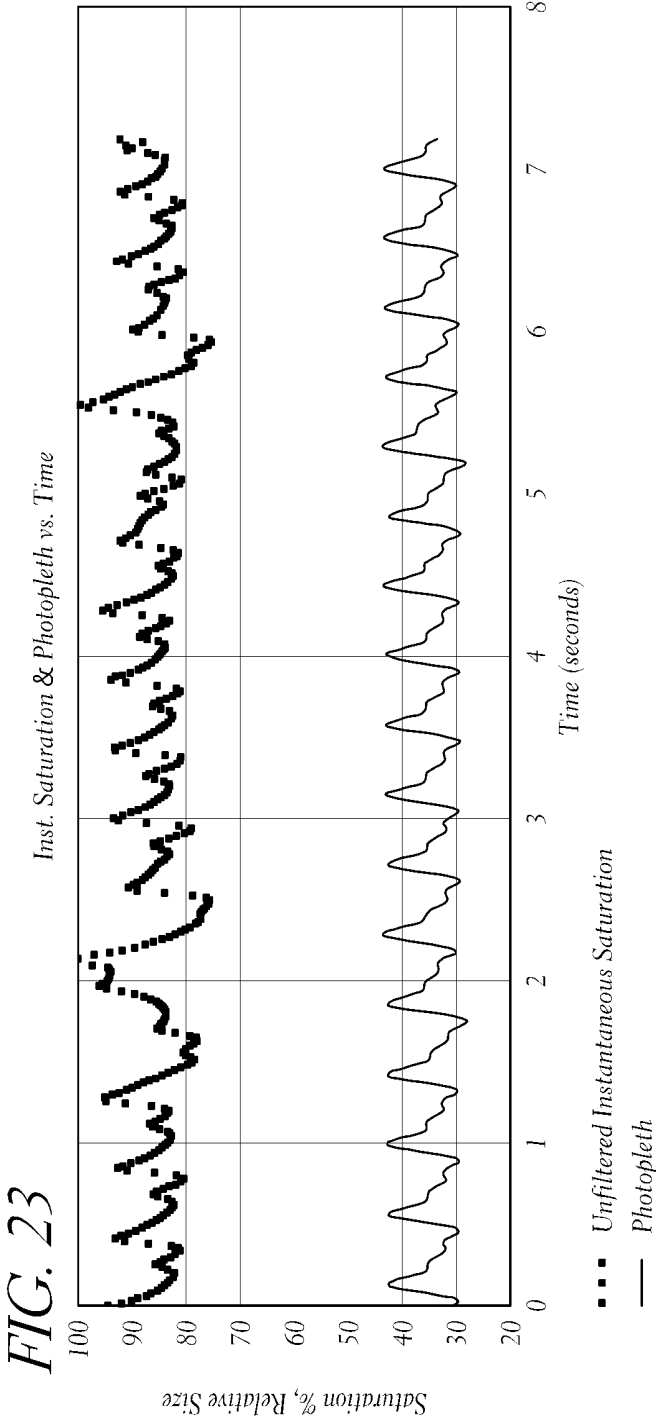

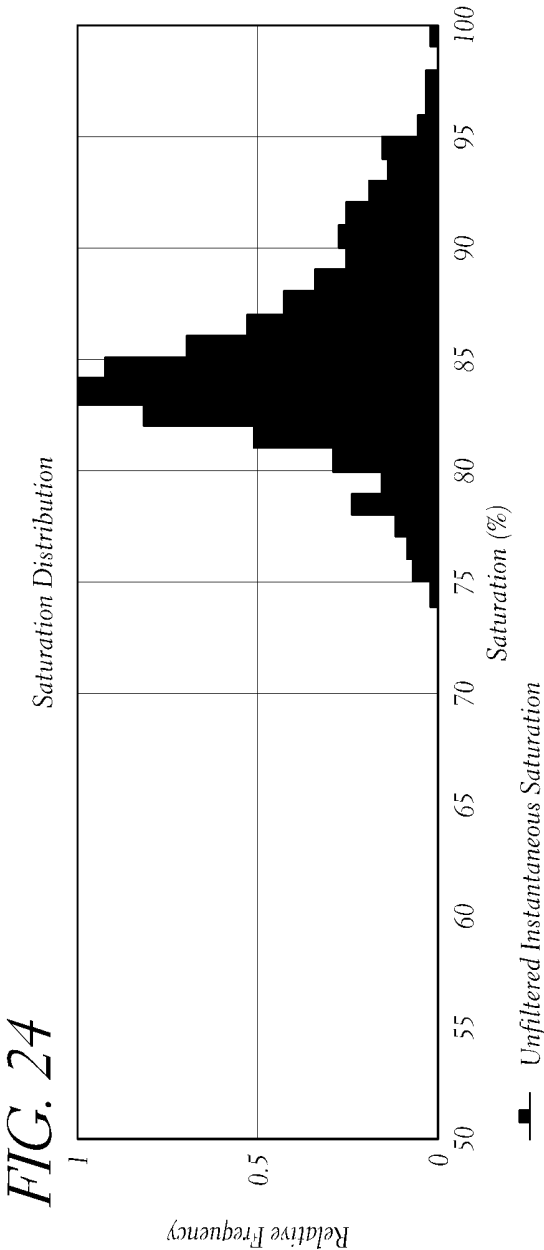

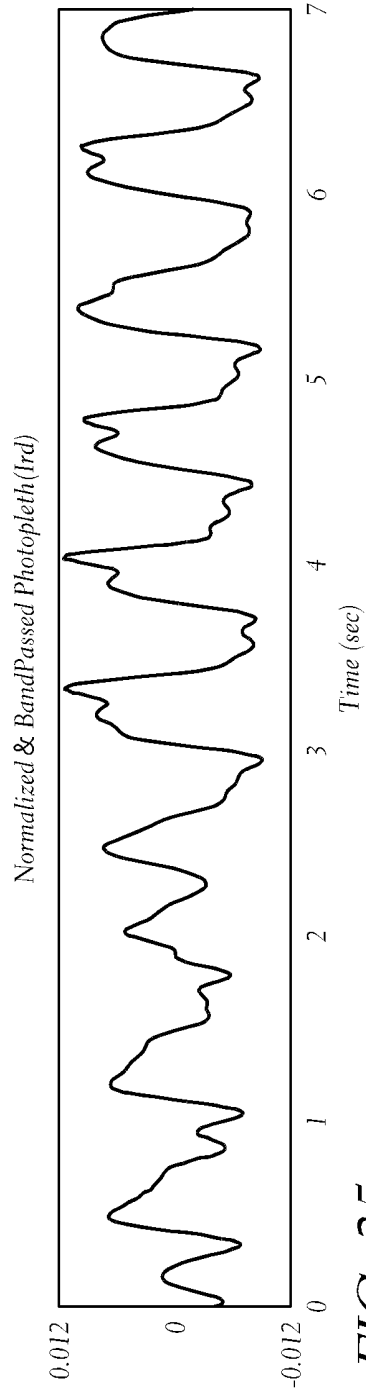


FIG. 25

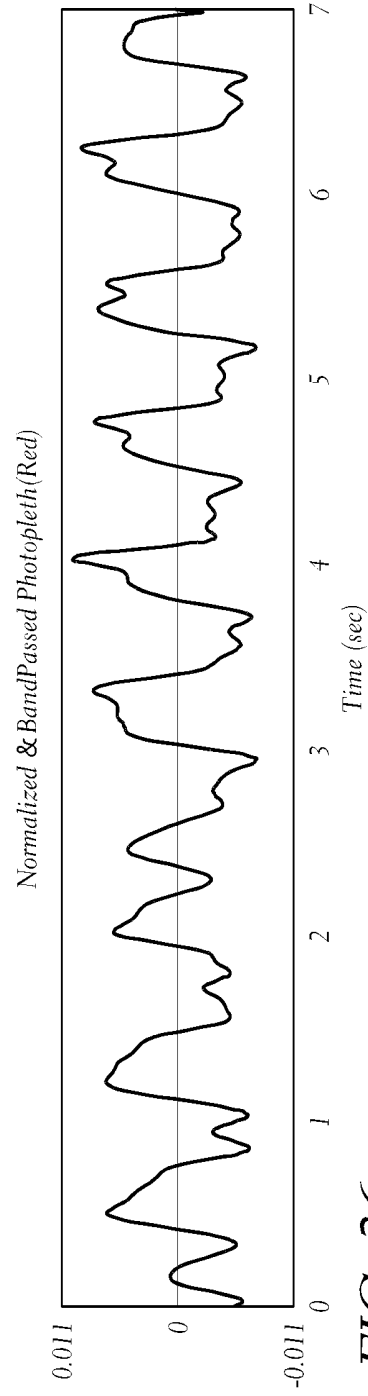


FIG. 26

FIG. 27





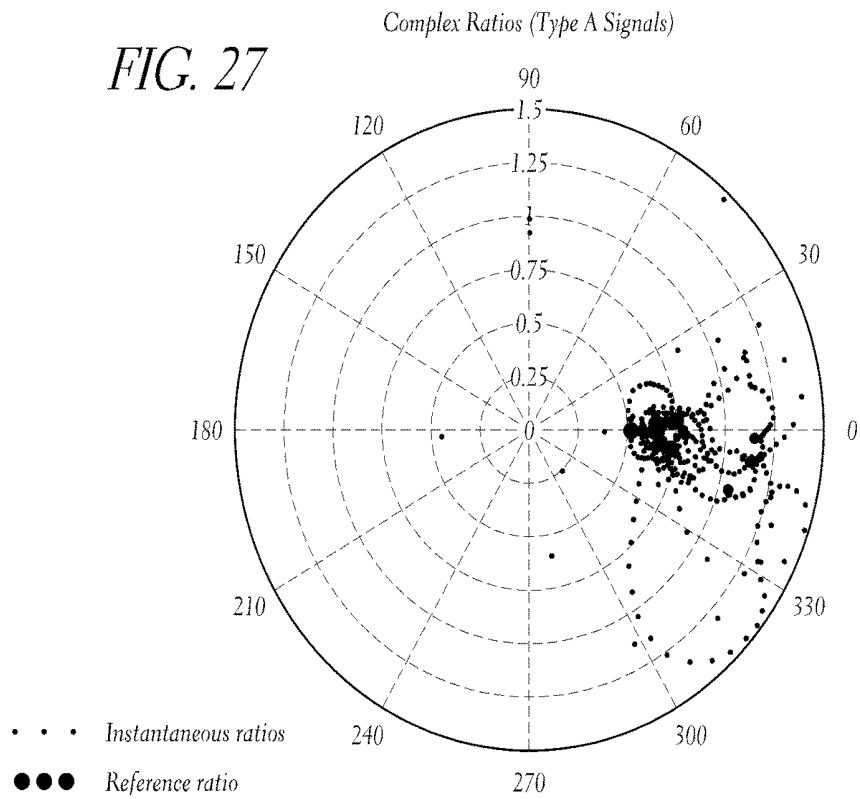



FIG. 28

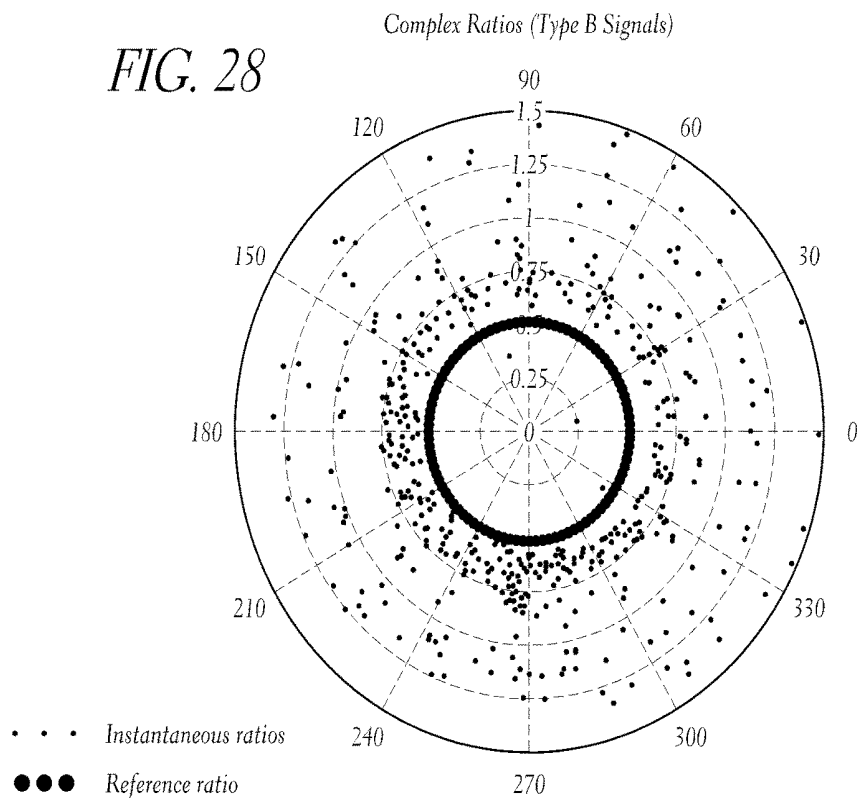


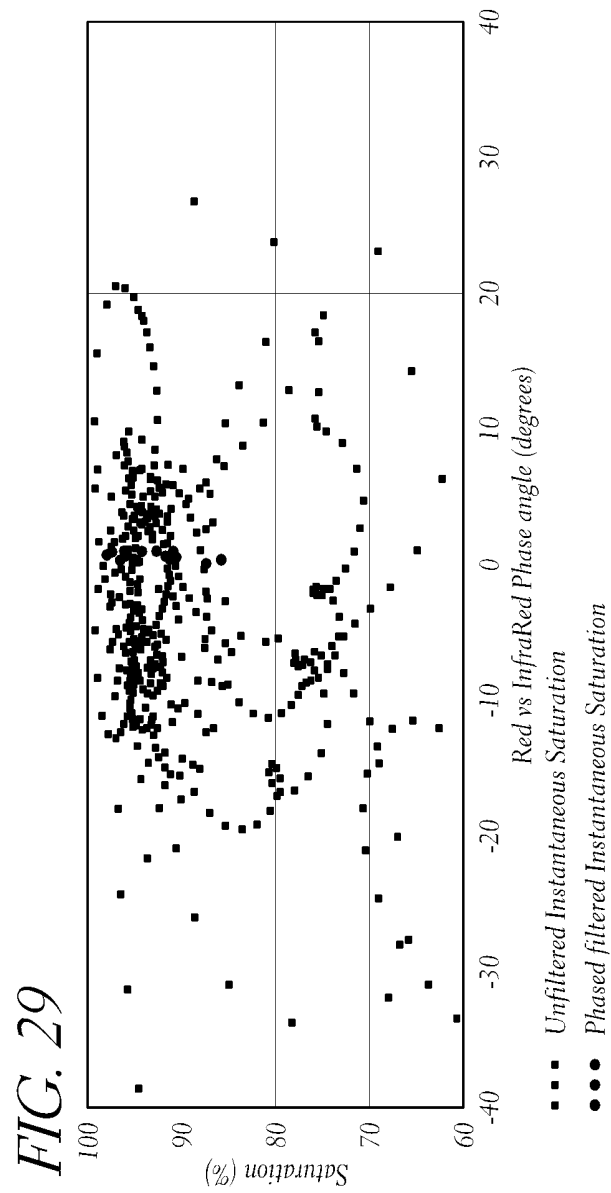


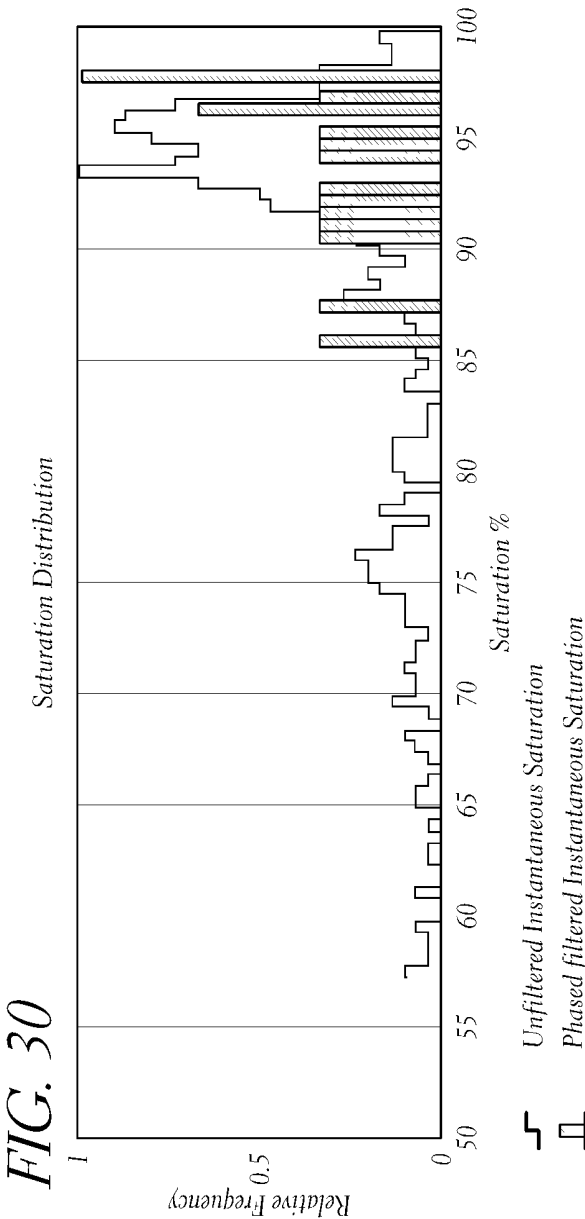

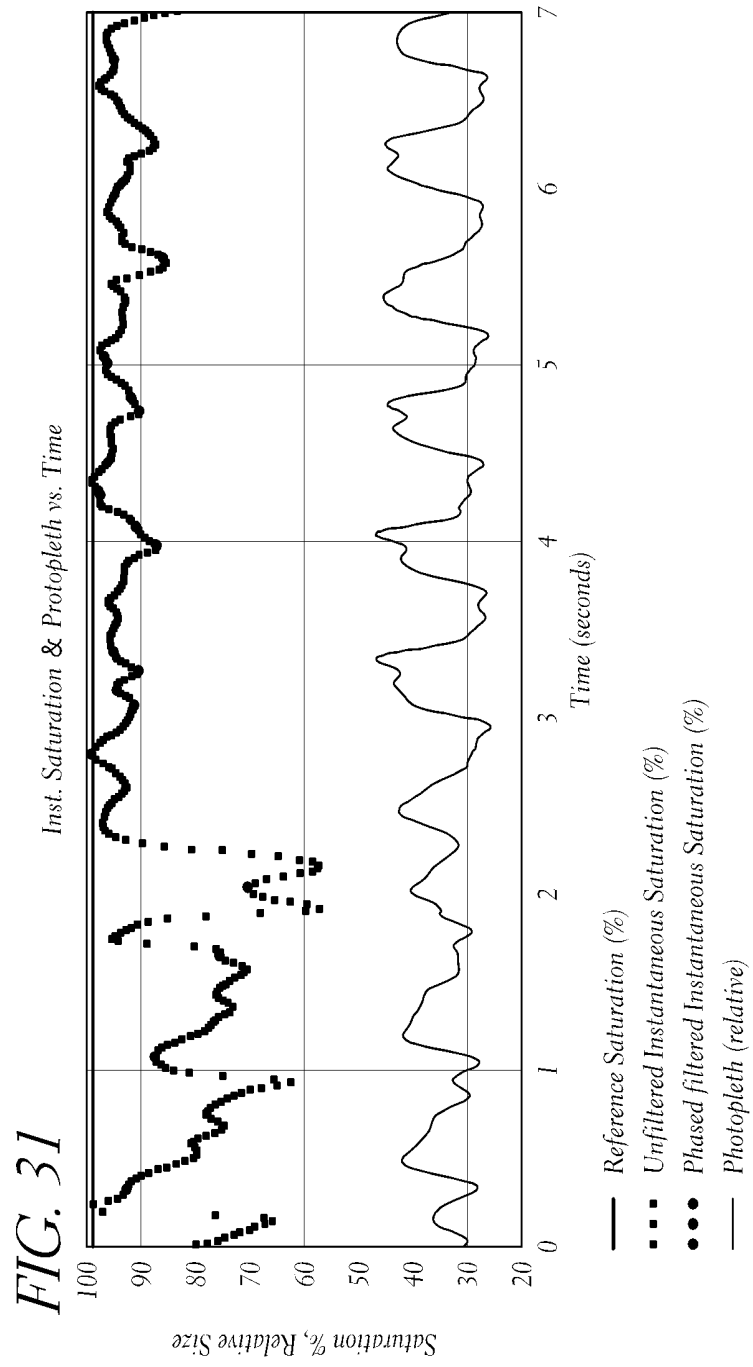

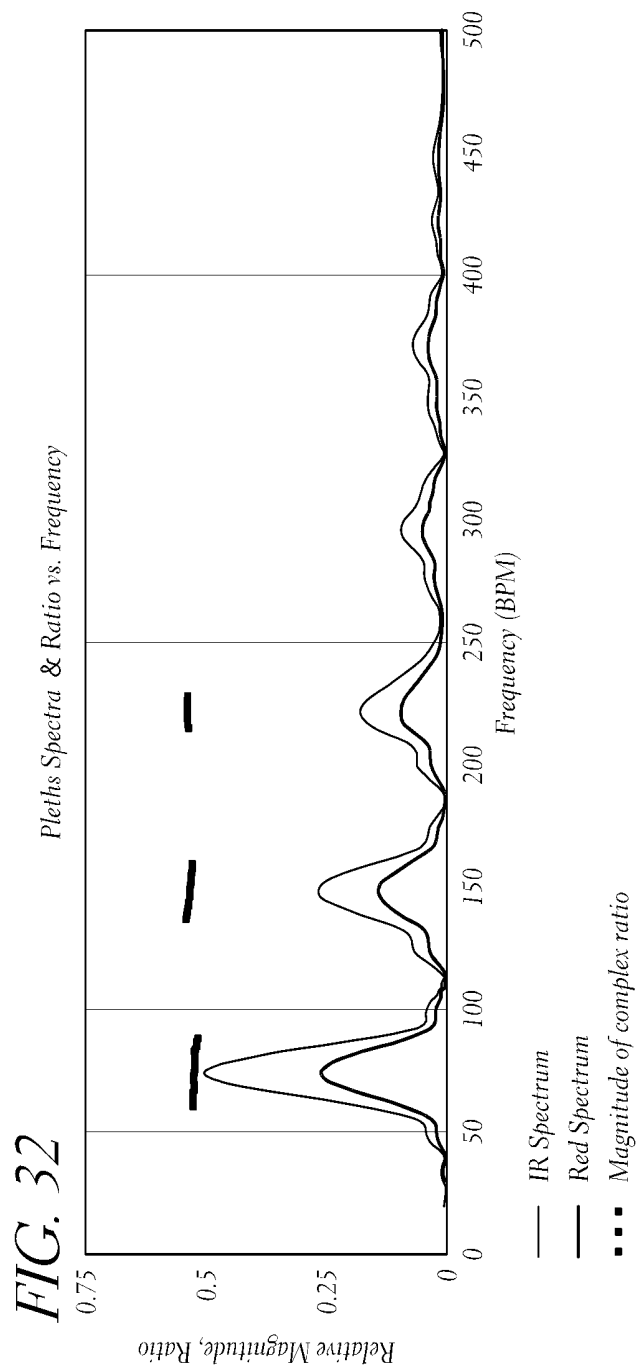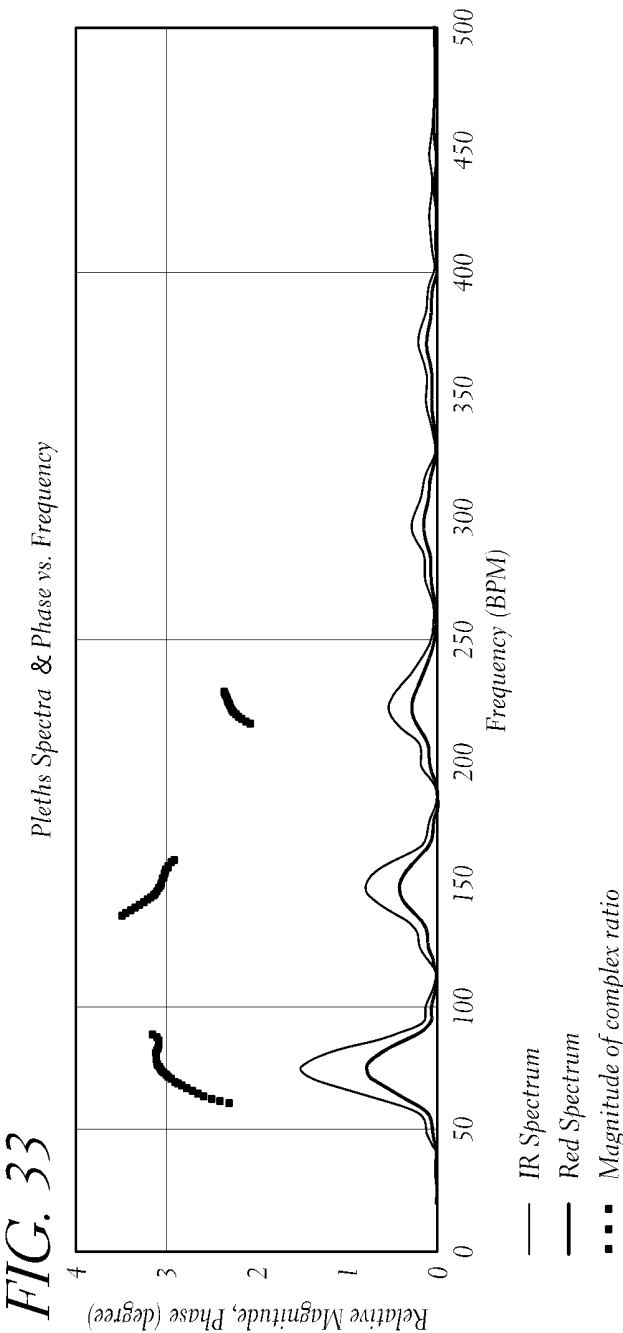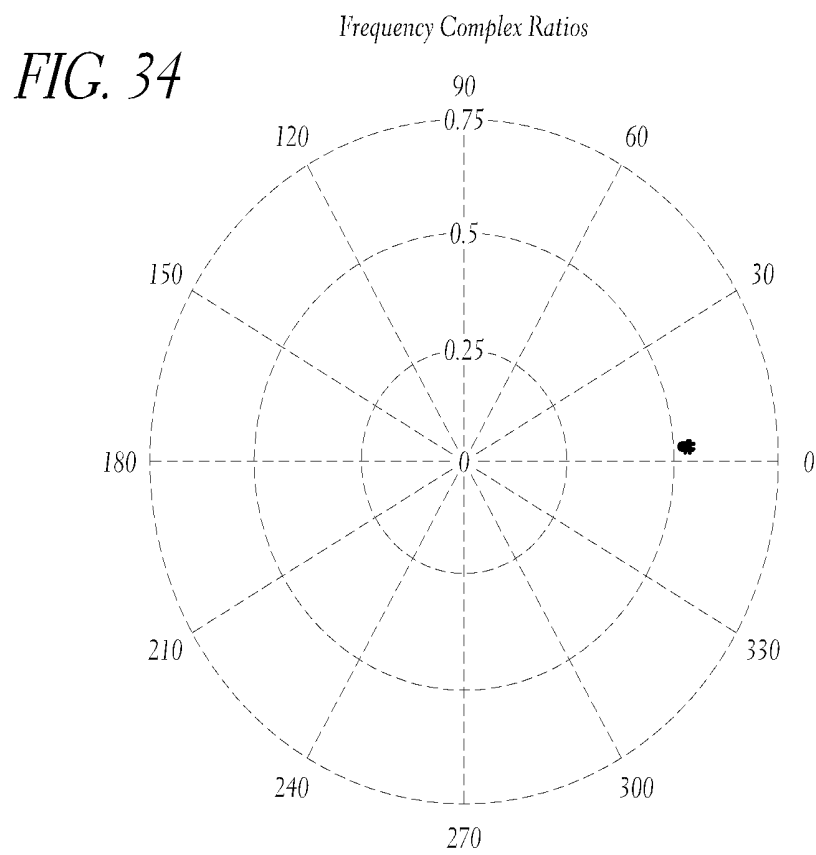





SYSTEMS AND METHODS FOR DETERMINING BLOOD OXYGEN SATURATION VALUES USING COMPLEX NUMBER ENCODING

REFERENCE TO RELATED APPLICATIONS

The present application claims priority benefit under 35 U.S.C. §120 to, and is a continuation of, U.S. patent application Ser. No. 13/896,731, filed May 17, 2013, entitled "Systems and Methods for Determining Blood Oxygen Saturation Values Using Complex Number Encoding," which is a continuation of U.S. patent application Ser. No. 12/248,868, filed Oct. 9, 2008, now U.S. Pat. No. 8,447,374, entitled "Systems and Methods for Determining Blood Oxygen Saturation Values Using Complex Number Encoding," which is a continuation of U.S. patent application Ser. No. 11/288,812, filed Nov. 28, 2005, now U.S. Pat. No. 7,440,787, entitled "Systems and Methods for Determining Blood Oxygen Saturation Values Using Complex Number Encoding," which is a continuation of U.S. patent application Ser. No. 10/727,348, filed Dec. 3, 2003, now U.S. Pat. No. 6,970,792, entitled "Systems and Methods for Determining Blood Oxygen Saturation Values Using Complex Number Encoding," which claims priority benefit under 35 U.S.C. §119(e) from U.S. Provisional Application No. 60/430,834, filed Dec. 4, 2002, entitled "Systems and Methods for Determining Blood Oxygen Saturation Values Using Complex Number Encoding." The present application hereby incorporates the foregoing disclosures herein by reference in their entirety.

FIELD OF THE INVENTION

The present invention relates to the field of pulse photometry. More specifically, the invention relates to calculating continuous saturation values using complex number analysis.

BACKGROUND OF THE INVENTION

Pulse photometry is a noninvasive technique for measuring blood analytes in living tissue. In this technique, multiple light sources emit light of differing wavelengths, which is transmitted through or reflected from a vascular bed. One or more photodetectors then detect the transmitted or reflected light as an optical signal. As the photons propagate through the tissue, they are subjected to random absorption and scattering processes due to the nonhomogeneous nature of the tissue. These effects manifest themselves as a loss of energy in the optical signal, and are generally referred to as bulk loss. In addition to bulk loss, the optical signal is modulated by the flow of arterial blood into the vascular bed. Moreover, the movement of venous blood into or out of the tissue, local tissue compression and local muscle movements super-impose yet another modulation on the optical signal, usually of lower frequency than the arterial flow. For example, FIG. 1 illustrates detected optical signals that include the foregoing attenuation, arterial flow modulation, and low frequency modulation. Each optical signal, with its combined attenuation and modulations, e.g., each combined optical signal, is generally referred to as a photoplethysmograph (photopleth).

Pulse oximetry is a special case of pulse photometry where the oxygenation of arterial blood is sought in order to estimate the state of oxygen exchange in the body. In order to calculate the oxygen saturation of arterial blood, two

wavelengths of light, e.g. Red, at about 660 nm, and Infrared, at about 900 nm, are used to calculate the ratio of two dominant hemoglobin components, oxygenated hemoglobin (HbO₂) and deoxygenated hemoglobin (Hb). The detected optical signals, which correspond to the Red and Infrared wavelengths, are first normalized in order to balance the effects of unknown source intensity as well as unknown bulk loss at each wavelength. The arterial pulses are then isolated by filtering each normalized signal, where a high pass or a band-pass filter takes advantage of the typically higher frequency of the pulsatile arterial blood, hence the name pulse oximetry. This normalized and filtered signal is referred to as the AC component and is typically sampled with the help of an analog to digital converter with a rate of about 30 to about 100 samples/second. For example, FIG. 2 illustrates the optical signals of FIG. 1 after they have been normalized and bandpassed.

In order to estimate blood oxygenation, a (Red/Infrared) ratio is calculated by dividing the strength of the Red AC (RdAC) by the corresponding strength of the Infrared AC (IrAC). The (RdAC/IrAC) ratio is then generally plugged into an empirical calibration curve equation that relates it to blood oxygenation. For example, reference can be made to Japanese Patent No. Sho 50/1975-128387, issued to Aoyagi, entitled "*Optical Type Blood Measuring Equipment*."

The arterial blood flow generally has a higher fundamental frequency than other components of the photopleth, however, there are cases where the two frequencies may overlap. One such example is the effect of motion artifacts on the optical signal, which is described in detail in U.S. Pat. No. 6,157,850, issued to Diab et al., entitled "Signal Processing Apparatus." Another effect occurs whenever the venous component of the blood is strongly coupled, mechanically, with the arterial component. This condition leads to a venous modulation of the optical signal that has the same or similar frequency as the arterial one. Such conditions are generally difficult to effectively process because of the overlapping effects.

As described in the Aoyagi patent, the strength of each AC waveform may be estimated by measuring its size through, for example, a peak-to-valley subtraction, by a root mean square (RMS) calculations, integrating the area under the waveform, or the like. These calculations are generally least averaged over one or more arterial pulses. It is desirable, however, to calculate instantaneous ratios (RdAC/IrAC) that can be mapped into corresponding instantaneous saturation values, based on the sampling rate of the photopleth. However, such calculations are problematic as the AC signal nears a zero-crossing where the signal to noise ratio (SNR) drops significantly. For example, dividing two signals with low SNR values can render the calculated ratio unreliable, or worse, can render the calculated ratio undefined, such as when a near zero-crossing area causes division by or near zero. To try to avoid division by zero, the Ohmeda Biox pulse oximeter calculated the small changes between consecutive sampling points of each photopleth in order to get instantaneous saturation values. FIG. 3 illustrates various techniques used to try to avoid the foregoing drawbacks related to zero or near zero-crossing, including the differential technique attempted by the Ohmeda Biox.

Note that Ohmeda's differential technique is equivalent to a calculation over a derivative of the photopleth, and the derivative has the same low SNR problem whenever a flattened section of the photopleth is used in the ratios calculations. For example, the derivative will have a zero or near zero value and the RdAC/IrAC ratio will become unreliable or undefined, even in a substantially noise free

signal. For example, FIG. 4 illustrates the derivative of the IrAC photopleth plotted along with the photopleth itself. As shown in FIG. 4, the derivative is even more prone to zero-crossing than the original photopleth as it crosses the zero line more often. Also, as mentioned, the derivative of a signal is often very sensitive to electronic noise. For example, according to "Pulse Oximetry: Analysis of Theory, Technology, and Practice," Journal of Clinical Monitoring, Vol. 4, Oct. 1988, a published paper by the designers of the Ohmeda Biox, the calculated instantaneous saturations over some sections of the photopleth can be off by more than 50 percent (0/0) from the real value over a time as short as 1/10th of a second. As the designers described in their paper, this result is clearly an artifact of the signal processing technique employed in the Biox pulse oximeter since the blood saturation value can not change by that amount in 1/10th of a second.

Because of some of the foregoing drawbacks associated with the determination of instantaneous or point-by-point saturation from RdAC/IrAC ratios, designers now typically unequally weigh the calculated instantaneous saturation values over each photopleth, even when the photopleth is substantially noise free, with the consequence that a significant number of saturation values receive insignificant weights. This is tantamount to filtering out or ignoring valid signal data during the troublesome sections described above.

SUMMARY OF THE INVENTION

The result of the foregoing drawbacks is that the previous attempts fail to determine a stream of point-by-point saturation values. However, it is noteworthy that the sensitivity of the ratio calculation near a zero-crossing section of the waveform is not intrinsic to the photopleth itself, but rather an artifact of passing the detected signal through a high-pass filter. Accordingly, an aspect of the present invention includes a method of determining continuous and reliable calculations of the (RdAC/IrAC) ratio for each sampling point without concern for zero-crossing areas. As discussed in the foregoing and disclosed in the following, such determination of continuous ratios is very advantageous, especially in cases of venous pulsation, intermittent motion artifacts, and the like. Moreover, such determination is advantageous for its sheer diagnostic value.

For purposes of summarizing the invention, certain aspects, advantages and novel features of the invention have been described herein. Of course, it is to be understood that not necessarily all such aspects, advantages or features will be embodied in any particular embodiment of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

A general architecture that implements the various features of the invention will now be described with reference to the drawings. The drawings and the associated descriptions are provided to illustrate embodiments of the invention and not to limit the scope of the invention.

FIG. 1 illustrates a photopleth including detected Red and Infrared signals.

FIG. 2 illustrates the photopleths of FIG. 1, after it has been normalized and bandpassed.

FIG. 3 illustrates conventional techniques for calculating strength of one of the photopleths of FIG. 2.

FIG. 4 illustrates the IrAC photopleth of FIG. 2 and its derivative.

FIG. 4A illustrates the photopleth of FIG. 1 and its Hilbert transform, according to an embodiment of the invention.

FIG. 5 illustrates a block diagram of a complex photopleth generator, according to an embodiment of the invention.

FIG. 5A illustrates a block diagram of a complex maker of the generator of FIG. 5.

FIG. 6 illustrates a polar plot of the complex photopleths of FIG. 5.

FIG. 7 illustrates an area calculation of the complex photopleths of FIG. 5.

FIG. 8 illustrates a block diagram of another complex photopleth generator, according to another embodiment of the invention.

FIG. 9 illustrates a polar plot of the complex photopleth of FIG. 8.

FIG. 10 illustrates a three-dimensional polar plot of the complex photopleth of FIG. 8.

FIG. 11 illustrates a block diagram of a complex ratio generator, according to another embodiment of the invention.

FIG. 12 illustrates complex ratios for the type A complex signals illustrated in FIG. 6.

FIG. 13 illustrates complex ratios for the type B complex signals illustrated in FIG. 9.

FIG. 14 illustrates the complex ratios of FIG. 13 in three (3) dimensions.

FIG. 15 illustrates a block diagram of a complex correlation generator, according to another embodiment of the invention.

FIG. 16 illustrates complex ratios generated by the complex ratio generator of FIG. 11 using the complex signals generated by the generator of FIG. 8.

FIG. 17 illustrates complex correlations generated by the complex correlation generator of FIG. 15.

FIG. 18 illustrates the square root of the magnitude of the complex ratios of FIG. 16 vs. the complex correlations of FIG. 17.

FIG. 19 illustrates a plot of the instantaneous saturation of the data used to generate the complex ratios shown in FIG. 12, as well as the corresponding complex photopleth from which the saturation was calculated.

FIG. 20 illustrates an expanded view of the saturation distribution results of FIG. 19.

FIGS. 21 and 22 illustrate Infrared and Red photopleths, respectively, modulated by venous pulsation.

FIG. 23 illustrates an instantaneous saturation which highlights a large spread of values over one photopleth, as compared to that of FIG. 19 and FIG. 20.

FIG. 24 illustrates a histogram of the distribution of the instantaneous saturation values of FIG. 23.

FIGS. 25 and 26 illustrate photopleth signals that are corrupted by motion artifacts.

FIG. 27 illustrates a polar plot for type A complex waveforms generated using the photopleths of FIGS. 25 and 26.

FIG. 28 illustrates a polar plot for type B complex waveforms generated using the photopleths of FIGS. 25 and 26.

FIG. 29 illustrates the complex ratios of FIG. 27 after being filtered, according to embodiments of the invention.

FIG. 30 illustrates a histogram of the filtered saturation points of FIG. 29.

FIG. 31 illustrates plots of unfiltered instantaneous saturation values generated from the photopleths of FIGS. 25 and 26, as well as the phase filtered saturation values of FIGS. 29 and 30.

FIG. 32 illustrates magnitudes of complex frequency ratios calculated from the fundamental and harmonics of the photopleths of FIG. 2.

FIG. 33 illustrates frequency transformed photopleths and phases of the corresponding ratios.

FIG. 34 illustrates the polar plot of the complex frequency ratios of FIG. 32 and FIG. 33.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Complex numbers were generally invented/discovered in the 1500's by Galiermo Cardano in Italy as he was struggling to solve a general third order polynomial equation. Later, Argand suggested that each complex number may be represented as a point in a plane where its imaginary part is plotted on the Y-axis and its real part on the X-axis, this is referred to as the Cartesian form of a complex number. An alternate representation of complex numbers is called the polar form where a magnitude and an angle can designate a unique point in the Argand plane, hence representing a complex number. Although mathematicians at that time looked at complex numbers with great suspicion, it turned out that they were useful for the general solutions of polynomial equations and applicable in such diverse fields as quantum mechanics to describe the state of elementary particles.

In the field of electrical engineering, students learn that circuit analysis, under alternating voltage conditions, can be significantly simplified if the concept of complex currents and voltages is introduced. When a voltage is applied to an electrical element, a current is caused to pass through it. Dividing the applied voltage by the corresponding current gives the resistance of the electrical element. In the complex domain, dividing the complex voltage by the complex current give rise to a complex form of resistance called "impedance," which is represented again by a complex number. The real part of the impedance is the resistance while the complex part is related to capacitance and inductance. The complex part affects the phase, lead or lag, of the driving signals. It can be shown that the response of a linear system to a sinusoidal excitation is a sinusoid with the same frequency but generally of different amplitude and phase. A resistor element, for example, affects the amplitude only, whereas a capacitor or an inductor affects the phase. A combination of resistors, capacitors and/or inductors can affect the amplitude as well as the phase of the driving excitation and are considered examples of a linear system. Since each complex number consists of amplitude and phase, it is natural that they be used to encode the amplitude and phase and track their evolution throughout a linear system. Therefore, when a linear system is driven by a complex excitation, its output will be the same complex input multiplied by a complex scaling factor that scales its amplitude appropriately and adds a certain phase in accordance with the rules of complex multiplication. Note that the phase in this context is a relative one between two fundamental variables of the system, e.g. for an electrical circuit they might be voltage and current at a certain node of the circuit, or output voltage and input voltage, or the like.

In pulse oximetry, there is no direct analog for voltages or currents. Generally, pulse oximetry deals with two highly correlated optical signals, e.g., the Red and Infrared signals, with fundamentally little or no discernible phase difference. Thus, encoding those signals as complex numbers seems to add little or no value to the signal processing. However, there are several conditions under which a variable phase difference may be introduced between the Red and Infrared signals. For example, motion artifacts create a condition where the sensor may decouple from the skin. In such a

condition, the detected optical signals will have components that depend on the refraction through the sensor material itself instead of the wavelength of light, as well as the desired components that have traveled through the vascular bed. Venous pulsation creates another condition, which, as disclosed in the foregoing, affects the phase difference. Under the foregoing conditions where the phase is changing, use of complex number encoding provides advantages in signal processing, including providing the ability to continuously monitor the arterial saturation vs. time without concern about signal zero-crossing, as disclosed in the following.

A Hilbert Transformer is a signal processing technique that takes a real signal and converts it into a related signal which has its frequency components shifted by $\pi/2$ radians for positive frequencies, and by $-\pi/2$ radians for negative frequencies, without affecting their respective amplitudes. The book, "*Theory and Application of Digital Signal Processing*, Prentice-Hall, Inc.," by Rabiner and Gold, introduces the subject. Formation of a complex signal is accomplished by considering the original signal itself as the real part of a complex signal and the output of the Hilbert Transformer as the imaginary part of the same complex signal. Such signals are generally referred to as an "analytical signal" in the signal processing field because the magnitudes of its negative frequencies are equal to zero. In the context of pulse photometry, we shall refer to such a complex signal as complex photopleth or complex AC.

It is noteworthy that the prior methodology of seeking a derivative of a signal shifts that signal's components by $\pi/2$ radians, similar to the Hilbert transform. However, the derivative of a signal also multiplies each corresponding amplitude by the value of the radian frequency ω , thus magnifying the signal's frequency components as the components increase in frequency. Thus, the derivative is often more sensitive to electronic noise. In contrast, the Hilbert Transformer generally has a flat response with respect to frequency. However, a skilled artisan will recognize other transforms, derivatives, or the like, can be used to encode the imaginary part of the complex photopleth.

When the foregoing complex encoding is applied to both RdAC and IrAC photopleths, as shown in a complex photopleth generator of FIG. 5, then both complex RdAC and IrAC are in phase. As shown in FIG. 5, the complex photopleth generator 500 includes one or more log filters 502, one or more high pass filters 504, one or more Hilbert transformers 506, and one or more complex makers 508. The log and high pass filter 502 and 508 generally normalize and filter the signals, as disclosed in the foregoing with reference to FIG. 2. The Hilbert transformers 506 converts the real signal into related signals shifted by $\pi/2$ and $-\pi/2$ radians, also as disclosed in the foregoing. The complex makers 508 combine the output of the Hilbert transformers 506 with the input of the Hilbert transformers 506 to generate complex in phase photopleths, generally referred to herein as type "A" complex signals, as shown in FIG. 5A. FIGS. 6 and 7 illustrate polar plots of the complex photopleths generated from the generator 500 of FIG. 5.

FIG. 8 illustrates a complex photopleth generator 800, according to another embodiment of the invention. As shown in FIG. 8, the generator 800 includes the one or more log filters 502, the one or more high pass filters 504, the one or more Hilbert transformers 506, and the one or more complex makers 508 disclosed with respect to FIG. 5. However, in the generator 800, the Hilbert transformer 506 accepting the exemplary Red signal encodes the real components of the RdAC signal rather than the complex com-

ponents. Thus, the generator **800** of FIG. **8** generates a complex photopleth, generally referred to herein as type "B" complex signals. FIGS. **9** and **10** illustrate polar plots of the complex photopleths generated from the generator **800** of FIG. **8**. Note that as time progresses, the locus of the complex points rotates around the origin but does not pass through it, regardless of type A or type B complex signals. Accordingly, the strength of each of the foregoing AC photopleth complex signals can be encoded in their respective magnitudes, which is the length between the origin and any point on the complex waveform in FIGS. **6**, **7**, **9** and **10**. The morphology of the complex signals depend on the condition of the subject, such as, for example, age, blood pressure, arterial impedance, posture, or the like.

Based on the foregoing disclosure, the complex photopleths of FIGS. **6**, **7**, **9** and **10** can be classified with techniques like the "Slant Line Transform" or other classification techniques available in the field of image recognition or the like. Such classification techniques can be advantageously employed to help reject photopleths that are corrupted by noise, which can be an invaluable during episodes of motion artifacts.

Generating Complex Ratios

FIG. **11** illustrates a complex ratio generator **1100** for generating what will generally be referred to as the "complex ratio." The complex ratio is a point-wise complex division of type A or type B RdAC and IrAC complex photopleth signals. The magnitude of each division carries along with it the conventional (RdAC/IrAC) ratio, in addition, its phase encodes the angle variation between the Red and Infrared signals, which as disclosed in the foregoing, can generally be equal to zero for undisturbed signals. Different plots in the complex plane result depending upon whether type A or type B complex waveforms are used to generate the complex ratios. The different plots also enable or suggest different types of signal processing, examples of which are disclosed as follows.

For example, when the arterial saturation is constant and type A complex waveforms are generated, the complex ratio plot in the complex plane looks like a fuzzy point very close to the real axis, as shown in FIG. **12**. This is remarkable for it indicates, unlike previous techniques, that the instantaneous ratios over one or several photopleths are nearly constant throughout, which matches the input signal data, i.e., that the saturation is constant. FIG. **19** illustrates a plot of the instantaneous saturation vs. time of the data used to generate the complex ratios shown in FIG. **12**, as well as the corresponding photopleth from which the saturation was calculated. Note that the saturation is generally calculated from the magnitudes of the complex ratios vs. time. Also, FIG. **20** illustrates that the maximum deviation from the mean value of the saturation is less than about 0.5 percent (%), which compares favorably to the more than about 50 percent (%) variations calculated using the Biox algorithm. Moreover, FIG. **20** illustrates that the standard deviation of the saturation is a mere about 0.18 percent (%). These results clearly and advantageously indicate that weighing or filtering is not needed to utilize the data, and that all points in the photopleth can be useful in the subsequent analysis.

FIG. **13** is a plot of the complex ratios generated by the photopleths used to generate FIG. **12**, but with type B complex waveforms. As shown in FIG. **13**, the constant saturation translated into a circle of fixed radius in the complex plane. A myriad of mapping techniques available in the field of complex analysis can be brought to bear to help analyze this type of signal. For example, the logarithm function may be used to map a circle in the complex plane

into a line in the same complex plane. FIG. **14** depicts a 3D plot of complex ratios vs. time, where time is plotted along the vertical 'Z' axis. As shown in FIG. **14**, a constant ratio, i.e. constant saturation, is reflected as a uniform helix.

Generating Confidence Measures

Normally, each of the instantaneous complex ratio values are valid and reliable. However, certain physiological or patient motion conditions may render a some or all of the calculated ratios unusable. Therefore, it is desirable to provide confidence measures by which such unreliable points may be discarded, filtered or corrected. Toward that end, FIG. **15** illustrates a complex correlation generator **1500**, which includes one or more conjugate generators **1502**, one or more signal multipliers **1504**, signal adders **1506** and signal dividers **1508**. As shown in FIG. **15**, the complex RdAC and the complex IrAC are input into the generator **1502**. The complex RdAC is multiplied by the conjugate of the complex IrAC. This product is divided by the sum of the complex IrAC multiplied with its conjugate, and the product of the complex RdAC and its conjugate. The resulting signal is then multiplied by the scalar two (2) to form a measure of the complex correlation, such as, for example, a complex confidence number associated with each calculated complex ratio.

This confidence may be used to gate or preferentially weigh each corresponding complex ratio in a filtering technique to provide more reliable saturation values. For example, FIG. **16** depicts a plot of instantaneous complex ratios calculated over several seconds and FIG. **17** depicts the instantaneous complex correlations associated with the calculated complex ratios. FIG. **18** depicts the joint relationship between the calculated complex ratios of FIG. **16** and associated the complex correlation of FIG. **17**. Note that a certain correlation threshold may be established below which all data point can be rejected, thereby advantageously enhancing the final saturation estimation. Note that in FIG. **18**, all the data points are acceptable. Situations where not all data points are acceptable, e.g. abnormal waveforms or motion artifacts, will be disclosed in the following.

The phase of the instantaneous complex ratios may also be used to assign a confidence measure to each complex ratio value. Typically the phase value should be very close to zero in the case of complex ratios generated from type A complex waveforms, as shown in FIG. **12**. However, example of the use of the phase in the filtering of unreliable complex ratios under the effects of motion artifacts will also be discussed in the following.

Implementing Filtering Techniques

Once the complex waveforms or their corresponding instantaneous complex ratios or saturation values are available, a myriad of linear, nonlinear and statistical filtering techniques may be applied to reliably estimate the blood saturation values. For example, when simple averaging is desired, the areas of the complex photopleth waveforms shown in FIG. **6** can be calculated over a certain span of time or integral number of pulses. The ratio between two values corresponding to the Red and Infrared waveforms' areas is calculated, the result of which can then be used to calculate the blood saturation value. Note that this is the analog of integrating the area of the Red and Infrared photopleths shown in FIG. **2** then taking their ratios. FIG. **3** shows an example of area integration of one real waveform. For the case of a complex waveform the area can be estimated by summing the individual areas of triangles that constitute the complex waveform, as shown in FIG. **7**. Introductory calculus textbooks may be consulted on the subject of area integration. This technique does not require the use of

complex ratios, rather straightforward real number division of waveform areas can be used.

Another powerful filtering technique takes advantage of the abundance of ratios values available over short period of time. For example, the continuous stream of instantaneous ratio or saturation values can be fed into a weighing filter along with their associated confidence values. The filter can then discard or appropriately weigh the corresponding value of the ratio or the saturation. The high number of values, e.g., 62.5 values per second in the present embodiment, available to the filter makes it more likely that some of them will be within an acceptable limit despite the affect of disturbances or noise.

Statistical techniques such as frequency distribution analysis can further be used alone or in combination with the previous techniques to estimate the true blood saturation values. Exemplary techniques where the statistics of the distribution of the ratio or saturation values can be used to extract a more accurate estimation of the true saturation value, as disclosed in the following.

Managing Abnormal Waveforms

Under certain physiological conditions, venous blood in the vascular bed may undergo pulsation that may or may not be coupled to the arterial pulsation. These pulsation can be strong enough as to disrupt the normal ratio calculations thus giving erroneous saturation readings. When the arterial pulsation has a distinct frequency from the venous pulsation, then the arterial pulsation can be isolated using frequency analysis such as the Fast Fourier Transform used to perform a Saturation Transform, as disclosed in U.S. Pat. No. 6,157,850, mentioned in the foregoing. Strong venous coupling may not be necessarily uniform in time across each arterial pulse, and under certain patient conditions the venous pulse may affect only a portion on the photopleth. This can be advantageous for an algorithm that analyzes the information in the time domain. FIGS. 21 and 22 depict Infrared and Red photopleths that are modulated by venous pulsation. Although their shape may look like a normal photopleth, the instantaneous saturation vs. time curve in FIG. 23 illustrates a large spread in the instantaneous saturation values over one photopleth, as compared to that of FIG. 19 and FIG. 20.

Under such conditions, taking the average value (or determining the area) of all the instantaneous saturation points may not be the best estimate of the true saturation value. For example, the distribution of the instantaneous saturation values of FIG. 23, e.g. the histogram illustrated in FIG. 24 shows a skewed distribution with a mode at about 83.5 percent (%). This is about 1.8 percent (%) below the average saturation value of about 85.3 percent (%). Another possibility is to phase filter the data and the use the distribution in a similar manner. Phase filtering will be discussed in more detail in the section on managing motion artifacts. In yet another approach, averaging the saturation values over a certain subsection of the photopleth, away from the location of the venous pulsation, can generate more accurate saturation values.

Managing Motion Artifacts

In the context of pulse oximetry, "motion artifacts" refer to any extraneous disturbing source that affects the shape or quality of the optically detected photopleth signal. The disturbance may be a deformation of the vascular bed, a decoupling of the photo detector from the skin, the movement of the sensor itself along the skin surface, or the like. The wide dynamic range of the effect, in terms of its frequency and size, as well as its multiple sources, makes the impact of motion artifacts on the photopleth quite dramatic. More importantly, the impact of motion artifacts on the

calculated saturation values can also be very large, thus causing drawbacks in many older generations of pulse oximeters. For example, when motion is repetitive and affects the photopleth over its entirety, then a combination of adaptive filtering and frequency-domain techniques can provide the best estimates of the saturation values. On the other hand, when motion is intermittent or non-repetitive, e.g. pseudo random, then a combination of a time-domain analysis and adaptive filtering techniques with fast adaptation rates works better. While each of the foregoing techniques has its strength and weaknesses, use of multiple parallel engines executing two or more of the foregoing techniques in parallel, and then fusing their results together, often provides best overall performance. Toward that end, the present technique of complex analysis can be a valuable addition to a set of parallel engines that advantageously improves the accuracy of pulse oximeters by correcting for a subset of conditions where the previous algorithms have failed. For example, the ability of the present algorithm to explicitly encode the phase of the signal on a point by point basis renders it very valuable in case of sensor decoupling from the skin where phase decorrelation between Red and Infrared photopleths is prevalent.

FIGS. 25 and 26 illustrate photopleth signals that are corrupted by motion artifacts. FIG. 27 illustrates a polar plot for type A complex waveforms generated using the photopleths of FIGS. 25 and 26, while and FIG. 28 illustrates a polar plot for type B complex waveforms generated using the photopleths of FIGS. 25 and 26. It is noteworthy to compare and contrast FIG. 12 with FIG. 27. As disclosed in the foregoing, FIG. 12 illustrates complex ratios where the input signals are motion artifact free. FIG. 12 exhibits a localized point with a magnitude of about 0.53, which generally corresponds to a saturation of about 99 percent (%). Note that the small angle it subtends near the real axis. On the other hand, FIG. 27 illustrates complex ratios where the input signals are riddled with motion artifacts, resulting in ratios with varying magnitudes having widely varying angles.

At the outset, it is difficult to tell which ratios of FIG. 27 are true and which ratios were affected by noise and are therefore, false. However, as shown in FIG. 28, a phase filter can select or pass values similar to those expected, such as, for example, values that subtend low angles from the origin. In one embodiment, the phase filter passes values corresponding to the type and value of phase angles determined, for example, through calibration processes performed and associated with valid data. In an embodiment, the phase filter selects or passes values corresponding to phase angles ranging from about -2.0 to about 3.0 degrees, and more preferably, selects values corresponding to phase angles ranging from about 0.0 to about 1.0 degrees. When the phase filtered saturation points are histogrammed, as shown in FIG. 30, the most likely saturation is somewhere near about 98 percent (%), which is only about 1 percent (%) away from the true saturation value of about 99 percent (%). FIG. 31 also includes plots of unfiltered instantaneous saturation values vs. time as well as the phase filtered saturation values plotted on top of them. The corresponding photopleth is also shown for comparison.

Using Frequency Domain Complex Ratios

When a real signal is transformed into the frequency domain, using the Fourier transform for example, the corresponding frequency representation is a series of complex numbers. These complex numbers denote complex frequencies each having a magnitude and a phase. When the Red and Infrared photopleths are transformed into the frequency

11

domain, their corresponding complex frequencies can advantageously be divided to generate complex ratios. Each complex ratio possesses a magnitude and a phase similar to the complex ratios generated in the time domain, as disclosed in the foregoing. The frequency domain complex ratios are a representation that has complex ratios vs. frequency, as opposed to representations that have time domain complex ratios vs. time. As disclosed, each technique has its advantages and disadvantages depending on the type of signals present and the nature of the perturbations.

An example of the use of frequency domain complex ratios according to aspects of the present invention are illustrated in FIG. 32 and FIG. 33. A series of ratios are calculated for the fundamental and first two (2) harmonics of the photoplethysm waveforms shown in FIG. 2. FIG. 32 illustrates the magnitudes of the complex frequency ratios calculated from the fundamental and harmonics of the photoplethysm of FIG. 2, while FIG. 33 illustrates frequency transformed photoplethysm and the phases of the corresponding ratios. FIG. 34 illustrates the polar plot of the complex frequency ratios of FIG. 32 and FIG. 33.

Although the foregoing disclosure generally references various signal processing mechanisms, a skilled artisan will recognize from the disclosure herein that the generators 500, 800, 1100, and 1500 can be implemented with software, firmware, or the like executing on hardware, such as, for example a digital signal processor (DSP). Moreover, the calculations incorporated into the generators can be carried out using software, hardware, or combinations of the same. In addition, the DSP can be part of a portable or stationary device, such as an oximeter, personal monitoring device, or the like.

Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. Accordingly, the present invention is not intended to be limited by the reaction of the preferred embodiments, but is to be defined by reference to the appended claims.

Additionally, all publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application was specifically and individually indicated to be incorporated by reference.

What is claimed is:

1. A physiological monitor that computes arterial oxygen saturation in tissue material, the physiological monitor comprising:

a light emitter which emits light of at least first and second wavelengths;

a light detector responsive to light from said light emitter attenuated by body tissue, said light detector providing an output signal indicative of at least first and second intensity signals associated with said at least first and second wavelengths; and

one or more hardware processors programmed to encode the first and second intensity signals in a complex domain; filter artifacts based on the complex encoding of the first and second intensity signals; compute arterial oxygen saturation from the filtered complex encoding

12

of the first and second intensity signals; and output the calculated arterial oxygen saturation.

2. The physiological monitor of claim 1, wherein the filtering of artifacts comprises filtering ratios corresponding to the encoded first and second intensity signals.

3. The physiological monitor of claim 2, wherein the filtering comprises using a phase filter including a first range of phases.

4. The physiological monitor of claim 3, wherein the first range of phases comprise phase angles from about -2.0 to about 3.0 degrees.

5. The physiological monitor of claim 3, wherein the first range of phases comprise phase angles from about 0 to about 1 degree.

6. The physiological monitor of claim 2, wherein the filtering comprises using a weighing filter on a continuous stream of instantaneous ratios corresponding to the first and the second intensity signals.

7. The physiological monitor of claim 1, wherein the complex domain comprises complex time domain.

8. The physiological monitor of claim 1, wherein the complex domain comprises complex frequency domain.

9. The physiological monitor of claim 1, wherein the one or more hardware processors are further programmed to determine a plurality of ratios over time from the first and the second intensity signals.

10. The physiological monitor of claim 1, wherein the artifacts comprise motion artifacts.

11. The physiological monitor of claim 1, wherein the artifacts comprise venous pulsation.

12. A physiological monitoring method for computing arterial oxygen saturation in tissue material, the physiological monitor method comprising:

driving a light emitter configured to emit light of at least first and second wavelengths;

receiving an output signal indicative from a light detector of at least first and second intensity signals associated with said at least first and second wavelengths;

encoding the first and second intensity signals in a complex domain;

filtering artifacts from the complex encoding of the first and second intensity signals;

computing arterial oxygen saturation based on the filtered complex encoding of the first and second intensity signals; and

output the computed arterial oxygen saturation.

13. The physiological monitoring method of claim 12, wherein the filtering comprises using a phase filter including a first range of phases.

14. The physiological monitoring method of claim 13, wherein the first range of phases comprise phase angles from about -2.0 to about 3.0 degrees.

15. The physiological monitoring method of claim 12, wherein the filtering comprises using a weighing filter on a continuous stream of instantaneous ratios corresponding to the first and the second intensity signals.

16. The physiological monitoring method of claim 12, further comprising determining a plurality of ratios over time from the first and the second intensity signals.

17. The physiological monitoring method of claim 12, wherein the artifacts comprise motion artifacts.

* * * * *

专利名称(译)	使用复数编码确定血氧饱和度值的系统和方法		
公开(公告)号	US9622693	公开(公告)日	2017-04-18
申请号	US14/609841	申请日	2015-01-30
[标]申请(专利权)人(译)	CERCACOR LAB		
申请(专利权)人(译)	CERCACOR LABORATORIES , INC.		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	DIAB MOHAMED K		
发明人	DIAB, MOHAMED K.		
IPC分类号	A61B5/1455 A61B5/024 A61B5/00		
CPC分类号	A61B5/14551 A61B5/02416 A61B5/7207 A61B5/7253 A61B5/7278 A61B5/742 A61B5/743 A61B5/7239		
优先权	12/248868 2013-05-21 US 11/288812 2008-10-21 US 10/727348 2005-11-29 US 60/430834 2002-12-04 US		
其他公开文献	US20150201874A1		
外部链接	Espacenet USPTO		

摘要(译)

本公开包括脉搏血氧测定系统和方法，用于通过编码复域中的光电容积描记器并处理复信号来确定逐点饱和度值。系统使用各种技术过滤运动伪影和其他噪声，包括统计分析，如相关或相位滤波。

