



US010231676B2

(12) **United States Patent**  
**Al-Ali et al.**

(10) **Patent No.:** **US 10,231,676 B2**  
(45) **Date of Patent:** **Mar. 19, 2019**

(54) **DUAL-MODE PATIENT MONITOR**

(71) Applicant: **MASIMO CORPORATION**, Irvine, CA (US)

(72) Inventors: **Ammar Al-Ali**, Tustin, CA (US); **Don Carothers**, Mission Viejo, CA (US); **David Dalke**, Irvine, CA (US); **Mohamed K. Diab**, Mission Viejo, CA (US); **Julian Goldman**, Irvine, CA (US); **Massi E. Kiani**, Laguna Niguel, CA (US); **Michael Lee**, Aliso Viejo, CA (US); **Jerome Novak**, Aliso Viejo, CA (US); **Robert Smith**, Lake Forest, CA (US); **Val E. Vaden**, Hillsborough, CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **14/022,106**

(22) Filed: **Sep. 9, 2013**

(65) **Prior Publication Data**

US 2014/0012100 A1 Jan. 9, 2014

**Related U.S. Application Data**

(63) Continuation of application No. 11/894,722, filed on Aug. 20, 2007, now Pat. No. 8,532,727, which is a (Continued)

(51) **Int. Cl.**  
**A61B 5/00** (2006.01)  
**A61B 5/1455** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61B 5/7445** (2013.01); **A61B 5/0002** (2013.01); **A61B 5/021** (2013.01);  
(Continued)

(58) **Field of Classification Search**

None  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,109,643 A 8/1978 Bond et al.  
4,331,962 A 5/1982 Neumann  
(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 0 553 372 A1 8/1993  
EP 0 601 589 12/1993  
(Continued)

**OTHER PUBLICATIONS**

US 8,845,543, 09/2014, Diab et al. (withdrawn)  
(Continued)


*Primary Examiner* — Etsub Berhanu

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

A portable patient monitor has an integrated mode in which it operates as a plug-in module for a multiparameter patient monitoring system (MPMS). The patient monitor also has a portable mode in which it operates separately from the MPMS as a battery-powered handheld or standalone instrument. The patient monitor has a sensor port that receives a signal indicative of physiological parameters as input to an internal processor. The patient monitor processes this sensor signal to derive patient measurements. In the portable mode, this information is provided on its display. In the integrated mode, the patient monitor provides patient measurements to the MPMS to be displayed on a MPMS monitor.

**20 Claims, 25 Drawing Sheets**

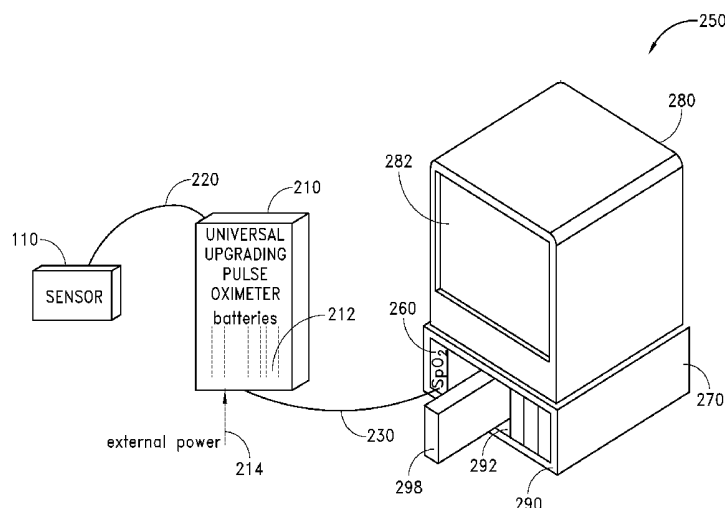

**Related U.S. Application Data**

continuation of application No. 10/911,391, filed on Aug. 3, 2004, now Pat. No. 7,530,949, which is a continuation of application No. 09/641,542, filed on Aug. 18, 2000, now Pat. No. 6,770,028, which is a continuation-in-part of application No. 09/491,175, filed on Jan. 25, 2000, now abandoned.

- (60) Provisional application No. 60/117,097, filed on Jan. 25, 1999, provisional application No. 60/161,565, filed on Oct. 26, 1999.

(51) **Int. Cl.**

**A61B 5/0205** (2006.01)

**A61B 5/021** (2006.01)

**A61B 5/0402** (2006.01)

**A61B 5/0476** (2006.01)

(52) **U.S. Cl.**

CPC ..... **A61B 5/0205** (2013.01); **A61B 5/0402** (2013.01); **A61B 5/0476** (2013.01); **A61B 5/14551** (2013.01); **A61B 5/742** (2013.01); **A61B 2560/0271** (2013.01); **A61B 2560/0443** (2013.01); **A61B 2560/0456** (2013.01)

(56) **References Cited**

## U.S. PATENT DOCUMENTS

|             |         |                          |              |         |                          |
|-------------|---------|--------------------------|--------------|---------|--------------------------|
| 4,704,007 A | 11/1987 | Landre et al.            | 5,687,717 A  | 11/1997 | Halpern et al.           |
| 4,715,385 A | 12/1987 | Cudahy et al.            | 5,701,900 A  | 12/1997 | Shehada et al.           |
| 4,960,128 A | 10/1990 | Gordon et al.            | D393,830 S   | 4/1998  | Tobler et al.            |
| 4,964,408 A | 10/1990 | Hink et al.              | 5,743,262 A  | 4/1998  | Lepper, Jr. et al.       |
| 5,041,187 A | 8/1991  | Hink et al.              | 5,758,644 A  | 6/1998  | Diab et al.              |
| 5,069,213 A | 12/1991 | Polczynski               | 5,760,910 A  | 6/1998  | Lepper, Jr. et al.       |
| 5,111,817 A | 5/1992  | Clark et al.             | 5,769,785 A  | 6/1998  | Diab et al.              |
| 5,163,438 A | 11/1992 | Gordon et al.            | 5,782,757 A  | 7/1998  | Diab et al.              |
| 5,231,981 A | 8/1993  | Schreiber et al.         | 5,785,659 A  | 7/1998  | Caro et al.              |
| 5,375,604 A | 2/1994  | Kelly et al.             | 5,791,347 A  | 8/1998  | Flaherty et al.          |
| 5,319,355 A | 6/1994  | Russek                   | 5,792,052 A  | 8/1998  | Isaacson et al.          |
| 5,331,333 A | 7/1994  | Tagawa et al.            | 5,807,247 A  | 9/1998  | Merchant et al.          |
| 5,337,744 A | 8/1994  | Branigan                 | 5,810,734 A  | 9/1998  | Caro et al.              |
| 5,341,805 A | 8/1994  | Stavridi et al.          | 5,823,950 A  | 10/1998 | Diab et al.              |
| 5,343,869 A | 9/1994  | Pross et al.             | 5,830,131 A  | 11/1998 | Caro et al.              |
| D353,195 S  | 12/1994 | Savage et al.            | 5,830,137 A  | 11/1998 | Scharf                   |
| D353,196 S  | 12/1994 | Savage et al.            | 5,833,618 A  | 11/1998 | Caro et al.              |
| 5,377,676 A | 1/1995  | Vari et al.              | 5,860,919 A  | 1/1999  | Kiani-Azarbayjany et al. |
| D359,546 S  | 6/1995  | Savage et al.            | 5,890,929 A  | 4/1999  | Mills et al.             |
| 5,431,170 A | 7/1995  | Mathews                  | 5,904,654 A  | 5/1999  | Wohlmann et al.          |
| D361,840 S  | 8/1995  | Savage et al.            | 5,910,882 A  | 6/1999  | Burrell                  |
| D362,063 S  | 9/1995  | Savage et al.            | 5,913,823 A  | 6/1999  | Hedberg et al.           |
| 5,448,991 A | 9/1995  | Poison et al.            | 5,919,134 A  | 7/1999  | Diab                     |
| 5,452,717 A | 9/1995  | Branigan et al.          | 5,931,791 A  | 8/1999  | Saltzstein et al.        |
| D363,120 S  | 10/1995 | Savage et al.            | 5,934,925 A  | 8/1999  | Tobler et al.            |
| 5,456,252 A | 10/1995 | Vari et al.              | 5,940,182 A  | 8/1999  | Lepper, Jr. et al.       |
| 5,479,934 A | 1/1996  | Imran                    | 5,944,659 A  | 8/1999  | Flach et al.             |
| 5,482,036 A | 1/1996  | Diab et al.              | 5,947,907 A  | 9/1999  | Duich                    |
| 5,490,505 A | 2/1996  | Diab et al.              | 5,995,855 A  | 11/1999 | Kiani et al.             |
| 5,494,043 A | 2/1996  | O'Sullivan et al.        | 5,997,343 A  | 12/1999 | Mills et al.             |
| 5,533,511 A | 7/1996  | Kaspari et al.           | 6,002,952 A  | 12/1999 | Diab et al.              |
| 5,534,851 A | 7/1996  | Russek                   | 6,011,986 A  | 1/2000  | Diab et al.              |
| 5,561,275 A | 10/1996 | Savage et al.            | 6,027,452 A  | 2/2000  | Flaherty et al.          |
| 5,562,002 A | 10/1996 | Lalin                    | 6,036,642 A  | 3/2000  | Diab et al.              |
| 5,590,649 A | 1/1997  | Caro et al.              | 6,045,509 A  | 4/2000  | Caro et al.              |
| 5,602,924 A | 2/1997  | Durand et al.            | 6,067,462 A  | 5/2000  | Diab et al.              |
| 5,627,531 A | 5/1997  | Posso et al.             | 6,081,735 A  | 6/2000  | Diab et al.              |
| 5,632,272 A | 5/1997  | Diab et al.              | 6,088,607 A  | 7/2000  | Diab et al.              |
| 5,638,816 A | 6/1997  | Kiani-Azarbayjany et al. | 6,110,522 A  | 8/2000  | Lepper, Jr. et al.       |
| 5,638,818 A | 6/1997  | Diab et al.              | 6,124,597 A  | 9/2000  | Shehada                  |
| 5,640,627 A | 6/1997  | Nakano et al.            | 6,128,521 A  | 10/2000 | Marro et al.             |
| 5,640,953 A | 6/1997  | Bishop et al.            | 6,129,675 A  | 10/2000 | Jay                      |
| 5,645,440 A | 7/1997  | Tobler et al.            | 6,137,468 A  | 10/2000 | Martinez et al.          |
| 5,661,632 A | 8/1997  | Register                 | 6,144,868 A  | 11/2000 | Parker                   |
| 5,685,299 A | 11/1997 | Diab et al.              | 6,151,516 A  | 11/2000 | Kiani-Azarbayjany et al. |
| 5,685,314 A | 11/1997 | Geheb et al.             | 6,152,754 A  | 11/2000 | Gerhardt et al.          |
|             |         |                          | 6,157,850 A  | 12/2000 | Diab et al.              |
|             |         |                          | 6,165,005 A  | 12/2000 | Mills et al.             |
|             |         |                          | 6,184,521 B1 | 2/2001  | Coffin, IV et al.        |
|             |         |                          | 6,206,830 B1 | 3/2001  | Diab et al.              |
|             |         |                          | 6,229,856 B1 | 5/2001  | Diab et al.              |
|             |         |                          | 6,232,609 B1 | 5/2001  | Snyder et al.            |
|             |         |                          | 6,236,872 B1 | 5/2001  | Diab et al.              |
|             |         |                          | 6,241,683 B1 | 6/2001  | Macklem et al.           |
|             |         |                          | 6,253,097 B1 | 6/2001  | Aronow et al.            |
|             |         |                          | 6,256,523 B1 | 7/2001  | Diab et al.              |
|             |         |                          | 6,263,222 B1 | 7/2001  | Diab et al.              |
|             |         |                          | 6,278,522 B1 | 8/2001  | Lepper, Jr. et al.       |
|             |         |                          | 6,280,213 B1 | 8/2001  | Tobler et al.            |
|             |         |                          | 6,285,896 B1 | 9/2001  | Tobler et al.            |
|             |         |                          | 6,301,493 B1 | 10/2001 | Marro et al.             |
|             |         |                          | 6,317,627 B1 | 11/2001 | Ennen et al.             |
|             |         |                          | 6,321,100 B1 | 11/2001 | Parker                   |
|             |         |                          | 6,325,761 B1 | 12/2001 | Jay                      |
|             |         |                          | 6,334,065 B1 | 12/2001 | Al-Ali et al.            |
|             |         |                          | 6,343,224 B1 | 1/2002  | Parker                   |
|             |         |                          | 6,349,228 B1 | 2/2002  | Kiani et al.             |
|             |         |                          | 6,360,114 B1 | 3/2002  | Diab et al.              |
|             |         |                          | 6,368,283 B1 | 4/2002  | Xu et al.                |
|             |         |                          | 6,371,921 B1 | 4/2002  | Caro et al.              |
|             |         |                          | 6,377,829 B1 | 4/2002  | Al-Ali                   |
|             |         |                          | 6,388,240 B2 | 5/2002  | Schulz et al.            |
|             |         |                          | 6,397,091 B2 | 5/2002  | Diab et al.              |
|             |         |                          | 6,430,437 B1 | 8/2002  | Marro                    |
|             |         |                          | 6,430,525 B1 | 8/2002  | Weber et al.             |
|             |         |                          | 6,463,311 B1 | 10/2002 | Diab                     |
|             |         |                          | 6,470,199 B1 | 10/2002 | Kopotic et al.           |
|             |         |                          | 6,501,975 B2 | 12/2002 | Diab et al.              |
|             |         |                          | 6,505,059 B1 | 1/2003  | Kollias et al.           |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |         |                          |              |         |                          |
|--------------|---------|--------------------------|--------------|---------|--------------------------|
| 6,515,273 B2 | 2/2003  | Al-Ali                   | 7,096,052 B2 | 8/2006  | Mason et al.             |
| 6,519,487 B1 | 2/2003  | Parker                   | 7,096,054 B2 | 8/2006  | Abdul-Hafiz et al.       |
| 6,525,386 B1 | 2/2003  | Mills et al.             | 7,132,641 B2 | 11/2006 | Schulz et al.            |
| 6,526,300 B1 | 2/2003  | Kiani et al.             | 7,142,901 B2 | 11/2006 | Kiani et al.             |
| 6,541,756 B2 | 4/2003  | Schulz et al.            | 7,149,561 B2 | 12/2006 | Diab                     |
| 6,542,764 B1 | 4/2003  | Al-Ali et al.            | 7,186,966 B2 | 3/2007  | Al-Ali                   |
| 6,580,086 B1 | 6/2003  | Schulz et al.            | 7,190,261 B2 | 3/2007  | Al-Ali                   |
| 6,584,336 B1 | 6/2003  | Ali et al.               | 7,215,984 B2 | 5/2007  | Diab                     |
| 6,595,316 B2 | 7/2003  | Cybulski et al.          | 7,215,986 B2 | 5/2007  | Diab                     |
| 6,597,932 B2 | 7/2003  | Tian et al.              | 7,221,971 B2 | 5/2007  | Diab                     |
| 6,597,933 B2 | 7/2003  | Kiani et al.             | 7,225,006 B2 | 5/2007  | Al-Ali et al.            |
| 6,606,511 B1 | 8/2003  | Ali et al.               | 7,225,007 B2 | 5/2007  | Al-Ali                   |
| 6,632,181 B2 | 10/2003 | Flaherty et al.          | RE39,672 E   | 6/2007  | Shehada et al.           |
| 6,639,668 B1 | 10/2003 | Trepagnier               | 7,239,905 B2 | 7/2007  | Kiani-Azarbayjany et al. |
| 6,640,116 B2 | 10/2003 | Diab                     | 7,245,953 B1 | 7/2007  | Parker                   |
| 6,643,530 B2 | 11/2003 | Diab et al.              | 7,254,429 B2 | 8/2007  | Schurman et al.          |
| 6,650,917 B2 | 11/2003 | Diab et al.              | 7,254,431 B2 | 8/2007  | Al-Ali                   |
| 6,654,624 B2 | 11/2003 | Diab et al.              | 7,254,433 B2 | 8/2007  | Diab et al.              |
| 6,658,276 B2 | 12/2003 | Kiani et al.             | 7,254,434 B2 | 8/2007  | Schulz et al.            |
| 6,661,161 B1 | 12/2003 | Lanzo et al.             | 7,272,425 B2 | 9/2007  | Al-Ali                   |
| 6,671,531 B2 | 12/2003 | Al-Ali et al.            | 7,274,955 B2 | 9/2007  | Kiani et al.             |
| 6,678,543 B2 | 1/2004  | Diab et al.              | D554,263 S   | 10/2007 | Al-Ali                   |
| 6,684,090 B2 | 1/2004  | Ali et al.               | 7,280,858 B2 | 10/2007 | Al-Ali et al.            |
| 6,684,091 B2 | 1/2004  | Parker                   | 7,289,835 B2 | 10/2007 | Mansfield et al.         |
| 6,697,656 B1 | 2/2004  | Al-Ali                   | 7,292,883 B2 | 11/2007 | De Felice et al.         |
| 6,697,657 B1 | 2/2004  | Shehada et al.           | 7,295,866 B2 | 11/2007 | Al-Ali                   |
| 6,697,658 B2 | 2/2004  | Al-Ali                   | 7,328,053 B1 | 2/2008  | Diab et al.              |
| RE38,476 E   | 3/2004  | Diab et al.              | 7,332,784 B2 | 2/2008  | Mills et al.             |
| 6,699,194 B1 | 3/2004  | Diab et al.              | 7,340,287 B2 | 3/2008  | Mason et al.             |
| 6,704,007 B1 | 3/2004  | Clapper                  | 7,341,559 B2 | 3/2008  | Schulz et al.            |
| 6,714,804 B2 | 3/2004  | Al-Ali et al.            | 7,343,186 B2 | 3/2008  | Lamego et al.            |
| RE38,492 E   | 4/2004  | Diab et al.              | D566,282 S   | 4/2008  | Al-Ali et al.            |
| 6,721,582 B2 | 4/2004  | Trepagnier et al.        | 7,355,512 B1 | 4/2008  | Al-Ali                   |
| 6,721,585 B1 | 4/2004  | Parker                   | 7,356,365 B2 | 4/2008  | Schurman                 |
| 6,725,075 B2 | 4/2004  | Al-Ali                   | 7,371,981 B2 | 5/2008  | Abdul-Hafiz              |
| 6,728,560 B2 | 4/2004  | Kollias et al.           | 7,373,193 B2 | 5/2008  | Al-Ali et al.            |
| 6,735,459 B2 | 5/2004  | Parker                   | 7,373,194 B2 | 5/2008  | Weber et al.             |
| 6,745,060 B2 | 6/2004  | Diab et al.              | 7,376,453 B1 | 5/2008  | Diab et al.              |
| 6,760,607 B2 | 7/2004  | Al-Ali                   | 7,377,794 B2 | 5/2008  | Al Ali et al.            |
| 6,770,028 B1 | 8/2004  | Ali et al.               | 7,377,899 B2 | 5/2008  | Weber et al.             |
| 6,771,994 B2 | 8/2004  | Kiani et al.             | 7,383,070 B2 | 6/2008  | Diab et al.              |
| 6,792,300 B1 | 9/2004  | Diab et al.              | 7,415,297 B2 | 8/2008  | Al-Ali et al.            |
| 6,813,511 B2 | 11/2004 | Diab et al.              | 7,428,432 B2 | 9/2008  | Ali et al.               |
| 6,816,741 B2 | 11/2004 | Diab                     | 7,438,683 B2 | 10/2008 | Al-Ali et al.            |
| 6,822,564 B2 | 11/2004 | Al-Ali                   | 7,440,787 B2 | 10/2008 | Diab                     |
| 6,826,419 B2 | 11/2004 | Diab et al.              | 7,454,240 B2 | 11/2008 | Diab et al.              |
| 6,830,711 B2 | 12/2004 | Mills et al.             | 7,467,002 B2 | 12/2008 | Weber et al.             |
| 6,850,787 B2 | 2/2005  | Weber et al.             | 7,469,157 B2 | 12/2008 | Diab et al.              |
| 6,850,788 B2 | 2/2005  | Al-Ali                   | 7,471,969 B2 | 12/2008 | Diab et al.              |
| 6,852,083 B2 | 2/2005  | Caro et al.              | 7,471,971 B2 | 12/2008 | Diab et al.              |
| 6,861,639 B2 | 3/2005  | Al-Ali                   | 7,483,729 B2 | 1/2009  | Al-Ali et al.            |
| 6,898,452 B2 | 5/2005  | Al-Ali et al.            | 7,483,730 B2 | 1/2009  | Diab et al.              |
| 6,920,345 B2 | 7/2005  | Al-Ali et al.            | 7,489,958 B2 | 2/2009  | Diab et al.              |
| 6,931,268 B1 | 8/2005  | Kiani-Azarbayjany et al. | 7,496,391 B2 | 2/2009  | Diab et al.              |
| 6,934,570 B2 | 8/2005  | Kiani et al.             | 7,496,393 B2 | 2/2009  | Diab et al.              |
| 6,939,305 B2 | 9/2005  | Flaherty et al.          | D587,657 S   | 3/2009  | Al-Ali et al.            |
| 6,943,348 B1 | 9/2005  | Coffin, IV               | 7,499,741 B2 | 3/2009  | Diab et al.              |
| 6,950,687 B2 | 9/2005  | Al-Ali                   | 7,499,835 B2 | 3/2009  | Weber et al.             |
| 6,961,598 B2 | 11/2005 | Diab                     | 7,500,950 B2 | 3/2009  | Al-Ali et al.            |
| 6,970,792 B1 | 11/2005 | Diab                     | 7,509,154 B2 | 3/2009  | Diab et al.              |
| 6,979,812 B2 | 12/2005 | Al-Ali                   | 7,509,494 B2 | 3/2009  | Al-Ali                   |
| 6,985,764 B2 | 1/2006  | Mason et al.             | 7,510,849 B2 | 3/2009  | Schurman et al.          |
| 6,993,371 B2 | 1/2006  | Kiani et al.             | 7,526,328 B2 | 4/2009  | Diab et al.              |
| 6,996,427 B2 | 2/2006  | Ali et al.               | 7,530,942 B1 | 5/2009  | Diab                     |
| 6,999,904 B2 | 2/2006  | Weber et al.             | 7,530,949 B2 | 5/2009  | Al Ali et al.            |
| 7,003,338 B2 | 2/2006  | Weber et al.             | 7,530,955 B2 | 5/2009  | Diab et al.              |
| 7,003,339 B2 | 2/2006  | Diab et al.              | 7,563,110 B2 | 7/2009  | Al-Ali et al.            |
| 7,015,451 B2 | 3/2006  | Dalke et al.             | 7,596,398 B2 | 9/2009  | Al-Ali et al.            |
| 7,024,233 B2 | 4/2006  | Ali et al.               | 7,618,375 B2 | 11/2009 | Flaherty                 |
| 7,027,849 B2 | 4/2006  | Al-Ali                   | D606,659 S   | 12/2009 | Kiani et al.             |
| 7,030,749 B2 | 4/2006  | Al-Ali                   | 7,647,083 B2 | 1/2010  | Al-Ali et al.            |
| 7,039,449 B2 | 5/2006  | Al-Ali                   | D609,193 S   | 2/2010  | Al-Ali et al.            |
| 7,041,060 B2 | 5/2006  | Flaherty et al.          | D614,305 S   | 4/2010  | Al-Ali et al.            |
| 7,044,918 B2 | 5/2006  | Diab                     | RE41,317 E   | 5/2010  | Parker                   |
| 7,067,893 B2 | 6/2006  | Mills et al.             | 7,729,733 B2 | 6/2010  | Al-Ali et al.            |
|              |         |                          | 7,734,320 B2 | 6/2010  | Al-Ali                   |
|              |         |                          | 7,761,127 B2 | 7/2010  | Al-Ali et al.            |
|              |         |                          | 7,761,128 B2 | 7/2010  | Al-Ali et al.            |
|              |         |                          | 7,764,982 B2 | 7/2010  | Dalke et al.             |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|              |         |                          |              |         |                      |
|--------------|---------|--------------------------|--------------|---------|----------------------|
| D621,516 S   | 8/2010  | Kiani et al.             | 8,346,330 B2 | 1/2013  | Lamego               |
| 7,791,155 B2 | 9/2010  | Diab                     | 8,353,842 B2 | 1/2013  | Al-Ali et al.        |
| 7,801,581 B2 | 9/2010  | Diab                     | 8,355,766 B2 | 1/2013  | MacNeish, III et al. |
| 7,822,452 B2 | 10/2010 | Schurman et al.          | 8,359,080 B2 | 1/2013  | Diab et al.          |
| RE41,912 E   | 11/2010 | Parker                   | 8,364,223 B2 | 1/2013  | Al-Ali et al.        |
| 7,844,313 B2 | 11/2010 | Kiani et al.             | 8,364,226 B2 | 1/2013  | Diab et al.          |
| 7,844,314 B2 | 11/2010 | Al-Ali                   | 8,374,665 B2 | 2/2013  | Lamego               |
| 7,844,315 B2 | 11/2010 | Al-Ali                   | 8,385,995 B2 | 2/2013  | Al-Ali et al.        |
| 7,865,222 B2 | 1/2011  | Weber et al.             | 8,385,996 B2 | 2/2013  | Smith et al.         |
| 7,873,497 B2 | 1/2011  | Weber et al.             | 8,388,353 B2 | 3/2013  | Kiani et al.         |
| 7,880,606 B2 | 2/2011  | Al-Ali                   | 8,399,822 B2 | 3/2013  | Al-Ali               |
| 7,880,626 B2 | 2/2011  | Al-Ali et al.            | 8,401,602 B2 | 3/2013  | Kiani                |
| 7,891,355 B2 | 2/2011  | Al-Ali et al.            | 8,405,608 B2 | 3/2013  | Al-Ali et al.        |
| 7,894,868 B2 | 2/2011  | Al-Ali et al.            | 8,414,499 B2 | 4/2013  | Al-Ali et al.        |
| 7,899,507 B2 | 3/2011  | Al-Ali et al.            | 8,418,524 B2 | 4/2013  | Al-Ali               |
| 7,899,518 B2 | 3/2011  | Trepagnier et al.        | 8,423,106 B2 | 4/2013  | Lamego et al.        |
| 7,904,132 B2 | 3/2011  | Weber et al.             | 8,428,967 B2 | 4/2013  | Olsen et al.         |
| 7,909,772 B2 | 3/2011  | Popov et al.             | 8,430,817 B1 | 4/2013  | Al-Ali et al.        |
| 7,910,875 B2 | 3/2011  | Al-Ali                   | 8,437,825 B2 | 5/2013  | Dalvi et al.         |
| 7,919,713 B2 | 4/2011  | Al-Ali et al.            | 8,455,290 B2 | 6/2013  | Siskavich            |
| 7,937,128 B2 | 5/2011  | Al-Ali                   | 8,457,703 B2 | 6/2013  | Al-Ali               |
| 7,937,129 B2 | 5/2011  | Mason et al.             | 8,457,707 B2 | 6/2013  | Kiani                |
| 7,937,130 B2 | 5/2011  | Diab et al.              | 8,463,349 B2 | 6/2013  | Diab et al.          |
| 7,941,199 B2 | 5/2011  | Kiani                    | 8,466,286 B2 | 6/2013  | Bellot et al.        |
| 7,951,086 B2 | 5/2011  | Flaherty et al.          | 8,471,713 B2 | 6/2013  | Poeze et al.         |
| 7,957,780 B2 | 6/2011  | Lamego et al.            | 8,473,020 B2 | 6/2013  | Kiani et al.         |
| 7,962,188 B1 | 6/2011  | Kiani et al.             | 8,483,787 B2 | 7/2013  | Al-Ali et al.        |
| 7,962,190 B1 | 6/2011  | Diab et al.              | 8,489,364 B2 | 7/2013  | Weber et al.         |
| 7,976,472 B2 | 7/2011  | Kiani                    | 8,498,684 B2 | 7/2013  | Weber et al.         |
| 7,988,637 B2 | 8/2011  | Diab                     | 8,509,867 B2 | 8/2013  | Workman et al.       |
| 7,990,382 B2 | 8/2011  | Kiani                    | 8,515,509 B2 | 8/2013  | Bruinsma et al.      |
| 7,991,446 B2 | 8/2011  | Al-Ali et al.            | 8,523,781 B2 | 9/2013  | Al-Ali               |
| 8,000,761 B2 | 8/2011  | Al-Ali                   | 8,529,301 B2 | 9/2013  | Al-Ali et al.        |
| 8,008,088 B2 | 8/2011  | Bellott et al.           | 8,532,727 B2 | 9/2013  | Ali et al.           |
| RE42,753 E   | 9/2011  | Kiani-Azarbayjany et al. | 8,532,728 B2 | 9/2013  | Diab et al.          |
| 8,019,400 B2 | 9/2011  | Diab et al.              | D692,145 S   | 10/2013 | Al-Ali et al.        |
| 8,028,701 B2 | 10/2011 | Al-Ali et al.            | 8,547,209 B2 | 10/2013 | Kiani et al.         |
| 8,029,765 B2 | 10/2011 | Bellott et al.           | 8,548,548 B2 | 10/2013 | Al-Ali               |
| 8,036,728 B2 | 10/2011 | Diab et al.              | 8,548,549 B2 | 10/2013 | Schurman et al.      |
| 8,046,040 B2 | 10/2011 | Ali et al.               | 8,548,550 B2 | 10/2013 | Al-Ali et al.        |
| 8,046,041 B2 | 10/2011 | Diab et al.              | 8,560,032 B2 | 10/2013 | Al-Ali et al.        |
| 8,046,042 B2 | 10/2011 | Diab et al.              | 8,560,034 B1 | 10/2013 | Diab et al.          |
| 8,048,040 B2 | 11/2011 | Kiani                    | 8,570,167 B2 | 10/2013 | Al-Ali               |
| 8,050,728 B2 | 11/2011 | Al-Ali et al.            | 8,570,503 B2 | 10/2013 | Vo et al.            |
| RE43,169 E   | 2/2012  | Parker                   | 8,571,617 B2 | 10/2013 | Reichgott et al.     |
| 8,118,620 B2 | 2/2012  | Al-Ali et al.            | 8,571,618 B1 | 10/2013 | Lamego et al.        |
| 8,126,528 B2 | 2/2012  | Diab et al.              | 8,571,619 B2 | 10/2013 | Al-Ali et al.        |
| 8,128,572 B2 | 3/2012  | Diab et al.              | 8,584,345 B2 | 10/2013 | Al-Ali et al.        |
| 8,130,105 B2 | 3/2012  | Al-Ali et al.            | 8,577,431 B2 | 11/2013 | Lamego et al.        |
| 8,145,287 B2 | 3/2012  | Diab et al.              | 8,581,732 B2 | 11/2013 | Al-Ali et al.        |
| 8,150,487 B2 | 4/2012  | Diab et al.              | 8,588,880 B2 | 11/2013 | Abdul-Hafiz et al.   |
| 8,175,672 B2 | 5/2012  | Parker                   | 8,600,467 B2 | 12/2013 | Al-Ali et al.        |
| 8,180,420 B2 | 5/2012  | Diab et al.              | 8,606,342 B2 | 12/2013 | Diab                 |
| 8,182,443 B1 | 5/2012  | Kiani                    | 8,626,255 B2 | 1/2014  | Al-Ali et al.        |
| 8,185,180 B2 | 5/2012  | Diab et al.              | 8,630,691 B2 | 1/2014  | Lamego et al.        |
| 8,190,223 B2 | 5/2012  | Al-Ali et al.            | 8,634,889 B2 | 1/2014  | Al-Ali et al.        |
| 8,190,227 B2 | 5/2012  | Diab et al.              | 8,641,631 B2 | 2/2014  | Sierra et al.        |
| 8,203,438 B2 | 6/2012  | Kiani et al.             | 8,652,060 B2 | 2/2014  | Al-Ali               |
| 8,203,704 B2 | 6/2012  | Merritt et al.           | 8,663,107 B2 | 3/2014  | Kiani                |
| 8,224,411 B2 | 7/2012  | Al-Ali et al.            | 8,666,468 B1 | 3/2014  | Al-Ali               |
| 8,228,181 B2 | 7/2012  | Al-Ali                   | 8,667,967 B2 | 3/2014  | Al-Ali et al.        |
| 8,229,533 B2 | 7/2012  | Diab et al.              | 8,670,811 B2 | 3/2014  | O'Reilly             |
| 8,233,955 B2 | 7/2012  | Al-Ali et al.            | 8,670,814 B2 | 3/2014  | Diab et al.          |
| 8,244,325 B2 | 8/2012  | Al-Ali et al.            | 8,676,286 B2 | 3/2014  | Weber et al.         |
| 8,255,026 B1 | 8/2012  | Al-Ali                   | 8,682,407 B2 | 3/2014  | Al-Ali               |
| 8,255,027 B2 | 8/2012  | Al-Ali et al.            | RE44,823 E   | 4/2014  | Parker               |
| 8,255,028 B2 | 8/2012  | Al-Ali et al.            | RE44,875 E   | 4/2014  | Kiani et al.         |
| 8,260,577 B2 | 9/2012  | Weber et al.             | 8,690,799 B2 | 4/2014  | Telfort et al.       |
| 8,265,723 B1 | 9/2012  | McHale et al.            | 8,700,112 B2 | 4/2014  | Kiani                |
| 8,274,360 B2 | 9/2012  | Sampath et al.           | 8,702,627 B2 | 4/2014  | Telfort et al.       |
| 8,301,217 B2 | 10/2012 | Al-Ali et al.            | 8,706,179 B2 | 4/2014  | Parker               |
| 8,310,336 B2 | 11/2012 | Muhsin et al.            | 8,712,494 B1 | 4/2014  | MacNeish, III et al. |
| 8,315,683 B2 | 11/2012 | Al-Ali et al.            | 8,715,206 B2 | 5/2014  | Telfort et al.       |
| RE43,860 E   | 12/2012 | Parker                   | 8,718,735 B2 | 5/2014  | Lamego et al.        |
| 8,337,403 B2 | 12/2012 | Al-Ali et al.            | 8,718,737 B2 | 5/2014  | Diab et al.          |
|              |         |                          | 8,718,738 B2 | 5/2014  | Blank et al.         |
|              |         |                          | 8,720,249 B2 | 5/2014  | Al-Ali               |
|              |         |                          | 8,721,541 B2 | 5/2014  | Al-Ali et al.        |
|              |         |                          | 8,721,542 B2 | 5/2014  | Al-Ali et al.        |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|           |    |         |                    |           |    |         |                    |
|-----------|----|---------|--------------------|-----------|----|---------|--------------------|
| 8,723,677 | B1 | 5/2014  | Kiani              | 9,161,713 | B2 | 10/2015 | Al-Ali et al.      |
| 8,740,792 | B1 | 6/2014  | Kiani et al.       | 9,167,995 | B2 | 10/2015 | Lamego et al.      |
| 8,754,776 | B2 | 6/2014  | Poeze et al.       | 9,176,141 | B2 | 11/2015 | Al-Ali et al.      |
| 8,755,535 | B2 | 6/2014  | Telfort et al.     | 9,186,102 | B2 | 11/2015 | Bruinsma et al.    |
| 8,755,856 | B2 | 6/2014  | Diab et al.        | 9,192,312 | B2 | 11/2015 | Al-Ali             |
| 8,755,872 | B1 | 6/2014  | Marinow            | 9,192,329 | B2 | 11/2015 | Al-Ali             |
| 8,761,850 | B2 | 6/2014  | Lamego             | 9,192,351 | B1 | 11/2015 | Telfort et al.     |
| 8,764,671 | B2 | 7/2014  | Kiani              | 9,195,385 | B2 | 11/2015 | Al-Ali et al.      |
| 8,768,423 | B2 | 7/2014  | Shakespeare et al. | 9,211,072 | B2 | 12/2015 | Kiani              |
| 8,771,204 | B2 | 7/2014  | Telfort et al.     | 9,211,095 | B1 | 12/2015 | Al-Ali             |
| 8,777,634 | B2 | 7/2014  | Kiani et al.       | 9,218,454 | B2 | 12/2015 | Kiani et al.       |
| 8,781,543 | B2 | 7/2014  | Diab et al.        | 9,226,696 | B2 | 1/2016  | Kiani              |
| 8,781,544 | B2 | 7/2014  | Al-Ali et al.      | 9,241,662 | B2 | 1/2016  | Al-Ali et al.      |
| 8,781,549 | B2 | 7/2014  | Al-Ali et al.      | 9,245,668 | B1 | 1/2016  | Vo et al.          |
| 8,788,003 | B2 | 7/2014  | Schurman et al.    | 9,259,185 | B2 | 2/2016  | Abdul-Hafiz et al. |
| 8,790,268 | B2 | 7/2014  | Al-Ali             | 9,267,572 | B2 | 2/2016  | Barker et al.      |
| 8,801,613 | B2 | 8/2014  | Al-Ali et al.      | 9,277,880 | B2 | 3/2016  | Poeze et al.       |
| 8,821,397 | B2 | 9/2014  | Al-Ali et al.      | 9,289,167 | B2 | 3/2016  | Diab et al.        |
| 8,821,415 | B2 | 9/2014  | Al-Ali et al.      | 9,295,421 | B2 | 3/2016  | Kiani et al.       |
| 8,830,449 | B1 | 9/2014  | Lamego et al.      | 9,307,928 | B1 | 4/2016  | Al-Ali et al.      |
| 8,831,700 | B2 | 9/2014  | Schurman et al.    | 9,323,894 | B2 | 4/2016  | Kiani              |
| 8,840,549 | B2 | 9/2014  | Al-Ali et al.      | 9,326,712 | B1 | 5/2016  | Kiani              |
| 8,847,740 | B2 | 9/2014  | Kiani et al.       | 9,333,316 | B2 | 5/2016  | Kiani              |
| 8,849,365 | B2 | 9/2014  | Smith et al.       | 9,339,220 | B2 | 5/2016  | Lamego et al.      |
| 8,852,094 | B2 | 10/2014 | Al-Ali et al.      | 9,341,565 | B2 | 5/2016  | Lamego et al.      |
| 8,852,994 | B2 | 10/2014 | Wojtczuk et al.    | 9,351,673 | B2 | 5/2016  | Diab et al.        |
| 8,868,147 | B2 | 10/2014 | Stippick et al.    | 9,351,675 | B2 | 5/2016  | Al-Ali et al.      |
| 8,868,150 | B2 | 10/2014 | Al-Ali et al.      | 9,364,181 | B2 | 6/2016  | Kiani et al.       |
| 8,870,792 | B2 | 10/2014 | Al-Ali et al.      | 9,368,671 | B2 | 6/2016  | Wojtczuk et al.    |
| 8,886,271 | B2 | 11/2014 | Kiani et al.       | 9,370,325 | B2 | 6/2016  | Al-Ali et al.      |
| 8,888,539 | B2 | 11/2014 | Al-Ali et al.      | 9,370,326 | B2 | 6/2016  | McHale et al.      |
| 8,888,708 | B2 | 11/2014 | Diab et al.        | 9,370,335 | B2 | 6/2016  | Al-Ali et al.      |
| 8,892,180 | B2 | 11/2014 | Weber et al.       | 9,375,185 | B2 | 6/2016  | Ali et al.         |
| 8,897,847 | B2 | 11/2014 | Al-Ali             | 9,386,953 | B2 | 7/2016  | Al-Ali             |
| 8,909,310 | B2 | 12/2014 | Lamego et al.      | 9,386,961 | B2 | 7/2016  | Al-Ali et al.      |
| 8,911,377 | B2 | 12/2014 | Al-Ali             | 9,392,945 | B2 | 7/2016  | Al-Ali et al.      |
| 8,912,909 | B2 | 12/2014 | Al-Ali et al.      | 9,397,448 | B2 | 7/2016  | Al-Ali et al.      |
| 8,920,317 | B2 | 12/2014 | Al-Ali et al.      | 9,408,542 | B1 | 8/2016  | Kinast et al.      |
| 8,921,699 | B2 | 12/2014 | Al-Ali et al.      | 9,436,645 | B2 | 9/2016  | Al-Ali et al.      |
| 8,922,382 | B2 | 12/2014 | Al-Ali et al.      | 9,445,759 | B1 | 9/2016  | Lamego et al.      |
| 8,929,964 | B2 | 1/2015  | Al-Ali et al.      | 9,466,919 | B2 | 10/2016 | Kiani et al.       |
| 8,942,777 | B2 | 1/2015  | Diab et al.        | 9,474,474 | B2 | 10/2016 | Lamego et al.      |
| 8,948,834 | B2 | 2/2015  | Diab et al.        | 9,480,422 | B2 | 11/2016 | Al-Ali             |
| 8,948,835 | B2 | 2/2015  | Diab               | 9,480,435 | B2 | 11/2016 | Olsen              |
| 8,965,471 | B2 | 2/2015  | Lamego             | 9,492,110 | B2 | 11/2016 | Al-Ali et al.      |
| 8,983,564 | B2 | 3/2015  | Al-Ali             | 9,510,779 | B2 | 12/2016 | Poeze et al.       |
| 8,989,831 | B2 | 3/2015  | Al-Ali et al.      | 9,517,024 | B2 | 12/2016 | Kiani et al.       |
| 8,996,085 | B2 | 3/2015  | Kiani et al.       | 9,532,722 | B2 | 1/2017  | Lamego et al.      |
| 8,998,809 | B2 | 4/2015  | Kiani              | 9,538,949 | B2 | 1/2017  | Al-Ali et al.      |
| 9,028,429 | B2 | 5/2015  | Telfort et al.     | 9,538,980 | B2 | 1/2017  | Telfort et al.     |
| 9,037,207 | B2 | 5/2015  | Al-Ali et al.      | 9,549,696 | B2 | 1/2017  | Lamego et al.      |
| 9,060,721 | B2 | 6/2015  | Reichgott et al.   | 9,554,737 | B2 | 1/2017  | Schurman et al.    |
| 9,066,666 | B2 | 6/2015  | Kiani              | 9,560,996 | B2 | 2/2017  | Kiani              |
| 9,066,680 | B1 | 6/2015  | Al-Ali et al.      | 9,560,998 | B2 | 2/2017  | Al-Ali et al.      |
| 9,072,474 | B2 | 7/2015  | Al-Ali et al.      | 9,566,019 | B2 | 2/2017  | Al-Ali et al.      |
| 9,078,560 | B2 | 7/2015  | Schurman et al.    | 9,579,039 | B2 | 2/2017  | Jansen et al.      |
| 9,084,569 | B2 | 7/2015  | Weber et al.       | 9,591,975 | B2 | 3/2017  | Dalvi et al.       |
| 9,095,316 | B2 | 8/2015  | Welch et al.       | 9,622,692 | B2 | 4/2017  | Lamego et al.      |
| 9,106,038 | B2 | 8/2015  | Telfort et al.     | 9,622,693 | B2 | 4/2017  | Diab               |
| 9,107,625 | B2 | 8/2015  | Telfort et al.     | D788,312  | S  | 5/2017  | Al-Ali et al.      |
| 9,107,626 | B2 | 8/2015  | Al-Ali et al.      | 9,636,055 | B2 | 5/2017  | Al-Ali et al.      |
| 9,113,831 | B2 | 8/2015  | Al-Ali             | 9,636,056 | B2 | 5/2017  | Al-Ali             |
| 9,113,832 | B2 | 8/2015  | Al-Ali             | 9,649,054 | B2 | 5/2017  | Lamego et al.      |
| 9,119,595 | B2 | 9/2015  | Lamego             | 9,662,052 | B2 | 5/2017  | Al-Ali et al.      |
| 9,131,881 | B2 | 9/2015  | Diab et al.        | 9,668,679 | B2 | 6/2017  | Schurman et al.    |
| 9,131,882 | B2 | 9/2015  | Al-Ali et al.      | 9,668,680 | B2 | 6/2017  | Bruinsma et al.    |
| 9,131,883 | B2 | 9/2015  | Al-Ali             | 9,668,703 | B2 | 6/2017  | Al-Ali             |
| 9,131,917 | B2 | 9/2015  | Telfort et al.     | 9,675,286 | B2 | 6/2017  | Diab               |
| 9,138,180 | B1 | 9/2015  | Coverston et al.   | 9,687,160 | B2 | 6/2017  | Kiani              |
| 9,138,182 | B2 | 9/2015  | Al-Ali et al.      | 9,693,719 | B2 | 7/2017  | Al-Ali et al.      |
| 9,138,192 | B2 | 9/2015  | Weber et al.       | 9,693,737 | B2 | 7/2017  | Al-Ali             |
| 9,142,117 | B2 | 9/2015  | Muhsin et al.      | 9,697,928 | B2 | 7/2017  | Al-Ali et al.      |
| 9,153,112 | B1 | 10/2015 | Kiani et al.       | 9,717,425 | B2 | 8/2017  | Kiani et al.       |
| 9,153,121 | B2 | 10/2015 | Kiani et al.       | 9,717,458 | B2 | 8/2017  | Lamego et al.      |
| 9,161,696 | B2 | 10/2015 | Al-Ali et al.      | 9,724,016 | B1 | 8/2017  | Al-Ali et al.      |
|           |    |         |                    | 9,724,024 | B2 | 8/2017  | Al-Ali             |
|           |    |         |                    | 9,724,025 | B1 | 8/2017  | Kiani et al.       |
|           |    |         |                    | 9,730,640 | B2 | 8/2017  | Diab et al.        |
|           |    |         |                    | 9,743,887 | B2 | 8/2017  | Al-Ali et al.      |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

|                 |         |                    |                 |         |                    |
|-----------------|---------|--------------------|-----------------|---------|--------------------|
| 9,749,232 B2    | 8/2017  | Sampath et al.     | 2013/0243021 A1 | 9/2013  | Siskavich          |
| 9,750,442 B2    | 9/2017  | Olsen              | 2013/0253334 A1 | 9/2013  | Al-Ali et al.      |
| 9,750,443 B2    | 9/2017  | Smith et al.       | 2013/0274571 A1 | 10/2013 | Diab et al.        |
| 9,750,461 B1    | 9/2017  | Telfort            | 2013/0296672 A1 | 11/2013 | O'Neil et al.      |
| 9,775,545 B2    | 10/2017 | Al-Ali et al.      | 2013/0317370 A1 | 11/2013 | Dalvi et al.       |
| 9,775,546 B2    | 10/2017 | Diab et al.        | 2013/0324808 A1 | 12/2013 | Al-Ali et al.      |
| 9,775,570 B2    | 10/2017 | Al-Ali             | 2013/0331670 A1 | 12/2013 | Kiani              |
| 9,778,079 B1    | 10/2017 | Al-Ali et al.      | 2013/0338461 A1 | 12/2013 | Lamego et al.      |
| 9,782,077 B2    | 10/2017 | Lamego et al.      | 2014/0012100 A1 | 1/2014  | Al-Ali et al.      |
| 9,782,110 B2    | 10/2017 | Kiani              | 2014/0025306 A1 | 1/2014  | Weber et al.       |
| 9,787,568 B2    | 10/2017 | Lamego et al.      | 2014/0034353 A1 | 2/2014  | Al-Ali et al.      |
| 9,788,735 B2    | 10/2017 | Al-Ali             | 2014/0051952 A1 | 2/2014  | Reichgott et al.   |
| 9,788,768 B2    | 10/2017 | Al-Ali et al.      | 2014/0051953 A1 | 2/2014  | Lamego et al.      |
| 9,795,300 B2    | 10/2017 | Al-Ali             | 2014/0051954 A1 | 2/2014  | Al-Ali et al.      |
| 9,795,310 B2    | 10/2017 | Al-Ali             | 2014/0058230 A1 | 2/2014  | Abdul-Hafiz et al. |
| 9,795,358 B2    | 10/2017 | Telfort et al.     | 2014/0066783 A1 | 3/2014  | Kiani et al.       |
| 9,795,739 B2    | 10/2017 | Al-Ali et al.      | 2014/0077956 A1 | 3/2014  | Sampath et al.     |
| 9,801,556 B2    | 10/2017 | Kiani              | 2014/0081100 A1 | 3/2014  | Muhsin et al.      |
| 9,801,588 B2    | 10/2017 | Weber et al.       | 2014/0081175 A1 | 3/2014  | Telfort            |
| 9,808,188 B1    | 11/2017 | Perea et al.       | 2014/0094667 A1 | 4/2014  | Schurman et al.    |
| 9,814,418 B2    | 11/2017 | Weber et al.       | 2014/0100434 A1 | 4/2014  | Diab et al.        |
| 9,820,691 B2    | 11/2017 | Kiani              | 2014/0114199 A1 | 4/2014  | Lamego et al.      |
| 9,833,152 B2    | 12/2017 | Kiani et al.       | 2014/0120564 A1 | 5/2014  | Workman et al.     |
| 9,833,180 B2    | 12/2017 | Shakespeare et al. | 2014/0121482 A1 | 5/2014  | Merritt et al.     |
| 9,839,379 B2    | 12/2017 | Al-Ali et al.      | 2014/0121483 A1 | 5/2014  | Kiani              |
| 9,839,381 B1    | 12/2017 | Weber et al.       | 2014/0125495 A1 | 5/2014  | Al-Ali             |
| 2002/0140675 A1 | 10/2002 | Al-Ali et al.      | 2014/0127137 A1 | 5/2014  | Bellott et al.     |
| 2002/0161291 A1 | 10/2002 | Kiani et al.       | 2014/0128696 A1 | 5/2014  | Al-Ali             |
| 2003/0197679 A1 | 10/2003 | Al-Ali et al.      | 2014/0128699 A1 | 5/2014  | Al-Ali et al.      |
| 2005/0065417 A1 | 3/2005  | Al-Ali et al.      | 2014/0129702 A1 | 5/2014  | Lamego et al.      |
| 2006/0258926 A1 | 11/2006 | Al-Ali et al.      | 2014/0135588 A1 | 5/2014  | Al-Ali et al.      |
| 2008/0030468 A1 | 2/2008  | Al-Ali et al.      | 2014/0142401 A1 | 5/2014  | Al-Ali et al.      |
| 2009/0076400 A1 | 3/2009  | Diab et al.        | 2014/0142402 A1 | 5/2014  | Al-Ali et al.      |
| 2009/0099430 A1 | 4/2009  | Diab et al.        | 2014/0163344 A1 | 6/2014  | Al-Ali             |
| 2009/0182211 A1 | 7/2009  | Diab et al.        | 2014/0163402 A1 | 6/2014  | Lamego et al.      |
| 2009/0247924 A1 | 10/2009 | Lamego et al.      | 2014/0166076 A1 | 6/2014  | Kiani et al.       |
| 2009/0275844 A1 | 11/2009 | Al-Ali             | 2014/0171763 A1 | 6/2014  | Diab               |
| 2009/0299157 A1 | 12/2009 | Telfort et al.     | 2014/0180038 A1 | 6/2014  | Kiani              |
| 2010/0004518 A1 | 1/2010  | Vo et al.          | 2014/0180154 A1 | 6/2014  | Sierra et al.      |
| 2010/0030040 A1 | 2/2010  | Poeze et al.       | 2014/0194709 A1 | 7/2014  | Al-Ali et al.      |
| 2010/0261979 A1 | 10/2010 | Kiani              | 2014/0194711 A1 | 7/2014  | Al-Ali             |
| 2011/0001605 A1 | 1/2011  | Kiani et al.       | 2014/0194766 A1 | 7/2014  | Al-Ali et al.      |
| 2011/0082711 A1 | 4/2011  | Poeze et al.       | 2014/0200420 A1 | 7/2014  | Al-Ali             |
| 2011/0105854 A1 | 5/2011  | Kiani et al.       | 2014/0200422 A1 | 7/2014  | Weber et al.       |
| 2011/0208015 A1 | 8/2011  | Welch et al.       | 2014/0206963 A1 | 7/2014  | Al-Ali             |
| 2011/0209915 A1 | 9/2011  | Telfort et al.     | 2014/0213864 A1 | 7/2014  | Abdul-Hafiz et al. |
| 2011/0213212 A1 | 9/2011  | Al-Ali             | 2014/0243627 A1 | 8/2014  | Diab et al.        |
| 2011/0230733 A1 | 9/2011  | Al-Ali             | 2014/0266790 A1 | 9/2014  | Al-Ali et al.      |
| 2011/0237911 A1 | 9/2011  | Lamego et al.      | 2014/0275808 A1 | 9/2014  | Poeze et al.       |
| 2011/0288384 A1 | 11/2011 | Ali et al.         | 2014/0275835 A1 | 9/2014  | Lamego et al.      |
| 2012/0059267 A1 | 3/2012  | Lamego et al.      | 2014/0275871 A1 | 9/2014  | Lamego et al.      |
| 2012/0116175 A1 | 5/2012  | Al-Ali et al.      | 2014/0275872 A1 | 9/2014  | Merritt et al.     |
| 2012/0179006 A1 | 7/2012  | Jansen et al.      | 2014/0275881 A1 | 9/2014  | Lamego et al.      |
| 2012/0209082 A1 | 8/2012  | Al-Ali             | 2014/0288400 A1 | 9/2014  | Diab et al.        |
| 2012/0209084 A1 | 8/2012  | Olsen et al.       | 2014/0296664 A1 | 10/2014 | Bruinsma et al.    |
| 2012/0227739 A1 | 9/2012  | Kiani              | 2014/0303520 A1 | 10/2014 | Telfort et al.     |
| 2012/0265039 A1 | 10/2012 | Kiani              | 2014/0309506 A1 | 10/2014 | Lamego et al.      |
| 2012/0283524 A1 | 11/2012 | Kiani et al.       | 2014/0309559 A1 | 10/2014 | Telfort et al.     |
| 2012/0286955 A1 | 11/2012 | Welch et al.       | 2014/0316228 A1 | 10/2014 | Blank et al.       |
| 2012/0296178 A1 | 11/2012 | Lamego et al.      | 2014/0323825 A1 | 10/2014 | Al-Ali et al.      |
| 2012/0319816 A1 | 12/2012 | Al-Ali             | 2014/0330092 A1 | 11/2014 | Al-Ali et al.      |
| 2012/0330112 A1 | 12/2012 | Lamego et al.      | 2014/0330098 A1 | 11/2014 | Merritt et al.     |
| 2013/0023775 A1 | 1/2013  | Lamego et al.      | 2014/0330099 A1 | 11/2014 | Al-Ali et al.      |
| 2013/0045685 A1 | 2/2013  | Kiani              | 2014/0333440 A1 | 11/2014 | Kiani              |
| 2013/0046204 A1 | 2/2013  | Lamego et al.      | 2014/0336481 A1 | 11/2014 | Shakespeare et al. |
| 2013/0041591 A1 | 3/2013  | Lamego             | 2014/0343436 A1 | 11/2014 | Kiani              |
| 2013/0060108 A1 | 3/2013  | Schurman et al.    | 2014/0357966 A1 | 12/2014 | Al-Ali et al.      |
| 2013/0060147 A1 | 3/2013  | Welch et al.       | 2015/0005600 A1 | 1/2015  | Blank et al.       |
| 2013/0096405 A1 | 4/2013  | Garfio             | 2015/0011907 A1 | 1/2015  | Purdon et al.      |
| 2013/0096936 A1 | 4/2013  | Sampath et al.     | 2015/0012231 A1 | 1/2015  | Poeze et al.       |
| 2013/0109935 A1 | 5/2013  | Al-Ali et al.      | 2015/0018650 A1 | 1/2015  | Al-Ali et al.      |
| 2013/0162433 A1 | 6/2013  | Muhsin et al.      | 2015/0032029 A1 | 1/2015  | Al-Ali et al.      |
| 2013/0190581 A1 | 7/2013  | Al-Ali et al.      | 2015/0038859 A1 | 2/2015  | Dalvi et al.       |
| 2013/0197328 A1 | 8/2013  | Diab et al.        | 2015/0045637 A1 | 2/2015  | Dalvi              |
| 2013/0211214 A1 | 8/2013  | Olsen              | 2015/0080754 A1 | 3/2015  | Purdon et al.      |
|                 |         |                    | 2015/0087936 A1 | 3/2015  | Al-Ali et al.      |
|                 |         |                    | 2015/0094546 A1 | 4/2015  | Al-Ali             |
|                 |         |                    | 2015/0097701 A1 | 4/2015  | Al-Ali et al.      |
|                 |         |                    | 2015/0099950 A1 | 4/2015  | Al-Ali et al.      |

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2015/0099955 A1 4/2015 Al-Ali et al.  
 2015/0101844 A1 4/2015 Al-Ali et al.  
 2015/0106121 A1 4/2015 Muhsin et al.  
 2015/0112151 A1 4/2015 Muhsin et al.  
 2015/0116076 A1 4/2015 Al-Ali et al.  
 2015/0126830 A1 5/2015 Schurman et al.  
 2015/0165312 A1 6/2015 Kiani  
 2015/0196237 A1 7/2015 Lamego  
 2015/0196249 A1 7/2015 Brown et al.  
 2015/0216459 A1 8/2015 Al-Ali et al.  
 2015/0230755 A1 8/2015 Al-Ali et al.  
 2015/0238722 A1 8/2015 Al-Ali  
 2015/0245773 A1 9/2015 Lamego et al.  
 2015/0245794 A1 9/2015 Al-Ali  
 2015/0257689 A1 9/2015 Al-Ali et al.  
 2015/0272514 A1 10/2015 Kiani et al.  
 2015/0351697 A1 12/2015 Weber et al.  
 2015/0351704 A1 12/2015 Kiani et al.  
 2015/0359429 A1 12/2015 Al-Ali et al.  
 2015/0366507 A1 12/2015 Blank  
 2015/0380875 A1 12/2015 Coverston et al.  
 2016/0029932 A1 2/2016 Al-Ali  
 2016/0051205 A1 2/2016 Al-Ali et al.  
 2016/0058347 A1 3/2016 Reichgott et al.  
 2016/0066823 A1 3/2016 Al-Ali et al.  
 2016/0066824 A1 3/2016 Al-Ali et al.  
 2016/0072429 A1 3/2016 Kiani et al.  
 2016/0081552 A1 3/2016 Wojtczuk et al.  
 2016/0095543 A1 4/2016 Telfort et al.  
 2016/0095548 A1 4/2016 Al-Ali et al.  
 2016/0103598 A1 4/2016 Al-Ali et al.  
 2016/0143548 A1 5/2016 Al-Ali  
 2016/0166182 A1 6/2016 Al-Ali et al.  
 2016/0166183 A1 6/2016 Poeze et al.  
 2016/0192869 A1 7/2016 Kiani et al.  
 2016/0196388 A1 7/2016 Lamego  
 2016/0197436 A1 7/2016 Barker et al.  
 2016/0213281 A1 7/2016 Eckerbom et al.  
 2016/0228043 A1 8/2016 O'Neil et al.  
 2016/0233632 A1 8/2016 Scruggs et al.  
 2016/0234944 A1 8/2016 Schmidt et al.  
 2016/0270735 A1 9/2016 Diab et al.  
 2016/0283665 A1 9/2016 Sampath et al.  
 2016/0287090 A1 10/2016 Al-Ali et al.  
 2016/0287786 A1 10/2016 Kiani  
 2016/0296169 A1 10/2016 McHale et al.  
 2016/0310052 A1 10/2016 Al-Ali et al.  
 2016/0314260 A1 10/2016 Kiani  
 2016/0324486 A1 11/2016 Al-Ali et al.  
 2016/0324488 A1 11/2016 Olsen  
 2016/0327984 A1 11/2016 Al-Ali et al.  
 2016/0328528 A1 11/2016 Al-Ali et al.  
 2016/0331332 A1 11/2016 Al-Ali  
 2016/0367173 A1 12/2016 Dalvi et al.  
 2017/0000394 A1 1/2017 Al-Ali et al.  
 2017/0007134 A1 1/2017 Al-Ali et al.  
 2017/0007190 A1 1/2017 Al-Ali et al.  
 2017/0007198 A1 1/2017 Al-Ali et al.  
 2017/0014083 A1 1/2017 Diab et al.  
 2017/0014084 A1 1/2017 Al-Ali et al.  
 2017/0027456 A1 2/2017 Kinast et al.  
 2017/0042488 A1 2/2017 Muhsin  
 2017/0055851 A1 3/2017 Al-Ali  
 2017/0055882 A1 3/2017 Al-Ali et al.  
 2017/0055887 A1 3/2017 Al-Ali  
 2017/0055896 A1 3/2017 Al-Ali et al.  
 2017/0079594 A1 3/2017 Telfort et al.  
 2017/0086723 A1 3/2017 Al-Ali et al.  
 2017/0143281 A1 5/2017 Olsen  
 2017/0147774 A1 5/2017 Kiani  
 2017/0156620 A1 6/2017 Al-Ali et al.  
 2017/0173632 A1 6/2017 Al-Ali  
 2017/0187146 A1 6/2017 Kiani et al.  
 2017/0188919 A1 7/2017 Al-Ali et al.  
 2017/0196464 A1 7/2017 Jansen et al.

2017/0196470 A1 7/2017 Lamego et al.  
 2017/0202490 A1 7/2017 Al-Ali et al.  
 2017/0224231 A1 8/2017 Al-Ali  
 2017/0224262 A1 8/2017 Al-Ali  
 2017/0228516 A1 8/2017 Sampath et al.  
 2017/0245790 A1 8/2017 Al-Ali et al.  
 2017/0251974 A1 9/2017 Shreim et al.  
 2017/0251975 A1 9/2017 Shreim et al.  
 2017/0258403 A1 9/2017 Abdul-Hafiz et al.

## FOREIGN PATENT DOCUMENTS

EP 0601589 6/1994  
 EP 0 707 824 A2 4/1996  
 EP 0 707 825 A2 4/1996  
 EP 0 707 867 A2 4/1996  
 EP 0821911 2/1998  
 EP 1 460 516 A2 9/2004  
 JP 60-163633 8/1985  
 JP 62-8738 1/1987  
 JP 62-197032 8/1987  
 JP 2-55033 2/1990  
 JP 4-12736 1/1992  
 JP 4-176445 6/1992  
 JP 7-152553 6/1995  
 WO WO 87/00027 1/1987  
 WO WO 89/00024 A1 1/1989  
 WO WO 89/00061 1/1989  
 WO WO 94/24929 11/1994  
 WO WO 96/16591 6/1996  
 WO WO 97/08605 3/1997  
 WO WO 97/22293 6/1997  
 WO WO 98/11820 3/1998  
 WO WO 00/42911 7/2000  
 WO WO 0042911 7/2000  
 WO WO 00/64346 11/2000  
 WO WO 01/26232 A2 4/2001  
 WO WO 02/15781 A1 2/2002

## OTHER PUBLICATIONS

A.L. Ronald et al., "Continuous Collection of Pulse Oximetry Data: New, Inexpensive, Portable computerized Method", British Journal of Anaesthesia 1992,69:105-107.  
 Advertisement for MediSense Precision PCx Glucose Monitor, Sep. 1999.  
 British Journal of Anaesthesia, 1991, "The World's Most Advanced Pulse Oximetry System Just Became Even More Versatile," in 2 pages.  
 Chih-Lung Lin et al., "A Portable Monitor for Fetal Heart Rate and Uterine Contraction", IEEE Engineering in Medicine & Biology, Nov./Dec. 1997,80-84.  
 Comus International, 3 pages alleged to be downloaded and printed from the World Wide Web on Mar. 15, 2002.  
 Confidential Declaration of Michelle Armond in Support of MASIMO Corporation's Responsive Claim Construction Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böblingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 19, 2010 (Redacted).  
 Copending U.S. Appl. No. 09/641,542, filed Aug. 18, 2000, and pending claims.  
 Copending U.S. Appl. No. 10/076,860, filed Feb. 12, 2002, and pending claims. (now U.S. Pat. No. 6,658,276).  
 Copending U.S. Appl. No. 10/076,860, published on Oct. 31, 2002, as a U.S. Pub. No. US 2002/0161291 A1. (now U.S. Pat. No. 6,658,276).  
 Copending U.S. Appl. No. 10/153,263, filed May 21, 2002, and pending claims.  
 Copending U.S. Appl. No. 10/911,391 filed Aug. 3, 2004 (citing publication).  
 Copending U.S. Appl. No. 11/431,151, filed May 8, 2006 (citing publication).  
 Copending U.S. Appl. No. 12/039,704, filed Feb. 28, 2008.  
 Correll G. et al., "Evaluation of several blood glucose monitoring systems for whole blood glucose measurements at the point of care", 52nd Annual MCC Meeting, Jul. 23-27,2000, Abstract 20.

(56)

## References Cited

## OTHER PUBLICATIONS

- David J. Farrar et al., "Portable Pneumatic Biventricular Driver for the Thoratec Ventricular Assist Device", *ASAIO Journal* 1997, 43: M631-M634.
- Declaration of Perry D. Oldham in Support of MASIMO Corporation's Opening Claim Construction Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010).
- Declaration of Robert T. Stone in Support of Philips' Responsive Markman Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 15, 2010).
- Defendant/Counterclaim-Plaintiff Philips Electronics North America Corporation Answer to Masimo's Counterclaims, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) dated Aug. 3, 2009, pp. 1-23.
- Defendants' Answer and Philips Electronics North America Corporation's Amended Counterclaims to Masimo's First Amended Complaint, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) dated Apr. 21, 2010.
- European Patent Office Official Communication pursuant to Article 96(2) EPC, Application No. 01 962 370.1-2305, dated Jun. 28, 2007, in 4 pages.
- European Search Report, App. No. 09002646.9-2319, dated Nov. 17, 2010.
- European Search Report, App. No. 07021807.8-2310, dated Jul. 31, 2009 in 4 pages.
- Extended European Search Report and European Search Opinion for App. No. 07021807.8-2310, dated Oct. 21, 2009 in 10 pages.
- Extended European Search Report, App. No. 08012674.1-2310, dated Oct. 21, 2009 in 7 pages.
- HP Component Monitoring System, Parameter Information, Edition 7—vol. 2, printed in Jul. 1994, in 252 pages.
- HP Component Monitoring System, System Information, Edition 7—vol. 1, printed in Jul. 1994, in 252 pages.
- J.D.E. Van Suijlen et al., "New Trends in bedside blood glucose monitoring", *Ned Tijdschr Klin Chem* 2000, Apr. 6, 2000, vol. 25, No. 2.
- James H. Nichols, "Management of Point-of-Care Testing", *Blood Gas News*, Dec. 9, 1999, vol. 8, No. 2.
- Jing Bai et al., "Home Telemonitoring Framework Based on Integrated Functional Modules", *IEEE 2000, Proceedings of the 22nd Annual EMBS Int'l Conference*, Jul. 23-28, 2000, 778-781.
- M. Nakagawara and K. Yamakoshi, "A portable instrument for non-invasive monitoring of beat-by-beat cardiovascular haemodynamic parameters based on the volume-compensation and electrical-admittance method", *Med. Biol. Eng. Comput.*, 2000, vol. 38, 17-25.
- Mallinckrodt inc. v. Masimo Corp.*, 2004 U.S. Dist. LEXIS 28518 (C.D. Cal. Jul. 12, 2004).
- Mallinckrodt Product Catalog*, Jan. 18, 2000.
- Mallinckrodt, Inc. v. Masimo Corp.*, 147 Fed. Appx. 158, 2005 WL 2139867 (Fed. Cir. 2005).
- Mallinckrodt, Inc. v. Masimo Corp.*, 254 F. Supp.2d 1140 (C.D. Cal. 2003).
- Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) Complaint for Patent Infringement dated Feb. 3, 2009.
- Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) First Amended Complaint for Patent Infringement dated May 12, 2009.
- Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) Defendants' Answer and Philips Electronics North America Corporation's Counterclaims to Masimo's First Amended Complaint dated Jun. 15, 2009.
- Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) Masimo's Answer to Philips' Counterclaims dated Jul. 9, 2009.
- Masimo Corporation's Opening Claim Construction Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010).
- MASIMO Corporation's Responsive Claim Construction Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 19, 2010 (Redacted)).
- Masimo's Answer to Philips' Amended Counterclaims, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) dated May 10, 2010.
- MASIMO's Technical Tutorial, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010).
- Michael A.E. Schneider, et al., "Use of a Relational Database for Patient- and Data-Management in the Electrophysiologic Catheter Laboratory", *Computers in Cardiology* 1994, 513-515.
- N.D. Harris et al., "Can Changes in QT Interval be used to Predict the Onset of Hypoglycemia in Type 1 Diabetes?", *Computers in Cardiology* 2000; 27:375-278.
- P. Draycon, "Advanced technology in patient monitoring is expected to reduce costs", *Min Invas Ther & Allied Technol* 1997; 6: 308-309.
- Philips Electronics North America Corporation's Answer to Masimo's Amended Counterclaims, *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) dated May 27, 2010.
- Philips North America Corporation and Philips Medizin Systeme Böttingen GMBH's Seventh Supplemental Objections and Responses to Masimo Corporation's First Set of Interrogatories (Nos. 1-8), *Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 09-00080(JJF)) dated Jun. 30, 2010 (Redacted).
- Philips' Opening Markman Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010).
- Philips' Responsive Markman Brief, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Nov. 22, 2010).
- Philips' Claim Construction Hearing, Presentation Materials, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010).
- Report and Recommendation re Claim Construction, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Feb. 18, 2011).
- Revised Joint Claim Construction Chart, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GMBH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Oct. 19, 2010).
- S. Weber, "Remote network (Ethernet) connectivity for glucose testing at the point-of-care", 51st Annual MCC Conference, Jul. 25-29, 1999, Abstract 111.
- Service Manual, Nellcor Interface/Display Module, Model N-50, 1992, in 21 pages.
- Thoratec VADIVAD System Clinical Operation & Patient Management, 2004.
- Toshiyo Tamura et al., "A system for monitoring temperature distribution in bed and its application to the assessment of body movement", *Physiol. Meas.* 14 (1993) 33-41.



(56)

## References Cited

## OTHER PUBLICATIONS

Transcript of Markman Hearing, *MASIMO Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme Böttingen GmbH*, (District of Delaware, Case No. 1:09-cv-00080 (LPS/MPT) dated Dec. 1, 2010.

U.S. Appl. No. 09/491,175, filed Jan. 25, 2000, now abandoned.

U.S. Appl. No. 10/153,263, filed May 21, 2002 in 48 pages. (citing publication).

U.S. Appl. No. 10/420,994, filed Apr. 22, 2003 in 48 pages. (citing Patent).

U.S. Appl. No. 10/911,391, filed May 8, 2006 in 63 pages. (citing publication).

U.S. Appl. No. 11/431,151, filed May 8, 2006 in 49 pages. (citing publication).

U.S. Patent and Trademark Office Notice of Allowance, U.S. Appl. No. 09/516,110, dated Feb. 5, 2003, in 6 pages.

U.S. Patent and Trademark Office Notice of Allowance, U.S. Appl. No. 09/516,110, dated Sep. 11, 2002, in 9 pages. (citing Patent).

U.S. Patent and Trademark Office Notice of Allowance, U.S. Appl. No. 09/641,542, dated Mar. 24, 2004, in 4 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 09/641,542, dated May 14, 2003, in 9 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 09/641,542, dated Oct. 10, 2002, in 9 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 09/641,542, dated Oct. 16, 2003, in 7 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/153,263, dated Apr. 30, 2007, in 12 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/153,263, dated Nov. 1, 2005, in 8 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/153,263, dated Sep. 22, 2004, in 11 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/153,263, dated Oct. 5, 2006, in 12 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/420,994, dated Feb. 24, 2006, in 6 pages.

U.S. Patent and Trademark Office Office Action, U.S. Appl. No. 10/420,994, dated Oct. 18, 2006, in 7 pages.

[PHIL01959608-635] Ep 0601589 B1, dated Mar. 8, 2000, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03325092-115] Ep 0601589 A2, dated Jun. 15, 1994, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02874644-651] Hp M1032A VueLink External Device User's Booklet, 4th Edition; Feb. 1995, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02875566-654] Operator's Manual Edwards Critical-Care Division Vigilance, date unknown at this time, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02873755] Nellcor Interface/Display Module, Model N-50 Service Manual Cover p., dated 1992, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02873756-758] Nellcor N-50 Service Manual, Section 13 Specifications date unknown at this time, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02873264-270] Nellcor N-50, except from manual, continuation of Section 3 Circuit Analysis, date unknown at this time, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02873254-263] Nellcor N-50, except from manual, Section 3 Circuit Analysis, date unknown at this time, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03325124-182] Final Report - an Evaluation of Potential Gprs 900/1800 MHz and Wcdma 1900 MHz Interference to Medi-

cal Devices, prepared by Telstra Research Laboratories, dated Jun. 30, 2004, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL02875414-417] "Pulse Oximeters," date unknown at this time, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03328740-954] Nellcor Symphony@ N-3000 Pulse Oximeter Operator's Manual, dated 1997, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03329054-9125] Nellcor Symphony@ N-3100 Blood Pressure Monitor Operator's Manual, dated 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03328955-9053] Nellcor Symphony@ N-3100 Blood Pressure Monitor Service Manual, dated 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03329126-199] Nellcor Symphony@ N-3200 Display/Printer Service Manual, dated 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03328371-440] Nellcor@ N-250 Pulse Oximeter/Ecg Monitor Operator's Manual, dated 1990 and 1991, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03329200-252] Operator's Manual, Nellcor Symphony@ N-3200 Display/Printer, dated 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03325116-120] 501(k) Summary: "SatMaster," Computerized Pulse Oximetry Software, dated Aug. 5, 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[PHIL03329200-252] Operator's Manual, Nellcor Symphony@ N-3200 Display/Printer, dated 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000001-2] Document Production "Nellcor Inc.", San Francisco Business Times, available at <http://go.galegroup.com/ps/i.do?id=Gale%7CA6676224&v=2.1&u=rock21695&1t=r&p=1TOF&sw=w&a=sld=4e76da87ab0bc8f1a28d9b14341aa278>, dated Jul. 18, 1988, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000003] Document Production Internet Archive Wayback Machine; "Patient Safety Monitoring", downloaded from <http://web.archive.org/web/19980131205732/http://www.nellcorpb.com/html/porducts.html>, archived Jan. 31, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000004] Document Production Internet Archive Wayback Machine; "Product Information", downloaded from [http://web.archive.org/web/19980131210002/http://www.nellcorpb.com/html/patient\\_safety.html](http://web.archive.org/web/19980131210002/http://www.nellcorpb.com/html/patient_safety.html), archived Jan. 31, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000005] Document Production Internet Archive Wayback Machine; "Welcome to Nellcor Puritan Bennett", downloaded from <http://web.archive.org/web/19980131205602/http://www.nellcorpb.com/>, archived Jan. 31, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000006-7] Document Production Internet Archive Wayback Machine; "Mallinckrodt Home p.", downloaded from <http://web.archive.org/web/19980110085227/http://www.mallinckrodt.com>, archived Jan. 10, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000008 - 010] Document Production Internet Archive Wayback Machine; "Pulse Oximeter Sensors", downloaded from <http://web.archive.org/web/19980131210915/http://www.nellcorpb.com/html/sensors.html>, archived Jan. 31, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000011-12] Document Production Internet Archive Wayback Machine; "Pulse Oximeters & Multiparameter Monitors", downloaded from <http://web.archive.org/web/19980131210903/http://>

(56)

## References Cited

## OTHER PUBLICATIONS

www.nellcorpb.com/html/pulse\_oximeters.html, archived Jan. 31, 1998, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000013-14] Document Production “Nellcor Inc.”, San Francisco Business Times, available at <http://go.galegroup.com/ps/i.do?id=Gale%7CA6676224&v=2.1&u=rock21695&it=r&p=1TOF&sw=w&a.sld=4e76da87ab0bc8f1a28d9b14341aa278>, dated Jul. 18, 1988, retrieved Jan. 29, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000015-110] Document Production Hewlett-Packard Journal, Oct. 1991, vol. 42, Issue 4, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000116-121] Document Production 501(k) Summary for Nellcor Symphonytm N-3000 Patient Monitor, dated Aug. 26, 1996, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000122-126] Document Production 501(k) Summary for Npb-290 Pulse Oximeter, dated Jul. 30, 1997, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000127-132] Document Production 501(k) Summary for Npb-295 Pulse Oximeter, dated Aug. 22, 1997, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000133-135] Document Production “Mallinckrodt to Buy Maker of Medical Gear for \$1.8 Billion”, the New York Times, available at <http://www.nytimes.com/1997/07/24/business/mallinckrodt-to-buy-maker-of-medical-gear-for-1.8-billion.html>, dated Jul. 24, 1997, retrieved Feb. 3, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000136-140] Document Production “Masimo - News Archive - 1998”, available at <http://www.masimo.com/news/1998.htm>, dated Jan. 29, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000141-142] Document Production “Nellcor N-250” Advertisement, British Journal of Anaesthesia, dated 1991, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000143-145] Document Production “Nellcor reports second quarter results”, Business Wire, Inc., dated Jan. 12, 1995, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000146-148] Document Production “Nellcor Reports Record Fourth Quarter and Year-End Results”, Business Wire, Inc., dated Jul. 27, 1995, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000149-154] Document Production “Nellcor Puritan Bennett Releases Four New Products for Monitoring, Ventilation and Sleep Therapy.”, available at <http://www.thefreelibrary.com/Nellcor+Puritan+Bennett+Releases+Four+New+Products+for+Monitoring...a018526362>, dated Jul. 25, 1996, retrieved Feb. 2, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000155-259] Document Production of Annual Report for Fiscal Year, dated Jun. 28, 1987, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000260-339] Document Production of Annual Report for Fiscal Year, dated Jun. 26, 1988, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000340-400] Document Production of Annual Report for Fiscal Year, dated Jul. 2, 1989, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000401-468] Document Production “Patent Owner’s Preliminary Response” in Medtronic Plc v. Masimo Corporation, Case No. IPR2016-00057, dated Jan. 29, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000469-470] Document Production “Second-generation Symphony system is music to Nellcor’s ears.”, Health Industry Today, Aug. 1, 1995, vol. v58, Issue n8, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000471-540] Document Production entitled M1032A VueLink Module Handbook, Hewlett-Packard GmbH, dated Nov. 1992, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000541] Document Production entitled Cable Interface M1032-Nellcor N-100 C, dated Feb. 1, 1993, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000542] Document Production entitled Cable Interface M1032-Nellcor N-200, dated Jun. 24, 1993, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR000000543-570] Document Production entitled Hp M1032A VueLink External Device User’s Booklet, Hewlett-Packard GmbH, dated Nov. 1993, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

Expert Report of Dr. Joseph F. Dyro Regarding the Invalidity of U.S. Pat. No. 7,530,949, dated Feb. 12, 2016, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt, C.A. No. 11-742-Lps.

Appendices A-C, Expert Report of Dr. Joseph F. Dyro Regarding the Invalidity of U.S. Pat. No. 7,530,949, dated Feb. 12, 2016, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt.

Declaration of Ray Larkin Regarding the Nellcor Symphony, dated Feb. 10, 2016, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt.

Declaration of Robert T. Stone Regarding the Nellcor N-200, the Nellcor N-250, and the Nellcor Symphony, dated Feb. 9, 2016, pp. 1-415, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt.

Declaration of Robert T. Stone Regarding the Nellcor N-200, the Nellcor N-250, and the Nellcor Symphony, dated Feb. 9, 2016, pp. 416-831, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt.

Declaration of Robert T. Stone Regarding the Nellcor N-200, the Nellcor N-250, and the Nellcor Symphony, dated Feb. 9, 2016, pp. 832-1246, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, C.A. No. 09-80-Lps-Mpt.

Complaint, dated Mar. 4, 2016, Masimo Corporation v. Philips Electronics North America Corporation and Philips Medizin Systeme BOblingen GmbH, Case No. 1:16-cv-00137-Lps.

2016-04-29 Reply Expert Report of Timothy J. Quill, M.D., Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.).

2016-04-29 Reply Expert Report of Professor James McNames Concerning the Infringement of U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.).

2016-07-05 Demand for Jury Trial, Masimo Corporation’s Opening Brief in Support of Its Motions for Summary Judgment and to Exclude Portions of the Testimony of Michael Keeley, Joseph Dyro, and Bryan Bergeron, Public Version Released Jul. 5, 2016, Doc. 1259, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

(56)

**References Cited****OTHER PUBLICATIONS**

2016-07-05 Demand for Jury Trial, Declaration of James McNames, Ph.D. In Support of Masimo Corporation's Motion for Summary Judgment of Infringement as to the '949 Patent, Public Version Released Jul. 5, 2016, Doc. 1260, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-07-06 Jury Trial Demanded, Philips Opening Brief in Support of Defendants' Motions for Summary Judgment, Public Version Released Jul. 6, 2016, Doc. 1263, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-07-28 Jury Trial Demanded, Defendants' Opposition to Plaintiff Masimo Corporation's Opening Brief in Support of Its Motions for Summary Judgment and to Exclude Portions of the Testimony of Michael Keeley, Joseph Dyro, and Bryan Bergeron, Public Version Released Jul. 28, 2016, Doc. 1291, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-02-12 Expert Report of Professor James McNames, Ph.D. Concerning Infringement of Masimo's U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-04-29 Reply Expert Report of Professor James McNames, Ph.D. Concerning Infringement of U.S. Pat. No. 7,530,949 Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-02-12 Expert Report of Dr. Joseph F. Dyro Regarding the Invalidity of U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-03-28 Rebuttal Expert Report of Professor James McNames, Ph.D. Concerning Validity of Masimo's U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-03-28 Rebuttal Expert Report of Dr. Joseph F. Dyro Regarding the Non-Infringement of U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-04-29 Reply Expert Report of Dr. Joseph F. Dyro Regarding the Invalidity of U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-04-29 Disclosure of Joe Kiani Pursuant to Fed. R. Civ. P. 26(a)(2)(C) and the Court's Request of Apr. 14, 2016, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-04-29 Reply Expert Report of Professor James McNames Concerning the Infringement of U.S. Pat. No. 7,530,949, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-04-29, Reply Expert Report of Timothy J. Quill, M.D., Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

Excerpted 2016-07-05 Demand for Jury Trial, Declaration of Michael C. Lee. In Support of Masimo Corporation's Motion for Summary Judgment and to Exclude Portions of the Testimony of Michael Keeley, Joseph Dyro, and Bryan Bergeron, Public Version Released Jul. 5, 2016, Doc. 1261, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

Excerpted 2016-07-28 Jury Trial Demanded, Appendix of Exhibits of Defendants' Opposition to Plaintiff Masimo Corporation's Opening Brief in Support of Its Motions for Summary Judgment and to Exclude Portions of the Testimony of Michael Keeley, Joseph Dyro, and Bryan Bergeron Exhibits 55-83, Public Version Released Jul. 28, 2016, Doc. 1292, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

Excerpted 2016-07-29 Demand for Jury Trial, Masimo Corporation's Compendium of Exhibits in Support of Its Opposition to Defendant's Motion for Summary Judgment Exhibits 1-73, Public Version Released Jul. 29, 2016, Doc. 1295-1, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-07-29 Demand for Jury Trial, Masimo Corporation's Opposition to Defendant's Motion for Summary Judgment, Public Version Released Jul. 29, 2016, Doc. 1294, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-08-25 Jury Trial Demanded, Reply Brief of in Support of Defendants' Motions for Summary Judgment, Public Version Released Aug. 25, 2016, Doc. 1306, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

2016-08-26 Demand for Jury Trial, Masimo Corporation's Reply Brief in Support of Its Motion for Summary Judgment and to Exclude Portions of the Testimony of Michael Keeley, Joseph Dyro, and Bryan Bergeron, Public Version Released Aug. 26, 2016, Doc. 1311, Masimo Corp. v. Philips Elecs. North America Corp. et al., No. 1:09-cv-00080-Lps-Mpt, 1:11-cv-00742-Lps-Mpt (D. Del.). (Redacted).

[DYR00000571-572] Document Production entitled Double, double, toil and trouble, dated Mar. 12, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000573-576] Document Production entitled Microprocessor Hall of Fame, dated Apr. 27, 2016, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000577-583] Document Production of 501(k) Summary for Model 2000 Pulse Oximeter, dated Oct. 22, 1998, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000584-585] Document Production entitled Capnography Providing the ultimate sidestream performance along with cost-effective disposables, Copyright 2014, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000586-588] Document Production of Roget's Thesaurus (selected portions), Third Edition, Copyright as early as 1975, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000589-592] Document Production of Communications Standard Dictionary (selected portions), Third Edition, dated Jan. 30, 1996, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000593-852] Document Production of Operator's Manual, Dash 2000 Patient Monitor Software Version 2, Copyright 1999, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000853-947] Document Production of Service Manual, Dash 2000 Patient Monitor Software Version 3, Copyright as early as 2001, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000948-951] Document Production of Health Devices (selected portions), dated Jun. 1989, vol. 18, Issue 6, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000952-958] Document Production of Health Devices (selected portions), dated Mar./Apr. 1991, vol. 20, Nos. 3-4, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000959-962] Document Production of Joseph J. Carr and John M. Brown, Chapter 7 (selected portions), Introduction to Biomedical Equipment Technology, Third Edition, Copyright as early as 1981, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000963-966] Document Production of 501(k) Summary for Lifesignstm Cardiac Monitoring System, dated Jul. 23, 1997, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

(56)


**References Cited**

OTHER PUBLICATIONS

[DYR00000967-971] Document Production of Webster, Chapter 14 (selected portions), Medical Instrumentation Application and Design, Second Edition, Copyright 1992, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000972-974] Document Production of 501 (k) Summary for Siemens Sc 6000 & Sc 6000 p. Portable Bedside Monitoring System, dated Jan. 17, 1997, Masimo Corporation v. Philips Electronics North America Corporation, et al., Case No. 1:09-cv-00080-Lps.

[DYR00000975-1121] Document Production of Service Manual, Siemens Sc 9000 Patient Monitors, Copyright 1996, Masimo Corporation v. Philips Electronics North American Corporation, et al., Case No. 1:09-cv-00080-Lps.

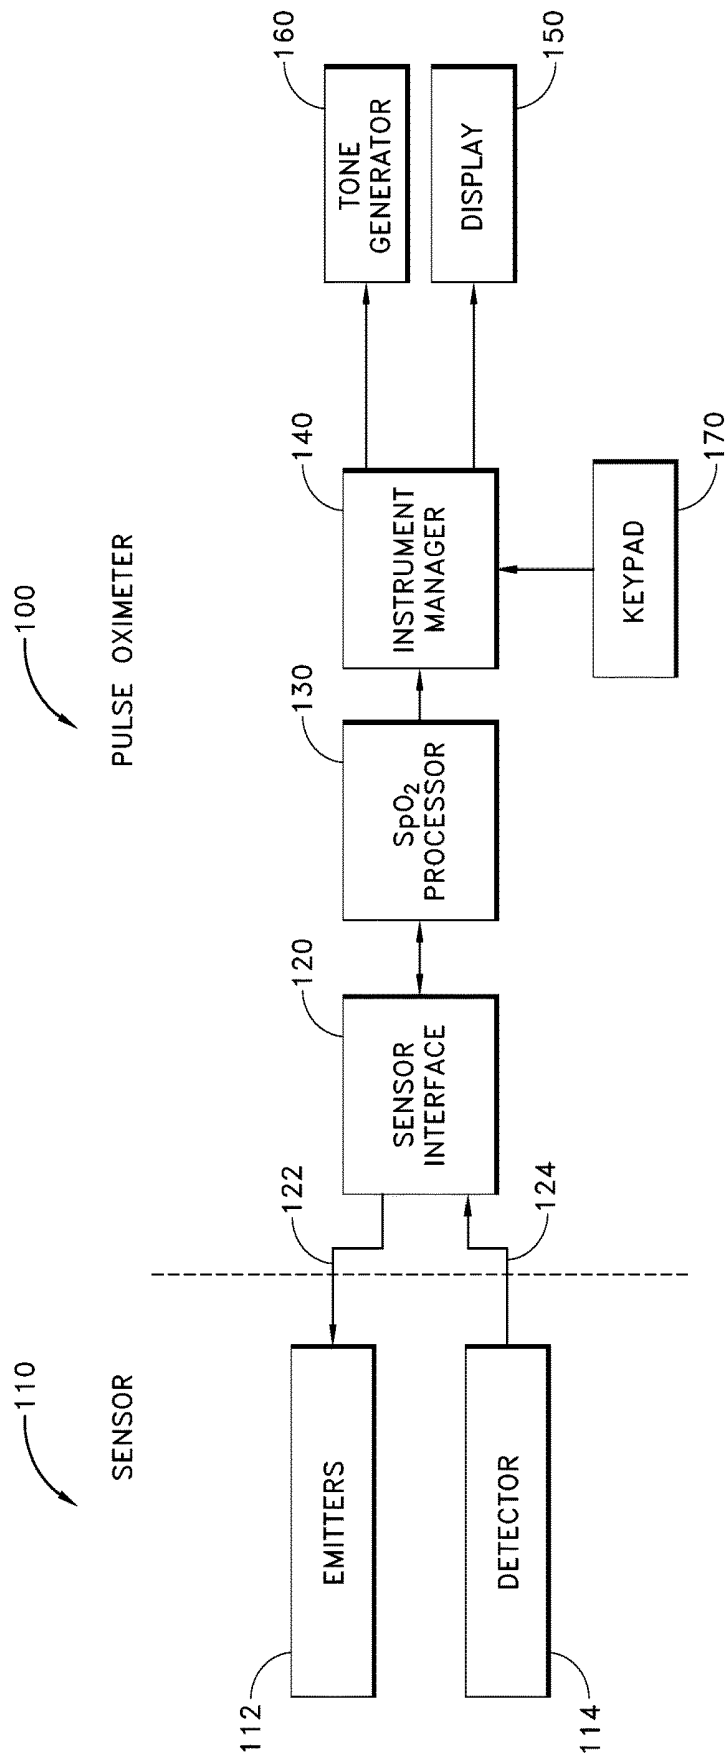

*FIG. 1*  
(PRIOR ART)

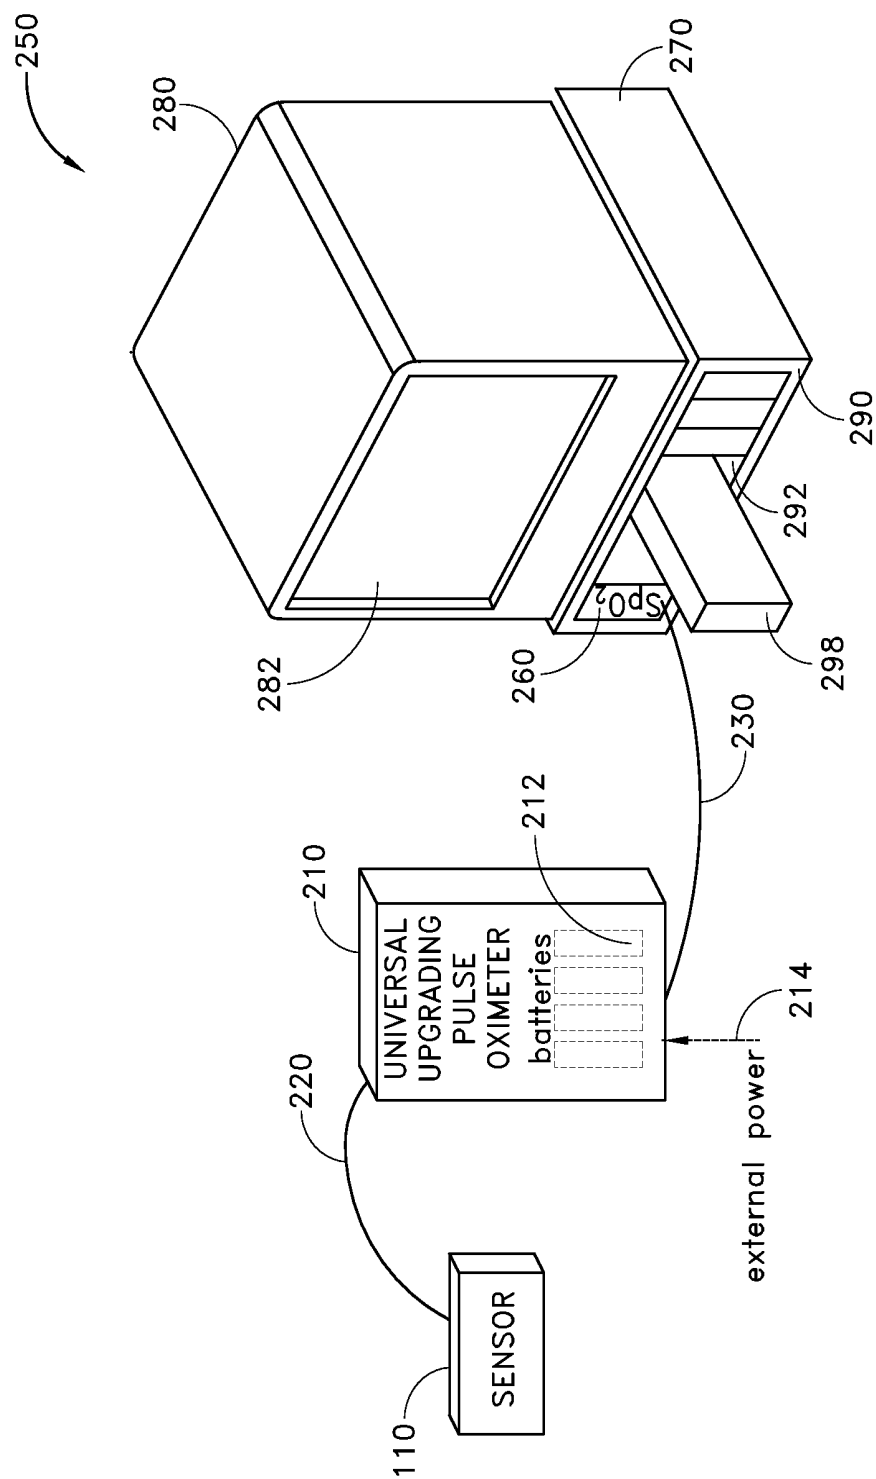


FIG. 2

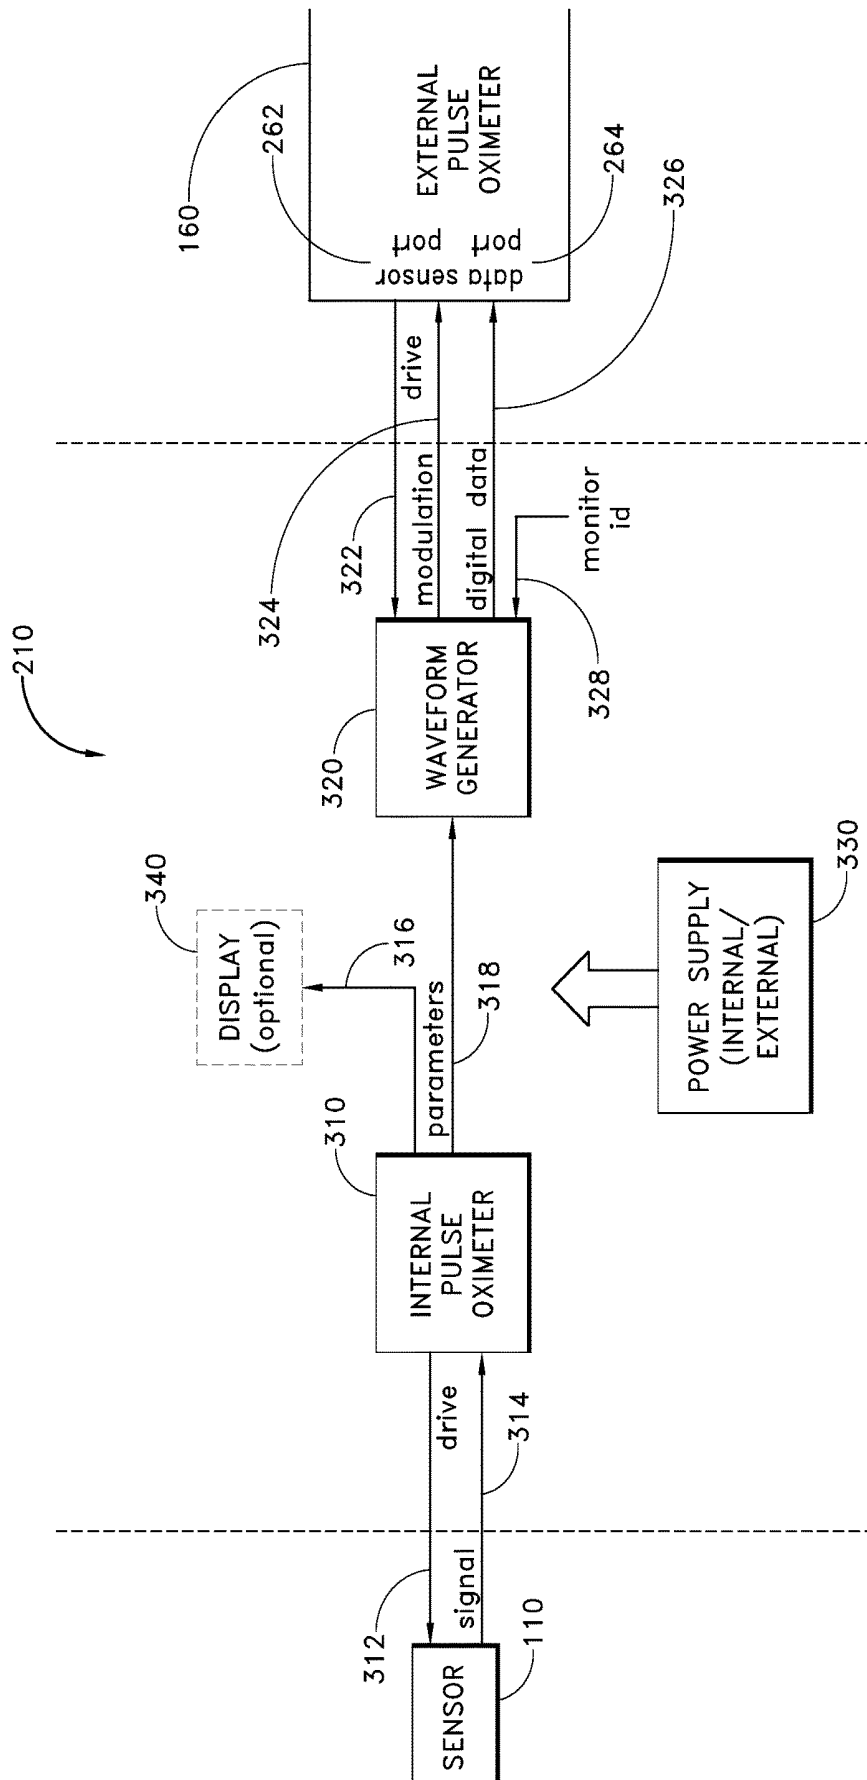


FIG. 3

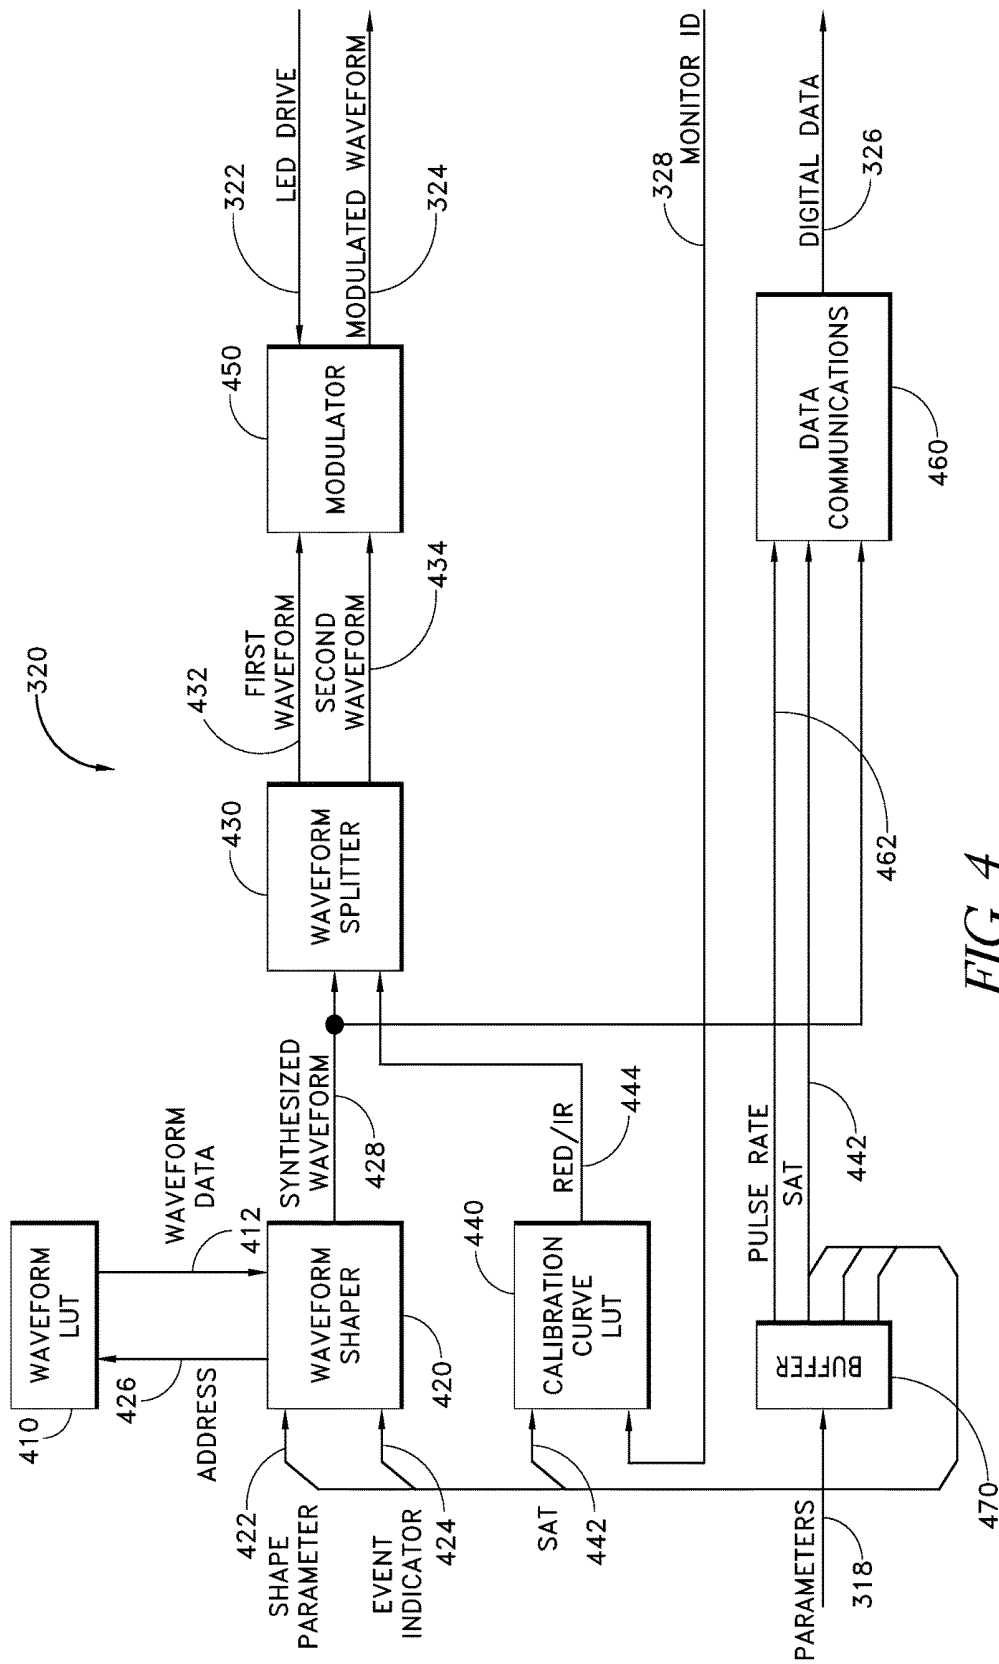


FIG. 4



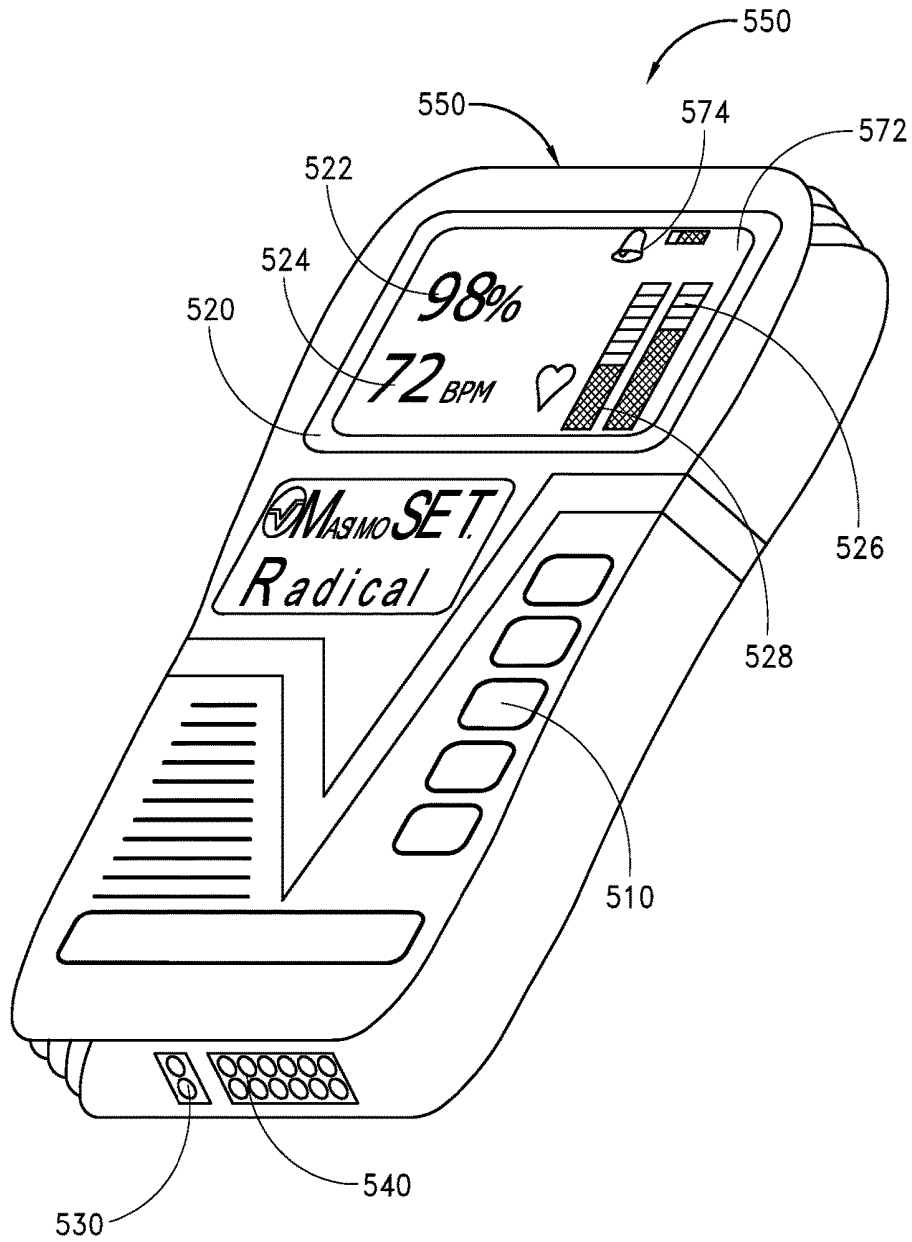


FIG. 5

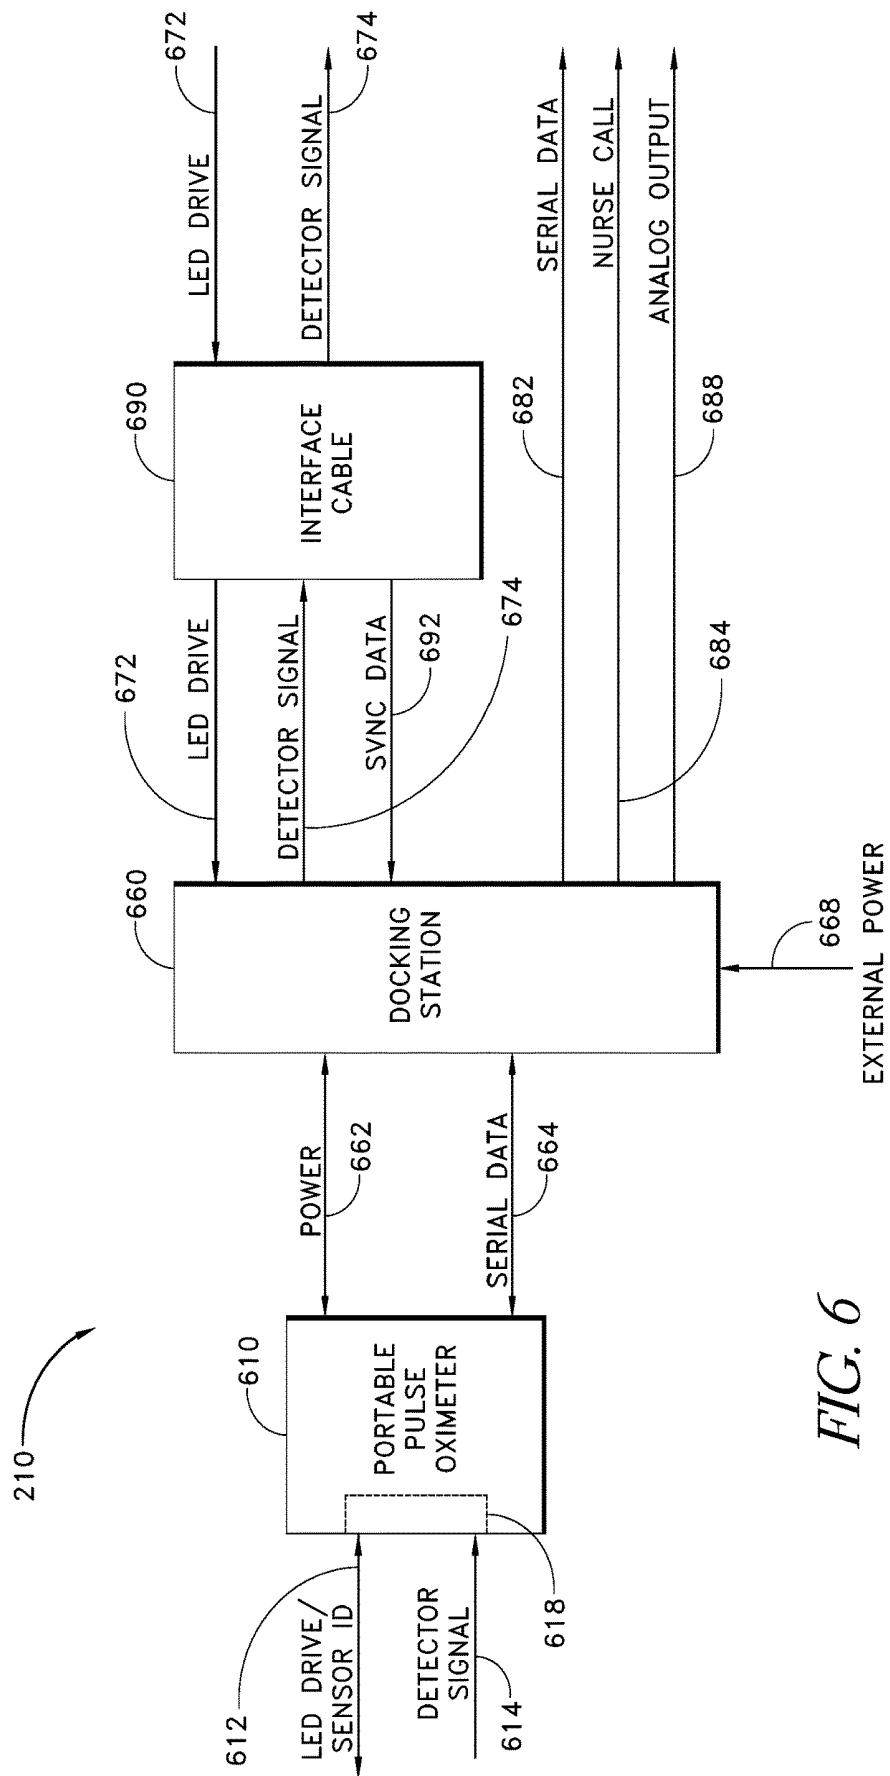


FIG. 6

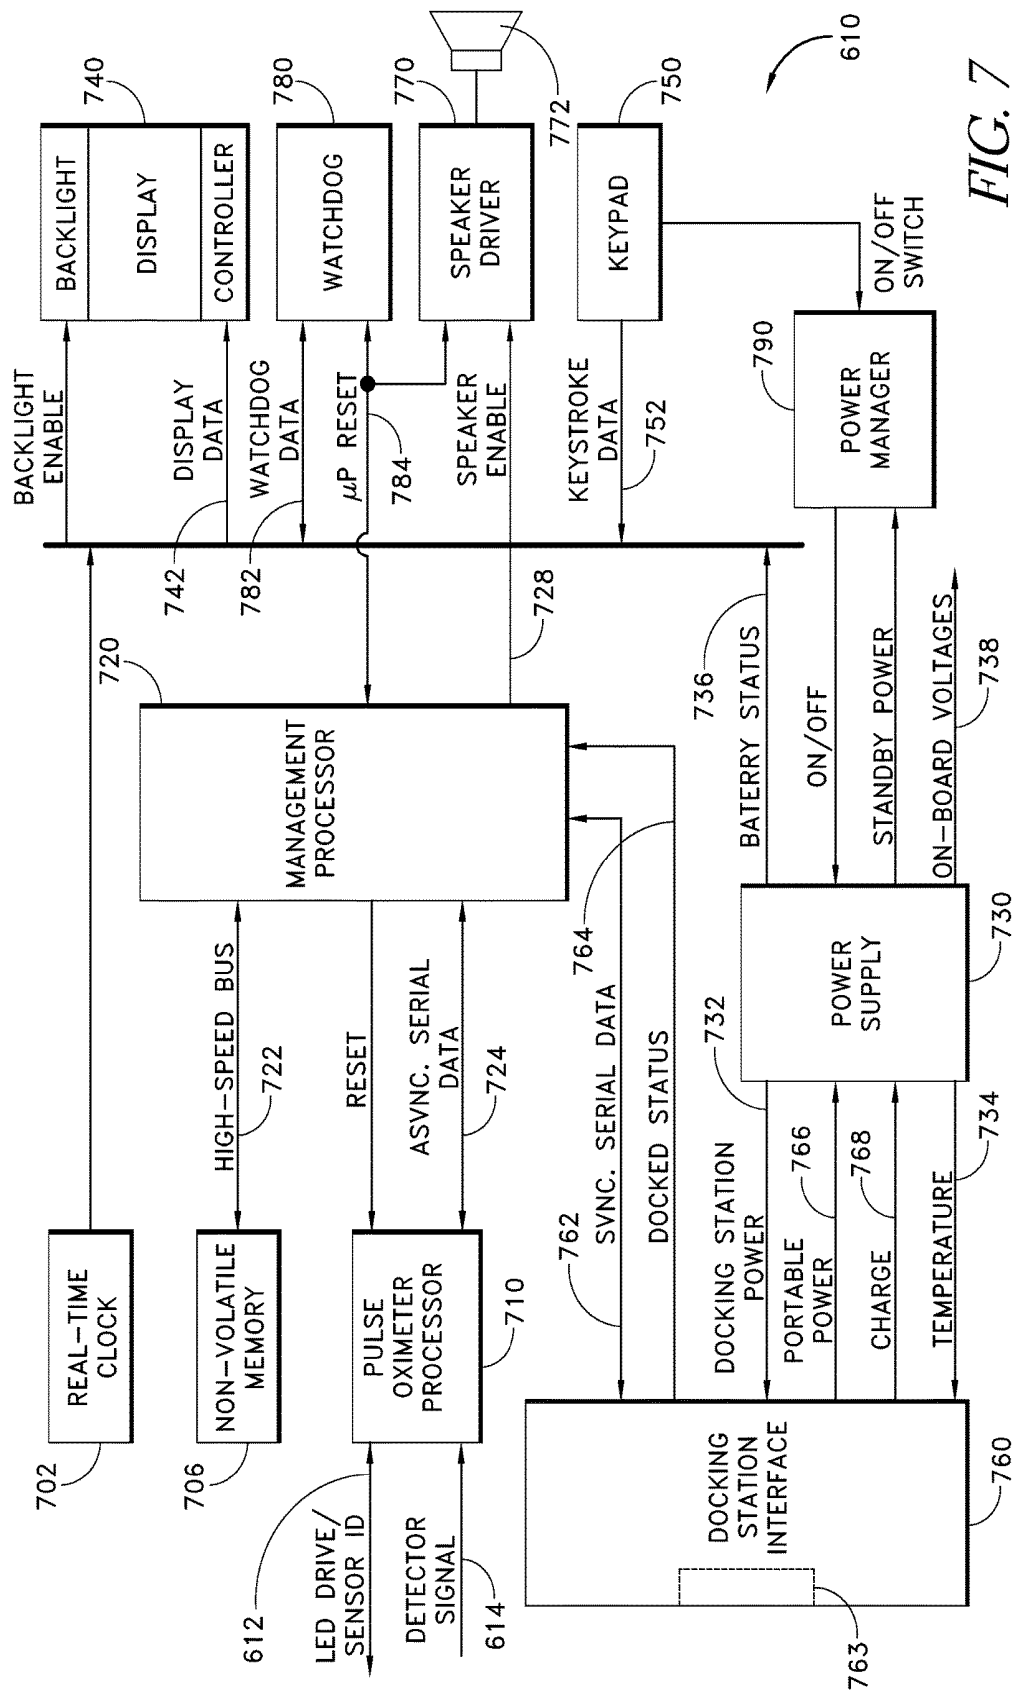


FIG. 7

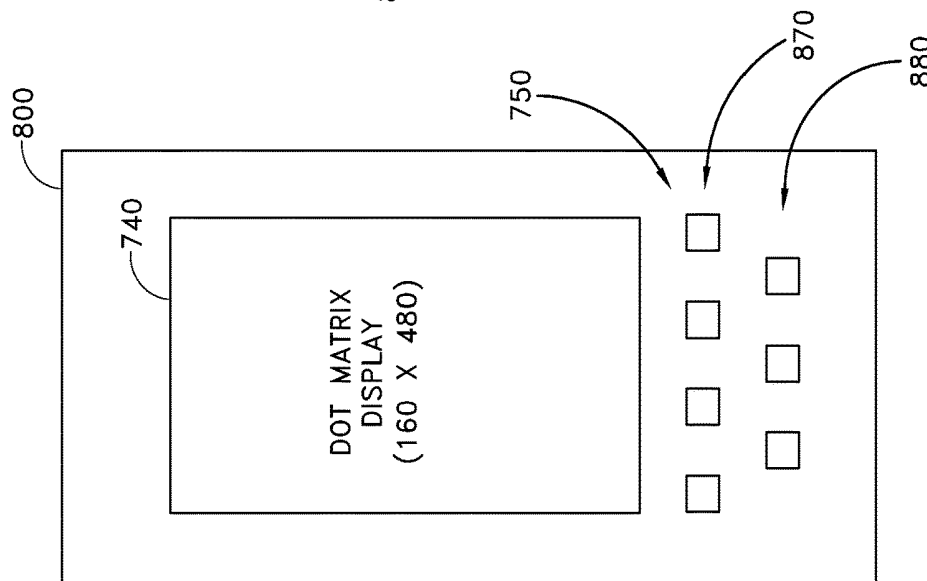


FIG. 8A

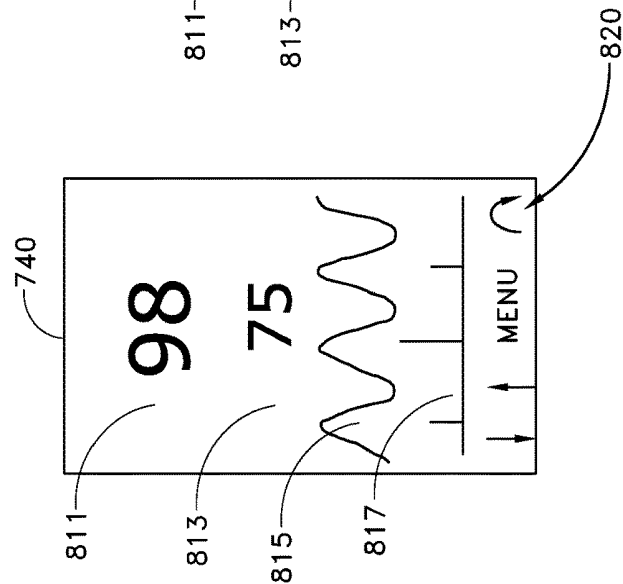


FIG. 8B

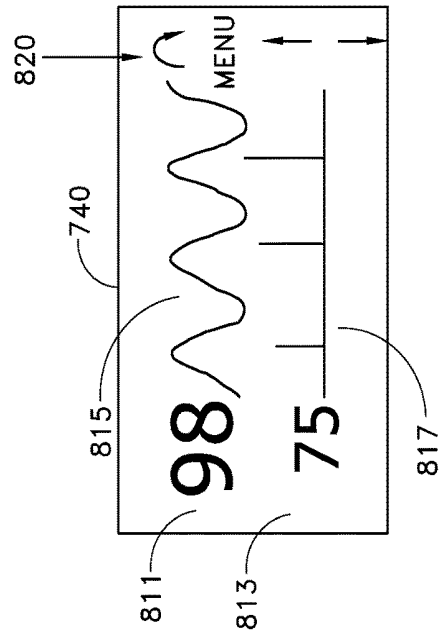


FIG. 8C

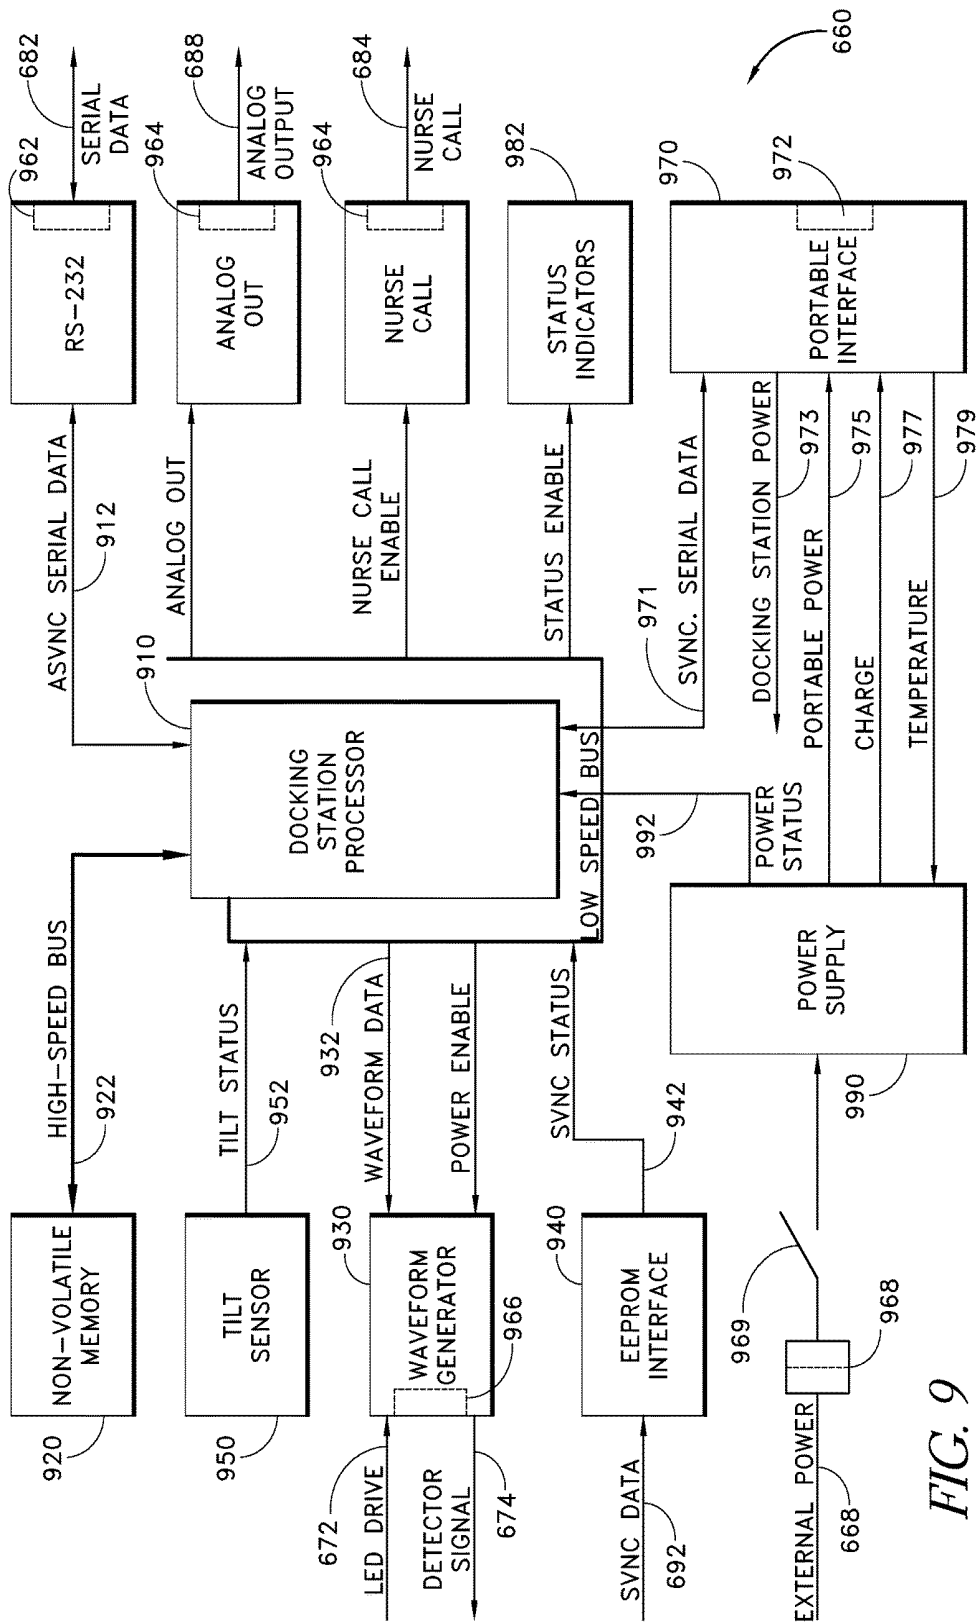


FIG. 9

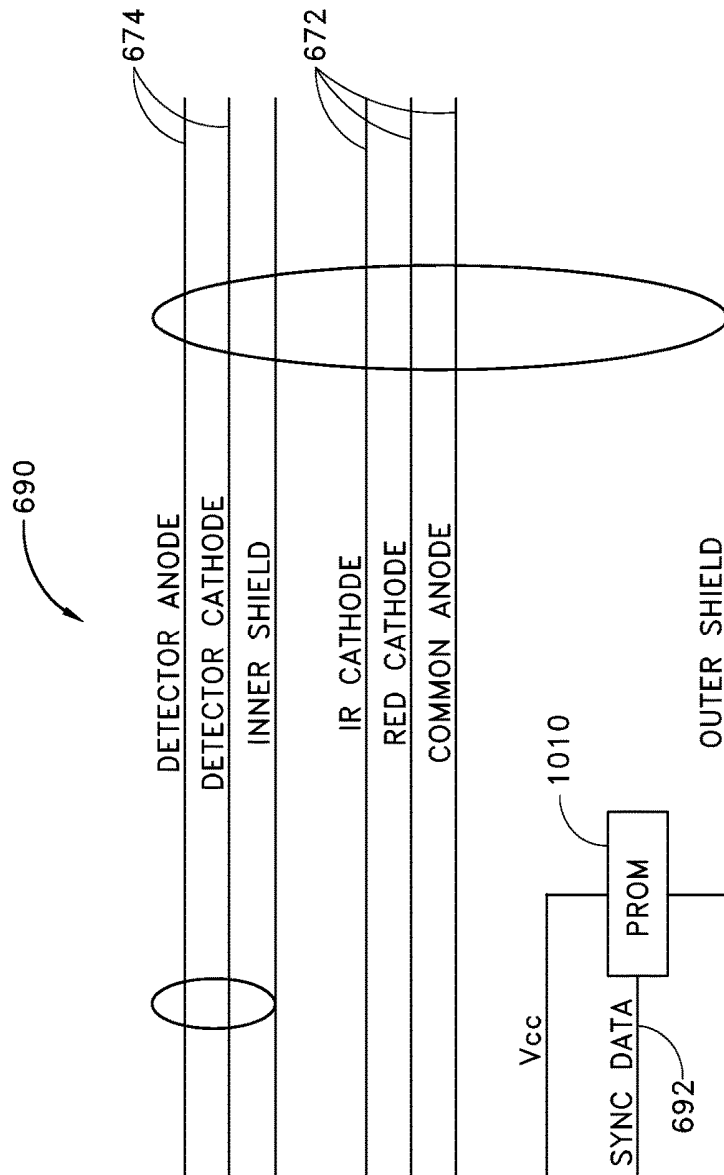


FIG. 10

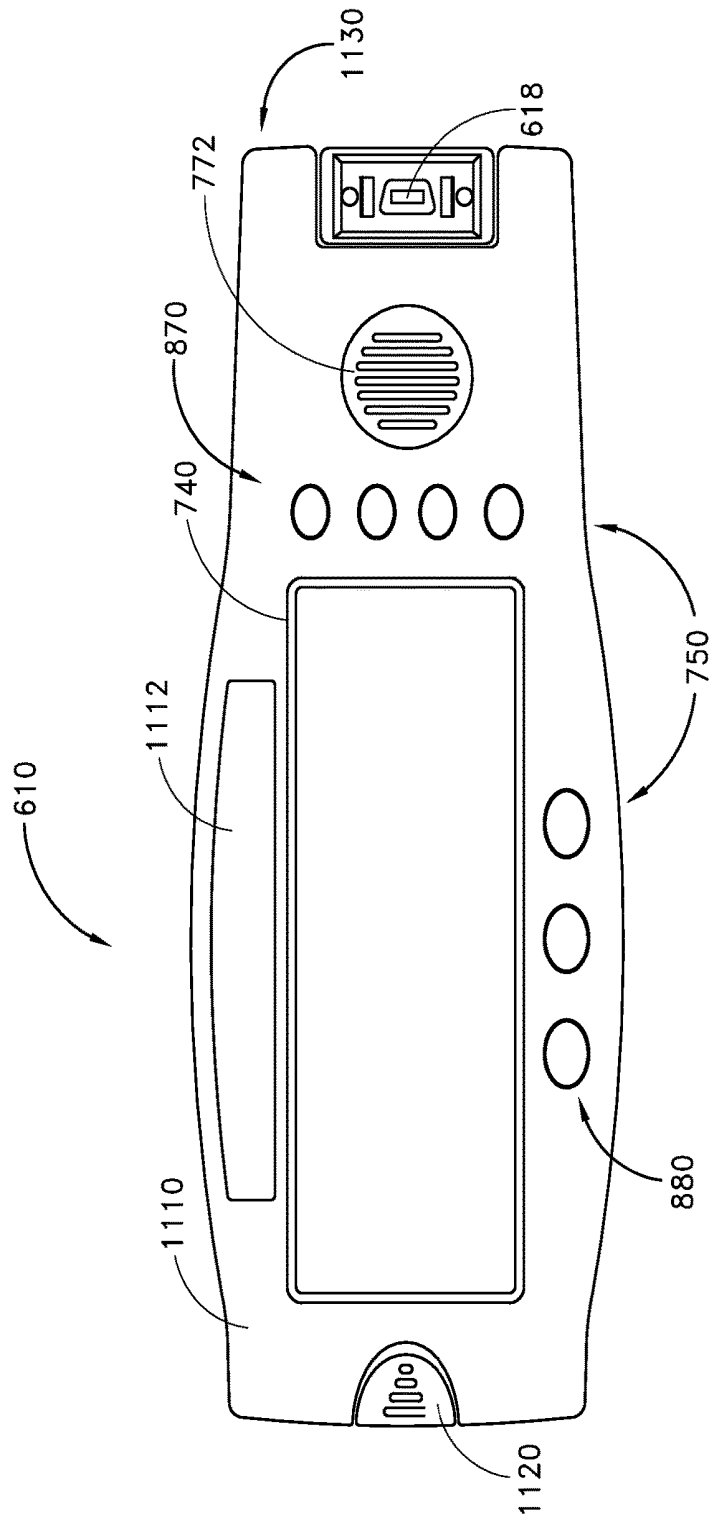


FIG. 11A

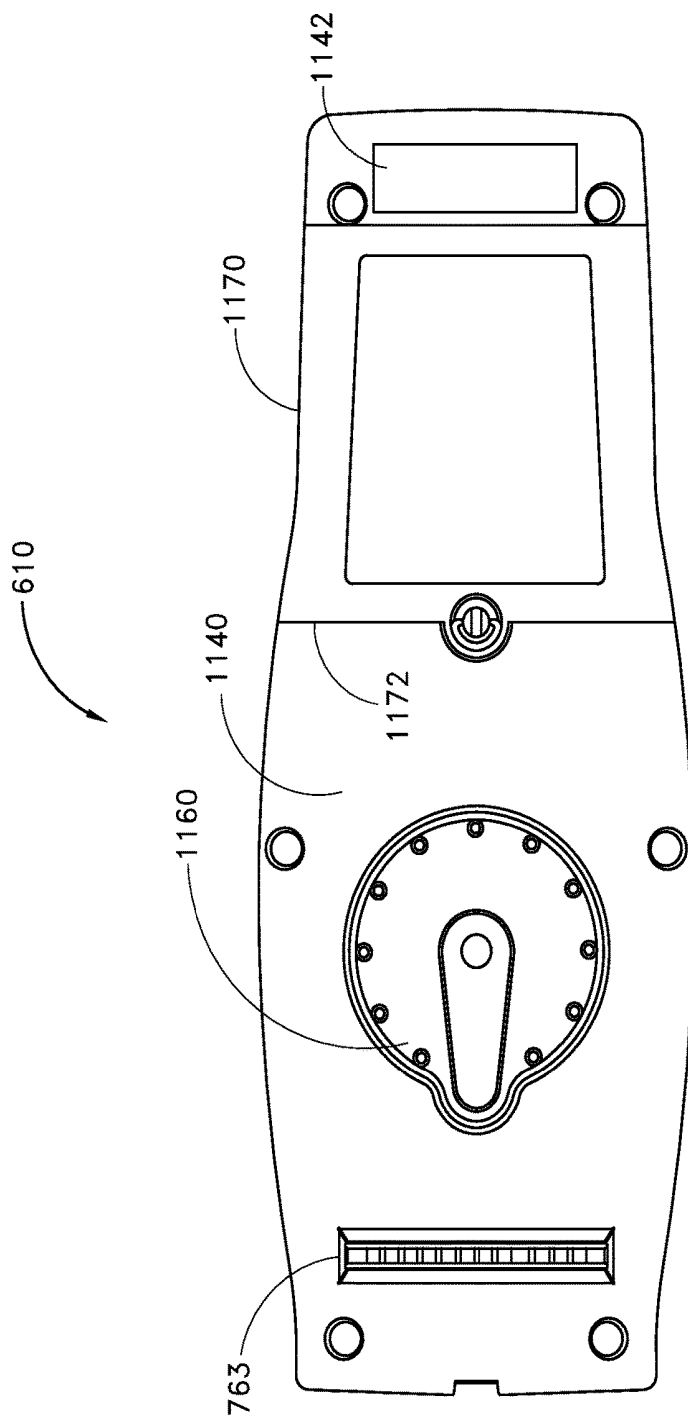


FIG. 11B



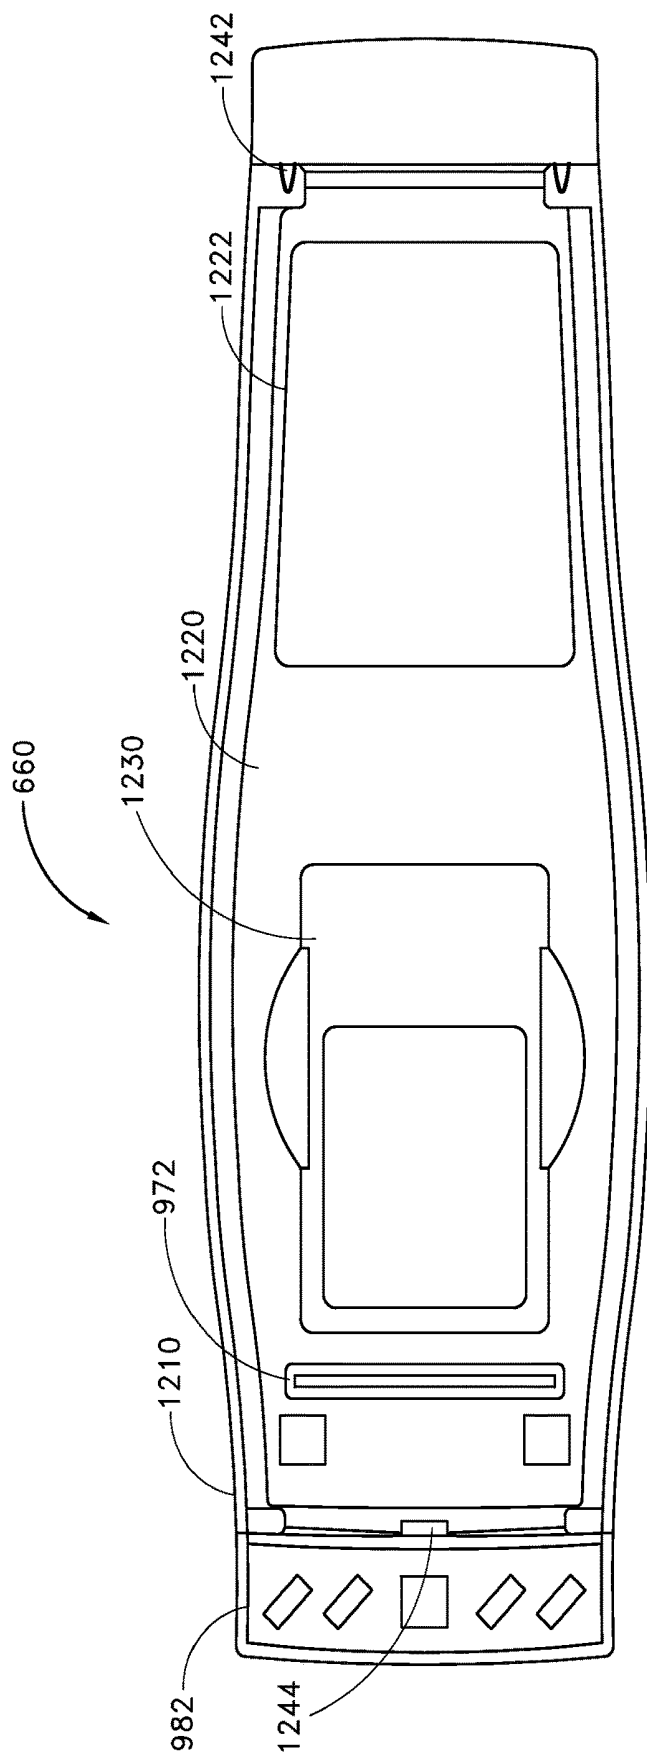


FIG. 12A

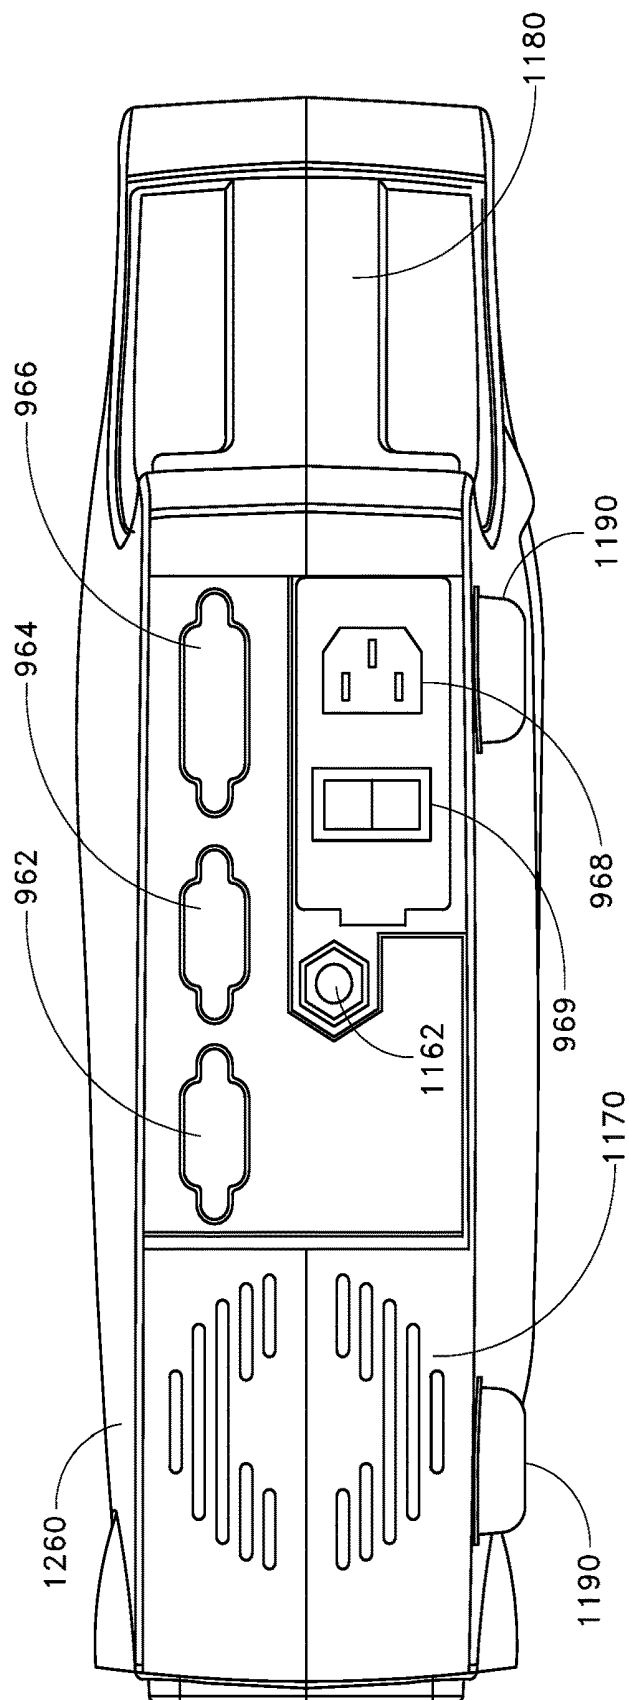


FIG. 12B

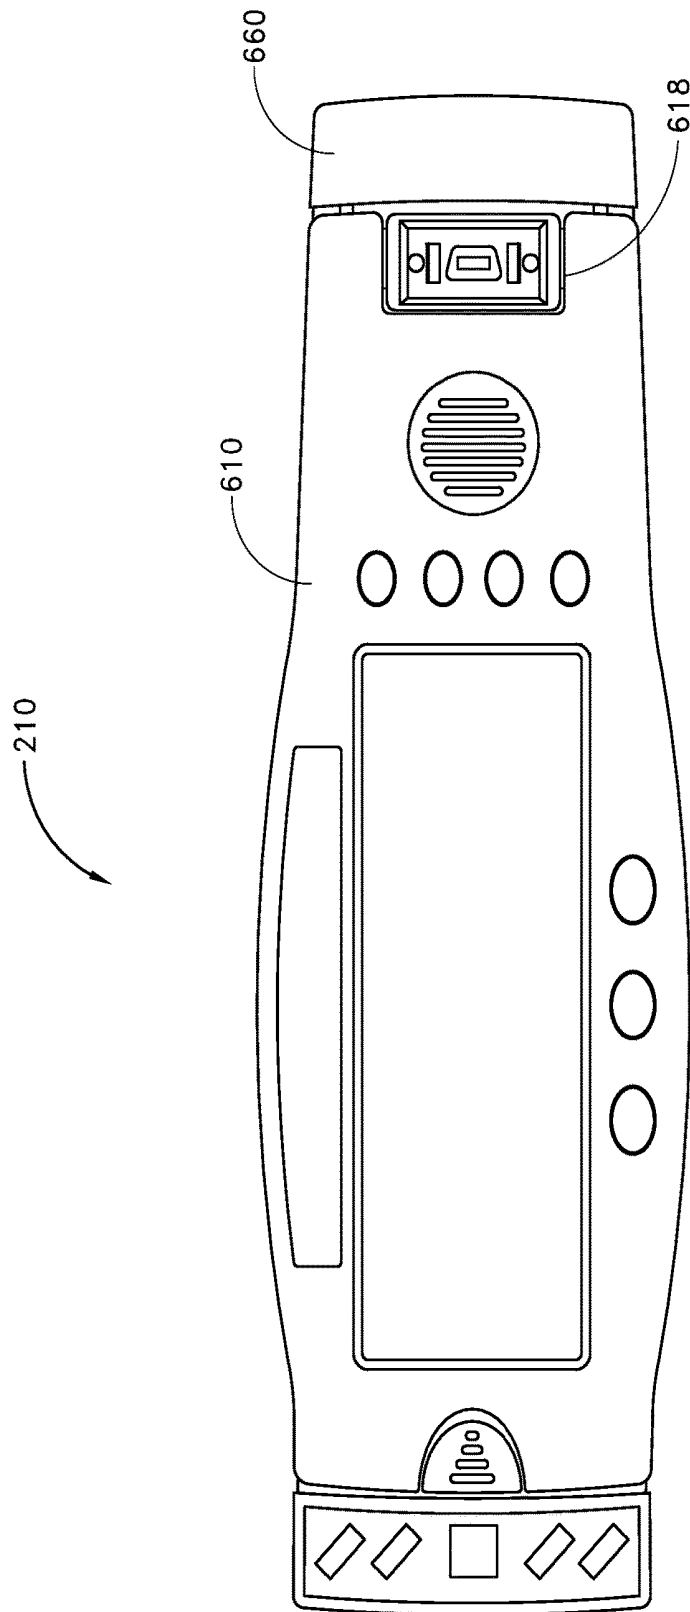
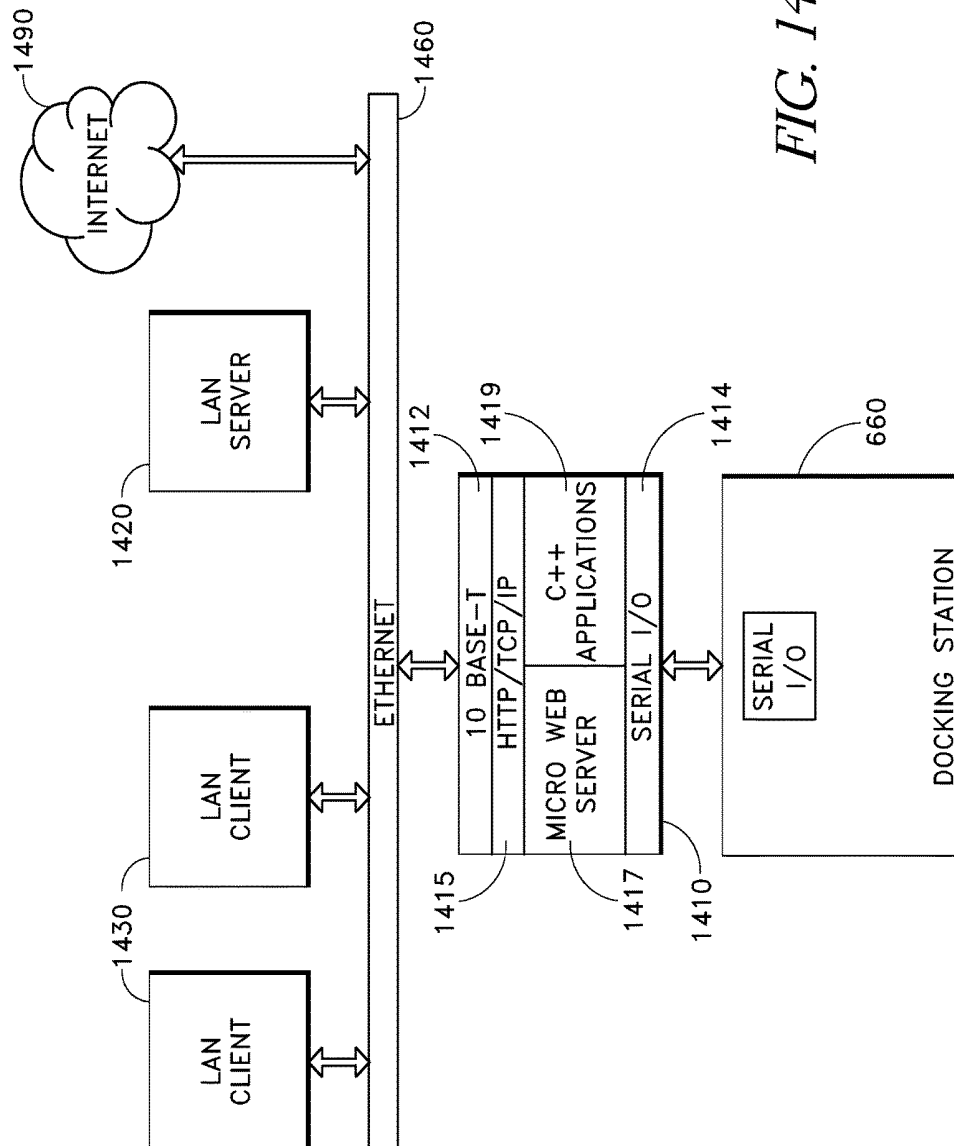


FIG. 13



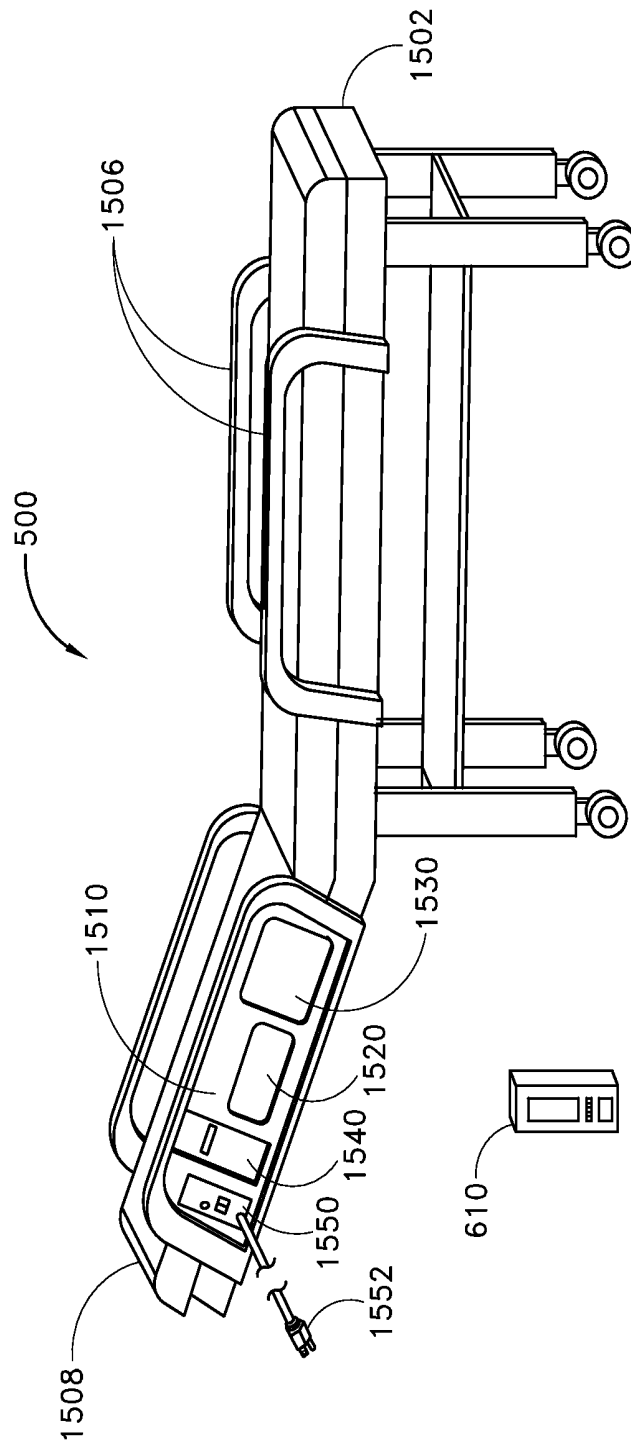


FIG. 15

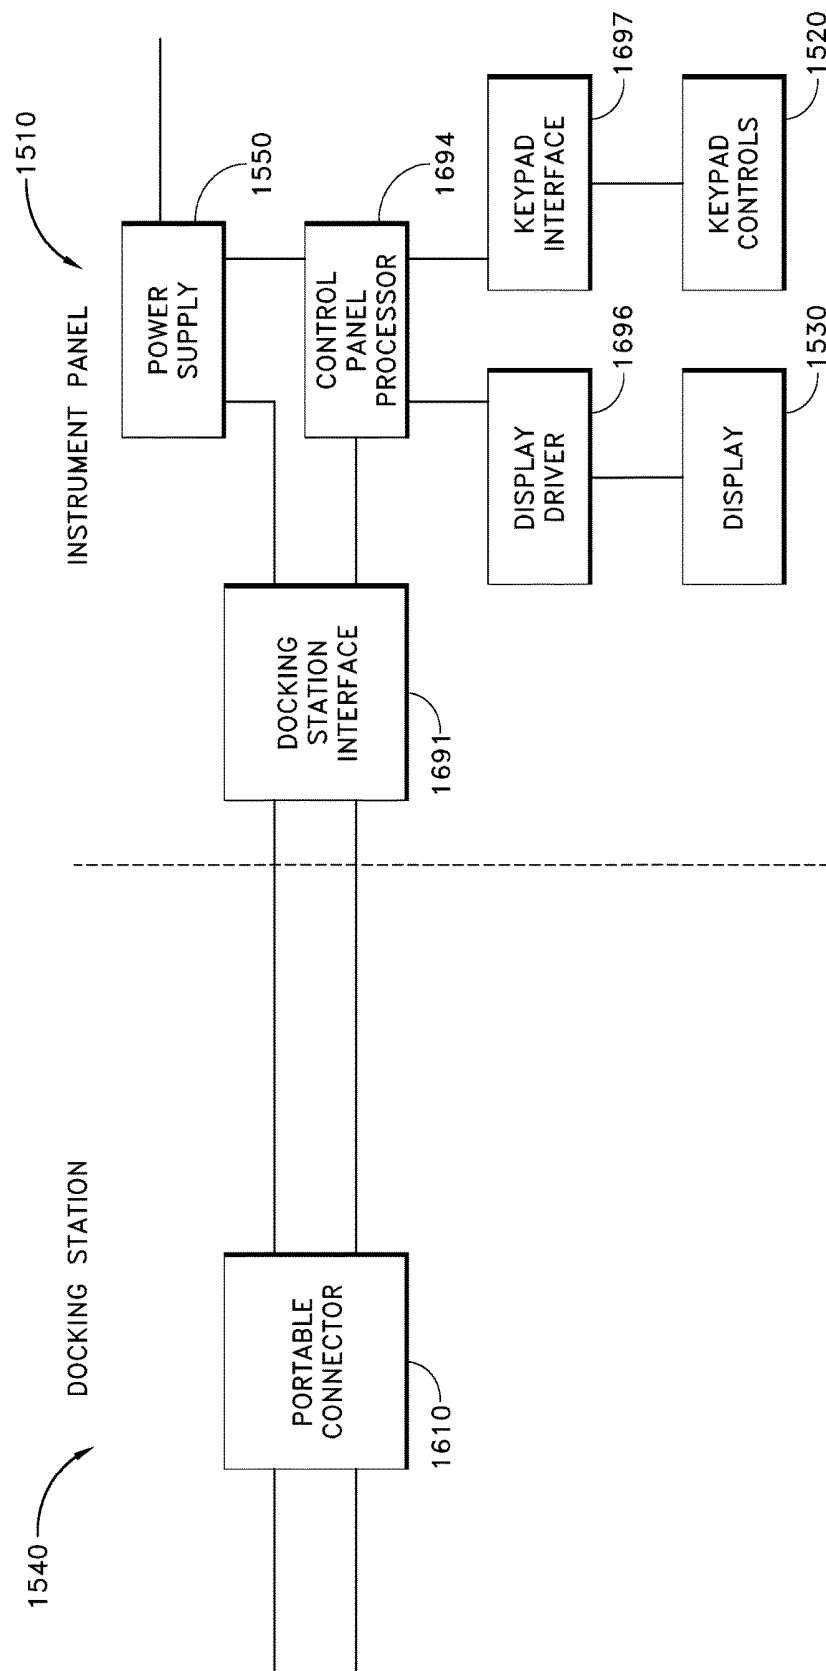


FIG. 16

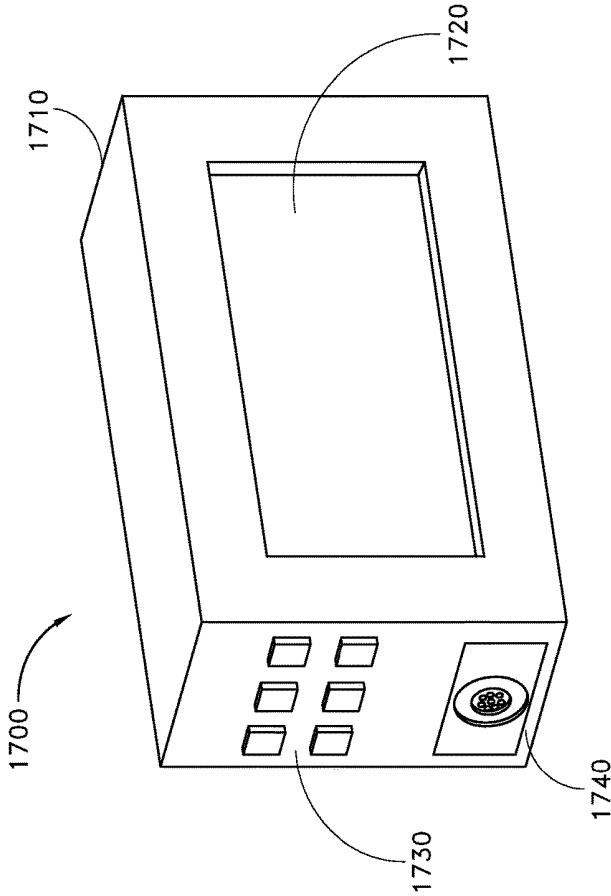


FIG. 17A

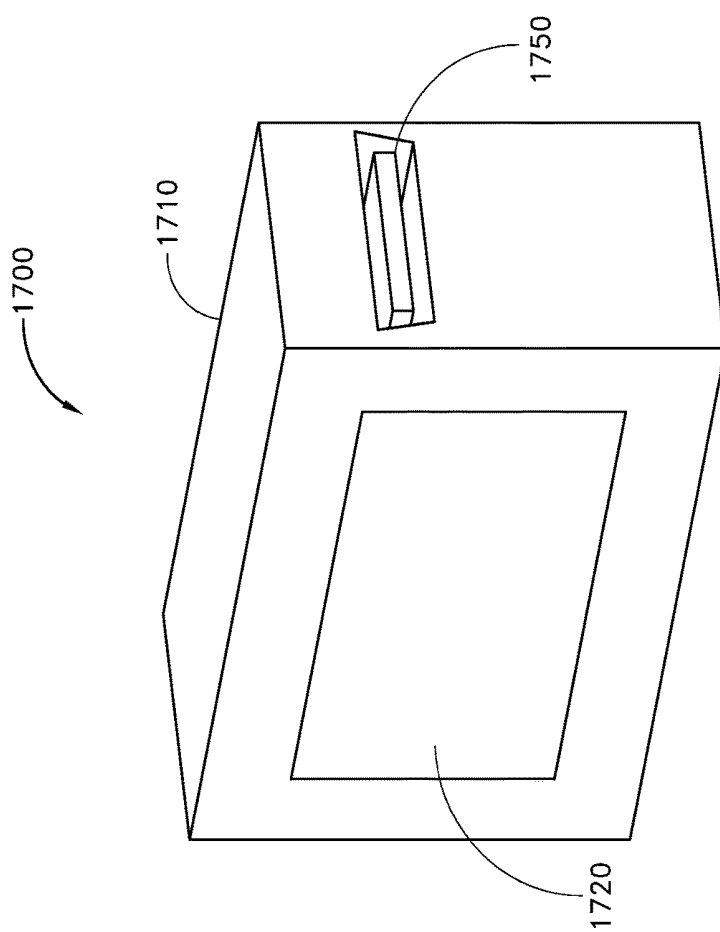


FIG. 17B



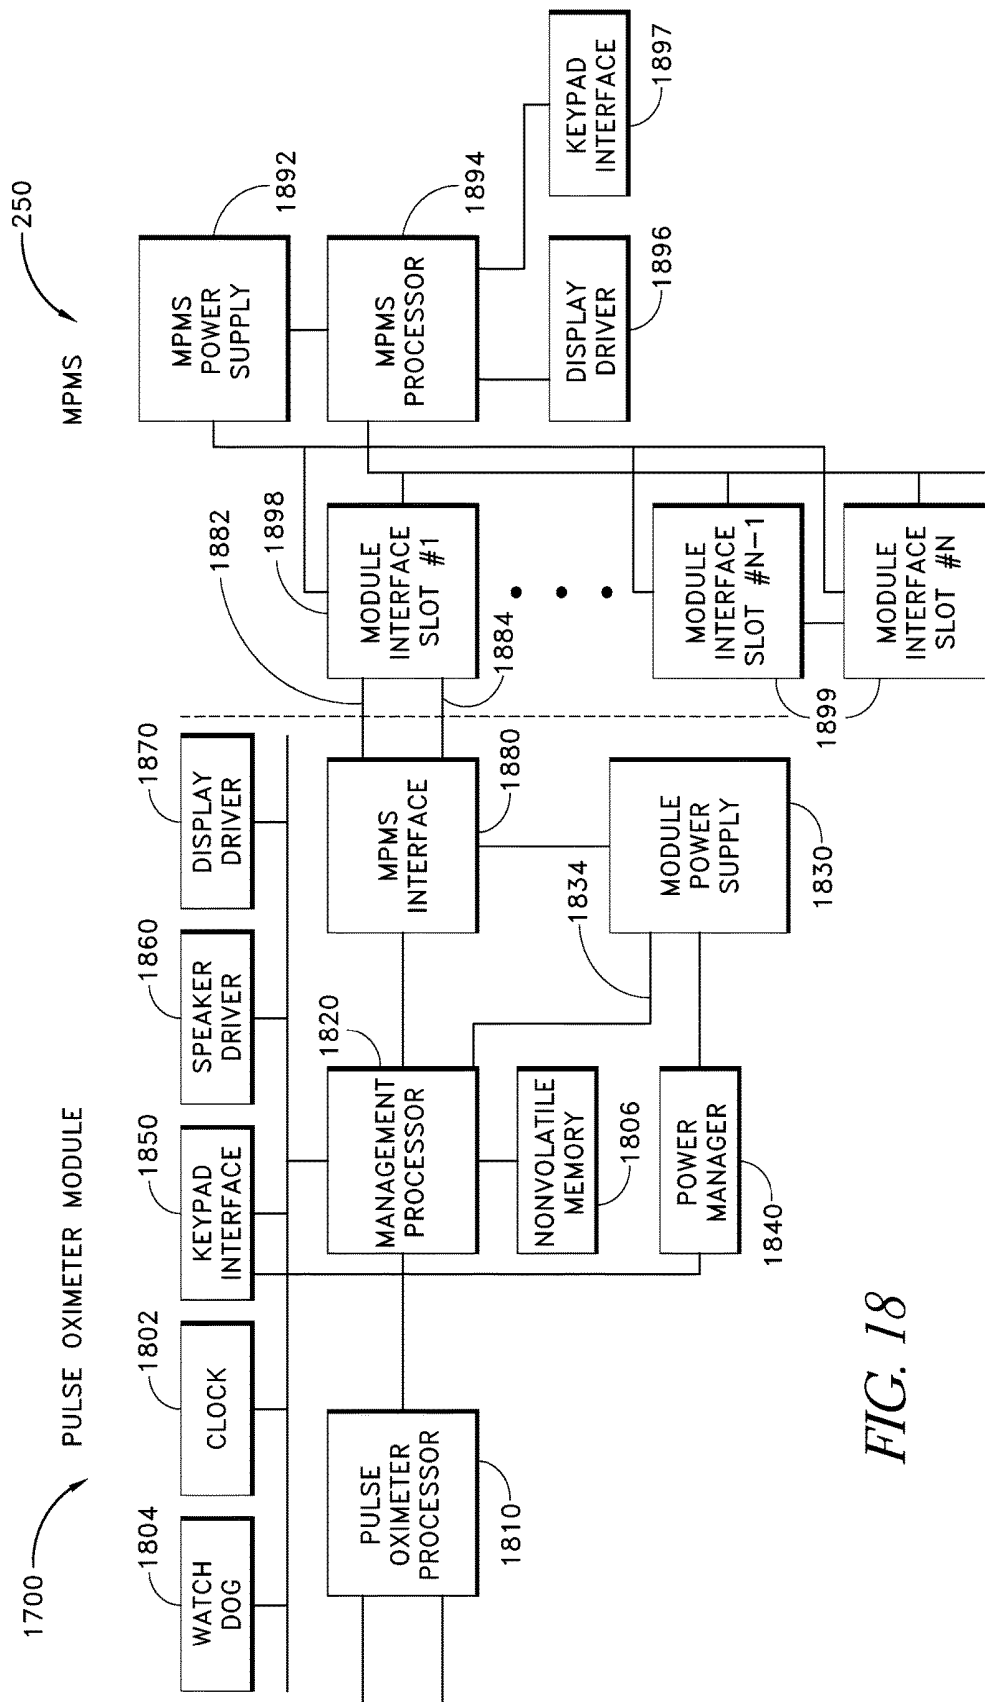
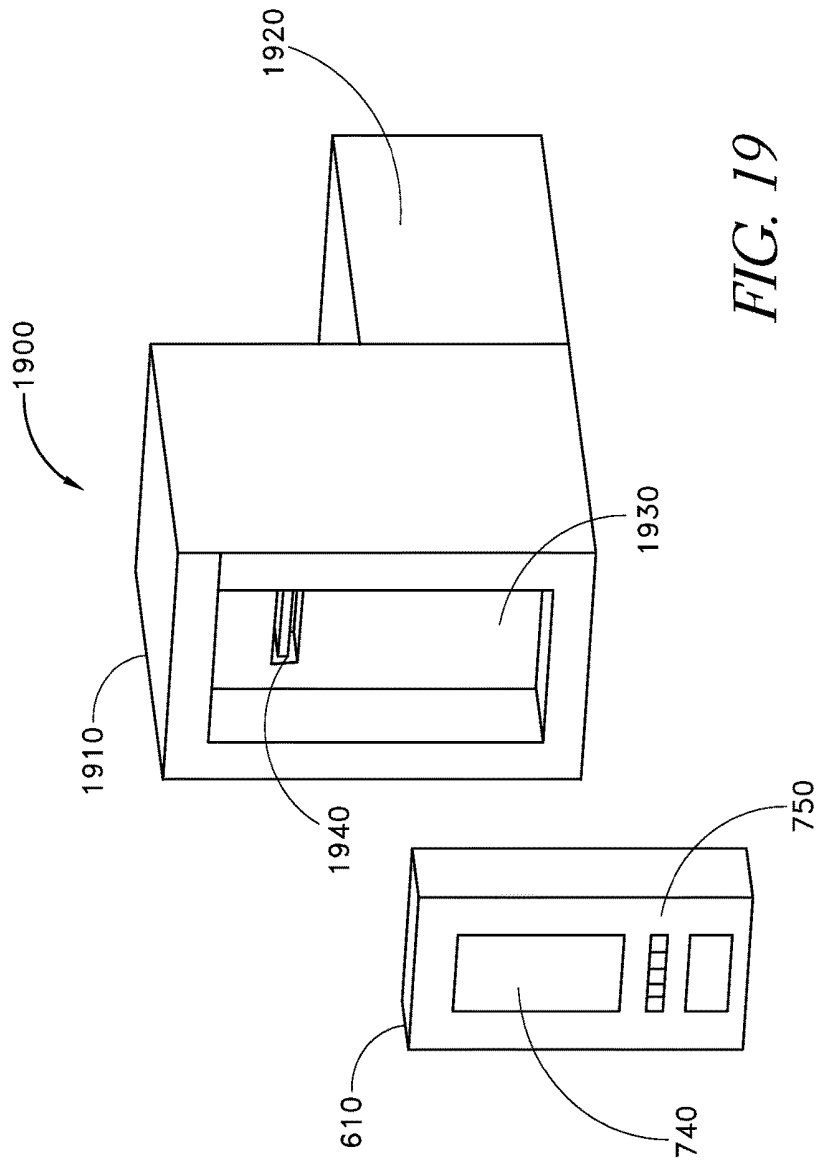


FIG. 18



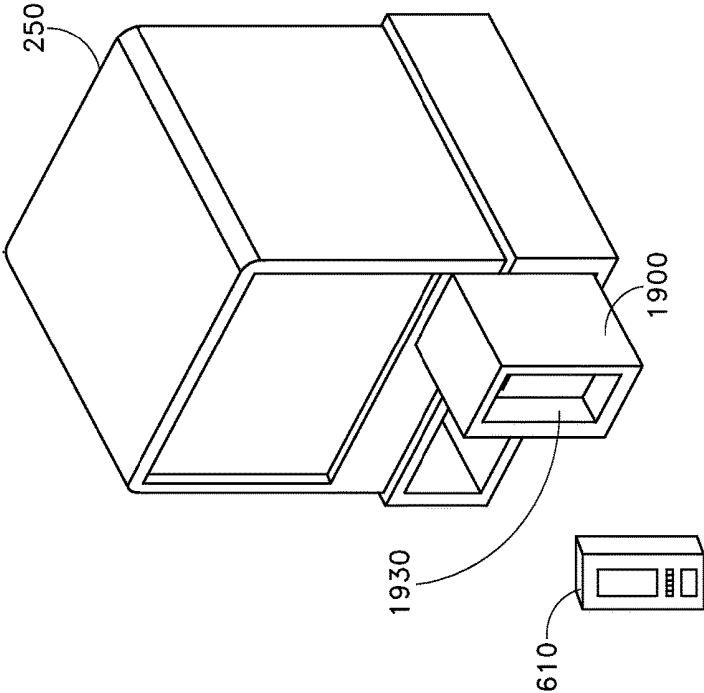


FIG. 20

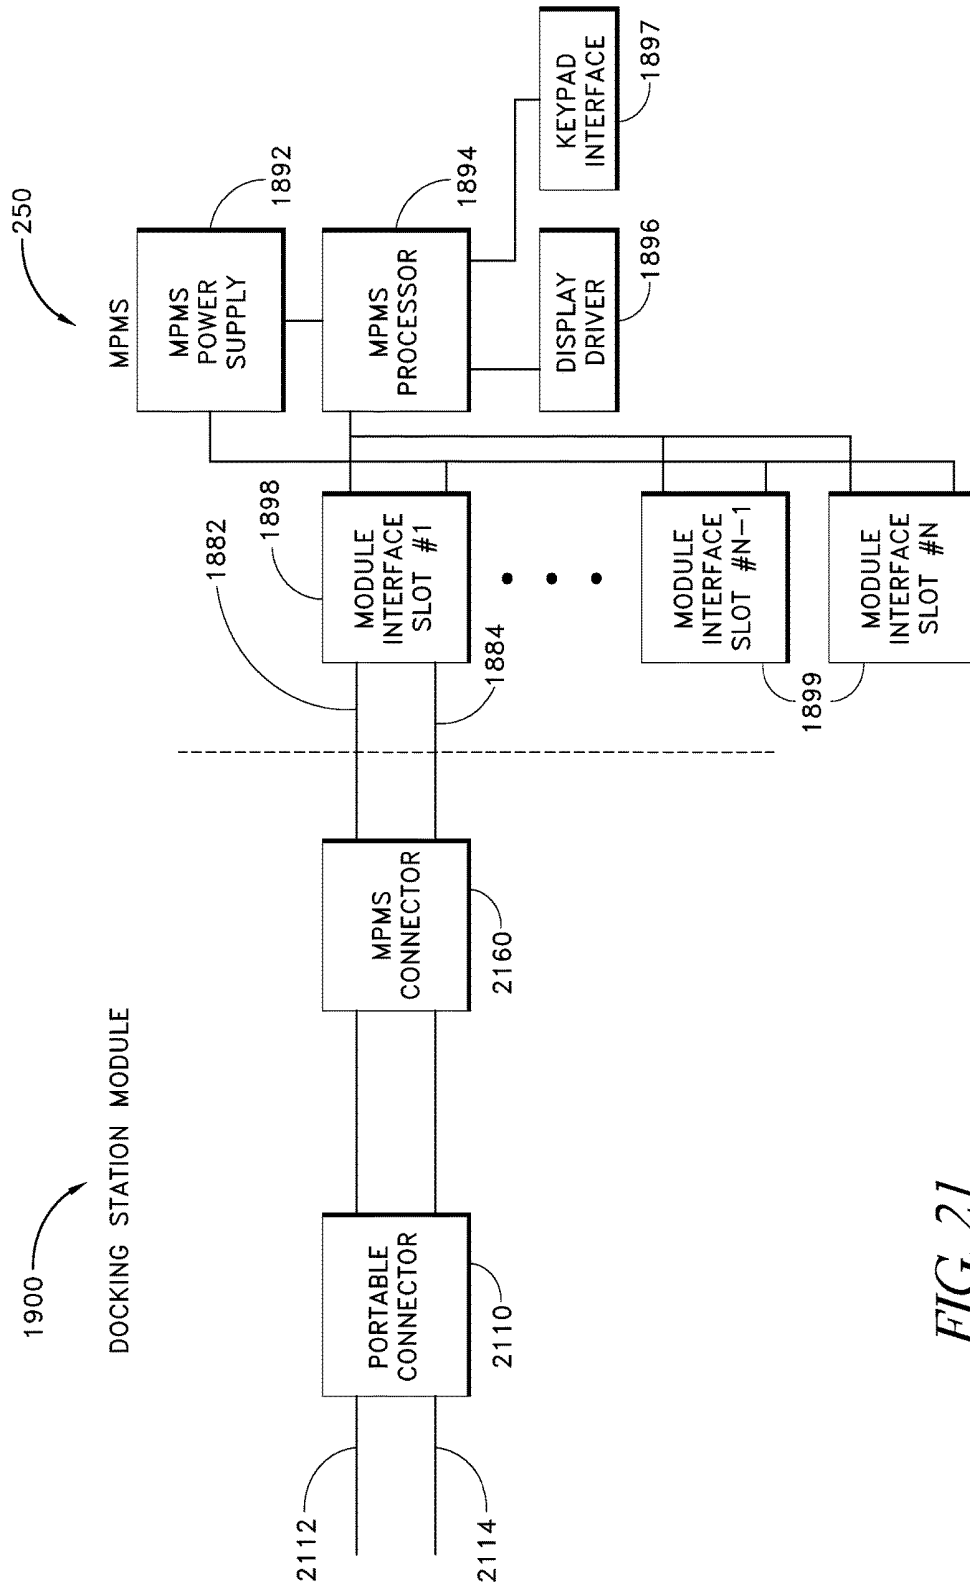


FIG. 21

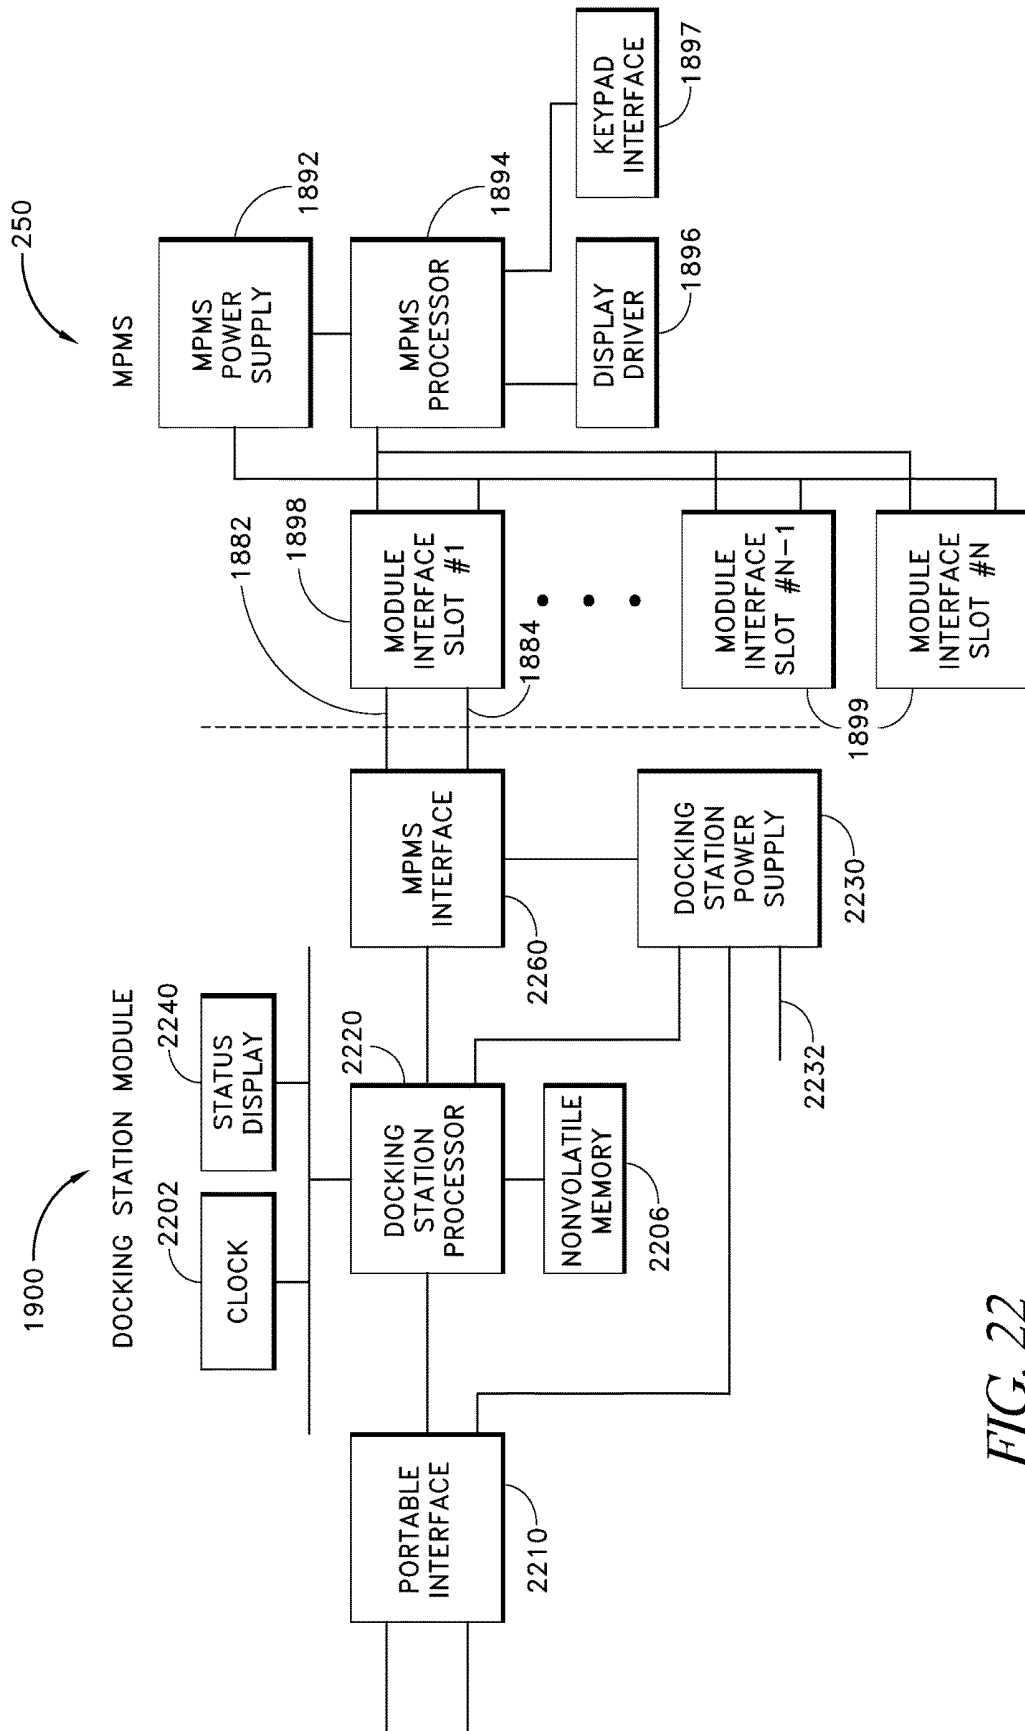


FIG. 22

## DUAL-MODE PATIENT MONITOR

## REFERENCE TO RELATED APPLICATION

This application is a continuation of U.S. patent application Ser. No. 11/894,722, entitled "Dual-Mode Pulse Oximeter," filed Aug. 20, 2007, which is a continuation of Ser. No. 10/911,391, entitled "Dual-Mode Pulse Oximeter," filed Aug. 3, 2004, now U.S. Pat. No. 7,530,949, which is a continuation of U.S. patent application Ser. No. 09/641,542, entitled "Dual-Mode Pulse Oximeter," filed Aug. 18, 2000, now U.S. Pat. No. 6,770,028, which is a continuation-in-part of U.S. patent application Ser. No. 09/491,175 entitled "Universal/Upgrading Pulse Oximeter," filed Jan. 25, 2000, now abandoned, which claims a priority benefit under 35 U.S.C. § 119(e) from U.S. Provisional Patent Application Nos. 60/161,565, filed Oct. 26, 1999, now abandoned, entitled "Improved Universal/Upgrading Pulse Oximeter," and 60/117,097, filed Jan. 25, 1999, now abandoned, entitled "Universal/Upgrading Pulse Oximeter." The present application incorporates the foregoing disclosures herein by reference.

## BACKGROUND OF THE INVENTION

Oximetry is the measurement of the oxygen level status of blood. Early detection of low blood oxygen level is critical in the medical field, for example in critical care and surgical applications, because an insufficient supply of oxygen can result in brain damage and death in a matter of minutes. Pulse oximetry is a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of oxygen supply. A pulse oximetry system generally consists of a sensor applied to a patient, a pulse oximeter, and a patient cable connecting the sensor and the pulse oximeter.

The pulse oximeter may be a standalone device or may be incorporated as a module or built-in portion of a multiparameter patient monitoring system, which also provides measurements such as blood pressure, respiratory rate and EKG. A pulse oximeter typically provides a numerical readout of the patient's oxygen saturation, a numerical readout of pulse rate, and an audible indicator or "beep" that occurs in response to each pulse. In addition, the pulse oximeter may display the patient's plethysmograph, which provides a visual display of the patient's pulse contour and pulse rate.

## SUMMARY OF THE INVENTION

FIG. 1 illustrates a prior art pulse oximeter 100 and associated sensor 110. Conventionally, a pulse oximetry sensor 110 has LED emitters 112, typically one at a red wavelength and one at an infrared wavelength, and a photodiode detector 114. The sensor 110 is typically attached to an adult patient's finger or an infant patient's foot. For a finger, the sensor 110 is configured so that the emitters 112 project light through the fingernail and through the blood vessels and capillaries underneath. The LED emitters 112 are activated by drive signals 122 from the pulse oximeter 100. The detector 114 is positioned at the fingertip opposite the fingernail so as to detect the LED emitted light as it emerges from the finger tissues. The photodiode generated signal 124 is relayed by a cable to the pulse oximeter 100.

The pulse oximeter 100 determines oxygen saturation (SpO<sub>2</sub>) by computing the differential absorption by arterial blood of the two wavelengths emitted by the sensor 110. The

pulse oximeter 100 contains a sensor interface 120, an SpO<sub>2</sub> processor 130, an instrument manager 140, a display 150, an audible indicator (tone generator) 160 and a keypad 170. The sensor interface 120 provides LED drive current 122 which alternately activates the sensor red and IR LED emitters 112. The sensor interface 120 also has input circuitry for amplification and filtering of the signal 124 generated by the photodiode detector 114, which corresponds to the red and infrared light energy attenuated from transmission through the patient tissue site. The SpO<sub>2</sub> processor 130 calculates a ratio of detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on that ratio. The instrument manager 140 provides hardware and software interfaces for managing the display 150, audible indicator 160 and keypad 170. The display 150 shows the computed oxygen status, as described above. The audible indicator 160 provides the pulse beep as well as alarms indicating desaturation events. The keypad 170 provides a user interface for such things as alarm thresholds, alarm enablement, and display options.

Computation of SpO<sub>2</sub> relies on the differential light absorption of oxygenated hemoglobin, HbO<sub>2</sub>, and deoxygenated hemoglobin, Hb, to determine their respective concentrations in the arterial blood. Specifically, pulse oximetry measurements are made at red and IR wavelengths chosen such that deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin, for example 660 nm (red) and 905 nm (IR).

To distinguish between tissue absorption at the two wavelengths, the red and IR emitters 112 are provided drive current 122 so that only one is emitting light at a given time. For example, the emitters 112 may be cycled on and off alternately, in sequence, with each only active for a quarter cycle and with a quarter cycle separating the active times. This allows for separation of red and infrared signals and removal of ambient light levels by downstream signal processing. Because only a single detector 114 is used, it responds to both the red and infrared emitted light and generates a time-division-multiplexed ("modulated") output signal 124. This modulated signal 124 is coupled to the input of the sensor interface 120.

In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site might also comprise skin, muscle, bone, venous blood, fat, pigment, etc., each of which absorbs light. It is generally assumed that the background absorption due to these surrounding tissues is relatively invariant over short time periods and can be easily removed. Thus, blood oxygen saturation measurements are based upon a ratio of the time-varying or AC portion of the detected red and infrared signals with respect to the time-invariant or DC portion:

$$RD/IR = (Red_{AC}/Red_{DC}) / (IR_{AC}/IR_{DC})$$

The desired SpO<sub>2</sub> measurement is then computed from this ratio. The relationship between RD/IR and SpO<sub>2</sub> is most accurately determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. In a pulse oximeter device, this empirical relationship can be stored as a "calibration curve" in a read-only memory (ROM) look-up

table so that SpO<sub>2</sub> can be directly read-out of the memory in response to input RD/IR measurements.

Pulse oximetry is the standard-of-care in various hospital and emergency treatment environments. Demand has lead to pulse oximeters and sensors produced by a variety of manufacturers. Unfortunately, there is no standard for either performance by, or compatibility between, pulse oximeters or sensors. As a result, sensors made by one manufacturer are unlikely to work with pulse oximeters made by another manufacturer. Further, while conventional pulse oximeters and sensors are incapable of taking measurements on patients with poor peripheral circulation and are partially or fully disabled by motion artifact, advanced pulse oximeters and sensors manufactured by the assignee of the present invention are functional under these conditions. This presents a dilemma to hospitals and other caregivers wishing to upgrade their patient oxygenation monitoring capabilities. They are faced with either replacing all of their conventional pulse oximeters, including multiparameter patient monitoring systems, or working with potentially incompatible sensors and inferior pulse oximeters manufactured by various vendors for the pulse oximetry equipment in use at the installation.

Hospitals and other caregivers are also plagued by the difficulty of monitoring patients as they are transported from one setting to another. For example, a patient transported by ambulance to a hospital emergency room will likely be unmonitored during the transition from ambulance to the ER and require the removal and replacement of incompatible sensors in the ER. A similar problem is faced within a hospital as a patient is moved between surgery, ICU and recovery settings. Incompatibility and transport problems are exacerbated by the prevalence of expensive and non-portable multi-parameter patient monitoring systems having pulse oximetry modules as one measurement parameter.

One aspect of the present invention is a dual-mode physiological measurement apparatus having a portable mode and an integrated mode. In the integrated mode, the measurement apparatus operates in conjunction with a multiparameter patient monitoring system (MPMS). In the portable mode, the measurement apparatus operates separately from the MPMS. The measurement apparatus has a physiological measurement processor, a display, a MPMS interface and a management processor. The physiological measurement processor has a sensor input and provides a physiological measurement output. In the portable mode, the display indicates a physiological parameter according to the physiological measurement output. In the integrated mode, the MPMS interface provides a communications link between the measurement apparatus and the MPMS. The management processor has as an input the physiological measurement output. The management processor controls the display in the portable mode and communicates the measurement output to the MPMS via the MPMS interface in the integrated mode.

In one embodiment, the measurement apparatus described in the previous paragraph further comprises a plug-in module. The plug-in module comprises the measurement processor and the MPMS interface and possibly the display and management processor and is configured to be removably retained by and electrically connected to the MPMS in the integrated mode. The plug-in module may further comprise a patient cable connector providing the sensor input, a keypad accepting user inputs in the portable mode, and a module connector mating with a corresponding MPMS backplane connector in the integrated mode. In another embodiment, the measurement apparatus further comprises

a docking station and a portable portion. The docking station has a docking portion, a plug-in portion and the MPMS interface. The plug-in portion is configured to be removably retained by and electrically connected to the MPMS. The portable portion comprises the measurement processor, the display and the management processor. In the integrated mode, the portable portion is configured to be removably retained by and electrically connected to the docking portion. In the portable mode, the portable portion is separated from the docking station and operated as a standalone patient monitoring apparatus. The portable portion may further comprise a patient cable connector providing the sensor input, a keypad accepting user inputs in the portable mode, and a portable connector mating with a corresponding docking station connector in the integrated mode.

Another aspect of the present invention is a patient monitoring method utilizing a standalone measurement apparatus and a multiparameter patient monitoring system (MPMS) comprising the steps of performing a first physiological measurement with the standalone apparatus physically and electrically isolated from the MPMS and presenting information related to the first measurement on a display portion of the standalone apparatus. Further steps include performing a second physiological measurement with the standalone apparatus interfaced to the MPMS, communicating the second physiological measurement to the MPMS, and presenting information related to the second measurement on a monitor portion of the MPMS.

One embodiment of the patient monitoring method described in the previous paragraph further comprises the step of plugging the measurement apparatus into a module slot portion of the MPMS so that the measurement apparatus is in electrical communications with the MPMS. Another embodiment further comprises the steps of plugging a docking station into a module slot portion of the MPMS so that the docking station is in electrical communications with the MPMS, and attaching the standalone apparatus to the docking station so that the standalone apparatus is in electrical communications with the docking station.

Yet another aspect of the present invention is a physiological measurement apparatus comprising a sensor responsive to a physiological state, a measurement processor means for calculating a physiological parameter based upon the physiological state, which presents the physiological parameter to a person, a packaging means for housing the measurement processor and the display and for providing a connection between the sensor and the measurement processor means, and an interface means for electrically connecting the packaging means to a multiparameter patient monitoring system (MPMS) in an integrated mode and for disconnecting the packaging means from the MPMS in a portable mode. In a particular embodiment, the packaging means comprises a module means for plugging into a slot portion of the MPMS. In another particular embodiment, the physiological measurement apparatus further comprises a docking station means for plugging into a slot portion of the MPMS. In the integrated mode, the packaging means is configured to attach to the docking station.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a block diagram of a prior art pulse oximeter;

FIG. 2 is a diagram illustrating a patient monitoring system incorporating a universal/upgrading pulse oximeter (UPO) according to the present invention;

FIG. 3 is top level block diagram of a UPO embodiment;

FIG. 4 is a detailed block diagram of the waveform generator portion of the UPO embodiment shown in FIG. 3;

FIG. 5 is an illustration of a handheld embodiment of the UPO;

FIG. 6 is a top level block diagram of another UPO embodiment incorporating a portable pulse oximeter and a docking station;

FIG. 7 is a detailed block diagram of the portable pulse oximeter portion of FIG. 6;

FIG. 8A is an illustration of the portable pulse oximeter user interface, including a keyboard and display;

FIGS. 8B-C are illustrations of the portable pulse oximeter display showing portrait and landscape modes, respectively;

FIG. 9 is a detailed block diagram of the docking station portion of FIG. 6;

FIG. 10 is a schematic of the interface cable portion of FIG. 6;

FIG. 11A is a front view of an embodiment of a portable pulse oximeter;

FIG. 11B is a back view of a portable pulse oximeter;

FIG. 12A is a front view of an embodiment of a docking station;

FIG. 12B is a back view of a docking station;

FIG. 13 is a front view of a portable docked to a docking station;

FIG. 14 is a block diagram of one embodiment of a local area network interface for a docking station;

FIG. 15 is a perspective view of a patient care bed incorporating a docking station;

FIG. 16 is a block diagram of a docking station integrated into a patient care bed;

FIGS. 17A-B are front and back perspective views of a dual-mode pulse oximeter module according to the present invention;

FIG. 18 is a block diagram of the dual-mode pulse oximeter module;

FIG. 19 is a perspective view of a docking station module according to the present invention;

FIG. 20 is a perspective view of the docking station module of FIG. 19 attached to a multiparameter patient monitoring system (MPMS);

FIG. 21 is a block diagram of a pass-through docking station module; and

FIG. 22 is a block diagram of a docking station module providing an MPMS interface.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

FIG. 2 depicts the use of a Universal/Upgrading Pulse Oximeter ("UPO") 210 to perform patient monitoring. A pulse oximetry sensor 110 is attached to a patient (not illustrated) and provides the UPO 210 with a modulated red and IR photo-plethysmograph signal through a patient cable 220. It should be understood that while a pulse oximeter is illustrated, the present invention has applicability to other physiological parameter such as ECG, blood pressure, respiration, etc. The UPO 210 computes the patient's oxygen saturation and pulse rate from the sensor signal and, optionally, displays the patient's oxygen status. The UPO 210 may incorporate an internal power source 212, such as common alkaline batteries or a rechargeable power source. The UPO 210 may also utilize an external power source 214, such as standard 110V AC coupled with an external step-down transformer and an internal or external AC-to-DC converter.

In addition to providing pulse oximetry measurements, the UPO 210 also separately generates a signal, which is received by a pulse oximeter 260 external to the UPO 210. This signal is synthesized from the saturation calculated by the UPO 210 such that the external pulse oximeter 260 calculates the equivalent saturation and pulse rate as computed by the UPO 210. The external pulse oximeter receiving the UPO signal may be a multiparameter patient monitoring system (MPMS) 250 incorporating a pulse oximeter module 260, a standalone pulse oximeter instrument, or any other host instrument capable of measuring SpO<sub>2</sub>.

As shown in FIG. 2, a MPMS 250 typically has a chassis 270, a multiparameter monitor 280, a processor 1894 (FIG. 18) and a power supply 1892 (FIG. 18), which derives power from a standard external AC power source. The monitor 280 typically incorporates a display 282. The chassis 270 typically has various slots 290 each configured to receive a plug-in module 298. A module connector, e.g. the connector 1750 (FIG. 17B) on the dual-mode pulse oximeter module described with respect to FIGS. 17A-B, below, mates and electrically connects with a corresponding backplane connector (not shown) within the chassis 270. A variety of modules having various patient monitoring functions, such as blood pressure, EKG, respiratory gas and pulse oximetry 260 can be plugged into the slots 290 so that the associated patient parameters can be jointly monitored by the MPMS 250 and logged on the multiparameter display 282.

Also shown in FIG. 2, the UPO 210 is connected to an existing MPMS 250 with a cable 230, advantageously integrating the UPO oxygen status measurements with other MPMS measurements. This allows the UPO calculations to be shown on a unified display of important patient parameters, networked with other patient data, archived within electronic patient records and incorporated into alarm management, which are all MPMS functions convenient to the caregiver.

FIG. 3 depicts a block diagram of the major functions of the UPO 210, including an internal pulse oximeter 310, a waveform generator 320, a power supply 330 and an optional display 340. Attached to the UPO 210 is a sensor 110 and an external pulse oximeter 260. The internal pulse oximeter 310 provides the sensor 110 with a drive signal 312 that alternately activates the sensor's red and IR LEDs, as is known in the art. A corresponding detector signal 314 is received by the internal pulse oximeter 310. The internal pulse oximeter 310 computes oxygen saturation, pulse rate, and, in some embodiments, other physiological parameters such as pulse occurrence, plethysmograph features and measurement confidence. These parameters 318 are output from the waveform generator 320. A portion of these parameters may also be used to generate display drive signals 316 so that patient status may be read from, for example, an LED or LCD display module 340 on the UPO.

The internal pulse oximeter 310 may be a conventional pulse oximeter or, for upgrading an external pulse oximeter 260, it may be an advanced pulse oximeter capable of low perfusion and motion artifact performance not found in conventional pulse oximeters. An advanced pulse oximeter for use as an internal pulse oximeter 310 is described in U.S. Pat. No. 5,632,272 assigned to the assignee of the present invention and incorporated herein by reference. An advanced pulse oximetry sensor for use as the sensor 110 attached to the internal pulse oximeter 310 is described in U.S. Pat. No. 5,638,818 assigned to the assignee of the present invention and incorporated herein by reference.



Further, a line of advanced Masimo SET® pulse oximeter OEM boards and sensors are available from the assignee of the present invention.

The waveform generator 320 synthesizes a waveform, such as a triangular waveform having a sawtooth or symmetric triangle shape, that is output as a modulated signal 324 in response to an input drive signal 322. The drive input 322 and modulation output 324 of the waveform generator 320 are connected to the sensor port 262 of the external pulse oximeter 260. The synthesized waveform is generated in a manner such that the external pulse oximeter 260 computes and displays a saturation and a pulse rate value that is equivalent to that measured by the internal pulse oximeter 310 and sensor 110. In the present embodiment, the waveforms for pulse oximetry are chosen to indicate to the external pulse oximeter 260 a perfusion level of 5%. The external pulse oximeter 260, therefore, always receives a strong signal. In an alternative embodiment, the perfusion level of the waveforms synthesized for the external pulse oximeter can be set to indicate a perfusion level at or close to the perfusion level of the patient being monitored by the internal pulse oximeter 310. As an alternative to the generated waveform, a digital data output 326, is connected to the data port 264 of the external pulse oximeter 260. In this manner, saturation and pulse rate measurements and also samples of the unmodulated, synthesized waveform can be communicated directly to the external pulse oximeter 260 for display, bypassing the external pulse oximeter's signal processing functions. The measured plethysmograph waveform samples output from the internal pulse oximeter 310 also may be communicated through the digital data output 326 to the external pulse oximeter 260.

It will be understood from the above discussion that the synthesized waveform is not physiological data from the patient being monitored by the internal pulse oximeter 310, but is a waveform synthesized from predetermined stored waveform data to cause the external pulse oximeter 260 to calculate oxygen saturation and pulse rate equivalent to or generally equivalent (within clinical significance) to that calculated by the internal pulse oximeter 310. The actual physiological waveform from the patient received by the detector is not provided to the external pulse oximeter 260 in the present embodiment. Indeed, the waveform provided to the external pulse oximeter will usually not resemble the plethysmographic waveform of physiological data from the patient being monitored by the internal pulse oximeter 310.

The cable 230 (FIG. 2) attached between the waveform generator 320 and external pulse oximeter 260 provides a monitor ID 328 to the UPO, allowing identification of predetermined external pulse oximeter calibration curves. For example, this cable may incorporate an encoding device, such as a resistor, or a memory device, such as a PROM 1010 (FIG. 10) that is read by the waveform generator 320. The encoding device provides a value that uniquely identifies a particular type of external pulse oximeter 260 having known calibration curve, LED drive and modulation signal characteristics. Although the calibration curves of the external pulse oximeter 260 are taken into account, the wavelengths of the actual sensor 110 need not correspond to the particular calibration curve indicated by the monitor ID 328 or otherwise assumed for the external pulse oximeter 260. That is, the wavelength of the sensor 110 attached to the internal pulse oximeter 310 is not relevant or known to the external pulse oximeter 260.

FIG. 4 illustrates one embodiment of the waveform generator portion 320 of the UPO 210 (FIG. 3). Although this illustration may suggest a hardware implementation, the

functions of the waveform generator may be implemented in software or firmware or a combination of hardware, software and firmware. The waveform generator 320 performs waveform synthesis with a waveform look-up table ("LUT") 410, a waveform shaper 420 and a waveform splitter 430. The waveform LUT 410 is advantageously a memory device, such as a ROM (read only memory) that contains samples of one or more waveform portions or segments containing a single waveform. These stored waveform segments may be as simple as a single period of a triangular waveform, having a sawtooth or symmetric triangle shape, or more complicated, such as a simulated plethysmographic pulse having various physiological features, for example rise time, fall time and dicrotic notch.

The waveform shaper 420 creates a continuous repeated waveform from the waveform segments provided by the waveform LUT 410. The waveform shaper 420 has a shape parameter input 422 and an event indicator input 424 that are buffered 470 from the parameters 318 output from the internal pulse oximeter 310 (FIG. 3). The shape parameter input 422 determines a particular waveform segment in the waveform LUT 410. The chosen waveform segment is specified by the first address transmitted to the waveform LUT 410 on the address lines 426. The selected waveform segment is sent to the waveform shaper 420 as a series of samples on the waveform data lines 412.

The event indicator input 424 specifies the occurrence of pulses in the plethysmograph waveform processed by the internal pulse oximeter 310 (FIG. 3). For example, the event indicator may be a delta time from the occurrence of a previously detected falling pulse edge or this indicator could be a real time or near real time indicator or flag of the pulse occurrence. The waveform shaper 420 accesses the waveform LUT 410 to create a corresponding delta time between pulses in the synthesized waveform output 428. In one embodiment, the waveform shaper is clocked at a predetermined sample rate. From a known number of samples per stored waveform segment and the input delta time from the event indicator, the waveform shaper 420 determines the number of sequential addresses to skip between samples and accesses the waveform LUT 410 accordingly. This effectively "stretches" or "shrinks" the retrieved waveform segment so as to fit in the time between two consecutive pulses detected by the UPO.

The waveform splitter 430 creates a first waveform 432 corresponding to a first waveform (such a red wavelength) expected by the external pulse oximeter 260 (FIG. 3) and a second waveform (such as infrared) 434 expected by the external pulse oximeter 260. The relative amplitudes of the first waveform 432 and second waveform 434 are adjusted to correspond to the ratio output 444 from a calibration curve LUT 440. Thus, for every value of measured oxygen saturation at the sat input 442, the calibration curve LUT 440 provides a corresponding ratio output 444 that results in the first waveform 432 and the second waveform 434 having an amplitude ratio that will be computed by the external pulse oximeter 260 (FIG. 3) as equivalent to the oxygen saturation measured by the internal pulse oximeter 310 (FIG. 3).

As described above, one particularly advantageous aspect of the UPO is that the operating wavelengths of the sensor 110 (FIG. 3) are not relevant to the operating wavelengths required by the external pulse oximeter 260 (FIG. 3), i.e. the operating wavelengths that correspond to the calibration curve or curves utilized by the external pulse oximeter. The calibration curve LUT 440 simply permits generation of a synthesized waveform as expected by the external oximeter 260 (FIG. 3) based on the calibration curve used by the

external pulse oximeter **260** (FIG. 3). The calibration curve LUT **440** contains data about the known calibration curve of the external pulse oximeter **260** (FIG. 3), as specified by the monitor ID input **328**. In other words, the waveform actually synthesized is not a patient plethysmographic waveform. It is merely a stored waveform that will cause the external pulse oximeter to calculate the proper oxygen saturation and pulse rate values. Although this does not provide a patient plethysmograph on the external pulse oximeter for the clinician, the calculated saturation and pulse rate values, which is what is actually sought, will be accurate.

A modulator **450** responds to an LED drive input **322** from the external pulse oximeter to generate a modulated waveform output **324** derived from the first waveform **432** and second waveform **434**. Also, a data communication interface **460** transmits as a digital data output **326** the data obtained from the sat **442**, pulse rate **462** and synthesized waveform **428** inputs.

FIG. 5 depicts a handheld UPO **500** embodiment. The handheld UPO **500** has keypad inputs **510**, an LCD display **520**, an external power supply input **530**, an output port **540** for connection to an external pulse oximeter and a sensor input **550** at the top edge (not visible). The display **520** shows the measured oxygen saturation **522**, the measured pulse rate **524**, a pulsating bar **526** synchronized with pulse rate or pulse events, and a confidence bar **528** indicating confidence in the measured values of saturation and pulse rate. Also shown are low battery **572** and alarm enabled **574** status indicators.

The handheld embodiment described in connection with FIG. 5 may also advantageously function in conjunction with a docking station that mechanically accepts, and electrically connects to, the handheld unit. The docking station may be co-located with a patient monitoring system and connected to a corresponding SpO<sub>2</sub> module sensor port, external power supply, printer and telemetry device, to name a few options. In this configuration, the handheld UPO may be removed from a first docking station at one location to accompany and continuously monitor a patient during transport to a second location. The handheld UPO can then be conveniently placed into a second docking station upon arrival at the second location, where the UPO measurements are displayed on the patient monitoring system at that location.

FIG. 6 shows a block diagram of a UPO embodiment, where the functions of the UPO **210** are split between a portable pulse oximeter **610** and a docking station **660**. The portable pulse oximeter **610** ("portable") is a battery operated, fully functional, stand-alone pulse oximeter instrument. The portable **610** connects to a sensor **110** (FIG. 2) through a UPO patient cable **220** (FIG. 2) attached to a patient cable connector **618**. The portable **610** provides the sensor **110** with a drive signal **612** that alternately activates the sensor's red and IR LEDs, as is well-known in the art. The portable also receives a corresponding detector signal **614** from the sensor. The portable can also input a sensor ID on the drive signal line **612**, as described in U.S. Pat. No. 5,758,644 entitled Manual and Automatic Probe Calibration, assigned to the assignee of the present invention and incorporated herein by reference.

The portable **610** can be installed into the docking station **660** to expand its functionality. When installed, the portable **610** can receive power **662** from the docking station **660** if the docking station **660** is connected to external power **668**. Alternately, with no external power **668** to the docking station **660**, the portable **610** can supply power **662** to the docking station **660**. The portable **610** communicates to the

docking station with a bi-directional serial data line **664**. In particular, the portable **610** provides the docking station with SpO<sub>2</sub>, pulse rate and related parameters computed from the sensor detector signal **614**. When the portable **610** is installed, the docking station **660** may drive a host instrument **260** (FIG. 2) external to the portable **610**. Alternatively, the portable **610** and docking station **660** combination may function as a standalone pulse oximeter instrument, as described below with respect to FIG. 13.

In one embodiment, the docking station **660** does not perform any action when the portable **610** is not docked. The user interface for the docking station **660**, i.e. keypad and display, is on the portable **610** in the present embodiment. An indicator LED on the docking station **660** is lit when the portable is docked. The docking station **660** generates a detector signal output **674** to the host instrument **260** (FIG. 2) in response to LED drive signals **672** from the host instrument and SpO<sub>2</sub> values and related parameters, received from the portable **610**. The docking station **660** also provides a serial data output **682**, a nurse call **684** and an analog output **688**.

An interface cable **690** connects the docking station **660** to the host instrument. The LED drive signals **672** and detector signal output **674** are communicated between the docking station **660** and the host instrument **260** (FIG. 2) via the interface cable **690**. The interface cable **690** provides a sync data output **692** to the docking station **660**, communicating sensor, host instrument (e.g. monitor ID **328**, FIG. 3) and calibration curve data. Advantageously, this data allows the docking station **660** to provide signals to a particular host instrument on which it can operate.

FIG. 7 provides further detail of the portable **610**. The portable components has a pulse oximeter processor **710**, a management processor **720**, a power supply **730**, a display **740** and a keypad **750**. The pulse oximeter processor **710** functions as an internal pulse oximeter, interfacing the portable to a sensor **110** (FIG. 2) and deriving SpO<sub>2</sub>, pulse rate, a plethysmograph and a pulse indicator. An advanced pulse oximeter for use as the pulse oximeter processor **710** is described in U.S. Pat. No. 5,632,272, referenced above. An advanced pulse oximetry sensor for use as the sensor **110** (FIG. 2) attached to the pulse oximeter processor **710** is described in U.S. Pat. No. 5,638,818, also referenced above. Further, a line of advanced Masimo SET® pulse oximeter OEM boards and sensors are available from the assignee of the present invention. In one embodiment, the pulse oximeter processor **710** is the Masimo SET® MS-3L board or a low power MS-5 board available from Masimo Corporation.

The management processor **720** controls the various functions of the portable **610**, including asynchronous serial data communications **724** with the pulse oximeter processor **710** and synchronous serial communications **762** with the docking station **660** (FIG. 6). The physical and electrical connection to the docking station **660** (FIG. 6) is via a docking station connector **763** and the docking station interface **760**, respectively. The processor **720** utilizes a real-time clock **702** to keep the current date and time, which includes time and date information that is stored along with SpO<sub>2</sub> parameters to create trend data. In one embodiment, the processor of the portable **610** and the docking station **660** (FIG. 6) can be from the same family of processors to share common routines and minimize code development time.

The processor **720** also controls the user interface **800** (FIG. 8A) by transferring display data **742** to the display **740**, including display updates and visual alarms, and by interpreting keystroke data **752** from the keypad **750**. The processor **720** generates various alarm signals, when

required, via an enable signal **728**, which controls a speaker driver **770**. The speaker driver **770** actuates a speaker **772**, which provides audible indications such as, for example, alarms and pulse beeps. The processor **720** also monitors system status, which includes battery status **736**, indicating battery levels, and docked status **764**, indicating whether the portable **610** is connected to the docking station **660** (FIG. 6). When the portable **610** is docked and is on, the processor **720** also decides when to turn on or off docking station power **732**.

Advantageously, the caregiver can set (i.e. configure or program) the behavior of the portable display **740** and alarms when the docked portable **610** senses that an interface cable **690** has connected the docking station **660** to an external pulse oximeter, such as a multiparameter patient monitoring system. In one user setting, for example, the portable display **740** stops showing the SpO<sub>2</sub> **811** (FIG. 8) and pulse rate **813** (FIG. 8) values when connected to an external pulse oximeter to avoid confusing the caregiver, who can read equivalent values on the patient monitoring system. The display **740**, however, continues to show the plethysmograph **815** (FIG. 8) and visual pulse indicator **817** (FIG. 8) waveforms. For one such user setting, the portable alarms remain active.

Another task of the processor **720** includes maintenance of a watchdog function. The watchdog **780** monitors processor status on the watchdog data input **782** and asserts the reset output **784** if a fault is detected. This resets the management processor **720**, and the fault is indicated with audible and visual alarms.

The portable **610** gets its power from batteries in the power supply **730** or from power **766** supplied from the docking station **660** (FIG. 6) via the docking station interface **760**. A power manager **790** monitors the on/off switch on the keypad **750** and turns-on the portable power accordingly. The power manager **790** turns off the portable on command by the processor **720**. DC/DC converters within the power supply **730** generate the required voltages **738** for operation of the portable **610** and docking station power **732**. The portable batteries are preferably rechargeable batteries or another renewable power source. The batteries of the power supply **730** supply docking station power **732** when the docking station **660** (FIG. 6) is without external power. A battery charger within the docking station power supply provides charging current **768** to rechargeable batteries within the power supply **730**. The docking station power supply **990** (FIG. 9) monitors temperature **734** from a thermistor in the rechargeable battery pack, providing an indication of battery charge status.

A non-volatile memory **706** is connected to the management processor **720** via a high-speed bus **722**. In the present embodiment, the memory **706** is an erasable and field re-programmable device used to store boot data, manufacturing serial numbers, diagnostic failure history, adult SpO<sub>2</sub> and pulse rate alarm limits, neonate SpO<sub>2</sub> and pulse rate alarm limits, SpO<sub>2</sub> and pulse rate trend data, and program data. Other types of non-volatile memory are well known. The SpO<sub>2</sub> and pulse rate alarm limits, as well as SpO<sub>2</sub> related algorithm parameters, may be automatically selected based on the type of sensor **110** (FIG. 2), adult or neonate, connected to the portable **610**.

The LCD display **740** employs LEDs for a backlight to increase its contrast ratio and viewing distance when in a dark environment. The intensity of the backlight is determined by the power source for the portable **610**. When the portable **610** is powered by either a battery pack within its power supply **730** or a battery pack in the docking station

power supply **990** (FIG. 9), the backlight intensity is at a minimum level. When the portable **610** is powered by external power **668** (FIG. 6), the backlight is at a higher intensity to increase viewing distance and angle. In one embodiment, a button on the portable permits overriding these intensity settings, and provides adjustment of the intensity. The backlight is controlled in two ways. Whenever any key is pressed, the backlight is illuminated for a fixed number of seconds and then turns off, except when the portable is docked and derives power from an external source. In that case, the backlight is normally on unless deactivated with a key on the portable **610**.

FIG. 8A illustrates the portable user interface **800**, which includes a display **740** and a keypad **750**. In one embodiment, the display **740** is an LCD device having **160** pixels by **480** pixels. The display **740** can be shown in portrait mode, illustrated in FIG. 8B, or in landscape mode, illustrated in FIG. 8C. A tilt (orientation) sensor **950** (FIG. 9) in the docking station **660** (FIG. 6) or a display mode key on the portable **610** (FIG. 6) determines portrait or landscape mode. The tilt sensor **950** (FIG. 9) can be a gravity-activated switch or other device responsive to orientation and can be alternatively located in the portable **610** (FIG. 6). In a particular embodiment, the tilt sensor **950** (FIG. 9) is a non-mercury tilt switch, part number CW 1300-1, available from Comus International, Nutley, N.J. (www.comus-intl.com). The tilt sensor **950** (FIG. 9) could also be a mercury tilt switch.

Examples of how the display area can be used to display SpO<sub>2</sub> **811**, pulse rate **813**, a plethysmographic waveform **815**, a visual pulse indicator **817** and soft key icons **820** in portrait and landscape mode are shown in FIGS. 8B and 8C, respectively. The software program of the management processor **720** (FIG. 7) can be easily changed to modify the category, layout and size of the display information shown in FIGS. 8B-C. Other advantageous information for display is SpO<sub>2</sub> limits, alarm limits, alarm disabled, exception messages and battery status.

The keypad **750** includes soft keys **870** and fixed keys **880**. The fixed keys **880** each have a fixed function. The soft keys **870** each have a function that is programmable and indicated by one of the soft key icons **820** located next to the soft keys **870**. That is, a particular one of the soft key icons **820** is in proximity to a particular one of the soft keys **870** and has a text or a shape that suggests the function of that particular one of the soft keys **870**. In one embodiment, the button portion of each key of the keypad **750** is constructed of florescent material so that the keys **870**, **880** are visible in the dark.

In one embodiment, the keypad **750** has one row of four soft keys **870** and one row of three fixed keys **880**. Other configurations are, of course, available, and specific arrangement is not significant. In one embodiment, the functions of the three fixed keys **880** are power, alarm silence and light/contrast. The power function is an on/off toggle button. The alarm silence function and the light/contrast function have dual purposes depending on the duration of the key press. A momentary press of the key corresponding to the alarm silence function will disable the audible alarm for a fixed period of time. To disable the audible alarm indefinitely, the key corresponding to the alarm silence function is held down for a specified length of time. If the key corresponding to the alarm silence function is pressed while the audible alarm has been silenced, the audible alarm is reactivated. If the key corresponding to the light/contrast function is pressed momentarily, it is an on/off toggle button for

the backlight. If the key corresponding to the light/contrast function is held down, the display contrast cycles through its possible values.

In the present embodiment, the default functions of the four soft keys **870** are pulse beep up volume, pulse beep down volume, menu select, and display mode. These functions are indicated on the display by the up arrow, down arrow, "menu" and curved arrow soft key icons **820**, respectively. The up volume and down volume functions increase or decrease the audible sound or "beep" associated with each detected pulse. The display mode function rotates the display **740** through all four orthogonal orientations, including portrait mode (FIG. **8B**) and landscape mode (FIG. **8C**), with each press of the corresponding key. The menu select function allows the functionality of the soft keys **870** to change from the default functions described above. Examples of additional soft key functions that can be selected using this menu feature are set SpO<sub>2</sub> high/low limit, set pulse rate high/low limit, set alarm volume levels, set display to show trend data, print trend data, erase trend data, set averaging time, set sensitivity mode, perform synchronization, perform rechargeable battery maintenance (deep discharge/recharge to remove battery memory), and display product version number.

FIG. **9** provides further details of the docking station **660**, which includes a docking station processor **910**, a non-volatile memory **920**, a waveform generator **930**, a PROM interface **940**, a tilt sensor **950**, a portable interface **970** and associated connector **972**, status indicators **982**, a serial data port **682**, a nurse call output **684**, an analog output **688** and a power supply **990**. In one embodiment, the docking station **660** is intended to be associated with a fixed (non-transportable) host instrument, such as a multiparameter patient monitoring instrument in a hospital emergency room. In a transportable embodiment, the docking station **660** is movable, and includes a battery pack within the power supply **990**.

The docking station processor **910** orchestrates the activity on the docking station **660**. The processor **910** provides the waveform generator **930** with parameters **932** as discussed above for FIGS. **3** and **4**. The processor **910** also provides asynchronous serial data **912** for communications with external devices and synchronous serial data **971** for communications with the portable **610** (FIG. **6**). In addition, the processor **910** determines system status including sync status **942**, tilt status **952** and power status **992**. The portable management processor **720** (FIG. **7**) performs the watchdog function for the docking station processor **910**. The docking station processor **910** sends watchdog messages to the portable processor **720** (FIG. **7**) as part of the synchronous serial data **972** to ensure the correct operation of the docking station processor **910**.

The docking station processor **910** can also perform resource downloading to the portable processor **720** (FIG. **7**) as part of the synchronous serial data **971**. That is, the docking station **660** can provide functionality not present in the portable **610** (FIG. **6**), and, when docked, that added capability can be reflected by the portable user interface, i.e. the soft keys **870** (FIG. **8A**) and the display **740** (FIG. **8A**). For example, a portable **610** (FIG. **6**) providing only pulse oximetry measurements can be docked to a docking station **660** having the added functionality of blood pressure measurements. The docking station **660** can download a blood pressure measurement menu and an associated user interface to the portable **610** (FIG. **6**) upon docking, allowing the portable **610** (FIG. **6**) to control and display this additional docking station functionality. Docking station resource

downloading would apply to other physiological measurements as well, such as respiration rate, EEG, ECG and EtCO<sub>2</sub> to name a few.

The docking station processor **910** accesses non-volatile memory **920** over a high-speed bus **922**. The non-volatile memory **920** is re-programmable and contains program data for the processor **910** including instrument communication protocols, synchronization information, a boot image, manufacturing history and diagnostic failure history.

The waveform generator **930** generates a synthesized waveform that a conventional pulse oximeter can process to calculate SpO<sub>2</sub> and pulse rate values or exception messages, as described above with respect to FIG. **4**. However, in the present embodiment, as explained above, the waveform generator output does not reflect a physiological waveform. It is merely a waveform constructed from stored memory data to cause the external pulse oximeter to calculate the correct saturation and pulse rate. In an alternative arrangement, physiological data could be scaled or otherwise mathematically converted and provided to the external pulse oximeter, but the external pulse oximeter would often not be able to calculate the proper saturation values, and the upgrading feature would be lost. This is particularly true due to the likely mismatch in the actual sensor wavelength and the calibration curves in the external pulse oximeter. The waveform generator **930** is enabled if an interface cable **690** (FIG. **6**), described below with respect to FIG. **10**, with valid synchronization information is connected. Otherwise, the power to the waveform generator **930** is disabled, thereby rendering the waveform generator inoperable.

The status indicators **982** are a set of LEDs on the front of the docking station **660** used to indicate various conditions including external power (AC), portable docked, portable battery charging, docking station battery charging and alarm. The serial data port **682** is used to interface with either a computer, a serial port of conventional pulse oximeters or serial printers via a standard RS-232 DB-9 connector **962**. This port **682** can output trend memory, SpO<sub>2</sub> and pulse rate and support the system protocols of various manufacturers. The analog output **688** is used to interface with analog input chart recorders via a connector **964** and can output "real-time" or trend SpO<sub>2</sub> and pulse rate data. The nurse call output **684** from a connector **964** is activated when alarm limits are exceeded for a predetermined number of consecutive seconds. In another embodiment, data, including alarms, could be routed to any number of communications ports, and even over the Internet, to permit remote use of the upgrading pulse oximeter.

The PROM interface **940** accesses synchronization data **692** from the PROM **1010** (FIG. **10**) in the interface cable **690** (FIGS. **6**, **10**) and provides synchronization status **942** to the docking station processor **910**. The portable interface **970** provides the interconnection to the portable **610** (FIG. **6**) through the docking station interface **760** (FIG. **7**).

As shown in FIG. **9**, external power **668** is provided to the docking station **660** through a standard AC connector **968** and on/off switch **969**. When the docking station **660** has external power **668**, the power supply **990** charges the battery in the portable power supply **730** (FIG. **7**) and the battery, if any, in the docking station power supply **990**. When the portable **610** (FIG. **6**) is either removed or turned off, the docking station power **973** is removed and the docking station **660** is turned off, except for the battery charger portion of the power supply **990**. The docking station power **973** and, hence, the docking station **660** powers on whenever a docked portable **610** (FIG. **6**) is switched on. The portable **610** (FIG. **6**) supplies power for

an embodiment of the docking station **660** without a battery when external power **668** is removed or fails.

FIG. **10** provides further detail regarding the interface cable **690** used to connect between the docking station **660** (FIG. **6**) and the host instrument **260** (FIG. **2**). The interface cable **690** is configured to interface to a specific host instrument via the sensor input to the host instrument. A PROM **1010** built into the interface cable **690** contains information identifying a sensor type, a specific host instrument, and the calibration data (if necessary) of the specific host instrument. This PROM information can be read by the docking station **660** (FIG. **6**) as synchronization data **692**. Advantageously, the synchronization data **692** allows the docking station **660** (FIG. **6**) to generate a waveform to the host instrument that causes the host instrument to display SpO<sub>2</sub> values equivalent to those calculated by the portable **610** (FIG. **6**). The interface cable **690** includes an LED drive path **672**. In the embodiment shown in FIG. **10**, the LED drive path **672** is configured for common anode LEDs and includes IR cathode, red cathode and common anode signals. The interface cable **690** also includes a detector drive path **674**, including detector anode and detector cathode signals.

A menu option on the portable **610** (FIG. **6**) also allows synchronization information to be calculated in the field. With manual synchronization, the docking station **660** (FIG. **6**) generates a waveform to the host instrument **260** (FIG. **2**) and displays an expected SpO<sub>2</sub> value. The user enters into the portable the SpO<sub>2</sub> value displayed on the host instrument using the portable keypad **750** (FIG. **7**). These steps are repeated until a predetermined number of data points are entered and the SpO<sub>2</sub> values displayed by the portable and the host instrument are consistent.

FIGS. **11A-B** depict an embodiment of the portable **610**, as described above with respect to FIG. **6**. FIGS. **12A-B** depict an embodiment of the docking station **660**, as described above with respect to FIG. **6**. FIG. **13** depicts an embodiment of the UPO **210** where the portable **610** is docked with the docking station **660**, also as described above with respect to FIG. **6**.

FIG. **11A** depicts the portable front panel **1110**. The portable **610** has a patient cable connector **618**, as described above with respect to FIG. **6**. Advantageously, the connector **618** is rotatably mounted so as to minimize stress on an attached patient cable (not shown). In one embodiment, the connector **618** can freely swivel between a plane parallel to the front panel **1110** and a plane parallel to the side panel **1130**. In another embodiment, the connector **618** can swivel between, and be releasably retained in, three semi-locked positions. The connector **618** can be rotated from a semi-locked position with moderate force. A first locked position is as shown, where the connector is in a plane parallel to the front panel **1110**. A second locked position is where the connector **618** is in a plane parallel to the side panel **1130**. The connector **618** also has an intermediate locked position 45° between the first and the second locked positions. The connector **618** is placed in the first locked position for attachment to the docking station **660**.

Shown in FIG. **11A**, the portable front panel **1110** also has a speaker **772**, as described with respect to FIG. **7**. Further, the front panel **1110** has a row of soft keys **870** and fixed keys **880**, as described above with respect to FIG. **8**. In addition, the front panel **1110** has a finger actuated latch **1120** that locks onto a corresponding catch **1244** (FIG. **12A**) in the docking station **660**, allowing the portable **610** to be

releasably retained by the docking station **660**. An OEM label can be affixed to a recessed area **1112** on the front panel **1110**.

FIG. **11B** depicts the portable back panel **1140**. The back panel **1140** has a socket **763**, a pole clamp mating surface **1160**, and a battery pack compartment **1170**. The socket **763** is configured to mate with a corresponding docking station plug **972** (FIG. **12A**). The socket **763** and plug **972** (FIG. **12A**) provide the electrical connection interface between the portable **610** and the docking station **660** (FIG. **12A**). The socket **763** houses multiple spring contacts that compress against plated edge-connector portions of the docking station plug **972** (FIG. **12A**). A conventional pole clamp (not shown) may be removably attached to the mating surface **1160**. This conveniently allows the portable **610** to be held to various patient-side or bedside mounts for hands-free pulse oximetry monitoring. The portable power supply **730** (FIG. **7**) is contained within the battery pack compartment **1170**. The compartment **1170** has a removable cover **1172** for protection, insertion and removal of the portable battery pack. Product labels, such as a serial number identifying a particular portable, can be affixed with the back panel indent **1142**.

FIG. **12A** depicts the front side **1210** of the docking station **660**. The front side **1210** has a docking compartment **1220**, a pole clamp recess **1230**, pivots **1242**, a catch **1244**, a plug connector **972** and LED status indicators **982**. The docking compartment **1220** accepts and retains the portable **610** (FIGS. **11A-B**), as shown in FIG. **13**. When the portable **610** (FIGS. **11A-B**) is docked in the compartment **1220**, the pole clamp recess **1230** accommodates a pole clamp (not shown) attached to the portable's pole clamp mating surface **1160** (FIG. **11B**), assuming the pole clamp is in its closed position. The portable **610** (FIGS. **11A-B**) is retained in the compartment **1220** by pivots **1242** that fit into corresponding holes in the portable's side face **1130** and a catch **1244** that engages the portable's latch **1120** (FIG. **11A**). Thus, the portable **610** (FIGS. **11A-B**) is docked by first attaching it at one end to the pivots **1242**, then rotating it about the pivots **1242** into the compartment **1220**, where it is latched in place on the catch **1244**. The portable **610** (FIGS. **11A-B**) is undocked in reverse order, by first pressing the latch **1120** (FIG. **11A**), which releases the portable from the catch **1244**, rotating the portable **610** (FIGS. **11A-B**) about the pivots **1242** out of the compartment **1220** and then removing it from the pivots **1242**. As the portable is rotated into the compartment, the docking station plug **972** inserts into the portable socket **763** (FIG. **11B**), providing the electrical interface between the portable **610** and the docking station **660**. The status indicators **982** are as described above with respect to FIG. **9**.

FIG. **12B** depicts the back side **1260** of the docking station **660**. The back side **1260** has a serial (RS-232 or USB) connector **962**, an analog output and nurse call connector **964**, an upgrade port connector **966**, an AC power plug **968**, an on/off switch **969** and a ground lug **1162**. A handle **1180** is provided at one end and fan vents **1170** are provided at the opposite end. A pair of feet **1190** are visible near the back side **1260**. A corresponding pair of feet (not visible) are located near the front side **1210** (FIG. **12A**). The feet near the front side **1210** extend so as to tilt the front side **1210** (FIG. **12A**) upward, making the display **740** (FIG. **13**) of a docked portable **610** (FIG. **13**) easier to read.

FIG. **13** illustrates both the portable **610** and the docking station **660**. The portable **610** and docking station **660** constitute three distinct pulse oximetry instruments. First, the portable **610** by itself, as depicted in FIGS. **11A-B**, is a

handheld pulse oximeter applicable to various patient monitoring tasks requiring battery power or significant mobility, such as ambulance and ER situations. Second, the portable **610** docked in the docking station **660**, as depicted in FIG. **13**, is a standalone pulse oximeter applicable to a wide-range of typical patient monitoring situations from hospital room to the operating room. Third, the portable **610** docked and the upgrade port **966** (FIG. **12B**) connected with an interface cable to the sensor port of a conventional pulse oximeter module **260** (FIG. **2**) within a multiparameter patient monitoring instrument **250** (FIG. **2**) or other conventional pulse oximeter, is a universal/upgrading pulse oximeter (UPO) instrument **210**, as described herein. Thus, the portable **610** and docking station **660** configuration of the UPO **210** advantageously provides a three-in-one pulse oximetry instrument functionality.

Another embodiment of the docking station **660** incorporates an input port that connects to a blood pressure sensor and an output port that connects to the blood pressure sensor port of a multiparameter patient monitoring system (MPMS). The docking station **660** incorporates a signal processor that computes a blood pressure measurement based upon an input from the blood pressure sensor. The docking station **660** also incorporates a waveform generator connected to the output port that produces a synthesized waveform based upon the computed measurement. The waveform generator output is adjustable so that the blood pressure value displayed on the MPMS is equivalent to the computed blood pressure measurement. Further, when the portable **610** is docked in the docking station **660** and the blood pressure sensor is connected to the input port, the portable displays a blood pressure value according to the computed blood pressure measurement. Thus, in this embodiment, the docking station **660** provides universal/upgrading capability for both blood pressure and SpO<sub>2</sub>.

Likewise, the docking station **660** can function as an universal/upgrading instrument for other vital sign measurements, such as respiratory rate, EKG or EEG. For this embodiment, the docking station **660** incorporates related sensor connectors and associated sensor signal processors and upgrade connectors to an MPMS or standalone instrument. In this manner, a variety of vital sign measurements can be incorporated into the docking station **660**, either individually or in combination, with or without SpO<sub>2</sub> as a measurement parameter, and with or without the portable **610**. In yet another embodiment, the docking station **660** can be configured as a simple SpO<sub>2</sub> upgrade box, incorporating a SpO<sub>2</sub> processor and patient cable connector for an SpO<sub>2</sub> sensor that functions with or without the portable **610**.

Unlike a conventional standalone pulse oximeter, the standalone configuration shown in FIG. **13** has a rotatable display **740** that allows the instrument to be operated in either a vertical or horizontal orientation. A tilt sensor **950** (FIG. **9**) indicates when the bottom face **1310** is placed along a horizontal surface or is otherwise horizontally-oriented. In this horizontal orientation, the display **740** appears in landscape mode (FIG. **8C**). The tilt sensor **950** (FIG. **9**) also indicates when the side face **1320** is placed along a horizontal surface or is otherwise horizontally oriented. In this vertical orientation, the display **740** appears in portrait mode (FIG. **8B**). A soft key **870** on the portable **610** can override the tilt sensor, allowing the display to be presented at any 90° orientation, i.e. portrait, landscape, "upside-down" portrait or "upside-down" landscape orientations. The handheld configuration (FIG. **11A**), can also present the display **740** at any 90° orientation using a soft key **870**. In the particular embodiment described above, however, the portable **610**

does not have a separate tilt sensor and, hence, relies on a soft key **870** to change the orientation of the display when not docked.

FIG. **14** illustrates the docking station **660** incorporated within a local area network (LAN). The LAN shown is Ethernet-based **1460**, using a central LAN server **1420** to interconnect various LAN clients **1430** and other system resources such as printers and storage (not shown). In this embodiment, an Ethernet controller module **1410** is incorporated with the docking station **660**. The controller module **1410** can be incorporated within the docking station **660** housing or constructed as an external unit. In this manner, the UPO, according to the present invention, can communicate with other devices on the LAN or over the Internet **1490**.

The Ethernet controller module **1410** can be embedded with web server firmware, such as the Hewlett-Packard (HP) BFOOT-10501. The module **1410** has both a 10 Base-T Ethernet interface for connection to the Ethernet **1460** and a serial interface, such as RS-232 or USB, for connection to the docking station **660**. The module firmware incorporates HTTP and TCP/IP protocols for standard communications over the World Wide Web. The firmware also incorporates a micro web server that allows custom web pages to be served to remote clients over the Internet, for example. Custom C++ programming allows expanded capabilities such as data reduction, event detection and dynamic web page configuration.

As shown in FIG. **14**, there are many applications for the docking station **660** to Ethernet interface. Multiple UPOs can be connected to a hospital's LAN, and a computer on the LAN could be utilized to upload pulse rate and saturation data from the various UPOs, displaying the results. Thus, this Ethernet interface could be used to implement a central pulse oximetry monitoring station within a hospital. Further, multiple UPOs from anywhere in the world can be monitored from a central location via the Internet. Each UPO is addressable as an individual web site and downloads web pages viewable on a standard browser, the web pages displaying oxygen saturation, pulse rate and related physiological measurements from the UPO. This feature allows a caregiver to monitor a patient regardless of where the patient or caregiver is located. For example a caregiver located at home in one city or at a particular hospital could download measurements from a patient located at home in a different city or at the same or a different hospital. Other applications include troubleshooting newly installed UPOs or uploading software patches or upgrades to UPOs via the Internet. In addition alarms could be forwarded to the URL of the clinician monitoring the patient.

The UPO may have other configurations besides the handheld unit described in connection with FIG. **5** or the portable **610** and docking station **660** combination described in connection with FIGS. **11-13**. The UPO may be a module, with or without a display, that can be removably fastened to a patient via an arm strap, necklace or similar means. In a smaller embodiment, this UPO module may be integrated into a cable or connector used for attaching a sensor to a pulse oximeter. The UPO may also be a circuit card or module that can externally or internally plug into or mate with a standalone pulse oximeter or multiparameter patient monitoring system. Alternatively, the UPO may be configured as a simple standalone upgrade instrument.

FIG. **15** illustrates a UPO configuration utilizing a patient care bed **1500**. The bed **1500** includes a bed frame and mattress **1502**, lower rails **1506** and upper rails **1508**. One of the upper rails **1508** incorporates an instrument panel **1510**

and the docking station **1540** is incorporated into the instrument panel **1510** according to the present invention. The instrument panel **1510** typically has keypad controls **1520**, a display **1530**, and a power supply **1550**. The power supply **1550** has a power cord **1552** that plugs into an AC power source. The docking station **1540** includes a docking station compartment that accepts and electrically connects to the portable **610**. In this manner, UPO can monitor a patient as a portable **610** during transport and then dock at the patient's destination as an integral part of the bedside instrument panel **1510**.

FIG. **16** is block diagram of the instrument panel **1510** and incorporated docking station **1540**. The instrument panel **1510** has a processor **1694**, which, in conjunction with a display driver **1696** and a keypad interface **1697**, drives the display **1530** and receives commands from the keypad controls **1520**. The processor **1694** also communicates with a docked portable **610** (FIG. **6**) via the docking station interface **1691** and a portable connector **1610** within the docking station receptacle. In one embodiment, the docking station **1540** simply provides a communications path and a DC power path between the docked portable **610** (FIG. **6**) and the instrument panel **1510** via the portable connector **1610** and the docking station interface **1690**. In that embodiment, the portable management processor **720** (FIG. **7**) is programmed with the communications protocol of the instrument panel processor **1694**. In another embodiment, the docking station **1540** provides communications and upgrade capability in a manner similar to that shown in FIG. **9**. In that embodiment, the bed-integrated UPO could also connect to and upgrade a MPMS pulse oximeter module **260** (FIG. **2**) or other external pulse oximeter located near the patient bed **1500**, in a manner as described with respect to FIG. **2**, above.

Although a universal/upgrading apparatus and method have been mainly described in terms of a pulse oximetry measurement embodiment, the present invention is equally applicable to other physiological measurement parameters such as blood pressure, respiration rate, EEG, ECG and EtCO<sub>2</sub> (capnography) to name a few. In addition, a universal/upgrading instrument having a single physiological measurement parameter or a multiple measurement parameter capability and configured as a handheld, standalone, portable, docking station, module, plug-in, circuit card, to name a few, is also within the scope of the present invention.

FIGS. **17A-B** illustrate one embodiment of a dual-mode pulse oximeter module according to the present invention. As shown in FIG. **17A**, a dual-mode pulse oximeter module **1700** is contained within a case **1710** having dimensions that conform to a multiparameter patient monitoring system (MPMS) slot **290** (FIG. **2**). The dual-mode module **1700** has a display **1720**, a keypad **1730**, and a patient cable connector **1740**. A module connector **1750** (FIG. **17B**) mates and electrically connects with a corresponding backplane connector (not shown) within an MPMS slot **292** (FIG. **2**).

In reference to FIGS. **17A-B**, the dual-mode pulse oximeter module **1700** has a portable mode, separate from MPMS **250** (FIG. **2**), and an integrated mode, plugged into an MPMS slot **292** (FIG. **2**). In the portable mode, the pulse oximeter module **1700** functions as a handheld or standalone pulse oximeter, in a manner similar to that described with respect to FIG. **6**, above. Specifically, the portable module **1700** is a battery-powered, pulse oximeter instrument. The portable module **1700** connects to a sensor through a patient cable attached to the patient cable connector **1740**. The module **1700** provides the sensor with a drive signal that alternately activates the sensor's red and IR LEDs, as is

well-known in the art. The pulse oximeter module **1700** also receives a corresponding photo-plethysmographic detector signal from the sensor, also well-known in the art. The portable module **1700** processes this sensor signal to derive oxygen saturation and pulse rate measurements. In the portable mode, this information is provided on the module display **1720**, and a keypad **1730** provides a user interface for operational control of the portable module **1700**.

Also in reference to FIGS. **17A-B**, in the integrated mode, the pulse oximeter module **1700** is a plug-in module that functions in conjunction with the MPMS **250** (FIG. **2**). When installed in a MPMS slot **290** (FIG. **2**), the integrated module **1700** receives power from the MPMS **250** (FIG. **2**), drives a sensor, receives a corresponding photo-plethysmographic sensor signal, and processes this sensor signal to derive oxygen saturation and pulse rate measurements, as described with respect to the portable mode, above. The integrated module **1700**, however, communicates oxygen saturation, pulse rate and related measurements to the MPMS **250** (FIG. **2**) via the module connector **1750**. Typically, the integrated module display **1720** and keypad **1730** are disabled, and the MPMS monitor **280** (FIG. **2**) displays the physiological measurements made by the integrated module **1700**.

FIG. **18** is a block diagram of the dual-mode pulse oximeter module **1700**. The pulse oximeter module **1700** includes a pulse oximeter processor **1810**, management processor **1820**, power supply **1830**, power manager **1840**, keypad interface **1850**, speaker driver **1860**, display driver **1870**, clock **1802**, watch dog timer **1804**, and MPMS interface **1880**. These components function in a manner similar to that described with respect to FIG. **7**, above. Specifically, the pulse oximeter processor **1810** functions as an internal pulse oximeter, interfacing the pulse oximeter module **1700** to a sensor and deriving oxygen saturation, pulse rate, a plethysmograph and a pulse indicator.

As shown in FIG. **18**, the management processor **1820** controls the various functions of the pulse oximeter module **1700**, including data communications with the pulse oximeter processor **1810** and communications with the MPMS **250** via the MPMS interface **1880**. The physical connection to the MPMS **250** is via the module connector **1750** (FIG. **17B**) and a corresponding MPMS backplane connector. The electrical connection is via a module interface **1898**. The management processor **1820** utilizes a real-time clock **1802** to keep the current date and time, which includes time and date information that is stored in nonvolatile memory **1806** along with oxygen saturation related parameters to create trend data. The management processor **1820** also controls a user interface by transferring data to a display driver **1870** and from a keypad interface **1850**. The management processor **1820** generates various alarm signals, which control a speaker driver **1860**. The management processor **1820** also monitors system status, which includes battery status, indicating battery levels, and plug-in status, indicating whether the pulse oximeter module **1700** is connected to the MPMS **250**. Another task of the management processor **1820** includes maintenance of a watchdog function. A watchdog **1804** monitors processor status on the watchdog data input and asserts a management processor reset if a fault is detected, along with audible and visual alarms.

Also shown in FIG. **18**, the pulse oximeter module **1700** gets its power from batteries in the power supply **1830** or from power supplied on line **1884** from the MPMS **250** via the MPMS interface **1880**. A power manager **1840** monitors the keypad on/off switch via the keypad interface **1850** and turns-on module power **1830** accordingly. The power man-



ager **1840** turns off module power **1830** on command by the management processor **1820**. DC/DC converters within the power supply **1830** generate the required voltages for module operation. A battery charger within the module power supply **1830** provides charging current to recharge the internal batteries. A non-volatile memory **1806** is connected to the management processor **1820** and used to store boot data, alarm limits trend data and program data.

FIG. **19** illustrates another embodiment of a dual-mode pulse oximeter according to the present invention. A docking station module **1900** has a docking portion **1910** and a plug-in portion **1920**. The docking portion **1910** has a docking compartment **1930** and a portable socket **1940**. The docking compartment **1930** is configured to accept and retain a portable pulse oximeter **610**, such as described with respect to FIGS. **6** and **11A-B**, above. In particular, the portable **610** has a socket **763** (FIG. **11B**) that mates with a corresponding plug **1940**, providing an electrical connection between the portable pulse oximeter **610** and the docking station module **1900**. The plug-in portion **1920** has dimensions that conform to an MPMS slot **290** (FIG. **2**). A module connector similar to that of the pulse oximeter module connector **1750** (FIG. **17B**) mates and electrically connects with a corresponding backplane connector (not shown) within an MPMS slot **290** (FIG. **2**).

In reference to FIG. **19**, the docking station module **1900** allows the portable **610** to function as a dual-mode pulse oximeter. That is, the portable **610** has a portable mode separate from the MPMS **250** (FIG. **2**) and an integrated mode connected to an MPMS slot **290** (FIG. **2**) via the docking station module **1900**. In this manner, the portable **610** functions much as the dual-mode module **1700** (FIGS. **17A-B**) described with respect to FIGS. **17A-B**, above. In the portable mode, the portable **610** functions as a handheld or standalone pulse oximeter as described with respect to FIG. **6**, above. In the integrated mode, the portable **610** is docked to the docking station module **1900** and functions in conjunction with the MPMS **250** (FIG. **2**). When installed in an MPMS slot **290** (FIG. **2**), the portable receives power from a MPMS **250** (FIG. **2**), drives a sensor, receives a corresponding photo-plethysmographic sensor signal, and processes this sensor signal to derive oxygen saturation and pulse rate measurements, as described with respect to FIG. **6**, above. The integrated portable **610**, however, communicates oxygen saturation, pulse rate and related measurements to the MPMS **250** (FIG. **2**) via the docking station module **1900**, as described below. Typically, the portable display **740** and keys **750** are disabled, and the MPMS monitor **280** (FIG. **2**) controls and displays the physiological measurements made by the integrated portable **610**.

Also in reference to FIG. **19**, in an alternative embodiment, the docking compartment **1930** is configured to accept and retain a pulse oximeter module **1700** (FIGS. **17A-B**). In that embodiment, the docking compartment **1930** has a docking connector (not shown) that mates with the module connector **1750** (FIG. **17B**), providing an electrical connection between the pulse oximeter module **1700** (FIGS. **17A-B**) and the docking station module **1900**.

FIG. **20** illustrates the docking station module **1900** attached to the MPMS **250**. The plug-in portion **1920** (FIG. **19**) plugs into at least one of the MPMS slots **290** (FIG. **2**) and electrically connects to the MPMS backplane as described with respect to FIG. **19**, above. In the portable mode (shown), the portable pulse oximeter **610** functions in a manner similar to the portable module **1700** (FIGS. **17A-B**), i.e. as handheld or standalone pulse oximeter. In the integrated mode, the portable **610** is installed into the

docking compartment **1930**, providing an electrical connection and communications interface between the MPMS **250** and the portable pulse oximeter **610**. In the integrated mode, the combination of the portable pulse oximeter **610** and the docking station module **1900** functions in a manner similar to the integrated module **1700** (FIGS. **17A-B**).

FIG. **21** is a block diagram of a pass-through embodiment of a docking station module **1900**, which includes a portable connector **2110**, an MPMS connector **2160** and a direct electrical path between the two connectors **2110**, **2160**. In this embodiment, the docking station module **1900** simply provides a physical interface between the portable **610** (FIG. **20**) and the MPMS **250**. A MPMS communications path **1882** is directly routed to the portable communications path **2112**. MPMS power **1884** is also directly routed to the portable input power line **2114**. The docking station module **1900**, with various configurations of the plug-in portion **1920** (FIG. **19**) and associated module connector can be adapted to the slots **290** (FIG. **2**) of various MPMS manufacturers. In this manner, the docking station module **1900** can function as a universal interface between the portable pulse oximeter **610** or, alternatively, the pulse oximeter module **1700** and various multiparameter patient monitoring systems.

FIG. **22** is a block diagram of another embodiment of a docking station module **1900a**, which includes a portable interface **2210**, docking station processor **2220**, power supply **2230** and monitor interface **2260**. These components function in a manner similar to that described with respect to FIG. **9**, above. Specifically, the docking station processor **2220** orchestrates the activity of the docking station module **1900**. The processor **2220** provides synchronous serial data for communications with the portable **610** (FIG. **6**) and sends watchdog messages to the portable processor **720** (FIG. **7**) as part of the synchronous serial data to ensure the correct operation of the docking station processor **2220**. The docking station processor **2220** accesses non-volatile, re-programmable memory **2206** over a high-speed bus to obtain program data for the processor **2220**. In one embodiment, the status display **2240** is a set of LEDs on the front of the docking station module **1900** used to indicate various conditions including portable docked, portable battery charging and alarm. The portable interface **2210** interconnects with the docking station interface **760** (FIG. **7**) of the portable **610** (FIG. **6**). External power **1884** is provided to the docking station module **1900a** from the MPMS **250**. The docking station power supply **2230** charges the battery in the portable power supply **730** (FIG. **7**). When the portable **610** (FIG. **6**) is either removed or turned off, the docking station power **2232** is removed and the docking station **1900** is turned off, except for the battery charger portion of the power supply **2230**. The docking station power **2232** and, hence, the docking station **1900** turns on whenever a docked portable **610** (FIG. **6**) is turned on.

Although the dual-mode physiological measuring apparatus and method of the present invention is described in detail with respect to pulse oximetry measurements, one of ordinary skill in the art will recognize that a dual-mode MPMS plug-in module or a portable apparatus that docks to a MPMS plug-in docking station module could incorporate physiological measurement capabilities other than or in addition to pulse oximetry, such as blood pressure, respiration rate, EEG, ECG and EtCO<sub>2</sub> (capnography) to name a few.

The dual-mode pulse oximeter has been disclosed in detail in connection with various embodiments of the present invention. These embodiments are disclosed by way of



23

examples only and are not to limit the scope of the present invention, which is defined by the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications within the scope of this invention.

What is claimed is:

1. A multi-monitor system for monitoring physiological parameters of a patient, the system comprising:

a portable monitor including a portable display and a portable processor, said portable monitor configured to operate in a portable mode and a docked mode, said portable monitor also configured to communicate with a noninvasive sensor, said portable processor configured to process signals from said noninvasive sensor to determine display values of physiological parameters of the patient, wherein when operating in said portable mode, said portable monitor operates as a standalone monitor to communicate at least some of said display values to said portable display for caregiver review; and

a multi-parameter monitor including a multi-parameter display other than said portable display and a plurality of receptacles, at least one of the receptacles configured to physically position and electrically communicate with a non-standalone parameter monitor module including a processor different than said portable processor, said non-standalone parameter monitor module not configured to operate without being physically positioned in or in electrical communication with the at least one of the receptacles of the multi-parameter monitor, said processor of the non-standalone parameter monitor configured to process signals other than said signals from said noninvasive sensor associated with said portable monitor to determine display values of physiological parameters of the patient and to communicate at least some of said determined display values to said multi-parameter display for caregiver review, and at least a second one of the receptacles configured to mechanically receive and physically position said portable monitor with respect to said multi-parameter monitor, and wherein when said portable monitor is received by the second one of the receptacles of said multi-parameter monitor, said portable monitor communicates with said multi-parameter monitor to communicate at least some of said display values of said portable monitor to said multi-parameter display for caregiver review.

2. The multi-monitor system of claim 1, wherein said physiological parameters include at least one of oxygen saturation, pulse rate, respiration rate, blood pressure, EEG, and ECG.

3. The multi-monitor system of claim 1, wherein said communications of said some display values from said portable monitor to said multi-parameter display includes a synthesized waveform.

4. The multi-monitor system of claim 3, further comprising a waveform look-up table, wherein said synthesized waveform is calculated with reference to a waveform look-up table.

5. The multi-monitor system of claim 3, wherein said synthesized waveform is configured to be manually synchronized.

6. The multi-monitor system of claim 1, wherein at least one of the receptacles includes a module slot portion.

7. The multi-monitor system of claim 1, wherein when said portable monitor is received in the said second one of said receptacles, said portable display does not display at least one of said display values.

24

8. A patient monitor comprising:

a first display;

a first processor in electronic communication with a non-standalone parameter monitor module and configured to receive a first signal indicative of at least one physiological parameter of a monitored patient from a first non-invasive sensor and further configured to process said first signal to determine at least a first measurement, and to communicate said first measurement to said first display for caregiver review, said non-standalone parameter monitor module not configured to operate without being in electronic communication with the first processor;

a second display;

a second processor configured to operate in a portable mode and a docked mode, and configured to receive a second signal from a second noninvasive sensor, said second processor configured to process said second signal to determine at least a second measurement, and to communicate said second measurement to said second display for caregiver review;

a portable housing arranging said second display and said second processor as a portable standalone monitoring device away from said first display and said first processor; and

a multi-parameter housing configured to physically position said portable housing, said non-standalone parameter monitor module, and said first processor with respect to said first display and configured to provide communication between said first and second processors and said first display in order to communicate said second measurement to said first processor, wherein said first processor communicates said first and second measurement to said first display.

9. The patient monitor of claim 8, wherein said second measurement comprises one of oxygen saturation, pulse rate, respiration rate, blood pressure, EEG, and ECG.

10. The patient monitor of claim 8, wherein said first processor is configured to process said first signal to determine a plurality of measurements, including said first measurement, and to communicate said plurality of first measurements to said first display for caregiver review.

11. The patient monitor of claim 8, wherein said second processor is configured to process said second signal to determine a plurality of measurements, including said second measurement, and to communicate said plurality of second measurements to said second display for caregiver review.

12. The patient monitor of claim 10, wherein at least some of said plurality of measurements are different from said second measurement.

13. The patient monitor of claim 10, wherein at least one of said plurality of measurements is for the same physiological parameter as said second measurement.

14. The patient monitor of claim 8, wherein said first display receives at least a portion of said second measurement by synthesized waveform.

15. The patient monitor of claim 8, wherein said multi-parameter housing comprises a module slot portion for positioning the portable housing.

16. A method of providing measurements for caregiver review, comprising:

receiving, at a standalone portable patient monitor, first signals indicative of physiological parameters of a monitored patient from a first physiological sensor;

25

processing said first signals to determine one or more first measurements using a first processor of said standalone portable patient monitor;  
 communicating said one or more first measurements to a first display for caregiver review;  
 mechanically receiving, into a receptacle of a multi-parameter patient monitor, said standalone portable patient monitor including said first processor and said first display, said multi-parameter patient monitor including a second display;  
 mechanically receiving, at a second receptacle of said multi-parameter patient monitor, a non-standalone patient monitor module including a second processor, said non-standalone parameter monitor module not configured to operate without being received by said multi-parameter patient monitor;  
 receiving at said second processor of said non-standalone patient monitor module second signals indicative of second physiological parameters of a monitored patient from a second physiological sensor associated with said second processor;

26

processing said second signals using said second processor to determine one or more second measurements; communicating said second measurements to said second display for caregiver review;  
 receiving at said multi-parameter patient monitor at least one of said one or more first measurements; and communicating an indication of said first measurements to said second display for caregiver review.

17. The method of claim 16, wherein at least some of said second measurements are different from said first measurements.

18. The method of claim 16, wherein the step of receiving at least one of said one or more first measurements further comprises receiving a synthesized waveform.

19. The method of claim 18, wherein the step of receiving a synthesized waveform further comprises receiving a synthesized waveform generated by manual synchronization at said standalone portable patient monitor.

20. The method of claim 16, wherein the step of mechanically receiving at a receptacle comprises receiving into a module slot portion of said multi-parameter patient monitor.

\* \* \* \* \*

|                |                                                                                                                                                                              |         |            |
|----------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 双模式病人监护仪                                                                                                                                                                     |         |            |
| 公开(公告)号        | <a href="#">US10231676</a>                                                                                                                                                   | 公开(公告)日 | 2019-03-19 |
| 申请号            | US14/022106                                                                                                                                                                  | 申请日     | 2013-09-09 |
| [标]申请(专利权)人(译) | 梅西莫股份有限公司                                                                                                                                                                    |         |            |
| 申请(专利权)人(译)    | Masimo公司                                                                                                                                                                     |         |            |
| 当前申请(专利权)人(译)  | Masimo公司                                                                                                                                                                     |         |            |
| [标]发明人         | AL ALI AMMAR<br>CAROTHERS DON<br>DALKE DAVID<br>DIAB MOHAMED K<br>GOLDMAN JULIAN<br>KIANI MASSI E<br>LEE MICHAEL<br>NOVAK JEROME<br>SMITH ROBERT<br>VADEN VAL E              |         |            |
| 发明人            | AL-ALI, AMMAR<br>CAROTHERS, DON<br>DALKE, DAVID<br>DIAB, MOHAMED K.<br>GOLDMAN, JULIAN<br>KIANI, MASSI E.<br>LEE, MICHAEL<br>NOVAK, JEROME<br>SMITH, ROBERT<br>VADEN, VAL E. |         |            |
| IPC分类号         | A61B5/00 A61B5/1455 A61B5/0476 A61B5/0402 A61B5/021 A61B5/0205                                                                                                               |         |            |
| CPC分类号         | A61B5/7445 A61B5/0002 A61B5/021 A61B5/0205 A61B5/0402 A61B5/14551 A61B5/742 A61B5/0476 A61B2560/0456 A61B2560/0271 A61B2560/0443                                             |         |            |
| 优先权            | 60/117097 1999-01-25 US<br>60/161565 1999-10-26 US                                                                                                                           |         |            |
| 其他公开文献         | US20140012100A1                                                                                                                                                              |         |            |
| 外部链接           | <a href="#">Espacenet</a>                                                                                                                                                    |         |            |

#### 摘要(译)

便携式患者监护仪具有集成模式，其中其作为用于多参数患者监测系统 ( MPMS ) 的插入模块操作。患者监护仪还具有便携式模式，其作为电池供电的手持式或独立式仪器与MPMS分开操作。患者监测器具有传感器端口，该传感器端口接收指示生理参数的信号作为内部处理器的输入。患者监测器处理该传感器信号以得出患者测量结果。在便携式模式中，该信息在其显示器上提供。在集成模式中，患者监视器向MPMS提供患者测量值以在MPMS监视器上显示。

