



US 20170181643A1

(19) **United States**

(12) **Patent Application Publication**
Pahlevan et al.

(10) **Pub. No.: US 2017/0181643 A1**

(43) **Pub. Date: Jun. 29, 2017**

(54) **NONINVASIVE SYSTEMS FOR BLOOD
PRESSURE MEASUREMENT IN ARTERIES**

Publication Classification

(71) Applicant: **CALIFORNIA INSTITUTE OF
TECHNOLOGY**, Pasadena, CA (US)

(72) Inventors: **Niema Pahlevan**, Pasadena, CA (US);
Morteza Gharib, Altadena, CA (US)

(21) Appl. No.: **15/459,581**

(22) Filed: **Mar. 15, 2017**

Related U.S. Application Data

(63) Continuation of application No. 13/715,743, filed on
Dec. 14, 2012, now Pat. No. 9,622,666.

(60) Provisional application No. 61/570,711, filed on Dec.
14, 2011.

(51) **Int. Cl.**

A61B 5/021 (2006.01)

A61B 5/00 (2006.01)

A61B 8/00 (2006.01)

A61B 8/04 (2006.01)


(52) **U.S. Cl.**

CPC *A61B 5/021* (2013.01); *A61B 8/04*
(2013.01); *A61B 5/742* (2013.01); *A61B*
8/4427 (2013.01); *A61B 5/0507* (2013.01)

(57)

ABSTRACT

Hardware and software methodology are described for a non-invasive approach to blood pressure measurement in pulmonary artery and systemic arteries by using wall displacement and blood velocity that are measured using ultrasound, microwave techniques and/or other radiofrequency (RF) techniques.

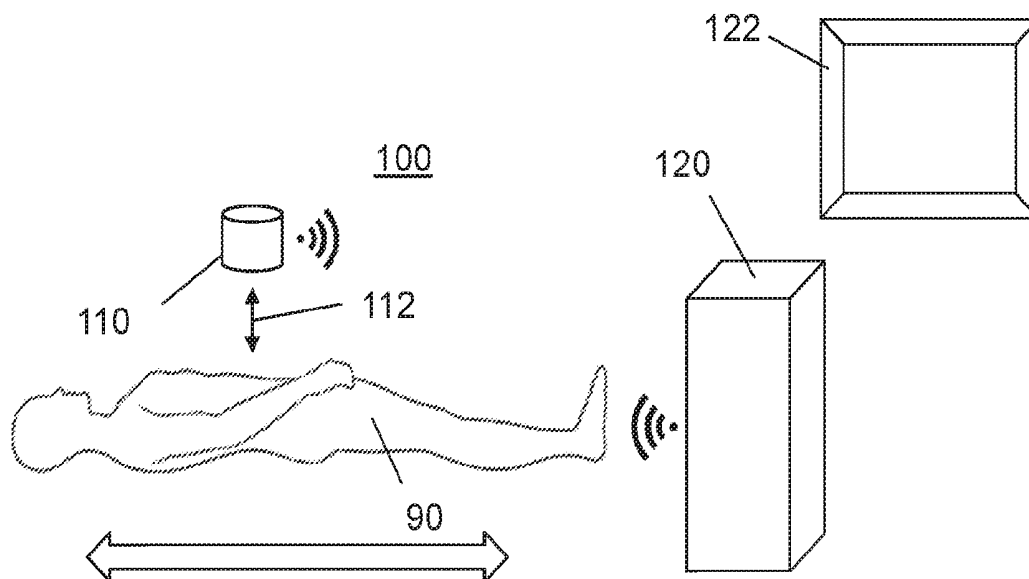

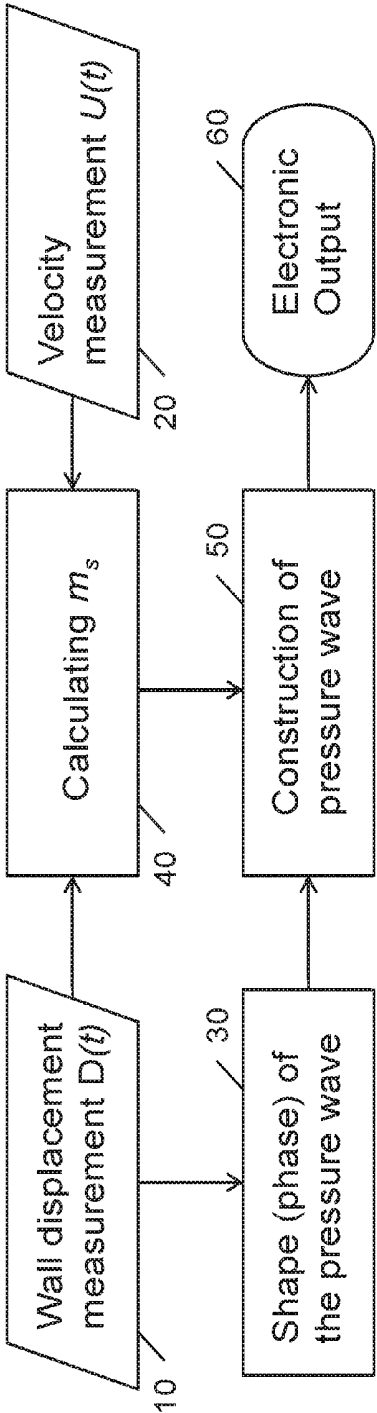


Fig. 1

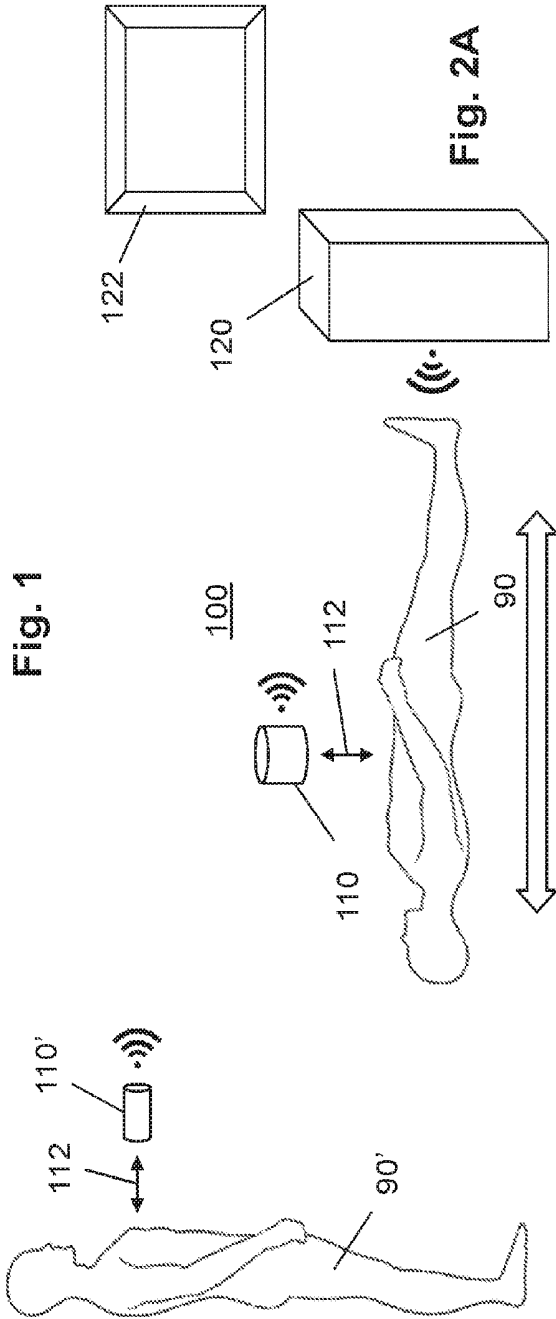


Fig. 2A

Fig. 2B

NONINVASIVE SYSTEMS FOR BLOOD PRESSURE MEASUREMENT IN ARTERIES

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 13/715,743, filed Dec. 14, 2012, which claims the benefit of U.S. Provisional Application No. 61/570,711, filed Dec. 14, 2011 and entitled, “Noninvasive Method and Device for Measurement of Instantaneous Pressure in Arteries,” both of which are incorporated by reference herein in their entirety for all purposes.

FIELD

[0002] This filing relates to non-invasive blood pressure measurement.

BACKGROUND

[0003] The pulmonary and systemic arterial pressure wave is an important parameter in the diagnosis of various pulmonary artery and systemic artery diseases such as pulmonary hypertension, pulmonary stenosis, systemic hypertension and arterial stenosis. Invasive methods of pressure measurement cause discomfort for the patients, and they include procedural and post-operative risks, the later including infection with an increasing incidence of mortality due to antibiotic resistant bacteria. Accordingly, non-invasive techniques for blood pressure measurement are preferred and may become increasingly important.

[0004] Once such technique is known as applanation tonometry. However, it is limited to measurement in certain locations such as the radial arteries at wrist or carotid arteries where these systemic arteries are close to the surface of the skin. Moreover, commercially-available tonometric devices are all quite motion-sensitive further limiting their use/applicability. Still further: affixing, wearing and ultimately removing the force or displacement sensor employed a tonometric monitoring system can be difficult and sometimes uncomfortable.

[0005] Another technique for estimating blood pressure is variously described in which blood velocity is measured via ultrasound Doppler and then the Bernoulli equation applied to calculate a result. However, the Bernoulli equation does not properly apply to moving boundary condition systems or those involving unsteady flow—both of which are features of the relevant biological systems. As such, the accuracy/applicability of these approaches are limited. These methods can only provide estimates for mean pressure, systolic pressure, and/or diastolic pressure. They are not able to provide the pressure wave or pressure at any time during a cardiac cycle.

[0006] Therefore, improved noninvasive techniques—especially noncontact methods—for measuring and/or monitoring the arterial pressure waveform are needed.

SUMMARY

[0007] The inventive embodiments include the subject devices and systems (e.g., including the sensor hardware referenced herein and the addition of a computer processor and other ancillary or support electronics and various housing elements), and methods (including the hardware and software for carrying out the same). These embodiments provide a noninvasive approach for blood pressure measure-

ment in pulmonary artery and systemic arteries by using wall displacement and blood velocity that are measured non-invasively using ultrasound and/or microwave or other radiofrequency (RF) techniques. Methods, devices, and systems are provided for calculating instantaneous pressure in the arteries and/or outputting highly accurate pressure wave estimates generated from a calculated slope of the D-U loop (as defined below) together with vessel wall displacement wave measurements.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] The figures provided herein are diagrammatic and not necessarily drawn to scale, with some components and features exaggerated and/or abstracted for clarity. Variations from the embodiments pictured are contemplated. Accordingly, depiction of aspects and elements in the figures are not intended to limit the scope of the claims, except when such intent is explicitly stated as such.

[0009] FIG. 1 is a flowchart illustrating activity in an example embodiment of the subject method.

[0010] FIGS. 2A-B illustrate options for systems operating according to an example embodiment of the subject method.

DETAILED DESCRIPTION

[0011] Various example embodiments are described below. Reference is made to these examples in a non-limiting sense. They are provided to illustrate more broadly applicable aspects of inventive aspects. Various changes may be made to the embodiments described and equivalents may be substituted without departing from their true spirit and scope. In addition, many modifications may be made to adapt a particular situation, material, composition of matter, process, process act(s) or step(s) to the objective(s), spirit or scope of the claims made herein.

[0012] That said, the subject technique is based on the fact that the walls of the large central pulmonary and systemic arteries are almost elastic. Therefore, the blood pressure and their wall displacement wave can be characterized as having the same shape. Stated another way, the wall displacement wave is in phase with the blood pressure wave.

[0013] Thus, in the absence of a reflected wave at the beginning of the cardiac cycle, the below relation between an increment of pressure (dP) and an increment of average velocity over cross-section area (dU) holds:

$$dP_+ = (\rho c) dU_+ \quad (1)$$

[0014] Where ρ is the density of fluid, c is the wave speed, and “+” sign corresponds to forward waves. In addition from 1D wave theory, wave speed can be written as a function of blood vessel distensibility (dis):

$$c = \sqrt{\frac{1}{\rho \cdot dis}} \quad (2)$$

where dis can be calculated as:

$$dis = \frac{1}{A} \frac{dA}{dP} \quad (3)$$

where A is the cross-section area, $A=\pi/4.D^2$, and D is the diameter of the vessel. Using the chain rule and substituting D in (3) results in:

$$dis = \frac{2}{D} \frac{dD}{dP}. \quad (4)$$

Combining (4) and (2) and substitute in (1) yields:

$$dD_+ = \left(\frac{D}{2c}\right)dU_+. \quad (5)$$

Accordingly, the slope of a graph of the vessel diameter plotted against blood velocity, generally center-line blood or cross-section area average of the velocity, (i.e., the D-U graph or loop) at the beginning of the cardiac cycle (m_s) is equal to $D/2c$.

[0015] Also, wall displacement wave speed is related to Young's modulus (E) and wall thickness (t) through Moens-Kortweg equation:

$$c = \sqrt{\frac{Eh}{\rho D}} \rightarrow Eh = \rho D c^2. \quad (6)$$

Using thin elastic tube theory with applied internal pressure, the following equation holds:

$$\sigma_{\theta\theta} = \frac{PR}{h} \quad (7)$$

where $\sigma_{\theta\theta}$ is the circumferential stress, R is the radius of the tube P is the internal pressure, and h is the thickness of the tube. Assuming that radial stress is much smaller than circumferential stress and by using (7) the circumferential strain can be written as:

$$\epsilon_{\theta\theta} = \frac{PR}{Eh}. \quad (8)$$

Based on the definition of the circumferential strain:

$$\epsilon_{\theta\theta} = \frac{\Delta R}{R} \quad (9)$$

And combining (8) and (9), replacing diameter for radius yields:

$$Eh = \frac{PD^2}{2(\Delta D)}. \quad (10)$$

Substituting Eh from (10) into (6) results in:

$$c = \sqrt{\frac{PD}{2\rho(\Delta D)}}. \quad (11)$$

From equation (5) the slope of D-U graph at the beginning of the cardiac cycle is

$$m_s = \frac{dD_+}{dU_+} = \frac{D}{2c}. \quad (12)$$

Combining (11) and (12) and solving for P yields:

$$P = \frac{\rho D(\Delta D)}{2m_s^2} \quad (13)$$

Where D_0 for ΔD (i.e., $D-D_0$) may be determined by any of a variety of approaches as typical in the art. For instance, any of a search algorithm, allometric equations (age-corrected), diastolic diameter, clinically derived values, or an approximate based on patient history may be employed.

[0016] With these principles in mind, FIG. 1 shows the steps for noninvasive instantaneous pressure measurement. At **10** and **20**, wall displacement and velocity waves are measured noninvasively at the same or substantially the same location (e.g., within about 1 cm for large/larger vessels and within about 5 mm in small/smaller vessels and more generally—though not necessarily—within ± 1 vessel diameter in separation) along any pulmonary or systemic artery using ultrasound, microwave, or other suitable technique(s). These measurements are accomplished with at least one sensor adapted to record a first data set that correlates to blood vessel distension and adapted to record a second data set that correlates to blood velocity, more particularly center-line blood velocity or cross-sectional area average of the velocity. Then at least one computer processor is programmed to convert the first data set to a measurement of blood vessel distention and the second data set to a measurement of relevant blood velocity.

[0017] At **30**, the shape of the pressure wave is captured or recorded and will be the same as the shape of the wall displacement (assuming a linear elastic vessel wall) measured at **10**.

[0018] At **40**, the D-U loop is determined and the slope (m_s) at the beginning of a cardiac cycle calculated therefrom. Or the slope may be calculated in another fashion. In any case, with m_s , the pressure may be calculated at any moment during the cardiac cycle using equation (13) or any similar equation. At **50**, the blood pressure wave, if desired, is so-constructed.

[0019] A highly accurate estimate (given the assumptions noted above) of blood pressure is thus determined from the shape and magnitude calculated at **30** and **40**. Any (or all) such data (e.g., instantaneous pressure, systolic/diastolic max/min pressure, pulse pressure, and/or the entire pressure wave) is output at **60** in a computer-readable format or data stream. This data can be in the form of an average over a given number of cycles or as a real time data stream. Accordingly, instantaneous pressure measurements and/or the calculated pressure wave may be displayed in real time

for physician evaluation and/or logged for monitoring or subsequent evaluation of a physician, or other analysis.

[0020] Regardless, what is meant by “real time” in the context above will generally mean that it takes about 1 second or less from the time of data acquisition for calculation and data presentation, more often such action is essentially without the delay perceptible to humans. In any case, real time activity in the subject embodiments concern manipulation of such a mass of data and calculations that the task is well beyond human capacity, thereby requiring the use of a computer processor.

[0021] FIG. 2A diagrammatically illustrates such a computer-based system 100 with various hardware and patient-handling options. Namely, a patient may be scanned in a supine position 90, in a standing position 90' or otherwise. The scanner 110 may be associated with an armature, a C-arm, a scanner “tunnel,” or otherwise configured. If scanner 110' is configured as a handheld scanner, then a standing position 90' may be preferable to accommodate the handheld operation as shown in FIG. 2B. The scanner may be moved relative to the patient to scan a selected area or areas. Or the patient may be moved relative to the scanner (as indicated). Notably, targeting larger central vessels (as opposed to smaller more distal vessels) may be desirable for improved accuracy. In the larger vessels, diameter displacements are generally larger. Also, the assumption of vessel elasticity is more perfect/pure, whereas peripheral vessels tend to exhibit a greater degree of visco-elastic behavior. Still, in most any location selected the subject embodiments offer useful improvement over previous techniques.

[0022] In any case, scanner 110/110' includes on-board electronics for sending and receiving signals 112 to perform the referenced measurements of blood flow velocity and/or vessel distension. Use of microwave sensor (at least for measuring vessel displacement) and/or ultrasound sensors (for measuring either or both vessel distension and blood velocity) for such purposes is well known. An example of suitable publicly-available hardware includes the GE LOGIQ Book Portable Ultrasound Machine, which technology is readily adapted to the subject methods and systems.

[0023] Alternatively, a hand-held scanner 110 incorporated in system 100 may advantageously be battery-powered so as to avoid connection to a wall socket. Whether hand-held or incorporated or in a larger unity, the scanner device (s) may interface by wireless (as indicated) or wired (not shown) communication with a general purpose computer 120, optionally including display 122 to perform and communicate results, respectively. Otherwise, on-board processing and/or display hardware may be provided in connection with the sensor housing itself. Such options would be especially useful for a hand-held or semi-portable device as these may be used by a patient/subject at home, during travel, etc.

[0024] Variations

[0025] In addition to the embodiments that been disclosed in detail above, still more are possible within the classes described and the inventors intend these to be encompassed within this Specification and claims. This disclosure is intended to be exemplary, and the claims are intended to cover any modification or alternative which might be predictable to a person having ordinary skill in the art.

[0026] Moreover, the various illustrative processes described in connection with the embodiments herein may be implemented or performed with a general purpose pro-

cessor, a Digital Signal Processor (DSP), an Application Specific Integrated Circuit (ASIC), a Field Programmable Gate Array (FPGA) or other programmable logic device, discrete gate or transistor logic, discrete hardware components, or any combination thereof designed to perform the functions described herein. A general purpose processor may be a microprocessor, but in the alternative, the processor may be any conventional processor, controller, microcontroller, or state machine. The processor can be part of a computer system that also has a user interface port that communicates with a user interface, and which receives commands entered by a user, has at least one memory (e.g., hard drive or other comparable storage, and random access memory) that stores electronic information including a program that operates under control of the processor and with communication via the user interface port, and a video output that produces its output via any kind of video output format, e.g., VGA, DVI, HDMI, DisplayPort, or any other form.

[0027] A processor may also be implemented as a combination of computing devices, e.g., a combination of a DSP and a microprocessor, a plurality of microprocessors, one or more microprocessors in conjunction with a DSP core, or any other such configuration. These devices may also be used to select values for devices as described herein. The camera may be a digital camera of any type including those using CMOS, CCD or other digital image capture technology.

[0028] The steps of a method or algorithm described in connection with the embodiments disclosed herein may be embodied directly in hardware, in a software module executed by a processor, or in a combination of the two. A software module may reside in Random Access Memory (RAM), flash memory, Read Only Memory (ROM), Electrically Programmable ROM (EPROM), Electrically Erasable Programmable ROM (EEPROM), registers, hard disk, a removable disk, a CD-ROM, or any other form of storage medium known in the art. An exemplary storage medium is coupled to the processor such that the processor can read information from, and write information to, the storage medium. In the alternative, the storage medium may be integral to the processor. The processor and the storage medium may reside in an ASIC. The ASIC may reside in a user terminal. In the alternative, the processor and the storage medium may reside as discrete components in a user terminal.

[0029] In one or more exemplary embodiments, the functions described may be implemented in hardware, software, firmware, or any combination thereof. If implemented in software, the functions may be stored on, transmitted over or resulting analysis/calculation data output as one or more instructions, code or other information on a computer-readable medium. Computer-readable media includes both computer storage media and communication media including any medium that facilitates transfer of a computer program from one place to another. A storage media may be any available media that can be accessed by a computer. By way of example, and not limitation, such computer-readable media can comprise RAM, ROM, EEPROM, CD-ROM or other optical disk storage, magnetic disk storage or other magnetic storage devices, or any other medium that can be used to carry or store desired program code in the form of instructions or data structures and that can be accessed by a computer. The memory storage can also be rotating mag-

netic hard disk drives, optical disk drives, or flash memory based storage drives or other such solid state, magnetic, or optical storage devices. Also, any connection is properly termed a computer-readable medium. For example, if the software is transmitted from a website, server, or other remote source using a coaxial cable, fiber optic cable, twisted pair, digital subscriber line (DSL), or wireless technologies such as infrared, radio, and microwave, then the coaxial cable, fiber optic cable, twisted pair, DSL, or wireless technologies such as infrared, radio, and microwave are included in the definition of medium. Disk and disc, as used herein, includes compact disc (CD), laser disc, optical disc, digital versatile disc (DVD), floppy disk and BLU-RAY disc where disks usually reproduce data magnetically, while discs reproduce data optically with lasers. Combinations of the above should also be included within the scope of computer-readable media.

[0030] Operations as described herein can be carried out on or over a website. The website can be operated on a server computer, or operated locally, e.g., by being downloaded to the client computer, or operated via a server farm. The website can be accessed over a mobile phone or a PDA, or on any other client. The website can use HTML code in any form, e.g., MHTML, or XML, and via any form such as cascading style sheets ("CSS") or other.

[0031] Also, the inventors intend that only those claims which use the words "means for" are intended to be interpreted under 35 USC 112, sixth paragraph. Moreover, no limitations from the specification are intended to be read into any claims, unless those limitations are expressly included in the claims. The computers described herein may be any kind of computer, either general purpose, or some specific purpose computer such as a workstation. The programs may be written in C, or Java, Brew or any other programming language. The programs may be resident on a storage medium, e.g., magnetic or optical, e.g. the computer hard drive, a removable disk or media such as a memory stick or SD media, or other removable medium. The programs may also be run over a network, for example, with a server or other machine sending signals to the local machine, which allows the local machine to carry out the operations described herein.

[0032] Also, it is contemplated that any optional feature of the embodiment variations described may be set forth and claimed independently, or in combination with any one or more of the features described herein. Reference to a singular item, includes the possibility that there is a plurality of the same items present. More specifically, as used herein and in the appended claims, the singular forms "a," "an," "said," and "the" include plural referents unless specifically stated otherwise. In other words, use of the articles allow for "at least one" of the subject item in the description above as well as the claims below. It is further noted that the claims may be drafted to exclude any optional element. As such, this statement is intended to serve as antecedent basis for use of such exclusive terminology as "solely," "only" and the like in connection with the recitation of claim elements, or use of a "negative" limitation.

[0033] Without the use of such exclusive terminology, the term "comprising" in the claims shall allow for the inclusion of any additional element irrespective of whether a given number of elements are enumerated in the claim, or the addition of a feature could be regarded as transforming the nature of an element set forth in the claims. Except as

specifically defined herein, all technical and scientific terms used herein are to be given as broad a commonly understood meaning as possible while maintaining claim validity.

[0034] The breadth of the present inventive subject matter is not to be limited to the examples provided and/or the subject specification, but rather only by the scope of the claim language. All references cited are incorporated by reference in their entirety. Although the foregoing embodiments been described in detail for purposes of clarity of understanding, it is contemplated that certain modifications may be practiced within the scope of the appended claims.

1. A system for noninvasive determination of blood pressure comprising:

at least one sensor that produces a first data set that correlates to distension of a blood vessel and a second data set that correlates to blood velocity within the vessel; and

at least one processor that converts the first data set to measurement of blood vessel distention and the second data set to measurement of blood velocity.

2. The system of claim 1, wherein the processor causes the system to capture the data sets at the beginning of a cardiac cycle.

3. The system of claim 2, wherein the processor selects from the data sets at the beginning of the cardiac cycle.

4. The system of claim 3, wherein the processor calculates a slope of a D-U loop at the beginning of the cardiac cycle.

5. The system of claim 4, wherein the processor calculates blood pressure based on the slope and the blood vessel distention.

6. The system of claim 5, adapted to record at least one of the first and second data sets, the measurements of blood vessel distention and average blood velocity, or the calculated blood pressure.

7. The system of claim 5, wherein the processor outputs the calculated blood pressure for visual display.

8. The system of claim 1, adapted to produce the first and second data sets at substantially the same location of the blood vessel.

9. The system of claim 1, wherein the at least one sensor is a radiofrequency sensor.

10. The system of claim 1, wherein the at least one sensor is an ultrasound or microwave sensor.

11. A method of blood pressure estimation, the method comprising:

selecting a blood vessel;

measuring blood vessel distention and blood velocity with at least one sensor;

calculating, in real time, blood pressure based on the blood vessel distention and blood velocity; and

displaying the calculated blood pressure on an electronic display.

12. The method of claim 11, wherein the blood vessel is a pulmonary or systemic artery.

13. The method of claim 11, wherein calculating includes determining a slope calculated for vessel diameter plotted against blood velocity at the beginning of a cardiac cycle.

14. The method of claim 11, wherein the blood velocity measured is selected from center-line blood velocity and cross-section area average of the velocity.

15. A computer readable medium having stored thereon instructions, which when executed cause one or more processors to:

receive input signals from at least one sensor corresponding to blood vessel distention and blood velocity; determine, using the input signals, vessel distention and blood velocity from sensor; calculate blood pressure based on the blood vessel distention and blood velocity; and output a signal corresponding to the calculated blood pressure.

16. The computer readable medium of claim **15**, wherein the blood pressure calculation includes determining a slope calculated for vessel diameter plotted against blood velocity at the beginning of a cardiac cycle.

17. The computer readable medium of claim **16**, wherein the blood velocity is selected from center-line blood velocity and cross-section area average of the velocity.

18. The computer readable medium of claim **16**, wherein the output is selected from instantaneous pressure, systolic/diastolic max/min pressure, pulse pressure, and an entire pressure wave.

19. The computer readable medium of claim **18**, wherein the instructions cause the output to be displayed in real time.

20. The computer readable medium of claim **18**, wherein the instructions cause the output to be displayed as an average over a number of cycles.

* * * * *

专利名称(译)	用于动脉血压测量的无创系统		
公开(公告)号	US20170181643A1	公开(公告)日	2017-06-29
申请号	US15/459581	申请日	2017-03-15
[标]申请(专利权)人(译)	加州理工学院		
申请(专利权)人(译)	加州理工大学		
当前申请(专利权)人(译)	加州理工大学		
[标]发明人	PAHLEVAN NIEMA GHARIB MORTEZA		
发明人	PAHLEVAN, NIEMA GHARIB, MORTEZA		
IPC分类号	A61B5/021 A61B5/00 A61B8/00 A61B8/04		
CPC分类号	A61B5/021 A61B8/04 A61B5/0507 A61B8/4427 A61B5/742 A61B5/02007 A61B8/06 A61B8/485 A61B8/5223 G16H50/30		
优先权	61/570711 2011-12-14 US		
外部链接	Espacenet USPTO		

摘要(译)

通过使用利用超声波，微波技术和/或其他射频（RF）技术测量的壁位移和血液速度来描述用于肺动脉和全身动脉中的血压测量的非侵入性方法的硬件和软件方法。

