



US009788785B2

(12) **United States Patent**
LeBoeuf

(10) **Patent No.:** **US 9,788,785 B2**
(45) **Date of Patent:** ***Oct. 17, 2017**

(54) **APPARATUS AND METHODS FOR ESTIMATING TIME-STATE PHYSIOLOGICAL PARAMETERS**

(71) Applicant: **Valencell, Inc.**, Raleigh, NC (US)

(72) Inventor: **Steven Francis LeBoeuf**, Raleigh, NC (US)

(73) Assignee: **Valencell, Inc.**, Raleigh, NC (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **15/369,629**

(22) Filed: **Dec. 5, 2016**

(65) **Prior Publication Data**

US 2017/0079582 A1 Mar. 23, 2017

Related U.S. Application Data

(63) Continuation of application No. 15/219,770, filed on Jul. 26, 2016, now Pat. No. 9,521,962, which is a (Continued)

(51) **Int. Cl.**

A61B 5/04 (2006.01)

A61B 5/00 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61B 5/4857** (2013.01); **A61B 5/0077** (2013.01); **A61B 5/02055** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC . A61B 5/4866; A61B 5/14551; A61B 5/4857; A61B 5/02055; A61B 5/021; A61B 2560/0242; A61B 5/02405; A61B 5/0816
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,595,219 A 7/1971 Friedlander et al.

4,240,882 A 12/1980 Ang et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CA 2 875 901 A1 12/2012
CN 101212927 A 7/2008

(Continued)

OTHER PUBLICATIONS

International Search Report corresponding to International Patent Application No. PCT/US2012/046446; dated Jan. 14, 2013; 3 pages.

(Continued)

Primary Examiner — Rex R Holmes


(74) *Attorney, Agent, or Firm* — Myers Bigel, P.A.

(57)

ABSTRACT

A method of determining a value of a physiological parameter for a subject at a selected state includes obtaining, via a device located a distance from the subject, a value of the physiological parameter of the subject at a particular time-of-day, and applying a time-dependent relationship function to the obtained physiological parameter value via a processor to determine a value of the physiological parameter at the selected state.

21 Claims, 11 Drawing Sheets

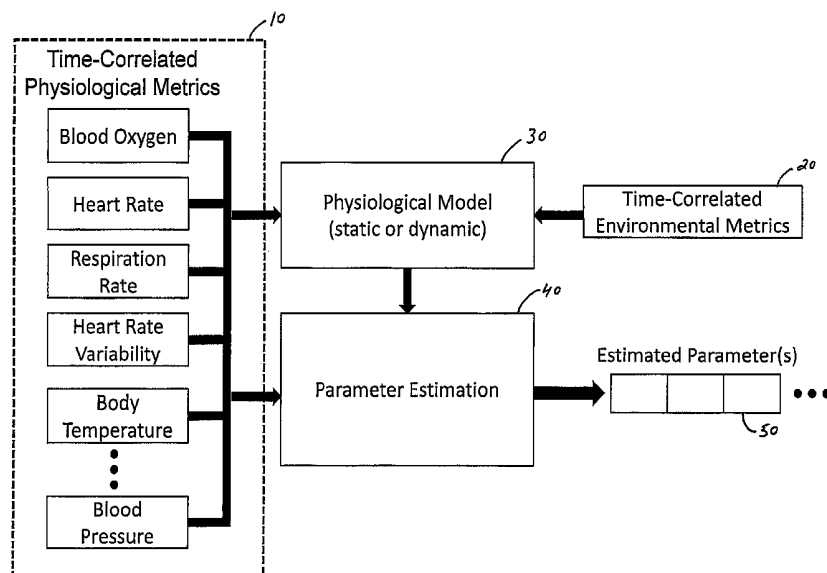

Related U.S. Application Data

continuation of application No. 14/116,641, filed as application No. PCT/US2012/046446 on Jul. 12, 2012, now Pat. No. 9,427,191.

- (60) Provisional application No. 61/511,238, filed on Jul. 25, 2011.

(51) **Int. Cl.**

A61B 5/0205 (2006.01)

A61B 5/08 (2006.01)

A61B 5/1455 (2006.01)

A61B 5/11 (2006.01)

A61B 5/145 (2006.01)

A61B 5/021 (2006.01)

A61B 5/024 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/02438* (2013.01); *A61B 5/0816* (2013.01); *A61B 5/1118* (2013.01); *A61B 5/14546* (2013.01); *A61B 5/14551* (2013.01); *A61B 5/4866* (2013.01); *A61B 5/6889* (2013.01); *A61B 5/6891* (2013.01); *A61B 5/6892* (2013.01); *A61B 5/6893* (2013.01); *A61B 5/021* (2013.01); *A61B 5/02405* (2013.01); *A61B 5/14542* (2013.01); *A61B 2560/0242* (2013.01); *A61B 2562/0204* (2013.01); *A61B 2562/0271* (2013.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,331,154 A 5/1982 Broadwater et al.
 4,438,772 A 3/1984 Slavin
 4,491,760 A 1/1985 Linvill
 4,521,499 A 6/1985 Switzer
 4,541,905 A 9/1985 Kuwana et al.
 4,592,807 A 6/1986 Switzer
 4,655,225 A 4/1987 Dahne et al.
 4,830,014 A 5/1989 Goodman et al.
 4,882,492 A 11/1989 Schlager
 4,896,676 A 1/1990 Sasaki
 4,928,704 A 5/1990 Hardt
 4,957,109 A 9/1990 Groeger et al.
 5,002,060 A 3/1991 Nedivi
 5,022,970 A 6/1991 Cook et al.
 5,025,791 A 6/1991 Niwa
 5,079,421 A 1/1992 Knudson et al.
 5,080,098 A 1/1992 Willett et al.
 5,086,229 A 2/1992 Rosenthal et al.
 5,143,078 A 9/1992 Mather et al.
 5,226,417 A 7/1993 Swedlow et al.
 5,237,994 A 8/1993 Goldberger
 5,348,002 A 9/1994 Caro
 5,377,100 A 12/1994 Pope et al.
 5,482,036 A 1/1996 Diab et al.
 5,492,129 A 2/1996 Greenberger
 5,499,301 A 3/1996 Sudo et al.
 5,581,648 A 12/1996 Sahagen
 5,596,987 A 1/1997 Chance
 5,662,117 A 9/1997 Bittman
 5,666,952 A 9/1997 Fuse et al.
 5,673,692 A 10/1997 Schulze et al.
 5,697,374 A 12/1997 Odagiri et al.
 5,711,308 A 1/1998 Singer
 5,725,480 A 3/1998 Oosta et al.
 5,743,260 A 4/1998 Chung et al.
 5,779,631 A 7/1998 Chance
 5,797,841 A 8/1998 Delonzor et al.
 5,807,114 A 9/1998 Hodges et al.
 5,807,267 A 9/1998 Bryars et al.
 5,853,005 A 12/1998 Scanlon
 5,904,654 A 5/1999 Wohltmann et al.

5,938,593 A 8/1999 Quellette
 5,964,701 A 10/1999 Asada et al.
 5,971,931 A 10/1999 Raff
 5,974,338 A 10/1999 Asano et al.
 6,013,007 A 1/2000 Root et al.
 6,023,541 A 2/2000 Merchant et al.
 6,030,342 A 2/2000 Amano et al.
 6,045,511 A 4/2000 Ott et al.
 6,067,006 A 5/2000 O'Brien
 6,070,093 A 5/2000 Oosta et al.
 6,078,829 A 6/2000 Uchida et al.
 6,080,110 A 6/2000 Thorgersen
 6,081,742 A 6/2000 Amano et al.
 6,186,145 B1 2/2001 Brown
 6,198,394 B1 3/2001 Jacobsen et al.
 6,198,951 B1 3/2001 Kosuda et al.
 6,205,354 B1 3/2001 Gellermann et al.
 6,231,519 B1 5/2001 Blants et al.
 6,285,816 B1 9/2001 Anderson et al.
 6,289,230 B1 9/2001 Chaiken et al.
 6,298,314 B1 10/2001 Blackadar et al.
 6,332,868 B1 12/2001 Sato et al.
 6,358,216 B1 3/2002 Kraus et al.
 6,361,660 B1 3/2002 Goldstein
 6,371,925 B1 4/2002 Imai et al.
 6,374,129 B1 4/2002 Chin et al.
 6,415,167 B1 7/2002 Blank et al.
 6,443,890 B1 9/2002 Schulze et al.
 6,444,474 B1 9/2002 Thomas et al.
 6,454,718 B1 9/2002 Clift
 6,458,080 B1 10/2002 Brown et al.
 6,470,893 B1 10/2002 Boesen
 6,513,532 B2 2/2003 Mault et al.
 6,514,278 B1 2/2003 Hibst et al.
 6,527,711 B1 3/2003 Stivoric et al.
 6,527,712 B1 3/2003 Brown et al.
 6,529,754 B2 3/2003 Kondo
 6,534,012 B1 3/2003 Hazen et al.
 6,556,852 B1 4/2003 Schulze et al.
 6,569,094 B2 5/2003 Suzuki et al.
 6,571,117 B1 5/2003 Marbach
 6,605,038 B1 8/2003 Teller et al.
 6,616,613 B1 9/2003 Goodman
 6,631,196 B1 10/2003 Taenzer et al.
 6,647,378 B2 11/2003 Kindo
 6,656,116 B2 12/2003 Kim et al.
 6,694,180 B1 2/2004 Boesen
 6,745,061 B1 6/2004 Hicks et al.
 6,748,254 B2 6/2004 O'Neil et al.
 6,760,610 B2 7/2004 Tschupp et al.
 6,783,501 B2 8/2004 Takahashi et al.
 6,808,473 B2 10/2004 Hisano et al.
 6,859,658 B1 2/2005 Krug
 6,893,396 B2 5/2005 Schulze et al.
 6,941,239 B2 9/2005 Unuma et al.
 6,953,435 B2 10/2005 Kondo et al.
 6,996,427 B2 2/2006 Ali et al.
 6,997,879 B1 2/2006 Turcott
 7,018,338 B2 3/2006 Vetter et al.
 7,024,369 B1 4/2006 Brown et al.
 7,030,359 B2 4/2006 Römhild
 7,034,694 B2 4/2006 Yamaguchi et al.
 7,039,454 B1 5/2006 Kaga et al.
 7,041,062 B2 5/2006 Friedrichs et al.
 7,043,287 B1 5/2006 Khalil et al.
 7,054,674 B2 5/2006 Cane et al.
 7,088,234 B2 8/2006 Naito et al.
 7,107,088 B2 9/2006 Aceti
 7,113,815 B2 9/2006 O'Neil et al.
 7,117,032 B2 10/2006 Childre et al.
 7,163,512 B1 1/2007 Childre et al.
 7,175,601 B2 2/2007 Verjus et al.
 7,190,986 B1 3/2007 Hannula et al.
 7,209,775 B2 4/2007 Bae et al.
 7,217,224 B2 5/2007 Thomas
 7,252,639 B2 8/2007 Kimura et al.
 7,263,396 B2 8/2007 Chen et al.
 7,289,837 B2 10/2007 Mannheimer et al.
 7,336,982 B2 2/2008 Yoo et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,341,559 B2	3/2008	Schultz et al.	2004/0133123 A1	7/2004	Leonhardt et al.
7,376,451 B2	5/2008	Mahony et al.	2004/0135571 A1	7/2004	Uutela et al.
7,483,730 B2	1/2009	Diab et al.	2004/0138578 A1	7/2004	Pineda et al.
7,486,988 B2	2/2009	Goodall et al.	2004/0186390 A1	9/2004	Ross et al.
7,507,207 B2	3/2009	Sakai et al.	2004/0219056 A1	11/2004	Tribelsky et al.
7,519,327 B2	4/2009	White	2004/0220488 A1	11/2004	Vyshedskiy et al.
7,526,327 B2	4/2009	Blondeau et al.	2004/0225207 A1	11/2004	Bae et al.
7,583,994 B2	9/2009	Scholz	2004/0228494 A1	11/2004	Smith
7,620,450 B2	11/2009	Kim et al.	2004/0242976 A1	12/2004	Abreu
7,625,285 B2	12/2009	Breving	2005/0004458 A1	1/2005	Kanayama et al.
7,652,569 B2	1/2010	Kiff et al.	2005/0027216 A1	2/2005	Guillemaud et al.
7,689,437 B1	3/2010	Teller et al.	2005/0030540 A1	2/2005	Thornton
7,695,440 B2	4/2010	Kondo et al.	2005/0033200 A1	2/2005	Soehren et al.
7,725,147 B2	5/2010	Li et al.	2005/0038349 A1	2/2005	Choi et al.
7,756,559 B2	7/2010	Abreu	2005/0043600 A1	2/2005	Diab et al.
7,843,325 B2	11/2010	Otto	2005/0043630 A1	2/2005	Buchert
7,894,869 B2	2/2011	Hoarau	2005/0058456 A1	3/2005	Yoo
7,991,448 B2	8/2011	Edgar et al.	2005/0059870 A1	3/2005	Aceti
7,998,079 B2	8/2011	Nagai et al.	2005/0070809 A1	3/2005	Acres
8,050,728 B2	11/2011	Al-Ali et al.	2005/0084666 A1	4/2005	Pong et al.
8,055,319 B2	11/2011	Oh et al.	2005/0101845 A1	5/2005	Nihtila
8,055,330 B2	11/2011	Egozi	2005/0101872 A1	5/2005	Sattler et al.
8,059,924 B1	11/2011	Letant et al.	2005/0113167 A1	5/2005	Buchner et al.
8,130,105 B2	3/2012	Al-Ali et al.	2005/0113656 A1	5/2005	Chance
8,137,270 B2	3/2012	Keenan et al.	2005/0113703 A1	5/2005	Farrington et al.
8,172,459 B2	5/2012	Abreu	2005/0116820 A1	6/2005	Goldreich
8,175,670 B2	5/2012	Baker, Jr. et al.	2005/0119833 A1	6/2005	Nanikashvili
8,204,730 B2	6/2012	Liu et al.	2005/0154264 A1	7/2005	Lecompte et al.
8,233,955 B2	7/2012	Al-Ali et al.	2005/0177034 A1	8/2005	Beaumont
8,251,903 B2	8/2012	LeBoeuf et al.	2005/0187448 A1	8/2005	Petersen et al.
8,255,027 B2	8/2012	Al-Ali et al.	2005/0187453 A1	8/2005	Petersen et al.
8,255,029 B2	8/2012	Addison et al.	2005/0192515 A1	9/2005	Givens et al.
8,303,512 B2	11/2012	Kosuda et al.	2005/0196009 A1	9/2005	Boesen
8,328,420 B2	12/2012	Abreu	2005/0203349 A1	9/2005	Nanikashvili
8,416,959 B2	4/2013	Lott et al.	2005/0203357 A1	9/2005	Debreczeny et al.
8,491,492 B2	7/2013	Shinar	2005/0209516 A1	9/2005	Fraden
		A61B 5/0205	2005/0222487 A1	10/2005	Miller et al.
		600/16	2005/0222903 A1	10/2005	Buchheit et al.
8,504,679 B2	8/2013	Spire et al.	2005/0228244 A1	10/2005	Banet
8,506,524 B2	8/2013	Graskov et al.	2005/0228299 A1	10/2005	Banet
8,512,242 B2	8/2013	LeBoeuf et al.	2005/0240087 A1	10/2005	Keenan et al.
8,679,008 B2	3/2014	Hughes et al.	2005/0258816 A1	11/2005	Zen et al.
8,730,048 B2	5/2014	Shen et al.	2005/0259811 A1	11/2005	Kimm et al.
9,005,129 B2	4/2015	Venkatraman et al.	2006/0009685 A1	1/2006	Finarov et al.
2001/0049471 A1	12/2001	Suzuki et al.	2006/0012567 A1	1/2006	Sicklinger
2002/0143242 A1	10/2002	Nemirovski	2006/0063993 A1	3/2006	Yu et al.
2002/0156386 A1	10/2002	Dardik et al.	2006/0064037 A1	3/2006	Shalon et al.
2002/0156654 A1	10/2002	Roe et al.	2006/0084878 A1	4/2006	Banet et al.
2002/0186137 A1	12/2002	Skardon	2006/0084879 A1	4/2006	Nazarian et al.
2002/0188210 A1	12/2002	Aizawa	2006/0122520 A1	6/2006	Banet et al.
2002/0194002 A1	12/2002	Petrushin	2006/0123885 A1	6/2006	Yates et al.
2003/0002705 A1	1/2003	Boesen	2006/0142665 A1	6/2006	Garay et al.
2003/0007631 A1	1/2003	Bolognesi et al.	2006/0202816 A1	9/2006	Crump et al.
2003/0045785 A1	3/2003	Diab et al.	2006/0205083 A1	9/2006	Zhao
2003/0050563 A1	3/2003	Suribhotla et al.	2006/0210058 A1	9/2006	Kock et al.
2003/0064712 A1	4/2003	Gaston et al.	2006/0211922 A1	9/2006	Al-Ali et al.
2003/0065257 A1	4/2003	Mault et al.	2006/0211924 A1	9/2006	Dalke et al.
2003/0083583 A1	5/2003	Kovtun et al.	2006/0217598 A1	9/2006	Miyajima et al.
2003/0109030 A1	6/2003	Uchida et al.	2006/0224059 A1	10/2006	Swedlow et al.
2003/0181795 A1	9/2003	Suzuki et al.	2006/0240558 A1	10/2006	Zhao
2003/0212336 A1	11/2003	Lee et al.	2006/0246342 A1	11/2006	MacPhee
2003/0222268 A1	12/2003	Yocom et al.	2006/0251334 A1	11/2006	Oba et al.
2004/0004547 A1	1/2004	Appelt et al.	2006/0252999 A1	11/2006	Devaul et al.
2004/0022700 A1	2/2004	Kim et al.	2006/0264730 A1	11/2006	Stivorice et al.
2004/0030581 A1	2/2004	Leven	2006/0292533 A1	12/2006	Selod
2004/0034289 A1	2/2004	Teller et al.	2006/0293921 A1	12/2006	McCarthy et al.
2004/0034293 A1	2/2004	Kimball	2007/0004449 A1	1/2007	Sham
2004/0054291 A1	3/2004	Schulz et al.	2007/0004969 A1	1/2007	Kong et al.
2004/0075677 A1	4/2004	Loyall et al.	2007/0015992 A1	1/2007	Filkins et al.
2004/0077934 A1	4/2004	Massad	2007/0021206 A1	1/2007	Sunnen
2004/0082842 A1	4/2004	Lumba et al.	2007/0036383 A1	2/2007	Romero
2004/0103146 A1	5/2004	Park	2007/0050215 A1	3/2007	Kil et al.
2004/0117204 A1	6/2004	Mazar et al.	2007/0060800 A1	3/2007	Drinan et al.
2004/0120844 A1	6/2004	Tribelsky et al.	2007/0063850 A1	3/2007	Devaul et al.
2004/0122294 A1	6/2004	Hatlestad et al.	2007/0082789 A1	4/2007	Nissila et al.
2004/0122702 A1	6/2004	Sabol et al.	2007/0083092 A1	4/2007	Rippo et al.
			2007/0083095 A1	4/2007	Rippo et al.
			2007/0088221 A1	4/2007	Stahmann
			2007/0093702 A1	4/2007	Yu et al.

(56)	References Cited		2010/0217099 A1*	8/2010	LeBoeuf	A61B 5/00 600/301
	U.S. PATENT DOCUMENTS		2010/0217102 A1	8/2010	LeBoeuf et al.	
2007/0106167 A1	5/2007	Kinast	2010/0217103 A1	8/2010	Abdul-Hafiz et al.	
2007/0112598 A1	5/2007	Heckerman et al.	2010/0222655 A1	9/2010	Starr et al.	
2007/0116314 A1	5/2007	Grilliot et al.	2010/0228315 A1	9/2010	Nielsen	
2007/0118043 A1	5/2007	Oliver et al.	2010/0234714 A1	9/2010	Mercier et al.	
2007/0165872 A1	7/2007	Bridger et al.	2010/0268056 A1	10/2010	Picard et al.	
2007/0167850 A1	7/2007	Russell et al.	2010/0274100 A1	10/2010	Behar et al.	
2007/0191718 A1	8/2007	Nakamura	2010/0274109 A1	10/2010	Hu et al.	
2007/0197878 A1	8/2007	Shklarski	2010/0292589 A1	11/2010	Goodman	
2007/0213020 A1	9/2007	Novac	2010/0298653 A1	11/2010	McCombie et al.	
2007/0233403 A1	10/2007	Alwan et al.	2011/0028810 A1	2/2011	Van Slyke et al.	
2007/0265097 A1	11/2007	Havukainen	2011/0028813 A1	2/2011	Watson et al.	
2007/0270667 A1	11/2007	Coppi et al.	2011/0081037 A1	4/2011	Oh et al.	
2007/0270671 A1	11/2007	Gal	2011/0105869 A1	5/2011	Wilson et al.	
2007/0293781 A1	12/2007	Sims et al.	2011/0112382 A1	5/2011	Li et al.	
2007/0299330 A1	12/2007	Couronne et al.	2011/0130638 A1	6/2011	Raridan, Jr.	
2008/0004536 A1	1/2008	Baxi et al.	2011/0142371 A1	6/2011	King et al.	
2008/0015424 A1	1/2008	Bernreuter	2011/0288379 A1	11/2011	Wu	
2008/0039731 A1	2/2008	McCombie et al.	2011/0311119 A1*	12/2011	Jeanne	G06T 7/20 382/128
2008/0076972 A1	3/2008	Dorogusker et al.	2012/0030547 A1	2/2012	Raptis et al.	
2008/0081963 A1	4/2008	Naghavi et al.	2012/0095303 A1	4/2012	He	
2008/0086533 A1	4/2008	Neuhauser et al.	2012/0116231 A1	5/2012	Liao et al.	
2008/0096726 A1	4/2008	Riley et al.	2012/0150052 A1	6/2012	Buchheim et al.	
2008/0114220 A1	5/2008	Banet et al.	2012/0156933 A1	6/2012	Kreger et al.	
2008/0132798 A1	6/2008	Hong et al.	2012/0179011 A1	7/2012	Moon et al.	
2008/0141301 A1	6/2008	Azzaro et al.	2012/0197093 A1	8/2012	LeBoeuf et al.	
2008/0146890 A1	6/2008	LeBoeuf et al.	2012/0277548 A1	11/2012	Burton	
2008/0146892 A1	6/2008	LeBoeuf et al.	2013/0053661 A1	2/2013	Alberth et al.	
2008/0154098 A1	6/2008	Morris et al.	2013/0072765 A1	3/2013	Kahn et al.	
2008/0154105 A1	6/2008	Lemay	2013/0131519 A1	5/2013	LeBoeuf et al.	
2008/0165017 A1	7/2008	Schwartz	2013/0245387 A1	9/2013	Patel	
2008/0170600 A1	7/2008	Sattler et al.	2013/0336495 A1	12/2013	Burgett et al.	
2008/0171945 A1	7/2008	Dotter	2014/0051940 A1	2/2014	Messerschmidt	
2008/0177162 A1	7/2008	Bae et al.	2014/0052567 A1	2/2014	Bhardwaj et al.	
2008/0200774 A1	8/2008	Luo	2014/0073486 A1	3/2014	Ahmed et al.	
2008/0203144 A1	8/2008	Kim	2014/0088433 A1	3/2014	Shan	
2008/0221461 A1	9/2008	Zhou et al.	2014/0100432 A1	4/2014	Golda et al.	
2008/0249594 A1	10/2008	Dietrich	2014/0127996 A1	5/2014	Park et al.	
2008/0287752 A1	11/2008	Stroetz et al.	2014/0219467 A1	8/2014	Kurtz	
2009/0005662 A1	1/2009	Petersen et al.	2014/0236531 A1	8/2014	Carter	
2009/0006457 A1	1/2009	Stivoric et al.	2014/0275852 A1	9/2014	Hong et al.	
2009/0010461 A1	1/2009	Klinghult et al.	2014/0288436 A1	9/2014	Venkatraman et al.	
2009/0030350 A1	1/2009	Yang et al.	2014/0323880 A1	10/2014	Ahmed et al.	
2009/0054751 A1	2/2009	Babashan et al.	2014/0378844 A1	12/2014	Fei	
2009/0054752 A1	2/2009	Jonnalagadda et al.	2015/0011898 A1	1/2015	Romesburg	
2009/0069645 A1	3/2009	Nielsen et al.	2015/0018636 A1	1/2015	Romesburg	
2009/0082994 A1	3/2009	Schuler et al.	2015/0057967 A1	2/2015	Albinali	
2009/0088611 A1	4/2009	Buschmann	2015/0190085 A1	7/2015	Nathan et al.	
2009/0093687 A1	4/2009	Telfort et al.	2015/0250396 A1	9/2015	Ahmed et al.	
2009/0105548 A1	4/2009	Bart	2015/0265217 A1	9/2015	Penders et al.	
2009/0105556 A1	4/2009	Fricke et al.	2015/0289820 A1	10/2015	Miller et al.	
2009/0112071 A1	4/2009	LeBoeuf et al.	2015/0342481 A1	12/2015	Liu et al.	
2009/0131761 A1	5/2009	Moroney, III et al.	2015/0366509 A1	12/2015	Romesburg	
2009/0131764 A1	5/2009	Lee et al.	2016/0022220 A1	1/2016	Lee et al.	
2009/0175456 A1	7/2009	Johnson	2016/0029964 A1	2/2016	LeBoeuf et al.	
2009/0177097 A1	7/2009	Ma et al.	2016/0094899 A1	3/2016	Aumer et al.	
2009/0214060 A1	8/2009	Chuang et al.	2016/0287108 A1	10/2016	Wei et al.	
2009/0221888 A1	9/2009	Wijesiriwardana	2017/0034615 A1	2/2017	Mankodi et al.	
2009/0227853 A1	9/2009	Wijesiriwardana				
2009/0240125 A1	9/2009	Such et al.				
2009/0253992 A1	10/2009	Van Der Loo				
2009/0253996 A1	10/2009	Lee et al.				
2009/0264711 A1	10/2009	Schuler et al.				
2009/0270698 A1	10/2009	Shioi et al.				
2009/0287067 A1	11/2009	Dorogusker et al.				
2009/0299215 A1	12/2009	Zhang				
2010/0004517 A1	1/2010	Bryenton et al.				
2010/0022861 A1	1/2010	Cinbis et al.				
2010/0045663 A1	2/2010	Chen et al.				
2010/0100013 A1	4/2010	Hu et al.				
2010/0113948 A1	5/2010	Yang et al.				
2010/0168531 A1	7/2010	Shaltis et al.				
2010/0172522 A1	7/2010	Mooring et al.				
2010/0179389 A1	7/2010	Moroney et al.				
2010/0185105 A1	7/2010	Baldinger				
2010/0217098 A1	8/2010	LeBoeuf et al.				
			FOREIGN PATENT DOCUMENTS			
			CN	201438747 U	4/2010	
			DE	3910749 A1	10/1990	
			EP	1 297 784 A1	4/2003	
			EP	1 480 278 A2	11/2004	
			EP	2 077 091 A2	7/2009	
			EP	2 182 839 B1	10/2011	
			GB	2 408 209 A	5/2005	
			JP	7-241279	9/1995	
			JP	9-253062	9/1997	
			JP	9-299342	11/1997	
			JP	2000-116611	4/2000	
			JP	2001-025462	1/2001	
			JP	2003-159221	6/2003	
			JP	2004-513750 A	5/2004	
			JP	2004-283523	10/2004	

(56)

References Cited

FOREIGN PATENT DOCUMENTS

JP	2007-044203	2/2007
JP	2007-185348	7/2007
JP	2008-136556 A	6/2008
JP	2008-279061 A	11/2008
JP	2009-153664 A	7/2009
JP	2010-526646	8/2010
JP	2014-068733 A	4/2014
KR	20-0204510 Y1	11/2000
WO	WO 00/24064	4/2000
WO	WO 00/47108 A1	8/2000
WO	WO 01/08552 A1	2/2001
WO	WO 2002/017782 A2	3/2002
WO	WO 2005/010568 A2	2/2005
WO	WO 2005/020121 A1	3/2005
WO	WO 2005/110238 A1	11/2005
WO	WO 2006/009830 A2	1/2006
WO	WO 2006/067690 A2	6/2006
WO	WO 2007/012931 A2	2/2007
WO	WO 2007/023426 A2	3/2007
WO	WO 2007/038432 A2	4/2007
WO	WO 2007/053146 A1	5/2007
WO	WO 2008/141306 A2	11/2008
WO	WO 2011/094875 A1	8/2011
WO	WO 2013/038296 A1	3/2013
WO	WO 2014/092932 A1	6/2014
WO	WO 2015/128226 A1	9/2015

OTHER PUBLICATIONS

"U.S. Army Fitness Training Handbook" by the Department of the Army, 2003, The Lyons Press. p. 17.

"Warfighter Physiological and Environmental Monitoring: A Study for the U.S. Army Research Institute in Environmental Medicine and the Soldier Systems Center", Massachusetts Institute of Technology Lincoln Laboratory, Final Report, Nov. 1, 2004, prepared for the U.S. Army under Air Force Contract F19628-00-C-0002; approved for public release.

Anpo et al. "Photocatalytic Reduction of CO₂ With H₂O on Titanium Oxides Anchored within Micropores of Zeolites: Effects of the Structure of the Active Sites and the Addition of Pt" *J. Phys. Chem. B*, 101:2632-2636 (1997).

Bärsan et al. "Understanding the fundamental principles of metal oxide based gas sensors; the example of CO sensing with SnO₂ sensors in the presence of humidity" *Journal of Physics: Condensed Matter* 15:R813-R839 (2003).

Bott "Electrochemistry of Semiconductors" *Current Separations* 17(3):87-91 (1998).

Colligan, M. J. et al. in "The psychological effects of indoor air pollution", Bulletin of the New York Academy of Medicine, vol. 57, No. 10, Dec. 1981, p. 1014-1026.

de Paula Santos, U. et al. in "Effects of air pollution on blood pressure and heart rate variability: a panel study of vehicular traffic controllers in the city of Sao Paulo, Brazil", *European Heart Journal* (2005) 26, 193-200.

Ebert, T et al., "Influence of Hydration Status on Thermoregulation and Cycling Hill Climbing," *Med. Sci. Sport Exerc.* vol. 39, No. 2, pp. 323-329, 2007.

European Search Report corresponding to European Application No. 07862660.3 dated Apr. 25, 2012; 7 pages.

Fittriner "The Only Trainer You Need"; <http://itami.com>; Downloaded Feb. 26, 2010; © 2008 FiTrainer™; 2 pages.

Fleming et al., "A Comparison of Signal Processing Techniques for the Extraction of Breathing Rate from the Photoplethysmogram," *World Academy of Science, Engineering and Technology*, vol. 30, Oct. 2007, pp. 276-280.

Geladas et al., "Effect of cold air inhalation on core temperature in exercising subjects under stress," *The American Physiological Society*, pp. 2381-2387, 1988.

Gold, D.R. et al. in "Ambient Pollution and Heart Rate Variability", *Circulation* 2000, 101:1267-1273.

International Search Report and Written Opinion of the International Searching Authority, corresponding to PCT/US2012/0948079, dated Oct. 9, 2012.

International Search Report and Written Opinion of the International Searching Authority, corresponding to PCT/US2007/025114, dated May 13, 2008.

International Search Report Corresponding to International Application No. PCT/US2012/022634, dated Aug. 22, 2012, 9 pages.

Maomao et al., "Mobile Context-Aware Game for the Next Generation," 2nd International Conference on Application and Development of Computer Games ADCOG 2003, p. 78-81.

Martins et al. "Zinc oxide as an ozone sensor" *Journal of Applied Physics* 96(3):1398-1408 (2004).

Maughan, R.J., "Impact of mild dehydration on wellness and on exercise performance," *European Journal of Clinical Nutrition*, 57, Suppl. 2, pp. S19-S23, 2003.

Maughan et al., "Exercise, Heat, Hydration and the Brain," *Journal of the American College of Nutrition*, vol. 26, No. 5, pp. 604S-612S, 2007.

Mostardi, R., et al., "The effect of increased body temperature due to exercise on the heart rate and the maximal aerobic power," *Europ. J. Appl. Physiol*, 33, pp. 237-245, 1974.

Nakajima et al., "Monitoring of heart and respiratory rates by photoplethysmography using a digital filtering technique," *Med. Eng. Phys.*, vol. 18, No. 5, Jul. 1996, pp. 365-372.

Notification of Transmittal of the International Search Report and Written Opinion of the International Search Authority dated Jul. 30, 2010 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2010/021936.

Notification of Transmittal of the International Search Report and Written Opinion of the International Search Authority dated Aug. 26, 2010 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2010/021629.

Notification of Transmittal of the International Search Report and the Written Opinion of the International Search Authority dated Sep. 16, 2010 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2010/024922.

Notification of Transmittal of the International Search Report and the Written Opinion of the International Search Authority dated Sep. 27, 2010 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2010/025216.

Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration corresponding to International Application No. PCT/US2013/070271; dated Feb. 26, 2014; 13 pages.

Shorten et al., "Acute effect of environmental temperature during exercise on subsequent energy intake in active men," *Am. J. Clin. Nutr.* 90, pp. 1215-1221, 2009.

Skubal et al. "Detection and identification of gaseous organics using a TiO₂ sensor" *Journal of Photochemistry and Photobiology A: Chemistry* 148:103-108 (2002).

Skubal et al. "Monitoring the Electrical Response of Photoinduced Organic Oxidation on TiO₂ Surfaces" Manuscript submitted Oct. 2000 to SPIE Intl. Symposium on Environment & Industrial Sensing, Boston, MA, Nov. 5-8, 2000, sponsored by SPIE, 10 pp.

Thompson, M.W., "Cardiovascular drift and critical core temperature: factors limiting endurance performance in the heat?" *J. Exerc. Sci. Fit.* vol. 4, No. 1, pp. 15-24, 2006.

Zhang et al. "Development of Chemical Oxygen Demand On-Line Monitoring System Based on a Photoelectrochemical Degradation Principle" *Environ. Sci. Technol.*, 40(7):2363-2368 (2006).

Edmison et al., "E-Textile Based Automatic Activity Diary for Medical Annotation and Analysis," *Proc. BSN 2006 Int. Workshop Wearable Implantable Body Sensor Netw.* (2006), pp. 131-145, Apr. 3-5, 2006.

European Search Report, EP Application No. 13863449.8, dated Oct. 19, 2015, 3 pages.

European Search Report, EP Application No. 14743615.8, dated Oct. 12, 2015, 3 pages.

European Search Report, EP Application No. 14743839.4, dated Oct. 12, 2015, 3 pages.

(56)

References Cited

OTHER PUBLICATIONS

- Gibbs et al., "Reducing Motion Artifact in Wearable Bio-Sensors Using MEMS Accelerometers for Active Noise Cancellation," 2005 American Control Conference, Jun. 8-10, 2005, Portland, OR, USA, pp. 1581-1586.
- International Preliminary Report on Patentability, PCT/US2014/012940, dated Jun. 17, 2015, 23 pages.
- International Search Report and Written Opinion of the International Searching Authority, corresponding to International Patent Application No. PCT/US2014/012940, dated Oct. 16, 2014, 13 pages.
- International Search Report corresponding to International Patent Application No. PCT/US2014/012909, dated May 13, 2014, 3 pages.
- Notification Concerning Transmittal of International Preliminary Report on Patentability, PCT/US2014/012909, dated Jul. 28, 2015.
- Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2015/014562, Oct. 28, 2015.
- Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2015/042636, dated Oct. 29, 2015.
- Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2015/042015, dated Oct. 29, 2015.
- Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2015/042035, dated Oct. 29, 2015.
- Wood et al., "Active Motion Artifact Reduction for Wearable Sensors Using Laguerre Expansion and Signal Separation," Proceedings of the 2005 IEEE Engineering in Medicine and Biology, 27th Annual Conference, Shanghai, China, Sep. 1-4, 2005, pp. 3571-3574.
- Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2015/046079, dated Dec. 29, 2015.
- Communication pursuant to Article 94(3) EPC, European Patent Application No. 13863449.8, dated Nov. 5, 2015, 7 pages.
- Communication pursuant to Article 94(3) EPC, European Patent Application No. 14743615.8, dated Dec. 23, 2015, 7 pages.
- Communication pursuant to Article 94(3) EPC, European Patent Application No. 14743839.4, dated Dec. 23, 2015, 6 pages.
- Communication pursuant to Article 94(3) EPC, European Patent Application No. 12820308.0, dated Feb. 3, 2016, 5 pages.
- Notification of Transmittal of the International Search Report and Written Opinion of the International Search Authority dated May 26, 2016 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2016/019126.
- Notification of Transmittal of the International Search Report and Written Opinion of the International Search Authority dated May 26, 2016 by the Korean Intellectual Property Office for corresponding International Application No. PCT/US2016/019132.
- Asada, et al., "Mobile Monitoring with Wearable Photoplethysmographic Biosensors," IEEE Engineering in Medicine and Biology Magazine, May/Jun. 2003, pp. 28-40.
- Bifulco et al., "Bluetooth Portable Device for Continuous ECG and Patient Motion Monitoring During Daily Life," Medicon 2007, IFMBE Proceedings 16, 2007, pp. 369-372.
- Brodersen et al., "In-Ear Acquisition of Vital Signs Discloses New Chances for Preventive Continuous Cardiovascular Monitoring," 4th International Workshop on Wearable and Implantable Body Sensor Networks (BSN 2007), vol. 13 of the series IFMBE Proceedings, pp. 189-194.
- Celka et al., "Motion Resistant Earphone Located Infrared based Heart Rate Measurement Device," Proceedings of the Second IASTED International Conference on Biomedical Engineering, Feb. 16-18, 2004, Innsbruck, Austria, pp. 582-585.
- Communication Pursuant to Article 94(3) EPC, EP 12 739 502.8, Jul. 19, 2016, 7 pages.
- Communication Pursuant to Article 94(3) EPC, EP 14 743 615.8, Jul. 19, 2016, 7 pages.
- Communication Pursuant to Article 94(3) EPC, EP 14 743 839.4, Jul. 20, 2016, 5 pages.
- Comtois et al., "A Wearable Wireless Reflectance Pulse Oximeter for Remote Triage Applications," 2006 IEEE, pp. 53-54.
- Comtois, Gary, W., "Implementation of Accelerometer-Based Adaptive Noise Cancellation in a Wireless Wearable Pulse Oximeter Platform for Remote Physiological Monitoring and Triage," Thesis, Worcester Polytechnic Institute, Aug. 31, 2007, 149 pages.
- Duun et al., "A Novel Ring Shaped Photodiode for Reflectance Pulse Oximetry in Wireless Applications," IEEE Sensors 2007 Conference, pp. 596-599.
- Geun et al., "Measurement Site and Applied Pressure Consideration in Wrist Photoplethysmography," the 23rd International Technical Conference on Circuits/Systems, Computers and Communications, 2008, pp. 1129-1132.
- Gibbs et al., "Active motion artifact cancellation for wearable health monitoring sensors using collocated MEMS accelerometers," Smart Structures and Materials, 2005: Sensors and Smart Structures Technologies for Civil, Mechanical, and Aerospace Systems, Proc. of SPIE, vol. 5765, pp. 811-819.
- Haahr et al., "A Wearable "Electronic Patch" for Wireless Continuous Monitoring of Chronically Diseased Patients," Proceedings of the 5th International Workshop on Wearable and Implantable Body Sensor Networks, in conjunction with the 5th International Summer School and Symposium on Medical Devices and Biosensors, The Chinese University of Hong Kong, HKSAR, China, Jun. 1-3, 2008, pp. 66-70.
- Jiang, Honghui, "Motion-Artifact Resistant Design of Photoplethysmograph Ring Sensor for Driver Monitoring," Thesis, Massachusetts Institute of Technology, Feb. 2004, 62 pages.
- Kuzmina et al., "Compact multi-functional skin spectrometry set-up," Advanced Optical Materials, Technologies, and Devices, Proc. of SPIE, vol. 6596, 2007, pp. 65960T-1 to 65960T-6.
- Lee et al., "Respiratory Rate Detection Algorithms by Photoplethysmography Signal Processing," 30th Annual International IEEE EMBS Conference, Vancouver, British Columbia, Canada, Aug. 20-24, 2008, pp. 1140-1143.
- Lindberg et al., "Monitoring of respiratory and heart rates using a fibre-optic sensor," Med Biol Eng Comput, Sep. 1992, vol. 30, No. 5, pp. 533-537.
- Luprano, Jean, "Sensors and Parameter Extraction by Wearable Systems: Present Situation and Future," pHealth 2008, May 21, 2008, 29 pages.
- Lygouras et al., "Optical-Fiber Finger Photo-Plethysmograph Using Digital Techniques," IEEE Sensors Journal, vol. 2, No. 1, Feb. 2002, pp. 20-25.
- Maguire et al., "The Design and Clinical Use of a Reflective Brachial Photoplethysmograph," Technical Report NUM/SS—/2002/04, Submitted Apr. 2002, Signals and Systems Research Group, National University of Ireland, Maynooth, Co. Kildare, Ireland, 13 pages.
- Mendelson et al., "Measurement Site and Photodetector Size Considerations in Optimizing Power Consumption of a Wearable Reflectance Pulse Oximeter," Proceedings of the 25th Annual International Conference of the IEEE EMBS, Cancun, Mexico, Sep. 17-21, 2003, pp. 3016-3019.
- Mendelson et al., "Noninvasive Pulse Oximetry Utilizing Skin Reflectance Photoplethysmography," IEEE Transactions on Biomedical Engineering, vol. 35, No. 10, Oct. 1988, pp. 798-805.
- Poh et al., "Motion Tolerant Magnetic Earring Sensor and Wireless Earpiece for Wearable Photoplethysmography," IEEE Transactions on Information Technology in Biomedicine, vol. 14, No. 3, May 2010, pp. 786-794.
- Renevey et al., "Wrist-Located Pulse Detection Using IR Signals, Activity and Nonlinear Artifact Cancellation," IEEE EMBS, 2001, 4 pages.
- Rhee et al., "Artifact-Resistant Power-Efficient Design of Finger-Ring Plethysmographic Sensors," IEEE Transactions on Biomedical Engineering, vol. 48, No. 7, Jul. 2001, pp. 795-805.
- Shaltis, Phillip Andrew, Analysis and Validation of an Artifact Resistant Design for Oxygen Saturation Measurement Using Photo

(56)

References Cited

OTHER PUBLICATIONS

Plethysmographic Ring Sensors, Thesis, Massachusetts Institute of Technology, Jun. 2004, 103 pages.

Shin et al., "A Novel Headset with a Transmissive PPG Sensor for Heart Rate Measurement," ICBME 2008, Proceedings 23, 2009, pp. 519-522.

Spigulis et al., "Wearable wireless photoplethysmography sensors," Proc. of SPIE, vol. 6991, 2008, pp. 69912O-1 to 69912O-7.

Takatani et al., "Optical Oximetry Sensors for Whole Blood and Tissue," IEEE Engineering in Medicine and Biology, Jun./Jul. 1994, pp. 347-357.

Vogel et al., "A System for Assessing Motion Artifacts in the Signal of a Micro-Optic In-Ear Vital Signs Sensor," 30th Annual International IEEE EMBS Conference, Vancouver, British Columbia, Canada, Aug. 20-24, 2008.

Vogel et al., "In-Ear Heart Rate Monitoring Using a Micro-Optic Reflective Sensor," Proceedings of the 29th Annual International Conference of the IEEE EMBS Cite Internationale, Lyon, France, Aug. 23-26, 2007, pp. 1375-1378.

Wang et al., "Multichannel Reflective PPG Earpiece Sensor With Passive Motion Cancellation," IEEE Transactions on Biomedical Circuits and Systems, vol. 1, No. 4, Dec. 2007, pp. 235-241.

Wang et al., "Reflective Photoplethysmograph Earpiece Sensor for Ubiquitous Heart Rate Monitoring," 4th International Workshop on Wearable and Implantable Body Sensor Networks, 2007, vol. 13 of the series IFMBE Proceedings, pp. 179-183.

Wei et al., "A New Wristband Wearable Sensor Using Adaptive Reduction Filter to Reduce Motion Artifact," Proceedings of the 5th

International Conference on Information Technology and Application in Biomedicine, in conjunction with the 2nd International Symposium & Summer School on Biomedical and Health Engineering, Shenzhen, China, May 30-31, 2008, pp. 278-281.

Wood, Levi Benjamin, "Motion Artifact Reduction for Wearable Photoplethysmogram Sensors Using Micro Accelerometers and Laguerre Series Adaptive Filters," Thesis, Massachusetts Institute of Technology, Jun. 2008, 74 pages.

Han et al., "Artifacts in wearable photoplethysmographs during daily life motions and their reduction with least mean square based active noise cancellation method," Computers in Biology and Medicine, 42, 2012, pp. 387-393.

Extended European Search Report, European Application No. 16184560.7, dated Dec. 20, 2016, 9 pages.

Extended European Search Report, European Application No. 16183137.5, dated Jan. 12, 2017, 12 pages.

Communication pursuant to Article 94(3) EPC, European Application No. 12 739 502.8, dated Nov. 30, 2016, 6 pages.

Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2016/046273, dated Nov. 25, 2016, 24 pages.

Notification of Transmittal of the International Search Report and the Written Opinion of the International Searching Authority, or the Declaration, PCT/US2016/058098, dated Jan. 10, 2017, 13 pages.

Communication pursuant to Article 94(3) EPC, European Application No. 14 743 615.8, Jan. 30, 2017, 5 pages.

Communication pursuant to Article 94(3) EPC, European Application No. 14 743 839.4, dated Jan. 30, 2017, 7 pages.

* cited by examiner

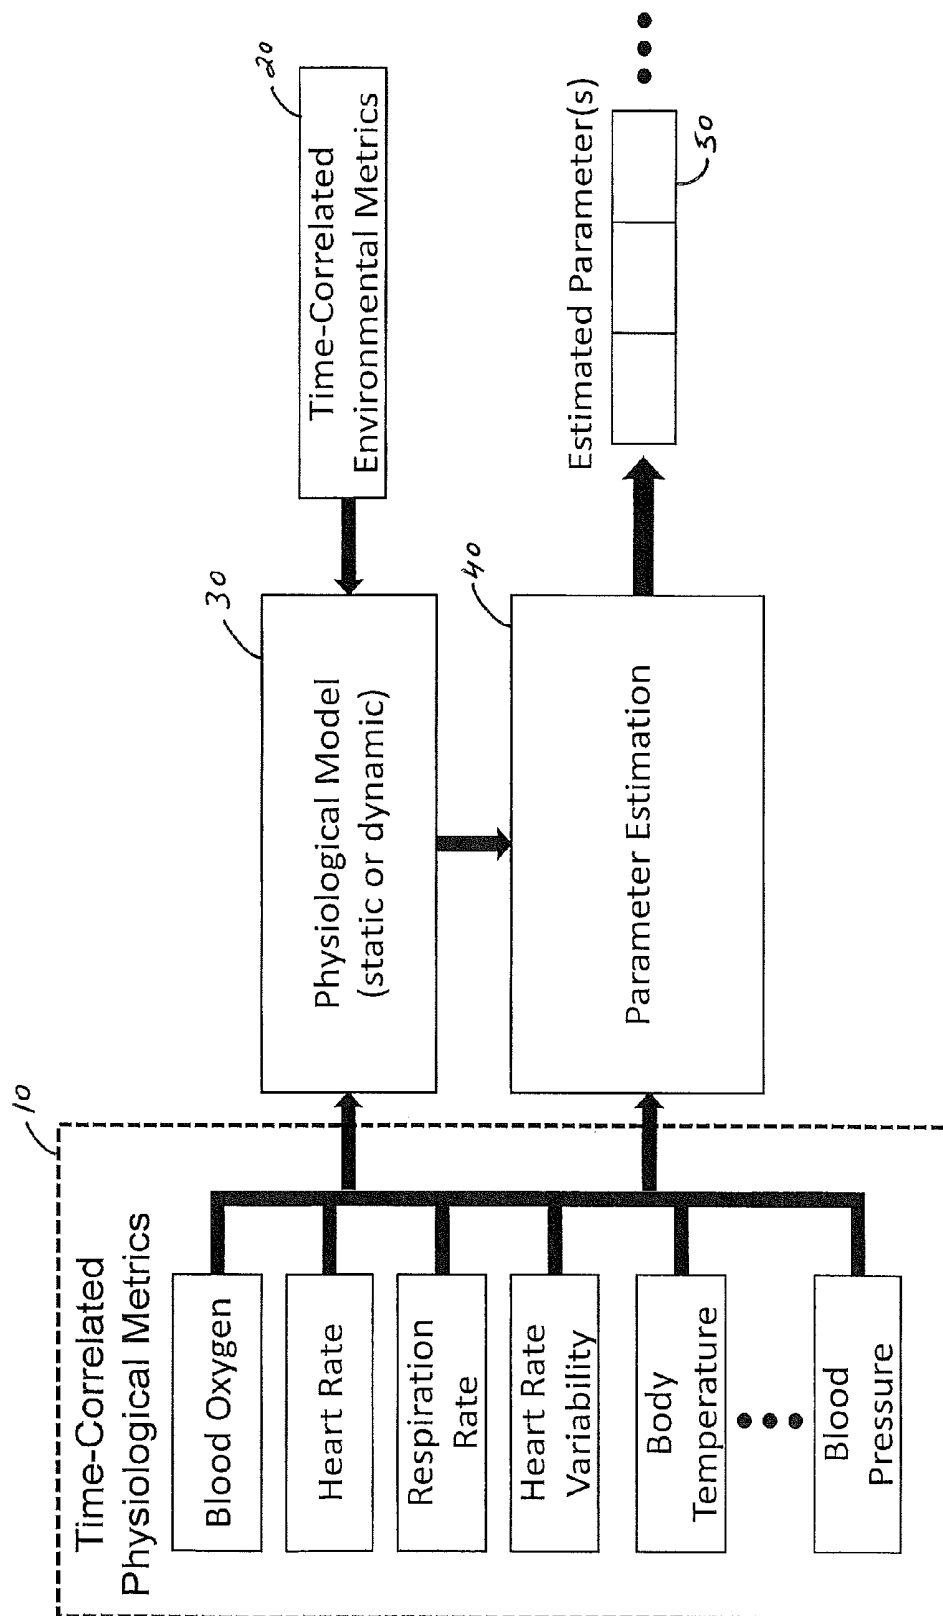


Figure 1

Average Core Body Temperature vs. Time
For average human over average day

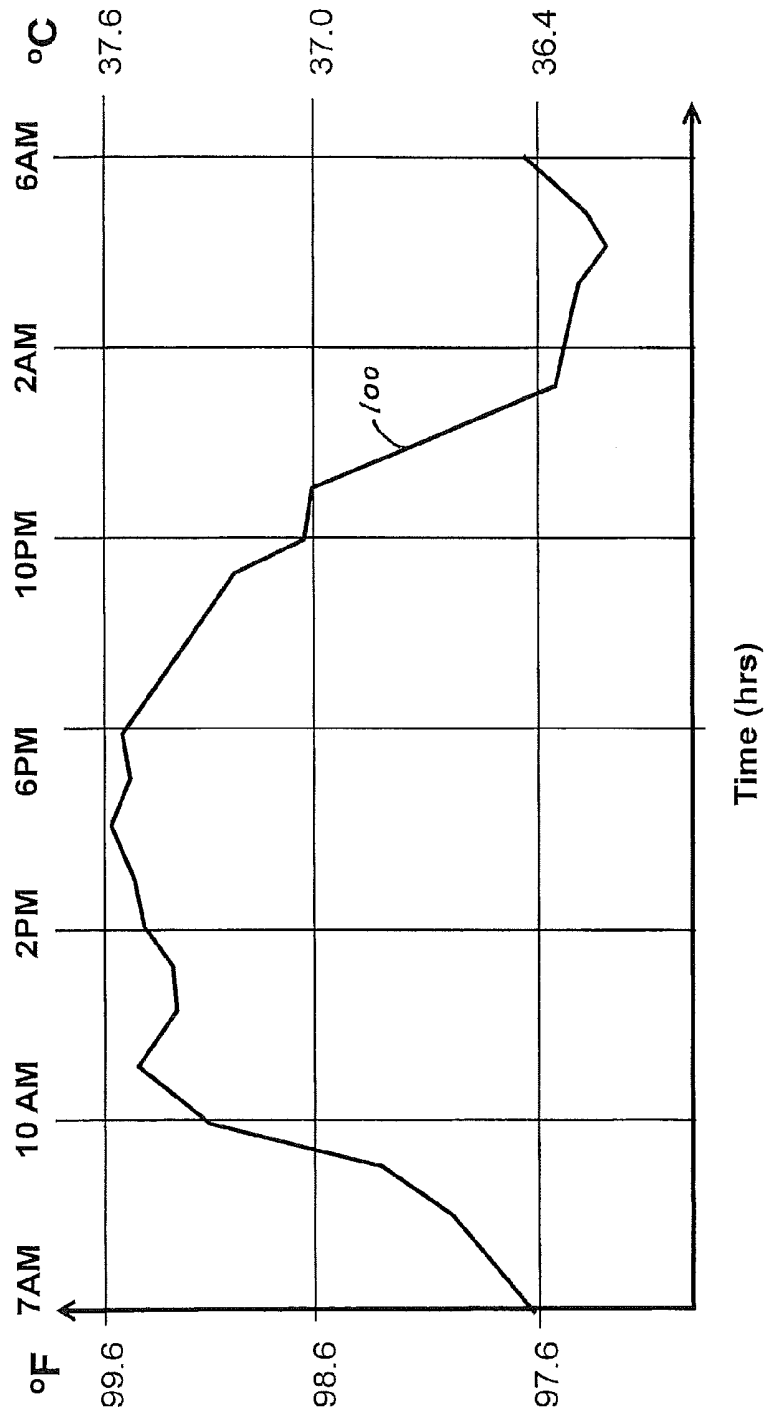


Figure 2

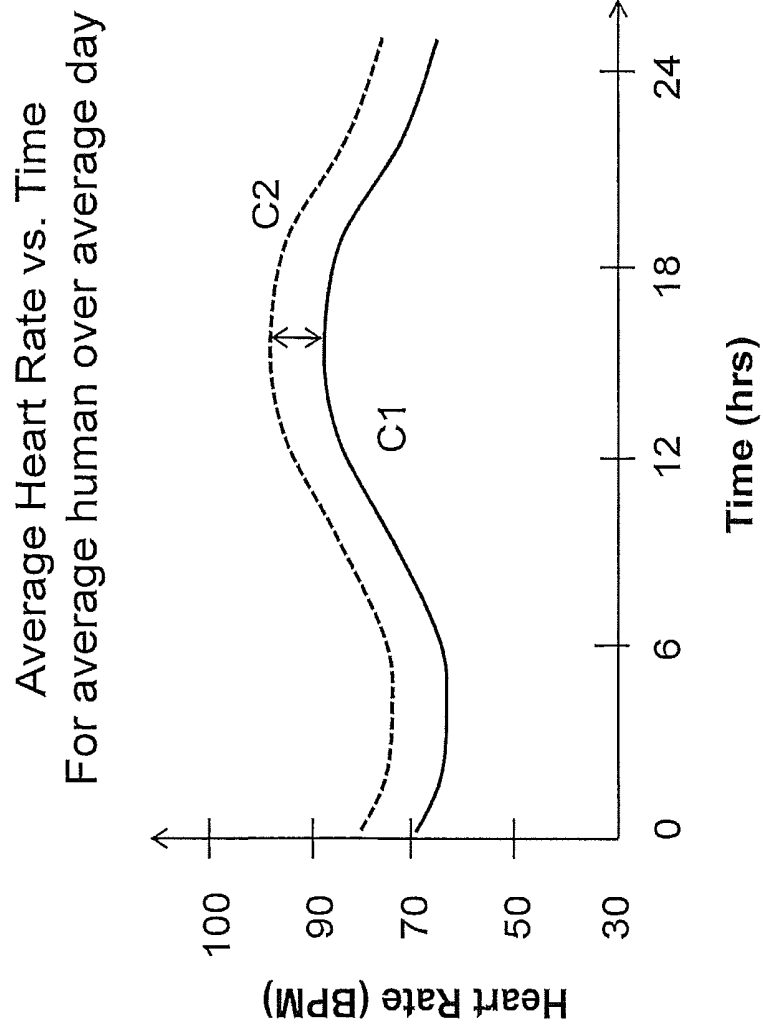


Figure 3

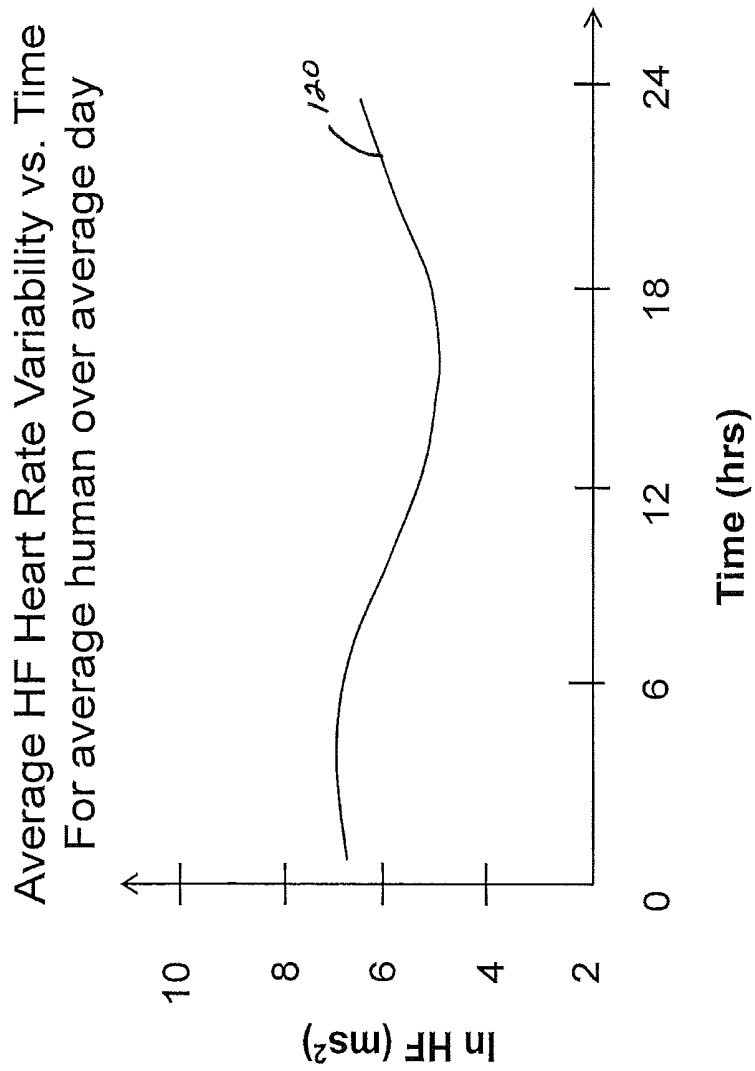


Figure 4

Exemplary Relationship between Heart Rate & Activity
for Average Human Wearing Accelerometer(s)

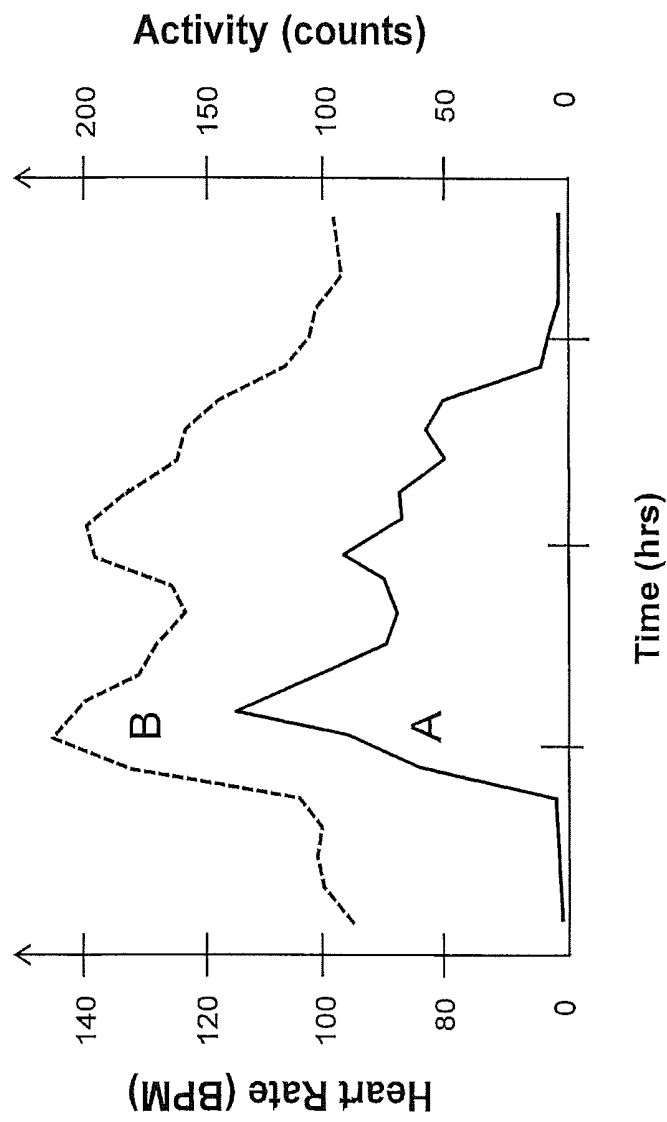
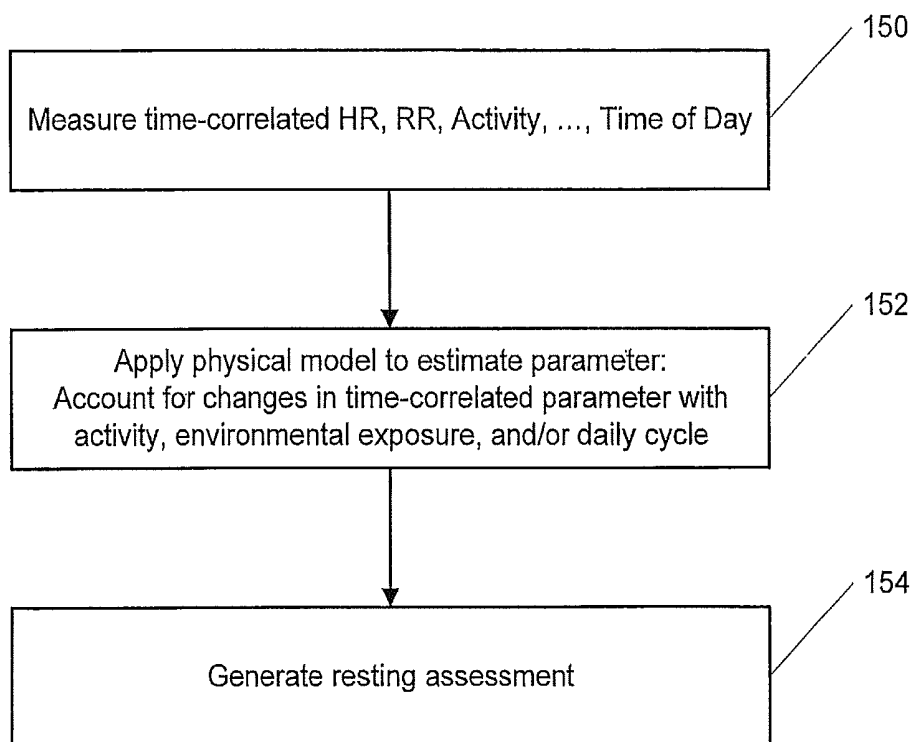


Figure 5

*Figure 6*

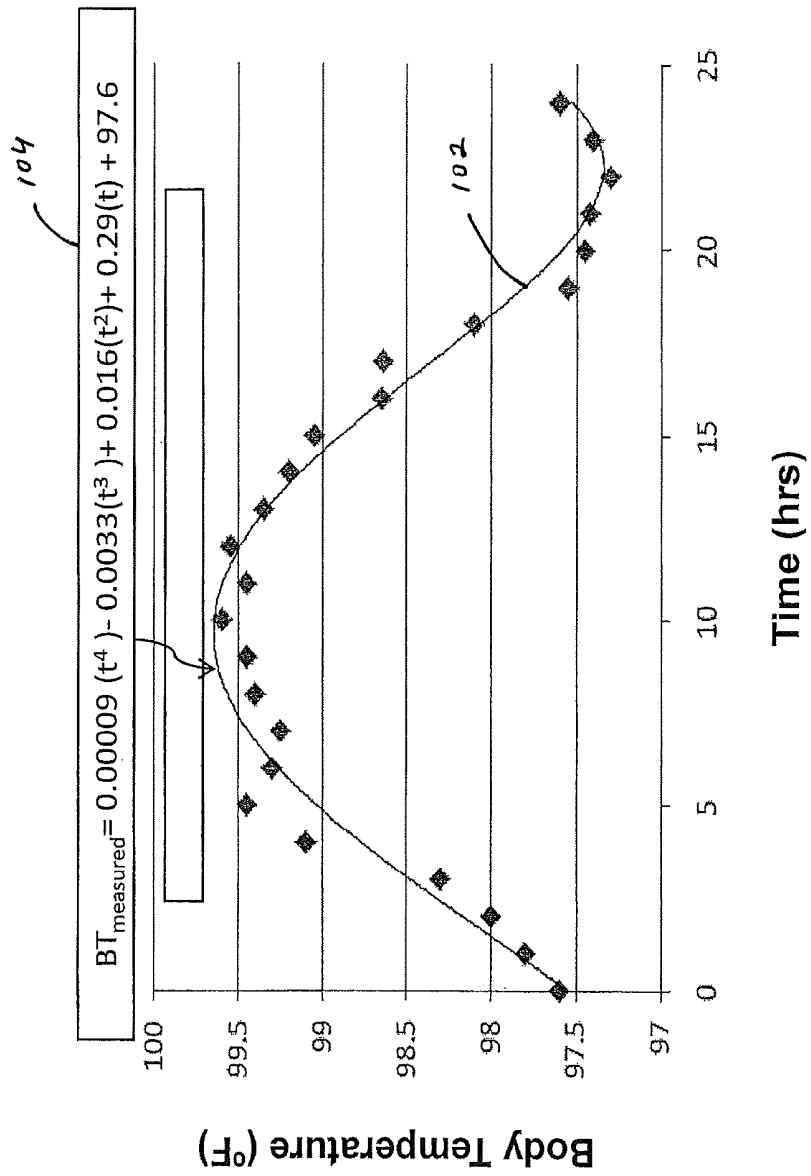


Figure 7

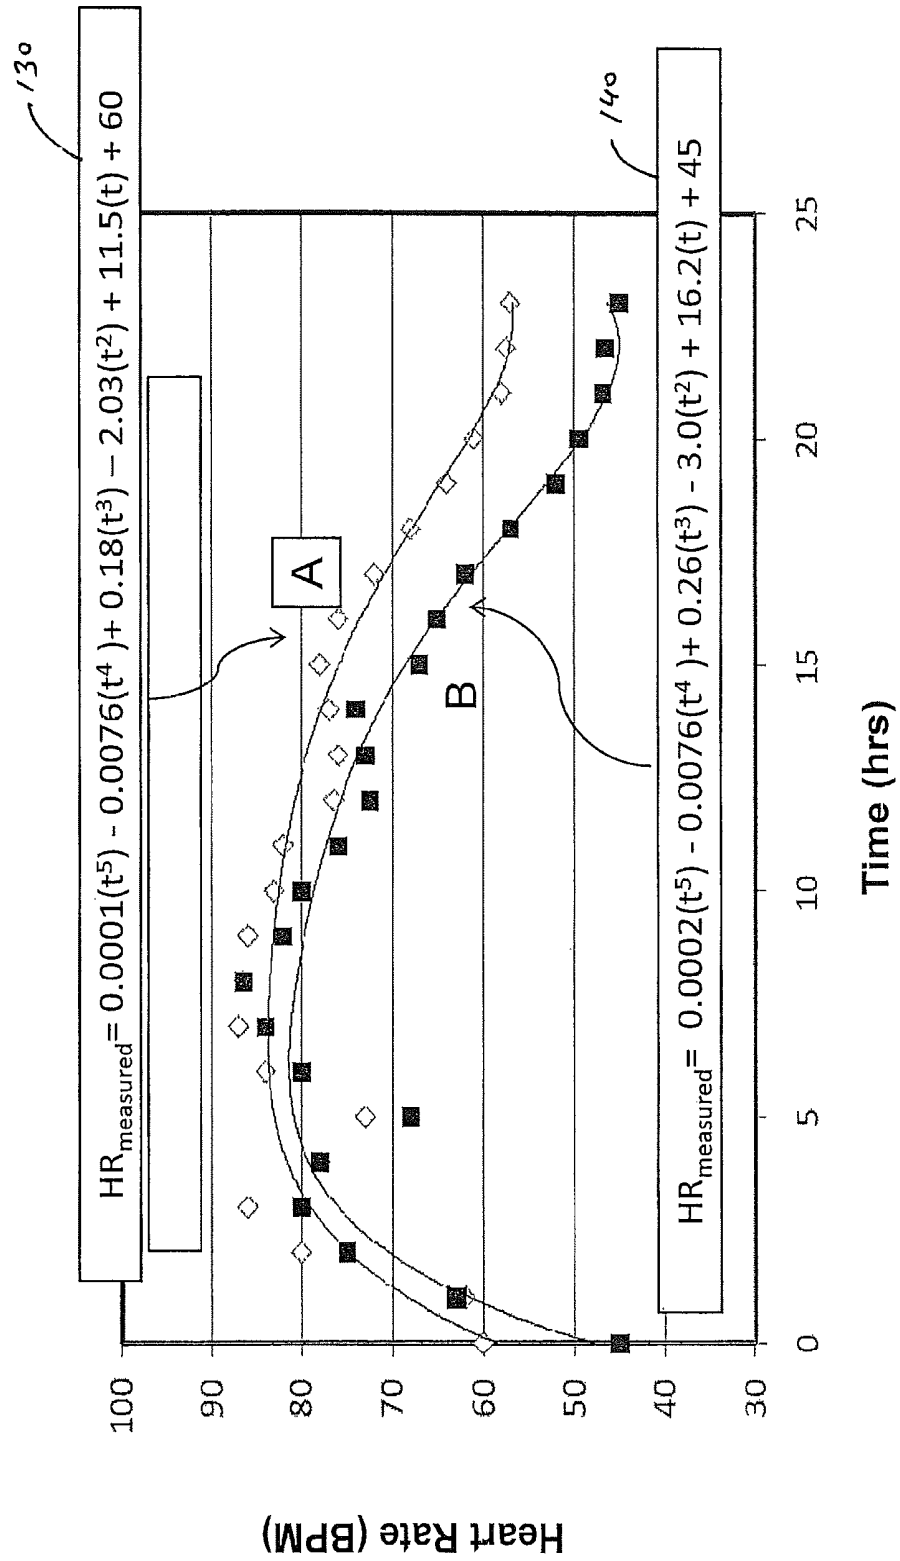


Figure 8

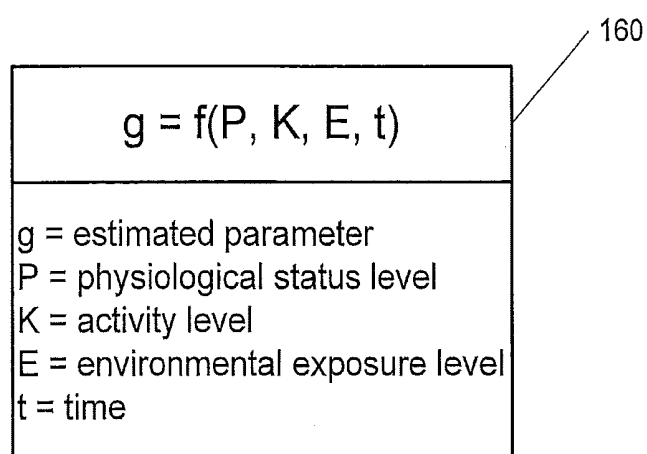



Figure 9



110

Time of Day	Measured Value	% Multiplier	Resting Estimation
7:00 AM		1	
9:00 AM		0.995918	
10:00 AM		0.992879	
12:00 PM		0.981398	
2:00 PM		0.983375	
4:00 PM		0.981398	
6:00 PM	99.5°F	0.981398	97.6°F
8:00 PM		0.982386	
10:00 PM		0.985361	
12:00 AM		0.989457	
2:00 AM		1.000513	
4:00 AM		1.001848	
6:00 AM		1.002053	

Figure 10

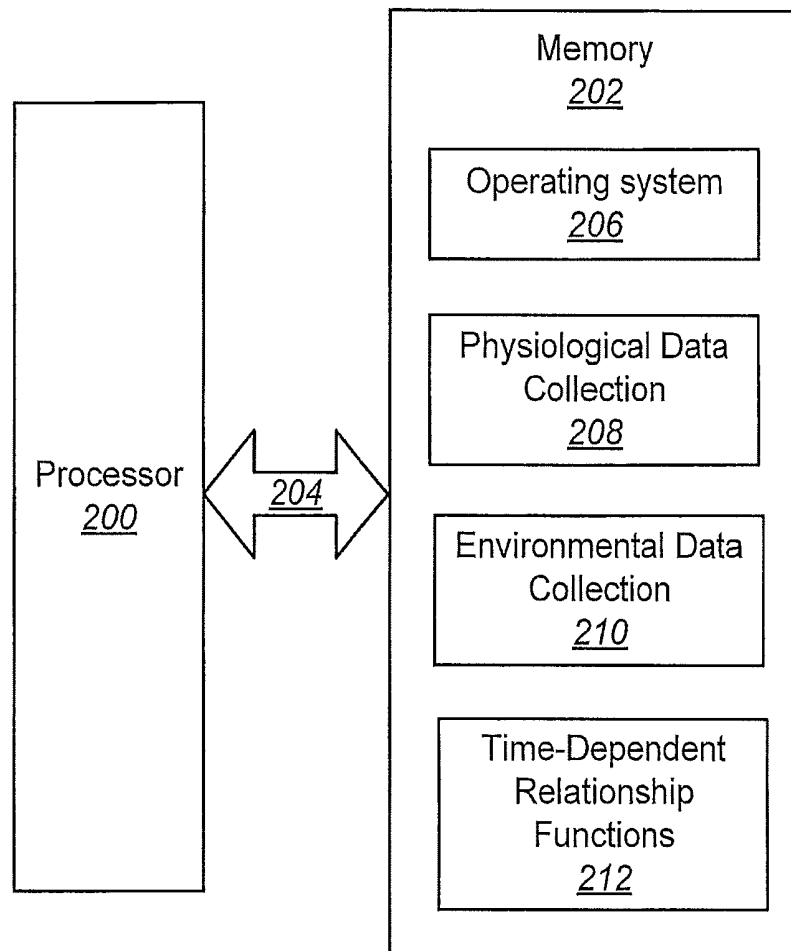*Figure 11*

APPARATUS AND METHODS FOR ESTIMATING TIME-STATE PHYSIOLOGICAL PARAMETERS

RELATED APPLICATIONS

This application is a continuation application of U.S. patent application Ser. No. 15/219,770, filed Jul. 26, 2016, now U.S. Pat. No. 9,521,962, which is a continuation application of U.S. patent application Ser. No. 14/116,641, filed Nov. 8, 2013, now U.S. Pat. Ser. No. 9,427,191, which is a 35 U.S.C. §371 national stage application of PCT Application No. PCT/US2012/046446, filed Jul. 12, 2012, which claims the benefit of and priority to U.S. Provisional Patent Application No. 61/511,238 filed Jul. 25, 2011, the disclosures of which are incorporated herein by reference as if set forth in their entireties.

FIELD OF THE INVENTION

The present invention relates generally to monitoring apparatus and methods and, more particularly, to physiological monitoring apparatus and methods.

BACKGROUND OF THE INVENTION

Physiological parameters for living beings are typically a function of one or more of the following: the time-of-day, environmental conditions to which a being is exposed, activity level of a being, and various other physiological parameters. Many of these are related. For example, the average change in heart rate, body temperature, and heart rate variability (HRV) with the time-of-day are generally known based on human and animal studies of the circadian cycle.

SUMMARY

It should be appreciated that this Summary is provided to introduce a selection of concepts in a simplified form, the concepts being further described below in the Detailed Description. This Summary is not intended to identify key features or essential features of this disclosure, nor is it intended to limit the scope of the invention.

According to some embodiments of the present invention, a method of determining a value of a physiological parameter for a subject at a selected state (e.g., state of peak metabolism, state of lowered metabolism, state of rest, etc.), includes obtaining, via a device attached to the subject, a value of the physiological parameter of the subject at a particular time-of-day, and applying a time-dependent relationship function to the obtained physiological parameter value via at least one processor to determine a value of the physiological parameter at the selected state. Exemplary physiological parameters include, but are not limited to, subject body temperature, subject heart rate, subject heart rate variability, subject blood gas levels, subject metabolic rate, subject respiration rate, subject blood analyte levels, subject blood pressure, subject pulse pressure, etc. In some embodiments of the present invention, the time-dependent relationship function is derived from a circadian rhythm for the subject. In some embodiments of the present invention, the time-dependent relationship function is a lookup table.

In some embodiments of the present invention, determining a value of the physiological parameter of the subject at a selected state may include obtaining the value of the physiological parameter at the same time-of-day for multiple

days and determining an average value for the multiple obtained values. Applying the time-dependent relationship function to the obtained physiological parameter value may include applying the time-dependent relationship function to the average value.

In some embodiments of the present invention, determining a value of a physiological parameter for a subject at a selected state may further include determining if the subject is in a condition of heightened activity at the selected time-of-day by determining via the device if at least one obtained physiological parameter value is at a level associated with the heightened activity condition. The time-dependent relationship function is adjusted for the heightened activity condition of the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, prior to obtaining a value of the physiological parameter of the subject at a particular time-of-day, values of the physiological parameter of the subject are obtained at multiple times during at least one previous day. A personalized time-dependent relationship function between at least one obtained value of the physiological parameter and a value of the physiological parameter at a time when the subject is at the selected state is generated for the subject using the obtained values from the at least one previous day. Applying the time-dependent relationship function to the obtained physiological parameter value includes applying the personalized time-dependent relationship function to the obtained physiological parameter value via at least one processor to determine a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for calories consumed by the subject prior to determining a value of the physiological parameter at a time when the subject is at the selected state.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for blood oxygen level of the subject prior to determining a value of the physiological parameter at a time when the subject is at the selected state.

In some embodiments of the present invention, the device includes at least one physiological sensor that is configured to detect and/or measure physiological information from the subject to which the device is attached.

In some embodiments of the present invention, the device includes at least one environmental sensor that detects and/or measures environmental condition information in a vicinity of the subject. Determining a value of a physiological parameter for a subject at a selected state, according to some embodiments of the present invention, further comprises obtaining, via the device, a value of an environmental parameter in a vicinity of the subject at the particular time-of-day. Applying the time-dependent relationship function to the obtained physiological parameter value comprises applying the time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value via the at least one processor to determine a value of the physiological parameter at a time when the subject is at the selected state.

Devices according to embodiments of the present invention may be configured to be attached to various portions of the body of a subject including, but not limited to, ear, arm, wrist, leg, hand, foot, finger, toe, chest, head, hair, nose, waist, trunk, shoulder, and neck. Devices according to embodiments of the present invention may also be configured to be embedded within clothing, foot apparel, and other

wearable objects, without limitation. Additionally, devices according to embodiments of the present invention may be worn outside the body so as to be noninvasive, may be worn inside the body so as to be invasive, or may be worn subdermally so as to be mildly invasive.

According to other embodiments of the present invention, a method of determining a value of a physiological parameter (e.g., subject body temperature, subject heart rate, subject heart rate variability, subject blood gas levels, subject metabolic rate, subject respiration rate, subject blood analyte levels, subject blood pressure, and subject pulse pressure, etc.) for a subject at rest comprises obtaining, via a device attached to the subject, a value of the physiological parameter of the subject at a particular time-of-day, and applying a time-dependent relationship function to the obtained physiological parameter value via at least one processor to determine a value of the physiological parameter at a time when the subject is at rest.

In some embodiments of the present invention, determining a value of the physiological parameter of the subject at rest comprises obtaining the value of the physiological parameter at the same time-of-day for multiple days and determining an average value for the multiple obtained values. Applying the time-dependent relationship function to the obtained physiological parameter value may include applying the time-dependent relationship function to the average value.

In some embodiments of the present invention, determining a value of a physiological parameter for a subject at rest may further include determining if the subject is in a condition of heightened activity at the time-of-day by determining via the device if at least one obtained physiological parameter value is at a level associated with heightened activity. The time-dependent relationship function is adjusted for the heightened activity condition of the subject prior to determining a value of the physiological parameter at a time when the subject is at rest.

In some embodiments of the present invention, prior to obtaining a value of the physiological parameter of the subject at the time-of-day, values of the physiological parameter of the subject are obtained at multiple times during at least one previous day. A personalized time-dependent relationship function between at least one obtained value of the physiological parameter and a value of the physiological parameter at a time when the subject is at rest is generated for the subject using the obtained values from the at least one previous day. Applying the time-dependent relationship function to the obtained physiological parameter value includes applying the personalized time-dependent relationship function to the obtained physiological parameter value via the processor to determine a value of the physiological parameter at a time when the subject is at rest.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for calories consumed by the subject prior to determining a value of the physiological parameter at a time when the subject is at rest.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for blood oxygen level of the subject prior to determining a value of the physiological parameter at a time when the subject is at rest.

In some embodiments of the present invention, the device includes at least one environmental sensor that detects and/or measures environmental condition information in a vicinity of the subject. Determining a value of a physiological parameter for a subject at rest, according to some embodiments of the present invention, further comprises

obtaining, via the device, a value of an environmental parameter in a vicinity of the subject at a particular time-of-day. Applying the time-dependent relationship function to the obtained physiological parameter value comprises applying the time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value via at least one processor to determine a value of the physiological parameter at a time when the subject is at rest.

According to other embodiments of the present invention, a method of determining a value of a physiological parameter for a subject at a selected state (e.g., state of peak metabolism, state of lowered metabolism, state of rest, etc.) includes obtaining, via a device attached to the subject, a value of the physiological parameter (e.g., subject body temperature, subject heart rate, subject heart rate variability, subject blood gas levels, subject metabolic rate, subject respiration rate, subject blood analyte levels, subject blood pressure, and subject pulse pressure, etc.) of the subject at a selected time-of-day; obtaining, via the device, a value of an environmental parameter in a vicinity of the subject at the selected time-of-day via the environmental sensor; determining if the subject is in a condition of heightened activity at the selected time-of-day by determining via the device if at least one obtained physiological parameter value is at a level associated with heightened activity; and applying a time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value via a processor to determine a value of the physiological parameter at the selected state, wherein the time-dependent relationship function is adjusted for the heightened activity condition of the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, obtaining a value of the physiological parameter of the subject at a particular time-of-day includes obtaining the value at the same time-of-day for multiple days and determining an average value for the multiple obtained values. Applying the time-dependent relationship function and the environmental-dependent relationship function to the obtained physiological parameter value includes applying the time-dependent relationship function and the environmental-dependent relationship function to the average value.

In some embodiments of the present invention, prior to obtaining a value of the physiological parameter of the subject at a particular time-of-day, values of the physiological parameter of the subject are obtained at multiple times during at least one previous day, and a personalized time-dependent relationship function between at least one obtained value of the physiological parameter and a value of the physiological parameter at the selected state is generated for the subject using the obtained values from the at least one previous day. Applying the time-dependent relationship function and the environmental-dependent relationship function to the obtained physiological parameter value includes applying the personalized time-dependent relationship function and the environmental-dependent relationship function to the obtained physiological parameter value via at least one processor to determine a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for calories consumed by the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the time-dependent relationship function is adjusted for blood oxygen

level of the subject prior to determining a value of the physiological parameter at the selected state.

According to other embodiments of the present invention, an apparatus includes a housing configured to be attached to a subject and at least one physiological sensor attached to the housing, wherein the at least one physiological sensor detects and/or measures physiological information from the subject. At least one processor may be attached to the housing or may be located remotely from the housing. The at least one processor is in communication with the at least one physiological sensor and is configured to obtain from the at least one physiological sensor a value of a physiological parameter of the subject at a particular time-of-day, and to apply a time-dependent relationship function to the obtained physiological parameter value to determine a value of the physiological parameter at a selected state.

In some embodiments of the present invention, the at least one processor is configured to obtain from the at least one physiological sensor the value of the physiological parameter at the same time-of-day for multiple days, determine an average value for the multiple obtained values, and apply the time-dependent relationship function to the average value.

In some embodiments of the present invention, the at least one processor is configured to determine if the subject is in a condition of heightened activity at the time-of-day by determining if at least one obtained physiological parameter value is at a level associated with heightened activity, and adjust the time-dependent relationship function for the heightened activity condition of the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the at least one processor is configured to obtain values of the physiological parameter of the subject at multiple times during at least one previous day, generate a personalized time-dependent relationship function between at least one obtained value of the physiological parameter and a value of the physiological parameter at the selected state using the obtained values from the at least one previous day, and apply the personalized time-dependent relationship function to the obtained physiological parameter value to determine a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the apparatus includes an environmental sensor that detects and/or measures environmental condition information in a vicinity of the subject. The at least one processor is configured to obtain a value of an environmental parameter in a vicinity of the subject at a particular time-of-day from the environmental sensor, and to apply the time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value to determine a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the at least one processor is configured to adjust the time-dependent relationship function for calories consumed by the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the at least one processor is configured to adjust the time-dependent relationship function for blood oxygen level of the subject prior to determining a value of the physiological parameter at the selected state.

In some embodiments of the present invention, the housing is configured to be attached to an ear of the subject. In other embodiments, the housing is configured to be attached to one or more of the following portions of a body of a

subject: arm, wrist, leg, hand, foot, finger, toe, chest, head, hair, nose, waist, trunk, shoulder, and neck. In other embodiments, the housing is configured to be embedded within clothing, foot apparel, and other wearable objects, without limitation.

Conventional methods and apparatus for studying the circadian cycle heretofore have not estimated resting state (or other) parameters of a being based on the current state of the being. There have been at least two major limitations preventing such an invention: 1) there has been no effort to estimate resting parameters based on what's already known about the relationships between resting state and current state and 2) there have been no apparatuses or methods for accurately and reliably measuring dynamically changing relationships between current and resting state parameters in everyday life activities.

It is noted that aspects of the invention described with respect to one embodiment may be incorporated in a different embodiment although not specifically described relative thereto. That is, all embodiments and/or features of any embodiment can be combined in any way and/or combination. Applicant reserves the right to change any originally filed claim or file any new claim accordingly, including the right to be able to amend any originally filed claim to depend from and/or incorporate any feature of any other claim although not originally claimed in that manner. These and other objects and/or aspects of the present invention are explained in detail below.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which form a part of the specification, illustrate various embodiments of the present invention. The drawings and description together serve to fully explain embodiments of the present invention.

FIG. 1 is a block diagram of methods and apparatus for estimating physiological parameters of a being at a selected state, according to some embodiments of the present invention.

FIG. 2 is an exemplary plot of how tympanic or core body temperature may change with time-of-day for an average person.

FIG. 3 is an exemplary plot of how heart rate may change with time-of-day for an average person, wherein curve C1 represents a normal cycle and wherein curve C2 represents an elevated cycle.

FIG. 4 is an exemplary plot of how heart rate variability (HRV) may change with time-of-day for an average person.

FIG. 5 is an exemplary plot of how heart rate of a person may change with the person's activity level.

FIG. 6 is a flow chart for an algorithm for estimating resting parameters, according to some embodiments of the present invention.

FIG. 7 is a plot of average body temperature vs. time calculated using a polynomial equation for body vs. time-of-day, according to some embodiments of the present invention.

FIG. 8 is a plot of heart rate vs. time for an average person, wherein curve (A) represents heart rate vs. time before a lifestyle change, wherein curve (B) represents heart rate vs. time after a lifestyle change, and wherein curve (A) and (B) are generated via respective polynomial equations according to some embodiments of the present invention.

FIG. 9 illustrates a functional relationship between an estimated parameter and multiple time-dependent inputs, according to some embodiments of the present invention.

FIG. 10 is an exemplary lookup table for estimating resting body temperature, according to some embodiments of the present invention.

FIG. 11 is a block diagram that illustrates details of an exemplary processor and memory that may be used in accordance with embodiments of the present invention.

DETAILED DESCRIPTION

The present invention will now be described more fully hereinafter with reference to the accompanying figures, in which embodiments of the invention are shown. This invention may, however, be embodied in many different forms and should not be construed as limited to the embodiments set forth herein. Like numbers refer to like elements throughout. In the figures, certain layers, components or features may be exaggerated for clarity, and broken lines illustrate optional features or operations unless specified otherwise. In addition, the sequence of operations (or steps) is not limited to the order presented in the figures and/or claims unless specifically indicated otherwise. Features described with respect to one figure or embodiment can be associated with another embodiment or figure although not specifically described or shown as such.

It will be understood that when a feature or element is referred to as being “on” another feature or element, it can be directly on the other feature or element or intervening features and/or elements may also be present. In contrast, when a feature or element is referred to as being “directly on” another feature or element, there are no intervening features or elements present. It will also be understood that, when a feature or element is referred to as being “connected”, “attached” or “coupled” to another feature or element, it can be directly connected, attached or coupled to the other feature or element or intervening features or elements may be present. In contrast, when a feature or element is referred to as being “directly connected”, “directly attached” or “directly coupled” to another feature or element, there are no intervening features or elements present. Although described or shown with respect to one embodiment, the features and elements so described or shown can apply to other embodiments. It will also be appreciated by those of skill in the art that references to a structure or feature that is disposed “adjacent” another feature may have portions that overlap or underlie the adjacent feature.

The terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. As used herein, the singular forms “a”, “an” and “the” are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms “comprises” and/or “comprising,” when used in this specification, specify the presence of stated features, steps, operations, elements, and/or components, but do not preclude the presence or addition of one or more other features, steps, operations, elements, components, and/or groups thereof. As used herein, the term “and/or” includes any and all combinations of one or more of the associated listed items.

Spatially relative terms, such as “under”, “below”, “lower”, “over”, “upper” and the like, may be used herein for ease of description to describe one element or feature’s relationship to another element(s) or feature(s) as illustrated in the figures. It will be understood that the spatially relative terms are intended to encompass different orientations of the device in use or operation in addition to the orientation depicted in the figures. For example, if a device in the figures is inverted, elements described as “under” or “beneath”

other elements or features would then be oriented “over” the other elements or features. Thus, the exemplary term “under” can encompass both an orientation of over and under. The device may be otherwise oriented (rotated 90 degrees or at other orientations) and the spatially relative descriptors used herein interpreted accordingly. Similarly, the terms “upwardly”, “downwardly”, “vertical”, “horizontal” and the like are used herein for the purpose of explanation only unless specifically indicated otherwise.

It will be understood that although the terms first and second are used herein to describe various features/elements, these features/elements should not be limited by these terms. These terms are only used to distinguish one feature/element from another feature/element. Thus, a first feature/element discussed below could be termed a second feature/element, and similarly, a second feature/element discussed below could be termed a first feature/element without departing from the teachings of the present invention.

Unless otherwise defined, all terms (including technical and scientific terms) used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. It will be further understood that terms, such as those defined in commonly used dictionaries, should be interpreted as having a meaning that is consistent with their meaning in the context of the specification and relevant art and should not be interpreted in an idealized or overly formal sense unless expressly so defined herein. Well-known functions or constructions may not be described in detail for brevity and/or clarity.

The term “housing”, as used herein, may refer to a physical structure for supporting and/or unifying one or more physical elements of the invention. For example, the housing of a wearable wrist sensor apparatus or headset sensor apparatus may comprise a structure to support the electronics, optics, and/or mechanical elements of the sensor. Two specific, non-limiting examples of a housing may be a “clamshell” of an earbud or one or more PCB boards for the sensor electronics. The structure may be composed of plastic, metal, polymer, ceramic, glass, composite material, or virtually any solid stable enough to support the physical elements of the apparatus.

The term “selected state”, as used herein, includes, but is not limited to, state of peak metabolism, state of lowered metabolism, state of rest, a state of one’s psychology or mental functioning or the body’s physiology or physiological functioning. Any example of mental functioning may include psychosocial stress, mental stress, mental acuity, brain activity, conscious state, state or phase of sleep, or the like. An example of physiological functioning may include the functioning of one or more organs individually or in unison. In addition, a selected state may refer to a particular time of day where a particular or noteworthy mental or physiological event may take place.

The term “heightened activity condition”, as used herein, includes, but is not limited to, elevated heart rate, elevated or lowered vital signs status, such as heart status (heart rate, ECG waveform intervals, cardiac output, cardiac stress or load, or the like), lung status (breathing rate, breathing volume, lung stress or load, or the like), blood pressure, blood oxygen level, heart rate variability, galvanic skin response, heat flux from the body, core body temperature, skin temperature, sympathetic or parasympathetic response, or the like.

The term “blood analyte” may refer to blood constituents, such as blood gases (blood oxygen, blood CO₂, blood

hemoglobin, and the like), blood glucose, blood cholesterol, blood lactic acid, blood bilirubin, dissolved species in the blood, and the like.

The term “headset” includes any type of device or ear-piece that may be attached to or near the ear (or ears) of a user and may have various configurations, without limitation. Headsets as described herein may include mono headsets (one earbud) and stereo headsets (two earbuds), earbuds, hearing aids, ear jewelry, face masks, headbands, and the like.

The term “real-time” is used to describe a process of sensing, processing, or transmitting information in a time frame which is equal to or shorter than the minimum timescale at which the information is needed. For example, the real-time monitoring of pulse rate may result in a single average pulse-rate measurement every minute, averaged over 30 seconds, because an instantaneous pulse rate is often useless to the end user. Typically, averaged physiological and environmental information is more relevant than instantaneous changes. Thus, in the context of embodiments of the present invention, signals may sometimes be processed over several seconds, or even minutes, in order to generate a “real-time” response.

The term “monitoring” refers to the act of measuring, quantifying, qualifying, estimating, sensing, calculating, interpolating, extrapolating, inferring, deducing, or any combination of these actions. More generally, “monitoring” refers to a way of getting information via one or more sensing elements. For example, “blood health monitoring” includes monitoring blood gas levels, blood hydration, and metabolite/electrolyte levels.

The term “physiological” refers to matter or energy of or from the body of a creature/subject (e.g., humans, animals, etc.). In embodiments of the present invention, the term “physiological” is intended to be used broadly, covering both physical and psychological matter and energy of or from the body of a creature. However, in some cases, the term “psychological” is called-out separately to emphasize aspects of physiology that are more closely tied to conscious or subconscious brain activity rather than the activity of other organs, tissues, or cells. Embodiments of the present invention are not limited to use by only humans.

The term “body” refers to the body of a subject (human or animal) who may wear a headset incorporating embodiments of the present invention.

The terms “being”, “creature”, “subject”, and “organism”, as used herein, are interchangeable and include, but are not limited to, humans and animals.

The terms “circadian rhythm” and “circadian cycle”, as used herein, are interchangeable and refer to an endogenously driven, roughly 24-hour cycle in biochemical, physiological, or behavioral processes.

The term “processor” refers to a device that takes one form of information and converts this information into another form, typically having more usefulness than the original form. For example, in this invention, a signal processor may collect raw physiological and environmental data from various sensors and process this data into a meaningful assessment, such as pulse rate, blood pressure, or air quality. A variety of microprocessors or other processors may be used herein. The terms “signal processor”, “processor”, “controller”, and “microcontroller”, as used herein, are interchangeable.

Embodiments of the present invention provide methods and apparatus for estimating time-state physiological parameters/assessments, such as resting parameters, of a subject by factoring functional relationships between the time-depen-

dent parameters and other measured factors. For example, current state parameters (such as vital signs, environmental exposures, time-of-day, and the like) are measured and a physiological model is applied to generate an estimation of resting state parameters (or other particular states) of the subject. These relationships can be static relationships based on models that apply knowledge of how a current state of the subject relates to a resting state of the subject. These relationships can also be dynamic relationships based on personalized monitoring of a subject throughout various life activities.

Average body temperature, heart rate, heart rate variability for a subject, as well as many other vital parameters, change throughout the day on a regular schedule dependent on the time-of-day, consistent with normal circadian rhythms. Additionally, average values of vital signs will change throughout the day based on changes in a subject’s physical activity or metabolic rate. As shown in FIGS. 2 and 7, average body temperature for a human subject may change by $\sim 2^\circ$ F. from early morning to mid-day. In FIG. 2, body temperature is plotted on the y-axis and time in hours is plotted on the x-axis. Curve 100 in FIG. 2 is a plot of average core body temperature vs. time for an average human over an average day. In FIG. 7, body temperature is plotted on the y-axis and time in hours is plotted on the x-axis. Polynomial equation 104 is used to calculate the plot 102.

Similarly, as shown in FIG. 3, average heart rate for a human subject may change by ~ 15 BPM (beats per minute) during that same period. FIG. 3 illustrates how heart rate may change with time-of-day for an average person, wherein curve C1 represents a normal cycle and wherein curve C2 represents an elevated cycle. In FIG. 3, heart rate is plotted on the y-axis and time in hours is plotted on the x-axis. Thus, if average body temperature and average heart rate are being monitored throughout the day, estimating resting body temperature and resting heart rate for a subject may be derived by applying the respective relationships to the existing measured state.

For example, if the current state at mid-day shows a body temperature of 99.6° F. and heart rate of 80 BPM, the resting state values may be estimated as 97.6° F. and 65 BPM, by subtracting 2° F. from body temperature and 15 BPM from heart rate, respectively. Percent (%) change relationships for estimating resting state, as opposed to absolute value changes, may also be used to estimate resting state. For example, the change from current state to resting state in the aforementioned case is $\sim 2\%$ and 18% for body temperature and resting heart rate, respectively. Thus, a lookup table (e.g., table 110, FIG. 10) may be generated with time-of-day in one column, measured value in a second column, and the associated percent multiplier in a third column, where the percent multiplier is the ratio between resting value and measured value. The estimation for resting value can then be generated by multiplying this time-of-day-dependent ratio by the measured vital parameter at the given time-of-day of the measurement.

A specific example for the case of body temperature is presented in FIG. 10, using the same relationships and data of FIG. 2, where a measurement of body temperature has been made at 6 PM, with a multiplier of ~ 0.981 , yielding a resting body temp estimate of 97.6° F. A complimentary lookup table may replace the % multiplier column with a $\pm$ add/subtract column, where the $\pm$ number is the amount to add or subtract from the measured value to generate an estimate of the resting value.

It should also be noted that a formula, rather than a lookup table, may also be used to relate resting estimates to measured estimates, depending on the time-of-day. For example, a polynomial formula representing the table of FIG. 10 may be: Estimated Resting Value=(Measured Value)*(-0.29x⁴+ 0.79x³-0.63x²+0.13x+1.0), where x=time in hours, starting at x=0 for 7 AM. It is apparent from this formula that at 7 AM (x=0), the Estimated Resting Value=Measured Value, which is expected in the aforementioned formalism.

FIG. 7 shows an exemplary plot 102 of average human body temperature during a day, along with an approximate functional relationship for average body temperature vs. time. In the illustrated embodiment, the functional relationship is a polynomial equation 104 of order n=4. The a₀ term is 97.6° F., representing the resting body temperature, or BT_{resting}=97.6° F. If a person's resting body temperature (BT_{resting}) had started higher or lower than 97.6° F., the polynomial equation may still hold, with the only substantial difference being the a₀ term for BT_{resting}. Thus, an equation for estimating BT_{resting} VS. BT_{measured} may be derived by rearranging terms such that a₀=BT_{resting}=BT_{measured}-[9E-05(t⁴)-0.0033(t³)+0.0161(t²)+0.2868(t)]. More generally, a₀=BT_{resting}=BT_{measured}-[a_n(tⁿ)+a_{n-1}(tⁿ⁻¹)+a_{n-2}(tⁿ⁻²)+ . . . a₁(t)], where "n" is the order of the polynomial equation and where t=0 represents the value of BT at the resting state. The second term in the brackets may be related to body temperature changes due to circadian rhythms, such that BT_{resting}=BT_{measured}-Δ BT_{circadian}. This same general relationship may be applied towards heart rate (HR) as shown in FIG. 3 and heart rate variability in FIG. 4. In FIG. 4, heart rate variability is plotted on the y-axis and time in hours is plotted on the x-axis. The units along the y-axis are milliseconds-squared. Plot 120 illustrates how heart rate variability (HRV) may change with time-of-day for an average person. For example, HR_{resting}=HR_{measured}-Δ HR_{circadian} and HRV_{resting}=HRV_{measured}-Δ HRV_{circadian}. This formalism may be applied towards blood oxygen (SPO₂), respiration rate (RR), blood pressure (BP), pulse pressure (PP), and other vital parameters (VP), that may change regularly throughout the day according to VP_{resting}=VP_{measured}-Δ VP_{circadian}.

In some embodiments of the present invention, the general relationships illustrated in FIGS. 2, 3, and 7 may not enable a prediction of resting state (or other selected state) as accurately as desired. For example, a person engaging in heightened activity or personal variations may cause substantial departures from the general relationships. Fortunately, these differences may effectively average out if vital signs measurements are made over a period of time. For example, if a vital sign of interest is measured over several days at the same time-of-day, during different activity levels, the average value of the vital sign may be largely divorced of convolutions caused by heightened or acute activity. This average value of VP_{measured} may then be used to estimate VP_{resting}. However, it may be difficult to measure the vital parameter at the same time-of-day for multiple days, and a one-time measurement of a vital parameter taken during or following high activity may not be sufficient to support an accurate estimate of the resting value, using the general relationships alone.

To correct for conditions of high activity, a general relationship between changes in activity and changes in vital parameters may be used to correct an estimate of resting parameters, according to some embodiments of the present invention. For example, during activity, the heart rate of a subject may increase in a predictable fashion, as shown in FIG. 5. In FIG. 5, heart rate is plotted on the left y-axis,

activity is plotted on the right y-axis, and time in hours is plotted on the x-axis. Curve A in FIG. 5 illustrates heart rate and activity for a person at a first state, and curve B in FIG. 5 illustrates heart rate and activity for the person at a heightened activity state.

Generally, as illustrated in FIG. 5, heart rate will increase with activity, and the rate of increase with activity may be proportional to the physical fitness or aerobic capacity (VO₂max) of the subject. Thus, if the relationship between heart rate and activity is known for a subject, then the differential increase in heart rate due to elevated activity, for a particular time-of-day, may be subtracted from the current heart rate measurement. Namely, the estimated resting heart rate can be defined as HR_{resting}=HR_{measured}-Δ HR_{circadian}-Δ HR_{activity}, where Δ HR_{activity} is the change in heart rate with activity (either positive/negative for increases/decreases in heart rate with activity). For other vital parameters, the term Δ VP_{activity} may be used instead.

Personal differences between individuals may cause deviations from the general, "universal" relationships previously described. For example, subjects having a higher metabolic rate change throughout a given day may have a larger total value or percent change in vital parameters between early morning and midday. Improving the accuracy of estimating resting parameters can be achieved by measuring vital parameters throughout the day, generating average time-dependent relationships based on these measured parameters, and deriving a personalized time-dependent relationship between measured and resting parameters. Once a personalized, functional, time-dependent relationship is generated between measured (current state) vital parameters and resting state vital parameters, this model may be used to estimate resting state parameters by inputting current state measurements into the model. For current state measurements taken at high activity, stored relationships between a subject's vital parameters and activity can be employed to subtract the change in vital parameter values with activity (Δ VP_{activity}) as with the heart rate example described above.

Environmental exposures (i.e., environmental conditions to which a subject is exposed) may also affect the time-dependent relationship between measured and resting parameters. For example, sunlight exposure may elevate metabolism, resulting in an increase in heart rate, breathing, rate, or other vital parameters, or the like. In such case, it may be insufficient to estimate resting parameters by simply measuring current resting parameters and inputting current parameters into the functional model. Rather, it may be more accurate to estimate resting vital parameters according to VP_{resting}=VP_{measured}-Δ VP_{circadian}-Δ VP_{environmental exposure} where Δ VP_{environmental exposure} is the change (positive or negative) in the vital parameter value due to environmental exposure (e.g., sunlight exposure, etc.). A change in vital parameters may be caused by many different forms of environmental exposures such as, but not limited to, loud noises, strong wind, extreme temperatures, short wavelength light (e.g., light at wavelengths <470 nm), airborne pollution, mechanical stress, and the like.

It should be noted that multiple parameters may simultaneously affect the relationship between resting values and measured values. For example, if physical activity and environmental exposure both have an impact on instantaneous vital parameters, then a more general relationship for resting vital parameters may be: VP_{resting}=VP_{measured}-Δ VP_{circadian}-Δ VP_{activity}-Δ VP_{environmental exposure}. Additional relationships, such as changes in a vital parameter with food intake (calories consumed), blood oxygen (SPO₂), and the like may also be incorporated. These additional relationships

can be accommodated by ΔVP_n , where the integer “n” represents an additional factor which may affect $VP_{measured}$.

The aforementioned models for estimating resting parameters have been presented as “static” models. A static model, once implemented or derived, stays fixed with time. However, models for determining a value of a physiological parameter for a subject at a selected state (e.g., at rest, etc.), according to some embodiments of the present invention, may also be dynamic, changing with time based on updated information about a particular person or group of people. For example, a person undergoing cardiac therapy, a new diet, drug therapy, or other lifestyle change may see an acute or chronic change in metabolism over time. In such case, static models may be insufficient for estimating resting parameters from current state measured parameters. Rather, it may be more accurate to measure vital parameters over a period of time and update the model based on updated relationships between resting and current state parameters.

FIG. 8 shows a specific example of a dynamic model for determining a value of a physiological parameter for a subject at a selected state (e.g., at rest, etc.) according to some embodiments of the present invention. FIG. 8 is a graph of heart rate vs. time-of-day for a twenty-four hour (24 hr) period. Curves A and B in FIG. 8 show the circadian change in average heart rate profile of an average person before and after a lifestyle change. Polynomial representations of these plots are also shown, with a polynomial order of $n=5$. Polynomial equation 130 is used to generate curve A in FIG. 8 and polynomial equation 140 is used to generate curve B in FIG. 8.

As illustrated in FIG. 8, after the lifestyle change, the average heart rate changes more dramatically as the time-of-day changes, as exemplified by the $2\times$ increase in the 5th-power coefficient in the “B” curve when compared with the “A” curve. The resting heart rate for each case is the a_0 terms of each, 60 and 45 BPM for curves A and B, respectively. Because the change in each model (for curves A and B) is not merely a scalar addition or subtraction, accurately estimating resting heart rate may require measuring average heart rate throughout the day, over the course of several days, modeling a relationship between resting and current state parameters, and then inputting current state parameters into the model. In one embodiment of the present invention, the model may be a polynomial equation fit to the measured data, as shown in FIG. 8. However, other models may be employed to improve accuracy or model simplicity, according to embodiments of the present invention.

FIG. 1 is a block diagram of methods and apparatus for generating estimated physiological parameters of a subject at a selected state based on current state measurements, according to some embodiments of the present invention. Time-correlated physiological metrics (Block 10) and/or time-correlated environmental metrics (Block 20) are collected and are input into a physiological model (static, dynamic, or a combination of both) (Block 30), and the desired parameters (such as resting state parameters) are estimated (Block 40) based on the metrics and physiological model. The estimated parameters are then reported in an organized fashion (Block 50).

An algorithm for estimating a resting parameter according to embodiments of the present invention is presented in the flow chart of FIG. 6. The algorithm includes measuring time-correlated heart rate (HR), respiration rate (RR), activity levels, etc., at a particular time of day (Block 150). A physical model is applied to estimate a parameter value that accounts for changes in the time-correlated parameter with

activity, environmental exposure, and/or daily cycle (Block 152). A resting assessment is then generated (Block 154).

FIG. 11 illustrates an exemplary processor 200 and memory 202 that may be used in a wearable device and/or a device remote from a subject to carry out various embodiments of the present invention. The processor 200 communicates with the memory 202 via an address/data bus 204. The processor 200 may be, for example, a commercially available or custom microprocessor or similar data processing device. The memory 202 is representative of the overall hierarchy of memory devices containing the software and data used to perform the various operations described herein. The memory 202 may include, but is not limited to, the following types of devices: cache, ROM, PROM, EPROM, EEPROM, flash, SRAM, and DRAM.

As shown in FIG. 11, the memory 202 may hold various categories of software and data: an operating system 206, a physiological data collection module 208, an environmental data collection module 210, and a time-dependent relationship function module 212. The operating system 206 controls operations of the physiological and environmental sensors.

It should be noted that estimating a physiological metric at a selected time state need not necessarily require a direct measurement of current time. For example, if the relationship between at least one physiological parameter and time is already known, or if that relationship is developed by recording data for a subject wearing a physiological sensor over time as shown in FIG. 11, then the current time may be inferred through this relationship and factored into an estimate for a second physiological metric at a selected time state. For example, if the relationship between the subject’s core body temperature over time is known (as shown in FIG. 2), then a subject’s HRV may be estimated for a selected time-state by estimating the current time based on the measured core body temperature at a current state. In such case, the current time need not be measured. However, in such case, because the current time is inferred and not directly noted or measured, it may be further beneficial to measure the subject’s activity and have this factored into the relationship function 212 (as discussed for FIG. 5) so as to prevent activity-based artifacts from causing inaccurate estimates of a second physiological metric at a selected state.

The physiological data collection module 208 comprises logic for obtaining from a physiological sensor a value of a physiological parameter of a subject at a particular time-of-day. The physiological data collection module 208 may also comprise logic for obtaining from a physiological sensor the value of a physiological parameter at the same time-of-day for multiple days, and logic for determining an average value for the multiple obtained values. The physiological data collection module 208 may also comprise logic for obtaining values of a physiological parameter of a subject at multiple times during at least one previous day.

The environmental data collection module 210 comprises logic for obtaining from an environmental sensor a value of an environmental parameter in a vicinity of a subject at a particular time-of-day.

The time-dependent relationship function module 212 comprises logic for applying a time-dependent relationship function to an obtained physiological parameter value to determine a value of the physiological parameter at a selected state, and logic for applying the time-dependent relationship function and an environmental-dependent relationship function to an obtained physiological parameter value (and average value) to determine a value of the physiological parameter at the selected state. In addition, the

time-dependent relationship function module **212** may comprise logic for determining if a subject is in a condition of heightened activity at a selected time-of-day by determining if at least one obtained physiological parameter value is at a level associated with heightened activity, and may comprise logic for adjusting the time-dependent relationship function for the heightened activity condition of the subject prior to determining a value of the physiological parameter at the selected state. The time-dependent relationship function module **212** may comprise logic for generating a personalized time-dependent relationship function between a measured value of a physiological value and a value of the physiological parameter at a selected state using obtained values from at least one previous day, and may comprise logic for applying the personalized time-dependent relationship function to a obtained physiological parameter value to determine a value of the physiological parameter at the selected state.

The time-dependent relationship function module **212** may also comprise logic for adjusting a time-dependent relationship function for calories consumed by a subject prior to determining a value of the physiological parameter at a selected state. The time-dependent relationship function module **212** may also comprise logic for adjusting a time-dependent relationship function for blood oxygen level of a subject prior to determining a value of the physiological parameter at a selected state.

According to some embodiments of the present invention, collecting measured time-dependent metrics may be manual or automatic. Records can be taken over time, recorded, and processed into time-dependent relationships by skilled professionals or personal recording. However, it may be easier to record this data with one or more wearable devices having multiple wearable sensors. For example, wired and wireless vital parameter modules may be located along several parts of the body, or integrated into a single device worn at a single place along the body. These wearable devices may measure vital parameters throughout the day and, with microprocessors or other processing devices, generate estimations for resting parameters. Memory devices, such as memory chips, data storage devices, and the like, may be used to store and update physiological models according to embodiments of the present invention, and at least one processor may be used to estimate parameters based on the metrics and model. At least one processor may also be used to organize the data into a string of outputs for each measured parameter. There is great flexibility in the electronics that may be used to implement embodiments of the present invention. Individual electronic components or chips may be used and integrated within circuit board, or the electronics may integrate memory storage, data processing, and data translation within a single chip, or other combinations or electronics configurations may be used.

Some types of wearable devices may be more suited for sensor integration than other devices. For example, an ear-worn device may be especially suited for measuring blood flow, heart rate, breathing rate, EEG, and body temperature, due in part to the location of the ear with respect to physiological structures such as the carotid artery, capillaries, ear blood vessels, the brain, and the tympanic membrane. However many other form-factors for a single wearable device may be employed. For example, strong blood flow and heat generation in the limbs, digits, and torso enable integrated sensor locations in the arms, wrist, legs, hands, feet, fingers, toes, chest, head, hair, nose, waist, trunk, shoulder, neck, and other locations. Furthermore, physiological and environmental sensors may be embedded in

clothing or other wearable devices, such as headsets, earbuds, wrist watches, adhesive patches, rings, bracelets, necklaces, footwear, socks, shirts, pants, underwear, earrings and other body piercings, hats, glasses, and the like.

The ear is an ideal location for wearable health and environmental monitors. The ear is a relatively immobile platform that does not obstruct a person's movement or vision. Headsets located at an ear have, for example, access to the inner-ear canal and tympanic membrane (for measuring core body temperature), muscle tissue (for monitoring muscle tension), the pinna and earlobe (for monitoring blood gas levels), the region behind the ear (for measuring skin temperature and galvanic skin response), and the internal carotid artery (for measuring cardiopulmonary functioning), etc. The ear is also at or near the point of exposure to: environmental breathable toxicants of interest (volatile organic compounds, pollution, etc.); noise pollution experienced by the ear; and lighting conditions for the eye. Furthermore, as the ear canal is naturally designed for transmitting acoustical energy, the ear provides a good location for monitoring internal sounds, such as heartbeat, breathing rate, and mouth motion.

Wireless, Bluetooth®-enabled, and/or other personal communication headsets may be configured to incorporate physiological and/or environmental sensors, according to some embodiments of the present invention. As a specific example, Bluetooth® headsets are typically lightweight, unobtrusive devices that have become widely accepted socially. Moreover, Bluetooth® headsets are cost effective, easy to use, and are often worn by users for most of their waking hours while attending or waiting for cell phone calls. Bluetooth® headsets configured according to embodiments of the present invention are advantageous because they provide a function for the user beyond health monitoring, such as personal communication and multimedia applications, thereby encouraging user compliance. Exemplary physiological and environmental sensors that may be incorporated into a Bluetooth® or other type of headsets include, but are not limited to accelerometers, auscultatory sensors, pressure sensors, humidity sensors, color sensors, light intensity sensors, pressure sensors, etc.

Optical coupling into the blood vessels of the ear may vary between individuals. As used herein, the term "coupling" refers to the interaction or communication between excitation light entering a region and the region itself. For example, one form of optical coupling may be the interaction between excitation light generated from within a light-guiding earbud and the blood vessels of the ear. Light guiding earbuds are described in co-pending U.S. Patent Application Publication No. 2010/0217102, which is incorporated herein by reference in its entirety. In one embodiment, this interaction may involve excitation light entering the ear region and scattering from a blood vessel in the ear such that the intensity of scattered light is proportional to blood flow within the blood vessel. Another form of optical coupling may be the interaction between excitation light generated by an optical emitter within an earbud and the light-guiding region of the earbud.

Embodiments of the present invention are not limited to headsets and devices that communicate wirelessly. In some embodiments of the present invention, headsets and devices configured to monitor an individual's physiology and/or environment may be wired to a device that stores and/or processes data. In some embodiments, this information may be stored on the headset itself.

Embodiments of the present invention may apply to the estimation of parameters at another state (other than resting

state) by measuring current state parameters and processing this data via a model to generate an estimate of parameters at the desired state. For example, embodiments of the present invention may be applied to estimating vital parameters at the state of peak metabolism during midday. In another example, embodiments of the present invention may be applied to estimating vital parameters at the state of lowered metabolism associated with evening time, for example, just before bedtime. A more general model or equation 160 for estimating vital parameters at a desired state is presented in FIG. 9.

It should also be understood that user input may be used to improve the accuracy of resting state (or other state) parameters. For example, relationships may exist between resting vs. measured parameters and weight, gender, height, habitual information, and the like. A particular example of habitual information may be the time-of-day someone wakes up in the morning. For example, the time of waking up may replace "7 AM" shown in FIG. 2.

Methods for estimating a physiological parameter at a selected state, according to some embodiments of the present invention, may be applied to wearable sensors as well as nonwearable sensors capable of measuring one or more physiological parameters and physical activity in a time-correlated manner, during enough times of the day to build or execute a time-correlated model. For example, whereas multiple examples of wearable devices have been described herein, alternative embodiments may employ wall-mounted sensors, bed-mounted sensors, car-mounted sensors, portable sensors, or other sensor configurations that can measure physiological parameters or physical activity at a "stand-off" distance from a subject. As a specific example, a wall-mounted camera may be configured to measure the heart rate, breathing rate, and physical activity of a subject and to record a time stamp of that subject. Measuring heart rate or breathing rate with a mounted camera may be achieved via algorithms capable of assessing individual video frames for changes in the chest size in time or by detecting certain wavelengths of light associated with heat changes, for example. Additionally, physical activity may be assessed by algorithms capable of identifying subjects and subject motion and translating this identified motion to activity level. In such case, a time-correlated relationship function may be generated for the subject. Thus, the heart rate or respiration rate of the subject may be accurately estimated for a selected state, such as a resting state or other state, when the subject is not in view of the camera by applying the time-correlated relationship function for the subject at the selected state. Suitable stand-off detection methods may employ, for example, electromagnetic, electrical, magnetic, inductive, capacitive, thermal, acoustic, or other energy detection techniques. For example, the heart rate, breathing rate, and activity of a subject sleeping in a bed, and coupled to a stand-off capacitive or inductive sensor, may be monitored through changes in capacitance or inductance. If this data is time-stamped by a processor, the inventive aspects described herein may be applied for determining one or more physiological parameters for that subject at a selected state, such as a state of reduced or elevated activity.

The foregoing is illustrative of the present invention and is not to be construed as limiting thereof. Although a few exemplary embodiments of this invention have been described, those skilled in the art will readily appreciate that many modifications are possible in the exemplary embodiments without materially departing from the teachings and advantages of this invention. Accordingly, all such modifi-

cations are intended to be included within the scope of this invention as defined in the claims. The invention is defined by the following claims, with equivalents of the claims to be included therein.

That which is claimed is:

1. A method of estimating a value of a physiological parameter for a subject at a selected metabolic state, the method comprising:

obtaining, via a non-wearable device located at a stand-off distance from the subject, a value of the physiological parameter of the subject at a time-of-day, wherein the non-wearable device comprises a sensor configured to measure heart rate, breathing rate, and/or physical activity of the subject, wherein the sensor is an electromagnetic energy sensor, an electrical energy sensor, a magnetic energy sensor, an inductive energy sensor, a capacitive energy sensor, a thermal energy sensor, or an acoustic energy sensor; and

estimating the value of the physiological parameter for the subject at the selected metabolic state by applying a time-dependent relationship function to the obtained physiological parameter value via at least one processor, wherein the selected metabolic state is different from a current metabolic state of the subject.

2. The method of claim 1, wherein the time-dependent relationship function is derived, from a circadian rhythm for the subject.

3. The method of claim 1, wherein the time-dependent relationship function is a lookup table.

4. The method of claim 1, wherein the physiological parameter includes one or more of the following: subject body temperature, subject heart rate, subject heart rate variability, subject blood gas levels, subject metabolic rate, subject respiration rate, subject blood analyte levels, subject blood pressure, and subject pulse pressure.

5. The method of claim 1, wherein estimating the value of the physiological parameter for the subject at the selected metabolic state comprises obtaining the value of the physiological parameter at the same time-of-day for multiple days and determining an average value for the multiple obtained values, and wherein applying the time-dependent relationship function to the obtained physiological parameter value comprises applying the time-dependent relationship function to the average value.

6. The method of claim 1, further comprising determining if the subject is in a condition of heightened activity at the time-of-day by determining via the non-wearable device if at least one obtained physiological parameter value is at a level associated with heightened activity, and wherein the time-dependent relationship function is adjusted for the heightened activity condition of the subject prior to estimating the value of the physiological parameter at the selected metabolic state.

7. The method of claim 1, wherein prior to obtaining a value of the physiological parameter of the subject at the time-of-day, values of the physiological parameter of the subject are obtained at multiple times during at least one previous day, and a personalized time-dependent relationship function between at least one of value of the physiological parameter and a value of the physiological parameter at the selected metabolic state is generated for the subject using the obtained values from the at least one previous day, and wherein applying the time-dependent relationship function to the obtained physiological parameter value comprises applying the personalized time-dependent relationship function to the obtained physiological

parameter value via the at least one processor to estimate the value of the physiological parameter at the selected metabolic state.

8. The method of claim 1, wherein the non-wearable device further includes an environmental sensor that detects and/or measures environmental condition information in a vicinity of the subject, and further comprising obtaining, via the non-wearable device, a value of an environmental parameter in a vicinity of the subject at the time-of-day, and wherein applying the time-dependent relationship function to the obtained physiological parameter value comprises applying the time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value via the at least one processor to estimate the value of the physiological parameter at the selected metabolic state.

9. The method of claim 1, further comprising adjusting the time-dependent relationship function for one or more of the following prior to estimating the value of the physiological parameter at the selected metabolic state: calories consumed by the subject and blood oxygen level of the subject.

10. The method of claim 1, wherein the selected metabolic state includes one or more of the following: state of peak metabolism, state of lowered metabolism, state of rest.

11. The method of claim 1, wherein the non-wearable device is a wall-mounted device, a bed-mounted device, a vehicle-mounted device, or a portable device.

12. The method of claim 1, wherein the non-wearable device is configured to identify subject motion and to translate identified subject motion to subject activity level.

13. A system, comprising:

a non-wearable sensor configured to measure heart rate, breathing rate, and/or physical activity of a subject located at a stand-off distance from the non-wearable sensor, wherein the non-wearable sensor is an electromagnetic energy sensor, an electrical energy sensor, a magnetic energy sensor, an inductive energy sensor, a capacitive energy sensor, a thermal energy sensor, or an acoustic energy sensor; and

at least one processor configured to obtain from the non-wearable sensor a value of a physiological parameter of the subject at a time-of-day, and to estimate a value of the physiological parameter for the subject at a selected metabolic state by applying a time-dependent relationship function to the obtained physiological parameter value, wherein the selected metabolic state is different from a current metabolic state of the subject.

14. The system of claim 13, wherein the at least one processor is configured to:

obtain from the non-wearable sensor the value of the physiological parameter at the same time-of-day for multiple days;

determine an average value for the multiple obtained values; and

apply the time-dependent, relationship function to the average value.

15. The system of claim 13, wherein the at least one processor is configured to:

determine if the subject is in a condition of heightened activity at the selected time-of-day by determining if a heart rate of the subject is at an elevated level; and adjust the time-dependent relationship function for the elevated heart rate level of the subject prior to estimating the value of the physiological parameter at the selected metabolic state.

16. The system of claim 13, wherein the at least one processor is configured to:

obtain values of the physiological parameter of the subject at multiple times during at least one previous day; generate a personalized time-dependent relationship function between a measured value of the physiological value and the estimated value of the physiological parameter at the selected metabolic state using the obtained values from the at least one previous day; and estimate the value of the physiological parameter for the subject at the selected metabolic state by applying the personalized time-dependent relationship function to the obtained physiological parameter value.

17. The system of claim 13, further comprising a non-wearable environmental sensor that detects and/or measures environmental condition information in a vicinity of the subject, and wherein the at least one processor is configured to obtain a value of an environmental parameter in a vicinity of the subject at the time-of-day from the non-wearable environmental sensor, and to apply the time-dependent relationship function and an environmental-dependent relationship function to the obtained physiological parameter value to estimate the value of the physiological parameter at the selected metabolic state.

18. The system of claim 13, wherein the at least one processor is configured to adjust the time-dependent relationship function for one or more of the following prior to estimating the value of the physiological parameter at the selected metabolic state: calories consumed by the subject and blood oxygen level of the subject.

19. The system of claim 13, wherein the at least one processor is configured to adjust the time-dependent relationship function for blood oxygen level of the subject prior to estimating the value of the physiological parameter at the selected metabolic state.

20. The system of claim 13, wherein the non-wearable sensor is configured to be wall-mounted, bed-mounted, vehicle-mounted, or portable.

21. The system of claim 13, wherein the non-wearable sensor is configured to identify subject motion and to translate identified subject motion to subject activity level.

* * * * *

专利名称(译)	用于估计时间 - 状态生理参数的装置和方法		
公开(公告)号	US9788785	公开(公告)日	2017-10-17
申请号	US15/369629	申请日	2016-12-05
[标]申请(专利权)人(译)	瓦倫賽爾公司		
申请(专利权)人(译)	VALENCELL INC.		
当前申请(专利权)人(译)	VALENCELL INC.		
[标]发明人	LEBOEUF STEVEN FRANCIS		
发明人	LEBOEUF, STEVEN FRANCIS		
IPC分类号	A61B5/04 A61B5/11 A61B5/1455 A61B5/08 A61B5/0205 A61B5/00 A61B5/145 A61B5/021 A61B5/024 G16H10/60		
CPC分类号	A61B5/4857 A61B5/0077 A61B5/02055 A61B5/02438 A61B5/0816 A61B5/1118 A61B5/14546 A61B5/14551 A61B5/4866 A61B5/6889 A61B5/6891 A61B5/6892 A61B5/6893 A61B5/021 A61B5/02405 A61B5/14542 A61B2560/0242 A61B2562/0204 A61B2562/0271		
优先权	14/116641 2016-08-30 US PCT/US2012/046446 2012-07-12 WO 61/511238 2011-07-25 US		
其他公开文献	US20170079582A1		
外部链接	Espacenet USPTO		

摘要(译)

确定处于选定状态的受试者的生理参数的值的方法包括经由位于距受试者的距离的装置获得在特定时间的受试者的生理参数的值，并且应用通过处理器对所获得的生理参数值进行时间依赖关系函数，以确定所选状态下的生理参数的值。

