



US 20150088007A1

(19) **United States**(12) **Patent Application Publication**
Bardy et al.(10) **Pub. No.: US 2015/0088007 A1**(43) **Pub. Date: Mar. 26, 2015**(54) **COMPUTER-IMPLEMENTED SYSTEM AND METHOD FOR PROVIDING A PERSONAL MOBILE DEVICE-TRIGGERED MEDICAL INTERVENTION**(52) **U.S. CL.**CPC *A61B 5/0022* (2013.01); *A61B 5/0205* (2013.01)USPC **600/484**; 600/483(71) Applicant: **Bardy Diagnostics, Inc.**, Vashon, WA (US)(72) Inventors: **Gust H. Bardy**, Carnation, WA (US);
Jason Felix, Vashon Island, WA (US);
Jon Mikalson Bishay, Seattle, WA (US)(21) Appl. No.: **14/217,402**(22) Filed: **Mar. 17, 2014****Related U.S. Application Data**

(63) Continuation-in-part of application No. 14/082,071, filed on Nov. 15, 2013, which is a continuation-in-part of application No. 14/080,717, filed on Nov. 14, 2013, which is a continuation-in-part of application No. 14/080,725, filed on Nov. 14, 2013.

(60) Provisional application No. 61/882,403, filed on Sep. 25, 2013.

Publication Classification(51) **Int. Cl.***A61B 5/00* (2006.01)*A61B 5/0205* (2006.01)(57) **ABSTRACT**

Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally on the patient's chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum) benefits extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. The wearable monitor can interoperate wirelessly with other physiology and activity sensors and mobile devices. An application executed by the sensor or device can trigger the dispatch of a wearable monitor to the patient upon detecting potentially medically-significant events. The dispatched wearable monitor would then be capable of providing precise medically-actionable data, not merely an alert that some abnormality may be present. The patient can then use the sensor or device to physically record the placement and use of the medically-actionable wearable monitor, thereby facilitating the authentication of the data recorded.

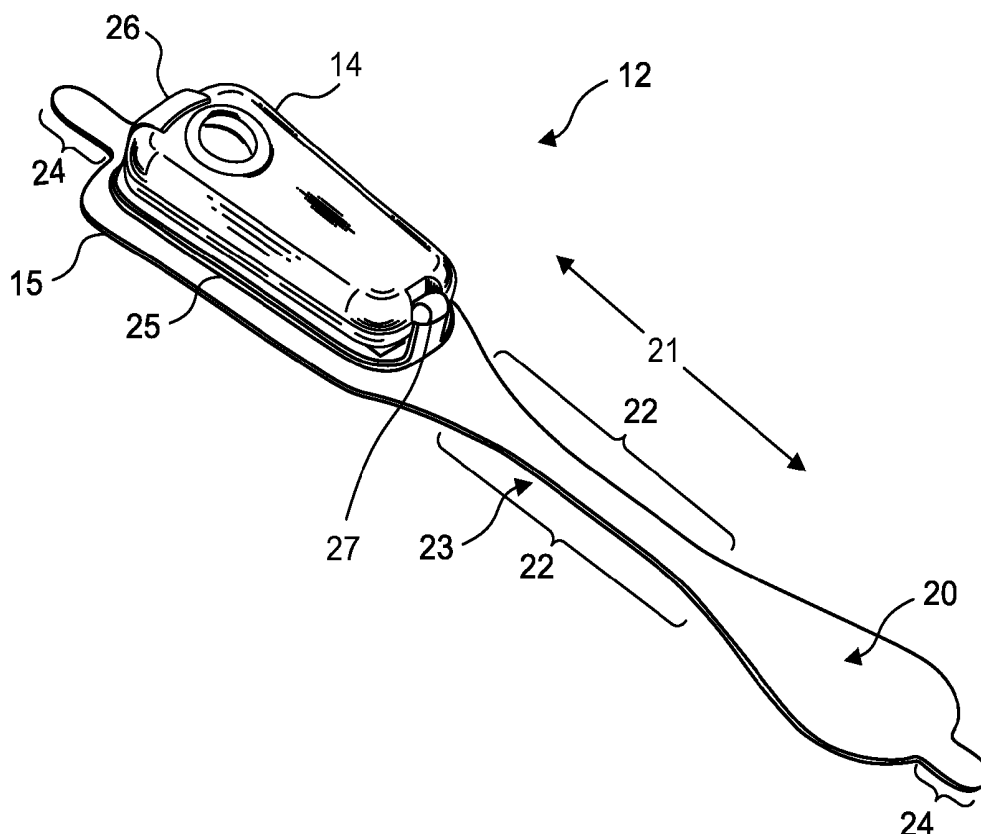


Fig. 1.

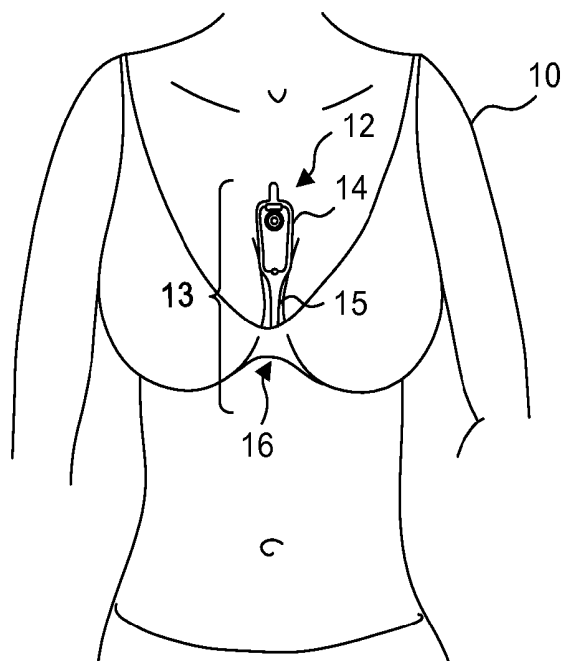


Fig. 2.

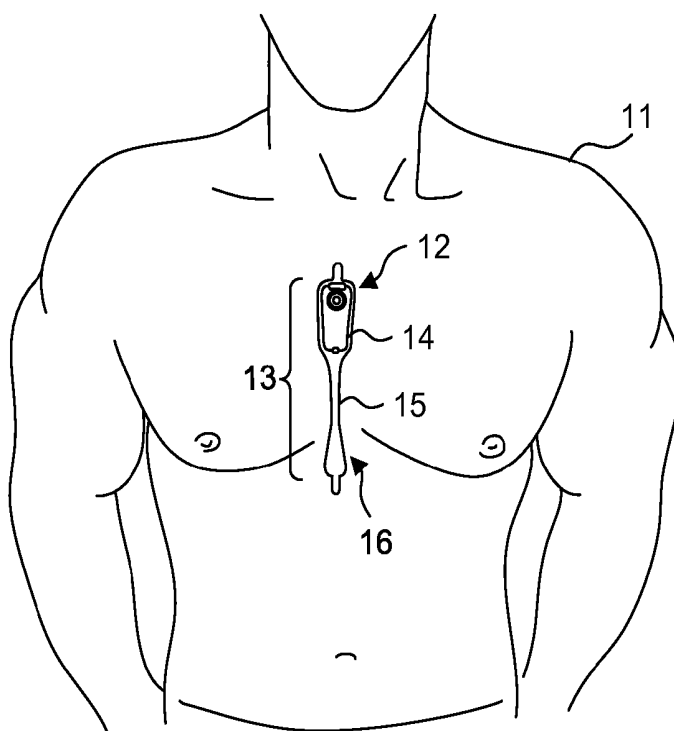


Fig. 3.

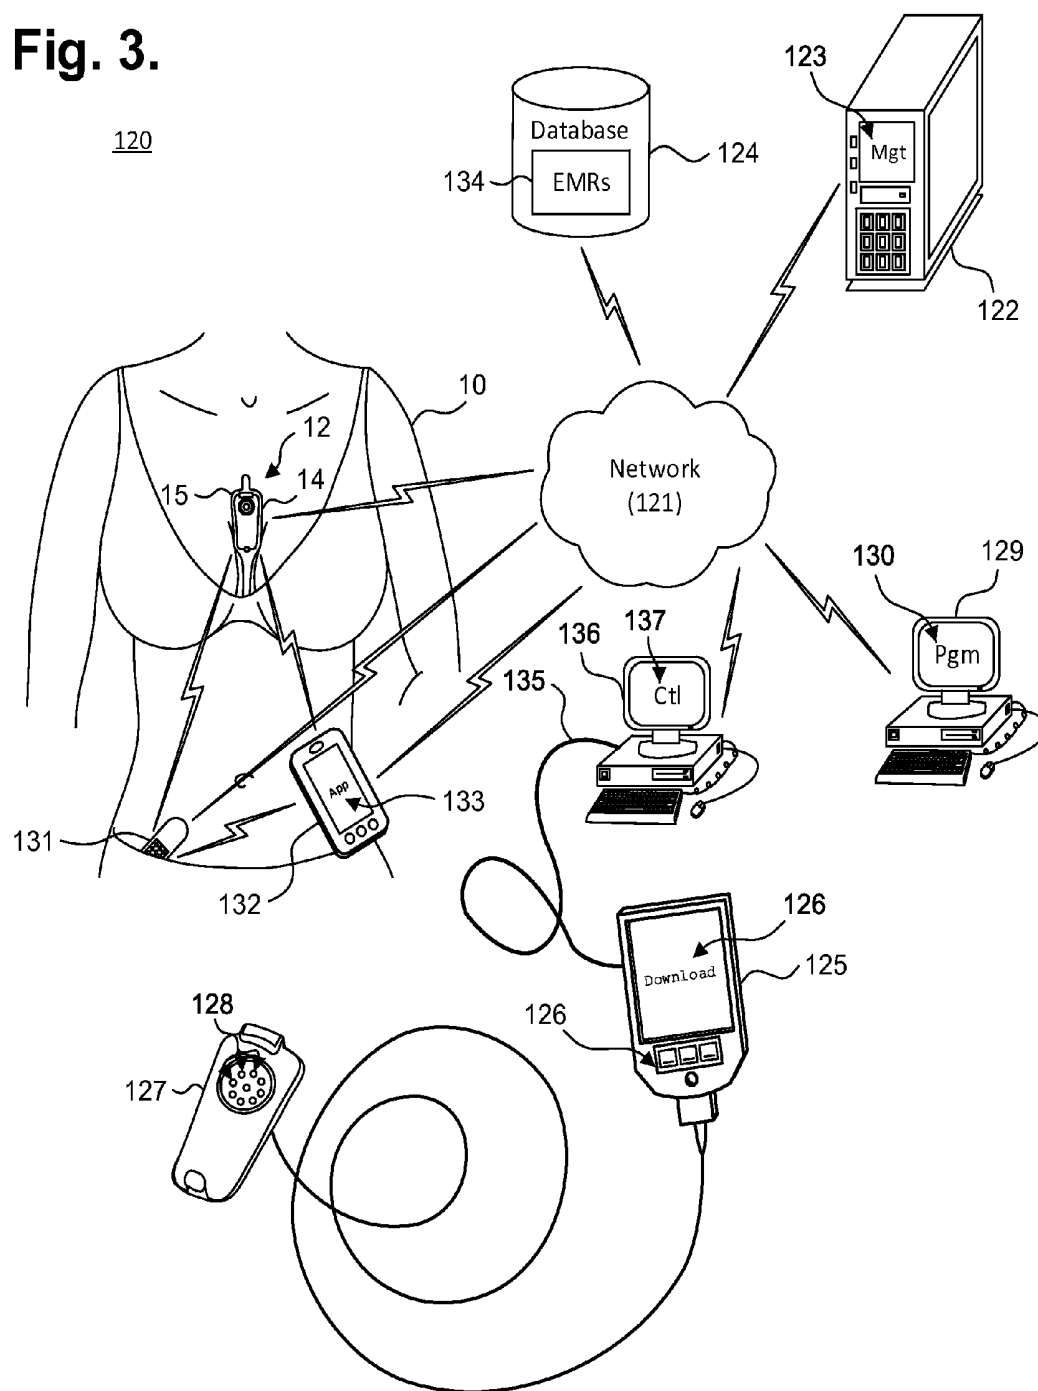


Fig. 4.

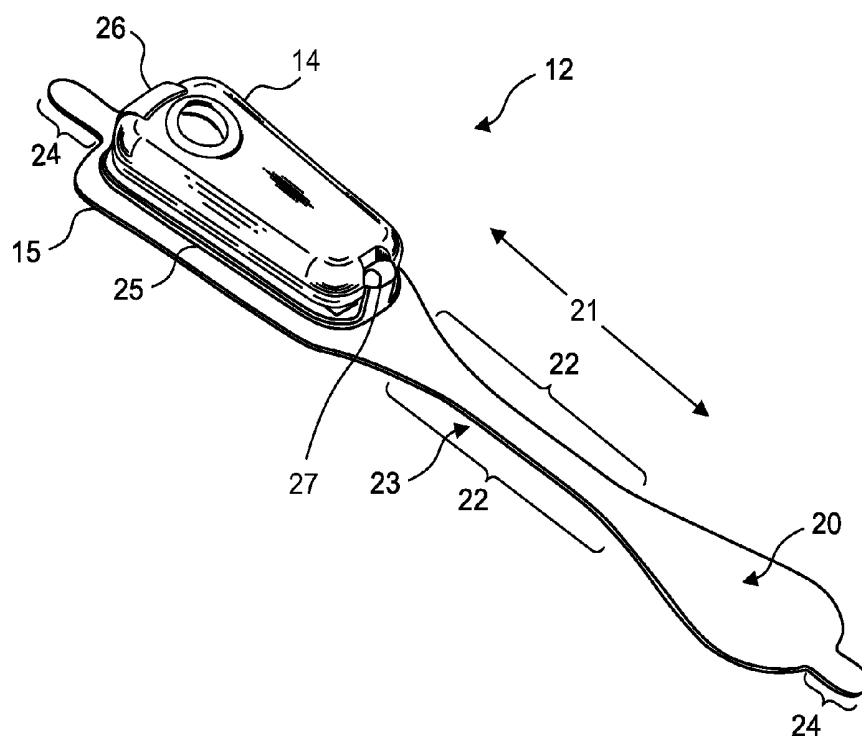


Fig. 5.

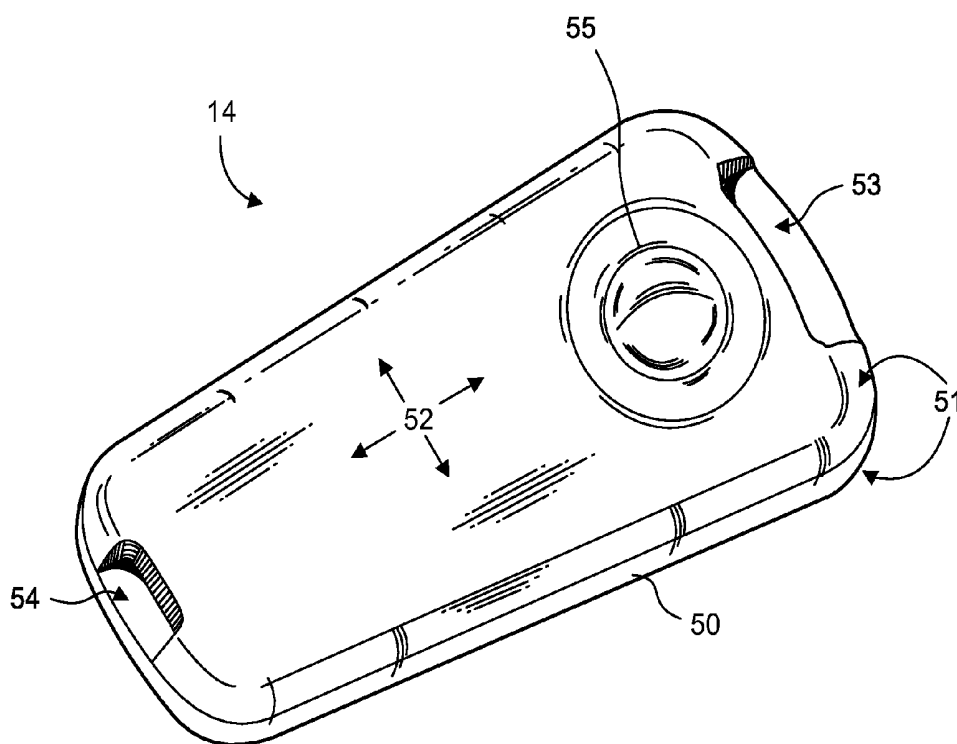


Fig. 6.

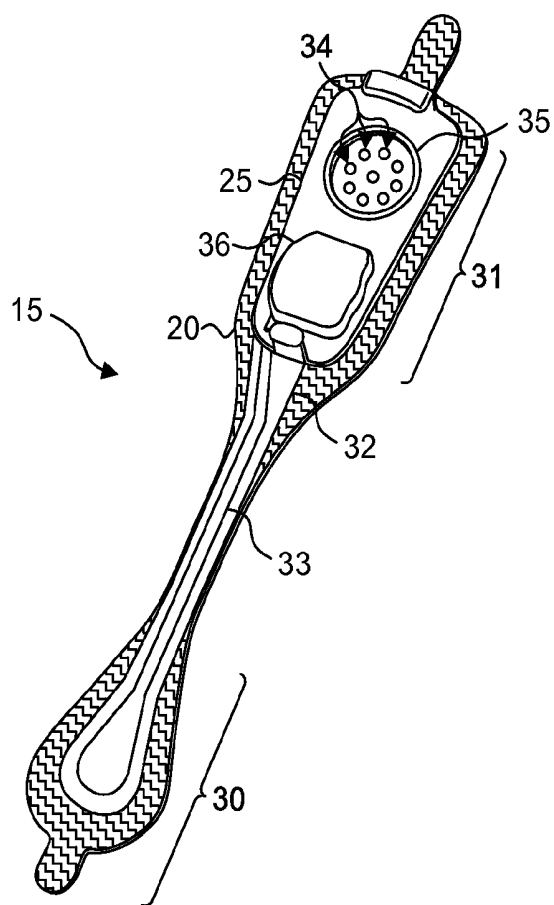


Fig. 7.

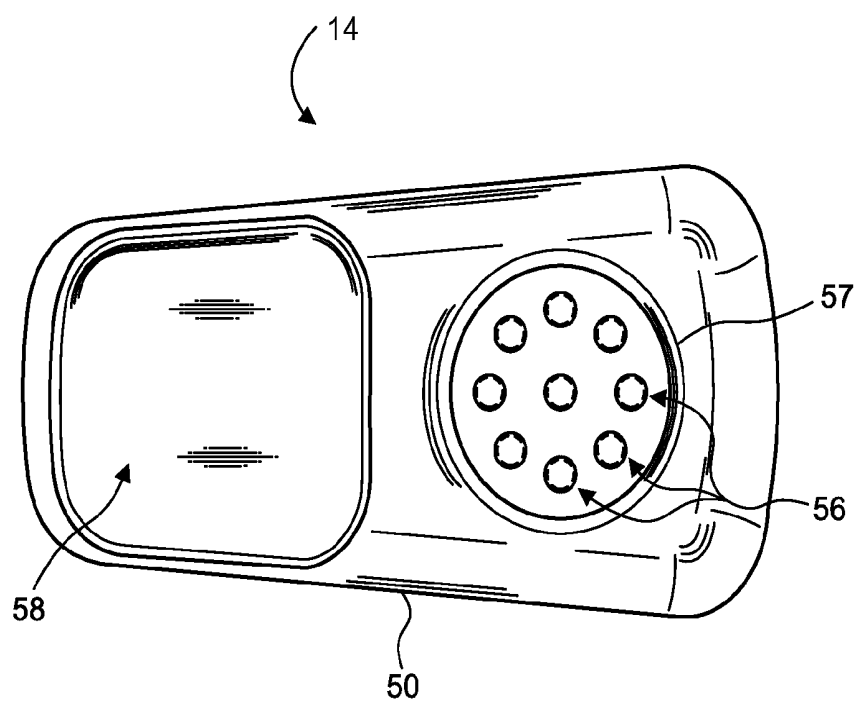


Fig. 8.

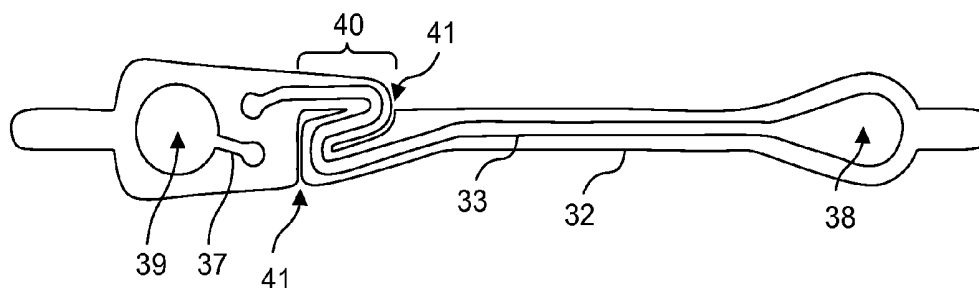


Fig. 9.

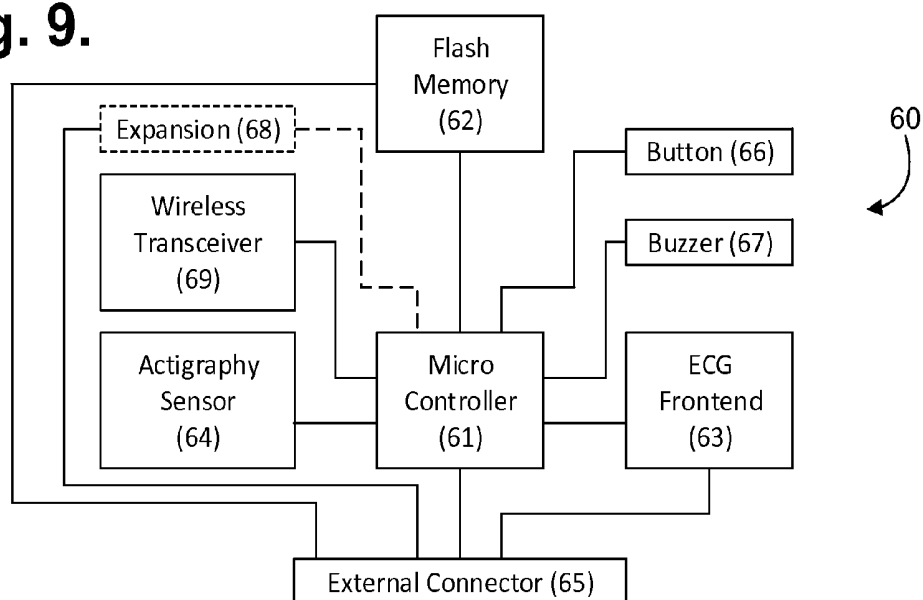


Fig. 10.

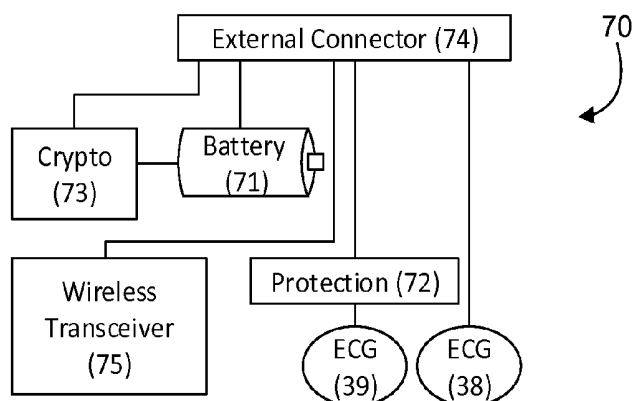


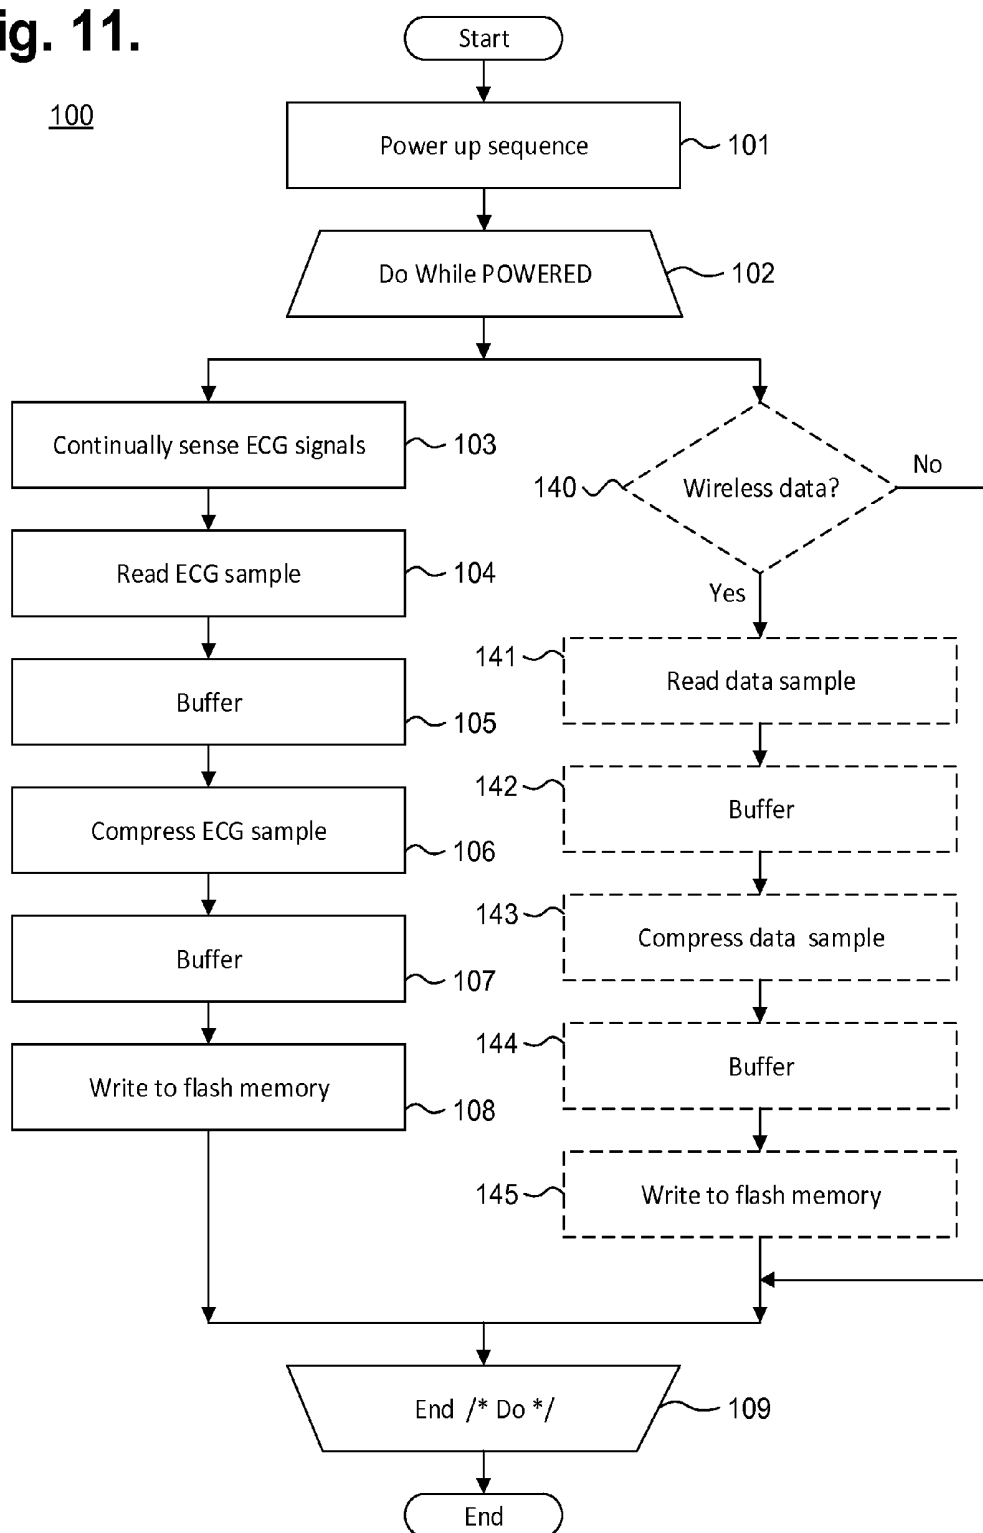
Fig. 11.

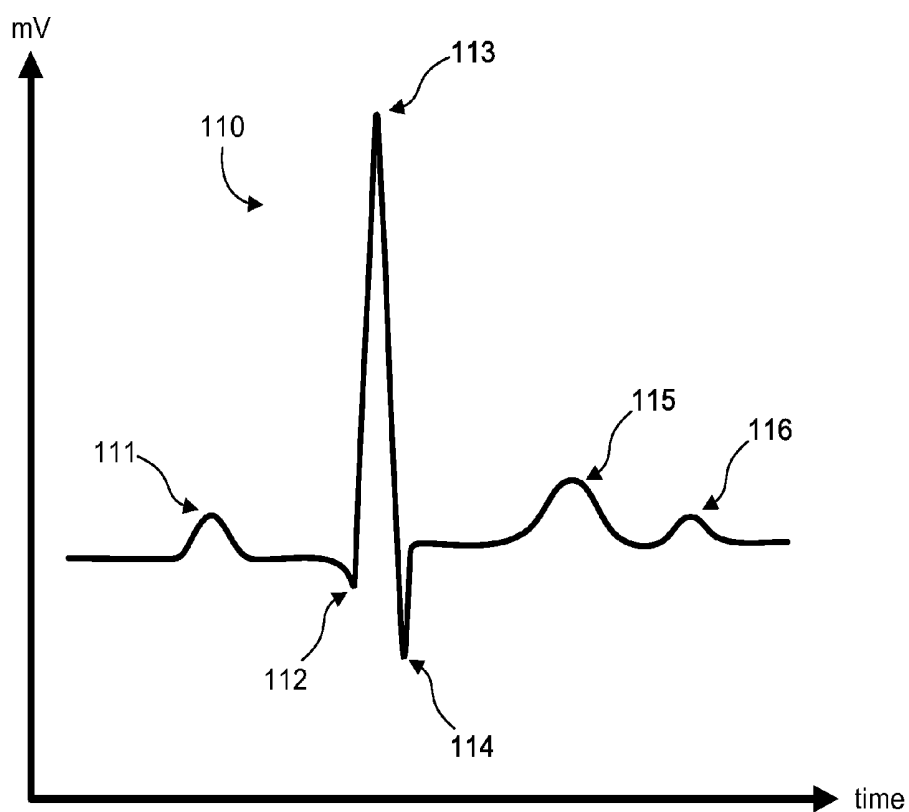
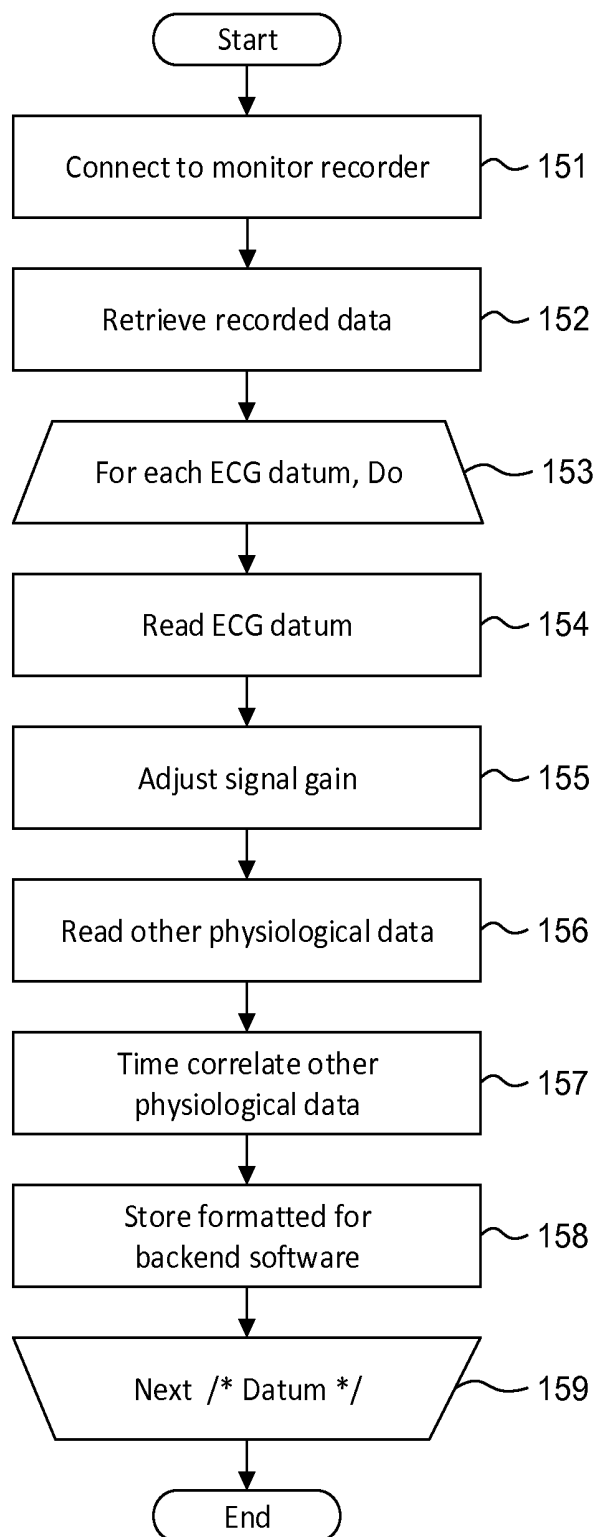
Fig. 12.

Fig. 13.150

**COMPUTER-IMPLEMENTED SYSTEM AND
METHOD FOR PROVIDING A PERSONAL
MOBILE DEVICE-TRIGGERED MEDICAL
INTERVENTION**

**CROSS-REFERENCE TO RELATED
APPLICATION**

[0001] This non-provisional patent application is a continuation-in-part of U.S. patent application Ser. No. 14/082,071, filed Nov. 15, 2013, pending; which is a continuation-in-part of U.S. patent application Ser. No. 14/080,717, filed Nov. 14, 2013, pending, and a continuation-in-part of U.S. patent application Ser. No. 14/080,725, filed Nov. 14, 2013, pending; and which further claims priority under 35 U.S.C. §119 (e) to U.S. Provisional Patent application, Ser. No. 61/882,403, filed Sep. 25, 2013, the disclosures of which are incorporated by reference.

FIELD

[0002] This application relates in general to electrocardiographic monitoring and, in particular, to a computer-implemented system and method for providing a personal mobile device-triggered medical intervention.

BACKGROUND

[0003] An electrocardiogram (ECG) records electrical potentials in the heart using a standardized set format 12-lead configuration to record cardiac electrical signals from well-established chest locations. Electrodes are placed on the skin over the anterior thoracic region of the body to the lower right and to the lower left of the sternum, on the left anterior chest, and on the limbs. The recorded cardiac electrical activity, represented by PQRSTU waveforms, can be interpreted to derive heart rate and physiology, where each P-wave represents atrial electrical activity and the QRS components represent ventricular electrical activity.

[0004] An ECG is a snapshot of heart function, typically recorded over 12 seconds, that can help diagnose rate and regularity of heartbeats, effect of drugs or implantable cardiac devices, and whether a patient has heart disease. ECGs are limited to recording those heart-related aspects present at the time of recording. Thus, an ECG only provides a partial picture and can be insufficient for complete patient diagnosis of many cardiac disorders. Sporadic conditions that may not show up during a spot ECG recording, including fainting or syncope; rhythm disorders, such as tachyarrhythmias and bradyarrhythmias; asystolic episodes; and other cardiac and related disorders, require other means of diagnosis.

[0005] Diagnostic efficacy of cardiac rhythm disorders in particular can be improved, when appropriate, through long-term extended ECG monitoring. Recording cardiac physiology over an extended period can be challenging, yet is often essential to enabling a physician to identify events of potential concern. Although a 30-day observation period is considered the “gold standard” of ECG monitoring, achieving 30-day coverage has proven unworkable because conventional ambulatory ECG monitoring systems are arduous to employ, cumbersome to wear, and excessively costly. Nevertheless, if a patient’s ECG could be recorded in an ambulatory setting over long periods of time, thereby allowing the patient to engage in activities of daily living, the chances of acquiring meaningful information and capturing an abnormal cardiac rhythm event becomes more likely to be achieved.

[0006] For instance, the long-term wear of ECG electrodes is complicated by skin irritation and the inability of conventional ECG electrodes to maintain continual skin contact after a day or two. Moreover, time, dirt, moisture, and other environmental contaminants, as well as perspiration, skin oil, and dead skin cells from the patient’s body, can get between an ECG electrode, the non-conductive adhesive used to adhere the ECG electrode, and the skin’s surface. These factors adversely affect electrode adhesion and the quality of cardiac signal recordings. Moreover, physical movement and clothing impart compressional, tensile, and torsional forces on electrode contact points decreasing signal quality, especially over long recording times. In addition, an inflexibly fastened ECG electrode is prone to dislodgement that often occurs unbeknownst to the patient, making the ECG recordings worthless. Further, some patients may have skin conditions, such as itching and irritation, aggravated by the wearing of most ECG electrodes. A patient may have to periodically remove or replace electrodes during a long-term monitoring period, whether to replace a dislodged electrode, reestablish better adhesion, alleviate itching or irritation, allow for cleansing of the skin, allow for showering and exercise, or for other purpose. Such replacement or slight alteration in electrode location can interfere with the goal of recording the ECG signal for long periods of time. Finally, such recording devices are often ineffective at recording atrial electrical activity, which is critical in the accurate diagnosis of heart rhythm disorders, because of the use of traditional ECG recording electronics or due to the location of the monitoring electrodes far from the origin of the atrial signal, for instance, the P-wave.

[0007] Conventionally, Holter monitors are widely used for long-term extended ECG monitoring, typically, for only 24-48 hours. A typical Holter monitor is a wearable and portable version of an ECG that includes cables for each electrode placed on the skin and a separate battery-powered ECG recorder. Similar to standard in-clinic ECG practice, the cable and electrode combination (or leads) are placed in the anterior thoracic region. The duration of a Holter monitoring recording depends on the sensing and storage capabilities of the monitor, as well as battery life. A “looping” Holter (or event) monitor can operate for a longer period of time by overwriting older ECG tracings, thence “recycling” storage in favor of extended operation, yet at the risk of losing crucial event data. Holter monitors remain cumbersome, expensive and typically for prescriptive use only, which limits their usability. Further, the skill required to properly place the ECG leads on the patient’s chest hinders or precludes a patient from replacing or removing the electrodes.

[0008] The ZIO XT Patch and ZIO Event Card devices, manufactured by iRhythm Tech., Inc., San Francisco, Calif., are wearable stick-on monitoring devices that are typically worn on the upper left pectoral region to respectively provide continuous and looping ECG recordings. The location is used to simulate surgically implanted monitors. These devices are prescription-only for single patient use. The ZIO XT Patch device is limited to 14-day monitoring, while the ZIO Event Card device’s electrodes can be worn for up to 30 days. The ZIO XT Patch device combines electronic recordation components, including battery, and physical electrodes into a unitary assembly that adheres to the skin. The ZIO XT Patch device uses adhesive strong enough to support the weight of both the monitor and the electrodes over an extended period of time. During monitoring, the battery is continually

depleted and can potentially limit overall monitoring duration. The ZIO Event Card device is a form of downsized Holter monitor with a recorder component that must be removed during activities that could damage the non-water-proof electronics. These patches have a further limitation because of a small inter-electrode distance coupled to its designed location of application, high on the left chest. The electrical design of the ZIO patch and its location make recording high quality atrial signals (P-waves) difficult, as the location is relatively far from the origin of these low amplitude signals. As well, the location is suboptimal for identification of these signals. Furthermore, this patch is problematical for woman by being placed in a location that may limit signal quality, especially in woman with large breasts or bosoms. Both ZIO devices represent compromises between length of wear and quality of ECG monitoring, especially with respect to ease of long term use, female-friendly fit, and quality of atrial (P-wave) signals.

[0009] Personal ambulatory monitoring, both with smartphones or via adjuncts to smartphones, such as with a wirelessly-connected monitor or activity tracker, of varying degrees of sophistication and interoperability, have become increasingly available. For instance, McManus et al., “A Novel Application for the Detection of an Irregular Pulse using an iPhone 4S in Patients with Atrial Fibrillation,” Vol. 10(3), pp. 315-319 (March 2013), the disclosure of which is incorporated by reference, discloses obtaining pulsatile time series recordings before and after cardioversion using the digital camera built into a smartphone. An algorithm implemented as an app executed by the smartphone analyzed recorded signals to accurately distinguish pulse recordings during atrial fibrillation from sinus rhythm, although such a smartphone-based approach provides non-continuous observation and would be impracticable for long term physiological monitoring. Further, the smartphone-implemented app does not provide continuous recordings, including the provision of pre-event and post-event context, critical for an accurate medical diagnosis that might trigger a meaningful and serious medical intervention. In addition, a physician would be loath to undertake a surgical or serious drug intervention without confirmatory evidence that the wearer in question was indeed the subject of the presumed rhythm abnormality. Validation of authenticity of the rhythm disorder for a specified patient takes on critical legal and medical importance.

[0010] The AliveCor heart monitor, manufactured by AliveCor, Inc., San Francisco, Calif., provides a non-continuous, patient-triggered event monitor, which is worn on the fingertip. Heart rate is sensed over a single lead (comparable to Lead I on a conventional ECG) and recorded by an app running on a smartphone, such as an iOS operating system-based smartphone, such as the iPhone, manufactured by Apple Inc., Cupertino, Calif., or an Android operating system-based smartphone, manufactured and offered by various companies, including Google Inc., Mountain View, Calif.; Samsung Electronics Co., Ltd., Suwon, S. Korea; Motorola Mobility LLC, a subsidiary of Google Inc., Libertyville, Ill.; and LG Electronics Inc., Seoul, S. Korea. The Android operating system is also licensed by Google Inc. The app can send the data recorded by an AliveCor heart monitor from the smartphone to healthcare providers, who ultimately decide whether to use the data for screening or diagnostic purposes. Furthermore, as explained supra with respect to the McManus reference, none of these devices provides the context of the

arrhythmia, as well as the medico-legal confirmation that would otherwise allow for a genuine medical intervention.

[0011] Similarly, adherents to the so-called “Quantified Self” movement combine wearable sensors and wearable computing to self-track activities of their daily lives. The Fitbit Tracker, manufactured by Fitbit Inc., San Francisco, Calif.; the Jawbone UP, manufactured by Jawbone, San Francisco, Calif.; the Polar Loop, manufactured by Polar Electro, Kempele, Finland; and the Nike+ FuelBand, manufactured by Nike Inc., Beaverton, Oreg., for instance, provide activity trackers worn on the wrist or body with integrated fitness tracking features, such as a heart rate monitor and pedometer to temporally track the number of steps taken each day with an estimation calories burned. The activity tracker can interface with a smartphone or computer to allow a wearer to monitor their progress towards a fitness goal. These activity trackers are accessories to smartphones, including iOS operating system-based smartphones, Android operating system-based smartphones, and Windows Phone operating-system based smartphones, such as manufactured by Microsoft Corporation, Redmond, WA, to which recorded data must be offloaded for storage and viewing.

[0012] The features of activity trackers can also be increasingly found in so-called “smart” watches that combine many of the features of activity trackers with smartphones. Entire product lines are beginning to be offered to provide a range of fitness- and health-tracking solutions. As one example, Samsung Electronics Co., Ltd., offers a line of mobile products with fitness-oriented features, including the Galaxy S5 smartphone, which incorporates a biometric fingerprint reader and heart rate monitor; the Gear 2 smart watch, which also incorporates a heart rate monitor; and the Gear Fit wearable device, which incorporates a heart rate monitor, real time fitness coaching, and activity tracker. The Galaxy S5 smartphone’s heart rate monitor is not meant for continuous tracking, while the both the Gear 2 smart watch and Gear Fit wearable device must be paired with a smartphone or computer to offload and view the recorded data.

[0013] With all manner of conventional “fitness-oriented” device, whether smartphone, smart watch, or activity tracker, quantified physiology is typically tracked for only the personal use of the wearer. Monitoring can be either continuous or non-continuous. The wearer must take extra steps to route recorded data to a health care provider; thus, with rare exception, the data is not time-correlated to physician-supervised monitoring nor validated. Furthermore, the monitoring is strictly informational and medically-significant events, such as serious cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias, while potentially detectable, are neither identified nor acted upon.

[0014] In today’s medical and legal environment, a mobile device, such as a smartphone, provides information that cannot be translated into data that triggers surgery or drug therapy by a physician. In the case of a smartphone detecting a fast heartbeat, for example, such a detection and the information on the smartphone would neither be identified as truly related to the patient in question or would be deemed sufficient for subjecting a patient to surgery or potentially toxic drug therapy. Thus, such data that is available today is not actionable in a medically therapeutic relevant way. To make such data actionable, one must have recorded data that allows a specific rhythm diagnosis, and a vague recording hinting that something may be wrong with the heart will not suffice. Further, the recorded data must not only identify the heart-

related event of concern, but the signals before and after the event, which provides critical medical information for a physician to diagnose the disorder specifically. Finally, the recorded data must be made certifiable, so that the relationship of the recorded data to the patient that the physician is seeing is clear and appropriately identifiable as an event originating in the patient being examined. Establishing this relationship of data-to-patient has become a legally mandatory step in providing medical care, which heretofore has been impracticable insofar as one cannot merely rely upon a smartphone to provide legally sufficient identification of an abnormality with actionable data such that a patient undergoes a serious medical intervention.

[0015] Therefore, a need remains for an extended wear continuously recording ECG monitor practicably capable of being worn for a long period of time in both men and women and capable of recording high quality atrial and ventricular signals reliably.

[0016] A further need remains for facilities to integrate wider-ranging physiological and “life tracking”-type data into long-term ECG and physiological data monitoring coupled with an onboard ability to cascade into the medical records and to the medical authorities appropriate medical intervention upon detection of a condition of potential medical concern.

SUMMARY

[0017] Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. The wearable monitor sits centrally (in the midline) on the patient’s chest along the sternum oriented top-to-bottom. The placement of the wearable monitor in a location at the sternal midline (or immediately to either side of the sternum), with its unique narrow “hourglass”-like shape, benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout the monitoring period. Instead, the patient is free to place an electrode patch anywhere within the general region of the sternum, the area most likely to record high quality atrial signals or P-waves. Moreover, the wearable monitor is worn in such a location that is comfortable to woman and allows wear during activity.

[0018] In a further embodiment, the wearable monitor can interoperate wirelessly with other wearable physiology monitors and activity sensors and with mobile devices, including so-called “smartphones,” as well as with personal computers and tablet or handheld computers, to download monitoring data either in real-time or in batches. Where a wearable physiology monitor, activity sensor, or mobile device worn or held by the patient includes the capability to sense cardiac activity, particularly heart rate, or other physiology, an application executed by the monitor, sensor, or device can trigger the dispatch of a medically-actionable wearable monitor to the patient upon detecting potentially medically-significant events, such as cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias. Upon receipt of the wearable monitor, the patient can use the sensor or device, if appropriately equipped with photographic, fingerprint or thumbprint, or other recording features, to physically record the placement and use of the wearable monitor, thereby facilitating the authentication of the data recorded by the wearable monitor. Finally, the monitor recorder can also be equipped with a wireless transceiver to either provide data or other

information to, or receive data or other information from, an interfacing wearable physiology monitor, activity sensor, or mobile device for relay to an external system or further device, such as a server, analysis, or for further legal validation of the relationship of the monitor to the patient, or for other purpose.

[0019] One embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor recorder. A sealed housing is adapted to be removably secured into the non-conductive receptacle on a disposable extended wear electrode patch. Electronic circuitry is included within the sealed housing. An externally-powered micro-controller is operable to execute under micro programmable control. An electrocardiographic front end circuit is electrically interfaced to the micro-controller and is operable to sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended wear electrode patch. A wireless transceiver is electrically interfaced with the micro-controller and is operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals. Externally-powered flash memory is electrically interfaced with the micro-controller and is operable to store the samples of the electrocardiographic signals.

[0020] A further embodiment provides a remotely-interfaceable extended wear electrocardiography and physiological sensor monitor. A disposable extended wear electrode patch includes a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal midsection and, on each end, a contact surface at least partially coated with an adhesive dressing provided as a crimp relief. A pair of electrocardiographic electrodes is conductively exposed on the contact surface of each end of the elongated strip. A non-conductive receptacle is adhered to an outward-facing end of the elongated strip and includes a plurality of electrical pads. A flexible circuit is affixed on each end of the elongated strip as a strain relief and includes a pair of circuit traces electrically coupled to the pair of electrocardiographic electrodes and a pair of the electrical pads. A reusable electrocardiography monitor has a sealed housing adapted to be removably secured into the non-conductive receptacle. A micro-controller is operable to execute under micro programmable control and is electrically interfaced to an electrocardiographic front end circuit that is operable to sense electrocardiographic signals through the electrocardiographic electrodes via the pair of electrical pads. A wireless transceiver is electrically interfaced with the micro-controller and is operable to wirelessly interface with an external wireless-enabled device to communicate samples of the electrocardiographic signals. Flash memory is electrically interfaced with the micro-controller and is operable to store the samples of the electrocardiographic signals.

[0021] A still further embodiment provides a computer-implemented system and method for providing a personal mobile device-triggered medical intervention. An activity monitor is adapted to be used proximal to a patient’s body and includes a physiology sensor operable to sense physiological data of the body. A personal mobile device includes an application executable by the mobile device that is configured to detect an event of potential medical significance within the sensed physiological data. The mobile device also includes a wireless transceiver operable to interface the mobile device with an external system and to send notification of a detection of the event. An extended wear electrocardiography and

physiological sensor monitor recorder is dispatched by the external system upon receipt of the notification.

[0022] The monitoring patch is especially suited to the female anatomy. The narrow longitudinal midsection can fit nicely within the intermammary cleft of the breasts without inducing discomfort, whereas conventional patch electrodes are wide and, if adhered between the breasts, particularly hypertrophic or pendulous breasts, would cause chafing, irritation, frustration, and annoyance, leading to low patient compliance and possibly premature removal of the monitoring patch. Furthermore, such conventional patches do not have the electrical design and signal processing that would allow recording of the P-wave, given the close spacing of the bipolar electrodes.

[0023] The foregoing aspects enhance ECG monitoring performance and quality, facilitating long-term ECG recording, critical to accurate arrhythmia diagnosis.

[0024] In addition, the foregoing aspects enhance comfort in women (and certain men), but not irritation of the breasts, by placing the monitoring patch in the best location possible for optimizing the recording of cardiac signals from the atrium, another feature critical to proper arrhythmia diagnosis.

[0025] Finally, the foregoing aspects as relevant to monitoring are equally applicable to recording other physiological data, such as heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar (with appropriate subcutaneous probe), oxygen saturation, minute ventilation, as well as other measures of body chemistry and physiology.

[0026] Still other embodiments will become readily apparent to those skilled in the art from the following detailed description, wherein are described embodiments by way of illustrating the best mode contemplated. As will be realized, other and different embodiments are possible and the embodiments' several details are capable of modifications in various obvious respects, all without departing from their spirit and the scope. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not as restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor respectively fitted to the sternal region of a female patient and a male patient.

[0028] FIG. 3 is a functional block diagram showing a system for remote interfacing of an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

[0029] FIG. 4 is a perspective view showing an extended wear electrode patch with a monitor recorder inserted.

[0030] FIG. 5 is a perspective view showing the monitor recorder of FIG. 4.

[0031] FIG. 6 is a perspective view showing the extended wear electrode patch of FIG. 4 without a monitor recorder inserted.

[0032] FIG. 7 is a bottom plan view of the monitor recorder of FIG. 4.

[0033] FIG. 8 is a top view showing the flexible circuit of the extended wear electrode patch of FIG. 4 when mounted above the flexible backing

[0034] FIG. 9 is a functional block diagram showing the component architecture of the circuitry of the monitor recorder of FIG. 4.

[0035] FIG. 10 is a functional block diagram showing the circuitry of the extended wear electrode patch of FIG. 4.

[0036] FIG. 11 is a flow diagram showing a monitor recorder-implemented method for monitoring ECG data for use in the monitor recorder of FIG. 4.

[0037] FIG. 12 is a graph showing, by way of example, a typical ECG waveform.

[0038] FIG. 13 is a flow diagram showing a method for offloading and converting ECG and other physiological data from an extended wear electrocardiography and physiological sensor monitor in accordance with one embodiment.

DETAILED DESCRIPTION

[0039] Physiological monitoring can be provided through a wearable monitor that includes two components, a flexible extended wear electrode patch and a removable reusable monitor recorder. FIGS. 1 and 2 are diagrams showing, by way of examples, an extended wear electrocardiography and physiological sensor monitor 12, including a monitor recorder 14 in accordance with one embodiment, respectively fitted to the sternal region of a female patient 10 and a male patient 11. The wearable monitor 12 sits centrally (in the midline) on the patient's chest along the sternum 13 oriented top-to-bottom with the monitor recorder 14 preferably situated towards the patient's head. In a further embodiment, the orientation of the wearable monitor 12 can be corrected post-monitoring, as further described infra. The electrode patch 15 is shaped to fit comfortably and conformal to the contours of the patient's chest approximately centered on the sternal midline 16 (or immediately to either side of the sternum 13). The distal end of the electrode patch 15 extends towards the Xiphoid process and, depending upon the patient's build, may straddle the region over the Xiphoid process. The proximal end of the electrode patch 15, located under the monitor recorder 14, is below the manubrium and, depending upon patient's build, may straddle the region over the manubrium.

[0040] The placement of the wearable monitor 12 in a location at the sternal midline 16 (or immediately to either side of the sternum 13) significantly improves the ability of the wearable monitor 12 to cutaneously sense cardiac electric signals, particularly the P-wave (or atrial activity) and, to a lesser extent, the QRS interval signals in the ECG waveforms that indicate ventricular activity, while simultaneously facilitating comfortable long-term wear for many weeks. The sternum 13 overlies the right atrium of the heart and the placement of the wearable monitor 12 in the region of the sternal midline 13 puts the ECG electrodes of the electrode patch 15 in a location better adapted to sensing and recording P-wave signals than other placement locations, say, the upper left pectoral region or lateral thoracic region or the limb leads. In addition, placing the lower or inferior pole (ECG electrode) of the electrode patch 15 over (or near) the Xiphoid process facilitates sensing of ventricular activity and provides superior recordation of the QRS interval.

[0041] When operated standalone, the monitor recorder 14 of the extended wear electrocardiography and physiological sensor monitor 12 senses and records the patient's ECG data into an onboard memory. In addition, the wearable monitor 12 can interoperate with other devices. FIG. 3 is a functional block diagram showing a system 120 for remote interfacing of an extended wear electrocardiography and physiological sensor monitor 12 in accordance with one embodiment. The monitor recorder 14 is a reusable component that can be fitted during patient monitoring into a non-conductive receptacle

provided on the electrode patch 15, as further described infra with reference to FIG. 4, and later removed for offloading of stored ECG data or to receive revised programming. The monitor recorder 14 can then be connected to a download station 125, which could be a programmer or other device that permits the retrieval of stored ECG monitoring data, execution of diagnostics on or programming of the monitor recorder 14, or performance of other functions. The monitor recorder 14 has a set of electrical contacts (not shown) that enable the monitor recorder 14 to physically interface to a set of terminals 128 on a paired receptacle 127 of the download station 125. In turn, the download station 125 executes a communications or offload program 126 ("Offload") or similar program that interacts with the monitor recorder 14 via the physical interface to retrieve the stored ECG monitoring data. The download station 125 could be a server, personal computer, tablet or handheld computer, smart mobile device, or purpose-built programmer designed specific to the task of interfacing with a monitor recorder 14. Still other forms of download station 125 are possible.

[0042] Upon retrieving stored ECG monitoring data from a monitor recorder 14, middleware first operates on the retrieved data to adjust the ECG capture quality, as necessary, and to convert the retrieved data into a format suitable for use by third party post-monitoring analysis software, as further described infra with reference to FIG. 13. The formatted data can then be retrieved from the download station 125 over a hard link 135 using a control program 137 ("Ctl") or analogous application executing on a personal computer 136 or other connectable computing device, via a communications link (not shown), whether wired or wireless, or by physical transfer of storage media (not shown). The personal computer 136 or other connectable device may also execute middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program, as further described infra with reference to FIG. 13. Note that formatted data stored on the personal computer 136 would have to be maintained and safeguarded in the same manner as electronic medical records (EMRs) 134 in the secure database 124, as further discussed infra. In a further embodiment, the download station 125 is able to directly interface with other devices over a computer communications network 121, which could be some combination of a local area network and a wide area network, including the Internet, over a wired or wireless connection.

[0043] A client-server model could be used to employ a server 122 to remotely interface with the download station 125 over the network 121 and retrieve the formatted data or other information. The server 122 executes a patient management program 123 ("Mgt") or similar application that stores the retrieved formatted data and other information in a secure database 124 cataloged in that patient's EMRs 134. In addition, the patient management program 123 could manage a subscription service that authorizes a monitor recorder 14 to operate for a set period of time or under pre-defined operational parameters.

[0044] The patient management program 123, or other trusted application, also maintains and safeguards the secure database 124 to limit access to patient EMRs 134 to only authorized parties for appropriate medical or other uses, such as mandated by state or federal law, such as under the Health Insurance Portability and Accountability Act (HIPAA) or per the European Union's Data Protection Directive. For example, a physician may seek to review and evaluate his

patient's ECG monitoring data, as securely stored in the secure database 124. The physician would execute an application program 130 ("Pgm"), such as a post-monitoring ECG analysis program, on a personal computer 129 or other connectable computing device, and, through the application 130, coordinate access to his patient's EMRs 134 with the patient management program 123. Other schemes and safeguards to protect and maintain the integrity of patient EMRs 134 are possible.

[0045] The wearable monitor 12 can interoperate wirelessly with other wearable physiology monitors and activity sensors 131, such as activity trackers worn on the wrist or body, and with mobile devices 133, including smart watches and smartphones. Wearable physiology monitors and activity sensors 131 encompass a wide range of wirelessly interconnectable devices that measure or monitor a patient's physiological data, such as heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar (with appropriate subcutaneous probe), oxygen saturation, minute ventilation, and so on; physical states, such as movement, sleep, footsteps, and the like; and performance, including calories burned or estimated blood glucose level. The physiology sensors in non-wearable mobile devices, particularly smartphones, are generally not meant for continuous tracking and do not provide medically precise and actionable data sufficient for a physician to prescribe a surgical or serious drug intervention; such data can be considered screening information that something may be wrong, but not data that provides the highly precise information that may allow for a surgery, such as implantation of a pacemaker for heart block or a defibrillator for ventricular tachycardia, or the application of serious medications, like blood thinners for atrial fibrillation or a cardiac ablation procedure. Such devices, like smartphones, are better suited to pre- and post-exercise monitoring or as devices that can provide a signal that something is wrong, but not in the sufficient detail and validation to allow for medical action. Conversely, medically actionable wearable sensors and devices sometimes provide continuous recording for relatively short time periods, but must be paired with a smartphone or computer to offload and evaluate the recorded data, especially if the data is of urgent concern.

[0046] Wearable physiology monitors and activity sensors 131, also known as "activity monitors," and to a lesser extent, "fitness" sensor-equipped mobile devices 133, can trace their life-tracking origins to ambulatory devices used within the medical community to sense and record traditional medical physiology that could be useful to a physician in arriving at a patient diagnosis or clinical trajectory, as well as from outside the medical community, from, for instance, sports or lifestyle product companies who seek to educate and assist individuals with self-quantifying interests. Data is typically tracked by the wearable physiology monitors or activity sensors 131 and mobile device 133 for only the personal use of the wearer. The physiological monitoring is strictly informational, even where a device originated within the medical community, and the data is generally not time-correlated to physician-supervised monitoring. Importantly, medically-significant events, such as cardiac rhythm disorders, including tachyarrhythmias, like ventricular tachycardia or atrial fibrillation, and bradyarrhythmias, like heart block, while potentially detectable with the appropriate diagnostic heuristics, are neither identified nor acted upon by the wearable physiology monitors and activity sensors 131 and the mobile device 133.

[0047] Frequently, wearable physiology monitors and activity sensors 131 are capable of wirelessly interfacing with mobile devices 133, particularly smart mobile devices, including so-called “smartphones” and “smart watches,” as well as with personal computers and tablet or handheld computers, to download monitoring data either in real-time or in batches. The wireless interfacing of such activity monitors is generally achieved using transceivers that provide low-power, short-range wireless communications, such as Bluetooth, although some wearable physiology monitors and activity sensors 131, like their mobile device cohorts, have transceivers that provide true wireless communications services, including 4G or better mobile telecommunications, over a telecommunications network. Other types of wireless and wired interfacing are possible.

[0048] Where the wearable physiology monitors and activity sensors 131 are paired with a mobile device 133, the mobile device 133 executes an application (“App”) that can retrieve the data collected by the wearable physiology monitor and activity sensor 131 and evaluate the data to generate information of interest to the wearer, such as an estimation of the effectiveness of the wearer’s exercise efforts. Where the wearable physiology monitors and activity sensors 131 has sufficient onboard computational resources, the activity monitor itself executes an app without the need to relay data to a mobile device 133. Generally, such more computationally-capable wearable physiology monitors and activity sensors are also equipped with wireless communications services transceivers, such as found in some smart watches that combine the features of activity monitors with mobile devices. Still other activity monitor and mobile device functions on the collected data are possible.

[0049] In a further embodiment, a wearable physiology monitor, activity sensor 131, or mobile device 133 worn or held by the patient 10, or otherwise be used proximal to the patient’s body, can be used to first obtain and then work collaboratively with a more definitive monitor recorder 14 to enable the collection of physiology by the monitor recorder 14 before, during, and after potentially medically-significant events. The wearable physiology monitor, activity sensor 131, or mobile device 133 must be capable of sensing cardiac activity, particularly heart rate or rhythm, or other types of physiology or measures, either directly or upon review of relayed data. Where the wearable physiology monitor or activity sensor 131 is paired with a mobile device 133, the mobile device 133 serves as a relay device and executes an application that will trigger the dispatch of a monitor recorder 14 to the patient 10 upon detecting potentially medically-significant events in the data provided by the paired activity monitor, such as cardiac rhythm disorders, including tachyarrhythmias and bradyarrhythmias. If the mobile device 133 is itself performing the monitoring of the patient’s physiology, the mobile device 133 executes an application that will trigger the dispatch of a monitor recorder 14 to the patient 10 in near-real time upon detecting potentially medically-significant events, thereby avoiding the delay incurred by data relay from an activity monitor. Finally, if the wearable physiology monitor or activity sensor 131 has sufficient onboard computational resources and also is equipped with a wireless communications services transceiver, the wearable physiology monitor or activity sensor 131 effectively becomes the mobile device 133 and executes an application that will trigger the dispatch of a monitor recorder 14 to the patient 10 in near-real time upon detecting potentially medically-signifi-

cant events without the need to first interface with a mobile device 133. Still other configurations of the detection app are possible.

[0050] The act of triggering the dispatch of a monitor recorder 14 represents the first step in a cascade of possible medical interventions of potentially increasing seriousness and urgency. Sensors 131 and devices 133 are generally not capable of detecting and recording medically precise and actionable data, whereas, as a device designed for extended wear, the monitor recorder 14 continually monitors the patient’s physiology over a long time period and will capture any medically-actionable data leading up to, throughout the occurrence of, and following an event of potential medical concern.

[0051] The monitoring data recorded by the monitor recorder 14 can be uploaded directly into the patient’s EMRs 134, either by using a mobile device 133 as a conduit for communications with a server 122 coupled to a secure database 124 within which the patient’s EMRs 134 are stored, or directly to the server 122, if the monitor recorder 14 is appropriately equipped with a wireless transceiver or similar external data communications interface, as further described infra. Thus, the data recorded by the monitor recorder 14 would directly feed into the patient’s EMRs 134, thereby allowing the data to be made certifiable for immediate use by a physician or healthcare provider. No intermediate steps would be necessary when going from cutaneously sensing cardiac electric signals and collecting the patient’s physiology using a monitor recorder 14 to presenting that recorded data to a physician or healthcare provider for medical diagnosis and care. The direct feeding of data from the monitor recorder 14 to the EMRs 134 clearly establishes the relationship of the data, as recorded by the monitor recorder 14, to the patient 10 that the physician is seeing and appropriately identifies any potentially medically-significant event recorded in the data as originating in the patient 10 and nobody else. Based on the monitoring data, physicians and healthcare providers can rely on the data as certifiable and can directly proceed with determining the appropriate course of treatment for the patient 10, including undertaking further medical interventions as appropriate. In a further embodiment, the server 122 can evaluate the recorded data, as fed into the patient’s EMRs 134, to refer the patient 10 for medical care to a general practice physician or medical specialist, for instance, a cardiac electrophysiologist referral from a cardiologist when the recorded data indicates an event of sufficient potential severity to warrant the possible implantation of a pacemaker for heart block or a defibrillator for ventricular tachycardia. Other uses of the data recorded by the monitor recorder 14 are possible.

[0052] For instance, a patient 10 who has previously suffered heart failure is particularly susceptible to ventricular tachycardia following a period of exercise or strenuous physical activity. A wearable sensor 131 or device 133 that includes a heart rate monitor would be able to timely detect an irregularity in heart rhythm. The application executed by the sensor 131 or device 133 allows those devices to take action by triggering the dispatch of a monitor recorder 14 to the patient 10, even though the data recorded by the sensor 131 or device 133 is itself generally medically-insufficient for purposes of diagnosis and care. Thus, rather than passively recording patient data, the sensor 131 or device 133 takes on an active role in initiating the provisioning of medical care to the patient 10 and starts a cascade of appropriate medical inter-

ventions under the tutelage of and followed by physicians and trained healthcare professionals.

[0053] In a still further embodiment, the monitor recorder **14** could upload an event detection application to the sensor **131** or device **133** to enable those devices to detect those types of potentially medically-significant events, which would trigger the dispatch of a monitor recorder **14** to the patient **10**. Alternatively, the event detection application could be downloaded to the sensor **131** or device **133** from an online application store or similar online application repository. Finally, the monitor recorder **14** could use the sensor **131** or device **133** to generate an appropriate alert, including contacting the patient's physician or healthcare services, via wireless (or wired) communications, upon detecting a potentially medically-significant event or in response to a patient prompting.

[0054] The patient **10** could be notified by the sensor **131** or device **133**, through the sensor's or device's user interface, that an event of potential medical concern has been detected coupled with an offer to have a monitor recorder **14** sent out to the patient **10**, assuming that the patient **10** is not already wearing a monitor recorder **14**. Alternatively, the sensor **131** or device **133** could unilaterally send out a request for a monitor recorder **14**. The request for a monitor recorder **14** could be sent via wireless (or wired) communications to the patient's physician, a medical service provider organization, a pharmacy, an emergency medical service, or other appropriate healthcare entity that would, in turn, physically provide the patient with a monitor recorder **14**. The patient **10** could also be told to pick up a monitor recorder **14** directly from one of the above-identified sources.

[0055] Conventional Holter monitors, as well as the ZIO XT Patch and ZIO Event Card devices, described supra, are currently available only by a physician's prescription for a specific patient **10**. As a result, the physiological data recorded by these monitors and devices are assumed by healthcare professional to belong to the patient **10**. In this prescriptive medicine context, grave questions as to the authenticity of the patient's identity and the data recorded do not generally arise, although current medical practice still favors requesting affirmative patient and caregiver identification at every step of healthcare provisioning. As a device intended for adoption and usage broader than prescriptive medicine, the monitor recorder **14** carries the potential to be used by more than one individual, which can raise concerns as to the veracity of the data recorded.

[0056] In a still further embodiment, the mobile device **133**, or, if properly equipped, the activity monitor, can be used to help authenticate the patient **10** at the outset of and throughout the monitoring period. The mobile device **133** (or activity monitor) must be appropriately equipped with a digital camera or other feature capable of recording physical indicia located within the proximity of the mobile device **133**. For instance, the Samsung Galaxy S5 smartphone has both a biometric fingerprint reader and autofocus digital camera built in. Upon receipt of a monitor recorder **14**, the patient **10** can use the photographic or other recording features of the mobile device **133** (or activity monitor) to physically record the placement and use of the monitor recorder **14**. For instance, the patient **10** could take a picture or make a video of the monitor recorder **14** using as applied to the chest using the built-in digital camera. The patient **10** could also swipe a finger over the biometric fingerprint reader. Preferably, the patient **10** would include both his or her face or similar uniquely-identifying marks or indicia, such as a scar, tattoo,

body piercing, or RFID chip, plus any visible or electronic indicia on the outside of the monitor recorder's housing, as further described infra with reference to FIG. 5, in the physical recording. The physical recording would then be sent by the mobile device **133** (or activity monitor) via wireless (or wired) communications to the patient's physician's office or other appropriate caregiver, thereby facilitating the authentication of the data recorded by the monitor recorder **14**. Alternatively, the physical recording could be securely stored by the monitor recorder **14** as part of the monitoring data set.

[0057] The mobile device **133** could also serve as a conduit for providing the data collected by the wearable physiology monitor or activity sensor **131** to a server **122**, or, similarly, the wearable physiology monitor or activity sensor **131** could itself directly provide the collected data to the server **122**. The server **122** could then merge the collected data into the wearer's EMRs **134** in the secure database **124**, if appropriate (and permissible), or the server **122** could perform an analysis of the collected data, perhaps based by comparison to a population of like wearers of the wearable physiology monitor or activity sensor **131**. Still other server **122** functions on the collected data are possible.

[0058] Finally, the monitor recorder **14** can also be equipped with a wireless transceiver, as further described infra with reference to FIGS. 9 and 10. Thus, when wireless-enabled, both wearable physiology monitors, activity sensors **131**, and mobile devices **133** can wirelessly interface with the monitor recorder **14**, which could either provide data or other information to, or receive data or other information from an interfacing device for relay to a further device, such as the server **122**, analysis, or other purpose. In addition, the monitor recorder **14** could wirelessly interface directly with the server **122**, personal computer **129**, or other computing device connectable over the network **121**, when the monitor recorder **14** is appropriately equipped for interfacing with such devices. Still other types of remote interfacing of the monitor recorder **14** are possible.

[0059] During use, the electrode patch **15** is first adhered to the skin along the sternal midline **16** (or immediately to either side of the sternum **13**). A monitor recorder **14** is then snapped into place on the electrode patch **15** to initiate ECG monitoring. FIG. 4 is a perspective view showing an extended wear electrode patch **15** with a monitor recorder **14** in accordance with one embodiment inserted. The body of the electrode patch **15** is preferably constructed using a flexible backing **20** formed as an elongated strip **21** of wrap knit or similar stretchable material with a narrow longitudinal mid-section **23** evenly tapering inward from both sides. A pair of cut-outs **22** between the distal and proximal ends of the electrode patch **15** create a narrow longitudinal midsection **23** or "isthmus" and defines an elongated "hourglass"-like shape, when viewed from above.

[0060] The electrode patch **15** incorporates features that significantly improve wearability, performance, and patient comfort throughout an extended monitoring period. During wear, the electrode patch **15** is susceptible to pushing, pulling, and torquing movements, including compressional and torsional forces when the patient bends forward, and tensile and torsional forces when the patient leans backwards. To counter these stress forces, the electrode patch **15** incorporates strain and crimp reliefs, such as described in commonly-assigned U.S. patent application, entitled "Extended Wear Electrocardiography Patch," Ser. No. 14/080,717, filed Nov. 14, 2013, pending, the disclosure of which is incorporated by reference.

In addition, the cut-outs **22** and longitudinal midsection **23** help minimize interference with and discomfort to breast tissue, particularly in women (and gynecomastic men). The cut-outs **22** and longitudinal midsection **23** further allow better conformity of the electrode patch **15** to sternal bowing and to the narrow isthmus of flat skin that can occur along the bottom of the intermammary cleft between the breasts, especially in buxom women. The cut-outs **22** and longitudinal midsection **23** help the electrode patch **15** fit nicely between a pair of female breasts in the intermammary cleft. Still other shapes, cut-outs and conformities to the electrode patch **15** are possible.

[0061] The monitor recorder **14** removably and reusably snaps into an electrically non-conductive receptacle **25** during use. The monitor recorder **14** contains electronic circuitry for recording and storing the patient's electrocardiography as sensed via a pair of ECG electrodes provided on the electrode patch **15**, such as described in commonly-assigned U.S. patent application, entitled "Extended Wear Ambulatory Electrocardiography and Physiological Sensor Monitor," Ser. No. 14/080,725, filed Nov. 14, 2013, pending, the disclosure of which is incorporated by reference. The non-conductive receptacle **25** is provided on the top surface of the flexible backing **20** with a retention catch **26** and tension clip **27** molded into the non-conductive receptacle **25** to conformably receive and securely hold the monitor recorder **14** in place.

[0062] The monitor recorder **14** includes a sealed housing that snaps into place in the non-conductive receptacle **25**. FIG. 5 is a perspective view showing the monitor recorder **14** of FIG. 4. The sealed housing **50** of the monitor recorder **14** intentionally has a rounded isosceles trapezoidal-like shape **52**, when viewed from above, such as described in commonly-assigned U.S. Design Patent application, entitled "Electrocardiography Monitor," Ser. No. 29/472,046, filed Nov. 7, 2013, pending, the disclosure of which is incorporated by reference. In addition, a label, barcode, QR code, or other visible or electronic indicia is printed on the outside of, applied to the outside of, or integrated into the sealed housing **50** to uniquely identify the monitor recorder **14** and can include a serial number, manufacturing lot number, date of manufacture, and so forth. The edges **51** along the top and bottom surfaces are rounded for patient comfort. The sealed housing **50** is approximately 47 mm long, 23 mm wide at the widest point, and 7 mm high, excluding a patient-operable tactile-feedback button **55**. The sealed housing **50** can be molded out of polycarbonate, ABS, or an alloy of those two materials. The button **55** is waterproof and the button's top outer surface is molded silicon rubber or similar soft pliable material. A retention detent **53** and tension detent **54** are molded along the edges of the top surface of the housing **50** to respectively engage the retention catch **26** and the tension clip **27** molded into non-conductive receptacle **25**. Other shapes, features, and conformities of the sealed housing **50** are possible.

[0063] The electrode patch **15** is intended to be disposable. The monitor recorder **14**, however, is reusable and can be transferred to successive electrode patches **15** to ensure continuity of monitoring. The placement of the wearable monitor **12** in a location at the sternal midline **16** (or immediately to either side of the sternum **13**) benefits long-term extended wear by removing the requirement that ECG electrodes be continually placed in the same spots on the skin throughout

the monitoring period. Instead, the patient is free to place an electrode patch **15** anywhere within the general region of the sternum **13**.

[0064] As a result, at any point during ECG monitoring, the patient's skin is able to recover from the wearing of an electrode patch **15**, which increases patient comfort and satisfaction, while the monitor recorder **14** ensures ECG monitoring continuity with minimal effort. A monitor recorder **14** is merely unsnapped from a worn out electrode patch **15**, the worn out electrode patch **15** is removed from the skin, a new electrode patch **15** is adhered to the skin, possibly in a new spot immediately adjacent to the earlier location, and the same monitor recorder **14** is snapped into the new electrode patch **15** to reinitiate and continue the ECG monitoring.

[0065] During use, the electrode patch **15** is first adhered to the skin in the sternal region. FIG. 6 is a perspective view showing the extended wear electrode patch **15** of FIG. 4 without a monitor recorder **14** inserted. A flexible circuit **32** is adhered to each end of the flexible backing **20**. A distal circuit trace **33** and a proximal circuit trace (not shown) electrically couple ECG electrodes (not shown) to a pair of electrical pads **34**. The electrical pads **34** are provided within a moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**. When the monitor recorder **14** is securely received into the non-conductive receptacle **25**, that is, snapped into place, the electrical pads **34** interface to electrical contacts (not shown) protruding from the bottom surface of the monitor recorder **14**, and the moisture-resistant seal **35** enables the monitor recorder **14** to be worn at all times, even during bathing or other activities that could expose the monitor recorder **14** to moisture.

[0066] In addition, a battery compartment **36** is formed on the bottom surface of the non-conductive receptacle **25**, and a pair of battery leads (not shown) electrically interface the battery to another pair of the electrical pads **34**. The battery contained within the battery compartment **35** can be replaceable, rechargeable or disposable.

[0067] The monitor recorder **14** draws power externally from the battery provided in the non-conductive receptacle **25**, thereby uniquely obviating the need for the monitor recorder **14** to carry a dedicated power source. FIG. 7 is a bottom plan view of the monitor recorder **14** of FIG. 4. A cavity **58** is formed on the bottom surface of the sealed housing **50** to accommodate the upward projection of the battery compartment **36** from the bottom surface of the non-conductive receptacle **25**, when the monitor recorder **14** is secured in place on the non-conductive receptacle **25**. A set of electrical contacts **56** protrude from the bottom surface of the sealed housing **50** and are arranged in alignment with the electrical pads **34** provided on the bottom surface of the non-conductive receptacle **25** to establish electrical connections between the electrode patch **15** and the monitor recorder **14**. In addition, a seal coupling **57** circumferentially surrounds the set of electrical contacts **56** and securely mates with the moisture-resistant seal **35** formed on the bottom surface of the non-conductive receptacle **25**.

[0068] The placement of the flexible backing **20** on the sternal midline **16** (or immediately to either side of the sternum **13**) also helps to minimize the side-to-side movement of the wearable monitor **12** in the left- and right-handed directions during wear. To counter the dislodgment of the flexible backing **20** due to compressional and torsional forces, a layer of non-irritating adhesive, such as hydrocolloid, is provided at least partially on the underside, or contact, surface of the

flexible backing 20, but only on the distal end 30 and the proximal end 31. As a result, the underside, or contact surface of the longitudinal midsection 23 does not have an adhesive layer and remains free to move relative to the skin. Thus, the longitudinal midsection 23 forms a crimp relief that respectively facilitates compression and twisting of the flexible backing 20 in response to compressional and torsional forces. Other forms of flexible backing crimp reliefs are possible.

[0069] Unlike the flexible backing 20, the flexible circuit 32 is only able to bend and cannot stretch in a planar direction. The flexible circuit 32 can be provided either above or below the flexible backing 20. FIG. 8 is a top view showing the flexible circuit 32 of the extended wear electrode patch 15 of FIG. 4 when mounted above the flexible backing 20. A distal ECG electrode 38 and proximal ECG electrode 39 are respectively coupled to the distal and proximal ends of the flexible circuit 32. A strain relief 40 is defined in the flexible circuit 32 at a location that is partially underneath the battery compartment 36 when the flexible circuit 32 is affixed to the flexible backing 20. The strain relief 40 is laterally extendable to counter dislodgment of the ECG electrodes 38, 39 due to tensile and torsional forces. A pair of strain relief cutouts 41 partially extend transversely from each opposite side of the flexible circuit 32 and continue longitudinally towards each other to define in 'S'-shaped pattern, when viewed from above. The strain relief respectively facilitates longitudinal extension and twisting of the flexible circuit 32 in response to tensile and torsional forces. Other forms of circuit board strain relief are possible.

[0070] ECG monitoring and other functions performed by the monitor recorder 14 are provided through a micro controlled architecture. FIG. 9 is a functional block diagram showing the component architecture of the circuitry 60 of the monitor recorder 14 of FIG. 4. The circuitry 60 is externally powered through a battery provided in the non-conductive receptacle 25 (shown in FIG. 6). Both power and raw ECG signals, which originate in the pair of ECG electrodes 38, 39 (shown in FIG. 8) on the distal and proximal ends of the electrode patch 15, are received through an external connector 65 that mates with a corresponding physical connector on the electrode patch 15. The external connector 65 includes the set of electrical contacts 56 that protrude from the bottom surface of the sealed housing 50 and which physically and electrically interface with the set of pads 34 provided on the bottom surface of the non-conductive receptacle 25. The external connector includes electrical contacts 56 for data download, microcontroller communications, power, analog inputs, and a peripheral expansion port. The arrangement of the pins on the electrical connector 65 of the monitor recorder 14 and the device into which the monitor recorder 14 is attached, whether an electrode patch 15 or download station (not shown), follow the same electrical pin assignment convention to facilitate interoperability. The external connector 65 also serves as a physical interface to a download station that permits the retrieval of stored ECG monitoring data, communication with the monitor recorder 14, and performance of other functions.

[0071] Operation of the circuitry 60 of the monitor recorder 14 is managed by a microcontroller 61. The micro-controller 61 includes a program memory unit containing internal flash memory that is readable and writeable. The internal flash memory can also be programmed externally. The micro-controller 61 draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts

56. The microcontroller 61 connects to the ECG front end circuit 63 that measures raw cutaneous electrical signals and generates an analog ECG signal representative of the electrical activity of the patient's heart over time.

[0072] The circuitry 60 of the monitor recorder 14 also includes a flash memory 62, which the micro-controller 61 uses for storing ECG monitoring data and other physiology and information. The flash memory 62 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. Data is stored in a serial flash memory circuit, which supports read, erase and program operations over a communications bus. The flash memory 62 enables the microcontroller 61 to store digitized ECG data. The communications bus further enables the flash memory 62 to be directly accessed externally over the external connector 65 when the monitor recorder 14 is interfaced to a download station.

[0073] The circuitry 60 of the monitor recorder 14 further includes an actigraphy sensor 64 implemented as a 3-axis accelerometer. The accelerometer may be configured to generate interrupt signals to the microcontroller 61 by independent initial wake up and free fall events, as well as by device position. In addition, the actigraphy provided by the accelerometer can be used during post-monitoring analysis to correct the orientation of the monitor recorder 14 if, for instance, the monitor recorder 14 has been inadvertently installed upside down, that is, with the monitor recorder 14 oriented on the electrode patch 15 towards the patient's feet, as well as for other event occurrence analyses, such as described in commonly-assigned U.S. patent application, entitled "Event Alerting Through Actigraphy Embedded within Electrocardiographic Data," Ser. No. 14/082,108, filed Nov. 16, 2013, pending, the disclosure of which is incorporated by reference.

[0074] The circuitry 60 of the monitor recorder 14 includes a wireless transceiver 69 that can provides wireless interfacing capabilities. The wireless transceiver 69 also draws power externally from the battery provided on the electrode patch 15 via a pair of the electrical contacts 56. The wireless transceiver 69 can be implemented using one or more forms of wireless communications, including the IEEE 802.11 computer communications standard, that is Wi-Fi; the 4G mobile phone mobile standard; the Bluetooth data exchange standard; or other wireless communications or data exchange standards and protocols. The type of wireless interfacing capability could limit the range of interoperability of the monitor recorder 14; for instance, Bluetooth-based implementations are designed for low power consumption with a short communications range.

[0075] The microcontroller 61 includes an expansion port that also utilizes the communications bus. External devices, separately drawing power externally from the battery provided on the electrode patch 15 or other source, can interface to the microcontroller 61 over the expansion port in half duplex mode. For instance, an external physiology sensor can be provided as part of the circuitry 60 of the monitor recorder 14, or can be provided on the electrode patch 15 with communication with the micro-controller 61 provided over one of the electrical contacts 56. The physiology sensor can include an SpO2 sensor, blood pressure sensor, temperature sensor, respiratory rate sensor, glucose sensor, airflow sensor, volumetric pressure sensing, or other types of sensor or telemetric input sources. For instance, the integration of an airflow sensor is described in commonly-assigned U.S. patent application, entitled "Self-Contained Personal Air Flow Sensing

Monitor,” Ser. No. 14/082,102, filed Nov. 15, 2013, pending, the disclosure which is incorporated by reference.

[0076] Finally, the circuitry 60 of the monitor recorder 14 includes patient-interfaceable components, including a tactile feedback button 66, which a patient can press to mark events or to perform other functions, and a buzzer 67, such as a speaker, magnetic resonator or piezoelectric buzzer. The buzzer 67 can be used by the microcontroller 61 to output feedback to a patient such as to confirm power up and initiation of ECG monitoring. Still other components as part of the circuitry 60 of the monitor recorder 14 are possible.

[0077] While the monitor recorder 14 operates under micro control, most of the electrical components of the electrode patch 15 operate passively. FIG. 10 is a functional block diagram showing the circuitry 70 of the extended wear electrode patch 15 of FIG. 4. The circuitry 70 of the electrode patch 15 is electrically coupled with the circuitry 60 of the monitor recorder 14 through an external connector 74. The external connector 74 is terminated through the set of pads 34 provided on the bottom of the non-conductive receptacle 25, which electrically mate to corresponding electrical contacts 56 protruding from the bottom surface of the sealed housing 50 to electrically interface the monitor recorder 14 to the electrode patch 15.

[0078] The circuitry 70 of the electrode patch 15 performs three primary functions. First, a battery 71 is provided in a battery compartment formed on the bottom surface of the non-conductive receptacle 25. The battery 71 is electrically interfaced to the circuitry 60 of the monitor recorder 14 as a source of external power. The unique provisioning of the battery 71 on the electrode patch 15 provides several advantages. First, the locating of the battery 71 physically on the electrode patch 15 lowers the center of gravity of the overall wearable monitor 12 and thereby helps to minimize shear forces and the effects of movements of the patient and clothing. Moreover, the housing 50 of the monitor recorder 14 is sealed against moisture and providing power externally avoids having to either periodically open the housing 50 for the battery replacement, which also creates the potential for moisture intrusion and human error, or to recharge the battery, which can potentially take the monitor recorder 14 off line for hours at a time. In addition, the electrode patch 15 is intended to be disposable, while the monitor recorder 14 is a reusable component. Each time that the electrode patch 15 is replaced, a fresh battery is provided for the use of the monitor recorder 14, which enhances ECG monitoring performance quality and duration of use. Finally, the architecture of the monitor recorder 14 is open, in that other physiology sensors or components can be added by virtue of the expansion port of the microcontroller 61. Requiring those additional sensors or components to draw power from a source external to the monitor recorder 14 keeps power considerations independent of the monitor recorder 14. Thus, a battery of higher capacity could be introduced when needed to support the additional sensors or components without effecting the monitor recorder circuitry 60.

[0079] Second, the pair of ECG electrodes 38, 39 respectively provided on the distal and proximal ends of the flexible circuit 32 are electrically coupled to the set of pads 34 provided on the bottom of the non-conductive receptacle 25 by way of their respective circuit traces 33, 37. The signal ECG electrode 39 includes a protection circuit 72, which is an inline resistor that protects the patient from excessive leakage current.

[0080] Last, in a further embodiment, the circuitry 70 of the electrode patch 15 includes a cryptographic circuit 73 to authenticate an electrode patch 15 for use with a monitor recorder 14. The cryptographic circuit 73 includes a device capable of secure authentication and validation. The cryptographic device 73 ensures that only genuine, non-expired, safe, and authenticated electrode patches 15 are permitted to provide monitoring data to a monitor recorder 14, such as described in commonly-assigned U.S. patent application, entitled “Self-Authenticating Electrocardiography Circuit,” Ser. No. 14/082,066, filed Nov. 15, 2013, pending, the disclosure which is incorporated by reference.

[0081] In a further embodiment, the circuitry 70 of the electrode patch 15 includes a wireless transceiver 75, in lieu the including of the wireless transceiver 69 in the circuitry 60 of the monitor recorder 14, which interfaces with the microcontroller 61 over the microcontroller’s expansion port via the external connector 74.

[0082] The monitor recorder 14 continuously monitors the patient’s heart rate and physiology. FIG. 11 is a flow diagram showing a monitor recorder-implemented method 100 for monitoring ECG data for use in the monitor recorder 14 of FIG. 4. Initially, upon being connected to the set of pads 34 provided with the non-conductive receptacle 25 when the monitor recorder 14 is snapped into place, the microcontroller 61 executes a power up sequence (step 101). During the power up sequence, the voltage of the battery 71 is checked, the state of the flash memory 62 is confirmed, both in terms of operability check and available capacity, and microcontroller operation is diagnostically confirmed. In a further embodiment, an authentication procedure between the microcontroller 61 and the electrode patch 15 are also performed.

[0083] Following satisfactory completion of the power up sequence, an iterative processing loop (steps 102-109) is continually executed by the microcontroller 61. During each iteration (step 102) of the processing loop, the ECG frontend 63 (shown in FIG. 9) continually senses the cutaneous ECG electrical signals (step 103) via the ECG electrodes 38, 29 and is optimized to maintain the integrity of the P-wave. A sample of the ECG signal is read (step 104) by the microcontroller 61 by sampling the analog ECG signal output front end 63. FIG. 12 is a graph showing, by way of example, a typical ECG waveform 110. The x-axis represents time in approximate units of tenths of a second. The y-axis represents cutaneous electrical signal strength in approximate units of millivolts. The P-wave 111 has a smooth, normally upward, that is, positive, waveform that indicates atrial depolarization. The QRS complex usually begins with the downward deflection of a Q wave 112, followed by a larger upward deflection of an R-wave 113, and terminated with a downward waveform of the S wave 114, collectively representative of ventricular depolarization. The T wave 115 is normally a modest upward waveform, representative of ventricular depolarization, while the U wave 116, often not directly observable, indicates the recovery period of the Purkinje conduction fibers.

[0084] Sampling of the R-to-R interval enables heart rate information derivation. For instance, the R-to-R interval represents the ventricular rate and rhythm, while the P-to-P interval represents the atrial rate and rhythm. Importantly, the PR interval is indicative of atrioventricular (AV) conduction time and abnormalities in the PR interval can reveal underlying heart disorders, thus representing another reason why the P-wave quality achievable by the extended wear ambulatory electrocardiography and physiological sensor monitor

described herein is medically unique and important. The long-term observation of these ECG indicia, as provided through extended wear of the wearable monitor **12**, provides valuable insights to the patient's cardiac function and overall well-being.

[0085] Each sampled ECG signal, in quantized and digitized form, is temporarily staged in buffer (step **105**), pending compression preparatory to storage in the flash memory **62** (step **106**). Following compression, the compressed ECG digitized sample is again buffered (step **107**), then written to the flash memory **62** (step **108**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

[0086] In a further embodiment, the monitor recorder **14** also continuously receives data from wearable physiology monitors or activity sensors **131** and mobile devices **133** (shown in FIG. **3**). The data is received in a conceptually-separate execution thread as part of the iterative processing loop (steps **102-109**) continually executed by the microcontroller **61**. During each iteration (step **102**) of the processing loop, if wireless data is available (step **140**), a sample of the wireless is read (step **141**) by the microcontroller **61** and, if necessary, converted into a digital signal by the onboard ADC of the microcontroller **61**. Each wireless data sample, in quantized and digitized form, is temporarily staged in buffer (step **142**), pending compression preparatory to storage in the flash memory **62** (step **143**). Following compression, the compressed wireless data sample is again buffered (step **144**), then written to the flash memory **62** (step **145**) using the communications bus. Processing continues (step **109**), so long as the monitoring recorder **14** remains connected to the electrode patch **15** (and storage space remains available in the flash memory **62**), after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

[0087] The monitor recorder **14** stores ECG data and other information in the flash memory **62** (shown in FIG. **9**) using a proprietary format that includes data compression. As a result, data retrieved from a monitor recorder **14** must first be converted into a format suitable for use by third party post-monitoring analysis software. FIG. **13** is a flow diagram showing a method **150** for offloading and converting ECG and other physiological data from an extended wear electrocardiography and physiological sensor monitor **12** in accordance with one embodiment. The method **150** can be implemented in software and execution of the software can be performed on a download station **125**, which could be a programmer or other device, or a computer system, including a server **122** or personal computer **129**, such as further described supra with reference to FIG. **3**, as a series of process or method modules or steps. For convenience, the method **150** will be described in the context of being performed by a personal computer **136** or other connectable computing device (shown in FIG. **3**) as middleware that converts ECG data and other information into a format suitable for use by a third-party post-monitoring analysis program. Execution of the method **150** by a computer system would be analogous mutatis mutandis.

[0088] Initially, the download station **125** is connected to the monitor recorder **14** (step **151**), such as by physically interfacing to a set of terminals **128** on a paired receptacle **127**

or by wireless connection, if available. The data stored on the monitor recorder **14**, including ECG and physiological monitoring data, other recorded data, and other information are retrieved (step **152**) over a hard link **135** using a control program **137** ("Ctl") or analogous application executing on a personal computer **136** or other connectable computing device.

[0089] The data retrieved from the monitor recorder **14** is in a proprietary storage format and each datum of recorded ECG monitoring data, as well as any other physiological data or other information, must be converted, so that the data can be used by a third-party post-monitoring analysis program. Each datum of ECG monitoring data is converted by the middleware (steps **153-159**) in an iterative processing loop. During each iteration (step **153**), the ECG datum is read (step **154**) and, if necessary, the gain of the ECG signal is adjusted (step **155**) to compensate, for instance, for relocation or replacement of the electrode patch **15** during the monitoring period.

[0090] In addition, depending upon the configuration of the wearable monitor **12**, other physiological data (or other information), including patient events, such as a fall, peak activity level, sleep detection, Detection of patient activity levels and states, and so on, may be recorded along with the ECG monitoring data. For instance, actigraphy data may have been sampled by the actigraphy sensor **64** based on a sensed event occurrence, such as a sudden change in orientation due to the patient taking a fall. In response, the monitor recorder **14** will embed the actigraphy data samples into the stream of data, including ECG monitoring data, that is recorded to the flash memory **62** by the microcontroller **61**. Post-monitoring, the actigraphy data is temporally matched to the ECG data to provide the proper physiological context to the sensed event occurrence. As a result, the three-axis actigraphy signal is turned into an actionable event occurrence that is provided, through conversion by the middleware, to third party post-monitoring analysis programs, along with the ECG recordings contemporaneous to the event occurrence. Other types of processing of the other physiological data (or other information) are possible.

[0091] Thus, during execution of the middleware, any other physiological data (or other information) that has been embedded into the recorded ECG monitoring data is read (step **156**) and time-correlated to the time frame of the ECG signals that occurred at the time that the other physiological data (or other information) was noted (step **157**). Finally, the ECG datum, signal gain adjusted, if appropriate, and other physiological data, if applicable and as time-correlated, are stored in a format suitable to the backend software (step **158**) used in post-monitoring analysis.

[0092] In a further embodiment, the other physiological data, if apropos, is embedded within an unused ECG track. For example, the SCP-ENG standard allows multiple ECG channels to be recorded into a single ECG record. The monitor recorder **14**, though, only senses one ECG channel. The other physiological data can be stored into an additional ECG channel, which would otherwise be zero-padded or altogether omitted. The backend software would then be able to read the other physiological data in context with the single channel of ECG monitoring data recorded by the monitor recorder **14**, provided the backend software implemented changes necessary to interpret the other physiological data. Still other forms of embedding of the other physiological data with formatted ECG monitoring data, or of providing the other physiological data in a separate manner, are possible.

[0093] Processing continues (step **159**) for each remaining ECG datum, after which the processing loop is exited and execution terminates. Still other operations and steps are possible.

[0094] While the invention has been particularly shown and described as referenced to the embodiments thereof, those skilled in the art will understand that the foregoing and other changes in form and detail may be made therein without departing from the spirit and scope.

What is claimed is:

1. A computer-implemented system for providing a personal mobile device-triggered medical intervention, comprising:

an activity monitor adapted to be used proximal to a patient's body comprising a physiology sensor operable to sense physiological data of the body;

a personal mobile device, comprising:

an application executable by the mobile device and configured to detect an event of potential medical significance within the sensed physiological data; and
a wireless transceiver operable to interface the mobile device with an external system and to send notification of a detection of the event; and

an extended wear electrocardiography and physiological sensor monitor recorder dispatched by the external system upon receipt of the notification.

2. A system according to claim 1, further comprising at least one of:

the activity monitor further adapted to sense the physiological data continuously;
the activity monitor further adapted to sense the physiological data non-continuously; and
the activity monitor further adapted to sense the physiological data upon patient triggering.

3. A system according to claim 1, wherein the activity monitor is comprised in the mobile device.

4. A system according to claim 1, wherein the activity monitor is a device physically independent from the mobile device, further comprising:

the mobile device operable to be paired with the activity monitor and further comprising:

a wireless communications services transceiver operable to interface the mobile device with a telecommunications network upon which the external system is located; and

the activity monitor further comprising:

a short-range wireless transceiver operable to interface the activity monitor with the mobile device and to relay the notification to the mobile device.

5. A system according to claim 1, wherein the physiological data is selected from the group comprising heart rate, temperature, blood pressure, respiratory rate, blood pressure, blood sugar, oxygen saturation, and minute ventilation.

6. A system according to claim 1, further comprising:

the sensor monitor recorder comprising:

a sealed housing adapted to be removably secured into the non-conductive receptacle on a disposable extended wear electrode patch; and

electronic circuitry comprised within the sealed housing, comprising:

an externally-powered micro-controller operable to execute under micro programmable control;

an electrocardiographic front end circuit electrically interfaced to the micro-controller and operable to

sense electrocardiographic signals through electrocardiographic electrodes provided on the disposable extended wear electrode patch; and
externally-powered flash memory electrically interfaced with the micro-controller and operable to store the samples of the electrocardiographic signals.

7. A system according to claim 6, further comprising:

a recorder wireless transceiver electrically interfaced with the micro-controller and operable to interface the mobile device with a telecommunications network upon which electronic medical records are located; and

an upload module configured to send the samples of the electrocardiographic signals directly to the electronic medical records via the recorder wireless transceiver.

8. A system according to claim 7, further comprising:

a server coupled to the electronic medical records, further comprising:

a data retrieval module configured to retrieve the samples of the electrocardiographic signals from the electronic medical records; and

an evaluation module configured to evaluate the samples of the electrocardiographic signals and to refer the patient for medical care.

9. A system according to claim 7, further comprising:

a recording feature comprised in the mobile device operable to record physical indicia proximal to the mobile device,

wherein a recording of both the placement of the sensor monitor recorder on the patient's body and indicia uniquely identifying the patient are provided to the electronic medical records with the samples of the electrocardiographic signals as certification.

10. A system according to claim 9, further comprising:

the sealed housing further comprising indicia uniquely identifying the sensor monitor recorder,

wherein the recording further comprises the indicia uniquely the sensor monitor recorder.

11. A system according to claim 10, wherein the indicia uniquely the sensor monitor recorder is selected from the group comprising visible indicia printed on the outside of the sealed housing, visible indicia applied to the outside of the sealed housing, and electronic indicia integrated into the sealed housing.

12. A system according to claim 7, further comprising:

a recording feature comprised in the mobile device operable to record physical indicia proximal to the mobile device,

wherein a recording of the placement of the sensor monitor recorder on the patient's body and indicia uniquely identifying the patient are securely stored as part of the samples of the electrocardiographic signals as certification.

13. A system according to claim 12, further comprising:

the sealed housing further comprising indicia uniquely identifying the sensor monitor recorder,

wherein the recording further comprises the indicia uniquely the sensor monitor recorder.

14. A system according to claim 13, wherein the indicia uniquely the sensor monitor recorder is selected from the group comprising visible indicia printed on the outside of the sealed housing, visible indicia applied to the outside of the sealed housing, and electronic indicia integrated into the sealed housing.

- 15.** A system according to claim 6, further comprising:
a download station comprising:
 a non-conductive receptacle adapted to removably receive the monitor recorder; and
 a download station controller operable to retrieve the samples of the electrocardiographic signals; and
a computer system operatively coupled to the download station controller and centrally accessible over a data communications network and operable to maintain the samples of the electrocardiographic signals upon retrieval.
- 16.** A system according to claim 6, further comprising:
a pair of electrical contacts external to the sealed housing and electrically connected to at least one of the micro-controller, the wireless transceiver, and the flash memory;
a battery provided on the disposable extended wear electrode patch; and
an pair of electrical pads external to the disposable extended wear electrode patch and disposed to operatively couple with the pair of electrical contacts, the electrical pads further electrically interfaced via battery leads to the battery.
- 17.** A system according to claim 6, the disposable extended wear electrode patch further comprising:
a flexible backing formed of an elongated strip of stretchable material with a narrow longitudinal midsection and, on each end, a contact surface at least partially coated with an adhesive dressing provided as a crimp relief;
a pair of electrocardiographic electrodes conductively exposed on the contact surface of each end of the elongated strip;
a non-conductive receptacle adhered to an outward-facing end of the elongated strip and comprising the electrical pads; and
a flexible circuit affixed on each end of the elongated strip as a strain relief and comprising a pair of circuit traces electrically coupled to the pair of electrocardiographic electrodes and a pair of the electrical pads.
- 18.** A system according to claim 1, wherein the activity tracker is selected from the group comprising a wearable physiology sensor, a wearable activity sensor, a smart watch, and a smartphone.
- 19.** A system according to claim 1, further comprising at least one of:
a server computer system centrally accessible over a data communications network and operable to wirelessly interface with the wireless transceiver to receive the samples of the electrocardiographic signals; and
a client computer system interconnected to the data communications network and operable to wirelessly interface with the wireless transceiver to access the samples of the electrocardiographic signals.
- 20.** A system according to claim 19, further comprising:
a secure database interconnected to the data communications network and operable to maintain the samples of the electrocardiographic signals on behalf of one or more of the server computer system and the client computer system in the patient's electronic medical records.
- * * * * *

专利名称(译)	用于提供个人移动设备触发的医疗干预的计算机实现的系统和方法		
公开(公告)号	US20150088007A1	公开(公告)日	2015-03-26
申请号	US14/217402	申请日	2014-03-17
[标]申请(专利权)人(译)	BARDY诊断		
申请(专利权)人(译)	BARDY诊断, INC.		
当前申请(专利权)人(译)	BARDY诊断, INC.		
[标]发明人	BARDY GUST H FELIX JASON BISHAY JON MIKALSON		
发明人	BARDY, GUST H. FELIX, JASON BISHAY, JON MIKALSON		
IPC分类号	A61B5/00 A61B5/0205		
CPC分类号	A61B5/0205 A61B5/0022 A61B5/024 A61B5/7282 G06F19/3418 G06F19/00 G16H40/63		
优先权	61/882403 2013-09-25 US		
其他公开文献	US10165946		
外部链接	Espacenet USPTO		

摘要(译)

可以通过可穿戴式监视器提供生理监测，该监视器包括两个组件，一个灵活的扩展耐磨电极贴片和一个可拆卸的可重复使用的监视器记录器。可穿戴式监视器位于患者胸部的中央，沿着胸骨从上到下。将可穿戴式监视器放置在胸骨中线（或紧邻胸骨的任一侧）的位置，通过消除在整个监测期间将ECG电极连续放置在皮肤上的相同斑点中的要求，有利于延长佩戴。可穿戴式监视器可以与其他生理和活动传感器以及移动设备进行无线互操作。由传感器或设备执行的应用程序可以在检测到潜在的医学上重要的事件时触发将可穿戴监视器发送给患者。然后，分派的可穿戴监视器将能够提供精确的可医学操作的数据，而不仅仅是可能存在某些异常的警报。然后，患者可以使用传感器或设备物理地记录可医疗操作的可穿戴监视器的放置和使用，从而便于对所记录的数据进行认证。

