



US 20180078202A1

(19) **United States**(12) **Patent Application Publication**
DeGroot et al.(10) **Pub. No.: US 2018/0078202 A1**(43) **Pub. Date: Mar. 22, 2018**(54) **VITAL SIGNS MONITORING SYSTEM**(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,
EINDHOVEN (NL)(72) Inventors: **Koen Theo Johan DeGroot**, Sevenum
(NL); **Alberto Giovanni Bonomi**,
Eindhoven (NL)(21) Appl. No.: **15/564,593**(22) PCT Filed: **Apr. 8, 2016**(86) PCT No.: **PCT/EP2016/057825**


§ 371 (c)(1),

(2) Date: **Oct. 5, 2017**(30) **Foreign Application Priority Data**

Apr. 9, 2015 (EP) 15162997.9

Publication Classification(51) **Int. Cl.****A61B 5/00** (2006.01)**A61B 5/0205** (2006.01)(52) **U.S. Cl.**CPC **A61B 5/4866** (2013.01); **A61B 5/02416**
(2013.01); **A61B 5/681** (2013.01); **A61B**
5/0205 (2013.01)(57) **ABSTRACT**

A vital signs monitoring system comprises a processing unit (300) for estimating an activity energy expenditure (AEE), a first activity energy expenditure determining unit (320) for determining a first activity energy expenditure (AEEHR) based on heart rate data (HR), a second activity energy expenditure determining unit (330) for determining a second activity energy expenditure (AEEAC) based on motion data (AC), and a weighting unit (340) for determining a first and second weighting factor (wHR, wAC) based on a first and second probability relating to a high exertion (hH) and relating to a low exertion (hL), and activity energy expenditure calculating unit (350) for computing an overall activity energy expenditure (AEEO) based on the first activity energy expenditure (AEEHR) weighted by the first weighting factor (wHR) and on the second activity energy expenditure (AEEAC) weighted by the second weighting factor (wAC).

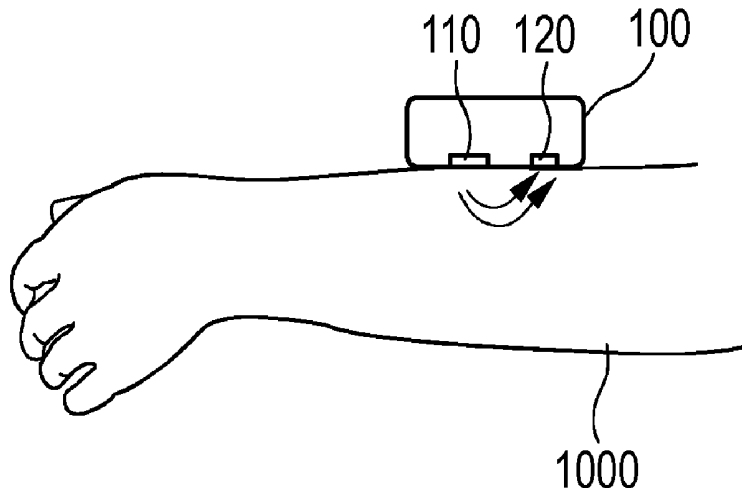

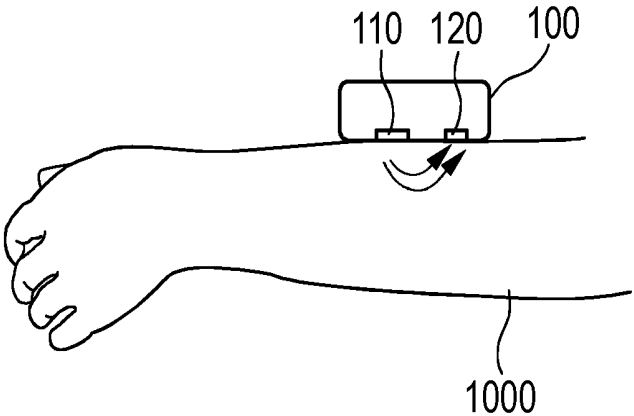


FIG. 1

FIG. 2

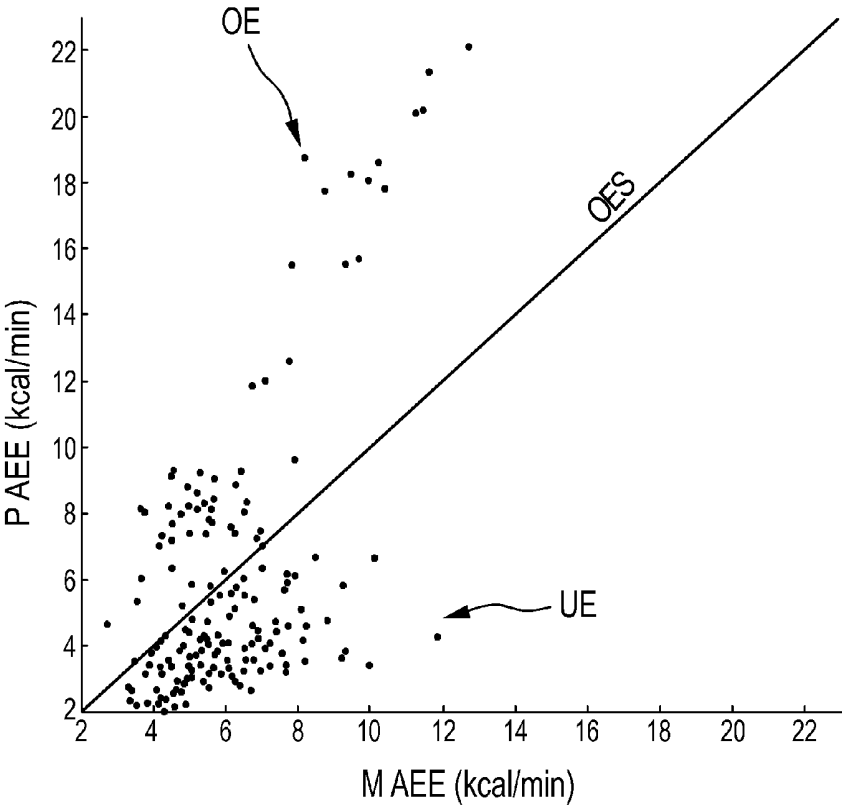
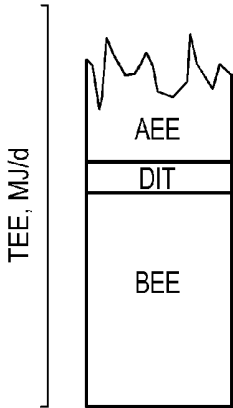


FIG. 3

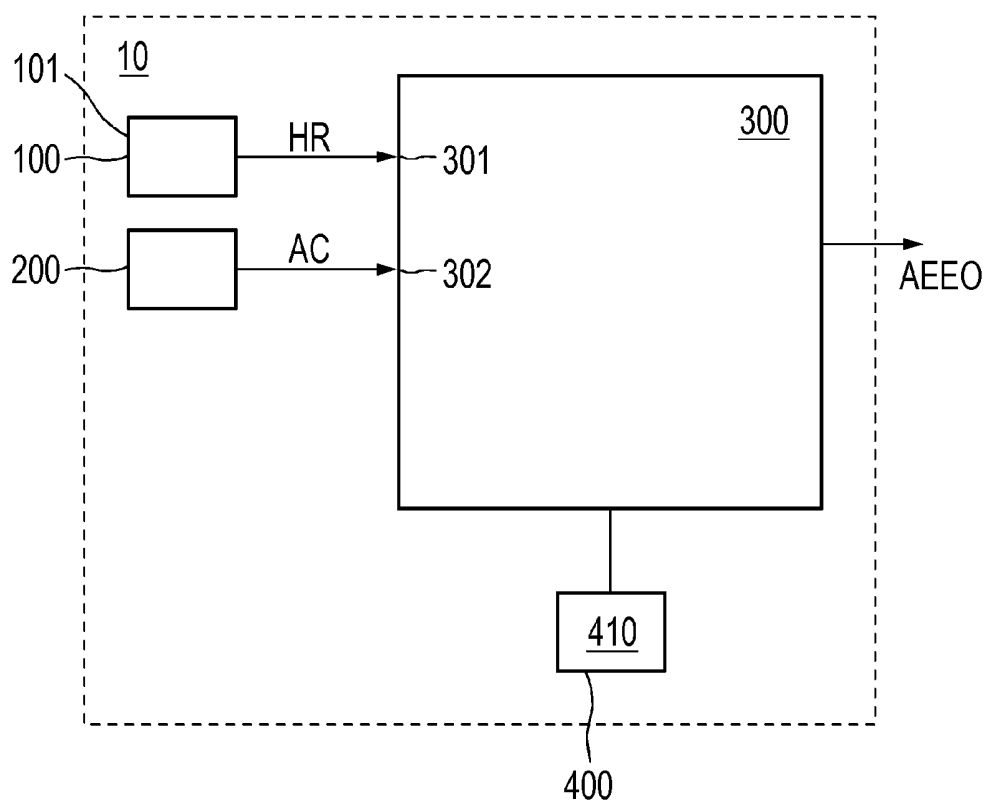


FIG. 4

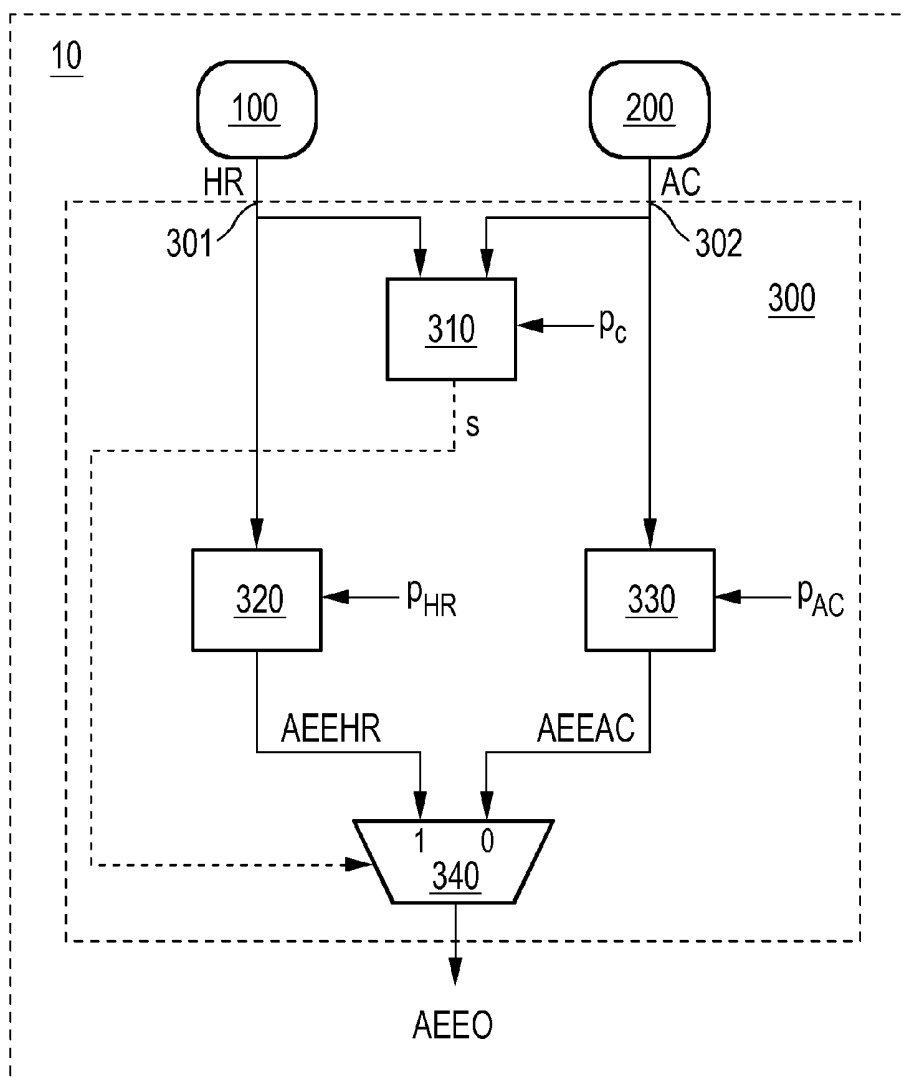


FIG. 5

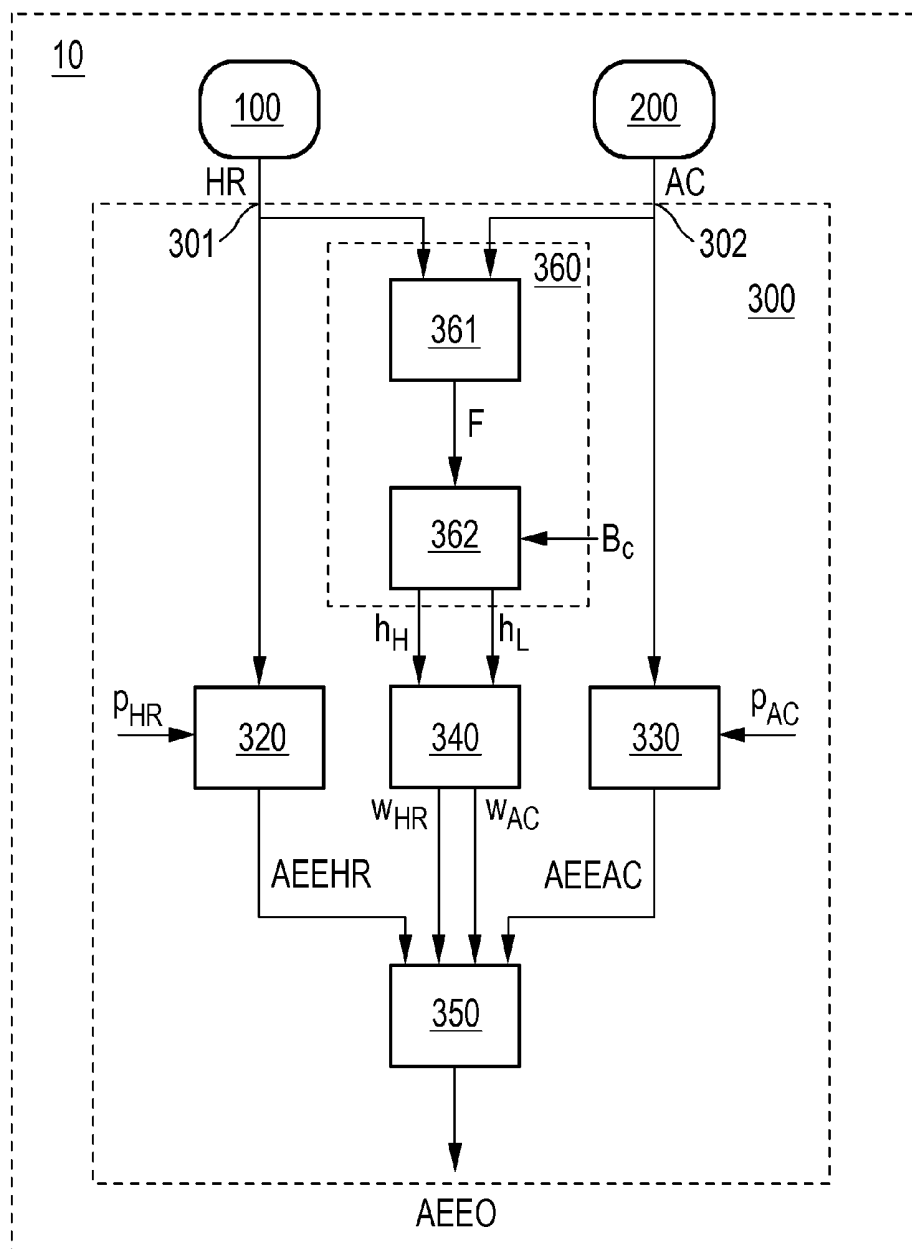


FIG. 6

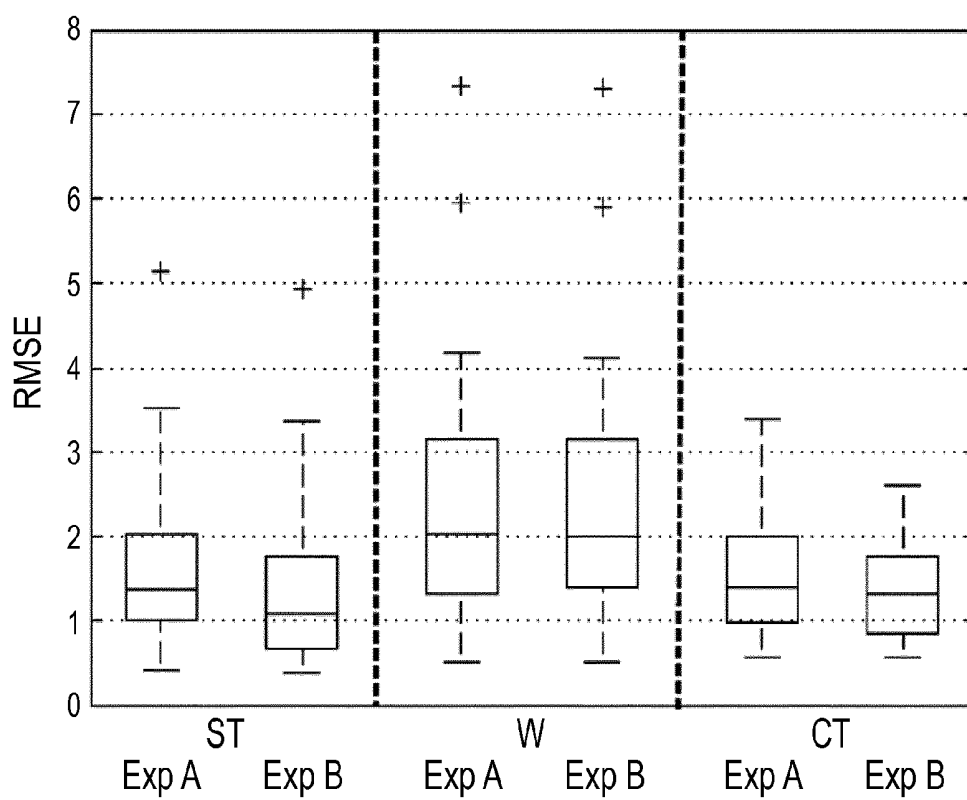


FIG. 7

VITAL SIGNS MONITORING SYSTEM

FIELD OF THE INVENTION

[0001] The invention relates to a vital signs monitoring system as well as to a method of monitoring vital signs or physiological parameters of a user.

BACKGROUND OF THE INVENTION

[0002] Heart rate sensors are well known to monitor or detect vital signs like a heart rate of a user. Such a heart rate sensor can be an optical heart rate sensor based on a photo-plethysmographic (PPG) sensor and can be used to acquire a volumetric organ measurement. By means of PPG sensors, changes in light absorption of a human skin is detected and based on these measurements a heart rate or other vital signs of a user can be determined. The PPG sensors comprise a light source like a light emitting diode (LED) which is emitting light into the skin of a user. The emitted light is scattered in the skin and is at least partially absorbed by the blood. Part of the light exits the skin and can be captured by a photodiode. The amount of light that is captured by the photo diode can be an indication of the blood volume inside the skin of a user. A PPG sensor can monitor the perfusion of blood in the dermis and subcutaneous tissue of the skin through an absorption measurement at a specific wavelength. If the blood volume is changed due to the pulsating heart, the scattered light coming back from the skin of the user is also changing. Therefore, by monitoring the detected light signal by means of the photodiode, a pulse of a user in his skin and thus the heart rate can be determined. Furthermore, compounds of the blood like oxygenated or de-oxygenated hemoglobin as well as oxygen saturation can be determined.

[0003] FIG. 1 shows a basic representation of an operational principle of a heart rate sensor. In FIG. 1, a heart rate sensor 100 is arranged on an arm of a user. The heart rate sensor 100 comprises a light source 110 and a photo detector 120. The light source 110 emits light onto or in the skin 1000 of a user. Some of the light is reflected and the reflected light can be detected by the photo detector 120. Some light can be transmitted through tissue of the user and be detected by the photo detector 120. Based on the reflected or transmitted light, vital signs of a user like a heart rate can be determined.

[0004] The results of a heart rate sensor can be used to estimate or measure a caloric Activity Energy Expenditure AEE.

[0005] FIG. 2 shows a representation of a total energy expenditure of a human being. The Total Energy Expenditure TEE is composed of a Basal Energy Expenditure BEE, a diet induced thermogenesis DIT and an Activity Energy Expenditure AEE. The Basal Energy Expenditure BEE is a combination of the sleeping metabolic rate and the energy expenditure from arousal.

[0006] If a user wants to for example reduce his weight, he must burn more calories than he is eating or drinking. The Activity Energy Expenditure AEE is that part of the Total Energy Expenditure TEE which is influenced by the activity of the person.

[0007] When a user is trying to reduce weight, it is often not easy for the user to determine how many calories he has spent throughout an activity or workout. Hence, there is a need for an accurate estimation or measurement of the energy spent during an activity.

[0008] An accurate estimation or measurement of the caloric Activity Energy Expenditure AEE is therefore an important factor for example for smart watches enabling sport and wellbeing applications.

[0009] Accordingly, it is desired to provide a monitor which can monitor the activity of a user during the day and which can measure or estimate the Activity Energy Expenditure, i.e. the energy expenditure of a user during a day.

[0010] FIG. 3 shows a graph indicating an Activity Energy Expenditure AEE prediction as a function of a measured Activity Energy Expenditure. In FIG. 3, the measured Activity Energy Expenditure MAEE is depicted at the X-axis and the predicted Activity Energy Expenditure PAEE is depicted at the Y-axis. Furthermore, in FIG. 3, several activity types like running, cycling, rowing, using a cross trainer etc. are depicted as data points. For some activities like walking, an overestimation OE (the estimated Activity Energy Expenditure AEE is too high) can be present. For other activities like cycling, rowing and using a cross trainer, an underestimation UE (the estimated Activity Energy Expenditure AEE is too low) can be present. In FIG. 3, furthermore, the optimal estimation OES is also depicted, namely the situation where the measured Activity Energy Expenditure MAEE corresponds to the predicted Activity Energy Expenditure.

[0011] The reasons why the measured and predicted Activity Energy Expenditure do not correspond to each other can be that the model based on which the predicted Activity Energy Expenditure AEE is determined is not accurate enough or the activity which the user is performing is not reflected good enough in the model.

[0012] According to FIG. 3, some activities requiring a high physical activity level may be misinterpreted or underestimated like cycling, rowing and using a cross trainer. In addition or alternatively to using heart rate data, the Activity Energy Expenditure AEE can be determined or estimated for example based on motion data of a user acquired from an acceleration sensor.

[0013] If a heart rate of a user is used to estimate the Activity Energy Expenditure AEE, it should be noted that the known linear relationship between the heart rate and the energy expenditure is only valid for aerobic activities with a moderate or vigorous exertion level. Furthermore, heart rate data which is measured for example during mental stress and fatigue may cause a biased prediction output in particular for low intensity activities. Furthermore, motion artifacts may be present in heart rate data. These motion artifacts may in particular occur during activities, which show an unpredictable thus non-repetitive movement pattern. Examples of such movements are several normal daily activities when full body motion is not represented by hand and wrist movement.

[0014] Furthermore, it should be noted that Activity Energy Expenditure AEE can be predicted quite accurately based on heart rate data during aerobic activities while acceleration and movement information are most suitable to predict Activity Energy Expenditure during sedentary, low intensity activities with a low exertion level or non-structured activities.

[0015] WO 2014/207294 A1 discloses a system for monitoring physical activity based on monitoring motion data of a user or alternatively based on a heart rate activity of a user.

[0016] EP 1 424 038 A1 discloses a device for measuring a calorie expenditure.

[0017] US 2008/0139952 A1 discloses a biometric information processing device which can display a calorie expenditure.

[0018] S. Brage. "Branched equation modeling of simultaneous accelerometry and heart rate monitoring improves estimate of directly measured physical activity energy expenditure", *Journal of Applied Physiology*, vol. 96, no. 1, 29 Aug. 2003, pages 343-351, discloses a vital signs monitoring system which computes an overall activity energy expenditure of a user. Static weight coefficients are determined offline during a training phase of a system. This is in particular performed by minimizing the root-mean-square error between a reference physical activity energy expenditure and an estimated activity energy expenditure derived from a mode with weight coefficients.

SUMMARY OF THE INVENTION

[0019] It is an object of the invention to provide a vital signs monitoring system which is able to accurately predict or measure an Activity Energy Expenditure of a user.

[0020] According to an aspect of the invention, a vital signs monitoring system is provided which comprises a processing unit configured to estimate an activity energy expenditure of a user. The processing unit comprises a first input configured to receive heart rate data HR from at least one heart rate sensor configured to measure or determine a heart rate HR of a user and a second input configured to receive motion or acceleration data AC from at least one motion sensor configured to detect motion or acceleration data AC of a user. The processing unit further comprises a first activity energy expenditure determining unit configured to determine a first activity energy expenditure based on heart rate data HR received via the first input. The processing unit further comprises a second activity energy expenditure determining unit configured to determine a second activity energy expenditure based on motion or acceleration data received via the second input. The processing unit furthermore comprises an estimation unit configured to estimate an exertion level of a user based on the current heart rate data from the at least one heart rate sensor and/or the current motion or acceleration data from the at least one motion sensor by estimating a first probability of a high exertion of a user and a second probability of a low exertion of a user. The processing unit further comprises a weighting unit configured to determine a first and second weighting factor based on a first probability relating to a high exertion level of the user and a second probability relating to a low exertion level of the user. The processing unit further comprises an activity energy expenditure calculating unit configured to compute overall activity energy expenditure based on the first activity energy expenditure weighted by the first weighting factor and on the second activity energy expenditure weighted by the second weighting factor.

[0021] According to an aspect of the invention the processing unit furthermore comprises a probability estimating unit configured for estimating a probability of a high or low exertion of a user. The weighting unit is then configured to determine the first and second weighting factor based on the probabilities of a high or low exertion level.

[0022] According to a further aspect of the invention an optical heart rate sensor in form of a photoplethysmographic sensor is configured to measure or determine a heart rate of

a user. Moreover, at least one motion or acceleration sensor is configured to determine motion or acceleration data of a user.

[0023] According to a further aspect of the invention the processing unit, the at least one heart rate sensor and the at least one motion or acceleration sensor is arranged in a wearable device or a smart watch.

[0024] According to a further aspect of the invention a method of monitoring vital signs or physiological parameters of a user is provided. Heart rate data HR from at least one heart rate sensor configured to measure or determine a heart rate HR of a user is received. Motion or acceleration data from at least one motion sensor configured to detect motion or acceleration data of a user is received. A first activity energy expenditure based on heart rate data, and a second activity energy expenditure based on motion or acceleration data are determined. A first and second weighting factor based on a first probability relating to a high exertion level of a user and a second probability relating to a low exertion level of a user are determined. Overall activity energy expenditure is computed based on the first activity energy expenditure weight by the first weighting factor and on the second activity energy expenditure weighted by the second weighting factor.

[0025] It shall be understood that a preferred embodiment of the present invention can also be a combination of the dependent claims, above embodiments or aspects with respective independent claims.

[0026] These and other aspects of the invention will be apparent from and elucidated with reference to the embodiment(s) described hereinafter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] In the following drawings:

[0028] FIG. 1 shows a basic representation of an operational principle of a vital signs monitoring system,

[0029] FIG. 2 shows a basic representation of a Total Energy Expenditure of a user,

[0030] FIG. 3 shows a graph depicting an Activity Energy Expenditure prediction as a function of measured Activity Energy Expenditure,

[0031] FIG. 4 shows a block diagram of a vital signs monitoring system according to an aspect of the invention,

[0032] FIG. 5 shows a further block diagram of a vital signs monitoring system according to an aspect of the invention,

[0033] FIG. 6 shows a block diagram of a vital signs monitoring system according to a further aspect of the invention, and

[0034] FIG. 7 shows a graph indicating an improved accuracy of a predicting Activity Energy Expenditure with a vital signs monitoring system according to an aspect of the invention.

DETAILED DESCRIPTION OF EMBODIMENTS

[0035] FIG. 4 shows a block diagram of a vital signs monitoring system according to an aspect of the invention. The vital signs monitoring system is used to monitor vital signs or physiological parameters of a user. The vital signs monitoring system 10 comprises at least one heart rate sensor 100, at least one motion sensor 200 for measuring or determining motion data or acceleration data AC of a user, a processing unit 300 such as a processor and optionally a

display 400 with a graphic user interface 410. The processing unit 300 receives heart rate data HR from the at least one heart rate sensor 100 at its first input 301 and a motion or acceleration data AC from the at least one motion sensor 200 at its second input 302. The processing unit 300 is adapted to determine or estimate an Activity Energy Expenditure AEE of a user based on the received heart rate data HR and/or the acceleration data AC. The heart rate sensor 100 can comprise a contact surface 101 which can be placed or arranged on a skin 1000 of a user to detect a heart rate of the user.

[0036] According to an aspect of the invention, an optical vital signs sensor is provided as a heart rate sensor 100 which is based on a photoplethysmographic PPG sensor. Such a PPG sensor is depicted in FIG. 1. A light source 110 emits light onto or into the skin 1000 of a user and some of the light is reflected and this reflected light can be detected by a photo detector 120. The output of the photo detector 120 can be analyzed to determine a heart rate or other vital signs of a user.

[0037] The output signal of the PPG sensor gives an indication on the blood movement in vessels of a user. The quality of the output signal of the PPG sensor can depend on the blood flow rate, skin morphology and skin temperature. In addition, optical losses in the PPG sensor may also have an influence on the quality of the output signal of the PPG sensor. The optical efficiency of the PPG sensor can depend on reflection losses when light penetrates from one media into another. Furthermore, a scattering of light at the surface of the skin of the user may also have an influence on the optical efficiency of the PPG sensor.

[0038] The PPG sensor or optical vital signs sensor according to an aspect of the invention can be implemented as a wearable device e.g. a wrist device (like a watch or smart watch). The optical vital signs sensor can also be implemented as a device worn behind the ear of a user, e.g. like a hearing aid. A wearable device is a device which can be worn or attached on a skin of a user.

[0039] The motion sensor 200 can also be implemented as a wearable device. Preferably, the motion sensor 120 and the heart rate sensor 110 are implemented in a common housing as part of a wearable device. The motion sensor 200 can be an acceleration sensor such as a piezoelectric, piezoresistive or a capacitive accelerometer.

[0040] FIG. 5 shows a further block diagram of a vital signs monitoring system according to an aspect of the invention. The vital signs monitor system 10 comprises at least one heart rate sensor 100, at least one motion or acceleration sensor 200 and a processing unit 300. The processing unit 300 receives the heart rate data HR from the at least one heart rate sensor 100 at its first input 301 as well as a acceleration or motion data AC from the acceleration sensor 200 at its second input 302. The processing unit 300 outputs a predicted or estimated Activity Energy Expenditure AEE.

[0041] The processing unit 300 can use the heart rate data HR from the at least one heart rate sensor 100 or the acceleration data AC from the acceleration sensor 200 to predict or determine an Activity Energy Expenditure AEE. In other words, the processing unit 300 can either use the heart rate data HR or the acceleration data AC. Alternatively, the processing unit 300 may also use a combination of the heart rate data HR and the acceleration data AC.

[0042] The processing unit 300 comprises an estimating unit 310 for estimating the exertion level of a person during a time interval. The estimating unit 310 receives the current heart rate data HR and the current acceleration data AC and analyzes these data. The estimation unit 310 outputs a signal *s* indicating whether the exertion level is high or low. The output signal *S* will correspond to "1" if the exertion level is estimated as high and will correspond to "0" if the exertion level is estimated as low. The estimating unit 310 has a further input for the parameter *pc*. This parameter *pc* can be used for controlling the sensitivity and specificity of the exertion level estimation performed by the estimation unit 310.

[0043] The processing unit 300 furthermore comprises a first Activity Energy Expenditure determining unit 320 which computes or estimates the Activity Energy Expenditure AEE based on the heart rate HR data from the at least one heart rate sensor 100. The first Activity Energy Expenditure determining unit 320 comprises a further input for a parameter set P_{HR} which can be used to determine the sensitivity of the first determining unit 320. The first determining unit 320 outputs an Activity Energy Expenditure AEEHR for the activity expenditure based on the heart rate data HR.

[0044] The processing unit 300 furthermore comprises a second Activity Energy Expenditure determining unit 330 which computes or determines the Activity Energy Expenditure AEE based on the acceleration data AC from the at least one acceleration sensor or motion sensor 200. The second determining unit 330 comprises an input for a parameter set P_{AC} for setting the sensitivity of the second determining unit 330. The second Activity Energy Expenditure determining unit 330 outputs an Activity Energy Expenditure AEEAC as determined based on the acceleration or motion data AC.

[0045] The processing unit 300 furthermore comprises a selecting unit 340 which selects the output of the first or second Activity Energy Expenditure determining unit 320, 330 based on the output signal *s* of the estimating unit 310. In particular, if the output signal *s* is high "1", then the output of the first Activity Energy Expenditure unit 320 is used while if the output signal is low "0", then the output of the second Activity Energy Expenditure determining unit 330 is used as output signal.

[0046] The vital signs monitoring system according to FIG. 5 has some drawbacks as a decision whether or not a high or low exertion level is present can sometimes not be accurately performed. Thus, in some cases, the decision whether or not the exertion level is high or low is prone to mistakes.

[0047] In addition, if the activity of a user is at the border between high and low exertion levels due to motion artifacts, the processing unit may switch between low and high exertion levels, thus changing the output of the processing unit and thereby the overall Activity Energy Expenditure during the physical activity such that the user may not receive an accurate and constant estimation of the activity level.

[0048] FIG. 6 shows a block diagram of a vital signs monitoring system according to a further aspect of the invention. The vital signs monitor system 10 comprises at least one heart rate sensor 100, at least one acceleration or motion sensor 200 and a processing unit 300. The heart rate sensor 100 outputs heart rate data HR and the acceleration

or motion sensor 200 outputs acceleration or motion data AC. The processing unit 300 comprises a first Activity Energy Expenditure determining unit 320 for determining the Activity Energy Expenditure AEEHR based on the heart rate data HR from the at least one heart rate sensor 100. The processing unit furthermore comprises a second Activity Energy Expenditure determining unit 330 for determining the Activity Energy Expenditure AEEAC based on the motion data or acceleration data AC from the at least one acceleration sensor 200. The processing unit 300 furthermore comprises a probability unit 360 for determining a probability of a high or low exertion based on the heart rate data HR from the at least one heart rate sensor 100 as well as based on current acceleration or motion data AC from the at least one acceleration sensor 200. In other words, the probability unit 360 serves to estimate the probability of a high exertion or a low exertion level. The probability estimating unit 360 comprises a feature set unit 361 for extracting a feature set F based on the heart rate data HR, the motion data or acceleration data AC or a combination of both. The feature set F are used as predictors for a high or low body exertion. These predictors can be an activity count, speed, number of steps, motion level etc. The motion level can be used together with cardiac features from the heart rate data.

[0049] The feature set F can be inputted into a classification unit 362. The classification unit 362 is used to classify the exertion level of a person. The classification unit 362 can receive a parameter set Be. This parameter Be can optionally be derived during a training phase. The classification unit 362 outputs a probability of the high and low exertion as a function of the feature set F. A High exertion level correspond to aerobic activities, activities having a consistent and repetitive temporal pattern, which may represent planned actions of exertion level higher than resting low exertion level consists of activities involving irregular body movement, which result in predominant anaerobic work or low intensity sedentary occupations. The classification unit 362 may also use an estimated resting heart rate, an estimated maximum heart rate, the sex, age, height and weight of the user during the classification process. Optionally, the probabilities can be defined as $h_H(F)=P(y=1|F; B_c)$ and $h_L(F)=P(y=0|F; B_c)$.

[0050] The processing unit 300 furthermore comprises a weighting unit 340 for transforming the probability estimates h_H and h_L into weighting factors wHR and wAC. The weighting factors can be between 0 and 1.

[0051] The processing unit 300 furthermore comprises an Activity Energy Expenditure calculating unit 350, which is computing or determining the overall Activity Energy Expenditure AEEO. The overall Activity Energy Expenditure AEEO is defined as: f_{WA} (wHR, wAC, AEEHR, AEEAC) such that the overall Activity Energy Expenditure $AEEO=wHR \cdot AEEHR+wAC \cdot AEEAC$. Accordingly, the overall Activity Energy Expenditure is based on a combination of the Activity Energy Expenditure determined based on the heart rate data HR as well as on the acceleration data AC with corresponding weighting factors.

[0052] According to a further aspect of the invention, instead of using two different parameters like heart rate HR and motion data AC for determining the Activity Energy Expenditure, the data of a plurality of sensors can be used to determine the Activity Energy Expenditure. The Activity Energy Expenditure AEE can be determined or estimated

based on each of the N sensors such that each i_{th} estimation unit produces an energy expenditure estimate. As in the aspect of the invention according to FIG. 6, weighting units are provided for analyzing the output signals of the sensor and optionally for incorporating supplementary subject specific information. The overall Activity Energy Expenditure AEE is then estimated by computing a weighted average of all separate energy expenditure estimates.

[0053] FIG. 7 shows a graph indicating an improved accuracy of a predicting Activity Energy Expenditure AEE with a vital signs monitoring system according to an aspect of the invention. In FIG. 7, a comparison is depicted between the aspect of the invention according to FIG. 5 and according to FIG. 6. The results as achieved by the vital signs monitor system according to FIG. 5 are depicted as Exp A while the results achieved by the vital signs monitor system according to FIG. 6 are depicted as Exp B. In particular, three different tests have been performed, namely a step test ST, a walking at 3 km/h W and using a cross trainer CT has been used.

[0054] In table 1, examples of the weighting factors wHR and wAC are depicted.

Activity type	wHR	wAC
Step Test ST	0.79	0.21
Walking 3 km/h W	0.97	0.03
Cross Trainer CT	0.83	0.17

[0055] For the walking activity W, the weighting factors of the mixture of the Activity Energy Expenditure AEEHR based on the heart rate and the Activity Energy Expenditure AEEAC based on the acceleration data AC has no limiting effect as the weighting factor for the heart rate data is approximately 1, i.e. the overall Activity Energy Expenditure corresponds to the Activity Energy Expenditure based on the heart rate data. On the other hand, for the step test T and the cross trainer CT, the weighting factor w_{HR} corresponds to 0.79 and 0.83, respectively while the weighting factor for the acceleration data corresponds to 0.21 and 0.17, respectively. Hence, the overall Activity Energy Expenditure can be calculated more accurately.

[0056] Table 2 shows the average RMSE as obtained from the two experiments described before.

	Exp A (kcal/min)	Exp B (kcal/min)
Step Test ST	1.67	1.47
Walking 3 km/h W	2.58	2.58
Cross Trainer CT	1.59	1.40

[0057] Accordingly, it can be seen that the average RMSE obtained from the second experiment has improved by 12% with respect to the first experiments. Regarding the walking exercise W, the RMSE substantially remains constant. Accordingly, the provision of the weighting factors is advantageous to estimate an exertion level.

[0058] In table 3, the standard deviations of the overall Activity Energy Expenditure AEE for the two experiments are disclosed.

	Exp A (kcal/min)	Exp B (kcal/min)
Step Test ST	1.05	0.88
Walking 3 km/h W	1.95	1.92
Cross Trainer CT	1.55	1.28

[0059] As can be seen from FIG. 3, by using the vital signs monitoring system according to FIG. 6, it is possible to reduce the variability in the overall Activity Energy Expenditure AEE. For the walking exercise W, the variation of the overall Activity Energy Expenditure remains substantially unchanged.

[0060] According to an aspect of the invention, a computer program product is provided which comprises: a computer readable memory storing computer program code means for causing the vital signs monitor system to carry out steps of the monitoring vital signs or physiological parameters of a user.

[0061] Other variations of the disclosed embodiment can be understood and effected by those skilled in the art in practicing the claimed invention from a study of the drawings, the disclosure and the appended claims.

[0062] In the claims, the word “comprising” does not exclude other elements or steps and in the indefinite article “a” or “an” does not exclude a plurality.

[0063] A single unit or device may fulfill the functions of several items recited in the claims. The mere fact that certain measures are recited in mutual different dependent claims does not indicate that a combination of these measurements cannot be used to advantage. A computer program may be stored/distributed on a suitable medium such as an optical storage medium or a solid state medium, supplied together with or as a part of other hardware, but may also be distributed in other forms such as via the internet or other wired or wireless telecommunication systems.

[0064] Any reference signs in the claims should not be construed as limiting the scope.

1. A vital signs monitoring system, comprising a processing unit configured to estimate an activity energy expenditure of a user, said processing unit comprises:

- a first input interface configured to receive heart rate data from at least one heart sensor configured to measure or determine a heart rate of a user,
- a second input interface configured to receive motion or acceleration data from at least one motion sensor configured to detect motion or acceleration data of a user,
- a first activity energy expenditure determining unit configured to determine a first activity energy expenditure based on heart rate data received via the first input interface,
- a second activity energy expenditure determining unit configured to determine a second activity energy expenditure based on motion or acceleration data received via the second input interface, characterized by
- a probability estimating unit configured to calculate a first probability of a high exertion of a user and a second probability of a low exertion of the user, wherein the probability estimating unit comprises
 - a feature set unit configured to extract a feature set based on at least one of the heart rate data and/or the motion or acceleration data, wherein the feature set serve as predictors of a high or low exertion,

- a classification unit configured to classify an exertion level and to output the first probability and the second probability as a function of the feature set,

- a weighing unit configured to determine a first weighting factor and a second weighting factor based on the first and the second probability, and

- an activity energy expenditure calculating unit configured to compute an overall activity energy expenditure based on the at least one first activity energy expenditure weighted by the first weighting factor and on the at least one second activity energy expenditure weighted by the second weighting factor.

2. The vital signs monitoring system according to claim 1, further comprising a heart rate sensor in form of a photoplethysmographic sensor configured to measure or determine a heart rate of a user, and at least one motion or acceleration sensor configured to determine motion or acceleration data of a user.

3. A wearable device, comprising:

- a heart rate sensor;

- a motion sensor; and

- a processing unit comprising:

- a first input interface configured to receive heart rate data from the heart rate sensor

- a second input interface configured to receive motion or acceleration data from the motion sensor;

- a first activity energy expenditure determining unit configured to determine a first activity energy expenditure based on heart rate data received via the first input interface,

- a second activity energy expenditure determining unit configured to determine a second activity energy expenditure based on motion or acceleration data received via the second input interface;

- a probability unit configured to calculate a first probability of a high exertion of a user and a second probability of a low exertion of the user, wherein the probability unit comprises:

- a feature set unit configured to extract a feature set based on at least one of the heart rate data and motion or acceleration data wherein the feature set serves as predictors of a high or low exertion; and

- a classification unit configured to classify an exertion level and to output the first probability and the second probability as a function of the feature set;

- a weighing unit configured to determine a first weighting factor and a second weighting factor based on the first probability and the second probability; and

- an activity energy expenditure calculating unit configured to compute an overall activity energy expenditure based on the at least one first activity energy expenditure weighted by the first weighting factor and on the at least one second activity energy expenditure weighted by the second weighting factor.

4. A method of monitoring vital signs or physiological parameters of a user, comprising the steps of:

- receiving heart rate data from at least one heart rate sensor configured to measure or determine a heart rate of a user,

- receiving motion or acceleration data from at least one motion sensor configured to detect motion or acceleration data of a user,

- determining a first activity energy expenditure based on the received heart rate data,

determining a second activity energy expenditure based on the received motion or acceleration data, characterized by

calculating a first probability of a high exertion of a user and a second probability of a low exertion of the user, extracting a feature set based on at least one of the heart rate data and the motion or acceleration data, wherein the feature set serve as predictors of a high or low exertion.

classifying an exertion level and outputting the first and second probability as a function of the feature set, determining a first and second weighting factor based on the first probability and the second probability, and computing an overall activity energy expenditure based on the first activity energy expenditure weighted by the first weighting factor and on the second activity energy expenditure weighted by the second weighting factor.

5. A non-transitory computer program product comprising computer program code instructions that, when executed, perform the steps of,

Receiving heart rate data from at least one heart rate sensor configured to measure or determine a heart rate of a user,

receiving motion or acceleration data from at least one motion sensor configured to detect motion or acceleration data of a user;

determining a first activity energy expenditure based on the received heart rate data;

determining a second activity energy expenditure based on the received motion or acceleration data;

calculating a first probability of a high exertion of a user and a second probability of a low exertion of the user;

extracting a feature set based on at least one of the heart rate data and the motion or acceleration data, wherein the feature set serve as predictors of a high or low exertion;

classifying an exertion level and outputting the first and second probability as a function of the feature set;

determining a first and second weighting factor based on the first probability and the second probability; and

computing an overall activity energy expenditure based on the first activity energy expenditure weighted by the first weighting factor and on the second activity energy expenditure weighted by the second weighting factor.

* * * * *

专利名称(译)	生命体征监测系统		
公开(公告)号	US20180078202A1	公开(公告)日	2018-03-22
申请号	US15/564593	申请日	2016-04-08
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	DEGROOT KOEN THEO JOHAN BONOMI ALBERTO GIOVANNI		
发明人	DEGROOT, KOEN THEO JOHAN BONOMI, ALBERTO GIOVANNI		
IPC分类号	A61B5/00 A61B5/0205		
CPC分类号	A61B5/4866 A61B5/0205 A61B5/681 A61B5/02416 A61B5/1118 A61B2562/0219		
优先权	2015162997 2015-04-09 EP		
其他公开文献	US10624580		
外部链接	Espacenet USPTO		

摘要(译)

甲生命体征监测系统包括处理单元 (的 300 的) , 用于确定第一估计活动能量消耗 (AEE) , 第一活动能量消耗确定单元 (的 320 的) 活性能量消耗 (AEEHR) 的基础上心脏速率数据 (HR) , 第二活动能量消耗确定单元 (的 330 的) 用于确定第二活性能量消耗 (AEEAC) 基于运动数据 (AC) , 和加权单元 (的 340 的) , 用于确定基于与一个高消耗 (HH) 的第一和第二概率的第一和第二加权因子 (WHR , WAC) 以及与较低的尽力 (HL) , 以及活性能量消耗计算单元 (的 350 的) 用于基于由所述第一加权因子 (WHR) 和对加权的第一活动能量消耗 (AEEHR) 的总活性能量消耗 (AEEO) 第二活动能量消耗 (AEEAC) 由第二加权因子 (wAC) 加权。

