



US010058668B2

(12) **United States Patent**  
**Wondka et al.**

(10) **Patent No.:** **US 10,058,668 B2**  
(45) **Date of Patent:** **Aug. 28, 2018**

(54) **METHODS AND DEVICES FOR SENSING RESPIRATION AND PROVIDING VENTILATION THERAPY**

(58) **Field of Classification Search**  
CPC .. A61M 2016/0015; A61M 2016/0018; A61M 2016/0021; A61M 2016/0027;  
(Continued)

(71) Applicant: **BREATHE TECHNOLOGIES, INC.**, Irvine, CA (US)

(56) **References Cited**

(72) Inventors: **Anthony Wondka**, Thousand Oaks, CA (US); **Gregory Kapust**, San Ramon, CA (US); **Robert Bryan**, San Ramon, CA (US); **Michael Khenansho**, Modesto, CA (US)

U.S. PATENT DOCUMENTS

50,641 A 10/1865 Stone  
428,592 A 5/1890 Chapman  
(Continued)

(73) Assignee: **Breathe Technologies, Inc.**, Irvine, CA (US)

FOREIGN PATENT DOCUMENTS

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1158 days.

CA 2535450 2/2005  
CN 1750854 3/2006  
(Continued)

(21) Appl. No.: **14/221,210**

OTHER PUBLICATIONS

(22) Filed: **Mar. 20, 2014**

Machine translation of EP 1820527 A1.\*  
(Continued)

(65) **Prior Publication Data**  
US 2014/0288456 A1 Sep. 25, 2014

*Primary Examiner* — Jackie Tan-Uyen T Ho  
*Assistant Examiner* — Joseph D Boecker  
(74) *Attorney, Agent, or Firm* — Stetina Brunda Garred & Brucker

**Related U.S. Application Data**


(62) Division of application No. 12/153,423, filed on May 19, 2008, now abandoned.  
(Continued)

(51) **Int. Cl.**  
**A61M 16/04** (2006.01)  
**A61B 5/00** (2006.01)  
(Continued)

(57) **ABSTRACT**  
Methods and systems are provided for intra-airway breath sensors where intra-airway breath sensors are not located within a ventilation gas delivery circuit, but are exposed to spontaneous respiration airflow from a patient. Furthermore, methods and systems of the present invention may be used to protect an intra-airway breath sensor from contacting tissue or accumulating debris that may impair abilities of the intra-airway breath sensors.

(52) **U.S. Cl.**  
CPC ..... **A61M 16/0427** (2014.02); **A61B 5/082** (2013.01); **A61B 5/085** (2013.01);  
(Continued)

**19 Claims, 15 Drawing Sheets**

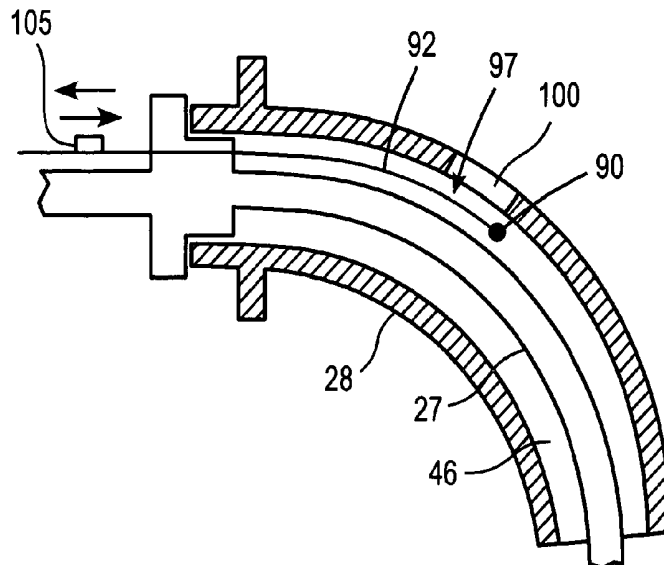

<b>Related U.S. Application Data</b>					
		3,460,533	A	8/1969	Riu Pla
		3,493,703	A	2/1970	Finan
		3,513,844	A	5/1970	Smith
(60)	Provisional application No. 60/924,514, filed on May 18, 2007.	3,610,247	A	10/1971	Jackson
		3,625,206	A	12/1971	Charnley
		3,625,207	A	12/1971	Agnew
(51)	<b>Int. Cl.</b>	3,631,438	A	12/1971	Lewin
	<i>A61B 5/08</i> (2006.01)	3,642,660	A	2/1972	Hudson et al.
	<i>A61B 5/085</i> (2006.01)	3,657,740	A	4/1972	Cialone
	<i>A61B 5/087</i> (2006.01)	3,682,171	A	8/1972	Dali et al.
	<i>A61B 5/097</i> (2006.01)	3,721,233	A	3/1973	Montgomery et al.
	<i>A61M 16/00</i> (2006.01)	3,726,275	A	4/1973	Jackson et al.
	<i>A61M 16/10</i> (2006.01)	3,727,606	A	4/1973	Sielaff
		3,733,008	A	5/1973	Churchill et al.
(52)	<b>U.S. Cl.</b>	3,741,208	A	6/1973	Jonsson et al.
	CPC .....	3,754,552	A	8/1973	King
	<i>A61B 5/0873</i> (2013.01); <i>A61B 5/0878</i> (2013.01); <i>A61B 5/097</i> (2013.01); <i>A61B 5/6853</i> (2013.01); <i>A61B 5/6858</i> (2013.01); <i>A61M 16/0003</i> (2014.02); <i>A61M 16/042</i> (2014.02); <i>A61M 16/0434</i> (2013.01); <i>A61M 16/0465</i> (2013.01); <i>A61M 16/0475</i> (2014.02); <i>A61M 16/0486</i> (2014.02); <i>A61M 2016/003</i> (2013.01); <i>A61M 2016/0021</i> (2013.01); <i>A61M 2016/0027</i> (2013.01); <i>A61M 2016/0036</i> (2013.01); <i>A61M 2016/102</i> (2013.01); <i>A61M 2205/332</i> (2013.01); <i>A61M 2205/3306</i> (2013.01); <i>A61M 2205/3375</i> (2013.01); <i>A61M 2230/43</i> (2013.01); <i>A61M 2230/65</i> (2013.01)	3,794,026	A	2/1974	Jacobs
		3,794,072	A	2/1974	Diedrich et al.
		3,802,431	A	4/1974	Farr
		3,831,596	A	8/1974	Cavallo
		3,881,480	A	5/1975	Lafourcade
		3,896,800	A	7/1975	Cibulka
		3,903,881	A	9/1975	Weigl
		3,905,362	A	9/1975	Eyrick et al.
		3,949,749	A	4/1976	Stewart
		3,951,143	A	4/1976	Kitrilakis et al.
		3,961,627	A	6/1976	Ernst et al.
		3,972,327	A	8/1976	Ernst et al.
		3,985,131	A	10/1976	Buck et al.
		3,991,790	A	11/1976	Russell
		4,003,377	A	1/1977	Dahl
		4,036,253	A	7/1977	Fegan et al.
(58)	<b>Field of Classification Search</b>	4,054,133	A	10/1977	Myers
	CPC ....	4,067,328	A	1/1978	Manley
	<i>A61M 2016/003</i> ; <i>A61M 2016/0033</i> ; <i>A61M 2016/0036</i> ; <i>A61M 16/0003</i> ; <i>A61M 16/04</i> ; <i>A61M 16/0402</i> ; <i>A61M 16/042</i> ; <i>A61M 16/0427</i> ; <i>A61M 16/0463</i> ; <i>A61M 16/0434</i> ; <i>A61M 16/0465</i> ; <i>A61M 16/0475</i> ; <i>A61M 16/0486</i> ; <i>A61M 2205/3306</i> ; <i>A61M 2205/332</i> ; <i>A61M 2205/3344</i> ; <i>A61M 2205/3375</i> ; <i>A61M 2230/43</i> ; <i>A61M 2230/65</i> ; <i>A61M 16/00</i> ; <i>A61M 16/0057</i> ; <i>A61B 5/087</i> ; <i>A61B 5/097</i>	4,106,505	A	8/1978	Salter et al.
		4,146,885	A	3/1979	Lawson, Jr.
		4,206,754	A	6/1980	Cox et al.
		4,211,086	A	7/1980	Leonard et al.
		4,216,769	A	8/1980	Grimes
		4,231,363	A	11/1980	Grimes
		4,231,365	A	11/1980	Scarberry
		4,256,101	A	3/1981	Ellestad
		4,261,355	A	4/1981	Glazner
		4,263,908	A	4/1981	Mizerak
		4,265,237	A	5/1981	Schwanbom et al.
	USPC .....	4,266,540	A	5/1981	Panzik et al.
	128/204.23, 207.14, DIG. 26; 600/532, 600/533, 537, 538, 120–125	4,270,530	A	6/1981	Baum .....
	See application file for complete search history.				<i>A61M 16/04</i> 128/204.25
		4,273,124	A	6/1981	Zimmerman
(56)	<b>References Cited</b>	4,274,162	A	6/1981	Joy et al.
	<b>U.S. PATENT DOCUMENTS</b>	4,278,082	A	7/1981	Blackmer
		4,282,869	A	8/1981	Zidulka
		4,306,567	A	12/1981	Krasner
		4,323,064	A	4/1982	Hoenic et al.
	697,181 A	4,354,488	A	10/1982	Bartos
	718,785 A	4,365,636	A	12/1982	Barker
	853,439 A	4,367,735	A	1/1983	Dali
	859,156 A	4,377,162	A	3/1983	Staver
	909,002 A	4,393,869	A	7/1983	Boyarsky et al.
	1,125,542 A	4,406,283	A	9/1983	Bir
	1,129,619 A	4,411,267	A	10/1983	Heyman
	1,331,297 A	4,413,514	A	11/1983	Bowman
	2,178,800 A	4,421,113	A	12/1983	Gedeon et al.
	2,259,817 A	4,422,456	A	12/1983	Tiep
	2,552,595 A	4,449,523	A	5/1984	Szachowicz et al.
	2,663,297 A	4,454,880	A	6/1984	Muto et al.
	2,693,800 A	4,462,398	A	7/1984	Durkan et al.
	2,735,432 A	4,469,097	A	9/1984	Kelman
	2,792,000 A	4,481,944	A	11/1984	Bunnell
	2,843,122 A	4,488,548	A	12/1984	Agdanowski
	2,859,748 A	4,495,946	A	1/1985	Lemer
	2,931,358 A	4,506,666	A	3/1985	Durkan
	2,947,938 A	4,506,667	A	3/1985	Ansite
	3,172,407 A	4,519,387	A	5/1985	Durkan et al.
	3,267,935 A	4,520,812	A	6/1985	Freitag et al.
	3,319,627 A	4,527,557	A	7/1985	DeVries et al.
	3,357,424 A	4,535,766	A	8/1985	Baum et al.
	3,357,427 A	4,537,188	A	8/1985	Phuc
	3,357,428 A	4,539,984	A	9/1985	Kiszal et al.
	3,437,274 A				

(56)	<b>References Cited</b>	5,058,580 A	10/1991	Hazard	
		5,074,299 A	12/1991	Dietz	
	U.S. PATENT DOCUMENTS	5,076,267 A	12/1991	Pastemack	
		5,080,107 A *	1/1992	Teves .....	A61B 7/023 128/207.15
4,548,590 A	10/1985 Green				
4,559,940 A	12/1985 McGinnis	5,090,408 A	2/1992	Spofford et al.	
4,567,888 A	2/1986 Robert	5,097,827 A	3/1992	Izumi	
4,570,631 A	2/1986 Durkan	5,099,836 A	3/1992	Rowland et al.	
4,571,741 A	2/1986 Guillaumot	5,099,837 A	3/1992	Russel, Sr. et al.	
4,584,996 A	4/1986 Blum	5,101,820 A	4/1992	Christopher	
4,590,951 A	5/1986 O'Connor	5,103,815 A	4/1992	Siegel et al.	
4,592,349 A	6/1986 Bird	5,105,807 A	4/1992	Kahn et al.	
4,621,632 A	11/1986 Bartels et al.	5,107,830 A	4/1992	Younes	
4,630,606 A	12/1986 Weerda et al.	5,107,831 A	4/1992	Halpern et al.	
4,630,614 A	12/1986 Atlas	5,113,857 A	5/1992	Dickerman et al.	
4,644,947 A	2/1987 Whitwam et al.	5,117,818 A	6/1992	Palfy	
4,648,395 A	3/1987 Sato et al.	5,117,819 A	6/1992	Servidio et al.	
4,648,398 A	3/1987 Agdanowski et al.	5,127,400 A	7/1992	DeVries et al.	
4,658,832 A	4/1987 Brugnoli	5,134,995 A	8/1992	Gruenke et al.	
4,660,555 A	4/1987 Payton	5,134,996 A	8/1992	Bell	
4,682,591 A	7/1987 Jones	5,140,045 A	8/1992	Askanazi et al.	
4,684,398 A	8/1987 Dunbar et al.	5,148,802 A	9/1992	Sanders et al.	
4,686,974 A	8/1987 Sato et al.	5,161,525 A	11/1992	Kimm et al.	
4,686,975 A	8/1987 Naimon et al.	5,165,397 A	11/1992	Arp	
4,688,961 A	8/1987 Shioda et al.	5,181,509 A	1/1993	Spofford et al.	
4,705,034 A	11/1987 Perkins	5,184,610 A	2/1993	Marten et al.	
4,744,356 A	5/1988 Greenwood	5,186,167 A	2/1993	Kolobow	
4,747,403 A	5/1988 Gluck et al.	5,193,532 A	3/1993	Moa et al.	
4,753,233 A	6/1988 Grimes	5,193,533 A	3/1993	Body et al.	
4,773,411 A	9/1988 Downs	5,199,424 A	4/1993	Sullivan et al.	
4,776,333 A	10/1988 Miyamae	5,211,170 A	5/1993	Press	
4,782,832 A	11/1988 Trimble et al.	5,217,008 A	6/1993	Lindholm	
4,784,130 A	11/1988 Kenyon et al.	5,233,978 A	8/1993	Callaway	
4,803,981 A	2/1989 Vickery	5,233,979 A	8/1993	Strickland	
4,807,616 A	2/1989 Adahan	5,239,994 A	8/1993	Atkins	
4,807,617 A	2/1989 Nesti	5,239,995 A	8/1993	Estes et al.	
4,808,160 A	2/1989 Timmons et al.	5,243,972 A	9/1993	Huang	
4,813,431 A	3/1989 Brown	5,245,995 A	9/1993	Sullivan et al.	
4,817,897 A	4/1989 Kreusel	5,255,675 A	10/1993	Kolobow	
4,818,320 A	4/1989 Weichselbaum	5,258,027 A	11/1993	Berghaus	
4,823,788 A	4/1989 Smith et al.	5,269,296 A	12/1993	Landis	
4,825,859 A	5/1989 Lambert	5,271,388 A	12/1993	Whitwam et al.	
4,827,922 A	5/1989 Champain et al.	5,271,391 A	12/1993	Graves	
4,832,014 A	5/1989 Perkins	5,275,159 A	1/1994	Griebel	
4,838,255 A	6/1989 Lambert	5,279,288 A	1/1994	Christopher	
4,841,953 A	6/1989 Dodrill	5,287,852 A	2/1994	Arkininstall	
4,848,333 A	7/1989 Waite	5,291,882 A	3/1994	Makhoul	
4,850,350 A	7/1989 Jackson	5,303,698 A	4/1994	Tobia et al.	
4,865,586 A	9/1989 Hedberg	5,303,700 A	4/1994	Weismann et al.	
4,869,718 A	9/1989 Brader	5,318,019 A	6/1994	Celaya	
4,899,740 A	2/1990 Napolitano	5,331,995 A	7/1994	Westfall et al.	
4,905,688 A	3/1990 Vicenzi et al.	5,335,656 A	8/1994	Bowe et al.	
4,915,103 A	4/1990 Visveshwara et al.	5,339,809 A	8/1994	Beck, Jr. et al.	
4,915,105 A	4/1990 Lee	5,349,946 A	9/1994	McComb	
4,919,128 A	4/1990 Kopala et al.	5,367,292 A	11/1994	Szoke	
4,919,132 A	4/1990 Miser	5,368,017 A	11/1994	Sorenson et al.	
4,938,212 A	7/1990 Snook et al.	5,370,112 A	12/1994	Perkins	
4,944,310 A	7/1990 Sullivan	5,373,842 A	12/1994	Olsson et al.	
4,967,743 A	11/1990 Lambert	5,375,593 A	12/1994	Press	
4,971,049 A	11/1990 Rotariu et al.	5,388,575 A	2/1995	Taube	
4,982,735 A	1/1991 Yagata et al.	5,394,870 A	3/1995	Johansson	
4,986,269 A	1/1991 Hakkinen	5,398,676 A	3/1995	Press et al.	
4,989,599 A	2/1991 Carter	5,398,682 A	3/1995	Lynn	
4,990,157 A	2/1991 Roberts et al.	5,400,778 A	3/1995	Jonson et al.	
5,000,175 A	3/1991 Pue	5,419,314 A	5/1995	Christopher	
5,002,050 A	3/1991 McGinnis	5,421,325 A *	6/1995	Cinberg .....	A61M 16/04 128/200.26
5,005,570 A	4/1991 Perkins				
5,018,519 A	5/1991 Brown	5,438,979 A	8/1995	Johnson, Jr. et al.	
5,022,394 A	6/1991 Chmielinski	5,438,980 A	8/1995	Phillips	
5,024,219 A	6/1991 Dietz	5,443,075 A	8/1995	Holscher	
5,025,805 A	6/1991 Nutter	5,460,174 A	10/1995	Chang	
5,038,771 A	8/1991 Dietz	5,460,613 A	10/1995	Ulrich et al.	
5,042,478 A	8/1991 Kopala et al.	5,474,062 A	12/1995	DeVires et al.	
5,046,491 A	9/1991 Derrick	5,477,852 A	12/1995	Landis et al.	
5,046,492 A	9/1991 Stackhouse et al.	5,485,850 A	1/1996	Dietz	
5,048,515 A	9/1991 Sanso	5,490,502 A	2/1996	Rapoport et al.	
5,048,516 A	9/1991 Soderberg	5,503,146 A	4/1996	Froehlich et al.	
5,052,400 A	10/1991 Dietz	5,503,497 A	4/1996	Dudley et al.	
5,054,484 A	10/1991 Hebel, Jr.	5,507,282 A	4/1996	Younes et al.	

(56)		References Cited					
		U.S. PATENT DOCUMENTS					
5,509,409	A	4/1996	Weatherholt	5,937,855	A	8/1999	Zdrojkowski et al.
5,513,628	A	5/1996	Coles et al.	5,938,118	A	8/1999	Cooper
5,513,631	A	5/1996	McWilliams	5,954,050	A	9/1999	Christopher
5,513,635	A	5/1996	Bedi	5,957,136	A	9/1999	Magidson et al.
5,522,382	A	6/1996	Sullivan et al.	5,964,223	A	10/1999	Baran
5,526,806	A	6/1996	Sansoni	5,975,077	A	11/1999	Hofstetter et al.
5,529,060	A	6/1996	Salmon et al.	5,975,081	A	11/1999	Hood et al.
5,533,506	A	7/1996	Wood	5,979,440	A	11/1999	Honkonen et al.
5,535,738	A	7/1996	Estes et al.	5,989,193	A	11/1999	Sullivan
5,537,997	A	7/1996	Mechlenburg et al.	6,000,396	A	12/1999	Melker et al.
5,538,002	A	7/1996	Boussignac et al.	6,019,101	A	2/2000	Cotner et al.
5,542,415	A	8/1996	Brody	6,039,696	A	3/2000	Bell
5,546,935	A *	8/1996	Champeau .....	6,050,260	A	4/2000	Daniell et al.
			A61M 16/04	6,076,519	A	6/2000	Johnson
			128/204.23	6,085,747	A	7/2000	Axe et al.
5,549,106	A	8/1996	Gruenke et al.	6,091,973	A	7/2000	Colla et al.
5,551,419	A	9/1996	Froehlich et al.	6,105,575	A	8/2000	Estes et al.
5,558,086	A	9/1996	Smith et al.	6,109,264	A	8/2000	Sauer
5,564,416	A	10/1996	Jones	6,112,746	A	9/2000	Kwok et al.
5,575,282	A	11/1996	Knoch et al.	6,119,694	A	9/2000	Correa et al.
5,582,164	A	12/1996	Sanders	6,120,460	A	9/2000	Abreu
5,593,143	A	1/1997	Ferrarin	6,123,668	A	9/2000	Abreu
5,595,174	A	1/1997	Gwaltney	6,131,571	A	10/2000	Lamptang et al.
5,598,837	A	2/1997	Sirianne, Jr. et al.	6,135,970	A	10/2000	Kadhiresan et al.
5,598,840	A	2/1997	Lund et al.	6,152,132	A	11/2000	Psaros
5,603,315	A	2/1997	Sasso, Jr.	6,152,134	A	11/2000	Webber et al.
5,605,148	A	2/1997	Jones	6,158,432	A	12/2000	Biondi et al.
5,626,131	A	5/1997	Chua et al.	6,192,883	B1	2/2001	Miller, Jr.
5,632,269	A	5/1997	Zdrojkowski	6,203,502	B1	3/2001	Hilgendorf et al.
5,636,630	A	6/1997	Miller et al.	6,213,119	B1	4/2001	Brydon et al.
5,645,053	A	7/1997	Remmers et al.	6,213,955	B1	4/2001	Karakasoglu et al.
5,645,054	A	7/1997	Cotner et al.	6,220,244	B1	4/2001	McLaughlin
5,647,351	A	7/1997	Weismann et al.	6,224,560	B1	5/2001	Gazula et al.
5,669,377	A	9/1997	Fenn	6,227,200	B1	5/2001	Crump et al.
5,669,380	A	9/1997	Garry et al.	6,247,470	B1	6/2001	Ketchedjian
5,676,132	A	10/1997	Tillotson et al.	6,269,811	B1	8/2001	Duff et al.
5,676,135	A	10/1997	McClellan	6,269,812	B1	8/2001	Wallace et al.
5,682,878	A	11/1997	Ogden	6,273,589	B1	8/2001	Remmers et al.
5,682,881	A	11/1997	Winthrop et al.	6,286,508	B1	9/2001	Remmers et al.
5,687,713	A	11/1997	Bahr et al.	D449,376	S	10/2001	McDonald et al.
5,687,714	A	11/1997	Kolobow et al.	D449,883	S	10/2001	McDonald et al.
5,687,715	A	11/1997	Landis et al.	6,298,850	B1	10/2001	Argraves
5,690,097	A	11/1997	Howard et al.	6,305,374	B1	10/2001	Zdrojkowski et al.
5,692,497	A	12/1997	Schnitzer et al.	6,314,957	B1	11/2001	Boissin et al.
5,697,364	A	12/1997	Chua et al.	6,315,739	B1	11/2001	Merilainen et al.
5,704,345	A	1/1998	Berthon-Jones	D451,598	S	12/2001	McDonald et al.
5,711,296	A	1/1998	Kolobow	6,328,038	B1	12/2001	Kessler et al.
5,715,812	A	2/1998	Deighan et al.	6,328,753	B1	12/2001	Zammit
5,715,815	A	2/1998	Lorenzen et al.	6,332,463	B1	12/2001	Farrugia et al.
5,720,278	A	2/1998	Lachmann et al.	6,345,619	B1	2/2002	Finn
5,735,268	A	4/1998	Chua et al.	6,349,720	B1 *	2/2002	Clark .....
5,735,272	A	4/1998	Dillon et al.				A61M 16/04
5,740,796	A	4/1998	Skog	6,357,438	B1	3/2002	128/200.26
5,752,511	A	5/1998	Simmons et al.	6,357,440	B1	3/2002	Hansen
5,762,638	A	6/1998	Shikani et al.	6,360,741	B2	3/2002	Hansen et al.
5,791,337	A	8/1998	Coles et al.	6,360,745	B1	3/2002	Truschel
5,819,723	A	10/1998	Joseph	6,363,933	B1	3/2002	Wallace et al.
5,826,579	A	10/1998	Remmers et al.	6,367,474	B1	4/2002	Berthon-Jones
5,845,636	A	12/1998	Gruenke et al.	6,369,838	B1	4/2002	Berthon-Jones et al.
5,865,173	A	2/1999	Froehlich	6,371,114	B1	4/2002	Wallace et al.
5,865,174	A	2/1999	Kloppel	6,378,520	B1	4/2002	Schmidt et al.
5,881,723	A	3/1999	Wallace et al.	6,390,091	B1	4/2002	Davenport
5,904,648	A	5/1999	Amdt et al.	6,394,088	B1	5/2002	Banner et al.
5,906,204	A	5/1999	Beran et al.	6,398,739	B1	5/2002	Frye et al.
5,911,756	A	6/1999	Debry	6,418,928	B1	6/2002	Sullivan et al.
5,915,379	A	6/1999	Wallace et al.	6,422,240	B1	7/2002	Bordewick et al.
5,915,381	A	6/1999	Nord	6,423,001	B1	7/2002	Levitsky et al.
5,918,597	A	7/1999	Jones et al.	6,427,690	B1	7/2002	Abreu
5,921,238	A	7/1999	Bourdon	6,431,172	B1	8/2002	McCombs et al.
5,921,942	A	7/1999	Remmers et al.	6,439,228	B1	8/2002	Bordewick
5,921,952	A	7/1999	Desmond, III et al.	6,439,229	B1	8/2002	Hete et al.
5,927,276	A	7/1999	Rodriguez	6,439,234	B1	8/2002	Du et al.
5,928,189	A	7/1999	Phillips et al.	6,439,235	B1	8/2002	Curti et al.
5,931,160	A	8/1999	Gilmore et al.	6,450,164	B1	8/2002	Larquet et al.
5,931,162	A	8/1999	Christian	6,450,166	B1	9/2002	Banner et al.
5,937,853	A	8/1999	Strom	6,450,166	B1	9/2002	McDonald et al.
				6,457,472	B1	10/2002	Schwartz et al.
				6,467,477	B1	10/2002	Frank et al.
				6,478,026	B1	11/2002	Wood
				6,494,202	B2	12/2002	Farmer

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,494,206	B1	12/2002	Bergamaschi et al.	6,758,217	B1	7/2004	Younes et al.
6,505,623	B1	1/2003	Hansen	6,761,172	B2	7/2004	Boussignac
6,505,624	B1	1/2003	Campbell, Sr.	6,763,832	B1	7/2004	Kirsch et al.
6,516,801	B2	2/2003	Boussignac	6,769,432	B1	8/2004	Keifer
6,520,176	B1	2/2003	Dubois et al.	6,776,162	B2	8/2004	Wood
6,520,183	B2	2/2003	Amar	6,776,163	B2	8/2004	Dougill et al.
6,668,829	B2	2/2003	Biondi et al.	6,789,539	B2	9/2004	Martinez
6,530,373	B1	3/2003	Patron et al.	6,796,305	B1	9/2004	Banner et al.
6,532,958	B1	3/2003	Buan et al.	6,799,575	B1	10/2004	Carter
6,532,960	B1	3/2003	Yurko	6,805,126	B2	10/2004	Dutkiewicz
6,536,432	B2	3/2003	Truschel	6,807,966	B2	10/2004	Wright
6,536,436	B1	3/2003	McGlothen	6,807,967	B2	10/2004	Wood
6,550,478	B2	4/2003	Remmers et al.	6,810,876	B2	11/2004	Berthon-Jones
6,553,992	B1	4/2003	Berthon-Jones et al.	6,814,073	B2	11/2004	Wickham
6,561,188	B1	5/2003	Ellis	6,814,077	B1	11/2004	Eistert
6,561,193	B1	5/2003	Noble	6,827,340	B2	12/2004	Austin et al.
6,564,797	B1	5/2003	Mechlenburg et al.	6,837,238	B2	1/2005	McDonald
6,564,800	B1	5/2003	Olivares	6,840,240	B1	1/2005	Berthon-Jones et al.
6,568,391	B1	5/2003	Tatarek et al.	6,843,247	B2	1/2005	Frye et al.
6,571,794	B1	6/2003	Hansen	6,915,803	B2	1/2005	Berthon-Jones et al.
6,571,796	B2	6/2003	Banner et al.	6,848,446	B2	2/2005	Noble
6,571,798	B1	6/2003	Thornton	6,854,462	B2	2/2005	Berthon-Jones et al.
6,575,159	B1	6/2003	Frye et al.	6,863,069	B2	3/2005	Wood
6,575,166	B2	6/2003	Boussignac	6,866,041	B2	3/2005	Hardy, Jr. et al.
6,575,944	B1	6/2003	McNary et al.	6,877,511	B2	4/2005	DeVries et al.
6,584,973	B1	7/2003	Biondi et al.	6,880,556	B2	4/2005	Uchiyama et al.
6,588,422	B1	7/2003	Berthon-Jones et al.	6,910,480	B1	6/2005	Berthon-Jones
6,588,423	B1	7/2003	Sinderby	6,910,482	B2	6/2005	Bliss et al.
6,591,834	B1	7/2003	Colla et al.	6,910,510	B2	6/2005	Gale et al.
6,591,835	B1	7/2003	Blanch	6,913,601	B2	7/2005	St Goar et al.
6,595,207	B1	7/2003	McDonald et al.	6,920,875	B1	7/2005	Hill et al.
6,595,215	B2	7/2003	Wood	6,920,877	B2	7/2005	Remmers et al.
6,640,806	B2	7/2003	Yurko	6,920,878	B2	7/2005	Sinderby et al.
6,609,517	B1	8/2003	Estes et al.	6,932,084	B2	8/2005	Estes et al.
6,629,529	B2	8/2003	Arnott	6,938,619	B1	9/2005	Hickle
6,622,726	B1	9/2003	Du	6,938,620	B2	9/2005	Payne, Jr.
6,626,174	B1	9/2003	Genger et al.	6,941,950	B2	9/2005	Wilson et al.
6,626,175	B2	9/2003	Jafari et al.	6,948,497	B2	9/2005	Zdrojkowski et al.
6,629,525	B2	10/2003	Hill et al.	6,951,217	B2	10/2005	Berthon-Jones
6,629,527	B1	10/2003	Estes et al.	6,971,382	B1	12/2005	Corso
6,631,919	B1	10/2003	West et al.	6,986,353	B2	1/2006	Wright
6,634,356	B1	10/2003	O'Dea et al.	6,994,089	B2	2/2006	Wood
6,635,021	B1	10/2003	Sullivan et al.	6,997,177	B2	2/2006	Wood
6,644,305	B2	11/2003	MacRae et al.	6,997,881	B2	2/2006	Green et al.
6,644,311	B1	11/2003	Truitt et al.	7,000,612	B2	2/2006	Jafari et al.
6,644,315	B2	11/2003	Ziaee	7,004,170	B1	2/2006	Gillstrom
6,651,653	B1	11/2003	Honkonen et al.	7,007,692	B2	3/2006	Aylsworth et al.
6,651,656	B2	11/2003	Demers et al.	7,011,091	B2	3/2006	Hill et al.
6,651,658	B1	11/2003	Hill et al.	7,013,892	B2	3/2006	Estes et al.
6,655,382	B1	12/2003	Kolobow	7,013,898	B2	3/2006	Rashad et al.
6,655,385	B1	12/2003	Curti et al.	7,017,574	B2	3/2006	Biondi et al.
6,666,208	B1	12/2003	Schumacher et al.	7,017,575	B2	3/2006	Yagi et al.
6,668,828	B1	12/2003	Figley et al.	7,024,945	B2	4/2006	Wallace
6,669,712	B1	12/2003	Cardoso	7,036,504	B2	5/2006	Wallace et al.
6,675,796	B2	1/2004	McDonald	7,044,129	B1	5/2006	Truschel et al.
6,675,801	B2	1/2004	Wallace et al.	7,047,969	B2	5/2006	Noble
6,679,265	B2	1/2004	Strickland et al.	7,047,974	B2	5/2006	Strickland et al.
6,681,764	B1	1/2004	Honkonen et al.	7,051,735	B2	5/2006	Mechlenbrug et al.
6,684,883	B1	2/2004	Bums	7,055,522	B2	6/2006	Berthon-Jones
6,691,702	B2	2/2004	Appel et al.	7,059,328	B2	6/2006	Wood
6,691,707	B1	2/2004	Gunaratnam et al.	7,066,173	B2	6/2006	Banner et al.
6,694,973	B1	2/2004	Dunhao et al.	7,066,178	B2	6/2006	Gunaratnam et al.
6,694,978	B1	2/2004	Bennarsten	7,077,132	B2	7/2006	Berthon-Jones
6,698,423	B1	3/2004	Honkonen et al.	7,077,133	B2	7/2006	Yagi et al.
6,705,314	B1	3/2004	O'Dea	7,080,645	B2	7/2006	Genger et al.
6,705,315	B2	3/2004	Sullivan et al.	7,080,646	B2	7/2006	Wiesmann et al.
6,722,360	B2	4/2004	Doshi	7,100,607	B2	9/2006	Zdrojkowski et al.
6,722,362	B2	4/2004	Hete et al.	7,100,609	B2	9/2006	Berthon-Jones et al.
6,742,517	B1	6/2004	Frye et al.	7,117,438	B2	10/2006	Wallace et al.
6,745,768	B2	6/2004	Colla et al.	7,121,277	B2	10/2006	Strom
6,752,150	B1	6/2004	Remmers et al.	7,128,578	B2	10/2006	Lampotang et al.
6,752,151	B2	6/2004	Hill	7,152,598	B2	12/2006	Morris et al.
6,752,152	B2	6/2004	Gale et al.	7,152,604	B2	12/2006	Hickle et al.
6,755,193	B2	6/2004	Berthon-Jones et al.	7,156,090	B2	1/2007	Nomori
6,823,866	B2	6/2004	Jafari et al.	7,156,097	B2	1/2007	Cardoso
				7,162,296	B2	1/2007	Leonhardt et al.
				7,168,429	B2	1/2007	Matthews et al.
				7,188,621	B2	3/2007	DeVries et al.
				7,188,624	B2	3/2007	Wood

(56)

References Cited

U.S. PATENT DOCUMENTS

7,195,016 B2	3/2007	Loyd et al.	7,832,400 B2	11/2010	Curti et al.
7,195,018 B1	3/2007	Goldstein	7,837,761 B2	11/2010	Bliss et al.
7,201,169 B2	4/2007	Wikie et al.	7,841,343 B2	11/2010	Deane et al.
7,201,269 B2	4/2007	Buscher et al.	7,845,350 B1	12/2010	Kayyali et al.
D542,912 S	5/2007	Gunaratnam et al.	7,849,854 B2	12/2010	DeVries et al.
7,222,623 B2	5/2007	DeVries et al.	7,856,982 B2	12/2010	Matula, Jr. et al.
7,225,811 B2	6/2007	Ruiz et al.	7,866,318 B2	1/2011	Bassin
7,234,465 B2	6/2007	Wood	7,874,290 B2	1/2011	Chalvignac
7,237,205 B2	6/2007	Sarel	7,874,291 B2	1/2011	Ging et al.
7,246,620 B2	7/2007	Conroy, Jr.	7,874,293 B2	1/2011	Gunaratnam et al.
D549,323 S	8/2007	Kwok et al.	7,878,980 B2	2/2011	Ricciardelli
7,255,103 B2	8/2007	Bassin	7,882,834 B2	2/2011	Gradon et al.
7,255,107 B1	8/2007	Gomez	7,886,740 B2	2/2011	Thomas et al.
7,267,122 B2	9/2007	Hill	7,891,353 B2	2/2011	Chalvignac
7,267,123 B2	9/2007	Aylsworth et al.	7,891,357 B2	2/2011	Carron et al.
7,270,126 B2	9/2007	Wallace et al.	7,896,958 B2	3/2011	Sermet et al.
7,270,128 B2	9/2007	Berthon-Jones et al.	7,900,627 B2	3/2011	Aylsworth et al.
7,296,569 B2	11/2007	Frye et al.	7,900,628 B2	3/2011	Matula, Jr. et al.
7,296,573 B2	11/2007	Estes et al.	7,900,635 B2	3/2011	Gunaratnam et al.
D557,802 S	12/2007	Miceli, Jr. et al.	7,901,361 B2	3/2011	Rapoport et al.
7,302,950 B2	12/2007	Berthon-Jones et al.	7,905,231 B2	3/2011	Chalvignac
7,305,987 B2	12/2007	Scholler et al.	7,913,691 B2	3/2011	Farrugia
7,318,437 B2	1/2008	Gunaratnam et al.	7,914,459 B2	3/2011	Green et al.
7,320,321 B2	1/2008	Pranger et al.	7,918,226 B2	4/2011	Acker et al.
7,328,703 B1	2/2008	Tiep	7,926,486 B2	4/2011	Childers
7,353,826 B2	4/2008	Sleeper et al.	7,926,487 B2	4/2011	Drew et al.
7,367,337 B2	5/2008	Berthon-Jones et al.	7,931,023 B2	4/2011	Berthon-Jones et al.
7,370,652 B2	5/2008	Matula, Jr. et al.	7,934,499 B2	5/2011	Berthon-Jones
7,373,939 B1	5/2008	DuBois et al.	7,938,114 B2	5/2011	Matthews et al.
7,406,966 B2	8/2008	Wondka	7,942,150 B2	5/2011	Guney et al.
7,416,532 B1*	8/2008	Broshears ..... A61B 5/01 600/549	7,942,380 B2	5/2011	Bertinetti et al.
7,418,965 B2	9/2008	Fukunaga et al.	7,958,892 B2	6/2011	Kwok et al.
7,422,015 B2	9/2008	Delisle et al.	7,975,694 B2	7/2011	Ho
7,431,035 B2	10/2008	Mizuta et al.	7,980,245 B2	7/2011	Rice et al.
7,451,762 B2	11/2008	Chua et al.	7,987,847 B2	8/2011	Wickham et al.
7,455,717 B2	11/2008	Sprinkel	7,987,850 B2	8/2011	Zollinger et al.
7,461,656 B2	12/2008	Gunaratnam et al.	7,987,851 B2	8/2011	Blom et al.
7,468,040 B2	12/2008	Hartley et al.	7,992,557 B2	8/2011	Nadjafizadeh et al.
7,469,697 B2	12/2008	Lee et al.	7,997,270 B2	8/2011	Meier
7,472,702 B2	1/2009	Beck et al.	7,997,271 B2	8/2011	Hickle et al.
7,478,641 B2	1/2009	Rousselet	7,997,272 B2	8/2011	Isaza
7,481,219 B2	1/2009	Lewis et al.	8,001,967 B2	8/2011	Wallace et al.
7,481,221 B2	1/2009	Kullik et al.	D645,557 S	9/2011	Scheiner et al.
7,487,774 B2	2/2009	Acker	8,011,365 B2	9/2011	Douglas et al.
7,487,778 B2	2/2009	Freitag	8,011,366 B2	9/2011	Knepper
7,490,605 B2	2/2009	Frye et al.	8,015,971 B2	9/2011	Kwok
D588,258 S	3/2009	Judson et al.	8,015,974 B2	9/2011	Christopher et al.
D589,139 S	3/2009	Guney et al.	8,020,558 B2	9/2011	Christopher et al.
7,500,482 B2	3/2009	Biederman	8,025,052 B2	9/2011	Matthews et al.
7,509,957 B2	3/2009	Duquette et al.	RE42,843 E	10/2011	Strickland et al.
D591,419 S	4/2009	Chandran et al.	8,042,535 B2	10/2011	Kenyon et al.
7,533,670 B1	5/2009	Freitag et al.	8,042,537 B2	10/2011	Mechlenburg et al.
7,556,038 B2	7/2009	Kirby et al.	8,042,539 B2	10/2011	Chandran et al.
7,559,327 B2	7/2009	Hernandez	8,042,546 B2	10/2011	Gunaratnam et al.
7,562,657 B2	7/2009	Blanch et al.	8,061,354 B2	11/2011	Schneider et al.
7,562,659 B2	7/2009	Matarasso	8,066,004 B2	11/2011	Morris et al.
7,578,294 B2	8/2009	Pierro et al.	8,393,328 B2*	3/2013	Angel ..... A61M 16/04 128/200.26
7,588,033 B2	9/2009	Wondka	2001/0035185 A1	11/2001	Christopher
7,591,265 B2	9/2009	Lee et al.	2001/0035186 A1	11/2001	Hill
7,631,642 B2	12/2009	Freitag et al.	2001/0042548 A1	11/2001	Boussignac
7,640,934 B2	1/2010	Zollinger et al.	2002/0014241 A1	2/2002	Gradon et al.
7,658,189 B2	2/2010	Davidson et al.	2002/0017300 A1	2/2002	Hickle et al.
D614,288 S	4/2010	Judson et al.	2002/0020930 A1	2/2002	Austin et al.
7,721,733 B2	5/2010	Hughes et al.	2002/0026941 A1	3/2002	Biondi et al.
7,721,736 B2	5/2010	Urias et al.	2002/0043264 A1	4/2002	Wickham
7,740,013 B2	6/2010	Ishizaki et al.	2002/0046751 A1	4/2002	MacRae et al.
7,743,770 B2	6/2010	Curti et al.	2002/0046755 A1	4/2002	De Voss
7,762,253 B2	7/2010	Acker et al.	2002/0046756 A1	4/2002	Laizzo et al.
7,766,009 B2	8/2010	Frye et al.	2002/0053346 A1	5/2002	Curti et al.
7,787,946 B2	8/2010	Stahmann et al.	2002/0055685 A1	5/2002	Levitsky et al.
7,814,906 B2	10/2010	Moretti	2002/0059935 A1	5/2002	Wood
7,819,120 B2	10/2010	Taylor et al.	2002/0066452 A1	6/2002	Kessler et al.
D626,646 S	11/2010	Lubke et al.	2002/0078957 A1	6/2002	Remmers et al.
D627,059 S	11/2010	Wood et al.	2002/0092527 A1	7/2002	Wood
			2002/0112730 A1	8/2002	Dutkiewicz
			2002/0153010 A1	10/2002	Rozenberg et al.
			2002/0157673 A1	10/2002	Kessler et al.
			2002/0159323 A1	10/2002	Makabe et al.

(56)		References Cited						
		U.S. PATENT DOCUMENTS						
2002/0179090	A1	12/2002	Boussignac	2006/0124134	A1	6/2006	Wood	
2003/0000522	A1	1/2003	Lynn et al.	2006/0137690	A1	6/2006	Gunaratnam et al.	
2003/0047185	A1	3/2003	Olsen et al.	2006/0144396	A1	7/2006	DeVries et al.	
2003/0069489	A1	4/2003	Abreu	2006/0149144	A1	7/2006	Lynn et al.	
2003/0079749	A1	5/2003	Strickland et al.	2006/0150972	A1	7/2006	Mizuta et al.	
2003/0094178	A1	5/2003	McAuley et al.	2006/0150973	A1	7/2006	Chalvignac	
2003/0111081	A1	6/2003	Gupta	2006/0150982	A1	7/2006	Wood	
2003/0116163	A1	6/2003	Wood	2006/0174877	A1	8/2006	Jagger et al.	
2003/0121519	A1	7/2003	Estes et al.	2006/0180149	A1	8/2006	Matarasso	
2003/0145852	A1	8/2003	Schmidt et al.	2006/0185669	A1	8/2006	Bassovithc	
2003/0145853	A1	8/2003	Muellner	2006/0201504	A1	9/2006	Singhal et al.	
2003/0145856	A1	8/2003	Zdrojkowski et al.	2006/0213518	A1	9/2006	DeVries et al.	
2003/0150455	A1	8/2003	Bliss et al.	2006/0213519	A1	9/2006	Schmidt et al.	
2003/0159696	A1	8/2003	Boussignac et al.	2006/0225737	A1	10/2006	Lobbi	
2003/0159697	A1	8/2003	Wallace	2006/0237013	A1	10/2006	Kwok	
2003/0168067	A1	9/2003	Dougill et al.	2006/0243278	A1	11/2006	Hamilton et al.	
2003/0213488	A1	11/2003	Remmers et al.	2006/0249155	A1	11/2006	Gambone	
2003/0221687	A1	12/2003	Kaigler	2006/0264772	A1	11/2006	Aljuri et al.	
2003/0230308	A1	12/2003	Linden	2006/0266361	A1	11/2006	Hernandez	
2004/0020493	A1	2/2004	Wood	2007/0000490	A1	1/2007	DeVries et al.	
2004/0025881	A1	2/2004	Gunaratnam et al.	2007/0000495	A1	1/2007	Matula et al.	
2004/0035431	A1	2/2004	Wright	2007/0017515	A1	1/2007	Wallace et al.	
2004/0040560	A1	3/2004	Euliano et al.	2007/0056590	A1	3/2007	Wolfson	
2004/0050387	A1	3/2004	Younes	2007/0062529	A1	3/2007	Choncholas et al.	
2004/0074494	A1	4/2004	Frater	2007/0068528	A1	3/2007	Bohm et al.	
2004/0159323	A1	8/2004	Schmidt et al.	2007/0074724	A1	4/2007	Duquette et al.	
2004/0206352	A1	10/2004	Conroy	2007/0089743	A1	4/2007	Hoffman	
2004/0221848	A1	11/2004	Hill	2007/0089745	A1	4/2007	Gabriel et al.	
2004/0221854	A1	11/2004	Hete et al.	2007/0095347	A1	5/2007	Lampotang et al.	
2004/0226566	A1	11/2004	Gunaratnam et al.	2007/0107728	A1	5/2007	Ricciardelli et al.	
2004/0231674	A1	11/2004	Tanaka	2007/0107732	A1	5/2007	Dennis et al.	
2004/0237963	A1	12/2004	Berthon-Jones	2007/0107737	A1	5/2007	Landis et al.	
2004/0254501	A1	12/2004	Mault	2007/0113850	A1	5/2007	Acker et al.	
2004/0255943	A1	12/2004	Morris et al.	2007/0113856	A1	5/2007	Acker et al.	
2005/0005936	A1	1/2005	Wondka	2007/0125379	A1	6/2007	Pierro et al.	
2005/0005938	A1	1/2005	Berthon-Jones et al.	2007/0137653	A1	6/2007	Wood	
2005/0010125	A1	1/2005	Joy et al.	2007/0144526	A1 *	6/2007	Blom .....	A61M 16/0468
2005/0011524	A1	1/2005	Thomlinson et al.	2007/0163600	A1	7/2007	Hoffman	128/207.16
2005/0016534	A1	1/2005	Ost	2007/0173705	A1	7/2007	Teller et al.	
2005/0033247	A1	2/2005	Thompson	2007/0181125	A1	8/2007	Mulier	
2005/0034721	A1 *	2/2005	Freitag .....	2007/0193705	A1	8/2007	Hsu	
			A61M 16/0072	2007/0199568	A1	8/2007	Diekens et al.	
			128/200.24	2007/0209662	A1	9/2007	Bowen et al.	
2005/0034724	A1	2/2005	O'Dea	2007/0215156	A1	9/2007	Kwok	
2005/0061322	A1	3/2005	Freitag	2007/0232950	A1	10/2007	West	
2005/0061326	A1	3/2005	Payne	2007/0240716	A1	10/2007	Marx	
2005/0072430	A1	4/2005	Djupesland	2007/0251528	A1	11/2007	Seitz et al.	
2005/0081849	A1	4/2005	Warren	2007/0272249	A1	11/2007	Chandran et al.	
2005/0087190	A1	4/2005	Jafari et al.	2008/0000475	A1	1/2008	Hill	
2005/0098179	A1	5/2005	Burton et al.	2008/0006271	A1	1/2008	Aylsworth et al.	
2005/0103343	A1	5/2005	Gosweiler	2008/0011298	A1	1/2008	Mazar et al.	
2005/0121033	A1	6/2005	Starr et al.	2008/0011301	A1	1/2008	Qian	
2005/0121037	A1	6/2005	Wood	2008/0041371	A1	2/2008	Freitag	
2005/0121038	A1	6/2005	Christopher	2008/0041386	A1	2/2008	Dodier et al.	
2005/0150498	A1	7/2005	McDonald	2008/0045815	A1	2/2008	Derchak et al.	
2005/0161049	A1	7/2005	Wright	2008/0047559	A1	2/2008	Fiori	
2005/0166924	A1	8/2005	Thomas et al.	2008/0051674	A1	2/2008	Davenport et al.	
2005/0199242	A1	9/2005	Matula et al.	2008/0053438	A1	3/2008	DeVries et al.	
2005/0205096	A1	9/2005	Matula et al.	2008/0053447	A1	3/2008	Ratajczak et al.	
2005/0247308	A1	11/2005	Frye et al.	2008/0060646	A1	3/2008	Isaza	
2005/0257793	A1	11/2005	Tatsumoto	2008/0060657	A1	3/2008	McAuley et al.	
2005/0274381	A1	12/2005	Deane et al.	2008/0066753	A1	3/2008	Martin et al.	
2005/0279360	A1 *	12/2005	Wei .....	2008/0072902	A1	3/2008	Setzer et al.	
			A61M 16/04	2008/0078392	A1	4/2008	Pelletier et al.	
			128/207.14	2008/0078407	A1	4/2008	Sherman	
2006/0005834	A1	1/2006	Aylsworth et al.	2008/0092904	A1	4/2008	Gunarathnam et al.	
2006/0005842	A1	1/2006	Rashad et al.	2008/0092905	A1	4/2008	Gunarathnam et al.	
2006/0011199	A1	1/2006	Rashad et al.	2008/0092906	A1	4/2008	Gunarathnam et al.	
2006/0027234	A1	2/2006	Gradon et al.	2008/0099024	A1	5/2008	Gunarathnam et al.	
2006/0048781	A1	3/2006	Nawata	2008/0099027	A1	5/2008	Gunarathnam et al.	
2006/0054169	A1	3/2006	Han et al.	2008/0105264	A1	5/2008	Gunarathnam et al.	
2006/0070625	A1	4/2006	Ayappa et al.	2008/0110462	A1	5/2008	Chekal et al.	
2006/0079799	A1	4/2006	Green et al.	2008/0121230	A1	5/2008	Cortez et al.	
2006/0096596	A1	5/2006	Occhialini et al.	2008/0135044	A1	6/2008	Freitag et al.	
2006/0107958	A1	5/2006	Sleeper	2008/0142019	A1	6/2008	Lewis et al.	
2006/0112959	A1	6/2006	Mechienburg et al.	2008/0161653	A1	7/2008	Lin et al.	
2006/0124131	A1	6/2006	Chandran et al.	2008/0173304	A1	7/2008	Zaiser et al.	
				2008/0178880	A1	7/2008	Christopher et al.	

(56)

## References Cited

## U.S. PATENT DOCUMENTS

2008/0178881 A1 7/2008 Whitcher et al.  
 2008/0178882 A1 7/2008 Christopher et al.  
 2008/0185002 A1 8/2008 Berthon-Jones et al.  
 2008/0185007 A1 8/2008 Sleeper et al.  
 2008/0190429 A1 8/2008 Tatarek  
 2008/0190436 A1 8/2008 Jaffe et al.  
 2008/0196715 A1 8/2008 Yamamori  
 2008/0196723 A1 8/2008 Tilley  
 2008/0196728 A1 8/2008 Ho  
 2008/0202528 A1 8/2008 Carter et al.  
 2008/0216834 A1 9/2008 Easley et al.  
 2008/0216838 A1 9/2008 Wondka  
 2008/0216841 A1 9/2008 Grimes et al.  
 2008/0223369 A1 9/2008 Warren  
 2008/0245369 A1 10/2008 Matula et al.  
 2008/0251079 A1 10/2008 Richey  
 2008/0264417 A1 10/2008 Manigel et al.  
 2008/0283060 A1 11/2008 Bassin  
 2008/0295846 A1 12/2008 Han et al.  
 2008/0302364 A1 12/2008 Garde et al.  
 2008/0308104 A1 12/2008 Blomberg et al.  
 2009/0007911 A1 1/2009 Cleary et al.  
 2009/0020121 A1 1/2009 Bassin  
 2009/0044808 A1 2/2009 Guney et al.  
 2009/0056708 A1 3/2009 Stenzler et al.  
 2009/0078255 A1 3/2009 Bowman et al.  
 2009/0078258 A1 3/2009 Bowman et al.  
 2009/0095298 A1 4/2009 Gunarathnam et al.  
 2009/0095300 A1 4/2009 McMorrow  
 2009/0095303 A1 4/2009 Sher et al.  
 2009/0099471 A1 4/2009 Broadley et al.  
 2009/0101147 A1 4/2009 Landis et al.  
 2009/0101154 A1 4/2009 Mutti et al.  
 2009/0107502 A1 4/2009 Younes  
 2009/0118632 A1 5/2009 Goepf  
 2009/0120437 A1 5/2009 Oates et al.  
 2009/0126739 A1 5/2009 Ng et al.  
 2009/0133699 A1 5/2009 Nalagatta et al.  
 2009/0139527 A1 6/2009 Ng et al.  
 2009/0145435 A1 6/2009 White et al.  
 2009/0151719 A1 6/2009 Wondka et al.  
 2009/0151724 A1 6/2009 Wondka et al.  
 2009/0151726 A1 6/2009 Freitag  
 2009/0151729 A1 6/2009 Judson et al.  
 2009/0165799 A1 7/2009 Duquette et al.  
 2009/0173347 A1 7/2009 Berthon-Jones  
 2009/0173349 A1 7/2009 Hernandez et al.  
 2009/0183739 A1 7/2009 Wondka  
 2009/0199855 A1 8/2009 Davenport  
 2009/0205662 A1 8/2009 Kwok et al.  
 2009/0241651 A1 10/2009 Jafari et al.  
 2009/0241947 A1 10/2009 Bedini et al.  
 2009/0250066 A1 10/2009 Daly  
 2009/0255533 A1 10/2009 Freitag et al.  
 2009/0260625 A1 10/2009 Wondka  
 2009/0277452 A1 11/2009 Lubke et al.  
 2009/0293877 A1 12/2009 Blanch et al.  
 2009/0301495 A1 12/2009 Pierro et al.  
 2009/0308395 A1 12/2009 Lee et al.  
 2009/0320851 A1 12/2009 Selvarajan et al.  
 2010/0043786 A1 2/2010 Freitag et al.  
 2010/0071693 A1 3/2010 Allum et al.  
 2010/0071697 A1 3/2010 Jafari et al.  
 2010/0083968 A1 4/2010 Wondka et al.  
 2010/0108073 A1 5/2010 Zollinger et al.  
 2010/0132716 A1 6/2010 Selvarajan et al.  
 2010/0132717 A1 6/2010 Davidson et al.  
 2010/0163043 A1 7/2010 Hart et al.  
 2010/0170512 A1 7/2010 Kuypers et al.  
 2010/0170513 A1 7/2010 Bowditch et al.  
 2010/0192957 A1 8/2010 Hobson et al.  
 2010/0218766 A1 9/2010 Milne  
 2010/0224196 A1 9/2010 Jablons  
 2010/0252037 A1 10/2010 Wondka et al.  
 2010/0252039 A1 10/2010 Cipollone et al.

2010/0252040 A1 10/2010 Kapust et al.  
 2010/0252041 A1 10/2010 Kapust et al.  
 2010/0252042 A1 10/2010 Kapust et al.  
 2010/0252043 A1 10/2010 Freitag  
 2010/0252044 A1 10/2010 Duquette et al.  
 2010/0269834 A1 10/2010 Freitag et al.  
 2010/0275920 A1 11/2010 Tham et al.  
 2010/0275921 A1 11/2010 Schindhelm et al.  
 2010/0282251 A1 11/2010 Calluaud et al.  
 2010/0282810 A1 11/2010 Hawes  
 2010/0288279 A1 11/2010 Selver et al.  
 2010/0288289 A1 11/2010 Nasir  
 2010/0300445 A1 12/2010 Chatburn et al.  
 2010/0300446 A1 12/2010 Nicolazzi et al.  
 2010/0307487 A1 12/2010 Dunsmore et al.  
 2010/0307495 A1 12/2010 Kepler et al.  
 2010/0307499 A1 12/2010 Eger et al.  
 2010/0307500 A1 12/2010 Armitstead  
 2010/0307502 A1 12/2010 Rummery et al.  
 2010/0313891 A1 12/2010 Veliss et al.  
 2010/0313898 A1 12/2010 Richard et al.  
 2010/0319703 A1 12/2010 Hayman et al.  
 2010/0326441 A1 12/2010 Zucker et al.  
 2010/0326446 A1 12/2010 Behimaier  
 2011/0000489 A1 1/2011 Laksov et al.  
 2011/0009763 A1 1/2011 Levitsky et al.  
 2011/0011402 A1 1/2011 Berthon-Jones  
 2011/0023878 A1 2/2011 Thiessen  
 2011/0023881 A1 2/2011 Thiessen  
 2011/0034819 A1 2/2011 Desforges et al.  
 2011/0036352 A1 2/2011 Estes et al.  
 2011/0041850 A1 2/2011 Vandine et al.  
 2011/0041855 A1 2/2011 Gunarathnam et al.  
 2011/0061647 A1 3/2011 Stahmann et al.  
 2011/0067704 A1 3/2011 Kooij et al.  
 2011/0067709 A1 3/2011 Doshi et al.  
 2011/0071444 A1 3/2011 Kassatly et al.  
 2011/0073107 A1 3/2011 Rodman et al.  
 2011/0073116 A1 3/2011 Genger et al.  
 2011/0087123 A9 4/2011 Choncholas et al.  
 2011/0088690 A1 4/2011 Djupesland et al.  
 2011/0094518 A1 4/2011 Cipollone et al.  
 2011/0100365 A1 5/2011 Wedler et al.  
 2011/0114098 A1 5/2011 McAuley et al.  
 2011/0125052 A1 5/2011 Davenport et al.  
 2011/0126841 A1 6/2011 Matula, Jr. et al.  
 2011/0132363 A1 6/2011 Chalvignac  
 2011/0139153 A1 6/2011 Chalvignac  
 2011/0146687 A1 6/2011 Fukushima  
 2011/0155140 A1 6/2011 Ho et al.  
 2011/0162650 A1 7/2011 Miller et al.  
 2011/0162655 A1 7/2011 Gunarathnam et al.  
 2011/0178419 A1 7/2011 Wood et al.  
 2011/0180068 A1 7/2011 Kenyon et al.  
 2011/0197885 A1 8/2011 Wondka et al.  
 2011/0209705 A1 9/2011 Freitag  
 2011/0214676 A1 9/2011 Allum et al.  
 2011/0220105 A1 9/2011 Meier  
 2011/0232642 A1 9/2011 Bliss et al.  
 2011/0247625 A1 10/2011 Blussignac  
 2011/0253147 A1 10/2011 Gusky et al.  
 2011/0259327 A1 10/2011 Wondka et al.  
 2011/0265796 A1 11/2011 Amarasinghe et al.  
 2011/0277765 A1 11/2011 Christopher et al.  
 2011/0284003 A1 11/2011 Douglas et al.

## FOREIGN PATENT DOCUMENTS

CN 200480029872 11/2006  
 DE 19626924 1/1998  
 DE 29902267 U1 7/1999  
 DE 19841070 5/2000  
 DE 19849571 5/2000  
 DE 10337138 8/2003  
 DE 10337138.9 3/2005  
 DE 102006023637.8 11/2007  
 EP 0125424 11/1984  
 EP 0692273 1/1996  
 EP 0778035 6/1997

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1359961	11/2003	
EP	1654023	5/2006	
EP	1820527	8/2007	..... A61B 1/267
EP	2377462	11/2010	
GB	2174609	11/1986	
GB	2201098	8/1988	
GB	1055148	6/1989	
GB	2338420	12/1999	
JP	S63-57060	3/1998	
JP	2002-204830	7/2002	
JP	2006-522883	2/2007	
WO	WO-1992/11054	7/1992	
WO	9745153	12/1997	
WO	WO-98/01176	1/1998	
WO	WO-1998/01176	1/1998	
WO	WO-1999/04841	2/1999	
WO	WO 9965552	12/1999	..... A61M 16/04
WO	WO-2009/109005	9/2000	
WO	WO-2009/115944	9/2000	
WO	WO-2000/064521	11/2000	
WO	WO-2006/138580	12/2000	
WO	WO-01/076655	10/2001	
WO	WO-2001/076655	10/2001	
WO	WO-2002/062413	8/2002	
WO	WO-2004/009169	1/2004	
WO	WO-2005/014091	2/2005	
WO	WO2005014091	2/2005	
WO	WO-2005/018524	3/2005	
WO	WO-2005/086943	9/2005	
WO	WO-2007/035804	3/2007	
WO	WO2007035804	3/2007	
WO	WO-2007/139531	12/2007	
WO	WO-2007/142812	12/2007	
WO	WO2007142812	12/2007	
WO	WO-2008/014543	2/2008	
WO	WO-2008/019102	2/2008	
WO	WO-2008/052534	5/2008	
WO	WO-2008/112474	9/2008	
WO	WO-2008/138040	11/2008	
WO	WO-2008/144589	11/2008	
WO	WO-2008/144669	11/2008	
WO	WO-2009/042973	4/2009	
WO	WO-2009/042974	4/2009	
WO	WO-2009/059353	5/2009	
WO	WO-2009/064202	5/2009	
WO	WO-2009/074160	6/2009	
WO	WO-2009/082295	7/2009	
WO	WO-2009/087607	7/2009	
WO	WO-2009/092057	7/2009	
WO	WO-2009/103288	8/2009	
WO	WO-2009/115948	9/2009	
WO	WO-2009/115949	9/2009	
WO	WO-2009/129506	10/2009	
WO	WO-2009/136101	11/2009	
WO	WO-2009/139647	11/2009	
WO	WO-2009/149351	12/2009	
WO	WO-2009/149353	12/2009	
WO	WO-2009/149355	12/2009	
WO	WO-2009/149357	12/2009	
WO	WO-2009/151344	12/2009	
WO	WO-2009/151791	12/2009	
WO	WO-2010/000135	1/2010	
WO	WO-2010/021556	2/2010	
WO	WO-2010/022363	2/2010	
WO	WO-2010/039989	4/2010	
WO	WO-2010/041966	4/2010	
WO	WO-2010/044034	4/2010	
WO	WO-2010/057268	5/2010	
WO	WO-2010/059049	5/2010	
WO	WO-2010/060422	6/2010	
WO	WO-2010/068356	6/2010	
WO	WO-2010/070493	6/2010	
WO	WO-2010/070497	6/2010	
WO	WO-2010/070498	6/2010	
WO	WO-2010/076711	7/2010	

WO	WO-2010/081223	7/2010
WO	WO-2010/091157	8/2010
WO	WO-2010/099375	9/2010
WO	WO-2010/102094	9/2010
WO	WO-2010/115166	10/2010
WO	WO-2010/115168	10/2010
WO	WO-2010/115169	10/2010
WO	WO-2010/115170	10/2010
WO	WO-2010/116275	10/2010
WO	WO-2010/132853	11/2010
WO	WO-2010/136923	12/2010
WO	WO-2010/139014	12/2010
WO	WO-2010/150187	12/2010
WO	WO-2011/002608	1/2011
WO	WO-2011/004274	1/2011
WO	WO-2011/006184	1/2011
WO	WO-2011/006199	1/2011
WO	WO-2011/014931	2/2011
WO	WO-2011/017033	2/2011
WO	WO-2011/017738	2/2011
WO	WO-2011/021978	2/2011
WO	WO-2011/022779	3/2011
WO	WO-2011/024383	3/2011
WO	WO-2011/029073	3/2011
WO	WO-2011/029074	3/2011
WO	WO2011035373	3/2011
WO	WO2011038950	4/2011
WO	WO2011038951	4/2011
WO	WO2011044627	4/2011
WO	WO2011057362	5/2011
WO	WO2011059346	5/2011
WO	WO2011061648	5/2011
WO	WO2011062510	5/2011
WO	WO2011086437	7/2011
WO	WO2011086438	7/2011
WO	WO2011112807	9/2011

OTHER PUBLICATIONS

Extended European Search Report for European Patent Application No. 08755904.3 dated Sep. 7, 2015.

Canadian Office Action for Canadian Patent Application No. 2,688,719; dated Feb. 23, 2015.

International Search Report and Opinion for Application No. PCT/US07/17400, dated Apr. 28, 2008.

European Search Report dated Oct. 19, 2007 EP 04762494.

International Search Report for wo2005/014091 (Application No. PCT/DE04/1646), dated Jan. 17, 2005.

International Search Report and Written Opinion for PCT/US07/12108, dated Aug. 8, 2008.

Christopher et al., "Transtracheal Oxygen Therapy for Refractory Hypoxemia," JAMA 1986, vol. 256, No. 4, pp. 494-497.

Teip et al., "Pulsed nasal and transtracheal oxygen delivery," Chest, 1990, vol. 97, pp. 364-368.

Yaeger et al., "Oxygen Therapy Using Pulse and Continuous Flow with a Transtracheal catheter and a nasal Cannula," Chest, 1994, vol. 106, pp. 854-860.

Christopher et al., "Preliminary Observations of Transtracheal Augmented Ventilation for Chronic Severe Respiratory Disease," Respiratory Care, Jan. 2001, vol. 46, No. 1, pp. 15-25.

Fink, J.B., "Helium-Oxygen: An Old Therapy Creates New Interest," J Respr Care Pract now RT for Decision Makers in Respiratory Care, Apr./May 1999, pp. 71-76.

Haenel et al., "Efficacy of Selective Intrabronchial Air Insufflation in Acute Lobar Collapse," AmJ Surg, 1992, vol. 164, No. 5, pp. 501-505.

AARC Clinical Practice Guideline: Oxygen Therapy in the Home or Extended Care Facility, Respiratory Care, Aug. 1992, vol. 37, No. 8, pp. 918-922.

McIntyre, N. R., "Long-Term Oxygen Therapy: Conference Summary," Respiratory Care, Feb. 2000, vol. 45, No. 2, pp. 237-245.

VHA/DOD Clinical Practice Guideline, "Management of Chronic Obstructive Pulmonary Disease," Ver. 1.1a, Aug. 1999, Updated Nov. 1999.

(56)

## References Cited

## OTHER PUBLICATIONS

- Blanch, L. L., "Clinical Studies of Tracheal Gas Insufflation," *Respiratory Care*, Feb. 2001, vol. 46, No. 2, pp. 158-166.
- Gregoretti et al., "Transtracheal Open Ventilation in Acute Respiratory Failure Secondary to Severe Chronic Obstructive Pulmonary Disease Exacerbation," *Am J Respir Crit Care Med*. 2006, vol. 173, No. 8, pp. 877-881.
- Chang et al., "Reduced Inspiratory Muscle Endurance Following Successful Weaning from Prolonged Mechanical Ventilation," *Chest*, 2005, vol. 128, No. 2, pp. 553-559.
- Gaughan et al., "A comparison in a Lung Model of Low-and-High-Flow Regulators for Transtracheal Jet Ventilation," *Anesthesiology*, 1992, vol. 77, No. 1, pp. 189-199.
- Menon et al., "Tracheal Perforation. A Complication Associated with Transtracheal Oxygen Therapy," *Chest*, 1993, vol. 140, No. 2, pp. 636-637.
- Rothe, et al. "Near Fatal Complication of Transtracheal Oxygen Therapy with the Scoop(r) System," *Pneumologie*, 1996, vol. 50, No. 10, pp. 700-702 (English Abstract provided).
- Ambrosino, "Weaning and Respiratory Muscle Dysfunction: The Egg Chicken Dilemma," *Chest*, 2005, vol. 128(2), pp. 481-483.
- Messinger et al., "Using Tracheal Pressure to Trigger the Ventilator and Control Airway Pressure During Continuous Positive Airway Pressure Decreases Work of Breathing," *Chest*, 1995, vol. 108, No. 2, pp. 509-514.
- Prigent et al., "Comparative Effects of Two Ventilatory Modes on Speech in Tracheostomized Patients with Neuromuscular Disease," *Am J Respir Crit Care Med*. 2003, vol. 167, No. 8, pp. 114-119.
- Koska et al., "Evaluation of a fiberoptic system for airway pressure monitoring," *J. Clin Monit*, 1993, vol. 10, No. 4, pp. 247-250.
- Banner et al., "Imposed work of breathing and methods of triggering demand-flow, continuous positive airway pressure system," *Critical Care Medicine*, 1993, vol. 21, No. 2, pp. 183-190.
- Banner et al., "Site of pressure measurement during spontaneous breathing with continuous positive airway pressure: Effect on calculating imposed work of breathing," *Critical Care*, 1992, vol. 20, No. 4, pp. 528-533.
- Sinderby et al., "Neural control of mechanical ventilation in respiratory failure" *Nat Med.*, 1999; 5:1433-1436.
- Passy-Muir Inc., "Clinical Inservice Outline", Apr. 2004, 19 pages.
- Charlotte Regional Medical Center, "Application of the Passy-Muir Tracheostomy and Ventilator", Speech-Language Pathology Department, Jan. 1995, 8 pages.
- "Passy-Muir Speaking Valves," *Respiratory*, Nov. 13, 1998, 7 pages.
- Porta et al., "Mask proportional assist vs pressure support ventilation in patients in clinically stable condition with chronic ventilatory failure," *Chest*, 2002; 122(2), pp. 479-488.
- Prigent et al., "Comparative effects of two ventilatory modes on speech in tracheostomized patients with neuromuscular disease," *Am. J. Resp. Crit. Care Med.*, 2003; 167(8), pp. 114-119.
- Puente-Maestu et al., "Dyspnea, ventilatory pattern, and changes in dynamic hyperinflation related to the intensity of constant work rate exercise in COPD," *Chest*, 2005; 128(2), pp. 651-656.
- Ram et al., "Non-invasive positive pressure ventilation for treatment of respiratory failure due to exacerbations of chronic obstructive pulmonary disease," *Cochrane Database Syst Rev.*, 2004(3): 1-72.
- Rothe et al., "Near fatal complication of transtracheal oxygen therapy with the SCOOP(R) system," *Pneumologie*, 1996; 50(10), pp. 700-702.
- Rothfleisch et al., Facillation of ftheroptic nasotracheal intubation in a morbidly obese patient by simultaneous use of nasal CPAP, *Chest*, 1994 106(1): 287-288.
- Sanders et al., "CPAP via nasal mask: A treatment for occlusive sleep apnea," *Chest*, 1983; 83(9), pp. 144-145.
- Sinderby et al., "Neural control of mechanical ventilation in respiratory failure," *Nat. Med.*, 1999; 5(12), pp. 1433-1436.
- Somfayet al., "Dose-Response effect of oxygen on hyperinflation and exercise endurance in nonhypoxaemic COPD patients," *Eur. Resp. J.*, 2001; 18, pp. 77-84.
- Sullivan et al., "Reversal of obstructive sleep apnoea by continuous positive airway pressure applied through the nares," *The Lancet*, 1981; 1(8225), pp. 862-865.
- Sullivan, "Home treatment of obstructive sleep apnoea with continuous positive airway pressure applied through a nose-mask," *Bull Eur Physiopathol Respir.*, 1984; 20(1), pp. 49-54.
- Tiep et al., "Pulsed nasal and transtracheal oxygen delivery," *Chest*, 1990; 97, pp. 364-368.
- Tsuboi et al., "Ventilatory support during exercise in patients with pulmonary tuberculosis sequelae," *Chest*, 1997; 112(4), pp. 1000-1007.
- VHA/DOD Clinical Practice Guideline, "Management of chronic obstructive pulmonary disease," Aug. 1999, Ver. 1.1a, Updated Nov. 1999.
- Wijkstra et al., "Nocturnal non-invasive positive pressure ventilation for stable chronic obstructive pulmonary disease," *Cochrane Database Syst. Rev.*, 2002, 3: 1-22.
- Yaeger et al., "Oxygen therapy using pulse and continuous flow with a transtracheal catheter and a nasal cannula," *Chest*, 1994; 106, pp. 854-860.
- Walsh, "McGraw Hill pocket reference machinists' and metal-worker pocket reference," New York McGraw-Hill, 2000, pp. 3-67, submitting 3 pages.
- International preliminary report and written opinion on patentability for PCT/DE2004/001646, dated Jul. 3, 2006.
- European patent office search report dated Oct. 19, 2007 in co-pending EP04762494.
- International preliminary report and written opinion on patentability for PCT/US04/26800 dated Jun. 22, 2006.
- International preliminary report and written opinion on patentability for PCT/US07/12108, dated Aug. 8, 2008.
- International preliminary report and written opinion on patentability for PCT/US07/17400, dated Apr. 28, 2008.
- International preliminary report and written opinion on patentability for PCT/US08/64015, dated Sep. 26, 2008.
- International preliminary report and written opinion on patentability for PCT/US08/64164, dated Sep. 29, 2008.
- International preliminary report and written opinion on patentability for PCT/US08//8031, dated Nov. 24, 2008.
- International preliminary report and written opinion on patentability for PCT/US08/78033, dated Dec. 3, 2008.
- International preliminary report and written opinion on patentability for PCT/US09/054673, dated Oct. 8, 2009.
- International preliminary report and written opinion on patentability for PCT/US09/41027, dated Dec. 14, 2009.
- International preliminary report and written opinion on patentability for PCT/US09/59272, dated Dec. 2, 2009.
- International preliminary report and written opinion on patentability for PCT/US2006/036600, dated Apr. 3, 2007.
- International preliminary report and written opinion on patentability for PCT/US2009/031355 dated Mar. 11, 2009.
- International preliminary report and written opinion on patentability for PCT/US2009/041034, dated Jun. 10, 2009.
- International preliminary report and written opinion on patentability for PCT/US2010/029871, dated Jul. 12, 2010.
- International preliminary report and written opinion on patentability for PCT/US2010/029873, dated Jun. 28, 2010.
- International preliminary report and written opinion on patentability for PCT/US2010/029874, dated Jul. 12, 2010.
- International preliminary report and written opinion on patentability for PCT/US/2010/029875, dated Jul. 12, 2010.
- International preliminary report and written opinion on patentability for PCT/US2010/047920, dated Nov. 1, 2010.
- International preliminary report and written opinion on patentability for PCT/US2010/047921, dated Jan. 27, 2011.
- International search report for PCT/De2004/001646, dated Jan. 17, 2005.
- In the U.S. Patent and Trademark Office, Supplemental Notice of Allowance dated in re: U.S. Appl. No. 10/771,803, dated Dec. 2, 2008, 2 pages.
- In the U.S. Patent and Trademark Office, Supplemental Notice of Allowance dated in re: U.S. Appl. No. 10/771,803, dated Nov. 7, 2008, 2 pages.

(56)

## References Cited

## OTHER PUBLICATIONS

In the U.S. Patent and Trademark Office, Examiner's Interview Summary in re: U.S. Appl. No. 10/771,803, dated Oct. 31, 2008, 4 pages.

In the U.S. Patent and Trademark Office, Supplemental Notice of Allowance dated in re: U.S. Appl. No. 10/771,803, dated Oct. 20, 2008, 8 pages.

In the U.S. Patent and Trademark Office, Examiner's Interview Summary in re: U.S. Appl. No. 10/771,803, dated Nov. 2, 2007, 2 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 10/771,803, dated Jun. 14, 2007, 12 pages.

In the U.S. Patent and Trademark Office, Restriction Requirement in re: U.S. Appl. No. 12/271,484, dated Feb. 9, 2011, 5 pages.

In the U.S. Patent and Trademark Office, Restriction Requirement in re: U.S. Appl. No. 12/754,437, dated Aug. 16, 2011, 5 pages.

In the U.S. Patent and Trademark Office, Non-Final Office Action re: U.S. Appl. No. 10/567,746, dated Oct. 5, 2009, 9 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance and Examiner's Interview Summary in re: U.S. Appl. No. 11/523,519, dated Jan. 16, 2009, 10 pages.

In the U.S. Patent and Trademark Office, Examiner's Interview Summary in re: U.S. Appl. No. 11/523,519, dated Jan. 13, 2009, 4 pages.

In the U.S. Patent and Trademark Office, Non Final Office Action re: U.S. Appl. No. 11/523,519, dated Jul. 11, 2008, 13 pages.

In the U.S. Patent and Trademark Office, Examiner's Interview Summary in re: U.S. Appl. No. 11/523,519, dated Apr. 10, 2008, 3 pages.

In the U.S. Patent and Trademark Office, Final Office Action re: U.S. Appl. No. 11/523,519, dated Nov. 26, 2007, 14 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 11/523,519, dated Mar. 7, 2007, 11 pages.

In the U.S. Patent and Trademark Office, Restriction Requirement in re: U.S. Appl. No. 11/523,518, dated Dec. 30, 2009, 4 pages.

In the U.S. Patent and Trademark Office, Supplemental Notice of Allowance dated in re: U.S. Appl. No. 11/798,965, dated Aug. 21, 2009, 4 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance dated in re: U.S. Appl. No. 11/798,965, dated Jul. 17, 2009, 5 pages.

In the U.S. Patent and Trademark Office, Final Office Action re: U.S. Appl. No. 11/798,965, dated Apr. 9, 2009, 6 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 11/798,965, dated Jul. 29, 2008, 12 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 12/578,283, dated Oct. 19, 2011, 5 pages.

In the U.S. Patent and Trademark Office, Restriction/Election Requirement in re: U.S. Appl. No. 11/882,530, dated Apr. 27, 2011, 5 pages.

In the U.S. Patent and Trademark Office, Supplemental Notice of Allowance dated in re: U.S. Appl. No. 10/870,849, dated Jun. 16, 2009, 2 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance dated in re: U.S. Appl. No. 10/870,849, dated Jun. 3, 2009, 4 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance dated in re: U.S. Appl. No. 10/870,849, dated May 14, 2009, 8 pages.

In the U.S. Patent and Trademark Office, Restriction in re: U.S. Appl. No. 10/870,849, dated Nov. 16, 2007, 5 pages.

In the U.S. Patent and Trademark Office, Examiner's Interview Summary in re: U.S. Appl. No. 10/870,849, dated Jul. 27, 2007, 2 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 10/870,849, dated Feb. 22, 2007, 13 pages.

In the U.S. Patent and Trademark Office, Restriction/Election Requirement in re: U.S. Appl. No. 12/493,677, dated Aug. 5, 2011, 5 pages.

In the U.S. Patent and Trademark Office, Restriction/Election Requirement in re: U.S. Appl. No. 12/4153,423, dated Oct. 6, 2011, 8 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance dated in re: U.S. Appl. No. 10/922,054, dated Feb. 12, 2008, 6 pages.

In the U.S. Patent and Trademark Office, Final Office Action re: U.S. Appl. No. 10/922,054, dated Nov. 27, 2007, 9 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 10/922,054, dated Mar. 14, 2007, 14 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 10/922,054, dated Sep. 7, 2006, 21 pages.

In the U.S. Patent and Trademark Office, Restriction Requirement in re: U.S. Appl. No. 10/922,054, dated May 17, 2006, 5 pages.

In the U.S. Patent and Trademark Office, Notice of Allowance dated in re: U.S. Appl. No. 12/076,062, dated Nov. 2, 2011, 7 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 12/076,062, dated Jan. 13, 2011, 14 pages.

In the U.S. Patent and Trademark Office, Office Action in re: U.S. Appl. No. 12/355,753, dated Sep. 28, 2011, 32 pages.

In the U.S. Patent and Trademark Office, Ex Parte Quayle Office Action in re: U.S. Appl. No. 29/388,700, dated Oct. 7, 2011, 5 pages.

"AARC Clinical Practice Guideline: Oxygen Therapy in the Home or Extended Care Facility," *Resp. Care*, 1992, 37(8), pp. 918-922.

"ATS Statement: Guidelines for the Six-Minute Walk Test," *Am. J. Respir. Crit. Care Med.*, 2002., 166, pp. 111-117.

Ambrosino, "Exercise and noninvasive ventilatory support," *Monaldi Arch Chest Dis.*, 2000, 55(3), pp. 242-246.

Ambrosino, "Weaning and Respiratory Muscle Dysfunction: The Egg Chicken Dilemma," *Chest*, 2005: 128(2), pp. 481-483.

Bach et al., "Intermittent Positive Pressure Ventilation via Nasal Access in the Management of Respiratory Insufficiency," *Chest*, 1987: 92(1), pp. 168-170.

Banner et al., "Extubating at a Pressure Support Ventilation Level Corresponding to Zero Imposed Work of Breathing," *Anesthesiology*, Sep. 1994: 81(3A), pp. A271.

Banner et al., "Imposed Work of Breathing and Methods of Triggering a Demand-Flow, Continuous Positive Airway Pressure System," *Critical Care Medicine*, 1993: 21(2), pp. 183-190.

Banner et al., "Site of Pressure Measurement During Spontaneous Breathing with Continuous Positive Airway Pressure: Effect on Calculating Imposed Work of Breathing," *Critical Care Medicine*, 1992: 20(4), pp. 528-533.

Barakat et al., "Effect of noninvasive ventilatory support during exercise of a program in pulmonary rehabilitation in patients with COPD," *Int. J. Chron. Obstruct. Pulmon. Dis.*, 2007: 2(4), pp. 585-591.

Barreiro et al., Noninvasive ventilation, *Crit Care Clin.*, 2007: 23(2): 201-22.

Bauer et al., "ADAM nasal CPAP Circuit Adaptation: A Case Report," *Sleep*, 1991: 14(3), pp. 272-273.

Blanch, "Clinical Studies of Tracheal Gas Insufflation," *Resp. Care*, 2001: 45(2), pp. 158-166.

Borghi-Silva et al., "Non-invasive ventilation improves peripheral oxygen saturation and reduces fatigability of quadriceps in patients with COPD," *Respirology*, 2009, 14:537-546.

Bossi et al., "Continuous Positive Airway Pressure in the Spontaneously Breathing Newborn by Means of Bilateral Nasal Cannulation," *Monatsschr Kinderheilkd*, 1975: 123(4), pp. 141-146.

Boussarsar et al., "Relationship between ventilatory settings and barotrauma in the acute respiratory distress syndrome," *Intensive Care Med.*, 2002: 28(4), 406-13.

Chang et al., "Reduced Inspiratory muscle Endurance Following Successful Weaning From Prolonged Mechanical Ventilation," *Chest*, 2005: 128(2), pp. 553-559.

Charlotte Regional Mediocl Center, "Application of the Passy-Muir Tracheostomy and Ventilator," *Speech-Language Pathology Department*, Jan. 1995, 8 pages.

Christopher et al., "Preliminary Observations of Transtracheal Augmented Ventilation for Chronic Severe Respiratory Disease," *Resp. Care*, 2001: 46(1), pp. 15-25.

Christopher, et al. "Transtracheal Oxygen Therapy for Refractory Hypoxemia," *JAMA*, 1986: 256(4), pp. 494-497.

Ciccolella et al.; "Administration of High-Flow, Vapor-phased, Humidified Nasal Cannula Air (HF-HNC) Decreases Work of

(56)


**References Cited**

## OTHER PUBLICATIONS



- Breathing (WOB) in Healthy Subjects During Exercise," *AmJRCCM*, Apr. 2001: 163(5), Part 2, pp. A622. (Abstract Only).
- Clini et al., "The Italian multicentre study on noninvasive ventilation in chronic obstructive pulmonary disease patients," *Eur. Respir. J.*, 2002, 20(3): 529-538.
- Costa et al., "Influence of noninvasive ventilation by BiPAP on exercise tolerance and respiratory muscle strength in chronic obstructive pulmonary disease patients (COPD)," *Rev. Lat. Am. Enfermagem.*, 2006: 14(3), pp. 378-382.
- Diaz et al., "Breathing Pattern and Gas Exchange at Peak Exercise in COPD Patients with and without Tidal Flow Limitation at Rest," *European Respiratory Journal*, 2001: 17, pp. 1120-1127.
- Enright, "The six-minute walk test," *Resp. Care*, 2003: 8, pp. 783-785.
- Ferreira et al., "Trigger Performance of Mid-level ICU Mechanical Ventilators During Assisted Ventilation: A Bench Study," *Intensive Care Medicine*, 2008, 34: 1669-1675.
- Fink, "Helium-Oxygen: An Old Therapy Creates New Interest," *J. Resp. Care. Pract. now RT for Decision Makers in Respiratory Care*, 1999, pp. 71-76.
- Gaughan et al. "A Comparison in a Lung Model of Low-and High-Flow Regulators for Transtracheal Jet Ventilation," *Anesthesiology*, 1992: 77(1), pp. 189-199.
- Gregoretti, et al., "Transtracheal Open Ventilation in Acute Respiratory Failure Secondary to Severe Chronic Obstructive Pulmonary Disease Exacerbation," *Am. J. Resp. Crit. Car. Med.*, 2006: 173(8), pp. 877-881.
- Haenel et al., "Efficacy of Selective Intrabronchial Air Insufflation in Acute Lobar Colapse," *Am. J. Surg.*, 1992: 164(5), pp. 501-505.
- Keilty et al., "Effect of inspiratory pressure support on exercise tolerance and breathlessness in patients with severe stable chronic obstructive pulmonary disease," *Thorax*, 1994, 49(10): 990-994.
- Kohnlein et al., "Noninvasive ventilation in pulmonary rehabilitation of COPD patients," *Respir. Med.*, 2009, 103: 1329-1336.
- Koska et al. "Evaluation of a Fiberopic System for Airway Pressure Monitoring," *J. Clin. Monit.*, 1993: 10(4), pp. 247-250.
- Lewis, "Breathless No More, Defeating Adult Sleep Apnea," *FDA Consumer Magazine*, Jun. 1992, pp. 33-37.
- Limberg et al., "Changes in Supplemental Oxygen Prescription in Pulmonary Rehabilitation," *Resp. Care*, 2006: 51(11), p. 1302.
- MacIntyre, "Long-Term Oxygen Therapy; Conference Summary," *Resp. Care*, 2000: 45(2), pp. 237-245.
- MacIntyre et al., "Acute exacerbations and respiratory failure in chronic obstructive pulmonary disease," *Proc. Am. Thorac. Soc.*, 5(4), pp. 530-535.
- Massie et al., "Clinical Outcomes Related to Interface Type in Patients with Obstructive Sleep Apnea/Hypopnea Syndrome Who are Using Continuous Positive Airway Pressure," *Chest*, 2003: 123(4), pp. 1112-1118.
- McCoy, "Oxygen Conservation Techniques and Devices," *Resp. Care*, 2000: 45(1), pp. 95-104.
- McGinley, "A nasal cannula can be used to treat obstructive sleep apnea"; *Am. J. Resp. Grit. Care Med.*, 2007: 176(2) pp. 194-200.
- Menadue et al., "Non-invasive ventilation during arm exercise and ground walking in patients with chronic hypercapnic respiratory failure," *Respirology*, 2009, 14(2): 251-259.
- Menon et al., "Tracheal Perforation. A Complication Associated with Transtracheal Oxygen therapy," *Chest*, 1993: 104(2), pp. 636-637.
- Messinger et al., "Tracheal Pressure Triggering a Demand-Flow CPAP System Decreases Work of Breathing," *Anesthesiology*, 1994: 81(3A) p. A272.
- Mettey, "Use of CPAP Nasal Cannula for Aids of the Newborns in Tropical Countries," *Medecine Tropicale*, 1985: 45(1), pp. 87-90.
- Nahmias et al., "Treatment of the Obstructive Sleep Apnea Syndrome Using a Nasopharyngeal Tube", *Chest*, 1988: 94(6), pp. 1142-1147.
- Nava et al., "Non-invasive ventilation," *Minerva Anesthesiol.*, 2009: 75(1-2), pp. 31-36.
- Peters et al., "Combined Physiological Effects of Bronchodilators and Hyperoxia on Exertional Dyspnea in Normoxic COPD," *Thorax*, 2006: 61, pp. 559-567.
- Polkey et al., "Inspiratory pressure support reduces slowing of inspiratory muscle relations rate during exhaustive treadmill walking in sever COPD," *Am. J. Resp. Crit. Care Med.*, 1996: 154(4,10), pp. 1146-1150.
- Examination Report for Indian Patent Application No. 7348/CHENP/2009, dated Nov. 24, 2017.

\* cited by examiner


PRIOR ART  
FIG. 1A

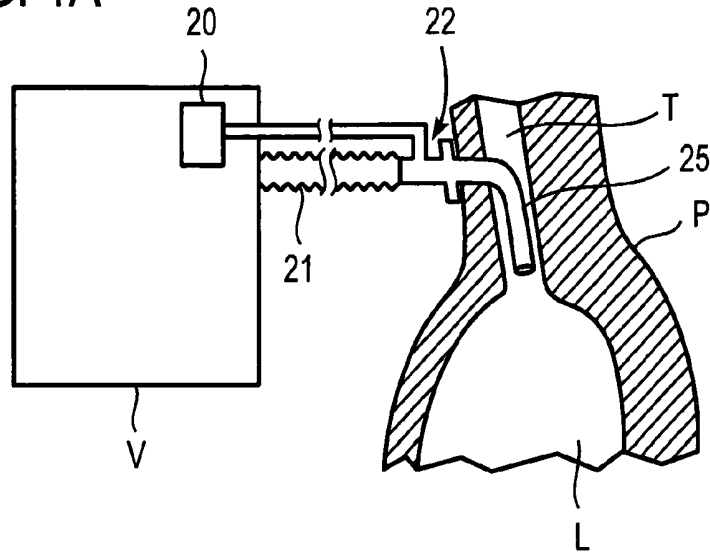


PRIOR ART  
FIG. 1B

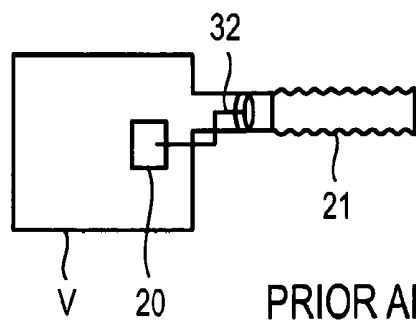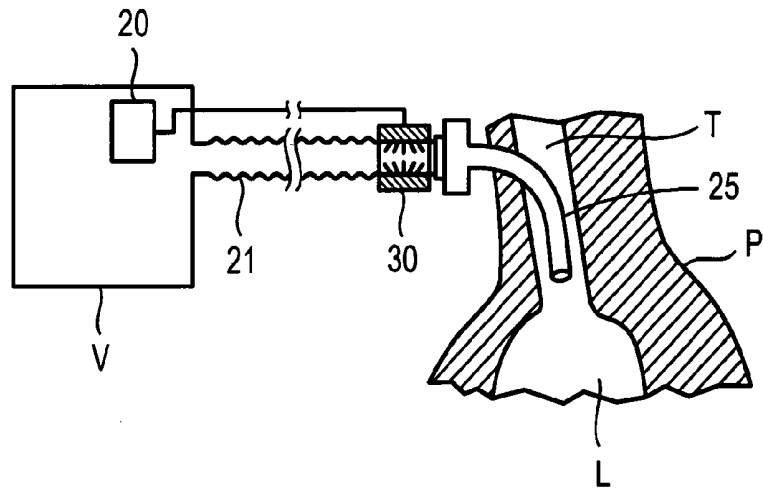


PRIOR ART  
FIG. 1C

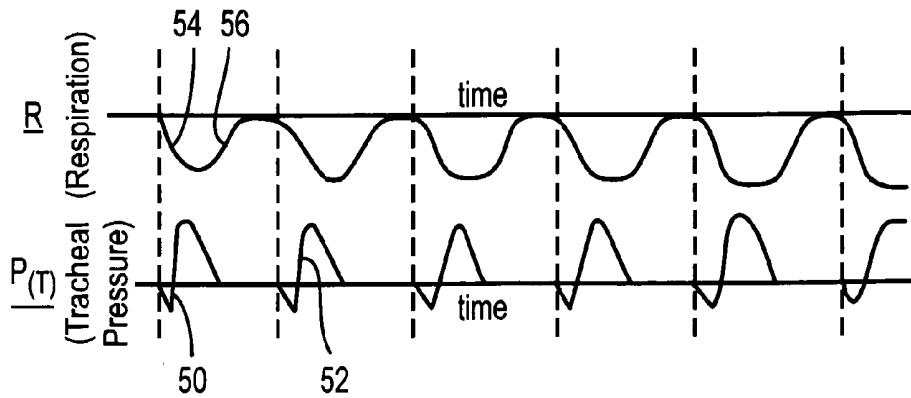


PRIOR ART  
FIG. 1D

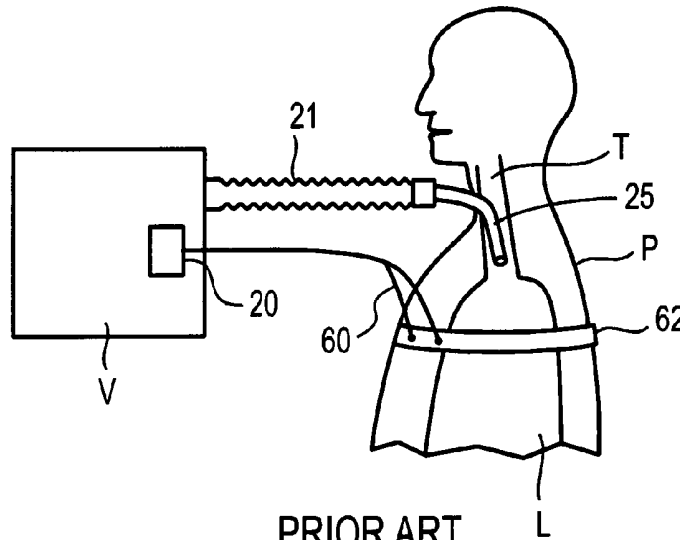


PRIOR ART  
FIG. 2A

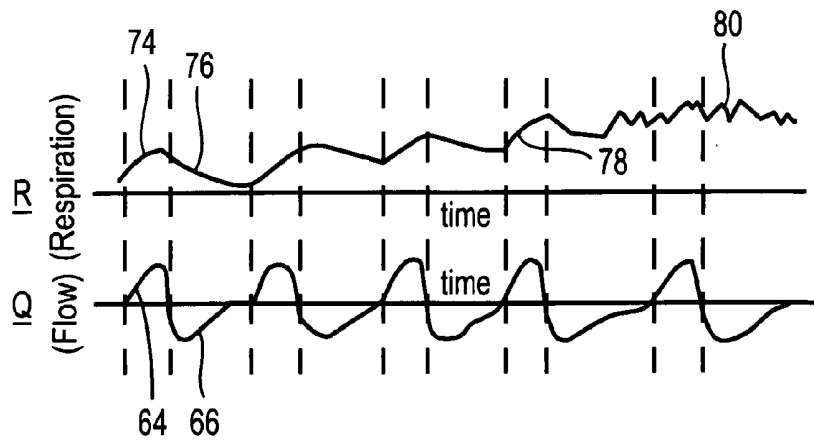

PRIOR ART  
FIG. 2B

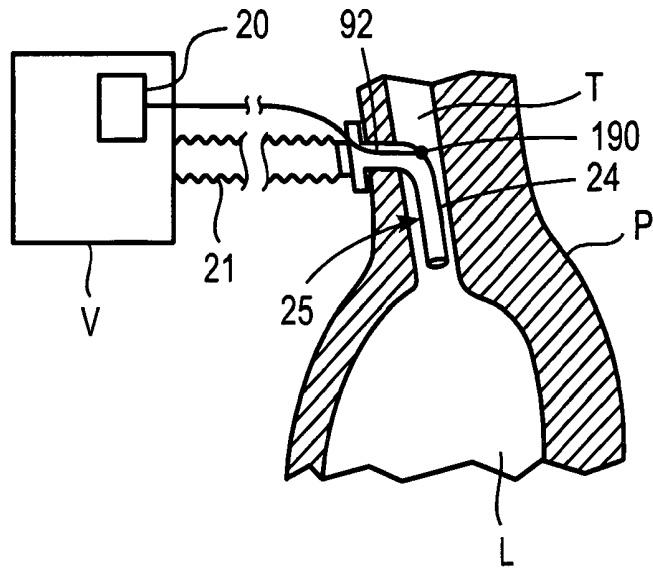

PRIOR ART  
FIG. 3A

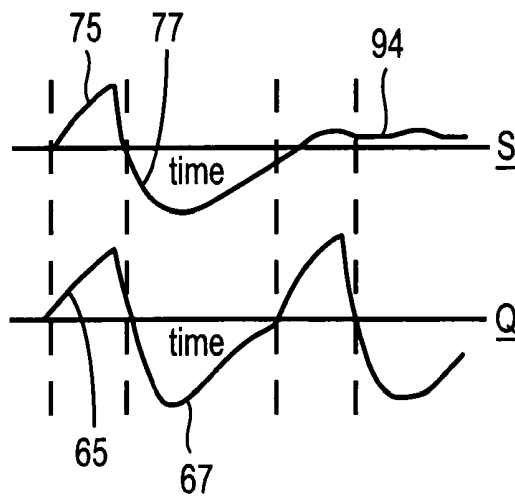

PRIOR ART  
FIG. 3B

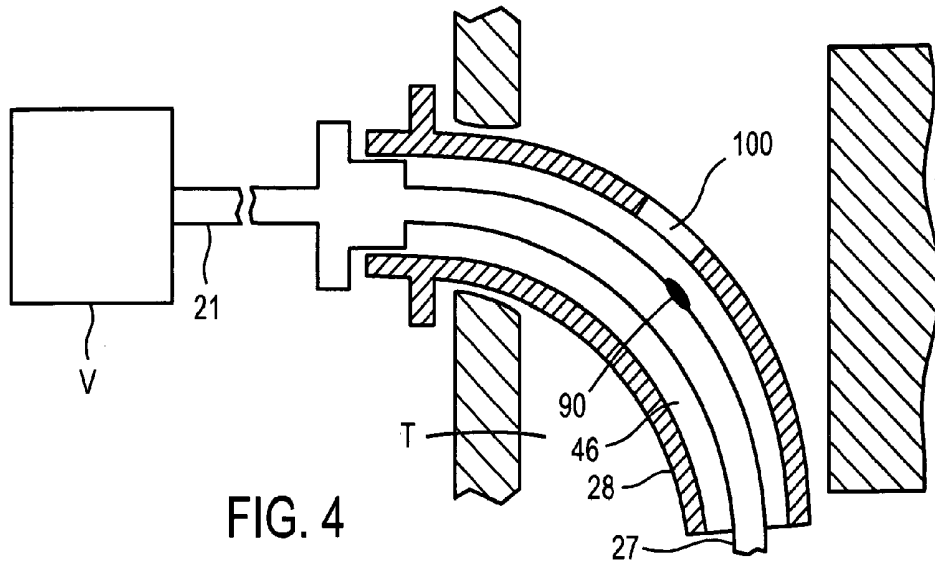


FIG. 4

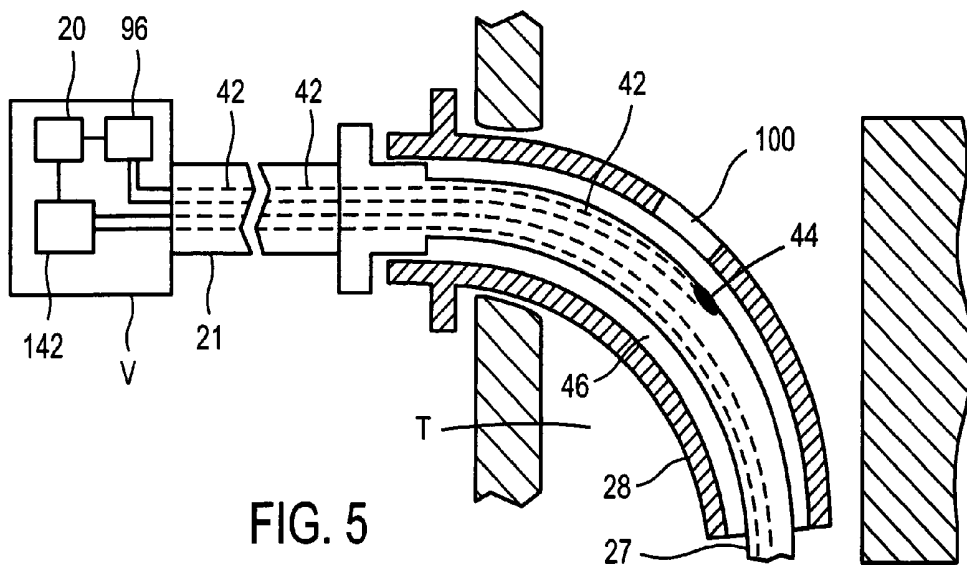
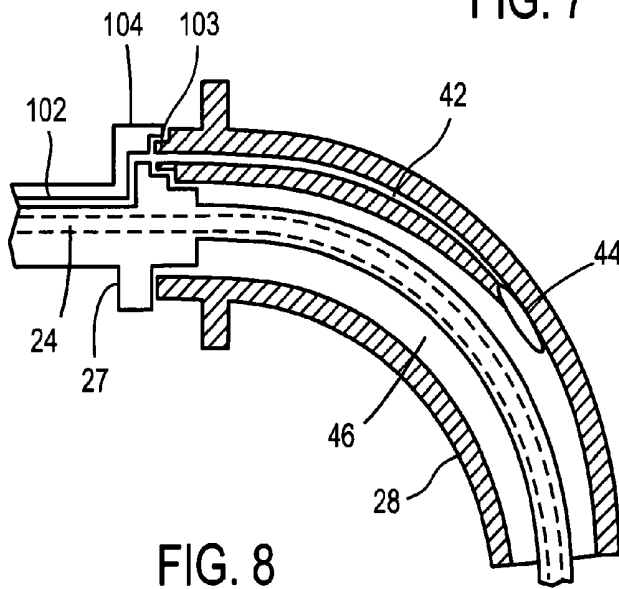
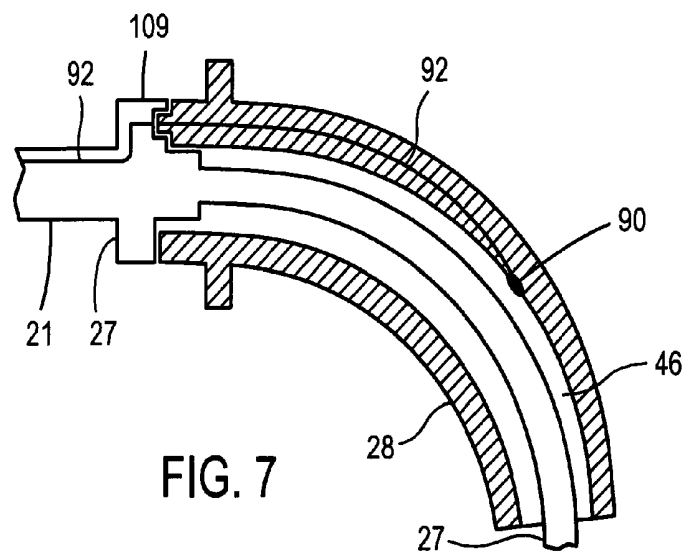
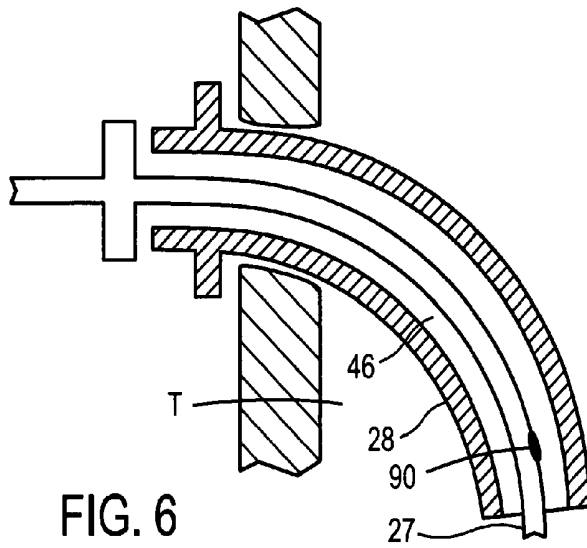


FIG. 5



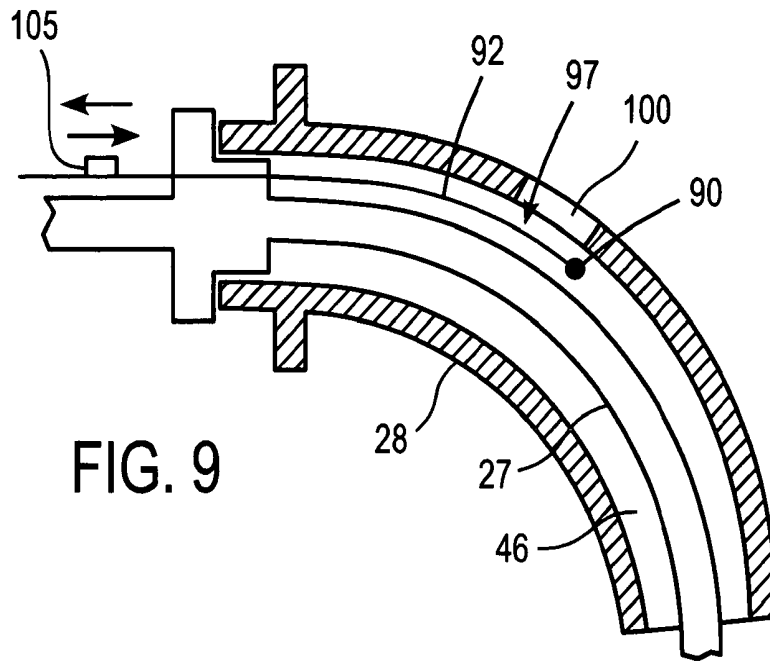


FIG. 9

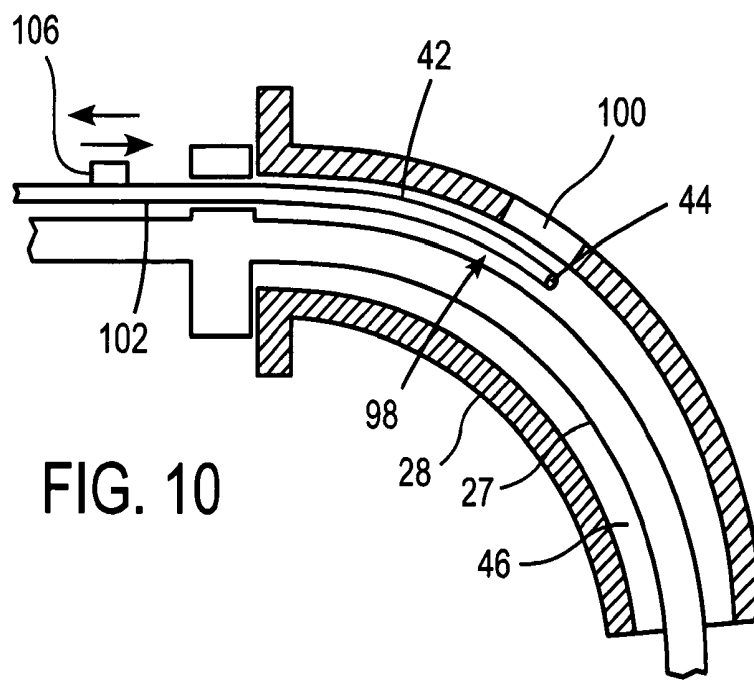


FIG. 10

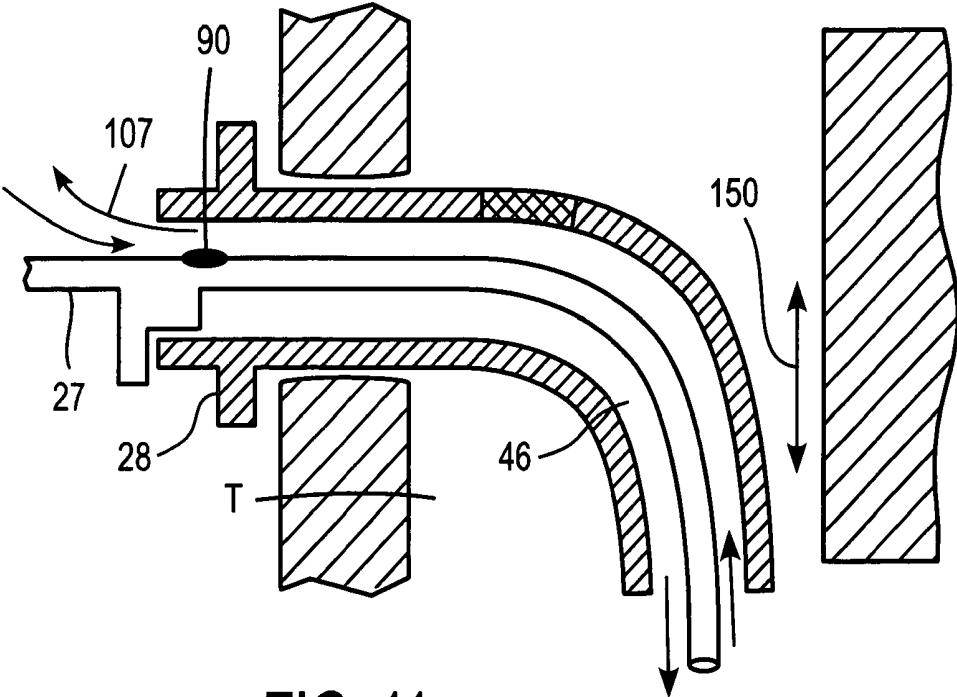
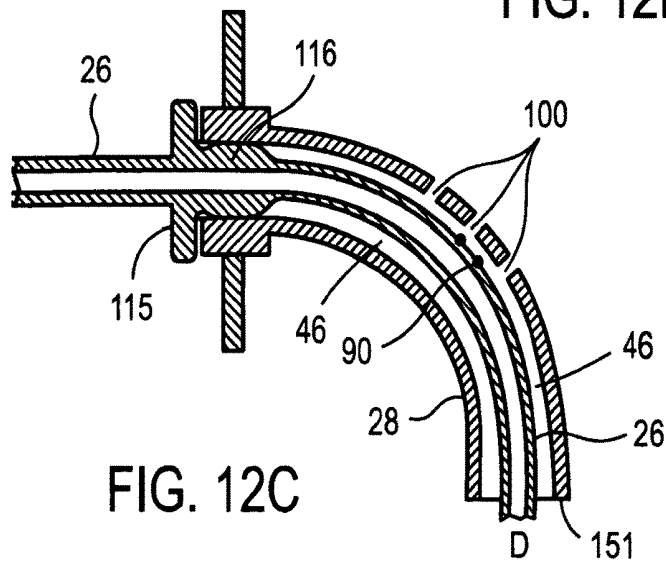
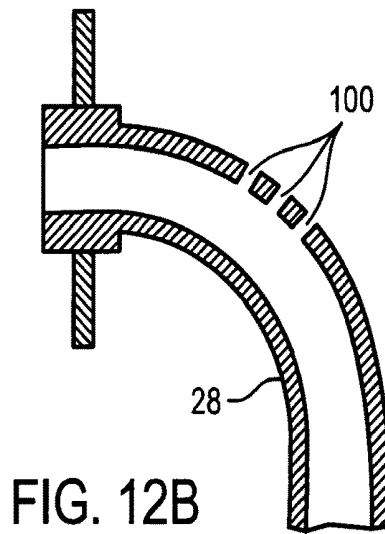
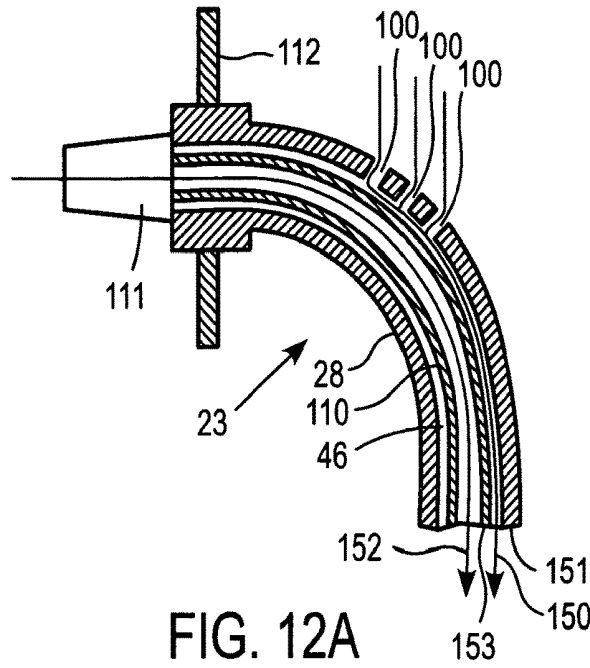


FIG. 11



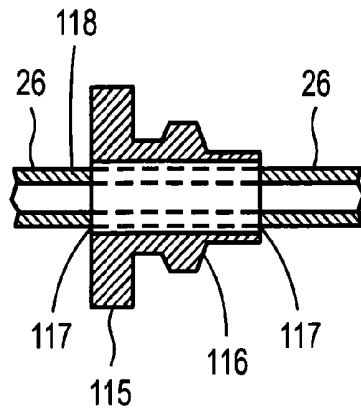


FIG. 13

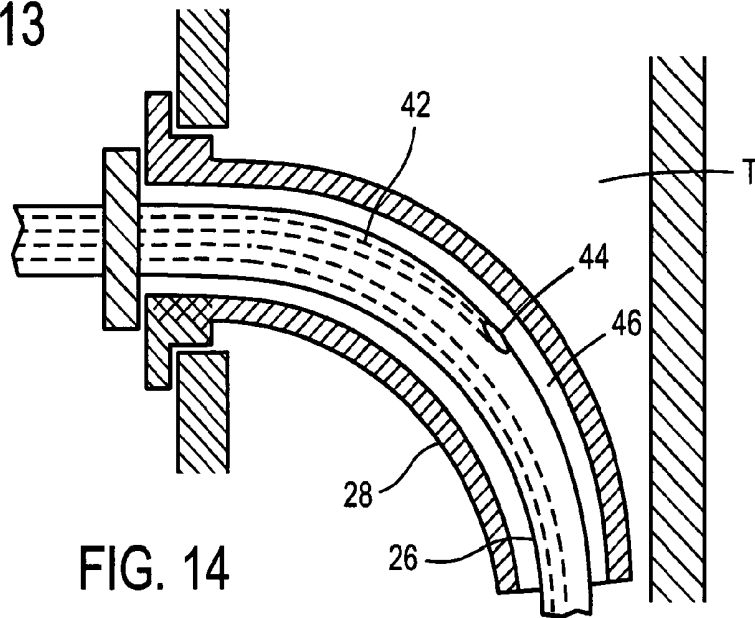


FIG. 14

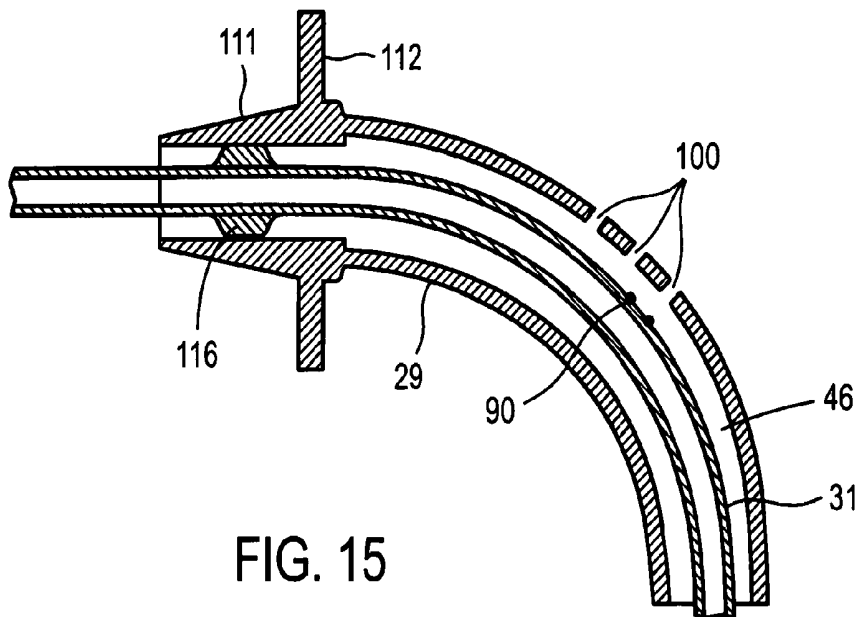


FIG. 15

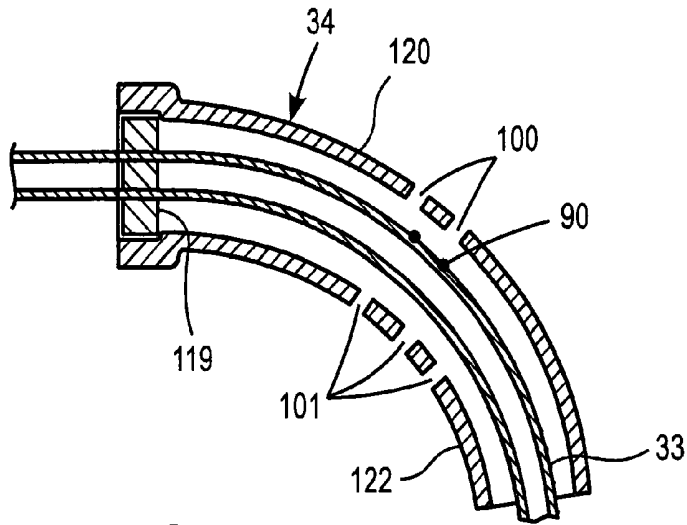


FIG. 16

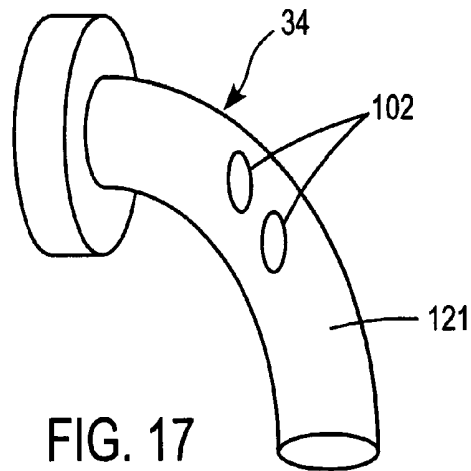


FIG. 17

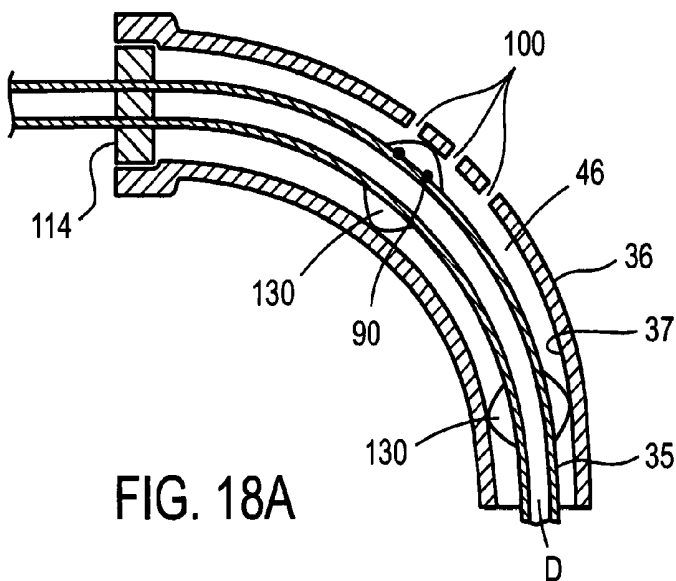


FIG. 18A




FIG. 18B

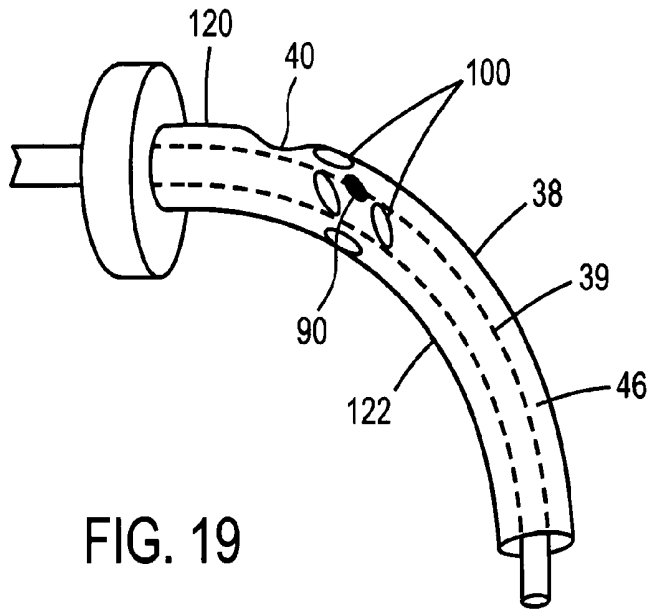


FIG. 19

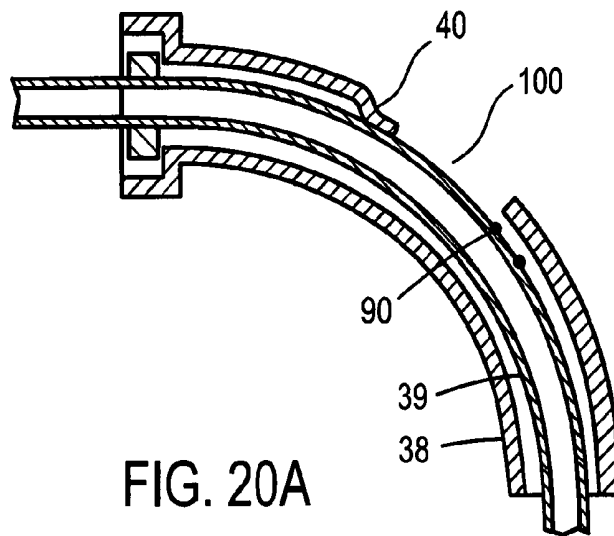


FIG. 20A

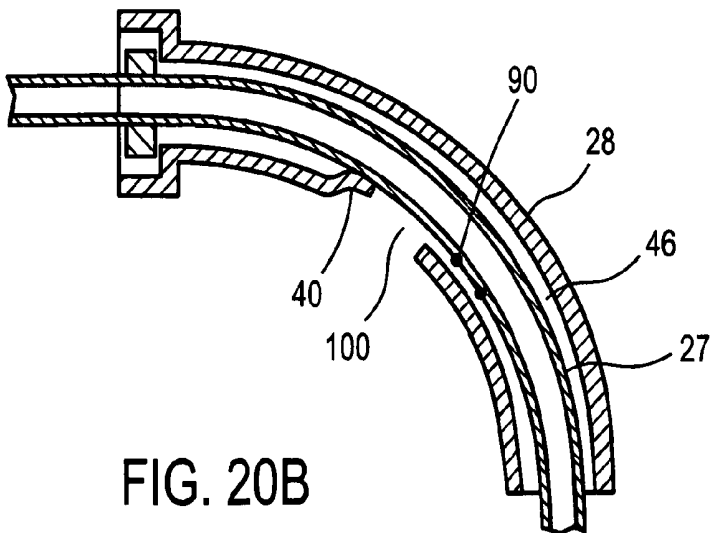
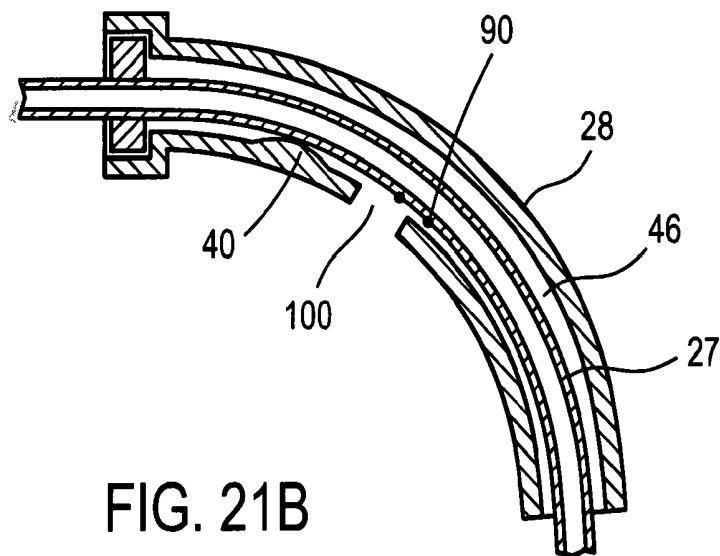
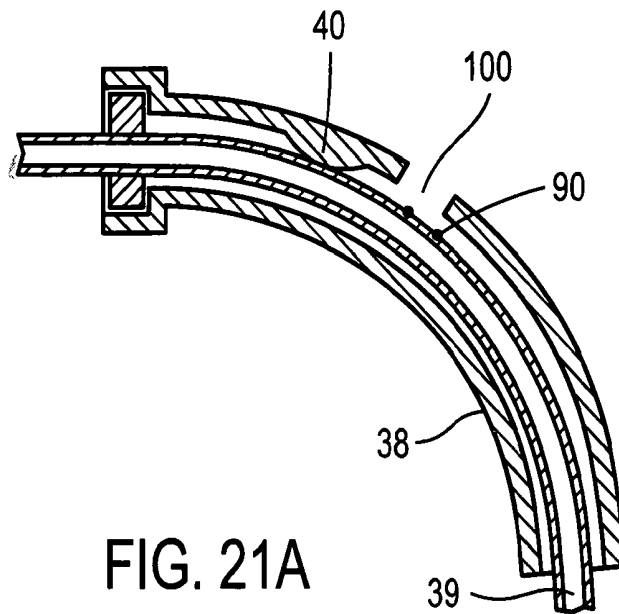
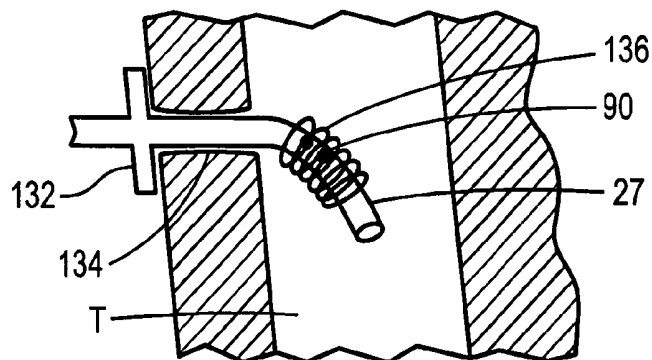
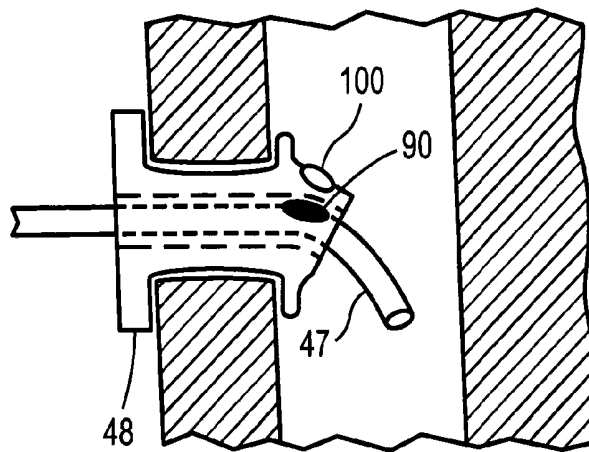
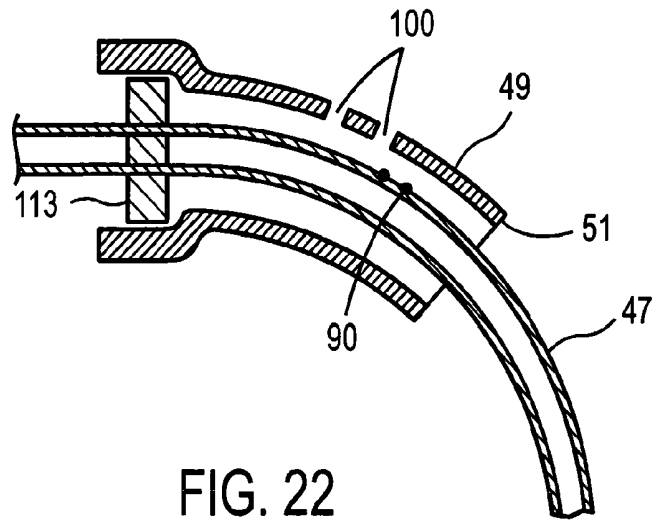


FIG. 20B






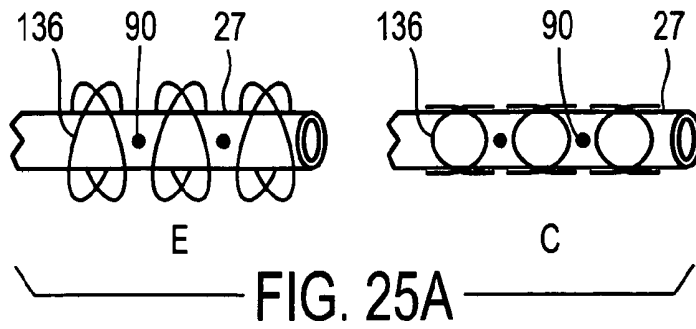
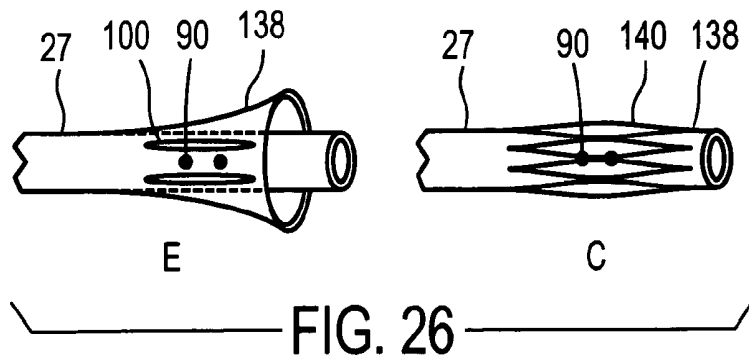


FIG. 25B



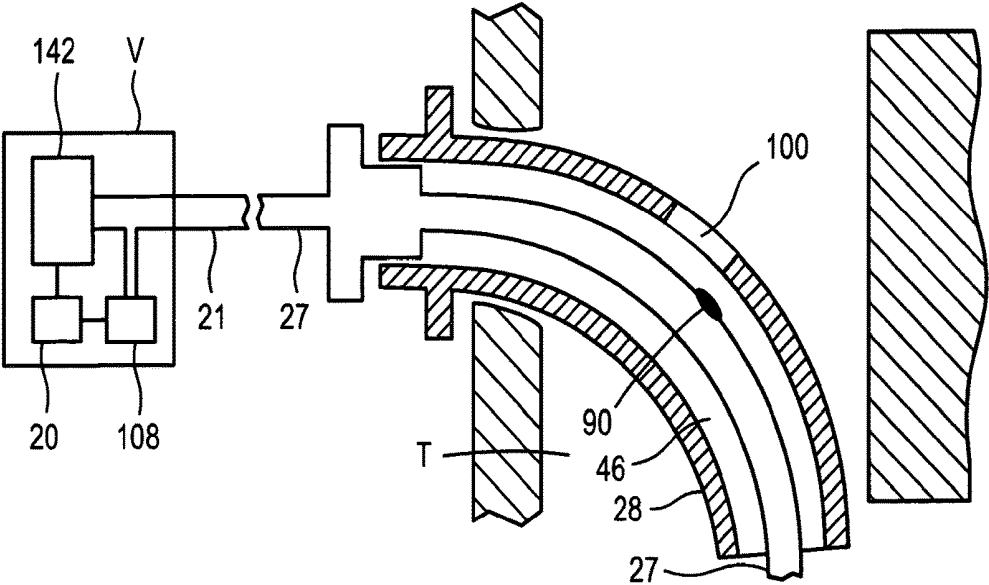


FIG. 27

## METHODS AND DEVICES FOR SENSING RESPIRATION AND PROVIDING VENTILATION THERAPY

### CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a divisional of U.S. patent application Ser. No. 12/153,423 which claims priority to U.S. Provisional Patent Application Ser. No. 60/924,514, filed May 18, 2007, the disclosure of which is hereby incorporated by reference in its entirety. This application further incorporates by reference in their entireties: U.S. Non-Provisional patent application Ser. No. 10/771,803 (U.S. Pat. No. 7,487,778, issued on Feb. 10, 2009), filed Feb. 4, 2004; U.S. Non-Provisional patent application Ser. No. 10/870,849 (U.S. Pat. No. 7,588,033, issued on Sep. 15, 2009), filed on Jun. 17, 2004, U.S. Non-Provisional patent application Ser. No. 11/523,519 (U.S. Pat. No. 7,533,670 issued on May 19, 2009), filed Sep. 20, 2006 and U.S. Non-Provisional patent application Ser. No. 11/523,518, filed Sep. 20, 2006.

### FIELD OF THE INVENTION

The present invention relates to ventilation therapy for persons suffering from respiratory impairment and breathing disorders, such as chronic obstructive pulmonary disease (COPD), pulmonary fibrosis, acute respiratory distress syndrome (ARDS), neuromuscular impairment, sleep apnea and/or other related conditions. More specifically, the present invention relates to accurately and reliably measuring a patient's respiratory pattern using breath sensing, including providing methods, systems and apparatus to protect breath sensors.

### STATEMENT RE: FEDERALLY SPONSORED RESEARCH/DEVELOPMENT

Not Applicable

### BACKGROUND

There are two general types of control systems for conventional ventilators. A first type is delivery of gas to a patient based on a frequency selected by the clinician. The frequency selected delivery is independent of patient activity. This control system is used when the patient is non-alert, sedated, unresponsive or paralyzed. In this type of system the ventilator is breathing for the patient. A second type of control system is delivery of gas to the patient in response to an inspiratory effort created by the patient. This type of ventilation helps the patient breathe. There are also ventilators and modes of ventilation that combine the two types of control systems.

In the case of a control system that responds to patient breathing effort, breath effort sensors are required to detect inspiration. In basic conventional systems, the breath sensors detect the start of inspiration using a pressure or flow sensor. The inspiratory effort sensor is located somewhere in the path of ventilation gas delivered by a ventilation gas delivery circuit. A ventilation gas delivery circuit is generally defined as the path of respiration gas delivered by a ventilator. The inspiratory effort sensor may be either inside the ventilator, or in the tubing between the ventilator and the patient, including at the patient end of the tubing. Various attempts have been made to place the inspiratory effort sensor(s) inside the patient, or externally attached to the

patient to improve breath effort detection and/or improve response time of the ventilator gas delivery.

Pressure or flow sensors within the ventilation gas delivery circuit have successfully been used to detect the start of inspiration to trigger the ventilator to deliver gas to the patient. However, when there is a need or desire to measure the entire respiratory curve in addition to start of inspiration, sensors within the ventilation gas delivery circuit produce inadequate results because the gas being delivered by the ventilator also moves past the sensor. Thus, the sensor no longer measures the patient's respiration, but rather the gas delivered through the ventilation gas circuit. In a closed ventilation system, the ventilator activity approximates the overall lung activity, hence this positioning of sensors may be adequate. In an open ventilation system, or in ventilation systems that augment a patient's spontaneous breathing, sensors within the ventilation gas delivery circuit are inadequate in measuring the entire respiratory curve.

Sensors not within the ventilator gas delivery circuit have the ability to measure the entire respiration activity. For example, chest impedance sensors can be used to measure the entire respiratory curve of a patient and to use that signal to control the ventilator and synchronize the ventilator to the patient's breathing. Although an improvement, this approach has the disadvantage that the chest impedance signal is prone to drift, noise and artifacts caused by patient motion and abdominal movement. In another technology, neural activity related to the respiratory drive is used to measure the respiration of a patient. However, this has the disadvantage that it is invasive and requires electrodes typically placed in the esophagus to detect the neural activity.

U.S. Non-Provisional patent application Ser. No. 10/870,849 (U.S. Printed Publication 2005/0034721), which is incorporated by reference in its entirety above, describes a new form of breath sensing with sensors not within a ventilation gas delivery circuit. The sensors may be located in the airway of a patient, for example, in the patient's trachea, but not within the ventilation gas delivery circuit. In this manner, the gas delivery from the ventilator may not dominate the sensor measurements. This intra-airway sensor may measure naturally inspired gas flow of the patient, naturally exhaled gas flow of the patient, and the effect of the ventilator gas delivery on lung volumes. The sensor may not measure gas flowing in the ventilator delivery circuit as in conventional systems. This breath sensing method may then measure, not just the start of inspiration, but the entire respiratory pattern of the patient. This may be advantageous to optimize the synchrony of the ventilator to the patient's natural breath pattern, so that the patient is comfortable. Also, if the goal is to provide therapy during different portions of the respiratory curve, such as during the middle of inspiration, or during a particular part of the expiratory phase, then this method may be used to accurately measure the entire respiratory curve. This new breath sensing technology, however, may not be simple or obvious to reduce to practice. Sensors within the airway of the patient are prone to problems stemming from tissue interaction, patient-to-patient variability, variability within a given patient over time, and a variable physiological environment that can not be controlled. For example, debris in the airway may collect on the sensors and may cause signal artifacts and disrupt the sensors' ability to accurately and reliably measure the entire breath curve. Or, the sensor could come into contact with the tracheal wall, which may disrupt the sensors' signal. Alternatively, tracheal movement during breathing can affect the signal.

Need exists for improved breath sensing systems and methods for ensuring reliable and accurate breath measurements.

#### BRIEF SUMMARY

The present invention may be directed to methods and systems for intra-airway breath sensors, especially those sensors not within a ventilation gas delivery circuit, but exposed to a patient's spontaneous respiration airflow. The present invention is an improvement over existing breath sensing techniques. Further, apparatus and methods for shielding and protecting the intra-airway sensors from disruptions such as contacting tissue or accumulating debris are provided.

One aspect of the invention is directed to a breath sensing and ventilation delivery apparatus comprising: a catheter, one or more intra-airway breath sensors coupled to an outer surface of the catheter, and an airflow permeable protector with a proximal end adapted to be positioned outside a patient and a distal end adapted to be placed in an airway of the patient, wherein the airflow permeable protector at least partially surrounds the catheter such that the airflow permeable protector prevents the one or more intra-airway breath sensors from contacting a tissue and reduces accumulation of debris on the one or more intra-airway breath sensors. The airflow permeable protector may be a tracheostomy tube cannula. The cannula may have one or more fenestrations. The cannula may at least partially surround the catheter forming an annular space between the cannula and the catheter. The airflow permeable protector may be a protective shield. The protective shield may be selected from the group consisting of a shield tapered on at least one end, a shield collapsible against an outer surface of the ventilation catheter, stoma sleeve, and combinations thereof. The one or more intra-airway breath sensors may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention is directed to a breath sensing and ventilation delivery apparatus comprising: a ventilation catheter, a tracheostomy tube cannula with one or more fenestrations, wherein the cannula at least partially surrounds the ventilation catheter to create an annular space between an inner diameter of the cannula and an outer diameter of the ventilation catheter, and one or more intra-airway breath sensors within the annular space between an inner diameter of the cannula and an outer diameter of the ventilation catheter. The ventilation catheter may extend beyond a distal portion of the cannula and into an airway. A positioner may be provided for positioning the ventilation catheter at a predetermined position within the cannula. The positioner may be a basket-type device. The positioner may be a deflector in a wall of the cannula. An anchor may be provided for preventing movement of a distal tip of the ventilation catheter. The one or more fenestrations may be located in a position selected from the group consisting of a superior side of the cannula, an inferior side of the cannula, a lateral side of the outer cannula, and combinations thereof. The one or more intra-airway breath sensors may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, tubes with sensing lumen, sensing subassemblies, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combina-

tions thereof. The one or more intra-airway breath sensors may be multiple elements placed in an array, wherein one element is used as a reference signal. The one or more intra-airway breath sensors may be coupled to the ventilation catheter. The one or more intra-airway breath sensors may be coupled to the cannula. The one or more intra-airway breath sensors may be de-coupled from the ventilation catheter and the cannula. The one or more intra-airway breath sensors may be a sensing lumen not in communication with a ventilation catheter gas delivery circuit, wherein the sensing lumen comprises a sensing element and a port positioned in the annular space and wherein the sensing element is located external to a body and communicating with the sensing lumen. The ventilation catheter may be removable from the cannula. A seal may be provided between the cannula and the ventilation catheter at a location proximal to the one or more intra-airway breath sensors. The ventilation catheter may comprise a moveable connection with the cannula.

Another aspect of the invention includes breath sensing and ventilation delivery apparatus comprising: (a) a tubular member with a proximal end and a distal end, wherein the proximal end is adapted to be positioned outside a patient and the distal end is adapted to be positioned in an airway of the patient, wherein the tubular member includes one or more fenestrations, wherein spontaneous respiration by a patient passes through the one or more fenestrations, (b) one or more intra-airway breath sensors within a lumen of the tubular member, wherein a distal end portion of the tubular member is positioned in the airway such that the one or more intra-airway breath sensors are located within the airway, and wherein the one or more intra-airway breath sensors are exposed to the spontaneous respiration by the patient while within the airway. The one or more fenestrations may be located in a position selected from the group consisting of a superior side of the tubular member, an inferior side of the tubular member, a lateral side of the tubular member, and combinations thereof. The one or more intra-airway breath sensors may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, tubes with sensing lumen, sensing subassemblies, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention includes a breath sensing and ventilation delivery apparatus comprising: (a) a ventilation catheter for ventilation gas delivery including at least one breath sensing lumen including a breath sensing lumen port, (b) an airflow permeable protector at least partially surrounding a portion of the catheter to protect the at least one breath sensing lumen port, (c) a connection to connect the at least one breath sensing lumen to an external sensor, and further wherein the catheter is configured to be placed into an airway of the patient to position the at least one breath sensing lumen port and permeable protector in the airway, and wherein the at least one breath sensing lumen port is protected by the airflow permeable protector but is exposed to spontaneous airflow in the airway. The airflow permeable protector may comprise one or more fenestrations, which are located in a position selected from the group consisting of a superior side of the airflow permeable protector, an inferior side of the airflow permeable protector, a lateral side of the airflow permeable protector, and combinations thereof. The external sensor is selected from the group consisting of thermal sensors, gas composition sen-

sors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention includes a breath sensing and ventilation catheter apparatus comprising: a ventilation catheter for ventilation gas delivery, at least one breath sensing lumen port positioned on an outside surface of the ventilation catheter, an airflow permeable shield at least partially surrounding the at least one breath sensing lumen port, and wherein the airflow permeable shield prevents contact of the at least one breath sensing lumen port with tissue and reduces accumulation of debris on the at least one breath sensing lumen port. The airflow permeable shield may be a collapsible basket. The airflow permeable shield may be a cone tapering from a proximal end to a distal end, and wherein the cone further comprises one or more fenestrations. The airflow permeable shield may be a cuff. The airflow permeable shield may be a stoma sleeve. The airflow permeable shield may be collapsible against an outer surface of the ventilation catheter. The at least one breath sensing lumen port may be connected to a sensor external to a patient, the sensor selected from the group consisting of thermal sensors, pressure sensors, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention includes a method for breath sensing and ventilation comprising: inserting at least one intra-airway breath sensor into a tubular guide positioned with a proximal end adapted to be outside of the patient and a distal end adapted to be inside an airway of a patient, wherein the at least one intra-airway breath sensor is not located within a ventilator gas flow, and wherein the at least one intra-airway breath sensor is shielded from contacting tissue and from accumulating debris by the tubular guide. The tubular guide may be a tracheostomy tube cannula. The cannula may at least partially surround a ventilation catheter for providing the ventilator gas flow, wherein the cannula forms an annular space between the cannula and the ventilation catheter. The at least one intra-airway breath sensor may be within the annular space. The cannula may have one or more fenestrations. The tubular guide may be a protective shield. The protective shield may be selected from the group consisting of a shield tapered on at least one end, a shield collapsible against an outer surface of the ventilation catheter, stoma sleeve, and combinations thereof. The at least one intra-airway breath sensor may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention relates to a method for breath sensing and ventilation comprising: inserting at least one intra-airway breath sensor in a path of a patient's airway airflow, but not within a ventilation gas delivery circuit, monitoring the patient's airway airflow with the at least one intra-airway breath sensor, operating at least one ventilation gas sensor within a ventilation gas delivery circuit, and monitoring the ventilator gas delivery with the at least one ventilation gas sensor simultaneous with monitoring the patient's airway airflow with the at least one intra-airway breath sensor. The at least one intra-airway breath sensor may be coupled to a ventilation catheter. The at least one intra-airway breath sensor can be at least partially surrounded by a protector. The protector may be a tracheostomy tube cannula. The cannula may comprise one or more

fenestrations. The protector may be an airflow permeable shield. The airflow permeable shield may be selected from the group consisting of a basket, a cone, a cuff, a grouping of wires or filaments, a shield tapered on at least one end, a shield collapsible against an outer surface of the ventilation catheter, stoma sleeve, and combinations thereof. The at least one intra-airway breath sensor may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention relates to an apparatus for breath sensing and ventilation comprising: a ventilation catheter for supplying ventilation gas to a patient via a ventilation gas delivery channel in the catheter, a sensing conduit not in communication with the ventilation catheter gas delivery circuit, an opening in the sensing conduit for sensing respiration of the patient through the sensing conduit when the opening is positioned within an airway, and a sensing element communicating with the sensing conduit for sensing respiration of the patient, wherein the sensing element is located external to the patient, and a protector at least partially surrounding the ventilation catheter and sensing conduit opening. The protector may be a tracheostomy tube cannula. The cannula may comprise one or more fenestrations. The sensing element may be selected from the group consisting of: a pressure sensor, a flow sensor, a thermal sensor, or an ultrasonic sensor. The protector may be selected from the group consisting of a basket, a cone, a cuff, a grouping of wires or filaments, a shield tapered on at least one end, a shield collapsible against an outer surface of the ventilation catheter, stoma sleeve, and combinations thereof.

Another aspect of the invention relates to a breath sensing and ventilation delivery apparatus comprising: a ventilation catheter, a tracheostomy tube cannula, wherein the tube cannula at least partially surrounds the ventilation catheter to create an annular space between an inner diameter of the cannula and an outer diameter of the ventilation catheter, and one or more intra-airway breath sensors within the annular space between an inner diameter of the cannula and an outer diameter of the ventilation catheter. The one or more intra-airway breath sensors may be coupled to the ventilation catheter. The one or more intra-airway breath sensors may be coupled to the cannula. The one or more intra-airway breath sensors may be de-coupled from the ventilation catheter and the outer cannula. The at least one intra-airway breath sensor may be selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

Another aspect of the invention relates to a breath sensing and ventilation delivery apparatus comprising: (a) a ventilation catheter including a ventilation gas delivery channel and a breath sensing lumen, wherein the breath sensing lumen includes a sensing port, and wherein the ventilation catheter is configured to be placed into the lumen of a tracheostomy tube such that the ventilation catheter is at least partially surrounded by the tracheostomy tube to prevent the sensing port from contacting the tracheal wall; and (b) a breath sensor external to the patient communicating with the breath sensing lumen. The external breath sensor may be a pressure sensor. The ventilation gas delivery channel may be connected to a flow or pressure sensor external to the patient. The tracheostomy tube may be a cannula of a dual cannula tracheostomy tube. The tracheos-

tomy tube may be a single cannula tube. The ventilation catheter may have a locking connector to connect to the tracheostomy tube. The tracheostomy tube may have a fenestration positioned in the airway. The ventilation catheter may have a centering feature to prevent the sensing port from touching the inner wall of the tracheostomy tube. The sensing port may be positioned at a distance away from the distal end of the ventilation catheter.

Another aspect of the invention is directed to a breath sensing and ventilation delivery apparatus comprising: (a) a ventilation catheter including (i) a ventilation gas delivery channel (ii) a breath sensing lumen including a sensing port, (iii) an airflow permeable shield at least partially surrounding the sensing port; (b) a breath sensor placed external to the patient communicating with the breath sensing lumen, wherein the catheter is configured to be placed into an airway of a patient such that the sensing port and at least a portion of the airflow permeable shield is positioned in the airway of the patient such that the airflow permeable shield prevents the sensing port from contacting the airway wall, and such that the sensing port is exposed to airflow in the airway. The external breath sensor may be a pressure sensor. The ventilation gas delivery channel may be connected to a flow or pressure sensor external to the patient. The sensing port may be positioned at a distance away from the distal end of the ventilation catheter. The ventilation catheter may be configured to be placed in through a stoma guide. The airflow permeable shield may be collapsible.

Another aspect relates to a method for breath sensing and ventilation delivery comprising: inserting a one end of a ventilation catheter into a tracheostomy tube of a patient, wherein the ventilation catheter includes a gas delivery channel and a breath sensing lumen and a breath sensing lumen port, and connecting at a second end of the ventilation catheter the gas delivery channel to a ventilation gas source and the breath sensing lumen to a breath sensor element. The step of connecting may include connecting to the external breath sensor that is a pressure sensor. The step of connecting may include connecting the ventilation gas delivery channel to a flow or pressure sensor external to the patient. The ventilation catheter may have a locking connector to the tracheostomy tube. The method may include positioning a fenestration in the tracheostomy tube in the airway. The method may include the step of centering the ventilation catheter using a centering feature on the ventilation catheter to prevent the sensing port from touching the inner wall of the tracheostomy tube. The method may include the step of positioning the sensing port at a distance away from the distal end of the ventilation catheter.

Another aspect of the invention relates to a method for breath sensing and ventilation delivery comprising: inserting a one end of a ventilation catheter through a stoma and into an airway of a patient, wherein the ventilation catheter includes a gas delivery channel a breath sensing lumen and a breath sensing lumen port, and a protective shield at least partially surrounding the catheter section inserted into the airway to prevent the sensing lumen port from contacting the airway wall and connecting, at a second end of the ventilation catheter, the gas delivery channel to a ventilation gas source and the breath sensing lumen to a breath sensor element. The step of connecting may include connecting to the external breath sensor is a pressure sensor. The step of connecting may include connecting the ventilation gas delivery channel to a flow or pressure sensor external to the patient. The method may include step of positioning the sensing port at a distance away from the distal end of the ventilation catheter. The method may include the step of

positioning the ventilation catheter through a stoma guide. The step of inserting may include inserting the airflow permeable shield that is collapsible.

Additional features, advantages, and embodiments of the invention are set forth or apparent from consideration of the following detailed description, drawings and claims. Moreover, it is to be understood that both the foregoing summary of the invention and the following detailed description are exemplary and intended to provide further explanation without limiting the scope of the invention as claimed.

#### BRIEF DESCRIPTION OF THE INVENTION

The accompanying drawings, which are included to provide a further understanding of the invention and are incorporated in and constitute a part of this specification, illustrate preferred embodiments of the invention and together with the detailed description serve to explain the principles of the invention. In the drawings:

FIG. 1a shows prior art for breath effort detection by using breath sensors within a ventilator gas delivery circuit.

FIG. 1b shows optional prior art using an ultrasonic flow meter. FIG. 1c shows optional prior art using a rotameter flow meter.

FIG. 1d is a graph illustrating a signal from the system of FIG. 1a where the sensed pressure does not necessarily correspond to respiration.

FIG. 2a shows prior art using chest impedance for breath sensing and ventilator control.

FIG. 2b is a graph illustrating a drift in the impedance signal of FIG. 2a caused by an environmental or stability problem.

FIG. 3a shows prior art in which intra-airway breath sensors are used for ventilator control and monitoring respiration activity.

FIG. 3b is a graph illustrating a disruption of the sensor signal of FIG. 3a caused by an environmental problem.

FIG. 4 shows a partial cross-sectional view of the overall system of the invention including a ventilation catheter and a fenestrated outer cannula and a breath sensor in the annular space, and a ventilator.

FIG. 5 shows a partial cross-sectional view of the overall system of the invention including a ventilation catheter, a fenestrated outer cannula and a breath sensing lumen and sensing port, and a sensor placed outside the patient in a ventilator

FIG. 6 shows a ventilation catheter and non-fenestrated outer cannula with a breath sensor in the annular space.

FIG. 7 shows a ventilation catheter and an outer cannula with a breath sensor pan of the outer cannula.

FIG. 8 shows a ventilation catheter and an outer cannula with a breath sensing lumen and port as pan of the outer cannula.

FIG. 9 shows a ventilation catheter and an outer cannula and a separate sensor assembly placed in the space between the ventilation catheter and outer cannula.

FIG. 10 shows a ventilation catheter and an outer cannula and a separate sensing lumen assembly placed in the space between the ventilation catheter and outer cannula.

FIG. 11 shows a ventilation catheter and an outer cannula with an channel open to ambient between the catheter and cannula and a sensor in the channel

FIG. 12A shows a dual lumen trach tube with fenestrated outer cannula.

FIG. 12B shows the outer cannula of FIG. 12A with the inner cannula removed.

FIG. 12C is a cross section of a ventilation catheter placed inside the fenestrated outer cannula of FIG. 12B where a sensing element is positioned in an annular space.

FIG. 13 is a detailed view of an alternative, adjustable ventilation catheter connector.

FIG. 14 is a partial cross section of a ventilation catheter placed inside the fenestrated outer cannula of FIG. 12B where a sensing lumen port is positioned in an annular space.

FIG. 15 shows a ventilation catheter with intra-airway breath sensing protected inside a fenestrated single cannula tracheostomy tube.

FIG. 16 is a cross section of a ventilation catheter with intra-airway breath sensor protected inside a fenestrated outer cannula with inferior and superior fenestration positions.

FIG. 17 shows a ventilation catheter with an outer cannula with fenestrations on a lateral wall of the outer cannula.

FIG. 18A is a cross section of a ventilation catheter with intra-airway breath sensors protected inside a fenestrated outer cannula, with positioning and anchoring features for the ventilation catheter.

FIG. 18B is an end view of the ventilation catheter shown in FIG. 18A.

FIG. 19 shows a ventilation catheter with a fenestrated outer cannula having a depression to create an annular gap between the ventilation catheter and the fenestrated outer cannula.

FIG. 20A is a cross section of a ventilation catheter inside a fenestrated outer cannula with a depression adjoining the fenestration in a wall of the outer cannula to create an annular gap between the ventilation catheter and the fenestrated outer cannula.

FIG. 20B is a view of the device in FIG. 20A however with the depression on the inferior side.

FIG. 21A is a cross section of a ventilation catheter inside a fenestrated outer cannula with a protrusion in an inner wall of the outer cannula to create an annular gap between the ventilation catheter and the fenestrated outer cannula.

FIG. 21B is a view of the device in FIG. 21A however with the depression on the inferior side.

FIG. 22 shows a ventilation catheter with intra-airway breath sensors protected inside a minimally penetrating fenestrated outer cannula.

FIG. 23 shows a ventilation catheter inserted through a stoma sleeve where a sensor is protected by a stoma sleeve.

FIG. 24 shows a ventilation catheter with intra-airway breath sensors protected by an air permeable shield that is collapsible.

FIG. 25A shows a ventilation catheter with intra-airway breath sensors protected by a permeable wire basket shield that may be collapsible against a catheter shaft and may be expanded when in use.

FIG. 25B is a cross sectional view of the ventilation catheter shown in FIG. 10a.

FIG. 26 shows a ventilation catheter with intra-airway breath sensors protected by a permeable conical shield that may be foldable, collapsible against a catheter shaft, and may be expanded when in use.

FIG. 27 shows a system layout of the system shown in FIG. 4, with an additional ventilator gas delivery sensor.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

FIG. 1a shows a prior art ventilator breath detection triggering system where a pressure sensor is located within

a ventilation gas delivery circuit 21. A ventilator V may deliver ventilation gas to a patient P through a ventilation gas delivery circuit 21 and a ventilation tube 25. A ventilation circuit pressure tap 22 may be located within the ventilation gas delivery circuit 21. The ventilation circuit pressure tap 22 may sense pressure in the ventilation gas delivery circuit 21. Thus, when the patient P inspires, a negative pressure created in the lung L may be transmitted to the trachea T, and the negative pressure may be detected in the ventilation circuit pressure tap 22. The ventilation circuit pressure tap 22 may be in communication with a ventilator breath delivery control unit 20.

Alternatively, as shown in FIG. 1b, a flow sensor may be used in place of the pressure sensor. The flow sensor may be an ultrasonic flow sensor 30 or another type of flow sensor. Alternatively, as shown in FIG. 1c, a rotameter flow sensor 32 may be located within the ventilation gas delivery circuit 21 to detect inspiration by the patient P, as shown in FIGS. 1a and 1b.

A signal representing the reading from the sensors, which may include, for example but without limitation, a ventilation circuit pressure tap 22, an ultrasonic flow sensor 30, or a rotameter flow sensor 32, may be communicated to the ventilator breath delivery control unit 20 in the ventilator V. The sensors within the ventilation gas delivery circuit 21 may measure the start of a breath. After the ventilator breath delivery unit 20 received the signal, the ventilator V may be triggered to deliver a mechanical breath to the patient P through the ventilation gas delivery circuit 21. After the ventilator V is triggered, the sensors may measure activity of the ventilator V. The sensors may not accurately measure patient breathing.

FIG. 1d shows the measurement of the patient's tracheal pressure P(t) detected by the sensors in comparison with a tracing R of a patient's actual respiration. A patient's inspiration 54 may be initially detected by the sensors as a decrease in pressure from a patient inspiration pressure 50. After triggering of the ventilator V, however, the sensors may only measure ventilator breath delivery pressure 52 and not patient exhalation 56.

FIG. 2a shows a prior art ventilator triggering system where the breath sensor is a chest impedance sensor. The breath sensor is not located within a ventilation gas delivery system 21. A chest impedance sensor may have the drawback that signals representing patient breathing may be affected by motion of the patient P not related to breathing. A chest impedance band 62 may be connected to a ventilator V and corresponding ventilator breath delivery control unit 20 by chest impedance wires 60.

FIG. 2b shows a respiration trace R of the patient P, which may correspond to the patient's actual breathing for a certain time, as compared to a flow of gas in a patient's trachea T as shown in tracheal airflow tracing Q. A patient inspiration tracheal flow curve 64 and a patient exhalation tracheal flow curve 66 may be detected by the chest impedance band 62 as seen in a chest impedance inspiration trace 74 and a chest impedance exhalation trace 76, respectively. However, due to motion and patient position and other factors, the chest impedance signal may have chest impedance signal drift 78 or may have chest impedance signal noise from patient motion 80.

FIG. 3a shows a prior art breath sensing system. An intra-airway breath sensor 190 may be located in an airflow path of a patient P in the patient's trachea T.

The intra-airway breath sensor 190 may be used to detect spontaneous breathing by the patient P. To effectively measure spontaneous breathing, the intra-airway breath sensor

**190** is preferably not located within a ventilation gas delivery circuit **21**. For purposes of this disclosure, a sensor not located within the ventilation gas delivery circuit **21** may be considered to be “in parallel” to the ventilation gas delivery circuit **21**. Sensors that are located within the ventilation gas delivery circuit **21** may be considered “in series” in relation to the ventilation gas delivery circuit **21** for purposes of this disclosure. Sensors that are within the ventilation gas delivery circuit **21** may not adequately measure spontaneous breathing after the triggering of a ventilator **V** because the sensor may then measure primarily the gas delivered by the ventilator **V** and because the spontaneous breathing may move substantially less air than the ventilator **V**. A benefit of not having sensors in communication with the ventilator gas delivery circuit is that the sensor may measure the entire spontaneous breathing signal even after triggering the ventilator **V** because the sensor would not be within the stream of gas supplied by the ventilator **V**. Sensors outside of the ventilator gas delivery circuit are not directly measuring gas delivered from the ventilator **V**.

The intra-airway breath sensor **190** of FIG. **3a** may not be in communication with the ventilation gas delivery circuit **21**. The intra-airway breath sensor **190** may be mounted on an outside surface of ventilation tube **25**. The intra-airway breath sensor **190** may measure spontaneous breathing and create a signal representing the spontaneous breathing. The signal may be communicated to a ventilator breath delivery control unit **20** within the ventilator **V** by intra-airway breath sensing wires **92**, wireless technology, RFID, or other communications technology.

The positioning of the intra-airway breath sensor **190** within the trachea **T** not in communication with a ventilator gas delivery circuit **21** may be an improvement over conventional systems because the intra-airway breath sensor **190** may be less prone to drift and disturbance from environmental influences and patient movement. The sensor may also be less invasive and obtrusive to the patient **P**, and may be more convenient for a supervising clinician. The intra-airway breath sensor **190** may be mounted on a portion **24** of a ventilation tube **25** inserted into the airway of a patient **P**. Additionally, when the ventilator **V** is triggered to deliver gas to the patient **P** through the ventilation gas delivery circuit **21**, a measurement by the intra-airway breath sensor **190** may not be dominated by action of the ventilator **V** and may continue to measure spontaneous respiration of the patient **P**.

FIG. **3b** shows a tracheal airflow trace **Q** compared with a breath sensor signal tracing **S**. Patient inspiration tracheal flow **65** and patient exhalation tracheal flow **67** compare well with an inspiration trace **75** and an expiration trace **77**, respectively. However, the intra-airway breath sensor **190** may be susceptible to contacting tissue, such as a wall of the trachea **T**, or accumulation of debris on a surface of the intra-airway breath sensor **190**. Contacting tissue and/or accumulation of debris may disrupt measurement from the intra-airway breath sensor **190** as shown by an intra-tracheal breath sensor signal attenuation from tissue contact or debris **94**. Protection of the efficacy and accuracy of the intra-airway breath sensor **190** may be important to ensure proper function of a ventilator gas delivery circuit **21**.

FIG. **4** shows a system diagram of an embodiment of the present invention. A ventilation catheter **27** may be placed inside an outer tube **28**, such as a tracheostomy tube, and a breath sensor or sensors **90** may be placed in an annular space **46** between the ventilation catheter **27** and the outer tube **28** for protection against accumulation of debris and tracheal wall contact. Typically, the system may be config-

ured to facilitate at least part of the patient’s spontaneous breathing airflow to travel in the annular space. The sensor signal may be transmitted to the ventilator **V** to control the ventilator, which may be attached to the ventilation catheter **27** with a gas delivery circuit **21**. The outer tube **28** may include fenestrations **100** so gas may flow easily in and out of the annular space **46**.

An intra-airway breath sensor **90** may be located in the trachea **T**, nose, mouth, throat, bronchial or any other location within the path of inhaled and exhaled air. Furthermore, it may be appreciated that embodiments of the present invention may apply to other physiological applications where a catheter is placed in any luminal structure for sensing and therapy. It should be further appreciated that with the appropriate modifications, embodiments of the present invention may be reusable or disposable and may be adapted for adult, pediatric or neonatal use.

The breath sensors in accordance with the principles of the present invention may be thermal sensors, pressure sensors, sensing lumens, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, or any other sensor capable of sensing respiration. The breath sensors may be a single sensing element/transducer. Alternatively, the breath sensors may contain multiple sensing elements/transducers for redundancy of signal measurements. Additionally, the breath sensors may contain multiple elements arranged in a sensing array such that at least one of the multiple elements may be used as a reference signal. In the present disclosure, a sensor may be referred to as either singular or plural, however, all of the above configurations may apply.

Preferably, the breath sensors may be mounted on a portion of a ventilation tube inserted into the airway of a patient **P** as shown in FIG. **4**. Alternatively, as shown in the system diagram in FIG. **5**, an external breath sensor **96** may be positioned outside the body. The external breath sensor **96** may measure airflow or breathing pressure occurring in the patient airway via a sensing conduit or lumen **42**. The sensing conduit or lumen **42** may have an opening or sensing port **44** within a patient airway in the annular space **46** between the ventilation tube **27** and the outer tube **28**. The conduit or lumen **42** may run from the opening **44** to an external breath sensor, for example a sensor **96**, located in the ventilator **V**. The sensor **96** may communicate with a control unit **20** to control a gas delivery device **142** to control the delivery of gas to the patient.

Fenestrations **100** in the outer tube **28** may be provided as shown in FIGS. **4** and **5** to facilitate spontaneously breathing airflow travels in the annular space. Alternatively, as shown in FIG. **6**, the outer tube **28** can be without fenestrations, and the sensor **90** may register the tracheal breathing pressures that are occurring without requiring an open flow path through the outer tube **28**.

The breath sensor or external breath sensor and corresponding sensing conduit may be coupled to a ventilation tube as shown in FIGS. **4-6**. Alternatively, the breath sensor or external breath sensor and corresponding sensing conduit may be integrated with other components of the present invention as described herein. For example, a breath sensor **90** may be part of the inner wall of the outer cannula **28**, as shown in FIG. **7**. The ventilation catheter **27**, when inserted into the outer cannula **28** may form an electrical connection with the sensor **90** so the sensor signal may be transmitted to the ventilator with wiring **92**.

Or, as shown in FIG. **8**, a sensing lumen **42** and sensing lumen port **44** can be coupled to the outer cannula **28**. When

the ventilation catheter **27** is connected to the outer cannula **28**, the outer cannula sensing lumen **42** connects via a pneumatic female and male connection **104**, **103**, respectively, to an external lumen **109** extending away from the patient to an external sensor (not shown), for example, a sensor **96** located in the ventilator **V** as previously shown in FIG. **5**. In FIGS. **7** and **8**, the sensor **90** or sensing lumen **42** and port **44** may be located on the superior side of the outer tube **28**, in which case fenestrations **102**, if present, may be located on lateral walls of the outer tube (described later). Alternatively, the sensor **90** or sensing lumen **42** and port **44** shown in FIGS. **7** and **8** can be located on the inferior side of the outer tube **28**, in which case fenestrations may be located on the superior side of the outer tube **28**. Further, the sensor **90** or sensing lumen **42** and port **44** can be located on a lateral wall of the outer tube **28**.

Alternatively, the breath sensor or external breath sensor may be decoupled from the various components of the present invention. For example, as shown in FIG. **9**, a separate assembly **97** including the sensor **90** can be inserted into the annular space **46** between the ventilation catheter **27** and outer cannula **28**. The separate assembly **97** and sensor **90** can be inserted or retracted using a handle **105**.

Or, alternatively, as shown in FIG. **10**, a separate assembly **98** comprising a sensing lumen **42** can be inserted into the annular space **46** between the ventilation catheter **27** and the outer cannula **28**, where the sensing lumen **42** connects via an external sensing lumen **109** to sensor positioned outside the body, for example a sensor **96** at the ventilator **V** as shown in FIG. **5**. The separate assembly **98** and sensing lumen **42** can be inserted and retracted using a handle **106**.

As described herein, various embodiment of protective configurations, apparatuses and methods for breath sensors may be provided to reduce tissue contact with the breath sensors and accumulation of debris on the breath sensors. The breath sensor may be at least partially surrounded by airflow-permeable coverings, protectors or shields that allow spontaneous respiration to pass through the airflow-permeable coverings and reach the breath sensors. Thus, in accordance with the principles of the invention, various embodiments and configurations described and shown are contemplated and the specific embodiments and configurations are not limiting.

FIG. **11** shows an alternative where the annular space **46** between the ventilation tube **27** and outer cannula **28** may communicate with ambient air depicted by arrows **107**. Some of the spontaneous breathing airflow in the trachea **T**, indicated by arrow **150**, may travel to and from ambient through the annular space **46**. The sensor **90** may be placed in the annular space **46** and may register the breathing signal.

FIGS. **12A-12C** show the sequence of operation and configuration when using a dual cannula tracheostomy tube assembly **23** containing a tracheostomy tube inner cannula **110** and a tracheostomy tube outer cannula **28**. For purposes of this invention, the terms ventilation catheter, ventilation tube, and related expressions are used interchangeably. Similarly, the terms tracheostomy tube, outer cannula, outer tube and related expressions are used interchangeably. Various combinations of elements in alternative embodiments may be combined together within the scope of the present invention.

FIG. **12A** shows the tracheostomy tube outer cannula **28** surrounding the tracheostomy tube inner cannula **110**. The tracheostomy tube outer cannula **28** may be disposed relative to the tracheostomy tube inner cannula **110** such that an annular space **46** may exist between an inner surface of the

tracheostomy tube outer cannula **28** and an outer surface of the tracheostomy tube inner cannula **110**. The tracheostomy tube outer cannula **28** may have one or more fenestrations **100** to allow airflow into the annular space **46**. As indicated by arrows **150**, spontaneous respiration may pass through the one or more fenestrations **100** into the annular space **46** and out an end **151** of the tracheostomy tube outer cannula **28**. Ventilation gas (arrow **152**) from a ventilator may pass through the tracheostomy tube inner cannula **110**, out an end **153** of the tracheostomy tube inner cannula **110** and into a patient airway. Ventilation gas (arrow **152**) and/or spontaneous respiration **150** may also pass through tracheostomy tube inner cannula **110** and the annular space **46**, respectively, in the reverse direction. Fenestrations **100** may permit flow of gas past the dual cannula tracheostomy tube **23** to and from the upper airway. The fenestrations **100** may also permit speech by allowing exhaled air flow past vocal cords.

The dual cannula tracheostomy tube **23** may include a tracheostomy tube neck flange **112** and/or a tracheostomy tube ventilation circuit connector **111**. The tracheostomy tube ventilation circuit connector **111** may allow the dual cannula tracheostomy tube **23** to be connected to various types of ventilators. The dual cannula tracheostomy tube **23** configuration may be used when it is preferred to have the option of removing the ventilator and ventilation catheter and allowing the patient to breathe through the outer cannula.

FIG. **12B** shows an embodiment of the present invention with the tracheostomy tube inner cannula **110** removed from the tracheostomy tube outer cannula **28** which is left in position in the patient airway.

FIG. **12C** shows another variation of an inner cannula ventilation catheter **26** substituted for the tracheostomy tube inner cannula **110**. The inner cannula ventilation catheter **26** may be configured to be placed inside the tracheostomy tube outer cannula **28** for precise positioning of intra-airway breath sensors **90** in the annular space **46** between the inner cannula ventilation catheter **26** and the tracheostomy tube outer cannula **28**. For example, the precise positioning may include obtaining the correct depth of insertion of the breath sensors relative to the outer cannula length, or the correct circumferential orientation of the sensors in relationship to the outer cannula inner wall, as will be explained later. Thus, the intra-airway breath sensors **90** may be protected within the annular space **46** and may not be susceptible to contacting tissue or accumulating debris. However, the intra-airway breath sensors **90** may be in communication with the spontaneous respiration **150** (shown in FIG. **12A**) in the inspiratory and expiratory direction and may detect and measure the breathing pattern of the patient **P**.

A ventilation catheter seal and connector **116** may connect the inner cannula ventilation catheter **26** to the tracheostomy tube outer cannula **28** for sealing, security and positioning and a flange **115** facilitates insertion and removal of the ventilation catheter **26** from the outer cannula **28**. The seal and connector may be, for example, a friction fit seal/connector, a twist and lock seal/connector, or a snap-fit seal/connector, a compressible gasket such as silicone, a line-to-line fit between the mating parts, a mating tapered interface, and/or a slight interference fit with one soft material and an opposing hard material. The location of the intra-airway breath sensors **90** may be anywhere inside the annular space **46**, however, preferably the intra-airway breath sensors **90** may be positioned at a location between the fenestrations **100** and the end **151** of the tracheostomy tube outer cannula **28**. If the sensors are positioned too close to the distal end of the outer cannula, the sensor may be

prone to Venturi artifacts created by gas flow exiting the ventilation catheter from the ventilator. Hence location of the sensors at a distance from the outer cannula opening is preferred.

Because the amount of airflow traveling through the annular space may be only a portion of the total tracheal airflow, the breath signal measured by the breath sensor may be a dampened signal. However, this is deemed acceptable, since the measurement accurately reflects flow or pressure, albeit not necessarily reflective of the true amplitude.

In FIG. 12C, the inner cannula ventilation catheter 26 may include rigidity to prevent unwanted flexure of the inner cannula ventilation catheter 26 that may inadvertently cause the intra-airway breath sensors 90 to contact the outer cannula inner wall.

FIG. 13 shows an alternative connection mechanism where the inner cannula ventilation catheter 26 may include a connector 116 and flange 115 assembly which includes an adjustable sliding seal 117 between the catheter shaft 118 and the connector/flange 116/115 assembly. The ventilation catheter connector/flange assembly 116/115 may be used to position a distal tip D of the inner cannula ventilation catheter 26 and the intra-airway breath sensors 90 in a desired position. The ventilation catheter connector/flange assembly 116/115 may be configured such that it locks or self-locks onto the catheter shaft 118 when not moving the inner cannula ventilation catheter 26. For example, the ventilation catheter connector/flange assembly 116/115 may use a detent system, a collet system, a compression clip a spring-loaded push button, or a locking pin. Alternatively, the position of the intra-airway breath sensors 90 may be adjustable. For example the sensor can be advanced or retracted by moving a rod or wire as shown previously in FIG. 10.

FIG. 14 shows a sensing lumen 42 extending from outside a patient P at a proximal end and into an airway, such as a trachea T. The sensing lumen 42 may have a distal end within the airway with a sensing lumen port/opening 44 positioned in the annular space 46. A sensor may be located outside of the patient P as shown previously in FIG. 5, but may be in communication with the sensing lumen 42, sensing lumen port/opening 44, and/or the airway. This may be advantageous to reduce cost of the ventilation catheter or to reduce the required size of the ventilation catheter.

In addition to the embodiments of FIGS. 12-14, other ventilation catheter and tracheostomy tube combinations and interconnections can be used.

FIG. 15 describes a ventilation catheter 31 adapted to be inserted into a signal cannula tracheostomy tube 29. The tracheostomy tube 29 may include one or more fenestrations 100 to allow spontaneous respiration to pass between the ventilation catheter 31 and the tracheostomy tube 28. One or more intra-airway breath sensors 90 may be located within the tracheostomy tube 29, or on the ventilation tube 31. The one or more intra-airway breath sensors 90 may be protected within an annular space 46 as previously described. The ventilation catheter 31 and tracheostomy tube 29 may have one or more mating features as those described previously to permit connecting the ventilation catheter 31 and the tracheostomy tube 29. The one or more mating features may position the one or more intra-airway breath sensors 90 in a desired position.

The embodiment of FIG. 15 may also include a tracheostomy tube neck flange 112, a ventilation catheter seal 116 and a tracheostomy tube ventilation circuit connector 111. This embodiment allows the ventilation catheter 31 to be removed and a conventional ventilator and breathing circuit

to be connected to the 15 mm connector 111 of the single cannula tracheostomy tube 29, for example, in the event conventional ventilation is required.

Embodiments of the present invention may include various patterns and configurations of fenestrations to allow gas to pass through a sensor protection device onto a sensor. Fenestrations may be located at any location and some preferred locations and configurations are described below. Gas permeable shields for sensors may come in various shapes and numbers, but the gas permeable shields preferably prevent tissue contact with the sensors and/or accumulation of debris on the sensors. For purposes of this invention, the superior direction refers to a position facing an exit of a patient airway from a body of the patient, for example, facing the upper airway. Additionally, the inferior direction refers to a position facing away from the exit of a patient airway from a body of the patient, for example, facing the lower airway. A lateral direction refers to any direction that is not superior or inferior. As discussed above, the fenestrations and/or gas permeable shields may be disposed in any position. The shape of fenestrations may be circular, oval, or any other reasonable shape. The location and shape of the fenestrations can be any combination of the above.

FIG. 16 shows an alternate embodiment of a ventilation catheter 33 and outer cannula tracheostomy tube 34. The outer cannula tracheostomy tube 34 may include one or more fenestrations 100 on a superior side of the tracheostomy tube 120 and/or one or more fenestrations 101 on an inferior side of the tracheostomy tube 122. One or more fenestrations 100, 101 on various surfaces of the outer cannula tracheostomy tube 34 may decrease resistance to inspired and expired gas flow through the outer cannula tracheostomy tube 34. Furthermore, one or more fenestrations 100, 101 on various surfaces of the outer cannula tracheostomy tube 34 may provide redundancy for gas flow through the outer tracheostomy tube 34 in the event that one or more fenestrations 100, 101 are miss-aligned, blocked and/or obscured. FIG. 16 also describes a connector/seal 119 that connects to the outer cannula 120.

FIG. 17 shows fenestrations 102 on a lateral sides 121 of the outer cannula tracheostomy tube 34.

Proper positioning of the one or more intra-airway sensors 90 may be important for proper functioning of the breath sensing and ventilator control system. Furthermore, it may be important for the one or more intra-airway sensors 90 to remain in an original or desired position over time. Configurations and methods for positioning and stabilizing the one or more intra-airway sensors 90 may be provided.

FIG. 18A shows an embodiment in which a ventilation catheter 35 includes one or more ventilation catheter stabilization/positioning anchors 130. The one or more ventilation catheter stabilization/positioning anchors 130 may locate and hold one or more intra-airway breath sensors 90 at a desired position within an outer cannula 36. The one or more ventilation catheter stabilization/positioning anchors 130 may help center the ventilation catheter 35 in the outer cannula 36 so the one or more intra-airway breath sensors 90 do not contact an inner wall 37 of the outer cannula 36. The one or more ventilation catheter stabilization/positioning anchors 130 may also prevent the ventilation catheter 35 from whipping when pressurized gas is delivered through the ventilation catheter 35. The one or more ventilation catheter stabilization/positioning anchors 130 may be positioned at one or multiple locations. For example, the one or more ventilation catheter stabilization/positioning anchors 130 may be positioned a location near the one or more intra-airway breath sensors 90 to assure that the one or more

intra-airway breath sensors 90 are properly positioned in the annular space 46. Alternatively, the one or more ventilation catheter stabilization/positioning anchors 130 may be positioned a location near a distal tip D of the ventilation catheter 35 to reduce movement of the distal tip during gas delivery. A ventilation catheter outer seal 114 is shown.

FIG. 18B is an end view of FIG. 18A. Other possible configurations of the one or more ventilation catheter stabilization/positioning anchors 130 are possible to locate the one or more intra-airway breath sensors in a desired position within the annular space 46. The anchors are for example compressible filaments or wires, such as an elastomeric filament or a shape memory alloy wire. The filaments or wires can be for example a loop shape, or spokes, or a braid, or a woven basket. The density of the anchor structure is very low offering little to no airflow resistance, unless the anchor is proximal to the fenestration, in which case the anchor can be resistive to airflow since airflow is not needed in that zone for the breath sensors to detect the breathing signal.

FIG. 19 shows a cannula deflector 40 for ensuring the one or more intra-airway sensors 90 are exposed to air flowing within the annular space 46. The cannula deflector 40 of FIG. 19 is shown in a superior side of the outer cannula 38 for the purpose of spacing a ventilation catheter 39 and sensor 90 away from the inner wall of the outer cannula 38. The ventilation catheter 39 may be formed and shaped into an arc radius that is larger than the arc radius of the outer cannula 38. The cannula deflector 40 may deflect the ventilation catheter 39 into a tighter radius. Therefore, exact matching of the radius of the ventilation catheter 39 to the radius of the outer cannula 38 during manufacturing may be unnecessary. The cannula deflector 40 may be shaped atraumatically to avoid any harsh contact should contact occur between the deflector and the tissue. One or more fenestrations 100 may be positioned at various locations on the outer cannula 38.

FIG. 20A shows a cannula deflector 40 in the outer cannula 38 adjoining a fenestration 100. One or more intra-airway breath sensors 90 and/or a sensing lumen port may be positioned just distal to the cannula deflector 40 and the fenestration 100. This may be advantageous when the superior or inferior portion of the cannula which extends into the tracheal lumen from the anterior wall of the trachea, is relatively short, and there is not enough distance between the anterior wall and posterior wall of the trachea for both a deflector and a fenestration if separated from one another.

FIG. 21A shows a cannula deflector 40 that protrudes only from an inner wall of the outer cannula 38. An outer diameter of the outer cannula 38 may not be affected by the cannula deflector 40. This may be advantageous for insertion and removal of the outer cannula 38 from an airway. The cannula deflector 40 may be near or adjoining one or more fenestrations 100 or may be separated from the one or more fenestrations 100 by a predetermined distance. Typically, the deflector and fenestration may have to be located close together due to the limited space requirements imposed by the tracheal diameter. The embodiments described in FIGS. 19, 20A and 21A may be especially applicable in cases in which a single cannula tracheostomy tube is being used, since a tracheostomy tube inner cannula is not placed into the tracheostomy tube. A tracheostomy tube inner cannula, when used with a dual cannula tracheostomy tube, is typically as large as possible to optimize gas delivery. The deflector may require a smaller diameter tracheostomy tube inner cannula contrary to common practice.

In addition to the location of the cannula deflector 40 and the one or more intra-airway sensors 90 shown in FIGS. 19, 20A and 21A as a superior location, the cannula deflector 40 may be located at other positions on the outer cannula 38. Other positions for the cannula deflector 40 may be an inferior side 122 of the outer cannula 38 as shown in FIGS. 20B and 21B and/or a lateral side 121 of the outer cannula 38 (not shown). Preferably, the one or more intra-airway sensors 90 may be located on corresponding sides of the ventilation catheter 39. For example, if the cannula deflector 40 is on the inferior side 122 of the outer cannula 38, the one or more intra-airway breath sensors 90 may be located on an inferior side of the ventilation catheter 39. Various positions and combination may be used. The sensor 90 may be positioned at a location away from the midline of the catheter 38 so that when inserted, the sensor does not get damaged by rubbing on the deflector.

FIG. 22 shows an embodiment of the present invention with a short tracheostomy tube 49. An inner ventilation catheter 47 may extend distally beyond a distal end 51 the short tracheostomy tube 49. The embodiment of FIG. 8a may be beneficial because the short tracheostomy tube 49 may extend into an airway only as far as necessary to prevent one or more intra-airway breath sensors 90 from contacting the tissue and/or and or reduce accumulation of debris on the one or more intra-airway breath sensors. The patient's airway, therefore, may be potentially more open to spontaneous breathing. In addition, this configuration may facilitate measuring a breathing signal that is closer to the true signal, since there is less obstruction of spontaneous gas flow by the device, for example less Venturi effects, turbulence and dampening of the tracheal flow and pressure. An inner ventilation catheter seal 113 is shown.

FIG. 23 shows an embodiment of the present invention where the ventilation catheter 47 may be adapted to be placed in a stoma sleeve 48. The stoma sleeve 48 may only marginally extend into the airway. The marginal extension into the airway may provide enough shielding for the one or more intra-airway breath sensors 90 to prevent contact with tissue and/or reduce accumulation of debris. The embodiment of FIG. 22 may be beneficial because the stoma sleeve 48 may be of a relatively small diameter and, therefore, less obtrusive to a patient P. Use of the stoma sleeve 48 may be useful when the patient P is not at risk of requiring full support ventilation because the stoma sleeve 48 typically does not include a standard 15 mm connector required for connection to a conventional ventilator. The stoma sleeve is preferably different than a similar conventional device known as the Montgomery T-Tube, because the stoma sleeve must be configured to create space between the sleeve and the ventilation catheter to define an annular space for the breath sensor. Also, the stoma sleeve is preferably different than a similar conventional device known as a stoma stent such as the Hood Stoma Stent, because the stoma stent does not elongate into the tracheal airway. The stoma sleeve and main lumen there through must elongate a distance into the tracheal lumen in order to define the annular space or protective zone for the breath sensors. Some patients may require the tracheostomy tube compatible version, rather than the stoma sleeve version. For example, if a patient requires other respiratory treatments and accessories on occasion or is at risk of requiring conventional mechanical ventilation, the 15 mm respiratory connector that is part of the tracheostomy tube will facilitate attachment to other respiratory treatments.

Other embodiments of the present invention may have alternative or supplemental protection for the one or more

intra-airway breath sensors. For the purposes of this disclosure, the terms protectors and shielding are used interchangeably. Various forms of protection may be used interchangeably or together. In the following exemplary embodiments, the outer cannula or stoma sleeve may be replaced or used with alternative protection devices. Preferably, protectors and/or shields may be airflow permeable.

FIG. 24 shows a fenestrated shield 136 on a ventilation catheter 27. The ventilation catheter 27 may be inserted into an airway, such as a trachea T through a stoma tract 134 or other similar opening. The ventilation catheter may preferably be inserted directly through the stoma tract 134, but may be inserted through a tracheostomy tube or other similar apparatus if needed. A ventilation catheter neck flange 132 may provide positioning and securing of the ventilation catheter 27. One or more intra-airway breath sensors 90 may be mounted on the ventilation catheter 27. The one or more intra-airway breath sensors may be protected by the fenestrated shield 136.

The fenestrated shield 136 may be a basket-type device and is permeable to airflow. The basket may be a woven or braided filament or wire structure with one or both ends of the structure attached to the ventilation catheter shaft. The structure has a normally expanded dimension, but can be easily compressed into a compressed dimension for insertion of the ventilation catheter 27 through the stoma 134.

FIG. 25A shows a basket type fenestrated shield 136 that may be collapsed by a pull wire mechanism or stretch mechanism (not shown) from a collapsed state C to an expanded state E and back. The pull wire mechanism is attached to the proximal end of the basket wire structure. Pulling on the wire in the proximal direction elongates the structure proximally, such that the structure diameter reduces or collapses. Therefore, the proximal end of the basket wire structure is slideably attached to the ventilation catheter shaft. The basket type fenestrated shield 136 may also be collapsed by temperature sensitive shape memory alloys that respond to temperature change. The materials may be in a first collapsed state at room temperature, but upon insertion into an airway, the materials may enter a second expanded state based upon the change in temperature from room temperature to the temperature within the airway. The basket type fenestrated shield 136 may also be tapered to facilitate insertion and removal of the ventilation catheter 27 through the stoma. The wires of the basket may be very resilient and pliable to facilitate insertion or removal without requiring uncomfortable amounts of forces. FIG. 25B is an end view of the device of FIG. 25A when in the expanded state. When the basket type fenestrated shield 136 is in an expanded state E, the basket type fenestrated shield 136 has a diameter larger than the diameter of the ventilation catheter 27. However, when the basket type fenestrated shield 136 is in a collapsed state C the basket type fenestrated shield 136 may have a diameter only marginally larger than the diameter of the ventilation catheter 27. In the collapsed state C, the basket type fenestrated shield 136 may collapsed against an outer surface of the ventilation catheter 27.

The one or more intra-airway breath sensors 90 may be disposed on the ventilation catheter 27. Preferably, the basket type fenestrated shield 136 may at least partially surround the one or more intra-airway breath sensors 90 when the basket type fenestrated shield 136 is in an expanded state E. The one or more intra-airway breath sensors 90 may prevent tissue contact and/or may reduce accumulation of debris on the one or more intra-airway breath sensors 90.

Alternatively, the protection device may be a cuff or any other similar structure that is airflow permeable.

FIG. 26 shows an airflow permeable shield 138 that may be conical and tapered to favor removal out of a stoma tract 134. The airflow permeable shield 138 may be coupled to a ventilation catheter 27 at a tapered end of the airflow permeable shield 138. The airflow permeable shield 138 may be collapsible. To collapse the airflow permeable shield 138 for insertion, the airflow permeable shield 138 may be composed of shape-memory materials. The airflow permeable shield 138 may be provided in a collapsed state C and then may then expand to an expanded state E after insertion into an airway by responding to body temperature. Alternatively, the airflow permeable shield 138 may be folded by hand or machine into the collapsed state C and then inserted into the airway and then self-expand or manually or mechanically expand to the expanded state E. The airflow permeable shield 138 may assume predetermined conical protective shield folds 140 when collapsed. The airflow permeable shield 138 may manually, mechanically or automatically collapse prior to or during removal from the airway and stoma.

The airflow permeable shield 138 may include one or more fenestrations 100. The one or more fenestrations 100 may be lengthened to facilitate collapsing and expanding of the airflow permeable shield 138. Alternatively, the airflow permeable shield may be permeable to airflow without the one or more fenestrations 100.

The intra-airway breath sensors of various embodiments of the present invention may be combined with breath sensors within the ventilation gas delivery circuit so patient breathing and ventilator activity may be monitored separately, but simultaneously. For example as shown in FIG. 27, the intra-airway breath sensor 90 as described in the above embodiments can be used to measure the patient's breathing, and the effect the ventilator V has on the patient's respiratory system, while a sensor 108 measuring the output of the ventilator V in the gas delivery circuit 21 is measuring the ventilator output.

Although the foregoing description is directed to the preferred embodiments of the invention, it is noted that other variations and modifications will be apparent to those skilled in the art, and may be made without departing from the spirit or scope of the invention. Moreover, features described in connection with one embodiment of the invention may be used in conjunction with other embodiments, even if not explicitly stated above.

What is claimed is:

1. A breath sensing and ventilation delivery apparatus comprising:

a ventilation catheter,

a tracheostomy tube cannula with one or more fenestrations in a wall thereof, wherein the cannula at least partially surrounds the ventilation catheter to create an annular space between an inner diameter of the cannula and an outer diameter of the ventilation catheter, and one or more adjustable depth intra-airway breath sensors structurally independent of the ventilation catheter and the tracheostomy tube cannula, and being positionable within the annular space between the inner diameter of the cannula and the outer diameter of the ventilation catheter and within a path of spontaneous patient respiration airflow passing through the one or more fenestrations.

2. The apparatus of claim 1, wherein the ventilation catheter extends beyond a distal portion of the cannula and into an airway.

3. The apparatus of claim 1, further comprising an anchor for preventing movement of a distal tip of the ventilation catheter.

4. The apparatus of claim 1, wherein the one or more fenestrations are located in a position selected from the group consisting of a superior side of the cannula, an inferior side of the cannula, a lateral side of the cannula, and combinations thereof.

5. The apparatus of claim 1, wherein the one or more intra-airway breath sensors are selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, tubes with sensing lumen, sensing subassemblies, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

6. The apparatus of claim 1, wherein the one or more intra-airway breath sensors are coupled to the ventilation catheter.

7. The apparatus of claim 1, wherein the ventilation catheter is removable from the cannula.

8. The apparatus of claim 1, further comprising a seal between the cannula and the ventilation catheter at a location proximal to the one or more intra-airway breath sensors.

9. A breath sensing and ventilation delivery apparatus comprising:

(a) a tubular member with a proximal end and a distal end, wherein the proximal end is adapted to be positioned outside a patient and the distal end is adapted to be positioned in an airway of the patient, wherein the tubular member includes one or more fenestrations in a wall thereof, wherein spontaneous respiration by the patient passes through the one or more fenestrations,

(b) one or more adjustable depth intra-airway breath sensors structurally independent of the tubular member and within a lumen of the tubular member,

wherein a distal end portion of the tubular member is positioned in the airway such that the one or more adjustable depth intra-airway breath sensors are located within the airway, and

wherein the one or more adjustable depth intra-airway breath sensors are positioned within a path of the spontaneous respiration by the patient passing through the one or more fenestrations while within the airway.

10. The apparatus of claim 9, wherein the one or more fenestrations are located in a position selected from the group consisting of a superior side of the tubular member, an inferior side of the tubular member, a lateral side of the tubular member, and combinations thereof.

11. The apparatus of claim 9, wherein the one or more intra-airway breath sensors are selected from the group

consisting of thermal sensors, pressure sensors, pressure sensing lumen, tubes with sensing lumen, sensing subassemblies, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

12. A method for breath sensing and ventilation comprising:

inserting at least one adjustable depth intra-airway breath sensor into a tubular guide positioned with a proximal end adapted to be outside of a patient and a distal end adapted to be inside an airway of the patient, the at least one intra-airway breath sensor being structurally independent of the tubular guide and being positionable within the tubular guide within a path of airflow from spontaneous patient respiration; and

monitoring the patient's airway airflow with the at least one intra-airway breath sensor during ventilation, wherein, during said monitoring, the at least one adjustable depth intra-airway breath sensor is not located within a ventilator gas flow, and

wherein, during said monitoring, the at least one adjustable depth intra-airway breath sensor is shielded from contacting tissue and from accumulating debris by the tubular guide.

13. The method of claim 12, wherein the tubular guide is a tracheostomy tube cannula.

14. The method of claim 13, wherein the cannula at least partially surrounds a ventilation catheter for providing the ventilator gas flow, wherein the cannula forms an annular space between the cannula and the ventilation catheter.

15. The method of claim 14, wherein the at least one intra-airway breath sensor is within the annular space.

16. The method of claim 13, wherein the cannula has one or more fenestrations.

17. The method of claim 12, wherein the tubular guide is a protective shield.

18. The method of claim 17, wherein the protective shield is selected from the group consisting of a shield tapered on at least one end, a shield collapsible against an outer surface of a ventilation catheter, stoma sleeve, and combinations thereof.

19. The method of claim 12, wherein the at least one intra-airway breath sensor is selected from the group consisting of thermal sensors, pressure sensors, pressure sensing lumen, gas composition sensors, flow sensors, ultrasonic sensors, resistivity sensors, piezoelectric sensors, light emittance/reflectance sensors, and combinations thereof.

\* \* \* \* \*

专利名称(译)	用于感测呼吸和提供通气治疗的方法和装置		
公开(公告)号	<a href="#">US10058668</a>	公开(公告)日	2018-08-28
申请号	US14/221210	申请日	2014-03-20
申请(专利权)人(译)	BREATHE TECHNOLOGIES , INC.		
当前申请(专利权)人(译)	BREATHE TECHNOLOGIES , INC.		
[标]发明人	WONDKA ANTHONY KAPUST GREGORY BRYAN ROBERT KHENANSHO MICHAEL		
发明人	WONDKA, ANTHONY KAPUST, GREGORY BRYAN, ROBERT KHENANSHO, MICHAEL		
IPC分类号	A61M16/04 A61B5/085 A61B5/08 A61B5/00 A61B5/087 A61M16/00 A61B5/097 A61M16/10		
CPC分类号	A61M16/0427 A61B5/082 A61B5/085 A61B5/0873 A61B5/0878 A61B5/097 A61B5/6853 A61B5/6858 A61M16/0003 A61M16/042 A61M16/0434 A61M16/0465 A61M16/0475 A61M2230/43 A61M2205/3375 A61M16/0486 A61M2016/003 A61M2016/0021 A61M2016/0027 A61M2016/0036 A61M2016/102 A61M2205/332 A61M2205/3306 A61M2230/65		
代理机构(译)	STETINA BRUNDA GARRED & BRUCKER		
助理审查员(译)	BOECKER , JOSEPH D		
优先权	60/924514 2007-05-18 US		
其他公开文献	US20140288456A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

提供了用于气道内呼吸传感器的方法和系统，其中气道内呼吸传感器不位于通气气体输送回路内，而是暴露于来自患者的自发呼吸气流。此外，本发明的方法和系统可用于保护气道内呼吸传感器免于接触组织或积聚可能损害气道内呼吸传感器能力的碎片。

