




US 20170053086A1

(19) **United States**(12) **Patent Application Publication**
MARTIN et al.(10) **Pub. No.: US 2017/0053086 A1**(43) **Pub. Date: Feb. 23, 2017**(54) **SYSTEMS AND METHODS FOR EMS
DEVICE COMMUNICATIONS INTERFACE****Publication Classification**(71) Applicant: **ZOLL Medical Corporation**,
Chelmsford, MA (US)(72) Inventors: **Michael Scott MARTIN**, Lakewood,
CO (US); **Chad ASHMORE**,
Broomfield, CO (US); **Eric A. DEINES**,
Broomfield, CO (US); **Gary A.**
FREEMAN, Waltham, MA (US);
Joseph L. HELMICK, Westminster,
CO (US); **Thomas E. KAIB**, North
Huntingdon, PA (US); **Richard A.**
RATTANNI, New Stanton, PA (US); **C.**
Shane REID, Denver, CO (US);
Jeremy Ryan SOLLER, Broomfield,
CO (US); **Shane S. VOLPE**, Saltsburg,
PA (US); **Gary RUGGIERO**,
Lexington, MA (US); **Frederick J.**
GEHEB, Danvers, MA (US)(51) **Int. Cl.****G06F 19/00** (2006.01)**A61B 5/0402** (2006.01)**A61B 5/024** (2006.01)**G06F 17/30** (2006.01)**A61B 5/00** (2006.01)(52) **U.S. Cl.**CPC **G06F 19/3418** (2013.01); **G06F 19/3406**
(2013.01); **G06F 19/322** (2013.01); **G06F**
17/30569 (2013.01); **G06F 17/30867**
(2013.01); **A61B 5/747** (2013.01); **A61B**
5/0006 (2013.01); **A61B 5/0022** (2013.01);
A61B 5/024 (2013.01); **A61B 5/0402**
(2013.01); **A61B 5/6898** (2013.01)(21) Appl. No.: **15/294,633**(22) Filed: **Oct. 14, 2016****Related U.S. Application Data**(63) Continuation-in-part of application No. 12/840,129,
filed on Jul. 20, 2010, Continuation-in-part of appli-
cation No. 12/840,117, filed on Jul. 20, 2010.(60) Provisional application No. 61/322,675, filed on Apr.
9, 2010, provisional application No. 61/227,187, filed
on Jul. 21, 2009, provisional application No. 61/322,
678, filed on Apr. 9, 2010, provisional application No.
61/227,187, filed on Jul. 21, 2009.

(57)

ABSTRACT

A system for supplementing communications capabilities of a patient monitoring device, the system including a card fitting within a device slot and configured to receive patient monitoring information from the device via the interface slot; a memory device hosted by the card and configured to store patient monitoring information; a wireless transceiver hosted by the card; an asset management database hosted by the card; and a processor communicably coupled to the wireless transceiver and the asset management database, the processor configured to format the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered, the processor further configured to store the one or more frames to the asset management database and to transmit the stream of one or more frames with the wireless transceiver.

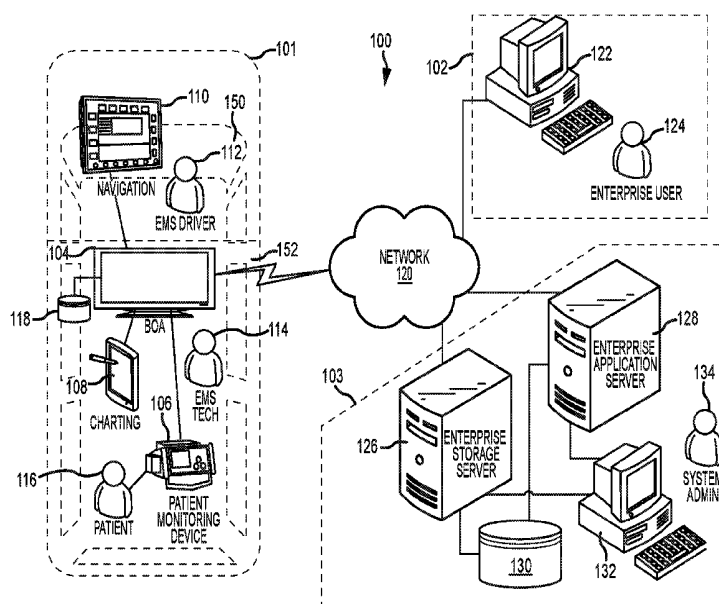

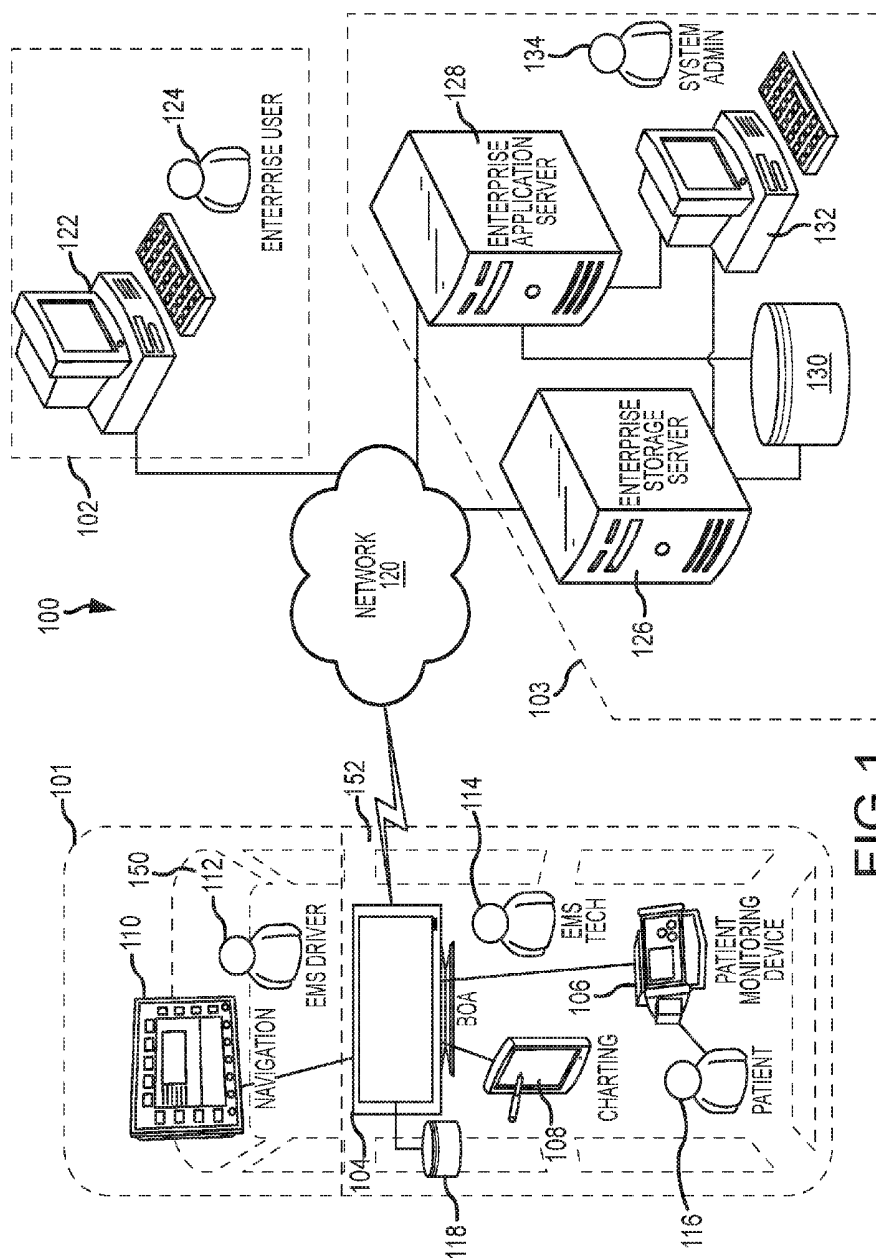


FIG.1

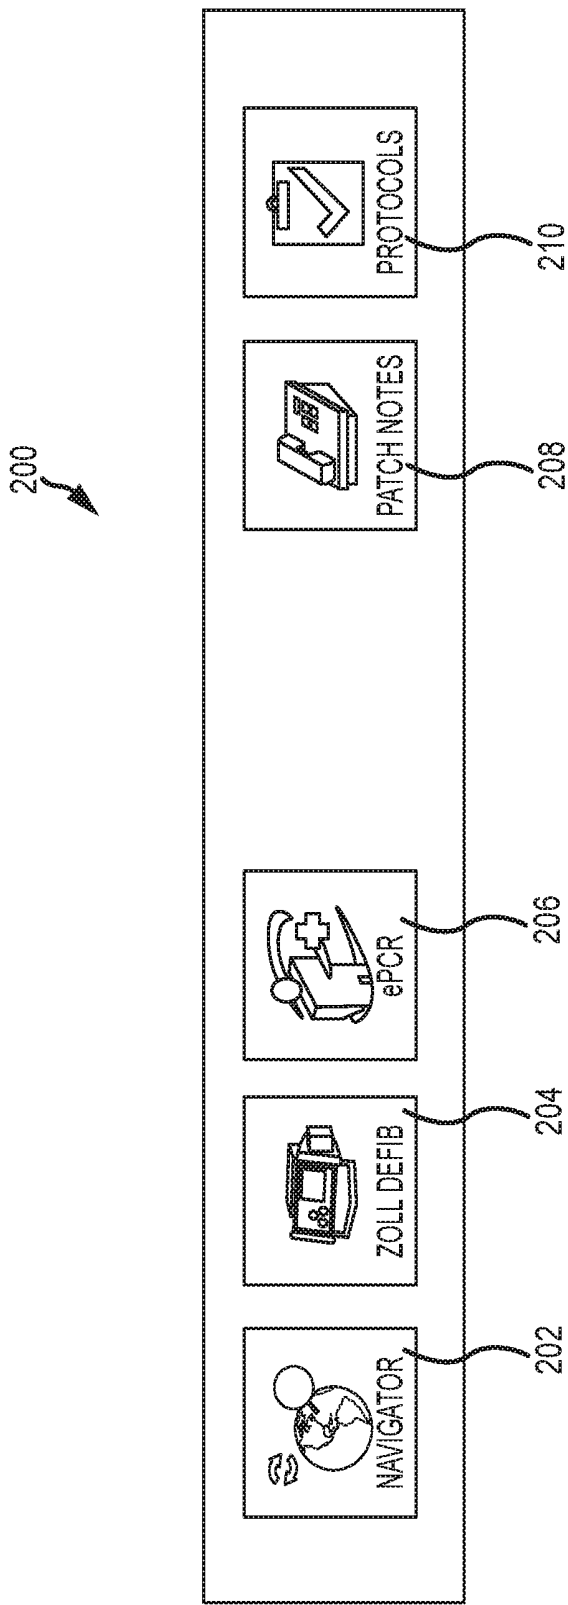
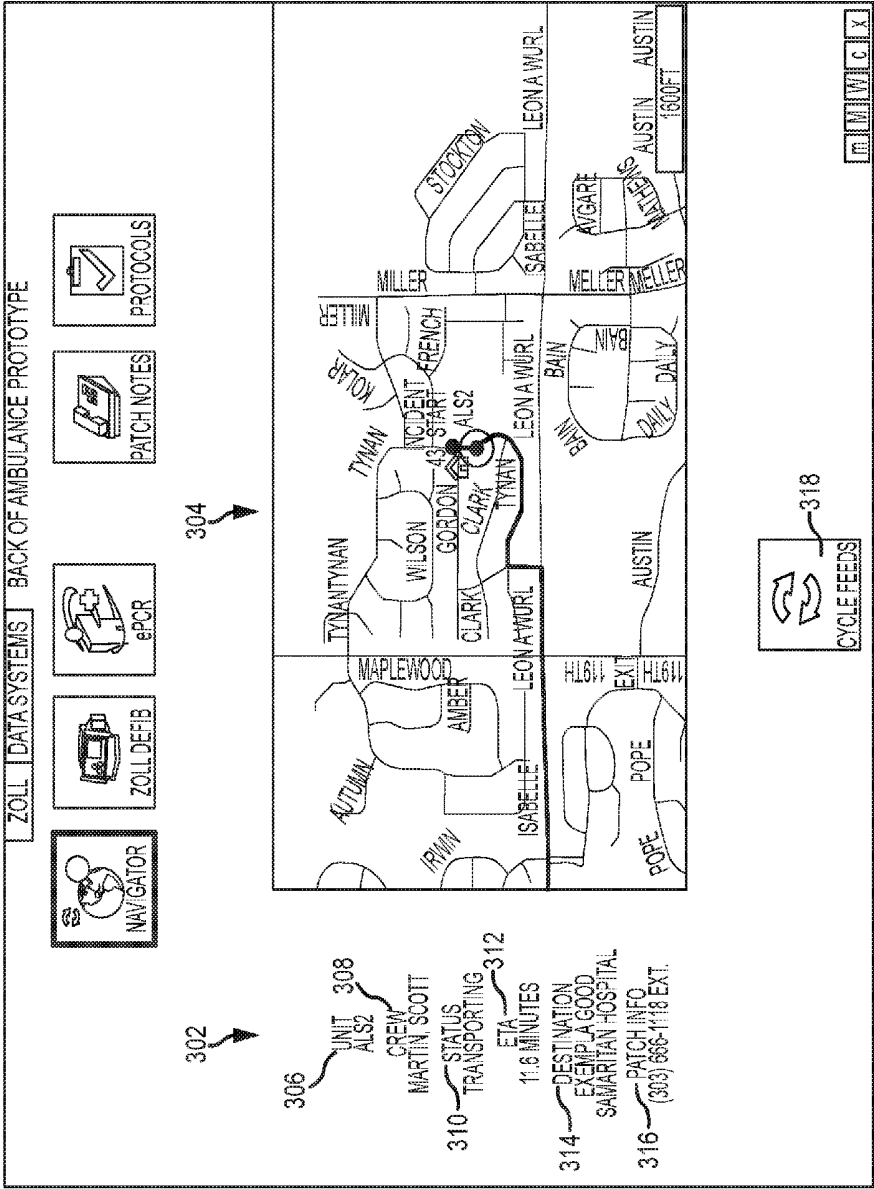


FIG. 2



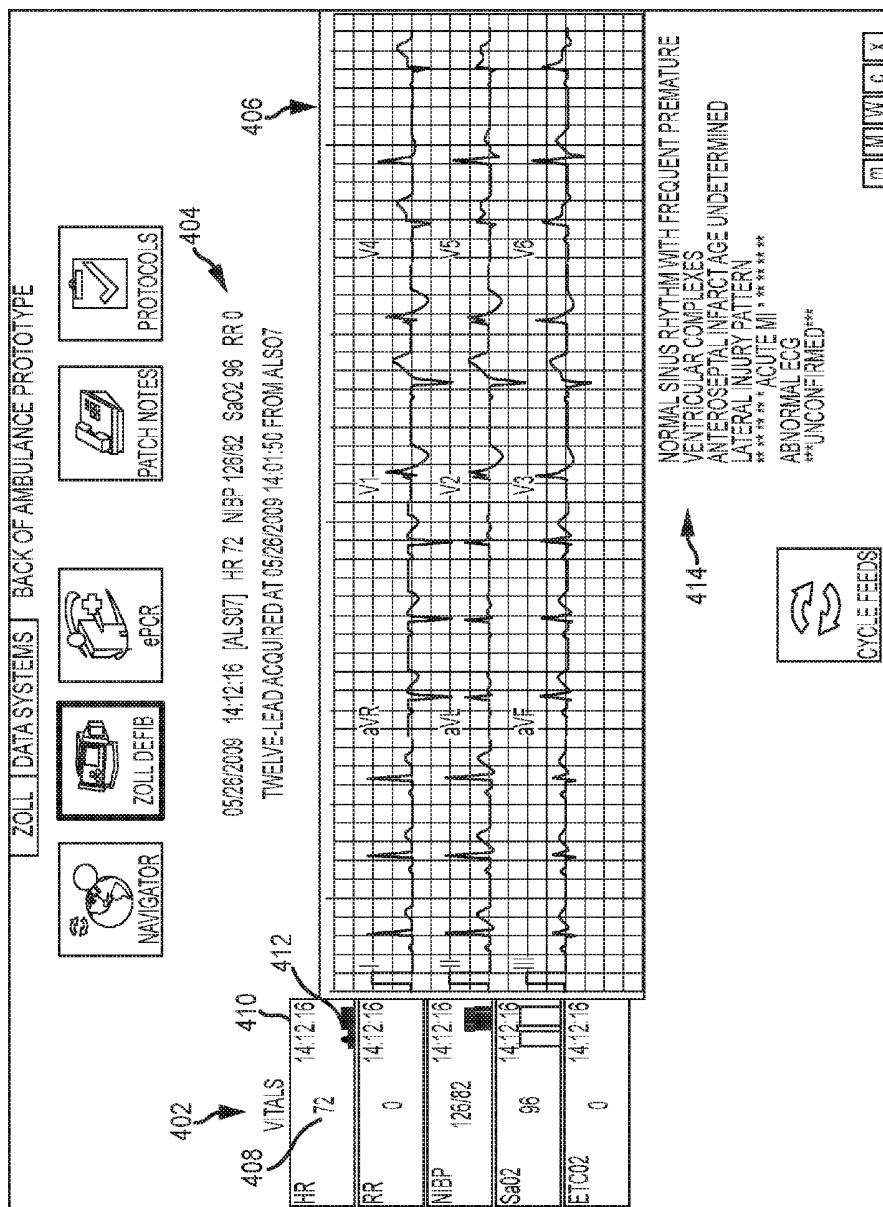


FIG. 4

ZOLL DATA SYSTEMS

BACK OF AMBULANCE PROTOTYPE

504

NAVIGATOR

502

ZOLL DEFIB

ePCR

PATCH NOTES

PROTOCOLS

NAME

ALAN JOHNSON

AGE

88 YEARS

GENDER

MALE

INTERVENTIONS

TIME	DESCRIPTION	BY
14:04	MORPHINE	MARTIN, SCOTT
14:01	IVIO	MARTIN, SCOTT
13:41	BABY ASPIRIN	RED, SHANE
13:41	NITROGLYCERINE	RED, SHANE
13:41	OXYGEN	RED, SHANE

VITALS

TIME	HR	BP	RR	SpO2	ETCO2	GLUCOSE	GCS	BY
14:02	68		20	98%			E4 V5 M6 = 15	
13:41	70	130/70	16	98%				
13:41	76	120/66	22	98%		110		

CYCLE FEEDS

M

M

W

C

X

FIG.5

NAVIGATOR

602

604

HOSPITAL

EXEMPLA GOOD SAMARITAN HOSPITAL

(000) 000-0000 EXT.

ZOLL DEFIB

ZOLL NOTES

PROTOCOLS

DATA SYSTEMS

BACK OF AMBULANCE PROTOTYPE

AGE

58 YEARS

HISTORY PRESENT ILLNESS

ONSET 20 MINUTES AGO

PROVOCATION EXERCISE

QUALITY CRUSHING

RADIATION LEFT ARM

SEVERITY 8/10

TIME

INTERVENTIONS

MORPHINE

IVIO

NITROGLYCERINE

BABY ASPIRIN

OXYGEN

UNIT

ALS2

GENDER

MALE

PAST MEDICAL HISTORY

DIABETES

AMI

PNEUMONIA

VASCULAR DISEASE

CHIEF COMPLAINT

CHEST PAIN

ASSESSMENTS

PRIMARY ACUTE MI

SECONDARY RESPIRATORY DISTRESS

ETA

3.5 MINUTES

ePCR VITALS

14:20 HR: 72 RR: 18 BP: 106/72 SpO2: 99%

14:10 HR: 80 RR: 18 BP: 110/76 SpO2: 98%

14:01 HR: 98 RR: 22 BP: 130/88 SpO2: 98%

DEFIB VITALS

16:02 HR: 72 RR: 0 BP: 115/78 SpO2: 98%

CYCLE FEEDS

m

M

W

C

X

FIG.6

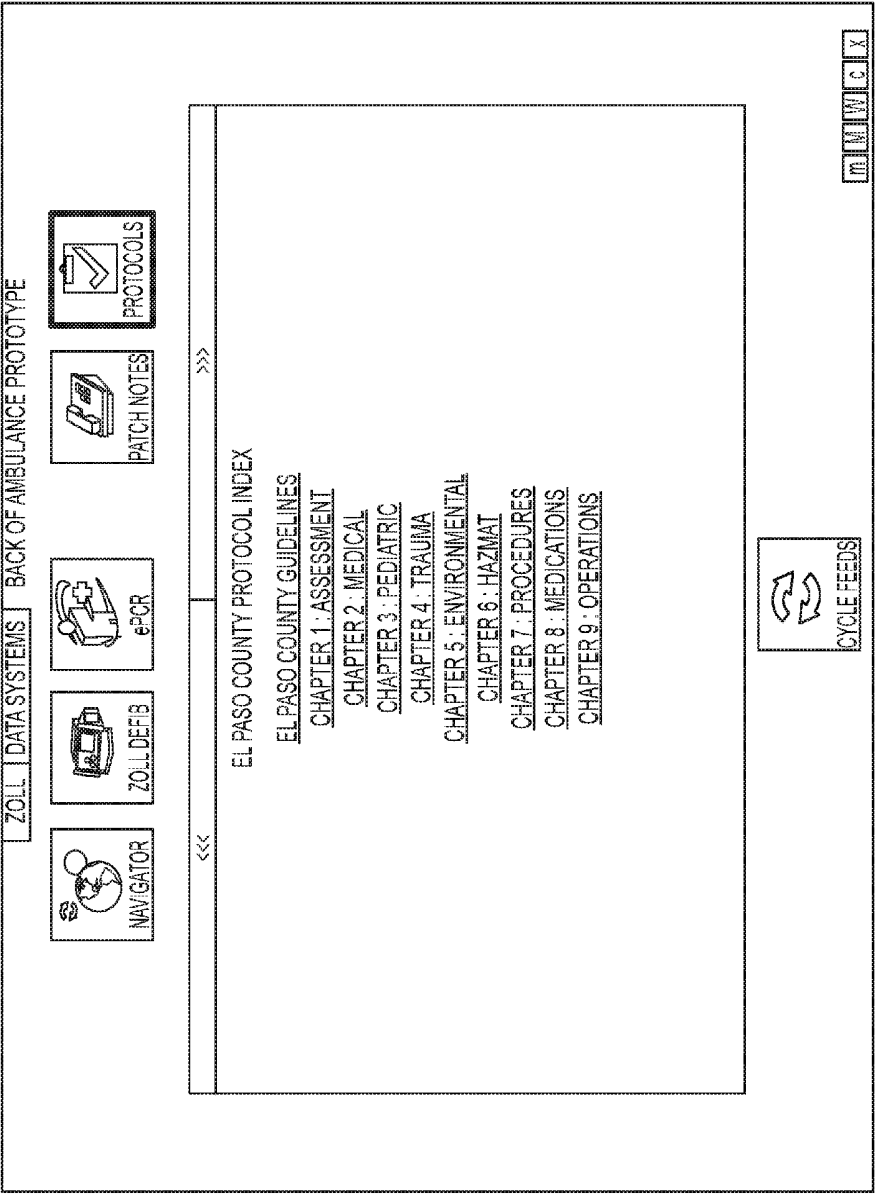


FIG.7


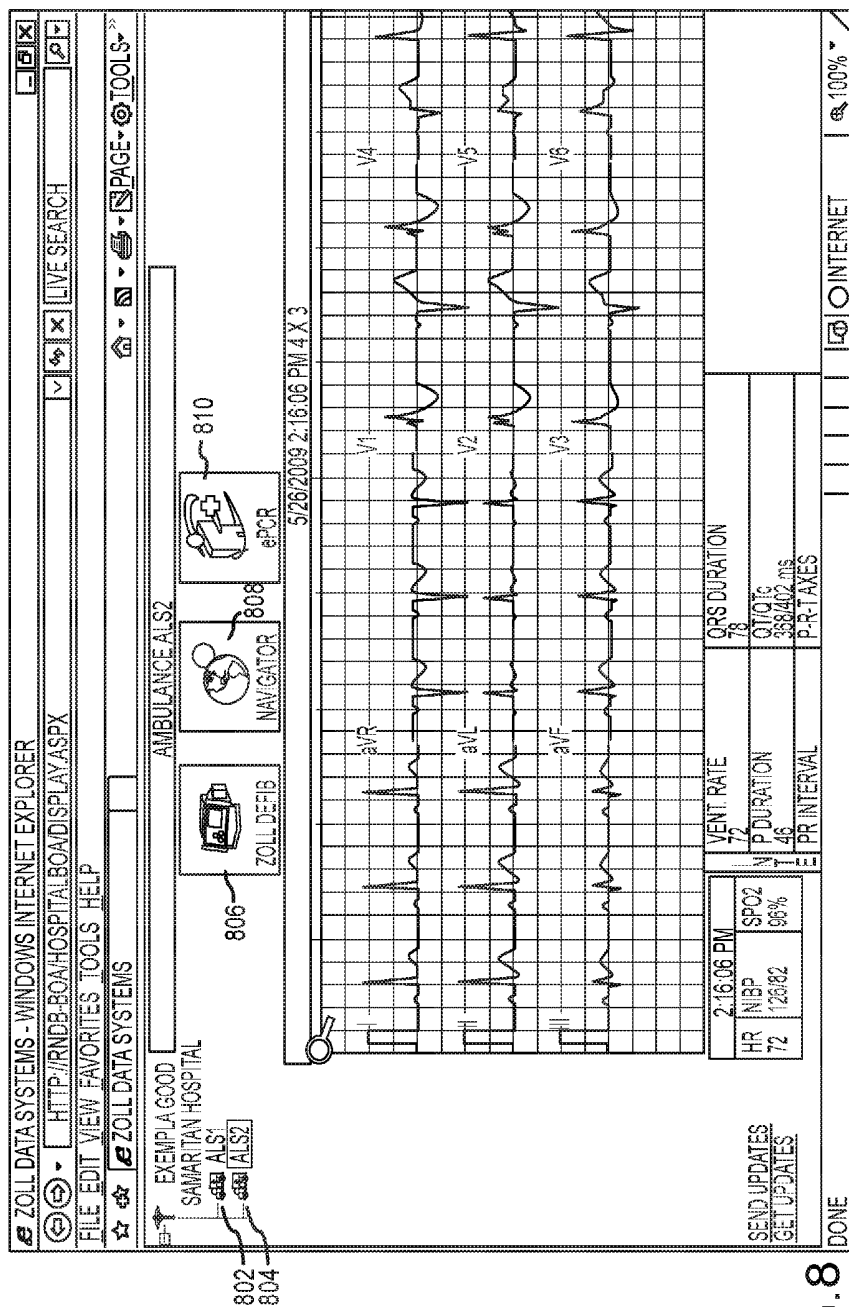


FIG. 8

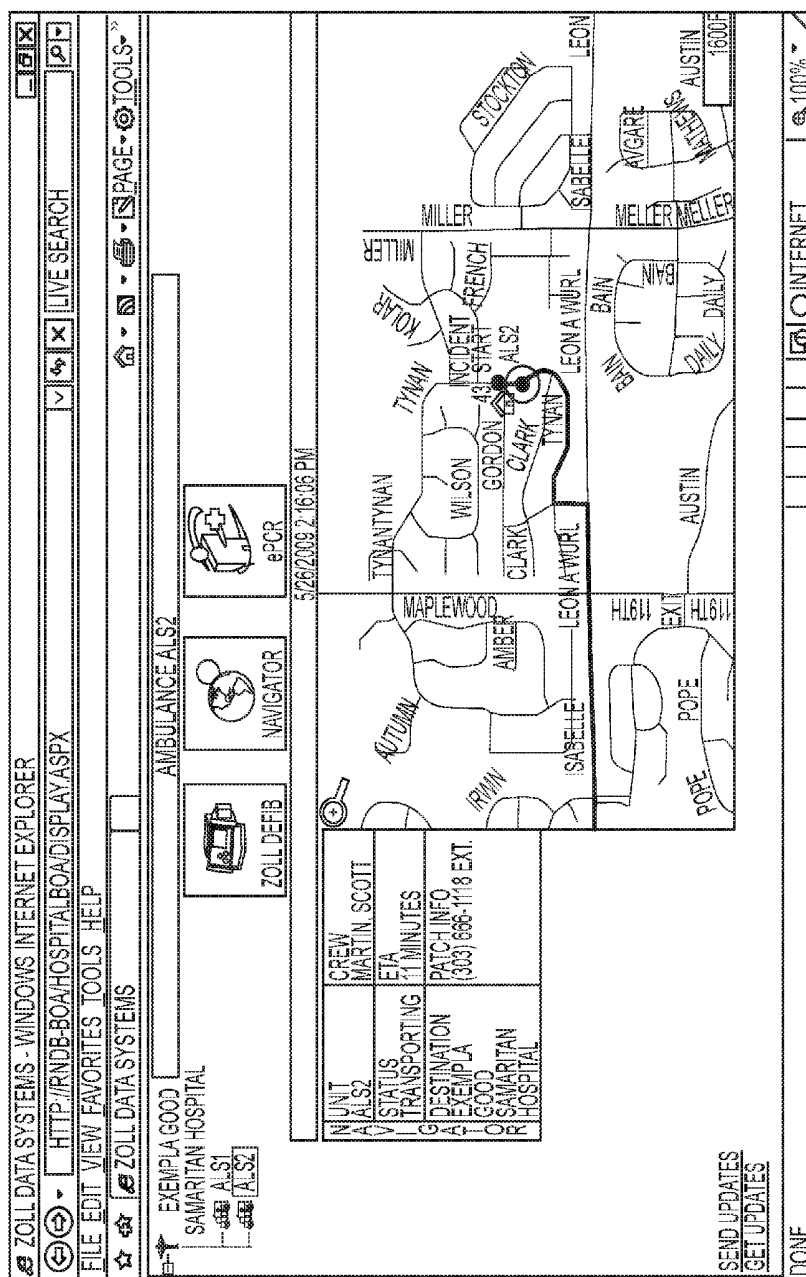

ZOLL DATA SYSTEMS - WINDOWS INTERNET EXPLORER							
HTTP://RND8-BOA.HOSPITALBOARD.DISPLAY.ASPX							
FILE EDIT VIEW FAVORITES TOOLS HELP		ZOLL DATA SYSTEMS					
EXAMPLE GOOD SAMARITAN HOSPITAL		AMBULANCE ALS2					
ZOLL DEFIB		NAVIGATOR		ePCR			
NAME: ALAN JOHNSON AGE: 88 YEARS GENDER: MALE 5/26/2009 2:16:06 PM							
TIME DESCRIPTION		V TIME HR BP RR SPO2 ETCO2 GLUCOSE CCS BY					
05/26/2009 14:02	MORPHINE	05/26/2009 14:04	66	20	96%	E4 V5 M6 = 15	MARTIN, SCOTT
05/25/2009 14:01	IV / IO	05/12/2009 13:41	70	130/70	16 98%		
05/12/2009 13:41	BABY ASPIRIN	05/12/2009 13:41	76	120/66	22 96%	110	
05/12/2009 13:41	NITROGLYCERINE						
05/12/2009 13:41	OXYGEN						
BY MARTIN SCOTT MARTIN SCOTT REID SHANE REID SHANE REID SHANE							

INTERNET WOUNDING

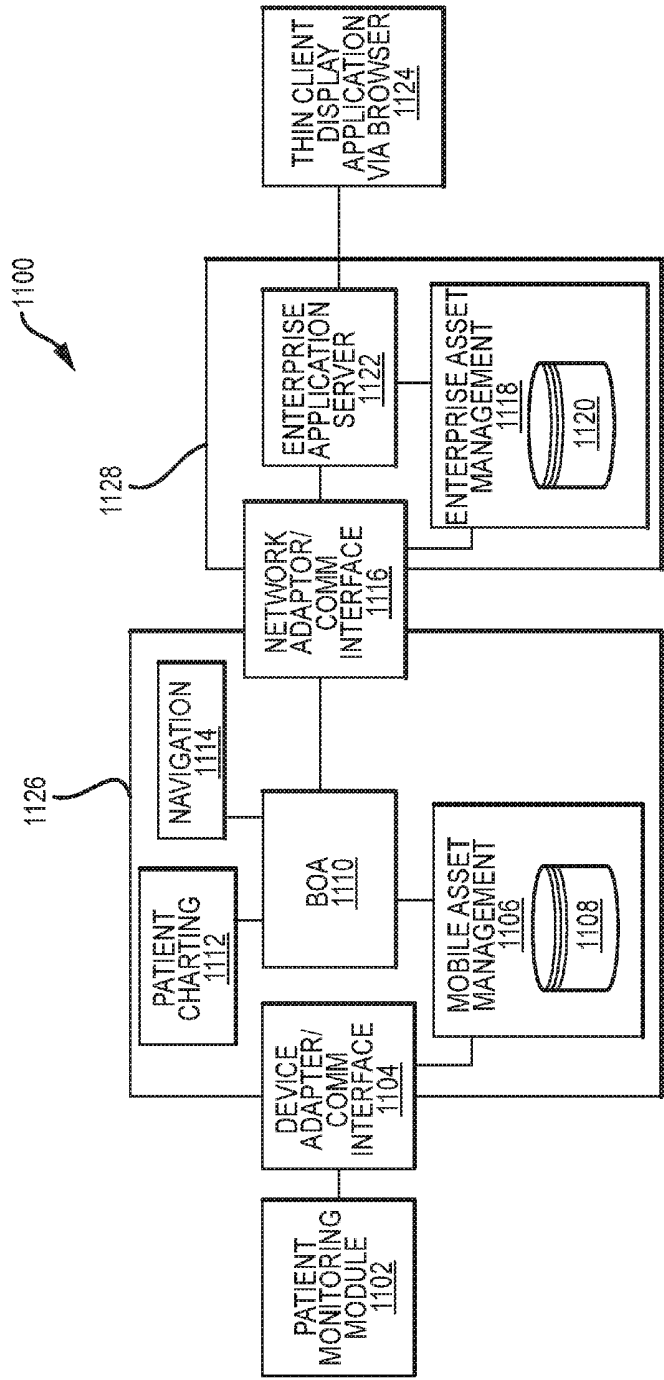


FIG. 11

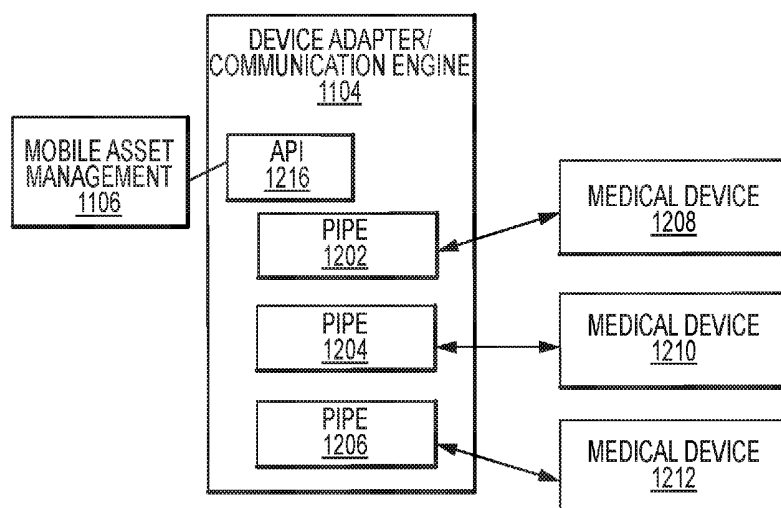


FIG. 12

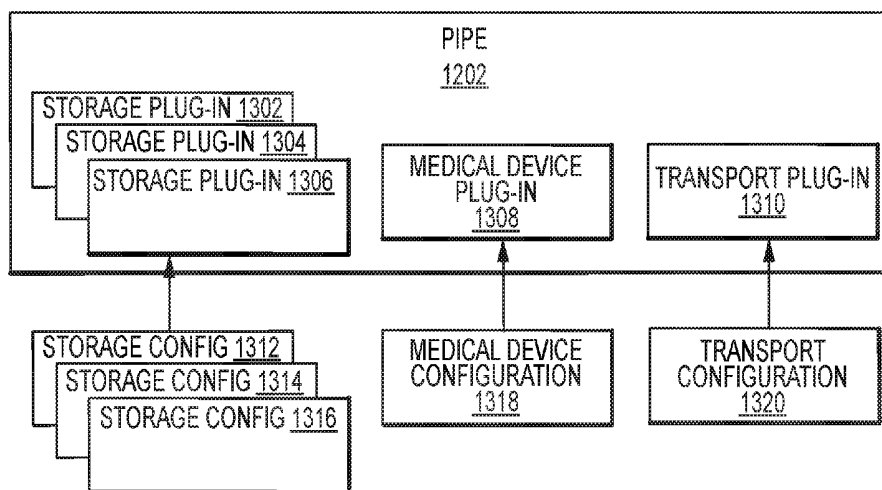


FIG. 13

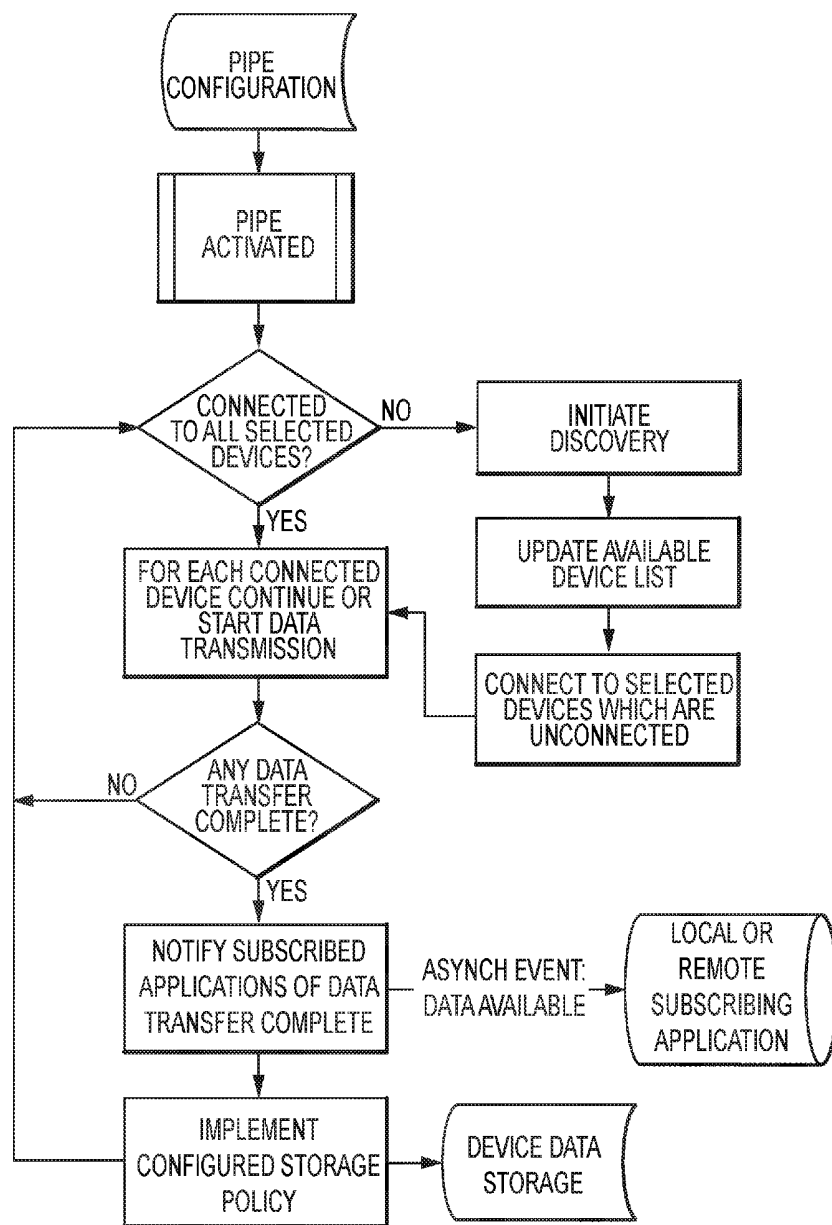


FIG. 14

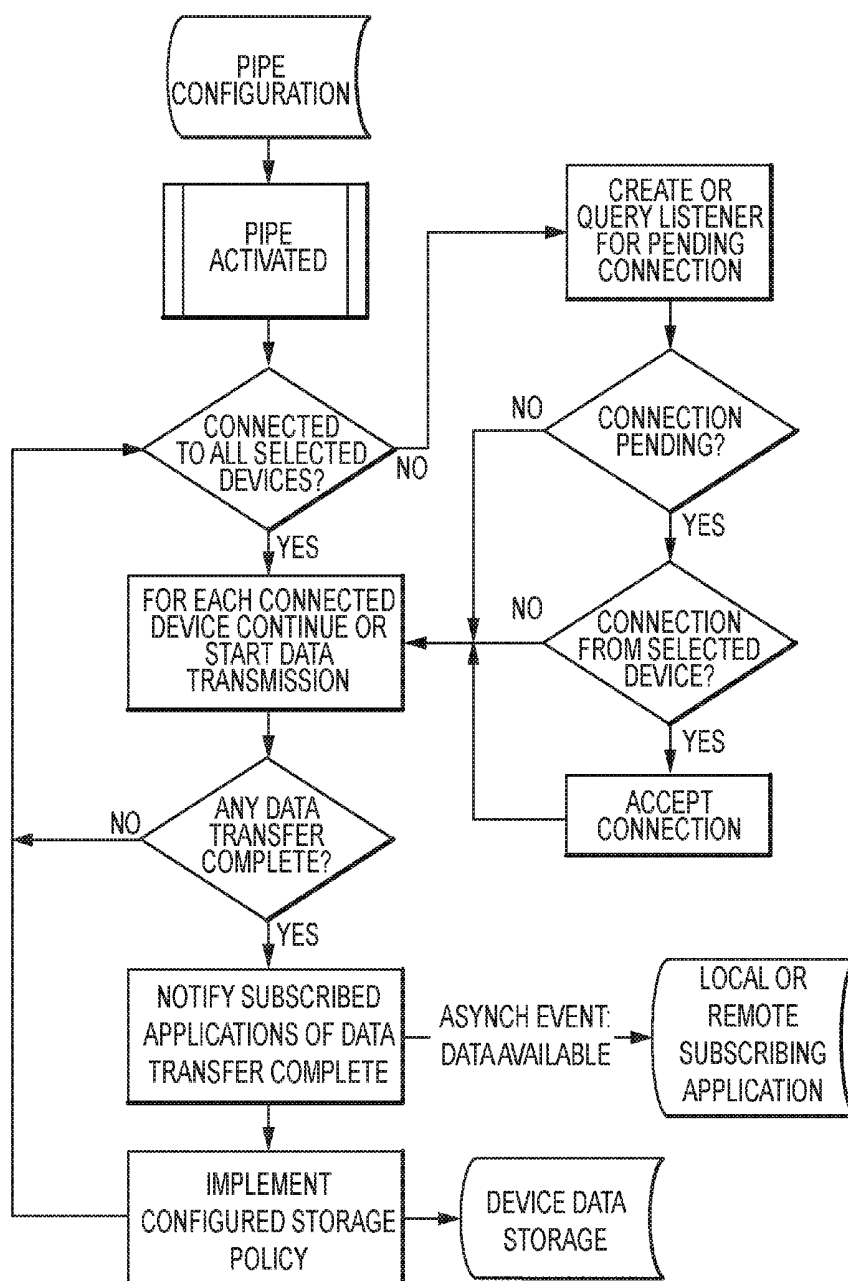


FIG. 15

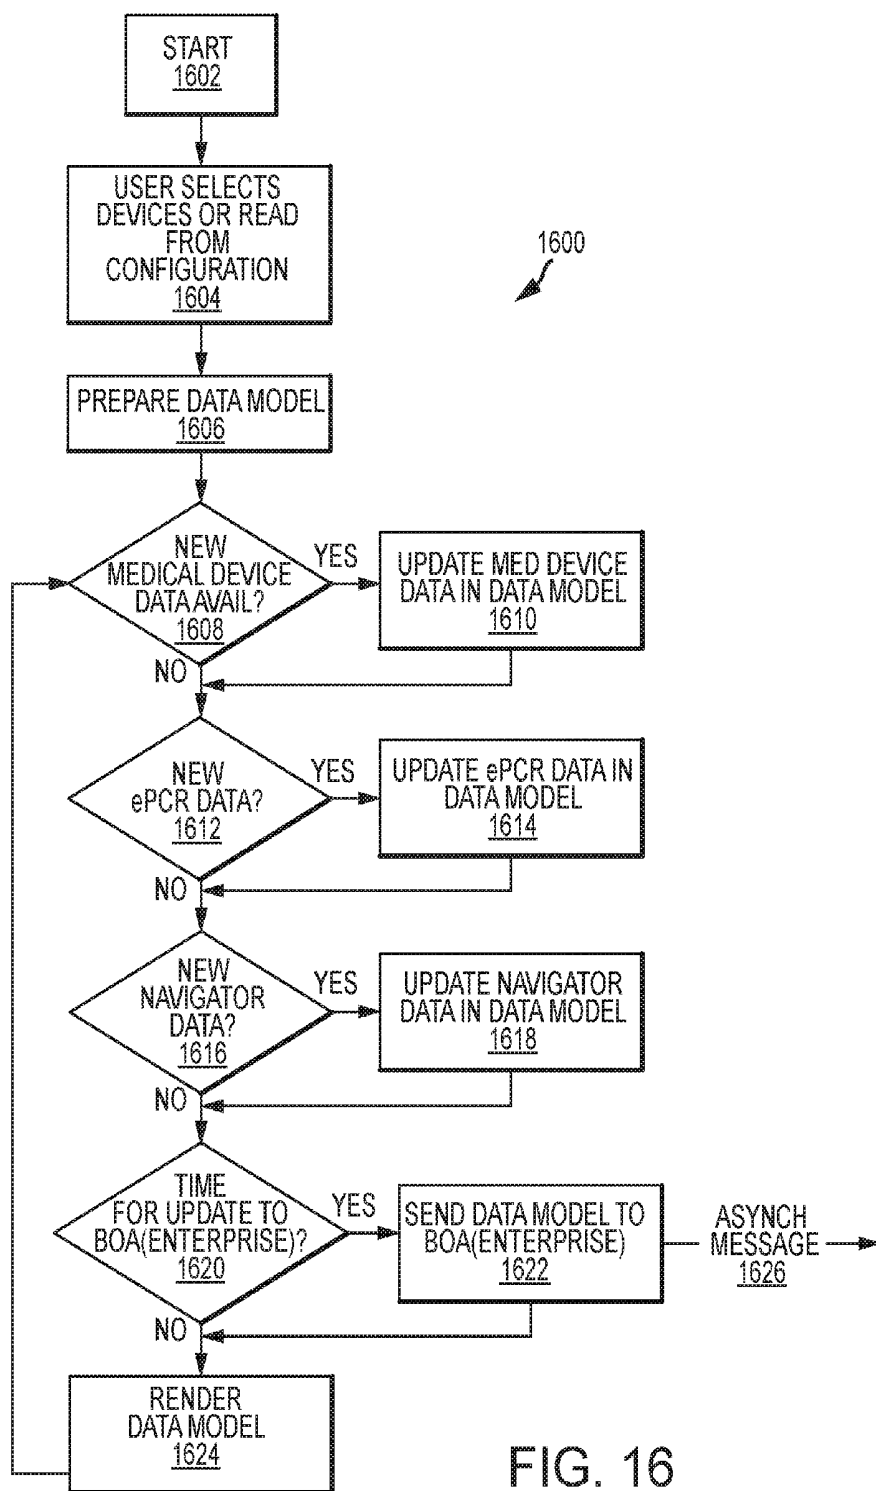


FIG. 16

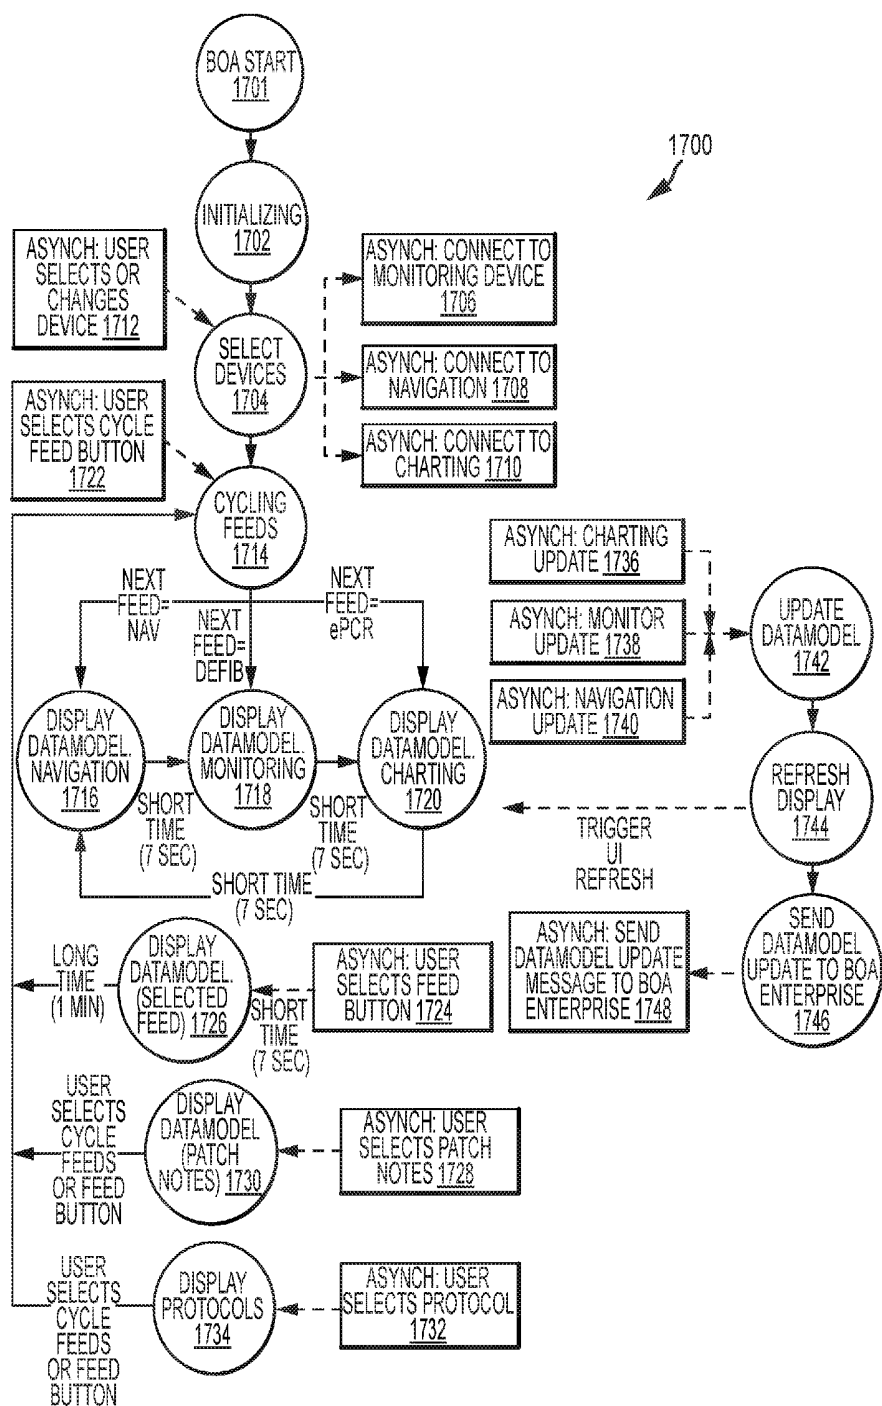


FIG. 17

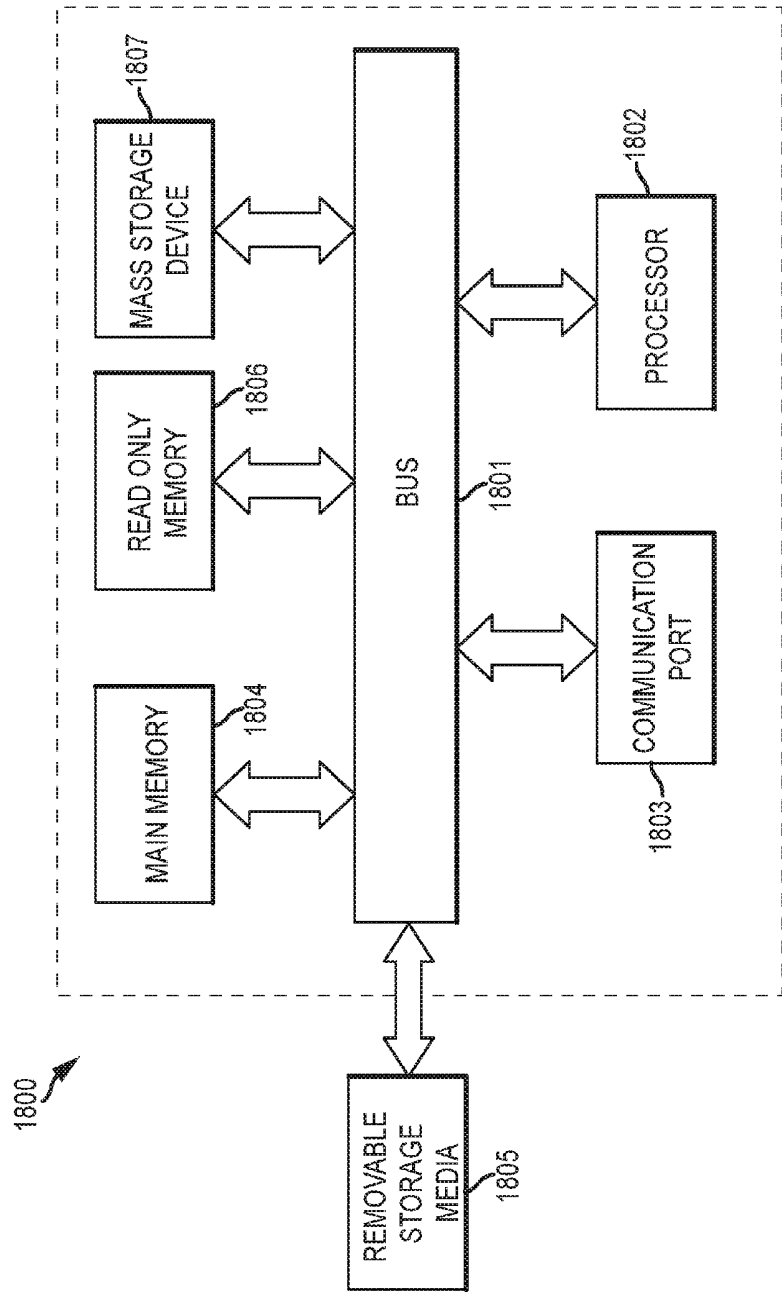


FIG. 18

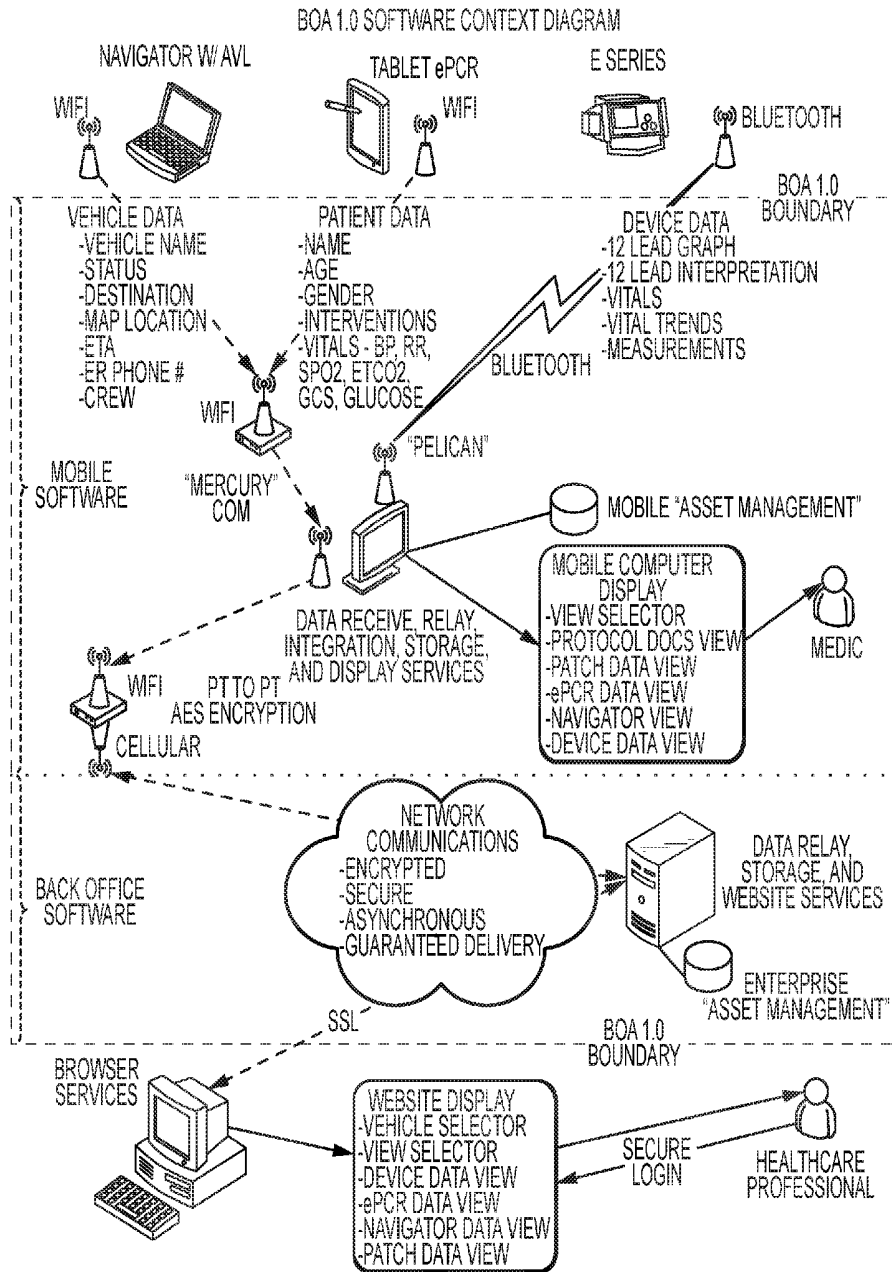


FIG. 19

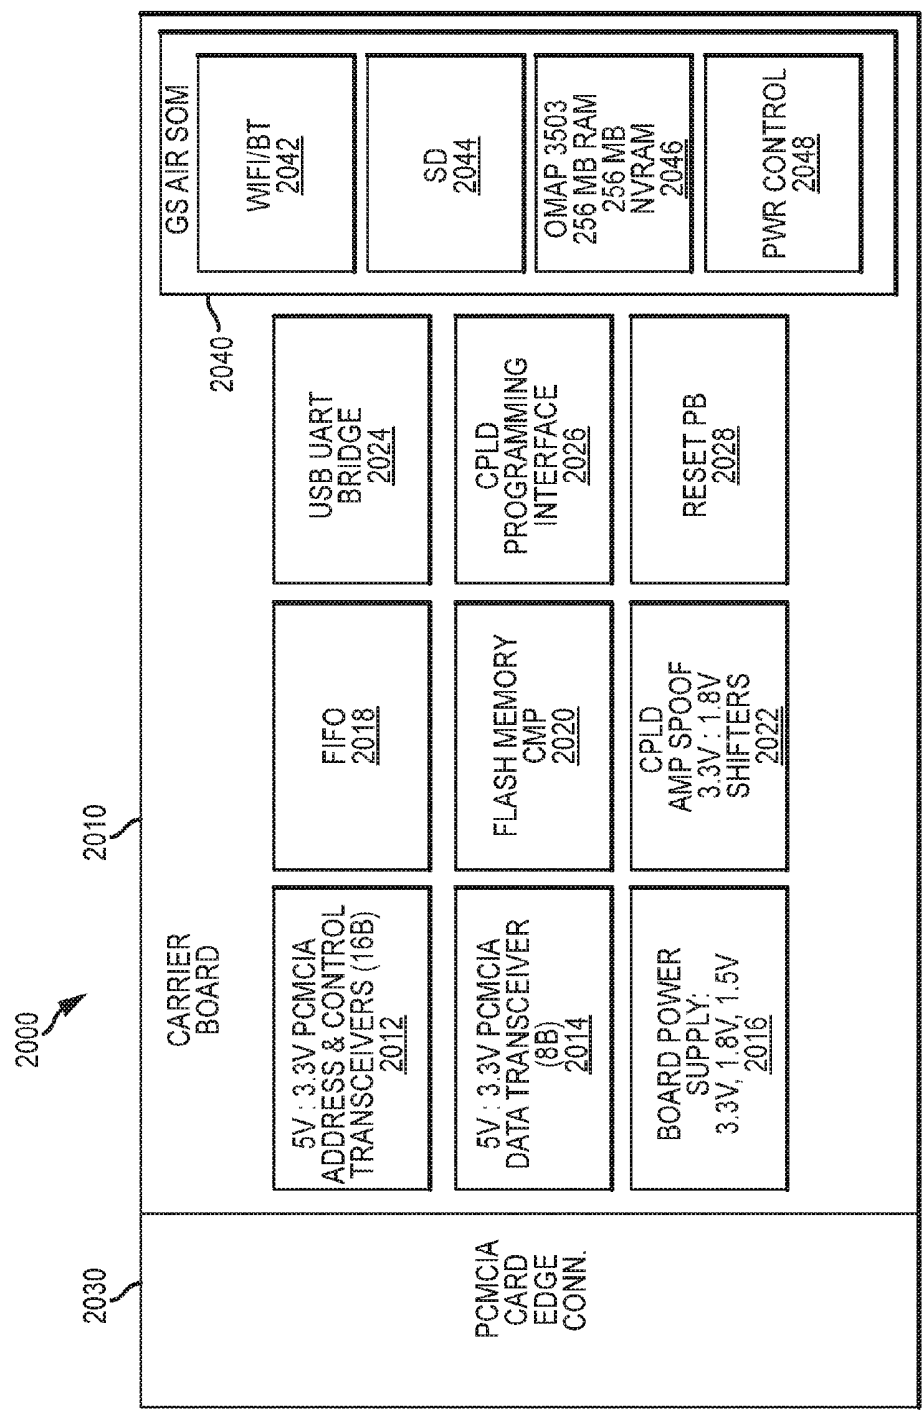


FIG. 20

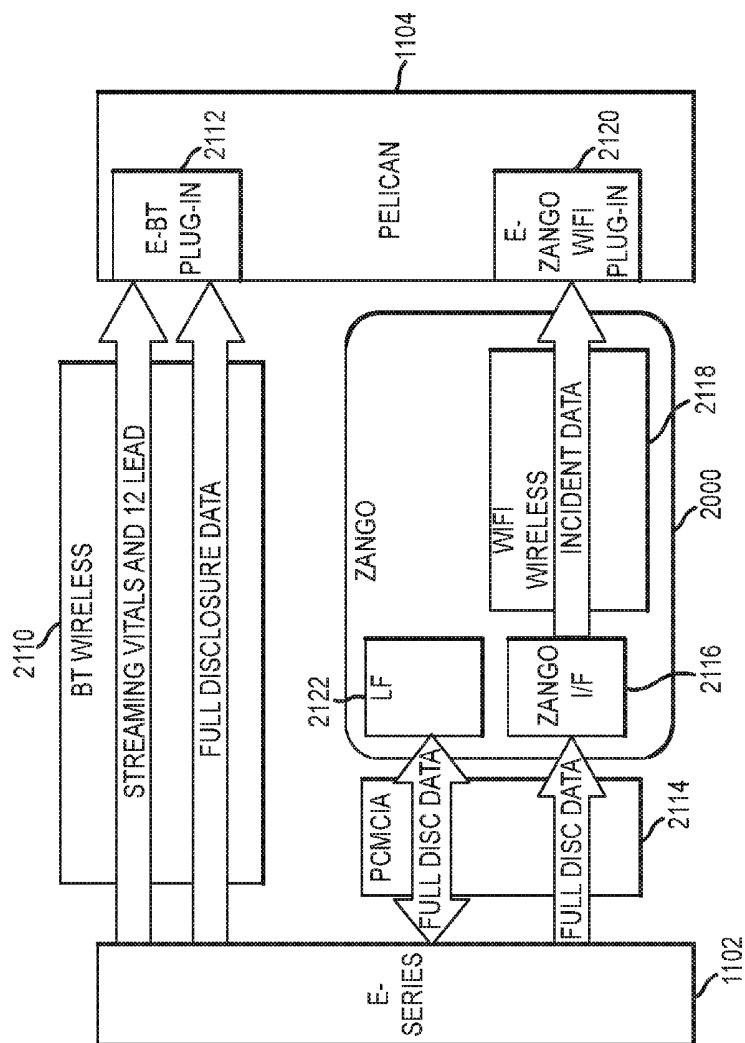


FIG. 21

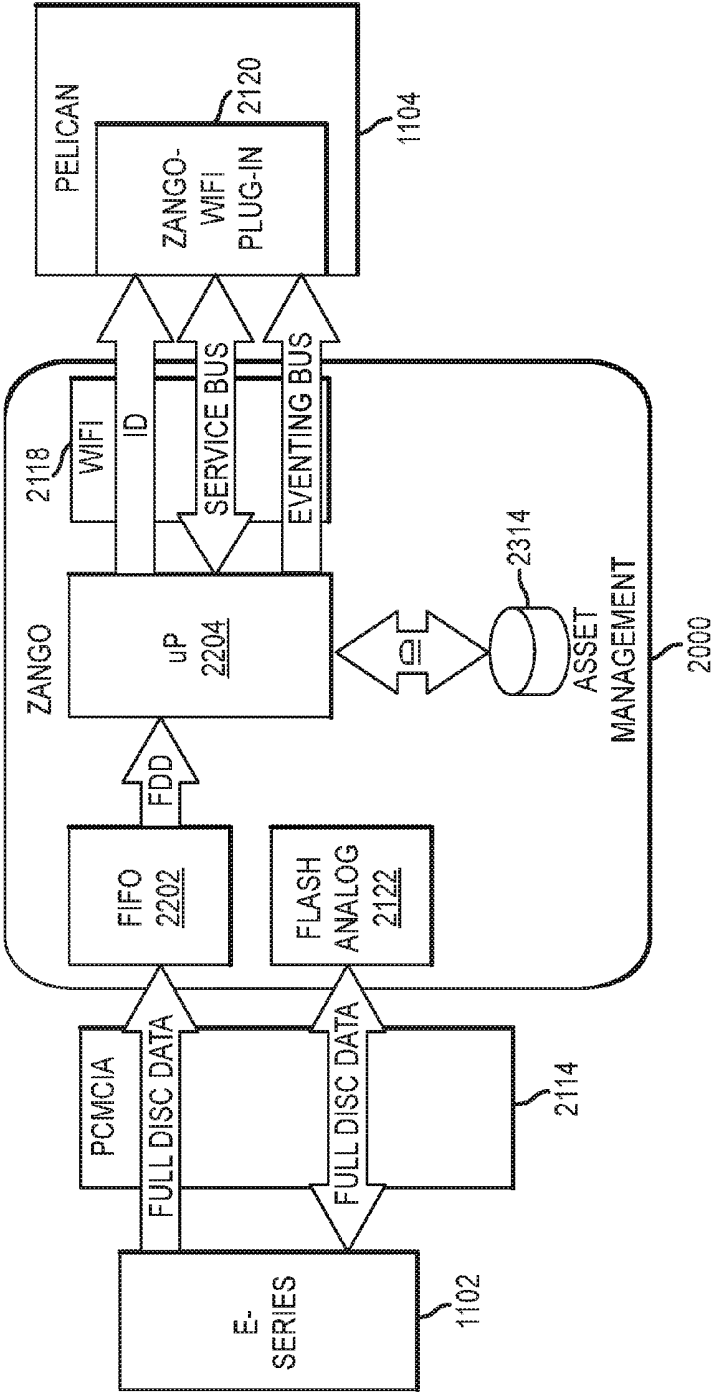


FIG. 22

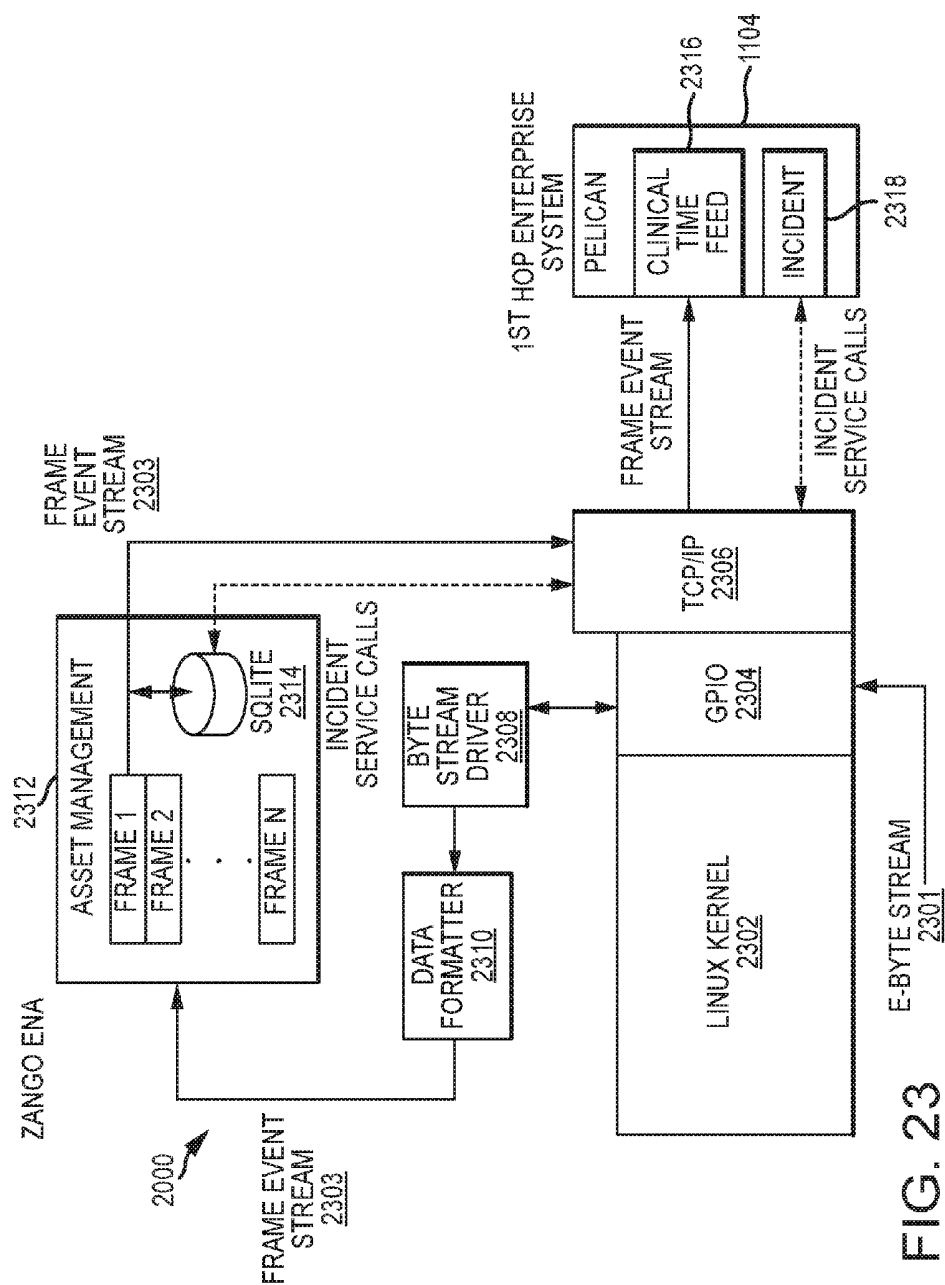
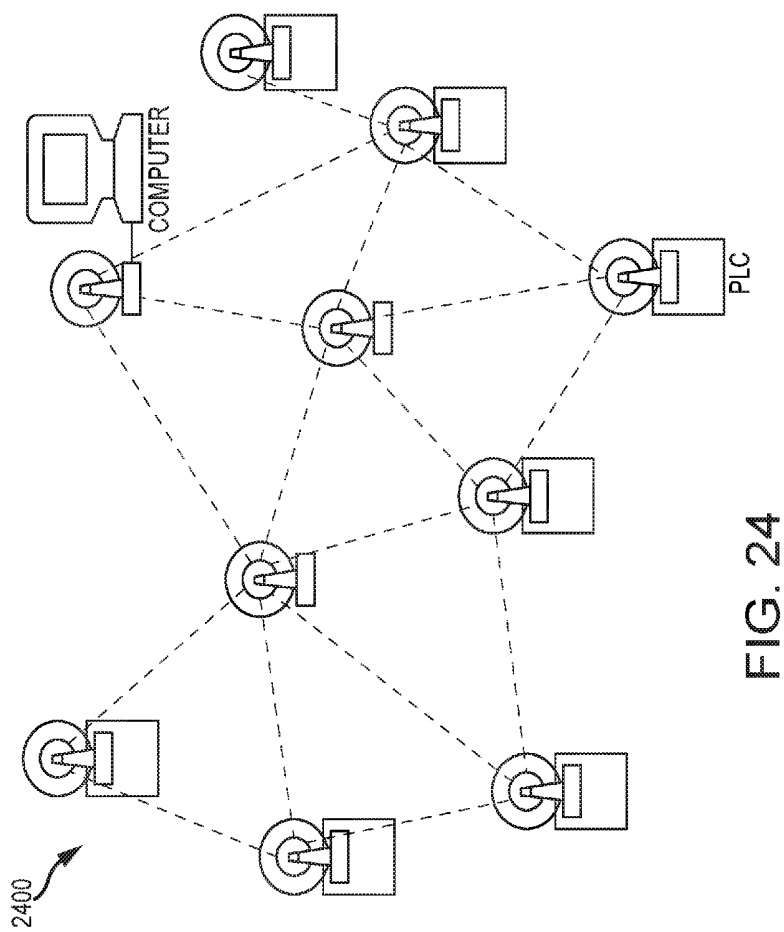


FIG. 23



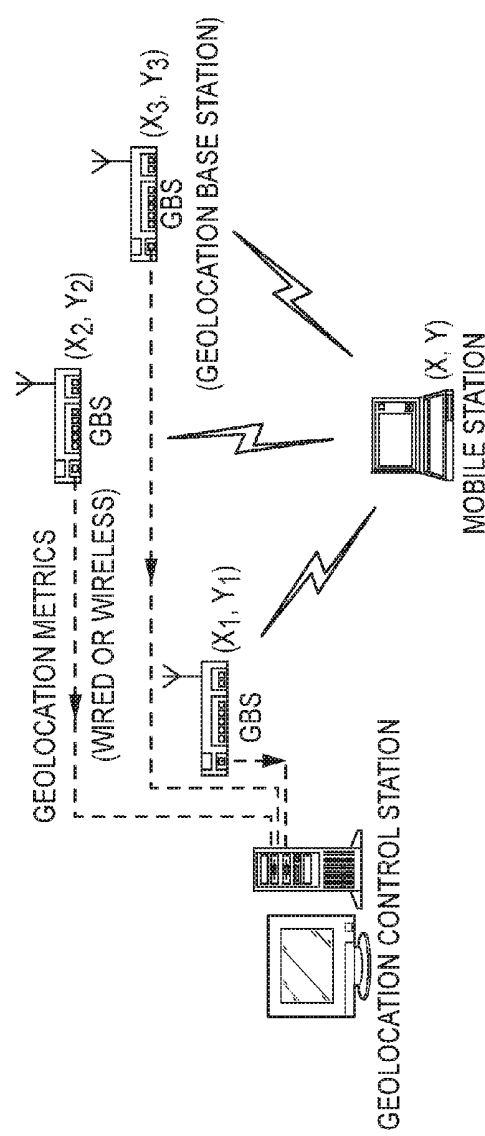


FIG. 25

DIFFERENTIAL DIAGNOSIS OF ACUTE DYSPNEA IN ADULTS

CARDIAC: CONGESTIVE HEART FAILURE, CORONARY ARTERY DISEASE, ARRHYTHMIA,
PERICARDITIS, ACUTE MYOCARDIAL INFARCTION, ANEMIA
PULMONARY: CHRONIC OBSTRUCTIVE PULMONARY DISEASE, ASTHMA, PNEUMONIA,
PNEUMOTHORAX, PULMONARY EMBOLISM, PLEURAL EFFUSION, METASTATIC DISEASE,
PULMONARY EDEMA, GASTROESOPHAGEAL REFLUX DISEASE WITH ASPIRATION, RESTRICTIVE
LUNG DISEASE
PSYCHOGENIC: PANIC ATTACKS, HYPERVENTILATION, PAIN, ANXIETY
UPPER AIRWAY OBSTRUCTION: EPIGLOTTITIS, FOREIGN BODY, CROUP, EPSTEIN-BARR VIRUS
ENDOCRINE: METABOLIC ACIDOSIS, MEDICATIONS
CENTRAL: NEUROMUSCULAR DISORDERS, PAIN, ASPIRIN OVERDOSE
PEDIATRIC: BRONCHIOLITIS, CROUP, EPIGLOTTITIS, FOREIGN BODY ASPIRATION, MYOCARDITIS

FIG. 26


CLUES TO THE DIAGNOSIS OF DYSPNEA	
SYMPTOMS OR FEATURES IN THE HISTORY	POSSIBLE DIAGNOSIS
COUGH	ASTHMA, PNEUMONIA
SEVERE SORE THROAT	EPIGLOTTITIS
PLEURITIC CHEST PAIN	PERICARDITIS, PULMONARY EMBOLISM, PNEUMOTHORAX, PNEUMONIA
ORTHOPNEA, NOCTURNAL PAROXYSMAL DYSPNEA, EDEMA	CONGESTIVE HEART FAILURE
TOBACCO USE	CHRONIC OBSTRUCTIVE PULMONARY DISEASE, CONGESTIVE HEART FAILURE, PULMONARY EMBOLISM
INDIGESTION, DYSPHAGIA	GASTROESOPHAGEAL REFUX DISEASE, ASPIRATION
BARKING COUGH	CROUP

PHYSICAL EXAMINATION FINDINGS IN THE DIAGNOSIS OF ACUTE DYSPNEA	
FINDINGS	POSSIBLE DIAGNOSIS
WHEEZING, PULSUS PARADOXUS, ACCESSORY MUSCLE USE	ACUTE ASTHMA, COPD EXACERBATION
WHEEZING, CLUBBING, BARREL CHEST, DECREASED BREATH SOUNDS	COPD EXACERBATION
FEVER, CRACKLES, INCREASED FREMITUS	PNEUMONIA
EDEMA, NECK VEIN DISTENSION, S ₃ OR S ₄ HEPATOJUGULAR REFLEX, MURMURS, RALES, HYPERTENSION, WHEEZING	CONGESTIVE HEART FAILURE, PULMONARY EDEMA
WHEEZING, FRICTION RUB, LOWER EXTREMITY SWELLING	PULMONARY EMBOLISM
ABSENT BREATH SOUNDS, HYPERRESONANCE	PNEUMOTHORAX
INSPIRATORY STRIDOR, RHONCHI, RETRACTIONS	CROUP
STRIDOR, DROOLING, FEVER	EPIGLOTTITIS
STRIDOR, WHEEZING, PERSISTENT PNEUMONIA	FOREIGN BODY ASPIRATION
WHEEZING, FLARING, INTERCOSTAL RETRACTIONS, APNEA	BRONCHOLITIS
SIGHING	HYPERVENTILATION

COPD = CHRONIC OBSTRUCTIVE PULMONARY DISEASE

FIG. 27

FIG. 28

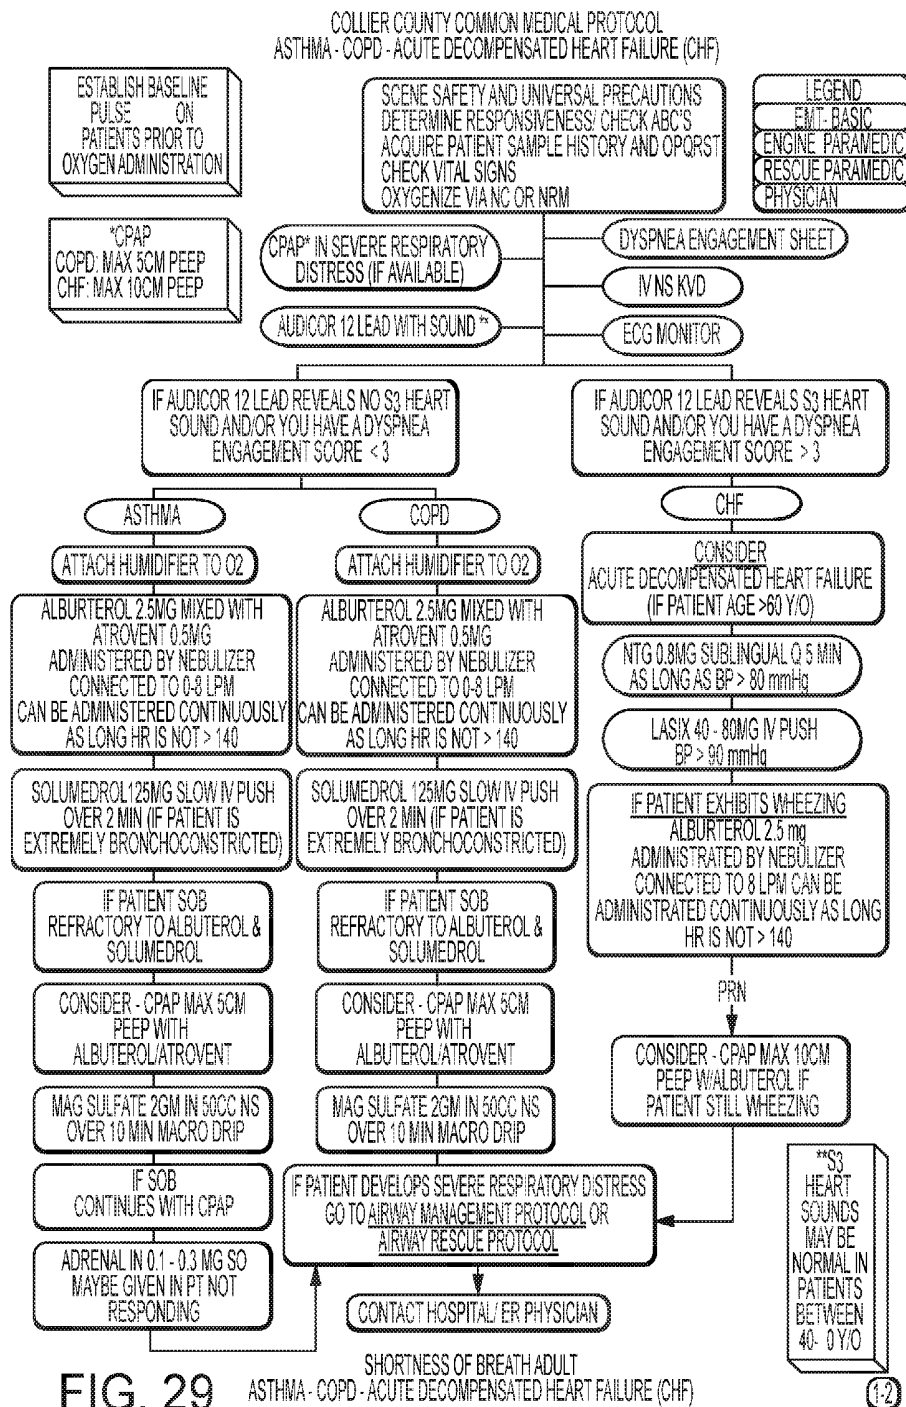

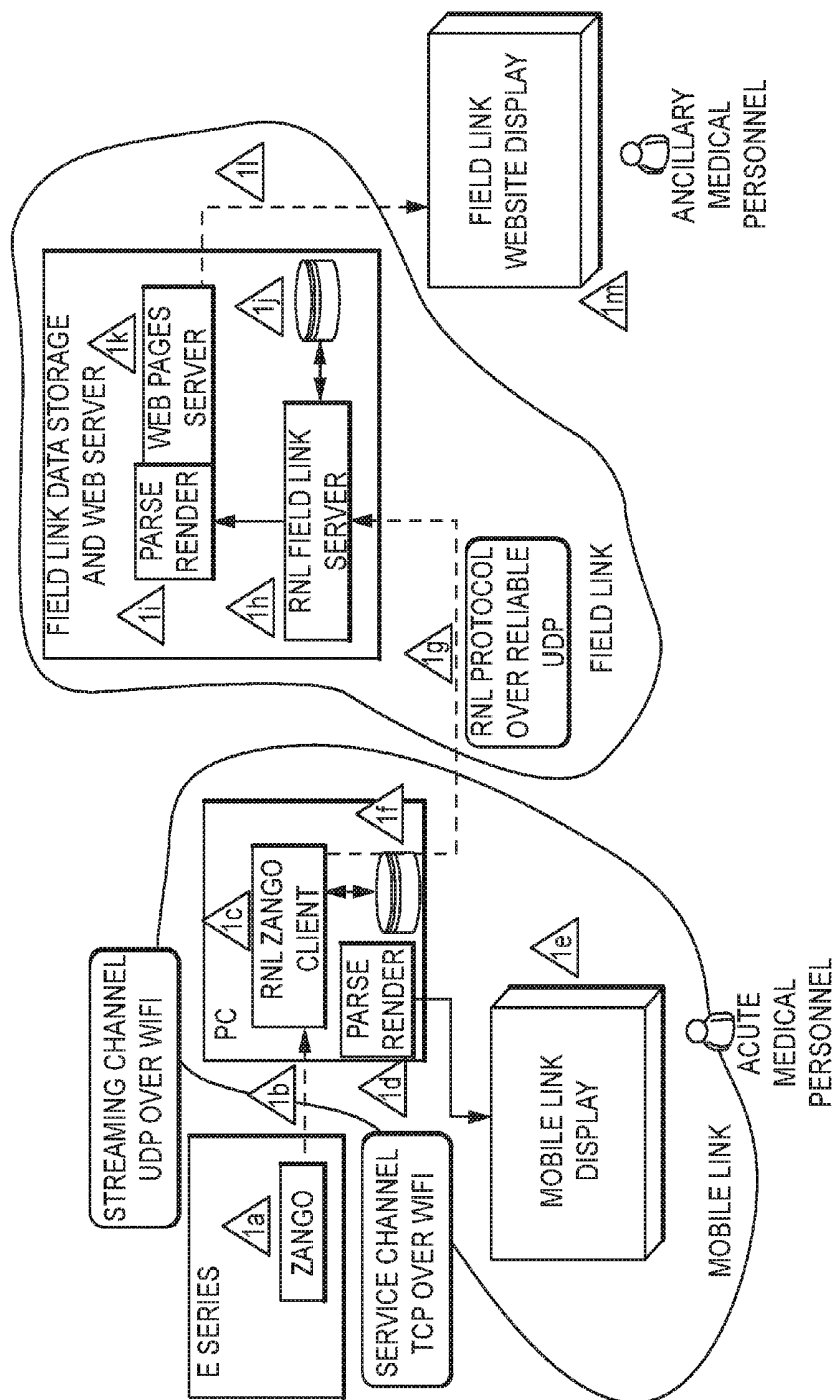


FIG. 30



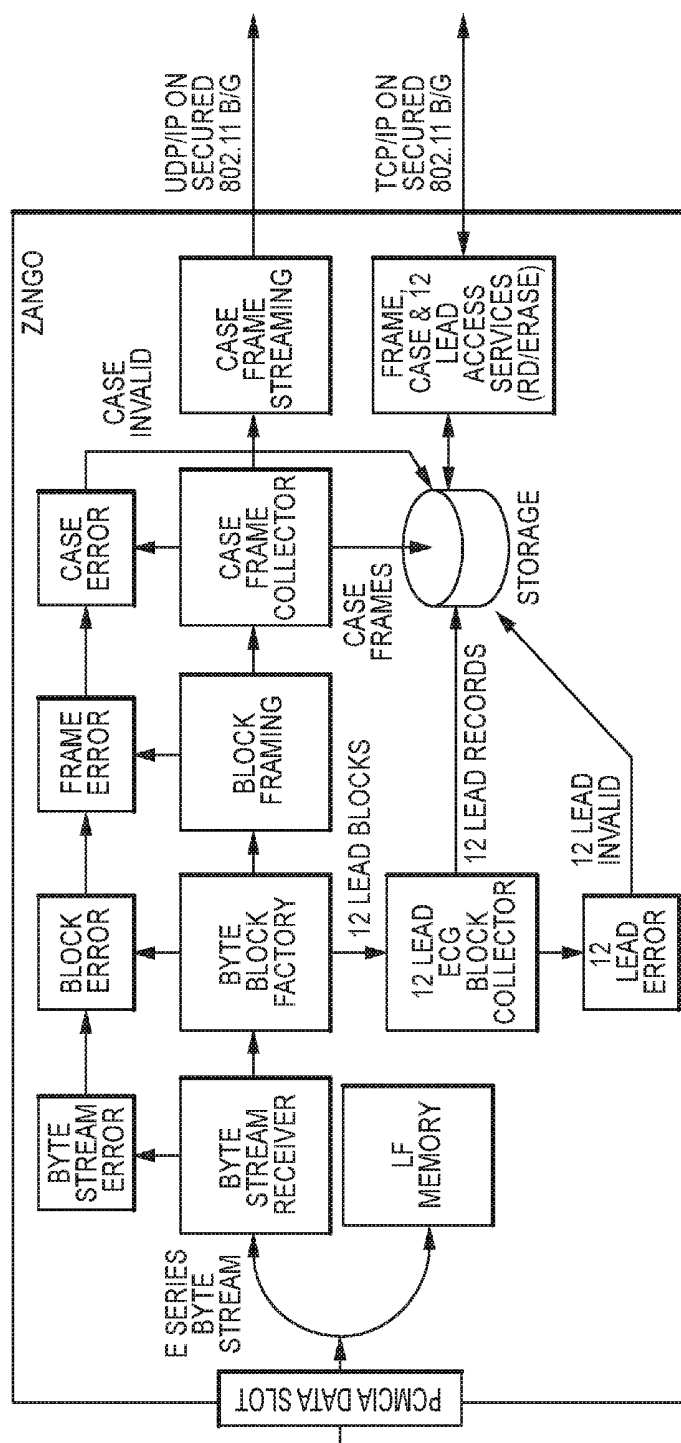


FIG. 31

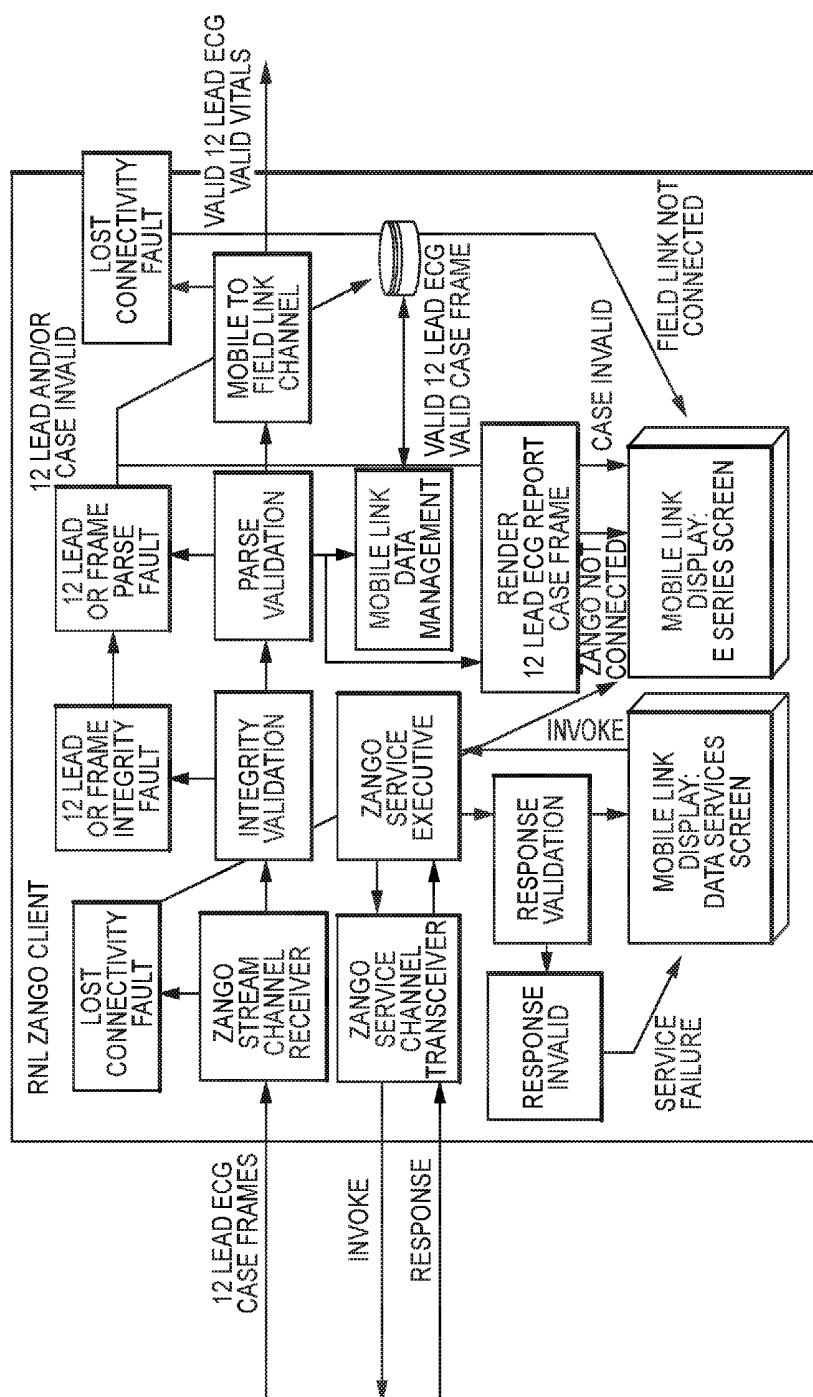

234

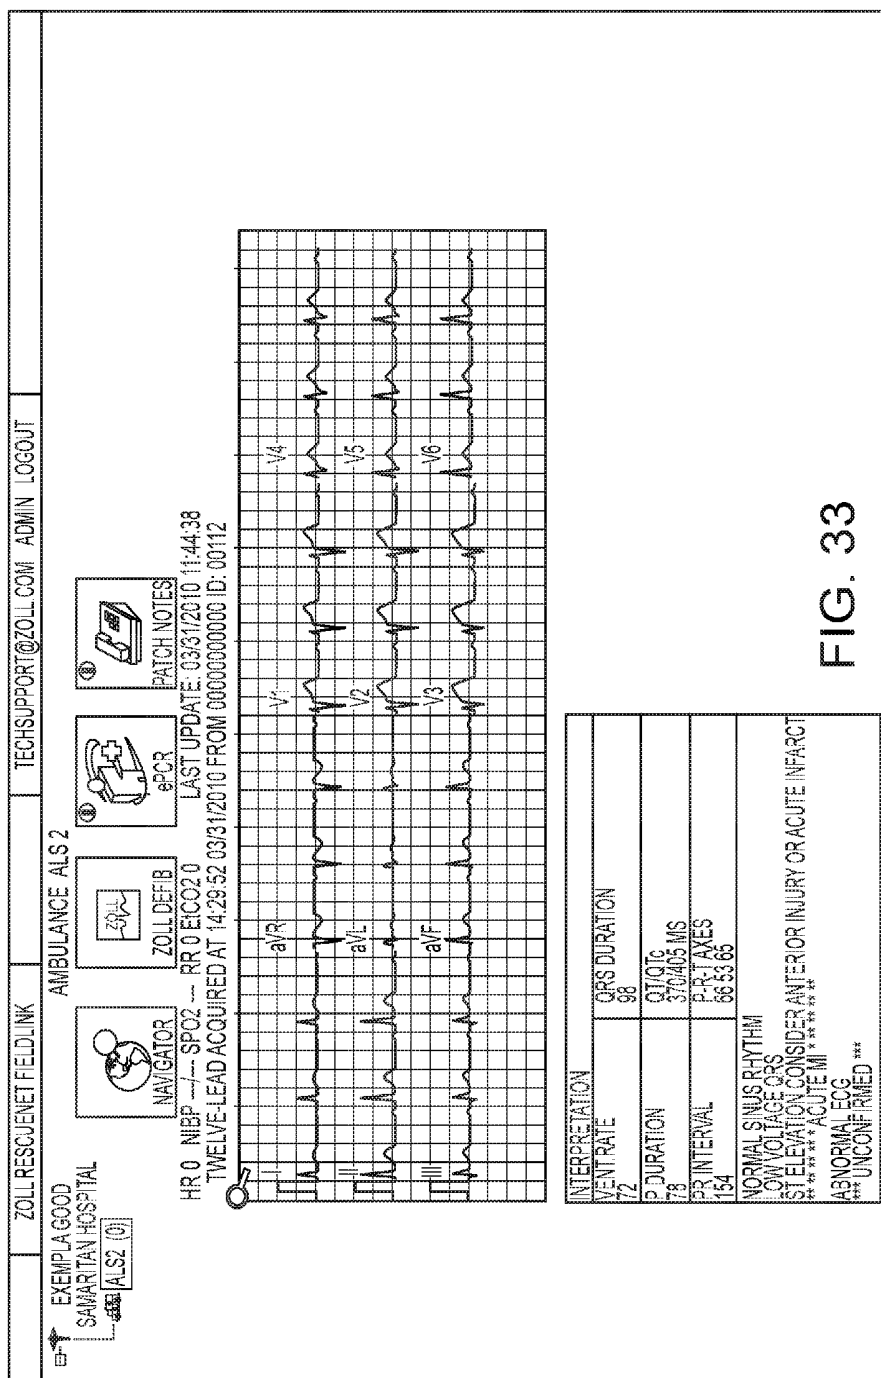

EXAMPLE GOOD

SAWARTAN HOSPITAL

ALS 2 (0)

ZOLL RESCUE NET FIELD LINK

AMBULANCE ALS 2

NAVIGATOR

ZOLL DEFIB

ePCR

PATCH NOTES

TECHSUPPORT@ZOLL.COM

ADMIN

LOGOUT

NAME: DOE, JOHN

AGE: 55 YEARS

GENDER: M

LAST UPDATE: 03/31/2010 15:09:33

INTERVENTIONS

TIME	DESCRIPTION	BY
11:45:38	ATROPINE	MUSTARD, ALASTAIR
11:45:32	EPI 10000	MUSTARD, ALASTAIR
11:45:28	OXYGEN BVM	MUSTARD, ALASTAIR
11:45:24	IV	MUSTARD, ALASTAIR
11:45:16	AIRWAY PATENT	MUSTARD, ALASTAIR

VITALS

TIME	HR	BP	RR	SpO2	ETCO2	BGL	GCS	BY
11:52:16	72		25	95				MUSTARD, ALASTAIR

FIG. 34

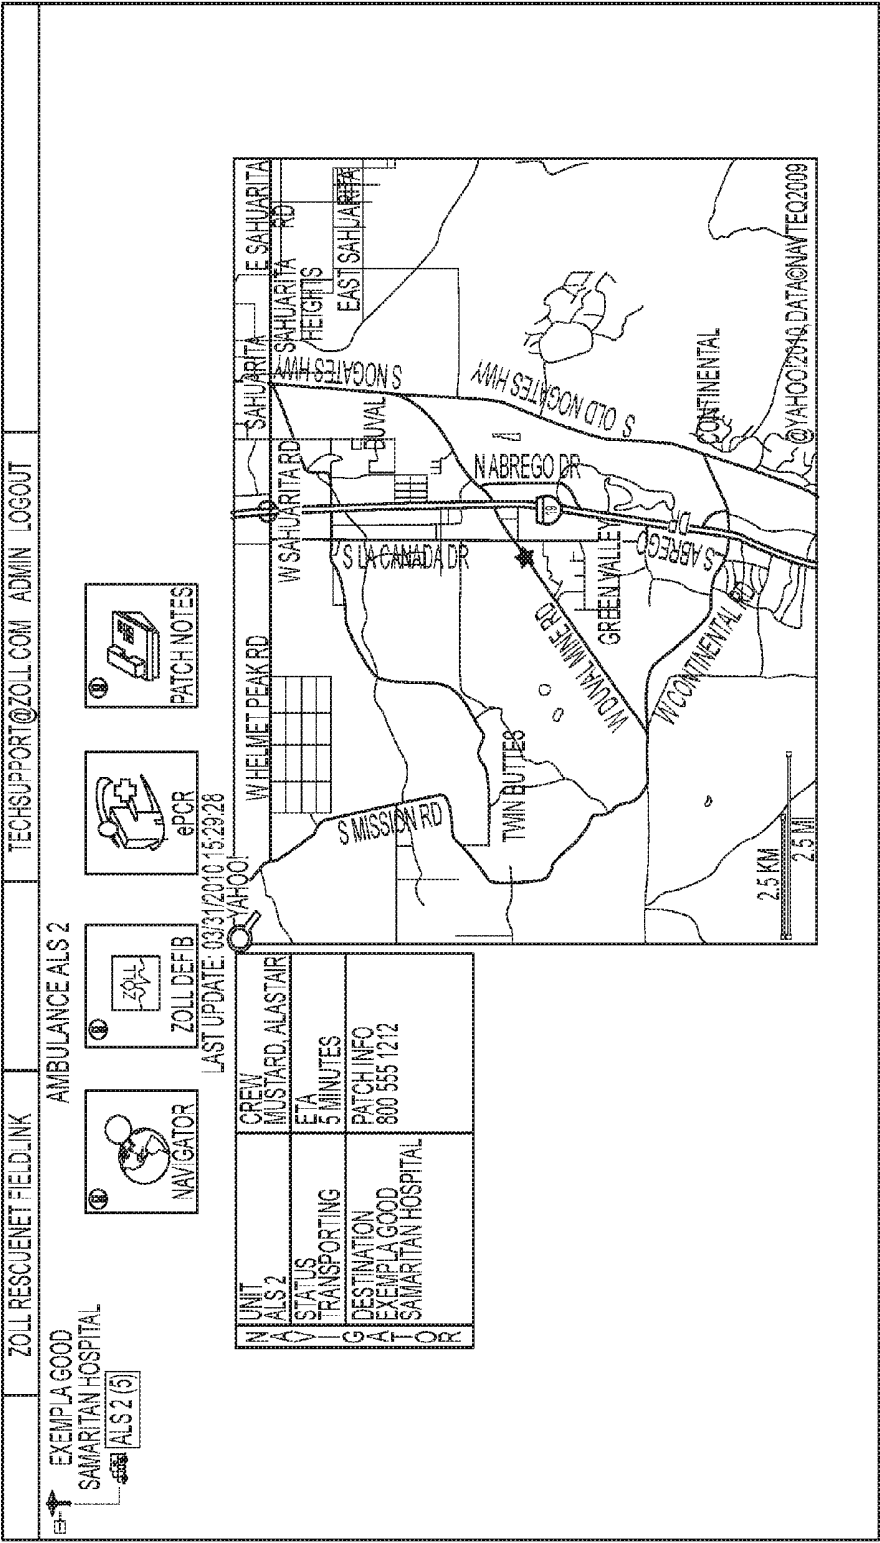


FIG. 35

	EXEMPLA GOOD SAMARITAN HOSPITAL	ZOLL RESCUE NET FIELD LINK	AMBULANCE ALS 2	TECH SUPPORT@ZOLL.COM ADMIN LOGOUT
NAVIGATOR ZOLL DEFIB ePCR PATCH NOTES				
LAST UPDATE: 03/31/2010 15:32:05				
N UNIT ALS 2	CREW MUSTARD ALASTAIR PLUM EUGENE			
G STATUS TRANSPORTING	ETA 24 MINUTES			
A DESTINATION EXEMPLA GOOD	PATCH INFO 800 555 1212			
O R SAMARITAN HOSPITAL				

33

ZOLL RESCUENET FIELDLINK		TECHSUPPORT@ZOLL.COM ADMIN LOGOUT	
 EXEMPLA GOOD SAMARITAN HOSPITAL ALS 2 [0]  NAVIGATOR  ZOLL DEFIB  ePCR  PATCH NOTES			
PATCH NOTES LAST UPDATE : 03/31/2010 15:09:33			
HOSPITAL EXEMPLA GOOD SAMARITAN HOSPITAL ALS 2 800 555 1212		UNIT AMBULANCE ALS 2	
AGE 55 YEARS		GENDER M	
INTERVENTIONS ATROPINE EPI 10000 OXYGEN BVM IV		PAST MEDICAL HISTORY CARDIAC - CORONARY HEART DISEASE ePCR VITALS 11:52:16 03/31/2010 HR: 72 BP: -- RR: 26 SPO2: 95 ETCO2: -- BGL: -- GCS: --	
AIRWAY PATENT		DEFIB VITALS 15:17:34 03/31/2010 HR: 0 NBP: --/-- RR: 0 SPO2: -- ETCO2: 0	
		ETA 0 SECONDS CHIEF COMPLAINT PRIMARY: CARDIAC ARREST ASSESSMENTS AIRWAY: WNL	

FIG. 37

ZOLL MOBILELINK					
NAME DOE, JOHN AGE 55 YEARS GENDER MALE					
INTERVENTIONS		VITALS			
TIME	DESCRIPTION	BY	RR	SpO2	GCS
11:45	ATROPINE	MUSTARD, ALAS...	26	95	BGL
11:45	EPI 10000	MUSTARD, ALAS...			ETCO2
11:45	OXYGEN 8MM IV	MUSTARD, ALAS...			
11:45	AIRWAY PATENT	MUSTARD, ALAS...			
11:45					BY MUSTARD, ALASTAIR

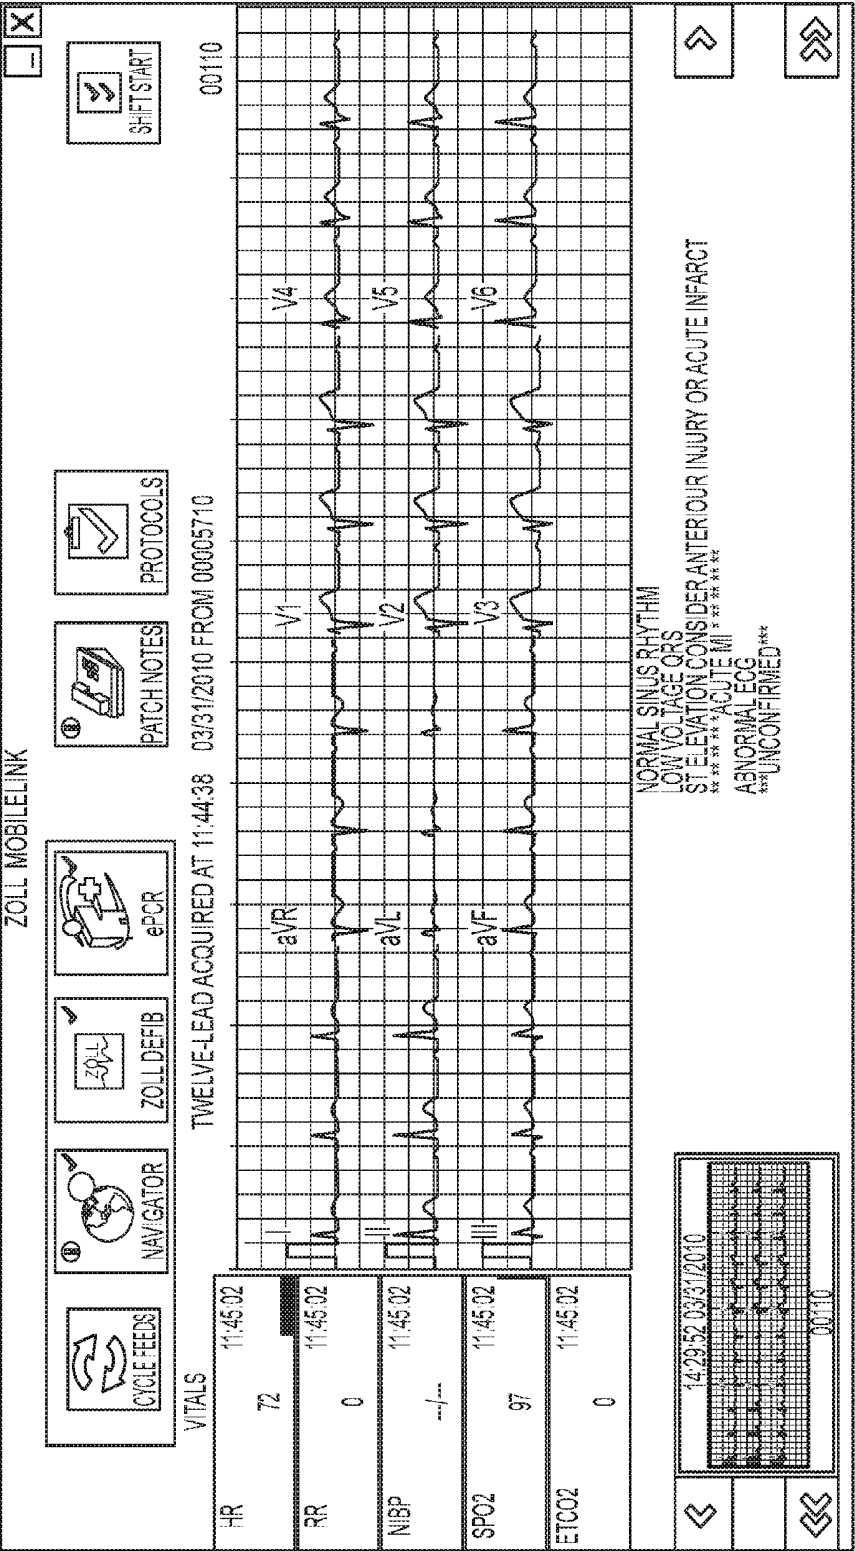


FIG. 39


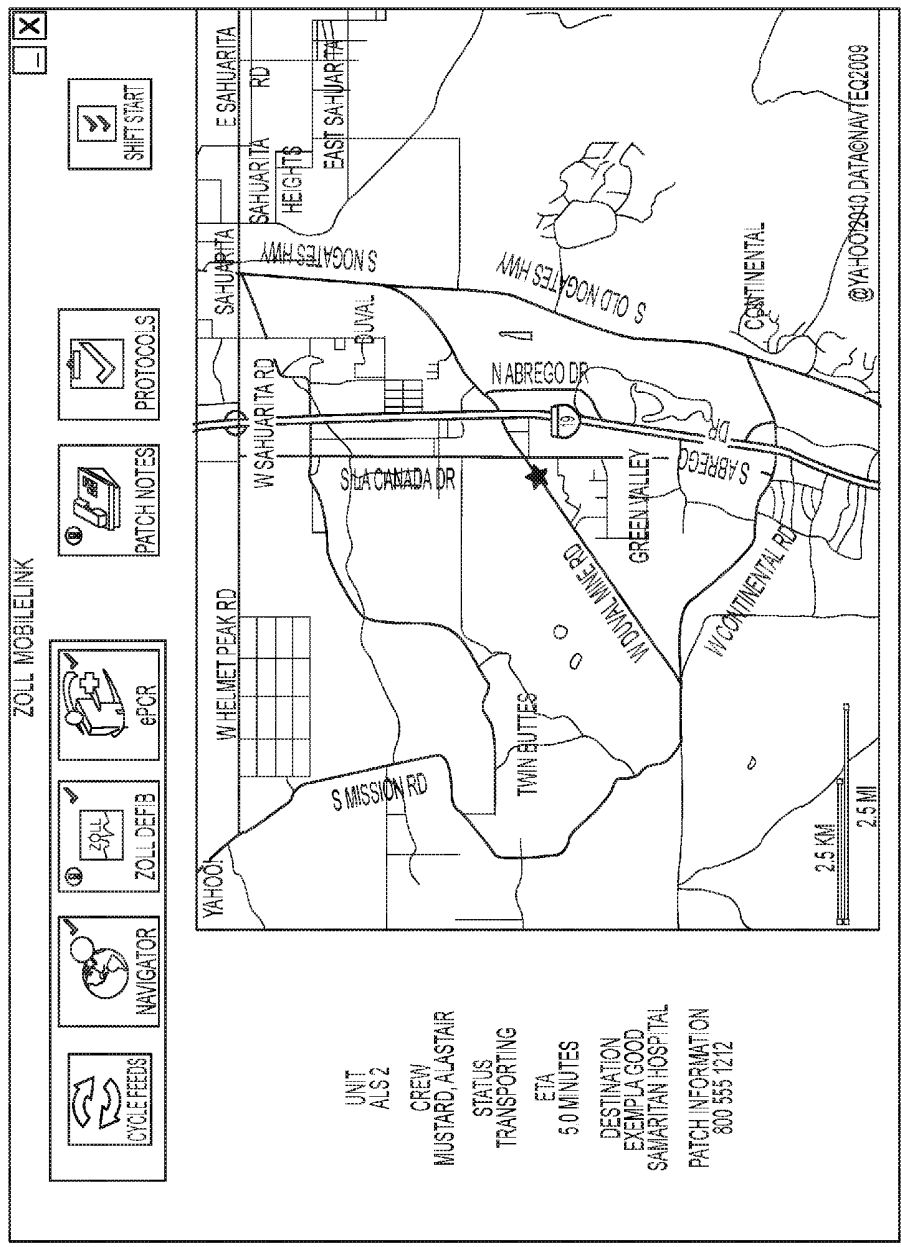


FIG. 40

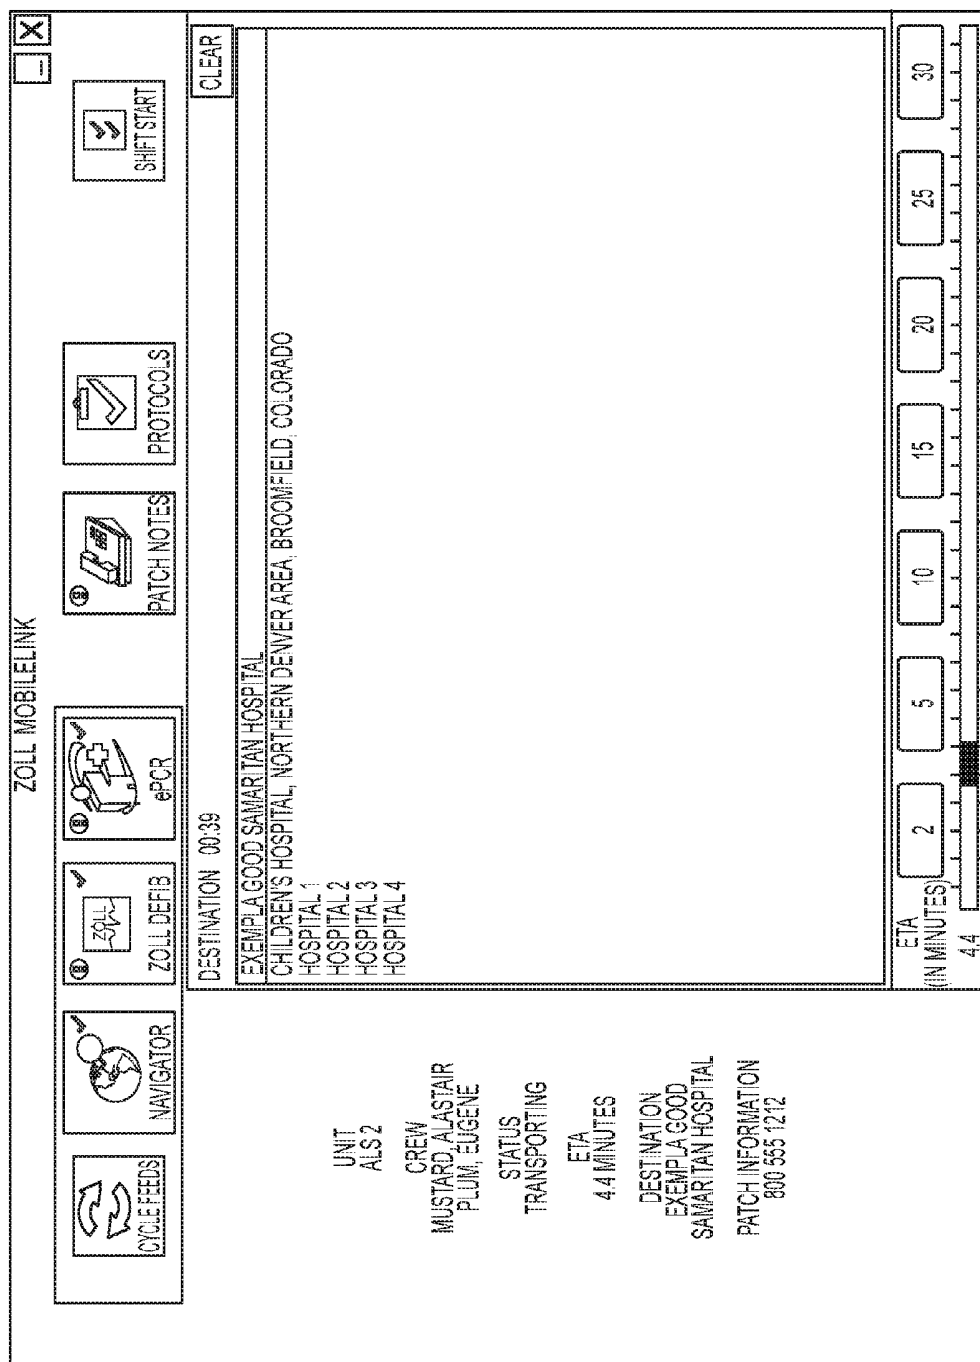

74

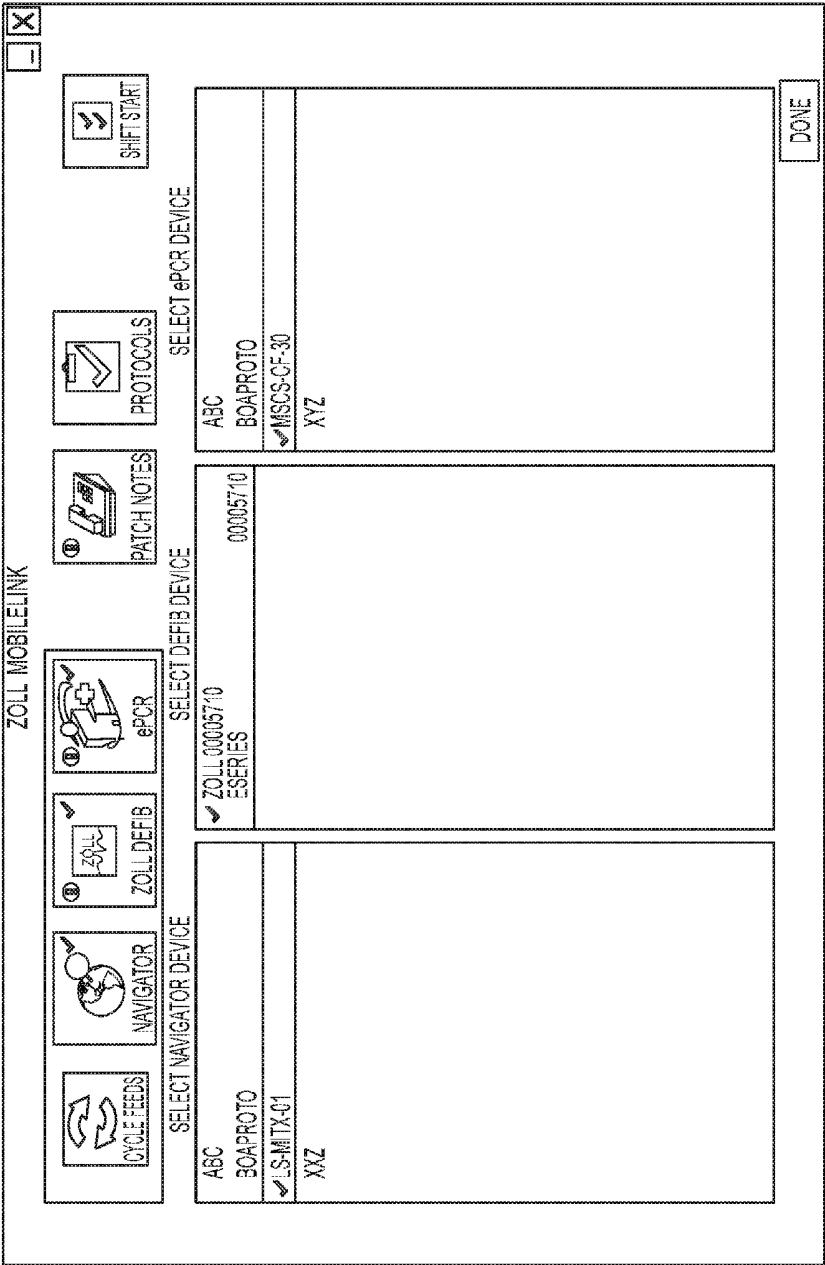


FIG. 42

CYCLE FEEDS

NAVIGATOR

ZOLL DEFIB

ePCR

PATCH NOTES

PROTOCOLS

SHIFT START

ZOLL MOBILELINK

SELECT UNIT

ALS 1

☒ ALS 2

ALS 3

ALS 4

BLS 1

BLS 2

BLS 3

SELECT CREW

☒ MUSTARD, ALASTAIR

☒ PLUM, EUGENE

SCARLET, JESSICA

PEACOCK, MARY

WHITE, EMMA

GREEN, WILLIAM

SELECT DEFIB DEVICE

☒ ZOLL 0005710
ESERIES

00005710

SELECT ePCR DEVICE

ABC

BOAPROTO

☒ MSCS-CF-30

XYZ

DONE

FIG. 43

ZOLL MOBILELINK			
 CYCLE FEEDS	 NAVIGATOR	 ZOLL DEFIB	 ePCR
DESTINATION EXEMPLA GOOD SAMARITAN HOSPITAL 800 555 1212			
UNIT ALS 2			
ETA 1.3 MINUTES			
 PATCH NOTES			
 PROTOCOLS			
 SHIFT START			
AGE 55 YEARS		GENDER MALE	
MEDICAL HISTORY CARDIAC - CORONARY HEART DISEASE		CHIEF COMPLAINT PRIMARY: CARDIAC ARREST	
[MORE...]		[MORE...]	
AIRWAY/MNL		ASSESSMENTS	
INTERVENTIONS ATROPINE EPI 1000 OXYGEN BVM IV AIRWAY PATENT		ePCR VITALS 11:52:16 03/31/2010 HR: 72 BP RR: 26 SPO2: 95 ETCO2 BGL GCS	
[MORE...]		[MORE...]	
DEFIB VITALS 15:09:36 03/31/2010 HR: 0 RR: 17 NIBP: --- SPO2: 95 ETCO2: 34		[MORE...]	

44 x FIG

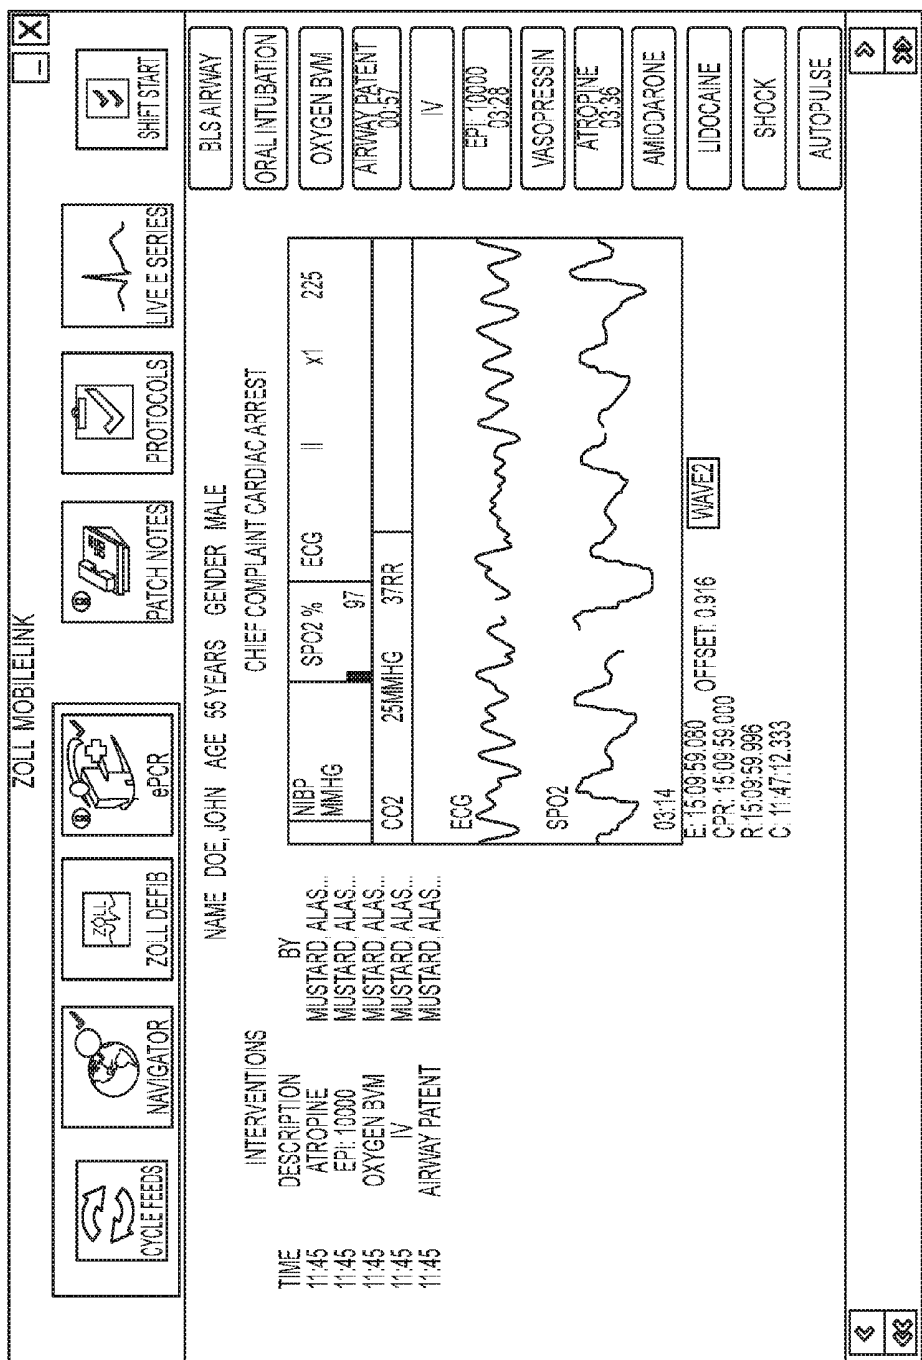


FIG. 45

AT&T 12:26 PM 92%

IP ADDRESS: 10.100.77.501

SEND PORT: 9020 RECEIVE PORT: 9021

MEDIC: MUSTARD, ALASTAIR

ROLE: MEDIC - LEAD

DONE

FIG. 46

AT&T 11:53 AM 79%

MEDIC - LEAD ✓

MEDIC - DRUGS

MEDIC - AIRWAY

MEDIC - CPR

QUICKLOG ECG GRAPH PATIENT DATA CHIEF COMPLAINT MEDIC-ROLE

FIG. 47

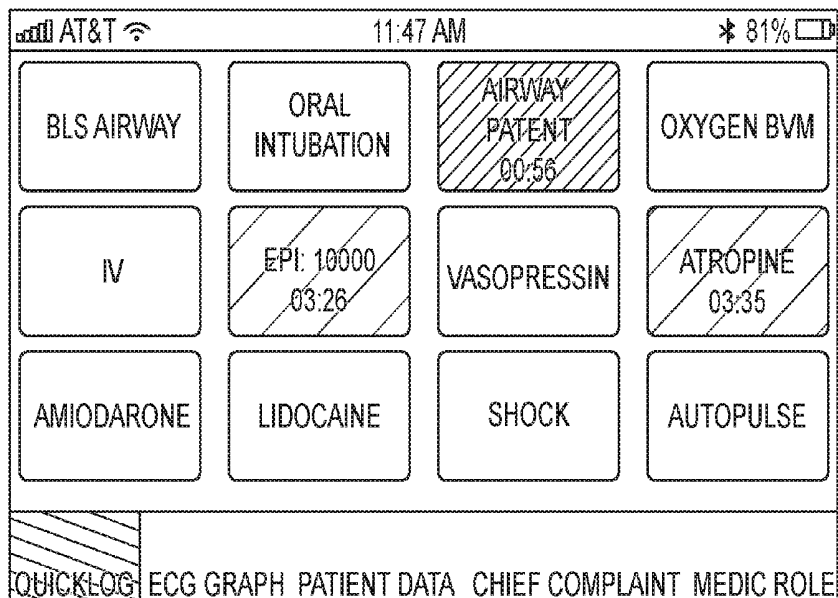


FIG. 48

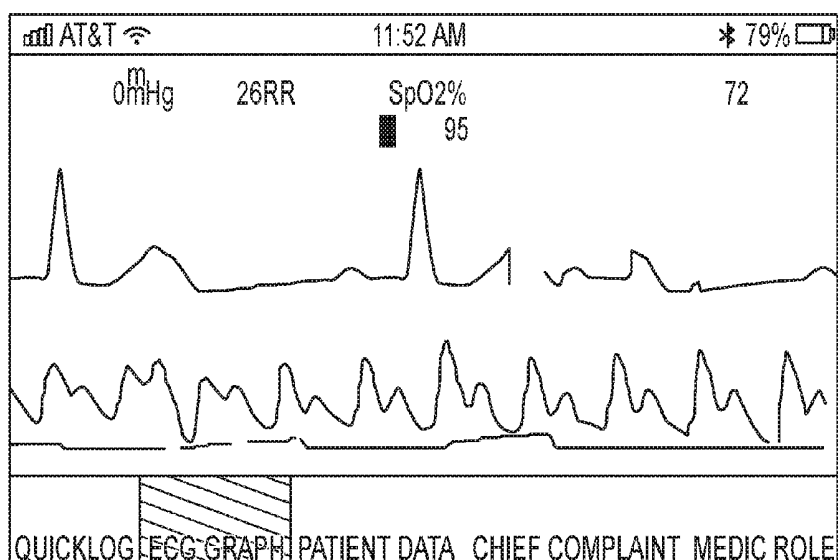


FIG. 49

AT&T 11:53 AM 79%		
PATIENT NAME: DOE, JOHN		
GENDER: MALE ☒		
FEMALE		
QUICKLOG	ECG GRAPH	PATIENT DATA
CHIEF COMPLAINT MEDIC ROLE		

FIG. 50

AT&T 11:53 AM 79%		
CHEST - PAIN		
CARDIAC ARREST ☒		
HEADACHE		
DIFFICULTY BREATHING		
PSYCH		
ALTERED MENTAL STATUS		
QUICKLOG	ECG GRAPH	PATIENT DATA CHIEF COMPLAINT MEDIC ROLE

FIG. 51

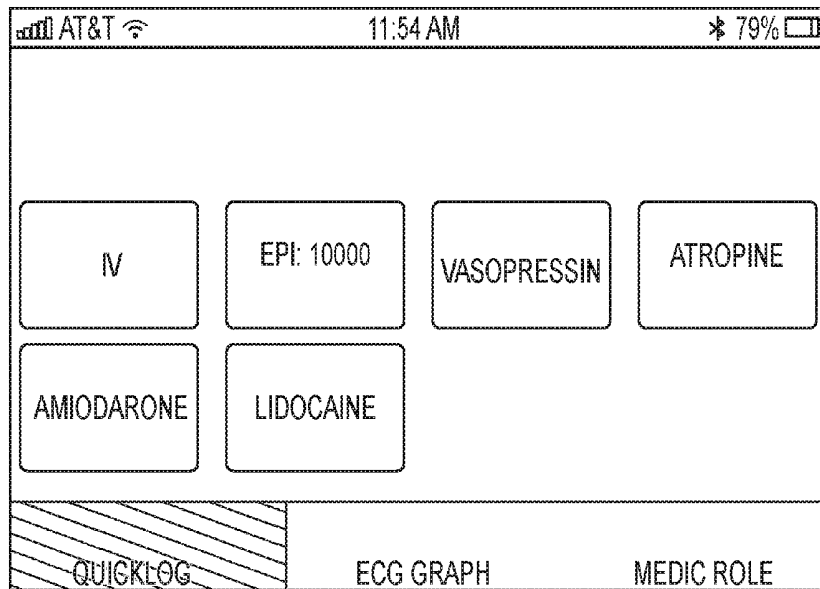


FIG. 52

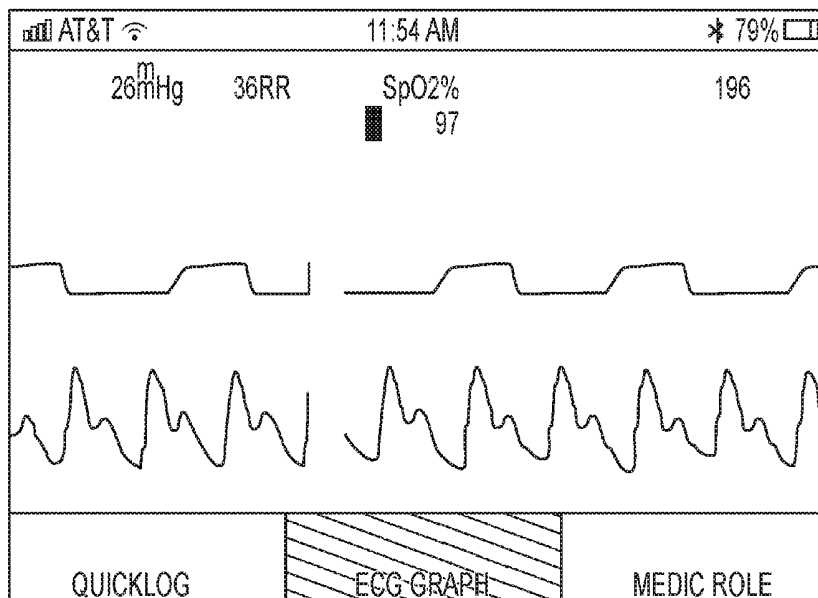


FIG. 53

AT&T 11:53 AM 79%		
MEDIC - LEAD		
MEDIC - DRUGS		
MEDIC - AIRWAY		✓
MEDIC - CPR		
QUICKLOG	ECG GRAPH	MEDIC ROLE

FIG. 54

AT&T 11:53 AM 79%		
28mHg	65RR	SpO2% 151
		
		
		
QUICKLOG	ECG GRAPH	MEDIC ROLE

FIG. 55

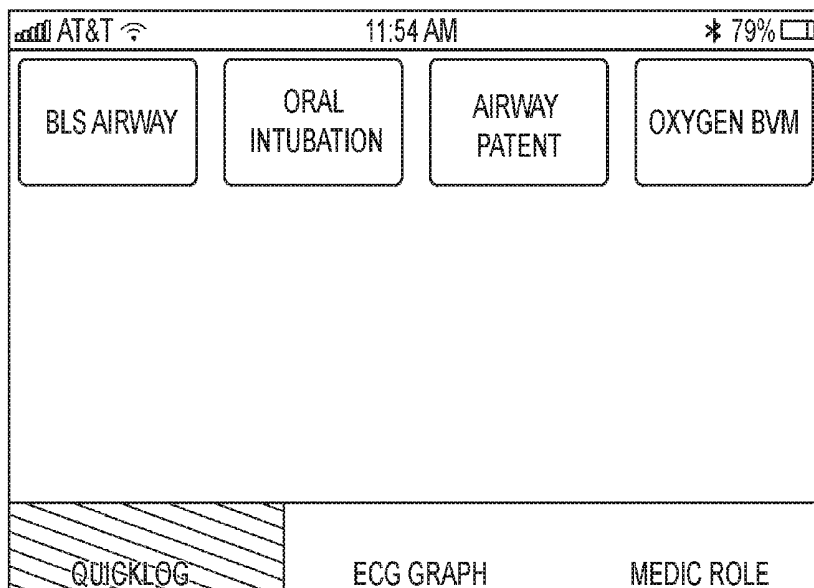


FIG. 56

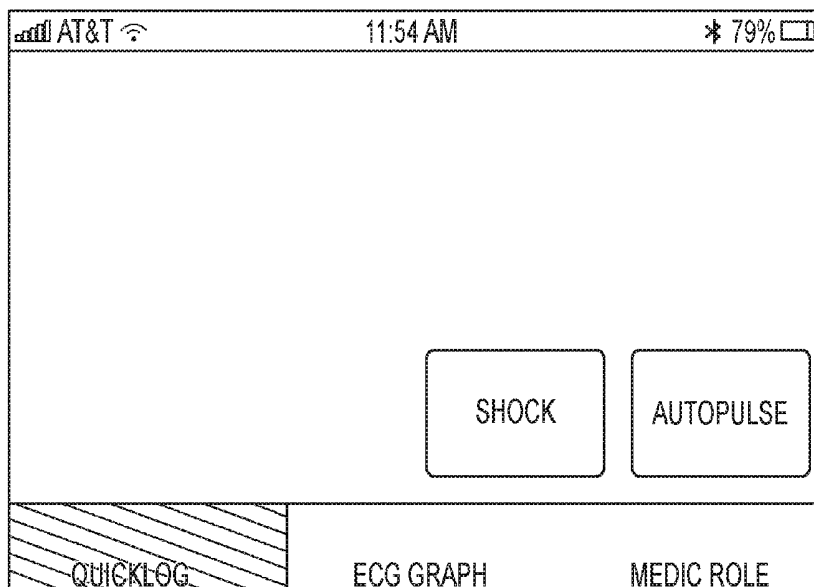


FIG. 57

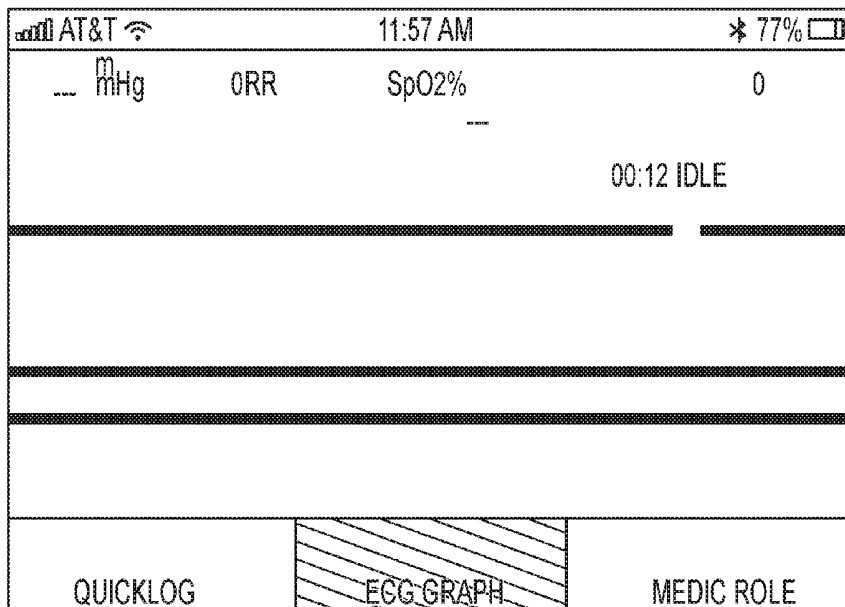


FIG. 58

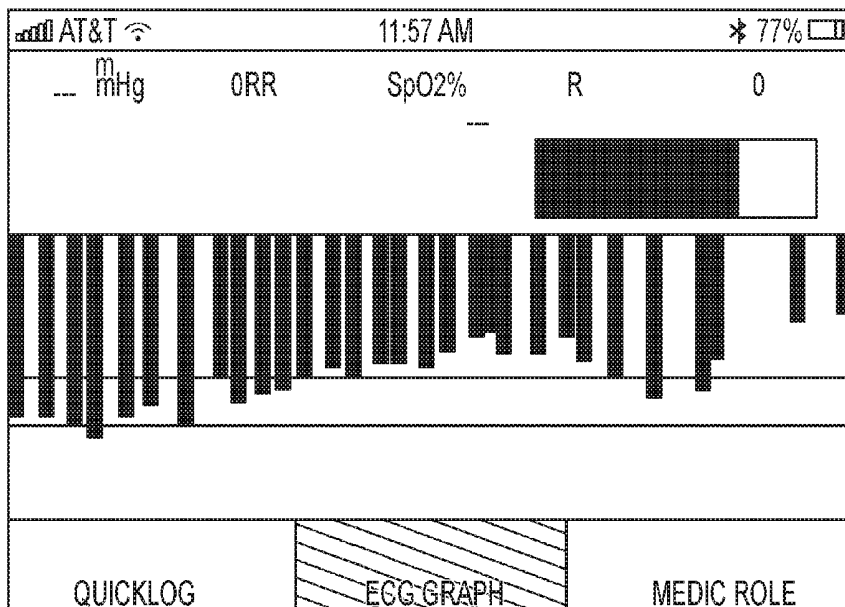


FIG. 59

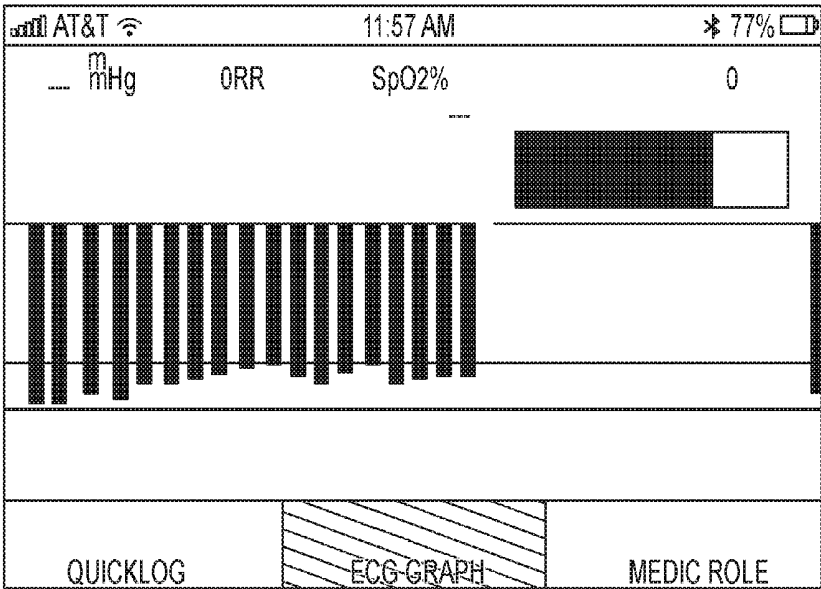


FIG. 60

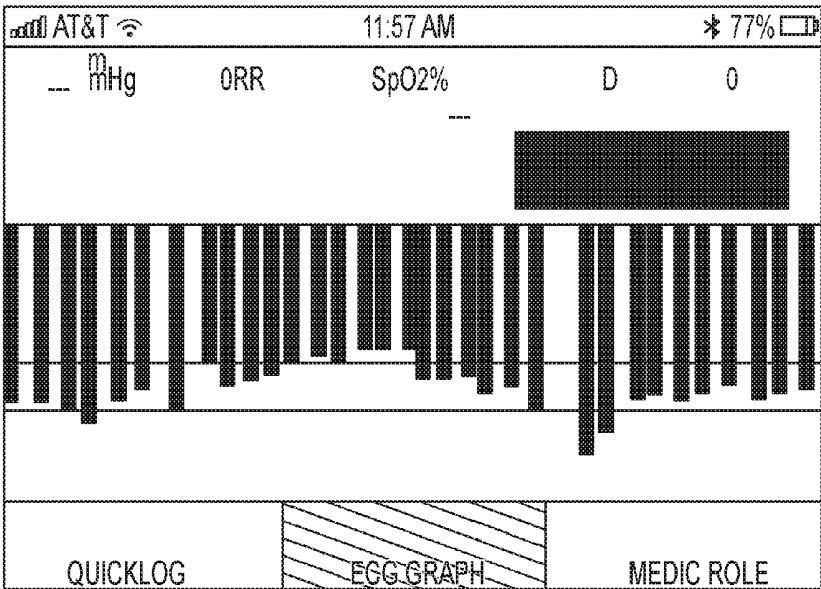


FIG. 61

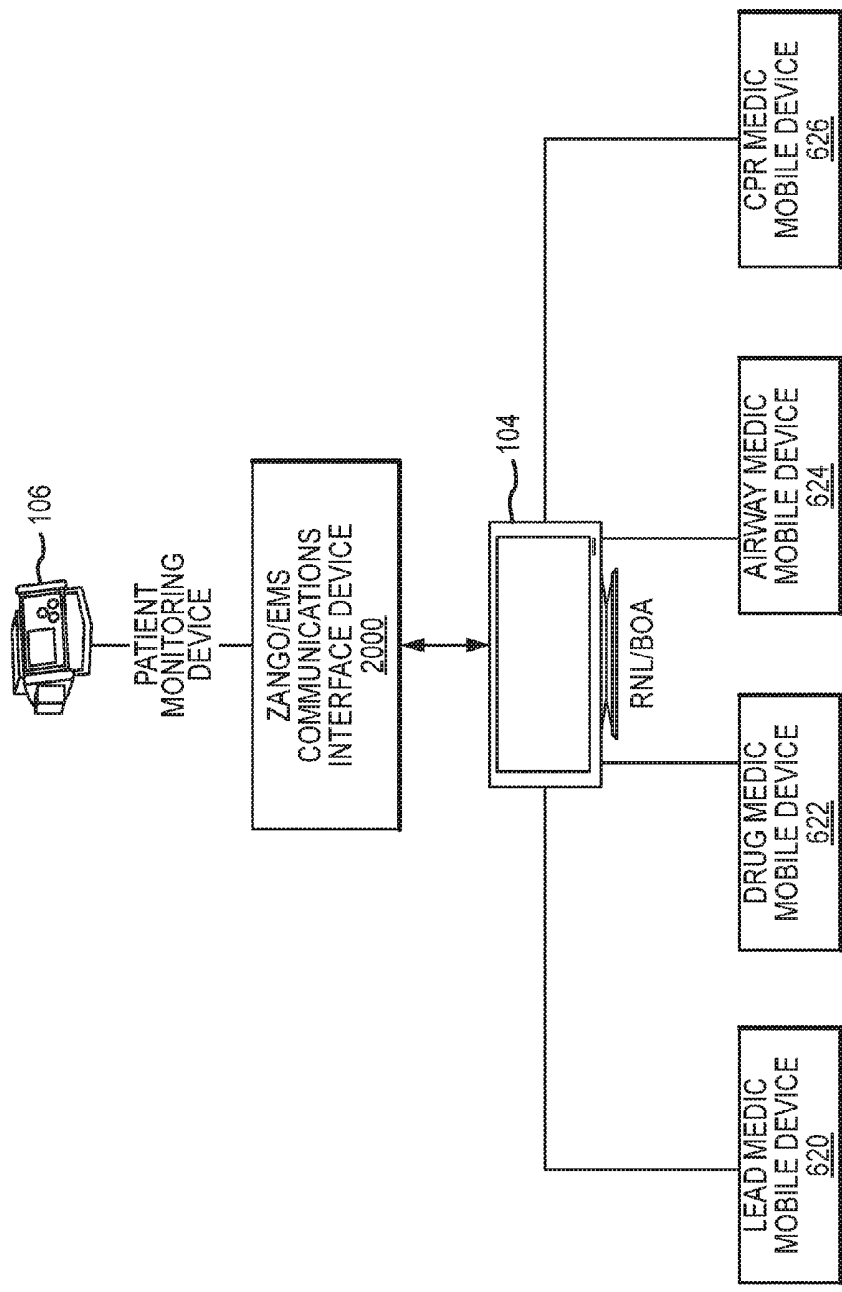


FIG. 62

SYSTEMS AND METHODS FOR EMS DEVICE COMMUNICATIONS INTERFACE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part of U.S. patent application Ser. No. 12/840,129, filed on Jul. 20, 2010, which claims the benefit of U.S. Provisional Patent Application Ser. No. 61/227,187, filed on Jul. 21, 2009, and 61/322,675, filed on Apr. 9, 2010, and this application is also a continuation-in-part of U.S. patent application Ser. No. 12/840,117, filed on Jul. 20, 2010, which claims the benefit of U.S. Provisional Patent Application Ser. No. 61/227,187, filed on Jul. 21, 2009, and 61/322,678, filed Apr. 9, 2010, and all of the five aforementioned patent applications are each incorporated herein by reference in their entireties for all purposes.

TECHNICAL FIELD

[0002] Embodiments of the present invention relate generally to emergency medical services information management, and more particularly to collection, organization, and communication of information gathered from a device used in emergency medical services.

BACKGROUND

[0003] Devices that are used to gather patient monitoring information in emergency medical services (“EMS”) applications, for example defibrillator devices, are often complex and expensive devices, primarily because they serve a very important purpose in an EMS setting, and must be durable, accurate, and reliable. The communications capabilities of such devices are often limited by their hardware, such that users must choose between buying a new defibrillator or continuing to use the same, often slower, communications interfaces available with an older defibrillator. A retrofit solution that involves changing the existing hardware or software of the device may be almost as costly and time-consuming to implement as device replacement itself.

[0004] Existing patient monitoring devices store various kinds of information during use. Users wishing to upload or download such information, typically after an incident or after a certain period of time (e.g. at the end of the day or end of the week), are often limited to retrieving only the entire content of the device’s memory card, regardless of whether the user is interested in only a specific subset of the entire card’s contents. This increases the time necessary for data transfer, as well as the time necessary to sort the data and/or identify the desired subset of the data.

[0005] When an ambulance or other emergency medical services (“EMS”) vehicle is dispatched to a medical emergency, the ambulance driver as well as the EMS technician typically rely on an array of devices in helping them locate, diagnose, treat, transport, chart information about, and deliver the patient. Although such devices typically facilitate particular aspects of the EMS experience, the manual interaction time for each device and the shifting of attention from device to device can in some cases increase transport time and/or shift valuable time away from patient care or can fail to give the crew a complete picture.

[0006] Sending certain data-intensive information from an ambulance to a hospital or other care provider often involves manually faxing or e-mailing such data between telephony

devices. For example, an EMS technician attempting to convey 12-lead data from a defibrillator must often verbally describe her own assessment of the data, or spend the time e-mailing or faxing a snapshot of the 12-lead data to the hospital. This may delay patient care and/or result in the time-consuming transmission of a patient snapshot that may already be several minutes old by the time it reaches the hospital. In fact, transmission of information between an EMS technician in the back of an ambulance and a hospital emergency room (“ER”) nurse often involves a mobile phone “patch” or call during which the EMS technician attempts to verbally convey the patient’s status and treatment, and the vehicle location, while manually sorting through various data sources including the patient’s chart, the defibrillator visual data, and/or the ambulance location data (e.g. looking out the window). This often results in inefficient and sometimes inaccurate communication between the EMS technician and the hospital.

SUMMARY

[0007] A system for supplementing communications capabilities of a patient monitoring device configured to monitor a patient and to make available patient monitoring information according to embodiments of the present invention includes a communications interface slot, the system including a card configured to fit within the communications interface slot and to receive the patient monitoring information from the patient monitoring device via the communications interface slot, a memory device hosted by the card and configured to store the patient monitoring information, a wireless transceiver hosted by the card, an asset management database hosted by the card, and a processor communicably coupled to the wireless transceiver and the asset management database, the processor configured to format the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered, the processor further configured to store the one or more frames to the asset management database and to transmit the stream of one or more frames with the wireless transceiver. In such a system, the processor may be further configured to receive, via the wireless transceiver, a request for frames associated with a specific EMS incident, query the asset management database to retrieve all frames associated with the specific EMS incident, and to transmit the frames associated with the specific EMS incident with the wireless transceiver.

[0008] A method for supplementing communications capabilities of a patient monitoring device configured to monitor a patient and to make available patient monitoring information according to embodiments of the present invention includes receiving the patient monitoring information from the patient monitoring device to an EMS communication interface device via a communications interface slot, storing the patient monitoring information to a memory hosted by the EMS communication interface device, formatting the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered, storing the one or more frames to an asset management database hosted by the EMS communication interface device, and transmitting the stream of one or more frames via a wireless transceiver of the EMS communication interface device.

[0009] According to embodiments of the present invention, a system for supplementing communications capabilities of a patient monitoring device configured to monitor a patient and to make available patient monitoring information, the patient monitoring device having a communications interface slot, the system comprising: a card configured to fit within the communications interface slot and to receive the patient monitoring information from the patient monitoring device via the communications interface slot; a memory device hosted by the card and configured to store the patient monitoring information; a wireless transceiver hosted by the card; an asset management database hosted by the card; and a processor communicably coupled to the wireless transceiver and the asset management database, the processor configured to format the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered, the processor further configured to store the one or more frames to the asset management database and to transmit the stream of one or more frames with the wireless transceiver.

[0010] The system of any of the preceding paragraphs, wherein the processor is further configured to receive, via the wireless transceiver, a request for frames associated with a specific EMS incident, query the asset management database to retrieve all frames associated with the specific EMS incident, and to transmit the frames associated with the specific EMS incident with the wireless transceiver.

[0011] The system of any of the preceding paragraphs, wherein the processor is restricted from editing the patient monitoring information on the memory device.

[0012] The system of any of the preceding paragraphs, wherein the patient monitoring device is configured to edit the patient monitoring information on the memory device.

[0013] The system of any of the preceding paragraphs, wherein patient monitoring information from the patient monitoring device is bifurcated into a first stream and a second stream, wherein the memory card is configured to store the first stream, and wherein the processor is configured to receive the second stream.

[0014] According to embodiments of the present invention, a method for streaming patient information from a clinical device, comprising: establishing a wireless data connection with the clinical device; receiving patient information from the clinical device via the wireless data connection at least once every five seconds; and displaying at least a portion of the patient information in an emergency medical services mobile environment.

[0015] The method of any of the preceding paragraphs, wherein the clinical device is a defibrillator.

[0016] The method of any of the preceding paragraphs, wherein receiving the patient information comprises receiving the patient information from the clinical device via the wireless data connection at least once every second.

[0017] The method of any of the preceding paragraphs, wherein the wireless data connection is a secure WiFi connection.

[0018] The method of any of the preceding paragraphs, wherein the patient information is clinical information, the method further comprising receiving non-clinical information and displaying the clinical information and the non-clinical information simultaneously in the emergency medical services mobile environment.

[0019] The method of any of the preceding paragraphs, wherein the patient information comprises an ECG waveform.

[0020] The method of any of the preceding paragraphs, wherein the patient information comprises a heart rate.

[0021] The method of any of the preceding paragraphs, wherein the patient information comprises an ECG waveform.

[0022] The method of any of the preceding paragraphs, further comprising: receiving full disclosure data from the clinical device; formatting the full disclosure data into a frame event stream, wherein the frame event stream comprises a plurality of frames in chronological order, wherein each of the plurality of frames comprises a time identifier, an incident identifier, and clinical information associated with a time identified by the time identifier and an incident identified by the incident identifier; and sending the frame event stream over the wireless data connection as the patient information.

[0023] The method of any of the preceding paragraphs, further comprising storing the plurality of frames in a computer readable medium.

[0024] The method of any of the preceding paragraphs, further comprising: sending a request over the wireless data connection, the request including a particular incident identifier; retrieving from the computer readable medium and adding to a response set each of the plurality of frames for which the incident identifier corresponds to the particular incident identifier of the request; and sending the response set over the wireless data connection.

[0025] The method of any of the preceding paragraphs, further comprising displaying at least a portion of the response set in the emergency medical services mobile environment.

[0026] The method of any of the preceding paragraphs, wherein the wireless data connection is a first wireless data connection, the method further comprising: transmitting the patient information via a second wireless data connection; receiving the patient information with a personal mobile device via the second wireless data connection; receiving, via the personal mobile device, a role indication; and determining a portion of the patient information for display on the mobile device based on the role indication.

[0027] The method of any of the preceding paragraphs, wherein the role indication is CPR medic, and wherein the portion of the patient information comprises chest compression measurement data.

[0028] The method of any of the preceding paragraphs, further comprising: receiving a patient intervention indication via the second wireless data connection from the personal mobile device; and displaying at least a portion of the patient information simultaneously with information associated with the patient intervention indication in the emergency medical services mobile environment.

[0029] The method of any of the preceding paragraphs, wherein the patient intervention indication is one of a plurality of patient intervention indications, and wherein the plurality of patient intervention indications displayed on the personal mobile device is determined based on the role indication.

[0030] The method of any of the preceding paragraphs, wherein the wireless data connection is a first wireless data connection, the method further comprising: transmitting the patient information via a second wireless data connection;

receiving the patient information with a personal mobile device via the second wireless data connection; receiving, via the personal mobile device, a role indication; and filtering the patient information for display on the mobile device based on the role indication.

[0031] According to embodiments of the present invention, a method for supplementing communications capabilities of a patient monitoring device configured to monitor a patient and to make available patient monitoring information, the patient monitoring device having a communications interface slot, the method comprising: receiving the patient monitoring information from the patient monitoring device to an EMS communication interface device via the communications interface slot; storing the patient monitoring information to a memory hosted by the EMS communication interface device; formatting the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered; storing the one or more frames to an asset management database hosted by the EMS communication interface device; and transmitting the stream of one or more frames via a wireless transceiver of the EMS communication interface device.

[0032] Embodiments of the present invention communicate with and gather relevant data from multiple EMS devices (including but not limited to a defibrillator monitoring a patient, a patient charting device, and a navigation device), organize and store the information, and display it in real-time on a screen in the back of an ambulance and to a hospital, or other location such as a physician's home, via a web browser interface. According to embodiments of the present invention, the display screen in the back of the ambulance is a touch-screen with various organizational options that instantly display different subsets of the EMS information for different uses.

[0033] A system for collecting and displaying emergency medical services information according to embodiments of the present invention includes a defibrillator device configured to monitor a patient, a navigation device, a patient charting device, a database, a display device separate and distinct from the defibrillator device, the navigation device, and the patient charting device, and a processor in communication with the defibrillator, the navigation device, the patient charting device, the database, and the display device. According to embodiments of the present invention, the processor is configured to receive emergency medical services information from the defibrillator device, the navigation device, and the patient charting device, store the emergency medical services information in the database, and display the emergency medical services information on the display device according to an information template.

[0034] According to embodiments of the present invention, a system for collecting and displaying emergency medical services information, the system comprising: a patient monitoring device configured to monitor a patient and to make available patient monitoring information; a patient charting device configured to make available patient charting information, wherein emergency medical services information includes at least some of the patient monitoring information and at least some of the patient charting information; a database; a display device; and a processor communicably coupled to the patient monitoring device, the patient charting device, the database, and the display device, the processor configured to receive the emergency medical

services information, store the emergency medical services information in the database, and display the emergency medical services information on the display device according to an information template.

[0035] The system of any of the preceding paragraphs, wherein the patient monitoring device is a defibrillator.

[0036] The system of any of the preceding paragraphs, wherein the information template is stored in the database.

[0037] The system of any of the preceding paragraphs, wherein the processor is configured to display at least some of the patient charting information and at least some of the patient monitoring information simultaneously on the display device.

[0038] The system of any of the preceding paragraphs, further comprising a navigation device configured to make available navigation information, wherein the processor is communicably coupled to the navigation device, and wherein the emergency medical services information further includes at least some of the navigation information.

[0039] The system of any of the preceding paragraphs, wherein the processor is configured to display at least some of the patient charting information, at least some of the patient monitoring information, and at least some of the navigation information simultaneously on the display device.

[0040] The system of any of the preceding paragraphs, wherein the navigation information is information about location of an emergency medical services vehicle.

[0041] The system of any of the preceding paragraphs, further comprising an emergency services vehicle, wherein the display device is mounted in the emergency services vehicle.

[0042] The system of any of the preceding paragraphs, wherein the emergency services vehicle is an ambulance, and wherein the display device is mounted in a back section of the ambulance.

[0043] The system of any of the preceding paragraphs, wherein the display device includes a touch screen input device for sending instructions to the processor.

[0044] The system of any of the preceding paragraphs, wherein the display device and the processor are part of a tablet PC.

[0045] The system of any of the preceding paragraphs, wherein the display device cycles display between an information template comprising primarily patient monitoring information and an information template comprising primarily patient charting information.

[0046] The system of any of the preceding paragraphs, wherein the display device cycles display between an information template comprising primarily patient monitoring information, an information template comprising primarily patient charting information, and a patch notes information template.

[0047] The system of any of the preceding paragraphs, further comprising: an enterprise server communicably coupled to the processor, the enterprise server configured to receive the emergency medical services information from the processor and send the emergency medical services information to an enterprise environment via a web browser interface.

[0048] The system of any of the preceding paragraphs, wherein the web browser interface is substantially similar to an interface displayed on the display device.

[0049] The system of any of the preceding paragraphs, wherein the database is a mobile database, the system further comprising an enterprise database on a storage medium, wherein the enterprise server is further configured to store at least a portion of the emergency medical services information in the enterprise database.

[0050] According to embodiments of the present invention, a system for collecting and displaying emergency medical services information, the system comprising: a patient monitoring device configured to monitor a patient and to make available patient monitoring information; a navigation device configured to make available navigation information about an emergency medical services vehicle, wherein emergency medical services information includes at least some of the patient monitoring information and at least some of the navigation information; a database; a display device; and a processor communicably coupled to the patient monitoring device, the navigation device, the database, and the display device, the processor configured to receive the emergency medical services information, store the emergency medical services information in the database, and display the emergency medical services information on the display device according to an information template.

[0051] According to embodiments of the present invention, a system for collecting and displaying emergency medical services information, the system comprising: a patient monitoring device configured to monitor a patient in a medical emergency and to make available patient monitoring information; a display device configured for placement in a mobile environment for deployment in the medical emergency; an EMS device that does not monitor the patient but that records or observes information about the medical emergency, the EMS device configured to make available EMS information based on recorded or observed information; and a processor communicably coupled to the patient monitoring device, the EMS device, and the display device, the processor configured to display at least a portion of the patient monitoring information and the EMS information on the display device according to a data model.

[0052] The system of any of the preceding paragraphs, wherein the EMS device is a patient charting device, and wherein the EMS information is patient charting information.

[0053] The system of any of the preceding paragraphs, wherein the EMS device is a navigation device, and wherein the EMS information is navigation information about the mobile environment.

[0054] The system of any of the preceding paragraphs, wherein the patient monitoring device is a defibrillator.

[0055] The system of any of the preceding paragraphs, wherein the EMS device is a first EMS device and the EMS information is a first type of EMS information, the system further comprising: a second EMS device that does not monitor the patient but that records or observes information about the medical emergency, the second EMS device configured to make available a second type of EMS information different from the first type of EMS information, wherein the processor is communicably coupled to the second EMS device, and is configured to display at least a portion of the second type of EMS information on the display device.

[0056] The system of any of the preceding paragraphs, wherein the first EMS device is a patient charting device, wherein the first type of EMS information is patient charting

information, wherein the second EMS device is a navigation device, and wherein the second type of EMS information is navigation information about the mobile environment.

[0057] The system of any of the preceding paragraphs, further comprising: an enterprise server communicably coupled to the processor, the enterprise server configured to receive the EMS information and the patient monitoring information from the processor and send the EMS information and patient monitoring information to an enterprise environment via a web browser interface.

[0058] The system of any of the preceding paragraphs, wherein the enterprise environment is a hospital.

[0059] According to embodiments of the present invention, a system for collecting and displaying emergency medical services information, the system comprising: a clinical device configured to gather clinical data related to a clinical encounter; a non-clinical device configured to gather non-clinical data related to a clinical encounter; wherein emergency medical services information includes at least some of the clinical data and at least some of the non-clinical data; a database; a display device; and a processor communicably coupled to the clinical device, the non-clinical device, the database, and the display device, the processor configured to receive the emergency medical services information, store the emergency medical services information in the database, and display the emergency medical services information on the display device according to an information template.

[0060] The system of any of the preceding paragraphs, wherein the clinical device is a defibrillator.

[0061] The system of any of the preceding paragraphs, wherein processor is further configured to display on the display device a differential diagnosis indication based on the emergency medical services information.

[0062] The system of any of the preceding paragraphs, wherein the information template is stored in the database.

[0063] The system of any of the preceding paragraphs, wherein the processor is configured to display at least some of the clinical data and at least some of the non-clinical data simultaneously on the display device.

[0064] The system of any of the preceding paragraphs, wherein the non-clinical device is a navigation device configured to make available navigation information, and wherein the non-clinical data is the navigation information.

[0065] The system of any of the preceding paragraphs, wherein the non-clinical device is a patient charting device configured to make available patient charting information, and wherein the non-clinical data is the patient charting information.

[0066] The system of any of the preceding paragraphs further comprising an emergency services vehicle, wherein the display device is mounted in the emergency services vehicle.

[0067] The system of any of the preceding paragraphs, wherein the emergency services vehicle is an ambulance, and wherein the display device is mounted in a back section of the ambulance.

[0068] The system of any of the preceding paragraphs, further comprising: an enterprise server communicably coupled to the processor, the enterprise server configured to receive the emergency medical services information from the processor and send the emergency medical services information to an enterprise environment via a web browser interface.

[0069] The system of any of the preceding paragraphs, wherein the web browser interface is substantially similar to an interface displayed on the display device.

[0070] The system of any of the preceding paragraphs, wherein the database is a mobile database, the system further comprising an enterprise database on a storage medium, wherein the enterprise server is further configured to store at least a portion of the emergency medical services information in the enterprise database.

[0071] While multiple embodiments are disclosed, still other embodiments of the present invention will become apparent to those skilled in the art from the following detailed description, which shows and describes illustrative embodiments of the invention. Accordingly, the drawings and detailed description are to be regarded as illustrative in nature and not restrictive.

BRIEF DESCRIPTION OF THE DRAWINGS

[0072] FIG. 1 illustrates a system for mobile and enterprise user real-time display of medical information collected from multiple different EMS devices, according to embodiments of the present invention.

[0073] FIG. 2 illustrates one example of a menu template for the display of a “back of ambulance” (“BOA”) device, according to embodiments of the present invention.

[0074] FIG. 3 illustrates a display and graphical user interface displayed when the user selects the navigation button of the menu template, according to embodiments of the present invention.

[0075] FIG. 4 illustrates a display and graphical user interface displayed when the user selects the patient monitoring button of the menu template, according to embodiments of the present invention.

[0076] FIG. 5 illustrates a display and graphical user interface displayed when the user selects the patient charting button of the menu template, according to embodiments of the present invention.

[0077] FIG. 6 illustrates a display and graphical user interface displayed when the user selects the “patch notes” button of the menu template, according to embodiments of the present invention.

[0078] FIG. 7 illustrates a display and graphical user interface displayed when the user selects the protocols button of the menu template, according to embodiments of the present invention.

[0079] FIG. 8 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient monitoring button, according to embodiments of the present invention.

[0080] FIG. 9 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the navigation button, according to embodiments of the present invention.

[0081] FIG. 10 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient charting button, according to embodiments of the present invention.

[0082] FIG. 11 illustrates a treatment domain system overview for real-time display of medical information collected from multiple different EMS devices, according to embodiments of the present invention.

[0083] FIG. 12 illustrates a device adapter/communication engine and medical device interface, according to embodiments of the present invention.

[0084] FIG. 13 illustrates an exemplary pipe, according to embodiments of the present invention.

[0085] FIG. 14 illustrates a method performed by a pipe of the device adapter that uses discovery supporting transport, according to embodiments of the present invention.

[0086] FIG. 15 illustrates a method performed by a pipe of the device adapter that uses non-discovery supporting transport, according to embodiments of the present invention.

[0087] FIG. 16 illustrates a method performed by a BOA module, according to embodiments of the present invention.

[0088] FIG. 17 illustrates a method performed by a BOA module, according to embodiments of the present invention.

[0089] FIG. 18 illustrates an exemplary computer system, according to embodiments of the present invention.

[0090] FIG. 19 illustrates a system for mobile and enterprise user real-time display of medical information collected from multiple different EMS devices, according to embodiments of the present invention.

[0091] FIG. 20 illustrates a carrier board design for an EMS communication interface device, according to embodiments of the present invention.

[0092] FIG. 21 illustrates a system overview for an EMS communication interface device, according to embodiments of the present invention.

[0093] FIG. 22 illustrates another system overview for an EMS communication interface device, according to embodiments of the present invention.

[0094] FIG. 23 illustrates a software logic diagram for an EMS communication interface device, according to embodiments of the present invention.

[0095] FIG. 24 illustrates a conventional mesh network.

[0096] FIG. 25 illustrates an indoor geolocation system.

[0097] FIG. 26 illustrates an example explanation of differential diagnosis of acute dyspnea in adults.

[0098] FIG. 27 illustrates an example explanation of clues to differential diagnosis of dyspnea.

[0099] FIG. 28 illustrates an example listing of physical exam findings in the diagnosis of acute dyspnea.

[0100] FIG. 29 shows an example treatment protocol for asthma, COPD, and acute decompensated heart failure.

[0101] FIG. 30 illustrates a data transmission interface, according to embodiments of the present invention.

[0102] FIG. 31 illustrates an EMS communication interface transmission processing block diagram, according to embodiments of the present invention.

[0103] FIG. 32 illustrates a EMS communications interface device client architecture, according to embodiments of the present invention.

[0104] FIG. 33 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient monitoring button, according to embodiments of the present invention.

[0105] FIG. 34 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient charting button, according to embodiments of the present invention.

[0106] FIG. 35 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the navigation button, according to embodiments of the present invention.

[0107] FIG. 36 illustrates an alternative enterprise display and graphical user interface shown when the enterprise user selects the navigation button, according to embodiments of the present invention.

[0108] FIG. 37 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patch notes button, according to embodiments of the present invention.

[0109] FIG. 38 illustrates a display and graphical user interface displayed when the user selects the patient charting button of a BOA menu template, according to embodiments of the present invention.

[0110] FIG. 39 illustrates a display and graphical user interface displayed when the user selects the patient monitoring button of a BOA menu template, according to embodiments of the present invention.

[0111] FIG. 40 illustrates a display and graphical user interface displayed when the user selects the navigation button of a BOA menu template, according to embodiments of the present invention.

[0112] FIG. 41 illustrates an alternative display and graphical user interface displayed when the user selects the navigation button of a BOA menu template, according to embodiments of the present invention.

[0113] FIG. 42 illustrates a display and graphical user interface displayed when the user selects the shift start button of a BOA menu template, according to embodiments of the present invention.

[0114] FIG. 43 illustrates an alternative display and graphical user interface displayed when the user selects the navigation button of a BOA menu template, according to embodiments of the present invention.

[0115] FIG. 44 illustrates a display and graphical user interface displayed when the user selects the patch notes button of a BOA menu template, according to embodiments of the present invention.

[0116] FIG. 45 illustrates a display and graphical user interface displayed when the user selects a live patient data button of a BOA menu template, according to embodiments of the present invention.

[0117] FIG. 46 illustrates a start screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0118] FIG. 47 illustrates a role selection screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0119] FIG. 48 illustrates a lead medic quick log screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0120] FIG. 49 illustrates a lead medic ECG graph screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0121] FIG. 50 illustrates a lead medic patient data screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0122] FIG. 51 illustrates a lead medic chief complaint screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0123] FIG. 52 illustrates a drug medic quick log screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0124] FIG. 53 illustrates a drug medic ECG graph screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0125] FIG. 54 illustrates a role selection screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0126] FIG. 55 illustrates an airway medic ECG graph screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0127] FIG. 56 illustrates an airway medic quick log screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0128] FIG. 57 illustrates a CPR medic quick log screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0129] FIG. 58 illustrates a CPR medic ECG graph screen during idle for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0130] FIG. 59 illustrates a CPR medic ECG graph screen during administration of compressions for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0131] FIG. 60 illustrates a CPR medic ECG graph screen during administration of compressions for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0132] FIG. 61 illustrates a CPR medic ECG graph screen during administration of compressions for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention.

[0133] FIG. 62 illustrates a system for role-based data feeds from a BOA device to EMS technician mobile devices, according to embodiments of the present invention.

[0134] While the invention is amenable to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and are described in detail below. The intention, however, is not to limit the invention to the particular embodiments described. On the contrary, the invention is intended to cover all modifications, equivalents, and alternatives falling within the scope of the invention as defined by the appended claims.

DETAILED DESCRIPTION

[0135] As illustrated in FIG. 1, a system 100 according to embodiments of the present invention performs advanced data management, integration and presentation of EMS data from multiple different devices. System 100 includes a mobile environment 101, an enterprise environment 102, and an administration environment 103. Devices within the various environments 101, 102, 103 may be communicably coupled via a network 120, such as, for example, the Internet.

[0136] As used herein, the phrase “communicably coupled” is used in its broadest sense to refer to any coupling whereby information may be passed. Thus, for example, communicably coupled includes electrically coupled by, for example, a wire; optically coupled by, for example, an

optical cable; and/or wirelessly coupled by, for example, a radio frequency or other transmission media. “Communicably coupled” also includes, for example, indirect coupling, such as through a network, or direct coupling.

[0137] The network **120** may also take the form of an ad hoc, self-configuring, self-healing network **2400** such as a MESH network, as illustrated in FIG. **24**, according to embodiments of the present invention. FIG. **24**, as well as the following information about MESH networks in paragraphs [00109] to [00117], is taken directly from Poor, Robert; WIRELESS MESH NETWORKS; Sensors (Feb. 1, 2003), available at <http://www.sensormag.com/networking-communications/standards-protocols/wireless-mesh-networks-968>, which is incorporated herein by reference. Wireless systems for industry conventionally use cellular phone-style radio links, using point-to-point or point-to-multipoint transmission. But research at MIT’s Media Lab in Cambridge, Mass., indicated that traditional wireless formats have limitations in industrial applications. These include rigid structure, meticulous planning requirements, and dropped signals. This can pose an acute challenge in an EMS or mass casualty environment in which existing infrastructure may be either sparse (e.g. a rural environment) or dysfunctional (e.g. a mass casualty or disaster situation).

[0138] In contrast, wireless mesh networks **2400** are multihop systems in which devices assist each other in transmitting packets through the network, especially in adverse conditions. Such ad hoc networks may be implemented with minimal preparation, and they provide a reliable, flexible system that can be extended to thousands of devices, according to embodiments of the present invention.

[0139] The wireless mesh network topology developed at MIT for industrial control and sensing is a point-to-point, or peer-to-peer, system called an ad hoc, multihop network. A node can send and receive messages, and in a mesh network, a node also functions as a router and can relay messages for its neighbors. Through the relaying process, a packet of wireless data will find its way to its destination, passing through intermediate nodes with reliable communication links, as illustrated in FIG. **24**.

[0140] In a wireless mesh network **2400**, multiple nodes cooperate to relay a message to its destination. The mesh topology enhances the overall reliability of the network, which is particularly important when operating in harsh industrial environments. Like the Internet and other peer-to-peer router-based networks, a mesh network offers multiple redundant communications paths throughout the network. If one link fails for any reason (including the introduction of strong RF interference), the network automatically routes messages through alternate paths. In a mesh network **2400**, the distance between nodes can be shortened, which dramatically increases the link quality. Reducing the distance by a factor of two, the resulting signal is at least four times more powerful at the receiver. This makes links more reliable without increasing transmitter power in individual nodes. The reach of a mesh network may be extended, redundancy added, and general reliability improved simply by adding more nodes.

[0141] Network **2400** may be a self-configuring and self-healing network, according to embodiments of the present invention. According to embodiments of the present invention, a network **2400** does not require a system administrator to tell it how to get a message to its destination. A mesh network **2400** is self-organizing and does not require manual

configuration. Because of this, adding new gear or relocating existing gear is as simple as plugging it in and turning it on, according to embodiments of the present invention. The network discovers the new node and automatically incorporates it into the existing system, according to embodiments of the present invention.

[0142] A mesh network **2400** is not only inherently reliable, it is also highly adaptable, according to embodiments of the present invention. For example, if a tank-level sensor and data logger are placed too far apart for a robust RF communications link, one or more repeater nodes may be added to fill the gaps in the network **2400**.

[0143] On the Internet, if one router goes down, messages are sent through an alternate path by other routers. Similarly, if a device or its link in a mesh network fails, messages are sent around it via other devices. Loss of one or more nodes does not necessarily affect the network’s operation. A mesh network is self-healing because human intervention is not necessary for re-routing of messages. Such networks **2400** provide redundancy and scalability, according to embodiments of the present invention.

[0144] In a mesh network, the degree of redundancy is essentially a function of node density. A network can be deliberately over-designed for reliability simply by adding extra nodes, so each device has two or more paths for sending data. This is a simpler way of obtaining redundancy than is possible in most other types of systems. A mesh network is also scalable and can handle hundreds or thousands of nodes. Because the operation of network **2400** does not depend on a central control point, adding multiple data collection points or gateways may be convenient.

[0145] Reliability, adaptability, and scalability are notable attributes of a wireless network for industrial control and sensing applications, according to embodiments of the present invention. Point-to-point networks provide reliability, but they are often challenging to scale to handle more than one pair of end points. Point-to-multipoint networks can handle more end points, but their reliability may depend on placement of the access point and end points. Mesh networks are inherently reliable, adapt easily to environmental or architectural constraints, and can scale to handle thousands of end points.

[0146] According to embodiments of the present invention, the mobile environment **101** is an ambulance or other EMS vehicle—for example a vehicular mobile environment (VME). The mobile environment may also be the local network of data entry devices as well as diagnostic and therapeutic devices established at time of treatment of a patient or patients in the field environment—the “At Scene Patient Mobile Environment” (ASPME). The mobile environment may also be a combination of one or more of VMEs and/or ASPMEs. The mobile environment may include a navigation device **110** used by the driver **112** to track the mobile environment’s position **101**, locate the mobile environment **101** and/or the emergency location, and locate the transport destination, according to embodiments of the present invention. The navigation device **110** may include a Global Positioning System (“GPS”), for example. The navigation device **110** may also be configured to perform calculations about vehicle speed, the travel time between locations, and estimated times of arrival. According to embodiments of the present invention, the navigation device **110** is located at the front of the ambulance to assist the driver **112** in navigating the vehicle. The navigation device

110 may be, for example, a RescueNet® Navigator onboard electronic data communication system available from Zoll Data Systems of Broomfield, Colo.

[0147] FIG. 25, as well as the following information about geolocation in paragraphs [00119] through [00120], is taken directly from K. Pahlavan, et al., “An Overview of Wireless Indoor Geolocation,” Mobile and Wireless Communications Networks IFIP-TC6/European Commission NETWORKING 2000 International Workshop, MWCN 2000 Paris, France, May 16-17, 2000, which is incorporated herein by reference. More generally, the mobile environment may include a geolocation sensor in one or more of the devices in the VME or ASPME. The geolocation sensor may be of a common type such as, for example, a Global Positioning System (GPS). GPS, though, may be subject to certain limitations: 1) line of sight to more than one GPS satellite, which may limit its performance in indoor environments; 2) in some urban environments, location accuracy is reduced due to signal reflections off of buildings; and 3) normal accuracy may be insufficient in the case of a mass casualty in which accuracies of better than ± 5 feet may be required when there are multiple casualties and the locations of each victim needs to be integrated into a software mapping environment, according to embodiments of the present invention.

[0148] Therefore, additional locator base stations may be deployed on-scene outdoors, or within buildings, that may augment or replace the conventional GPS-based geolocator systems, according to embodiments of the present invention. Similar to the cellular geolocation system, the architecture of indoor geolocation systems may fall within one of two main categories: mobile-based architecture and network-based architecture. Most conventional indoor geolocation applications have been focused on network-based system architecture as shown in FIG. 25. The geolocation base stations (GBS) extract location metrics from the radio signals transmitted by the mobile station and relay the information to a geolocation control station (GCS). The connection between GBS and GCS can be either wired or wireless, according to embodiments of the present invention. Then the position of the mobile station may be estimated, in an indoor environment. As a result, dedicated indoor geolocation systems provide accurate indoor geolocation services. This may be applied as well to a mobile environment such as a battlefield or other mass casualty situation in which base stations with better known accuracy based on landmarks or more sophisticated GPS systems such as differential GPS (DGPS) can be deployed to provide highly accurate and complete information about the patient status integrated into the navigation software or other mapping software, such as, for example, Google maps.

[0149] As illustrated in FIG. 1, a patient monitoring device **106** and a patient charting device **108** are also often used for patient care in the mobile environment **101**, according to embodiments of the present invention. The EMS technician **114** attaches the patient monitoring device **106** to the patient **116** to monitor the patient **116**. The patient monitoring device **106** may be, for example, a defibrillator device with electrodes and/or sensors configured for attachment to the patient **116** to monitor heart rate and/or to generate electrocardiographs (“ECG’s”), according to embodiments of the present invention. The patient monitoring device **106** may also include sensors to detect or a processor to derive or calculate other patient conditions. For example, the patient

monitoring device **106** may monitor, detect, treat and/or derive or calculate blood pressure, temperature, respiration rate, blood oxygen level, end-tidal carbon dioxide level, pulmonary function, blood glucose level, and/or weight, according to embodiments of the present invention. The patient monitoring device **106** may be a Zoll E-Series® defibrillator available from Zoll Medical Corporation of Chelmsford, Mass., according to embodiments of the present invention. A patient monitoring device may also be a patient treatment device, or another kind of device that includes patient monitoring and/or patient treatment capabilities, according to embodiments of the present invention.

[0150] The patient charting device **108** is a device used by the EMS technician **114** to generate records and/or notes about the patient’s **116** condition and/or treatments applied to the patient, according to embodiments of the present invention. For example, the patient charting device **108** may be used to note a dosage of medicine given to the patient **116** at a particular time. The patient charting device **108** and/or patient monitoring device **106** may have a clock, which may be synchronized with an external time source such as a network or a satellite to prevent the EMS technician from having to manually enter a time of treatment or observation (or having to attempt to estimate the time of treatment for charting purposes long after the treatment was administered), according to embodiments of the present invention. The patient charting device **108** may also be used to record biographic and/or demographic and/or historical information about a patient, for example the patient’s name, identification number, height, weight, and/or medical history, according to embodiments of the present invention. According to embodiments of the present invention, the patient charting device **108** is a tablet PC, such as for example the TabletPCR component of the RescueNet® ePCR Suite available from Zoll Data Systems of Broomfield, Colo. According to some embodiments of the present invention, the patient charting device **108** is a wristband or smartphone such as an Apple iPhone or iPad with interactive data entry interface such as a touch screen or voice recognition data entry that may be communicably connected to the BOA device **104** and tapped to indicate what was done with the patient **116** and when it was done.

[0151] The navigation device **110**, the charting device **108**, and the monitoring device **106** are each separately very useful to the EMS drivers **112** and technicians **114** before, during, and after the patient transport. A “back of ambulance” (“BOA”) device **104** receives, organizes, stores, and displays data from each device **108**, **110**, **112** to further enhance the usefulness of each device **108**, **110**, **112** and to make it much easier for the EMS technician **114** to perform certain tasks that would normally require the EMS technician **114** to divert visual and manual attention to each device **108**, **110**, **112** separately, according to embodiments of the present invention. In other words, the BOA device centralizes and organizes information that would normally be de-centralized and disorganized, according to embodiments of the present invention.

[0152] Although device **104** is referred to herein as a “back of ambulance” device because the EMS technician **114** would normally benefit the most from having such a display device mounted in the back **152** of an ambulance, one of ordinary skill in the art, based on the disclosure provided herein, will recognize that some or all of the BOA device **104** may be located in any part of a mobile environ-

ment **101**, EMS vehicle, and/or anywhere else useful to an EMS technician **114**. For example, the BOA device **104** may be located in the front **150** of an ambulance, and/or may include components that are portable and can be carried into a patient residence, according to embodiments of the present invention.

[0153] The BOA device **104** is communicably coupled to the patient monitoring device **106**, the patient charting device **108**, and the navigation device **110**, according to embodiments of the present invention. The BOA device **104** is also communicably coupled to a storage medium **118**. The BOA device **104** may be a touch-screen, flat panel PC, and the storage medium **118** may be located within or external to the BOA device **104**, according to embodiments of the present invention. The BOA device **104** may include a display template serving as a graphical user interface, which permits the user (e.g. EMS tech **114**) to select different subsets and/or display modes of the information gathered from and/or sent to devices **106**, **108**, **110**, according to embodiments of the present invention.

[0154] FIG. 2 illustrates one example of a menu template **200** for the display of BOA device **104**, according to embodiments of the present invention. The menu template **200** includes a navigation button **202**, a patient monitoring device button **204**, a patient charting device button **206**, a “patch notes” button **208**, and a protocols button **210**, according to embodiments of the present invention. Pressing one of the buttons takes the user (e.g. EMS tech **114**) to a particular page displaying all or a subset of information from devices **106**, **108**, **110**. FIGS. 3-7 illustrate examples of particular information templates according to which information from the one or more EMS devices **106**, **108**, **110** is displayed, according to embodiments of the present invention. Based on the disclosure provided herein, one of ordinary skill in the art will recognize various other information templates according to which such information may be displayed.

[0155] FIG. 3 illustrates a graphical user interface displayed when the user selects the navigation button **202**, according to embodiments of the present invention. One part of the display includes a status section **302** and another part of the display includes a map section **304**, according to embodiments of the present invention. The status section **302** includes one or more fields identifying information about the EMS vehicle trip, according to embodiments of the present invention. For example, the fields of the status section **302** may include one or more of a Unit field **306** identifying the name of the EMS vehicle for which information is displayed, a Crew unit **308** identifying one or more crew members of the EMS vehicle, a Status unit **310** identifying the status of the trip (e.g. “transporting” or “en route to patient”), an ETA field **312** identifying an estimated time of arrival at the destination, a Destination field **314** identifying the destination of the EMS vehicle (e.g. the hospital), and a Patch Info field **316** identifying a phone number or other information for contacting the EMS vehicle destination (e.g. the hospital), according to embodiments of the present invention.

[0156] The map section **304** may display street information along with the origin, destination, route identification, and/or progress information, according to embodiments of the present invention. The navigation device **110** may also supply vehicle status information for display, which may also be useful when a transport has not yet begun. A user

may select a Cycle Feeds button **318** in order to continuously transition the display between one or more of the various displays of FIGS. 3-7, according to embodiments of the present invention. The information illustrated in FIG. 3 would normally be available only to the driver **112** in the front of the ambulance **101**, but because BOA device **104** is communicably coupled to the navigation device **110**, the BOA device **104** can display all or a selected subset of the information available to the navigation device **110**.

[0157] FIG. 4 illustrates a graphical user interface displayed when the user selects the patient monitoring button **204** of the menu template, according to embodiments of the present invention. FIG. 4 displays information received by the BOA device **104** from a patient monitoring device **106** that is a Zoll E-Series® defibrillator. The display includes a vertical vital signs section **402**, a horizontal vital signs summary section **404**, a graphical section **406**, and interpretation section **414**, according to embodiments of the present invention. The vertical vital signs section **402** includes one or more fields indicating a condition of the patient **116** to which the device **106** is attached. For example, the vital signs section **402** includes a heart rate field, a respiration rate field, a blood pressure field, a blood oxygen level field, and an end-tidal carbon dioxide level field. Each field may include a visual indication of a further subset of information. For example, the heart rate field may include a numerical indication **408** of the heart rate, a time indication **410** reflecting the time that the measurement was taken or derived, and a historical graph **412** indicating generally how the heart rate has increased or decreased since the first measurement or a predetermined time, according to embodiments of the present invention. Other fields may include similar indicators, according to embodiments of the present invention. Vital sign trending may also be displayed.

[0158] A horizontal vital signs summary section **404** indicates, for example, the numerical values represented simultaneously in the vertical vital signs section **402**, according to embodiments of the present invention. The graphical section **406** includes a visual representation of an electrocardiograph, such as that acquired from a twelve-lead sensor placement on the patient **116**, according to embodiments of the present invention. Just above the ECG is an indication of when the ECG was acquired. As new vital signs information and/or new ECG information becomes available, the display of FIG. 4 is automatically refreshed to show the most recent data from the patient monitoring device **106**, according to embodiments of the present invention. The interpretation section **414** includes automatically-generated information from the device **106**, for example, indicating potential causes of the symptoms observed by the device **106**, according to embodiments of the present invention.

[0159] FIG. 5 illustrates a graphical user interface displayed when the user selects the patient charting button **206** of the menu template, according to embodiments of the present invention. The display of FIG. 5 includes a biographical summary **502**, an interventions section **504**, and a vital signs section **506**, according to embodiments of the present invention. The biographical summary **502** may display the patient’s name, age, and gender as recorded by the EMS technician **114** with the patient charting device **108**, according to embodiments of the present invention. The interventions section **504** displays the patient **116** interventions (e.g. treatments administered) recorded with the patient charting device **108**, according to embodiments of the present invention.

ent invention. For example, the interventions section **504** includes a listing of each intervention made, the time of the intervention, a description of the intervention (e.g. name of the drug administered), and the name of the person administering the treatment, according to embodiments of the present invention.

[0160] The vital signs section **506** includes a historical listing of certain vital signs data observed by the EMS technician **114** and recorded in the patient charting device **108**, and stored in the patient charting device **108** and/or the database **118**, according to embodiments of the present invention. The historical listing of vital signs data in the vital signs section **506** includes a time stamp, heart rate, blood pressure, respiration rate, blood oxygen level, end-tidal carbon dioxide level, blood glucose level, Glasgow Coma Scale rating (“GCS”), and the name of the technician or device that observed or recorded the vital sign, according to embodiments of the present invention.

[0161] FIG. 6 illustrates a graphical user interface displayed when the user selects the “patch notes” button **208** of the menu template, according to embodiments of the present invention. Patch notes are notes used by an EMS technician **114** to place a call to a hospital or other treatment facility to confirm that the hospital will accept the patient **116** and/or to provide information about the patient **116** to help the hospital or treatment facility prepare for admission. Because time is typically of the essence for such phone calls (because placing the call can temporarily divert the EMS technician’s **114** attention away from patient **116** care), the EMS technician typically consults and interacts with several different devices **106**, **108**, **110** and/or informal data sources to compile a list of notes to convey to the nurse or other responsible party at the hospital or treatment facility. Such patch notes often take considerable time to assemble, and are often hastily written on a glove, for example, which also results in inaccuracy and in some of the patch notes representing old information by the time the call is placed and the information conveyed to the hospital.

[0162] The BOA device **104**, on the other hand, automatically creates a display of several different fields that would typically comprise patch notes, according to embodiments of the present invention. The display of FIG. 6 includes fields representing information from multiple different devices, such as, for example, devices **106**, **108**, **110**. The patch notes display may organize the information into a predefined template, and/or may organize the information into a customized template associated with a particular EMS technician **114**, according to embodiments of the present invention. Not only does the BOA device **104** automatically receive and display information from multiple different devices **106**, **108**, **110** in a single display summarized to function as patch notes, but it also automatically refreshes the display to reflect the most recent information, thus permitting real-time conveyance of patient information, according to embodiments of the present invention.

[0163] For example, without the BOA device **104**, if a patient’s heart rate rose from **75** to **115** over the course of three minutes, and if an EMS technician **114** wrote “HR **75**” on his glove before consulting his patient chart for name and background information and the driver **112** for location information before calling the hospital three minutes later, the EMS technician **114** might report a heart rate of **75** to the hospital. With the BOA device **104**, however, the patch notes are generated automatically and displayed as in FIG. 6, and

the Defib Vitals section would list the current heart rate of **115** when the EMS technician **114** conveyed the patient status to the hospital.

[0164] In addition to one or more of a Hospital field **602** identifying the name and phone number of the hospital to which the patient **116** is en route and an age field **604** identifying the patient’s age, the display of FIG. 6 may also include one or more of a History Present Illness field, an Interventions field, a Unit identification field (e.g. identifying the particular EMS vehicle), a Gender field, a Past Medical History Field, a patient charting device vital signs field, an Expected Time of Arrival field, a Chief Complaint field, an Assessments field, and a patient monitoring device vital signs field, according to embodiments of the present invention.

[0165] Each of the fields may be configured to display either past or current or derived content from one or more of the EMS devices (e.g. devices **106**, **108**, **110**) which are communicably coupled with the BOA device **104**, according to embodiments of the present invention. For example, the Hospital, Unit, and ETA fields may be based on information received from the navigation unit **110**. The Age, Gender, Chief Complaint, History Present Illness, Past Medical History, and Interventions fields may be based on information received from the patient charting unit **108**. The patient charting device vital signs field may be based on information received from the patient charting unit **108** (e.g. GCS score), and the patient monitoring device vital signs field may be based on information received from the patient monitoring device **106** (e.g. ECG), according to embodiments of the present invention. According to embodiments of the present invention, a BOA device **104** may be located in the front of the ambulance to permit the driver **112** or another EMS technician to place the call to the hospital based on the real-time patch notes, thereby providing the attending EMS technician **114** more time and attention for direct patient care.

[0166] According to embodiments of the present invention, the BOA device **104** receives information from at least one patient monitoring EMS device and at least one non-patient monitoring EMS device. The patch notes screen of FIG. 6 illustrates one example of EMS information (e.g. information related to an emergency medical encounter or transport) from at least one patient monitoring device and at least one other device that does not directly monitor a patient (e.g. a navigation device and/or a patient charting device) on the same display, according to embodiments of the present invention. Similarly, in another embodiment of the present invention, the BOA device **104** receives information from at least one patient clinical device and at least one non-clinical device, and analyzes, combines, stores, displays, and/or transmits the clinical and non-clinical information in a format useful to the user. As used herein, the term “clinical” is used in its broadest sense to refer to that which is directly implicated in monitoring or treatment or diagnosis of a patient. As used herein, the term “non-clinical” is used in its broadest sense to refer to that which is not directly implicated in monitoring or treatment or diagnosis of a patient. For example, a defibrillator is a clinical device, and a navigation device is a non-clinical device. As another example, a patient’s ECG information or heart rate is clinical information, while a patient’s address is non-clinical information.

[0167] FIG. 7 illustrates a graphical user interface displayed when the user selects the protocols button 210 of the menu template, according to embodiments of the present invention. The display of FIG. 7 includes an interactive guidelines manual for the particular locale where the medical emergency occurred, where the treatment occurs, and/or where the patient is delivered, according to embodiments of the present invention. Alternatively, the protocols button 210 may link to a manual or guideline document for the use of a particular device and/or the administration of a particular technique and/or information about a drug. For example, the display of FIG. 7 may include an interactive page listing of chapters in a county's protocol index, which may be a locally-stored protocol index and/or a protocol index accessed through an Internet connection. Clicking on one or more of the chapters or links opens a page containing more detail about the particular chapter or subject selected, for example.

[0168] Based on the disclosure provided herein, one of ordinary skill in the art will appreciate that the BOA device 104 may be configured to display additional or different subsets of information from one or more EMS devices and/or external data sources. According to embodiments of the present invention, the BOA device 104 not only seamlessly integrates information from a patient monitoring device 106, a patient charting device 108, and a navigation device 110 for display in mobile environment 101, but it also does so for display in a remote environment such as, for example, enterprise environment 102. Enterprise environment 102 may be a hospital and/or dispatch environment, for example.

[0169] Data from the BOA device 104 (and therefore data from the devices 106, 108, 110 communicably coupled with the BOA device 104) may be received by one or more enterprise storage servers 126 in an administration environment 103 and stored in an enterprise database 130, and the same information may be accessed and provided by one or more enterprise application servers 128 to a workstation 122 of an enterprise user 124, according to embodiments of the present invention. According to embodiments of the present invention, the BOA device 104 is communicably coupled to the storage server 126 which is communicably coupled to the database 130, and the application server 128 is communicably coupled to the database and to the enterprise workstation 122. Such devices may be communicably coupled via a network 120 such as, for example, the Internet.

[0170] When the BOA device 104 receives updated information from one or more of the devices (e.g. devices 106, 108, 110) to which it is communicably coupled, the BOA device 104 sends the updated information to the enterprise storage server 126, which stores the updated information in a database which may be contained on a storage medium 130, according to embodiments of the present invention. Hence, information from one or more devices (e.g. devices 106, 108, 110) may be stored in mobile database 118, remote enterprise database 130, or both, according to embodiments of the present invention. An enterprise user 124, who may be an emergency room nurse monitoring and/or preparing for ambulance arrivals, an emergency room physician, and/or a medical director at home, for example, may access information similar to information displayed by the BOA device 104 by requesting the information via an enterprise workstation 122. For example, the enterprise workstation 122 accesses a web interface and/or thin client web browser

application which requests the information over the network 120 from application server 128. Application server 128 queries the database 130 for the information, and returns a display to enterprise workstation 122 that looks the same as or similar to what the EMS technician 114 is currently seeing on the BOA device 104 display, according to embodiments of the present invention.

[0171] FIGS. 8-10 illustrate examples of user interface and display screens available to the enterprise user 124 via the enterprise workstation 122, according to embodiments of the present invention. FIG. 8 illustrates a web browser based client interface including, in one portion of the display, a list of available EMS vehicles 802, 804 for which EMS device data is available, according to embodiments of the present invention. Clicking on ALS2 804, for example, brings up a screen similar to FIG. 8 which allows the enterprise user 124 to select one of the buttons, including but not limited to the patient monitoring button 806, the navigation button 808, and/or the patient charting button 810. When user 124 clicks on the patient monitoring button 806, the screen display of FIG. 8 is presented and includes current information from the patient monitoring device 106 of ambulance ALS2, according to embodiments of the present invention. According to embodiments of the present invention, the patient monitoring display of FIG. 8 is automatically updated continuously or semi-continuously; according to other embodiments of the present invention, the user 124 selects "get updates" or the browser's "refresh" button in order to obtain the most current information available. The enterprise display of FIG. 8 contains information similar to the mobile display of FIG. 4, according to embodiments of the present invention.

[0172] According to embodiments of the present invention, the website display in the enterprise environment 102 is accessed via a generic internet browser by a doctor waiting in the emergency room for the patient to arrive by ambulance. The website may be secured by logon username and password, for example. Each ambulance may be identified by a vehicle name; the doctor chooses from a list of incoming vehicle, after which the data for that patient is displayed. The data may be shown just as it appears on the mobile screen, also in "clinical time." According to embodiments of the present invention, the enterprise environment 102 website displays data only for those patients whose destination is the same as the destination logged on the user's facility.

[0173] When the user 124 clicks on the navigator button 808, the screen display of FIG. 9 is presented and includes current information from the navigation device 110 of ambulance ALS2, according to embodiments of the present invention. The enterprise display of FIG. 9 contains information similar to the mobile display of FIG. 3, according to embodiments of the present invention.

[0174] When the user 124 clicks on the patient charting button 810, the screen display of FIG. 10 is presented and includes current information from the patient charting device 108 of ambulance ALS2, according to embodiments of the present invention. The enterprise display of FIG. 10 contains information similar to the mobile display of FIG. 5, according to embodiments of the present invention.

[0175] Although FIG. 1 depicts a single BOA device 104 in the mobile environment 101, more than one BOA device 104 may be used in the mobile environment 101 to communicably connect to the same or a different set of devices

106, 108, 110. And although FIG. 1 depicts one mobile environment **101**, more than one mobile environment **101** and/or more than one BOA device **104** may be communicably coupled with the administration environment **103** and/or the enterprise storage server **126**, according to embodiments of the present invention. According to embodiments of the present invention, the enterprise storage server **126** receives EMS device information from BOA device **104** and stores it in database **130** along with an authenticated time stamp and an identifier associating the information with a particular EMS device and/or a particular EMS vehicle. In this way, data from multiple vehicles and/or multiple devices may be accessed by the enterprise user **124**.

[0176] Also, the enterprise storage server **130** may securely store the information received from one or more BOA devices **104** for longer periods of time to permit later use of the information. For example, the BOA device **104** may receive patient-identifying information such as name, address, and/or social security number via the patient charting device **108** or directly through the BOA device **104**, and then may convey some or all of the patient-identifying information to enterprise storage server **126** with a request for the enterprise storage server **126** to query the database **130** for past records involving the same patient **116**. The enterprise storage server **126** may then forward any such records or portions of such records back to the BOA device **104** (e.g. for display in the patient charting screen or the Past Medical History in the patch notes screen) to assist the EMS technician **114** with the current emergency. Similarly, such past EMS encounter record information may also be accessed by the enterprise user **124**, according to embodiments of the present invention. A system administrator **134** may access and/or monitor the data in database **130** and/or modify the instructions of the servers **126, 128** via administration workstation **132**, which may be communicably coupled to the servers **126, 128**, according to embodiments of the present invention.

[0177] According to some embodiments of the present invention, the BOA device **104** may connect with (e.g. automatically or manually or selectively) a wearable medical device, such as, for example, a Lifevest® wearable defibrillator, to receive and display patient monitoring information therefrom. The BOA device **104** may also be configured to receive patient-identifying information from such a wearable device, to permit the BOA device **104** to query an external database, for example across network **120**, to retrieve additional information about the patient. The BOA device **104** may also be configured to connect with an implantable cardioverter-defibrillator (“ICD”) in a similar fashion, according to embodiments of the present invention.

[0178] FIG. 11 illustrates a treatment domain system **1100** overview for real-time display of medical information collected from multiple different EMS devices, according to embodiments of the present invention. System **1100** includes a patient monitoring device module **1102** communicably coupled with mobile domain modules **126** communicably coupled with remote or enterprise domain modules **1128** communicably coupled with a thin client display module **1124**, according to embodiments of the present invention. According to embodiments of the present invention, the database **130** may be accessed by multiple hospitals throughout a region, state, country, and/or the world.

[0179] The mobile domain modules **1126** includes the device adapter **1104**, a mobile asset management module

1106 which may access a mobile database **1108**, a BOA module **1110**, a patient charting module **1112**, a navigation module **1114**, and a network adapter **1116**, according to embodiments of the present invention. The remote/enterprise modules **1128** include the network adapter **1116**, an enterprise asset management module **1118** which may access an enterprise database **1120**, and an enterprise application server module **1122**, according to embodiments of the present invention.

[0180] The patient monitoring device module **1102** operates the patient monitoring device **106** and generates one or more data pipes containing information about a patient **116** condition. The device adapter communication interface module **1104** manages data communications between a computing device and one or more medical devices such as, for example, between the patient monitoring device module **1102** and the mobile asset management module **1106** and/or BOA module **1110**. The device adapter module **1104** includes one or more of the following attributes, according to embodiments of the present invention:

[0181] Supports multiple communications transports (e.g., devices can use Bluetooth, 802.11, Ethernet, Serial cable).

[0182] Supports multiple data transfer protocols.

[0183] Supports multiple medical device types.

[0184] Supports multiple data storage profiles (e.g., storage to file system, storage by asset management module **1106** to database **1108**).

[0185] Allows administrator or user to associate transport, protocol, device and multiple storage profiles together to represent a communication “pipe” over which data can be exchanged with medical devices.

[0186] Supports multiple pipes at the same time.

[0187] Allows administrators or users to specify one or more specific medical devices to which it communicates in which case the module **1104** will use transport specific discovery protocols to find and attach to the devices.

[0188] Allows administrators or users to specify ANY as a medical device in which case it will use transport specific discovery protocols to find and attach to any compatible medical device found.

[0189] When a pipe is configured to use a protocol which does not support discovery (e.g. serial cable), module **1104** will allow the device to initiate the connection and then allow or deny it based on whether the specific medical device is selected or not.

[0190] Supports multiple client applications (local or remote) by allowing them to connect to module **1104** and receive asynchronous notification of data arrival from medical devices and a means to retrieve the data.

[0191] Maintains a communications ‘pipe’ should the medical device have a data asset to communicate, regardless of whether any application is running or ready to receive the data asset.

[0192] A user may configure the medical device(s) applications communicate with, and such configuration may be persistent and easily changed.

[0193] Communications policies may be configurable. For instance, Bluetooth may require pairing with a device before communications occur. A user may configure whether the pairing is ‘automatic’ or ‘manual’ or ‘continuously reacquired’, for example.

[0194] Applications may access previously received data assets via a relatively simple, expressive API.

[0195] Applications may be notified of newly received assets and may filter those notifications based on specific devices and/or asset type.

[0196] Applications may query the communications layer for status, available devices, and the like, for customizable user interface elements.

[0197] The communications layer may be controllable from a notification icon which also indicates status.

[0198] Configurable items may be protected from malicious or erroneous alteration by common users through the use of a privileged 'admin' mode and a common user mode in the notification area icon applet.

[0199] Configuration may be 'portable' and 'distributable,' such that one configuration may be created and copied to each device rather than having to actually configure each device through a notification applet.

[0200] Particular features or limitations of the communications 'pipe' may be hidden from the application by default.

[0201] The communications layer may itself be layered and support multiple plug-in style transport drivers for managing different communications transports and multiple plug-in style protocol drivers for handling the receipt of data assets from different devices and different asset types. This may allow for the rapid extension of the communications layer to new transports or to new protocols as they are developed.

[0202] FIG. 12 illustrates a diagram of the device adapter communication module 1104, which includes one or more pipes 1202, 1204, 1206 each associated with a medical device 1208, 1210, 1212. The communication module 1104 may be a PELICAN™ communication interface available from Zoll Data Systems of Broomfield, Colo., according to embodiments of the present invention. According to embodiments of the present invention, the communication engine 1104 is an "always on" operating system service which implements the communications pipes 1202, 1204, 1206 and handles the incoming data from medical devices 1208, 1210, 1212. Communication engine 1104 also includes an API 1216, which is a collection of objects and methods exposed by the communications engine 1104 which can be used by an application to configure and interact with the engine 1104 for tasks like getting data assets and configuring the engine 1104, according to embodiments of the present invention. For example, the mobile asset management module 1106 may interact with the API 1216 to receive medical device data.

[0203] FIG. 13 illustrates a diagram of pipe 1202, according to embodiments of the present invention. Pipe 1202 includes one or more storage plug-ins 1302, 1304, 1306 associated with one or more storage configurations 1312, 1314, 1316 of the medical device; a medical device plug-in 1308 associated with a medical device configuration 1318 of the medical device, and a transport plug-in 1310 associated with a transport configuration 1320 of the medical device, according to embodiments of the present invention. As used herein, a "transport" is an operating system supported underlying communications medium, for example TCP/IP, Bluetooth, and Serial. Some transports are packet oriented (e.g. TCP) while others are stream oriented (e.g. Serial). Some support discovery, some do not. Some support pairing, some do not. Each transport may include unique configurations.

[0204] A transport plug-in may be a .NET assembly that is dynamically loaded by the communications engine 1104 and which provides data communications support for a specific transport (e.g. Serial Port, Bluetooth, TCP/IP, and File System). The communications engine 1104 may be configured for auto-pairing (e.g. for transports that support pairing, the engine 1104 uses rules specific to the transport to automatically create and maintain pairings with medical devices depending on configuration and user preference) and/or for auto-discovery (e.g. for transports that support discovery, the engine 1104 may be configured to automatically find new medical devices and enter them into the known device list), according to embodiments of the present invention.

[0205] A medical device plug-in may be a .NET assembly that is dynamically loaded by the communications engine 1104 which provides transport independent data communications services for a particular type of medical device, for example ZOLL M/E-Series ZOLLModem or ZOLL E-Series DUN. A storage plug-in may be a .NET assembly that is dynamically loaded by the communications engine 1104 which provides storage services to the engine.

[0206] As shown in FIG. 13, a pipe may be a combination of transport, medical device, and storage configurations which represent a medical device from which the user has indicated data will be received, and which allows communications to occur. Pipes may be configured by the user and/or may be predefined. For example, a pipe may specify Transport Serial Port with configuration (COM1, Baud=9600), Medical Device E/M Series ZOLLModem (Any Medical Device) and Storage (Local File System). This configuration would accept data assets from any device connected to COM1 at 9600 baud and store them to the local file system. As another example, a pipe may specify Transport Bluetooth (Baud=115200, Auto-Pair), Medical Device E/M Series ZollModem (ZOLL005611), Storage (Local File System) and Storage (Asset Management). This configuration would cause Bluetooth to pair to ZOLL005611, maintain that pairing even when broken and accept any data assets from that specific device and store them both to the local file system and submit them to Asset Management (e.g. mobile asset management module 1106 and/or enterprise asset management module 1118).

[0207] As yet another example, a pipe may specify Transport Bluetooth (Baud=115200, Auto-Pair), Medical Device E/M Series ZOLLModem (Any Device). This configuration would cause Bluetooth to automatically pair with any medical device found during periodic discovery and accept any data assets from any paired device and store them via all loaded and enabled storage plug-ins. As yet another example, a pipe may specify Transport TCP/IP (LocalIP=192.168.1.20, Port=7743), Medical Device E/M Series DUN (Any Device), Storage (Asset Management). This configuration would cause the engine 1104 to start listening on the specified IP address and port for DUN traffic and store it via Asset Management (e.g. by sending it to mobile asset management module 1106 and/or enterprise asset management module 1118), according to embodiments of the present invention.

[0208] For each "pipe" of device adapter 1104 that uses Discovery Supporting Transport, the adapter 1104 performs the method outlined in FIG. 14, and for each pipe of device adapter 1104 that uses Non-Discovery Supporting Transport,

the adapter **1104** performs the method illustrated in FIG. **15**, according to embodiments of the present invention.

[0209] As described above, the mobile asset management module **1106** receives medical device data from the device adapter and communications interface **1104**, according to embodiments of the present invention. The mobile asset management module **1106** performs the secure storage, retrieval and management of medical device data together with asynchronous events informing other applications of the storage or modification of these data assets. The mobile asset management module **1106** supports local or remote service oriented API to store, retrieve and modify medical device data, and provides local or remote asynchronous message-based notification of events to applications which subscribe for them, according to embodiments of the present invention. These events may include notification of the arrival of medical device data.

[0210] The BOA module manages data feeds from multiple data providers (including but not limited to, the device adapter **1104**, the patient charting module **1112**, and the navigation module **1114**) and presents these feeds on a touch-screen flat panel, according to embodiments of the present invention. The BOA module **1110** also communicates these aggregated data elements to a back-office module (e.g. the enterprise asset management module **1118**). The patient charting module **1112** controls the patient charting device **108** and the information sent and received by it, and the navigation module **1114** controls the navigation device **110** and the information sent and received by it, according to embodiments of the present invention. The BOA module **1110** includes one or more of the following attributes, according to embodiments of the present invention:

[0211] Allows the user to configure the device adapter/communication interface module **1104**, including but not limited to selection of a medical device.

[0212] Allows the user to select a patient charting device from which it will receive a data feed containing medical record information as it is entered in patient charting device.

[0213] Allows the user to select a navigation device from which it will receive a data feed containing navigational and dispatch information on a periodic basis.

[0214] Receives notification from the communication interface module **1104** and/or the mobile asset management module **1106** about the arrival of new medical device data including but not limited to 12-lead ECG and vital trend records.

[0215] Receives asynchronous messages from a selected patient charting device which contain data about the currently open patient record including but not limited to: patient demographics, medical history, current assessments, interventions performed and/or vital signs.

[0216] Receives asynchronous messages from a selected navigation device which contains data about the current dispatch state, destination, crew, location, route and/or map of current position.

[0217] Cyclically presents a graphic display of each of the received data feeds for viewing in the back of the ambulance on the flat panel, or elsewhere on another display device.

[0218] Allows the caregiver or EMS technician **114** to temporarily freeze the cycling display on a feed for

more careful examination of that particular data in that particular information template.

[0219] Aggregates the data feeds into a data construct which is sent periodically to the enterprise asset management module **1118**.

[0220] Presents a customer customizable view of the aggregated data feed for the purpose of facilitating a verbal report to the receiving facility (e.g. a report in the Patch Notes information template displayed on the BOA device **104**).

[0221] Presents the user with the ability to view the regional EMS protocols for reference.

[0222] FIG. **16** illustrates a logic flow chart **1600** executed by the BOA module **1110**, according to embodiments of the present invention. The logic flow chart **1600** starts at block **1602**. A user selects particular devices or selects a “read from” configuration to determine which devices’ data will be read and displayed by the BOA device **104** (block **1604**). A data model is prepared (block **1606**), for example the current state of the system that will be displayed on the BOA device **104** and which may eventually be communicated to the enterprise environment **102** and/or enterprise application server **128**. The data model may expand to contain other data elements as feeds are added, and may contract to eliminate container properties for unused data feeds (e.g. installations that do not include a patient charting device **108**), according to embodiments of the present invention. The BOA module **1110** queries the mobile asset management module **1106** to determine whether new medical device data is available (block **1608**) and, if so, updates the medical device data in the data model (block **1610**). The BOA module **1110** queries the mobile asset management module **1106** to determine whether new patient charting data is available (block **1612**) and, if so, updates the patient charting data in the data model (block **1614**).

[0223] The BOA module **1110** queries the mobile asset management module **1106** to determine whether new navigation data is available (block **1616**) and, if so, updates the navigation data in the data model (block **1618**). The BOA module **1110** determines whether it is time to send updated information to the enterprise asset management module **1118** (block **1620**) and, if so, sends the data model to the enterprise asset management module (block **1622**) and generates an asynchronous message (block **1626**). According to embodiments of the present invention, the asynchronous message generated at block **1626** is destined for the enterprise application server **128**; according to alternative embodiments of the present invention, the asynchronous message generated at block **1626** is destined for the enterprise storage server **126** which, in turn, stores the data and notifies the enterprise application server **128** of the data’s availability. The data model is then rendered (block **1624**), for example in the form of a display update on the BOA device **104**, according to embodiments of the present invention. According to embodiments of the present invention, the procedures indicated by blocks **1608**, **1612**, **1616**, and **1620** are not executed as “stages” but are instead each events which trigger a different thread of execution that modifies a data model, which in turn triggers the update of the BOA device **104** display.

[0224] The network adapter/communication interface module **1116** is a communications channel that includes one or more of the following attributes, according to embodiments of the present invention:

- [0225] General purpose and data format independent. Each application may be responsible for the format of its messages.
- [0226] Message addressing may be by name rather than transport address (IP address for instance) so that messages can be sent to entities for which no route currently exists (e.g. when the sender is disconnected from the Internet). Name resolution into actual machine address may be deferred until a route actually exists.
- [0227] Tree relationship between entities that use communication interface module 1116, in which name information may be “percolated” up the tree but not down. As such, each node has a simple routing choice: if the name is the current device or below, route there, otherwise route to the current device’s parent. The root of the tree may be the primary message broker and it accumulates all name information. The primary message broker is the unique node in the communications tree which contains all name information and thus can perform routing from one sub-tree to another, according to embodiments of the present invention.
- [0228] Message delivery may be deferred until the recipient actually appears. Messages may be stored until the recipient becomes routable.
- [0229] Messages may be stored in a transaction safe database at each node so that even a node unexpectedly failing does not risk message loss.
- [0230] Full encryption of messages may be maintained until the recipient actually receives them. While stored in databases, the messages may remain encrypted.
- [0231] Robust operation over intermittently connected wireless connections. Messages may be stored until a connection is resumed. Within certain time-limits, if the connection is restored, message transmission may continue from where it left off rather than starting anew.
- [0232] Messages intended for machines or applications that are ‘local’ may be routed locally even when that segment of the tree is disconnected from the primary message broker.
- [0233] Messages may be sent with an expiration time after which the message will not be delivered and the sender may be notified of the expiration.
- [0234] The communications interface 1116 may be a MERCURY™ communication interface available from Zoll Data Systems of Broomfield, Colo., according to embodiments of the present invention.
- [0235] The messaging components for the BOA module 1110 may be implemented using the communication interface module 1116 as a channel. These messaging components implement one or more of the following characteristics, according to embodiments of the present invention:
- [0236] Publish-Subscribe Model: The data feed consumers (e.g. the BOA mobile module 1110) subscribe with the providers (e.g. the patient charting module 1112) to receive the data feed. The subscription request includes the duration of the subscription. As the providers modify the data feed items, the data feed items are sent to all subscribers. According to embodiments, the BOA module 1110 is a data feed consumer for feeds from the patient charting module 1112 and the navigation module 1114 but a data feed provider for the aggregated feed going to the enterprise asset management module 1118.
- [0237] Message Queue Throttling: Using the message expiration feature of the communications interface module 1116, all messages may be sent with a short expiration time and then a new, current copy is sent upon expiration notification. This keeps the system from having a large queue of stale data feed messages when components are disconnected; at most, one current message is in the system.
- [0238] Complex message format: The data feed messages include graphical, textual and binary data which may be turned into objects by the recipient for ease of use.
- [0239] The enterprise asset management module 1118 receives an aggregated data feed from multiple BOA modules 1110 and provides presentation of those aggregated data feeds on displays remote from the originating ones. For example, such aggregated data feeds may be fetched from the database 1120 associated with the enterprise asset management module 1118 by the enterprise application server module 1122 and displayed to an enterprise user via a thin client display application module 1124 running on a web browser, according to embodiments of the present invention. Such a web page may be secured, encrypted, password-protected, and/or HIPAA compliant, according to embodiments of the present invention. The enterprise asset management module 1118 includes one or more of the following attributes, according to embodiments of the present invention:
- [0240] Receives asynchronous messages from multiple BOA modules 1110 containing aggregated data feeds including but not limited to data feeds from patient charting modules 1112, navigation modules 1114, and medical devices.
- [0241] Uses destination data from the BOA module 1110, set either by the navigation module 1114 or manually by the user on the flat panel BOA device 104, creates a web page for each hospital destination containing the feeds from each BOA module 1110 with that hospital as the destination.
- [0242] Asynchronously updates the web page as new versions of the aggregated data feeds arrive for each BOA module 1110 sending data regarding a patient 116 en route to the hospital or treatment facility.
- [0243] Renders the aggregated data feeds with diagnostic resolution of the 12-Lead data.
- [0244] Prevents unauthorized access by employing hospital specific logins to the secured EMS data feed web page module 1124.
- [0245] Although FIG. 1 illustrates the BOA device 104 communicably coupled with a patient monitoring device 106, a patient charting device 108, and a navigation device 110, in alternative embodiments of the present invention the BOA device 104 is communicably coupled with additional EMS-related devices not shown in FIG. 1, and/or is communicably coupled with multiple devices of the kind shown in FIG. 1, and/or is communicably coupled with different models or versions of the devices of the kind shown in FIG. 1. For example, the BOA module 1110 may be configured to communicate EMS-related device data to and from, either directly and/or indirectly via a device adapter/communication interface module 1104, one or more of the following devices: a defibrillator, a patient charting device, a navigation device, a GPS device, a pulse oximeter, an automatic cardiopulmonary resuscitation device (e.g. Autopulse® non-

invasive cardiac support pump), a driver safety monitoring system, a standalone blood pressure monitor, a blood glucose measurement device, an inventory control system, a blood alcohol monitor, a breathalyzer instrument, and a crew scheduling system. A defibrillator or patient monitoring device may be one of a broad range of defibrillators or patient monitoring devices made and/or sold by a number of different manufacturers, according to embodiments of the present invention. The BOA device 104 may also be communicably coupled with, and configured to aggregate with patient data, data obtained from a CodeNet Writer™ device manufactured by Zoll Medical Corporation, or the like, according to embodiments of the present invention.

[0246] According to embodiments of the present invention, the BOA device 104 is communicably coupled to only one or two of the patient monitoring device 106, the patient charting device 108, and the navigation device 110, and is configured to organize and display EMS information from only the one or two such devices.

[0247] Although the modules and applications described with respect to FIG. 11 can roughly correspond to the hardware devices with similar designations in FIG. 1, one of ordinary skill in the art, based on the disclosure provided herein, will understand that the various modules and/or instructions for performing the described procedures may be located on different and various hardware devices and/or on hardware devices not depicted, in different combinations, according to embodiments of the present invention. For example, although the BOA device 104 may be a touch-screen PC including and configured to perform the tasks of the BOA module 1110, the BOA device 104 may alternatively be a simple display device such as a monitor, with the computational functions of the BOA module 1110 and/or mobile asset management module 1106 performed by other hardware, such that only the display information is communicated to the BOA device 104, according to embodiments of the present invention.

[0248] The BOA device 104 according to embodiments of the present invention may be configured to facilitate data entry via a touch screen device with software that permits rapid and easy data entry, similar to the Quicklog capability of the Zoll Data Systems RescueNet® ePCR Suite. In addition, the BOA device 104 may be configured to permit selection and display of patient monitoring data (e.g. 12-lead ECG data) from prior transports and/or other agencies retrieved from mobile database 118 and/or enterprise database 130, according to embodiments of the present invention. Such historical and/or shared patient data may also be made available to hospitals, and/or stored by hospitals or other care institutions as part of a data management program. The BOA device 104 may also be configured to display streaming ECG information similar to the “live” display of such information by a defibrillator device, for example. The BOA device 104 may also be configured to display feedback to the EMS technician 114 about cardiopulmonary resuscitation being performed, to evaluate the CPR technique during and/or after it is administered. According to embodiments of the present invention, the BOA device 104 may be configured to communicably couple with and receive information from an accelerometer and/or other CPR evaluation device, such as a device configured to detect the presence of and/or the timing of and/or the depth/displacement of and/or the velocity of and/or the acceleration of chest compressions, for example

the devices and methods described or referenced in U.S. Pat. No. 6,390,996 issued on May 21, 2002, U.S. Pat. No. 6,827,695 issued on Dec. 7, 2004, U.S. Pat. No. 7,122,014 issued on Oct. 17, 2006, and U.S. Pat. App. Pub. No. 2006/0009809 published on Jan. 12, 2006, which are incorporated by reference herein in their entireties.

[0249] FIG. 17 depicts a flow chart 1700 illustrating a method performed by BOA module 1110, according to embodiments of the present invention. The process begins at block 1701. The BOA module 1110 is initialized (block 1702), and the user may then select devices (block 1704) from which medical and/or EMS information will be received. For example, such device selection may involve generating an asynchronous message to be received by the patient monitoring module 1102 for establishing a connection (block 1706), an asynchronous message to be received by the navigation module 1114 for establishing a connection (block 1708), and/or an asynchronous message to be received by the patient charting module 1112 for establishing a connection (block 1710). A different subset of devices (different devices, fewer devices, or more devices) may be selected at any time when the user initiates an asynchronous event to select or change devices (block 1712).

[0250] Once devices have been selected, the BOA device 104 cycles through a series of different displays (block 1714). This cycling may be programmed to occur at preset intervals; for example, the BOA device 104 may be configured to cycle the display between different data models every seven seconds. For example, a navigation device data model may be displayed (block 1716), which may be similar to the data model depicted in FIG. 3, for example. After a preset time, the display may be switched to a patient monitoring device data model (block 1718), similar to the data model depicted in FIG. 4, for example. After another preset time, the display may be switched to a patient charting device data model (block 1720), similar to the data model depicted in FIG. 5, for example. Once the display has cycled through each data model, it may return to the first data model displayed and repeat the cycle, according to embodiments of the present invention. Such a cycling may be initiated or re-initiated during other tasks when the user initiates an asynchronous event (block 1722) by selecting the cycle feed button (similar to the button 318 of FIG. 3), for example.

[0251] When a user selects one of the “feed” buttons (block 1724), an asynchronous event is generated causing the data model corresponding to that feed to be displayed (block 1726) for a longer predetermined period of time, for example one minute. As an example, if the user selects the patient charting button 206 (see FIG. 2), the patient charting data model similar to FIG. 5 will immediately be displayed and will remain displayed for a period of time longer than the default cycle time. When a user selects the patch notes button 208 (block 1728), an asynchronous event is generated causing the patch notes data model similar to FIG. 6 to be displayed (block 1730) until the user next selects the cycle feeds button 318 or a particular feed button 202, 204, 206, according to embodiments of the present invention. When a user selects the protocols button (block 1732), an asynchronous event is generated causing the protocols data model similar to FIG. 7 to be displayed (block 1734) until the user next selects the cycle feeds button 318 or a particular feed button 202, 204, 206, according to embodiments of the present invention.

[0252] When one of the EMS devices receives or generates new data, it may be configured to generate an asynchronous notification to be received by the BOA module 1110, according to embodiments of the present invention. For example, the patient charting module 1112 may generate an asynchronous message when it has new information to share (block 1736), the patient monitoring module 1102 may generate an asynchronous message when it has new information to share (block 1738), and the navigation module 1114 may generate an asynchronous message when it has new information to share (block 1740), according to embodiments of the present invention. These asynchronous messages may include within them the new or updated data itself. When the BOA module 1110 receives one or more of these notifications, it updates the data model or data models that correspond to the particular device and/or information received (block 1742). For example, if new patient charting information is received from the patient charting module 1112 (which may be running on the patient charting device 108), the BOA module 1110 will update the patient charting data model to reflect the most recent data. The BOA module 1110 then refreshes its display (block 1744), which results in the currently displayed data model being replaced with the new data model immediately if any data in the data model was updated in block 1742. The data model update may then be sent to the BOA enterprise module which may reside on enterprise application server 128 (block 1746), which may result in an asynchronous message being generated to the BOA enterprise module (block 1748), according to embodiments of the present invention.

[0253] Some embodiments of the present invention include various steps, some of which may be performed by hardware components or may be embodied in machine-executable instructions. These machine-executable instructions may be used to cause a general-purpose or a special-purpose processor programmed with the instructions to perform the steps. Alternatively, the steps may be performed by a combination of hardware, software, and/or firmware. In addition, some embodiments of the present invention may be performed or implemented, at least in part (e.g., one or more modules), on one or more computer systems, mainframes (e.g., IBM mainframes such as the IBM zSeries, Unisys ClearPath Mainframes, HP Integrity NonStop servers, NEG Express series, and others), or client-server type systems. In addition, specific hardware aspects of embodiments of the present invention may incorporate one or more of these systems, or portions thereof.

[0254] As such, FIG. 18 is an example of a computer system 1800 with which embodiments of the present invention may be utilized. According to the present example, the computer system includes a bus 1801, at least one processor 1802, at least one communication port 1803, a main memory 1804, a removable storage media 1805, a read only memory 1806, and a mass storage 1807.

[0255] Processor(s) 1802 can be any known processor, such as, but not limited to, an Intel® Itanium® or Itanium 2® processor(s), or AMD® Opteron® or Athlon MP® processor(s), or Motorola® lines of processors. Communication port(s) 1803 can be any of an RS-232 port for use with a modem based dialup connection, a 10/100 Ethernet port, or a Gigabit port using copper or fiber, for example. Communication port(s) 1803 may be chosen depending on a network such a Local Area Network (LAN), Wide Area Network (WAN), or any network to which the computer system

1800 connects. Main memory 1804 can be Random Access Memory (RAM), or any other dynamic storage device(s) commonly known to one of ordinary skill in the art. Read only memory 1806 can be any static storage device(s) such as Programmable Read Only Memory (PROM) chips for storing static information such as instructions for processor 1802, for example.

[0256] Mass storage 1807 can be used to store information and instructions. For example, hard disks such as the Adaptec® family of SCSI drives, an optical disc, an array of disks such as RAID (e.g. the Adaptec family of RAID drives), or any other mass storage devices may be used, for example. Bus 1801 communicably couples processor(s) 1802 with the other memory, storage and communication blocks. Bus 1801 can be a PCI/PCI-X or SCSI based system bus depending on the storage devices used, for example. Removable storage media 1805 can be any kind of external hard-drives, floppy drives, flash drives, IOMEGA® Zip Drives, Compact Disc-Read Only Memory (CD-ROM), Compact Disc-Re-Writable (CD-RW), or Digital Video Disc-Read Only Memory (DVD-ROM), for example. The components described above are meant to exemplify some types of possibilities. In no way should the aforementioned examples limit the scope of the invention, as they are only exemplary embodiments.

[0257] Embodiments of the present invention may be configured to achieve various other solutions in an emergency medical services environment. For example, the BOA device 104, in communication with the navigation device 110, may be configured to provide additional mapping and/or navigation information. The BOA device 104 may display status information about a hospital destination, and may indicate diversion or alternative destinations to direct the ambulance 101 to an appropriate destination, according to embodiments of the present invention. The BOA device 104 may also display characteristics about hospitals and/or other destinations, such as the hospital's capabilities (e.g. heart specialty, burn specialty), insurance accepted, patient capacity and current patient capacity status, according to embodiments of the present invention. The BOA device 104 may also be in communication with the enterprise workstation 122 of the hospital or other destination to permit preregistration or partial preregistration of the patient 116. According to embodiments of the present invention, a hospital without availability shows up for the ambulance driver 112 as not available. The BOA device 104 may be configured to display such information simultaneously with a map and/or during navigation, to facilitate destination selection. This information may be obtained over the network 120 from an enterprise server 126 or 128 and/or from an enterprise workstation 122 and/or from the navigation device 110, according to embodiments of the present invention.

[0258] The BOA device 104 may also be configured to communicate in various ways with the user, including with the EMS driver 112 and/or the EMS technician 114, according to embodiments of the present invention. For example, the BOA device 104 may be configured to provide audio prompts, alarms, scheduling, timing, and/or audio streams to EMS users. The BOA device 104 may be configured with Bluetooth® connectivity or capability, such that a user may connect or pair a unique Bluetooth® device with BOA 104 to receive audio information and/or to communicate voice prompts. An alarm may be configured to sound or to display visually upon a triggering event, for example upon receipt

by the BOA device 104 of an asynchronous event signal from a sensor indicating that a detected parameter is outside an acceptable range or value, according to embodiments of the present invention. Audio and/or visual cues may be used to alert a user to a particular dosage schedule, for example beeping when a certain amount of time has elapsed since a first administration of a drug. Such alarms and/or schedules may be set or customized by the users, or may be selected from a predetermined set of alarm and scheduling options, according to embodiments of the present invention.

[0259] According to embodiments of the present invention, the BOA device 104 may provide role-based data and/or audio streams; for example, a technician administering CPR may receive audio and/or visual information about the patient's cardiac condition, but the BOA device 104 may filter out other information such as mapping and/or routing information for that user. Private, customized feedback and/or information may be provided to EMS users based on their roles, according to embodiments of the present invention.

[0260] The BOA device 104 may further provide decision support for an EMS technician, according to embodiments of the present invention. Based on information entered by the technician 114 (e.g. via a patient charting device 108) and/or information received from a patient monitoring device 106, BOA device 104 may compare the information with internal or external databases to display or otherwise convey a differential diagnosis, and/or predictive diagnosis (e.g. based on vectors or EKG information), according to embodiments of the present invention. For example, the BOA device 104 may present the EMS technician 114 with a decision matrix based on symptoms and/or responses to treatments to help the EMS technician 114 determine, for example in an interactive format, a potential diagnosis. The BOA device 104 may provide protocols or links to protocols based on the information received, either from the technician 114 or from one of the devices with which it is in communication.

[0261] In one embodiment, the data for the patient's history may be entered via the BOA device 104 with patient physiological measures via the monitor of BOA device 104. As the differential diagnosis requires both patient history, patient examination findings, and measures of the patient's physiological state via such monitoring as ECG, capnography and pulse oximetry, these data elements are integrated into a user interface that automatically or semi-automatically integrates the various data elements on a single differential diagnosis screen within the application on the BOA device 104, according to embodiments of the present invention. The interface of BOA 104 begins by asking the rescuer to choose from a list of common presenting symptoms or complaints by the patient, e.g. dyspnea or respiratory distress. The information such as on the screens illustrated in FIGS. 26-28 (taken directly from Am Fam Physician 2003; 68:1803-10, which is incorporated by reference herein) and FIG. 29 (taken directly from the Collier County Common Medical Protocol, revised Feb. 1, 2008), provides a structured approach for rescuers to obtain information. As patient history and physical examination findings are entered into the BOA device 104, the differential diagnosis page may gradually narrow down the possible diagnoses. Heart sound measurement and detection may be incorporated into the monitoring device 106 for the detection of S3 and S4 heart sounds and automatically narrow the differential, or suggest

for the rescuer to confirm agreement with the software diagnosis, of heart failure or pulmonary edema. A flowchart for incorporating heart sounds is shown in FIGS. 26-29. Pulse oximetry and capnography are also very helpful measures and may be automatically incorporated into the algorithm for more accurate diagnosis.

[0262] In one embodiment, rescuers may be able to simply touch the cursor to the history or physical exam findings listed as possible from the screen-displayed lists of FIGS. 26-29, thereby minimizing unnecessary keying inputs. At the bottom of each list of possible findings or history is a data entry position for "Other", for those findings or history which are not normally consistent with the presenting condition. In one embodiment, these additional findings, history or physiological measurements can be compared with a larger differential diagnosis database to suggest other possibilities to the rescuer based on a calculated probability or if the other possible causes have been ruled out, according to embodiments of the present invention.

[0263] In much the same way that twelve-lead data and other BOA 104 device data may be sent to an enterprise environment 102 and displayed and/or retrieved on an enterprise workstation 122 or web-based environment, the BOA device 104 may also be configured to receive, display, and/or store similar information from an enterprise environment 102, according to embodiments of the present invention. For example, in a situation in which a patient is being transported from one hospital to another to receive specialized care, the hospital may send to the BOA device 104 information about the patient's vitals and/or health history and/or physician recommendations. Alternatively, the hospital may grant electronic authorization for the remote EMS technician to query its database or databases where such information is kept, to enable the EMS technician 114 to select, using the BOA device 104 interface, which and how much information he would like to receive. In this way, technicians in an ambulance 101 can see what is happening to a patient at the hospital, for example.

[0264] The BOA device 104 may also include speech recognition software and/or text-to-speech software, according to embodiments of the present invention. As such, the BOA device 104 may provide an audio signal that reads text or numeric data received from one or more devices, to convey the data to the EMS technician 114 audibly, such that the EMS technician 114 need not divert visual attention from the patient or from another task, according to embodiments of the present invention. The BOA device 104 may also recognize voice command prompts, to enable the user to operate the BOA device 104 by voice instead of having to divert manual attention from the patient or the task at hand, according to embodiments of the present invention.

[0265] The BOA device 104 also be configured to retrieve audio data stored on a device, such as a patient monitoring device 106, to help the EMS technician 114 in treatment or diagnosis, and/or for storage, technician evaluation, quality control, or later playback. For example, the patient monitoring device 114 may be a defibrillator that records a continuous audio stream; the BOA device 104 may access the continuous audio stream and permit selective play back of certain portions and/or transmit the audio stream or audio file for remote access or storage, according to embodiments of the present invention. The BOA device 104 may also be configured to receive audio information from a patient monitoring device 106 or other device even before the EMS

technician 114 has reached the patient, to help the EMS technician 114 to prepare for the scene.

[0266] The BOA device 104 may be configured to connect with a video monitoring device, for example a webcam, or a standalone video camera, and/or a video capture device that is mounted on or part of another device to which the BOA device 104 connects, according to embodiments of the present invention. For example, a video or still camera mounted in the back of an ambulance 101 may provide visual data to BOA 104 for storage and/or transmission and/or retransmission to the enterprise environment 102 and/or the administration environment 103. Such a video feed may permit a physician waiting at a hospital to view the patient's status before the patient arrives, for example.

[0267] With an ability to connect with and interface multiple EMS-related devices, both clinical and non-clinical, and aggregate such EMS-information (both clinical and non-clinical) from multiple devices, the BOA device 104 may also be configured for inventory monitoring and control. For example, the BOA device 104 may be communicably coupled with a bar code scanner, a radio frequency identification ("RFID") receiver or transceiver, or other inventory monitoring device. The BOA device 104 may maintain or communicate with a database that tracks a particular set of inventoried items, whether they be medical devices, supplies, drugs, personnel, or the like.

[0268] For example, the BOA device 104 may include a database that tracks the inventory of devices, supplies, and drugs on board a particular ambulance 101. When a new device is placed on the ambulance 101, the new device is equipped with a tag or bar code or some other unique identifier, and the BOA device 104 may be configured to automatically sense, or to be instructed to sense (e.g. by scanning a bar code with the bar code scanner), the presence of a new inventory item. The BOA device 104 may also prompt the user with a status update request, for example: new item, item being removed, item being dispensed, item destroyed, item transferred. Hence, at the beginning of an ambulance 101 shift, the crew may query the BOA device 104 to display the inventory of devices, supplies, and/or drugs on board, and may supplement the inventory for any deficient item. When a drug is administered, it may be scanned into the BOA device 104 system with an indication that it has been dispensed and should be replaced. At the end of a shift, the crew may check the inventory via the BOA device 104 and restock necessary supplies and/or transmit the inventory situation to a third party for any appropriate restocking, monitoring, and/or verification activity.

[0269] Such inventory information may also be conveyed by BOA 104 for remote use and/or storage. For example, a defibrillator patient monitoring device 106 may be checked out to each crew of each ambulance 101, and this information may be sent by BOA device 104 through network 120 to the enterprise storage server 126, which may aggregate such information across multiple ambulances 101. A shift supervisor using a remote enterprise workstation 122 may query such database to determine which defibrillators are out in the field on which ambulances 101, according to embodiments of the present invention. In this way, the BOA device 104 may auto-upload inventory information to a central system.

[0270] The BOA device 104 may also be configured to connect with devices (clinical and/or non-clinical) that track EMS technician 114 and patient 116 safety, according to

embodiments of the present invention. For example, the BOA device 104 may be configured to connect with accelerometer and/or tire pressure sensors, and/or other vehicle-related sensors to track driving conditions, driving behavior, safety level, and/or event occurrences, according to embodiments of the present invention. According to one embodiment of the present invention, the BOA device 104 may be configured to connect with a breathalyzer device, which may be used to sense and/or estimate the blood alcohol content of the driver and/or patient. The BOA device 104 may collect such data and display it to the user in a feedback format, and/or may send such data through the network 120 for storage and/or remote evaluation, according to embodiments of the present invention. The BOA device 104 may also monitor a vehicle's maintenance schedule and alert the user when maintenance is needed or recommended, according to embodiments of the present invention.

[0271] Due to its connection with the network 120 and also with other devices 106, 108, 110, the BOA device 104 may also serve as an ambulance headquarters and/or a type of "repeater" in a trauma or disaster situation, according to embodiments of the present invention. For example, the BOA device 104 may be configured to connect with multiple devices including devices outside the ambulance 101 and/or in a different ambulance 101, to permit the BOA device 104 user to view and manage response treatments, for example. Such a configuration also permits data from multiple devices (e.g. multiple defibrillators or other patient monitoring devices) to be conveyed through the network 120 to an enterprise environment 102 and/or administration environment 103, according to embodiments of the present invention. In another example, a single ambulance 101 equipped with a BOA device 104 system as described above may be deployed to a disaster or trauma situation, and the BOA device 104 may be connected to and aggregating information from multiple patient monitoring devices 106. A supervisor or situation manager may use the BOA device 104 to monitor treatment status, prioritize patient medical needs, transmit relevant information to selected outside caregivers, hospitals, and/or treatment centers, and to distribute resources accordingly.

[0272] According to some embodiments of the present invention, the BOA device 104 is configured to perform diagnostics on and/or to initiate self-diagnostics for devices with which it is connected. The BOA device 104 may also be used for training and/or education of EMS technicians 114, by making downloaded protocols available for display, and/or by simulating a medical emergency (e.g. simulating the device feeds from multiple clinical and non-clinical devices during a medical emergency or transport).

[0273] According to some embodiments of the present invention, the BOA device 104 provides a visual indication of whether its connection with the navigation device 110 (or other predetermined device) is online or offline. According to some embodiments, the user can select to view historical rather than current patient information; for example, the user may select to view thumbnails of previous twelve-leads, and can send a collection of twelve-lead data snapshots to an enterprise environment 102 (e.g. a hospital), each with a unique serial number, for example. The enterprise user 124 may also view the patch notes from the BOA device 104, so that the EMS technician 114 need not convey them telephonically, according to embodiments of the present invention.

[0274] The BOA device **104** may also include a drop-down menu interface, listing each device to which the BOA device **104** is connected and its connection status, according to embodiments of the present invention. The BOA device **104** may also be connected with a biometric device such as a fingerprint reader or a retinal scanner, or a non-biometric device such as a keypad, to assist in verifying the identity of a patient and/or in authorizing access to patient medical records. Such records may be stored in remote databases and/or stored by different entities, for example.

[0275] FIGS. 20-23 illustrate an EMS communication interface device **2000**, configured to facilitate communication between a patient monitoring module **1102** and a device adapter/communication interface **1104** (see FIG. 11). Not all patient monitoring devices **106** include the hardware necessary for certain kinds of communication (e.g. wireless communication), either with BOA device **104** or with other enterprise environments **103**. An EMS communication interface device **2000** may be added as an accessory to the patient monitoring device **106** in order to supplement its communication capability, as well as provide additional functionality, according to embodiments of the present invention.

[0276] The EMS communication interface device **2000** may be configured to interface with the patient monitoring device **106** via an existing hardware interface, such as, for example, via a PCMCIA card slot, a USB slot, or the like, according to embodiments of the present invention. The following example illustrates an EMS communication interface device **2000** that interfaces with a patient monitoring device **106** via a PCMCIA card slot in the device **106**, according to embodiments of the present invention.

[0277] FIG. 20 illustrates a carrier board **2010** design for an EMS communication interface device **2000**, according to embodiments of the present invention. The carrier board **2010** may be a custom carrier board for a systems-on-module ("SOM") hosting of various subsystems. The carrier board **2010** may host a PCMCIA edge connector **2030**, PCMCIA address and control transceivers **2012**, PCMCIA data transceivers **2014**, a board power supply **2016**, a first-in-first-out ("FIFO") co-processor input memory buffer **2018**, a flash memory common memory plane ("CMP") **2020**, a complex programmable logic device ("CPLD") attribute memory plane ("AMP") spoof shifter **2022**; a universal serial bus ("USB") universal asynchronous receiver-transmitter ("UART") bridge **2024**, a CPLD programming interface **2026**, and a reset push button **2028**. The power supplies for 3.3V, 1.8V, and 1.5V levels may be derived from PCMCIA 5V and possibly 12V inputs, according to embodiments of the present invention. Device **2000** may further include a USB 2.0 port.

[0278] The carrier board **2010** may also include a SOM coprocessor subsystem **2040** such as, for example, a Gumstix Overo Air SOM or a LogicPO xxxSOM. SOM **2040** may include a Bluetooth ("BT") radio and/or antenna and/or a WiFi (e.g. 802.11a/g) radio and/or antenna **2042**. The 802.11 a/g subsystem may be initialized and configured during boot, and may also be configured via terminal session, according to embodiments of the present invention. SOM **2040** may also include a storage device **2044**, such as, for example, a removable micro SO storage/memory slot. A micro SO card may be used in such a slot as random access storage as well as a source of the boot strap code to initialize the co-processor subsystem **2040**. SOM **2040** may also include a power management integrated circuit ("IC") **2048**,

such as, for example, a Texas Instruments TPS65950 integrated power management IC. SOM **2040** may also include a processor **2046** such as, for example, a TI Open Multimedia Applications Platform ("OMAP") 3503 processor with 256 MB of random access memory ("RAM") and 256 MB of non-volatile RAM ("NVRAM") in a package-on-package ("POP") package. The coprocessor subsystem **2040** may be communicably coupled to the carrier board **2010** via dual 70-pin headers, according to embodiments of the present invention. The carrier board **2010** may also include a Joint Test Action Group ("JTAG") interface for programming, according to embodiments of the present invention.

[0279] The device **2000** may include CPLO firmware, such as, for example, Actel Igloo Nano AGL250V2-VQG100_0. Such CPLO firmware may govern linear flash ("LF") control signals for read/write operations, may govern FIFO control signals for write and read operations in a manner of a FIFO dual-ported implementation, and may employ level shifted address and data buses for LF, FIFO, and the OMAP, according to embodiments of the present invention. The device **2000** may include an operating system, such as, for example, OE 2.6.x Open Embedded Linux. The device **2000** may employ the C# Common Language Runtime (2.6.2), for example the Mono common language runtime ("CLR"), according to embodiments of the present invention. The device **2000** may include persistent data storage using SQLite software library, according to embodiments of the present invention. The device **2000** may perform asset management patterned data storage for framed data, and/or asset management patterned services for parameterized frame retrieval, according to embodiments of the present invention. The device **2000** may accomplish WiFi communications using User Datagram Protocol/Internet Protocol ("UDP/IP") for streaming data output, a .NET remoting service bus, and/or a .NET remoting eventing bus, according to embodiments of the present invention.

[0280] FIG. 21 illustrates a system overview for an EMS communication interface device **200**, according to embodiments of the present invention. A patient monitoring module **1102** processes and sends patient monitoring data. The patient monitoring module **1102** may be implemented by a Zoll E-Series Defibrillator, according to embodiments of the present invention. Such patient monitoring module **1102** is configured to transmit streaming patient vital signs and twelve lead information, as well as full disclosure data, over a BT wireless connection **2110**, to a BT plug-in **2112** that is part of a device adapter **1104**, according to embodiments of the present invention. As used herein, the term "Full Disclosure Data" means all data recorded by a patient monitoring device **106**, and includes, without limitation, patient vital signs, twelve-lead data, audio information, ECG information, lead type, gain, defibrillator shock information, system mode, paddle type, heart rate alarm status, heart rate, configuration information, code marker information, non-invasive blood pressure measurements, patient name, patient identification, biphasic defibrillator data, invasive blood pressure information, invasive blood pressure waveform data, temperature data, SpO2 information, SpO2 waveform, sample number information, accelerometer information, accelerometer waveform, impedance waveform, CPR field data, APLS waveform, and/or APLS compression detection.

[0281] A WiFi wireless connection has a much higher bandwidth for the transfer of information than a BT wireless connection. However, in some cases, the patient monitoring

device **106** on which the patient monitoring module **1102** runs may not include WiFi capabilities, but it may include a personal computer memory card international association (“PCMCIA”) card slot with a PCMCIA interface **2114**. A PCMCIA card may also be referred to as a PC card. The EMS communication interface device **2000** may be plugged in to the PCMCIA card slot **2114**. The device **2000** may include a linear flash memory card **2122** or other memory element for recording full disclosure data from the patient monitoring device **106**, according to embodiments of the present invention. The memory card **2122** may be used to replicate all existing memory card functionality of the patient monitoring device **106**, by storing in linear flash memory **2122** all data written to the patient monitoring device **106** data slot, by permitting a utility mode user-initiated retrieval of stored data from linear flash memory **2122**, and/or by permitting a utility mode user-initiated erasure of the linear flash memory **2122**, according to embodiments of the present invention.

[0282] The full disclosure data stream from the patient monitoring module **1102** may also be received through the PCMCIA slot **2114** by an EMS communication interface module **2116**, which transforms the full disclosure data into incident data, and provides the incident data over a WiFi connection **2118** to a WiFi plug-in **2120** that is part of the communication interface **1104**, according to embodiments of the present invention.

[0283] FIG. 22 illustrates another system overview for an EMS communication interface device **2000**, according to embodiments of the present invention. As illustrated in FIG. 21, full disclosure data is recorded in a memory module **2122**, for example a flash linear analog memory module **2122**, according to embodiments of the present invention. The flash analog module **2122** may be read, written, and/or erased by the patient monitoring module **1102** similarly to the fashion in which any memory element permanently associated with the patient monitoring device **106** may be read, written, and/or erased by via the device **106**, according to embodiments of the present invention. This may be accomplished by using a utility mode of the device **106**, for example. As such, the flash analog **2122** is not interfaced to the SOM (e.g. to microprocessor **2204**), but only to the patient monitoring module **1102** in write/read/erase fashion.

[0284] According to embodiments of the present invention, the flash analog memory **2122** is designed to resemble the linear flash card that is normally associated with, and which may be embedded within, the patient monitoring device **106**. Certain information may be stored in a non-volatile memory area, for example in the attribute memory plane, and certain other information may be stored in the first series of bytes of the common memory plane, to make the memory **2122** resemble the internal memory of the patient monitoring device **106**. The communications interface **2116** may be a FIFO buffer **2202**, which may receive full disclosure data from the patient monitoring module **1102** via the PCMCIA interface **2114**, and pass the full disclosure data to a microprocessor **2204**. The FIFO **2202** is unidirectional from the patient monitoring module **106** to the microprocessor **2204**, according to embodiments of the present invention. Incident data sent may also be persisted in the asset management database **2314**.

[0285] According to embodiments of the present invention, the FIFO buffer **2202** and/or the flash analog memory module **2122** are hardware-only solutions that function even

when the SOM **2040** is non-operational. This functionality permits data protection in the case in which the SOM **2040** is not functional, and permits data buffering for the SOM **2040** to initialize (e.g. to boot and start the EMS communication interface services), according to embodiments of the present invention. During therapy mode data capture to the card **2122**, if the SOM **2040** were to be disabled, device **106** data would not be lost, according to embodiments of the present invention. This also permits users who have been trained on utility modes of a patient monitoring device **106** related to the storage of data on a memory module to continue using such utility modes, even with the data being stored on memory module **2122** instead of a memory module internal to device **106**, according to embodiments of the present invention.

[0286] Using a plug-in **2120** that is part of the communication interface **1104**, incident data (“ID”) may be streamed from the microprocessor **2204** over a WiFi connection **2118**. Such information may be received and displayed by BOA device **104**, for example, and may be displayed in real time and/or in clinically significant time (e.g. with a delay not larger than that which permits a medically accurate and timely observation, diagnosis, and/or treatment decision to be made). According to embodiments of the present invention, the incident data may be streamed on a BOA device **104** with no more than a one-second delay. For example, twelve-lead data generated by a defibrillator patient monitoring device **106** may be updated at least once each second, according to embodiments of the present invention.

[0287] The microprocessor **2204** may also be programmed to generate asynchronous (e.g. event based) notifications via an eventing bus, over the WiFi connection **2118**, according to embodiments of the present invention. For example, if a patient vital sign falls outside of present parameters, the microprocessor **2204** may be programmed to send an alarm event via eventing bus across the communication interface **1104**.

[0288] In addition, the microprocessor **2204** may be programmed to permit a two-way service bus/service interface, to permit the requesting of incident data related specific incidents, according to embodiments of the present invention. For example, after a treatment incident, the user may request, via a service bus, from microprocessor **2204** all information associated with the particular incident (using a unique incident identifier, such as a case number, patient name, or the like). The microprocessor **2204** would then query the asset management module **2314** and retrieve any records associated with the particular incident, and send them back out through service bus, according to embodiments of the present invention. In this way, users may retrieve specific incident data rather than having to download all of the card file data (which in many cases will relate to multiple incidents, or information beyond the specific subset of information sought). This is made possible by the conversion of full disclosure data into incident data by the microprocessor **2204** prior to storage and/or forwarding. In some cases, users may wish to request all data stored by asset management module **2314**, which would be a similar operation to the request for the card file directly from the patient monitoring module **1102**.

[0289] FIG. 23 illustrates a software logic diagram for an EMS communication interface device **2000**, according to embodiments of the present invention. A Linux Kernel **2302** may include a general purpose input/output (“GPIO”) mod-

ule **2304** configured to receive the data stream (e.g. the full disclosure data) **2301** from the patient monitoring device **106**. The data stream **2301** is interfaced to the system **2000** through the FIFO module **2202** which is controlled with several GPIO **2304** lines, according to embodiments of the present invention. The FIFO is read to the SOM using GPIO status, control and eight bits of data, according to embodiments of the present invention. The byte stream driver **2308** may be implemented in user space rather than a device driver to facilitate debugging, in some embodiments. The byte stream driver **2308** may keep the FIFO **2202** drained by monitoring the FIFO **2202** empty flag (which may be polled as opposed to interrupt driven for debugging efficiency in one embodiment).

[0290] Bytes read from the FIFO by the byte stream driver **2308** are re-assembled as blocks similar to those delivered by the patient monitoring device **106** and framed in the data formatter **2310**, according to embodiments of the present invention. This results in a frame event stream **2303** from the data formatter **2310**. The frame event stream is then sent to an asset management module **2312**, which saves the frames to the database **2314** and forwards them out the WiFi channel to the TCP/IP module **2306** of the Linux Kernel **2302**. According to some embodiments of the present invention, the frame event stream **2303** is sent over the WiFi connection via an encrypted UDP broadcast, so that it may be received by a wide range of clients (e.g. an iPhone may be configured to receive the UDP broadcast). The frame event stream **2303** may also be received by a clinical time feed plug-in **2316** of the communications interface module **1104**, according to embodiments of the present invention.

[0291] Asynchronous requests for incident data stored in the database **2314** may be made by authorized external clients, such as via an incident plug-in **2318** of the communications interface module **1104**, according to embodiments of the present invention. Such incident service calls are shown in dashed lines in FIG. 23. Although database **2314** is shown as an SQLite database, one of ordinary skill in the art will appreciate, based on the disclosure provided herein, that other database formats may be employed by asset management module **2312**, according to embodiments of the present invention.

[0292] According to embodiments of the present invention, the byte stream is formatted by data formatter **2310** into blocks of data resembling device **106** data blocks, and these full data blocks are broadcast in a WiFi format upon construction (e.g. as a block is made, it is sent over the WiFi interface). According to embodiments of the present invention, the asset management module **2312** frames the byte stream into consistent blocks of time, for example one second per frame, and each frame is saved into the asset management patterned data storage (e.g. database **2314**).

[0293] Although FIGS. 21-22 show full disclosure data as two separate feeds, a single full disclosure data feed may be bifurcated and sent to both the flash analog module **2122** and the FIFO **2202** simultaneously, according to embodiments of the present invention.

[0294] A user may query the device **2000** to request health information, for example, running time, exceptions detected, and other information from the patient monitoring device **106**, according to embodiments of the present invention. A user may also request specific incident-based data from the device **2000**; for example, a user may send a query that says "send all of the cases," or "send data relating to a specific

case" or "send all twelve-lead data from a specific case." The device **2000** may also stream delivery of case data so as to permit multiple authorized receivers (e.g. multiple BOA devices **104**) to obtain the data simultaneously, according to embodiments of the present invention. According to some embodiments of the present invention, device **2000** facilitates data sharing between the patient monitoring device **106** and the enterprise environment **103**.

[0295] On power up, the device **106** interrogates the occupant of the PCMCIA slot **2114** to ascertain if a valid linear flash card **2122** is present. The validity test may consist of reading a series of bytes from the LF AMP and validating the values against sets of acceptable cards or an acceptable card. If a valid card is found, the device **106** reads a series of bytes from the CMP to test for validity and to determine if the card has been "formatted" according to the requirements of the device **106**. In the absence of such a series of bytes, the device **106** may write such information to the card **2122**, according to embodiments of the present invention. Once the card **2122** is validated, the device **106** begins to write the device data to the LF card **2122** as byte streams that are formatted into blocks as described, above.

[0296] Although the device **2000** is depicted as interacting with device **106** in a one-way fashion, the device **2000** may also be configured to interact bi-directionally with device **2000**. For example, the device **2000** may be configured to provide a WiFi user interface similar to the user interface observed directly on the patient monitoring device **106**, to permit total or partial remote control of the patient monitoring device **106**, according to embodiments of the present invention.

[0297] Packaged in a PCMCIA type x housing, each card **2010** contains a connector **2030**, an array of flash memories packaged in thin small outline packages ("TSOP") and card control logic. The card control logic provides the system interface and controls the internal flash memories as well as the input FIFO to the SOM, according to embodiments of the present invention. Level shifters are present to adapt PCMCIA logic voltages to card logic voltages.

[0298] Card logic voltages of 3.3V, 1.8V, and 1.5V may be derived from the PCMCIA VCC voltage (TTL, +5V, possibly +12V). A single stage for 3.3V and 5V conversions is built using three discrete transceivers. A CPLD is used to perform 3.3V and 1.8V conversions.

Part	Logic Voltages	Power	Notes
J1	+5 V	+5 V, +12 V	2X34 PCMCIA connector
U5, U6, U7	+5 V; +3.3 V	+5 V, +3.3 V	Level Shifters
U3	+3.3 V	+3.3 V	Flash Memory
U7	+3.3 V	+3.3 V	FIFO
U1	+3.3 V; +1.8 V	+3.3 V, +1.8 V	CPLD
MCU	+1.8 V	+4.0 V	OMAPSOM

[0299] Data enters FIFO at 3.3V from the PCMCIA byte stream. Reading the FIFO is clocked an 8 bit byte at a time on the read clock shifted between 3.3 and 1.8 to OMAP, through the CPLD. OMAP control and status interface bits may be converted in a similar fashion. Each carrier card **2010** may have a USB2.0 port. OMAP UART signals are connected to a USB to UART serial bridge **2024**, according to embodiments of the present invention.

[0300] A JTAG interface for programming the CPLD may be provided. A 2x34, A and B sided PCMCIA Connector (J1)

may be used, that inter-connects I/O, status and power signals between the device and the card, according to embodiments of the present invention. For the device signals that the card interface is interested in, there is a group of three transceivers (U5, U6, and U7) that inter-convert PCMCIA voltage (VCC) and board voltage (3V3), according to embodiments of the present invention. Device **2000** is interested in 26 address bits, 8 data bits, and 6 control signals that are intended to be level-shifted, according to embodiments of the present invention. U5 and U6 are uni-directional **16b** input shifters from device to card for address and control information, according to embodiments of the present invention. U7 is a bi-directional **8b** level shifter for 8 bits of data.

[0301] According to embodiments of the present invention, the device **2000** reads and writes data through this interface to LF memory. U5 shifting 16 address bits [PCAO: PCA15] to [AO:A15]. U6 shifting 10 address bits [PC16: PC25] to [A16:A25], and 6 control signals {PC_REGn, PC_RESET, PC_CE1n, PC_CE2n, PC_OEn, PC_BWEn} to {REGn, RESET, CE1n, CE2n, OEn, BWEn}.

Sig	Description	Active
REGn	Attribute Memory Select	Low
CE1n	Card enable 1	Low
CE2n	Card enable 2	Low
OEn	Output enable	Low
BWEn	Write enable	Low
RESET	Reset	High

[0302] [PCDO:PCD7] 8 data bits (U2). Address shifters may be input only, in which case the card does not generate address information to the device **2000**, only outbound addressing (device to card) is exposed, according to embodiments of the present invention. The data shifter is bi-directional as the device can read and write data to and from the card, according to embodiments of the present invention. U5 shifts 16 bits of address and U6 shifts 8 control signals and the upper 8 bits of the address and control signals from PCMCIA vee to 3V3.

[0303] Device **2000** is configured to permit streaming data transmission via WiFi during therapy mode operations of the device **106**, as well as post-case upload of device data. The device **2000** has hardware components as well as program-mable elements using both firmware and embedded software, including an embedded operating system as described, above. According to some embodiments, the EMS communication interface device **2000** is thicker than a standard Type III PCMCIA card.

[0304] An embodiment of the present invention may include one of more of the following features and/or characteristics:

[0305] The carrier may be a PCMCIA card

[0306] The carrier may be inserted into a patient monitoring device PCMCIA data slot.

[0307] The card **2000** interfaces to the patient monitoring device **106** in such a way as to appear to the patient monitoring device **106** as a valid LF card ("linear flash analog") **2122**.

[0308] The card **2000** presents the PCMCIA byte stream, written by the patient monitoring device **106**, via a buffered hardware interface, to a SOM processor.

[0309] The carrier stores the received PCMCIA byte stream to a non-volatile storage subsystem ("linear flash analog") such that all of the patient monitoring device **106** read/write/erase functionality is preserved in all device **106** modes of operation supporting these operations.

[0310] The SOM provides IEEE 802.11. b/g wireless communications capability.

[0311] The SOM provides Bluetooth V2.0+EDR wireless communications capability.

[0312] The SOM provides a micro SO card slot.

[0313] The SOM supports watchdog type monitoring to provide for automatic reset if the SOM becomes non-functional.

[0314] During patient monitoring device **106** or SOM reset or initialization, data is captured to flash analog memory.

[0315] Data capture continues uninterrupted during SOM reset.

[0316] The system **5000** is designed such that data being written by the patient monitoring device **106** is saved to the flash analog regardless of SOM state

[0317] The SOM is able to access data saved while the SOM was unavailable.

[0318] The carrier board provides a USB connector.

[0319] The carrier SOM combination supports USB 2.0 On-The-Go ("OTG").

[0320] Device **2000** form factor includes PCMCIA standard dimensions in width and height.

[0321] Device **2000** form factor includes a width of 85.6 mm×54.0 mm×a thickness (in some cases, this thickness is greater than type III which is 10.5 mm)

[0322] Device **2000** thickness is no larger than permitted by device **106** PCMCIA slot.

[0323] All carrier board components are mounted on one side of the carrier card.

[0324] The interface to the patient monitoring device **106** is via slot bay via 68-pin PCMCIA card edge connector.

[0325] Device **2000** is encapsulated to meet medical device requirements for EMC/RFI.

[0326] The SOM is mounted on the carrier using 2 AVX 5602 70 pin connectors.

[0327] Device **2000** is powered from the PCMCIA data slot, which may be on the order of 2.5 W continuous with peak current not exceeding 600 mA.

[0328] Device **2000** may utilize 15 GPIO pins to control reading FIFO byte stream buffer.

[0329] Device **2000** may utilize 3 UART lines from the SOM connected and a USB bridge on the carrier.

[0330] Device **2000** may include an antenna for WiFi.

[0331] Device **2000** may include an antenna for BT.

[0332] Device **2000** may use an Angstrom Open Embedded Linux operating system ("O/S").

[0333] The device **2000** O/S may include Mono for the purposes of running code implemented inC#.

[0334] The device **2000** O/S may include SQLite.

[0335] The device **2000** may support the use of USB for bidirectional serial communications.

[0336] The device **2000** provides secure wireless communications, including end-point authentication, confidentiality, integrity, and/or delivery confirmation.

[0337] External data recipients (external processes to the device 2000) are able to request streaming data delivery.

[0338] Data recipients are able to request complete incident data delivery by incident identifier, e.g. post-incident data.

[0339] Device 2000 software is upgradeable via wireless interface.

[0340] Device 2000 software is verified at run time using a cyclic redundancy code ("CRC")-like mechanism.

[0341] A device 2000 according to an embodiment of the present invention may permit individual screens for different receiving devices (e.g. different receiving devices using the communications interface 1104) to permit different users to obtain different data. For example, one user's settings could be configured to receive and display the frame event stream data relating to a patient's twelve-lead data, while an administrative technician user's settings could be configured to periodically request only frames associated with error codes generated by the patient monitoring device 106, according to embodiments of the present invention. Similarly, the same data may be received by and/or displayed by multiple users simultaneously over a WiFi connection, according to embodiments of the present invention.

[0342] In this way, the data from a patient monitoring device 106 may be streamed, e.g. over a wireless WiFi connection, from a patient's house to or from an ambulance, and/or from an ambulance to or from a hospital. Various frames in the event stream may be filtered and/or requested, such that a specific subset of data may be obtained. For example, respiration data may be included in a frame event stream generated by device 2000, according to embodiments of the present invention.

[0343] A device 2000 according to an embodiment of the present invention may be combined with other types of patient monitoring devices 106, for example an automatic external defibrillator ("AED"). The device 2000 may thus be configured to send status information from the AED, to facilitate software updates for the AED, and/or to remotely test the AED, according to embodiments of the present invention. Such a device 2000 may also be used with a patient charting device, for example to combine the patient charting device 108 information from one vendor/platform with the patient monitoring device 106 information from another vendor/platform, according to embodiments of the present invention. The device 2000 may also function as a data aggregator, to parse, organize, and place streams of information into discrete frames information that are more easily sorted, queried, and supplied at a later, post-incident time frame, according to embodiments of the present invention.

[0344] According to embodiments of the present invention, the patient monitoring device 106 (e.g. defibrillator) sends data to the device 2000 in data blocks, for example ECG data, or patient's current heart rate. A collection of data blocks corresponding to one incident may be referred to as incident data. Full disclosure data is the concatenation of data associated with all incidents, and may be broken into sequences of data blocks corresponding to each individual/patient. When a service request is received for an incident, all of the frames stored on device 2000 for that incident are collected and put together in sequence. According to embodiments of the present invention, each ECG block

corresponds to 100 ms of ECG data, which provides ten data blocks per second. The defibrillator may add to each data block an incident identifier, time information about when the data block was recorded, and/or a computing hash for data integrity purposes, according to embodiments of the present invention.

[0345] Device 2000 (which is referred to in some figures as a "Zango" device) and BOA device 104 (which is referred to in some figures as a RescueNet Link, or RNL, device) work together, according to embodiments of the present invention. Device 2000, by virtue of its embedded computer, embodies a powerful processing engine. This processing engine is used to manage sophisticated data, communications, and applications operations on behalf of BOA device 104 users, according to embodiments of the present invention. According to one embodiment of the present invention, the device 2000 does not have input/output user interfaces (e.g., no keyboard, or display), so it works in conjunction with BOA device 104 to provide users access to the communications and data management services it supports, according to embodiments of the present invention.

[0346] FIGS. 20 and 23 illustrate the logical and functional architecture of the EMS communications interface card 2000 processing and the BOA device 104 processing, respectively. When device 2000 is not connected to device 104, device 2000 stores all device data and can transmit it to device 104 when a connection is established or restored.

[0347] FIG. 30 illustrates a data transmission interface, according to embodiments of the present invention. Zango device (1a), can be configured to perform a number of functions, according to embodiments of the present invention:

[0348] Frame defibrillator incident data blocks.

[0349] Stream framed incident data.

[0350] Save incident data frames to Zango database.

[0351] Host a set of data management services upon the Zango database.

In one embodiment, data management services are read/erase only. Services to modify incident data are not supplied.

[0352] The "EMS communications interface channel" (1a, 1b, 1c) provides a means to transmit patient monitoring data (e.g. E Series data) to the BOA device 104. This channel uses the device 2000 to connect to BOA 104.

[0353] The RNL Zango Client (1c) can be configured to perform a number of functions:

[0354] Receive streamed incident frame data (1b).

[0355] Present incident frame data on the Mobile Link Display (1e) (parse, render, 1d).

[0356] Store incident frame data into the Mobile Link database (1f)

[0357] Host a set of data management services upon the Mobile Link database (1f). In some embodiments, data management services are read/erase only; and services to modify incident data are not supplied.

[0358] Forward 12 lead ecg and vitals data to Field Link. (1g)

[0359] Consume Zango data management services (1b).

[0360] The following table lists and describes various elements of FIG. 30, described with respect to one embodiment of the present invention.

Notation (FIG.)	Description	Notes
1a	Zango accessory	Data management accessory for ZOLL E Series. Captures, stores, and transmits E the E Series data slot to connect the E Series data to
1b	Zango UDP/IP transmissions over WPA2 secured	
1b	Zango TCP/IP service invocation response transactions over RNL Zango Client	
1c		RNL receiver of Zango
1a, 1b, 1c	Zango channel	
1d	Zango parsing and rendering engine	Zango messages from the E Series are parsed and rendered for acute
1e	Mobile Link Display	
1f	Mobile Link Storage	
1g	RNL Protocol: Reliable UDP/IP over secured	
1h	RNL Field Link Server	Mobile link message receiver in Field
1c, 1g, 1h	RNL Mobile Link to Field Link Communications Channel	The RNL Mobile Link to Field Link Channel connects Mobile Link to Field Link using reliable UDP/IP
1j	Field Link Storage	
1i	Field Link parsing and rendering	
1k	Field Link web server	
1l	Secured connection to	
1m	Field Link web	

[0361] FIG. 31 illustrates an EMS communication interface transmission processing block diagram, according to embodiments of the present invention. The E Series writes a continuous byte stream of data to the PCMCIA Data Slot. The byte stream consists of E Series data block messages some of which are sent periodically and some of which are sent episodically. An example a periodic message is the ecg message. The E Series writes the ecg values for the currently displayed lead once per 100 ms, the message contains 25 data values (250 Hz samples, 4 ms apart), according to embodiments of the present invention.

[0362] Examples of episodic messages are the vital sign messages. The E Series sends a particular vital sign message when a particular vital sign parameter value has changed; asynchronous messages are sent with no particular frequency, according to embodiments of the present invention.

[0363] The byte stream is bifurcated at the input to the Zango card. One branch stores data into an on board (16 MB) linear flash, replicating all of the E Series linear flash operations. All data written is stored in the linear flash subsystem. The interface is hardware level, instant on prepared to receive and save the E Series byte stream to flash subsystem.

[0364] The second byte stream branch goes into the processor side of the Zango card. The processor side of the Zango card functions to process the byte stream performing

the logical operations illustrated in FIG. 31. In the non-faulted case the byte stream receiver passes bytes to the byte block factory. The byte block factory re-constructs E Series data block messages from the byte stream. In this operation, 12 lead ecg data blocks are reconstructed and managed on a separate path to the incident path (sets of 12 lead data blocks are collected into entire 12 lead messages). The 12 lead data is entirely preserved in the case stream. One of the reasons for storing them separately is to permit a service user to request to see a 12 lead record on the service channel, rather than uploading the entire incident to get the 12 lead data, according to embodiments of the present invention.

[0365] Blocks are then framed into a configurable time interval's worth of data blocks. For example, frames of one second in size might have on the order of 15 data blocks in the one second frame. Frames are collected into constructs of cases or incidents. Frames are stored in the Zango database. Complete incidents are marked (collection of all incident frames) and managed as incidents as they are completed. Frames are also streamed on WiFi where they can be received by authorized client applications, such as the RNL Zango Client described, below, with respect to FIG. 32.

[0366] The upper row of boxes in FIG. 31 identify detection and error handling processes for risk control of compromised data faults, according to embodiments of the present invention. Byte stream, block, framing, 12 Lead, or incident error all result in the following behaviors, according to embodiments of the present invention:

[0367] Data is marked as invalid.

[0368] Invalid data is not rendered for a user to view during the acute treatment phase of an incident

[0369] Data is stored marked as invalid for forensic analysis.

[0370] Any one of these faults will cause the incident to be marked invalid.

[0371] Acute medical personnel are informed of data faults, assuming connectivity to RNL.

[0372] These are the control measures and behaviors that trace directly to the hazard analysis for data compromised faults, in one embodiment of the present invention.

[0373] FIG. 32 illustrates a EMS communications interface device client architecture, according to embodiments of the present invention. In some cases, Zango connectivity to RNL may be volatile as a result of the nature of wireless communications in mobile environments. For example, an E Series equipped with a Zango card may be moved out of range of the wireless access point to which it had been connected. When the device is back in range and reconnects, processing resumes as illustrated. Data written by the E Series while not connected to RNL is persisted in the Zango database and can be obtained in RNL upon re-connect, according to embodiments of the present invention.

[0374] The upper row of boxes in FIG. 32 identify detection and error handling processes for risk control of compromised data faults and communications faults. Integrity or framing faults detected on the streamed data result in the following behaviors, according to embodiments of the present invention:

[0375] Data is marked as invalid.

[0376] Invalid data is not rendered for a user to view during the acute treatment phase of an incident

[0377] Data is stored marked as invalid for forensic analysis.

[0378] Either of these faults will cause the incident to be marked invalid.

[0379] Acute medical personnel are informed of data faults for either 12 leads or case frames.

[0380] Acute medical personnel are informed of communications faults.

[0381] Acute medical personnel are informed of service faults.

[0382] Service responses are validated and invalid service responses are notified to the user and invalid data is not displayed, according to embodiments of the present invention. Connectivity status between Zango and the Zango Stream Channel Receiver is monitored and reported to users on the Mobile Link Display. Lost connectivity between Zango and RNL does not result in lost data as Zango stores data in the Zango database regardless of connection status. Service channel connectivity is not continuously monitored, service requests will fail (response invalid) if service connectivity is not present.

[0383] FIGS. 33-37 illustrate various embodiments of screen shots available as viewed by the enterprise user 124 via the enterprise workstation 122, according to embodiments of the present invention. FIG. 33 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient monitoring button (e.g. the "Zoll Defib" button), according to embodiments of the present invention. FIG. 34 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patient charting button (e.g. the "ePCR" button), according to embodiments of the present invention. FIG. 35 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the navigation button, according to embodiments of the present invention.

[0384] FIG. 36 illustrates an alternative enterprise display and graphical user interface shown when the enterprise user selects the navigation button, according to embodiments of the present invention. The display of FIG. 36 would correspond to a display created when the BOA device 104 is not communicably coupled with a navigation device; hence, in this situation, the enterprise display lists the positional and/or navigation information as input by the BOA 104 user. FIG. 37 illustrates an enterprise display and graphical user interface shown when the enterprise user selects the patch notes button, according to embodiments of the present invention. According to some embodiments of the present invention, the EMS technician 114 who is interacting with the BOA device 104 need not select the patch notes screen and relay the information to the enterprise user 124; instead, the enterprise user may select the patch notes button via the enterprise workstation 122 to observe the same information.

[0385] FIGS. 38-44 illustrate additional examples of screen shots displayed by BOA device 104, according to embodiments of the present invention. FIG. 38 illustrates a display and graphical user interface displayed when the user selects the patient charting button of a BOA menu template, according to embodiments of the present invention. FIG. 39 illustrates a display and graphical user interface displayed when the user selects the patient monitoring button of a BOA menu template, according to embodiments of the present invention. As illustrated by the thumbnail twelve-lead image in the bottom left corner, this BOA device 104 may be configured to display historical snapshots of past twelve-lead data, according to embodiments of the present invention.

[0386] FIG. 40 illustrates a display and graphical user interface displayed when the user selects the navigation button of a BOA menu template, according to embodiments of the present invention. FIG. 41 illustrates an alternative display and graphical user interface displayed when the user selects the navigation button of a BOA menu template, in situations in which a navigation device 110 is not communicably coupled to the BOA device 104. In such situations, the screen of FIG. 41 is configured to permit a user to manually select a destination, as well as select an estimated time of arrival, according to embodiments of the present invention. This information may be replicated or otherwise transmitted to the corresponding enterprise view (e.g. FIG. 36), according to embodiments of the present invention.

[0387] FIGS. 38-44 illustrate that a "shift start" button maybe included on the BOA device 104 interface. The shift start button may be used, for example, at the beginning of a shift, in order to permit the EMS technician or other user to communicably couple the BOA device 104 with other devices, according to embodiments of the present invention. FIG. 42 illustrates a display and graphical user interface displayed when the user selects the shift start button of a BOA menu template, according to embodiments of the present invention. In this screen, the user is permitted to select a navigation device, a defibrillator device, and a patient charting device; in this screen, the user is also able to confirm the identities of the devices to which the BOA device 104 is already communicably coupled, as indicated in this particular example by a checkmark next to the device name, according to embodiments of the present invention.

[0388] FIG. 43 illustrates an alternative display and graphical user interface displayed when the user selects the shift start button of a BOA menu template, according to embodiments of the present invention. In this alternative display, the BOA device 104 has sensed that a navigation device 110 is not available or is disconnected, and thus prompts the user to identify the EMS transport unit and/or the crew members present with the unit. This information may be used in the corresponding navigation screens for the BOA device (FIG. 41) and the enterprise environment 102 (FIG. 36). FIG. 44 illustrates a display and graphical user interface displayed when the user selects the patch notes button of a BOA menu template, according to embodiments of the present invention.

[0389] FIG. 62 illustrates a system for role-based data feeds from a BOA device to EMS technician mobile devices, according to embodiments of the present invention. BOA device 104 receives streaming ECG data and other data from the patient monitoring device 106, which may be accomplished wirelessly via an EMS communications interface device 2000 as described above, according to embodiments of the present invention. The BOA device 104 displays such information on a screen such as the screen illustrated in FIG. 45.

[0390] FIG. 45 illustrates a display and graphical user interface displayed when the user selects a live patient data button of a BOA menu template, according to embodiments of the present invention. This display includes a list of interventions, a display of patient information, a display of chief complaint, an ECG wave form and/or an SpO2 waveform, as well as a button console (shown as extending vertically on the right side of the screen) listing buttons for available patient interventions, according to embodiments of the present invention. The intervention button console may

be dynamic and/or color-coded. The intervention button console may also include timers.

[0391] For example, when a patient's airway is checked, the EMS technician activates (e.g. pushes or touches) the "patient airway" button on the intervention button console. The button activates and displays a timer, which counts down to the next time when the patient's airways should be checked. This amount of time may be customized by the user and/or preprogrammed into the BOA module operating the BOA device 104 based on established treatment protocols for the locale in which the patient is treated. Color may also be used; for example, the buttons of the intervention button console may be normally gray, and the "patient airway" button may turn yellow as soon as the button is pushed and the timer activated. The button may turn red within a predetermined amount of time before expiry of the timer, for example one minute before the expiration of the time period being timed. For example, a user may look at the intervention button console of FIG. 45 and see that doses of Epi and Atropine have recently been administered, because those buttons are yellow and their timers activated, while also seeing that the patient's airway was previously checked and is about ready to be checked again, because that button is red. This permits the EMS technician to rapidly visually assess which interventions have been made, as well as which interventions should (or may, according to protocol) be considered in the near future, for any point in time.

[0392] Different EMS technicians may have different roles to play in an EMS scenario, based on their training or qualifications, the number of available technicians, and the status of the patient. In the same way, a single EMS technician may need to play multiple roles in an EMS encounter. Such EMS technicians may more effectively and efficiently perform their corresponding tasks if they are presented only with the information related to their particular role, such that they do not see extraneous information which they must mentally process and filter, and such that they are not presented with decision-making or data input options that do not apply to their role. One way in which such role-based information delivery may be accomplished is by providing each EMS technician with a mobile device with software configured to permit an interface with a BOA device 104 based on the user's role.

[0393] FIG. 62 illustrates examples of such mobile devices communicably coupled to BOA device 104, including a lead medic mobile device 620, drug medic mobile device 622, airway medic mobile device 624, and CPR medic mobile device 626, according to embodiments of the present invention. According to embodiments of the present invention, each mobile device 620, 622, 624, 626 includes a WiFi transceiver that communicates wirelessly with a WiFi transceiver of BOA device 104.

[0394] FIG. 46 illustrates a start screen for a role-based EMS technician mobile device 620 in communication with a BOA device 104, according to embodiments of the present invention. The software instructions contained on the mobile device render this start screen to permit the medic to identify the IP Address, send port, receive port, medic name, and medic role, according to embodiments of the present invention. FIG. 47 illustrates a role selection screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention. A checkmark next to the "Medic-Lead" listing indicates that the user of the mobile device is the lead medic.

According to embodiments of the present invention, a password or other authentication may be required in order to restrict role based on identity.

[0395] FIG. 48 illustrates a lead medic quick log screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention. The mobile device may be configured to display a list of menu options, for example the menu options shown extending horizontally along the bottom of the screen of FIG. 48 permit the lead medic to choose Quick Log, ECG Graph, Patient Data, Chief Complaint, and Medic Role. These options may differ based on the user's role. When the lead medic clicks on the Quick Log tab, the lead medic is presented with an intervention button panel, according to embodiments of the present invention. The quick log tab display replicates the intervention button console of the BOA live ECG display of FIG. 45, such that when a lead medic pushes an intervention button on the mobile device via the screen of FIG. 48, the same button (and corresponding timer and/or color) is indicated as being activated in the BOA display screen of FIG. 45, and vice versa, according to embodiments of the present invention.

[0396] FIG. 49 illustrates a lead medic ECG graph screen for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention, which is displayed for the lead medic when the lead medic selects the ECG graph menu button. Because the lead medic's role typically requires a broad swath of patient information, the lead medic ECG graph screen essentially recreates the patient data display screen of the BOA device 104 of FIG. 45, according to embodiments of the present invention. FIG. 50 illustrates a lead medic patient data screen, which permits the lead medic to enter patient information, including the patient's name and gender, according to embodiments of the present invention. FIG. 51 illustrates a lead medic chief complaint screen which permits the lead medic to identify the patient's chief complaint, according to embodiments of the present invention.

[0397] FIG. 52 illustrates a drug medic quick log screen and FIG. 53 illustrates a drug medic ECG graph screen for a medic who has identified his or her role as drug medic, according to embodiments of the present invention. Because the medic has identified a role of drug medic, the quick log screen presents only a subset of the interventions which relate to drugs, according to embodiments of the present invention. Although the drug medic role accesses only a subset of the full set of intervention buttons, the same intervention buttons are tied together across the entire platform, according to embodiments of the present invention. For example, if the drug medic indicates that a dose of atropine has been given by tapping the atropine intervention button on his mobile device 622, the atropine button will turn yellow as activated, and begin a timer, not only on his mobile device 622, but also on atropine buttons of the quick log screen of the lead medic device 620 and on the intervention button console of the BOA device 104 display, as well as any other devices whose quick log screens include the atropine intervention button, according to embodiments of the present invention.

[0398] FIG. 54 illustrates a role selection screen in which an airway medic role has been identified (e.g. by tapping or otherwise selecting that option on the mobile device 624). FIG. 55 illustrates an airway medic ECG graph screen, and

FIG. 56 illustrates an airway medic quick log screen listing the subset of interventions that relate to the airway medic's role, according to embodiments of the present invention.

[0399] FIG. 57 illustrates a CPR medic quick log screen illustrating a subset of interventions that relate to the CPR medic's role, according to embodiments of the present invention. FIG. 58 illustrates a CPR medic ECG graph screen during idle for a role-based EMS technician mobile device in communication with a BOA device, according to embodiments of the present invention. FIGS. 59-61 illustrate a CPR medic ECG graph screen during administration of compressions, which do not show the ECG wave form but instead show measurement and/or evaluation of chest compressions (because the CPR medic is concerned primarily with resuscitation), according to embodiments of the present invention. The CPR feedback provided by the screen interface of FIGS. 58-61 may take many different forms. For example, as illustrated in FIG. 59, vertically descending bars may be used to represent depth of each chest compression, spaced horizontally in a manner along a time axis. The chest compression bars descend from an axis toward another set of axes, which specify the desirable or optimal range of depth for each chest compression. A qualitative indicator bar, shown in the upper right, gives the user a combined visual feedback relating to depth and rate of chest compressions; a full box means that both the rate and depth are within desired limits. The letter "R" on FIG. 58 indicates a potential alert regarding the rate of the chest compressions, and the letter "D" on FIG. 61 indicates a potential alert regarding the depth of chest compressions, according to embodiments of the present invention. According to embodiments of the present invention, the CPR feedback screen of device 626 provides information about the rate and volume of patient ventilation.

[0400] According to embodiments of the present invention, the patient monitoring device 106 and/or EMS communications interface device 2000 and/or the BOA device 104 includes a filtering mechanism (e.g. a circuit or processing instructions) that filters or removes chest compression interference from ECG signal data. Embodiments of the present invention may include a device or utilize a method similar to those described in U.S. Pat. No. 7,295,871, issued Nov. 13, 2007, which is incorporated by reference herein. Embodiments of the present invention may also employ Real CPR Help® technology available from Zoll Medical Corporation.

[0401] The use of role-based information delivery and intervention tracking permits a more efficient EMS treatment scenario by filtering data based on role, according to embodiments of the present invention. For example, the drug medic, airway medic, and CPR medic do not have menu tab selections available for patient data entry or for chief complaint entry, while the lead medic has those options.

[0402] Although only four mobile devices 620, 622, 624, and 626 are shown in FIG. 62, the BOA device 104 may communicably couple with a greater or fewer number of role-based mobile devices. Also, although particular intervention options and data feed displays are shown as being related to particular roles, one of ordinary skill in the art, based on the present disclosure, will appreciate the numerous different roles that may be identified and implemented, as well as the numerous different data feeds and/or options that may be associated with each role. Further, mobile

devices (e.g. 620) may be configured to communicably couple with multiple BOA devices 104 and/or to receive information for multiple patients from the same BOA device 104, to permit the medic to toggle between various patient data feeds and/or to treat different patients, possibly in different roles, according to embodiments of the present invention.

[0403] According to embodiments of the present invention, the software modules and hardware contained within the BOA device 104 for feeding the data to and from the mobile devices 620 may be consolidated into an EMS communications interface device 2000, and/or directly into a patient monitoring device 106.

[0404] Various modifications and additions can be made to the exemplary embodiments discussed without departing from the scope of the present invention. For example, while the embodiments described above refer to particular features, the scope of this invention also includes embodiments having different combinations of features and embodiments that do not include all of the described features. Accordingly, the scope of the present invention is intended to embrace all such alternatives, modifications, and variations as fall within the scope of the claims, together with all equivalents thereof.

What is claimed is:

1. A system for supplementing communications capabilities of a patient monitoring device configured to monitor a patient and to make available patient monitoring information, the patient monitoring device having a communications interface slot, the system comprising:

- a card configured to fit within the communications interface slot and to receive the patient monitoring information from the patient monitoring device via the communications interface slot;
- a memory device hosted by the card and configured to store the patient monitoring information;
- a wireless transceiver hosted by the card;
- an asset management database hosted by the card; and
- a processor communicably coupled to the wireless transceiver and the asset management database, the processor configured to format the patient monitoring information into a stream of one or more frames, each of the one or more frames associated with an EMS incident during which the patient monitoring information was gathered, the processor further configured to store the one or more frames to the asset management database and to transmit the stream of one or more frames with the wireless transceiver.

2. The system of claim 1, wherein the processor is further configured to receive, via the wireless transceiver, a request for frames associated with a specific EMS incident, query the asset management database to retrieve all frames associated with the specific EMS incident, and to transmit the frames associated with the specific EMS incident with the wireless transceiver.

3. The system of claim 1, wherein the processor is restricted from editing the patient monitoring information on the memory device.

4. The system of claim 3, wherein the patient monitoring device is configured to edit the patient monitoring information on the memory device.

5. The system of claim 1, wherein patient monitoring information from the patient monitoring device is bifurcated into a first stream and a second stream, wherein the memory

card is configured to store the first stream, and wherein the processor is configured to receive the second stream.

6. A method for streaming patient information from a clinical device comprising:

establishing a wireless data connection with the clinical device;

receiving patient information from the clinical device via the wireless data connection at least once every five seconds; and

displaying at least a portion of the patient information in an emergency medical services mobile environment.

7. The method of claim 6, wherein the clinical device is a defibrillator.

8. The method of claim 6, wherein receiving the patient information comprises receiving the patient information from the clinical device via the wireless data connection at least once every second.

9. The method of claim 6, wherein the wireless data connection is a secure WiFi connection.

10. The method of claim 6, wherein the patient information is clinical information, the method further comprising receiving non-clinical information and displaying the clinical information and the non-clinical information simultaneously in the emergency medical services mobile environment.

11. The method of claim 6, wherein the patient information comprises an ECG waveform.

12. The method of claim 6, wherein the patient information comprises a heart rate.

13. The method of claim 8, wherein the patient information comprises an ECG waveform.

14. The method of claim 6, further comprising:

receiving full disclosure data from the clinical device;

formatting the full disclosure data into a frame event stream, wherein the frame event stream comprises a plurality of frames in chronological order, wherein each of the plurality of frames comprises a time identifier, an incident identifier, and clinical information associated

with a time identified by the time identifier and an incident identified by the incident identifier; and sending the frame event stream over the wireless data connection as the patient information.

15. The method of claim 14, further comprising storing the plurality of frames in a computer readable medium.

16. The method of claim 15, further comprising:

sending a request over the wireless data connection, the request including a particular incident identifier;

retrieving from the computer readable medium and adding to a response set each of the plurality of frames for which the incident identifier corresponds to the particular incident identifier of the request; and

sending the response set over the wireless data connection.

17. The method of claim 16, further comprising displaying at least a portion of the response set in the emergency medical services mobile environment.

18. The method of claim 6, wherein the wireless data connection is a first wireless data connection, the method further comprising:

transmitting the patient information via a second wireless data connection;

receiving the patient information with a personal mobile device via the second wireless data connection;

receiving, via the personal mobile device, a role indication; and

determining a portion of the patient information for display on the mobile device based on the role indication.

19. The method of claim 18, wherein the role indication is CPR medic, and wherein the portion of the patient information comprises chest compression measurement data.

20. The method of claim 18, further comprising:

receiving a patient intervention indication via the second wireless data connection from the personal mobile device.

* * * * *

专利名称(译)	用于EMS设备通信接口的系统和方法		
公开(公告)号	US20170053086A1	公开(公告)日	2017-02-23
申请号	US15/294633	申请日	2016-10-14
[标]申请(专利权)人(译)	卓尔医学产品公司		
申请(专利权)人(译)	ZOLL医疗公司		
当前申请(专利权)人(译)	ZOLL医疗公司		
[标]发明人	MARTIN MICHAEL SCOTT ASHMORE CHAD DEINES ERIC A FREEMAN GARY A HELMICK JOSEPH L KAIB THOMAS E RATTANNI RICHARD A REID C SHANE SOLLER JEREMY RYAN VOLPE SHANE S RUGGIERO GARY GEHEB FREDERICK J		
发明人	MARTIN, MICHAEL SCOTT ASHMORE, CHAD DEINES, ERIC A. FREEMAN, GARY A. HELMICK, JOSEPH L. KAIB, THOMAS E. RATTANNI, RICHARD A. REID, C. SHANE SOLLER, JEREMY RYAN VOLPE, SHANE S. RUGGIERO, GARY GEHEB, FREDERICK J.		
IPC分类号	G06F19/00 A61B5/0402 A61B5/024 G06F17/30 A61B5/00		
CPC分类号	G06F19/3418 G06F19/3406 G06F19/322 G06F17/30569 G06F17/30867 A61B5/6898 A61B5/0006 A61B5/0022 A61B5/024 A61B5/0402 A61B5/747 G06F16/258 G06F16/9535 G16H10/60 G16H40/63 G16H40/67		
优先权	61/322675 2010-04-09 US 61/227187 2009-07-21 US 61/322678 2010-04-09 US		
外部链接	Espacenet USPTO		

摘要(译)

一种用于补充患者监测设备的通信能力的系统，该系统包括设备插槽内的卡配件，并且被配置为经由接口插槽从设备接收患者监测信息;由卡托管并配置为存储患者监测信息的存储器设备;由卡托管的无线收发器;由卡托管的资产管理数据库;处理器，可配置为将患者监测信息格式化为一个或多个帧的流，所述一个或多个帧中的每一个与EMS事件相关联，在此期间患者监测在收集信息之后，处理器还被配置为将一个或多个帧存储到资产管理数据库并且利用无线收发器发送一个或多个帧的流。

