



US 20180317815A1

(19) **United States**(12) **Patent Application Publication****Moore et al.**(10) **Pub. No.: US 2018/0317815 A1**(43) **Pub. Date: Nov. 8, 2018**(54) **REUSABLE RESPIRATORY EFFORT
SENSOR MODULE****Publication Classification**(51) **Int. Cl.***A61B 5/113* (2006.01)*A61B 5/00* (2006.01)*A61B 5/08* (2006.01)(52) **U.S. Cl.**CPC *A61B 5/1135* (2013.01); *A61B 5/4806*(2013.01); *A61B 5/08* (2013.01); *A61B 5/6831*


(2013.01)

(71) Applicant: **Dymedix Corporation**, Shoreview, MN
(US)(72) Inventors: **James P. Moore**, Bloomington, MN
(US); **Alan B. Jones**, Maple Grove,
Minnesota, MN (US); **Todd M. Eiken**,
Lindstrom, MN (US)(21) Appl. No.: **16/027,615**(22) Filed: **Jul. 5, 2018****Related U.S. Application Data**(60) Division of application No. 14/827,676, filed on Aug.
17, 2015, which is a continuation-in-part of applica-
tion No. 14/339,778, filed on Jul. 24, 2014, now
abandoned.

(57)

ABSTRACT

A respiratory effort sensing belt that incorporates a PVDF transducer is constructed such that the transducer is contained within an elastic, moisture impervious plastic envelope and affixed to the envelope are a pair of connectors adapted to receive opposed ends of a body-encircling, single-use band and which provide the ability to adjust belt tension. Because of the construction of the sensor module, it may be sterilized for reuse.

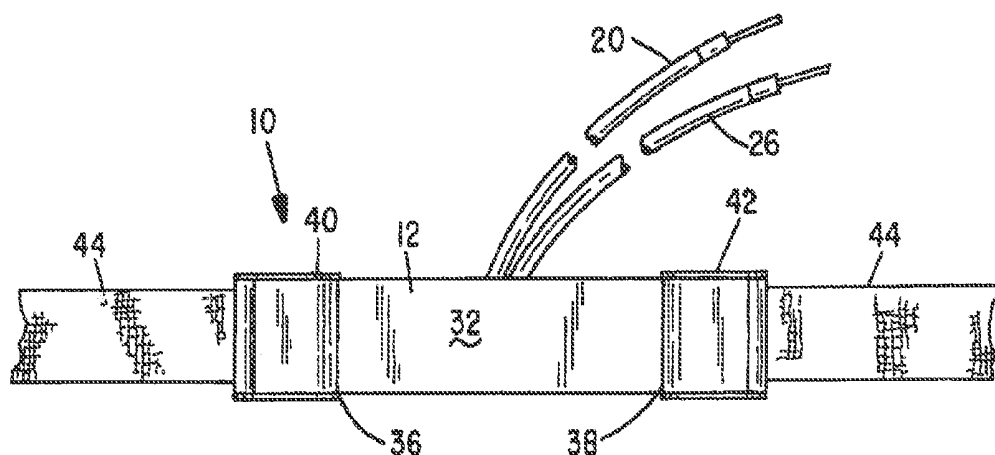

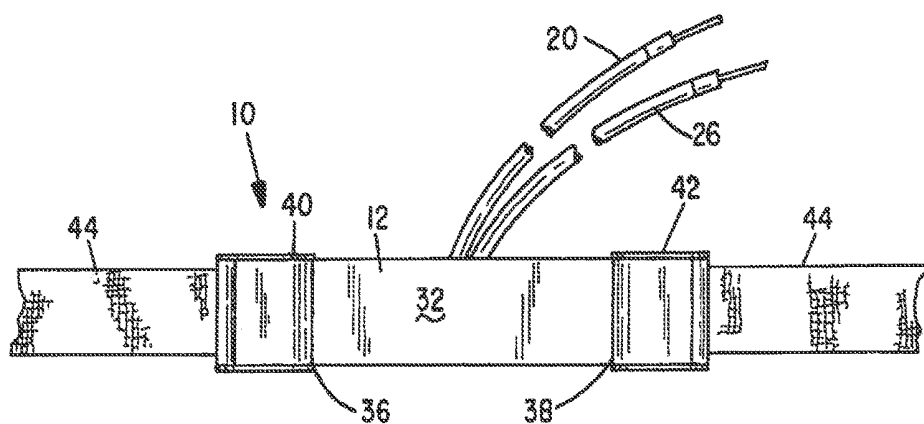


FIG. 1

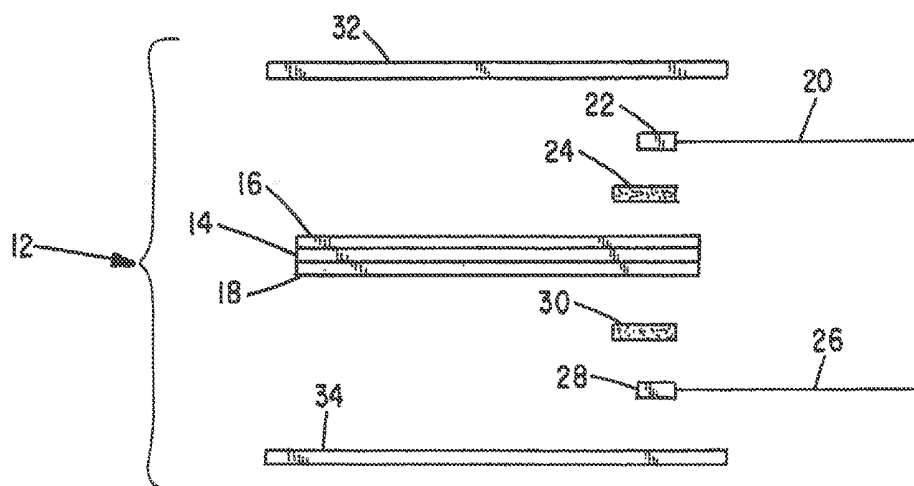


FIG. 2

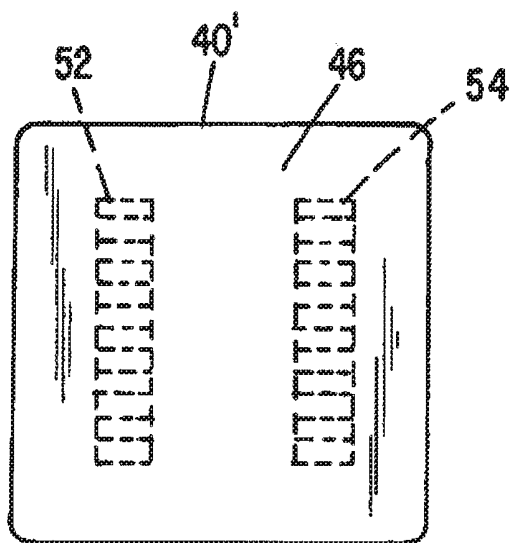


FIG. 3

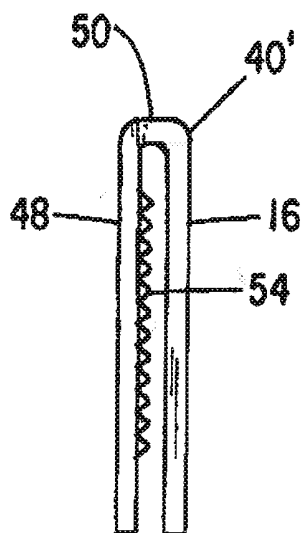


FIG. 4

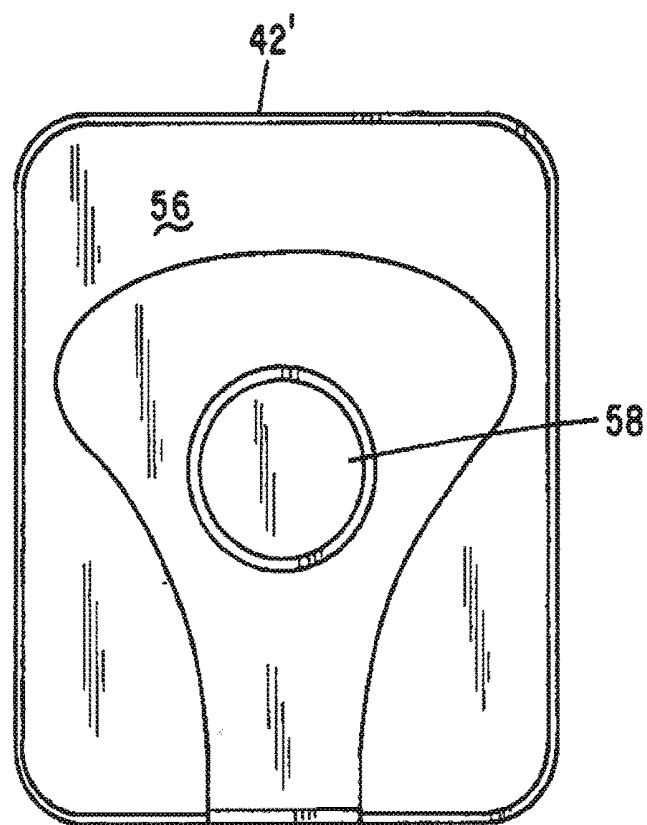


FIG. 5

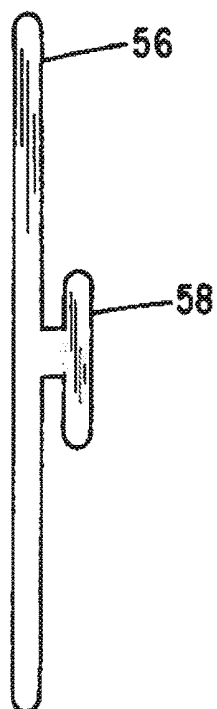


FIG. 6

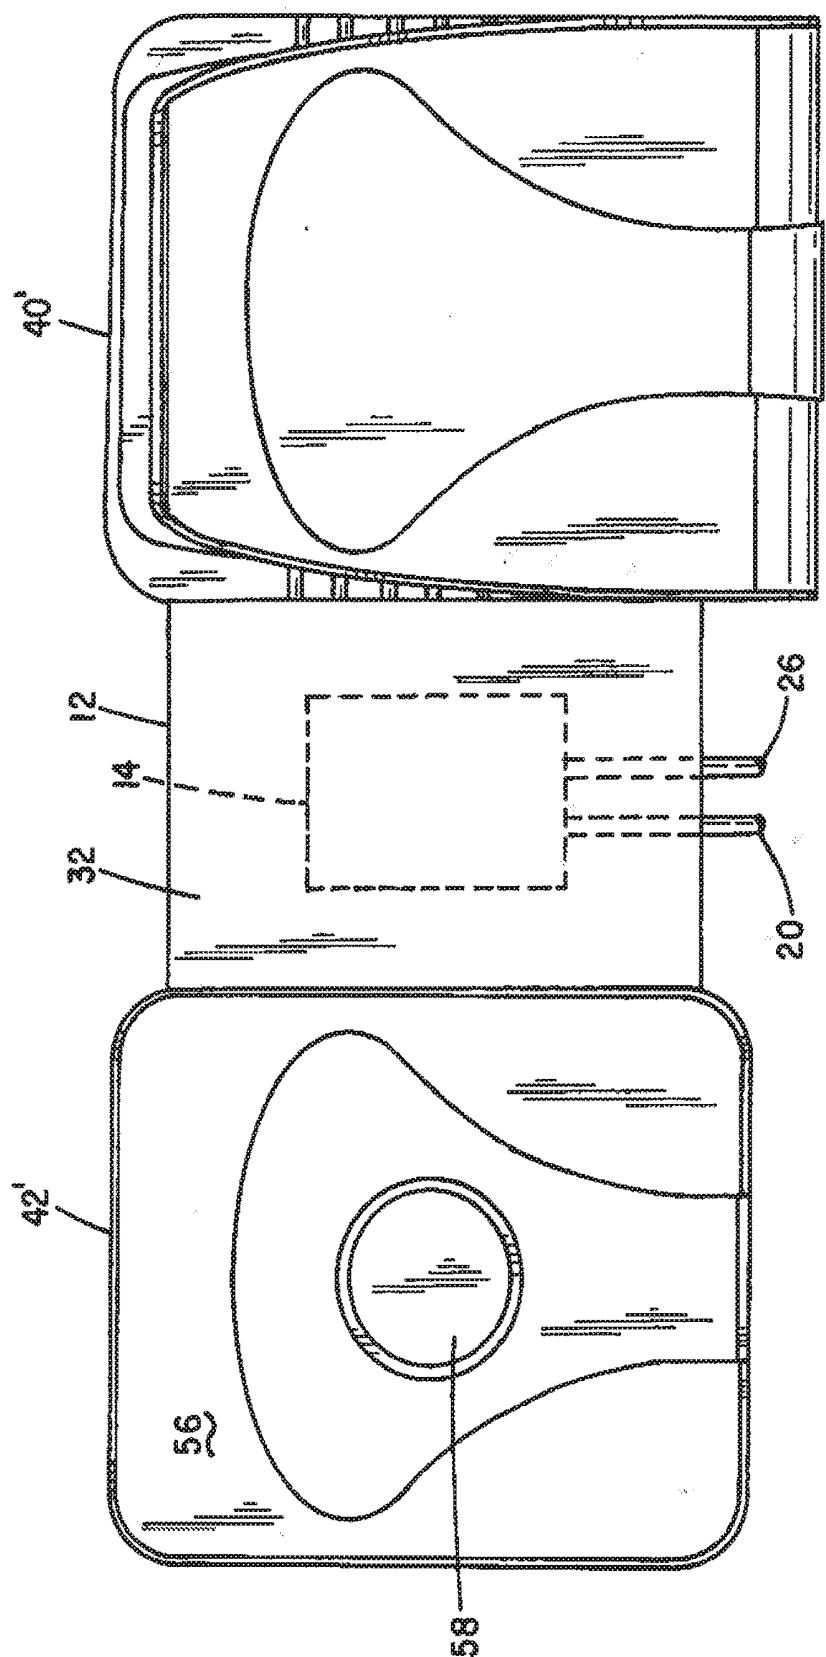


FIG. 7

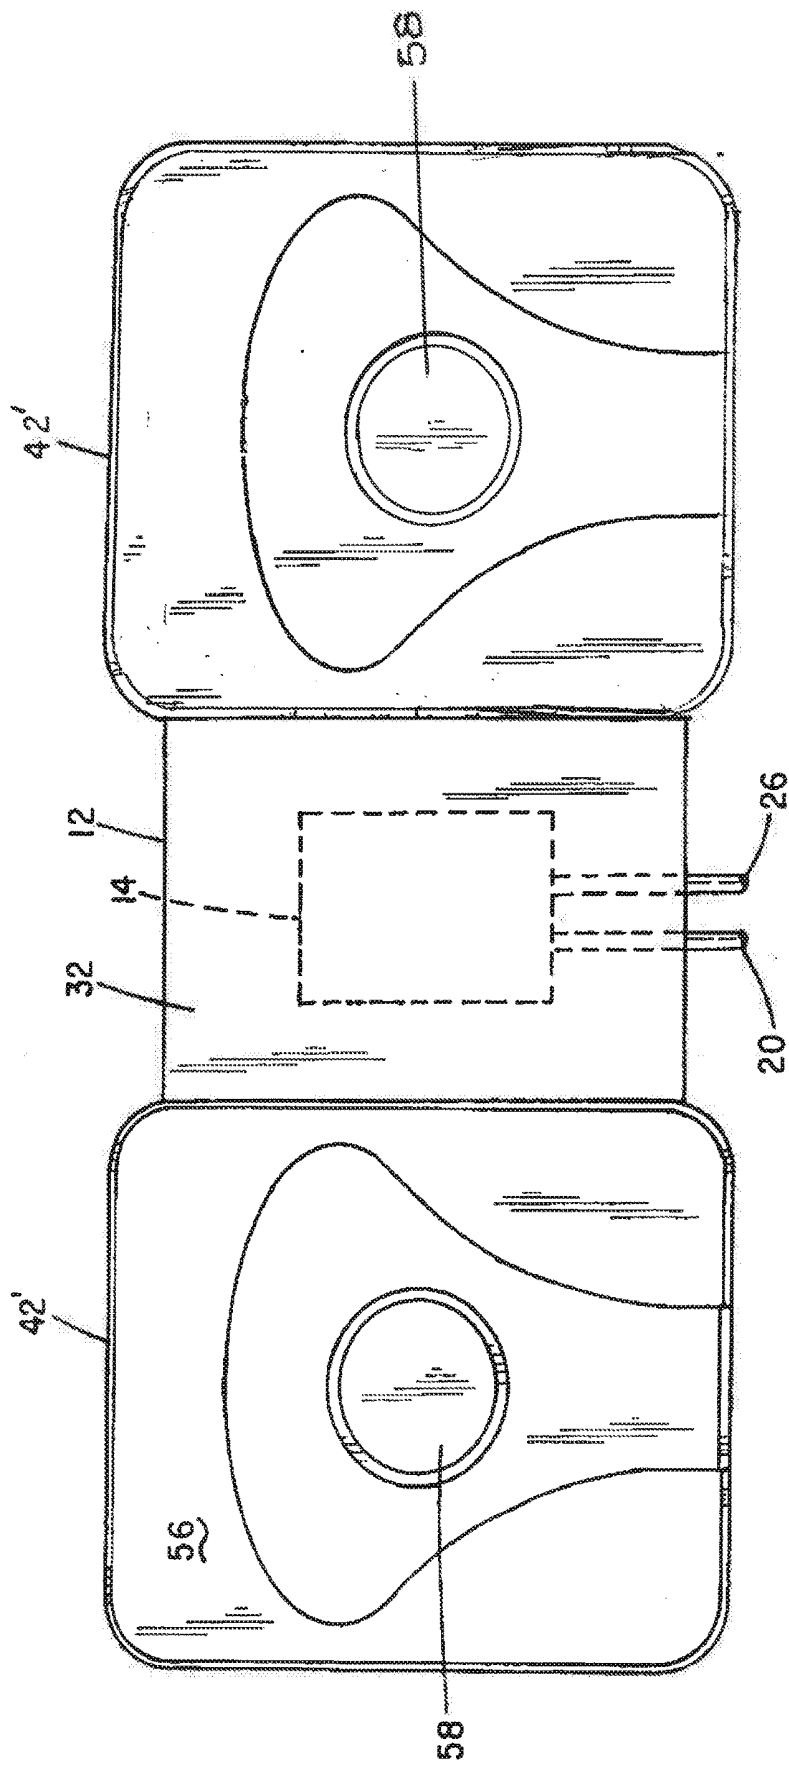


FIG. 8

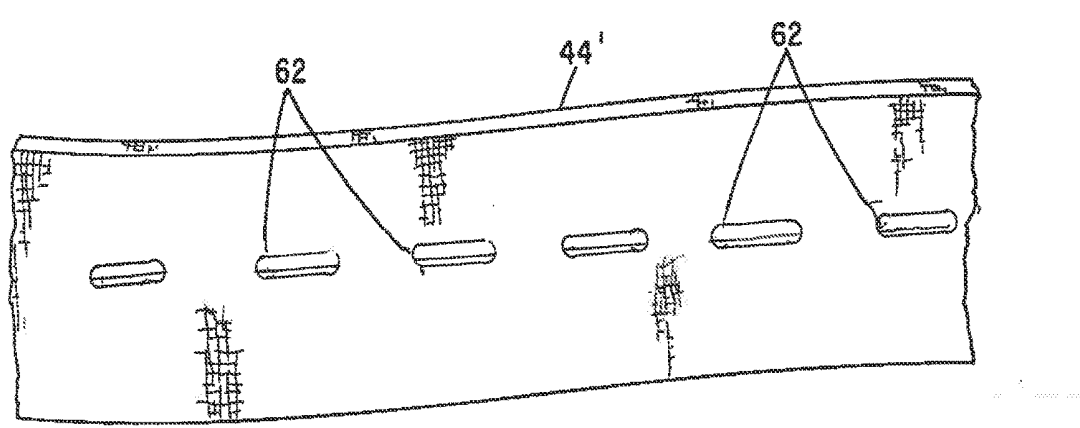


FIG. 9

REUSABLE RESPIRATORY EFFORT SENSOR MODULE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part of application Ser. No. 14/339,778, filed Jul. 24, 2014, entitled REUSABLE RESPIRATORY EFFORT SENSOR MODULE, which is deemed incorporated herein by reference in its entirety.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0002] Not applicable

BACKGROUND OF THE INVENTION

I. Field of the Invention

[0003] This invention relates generally to apparatus for monitoring respiratory activity in the course of a sleep study and more particularly to a respiratory effort sensor designed such that the sensor electronics and associated leads for connecting the electronics to a polysomnograph machine (PSG) or home sleep test (HST) device is adapted for connection to a body-encircling band and remains reusable and only the low-cost, body-encircling band position is disposable following a use thereof.

II. Discussion of the Prior Art

[0004] In published U.S. Application 2008/0275356, there is described a respiratory effort belt that has been marketed by Dymedix Corporation of Shoreview, Minn. for a number of years. It comprises a PVDF film member having first and second metalized major surfaces to which a pair of approximately six foot long tabbed leads is electrically connected. The resulting assembly is permanently affixed to the surface of a body-encircling belt member. Signals are generated when the PVDF film on the belt member is stressed due to stretching as the user breathes in and out. The leads connect to a PSG, allowing the signals to be used in diagnosis and analysis.

[0005] Approximately 95% of the manufacturing cost of the respiratory effort belt resides in its sensor electronics and associated leads while the remaining 5% of the cost resides in the body-encircling belt on which the sensor electronics are affixed.

[0006] For infection control reasons, many sleep labs dispose of the respiratory effort belts after a use on a given patient. It is, of course, advantageous to reduce the cost of the diagnostic procedure and the present invention achieves this desired result.

SUMMARY OF THE INVENTION

[0007] In accordance with the present invention, there is provided a respiratory effort belt comprising a PVDF film strip having a layer of metallization on opposed major surfaces thereof. First and second insulated conductive leads, each with first and second ends, have the first end of the first lead electrically connected to the layer of metallization on one of the opposed major surfaces and the second lead electrically connected to the layer of metallization on another of the opposed major surfaces. A flexible, elastic,

moisture impervious, generally rectangular envelope is made to contain the metalized PVDF film strip and only a distal end portion of the first and second conductive leads. A pair of connectors is releasably attached individually to the first and second ends of the envelope. A disposable elastic or inelastic band, whose length is sufficient to encircle a human's torso, is adapted to be selectively joined and released to and from the pair of connectors. This allows the band to be disposed of after use while the envelope, with its connectors and containing the sensor element and leads, remains reusable following sterilization.

DESCRIPTION OF THE DRAWINGS

[0008] The foregoing features, objects and advantages of the invention will become apparent to those skilled in the art from the following detailed description of a preferred embodiment, especially when considered in conjunction with the accompanying drawings in which like numerals in the several views refer to corresponding parts.

[0009] FIG. 1 is a partial frontal view of a respiratory effort belt comprising a preferred embodiment of the present invention;

[0010] FIG. 2 is an exploded view of the reusable sensor module;

[0011] FIG. 3 is a front plan view of an alternative connector attachable to a first end of a sensor module;

[0012] FIG. 4 is a side view of the connector of FIG. 3;

[0013] FIG. 5 is a front plan view of an alternative connector attachable to a second end of the sensor module;

[0014] FIG. 6 is a side view of the connector of FIG. 5;

[0015] FIG. 7 is a front view of a sensor module with the connectors of FIGS. 3 and 5 joined thereto;

[0016] FIG. 8 is a front view of a sensor module having two connectors like those of FIGS. 5 and 6; and

[0017] FIG. 9 is a view of a belt used with the sensor module of FIG. 7.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0018] This description of the preferred embodiments is intended to be read in connection with the accompanying drawings, which are to be considered part of the entire written description of this invention. In the description, relative terms such as "lower", "upper", "horizontal", "vertical", "above", "below", "up", "down", "top" and "bottom" as well as derivatives thereof (e.g., "horizontally", "downwardly", "upwardly", etc.) should be construed to refer to the orientation as then described or as shown in the drawings under discussion. These relative terms are for convenience of description and do not require that the apparatus be constructed or operated in a particular orientation. Terms such as "connected", "connecting", "attached", "attaching", "join" and "joining" are used interchangeably and refer to one structure or surface being secured to another structure or surface or integrally fabricated in one piece, unless expressly described otherwise.

[0019] Referring first to FIG. 1, there is indicated generally by numeral 10 a respiratory effort belt constructed in accordance with the present invention. It is seen to comprise a reusable, sterilizable sensor module 12, the construction of which is best illustrated in the exploded view of FIG. 2. In FIG. 2, a strip of polyvinylidene fluoride (PVDF) is identified by numeral 14. The strip is generally rectangular and

deposited on the opposed major surfaces thereof are metallization layers 16 and 18. An electrical lead 20 has a conductive terminal pad 22 bonded to the metallization layer 16 by a conductive adhesive member 24. Likewise, an electrical lead 26 has its conductive terminal pad 28 conductively affixed to the metallization layer 18 by means of a conductive adhesive layer 30.

[0020] The PVDF film 14, as well as distal end portions of the leads 20 and 26, is contained within a moisture impervious plastic envelope comprising elastic polymer layers 32 and 34 that are laminated together about the perimeters thereof to form the envelope.

[0021] Without limitation, the resulting module 12 may be about 5 inches in length and about 1½ inches in width.

[0022] Referring again to FIG. 1, affixed to the end portions 36 and 38 of the envelope comprising the module 12 are connectors 40 and 42 that are used to releasably couple the module 12 to a body-encircling band 44. Without limitation, the connectors 40 and 42 preferably comprise cam buckles, many types of which are commercially available. Such cam buckles releasably clamp to the opposed ends 36 and 38 of the envelope comprising the module 12 and permit adjustment of the body-encircling band 44 to a desired degree of snugness.

[0023] It is contemplated that the body-encircling band 44 be of an inexpensive cloth fabric that is somewhat elastic.

[0024] In use, the respiratory effort belt 10 will be placed about a patient's torso, either about the chest or abdomen, and any slack taken up by tensioning the band with the cam buckle 40 or 42 open and when the tension is deemed appropriate, the cam lever is released, locking the band 44 from moving relative to the module 12. As the subject breathes, the envelope comprising the sensor module 12, being elastic, will stretch upon inspiration and shrink during expiration. This places corresponding stresses on the PVDF film element 14 thereby producing, via the piezoelectric effect, electrical output signals on the leads 20 and 26.

[0025] Upon completion of a patient's sleep study, the body-encircling band 44 can be separated from the buckles 40 and 42 and properly disposed of. The module 12, however, can be retained for reuse following sterilization and/or cleaning and only the relatively inexpensive band 44 needs replacement. In that the great majority of the cost resides in the module 12 and because this module is reusable, a substantial savings results for the consumer who need only replace the fabric belt 44 and not the entire respiratory effort belt each time the belt is used.

[0026] FIGS. 3 and 4 illustrate an alternative connector construction 40' adapted to be attached to a first end of the sensor module 12. It is seen to comprise a molded plastic piece having generally planar front and rear surfaces 46 and 48 joined together at an upper end 50 to form a U-shaped cross section. Integrally molded on the inner side of the rear surface 48 are first and second rows of teeth 52 and 54. The upper end 50 is flexible such that front surface 46 can be squeezed against the rows of teeth 52 and 54 to engage the teeth with the belt fabric.

[0027] FIGS. 5 and 6 illustrate an alternative connector construction 42' adapted to be attached to a second end of the sensor module 12. It is seen to comprise a molded, plastic, rectangular and generally planar sheet 56 and having an integrally molded and rounded button member 58 joined to a central portion of the sheet 56 and projecting outwardly therefrom. FIG. 7 shows the reusable PVDF sensor module

12 permanently joined to the connectors 40' and 42'. More particularly, the envelope 32 containing the PVDF film 14 is adhesively or otherwise bonded to back surfaces of the connectors 40' and 42'.

[0028] FIG. 8 illustrates yet another reusable sensor module embodiment which two of the connectors of FIGS. 5 and 6 are utilized. The moisture impervious envelope 32 containing the PVDF transducer 14 is permanently bonded to the connectors 42', one on each end thereof.

[0029] FIG. 9 illustrates the body encircling flexible, disposable, elastic fabric belt 44'. It is seen to include a series of regularly, longitudinally spaced buttonhole slits 62 formed through its thickness.

[0030] In use with the embodiment of FIG. 7, one end of the belt 44' will be inserted into the gap of the U-shaped connector 40' and by squeezing the surface 46 relative to surface 48, the rows of teeth 52, 54 will penetrate into the belt material and be releasably secured to one end thereof. The belt 44' will then be deployed from a supply roll thereof and wrapped about the torso of the patient and when snug, the button member 58 of connector 42' will be made to pass through a nearby one of the buttonholes 62 in the fabric belt 44' to secure the belt to the sensor module 12. The excess belt material still on the roll can now be cut free of the deployed sensor belt. Any further needed adjustment can be made by repositioning the belt on the teeth of the connector 40'.

[0031] With the embodiment of FIG. 8, a free end of the belt material of FIG. 9 is affixed to the button 58 of one of the connectors 42' and as the belt material is dispensed from a roll thereof, it is wrapped above the subject and when snug, is fitted onto one button 58 of the other connector 42' and then cut off from the roll of belt material.

[0032] This invention has been described herein in considerable detail in order to comply with the patent statutes and to provide those skilled in the art with the information needed to apply the novel principles and to construct and use such specialized components as are required. However, it is to be understood that the invention can be carried out by specifically different equipment and devices. Also, various modifications, both as to the equipment and operating procedures, can be accomplished without departing from the scope of the invention itself.

What is claimed is:

1-7. (canceled)

8. A method for formation of a respiratory effort belt to match a patient in a sleep lab setting comprising the steps of:

- (a) providing a supply roll of webbing material of a predetermined width, the webbing material having a plurality of apertures formed therethrough at regularly spaced intervals along a length dimension of the webbing material comprising the roll;
- (b) providing a reusable sensor module comprising polyvinylidene fluoride (PVDF) film strip having a layer of metallization on opposed major surfaces thereof and first and second insulated leads, each with first and second ends, where the first end of the first lead is electrically connected to the layer of metallization on one of the opposed major surfaces and the first end of the second lead is electrically connected to the layer of material on another of the opposed major surfaces, with the metallized PVDF film and a portion of the first and second leads enclosed in a moisture impervious elastomeric envelope;

- (c) providing a pair of connectors adapted to be releasably attached to opposed ends of the elastomeric envelope, said connectors having a flat abutment surface and a button member projecting outward from the abutment surface, the button shaped to pass through a selected one of the plurality of apertures formed through the webbing material;
- (d) cutting a length of the webbing material from the roll sufficient to span the waist or chest of a particular patient;
- (e) affixing the pair of connectors to opposed ends of the elastomeric envelope;
- (f) extending the button on at least one of the pair of connectors through a selected one of the plurality of apertures on the cut length of webbing material; and
- (g) removing the envelope containing the sensor module and the pair of connectors from the length of webbing material obtained in step (d) following a single use of the respiratory effort belt on a patient.

* * * * *

专利名称(译)	可重复使用的呼吸努力传感器模块		
公开(公告)号	US20180317815A1	公开(公告)日	2018-11-08
申请号	US16/027615	申请日	2018-07-05
[标]申请(专利权)人(译)	DYMEDIX		
申请(专利权)人(译)	DYMEDIX CORPORATION		
当前申请(专利权)人(译)	DYMEDIX CORPORATION		
[标]发明人	MOORE JAMES P JONES ALAN B EIKEN TODD M		
发明人	MOORE, JAMES P. JONES, ALAN B. EIKEN, TODD M.		
IPC分类号	A61B5/113 A61B5/00 A61B5/08		
CPC分类号	A61B5/4806 A61B5/6831 A61B5/1135 A61B5/08		
外部链接	Espacenet USPTO		

摘要(译)

包含PVDF换能器的呼吸努力感应带被构造使得换能器包含在弹性的，不透水的塑料外壳内并且固定到外壳上的是一对适于接收身体环绕的相对端的连接器，一次性使用带和它提供调整皮带张力的能力。由于传感器模块的结构，它可以被消毒以便重复使用。

