



US009259159B2

(12) **United States Patent**
Tsuboi et al.

(10) **Patent No.:** **US 9,259,159 B2**
(45) **Date of Patent:** **Feb. 16, 2016**

(54) **INFORMATION PROCESSING APPARATUS,
INFORMATION PROCESSING METHOD,
AND COMPUTER PROGRAM FOR
MEASURING EARDRUM TEMPERATURE**

(58) **Field of Classification Search**

CPC A61B 5/0059; A61B 5/01; A61B 5/6817;
G01J 5/0011; G01J 5/049; G01J 5/089;
G01J 5/0896

See application file for complete search history.

(71) Applicant: **Sony Corporation**, Tokyo (JP)

(56) **References Cited**

(72) Inventors: **Toshimitsu Tsuboi**, Tokyo (JP);
Akichika Tanaka, Chiba (JP); **Takeshi
Asakawa**, Chiba (JP); **Naoya Sazuka**,
Tokyo (JP); **Seiji Wada**, Kanagawa (JP)

U.S. PATENT DOCUMENTS

6,832,989	B2	12/2004	Sato et al.	
7,108,419	B2 *	9/2006	Harr	374/121
7,369,686	B2	5/2008	Yokono et al.	
7,574,037	B2	8/2009	Hidai et al.	
RE43,873	E	12/2012	Hidai et al.	
2003/0067957	A1 *	4/2003	Ko et al.	374/130
2004/0225207	A1 *	11/2004	Bae et al.	600/340
2009/0124873	A1 *	5/2009	Uchida	600/310

(73) Assignee: **SONY CORPORATION**, Tokyo (JP)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 212 days.

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **13/847,113**

JP	2671946	B2	11/1997
JP	11-028194	A	2/1999
JP	2002-340681	A	11/2002
JP	2005-157679	A	6/2005
JP	3896807	B2	3/2007
JP	4333364	B2	9/2009
JP	4517633	B2	8/2010

(22) Filed: **Mar. 19, 2013**

(65) **Prior Publication Data**

US 2013/0296685 A1 Nov. 7, 2013

* cited by examiner

(30) **Foreign Application Priority Data**

Mar. 29, 2012 (JP) 2012-076046

Primary Examiner — Ruth S Smith

(74) Attorney, Agent, or Firm — Hazuki International, LLC

(51) **Int. Cl.**

A61B 5/01	(2006.01)
A61B 5/00	(2006.01)
G01J 5/08	(2006.01)
G01J 5/04	(2006.01)
G01J 5/00	(2006.01)

(52) **U.S. Cl.**

CPC **A61B 5/01** (2013.01); **A61B 5/0059**
(2013.01); **A61B 5/6817** (2013.01); **G01J**
5/0011 (2013.01); **G01J 5/049** (2013.01); **G01J**
5/089 (2013.01); **G01J 5/0896** (2013.01)

(57) **ABSTRACT**

There is provided an information processing apparatus including an eardrum recognition unit configured to recognize a position of an eardrum based on image information regarding the eardrum, a temperature measurement unit configured to acquire a temperature within an external ear canal including the eardrum, and a temperature processing unit configured to determine a temperature of the eardrum based on a recognition result of the eardrum recognition unit and a measured temperature of the temperature measurement unit.

11 Claims, 21 Drawing Sheets

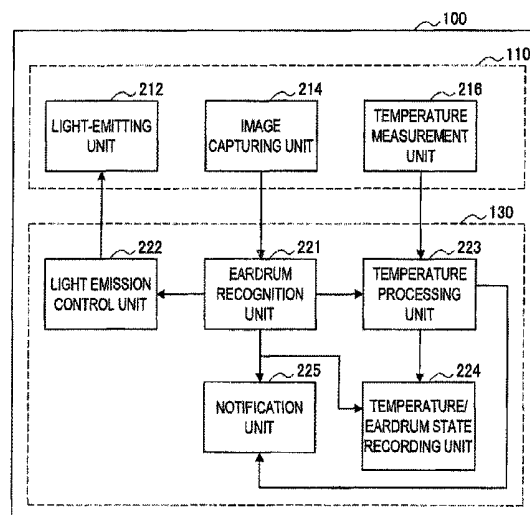


FIG. 1

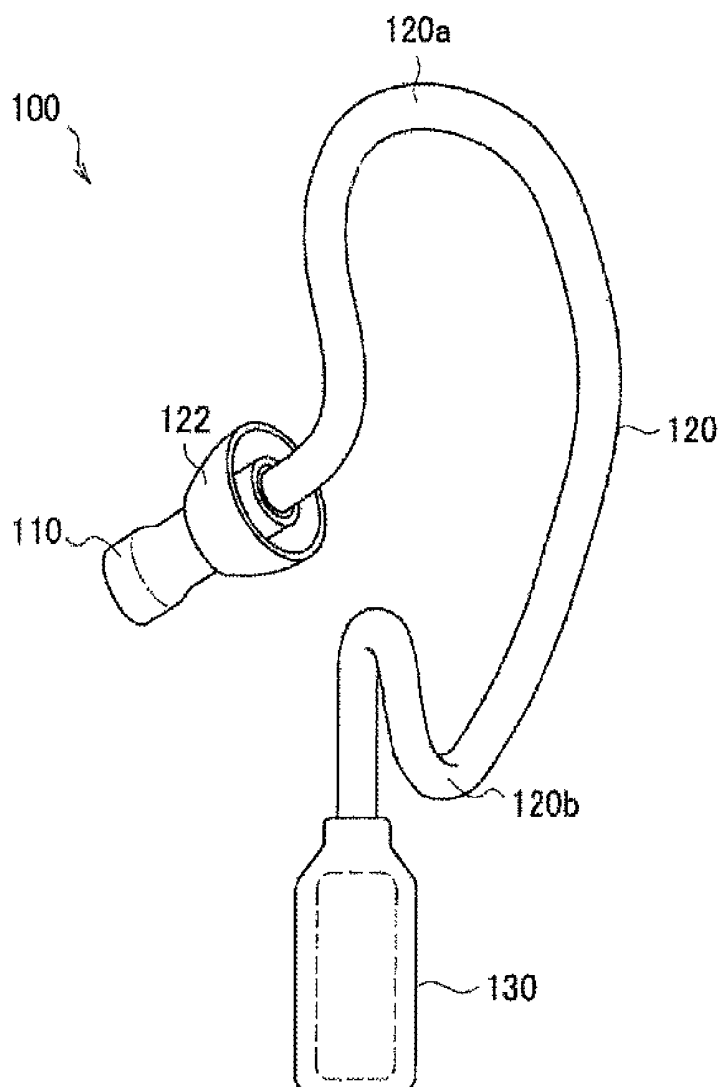


FIG. 2

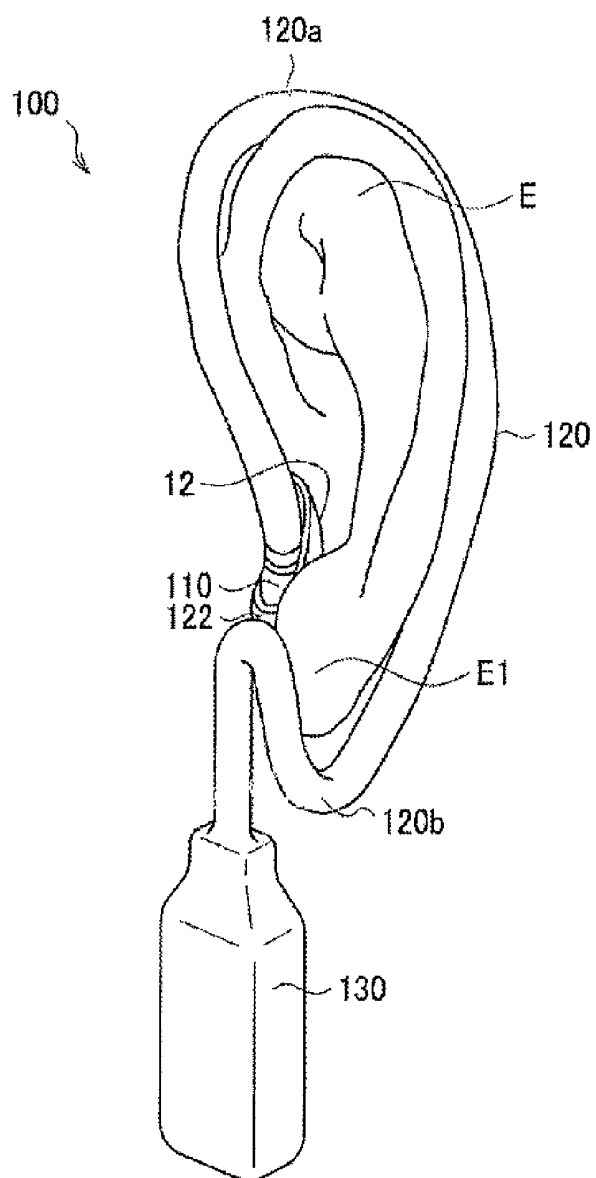


FIG. 3

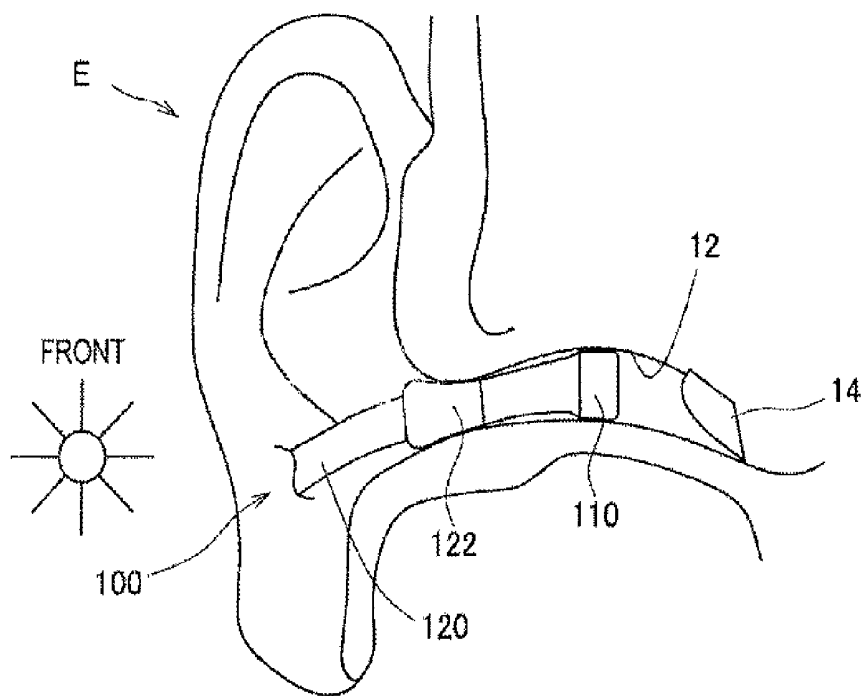


FIG. 4

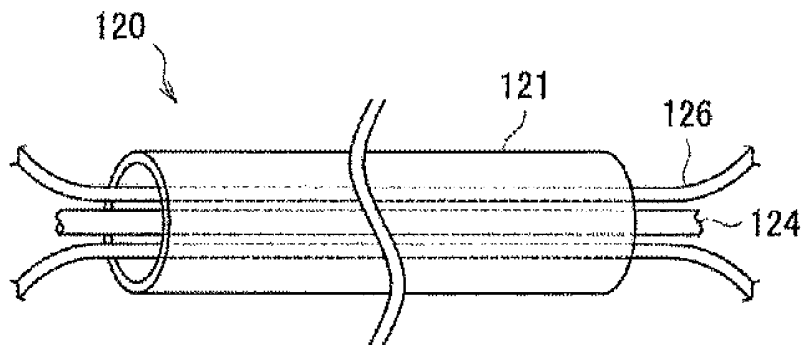


FIG. 5

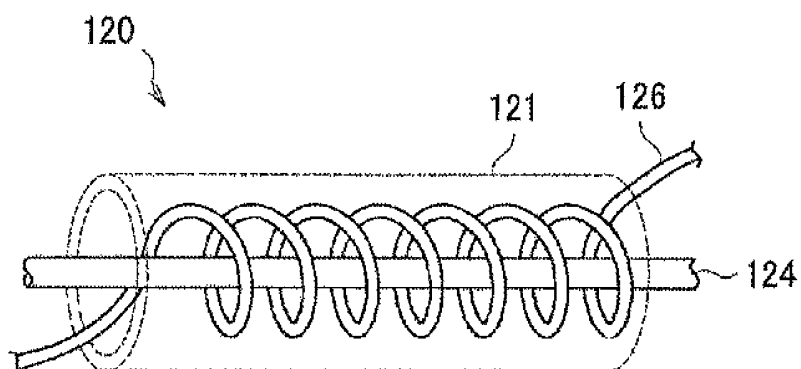


FIG. 6

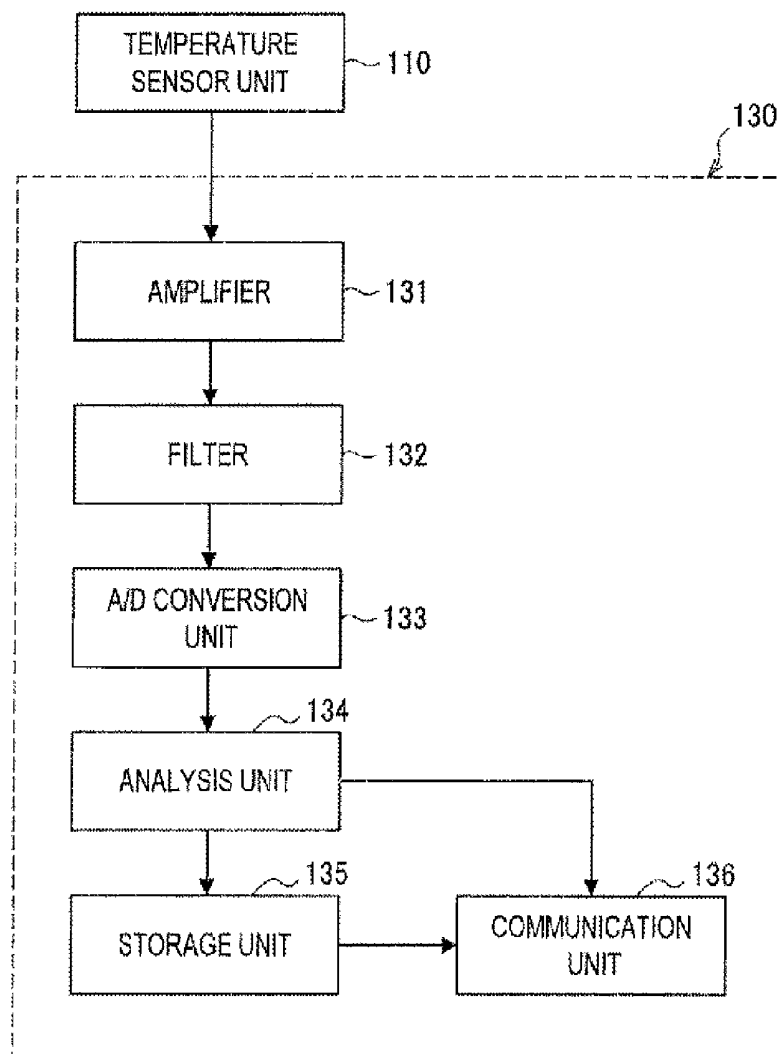


FIG. 7

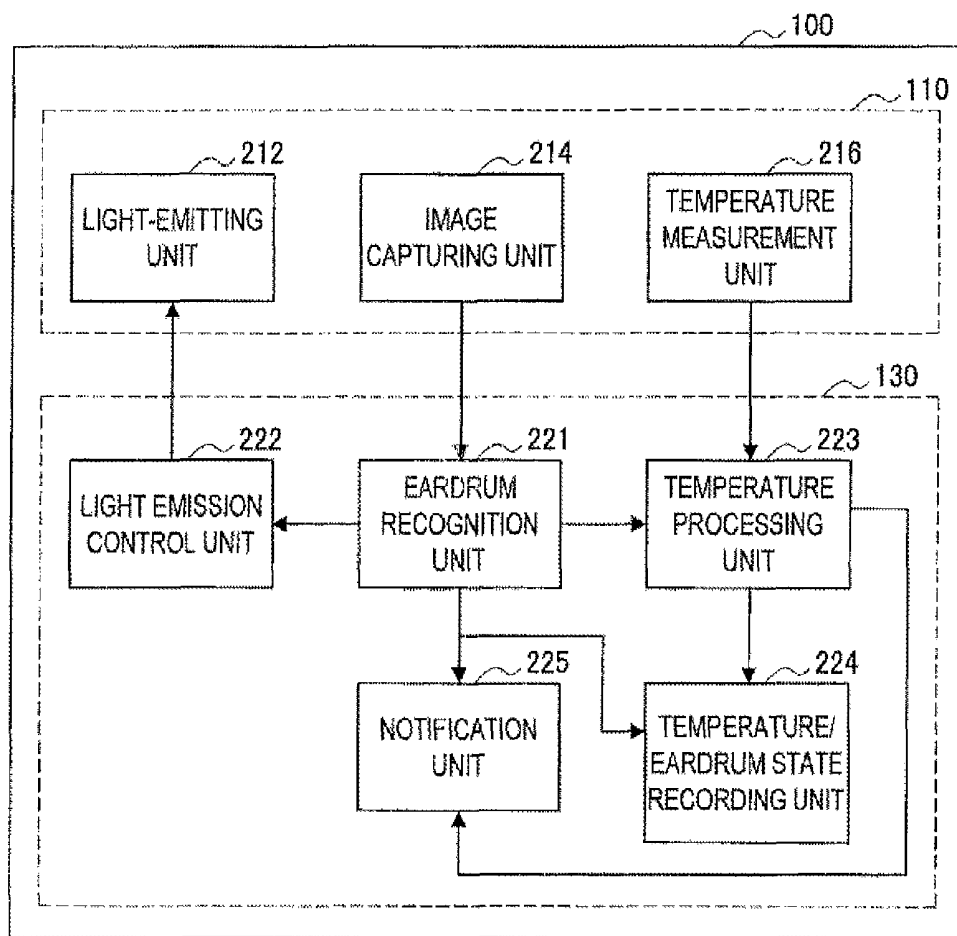


FIG. 8

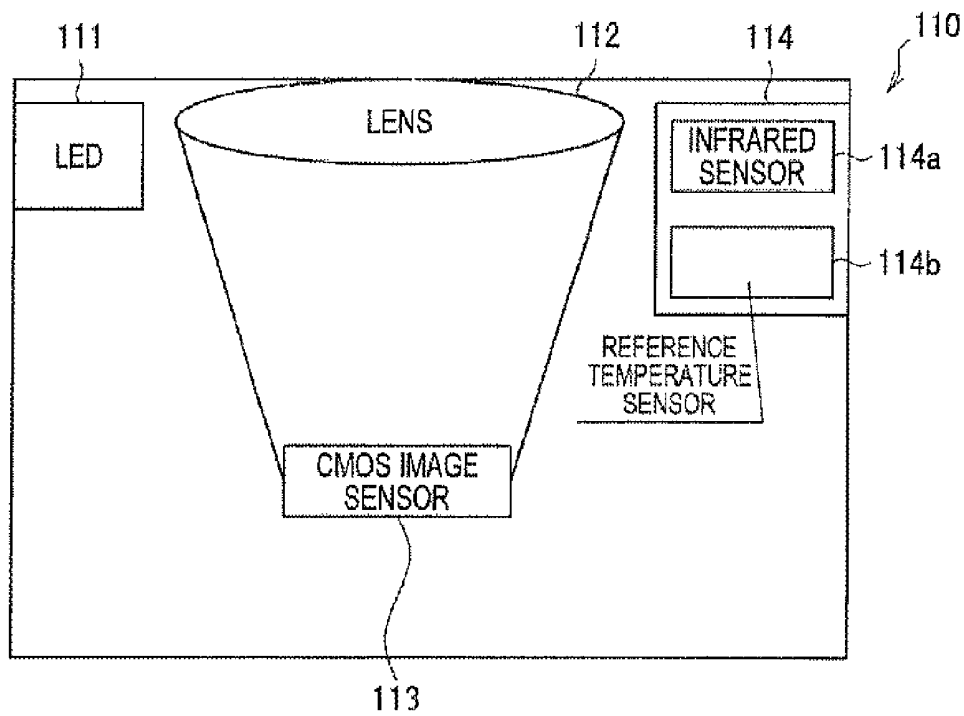


FIG. 9

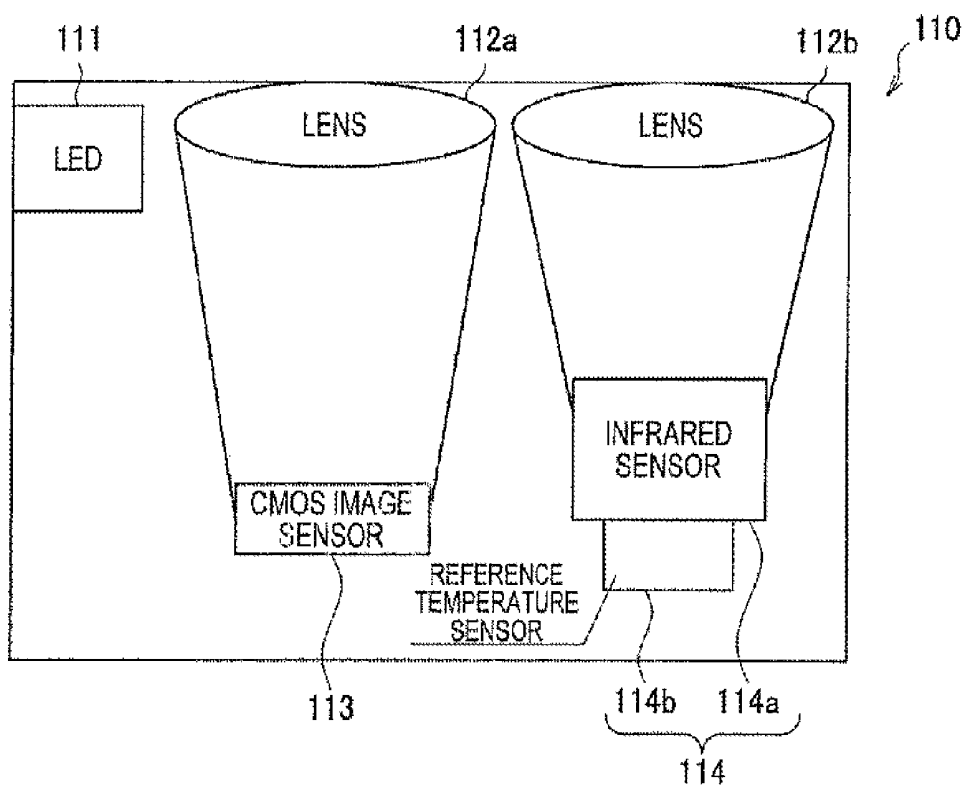


FIG. 10

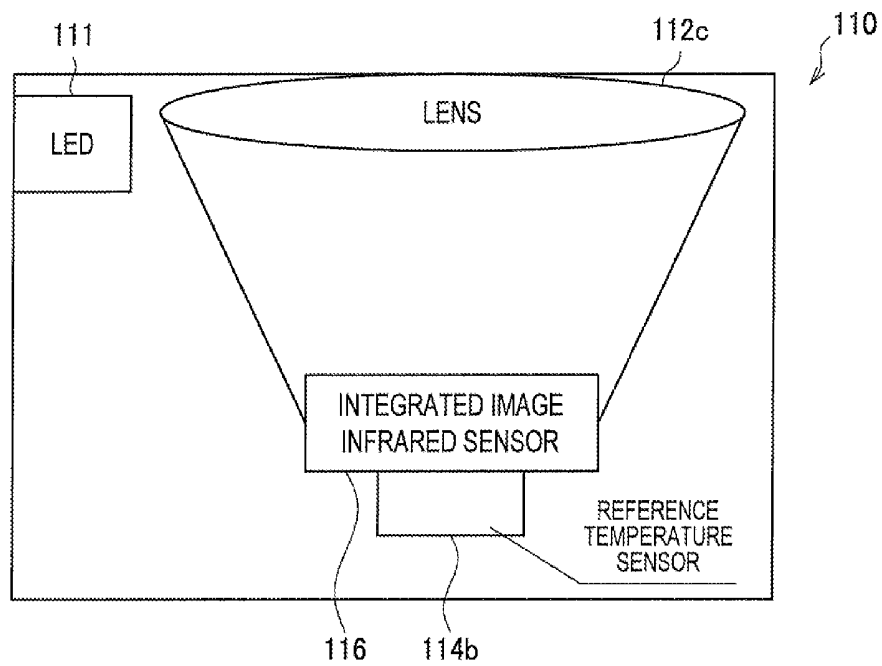


FIG. 11

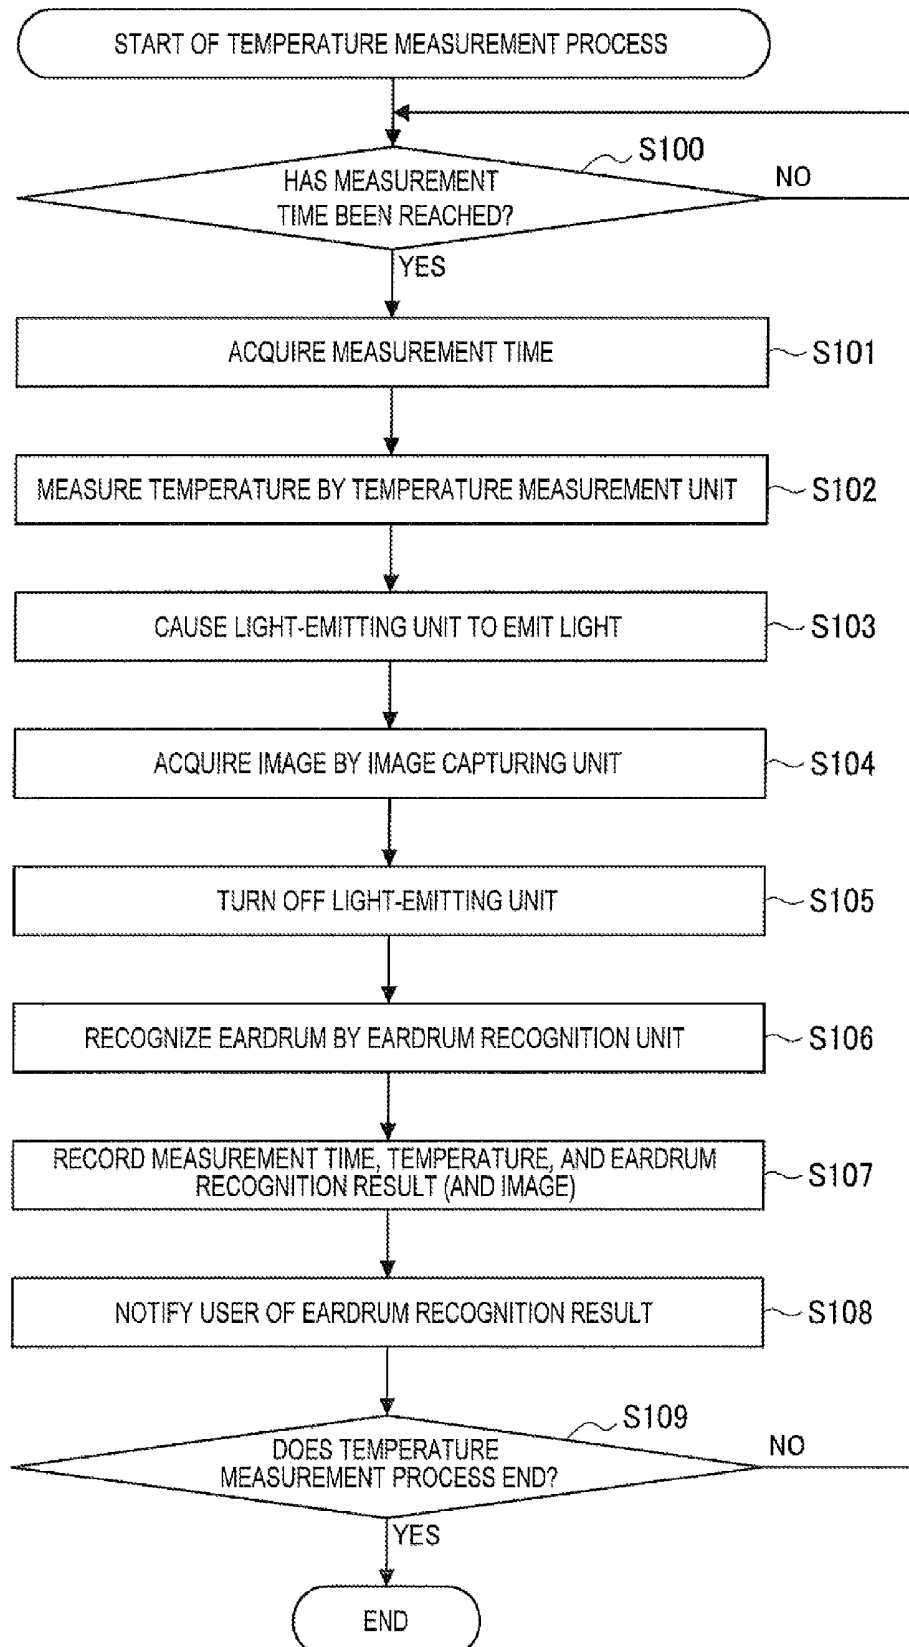


FIG. 12

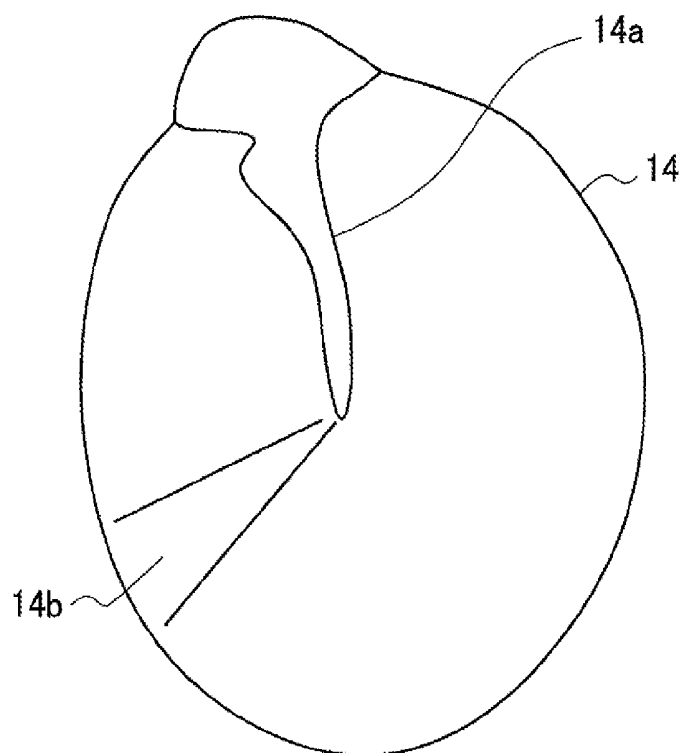


FIG. 13

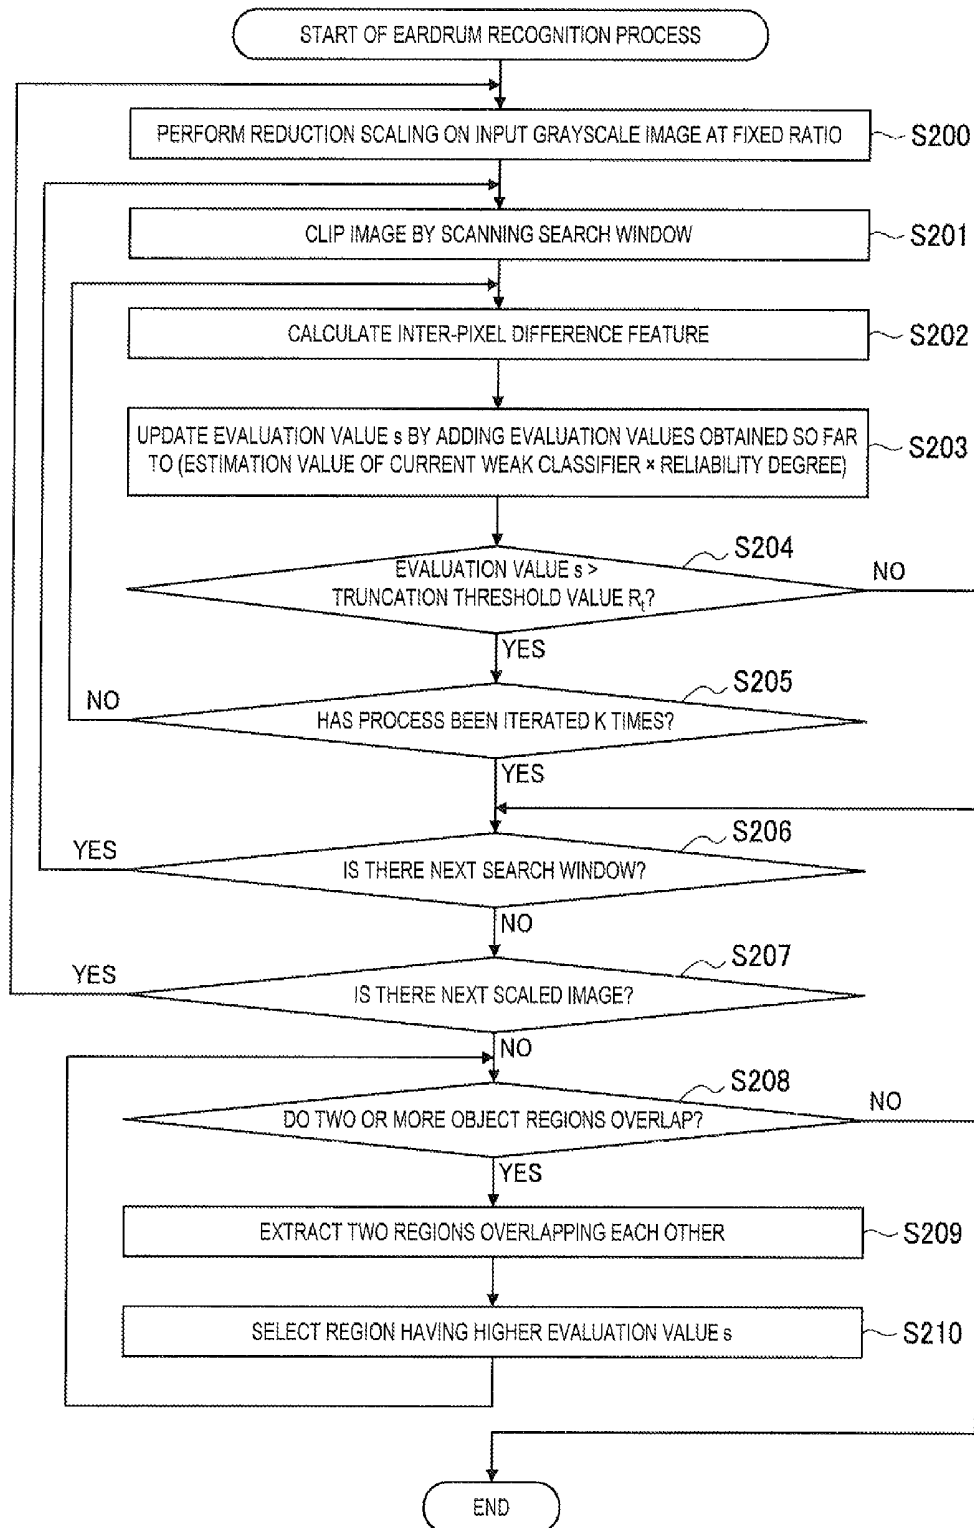


FIG. 14

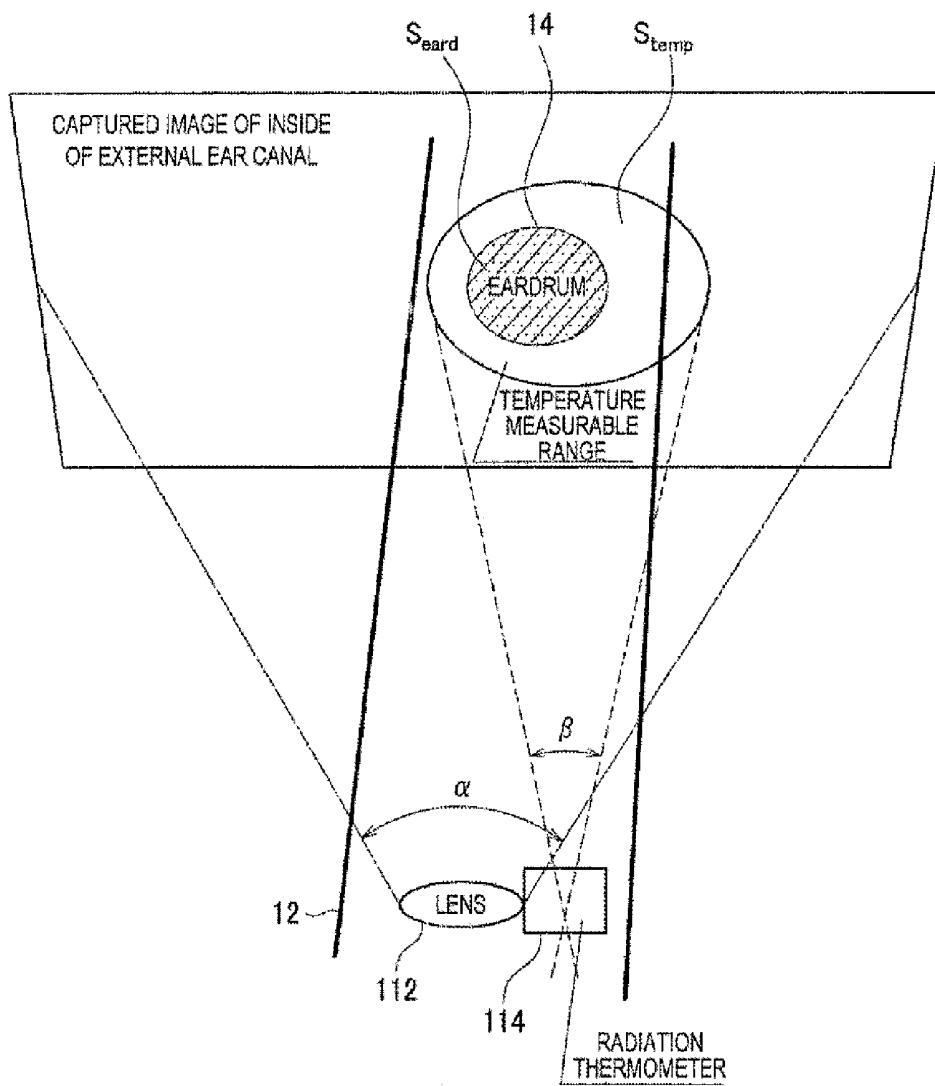


FIG. 15

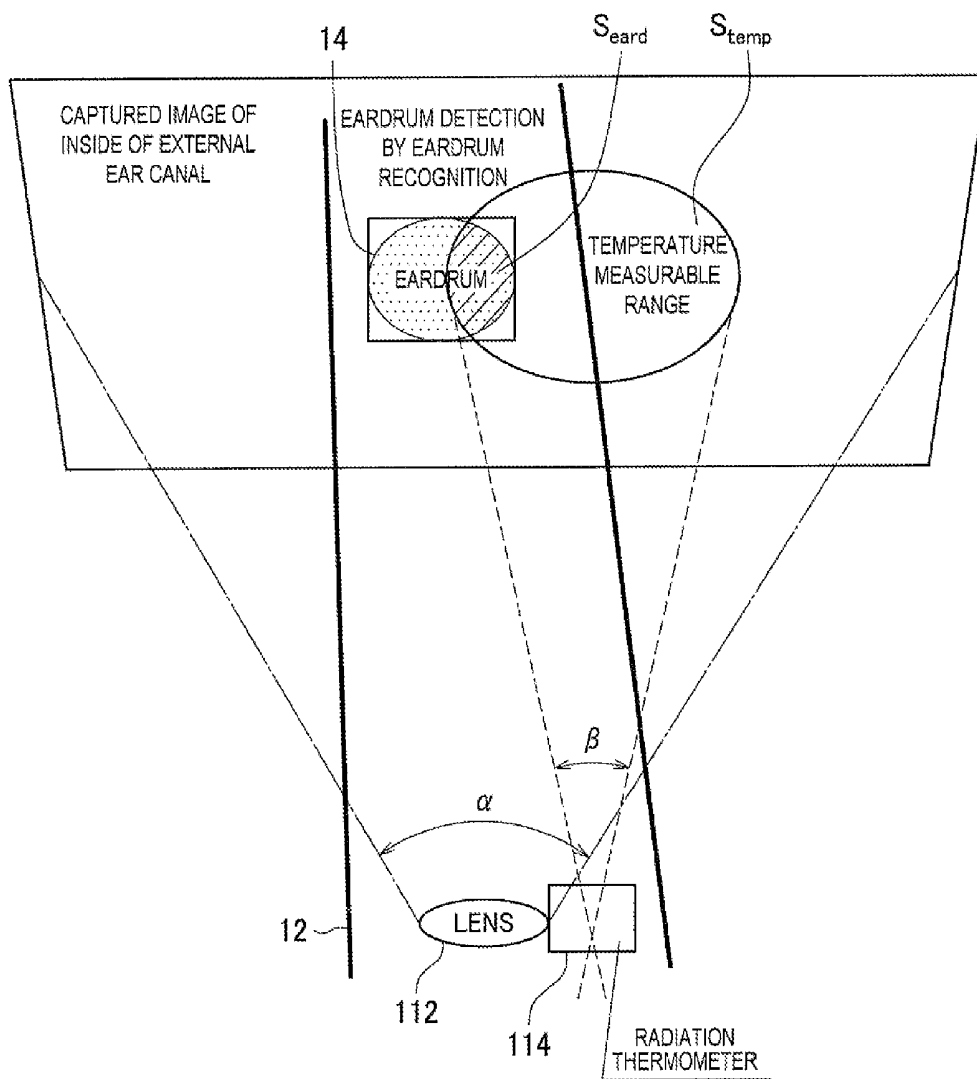


FIG. 16

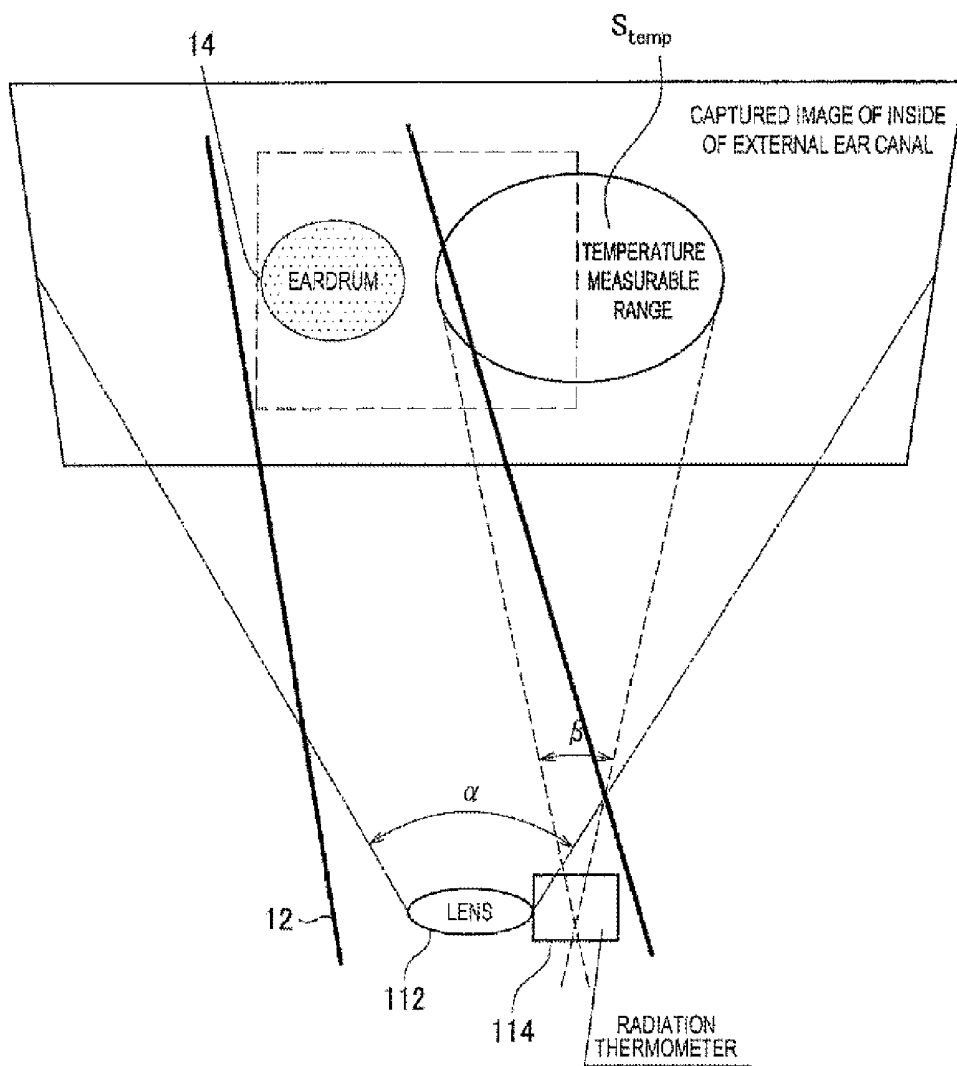


FIG. 17

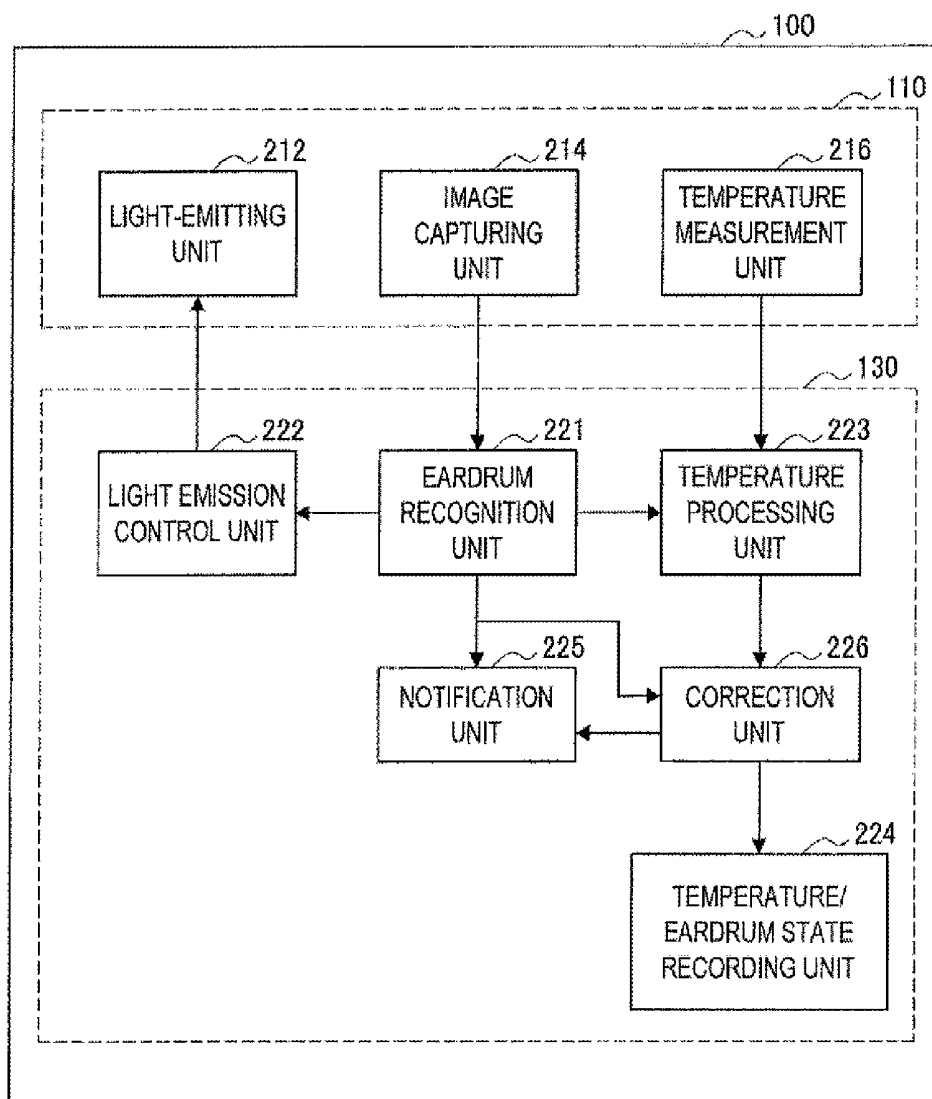


FIG. 18

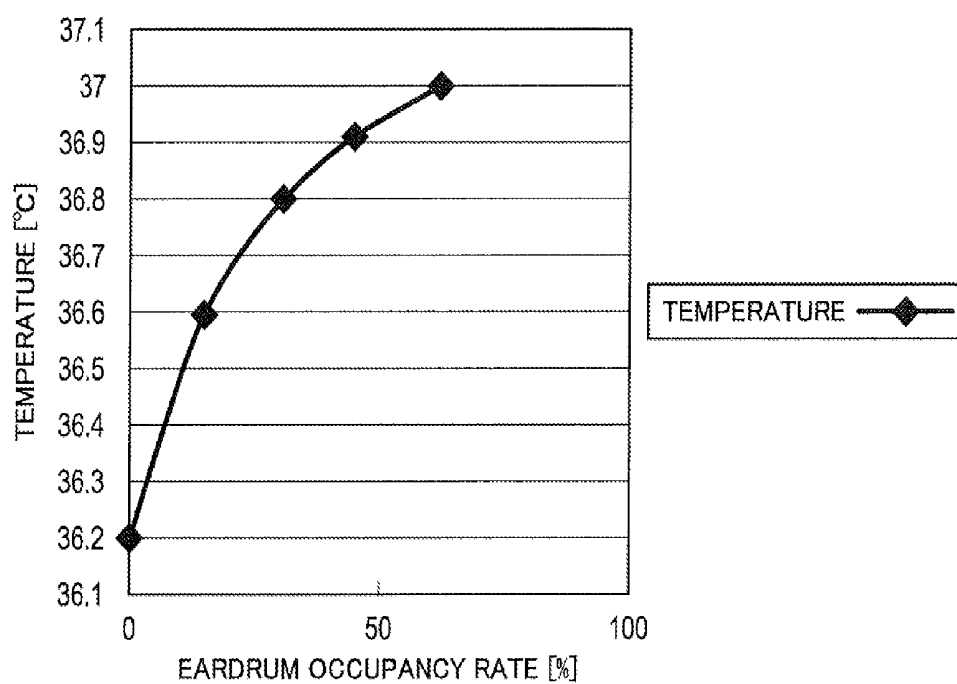


FIG. 19

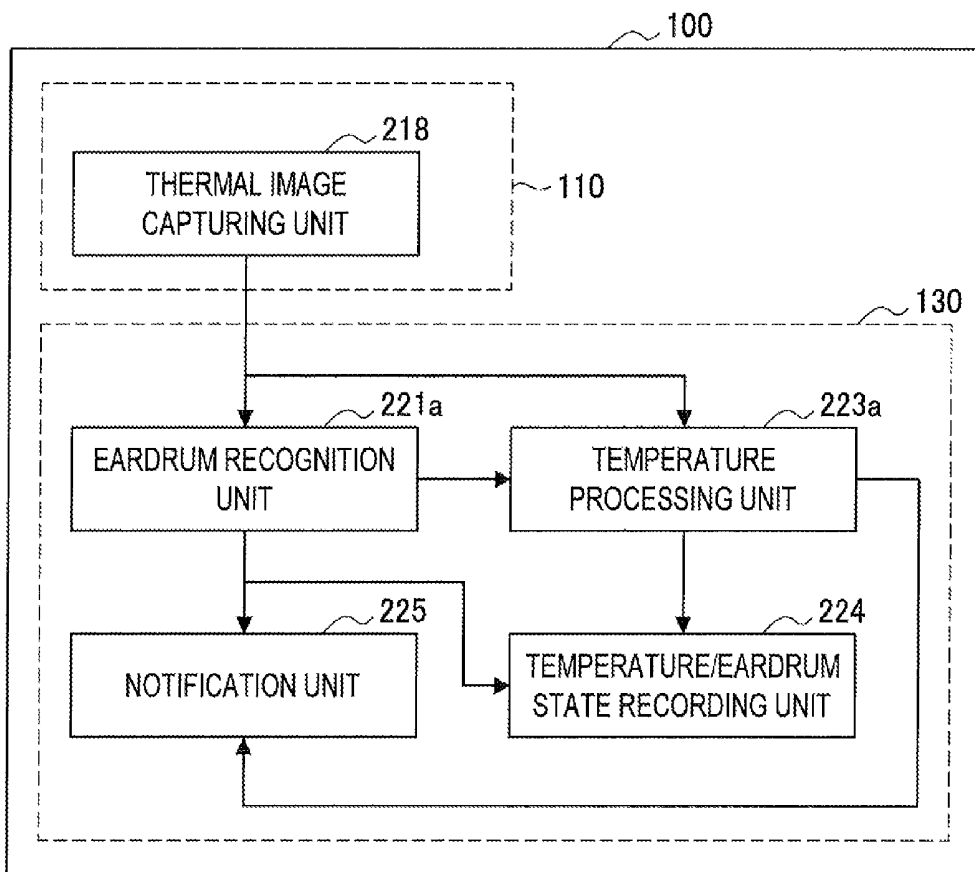


FIG. 20

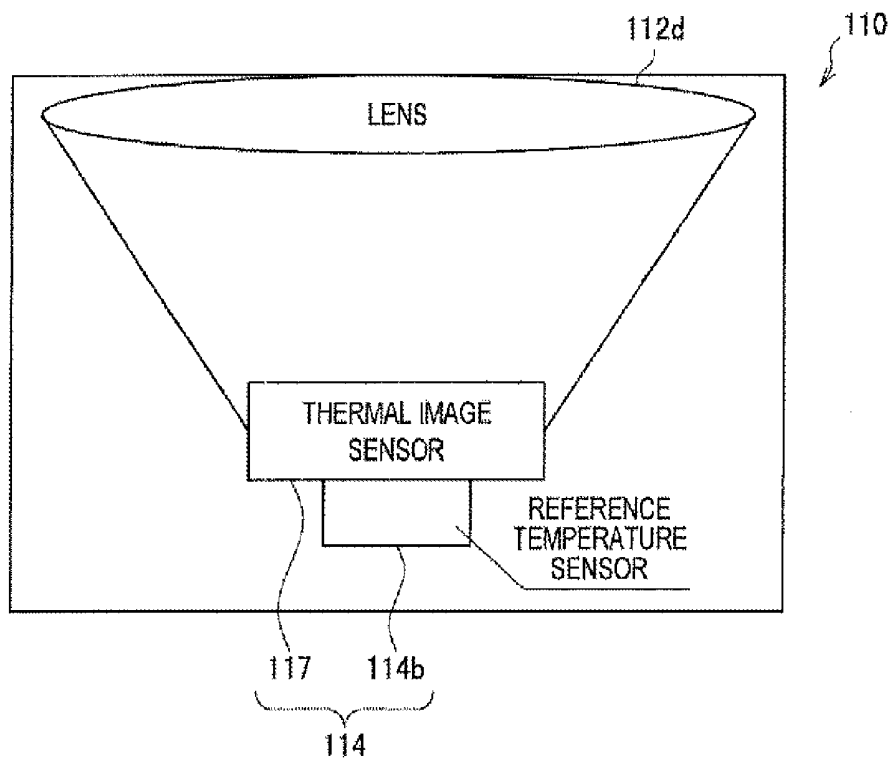


FIG. 21

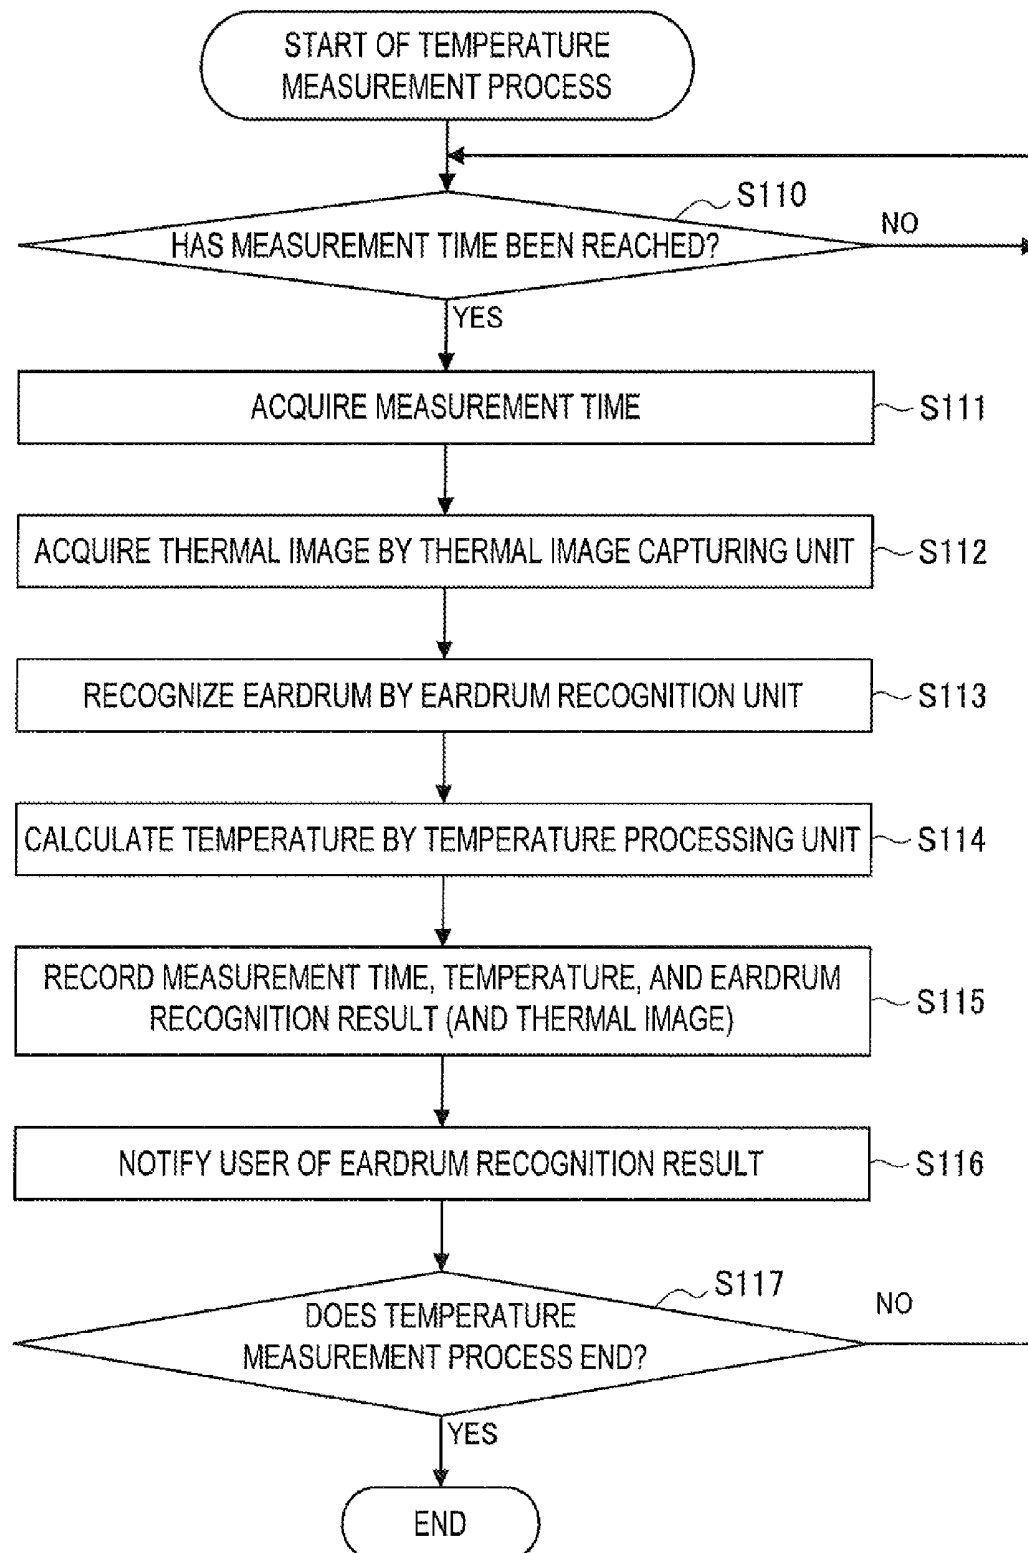


FIG. 22


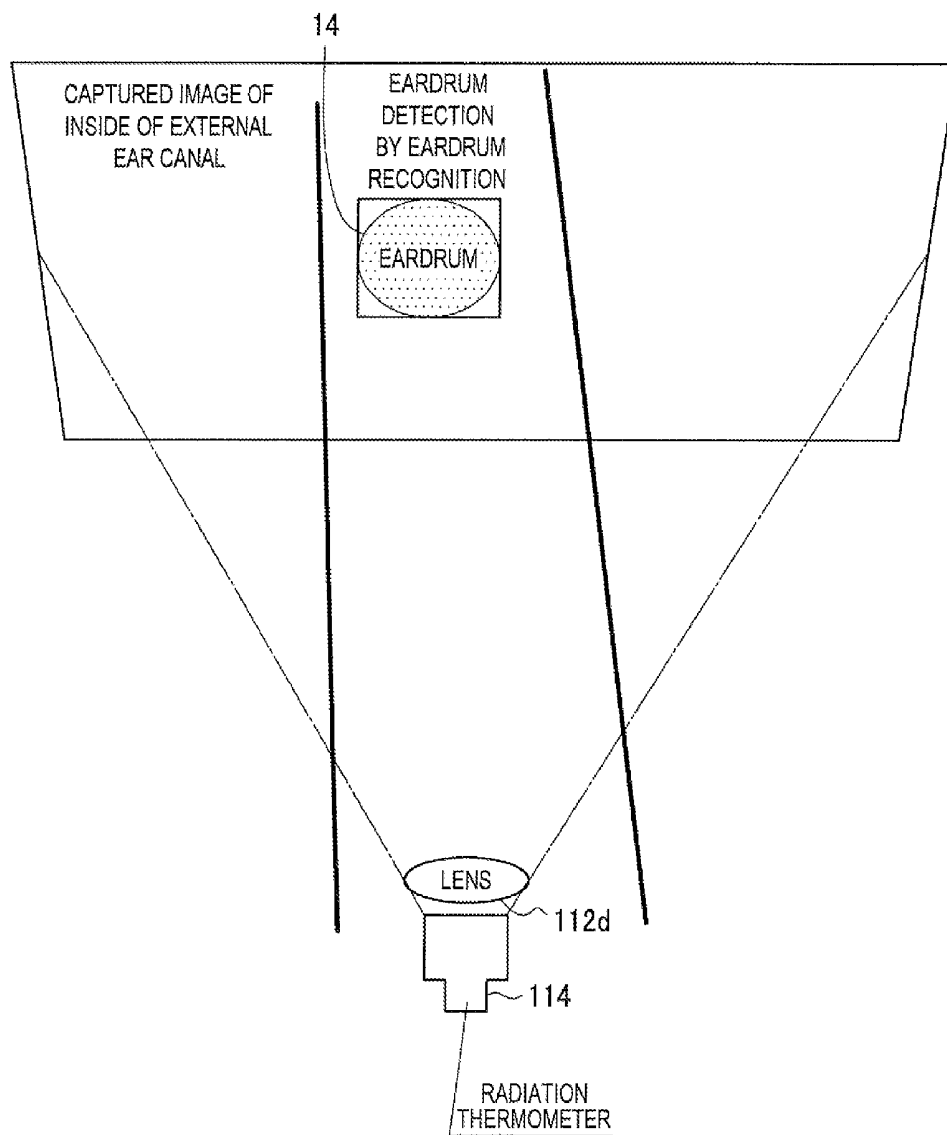


FIG. 23

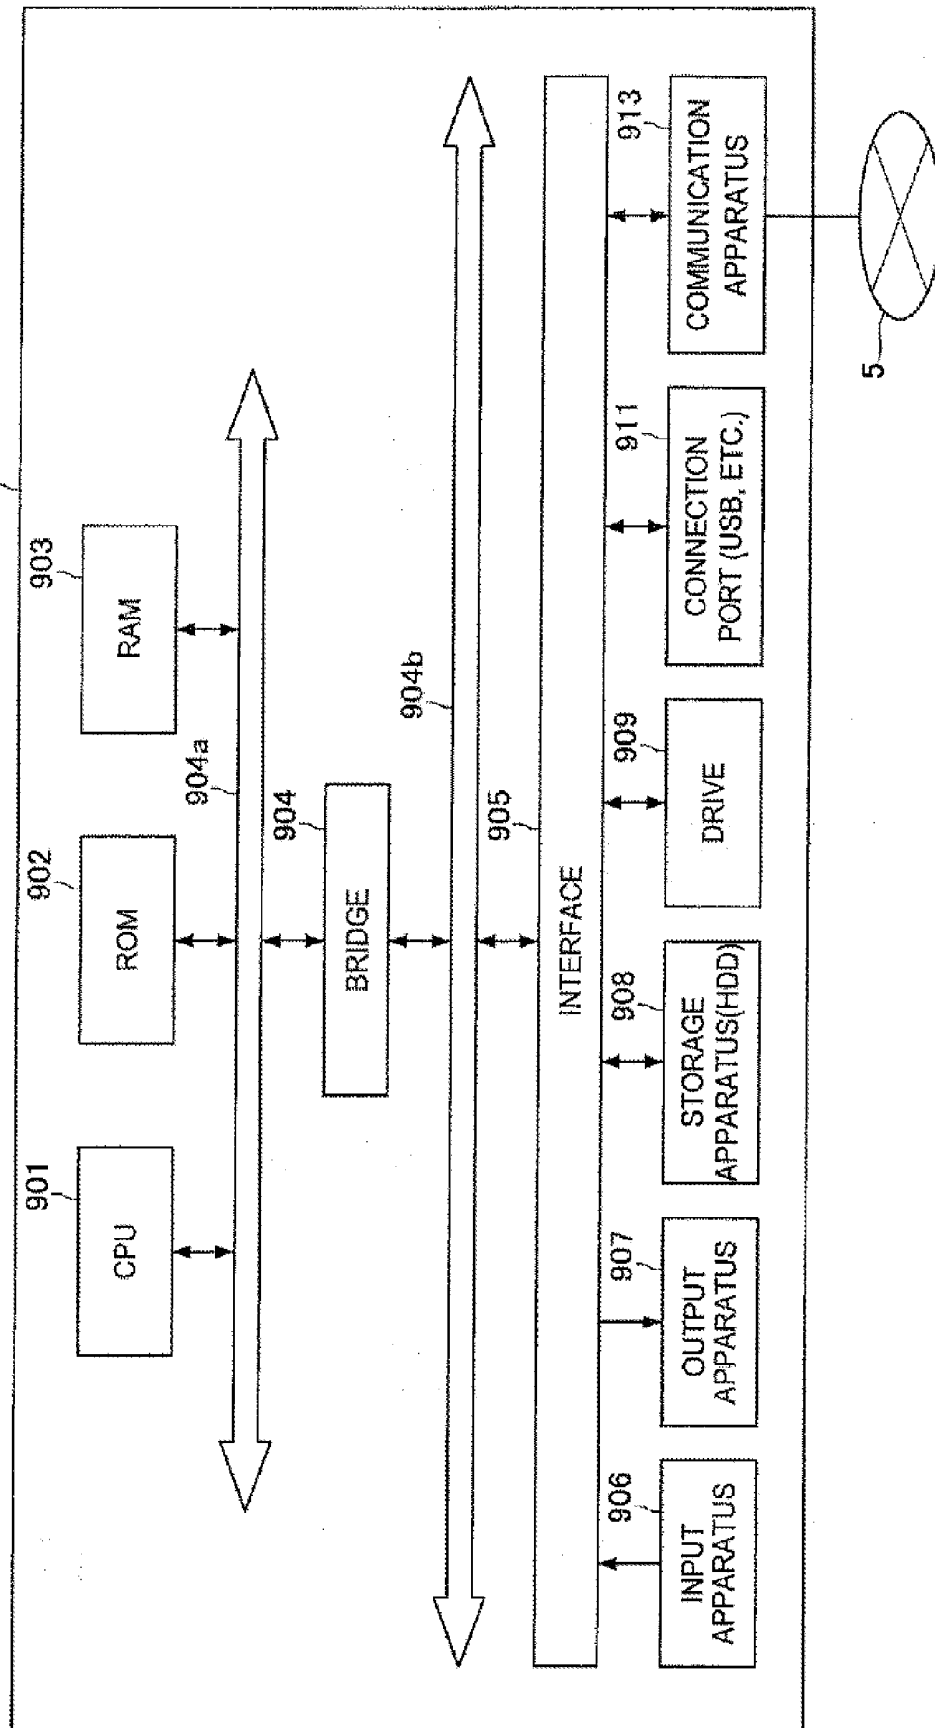

INFORMATION PROCESSING APPARATUS, INFORMATION PROCESSING METHOD, AND COMPUTER PROGRAM FOR MEASURING EARDRUM TEMPERATURE

CROSS-REFERENCE TO RELATED APPLICATION

The present application claims priority from Japanese Patent Application No. JP 2012-076046 filed in the Japanese Patent Office on Mar. 29, 2012, the entire content of which is incorporated herein by reference.

BACKGROUND

The present disclosure relates to an information processing apparatus, an information processing method, and a computer program that measure an eardrum temperature.

Recently, a type of clinical thermometer that measures a body temperature by measuring radiant heat emitted from an eardrum has been proposed. In such a clinical thermometer, a sensor that measures the radiant heat of the eardrum from an external ear canal is inserted and the radiant heat emitted from the eardrum is measured in a non-contact form. For example, in Japanese Patent No. 2671946, an eardrum temperature measurement apparatus for inserting a sensor unit including a first temperature sensor, which detects infrared rays from an eardrum and generates an output voltage in proportion to a temperature difference between an ambient temperature and an eardrum temperature, and a second temperature sensor, which detects a temperature around the first temperature sensor, into an external ear canal is disclosed. A package in which the sensor unit is housed can be held by a support including silicone rubber having a shape that approximately fills between an external ear canal entrance and a first bent portion of the external ear canal. The package can be positioned inside the external ear canal by inserting the support into the external ear canal.

For stable fixing inside the external ear canal, a shape of an insertion portion of a thermometer that measures radiant heat of the eardrum in the related art, a shape along the external ear canal (for example, Japanese Patent No. 2671946 and Japanese Unexamined Patent Application Publication No. 2002-340681) or a cone shape (for example, Japanese Unexamined Patent Application Publication No. H11-28194) is generally formed. In addition, for measurement of a distance from the eardrum to the temperature sensor, a method using distance measurement by laser irradiation or bouncing of sound waves is general.

SUMMARY

However, in Japanese Patent No. 2671946 and Japanese Unexamined Patent Application Publication Nos. 2002-340681 and H11-28194 described above, only one measurement operation for a short time is assumed, and continuous measurement for a long time is not considered. Because the thermometer falls out of the ear if the insertion portion of the thermometer is not firmly pressed into the eardrum at the external ear canal entrance side, it is difficult to constantly hold a direction of the sensor unit inserted into the external ear canal or the user may also experience a large sense of discomfort.

In addition, in Japanese Patent No. 3896807, an infrared clinical thermometer that determines whether an insertion state of a probe into the external ear canal is appropriate by detecting infrared rays radiated from the eardrum using a

detection sensor is disclosed. In the infrared clinical thermometer of Japanese Patent No. 3896807, a body temperature is measured only when the probe is accurately inserted into the external ear canal. However, in the infrared clinical thermometer of Japanese Patent No. 3896807, a predetermined temperature range is set as a measurable range and hence it is difficult to say that radiant heat of the eardrum is accurately measured.

It is desirable to provide a technique of more accurately measuring an eardrum temperature so as to measure a deep body temperature of a human body.

According to an embodiment of the present disclosure, there is provided an information processing apparatus including an eardrum recognition unit configured to recognize a position of an eardrum based on image information regarding the eardrum, a temperature measurement unit configured to acquire a temperature within an external ear canal including the eardrum, and a temperature processing unit configured to determine a temperature of the eardrum based on a recognition result of the eardrum recognition unit and a measured temperature of the temperature measurement unit.

According to an embodiment of the present disclosure, there is provided an information processing method including recognizing a position of an eardrum based on image information regarding the eardrum, acquiring a temperature within an external ear canal including the eardrum, and determining a temperature of the eardrum based on a recognition result of the position of the eardrum and the acquired temperature.

According to an embodiment of the present disclosure, there is provided a computer program for causing a computer to function as an information processing apparatus including an eardrum recognition unit configured to recognize a position of an eardrum based on image information regarding the eardrum, a temperature measurement unit configured to acquire a temperature within an external ear canal including the eardrum, and a temperature processing unit configured to determine a temperature of the eardrum based on a recognition result of the eardrum recognition unit and a measured temperature of the temperature measurement unit.

In accordance with the embodiments of the present disclosure described above, an eardrum temperature can be reliably measured by recognizing an eardrum from an image and performing temperature measurement.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an external appearance diagram illustrating a configuration of an auricle-worn device in accordance with an embodiment of the present disclosure;

FIG. 2 is an explanatory diagram illustrating a state in which the auricle-worn device illustrated in FIG. 1 has been attached to a user's ear;

FIG. 3 is an explanatory diagram illustrating a state of an inside of an external ear canal when the auricle-worn device has been attached;

FIG. 4 is a partially enlarged diagram illustrating a configuration example of a main body unit;

FIG. 5 is a partially enlarged diagram illustrating another configuration example of the main body unit;

FIG. 6 is a block diagram illustrating a configuration of an information processing unit in accordance with the same embodiment;

FIG. 7 is a block diagram illustrating a configuration of an eardrum temperature processing apparatus that performs an eardrum recognition process using a captured image;

FIG. 8 is an explanatory diagram illustrating a specific configuration example of a temperature sensor unit;

FIG. 9 is an explanatory diagram illustrating another specific configuration example of the temperature sensor unit;

FIG. 10 is an explanatory diagram illustrating another specific configuration example of the temperature sensor unit;

FIG. 11 is a flowchart illustrating a temperature measurement process by the eardrum temperature processing apparatus in accordance with the same embodiment;

FIG. 12 is an explanatory diagram illustrating an example of a captured image of an eardrum;

FIG. 13 is a flowchart illustrating an example of the eardrum recognition process;

FIG. 14 is an explanatory diagram illustrating a positional relationship between the eardrum and a temperature measurable range by a radiation thermometer;

FIG. 15 is an explanatory diagram illustrating a state in which part of the eardrum is included in the temperature measurable range by the radiation thermometer;

FIG. 16 is an explanatory diagram illustrating a state in which the eardrum is not included in the temperature measurable range by the radiation thermometer;

FIG. 17 is a block diagram illustrating a configuration of an eardrum temperature processing apparatus including a correction unit that corrects an eardrum temperature;

FIG. 18 is a graph illustrating an example of a correlation relationship between an eardrum occupancy rate and an eardrum temperature;

FIG. 19 is a block diagram illustrating a configuration of an eardrum temperature processing apparatus that performs an eardrum recognition process using a thermal image;

FIG. 20 is an explanatory diagram illustrating a specific configuration example of a temperature sensor unit that acquires a thermal image;

FIG. 21 is a flowchart illustrating a temperature measurement process by the eardrum temperature processing apparatus using a thermal image;

FIG. 22 is an explanatory diagram illustrating a relationship between a thermal image and an eardrum region within the thermal image; and

FIG. 23 is a hardware configuration diagram illustrating a hardware configuration example of the eardrum temperature processing apparatus in accordance with the same embodiment.

DETAILED DESCRIPTION OF THE EMBODIMENT(S)

Hereinafter, preferred embodiments of the present disclosure will be described in detail with reference to the appended drawings. Note that, in this specification and the appended drawings, structural elements that have substantially the same function and structure are denoted with the same reference numerals, and repeated explanation of these structural elements is omitted.

Description will be given in the following order.

1. Configuration of Auricle-Worn Device

2. Body-Temperature Measurement by Auricle-Worn Device

2-1. Configuration of Information Processing Unit

2-2. Eardrum Recognition Process

(1) Eardrum Temperature Processing Apparatus that Performs Eardrum Recognition Process Using Captured Image

(1-A) Configuration of Eardrum Temperature Processing Apparatus

(1-B) Temperature Measurement Process by Eardrum Temperature Processing Apparatus

(1-C) Correction of Measured Temperature

(2) Eardrum Temperature Processing Apparatus that Performs Eardrum Recognition Process Using Thermal Image

(2-A) Configuration of Eardrum Temperature Processing Apparatus

(2-B) Temperature Measurement Process by Eardrum Temperature Processing Apparatus

3. Hardware Configuration Example

<1. Configuration of Auricle-Worn Device>

First, the configuration of the auricle-worn device 100

having an information processing apparatus that measures an eardrum temperature in accordance with an embodiment of the present disclosure will be described with reference to FIGS. 1 to 5. FIG. 1 is an external appearance diagram illustrating the configuration of the auricle-worn device 100 in

accordance with this embodiment. FIG. 2 is an explanatory diagram illustrating a state in which the auricle-worn device 100 illustrated in FIG. 1 has been attached to a user's ear. FIG. 3 is an explanatory diagram illustrating a state of an inside of an external ear canal when the auricle-worn device 100 has

been attached. FIG. 4 is a partially enlarged diagram illustrating a configuration example of a main body unit 120. FIG. 5 is a partially enlarged diagram illustrating another configuration example of the main body unit 120.

The auricle-worn device 100 in accordance with this embodiment is a non-contact thermometer for measuring a deep body temperature by detecting an eardrum temperature of the user's eardrum. For example, as illustrated in FIG. 1, the auricle-worn device 100 includes a temperature sensor unit 110 that detects the eardrum temperature, the main body unit 120, and an information processing unit 130 that performs temperature processing.

The temperature sensor unit 110 is a detection unit that detects the eardrum temperature in a non-contact form. For example, a pyroelectric infrared sensor can be used as the temperature sensor unit 110. The temperature sensor unit 110 is inserted into an external ear canal 12 of the user as illustrated in FIG. 2, and detects infrared rays radiated from the eardrum. Therefore, the temperature sensor unit 110 outputs the detection result as an electric signal to the information processing unit 130 via a wiring arranged within the main body unit 120. An earpiece 122 for holding the temperature sensor unit 110 inside the external ear canal 12 is provided in a connection portion between the temperature sensor unit 110 and the main body unit 120. The earpiece 122 is formed of a material such as a silicone resin.

The main body unit 120 is an attachment member for holding a state in which the temperature sensor unit 110 has been inserted into the external ear canal 12 of the user. As illustrated in FIG. 1, the main body unit 120 has one end connected to the temperature sensor unit 110 and the other end connected to the information processing unit 130. In an intermediate portion that connects the temperature sensor unit 110 and the information processing unit 130, a first bent portion 120a to be attached to an upper part of an auricle E of the user and a second bent portion 120b to be attached to an earlobe E1 at a lower part of the auricle E of the user are formed in correspondence with an ear shape. When the auricle-worn device 100 is attached as illustrated in FIG. 2, the temperature sensor unit 110 is in a state in which the temperature sensor unit 110 faces an eardrum 14 within the external ear canal 12 as illustrated in FIG. 3. This state is held by the earpiece 122 around an opening of the external ear canal 12.

In addition, a wiring that transfers the detection result by the temperature sensor unit 110 to the information processing unit 130 is provided inside the main body unit 120. An internal structure of the main body unit 120 is illustrated in FIGS.

4 and 5. The main body unit **120** is formed of a plastically deformable shape-retaining material.

For example, as illustrated in FIG. 4, the main body unit **120** can include a cylindrical cover **121** formed of an elastic material such as a silicone resin, and one wire **124** and a wiring **126** provided inside the cover **121**. The wire **124** can be provided to hold the shape of the main body unit **120**, and the main body unit **120** can be aligned on the shape of the ear by deforming the shape of the wire **124**. The wiring **126** is a cable through which a signal flows by connecting the temperature sensor unit **110** and the information processing unit **130**, and is provided in a longitudinal direction of the cover **121** along with the wire **124** as illustrated in FIG. 4. As described above, it is possible to implement the lightweight auricle-worn device **100** by simplifying the configuration of the main body unit **120**.

Alternatively, as illustrated in FIG. 5, the wiring **126** may be wound around the wire **124**. Thereby, it is possible to prevent the wiring **126** from being disconnected when the shape of the main body unit **120** is changed. At this time, all or only part of the wiring **126** may be wound over the temperature sensor unit **110** to the information processing unit **130**.

The information processing unit **130** is a functional unit that calculates the eardrum temperature based on the detection result of the temperature sensor unit **110**, and is connected to the other end of the main body unit **120** and arranged on a lower part of the earlobe **E1** as illustrated in FIG. 2. The information processing unit **130** includes an electronic circuit board or the like, and performs a process of converting an electric signal output from the temperature sensor unit **110** via the wiring **126** into a measured value of the body temperature of the user or the like. In addition, the information processing unit **130** in accordance with this embodiment also executes an eardrum recognition process of recognizing a position of the eardrum **14** based on image information. It is possible to precisely measure the eardrum temperature by performing the eardrum recognition process.

For the attachment of the above-described auricle-worn device **100**, first, the main body unit **120** is deformed so that the temperature sensor unit **110** is easily attached to the auricle **E**. By loosely bending the first bent portion **120a** and the second bent portion **120b**, it is possible to extend a linear distance between both ends of the main body unit **120** and it is easy to attach the main body unit **120** to the auricle **E**. In addition, it is also possible to extend the distance between the first bent portion **120a** and the second bent portion **120b** so that the distance is greater than or equal to a distance from an upper end of the auricle **E** to a lower end of the earlobe **E1**. In this case, the first bent portion **120a** and the second bent portion **120b** can maintain a deformed bent shape.

Then, the temperature sensor unit **110** is inserted into the external ear canal **12**, and the earpiece **122** is arranged around the opening of the external ear canal **12**. In this state, the main body unit **120** is deformed and adjusted so that the main body unit **120** is aligned on the auricle **E** of the user, and the auricle-worn device **100** is attached. For example, the auricle-worn device **100** can be stably attached to the auricle **E** by narrowing the extended distance between the first bent portion **120a** and the second bent portion **120b** to the distance from the upper end of the auricle **E** to the lower end of the earlobe **E1**. In addition, the bent shape of the first bent portion **120a** may be formed to be placed on the auricle **E** and the bent shape of the second bent portion **120b** may be deformed to lightly pinch the auricle **E** of the user. In this case, the first bent portion **120a** and the second bent portion **120b** can maintain their bent shapes.

As described above, the auricle-worn device **100** can maintain the attachment state without applying a pressure around the auricle **E** of the user. In addition, because the first bent portion **120a** is placed on the auricle **E** of the user, and the second bent portion **120b** is further attached to sandwich the earlobe **E1**, detachment from the auricle **E** can be prevented and the body temperature can be stably measured even when a direction of external force to the auricle-worn device **100** is not constant. Further, because the lightweight auricle-worn device **100** can be configured, it is possible to reduce a burden imposed on the user even in the attachment for a long time. Accordingly, the auricle-worn device **100** can be used even for body-temperature measurement under a condition that external force from many directions is loaded for a long time, for example, such as body-temperature measurement during activity or during sleep.

<2. Body-Temperature Measurement by Auricle-Worn Device>

The auricle-worn device **100** in accordance with this embodiment acquires a position of the eardrum **14** and a temperature inside the external ear canal **12** including the eardrum **14** as eardrum information by inserting the temperature sensor unit **110** into the external ear canal **12** and causing the temperature sensor unit **110** to face the eardrum **14**. Therefore, the information processing unit **130** calculates an eardrum temperature based on the eardrum information acquired by the temperature sensor unit **110**. Hereinafter, a body-temperature measurement method by the auricle-worn device **100** in accordance with this embodiment will be described based on FIGS. 6 to 21.

[2-1. Configuration of Information Processing Unit]

First, the configuration of the information processing unit **130** in accordance with this embodiment will be described based on FIG. 6. FIG. 6 is a block diagram illustrating the configuration of the information processing unit **130** in accordance with this embodiment. As illustrated in FIG. 6, the information processing unit **130** includes an amplifier **131**, a filter **132**, an analog-to-digital (A/D) conversion unit **133**, an analysis unit **134**, a storage unit **135**, and a communication unit **136**.

The amplifier **131** amplifies an electric signal transmitted from the temperature sensor unit **110**, and outputs the amplified electric signal to the filter **132**. The filter **132** corrects the amplified electric signal by removing a predetermined band of noise from the amplified electric signal, and outputs the corrected electric signal to the A/D conversion unit **133**. The A/D conversion unit **133** converts the electric signal from an analog signal into a digital signal, and outputs the digital signal to the analysis unit **134**. The analysis unit **134** is a processing unit that determines a measured temperature by analyzing the digital signal, and can include an integrated circuit. The measured temperature determined by the analysis unit **134** is transmitted to at least one of the storage unit **135** and the communication unit **136**.

The communication unit **136** outputs the measured temperature determined by the analysis unit **134** to an external device (not illustrated) such as a computer. A communication form of the communication unit **136** may be wireless communication or wired communication. When the wireless communication is performed, for example, it is possible to transmit a measurement result of a body temperature to a computer or the like while the user wears the auricle-worn device **100**. In addition, when the wired communication is performed, for example, the measurement result is stored in the storage unit **135**. After the end of the measurement, the auricle-worn device **100** is removed from the auricle and connected to the computer or the like by a cable or the like,

and the measurement result stored in the storage unit **135** can be transmitted to the computer or the like. Specifically, there is a universal serial bus (USB), a wireless local area network (LAN), ZigBee (registered trademark), Bluetooth (registered trademark), or the like.

As described above, the auricle-worn device **100** measures the eardrum temperature of the user. In addition, because the auricle-worn device **100** can maintain its attachment state without pressing against the auricle E of the user even in the attachment for a long time, for example, it is possible to measure a body temperature at fixed intervals while the auricle-worn device **100** is attached for a long time, and perform analysis of daily fluctuation in the body temperature.

A display unit (not illustrated) connected to the communication unit **136** is further provided in the auricle-worn device **100**, and hence the auricle-worn device **100** can cause the display unit to display the obtained measured temperature. Further, the auricle-worn device **100** may include a battery that supplies power to the information processing unit **130** and the like. When the display unit, the battery, and the like are provided in the auricle-worn device **100**, arrangement positions thereof are not particularly limited. For example, the battery and the display unit may be connected to the other end of the main body unit **120** along with the information processing unit **130**. The display unit and the battery may be provided between the first bent portion **120a** and the second bent portion **120b**.

[2-2. Eardrum Recognition Process]

Next, the configuration of the temperature sensor unit **110** will be described. It is necessary to accurately direct the temperature sensor unit **110** of the auricle-worn device **100** toward the eardrum **14** so as to continuously measure the eardrum temperature of the user accurately for a long time using the auricle-worn device **100**.

There is a small temperature difference between the external ear canal **12** and the eardrum **14**. The temperature of the normal eardrum **14** is set to be higher and a peak of the eardrum **14** measured by the temperature sensor unit **110** is set as the temperature of the eardrum **14**. Therefore, the auricle-worn device **100** in accordance with this embodiment performs the eardrum recognition process of recognizing that the temperature sensor unit **110** accurately faces the eardrum **14**, and measures the eardrum temperature. Thereby, it is possible to measure the eardrum temperature with a higher precision than in the related art.

Hereinafter, an eardrum temperature processing apparatus (information processing apparatus) that performs an eardrum recognition process provided in the auricle-worn device **100** in accordance with this embodiment and measures the eardrum temperature will be described. The eardrum temperature processing apparatus recognizes a position of the eardrum **14** and a temperature inside the ear canal including the eardrum from image information regarding the eardrum acquired by the temperature sensor unit **110** and calculates the eardrum temperature based on the above-described information. The eardrum temperature processing apparatus is the information processing apparatus provided in the auricle-worn device **100**, and can include the temperature sensor unit **110** of the auricle-worn device **100**, the wiring **126**, and the information processing unit **130** described above. In addition, although an example of the eardrum temperature processing apparatus shown hereinafter fully provided in the auricle-worn device **100** will be described, the present technology is not limited thereto. Some functions can also be provided in an external device communicable with the auricle-worn device **100**.

For example, an example of image information regarding the eardrum to be analyzed by the eardrum temperature processing apparatus is a captured image, a thermal image, or the like. Therefore, eardrum recognition processes when the captured image is used and when the thermal image is used will be described hereinafter.

(1) Eardrum Temperature Processing Apparatus that Performs Eardrum Recognition Process Using Captured Image (1-A) Configuration of Eardrum Temperature Processing Apparatus

First, the configuration of the eardrum temperature processing apparatus that performs the eardrum recognition process using the captured image will be described based on FIG. 7. FIG. 7 is a block diagram illustrating the configuration of the eardrum temperature processing apparatus that performs the eardrum recognition process using the captured image.

For the eardrum temperature processing apparatus, which is provided in the auricle-worn device **100** and performs the eardrum recognition process using the captured image, a light-emitting unit **212**, an image capturing unit **214**, and a temperature measurement unit **216** are first provided in the temperature sensor unit **110** as illustrated in FIG. 7. The light-emitting unit **212** is a light-emitting element that emits light based on an instruction from the information processing unit **130**. For example, a light-emitting diode (LED) or the like can be used as the light-emitting unit **212**. The image capturing unit **214** is an imaging element that captures image information including the eardrum **14**. For example, a complementary metal oxide semiconductor (CMOS) image sensor or the like can be used as the image capturing unit **214**. The image capturing unit **214** performs imaging based on an instruction from the information processing unit **130**, and outputs an acquired image to the information processing unit **130**. The temperature measurement unit **216** is a measurement unit that measures a temperature inside the auricle including the eardrum **14**. For example, a thermal infrared sensor such as a thermopile using thermal electromotive force or a thermistor using a temperature change in electrical resistance can be used. Temperature information measured by the temperature measurement unit **216** is output to the information processing unit **130**.

Here, a specific configuration example of the temperature sensor unit **110** will be described based on FIGS. 8 to 10. For the temperature sensor unit **110**, for example, as illustrated in FIG. 8, an LED **111** is provided as the light-emitting unit **212** at its tip end. The LED **111** is arranged to emit light to the eardrum **14**, and emits light based on an instruction of the information processing unit **130**. In addition, as the image capturing unit **214**, a lens **112** and a CMOS image sensor **113** are provided. For light reflected by the external ear canal **12** or the eardrum **14** according to light emitting of the LED **111**, an image is formed on the CMOS image sensor **113** via the lens **112** and output to the information processing unit **130**. Further, as the temperature measurement unit **216**, a radiation thermometer **114** including an infrared sensor **114a**, which measures a temperature difference by receiving infrared rays emitted from an object, and a reference temperature sensor **114b**, which measures an absolute temperature of a measuring instrument, is provided. For example, a thermopile or the like can be used as the infrared sensor **114a**. For example, a thermistor or the like can be used as the reference temperature sensor **114b**. Infrared-domain light detected by the radiation thermometer **114** is converted into an electric signal, and the electric signal is output to the information processing unit **130**.

As another configuration example of the temperature sensor unit **110**, for example, as illustrated in FIG. 9, a lens **112b**

for forming an image of infrared-domain light on the radiation thermometer 114, which is the temperature measurement unit 216, may be provided in addition to a lens 112a and the CMOS image sensor 113, in the temperature sensor unit 110. Thereby, the temperature measurement unit 216 can more reliably receive the infrared-domain light.

As still another configuration example of the temperature sensor unit 110, for example, as illustrated in FIG. 10, the image capturing unit 214 and the temperature measurement unit 216 may be configured using an integrated image infrared sensor 116 in which a CMOS image sensor and an infrared sensor are integrally formed and a reference temperature sensor 114b. Thereby, the number of components constituting the temperature sensor unit 110 can be reduced.

Returning to the description of FIG. 7, the information processing unit 130 includes an eardrum recognition unit 221, a light emission control unit 222, a temperature processing unit 223, a temperature/eardrum state recording unit 224, and a notification unit 225. The eardrum recognition unit 221 determines whether a tip end of the temperature sensor unit 110 faces the eardrum 14, and controls each functional unit based on the determination result. The eardrum recognition unit 221 acquires image information including the eardrum 14, and recognizes a position of the eardrum 14. When the temperature sensor unit 110 has been inserted into the external ear canal 12, the eardrum recognition unit 221 instructs the light emission control unit 222 to cause the light-emitting unit 212 to emit light based on an input of a temperature measurement instruction from the user. In addition, the eardrum recognition unit 221 acquires an image captured by the image capturing unit 214 as image information according to light emitting of the light-emitting unit 212, and analyzes a position of the eardrum 14. When the image information is accurately acquired, the eardrum recognition unit 221 instructs the light emission control unit 222 to turn off the light-emitting unit 212.

The eardrum recognition unit 221 further performs an image recognition process on the acquired image information, and calculates a rate occupied by the eardrum 14 (an eardrum occupancy rate) in the image. Therefore, the eardrum recognition unit 221 outputs the calculated eardrum occupancy rate to the temperature processing unit 223 and at least one of the temperature/eardrum state recording unit 224 and the notification unit 225.

The light emission control unit 222 controls the light emitting of the light-emitting unit 212. The light emission control unit 222 causes the light-emitting unit 212 to emit light based on a light emission instruction from the eardrum recognition unit 221 and turns off the light-emitting unit 212 based on a turn-off instruction.

The temperature processing unit 223 determines an eardrum temperature of the eardrum 14 based on a temperature measured by the temperature measurement unit 216 and the recognition result of the eardrum recognition unit 221. The temperature processing unit 223 determines that the temperature sensor unit 110 faces the eardrum 14 when the eardrum occupancy rate calculated by the eardrum recognition unit 221 is greater than or equal to a predetermined value, and determines that the measured temperature of the temperature measurement unit 216 is reliable. At this time, the temperature processing unit 223 determines the measured temperature as the eardrum temperature. The eardrum temperature is output to at least one of the temperature/eardrum state recording unit 224 and the notification unit 225.

The temperature/eardrum state recording unit 224 is a storage unit that records the eardrum determination result detected by the eardrum recognition unit 221 and the eardrum

temperature measured by the temperature measurement unit 216 in a storage unit (not illustrated). The storage unit may be a memory or the like provided in the eardrum recognition processing apparatus or a memory card or the like attachable to or detachable from the eardrum recognition processing apparatus. The eardrum determination result and the eardrum temperature recorded by temperature/eardrum state recording unit 224, for example, are used to determine the validity/invalidity of the temperature measurement result.

The notification unit 225 notifies the user of a position state of the temperature sensor unit 110, which is a temperature measurement unit for the eardrum 14, that is, whether the tip end of the temperature sensor unit 110 faces the eardrum 14, based on the detection result of the eardrum recognition unit 221. The notification unit 225, for example, may provide notification by sound or the like when the tip end of the temperature sensor unit 110 does not face the eardrum 14, and provide notification by sound or the like when the tip end of the temperature sensor unit 110 faces the eardrum 14. Alternatively, by outputting different sounds when the tip end of the temperature sensor unit 110 does not face the eardrum 14 and when the tip end of the temperature sensor unit 110 faces the eardrum 14, notification of whether the temperature sensor unit 110 faces the eardrum 14 may be provided. In addition, the notification unit 225 notifies the user of the eardrum temperature determined by the temperature processing unit 223.

(1-B) Temperature Measurement Process by Eardrum Temperature Processing Apparatus

The temperature measurement process by the eardrum temperature processing apparatus illustrated in FIG. 7 will be described based on FIG. 11. FIG. 11 is a flowchart illustrating the temperature measurement process by the eardrum temperature processing apparatus in accordance with the same embodiment.

The temperature measurement process by the eardrum temperature processing apparatus is started when a measurement time has been reached as illustrated in FIG. 11 (S100). The measurement time, for example, such as every second, every minute, or a designated time set by the user, can be arbitrarily set. The eardrum recognition unit 221 iteratively executes the process of step S100 when the measurement time has not been reached. When reaching a measurement time, the measurement time is acquired (S101), and thereafter, the temperature measurement unit 216 first measures a temperature within the external ear canal 12 (S102). The temperature measured in step S102 becomes the temperature (eardrum temperature) of the eardrum 14. In this embodiment, the following eardrum recognition process is performed. When the temperature sensor unit 110 accurately faces the eardrum 14, the measured temperature is determined to be the eardrum temperature. Thereby, it is possible to accurately measure the eardrum temperature.

Then, in order to perform the eardrum recognition process, the eardrum recognition unit 221 instructs the light emission control unit 222 to cause the light-emitting unit 212 to emit light. The light emission control unit 222 causes the light-emitting unit 212 to emit the light by receiving the light emission instruction (S103). When the light-emitting unit 212 emits the light, the image capturing unit 214 acquires an image of the eardrum 14 (S104), and outputs the acquired image to the eardrum recognition unit 221. Upon receipt of an input of the image of the eardrum 14, the eardrum recognition unit 221 instructs the light emission control unit 222 to turn off the light-emitting unit 212, and the light-emitting unit 212 is turned off (S105). Because there is a concern that the temperature within the external ear canal 12 is likely to rise

while the light-emitting unit 212 emits the light and the eardrum temperature is not accurately measureable, the light-emitting unit 212 may be turned off except for when the measurement is performed.

When the captured image of the eardrum 14 is acquired in the process of steps S103 to S105, the eardrum recognition unit 221 performs the eardrum recognition process based on the image (S106). In the eardrum recognition process, a position of the eardrum 14 is specified by recognizing a light cone from the image obtained by capturing the eardrum 14. An example of the captured image of the eardrum 14 is illustrated in FIG. 12. When the eardrum 14 is imaged, a malleus 14a and a light cone 14b are characteristically viewed. The malleus 14a is a bone attached closely to the inside of the eardrum 14, and is viewed simultaneously when the eardrum 14 is viewed. The light cone 14b is viewed when light emitted by the light-emitting unit 212 is reflected on the eardrum 14 in the ear. The eardrum recognition unit 221 specifies a position of the eardrum within the captured image by recognizing the above-described feature.

An example of an image recognition algorithm for use in the eardrum recognition process is a technique of boosting and learning a pixel difference feature (Japanese Patent No. 4517633). Further, a technique using a Gabor filter in a filter base (Japanese Patent No. 4333364), a technique using a Haar-like feature, or the like is also applicable to the eardrum recognition process.

In these techniques, an eardrum image, an image in which only part (for example, a half) of the eardrum is shown, an image in which only the external ear canal is shown, and the like are collected in a large volume. A designer of the eardrum temperature processing apparatus labels the images one by one by cutting the image into a part which is the eardrum 14 and a part which is not the eardrum 14. The labeling is performed in the following order.

Procedure 1: Collection of Images

First, a captured image of the inside of the external ear canal is collected. In this case, it is desirable to perform imaging using a lens having an angle of view equivalent to that of a lens used in the radiation thermometer 114. Various images including an image in which the front of the eardrum 14 is clearly shown, an image in which the eardrum 14 is obliquely shown, an image in which no eardrum 14 is shown, and the like are captured and collected.

Procedure 2: Determination of Eardrum Region (Labeling)

A human determines whether a region (eardrum region) of the eardrum 14 is shown or not shown in the image collected in Procedure 1. When the eardrum is shown in the image, the human encloses the eardrum region in the rectangle. Further, when the malleus 14a is viewed, an angle of the malleus 14a is measured. Alternatively, a straight line may be drawn along the malleus 14a. This is because the eardrum region and the angle of the malleus 14a within the image become important information as teacher data of machine learning.

For the image in which the eardrum 14 is shown on the occasion of labeling, the image may be rotated and normalized so that the direction of the malleus 14a is aligned in a fixed direction (for example, in a vertical direction as illustrated in FIG. 12). Thereby, a feature quantity is likely to be produced and a strong classifier can be created.

Here, an example of the eardrum recognition process of step S106 will be described in detail based on FIG. 13. FIG. 13 is a flowchart illustrating the example of the eardrum recognition process to which an object detection process disclosed in Japanese Unexamined Patent Application Publication No. 2005-157679 has been applied. The eardrum 14 serves as an object. In this case, the eardrum recognition unit

221 functions as a scaling unit that performs scaling by enlarging or reducing a grayscale image, which is an input image, and a scanning unit that sequentially scans the scaled input image in a size of a predetermined-size window image. Further, the eardrum recognition unit 221 functions as a classifier that classifies whether each window image sequentially scanned by the scanning unit is an object or a non-object. That is, the eardrum recognition unit 221 generates scaled images by enlarging or reducing the input image to all designated scales, clips a window image by sequentially scanning a window having a size of an object desired to be detected, and classifies whether the clipped image is an object.

According to a detailed description, first, the eardrum recognition unit 221 scales an image captured by the image capturing unit 214 at a fixed ratio (S200). The image processed by the eardrum recognition unit 221 is a grayscale image. The timing at which the scaled image is generated is set as a point in time at which eardrum detection from the entire region of a previous output scaled image has ended. The process moves to processing on an input image of the next frame at a point in time at which the scaled image is smaller than a window image. When the scaled image is generated, the eardrum recognition unit 221 clips a window image by scanning a position of a search window in length and width for the scaled image (S201).

Then, the eardrum recognition unit 221 determines whether the window image clipped in step S201 is an object, that is, the eardrum 14. The eardrum recognition unit 221 calculates a value (an updated value of a weighted majority decision value) obtained by sequentially weighting and adding estimation values $f(x)$ of a plurality of weak classifiers for the window image as an evaluation value s . It is determined whether the window image is the object and whether the classification is truncated based on the evaluation value s .

That is, when the window image is input, the eardrum recognition unit 221 initializes its evaluation value to $s=0$, and calculates an inter-pixel difference feature d_i (S202). The inter-pixel difference feature d_i is a difference between luminance values I_1 and I_2 of two arbitrary pixels, and is expressed by the following Expression (1). The pixel luminance value I is expressed by the following Expression (2). (x, y) represents a position of a pixel constituting an image.

$$d_i = I_1 - I_2 \quad (1)$$

$$I(x, y) = \sum_{x' < x, y' < y} S(x', y') \quad (2)$$

The eardrum recognition unit 221 further reflects an estimation value of whether the window image is the object in the evaluation value s for determining whether the window image is the object (S203). Therefore, the eardrum recognition unit 221 determines whether the evaluation value s is greater than a truncation threshold value R_t for truncation in mid-course of detection in a classification process (S204). When the evaluation value s is greater than the truncation threshold value R_t , the eardrum recognition unit 221 determines whether the process has been iterated a predetermined number of times (K times) (S205). When the process has not been iterated a predetermined number of times (K times), the process from step S202 is iterated.

On the other hand, when it is determined that the process has been iterated a predetermined number of times (K times) in step S205 or when it is determined that the evaluation value s is less than the truncation threshold R_t in step S204, the

eardrum recognition unit 221 determines whether there is the next search window (S206). The eardrum recognition unit 221 determines whether the next search window is the object according to whether the acquired evaluation value s is greater than 0. When the next search window is the object, the eardrum recognition unit 221 stores a current window position, classifies whether there is the next search window, and iterates the process from step S201 when there is the next search window. On the other hand, when the search window has been scanned in all the next regions, the eardrum recognition unit 221 determines whether there is the next scaled image (S207).

When it is determined that there is the next scaled image in step S207, the eardrum recognition unit 221 iterates the process from step S200. The scaling process of step S200 ends at a point in time at which the scaled image is smaller than the window image. On the other hand, when it is determined that there is no next scaled image in step S207, the eardrum recognition unit 221 executes a process of deleting an overlapping region (S208 to S210). The process of deleting an overlapping region is a process of removing regions overlapping each other when a region determined to be a target physical object overlaps in one input image.

First, the eardrum recognition unit 221 determines whether there are regions overlapping each other (S208). Therefore, when there are a plurality of overlapping regions stored in step S205, the eardrum recognition unit 221 extracts two regions overlapping each other, deletes a region having a lower evaluation value s between the two regions by regarding the region as having a lower reliability degree, and selects a region having a higher evaluation value s (S210). Therefore, the process from step S208 is reiterated. Thereby, only one region having a highest evaluation value s is selected from among extracted regions overlapping a plurality of times. When two or more object regions do not overlap and when there is no object region, the process for one input image ends and the process moves to the next frame processing.

According to the above-described eardrum recognition process, an object is detected using a classifier that has learned from a weak classifier, which performs weak classification by an inter-pixel difference feature, according to group learning. Thus, a process of reading luminance values of two corresponding pixels in a window image and calculating a feature quantity of an object by merely calculating a difference therebetween ends. Because the eardrum recognition process can be performed at a very high speed, real-time eardrum recognition is possible.

In addition, the eardrum recognition unit 221 makes a comparison with the truncation threshold value R_t every time the evaluation value s is sequentially updated by adding a value obtained by multiplying a classification result (estimation value) classified from the feature quantity by a reliability degree for the weak classifier used in the classification. At this time, the calculation of the weak classifier is truncated when the evaluation value s is less than the truncation threshold value R_t , and the eardrum recognition can be performed at a higher speed by moving the process to processing on the next window image and rapidly reducing an ineffective calculation.

That is, when window images have been clipped by scanning all regions of an input image, an image obtained by performing reduction scaling on the input image, and a scaled image, the window images are unlikely to be an object and most of the window images are a non-object. It is possible to extremely increase the efficiency of the classification process by truncating the classification of the window image, which is a non-object, in mid-course. On the other hand, when there

are a large number of objects to be detected, a threshold value for truncating a calculation of a window image obviously determined to be an object in mid-course may be provided according to a technique similar to that of the above-described truncation threshold value. Further, it is possible to set a search window with an arbitrary size and detect an object with an arbitrary size by scaling the input image using the scaling unit.

In addition, when the eardrum recognition process is performed, it is possible to obtain a recognition result without depending upon an insertion direction of the temperature sensor unit 110 by rotating a capturing image by a fixed angle (for example, about 15 degrees) and making a determination by the eardrum recognition unit 221. Highly precise recognition is performed for eardrums with various sizes by performing scaling for enlarging or reducing an image to correspond to a large or small eardrum size in addition to the rotation and making a determination by the eardrum recognition unit 221.

In addition, a recognition process is possible, without performing rotation or scaling in advance, using a processing method using a scale invariant feature transform (SIFT) feature quantity, which is a rotation invariant feature quantity, a processing method of obtaining a luminance gradient of an image or creating a histogram discretized for every angle in each local region, or the like.

When position information regarding the eardrum 14 is acquired according to the eardrum recognition process, the eardrum recognition unit 221 calculates an eardrum occupancy rate, which is a ratio of a part in which the eardrum 14 is shown in a captured image. It is possible to determine whether the temperature sensor unit 110 substantially directly faces the eardrum 14 and temperature measurement is accurately performed from the eardrum occupancy rate. The eardrum recognition unit 221 outputs the calculated eardrum occupancy rate to the temperature processing unit 223. The temperature processing unit 223 determines the measured temperature of the temperature measurement unit 216 as the eardrum temperature when the eardrum occupancy rate is greater than or equal to a predetermined value.

In addition, the eardrum recognition unit 221 determines whether the temperature sensor unit 110 faces the eardrum 14 based on the eardrum occupancy rate, and allows the user to adjust the direction of the temperature sensor unit 110 when the temperature sensor unit 110 does not face the eardrum 14. Thus, the eardrum recognition unit 221 continuously recognizes the position of the eardrum 14. The recognition of the position of the eardrum 14 may be performed by executing the eardrum recognition process as described above or by tracking the position of the eardrum 14 recognized once. Because the eardrum recognition process is generally time-consuming, sight of the eardrum 14 is lost until the process is completed. Because a processing load of the tracking is lower than that of the eardrum recognition process, it is possible to specify the position of the eardrum 14 at a high speed and reduce power consumption.

The tracking of the eardrum 14 will be specifically described based on FIGS. 14 to 16. The tracking is executed when the position of the eardrum 14 is specified in the eardrum recognition process, and continuously performed until sight of the eardrum 14 is lost. FIG. 14 is an explanatory diagram illustrating the eardrum occupancy rate, and illustrates a state in which the temperature sensor unit 110 is inserted into the external ear canal 12 and faces the eardrum 14. At this time, it is assumed that an angle of view of the lens 112 of the temperature sensor unit 110 is α and a temperature measureable angle of the radiation thermometer 114 is β ($<\alpha$). According to the angle of view of the lens 112, a size of

15

an image captured by the CMOS image sensor 113 (a captured image of the inside of the external ear canal) is determined. On the other hand, a temperature measurable range of the radiation thermometer 114 is determined by the temperature measurable angle β .

An eardrum occupancy rate O_R is represented by an eardrum area S_{eard} within the temperature measurable range compared to a temperature measurable area S_{temp} ($O_R = S_{eard}/S_{temp}$). Accordingly, when the eardrum area S_{eard} included in the temperature measurable range is smaller, the eardrum occupancy rate O_R is lower. For example, as illustrated in FIG. 15, when the temperature sensor unit 110 within the external ear canal 12 does not sufficiently face the eardrum 14, only part of the eardrum 14 is included in the temperature measurable range of the radiation thermometer 114. In addition, as illustrated in FIG. 16, when the direction of the temperature sensor unit 110 inserted into the external ear canal 12 is different from a direction in which the eardrum 14 is directed, the eardrum 14 is also considered not to be included in the temperature measurable range of the radiation thermometer 114. When the eardrum occupancy rate O_R is less than a predetermined value, the measured temperature of the radiation thermometer 114 is far from an actual eardrum temperature and an accurate eardrum temperature is not measurable.

Therefore, because the eardrum 14 is tracked when the position of the eardrum 14 is specified according to the eardrum recognition process, the eardrum recognition unit 221 extracts a detected feature quantity of a luminance gradient or the like of the eardrum 14 based on the eardrum recognition result. Therefore, the eardrum recognition unit 221 tracks the eardrum 14 by searching for the eardrum 14 only in the vicinity thereof based on the extracted feature quantity. When the position of the eardrum 14 for the temperature measurable range is specified according to the tracking, the eardrum recognition unit 221 calculates an accurate direction of the temperature sensor unit 110 so that the eardrum 14 is in the temperature measurable range of the radiation thermometer 114. Therefore, the eardrum recognition unit 221 outputs the calculated accurate direction of the temperature sensor unit 110 to the notification unit 225.

When sight of the eardrum 14 is lost during the tracking, the eardrum recognition unit 221 executes the eardrum recognition process again. Alternatively, the eardrum recognition unit 221 may reset the position of the eardrum 14 by executing the eardrum recognition process after a predetermined time has elapsed from the start of the tracking even when the sight of the eardrum 14 is lost. Because the tracking process is performed using simpler information than in the eardrum recognition process, the eardrum recognition process is superior to the tracking in terms of precision. Thus, because the position of the eardrum 14 is accurately recognized, it is preferable to recognize the position of the eardrum 14 according to the eardrum recognition process periodically even during the tracking.

Returning to the description of FIG. 11, when the eardrum 14 is recognized in step S106, the eardrum recognition unit 221 records the recognition result of the eardrum 14 on the temperature/eardrum state recording unit 224 (S107). The measurement time acquired in step S101 and the eardrum temperature measured in step S102 are also recorded on the temperature/eardrum state recording unit 224. Thereafter, the eardrum recognition unit 221 notifies the user of the eardrum recognition result via the notification unit 225 (S108). Therefore, the eardrum recognition unit 221 checks whether there is an instruction to end the temperature measurement process, the process from step S100 is iteratively executed if there is no

16

end instruction, and the process illustrated in FIG. 11 ends if there is an end instruction (S109).

As described above, in the eardrum temperature processing apparatus in accordance with this embodiment, the eardrum recognition process of recognizing the position of the eardrum 14 is performed and the eardrum temperature of the eardrum 14 is measured. It is possible to reliably measure the eardrum temperature by recognizing an image of the eardrum from image information regarding the eardrum 14 and performing temperature measurement. In addition, the user is notified of a position state of the temperature sensor unit 110 for the eardrum 14, and notified of an adjustment instruction so that the temperature sensor unit 110 is accurately directed to the eardrum 14 when there is a deviation. It is possible to accurately measure a temperature by recognizing a state in which the eardrum temperature is not accurately measurable as described above and allowing the user to adjust an attachment state of a device.

Further, it is possible to perform history management on a time change in the eardrum temperature by outputting the measurement time to the temperature/eardrum state recording unit 224 along with the eardrum temperature and the image information and storing the output measurement time in the storage medium. Accordingly, for example, it is possible to perform analysis of daily fluctuation in a body temperature by attaching the auricle-worn device 100 for a long time and measuring the eardrum temperature at fixed intervals.

(1-C) Correction of Measured Temperature

The eardrum temperature processing apparatus illustrated in FIG. 7 calculates an eardrum temperature based on an occupancy rate (eardrum occupancy rate) in an image of the eardrum 14 recognized in the eardrum recognition process and the measured temperature from the temperature measurement unit 216. Here, the eardrum temperature processing apparatus may further include a correction unit that corrects an eardrum temperature calculated according to a magnitude of an area in which the eardrum 14 is shown. It is possible to calculate the eardrum temperature with a higher precision by including the above-described correction unit. The above-described tracking is also performed to recognize how far the temperature measurable range of the radiation thermometer 114 is from a range of the eardrum 14. The correction unit determines how much the measured temperature should be corrected according to a distance between the temperature measurable range and the range of the eardrum 14.

A configuration example of the eardrum temperature processing apparatus including the correction unit that corrects the eardrum temperature is illustrated in FIG. 17. The eardrum temperature processing apparatus illustrated in FIG. 17 is different from the eardrum temperature processing apparatus of FIG. 7 in that the correction unit is included. Because configurations and functions of the other functional units are the same, description thereof is omitted here.

The correction unit 226 corrects the eardrum temperature based on the eardrum occupancy rate, which is a ratio of an area in which the eardrum is shown in a captured image. The correction unit 226 corrects a temperature according to the eardrum occupancy rate in the captured image to determine the eardrum temperature based on the recognition result of the eardrum recognition process of the eardrum recognition unit 221, the eardrum temperature determined by the temperature processing unit 223, and the measured temperature from the temperature measurement unit 216. There is a correlation relationship between the eardrum occupancy rate and the eardrum temperature. The correction unit 226 can correct the measured temperature based on the correlation relation-

ship. An example of the correlation relationship between the eardrum occupancy rate and the eardrum temperature is illustrated in FIG. 18. When the horizontal axis represents an eardrum occupancy rate [%] and the vertical axis represents an eardrum temperature [$^{\circ}$ C.], the graph of FIG. 18 illustrates a relationship therebetween. It can be seen that the eardrum temperature is also higher when the eardrum occupancy rate is higher.

The correlation relationship between the eardrum occupancy rate and the eardrum temperature may be created while the eardrum temperature is measured for each person whose eardrum temperature is measured. According to the result of the eardrum recognition process and the tracking, the eardrum temperature is also measured along with the position of the eardrum 14 and the eardrum occupancy rate. Therefore, it is possible to precisely perform temperature correction by measuring the correlation relationship between the eardrum occupancy rate and the eardrum temperature as illustrated in FIG. 18 while a position in which the eardrum occupancy rate is high is initially searched for and creating the correlation relationship between the eardrum occupancy rate and the eardrum temperature unique to the person whose eardrum temperature is measured. Because the correlation relationship between the eardrum occupancy rate and the eardrum temperature is likely to change even when measurement is performed on the same person, it is desirable to create the correlation relationship for every measurement time of the eardrum temperature and appropriately update the correlation relationship.

When the correlation relationship between the eardrum occupancy rate and the eardrum temperature as illustrated in FIG. 18 is obtained, the eardrum recognition unit 221, for example, calculates the eardrum occupancy rate according to the eardrum recognition process or the tracking. The correction unit 226 calculates a temperature difference between a measured temperature at the calculated eardrum occupancy rate and a temperature when the eardrum occupancy rate is highest by referring to the correlation relationship between the eardrum occupancy rate and the eardrum temperature. For example, in FIG. 18, when the temperature at the highest eardrum occupancy rate is 37° C. and the eardrum occupancy rate is 20%, the measured temperature is 0.4° C. lower than 37° C. That is, when the eardrum occupancy rate is lower, the measured temperature is lower than an actual eardrum temperature. Therefore, the correction unit 226 corrects the measured temperature based on the calculated eardrum occupancy rate. For example, when the eardrum occupancy rate is 20% and the measured temperature is 36.4° C., the correction unit 226 adds an amount (in this case, 0.4° C.) by which the measured temperature is lower than the actual eardrum temperature to the measured temperature of 36.4° C., and hence the temperature of 36.8° C. after the addition is given as the eardrum temperature.

After correcting the measured temperature based on the correlation relationship and calculating the eardrum temperature, the correction unit 226 outputs the eardrum temperature and the eardrum recognition result from the eardrum recognition unit 221 to the temperature/eardrum state recording unit 224. In addition, the eardrum temperature after the correction is also output to the notification unit 225 and the user is notified thereof. As described above, it is possible to acquire a more accurate eardrum temperature by providing the correction unit 226 to correct the measured temperature.

The configuration of the eardrum temperature processing apparatus that performs the eardrum recognition process

using the captured image and the process of measuring the temperature of the eardrum 14 according to the configuration have been described above.

(2) Eardrum Temperature Processing Apparatus that Performs Eardrum Recognition Process Using Thermal Image
(2-A) Configuration of Eardrum Temperature Processing Apparatus

First, the configuration of the eardrum temperature processing apparatus that performs the eardrum recognition process using the thermal image will be described based on FIG. 19. FIG. 19 is a block diagram illustrating the configuration of the eardrum temperature processing apparatus that performs the eardrum recognition process using the thermal image.

First, the eardrum temperature processing apparatus provided in the auricle-worn device 100 includes a thermal image capturing unit 218 in the temperature sensor unit 110 as illustrated in FIG. 19. The thermal image capturing unit 218 is a detection unit that acquires a thermal image including the eardrum 14 as image information, and, for example, can include a detection element such as a bolometer or a thermopile. Because the thermal image is visually displayed as an image of a temperature distribution of an object, it is possible to simultaneously acquire a position of the eardrum and a measured temperature. The thermal image capturing unit 218 outputs the acquired thermal image to the information processing unit 130.

Here, a specific configuration example of the temperature sensor unit 110 is illustrated in FIG. 20. For example, as illustrated in FIG. 20, for the temperature sensor unit 110, a lens 112d and a thermal image sensor 117 are provided as the thermal image capturing unit 218. In the thermal image sensor 117, an image acquisition unit having an image acquisition function and a temperature measurement unit having a temperature measurement function are implemented by one device. For infrared-domain light emitted from a human body, an image is formed on the thermal image sensor 117 via the lens 112d and converted into an electric signal, and the electric signal is output to the information processing unit 130.

Returning to the description of FIG. 19, the information processing unit 130 includes an eardrum recognition unit 221a, a temperature processing unit 223a, a temperature/eardrum state recording unit 224, and a notification unit 225. Because the temperature/eardrum state recording unit 224 and the notification unit 225 have the same configurations and functions as those of the eardrum temperature processing apparatus using the captured image illustrated in FIG. 7, description thereof is omitted here.

The eardrum recognition unit 221a determines whether a tip end of the temperature sensor unit 110 faces the eardrum 14, and controls the functional units based on the determination result. The eardrum recognition unit 221a acquires a thermal image as image information including the eardrum 14 from the thermal image acquisition unit 218 and recognizes the position of the eardrum 14. The eardrum recognition process can be performed as in the eardrum recognition process on the above-described captured image. This process will be described later. The eardrum recognition unit 221a performs the image recognition process on the acquired thermal image, and calculates a ratio occupied by the eardrum 14 (an eardrum occupancy rate) in the image. Therefore, the eardrum recognition unit 221a outputs the calculated eardrum occupancy rate to at least one of the notification unit 225 and the temperature/eardrum state recording unit 224.

The temperature processing unit 223a calculates the eardrum temperature based on the thermal image. As will be described later, in the case of the thermal image, a tempera-

ture measurable range corresponds to a captured image. The temperature processing unit **223a** calculates a region of the eardrum **14** for the thermal image from the result of the eardrum recognition process, and outputs an average temperature within the eardrum region as the eardrum temperature to the temperature/eardrum state recording unit **224**.

(2-B) Temperature Measurement Process by Eardrum Temperature Processing Apparatus

The temperature measurement process by the eardrum temperature processing apparatus illustrated in FIG. **19** will be described based on FIG. **21**. FIG. **21** is a flowchart illustrating the temperature measurement process by the eardrum temperature processing apparatus using the thermal image. The detailed description of the same process as the temperature measurement process by the eardrum temperature processing apparatus using the captured image described based on FIG. **11** is omitted.

The temperature measurement process by the eardrum temperature processing apparatus using the thermal image is started when a measurement time has been reached as illustrated in FIG. **21** (S110). The measurement time, for example, such as every second, every minute, or a designated time set by the user, can be arbitrarily set. The eardrum recognition unit **221a** iteratively executes the process of step S110 when not reaching the measurement time. When reaching the measurement time, the measurement time is acquired (S111), and thereafter, the thermal image capturing unit **218** acquires the thermal image (S112). When acquiring the thermal image, the thermal image capturing unit **218** outputs the thermal image to the information processing unit **130**.

The information processing unit **130** receiving the input of the thermal image from the thermal image capturing unit **218** performs the eardrum recognition process based on the thermal image according to the eardrum recognition unit **221a** (S113). The eardrum recognition process can be performed as in the above-described step S106 of FIG. **11**. That is, a thermal image, an image in which only a half of the eardrum is shown, an image in which only the external ear canal is shown, and the like are collected in a large volume. The user labels the images one by one in advance by cutting the image into a part which is the eardrum **14** and a part which is not the eardrum **14**. By creating a classifier created by statistically learning the above, the eardrum recognition unit **221a** can recognize the position of the eardrum **14** from the thermal image.

Then, when the eardrum **14** is recognized in step S114, the temperature processing unit **223a** calculates an eardrum temperature (S114). FIG. **22** illustrates a relationship between a thermal image and a region of the eardrum **14** (an eardrum region) within the thermal image. As illustrated in FIG. **22**, in the thermal image, a range of the thermal image becomes a temperature measurable range. While only one measured value can be acquired in the case of the temperature sensor, temperature information can be acquired at an image resolution in the thermal image. The temperature processing unit **223a** obtains the eardrum region for the thermal image from the eardrum recognition processing result, and sets an average value of temperatures within the eardrum region to the eardrum temperature.

The eardrum recognition unit **221a** records the recognition result of the eardrum **14** on the temperature/eardrum state recording unit **224** (S115). On the temperature/eardrum state recording unit **224**, the measurement time acquired in step S111 and the eardrum temperature measured in step S113 are also recorded. Thereafter, the eardrum recognition unit **221a** notifies the user of the eardrum recognition result via the notification unit **225** (S116). Therefore, the eardrum recog-

nition unit **221a** checks whether there is an instruction to end the temperature measurement process, the process from step S110 is iteratively executed if there is no end instruction, and the process illustrated in FIG. **21** ends if there is an end instruction (S117).

As described above, in the eardrum temperature processing apparatus using the thermal image, the eardrum recognition process of recognizing the position of the eardrum from the thermal image is performed and the eardrum temperature of the eardrum **14** is measured. As described above, it is possible to more accurately measure the eardrum temperature by checking whether the temperature sensor unit **110** is directed to the eardrum **14** and determining the eardrum temperature. In addition, the user is notified of a position state of the temperature sensor unit **110** for the eardrum **14**, and notified of an adjustment instruction so that the temperature sensor unit **110** is accurately directed to the eardrum **14** when there is a deviation. As described above, it is possible to accurately measure a temperature by recognizing a state in which the eardrum temperature is not accurately measurable and allowing the user to adjust an attachment state of a device. Further, it is possible to perform history management on a time change in the eardrum temperature by outputting the measurement time to the temperature/eardrum state recording unit **224** along with the eardrum temperature and the image information and storing the output measurement time in the storage medium. Accordingly, for example, it is possible to perform analysis of daily fluctuation in the body temperature by attaching the auricle-worn device **100** for a long time and measuring the eardrum temperature at fixed intervals.

<3. Hardware Configuration Example>

A process by the eardrum temperature processing apparatus in accordance with this embodiment can also be executed by hardware or software. In this case, the eardrum temperature processing apparatus can also be configured as illustrated in FIG. **23**. Hereinafter, the hardware configuration example of the eardrum temperature processing apparatus in accordance with this embodiment will be described based on FIG. **23**.

The eardrum temperature processing apparatus in accordance with this embodiment can be implemented by a processing apparatus such as a computer as described above. As illustrated in FIG. **23**, the eardrum temperature processing apparatus includes a central processing unit (CPU) **901**, a read only memory (ROM) **902**, a random access memory (RAM) **903**, and a host bus **904a**. In addition, the eardrum temperature processing apparatus includes a bridge **904**, an external bus **904b**, an interface **905**, an input apparatus **906**, an output apparatus **907**, a storage apparatus (hard disk drive (HDD)) **908**, a drive **909**, a connection port **911**, and a communication apparatus **913**.

The CPU **901** functions as an arithmetic processing apparatus and a control apparatus, and controls the overall operation of the eardrum temperature processing apparatus according to various programs. In addition, the CPU **901** may be a microprocessor. The ROM **902** stores programs, arithmetic parameters, and the like for use by the CPU **901**. The RAM **903** temporarily stores a program for use in execution of the CPU **901** and parameters that change appropriately during the execution. These components are mutually connected through the host bus **904a** including a CPU bus or the like.

The host bus **904a** is connected to the external bus **904b** such as a peripheral component interconnect/interface (PCI) via the bridge **904**. The host bus **904a**, the bridge **904**, and the external bus **904b** are not necessarily configured separately, and these functions may be implemented by one bus.

The input apparatus **906** includes an input mechanism for allowing the user to input information such as a mouse, a keyboard, a touch panel, a button, a microphone, a switch, and a lever, an input control circuit for generating an input signal based on the user's input and outputting the generated input signal to the CPU **901**, and the like. The output apparatus **907**, for example, includes a liquid crystal display (LCD) apparatus, an organic light emitting diode (OLED) apparatus, a display apparatus such as a lamp, and a sound output apparatus such as a speaker.

The storage apparatus **908** is an example of the storage unit of the eardrum temperature processing apparatus, and is a data storage apparatus. The storage apparatus **908** can include a storage medium, a recording apparatus for recording data on the storage medium, a read apparatus for reading data from the storage medium, and an erasing apparatus for erasing data recorded on the storage medium. The storage apparatus **908**, for example, includes an HDD. This storage apparatus **908** drives a hard disk, and stores a program to be executed by the CPU **901** and various data.

The drive **909** is a reader/writer for the storage medium and embedded in the eardrum temperature processing apparatus or attached externally thereto. The drive **909** reads information recorded on a removable recording medium such as a magnetic disk, an optical disc, a magneto-optical disc or a semiconductor memory, and outputs the read information to the RAM **903**.

The connection port **911** is an interface connected to an external device, and, for example, is a connection port to an external device to which data can be transmitted using a USB or the like. In addition, the communication apparatus **913**, for example, is a communication interface including a communication device for connecting to a communication network **5** and the like. In addition, the communication apparatus **913** may be a communication apparatus corresponding to wireless LAN, a communication apparatus corresponding to wireless USB, or a wired communication apparatus that executes wired communication.

The preferred embodiments of the present disclosure have been described above with reference to the accompanying drawings, whilst the present disclosure is not limited to the above examples, of course. It should be understood by those skilled in the art that various modifications, combinations, sub-combinations and alterations may occur depending on design requirements and other factors insofar as they are within the scope of the appended claims or the equivalents thereof.

Additionally, the present technology may also be configured as below.

(1) An information processing apparatus including:
an eardrum recognition unit configured to recognize a position of an eardrum based on image information regarding the eardrum;

a temperature measurement unit configured to acquire a temperature within an external ear canal including the eardrum; and

a temperature processing unit configured to determine a temperature of the eardrum based on a recognition result of the eardrum recognition unit and a measured temperature of the temperature measurement unit.

(2) The information processing apparatus according to (1), wherein the image information regarding the eardrum is a captured image including the eardrum, and wherein the eardrum recognition unit recognizes the position of the eardrum based on the captured image.

(3) The information processing apparatus according to (2), including:

an imaging unit configured to acquire the image information regarding the eardrum.

(4) The information processing apparatus according to (1), wherein the image information regarding the eardrum is a thermal image including the eardrum,

wherein the eardrum recognition unit recognizes the position of the eardrum based on the thermal image, and

wherein the temperature measurement unit acquires a temperature within an ear canal including the eardrum based on the thermal image.

(5) The information processing apparatus according to (4), wherein acquisition of the image information regarding the eardrum and temperature measurement by the temperature measurement unit are performed by an identical device.

(6) The information processing apparatus according to any one of (1) to (5), including:

a notification unit configured to notify a user of eardrum information regarding the eardrum,

wherein the notification unit provides at least notification of a calculated temperature of the eardrum.

(7) The information processing apparatus according to (6), wherein the eardrum recognition unit calculates an eardrum occupancy rate representing a ratio occupied by the eardrum in a predetermined range in an image of the eardrum based on a recognition result of the image information regarding the eardrum, and

wherein the notification unit notifies the user of a position state of the temperature measurement unit with respect to the eardrum based on the eardrum occupancy rate.

(8) The information processing apparatus according to (7), wherein the notification unit notifies the user of a direction for adjusting the direction of the temperature measurement unit in a manner that the eardrum occupancy rate increases.

(9) The information processing apparatus according to any one of (1) to (8), further including:

a correction unit configured to correct the temperature of the eardrum calculated by the temperature processing unit,

wherein the eardrum recognition unit calculates an eardrum occupancy rate representing a ratio occupied by the eardrum in a predetermined range in an image of the eardrum based on a recognition result of the image information regarding the eardrum, and

wherein the correction unit corrects the temperature of the eardrum calculated by the temperature processing unit based on the eardrum occupancy rate.

(10) The information processing apparatus according to (9), wherein the correction unit corrects the temperature of the eardrum based on a correlation relationship between the eardrum occupancy rate and the temperature of the eardrum.

What is claimed is:

1. An information processing apparatus comprising:

an image sensor operable to capture an image of an eardrum;

a temperature sensor; and

a central processing unit (CPU) operable to:

acquire image information regarding the eardrum from the captured image of the eardrum;

determine a first area corresponding to a temperature measurable area of the temperature sensor in the captured image;

determine a second area occupied by the eardrum within the first area corresponding to the temperature measurable area of the temperature sensor based on the acquired image information;

calculate an eardrum occupancy rate, wherein the eardrum occupancy rate represents a ratio of the second area to the first area;

23

- acquire a temperature, within an external ear canal including the eardrum, measured by the temperature sensor; and
 determine a temperature of the eardrum based on, the calculated eardrum occupancy rate, and the acquired temperature. 5
2. The information processing apparatus according to claim 1,
 wherein the CPU recognizes a position of the eardrum based on the captured image. 10
3. The information processing apparatus according to claim 1,
 wherein the acquired image information regarding the eardrum is a thermal image including the eardrum,
 wherein the CPU recognizes a position of the eardrum based on the thermal image, and 15
 wherein the CPU acquires a temperature within the external ear canal including the eardrum based on the thermal image.
4. The information processing apparatus according to claim 3, wherein the CPU is operable to: 20
 acquire the image information regarding the eardrum and determine the temperature from the captured image of the eardrum, simultaneously.
5. The information processing apparatus according to claim 1, wherein the CPU is further operable to: 25
 notify a user of the acquired image information regarding the eardrum, wherein the CPU provides at least notification of the determined temperature of the eardrum.
6. The information processing apparatus according to claim 1, 30
 wherein the CPU notifies a user of a position state of the temperature sensor with respect to the eardrum based on the calculated eardrum occupancy rate.
7. The information processing apparatus according to claim 6, 35
 wherein the CPU notifies the user of a direction for adjusting the direction of the temperature sensor in a manner that the eardrum occupancy rate increases.
8. The information processing apparatus according to claim 1, wherein the CPU is operable to: 40
 correct the determined temperature of the eardrum,
 wherein the CPU corrects the determined temperature of the eardrum based on the calculated eardrum occupancy rate. 45
9. The information processing apparatus according to claim 8,

24

wherein the CPU corrects the determined temperature of the eardrum based on a correlation relationship between the calculated eardrum occupancy rate and the acquired temperature of the eardrum.

10. An information processing method comprising:
 capturing an image of an eardrum;
 acquiring image information regarding the eardrum from the captured image of the eardrum;
 determining a first area corresponding to a temperature measurable area of a temperature sensor in the captured image;
 determining a second area occupied by the eardrum within the first area corresponding to the temperature measurable area of the temperature sensor based on the acquired image information;
 calculating an eardrum occupancy rate, wherein the eardrum occupancy rate represents a ratio of the second area to the first area;
 acquiring a temperature, within an external ear canal including the eardrum, measured by the temperature sensor; and
 determining a temperature of the eardrum based on, the calculated eardrum occupancy rate, and the acquired temperature.
11. A non-transitory computer readable medium having stored thereon, a set of computer-executable instructions for causing the computer to perform steps comprising:
 capturing an image of an eardrum;
 acquiring image information regarding the eardrum from the captured image of the eardrum;
 determining a first area corresponding to a temperature measurable area of a temperature sensor in the captured image;
 determining a second area occupied by the eardrum within the first area corresponding to the temperature measurable area of the temperature sensor based on the acquired image information;
 calculating an eardrum occupancy rate, wherein the eardrum occupancy rate represents a ratio of the second area to the first area;
 acquiring a temperature, within an external ear canal including the eardrum, measured by the temperature sensor; and
 determining a temperature of the eardrum based on, the calculated eardrum occupancy rate, and the acquired temperature.

* * * * *

专利名称(译)	用于测量鼓膜温度的信息处理设备，信息处理方法和计算机程序		
公开(公告)号	US9259159	公开(公告)日	2016-02-16
申请号	US13/847113	申请日	2013-03-19
[标]申请(专利权)人(译)	索尼公司		
申请(专利权)人(译)	索尼公司		
当前申请(专利权)人(译)	索尼公司		
[标]发明人	TSUBOI TOSHIMITSU TANAKA AKICHIKA ASAKAWA TAKESHI SAZUKA NAOYA WADA SEIJI		
发明人	TSUBOI, TOSHIMITSU TANAKA, AKICHIKA ASAKAWA, TAKESHI SAZUKA, NAOYA WADA, SEIJI		
IPC分类号	A61B5/01 G01J5/00 A61B5/00 G01J5/08 G01J5/04		
CPC分类号	A61B5/01 A61B5/0059 A61B5/6817 G01J5/0011 G01J5/049 G01J5/089 G01J5/0896		
优先权	2012076046 2012-03-29 JP		
其他公开文献	US20130296685A1		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种信息处理装置，包括鼓膜识别单元，被配置为基于关于鼓膜的图像信息来识别鼓膜的位置；温度测量单元，被配置为获取包括鼓膜的外耳道内的温度；以及温度处理单元，被配置为基于所述鼓膜识别单元的识别结果和所述温度测量单元的测量温度来确定所述鼓膜的温度。

