




US 20180310881A1

(19) **United States**(12) **Patent Application Publication**
Yoon et al.(10) **Pub. No.: US 2018/0310881 A1**(43) **Pub. Date: Nov. 1, 2018**(54) **INTELLIGENT FITNESS AND SPORTS
MOUTHGUARD**(71) Applicant: **University of Florida Research
Foundation, Inc.**, Gainesville, FL (US)(72) Inventors: **Yong Kyu Yoon**, Gainesville, FL (US);
Justin M. Correll, Ann Arbor, MI
(US); **Todd R. Schumann**, Gainesville,
FL (US); **Sheng-Po Fang**, Beaverton,
OR (US); **Fong Wong**, Madison, WI
(US)*A61B 5/021* (2006.01)*A61F 5/56* (2006.01)*A63B 71/06* (2006.01)*A63B 71/08* (2006.01)*G16H 40/63* (2006.01)(52) **U.S. Cl.**CPC *A61B 5/682* (2013.01); *A61B 5/002*
(2013.01); *A61B 5/01* (2013.01); *A61B 5/021*
(2013.01); *A61B 5/02433* (2013.01); *A61F*
5/56 (2013.01); *A63B 71/0619* (2013.01);
A63B 71/085 (2013.01); *G16H 40/63*
(2018.01); *A61B 5/4557* (2013.01)(21) Appl. No.: **15/769,584**(22) PCT Filed: **Oct. 20, 2016**(86) PCT No.: **PCT/US2016/057908**

§ 371 (c)(1),

(2) Date: **Apr. 19, 2018****Related U.S. Application Data**(60) Provisional application No. 62/245,580, filed on Oct.
23, 2015.**Publication Classification**(51) **Int. Cl.***A61B 5/00* (2006.01)*A61B 5/01* (2006.01)(57) **ABSTRACT**

Various examples are provided for intelligent mouthguards that can be used in fitness and sport activities. In one example, an intelligent mouthguard system includes a mouthguard including sensors and an internal module in communication with the sensors. The sensors can include a nine-axis inertial sensor comprising a three-axis magnetometer, a three-axis accelerometer and a three-axis gyroscope. The three-axis magnetometer can provide a reference plane in relation to the earth's magnetic field for the three-axis accelerometer and the three-axis gyroscope. The internal module can provide sensor data to an external processing unit when located in an oral cavity.

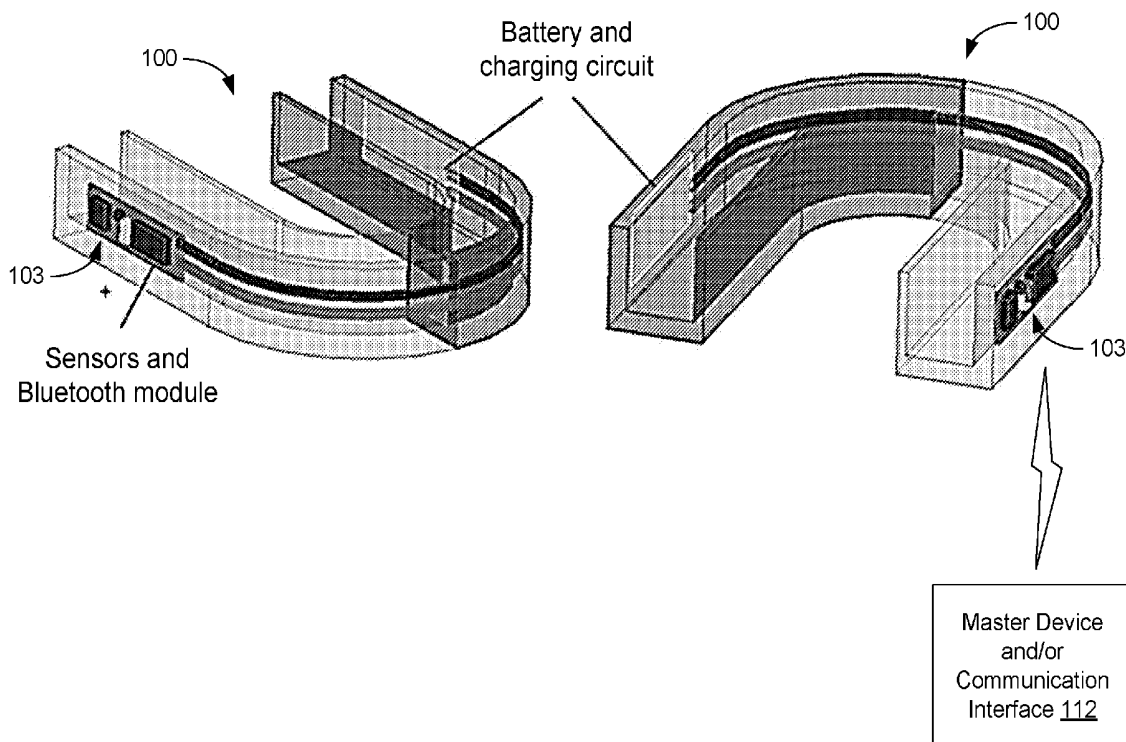

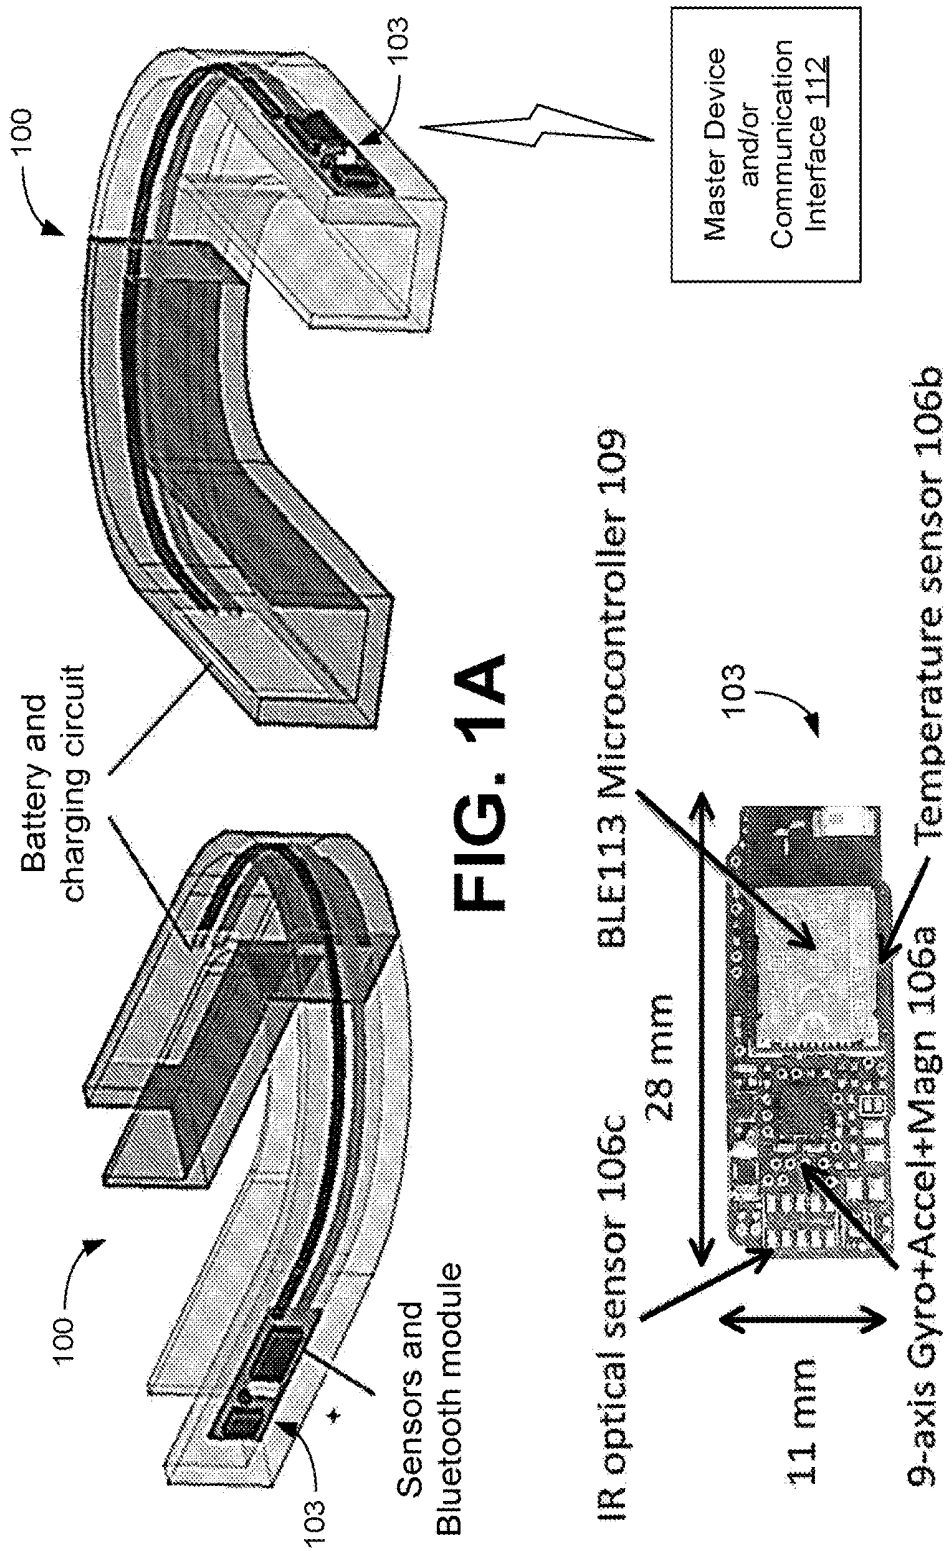


FIG. 1A

FIG. 1B

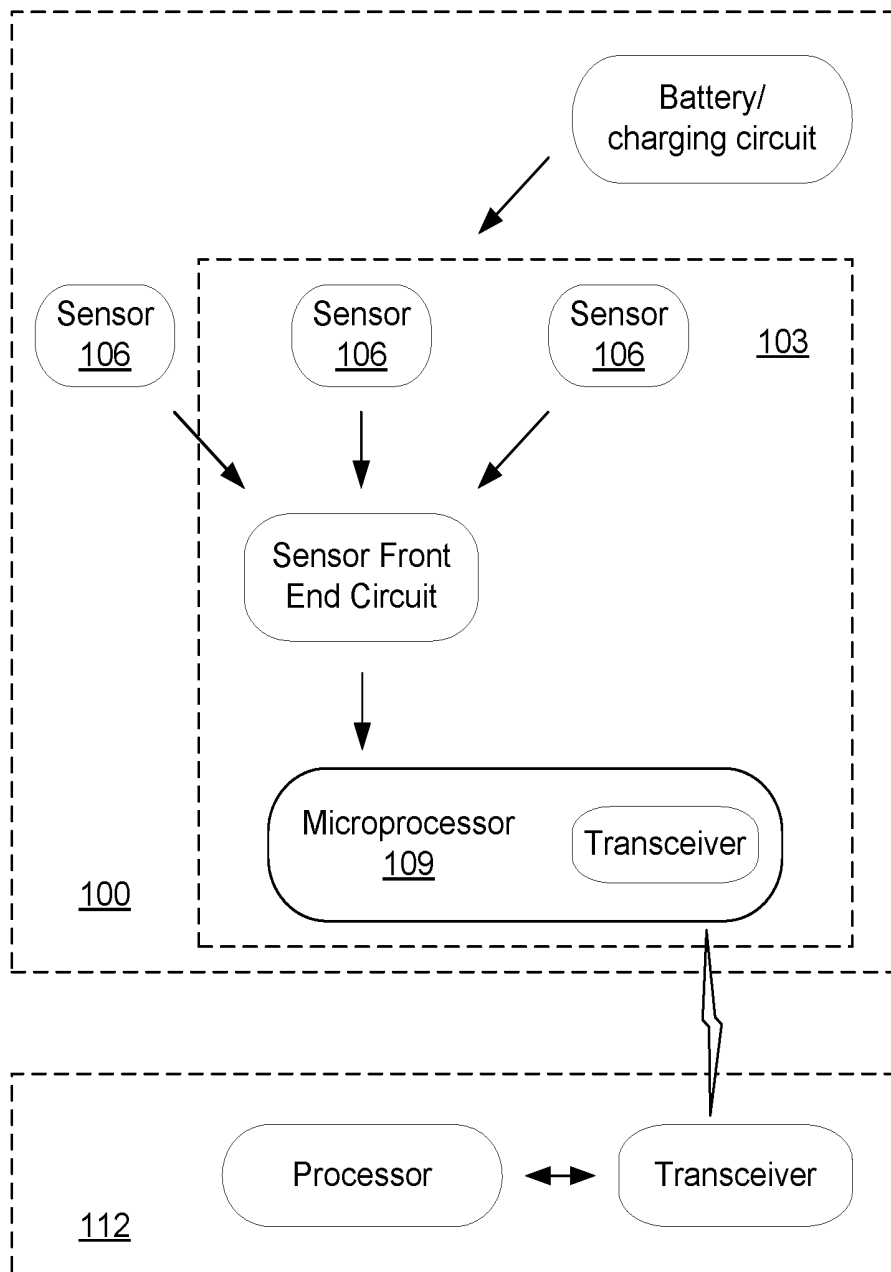


FIG. 1C

Customized Mouthguard General Mouthguard

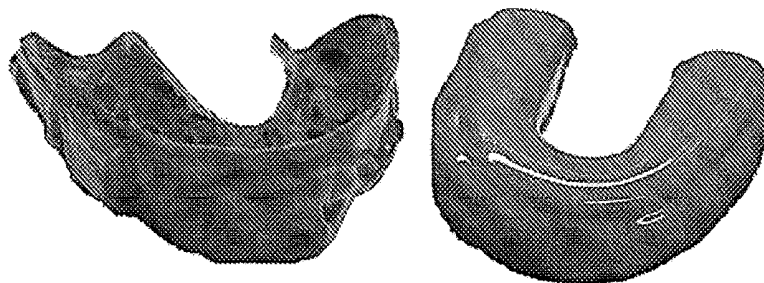


FIG. 1D

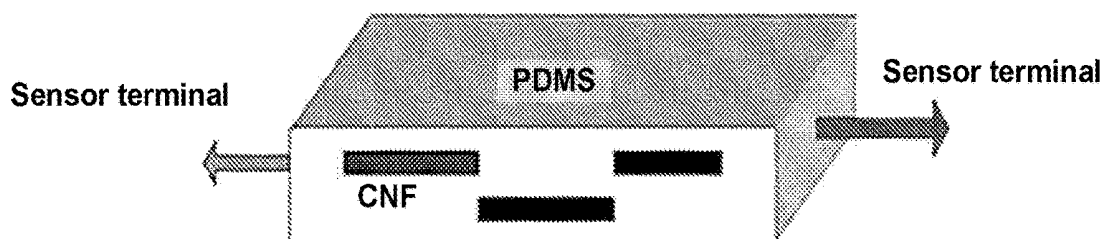


FIG. 2A

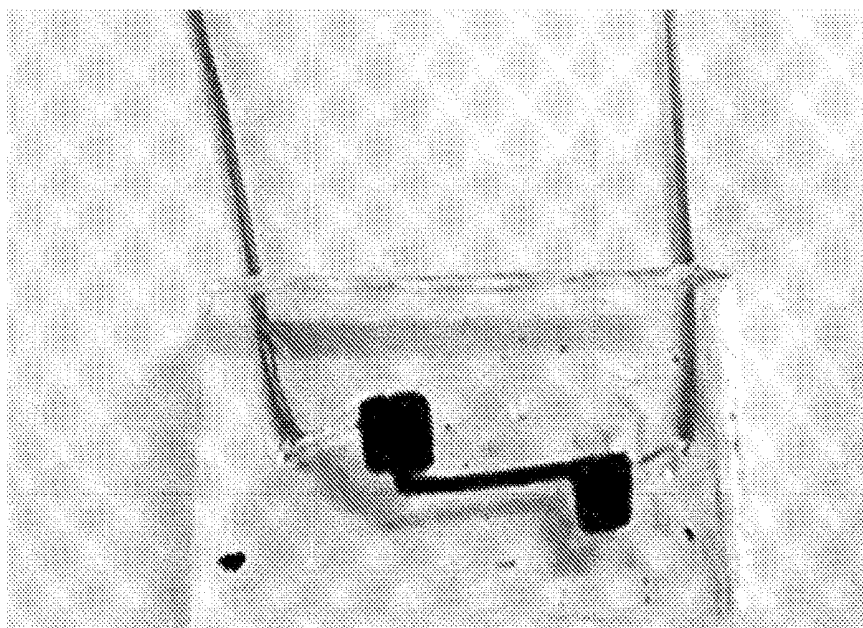
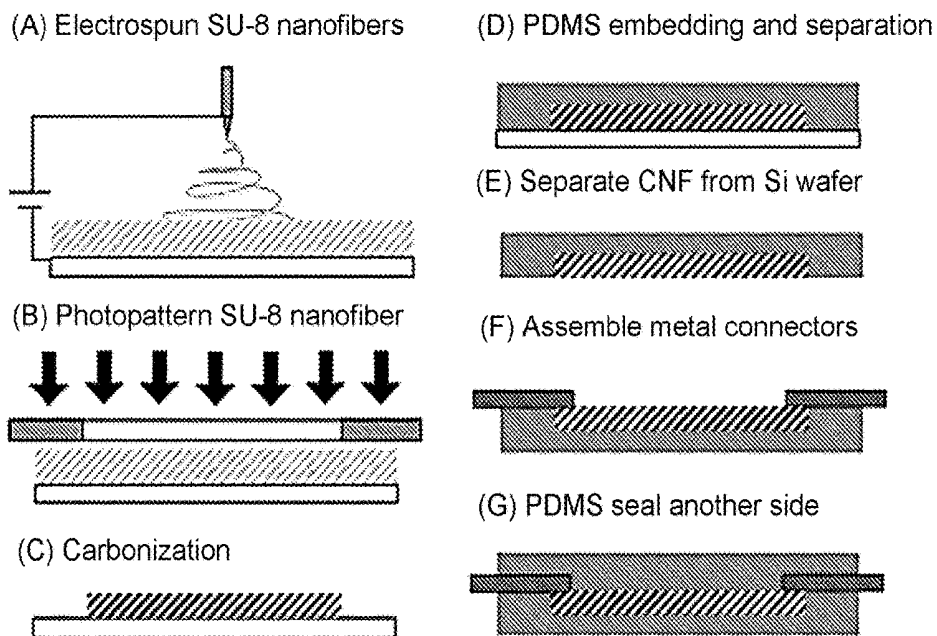
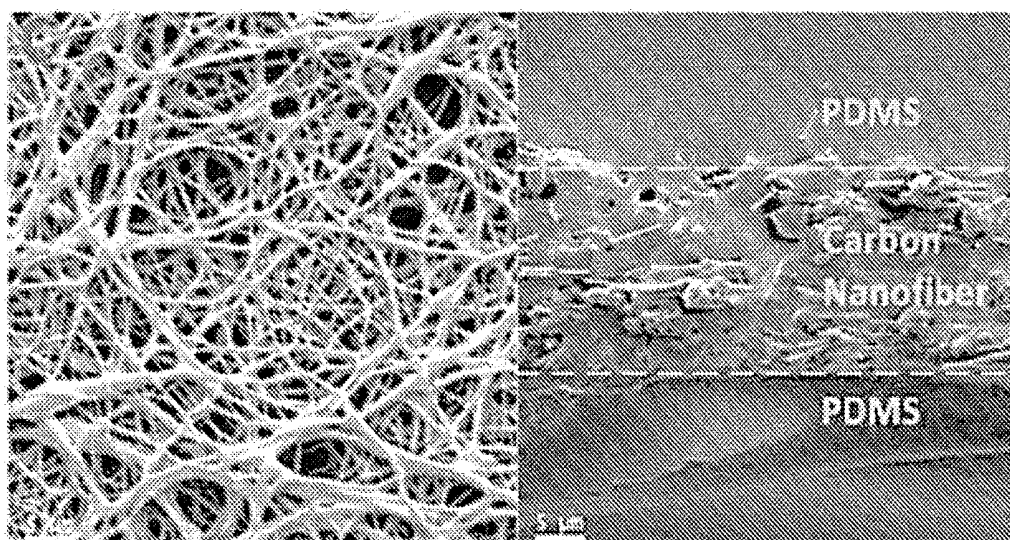


FIG. 2B

**FIG. 2C****FIG. 2D****FIG. 2E**

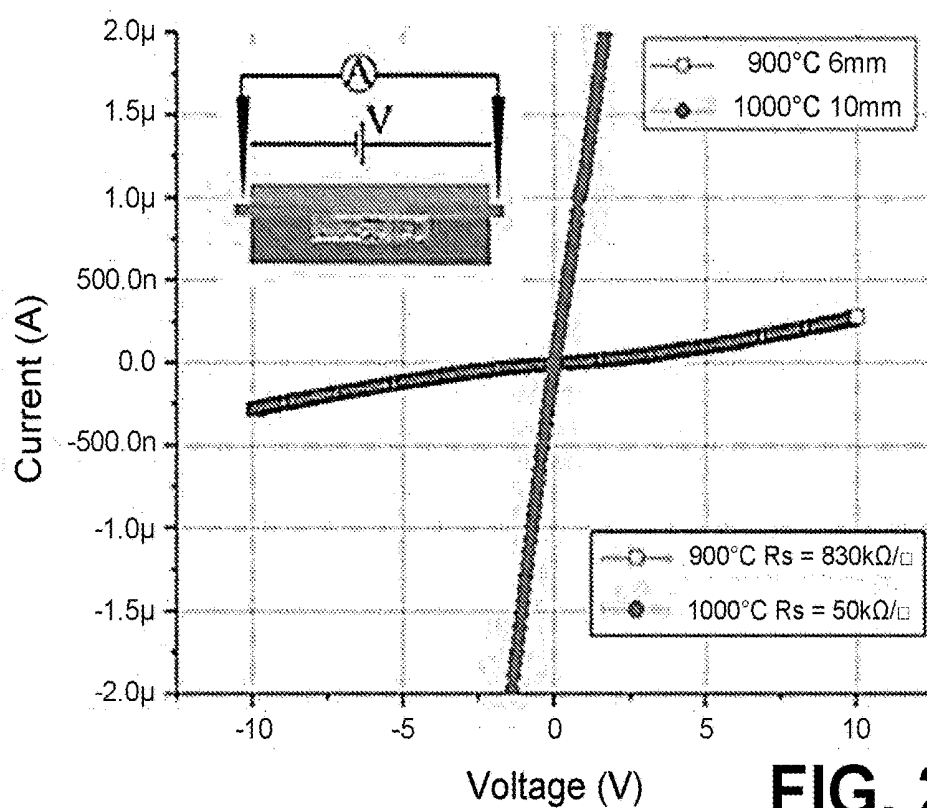


FIG. 2F

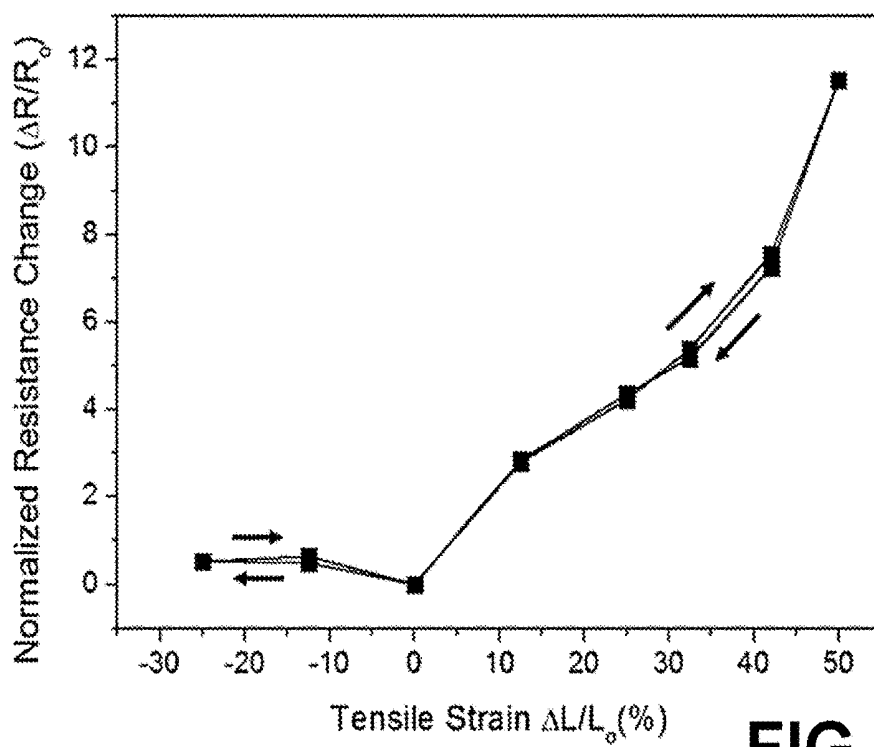


FIG. 2G

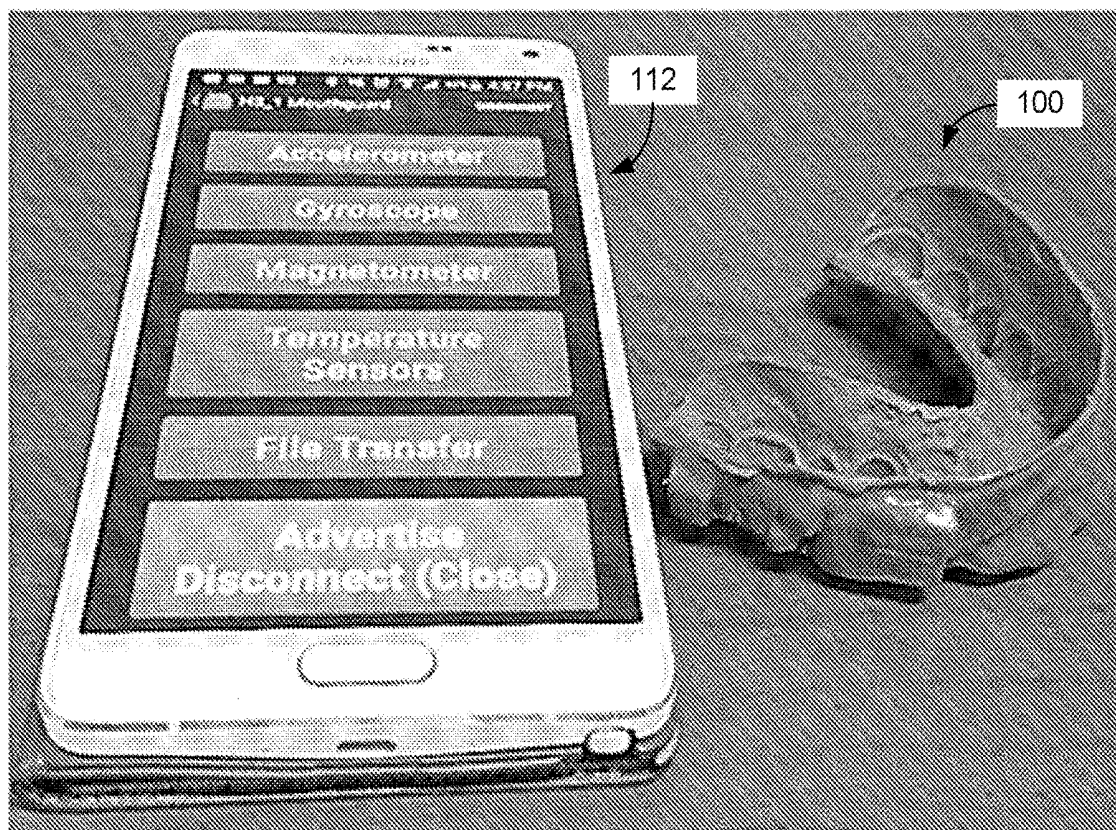


FIG. 3A

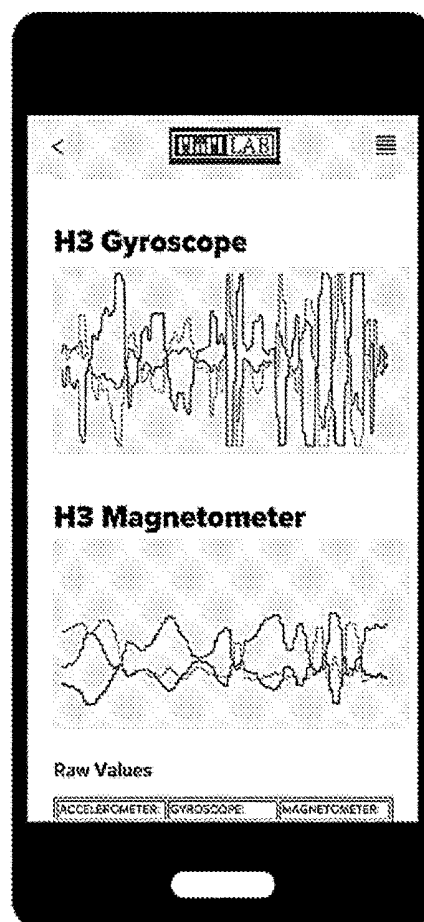


FIG. 3B

INTELLIGENT FITNESS AND SPORTS MOUTHGUARD

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to, and the benefit of, co-pending U.S. provisional application entitled “Intelligent Fitness and Sports Mouthguard” having Ser. No. 62/245,580, filed Oct. 23, 2015, the entirety of which is hereby incorporated by reference. This application is also related to co-pending U.S. patent application entitled “MULTIFUNCTIONAL ORAL PROSTHETIC SYSTEM” having Ser. No. 14/347,951, filed Mar. 27, 2014, the entirety of which is hereby incorporated by reference.

BACKGROUND

[0002] Concern has increased about injuries that occur during sporting activities. In particular, head traumas that can result in concussion have come under greater scrutiny. According to the US Centers for Disease Control and Prevention (CDC), more than 3.8 million sports brain injuries occur per year with 300 thousand resulting in loss of consciousness (LoC). These injuries are not limited to occurrence at the professional or collegiate level, but also include an estimated number of 250 thousand sports brain injuries occurring at the high school level. Diagnosis and treatment of such injuries can be enhanced by monitoring athletes during the sporting events.

SUMMARY

[0003] Embodiments of the present disclosure are related to intelligent mouthguards that can be used in fitness and sport activities.

[0004] In one embodiment, among others, an intelligent mouthguard system comprises a mouthguard including a nine-axis inertial sensor comprising a three-axis magnetometer, a three-axis accelerometer and a three-axis gyroscope, and an internal module in communication with the nine-axis inertial sensor. The three-axis magnetometer is configured to provide a reference plane in relation to the earth's magnetic field for the three-axis accelerometer and the three-axis gyroscope and the internal module is configured to provide sensor data corresponding to the three-axis magnetometer, the three-axis accelerometer and the three-axis gyroscope to an external processing unit when located in an oral cavity, and the external processing unit communicatively coupled to the mouthguard. In one or more aspects of these embodiments, the external processing unit can be a master device communicatively coupled to the mouthguard via a Bluetooth® link. The master device can be a smartphone. The master device can be configured to provide an indication of acceleration experienced by a wearer of the mouthguard through a user interface rendered on the master device. The master device can be configured to adjust the acceleration based upon the reference plane provided by the three-axis magnetometer.

[0005] In one or more aspects of these embodiments, the external processing unit can be a communication interface module communicatively coupled to the mouthguard and communicatively coupled to a remotely located processing device. The communication interface module can be communicatively coupled to the mouthguard via a Bluetooth® link and communicatively coupled to the remotely located

processing device via a WLAN link. The internal module can be configured to transmit the sensor data from the three-axis magnetometer, the three-axis accelerometer and the three-axis gyroscope to the external processing unit. The sensor data can be transmitted to the external processing unit in real-time. The internal module can transmit the sensor data to the external processing unit from memory in response to a transmission request received from the external processing unit.

[0006] In one or more aspects of these embodiments, the intelligent mouthguard system comprises a temperature sensor. The intelligent mouthguard system comprises an infrared (IR) sensor, wherein heart rate or blood pressure can be determined based upon sensor data from the IR sensor. The intelligent mouthguard system comprises a strain gauge sensor sealed in the mouthguard. The strain gauge sensor can comprise a polydimethylsiloxane (PDMS) and carbon nanofiber (CNF) composite sensing element. The sensing element can comprise electrospun polymer derived conductive carbon nanofiber (EPD-CNF) sealed in polydimethylsiloxane (PDMS).

[0007] Other systems, methods, features, and advantages of the present disclosure will be or become apparent to one with skill in the art upon examination of the following drawings and detailed description. It is intended that all such additional systems, methods, features, and advantages be included within this description, be within the scope of the present disclosure, and be protected by the accompanying claims. In addition, all optional and preferred features and modifications of the described embodiments are usable in all aspects of the disclosure taught herein. Furthermore, the individual features of the dependent claims, as well as all optional and preferred features and modifications of the described embodiments are combinable and interchangeable with one another.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] Many aspects of the present disclosure can be better understood with reference to the following drawings. The components in the drawings are not necessarily to scale, emphasis instead being placed upon clearly illustrating the principles of the present disclosure. Moreover, in the drawings, like reference numerals designate corresponding parts throughout the several views.

[0009] FIGS. 1A, 1B, and 1C illustrate an example of an intelligent mouthguard, in accordance with various embodiments of the present disclosure.

[0010] FIG. 1D includes images of examples of custom and general intelligent mouthguards, in accordance with various embodiments of the present disclosure.

[0011] FIGS. 2A and 2B illustrate an example of a composite material strain gauge sensor, in accordance with various embodiments of the present disclosure.

[0012] FIG. 2C illustrates an example of fabrication of a strain gauge sensor using electrospun polymer derived conductive carbon nanofiber (EPD-CNF) and polydimethylsiloxane (PDMS), in accordance with various embodiments of the present disclosure.

[0013] FIGS. 2D and 2E are images of the carbon nanofiber embedded in the PDMS, in accordance with various embodiments of the present disclosure.

[0014] FIGS. 2F and 2G illustrate test results of the EPD-CNF/PDMS strain sensor, in accordance with various embodiments of the present disclosure.

[0015] FIGS. 3A and 3B illustrate a prototype mouthguard of FIGS. 1A and 1B, and master device in communication with the mouthguard, in accordance with various embodiments of the present disclosure.

DETAILED DESCRIPTION

[0016] Disclosed herein are various embodiments related to an intelligent mouthguard for fitness and sport activities. Reference will now be made in detail to the description of the embodiments as illustrated in the drawings, wherein like reference numbers indicate like parts throughout the several views.

[0017] In this Internet of Things (IoT) era, there is a great deal of interest in wearable devices with wireless functionality that are networked together to provide up-to-date real-time data to a central hub such as a cell phone, personal computer, or network server. The device presented here is a smart mouthguard platform with 11 sensor channels and a friendly user interface. The mouthguard platform is targeted for use in all fitness and sports activities where the user is interested in monitoring their biometric data from physical activity and their potential exposure to life threatening (head, heat, and heart related) injury. The oral cavity is a region that offers easy access and noninvasive device placement. Further, the same platform can be extended for use in bruxism monitoring and intervention. The smart mouthguard can provide real-time feedback to the user(s) or a designated official or healthcare professional. In the case of bruxism, it offers the ability to implement intervention mechanisms such as a muscle massager, heating pad and/or behavior modification through biofeedback.

[0018] The devices focus on providing a holistic approach to health monitoring by using an array of sensors to cover a complete application instead of a single sensor. For example, the sports mouthguard can implement a 9-axis inertial sensor and pressure sensors to detect dangerous force levels to which the head is subjected to, an infrared (IR) sensor for heart pulse rate and osmolality monitoring, and a temperature sensor to detect dangerous rises in core body temperature. A bruxism mouthguard can implement different sensitivity pressure sensors to detect biting force from “chattering” to clenching, an inertial sensor to detect restlessness, and a thermistor to detect rises in body temperature.

[0019] Referring to FIG. 1A, shown is a graphical representation illustrating an example of an intelligent mouthguard 100 including sensors, a battery, charging and wireless electronics circuitry. The intelligent mouthguard system comprises a printed circuit board 103 embedded in a mouthguard 100 and a software application that enables low-energy wireless communications (e.g., Bluetooth®, WiFi, WLAN, etc.) between the electronics in the mouthguard 100 and an external hub or server. Referring to FIG. 1B, shown is an example of the printed circuit board 103, which contains a plurality of sensors 106 (e.g., a 9-axis inertial sensor 106a, a temperature sensor 106b, an infrared (IR) optical sensor 106c, etc.) used to track user activity and/or condition. A microcontroller 109 can be configured to communicate with each of the sensors and to communicate various information to the external hub or server.

[0020] The biometric data collected from the sensor can provide the user with biometric information from physical activity and exposure to head, heat, and heart-related injuries. The software application can provide a unique user

interface to interact with the mouthguard 100 and to display the acquired biometric data and injury exposure information. Further, the software application can be connected to a back-end server interface located on a remote storage device.

[0021] In the example of FIG. 1B, the printed circuit board 103 comprises an ARM Cortex microprocessor 109 with an integrated Bluetooth Low Energy (BLE) 2.4 GHz transceiver such as the Silicon Labs Blue Gecko BGM111. The Bluetooth Special Interest group outlines the communication protocol employed by BLE enabled devices as a master—peripheral relationship. In this case, the ARM Cortex BLE microprocessor 109 fulfills the peripheral role and collects the data from several sensors 106 located on the circuit board 103. The data can be transmitted to an external processing unit 112 such as a master device, e.g., a more powerful smart phone (Android or iPhone), tablet, laptop computer, or other computing device, where it can be processed and/or provided for display, or a communication interface module that can forward the data to a remotely located processing device for processing, display and/or storage. In this setup, the printed circuit board 103 maintains the smallest electrical footprint to be sufficient for integration into the mouthguard 100. This mouthguard platform provides for non-invasive and easy access to a number of biological markers and/or signals via, for example, salivary analysis.

[0022] Referring next to FIG. 10, shown is an example of a sensor network of a intelligent mouthguard 100. Signals from one or more sensors 106 mounted on the printed circuit board 103 and/or in the mouthguard 100 may be received by a sensor front end circuit (e.g., a MUX/ADC) for processing by the microprocessor 109. The microprocessor 109 can provide the acquired sensor data to the master device 112 through a transceiver, which may be integrated into the microprocessor 109 or may be a separate device. The printed circuit board 103 and/or microprocessor 109 can include memory to store sensor data for subsequent transmission to the master device 112 and/or code or instructions that may be executed by the microprocessor 109. The master device 112 includes a transceiver that receives the transmitted sensor information and provides it to a processor for analysis and processing. Transmission between the mouthguard 100 and the master device 112 may be over a wireless communications link (e.g., Bluetooth®, WiFi, WLAN, etc.).

[0023] The mouthguard 100 can also be referred to as the H³ mouthguard as it deals with head, heat, and heart-related injuries. The mouthguard 100 is a multifunctional smart oral platform that offers real time biometric monitoring including potential danger detection and real time compliance reporting. FIG. 1D shows examples of customized and general mouthguards 100 with the printed circuit board 103, sensors, battery, and charging circuitry encased in a protective coating. The mouthguard 100 can be loaded with 11 sensor nodes which track various biomarkers such as, e.g., core body temperature, heart rate, blood pressure, and impact parameters. The system application can be extended by the addition of pressure sensors to find applications in bruxism monitoring.

[0024] 9-axis Inertial Sensors. The 9-axis inertial sensor 106a of FIG. 1B can include a 3-axis accelerometer, a 3-axis gyroscope, and a 3-axis magnetometer such as in an InvenSense MPU-9250. The accelerometer can provide gravitational force data, the gyroscope can provide rota-

tional data about an axis, and the magnetometer can provide a reference plane in relation to the earth's magnetic field. Together, the 9-axis of data can be used to create a three-dimensional (3-D) mapping of the mouthguard **100** that tracks the forces and direction of perturbations that the user experiences during physical activity. Both magnitude and direction of an impact force on the head can be detected and recorded.

[0025] Temperature Sensor. The temperature sensor **106b** of FIG. 1B can be, e.g., a diode type located in the microcontroller silicon, an external low-power temperature sensor such as the Texas Instruments LM94022 multi-gain sensor, or other appropriate type of temperature sensor. The LM94022 is well suited to source the input of a sample and hold analog-to-digital converter (ADC) signals similar to the analog inputs on the Silicon Labs BGM111. The temperature sensor can be implemented to record oral temperatures, providing potential heat related injury alerts in advance. The mouthguard **100** is not limited to only analog temperature sensors but could be loaded with a digital sensor with serial output. The mouthguard **100** is not limited to a single sensor, but can use several sensors to provide a differential measurement to improve accuracy in identifying the user's core body temperature.

[0026] Heart Rate and Blood Pressure Sensor. An infrared (IR) sensor **106c** such as the Silicon Labs Si1147 can be used to provide heart rate and blood pressure measurements using photoplethysmography (PPG), an optical technique that detects blood volume changes in microvascular tissues. The Si1147 comprises an IR LED and a CMOS ambient light sensor module. A portion of the infrared light projected into microvascular tissue is absorbed. Further, as the microvascular tissues expand and contract, the IR absorption changes. The ambient light sensor captures the changes and an algorithm can be used to resolve the data into a heart rate and blood pressure measurement. The IR sensor information can be used to track body condition and fitness level, which can be evaluated in real-time or stored (e.g., in the smartphone) for subsequent access.

[0027] Capacitive Pressure Sensor. The mouthguard **100** can include pressure sensors, such as capacitors with a compressible dielectric layer. As a force is applied, the effective thickness of the dielectric layer changes causing a change in capacitance. This change can be measured by detecting a change in the time constant for an RC circuit or the center frequency of an LC circuit and the relative force can be extracted. These sensors are linear for a limited range of force, and so sensors with different deflection coefficients can be used to create an array of sensors which can linearly measure the entire range of biting force for either bruxism or impact force for concussion detection.

[0028] Strain Gauge Pressure Sensor. The mouthguard **100** can also include a strain gauge pressure sensor, which can be used for biting force measurement. Biting during Bruxism produces a pressure of about 100 lbs to 200 lbs (or about 2000 kPa). Hence, the sensor should be able to withstand this pressure level with a reasonable resolution. For the strain gauge sensor, various options are available. For example, two options include:

[0029] A commercially available strain gauge sensor like a match stick type strain gauge, such as a pressure sensor like SCP 100 (120 kPa range) from VTI technologies, and pressure membrane.

[0030] An engineered composite material made of polydimethylsiloxane (PDMS) and carbon nanofiber (CNF) considering size constraints and biocompatibility issues is used. FIG. 2A is a schematic diagram illustrating the PDMS/CNF sensor and FIG. 2B is an image showing a fabricated PDMS/CNF sensor.

[0031] In some implementations, the PDMS/CNF sensor or FIG. 2B can be made of electrospun polymer (e.g., SU-8) derived conductive carbon nanofiber (EPD-CNF) and PDMS. This EPD-CNF/PDMS composite exhibits strong piezoresistivity that translates into excellent sensitivity with an extremely high gauge factor of 23.1, which is about 12-30 times higher than produced by graphene nanoribbon or carbon nanotube based nanocomposite sensors. The EPD-CNF/PDMS composite offers a low cost, high sensitivity sensor that can be manufactured and incorporated into the mouthguard **100**. The composite remains intact under high mechanical strain, such as occurs during use, which may be attributed to the continuous and tangled electrospun nanofibers in the sensor. The strain sensor can be embedded in a side or bottom surface of the mouthguard **100** and communicatively coupled to the microprocessor **109** on the printed circuit board **103**.

[0032] FIG. 2C illustrates an example of the fabrication of the composite sensor. Initially, SU-8 nanofibers can be electrospun (A) on a silicon (Si) wafer and patterned (B) using photolithography. Men deposited, the electrospun nanofibers form a continuous and randomly oriented layer that form a microscale spring. Carbonization (C) of the electrospun nanofibers enables the formation of stretchable conductive EPD-CNF within the embedding elastomers. The EPD-CNF can then be partially embedded (D) in PDMS and separated (E) from the Si wafer. Connectors can be assembled (F) on the EPD-CNF, which are then sealed (G) in PDMS as shown. FIG. 2D is a scanning electron microscope (SEM) image of carbonized nanofibers and FIG. 2E shows a cross-sectional view of the EPD-CNF embedded within the PDMS.

[0033] FIG. 2F shows the measured current-voltage (I-V) curves for strain sensors of FIG. 2B including EPD-CNFs that were carbonized at 900° C. and 1000° C. The measuring setup is shown in inset of FIG. 2F. The extracted sheet resistances (R_s) of those carbonized nanofibers at 900° C. and 1000° C. were 830 k $\Omega/\square$ and 50 k $\Omega/\square$, respectively, where $\Omega/\square$ is ohms per square. FIG. 2G shows a measured gauge factor ($GF = \Delta R/R \in$) of 23.1 with 50% strain at room temperature. The strain range can be further improved by optimizing the PDMS thickness.

[0034] Wireless Power Delivery. As shown in FIG. 1A, the mouthguard **100** can include a battery and charging circuit for wireless power delivery to the circuit board **103**. Power can be delivered between a transmitter and a receiver located in the mouthguard **100** by inductive coupling between the antennas **809**. The charging circuit can be part of a wireless power delivery system configured to supply power to the battery through inductive coupling. The delivered power may then be regulated by the charging circuit for delivery to loads on the circuit board **103** and/or sensors in the mouthguard **100**. For example, BQ500110 and BQ51013 ICs from Texas Instruments Inc. may be used as the transmitter and the receiver, respectively, with near field power coupling provided through antennas. Since the BQ500110 and

BQ51013 ICs are highly integrated chips, nearly no peripherals are needed on the mouthguard **100** for power collection.

[0035] Long Distance Communication. The mouthguard **100** can be extended to support team applications. A software application deployed on a trainer's tablet (or other computing device) can communicate with and take measurements from a plurality of mouthguards **100** by pinging each individually to transfer their data to prevent channel crowding. The microcontroller **109** can transfer data to internal memory and/or external memory on the circuit board **103** during acquisition, and then transfer the stored information in response to the ping requesting transfer.

[0036] In the case of long distance transmission, the 434 MHz or 915 MHz ISM frequency bands can be used to implement a multi-layer system that includes an additional wireless module. The communication interface module **112** can either be located in the player's helmet or other equipment worn by the player, or integrated into the players clothing. Further, an external patch, which can be secured to the equipment and/or player, could be used for implementation of the communication interface module **112**. The additional wireless module or communication interface **112** (external) can communicate using both 2.4 GHz (to mouthguard **100**) and ISM bands (434 MHz or 915 MHz) as a virtual waypoint between the close range mouthguard **100** and externally located transceiver module located on the sideline or in coach's booth.

[0037] Referring to FIG. 3A, shown is an image of a prototype mouthguard **100** and a smartphone acting as the master device **112**. The image shows example of an interface of the system application that is implemented on the smartphone. As shown in FIG. 3A, the interface allows a user to access the sensor information (e.g., accelerometer, gyroscope, magnetometer, temperature sensors, etc.). FIG. 3B illustrates an example of the sensor information that can be displayed on the master device. The information (e.g., biometric data) can be displayed in graphs through a user friendly mobile app for iOS or Android systems. The interface can also facilitate file transfer of the recorded sensor information from the mouthguard **100** to the master device **112** or to another externally located processing device, as described above. The interface can also allow the master device **112** to be disconnected from the mouthguard **100**, allowing another device to connect as the master device.

[0038] The intelligent mouthguard **100** utilizes wearable electronics as part of a self-fitness monitoring system with wireless connectivity. Wearable electronics for fitness and wellness can help individuals monitor physical activity, diet, and sleep with continuous updates of biometric data. The mouthguard **100** can include a detection mechanism that can provide awareness of vital signs and potential sustained injury. The design and fabrication of the H³ (Head, Heat, and Heart-Related) mouthguard platform with **11** sensor channels and a friendly user interface has been presented. The device can be used in all sports or fitness activities where the user is interested in their biometric data from physical activity and their potential exposure to life threatening (head) injury. The H³ mouthguard platform is not limited to applications in sports fitness and wellness, but could find similar applications in the public safety (firefighter) and military sectors.

[0039] The concept can be further extended to a smart denture or retainer with a detection capability of diabetes,

HIV, and cancer biomarkers from saliva and an integrated drug delivery functionality. In addition, as the mouthguard **100** is in good contact with saliva, which contains lots of biomarkers for health and disease monitoring and detection, the H³ mouthguard **100** can be extended to be used as a general health monitoring and intervention tool.

[0040] The H³ mouthguard **100** offers a multifunctional smart oral platform with real time biometric monitoring that includes potential danger detection and real time compliance report. The mouthguard **100** can be loaded with a plurality of sensor nodes, which track core body temperature, heart rate, blood pressure, impact parameters and/or other biometric indications. A temperature sensor **106b** (FIG. 1B) can be used to measure the body temperature inside the mouth, eliminating inaccuracies found in common external wearable devices that arise from the temperature gradient between the skin and environment. An infrared sensor **106c** (FIG. 1B) can be included to provide heart rate and blood pressure measurements using photoplethysmography (PPG), an optical technique that detects blood volume changes in microvascular tissues. Impact parameters can be tracked using a 9-axis inertial sensor **106a** (FIG. 1B) including a 3-axis accelerometer, 3-axis gyroscope, and 3-axis magnetometer. The 3-axis magnetometer uses the earth's magnetic field to allow the sensing algorithm to compensate for drift errors over longer periods of time thus providing a more accurate measurement of impacts from a lateral force and angular momentum. The H³ mouthguard **100** development includes electronics and firmware design, form factor integration, and software development. The device can provide accurate biometric analysis that can inform the user of their fitness level and exposure to risk of heat or impact related injuries. Functionalities include head impact detection (e.g., serious impact alerts and/or long term impact tracking), body temperature monitoring (e.g., potential injury alerts such as for heat stroke or dehydration), and vital sign tracking (e.g., personal fitness tracking).

[0041] It should be emphasized that the above-described embodiments of the present disclosure are merely possible examples of implementations set forth for a clear understanding of the principles of the disclosure. Many variations and modifications may be made to the above-described embodiment(s) without departing substantially from the spirit and principles of the disclosure. All such modifications and variations are intended to be included herein within the scope of this disclosure and protected by the following claims.

[0042] It should be noted that ratios, concentrations, amounts, and other numerical data may be expressed herein in a range format. It is to be understood that such a range format is used for convenience and brevity, and thus, should be interpreted in a flexible manner to include not only the numerical values explicitly recited as the limits of the range, but also to include all the individual numerical values or sub-ranges encompassed within that range as if each numerical value and sub-range is explicitly recited. To illustrate, a concentration range of "about 0.1% to about 5%" should be interpreted to include not only the explicitly recited concentration of about 0.1 wt % to about 5 wt %, but also include individual concentrations (e.g., 1%, 2%, 3%, and 4%) and the sub-ranges (e.g., 0.5%, 1.1%, 2.2%, 3.3%, and 4.4%) within the indicated range. The term "about" can include traditional rounding according to significant figures of

numerical values. In addition, the phrase “about ‘x’ to ‘y’” includes “about ‘x’ to about ‘y’”.

1. An intelligent mouthguard system, comprising:
a mouthguard including:
a nine-axis inertial sensor comprising a three-axis magnetometer, a three-axis accelerometer and a three-axis gyroscope, the three-axis magnetometer configured to provide a reference plane in relation to the earth's magnetic field for the three-axis accelerometer and the three-axis gyroscope; and
an internal module in communication with the nine-axis inertial sensor, the internal module configured to provide sensor data corresponding to the three-axis magnetometer, the three-axis accelerometer and the three-axis gyroscope to an external processing unit when located in an oral cavity, the external processing unit communicatively coupled to the mouthguard.
2. The intelligent mouthguard system of claim 1, wherein the external processing unit is a master device communicatively coupled to the mouthguard via a Bluetooth® link.
3. The intelligent mouthguard system of claim 2, wherein the master device is a smartphone.
4. The intelligent mouthguard system of claim 2, wherein the master device is configured to provide an indication of acceleration experienced by a wearer of the mouthguard through a user interface rendered on the master device.
5. The intelligent mouthguard system of claim 4, wherein the master device is configured to adjust the acceleration based upon the reference plane provided by the three-axis magnetometer.
6. The intelligent mouthguard system of claim 1, wherein the external processing unit is a communication interface module communicatively coupled to the mouthguard and communicatively coupled to a remotely located processing device.

7. The intelligent mouthguard system of claim 6, wherein the communication interface module is communicatively coupled to the mouthguard via a Bluetooth® link and communicatively coupled to the remotely located processing device via a WLAN link.

8. The intelligent mouthguard system of claim 1, wherein the internal module is configured to transmit the sensor data from the three-axis magnetometer, the three-axis accelerometer and the three-axis gyroscope to the external processing unit.

9. The intelligent mouthguard system of claim 8, wherein the sensor data is transmitted to the external processing unit in real-time.

10. The intelligent mouthguard system of claim 8, wherein the internal module transmits the sensor data to the external processing unit from memory in response to a transmission request received from the external processing unit.

11. The intelligent mouthguard system of claim 1, further comprising a temperature sensor.

12. The intelligent mouthguard system of claim 1, further comprising an infrared (IR) sensor, wherein heart rate or blood pressure can be determined based upon sensor data from the IR sensor.

13. The intelligent mouthguard system of claim 1, further comprising a strain gauge sensor sealed in the mouthguard.

14. The intelligent mouthguard system of claim 13, wherein the strain gauge sensor comprises a polydimethylsiloxane (PDMS) and carbon nanofiber (CNF) composite sensing element.

15. The intelligent mouthguard system of claim 14, wherein the sensing element comprises electrospun polymer derived conductive carbon nanofiber (EPD-CNF) sealed in polydimethylsiloxane (PDMS).

* * * * *

专利名称(译)	智能健身和运动护齿		
公开(公告)号	US20180310881A1	公开(公告)日	2018-11-01
申请号	US15/769584	申请日	2016-10-20
[标]申请(专利权)人(译)	佛罗里达大学研究基金会有限公司		
申请(专利权)人(译)	佛罗里达州研究基金会，Inc.的大学.		
[标]发明人	YOON YONG KYU CORRELL JUSTIN M SCHUMANN TODD R FANG SHENG PO WONG FONG		
发明人	YOON, YONG KYU CORRELL, JUSTIN M. SCHUMANN, TODD R. FANG, SHENG-PO WONG, FONG		
IPC分类号	A61B5/00 A61B5/01 A61B5/021 A61F5/56 A63B71/06 A63B71/08 G16H40/63		
CPC分类号	A61B5/682 A61B5/002 A61B5/01 A61B5/021 A61B5/4557 A61F5/56 A63B71/0619 A63B71/085 G16H40/63 A61B5/02433 A61B2503/10 A61B2562/0219 A61B2562/0223 A61B2562/0261 A61B2562 /0285 A61F2005/563 A63B2225/52 A61B5/0002 A61B5/02055 A61B5/02416 A61B2562/0214 A61B2562/06 A61B2562/12		
优先权	62/245580 2015-10-23 US		
外部链接	Espacenet USPTO		

摘要(译)

提供了可用于健身和运动活动的智能护齿器的各种示例。在一个示例中，智能护口器系统包括护口器，护口器包括传感器和与传感器通信的内部模块。传感器可包括九轴惯性传感器，其包括三轴磁力计，三轴加速度计和三轴陀螺仪。三轴磁力计可以为三轴加速度计和三轴陀螺仪提供与地球磁场相关的参考平面。当位于口腔中时，内部模块可以向外部处理单元提供传感器数据。

