



US009913589B2

(12) **United States Patent**
Scharf et al.

(10) **Patent No.:** **US 9,913,589 B2**
(45) **Date of Patent:** ***Mar. 13, 2018**

(54) **DEVICE AND METHOD FOR THE GEOMETRIC DETERMINATION OF ELECTRICAL DIPOLE DENSITIES ON THE CARDIAC WALL**

(52) **U.S. Cl.**
CPC **A61B 5/04012** (2013.01); **A61B 5/0402** (2013.01); **A61B 5/044** (2013.01);
(Continued)

(71) Applicant: **Christoph Scharf**, Zurich (CH)

(58) **Field of Classification Search**
CPC **A61B 5/04005**; **A61B 5/0402**
See application file for complete search history.

(72) Inventors: **Christoph Scharf**, Zurich (CH);
Gunter Scharf, Zurich (CH)

(56) **References Cited**

(73) Assignee: **Christoph Scharf** (CH)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

5,555,883 A 9/1996 Avitall
5,601,084 A 2/1997 Sheehan et al.
(Continued)

This patent is subject to a terminal disclaimer.

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **15/333,378**

CA 2829626 9/2012
CN 201223445 4/2009
(Continued)

(22) Filed: **Oct. 25, 2016**

OTHER PUBLICATIONS

(65) **Prior Publication Data**

US 2017/0100049 A1 Apr. 13, 2017

Japanese Office Action dated Jan. 31, 2017 issued in corresponding Japanese Application No. 2013-557926, together with the English translation.

(Continued)

Related U.S. Application Data

(63) Continuation of application No. 14/886,449, filed on Oct. 19, 2015, now Pat. No. 9,504,395, which is a
(Continued)

Primary Examiner — Eric D. Bertram

(74) *Attorney, Agent, or Firm* — Onello & Mello, LLP

(30) **Foreign Application Priority Data**

Jan. 17, 2008 (CH) 0068/08


(57) **ABSTRACT**

Disclosed are devices, a systems, and methods for determining the dipole densities on heart walls. In particular, a triangularization of the heart wall is performed in which the dipole density of each of multiple regions correlate to the potential measured at various locations within the associated chamber of the heart.

(51) **Int. Cl.**
A61B 5/04 (2006.01)
A61B 5/046 (2006.01)

(Continued)

26 Claims, 2 Drawing Sheets

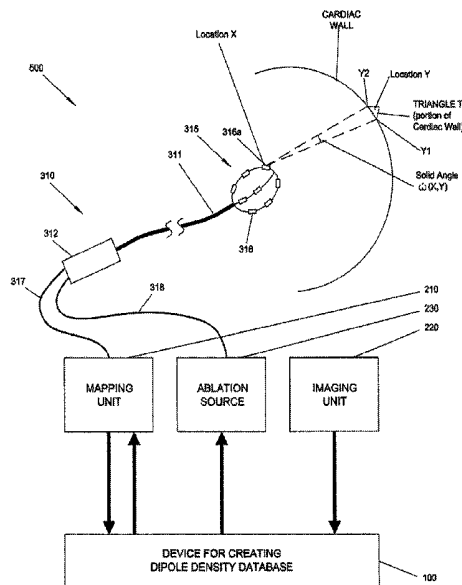

Related U.S. Application Data

continuation of application No. 13/946,712, filed on Jul. 19, 2013, now Pat. No. 9,192,318, which is a continuation of application No. 12/863,411, filed as application No. PCT/IB2009/000071 on Jan. 16, 2009, now Pat. No. 8,512,255.

(51) **Int. Cl.**

A61B 5/042 (2006.01)
A61B 5/0432 (2006.01)
A61B 5/00 (2006.01)
A61N 7/00 (2006.01)
A61B 5/044 (2006.01)
A61B 18/02 (2006.01)
A61B 18/12 (2006.01)
A61B 5/0402 (2006.01)
A61B 18/00 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/04005* (2013.01); *A61B 5/046* (2013.01); *A61B 5/0422* (2013.01); *A61B 5/0432* (2013.01); *A61B 5/4836* (2013.01); *A61B 5/6852* (2013.01); *A61B 18/02* (2013.01); *A61B 18/12* (2013.01); *A61N 7/00* (2013.01); *A61B 2018/00351* (2013.01); *A61B 2018/00577* (2013.01)

(56)

References Cited

U.S. PATENT DOCUMENTS

5,647,367 A 7/1997 Lum et al.
 5,662,108 A 9/1997 Budd et al.
 5,722,402 A 3/1998 Swanson et al.
 5,740,808 A 4/1998 Panescu et al.
 5,795,298 A 8/1998 Vesley et al.
 6,066,096 A 5/2000 Smith et al.
 6,187,032 B1* 2/2001 Ohyu A61B 5/04007
 600/409
 6,216,027 B1 4/2001 Willis et al.
 6,240,307 B1 5/2001 Beatty et al.
 6,301,496 B1 10/2001 Reisfeld
 6,400,981 B1 6/2002 Govari
 6,490,474 B1 12/2002 Willis et al.
 6,514,249 B1 2/2003 Maguire et al.
 6,574,492 B1 6/2003 Ben-Haim et al.
 6,640,119 B1 10/2003 Budd et al.
 6,716,166 B2 4/2004 Govari
 6,728,562 B1 4/2004 Budd et al.
 6,772,004 B2 8/2004 Rudy
 6,773,402 B2 8/2004 Govari et al.
 6,824,515 B2 11/2004 Suorsa et al.
 6,826,420 B1 11/2004 Beatty et al.
 6,826,421 B1 11/2004 Beatty et al.
 6,950,689 B1 9/2005 Willis et al.
 6,970,733 B2 11/2005 Willis et al.
 6,978,168 B2 12/2005 Beatty et al.
 6,990,370 B1 1/2006 Beatty et al.
 7,187,964 B2 3/2007 Khoury
 7,285,119 B2 10/2007 Stewart et al.
 7,289,843 B2 10/2007 Beatty et al.
 7,505,810 B2 3/2009 Harlev et al.
 7,573,182 B2 8/2009 Savage
 7,841,986 B2 11/2010 He et al.
 7,918,793 B2 4/2011 Altmann et al.
 7,953,475 B2 5/2011 Harlev et al.
 8,103,327 B2 1/2012 Harlev et al.
 8,147,486 B2 4/2012 Honour et al.
 8,175,680 B2 5/2012 Panescu
 8,208,998 B2 6/2012 Beatty et al.
 8,412,307 B2 4/2013 Willis et al.
 8,417,313 B2 4/2013 Scharf et al.
 8,428,690 B2 4/2013 Li et al.
 8,447,377 B2 5/2013 Harlev et al.

8,465,433 B2 6/2013 Zwirn
 8,512,255 B2* 8/2013 Scharf A61B 5/0422
 600/508
 8,700,119 B2 4/2014 Scharf et al.
 8,755,861 B2 6/2014 Harlev et al.
 8,825,134 B2 9/2014 Danehorn
 8,918,158 B2 12/2014 Scharf et al.
 8,948,837 B2 2/2015 Harlev et al.
 9,167,982 B2 10/2015 Scharf et al.
 9,186,081 B2 11/2015 Afonso et al.
 9,192,318 B2* 11/2015 Scharf A61B 5/0422
 9,492,227 B2 11/2016 Lopes et al.
 9,492,228 B2 11/2016 Lopes et al.
 9,504,395 B2* 11/2016 Scharf A61B 5/0422
 9,526,573 B2 12/2016 Lopes et al.
 9,610,024 B2 4/2017 Scharf et al.
 9,675,401 B2 6/2017 Lopes et al.
 9,757,044 B2 9/2017 Scharf et al.
 2001/0007070 A1 7/2001 Stewart et al.
 2002/0128565 A1 9/2002 Rudy
 2002/0165441 A1 11/2002 Coleman et al.
 2003/0065271 A1 4/2003 Khoury
 2003/0078494 A1 4/2003 Panescu et al.
 2003/0158477 A1 8/2003 Panescu
 2003/0236466 A1 12/2003 Tarjan et al.
 2005/0148836 A1 7/2005 Klee et al.
 2005/0203375 A1 9/2005 Willis et al.
 2006/0058692 A1 3/2006 Beatty et al.
 2006/0058693 A1 3/2006 Beatty et al.
 2006/0084884 A1 4/2006 Beatty et al.
 2006/0084970 A1 4/2006 Beatty et al.
 2006/0084971 A1 4/2006 Beatty et al.
 2006/0084972 A1 4/2006 Beatty et al.
 2006/0116576 A1 6/2006 McGee et al.
 2007/0106146 A1 5/2007 Altmann et al.
 2007/0219551 A1 9/2007 Honour et al.
 2007/0232949 A1 10/2007 Saksena
 2008/0009758 A1 1/2008 Voth
 2009/0024086 A1 1/2009 Zhang et al.
 2009/0076483 A1 3/2009 Danehorn
 2009/0131930 A1 5/2009 Gelbart et al.
 2009/0171274 A1 7/2009 Harlev et al.
 2009/0264781 A1 10/2009 Scharf
 2010/0168578 A1 7/2010 Garson, Jr. et al.
 2010/0298690 A1 11/2010 Scharf
 2011/0077526 A1 3/2011 Zwirn
 2011/0172658 A1 7/2011 Gelbart et al.
 2011/0270237 A1 11/2011 Werneth et al.
 2012/0078077 A1 3/2012 Harlev et al.
 2012/0143298 A1 6/2012 Just et al.
 2012/0184863 A1 7/2012 Harlev et al.
 2012/0277574 A1 11/2012 Panescu
 2013/0158537 A1 6/2013 Deladi et al.
 2013/0225983 A1 8/2013 Willis et al.
 2013/0226017 A1 8/2013 Scharf et al.
 2013/0253298 A1 9/2013 Harlev et al.
 2013/0274582 A1 10/2013 Afonso et al.
 2013/0304065 A1 11/2013 Lopes et al.
 2014/0024910 A1 1/2014 Scharf et al.
 2014/0180150 A1 6/2014 Scharf et al.
 2014/0275921 A1 9/2014 Harlev et al.
 2016/0100770 A1 4/2016 Afonso et al.
 2017/0035486 A1 2/2017 Lopes et al.
 2017/0100049 A1 4/2017 Scharf et al.

FOREIGN PATENT DOCUMENTS

CN 201275144 7/2009
 EP 1166714 1/2002
 EP 1760661 3/2007
 EP 1779787 5/2007
 EP 2051625 2/2008
 EP 2051625 4/2009
 EP 2252203 7/2009
 EP 2683293 1/2014
 JP 08501477 2/1996
 JP 10137207 5/1998
 JP 2001070269 3/2001
 JP 2002113004 4/2002

(56) **References Cited**

FOREIGN PATENT DOCUMENTS

JP	2002522106	7/2002
JP	2003511098	3/2003
JP	2004350702	12/2004
JP	2011507656	3/2011
WO	94/06349	3/1994
WO	09905971	2/1999
WO	9905971	2/1999
WO	00/07501	2/2000
WO	0245608	6/2002
WO	2003026722	4/2003
WO	2006060613	6/2006
WO	2008014629	2/2008
WO	2009090547	7/2009
WO	2011136867	11/2011
WO	2012092016	7/2012
WO	2012100184	7/2012
WO	2012100185	7/2012
WO	2014036439	3/2014

OTHER PUBLICATIONS

International Search Report and Written Opinion dated Jun. 26, 2015 issued in International Application No. PCT/US2015/022187.
 International Search Report dated Mar. 10, 2015 issued in corresponding International Application No. PCT/US14/54942.
 Gupta, et al., "Point of View Cardiac Mapping: Utility or Futility?", *Indian Pacing and Electrophysiology Journal*, vol. 2, No. 1, Jan. 1, 2002, pp. 20-32.
 European SR dated Sep. 29, 2014, issued in European Application No. 13176658.6.
 P. Della Bella, Non-Contact Mapping to Guide Catheter Ablation of Untolerated Ventricular Tachycardia, *European Heart Journal* (2002) 23, p. 742-752.
 PCT ISRWO dated Jun. 5, 2014, issued in corresponding PCT Application No. PCT/US2013/057579.
 European Office Action dated Apr. 28, 2014, issued in corresponding European Application No. 09 702 094.5-1660.
 ISRWO dated May 20, 2014 in International application No. PCT/US14/15261.
 William G. Stevenson et al: "Recording Techniques for Clinical Electrophysiology", *Journal of Cardiovascular Electrophysiology*, vol. 16, No. 9, Sep. 1, 2005, pp. 1017-1022.
 Wolfgang Nolting: *Elektrodynamik—Grundkurs Theoretische Physik 3*, Springer Spektrum, p. 89-91.
 Office Action dated Mar. 9, 2016 in corresponding European Patent Application No. 09702094.5.
 European Office Action dated Feb. 29, 2016, issued in corresponding European Application No. 07 785 075.8-1657.
 Van Oosterom A: "Solidifying the solid angle.", 2002, *Journal of Electrocardiology* 2002, vol. 35 Suppl, p. 181-192 ISSN: 0022-0736.
 Office Action dated Mar. 9, 2016 in corresponding European Patent Application No. 13176658.6.
 Invitation to Pay Additional Fees dated Jan. 8, 2014 in corresponding International Application No. PCT/US2013/057579.

Office Action dated Oct. 4, 2013 in corresponding Canadian Patent Application No. 2,659,898.

Pullan et al. "The inverse problem of electrocardiology" *Northeastern University Electrical and Computer Engineering*, Feb. 23, 2007.
 Christoph Scharft et al. Declaration under 37 C.F.R. 1.132, Nov. 15, 2012.

He et al. "An equivalent body surface charge model representing three-dimensional bioelectrical activity" *IEEE Transactions on Biomedical Engineering*, 42.7 (1995) pp. 637-646.

Partial European Search Report dated Apr. 29, 2014 in corresponding European Application No. 13176658.

International Search Report dated Sep. 10, 2014 issued in corresponding International Application No. PCT/US14/54942.

Examiner's Report dated Dec. 22, 2015 in related Canadian Application No. 2,656,898.

Office Action dated Apr. 27, 2016 in corresponding Canadian Application No. 2,747,859.

Extended European Search Report for related Application No. 13176658 dated Sep. 29, 2014.

International Search Report and Written Opinion in related Application No. PCT/US2012/028593 dated Mar. 5, 2013.

International Search Report in related Application No. PCT/IB2009/000071 dated Oct. 7, 2009.

Chinese Office Action dated Apr. 17, 2017 issued in corresponding Chinese Application No. 201480018328.4.

European Office Action dated Mar. 21, 2017 issued in corresponding European Application No. 07785075.8.

Jackson, JD, "Surface Distributions of Charges and Dipoles and Discontinuities in the Electric Field and Potential", *Classical Electrodynamics*, 3rd edition, Dec. 1998, pp. 31-34.

Canadian Office Action dated Apr. 26, 2017 issued in corresponding Canadian Application No. 2932956.

Canadian Office Action dated Mar. 30, 2017 issued in corresponding Canadian Application No. 2747859.

Leif et al., "Geometric modeling based on polygonal meshes". *Eurographics 2000 Tutorial*, Aug. 21, 2000.

Japanese Office Action dated Jun. 27, 2017 issued in corresponding Japanese Application No. 2015-530101, with English language translation.

Australian Office Action dated Jun. 27, 2017 issued in Australian Application No. 2013308531.

Australian Office Action dated Jul. 6, 2017, issued in Australian Application No. 2014/214756.

Japanese Notice of Allowance dated Jul. 11, 2017 issued in Japanese Application No. 2013-557926.

Extended European Search Report dated Oct. 18, 2017, issued in European Application No. 15768711.

Office Action dated Oct. 10, 2017 in Japanese Application No. 2015-557091 with machine translation to English.

Rule 70(2) Communication dated Nov. 7, 2017 issued in corresponding European Application No. 15768711.2.

Japanese Office Action dated Sep. 26, 2017 issued in corresponding Japanese Application No. 2017-155346, with English translation.

Canadian Office Action dated Nov. 27, 2017 issued in corresponding Canadian Application No. 2829626.

* cited by examiner

Fig. 1

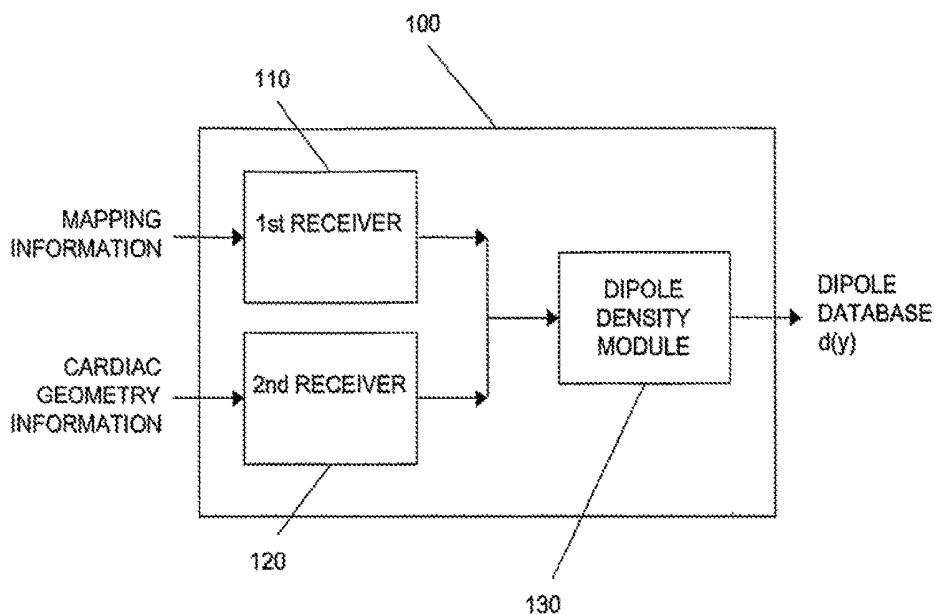


Fig. 2


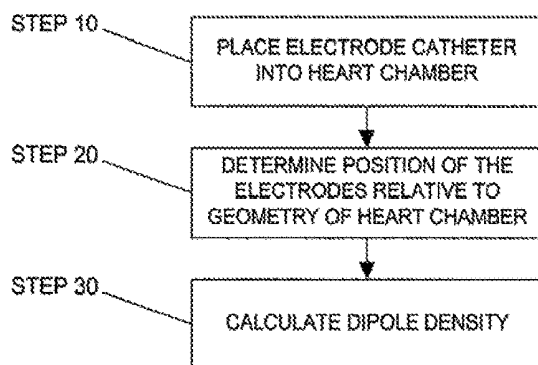


Fig. 3

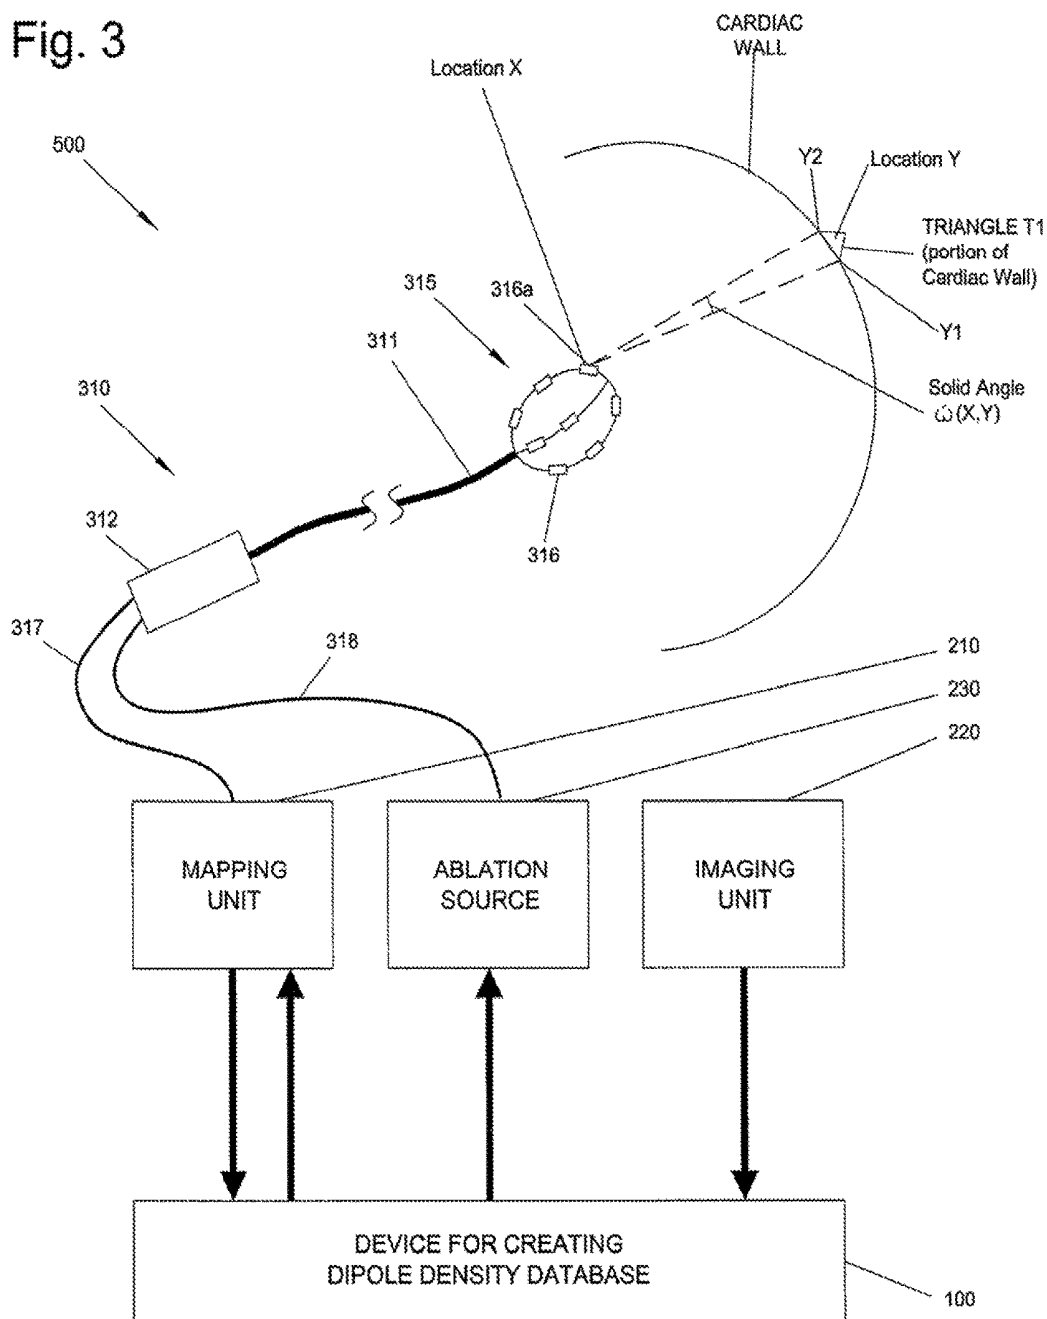

**DEVICE AND METHOD FOR THE
GEOMETRIC DETERMINATION OF
ELECTRICAL DIPOLE DENSITIES ON THE
CARDIAC WALL**

CROSS REFERENCE TO RELATED
APPLICATIONS

The present application is a continuation application of U.S. patent application Ser. No. 14/886,449 filed on Oct. 19, 2015, now U.S. Pat. No. 9,504,395, which is a continuation application of U.S. patent application Ser. No. 13/946,712 filed on Jul. 19, 2013, now U.S. Pat. No. 9,192,318, which is a continuation application of U.S. patent application Ser. No. 12/836,411, filed on Jul. 16, 2010, now U.S. Pat. No. 8,512,255, which is a 371 national stage application of Patent Cooperation Treaty Application No. PCT/IB2009/000071 filed Jan. 16, 2009, entitled A DEVICE AND METHOD FOR THE GEOMETRIC DETERMINATION OF ELECTRICAL DIPOLE DENSITIES ON THE CARDIAC WALL, which in turn claims priority to Swiss Patent Application 00068/08 filed Jan. 17, 2008, each of which is incorporated herein by reference.

FIELD OF THE INVENTION

The present invention relates generally to the localization and treatment of cardiac arrhythmias, and more particularly to devices and methods for the geometric determination of electrical dipole densities on the cardiac wall.

BACKGROUND

Systems used to localize the origin of cardiac arrhythmias measure potentials (e.g. in millivolts) in the cardiac chambers and localize them on a three dimensional representation of the cardiac chamber wall. The measurement of the electrical activity present on the cardiac walls is called mapping. For this purpose, a multiple electrode mapping catheter may be positioned within the heart such that multiple potentials can be simultaneously measured at different locations on the wall of the cardiac chamber without having direct wall contact (non-contact mapping). The cardiac chamber is visualized as a three dimensional structure, either directly by moving one or more mapping electrodes within the corresponding heart chamber or by importing an anatomical geometry of the cardiac chamber from an imaging device (e.g. Computed Tomography, MRI, or ultrasound). The electrical activity within the heart can be measured with the multi-electrode mapping catheter, which may be able to simultaneously measure potentials at different points in three dimensional space. In the current systems, the measured potentials from the non-contact multi-electrode mapping catheter do not directly correspond to the electrical activity on the cardiac wall as measured with an electrode with direct wall contact (contact mapping). The measured potentials of the non-contact mapping system have to be converted with computer programs and extrapolated into virtual electrograms projected on the heart chamber of the mapping system.

The current conversion methods are inaccurate, and further processing, termed regularization methods, have to be used. These regularization methods decrease spatial resolution. Another limitation of the current methods is that the provided potentials represent only the mean electrical activity that emanates from different cells, consisting of membranes separating electrical dipoles.

Since the localization of cardiac arrhythmias by the use of potentials is imprecise, the successful treatment of cardiac arrhythmias has been difficult and has demonstrated limited success and reliability. There is, therefore, a need for improved methods of localizing cardiac arrhythmias.

SUMMARY OF THE INVENTION

Several unique devices, systems, and methods for creating a database of dipole densities at a surface of a patient's heart are provided. Dipole density information can be used by a clinician to diagnose and treat heart diseases such as arrhythmias. The dipole density information is based on anatomical models of the patient's heart and mapping information recorded by multiple electrodes, such as electrodes included on the distal end of a three dimensional mapping catheter.

According to a first aspect of the invention, a device for creating a database of dipole densities at the surface of one or more cardiac chambers of a patient is provided. The device includes a first receiver that receives mapping information from multiple electrodes included in one or more mapping catheters. The electrodes are placed in a cardiac chamber of the patient's heart. The device further includes a second receiver that receives anatomical information. The anatomical information may be a generic heart model, or more preferably tissue contour and other anatomical information recorded from the patient's own heart. A dipole density module determines the database of dipole densities, in the table form $d(y)$, where y represents the location on the heart tissue including that particular dipole density. The potential at various locations x , within a cardiac chamber and termed $V(x)$, are recorded by the multiple electrodes. Solid angle $\omega(x,y)$ represents the solid angle for a triangle projection between location x (electrode location in chamber) and y (triangle location on chamber wall). The dipole density module determines the dipole density for individual triangle shaped projections onto the cardiac chamber wall based on the following: each triangle projection at location y contributes $\omega(x,y)$ times the dipole density $d(y)$ to the potential $V(x)$ at the point x .

In a preferred embodiment, the device comprises a software program, e.g., such as a software program loaded onto a personal computer; an ECG system; a cardiac tissue ablation system and/or an imaging system. The number of triangles determined by the dipole density module is sufficiently large (triangle area small enough) such that the dipole density for each triangle projection is relatively constant. Typically 1000 or more triangles are used in the calculations, such as a calculation based on a standard sized Left Atrium. Larger numbers of triangles are used for larger sized chambers.

In another preferred embodiment, the patient is being diagnosed and/or treated for a heart condition, such as an arrhythmia. The electrodes are included at the distal end of one or more mapping catheters and are placed into a chamber of the patient's heart to record potentials. An imaging instrument, such as an instrument that provides a generic model of a heart, or an instrument which provides an anatomical model of the patient's heart, delivers the anatomical information to the second receiver. In a preferred embodiment, the imaging instrument is one or more of: Computed Tomography; MRI; ultrasound; and an ECG system with mapping catheter.

In another preferred embodiment, the dipole density module implements an algorithm configured to assist in the creation of the database of dipole densities. The algorithm may be a progressive algorithm configured to be modified or

refined to improve spatial and/or time resolution of the database. The dipole density module may determine a map of dipole densities at corresponding time intervals. A synthesis of maps represents a cascade of activation sequences of each corresponding heart beat.

In another preferred embodiment, the device includes a third receiver. The third receiver receives mapping information from one or more skin electrodes. The dipole density module uses the skin electrode signals to calculate or recalculate the database of dipole densities, using equations listed herebelow.

According to another aspect of the invention, a system for creating a database of dipole densities at the surface of one or more cardiac chambers of a patient's heart is provided. In addition to the device of the present invention, the system includes one or more of a multiple electrode catheter; an imaging instrument; an ablation device; and at least one surface or skin electrode. In a preferred embodiment, the mapping catheter is also used for ablating tissue identified by the database of dipole densities. The system includes a monitor to display the dipole density information, such as information displayed in relative geometry to the chamber of the patient's heart.

According to another aspect of the invention, a method of creating a database of dipole densities at the surface of one or more cardiac chambers of a patient's heart is provided. The method can be used to diagnose and/or treat cardiac disease. In a preferred embodiment, the method is used to diagnose and treat Atrial Fibrillation (AF). In another preferred embodiment, the method is used to detect ventricular ischemia and/or quantify myocardial function. The method includes placing an array of multiple electrodes within a chamber of the patient's heart to measure potentials. The array of multiple electrodes may or may not be repositioned to determine dipole densities.

In another preferred embodiment, the method further includes placing one or more skin electrodes. The information recorded by the skin electrodes is used to determine the database of dipole densities.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate various embodiments in accordance with the present invention, and, together with the description, serve to explain the principles of the invention. In the drawings:

FIG. 1 illustrates a schematic view of an embodiment of a device for determining a database table of dipole densities $d(y)$ of at least one heart chamber, consistent with aspects of the present invention.

FIG. 2 illustrates a flow chart of an embodiment of a preferred method for determining a database table of dipole densities of at least one heart chamber, consistent with aspects of the present invention.

FIG. 3 illustrates a schematic view of an embodiment of a system for determining a database table of dipole densities of at least one heart chamber with help of the solid angle $\omega(x,y)$, consistent with aspects of the present invention.

DESCRIPTION OF THE EMBODIMENTS

Reference will now be made in detail to the embodiments in accordance with aspects of the present invention, examples of which are illustrated in the accompanying

drawings. Wherever possible, the same reference numbers will be used throughout the drawings to refer to the same or like parts.

A device for calculating surface charge densities has been described in detail in PCT International Application Number PCT/CH2007/000380 (hereinafter the '380 patent application) naming Scharf as inventor, filed Aug. 3, 2007, and entitled METHOD AND DEVICE FOR DETERMINING AND PRESENTING SURFACE CHARGE AND DIPOLE DENSITIES ON CARDIAC WALLS, and is incorporated by reference herein in its entirety. The present invention provides an improved device, system and method for calculating and visualizing the distribution and activity of dipole charge densities on a cardiac wall. The dipole densities are directly determined geometrically, avoiding the errors encountered using previous extrapolation algorithms.

In accordance with the present invention, provided is a device that measures and calculates a database of dipole densities $d(y)$ on the cardiac wall. The actual measured potentials in the heart result from electrical activity of cells, which can be regarded as dipoles. The dipoles consist of ion charges on both sides of biological membranes. The use of dipole densities offers a precise representation of the electrical activity. Systems and methods in accordance with the present invention efficiently and effectively calculate the dipole densities utilizing one or more mathematical theorems. This calculation is significantly more precise than calculations of virtual potentials produced by current systems, which lose spatial precision because of the required numerical methods and the use of potentials instead of dipole densities. Systems and methods in accordance with the present invention are efficient in calculating dipole densities geometrically, such as through the use of computer systems, or similar microcontroller and/or mathematical processing equipment.

Definitions

To facilitate an understanding of the invention, a number of terms are defined below.

As used herein, the terms "subject" and "patient" refer to any animal, such as a mammal like livestock, pets, and preferably a human. Specific examples of "subjects" and "patients" include, but are not limited, to individuals requiring medical assistance, and in particular, patients with an arrhythmia such as atrial fibrillation (AF).

As used herein, the term "solid angle" is the angle subtended by a triangle on the heart wall at the position x of observation. When viewed from location x , straight lines are drawn from point x to the boundaries of the triangle, and a sphere is constructed of radius $r=1$ with center of x . The straight lines then define the spherical triangle on the surface of the sphere. The solid angle is proportional to the surface area of the projection of that object onto a sphere centered at the point x .

The methods and devices of the present invention have advantages over previous prior art devices. FIGS. 1-3 illustrate various preferred embodiments of devices, systems and methods in accordance with aspects of the present invention. However, the present invention is not limited to these particular configurations.

Referring now to FIG. 1, a schematic view of an embodiment of a device for determining a database table of dipole densities of at least one heart chamber of a patient is illustrated. Device 100 includes a first receiver 110 configured to receive electrical potentials from a separate device, such as a device including a multi-electrode mapping cath-

eter placed in the circulating blood within a chamber of the patient's heart. Device **100** further includes a second receiver **120** configured to receive cardiac geometry information (e.g. the geometric contour of the cardiac chamber wall), such as from an instrument including, but not limited to: Computed Tomography; MRI; Ultrasound; a multi-electrode mapping catheter; and combinations of these. Alternatively, a standard geometry can be loaded representing a model of the cardiac chamber. Device **100** further includes a dipole density module **130** which comprises mathematical processing element, such as a computer or other electronic module including software and/or hardware for performing mathematical or other calculations. Dipole density module **130** receives mapping information from first receiver **110** and cardiac geometry information from second receiver **120**. Dipole density module **130** preferably uses one or more algorithms to process the received mapping and geometry information to produce a database table of dipole densities.

The geometrical model of the cardiac chamber is processed by dipole density module **130** into multiple small triangles (triangularization). When the triangles are sufficiently small, the dipole density at each triangle can be regarded as constant. In a preferred embodiment, a standard cardiac chamber of 4-6 cm diameter is divided up into over 1000 triangles. In another preferred embodiment, the number of triangles determined by dipole density module **130** is based on the size of the heart chamber. With the electrodes positioned in a cardiac chamber by a clinician, such as an electrophysiologist, the potentials at each electrode are recorded. Each triangle is seen by the corresponding electrode under a certain solid angle. The dipole density module **130** computes the solid angle $\omega(x,y)$ subtended by each triangle at position y on each electrode at position x on the multi-electrode catheter. If the dipole density at the triangle is $d(y)$, the triangle contributes $\omega(x,y)$ times $d(y)$ to the potential $V(x)$ at the position x on the multi-electrode catheter. The total measured potential $V(x)$ is the sum resulting from all the triangles. A detailed description is provided in reference to FIG. 3 herebelow.

In a preferred embodiment, dipole density module **130** implements a progressive algorithm that can be modified and/or refined in order to improve spatial and/or time resolution of the database of dipole densities that are produced. The dipole densities $d(y)$ are obtained by solving a linear system of equations. This calculation requires some care to avoid numerical instabilities. Thereby a map of dipole densities can be created at each corresponding time interval. The synthesis of the maps generates a cascade of the activation sequence of each corresponding heart beat that can be used to define the origin of the electrical activity, arrhythmias or diagnose cardiac disease.

The measuring electrodes used in the present invention are placed in the blood flow in a heart chamber, a relatively homogeneous condition, such that the mathematical analysis of the present invention is well applicable. In a preferred embodiment, skin electrodes are also implemented such that dipole density module **130** can use the information received from the skin electrodes to calculate and/or recalculate the dipole densities for the cardiac wall. The spatial resolution which can be obtained by invasive (i.e., placed in the heart chamber) multi-electrode potential measurements is limited by the number of electrodes that can be placed in any cardiac chamber, such as the Left Atrium (LA). Skin placed electrodes, such as electrodes placed on the thorax, are not as space limited. However, due mainly to the inhomogeneous structure of the body, it is difficult to localize the actual sources of the skin electrode measured potentials. A highly

complicated boundary value problem must be solved with boundary conditions that are poorly known, and previous attempts at determining the "action potential" from body surface ECG (alone) have not been very successful.

The badly defined boundary value problem can be avoided by an additional measurement (in addition to the skin electrode measurements) of the multi-electrode array of the present invention. A small sinusoidal voltage V_i is applied to each electrode $i=1, \dots, L$ on the electrode array in the heart, and the resulting voltages W_k , $k=1, \dots, K$ is measured at the surface electrodes. This yields the $K \times L$ transition matrix A_{ki}

$$W_k = \sum_{i=1}^L A_{ki} V_i. \quad (1)$$

Calculating solid angles produces the linear transformation B_{in} between the electrode array potentials V_i and the dipole densities d_n , $n=1, \dots, N$ of N regions of the heart wall:

$$V_i = \sum_{n=1}^N B_{in} d_n. \quad (2)$$

N is chosen to be $N=K+L$ where K is the number of surface electrodes and L is the number of internally placed array electrodes.

Substituting equation (2) into (1) we have:

$$W_k = \sum_{i=1}^L \sum_{n=1}^N A_{ki} B_{in} d_n. \quad (3)$$

Therefore, by simultaneous measuring of the potentials of the cardiac activity with all $K+L$ electrodes, $N=K+L$ dipole densities of N regions on the heart wall can be calculated. This method yields a higher spatial resolution than the L array electrodes alone. In the solution of the linear system of equations (2)+(3), regularization techniques must be used (e.g. Tikhonov regularization and its modifications) in order to avoid numerical instabilities.

Referring now to FIG. 2, an embodiment of a preferred method for determining a database table of dipole densities of at least one heart chamber of a patient is illustrated. In Step **10**, a multi-electrode array is placed within the corresponding heart chamber. In Step **20**, the geometry of the corresponding heart chamber is obtained in relation to the multi-electrode array position, such as by moving around a second mapping electrode or by importing a geometry model from an imaging study (e.g. using computed tomography, MRI or ultrasound before or after the multi-electrode array of electrodes has been placed in the heart chamber). The surface of the geometry of the corresponding heart chamber is divided into small triangles, typically at least 1000 small triangles.

In Step **30**, the dipole density $d(y)$ can be calculated from the measured potential values and the calculated solid angles. The measurements can be repeated successively during the cardiac cycle giving a high timely resolution during each millisecond. The information of the timely dependent dipole densities can be depicted as an activation map of the corresponding heart chamber for the given heart

beat. The information can be used to diagnose and/or treat a patient with a cardiac arrhythmia, such as an atrial fibrillation patient.

In a preferred embodiment, the information is used to determine cardiac wall treatment locations for lesion creation, such as a lesion created in the Left or Right atrium, by an RF, ultrasound or cryogenic ablation catheter. In another preferred embodiment, the multiple electrode mapping array is placed in a ventricle and the dipole densities are determined for the ventricular wall, such as to detect ischemia or quantify myocardial function.

Referring now to FIG. 3, an embodiment of a system for determining a database table of dipole densities of at least one heart chamber of a patient is illustrated. System 500 includes device 100, which is configured to create a database table of dipole densities $d(y)$ based on voltage potential measurements within the heart chamber and image information relating to the heart chamber, as has been described hereabove. System 500 further includes imaging unit 220, which is configured to provide a two or three-dimensional image of the heart chamber to device 100. Imaging unit 220 may perform at least one of Computed Tomography, MRI and/or ultrasound imaging. Imaging unit 220 may produce any form of real or virtual models of the cardiac chambers, such that a triangularization analysis is possible.

System 500 further includes mapping catheter 310, which includes shaft 311, shown inserted into a chamber of a patient's heart, such as the Left Atrium (LA). At the distal end of shaft 311 is an electrode array 315 including multiple electrodes 316. Electrode array 315 is shown in a basket construction, but numerous other constructions can be used including multiple independent arms, spiral arrays, electrode covered balloons, and other constructions configured to place multiple electrodes into a three-dimensional space. In a preferred embodiment, any catheter with a three-dimensional array of electrodes can be used to supply the mapping information to device 100.

In this embodiment, electrodes 316 are connected to wires, not shown, but traveling proximally to cable 317, which is electrically connected to a mapping unit 210, such as an electrocardiogram (ECG) unit. ECG unit 210 includes a monitor for displaying information, such as the potentials recorded by electrodes 316, as well as the dipole density information produced by device 100. In an alternative embodiment, device 100 further includes a monitor, not shown, but configured to display one or more of: dipole density information; potentials recorded by electrodes 316; and cardiac chamber contours and other geometry information. In a preferred embodiment, dipole density and or recorded potentials information is shown in reference to a three-dimensional representation of the heart chamber into which catheter 310 is inserted. In an alternative embodiment, imaging unit 220 may include a device configured to create an image of the cardiac chamber from signals recorded from an electrode catheter, such as catheter 310.

System 500 may include a device for treating a cardiac arrhythmia, such as ablation source 230, which is electrically attached to electrodes 316 via cable 318. Alternatively or additionally, ablation source 230 can be attached to a different ablation catheter, such as a single or multiple ablation element catheter configured to deliver ablation energy such as RF energy, cryogenic energy, or other tissue disrupting energy.

As shown in FIG. 3, triangle T1, defined by device 100, is at location Y. Electrode 316a of catheter 310 is at location X. The geometric relationship between triangle T1 and Location X is defined by the solid angle, angle $\omega(X,Y)$.

Device 100 includes dipole density module 130 such that each triangle at location y contributes $\omega(x,y)$ times the dipole density $d(y)$ to the potential $V(x)$ at the position x on a multi-electrode. Solid angle $\omega(x,y)$, as defined above, corresponds to the triangle at a location y and the electrode at positions x on the multi-electrode array. The dipole density module 130 of device 100 determines from the total measured potential $V(x)$, which is the sum resulting from all the triangles defined by device 100, the desired dipole density $d(y)$.

When sufficient potentials values $V(x)$ are measured (e.g. from 10 to 10,000 with increasing number of measured potentials providing more accurate results), the dipole density $d(y)$ at many equally distributed regions y on the cardiac wall is calculated by solving a linear equation system. By interpolation of the measured potentials (e.g. with help of splines) their number can be increased to a higher number of regions. The solid angle $\omega(x,y)$ of a region is the sum of the solid angles of the individual triangles in the region on the cardiac wall. This calculation of dipole density results, such as via an automatic computer program forming at least part of dipole density module 130.

In a preferred embodiment, the results are presented in a visual, anatomical format, such as depicting the dipole densities on a geometric image of the cardiac wall in relation to time (t). This format allows a clinician, such as an electrophysiologist, to determine the activation sequence on the cardiac wall, such as to determine treatment locations for a cardiac arrhythmia. The results may be shown on a display of mapping unit 210, or on a separate unit such as a display included with device 100, display not shown but preferably a color monitor. In a preferred embodiment, the device of the present invention is implemented as, or includes, a software program that is executable by at least one processor. The software program can be integrated into one or more of: an ECG system; a cardiac tissue ablation system; an imaging system; a computer; and combinations of these.

In a preferred embodiment, the multi-electrode catheter includes at least 10 electrodes, configured to represent a three dimensional body with known geometry. The electrodes are preferably positioned in a spherical geometry, such as a spherical geometry created in a basket catheter. Elliptical electrode array geometries may be used, such as those provided in the Ensite Array Catheter, manufactured by St. Jude Medical of St. Paul Minn. In an alternative embodiment, multiple catheters are inserted into the heart chamber to provide the multiple electrodes.

In an alternative embodiment, the electrodes of the multi-electrode mapping array are repositioned during the method of determining dipole densities. Repositioning of electrodes can be beneficial to increase the number of measured potential values, if electrode positions are known. Therefore, repositioning is in concordance with adjustment of the geometry map in relation to the multi-electrode mapping catheter.

Other embodiments of the invention will be apparent to those skilled in the art from consideration of the specification and practice of the embodiments disclosed herein. It is intended that the specification and examples be considered as exemplary only, with a true scope and spirit of the invention being indicated by the following claims. In addition, where this application has listed the steps of a method or procedure in a specific order, it may be possible, or even expedient in certain circumstances, to change the order in which some steps are performed, and it is intended that the particular steps of the method or procedure claims set forth

herebelow not be construed as being order-specific unless such order specificity is expressly stated in the claim.

We claim:

1. A device for treating a cardiac condition, said device 5 comprising:

computer storage media for storing a geometrical representation of one or more cardiac chambers;
multiple electrodes for sensing and recording a plurality of potentials generated from cardiac activity;

a dipole density module for generating a database of dipole densities $d(y)$ associated with one or more surfaces of the one or more cardiac chambers based on the plurality of potentials and the geometrical representation of the one or more cardiac chambers;

a computer processor for diagnosing a cardiac condition based on the database of dipole densities, wherein the computer processor further comprises an algorithm configured to improve time resolution of the database of dipole densities; and

a treatment device for treating the cardiac condition.

2. The device according to claim 1, wherein the cardiac condition diagnosed comprises an arrhythmia.

3. The device according to claim 2, wherein the arrhythmia comprises atrial fibrillation.

4. The device according to claim 1, wherein the cardiac condition diagnosed comprises ischemia.

5. The device according to claim 4, wherein the ischemia comprises ventricular ischemia.

6. The device according to claim 1, wherein the cardiac condition diagnosed comprises a myocardial function issue.

7. The device according to claim 6, wherein the device is configured to quantify myocardial function.

8. The device according to claim 1, wherein the database of dipole densities is used to determine cardiac wall treatment locations for lesion creation.

9. The device according to claim 1, wherein the dipole density module determines a dipole density for individual triangle shaped projections onto the cardiac chamber wall, where each triangle projection at a location y contributes $\omega(x,y)$ times the dipole density $d(y)$ to a potential $V(x)$ at a point x , wherein $\omega(x,y)$ is the solid angle for that triangle projection, and where:

a) x represents a series of locations within one or more cardiac chambers; and

b) $V(x)$ is a measured potential at point x , said measured potential recorded by the multiple electrodes.

10. The device according to claim 9, wherein said triangle projections are sized such that the dipole density for each triangle projection is substantially constant.

11. The device according to claim 10, wherein the dipole density is determined for at least 1000 triangle shaped projections.

12. The device according to claim 9, wherein a number of measured potentials $V(x)$ is in a range of 10 through 10,000 potentials $V(x)$.

13. The device according to claim 1, wherein the computer processor further comprises an algorithm configured to improve spatial resolution of the database of dipole densities.

14. The device according to claim 1, wherein the multiple electrodes are included in a single catheter.

15. The device according to claim 1, wherein the multiple electrodes are included in two or more catheters.

16. The device of claim 1, wherein the dipole density module calculates and/or recalculates the dipole densities $d(y)$ using the following equations:

$$W_k = \sum_{l=1}^L A_{kl} V_l, \quad (1)$$

wherein a small sinusoidal voltage V_1 is applied to each electrode $l=1, \dots, L$ on the electrode array in the heart, and the resulting voltages W_k , $k=1, \dots, K$ is measured at the surface electrodes, which yields the $K \times L$ transition matrix A_{kl} ;

$$V_l = \sum_{n=1}^N B_{ln} d_n, \quad (2)$$

wherein calculating solid angles produces the linear transformation B_{ln} between the electrode array potentials V_l and the dipole densities d_n , $n=1, \dots, N$ of N regions of the cardiac chamber wall; and

$$W_k = \sum_{l=1}^L \sum_{n=1}^N A_{kl} B_{ln} d_n, \quad (3)$$

where equation (2) above is substituted into equation (1) to form equation (3).

17. The device according to claim 16, wherein the dipole density module is configured to solve equations (2) and (3) using regularization techniques.

18. The device according to claim 17, wherein the regularization technique is Tikhonov regularization.

19. The device according to claim 1, wherein the treatment device comprises an ablation device configured to deliver one or more of: radio frequency (RF) energy; ultrasound energy, and cryogenic energy.

20. A device for diagnosing a cardiac condition, said device comprising:

computer storage media for storing a geometrical representation of one or more cardiac chambers;

multiple electrodes for sensing and recording a plurality of potentials generated from cardiac activity;

a dipole density module for generating a database of dipole densities $d(y)$ associated with one or more surfaces of the one or more cardiac chambers based on the plurality of potentials and the geometrical representation of the one or more cardiac chambers;

a computer processor for diagnosing a cardiac condition based on the database of dipole densities, wherein the computer processor further comprises an algorithm configured to improve spatial resolution and time resolution of the database of dipole densities.

21. The device according to claim 20, wherein the device is further configured for treating the cardiac condition and comprises a treatment device for treating the cardiac condition.

22. A device for diagnosing a cardiac condition, said device comprising:

computer storage media for storing a geometrical representation of one or more cardiac chambers;

multiple electrodes for sensing and recording a plurality of potentials generated from cardiac activity;

a dipole density module for generating a database of dipole densities $d(y)$ associated with one or more surfaces of the one or more cardiac chambers based on

the plurality of potentials and the geometrical representation of the one or more cardiac chambers and for generating maps of dipole densities corresponding time intervals;

a computer processor for diagnosing a cardiac condition 5 based on the database of dipole densities, wherein the computer processor is configured to synthesize the maps of dipole densities to create an activation sequence of corresponding heart beats.

23. The device according to claim **22**, wherein the cardiac 10 condition is diagnosed based on the activation sequence of the corresponding heart beats.

24. The device according to claim **23**, wherein an origin of an arrhythmia is defined based on the activation sequence of the corresponding heart beats. 15

25. The device according to claim **24**, wherein the maps of the dipole densities are created successively during a cardiac cycle to provide resolution during each millisecond.

26. The device according to claim **22**, wherein the device is further configured for treating the cardiac condition and 20 comprises a treatment device for treating the cardiac condition.

* * * * *

专利名称(译)	用于几何确定心壁上的电偶极子密度的装置和方法		
公开(公告)号	US9913589	公开(公告)日	2018-03-13
申请号	US15/333378	申请日	2016-10-25
[标]申请(专利权)人(译)	克里斯托夫		
申请(专利权)人(译)	SCHARF, CHRISTOPH		
当前申请(专利权)人(译)	SCHARF, CHRISTOPH		
[标]发明人	SCHARF CHRISTOPH SCHARF GUNTER		
发明人	SCHARF, CHRISTOPH SCHARF, GUNTER		
IPC分类号	A61B5/04 A61B5/0432 A61B5/00 A61N7/00 A61B5/042 A61B5/046 A61B5/044 A61B5/0402 A61B18/12 A61B18/02 A61B18/00		
CPC分类号	A61B5/04012 A61B5/0402 A61B5/044 A61B5/04005 A61B5/046 A61B5/0422 A61B5/4836 A61B5/6852 A61B18/02 A61B18/12 A61N7/00 A61B5/0432 A61B2018/00577 A61B2018/00351 A61B6/032 A61B8/13 A61B18/0206 A61B18/18 A61B5/0036 A61B5/02028		
优先权	2008000068 2008-01-17 CH 13/946712 2015-11-24 US 12/863411 2013-08-20 US PCT/IB2009/000071 2009-01-16 WO		
其他公开文献	US20170100049A1		
外部链接	Espacenet USPTO		

摘要(译)

公开了用于确定心脏壁上的偶极密度的装置，系统和方法。具体而言，执行心壁的三角形化，其中多个区域中的每一个的偶极密度与在心脏的相关腔室内的各个位置处测量的电位相关。

