



US 20180317814A1

(19) **United States**

(12) **Patent Application Publication**
NURKKA

(10) **Pub. No.: US 2018/0317814 A1**

(43) **Pub. Date: Nov. 8, 2018**

(54) **SYSTEMS AND METHODS FOR
MONITORING RESPIRATION IN A
BIOSENSING GARMENT**

(52) **U.S. Cl.**
CPC *A61B 5/1135* (2013.01); *D04B 21/18*
(2013.01); *A61B 5/6805* (2013.01)

(71) Applicant: **OMsignal Inc.**, Montreal (CA)

(57) **ABSTRACT**

(72) Inventor: **Maria Elina NURKKA**, Verdun (CA)

(21) Appl. No.: **15/907,913**

(22) Filed: **Feb. 28, 2018**

Related U.S. Application Data


(63) Continuation of application No. PCT/CA2016/051034, filed on Aug. 31, 2016.

(60) Provisional application No. 62/212,899, filed on Sep. 1, 2015, provisional application No. 62/247,049, filed on Oct. 27, 2015.

Publication Classification

(51) **Int. Cl.**
A61B 5/113 (2006.01)
A61B 5/00 (2006.01)

Embodiments described herein relate generally to biosensing garments, and in particular, to systems and methods for monitoring respiration in a biosensing garment, whereby an improved integration of the respiration monitoring circuit into the garment is achieved, resulting in improved signal quality and durability. In some embodiments, an apparatus includes an elongate member having a longitudinal axis and configured to be stretchable along its longitudinal axis. The elongate member includes a plurality of elastic members (e.g., a first elastic member, a second elastic member, and a third elastic member) that extend along the longitudinal axis. A conductive member is coupled to the first, second and third members, and forms a “curved” pattern along the longitudinal axis of the elongate member. The conductive member is configured to change from a first configuration to a second configuration as the elongate member stretches along its longitudinal axis.

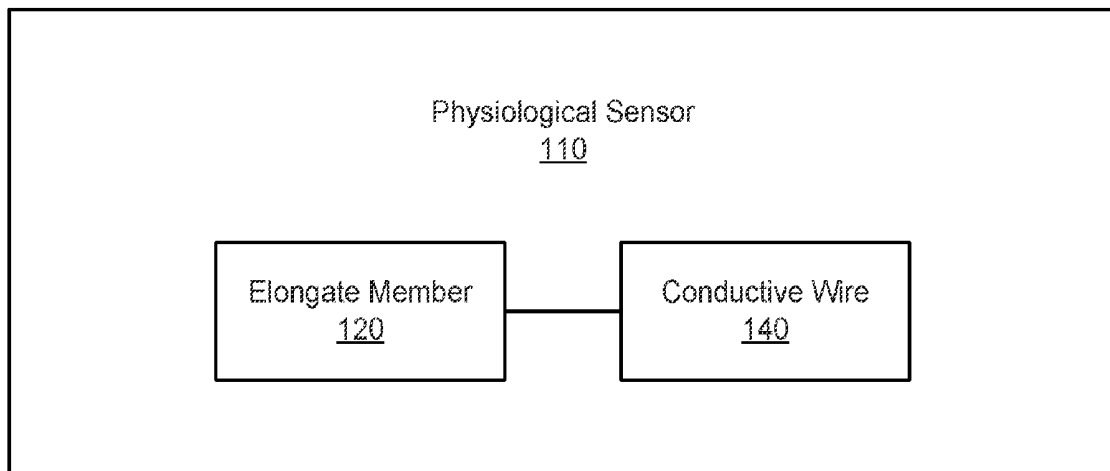

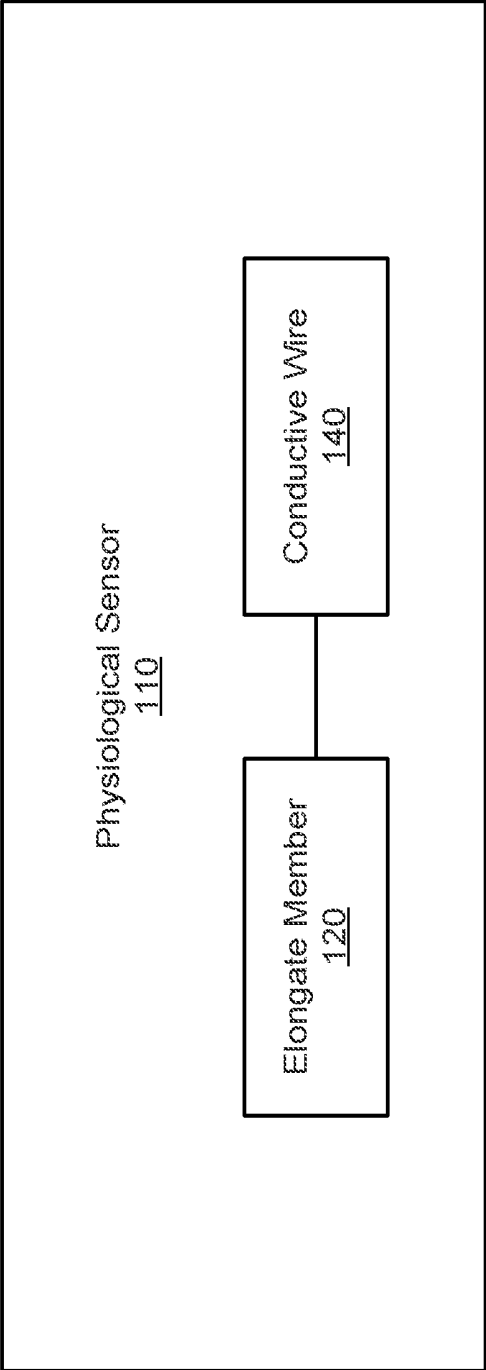


FIG. 1

FIG. 2B

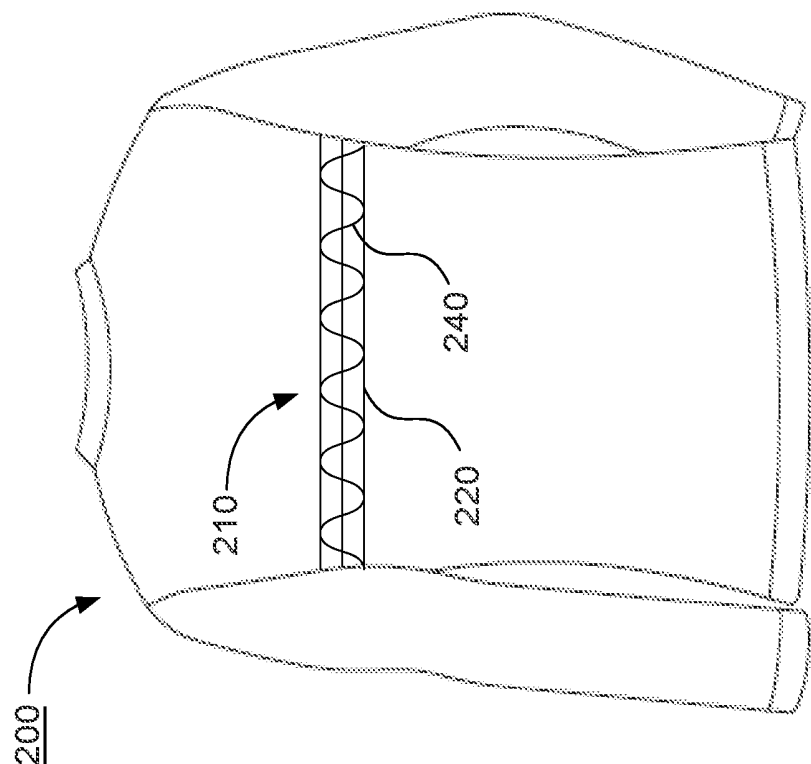


FIG. 2A

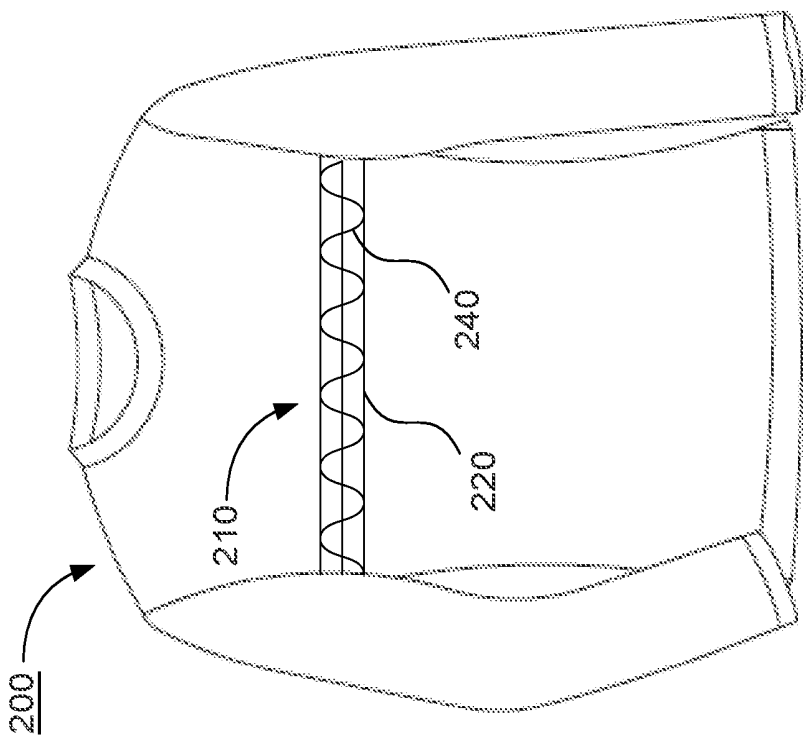


FIG. 3

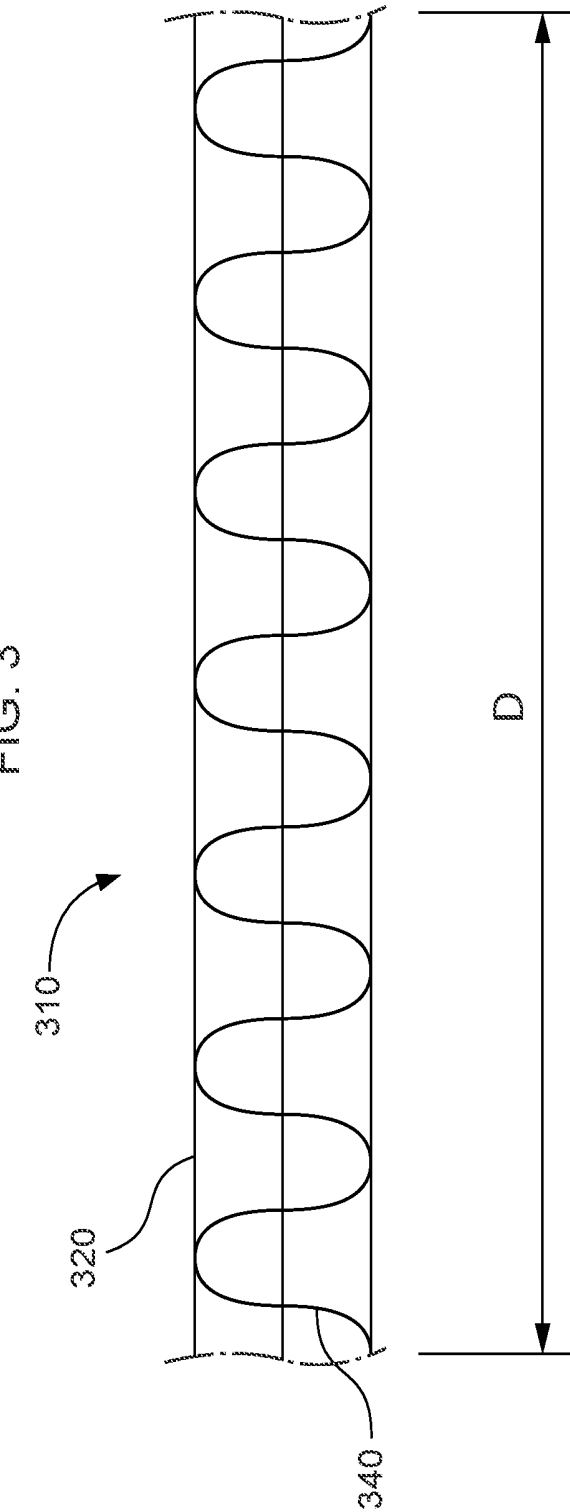


FIG. 4

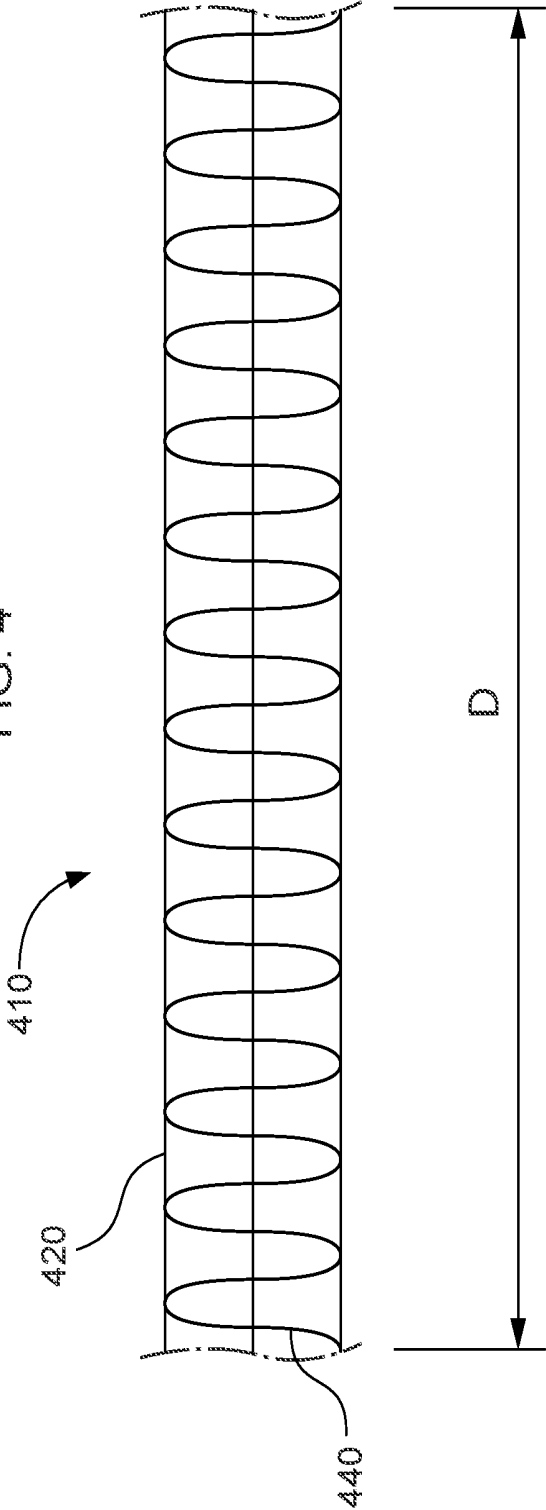


FIG. 5

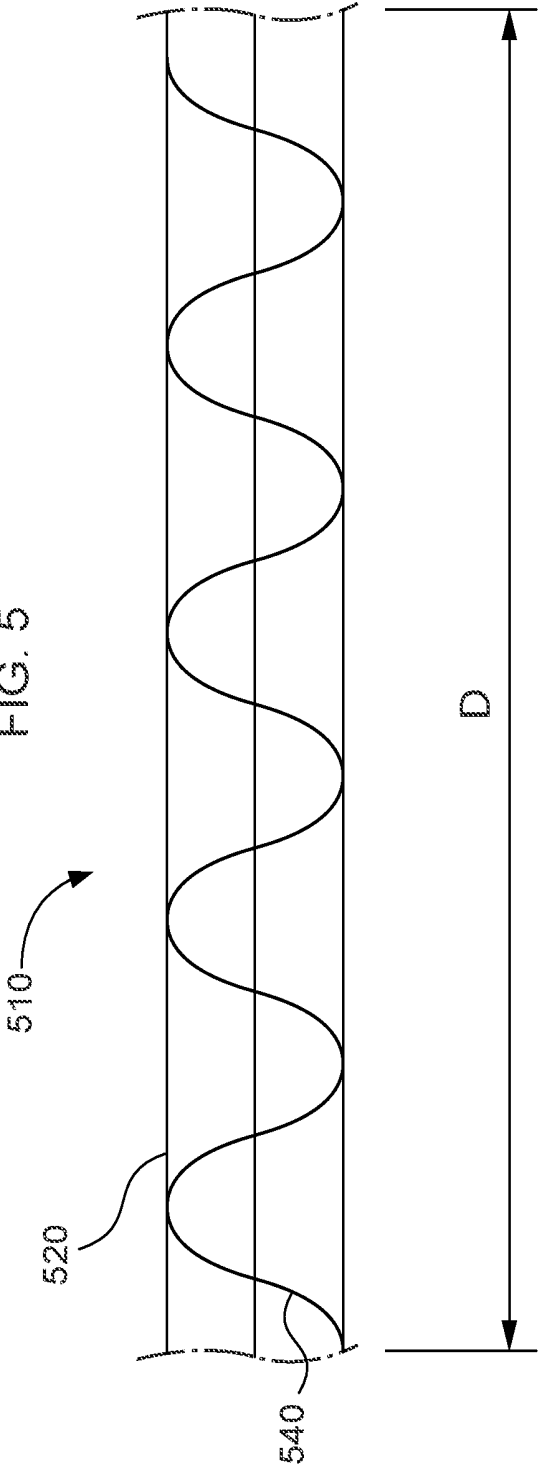
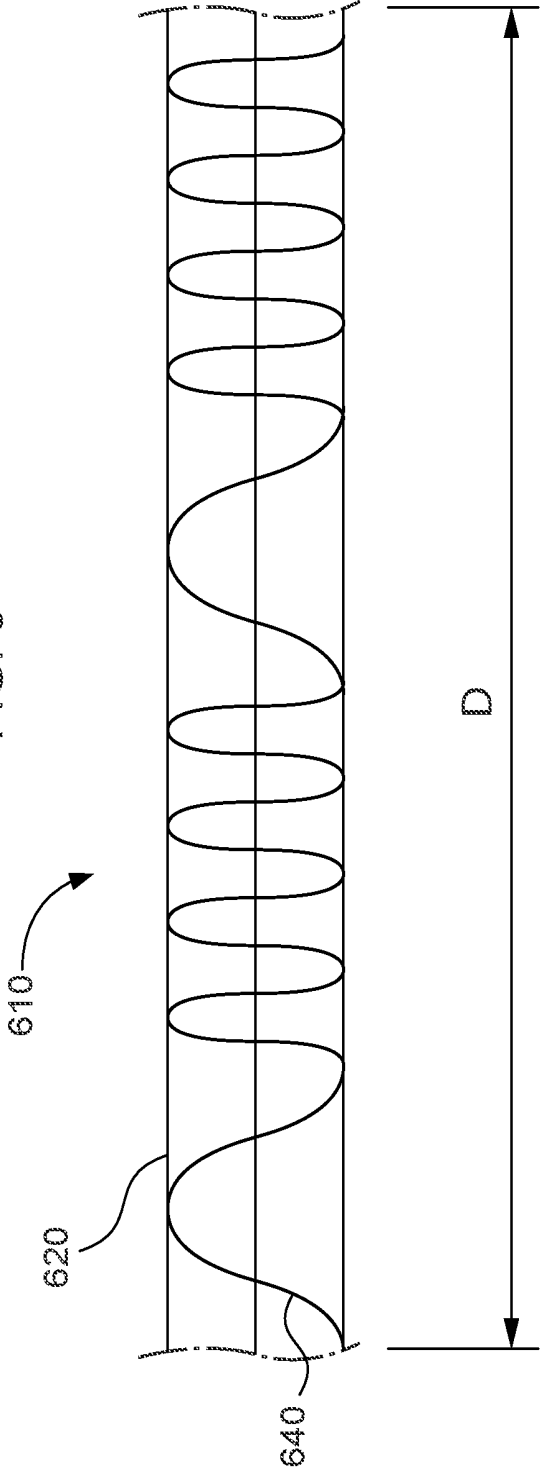


FIG. 6



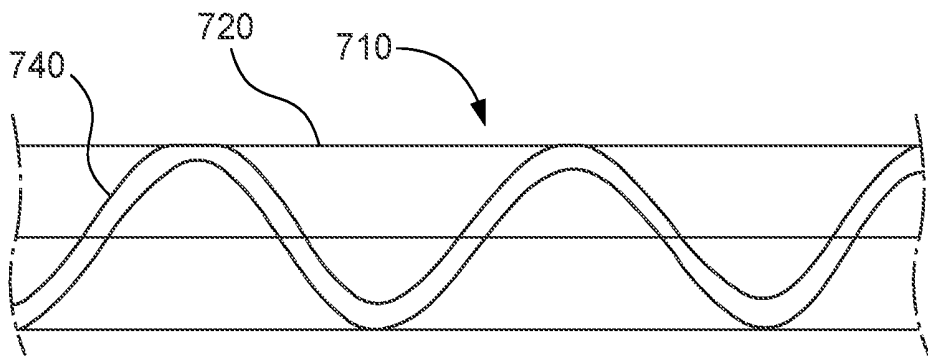


FIG. 7A

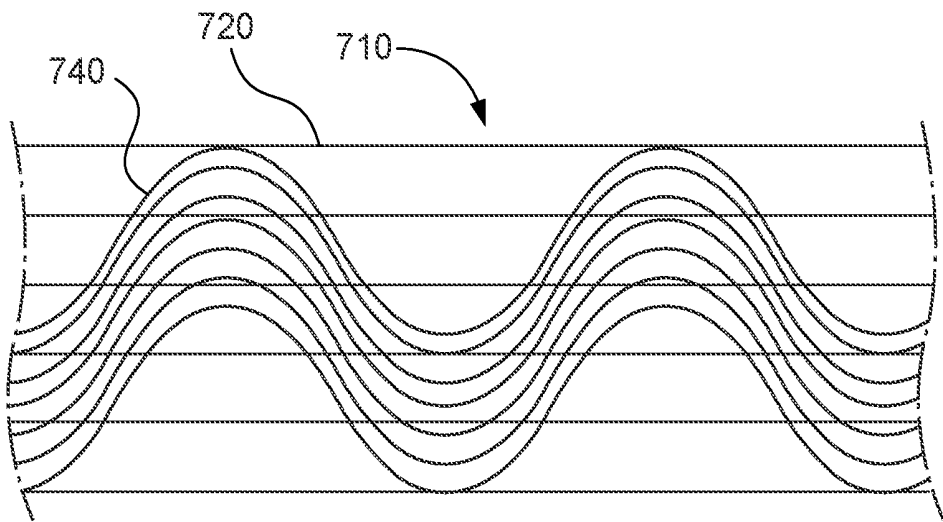


FIG. 7B

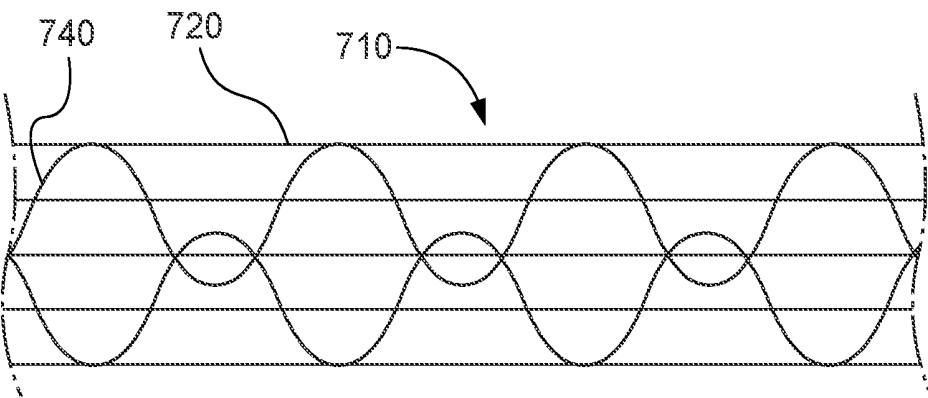


FIG. 7C

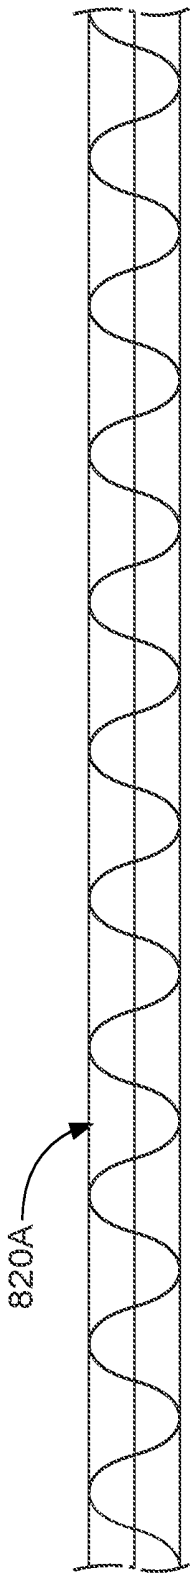


FIG. 8A

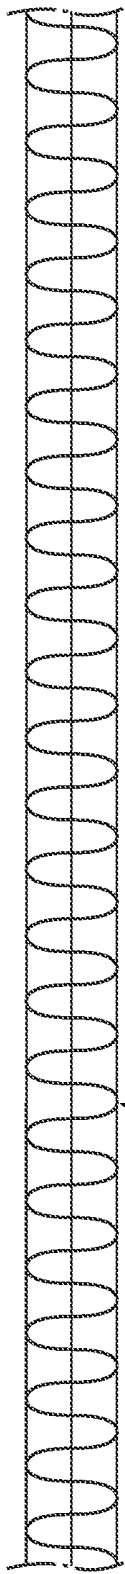
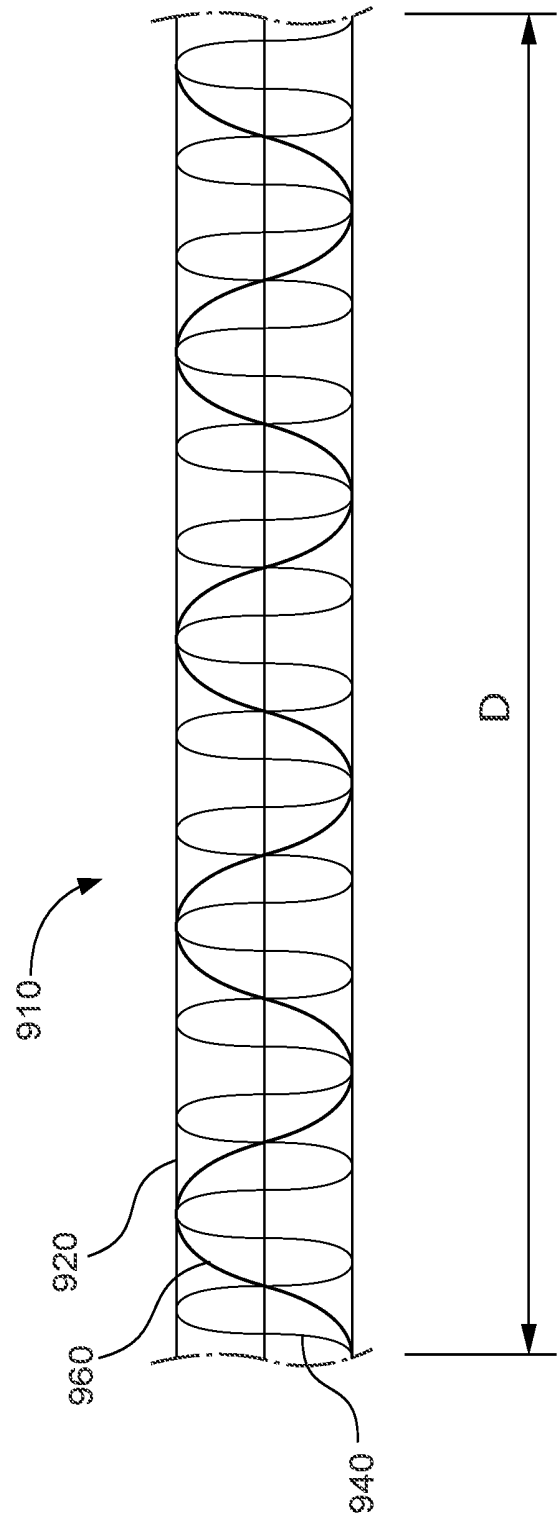


FIG. 8B

FIG. 9



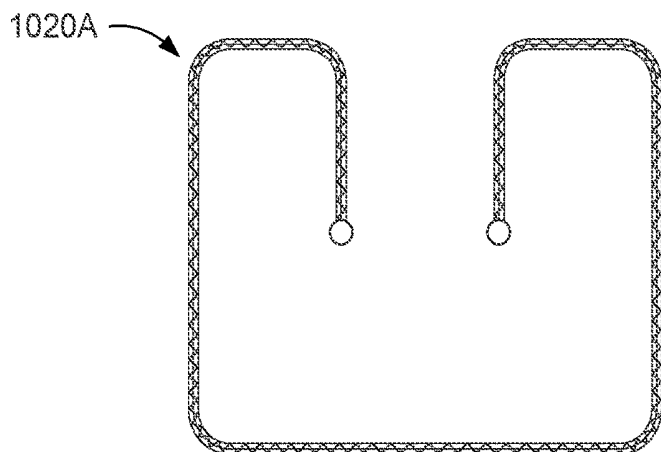


FIG. 10A

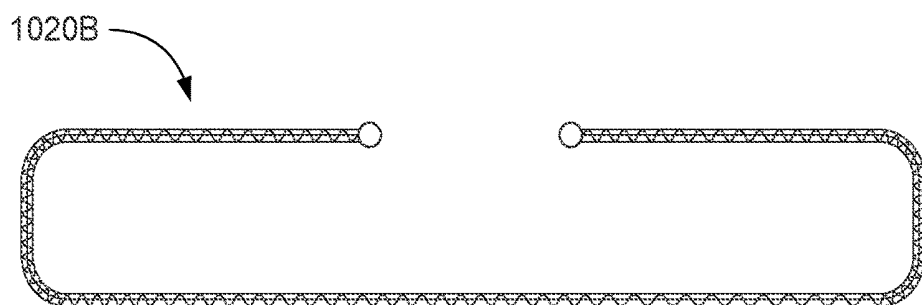


FIG. 10B

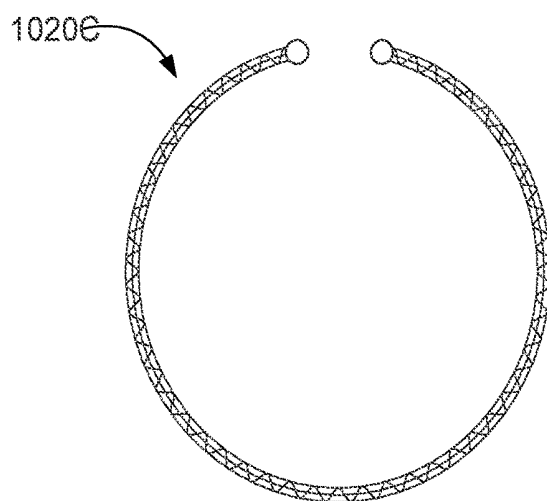


FIG. 10C

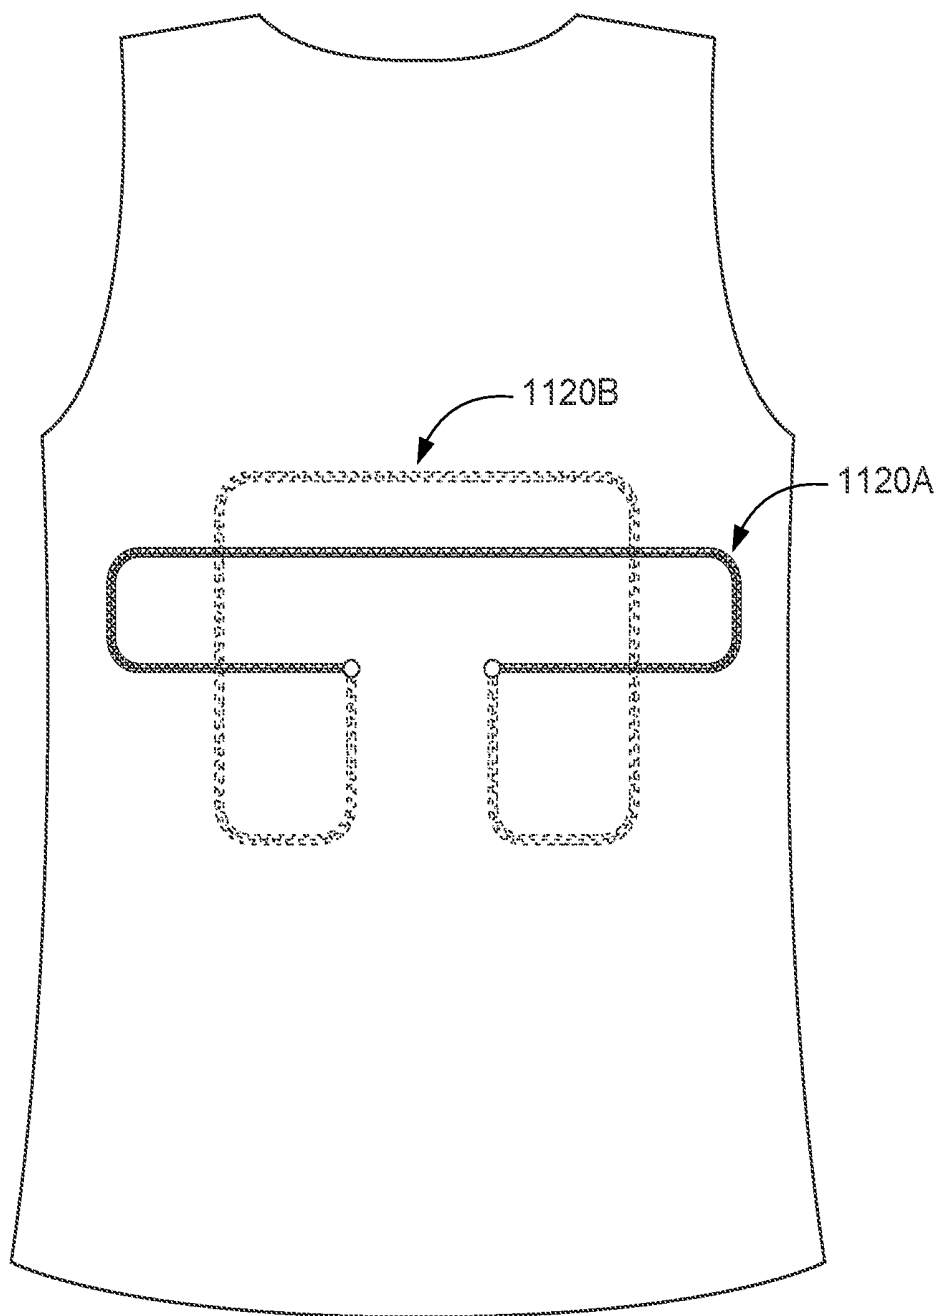


FIG. 11

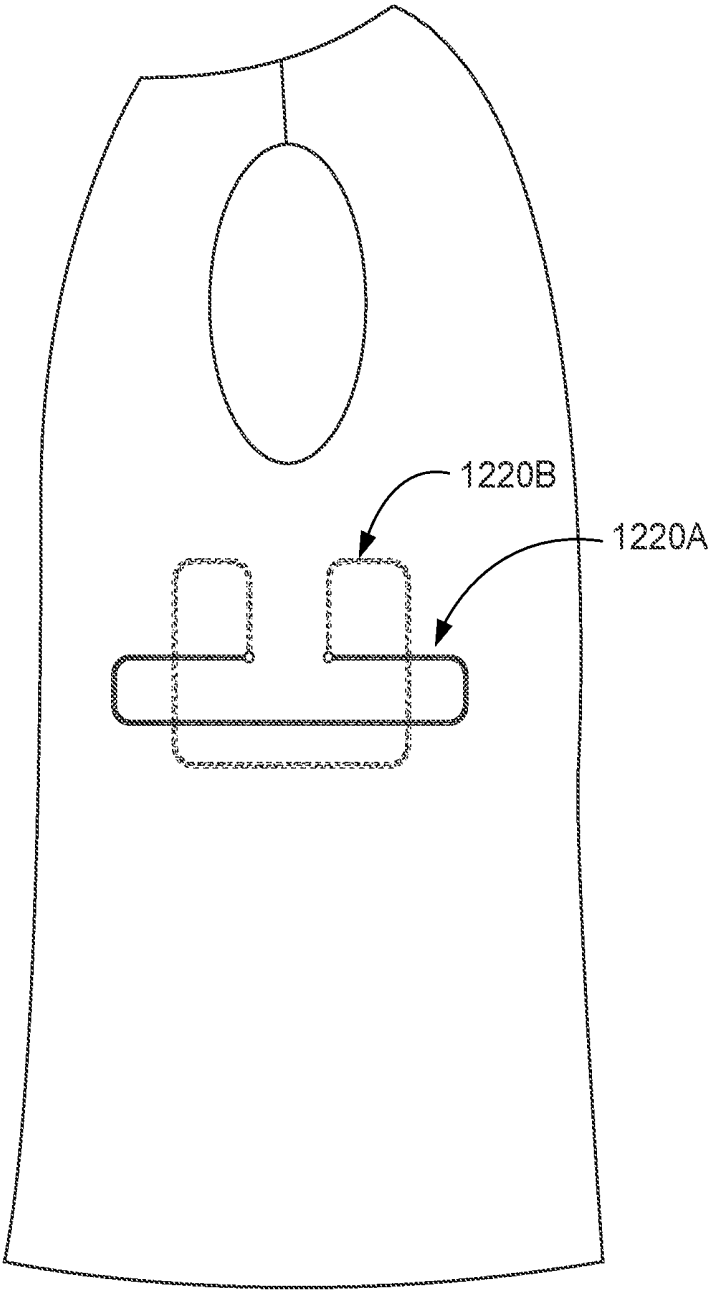


FIG. 12

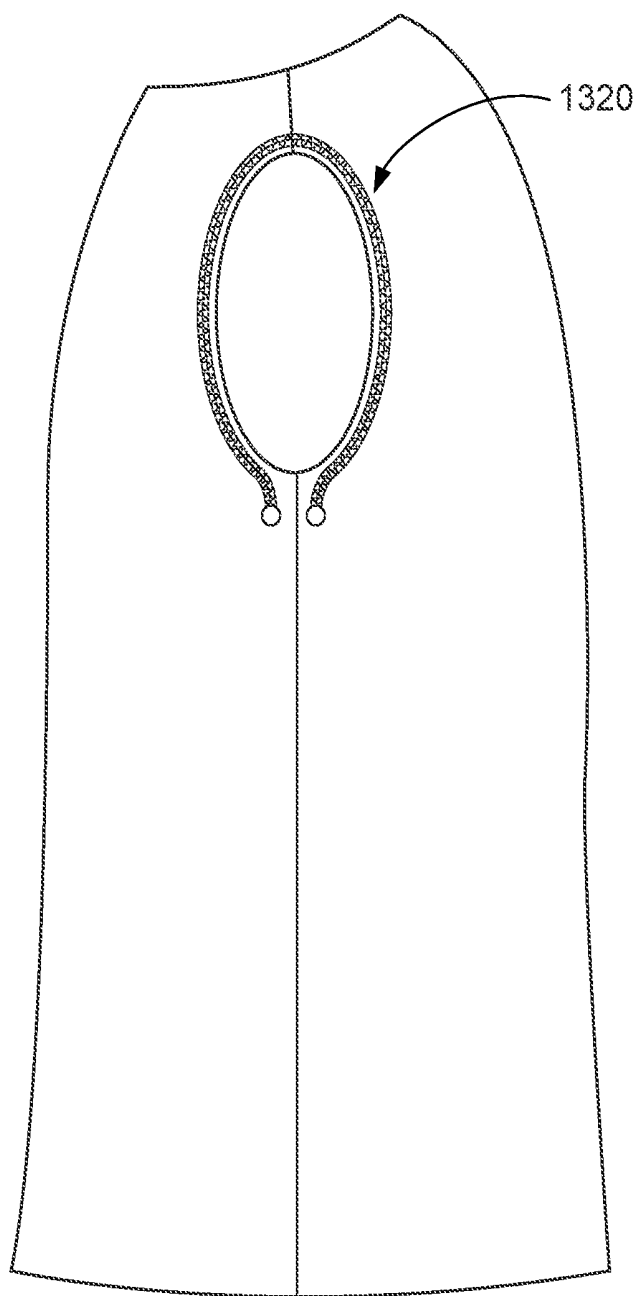
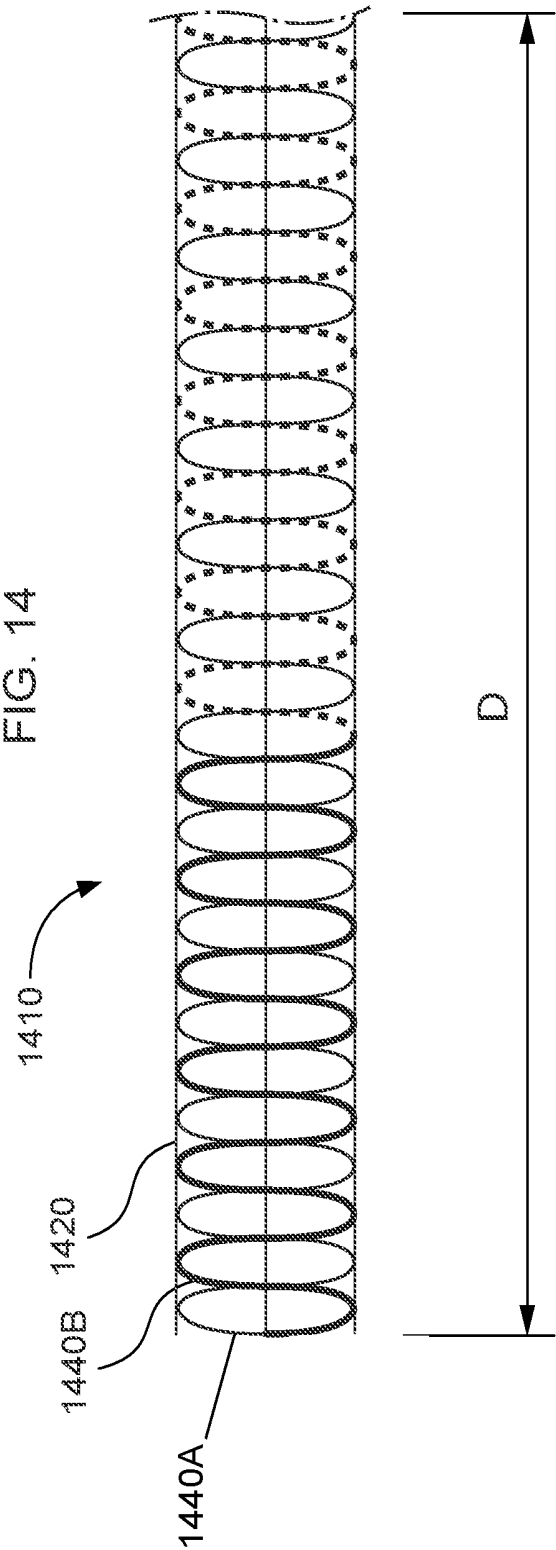


FIG. 13

FIG. 14



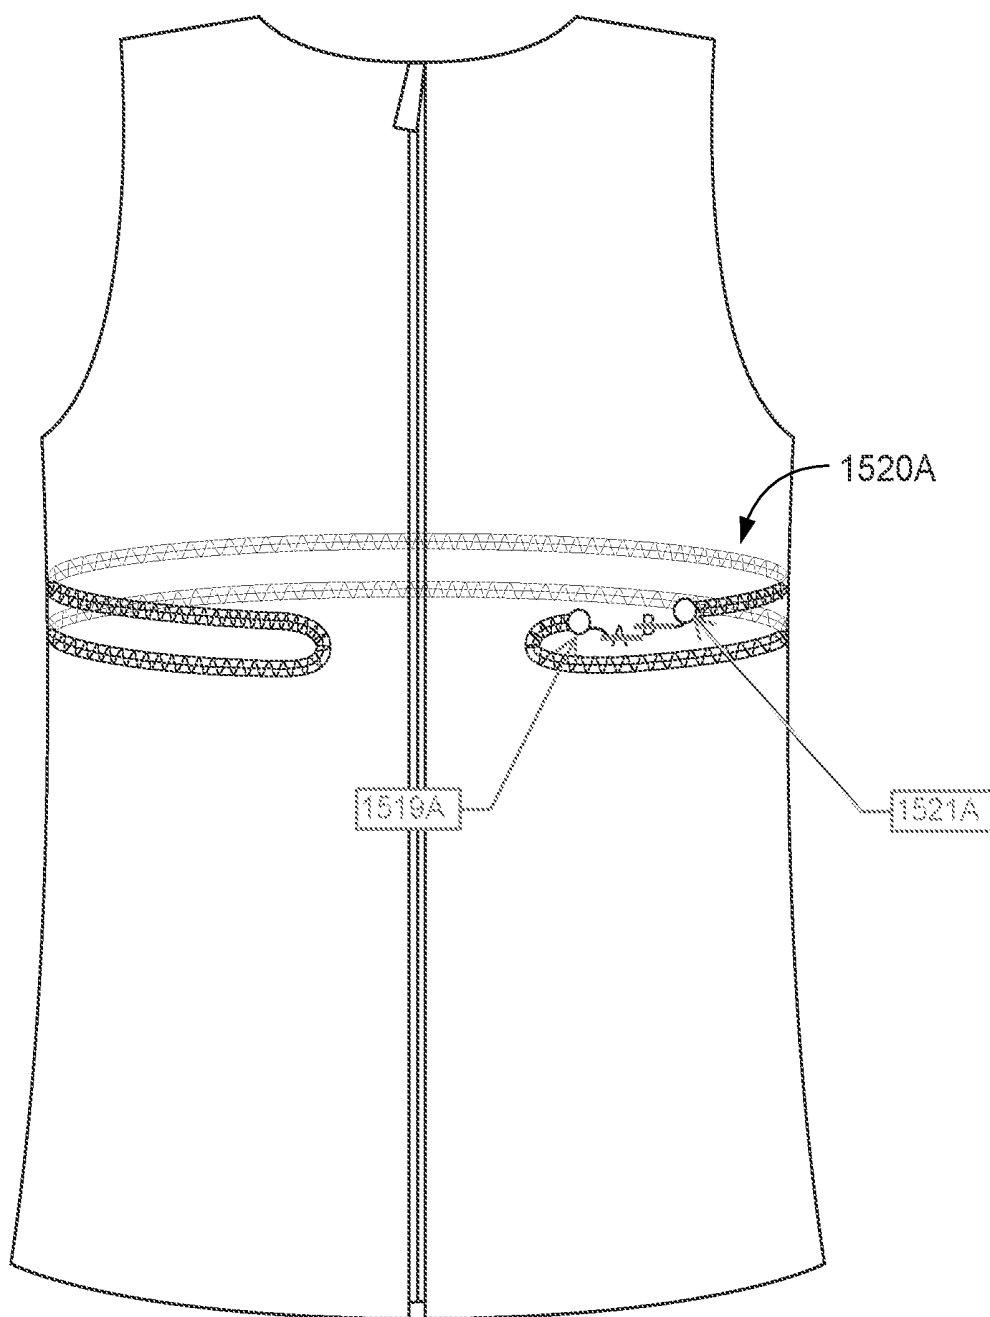


FIG. 15A

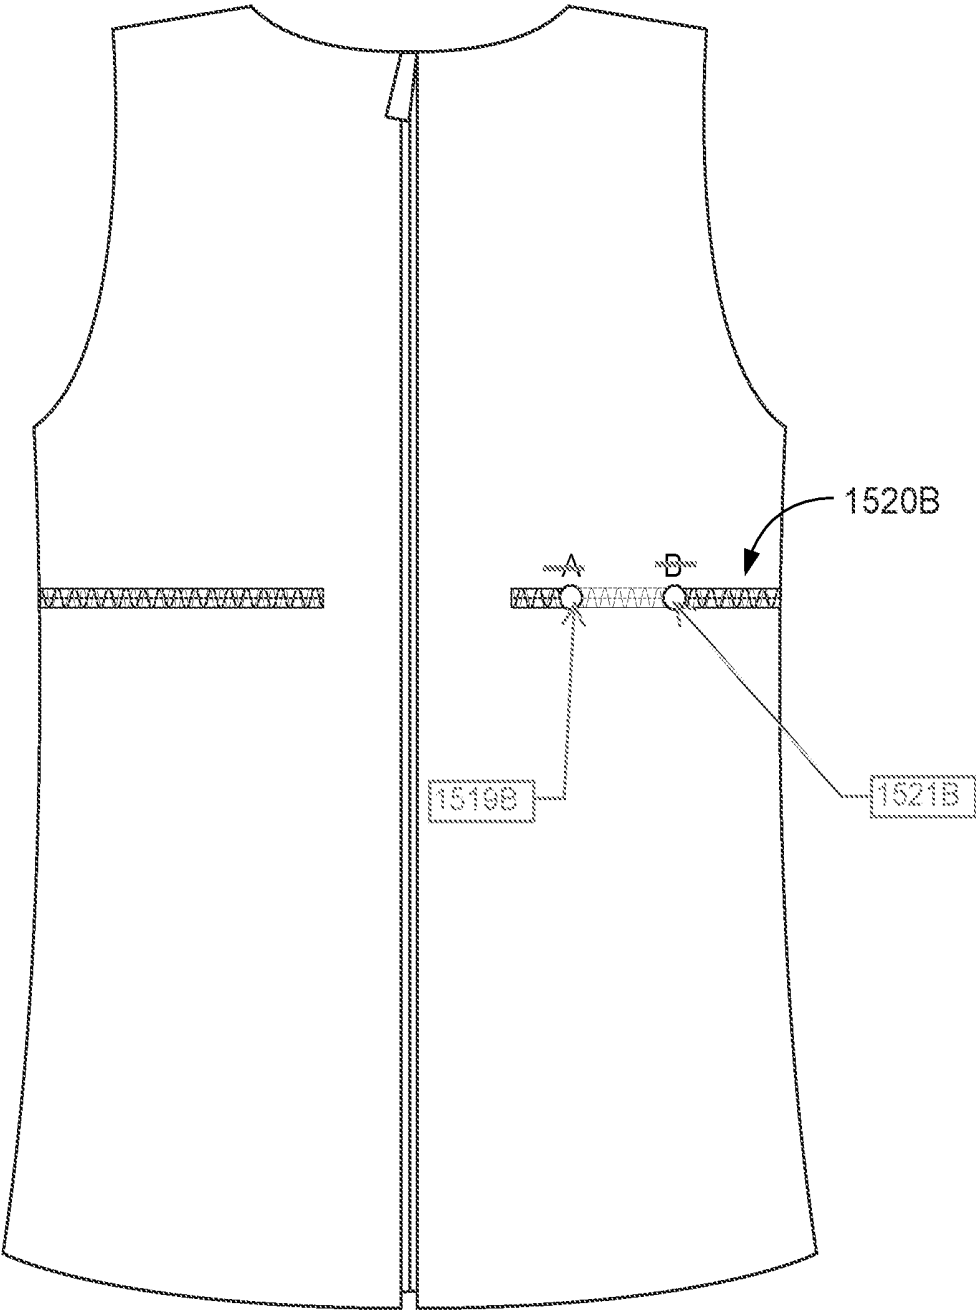
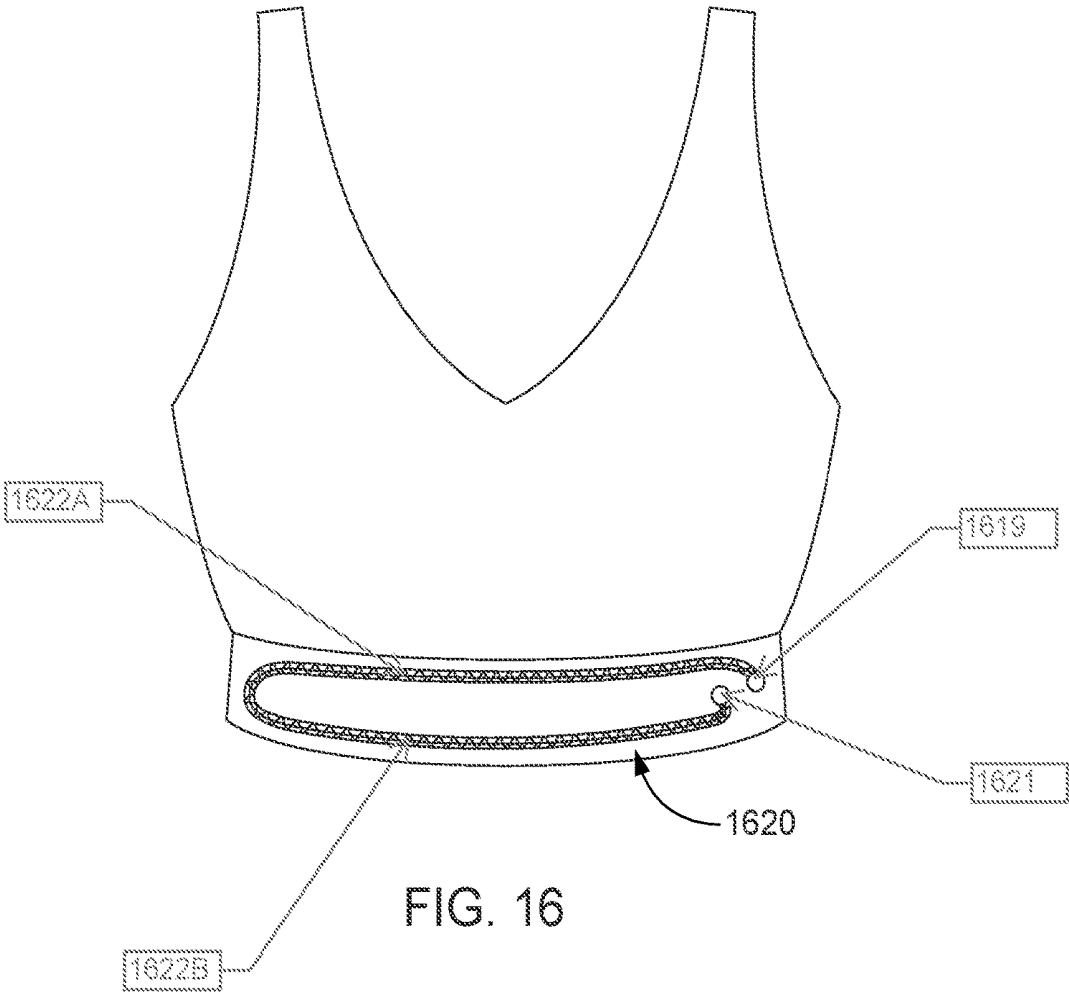
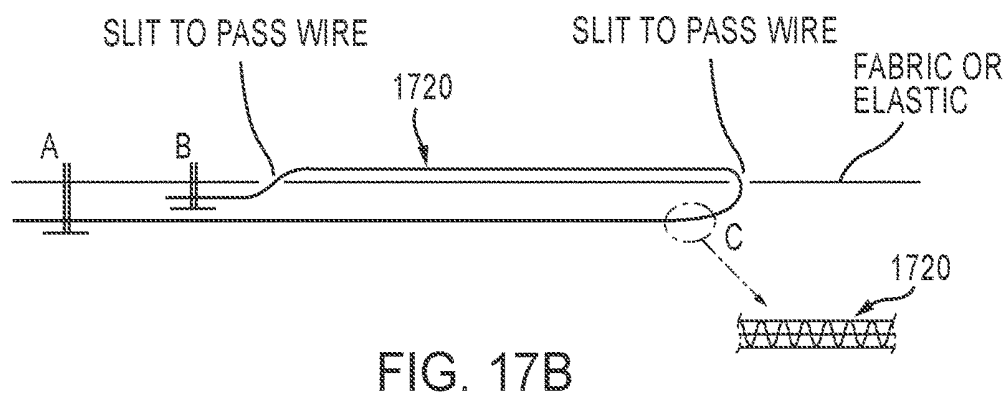
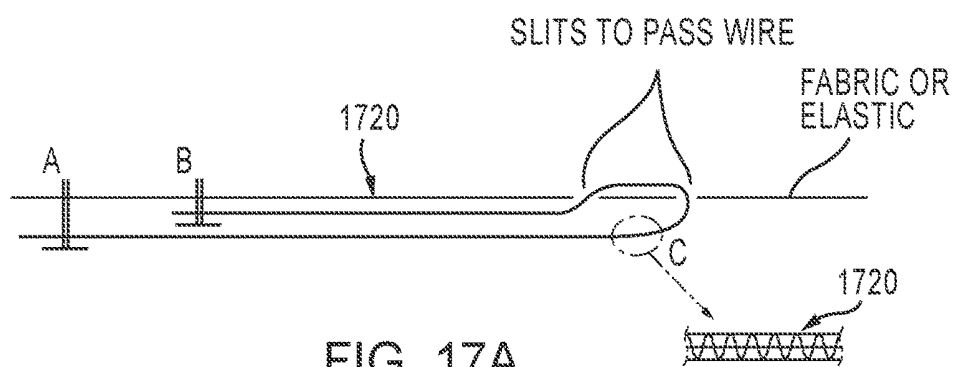
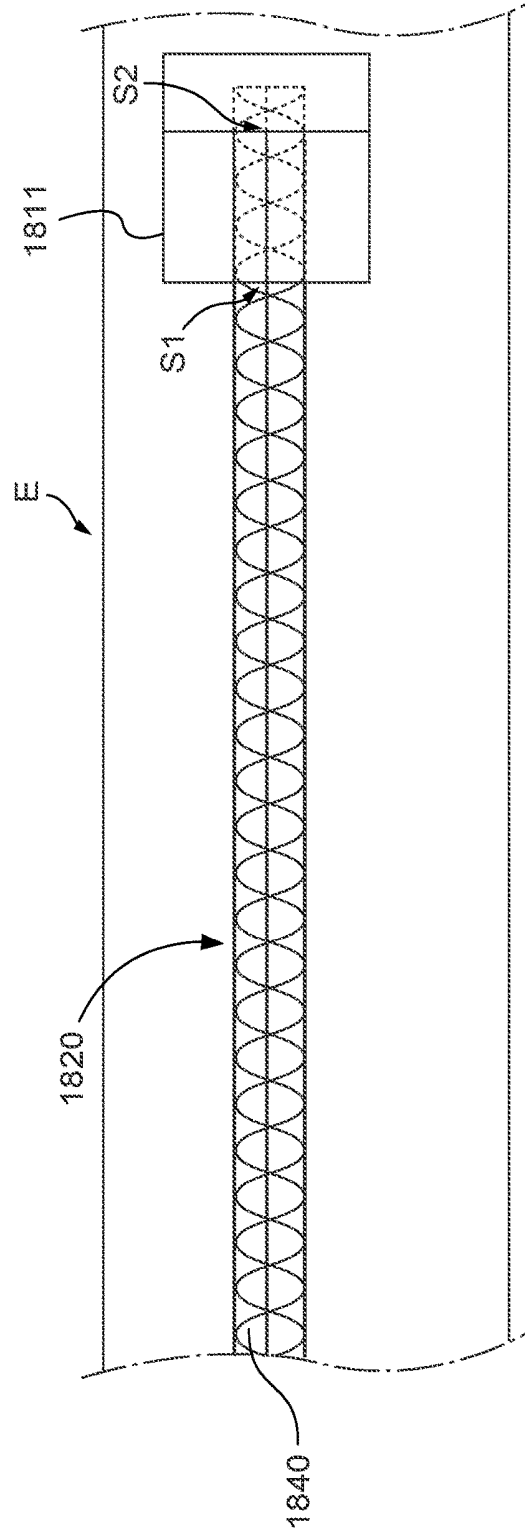
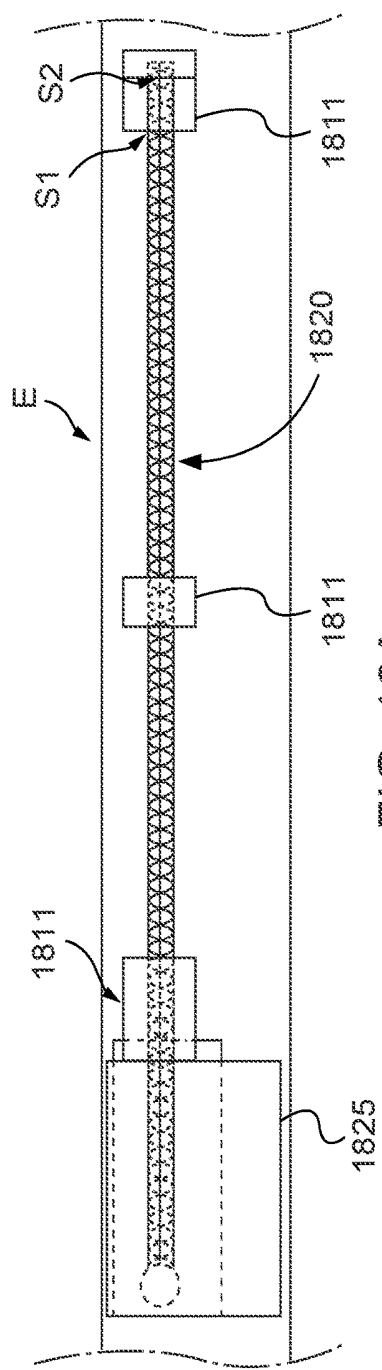
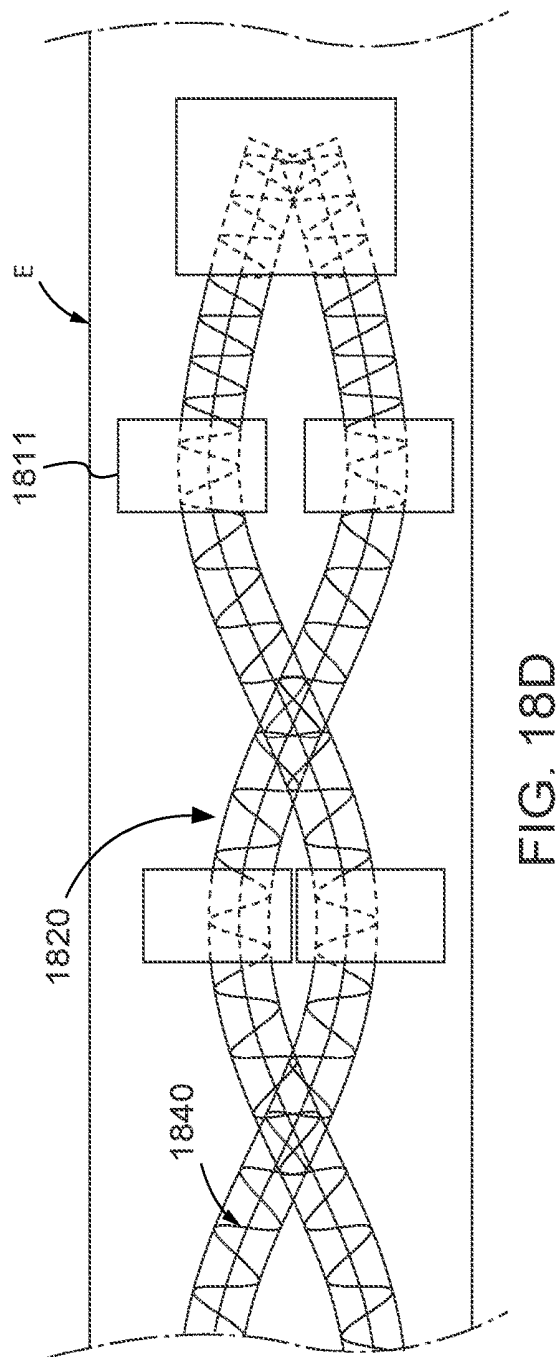
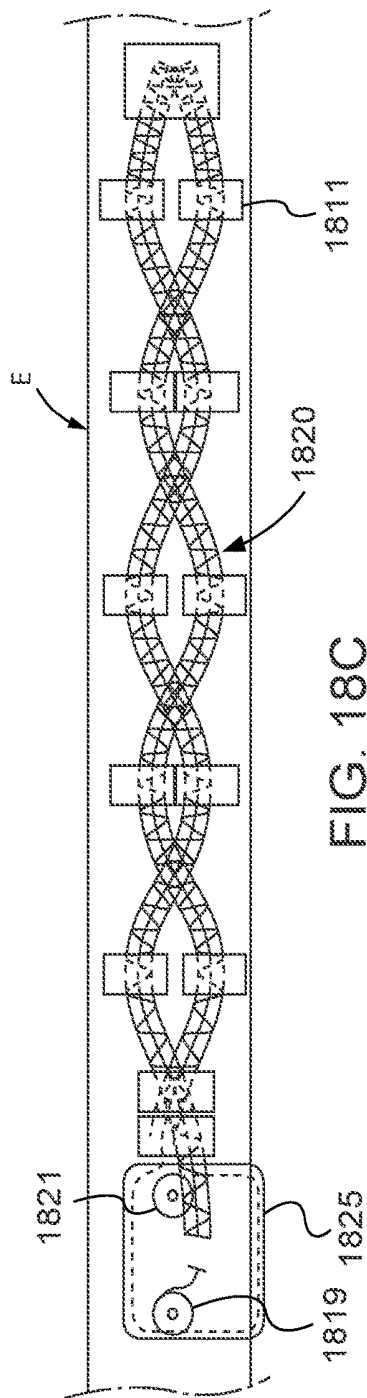


FIG. 15B









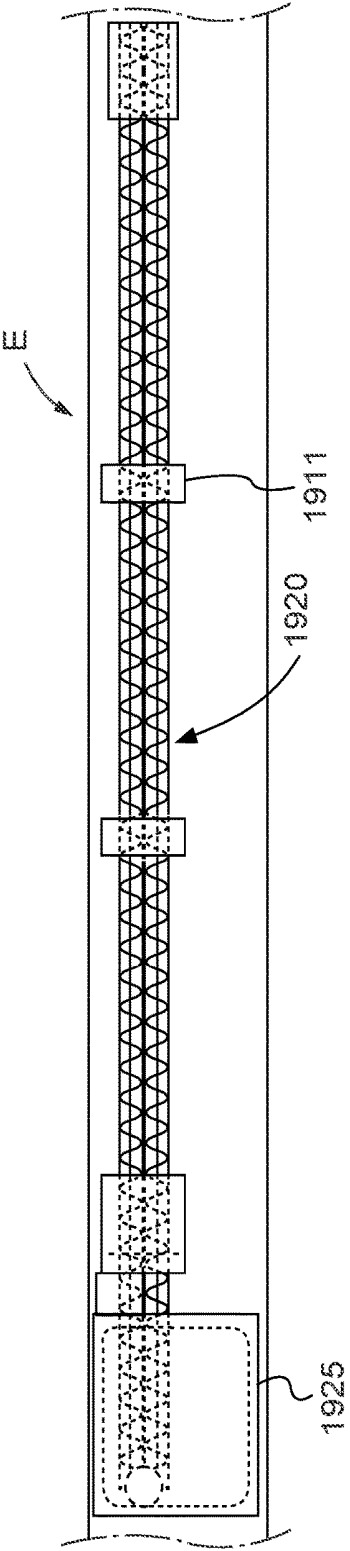


FIG. 19A

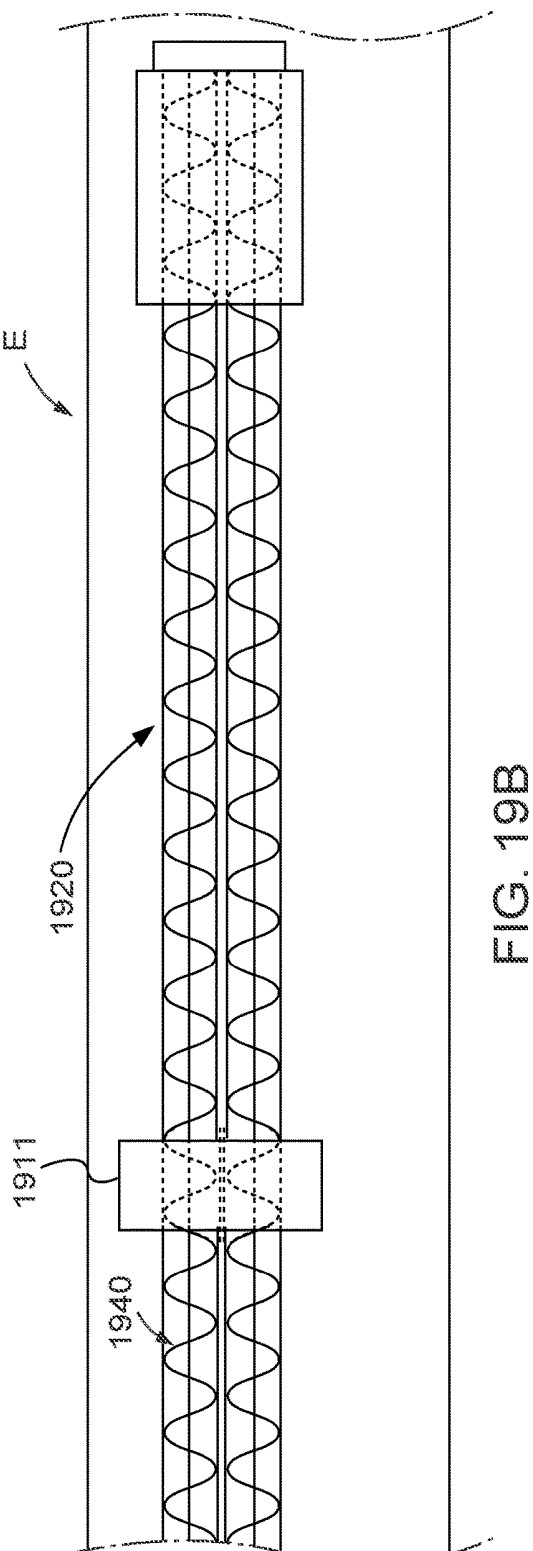
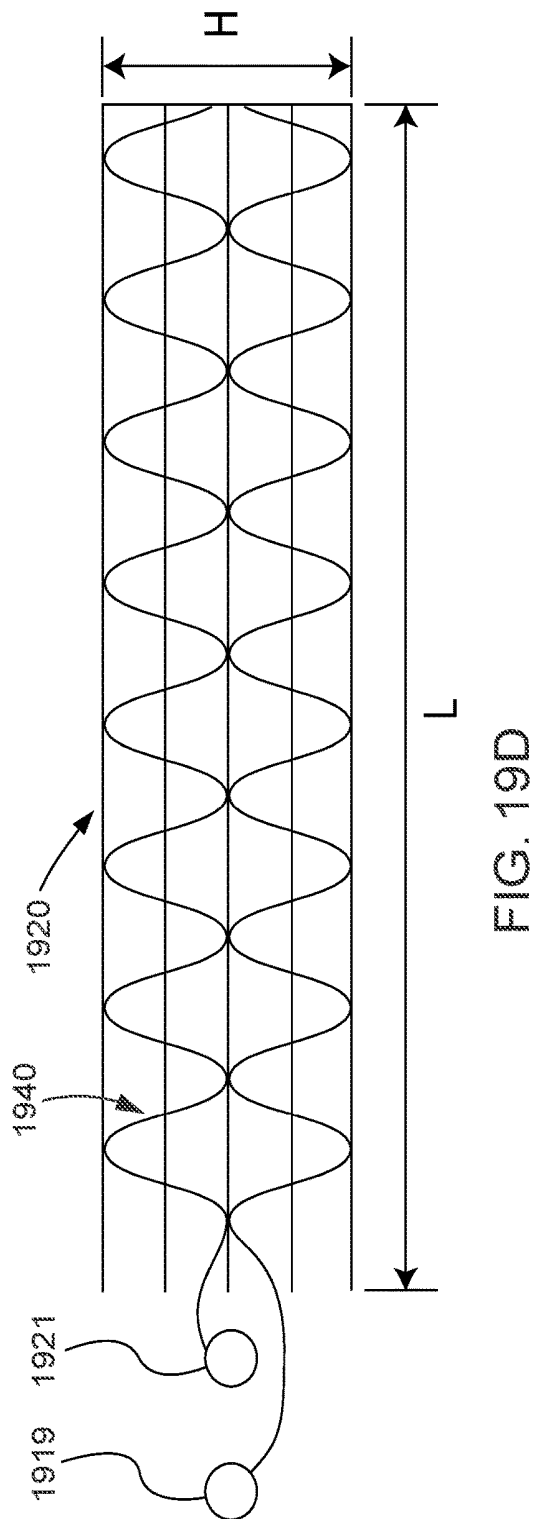
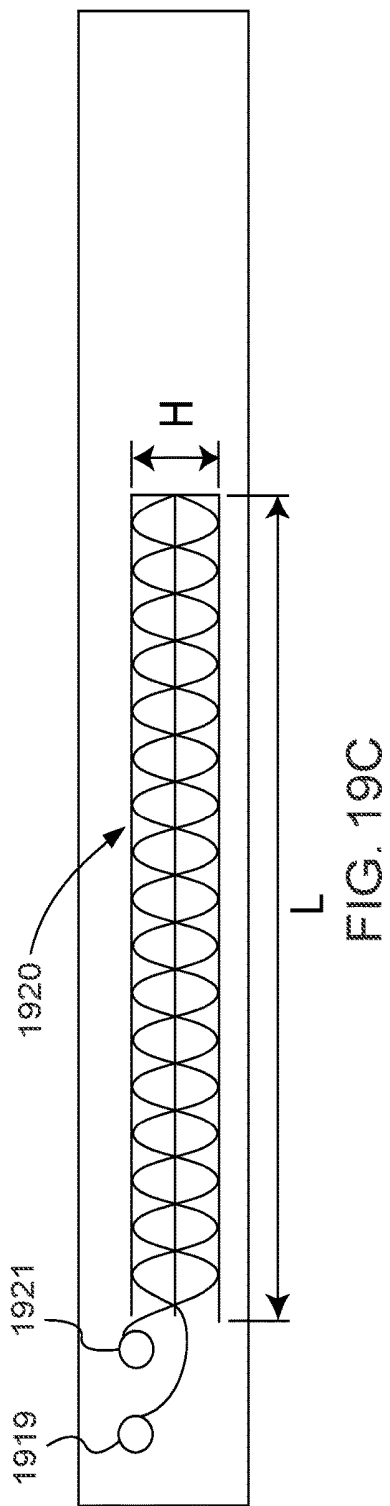


FIG. 19B



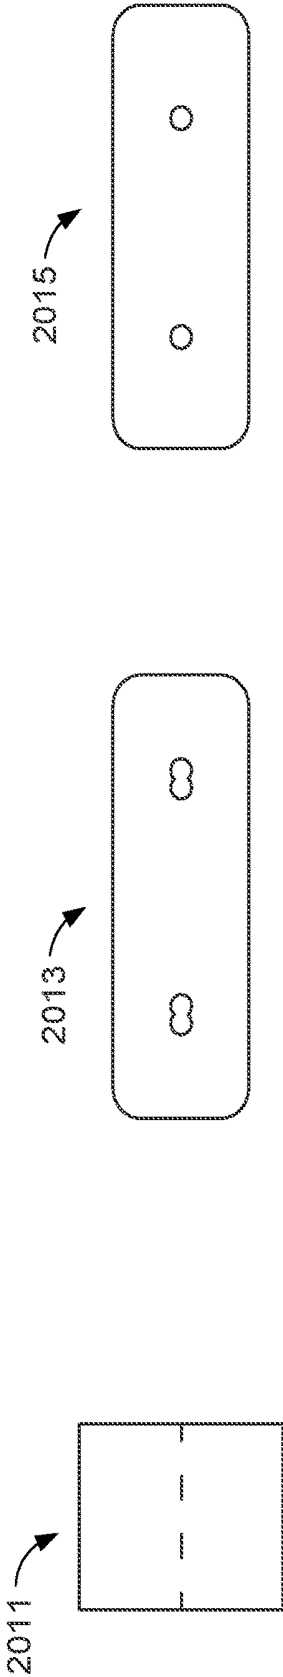


FIG. 20A

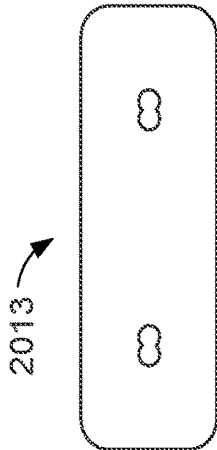


FIG. 20B

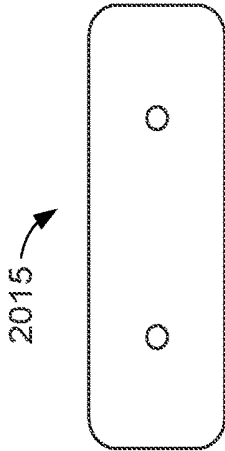


FIG. 20C

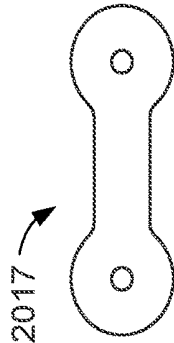


FIG. 20D




FIG. 20E




FIG. 20F

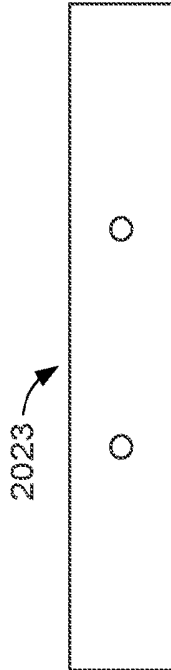


FIG. 20G

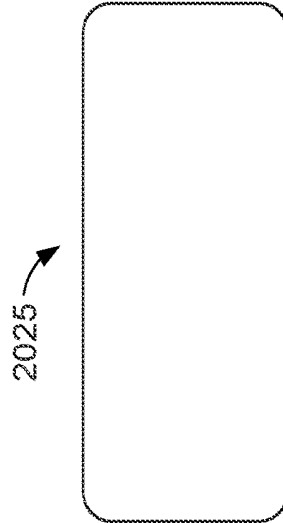


FIG. 20H

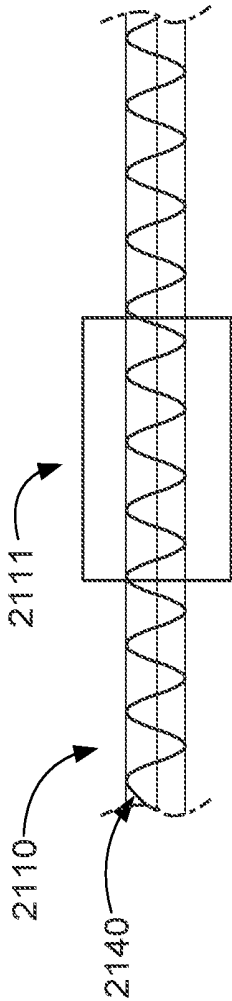


FIG. 21A

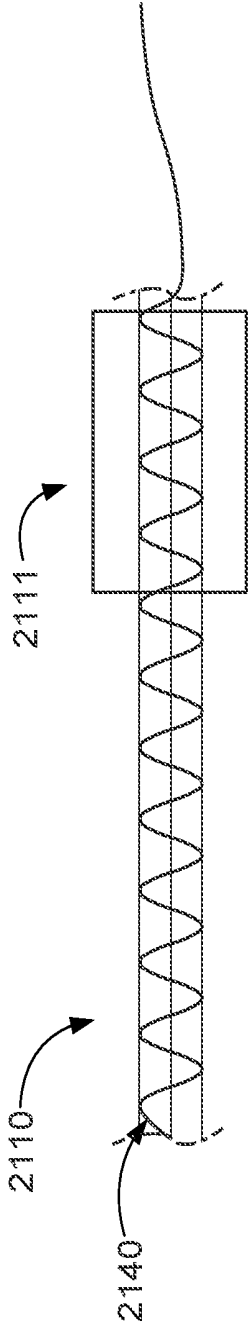


FIG. 21B

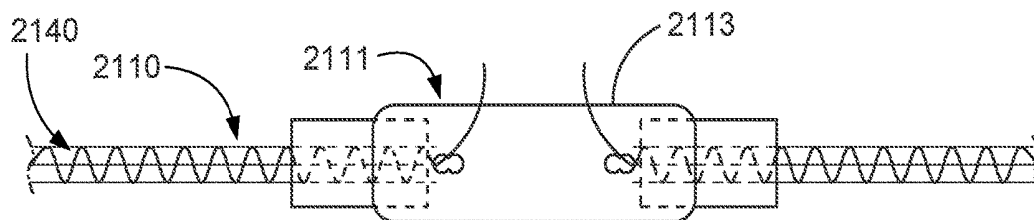


FIG. 21C

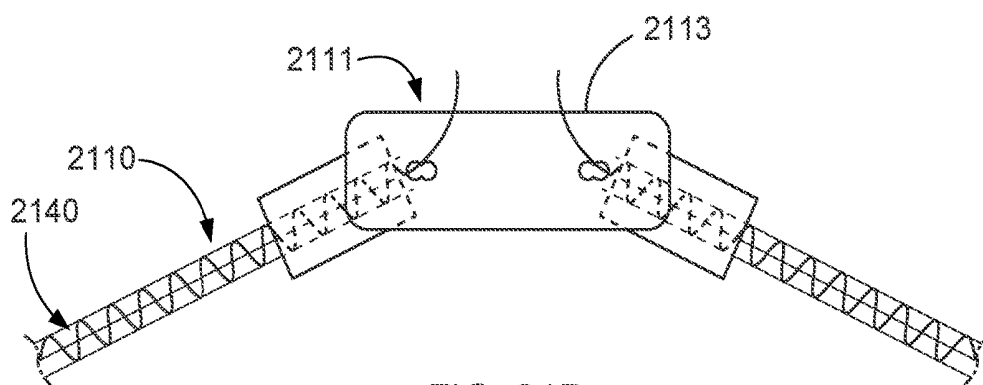


FIG. 21D

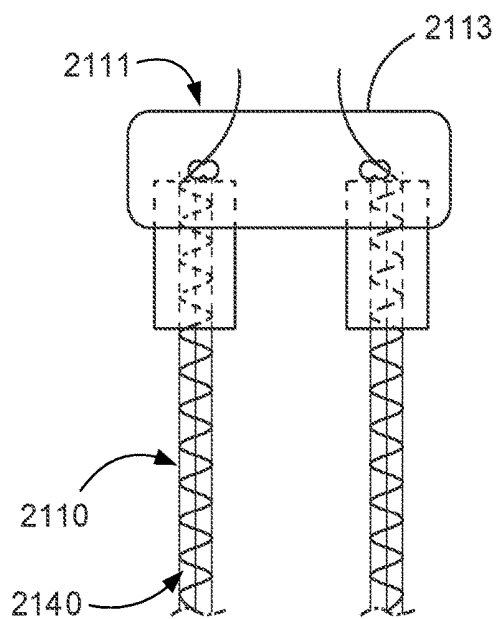


FIG. 21E

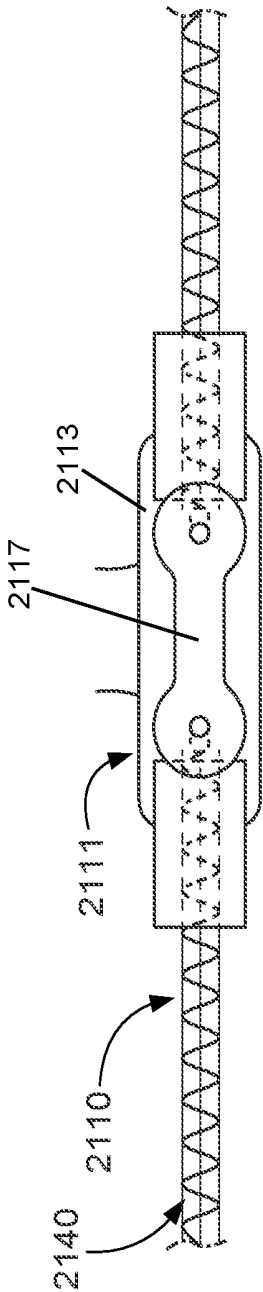


FIG. 21F

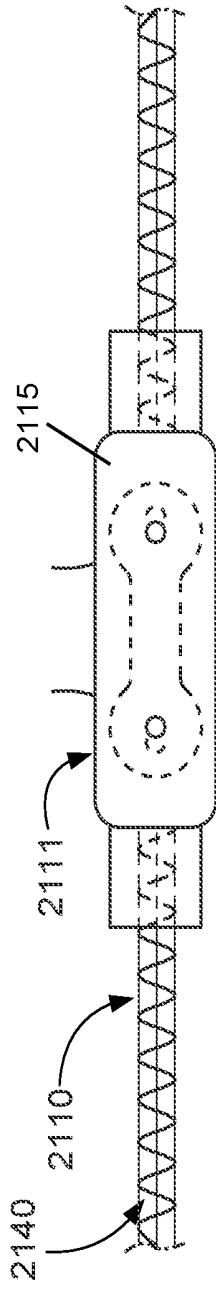


FIG. 21G

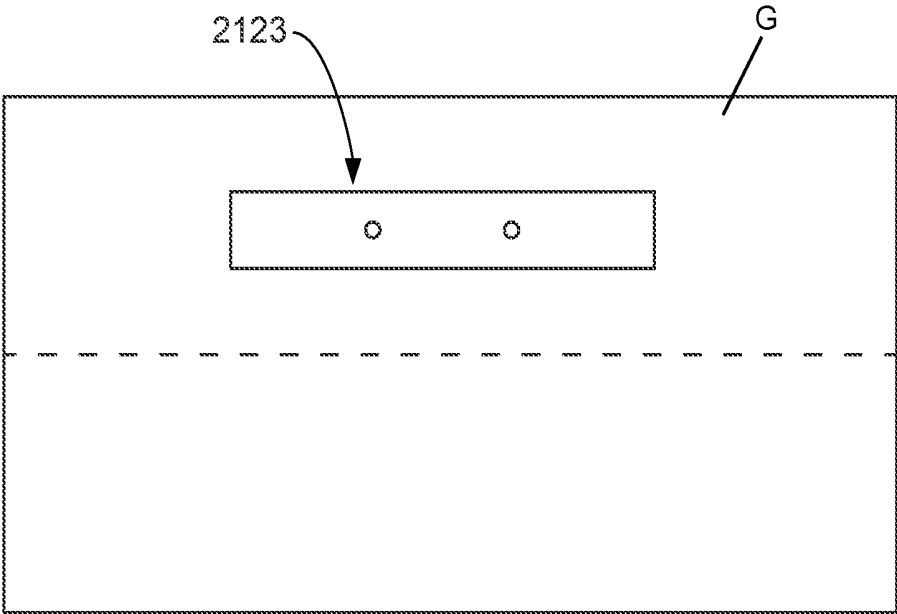


FIG. 21H

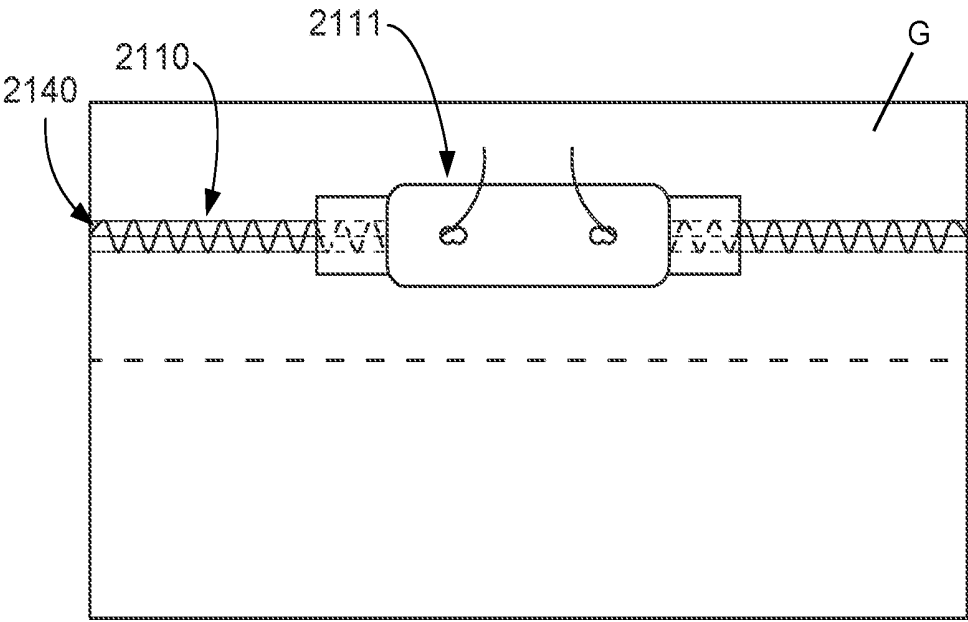


FIG. 21I

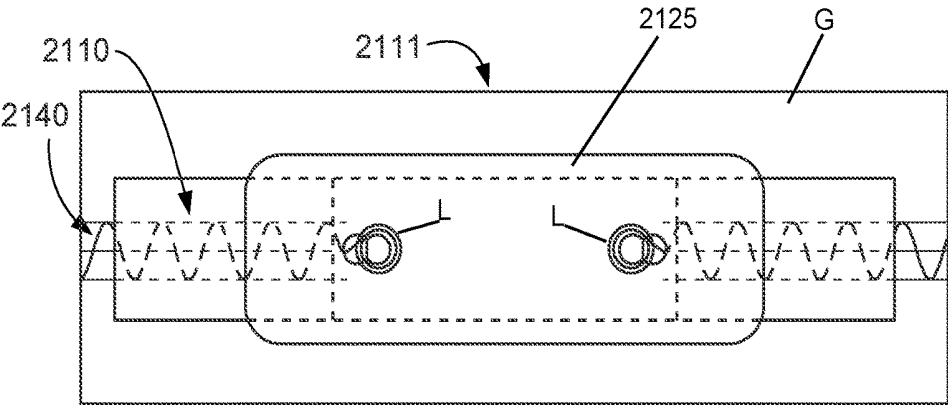


FIG. 21J

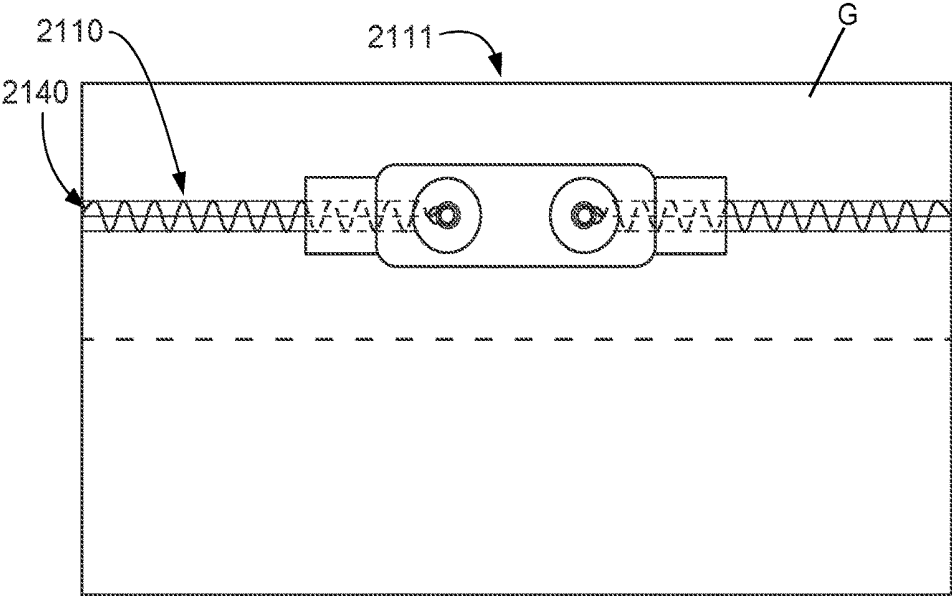


FIG. 21K

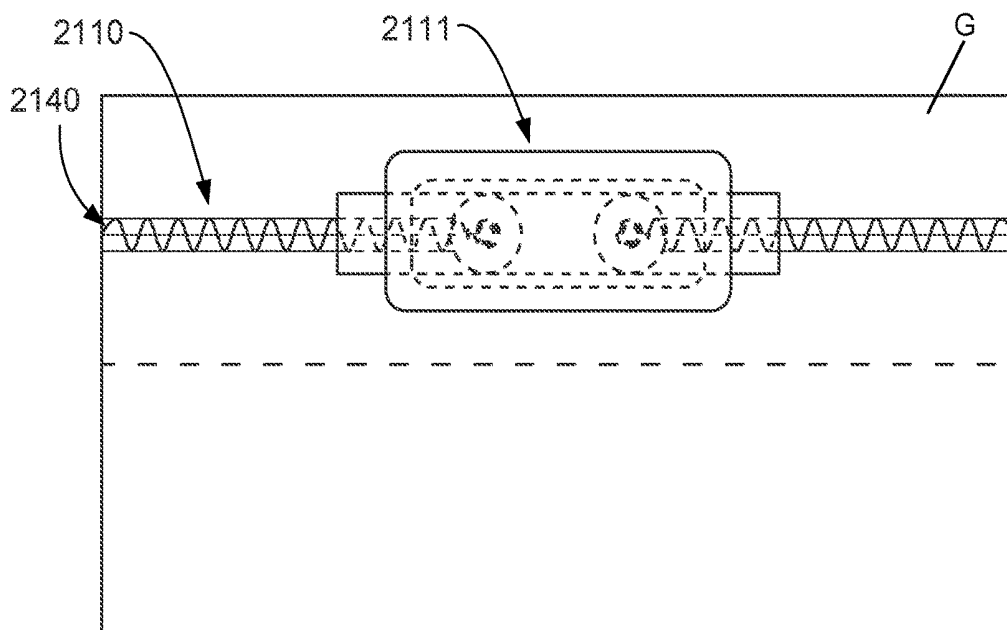


FIG. 21L

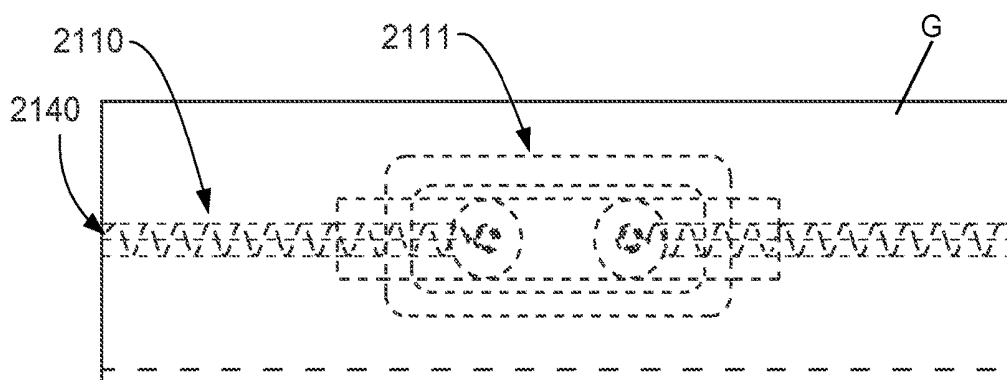


FIG. 21M

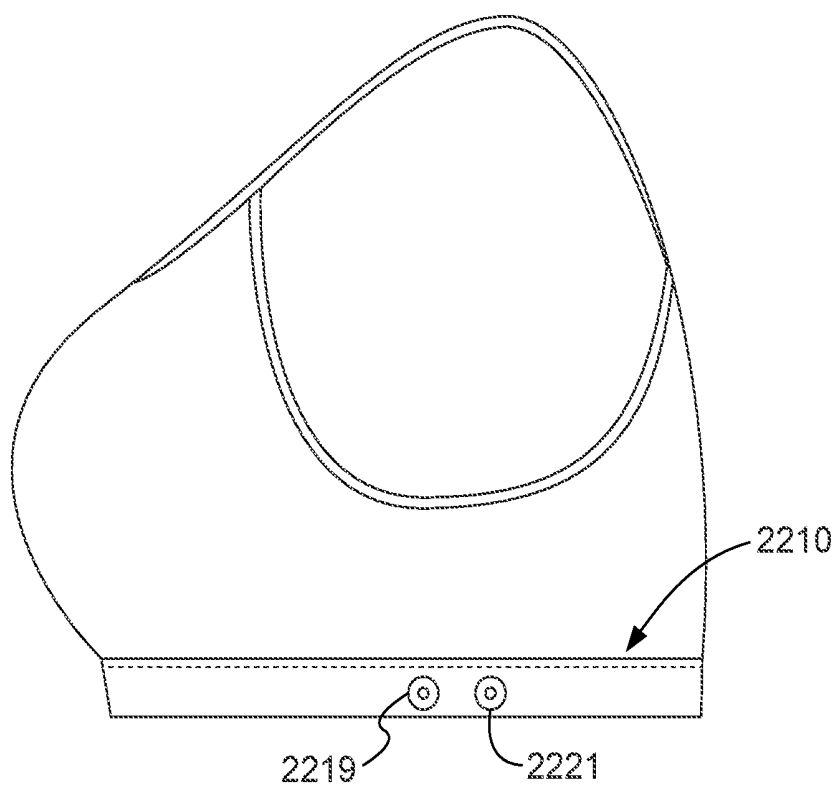


FIG. 22A

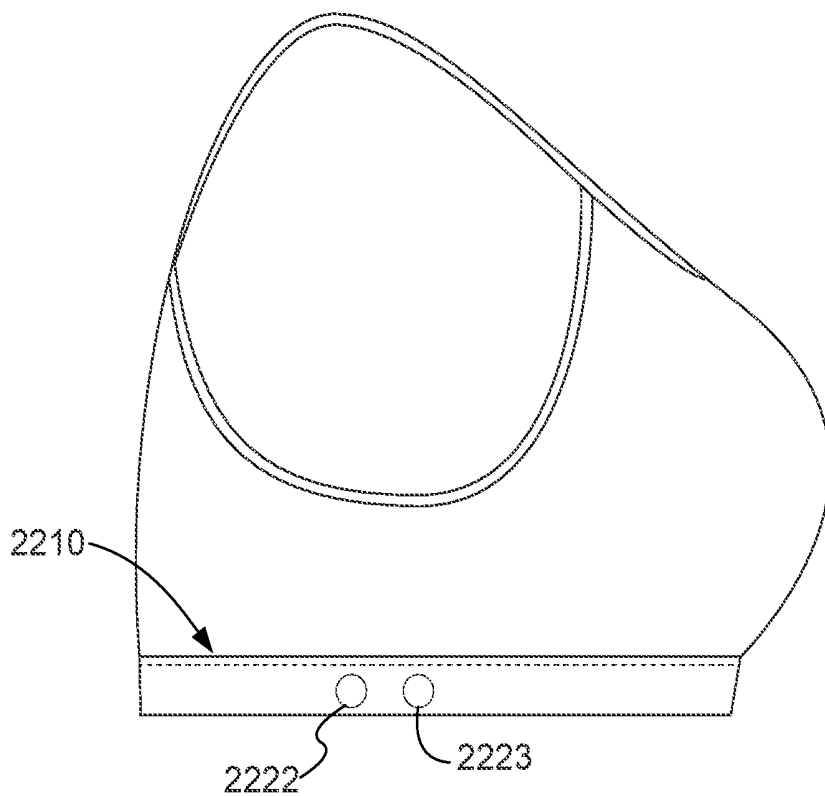
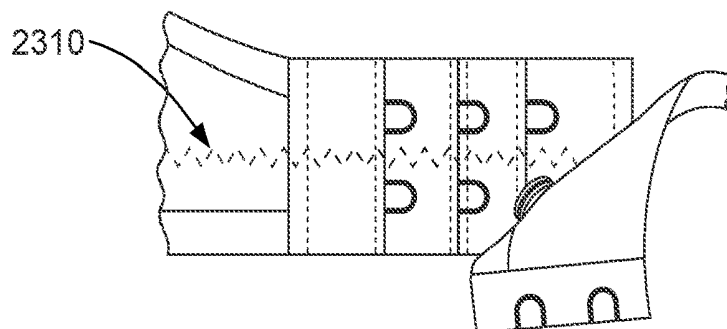
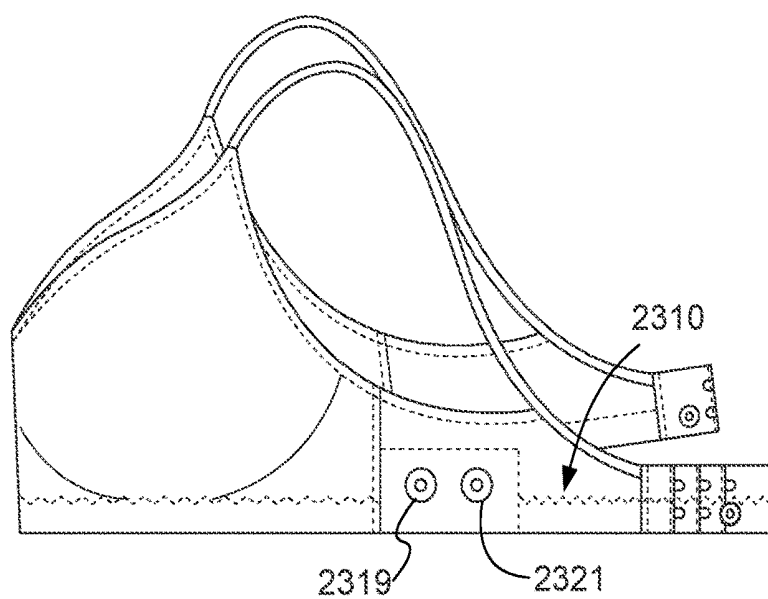
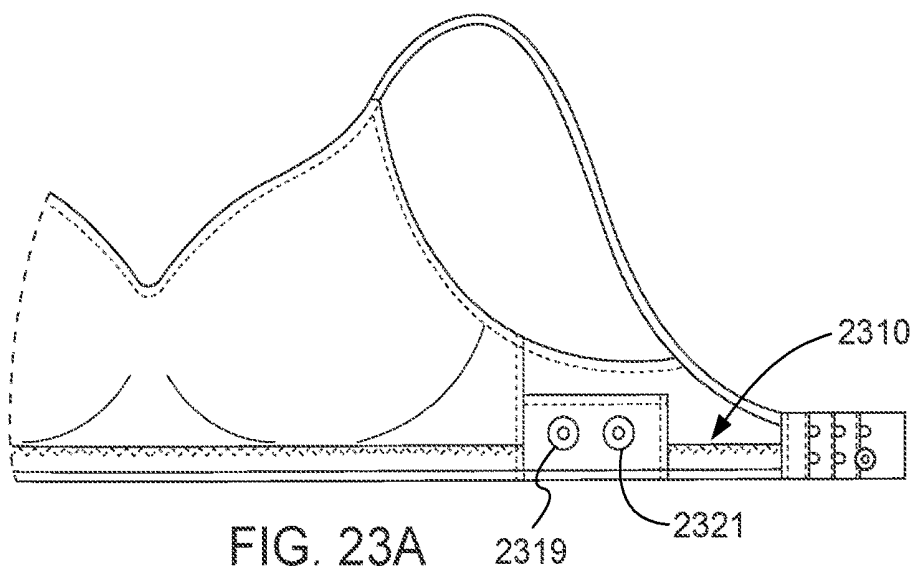


FIG. 22B



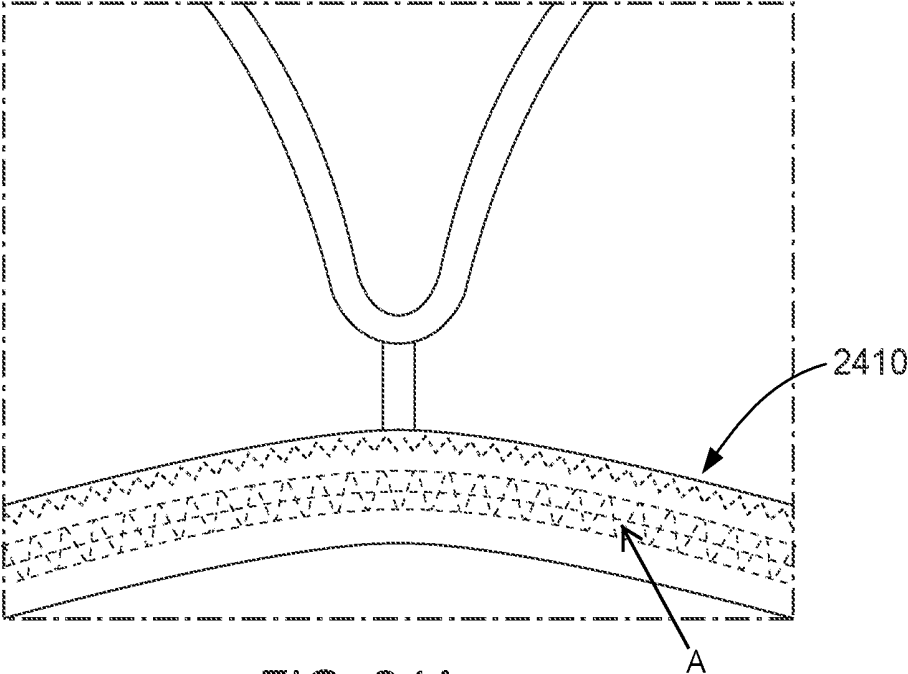


FIG. 24A

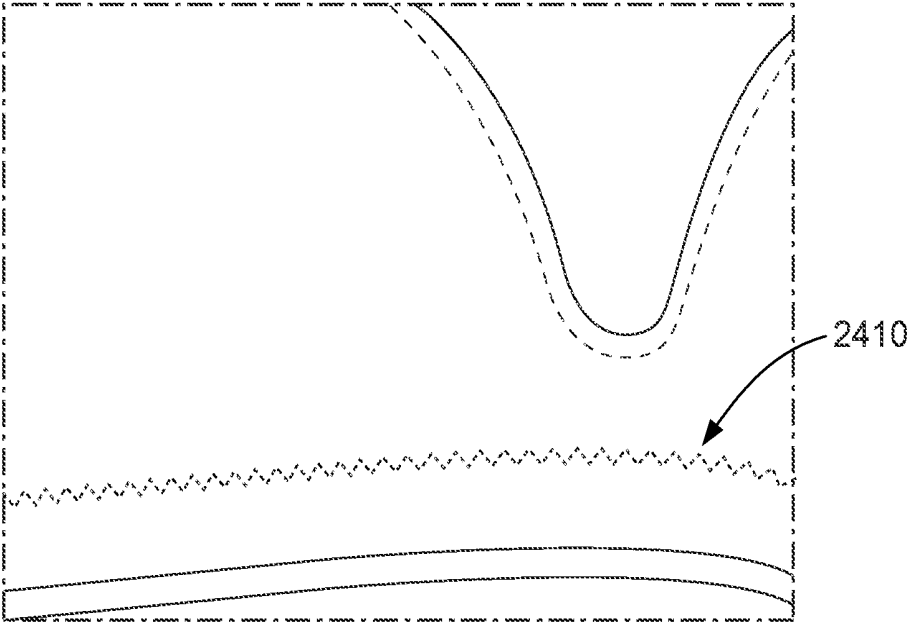


FIG. 24B

FIG. 25A

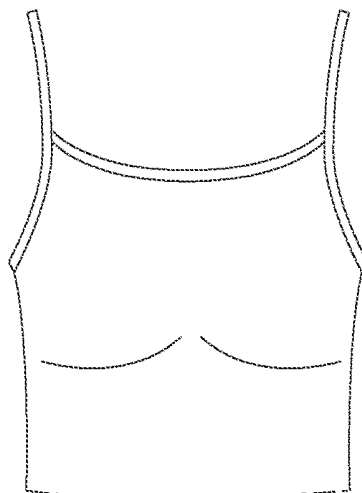


FIG. 25B


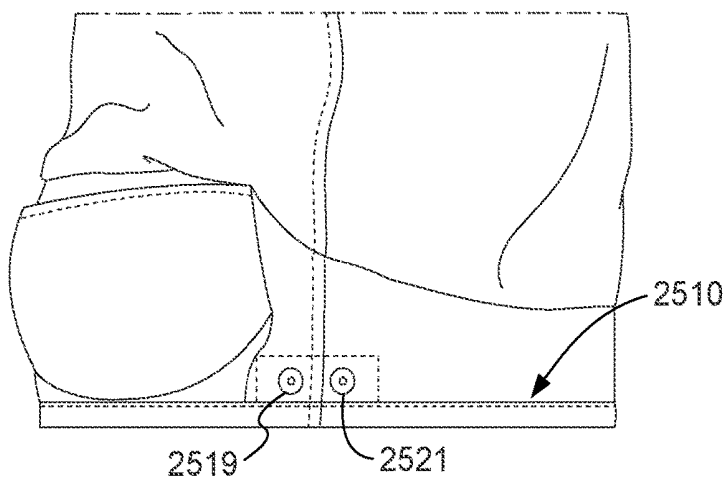


FIG. 25C

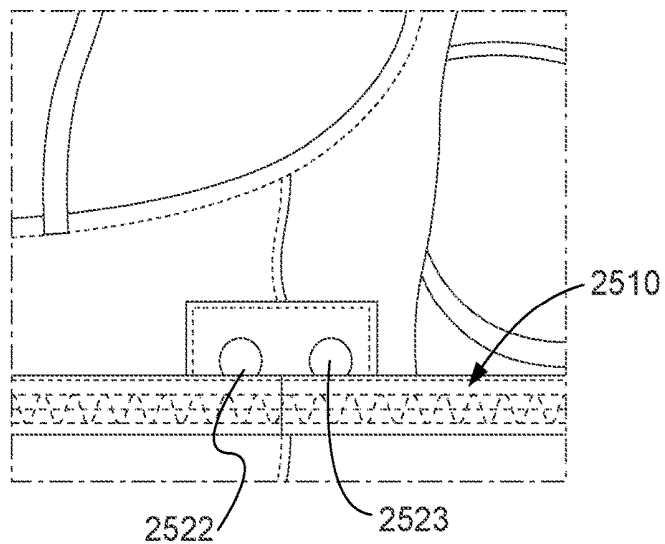

SYSTEMS AND METHODS FOR MONITORING RESPIRATION IN A BIOSENSING GARMENT

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to and the benefit of U.S. Provisional Application No. 62/212,899, entitled “Systems And Methods For Monitoring Respiration In A Biosensing Garment,” filed Sep. 1, 2015, and U.S. Provisional Application No. 62/247,049, entitled “Systems And Methods For Monitoring Respiration In A Biosensing Garment,” filed Oct. 27, 2015, the disclosures of which are incorporated herein by reference in their entirety.

BACKGROUND

[0002] Consumers of wearable electronics and other electronic textiles (“e-textiles”) demand ever-increasing levels of performance and functionality. Such functionality can include biosensors as well as interfaces with other smart technology. Although e-textile technology is theoretically applicable to a wide range of industries and applications, in practice electronic garment designs differ from traditional circuit designs in ways that make them less robust and, as a result, less reliable.

SUMMARY

[0003] Embodiments described herein relate generally to biosensing garments, and in particular, to systems and methods for monitoring respiration in a biosensing garment, whereby an improved integration of the respiration monitoring circuit into the garment is achieved, resulting in improved signal quality and durability. In some embodiments, an apparatus includes an elongate member having a longitudinal axis and configured to be stretchable along its longitudinal axis. The elongate member includes a plurality of elastic members (e.g., a first elastic member, a second elastic member, and a third elastic member) that extend along the longitudinal axis. For example, the elongate member can include a first elastic member extending along the longitudinal axis, a second elastic member that extends substantially parallel to the first elastic member, and a third elastic member that extends substantially parallel to the second elastic member. A conductive member is coupled to the first, second and third members, and forms a “curved” pattern along the longitudinal axis of the elongate member. The conductive member (and, correspondingly, its curved pattern) is configured to change from a first configuration to a second configuration as the elongate member stretches along its longitudinal axis. This change of configuration results in a change in an inductance value of the conductive member.

BRIEF DESCRIPTION OF THE DRAWINGS

[0004] FIG. 1 is a schematic illustration of an elongate member according to an embodiment, in an exemplary environment.

[0005] FIG. 2A shows a front schematic plan view, and FIG. 2B shows a back schematic plan view, of a biosensing garment having an elongate member disposed on an interior surface thereof, according to an embodiment.

[0006] FIG. 3 is a schematic illustration of an elongate member, according to an embodiment.

[0007] FIG. 4 is a schematic illustration of an elongate member, according to an embodiment.

[0008] FIG. 5 is a schematic illustration of an elongate member, according to an embodiment.

[0009] FIG. 6 is a schematic illustration of an elongate member, according to an embodiment.

[0010] FIGS. 7A-7C are schematic illustrations showing elongate member/conductive wire combinations, according to embodiments of the disclosure.

[0011] FIGS. 8A and 8B show elongate members, according to embodiments of the disclosure.

[0012] FIG. 9 is a schematic illustration of an elongate member, according to an embodiment.

[0013] FIGS. 10A-10C are schematic illustrations showing configurations of an elongate member, according to some embodiments.

[0014] FIG. 11 is a schematic illustration showing a configuration of an elongate member, according to some embodiments.

[0015] FIG. 12 is a schematic illustration showing a configuration of an elongate member, according to some embodiments.

[0016] FIG. 13 is a schematic illustration showing a configuration of an elongate member, according to some embodiments.

[0017] FIG. 14 is a schematic illustration showing a folded configuration of an elongate member, according to some embodiments.

[0018] FIGS. 15A-15B are schematic illustrations showing configurations of an elongate member, according to some embodiments.

[0019] FIG. 16 is a schematic illustration showing a configuration of an elongate member, according to some embodiments.

[0020] FIGS. 17A-17B are schematic illustrations showing cross-sectional views of a folded configuration of an elongate member, according to some embodiments.

[0021] FIGS. 18A-18B are schematic illustrations showing a folded configuration of an elongate member incorporated into a garment, according to an embodiment.

[0022] FIGS. 18C-18D are schematic illustrations showing a folded configuration of an elongate member incorporated into a garment, according to an embodiment.

[0023] FIGS. 19A-19B are schematic illustrations showing a folded configuration of an elongate member incorporated into a garment, according to an embodiment.

[0024] FIGS. 19C-19D are schematic illustrations showing a looped wire configuration of an elongate member incorporated into a garment, according to an embodiment.

[0025] FIGS. 20A-20H show components of an assembly process, according to an embodiment.

[0026] FIGS. 21A-21M show aspects of an assembly process, according to an embodiment.

[0027] FIG. 22A shows an exterior view, and FIG. 22B shows an interior view, of an assembled biosensing garment, according to an embodiment.

[0028] FIGS. 23A-23C show views of an assembled biosensing garment, according to an embodiment.

[0029] FIG. 24A shows an interior view, and FIG. 24B shows an exterior view, of an assembled biosensing garment, according to an embodiment.

[0030] FIGS. 25A-25C show views of an assembled biosensing garment, according to an embodiment.

DETAILED DESCRIPTION

[0031] Wearable electronics such as biosensing garments (and the electronic textiles from which they are made) are subjected to different mechanical stresses than traditional electronic systems. For example, biosensing garments may be stretched during enrobing, disrobing, and wear (e.g., during physical activity of the wearer). This stretching can result in deformation of conductors and/or sensor elements that are embedded within and/or secured to a surface of the biosensing garment. As a result, wearable electronics often suffer from compromised performance after only limited period of use. According to embodiments of the present disclosure, an improved integration of a physiological sensor (or components thereof) into a biosensing garment is achieved, resulting in improved signal quality, durability and reliability. Such physiological sensors include an elongate member and a conductive member (also referred to herein as a “conductive wire”). Specifically, embodiments of the present disclosure describe a respiration monitoring circuit that includes the elongate member and the conductive wire coupled to the elongate member in a pre-defined pattern and using knitting, braiding, weaving, and/or other attachment methods described herein.

[0032] Biosensing garments of the present disclosure are flexible enough to accommodate enrobing and disrobing (“putting on” and “taking off,” respectively) in a manner that is comfortable or tolerable to a user, yet remains capable of detecting subtle changes in inductance during use, with an improved performance lifespan (e.g., reduced degradation of signal or “wearing out” of the biosensing infrastructure). In some embodiments, an elongate member, bearing an extensible, insulated or non-insulated (bare) conductive wire (collectively also referred to herein as a “breathing cable”), forms at least part of a respiration monitoring circuit (e.g., is a “respiratory inductance plethysmography” or “RIP” sensor), and is incorporated into a biosensing garment. The elongate member is configured to be disposed around an at least partial circumferential region of a wearer (also referred to herein as “user”). The at least partial circumferential region of the user may include at least a portion of the user’s chest, rib cage, abdomen, and/or waist. The elongate member, when disposed about the circumference of a user, is configured to be held closely to the user’s body. When the elongate member is disposed in this manner, the conductive wire has an intrinsic inductance value (“self-inductance”) related to its shape or “pattern” (for example, its frequency, amplitude and/or periodicity). The inductance value of the conductive wire changes substantially proportionately in response to changes in the geometry (e.g., antero-posterior diameter, circumference, cross-sectional area, etc.) of the user’s anatomy, for example as a result of the user’s respiratory movements (breathing, inhalation, inspiration, exhalation, coughing, yawning, and/or the like) or other movements (exertion, muscle flexion, coughing, yawning, stretching, posture, and/or the like). The user’s respiratory movements involve changes in the user’s lung volume, compartmental torso volume, ventilation, inspired breath volume, etc. As a result, a user’s lung volume, respiratory rate (e.g., breaths per minute), tidal volume, ventilation (e.g., minute ventilation), peak inspiratory flow, fractional inspiratory time, work of breathing, peak/mean inspiratory and expiratory flow, % RCi (percent contribution of rib cage excursions to the tidal volume), phase angle (“phi”), apnea status and/or classification, hypopnea status and/or classification,

qDEEL (quantitative difference of end expiratory lung volume) and/or inspired breath volume, along with other parameters like breathing patterns, can be measured through transduction or “sensing” of the changing inductance (including the timing of such changes) of the conductive wire. In order to continuously measure the user’s respiration, the conductive wire can be used as the inductor in a variable frequency LC oscillator (i.e., the conductive wire is connected to an LC circuit, in which the conductive wire acts as the inductor “L”). The LC oscillator can in turn be connected to a frequency-to-voltage converter, which can be connected to a scaling amplifier, which can be connected to a digital voltmeter or other suitable display.

[0033] Biosensing garments of the present disclosure include at least one, and in some embodiments multiple, elongate member/conductive wire combinations. Where multiple elongate member/conductive wire combinations are used, they may be co-located, or may be spaced apart by a pre-determined distance (for example, to measure and/or compare geometric information at disparate locations on a user’s anatomy, e.g., substantially concurrently at the chest and the abdomen). In some embodiments, a biosensing garment comprises elastic fabric that is designed to fit over a user’s body. At selected intervals, the elastic fabric includes one or more elongate members integrally (i.e., “monolithically”) with it, and the elongate members can be impregnated with a conductive material, such as silver. The elongate members can be spaced, for example, in parallel pairs and can serve as electrodes for impedance plethysmography instruments to be attached. The elongate members themselves can be at least partially elastic. The conductive material can be aluminum, gold, copper, or any other suitable conductor material. Impregnated elongate members can be woven or knit into the elastic fabric at the selected intervals as the garment is being manufactured, such that the finished garment presents a uniform interior and/or exterior surface. For example, in some embodiments, the biosensing garment and/or sensors can be substantially similar to or the same as the biosensing garment, sensors and/or electrodes included in U.S. Patent Publication No. 2014/0343390 entitled, “Textile Blank With Seamless Knitted Electrode,” (“the ‘390 Publication”), the disclosure of which is incorporated herein by reference in its entirety.

[0034] There are a number of drawbacks to existing biosensing garment technology. For example, in existing RIP sensor technology, differences in posture and/or thoraco-abdominal respiratory synchronization, accurate respiratory volumes often cannot be obtained using a single sensor (i.e., multiple sensors are required). Other difficulties include non-linear responses due to inexact coordination of the chest and abdomen (i.e., the two respiratory compartments). This makes certain respiratory indices difficult to measure, and limits the utility of some sensors to only respiration rates and other basic timing indices, and requiring a dual sensor system. Compounding these problems is the fact that existing RIP sensor implementations suffer from unwanted hysteresis effects, for example being unable to accommodate repeated use without changing its sensing characteristics. An illustration of the hysteresis-caused inductance variation of an RIP sensor “belt” that was stretched and released three times can be found in “A Wearable Respiration Monitoring System Based on Digital Respiratory Inductive Plethysmography,” by Dan Wu, et al., *Bulletin of Advanced Technology Research*, Vol. 3, No. 9, September 2009. After an undesir-

ably low amount of repeated use, not only do existing RIP sensors suffer from hysteretic effects (e.g., inelastically deformed, or “stretched out of shape”), but they can also become inoperable.

[0035] Embodiments of biosensing garment physiological sensors described herein provide several advantages over known biosensing garment sensors, such as: improved measurement-to-measurement signal consistency (i.e., high reproducibility), a more robust and prolonged sensor sensitivity (i.e., high reliability), ease and comfort of biosensing garment use, manufacturing efficiency, and reduced wear-related hysteresis.

[0036] FIG. 1 shows a schematic illustration of a physiological sensor 110 including an elongate member 120 and a conductive wire 140. The elongate member 120 is in contact with a conductive wire 140. The physiological sensor 110 can comprise an electronic textile, for example such that may be used in the manufacture of a biosensing garment. In some embodiments, the physiological sensor 110 comprises a biosensing garment (e.g., one or more of shirts, jerseys, vests, jackets, pants, shorts, bras, sports bras, bra camis, brassieres, swimsuits, hats, helmets, goggles, socks, shoes, footwear, headsets, watches, bracelets, underwear, athletic supporters, gloves, collars, neckbands, headbands, visors, scarves, mittens, arm sleeves, arm bands, leg sleeves, leg bands, head bands, waist bands, chest plates, tights, watches, undergarments, diapers, hospital gowns, bandages, smocks, girdles, blankets, and/or the like). The biosensing garment may comprise one or more textiles (e.g., cloths, fabrics etc.), for example consisting of a network of natural or artificial fibers. The textiles may derive from one or more sources, including plant sources (e.g., cotton, flax, hemp, jute, modal, bamboo, piña, ramie, milkweed stalk, lyocell, etc.), animal sources (e.g., wool, silk, milk proteins, etc.), mineral sources (e.g., glass fibers, etc.), and/or synthetic sources (e.g., nylon, polyester, polyamides, acrylic, aramid fibre, spandex, polyurethane, olefin fiber, ingeo, polylactide, lurex, carbon fibre, etc.). Strands from which the textiles are composed may include coatings such as waxes. Such textiles may be formed from one or more processes, including (but not limited to): weaving, knitting, crocheting, forming from tow, braiding, felting, thermal and/or mechanical bonding, and/or the like. As described herein, a textile formed by knitting is formed using any suitable knitting pattern or structure, for example, warp, weft, course/wale, knit-and-purl, plaited stitches, flat, circular, single, double, jersey, interlocked, mock rib, ribbed, two-way stretch, or any other suitable knitting pattern or combination thereof.

[0037] The elongate member 120 has a longitudinal axis and is stretchable along the longitudinal axis. The elongate member 120 includes a plurality of elastic members that can be arranged substantially in parallel with one another. In some embodiments, the elongate member 120 includes 2 elastic members. In some embodiments, the elongate member 120 includes 3 elastic members. In some embodiments, the elongate member 120 includes 3 elastic members. In some embodiments, the elongate member 120 includes up to 10 elastic members. In some embodiments, the elongate member 120 has a “width” (i.e., in a direction perpendicular to the longitudinal axis) of about 6 mm, or about 8 mm, or between about 6 mm and about 8 mm. At least one of the elastic members is knitted (using any suitable knitting method or structure as disclosed herein, for example: warp,

weft, modified weft, weaving, course/wale, knit-and-purl, plaited stitches, flat, circular, single, double, jersey, interlocked, mock rib, ribbed, two-way stretch, or any other suitable knitting pattern or combination thereof) from a single yarn. The single yarn includes at least one elastic filament (e.g., elastane) and at least one non-elastic multifilament (e.g., nylon). In some embodiments, the elastic filament comprises one or more fibers, such as (but not limited to): nylon, modacrylic, olefin, polyolefins, acrylic, polyester, carbon fiber, rayon, vinyon, saran, spandex, vinalon, aramids (e.g., Nomax, Kevlar, or Twaron), modal, dyneema/spectra, polybenzimidazole fiber, sulfar, lyocell, polylactic acid (PLA), orlon, zylon, vectran, derclon, acrylonitrile rubber, glass fiber, metallic fiber, and polyhydroquinone-diimidazopyridine (“M5 fiber”), bamboo fiber, diacetate fiber, triacetate fiber, silicon carbide fibers, polymer fibers, polyamide nylon, polyethylene terephthalate (“PET”) polyester or polybutylene terephthalate (“PBT”) polyester, phenol-formaldehyde, elastane, elastolefin, and/or the like. In some embodiments, the non-elastic multifilament is texturized, for example to improve its stretchability. In some embodiments, the non-elastic multifilament comprises one or more fibers, such as (but not limited to): nylon, modacrylic, olefin, polyolefins, acrylic, polyester, carbon fiber, rayon, vinyon, saran, vinalon, aramids (e.g., Nomex, Kevlar, or Twaron), modal, dyneema/spectra, polybenzimidazole fiber, sulfar, lyocell, polylactic acid (PLA), orlon, zylon, vectran, derclon, acrylonitrile rubber, glass fiber, metallic fiber, and polyhydroquinone-diimidazopyridine (“M5 fiber”), bamboo fiber, diacetate fiber, triacetate fiber, silicon carbide fibers, polymer fibers, polyamide nylon, PET or PBT polyester, phenol-formaldehyde, and/or the like. In some embodiments, the yarn (or “thread”) used in the knitting is a twisted yarn including 2 “strands” of multifilament nylon yarn and 1 filament of elastane that are twisted together. The composition of the yarn can be about 65% nylon and about 35% elastane. In some embodiments, each elastic member comprises a single yarn, and the single yarn comprises multiple filaments in a series of knitted loops. In some embodiments, the yarn comprises one or more texturized filaments, such as “curled” nylon.

[0038] In some embodiments, the yarn used to form one or more elastic members of the elongate member 120 comprises both elastane and a non-elastic or “conventional” fiber. In such embodiments, the combined elongate member and conductive wire exhibit certain desirable properties (for example due to the high “stretchability” of the yarn) that would not be observed if the same materials were used in isolation. For example, pure elastane fibers are relatively weak. When stretched into a tensile state, elastane fibers slowly begin to degrade, and they are easy to break once stretched beyond a maximum length. However, when combined with one or more non-elastic fibers, as described herein, the elastane is advantageously prevented from stretching to its maximum capacity (i.e., to the point of mechanical failure), and the structural integrity of the collective yarn is thus enhanced. Furthermore, the addition of elastane to the one or more non-elastic fibers enhances the mechanical stretchability of the collective yarn beyond what it would be if only non-elastic fibers were used.

[0039] The conductive wire 140 is any suitable electrical conductor (e.g., copper, aluminum, silver, tin, and/or alloys thereof, and/or any other conductive material, such as a metal, a metalloid, conductive paints or nanoparticle disper-

sions, a conductive polymer, a conductive ceramic material, etc.). For example, in some embodiments, the conductive wire **140** is 32 AWG silver plated copper wire (SPC), e.g., including 7 strands, that is insulated (e.g., with PVC, silicone, fluoropolymer resins such as PTFE, etc.). In some embodiments, the conductive wire **140** is a tinsel wire (silver plated copper alloy twisted around a textile yarn), a metal plated textile yarn that is insulated (e.g., with PTFE, silicone, etc.), or a “bare” metal plated textile yarn (i.e., that is not insulated). In some embodiments, using a bare metal plated textile yarn results in an improved signal strength and/or quality (e.g., in terms of amplitude, depth, noise). The conductive wire **140** can include multiple conductor “strands.” For example, in some embodiments the conductive wire **140** includes 7 filaments. In some embodiments, the conductive wire **140** is coated with an electrically insulating layer (e.g., a plastics or rubberized material). In other words, the conductive wire **140** may be an insulated wire.” For example, the conductive wire **140** may be a plastic-coated, silver-plated copper wire. In some embodiments, the conductive wire **140** is extensible or can be elastically deformed (e.g., by virtue of its physical configuration and/or the materials from which it is made).

[0040] The conductive wire **140** is in physical contact (i.e., “engaged”) with each of the plurality of elastic members of the elongate member **120**. In some embodiments, the conductive wire **140** is disposed on (e.g., atop, beneath, or adjacent to) one or more of the elastic members. In some embodiments, the conductive wire **140** is affixed to, knitted into (e.g., by weft knitting), woven into, interleaved with, enmeshed with, stitched to, looped through, braided with, or otherwise entangled with one or more of the elastic members. In some embodiments, the conductive wire **140** is affixed to, knitted into (e.g., by weft knitting), woven into, interleaved with, enmeshed with, stitched to, looped through, braided with, or otherwise entangled with one or more of the filaments of one of the elastic members. In some embodiments, the conductive wire **140** is affixed to, knitted into (e.g., by weft knitting), woven into, interleaved with, enmeshed with, stitched to, looped through, braided with, or otherwise entangled with one or more of the filaments of multiple elastic members. In some embodiments, the conductive wire **140**, by way of its engagement with the elastic members, provides support to the elastic members (and, hence, to the elongate member **120**). For example, the presence and positioning (e.g., attachment or coupling) of the conductive wire **140** with respect to the elastic members can help to set and/or maintain the spacing between two or more of the elastic members while also holding them together. In still further embodiments, the attachment between the conductive wire **140** and one or more elastic members (or portions thereof) can involve heat bonding with a fusible (hot melt) material (e.g., by a heat press or ironing). In such embodiments, one or more of the elastic members will have been knitted with fusible hot melt material, for example such that when multiple elastic members are assembled together (e.g., forming a “band” of elastic members), the fusible material is present on one side of the band of elastic members.

[0041] In some embodiments, a method of forming at least one of the plurality of elastic members of the elongate member **120** includes knitting individual yarns (for example, at multiple needles operating substantially “in parallel” or “serially” in time and/or physically “in parallel” or “seri-

ally”) by producing a continuous series of loops. Separately or in parallel, the conductive wire **140** is “fed” through the elongate member **120**, for example by passing the conductive wire **140** through at least one loop of at least one of the plurality of elastic members (i.e., that has been formed as herein described) such that it forms a predetermined pattern. By changing the wire “feed” per unit length (i.e., the length of conductive wire **140** per unit length of the elastic member and/or of the elongate member **120**), different pattern shapes (e.g., periodicity, amplitude, and/or frequency) can be obtained. A “100% wire feed” is defined as the amount of conductive wire **140** per unit length (e.g., of the elongate member **120**) that results in a straight wire profile (no oscillations). As such, exemplary wire feeds (or “feed rates”) of the disclosure are 200% (i.e., 2 times the length of wire required for a straight run for a given reference length, such that a meandering or sinusoidal pattern is established), 250% (i.e., 2.5 times the length of wire required for a straight run for a given reference length, such that a meandering or sinusoidal pattern is established) and 400% (i.e., 4 times the length of wire required for a straight run for a given reference length, such that a meandering or sinusoidal pattern is established). In some embodiments, using a higher feed rate or a higher frequency pattern (e.g., an increased number of sinusoidal oscillations per unit length, or a “higher periodicity”) results in an improved signal strength and/or quality. In some embodiments, the “feed rate” (and, correspondingly, the frequency/amplitude of the resulting pattern) of the conductive wire **140** is selected such that when the stretchable physiological sensor **110** is elongated to its maximum, the conductive wire **140** still maintains a sinusoidal shape (i.e., the conductive wire **140** is not pulled straight). For values of the feed rate that are below the threshold value at which the conductive wire **140** is not flattened upon full elongation of the physiological sensor **110**, increases in feed rate can have a significant effect on the robustness of the physiological sensor **110**. In some embodiments, the conductive wire **140** is combined with the elastic members such that it has a curved (e.g., sinusoidal) pattern. In some embodiments, instead of a curved pattern, the conductive wire **140** is combined with the elastic members such that it has a sawtooth, square, or triangle shape along at least a portion of its length. In some embodiments, the elongate member **120** includes a single conductive wire **140** having a substantially constant pattern (i.e., shape and/or periodicity). In some embodiments, the elongate member **120** includes a single conductive wire **140** having a pattern (i.e., shape and/or periodicity) that varies along the longitudinal axis of the elongate member **120**. Patterns of the conductive wires **140** described herein may be periodic, aperiodic, symmetric, and/or asymmetric along portions of or the entireties of their length(s). In some embodiments, the patterns of the conductive wires **140** described herein may be present along only portions of the elongate member **120**, with the rest of the elongate member **120** (and/or the conductive wire **140** embedded therewithin) being substantially “straight.”

[0042] In some embodiments, a method of forming at least one of the plurality of elastic members of the elongate member **120** includes knitting individual yarns (for example, at multiple needles operating substantially “in parallel” or “serially” in time and/or physically “in parallel” or “seri-

continuous series of loops, are then knitted together to form the elongate member 120 (essentially, at this stage, an elongate knitted fabric). Separately or in parallel, the conductive wire 140 is “fed” through the elongate member 120, for example by passing the conductive wire 140 through at least one loop of at least one of the plurality of elongate members (i.e., that has been formed as herein described) such that it forms a predetermined pattern. For example, the conductive wire 140 may pass beneath one or more elastic member segments, then pass above one or more elastic member segments (e.g., portions of the interlocked loops or stitches of the knitting), continuing in an “over” and “under” manner in order to ensure a good integration of the conductive wire 140 into the elongate member 120. By changing the wire “feed” per unit length (i.e., the length of conductive wire 140 per unit length of the elastic member and/or of the elongate member 120), different pattern shapes (e.g., periodicity, amplitude, and/or frequency) can be obtained.

[0043] In some embodiments, multiple conductive wires 140 are coupled to the elongate member 120, the conductive wires 140 having substantially similar patterns (in terms of shape and/or periodicity). In some embodiments, multiple conductive wires 140 are coupled to the elongate member 120, each of said conductive wires 140 having a pattern (in terms of shape and/or periodicity) different from at least one of the other conductive wires. Where multiple conductive wires 140 are used, their patterns may be superimposed (e.g., one atop the other), or may be spatially arranged such that they run substantially parallel to one another along the longitudinal axis of the elongate member 120. In some embodiments, where multiple conductive wires 140 are used, those conductive wires 140 whose patterns are substantially similar may be arranged such that they are schematically “in phase” with one another (i.e., their peaks and valleys are aligned). In some embodiments, where multiple conductive wires 140 are used, conductive wires 140 whose patterns are substantially similar may be arranged such that they are schematically “out of phase” from one another (i.e., their peaks and valleys do not align, but rather are shifted along an axis with respect to one another). In some embodiments, using multiple conductive wires 140 results in an improved signal strength and/or quality (e.g., in terms of amplitude, depth, noise, and/or the like).

[0044] The elongate member 120 is disposed within and/or on a surface of the physiological sensor 110. For example, one or more portions of the elongate member 120 may be sewn, knitted (e.g., circular, “knitting in the round,” single, double, jersey, interlocked, mock rib, ribbed, two-way stretch, or any other suitable knitting pattern or combination thereof), crocheted, felted, stitched, woven, or otherwise embedded into the physiological sensor. Instead or in addition, one or more portions of the elongate member 120 may be also glued, adhered, fastened, clipped, snapped, soldered, bonded, fused, or otherwise secured to a surface of the physiological sensor 110. The elongate member 120 can be positioned on or within the physiological sensor 110 in a number of configurations, as described in greater detail below. For example, the elongate member 120 can be disposed as a single, planar layer on a surface of the physiological sensor 110. In other embodiments, the elongate member 120 can follow a U-shaped path along a surface of the physiological sensor 110. In still other embodiments, the elongate member 120 can be disposed as a double layer that is folded back on itself (i.e., such that a single elongate

member forms a two-ply layer along substantially the entirety of its length), on a surface of the physiological sensor 110. In some embodiments, the physiological sensor 110 is a biosensing garment, and the elongate member 120 (bearing the conductive wire 140) is attached to the shirt using one or more of the methods described herein. A portion of the insulating layer can be removed from both ends of the conductive wire 140, thereby exposing the bare conductor at each end. The exposed conductor can then be attached to a “connector” (e.g., a mechanical fastener that also provides for electrical connection), for example by placing it under a snap and laminating it in place to reinforce it. For embodiments in which the physiological sensor 110 comprises multiple conductive wires 140, portions of the insulating layer can be removed from both ends of each of the multiple conductive wires 140 and attached to a common connector. In such embodiments, the electrical resistance of the physiological sensor 110 is proportionally reduced (e.g., approximately halved, in the case of two wires), thereby improving the signal quality and reducing power consumption. In some embodiments, the elongate member 120 is formed integrally or “monolithically” with the physiological sensor 110. The physiological sensor 110 may include one or more electrical leads connectable with a unit for receiving data from the physiological sensor 110 and for storing the data in a computer-readable medium. The unit may be configured to communicate (e.g., wirelessly) with a central data repository for receiving, storing and processing data generated by the physiological sensor 110, and for making stored data available to the user and/or to others (e.g., a health care provider).

[0045] FIG. 2A shows a front schematic plan view, and FIG. 2B shows a back schematic plan view, of a biosensing garment 200 incorporating a physiological sensor 210 as described herein. Although the biosensing garment 200 in FIGS. 2A and 2B is shown as a biosensing shirt, embodiments of biosensing garments as described herein can be any type of garment (e.g., one or more of shirts, jerseys, vests, jackets, pants, shorts, bras, sports bras, bra camis, brassieres, swimsuits, hats, helmets, goggles, socks, shoes, footwear, headsets, watches, bracelets, underwear, athletic supporters, gloves, collars, neckbands, headbands, visors, scarves, mittens, arm sleeves, arm bands, leg sleeves, leg bands, head bands, waist bands, chest plates, tights, watches, undergarments, diapers, hospital gowns, bandages, smocks, girdles, blankets, and/or the like).

[0046] In some embodiments, the physiological sensor 210 includes an elongate member 220 and a conductive wire 240 having a substantially sinusoidal pattern coupled to the elongate member 220 to form at least part of the respiration monitoring sensor 210 (e.g., a “respiratory inductance plethysmography” or “RIP” sensor). In some embodiments, the physiological sensor 210 is disposed on an interior surface of the biosensing garment 200. The elongate member 220 is configured to be disposed around an at least partial circumferential region of a user. The at least partial circumferential region of the user can include at least a portion of the user’s chest, rib cage and/or abdomen. The elongate member 220, when disposed about the circumference of a user as shown in FIGS. 2A and 2B, is configured to be held closely to the user’s body. The conductive wire 240 has an intrinsic inductance value (“self-inductance”) related to its sinusoidal shape or “pattern” (for example, related to a frequency, amplitude and/or periodicity thereof). The induc-

tance value of the conductive wire **240** changes substantially in response to changes in the geometry (e.g., antero-posterior diameter, circumference, cross-sectional area, etc.) of the user's anatomy, for example as a result of the user's respiratory movements (breathing, inhalation, inspiration, exhalation, coughing, yawning, and/or the like) or other movements (exertion, muscle flexion, coughing, yawning, stretching, posture, and/or the like). The user's respiratory movements involve changes in the user's lung volume, compartmental torso volume, ventilation, inspired breath volume, etc. As a result, a user's lung volume, respiratory rate (e.g., breaths per minute), tidal volume, ventilation (e.g., minute ventilation), peak inspiratory flow, fractional inspiratory time, work of breathing, peak/mean inspiratory and expiratory flow, % RCI (percent contribution of rib cage excursions to the tidal volume), phase angle ("phi"), apnea status and/or classification, hypopnea status and/or classification, qDEEL (quantitative difference of end expiratory lung volume) and/or inspired breath volume, along with other parameters like breathing patterns, can be measured through transduction or "sensing" of the changing inductance (including the timing of such changes) of the conductive wire. In order to continuously measure the user's respiration, the conductive wire can be used as the inductor in a variable frequency LC oscillator (i.e., the conductive wire is connected to an LC circuit, in which the conductive wire acts as the inductor "L"). The LC oscillator can in turn be connected to a frequency-to-voltage converter, which can be connected to a scaling amplifier, which can be connected to a digital voltmeter or other suitable display. In some embodiments, the physiological sensor **210** is incorporated into the biosensing garment **200** during the manufacturing of the biosensing garment **200**. In some embodiments, the elongate members **220** and the conductive wire **240** are knitted on sequential tubular textile sections that are connected to further tubular textile sections, followed by folding over and stitching together the necessary components in order to assemble the biosensing garment **200**. In still further embodiments, the elongate members **220** and the conductive wire **240** are knitted into a tubular "band" independent of the manufacturing of the biosensing garment **200**. In such embodiments, the tubular band is printed and/or laminated with insulation while not yet incorporated into the biosensing garment **200**, and then the tubular band is integrated into a completed biosensing garment **200** through stitching and/or bonding.

[0047] FIG. 3 is a schematic illustration of an elongate member **320** for incorporation into and/or use as a physiological sensor **310**, according to an embodiment. A conductive wire **340** having a continuous substantially sinusoidal pattern is coupled to the elongate member **320**. The elongate member **320** can be of any length suitable for a physiological sensing application (e.g., of sufficient length to cover the at least partial circumferential region of a user discussed above). The pattern of the conductive wire **340** may be said to have a periodicity of about 7 over a distance "D."

[0048] FIG. 4 is a schematic illustration of an elongate member **420** for incorporation into and/or use as a physiological sensor **410**, according to an embodiment. A conductive wire **440** having a continuous substantially sinusoidal pattern is coupled to the elongate member **420**. The elongate member **420** can be of any length suitable for a physiological sensing application (e.g., of sufficient length

to cover the at least partial circumferential region of a user discussed above). The pattern of the conductive wire **440** may be said to have a periodicity of about 14 over distance D.

[0049] FIG. 5 is a schematic illustration of an elongate member **520** for incorporation into and/or use as a physiological sensor **510**, according to an embodiment. A conductive wire **540** having a continuous substantially sinusoidal pattern is coupled to the elongate member **520**. The elongate member **520** can be of any length suitable for a physiological sensing application (e.g., of sufficient length to cover the at least partial circumferential region of a user discussed above). The pattern of the conductive wire **540** may be said to have a periodicity of about 4.5 over distance D.

[0050] FIG. 6 is a schematic illustration of an elongate member **620** for incorporation into and/or use as a physiological sensor **610**, according to an embodiment. A conductive wire **640** having a continuous, asymmetric pattern of varying periodicity is coupled to the elongate member **620**. The elongate member **620** can be of any length suitable for a physiological sensing application (e.g., of sufficient length to cover the at least partial circumferential region of a user discussed above). The pattern of the conductive wire **640** may be said to include regions having a periodicity of about 1, and regions having a periodicity of about 4. Said regions having a periodicity of about 1, and regions having a periodicity of about 4 may be said to "alternate" along a longitudinal axis of the elongate member **620**. A single region having a periodicity of about 1 and a single region having a periodicity of about 4, when viewed together, may be said to collectively comprise a "composite pattern," said composite pattern having a periodicity of 2 over distance D.

[0051] FIGS. 7A-7C show schematic illustrations of elongate member/conductive wire combinations (also referred to herein as "constructions," or "tape") for incorporation into and/or use as a physiological sensor **710**, including an elongate member **720** and a plurality of conductive wires **740**, according to embodiments of the disclosure. FIGS. 7A and 7B depict elongate member/conductive wire combinations (having two and seven periodic conducting wires, respectively) that have been knitted with a fusing thread and are loosely connected to one side of the tape. FIG. 7C shows an elongate member/conductive wire combination, having two periodic conductive wires that are substantially out-of-phase with one another and partially overlapping, that has been found to show superior signal detection and accuracy.

[0052] FIG. 8A shows a first elongate member (or "tape") **820A**, and FIG. 8B shows a second elongate member (or "tape") **820B**, both in a "relaxed" (i.e., not stretched) configuration, according to embodiments of the disclosure. Elongate members **820A** and **820B** have wire feeds of about 200% and about 400%, respectively. The frequency of the first elongate member **820A** is about half the frequency of the second elongate member **820B**. In other words, the period of the first elongate member **820A** is about double the period of the second elongate member **820B**. The second elongate member **820B** may be said to comprise a "denser" sinusoid than the first elongate member **820A**. In some embodiments, the elongate members **820A** and **820B** are approximately 8 mm wide.

[0053] FIG. 9 is a schematic illustration of an elongate member **920**, for incorporation into and/or use as a physiological sensor **910**, according to an embodiment. A first

conductive wire **940**, having a continuous substantially sinusoidal pattern, is coupled to the elongate member **920**. The pattern of the conductive wire **940** may be said to have a periodicity of about 14 over distance *D*. A second conductive wire **960**, having a continuous substantially sinusoidal pattern, is also coupled to the elongate member **920**. The pattern of the conductive wire **960** may be said to have a periodicity of about 4.5 over distance *D*. As such, the frequency of the first conductive wire **940** has about three times the frequency of the second conductive wire **960**. In other words, the period of the first conductive wire **940** is about one-third the period of the second conductive wire **960**.

[0054] FIG. 10 shows three example (open loop) configurations of elongate members with conductive wires coupled thereto, according to some embodiments: (A) a substantially square or “u-shaped” configuration **1020A**; (B) a substantially rectangular-shaped configuration **1020B**; and (C) a substantially circular shape/configuration **1020C**. In some embodiments, the configurations of elongate members include at least one of a substantially oval shape, and any other shape, including an irregularly shape.

[0055] FIGS. 11-16 are schematic illustrations showing configurations of elongate members with conductive wires coupled thereto, according to some embodiments. FIG. 11 shows a front view of a biosensing garment, according to an embodiment, with two example configurations of an elongate member (shape “**1120A**” and shape “**1120B**”). FIG. 12 shows a side view of a biosensing garment, according to an embodiment, with two example configurations of an elongate member (shape “**1220A**” and shape “**1220B**”). FIG. 13 shows a side view of a biosensing garment, according to an embodiment, with an example configuration of an elongate member **1320** that is disposed around a perimeter of an armhole of the biosensing garment.

[0056] FIG. 14 is a schematic illustration showing a folded configuration of a partially-constructed elongate member **1420**, for incorporation into and/or use as a physiological sensor **1410**, according to some embodiments. As shown in FIG. 14, a single conductive wire, having a continuous, substantially sinusoidal pattern, is coupled to the elongate member **1420**, and is folded back over onto itself, thereby forming two sections (**1440A** and **1440B**) that overlay one another. The pattern of the conductive wire section **1440A** (i.e., a top layer of the folded configuration, disposed along a first “pass” of the elongate member **1420**, moving from right to left) may be said to have a periodicity of about 13.5 or 14 over distance *D*. The elongate member **1420** and conductive wire are folded at the left edge of FIG. 14, such that the elongate member continues, extending from left to right behind or beneath the top layer of the folded configuration (thereby forming a bottom layer of the folded configuration). This second “pass” of the elongate member **1420**, moving from left to right, includes the conductive wire section **1440B** (shown in bold, where **1440B** is electrically and/or physically continuous with conductive wire section **1440A**, i.e., conductive wire section **1440A** and conductive wire section **1440B** are part of the same conductive wire) coupled thereto, and the conductive wire section **1440B** also has a continuous substantially sinusoidal pattern. The pattern of the conductive wire section **1440B** may also be said to have a periodicity of about 13.5 or 14 over distance *D*. As such, the frequency and period of the entire conductive wire (including **1440A** and **1440B**) is

substantially constant. However, as can be seen in FIG. 14, conductive wire sections **1440A** and **1440B** are out-of-phase with one another (i.e., $\sim 180^\circ$ out-of-phase). Depending upon where the fold is made in the elongate member **1420** and conductive wire, the conductive wire sections **1440A** and **1440B** may be in-phase with one another, substantially in-phase with one another, or out-of-phase with one another (e.g., by 45° , 90° , 180° , etc.). To complete the construction of the elongate member **1420** shown in FIG. 14, the conductive wire section **1440B** would continue rightward, traversing the path shown by a dashed line. Such folded configurations can provide a smaller physical footprint of the elongate member, for example so that it is more readily incorporated into a physiological sensor, and/or so that closure mechanisms such as zippers and snaps in a biosensing garment can be actuated in the presence of the elongate member without said closure mechanisms interfering with or interrupting the continuity (e.g., including the electrical conductivity) of the conductive wire coupled to the elongate member, as described in further detail below.

[0057] FIG. 15A shows a front view of a biosensing garment, according to an embodiment, having a vertically disposed zipper closure substantially centered on the front of the garment, and including a perspective view of an example configuration of an elongate member **1520A** extending in an elongated loop shape around a portion of a circumference of the biosensing garment. As shown in FIG. 15A, an elongate member **1520A** originates from a first connector **1519A** on the front of the biosensing garment, extends in a first direction (to the left in FIG. 15A), and bends, in the plane of the garment, in a substantially “U” shape such that the elongate member **1520A** continues in a second direction opposite the first direction (to the right in FIG. 15A). The elongate member **1520A** continues circumferentially around the back of the biosensing garment (right to left in FIG. 15A) and onto the front of the biosensing garment, bending once again, in the plane of the biosensing garment, in a substantially “U” shape prior to reaching the zipper closure, again reversing its direction of travel (to the left in FIG. 15A). The elongate member **1520A** continues circumferentially around the back of the biosensing garment (left to right in FIG. 15A) and onto the front of the biosensing garment where it terminates at a second connector **1521A**. As such, the elongate member **1520A** forms a complete loop, and traverses a substantial percentage of the circumference of the biosensing garment, without crossing the zipper closure. In the configuration of FIG. 15A, the elongate member **1520A** may be said to have a planar, elongated loop shape, in which two sections of the elongate member **1520A** are disposed parallel to one another (e.g., everywhere except at the bends and between connectors A and B) along a majority of the biosensing garment’s circumference.

[0058] FIG. 15B shows a front view of a biosensing garment, according to an embodiment, having a vertically disposed zipper closure substantially centered on the front of the garment, and including an example configuration of an elongate member **1520B** extending in a folded configuration around a portion of a circumference of the biosensing garment. As shown in FIG. 15B, an elongate member **1520B** originates from a first connector **1519B** on the front of the biosensing garment, extends in a first direction (to the left in FIG. 15B), and is folded back onto itself such that the elongate member **1520B** continues in a second direction opposite the first direction (to the right in FIG. 15B). In other

words, the elongate member **1520B** includes a first portion extending from the first connector **1519B** in the first direction, and a second portion extending in the second direction from the first portion to the second connector **1521B**. The elongate member **1520B** continues circumferentially around the back of the biosensing garment (right to left in FIG. **15B**) and onto the front of the biosensing garment, folded back onto itself once again prior to reaching the zipper closure, again reversing its direction of travel (to the left in FIG. **15B**). The elongate member **1520B** continues circumferentially around the back of the biosensing garment (left to right in FIG. **15B**) and onto the front of the biosensing garment where it terminates at the second connector **1521B**. As such, the elongate member **1520B** forms a complete loop, and traverses a substantial percentage of the circumference of the biosensing garment, without crossing the zipper closure. In the configuration of FIG. **15B**, the elongate member **1520B** may be said to have a folded, bilayer, or “overlay” configuration (e.g., everywhere except between connectors **1519B** and **1521B**), in which two sections of the elongate member **1520B** are disposed parallel to and atop one another along a majority of the biosensing garment’s circumference.

[0059] In some embodiments, the first portion of the elongate member **1520B** has a length approximately the circumference of the biosensing garment. In some embodiments, the first portion of the elongate member **1520B** has a length less than the full circumference of the biosensing garment. In some embodiments, the first portion of the elongate member **1520B** is less than about 99%, less than about 95%, less than about 90%, less than about 85%, less than about 80%, less than about 75%, less than about 70%, less than about 65%, less than about 60%, less than about 55%, less than about 50%, less than about 45%, less than about 40%, less than about 35%, less than about 30%, less than about 25%, less than about 20%, less than about 15%, less than about 10%, or less than about 5% of the circumference of the biosensing garment.

[0060] In some embodiments, a vertically disposed zipper closure is disposed on the back of the garment instead of, or in addition to, the front of the garment. In some embodiments, a zipper closure is included in the garment in an orientation other than vertical (e.g., horizontal, diagonal, etc.), and/or may extend only partway across the garment along its direction of travel.

[0061] FIG. **16** shows a front view of a biosensing garment (e.g., a biosensing bra) having a loop-shaped elongate member **1620** disposed in a lower band (e.g., wholly disposed within a “front” portion of the lower band of the biosensing bra), and having a hook (e.g., “hook-and-eye”) opening in the back (e.g., instead of a zip opening in the front).

[0062] In some embodiments, an apparatus, such as a biosensing garment, can include an elongate member **1620** defining a longitudinal axis and configured to be stretchable along the longitudinal axis. In some embodiments, the elongate member **1620** includes a plurality of substantially parallel elastic members. In some embodiments, a conductive member comprising an electrical conductor can be fixedly coupled to at least one of the plurality of substantially parallel elastic members. In some embodiments, the conductive member can be disposed in a regular pattern along the longitudinal axis of the elongate member **1620** and configured to move between a first configuration and a second configuration.

[0063] In some embodiments, an apparatus, such as a biosensing garment, can include a plurality of substantially parallel elastic members disposed along an axis and configured to be stretchable along the axis. In some embodiments, a conductive member is disposed in a regular pattern and fixedly coupled to at least one of the plurality of substantially parallel elastic members. In some embodiments, the conductive member is configured to move between a first configuration and a second configuration.

[0064] In some embodiments, the conductive member has a first inductance value in the first configuration, and a second inductance value in the second configuration. In some embodiments, the regular pattern of the conductive member is a curved pattern. In some embodiments, the curved pattern of the conductive member is substantially sinusoidal.

[0065] In some embodiments, a biosensing garment can include a first connector coupled to a first end of the elongate member and a second connector coupled to a second end of the elongate member, and the first connector is disposed proximate the second connector to form an open loop. In some embodiments, the open loop is disposed in at least one of a substantially circular shape, a substantially oval shape, a substantially square shape, a substantially rectangular shape, and an irregularly shape.

[0066] In some embodiments, the elongate member **1620** includes a first portion **1622A** and a second portion **1622B**. In some embodiments, a first connector **1619** is coupled to a first end or a first portion of the elongate member, and a second connector **1621** is coupled to a second end or a second portion of the elongate member. The first connector **1619** and/or first portion **1622A** can be disposed proximate the second connector **1621** and/or second portion **1622B** thereby forming an open loop. In some embodiments, the first portion **1622A** can extend from the first connector **1619** in a first direction, and the second portion **1622B** can extend in a second direction from the first portion **1622A** to a second connector **1621**. In some embodiments, the second direction is opposite the first direction. Although the first portion **1622A** and second portion **1622B** are shown “separated” from each other in FIG. **16**, the first portion **1622A** and second portion **1622B** can at least partially overlap each other. In other words, in some embodiments, the second portion **1622B** can be folded back onto the first portion **1622A**. In some embodiments, the first portion **1622A** is disposed substantially parallel to the second portion **1622B**. In some embodiments, the first portion **1622A** is disposed non-zero distance from the second portion **1622B**. In some embodiments, the first portion **1622A** and the second portion **1622B** are disposed substantially overlapped, similar to the illustration as shown in FIG. **15B**.

[0067] In some embodiments, at least one of the first portion **1622A** and the second portion **1622B** of the elongate member **1620** has a length approximately the circumference of the biosensing garment. In some embodiments, at least one of the first portion **1622A** and the second portion **1622B** of the elongate member **1620** has a length less than the full circumference of the biosensing garment. In some embodiments, at least one of the first portion **1622A** and the second portion **1622B** of the elongate member **1620** is less than about 99%, less than about 95%, less than about 90%, less than about 85%, less than about 80%, less than about 75%, less than about 70%, less than about 65%, less than about 60%, less than about 55%, less than about 50%, less than

about 45%, less than about 40%, less than about 35%, less than about 30%, less than about 25%, less than about 20%, less than about 15%, less than about 10%, or less than about 5% of the circumference of the biosensing garment.

[0068] FIGS. 17A-17B are schematic illustrations showing cross-sectional views of a folded configuration of an elongate member bearing a conductive wire (e.g., a RIP sensor), according to some embodiments. As shown in FIGS. 17A and 17B, an elongate member 1720 (a detail view of which is shown at sections “C”) is disposed adjacent to a first surface of a fabric or elastic substrate (e.g., a biosensing garment or portion thereof) and passes through two slits in said fabric or elastic substrate such that at least a portion of the elongate member 1720 is disposed on a second surface of the fabric or elastic substrate, and such that the elongate member 1720 folds back on itself. Described sequentially, the elongate member 1720 is connected to connector “A,” then: (1) extends in a first direction substantially parallel to a first surface of the fabric or elastic substrate; (2) passes through a first slit in the fabric or elastic substrate, forming a fold in the elongate member 1720; (3) extends in a second direction, opposite the first direction, adjacent and substantially parallel to a second surface of the fabric or elastic substrate; (3) passes through a second slit in the fabric; (4) extends in the second direction, adjacent and substantially parallel to the first surface of the fabric or elastic substrate; and (5) is connected to connector “B.” As shown in FIGS. 17A and 17B, the elongate member 1720 has a modified configuration as compared with the planar configurations of FIGS. 15 and 16. Instead of looping the elongate member around a specific shape (circle, rectangle etc.), where the loop forms a specific shape and surface area, the elongate member of FIGS. 17A and 17B is folded and relayed back along substantially the same axis (i.e., multilayered, or “overlaid”). In the configurations of FIGS. 17A and 17B, the spacing between the slits determines the proportion of the elongate member 1720 that is disposed on/adjacent to the first surface of the fabric or elastic substrate and the proportion of the elongate member that is disposed on/adjacent to the second surface of the fabric or elastic substrate. In some embodiments, the elongate member includes more than one fold (e.g., 2 or 3 folds).

[0069] FIGS. 18A-18B are schematic illustrations showing planar views of a folded configuration of an elongate member bearing a conductive wire incorporated into a garment (or portion thereof), the elongate member having overlaying sections, according to some embodiments. As shown in FIG. 18A, the elongate member 1820, including a conductive wire 1840, is folded and looped through slits “S1” and “S2” in an elastic band “E,” and relayed back along the same axis, such that first and second sections of the elongate member 1820 are substantially overlapping. As shown in FIGS. 18A and 18B, the elongate member can be supported by one or more fabric or thermoplastic portions 1811 and 1825, for example, that are stitched into, adhered to, or otherwise secured to the elastic band “E.” The length of the folded elongate member 1820 can be any appropriate length, e.g. 10 cm, 20 cm, 30 cm, or any other desired length, depending on the application. The overlapping sections of conductive wire 1840 (i.e., the portion of conductive wire 1840 that extends from left to right prior to folding and the portion of conductive wire 1840 that extends from right to left after folding) are shown in FIGS. 18A and 18B to be out-of-phase with one another (i.e., $\sim 180^\circ$ out-of-phase) by

a substantially constant amount across the entire length of the elongate member 1820. However, depending upon where the fold is made in the elongate member 1820 and conductive wire, the conductive wire sections may be in-phase with one another, substantially in-phase with one another, or out-of-phase with one another (e.g., by 45° , 90° , 180° , etc.).

[0070] FIGS. 18C-18D are schematic illustrations showing planar views of a further folded configuration of an elongate member bearing a conductive wire incorporated into a garment (or portion thereof), the elongate member having alternating sections, according to an embodiment. As shown in FIG. 18C, the elongate member 1820, including a conductive wire 1840 electrically connected to connector 1819, extends in a sinusoidal or periodic pattern (from left to right in FIG. 18C) and is folded back on itself (e.g., at the right edge of the elongate member 1810 in FIGS. 18C and 18D) such that it is relayed back along the same axis (from right to left in FIG. 18C), also in a sinusoidal or periodic pattern, and such that first and second sections of the elongate member 1820 (e.g., top and bottom sections) are only partially (e.g., periodically) overlapping. The conductive wire coupled to elongate member 1820 is electrically connected to connector 1821. As shown in FIGS. 18C and 18D, the elongate member 1820 can be supported by one or more fabric or thermoplastic portions 1811 and 1825, for example, that are stitched into, adhered to, or otherwise secured to an elastic band “E.” The length of the folded elongate member 1820 can be any appropriate length, e.g. 10 cm, 20 cm, 30 cm, or any other desired length, depending on the application. In some embodiments, both the elongate member 1820 and the conductive wire 1840 coupled thereto are “folded,” such that a single elongate member and a single conductive wire are disposed between connectors 1819 and 1821. In other embodiments, the elongate member 1820 comprises two separate segments (e.g., a top segment and a bottom segment) and a single conductive wire that is folded as it passes from the first elongate member segment into the second elongate member segment.

[0071] FIGS. 19A-19B are schematic illustrations showing planar views of a folded configuration of an elongate member bearing a conductive wire incorporated into a garment (or portion thereof), the elongate member having parallel sections, according to some embodiments. As shown in FIG. 19A, the elongate member 1920, including a conductive wire 1940, traverses a longitudinal path along an elastic band “E,” and is folded (e.g., by passing through slits in the elastic band “E”) and relayed back along a substantially parallel axis, such that first and second sections of the elongate member 1920 are substantially parallel and non-overlapping. As shown in FIGS. 19A and 19B, the elongate member 1920 can be supported by one or more fabric or thermoplastic portions 1911 and 1925, for example, that are stitched into, adhered to, or otherwise secured to the elastic band “E.” The length of the folded elongate member 1920 can be any appropriate length, e.g. 10 cm, 20 cm, 30 cm, or any other desired length, depending on the application.

[0072] FIGS. 19C-19D are schematic illustrations showing a looped wire configuration of an elongate member bearing a conductive wire incorporated into a garment (or portion thereof), according to an embodiment. In the configuration of FIGS. 19C-19D, instead of having a folded elongate member or having the elongate members looped around a specific shape, the conductive wire itself is inter-

weaved back and forth within the same assembly (e.g., a single elongate member **1920**). The length and height (amplitude) of the conductive wire can be determined based on the desired application. As shown in FIG. **19C**, a single elongate member **1920** includes a single conductive wire that originates at connector **1919**, traverses a length “L” of a longitudinal axis of an assembly (e.g., an elastic band, a segment of fabric, a garment or portion thereof, etc.) with a sinusoidal or periodic pattern, and is then woven, affixed, folded or otherwise made to traverse back along the length “L” of the longitudinal axis of the assembly for connection at connector **1921**. The period of the conductive wire of FIG. **19C** for each traversal of the length “L” repeats approximately 8.5 times.

[0073] In FIG. **19D**, a single elongate member **1920** includes five elastic members and a single conductive wire that originates at connector **1919**, traverses a length “L” of a first longitudinal axis of the elongate member **1920** (i.e., spanning the bottom three elastic members of the elongate member **1920**) with a sinusoidal or periodic pattern, and is then woven, affixed, folded or otherwise made to traverse back along the length “L” of a second longitudinal axis of the elongate member **1920** (i.e., spanning the top three elastic members of the elongate member **1920**) for connection at connector **1921**. The period of the conductive wire of FIG. **19D** for each traversal of the length “L” repeats approximately 8.25 times.

[0074] FIGS. **20A-20H** show components for use in an assembly process, according to an embodiment. Some or all of the materials described with reference to FIGS. **20A-20H** can be used for assembly steps of the present disclosure, for example such as those discussed below with reference to FIGS. **21A-21M**. FIG. **20A** depicts a breathing cable attachment **2011**, which may comprise thermoplastic polyurethane (“TPU”) or any other type of material that is suitable for lamination. The breathing cable attachment can be colored (e.g., black) or transparent. In some embodiments, the breathing cable attachment **2011** has a width of about 25 mm and a height of about 30 mm. As shown in FIG. **20A**, the breathing cable attachment **2011** has a fold line down its middle, e.g., along a longitudinally extending centerline thereof (see, e.g., the dashed line in FIG. **20A**).

[0075] FIG. **20B** depicts a middle part with double holes **2013**, which may comprise thermoplastic polyurethane (“TPU”) or any other type of material that is suitable for lamination. Each hole of the double holes **2013** can have a diameter of about 3 mm, or any other suitable diameter depending on the snap that is used. The middle part with double holes **2013** can be colored (e.g., black) or transparent. In some embodiments, the middle part with double holes **2013** has a width of about 60 mm and a height of about 20 mm.

[0076] FIG. **20C** depicts a middle part with single holes **2015**, which may comprise TPU or any other type of material that is suitable for lamination. Each of the single holes **2015** can have a diameter of about 3 mm, or any other suitable diameter depending on the snap that is used. The middle part with single holes **2015** can be colored (e.g., black) or transparent. In some embodiments, the middle part with single holes **2015** has a width of about 60 mm and a height of about 20 mm.

[0077] FIG. **20D** depicts a support bridge **2017**, which may comprise PET film, PA, PTFE, PE (HDPE, LDPE, MDPE, UHMWPE, ULMWPE), PP or other suitable plastic.

[0078] FIG. **20E** depicts a conductive tape ring **2019** which may comprise any conductive tape, such as silver tape, copper tape, aluminum tape, carbon conductive tape, single-sided or double-sided tapes, e.g., having XY or XYZ axis conductivity, conductive fiber or particle filled adhesives and/or the like. In some embodiments, the conductive tape ring **2019** has an outer diameter of about 14 mm or other suitable diameter depending upon the snap size being used. In some embodiments, the conductive tape ring **2019** has an inner hole diameter of about 3 mm or other suitable diameter depending upon the snap size being used. In some embodiments, the conductive tape ring **2019** is double-sided and/or comprises one or more “liner sheets” (for example, to protect one or more adhesive surfaces thereof).

[0079] FIG. **20F** depicts a PET film ring **2021** comprising PET. In some embodiments, the PET film ring **2021** has an outer diameter of about 14 mm or other suitable diameter depending upon the snap size being used. In some embodiments, the PET film ring **2021** has an inner hole diameter of about 3 mm or other suitable diameter depending upon the snap size being used.

[0080] FIG. **20G** depicts a garment TPU segment **2023**. The garment TPU segment **2023** can be transparent, or can be colored (e.g., black). In some embodiments, the garment TPU segment **2023** has a width of about 90 mm and a height of about 15 mm.

[0081] FIG. **20H** depicts a final cover **2025**, which may comprise thermoplastic polyurethane (“TPU”) or any other type of material that is suitable for lamination. The final cover **2025** can be colored (e.g., black) or transparent. In some embodiments, the final cover **2025** has a width of about 70 mm and a height of about 30 mm.

[0082] In some embodiments, the breathing cable attachment **2011**, the middle part with double holes **2013**, the middle part with single holes **2015**, the garment TPU segment **2023** and/or the final cover **2025**, and/or any other TPU segment (or “membrane”) used in assembling the biosensing garment(s) described herein, have one or more release layers (also referred to herein as “backing papers”) disposed thereon (e.g., on both sides), to protect adjacent surfaces during assembly steps involving the application of heat. Such paper layers can be removed at some point after lamination such that no paper remains in the final construction of the biosensing garment. In some embodiments, the breathing cable attachment **2011**, the middle part with double holes **2013**, the middle part with single holes **2015**, the garment TPU segment **2023** and/or the final cover **2025**, and/or any other TPU segment (or “membrane”) used in assembling the biosensing garment(s) described herein, is double-sided (i.e., can be laminated on both sides and/or includes a backing paper on one or both sides). In some embodiments, instead of or in addition to TPU, a different polyurethane plastic or other suitable strain relief material is used for one or more of the foregoing components. In some embodiments, using plastic and/or other laminating materials allows the connector regions to be flexible but not stretchable.

[0083] In some embodiments, an assembly process for a biosensing garment begins with measuring and cutting a breathing wire to a desired width. For example, if assembling a biosensing brassiere (“bra”), the width of a bra may be calculated as follows:

$$((\text{BRA WIDTH} * 2) + 2 \text{ cm}) + 5\%;$$

and if assembling a biosensing shirt, the width of a shirt may be calculated as follows:

$$((\text{SHIRT WIDTH} * 2) + 2 \text{ cm}) + 3.5\%.$$

Subsequent assembly steps are described below, with reference to FIGS. 21A-21M.

[0084] FIG. 21A shows a first end of a physiological sensor 2110 (produced as described herein) near which a “first” segment of TPU (breathing cable attachment 2111) has been laminated (e.g., by application of heat, or “heat press”). As shown in FIG. 21A, the breathing cable attachment 2111 has been placed about 2.5 cm from an end of the physiological sensor 2110. In some embodiments, the breathing cable attachment 2111 is folded along a fold line (see, e.g., FIG. 20A) such that it envelops the physiological sensor 2110, covering both faces thereof, while ensuring that the physiological sensor 2110 itself is not folded. A further breathing cable attachment 2111 can be positioned at the opposite end of the physiological sensor 2110 and attached in the same manner as described with reference to FIG. 21A. The breathing cable attachments 2111 should be well-bonded (i.e., bonded “through”) to the cable such that the conductive wire 2140 is not able to move inside the breathing cable attachments 2111 when the physiological sensor 2110 is pulled or stretched.

[0085] A portion of each of the end of the physiological sensor 2110 depicted in FIG. 21A may then be further cut (if needed), a segment of the textile portions (e.g., the elastic members) of the physiological sensor 2110 removed (e.g., by cutting and pulling away), and the conducting wire 2140 insulation (if present) stripped (see, e.g., location “S” in FIG. 21B). As shown in FIG. 21B, the conducting wire 2140 can be stripped such that there is about 0.5 cm of insulation intact that extends beyond the end of the respective breathing cable attachment 2111.

[0086] As shown in FIG. 21C, the stripped wires are fed through the outermost holes of a middle part with double holes 2113 (e.g., having its backing paper removed from a face to be bonded), and both breathing cable attachments 2111 are then laminated (e.g., ironed such that the wires remain in the outer holes) at least partially to the middle part with double holes 2113. In some embodiments, a backing paper disposed on the not-yet-bonded face of the middle part with double holes 2113 is left in place at this stage in the process. The lamination of the breathing cable attachments 2111 to the middle part with double holes 2113 physically secures them to one another, and can be done at an angle (see FIGS. 21D and 21E), for example if necessary or desired for subsequent assembly steps (e.g., based upon the design). For example, the lamination can be done at any angle (e.g., with respect to a longitudinal axis of the further, elongate TPU segment) required by the design, e.g., about 25 degrees, about 30 degrees, about 45 degrees, about 90 degrees, etc.

[0087] Next, an elongate (and, optionally, rigid) support bridge 2117 (shown in FIG. 21F), also bearing holes therethrough, is placed on the side of the middle part with double holes 2113 that is opposite where the exposed conductor ends have been fed through, and corresponding holes of the support bridge 2117 and the middle part with double holes 2113 (i.e., the “innermost” holes of the middle part with double holes 2113, as shown in FIG. 21F) are substantially aligned. The support bridge 2117 is then laminated to the middle part with double holes 2113 by applying heat (e.g., ironing or “heat press”), and a middle part with single holes

2115, comprising two holes, is positioned on top of the support bridge 2117, substantially aligned with the middle part with double holes 2113 (e.g., the innermost holes of the middle part with double holes 2113 are aligned with the holes of the middle part with single holes 2115), and laminated (again, optionally, with the assistance of a paper laminating sheet that is subsequently removed) thereto, resulting in the assembly (or “breathing cable structure”) shown in FIG. 21G.

[0088] Separately, a garment TPU segment 2123 is laminated onto a desired garment or fabric section (see “G” in FIGS. 21H-21M), for example, on a “reverse” or interior side of a garment, and holes (corresponding with the holes of garment TPU segment 2123) are made through the fabric of the garment G for subsequent placement of snaps or other connector hardware, such as a hook connector, a Velcro® based connector, or the like. The assembly (or “breathing cable structure” of FIG. 21G) is placed onto the garment TPU segment 2123 that has been applied to the garment G, the holes are aligned, and the assembly is laminated to the garment TPU segment 2123 (again, optionally, with the assistance of a paper laminating sheet, after which lamination, the paper is removed). The result is shown in FIG. 21I.

[0089] Turning now to FIG. 21J, the backing paper of the middle part with double holes 2113 is removed, and the exposed wire ends protruding through the outer holes of the middle part with double holes 2113 are twisted/coiled into loops “L” about the innermost holes of the middle part with double holes 2113.

[0090] As shown in FIG. 21K, a first liner sheet is removed from each of two conductive tape rings 2119 to reveal bare adhesive faces thereof, and the bare adhesive faces of the conductive tape rings 2119 are positioned atop loops L, aligning the holes of the conductive tape rings 2119 with corresponding holes in the middle part with double holes 2113, and adhered thereto. A second liner sheet is then removed from each of two conductive tape rings 2119 to reveal further bare adhesive faces thereof. Snap posts are emplaced through each of the wire loops L and corresponding holes in the garment G, and snaps are affixed thereto.

[0091] FIG. 21L shows garment G with the assembly and snaps in place, and a final cover 2125 covering the snaps (e.g., adhered in place by ironing, heat sealing, and/or the like). The garment G is then folded along a longitudinal fold line (see dashed line in FIGS. 21K and 21L), resulting in a folded band shown in FIG. 21M. In some embodiments, the folded band is stitched along at least one edge thereof.

[0092] FIG. 22A shows an exterior view, and 22B shows an interior view, of an assembled biosensing sports bra according to an embodiment. In FIG. 22A, two “sockets” 2219 and 2221 are visible along the lower hem of the sports bra, substantially near a side of the biosensing sports bra. In FIG. 22B an interior portion of the biosensing sports bra of FIG. 22A is shown, in which two “caps” 2222 and 2223 (of the connectors comprising the socket connectors of FIG. 22A) are visible and are covered by an inner layer of fabric of the biosensing sports bra.

[0093] FIGS. 23A-23C show views of an assembled biosensing brassiere according to an embodiment. In FIG. 23A, two “sockets” 2319 and 2321 are visible near a lower band (e.g., an elastic material and/or a “soft” or “comfort material, etc.) of the biosensing brassiere, substantially near a left side (wearer’s perspective) of the biosensing brassiere. FIG. 23B shows both an outer view of the left brassiere strap, includ-

ing the sockets **2319** and **2321** of FIG. **23A** as well as a modified “eye” portion of a traditional “hook and eye” closure. One of the six “eyes” of the hook and eye closure has been replaced with a “stud” that is connectable with a corresponding socket located on an inner surface of the right strap of the brassiere (also shown in FIG. **23B**). FIG. **23C** shows a close-up view of the connection made between the stud and the socket connectors of the brassiere of FIGS. **23A-23B**. In some embodiments, the connection may instead be made by connecting stripped ends of the physiological sensor wires, on an inner surface of the biosensing brassiere, to multiple (e.g., **3**) of the “hook” closure elements, thereby maintaining the adjustability of the brassier closure. Such connection can be made, for example, by stitching, crimping, twisting, applying conductive adhesive and/or laminating.

[0094] FIG. **24A** shows an interior view of the lower band of the biosensing brassiere of FIGS. **23A-23C**. As indicated by the arrow “A,” the physiological sensor is positioned beneath an inner fabric layer of the lower band of the brassiere, and its contours are faintly visible through the inner fabric. The physiological sensor is thus disposed such that, when the straps of the biosensing brassiere are connected during use by a user, the physiological sensor (e.g., including an elongate member and conductive wire, as described herein) traverses the circumference of the user. FIG. **24B** shows an exterior view of the biosensing brassiere of FIGS. **23A-23C** and FIG. **24A**, illustrating that the physiological sensor is not externally visible.

[0095] FIGS. **25A-25C** show views of a biosensing bra cami (or “camisole brassiere”) according to an embodiment. A bra cami is a camisole that has an integral brassiere connected to it (e.g., stitched to it, and in some instances sharing common shoulder straps). FIG. **25A** shows an overall, exterior view of a biosensing bra, illustrating that the physiological sensor is not externally visible. FIG. **25B** shows an interior view of the biosensing bra cami, including an exterior left side (wearer’s perspective) view of the integral brassiere. In FIG. **25B**, two “sockets” **2519** and **2521** are visible near a lower band of the integral brassiere. FIG. **25C** shows an interior portion of the biosensing bra cami of FIG. **25A**. Two “caps” **2522** and **2523** (of the connectors comprising the socket connectors of FIG. **25B**) are visible and are covered by an inner layer of fabric of the biosensing bra cami.

[0096] In some embodiments, an apparatus according to the present disclosure includes an elongate member having a longitudinal axis and configured to be stretchable along its longitudinal axis. The elongate member includes a plurality of elastic members: a first elastic member, a second elastic member that extends substantially parallel to the first elastic member, and a third elastic member that extends substantially parallel to the second elastic member. A conductive member (or “wire”) is coupled to the first, second and third members, and forms a “curved” pattern along the longitudinal axis of the elongate member. The conductive member (and, correspondingly, its curved pattern) is configured to change from a first configuration to a second configuration as the elongate member stretches along its longitudinal axis. This change of configuration results in a change in an inductance value of the conductive member. In some embodiments, instead of a curved pattern, the conductive member may be combined with the first, second and third elastic members such that it has a sawtooth, square, or

triangle shape along at least a portion of its length. In some embodiments, multiple conductive members may be coupled to the elongate member, the conductive members having like or different patterns, or a single conductive member with a substantially constant pattern (i.e., shape and/or periodicity), or multiple conductive members each having a different pattern (i.e., shape and/or periodicity). The patterns of the conductive members described herein may be periodic, aperiodic, symmetric, and/or asymmetric along portions of or the entireties of their length(s). In some embodiments, the patterns of the conductive members described herein may be present along only portions of the elongate member, the rest of the elongate member (and/or the conductive member embedded therewithin) being substantially “straight.”

[0097] In some embodiments, a method of making an elongate member involves forming a first elastic member, forming a second elastic member, forming a third elastic member, and braiding a conductive member (e.g., a wire having an insulating coating or shielding) with the first, second and third elastic members such that the conductive member has a curved (e.g., sinusoidal) pattern. In some embodiments, instead of a curved pattern, the conductive member may be combined with the first, second and third elastic members such that it has a sawtooth, square, or triangle shape along at least a portion of its length. In some embodiments, multiple conductive members may be coupled to the elongate member, the conductive members having like or different patterns, or a single conductive member with a substantially constant pattern (i.e., shape and/or periodicity), or multiple conductive members each having a different pattern (i.e., shape and/or periodicity). The patterns of the conductive members described herein may be periodic, aperiodic, symmetric, and/or asymmetric along portions of or the entireties of their length(s). In some embodiments, the patterns of the conductive members described herein may be present along only portions of the elongate member, the rest of the elongate member (and/or the conductive member embedded therewithin) being substantially “straight.”

[0098] In some embodiments, a method of manufacturing a biosensing element includes knitting a first elastic member from a single yarn, forming at least one further elastic member, and threading a conductive wire through a filament of the single yarn and the at least one further elastic member. The conductive wire has a substantially fixed curved pattern and joins the single yarn and the at least one further elastic member to form an elongate member.

[0099] In some embodiments, an apparatus according to the present disclosure includes an elongate member having a longitudinal axis and configured to be stretchable along its longitudinal axis. The elongate member includes a plurality of substantially parallel elastic members and a conductive member comprising an electrical conductor. The conductive member is coupled to the elongate member by physical connection to at least one of the plurality of elastic members. The conductive member is disposed in a regular pattern along the longitudinal axis of the elongate member. The regular pattern corresponds to a first inductance value of the conductive member. The conductive member is configured to change from a first configuration to a second configuration in response to an applied force, the change from the first configuration to the second configuration resulting in a

change from the first inductance value of the conductive member to a second inductance value of the conductive member.

[0100] As used herein, the terms “about” and “approximately” generally mean plus or minus 10% of the value stated, for example about 250 μm would include 225 μm to 275 μm , about 1,000 μm would include 900 μm to 1,100 μm .

[0101] While various embodiments of the system, methods and devices have been described above, it should be understood that they have been presented by way of example only, and not limitation. Where methods and steps described above indicate certain events occurring in a certain order, those of ordinary skill in the art having the benefit of this disclosure would recognize that the ordering of certain steps may be modified and such modification are in accordance with the variations of the invention. Additionally, certain of the steps may be performed concurrently in a parallel process when possible, as well as performed sequentially as described above. The embodiments have been particularly shown and described, but it will be understood that various changes in form and details may be made.

1. An apparatus comprising:

an elongate member defining a longitudinal axis and configured to be stretchable along the longitudinal axis, the elongate member including a first elastic member, a second elastic member extending substantially parallel to the first elastic member, and a third elastic member extending substantially parallel to the second elastic member; and

a conductive member coupled to the first, second and third elastic members in a curved pattern along the longitudinal axis of the elongate member, the curved pattern of the conductive member configured to change from a first configuration to a second configuration as the elongate member stretches along the longitudinal axis, the change from the first configuration to the second configuration resulting in a change of inductance of the conductive member.

2. The apparatus of claim 1, wherein the second elastic member is spaced a non-zero distance from the first elastic member.

3. The apparatus of claim 2, wherein the third elastic member is spaced a non-zero distance from the second elastic member.

4. The apparatus of claim 1, wherein at least one of the first, second and third elastic members is formed of an elastic material and a non-elastic material.

5. The apparatus of claim 1, wherein at least one of the first, second and third elastic members is knitted from a single yarn.

6. The apparatus of claim 5, wherein the single yarn includes an elastic filament and a texturized, non-elastic multifilament.

7. The apparatus of claim 6, wherein the elastic filament and the texturized, non-elastic multifilament are twisted together to form the single yarn.

8. The apparatus of claim 7, wherein the texturized, non-elastic multifilament is a first texturized, non-elastic multifilament, the single yarn further including a second texturized, non-elastic multifilament twisted together with the first texturized, non-elastic multifilament and the elastic filament to form the single yarn.

9. The apparatus of claim 7, wherein the elastic filament is elastane.

10. The apparatus of claim 7, wherein the texturized, non-elastic multifilament is nylon.

11. The apparatus of claim 1, wherein the curved pattern of the conductive member is substantially sinusoidal.

12. The apparatus of claim 1, wherein the conductive member is integrally formed with the elongate member in the curved pattern.

13. The apparatus of claim 12, wherein the conductive member is knitted with the first, second, and third elastic members in the curved pattern.

14. The apparatus of claim 13, wherein the conductive member is weft knitted.

15. An apparatus comprising:

an elongate member defining a longitudinal axis and configured to be stretchable along the longitudinal axis, the elongate member including a plurality of substantially parallel elastic members; and

a conductive member comprising an electrical conductor, the conductive member fixedly coupled to at least one of the plurality of substantially parallel elastic members,

the conductive member disposed in a regular pattern along the longitudinal axis of the elongate member and configured to move between a first configuration and a second configuration,

the conductive member having a first inductance value in the first configuration, and a second inductance value in the second configuration.

16. The apparatus of claim 15, wherein the regular pattern of the conductive member is a curved pattern.

17. The apparatus of claim 16, wherein the curved pattern of the conductive member is substantially sinusoidal.

18. The apparatus of claim 15, further comprising:

a first connector coupled to a first end of the elongate member and a second connector coupled to a second end of the elongate member, the first connector disposed proximate the second connector thereby forming an open loop.

19. The apparatus of claim 18, wherein the open loop is disposed in at least one of a substantially circular shape, a substantially oval shape, a substantially square shape, a substantially rectangular shape, and an irregularly shape.

20. The apparatus of claim 15, wherein the elongate member includes a first portion extending from a first connector in a first direction, and a second portion extending in a second direction from the first portion to a second connector.

21. The apparatus of claim 20, wherein the second direction is opposite the first direction.

22. The apparatus of claim 20, wherein the second connector is proximate the first connector.

23. The apparatus of claim 20, wherein the second portion is folded back onto the first portion.

24. An apparatus comprising:

a plurality of substantially parallel elastic members disposed along an axis and configured to be stretchable along the axis; and

a conductive member disposed in a regular pattern and fixedly coupled to at least one of the plurality of substantially parallel elastic members, the conductive member configured to move between a first configuration and a second configuration,

the conductive member having a first inductance value in the first configuration, and a second inductance value in the second configuration.

25. The apparatus of claim **24**, wherein the regular pattern is substantially sinusoidal.

26. The apparatus of claim **24**, wherein the plurality of substantially parallel elastic members includes a first elastic member, a second elastic member spaced a non-zero distance from the first elastic member, and a third elastic member spaced a non-zero distance from the second elastic member.

27. The apparatus of claim **24**, further comprising:
a first connector coupled to a first end of the conductive member and a second connector coupled to a second end of the conductive member, the first connector disposed proximate the second connector thereby forming an open loop.

28. The apparatus of claim **27**, wherein the open loop is disposed in at least one of a substantially circular shape, a substantially oval shape, a substantially square shape, a substantially rectangular shape, and an irregularly shape.

29. The apparatus of claim **24**, wherein the conductive member includes a first portion extending from a first connector in a first direction, and a second portion extending in a second direction from the first portion to a second connector.

30. The apparatus of claim **29**, wherein the second direction is opposite the first direction.

31. The apparatus of claim **29**, wherein the second connector is proximate the first connector.

32. The apparatus of claim **29**, wherein the second portion is folded back onto the first portion.

* * * * *

专利名称(译)	用于监测生物传感服装中的呼吸的系统和方法		
公开(公告)号	US20180317814A1	公开(公告)日	2018-11-08
申请号	US15/907913	申请日	2018-02-28
[标]申请(专利权)人(译)	OMSIGNAL		
申请(专利权)人(译)	OMSIGNAL INC.		
当前申请(专利权)人(译)	OMSIGNAL INC.		
[标]发明人	NURKKA MARIA ELINA		
发明人	NURKKA, MARIA ELINA		
IPC分类号	A61B5/113 A61B5/00		
CPC分类号	A61B5/1135 A61B5/6805 D04B21/18 D10B2403/02431 D10B2403/0311 H05K2201/0133 H05K3/103 D04B21/16 A61B5/0806 G01B7/16		
优先权	62/212899 2015-09-01 US 62/247049 2015-10-27 US		
外部链接	Espacenet USPTO		

摘要(译)

本文描述的实施例总体上涉及生物传感服装，并且具体地涉及用于监测生物传感服装中的呼吸的系统和方法，由此实现呼吸监测电路到服装中的改进的集成，从而改善信号质量和耐久性。在一些实施例中，一种装置包括细长构件，所述细长构件具有纵向轴线并且构造成沿其纵向轴线可拉伸。细长构件包括沿纵向轴线延伸的多个弹性构件（例如，第一弹性构件，第二弹性构件和第三弹性构件）。导电构件连接到第一，第二和第三构件，并沿细长构件的纵向轴线形成“弯曲”图案。当细长构件沿其纵向轴线伸展时，导电构件构造成从第一构型变为第二构型。

