

(43) **Pub. Date:** **Jun. 19, 2014**

The diagram illustrates a closed-loop control system for a prosthetic arm. A human arm (30) is connected to a hydraulic cylinder (46) via a line (32). The cylinder is actuated by a servo motor (40) through a motor (M, 38) and a pulley (34). The servo motor receives a setpoint $P_{set}(t)$. The hydraulic cylinder is connected to a pressure transducer (53) and a flow transducer (56). The pressure transducer outputs $P(t)$ and the flow transducer outputs $f(t)$. Both signals are processed by comparators (60, 58) and an ADC (54) to generate a control signal. The control signal is processed by a microcontroller (62) and a DAC (64) to drive the servo motor.

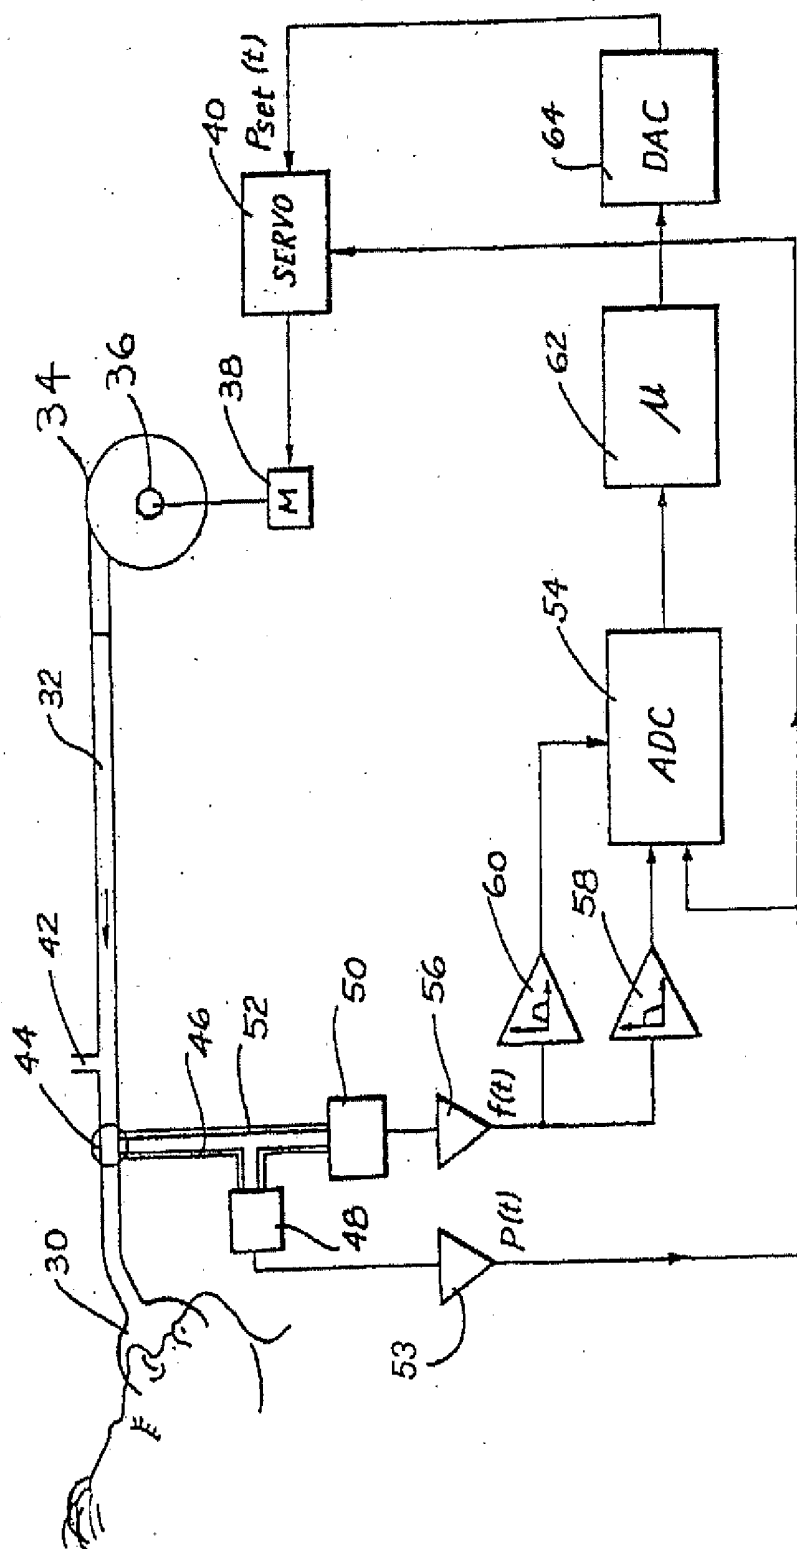


FIG. 1

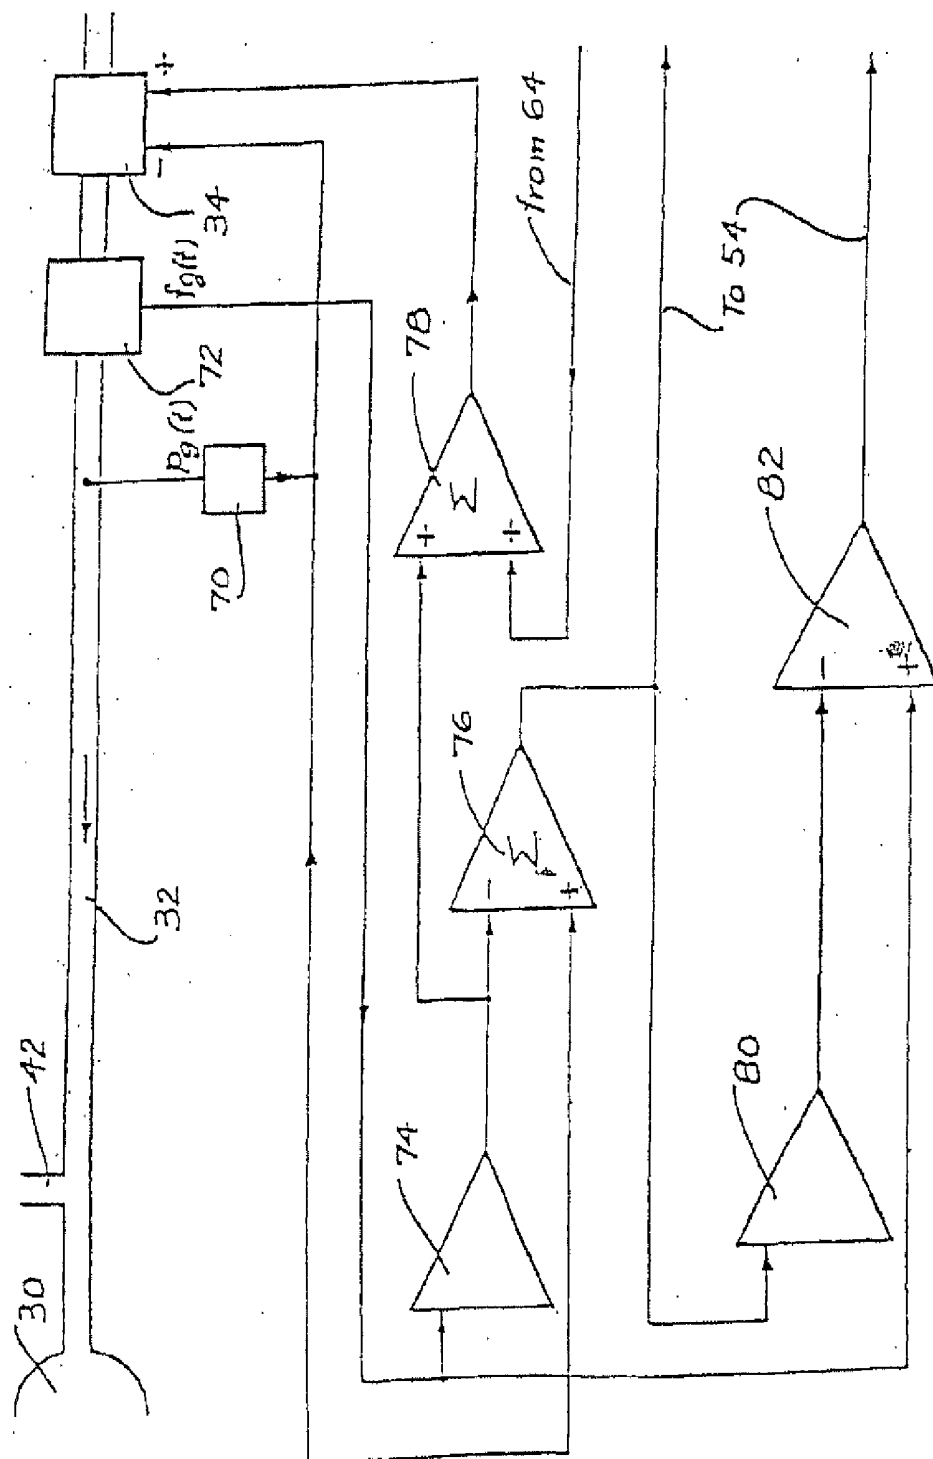


FIG. 2

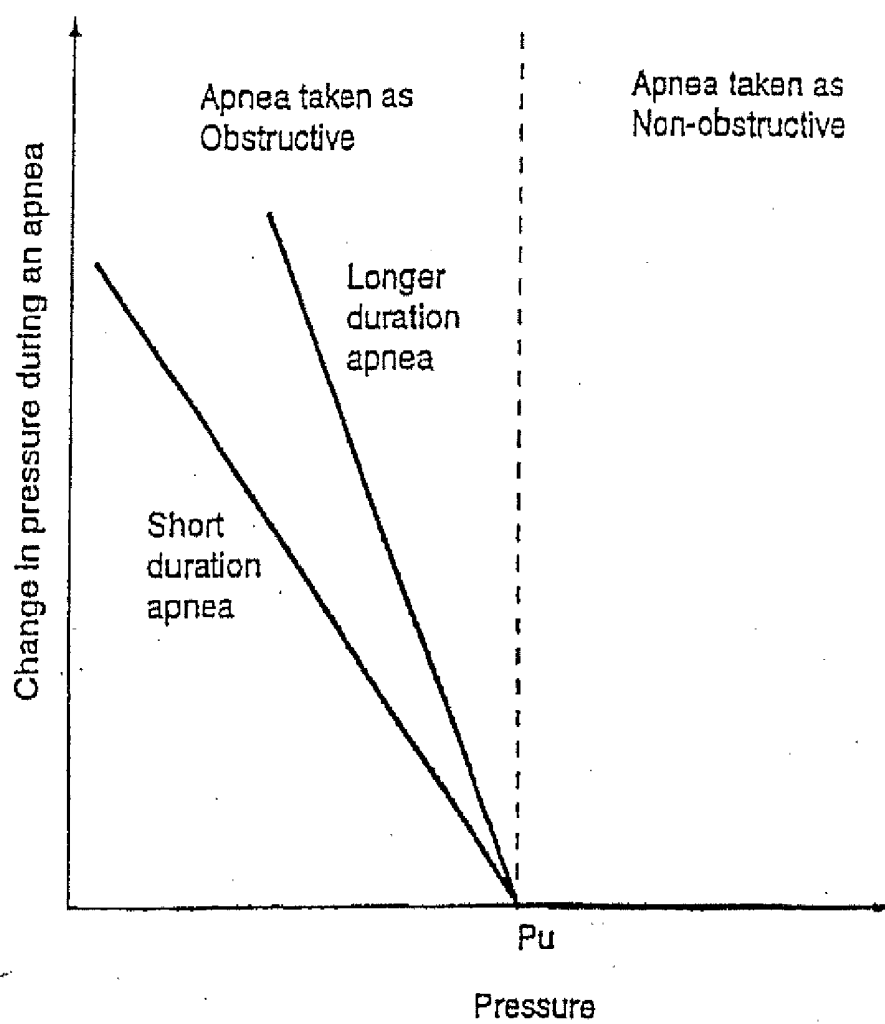
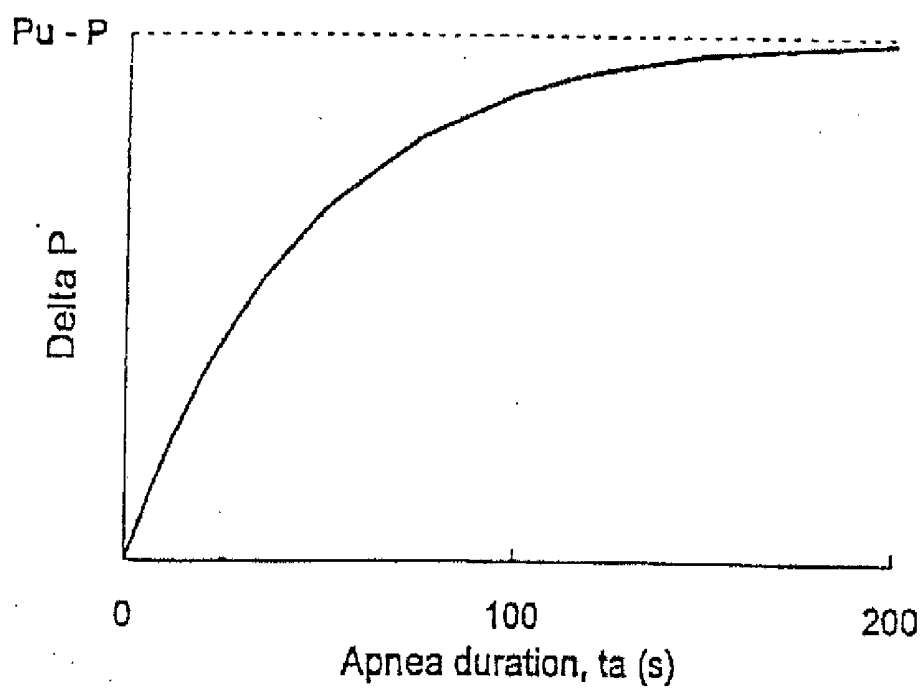


FIG. 3

**FIG. 4**

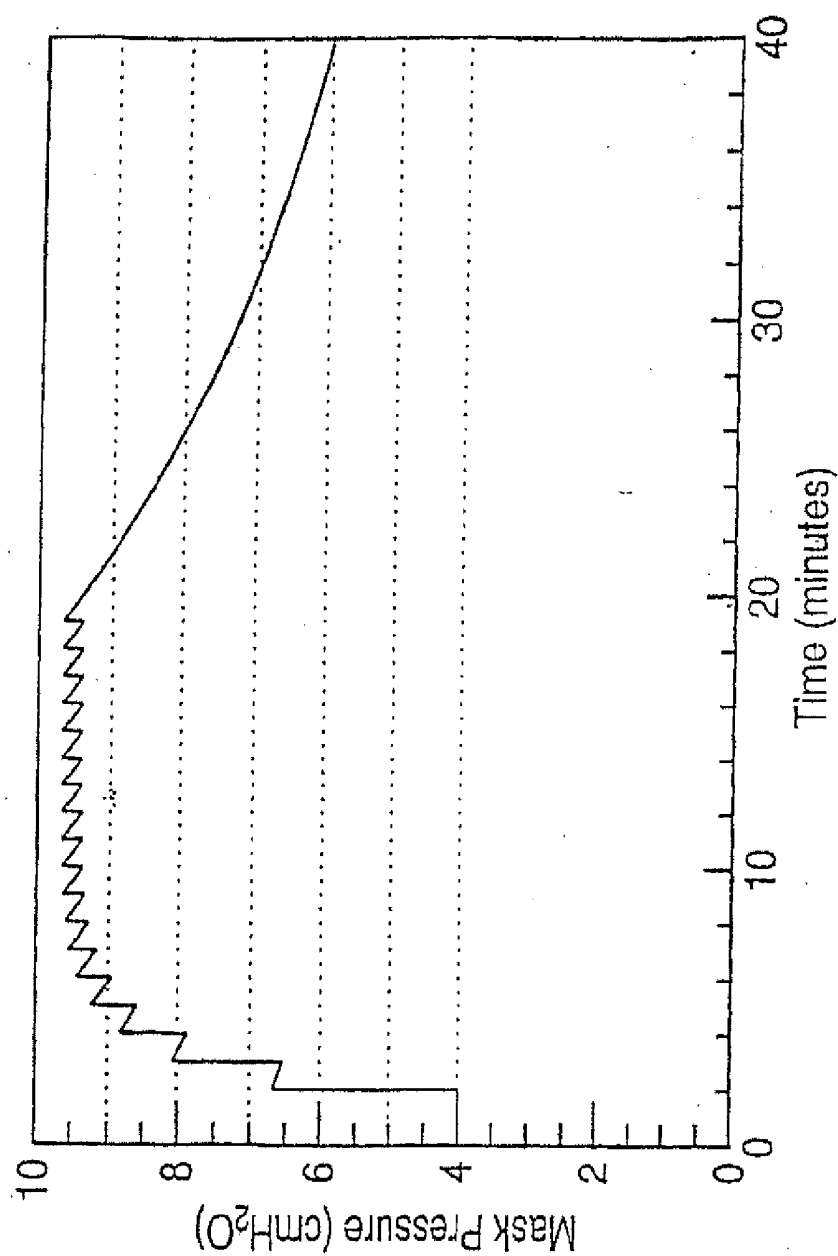


FIG. 5

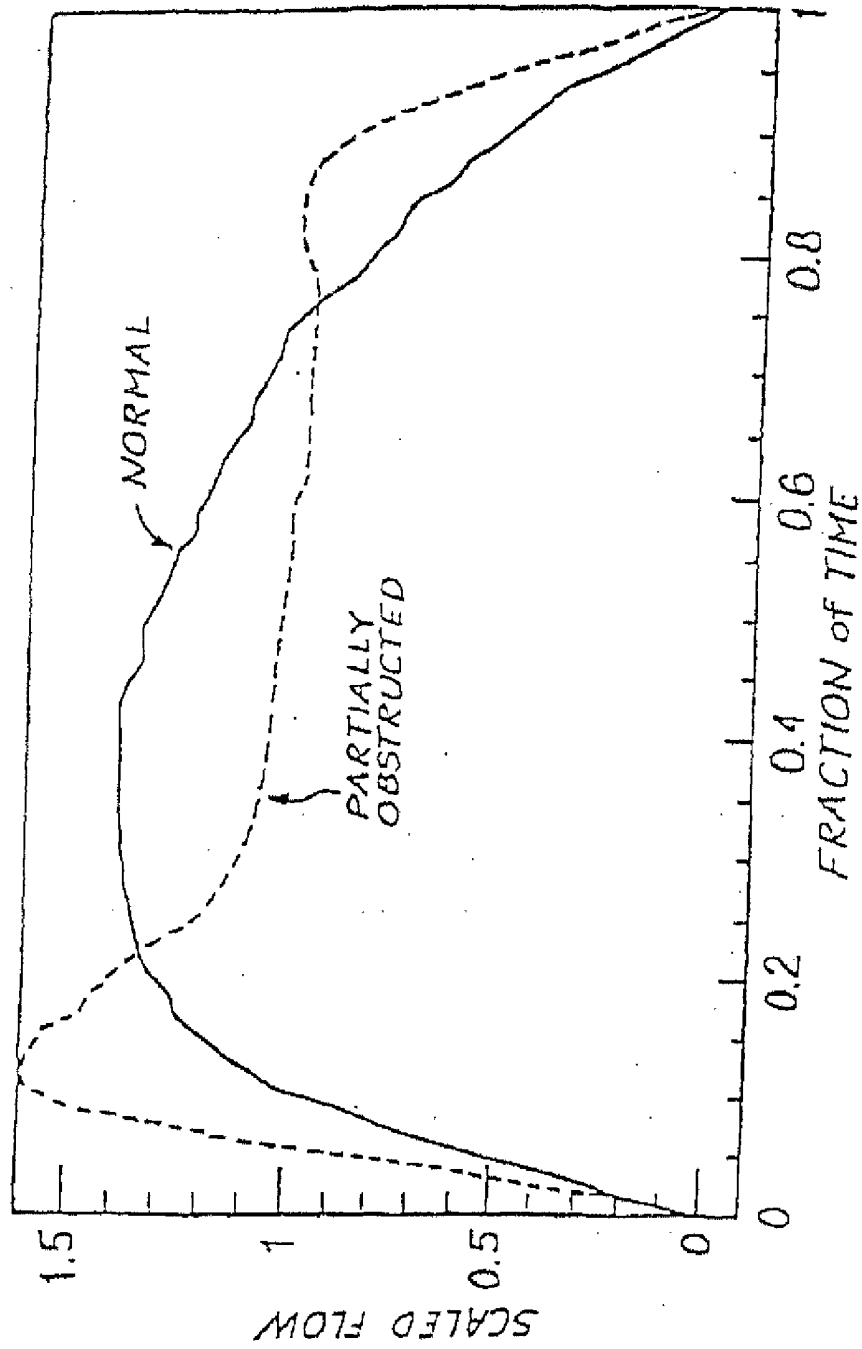


FIG. 6

ADMINISTRATION OF CPAP TREATMENT PRESSURE IN PRESENCE OF APNEA

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation of U.S. patent application Ser. No. 13/477,505, filed May 22, 2012, which is a continuation of U.S. patent application Ser. No. 12/250,188, filed Oct. 13, 2008, which is a continuation of U.S. patent application Ser. No. 11/237,278, filed Sep. 28, 2005, which is a continuation of U.S. Pat. No. 6,988,498, issued Jan. 24, 2006, which is a continuation of U.S. Pat. No. 6,817,361, issued Nov. 16, 2004, which is a continuation of U.S. Pat. No. 6,502,572, issued Jan. 7, 2003, which is a continuation-in-part of U.S. Pat. No. 6,367,474, issued Apr. 9, 2002, which claims priority from Australian Application No. PP0269, filed Nov. 7, 1997, the disclosure of which is incorporated herein by reference.

FIELD OF THE INVENTION

[0002] This invention relates to the administration of continuous positive airway pressure (CPAP) treatment for partial or complete upper airway obstruction.

BACKGROUND OF THE INVENTION

[0003] In the Sleep Apnea syndrome a person stops breathing during sleep. Cessation of airflow for more than 10 seconds is called an "apnea". Apneas lead to decreased blood oxygenation and thus to disruption of sleep. Apneas are traditionally (but confusingly) categorized as either central, where there is no respiratory effort, or obstructive, where there is respiratory effort. With some central apneas, the airway is open, and the subject is merely not attempting to breathe. Conversely, with other central apneas and all obstructive apneas, the airway is closed. The occlusion is usually at the level of the tongue or soft palate. The airway may also be partially obstructed (i.e., narrowed or partially patent). This also leads to decreased ventilation (hypopnea), decreased blood oxygenation and disturbed sleep.

[0004] The common form of treatment of these syndromes is the administration of Continuous Positive Airway Pressure (CPAP). The procedure for administering CPAP treatment has been well documented in both the technical and patent literature. An early description can be found in U.S. Pat. No. 4,944,310 (Sullivan). Briefly stated, CPAP treatment acts as a pneumatic splint of the airway by the provision of a positive pressure usually in the range 4-20 cm H₂O. The air is supplied to the airway by a motor driven blower whose outlet passes via an air delivery hose to a nose (or nose and/or mouth) mask sealingly engaged to a patient's face. An exhaust port is provided in the delivery tube proximate to the mask. The mask can take the form of a nose and/or face mask or nasal prongs, pillows or cannulae.

[0005] Various techniques are known for sensing and detecting abnormal breathing patterns indicative of obstructed breathing. U.S. Pat. No. 5,245,995 (Sullivan et al.), for example, generally describes how snoring and abnormal breathing patterns can be detected by inspiration and expiration pressure measurements made while a subject is sleeping, thereby leading to early indication of preobstructive episodes or other forms of breathing disorder. Particularly, patterns of respiratory parameters are monitored, and CPAP pressure is raised on the detection of pre-defined patterns to

provide increased airway pressure to, ideally, subvert the occurrence of the obstructive episodes and the other forms of breathing disorder.

[0006] Automatic detection of partial upper airway obstruction and pre-emptive adjustment of nasal CPAP pressure works to prevent frank obstructive apneas in the majority of subjects with obstructive sleep apnea syndrome. However, some subjects with severe disease progress directly from a stable open upper airway to a closed airway apnea with complete airway closure, with little or no intervening period of partial obstruction. Therefore it is useful for an automatically adjusting CPAP system to also respond to a closed airway apnea by an increase in CPAP pressure. However, it is not desirable to increase CPAP pressure in response to open airway apneas, firstly because this leads to an unnecessarily high pressure and secondly because the high pressure can reflexly cause yet further open airway apneas, leading to a vicious circle of pressure increase.

[0007] One method for distinguishing open airway apneas (requiring no increase in pressure) from closed airway apneas (requiring a pressure increase) is disclosed in commonly owned European Publication No. 0 651 971 A1 (corresponding to U.S. Pat. No. 5,704,345). During an apnea, the mask pressure is modulated at 4 Hz with an amplitude of the order of 1 cmH₂O, the induced airflow at 4 Hz is measured, and the conductance of the airway is calculated. A high conductance indicates an open airway. This 'forced oscillation method' requires the ability to modulate the mask pressure at 4 Hz, which increases the cost of the device. Furthermore, the method does not work in the presence of high leak, and can falsely report that the airway is closed if the subject has a high nasal or intrapulmonary resistance.

[0008] The present invention is directed to overcoming or at least ameliorating one or more of the foregoing disadvantages in the prior art.

BRIEF SUMMARY OF THE INVENTION

[0009] Therefore, the invention discloses a method for the administration of CPAP treatment pressure comprising the steps of:

[0010] supplying breathable gas to the patient's airway at a treatment pressure;

[0011] determining a measure of respiratory airflow; and

[0012] determining the occurrence of an apnea from a reduction in the measure of respiratory airflow below a threshold, and, if having occurred

[0013] (i) determining the duration of the apnea; and

[0014] (ii) increasing the treatment pressure by an amount which is an increasing function of the duration of the apnea, and a decreasing function of the treatment pressure immediately before the apnea.

[0015] The invention further discloses CPAP treatment apparatus comprising:

[0016] a controllable flow generator operable to produce breathable gas at a pressure elevated above atmosphere;

[0017] a gas delivery tube coupled to the flow generator;

[0018] a patient mask coupled to the tube to receive said breathable gas from the flow generator and provide said gas, at a desired treatment pressure, to the patient's airway;

[0019] a controller operable to receive input signals and to control operation of said flow generator and hence the treatment pressure; and

[0020] sensor means located to sense patient respiratory airflow and generate a signal input to the controller from which patient respiratory airflow is determined;

[0021] and wherein said controller is operable to determine the occurrence of an apnea from a reduction in said respiratory airflow below a threshold, and if having occurred, to determine the duration of said apnea and cause said flow generator to increase CPAP treatment pressure by an amount that is an increasing function of said apnea duration, and a decreasing function of the treatment pressure immediately prior to said apnea.

[0022] The invention yet further provides CPAP treatment apparatus comprising:

[0023] a controllable flow generator operable to produce breathable gas to be provided to a patient at a treatment pressure elevated above atmosphere; and

[0024] a controller operable to receive input signals representing patient respiratory airflow, and to control operation of said flow generator and hence the treatment pressure;

[0025] and wherein said controller is operable to determine the occurrence of an apnea

[0026] from a reduction in said respiratory airflow below a threshold, and, if having occurred,

[0027] to determine the duration of said apnea and cause said flow generator to increase CPAP

[0028] treatment pressure by an amount that is an increasing function of said apnea duration, and a decreasing function of the treatment pressure immediately prior to said apnea.

[0029] Preferably, the increase in treatment pressure is zero if the treatment pressure before the apnea exceeds a pressure threshold. The increase in pressure below the pressure threshold can be an increasing function of the duration of the apnea, multiplied by the difference between the pressure threshold and the current treatment pressure. Further, the increasing function of apnea duration is linear on apnea duration. Advantageously, said increasing function of apnea duration is zero for zero apnea duration, and exponentially approaches an upper limit as apnea duration goes to infinity.

[0030] The occurrence of an apnea can be determined by calculating the RMS respiratory airflow over a short time interval, calculating the RMS respiratory airflow over a longer time interval, and declaring an apnea if the RMS respiratory airflow over the short time interval is less than a predetermined fraction of the RMS respiratory airflow over the longer time interval. There also can be the further step or action of reducing the treatment pressure towards an initial treatment pressure in the absence of a further apnea.

[0031] In a preferred form, said sensor means can comprise a flow sensor, and said controller derives respiratory airflow therefrom.

[0032] In one preferred form said initial treatment pressure is 4 cmH₂O, said measure of respiratory airflow is the 25% of the RMS airflow over the preceding 5 minutes. In this preferred form no increase in pressure is made for apneas of less than 10 seconds duration, or for apneas where the treatment pressure immediately prior to the apnea is more than 10 cmH₂O, but otherwise, the lower the treatment pressure immediately prior to the apnea, and the longer the apnea, the greater the increase in treatment pressure, up to a maximum of 8 cmH₂O per minute of apnea. In this preferred form, if there is no apnea the treatment pressure is gradually reduced towards the initial minimum pressure with a time constant of 20 minutes.

[0033] The method and apparatus can advantageously be used in concert with one or more other methods for determining the occurrence of partial upper airway obstruction, such that either complete or partial upper airway obstruction can lead to an increase in pressure, but once there is no longer either complete or partial obstruction, the pressure will gradually reduce towards the initial minimum pressure.

[0034] In one particularly preferred form, partial obstruction is detected as either the presence of snoring, or the presence of characteristic changes in the shape of the inspiratory flow-vs-time curve indicative of inspiratory airflow limitation.

[0035] The method and apparatus can also advantageously be used in concert with the 'forced oscillation method' for measuring airway patency (referred to above as European Publication No. 0 651 971 A1, U.S. Pat. No. 5,704,345 whose disclosure is hereby incorporated by reference), in which the CPAP pressure is modulated with an amplitude of for example 1 cm H₂O at 4 Hz, the induced airflow at 4 Hz is measured, the conductance of the airway calculated by dividing the amplitude of the induced airflow by the pressure modulation amplitude, and the additional requirement imposed that the treatment pressure is only increased if said conductance is greater than a threshold.

[0036] Closed airway apneas are most likely to occur at low CPAP pressures, because high CPAP pressures splint the airway partially or completely open whereas pressure-induced open airway apneas are most likely to occur at high CPAP pressures, at least partially because high CPAP pressures increase lung volume and thereby stimulate the Hering-Breuer reflex, leading to inhibition of breathing. Therefore, the lower the existing CPAP pressure, the more likely an apnea is to be of the closed airway variety, and the more appropriate it is to increase the treatment pressure, whereas the higher the existing CPAP pressure, the more likely an apnea is to be of the open airway variety, and the more appropriate it is to leave the CPAP pressure unchanged. Generally apneas of less than 10 seconds duration are regarded as non-pathological, and there is no need to increase CPAP pressure, whereas very long apneas require treatment. The present invention will correctly increase the CPAP pressure for most closed airway apneas, and correctly leave the CPAP pressure unchanged for most open airway apneas.

[0037] The present invention can be combined with an independent pressure increase in response to indicators of partial upper airway obstruction such as snoring or changes in shape of the inspiratory flow-time curve. In this way it is possible in most subjects to achieve pre-emptive control of the upper airway, with pressure increases in response to partial upper airway obstruction preventing the occurrence of closed airway apneas. In the minority of subjects in whom pre-emptive control is not achieved, this combination will also correctly increase the CPAP pressure in response to those closed airway apneas that occur at low CPAP pressure without prior snoring or changes in the shape of the inspiratory flow-time curve. Furthermore, the combination will avoid falsely increasing the CPAP pressure in response to open airway apneas induced by high pressure.

[0038] Some open airway apneas can occur at low pressure. By combining the forced oscillation method with the present invention, with the additional requirement that there be no increase in pressure if the forced oscillation method detects an open airway, false increases in pressure in response to open airway apneas at low pressure will be largely avoided.

BRIEF DESCRIPTION OF THE DRAWINGS

[0039] Embodiments of the invention will now be described with reference to the accompanying drawings, in which:

[0040] FIG. 1 shows, in diagrammatic form, apparatus embodying the invention;

[0041] FIG. 2 shows an alternative arrangement of the apparatus of FIG. 1;

[0042] FIG. 3 shows a plot of two pressure change characteristics as a function of apnea duration;

[0043] FIG. 4 shows a plot of the apnea duration function;

[0044] FIG. 5 shows a graph of CPAP treatment pressure versus time for a preferred embodiment of the invention; and

[0045] FIG. 6 shows a graph of scaled (normalized) air flow with time for normal and partially obstructed inspiration.

DETAILED DESCRIPTION

[0046] FIG. 1 shows, in diagrammatic form, CPAP apparatus in accordance with one embodiment. A mask 30, whether either a nose mask and/or a face mask, is sealingly fitted to a patient's face. Breathable gas in the form of fresh air, or oxygen enriched air, enters the mask 30 by flexible tubing 32 which, in turn is connected with a motor driven turbine 34 to which there is provided an air inlet 36. The motor 38 for the turbine is controlled by a motor-servo unit 40 to commence, increase or decrease the pressure of air supplied to the mask 30 as CPAP treatment. The mask 30 also includes an exhaust port 42 that is close to the junction of the tubing 34 with the mask 30.

[0047] Interposed between the mask 30 and the exhaust 42 is a linear flow-resistive element 44. In practice, the distance between mask 30 and exhaust 42, including flow resistive element 44 is very short so as to minimize deadspace volume. The mask side of the flow-resistive element 44 is connected by a small bore tube 46 to a mask pressure transducer 48 and to an input of a differential pressure transducer 50. Pressure at the other side of the flow-resistive element 44 is conveyed to the other input of the differential pressure transducer 50 by another small bore tube 52.

[0048] The mask pressure transducer 48 generates an electrical signal in proportion to the mask pressure, which is amplified by amplifier 52 and passed both to a multiplexer/ADC unit 54 and to the motor-servo unit 40. The function of the signal provided to the motor-servo unit 40 is as a form of feedback to ensure that the actual mask static pressure is controlled to be closely approximate to the set point pressure.

[0049] The differential pressure sensed across the linear flow-resistive element 44 is output as an electrical signal from the differential pressure transducer 50, and amplified by another amplifier 56. The output signal from the amplifier 56 therefore represents a measure of the mask airflow. The linear flow-resistive element 44 can be constructed using a flexible-vented iris. Alternatively, a fixed orifice can be used, in which case a linearization circuit is included in amplifier 52, or a linearization step such as table lookup included in the operation of controller 62.

[0050] The output signal from the amplifier 56 is low-pass filtered by the low-pass filter 58, typically with an upper limit of 10 Hz, in order to remove non-respiratory noise. The amplifier 56 output signal is also bandpassed by the bandpass filter 60, and typically in a range of 30-100 Hz to yield a snoring signal. The outputs from both the low-pass filter 58 and the bandpass filter 60 are provided to the digitizer (ADC)

unit 54. The digitized respiratory airflow (FLOW), snore, and mask pressure (P.sub.mask) signals from ADC 54 are passed to a controller 62 typically constituted by a micro-processor based device also provided with program memory and data processing storage memory.

[0051] The controller 62 outputs a pressure request signal which is converted to a voltage by DAC 64, and passed to the motor-servo unit 40. This signal therefore represents the set point pressure P.sub.set(t) to be supplied by the turbine 34 to the mask 30 in the administration of CPAP treatment. The controller 62 is programmed to perform a number of processing functions, as presently will be described.

[0052] As an alternative to the mask pressure transducer 48, a direct pressure/electrical solid state transducer (not shown) can be mounted from the mask with access to the space therewithin, or to the air delivery tubing 32 proximate the point of entry to the mask 30.

[0053] Further, it may not be convenient to mount the flow transducer 44 at or near the mask 30, nor to measure the mask pressure at or near the mask. An alternative arrangement, where the flow and pressure transducers are mounted at or near the air pressure generator (in the embodiment being the turbine 34) is shown in FIG. 2.

[0054] The pressure p.sub.g(t) occurring at the pressure generator 34 outlet is measured by a pressure transducer 70. The flow f.sub.g(t) through tubing 32 is measured with flow sensor 72 provided at the output of the turbine 34. The pressure loss along tubing 32 is calculated in element 74 from the flow through the tube f.sub.g(t), and a knowledge of the pressure-flow characteristic of the tubing, for example by table lookup. The pressure at the mask p.sub.m is then calculated in subtraction element 76 by subtracting the tube pressure loss from p.sub.g(t).

[0055] The pressure loss along tube 32 is then added to the desired set pressure at the mask p.sub.set(t) in summation element 78 to yield the desired instantaneous pressure at the pressure generator 34. Preferably, the controller of the pressure generator 34 has a negative feedback input from the pressure transducer 70, so that the desired pressure from step 78 is achieved more accurately. The flow through the exhaust 42 is calculated from the pressure at the mask (calculated in element 76) from the pressure-flow characteristic of the exhaust in element 80, for example by table lookup. Finally, the mask flow is calculated by subtracting the flow through the exhaust 42 from the flow through the tubing 32, in subtraction element 82.

[0056] The methodology put into place by the controller 62 will now be described. In a first embodiment, there is a pressure response to apneas, but not to indicators of partial obstruction, and therefore snore detection bandpass filter 60 is not required.

[0057] An initial CPAP treatment pressure, typically 4 cmH.sub.2O, is supplied to the subject. The FLOW signal is processed to detect the occurrence of an apnea (as will presently be discussed) and, at the same time the P.sub.mask signal is recorded. When it is determined that an apnea has occurred its duration is recorded. At the same time P.sub.mask is compared against a pressure threshold, P.sub.u. If P.sub.mask is at or above P.sub.u the controller will act to maintain or reduce that pressure. If, on the other hand, P.sub.mask is below P.sub.u, the controller will act to increase the treatment pressure by an amount .DELTA.P.

[0058] In a preferred form, .DELTA.P is determined as follows

$$.DELTA.P = [P_{sub.u} - P] / f(t_{sub.a}) \quad (1)$$

[0059] where

[0060] .DELTA.P is the change in pressure (cmH.sub.2O)

[0061] P.sub.u is the pressure threshold, which in an embodiment can be 10 cmH.sub.2O

[0062] P is the current treatment pressure immediately before the apnea (cmH.sub.2O)

[0063] t.sub.a is the apnea duration(s)

[0064] f(t.sub.a) is a function that is a monotonically increasing function of t.sub.a, zero for t.sub.a=0

[0065] FIG. 3 is a graphical representation of equation (1), showing a region below P.sub.u where it is taken that an apnea is obstructive and demonstrating two cases of the .DELTA.P characteristic as a function of apnea duration (i.e., short and longer) such that .DELTA.P is an increasing function of apnea duration and a decreasing function of the current treatment pressure. Above P.sub.u, it is taken that the apnea is non-obstructive, and .DELTA.P is held to be zero for all values of the current treatment pressure.

[0066] One form of the function f(t.sub.a) is:

$$1/f(t.a) = r + P_{max} \quad (2)$$

[0067] In one embodiment the parameters can be:

[0068] r=0.13 cmH.sub.2O.s.sup.-1

[0069] .DELTA.P.sub.max=6 cmH.sub.2O

[0070] Another form of the function f(t.sub.a) is:

$$f(t_{sub.a}) = 1 - \exp(-kt_{sub.a}) \quad (3)$$

[0071] In one embodiment the parameter can be k=0.02 s.sup.-1

[0072] FIG. 4 is a graphical representation of equation (3) for the parameters given above.

[0073] The controller 62 implements the foregoing methodology using the following pseudo-code.

```

Set apnea duration to zero
Clear "start of breath" flag
Set initial CPAP pressure to 4 cmH.sub.2O.
Set maximum delta pressure due to apnea to 6
cmH.sub.2O.
Set top roll-off pressure to initial CPAP pressure
plus maximum delta pressure due to apnea.
REPEAT
  Sample mask airflow (in L/sec) at 50 Hz.
  Calculate mask leak as mask airflow low pass
  filtered with a time constant of 10 seconds.
  Check for presence and duration of any apnea
  Check for start of breath.
  IF start of breath flag set:
    IF apnea duration greater than 10 seconds AND
    current CPAP pressure less than top roll-off pressure:
      Set delta pressure for this apnea to (top roll-off
      pressure-current CPAP pressure)/maximum delta pressure due to
      apnea times 8 cmH.sub.2O per minute of apnea duration.
      Add delta pressure for this apnea to total delta
      pressure due to apnea, and truncate to maximum delta pressure
      due to apnea.
      Reset apnea duration to zero.
    ELSE
      Reduce total delta pressure due to apnea with a time
      constant of 20 minutes.
    End
  Set CPAP pressure to initial CPAP pressure plus
  total delta pressure due to apnea.

```

-continued

```

Clear start of breath flag.
END
END

```

[0074] This implementation is suitable for subjects in whom obstructive apneas are controlled at a CPAP pressure of less than 10 cmH.sub.2O. Increasing the maximum delta pressure due to apnea from 6 cmH.sub.2O to 10 cmH.sub.2O would permit the prevention of obstructive apneas in the majority of subjects, in exchange for an increase in undesirable pressure increases due to open airway apneas.

[0075] The procedure "Check for presence and duration of any apnea" can be implemented using the following pseudocode:

```

Calculate 2 second RMS airflow as the RMS airflow
over the previous 2 seconds.
Calculate long term average RMS airflow as the 2
second RMS airflow, low pass filtered with a time constant of
300 seconds.
IF 2 second RMS airflow is less than 25% of long
term average RMS airflow:
  Mark apnea detected and increment apnea duration by
  {fraction (1/50)} second.
END
The procedure, "Check for start of breath" is
implemented by the following pseudocode:
IF respiratory airflow is inspiratory AND
respiratory airflow on previous sample was not inspiratory.
  Set "start of breath" flag.
END

```

[0076] FIG. 5 shows the above method and apparatus in operation. The mask 30 was connected to a piston driven breathing simulator set to a normal respiratory rate and depth, and programmed to introduce a 20 second apnea once per minute from the 2nd minute to the 20th minute. In operation, the pressure remained at the initial pressure of 4 cmH.sub.2O until the first apnea, which led to a brisk increase in mask pressure. The pressure then decayed slightly during the subsequent 40 seconds of normal breathing.

[0077] Subsequent apneas produced smaller increments, and the mask pressure settled out to approximately 9.5 cmH.sub.2O. In most actual patients, the number of apneas would reduce as the pressure increased. Because the pressure due to repetitive apneas cannot exceed 10 cmH.sub.2O, and most pressure-induced open airway apneas occur at very high pressures typically above 10 cmH.sub.2O, this algorithm will not falsely or needlessly increase pressure in response to most pressure-induced open airway apneas, thus avoiding a vicious cycle of high pressure leading to open airway apneas leading to yet further pressure increase.

[0078] The above embodiment can be considerably improved by the addition of independent pressure increases in response to partial upper airway obstruction indicated by the presence of snoring or changes in the shape of the inspiratory flow-vs-time curve. In the majority of subjects, in whom substantial periods of snoring or flow limitation exist prior to any closed airway apneas, the CPAP pressure will increase in response to said snoring and/or changes in the shape of the inspiratory flow-vs-time curve, to a sufficient level to largely eliminate severe partial obstruction, without any apneas of any kind occurring. In those subjects in whom closed airway

apneas appear with little or no prior period of partial obstruction, the first few apneas will produce a brisk increase in CPAP pressure as previously discussed, and in general this will provide sufficient partial support to the airway to permit periods of detectable partial obstruction, preventing any further apneas from occurring.

[0079] This second embodiment is implemented using the following pseudocode.

```

Set initial CPAP pressure to 4 cmH.sub.2O.
Set apnea duration to zero
Clear "start of breath" flag
REPEAT every {fraction (1/50)} of a second
Sample mask pressure (in cmH.sub.2O), mask airflow
(in L/sec), and snore (1 unit corresponds loosely to a typical
snore).
    Calculate mask leak as mask airflow low pass
    filtered with a time constant of 10 seconds.
    Adjust snore signal for machine noise.
    Check for presence and duration of any apnea.
    Check for start of breath.
    IF start of breath flag set:
    IF apnea duration greater than 10 seconds AND
    current CPAP pressure less than 10 cmH.sub.2O:
        Set delta pressure for this apnea to (10--current
        CPAP pressure)/6 times 8 cmH.sub.2O per minute of apnea
        duration.
        Add delta pressure for this apnea to total delta
        pressure due to apnea, and truncate to 16 cmH.sub.2O
        Reset apnea duration to zero.
    ELSE
        Reduce total delta pressure due to apnea with a time
        constant of 20 minutes.
    END
    Calculate flow limitation index.
    Calculate flow limitation threshold.
    IF flow limitation index is less than said
    threshold:
        Set flow limitation delta pressure for this breath
        to 3 cmH.sub.2O times (threshold-flow limitation index).
        Add flow limitation delta pressure for this breath
        to total delta pressure due to flow limitation, and truncate
        to 16 cmH.sub.2O.
    ELSE
        Reduce total delta pressure due to flow limitation
        with a time constant of 10 minutes.
    END
    Calculate mean snore for breath.
    Calculate snore threshold.
    IF mean snore exceeds said threshold:
        set delta pressure due to snore for this breath to 3
        cmH.sub.2O times (mean snore for this breath--threshold).
        Add delta pressure due to snore for this breath to
        total delta pressure due to snore, and truncate to 16
        cmH.sub.2O.
    ELSE
        Reduce total delta pressure due to snore with a time
        constant of 10 minutes.
    END
    Set CPAP pressure to 4 cmH.sub.2O plus total delta
    pressure due to apnea plus total delta pressure due to snore
    plus total delta pressure due to flow limitation, and truncate
    to 20 cmH.sub.2O.
    Clear start of breath flag.
END
END

```

[0080] In the above implementation, apneas can only cause the CPAP pressure to rise as far as 10 cmH.sub.2O, but subsequently, indicators of partial obstruction can increase the CPAP pressure to 20 cmH.sub.2O, which is sufficient to treat the vast majority of subjects.

[0081] The procedure "Adjust snore for machine noise" is described by the following pseudocode

```

Machine noise=K1*mask pressure+K2*mask pressure
squared+K3*mask flow+K4*time derivative of mask flow+K5*time
derivative of mask pressure.
Adjusted snore signal=raw snore signal-machine
noise.
    where the constants K1 to K5 are determined
    empirically for any particular physical embodiment, and for a
    particular machine may be zero. In other embodiments, blower
    fan speed measured with a tachometer or pressure at the blower
    may be used instead of mask pressure.

```

[0082] The procedure "Calculate flow limitation index" is described by the following pseudocode:

```

Identify the inspiratory portion of the preceding
breath
Note the duration of inspiration.
Calculate the mean inspiratory airflow.

```

[0083] For each sample point over said inspiratory portion, calculate a normalized inspiratory airflow by dividing the inspiratory airflow by the mean inspiratory airflow.

[0084] Identify a mid-portion consisting of those sample points between 25% and 75% of the duration of inspiration.

[0085] Calculate the flow limitation index as the RMS deviation over said mid-portion of (normalized inspiratory airflow-1)

[0086] The logic of the above algorithm is as follows: partial upper airway obstruction in untreated or partially treated Obstructive Sleep Apnea syndrome, and the related Upper Airway Resistance syndrome, leads to mid-inspiratory flow limitation, as shown in FIG. 6, which shows typical inspiratory waveforms respectively for normal and partially obstructed breaths after scaling (normalizing) to equal mean amplitude and duration.

[0087] For a totally flow-limited breath, the flow amplitude vs. time curve would be a square wave and the RMS deviation would be zero. For a normal breath, the RMS deviation is approximately 0.2 units, and this deviation decreases as the flow limitation becomes more severe.

[0088] In some patients, it is not possible to prevent all upper airway obstruction, even at maximum pressure. In addition, there is a trade-off between the possible advantage of increasing the pressure in response to snoring and the disadvantage of increased side effects. This trade-off is implemented in procedure "calculate snore threshold" by looking up the snore threshold in the following table:

1	Pressure Threshold (cmH.sub.2O)	(snore units)	Description
<10	0.2	very soft	10-12 0.25 12-14 0.3 soft 14-16 0.4 16-18
0.6	moderate	>18 1.8	loud

[0089] For similar reasons, the procedure "calculate flow limitation threshold" sets the flow limitation threshold to a lower value corresponding to more severe flow limitation, if the pressure is already high or if there is a large leak:

```

IF mask leak is greater than 0.7 L/sec
set leak roll-off to 0.0
ELSE if mask leak is less than 0.3 L/sec
set leak roll-off to 1.0
ELSE
set leak roll-off to (0.7-mask leak)/0.4
END
Set pressure roll-off to (20-mask pressure)/16
Set flow limitation threshold to 0.15 times pressure
roll-off times leak roll-off

```

[0090] Some subjects will have occasional open airway apneas at sleep onset during stage 1 sleep and therefore at low pressure, and the above algorithm will incorrectly increase CPAP pressure in response to these events. However, such apneas are not usually repetitive, because the subject quickly becomes more deeply asleep where such events do not occur, and furthermore, the false pressure increments become smaller with repeated events. Once the subject reaches deeper sleep, any such falsely increased pressure will diminish. However, it is still advantageous to avoid falsely or needlessly increasing pressure in response to such sleep onset open airway apneas.

[0091] As previously discussed, one prior art method for avoiding unnecessary increases in pressure in response to open airway apneas is to determine the conductance of the airway during an apnea using the forced oscillation method, and only increase mask pressure if the conductance is less than a threshold. However, if the nasal airway is narrow or if the subject has lung disease, the airway conductance may be low even in the presence of an open airway and the forced oscillation method may still falsely increase pressure in response to open airway apneas. Conversely, the combination of the forced oscillation method with embodiments of the present invention has the added advantage that in most cases open airway apneas are correctly detected by the ‘forced oscillation method’, but in those cases where the forced oscillation method falsely reports a closed airway, the mask pressure will not increase above 10 cmH.sub.2O, thus preventing run-away increases in pressure. This is demonstrated in a third embodiment using the following pseudo-code:

```

Set apnea duration to zero
Clear “start of breath” flag
REPEAT every {fraction (1/50)} of a second
Sample mask pressure (in cmH2O), mask airflow (in
L/sec), and snore (1 unit corresponds loosely to a typical
snore).
Calculate mask leak as mask airflow low pass
filtered with a time constant of 10 seconds.
Adjust snore signal for machine noise.
Check for presence and duration of any apnea.
IF apnea in progress:
measure conductance of airway using forced oscillation
method.
END
Check for start of breath.
IF start of breath flag set:
IF apnea duration greater than 10 seconds AND
current CPAP pressure less than 10 cmH.sub.2O AND airway
conductance measured using forced oscillation method is less
than 0.05 cmH.sub.2O/L/sec:
Set delta pressure for this apnea to (10--current
CPAP pressure)/6 times 8 cmH.sub.2O per minute of apnea
duration.

```

-continued

```

Add delta pressure for this apnea to total delta
pressure due to apnea, and truncate to 16 cmH.sub.90
Reset apnea duration to zero.
ELSE
Reduce total delta pressure due to apnea with a time
constant of 20 minutes.
END
Calculate flow limitation index.
Calculate flow limitation threshold.
IF flow limitation index is less than said
threshold:
Set flow limitation delta pressure for this breath
to 3 cmH.sub.2O times (threshold-flow limitation index).
Add flow limitation delta pressure for this breath
to total delta pressure due to flow limitation, and truncate
to 16 cmH.sub.2O.
ELSE
Reduce total delta pressure due to flow limitation
with a time constant of 10 minutes.
END
Calculate mean snore for breath.
Calculate snore threshold.
IF mean snore exceeds said threshold:
set delta pressure due to snore for this breath to 3
cmH.sub.2O times (mean snore for this breath--threshold).
Add delta pressure due to snore for this breath to
total delta pressure due to snore, and truncate to 16
cmH.sub.2O.
ELSE
Reduce total delta pressure due to snore with a time
constant of 10 minutes.
END
Set CPAP pressure to 4 cmH.sub.2O plus total delta
pressure due to apnea plus total delta pressure due to snore
plus total delta pressure due to flow limitation, and truncate
to 20 cmH.sub.2O.
Clear start of breath flag.
END
END

```

[0092] The procedure, “measure airway conductance using the forced oscillation method” can be implemented using the following pseudocode:

```

Modulate airway pressure with an amplitude of 1
cmH.sub.2O peak to peak at 4 Hz.
Measure amplitude of airflow signal at 4 Hz.
Measure component of mask pressure signal at 4 Hz.
Set conductance equal to said airflow amplitude
divided by said mask pressure amplitude.
An alternate expression of the combination of an
embodiment of the invention and the forced oscillation method
is:
IF
(a) the current pressure is low AND (b) the
alternative method scores the airway as closed, THEN score the
airway as closed.
ELSE IF
(a) the current pressure is high AND (b) the
alternative method scores the airway as open, THEN score the
airway as open.
ELSE
score the apnea as of unknown type.

```

[0093] A further possible arrangement is to substitute the ‘cardiogenic method’ for determining airway patency for the ‘forced oscillation method’, also disclosed in European Publication No. 0 651 971 A1 (and U.S. Pat. No. 5,704,345).

[0094] More complex variants of CPAP therapy, such as bi-level CPAP therapy or therapy in which the mask pressure

is modulated within a breath, can also be monitored and/or controlled using the methods described herein.

[0095] Although the invention herein has been described with reference to particular embodiments, it is to be understood that these embodiments are merely illustrative of the principles and applications of the present invention. It is therefore to be understood that numerous modifications may be made to the illustrative embodiments and that other arrangements may be devised without departing from the spirit and scope of the present invention as defined by the appended claims.

1. A method for the administration of CPAP treatment pressure comprising the steps of: supplying breathable gas to a patient's airway at a treatment pressure; determining a measure of respiratory airflow; and determining the occurrence of an apnea from a reduction in the measure of respiratory airflow below a threshold, and, if having occurred, (i) determining the duration of the apnea; and (ii) increasing the treatment pressure by an amount which is an increasing function of the duration of the apnea, and a decreasing function of the treatment pressure immediately before the apnea.

2. The method of claim 1, whereby the increase in treatment pressure is substantially zero if the treatment pressure before the apnea exceeds a pressure threshold.

3. The method of claim 2, whereby the increase in pressure below the pressure threshold is an increasing function of the duration of the apnea, multiplied by the difference between the pressure threshold and the current treatment pressure.

4. The method of claim 3, whereby said increasing function of apnea duration is linear on apnea duration.

5. The method of claim 3, whereby said increasing function of apnea duration is zero for zero apnea duration, and exponentially approaches upper limit as apnea duration goes to infinity.

6. The method of claim 2, in which the pressure threshold is substantially 10 cmH₂O.

7. The method of claim 1, whereby the occurrence of an apnea is determined by the steps of: calculating the RMS respiratory airflow over a short time interval; calculating the RMS respiratory airflow over a longer time interval; and declaring an apnea if the RMS respiratory airflow over the short time interval is less than a predetermined fraction of the RMS respiratory airflow over longer time interval.

8. The method of claim 1, comprising the further step of reducing the treatment pressure toward an initial treatment pressure in the absence of a further apnea.

9. The method of claim 1, comprising the further steps of: in the absence of an apnea, determining the presence of partial obstruction; and if present, increasing the treatment pressure.

10. The method of claim 9, in which the presence of partial obstruction is determined from the shape of the patient's inspiratory flow vs time curve.

11. The method of claim 9, in which the presence of partial obstruction is determined from the presence of snoring.

12. The method of claim 9, in which the presence of partial obstruction is determined from both the shape of the patient's inspiratory flow vs time curve, and the presence of snoring.

13. The method of claim 1, comprising the further steps of: if an apnea is occurring, determining whether the patient's airway is patent during the apnea; and if the airway is patent, setting the increase in treatment pressure to zero.

14. The method of claim 13, in which the patency of the airway is determined by the presence of a cardiogenic component in the respiratory airflow.

15. The method of claim 13, in which the patency of the airway is determined by the steps of: modulating the treatment pressure at a known frequency; measuring the component of the respiratory airflow at said modulation frequency; calculating the conductance of the airway as the ratio of the amplitude of said component of the respiratory airflow to the amplitude of the mask pressure modulation; and determining that the airway is patent if the conductance exceeds a conductance threshold.

16. A CPAP treatment apparatus comprising: a controllable flow generator operable to provide breathable gas at a pressure elevated above atmospheric; a gas delivery tube coupled to the flow generator; a patient mask coupled to the tube to receive said breathable gas from the flow generator and to provide said gas, at a desired treatment pressure, to a patient's airway; a controller operable to receive an input signals and to control operation of said flow generator and hence the treatment pressure; and sensor means located to sense patient respiratory airflow and generate a signal input to the controller from which patient respiratory airflow is determined; and wherein said controller is operable to determine the occurrence of an apnea from a reduction in said respiratory airflow below threshold, and if having occurred, to determine the duration of said apnea and cause said flow generator to increase CPAP treatment pressure by an amount which is an increasing function of said apnea duration, and a decreasing function of the treatment pressure immediately prior to said apnea.

17. A CPAP treatment apparatus comprising: a controllable flow generator operable to produce breathable gas to be provided to a patient at a treatment pressure elevated above atmosphere; and a controllable operable to receive input signals representing patient respiratory airflow, and to control operation of said flow generator and hence the treatment pressure; and wherein said controller is operable to determine the occurrence of an apnea from a reduction in said respiratory airflow below the threshold, and, if having occurred, to determine the duration of said apnea and to cause said flow generator to increase CPAP treatment pressure by an amount that is an increasing function of said apnea duration, and a decreasing function of the treatment pressure immediately prior to said apnea.

* * * * *

专利名称(译)	在呼吸暂停的情况下施用CPAP治疗压力		
公开(公告)号	US20140166014A1	公开(公告)日	2014-06-19
申请号	US14/187919	申请日	2014-02-24
[标]申请(专利权)人(译)	雷斯梅德有限公司		
申请(专利权)人(译)	瑞思迈有限公司		
当前申请(专利权)人(译)	瑞思迈有限公司		
[标]发明人	BERTHON JONES MICHAEL FARRUGIA STEVEN PAUL		
发明人	BERTHON-JONES, MICHAEL FARRUGIA, STEVEN PAUL		
IPC分类号	A61M16/00 A61M16/08 A61M16/06 A61B5/00 A61B5/0205		
CPC分类号	A61M16/0069 A61B5/0205 A61B5/4818 A61M16/0875 A61M16/0003 A61M16/0051 A61M16/06 A61B5/4836 A61M16/00 A61M16/024 A61M2016/0036		
优先权	1997PP0269 1997-11-07 AU		
其他公开文献	US9526855		
外部链接	Espacenet USPTO		

摘要(译)

公开了CPAP治疗装置，其具有可控制的流量发生器（34,38,40），其可操作以通过连接到具有与a连接的面罩（30）的输送管（32）在高于大气压的治疗压力下产生可呼吸气体。病人的呼吸道。传感器（44,50,56,58）产生代表患者呼吸流量的信号，该信号被提供给控制器（54,62,64）。控制器（54，压力。在一种优选形式中，如果呼吸暂停前的治疗压力超过压力阈值，则压力增加为零。低于压力阈值，压力增加是呼吸暂停持续时间乘以的增加函数。压力阈值和当前治疗压力之间的差异。

