



US009717424B2

(12) **United States Patent**
Kulach

(10) **Patent No.:** **US 9,717,424 B2**
(45) **Date of Patent:** **Aug. 1, 2017**

(54) **SYSTEM AND METHOD FOR GENERATING
A PPG SIGNAL**

(71) Applicant: **Garmin Switzerland GmbH,**
Schaffhausen (CH)

(72) Inventor: **Christopher J. Kulach,** Calgary (CA)

(73) Assignee: **Garmin Switzerland GmbH** (CH)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

(21) Appl. No.: **15/296,938**

(22) Filed: **Oct. 18, 2016**

(65) **Prior Publication Data**

US 2017/0105638 A1 Apr. 20, 2017

Related U.S. Application Data

(60) Provisional application No. 62/243,447, filed on Oct.
19, 2015.

(51) **Int. Cl.**
A61B 5/02 (2006.01)
A61B 5/024 (2006.01)

(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/02416** (2013.01); **A61B 5/1112**
(2013.01); **A61B 5/1118** (2013.01); **A61B**
5/7278 (2013.01); **A61B 5/7285** (2013.01)

(58) **Field of Classification Search**

None

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,258,719 A * 3/1981 Lewyn A61B 5/02416
307/650

5,277,181 A * 1/1994 Mendelson A61B 5/14551
356/41

(Continued)

FOREIGN PATENT DOCUMENTS

EP 0319160 A1 * 6/1989
WO WO2006/067690 A2 6/2006

(Continued)

OTHER PUBLICATIONS

U.S. Appl. No. 15/296,956, filed Oct. 18, 2016.


Primary Examiner — Brian T Gedeon

(74) *Attorney, Agent, or Firm* — Samuel M. Korte; Max
M. Ali

(57) **ABSTRACT**

Characterization of a fitness monitor based on its operation enables a processor to account for variations in device operating modes and biometric characteristics of the user. The fitness monitor includes an emitter (e.g., LED) for transmitting light toward skin of the user, a receiver (e.g., photodiode) for receiving a reflection of the transmitted light, a photometric front end for generating a photoplethysmogram (PPG) signal based on the received reflection, and a processor configured to select an intensity level for the emitter based on a comparison of a determined component of the PPG signal and a reference value. The reference value, which may characterize the fitness monitor based on a determined variability or range of the PPG signal, may be utilized by the processor to improve or maintain the signal quality of the PPG signal to enable determination of a cardiac component and/or reduction of power consumption by the fitness device.

20 Claims, 8 Drawing Sheets

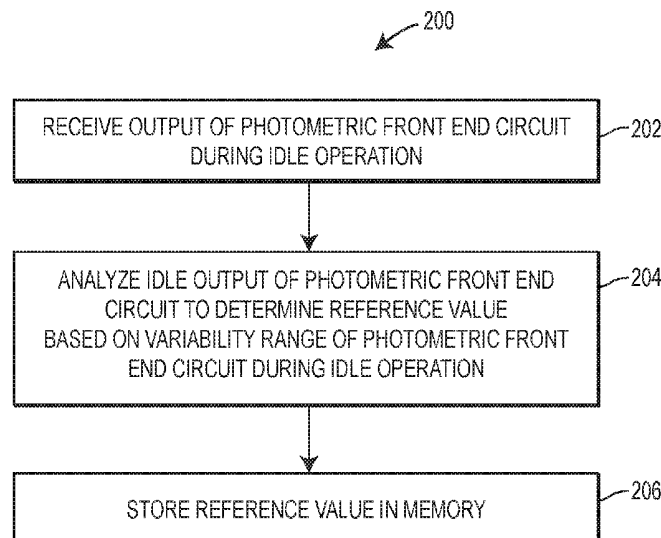

US 9,717,424 B2

Page 2

(51) **Int. Cl.**
A61B 5/11 (2006.01)
A61B 5/00 (2006.01)

(56) References Cited

U.S. PATENT DOCUMENTS


6,178,343 B1 1/2001 Bindzus 600/323
6,702,752 B2 3/2004 Dekker 600/484
6,997,879 B1 2/2006 Turcott 600/507
7,035,679 B2 4/2006 Addison 600/323
7,169,110 B2* 1/2007 Lee A61B 5/14551
600/481
7,215,987 B1* 5/2007 Sterling A61B 5/14551
600/322
7,336,982 B2 2/2008 Yoo 600/323
7,470,234 B1 12/2008 Elhag 600/485
7,625,344 B1 12/2009 Brady 600/485
7,729,748 B2 6/2010 Florian 600/476
7,794,406 B2* 9/2010 Reisfeld A61B 5/0402
600/479
7,867,142 B2 1/2011 Kim 482/8
8,109,874 B2 2/2012 Kong 600/300
8,251,903 B2 8/2012 LeBoeuf et al. 600/309
8,260,405 B2 9/2012 Aarts 600/509
8,460,199 B2 6/2013 Rulkov 600/503
8,463,347 B2 6/2013 Watson 600/324
8,509,882 B2 8/2013 Albert 600/509
8,512,242 B2 8/2013 LeBoeuf et al. 600/309
8,554,297 B2* 10/2013 Moon A61B 5/746
600/310
8,591,411 B2 11/2013 Banet 600/300
8,647,270 B2 2/2014 LeBoeuf et al. 600/301
8,652,040 B2 2/2014 LeBoeuf et al. 600/301
8,670,123 B2 3/2014 Schleipen 356/445
8,700,111 B2 4/2014 LeBoeuf et al. 600/310
8,788,002 B2 7/2014 LeBoeuf et al. 600/310
8,827,906 B2 9/2014 Yuen 600/301
8,886,269 B2 11/2014 LeBoeuf et al. 600/310
8,888,701 B2 11/2014 LeBoeuf et al. 600/300
8,923,941 B2 12/2014 LeBoeuf et al. 600/310
8,929,965 B2 1/2015 LeBoeuf et al. 600/310
8,929,966 B2 1/2015 LeBoeuf et al. 600/310
8,934,952 B2 1/2015 LeBoeuf et al. 600/310
8,942,776 B2 1/2015 LeBoeuf et al. 600/310
8,945,017 B2 2/2015 Venkatraman 600/500


8,954,135 B2 2/2015 Yuen 600/476
8,974,396 B1* 3/2015 Brady A61B 5/02416
600/508
8,989,830 B2 3/2015 LeBoeuf et al. 600/310
8,998,815 B2 4/2015 Venkatraman 600/300
9,005,129 B2 4/2015 Venkatraman 600/300
9,014,790 B2* 4/2015 Richards A61B 5/02438
600/473
9,039,614 B2 5/2015 Yuen
9,044,171 B2 6/2015 Venkatraman 342/357.74
9,044,180 B2 6/2015 LeBoeuf et al. 600/310
9,131,312 B2 9/2015 LeBoeuf et al.
9,289,135 B2 3/2016 LeBoeuf et al. 600/310
9,289,175 B2 3/2016 LeBoeuf et al. 600/310
9,301,696 B2 4/2016 LeBoeuf et al. 600/310
9,307,917 B2 4/2016 Hong et al.
9,314,167 B2 4/2016 LeBoeuf et al. 600/310
9,538,921 B2 1/2017 LeBoeuf et al.
2005/0143665 A1 6/2005 Huiku 600/500
2009/0048526 A1 2/2009 Aarts 600/508
2009/0105556 A1 4/2009 Fricke 600/301
2009/0259116 A1* 10/2009 Wasserman A61B 5/14551
600/323
2010/0113948 A1 5/2010 Yang 600/500
2011/0054277 A1* 3/2011 Pinter A61B 5/0205
600/310
2011/0082355 A1 4/2011 Eisen 600/324
2012/0197137 A1 8/2012 Jeanne 600/479
2013/0231926 A1 9/2013 Gigi 704/207
2013/0261415 A1* 10/2013 Ashe A61B 5/14552
600/324
2014/0213858 A1 7/2014 Presura 600/301
2014/0276099 A1 9/2014 Kirenko 600/476
2014/0288436 A1 9/2014 Venkatraman 600/479
2014/0316305 A1 10/2014 Venkatraman 600/595
2015/0173628 A1 6/2015 Yuen
2015/0196256 A1 7/2015 Venkatraman
2016/0235313 A1* 8/2016 Sharma A61B 5/02427

FOREIGN PATENT DOCUMENTS

WO WO2011/051888 A2 5/2011
WO WO2013/042070 A1 3/2013
WO WO2013/124750 A1 8/2013
WO WO2013/190423 A1 12/2013

* cited by examiner

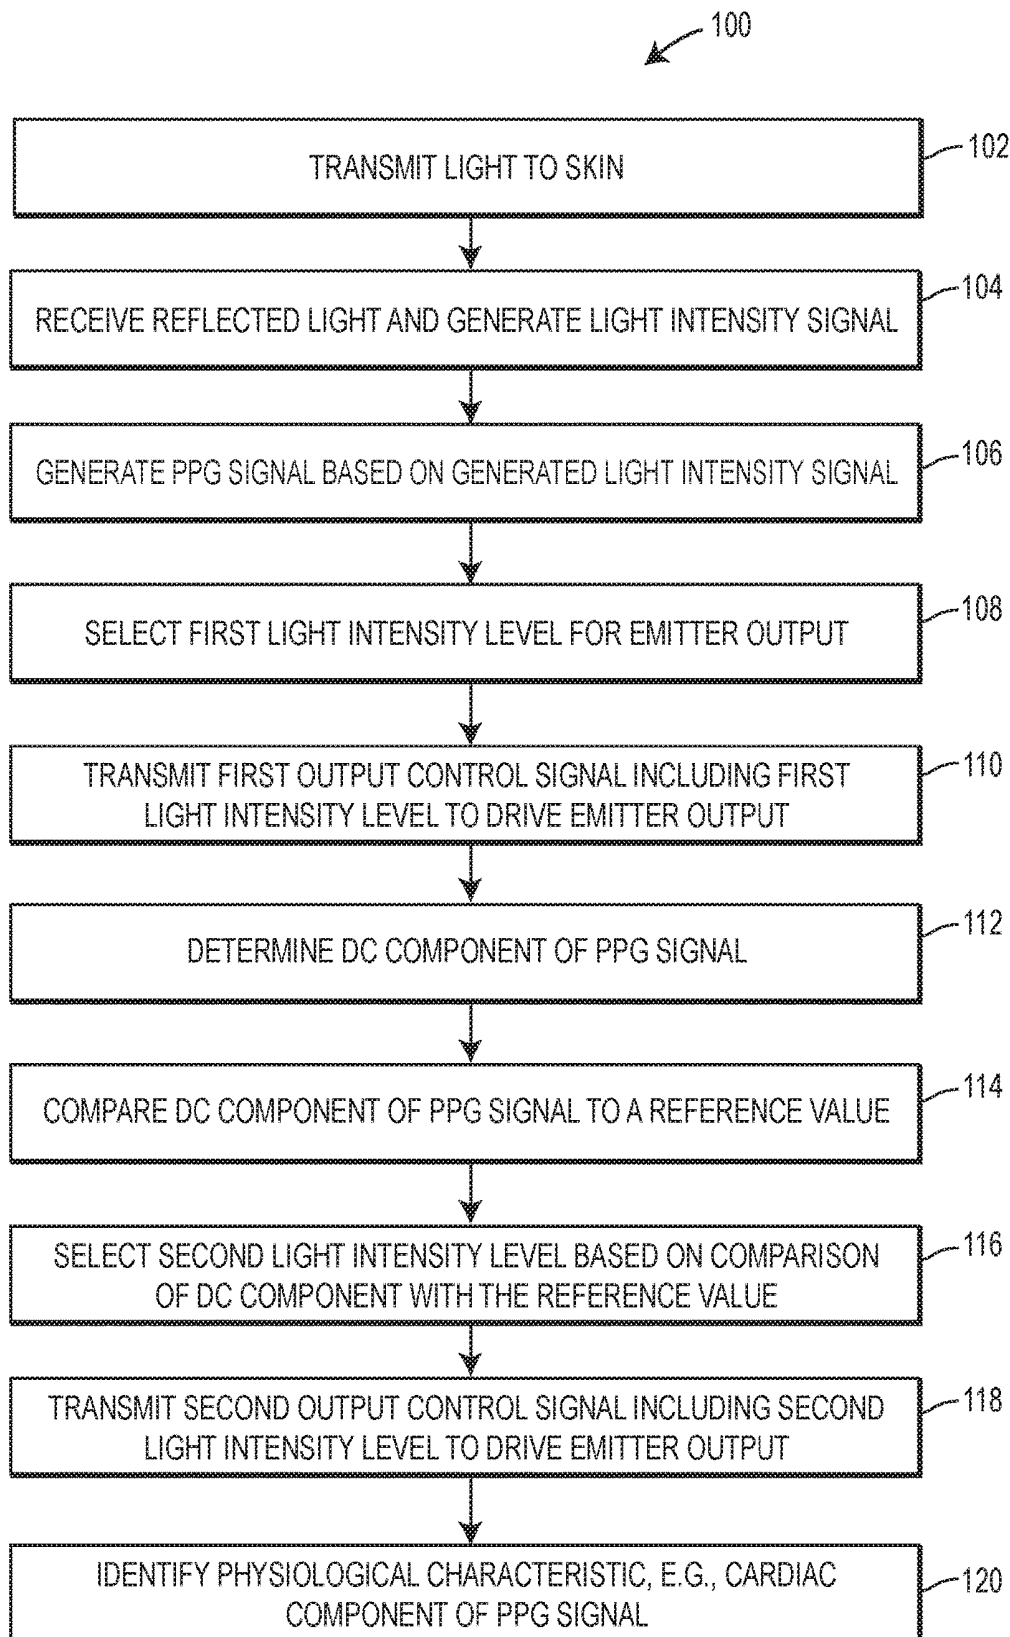**FIG. 1**

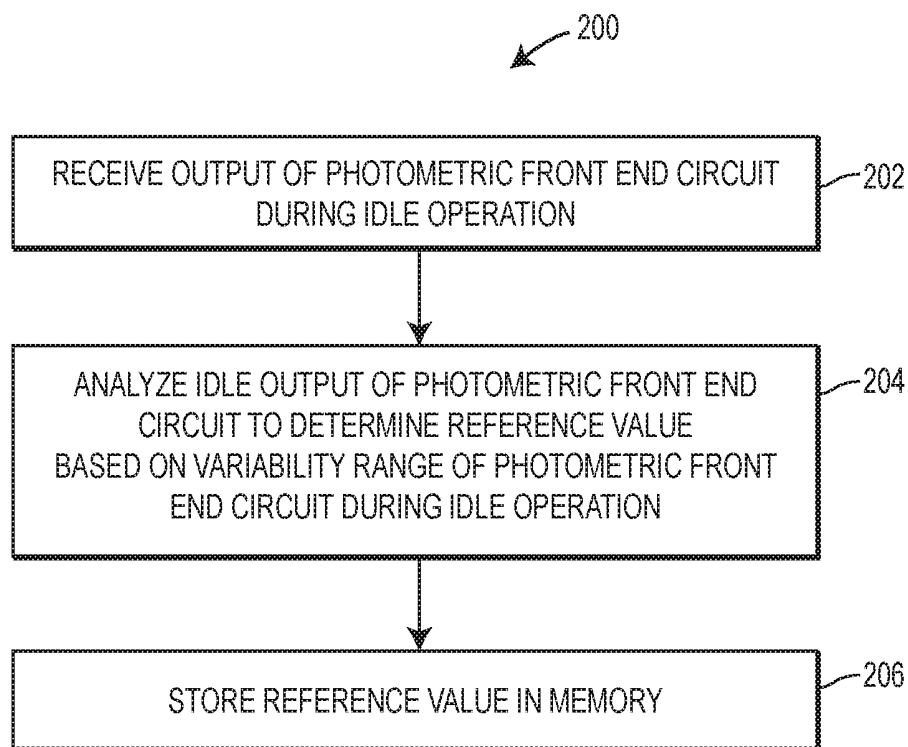**FIG. 2**

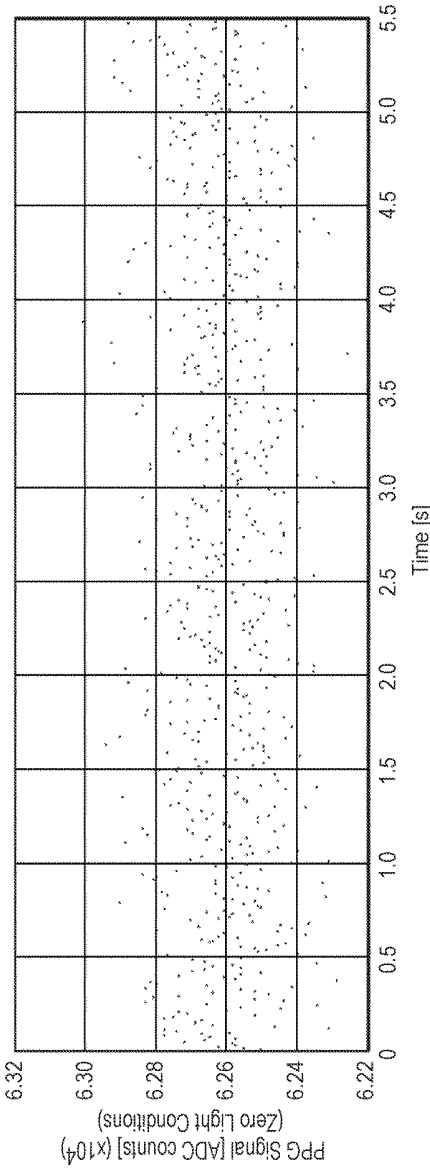


FIG. 3

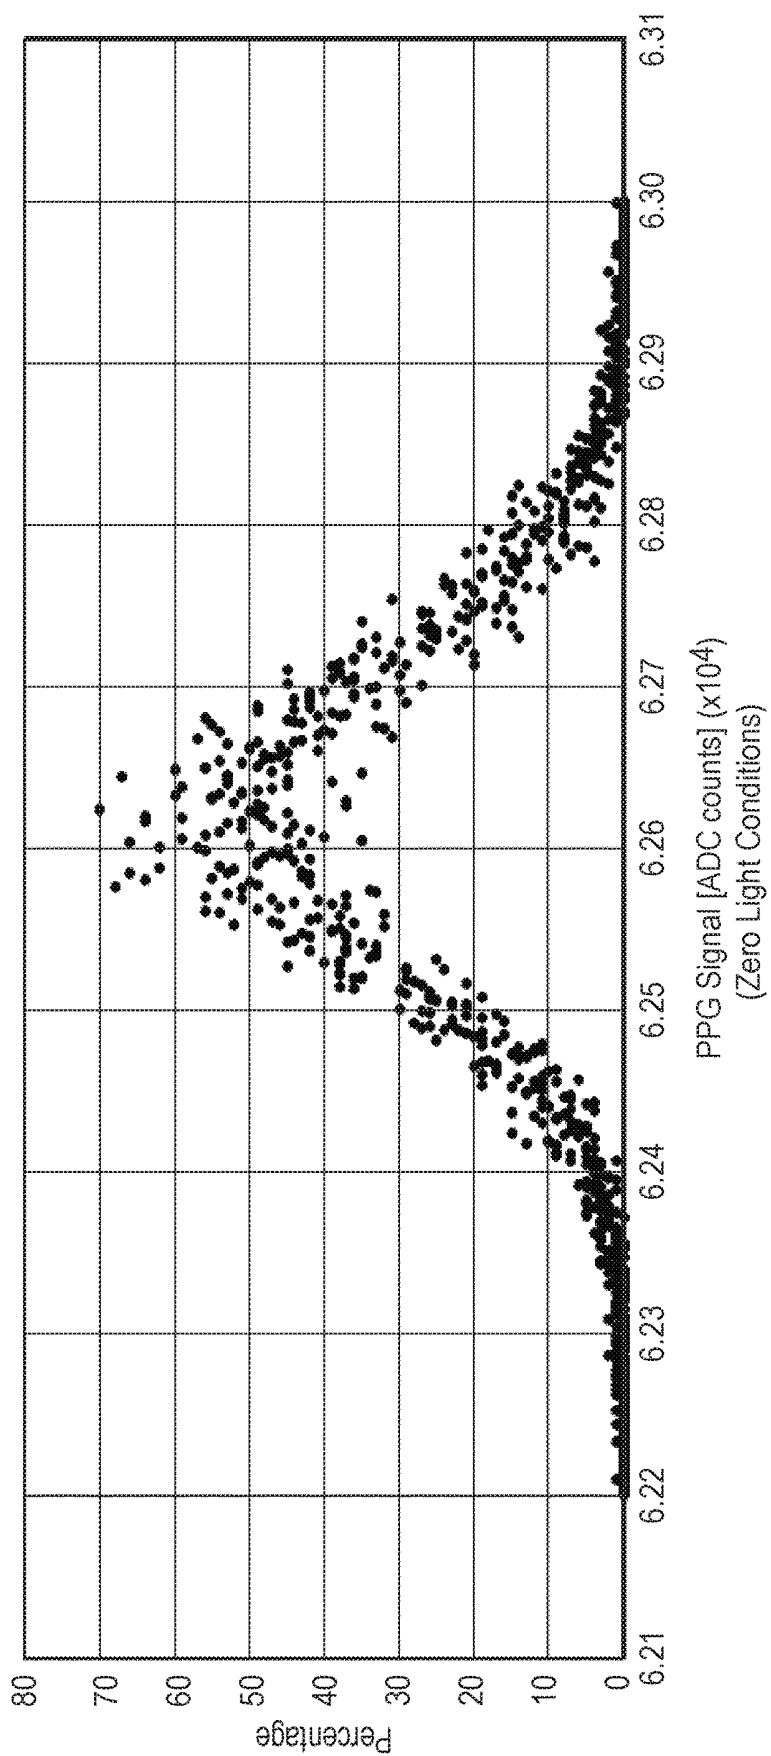


FIG. 4

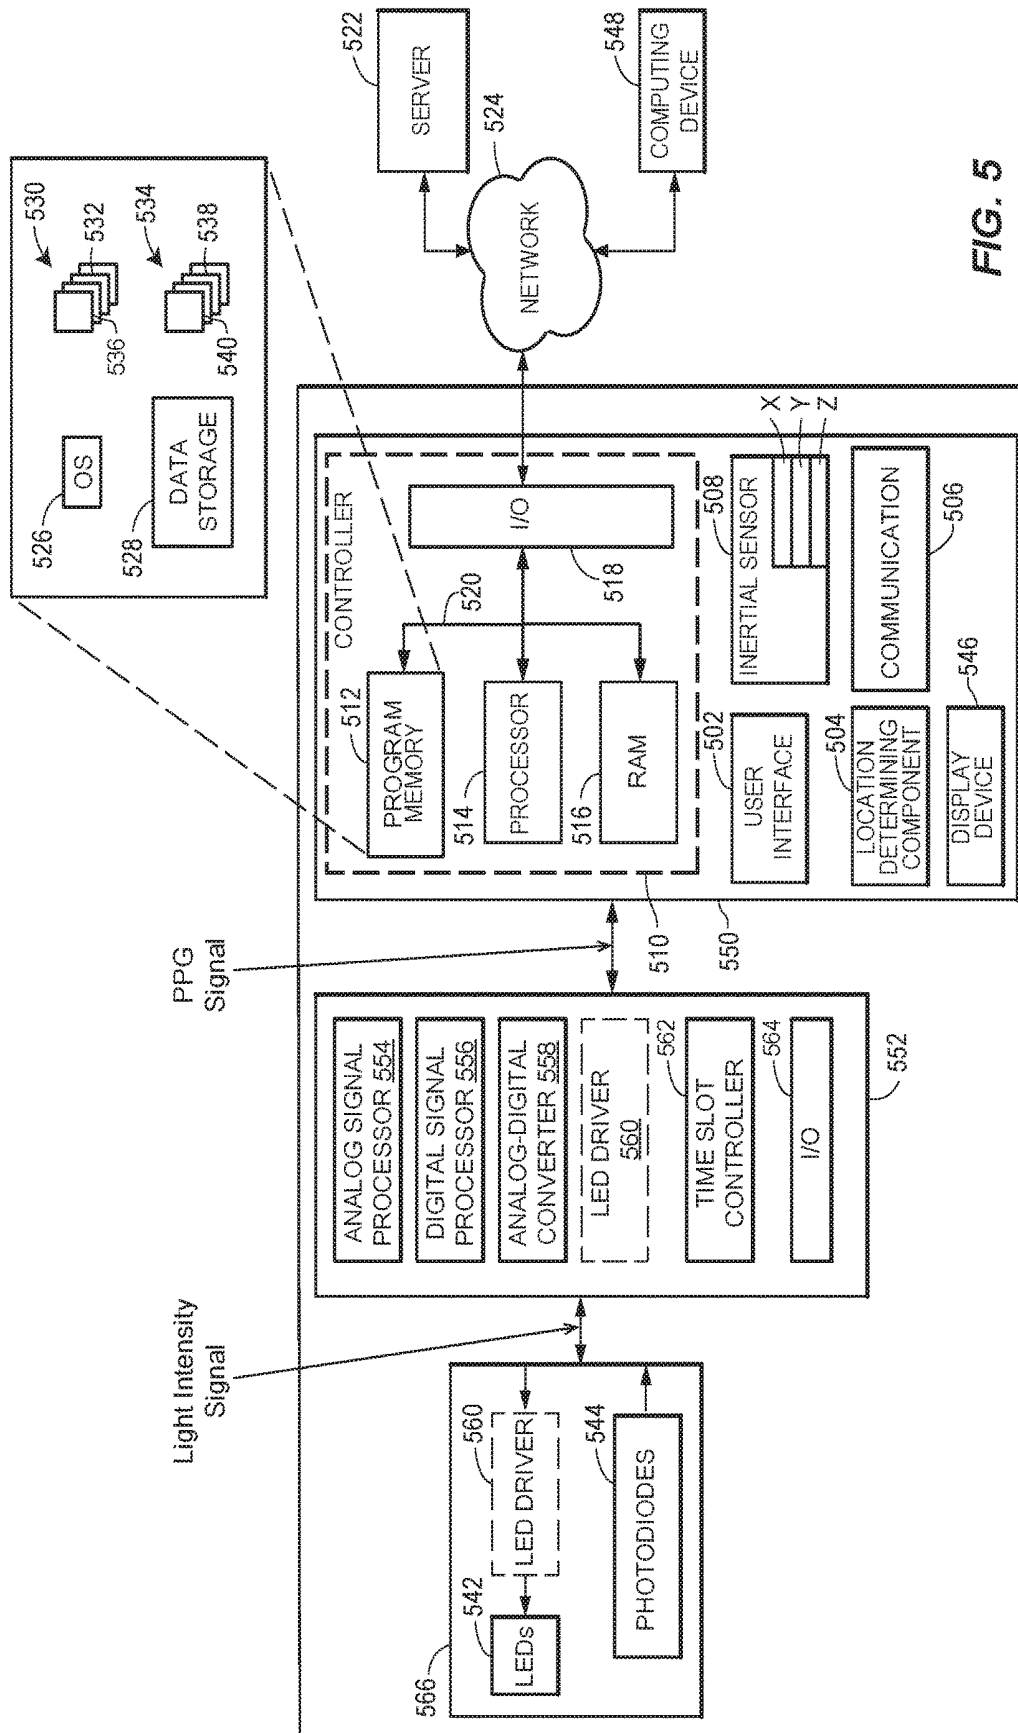
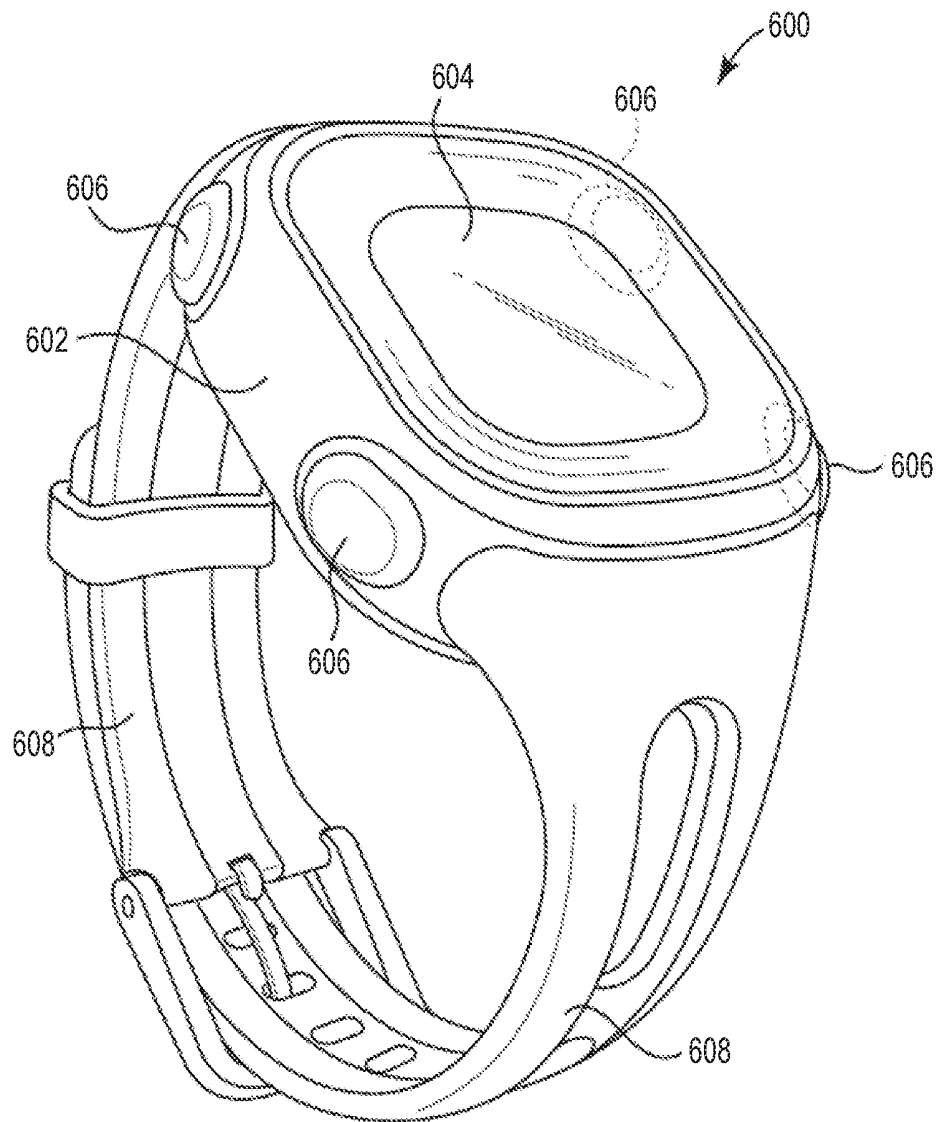


FIG. 5

**FIG. 6A**

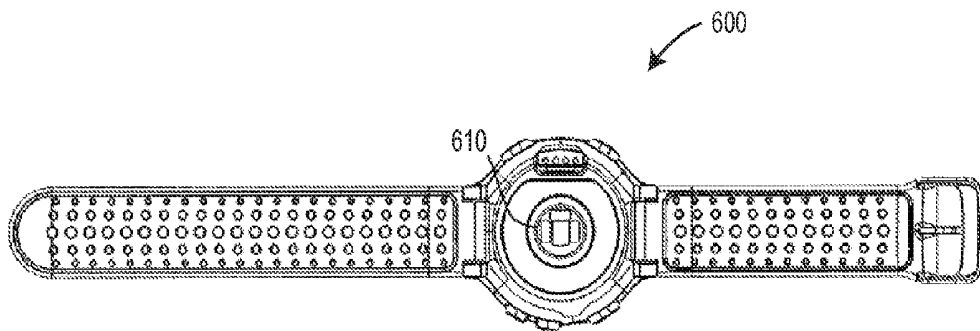


FIG. 6B

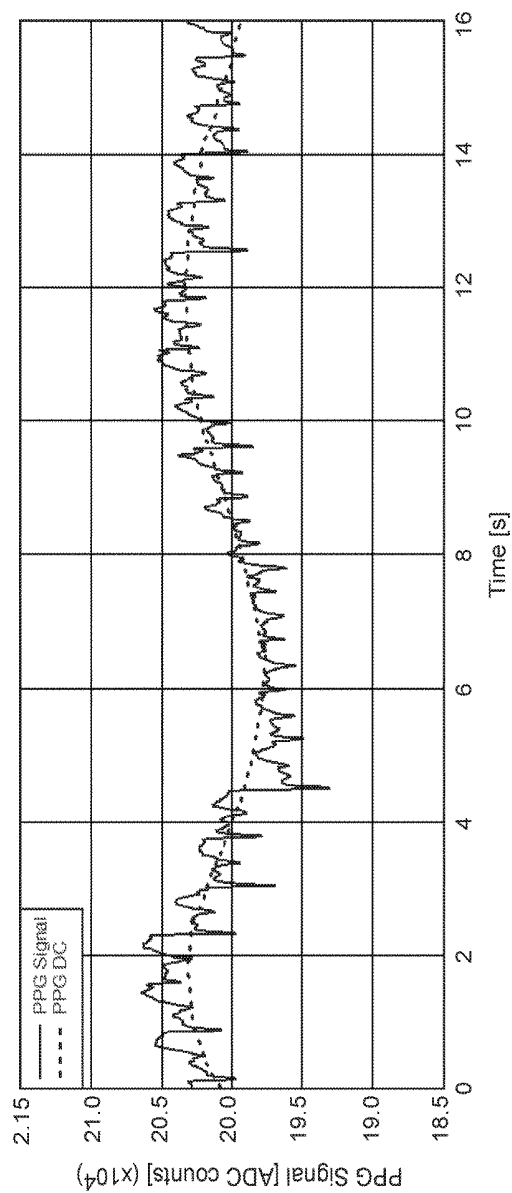


FIG. 7

1

SYSTEM AND METHOD FOR GENERATING A PPG SIGNAL

CROSS-REFERENCE TO RELATED APPLICATIONS

This patent application claims priority benefit under 35 U.S.C. §119(e), with regard to all common subject matter, of U.S. Provisional Application Ser. No. 62/243,447, filed Oct. 19, 2015, titled “PPG SIGNAL ANALYSIS,” which is hereby incorporated by reference in its entirety. This application is related to simultaneously filed U.S. patent application Ser. No. 15/296,956, entitled “HEART RATE MONITOR WITH TIME-VARYING LINEAR FILTERING”, the entire contents of which is expressly incorporated herein.

BACKGROUND

A photoplethysmogram (PPG) signal is commonly utilized to monitor physiological metrics of an individual, such as cardiac information, for example, a heartbeat signal or a heart-rate. Devices that generate a PPG signal using optical techniques typically include an emitter configured to output light toward skin of the user and a receiver, which may include a photodiode and electrical circuitry, configured to generate a light intensity signal based on a light reflections received by the photodiode and using the electrical circuitry to generate a PPG signal based on the light intensity signal. The PPG signal typically includes a cardiac component, a motion component, a respiratory component and other components may be included as well.

To effectively monitor the physiological characteristic, several factors that may adversely affect the measurement of the physiological characteristic are generally considered. For example, a PPG signal quality for a desired cardiac component of the PPG signal is sensitive to variations in operating parameters of the device and biometric characteristics of the user (e.g., skin tone or complexion, skin density, body fat of the user, moisture level of the user's skin, hair density or color, etc.) at a location on the user's body (e.g., the user's wrist) against which the monitoring device is positioned to output light and receive reflections (e.g., output to and received from the skin on the top of the user's wrist). Operating parameters of the device may include a particular gain setting, number of channels for one or more photodiodes, a number of pulses of light output by one or more emitters (LEDs), a width of each pulse output by the one or more emitters (LEDs), a voltage of the one or more emitters (LEDs), or a current of the one or more emitters (LEDs). These variations may rapidly degrade the signal-to-noise ratio (SNR) for the cardiac component of the PPG signal and adversely impact the accuracy of measurements. Additionally, the components utilized to perform the measurements have an inherent range of operating characteristics that may affect the accuracy of the monitoring device.

Known techniques for accounting for certain variations of amongst users of fitness monitors includes characterizing the user by determining mathematical relationships for each user while the device is in use. For example, a fitness monitor may operate in a first mode to measure a heart rate by using light pulses of constant intensity and a characterization mode to determine a relationship between varying intensity levels of light and collected data points. For instance, the characterization mode may include varying the intensity of a light source, measuring light reflected to a photodiode and determining a relationship between the collected data points and the varying levels of light. It is

2

therefore desired to provide a monitoring device, for example, a fitness monitor device, that characterizes the fitness monitor instead of characterizing the user while the device is in use. Characterization of a fitness monitor based on its operation enables the fitness monitor to account for variations in operating parameters of the device and biometric characteristics of the user without utilizing a characterization mode.

SUMMARY

In one aspect of the invention, a fitness monitor attached to a user for monitoring a cardiac signal of the user includes an emitter configured to output light toward skin of the user, an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels, a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection, a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal, the PPG signal including a cardiac signal, and a memory device configured to store a reference value based on the variability of the PPG signal output from the photometric front end during idle operation. The fitness monitor may further include a processor communicatively coupled to the emitter, the emitter driver, the receiver, photometric front end, and the memory device, wherein the processor is configured to select a first intensity level for the emitter to output light, transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level, determine a DC component of the PPG signal, select a second intensity level based on a comparison of the determined DC component of the PPG signal with the stored reference value, transmit a second output control signal including the selected second intensity level to the emitter driver causing the emitter to output light at the selected second intensity level, and identify the cardiac component in the PPG signal.

Another aspect of the invention is directed to a fitness monitor for monitoring a cardiac signal of a user, wherein the fitness monitor includes an emitter configured to output light toward skin of the user, an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels, a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection, a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal, the PPG signal including a cardiac signal, a reference value based on the variability of the PPG signal output from the photometric front end when the fitness monitor is not proximate to the skin of the user and a memory device configured to store the reference value. The fitness monitor further includes a processor communicatively coupled to the emitter, the receiver, photometric front end and the memory device, the processor configured to select a first intensity level for the emitter to output light, transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level, determine a DC component of the PPG signal, select a second intensity level based on a comparison of the determined DC component of the PPG signal with the stored reference value, transmit a second output control signal including the selected second intensity level to the emitter driver causing

the emitter to output light at the selected second intensity level, and identify the cardiac component in the PPG signal.

In a further aspect of the invention, a fitness monitor for monitoring a cardiac signal of a user includes an emitter configured to output light toward skin of the user, an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels, a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection, a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal and representing the cardiac signal, and a tangible non-transitory computer-readable medium storing instructions and a reference value based on the variability of the PPG signal output from the photometric front end during idle operation, wherein the instructions, when executed by one or more processors, cause the fitness monitor to select a first intensity level for the emitter to output light, transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level, determine a DC component of the PPG signal, select a second intensity level based on a comparison of the determined DC component of the PPG signal with the stored reference value, transmit a second output control signal including the selected second intensity level to the emitter driver causing the emitter to output light at the selected second intensity level, and identify the cardiac component in the PPG signal.

Many of the inventive principles and much of the inventive functionality may be implemented with or in software programs or instructions and integrated circuits (ICs) such as application specific ICs. It is expected that one of ordinary skill, notwithstanding possibly significant effort and many design choices motivated by, for example, available time, current technology, and economic considerations, when guided by the concepts and principles disclosed herein will be readily capable of generating such software instructions and programs and ICs with minimal experimentation. Therefore, in the interest of brevity and minimization of any risk of obscuring the principles and concepts in accordance to the present invention, further discussion of such software and ICs, if any, is limited to the essentials with respect to the principles and concepts of the described embodiments.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 depicts an exemplary process for operating a fitness monitor for monitoring a physiological characteristic of a user as described herein;

FIG. 2 depicts a portion of an exemplary process for determining the reference value used for the comparison with the determined DC component of the PPG signal as described herein;

FIG. 3 depicts an example dot-plot graph depicting received signals of the fitness monitor during the idle state as described herein;

FIG. 4 depicts a Gaussian curve of the data of FIG. 3 relating to the determination of the reference value as described herein;

FIG. 5 is a block diagram of an example embodiment of a fitness monitor for monitoring a physiological characteristic of a user as described herein;

FIGS. 6A and 6B are illustrations depicting one embodiment of the fitness monitor for monitoring one or more physiological and/or performance characteristics of a user as described herein; and

FIG. 7 is a graph of a PPG signal generated by a photometric front end circuit of a fitness monitor while the fitness monitor is worn by a user.

DETAILED DESCRIPTION

Aspects of the present invention enable the monitoring device, e.g., a fitness monitor, to generate a PPG signal having enhanced signal quality and/or reduced power consumption based on operation of the monitoring device during idle operation, such as when the monitoring device is not proximate to the skin of a user. Idle operation refers to the operation of the monitoring device in an environment that enables characterization of the monitoring device based on inherent operating characteristics of components implemented within a monitoring device used to measure physiological characteristics of an individual in one or more configurations or operating parameters of the monitor device. For example, characterization of the monitoring device may occur during idle operation, which may occur at a time the monitoring device is manufactured, when one or more components of the monitoring device are configured to operate in a predetermined configuration and the device is not worn by a user.

Characterization of the monitoring device prior to its use by a user may enable a processor of the monitoring device to dynamically account for variations in operating parameters of the device and biometric characteristics of the user without utilizing an operating mode that characterizes the user while the device is worn by the user, such as by outputting light in predetermined intensities and/or patterns to determine signal quality of a PPG signal generated based on reflections of the outputted light. The biometric characteristics of a user may include a skin tone or complexion of the user, the user's skin density, body fat of the user, moisture level of the user's skin, or the hair density or color of the user, at a location on the user's body against which the monitoring device is positioned to output light and receive reflections.

The monitoring device may include a receiver, which may include one or more photodiodes and a photometric front end, configured to receive a reflection of the transmitted light from the user's skin and generate a light intensity signal based on the received reflection. The light intensity signal may be an analog signal that is filtered, processed and converted into a digital PPG signal by the photometric front end of the receiver. In embodiments, the light intensity signal is processed and digitized into a PPG signal by a processor of the monitoring device directly or by controlling circuitry, such as the photometric front end.

A processor of the monitoring device controls the amount of light output by one or more emitters (e.g., LEDs) by selecting an intensity level for the emitters based on a comparison of a determined DC component of a PPG signal and a stored reference value. A selected intensity level may include one of more sample-configuration parameters including, for instance, peak pulse current, pulse duration, or number of pulses per sample. The processor may determine a DC component of a PPG signal, as illustrated in FIG. 7, provided by a photometric front end circuit by analyzing levels of the PPG signal over a period of time. In embodiments, the processor may determine the average of PPG signal levels over a period of time as the DC component of the PPG signal. The monitoring device may utilize the reference value based on the variability of the PPG signal, which is generated by an analog front end during an idle state of the monitoring device, to improve or maintain the

signal quality of the PPG signal enables determination of a cardiac component that may be used to determine an accurate heart rate for the user and/or reduce power consumption of the fitness device. The signal quality of the PPG signal may be associated with a noise power of the PPG signal and other signal-path components of the monitoring device.

FIG. 1 depicts a block diagram of an exemplary process 100 for improving the accuracy of and/or minimizing the power consumed by a monitoring device, a fitness monitor, for measuring a physiological characteristic of an individual. The fitness monitor includes one or more processors and transmits light toward the skin of an individual (block 102) to facilitate identification of a physiological characteristic within a generated photoplethysmogram (PPG) signal (block 120). The physiological characteristic may be a cardiac component of the PPG signal. An emitter and emitter driver are configured to transmit light having one of a variety of selectable intensity levels.

A receiver of the fitness monitor receives a reflection of the transmitted light and generates an analog light intensity signal based on the received light (block 104). Photometric front end circuitry receives the analog light intensity signal, filters the signal and generates a digital PPG signal based on the received light intensity signal (block 106). The PPG signal includes information associated with a physiological characteristic of the individual. For example, a cardiac component of the PPG signal may provide a user's heartbeat signal.

One or more processors of the fitness monitor are configured to select a first intensity level for the emitter to output light (block 108) and transmit a first output control signal to the emitter driver, to cause the emitter to output light at the selected first intensity level (block 110). The one or more processors determine a DC component of the PPG signal (block 112) and a second intensity level is selected (block 116) based on a comparison of the determined DC component with a reference value (block 114).

The one or more processors of the fitness monitor transmit a second output control signal including the selected second light intensity level to the emitter driver to cause the emitter to output light (block 118) at the selected second intensity level. In embodiments, the selected second light intensity level may cause a PPG signal having a DC component determined to be lower than desired, based on a comparison of the DC component with the stored reference value, to be increased to a level that enables determination of a cardiac component that may be used to determine an accurate heart rate for the user. Similarly, the selected second light intensity level may cause a PPG signal having a DC component determined to be greater than desired, based on a comparison of the DC component with the stored reference value, to be reduced to a level that enables determination of a cardiac component that may be used to determine an accurate heart rate for the user while reducing consumed power.

The one or more stored reference values characterize performance of the fitness monitor independent of its use by an individual. Rather, a reference value is determined for the fitness monitor based on at least one configuration of one or more components of the fitness monitor at a time when the fitness monitor is not proximate to the skin of a user. Subsequently, the processor may utilize the stored reference value to dynamically alter operation of the one or more components of the fitness monitor when the device is being used by a user (the fitness monitor is now proximate to the skin of the user) to acquire a PPG signal having adequate signal quality and/or reduced power consumption.

This dynamic configuration of one or more fitness monitor components accounts for variations in operating parameters of the device and biometric characteristics of the user without utilizing an operating mode that characterizes the user while the device is worn by the user. For example, a selected second light intensity level may cause a PPG signal having a DC component determined to be lower than desired due to selected operating parameters of the device and/or one or more biometric characteristics of a user to be increased to a level that enables determination of a cardiac component. Biometric characteristics that may require the light intensity level to be increased may include such as a darker skin tone or complexion of the user, high body fat of the user, increased moisture level of the user's skin, high hair density or dark hair color of the user at a location on the user's body against which the monitoring device is positioned to output light and receive reflections. The processor may determine that the light intensity level must be increased based on a comparison of the DC component with the stored reference value that characterized performance of the fitness monitor independent of its use by an individual.

FIG. 2 depicts a block diagram of an exemplary process 200 for determining the reference value used by the processor in the comparison with the determined DC component of the PPG signal, referred to at block 114 of FIG. 1. An exemplary PPG signal and DC component of the PPG signal is illustrated in FIG. 7. One or more reference values may be determined by the processor of the fitness monitor when the fitness monitor is not worn by or otherwise in use by a user (e.g., prior to the intended operation of the fitness monitor) in one or more configurations of the fitness monitor to characterize performance of the fitness monitor independent of its use by an individual.

In embodiments, the techniques disclosed herein for determining one or more reference values may be implemented after initial use by a user during any moment when the fitness monitor is not being worn by a user. For example, the reference value may be determined based on the PPG signal output by the photometric front end circuitry when the fitness monitor is not being worn by a user and has been placed on a table (for storage or charging of the fitness monitor). In embodiments, the one or more processors of the fitness monitor may utilize a signal from an inertial sensor and/or a received PPG signal to automatically determine that the device is not being worn by a user and then initiate determination of one or more reference values for storage in the memory device of the fitness monitor. In embodiments, the processor of the fitness device may account for any ambient light received by photodiodes of the fitness device when the device is not in a controlled environment having a known amount of light.

The processor of the fitness monitor may compare a stored reference value with a recently determined reference value to determine whether both reference values should be retained or whether only one of the reference values should continue to be stored. For example, the memory device of the fitness monitor may include a data table providing a reference value for a plurality of configurations of one or more components of the fitness monitor, each reference value determined at a time when the fitness monitor is not proximate to the skin of a user. For instance, the data table may provide the processor of the fitness device a reference value for particular configuration of operating parameters of the device (e.g., a particular gain setting, number of channels for one or more photodiodes, a number of pulses of light output by one or more emitters (LEDs), a width of each

pulse output by the one or more emitters (LEDs), a voltage of the one or more emitters (LEDs), a current of the one or more emitters (LEDs), etc.).

Determination of one or more reference values in an idle state or condition of the fitness monitor may occur at any moment when the fitness monitor is not being worn by a user. For example, the photodiodes of the fitness monitor may be shielded from light or the fitness monitor may be placed in a dark, light-absorbing room or calibration box before, shortly after, or during the manufacture of the fitness monitor. Alternately, the idle state of the photometric front end circuit may occur after initial use of the fitness monitor by the user at a time when the fitness monitor is not proximate to the skin of the user and is not receiving reflections of the light transmitted by the emitter, the reflections from which are modulated by the user's skin. In embodiments, the fitness monitor may receive reflected light originating from an emitter (e.g., LED) or other sources (e.g., ambient light) and the processor of the fitness monitor may determine the reference value based on the PPG signal output by the photometric front end circuit, provided that the fitness monitor is not worn by a user whose skin the received light passed through.

The one or more processors of the fitness monitor receive the PPG signal output by the photometric front end circuitry during idle operation (block 202), analyze the output of the photometric front end during the idle state to determine a reference value characterizing the fitness monitor based on a determined variability of the PPG signal provided by the photometric front end circuit (block 204), and store the determined reference value in a memory device of the fitness monitor (block 206). The predetermined reference value may be calculated when the one or more photodiodes of the receiver are not receiving reflections of light output by the one or more emitters (e.g., LEDs) or receiving only predictable reflections (for example, from surfaces that are not living tissue) to characterize fitness monitor based on the inherent range of operating characteristics of components utilized to perform the measurements that may affect the accuracy of the monitoring device. In the idle state, the PPG signal output provided by the photometric front end circuit is not in response to, based on, or associated with unpredictable modulation of reflected light originating from the emitter, and thus the output of the photometric front end circuit during the idle state may be considered as an inherent "noise" characteristic, e.g., noise floor or base-level, of the fitness monitor, including the photometric front end circuitry.

In embodiments, reference values may be determined by the processor when one or more components of the fitness monitor are configured to operate in one of a plurality of operating modes that are anticipated to be used when the fitness monitor may be worn and used by a user. For example, the processor of the fitness device may determine a reference value characterizing operation of the fitness device for each gain setting of a transimpedance amplifier (TIA) by collecting PPG signal output by the photometric front end circuitry during idle operation. Similarly, the processor of the fitness device may determine a reference value characterizing operation of the fitness device for varying number of channels (signal paths) between the photometric front end and one or more photodiodes by collecting PPG signal output by the photometric front end circuitry during idle operation. For example, two or more channels may be used to distribute charge from one or more photodiodes amongst the two or more channels to increase dynamic range. Alternatively, the processor of the fitness

device may determine a reference value characterizing operation of the fitness device based on varying number of pulses and/or width of pulses output by the LEDs by collecting PPG signal output by the photometric front end circuitry during idle operation. The processor of the fitness device may determine a reference value characterizing operation of the fitness device based on a varying voltage or current of the LEDs by collecting PPG signal output by the photometric front end circuitry during idle operation.

One or more reference values may be stored in memory device of the fitness device corresponding to each configuration of the fitness device. For example, reference values may be determined once for a plurality of fitness devices based on a shared hardware and/or software platform of a fitness device. A sample of one or more fitness devices representative of similar fitness devices may be utilized to determine the reference values for all of the fitness devices. For example, a reference value may be determined as representative of a plurality of fitness devices that share substantially the same hardware and/or software or that share a common component (e.g., a photometric front end circuit, an optical sensing module having one or more LEDs and one or more photodiodes, power supply, etc.). Alternatively, reference values may be independently determined for each fitness device based on the hardware and software platform for each respective fitness device. In embodiments, a memory device of a fitness device may include a combination of reference values determined for a plurality of similar fitness devices and reference values determined for that device. In embodiments, the stored reference values are based on the expected noise levels for the photometric front end circuit and/or optical sensing module.

When the processor compares the determined DC component of the PPG signal with a determined reference value, the processor may retrieve a reference value corresponding to the current configuration of the fitness device to select a second intensity signal. The processor may select a first intensity level for one or more emitters (e.g., LEDs) based on a default intensity level stored in memory.

FIG. 3 depicts an exemplary dot-plot of a PPG signal output from a photometric front end circuit of the fitness monitor in an idle state (when there is no light input to the photometric front end circuit from one or more photodiodes). Discrete digitized output points of the idle photometric front end circuit are collected over time, e.g., approximately 5.5 seconds, and provide a range of measurement variability or uncertainty in the amplitude of the PPG signal output that may be used to characterize performance of the fitness monitor independent of its use by an individual. In contrast, it may be expected by some that the theoretical PPG signal output in a controlled environment without light that may be received by one or more photodiodes (absence of light) would exhibit a near-zero output level of the PPG signal and/or an output level of the PPG signal that is flat (i.e., all PPG signal values are the same).

The reference value characterizing performance of the fitness monitor that may be representative of the range or variability of the PPG signal output from the photometric front end circuit while in the idle state may be determined from empirical and/or statistical analysis of the sampled output of the digitized PPG signal from the idle photometric front end circuit. The statistical analysis may include a normal or Gaussian distribution of the digitized PPG signal output, as shown in FIG. 4. The reference value stored on a memory device internal to and/or external of the fitness monitor may be any mathematical representation of the variation or dispersion of data values. For example, in

embodiments, the reference value may be a standard deviation of the PPG signal, a mean value of the PPG signal, a variance of the PPG signal outputs, a root mean square (RMS) of the PPG signal outputs, a peak-to-peak value of the PPG signal outputs, or any combination thereof. The memory device may store a plurality of reference values characterizing performance of the fitness monitor in a plurality of configurations (e.g., different gain settings, numbers of channels for photodiodes, number of pulses, width of pulses, voltage of LEDs, current of the LEDs, etc.). Thus, the memory device may include a table having a determined reference value corresponding to each configuration of the fitness monitor that may be implemented when the fitness monitor is worn and used by a user.

When the processor compares the determined DC component of the PPG signal with a determined reference value, the processor may retrieve a reference value corresponding to the current configuration of the fitness device to select a second intensity signal different from a first intensity signal (e.g., a default LED intensity level). This dynamic configuration of one or more fitness monitor components accounts for variations in operating parameters of the device and biometric characteristics of the user without utilizing an operating mode that characterizes the user while the device is worn by the user. When the fitness monitor is in use, for example, attached to and proximate the skin of a user and monitoring a physiological aspect of the user, the processor may retrieve a reference value characterizing the fitness monitor based on a determined variability or range of the PPG signal provided by the photometric front end circuit, compare a determined DC component of the PPG signal to the reference value and select a light intensity level based on the comparison. For example, a selected second light intensity level may cause a PPG signal having a DC component determined to be lower than desired due to selected operating parameters of the device and/or one or more biometric characteristics of a user to be increased to a level that enables determination of a cardiac component of the PPG signal.

An example embodiment of a fitness monitor **500** capable of executing the methods and processes described above is illustrated in FIG. **5**. The fitness monitor **500** includes an application processor **550** further including a user interface module **502**, a location determining component **504** (e.g., a global positioning system (GPS) receiver, Assisted-GPS, etc.), a communication module **506**, an inertial sensor **508** (e.g., accelerometer, gyroscope, etc.), and a controller **510**.

The fitness monitor **500** may be a general-use wearable computer (e.g., a watch, smart glasses, etc.), a cellular phone, a smartphone, a tablet computer, or a mobile personal computer, capable of monitoring a physiological aspect of an individual as described herein. The fitness monitor **500** may be a thin-client device or terminal that sends processing functions to a server device **522** via a network **524**. Communication via the network **524** may include any combination of wired and wireless technology. For example, network **524** may include a USB cable between fitness monitor **500** and computing device **548** to facilitate the bi-directional transfer of data between fitness monitor **500** and computing device **544**.

The controller **510** of the application processor **550** may include a program memory **512**, a microprocessor (MP) **514**, a random-access memory (RAM) **516**, and an input/output (I/O) circuitry **518**, all of which may be communicatively interconnected via an address/data bus **520**. Although the I/O circuitry **518** is depicted in FIG. **5** as a single block, the I/O circuitry **518** may include a number of different types of

I/O circuits. The program memory **512** may include an operating system **526**, a data storage device **528**, a plurality of software applications **530**, and/or a plurality of software routines **534**. The operating system **526** of program memory **512** may include any of a plurality of mobile platforms, such as the iOS®, Android™, Palm® webOS, Windows® Mobile/Phone, BlackBerry® OS, or Symbian® OS mobile technology platforms, developed by Apple Inc., Google Inc., Palm Inc. (now Hewlett-Packard Company), Microsoft Corporation, Research in Motion (RIM), and Nokia, respectively. The data storage device **528** of program memory **512** may include application data for the plurality of applications **530**, routine data for the plurality of routines **534**, and other data necessary to interact with the server **522** through the network **524**.

In particular, the data storage device **528** may include one or more reference values characterizing performance of the fitness monitor representative of the range of variability of the PPG signal output from the photometric front end circuit while in the idle state of the fitness monitor **500** (e.g., PPG signal output in response to a zero light input). Additional data stored within the data storage device **528** may include cardiac component data associated with one or more other individuals who wear and use of the fitness monitor **500**. The cardiac component data may include one or more compilations of recorded physiological aspects of the user, including, but not limited to, a heartbeat, heart rate, heart-rate variability, speed, distance traveled, calculating calories burned, body temperature, and the like. In some embodiments, the controller **510** may also include, or otherwise be operatively coupled for communication with other data storage mechanisms (e.g., one or more hard disk drives, optical storage drives, solid state storage devices, etc.) that may reside within the fitness monitor **500** and/or operatively coupled to the network **524** and/or server device **522**.

The fitness monitor **500** further includes a photometric front end circuit **552** communicably coupled between the application processor **550** and an optical sensing module **566**. The optical sensing module **566** includes one or more LEDs **542** and one or more photodiodes **544**, and is configured for placement adjacent the skin of a user when the fitness device **500** is secured or attached to the user. The photometric front end **552** may include an analog signal processor **554**, a digital signal processor **556**, an analog-to-digital converter **558**, a time slot controller **562**, I/O circuitry **562**, and one or more LED drivers **560** causing the LED(s) **542** to output light at one of a plurality of intensity levels. In embodiments, the LED driver **560** may alternately be integrated within the optical sensing module **566** as indicated by the dotted lines of the component. Further still, the LEDs **542**, LED driver **560**, and the photodiodes **544** may be integrated within the photometric front end **552**.

Operation of the photometric front end **552** facilitates stimulating the LED(s) **542** and measuring reflections of the light from the user's skin using one or more photodiodes **544**. The reflected signals may be output by the photodiodes **544** as a light intensity signal analyzed and filtered by the analog signal processor **554**, digitized by the analog-to-digital converter **558**, and analyzed by the digital signal processor **556**. Control and/or data communication amongst the application processor **550**, photometric front end **552**, and optical sensing module **566** is facilitated via the I/O circuitry **564**. In embodiments, any signals provided by the photometric front end **552** or optical sensing module **566** or any information determined based on such signals may be stored in the data storage **526** of the application processor **550**.

The LEDs (e.g., emitters) **542** output visible and/or non-visible light, and one or more photodiodes (e.g., receivers) **544** receive the visible and/or non-visible light and generate a light intensity signal based on the received reflections of the electromagnetic radiation. For example, LEDs **542** may include any combination of green light-emitting diodes (LEDs), red LEDs, and/or infrared LEDs that emit light into the user's skin. The photodiodes **544** receive reflections of visible-light and/or infrared (IR) light output by the LEDs **542** into the user's skin and generate the light intensity signal based on the received reflection. The light intensity signals generated by the one or more photodiodes **544** may be communicated to the photometric front end **552** for signal processing and digitization. The photometric front end **552** may include filters for the light intensity signals and analog-to-digital converters to digitize the light intensity signals into PPG signals including a cardiac cycle signal component associated with the user's heartbeat.

Typically, the one or more LEDs **542** are positioned against the user's skin to emit light into the user's skin and the one or more photodiodes **544** are positioned near the LEDs **542** to receive light emitted by the one or more emitters **542** after reflection from the user's skin. The photometric front end **552** and/or the processor **514** of fitness monitor **500** may determine a PPG signal based on a light intensity signal output by one or more photodiodes **544** based on light reflected after transmission of the light through or reflection from the user's skin that has been received by the photodiodes **544**.

The photometric front end **552** may utilize multiple time slots during operation, wherein the time slot controller **562** coordinates sequential operation of the signal path from LED stimulation to data capture and processing for each time slot and desired sampling period.

In both the transmitted and reflected uses, the intensity of measured light may be modulated by the cardiac cycle due to variation in tissue blood perfusion during the cardiac cycle. In activity environments, the intensity of measured light may also be strongly influenced by many other factors, including, but not limited to, the inherent "noise" characteristic static and/or variable ambient light intensity, body motion at the measurement location, static and/or variable sensor pressure on the skin, motion of the sensor relative to the body at the measurement location, breathing, and/or light barriers (including hair, opaque skin layers, sweat, etc.). Relative to these sources, the cardiac cycle component of the PPG signal can be very weak, frequently by one or more orders of magnitude.

The location determining component **504** may be a GPS receiver that is configured to provide geographic location information of the fitness monitor **500**. The location determining component may be, for example, a GPS receiver such as those provided in various products by GARMIN®. Generally, GPS is a satellite-based radio navigation system capable of determining continuous position, velocity, time, and direction information. Multiple users may simultaneously utilize GPS. GPS incorporates a plurality of GPS satellites that orbit the earth. Based on these orbits, GPS satellites can relay their location to a GPS receiver. For example, upon receiving a GPS signal, e.g., a radio signal, from a GPS satellite, the fitness monitor **500** disclosed herein can determine a location of that satellite. The fitness monitor **500** can continue scanning for GPS signals until it has acquired a number, e.g., at least three, of different GPS satellite signals. The fitness monitor **500** may employ geometrical triangulation, e.g., where the watch utilizes the known GPS satellite positions to determine a position of the

fitness monitor **500** relative to the GPS satellites. Geographic location information and/or velocity information can be updated, e.g., in real time on a continuous basis, for the fitness monitor **500**.

In embodiments, inertial sensor **508** may incorporate one or more accelerometers positioned to determine the acceleration and direction of movements of fitness monitor **500**. The accelerometer may determine magnitudes of acceleration in an X-axis, a Y-axis, and a Z-axis to measure the acceleration and direction of movement of fitness monitor **500** in each respective direction (or plane). It will be appreciated by those of ordinary skill in the art that a three dimensional vector describing a movement of the fitness monitor **500** through three dimensional space can be established by combining the outputs of the X-axis, Y-axis, and Z-axis accelerometers using known methods. Single and multiple axis models of the inertial sensor **508** are capable of detecting magnitude and direction of acceleration as a vector quantity, and may be used to sense orientation and/or coordinate acceleration of the user.

The photodiodes **544**, location determining component **504** and the inertial sensors **508** may be referred to collectively as the "sensors" of the fitness monitor **500**. It is also to be appreciated that additional location determining components **504** and/or inertial sensor(s) **508** may be operatively coupled to the fitness monitor **500**. In embodiments, the fitness monitor **500** may also include or be coupled to a microphone incorporated with the user interface module **502** and used to receive voice inputs from the user while the fitness monitor **500** monitors a cardiac signal of a user and determines physiological information based on the cardiac signal.

The communication module **506** may communicate with computing device **544** and/or server device **522** via any suitable wired or wireless communication protocol independently or using I/O circuitry **518**. The wired or wireless network **524** may include a wireless telephony network (e.g., GSM, CDMA, LTE, etc.), one or more standard of the Institute of Electrical and Electronics Engineers (IEEE), such as 802.11 or 802.16 (Wi-Max) standards, Wi-Fi standards promulgated by the Wi-Fi Alliance, Bluetooth standards promulgated by the Bluetooth Special Interest Group, a near field communication standard (e.g., ISO/IEC 18092, standards provided by the NFC Forum, etc.), and so on. Wired communications are also contemplated such as through universal serial bus (USB), Ethernet, serial connections, and so forth.

The fitness monitor **500** may be configured to communicate via one or more networks **524** with a cellular provider and an Internet provider to receive mobile phone service and various content, respectively. Content may represent a variety of different content, examples of which include, but are not limited to: map data, which may include route information; web pages; services; music; photographs; video; email service; instant messaging; device drivers; real-time and/or historical weather data; instruction updates; and so forth.

The user interface **502** of the fitness monitor **500** may include a "soft" keyboard that is presented on a display screen of the fitness monitor **500**, an external hardware keyboard communicating via a wired or a wireless connection (e.g., a Bluetooth keyboard), and/or an external mouse, or any other suitable user-input device or component. As described earlier, the user interface **502** may also include or communicate with a microphone capable of receiving voice input from a vehicle operator as well as a display device **546** having a touch input.

With reference to the controller **510**, it should be appreciated that controller **510** may include multiple microprocessors **514**, multiple RAMs **516**, and multiple program memories **512**. The controller **510** may implement the RAM **516** and the program memories **512** as semiconductor memories, magnetically readable memories, and/or optically readable memories, for example. The one or more processors **514** may be adapted and configured to execute any of the plurality of software applications **530** and/or any of the plurality of software routines **534** residing in the program memory **512**, in addition to other software applications. One of the plurality of applications **530** may be a client application **532** that may be implemented as a series of machine-readable instructions for performing the various functions associated with implementing the performance monitoring system as well as receiving information at, displaying information on, and transmitting information from the fitness monitor **500**. The client application **532** may function to implement a system wherein the front-end components communicate and cooperate with back-end components as described above. The client application **532** may include machine-readable instructions for implementing the user interface **502** to allow a user to input commands to, and receive information from, the fitness monitor **500**. One of the plurality of applications **530** may be a native web browser **536**, such as Apple's Safari®, Google Android™ mobile web browser, Microsoft Internet Explorer® for Mobile, Opera Mobile™, that may be implemented as a series of machine-readable instructions for receiving, interpreting, and displaying web page information from the server device **522** or other back-end components while also receiving inputs from the fitness monitor **500**. Another application of the plurality of applications **530** may include an embedded web browser **542** that may be implemented as a series of machine-readable instructions for receiving, interpreting, and displaying web page information from the server device **522** or other back-end components within the client application **532**.

The client applications **530** or routines **534** may include one or more processes for determining one or more reference value(s) associated with the non-ideal operating characteristics of the fitness monitor **500**. Namely, the analysis and determination of the reference values based on the output values of the PPG signal provided by the optical sensing module **566** in a controlled environment (e.g., no light is received by the photodiodes **544**) during the idle state of the fitness monitor **500**.

The client applications **530** or routines **534** may further include an accelerometer routine **538** that determines the acceleration and direction of movements of the fitness monitor **500**, which correlate to the acceleration, direction, and movement of the user. The accelerometer routine **538** may receive and process data from the inertial sensor **508** to determine one or more vectors describing the motion of the user for use with the client application **532**. In some embodiments where the inertial sensor **508** includes an accelerometer having X-axis, Y-axis, and Z-axis accelerometers, the accelerometer routine **538** may combine the data from each accelerometer to establish the vectors describing the motion of the user through three dimensional space. In some embodiments, the accelerometer routine **538** may use data pertaining to less than three axes.

The client applications **530** or routines **534** may further include a velocity routine **540** that coordinates with the location determining component **504** to determine or obtain velocity and direction information for use with one or more

of the plurality of applications, such as the client application **532**, or for use with other routines.

The user may also launch or instantiate any other suitable user interface application (e.g., the native web browser **536**, or any other one of the plurality of software applications **530**) to access the server device **522** to implement the monitoring process. Additionally, the user may launch the client application **532** from the fitness monitor **500** to access the server device **522** to implement the monitoring process.

After data has been gathered or determined by the sensors of the fitness monitor **500**, processor **514** may utilize a stored reference value to select (and thereby adjust) an intensity level for one or more emitters (e.g., LEDs) to improve or maintain the signal quality of the PPG signal enables determination of a cardiac component that may be used to determine an accurate heart rate for the user of fitness monitor **500** and/or reduction of power consumed by the fitness monitor **500**. The fitness monitor **500** may also implement time, frequency, pre-conditioning and post-conditioning, and time-variant filtering techniques as described in simultaneously filed U.S. patent application Ser. No. 15/296,956, entitled, "HEART RATE MONITOR WITH TIME-VARYING LINEAR FILTERING"; the contents of which are expressly incorporated herein by reference. Once the extent of the adjustment has been assessed, a cardiac signal can be determined. The fitness monitor **500** may also transmit information associated with the cardiac component of the user. For example, the transmitted information may be sent to a fitness facility capable of analyzing the data.

After data has been gathered or determined by the sensors of the fitness monitor **500**, previously acquired data may be utilized to determine the extent of adjustment to the time-variant filters. Once the extent of the adjustment has been assessed, a cardiac signal can be determined. The fitness monitor **500** may also transmit information associated with the cardiac component of the user. For example, the transmitted information may be sent to a fitness facility capable of analyzing the data.

In embodiments where the fitness monitor **500** is a thin-client device, the server device **522** may perform one or more processing functions remotely that may otherwise be performed by the fitness monitor **500**. In such embodiments, the server device **522** may include a number of software applications capable of receiving user information gathered by the sensors to be used in determining the cardiac component of the user. For example, the fitness monitor **500** may gather information from its sensors as described herein, but instead of using the information locally, the fitness monitor **500** may send the information to the server device **522** for remote processing. The server device **522** may perform the analysis of the gathered user information to determine a fitness aspect of the user as described herein. The server device **522** may also transmit information associated with the cardiac component of the user. For example, the information transmitted by the server device **522** may be sent to a fitness facility and include a request for analysis.

FIGS. 6A and 6B illustrate views of one example embodiment of the fitness monitor in accordance with one or more aspects described herein. The fitness monitor **600** described above may be configured in a variety of ways to determine and provide fitness information, including one or more cardiac components, as well as navigation functionality to the user of the device **600**. For instance, fitness monitor **600** includes a housing **602** of a sports watch or a pedometer including a processor configured for use during fitness and/or sporting activities. It is contemplated, however, that the disclosed techniques may be implemented in a mobile

phone, a hand-held portable computer, a tablet computer, a personal digital assistant, a multimedia device, a media player, a game device, any combination thereof, and so forth.

The fitness monitor **600** includes a case or housing **602** configured to house, e.g., substantially enclose, various components of the fitness monitor **600**. The housing **602** may be formed from a lightweight and impact-resistant material such as plastic, nylon, or combinations thereof, for example. The housing **602** may be formed from a non-conductive material, such as a non-metal material, for example. The housing **602** may include one or more gaskets, e.g., a seal, to make it substantially waterproof or water resistant. The housing **602** may include a location for a battery and/or another power source for powering one or more components of the fitness monitor **600**. The housing **602** may be a singular piece or may include a plurality of sections. In some embodiments, the housing **602** may be formed from a conductive material, such as metal, or a semi-conductive material.

The fitness monitor **600** includes a display device **604**. The display device **604** may include a liquid crystal display (LCD), a thin film transistor (TFT), a light-emitting diode (LED), a light-emitting polymer (LEP), and/or a polymer light-emitting diode (PLED). The display device **604** may be capable of displaying text and/or graphical information. The display device **604** may be backlit such that it may be viewed in the dark or other low-light environments. One example embodiment of the display device **604** is a 100 pixel by 64 pixel film compensated super-twisted nematic display (FSTN) including a bright white light-emitting diode (LED) backlight. The display device **604** may include a transparent lens that covers and/or protects components of the fitness monitor **600**. The display device **604** may be provided with a touch screen to receive input (e.g., data, commands, etc.) from a user. For example, a user may operate the fitness monitor **600** by touching the touch screen and/or by performing gestures on the screen. In some embodiments, the touch screen may be a capacitive touch screen, a resistive touch screen, an infrared touch screen, combinations thereof, and the like. The fitness monitor **600** may further include one or more input/output (I/O) devices (e.g., a keypad, buttons, a wireless input device, a thumb-wheel input device, a trackstick input device, and so on). The I/O devices may include one or more audio I/O devices, such as a microphone, speakers, and so on.

In accordance with one or more embodiments of the present disclosure, the fitness monitor **600** includes a user interface with one or more control buttons **606**. As illustrated in FIG. 6A, four control button **606** are associated with, e.g., adjacent, the housing **602**. While FIG. 6A illustrates four control buttons **606** associated with the housing **602**, it is to be understood that the fitness monitor **600** may include more or less control buttons **606**. Each control button **606** is configured to generally control a function of the fitness monitor **600**. Functions of the mobile electronic device **600** may be associated with a location determining component and/or a performance monitoring component. Functions of the fitness monitor **600** may include, but are not limited to, displaying a current geographic location of the fitness monitor **600**, mapping a location on the display **604**, locating a desired location and displaying the desired location on the display **604**, and presenting information based on a cardiac component of the PPG signal including, but not limited to, a cardiac cycle signal, a heartbeat signal, a heart-rate signal or variability of a heart rate signal for the user. User input may be provided from movement of the housing **602**, for

example, an inertial sensor(s), e.g., accelerometer, may be used to identify vertical, horizontal, and/or angular movement of the housing **602**. In addition or alternately, user input may be provided from touch inputs identified using various touch sensing technologies, such as resistive touch or capacitive touch interfaces.

The fitness monitor **600** also includes an optical sensing module **610**, as shown in FIG. 6B, including one or more emitters (e.g., LEDs) of visible and/or non-visible light and one or more receivers (e.g., photodiodes) of visible and/or non-visible light that generate a light intensity signal based on the received reflection of light.

The fitness monitor **600** includes a strap **608** that enables one or more LEDs and one or more photodiodes to be securely placed against the skin of a user. The strap **608** is associated with, e.g., coupled to and/or integrated with, the housing **602** and may be removably secured to the housing **602** via attachment of securing elements to corresponding connecting elements. Some examples of securing elements and/or connecting elements include, but are not limited to, hooks, latches, clamps, snaps, and the like. The strap **608** may be made of a lightweight and resilient thermoplastic elastomer and/or a fabric, for example, such that the strap **608** may encircle a portion of a user without discomfort while securing the fitness monitor to the user. The strap **608** may be configured to attach to various portions of a user, such as a user's leg, waist, wrist, forearm, and/or upper arm.

The processor of the fitness monitor may periodically determine a DC component of a received PPG signal. In other words, the processor continuously determines whether a different light intensity level must be selected based on a comparison of the determined DC component with a stored reference value. As illustrated in FIG. 7, a PPG signal provided by a photometric front end of the fitness device includes a cardiac component and the levels of the PPG signal may vary over a period of time. In addition to changes between peak-to-peak levels of the cardiac component of the PPG signal, the DC component (illustrated with a broken line) may vary significantly due to movement of the fitness device (caused by movement of the user's arm) or other factors. In some embodiments, the DC component of the PPG signal is determined by the processor to be a simple average or a moving average of PPG signal levels over a period of time. For example, for PPG signal illustrated in FIG. 7, the processor may determine an average of the various PPG signal levels over a period of sixteen seconds or a different duration (e.g., 2 seconds, 8 seconds, etc.). Other techniques, such as utilization of low-pass filtering, may be implemented to determine the DC component of the PPG signal.

The comparison of the determined DC component of the PPG signal to a stored reference value, which may correspond to a variance associated with a current configuration of one or more components, by processor may include determining a mathematical difference between or ratio of the values. In embodiments, the memory device may store a predetermined range of acceptable differences or ratios that do not require selection of a second intensity level based on the comparison. For example, if the determined DC component is determined to have an acceptable amount of variation, the processor of the fitness device may continue to use a selected first intensity level (e.g., default intensity level, a previously determined intensity level, etc.) without modification.

The applications and benefits of the systems, methods, and techniques described herein are not limited to only the above examples. Many other applications and benefits are

possible by using the systems, methods, and techniques described herein. Thus, many modifications and variations may be made in the techniques and structures described and illustrated herein without departing from the spirit and scope of the present invention. Accordingly, it should be understood that the methods and apparatus described herein are illustrative only and are not limiting upon the scope of the invention.

It should also be understood that, unless a term is expressly defined in this patent using the sentence "As used herein, the term '_____' is hereby defined to mean . . ." or a similar sentence, there is no intent to limit the meaning of that term, either expressly or by implication, beyond its plain or ordinary meaning, and such term should not be interpreted to be limited in scope based on any statement made in any section of this patent (other than the language of the claims). To the extent that any term recited in the claims at the end of this patent is referred to in this patent in a manner consistent with a single meaning, that is done for sake of clarity only so as to not confuse the reader, and it is not intended that such claim term be limited, by implication or otherwise, to that single meaning. Also, unless a claim element is defined by reciting the word "means" and a function without the recital of any structure, it is not intended that the scope of any claim element be interpreted based on the application of 35 U.S.C. §112(f) and/or pre-AIA 35 U.S.C. §112, sixth paragraph.

Moreover, although the foregoing text sets forth a detailed description of numerous different embodiments, it should be understood that the scope of the patent is defined by the words of the claims set forth at the end of this patent. The detailed description is to be construed as exemplary only and does not describe every possible embodiment because describing every possible embodiment would be impractical, if not impossible. Numerous alternative embodiments could be implemented, using either current technology or technology developed after the filing date of this patent, which would still fall within the scope of the claims.

What is claimed is:

1. A fitness monitor for monitoring a cardiac signal of a user, the device comprising:
 - an emitter configured to output light toward skin of the user;
 - an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels;
 - a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection;
 - a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal, the PPG signal including a cardiac signal of the user;
 - a memory device configured to store a reference value characterizing performance of the photometric front end based on a variability of the PPG signal output from the photometric front end during idle operation; and
 - a processor communicatively coupled to the emitter, the receiver, photometric front end and the memory device, the processor configured to:
 - select a first intensity level for the emitter to output light,
 - transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level,

- determine a DC component of a PPG signal received from photometric front end,
 - select a second intensity level based on a comparison of the determined DC component of the received PPG signal with the stored reference value,
 - transmit a second output control signal including the selected second intensity level to the emitter driver causing the emitter to output light at the selected second intensity level, and
 - identify the cardiac component in the received PPG signal.
2. The fitness monitor of claim 1, wherein the emitter driver is integrated within the photometric front end.
 3. The fitness monitor of claim 1, wherein the photometric front end is integrated within the processor.
 4. The fitness monitor of claim 1, wherein the emitter is a LED and the receiver is a photodiode.
 5. The fitness monitor of claim 1, wherein the processor is further configured to transmit a receiver control signal to the receiver causing the receiver to generate the light intensity signal.
 6. The fitness monitor of claim 1, wherein the processor is further configured to transmit a receive timing signal to the photometric front end causing the photometric front end to receive the light intensity signal from the receiver.
 7. The fitness monitor of claim 6, wherein the processor is further configured to cause the photometric front end to receive the light intensity signal in a first time period and a second time period based on the receive timing signal.
 8. The fitness monitor of claim 1, wherein the first output control signal causes the emitter to output light in a first time period and a second output control signal causes the emitter to output light in the second time period.
 9. The fitness monitor of claim 1, wherein the variability of the PPG signal output from the photometric front end during idle operation is determined when the receiver does not receive a reflection of the transmitted light.
 10. The fitness monitor of claim 1, wherein the variability of the PPG signal output from the photometric front end during idle operation is a mathematical representation of a variation of the PPG signal measurements.
 11. The fitness monitor of claim 1, wherein the reference value is determined when the fitness monitor is not proximate to the skin of the user.
 12. The fitness monitor of claim 1, further comprising an inertial sensor configured to provide a motion signal based on sensed movement of the fitness monitor, wherein the processor is further configured to transmit the second output control signal when the motion signal is below a predetermined motion level.
 13. A fitness monitor for monitoring a cardiac signal of a user, the device comprising:
 - an emitter configured to output light toward skin of the user;
 - an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels;
 - a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection;
 - a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal, the PPG signal including a cardiac signal;
 - a reference value characterizing performance of the photometric front end based on a variability of the PPG signal output from the photometric front end when the fitness monitor is not proximate to the skin of the user;

19

a memory device configured to store the reference value; and
 a processor communicatively coupled to the emitter, the receiver, photometric front end and the memory device, the processor configured to:
 select a first intensity level for the emitter to output light,
 transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level,
 determine a DC component of a PPG signal received from the photometric front end,
 select a second intensity level based on a comparison of the determined DC component of the received PPG signal with the stored reference value,
 transmit a second output control signal including the selected second intensity level to the emitter driver causing the emitter to output light at the selected second intensity level, and
 identify the cardiac component in the received PPG signal.

14. The fitness monitor of claim 13, wherein the emitter driver is integrated within the photometric front end.

15. The fitness monitor of claim 13, wherein the photometric front end is integrated within the processor.

16. The fitness monitor of claim 13, wherein the emitter is a LED and the receiver is a photodiode.

17. The fitness monitor of claim 13, wherein the processor is further configured to transmit a receiver control signal to the receiver causing the receiver to generate the light intensity signal.

18. The fitness monitor of claim 13, wherein the processor is further configured to transmit a receive timing signal to the photometric front end causing the photometric front end to receive the light intensity signal from the receiver.

20

19. The fitness monitor of claim 18, wherein the processor is further configured to cause the photometric front end to receive the light intensity signal in a first time period and a second time period based on the receive timing signal.

20. A fitness monitor for monitoring a cardiac signal of a user comprising an emitter configured to output light toward skin of the user, an emitter driver configured to cause the emitter to output light at one of a plurality of intensity levels, a receiver configured to receive a reflection of the transmitted light and generate a light intensity signal based on the received reflection, a photometric front end configured to receive the light intensity signal and generate a photoplethysmogram (PPG) signal based on the light intensity signal and representing the cardiac signal, and a tangible non-transitory computer-readable medium storing instructions and a reference value characterizing performance of the photometric front end based on a variability of the PPG signal output from the photometric front end during idle operation, wherein the instructions, when executed by one or more processors, cause the fitness monitor to:

select a first intensity level for the emitter to output light,
 transmit a first output control signal including the selected first intensity level to the emitter driver causing the emitter to output light at the selected first intensity level,

determine a DC component of the PPG signal,
 select a second intensity level based on a comparison of the determined DC component of the PPG signal with the stored reference value,

transmit a second output control signal including the selected second intensity level to the emitter driver causing the emitter to output light at the selected second intensity level, and

identify the cardiac component in the PPG signal.

* * * * *

专利名称(译)	用于生成PPG信号的系统和方法		
公开(公告)号	US9717424	公开(公告)日	2017-08-01
申请号	US15/296938	申请日	2016-10-18
申请(专利权)人(译)	GARMIN瑞士GMBH		
当前申请(专利权)人(译)	GARMIN瑞士GMBH		
[标]发明人	KULACH CHRISTOPHER J		
发明人	KULACH, CHRISTOPHER J.		
IPC分类号	A61B5/02 A61B5/11 A61B5/024 A61B5/00		
CPC分类号	A61B5/02416 A61B5/1112 A61B5/1118 A61B5/7278 A61B5/7285 A61B5/02438 A61B5/681 A61B5/725 A61B2562/0219 A61B5/02405 A61B5/02427 A61B5/0833 A61B5/165 A61B5/4815 A61B5/486 A61B5/721		
优先权	62/243447 2015-10-19 US		
其他公开文献	US20170105638A1		
外部链接	Espacenet USPTO		

摘要(译)

基于其操作的健身监测器的表征使得处理器能够考虑设备操作模式和用户的生物特征的变化。健身监测器包括用于向用户的皮肤传输光的发射器（例如，LED），用于接收透射光的反射的接收器（例如，光电二极管），用于基于产生光电容积描记图（PPG）信号的光度计前端。所接收的反射和处理器被配置为基于PPG信号的确分量与参考值的比较来选择发射器的强度水平。可以基于所确定的PPG信号的可变性或范围来表征健康监测器的参考值可以由处理器用于改善或维持PPG信号的信号质量以使得能够确定心脏成分和/或减少健身装置的耗电量。

