



US009566019B2

(12) **United States Patent**
Al-Ali et al.

(10) **Patent No.:** **US 9,566,019 B2**
(45) **Date of Patent:** ***Feb. 14, 2017**

(54) **RESPIRATORY MONITORING**

- (71) Applicant: **MASIMO Corporation**, Irvine, CA (US)
- (72) Inventors: **Ammar Al-Ali**, Tustin, CA (US);
Mohamed K. Diab, Ladera Ranch, CA (US)
- (73) Assignee: **MASIMO CORPORATION**, Irvine, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 456 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/153,656**

(22) Filed: **Jan. 13, 2014**

(65) **Prior Publication Data**

US 2014/0194766 A1 Jul. 10, 2014

Related U.S. Application Data

- (63) Continuation of application No. 13/224,266, filed on Sep. 1, 2011, now Pat. No. 8,667,967, which is a (Continued)

- (51) **Int. Cl.**
A61M 11/00 (2006.01)
A61B 5/083 (2006.01)
(Continued)

- (52) **U.S. Cl.**
CPC **A61B 5/0836** (2013.01); **A61B 5/0004** (2013.01); **A61B 5/0816** (2013.01); **A61B 5/097** (2013.01);
(Continued)

(58) **Field of Classification Search**

CPC A61B 5/0836; A61B 5/004; A61B 5/6822; A61B 5/0816; A61B 5/682; A61B 5/6819; A61B 5/097; A61M 16/0672; A61M 16/0666; A61M 5/682; A61M 16/10; A61M 2230/42; A61M 2205/18; A61M 2205/582; A61M 2205/581; A61M 2230/432; A61M 2230/435; A61M 2202/0208; A61M 2205/583; A61M 2205/3561

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,924,876 A 5/1990 Cameron
4,960,128 A 10/1990 Gordon et al.
(Continued)


Primary Examiner — Steven Douglas

(74) *Attorney, Agent, or Firm* — Knobbe Martens Olson & Bear LLP

(57) **ABSTRACT**

A patient interface in accordance with one embodiment of the present disclosure is configured to be at least partially carried by a patient and to receive gas exhaled by the patient. The patient interface includes first and second cannula tubes each having a first end and a second end, the first ends are configured to be inserted into the nostrils of a patient, the first and second cannula tubes are configured to direct exhaled gas from the patient from the first ends to said second ends. The patient interface also includes first and second sensors positioned near the second ends, and the first and second sensors are configured to provide first and second signals based upon the gas, wherein the first and second signals are indicative of a physiological parameter of the patient. The patient interface also includes a communications link configured to provide the signal to a physiological monitor.

20 Claims, 4 Drawing Sheets

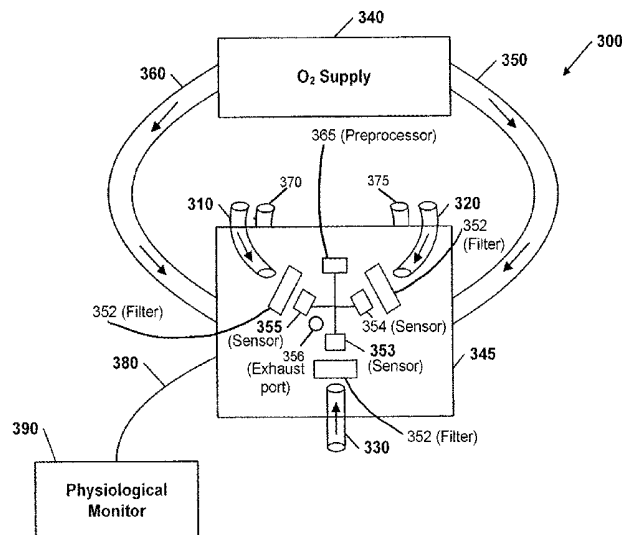

Related U.S. Application Data

- continuation of application No. 11/756,501, filed on May 31, 2007, now Pat. No. 8,028,701.
- (60) Provisional application No. 60/809,882, filed on May 31, 2006.
- (51) **Int. Cl.**
A61B 5/097 (2006.01)
A61B 5/00 (2006.01)
A61M 16/06 (2006.01)
A61M 16/10 (2006.01)
A61B 5/08 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 5/682* (2013.01); *A61B 5/6819* (2013.01); *A61B 5/6822* (2013.01); *A61M 16/0666* (2013.01); *A61M 16/0672* (2014.02); *A61M 16/10* (2013.01); *A61M 2202/0208* (2013.01); *A61M 2205/18* (2013.01); *A61M 2205/3561* (2013.01); *A61M 2205/581* (2013.01); *A61M 2205/583* (2013.01); *A61M 2230/42* (2013.01); *A61M 2230/432* (2013.01); *A61M 2230/435* (2013.01)
- (58) **Field of Classification Search**
 USPC 128/206.11, 207.18, 204.12, 206.18, 128/207.13, 207.29, 204.22, 204.23
 See application file for complete search history.

(56) References Cited

U.S. PATENT DOCUMENTS

4,964,408 A	10/1990	Hink et al.	5,791,347 A	8/1998	Flaherty et al.
5,041,187 A	8/1991	Hink et al.	5,810,734 A	9/1998	Caro et al.
5,069,213 A	12/1991	Polczynski	5,823,950 A	10/1998	Diab et al.
5,163,438 A	11/1992	Gordon et al.	5,830,131 A	11/1998	Caro et al.
5,319,355 A	6/1994	Russek	5,833,618 A	11/1998	Caro et al.
5,337,744 A	8/1994	Branigan	5,860,919 A	1/1999	Kiani-Azarbayjany et al.
5,341,805 A	8/1994	Stavridi et al.	5,890,929 A	4/1999	Mills et al.
D353,195 S	12/1994	Savage et al.	5,904,654 A	5/1999	Wohltmann et al.
D353,196 S	12/1994	Savage et al.	5,919,134 A	7/1999	Diab
5,377,676 A	1/1995	Vari et al.	5,934,925 A	8/1999	Tobler et al.
5,404,885 A	4/1995	Sheehan et al.	5,940,182 A	8/1999	Lepper, Jr. et al.
D359,546 S	6/1995	Savage et al.	5,995,855 A	11/1999	Kiani et al.
5,431,170 A	7/1995	Mathews	5,997,343 A	12/1999	Mills et al.
D361,840 S	8/1995	Savage et al.	6,002,952 A	12/1999	Diab et al.
D362,063 S	9/1995	Savage et al.	6,011,986 A	1/2000	Diab et al.
5,452,717 A	9/1995	Branigan et al.	6,027,452 A	2/2000	Flaherty et al.
D363,120 S	10/1995	Savage et al.	6,036,642 A	3/2000	Diab et al.
5,456,252 A	10/1995	Vari et al.	6,045,509 A	4/2000	Caro et al.
5,479,934 A	1/1996	Imran	6,067,462 A	5/2000	Diab et al.
5,482,036 A	1/1996	Diab et al.	6,081,735 A	6/2000	Diab et al.
5,490,505 A	2/1996	Diab et al.	6,088,607 A	7/2000	Diab et al.
5,494,043 A	2/1996	O'Sullivan et al.	6,110,522 A	8/2000	Lepper, Jr. et al.
5,533,511 A	7/1996	Kaspari et al.	6,124,597 A	9/2000	Shehada
5,534,851 A	7/1996	Russek	6,128,521 A	10/2000	Marro et al.
5,561,275 A	10/1996	Savage et al.	6,129,675 A	10/2000	Jay
5,562,002 A	10/1996	Lalin	6,144,868 A	11/2000	Parker
5,590,649 A	1/1997	Caro et al.	6,151,516 A	11/2000	Kiani-Azarbayjany et al.
5,602,924 A	2/1997	Durand et al.	6,152,754 A	11/2000	Gerhardt et al.
5,632,272 A	5/1997	Diab et al.	6,157,850 A	12/2000	Diab et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	6,165,005 A	12/2000	Mills et al.
5,638,818 A	6/1997	Diab et al.	6,184,521 B1	2/2001	Coffin, IV et al.
5,645,440 A	7/1997	Tobler et al.	6,206,830 B1	3/2001	Diab et al.
5,685,299 A	11/1997	Diab et al.	6,229,856 B1	5/2001	Diab et al.
D393,830 S	4/1998	Tobler et al.	6,232,609 B1	5/2001	Snyder et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,236,872 B1	5/2001	Diab et al.
5,758,644 A	6/1998	Diab et al.	6,241,683 B1	6/2001	Macklem et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,253,097 B1	6/2001	Aronow et al.
5,769,785 A	6/1998	Diab et al.	6,256,523 B1	7/2001	Diab et al.
5,782,757 A	7/1998	Diab et al.	6,263,222 B1	7/2001	Diab et al.
5,785,659 A	7/1998	Caro et al.	6,278,522 B1	8/2001	Lepper, Jr. et al.
			6,280,213 B1	8/2001	Tobler et al.
			6,285,896 B1	9/2001	Tobler et al.
			6,301,493 B1	10/2001	Marro et al.
			6,317,627 B1	11/2001	Ennen et al.
			6,321,100 B1	11/2001	Parker
			6,325,761 B1	12/2001	Jay
			6,334,065 B1	12/2001	Al-Ali et al.
			6,343,224 B1	1/2002	Parker
			6,349,228 B1	2/2002	Kiani et al.
			6,360,114 B1	3/2002	Diab et al.
			6,368,283 B1	4/2002	Xu et al.
			6,371,921 B1	4/2002	Caro et al.
			6,377,829 B1	4/2002	Al-Ali
			6,388,240 B2	5/2002	Schulz et al.
			6,397,091 B2	5/2002	Diab et al.
			6,430,437 B1	8/2002	Marro
			6,430,525 B1	8/2002	Weber et al.
			6,463,311 B1	10/2002	Diab
			6,470,199 B1	10/2002	Kopotic et al.
			6,501,975 B2	12/2002	Diab et al.
			6,505,059 B1	1/2003	Kollias et al.
			6,515,273 B2	2/2003	Al-Ali
			6,519,487 B1	2/2003	Parker
			6,525,386 B1	2/2003	Mills et al.
			6,526,300 B1	2/2003	Kiani et al.
			6,541,756 B2	4/2003	Schulz et al.
			6,542,764 B1	4/2003	Al-Ali et al.
			6,580,086 B1	6/2003	Schulz et al.
			6,584,336 B1	6/2003	Ali et al.
			6,595,316 B2	7/2003	Cybulski et al.
			6,597,932 B2	7/2003	Tian et al.
			6,597,933 B2	7/2003	Kiani et al.
			6,606,511 B1	8/2003	Ali et al.
			6,632,181 B2	10/2003	Flaherty et al.
			6,639,668 B1	10/2003	Trepagnier
			6,640,116 B2	10/2003	Diab
			6,643,530 B2	11/2003	Diab et al.
			6,650,917 B2	11/2003	Diab et al.
			6,654,624 B2	11/2003	Diab et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,658,276 B2	12/2003	Kiani et al.	7,255,107 B1	8/2007	Gomez
6,661,161 B1	12/2003	Lanzo et al.	7,272,425 B2	9/2007	Al-Ali
6,671,531 B2	12/2003	Al-Ali et al.	7,274,955 B2	9/2007	Kiani et al.
6,678,543 B2	1/2004	Diab et al.	D554,263 S	10/2007	Al-Ali
6,684,090 B2	1/2004	Ali et al.	7,280,858 B2	10/2007	Al-Ali et al.
6,684,091 B2	1/2004	Parker	7,289,835 B2	10/2007	Mansfield et al.
6,697,656 B1	2/2004	Al-Ali	7,292,883 B2	11/2007	De Felice et al.
6,697,657 B1	2/2004	Shehada et al.	7,295,866 B2	11/2007	Al-Ali
6,697,658 B2	2/2004	Al-Ali	7,328,053 B1	2/2008	Diab et al.
RE38,476 E	3/2004	Diab et al.	7,332,784 B2	2/2008	Mills et al.
6,699,194 B1	3/2004	Diab et al.	7,340,287 B2	3/2008	Mason et al.
6,714,804 B2	3/2004	Al-Ali et al.	7,341,559 B2	3/2008	Schulz et al.
RE38,492 E	4/2004	Diab et al.	7,343,186 B2	3/2008	Lamego et al.
6,721,582 B2	4/2004	Trepagnier et al.	D566,282 S	4/2008	Al-Ali et al.
6,721,585 B1	4/2004	Parker	7,355,512 B1	4/2008	Al-Ali
6,725,075 B2	4/2004	Al-Ali	7,356,365 B2	4/2008	Schurman
6,728,560 B2	4/2004	Kollias et al.	7,371,981 B2	5/2008	Abdul-Hafiz
6,735,459 B2	5/2004	Parker	7,373,193 B2	5/2008	Al-Ali et al.
6,745,060 B2	6/2004	Diab et al.	7,373,194 B2	5/2008	Weber et al.
6,760,607 B2	7/2004	Al-Ali	7,376,453 B1	5/2008	Diab et al.
6,770,028 B1	8/2004	Ali et al.	7,377,794 B2	5/2008	Al-Ali et al.
6,771,994 B2	8/2004	Kiani et al.	7,377,899 B2	5/2008	Weber et al.
6,792,300 B1	9/2004	Diab et al.	7,383,070 B2	6/2008	Diab et al.
6,813,511 B2	11/2004	Diab et al.	7,415,297 B2	8/2008	Al-Ali et al.
6,816,741 B2	11/2004	Diab	7,428,432 B2	9/2008	Ali et al.
6,822,564 B2	11/2004	Al-Ali	7,438,683 B2	10/2008	Al-Ali et al.
6,826,419 B2	11/2004	Diab et al.	7,440,787 B2	10/2008	Diab
6,830,711 B2	12/2004	Mills et al.	7,448,381 B2 *	11/2008	Sasaki A61M 16/20 128/204.18
6,850,787 B2	2/2005	Weber et al.	7,454,240 B2	11/2008	Diab et al.
6,850,788 B2	2/2005	Al-Ali	7,467,002 B2	12/2008	Weber et al.
6,852,083 B2	2/2005	Caro et al.	7,469,157 B2	12/2008	Diab et al.
6,861,639 B2	3/2005	Al-Ali	7,471,969 B2	12/2008	Diab et al.
6,898,452 B2	5/2005	Al-Ali et al.	7,471,971 B2	12/2008	Diab et al.
6,920,345 B2	7/2005	Al-Ali et al.	7,483,729 B2	1/2009	Al-Ali et al.
6,931,268 B1	8/2005	Kiani-Azarbayjany et al.	7,483,730 B2	1/2009	Diab et al.
6,934,570 B2	8/2005	Kiani et al.	7,489,958 B2	2/2009	Diab et al.
6,939,305 B2	9/2005	Flaherty et al.	7,496,391 B2	2/2009	Diab et al.
6,943,348 B1	9/2005	Coffin IV	7,496,393 B2	2/2009	Diab et al.
6,950,687 B2	9/2005	Al-Ali	D587,657 S	3/2009	Al-Ali et al.
6,961,598 B2	11/2005	Diab	7,499,741 B2	3/2009	Diab et al.
6,970,792 B1	11/2005	Diab	7,499,835 B2	3/2009	Weber et al.
6,979,812 B2	12/2005	Al-Ali	7,500,950 B2	3/2009	Al-Ali et al.
6,985,764 B2	1/2006	Mason et al.	7,509,154 B2	3/2009	Diab et al.
6,993,371 B2	1/2006	Kiani et al.	7,509,494 B2	3/2009	Al-Ali
6,996,427 B2	2/2006	Ali et al.	7,510,849 B2	3/2009	Schurman et al.
6,999,904 B2	2/2006	Weber et al.	7,526,328 B2	4/2009	Diab et al.
7,003,338 B2	2/2006	Weber et al.	7,530,942 B1	5/2009	Diab
7,003,339 B2	2/2006	Diab et al.	7,530,949 B2	5/2009	Al Ali et al.
7,015,451 B2	3/2006	Dalke et al.	7,530,955 B2	5/2009	Diab et al.
7,024,233 B2	4/2006	Ali et al.	7,563,110 B2	7/2009	Al-Ali et al.
7,027,849 B2	4/2006	Al-Ali	7,596,398 B2	9/2009	Al-Ali et al.
7,030,749 B2	4/2006	Al-Ali	7,618,375 B2	11/2009	Flaherty
7,039,449 B2	5/2006	Al-Ali	D606,659 S	12/2009	Kiani et al.
7,041,060 B2	5/2006	Flaherty et al.	7,647,083 B2	1/2010	Al-Ali et al.
7,044,918 B2	5/2006	Diab	D609,193 S	2/2010	Al-Ali et al.
7,067,893 B2	6/2006	Mills et al.	D614,305 S	4/2010	Al-Ali et al.
7,096,052 B2	8/2006	Mason et al.	RE41,317 E	5/2010	Parker
7,096,054 B2	8/2006	Abdul-Hafiz et al.	7,729,733 B2	6/2010	Al-Ali et al.
7,132,641 B2	11/2006	Schulz et al.	7,734,320 B2	6/2010	Al-Ali
7,142,901 B2	11/2006	Kiani et al.	7,761,127 B2	7/2010	Al-Ali et al.
7,149,561 B2	12/2006	Diab	7,761,128 B2	7/2010	Al-Ali et al.
7,186,966 B2	3/2007	Al-Ali	7,764,982 B2	7/2010	Dalke et al.
7,190,261 B2	3/2007	Al-Ali	D621,516 S	8/2010	Kiani et al.
7,215,984 B2	5/2007	Diab	7,791,155 B2	9/2010	Diab
7,215,986 B2	5/2007	Diab	7,801,581 B2	9/2010	Diab
7,221,971 B2	5/2007	Diab	7,822,452 B2	10/2010	Schurman et al.
7,225,006 B2	5/2007	Al-Ali et al.	RE41,912 E	11/2010	Parker
7,225,007 B2	5/2007	Al-Ali	7,844,313 B2	11/2010	Kiani et al.
RE39,672 E	6/2007	Shehada et al.	7,844,314 B2	11/2010	Al-Ali
7,239,905 B2	7/2007	Kiani-Azarbayjany et al.	7,844,315 B2	11/2010	Al-Ali
7,245,953 B1	7/2007	Parker	7,865,222 B2	1/2011	Weber et al.
7,254,429 B2	8/2007	Schurman et al.	7,873,497 B2	1/2011	Weber et al.
7,254,431 B2	8/2007	Al-Ali	7,880,606 B2	2/2011	Al-Ali
7,254,433 B2	8/2007	Diab et al.	7,880,626 B2	2/2011	Al-Ali et al.
7,254,434 B2	8/2007	Schulz et al.	7,891,355 B2	2/2011	Al-Ali et al.
			7,894,868 B2	2/2011	Al-Ali et al.
			7,899,507 B2	3/2011	Al-Ali et al.
			7,899,518 B2	3/2011	Trepagnier et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,904,132 B2	3/2011	Weber et al.	8,385,995 B2	2/2013	Al-ali et al.
7,909,772 B2	3/2011	Popov et al.	8,385,996 B2	2/2013	Smith et al.
7,910,875 B2	3/2011	Al-Ali	8,388,353 B2	3/2013	Kiani et al.
7,919,713 B2	4/2011	Al-Ali et al.	8,399,822 B2	3/2013	Al-Ali
7,937,128 B2	5/2011	Al-Ali	8,401,602 B2	3/2013	Kiani
7,937,129 B2	5/2011	Mason et al.	8,405,608 B2	3/2013	Al-Ali et al.
7,937,130 B2	5/2011	Diab et al.	8,414,499 B2	4/2013	Al-Ali et al.
7,941,199 B2	5/2011	Kiani	8,418,524 B2	4/2013	Al-Ali
7,951,086 B2	5/2011	Flaherty et al.	8,423,106 B2	4/2013	Lamego et al.
7,957,780 B2	6/2011	Lamego et al.	8,428,967 B2	4/2013	Olsen et al.
7,962,188 B2	6/2011	Kiani et al.	8,430,817 B1	4/2013	Al-Ali et al.
7,962,190 B1	6/2011	Diab et al.	8,437,825 B2	5/2013	Dalvi et al.
7,976,472 B2	7/2011	Kiani	8,455,290 B2	6/2013	Siskavich
7,988,637 B2	8/2011	Diab	8,457,703 B2	6/2013	Al-Ali
7,990,382 B2	8/2011	Kiani	8,457,707 B2	6/2013	Kiani
7,991,446 B2	8/2011	Al-Ali et al.	8,463,349 B2	6/2013	Diab et al.
8,000,761 B2	8/2011	Al-Ali	8,466,286 B2	6/2013	Bellott et al.
8,008,088 B2	8/2011	Bellott et al.	8,471,713 B2	6/2013	Poeze et al.
RE42,753 E	9/2011	Kiani-Azarbayjany et al.	8,473,020 B2	6/2013	Kiani et al.
8,019,400 B2	9/2011	Diab et al.	8,483,787 B2	7/2013	Al-Ali et al.
8,028,701 B2	10/2011	Al-Ali et al.	8,489,364 B2	7/2013	Weber et al.
8,029,765 B2	10/2011	Bellott et al.	8,498,684 B2	7/2013	Weber et al.
8,036,728 B2	10/2011	Diab et al.	8,509,867 B2	8/2013	Workman et al.
8,046,040 B2	10/2011	Ali et al.	8,515,509 B2	8/2013	Bruinsma et al.
8,046,041 B2	10/2011	Diab et al.	8,523,781 B2	9/2013	Al-Ali
8,046,042 B2	10/2011	Diab et al.	8,529,301 B2	9/2013	Al-Ali et al.
8,048,040 B2	11/2011	Kiani	8,532,727 B2	9/2013	Ali et al.
8,050,728 B2	11/2011	Al-Ali et al.	8,532,728 B2	9/2013	Diab et al.
RE43,169 E	2/2012	Parker	D692,145 S	10/2013	Al-Ali et al.
8,118,620 B2	2/2012	Al-Ali et al.	8,547,209 B2	10/2013	Kiani et al.
8,126,528 B2	2/2012	Diab et al.	8,548,548 B2	10/2013	Al-Ali
8,128,572 B2	3/2012	Diab et al.	8,548,550 B2	10/2013	Al-Ali et al.
8,130,105 B2	3/2012	Al-Ali et al.	8,560,032 B2	10/2013	Al-Ali et al.
8,145,287 B2	3/2012	Diab et al.	8,560,034 B1	10/2013	Diab et al.
8,150,487 B2	4/2012	Diab et al.	8,570,167 B2	10/2013	Al-Ali
8,175,672 B2	5/2012	Parker	8,570,503 B2	10/2013	Vo et al.
8,180,420 B2	5/2012	Diab et al.	8,571,618 B1	10/2013	Lamego et al.
8,182,443 B1	5/2012	Kiani	8,571,619 B2	10/2013	Al-Ali et al.
8,185,180 B2	5/2012	Diab et al.	8,577,431 B2	11/2013	Lamego et al.
8,190,223 B2	5/2012	Al-Ali et al.	8,584,345 B2	11/2013	Al-Ali et al.
8,190,227 B2	5/2012	Diab et al.	8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,203,438 B2	6/2012	Kiani et al.	8,600,467 B2	12/2013	Al-Ali et al.
8,203,704 B2	6/2012	Merritt et al.	8,606,342 B2	12/2013	Diab
8,224,411 B2	7/2012	Al-Ali et al.	8,626,255 B2	1/2014	Al-Ali et al.
8,228,181 B2	7/2012	Al-Ali	8,630,691 B2	1/2014	Lamego et al.
8,229,533 B2	7/2012	Diab et al.	8,634,889 B2	1/2014	Al-Ali et al.
8,233,955 B2	7/2012	Al-Ali et al.	8,641,631 B2	2/2014	Sierra et al.
8,244,325 B2	8/2012	Al-Ali et al.	8,652,060 B2	2/2014	Al-Ali
8,255,026 B1	8/2012	Al-Ali	8,663,107 B2	3/2014	Kiani
8,255,027 B2	8/2012	Al-Ali et al.	8,666,468 B1	3/2014	Al-Ali
8,255,028 B2	8/2012	Al-Ali et al.	8,667,967 B2	3/2014	Al-Ali et al.
8,260,577 B2	9/2012	Weber et al.	8,670,811 B2	3/2014	O'Reilly
8,265,723 B1	9/2012	McHale et al.	8,670,814 B2	3/2014	Diab et al.
8,274,360 B2	9/2012	Sampath et al.	8,676,286 B2	3/2014	Weber et al.
8,301,217 B2	10/2012	Al-Ali et al.	2002/0017300 A1	2/2002	Hickle et al.
8,310,336 B2	11/2012	Muhsin et al.	2003/0154981 A1	8/2003	Spruiell
8,315,683 B2	11/2012	Al-Ali et al.	2003/0216660 A1 *	11/2003	Ben-Oren A61B 5/083 600/532
8,337,403 B2	12/2012	Al-Ali et al.	2005/0245836 A1	11/2005	Star et al.
8,346,330 B2	1/2013	Lamego	2005/0288571 A1	12/2005	Perkins et al.
8,353,842 B2	1/2013	Al-Ali et al.	2009/0299672 A1 *	12/2009	Zhang A61B 5/02156 702/98
8,355,766 B2	1/2013	MacNeish, III et al.	2010/0078024 A1 *	4/2010	Andrieux A61M 16/0051 128/204.21
8,359,080 B2	1/2013	Diab et al.	2014/0276100 A1 *	9/2014	Satterfield A61B 5/082 600/476
8,364,223 B2	1/2013	Al-Ali et al.			
8,364,226 B2	1/2013	Diab et al.			
8,374,665 B2	2/2013	Lamego			

* cited by examiner

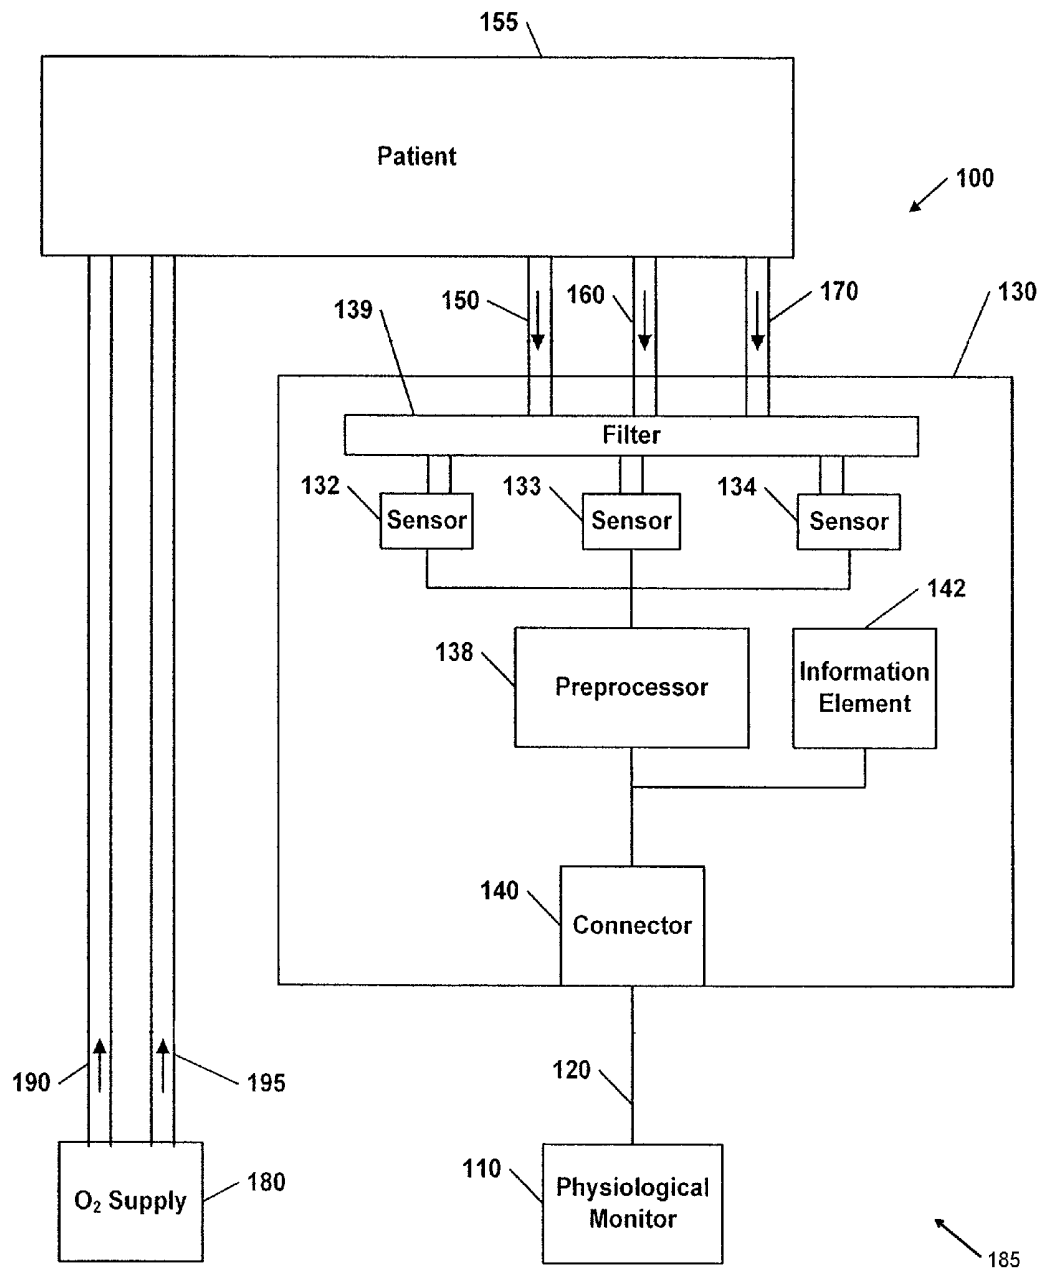


Figure 1

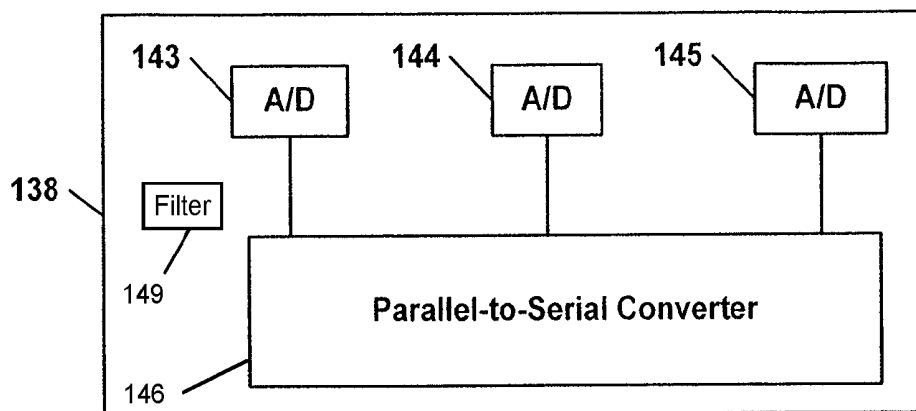


Figure 1A

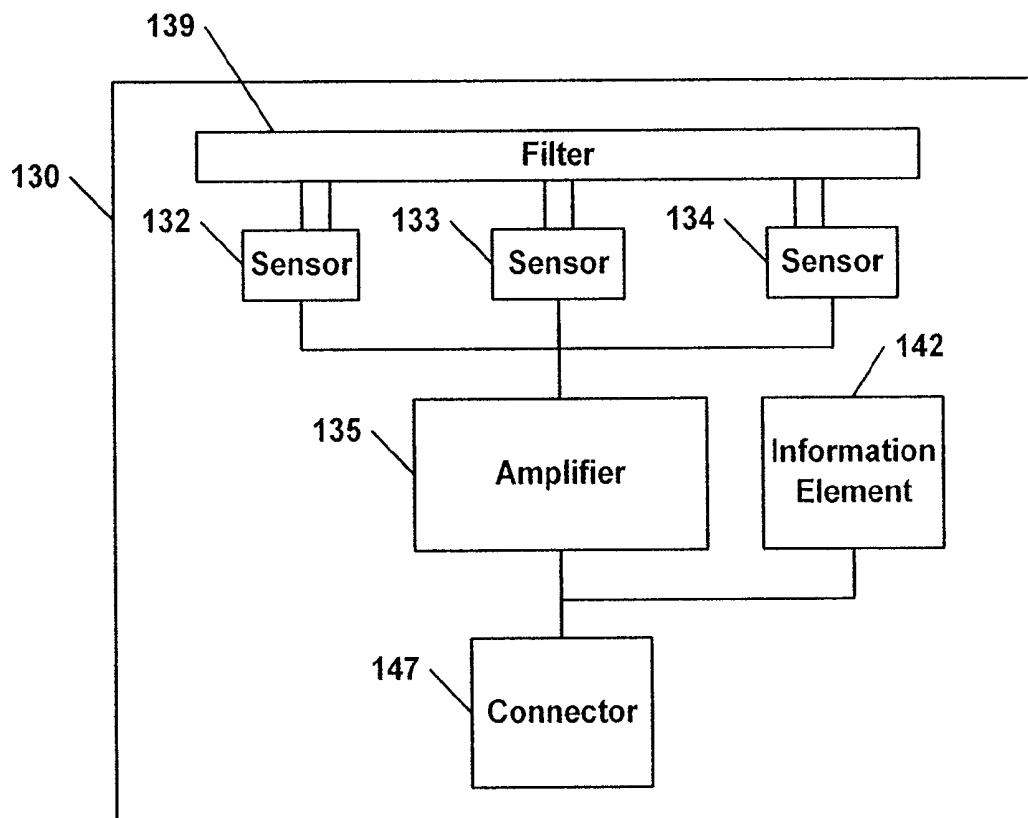


Figure 1B

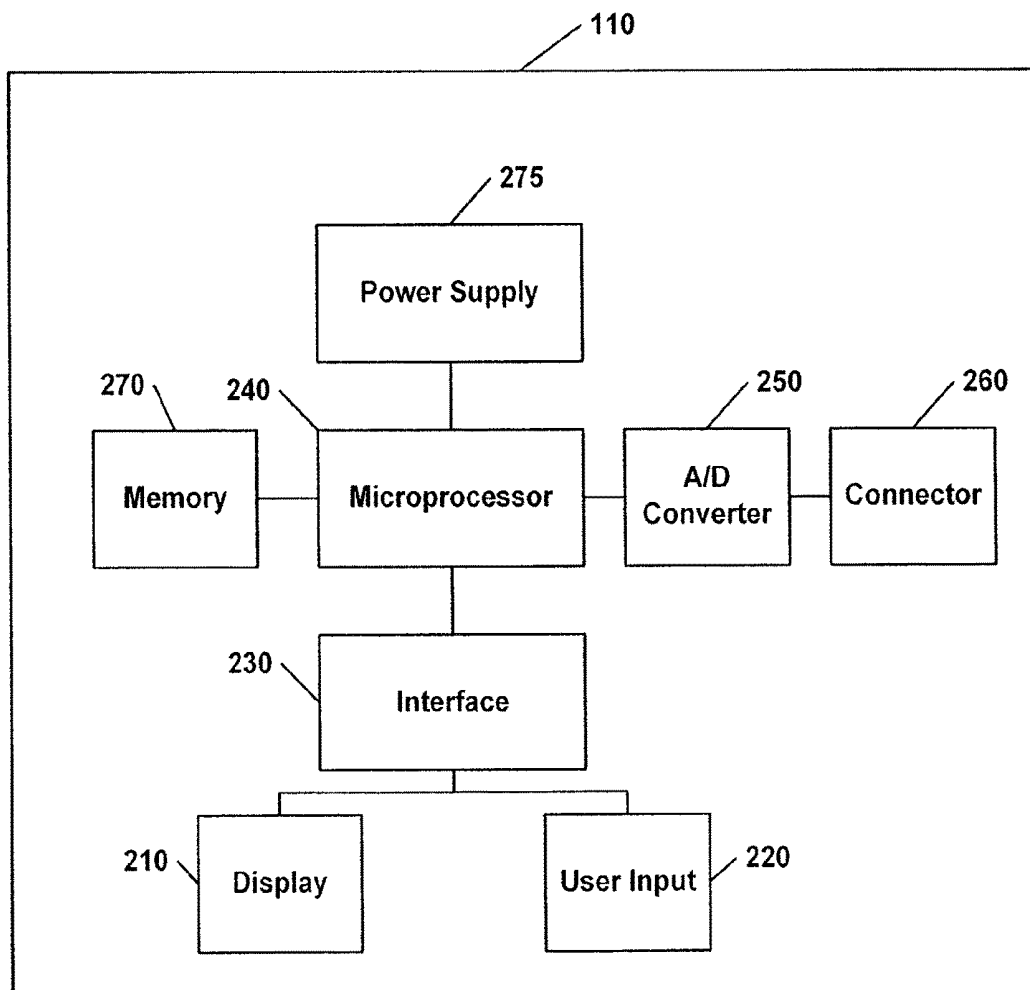


Figure 2

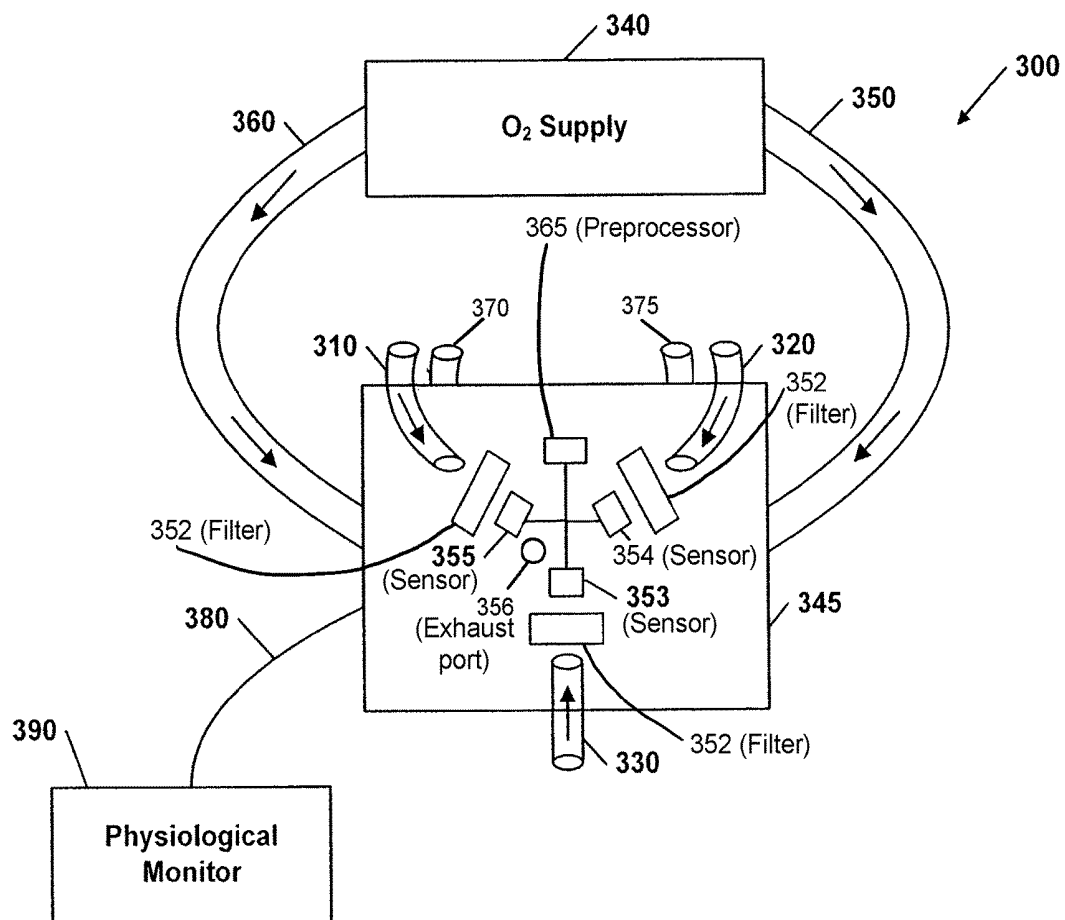


Figure 3

RESPIRATORY MONITORING**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation of U.S. application Ser. No. 13/224,266, filed Sep. 1, 2011, which is a continuation of U.S. application Ser. No. 11/756,501, filed May 31, 2007, which claims priority from U.S. Provisional No. 60/809,882, filed May 31, 2006, each of which is hereby incorporated by reference herein.

BACKGROUND**Field of the Invention**

The invention relates generally to systems, devices, and methods for monitoring a patient's respiratory system and health, including capnographers and other devices that deliver oxygen to a patient.

Description of the Related Art

Capnographers have been widely used for measuring concentration of carbon dioxide in a patient's exhaled breath and monitoring respiratory rate. The amount of carbon dioxide in a person's breath can indicate the overall efficiency of the cardio-pulmonary system and quality of breathing. For example, the concentration of carbon dioxide can indicate shallow breathing and poor oxygen intake. Thus, capnographers are used in hospitals and other medical institutions for monitoring the condition of a patient's respiratory system, pulmonary perfusion, and metabolism, and are most often used for patients in intensive care and under anesthesia.

A capnographer generally includes cannula tubes that conduct a patient's exhaled breath from the nasal and/or oral cavity to a collection tube that further transfers the exhaled breath to sensors. The sensors measure the concentration of carbon dioxide in the breath, and are generally located some distance away from the cannula tubes.

Capnographers are typically expensive, relatively large, and consume a large amount of power. Thus, their use is generally limited to hospitals and other controlled environments. Accordingly, there is a need for compact, inexpensive respiratory monitoring devices than can be used in and outside of hospitals to provide valuable respiratory information to doctors, nurses, paramedics, and other health care providers.

SUMMARY

A patient interface in accordance with one embodiment of the present invention is configured to be at least partially carried by a patient and to receive gas exhaled by the patient. The patient interface includes first and second cannula tubes each having a first end and a second end, the first ends are configured to be inserted into the nostrils of a patient, the first and second cannula tubes are configured to direct exhaled gas from the patient from the first ends to said second ends. The patient interface also includes first and second sensors positioned near the second ends, and the first and second sensors are configured to provide first and second signals based upon the gas and/or the contents of the gas, wherein the first and second signals are indicative of a physiological parameter of the patient. The patient interface also includes a communications link configured to provide the signal to a physiological monitor.

The patient interface can also include an information element coupled to the communications link. The informa-

tion element can include calibration information regarding the first and second sensors. The patient interface can also include a filter, wherein the filter removes moisture from the gas. The first and second sensors can include nanoelectric sensors or nanotechnology sensors. The first and second signals can be indicative of a carbon dioxide concentration of said gas or a respiratory rate of said patient.

In some embodiments, the communications link includes a wireless link, such as an IEEE 802.11 standard-compatible link. The patient interface can also include the physiological monitor. The physiological monitor can be configured to determine the physiological parameter from the first and second signals. In other embodiments, the length of the first and second cannula tubes is selected from the group consisting of about 1 inch, about 2 inches, about 4 inches, about six inches, and no longer than about 5 inches.

In other embodiments, the patient interface also includes a third sensor and a third cannula tube, said third cannula tube configured to be inserted into the patient's mouth and to direct breath exhaled from said patient to said third sensor. In some embodiments, the patient interface also includes a preprocessor configured to condition the first and second signals. For example, in some embodiments, the preprocessor includes a filter, an amplifier, and/or an analog-to-digital converter. In one embodiment, the patient interface is configured to be suspended from the neck of the patient.

In accordance with yet another embodiment of the present invention, a method of determining a physiological parameter of a patient, comprises: receiving gas exhaled from a patient in a patient interface carried by the patient; generating a signal indicative of a physiological parameter of said patient by sensing a parameter of said gas with a sensor positioned within said patient interface; and providing said signal to a physiological monitor.

In some embodiments, the generating a signal comprises generating a signal indicative of a carbon dioxide concentration of said gas and/or generating a signal indicative of a respiratory rate of said patient. The providing said signal can include wirelessly transmitting the signal. In other embodiments, the method also includes controlling the transfer of said gas to a selected one of two or more sensors located within said patient interface. In one embodiment, controlling the transfer of said gas extends the useful life of said patient interface.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a block diagram of a respiratory monitoring system in accordance with one embodiment of the present invention.

FIG. 1A is a block diagram of a preprocessing element in accordance with one embodiment of the present invention.

FIG. 1B is a block diagram of a sensing module in accordance with another embodiment of the present invention.

FIG. 2 is a block diagram of a physiological monitor in accordance with one embodiment of the present invention.

FIG. 3 is a partial front view of a respiratory monitoring system in accordance with one embodiment of the present invention.

DETAILED DESCRIPTION

FIG. 1 illustrates a respiratory monitoring system **100** in accordance with one embodiment of the present invention. The respiratory monitoring system **100** generally includes a physiological monitor **110** coupled to or in communication

with a patient interface **185** via a communication link **120**. The patient interface **185** is coupled to a patient **155**. Exhaled breath from the patient **155** is received by the patient interface **185**. Oxygen from an oxygen supply **180** can also be provided to the patient **155** with the patient interface **185**.

The patient interface **185** of the respiratory monitoring system **100** generally includes two nasal cannulae **150**, **160**, e.g., tubes, for insertion into or placement adjacent the nostrils of the patient **155**. The patient interface **185** may also optionally include an oral cannula tube **170** for insertion into or placement adjacent the patient's mouth. The tubes **150**, **160**, and **170** are configured to transfer or guide gases exhaled from the patient **155** to a carbon diode sensing module **130** of the patient interface **185**. In some embodiments, the tubes are about 1 inch, about 2 inches, about 4 inches, or about six inches long. In other embodiments, the tubes are no longer than about 5 inches. In some embodiments, the patient interface **185** is configured to be carried around or suspended from the neck of the patient **155**.

The system **100** may also optionally include an oxygen supply **180** for storing oxygen and providing oxygen to the patient **155**. Oxygen tubes **190** and **195** facilitate the transfer of oxygen stored in the supply **180** to the patient **155**. Although two tubes **190**, **195** are illustrated, a single or multiple tubes may be employed. The tubes **190** and **195** may have one or more oxygen-emitting apertures (not shown) that include openings located on sections of the tubes **190** and **195** that are adjacent to the nostrils and/or the mouth of the patient.

The sensing module **130** is configured to measure a physiological parameter of the patient **155**. For example, in one embodiment, the sensing module **130** measures the carbon dioxide concentration of gases exhaled by the patient **155**. The sensing module **130** is further configured to generate at least one parameter signal indicative of the physiological parameter, and to transmit the parameter signal through a communications link **120** to a physiological monitor **110**. The parameter signal can include measurement data, an alarm value, or any other parameter signal known to those of skill in the art.

The communications link **120** can be a wired or wireless link or a combination of a wired and a wireless link. For example, the communications link can include a single, dual, or a multi-conductor cable. A wireless communication link **120** may be established by utilizing a wireless transmitter, receiver, and/or a transceiver, such as a BLUETOOTH-compatible transceiver. In addition, a transceiver that utilizes any other wireless communication protocol, such as any of the IEEE 802.11 standards (including, but not limited to 802.11(a), (b) or (g)), may be used.

The sensing module **130** also includes one or more sensors (e.g., sensors including or constructed using nanotechnology) located at or near the output end of the cannulae **150**, **160**, **170**. In one embodiment, three sensors **132-134** are used. The sensors **132-134** are positioned inside of the sensing module **130** near the output ends of the cannulae **150**, **160**, **170**. In one embodiment, the sensors are carbon dioxide sensors **132-134**. The sensors **132-134** can be nanotechnology carbon dioxide sensors, or can be any of a variety of nano-sensors known to those of skill in the art. For example, the sensors **132-134** can be any sensor that monitors or measures carbon dioxide concentrations, including nanoelectric sensors described in U.S. patent application Ser. No. 10/940,324, the entirety of which is hereby incorporated by reference. Other sensors, such as infrared sensors, can also be used.

Because the sensors **132-134** are placed close to the output ends of the cannula tubes, the force of the patient's exhalation pushes the breath to be sampled into the sensors **132-134** of the sensing module **130**. Unlike other systems where a pump is used to draw the patient's exhaled breath into a sensor, in some embodiments, a pump is not utilized. A sensing module that includes sensors close to the output ends of cannula tubes provides the advantage of not having to use a pump to assist in drawing the patient's exhalation from the patient's nose (or mouth), to the sensor. Another advantage provided by providing sensors at the ends of the cannula tubes, near the patient's nose (or mouth), is that ill or weak patients, with shallow breathing, can be monitored without utilizing a pump to assist in drawing the patient's exhalation to the sensor. This helps reduce the size, cost, and noise level of the sensor, sensing module, and system.

In other embodiments, a pump or other suction or vacuum device is used to help draw air from the patient to the sensors **132-134** of the sensing module **130**. A filter **139** can be provided between the output of the cannulae **150**, **160**, **170** and the input of the sensors **132-134** to remove contaminants, moisture, mucous, and/or particulate matter from the patient's breath prior to entry into the sensor **132-134**.

In addition, the sensing module **130** can also include an information element **142**, a preprocessor **138**, and a connector **140**. The information element **142** stores information specific to each of the sensors **132-134**. For example, in one embodiment, the information element **142** includes calibration parameters for each of the sensors **132-134**. The information element **142** can include an EPROM, an EEPROM, a resistor, a capacitor, a microchip, a memory, a RAM, a ROM, or any other information storage element. In addition, the information element can include a combination of one or more of any of the above.

The preprocessor **138** generally includes circuitry that process the parameter signal(s) generated by the sensor **132-134** prior to transmission to the physiological monitor **110**. For example, the preprocessor **138** can include any of a variety of front-end signal conditioners, such as filters, amplifiers, buffers, memories and/or analog-to-digital (A/D) converters known to those of skill in the art. The connector **140** provides a mechanical and electrical link between the patient interface **185**, communication link **120**, and physiological monitor **110**. When the communication link **120** is a wireless link, as described above, the connector **140** can be omitted and/or can include any of the wireless transmitters, receivers, or transceivers described above.

FIG. 1A illustrates one embodiment of the preprocessor **138**. In some embodiments, the preprocessor **138** includes A/D converters **143**, **144**, and **145** and can further include a serial-to-parallel converter **146**. Although three A/D converters **143-145** are illustrated, it should be understood that one or more A/D converters may be employed. For example, in some embodiments, a multi-channel A/D converter is provided. The A/D converters **143-145** are coupled to the sensors **132-134**, respectively, and are configured to convert the analog signals outputted by the sensors **132-134** to digital signals for transmission to the physiological monitor **110**. Additional front-end conditioning electronics, such as an amplifier, filter **149**, and/or buffer may also be provided. The parallel converter **146** receives the digital signals from the A/D converters **143-145** and produces a serial signal that can be transmitted through a single channel communications link. The serial signal is provided to the connector **140**, which passes the signal to the communications link **120**, which provides the signal to the physiological monitor **110**. In some embodiments, the A/D converters are provided in

the physiological monitor **110**, and one or more analog signals are provided from the sensing module **130** to the physiological monitor **110**. In addition to the components shown, the preprocessor **138** can also include a variety of additional signal conditioning elements, such as amplifiers and/or filters. In one embodiment, the sensing module **130** may also include processing hardware such as a microprocessor, a microcontroller, a microchip, and/or memory to perform one or more of the processing functions described herein.

FIG. 1B illustrates another embodiment of a sensing module **130**, such as a carbon dioxide sensing module, that provides analog signals to the physiological monitor **110**. The sensing module **130** includes sensors **132-134** that are coupled to an amplifier **135**. The amplifier **135** amplifies the signals outputted by the sensors **132-134** and provides amplified signals to the connector **147**. The connector **147** provides the amplified signal to the communications link **120** to the physiological monitor **110**. In this embodiment, the physiological monitor **110** converts the received analog signals to digital signals. In yet another embodiment, the sensing module **130** can include one or more A/D converters that convert the output of each of the sensors **132-134** to digital signals prior to transmission to the physiological monitor **110**, as described above.

In other embodiments, one or more of the preprocessing elements are included within, and/or are performed within, the communications link **120** and/or the physiological monitor **110**. For example, A/D converter, amplifier, and/or filter may be located inside the communications link **120** or the physiological monitor **110**. In some embodiments, for example, preprocessing elements, such as electronics components including an A/D converter, an amplifier, and/or a filter, are included within the communications link **120**. For example, the preprocessing elements can be included within the connector or the insulation of the conductors of the communications link **120**.

Although in the embodiment illustrated in FIG. 1 the sensors are located inside the housing of the sensing module **130**, various other configurations are also possible. For example, in one embodiment, the sensors may be placed inside each of the cannula tubes **140**, **150**, and **160**. The output of the sensors then can be transmitted to the sensing module **130** where the signals from each of the sensors can be preprocessed and sent to the physiological monitor **110** in any of the variety of methods previously described.

In another embodiment, the cannula tubes' outputs are directed to a volume of space within the patient interface **185**, such as a plenum. The plenum is generally a volume inside the sensing module **130** that is filled with the patient's exhaled gases. One or more sensors may be placed near the plenum for measuring the concentration of carbon dioxide in the gases. The signals from the sensors are then preprocessed and transmitted to the physiological monitor **110** in any of the variety of methods described above.

Some sensors, such as nanoelectric sensors, can have a limited useful life of 6-24 hours. In addition, the accuracy of such sensors may decay over time due. Thus, according to another embodiment of the present invention, the patient interface **185** can be disposable. In another embodiment, the patient interface **185** is reusable, for example, by including replaceable sensors. Thus, in such an embodiment, the sensing module **130** of the patient interface **185** is replaceable. Alternatively, the sensing module **130**, itself may be disposable.

In other embodiments, to prolong the life of the sensing module **130**, each cannula tube **140**, **150**, **160** is sequentially

or serially exposed to more than one sensor over time. For example, the output of a tube is directed to a first sensor, and before the useful life of the sensor ends, the output of the tube is directed to a second sensor. In addition, for example, before the first sensor's accuracy falls below a predetermined level, the second sensor may be put in use. For example, before the first sensor's accuracy falls below the predetermined level, or after the passage of a predetermined amount of time, the patient interface **185** can redirect the exhaled airflow out of the cannulae to a replacement or second sensor. Any of a variety of mechanisms known to those of skill in the art can be used to redirect exhaled airflow in this manner.

For example, exchanging of the sensors may be done either manually or automatically and can be achieved in a variety of different ways. For example, the sensing module **130** can include a rotating knob that when manually turned rotates a disc or plate onto which sensors are mounted. By rotating the knob, the disc rotates with respect to the cannula output, the first sensor is moved away from the cannula output, and the second sensor is moved into position to receive exhaled air from the cannula output. In another embodiment, the cannula output and sensors are fixed in position with respect to each other, and a separation plate or disc separates the cannula output from the sensors. A window in the separation plate allows air flow from the cannula output to pass to a selected sensor. Sensors can be selected by rotating a knob. In other embodiments, the sensing module **130** includes a slideable plate that operates similarly to the rotating embodiments described above. For example, the sensors can be mounted to a slideable plate, or a slideable plate with window can be slid along its axis to control cannula to sensor coupling. Sensor selection can be performed automatically by including a motor, such as a stepper motor, linear translator, or a ratcheting mechanism, as are well known to those of skill in the art. In some cases, gear assemblies are used to control motion and orientation of the sensors with respect to the cannulae outputs.

In addition, the outputs of the cannulae can be moved or displaced with respect to the sensors. In such cases, the sensors can be mounted to the sensing module **185** and the cannulae outputs can be moved or positioned using any of the mechanisms and techniques described above.

In yet another embodiment, cannula tubes having forked outputs that can be individually opened and/or closed are provided. For example, each nostril cannula can include a first input end that is inserted into a patient's nose, and two or more output ends that are coupled to two or more sensors. For example, when the cannula has two output ends, the cannula can have a Y-shape or a T-shape. In this embodiment, one sensor can be placed at each of the forked outputs of the cannula tubes. A valve can be positioned at each of the cannula outputs that control airflow out of the cannula. In this manner, the desired sensor can be individually selected. Before the first sensor expires, the first cannula output to the first sensor is closed with a first valve and the second cannula output to the second sensor is opened with a second valve. Additional embodiments include movable cannula tubes with sensors placed at each of the possible positions of the cannula tubes or automatically exchanging the position of the sensors. Various other configurations are also possible.

One or more timers may also be provided to keep track of the length of time each of the sensors has been in operation. When any of the sensors has been in operation for a predetermined length of time, the timer may output a signal and/or trigger an alarm to notify the user that it is time to

exchange the sensor. For example, the predetermined length of time can be about 2, about 4, about 5, or about 6 hours. In other cases, the predetermined time is about 5 hours, about 10 hours, about 15 hours, or about 20 hours. The output signal and/or alarm may be an audible signal such as an alarm beep, a visual signal such as an LED light, a vibration, or any other known method of notifying users.

FIG. 2 illustrates a block diagram of a physiological monitor 110. The physiological monitor 110 can be a handheld monitor, such as a pulse oximeter, an example of which is the SpO₂ monitor manufactured by Masimo Corporation. The physiological monitor 110 may also be a non-handheld monitoring device, such as a computer board, or a module, such as a module that attached to a rack of monitoring equipment and/or a hospital bed. The monitor 110 generally includes a connector 260, a memory 270, a microprocessor 240, a power supply 275, an interface 230, a user input device 220, and a display 210. The connector 260 may be a transceiver and/or receiver, such as a BLUETOOTH-compatible transceiver, that is coupled to and receives signals from the patient interface 185 via the communications link 120.

Depending on whether or not the signals received by the connector 260 have already been converted to digital signals, the physiological monitor 110 may or may not include the A/D converter 250. The microprocessor analyzes the information received from the patient interface 185 and determines a physiological parameter of the patient. For example, the microprocessor can determine the CO₂ concentration of the patient's breath and/or the patient's respiratory rate, or breathing frequency. The physiological parameter is provided as a signal to the interface 230, which then provides the signal to the display 210. The interface 230 can include electronics, such as driver circuits, to drive the display 210 such that it displays the physiological parameter, or an indication of the physiological parameter. Indications of the physiological parameter can include an alarm, an icon, or a color that generally represents the quality of the measured physiological parameter. The memory 270 may be used to store a patient's medical data and history, for example, the history of measured physiological parameters and identification of the patient interface 185. The physiological monitor 110 can determine when it is time to replace the patient interface 185 by measuring the time the patient interface has been used. In other embodiments, the physiological monitor indicates that the patient interface 185 is to be replaced after it receives an alarm or signal from the patient interface 185. In other embodiments, the physiological monitor 110 controls the coupling of the output of the cannulae to the sensors located within the patient interface 185. As will be understood by those skilled in the art, the physiological monitor 110 may include other components as well.

FIG. 3 illustrates a partial front view of a respiratory monitoring system 300 in accordance with another embodiment of the present invention. The system 300 is used by inserting a first end of the cannula tubes 310, 320, and 330 into the patient's nostrils (not shown) and mouth (not shown). As the patient breathes, the gases he/she exhales enter the first end of the cannula tubes and exit from their second ends. Before entering a plenum, or volume within the sensing module 345, the gases pass through a filter 352. The filter 352 absorbs moisture, mucus, and/or other contaminants or debris contained in the gases, and protects the sensing module from contamination. After passing through the filter 352, the gases contact the sensors 353-355. The sensors 353-355 determine the concentration of a desired

substance (such as carbon dioxide, alcohol, oxygen, etc.), in the exhaled gases and transfer this data to the preprocessor 365. The preprocessor 365 processes the signals and transmits them through a connector (not shown) to the physiological monitor 390 via a communications link 380, where they are further processed (as described above) and displayed to the user. The gases accumulated in the plenum then exit through an exhaust port 356 as the patient exhales the next breath. A one-way valve can be provided with the patient interface to prevent air from being drawn through the patient interface and into the patient upon patient inhalation.

As illustrated in FIG. 3, the monitoring system 300 may also include an oxygen supply 340. The oxygen supply releases oxygen into the oxygen tubes 350 and 360. Oxygen travels through the oxygen tubes and exits through oxygen emitters 370 and 375 that are located close to the nostrils and/or mouth of the patient.

In some embodiments, the monitoring system is used with patients that weigh more than about 5 kg, 10 kg, 15 kg, or 20 kg. In other embodiments, monitoring system measures carbon dioxide concentrations between about 0 and 5%, between about 0 and 10%, or between about 0 and 15%. In some embodiments, the resolution of the system is about 0.1%, about 0.05%, about 1% or about 1.5%. In other embodiments, the monitoring system has a response time of about 50, 100, 250, 500, or 600 μ s. In other embodiments, the monitoring system has a shelf life of about one year, about 2 years, or more than one year.

Although this invention has been disclosed in the context of certain preferred embodiments, it will be understood by those skilled in the art that the present invention extends beyond the specifically disclosed embodiment to other alternative embodiments and/or uses of the invention and obvious modifications and equivalents thereof. In particular, while the present respiratory monitoring system and methods of monitoring respiration have been described in the context of a particularly preferred embodiment, the skilled artisan will appreciate, in view of the present disclosure, that certain advantages, features and aspects of the monitoring system and method may be realized in a variety of other devices. Additionally, it is contemplated that various aspects and features of the invention described can be practiced separately, combined together, or substituted for one another, and that a variety of combination and sub-combinations of the features and aspects can be made and still fall within the scope of the invention. Thus, it is intended that the scope of the present invention herein disclosed should not be limited by the particular disclosed embodiment described above, but should be determined only by a fair reading of the claims that follow.

The invention claimed is:

1. A method of detecting a physiological parameter of a patient, comprising:

receiving, in a sensing module, gas exhaled by a patient, the sensing module comprising:
a plurality of sensors each configured, when activated, to provide a signal indicative of a physiological parameter of the patient based on the gas; and
a sensor selector configured to cause the gas exhaled by the patient to be directed to an active sensor, the active sensor selected from the plurality of sensors.

2. The method of claim 1, wherein when a predetermined event occurs, the sensor selector directs the gas to a second sensor selected from the plurality of sensors.

3. The method of claim 2, wherein the predetermined event is at least one of: an accuracy of the active sensor falling below a predetermined level, an end of a useful life

9

of the active sensor, a passing of a predetermined amount of time, or a triggering of an alarm based on an expiration of a timer.

4. The method of claim 1, wherein at least one of the plurality of sensors does not receive gas at a particular time.

5. The method of claim 1, wherein the sensing module is configured to be suspended from the neck of the patient.

6. The method of claim 1, wherein the sensor selector comprises at least one of a rotatable plate, a slidable plate, or one or more valves.

7. The method of claim 1 further comprising:

providing the signal to a physiological monitor via a communications link.

8. The method of claim 1, wherein at least one of the plurality of sensors comprises at least one of a nanotechnology sensor or an infrared sensor.

9. The method of claim 1, wherein the signal is indicative of at least one of a carbon dioxide concentration of the gas or a respiratory rate of the patient.

10. A sensing module configured to receive exhaled gas by a patient via a cannula tube and detect a physiological parameter of a patient, the sensing module comprising:

a plurality of sensors each configured, when activated, to provide a signal indicative of a physiological parameter of the patient based on the gas; and

a sensor selector configured to cause the gas exhaled by the patient to be directed to an active sensor, the active sensor selected from the plurality of sensors.

11. The sensing module of claim 10, wherein when a predetermined event occurs, the sensor selector directs the gas to a second sensor selected from the plurality of sensors.

12. The sensing module of claim 10, wherein at least one of the plurality of sensors does not receive gas at a particular time.

10

13. The sensing module of claim 10, wherein the sensor selector comprises at least one of a rotatable plate, a slidable plate, or one or more valves.

14. The sensing module of claim 10, wherein the sensing module is configured to be suspended from a neck of the patient.

15. The sensing module of claim 10, wherein the sensor selector is configured to control a location of at least one of the plurality of sensors within the sensing module.

16. The sensing module of claim 10, wherein the sensor selector is configured to direct the gas from a first sensor to a second sensor before the useful life of the first sensor ends.

17. A patient interface configured to receive gas exhaled by a patient, said patient interface comprising:

a plurality of sensors each configured, when activated, to receive exhaled gas by a patient and provide a signal indicative of a physiological parameter of the patient based on the gas;

a sensor selector configured to cause the gas exhaled by the patient to be directed to an active sensor, the active sensor selected from the plurality of sensors; and

an information element coupled to the plurality of sensors, wherein the information element includes calibration information regarding the plurality of sensors.

18. The patient interface of claim 17, further comprising a communications link configured to provide the signal to a physiological monitor.

19. The patient interface of claim 17, wherein the at least one of the plurality of sensors comprises at least one of a nanotechnology sensor or an infrared sensor.

20. The patient interface of claim 17, wherein the signal is indicative of at least one of a carbon dioxide concentration of the gas or a respiratory rate of the patient.

* * * * *

专利名称(译)	呼吸监测		
公开(公告)号	US9566019	公开(公告)日	2017-02-14
申请号	US14/153656	申请日	2014-01-13
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR DIAB MOHAMED K		
发明人	AL-ALI, AMMAR DIAB, MOHAMED K.		
IPC分类号	A61M11/00 A61B5/083 A61B5/097 A61B5/00 A61M16/10 A61M16/06 A61B5/08		
CPC分类号	A61B5/0836 A61B5/0004 A61B5/0816 A61B5/097 A61B5/682 A61B5/6819 A61B5/6822 A61M16/0666 A61M16/0672 A61M16/10 A61M2202/0208 A61M2205/18 A61M2205/3561 A61M2205/581 A61M2205/583 A61M2230/42 A61M2230/432 A61M2230/435 A61M16/085 A61M16/1065		
审查员(译)	DOUGLAS, 史蒂芬		
优先权	60/809882 2006-05-31 US		
其他公开文献	US20140194766A1		
外部链接	Espacenet USPTO		

摘要(译)

根据本公开的一个实施例的患者接口被配置为至少部分地由患者携带并且接收由患者呼出的气体。患者接口包括第一和第二套管管，每个套管管具有第一端和第二端，第一端构造插入患者的鼻孔中，第一和第二套管管构造将来自患者的呼出气体所述第一端部到所述第二端部。患者接口还包括位于第二端附近的第一和第二传感器，并且第一和第二传感器被配置为基于气体提供第一和第二信号，其中第一和第二信号指示患者的生理参数。患者接口还包括被配置为向生理监视器提供信号的通信链路。

